
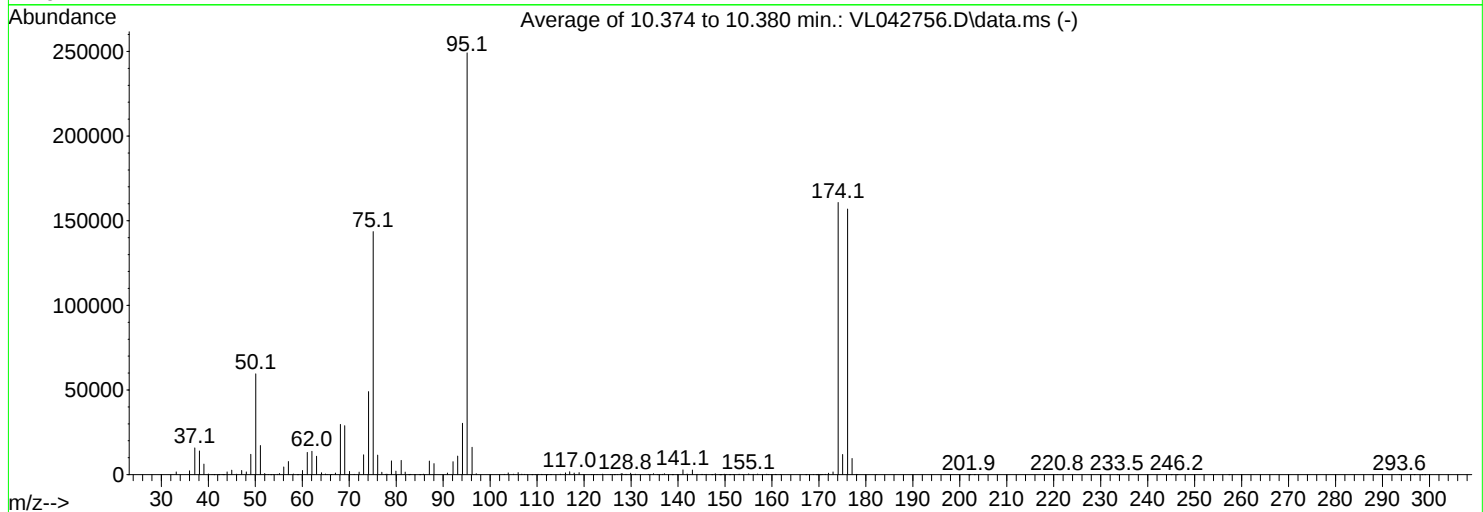


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072425\
Data File : VL042756.D
Acq On : 24 Jul 2025 07:39
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 24 05:24:41 2025

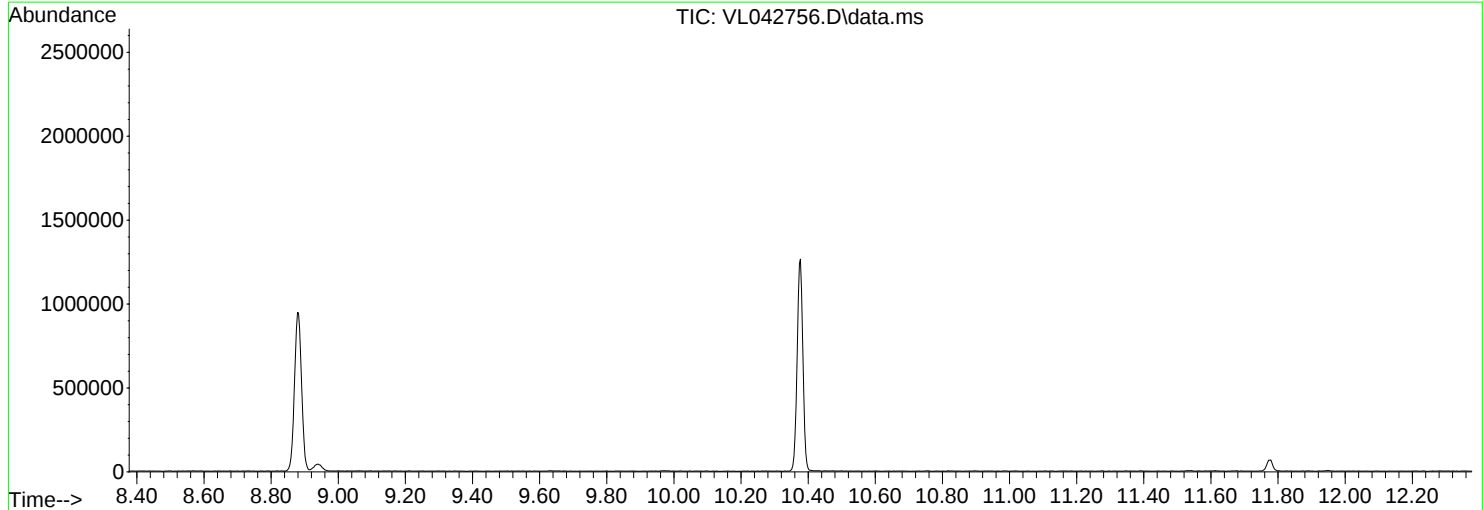

AutoFind: Scans 3178, 3179, 3180; Background Corrected with Scan 3162

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	23.9	59533	PASS
75	95	30	66	57.6	143544	PASS
95	95	100	100	100.0	249173	PASS
96	95	5	9	6.5	16190	PASS
173	174	0.00	2	1.0	1612	PASS
174	95	50	120	64.5	160811	PASS
175	174	4	9	7.4	11880	PASS
176	174	93	101	97.6	156928	PASS
177	176	5	9	6.1	9565	PASS

Average of 10.374 to 10.380 min.: VL042756.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.15	1610	44.00	1621	53.30	21	63.05	1088
36.00	2305	45.00	2618	53.90	131	64.10	113
37.10	15810	46.05	259	54.70	232	64.95	42
38.10	13986	47.10	2448	55.15	694	65.30	7
39.05	6272	48.10	1663	56.05	4584	66.25	68
40.00	352	49.05	11999	57.05	7757	67.05	963
40.80	115	50.10	59533	58.10	431	68.10	29648
41.20	20	51.10	17169	59.00	20	69.05	28904
42.20	19	52.00	667	60.05	2458	70.05	1913
42.95	145	52.20	134	61.05	13101	71.05	157
43.20	39	52.75	96	62.05	13791	72.10	1567

Average of 10.374 to 10.380 min.: VL042756.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.05	11709	81.90	1474	94.10	30304	108.90	20
74.10	49088	82.70	36	95.10	249173	109.60	60
75.10	143544	83.10	202	96.15	16190	110.20	175
76.05	11564	83.90	39	97.05	567	110.95	214
76.95	1416	85.00	36	103.00	155	111.20	89
77.70	214	85.80	311	103.85	1030	111.70	98
78.00	305	87.05	8048	105.00	329	112.10	54
78.20	185	88.05	6496	105.95	1212	112.80	57
79.00	8125	90.90	914	106.75	259	113.05	143
79.95	2110	92.10	7686	107.35	152	114.95	298
81.05	8452	93.10	11013	107.90	89	116.05	1011

Average of 10.374 to 10.380 min.: VL042756.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
116.95	1683	127.90	528	136.70	165	145.70	64
117.90	991	128.10	541	137.10	542	146.00	182
118.95	1277	128.75	203	138.80	26	147.20	48
119.85	144	129.10	182	138.95	113	147.95	536
121.65	70	129.90	852	139.85	101	148.90	48
122.15	78	130.90	291	141.05	2840	149.10	34
122.75	83	133.70	159	141.95	422	149.85	302
123.95	277	134.10	104	143.05	2781	150.20	159
125.65	98	134.80	564	144.05	206	151.00	21
126.45	41	135.60	68	144.95	204	151.80	115
127.10	142	135.90	19	145.20	161	153.00	282

Average of 10.374 to 10.380 min.: VL042756.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
153.70	63	169.50	32	177.05	9565	257.30	18
155.05	444	169.90	178	178.00	175	293.65	58
156.00	186	170.30	54	178.20	98	296.75	35
156.95	412	170.75	82	182.30	68	298.40	41
158.90	272	171.10	141	201.90	43	299.00	43
159.20	69	171.40	211	202.10	24		
160.70	177	172.05	838	203.10	25		
160.90	88	173.00	1612	220.75	57		
161.80	73	174.10	160811	233.50	40		
167.20	41	175.05	11880	245.00	21		
168.85	101	176.10	156928	246.20	53		