

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072825\
 Data File : VX047159.D
 Acq On : 28 Jul 2025 12:20
 Operator : JC/MD
 Sample : Q2693-02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 STORAGE-BLANK-WATER-REF-5

Quant Time: Jul 29 02:41:54 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 22 03:59:51 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	303849	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.769	114	541367	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	484958	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	241227	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	187065	49.423	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	98.840%
35) Dibromofluoromethane	5.397	113	161741	48.388	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	96.780%
50) Toluene-d8	8.647	98	494526	45.684	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	91.360%#
62) 4-Bromofluorobenzene	11.079	95	227868	48.847	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	97.700%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX072825\
Data File : VX047159.D
Acq On : 28 Jul 2025 12:20
Operator : JC/MD
Sample : Q2693-02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Quant Time: Jul 29 02:41:54 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 22 03:59:51 2025
Response via : Initial Calibration




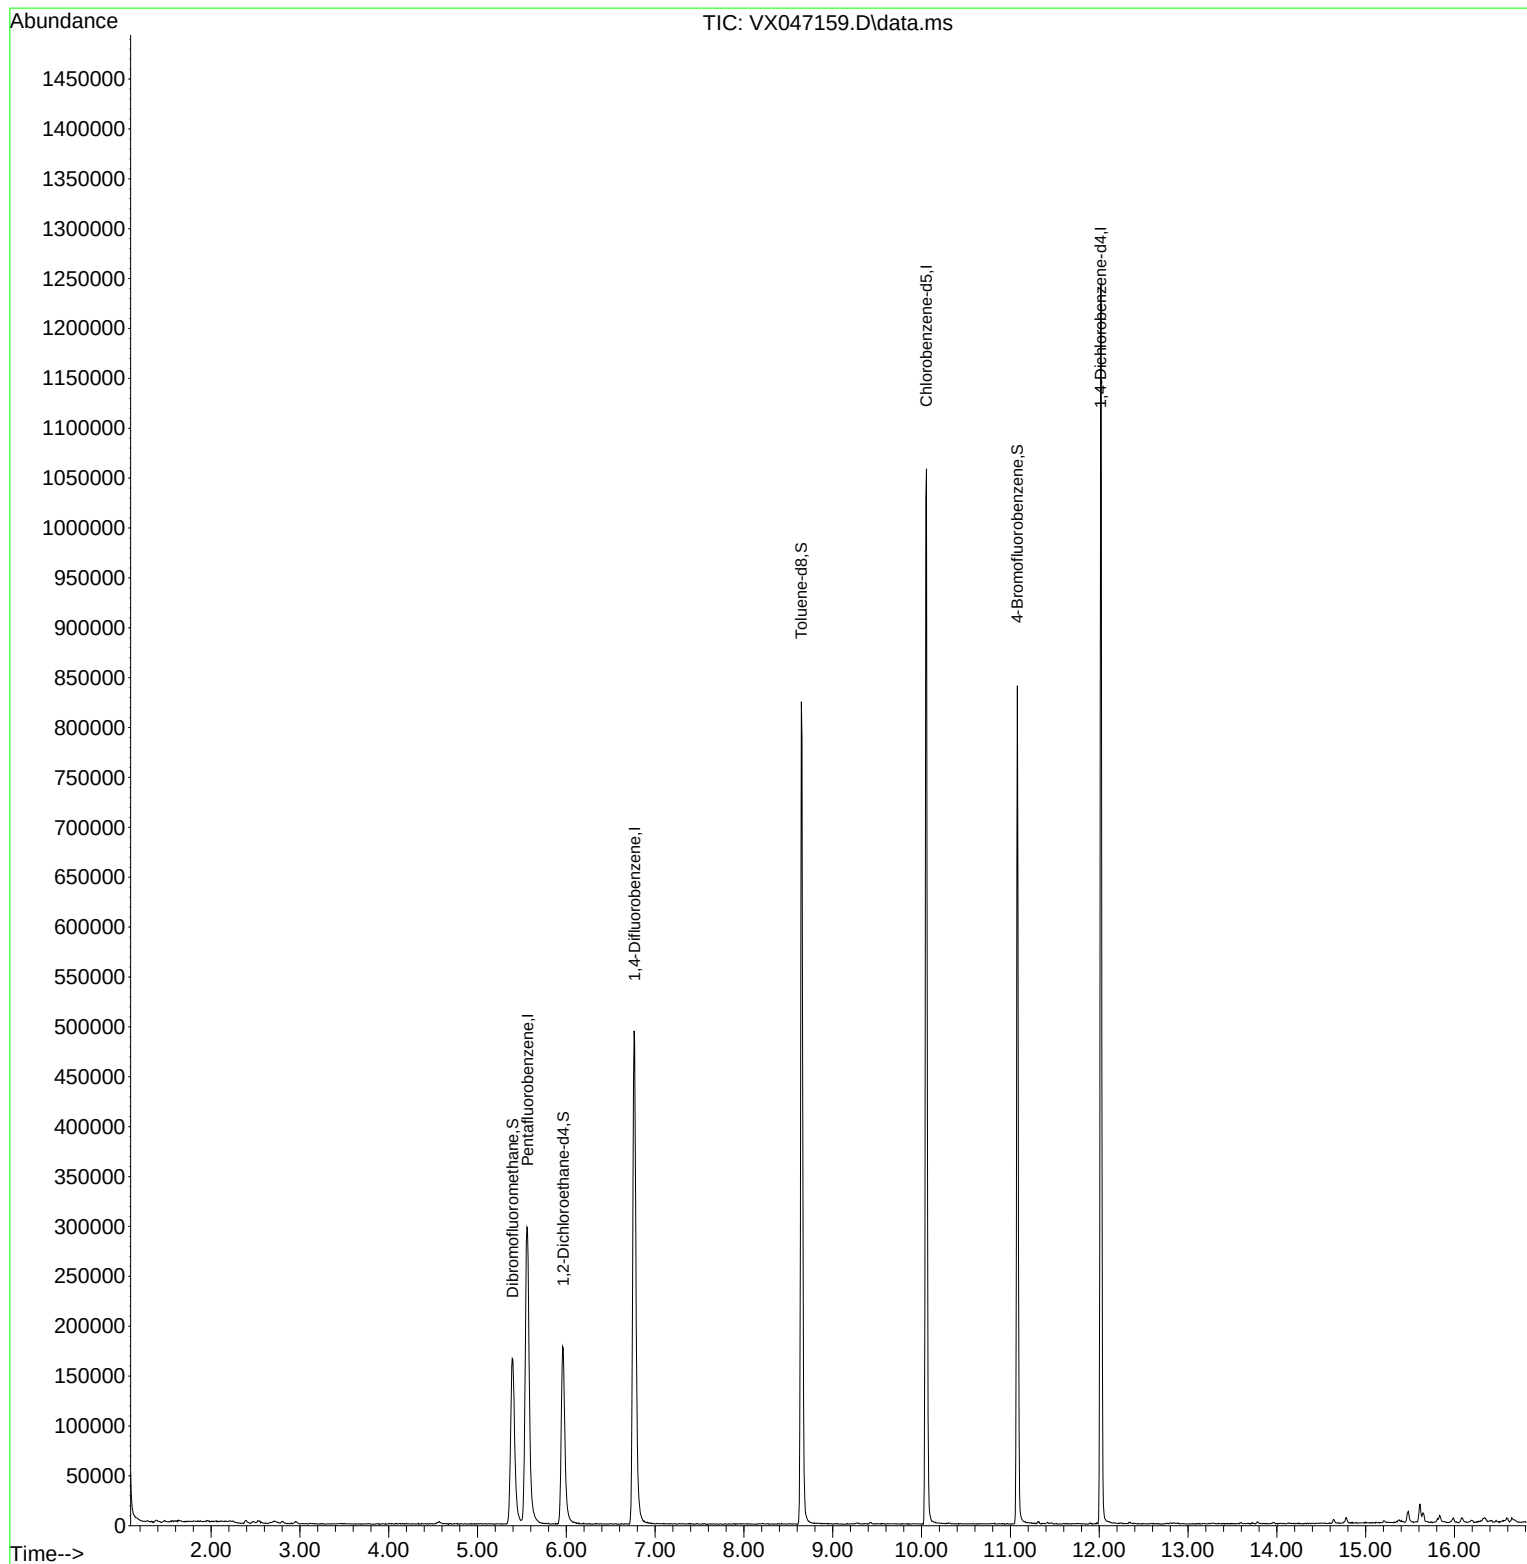


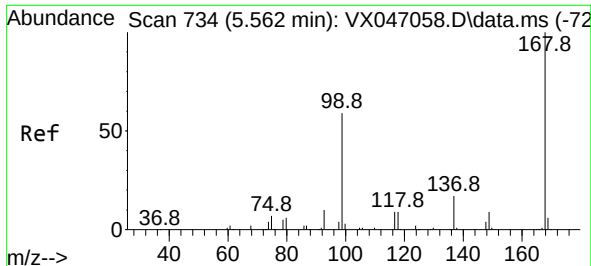

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. -0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:168 Resp: 303849
Ion Ratio Lower Upper
168 100
99 61.4 48.0 72.0

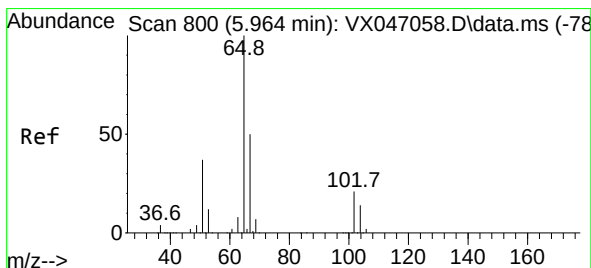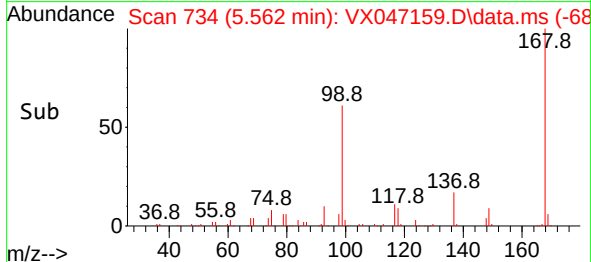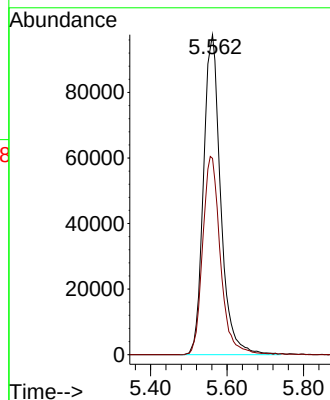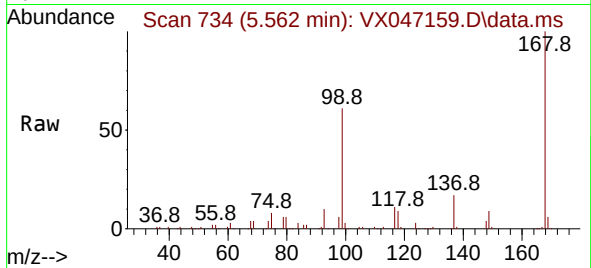

#33
1,2-Dichloroethane-d4
Concen: 49.423 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20

Tgt Ion: 65 Resp: 187065
Ion Ratio Lower Upper
65 100
67 53.1 0.0 104.8


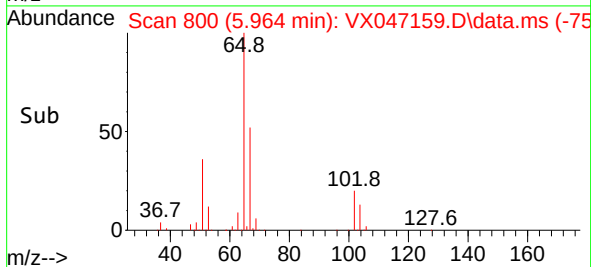
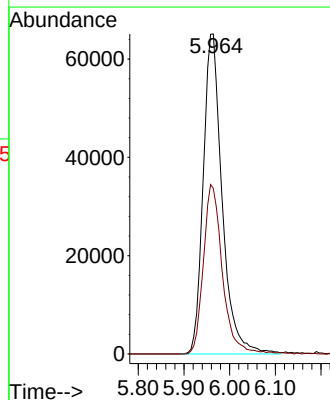
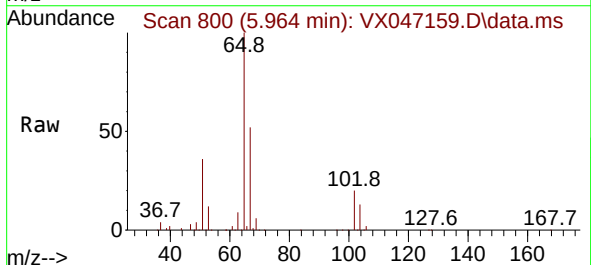


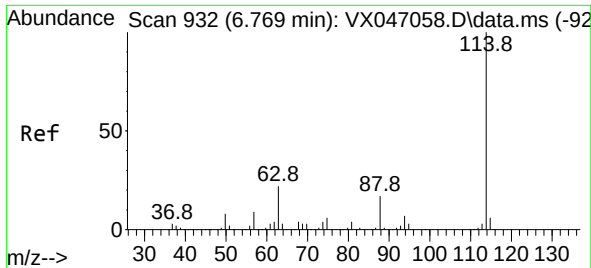

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.769 min Scan# 911
Delta R.T. 0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion:114 Resp: 541367
Ion Ratio Lower Upper
114 100
63 21.5 0.0 43.2
88 15.6 0.0 33.8

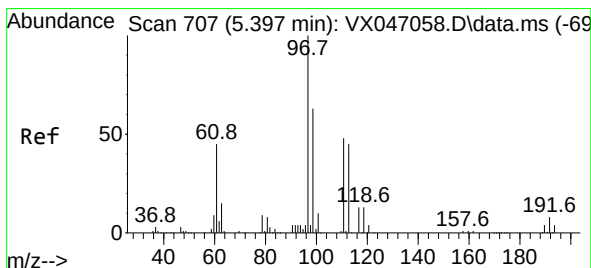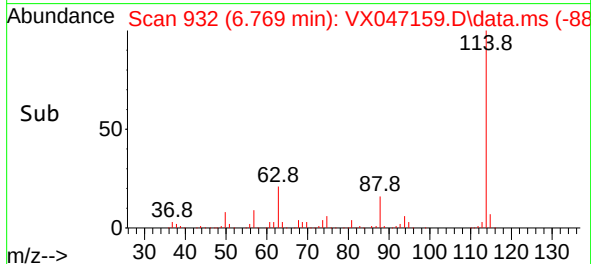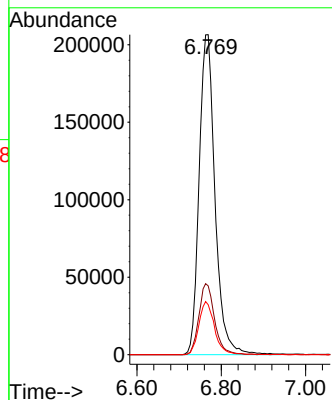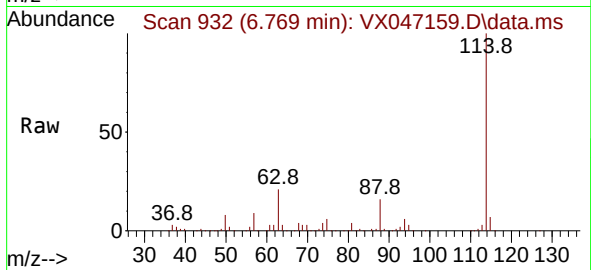

#35
Dibromofluoromethane
Concen: 48.388 ug/l
RT: 5.397 min Scan# 707
Delta R.T. 0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20

Tgt Ion:113 Resp: 161741
Ion Ratio Lower Upper
113 100
111 102.9 82.6 124.0
192 18.4 14.9 22.3


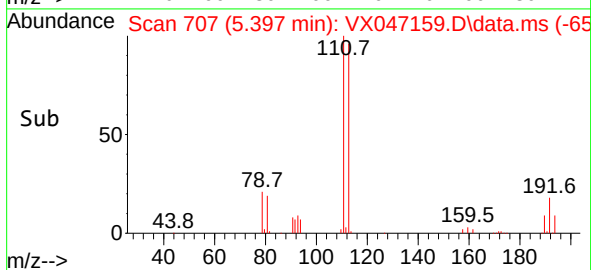
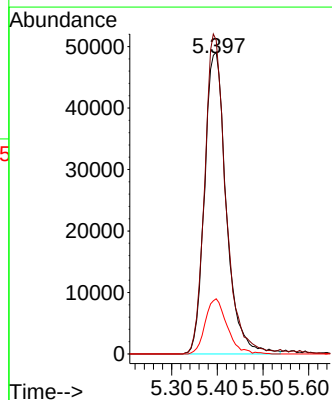
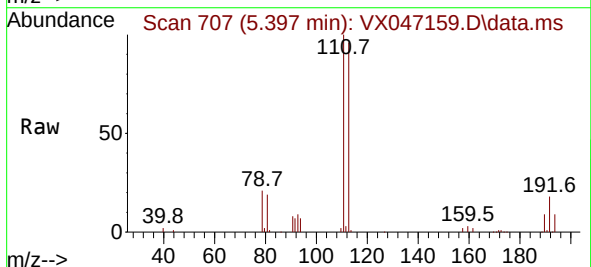


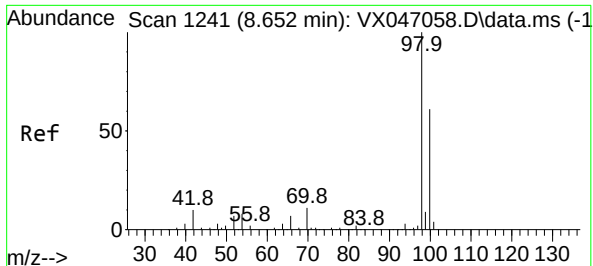

#50
Toluene-d8
Concen: 45.684 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20




Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5


Tgt Ion: 98 Resp: 494526
Ion Ratio Lower Upper
98 100
100 67.0 53.3 79.9

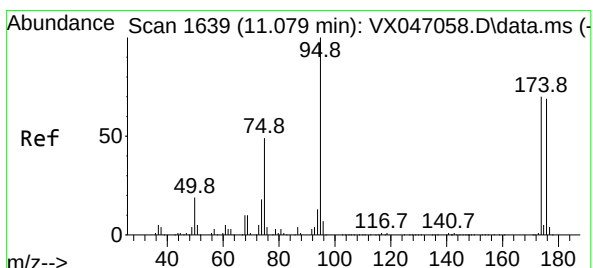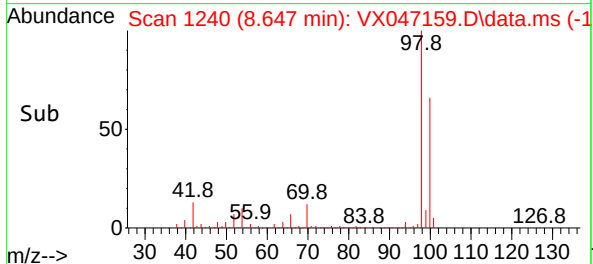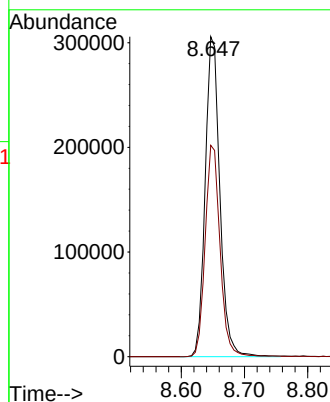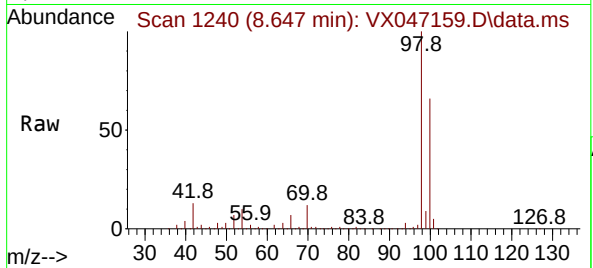

#62
4-Bromofluorobenzene
Concen: 48.847 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20

Tgt Ion: 95 Resp: 227868
Ion Ratio Lower Upper
95 100
174 72.1 0.0 144.6
176 69.2 0.0 139.6


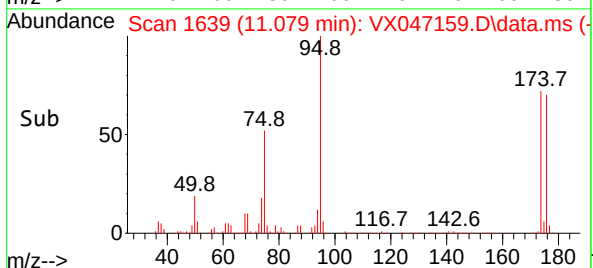
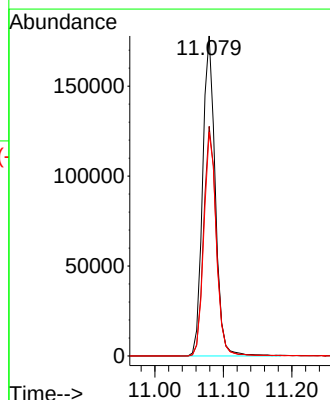
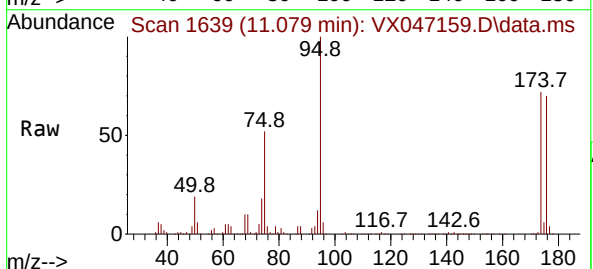


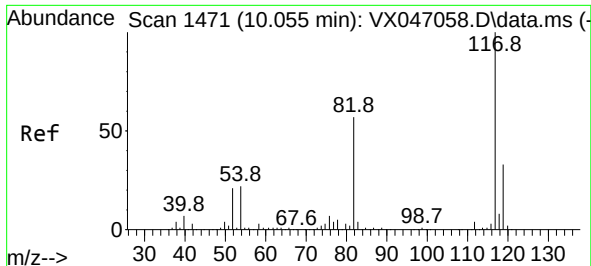

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.055 min Scan# 1471
Delta R.T. 0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20

Instrument :
MSVOA_X
ClientSampleId :
STORAGE-BLANK-WATER-REF-5

Tgt Ion:117 Resp: 484958
Ion Ratio Lower Upper
117 100
82 58.3 45.4 68.2
119 33.5 26.1 39.1

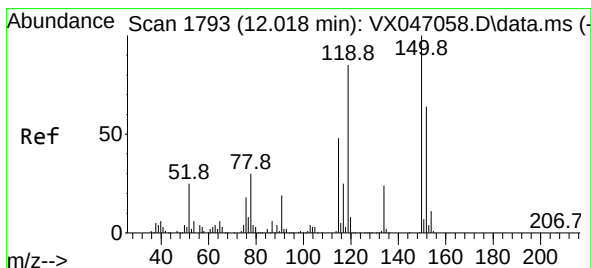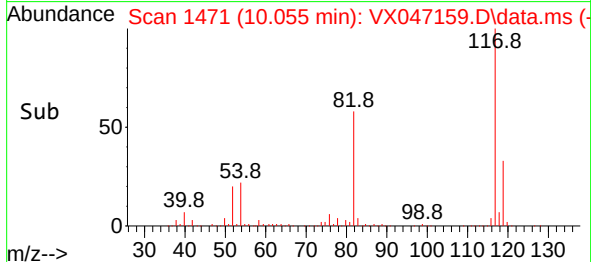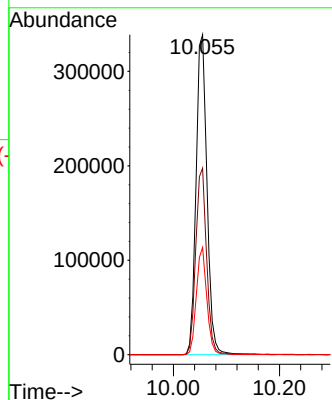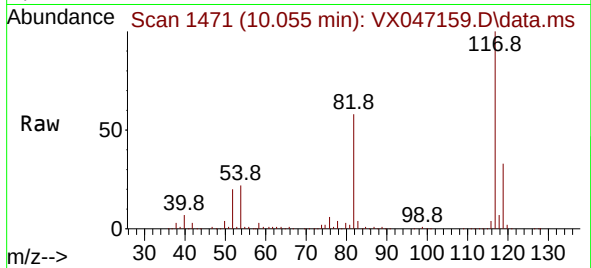

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.018 min Scan# 1793
Delta R.T. 0.000 min
Lab File: VX047159.D
Acq: 28 Jul 2025 12:20

Tgt Ion:152 Resp: 241227
Ion Ratio Lower Upper
152 100
115 62.8 45.6 136.7
150 156.4 0.0 354.6

