
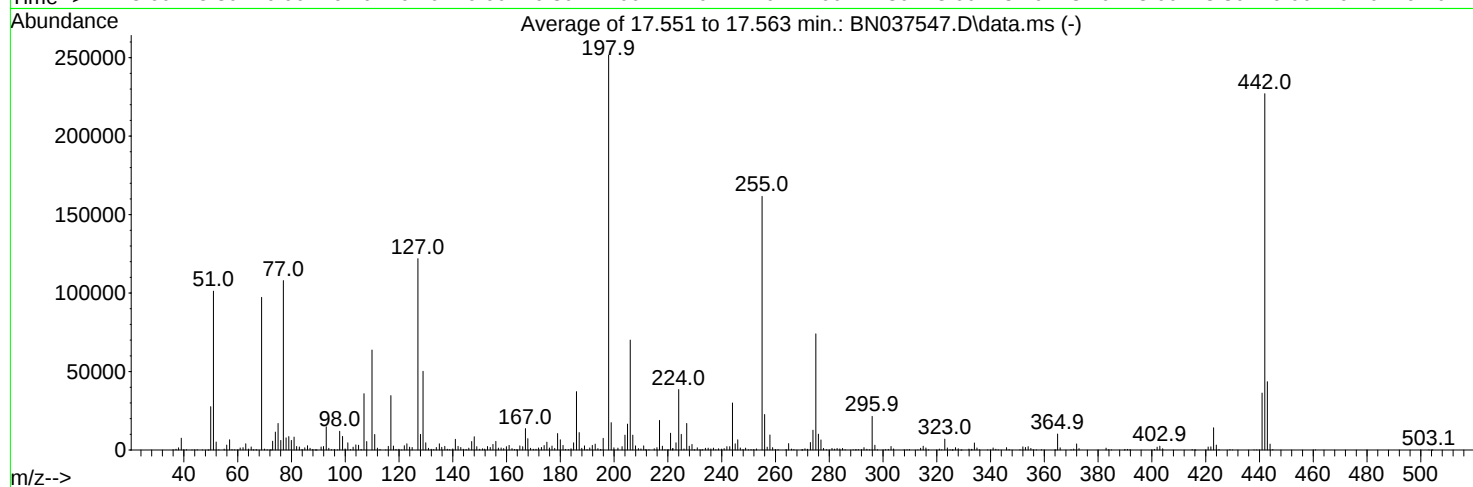


Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073025\
Data File : BN037547.D
Acq On : 30 Jul 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270-SIM-BN071525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Jul 19 01:46:16 2025

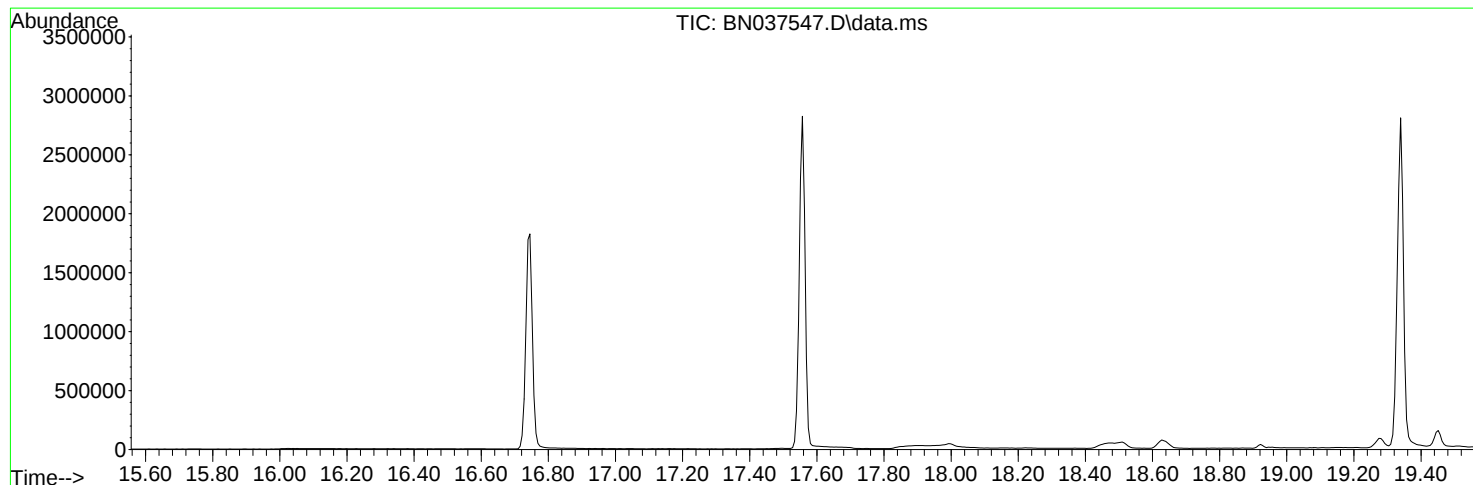




AutoFind: Scans 2459, 2460, 2461; Background Corrected with Scan 2452

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	0.0	0	PASS
69	69	100	100	100.0	97318	PASS
70	69	0.00	2	0.6	593	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	251584	PASS
199	198	5	9	6.9	17470	PASS
365	198	1	100	4.1	10254	PASS
441	443	0.01	150	83.3	36269	PASS
442	442	100	100	100.0	227008	PASS
443	442	15	24	19.2	43515	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073025\
Data File : BN037547.D
Acq On : 30 Jul 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 30 11:16:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

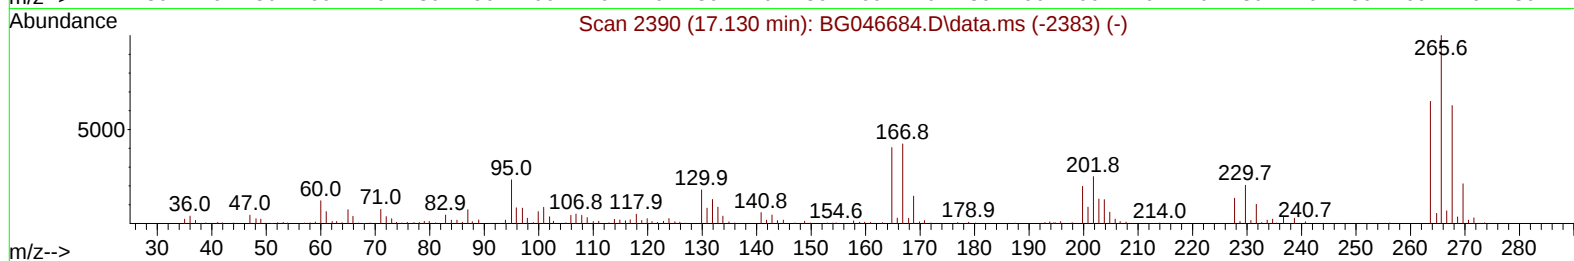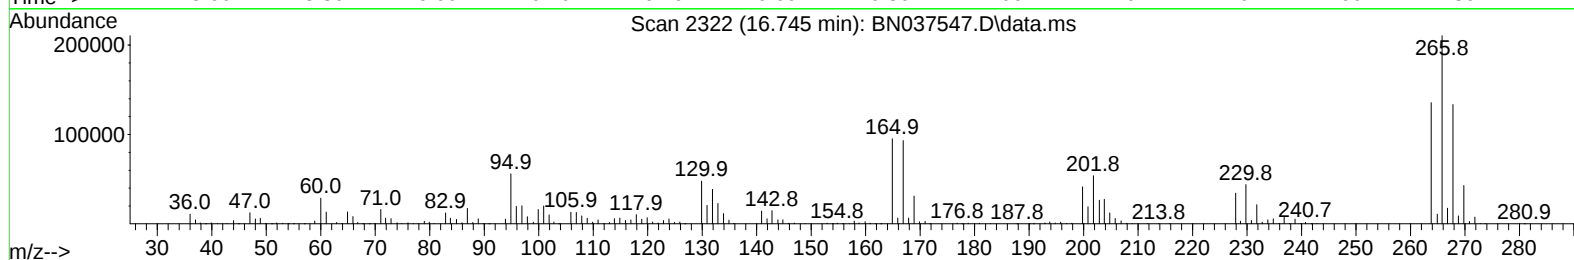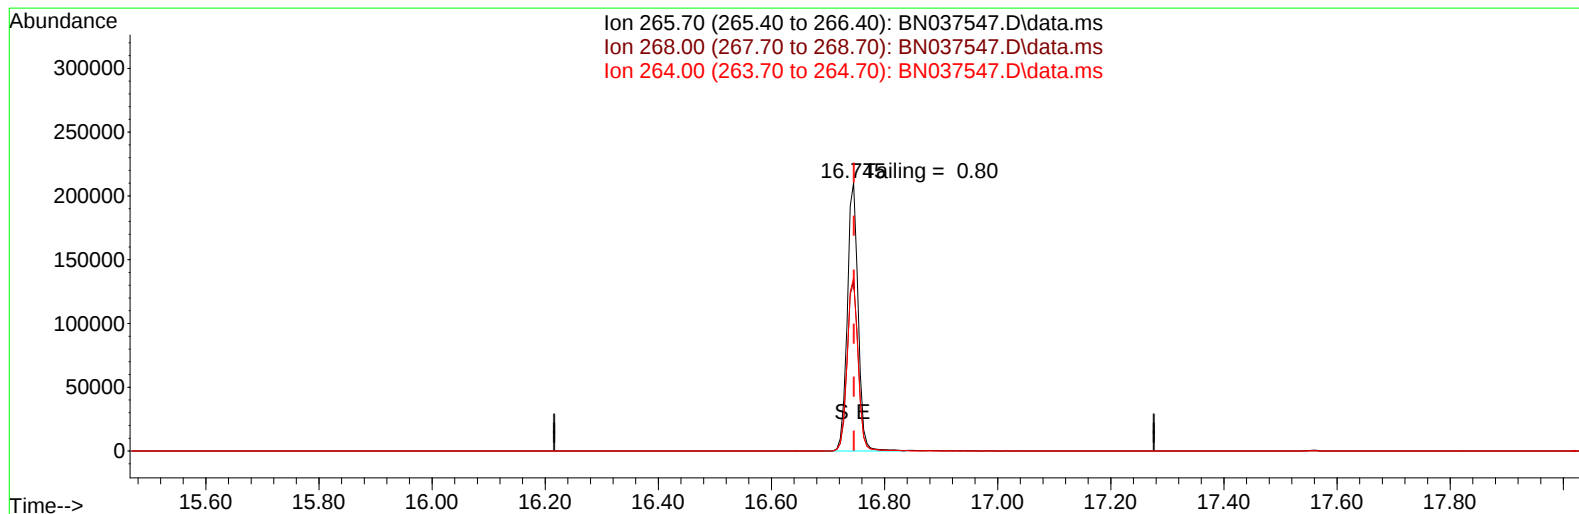

TIC: BN037547.D\data.ms

(70) Pentachlorophenol (C)

16.745min (-0.001) 22431.87 ng




response 279375

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	63.41
264.00	61.60	64.48
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_N\Data\BN073025\
Data File : BN037547.D
Acq On : 30 Jul 2025 08:59
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_N
ClientSampleId :
DFTPP

Quant Time: Jul 30 11:16:19 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_N\Methods\8270E-Tune.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 10 02:20:59 2025
Response via : Initial Calibration

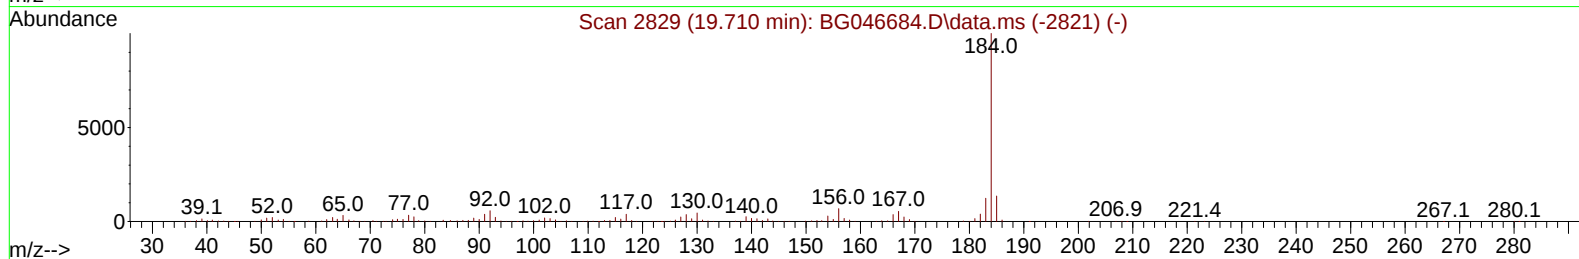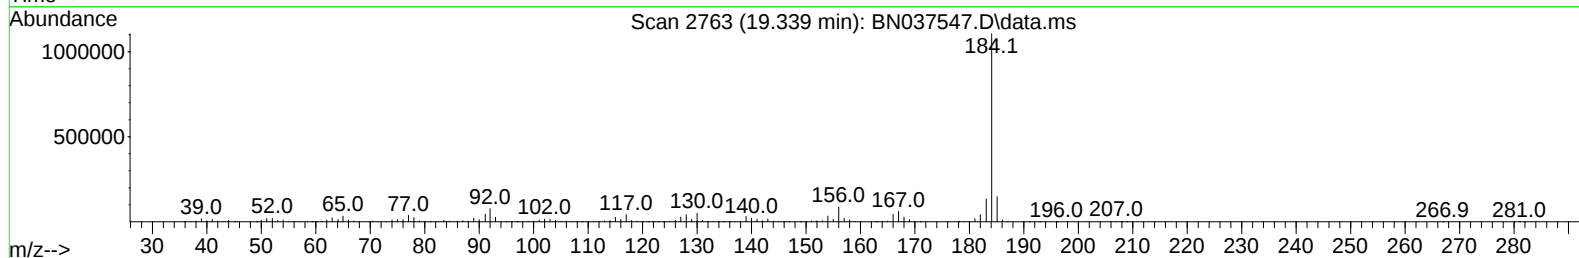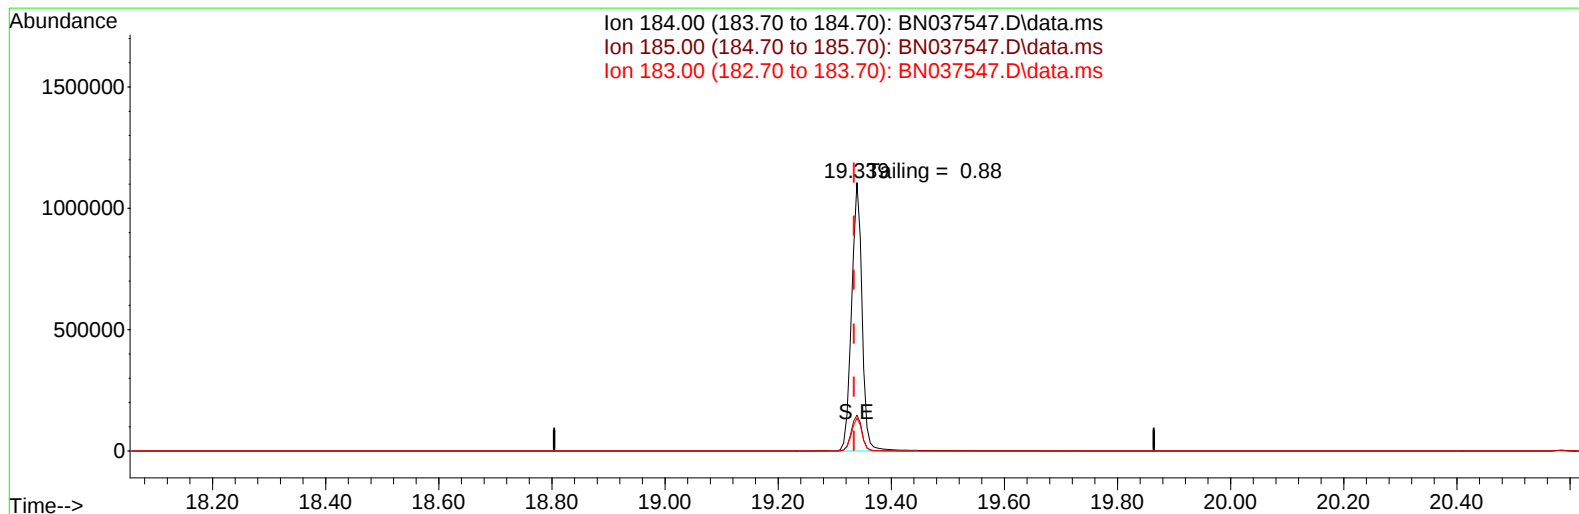

TIC: BN037547.D\data.ms

(77) Benzidine

19.339min (+ 0.005) 0.00 ng

response 1419194

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	13.39
183.00	13.20	12.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/30/2025	BNA_N	<u>BN037547.D</u>
Compound Name	Response	Retention Time
DDT	694938	20.586
DDD	7839	20.192
DDE	238	19.633
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8077	703015	1.15

Instrument :
BNA_N
ClientSampleId :
DFTPP