Instrument IC-1 Analyst : NF Method: 300.0 / 9056A

Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial \ Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-072125	7/21/2025 15:51	10 RM/IZ
STD2	0.421	0.581	0.637	2.105	0.531	1.061	3.266	IC1-072125	7/21/2025 16:12	10 RM/IZ
STD3	0.807	1.166	1.210	4.034	1.010	2.025	6.067	IC1-072125	7/21/2025 16:34	10 RM/IZ
STD4	1.035	1.665	1.541	5.126	1.284	2.567	7.677	IC1-072125	7/21/2025 16:55	10 RM/IZ
STD5	1.936	2.890	2.908	9.732	2.422	4.827	14.481	IC1-072125	7/21/2025 17:17	10 RM/IZ
STD6	3.931	5.899	5.898	19.673	4.913	9.865	29.296	IC1-072125	7/21/2025 17:38	10 RM/IZ
STD7	5.071	7.599	7.605	25.329	6.340	12.655	37.713	IC1-072125	7/21/2025 18:00	10 RM/IZ
ICV	1.900	2.803	2.815	9.537	2.323	4.754	14.170	IC1-072125	7/21/2025 18:21	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-072125	7/21/2025 18:42	10 RM/IZ
CCV	2.037	3.065	3.019	10.110	2.521	5.049	14.895	IC1-072225	7/25/2025 11:50	10 RM/IZ
CCB	0.000	0.076	0.000	0.000	0.000	0.000	0.000	IC1-072225	7/25/2025 12:12	10 RM/IZ
LB136635BLW	0.000	0.078	0.000	0.000	0.000	0.000	0.000	IC1-072225	7/25/2025 12:33	10 RM/IZ
LB136635BSW	2.035	3.072	3.021	10.164	2.545	5.115	14.989	IC1-072225	7/25/2025 12:55	10 RM/IZ
Q2695-01	0.000	10.777	0.000	0.249	3.921	0.000	2.627	IC1-072225	7/25/2025 13:16	10 RM/IZ
Q2695-01MS	2.037	13.432	2.968	10.116	6.340	5.074	16.942	IC1-072225	7/25/2025 13:38	10 RM/IZ
Q2695-01MSD	2.007	13.440	2.945	10.009	6.320	5.021	16.678	IC1-072225	7/25/2025 14:00	10 RM/IZ
Q2696-01	0.000	12.185	0.000	0.232	0.150	0.000	9.534	IC1-072225	7/25/2025 14:21	10 RM/IZ
Q2697-01	0.000	7.436	0.000	0.223	3.029	0.000	1.436	IC1-072225	7/25/2025 14:43	10 RM/IZ
Q2704-01	0.225	408.661	0.000	0.231	0.065	0.000	350.807	IC1-072225	7/25/2025 15:04	10 RM/IZ
Q2704-02	0.381	2397.121	0.000	0.210	0.000	0.000	10.982	IC1-072225	7/25/2025 15:26	10 RM/IZ
Q2704-03	0.260	1962.958	0.000	0.208	0.000	0.000	71.683	IC1-072225	7/25/2025 15:47	10 RM/IZ
CCV	1.991	3.065	3.023	10.163	2.534	5.057	15.079	IC1-072225	7/25/2025 16:30	10 RM/IZ
CCB	0.000	0.077	0.000	0.000	0.000	0.000	0.000	IC1-072225	7/25/2025 16:52	10 RM/IZ
Q2704-01DLX100	0.000	2.889	0.000	0.000	0.000	0.000	3.220	IC1-072225	7/25/2025 17:56	10 RM/IZ
Q2704-02DLX500	0.000	3.120	0.000	0.000	0.000	0.000	0.000	IC1-072225	7/25/2025 18:39	10 RM/IZ
Q2704-03DLX500	0.000	2.530	0.000	0.000	0.000	0.000	0.586	IC1-072225	7/25/2025 19:22	10 RM/IZ
CCV	2.034	3.073	3.020	10.153	2.528	5.081	14.956	IC1-072225	7/25/2025 20:05	10 RM/IZ
CCB	0.000	0.080	0.000	0.000	0.000	0.000	0.000	IC1-072225	7/25/2025 20:26	10 RM/IZ

Reviewed By:Iwona
On:7/29/2025 1:29:58 PM
Inst Id :IC-1
LB :LB136635

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A

ident	concentration F-	concentration CL-	concentration NO2	concentration BR-	concentration NO3	concentration HPO4	concentration SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-072225	7/22/2025 9:56	10	RM/IZ
STD2	0.4100	0.6170	0.6240	2.0670	0.5210	1.0490	3.2130	IC1-072225	7/22/2025 10:17	10	RM/IZ
STD3	0.8140	1.2160	1.2160	4.0280	1.0140	1.9750	6.0380	IC1-072225	7/22/2025 10:39	10	RM/IZ
STD4	1.0180	1.5360	1.5370	5.1300	1.2780	2.5790	7.7180	IC1-072225	7/22/2025 11:00	10	RM/IZ
STD5	1.9700	2.9530	2.9420	9.8490	2.4540	4.9430	14.6590	IC1-072225	7/22/2025 11:22	10	RM/IZ
STD6	3.9130	5.8540	5.8490	19.5060	4.8730	9.7400	28.9480	IC1-072225	7/22/2025 11:43	10	RM/IZ
STD7	5.0750	7.6250	7.6320	25.4200	6.3600	12.7160	37.9230	IC1-072225	7/22/2025 12:04	10	RM/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	2.5000	2.8333	4.0000	3.3500	4.2000	4.9000	7.1000
STD3	1.7500	1.3333	1.3333	0.7000	1.4000	-1.2500	0.6333
STD4	1.8000	2.4000	2.4667	2.6000	2.2400	3.1600	2.9067
STD5	-1.5000	-1.5667	-1.9333	-1.5100	-1.8400	-1.1400	-2.2733
STD6	-2.1750	-2.4333	-2.5167	-2.4700	-2.5400	-2.6000	-3.5067
STD7	1.5000	1.6667	1.7600	1.6800	1.7600	1.7280	2.4946

Reviewed By:Iwona
On:7/29/2025 1:29:58 PM
Inst Id :IC-1
LB :LB136635

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Fluoride (Anions)

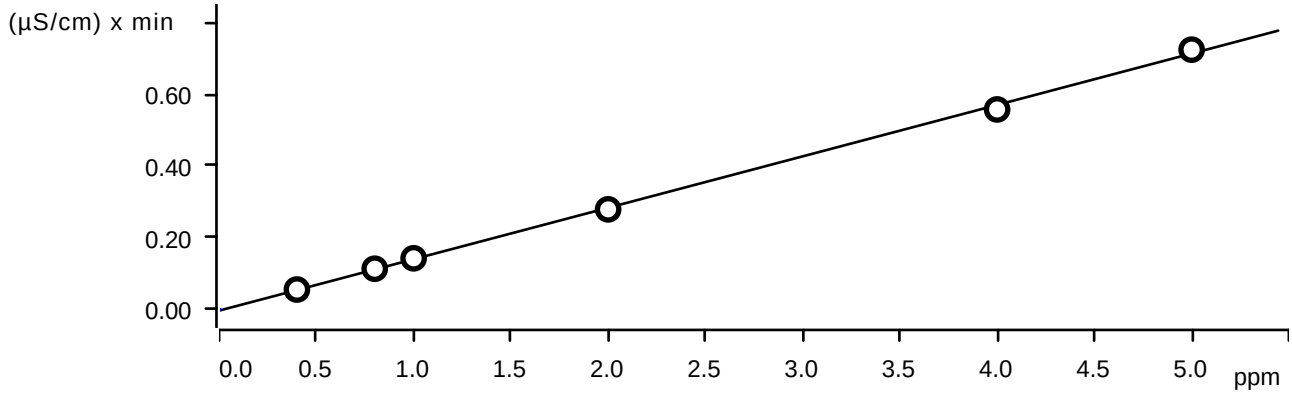

Function: . . . . . *A = - 3.58174E-3 + 0.0143356× Q*

Relative standard deviation . . . . . *2.796546 %*

Correlation coefficient *0.999584*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.113	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.142	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.279	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.557	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.724	STD7	2025-07-22 12:04:57 UTC-4	used

Chloride (Anions)

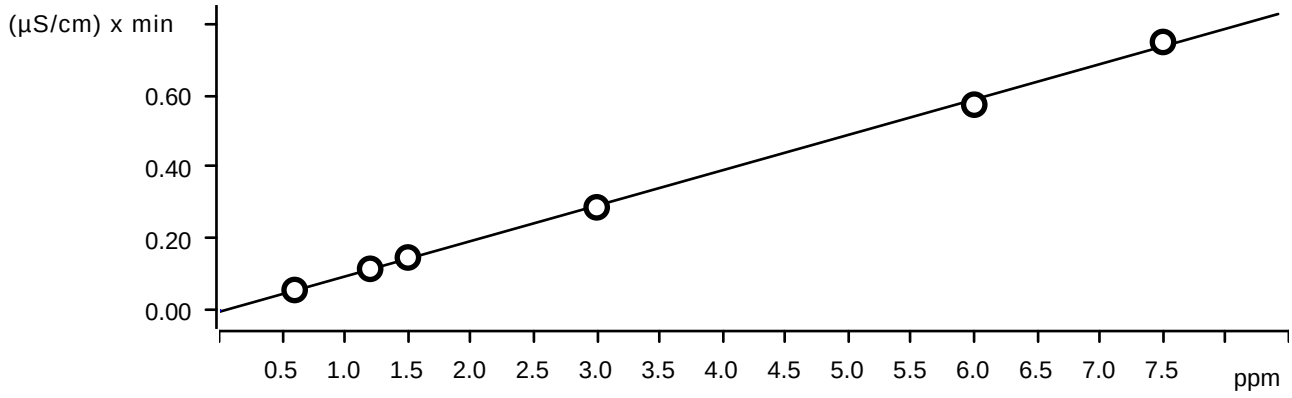

Function: . . . . . *A = - 3.86940E-3 + 9.86796E-3× Q*

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Relative standard deviation . . . . . *3.106817 %*

Correlation coefficient *0.999487*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.116	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.148	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.288	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.574	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.749	STD7	2025-07-22 12:04:57 UTC-4	used

Nitrite (Anions)

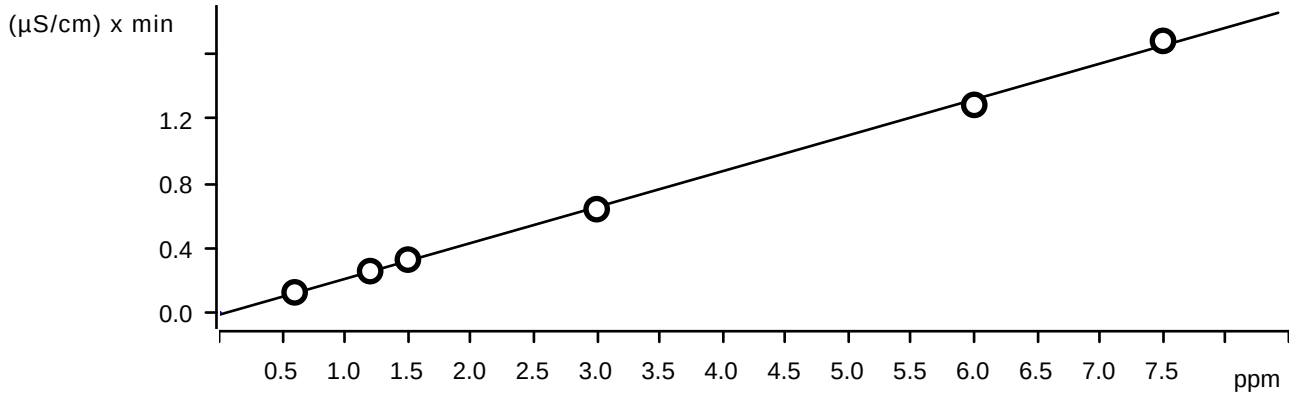

Function: . . . . . *A = - 0.0146099 + 0.0222310× Q*

Relative standard deviation . . . . . *3.309342 %*

Correlation coefficient *0.999427*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.124	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.256	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.639	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.286	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.682	STD7	2025-07-22 12:04:57 UTC-4	used

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Bromide (Anions)

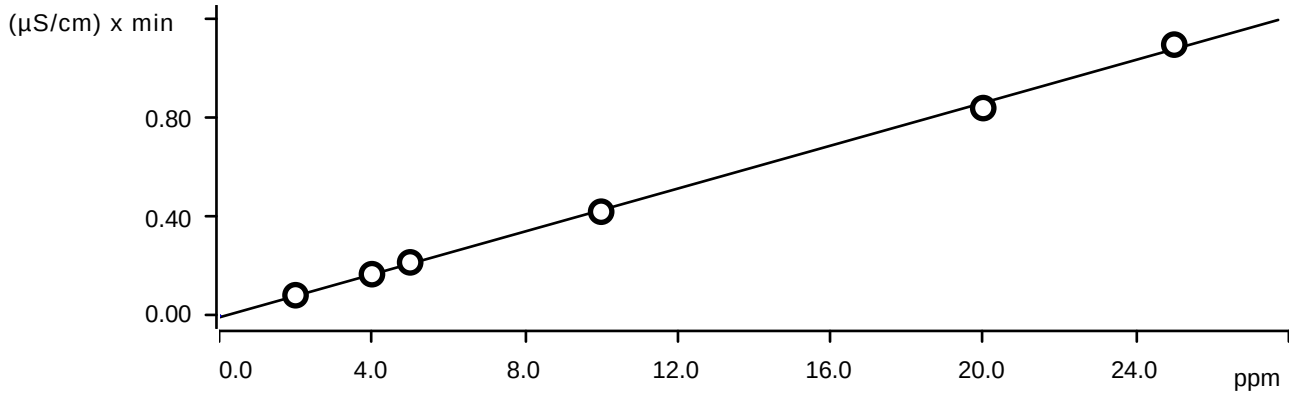

Function: . . . . . *A = - 6.30685E-3 + 4.32181E-3× Q*

Relative standard deviation . . . . . *3.140470 %*

Correlation coefficient *0.999477*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.083	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.168	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.215	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.419	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.837	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.092	STD7	2025-07-22 12:04:57 UTC-4	used

Nitrate (Anions)

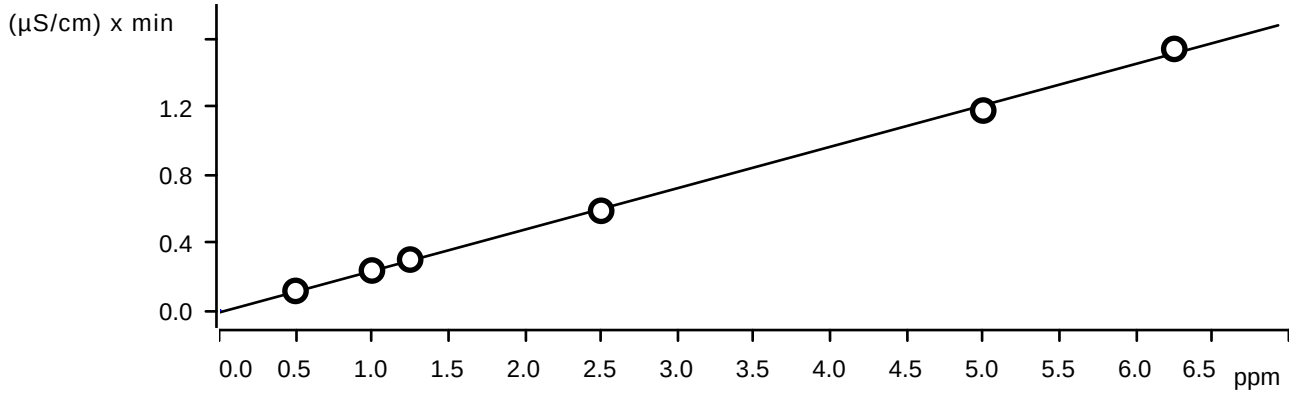

Function: . . . . . *A = - 0.0124015 + 0.0243912× Q*

Relative standard deviation . . . . . *3.299301 %*

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Correlation coefficient *0.999429*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.235	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.299	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.586	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.176	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.539	STD7	2025-07-22 12:04:57 UTC-4	used

Phosphate (Anions)

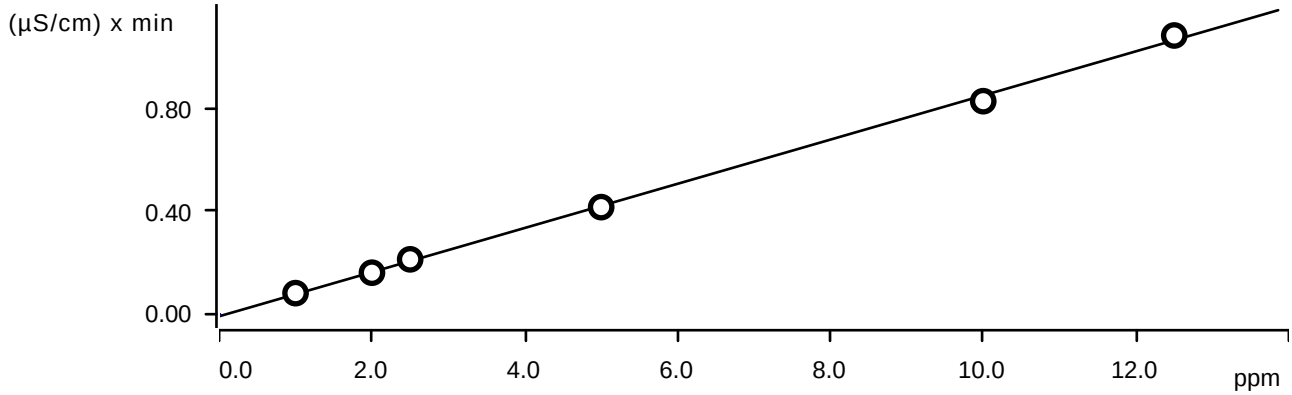

Function: . . . . . *A = - 6.54124E-3 + 8.55235E-3× Q*

Relative standard deviation . . . . . *3.281294 %*

Correlation coefficient *0.999430*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.083	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.162	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.214	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.416	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.826	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.081	STD7	2025-07-22 12:04:57 UTC-4	used

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sulfate (Anions)

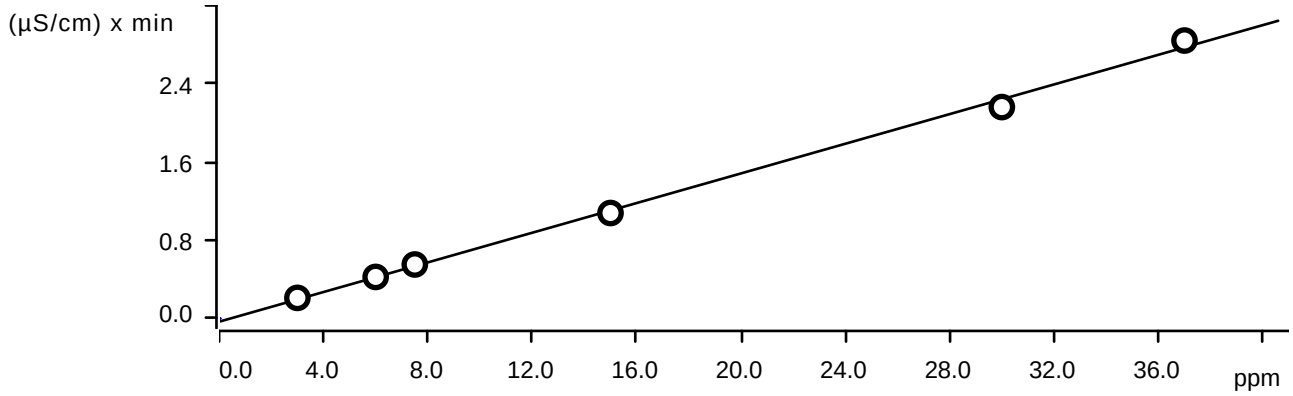

Function: . . . . . *A = - 0.0328648 + 7.57930E-3× Q*

Relative standard deviation . . . . . *4.607752 %*

Correlation coefficient *0.998893*

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-07-22 09:56:27 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.211	STD2	2025-07-22 10:17:50 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.425	STD3	2025-07-22 10:39:14 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.552	STD4	2025-07-22 11:00:38 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.078	STD5	2025-07-22 11:22:04 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.161	STD6	2025-07-22 11:43:30 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.841	STD7	2025-07-22 12:04:57 UTC-4	used

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD1	
Sample type	Standard 1	
Determination start	2025-07-22 09:56:27 UTC-4	
Method	IC1-072225	
Operator		

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.95	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

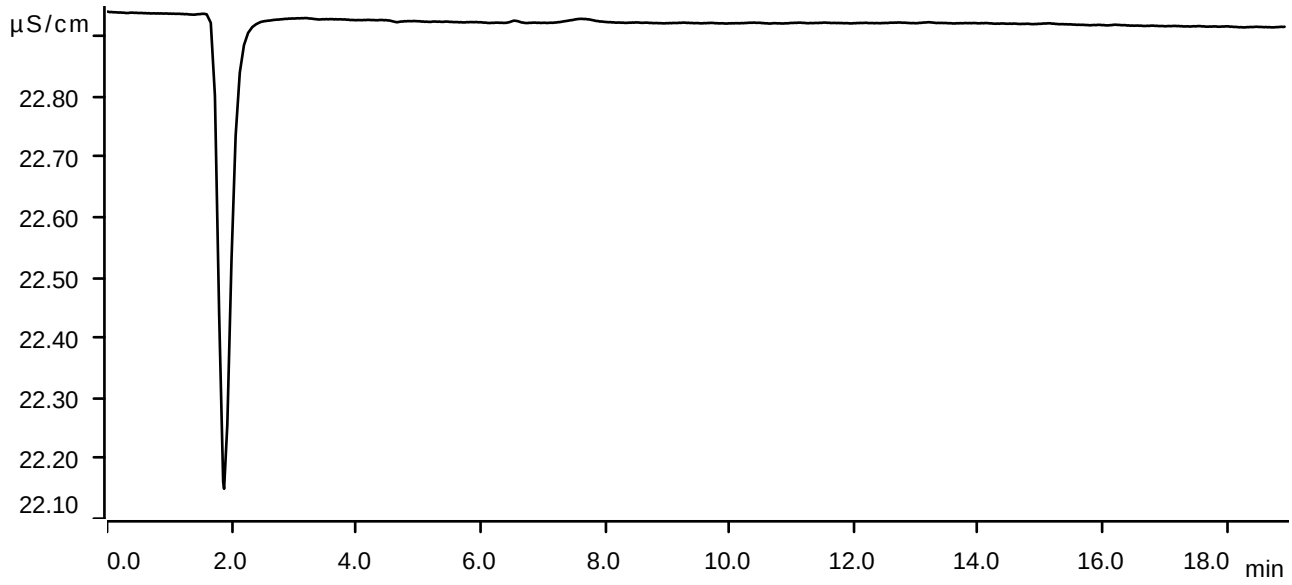

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD2
Sample type	Standard 2
Determination start	2025-07-22 10:17:50 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.78	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

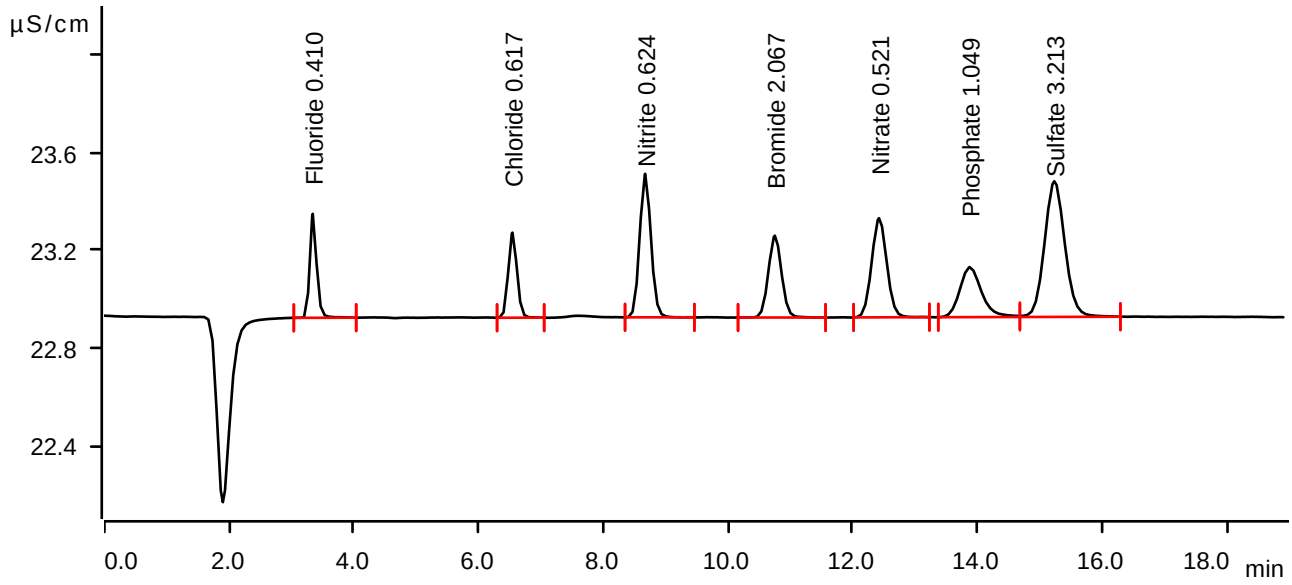

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.0552	0.426	0.410	Fluoride
2	6.543	0.0570	0.349	0.617	Chloride
3	8.672	0.1241	0.588	0.624	Nitrite
4	10.750	0.0830	0.336	2.067	Bromide
5	12.420	0.1146	0.406	0.521	Nitrate
6	13.872	0.0831	0.205	1.049	Phosphate
7	15.230	0.2106	0.556	3.213	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD3
Sample type	Standard 3
Determination start	2025-07-22 10:39:14 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.61	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

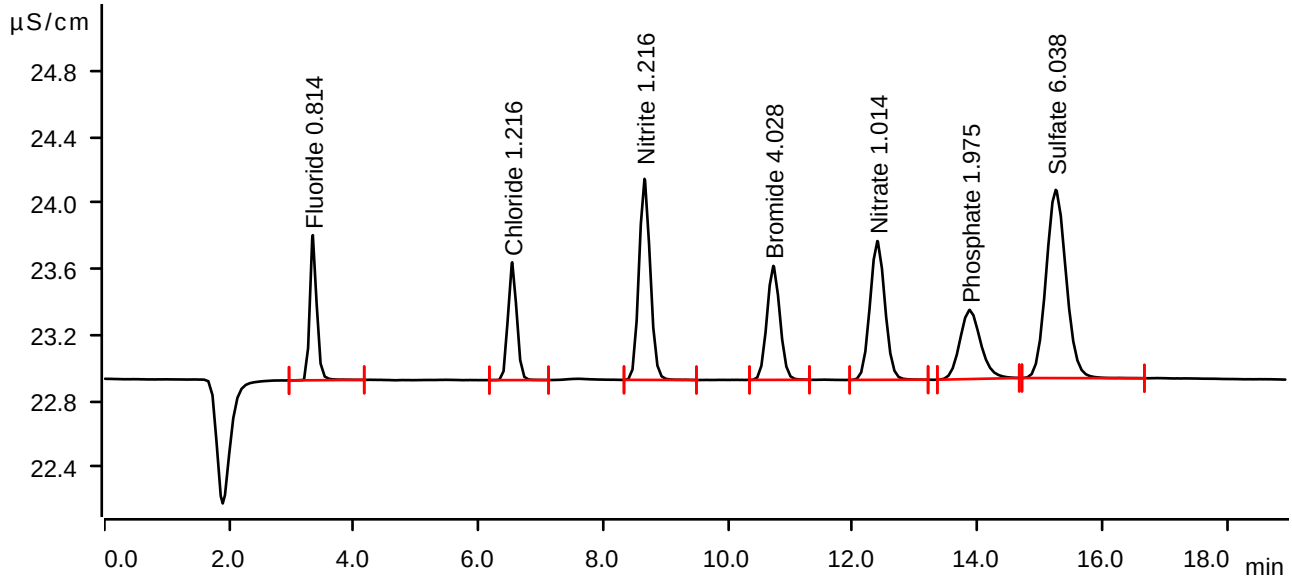

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.1132	0.878	0.814	Fluoride
2	6.540	0.1161	0.713	1.216	Chloride
3	8.660	0.2557	1.217	1.216	Nitrite
4	10.725	0.1678	0.690	4.028	Bromide
5	12.393	0.2349	0.840	1.014	Nitrate
6	13.875	0.1623	0.418	1.975	Phosphate
7	15.253	0.4248	1.139	6.038	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD4
Sample type	Standard 4
Determination start	2025-07-22 11:00:38 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.61	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

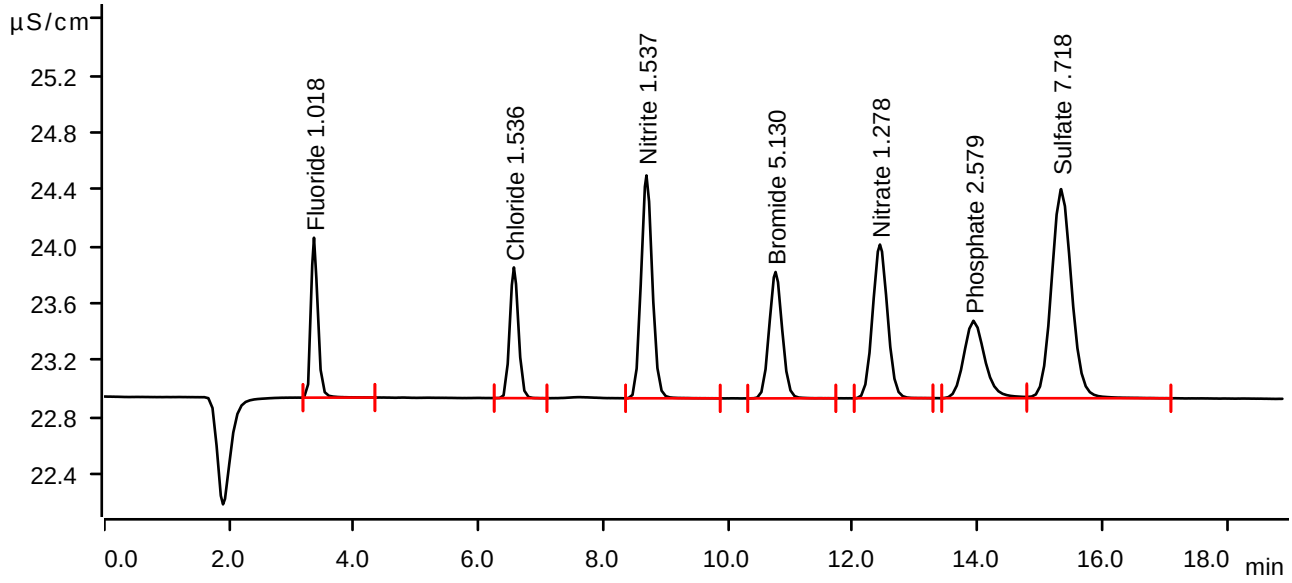

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.1423	1.123	1.018	Fluoride
2	6.567	0.1477	0.919	1.536	Chloride
3	8.692	0.3270	1.566	1.537	Nitrite
4	10.762	0.2154	0.888	5.130	Bromide
5	12.435	0.2992	1.080	1.278	Nitrate
6	13.935	0.2140	0.544	2.579	Phosphate
7	15.340	0.5521	1.470	7.718	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD5
Sample type	Standard 5
Determination start	2025-07-22 11:22:04 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.50	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

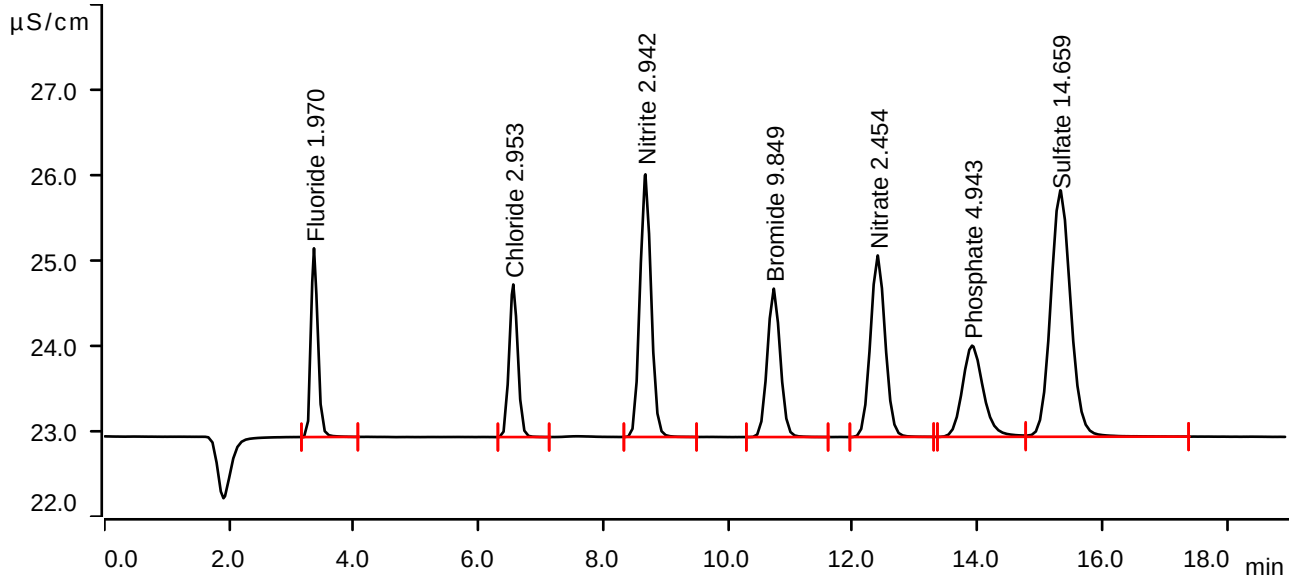

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2788	2.210	1.970	Fluoride
2	6.557	0.2875	1.787	2.953	Chloride
3	8.675	0.6394	3.077	2.942	Nitrite
4	10.732	0.4194	1.738	9.849	Bromide
5	12.398	0.5862	2.127	2.454	Nitrate
6	13.912	0.4162	1.068	4.943	Phosphate
7	15.327	1.0782	2.887	14.659	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD6
Sample type	Standard 6
Determination start	2025-07-22 11:43:30 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.44	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

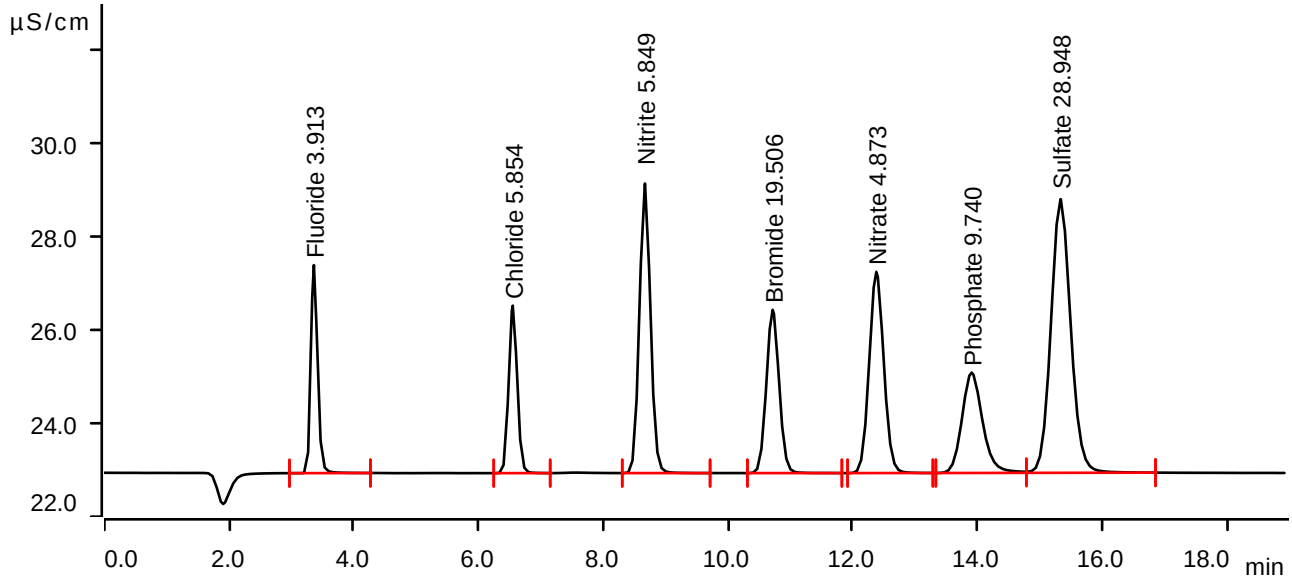

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.5573	4.466	3.913	Fluoride
2	6.548	0.5738	3.596	5.854	Chloride
3	8.667	1.2857	6.219	5.849	Nitrite
4	10.715	0.8367	3.507	19.506	Bromide
5	12.377	1.1762	4.321	4.873	Nitrate
6	13.905	0.8264	2.155	9.740	Phosphate
7	15.330	2.1612	5.877	28.948	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	STD7
Sample type	Standard 7
Determination start	2025-07-22 12:04:57 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.44	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Anions

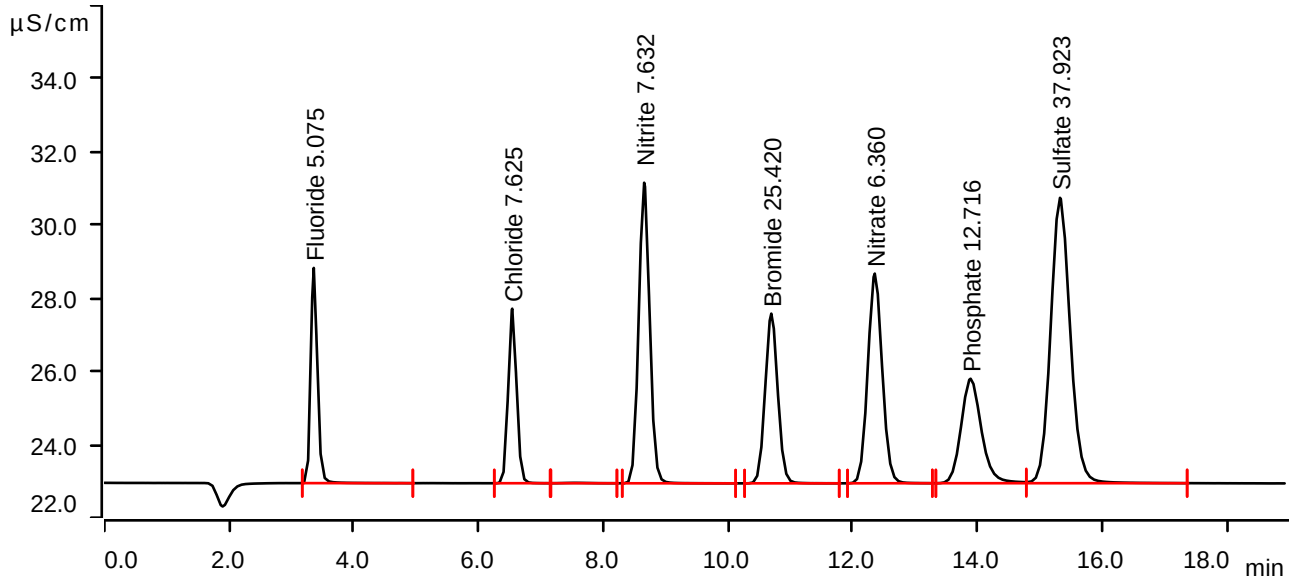

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.7240	5.880	5.075	Fluoride
2	6.540	0.7486	4.770	7.625	Chloride
3	7.532	0.0048	0.011	invalid	
4	8.655	1.6821	8.216	7.632	Nitrite
5	10.693	1.0923	4.639	25.420	Bromide
6	12.352	1.5390	5.732	6.360	Nitrate
7	13.888	1.0809	2.856	12.716	Phosphate
8	15.322	2.8415	7.800	37.923	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	ICV
Sample type	Check standard 1
Determination start	2025-07-22 12:26:25 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.39	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

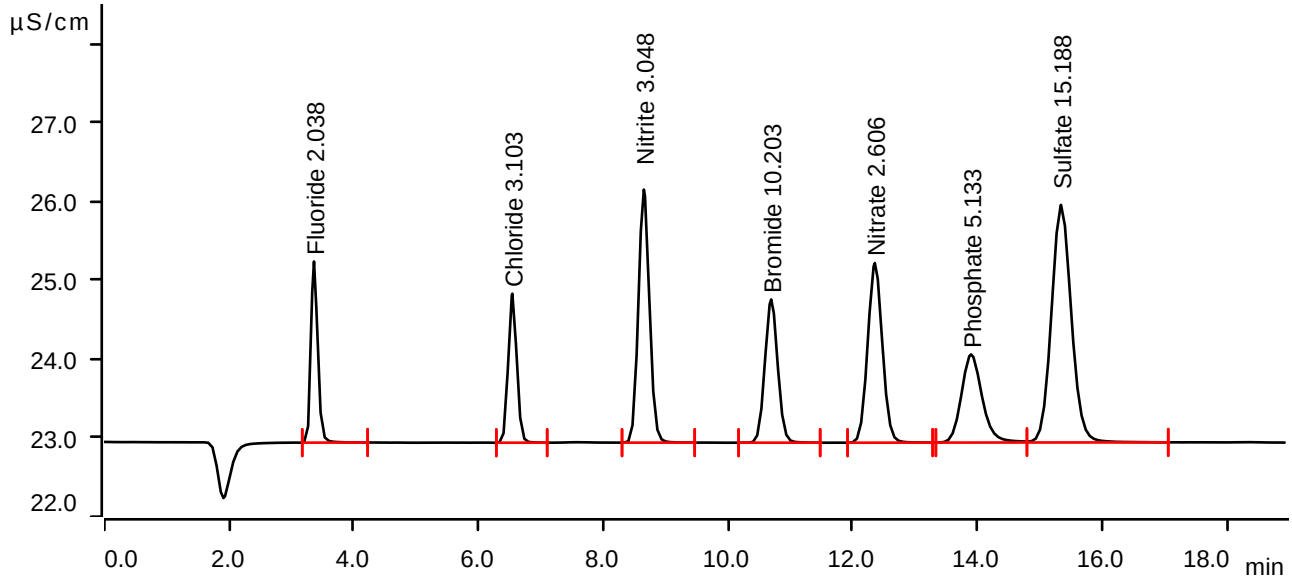

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2885	2.298	2.038	Fluoride
2	6.542	0.3023	1.891	3.103	Chloride
3	8.650	0.6629	3.211	3.048	Nitrite
4	10.692	0.4347	1.818	10.203	Bromide
5	12.353	0.6232	2.280	2.606	Nitrate
6	13.897	0.4324	1.119	5.133	Phosphate
7	15.338	1.1182	3.014	15.188	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	ICB	
Sample type	Sample	
Determination start	2025-07-22 12:47:54 UTC-4	
Method	IC1-072225	
Operator		

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.39	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

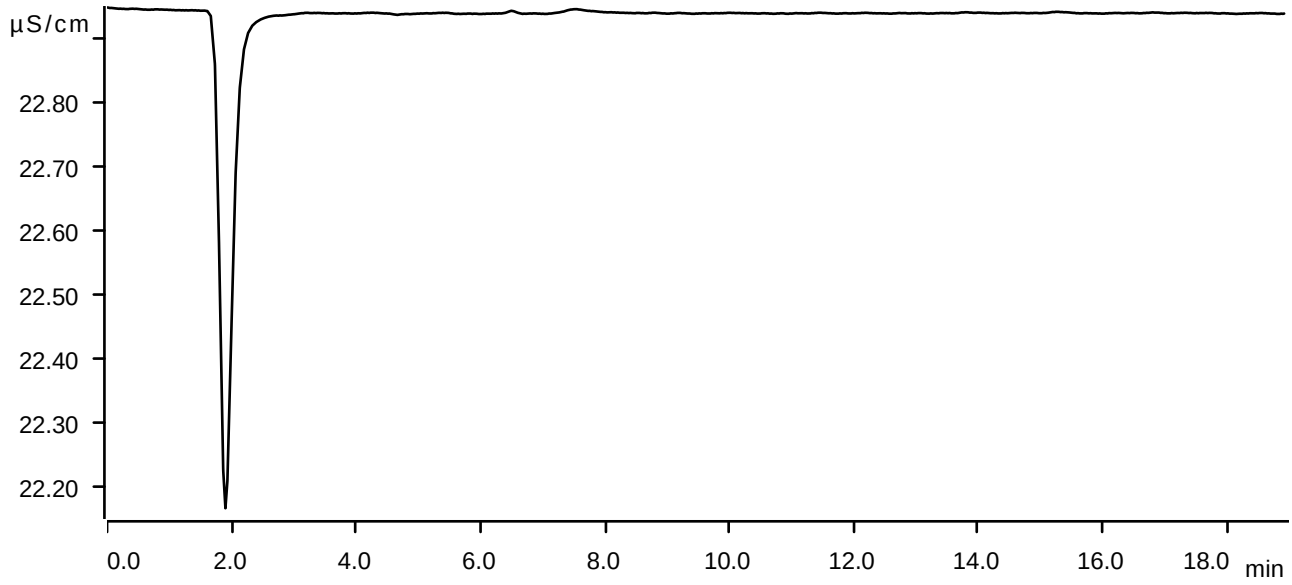

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	CCV
Sample type	Check standard 1
Determination start	2025-07-25 11:50:52 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	12.11	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

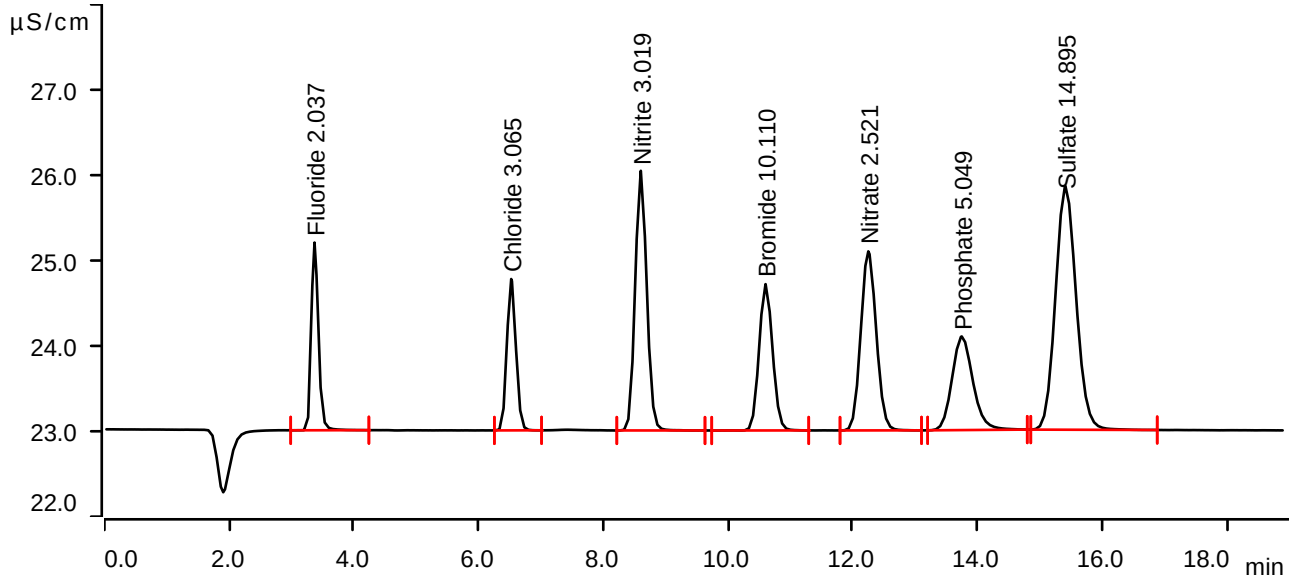

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.2884	2.199	2.037	Fluoride
2	6.523	0.2986	1.773	3.065	Chloride
3	8.600	0.6566	3.042	3.019	Nitrite
4	10.602	0.4306	1.714	10.110	Bromide
5	12.248	0.6025	2.097	2.521	Nitrate
6	13.747	0.4253	1.097	5.049	Phosphate
7	15.408	1.0961	2.854	14.895	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	CCB
Sample type	Sample
Determination start	2025-07-25 12:12:22 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.99	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

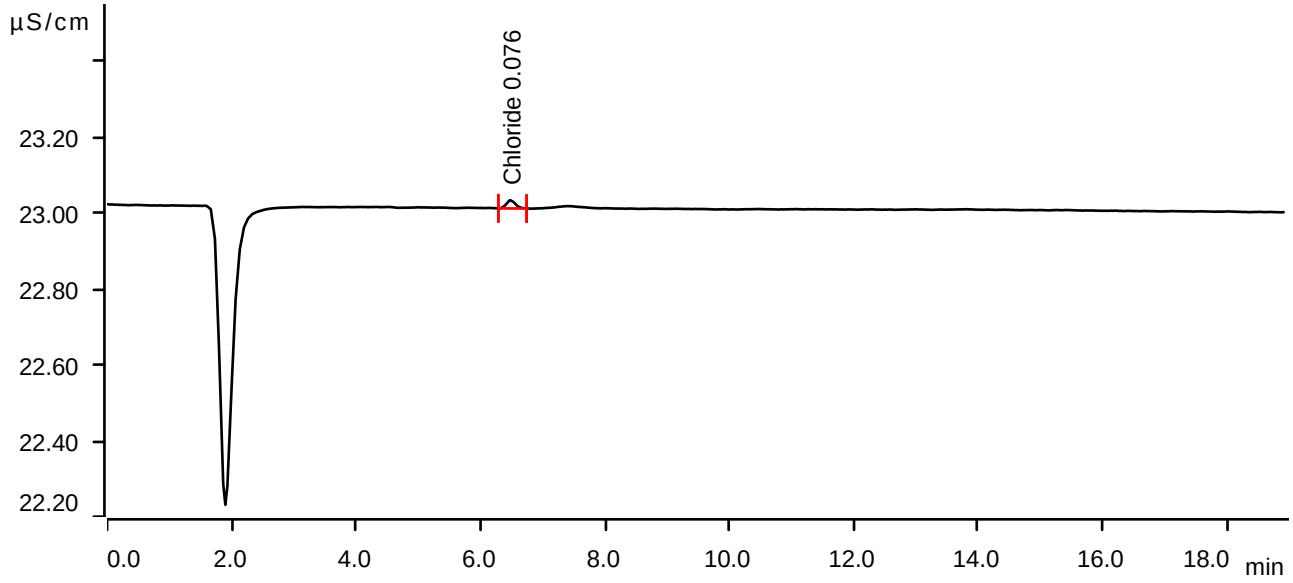

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.483	0.0036	0.021	0.076	Chloride

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	LB136635BLW
Sample type	Sample
Determination start	2025-07-25 12:33:52 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.88	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

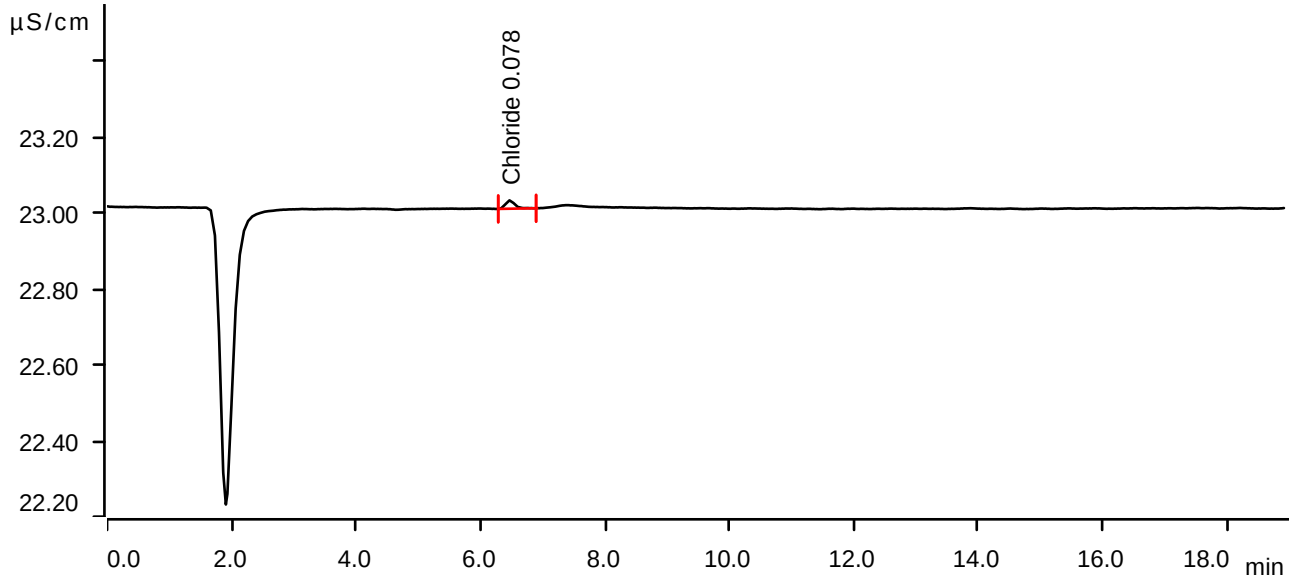

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	6.468	0.0038	0.022	0.078	Chloride

Metrohm

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	LB136635BSW
Sample type	Check standard 1
Determination start	2025-07-25 12:55:23 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.88	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

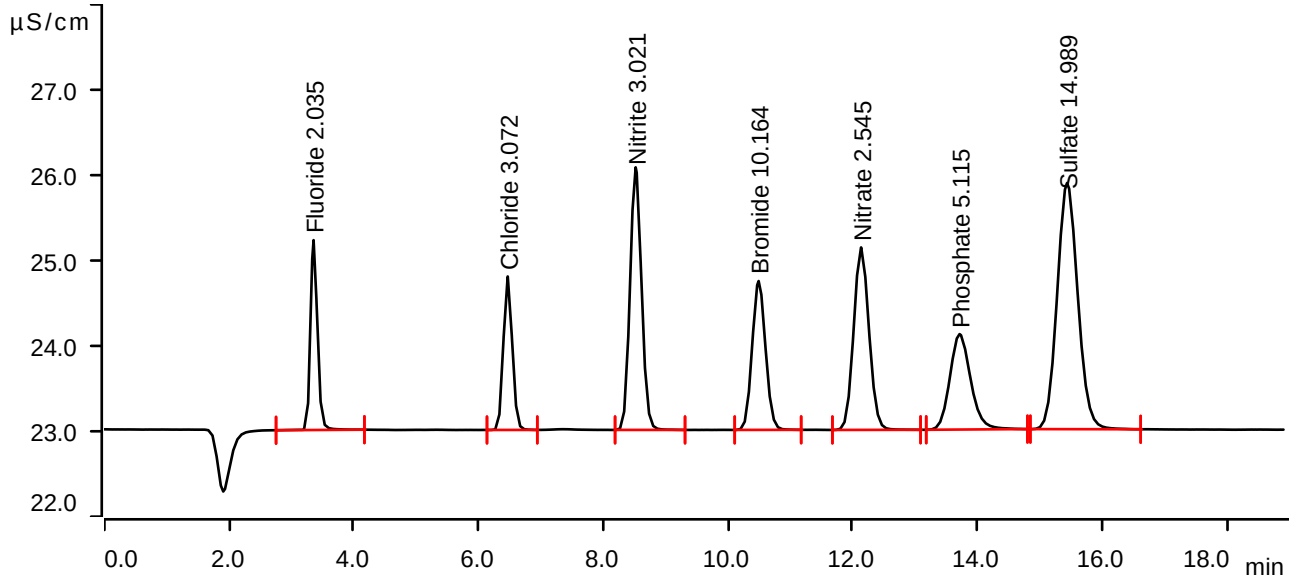

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2881	2.224	2.035	Fluoride
2	6.467	0.2992	1.798	3.072	Chloride
3	8.518	0.6570	3.076	3.021	Nitrite
4	10.490	0.4330	1.744	10.164	Bromide
5	12.132	0.6085	2.137	2.545	Nitrate
6	13.712	0.4309	1.118	5.115	Phosphate
7	15.435	1.1032	2.883	14.989	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2695-01
Sample type	Sample
Determination start	2025-07-25 13:16:56 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.77	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

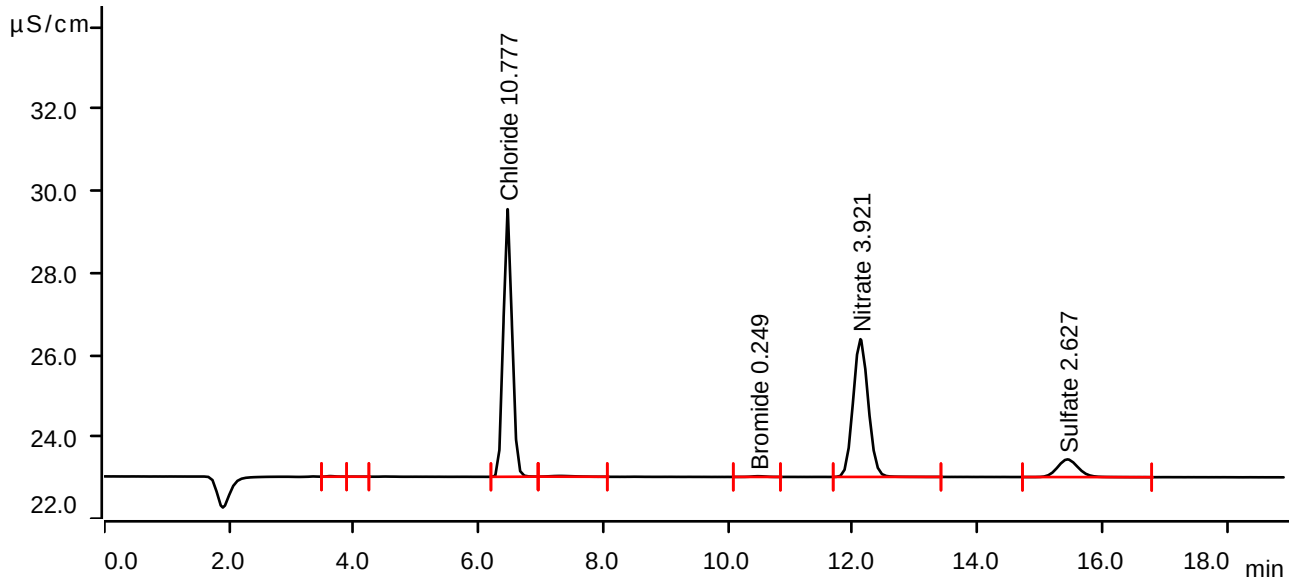

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.625	0.0023	0.015	invalid	
2	3.958	0.0002	0.001	invalid	
3	6.465	1.0596	6.530	10.777	Chloride
4	7.285	0.0083	0.018	invalid	
5	10.480	0.0045	0.017	0.249	Bromide
6	12.122	0.9439	3.361	3.921	Nitrate
7	15.442	0.1663	0.431	2.627	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2695-01MS	
Sample type	Sample	
Determination start	2025-07-25 13:38:29 UTC-4	
Method	IC1-072225	
Operator		

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.77	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Anions

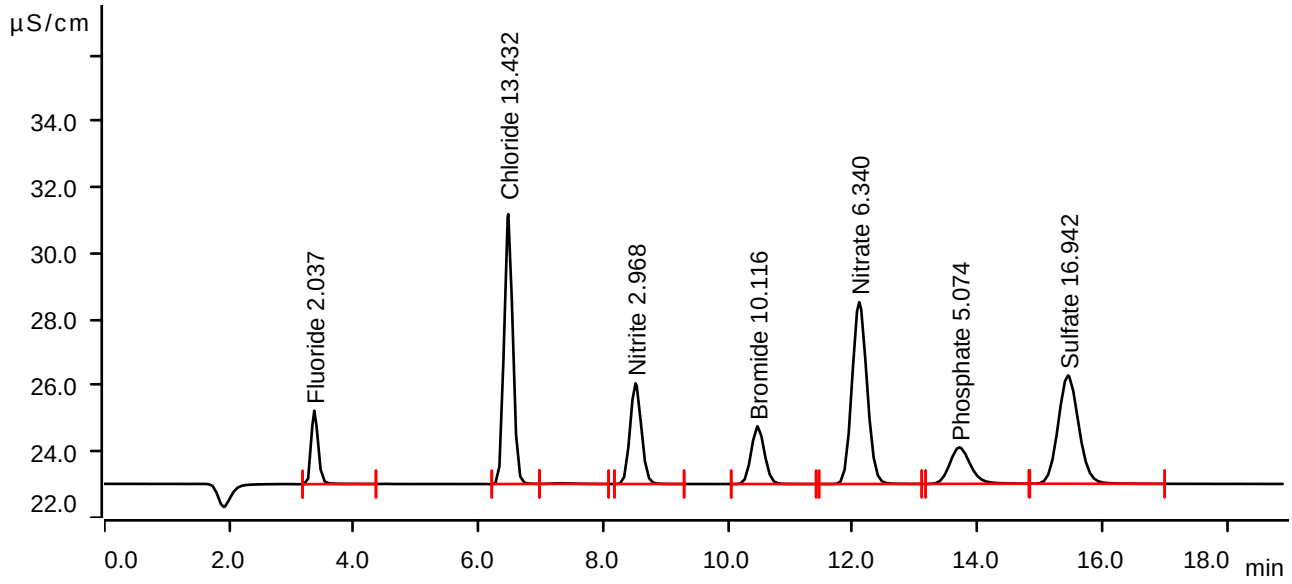

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.2884	2.223	2.037	Fluoride
2	6.477	1.3216	8.165	13.432	Chloride
3	7.300	0.0083	0.019	invalid	
4	8.517	0.6451	3.045	2.968	Nitrite
5	10.473	0.4309	1.746	10.116	Bromide
6	12.103	1.5340	5.503	6.340	Nitrate
7	13.708	0.4274	1.105	5.074	Phosphate
8	15.450	1.2512	3.276	16.942	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2695-01MSD	
Sample type	Sample	
Determination start	2025-07-25 14:00:02 UTC-4	
Method	IC1-072225	
Operator		

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.77	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Anions

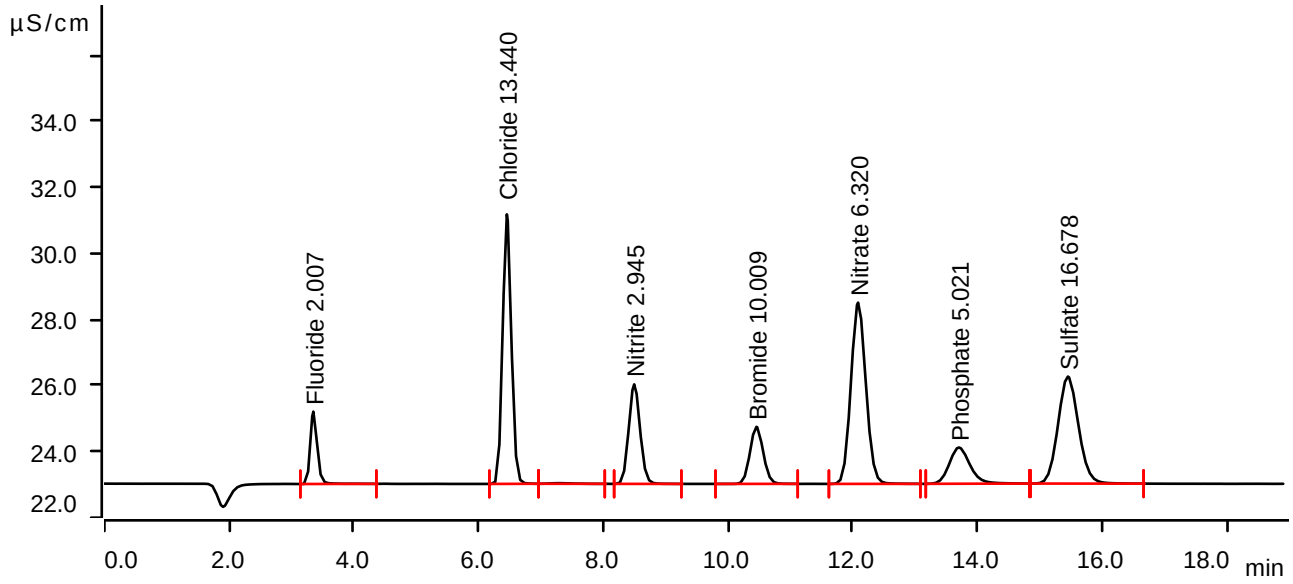

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2841	2.189	2.007	Fluoride
2	6.453	1.3224	8.155	13.440	Chloride
3	7.302	0.0077	0.019	invalid	
4	8.495	0.6401	3.012	2.945	Nitrite
5	10.455	0.4263	1.727	10.009	Bromide
6	12.085	1.5290	5.486	6.320	Nitrate
7	13.702	0.4229	1.098	5.021	Phosphate
8	15.448	1.2312	3.240	16.678	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2696-01
Sample type	Sample
Determination start	2025-07-25 14:21:37 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.71	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

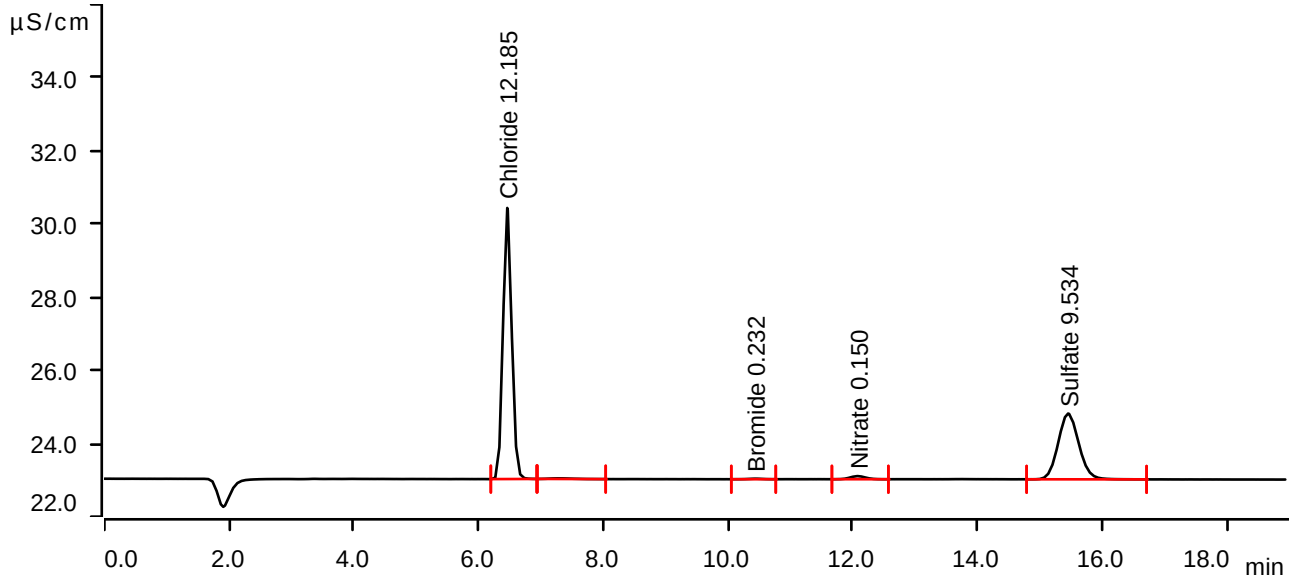

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.460	1.1985	7.409	12.185	Chloride
2	7.300	0.0074	0.017	invalid	
3	10.432	0.0037	0.015	0.232	Bromide
4	12.080	0.0242	0.085	0.150	Nitrate
5	15.452	0.6898	1.798	9.534	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2697-01
Sample type	Sample
Determination start	2025-07-25 14:43:11 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.71	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

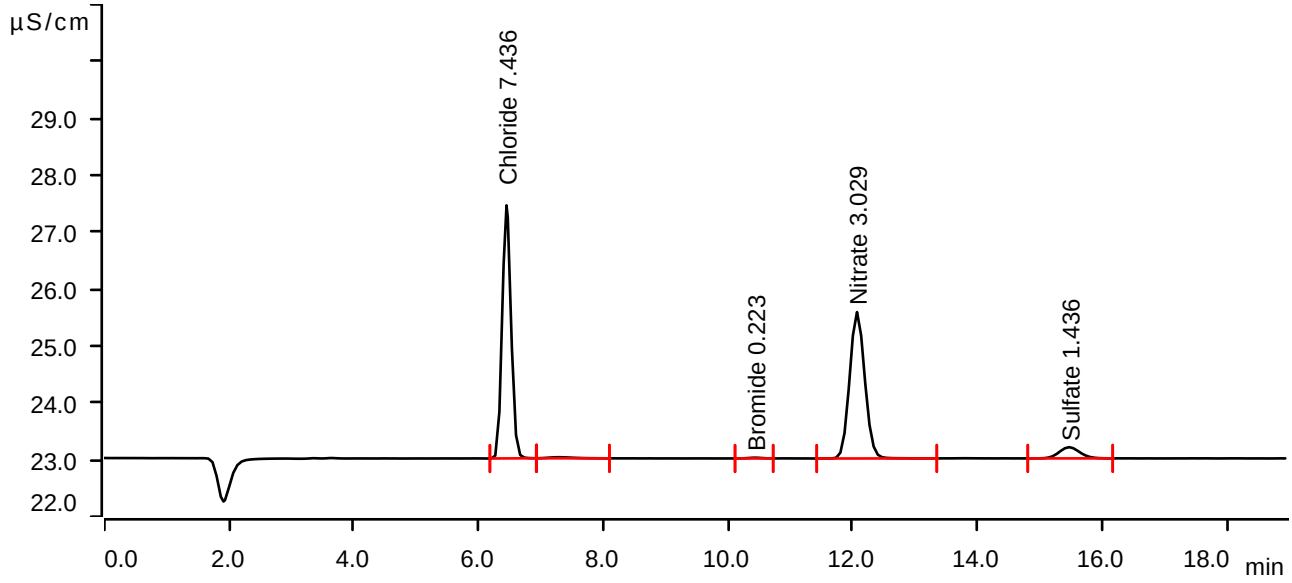

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.448	0.7299	4.446	7.436	Chloride
2	7.265	0.0086	0.019	invalid	
3	10.437	0.0033	0.013	0.223	Bromide
4	12.067	0.7263	2.572	3.029	Nitrate
5	15.472	0.0760	0.196	1.436	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2704-01	
Sample type	Sample	
Determination start	2025-07-25 15:04:46 UTC-4	
Method	IC1-072225	
Operator		

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.60	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Anions

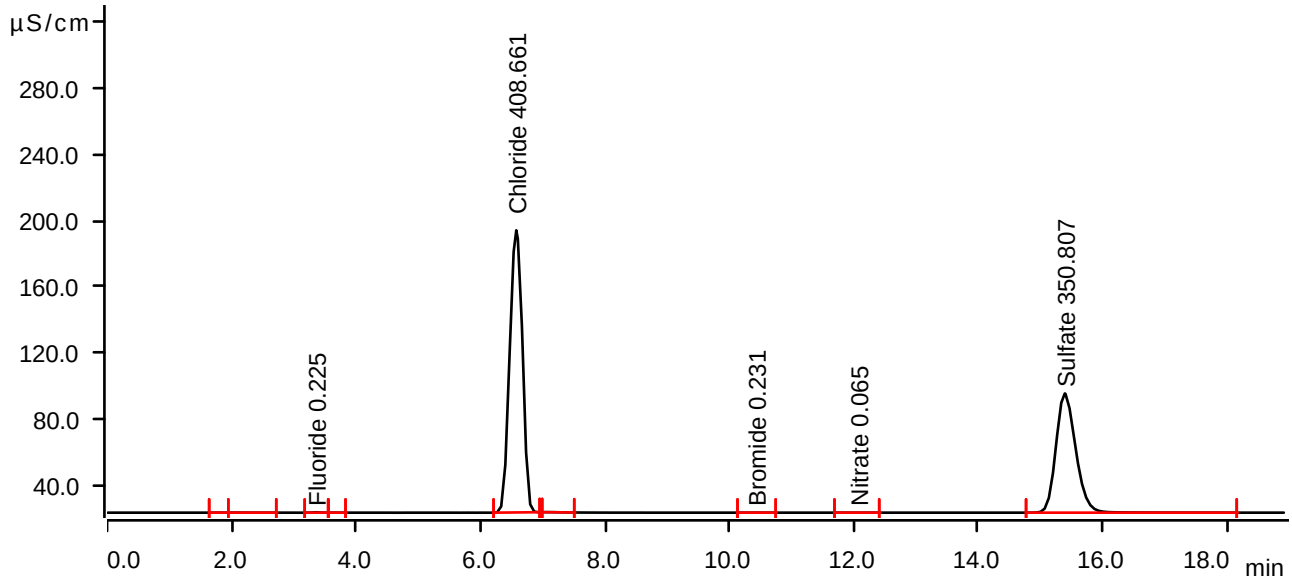

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.833	0.0047	0.029	invalid	
2	2.092	0.0092	0.033	invalid	
3	3.355	0.0287	0.225	0.225	Fluoride
4	3.648	0.0011	0.008	invalid	
5	6.577	40.3227	170.758	408.661	Chloride
6	7.075	0.0164	0.057	invalid	
7	10.425	0.0037	0.015	0.231	Bromide
8	12.070	0.0034	0.012	0.065	Nitrate
9	15.390	26.5558	72.161	350.807	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2704-02
Sample type	Sample
Determination start	2025-07-25 15:26:20 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.71	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

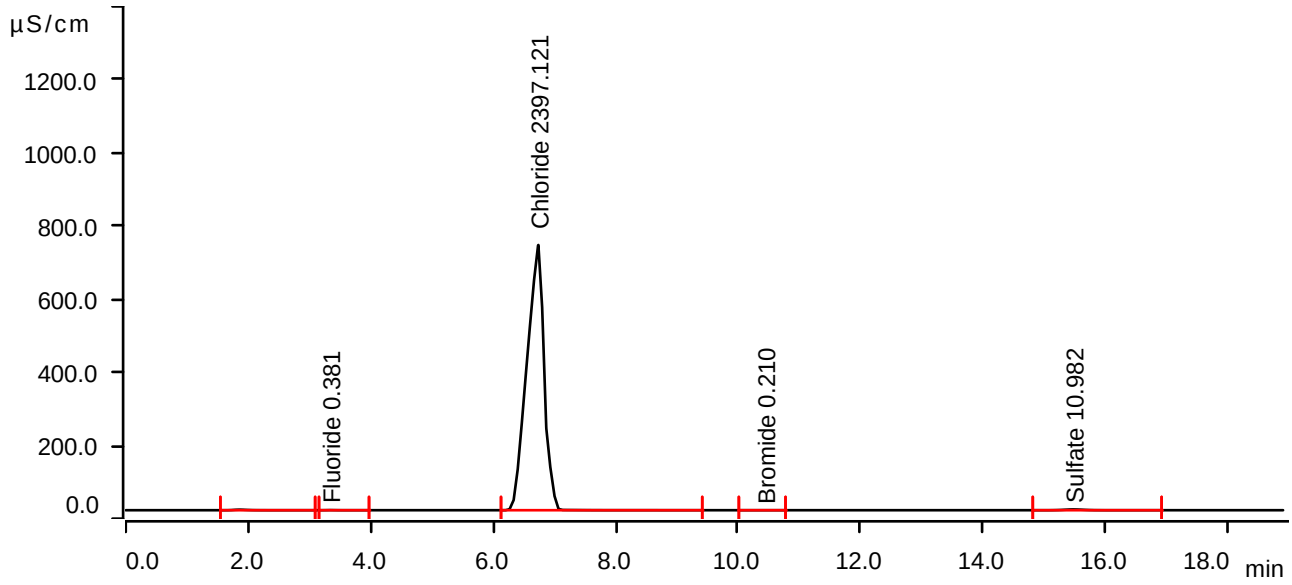

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.857	0.3886	1.531	invalid	
2	3.338	0.0510	0.365	0.381	Fluoride
3	6.738	236.5432	724.889	2397.121	Chloride
4	10.440	0.0028	0.011	0.210	Bromide
5	15.473	0.7995	2.100	10.982	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2704-03
Sample type	Sample
Determination start	2025-07-25 15:47:52 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.60	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

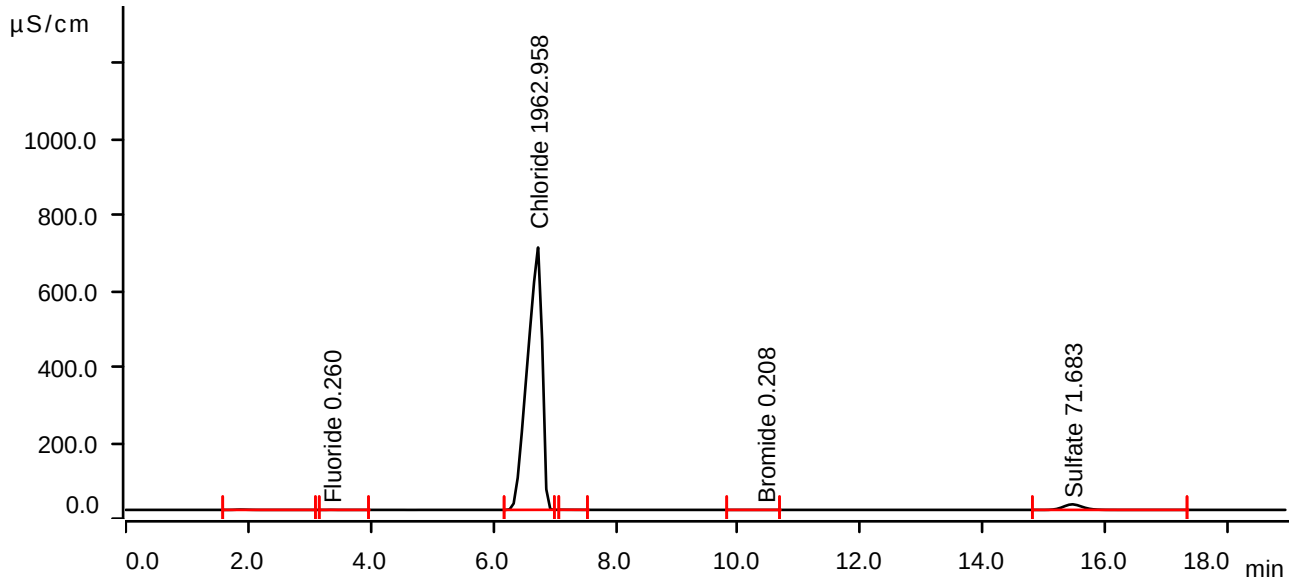

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.880	0.2183	0.874	invalid	
2	3.353	0.0337	0.245	0.260	Fluoride
3	6.732	193.7001	691.411	1962.958	Chloride
4	7.138	0.0165	0.066	invalid	
5	10.410	0.0027	0.010	0.208	Bromide
6	15.455	5.4002	14.626	71.683	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	CCV
Sample type	Check standard 1
Determination start	2025-07-25 16:30:41 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.71	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

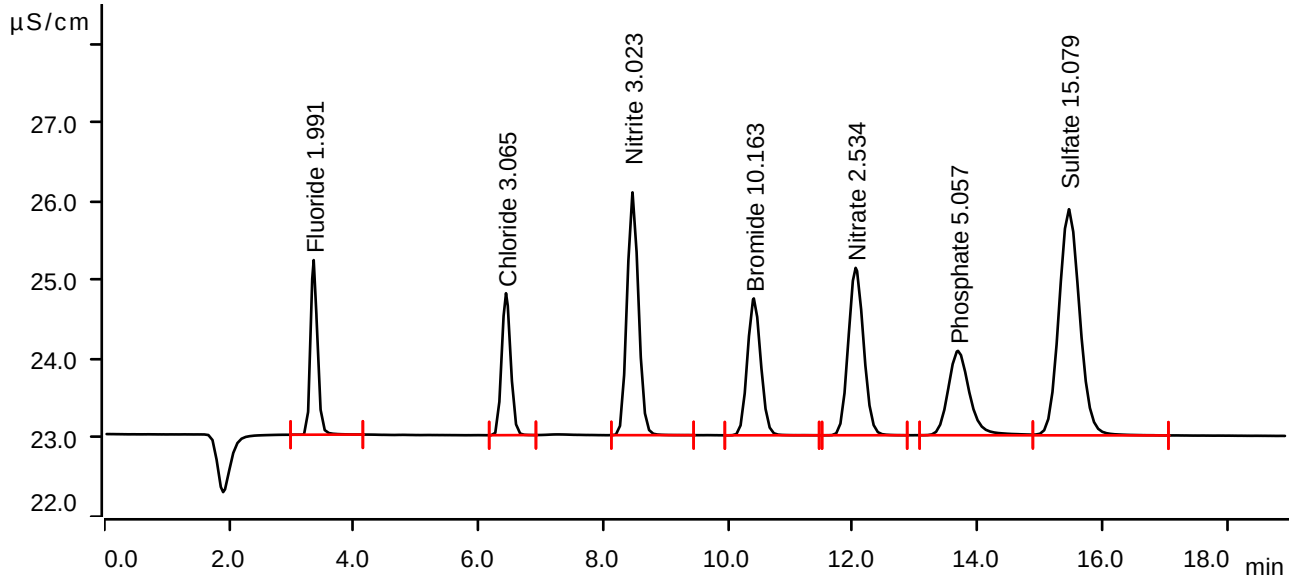

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.2819	2.215	1.991	Fluoride
2	6.440	0.2986	1.801	3.065	Chloride
3	8.468	0.6575	3.081	3.023	Nitrite
4	10.413	0.4329	1.737	10.163	Bromide
5	12.045	0.6057	2.124	2.534	Nitrate
6	13.687	0.4260	1.071	5.057	Phosphate
7	15.465	1.1100	2.870	15.079	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	CCB	
Sample type	Sample	
Determination start	2025-07-25 16:52:00 UTC-4	
Method	IC1-072225	
Operator		

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.66	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

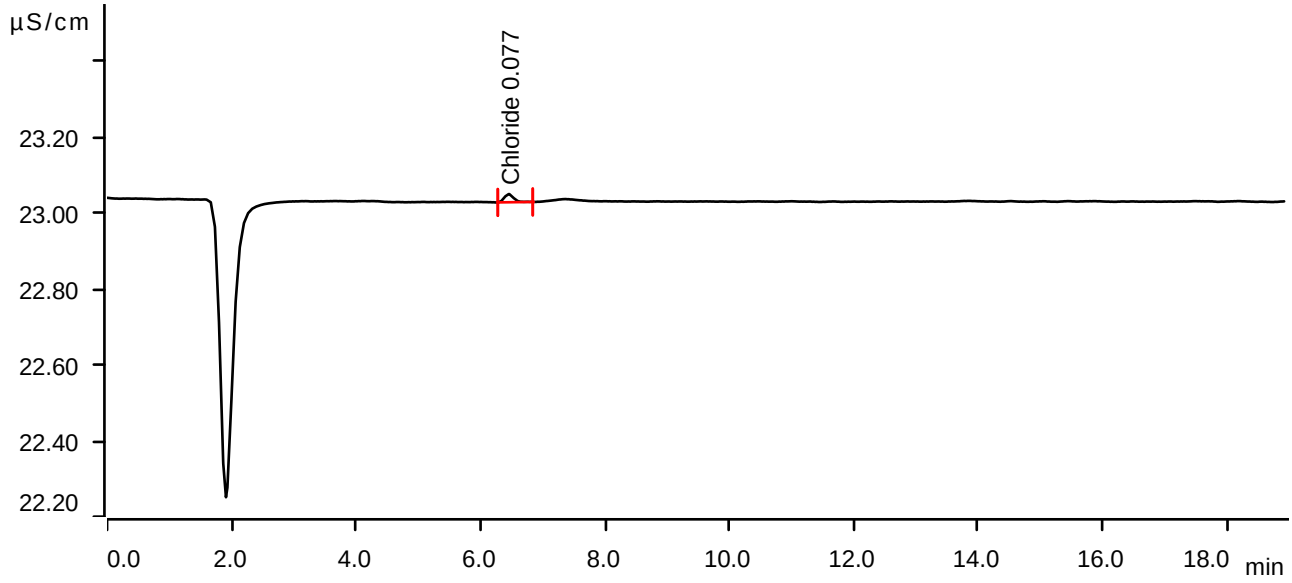

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.457	0.0037	0.022	0.077	Chloride

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2704-01DLX100
Sample type	Sample
Determination start	2025-07-25 17:56:29 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.77	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

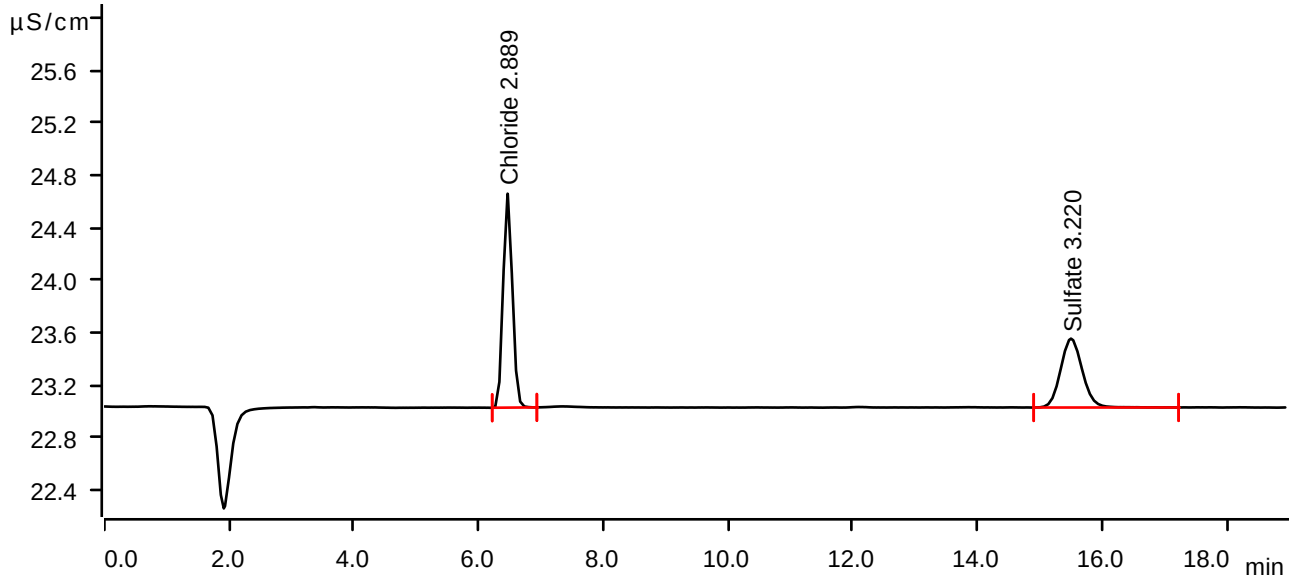

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.465	0.2812	1.629	2.889	Chloride
2	15.498	0.2112	0.524	3.220	Sulfate

Metrohm

Reviewed By:Iwon
On:7/29/2025 1:29 PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2704-02DLX500
Sample type	Sample
Determination start	2025-07-25 18:39:30 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.66	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

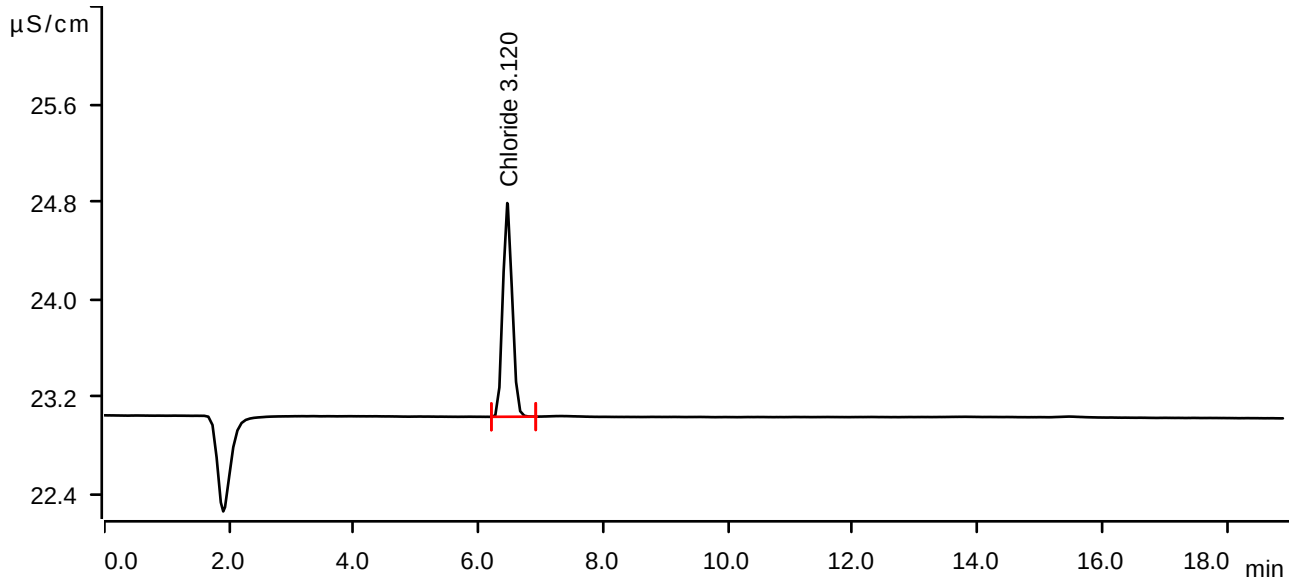

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.460	0.3040	1.752	3.120	Chloride

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	Q2704-03DLX500
Sample type	Sample
Determination start	2025-07-25 19:22:27 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.66	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

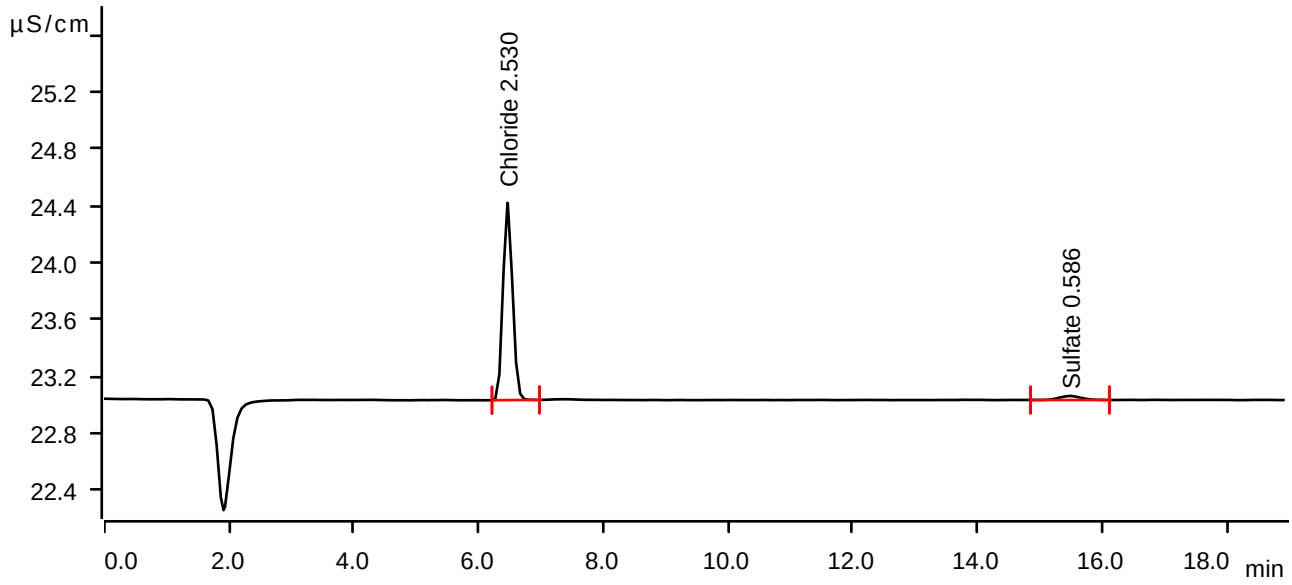

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.463	0.2458	1.387	2.530	Chloride
2	15.480	0.0116	0.028	0.586	Sulfate

Metrohm

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	CCV
Sample type	Check standard 1
Determination start	2025-07-25 20:05:20 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.66	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

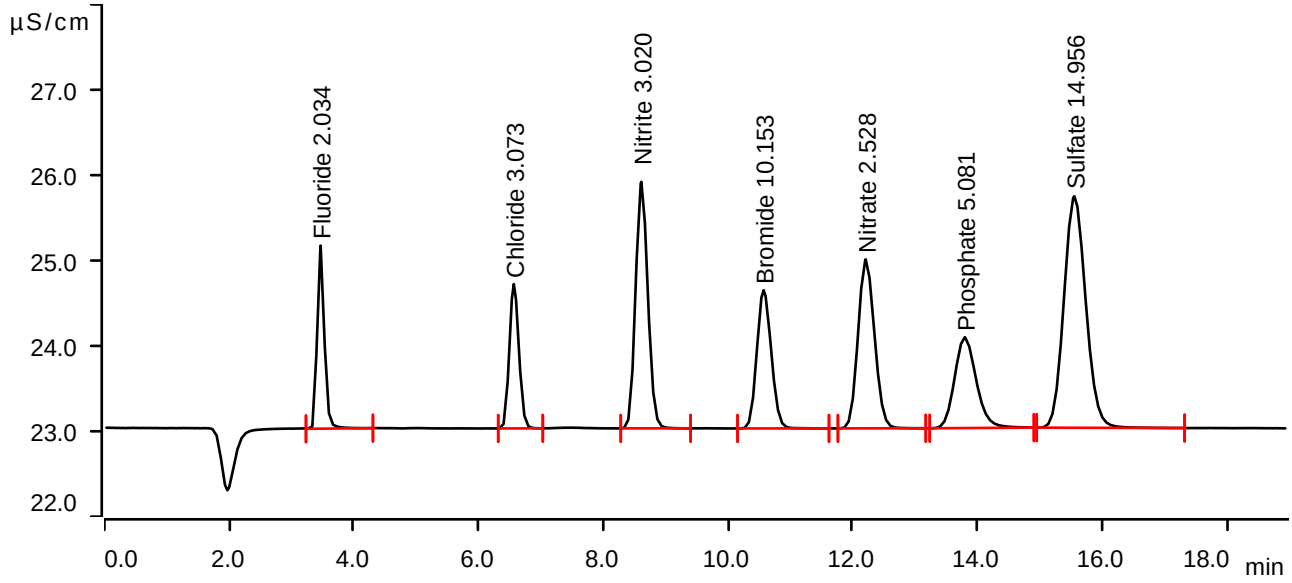

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.465	0.2880	2.144	2.034	Fluoride
2	6.565	0.2994	1.690	3.073	Chloride
3	8.610	0.6569	2.888	3.020	Nitrite
4	10.570	0.4325	1.619	10.153	Bromide
5	12.207	0.6042	1.979	2.528	Nitrate
6	13.795	0.4280	1.064	5.081	Phosphate
7	15.552	1.1007	2.712	14.956	Sulfate

Reviewed By:Iwon
On:7/29/2025 1:29
PM
Inst Id :IC-1
LB :LB136635

Sample data

Ident	CCB
Sample type	Sample
Determination start	2025-07-25 20:26:50 UTC-4
Method	IC1-072225
Operator	

Anions

Data source	Conductivity detector 1 (Eco IC 1)	
Channel	Conductivity	
Recording time	19.0	min
Integration	Automatically	
Column type	Metrosep A Supp 19 - 150/4.0	
Eluent composition	not defined	
Flow	0.700	mL/min
Maximum flow monitored	yes	
Pressure	11.77	MPa
Maximum pressure monitored	yes	
Temperature	-----	°C

Anions

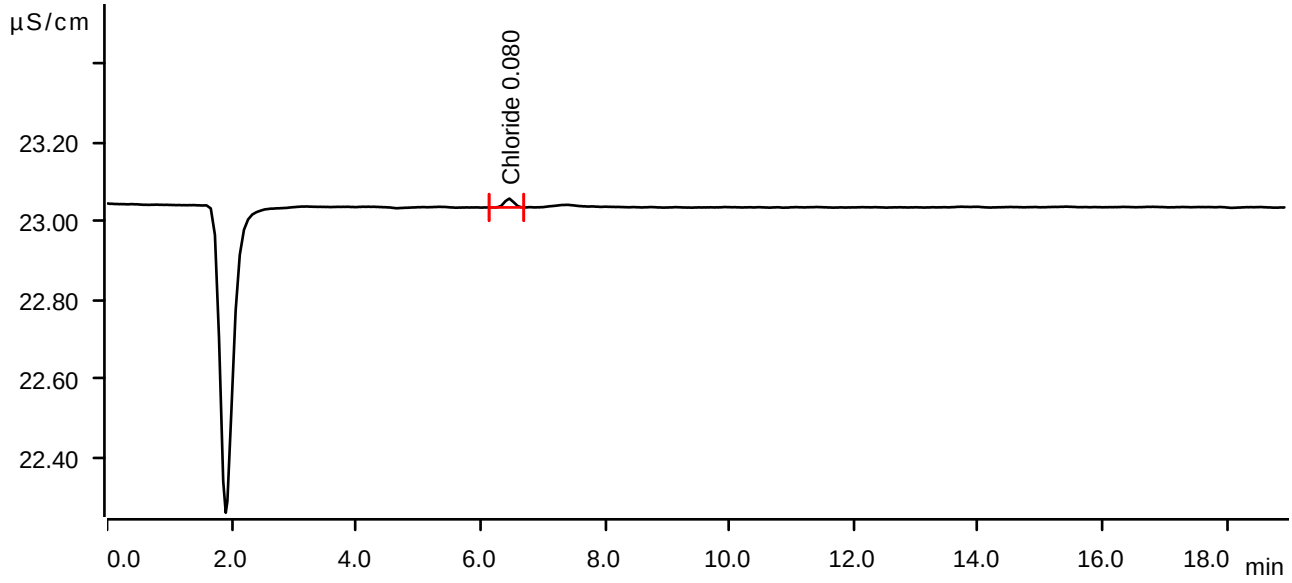

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.463	0.0040	0.022	0.080	Chloride

WORKLIST(Hardcopy Internal Chain)

LB136635

WorkList Name : Anions-072525 **WorkList ID :** 190958 **Department :** Wet-Chemistry **Date :** 07-25-2025 11:08:05

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2695-01	RW5-SP100-20250725	Water	Anions Group4	Cool 4 deg C	TETR06	D31	07/24/2025	300.0
Q2696-01	RW8-SP100-20250724	Water	Anions Group4	Cool 4 deg C	TETR06	D31	07/24/2025	300.0
Q2697-01	RW7-SP100-20250724	Water	Anions Group4	Cool 4 deg C	TETR06	D51	07/24/2025	300.0

Date/Time 07/25/25 12:20
Raw Sample Received by: IC(WC)
Raw Sample Relinquished by: [illegible]

Date/Time 07/25/25 13:35
Raw Sample Received by: [illegible]
Raw Sample Relinquished by: IC(WC)

Reviewed By:Iwona
On:7/29/2025 1:29:58 PM
Inst Id :IC-1
LB :LB136635

WORKLIST(Hardcopy Internal Chain)

LB136635

WorkList Name : Anions-072525-2 **WorkList ID :** 190963 **Department :** Wet-Chemistry **Date :** 07-25-2025 13:56:46

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2704-01	MW3	Water	Anions Group1	Cool 4 deg C	GENV01	D31	07/23/2025	300.0
Q2704-02	MW4	Water	Anions Group1	Cool 4 deg C	GENV01	D31	07/23/2025	300.0
Q2704-03	MW2D	Water	Anions Group1	Cool 4 deg C	GENV01	D31	07/23/2025	300.0

Date/Time 07/25/25 14:30
Raw Sample Received by: [signature]
Raw Sample Relinquished by: [signature]

Date/Time 07/25/25 15:25
Raw Sample Received by: [signature]
Raw Sample Relinquished by: [signature]

Reviewed By:lwona
On:7/29/2025 1:29:58 PM
Inst Id :IC-1
LB :LB136635