

SOP ID:	M3541-ASE Extraction-15		
Clean Up SOP #:	Acid Cleanup	Extraction Start Date :	07/30/2025
Matrix :	Solid	Extraction Start Time :	08:45
Welgh By:	EH	Extraction By:	RJ
Balance check:	RJ	Filter By:	RJ
Balance ID:	EX-SC-2	pH Meter ID:	N/A
pH Strip Lot#:	N/A	Hood ID:	3,7
		Concentration By:	EH
		Supervisor By :	RUPESH
Extraction Method:	☐ Seperatory Funnel ☐ Continous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet		

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	5000 PPB	PP24650
Surrogate	1.0ML	200 PPB	PP24663
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2627
Baked Na2SO4	N/A	EP2629
Hexane	N/A	E3956
H2SO4 1:1	N/A	EP2610
Sand	N/A	E3951
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40ML Vial Lot # 03-40BTS721, No MS/MSD performed as samples are Caulk Matrix.


KD Bath ID:	N/A	Envap ID:	NEVAP-02
KD Bath Temperature:	N/A	Envap Temperature:	40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
7/30/25	RSC (B4 Lab)	Y-P-Rest/143
11:50	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-15

Concentration Date: 07/30/2025

Sample ID	Client Sample ID	Test	g/ mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB169057BL	ABLK057	PCB Group1	30.02	N/A	ritesh	Evelyn	10			U2-1
PB169057BS	ALCS057	PCB Group1	30.01	N/A	ritesh	Evelyn	10			2
Q2711-01	PCB15-33	PCB Group1	3.75	N/A	ritesh	Evelyn	10		Caulk Mat.	3
Q2711-02	PCB15-31	PCB Group1	3.22	N/A	ritesh	Evelyn	10		Caulk Mat.	4
Q2711-03	PCB15-28	PCB Group1	3.89	N/A	ritesh	Evelyn	10		Caulk Mat.	5
Q2711-04	PCB14-3	PCB Group1	2.55	N/A	ritesh	Evelyn	10		Caulk Mat.	6
Q2711-05	PCB14-5	PCB Group1	3.28	N/A	ritesh	Evelyn	10		Caulk Mat.	U3-1

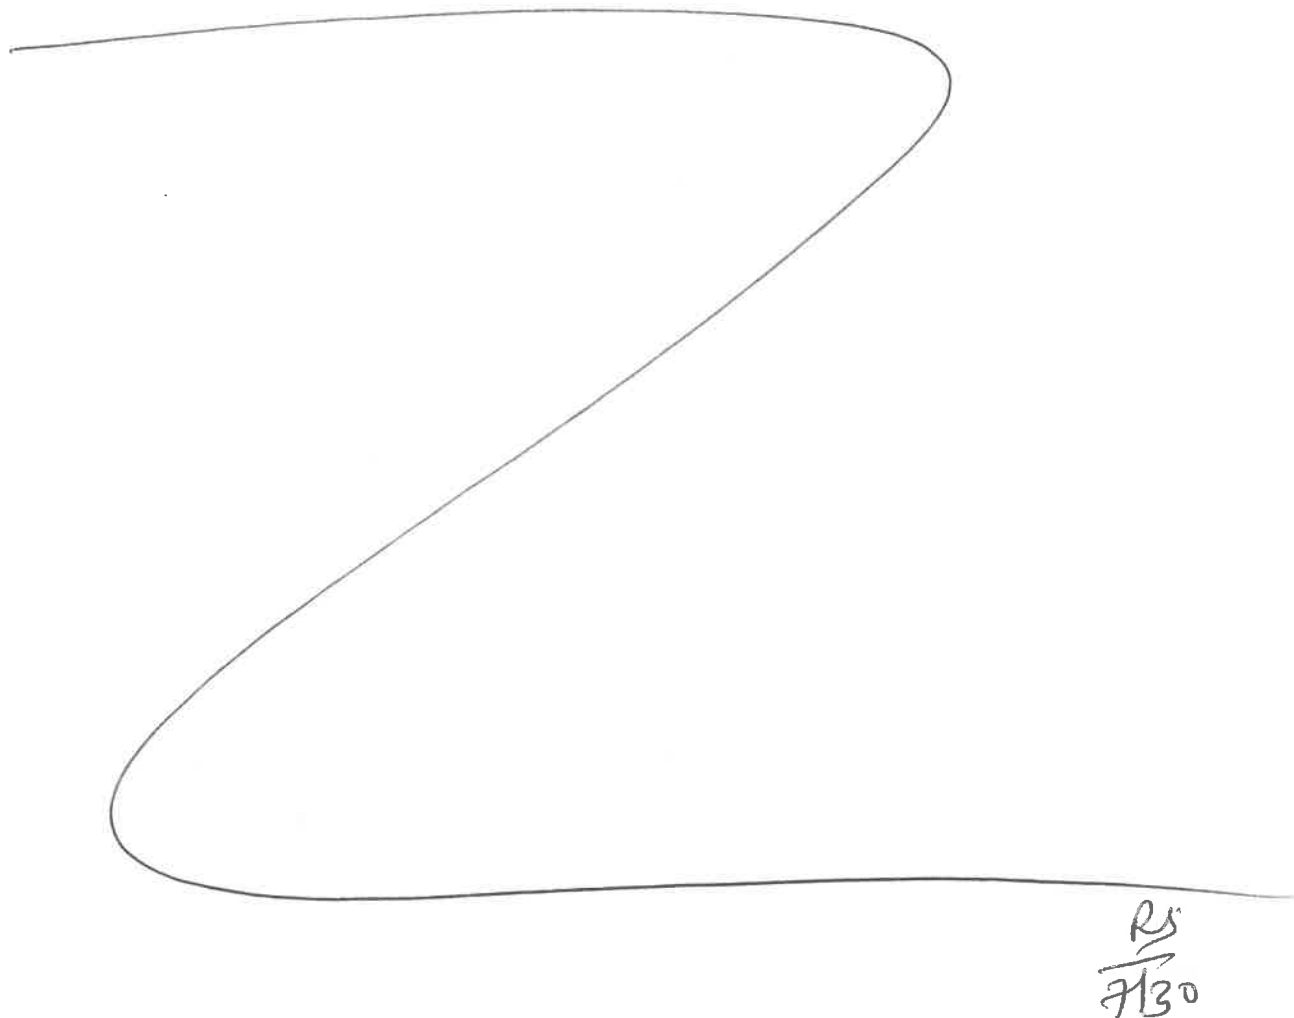

RS
7/30