
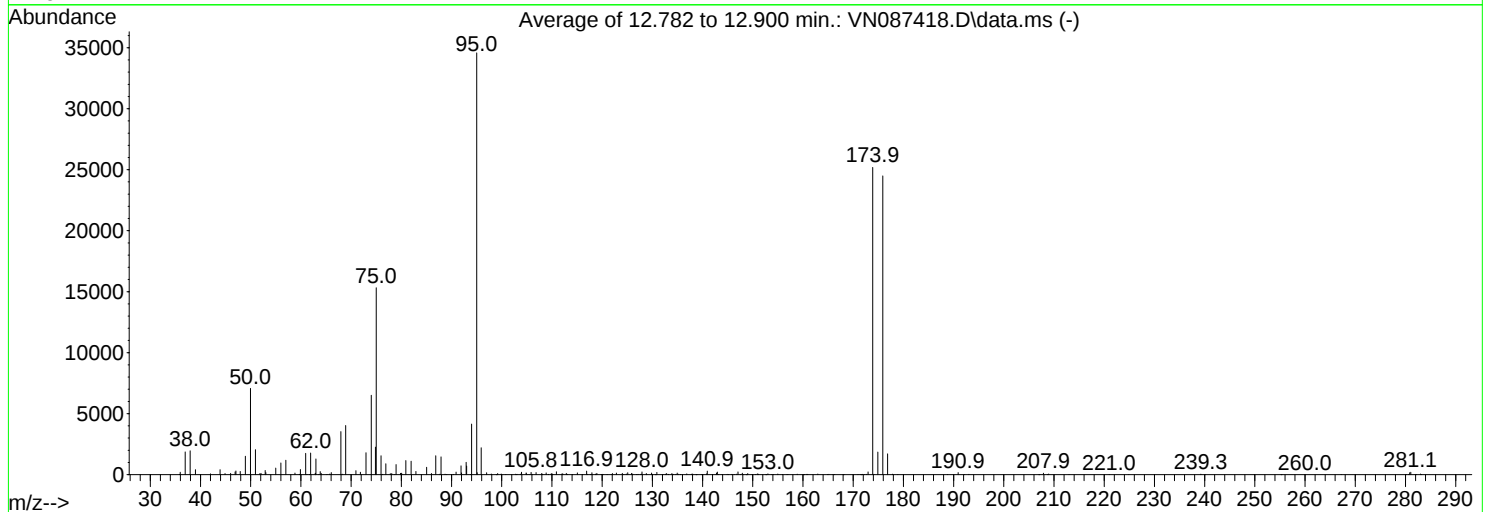


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN072825\
Data File : VN087418.D
Acq On : 28 Jul 2025 08:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072825W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Jul 28 11:35:47 2025

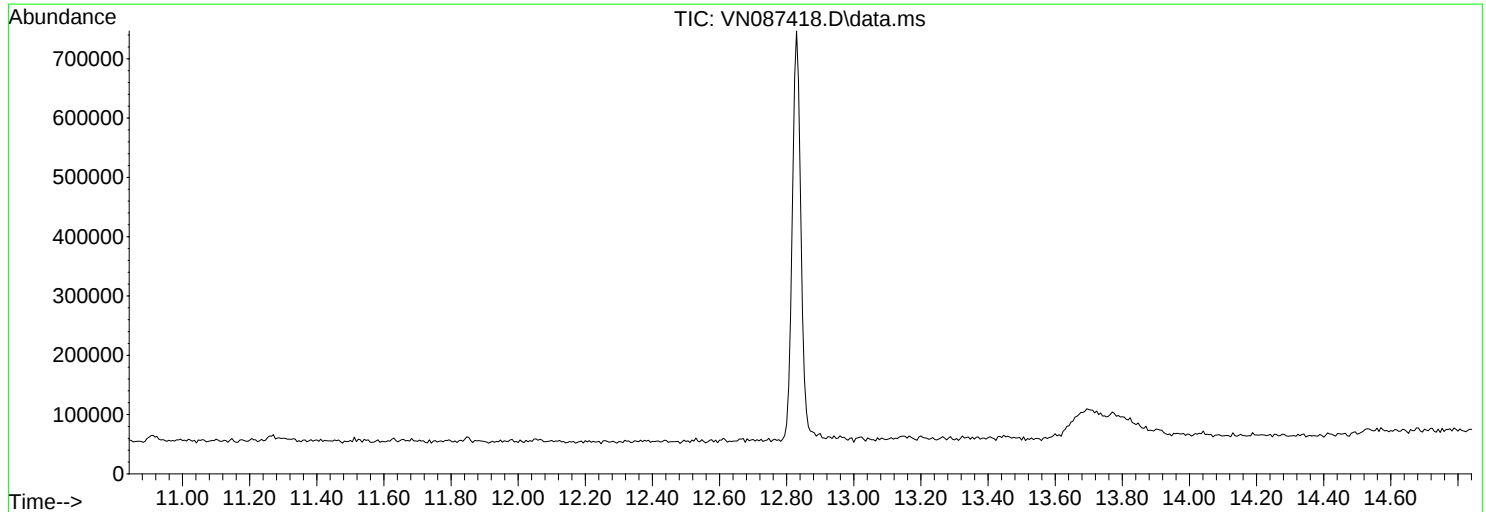

AutoFind: Averaged scan 1841 to 1861; Bkg corrected with scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.4	7071	PASS
75	95	30	60	44.3	15317	PASS
95	95	100	100	100.0	34582	PASS
96	95	5	9	6.4	2201	PASS
173	174	0.00	2	0.9	222	PASS
174	95	50	100	72.8	25188	PASS
175	174	5	9	7.3	1848	PASS
176	174	95	101	97.2	24487	PASS
177	176	5	9	7.0	1704	PASS