
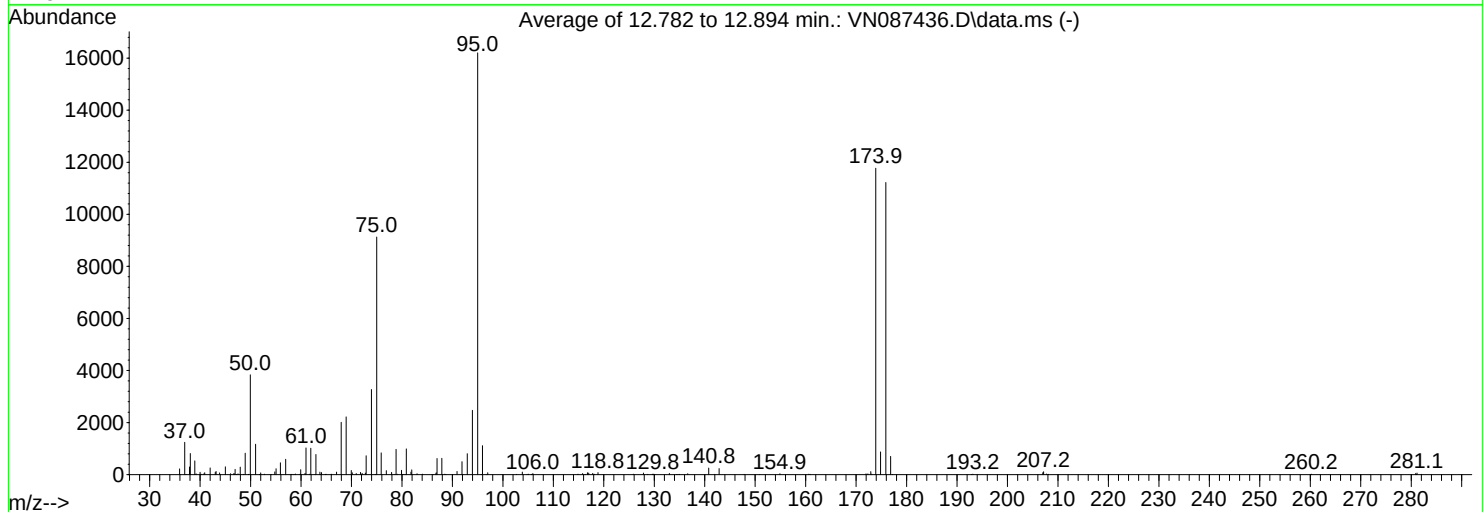


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN073025\
Data File : VN087436.D
Acq On : 30 Jul 2025 08:46
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N072825W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Mon Jul 28 11:35:47 2025

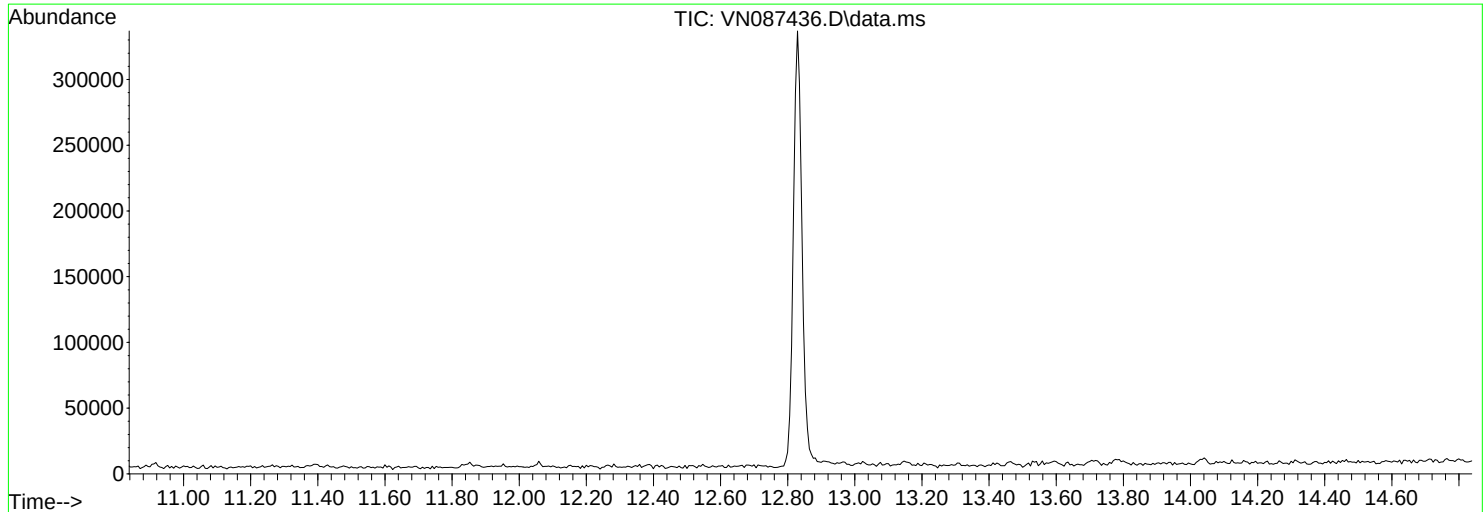

AutoFind: Averaged scan 1841 to 1860; Bkg corrected with scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.7	3835	PASS
75	95	30	60	56.3	9127	PASS
95	95	100	100	100.0	16202	PASS
96	95	5	9	6.9	1110	PASS
173	174	0.00	2	1.0	115	PASS
174	95	50	100	72.6	11769	PASS
175	174	5	9	7.4	871	PASS
176	174	95	101	95.3	11221	PASS
177	176	5	9	6.2	701	PASS