

## Prep Standard - Chemical Standard Summary

**Order ID :** Q2732

**Test :** TCLP Herbicide

**Prepbatch ID :** PB169278,

**Sequence ID/Qc Batch ID:** PS081525,PS081825,

**Standard ID :**

EP2605,EP2606,EP2633,PP24553,PP24556,PP24557,PP24558,PP24559,PP24560,PP24654,PP24737,PP24802,PP24803,PP24804,

**Chemical ID :**

E3554,E3657,E3875,E3933,E3940,E3952,E3956,E3962,M6041,M6157,P 11183,P12620,P12630,P12689,P12711,P13543,P13544,P13545,P13546,P13971,P13977,P14064,P14065,P14066,P8829,W3112,

## Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3883	12N H2SO4 solution	<a href="#">EP2605</a>	04/21/2025	10/21/2025	RUPESHKUMAR SHAH	None	None	Riteshkumar Patel
04/21/2025								

**FROM** 333.00000ml of M6041 + 667.00000ml of W3112 = Final Quantity: 1000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3884	6 N NAOH	<a href="#">EP2606</a>	04/21/2025	10/21/2025	RUPESHKUMAR SHAH	Extraction_SC ALE_2 (EX-SC-2)	None	Riteshkumar Patel
04/21/2025								

**FROM** 1000.00000ml of W3112 + 240.00000gram of E3657 = Final Quantity: 1000.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
601	Acidified Sodium Sulphate 2	<a href="#">EP2633</a>	08/15/2025	11/07/2025	RUPESHKUMAR SHAH	Extraction_SCALE_2 (EX-SC-2)	None	Riteshkumar Patel  08/18/2025
<u>FROM</u>	1000.00000ml of E3952 + 150.00000ml of M6157 + 3000.00000ml of E3875 = Final Quantity: 3000.000 gram							

[illegible]

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1456	200 PPB Herb MIX STD	<a href="#">PP24556</a>	05/12/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025

**FROM** 0.90000ml of E3933 + 0.10000ml of PP24553 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1455	500 PPB Herb MIX STD	<a href="#">PP24557</a>	05/12/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025

**FROM** 0.75000ml of E3933 + 0.25000ml of PP24553 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1453	1000 PPB Herb MIX STD	<a href="#">PP24558</a>	05/12/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025

**FROM** 0.50000ml of E3933 + 0.50000ml of PP24553 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1454	750 PPB Herb MIX STD	<a href="#">PP24559</a>	05/12/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025

**FROM** 0.25000ml of E3933 + 0.75000ml of PP24558 = Final Quantity: 1.000 ml

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1452	1500 PPB HERB MIX STD	<a href="#">PP24560</a>	05/12/2025	11/05/2025	Abdul Mirza	None	None	Yogesh Patel
								05/22/2025

**FROM** 0.25000ml of E3933 + 0.75000ml of PP24553 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1848	5000/500000 PPB Herbicide Spike (Free Acid)	<a href="#">PP24654</a>	06/18/2025	12/11/2025	Abdul Mirza	None	None	Yogesh Patel
								07/23/2025

**FROM** 1.25000ml of P13543 + 1.25000ml of P13544 + 1.25000ml of P13545 + 1.25000ml of P13546 + 95.00000ml of E3940 = Final Quantity: 100.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
60	5000 PPB Herbicide Surg Spike (Free Acid)	<a href="#">PP24737</a>	07/18/2025	01/18/2026	Abdul Mirza	None	None	Yogesh Patel 07/21/2025
<b><u>FROM</u></b> 1.25000ml of P13977 + 1.25000ml of P14064 + 1.25000ml of P14065 + 1.25000ml of P14066 + 195.00000ml of E3956 = Final Quantity: 200.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1851	2/200 PPM Herb Mega Mix 2nd Source	<a href="#">PP24802</a>	08/07/2025	08/31/2025	Abdul Mirza	None	None	Yogesh Patel 08/19/2025
<b><u>FROM</u></b> 0.50000ml of P13971 + 1.00000ml of P12711 + 48.50000ml of E3962 = Final Quantity: 50.000 ml								

## Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1854	1000 PPB HERB MIX ICV STD	<a href="#">PP24803</a>	08/07/2025	08/31/2025	Abdul Mirza	None	None	Yogesh Patel
								08/19/2025

**FROM** 0.50000ml of E3962 + 0.50000ml of PP24802 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1691	750 PPB ICV HERB STD	<a href="#">PP24804</a>	08/07/2025	08/31/2025	Abdul Mirza	None	None	Yogesh Patel
								08/19/2025

**FROM** 0.25000ml of E3962 + 0.75000ml of PP24803 = Final Quantity: 1.000 ml



## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9335-02 / Iso-Octane (2,2,4-Trimethylpentane) Ultra Resi-Analyzed Grade	63160	11/05/2025	08/09/2023 / Rajesh	08/09/2023 / Rajesh	E3554

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19510-5 / Sodium Hydroxide Pellets 2.5 Kg, Pk of 4	23B1556310	12/31/2025	12/04/2023 / Rajesh	12/01/2023 / Rajesh	E3657

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	417203	01/28/2026	07/28/2025 / RUPESH	01/29/2025 / Rajesh	E3875

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	11/05/2025	05/05/2025 / RUPESH	04/23/2025 / RUPESH	E3933

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	12/11/2025	06/11/2025 / Rajesh	06/04/2025 / Rajesh	E3940

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9244-03 / Ether, Anhydrous, Purified (cs/4x4L)	250419	05/31/2026	07/09/2025 / RUPESH	07/09/2025 / RUPESH	E3952

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/16/2025 / RUPESH	07/16/2025 / RUPESH	E3956

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	08/05/2025 / RUPESH	07/30/2025 / RUPESH	E3962

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	23D2462010	03/20/2028	08/16/2024 / mohan	08/16/2024 / mohan	M6041

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L)	24i1262013	11/07/2025	05/07/2025 / RUPESH	02/18/2025 / Mohan	M6157

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0172864	11/12/2025	05/12/2025 / Abdul	11/01/2021 / Abdul	P11183

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32062 / Herbicide Mix, 500/8000, Standard #4 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A0155055	11/12/2025	05/12/2025 / Abdul	07/03/2023 / Abdul	P12620

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32055 / Herbicide Mix, 500/8000, Standard #1 [methyl ester] 200ug/mL, hexane, 1mL/ampul	A192429	11/12/2025	05/12/2025 / Abdul	07/03/2023 / Abdul	P12630

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32059 / Herbicide Mix#3 (Methyl Ester), 20000 ug/ml	A0199844	11/12/2025	05/12/2025 / Abdul	07/24/2023 / Abdul	P12689

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	08/31/2025	08/07/2025 / Abdul	08/09/2023 / Abdul	P12711

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151M / Chlorinated Herbicide Mixtures, Methyl Esters	0006752480	08/31/2025	08/07/2025 / Abdul	08/09/2023 / Abdul	P12711

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13543

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13543

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13544

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13544

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13545

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13545

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13546

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Agilent Technologies	HBM-8151A / Chlorinated Herbicide Mixtures, Free Acids	0006810955	12/18/2025	06/18/2025 / Abdul	09/24/2024 / Abdul	P13546

## CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0221255	11/12/2025	05/12/2025 / Abdul	04/02/2025 / Abdul	P13971

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0221255	01/18/2026	07/18/2025 / Abdul	04/02/2025 / Abdul	P13977

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0221255	01/18/2026	07/18/2025 / Abdul	06/23/2025 / anahy	P14064

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0221255	01/18/2026	07/18/2025 / Abdul	06/23/2025 / anahy	P14065

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32050 / Herbicide, 8000 series, 515 Surrogate [ester] 2,4-dichlorophenyl acetic acid methyl ester, 1mL, 200ug/mL, Hexane	A0221255	01/18/2026	07/18/2025 / Abdul	06/23/2025 / anahy	P14066

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32254 / Dalapon Methyl Ester, 1000 ug/ml	A0148063	11/12/2025	05/12/2025 / Abdul	08/16/2019 / Stephen	P8829

### **CHEMICAL RECEIPT LOG BOOK**

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / lwona	07/03/2024 / lwona	W3112

# Certificate of Analysis



Date of Release: 6/9/2023  
Name: 2,2,4-Trimethylpentane [Isooctane]  
OmniSolv®  
Item No: TX1389 all size codes  
Lot / Batch No: 63160  
Country of Origin: Germany

Characteristic	Requirement		Results	Units
	Min.	Max.		
Assay (GC)	99.5		> 99.99	%
Capillary ECD responsive substances (as PCNB)		5	0.24	ng/L
Color (APHA)		10	< 10	
Evaporation residue		1	< 0.5	ppm
Filtered through 0.2 µm filter			Passes test	
Fluorescence (as quinine base)		250	71	ppt
Form			Clear liquid	
Infrared Spectrum			Conforms	
Refractive index (at 20°C)			1.3915	
UV Abs. at 200 nm		1.00	0.137	AU
UV Abs. at 220 nm		0.05	0.024	AU
UV Abs. at 230 nm		0.02	0.003	AU
UV Abs. at 250 nm		0.005	0.003	AU
UV Abs. at 270 nm		0.005	0.002	AU
UV Abs. at 300 nm		0.005	0.004	AU
UV Cut-off		200	191.1	nm
Water (H <sub>2</sub> O)		0.01	0.001	%

Michael Hutchinson,

Quality Control Manager

This document has been produced electronically and is valid without a signature.

EMD Millipore is a division of Merck KGaA, Darmstadt, Germany  
EMD Millipore Corporation  
400 Summit Drive,  
Burlington, MA 01803  
U.S.A.

Recd by RP on 8/9/23

E3554



# Certificate of Analysis

## Sodium Hydroxide (Pellets)

**Material:** 0583  
**Grade:** ACS GRADE  
**Batch Number:** 23B1556310

**Chemical Formula:** NaOH  
**Molecular Weight:** 40  
**CAS #:** 1310-73-2  
**Appearance:**

**Manufacture Date:** 12/14/2022  
**Expiration Date:** 12/31/2025

**Storage:** Room Temperature

Pellets

TEST	SPECIFICATION	ANALYSIS	DISPOSITION
Calcium	$\leq 0.005 \%$	$< 0.005 \%$	PASS
Chloride	$\leq 0.005 \%$	0.002 %	PASS
Heavy Metals	$\leq 0.002 \%$	$< 0.002 \%$	PASS
Iron	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Magnesium	$\leq 0.002 \%$	$< 0.002 \%$	PASS
Mercury	$\leq 0.1 \text{ ppm}$	$< 0.1 \text{ ppm}$	PASS
Nickel	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Nitrogen Compounds	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Phosphate	$\leq 0.001 \%$	$< 0.001 \%$	PASS
Potassium	$\leq 0.02 \%$	$< 0.02 \%$	PASS
Purity	$\geq 97.0 \%$	99.2 %	PASS
Sodium Carbonate	$\leq 1.0 \%$	0.5 %	PASS
Sulfate	$\leq 0.003 \%$	$< 0.003 \%$	PASS

Internal ID #: 710

### Signature

We certify that this batch conforms to the specifications listed.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon  
VWR Chemicals, LLC.  
28600 Fountain Parkway, Solon OH 44139 USA

### Additional Information

Analysis may have been rounded to significant digits in specification limits.

Product meets analytical specifications of the grades listed.







**PRODUCTOS  
QUÍMICOS  
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR  
MONTERREY, N.L. MÉXICO  
CP 64070  
TEL +52 81 13 52 67 67  
www.pqm.com.mx

# CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na <sub>2</sub> SO <sub>4</sub>
SPECIFICATION NUMBER:	6399	RELEASE DATE:	MAY/23/2024
LOT NUMBER :	417203		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na <sub>2</sub> SO <sub>4</sub> )	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.2
Insoluble matter	Max. 0.01%	0.001 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO <sub>4</sub> )	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.001 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.001 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	96.2 %
Through US Standard No. 60 sieve	Max. 5%	3.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

## COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors**<sup>TM</sup>



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	5
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3933



Jamie Croak  
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Acetone

BAKER RESI-ANALYZED® Reagent

For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
Assay ((CH <sub>3</sub> ) <sub>2</sub> CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H <sub>2</sub> O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Rec'd by RP on 6/11/25

E3940

*J. Croak*

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

## CERTIFICATE OF ANALYSIS

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System Standard ISO9001:2015 by Intertek Global Certificate Number. CERT-0120633

Catalogue Number	E198
Lot Number	250419
Description	ETHYL ETHER, HPLC GRADE
CAS Number	60-29-7
Quality Test/Release Date	02/Jun/2025
Suggested retest date	31/May/2026
Country of Origin	Mexico
Declaration of Origin	Organic - synthetic
BSE/TSE	This product was derived from synthetic raw materials and the manufacturing process excluded contamination with any animal products.

Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid free of suspended matter
ASSAY	%	>= 99	99.95
CARBONYL COMPOUNDS	%	<= 0.001	<0.001
COLOR	APHA	<= 10	5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.708 - 0.710	0.710
EVAPORATION RESIDUE	ppm	<= 5	0.1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 218 NM	ABSORBANCE UNITS	<= 1.00	0.15
OPTICAL ABS AT 254 NM	ABSORBANCE UNITS	<= 0.07	0.03
OPTICAL ABS AT 280 NM	ABSORBANCE UNITS	<= 0.02	0.003
OPTICAL ABS AT 350 NM	ABSORBANCE UNITS	<= 0.01	<0.001
PEROXIDE	ppm	<= 5	<1
PRESERVATIVE - ETHANOL	%	Inclusive Between 1.5 - 2.5	1.6
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.3490 - 1.3520	1.3498
SUBSTANCES DARKENED BY H2SO4	PASS/FAIL	= PASS TEST	PASS TEST
TITRATABLE ACID	MEQ/G	<= 0.0002	<0.00003
WATER (H2O)	%	<= 0.01	0.008



Matthew Micek  
QC Supervisor

Received on 7/9/25

E3952

Products are processed under ISO 9001:2015 quality management systems and samples are tested for conformance to the noted specifications. Certain data may have been supplied by third parties. We disclaim the implied warranties of merchantability and fitness for a particular purpose, and the accuracy of third-party data or information associated with the product. Products are for research use or further manufacturing. Products are not for direct administration to humans or animals. It is the responsibility of the final formulator or end user to determine suitability, and to qualify and/or validate each product for its intended use.

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis

 **avantors**<sup>™</sup>



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	5
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

*Received on 7/16/25*

**E3956**



Jamie Croak  
Director Quality Operations, Bioscience Production

n-Hexane 95%  
ULTRA RESI-ANALYZED  
For Organic Residue Analysis



Material No.: 9262-03  
Batch No.: 25C0362005  
Manufactured Date: 2025-01-29  
Expiration Date: 2026-04-30  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	$\leq 5$	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	$\leq 10$	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	$\leq 5$	5
Assay (Total Saturated C <sub>6</sub> Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	$\leq 10$	10
Residue after Evaporation	$\leq 1.0$ ppm	0.1 ppm
Substances Darkened by H <sub>2</sub> SO <sub>4</sub>	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use  
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States  
Packaging Site: Phillipsburg Mfg Ctr & DC

*Received on 7/30/25*

E3962

Jamie Croak  
Director Quality Operations, Bioscience Production

Sulfuric Acid  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis  
Low Selenium

avantor™



M 6041-4b  
MS

Material No.: 9673-33  
Batch No.: 23D2462010  
Manufactured Date: 2023-03-22  
Retest Date: 2028-03-20  
Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
ACS – Assay (H <sub>2</sub> SO <sub>4</sub> )	95.0 – 98.0 %	96.1 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Substances Reducing Permanganate (as SO <sub>2</sub> )	≤ 2 ppm	< 2 ppm
Ammonium (NH <sub>4</sub> )	≤ 1 ppm	1 ppm
Chloride (Cl)	≤ 0.1 ppm	< 0.1 ppm
Nitrate (NO <sub>3</sub> )	≤ 0.2 ppm	< 0.1 ppm
Phosphate (PO <sub>4</sub> )	≤ 0.5 ppm	< 0.1 ppm
Trace Impurities – Aluminum (Al)	≤ 30.0 ppb	< 5.0 ppb
Arsenic and Antimony (as As)	≤ 4.0 ppb	< 2.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	8.5 ppb
Trace Impurities – Cadmium (Cd)	≤ 2.0 ppb	< 0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 6.0 ppb	< 0.4 ppb
Trace Impurities – Cobalt (Co)	≤ 0.5 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gold (Au)	≤ 10.0 ppb	0.5 ppb
Heavy Metals (as Pb)	≤ 500.0 ppb	< 100.0 ppb
Trace Impurities – Iron (Fe)	≤ 50.0 ppb	1.3 ppb
Trace Impurities – Lead (Pb)	≤ 0.5 ppb	< 0.5 ppb
Trace Impurities – Magnesium (Mg)	≤ 7.0 ppb	0.8 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	< 0.1 ppb
Trace Impurities – Nickel (Ni)	≤ 2.0 ppb	0.3 ppb
Trace Impurities – Potassium (K)	≤ 500.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se)	≤ 50.0 ppb	< 0.1 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	31.5 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	< 0.3 ppb

>>> Continued on page 2 >>>

Sulfuric Acid  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis  
Low Selenium



Material No.: 9673-33  
Batch No.: 23D2462010

Test	Specification	Result
Trace Impurities - Sodium (Na)	$\leq 500.0$ ppb	5.4 ppb
Trace Impurities - Strontium (Sr)	$\leq 5.0$ ppb	< 0.2 ppb
Trace Impurities - Tin (Sn)	$\leq 5.0$ ppb	< 0.8 ppb
Trace Impurities - Zinc (Zn)	$\leq 5.0$ ppb	0.4 ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: USA  
Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in cursive script that reads 'Jamie Ethier'.  
Jamie Ethier  
Vice President Global Quality



Sulfuric Acid  
BAKER INSTRA-ANALYZED® Reagent  
For Trace Metal Analysis  
Low Selenium

avantor™



M6157  
MS

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

## Certificate of Analysis

Test	Specification	Result
ACS – Assay (H <sub>2</sub> SO <sub>4</sub> )	95.0 – 98.0 %	96.2 %
Appearance	Passes Test	Passes Test
ACS – Color (APHA)	<= 10	5
ACS – Residue after Ignition	<= 3 ppm	<1 ppm
ACS – Substances Reducing Permanganate(as SO <sub>2</sub> )	<= 2 ppm	<2 ppm
Ammonium (NH <sub>4</sub> )	<= 1 ppm	<1 ppm
Chloride (Cl)	<= 0.1 ppm	<0.1 ppm
Nitrate (NO <sub>3</sub> )	<= 0.2 ppm	0.1 ppm
Phosphate (PO <sub>4</sub> )	<= 0.5 ppm	<0.1 ppm
Trace Impurities – Aluminum (Al)	<= 30.0 ppb	<5.0 ppb
Arsenic & Antimony (as As)	<= 4.0 ppb	<2.0 ppb
Trace Impurities – Boron (B)	<= 10.0 ppb	<5.0 ppb
Trace Impurities – Cadmium (Cd)	<= 2.0 ppb	<1.0 ppb
Trace Impurities – Chromium (Cr)	<= 6.0 ppb	<1.0 ppb
Trace Impurities – Cobalt (Co)	<= 0.5 ppb	<0.3 ppb
Trace Impurities – Copper (Cu)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Gold (Au)	<= 10.0 ppb	<5.0 ppb
Heavy Metals (as Pb)	<= 500.0 ppb	<100.0 ppb
Trace Impurities – Iron (Fe)	<= 50.0 ppb	<1.0 ppb
Trace Impurities – Lead (Pb)	<= 0.5 ppb	<0.5 ppb
Trace Impurities – Magnesium (Mg)	<= 7.0 ppb	<1.0 ppb
Trace Impurities – Manganese (Mn)	<= 1.0 ppb	<1.0 ppb
Trace Impurities – Mercury (Hg)	<= 0.5 ppb	<0.1 ppb
Trace Impurities – Nickel (Ni)	<= 2.0 ppb	<0.3 ppb
Trace Impurities – Potassium (K)	<= 500.0 ppb	<10.0 ppb
Trace Impurities – Selenium (Se)	<= 50.0 ppb	7.2 ppb
Trace Impurities – Silicon (Si)	<= 100.0 ppb	12.8 ppb
Trace Impurities – Silver (Ag)	<= 1.0 ppb	<1.0 ppb

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Sulfuric Acid

BAKER INSTRA-ANALYZED® Reagent

For Trace Metal Analysis

Low Selenium

 **avantors**™



Material No.: 9673-33

Batch No.: 2411262013

Test	Specification	Result
Trace Impurities – Sodium (Na)	$\leq 500.0$ ppb	$< 5.0$ ppb
Trace Impurities – Strontium (Sr)	$\leq 5.0$ ppb	$< 1.0$ ppb
Trace Impurities – Tin (Sn)	$\leq 5.0$ ppb	1.1 ppb
Trace Impurities – Zinc (Zn)	$\leq 5.0$ ppb	$< 1.0$ ppb

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC



Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

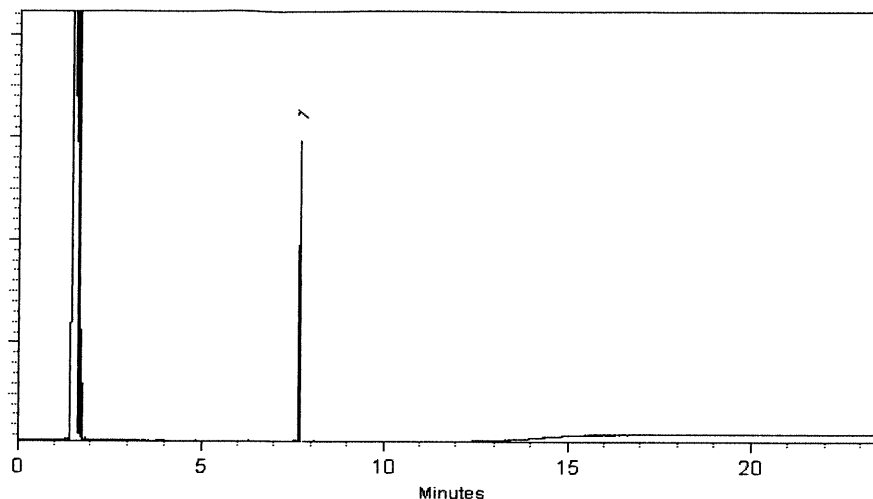

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Katelyn McGinnis - Operations Tech I

Date Mixed: 28-May-2021

Balance: B345965662

  
Marlene Cowan - Operations Tech I

Date Passed: 02-Jun-2021

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

1911177  
70  
P 111 86  
AR  
11/02/21



CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# Certificate of Analysis



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0172864

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** February 29, 2028 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

## CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	202.0 µg/mL	+/- 1.4323 µg/mL Gravimetric
	CAS # 55954-23-9 (Lot CSC42194-01)		+/- 6.8182 µg/mL Unstressed
	Purity 99%		+/- 6.8182 µg/mL Stressed

**Solvent:** Hexane  
CAS # 110-54-3  
Purity 99%

P11177  
↓  
P11186  
—  
AR  
01/02/21



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

# CERTIFIED REFERENCE MATERIAL

## Certificate of Analysis



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32062 **Lot No.:** A0155055

**Description :** Herbicide Mix #4/ME (Methyl Ester)

Herbicide Mix #4/ME (Methyl Ester) 200µg/mL,  
Hexane/Methyl-tert-butyl-ether, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** November 30, 2026 **Storage:** 10°C or colder

P12616 / (5)  
↓  
P12620  
✓ *Paul* = 7/5/2023

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	3,5-Dichlorobenzoic acid methyl ester CAS # 2905-67-1 (Lot 3903900) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 6.7507 µg/mL Unstressed +/- 6.7507 µg/mL Stressed
2	4-Nitroanisole CAS # 100-17-4 (Lot 24765/7) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 6.7507 µg/mL Unstressed +/- 6.7507 µg/mL Stressed
3	Pentachloroanisole CAS # 1825-21-4 (Lot 7921100) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 6.7507 µg/mL Unstressed +/- 6.7507 µg/mL Stressed
4	Chloramben methyl ester CAS # 7286-84-2 (Lot 6487100) Purity 98%	199.9 µg/mL	+/- 1.4176 µg/mL Gravimetric +/- 6.7480 µg/mL Unstressed +/- 6.7480 µg/mL Stressed
5	Bentazon methyl ester CAS # 61592-45-8 (Lot 817100) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 6.7507 µg/mL Unstressed +/- 6.7507 µg/mL Stressed
6	Picloram methyl ester CAS # 14143-55-6 (Lot 386-21B) Purity 98%	201.9 µg/mL	+/- 1.4315 µg/mL Gravimetric +/- 6.8141 µg/mL Unstressed +/- 6.8141 µg/mL Stressed
7	DCPA methyl ester (Chlorthal-dimethyl) CAS # 1861-32-1 (Lot 8008700) Purity 99%	200.0 µg/mL	+/- 1.4182 µg/mL Gravimetric +/- 6.7507 µg/mL Unstressed +/- 6.7507 µg/mL Stressed

8	Acifluorfen methyl ester	200.0 µg/mL	+/- 1.4182	µg/mL	Gravimetric
	CAS # 50594-67-7 (Lot 6282300)		+/- 6.7507	µg/mL	Unstressed
	Purity 99%		+/- 6.7507	µg/mL	Stressed

**Solvent:** Hexane/Methyl-tert-butyl-ether  
**CAS #** 110-54-3/1634-04-4  
**Purity** 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

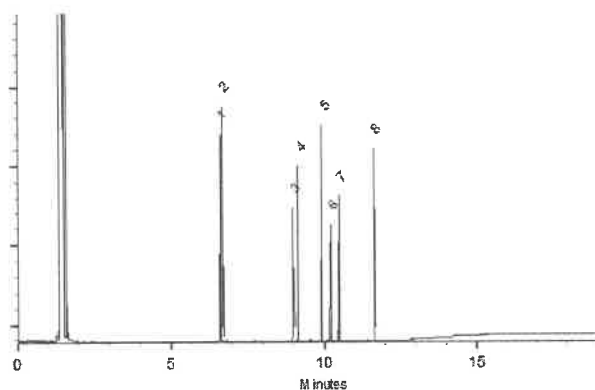

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Michael Maje*

**Date Mixed:** 14-Nov-2019 **Balance:** 1128353505

*Justine Albertson*  
Justine Albertson - Operations Tech-ARM QC

**Date Passed:** 18-Nov-2019

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis chromatographic plus



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32055 **Lot No.:** A0192429

**Description :** Herbicide Mix #1/ME (Methyl Ester)  
Herbicide Mix #1/ME (Methyl Ester) 200 µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** December 31, 2029 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

P12626 / 5  
P12630  
7/5/2023

#### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Dicamba methyl ester	6597-78-0	11705400	99%	201.6 µg/mL	+/- 3.4204
2	Dichlorprop methyl ester	57153-17-0	11672100	99%	201.4 µg/mL	+/- 3.4170
3	2,4-D methyl ester	1928-38-7	10048000	99%	201.2 µg/mL	+/- 3.4136
4	2,4,5-TP (silvex) methyl ester	4841-20-7	6364900	99%	201.2 µg/mL	+/- 3.4136
5	2,4,5-T methyl ester	1928-37-6	6875800	98%	200.7 µg/mL	+/- 3.4052
6	Dinoseb methyl ether	6099-79-2	12914300	99%	200.8 µg/mL	+/- 3.4068
7	2,4-DB methyl ester	18625-12-2	12542000	99%	201.0 µg/mL	+/- 3.4102

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

40°C (hold 2 min.) to 330°C  
@ 10°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

2 ml/min.

**Inj. Vol**

1µl

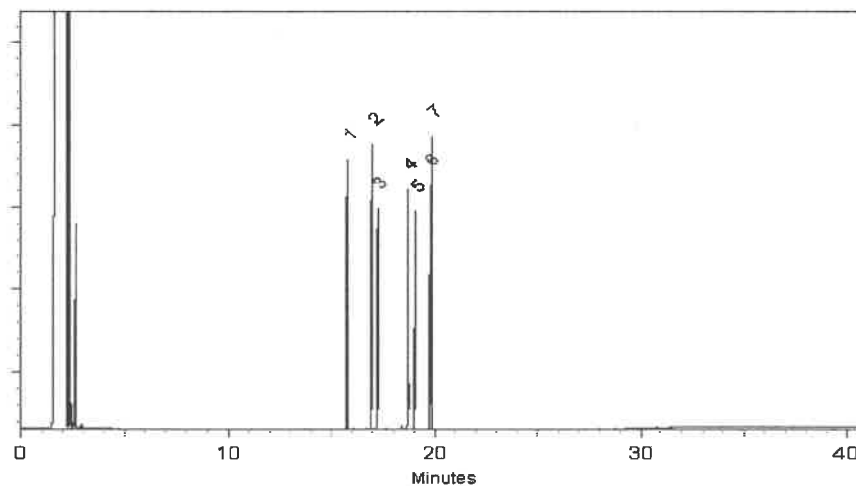

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

*Penelope Riglin*  
Penelope Riglin - Operations Tech I

Date Mixed: 09-Dec-2022

Balance Serial # 1128360905

*Jennifer Pollino*  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 12-Dec-2022

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

### Certificate of Analysis chromatographic plus



#### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32059 **Lot No.:** A0199844  
**Description :** Herbicide Mix #3/ME (Methyl Ester)  
Herbicide Mix #3/ME (Methyl Ester) 20,000 µg/mL, Hexane, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** July 31, 2030 **Storage:** 10°C or colder  
**Handling:** This product is photosensitive. **Ship:** Ambient

P 12685 / (S)  
↓  
P 12689  
↓  
RAU= 7/24/23

#### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	MCPP (Mecoprop) methyl ester	23844-56-6	14546400	99%	20,035.0 µg/mL	+/- 360.1907
2	MCPA methyl ester	2436-73-9	SL201209	99%	20,055.0 µg/mL	+/- 360.5503

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

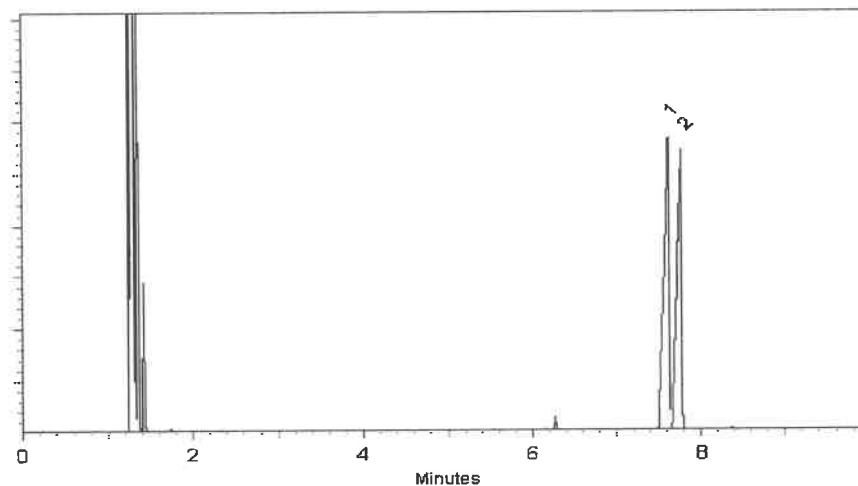

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Morgan Craighead - Mix Technician

Date Mixed: 12-Jul-2023

Balance Serial # B442140311

  
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 19-Jul-2023

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397

P12706  
↓  
P12715  
/ (10)  
/ 1  
/ 8/15/23

**ISO 17034**

**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Methylated Herbicides Standard

**Lot Number:** 0006752480

**Product Number:** HBM-8151M-1

**Lot Issue Date:** 18-Jul-2023

**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Expiration Date:** 31-Aug-2025

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen methyl ester	100.3 ±	0.5 µg/mL	050594-67-7	RM03058
bentazon methyl derivative	100.2 ±	0.5 µg/mL	061592-45-8	RM13829
chloramben methyl ester	100.4 ±	0.5 µg/mL	007286-84-2	RM03055
2,4-D methyl ester	100.2 ±	0.5 µg/mL	001928-38-7	RM03040
dalapon methyl ester	100.4 ±	0.5 µg/mL	017640-02-7	RM14219
2,4-DB methyl ester	100.2 ±	0.5 µg/mL	018625-12-2	RM03029
DCPA	100.2 ±	0.5 µg/mL	001861-32-1	RM13426
dicamba methyl ester	100.4 ±	0.5 µg/mL	006597-78-0	RM03039
methyl-3,5-dichlorobenzoate	100.1 ±	0.5 µg/mL	002905-67-1	RM03048
dichlorprop methyl ester	100.4 ±	0.5 µg/mL	057153-17-0	NT02086
dinoseb methyl ether	100.5 ±	0.5 µg/mL	006099-79-2	RM03051
MCPA methyl ester	10031 ±	50 µg/mL	002436-73-9	RM12863
MCPP methyl ester	10031 ±	50 µg/mL	023844-56-6	RM20060
4-nitroanisole	100.3 ±	0.5 µg/mL	000100-17-4	RM02806
pentachloroanisole	100.4 ±	0.5 µg/mL	001825-21-4	RM02457
picloram methyl ester	100.2 ±	0.5 µg/mL	014143-55-6	RM03044
silvex methyl ester	100.2 ±	0.5 µg/mL	004841-20-7	RM03799
2,4,5-T methyl ester	100.4 ±	0.5 µg/mL	001928-37-6	RM03033

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

**Instructions for Use:**

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

**Safety:**

Refer to the Safety Data Sheet on [www.agilent.com](http://www.agilent.com) for information regarding this analytical reference material.

**Intended Use:**

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

**Expiration of Certification:**

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

  
Monica Bourgeois  
QMS Representative

P12706 / (10)  
↓  
P12715  
✓ RAUF  
8.15.23



ISO 17034  
Cert No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

[www.agilent.com/quality/](http://www.agilent.com/quality/)  
CSD-QA-015.2

ISO 17025  
Cert No. AT-1937

**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Herbicides Standard  
**Product Number:** HBM-8151A-1  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Lot Number:** 0006810955  
**Lot Issue Date:** 20-Aug-2024  
**Expiration Date:** 30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

P13541  
↓  
P13561  
20  
9/25/2024



**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Herbicides Standard  
**Product Number:** HBM-8151A-1  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Lot Number:** 0006810955  
**Lot Issue Date:** 20-Aug-2024  
**Expiration Date:** 30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

P13541  
↓  
P13561  
20  
9/25/2024





**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Herbicides Standard  
**Product Number:** HBM-8151A-1  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Lot Number:** 0006810955  
**Lot Issue Date:** 20-Aug-2024  
**Expiration Date:** 30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

P13541  
↓  
P13561  
20  
9/25/2024



**Reference Material Certificate**  
**Product Information Sheet**

**Product Name:** Chlorinated Herbicides Standard  
**Product Number:** HBM-8151A-1  
**Storage Conditions:** Store at Room Temperature (15° to 30°C).

**Lot Number:** 0006810955  
**Lot Issue Date:** 20-Aug-2024  
**Expiration Date:** 30-Sep-2026

Component Name	Concentration	Uncertainty	CAS#	Analyte Lot
acifluorfen	100.2 ±	0.5 µg/mL	050594-66-6	NT02057
bentazon	100.4 ±	0.5 µg/mL	025057-89-0	RM21359
chloramben	100.3 ±	0.5 µg/mL	000133-90-4	RM02698
2,4-D	100.4 ±	0.5 µg/mL	000094-75-7	RM17172
dalapon	100.4 ±	0.5 µg/mL	000075-99-0	RM19677
2,4-DB	100.1 ±	0.5 µg/mL	000094-82-6	RM02866
tetrachloroterephthalic acid	100.4 ±	0.5 µg/mL	002136-79-0	RM15140
dicamba	100.3 ±	0.5 µg/mL	001918-00-9	RM22113
3,5-dichlorobenzoic acid	100.4 ±	0.5 µg/mL	000051-36-5	RM02768
dichlorprop	100.2 ±	0.5 µg/mL	000120-36-5	RM21688
dinoseb	100.3 ±	0.5 µg/mL	000088-85-7	RM22275
MCPA	10019 ±	50 µg/mL	000094-74-6	RM12220
MCPP (mecoprop)	10011 ±	50 µg/mL	000093-65-2	RM09273
4-nitrophenol	100.4 ±	0.5 µg/mL	000100-02-7	RM02391
pentachlorophenol	100.2 ±	0.5 µg/mL	000087-86-5	RM02474
picloram	100.4 ±	0.5 µg/mL	001918-02-1	RM20442
silvex	100.5 ±	0.5 µg/mL	000093-72-1	RM22116
2,4,5-T	100.3 ±	0.5 µg/mL	000093-76-5	RM19314

**Matrix:** methanol (methyl alcohol)

**Description:**

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

**Traceability:**

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

**Homogeneity:**

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

P13541  
↓  
P13561  
20  
9/25/2024





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0221255

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2031 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

## CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	55954-23-9	13054200	99%	202.0 µg/mL	+/- 3.4272

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

13968  
↓  
13977

10

AWF  
4/16/2025

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

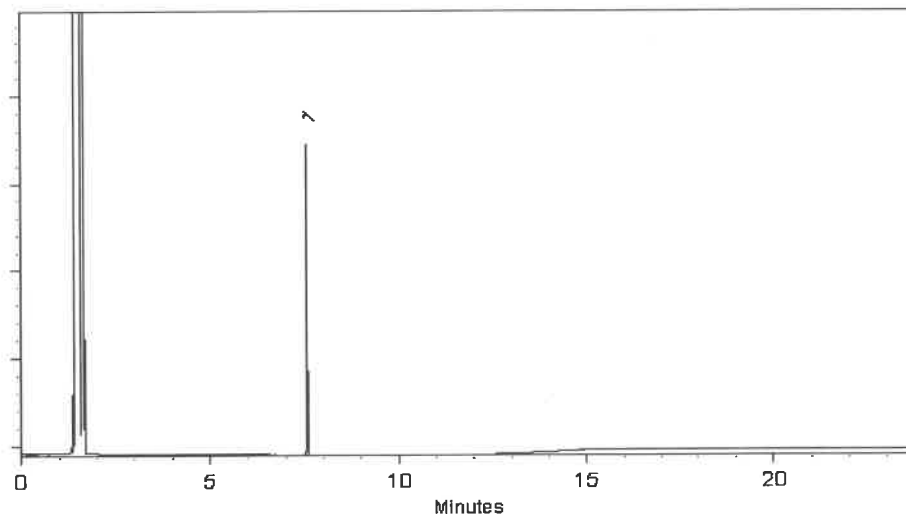

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Ethan Winiarski - Operations Tech I

Date Mixed: 20-Jan-2025

Balance Serial # B345965662

  
Brittany Federinko - Operations Tech I

Date Passed: 22-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



## FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0221255

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2031 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

## CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	55954-23-9	13054200	99%	202.0 µg/mL	+/- 3.4272

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%

13968  
↓  
13977

10

AWF  
4/16/2025

## Quality Confirmation Test

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**

250°C

**Det. Temp:**

330°C

**Det. Type:**


FID

**Split Vent:**

10 ml/min.

**Inj. Vol**

1µl

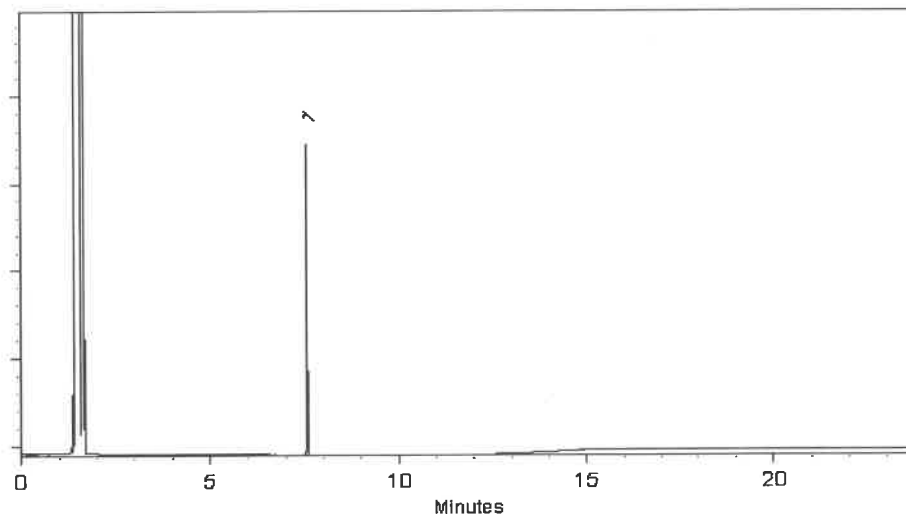

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

  
Ethan Winiarski - Operations Tech I

Date Mixed: 20-Jan-2025

Balance Serial # B345965662

  
Brittany Federinko - Operations Tech I

Date Passed: 22-Jan-2025

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397





110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0221255

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2031 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

P14064  
↓  
P14073 } AC  
6/23/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	55954-23-9	13054200	99%	202.0 µg/mL	+/- 3.4272

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0221255

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2031 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

P14064  
↓  
P14073 } AC  
6/23/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	55954-23-9	13054200	99%	202.0 µg/mL	+/- 3.4272

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%



110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: 1-814-353-1300  
Fax: 1-814-353-1309

www.restek.com

## CERTIFIED REFERENCE MATERIAL

# Certificate of Analysis

chromatographic plus



### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32050 **Lot No.:** A0221255

**Description :** 2,4-Dichlorophenylacetic Acid Methyl Ester Standard

515 Surrogate (ester) 2, 4-dichlorophenyl Acetic Acid Methyl Ester  
200µg/mL, Hexane, 1mL/ampul

**Container Size :** 2 mL **Pkg Amt:** > 1 mL

**Expiration Date :** October 31, 2031 **Storage:** 10°C or colder

**Handling:** This product is photosensitive. **Ship:** Ambient

P14064  
↓  
P14073 } AC  
6/23/25

### CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4-Dichlorophenyl acetic acid methyl ester	55954-23-9	13054200	99%	202.0 µg/mL	+/- 3.4272

\* Expanded Uncertainty displayed in same units as Grav. Conc.

**Solvent:** Hexane  
**CAS #** 110-54-3  
**Purity** 99%



CERTIFIED REFERENCE MATERIAL

110 Benner Circle  
Bellefonte, PA 16823-8812  
Tel: (800)356-1688  
Fax: (814)353-1309

www.restek.com

## Certificate of Analysis



ISO 17034 Accredited  
Reference Material Producer  
Certificate #3222.01



ISO/IEC 17025 Accredited  
Testing Laboratory  
Certificate #3222.02

### FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

*This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.*

**Catalog No. :** 32254 **Lot No.:** A0148063  
**Description :** Dalapon methyl ester Standard  
Dalapon methyl ester 1000µg/mL, Methanol, 1mL/ampul  
**Container Size :** 2 mL **Pkg Amt:** > 1 mL  
**Expiration Date :** April 30, 2026 **Storage:** 10°C or colder  
**Handling:** This product is photosensitive.

Received by  
SG on 8/16/19  
P8828  
P8826

### CERTIFIED VALUES

Elution Order	Compound	Grav. Conc. (weight/volume)	Expanded Uncertainty (95% C.L.; K=2)
1	Dalapon methyl ester CAS # 17640-02-7 Purity 98% (Lot 1764600)	999.6 µg/mL	+/- 10.0697 µg/mL Gravimetric +/- 34.4896 µg/mL Unstressed +/- 34.4896 µg/mL Stressed

**Solvent:** Methanol  
CAS # 67-56-1  
Purity 99%

**Column:**

30m x 0.25mm x 0.25µm  
Rtx-5 (cat.#10223)

**Carrier Gas:**

hydrogen-constant pressure 10 psi.

**Temp. Program:**

75°C (hold 1 min.) to 330°C  
@ 20°C/min. (hold 10 min.)

**Inj. Temp:**


250°C

**Det. Temp:**

330°C

**Det. Type:**

FID

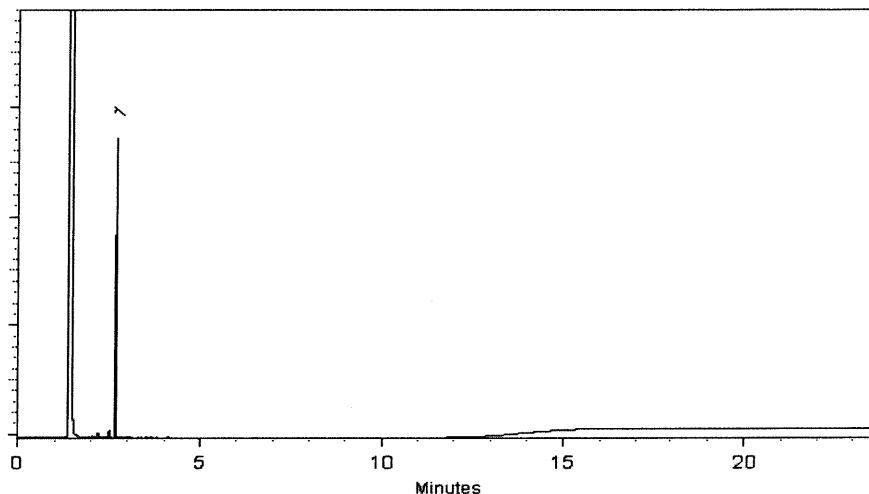

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Bookhamer - Operations Technician I

Date Mixed: 11-Apr-2019

Balance: 1127510105

  
Feng-Yin Lo - QC Analyst

Date Passed: 15-Apr-2019

Manufactured under Restek's ISO 9001:2015  
Registered Quality System  
Certificate #FM 80397