


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080125\
Data File : BF143273.D
Acq On : 01 Aug 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

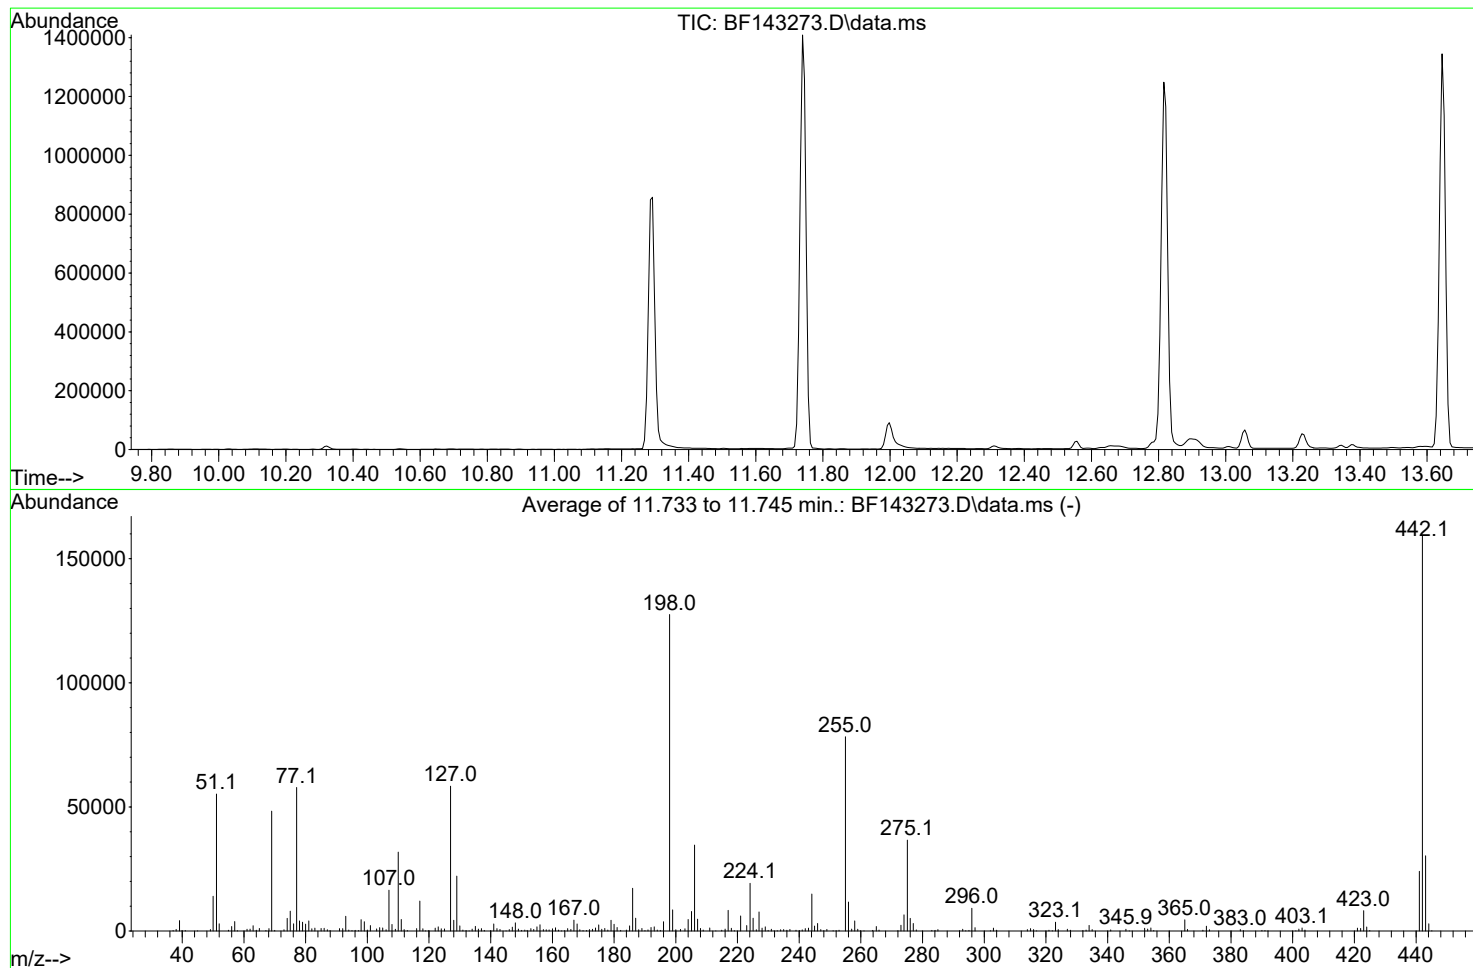

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	959	PASS
69	69	100	100	100.0	48280	PASS
70	69	0.00	2	0.6	289	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	127555	PASS
199	198	5	9	6.7	8538	PASS
365	198	1	100	3.6	4535	PASS
441	443	0.01	150	79.2	24026	PASS
442	442	100	100	100.0	159096	PASS
443	442	15	24	19.1	30336	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/1/2025	BNA_F	<u>BF143273.D</u>
Compound Name	Response	Retention Time
DDT	329297	13.645
DDD	6311	13.345
DDE	2628	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8939	338236	2.64

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080125\
Data File : BF143273.D
Acq On : 01 Aug 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 01 11:46:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

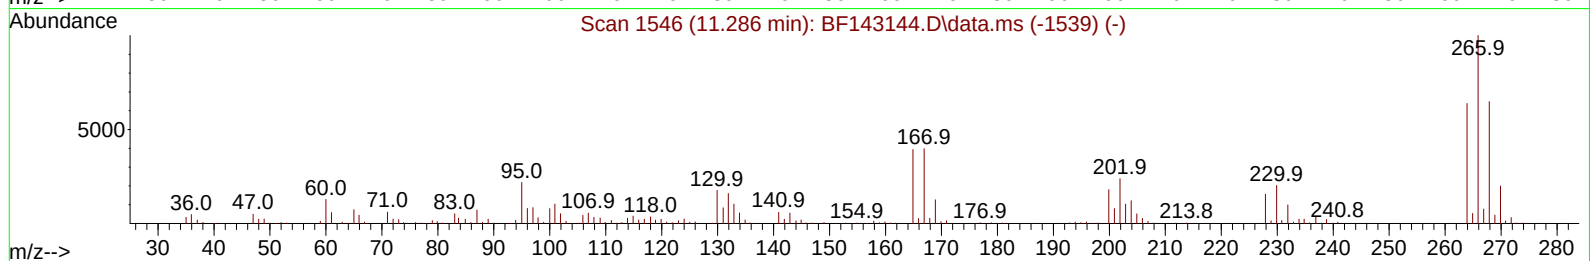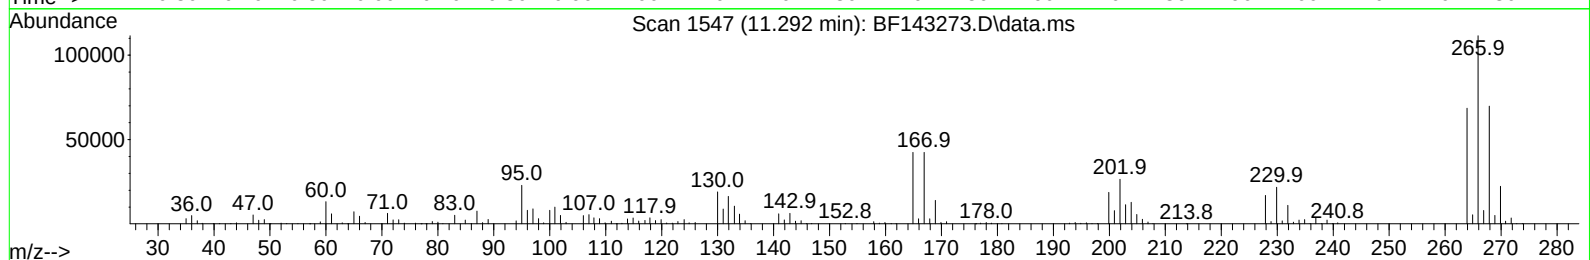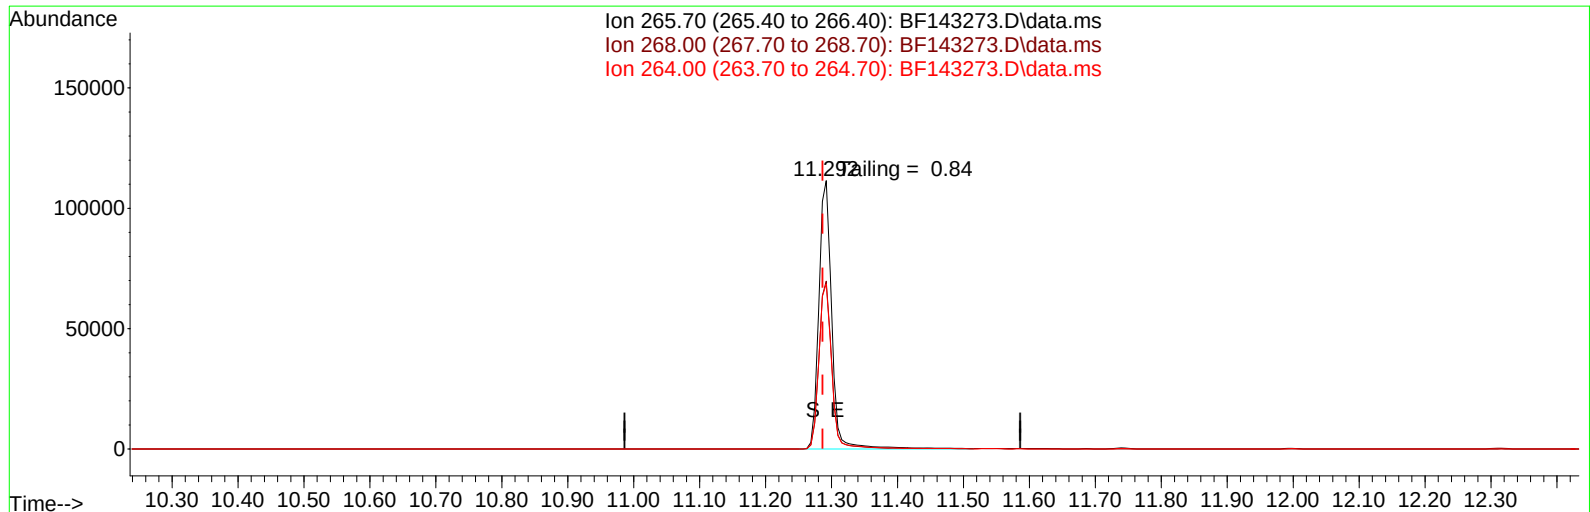

TIC: BF143273.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.006) 167924.22 ng




response 151300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.57
264.00	63.80	61.53
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080125\
Data File : BF143273.D
Acq On : 01 Aug 2025 10:11
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 01 11:46:27 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

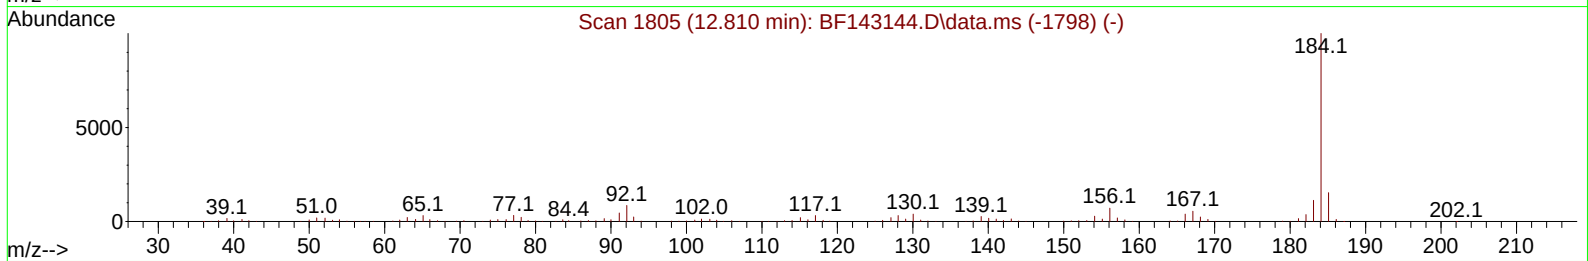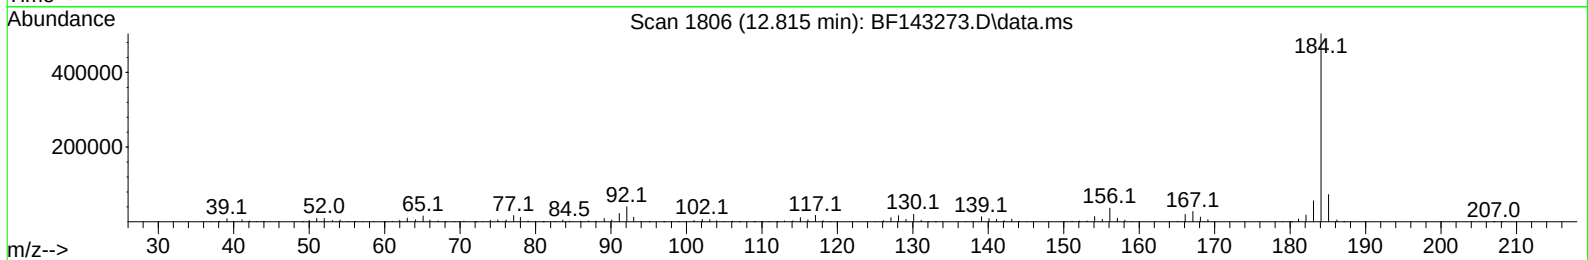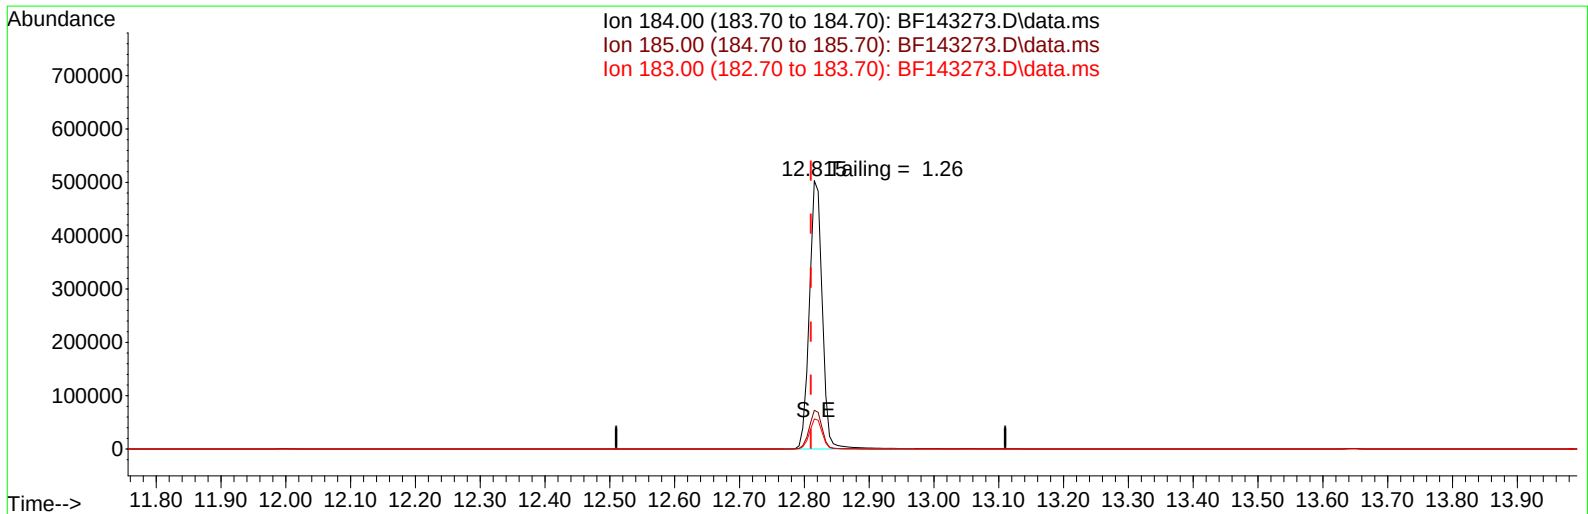

TIC: BF143273.D\data.ms

(77) Benzidine

12.815min (+ 0.005) 3314.55 ng

response 699417

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.47
183.00	11.20	11.20
0.00	0.00	0.00