
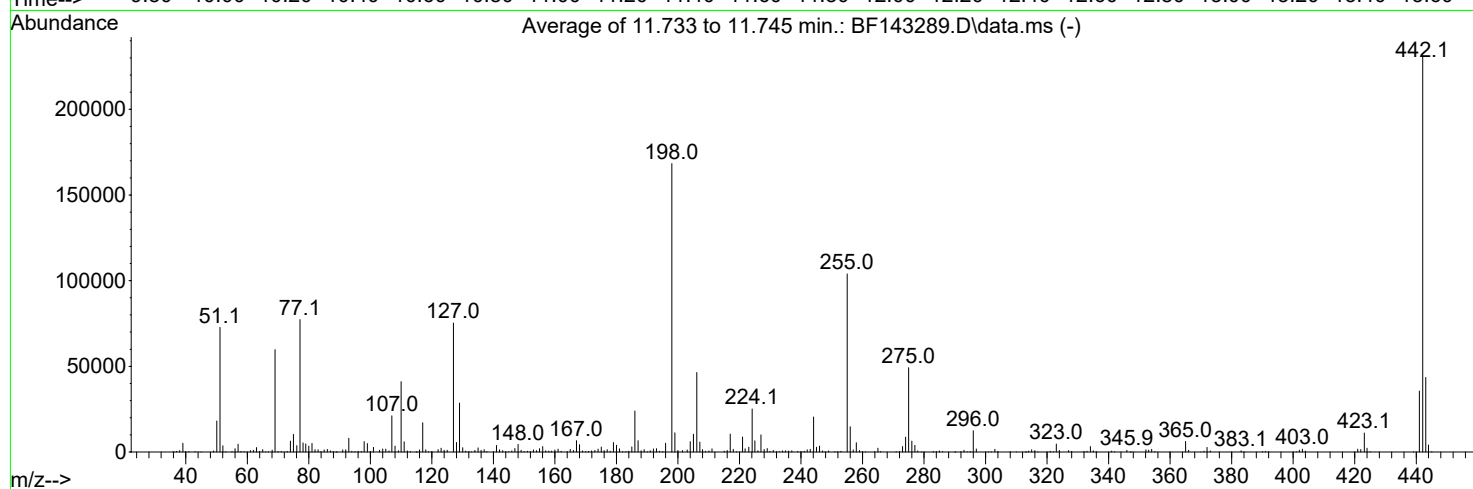


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080425\
Data File : BF143289.D
Acq On : 04 Aug 2025 11:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

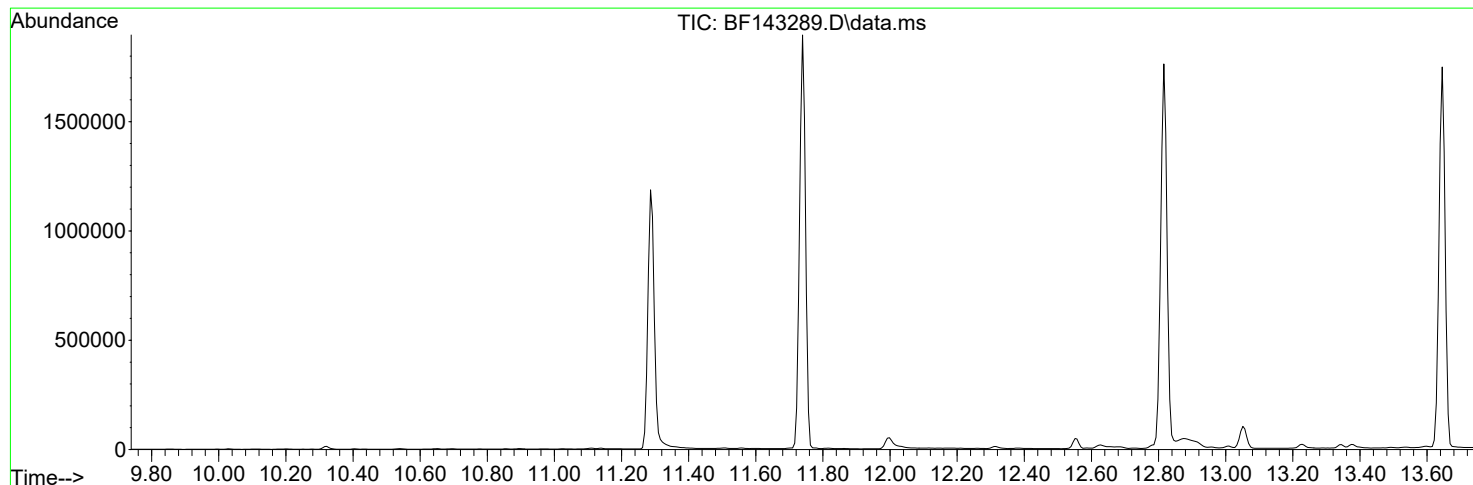

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	1130	PASS
69	69	100	100	100.0	59750	PASS
70	69	0.00	2	0.6	372	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	168363	PASS
199	198	5	9	6.7	11252	PASS
365	198	1	100	3.7	6150	PASS
441	443	0.01	150	81.8	35592	PASS
442	442	100	100	100.0	230443	PASS
443	442	15	24	18.9	43515	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/4/2025	BNA_F	<u>BF143289.D</u>
Compound Name	Response	Retention Time
DDT	434376	13.645
DDD	8792	13.345
DDE	3435	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12227	446603	2.74

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080425\
Data File : BF143289.D
Acq On : 04 Aug 2025 11:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 04 12:42:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

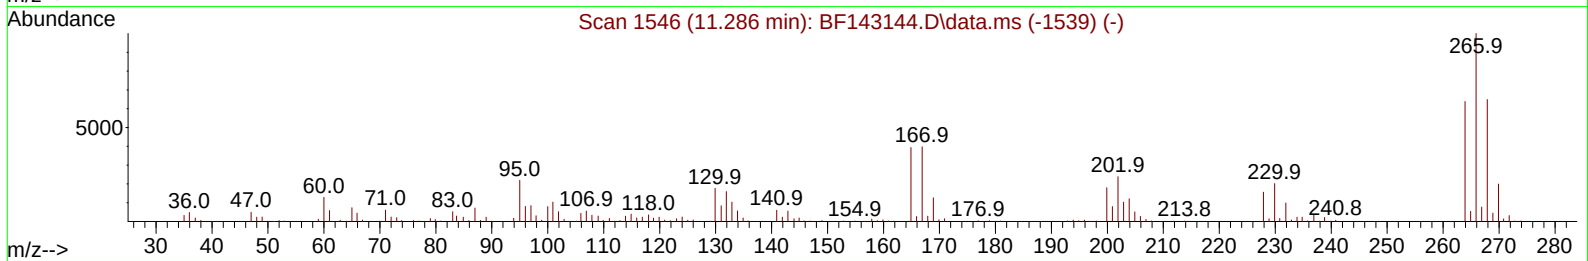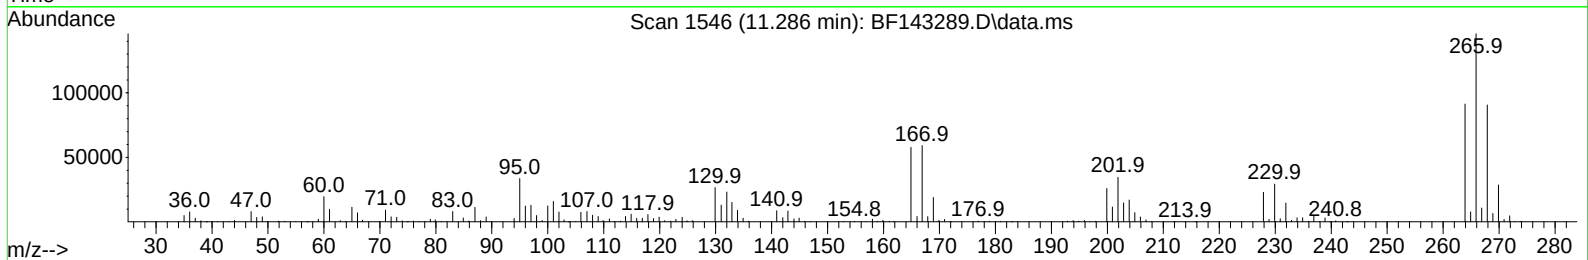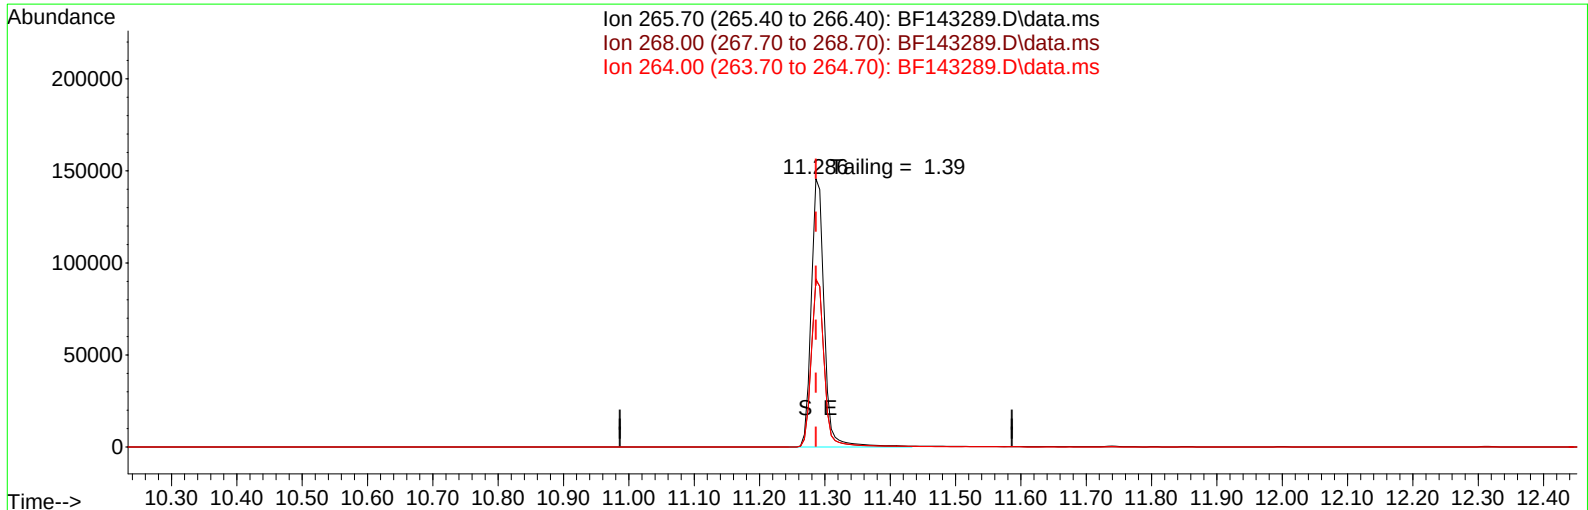

TIC: BF143289.D\data.ms

(70) Pentachlorophenol (C)

11.286min (+ 0.000) 41058.93 ng




response 202716

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	62.18
264.00	63.80	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080425\
Data File : BF143289.D
Acq On : 04 Aug 2025 11:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 04 12:42:57 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

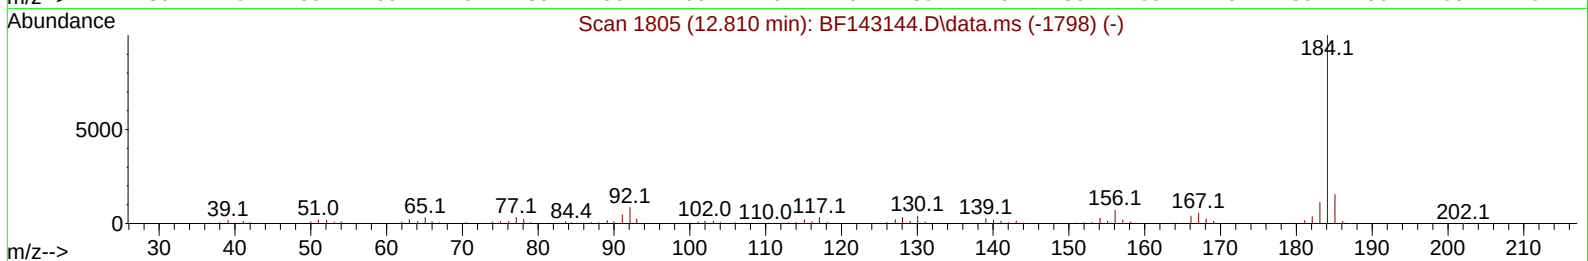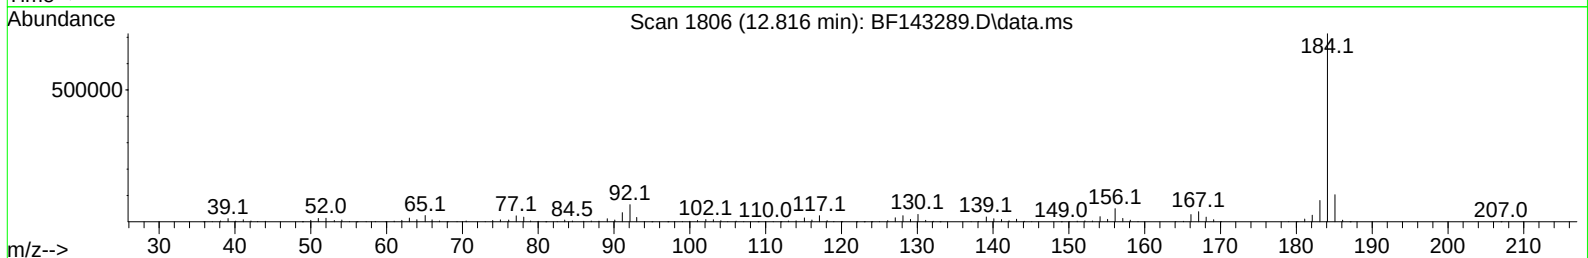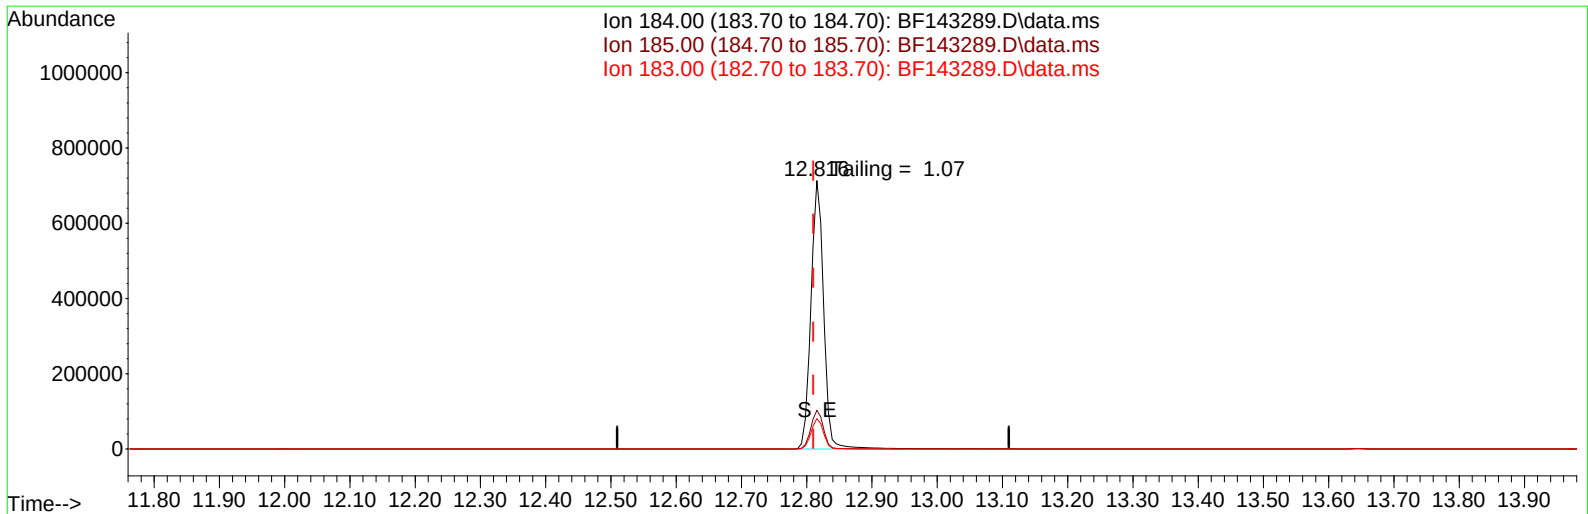

TIC: BF143289.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 3883.80 ng

response 966325

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.44
183.00	11.20	11.34
0.00	0.00	0.00