

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080525\  
 Data File : BF143306.D  
 Acq On : 05 Aug 2025 10:29  
 Operator : RC/JU  
 Sample : PB169095BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB169095BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143306.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.352       | 18            | 27          | 37           | rVB      | 42283          | 77541         | 1.97%           | 0.326%        |
| 2         | 5.210       | 506           | 513         | 526          | rBV      | 246665         | 389234        | 9.89%           | 1.637%        |
| 3         | 5.598       | 573           | 579         | 585          | rBV      | 2291745        | 3235344       | 82.20%          | 13.611%       |
| 4         | 6.587       | 740           | 747         | 752          | rBV      | 2283548        | 3268387       | 83.04%          | 13.750%       |
| 5         | 6.963       | 805           | 811         | 816          | rBV      | 542300         | 687976        | 17.48%          | 2.894%        |
| 6         | 7.516       | 898           | 905         | 910          | rBV      | 1649522        | 2272855       | 57.75%          | 9.562%        |
| 7         | 8.239       | 1022          | 1028        | 1044         | rBV      | 705883         | 918961        | 23.35%          | 3.866%        |
| 8         | 9.316       | 1204          | 1211        | 1216         | rBV      | 2952221        | 3935904       | 100.00%         | 16.558%       |
| 9         | 9.998       | 1321          | 1327        | 1350         | rBV      | 775851         | 1004816       | 25.53%          | 4.227%        |
| 10        | 10.786      | 1455          | 1461        | 1488         | rBV      | 1594812        | 2188311       | 55.60%          | 9.206%        |
| 11        | 11.486      | 1574          | 1580        | 1587         | rBV      | 726109         | 952322        | 24.20%          | 4.006%        |
| 12        | 13.069      | 1843          | 1849        | 1865         | rBV      | 2567117        | 3380766       | 85.90%          | 14.222%       |
| 13        | 14.127      | 2023          | 2029        | 2038         | rBV      | 433829         | 616516        | 15.66%          | 2.594%        |
| 14        | 14.216      | 2038          | 2044        | 2052         | rVV      | 57955          | 96797         | 2.46%           | 0.407%        |
| 15        | 15.633      | 2279          | 2285        | 2313         | rVB      | 374587         | 745089        | 18.93%          | 3.134%        |




Sum of corrected areas: 23770819

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080525\  
Data File : BF143306.D  
Acq On : 05 Aug 2025 10:29  
Operator : RC/JU  
Sample : PB169095BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB169095BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

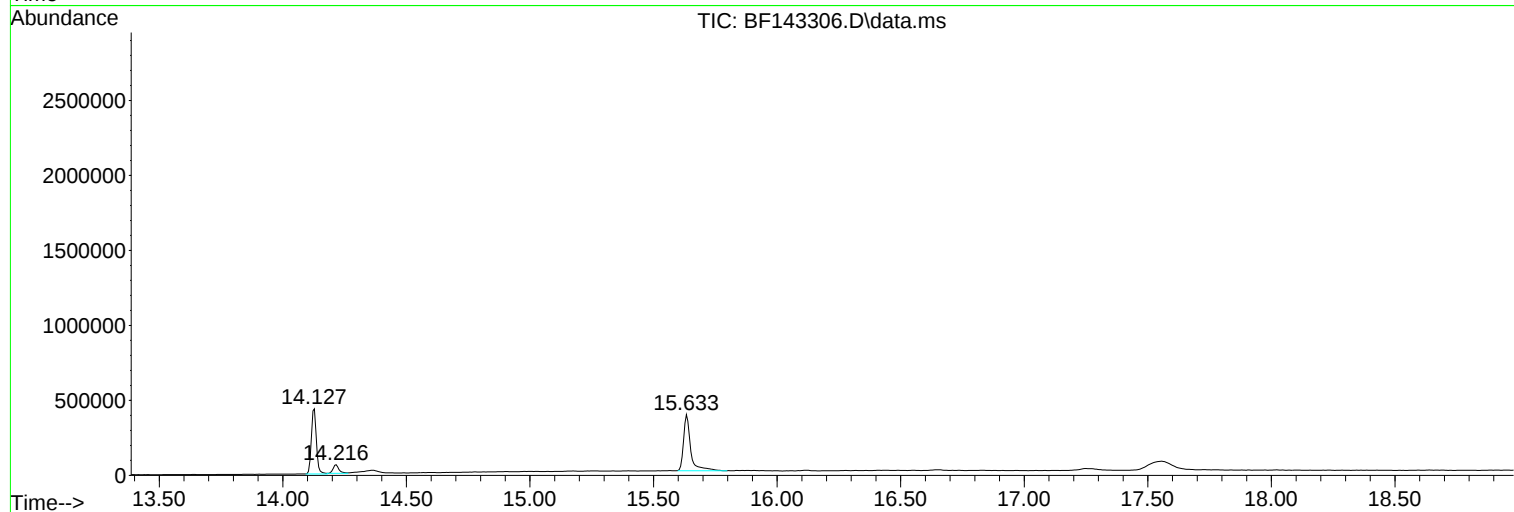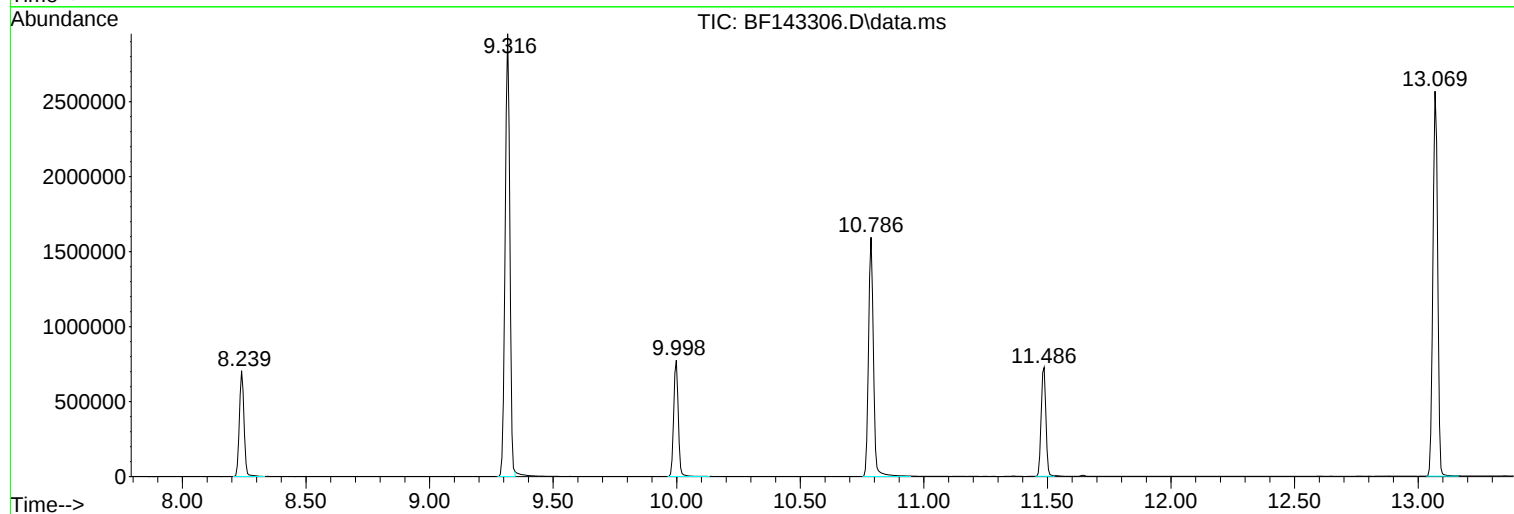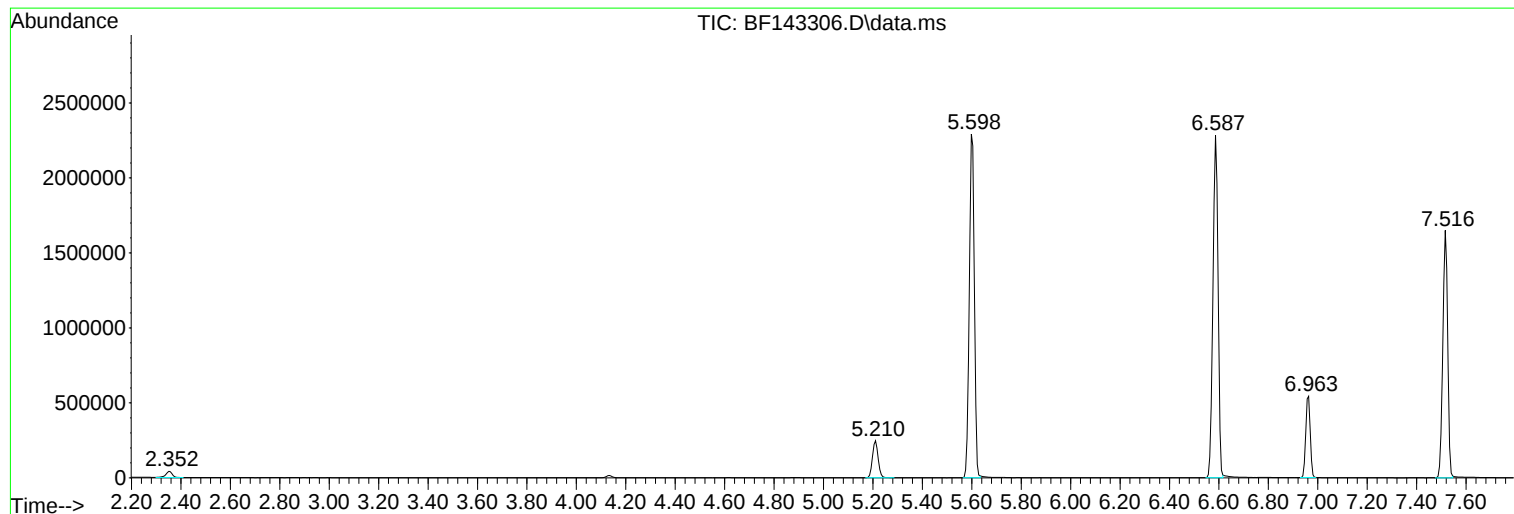

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080525\  
Data File : BF143306.D  
Acq On : 05 Aug 2025 10:29  
Operator : RC/JU  
Sample : PB169095BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB169095BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF080525\  
Data File : BF143306.D  
Acq On : 05 Aug 2025 10:29  
Operator : RC/JU  
Sample : PB169095BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB169095BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF071725.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|