

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080525\
 Data File : PP074223.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Aug 2025 09:46
 Operator : YP\AJ
 Sample : Q2747-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OU4-TS-GRILLO-TSCP02-073125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 05 11:42:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.654	3.800	18795670	46396708	16.807	12.100 #
2) SA Decachlor...	10.426	8.817	16995858	87068997	17.501	14.479

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080525\
Data File : PP074223.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Aug 2025 09:46
Operator : YP\AJ
Sample : Q2747-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 05 11:42:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

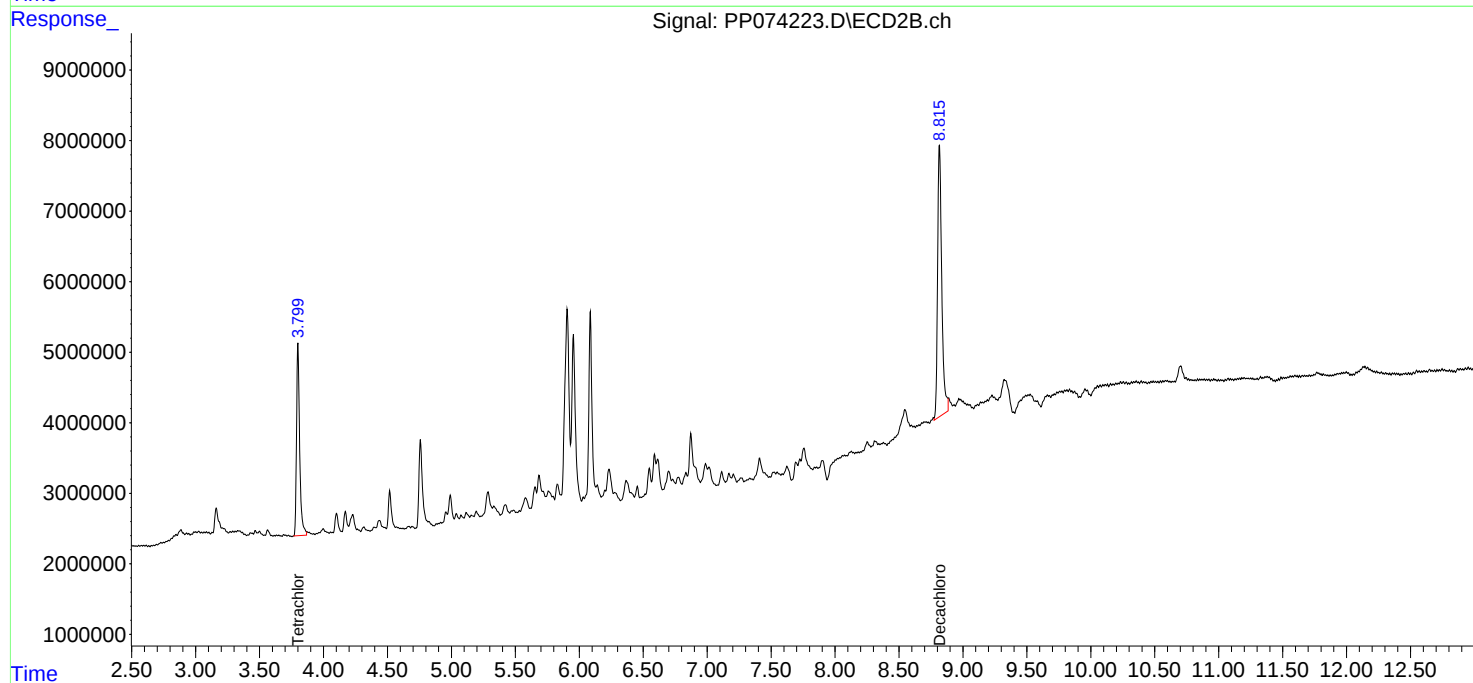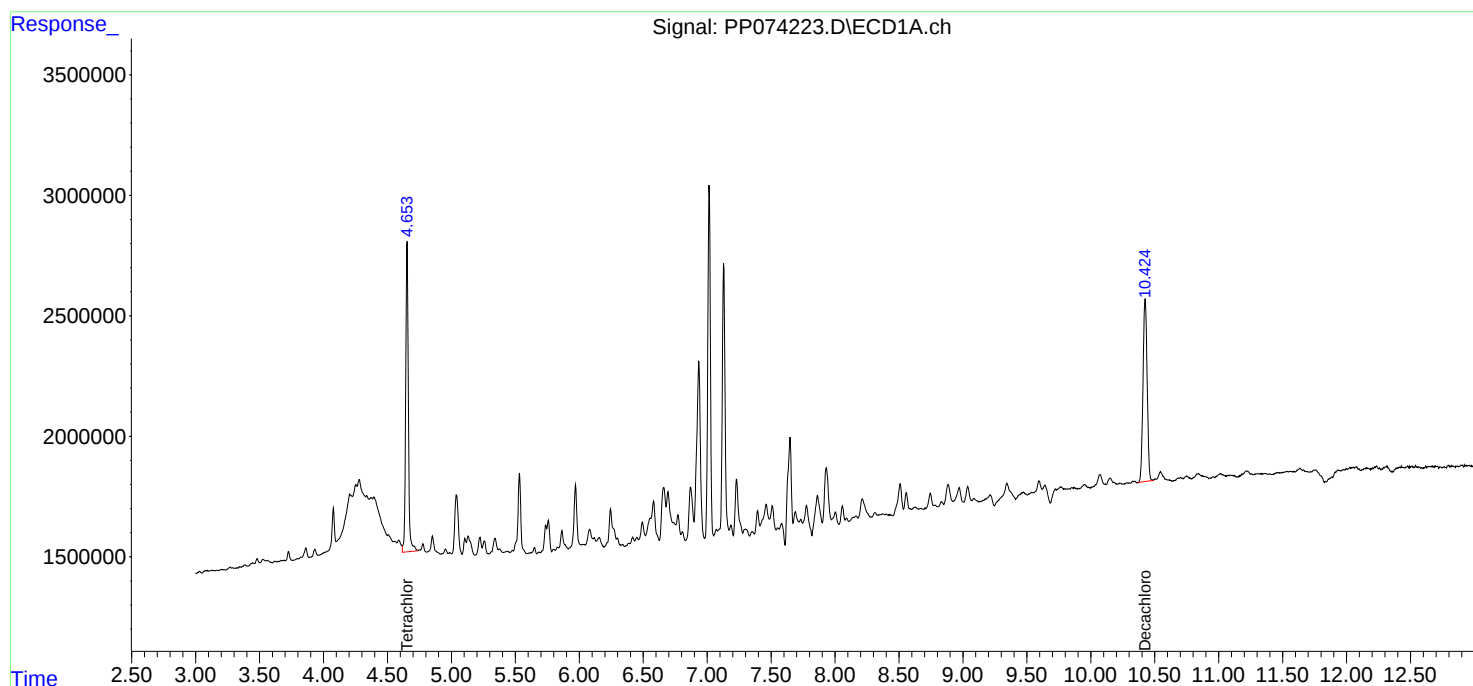


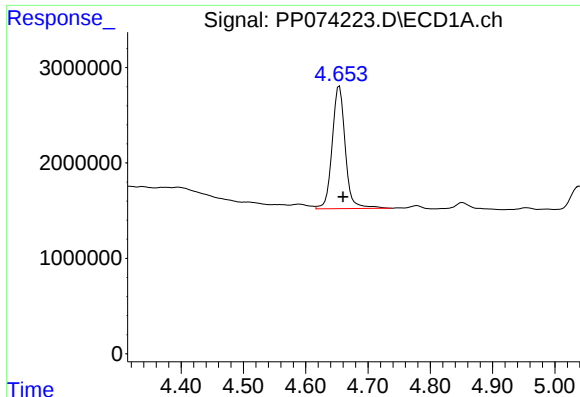

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: -0.006 min
Response: 18795670
Conc: 16.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

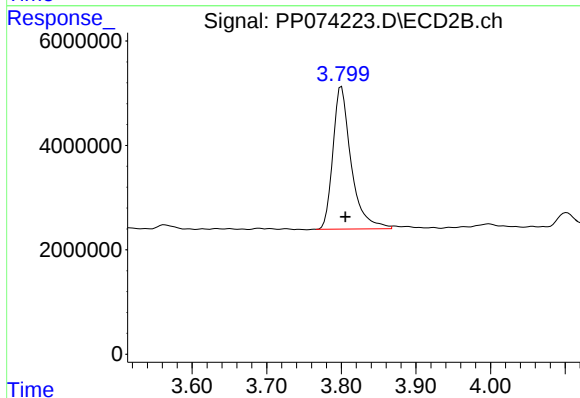


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: -0.005 min
Response: 46396708
Conc: 12.10 ng/ml

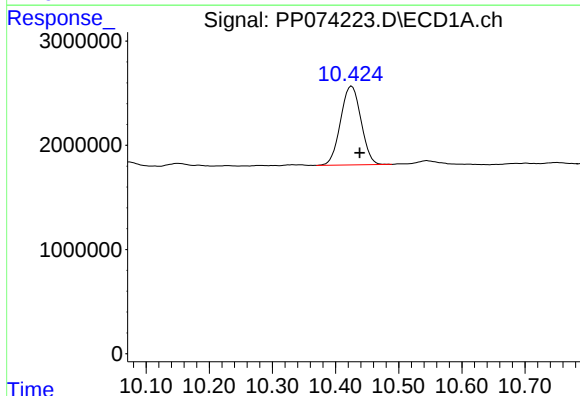

#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.012 min
Response: 16995858
Conc: 17.50 ng/ml

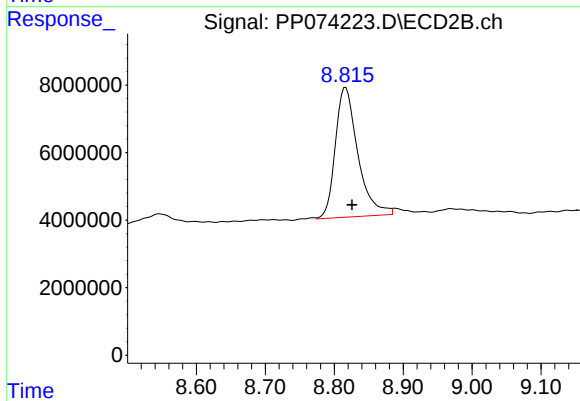

#2 Decachlorobiphenyl

R.T.: 8.817 min
Delta R.T.: -0.009 min
Response: 87068997
Conc: 14.48 ng/ml