

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 11:34
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 07:05:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.877	43497342	289.6E6	17.635	18.287
28)	SA Decachlor...	9.080	8.070	68540687	368.9E6	18.443	18.373
Target Compounds							
9)	A Endosulfan I	6.080	5.243	32929310	180.8E6	8.308	9.250
10)	B gamma-Chl...	5.952	5.123	36168921	212.0E6	8.655	9.788
12)	B 4,4'-DDE	6.202	5.372	65872916	408.9E6	17.661	19.345
13)	MA Dieldrin	6.353	5.510	73492529	408.2E6	17.401	18.863
19)	B Endosulfa...	7.156	6.480	62490576	353.7E6	18.008	19.054
20)	A Methoxychlor	7.501	6.752	158.7E6	839.7E6	88.775	85.727
21)	B Endrin ke...	7.637	6.989	66017266	381.6E6	17.775	19.017



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 11:34
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:05:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

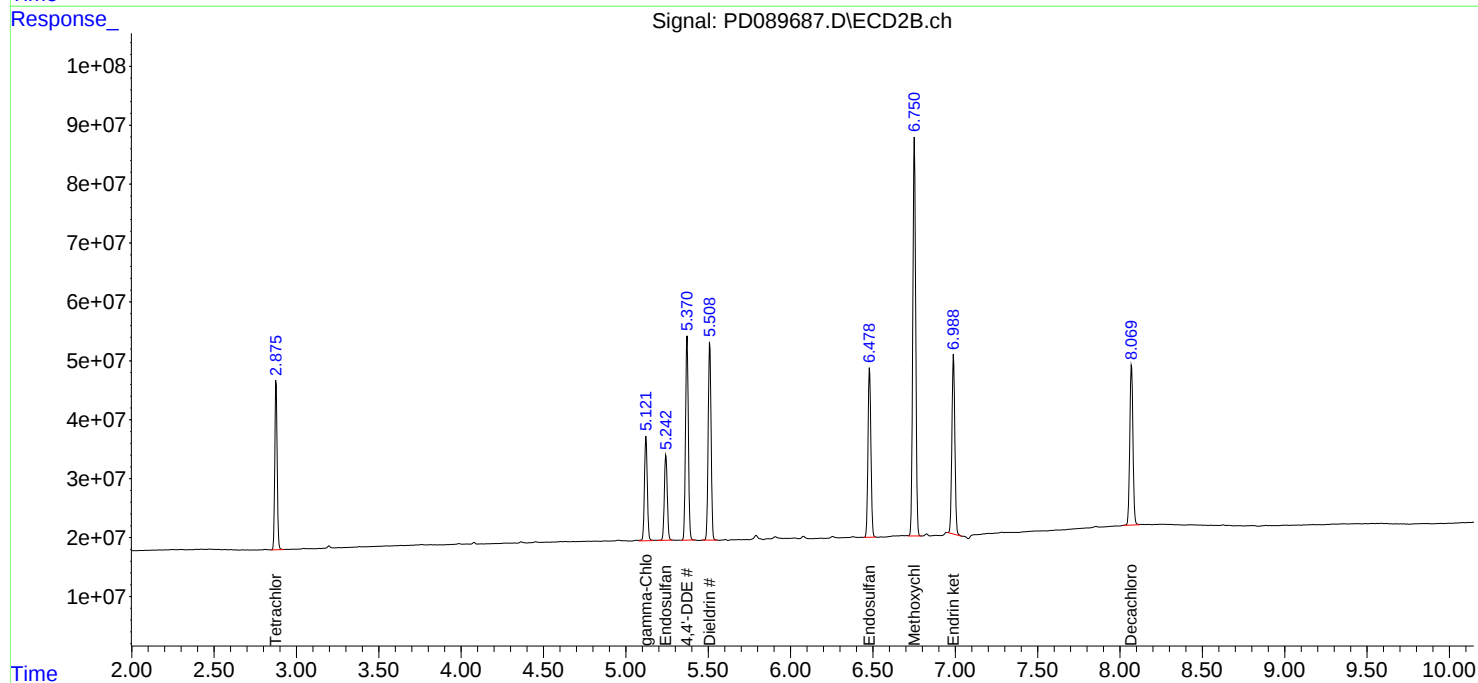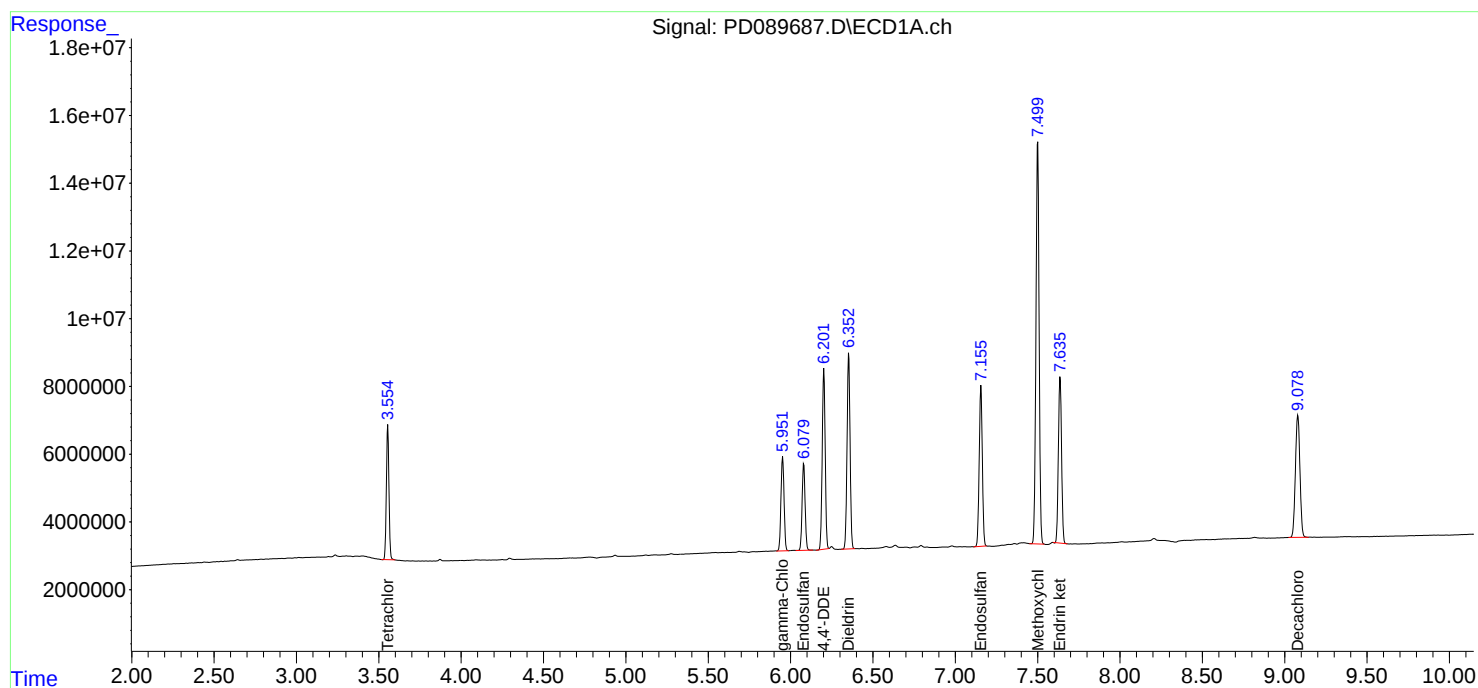


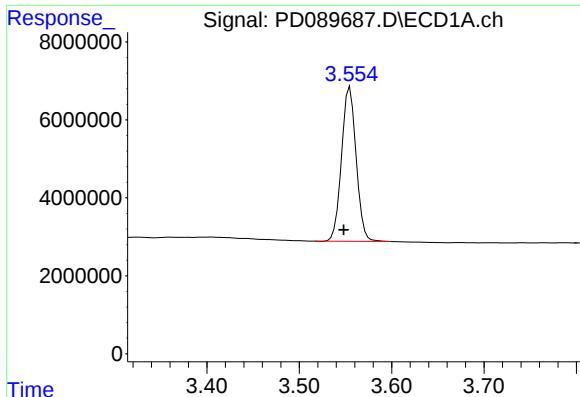

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.007 min
Response: 43497342
Conc: 17.63 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

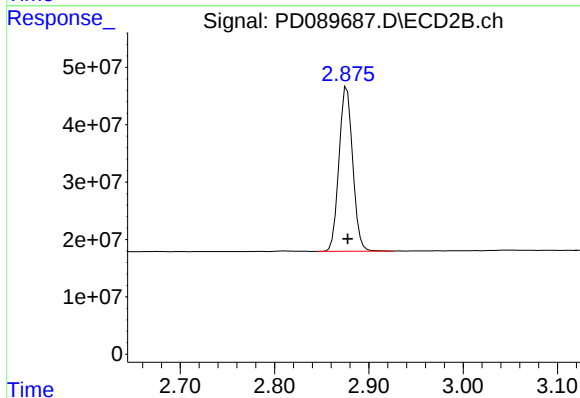


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 289618858
Conc: 18.29 ng/ml

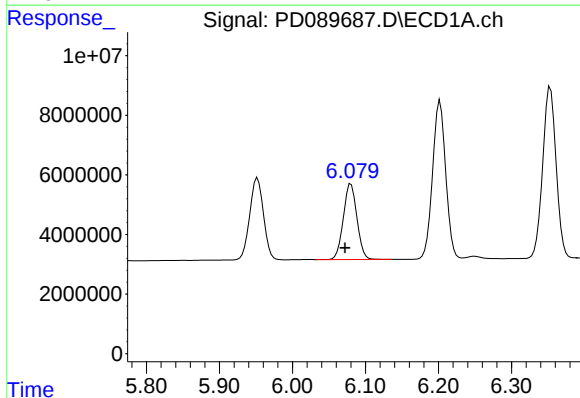


#9 Endosulfan I

R.T.: 6.080 min
Delta R.T.: 0.008 min
Response: 32929310
Conc: 8.31 ng/ml

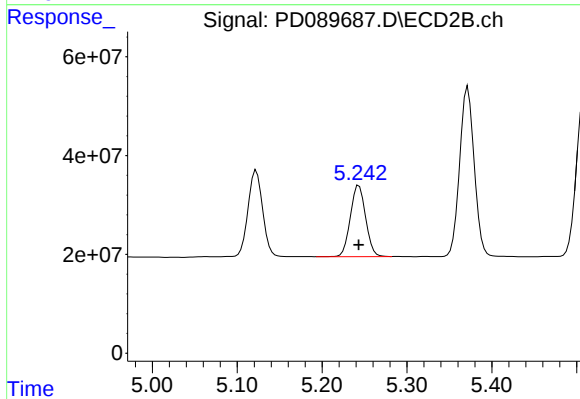

#9 Endosulfan I


R.T.: 5.243 min
Delta R.T.: 0.000 min
Response: 180827207
Conc: 9.25 ng/ml

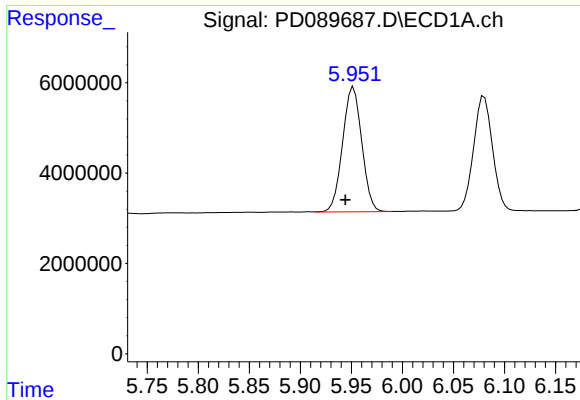

#10 gamma-Chlordane


R.T.: 5.952 min
Delta R.T.: 0.008 min
Response: 36168921
Conc: 8.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

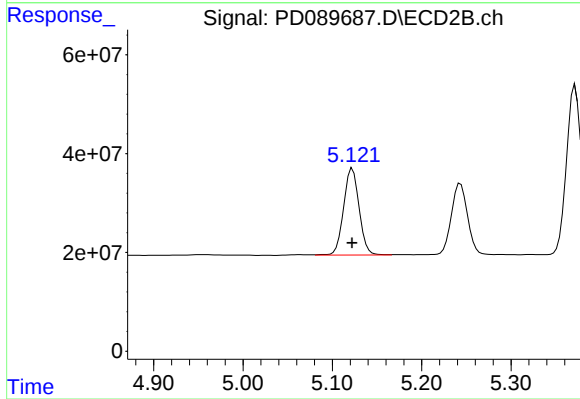


#10 gamma-Chlordane

R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 211952045
Conc: 9.79 ng/ml

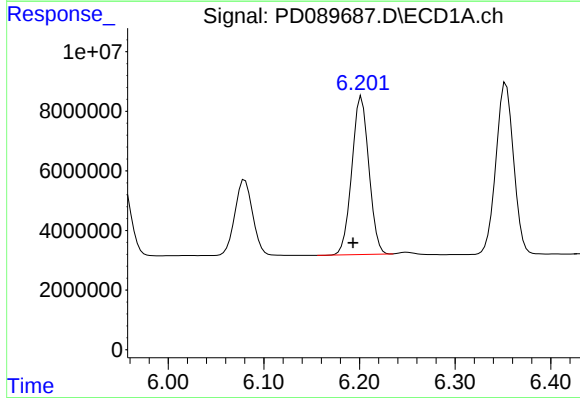


#12 4,4'-DDE

R.T.: 6.202 min
Delta R.T.: 0.009 min
Response: 65872916
Conc: 17.66 ng/ml

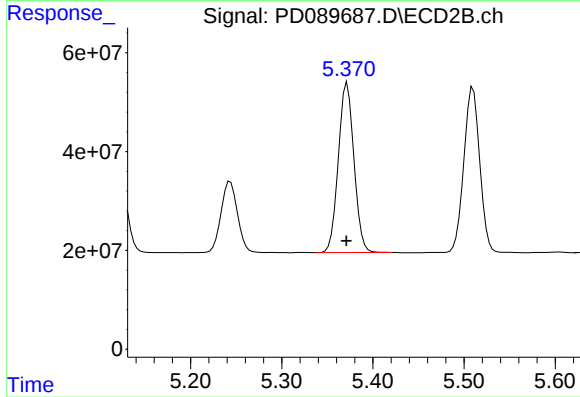

#12 4,4'-DDE


R.T.: 5.372 min
Delta R.T.: 0.000 min
Response: 408894440
Conc: 19.34 ng/ml

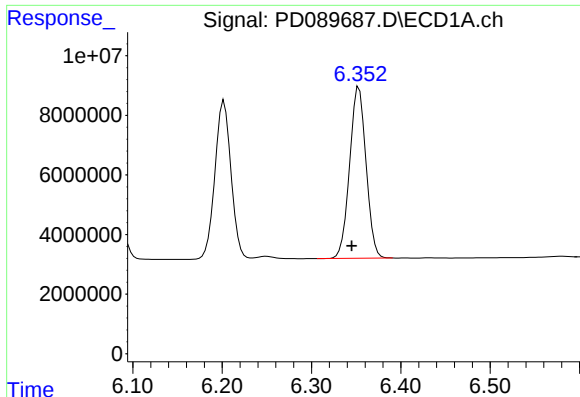

#13 Dieldrin


R.T.: 6.353 min
Delta R.T.: 0.008 min
Response: 73492529
Conc: 17.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

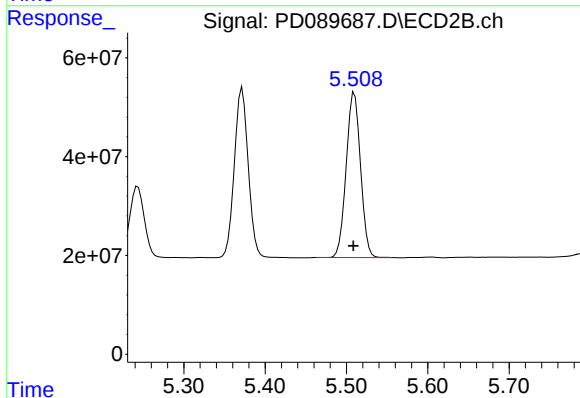


#13 Dieldrin

R.T.: 5.510 min
Delta R.T.: 0.001 min
Response: 408173177
Conc: 18.86 ng/ml

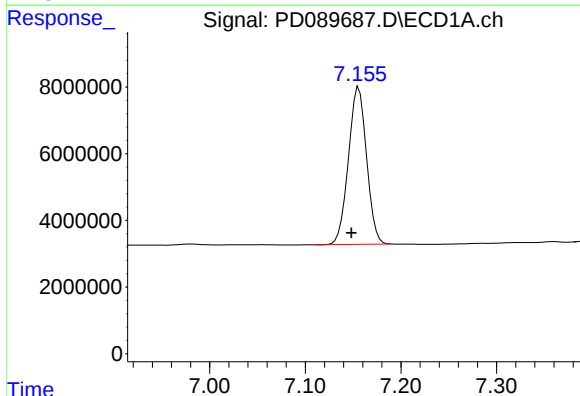


#19 Endosulfan Sulfate

R.T.: 7.156 min
Delta R.T.: 0.008 min
Response: 62490576
Conc: 18.01 ng/ml

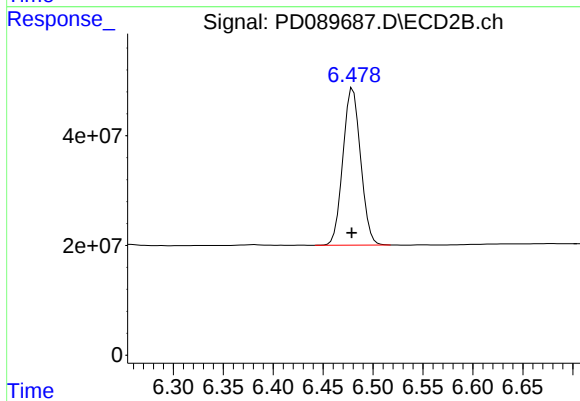

#19 Endosulfan Sulfate


R.T.: 6.480 min
Delta R.T.: 0.001 min
Response: 353740083
Conc: 19.05 ng/ml

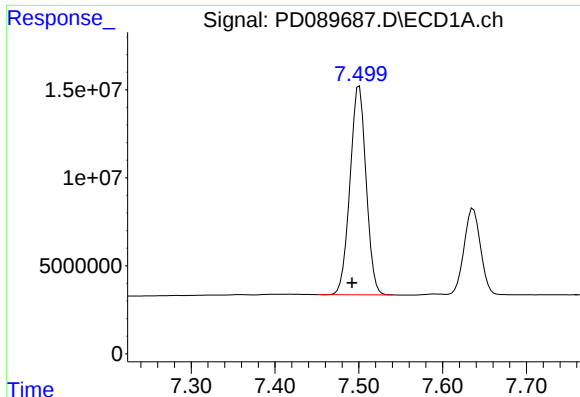

#20 Methoxychlor


R.T.: 7.501 min
Delta R.T.: 0.009 min
Response: 158727415
Conc: 88.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

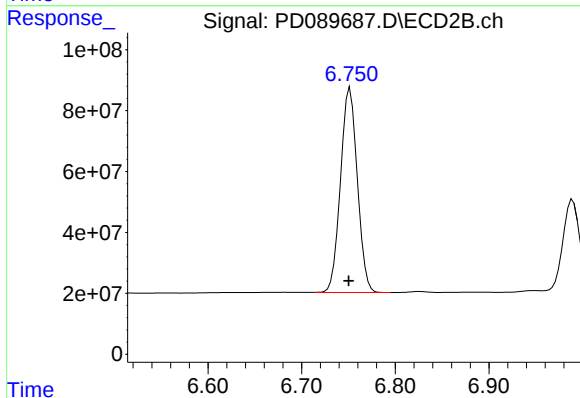


#20 Methoxychlor

R.T.: 6.752 min
Delta R.T.: 0.001 min
Response: 839734343
Conc: 85.73 ng/ml

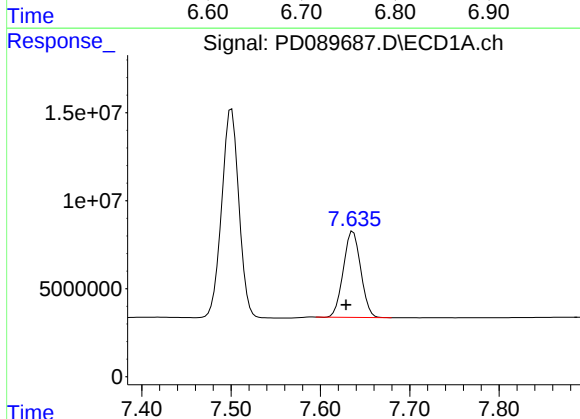


#21 Endrin ketone

R.T.: 7.637 min
Delta R.T.: 0.008 min
Response: 66017266
Conc: 17.77 ng/ml

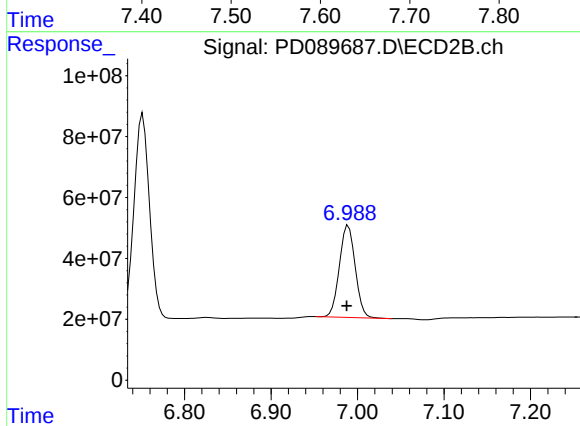

#21 Endrin ketone


R.T.: 6.989 min
Delta R.T.: 0.002 min
Response: 381645681
Conc: 19.02 ng/ml

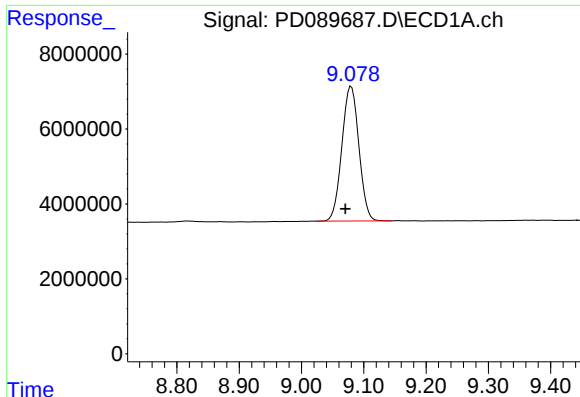

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.009 min
Response: 68540687
Conc: 18.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
RESCHK

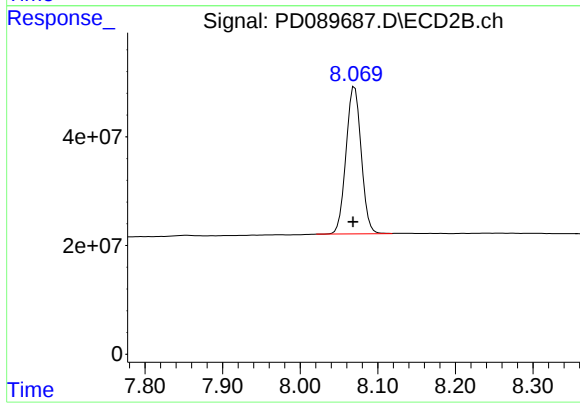

#28 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: 0.002 min
Response: 368884110
Conc: 18.37 ng/ml