

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
 Data File : PL096603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Jul 2025 18:27
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 29 08:11:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
 Quant Title : GC Extractables
 QLast Update : Tue Jul 29 08:08:04 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.827	154.7E6	305.4E6	50.000	50.000
28)	SA Decachlor...	9.015	7.991	113.6E6	210.4E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.689	3.838	80999277	100.1E6	500.000	500.000
24)	Chlordane-2	5.213	4.418	83409909	115.0E6	500.000	500.000
25)	Chlordane-3	5.917	5.052	326.5E6	336.1E6	500.000	500.000
26)	Chlordane-4	6.001	5.115	403.5E6	300.6E6	500.000	500.000
27)	Chlordane-5	6.838	6.009	63996555	122.4E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL072825\
Data File : PL096603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Jul 2025 18:27
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 29 08:11:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL072825.M
Quant Title : GC Extractables
QLast Update : Tue Jul 29 08:08:04 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

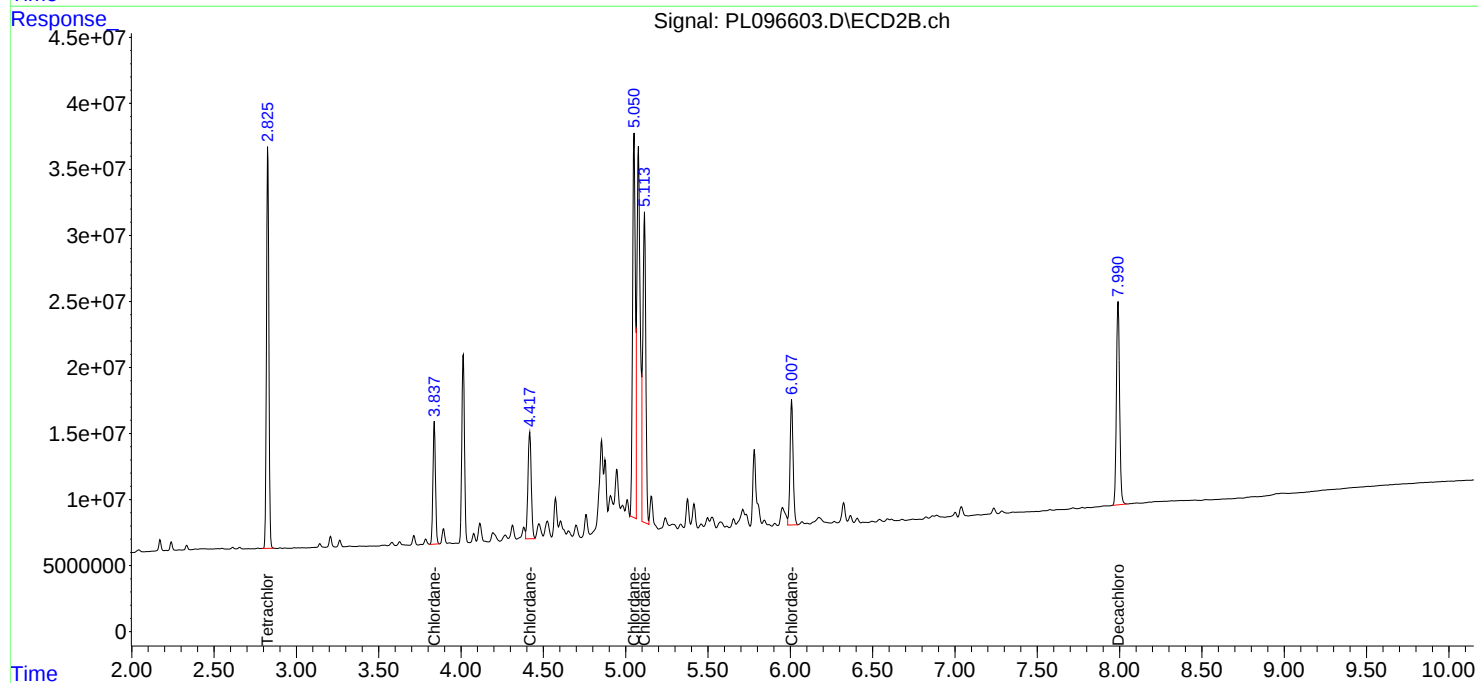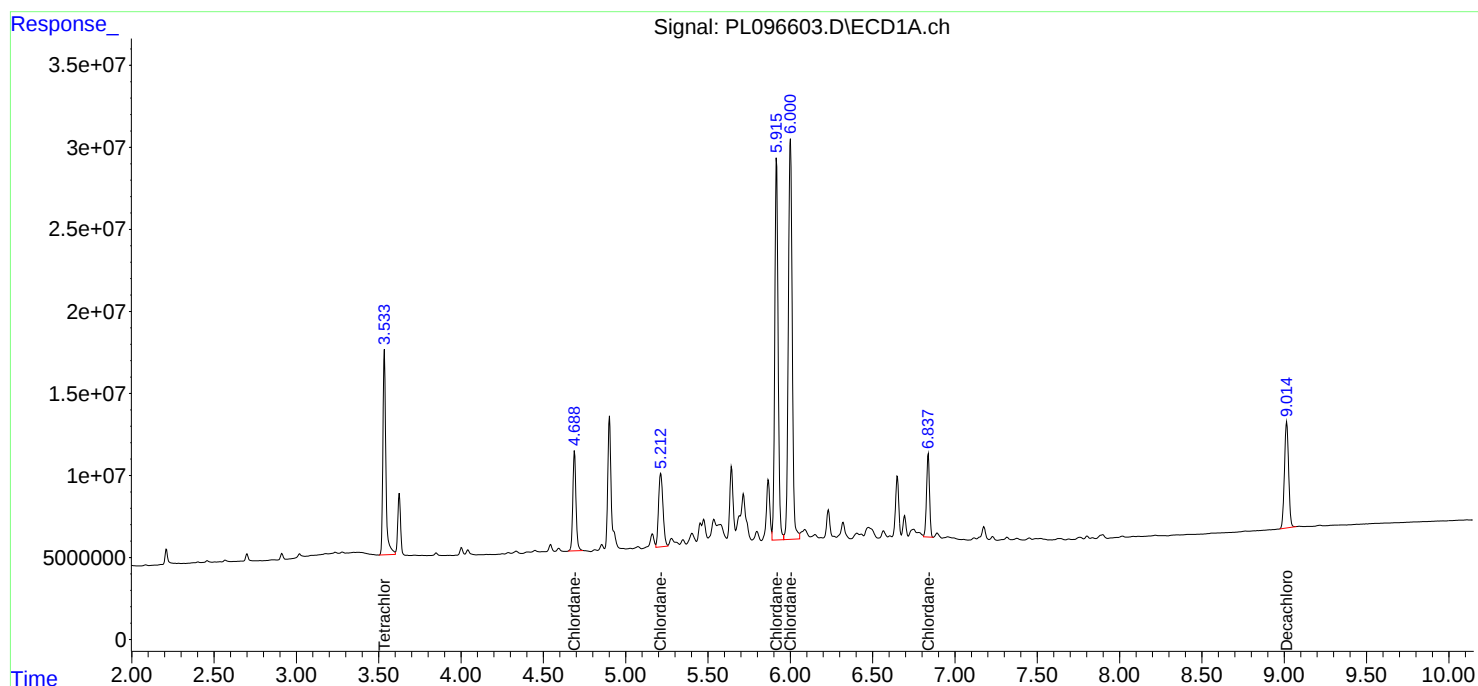


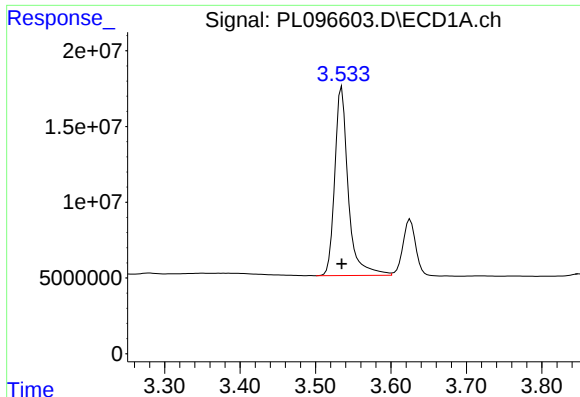

#1 Tetrachloro-m-xylene


R.T.: 3.535 min
Delta R.T.: 0.000 min
Response: 154680305
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

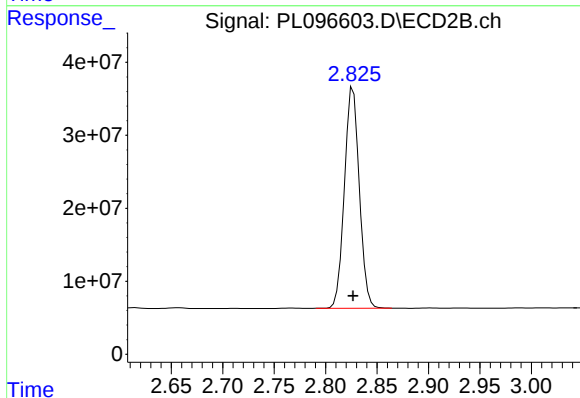


#1 Tetrachloro-m-xylene

R.T.: 2.827 min
Delta R.T.: 0.000 min
Response: 305382843
Conc: 50.00 ng/ml

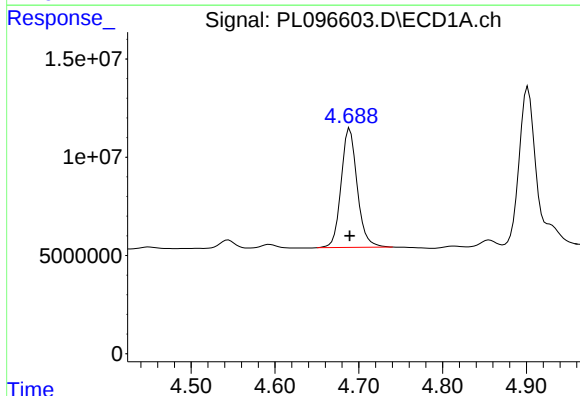


#23 Chlordane-1

R.T.: 4.689 min
Delta R.T.: 0.000 min
Response: 80999277
Conc: 500.00 ng/ml

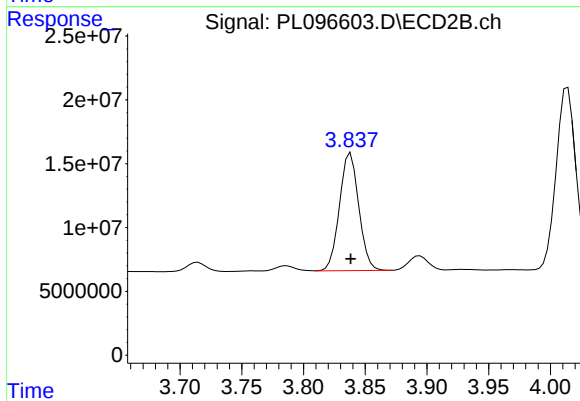

#23 Chlordane-1


R.T.: 3.838 min
Delta R.T.: 0.000 min
Response: 100066760
Conc: 500.00 ng/ml

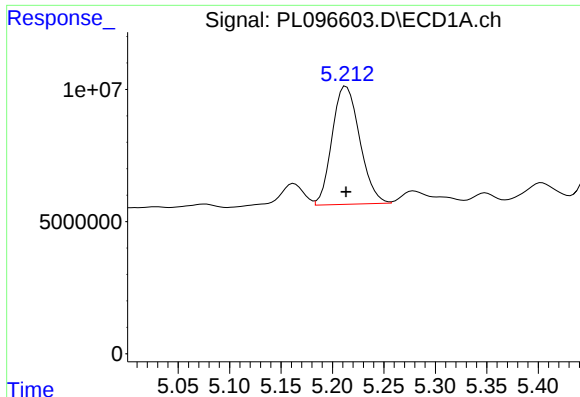

#24 Chlordane-2


R.T.: 5.213 min
Delta R.T.: 0.000 min
Response: 83409909
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

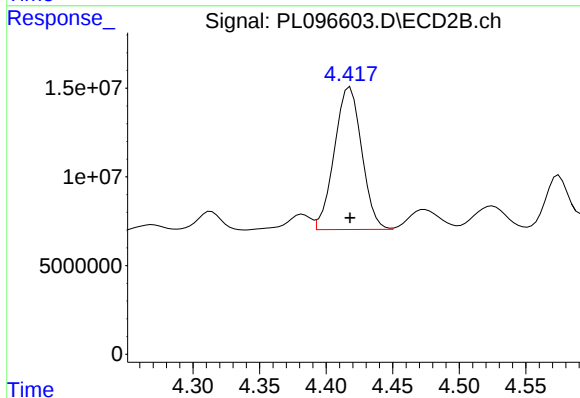


#24 Chlordane-2

R.T.: 4.418 min
Delta R.T.: 0.000 min
Response: 115003204
Conc: 500.00 ng/ml

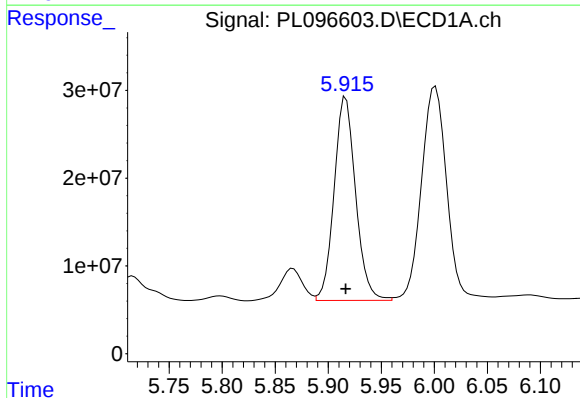


#25 Chlordane-3

R.T.: 5.917 min
Delta R.T.: 0.000 min
Response: 326513783
Conc: 500.00 ng/ml

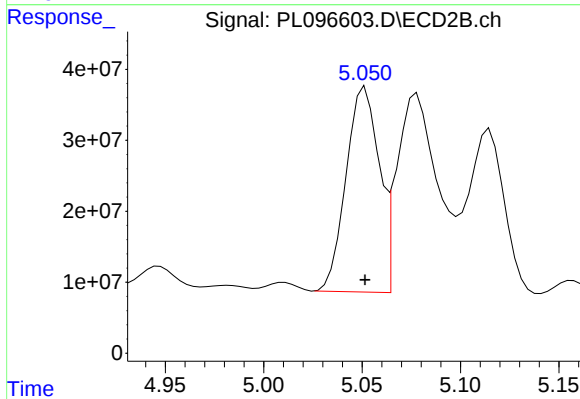

#25 Chlordane-3


R.T.: 5.052 min
Delta R.T.: 0.000 min
Response: 336093734
Conc: 500.00 ng/ml

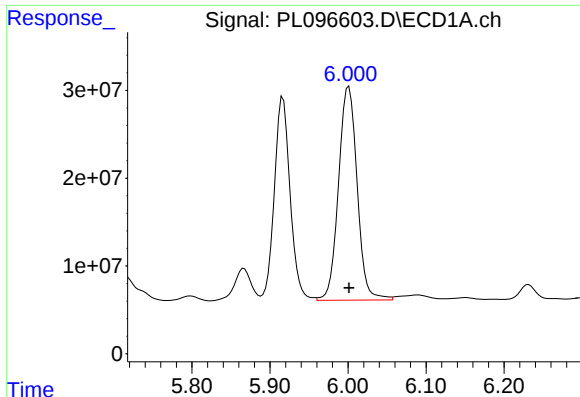

#26 Chlordane-4


R.T.: 6.001 min
Delta R.T.: 0.000 min
Response: 403531433
Conc: 500.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

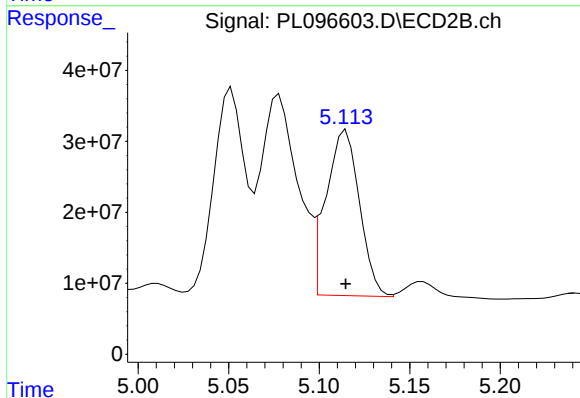


#26 Chlordane-4

R.T.: 5.115 min
Delta R.T.: 0.000 min
Response: 300621016
Conc: 500.00 ng/ml

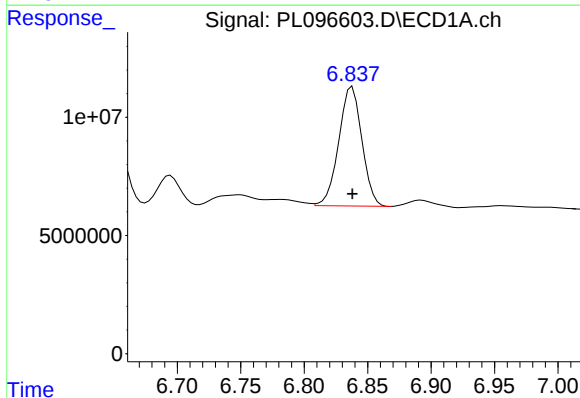


#27 Chlordane-5

R.T.: 6.838 min
Delta R.T.: 0.000 min
Response: 63996555
Conc: 500.00 ng/ml

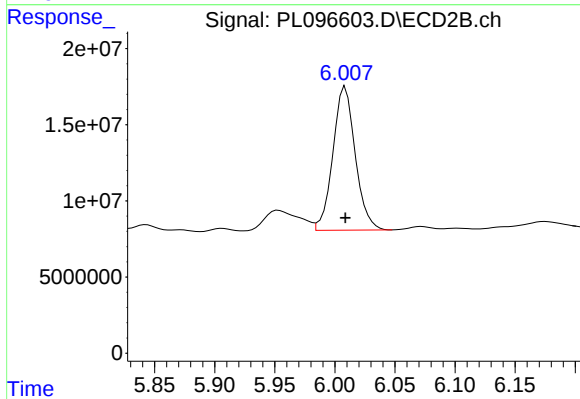

#27 Chlordane-5


R.T.: 6.009 min
Delta R.T.: 0.000 min
Response: 122398851
Conc: 500.00 ng/ml

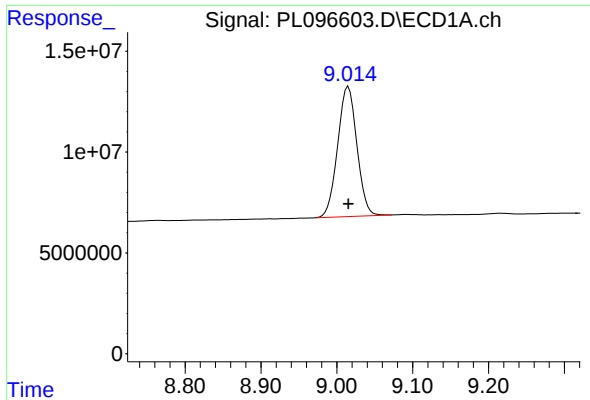

#28 Decachlorobiphenyl

R.T.: 9.015 min
Delta R.T.: 0.000 min
Response: 113631254
Conc: 50.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
PCHLORICC500

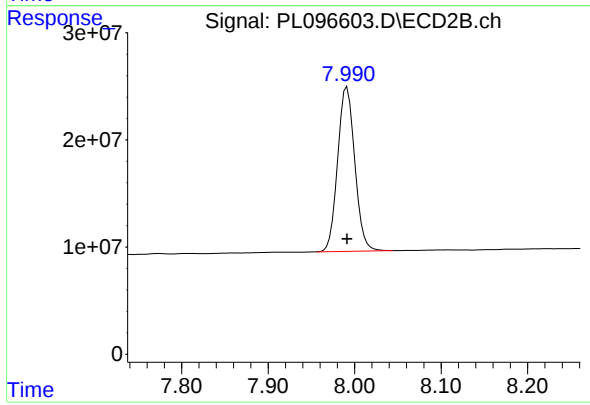

#28 Decachlorobiphenyl

R.T.: 7.991 min
Delta R.T.: 0.000 min
Response: 210412831
Conc: 50.00 ng/ml