

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
 Data File : BF143306.D
 Acq On : 05 Aug 2025 10:29
 Operator : RC/JU
 Sample : PB169095BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB169095BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.352	18	27	37	rVB	42283	77541	1.97%	0.326%
2	5.210	506	513	526	rBV	246665	389234	9.89%	1.637%
3	5.598	573	579	585	rBV	2291745	3235344	82.20%	13.611%
4	6.587	740	747	752	rBV	2283548	3268387	83.04%	13.750%
5	6.963	805	811	816	rBV	542300	687976	17.48%	2.894%
6	7.516	898	905	910	rBV	1649522	2272855	57.75%	9.562%
7	8.239	1022	1028	1044	rBV	705883	918961	23.35%	3.866%
8	9.316	1204	1211	1216	rBV	2952221	3935904	100.00%	16.558%
9	9.998	1321	1327	1350	rBV	775851	1004816	25.53%	4.227%
10	10.786	1455	1461	1488	rBV	1594812	2188311	55.60%	9.206%
11	11.486	1574	1580	1587	rBV	726109	952322	24.20%	4.006%
12	13.069	1843	1849	1865	rBV	2567117	3380766	85.90%	14.222%
13	14.127	2023	2029	2038	rBV	433829	616516	15.66%	2.594%
14	14.216	2038	2044	2052	rVV	57955	96797	2.46%	0.407%
15	15.633	2279	2285	2313	rVB	374587	745089	18.93%	3.134%




Sum of corrected areas: 23770819

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143306.D
Acq On : 05 Aug 2025 10:29
Operator : RC/JU
Sample : PB169095BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169095BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

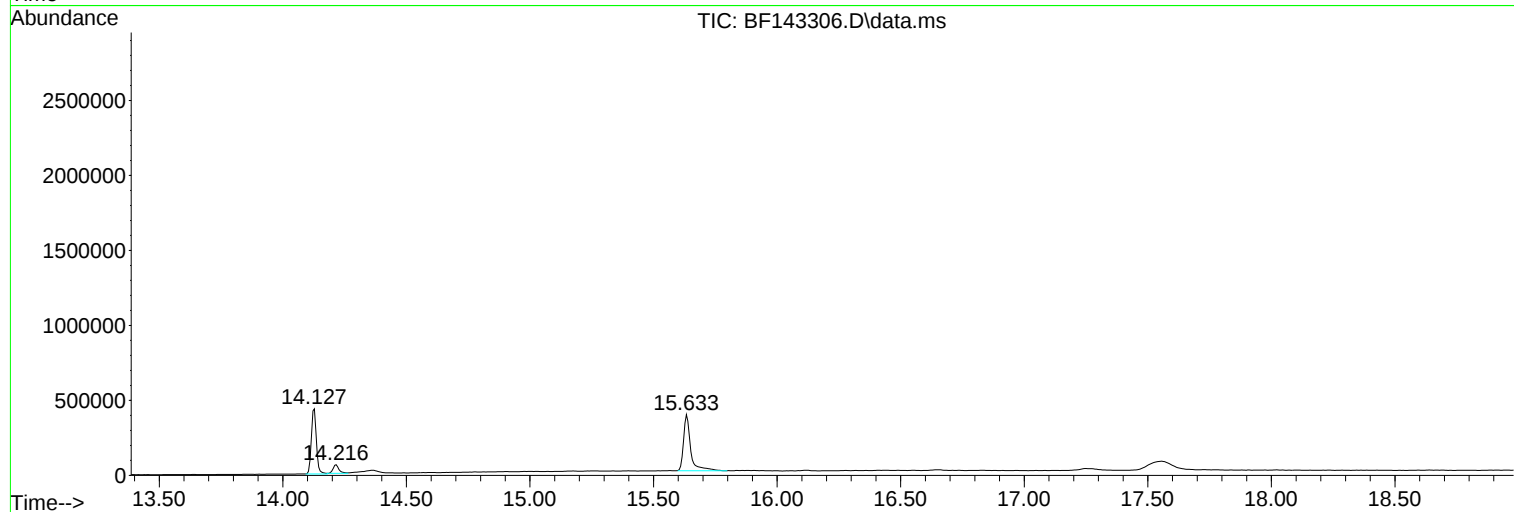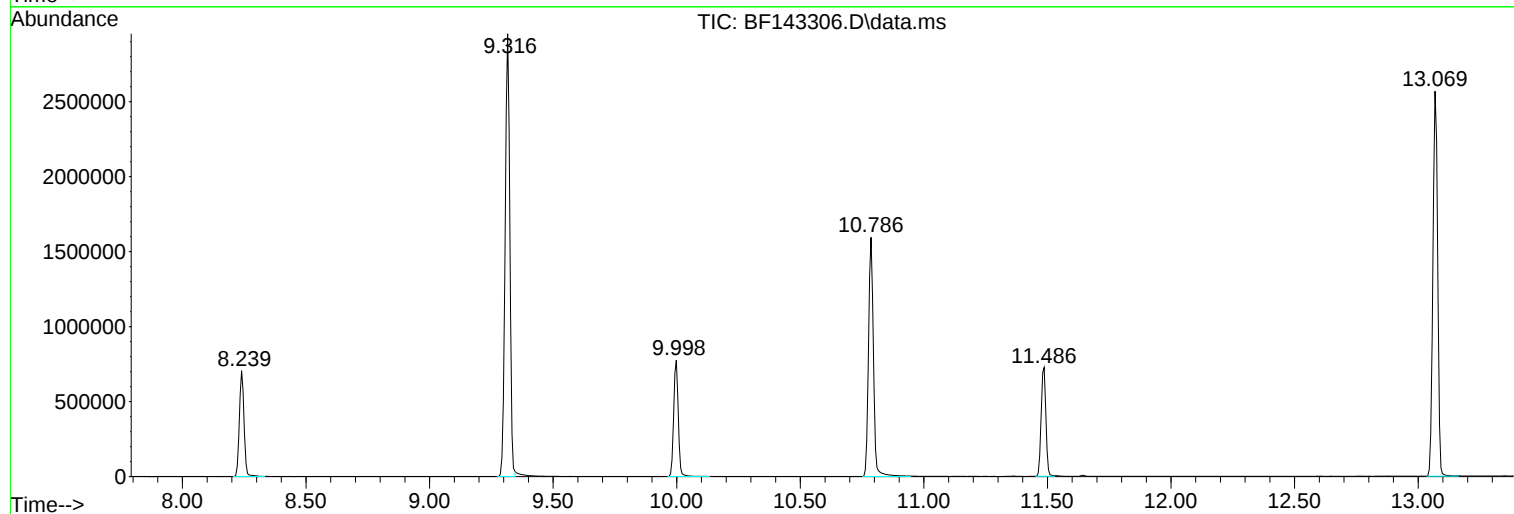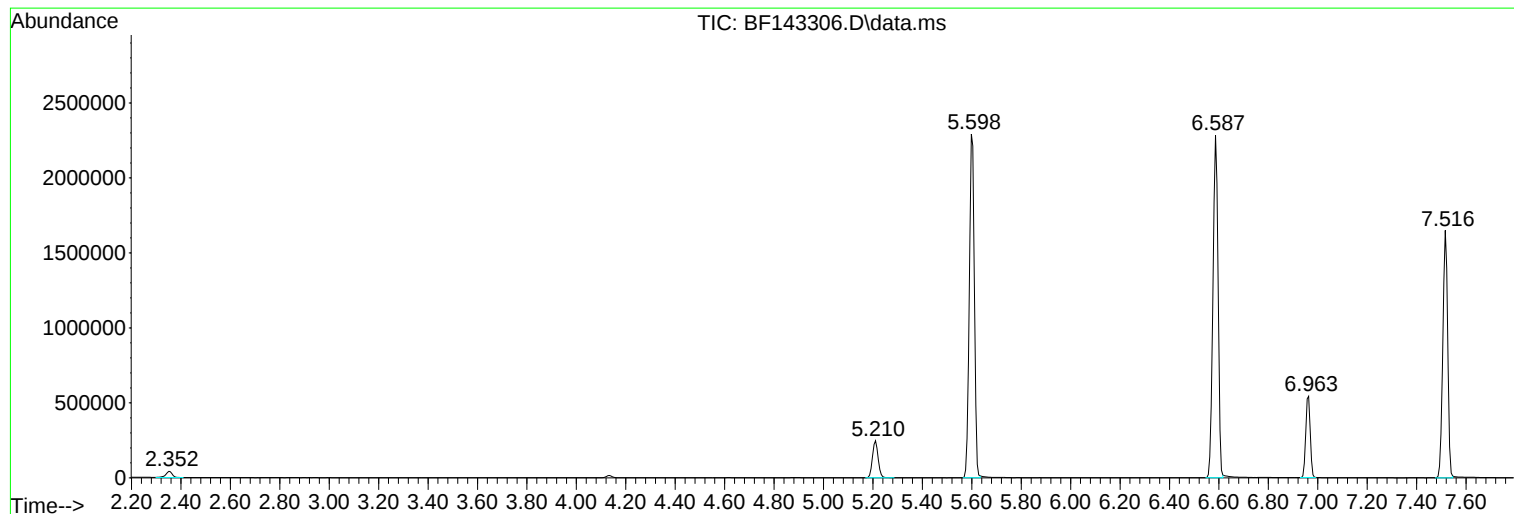

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143306.D
Acq On : 05 Aug 2025 10:29
Operator : RC/JU
Sample : PB169095BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169095BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143306.D
Acq On : 05 Aug 2025 10:29
Operator : RC/JU
Sample : PB169095BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB169095BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------