

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
 Data File : BF143308.D
 Acq On : 05 Aug 2025 11:34
 Operator : RC/JU
 Sample : Q2747-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-OG2-073125

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143308.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.322	15	22	30	rVB	751967	1207349	26.93%	3.247%
2	5.198	504	511	526	rBV	191029	277486	6.19%	0.746%
3	5.598	572	579	584	rBV	1712610	2361061	52.66%	6.349%
4	6.587	740	747	752	rBV	1751558	2410521	53.77%	6.482%
5	6.957	805	810	816	rBV	574655	740718	16.52%	1.992%
6	7.516	899	905	910	rBV	1228184	1611877	35.95%	4.335%
7	8.239	1023	1028	1043	rVB	756768	971100	21.66%	2.612%
8	9.316	1205	1211	1221	rBV	2054724	2708876	60.42%	7.285%
9	9.998	1321	1327	1339	rBV	783420	1042299	23.25%	2.803%
10	10.704	1442	1447	1455	rVB	181617	238802	5.33%	0.642%
11	10.786	1455	1461	1468	rBV	1052888	1427603	31.84%	3.839%
12	11.486	1574	1580	1586	rBV	643531	886426	19.77%	2.384%
13	11.857	1639	1643	1651	rVB3	34993	65601	1.46%	0.176%
14	12.004	1659	1668	1682	rBV2	418919	749263	16.71%	2.015%
15	12.186	1695	1699	1706	rVB4	70469	105942	2.36%	0.285%
16	12.639	1771	1776	1781	rBV2	36561	60931	1.36%	0.164%
17	12.698	1782	1786	1791	rBV	89637	144640	3.23%	0.389%
18	12.792	1797	1802	1815	rBV	91434	162584	3.63%	0.437%
19	12.927	1819	1825	1833	rVB	59560	115812	2.58%	0.311%
20	13.069	1843	1849	1856	rBV	1410914	1845240	41.16%	4.962%
21	13.504	1920	1923	1927	rVB2	46282	55259	1.23%	0.149%
22	13.968	1997	2002	2012	rVB	181920	347865	7.76%	0.935%
23	14.127	2024	2029	2039	rVB	505186	743568	16.59%	2.000%
24	14.216	2040	2044	2050	rVB	85063	124766	2.78%	0.336%
25	14.280	2052	2055	2062	rVB2	47653	71588	1.60%	0.193%
26	14.586	2103	2107	2120	rVB2	161746	300203	6.70%	0.807%
27	14.986	2171	2175	2183	rVB	226758	331490	7.39%	0.891%
28	15.145	2198	2202	2205	rBV	53389	88111	1.97%	0.237%
29	15.257	2217	2221	2227	rVB	548108	760396	16.96%	2.045%
30	15.633	2280	2285	2297	rVB	407527	696619	15.54%	1.873%
31	16.009	2345	2349	2360	rVB	57744	119443	2.66%	0.321%
32	16.121	2362	2368	2374	rVB	407283	713486	15.91%	1.919%
33	16.404	2411	2416	2430	rVB	162942	416286	9.29%	1.119%
34	17.568	2608	2614	2636	rVB5	184170	629000	14.03%	1.692%
35	17.868	2650	2665	2676	rBV4	1143391	4483362	100.00%	12.057%
36	18.051	2691	2696	2704	rVB	309959	730521	16.29%	1.965%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143308.D
Acq On : 05 Aug 2025 11:34
Operator : RC/JU
Sample : Q2747-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG2-073125

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.321	2734	2742	2753	rBV	631575	2291112	51.10%	6.161%
38	18.427	2755	2760	2772	rVB5	449144	1434502	32.00%	3.858%
39	18.698	2796	2806	2825	rBV7	508685	3199025	71.35%	8.603%
40	18.851	2826	2832	2837	rBV2	209462	514323	11.47%	1.383%




Sum of corrected areas: 37185056

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143308.D
Acq On : 05 Aug 2025 11:34
Operator : RC/JU
Sample : Q2747-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG2-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

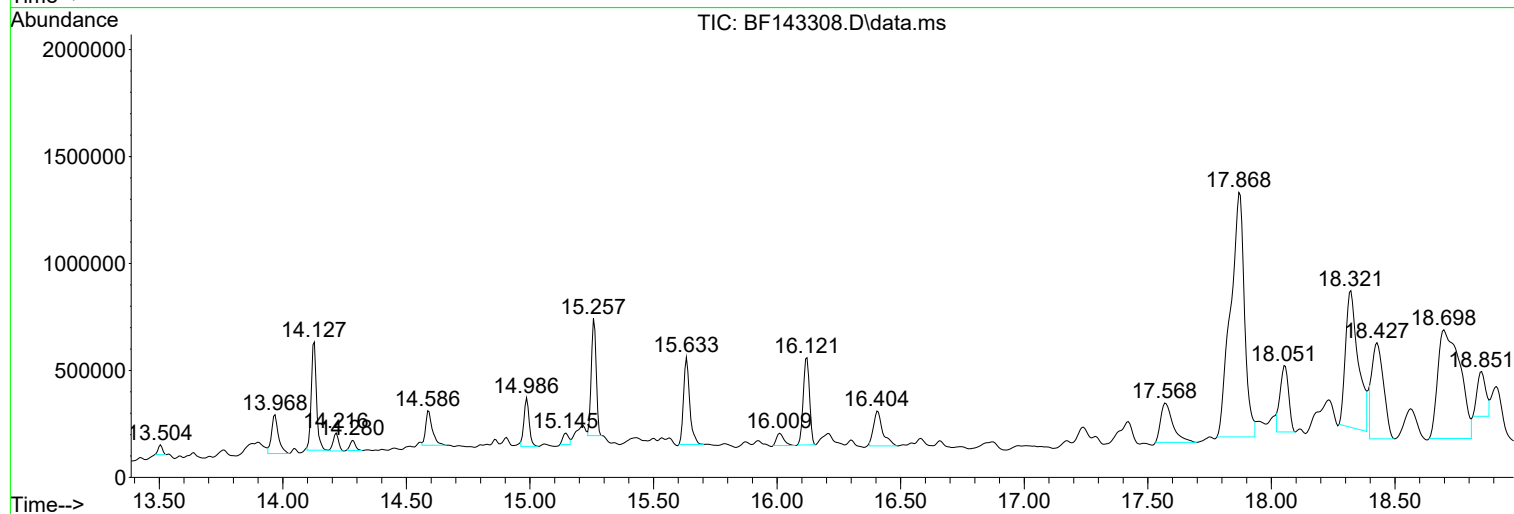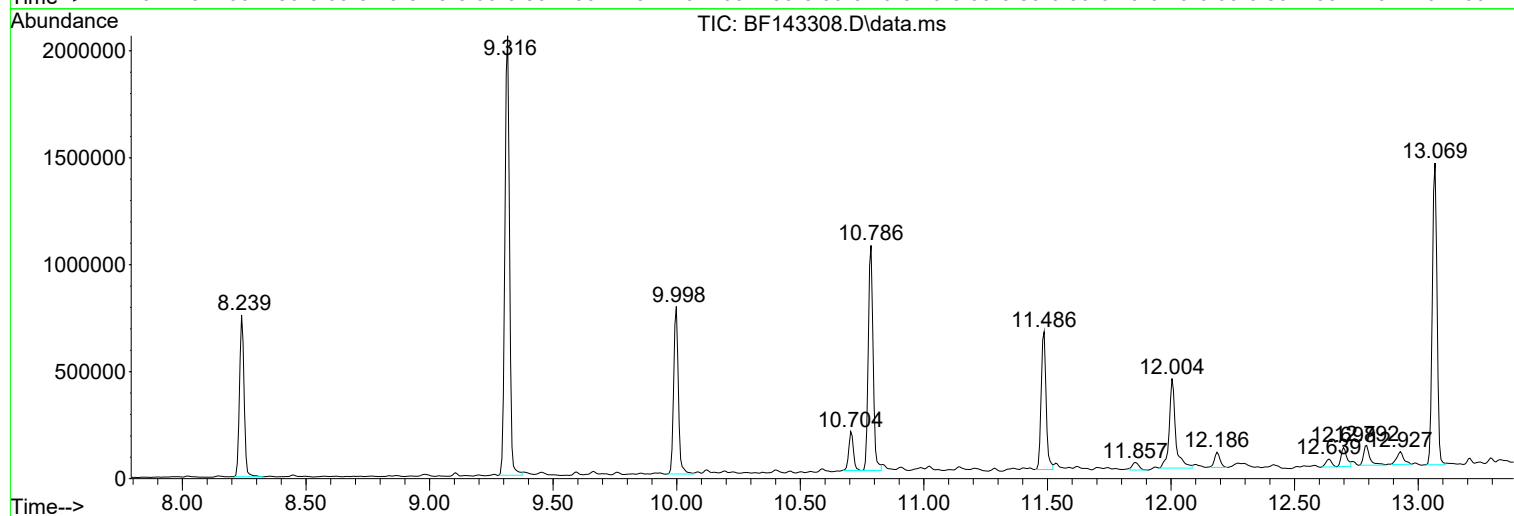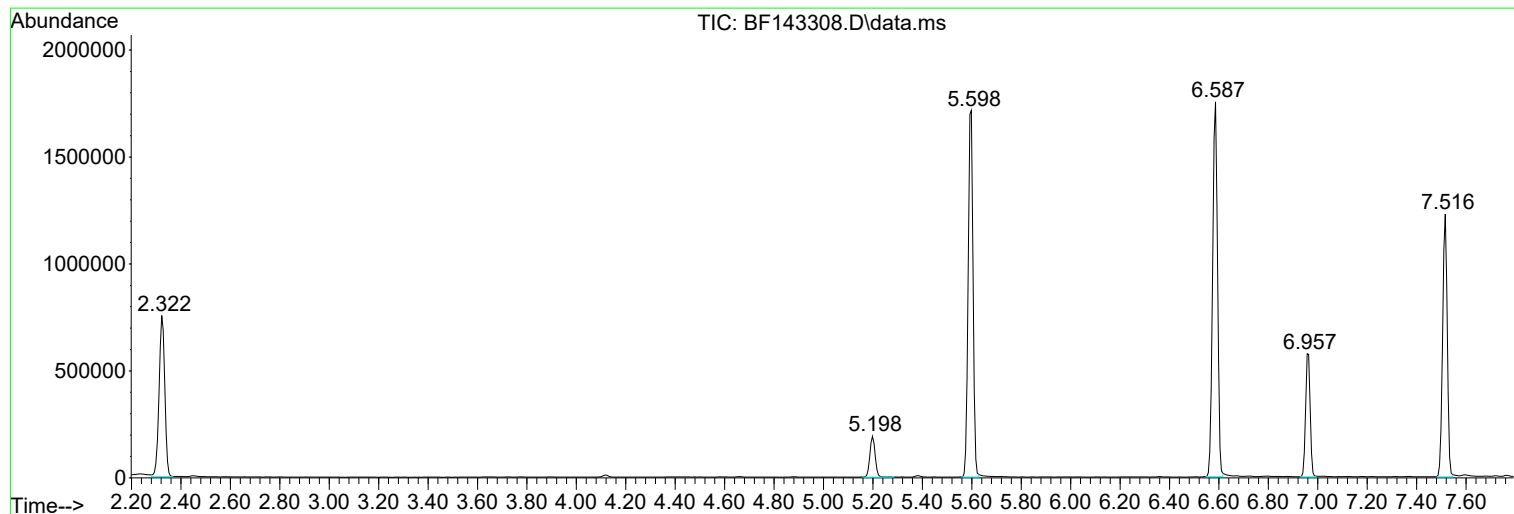

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143308.D
Acq On : 05 Aug 2025 11:34
Operator : RC/JU
Sample : Q2747-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG2-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143308.D
Acq On : 05 Aug 2025 11:34
Operator : RC/JU
Sample : Q2747-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG2-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc