

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
 Data File : BF143310.D
 Acq On : 05 Aug 2025 12:32
 Operator : RC/JU
 Sample : Q2747-05
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-OG4-073125

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143310.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.304	12	19	29	rVB	835877	1323904	23.83%	2.992%
2	5.198	504	511	523	rBV	209269	306227	5.51%	0.692%
3	5.598	572	579	584	rBV	1795144	2449386	44.09%	5.535%
4	6.587	737	747	759	rBV	1812303	2500115	45.01%	5.649%
5	6.963	806	811	816	rBV	618697	759668	13.68%	1.717%
6	7.516	899	905	910	rBV	1259477	1651129	29.72%	3.731%
7	8.239	1023	1028	1043	rVB	737955	955714	17.20%	2.160%
8	9.316	1205	1211	1219	rBV	2008826	2571993	46.30%	5.812%
9	9.998	1321	1327	1339	rBV	726918	960905	17.30%	2.171%
10	10.704	1443	1447	1454	rVB	160149	209575	3.77%	0.474%
11	10.786	1455	1461	1477	rVB	909330	1260247	22.69%	2.848%
12	11.486	1575	1580	1586	rBV	565486	753751	13.57%	1.703%
13	11.851	1639	1642	1652	rVB3	37700	71274	1.28%	0.161%
14	12.010	1664	1669	1682	rVB	419547	676347	12.18%	1.528%
15	12.186	1695	1699	1710	rVB4	92598	149420	2.69%	0.338%
16	12.627	1770	1774	1782	rVB	73403	125294	2.26%	0.283%
17	12.698	1782	1786	1797	rBV2	95497	246157	4.43%	0.556%
18	12.792	1798	1802	1809	rBV	104663	166904	3.00%	0.377%
19	13.068	1844	1849	1854	rBV	1414467	1795433	32.32%	4.057%
20	13.504	1920	1923	1927	rBV3	75402	102278	1.84%	0.231%
21	13.962	1997	2001	2011	rVB	308415	505881	9.11%	1.143%
22	14.051	2013	2016	2018	rBV	51252	72728	1.31%	0.164%
23	14.127	2021	2029	2040	rVB	857355	1890546	34.03%	4.272%
24	14.592	2103	2108	2115	rBV2	368554	576788	10.38%	1.303%
25	14.986	2171	2175	2183	rVB	328748	469026	8.44%	1.060%
26	15.145	2199	2202	2206	rBV2	66013	94140	1.69%	0.213%
27	15.262	2217	2222	2233	rVB	929884	1480059	26.64%	3.344%
28	15.633	2280	2285	2303	rVB	383118	725523	13.06%	1.639%
29	16.009	2345	2349	2359	rVB	120621	237301	4.27%	0.536%
30	16.121	2362	2368	2374	rBV	653763	1132167	20.38%	2.558%
31	16.409	2412	2417	2430	rVB	248651	575911	10.37%	1.301%
32	17.568	2607	2614	2625	rBV5	286244	805644	14.50%	1.820%
33	17.880	2651	2667	2684	rBV4	1263036	5555050	100.00%	12.552%
34	18.062	2692	2698	2705	rVB	467551	1117849	20.12%	2.526%
35	18.327	2734	2743	2755	rBV	903244	3218926	57.95%	7.274%
36	18.433	2756	2761	2773	rVB5	618997	1890923	34.04%	4.273%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143310.D
Acq On : 05 Aug 2025 12:32
Operator : RC/JU
Sample : Q2747-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG4-073125

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	18.697	2796	2806	2825	rBV4	732873	4066890	73.21%	9.190%
38	18.856	2826	2833	2839	rBV2	303922	803938	14.47%	1.817%




Sum of corrected areas: 44255011

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143310.D
Acq On : 05 Aug 2025 12:32
Operator : RC/JU
Sample : Q2747-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG4-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

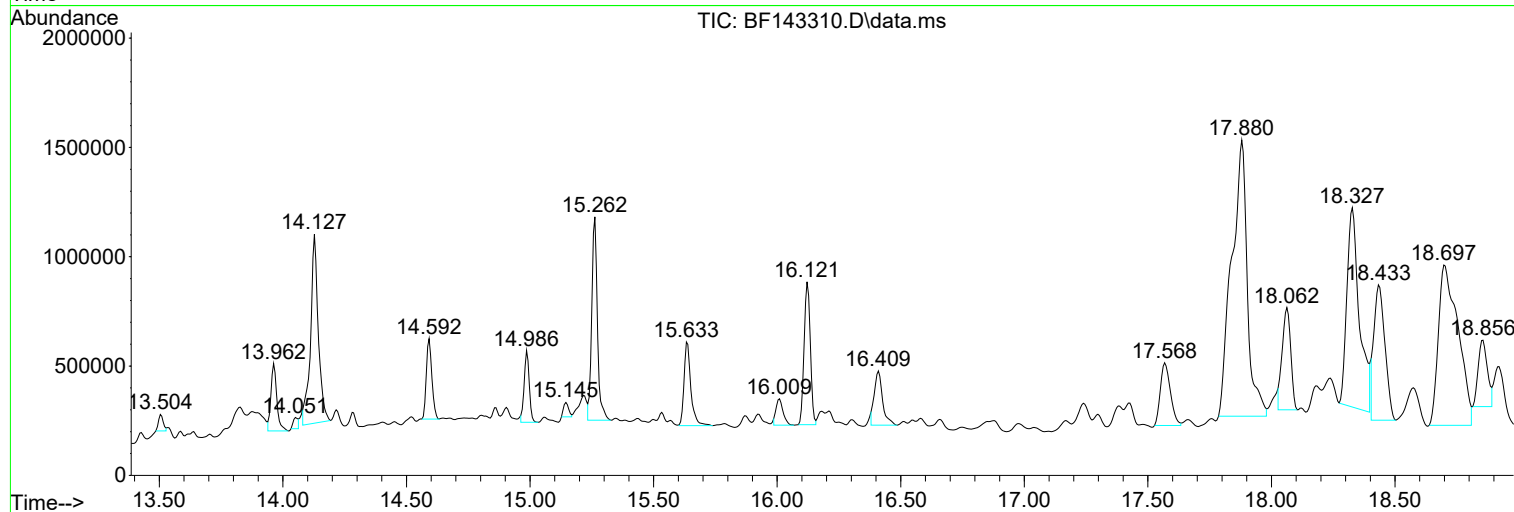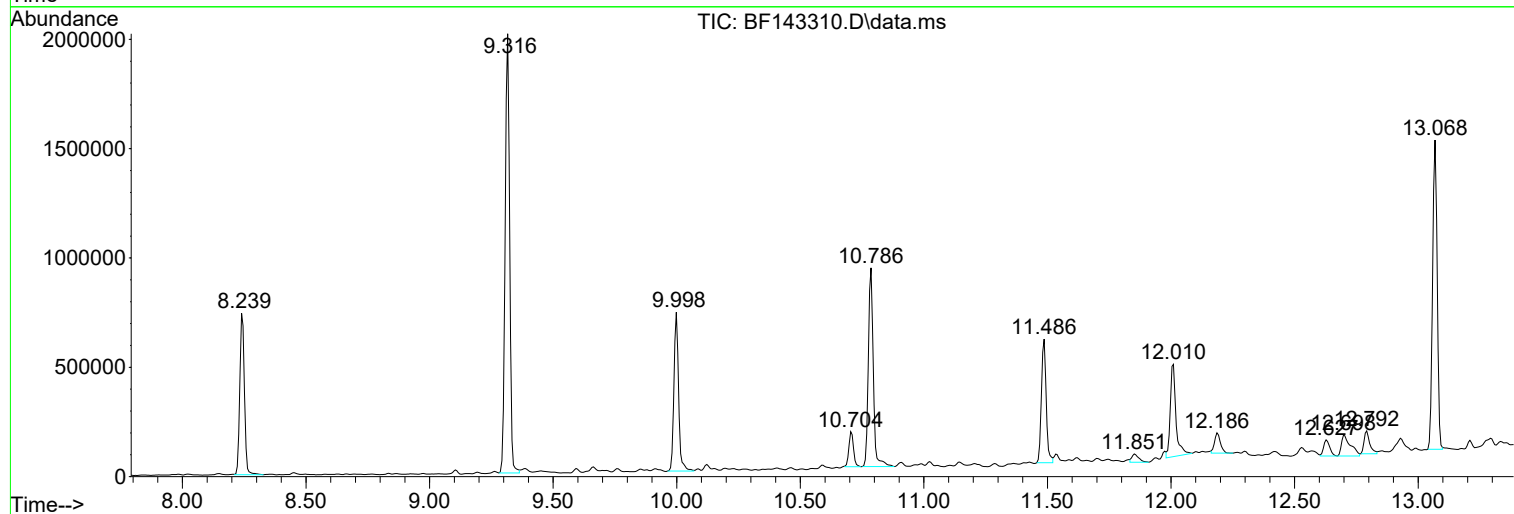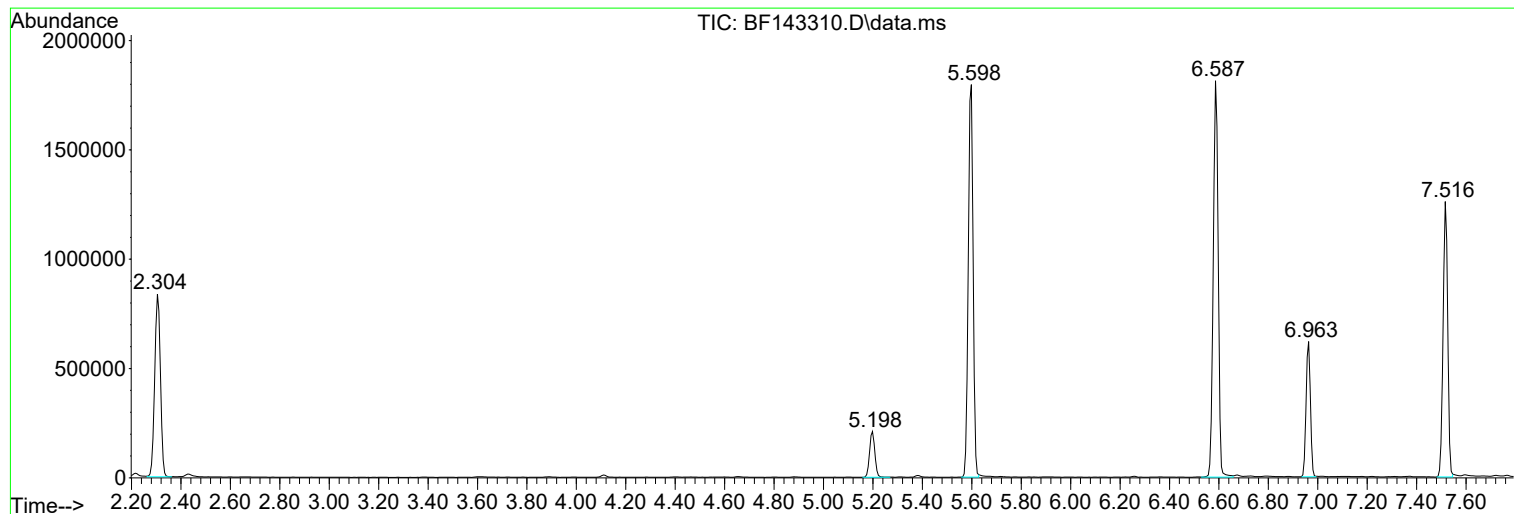

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143310.D
Acq On : 05 Aug 2025 12:32
Operator : RC/JU
Sample : Q2747-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG4-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143310.D
Acq On : 05 Aug 2025 12:32
Operator : RC/JU
Sample : Q2747-05
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-OG4-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc