

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
 Data File : BF143311.D
 Acq On : 05 Aug 2025 13:01
 Operator : RC/JU
 Sample : Q2747-07
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP01-073125

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143311.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.287	9	16	28	rVB	751718	1206492	38.36%	3.081%
2	5.193	502	510	518	rBV	190642	275487	8.76%	0.703%
3	5.375	537	541	552	rBV	19043	31773	1.01%	0.081%
4	5.593	572	578	596	rBV	1653057	2232348	70.97%	5.700%
5	6.587	737	747	759	rBV	1690067	2302718	73.21%	5.880%
6	6.963	806	811	816	rBV	642433	790781	25.14%	2.019%
7	7.516	899	905	910	rBV	1159690	1496849	47.59%	3.822%
8	8.240	1023	1028	1037	rBV	774276	999362	31.77%	2.552%
9	9.316	1205	1211	1220	rBV	1895781	2409683	76.61%	6.153%
10	9.663	1266	1270	1277	rBV3	18415	32214	1.02%	0.082%
11	9.998	1321	1327	1339	rBV	787997	1027567	32.67%	2.624%
12	10.122	1344	1348	1352	rBV3	19915	31558	1.00%	0.081%
13	10.704	1443	1447	1455	rBV	166767	217993	6.93%	0.557%
14	10.786	1456	1461	1477	rVB	873169	1165148	37.04%	2.975%
15	10.910	1478	1482	1488	rBV6	19927	32761	1.04%	0.084%
16	11.028	1498	1502	1510	rVB3	37927	60972	1.94%	0.156%
17	11.145	1518	1522	1526	rBV3	34301	47538	1.51%	0.121%
18	11.428	1566	1570	1573	rBV	82831	108402	3.45%	0.277%
19	11.486	1574	1580	1586	rVV	615435	862109	27.41%	2.201%
20	11.533	1586	1588	1592	rVB	62450	70955	2.26%	0.181%
21	11.851	1639	1642	1651	rVB4	78801	131320	4.17%	0.335%
22	11.939	1653	1657	1659	rBV	57668	81648	2.60%	0.208%
23	11.975	1660	1663	1665	rVV	69335	91178	2.90%	0.233%
24	12.010	1665	1669	1682	rVB	701429	1032163	32.81%	2.635%
25	12.186	1695	1699	1708	rVB2	208734	345533	10.99%	0.882%
26	12.263	1709	1712	1715	rBV2	44677	60324	1.92%	0.154%
27	12.628	1770	1774	1782	rVB2	136273	212507	6.76%	0.543%
28	12.704	1782	1787	1798	rBV2	205148	561598	17.85%	1.434%
29	12.792	1798	1802	1810	rBV	181744	276314	8.78%	0.706%
30	13.069	1844	1849	1855	rBV	1343166	1720635	54.70%	4.393%
31	13.210	1870	1873	1876	rBV	62692	76311	2.43%	0.195%
32	13.963	1997	2001	2007	rVB2	289072	424700	13.50%	1.084%
33	14.127	2024	2029	2041	rVB2	979978	2307349	73.36%	5.891%
34	14.592	2104	2108	2114	rVB2	390055	600908	19.10%	1.534%
35	14.986	2172	2175	2183	rVB	359152	505519	16.07%	1.291%
36	15.263	2217	2222	2233	rVB	824460	1391096	44.23%	3.552%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143311.D
Acq On : 05 Aug 2025 13:01
Operator : RC/JU
Sample : Q2747-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.639	2281	2286	2303	rVB	345710	679077	21.59%	1.734%
38	16.010	2345	2349	2362	rVB2	210209	434338	13.81%	1.109%
39	16.121	2363	2368	2374	rVV	579352	970504	30.85%	2.478%
40	16.410	2412	2417	2430	rVB	367361	868013	27.60%	2.216%
41	17.574	2609	2615	2624	rVB4	237541	630827	20.06%	1.611%
42	17.845	2652	2661	2663	rBV2	751013	1901305	60.45%	4.855%
43	18.333	2736	2744	2756	rBV	804719	3145446	100.00%	8.031%
44	18.445	2758	2763	2775	rVB6	660788	2032432	64.62%	5.189%
45	18.709	2798	2808	2812	rBV2	694510	2266930	72.07%	5.788%
46	18.862	2828	2834	2841	rBV2	418672	1014194	32.24%	2.590%




Sum of corrected areas: 39164879

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143311.D
Acq On : 05 Aug 2025 13:01
Operator : RC/JU
Sample : Q2747-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

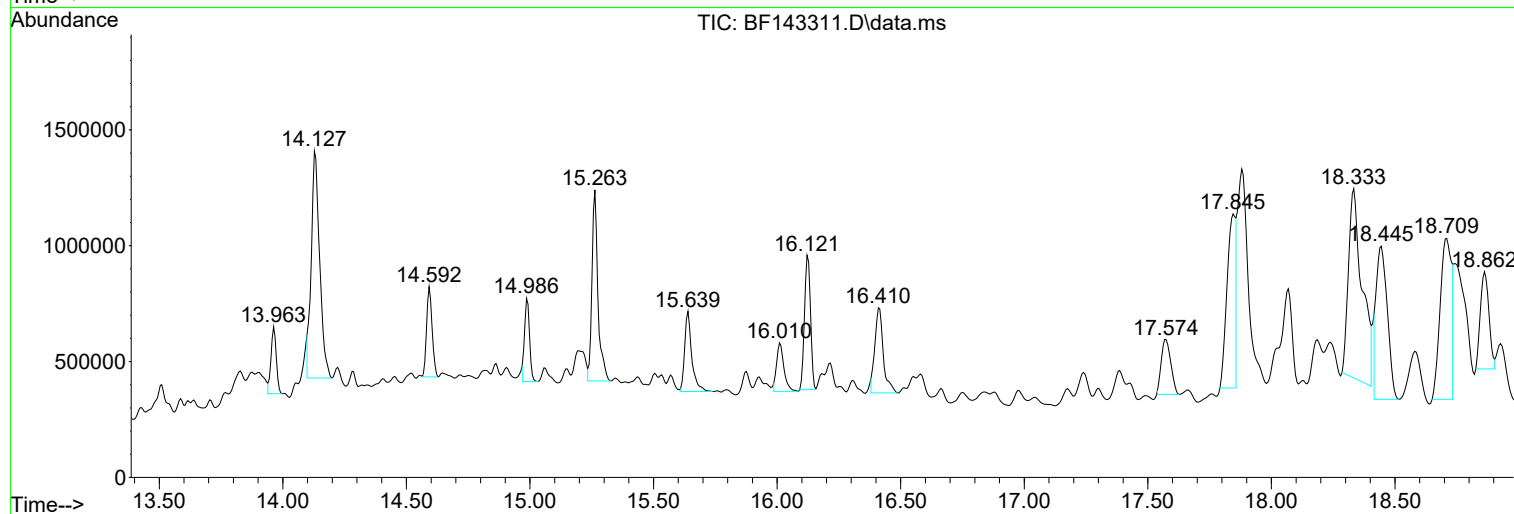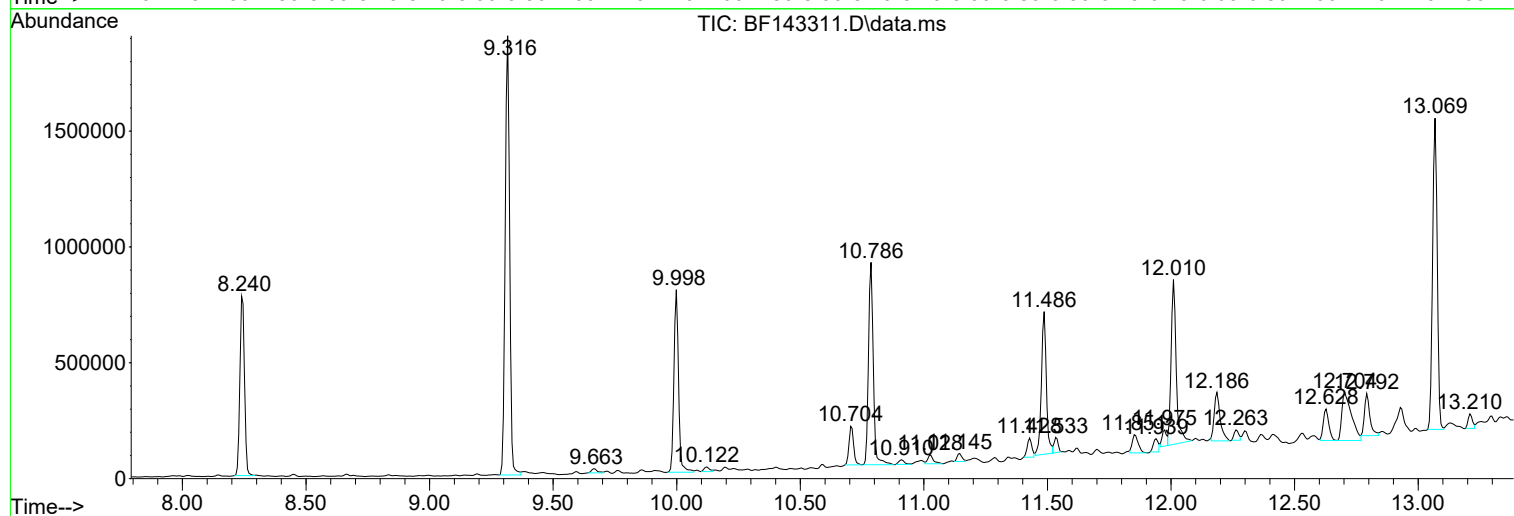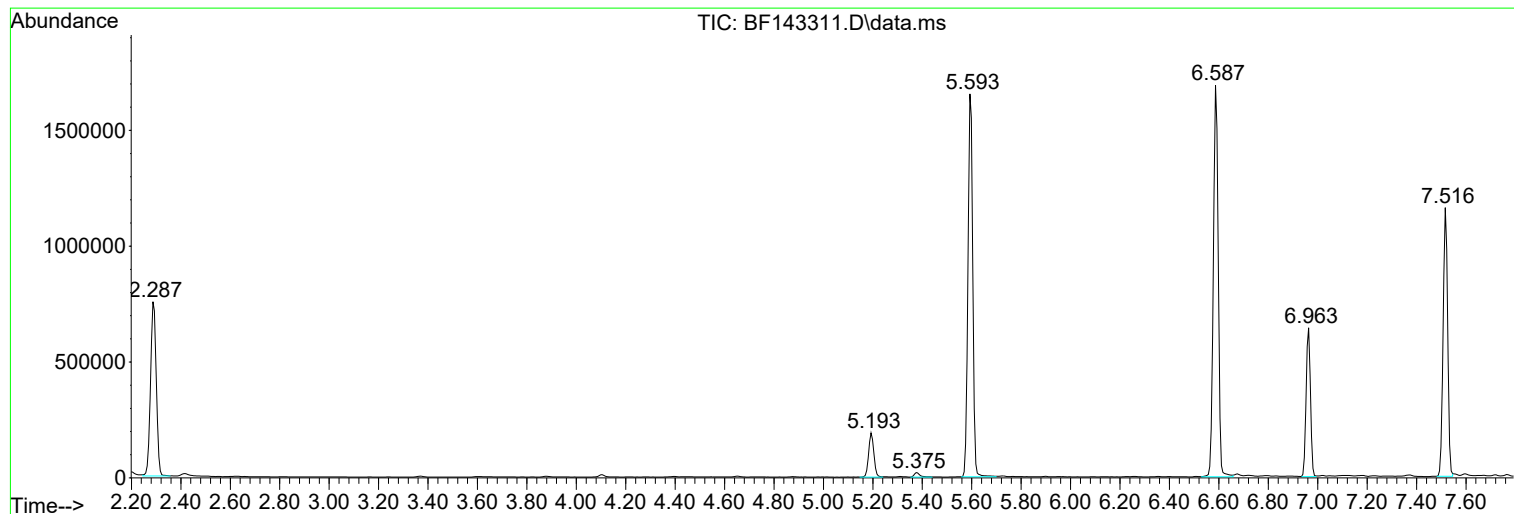

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143311.D
Acq On : 05 Aug 2025 13:01
Operator : RC/JU
Sample : Q2747-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143311.D
Acq On : 05 Aug 2025 13:01
Operator : RC/JU
Sample : Q2747-07
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP01-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------