

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
 Data File : BF143312.D
 Acq On : 05 Aug 2025 13:30
 Operator : RC/JU
 Sample : Q2747-09
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-TS-GRILLO-TSCP02-073125

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF143312.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.293	10	17	32	rVB	819380	1324739	44.05%	3.465%
2	5.199	502	511	518	rBV	200530	301247	10.02%	0.788%
3	5.598	573	579	584	rBV	1795905	2376479	79.03%	6.216%
4	6.593	738	748	753	rBV	1769906	2423572	80.59%	6.339%
5	6.963	806	811	816	rBV	644445	780742	25.96%	2.042%
6	7.516	899	905	911	rBV	1209895	1611067	53.57%	4.214%
7	8.245	1023	1029	1036	rBV	749635	976264	32.46%	2.553%
8	9.316	1205	1211	1216	rBV	2029139	2536966	84.36%	6.635%
9	9.663	1266	1270	1276	rBV3	20703	31119	1.03%	0.081%
10	9.998	1322	1327	1339	rBV	733764	950511	31.61%	2.486%
11	10.122	1344	1348	1352	rBV2	20029	32295	1.07%	0.084%
12	10.710	1443	1448	1456	rBV	150841	204417	6.80%	0.535%
13	10.786	1456	1461	1477	rVV	930813	1236418	41.12%	3.234%
14	10.910	1478	1482	1489	rVB7	18479	34219	1.14%	0.090%
15	11.022	1498	1501	1506	rVB3	33784	45411	1.51%	0.119%
16	11.145	1518	1522	1527	rBV	36609	51933	1.73%	0.136%
17	11.428	1566	1570	1574	rBV	98002	139304	4.63%	0.364%
18	11.486	1574	1580	1586	rVV	600841	842399	28.01%	2.203%
19	11.533	1586	1588	1592	rVB	68248	84108	2.80%	0.220%
20	11.851	1639	1642	1651	rVB3	70162	127020	4.22%	0.332%
21	11.939	1653	1657	1659	rBV	63756	88642	2.95%	0.232%
22	11.975	1659	1663	1665	rVV	90229	119076	3.96%	0.311%
23	12.010	1665	1669	1682	rVB	732966	1099817	36.57%	2.877%
24	12.186	1695	1699	1709	rBV3	224303	402770	13.39%	1.053%
25	12.627	1770	1774	1782	rVB	137419	214096	7.12%	0.560%
26	12.704	1782	1787	1798	rBV2	219213	552191	18.36%	1.444%
27	12.792	1798	1802	1810	rBV	173798	276348	9.19%	0.723%
28	12.933	1823	1826	1833	rVB	120050	177517	5.90%	0.464%
29	13.069	1844	1849	1855	rBV	1442048	1858180	61.79%	4.860%
30	13.963	1998	2001	2007	rVB3	319296	467221	15.54%	1.222%
31	14.133	2025	2030	2043	rVB3	997277	3007198	100.00%	7.865%
32	14.592	2104	2108	2114	rVB2	435235	679601	22.60%	1.778%
33	14.986	2172	2175	2183	rVB	317804	461040	15.33%	1.206%
34	15.263	2217	2222	2233	rVB	945395	1585940	52.74%	4.148%
35	15.639	2282	2286	2303	rVB	331498	698740	23.24%	1.828%
36	16.010	2346	2349	2358	rVB	205712	392763	13.06%	1.027%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143312.D
Acq On : 05 Aug 2025 13:30
Operator : RC/JU
Sample : Q2747-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	16.127	2363	2369	2374	rBV	628008	1078008	35.85%	2.820%
38	16.415	2413	2418	2431	rVB	328547	713681	23.73%	1.867%
39	17.574	2610	2615	2624	rVB3	213784	547623	18.21%	1.432%
40	17.845	2652	2661	2663	rBV2	674762	1731448	57.58%	4.529%
41	18.068	2694	2699	2706	rVB	377212	854580	28.42%	2.235%
42	18.327	2736	2743	2756	rBV	693825	2326703	77.37%	6.086%
43	18.709	2799	2808	2813	rBV2	575602	1985812	66.04%	5.194%
44	18.862	2828	2834	2841	rBV2	331531	804174	26.74%	2.103%




Sum of corrected areas: 38233399

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143312.D
Acq On : 05 Aug 2025 13:30
Operator : RC/JU
Sample : Q2747-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

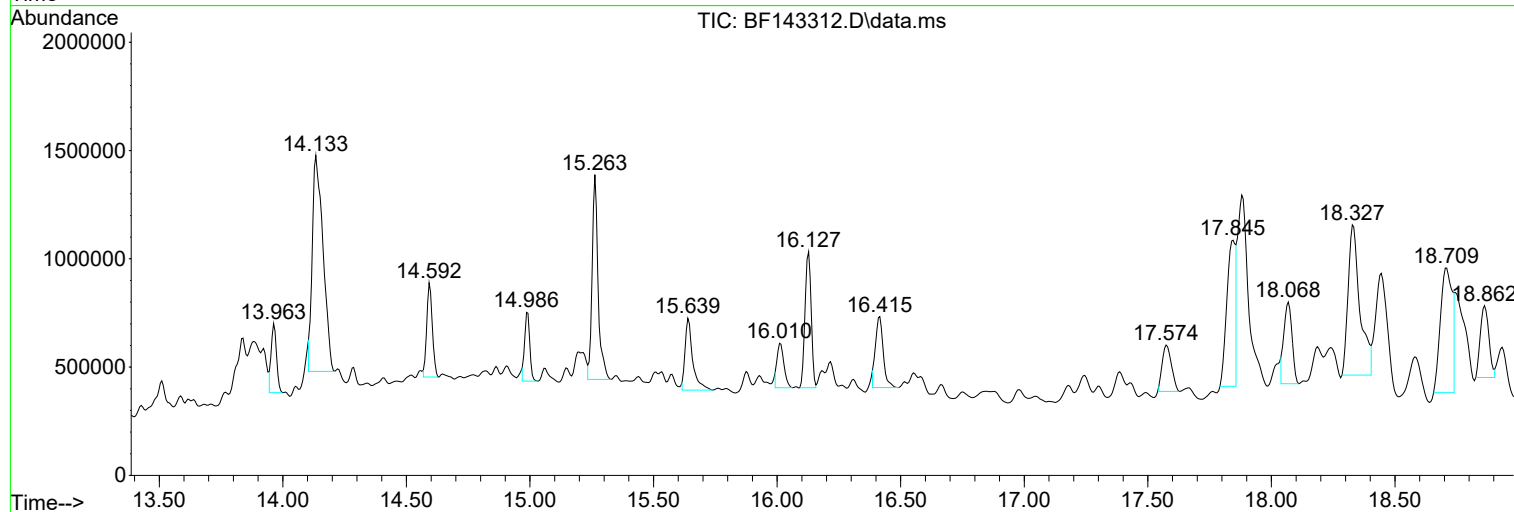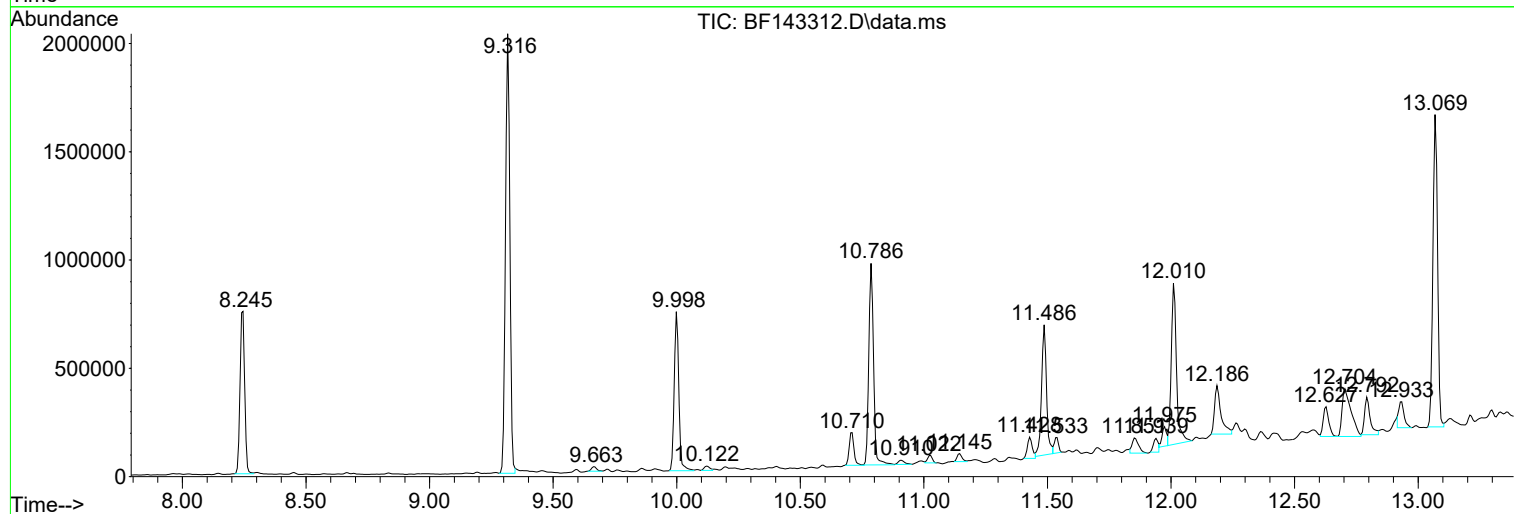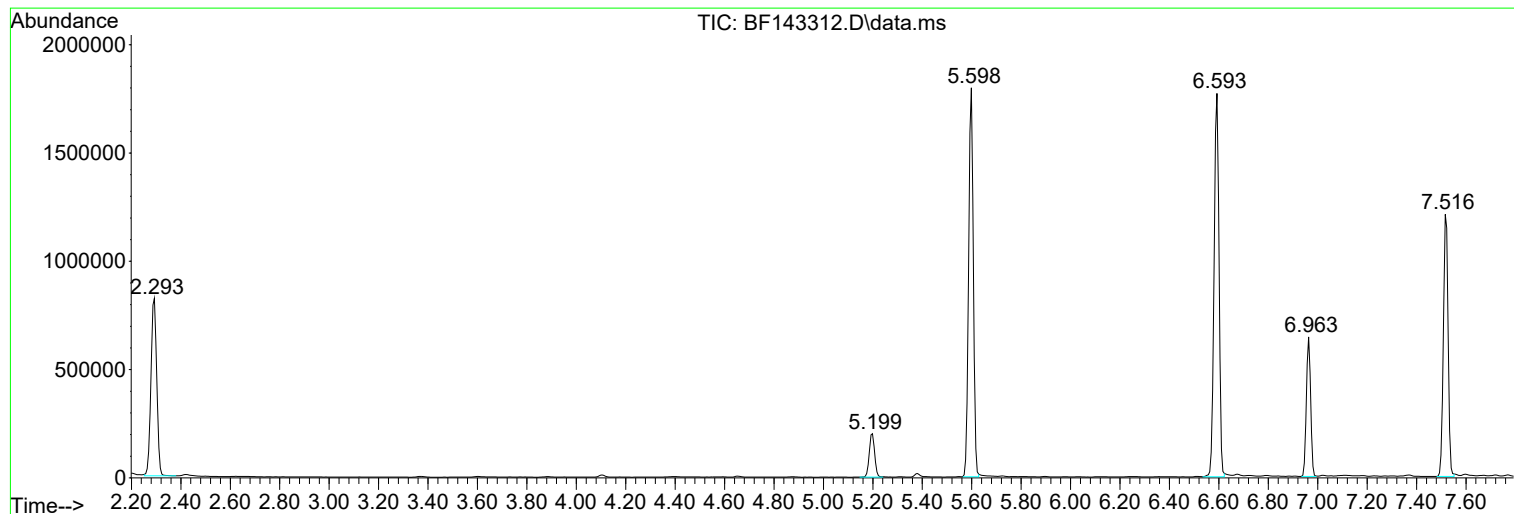

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143312.D
Acq On : 05 Aug 2025 13:30
Operator : RC/JU
Sample : Q2747-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143312.D
Acq On : 05 Aug 2025 13:30
Operator : RC/JU
Sample : Q2747-09
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-TS-GRILLO-TSCP02-073125

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc