
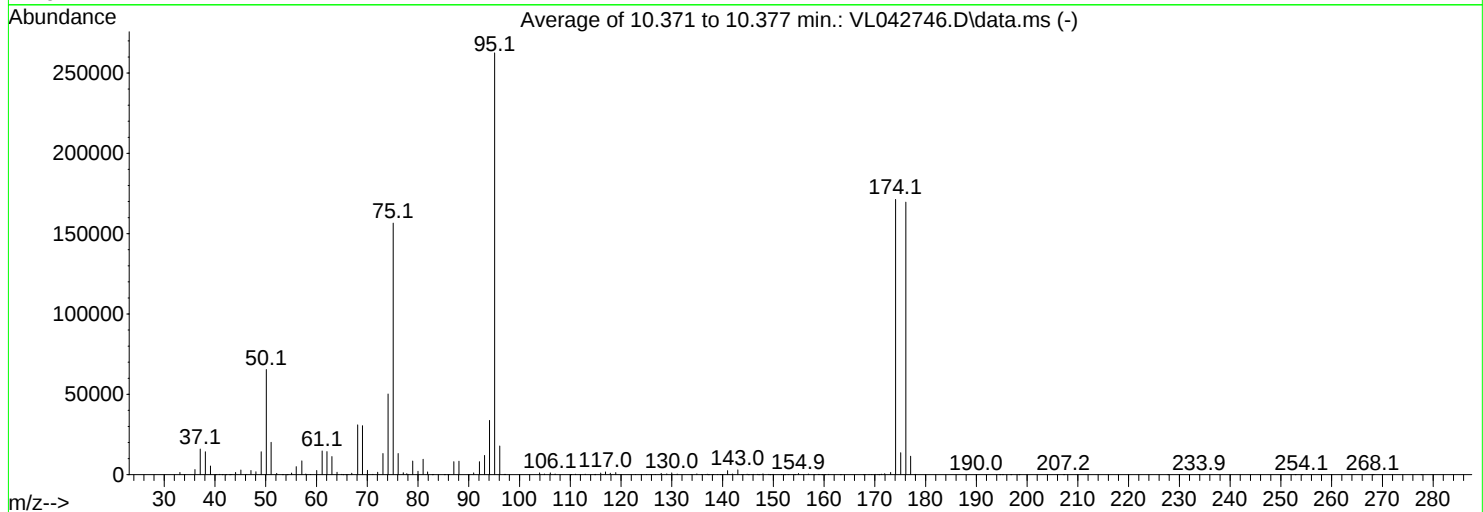


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL072325\
Data File : VL042746.D
Acq On : 23 Jul 2025 08:00
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 24 05:24:41 2025

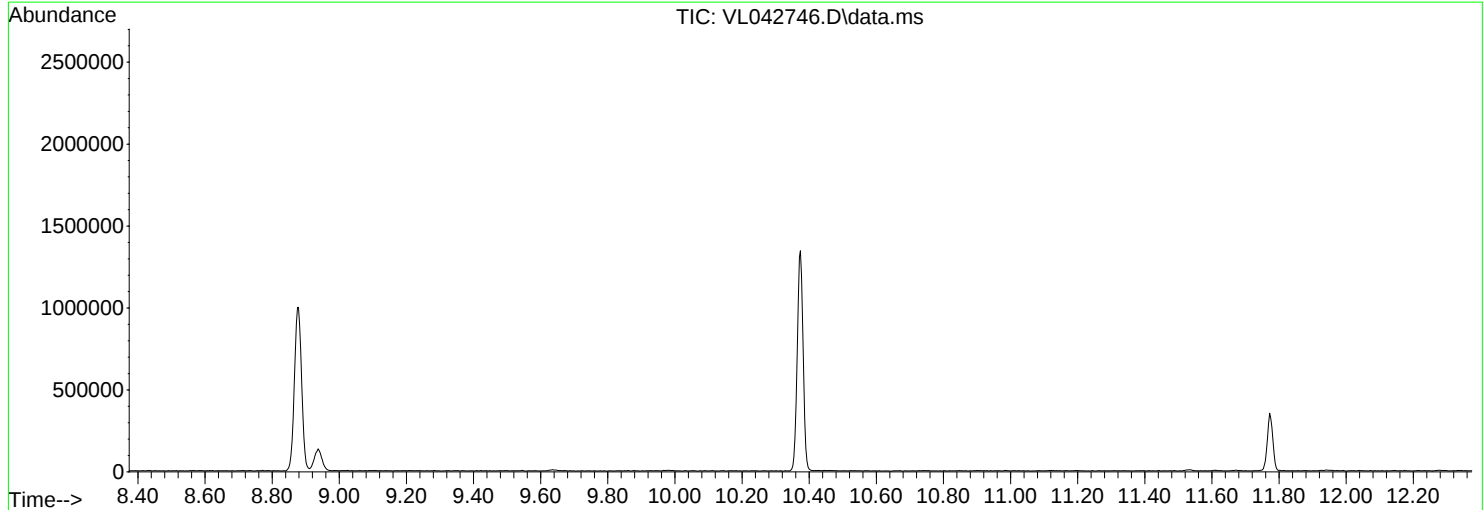

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3150

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.9	65392	PASS
75	95	30	66	59.7	156629	PASS
95	95	100	100	100.0	262571	PASS
96	95	5	9	6.8	17820	PASS
173	174	0.00	2	0.8	1428	PASS
174	95	50	120	65.3	171349	PASS
175	174	4	9	8.0	13693	PASS
176	174	93	101	99.0	169621	PASS
177	176	5	9	6.7	11431	PASS

Average of 10.371 to 10.377 min.: VL042746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1369	43.30	125	54.20	18	64.05	154
33.90	43	44.05	1422	55.10	1040	64.95	18
36.05	3236	45.10	2895	56.00	5005	65.20	5
37.10	15944	46.10	249	57.10	8550	65.80	5
38.10	14231	47.10	2650	57.90	360	66.20	110
39.10	5435	48.05	1854	58.10	92	66.95	924
40.05	14	49.10	14225	58.80	138	68.10	30979
40.95	190	50.10	65392	60.05	2548	69.05	30510
41.40	38	51.05	20174	61.10	14709	70.05	2713
42.10	41	52.15	765	62.05	14328	71.10	169
42.90	56	53.30	34	63.05	11233	72.05	1474

Average of 10.371 to 10.377 min.: VL042746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
73.10	13120	82.80	40	94.10	33749	111.05	341
74.10	50187	83.10	154	95.10	262571	111.95	142
75.10	156629	85.20	20	96.10	17820	112.95	337
76.10	13183	85.90	18	97.00	185	114.80	39
77.10	1177	86.10	78	97.20	167	114.95	193
77.80	567	87.05	8039	103.95	1104	116.00	985
78.00	211	88.05	8386	104.90	399	116.95	1737
78.95	8439	89.90	63	106.05	1080	117.90	929
80.00	2100	90.95	1122	107.00	361	118.95	1287
81.00	9549	92.10	8075	110.00	62	120.00	85
81.90	1728	93.10	11994	110.15	116	122.85	115

Average of 10.371 to 10.377 min.: VL042746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
124.00	81	136.70	128	144.15	116	151.65	87
125.00	90	137.00	342	144.85	278	152.20	43
125.95	131	137.20	40	145.10	42	152.90	73
126.75	97	138.20	64	145.80	133	153.05	134
127.90	806	139.05	122	146.10	219	154.20	58
129.00	544	139.65	92	146.90	194	154.95	716
130.00	1065	139.90	25	147.10	63	156.90	423
131.05	458	141.00	2537	147.95	546	158.00	21
133.80	139	141.95	459	149.10	187	158.90	176
134.95	492	143.00	3049	149.30	59	159.10	74
135.90	71	143.80	65	149.95	225	159.60	21

Average of 10.371 to 10.377 min.: VL042746.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
160.10	38	171.95	628	196.80	35		
160.90	253	173.10	1428	198.40	32		
163.20	57	174.10	171349	207.20	32		
167.80	30	175.10	13693	227.70	17		
168.10	69	176.10	169621	233.90	71		
168.85	148	177.05	11431	252.80	17		
169.40	135	177.90	77	254.10	43		
170.05	234	178.05	216	268.15	59		
170.60	80	190.00	93	277.60	38		
170.80	29	194.60	17				
171.30	280	195.15	44				