
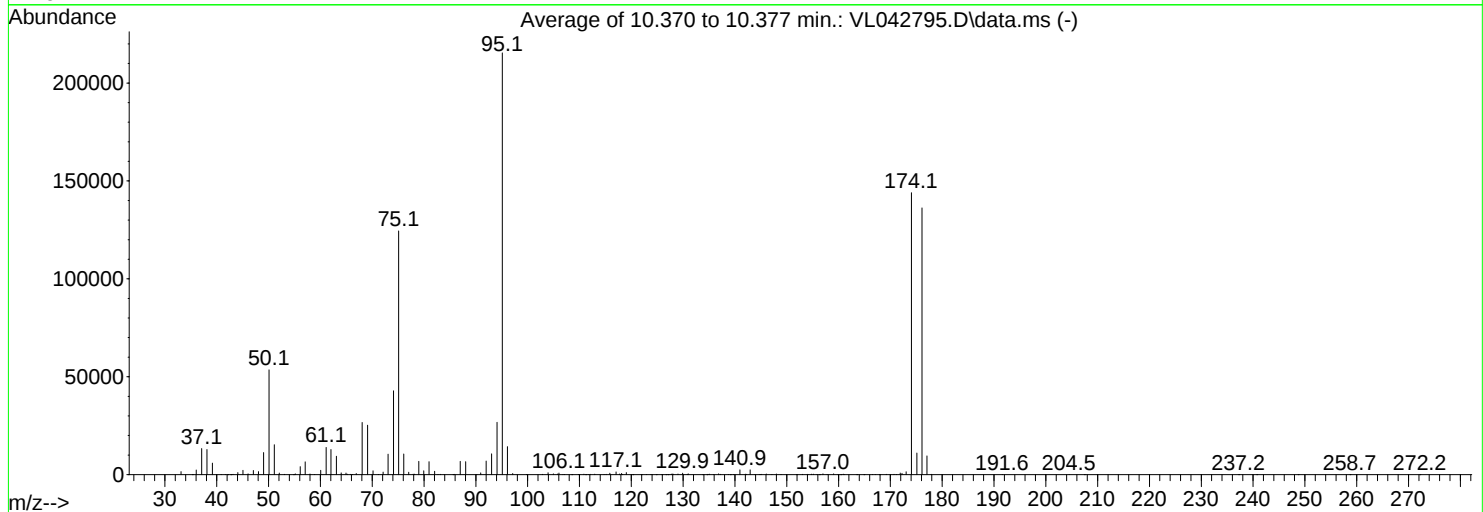


Data Path : Z:\voasrv\HPCHEM1\MSVOA_L\Data\VL080425\
Data File : VL042795.D
Acq On : 04 Aug 2025 07:40
Operator : SY/MD
Sample : BFB
Misc : 400mL/MSVOA_L
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_L
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_L\methods\VL072325AIR.M
Title : AIR ANALYSIS BY METHOD TO-15 Instrument: MSVOA_L Fri Aug 26 06:05:16 2022
Last Update : Thu Jul 24 05:24:41 2025

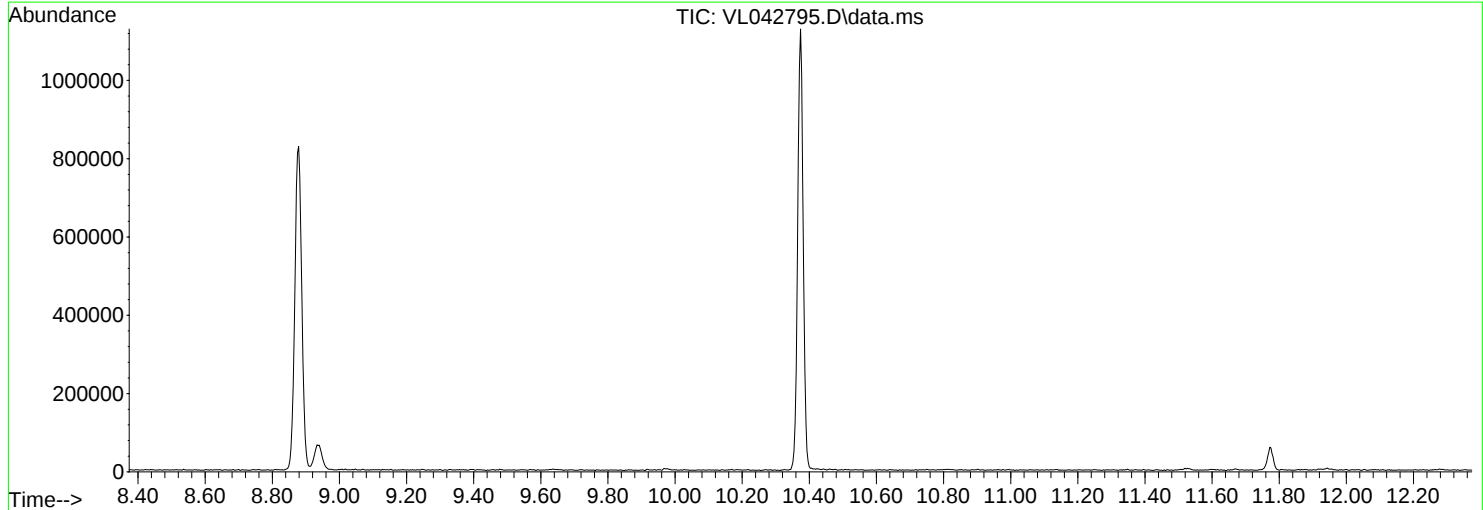

AutoFind: Scans 3177, 3178, 3179; Background Corrected with Scan 3147

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	8	40	24.8	53528	PASS
75	95	30	66	57.8	124445	PASS
95	95	100	100	100.0	215424	PASS
96	95	5	9	6.6	14276	PASS
173	174	0.00	2	1.0	1500	PASS
174	95	50	120	66.8	143979	PASS
175	174	4	9	7.7	11033	PASS
176	174	93	101	94.6	136259	PASS
177	176	5	9	7.0	9581	PASS

Average of 10.370 to 10.377 min.: VL042795.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
33.10	1572	43.15	156	54.80	14	64.95	83
35.30	33	44.05	1074	55.15	386	65.20	22
36.05	2386	45.05	2223	56.10	4054	65.85	19
37.10	13298	46.05	412	57.05	6521	66.20	11
38.10	12800	47.05	2115	58.00	343	66.90	557
39.15	5855	48.05	1522	58.90	71	68.05	26611
40.85	109	49.05	11253	60.05	2240	69.10	25293
41.65	56	50.10	53528	61.10	13909	70.15	1957
42.10	21	51.10	15327	62.05	12871	71.20	72
42.70	31	52.05	811	63.10	9409	72.10	1290
42.90	63	53.05	193	64.00	892	73.05	10460

Average of 10.370 to 10.377 min.: VL042795.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
74.10	42840	83.15	136	95.10	215424	108.50	41
75.10	124445	83.90	77	96.10	14276	109.80	62
76.10	10555	85.60	19	97.10	572	110.05	107
77.05	1271	85.80	181	99.80	63	110.85	245
77.90	265	87.00	6774	102.85	176	111.20	44
78.20	231	88.05	6627	103.95	986	111.70	58
79.00	6821	90.20	107	104.95	434	112.05	205
79.95	1966	90.95	890	105.80	312	112.95	287
80.95	6609	92.00	6938	106.05	799	114.75	106
82.05	1714	93.05	10643	106.80	92	115.15	200
82.70	53	94.10	26720	107.10	105	115.85	722

Average of 10.370 to 10.377 min.: VL042795.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
117.05	1439	125.90	41	134.60	42	142.20	148
117.75	305	126.70	20	134.80	164	142.95	2434
118.10	607	127.10	27	135.05	263	143.85	87
118.30	180	127.70	261	135.90	91	144.70	84
119.05	1068	127.90	334	136.85	382	144.90	82
120.30	35	128.10	234	137.20	136	145.10	163
121.90	34	129.00	372	138.75	62	146.05	346
122.95	74	129.90	730	139.10	46	147.15	112
123.80	52	130.80	136	139.75	107	148.00	375
124.00	55	131.00	412	140.95	2483	148.90	72
124.80	17	133.80	36	142.00	256	149.95	125

Average of 10.370 to 10.377 min.: VL042795.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
151.90	37	160.40	30	171.20	104	207.45	40
153.05	140	160.90	230	171.90	829	237.20	22
154.05	128	161.10	92	172.25	660	240.70	18
154.75	273	163.50	22	173.05	1500	248.70	17
155.15	269	164.90	36	174.05	143979	258.70	37
155.85	76	166.55	48	175.10	11033	272.20	39
156.30	19	167.10	67	176.10	136259		
157.00	400	167.90	27	177.05	9581		
157.80	104	169.20	180	177.90	207		
159.05	382	170.00	62	191.60	58		
159.90	17	170.70	146	204.50	68		