
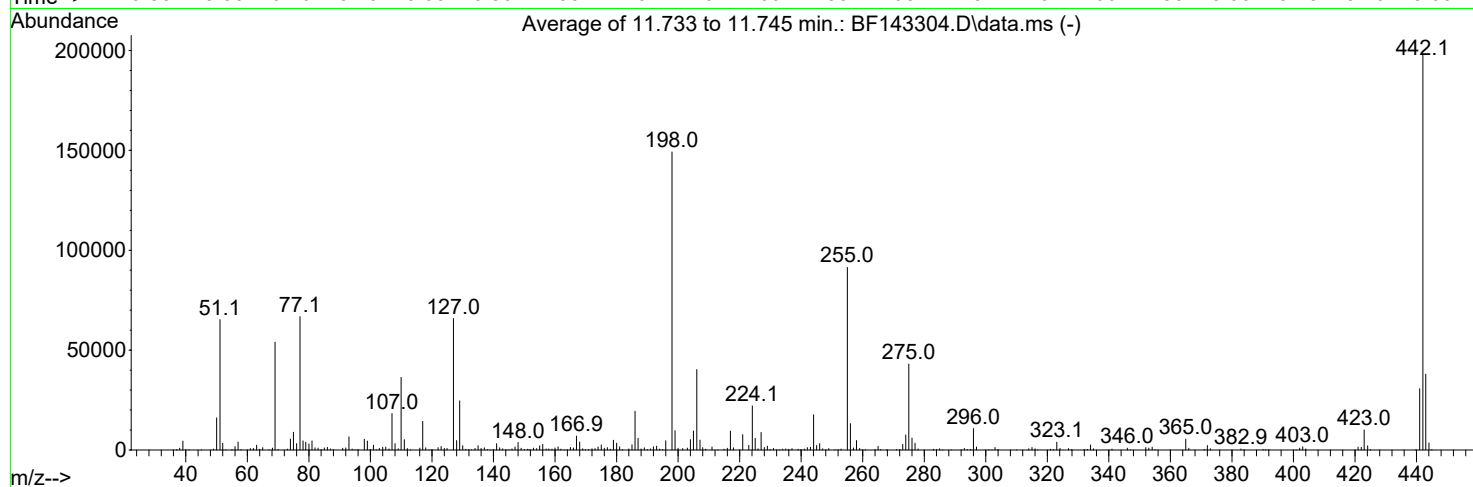


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143304.D
Acq On : 05 Aug 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

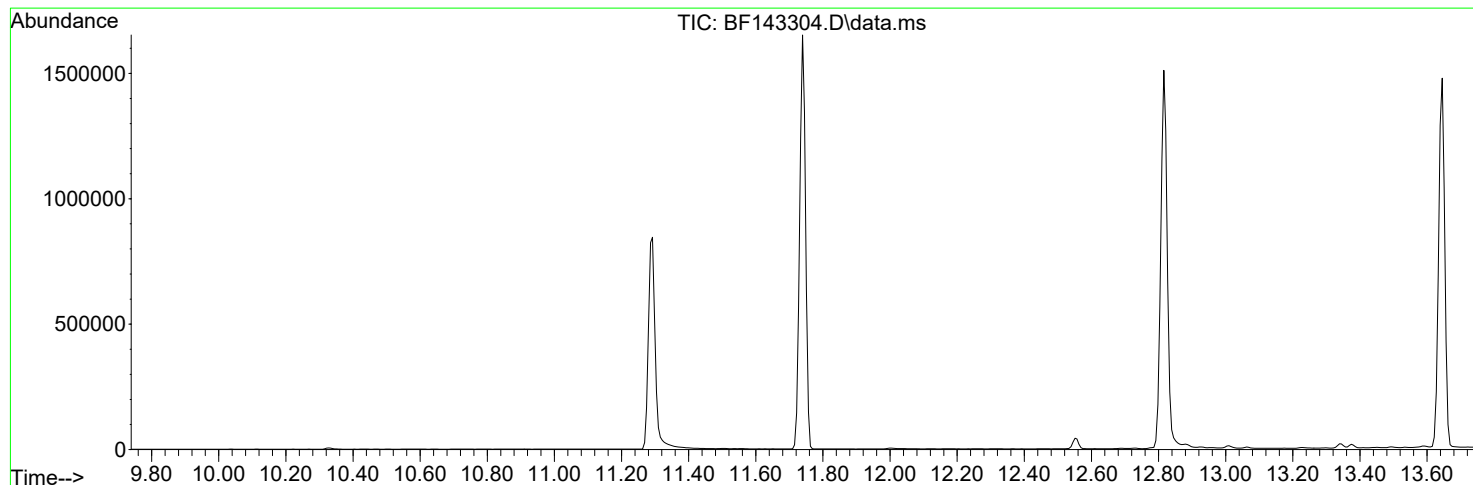

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	990	PASS
69	69	100	100	100.0	54003	PASS
70	69	0.00	2	0.6	308	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	149269	PASS
199	198	5	9	6.5	9674	PASS
365	198	1	100	3.6	5435	PASS
441	443	0.01	150	80.9	30712	PASS
442	442	100	100	100.0	197653	PASS
443	442	15	24	19.2	37949	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/5/2025	BNA_F	<u>BF143304.D</u>
Compound Name	Response	Retention Time
DDT	370669	13.645
DDD	8918	13.345
DDE	3130	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12048	382717	3.15

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143304.D
Acq On : 05 Aug 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 10:59:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

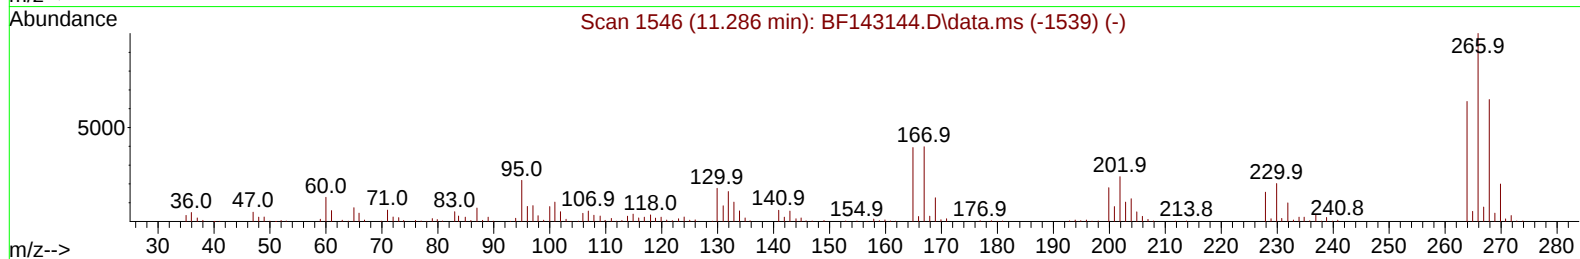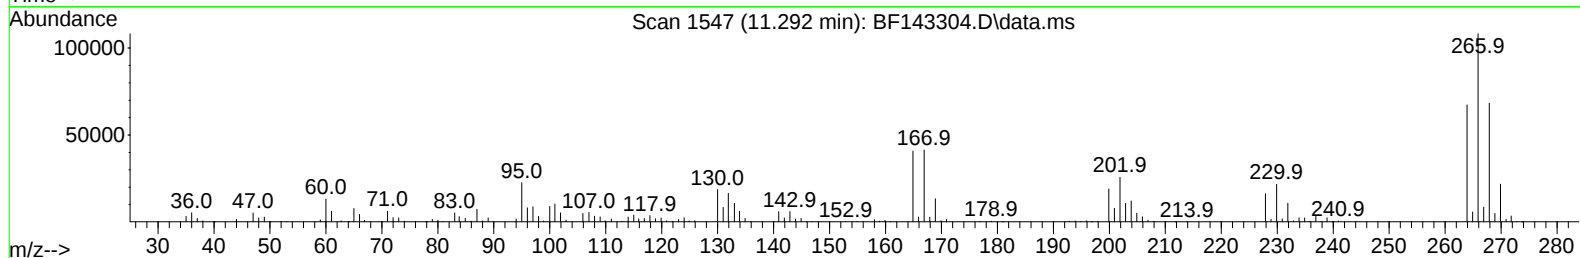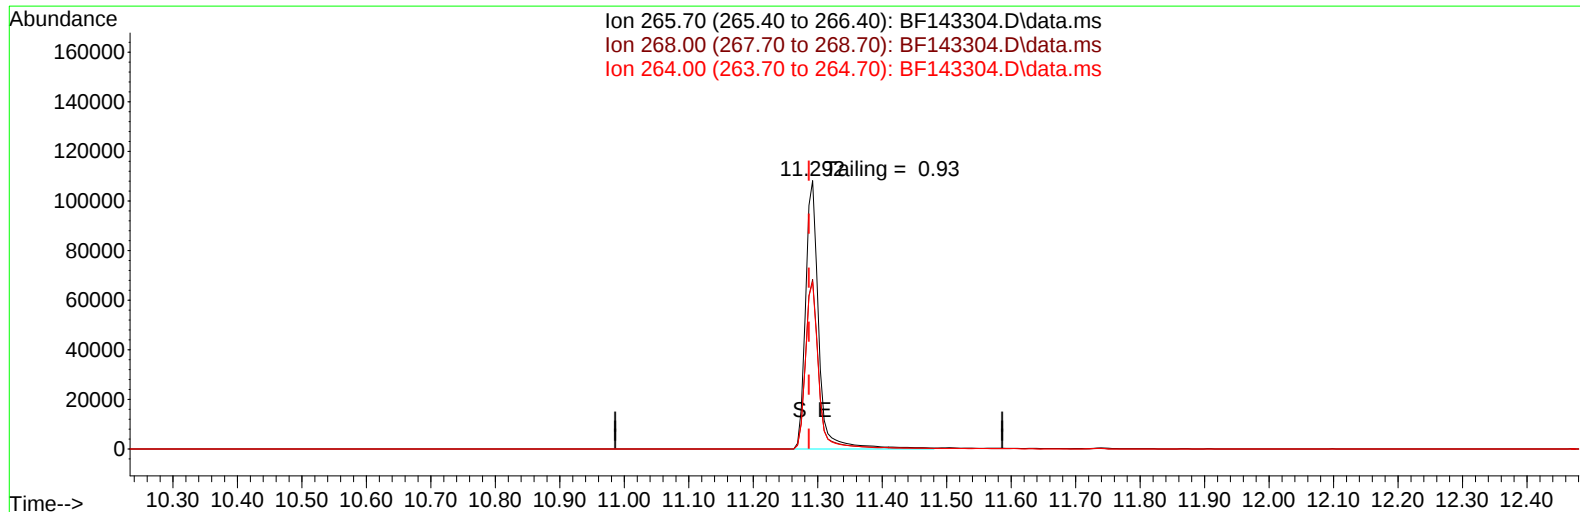

TIC: BF143304.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.006) 26944.60 ng




response 154742

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	63.16
264.00	63.80	62.23
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080525\
Data File : BF143304.D
Acq On : 05 Aug 2025 09:02
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 05 10:59:37 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

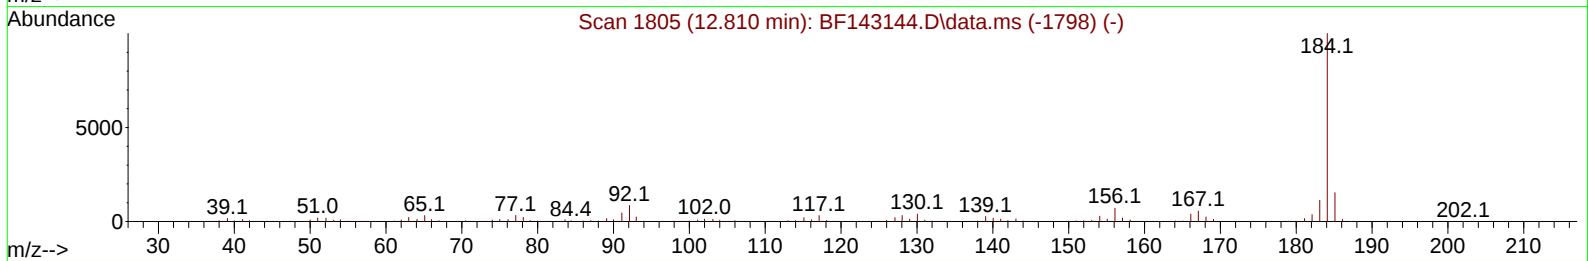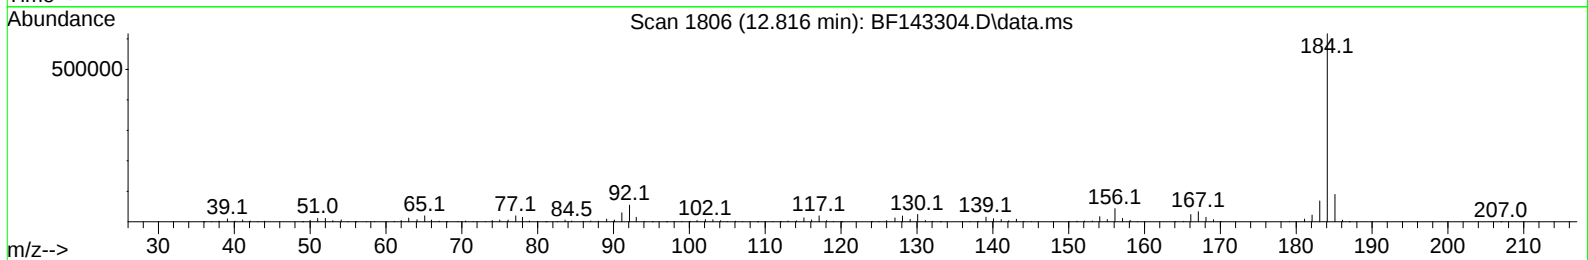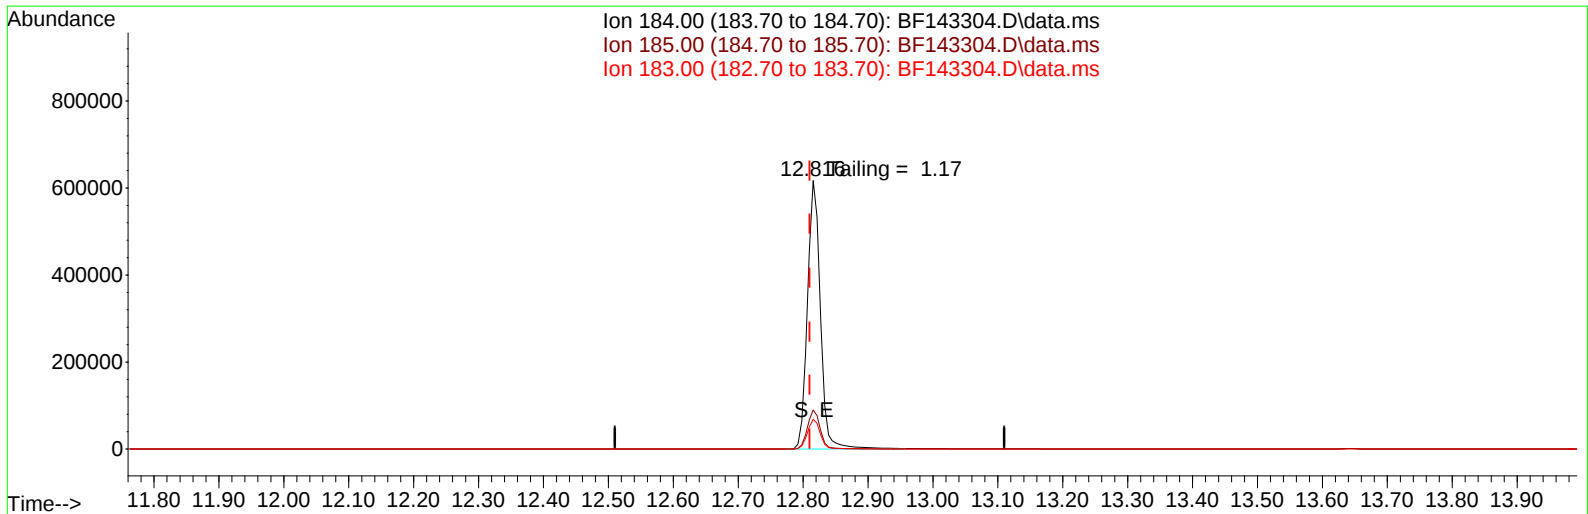

TIC: BF143304.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 856718

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.56
183.00	11.20	11.12
0.00	0.00	0.00