
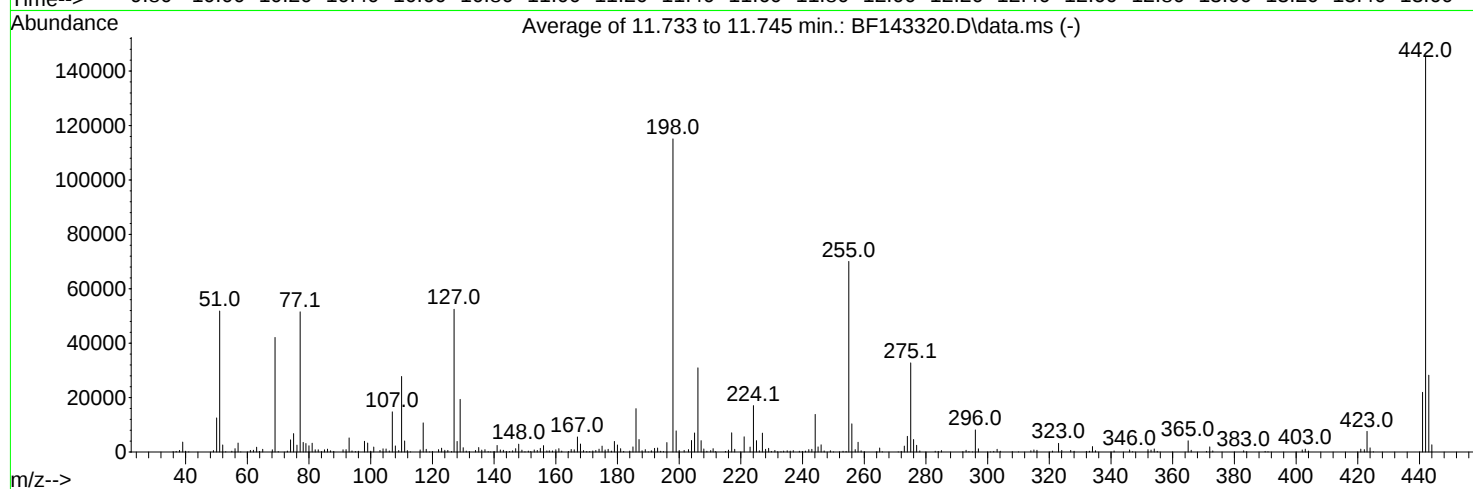


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080625\
Data File : BF143320.D
Acq On : 06 Aug 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 17 15:14:05 2025

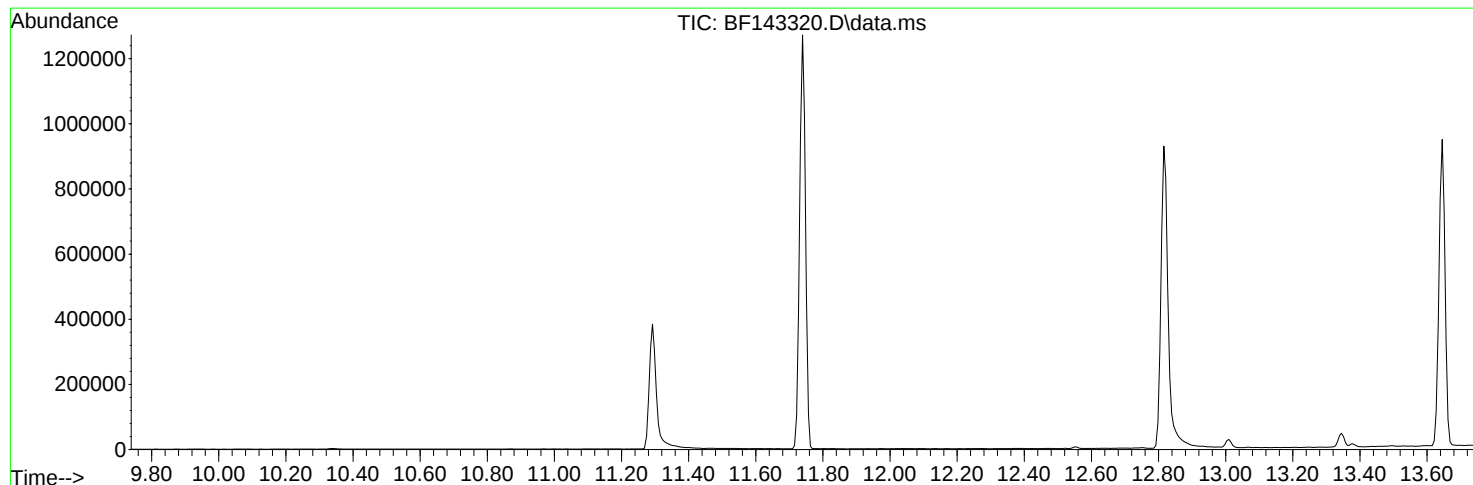

AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	818	PASS
69	69	100	100	100.0	42139	PASS
70	69	0.00	2	0.4	187	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	115091	PASS
199	198	5	9	6.7	7756	PASS
365	198	1	100	3.6	4108	PASS
441	443	0.01	150	77.6	21928	PASS
442	442	100	100	100.0	145123	PASS
443	442	15	24	19.5	28240	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/6/2025	BNA_F	<u>BF143320.D</u>
Compound Name	Response	Retention Time
DDT	235820	13.645
DDD	14159	13.345
DDE	4954	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
19113	254933	7.50

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080625\
Data File : BF143320.D
Acq On : 06 Aug 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 06 10:49:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

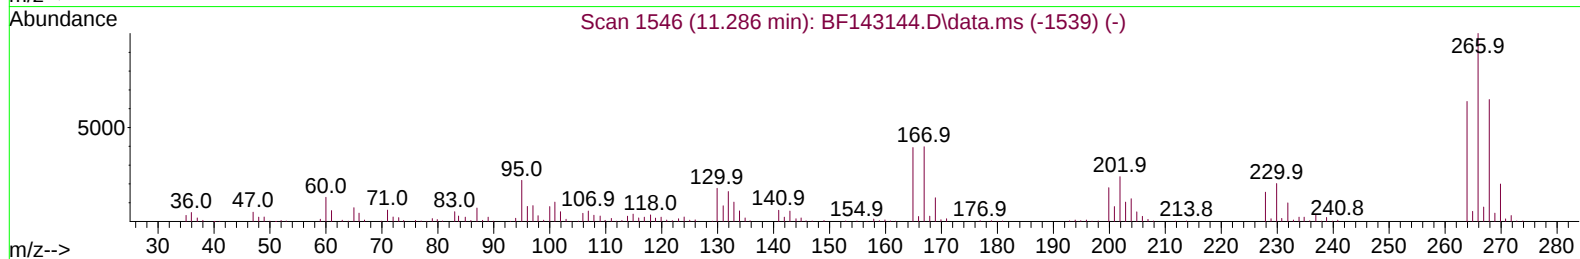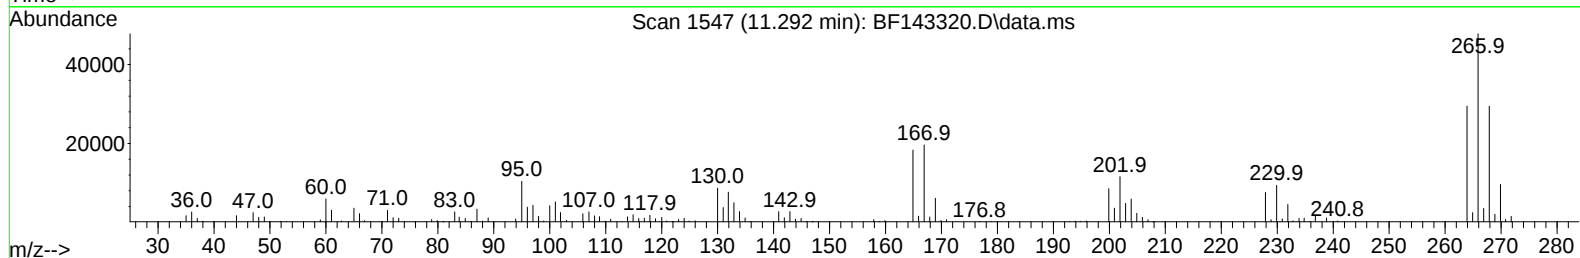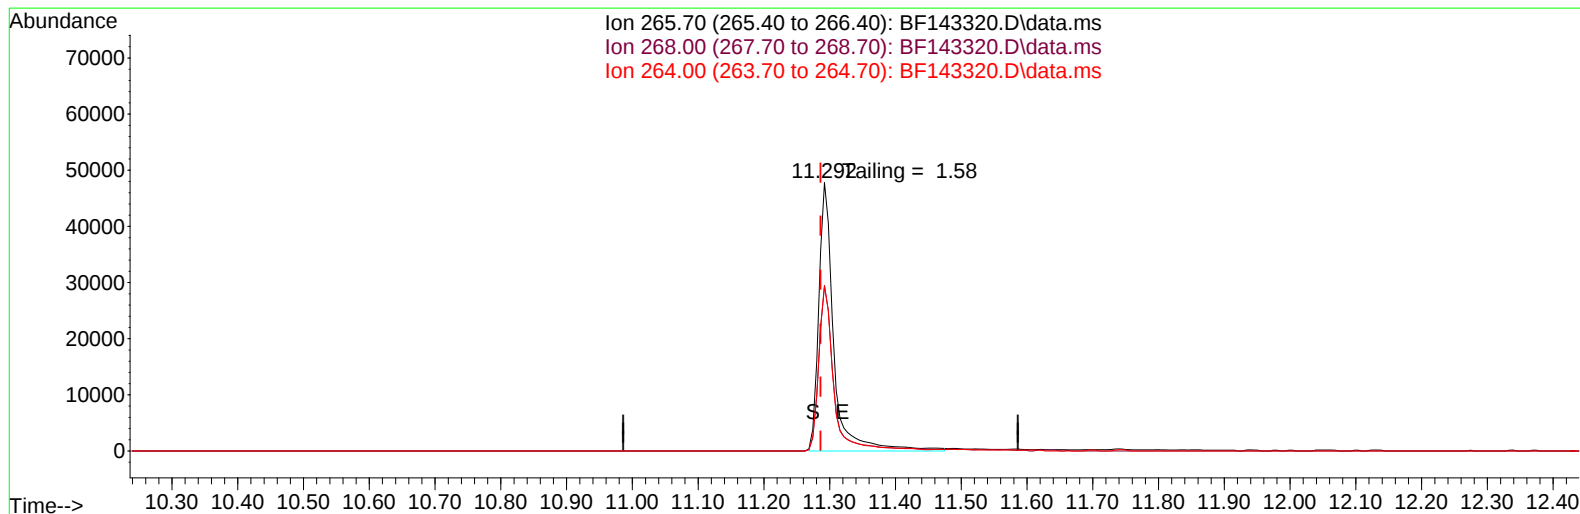

TIC: BF143320.D\data.ms

(70) Pentachlorophenol (C)

11.292min (+ 0.006) 15325.61 ng




response 75441

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.90	61.54
264.00	63.80	61.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080625\
Data File : BF143320.D
Acq On : 06 Aug 2025 09:39
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 06 10:49:49 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF071725.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 17 15:14:05 2025
Response via : Initial Calibration

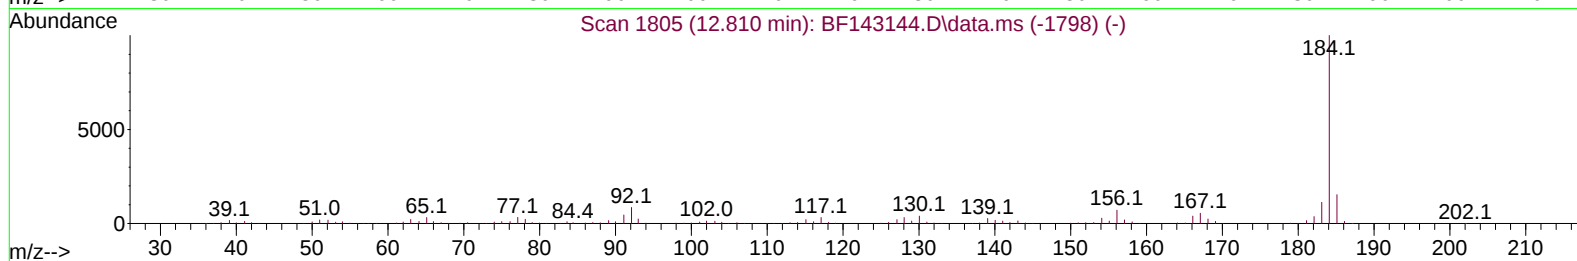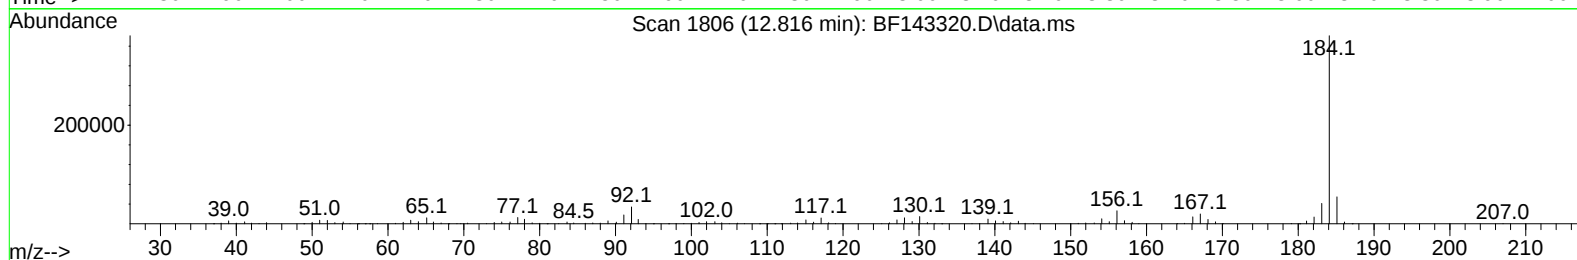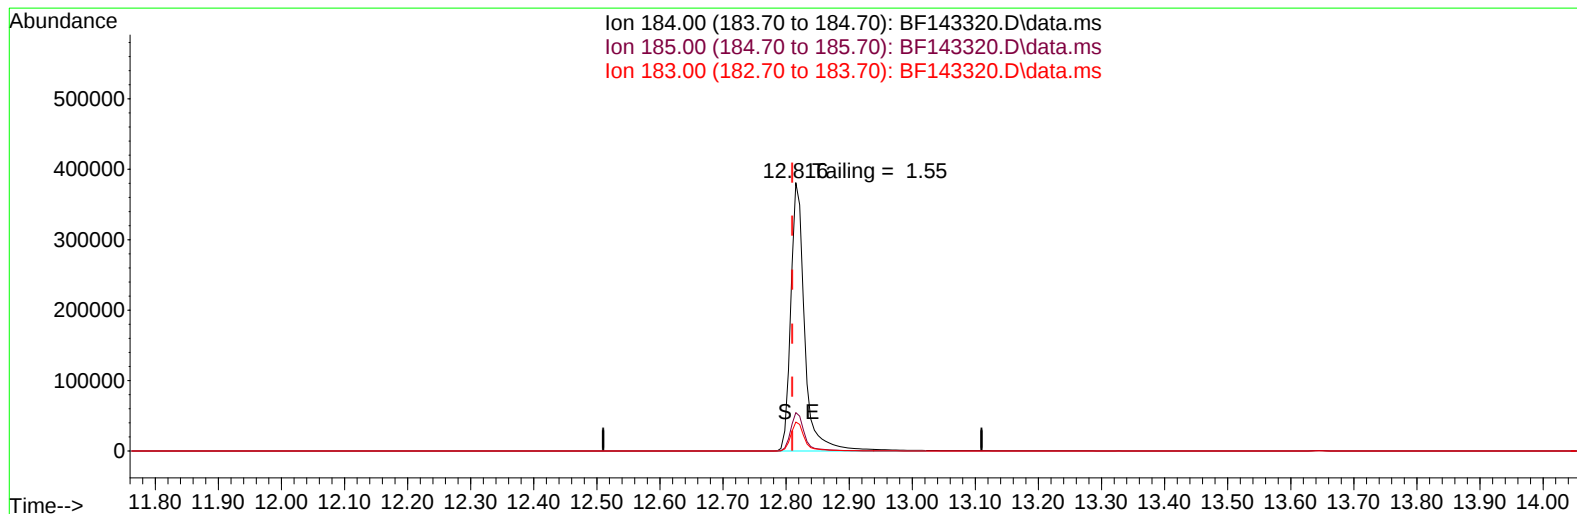

TIC: BF143320.D\data.ms

(77) Benzidine

12.816min (+ 0.006) 0.00 ng

response 588438

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.32
183.00	11.20	10.83
0.00	0.00	0.00