
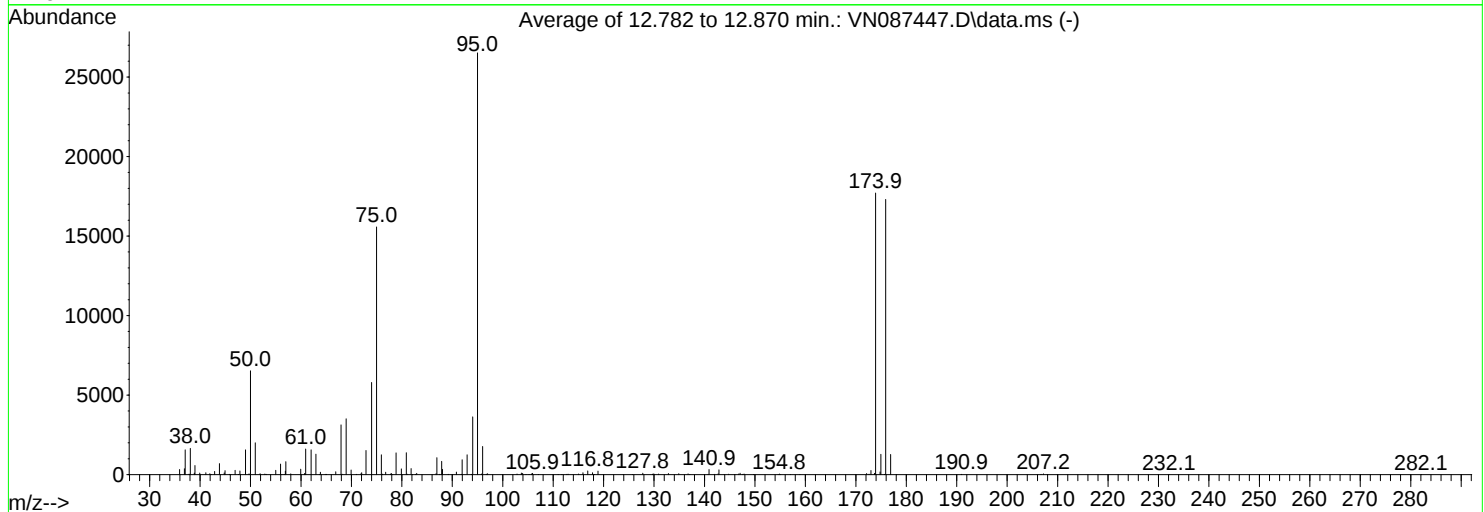


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080525\
Data File : VN087447.D
Acq On : 05 Aug 2025 09:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080525W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 06 02:01:21 2025

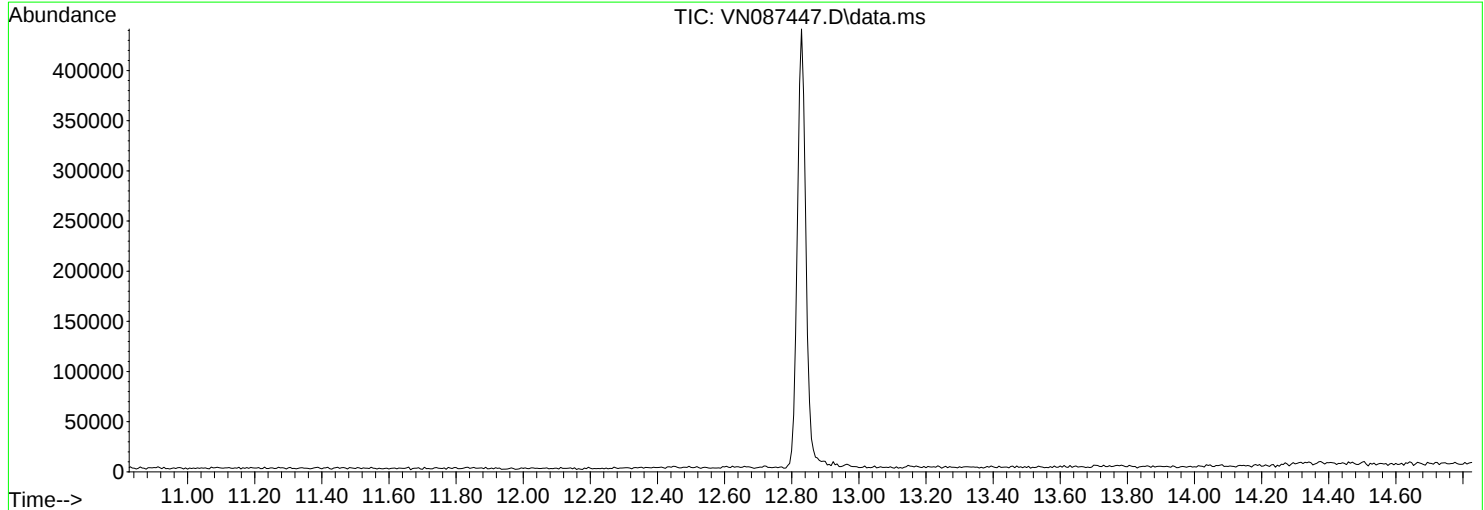

AutoFind: Averaged scan 1841 to 1856; Bkg corrected with scan 1840

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	24.6	6530	PASS
75	95	30	60	58.7	15571	PASS
95	95	100	100	100.0	26522	PASS
96	95	5	9	6.7	1774	PASS
173	174	0.00	2	1.5	263	PASS
174	95	50	100	66.8	17704	PASS
175	174	5	9	7.2	1276	PASS
176	174	95	101	97.7	17301	PASS
177	176	5	9	7.3	1269	PASS