
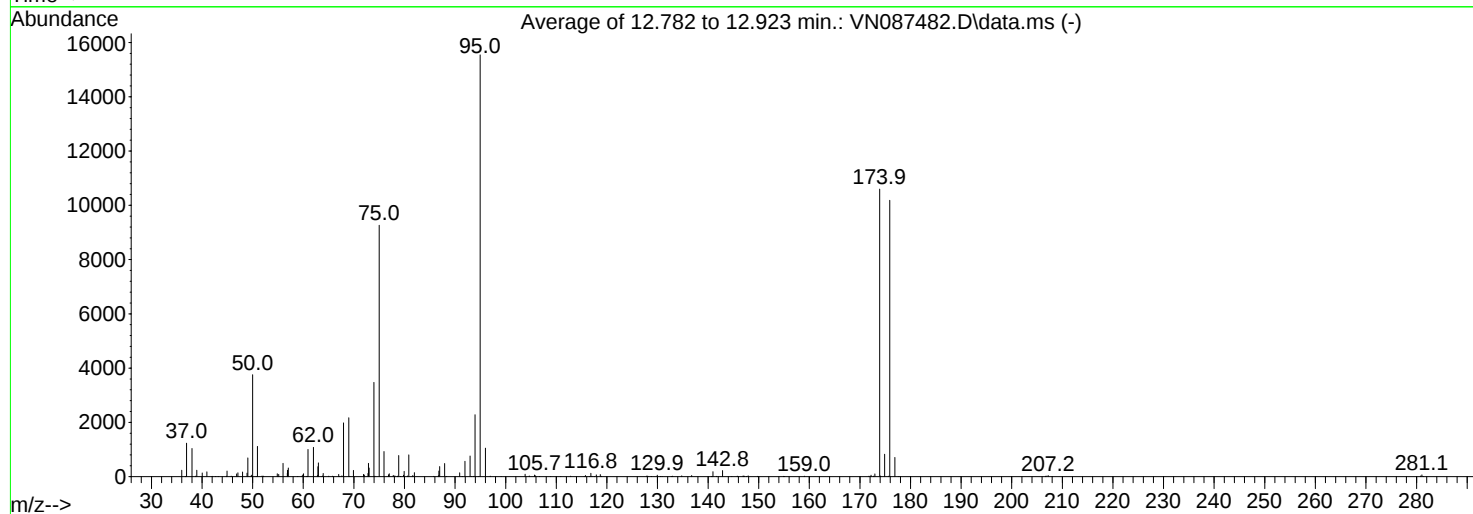


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080725\
Data File : VN087482.D
Acq On : 07 Aug 2025 09:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080525W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Wed Aug 06 02:01:21 2025

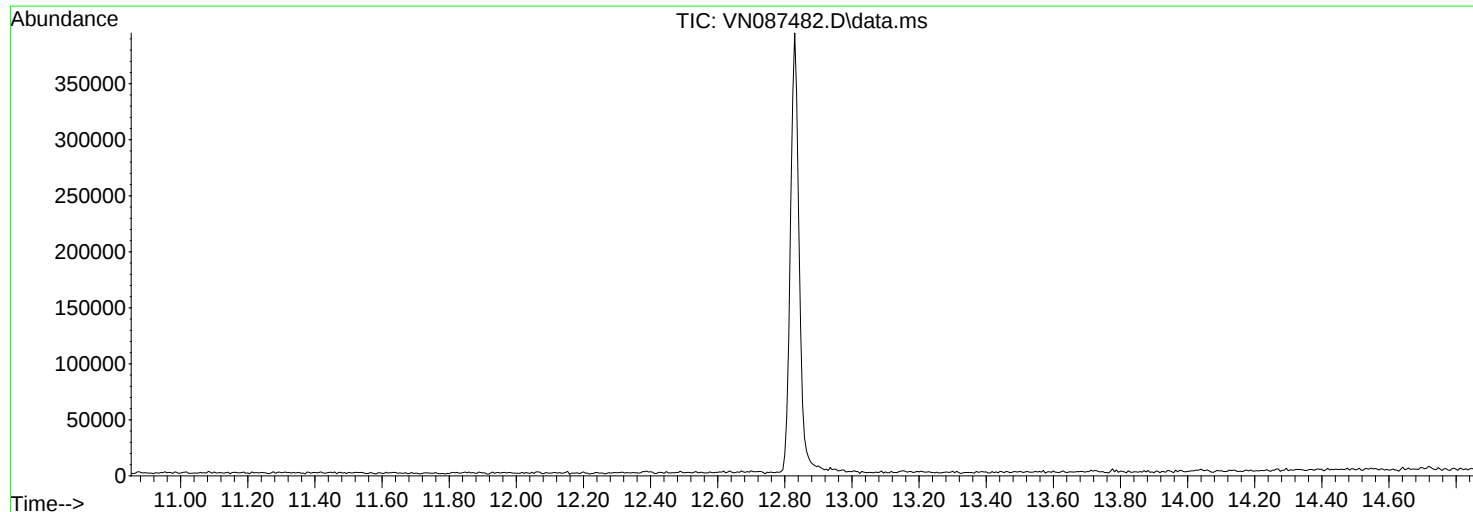

AutoFind: Averaged scan 1841 to 1865; Bkg corrected with scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	3758	PASS
75	95	30	60	59.6	9266	PASS
95	95	100	100	100.0	15546	PASS
96	95	5	9	6.8	1051	PASS
173	174	0.00	2	0.9	98	PASS
174	95	50	100	68.2	10597	PASS
175	174	5	9	7.8	825	PASS
176	174	95	101	96.1	10184	PASS
177	176	5	9	7.0	710	PASS