

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080725\
 Data File : VN087486.D
 Acq On : 07 Aug 2025 11:30
 Operator : JC\MD
 Sample : VN0807WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0807WBL01

Quant Time: Aug 08 01:17:56 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080525W.M
 Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 QLast Update : Wed Aug 06 02:01:21 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Bromochloromethane	7.794	128	59451	30.000	ug/l	0.00
28) 1,4-Difluorobenzene	9.082	114	325046	30.000	ug/l	0.00
57) Chlorobenzene-d5	11.847	117	285832	30.000	ug/l	0.00

System Monitoring Compounds						
27) 1,2-Dichloroethane-d4	8.559	65	168819	30.787	ug/l	0.00
Spiked Amount	30.000	Range	91 - 110	Recovery	=	102.633%
60) 4-Bromofluorobenzene	12.829	95	139109	28.280	ug/l	0.00
Spiked Amount	30.000	Range	63 - 112	Recovery	=	94.267%
63) Toluene-d8	10.547	98	403413	30.674	ug/l	0.00
Spiked Amount	30.000	Range	91 - 112	Recovery	=	102.233%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN080725\
Data File : VN087486.D
Acq On : 07 Aug 2025 11:30
Operator : JC\MD
Sample : VN0807WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0807WBL01

Quant Time: Aug 08 01:17:56 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\624N080525W.M
Quant Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
QLast Update : Wed Aug 06 02:01:21 2025
Response via : Initial Calibration




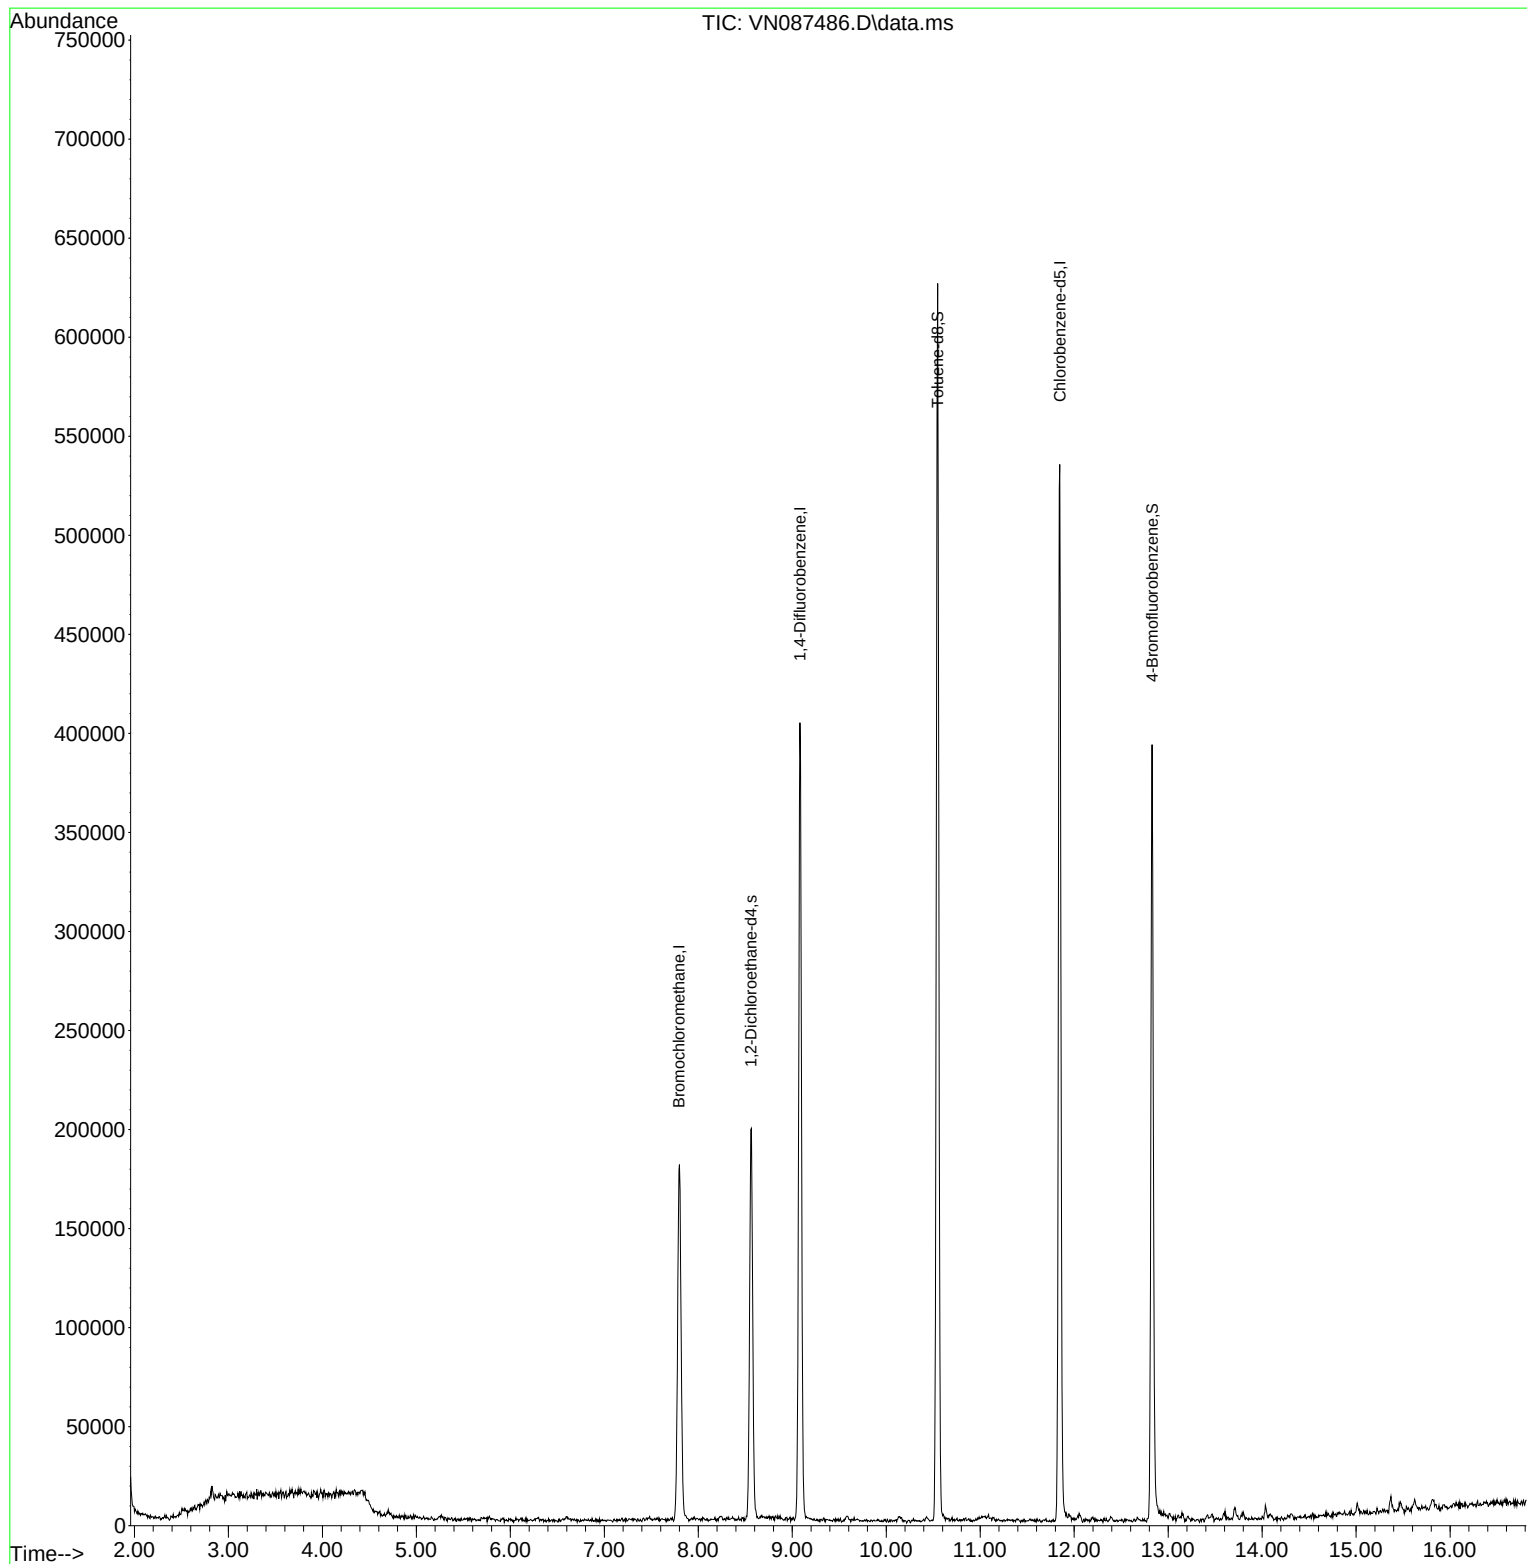


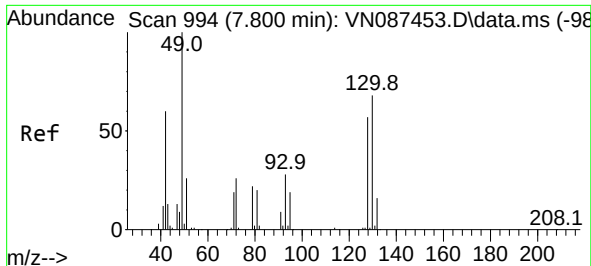

#1
Bromochloromethane
Concen: 30.000 ug/l
RT: 7.794 min Scan# 994
Delta R.T. -0.006 min
Lab File: VN087486.D
Acq: 07 Aug 2025 11:30




Instrument :
MSVOA_N
ClientSampleId :
VN0807WBL01


Tgt Ion:128 Resp: 59451
Ion Ratio Lower Upper
128 100
49 194.7 0.0 494.8
130 125.5 0.0 321.5

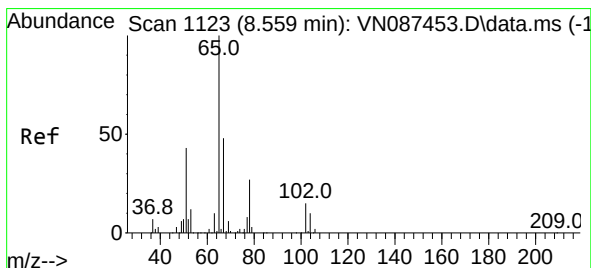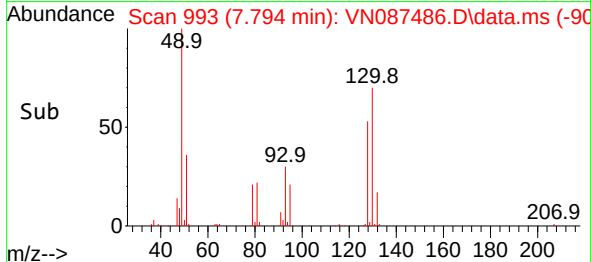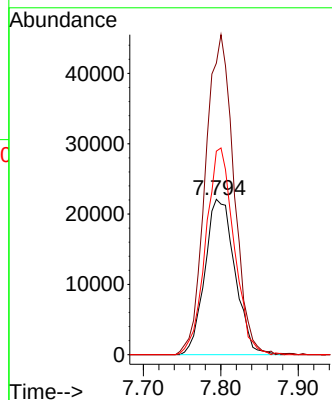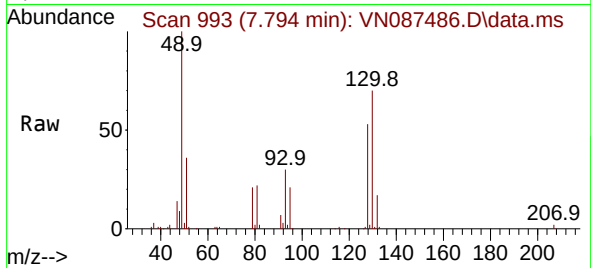

#27
1,2-Dichloroethane-d4
Concen: 30.787 ug/l
RT: 8.559 min Scan# 1123
Delta R.T. -0.000 min
Lab File: VN087486.D
Acq: 07 Aug 2025 11:30

Tgt Ion: 65 Resp: 168819
Ion Ratio Lower Upper
65 100
67 49.3 40.8 61.2

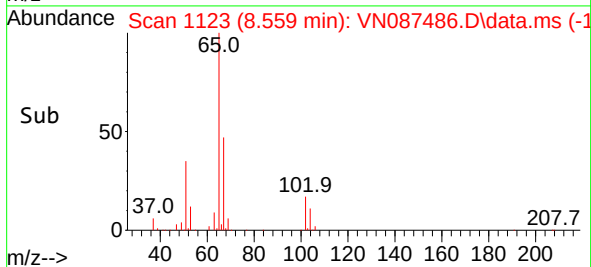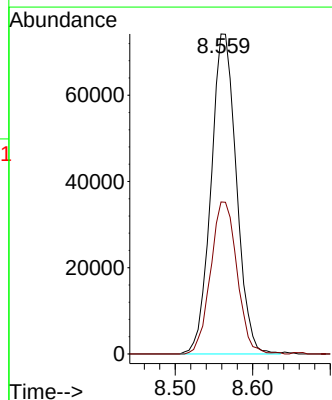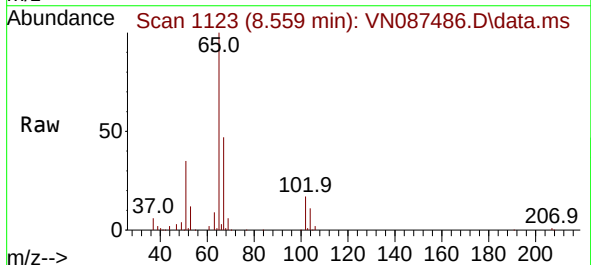

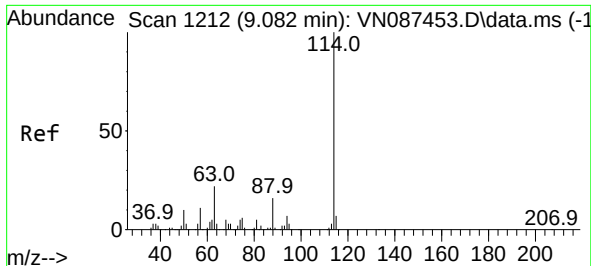

#28

1,4-Difluorobenzene

Concen: 30.000 ug/l

RT: 9.082 min Scan# 11

Delta R.T. -0.000 min

Lab File: VN087486.D

Acq: 07 Aug 2025 11:30

Instrument :

MSVOA_N

ClientSampleId :

VN0807WBL01





Tgt Ion:114 Resp: 325046

Ion Ratio Lower Upper

114 100

63 24.0 18.9 28.3

88 16.4 13.1 19.7

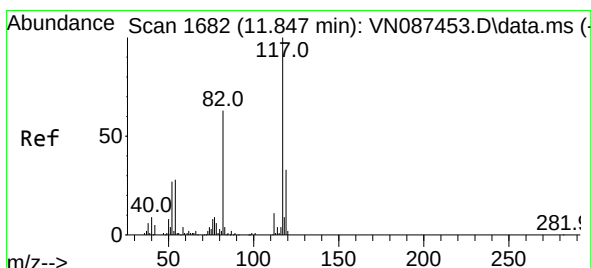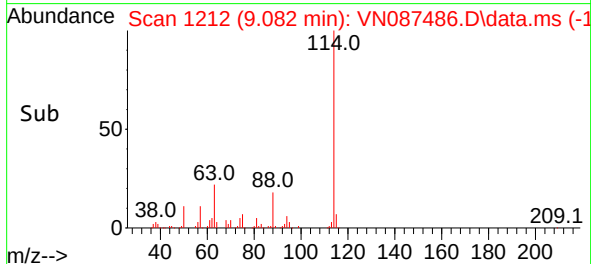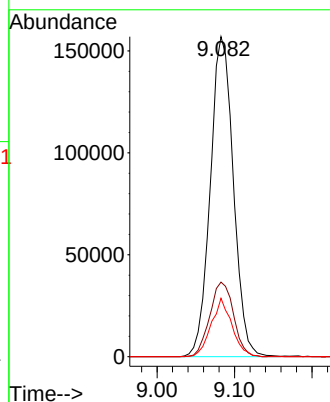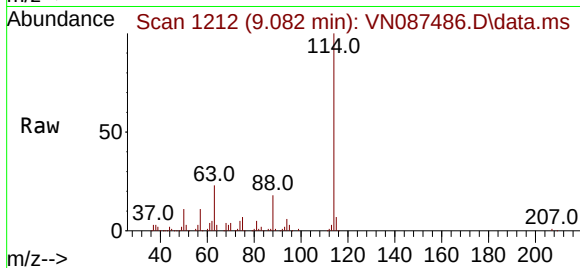

#57

Chlorobenzene-d5

Concen: 30.000 ug/l

RT: 11.847 min Scan# 1682

Delta R.T. -0.000 min

Lab File: VN087486.D

Acq: 07 Aug 2025 11:30




Tgt Ion:117 Resp: 285832


Ion Ratio Lower Upper

117 100

82 62.4 49.2 73.8

119 31.2 25.7 38.5


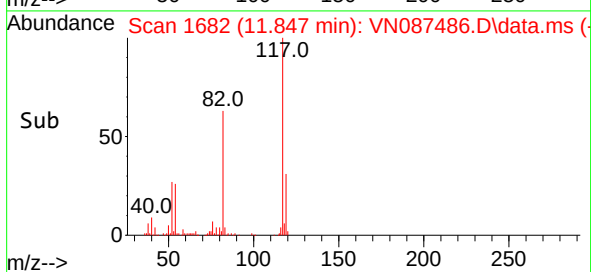
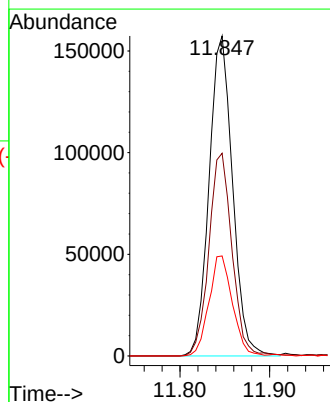
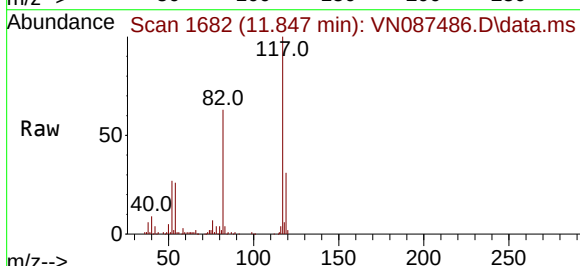


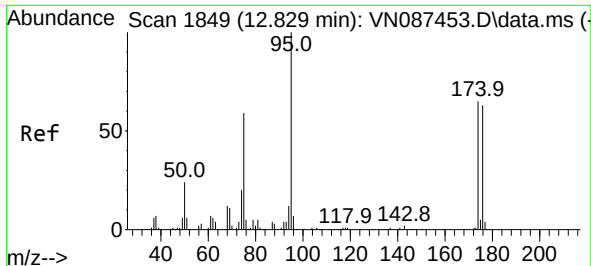

#60
4-Bromofluorobenzene
Concen: 28.280 ug/l
RT: 12.829 min Scan# 1849
Delta R.T. -0.000 min
Lab File: VN087486.D
Acq: 07 Aug 2025 11:30

Instrument :
MSVOA_N
ClientSampleId :
VN0807WBL01

Tgt Ion: 95 Resp: 139109
Ion Ratio Lower Upper
95 100
174 67.4 52.3 78.5
176 63.3 49.8 74.8

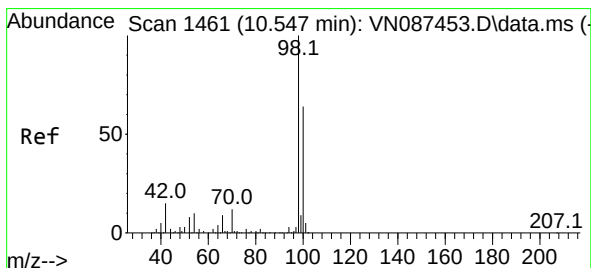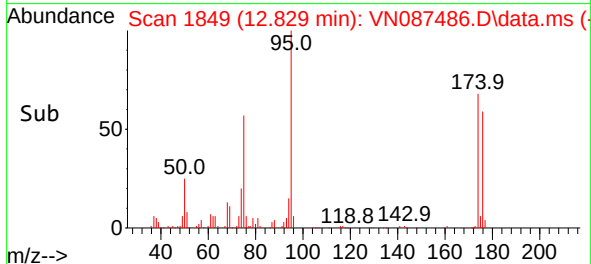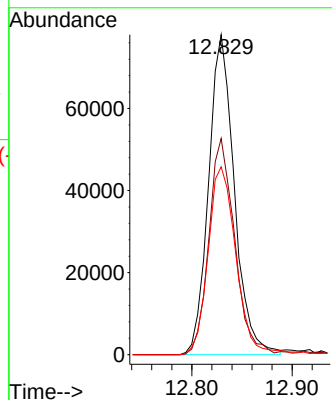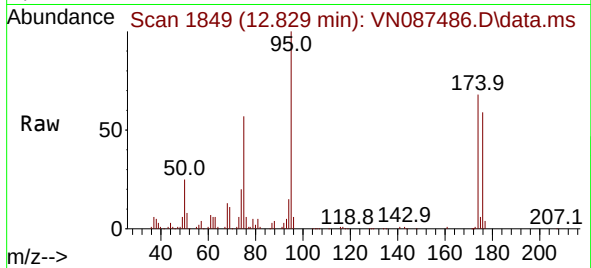

#63
Toluene-d8
Concen: 30.674 ug/l
RT: 10.547 min Scan# 1461
Delta R.T. -0.000 min
Lab File: VN087486.D
Acq: 07 Aug 2025 11:30

Tgt Ion: 98 Resp: 403413
Ion Ratio Lower Upper
98 100
100 63.5 50.5 75.7

