


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080525\
Data File : BP025297.D
Acq On : 05 Aug 2025 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 06 06:41:44 2025

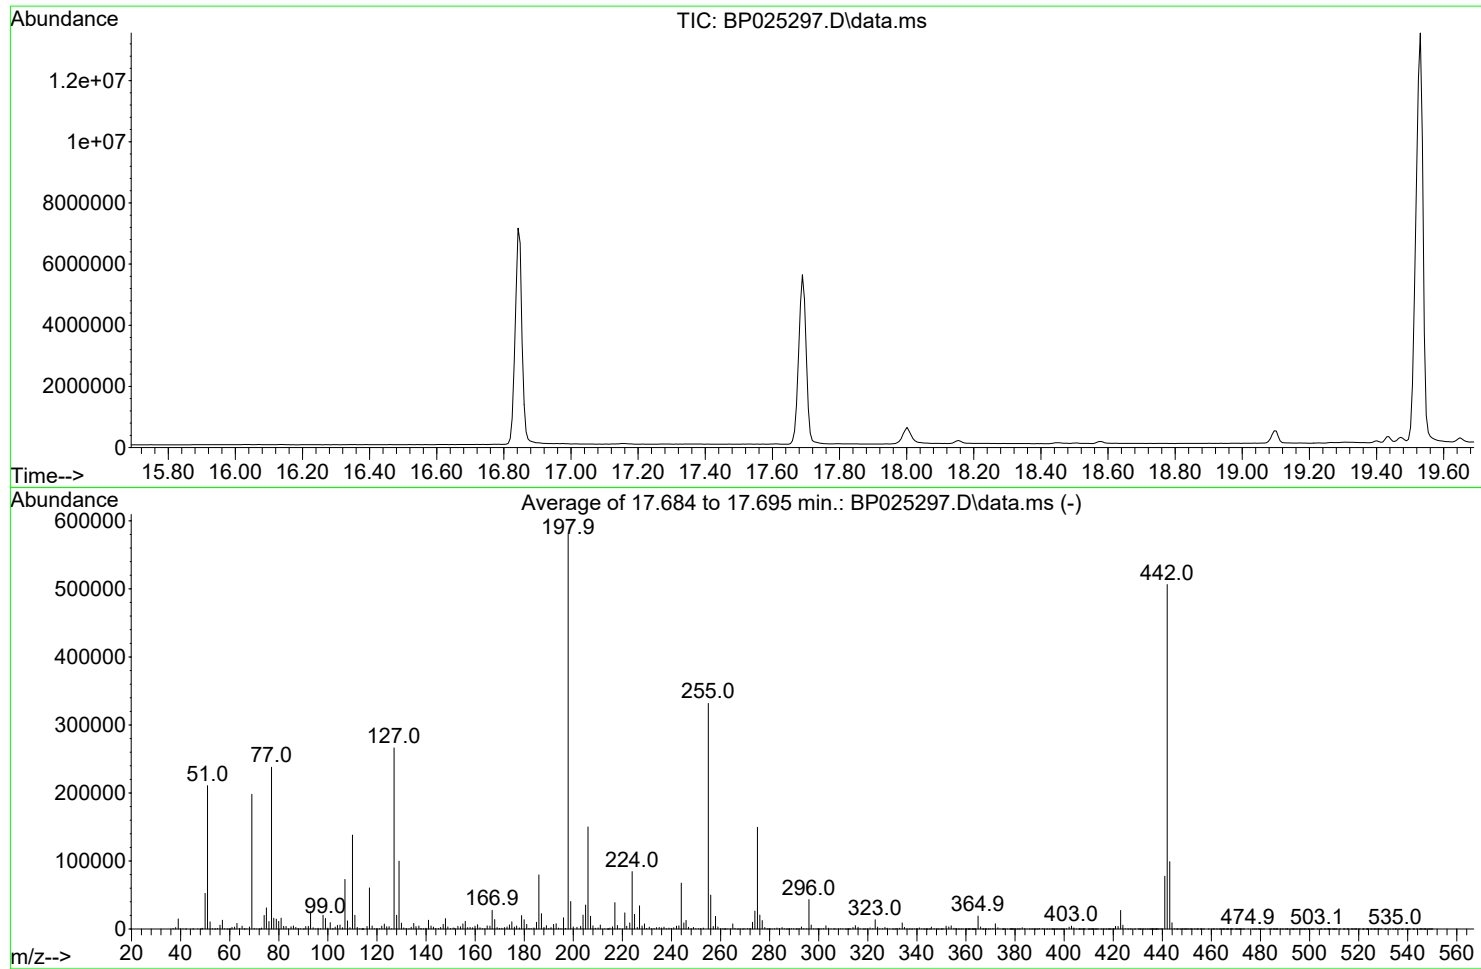

AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2497

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.6	3139	PASS
69	69	100	100	100.0	197961	PASS
70	69	0.00	2	0.5	1001	PASS
197	198	0.00	2	0.2	934	PASS
198	198	100	100	100.0	580472	PASS
199	198	5	9	7.0	40411	PASS
365	198	1	100	3.3	19143	PASS
441	443	0.01	150	78.4	77662	PASS
442	442	100	100	100.0	506491	PASS
443	442	15	24	19.6	99034	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/5/2025	BNA_P	<u>BP025297.D</u>
Compound Name	Response	Retention Time
DDT	2359483	20.83
DDD	25464	20.425
DDE	1490	19.836
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26954	2386437	1.13

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080525\
Data File : BP025297.D
Acq On : 05 Aug 2025 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 06 07:09:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

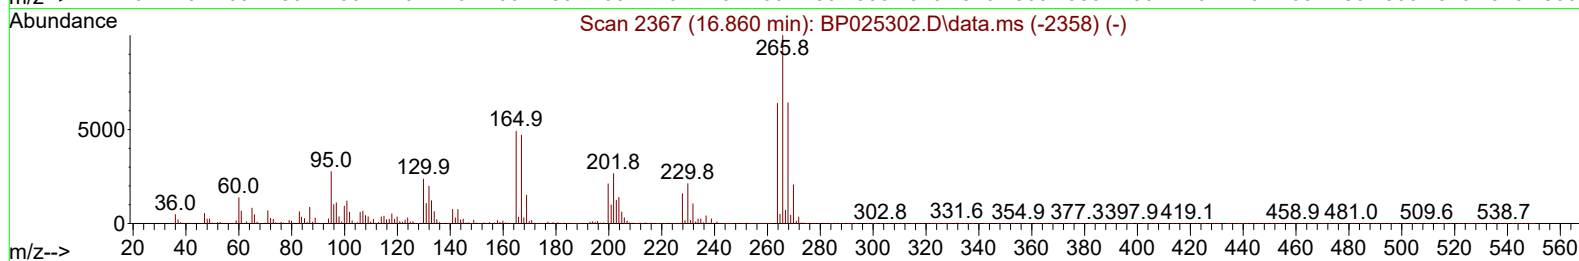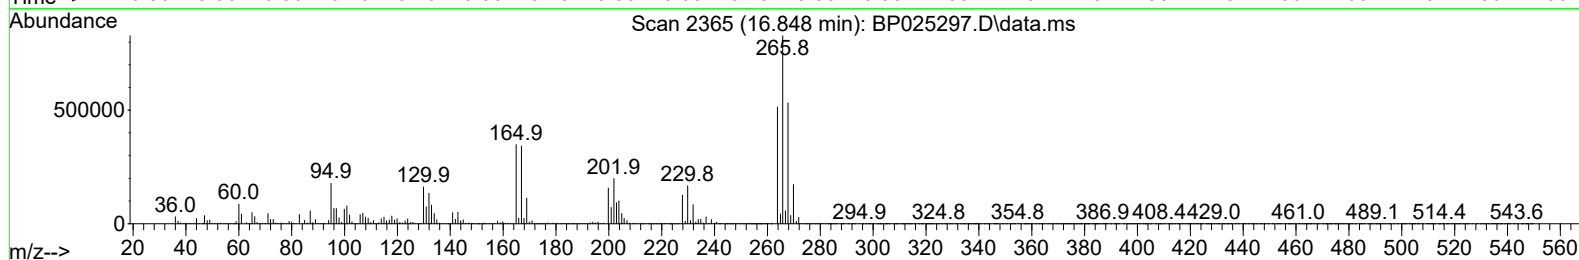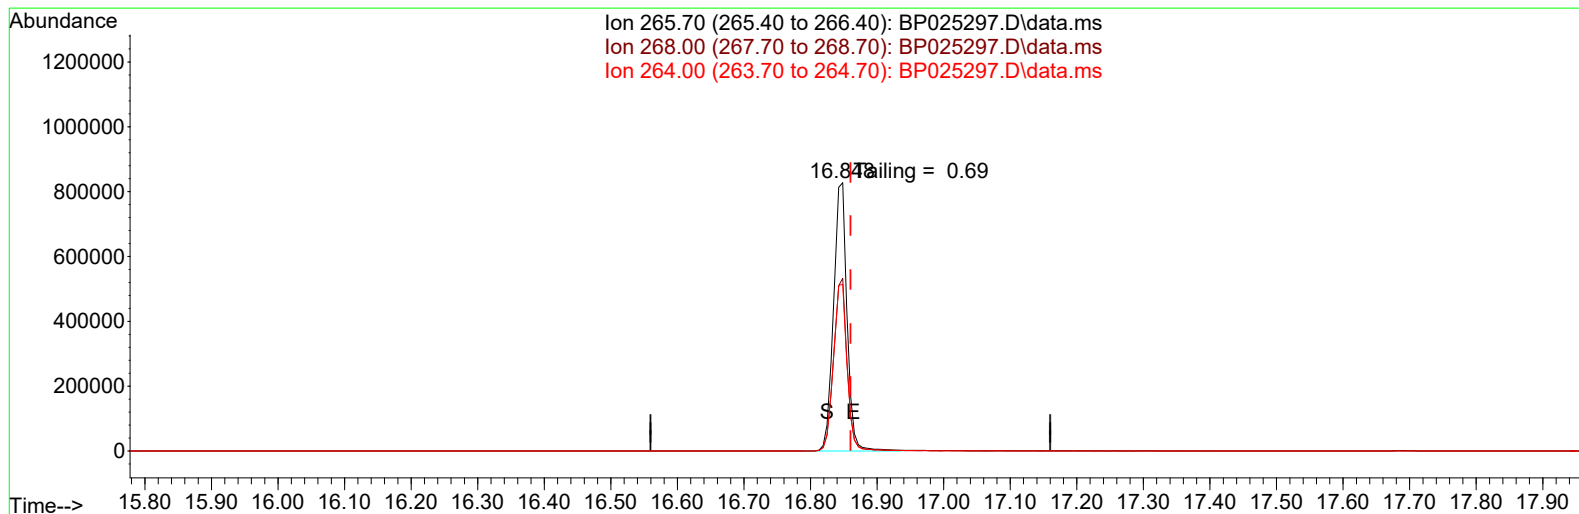

TIC: BP025297.D\data.ms

(70) Pentachlorophenol (C)

16.848min (-0.012) 1707314.09 ng




response 1166643

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.31
264.00	63.90	62.13
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080525\
Data File : BP025297.D
Acq On : 05 Aug 2025 11:21
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 06 07:09:02 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

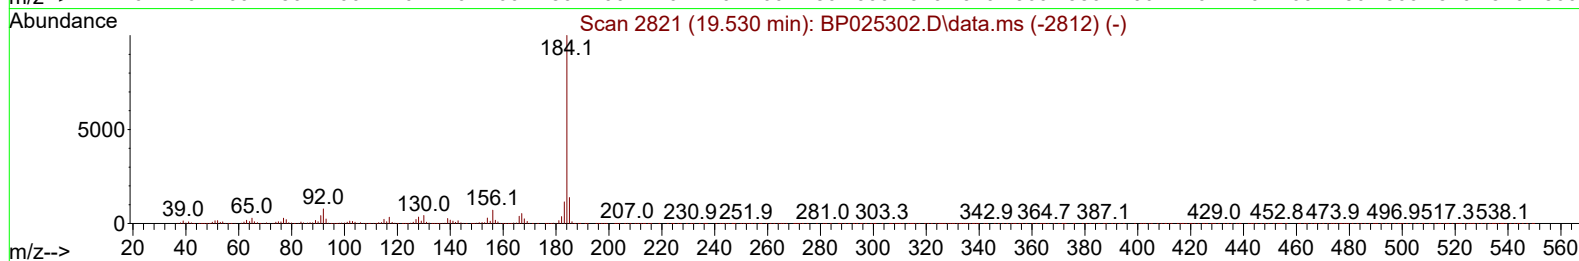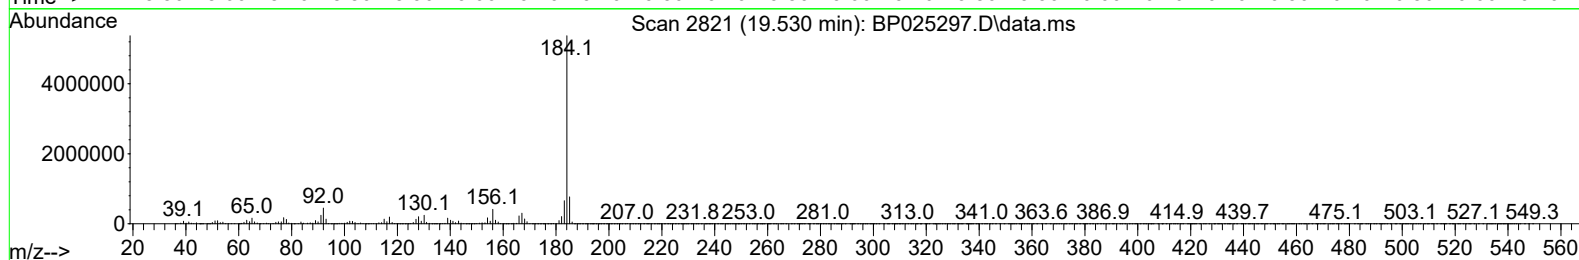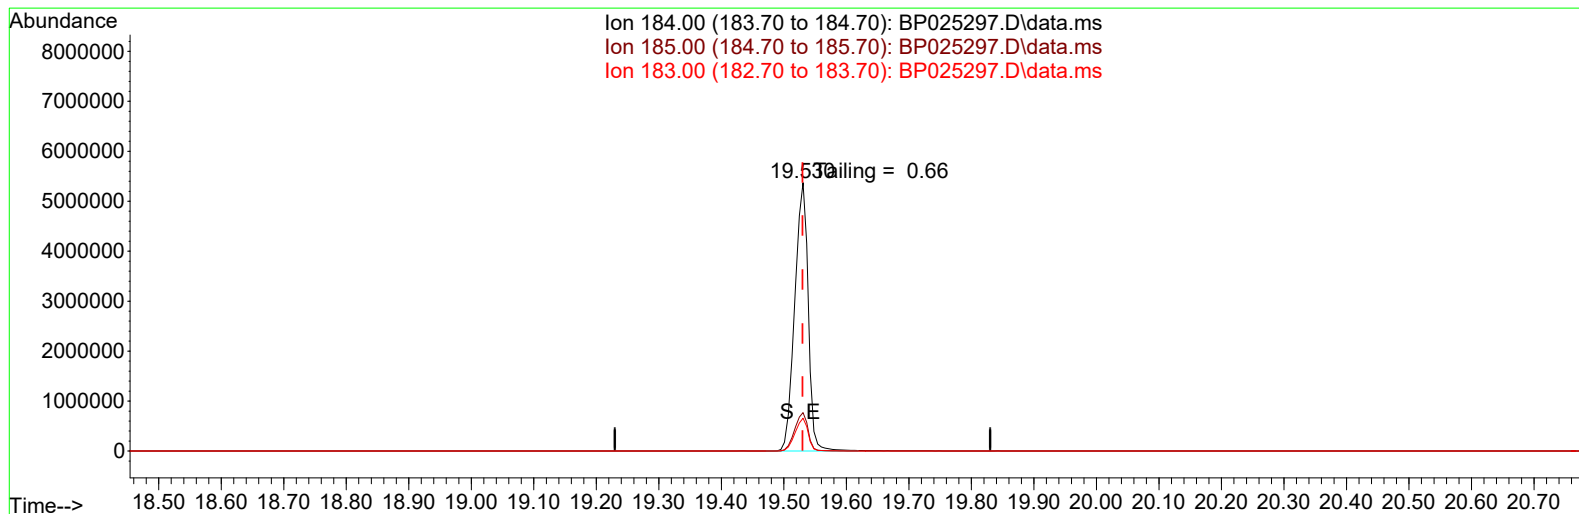

TIC: BP025297.D\data.ms

(77) Benzidine

19.530min (+ 0.000) 113432.74 ng

response 8120949

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.30
183.00	11.50	12.22
0.00	0.00	0.00