
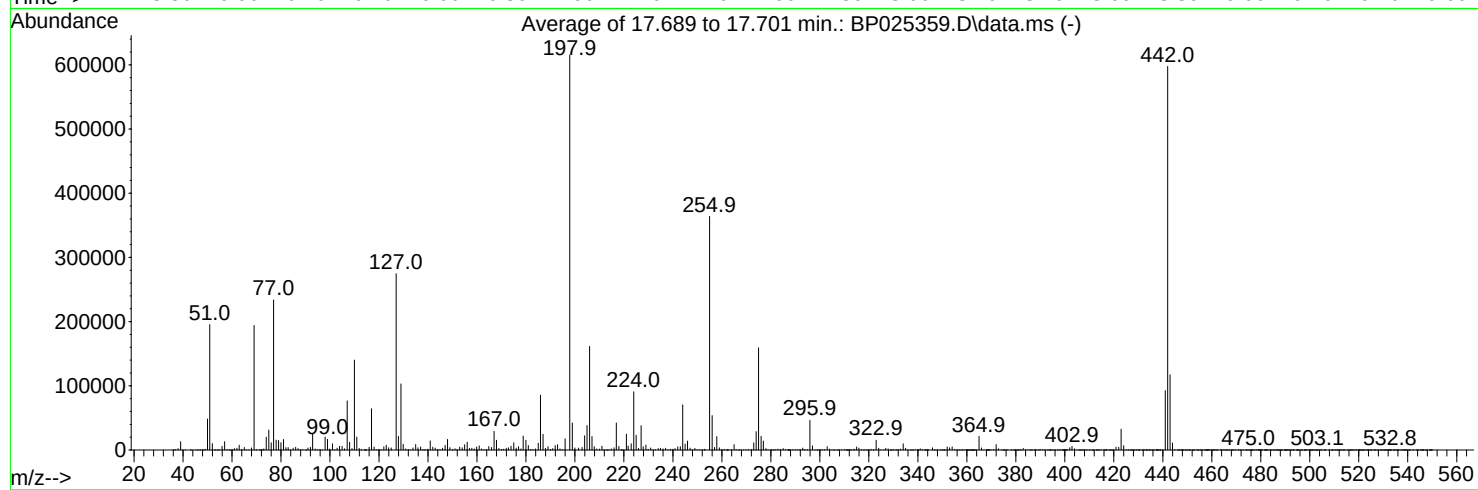


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081225\
Data File : BP025359.D
Acq On : 12 Aug 2025 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 06 06:41:44 2025

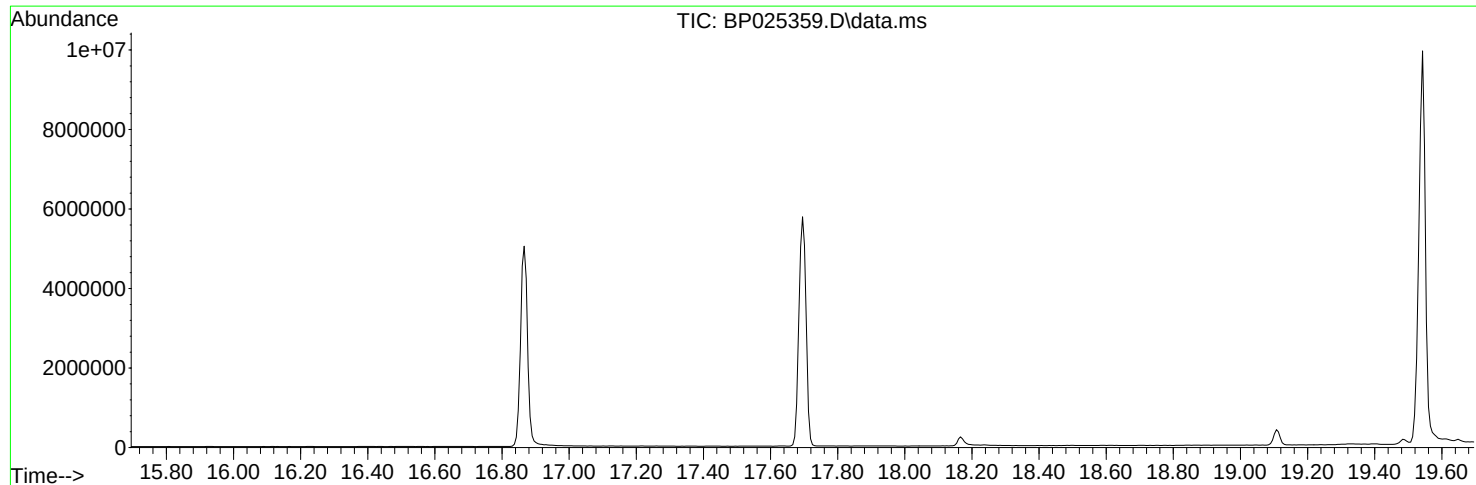

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2499

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.6	3158	PASS
69	69	100	100	100.0	194138	PASS
70	69	0.00	2	0.5	928	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	615091	PASS
199	198	5	9	6.8	42032	PASS
365	198	1	100	3.4	21184	PASS
441	443	0.01	150	79.0	92605	PASS
442	442	100	100	100.0	597468	PASS
443	442	15	24	19.6	117267	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/12/2025	BNA_P	<u>BP025359.D</u>
Compound Name	Response	Retention Time
DDT	2590799	20.831
DDD	48921	20.372
DDE	3872	19.848
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
52793	2643592	2.00

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081225\
Data File : BP025359.D
Acq On : 12 Aug 2025 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 12 11:27:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

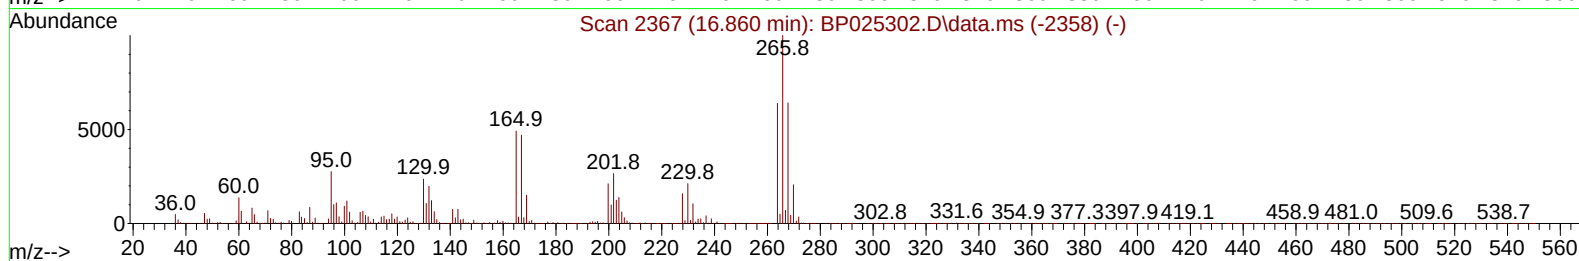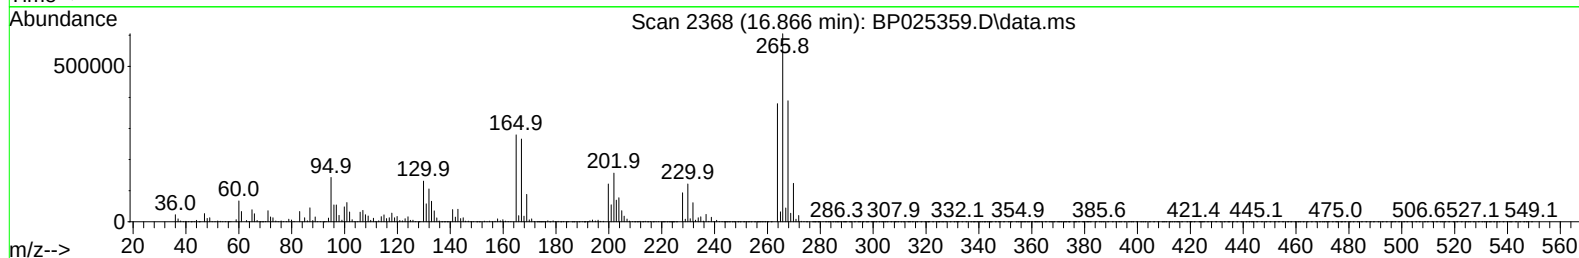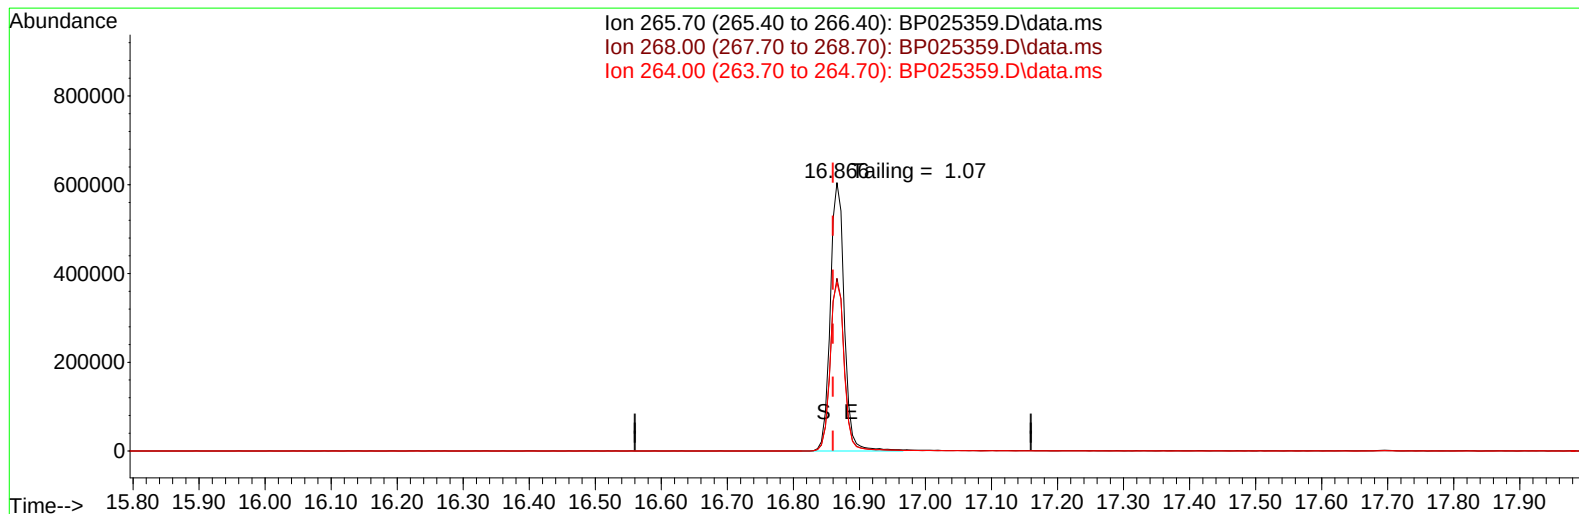

TIC: BP025359.D\data.ms

(70) Pentachlorophenol (C)

16.866min (+ 0.006) 2105985.22 ng




response 893734

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.31
264.00	63.90	62.80
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081225\
Data File : BP025359.D
Acq On : 12 Aug 2025 09:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 12 11:27:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

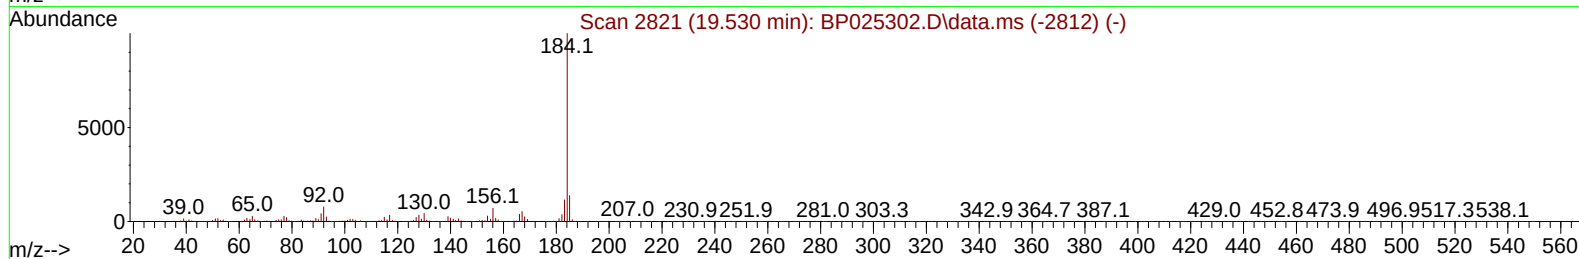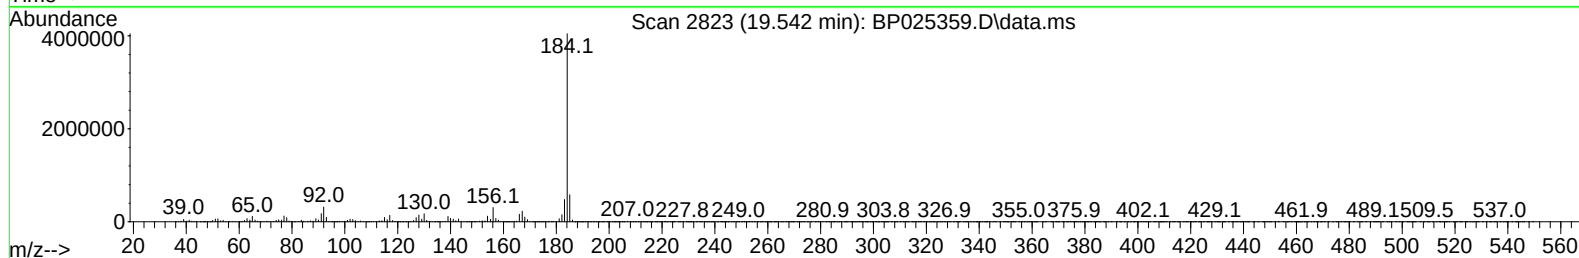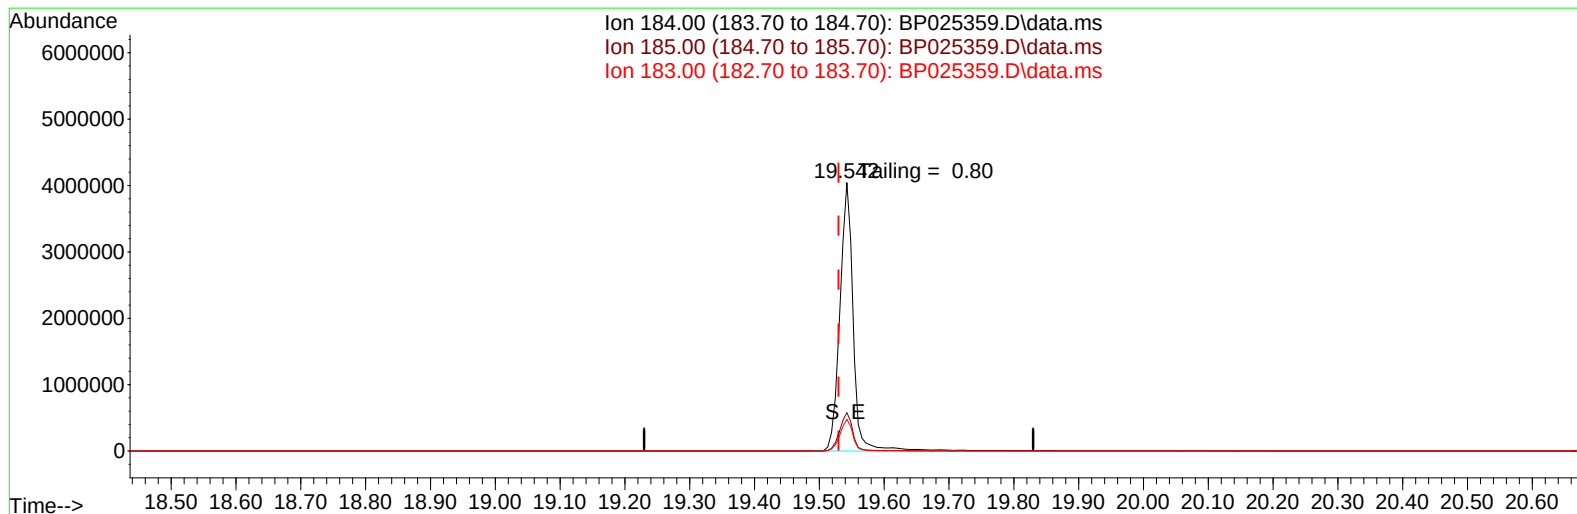

TIC: BP025359.D\data.ms

(77) Benzidine

19.542min (+ 0.012) 1326377.90 ng

response 5712896

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.35
183.00	11.50	11.85
0.00	0.00	0.00