


Instrument IC-1		Analyst : NF		Method: 300.0 / 9056A							
Ident	Con F-	Con CL-	Con NO;	Con BR-	Con NO;	Con HPC	Con SO4	Method name	date time	Initial wt/Final \	Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 10:18	10	RM/IZ
STD2	0.413	0.620	0.623	2.052	0.515	1.033	3.185	IC1-080625	8/6/2025 10:40	10	RM/IZ
STD3	0.794	1.184	1.185	3.953	0.990	2.067	5.931	IC1-080625	8/6/2025 11:01	10	RM/IZ
STD4	1.023	1.524	1.519	5.070	1.270	2.633	7.597	IC1-080625	8/6/2025 11:23	10	RM/IZ
STD5	1.972	2.981	2.982	9.960	2.483	4.695	14.838	IC1-080625	8/6/2025 11:44	10	RM/IZ
STD6	3.956	5.938	5.934	19.801	4.945	9.953	29.505	IC1-080625	8/6/2025 12:06	10	RM/IZ
STD7	5.041	7.553	7.556	25.165	6.298	12.620	37.443	IC1-080625	8/6/2025 12:27	10	RM/IZ
ICV	2.038	3.184	3.095	10.343	2.641	4.970	15.425	IC1-080625	8/6/2025 12:48	10	RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 13:10	10	RM/IZ
CCV	2.039	3.047	3.026	10.152	2.527	5.131	15.069	IC1-080625	8/7/2025 9:06	10	RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/7/2025 9:28	10	RM/IZ
LB136743BLS	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/7/2025 9:49	5.00g/100ml	RM/IZ
LB136743BSS	2.038	3.048	3.025	10.165	2.532	5.157	15.088	IC1-080625	8/7/2025 10:11	5.00g/100ml	RM/IZ
Q2795-01	0.122	0.456	0.000	0.000	0.242	0.579	3.241	IC1-080625	8/7/2025 13:56	5.01g/100ml	RM/IZ
Q2795-01MS	2.041	3.483	3.055	10.257	2.730	5.121	17.600	IC1-080625	8/7/2025 14:18	5.03g/100ml	RM/IZ
Q2795-01MSD	2.059	3.514	3.064	10.281	2.735	5.055	17.748	IC1-080625	8/7/2025 14:40	5.01g/100ml	RM/IZ
Q2795-02	0.217	2.654	0.000	0.000	0.068	0.339	0.850	IC1-080625	8/7/2025 15:01	5.02g/100ml	RM/IZ
Q2795-03	0.142	0.817	0.000	0.000	0.059	0.406	0.564	IC1-080625	8/7/2025 15:23	5.03g/100ml	RM/IZ
CCV	2.033	3.054	3.030	10.153	2.533	5.104	15.150	IC1-080625	8/7/2025 15:44	10	RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/7/2025 16:06	10	RM/IZ

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio n HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-080625	8/6/2025 10:18	10	RM/IZ
STD2	0.4130	0.6200	0.6230	2.0520	0.5150	1.0330	3.1850	IC1-080625	8/6/2025 10:40	10	RM/IZ
STD3	0.7940	1.1840	1.1850	3.9530	0.9900	2.0670	5.9310	IC1-080625	8/6/2025 11:01	10	RM/IZ
STD4	1.0230	1.5240	1.5190	5.0700	1.2700	2.6330	7.5970	IC1-080625	8/6/2025 11:23	10	RM/IZ
STD5	1.9720	2.9810	2.9820	9.9600	2.4830	4.6950	14.8380	IC1-080625	8/6/2025 11:44	10	RM/IZ
STD6	3.9560	5.9380	5.9340	19.8010	4.9450	9.9530	29.5050	IC1-080625	8/6/2025 12:06	10	RM/IZ
STD7	5.0410	7.5530	7.5560	25.1650	6.2980	12.6200	37.4430	IC1-080625	8/6/2025 12:27	10	RM/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	3.2500	3.3333	3.8333	2.6000	3.0000	3.3000	6.1667				
STD3	-0.7500	-1.3333	-1.2500	-1.1750	-1.0000	3.3500	-1.1500				
STD4	2.3000	1.6000	1.2667	1.4000	1.6000	5.3200	1.2933				
STD5	-1.4000	-0.6333	-0.6000	-0.4000	-0.6800	-6.1000	-1.0800				
STD6	-1.1000	-1.0333	-1.1000	-0.9950	-1.1000	-0.4700	-1.6500				
STD7	0.8200	0.7067	0.7467	0.6600	0.7680	0.9600	1.1973				

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

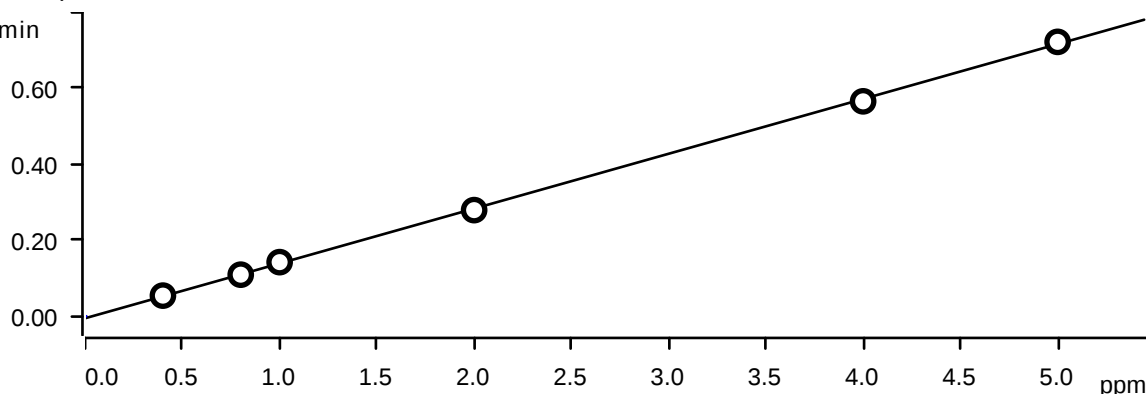

Function: $A = -5.18233E-3 + 0.0144368 \times Q$


Relative standard deviation: 1.650446 %

Correlation coefficient: 0.999856

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.110	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.280	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.723	STD7	2025-08-06 12:27:27 UTC-4	used

Chloride (Anions)

($\mu\text{S}/\text{cm}$) x min

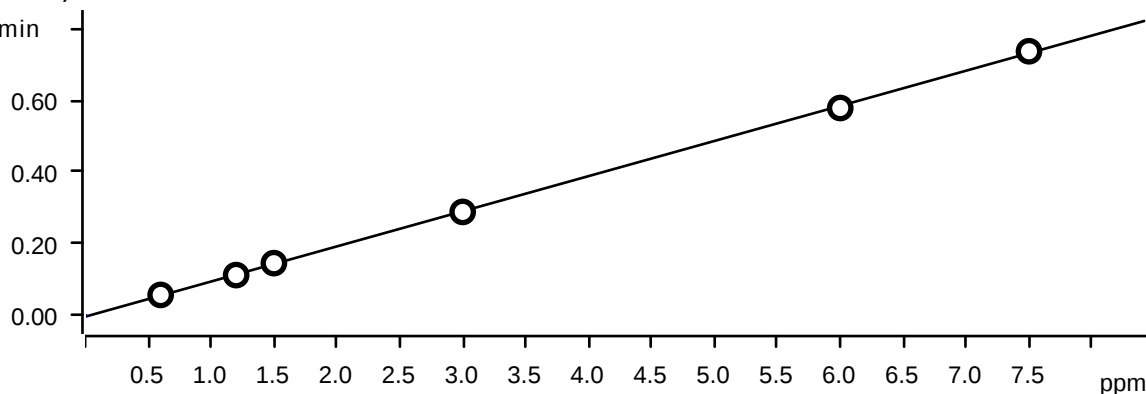

Function: $A = -3.45407E-3 + 9.79772E-3 \times Q$


Relative standard deviation 1.384132 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.113	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.289	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.578	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.737	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

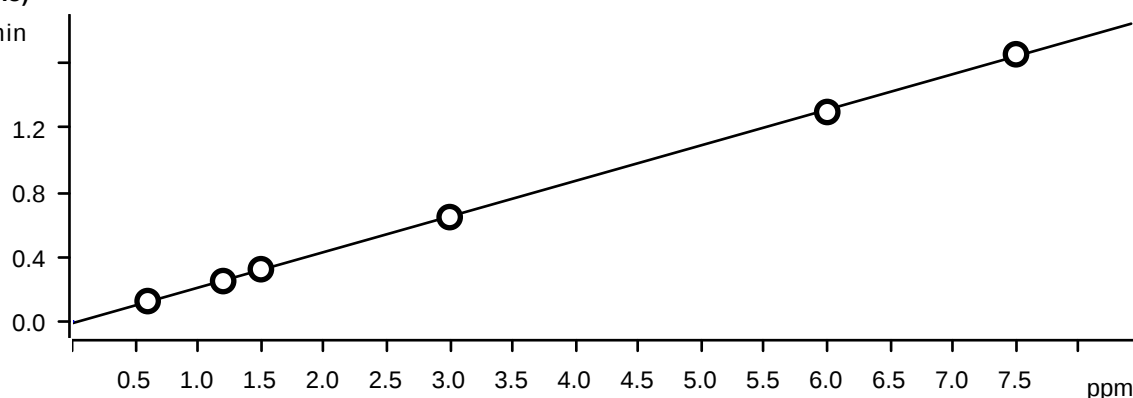Function: $A = -0.0116303 + 0.0220561 \times Q$


Relative standard deviation 1.449488 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.250	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.323	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.646	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.297	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.655	STD7	2025-08-06 12:27:27 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

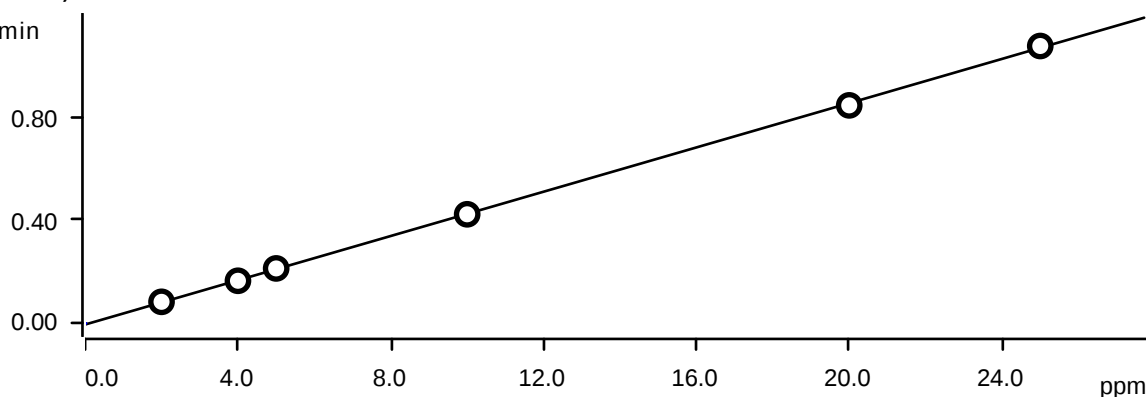

Function: $A = -4.59233\text{E-}3 + 4.28617\text{E-}3 \times Q$


Relative standard deviation: 1.283698 %

Correlation coefficient: 0.999912

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.083	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.165	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.422	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.844	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.074	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

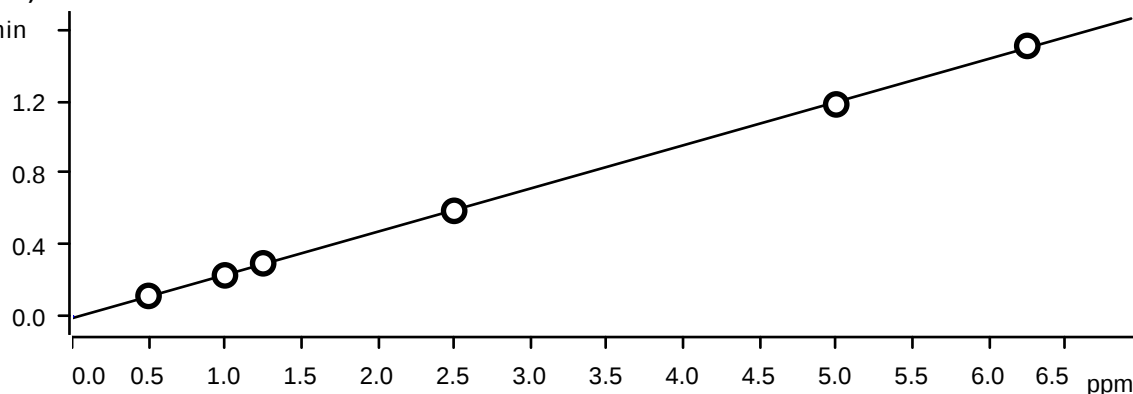


Function: $A = -9.68516\text{E-}3 + 0.0241085 \times Q$

Relative standard deviation: 1.469135 %

Correlation coefficient 0.999886

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.296	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.589	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.182	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.509	STD7	2025-08-06 12:27:27 UTC-4	used

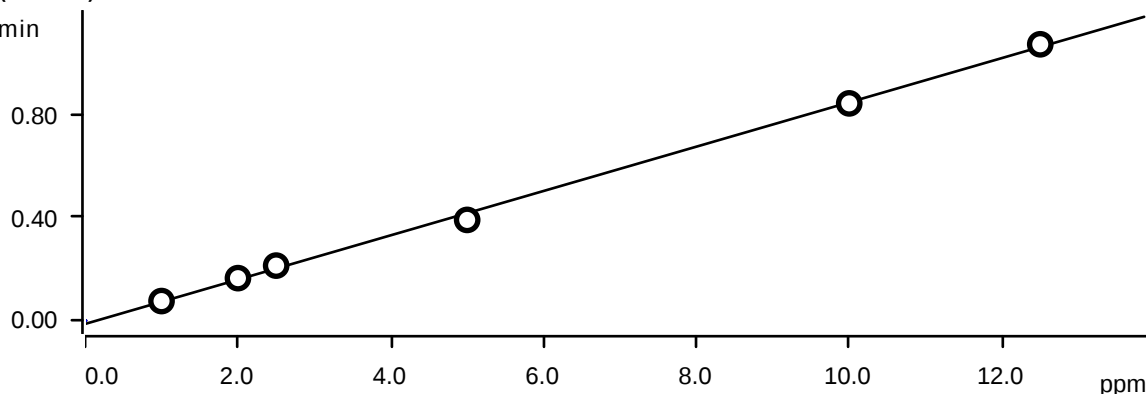
Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0128563 + 8.58091E-3 \times Q$

Relative standard deviation 3.406332 %

Correlation coefficient 0.999402

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.076	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.164	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.390	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.841	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.070	STD7	2025-08-06 12:27:27 UTC-4	used

Sulfate (Anions)

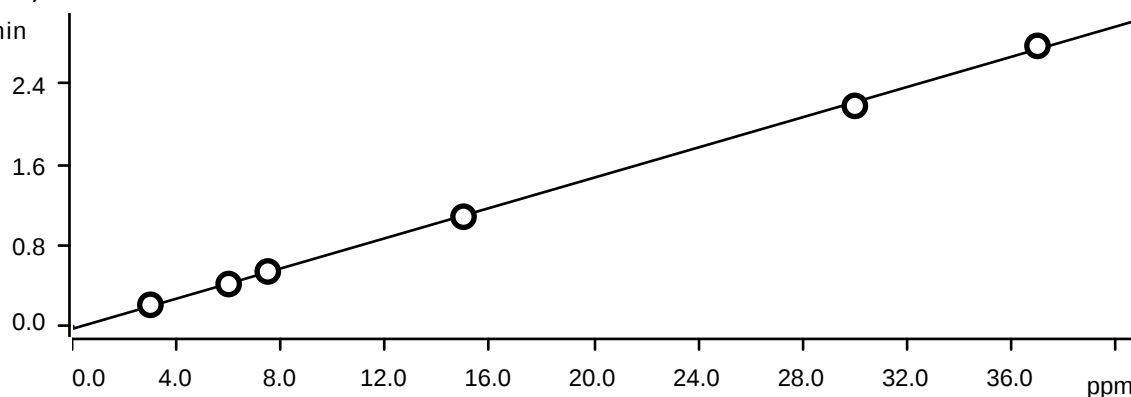 $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0267558 + 7.49232E-3 \times Q$

Relative standard deviation 2.236460 %

Correlation coefficient 0.999736


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.418	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.542	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.085	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.184	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.779	STD7	2025-08-06 12:27:27 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-08-06 10:18:54 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

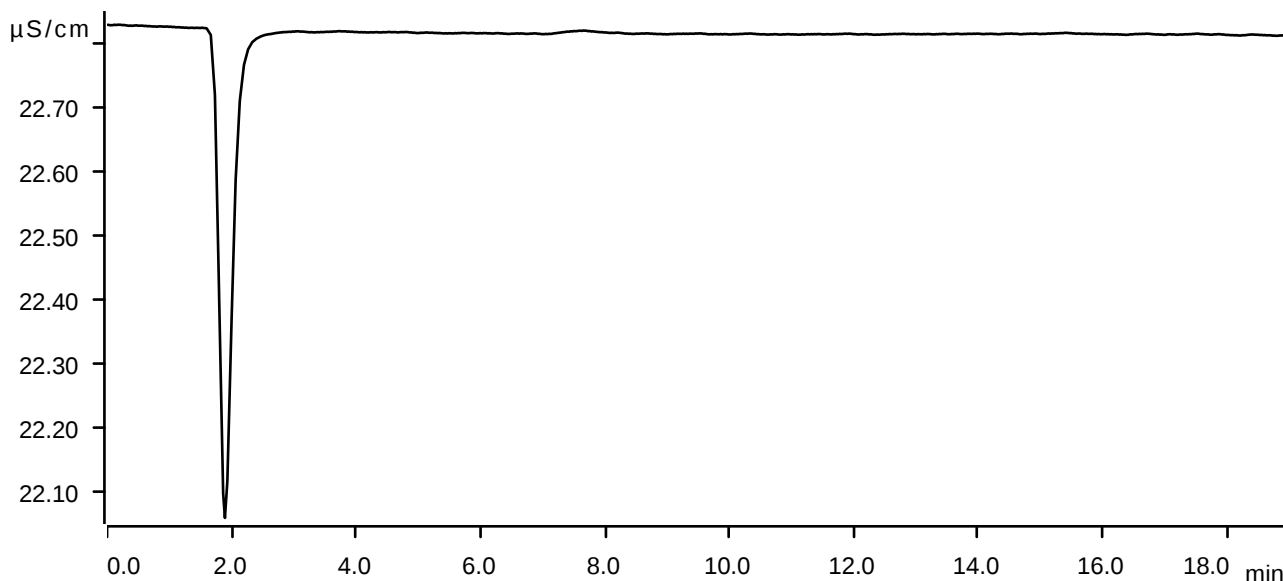Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-08-06 10:40:18 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

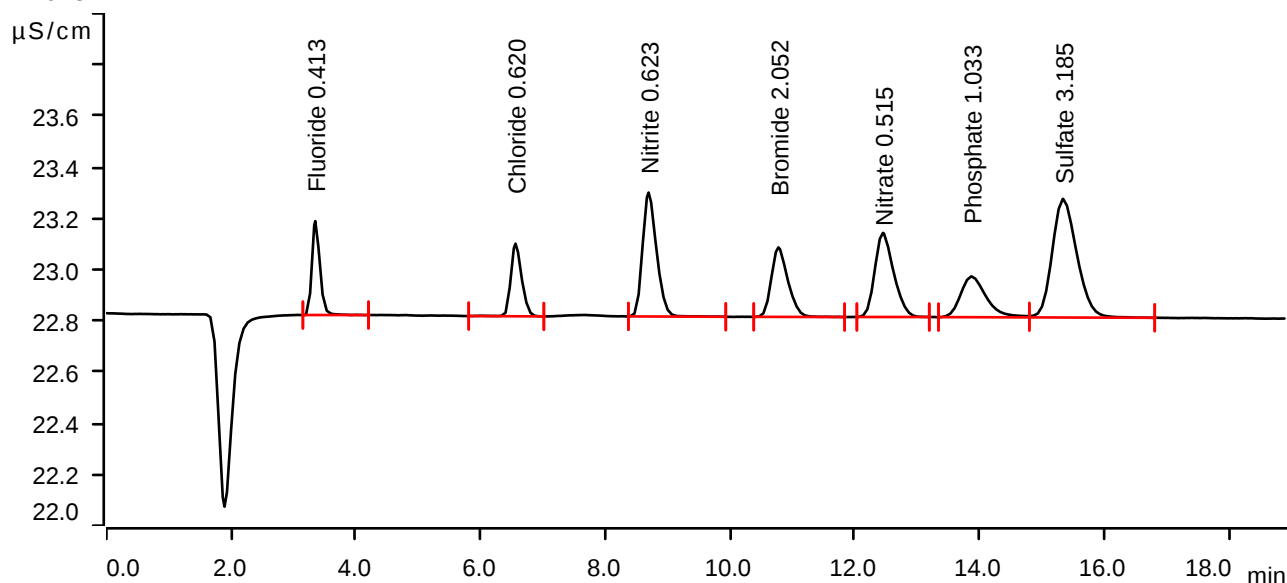

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.0544	0.367	0.413	Fluoride
2	6.560	0.0573	0.284	0.620	Chloride
3	8.693	0.1258	0.484	0.623	Nitrite
4	10.775	0.0833	0.271	2.052	Bromide
5	12.452	0.1145	0.328	0.515	Nitrate
6	13.870	0.0758	0.159	1.033	Phosphate
7	15.340	0.2119	0.463	3.185	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-08-06 11:01:42 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

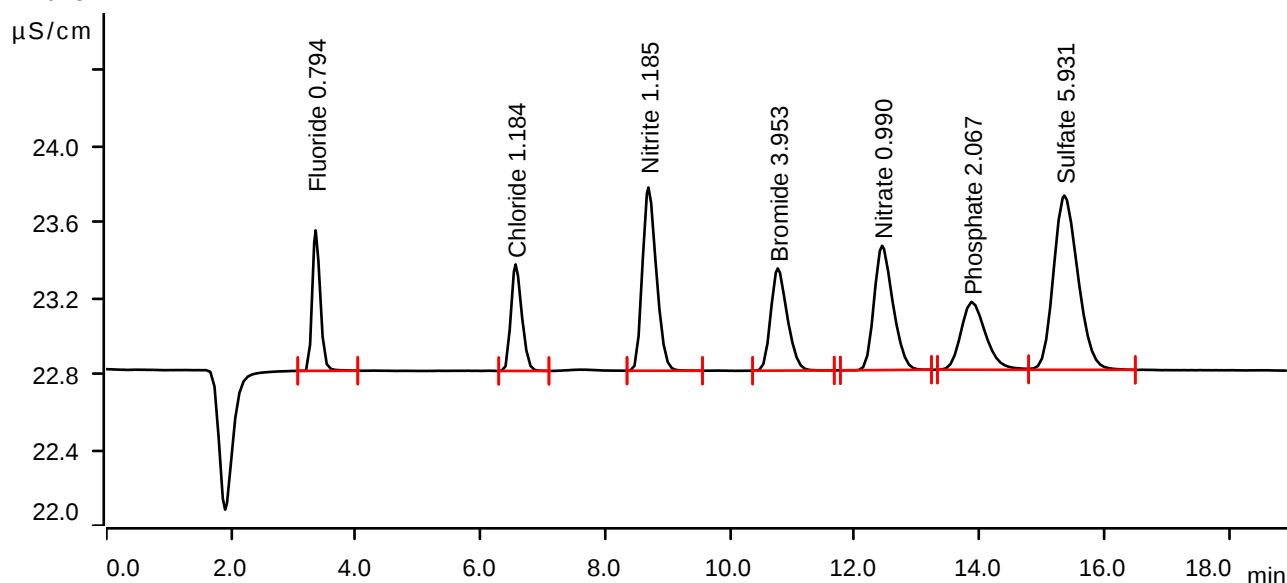

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.1095	0.740	0.794	Fluoride
2	6.562	0.1125	0.561	1.184	Chloride
3	8.692	0.2498	0.966	1.185	Nitrite
4	10.765	0.1649	0.539	3.953	Bromide
5	12.438	0.2291	0.655	0.990	Nitrate
6	13.875	0.1645	0.358	2.067	Phosphate
7	15.360	0.4176	0.918	5.931	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-08-06 11:23:08 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

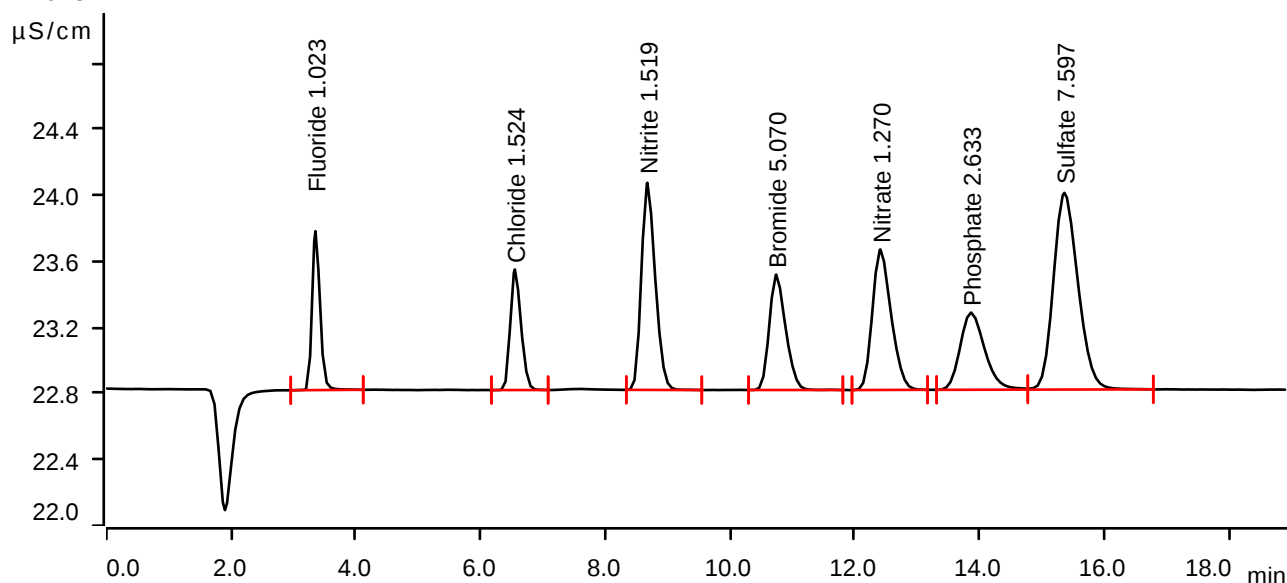

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1425	0.962	1.023	Fluoride
2	6.552	0.1459	0.730	1.524	Chloride
3	8.675	0.3233	1.254	1.519	Nitrite
4	10.740	0.2127	0.698	5.070	Bromide
5	12.410	0.2964	0.850	1.270	Nitrate
6	13.862	0.2131	0.467	2.633	Phosphate
7	15.360	0.5424	1.191	7.597	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-08-06 11:44:33 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

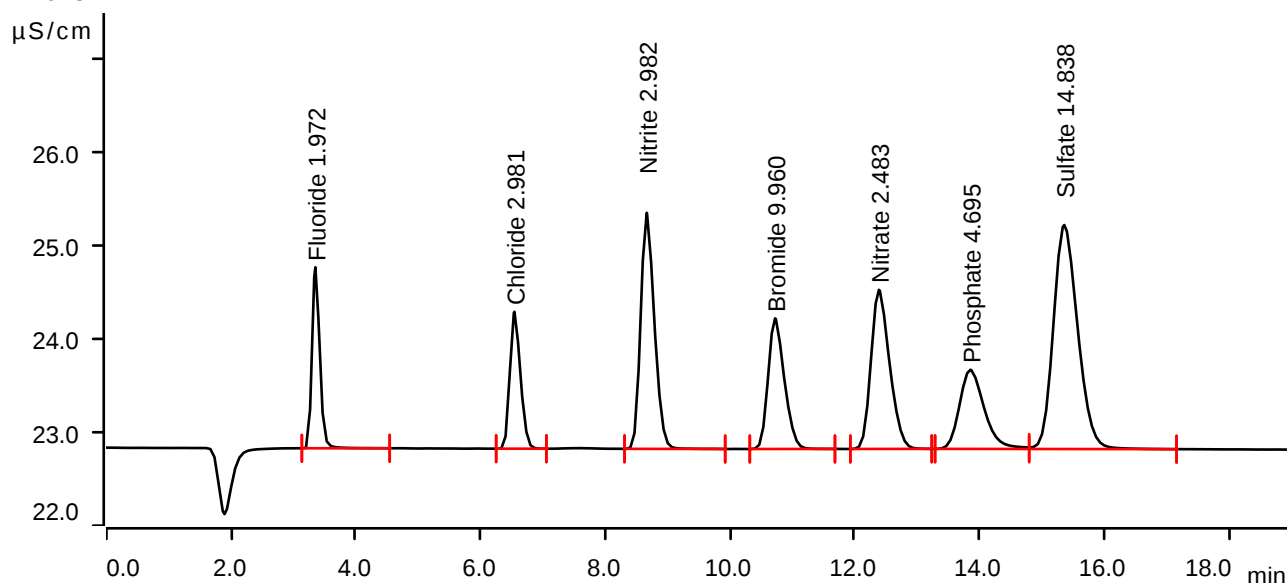

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2796	1.943	1.972	Fluoride
2	6.543	0.2887	1.470	2.981	Chloride
3	8.663	0.6461	2.534	2.982	Nitrite
4	10.722	0.4223	1.403	9.960	Bromide
5	12.387	0.5889	1.709	2.483	Nitrate
6	13.853	0.3900	0.850	4.695	Phosphate
7	15.358	1.0850	2.405	14.838	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-08-06 12:06:00 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

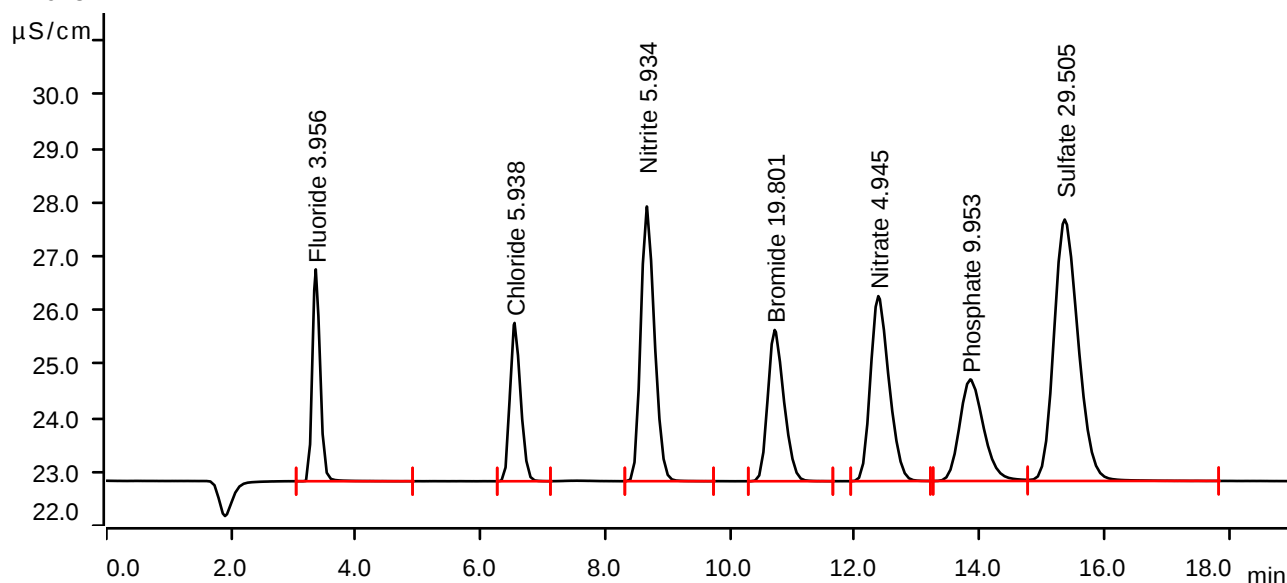

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.5660	3.928	3.956	Fluoride
2	6.545	0.5784	2.936	5.938	Chloride
3	8.665	1.2973	5.095	5.934	Nitrite
4	10.715	0.8441	2.805	19.801	Bromide
5	12.377	1.1824	3.431	4.945	Nitrate
6	13.852	0.8412	1.884	9.953	Phosphate
7	15.365	2.1839	4.849	29.505	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-08-06 12:27:27 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

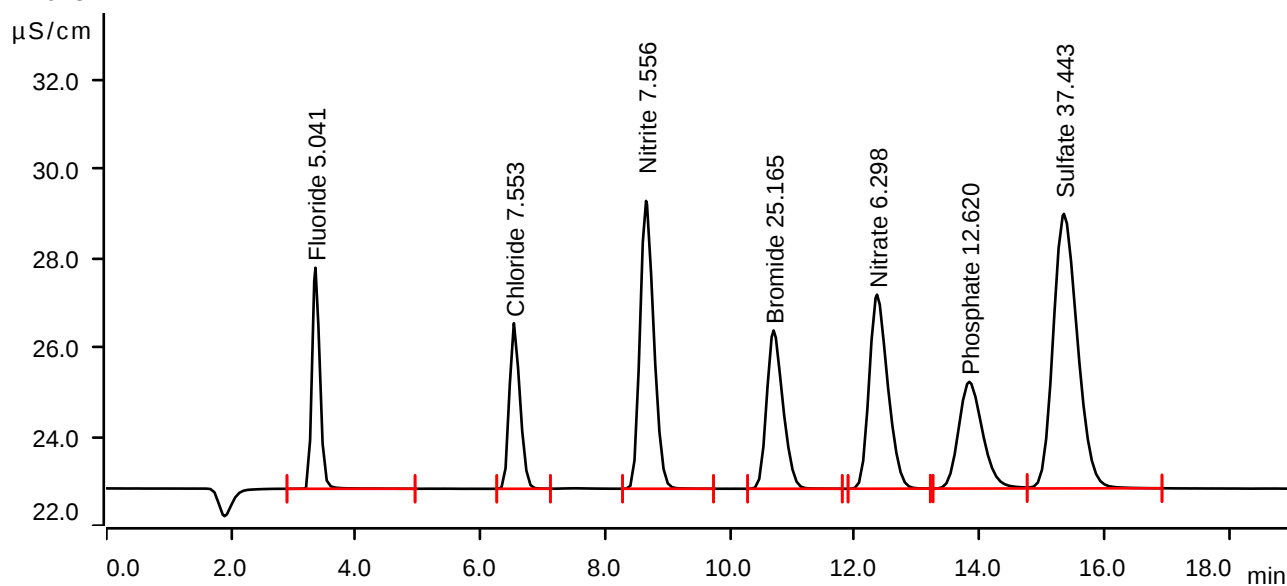

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.7226	4.963	5.041	Fluoride
2	6.535	0.7366	3.716	7.553	Chloride
3	8.653	1.6550	6.462	7.556	Nitrite
4	10.698	1.0740	3.554	25.165	Bromide
5	12.357	1.5086	4.357	6.298	Nitrate
6	13.835	1.0700	2.396	12.620	Phosphate
7	15.353	2.7786	6.163	37.443	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-08-06 12:48:56 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

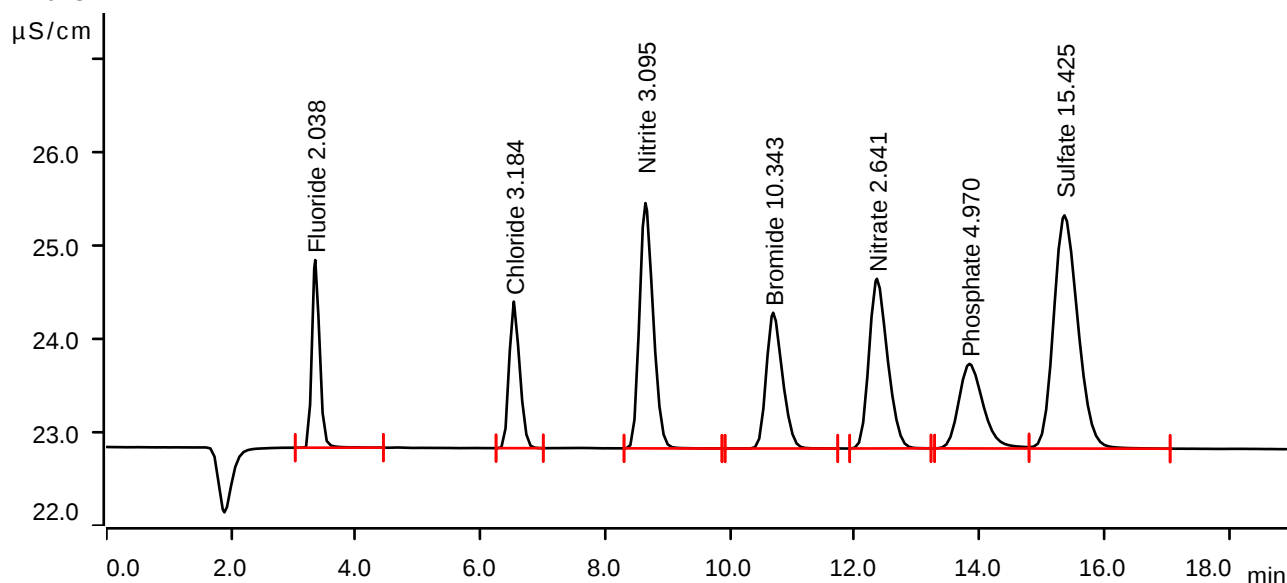


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.2890	2.015	2.038	Fluoride
2	6.532	0.3085	1.574	3.184	Chloride
3	8.643	0.6711	2.634	3.095	Nitrite
4	10.692	0.4387	1.458	10.343	Bromide
5	12.355	0.6270	1.822	2.641	Nitrate
6	13.838	0.4136	0.908	4.970	Phosphate
7	15.362	1.1289	2.504	15.425	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-08-06 13:10:25 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

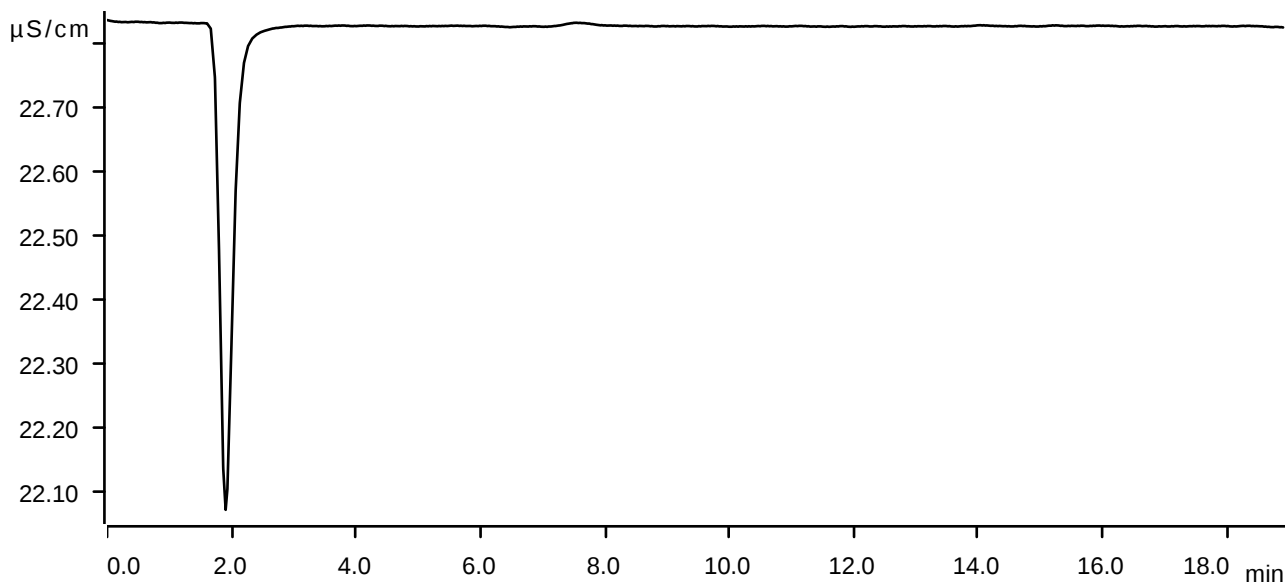Anions


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-08-07 09:06:49 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 13.01 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

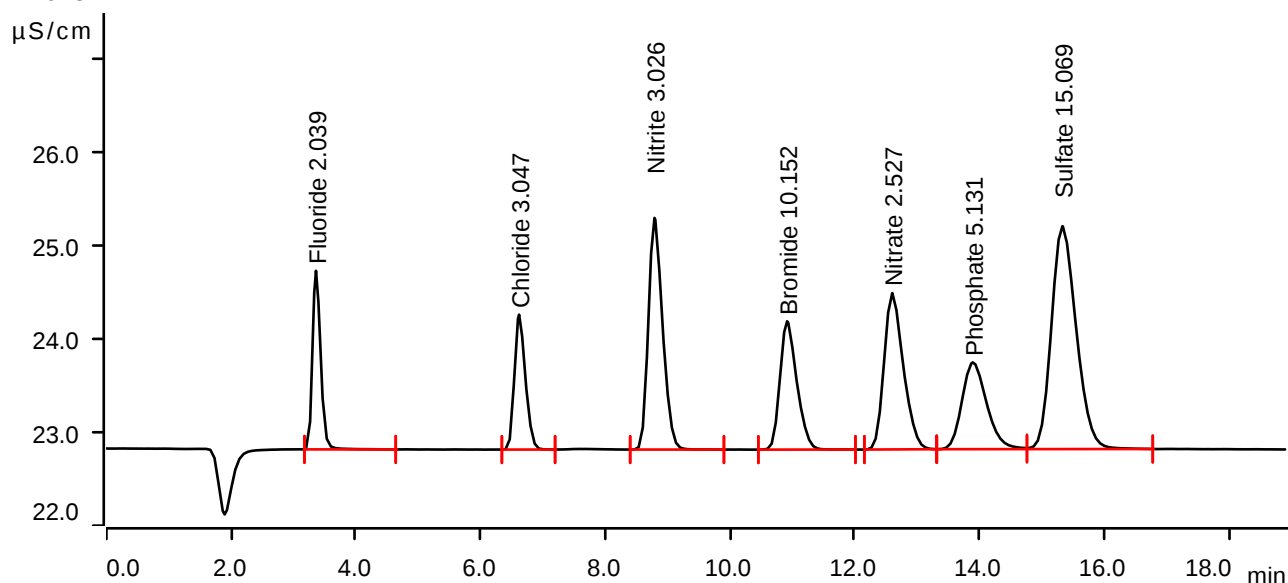


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2891	1.918	2.039	Fluoride
2	6.618	0.2951	1.449	3.047	Chloride
3	8.788	0.6559	2.488	3.026	Nitrite
4	10.915	0.4306	1.378	10.152	Bromide
5	12.600	0.5994	1.678	2.527	Nitrate
6	13.893	0.4274	0.932	5.131	Phosphate
7	15.328	1.1023	2.394	15.069	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-07 09:28:20 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.89 MPa
Maximum pressure monitored yes
Temperature ---- °C

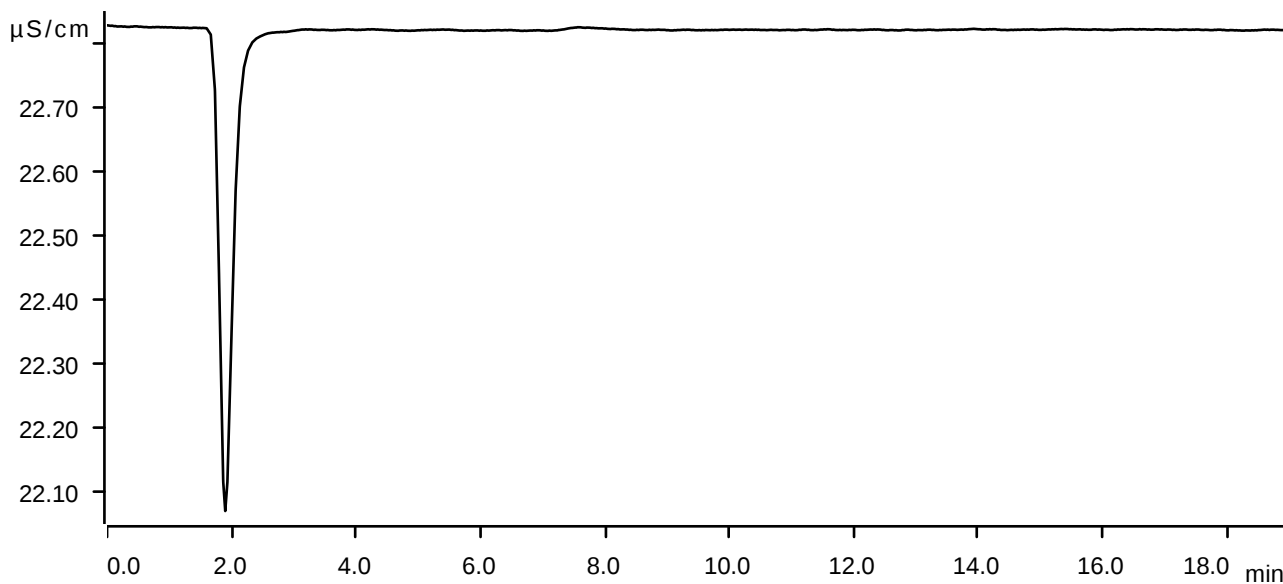
Anions

Sample data

Ident LB136743BLS
Sample type Sample
Determination start 2025-08-07 09:49:51 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.78 MPa
Maximum pressure monitored yes
Temperature ---- °C

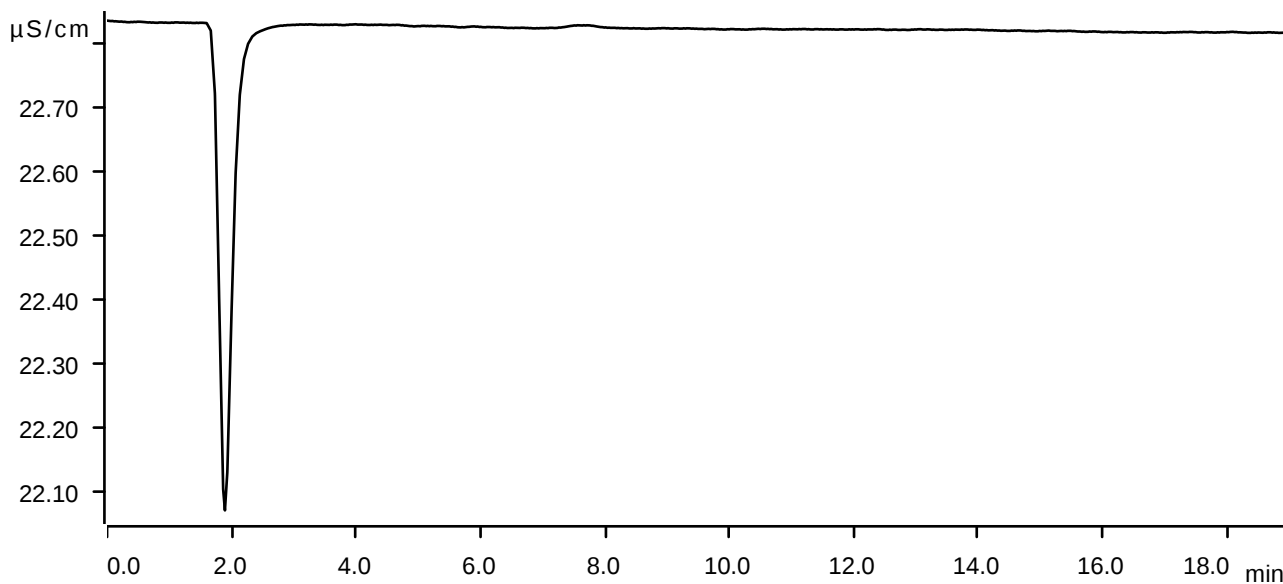Anions


Sample data

Ident LB136743BSS
 Sample type Check standard 1
 Determination start 2025-08-07 10:11:22 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.84 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

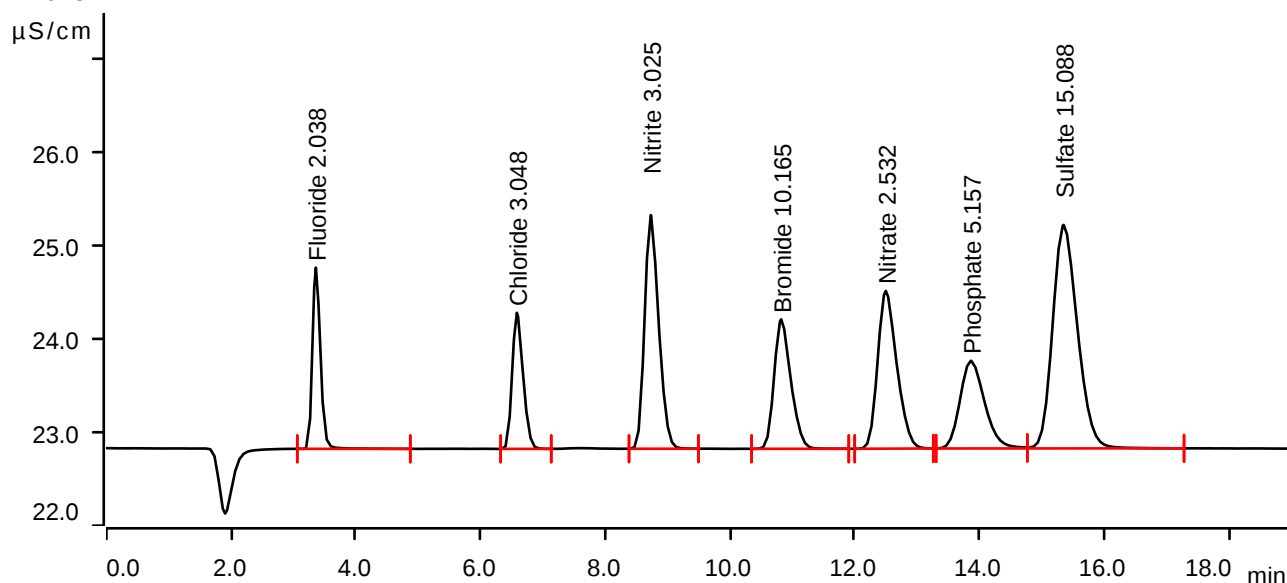

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.2890	1.945	2.038	Fluoride
2	6.582	0.2952	1.462	3.048	Chloride
3	8.728	0.6556	2.509	3.025	Nitrite
4	10.820	0.4311	1.391	10.165	Bromide
5	12.497	0.6007	1.694	2.532	Nitrate
6	13.860	0.4296	0.942	5.157	Phosphate
7	15.348	1.1037	2.400	15.088	Sulfate


Sample data

Ident Q2795-01
Sample type Sample
Determination start 2025-08-07 13:56:55 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.84 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

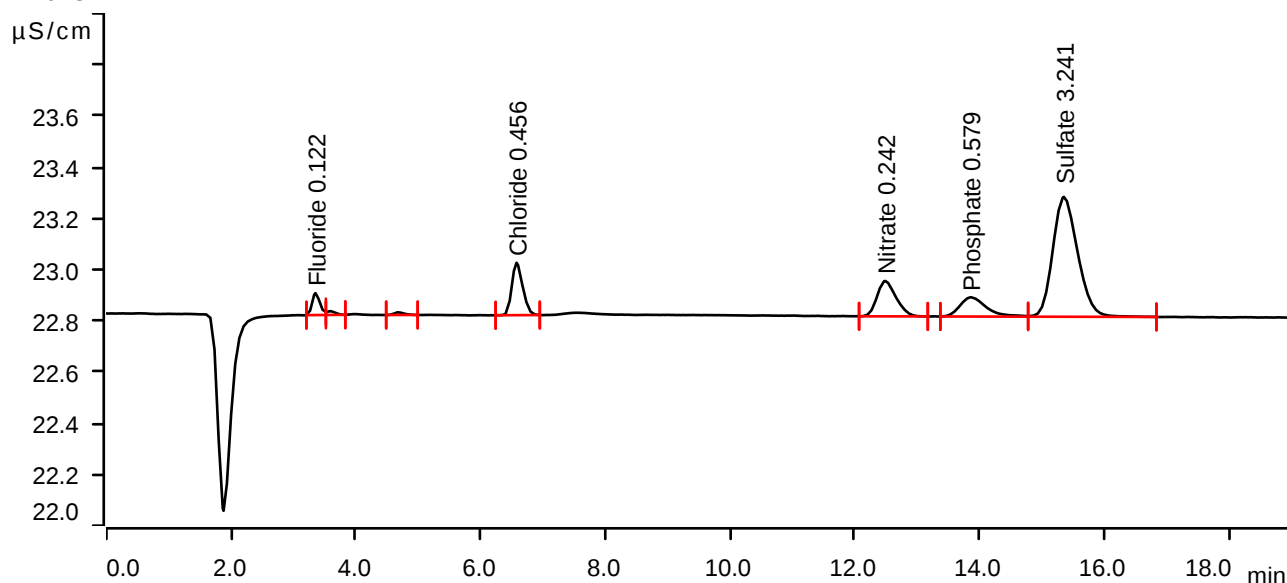


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.0124	0.086	0.122	Fluoride
2	3.593	0.0024	0.015	invalid	
3	4.678	0.0019	0.010	invalid	
4	6.577	0.0412	0.205	0.456	Chloride
5	12.488	0.0487	0.138	0.242	Nitrate
6	13.850	0.0368	0.075	0.579	Phosphate
7	15.352	0.2160	0.468	3.241	Sulfate

Sample data

Ident Q2795-01MS
 Sample type Sample
 Determination start 2025-08-07 14:18:33 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.61 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

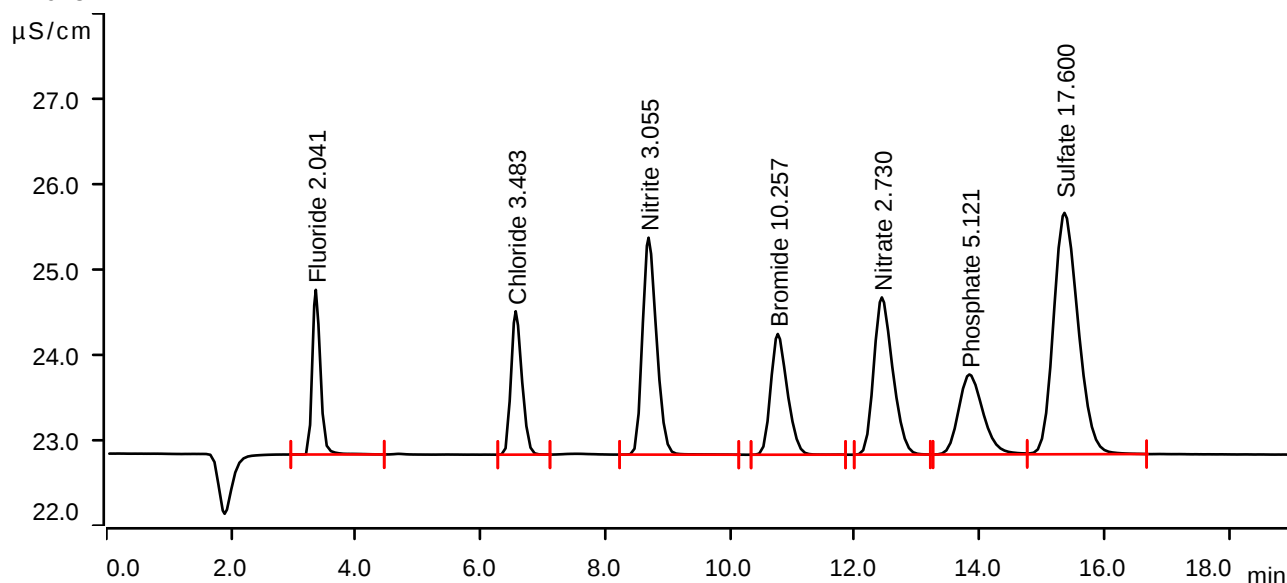Anions

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.2894	1.928	2.041	Fluoride
2	6.563	0.3378	1.680	3.483	Chloride
3	8.693	0.6622	2.541	3.055	Nitrite
4	10.765	0.4350	1.414	10.257	Bromide
5	12.433	0.6484	1.842	2.730	Nitrate
6	13.838	0.4266	0.937	5.121	Phosphate
7	15.362	1.2919	2.828	17.600	Sulfate


Sample data

Ident Q2795-01MSD
Sample type Sample
Determination start 2025-08-07 14:40:07 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.56 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

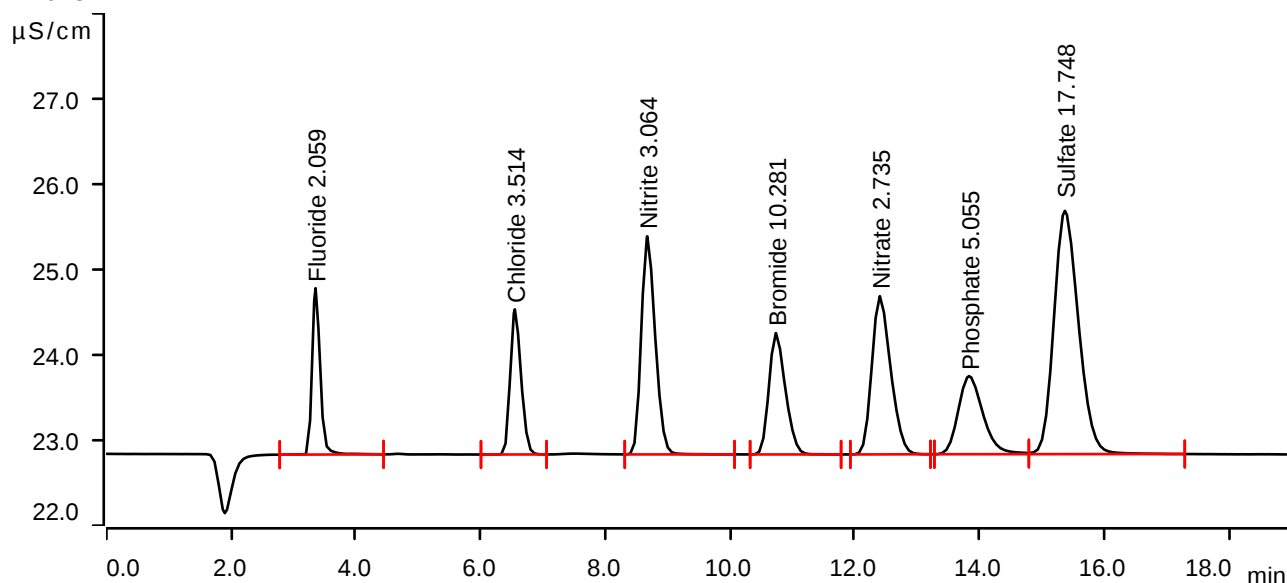

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2921	1.948	2.059	Fluoride
2	6.550	0.3408	1.700	3.514	Chloride
3	8.673	0.6641	2.555	3.064	Nitrite
4	10.737	0.4360	1.421	10.281	Bromide
5	12.402	0.6498	1.853	2.735	Nitrate
6	13.832	0.4209	0.915	5.055	Phosphate
7	15.368	1.3030	2.849	17.748	Sulfate


Sample data

Ident Q2795-02
Sample type Sample
Determination start 2025-08-07 15:01:43 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

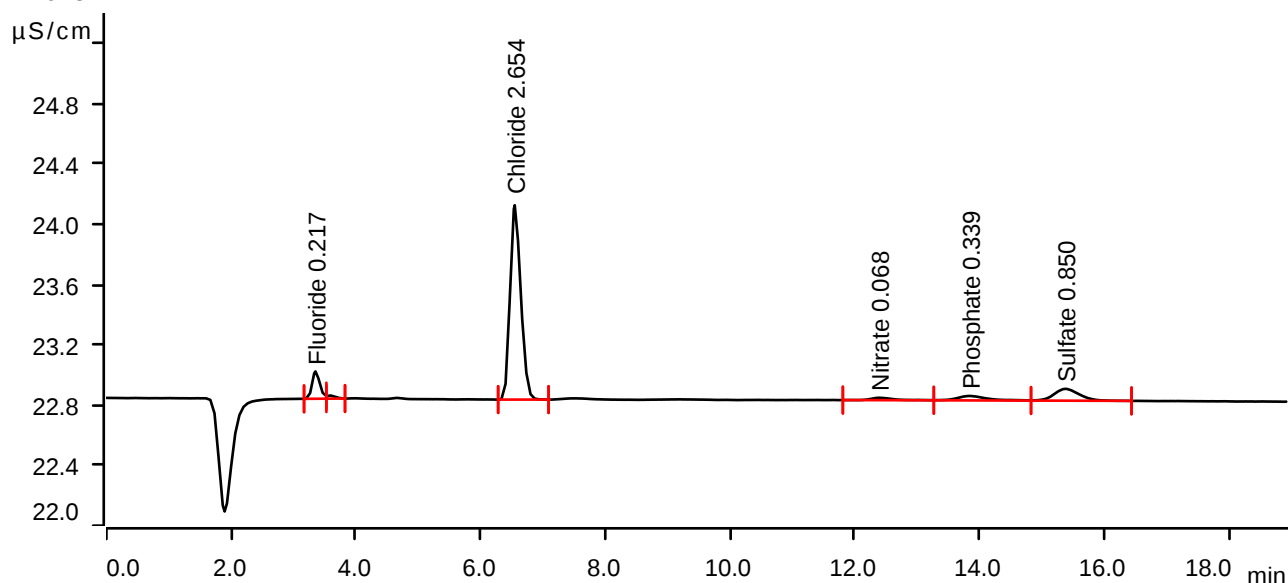

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.0261	0.181	0.217	Fluoride
2	3.593	0.0032	0.021	invalid	
3	6.548	0.2566	1.290	2.654	Chloride
4	12.385	0.0068	0.016	0.068	Nitrate
5	13.842	0.0162	0.030	0.339	Phosphate
6	15.370	0.0369	0.078	0.850	Sulfate


Sample data

Ident Q2795-03
Sample type Sample
Determination start 2025-08-07 15:23:21 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

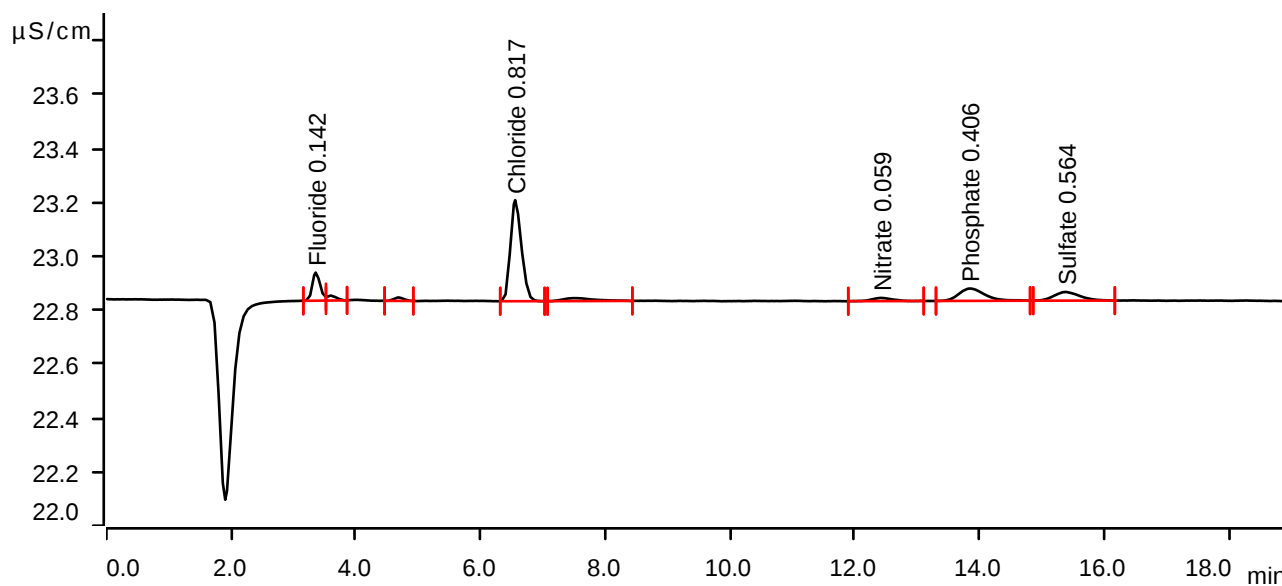

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0154	0.104	0.142	Fluoride
2	3.598	0.0032	0.018	invalid	
3	4.687	0.0023	0.013	invalid	
4	6.555	0.0765	0.375	0.817	Chloride
5	7.500	0.0062	0.011	invalid	
6	12.423	0.0046	0.012	0.059	Nitrate
7	13.833	0.0220	0.046	0.406	Phosphate
8	15.387	0.0155	0.032	0.564	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-08-07 15:44:56 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

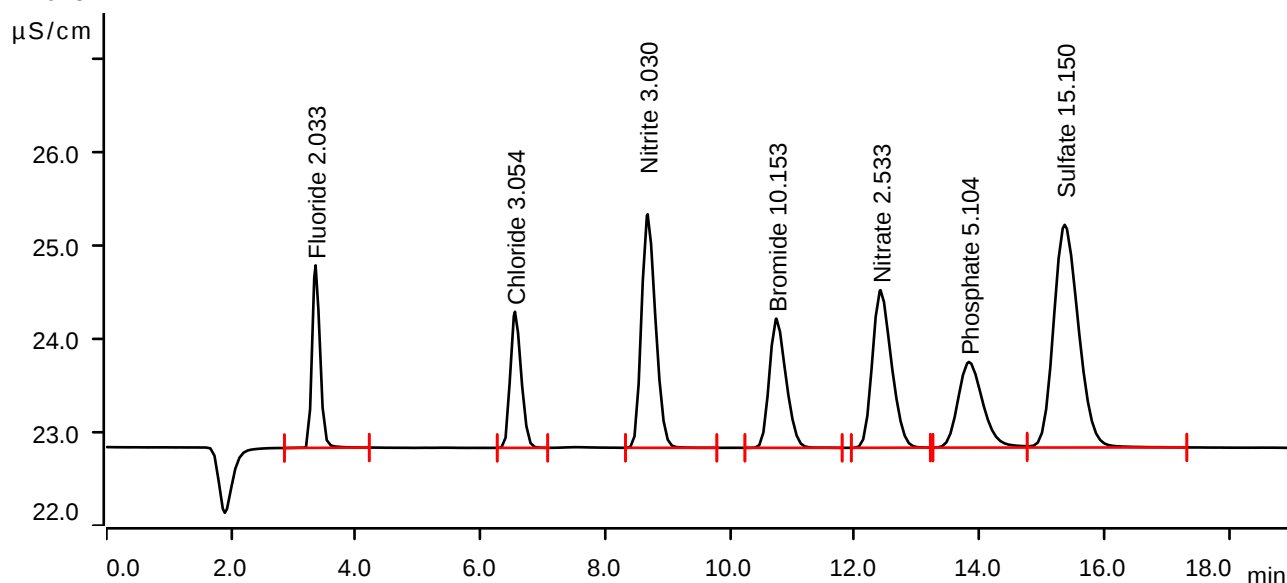

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.2883	1.959	2.033	Fluoride
2	6.552	0.2957	1.462	3.054	Chloride
3	8.678	0.6568	2.508	3.030	Nitrite
4	10.743	0.4306	1.387	10.153	Bromide
5	12.412	0.6010	1.692	2.533	Nitrate
6	13.830	0.4251	0.920	5.104	Phosphate
7	15.365	1.1083	2.392	15.150	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-08-07 16:06:26 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions