

LB136768 INSTRUMENT ID:CV1

Method: 7471B

Operator: Admin

Date of Analysis: 11 Aug 2025 09:48:30

Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50.0	-	-23	PPB	Std	0.0000	7471B	11 Aug 2025 09:58:05
S	0.2 - 1	50.2	-	514	PPB	Std	0.2000	7471B	11 Aug 2025 10:10:37
S	2.5 - 1	52.5	-	12153	PPB	Std	2.5000	7471B	11 Aug 2025 10:19:34
S	5.0 - 1	55.0	-	23326	PPB	Std	5.0000	7471B	11 Aug 2025 10:25:28
S	7.5 - 1	57.5	-	37047	PPB	Std	7.5000	7471B	11 Aug 2025 10:27:44
S	10.0 - 1	510.0	-	49186	PPB	Std	10.0000	7471B	11 Aug 2025 10:30:04
U	ICV06 - 1	ICV06	3.6938	17865	PPB	SMPL	-7471B		11 Aug 2025 10:33:10
U	ICB06 - 1	ICB06	0.0045	-371	PPB	SMPL	-7471B		11 Aug 2025 10:35:28
U	CCV15 - 1	CCV15	5.1611	25118	PPB	SMPL	-7471B		11 Aug 2025 11:06:26
U	CCB15 - 1	CCB15	-0.0035	-411	PPB	SMPL	-7471B		11 Aug 2025 11:08:43
U	CRA - 1	CRA	0.2073	631	PPB	SMPL	-7471B		11 Aug 2025 11:11:02
U	HighStd - 1	HighStd	10.1378	49718	PPB	SMPL	-7471B		11 Aug 2025 11:16:27
U	ChkStd - 1	ChkStd	7.4047	36208	PPB	SMPL	-7471B		11 Aug 2025 11:25:06
U	PB169179BL - 1	PB169179BL	-0.0222	-503	PPB	SMPL	-7471B		11 Aug 2025 11:27:22
U	PB169179BS - 1	PB169179BS	3.7656	18220	PPB	SMPL	-7471B		11 Aug 2025 11:29:44
U	Q2779-01 - 1	TP-4	3.1931	15390	PPB	SMPL	-7471B		11 Aug 2025 11:32:01
U	Q2779-05 - 1	TP-5	48.2140	237929	PPB	SMPL	-7471B		11 Aug 2025 11:34:21
U	Q2788-01 - 1	OK-01-08062025	0.4680	1920	PPB	SMPL	-7471B		11 Aug 2025 11:36:41
U	Q2793-01 - 1	VNJ-231	1.1648	5364	PPB	SMPL	-7471B		11 Aug 2025 11:39:40
U	Q2795-01 - 1	COMP-1	32.0247	157905	PPB	SMPL	-7471B		11 Aug 2025 11:41:57
U	CCV16 - 1	CCV16	5.2702	25657	PPB	SMPL	-7471B		11 Aug 2025 11:53:19
U	CCB16 - 1	CCB16	-0.0070	-428	PPB	SMPL	-7471B		11 Aug 2025 11:55:37
U	Q2795-02 - 1	COMP-2	33.9834	167587	PPB	SMPL	-7471B		11 Aug 2025 11:57:56
U	Q2795-03 - 1	COMP-3	22.4306	110481	PPB	SMPL	-7471B		11 Aug 2025 12:00:11
U	Q2798-01 - 1	TP-6	0.5443	2297	PPB	SMPL	-7471B		11 Aug 2025 12:03:06
U	Q2800-01 - 1	VNJ-222	1.5763	7398	PPB	SMPL	-7471B		11 Aug 2025 12:05:51
U	Q2801-01 - 1	TR-04-080725	0.4593	1877	PPB	SMPL	-7471B		11 Aug 2025 12:08:08
U	Q2807-01 - 1	COMP-4	10.7757	52871	PPB	SMPL	-7471B		11 Aug 2025 12:10:27
U	Q2807-02 - 1	COMP-5	13.9734	68677	PPB	SMPL	-7471B		11 Aug 2025 12:12:46
U	Q2807-03 - 1	COMP-6	16.1380	79377	PPB	SMPL	-7471B		11 Aug 2025 12:15:19
U	Q2807-03DUP - 1	COMP-6DUP	11.5538	56717	PPB	SMPL	-7471B		11 Aug 2025 12:17:55
U	Q2807-03MS - 1	COMP-6MS	15.9104	78252	PPB	SMPL	-7471B		11 Aug 2025 12:24:29
U	CCV17 - 1	CCV17	4.8967	23811	PPB	SMPL	-7471B		11 Aug 2025 12:26:46
U	CCB17 - 1	CCB17	-0.0112	-449	PPB	SMPL	-7471B		11 Aug 2025 12:29:22
U	Q2807-03MSD - 1	COMP-6MSD	16.2050	79708	PPB	SMPL	-7471B		11 Aug 2025 12:39:34
U	Q2807-03LX5 - 1		1.0745	4918	PPB	SMPL	-7471B		11 Aug 2025 12:41:49
U	Q2807-03A - 1		3.7980	18380	PPB	SMPL	-7471B		11 Aug 2025 12:44:22
U	PB169125BL - 1	PB169125BL	0.0810	7	PPB	SMPL	-7471B		11 Aug 2025 13:02:06
U	PB169125BS - 1	PB169125BS	4.2012	20373	PPB	SMPL	-7471B		11 Aug 2025 13:04:22
U	Q2779-05DXL50 - 1		17.7781	87484	PPB	SMPL	-7471B		11 Aug 2025 13:14:18
U	Q2795-01DXL10 - 1		7.1724	35060	PPB	SMPL	-7471B		11 Aug 2025 13:17:40
U	Q2795-02DXL10 - 1		6.3669	31078	PPB	SMPL	-7471B		11 Aug 2025 13:20:04
U	Q2795-03DXL10 - 1		3.8152	18465	PPB	SMPL	-7471B		11 Aug 2025 13:22:52
U	Q2807-01DXL10 - 1		4.7438	23055	PPB	SMPL	-7471B		11 Aug 2025 13:25:28
U	CCV18 - 1	CCV18	5.0683	24659	PPB	SMPL	-7471B		11 Aug 2025 13:32:34
U	CCB18 - 1	CCB18	-0.0094	-440	PPB	SMPL	-7471B		11 Aug 2025 13:34:49
U	Q2807-02DXL10 - 1		1.8997	8997	PPB	SMPL	-7471B		11 Aug 2025 13:37:09
U	Q2807-03DXL10 - 1		2.8585	13736	PPB	SMPL	-7471B		11 Aug 2025 13:39:25
U	Q2807-03DUPDXL10 - 1		2.4146	11542	PPB	SMPL	-7471B		11 Aug 2025 13:41:43
U	Q2807-03MSDDXL10 - 1		2.1963	10463	PPB	SMPL	-7471B		11 Aug 2025 13:44:01
U	Q2779-05DXL50DXL10 - 1		2.6552	12731	PPB	SMPL	-7471B		11 Aug 2025 13:46:21
U	Q2807-03DXL10 - 1		2.5344	12134	PPB	SMPL	-7471B		11 Aug 2025 13:54:34
U	CCV19 - 1	CCV19	5.0296	24468	PPB	SMPL	-7471B		11 Aug 2025 13:56:50
U	CCB19 - 1	CCB19	-0.0068	-427	PPB	SMPL	-7471B		11 Aug 2025 13:59:10

LB136768


INSTRUMENT ID: CV1

Reviewed By: jaswal
On: 8/12/2025 4:00:23 PM
Inst Id: CV1
LB: LB136768

7471B

μ Abs.:

4918E

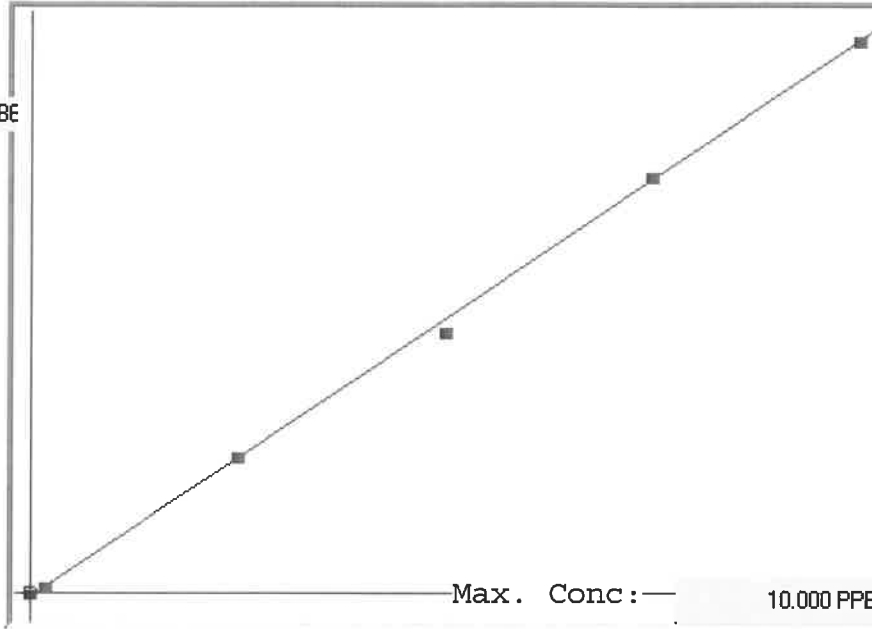

Linear

A= 0.0000e+000

B= 2.0231e-004

C= 7.9603e-002

Rho= 0.9996672

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	0.075	0.075	-23	0.000	-23					-8
0.2	0.200	0.184	-0.016	514	0.0 %	514					2
2.5	2.500	2.538	0.038	12153	0.0 %	12153					-4
5.0	5.000	4.799	-0.201	23326	0.0 %	23326					1
7.5	7.500	7.574	0.074	37047	0.0 %	37047					0
10.0	10.000	10.030	0.030	49186	0.0 %	49186					