

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

Value	If the result is a value greater than or equal to the detection limit, report the value
U	Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
ND	Indicates the analyte was analyzed for, but not detected
J	Indicates an estimated value. This flag is used: (1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.) (2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
B	Indicates the analyte was found in the blank as well as the sample report as "12 B".
E	Indicates the analyte 's concentration exceeds the calibrated range of the instrument for that specific analysis.
D	This flag identifies all compounds identified in an analysis at a secondary dilution factor.
P	This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
N	This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
A	This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
Q	Indicates the LCS did not meet the control limits requirements

LAB CHRONICLE

OrderID:	Q2795	OrderDate:	8/7/2025 11:57:00 AM
Client:	Kleinfelder	Project:	Girard school
Contact:	Mark Warchol	Location:	D31,VOA Ref. #2 Soil

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2795-01	COMP-1	SOIL	PESTICIDE Group1	8081B	08/06/25	08/08/25	08/08/25	08/07/25
Q2795-02	COMP-2	SOIL	PESTICIDE Group1	8081B	08/06/25	08/08/25	08/08/25	08/07/25
Q2795-03	COMP-3	SOIL	PESTICIDE Group1	8081B	08/06/25	08/08/25	08/08/25	08/07/25



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Hit Summary Sheet
SW-846

SDG No.: Q2795

Order ID: Q2795

Client: Kleinfelder

Project ID: Girard school

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	RDL	Units
-----------	-----------	--------	-----------	---------------	---	-----	-----	-------

Client ID :

Total Concentration: 0.000



QC SUMMARY

Surrogate Summary

SDG No.: Q2795

Client: Kleinfelder

Analytical Method: 8081B

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PD089685.D	PIBLK-PD089685.D	Decachlorobiphen	1	20	20.9	104		57	171
		Tetrachloro-m-xyl	1	20	19.6	98		61	148
		Decachlorobiphen	2	20	20.9	104		57	171
		Tetrachloro-m-xyl	2	20	20.4	102		61	148
I.BLK-PD089808.D	PIBLK-PD089808.D	Decachlorobiphen	1	20	23.2	116		57	171
		Tetrachloro-m-xyl	1	20	22.9	115		61	148
		Decachlorobiphen	2	20	20.8	104		57	171
		Tetrachloro-m-xyl	2	20	26.1	130		61	148
PB169173BL	PB169173BL	Decachlorobiphen	1	20	18.4	92		20	144
		Tetrachloro-m-xyl	1	20	18.5	93		19	148
		Decachlorobiphen	2	20	18.9	95		20	144
		Tetrachloro-m-xyl	2	20	21.8	109		19	148
PB169173BS	PB169173BS	Decachlorobiphen	1	20	18.6	93		20	144
		Tetrachloro-m-xyl	1	20	18.5	92		19	148
		Decachlorobiphen	2	20	19.5	98		20	144
		Tetrachloro-m-xyl	2	20	22.2	111		19	148
I.BLK-PD089820.D	PIBLK-PD089820.D	Decachlorobiphen	1	20	21.2	106		57	171
		Tetrachloro-m-xyl	1	20	22.3	112		61	148
		Decachlorobiphen	2	20	22.2	111		57	171
		Tetrachloro-m-xyl	2	20	26.1	131		61	148
Q2795-01	COMP-1	Decachlorobiphen	1	20	14.7	74		20	144
		Tetrachloro-m-xyl	1	20	19.6	98		19	148
		Decachlorobiphen	2	20	15.7	78		20	144
		Tetrachloro-m-xyl	2	20	23.0	115		19	148
Q2795-01MS	COMP-1MS	Decachlorobiphen	1	20	12.8	64		20	144
		Tetrachloro-m-xyl	1	20	16.3	81		19	148
		Decachlorobiphen	2	20	13.4	67		20	144
		Tetrachloro-m-xyl	2	20	19.2	96		19	148
Q2795-01MSD	COMP-1MSD	Decachlorobiphen	1	20	12.9	64		20	144
		Tetrachloro-m-xyl	1	20	16.2	81		19	148
		Decachlorobiphen	2	20	13.2	66		20	144
		Tetrachloro-m-xyl	2	20	19.2	96		19	148
Q2795-02	COMP-2	Decachlorobiphen	1	20	16.4	82		20	144
		Tetrachloro-m-xyl	1	20	21.4	107		19	148
		Decachlorobiphen	2	20	17.0	85		20	144
		Tetrachloro-m-xyl	2	20	24.7	123		19	148
Q2795-03	COMP-3	Decachlorobiphen	1	20	17.0	85		20	144
		Tetrachloro-m-xyl	1	20	20.9	104		19	148
		Decachlorobiphen	2	20	17.2	86		20	144
		Tetrachloro-m-xyl	2	20	24.2	121		19	148
I.BLK-PD089828.D	PIBLK-PD089828.D	Decachlorobiphen	1	20	21.0	105		57	171

Surrogate Summary

SDG No.: Q2795

Client: Kleinfelder

Analytical Method: 8081B

Lab Sample ID	Client ID	Parameter	Column	Spike	Result	Recovery(%)	Qual	Limits(%)	
								Low	High
I.BLK-PD089828.D	PIBLK-PD089828.D	Tetrachloro-m-xyl	1	20	22.5	112		61	148
		Decachlorobiphen	2	20	21.1	106		57	171
		Tetrachloro-m-xyl	2	20	26.6	133		61	148

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.:	<u>Q2795</u>	Analytical Method:	<u>8081B</u>
Client:	<u>Kleinfelder</u>	DataFile :	<u>PD089823.D</u>

	Parameter	Spike	Sample		Units	Rec	Rec		RPD		Limits	
			Result	Result			Qual	RPD	Qual	Low	High	RPD
Lab Sample ID:	Q2795-01MS (Column 1)	Client Sample ID:		COMP-1MS								
	Aldrin	20.16	0	20.2	ug/kg	100				49	139	
	Dieldrin	20.16	0	17.6	ug/kg	87				47	161	
	4,4'-DDE	20.16	0	19.2	ug/kg	95				55	136	
	4,4'-DDD	20.16	0	19.7	ug/kg	98				47	163	
	4,4'-DDT	20.16	0	13.8	ug/kg	68				51	146	
Lab Sample ID:	Q2795-01MS (Column 2)	Client Sample ID:		COMP-1MS								
	Aldrin	20.16	0	22.6	ug/kg	112				49	139	
	Dieldrin	20.16	0	20.9	ug/kg	104				47	161	
	4,4'-DDE	20.16	0	22.5	ug/kg	112				55	136	
	4,4'-DDD	20.16	0	22.1	ug/kg	110				47	163	
	4,4'-DDT	20.16	0	18.1	ug/kg	90				51	146	

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.:	<u>Q2795</u>	Analytical Method:	<u>8081B</u>
Client:	<u>Kleinfelder</u>	DataFile :	<u>PD089824.D</u>

	Parameter	Spike	Sample		Units	Rec	Rec	RPD		Limits		
			Result	Result			Qual	RPD	Qual	Low	High	RPD
Lab Sample ID:	Q2795-01MSD (Column 1)	Client Sample ID:		COMP-1MSD								
	Aldrin	20.18	0	20.1	ug/kg	100		0		49	139	20
	Dieldrin	20.18	0	18.7	ug/kg	93		7		47	161	20
	4,4'-DDE	20.18	0	19.5	ug/kg	97		2		55	136	20
	4,4'-DDD	20.18	0	19.9	ug/kg	99		1		47	163	20
	4,4'-DDT	20.18	0	15.5	ug/kg	77		12		51	146	20
Lab Sample ID:	Q2795-01MSD (Column 2)	Client Sample ID:		COMP-1MSD								
	Aldrin	20.18	0	22.6	ug/kg	112		0		49	139	20
	Dieldrin	20.18	0	21.9	ug/kg	109		5		47	161	20
	4,4'-DDE	20.18	0	22.3	ug/kg	111		1		55	136	20
	4,4'-DDD	20.18	0	22.0	ug/kg	109		1		47	163	20
	4,4'-DDT	20.18	0	19.7	ug/kg	98		9		51	146	20

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.:	<u>Q2795</u>	Analytical Method:	<u>8081B</u>
Client:	<u>Kleinfelder</u>	Datafile :	<u>PD089812.D</u>

Lab Sample ID	Parameter	Spike	Result	Units	Rec	RPD	Qual	RPD		Limits		RPD
								Qual	Low	High		
PB169173BS (Column 1)	Aldrin	16.66	16.0	ug/kg	96				82	124		
	Dieldrin	16.66	15.5	ug/kg	93				85	121		
	4,4'-DDE	16.66	15.6	ug/kg	94				81	123		
	4,4'-DDD	16.66	15.9	ug/kg	95				80	131		
	4,4'-DDT	16.66	13.8	ug/kg	83				70	129		
PB169173BS (Column 2)	Aldrin	16.66	17.7	ug/kg	106				82	124		
	Dieldrin	16.66	17.6	ug/kg	106				85	121		
	4,4'-DDE	16.66	17.7	ug/kg	106				81	123		
	4,4'-DDD	16.66	18.5	ug/kg	111				80	131		
	4,4'-DDT	16.66	16.4	ug/kg	98				70	129		

4C

PESTICIDE METHOD BLANK SUMMARY

Client ID

PB169173BL

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Lab Sample ID: PB169173BL

Lab File ID: PD089811.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 08/08/2025

Date Analyzed (1): 08/08/2025

Date Analyzed (2): 08/08/2025

Time Analyzed (1): 14:51

Time Analyzed (2): 14:51

Instrument ID (1): ECD_D

Instrument ID (2): ECD_D

GC Column (1): ZB-MR1 ID: 0.32 (mm)

GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

EPA SAMPLE NO.	LAB SAMPLE ID	LAB FILE ID	DATE ANALYZED 1	DATE ANALYZED 2
PB169173BS	PB169173BS	PD089812.D	08/08/2025	08/08/2025
COMP-1	Q2795-01	PD089822.D	08/08/2025	08/08/2025
COMP-1MS	Q2795-01MS	PD089823.D	08/08/2025	08/08/2025
COMP-1MSD	Q2795-01MSD	PD089824.D	08/08/2025	08/08/2025
COMP-2	Q2795-02	PD089825.D	08/08/2025	08/08/2025
COMP-3	Q2795-03	PD089826.D	08/08/2025	08/08/2025

COMMENTS: _____



SAMPLE DATA

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/06/25
Project:	Girard school	Date Received:	08/07/25
Client Sample ID:	COMP-1	SDG No.:	Q2795
Lab Sample ID:	Q2795-01	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	82.5 Decanted:
Sample Wt/Vol:	30.1 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089822.D	1	08/08/25 08:43	08/08/25 18:10	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	0.14	U	0.14	2.10	ug/kg
60-57-1	Dieldrin	0.17	U	0.17	2.10	ug/kg
72-55-9	4,4-DDE	0.17	U	0.17	2.10	ug/kg
72-54-8	4,4-DDD	0.18	U	0.18	2.10	ug/kg
50-29-3	4,4-DDT	0.17	U	0.17	2.10	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	15.7		20 - 144	78%	SPK: 20
877-09-8	Tetrachloro-m-xylene	23.0		19 - 148	115%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089822.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 18:10
 Operator : AR\AJ
 Sample : Q2795-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-1

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:35:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.876	48301486	364.1E6	19.582	22.987m
28) SA Decachlor...	9.068	8.066	54760397	314.7E6	14.735	15.676

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089822.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 18:10
Operator : AR\AJ
Sample : Q2795-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2025
Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:35:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

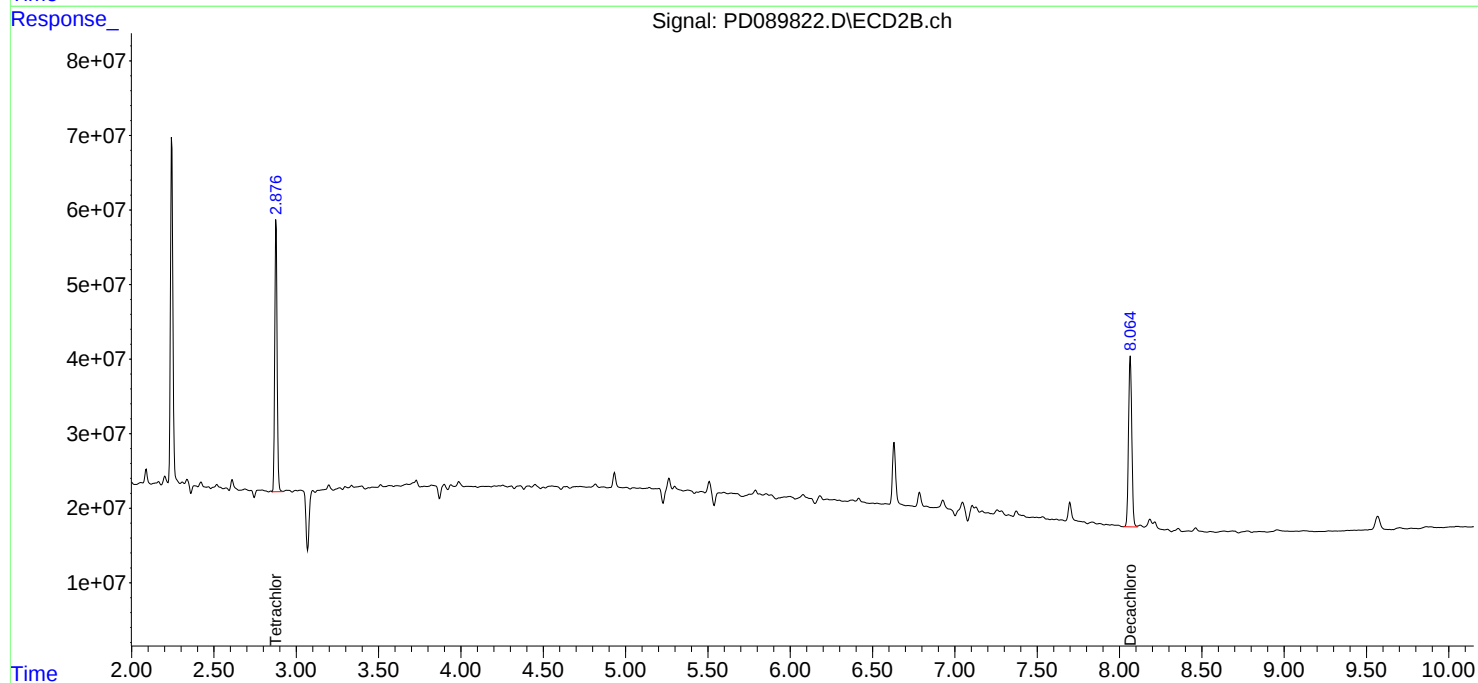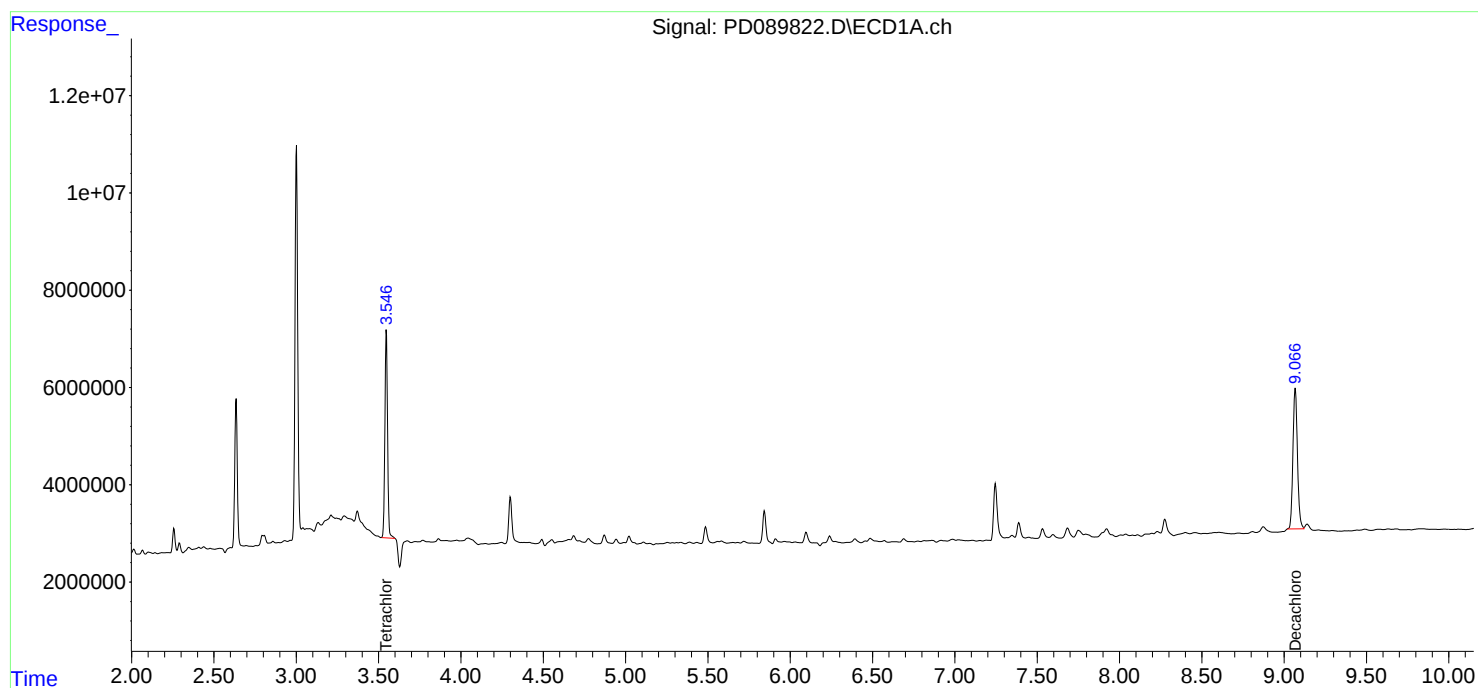

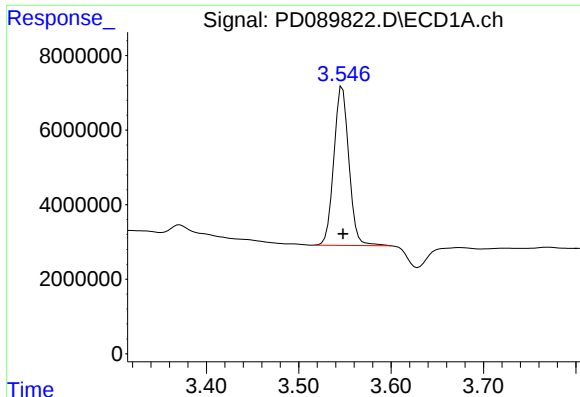


#1 Tetrachloro-m-xylene

R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 48301486
Conc: 19.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-1


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2025
Supervised By :mohammad ahmed 08/12/2025

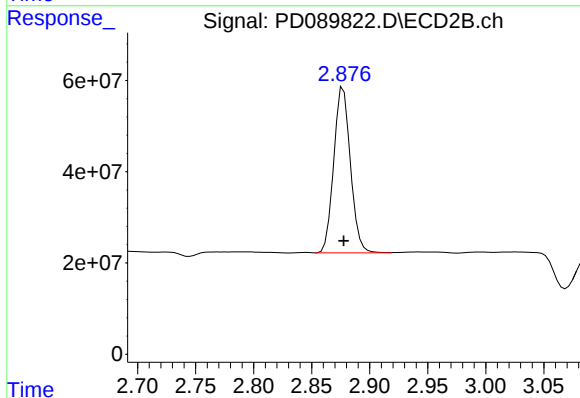


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: -0.002 min
Response: 364070770
Conc: 22.99 ng/ml m

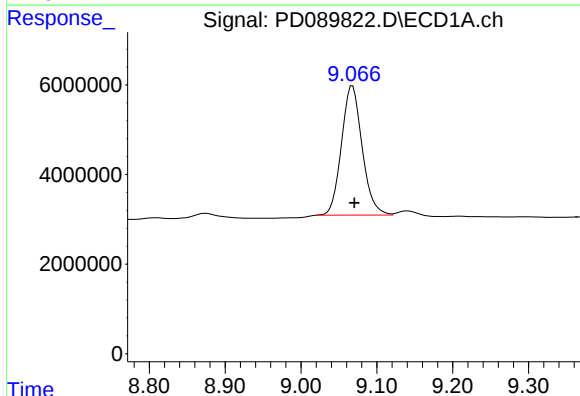

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.003 min
Response: 54760397
Conc: 14.74 ng/ml

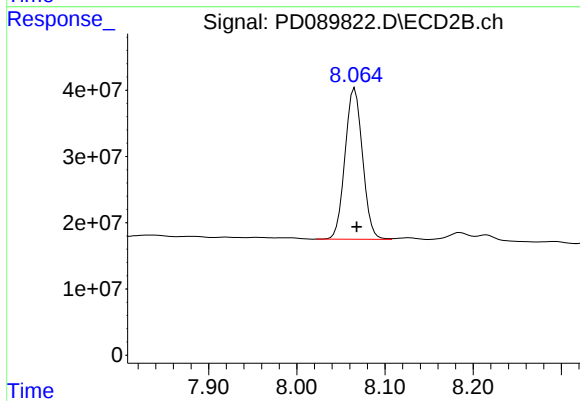

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 314743859
Conc: 15.68 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/06/25
Project:	Girard school	Date Received:	08/07/25
Client Sample ID:	COMP-2	SDG No.:	Q2795
Lab Sample ID:	Q2795-02	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	80.8 Decanted:
Sample Wt/Vol:	30.04 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089825.D	1	08/08/25 08:43	08/08/25 18:51	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	0.15	U	0.15	2.10	ug/kg
60-57-1	Dieldrin	0.17	U	0.17	2.10	ug/kg
72-55-9	4,4-DDE	0.17	U	0.17	2.10	ug/kg
72-54-8	4,4-DDD	0.19	U	0.19	2.10	ug/kg
50-29-3	4,4-DDT	0.17	U	0.17	2.10	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	17.0		20 - 144	85%	SPK: 20
877-09-8	Tetrachloro-m-xylene	24.7		19 - 148	123%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089825.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 18:51
 Operator : AR\AJ
 Sample : Q2795-02
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-2

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:36:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.876	52864526	390.8E6	21.432	24.673m
28) SA Decachlor...	9.067	8.066	60943658	341.4E6	16.399	17.002

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089825.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 18:51
Operator : AR\AJ
Sample : Q2795-02
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2025
Supervised By :mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:36:16 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

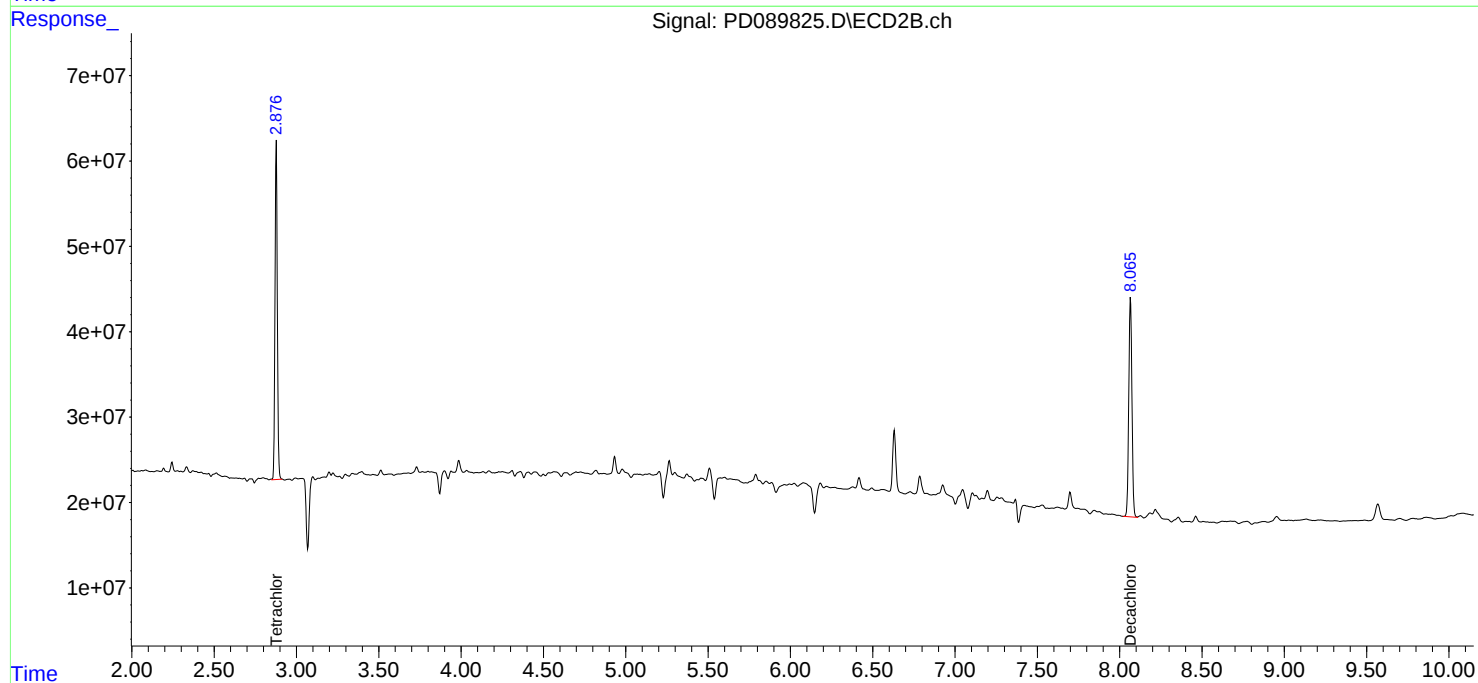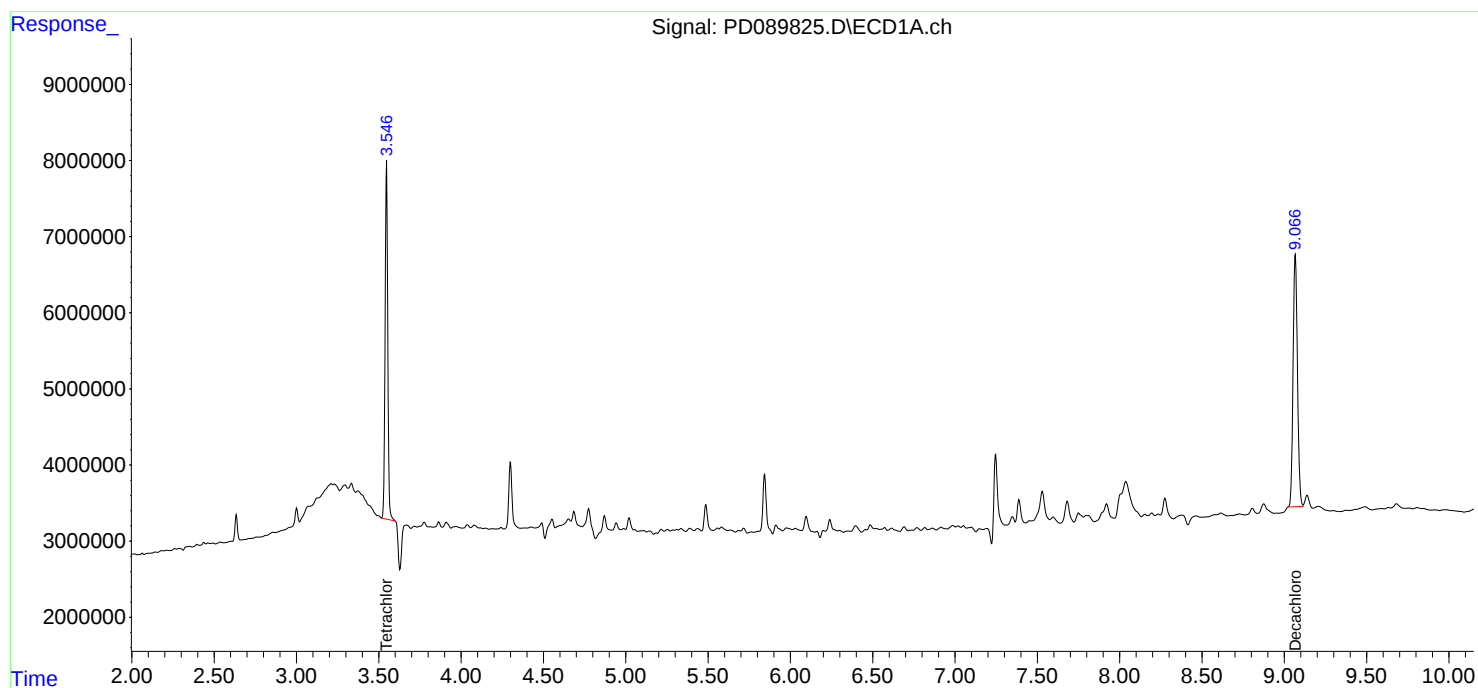

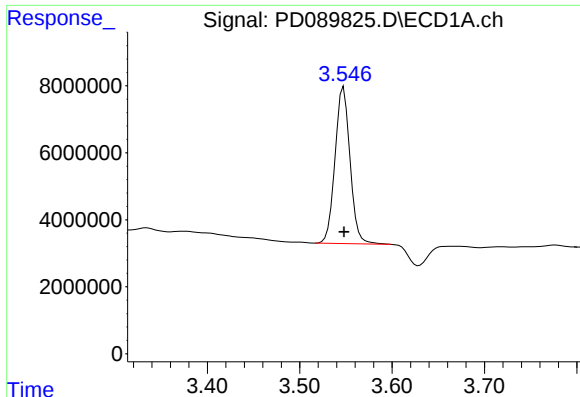


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 52864526
Conc: 21.43 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-2


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2025
Supervised By :mohammad ahmed 08/12/2025

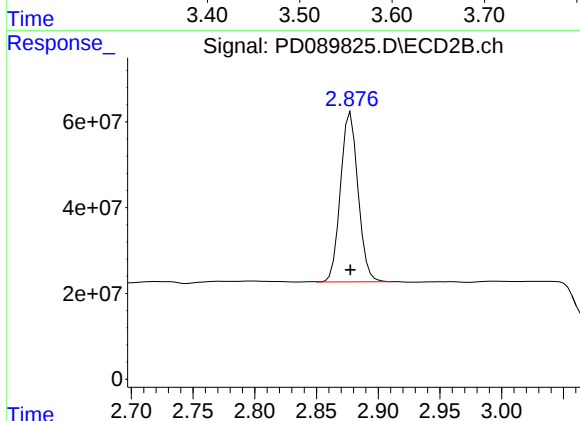


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: -0.001 min
Response: 390760603
Conc: 24.67 ng/ml m

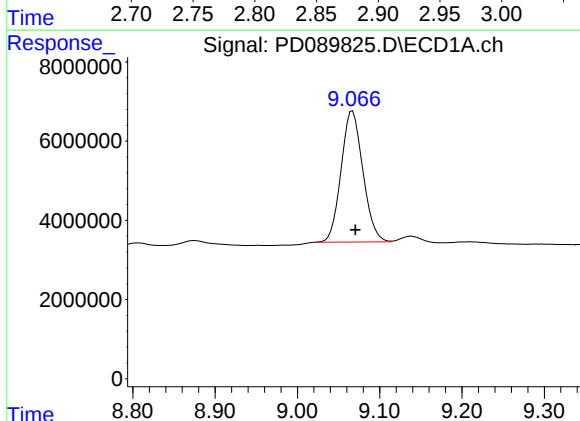

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: -0.004 min
Response: 60943658
Conc: 16.40 ng/ml

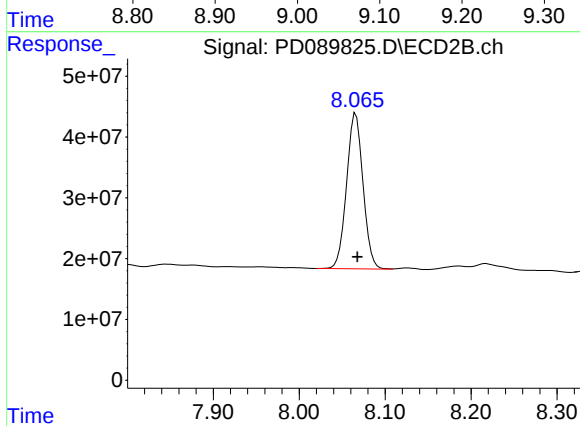

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 341368866
Conc: 17.00 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/06/25
Project:	Girard school	Date Received:	08/07/25
Client Sample ID:	COMP-3	SDG No.:	Q2795
Lab Sample ID:	Q2795-03	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	82
Sample Wt/Vol:	30.08	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PESTICIDE Group1
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089826.D	1	08/08/25 08:43	08/08/25 19:05	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	0.15	U	0.15	2.10	ug/kg
60-57-1	Dieldrin	0.17	U	0.17	2.10	ug/kg
72-55-9	4,4-DDE	0.17	U	0.17	2.10	ug/kg
72-54-8	4,4-DDD	0.18	U	0.18	2.10	ug/kg
50-29-3	4,4-DDT	0.17	U	0.17	2.10	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	17.2		20 - 144	86%	SPK: 20
877-09-8	Tetrachloro-m-xylene	24.2		19 - 148	121%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089826.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 19:05
 Operator : AR\AJ
 Sample : Q2795-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-3

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:36:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.548	2.877	51516232	383.1E6	20.886	24.191m
28) SA Decachlor...	9.067	8.065	63336406	344.6E6	17.043	17.163

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089826.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 19:05
Operator : AR\AJ
Sample : Q2795-03
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2025
Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:36:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

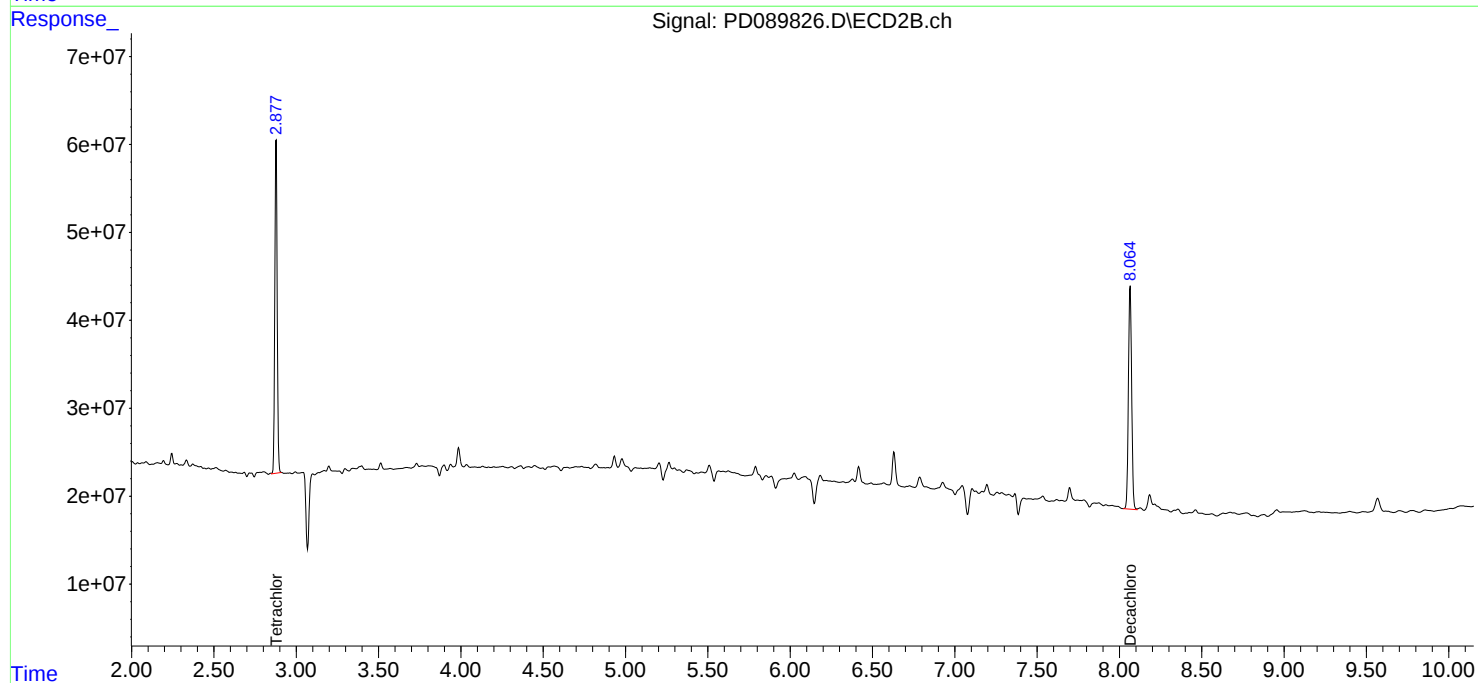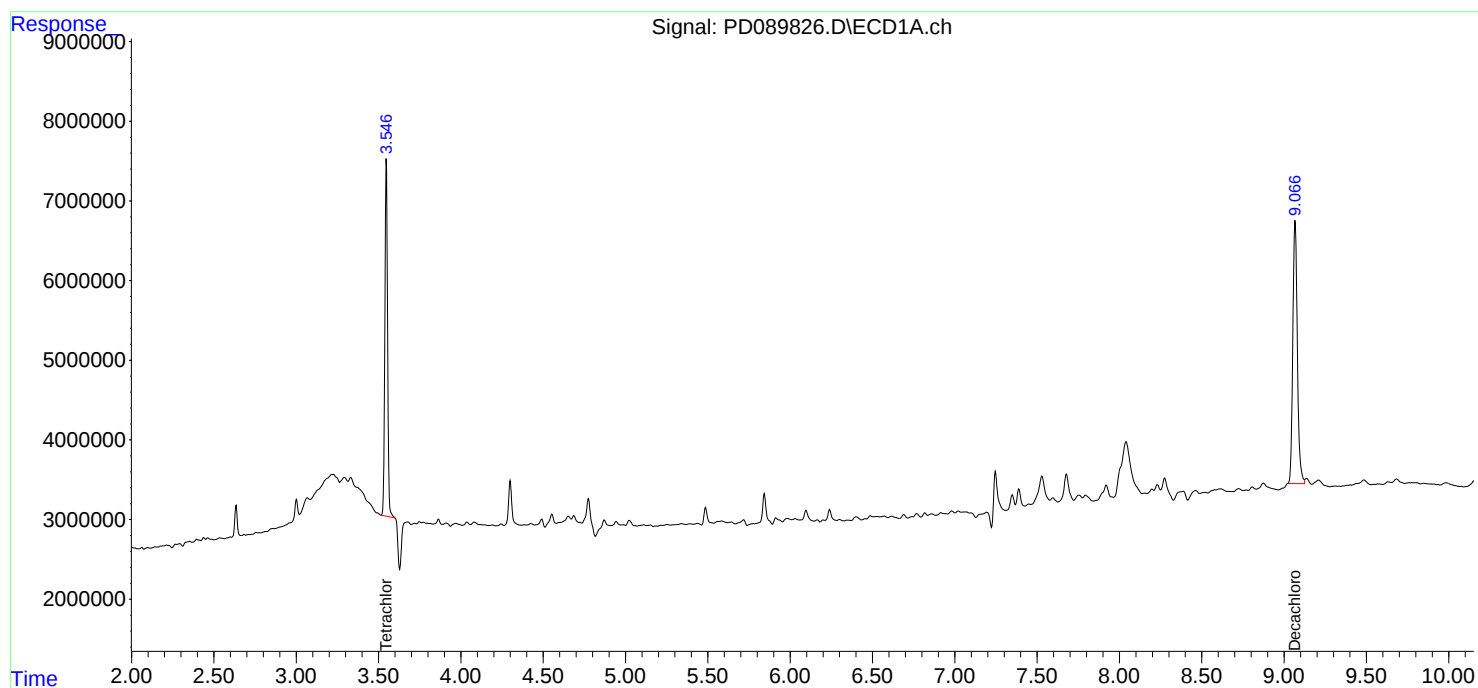

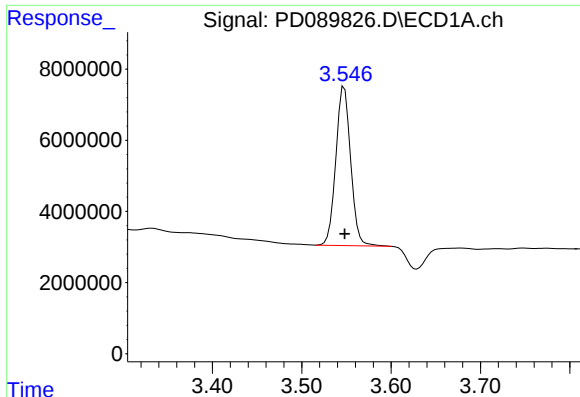


#1 Tetrachloro-m-xylene

R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 51516232
Conc: 20.89 ng/ml

Instrument :
ECD_D
ClientSampleId :
COMP-3


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/11/2025
Supervised By :mohammad ahmed 08/12/2025

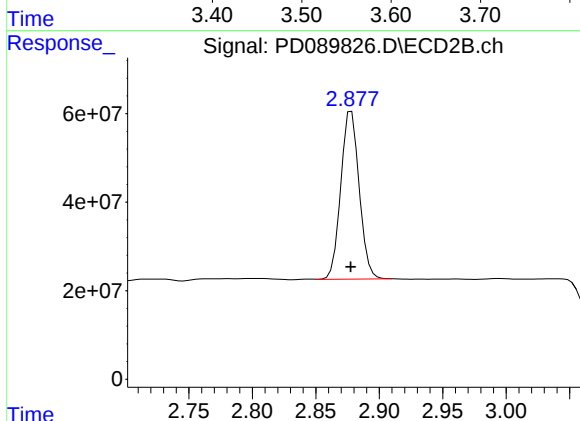


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 383134952
Conc: 24.19 ng/ml m

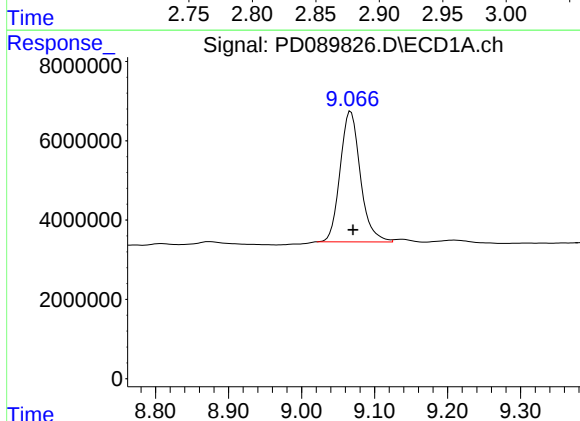

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: -0.003 min
Response: 63336406
Conc: 17.04 ng/ml

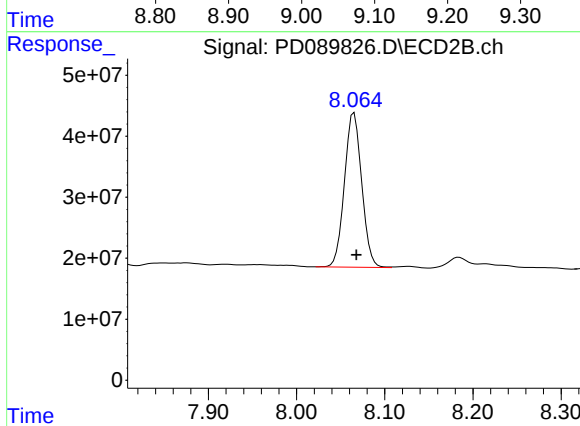

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: -0.003 min
Response: 344592716
Conc: 17.16 ng/ml



CALIBRATION SUMMARY

Calibration Times: 11:47 12:41

LAB FILE ID:	RT 100 =	<u>PD089688.D</u>	RT 075 =	<u>PD089689.D</u>
	RT 050 =	PD089690.D	RT 025 =	PD089691.D
			RT 005 =	PD089692.D

[illegible]

Calibration Times: 11:47 12:41

LAB FILE ID:	RT 100 =	<u>PD089688.D</u>	RT 075 =	<u>PD089689.D</u>
	RT 050 =	PD089690.D	RT 025 =	PD089691.D
			RT 005 =	PD089692.D

[illegible]



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Instrument ID: ECD_D

Calibration Date(s): 07/31/2025 07/31/2025

Calibration Times: 11:47 12:41

GC Column: ZB-MR1

ID: 0.32 (mm)

LAB FILE ID:		CF 100 =	<u>PD089688.D</u>	CF 075 =	<u>PD089689.D</u>		
CF 050 =		<u>PD089690.D</u>	CF 025 =	<u>PD089691.D</u>	CF 005 =	<u>PD089692.D</u>	
COMPOUND	CF 100	CF 075	CF 050	CF 025	CF 005	CF	% RSD
4,4'-DDD	3170910000	3047700000	2999940000	2847680000	2907880000	2994820000	4
4,4'-DDE	4003810000	3817790000	3749630000	3527790000	3549710000	3729750000	5
4,4'-DDT	3548070000	3416270000	3370890000	3205660000	3260320000	3360240000	4
Aldrin	4875360000	4656550000	4601860000	4327300000	4363460000	4564910000	5
Decachlorobiphenyl	3483240000	3499950000	3619460000	3726220000	4252410000	3716260000	8
Dieldrin	4482180000	4304270000	4237810000	4013690000	4079190000	4223430000	4
Tetrachloro-m-xylene	2500060000	2427080000	2456600000	2403480000	2545710000	2466590000	2



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Instrument ID: ECD_D

Calibration Date(s): 07/31/2025 07/31/2025

Calibration Times: 11:47 12:41

GC Column: ZB-MR2

ID: 0.32 (mm)

LAB FILE ID:		CF 100 =	<u>PD089688.D</u>	CF 075 =	<u>PD089689.D</u>		
CF 050 =		<u>PD089690.D</u>	CF 025 =	<u>PD089691.D</u>	CF 005 =	<u>PD089692.D</u>	
COMPOUND	CF 100	CF 075	CF 050	CF 025	CF 005	CF	% RSD
4,4'-DDD	17134400000	16787300000	17354900000	17662200000	19224300000	17632600000	5
4,4'-DDE	20430900000	20064600000	20732800000	21183800000	23273600000	21137100000	6
4,4'-DDT	18425400000	17982900000	18452700000	18412200000	18590200000	18372700000	1
Aldrin	21657100000	21218800000	21871300000	22261000000	24245900000	22250800000	5
Decachlorobiphenyl	19095200000	18752300000	19614700000	20093800000	22833900000	20078000000	8
Dieldrin	20963500000	20551400000	21238000000	21609600000	23832300000	21639000000	6
Tetrachloro-m-xylene	15162800000	14913400000	15457700000	15824900000	17830500000	15837800000	7



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Instrument ID: _____

Date(s) Analyzed: _____

GC Column: _____

ID: _____ (mm)

COMPOUND	AMOUNT (ng)	PEAK	RT	RT WINDOW		CALIBRATION FACTOR
				FROM	TO	
		1				
		2				
		3				
		4				
		5				

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 11:47
 Operator : AR\AJ
 Sample : PSTDICC100
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDICC100

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:03:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:01:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.877	250.0E6	1516.3E6	101.769	98.092
2)	SA Decachlor...	9.072	8.068	348.3E6	1909.5E6	96.236	97.351
Target Compounds							
2)	A alpha-BHC	3.998	3.390	547.4E6	2388.1E6	108.020	99.616
3)	MA gamma-BHC...	4.329	3.726	513.4E6	2205.4E6	106.475	99.619
4)	MA Heptachlor	4.928	4.079	512.5E6	2240.7E6	105.919	98.571
5)	MB Aldrin	5.269	4.365	487.5E6	2165.7E6	105.943	99.021
6)	B beta-BHC	4.515	4.022	183.5E6	915.8E6	100.635	97.407
7)	B delta-BHC	4.763	4.258	503.3E6	2221.1E6	107.623	99.433
8)	B Heptachlo...	5.689	4.869	434.5E6	1971.2E6	104.739	98.086
9)	A Endosulfan I	6.073	5.243	408.8E6	1871.0E6	103.749	97.985
10)	B gamma-Chl...	5.945	5.121	437.2E6	2093.9E6	104.922	98.851
11)	B alpha-Chl...	6.025	5.186	433.4E6	2001.7E6	103.753	98.554
12)	B 4,4'-DDE	6.194	5.371	400.4E6	2043.1E6	106.779	98.544
13)	MA Dieldrin	6.345	5.508	448.2E6	2096.4E6	105.766	98.708
14)	MA Endrin	6.573	5.785	378.7E6	1895.6E6	105.625	97.723
15)	B Endosulfa...	6.785	6.077	370.7E6	1807.1E6	102.908	98.240
16)	A 4,4'-DDD	6.704	5.926	317.1E6	1713.4E6	105.699	98.730
17)	MA 4,4'-DDT	7.020	6.180	354.8E6	1842.5E6	105.256	99.852
18)	B Endrin al...	6.914	6.255	253.1E6	1252.9E6	102.502	98.551
19)	B Endosulfa...	7.149	6.478	352.0E6	1784.3E6	102.563	98.378
20)	A Methoxychlor	7.492	6.750	177.1E6	941.0E6	99.649	96.986
21)	B Endrin ke...	7.630	6.987	380.4E6	1936.5E6	102.798	98.099
22)	Mirex	8.113	7.181	264.5E6	1440.6E6	97.646	97.171



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 11:47
Operator : AR\AJ
Sample : PSTDICC100
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDICC100

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:03:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:01:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

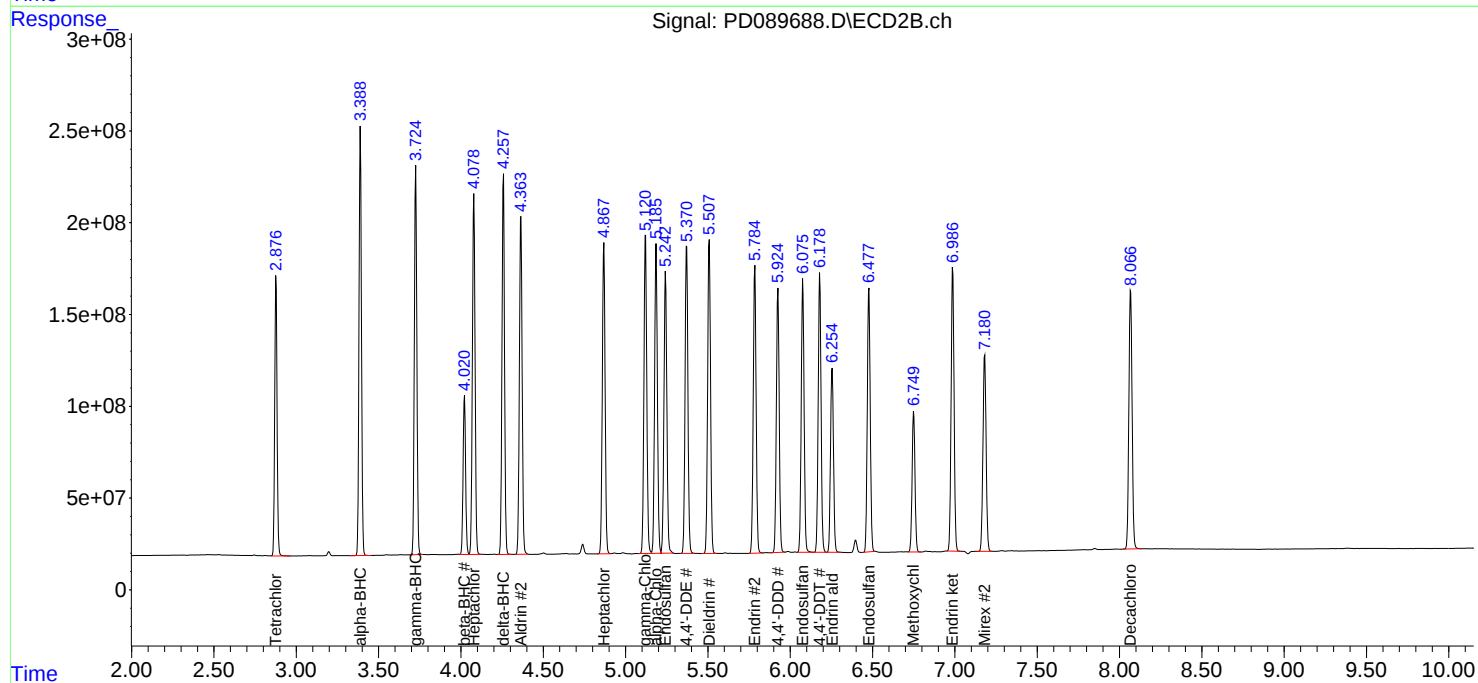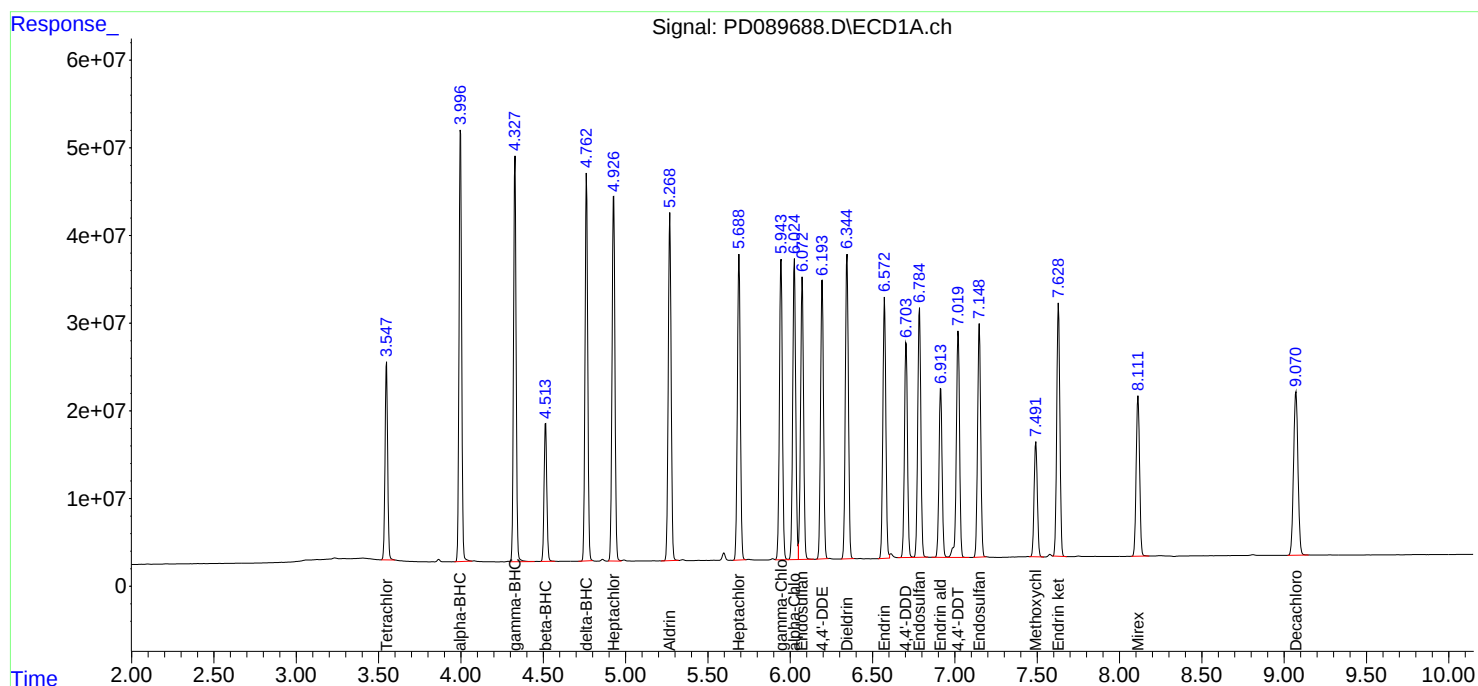

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089689.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 12:01
 Operator : AR\AJ
 Sample : PSTDICC075
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDICC075

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/01/2025
 Supervised By : mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:03:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:01:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.878	182.0E6	1118.5E6	74.099	72.359
28)	SA Decachlor...	9.071	8.067	262.5E6	1406.4E6	72.524	71.702
Target Compounds							
2)	A alpha-BHC	3.998	3.390	389.2E6	1750.2E6	76.799	73.008
3)	MA gamma-BHC...	4.327	3.727	364.1E6	1617.8E6	75.509m	73.078
4)	MA Heptachlor	4.927	4.079	367.5E6	1652.1E6	75.953	72.679
5)	MB Aldrin	5.269	4.365	349.2E6	1591.4E6	75.891	72.762
6)	B beta-BHC	4.514	4.022	134.4E6	678.1E6	73.687	72.127
7)	B delta-BHC	4.763	4.259	358.2E6	1631.4E6	76.586	73.032
8)	B Heptachlo...	5.689	4.869	313.4E6	1455.4E6	75.540	72.419
9)	A Endosulfan I	6.073	5.243	295.7E6	1384.3E6	75.057	72.494
10)	B gamma-Chl...	5.945	5.122	316.5E6	1536.8E6	75.953	72.551
11)	B alpha-Chl...	6.025	5.186	314.3E6	1475.9E6	75.227	72.665
12)	B 4,4'-DDE	6.194	5.371	286.3E6	1504.8E6	76.363	72.583
13)	MA Dieldrin	6.345	5.509	322.8E6	1541.4E6	76.176	72.575
14)	MA Endrin	6.572	5.785	272.7E6	1402.6E6	76.049	72.311
15)	B Endosulfa...	6.785	6.076	271.1E6	1331.9E6	75.250	72.403
16)	A 4,4'-DDD	6.703	5.925	228.6E6	1259.0E6	76.194	72.547
17)	MA 4,4'-DDT	7.019	6.179	256.2E6	1348.7E6	76.010	73.090
18)	B Endrin al...	6.913	6.255	183.3E6	916.8E6	74.217	72.118
19)	B Endosulfa...	7.148	6.479	257.0E6	1313.6E6	74.880	72.427
20)	A Methoxychlor	7.492	6.750	131.3E6	697.3E6	73.886	71.862
21)	B Endrin ke...	7.629	6.987	277.5E6	1426.8E6	74.979	72.278
22)	Mirex	8.112	7.181	197.2E6	1065.3E6	72.806	71.858

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089689.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 12:01
Operator : AR\AJ
Sample : PSTDICC075
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

PSTDICC075

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 08/01/2025

Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:03:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:01:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

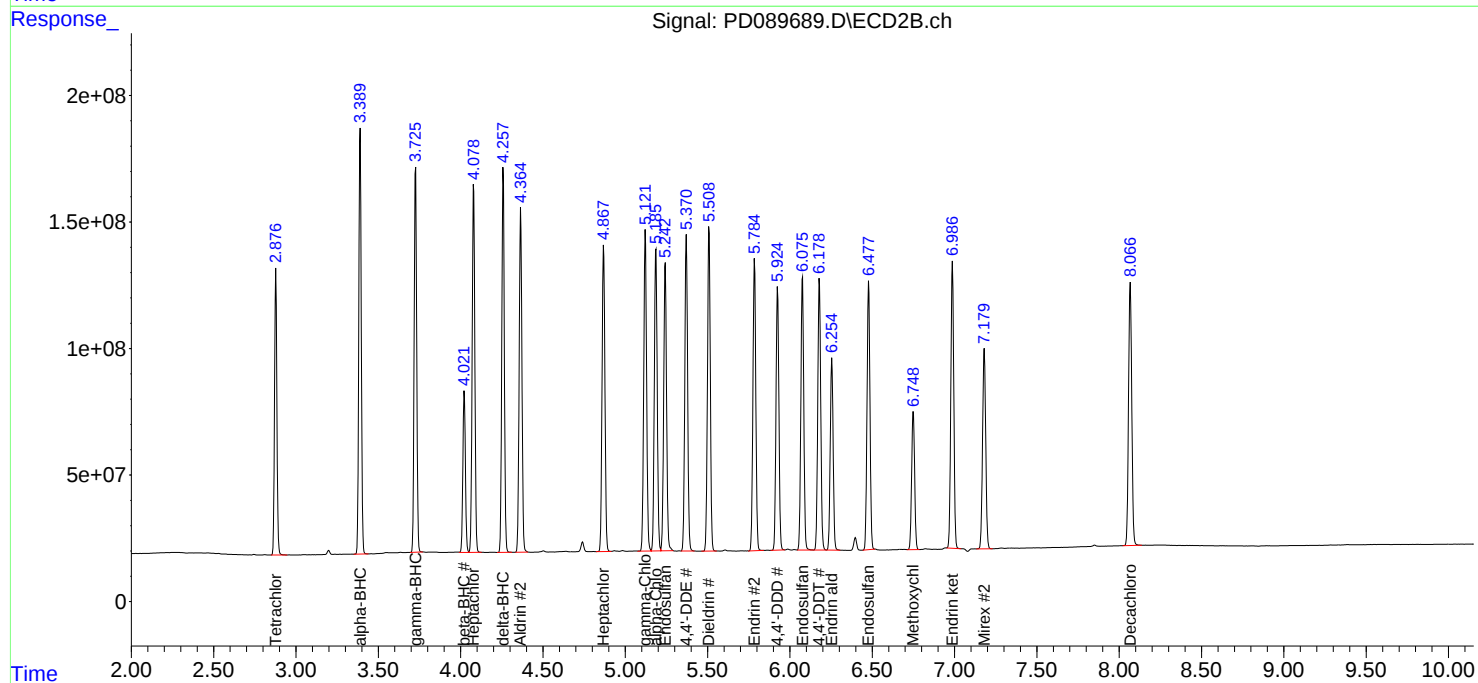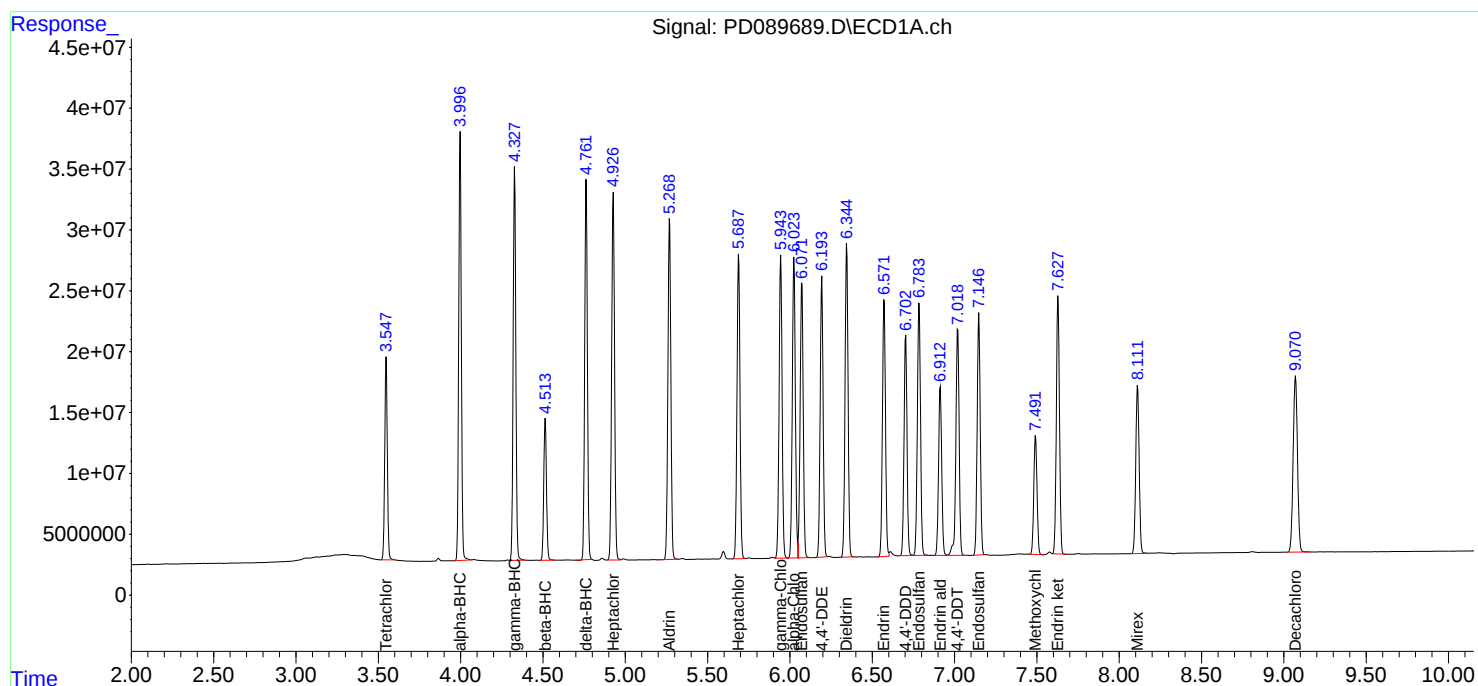

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089690.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 12:14
 Operator : AR\AJ
 Sample : PSTDICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:04:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:01:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.878	122.8E6	772.9E6	50.000	50.000
28)	SA Decachlor...	9.071	8.068	181.0E6	980.7E6	50.000	50.000
Target Compounds							
2)	A alpha-BHC	3.997	3.390	253.4E6	1198.6E6	50.000	50.000
3)	MA gamma-BHC...	4.328	3.726	241.1E6	1106.9E6	50.000	50.000
4)	MA Heptachlor	4.927	4.079	241.9E6	1136.6E6	50.000	50.000
5)	MB Aldrin	5.269	4.365	230.1E6	1093.6E6	50.000	50.000
6)	B beta-BHC	4.514	4.022	91190240	470.1E6	50.000	50.000
7)	B delta-BHC	4.763	4.259	233.8E6	1116.9E6	50.000	50.000
8)	B Heptachlo...	5.689	4.869	207.4E6	1004.8E6	50.000	50.000
9)	A Endosulfan I	6.072	5.243	197.0E6	954.8E6	50.000	50.000
10)	B gamma-Chl...	5.944	5.122	208.3E6	1059.1E6	50.000	50.000
11)	B alpha-Chl...	6.025	5.186	208.9E6	1015.5E6	50.000	50.000
12)	B 4,4'-DDE	6.194	5.371	187.5E6	1036.6E6	50.000	50.000
13)	MA Dieldrin	6.345	5.509	211.9E6	1061.9E6	50.000	50.000
14)	MA Endrin	6.572	5.785	179.3E6	969.9E6	50.000	50.000
15)	B Endosulfa...	6.784	6.077	180.1E6	919.8E6	50.000	50.000
16)	A 4,4'-DDD	6.704	5.925	150.0E6	867.7E6	50.000	50.000
17)	MA 4,4'-DDT	7.019	6.179	168.5E6	922.6E6	50.000	50.000
18)	B Endrin al...	6.913	6.255	123.5E6	635.6E6	50.000	50.000
19)	B Endosulfa...	7.148	6.478	171.6E6	906.8E6	50.000	50.000
20)	A Methoxychlor	7.492	6.750	88865799	485.1E6	50.000	50.000
21)	B Endrin ke...	7.629	6.988	185.0E6	987.0E6	50.000	50.000
22)	Mirex	8.112	7.181	135.4E6	741.3E6	50.000	50.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089690.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 12:14
Operator : AR\AJ
Sample : PSTDICC050
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDICC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:04:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:01:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

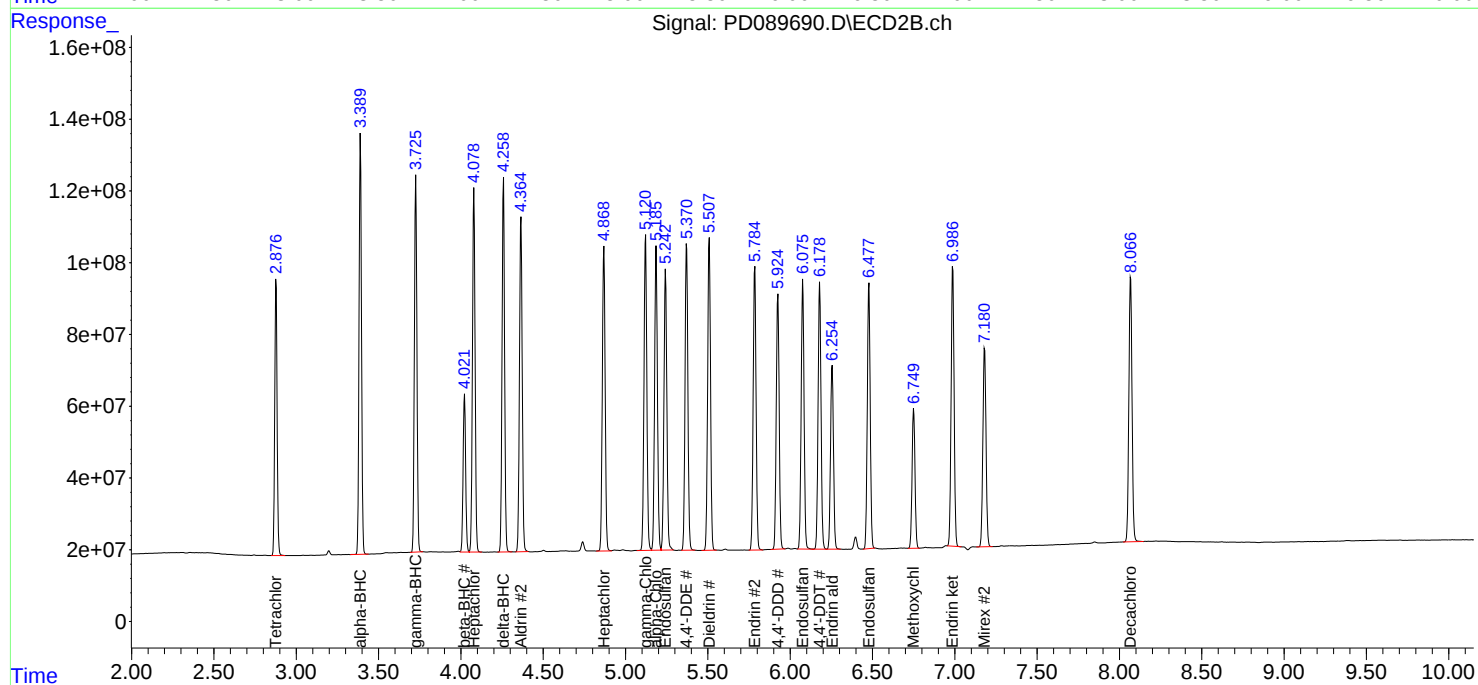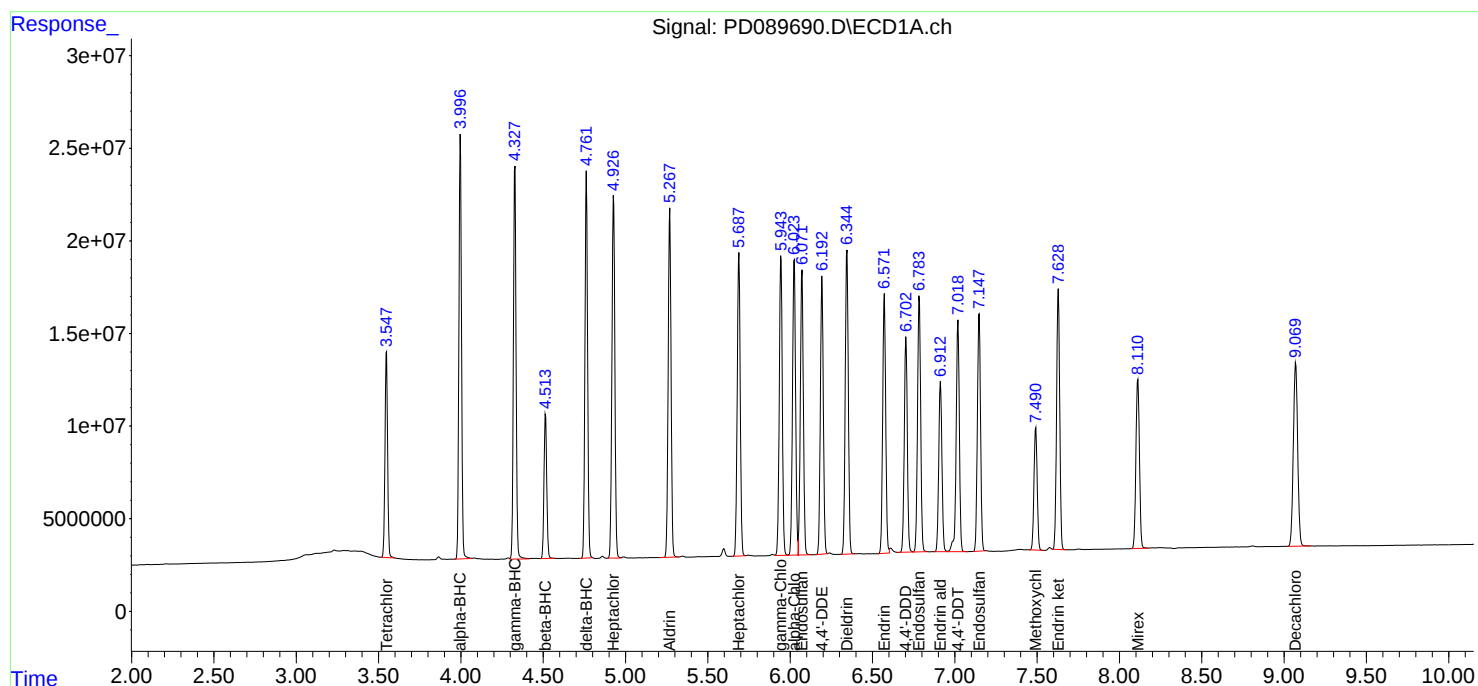

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 12:28
 Operator : AR\AJ
 Sample : PSTDICC025
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDICC025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:04:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:01:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.878	60086888	395.6E6	24.459	25.594
2)	SA Decachlor...	9.070	8.068	93155610	502.3E6	25.737	25.611
Target Compounds							
2)	A alpha-BHC	3.997	3.390	115.9E6	602.6E6	22.877	25.138
3)	MA gamma-BHC...	4.328	3.726	112.0E6	560.3E6	23.240	25.309
4)	MA Heptachlor	4.927	4.079	114.0E6	579.4E6	23.566	25.490
5)	MB Aldrin	5.268	4.365	108.2E6	556.5E6	23.508	25.445
6)	B beta-BHC	4.515	4.022	45165459	242.6E6	24.764	25.805
7)	B delta-BHC	4.763	4.259	107.4E6	564.0E6	22.958	25.251
8)	B Heptachlo...	5.688	4.869	99446385	517.2E6	23.970	25.737
9)	A Endosulfan I	6.072	5.243	95423575	490.8E6	24.218	25.703
10)	B gamma-Chl...	5.944	5.122	99925801	541.3E6	23.981	25.556
11)	B alpha-Chl...	6.024	5.186	101.2E6	520.3E6	24.230	25.616
12)	B 4,4'-DDE	6.193	5.372	88194803	529.6E6	23.521	25.544
13)	MA Dieldrin	6.344	5.509	100.3E6	540.2E6	23.678	25.437
14)	MA Endrin	6.572	5.786	84843783	493.4E6	23.664	25.438
15)	B Endosulfa...	6.784	6.077	88566720	470.7E6	24.585	25.586
16)	A 4,4'-DDD	6.703	5.926	71191879	441.6E6	23.731	25.443
17)	MA 4,4'-DDT	7.019	6.179	80141596	460.3E6	23.775	24.945
18)	B Endrin al...	6.913	6.255	60887538	325.1E6	24.658	25.572
19)	B Endosulfa...	7.148	6.479	83927332	464.7E6	24.451	25.620
20)	A Methoxychlor	7.491	6.750	44254083	248.8E6	24.899	25.639
21)	B Endrin ke...	7.628	6.988	90082871	504.5E6	24.342	25.556
22)	Mirex	8.111	7.181	69660388	385.5E6	25.718	26.005



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 12:28
Operator : AR\AJ
Sample : PSTDICC025
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDICC025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:04:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:01:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

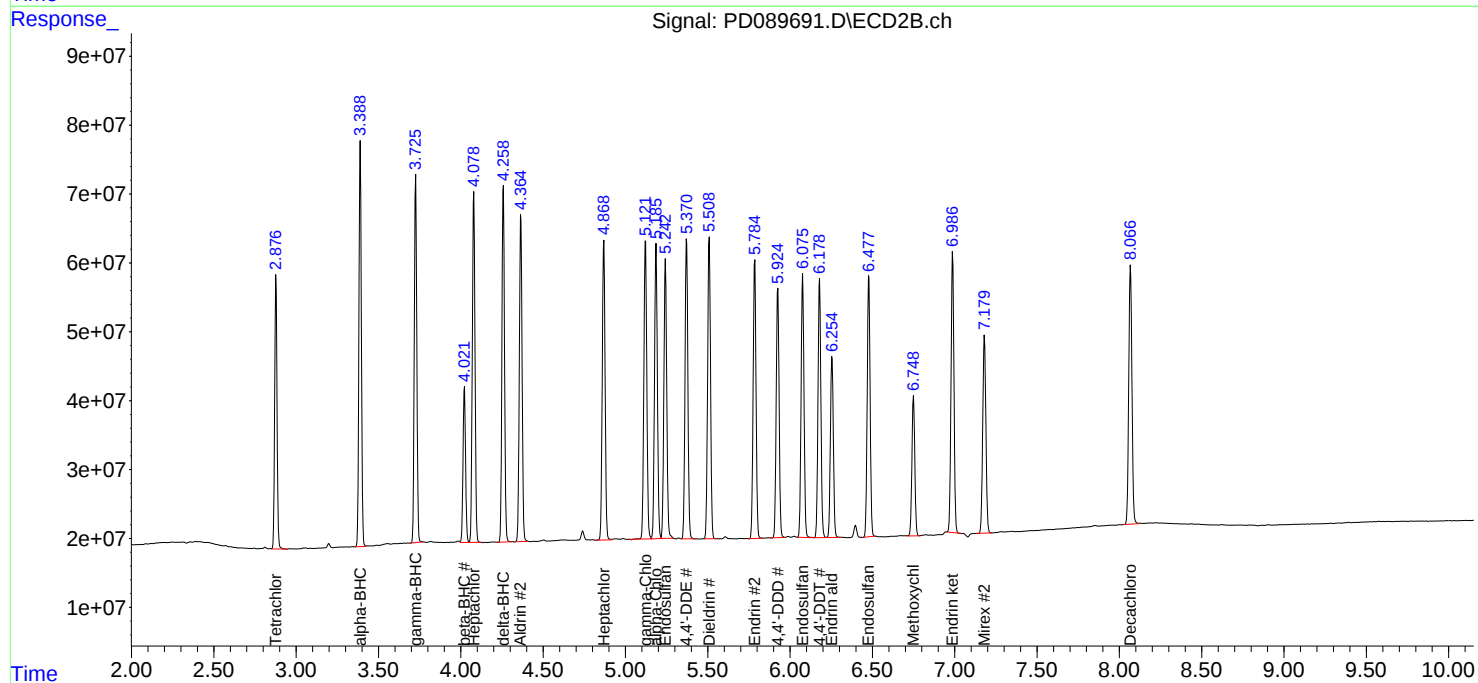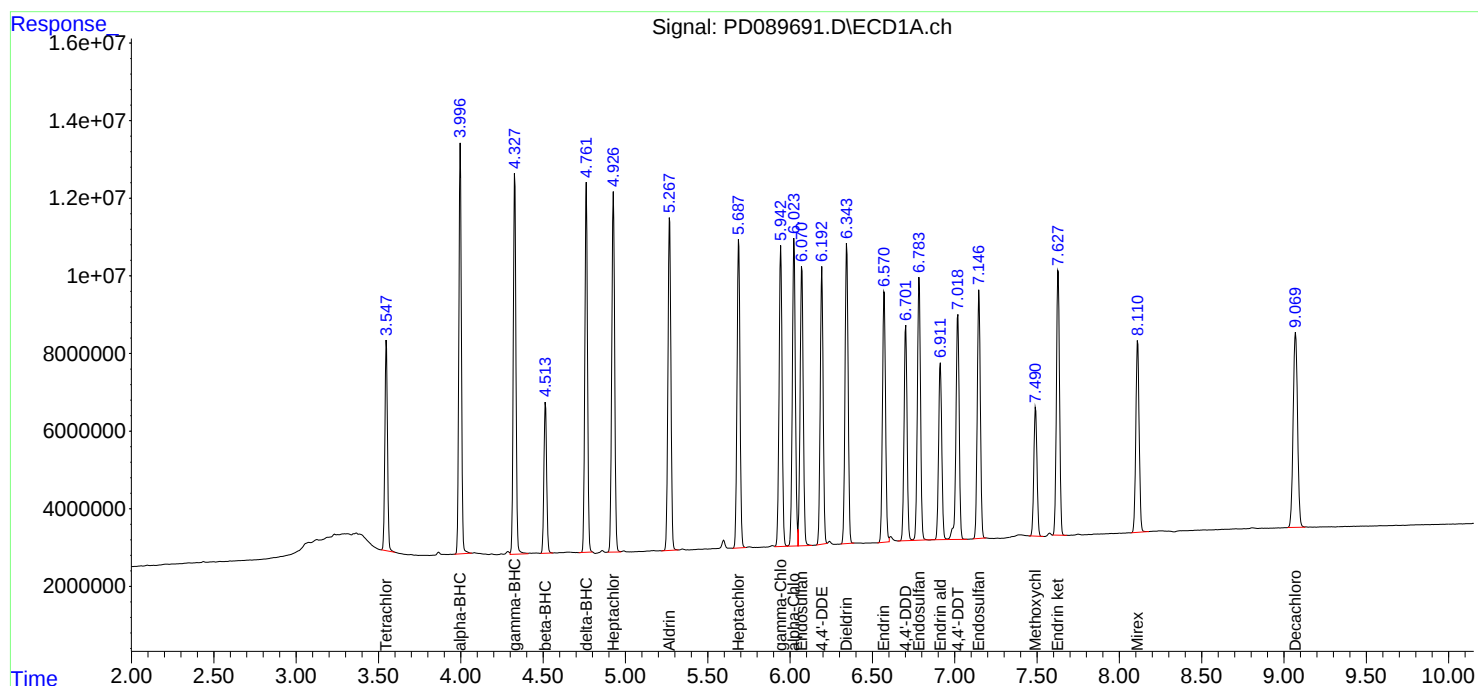

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089692.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 12:41
 Operator : AR\AJ
 Sample : PSTDICC005
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDICC005

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/01/2025
 Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:04:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:01:48 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.878	12728556	89152363	5.181	5.768
28) SA Decachlor...	9.070	8.068	21262032	114.2E6	5.874	5.821
Target Compounds						
2) A alpha-BHC	3.997	3.390	21991813	131.1E6	4.339	5.471 #
3) MA gamma-BHC...	4.328	3.726	22352025	122.2E6	4.636	5.521
4) MA Heptachlor	4.927	4.079	23169413	128.5E6	4.789	5.653
5) MB Aldrin	5.268	4.365	21817288	121.2E6	4.741	5.543
6) B beta-BHC	4.514	4.022	9828461	54697788	5.389	5.818
7) B delta-BHC	4.762	4.259	20752633	123.6E6	4.437	5.532
8) B Heptachlo...	5.688	4.869	21263659	114.2E6	5.125	5.685
9) A Endosulfan I	6.072	5.243	20149074	109.2E6	5.114	5.721
10) B gamma-Chl...	5.943	5.122	20699286	120.0E6	4.968	5.665
11) B alpha-Chl...	6.024	5.186	21350809	116.5E6	5.111	5.734
12) B 4,4'-DDE	6.193	5.369	17748555	116.4E6	4.733	5.613m
13) MA Dieldrin	6.345	5.509	20395942	119.2E6	4.813	5.611
14) MA Endrin	6.571	5.786	17435369	114.2E6	4.863	5.886
15) B Endosulfa...	6.784	6.077	19400476	104.7E6	5.385	5.693
16) A 4,4'-DDD	6.703	5.926	14539424	96121739	4.847	5.539
17) MA 4,4'-DDT	7.019	6.180	16301577	92950908	4.836	5.037
18) B Endrin al...	6.911	6.255	12992981	70660838	5.262m	5.558
19) B Endosulfa...	7.147	6.478	18066498	103.7E6	5.263	5.719
20) A Methoxychlor	7.491	6.750	9351951	53085396	5.262	5.471
21) B Endrin ke...	7.628	6.987	18813895	110.2E6	5.084	5.581
22) Mirex	8.111	7.181	15861435	86238194	5.856	5.817

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089692.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 12:41
Operator : AR\AJ
Sample : PSTDICC005
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

PSTDICC005

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 08/01/2025

Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:04:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:01:48 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

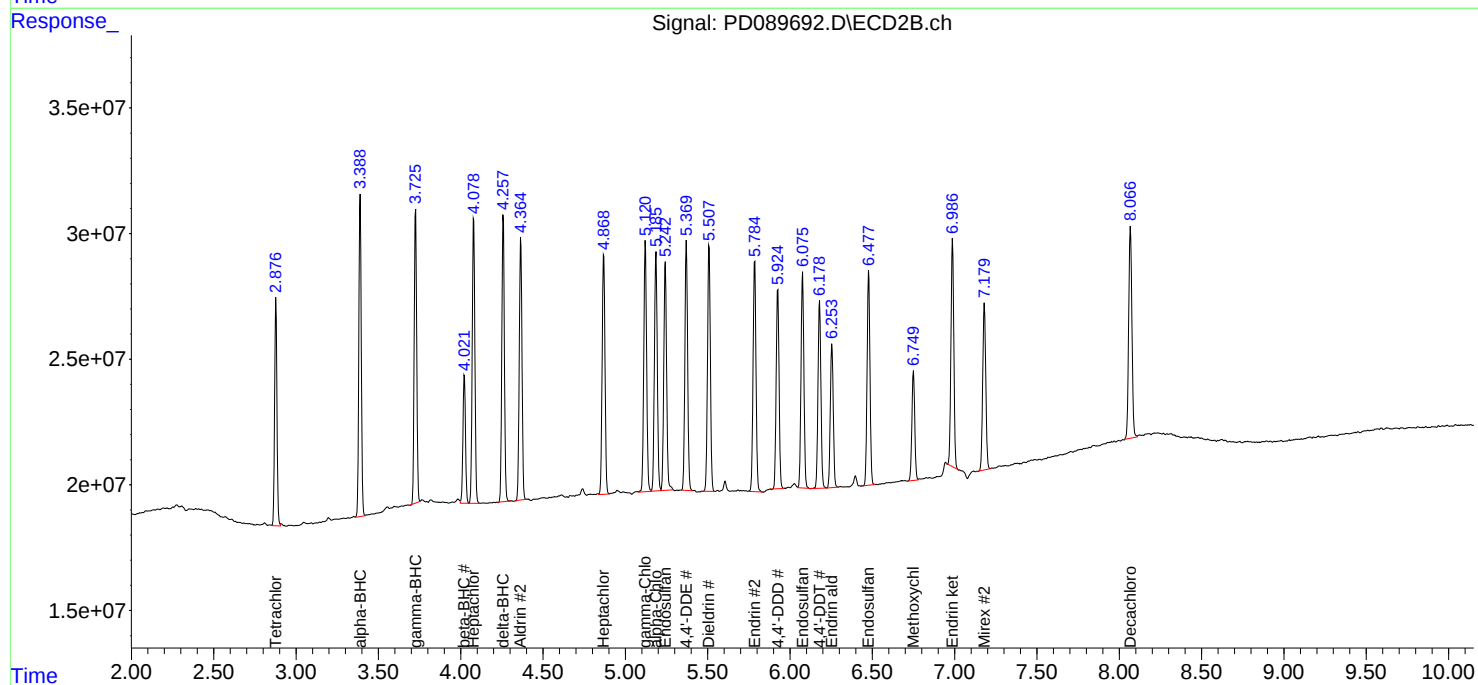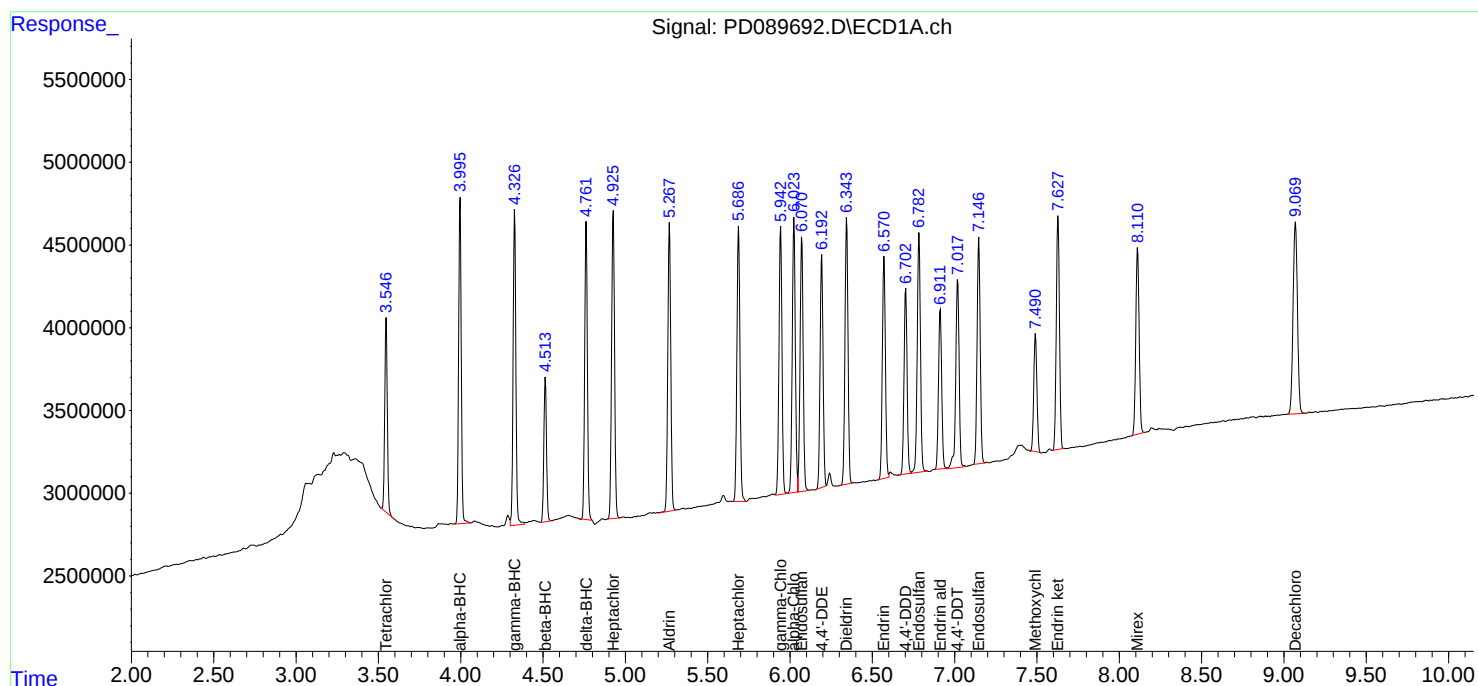

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089695.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 13:23
 Operator : AR\AJ
 Sample : PCHLORICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:19:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:17:51 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	120.5E6	945.6E6	50.000	50.000
28)	SA Decachlor...	9.069	8.067	176.9E6	974.5E6	50.000	50.000
Target Compounds							
23)	Chlordane-1	4.712	3.902	84493998	372.7E6	500.000	500.000
24)	Chlordane-2	5.238	4.483	85139038	388.8E6	500.000	500.000
25)	Chlordane-3	5.944	5.122	351.5E6	1170.3E6	500.000	500.000
26)	Chlordane-4	6.029	5.186	426.3E6	1005.1E6	500.000	500.000
27)	Chlordane-5	6.868	6.086	72983349	462.5E6	500.000	500.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089695.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 13:23
Operator : AR\AJ
Sample : PCHLORICC500
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:19:33 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:17:51 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

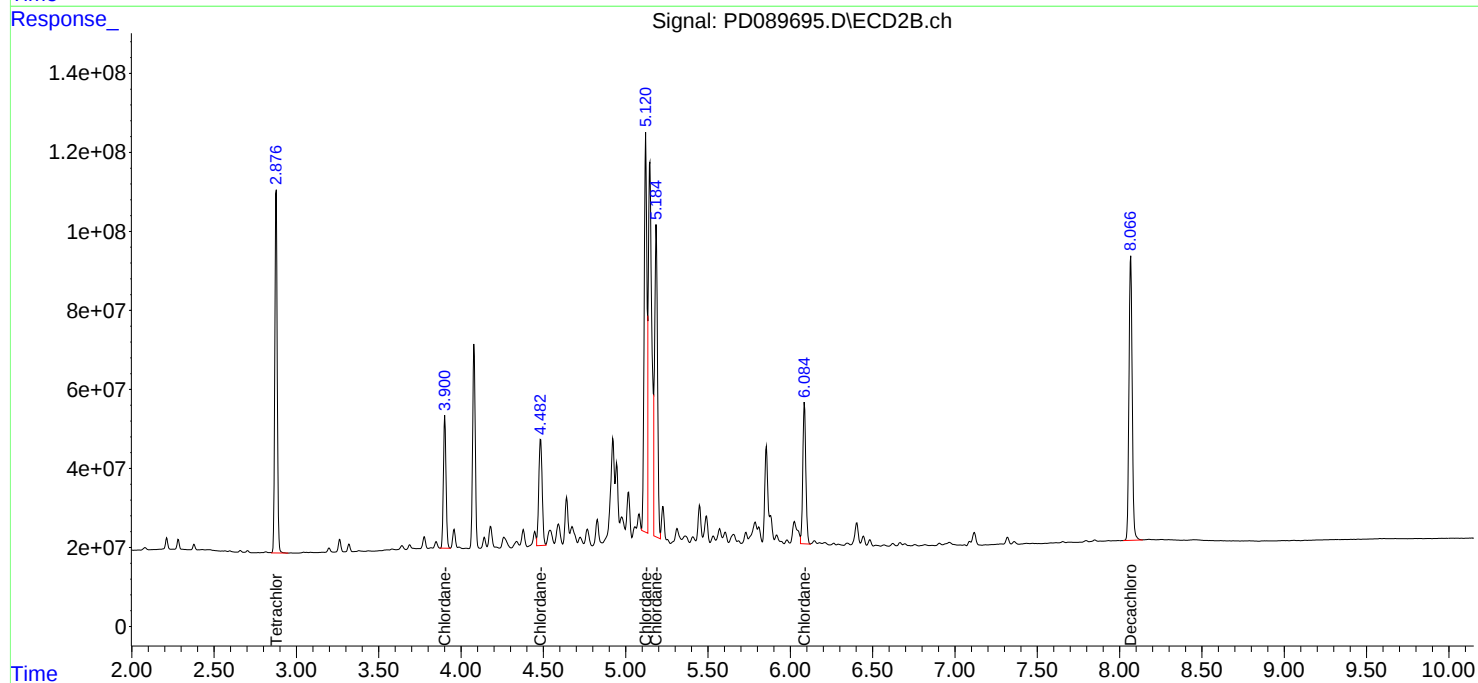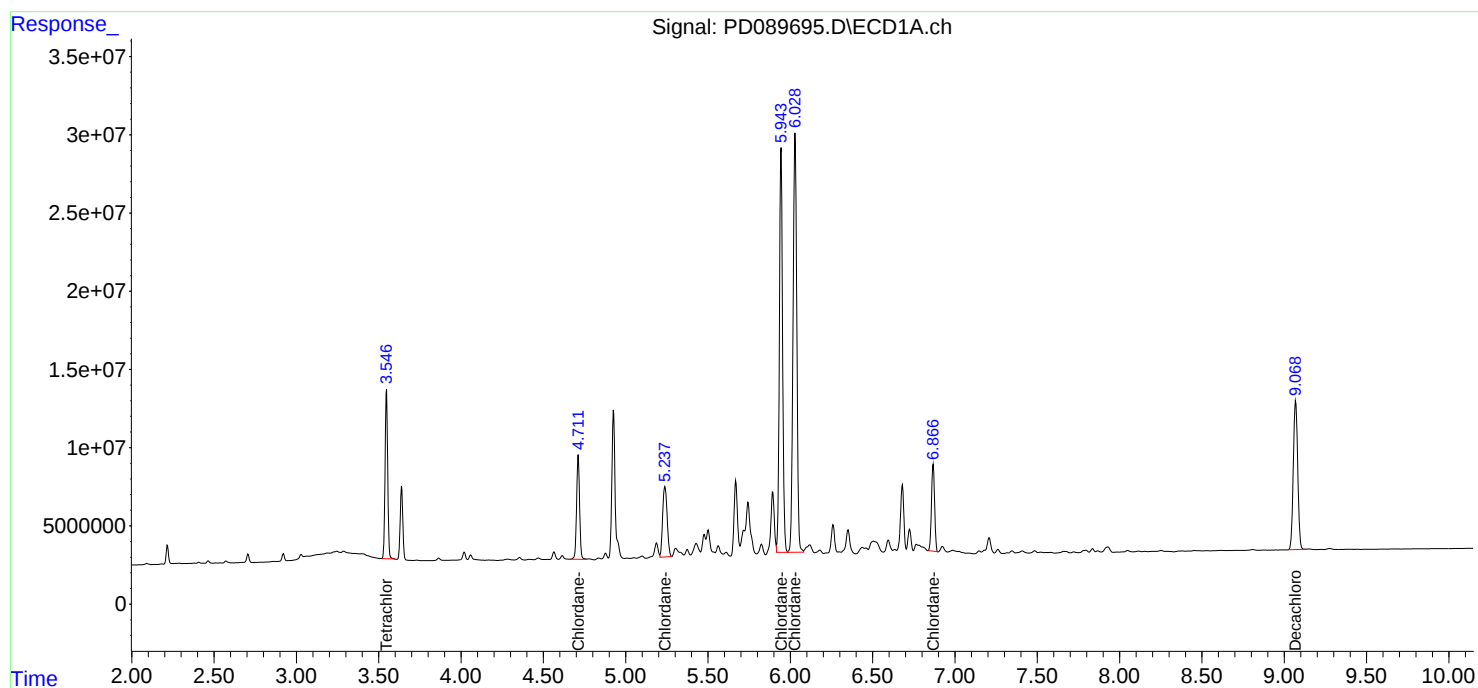

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089700.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 14:31
 Operator : AR\AJ
 Sample : PTOXICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:37:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:37:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.878	124.8E6	773.4E6	50.000	50.000
7) SA Decachlor...	9.068	8.066	184.8E6	987.6E6	50.000	50.000
Target Compounds						
2) Toxaphene-1	6.239	5.471	17443475	79994774	500.000	500.000
3) Toxaphene-2	6.439	5.642	23341665	54280922	500.000	500.000
4) Toxaphene-3	7.146	6.752	45826320	259.8E6	500.000	500.000
5) Toxaphene-4	7.561	7.193	60366168	180.8E6	500.000	500.000
6) Toxaphene-5	7.926	7.324	34082893	127.1E6	500.000	500.000

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089700.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 14:31
Operator : AR\AJ
Sample : PTOXICC500
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:37:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:37:33 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

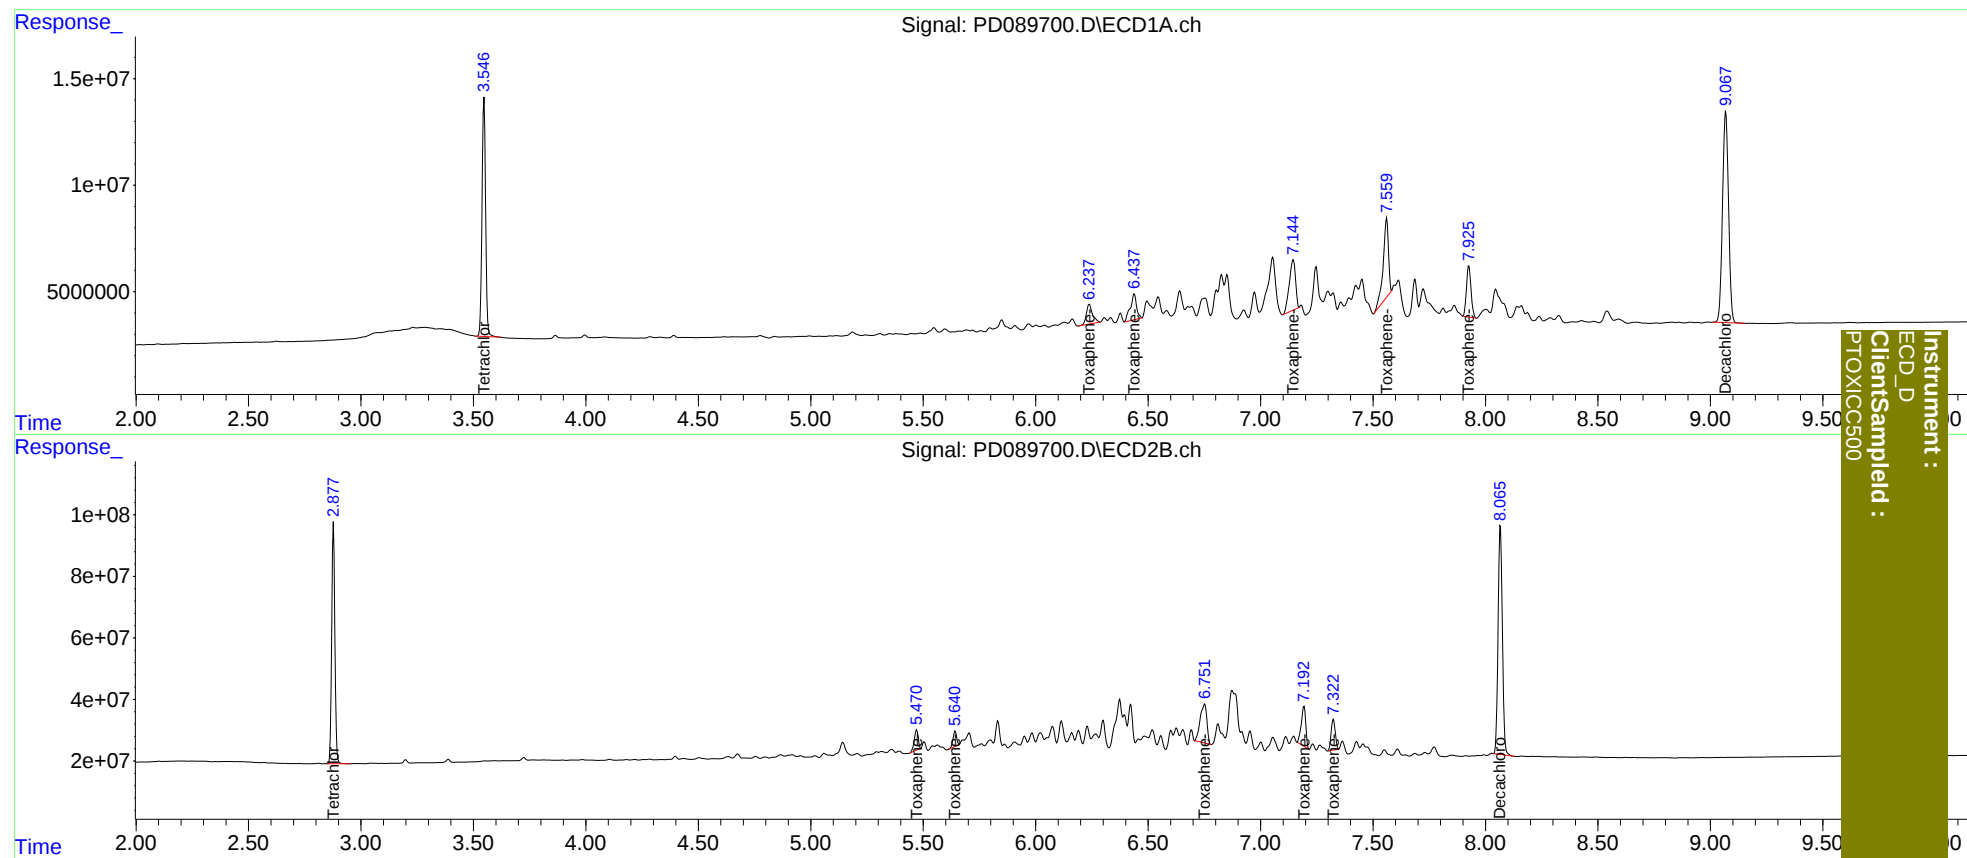

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089703.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 15:11
 Operator : AR\AJ
 Sample : PSTDICV050
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICPD073125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:51:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:29:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.878	120.0E6	761.1E6	48.643	48.054
28)	SA Decachlor...	9.068	8.067	181.6E6	1003.9E6	48.862	50.002
Target Compounds							
2)	A alpha-BHC	3.997	3.390	247.1E6	1174.9E6	49.894	48.341
3)	MA gamma-BHC...	4.328	3.726	235.0E6	1091.3E6	49.442	48.451
4)	MA Heptachlor	4.927	4.079	236.5E6	1118.2E6	49.144	48.177
5)	MB Aldrin	5.269	4.365	226.3E6	1080.5E6	49.573	48.561
6)	B beta-BHC	4.514	4.022	89444936	462.6E6	48.488	47.941
7)	B delta-BHC	4.762	4.258	227.8E6	1097.8E6	49.674	48.330
8)	B Heptachlo...	5.689	4.869	203.2E6	996.0E6	48.615	48.467
9)	A Endosulfan I	6.072	5.243	193.3E6	951.2E6	48.760	48.657
10)	B gamma-Chl...	5.943	5.122	205.3E6	1052.1E6	49.121	48.590
11)	B alpha-Chl...	6.025	5.186	205.4E6	1010.4E6	48.847	48.528
12)	B 4,4'-DDE	6.193	5.371	184.6E6	1030.8E6	49.482	48.768
13)	MA Dieldrin	6.344	5.508	208.4E6	1056.1E6	49.341	48.805
14)	MA Endrin	6.572	5.785	174.3E6	956.4E6	48.704	47.998
15)	B Endosulfa...	6.784	6.076	177.5E6	917.6E6	48.364	48.811
16)	A 4,4'-DDD	6.703	5.925	148.3E6	869.0E6	49.533	49.286
17)	MA 4,4'-DDT	7.019	6.179	166.6E6	923.5E6	49.583	50.264
18)	B Endrin al...	6.913	6.255	124.7E6	648.5E6	49.955	50.191
19)	B Endosulfa...	7.147	6.478	169.4E6	910.4E6	48.814	49.036
20)	A Methoxychlor	7.491	6.750	87549683	489.2E6	48.966	49.945
21)	B Endrin ke...	7.628	6.987	184.0E6	1003.7E6	49.547	50.012
22)	Mirex	8.111	7.181	134.7E6	755.7E6	48.321	49.648



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089703.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 15:11
Operator : AR\AJ
Sample : PSTDICV050
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD073125

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:51:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:29:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

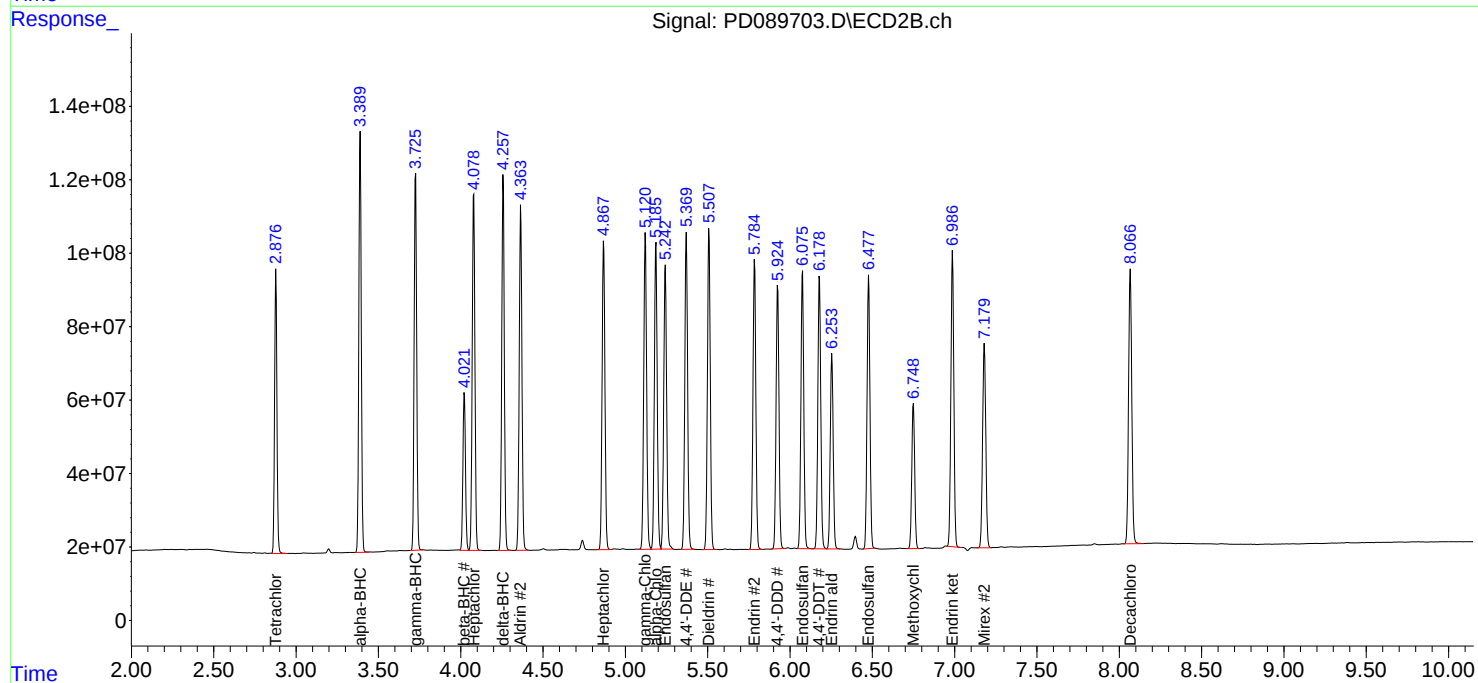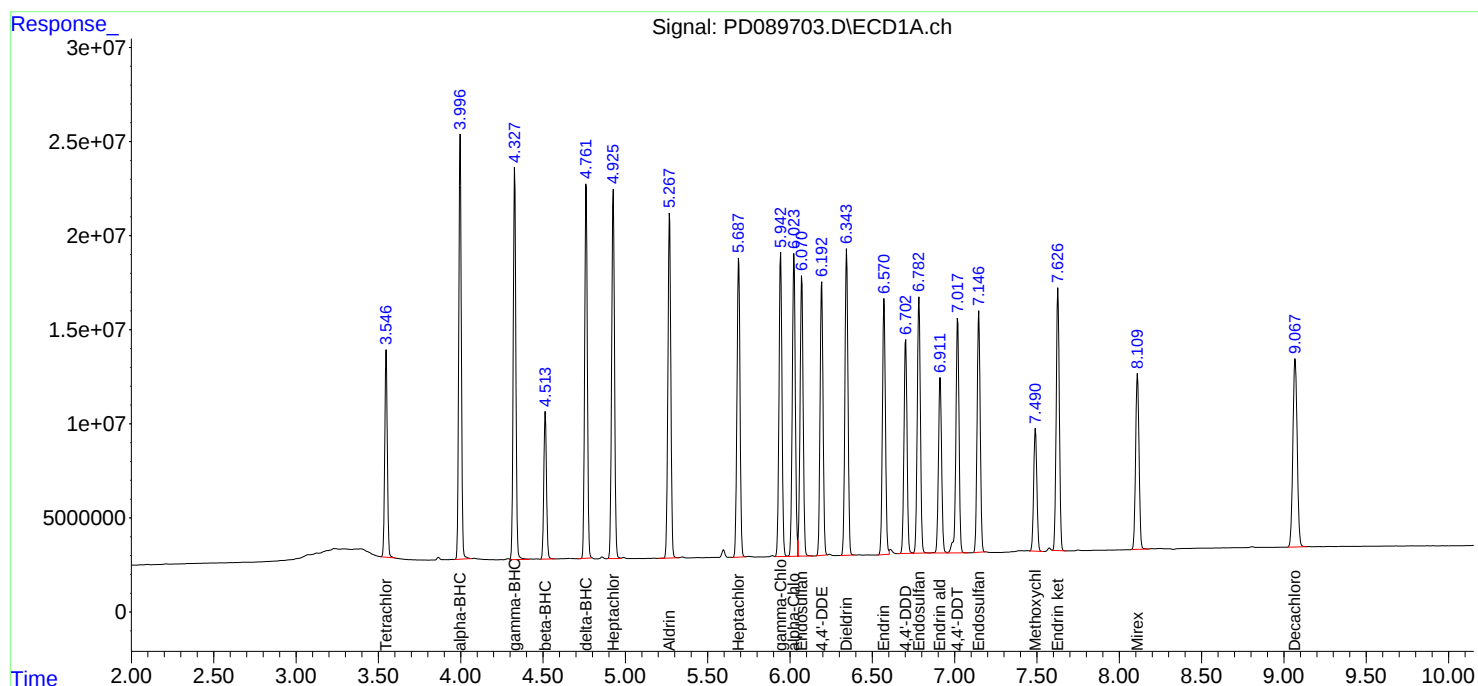

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089704.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 15:25
 Operator : AR\AJ
 Sample : PCHLORICV500
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD073125CHLOR

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 06:57:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:55:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	116.8E6	920.9E6	48.720	49.345
28)	SA Decachlor...	9.068	8.068	173.9E6	968.6E6	48.439	49.120
Target Compounds							
23)	Chlordane-1	4.712	3.902	81245774	362.8E6	487.797	495.995
24)	Chlordane-2	5.239	4.484	82083462	377.5E6	483.066	493.864
25)	Chlordane-3	5.944	5.122	339.6E6	1127.1E6	495.100	487.029
26)	Chlordane-4	6.030	5.186	410.6E6	968.1E6	490.532	486.594
27)	Chlordane-5	6.868	6.086	70531851	450.9E6	488.923	498.388



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089704.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 15:25
Operator : AR\AJ
Sample : PCHLORICV500
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
ICVPD073125CHLOR

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 06:57:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:55:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

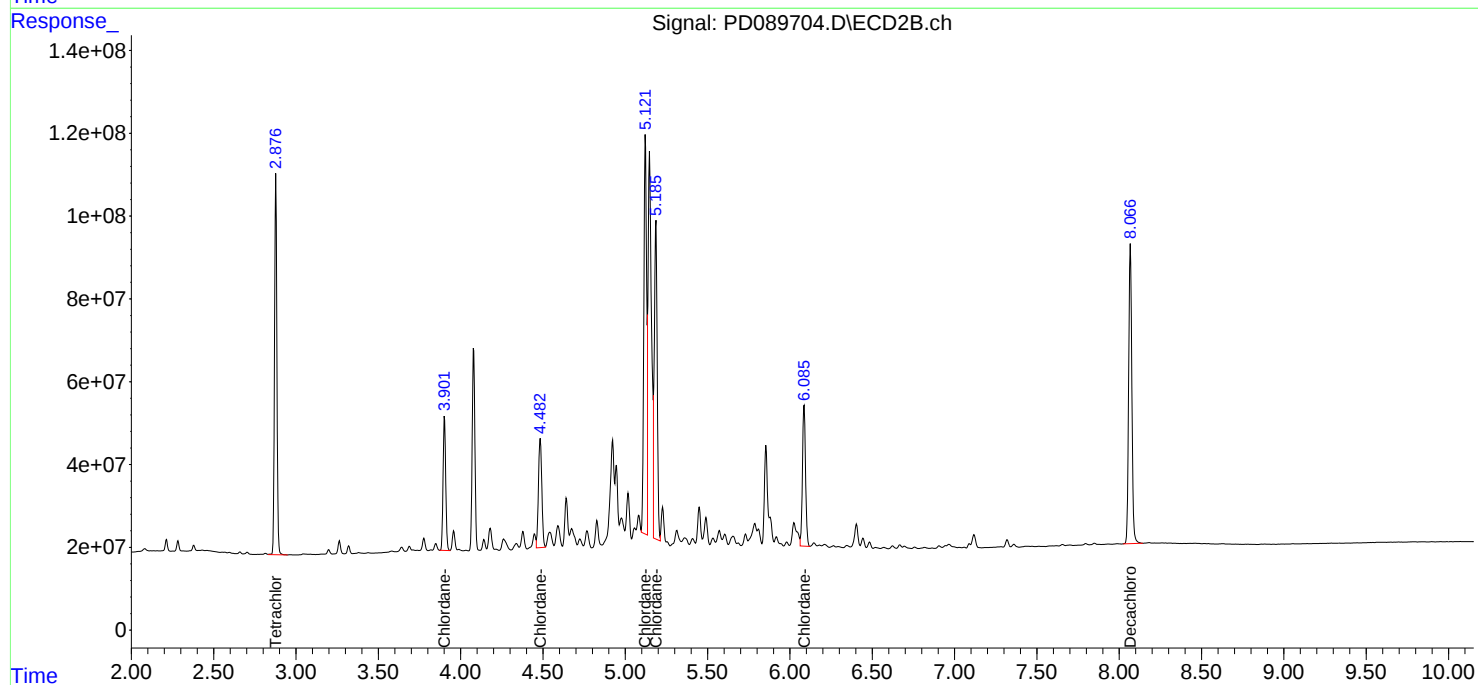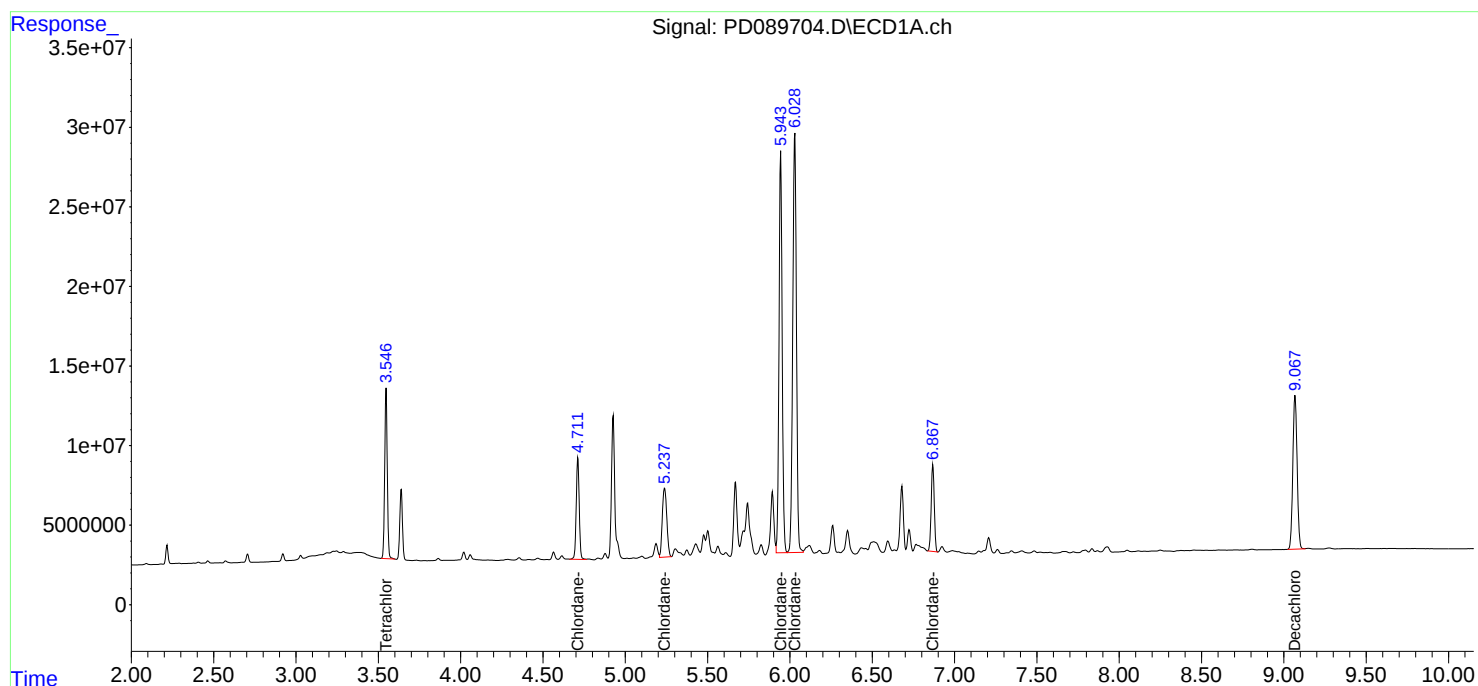

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089705.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 15:39
 Operator : AR\AJ
 Sample : PTOXICV500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 ICVPD073125TOX

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 07:12:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 06:37:50 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.547	2.878	121.0E6	763.7E6	49.297	49.152
7) SA Decachlor...	9.068	8.067	180.0E6	1004.8E6	48.913	50.328
Target Compounds						
2) Toxaphene-1	6.239	5.471	16790342	79371176	450.215	495.332
3) Toxaphene-2	6.438	5.642	22399003	54781356	491.263	516.501
4) Toxaphene-3	7.145	6.751	44678983	257.9E6	496.518	512.065
5) Toxaphene-4	7.560	7.193	58879040	179.0E6	503.289	505.290
6) Toxaphene-5	7.925	7.324	32919996	126.7E6	493.281	522.829

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089705.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 15:39
Operator : AR\AJ
Sample : PTOXICV500
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:12:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 06:37:50 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0. Signal #2 Info : 30M x 0.32mm x0.25µm

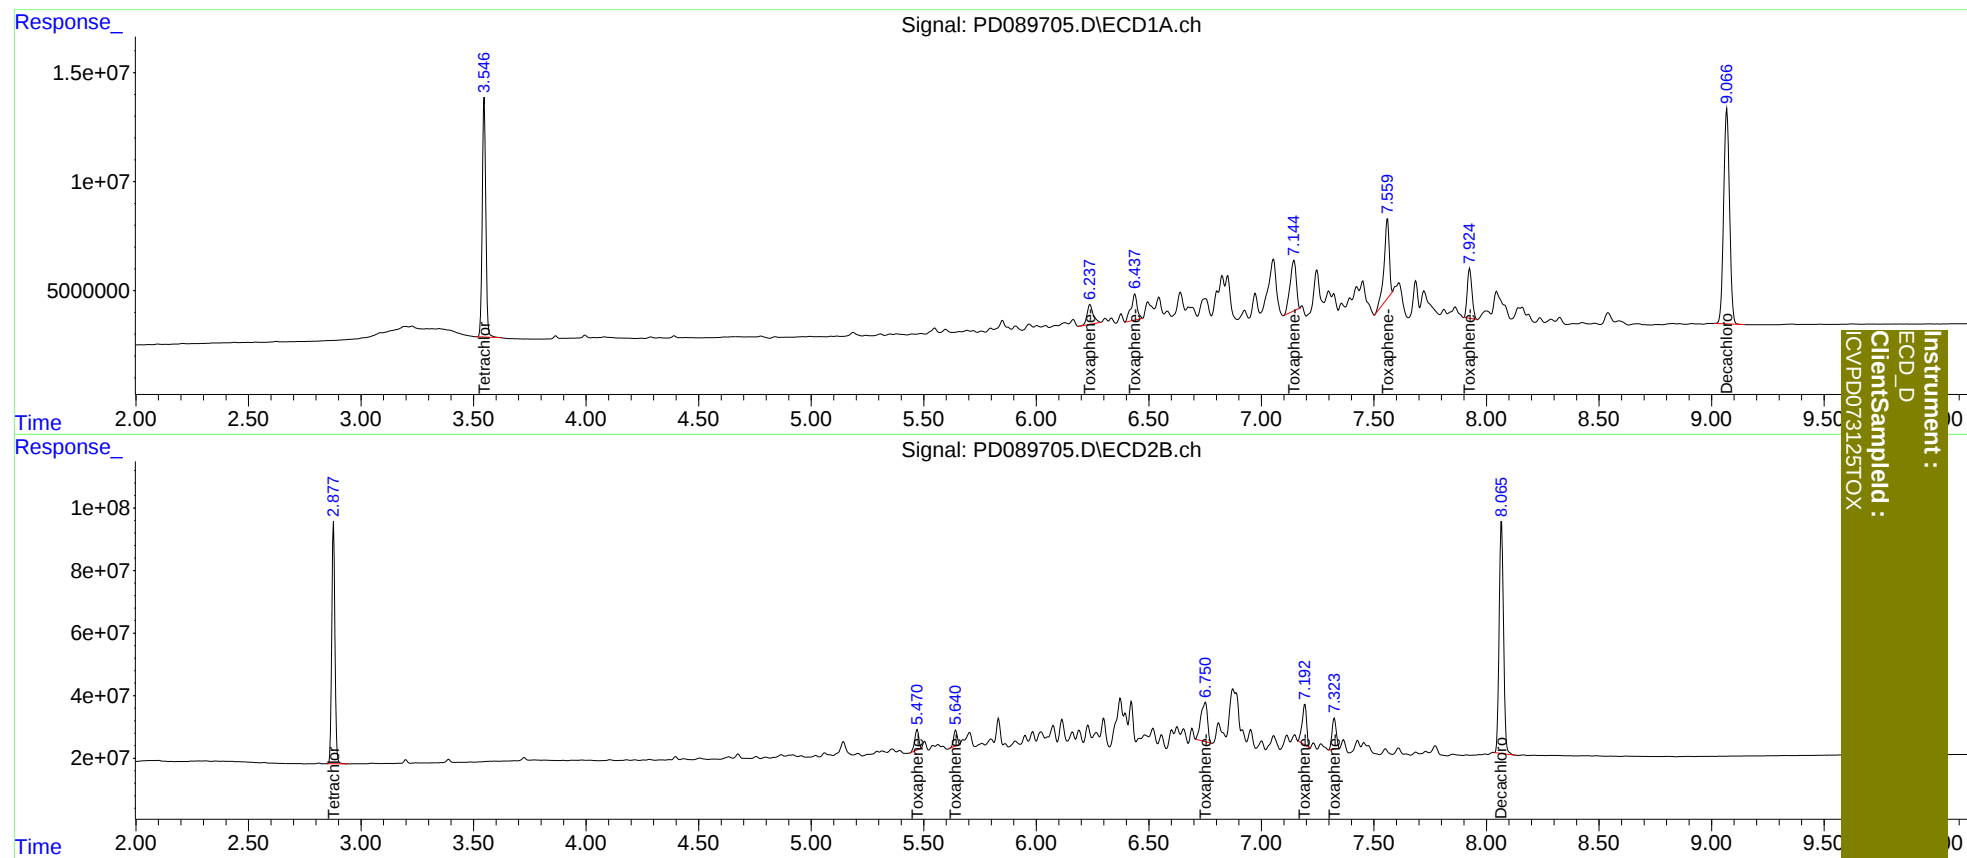



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Continuing Calib Date: 08/08/2025

Initial Calibration Date(s): 07/31/2025 07/31/2025

Continuing Calib Time: 13:53

Initial Calibration Time(s): 11:47 12:41

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	9.07	9.07	8.97	9.17	0.00
Tetrachloro-m-xylene	3.55	3.55	3.45	3.65	0.00
Aldrin	5.27	5.27	5.17	5.37	0.00
Dieldrin	6.34	6.35	6.25	6.45	0.01
4,4'-DDE	6.19	6.19	6.09	6.29	0.00
4,4'-DDD	6.70	6.70	6.60	6.80	0.00
4,4'-DDT	7.02	7.02	6.92	7.12	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Continuing Calib Date: 08/08/2025

Initial Calibration Date(s): 07/31/2025

07/31/2025

Continuing Calib Time: 13:53

Initial Calibration Time(s): 11:47

12:41

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	8.07	8.07	7.97	8.17	0.01
Tetrachloro-m-xylene	2.88	2.88	2.78	2.98	0.00
Aldrin	4.36	4.37	4.27	4.47	0.01
Dieldrin	5.51	5.51	5.41	5.61	0.00
4,4'-DDE	5.37	5.37	5.27	5.47	0.00
4,4'-DDD	5.92	5.93	5.83	6.03	0.01
4,4'-DDT	6.18	6.18	6.08	6.28	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance Contract: POWE02
 Lab Code: ACE SDG NO.: Q2795
 GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No.: CCAL01 Date Analyzed: 08/08/2025
 Lab Sample No.: PSTDCCC050 Data File : PD089810.D Time Analyzed: 13:53

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
4,4'-DDD	6.701	6.604	6.804	54.010	50.000	8.0
4,4'-DDE	6.192	6.094	6.294	51.610	50.000	3.2
4,4'-DDT	7.017	6.919	7.119	47.220	50.000	-5.6
Aldrin	5.267	5.169	5.369	53.980	50.000	8.0
Decachlorobiphenyl	9.067	8.971	9.171	46.030	50.000	-7.9
Dieldrin	6.343	6.245	6.445	51.730	50.000	3.5
Tetrachloro-m-xylene	3.547	3.448	3.648	53.480	50.000	7.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance Contract: POWE02
 Lab Code: ACE SDG NO.: Q2795
 GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No.: CCAL01 Date Analyzed: 08/08/2025
 Lab Sample No.: PSTDCCC050 Data File : PD089810.D Time Analyzed: 13:53

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
4,4'-DDD	5.924	5.825	6.025	59.510	50.000	19.0
4,4'-DDE	5.369	5.271	5.471	58.910	50.000	17.8
4,4'-DDT	6.178	6.079	6.279	56.780	50.000	13.6
Aldrin	4.364	4.265	4.465	59.050	50.000	18.1
Decachlorobiphenyl	8.065	7.968	8.168	48.520	50.000	-3.0
Dieldrin	5.507	5.409	5.609	58.500	50.000	17.0
Tetrachloro-m-xylene	2.877	2.778	2.978	58.790	50.000	17.6

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089810.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 13:53
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:33:50 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	131.9E6	931.1E6	53.481	58.790
2)	SA Decachlor...	9.067	8.065	171.1E6	974.3E6	46.035	48.524
Target Compounds							
2)	A alpha-BHC	3.996	3.389	275.0E6	1450.1E6	55.523	59.661
3)	MA gamma-BHC...	4.327	3.726	262.0E6	1338.2E6	55.126	59.414
4)	MA Heptachlor	4.926	4.078	251.8E6	1323.0E6	52.341	57.003
5)	MB Aldrin	5.267	4.364	246.4E6	1313.9E6	53.976	59.048
6)	B beta-BHC	4.513	4.021	100.1E6	563.2E6	54.256	58.372
7)	B delta-BHC	4.761	4.257	253.5E6	1350.0E6	55.278	59.430
8)	B Heptachlo...	5.687	4.867	221.3E6	1187.5E6	52.942	57.788
9)	A Endosulfan I	6.070	5.241	205.3E6	1075.8E6	51.794	55.030
10)	B gamma-Chl...	5.942	5.120	219.5E6	1275.6E6	52.512	58.909
11)	B alpha-Chl...	6.023	5.185	219.3E6	1220.2E6	52.166	58.600
12)	B 4,4'-DDE	6.192	5.369	192.5E6	1245.3E6	51.614	58.914
13)	MA Dieldrin	6.343	5.507	218.5E6	1265.9E6	51.731	58.502
14)	MA Endrin	6.570	5.784	175.1E6	1169.1E6	48.955	58.676
15)	B Endosulfa...	6.782	6.075	182.3E6	1085.8E6	49.670	57.759
16)	A 4,4'-DDD	6.701	5.924	161.7E6	1049.4E6	54.007	59.514
17)	MA 4,4'-DDT	7.017	6.178	158.7E6	1043.3E6	47.219	56.783
18)	B Endrin al...	6.911	6.253	129.9E6	769.4E6	52.053	59.548
19)	B Endosulfa...	7.146	6.476	167.3E6	1029.5E6	48.201	55.452
20)	A Methoxychlor	7.489	6.748	77516890	511.3E6	43.355	52.198
21)	B Endrin ke...	7.627	6.986	177.3E6	1088.1E6	47.737	54.220
22)	Mirex	8.110	7.179	126.7E6	825.3E6	45.424	54.220



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089810.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 13:53
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:33:50 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

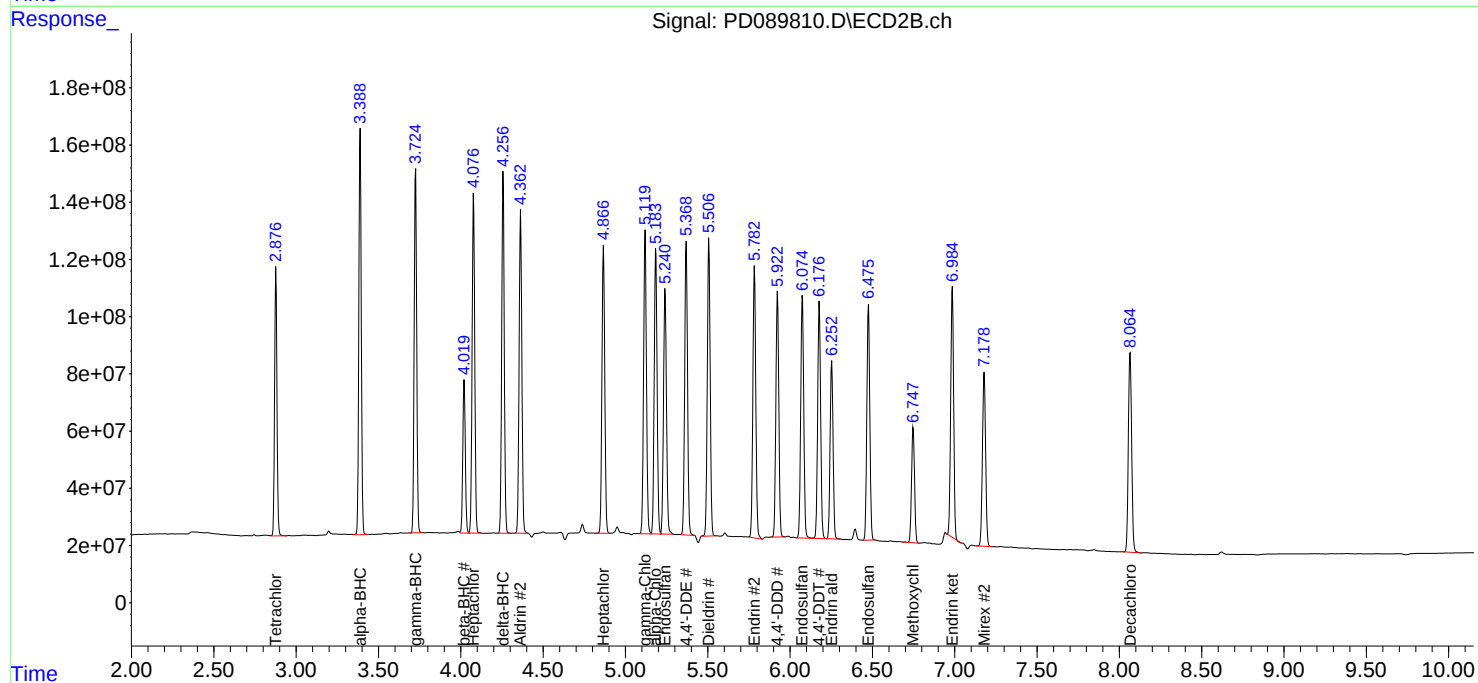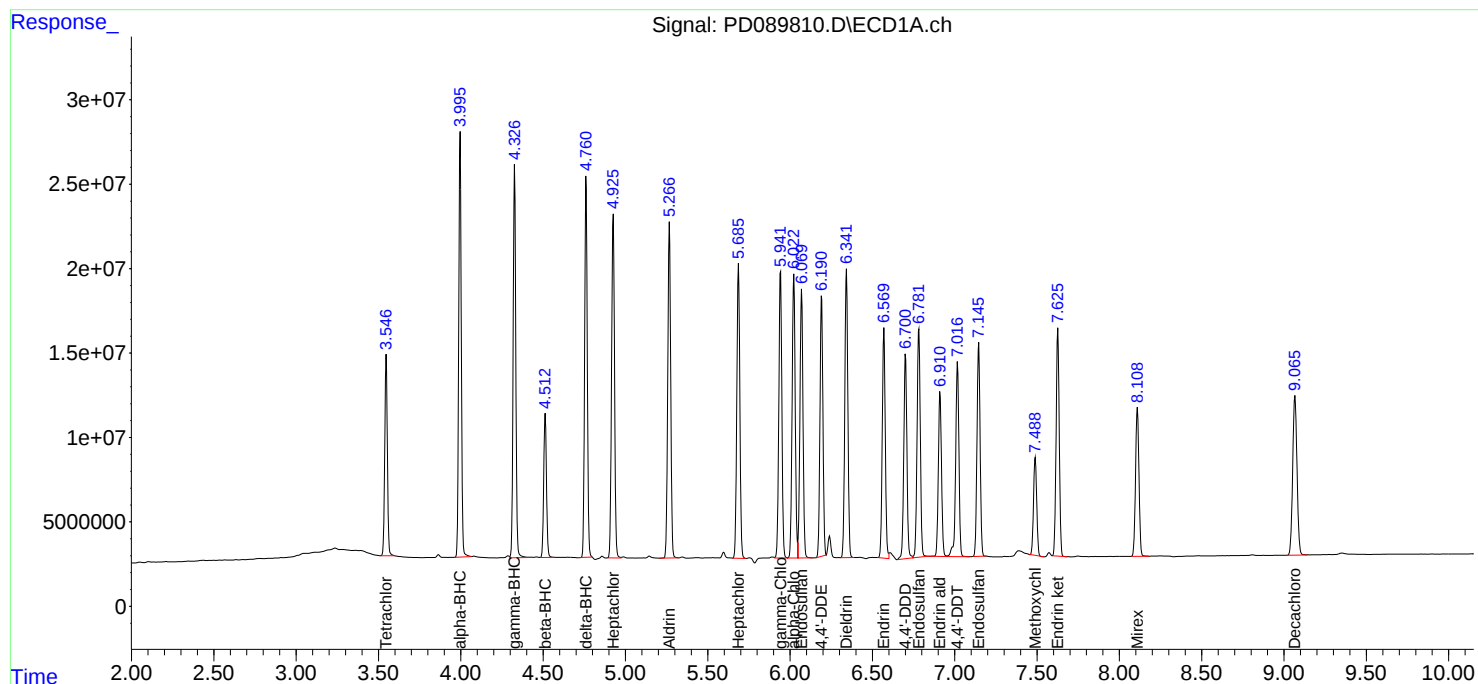



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Continuing Calib Date: 08/08/2025

Initial Calibration Date(s): 07/31/2025 07/31/2025

Continuing Calib Time: 17:43

Initial Calibration Time(s): 11:47 12:41

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	9.07	9.07	8.97	9.17	0.00
Tetrachloro-m-xylene	3.55	3.55	3.45	3.65	0.00
Aldrin	5.27	5.27	5.17	5.37	0.00
Dieldrin	6.34	6.35	6.25	6.45	0.01
4,4'-DDE	6.19	6.19	6.09	6.29	0.00
4,4'-DDD	6.70	6.70	6.60	6.80	0.00
4,4'-DDT	7.02	7.02	6.92	7.12	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Continuing Calib Date: 08/08/2025

Initial Calibration Date(s): 07/31/2025 07/31/2025

Continuing Calib Time: 17:43

Initial Calibration Time(s): 11:47 12:41

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	8.07	8.07	7.97	8.17	0.00
Tetrachloro-m-xylene	2.88	2.88	2.78	2.98	0.00
Aldrin	4.36	4.37	4.27	4.47	0.01
Dieldrin	5.51	5.51	5.41	5.61	0.00
4,4'-DDE	5.37	5.37	5.27	5.47	0.00
4,4'-DDD	5.92	5.93	5.83	6.03	0.01
4,4'-DDT	6.18	6.18	6.08	6.28	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance Contract: POWE02
 Lab Code: ACE SDG NO.: Q2795
 GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No.: CCAL02 Date Analyzed: 08/08/2025
 Lab Sample No.: PSTDCCC050 Data File : PD089821.D Time Analyzed: 17:43

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
4,4'-DDD	6.701	6.604	6.804	51.660	50.000	3.3
4,4'-DDE	6.192	6.094	6.294	48.680	50.000	-2.6
4,4'-DDT	7.017	6.919	7.119	42.180	50.000	-15.6
Aldrin	5.267	5.169	5.369	51.350	50.000	2.7
Decachlorobiphenyl	9.066	8.971	9.171	44.620	50.000	-10.8
Dieldrin	6.343	6.245	6.445	48.960	50.000	-2.1
Tetrachloro-m-xylene	3.547	3.448	3.648	51.380	50.000	2.8



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance Contract: POWE02
 Lab Code: ACE SDG NO.: Q2795
 GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No.: CCAL02 Date Analyzed: 08/08/2025
 Lab Sample No.: PSTDCCC050 Data File : PD089821.D Time Analyzed: 17:43

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
4,4'-DDD	5.924	5.825	6.025	57.790	50.000	15.6
4,4'-DDE	5.370	5.271	5.471	56.640	50.000	13.3
4,4'-DDT	6.178	6.079	6.279	51.020	50.000	2.0
Aldrin	4.364	4.265	4.465	57.180	50.000	14.4
Decachlorobiphenyl	8.066	7.968	8.168	47.200	50.000	-5.6
Dieldrin	5.508	5.409	5.609	56.430	50.000	12.9
Tetrachloro-m-xylene	2.878	2.778	2.978	56.850	50.000	13.7

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089821.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 17:43
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:35:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.878	126.7E6	900.4E6	51.384	56.853
2)	SA Decachlor...	9.066	8.066	165.8E6	947.7E6	44.623	47.199
Target Compounds							
2)	A alpha-BHC	3.997	3.390	261.8E6	1407.3E6	52.843	57.901
3)	MA gamma-BHC...	4.327	3.726	247.9E6	1289.7E6	52.168	57.260
4)	MA Heptachlor	4.926	4.079	228.7E6	1242.1E6	47.523	53.520
5)	MB Aldrin	5.267	4.364	234.4E6	1272.3E6	51.347	57.181
6)	B beta-BHC	4.513	4.022	95965997	547.5E6	52.023	56.740
7)	B delta-BHC	4.762	4.258	241.3E6	1303.6E6	52.619	57.389
8)	B Heptachlo...	5.687	4.868	207.7E6	1152.3E6	49.686	56.071
9)	A Endosulfan I	6.071	5.242	194.8E6	1034.4E6	49.136	52.914
10)	B gamma-Chl...	5.942	5.121	209.8E6	1235.1E6	50.195	57.041
11)	B alpha-Chl...	6.023	5.185	208.1E6	1178.2E6	49.488	56.584
12)	B 4,4'-DDE	6.192	5.370	181.6E6	1197.2E6	48.684	56.639
13)	MA Dieldrin	6.343	5.508	206.8E6	1221.1E6	48.959	56.431
14)	MA Endrin	6.570	5.785	166.2E6	1171.3E6	46.444	58.784 #
15)	B Endosulfa...	6.782	6.075	173.8E6	1036.9E6	47.360	55.157
16)	A 4,4'-DDD	6.701	5.924	154.7E6	1019.0E6	51.664	57.790
17)	MA 4,4'-DDT	7.017	6.178	141.7E6	937.3E6	42.180	51.017
18)	B Endrin al...	6.912	6.254	119.7E6	720.3E6	47.975	55.752
19)	B Endosulfa...	7.146	6.477	161.2E6	991.9E6	46.467	53.425
20)	A Methoxychlor	7.489	6.749	71823073	473.9E6	40.170	48.379
21)	B Endrin ke...	7.626	6.986	170.8E6	1075.3E6	45.980	53.582
22)	Mirex	8.109	7.179	123.2E6	796.7E6	44.173	52.343



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089821.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 17:43
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PSTDCCC050

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:35:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

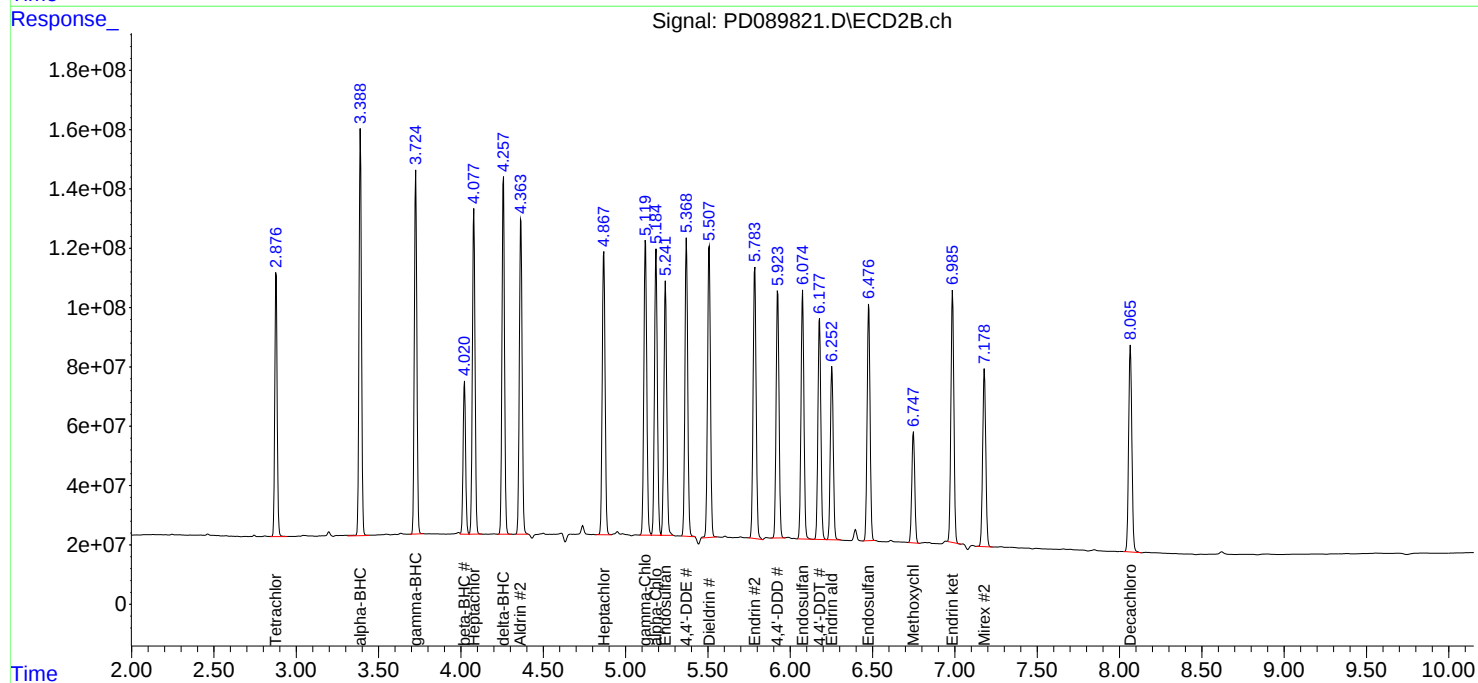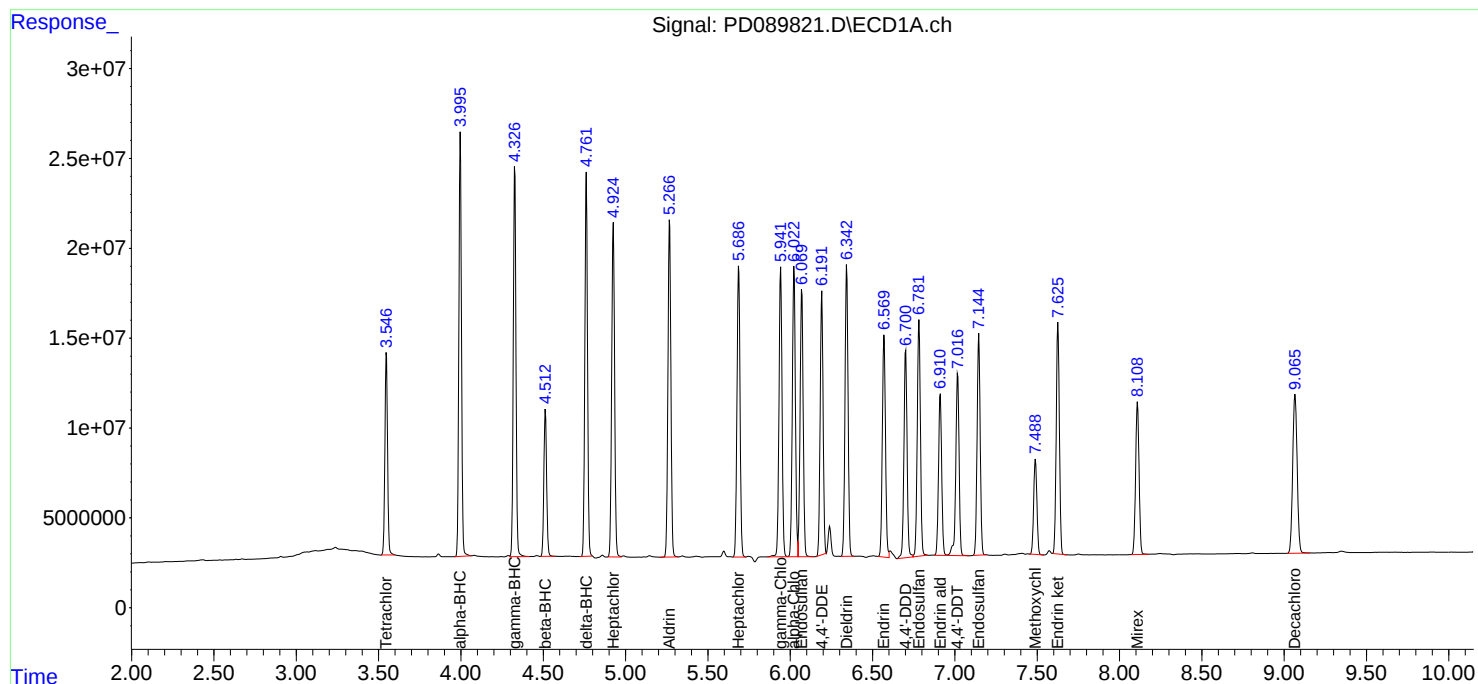



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Continuing Calib Date: 08/08/2025

Initial Calibration Date(s): 07/31/2025

07/31/2025

Continuing Calib Time: 19:46

Initial Calibration Time(s): 11:47

12:41

GC Column: ZB-MR1 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	9.07	9.07	8.97	9.17	0.00
Tetrachloro-m-xylene	3.55	3.55	3.45	3.65	0.00
Aldrin	5.27	5.27	5.17	5.37	0.00
Dieldrin	6.34	6.35	6.25	6.45	0.01
4,4'-DDE	6.19	6.19	6.09	6.29	0.00
4,4'-DDD	6.70	6.70	6.60	6.80	0.00
4,4'-DDT	7.02	7.02	6.92	7.12	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Continuing Calib Date: 08/08/2025

Initial Calibration Date(s): 07/31/2025 07/31/2025

Continuing Calib Time: 19:46

Initial Calibration Time(s): 11:47 12:41

GC Column: ZB-MR2 ID: 0.32 (mm)

COMPOUND	CCAL RT	AVG RT	RT WINDOW FROM TO		DIFF RT
Decachlorobiphenyl	8.07	8.07	7.97	8.17	0.00
Tetrachloro-m-xylene	2.88	2.88	2.78	2.98	0.00
Aldrin	4.37	4.37	4.27	4.47	0.01
Dieldrin	5.51	5.51	5.41	5.61	0.00
4,4'-DDE	5.37	5.37	5.27	5.47	0.00
4,4'-DDD	5.92	5.93	5.83	6.03	0.01
4,4'-DDT	6.18	6.18	6.08	6.28	0.00



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance **Contract:** POWE02
Lab Code: ACE **SDG NO.:** Q2795
GC Column: ZB-MR1 **ID:** 0.32 (mm) **Initi. Calib. Date(s):** 07/31/2025 07/31/2025

Client Sample No.: CCAL03 **Date Analyzed:** 08/08/2025
Lab Sample No.: PSTDCCC050 **Data File :** PD089829.D **Time Analyzed:** 19:46

COMPOUND	RT	RT WINDOW FROM TO		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
4,4'-DDD	6.702	6.604	6.804	50.340	50.000	0.7
4,4'-DDE	6.192	6.094	6.294	47.750	50.000	-4.5
4,4'-DDT	7.016	6.919	7.119	40.290	50.000	-19.4
Aldrin	5.267	5.169	5.369	50.440	50.000	0.9
Decachlorobiphenyl	9.067	8.971	9.171	44.280	50.000	-11.4
Dieldrin	6.343	6.245	6.445	47.040	50.000	-5.9
Tetrachloro-m-xylene	3.547	3.448	3.648	50.490	50.000	1.0



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance Contract: POWE02
 Lab Code: ACE SDG NO.: Q2795
 GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No.: CCAL03 Date Analyzed: 08/08/2025
 Lab Sample No.: PSTDCCC050 Data File : PD089829.D Time Analyzed: 19:46

COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
4,4'-DDD	5.923	5.825	6.025	57.320	50.000	14.6
4,4'-DDE	5.370	5.271	5.471	56.120	50.000	12.2
4,4'-DDT	6.178	6.079	6.279	48.390	50.000	-3.2
Aldrin	4.365	4.265	4.465	56.940	50.000	13.9
Decachlorobiphenyl	8.066	7.968	8.168	45.750	50.000	-8.5
Dieldrin	5.507	5.409	5.609	55.510	50.000	11.0
Tetrachloro-m-xylene	2.878	2.778	2.978	57.130	50.000	14.3

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089829.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 19:46
 Operator : AR\AJ
 Sample : PSTDCCC050
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PSTDCCC050

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:36:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.878	124.5E6	904.9E6	50.487	57.133
28)	SA Decachlor...	9.067	8.066	164.6E6	918.6E6	44.282	45.751
Target Compounds							
2)	A alpha-BHC	3.996	3.390	256.4E6	1401.1E6	51.771	57.647
3)	MA gamma-BHC...	4.327	3.726	242.4E6	1289.6E6	51.014	57.256
4)	MA Heptachlor	4.926	4.079	224.3E6	1241.2E6	46.610	53.481
5)	MB Aldrin	5.267	4.365	230.3E6	1267.0E6	50.442	56.942
6)	B beta-BHC	4.513	4.022	93596272	547.5E6	50.739	56.746
7)	B delta-BHC	4.762	4.258	235.0E6	1293.4E6	51.246	56.941
8)	B Heptachlo...	5.687	4.868	203.8E6	1144.7E6	48.751	55.704
9)	A Endosulfan I	6.070	5.242	189.7E6	1026.4E6	47.868	52.507
10)	B gamma-Chl...	5.942	5.120	205.6E6	1228.3E6	49.201	56.727
11)	B alpha-Chl...	6.023	5.185	203.6E6	1171.5E6	48.424	56.261
12)	B 4,4'-DDE	6.192	5.370	178.1E6	1186.3E6	47.745	56.124
13)	MA Dieldrin	6.343	5.507	198.7E6	1201.3E6	47.042	55.514
14)	MA Endrin	6.570	5.784	156.7E6	1139.3E6	43.795	57.179 #
15)	B Endosulfa...	6.783	6.075	168.1E6	1017.8E6	45.822	54.141
16)	A 4,4'-DDD	6.702	5.923	150.8E6	1010.7E6	50.339	57.318
17)	MA 4,4'-DDT	7.016	6.178	135.4E6	889.0E6	40.288m	48.387
18)	B Endrin al...	6.911	6.253	115.1E6	696.2E6	46.106	53.887
19)	B Endosulfa...	7.145	6.477	153.9E6	960.5E6	44.362	51.735
20)	A Methoxychlor	7.489	6.748	65629351	446.4E6	36.706	45.576
21)	B Endrin ke...	7.627	6.986	164.4E6	1051.5E6	44.259	52.395
22)	Mirex	8.109	7.179	118.1E6	785.1E6	42.363	51.582

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089829.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 19:46
Operator : AR\AJ
Sample : PSTDCCC050
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

PSTDCCC050

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 08/11/2025

Supervised By :mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:36:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

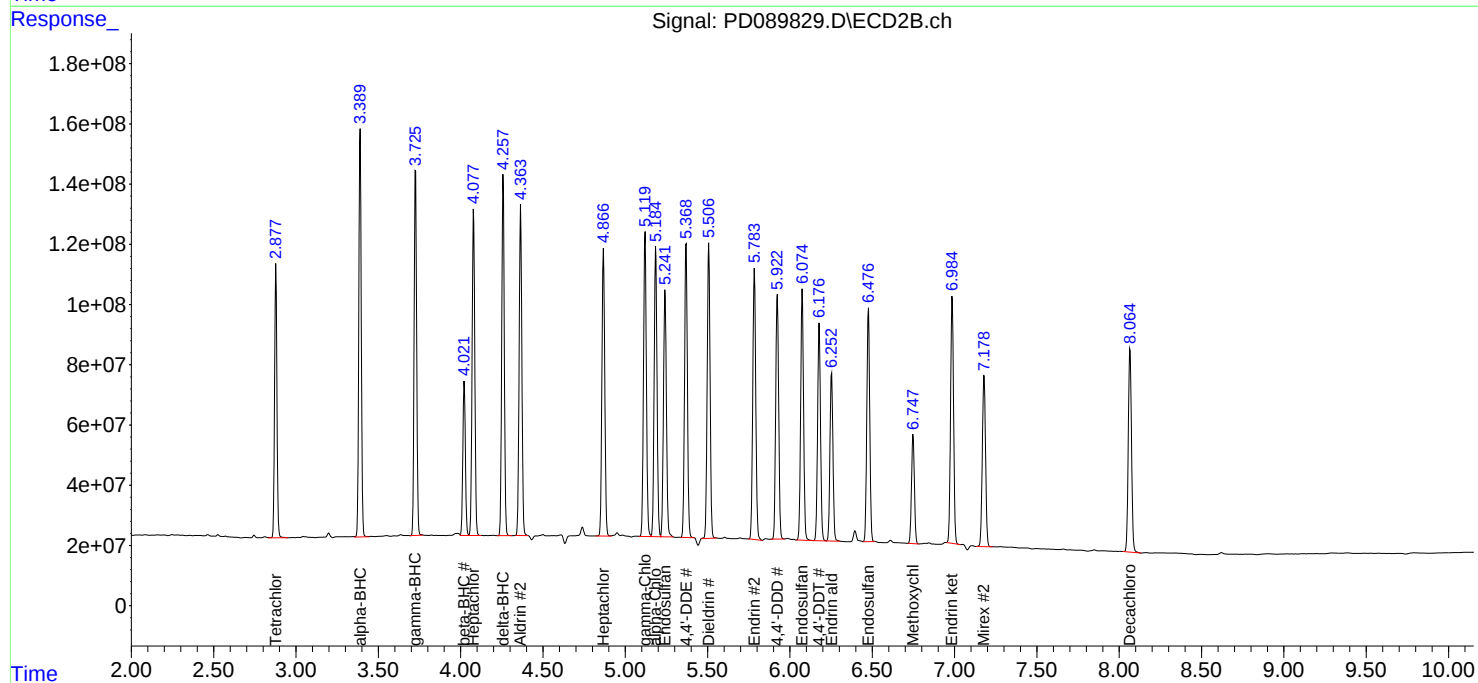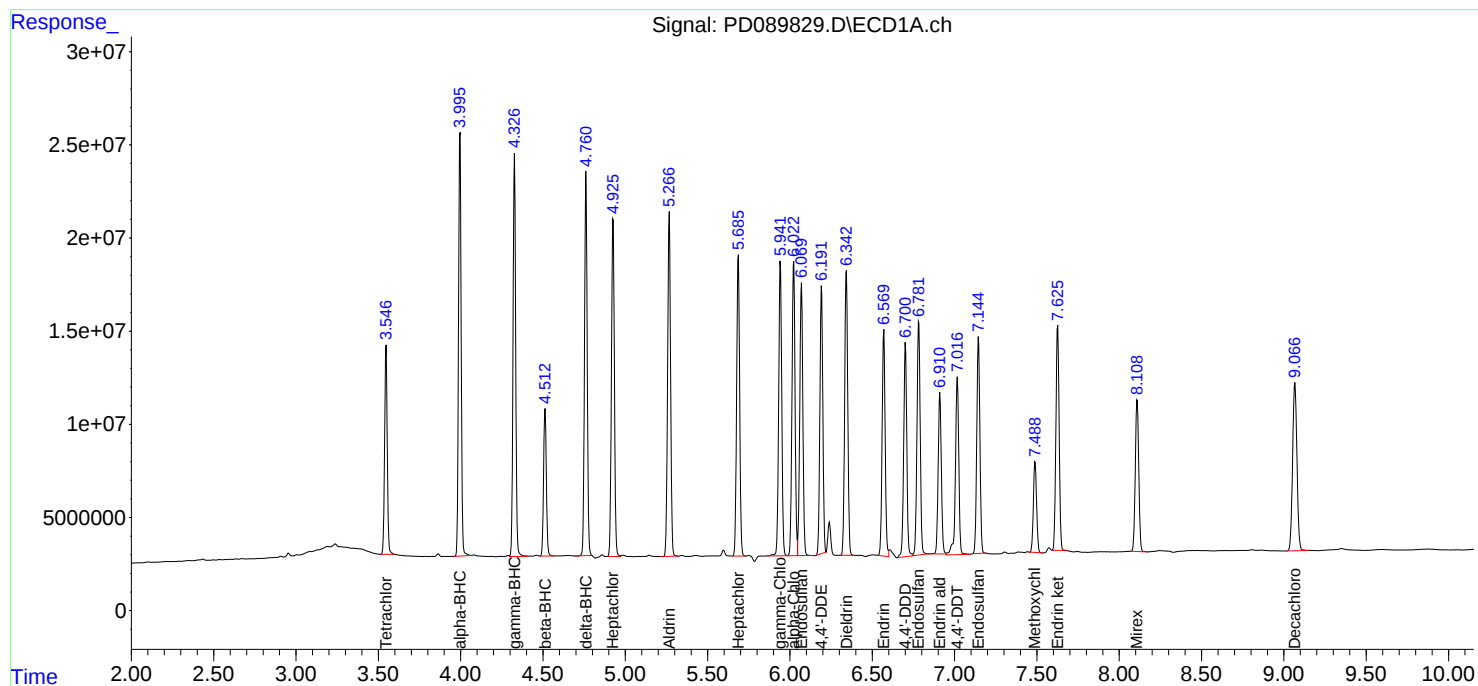

PESTICIDE CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No. (PEM): PEM - PD089686.D Date Analyzed: 07/31/2025

Lab Sample No.(PEM): PEM Time Analyzed: 10:47

PEM COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	9.070	8.970	9.170	21.540	20.000	7.7
Tetrachloro-m-xylene	3.548	3.500	3.600	20.670	20.000	3.4
alpha-BHC	3.997	3.950	4.050	9.820	10.000	-1.8
beta-BHC	4.514	4.460	4.560	10.760	10.000	7.6
gamma-BHC (Lindane)	4.328	4.280	4.380	10.080	10.000	0.8
Endrin	6.572	6.500	6.640	54.730	50.000	9.5
4,4'-DDT	7.020	6.950	7.090	108.560	100.000	8.6
Methoxychlor	7.491	7.420	7.560	258.930	250.000	3.6

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No. (PEM): PEM - PD089686.D Date Analyzed: 07/31/2025

Lab Sample No.(PEM): PEM Time Analyzed: 10:47

PEM COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	8.068	7.970	8.170	22.080	20.000	10.4
Tetrachloro-m-xylene	2.878	2.830	2.930	21.990	20.000	10.0
alpha-BHC	3.390	3.340	3.440	11.660	10.000	16.6
beta-BHC	4.022	3.970	4.070	11.840	10.000	18.4
gamma-BHC (Lindane)	3.726	3.680	3.780	11.700	10.000	17.0
Endrin	5.785	5.710	5.860	54.470	50.000	8.9
4,4'-DDT	6.179	6.110	6.250	108.020	100.000	8.0
Methoxychlor	6.750	6.680	6.820	237.190	250.000	-5.1

PEM
 Data File: PD089686.D Date Acquired 7/31/2025 10:47
 Operator: AR\AJ

ENDRIN BREAK DOWN

Column #1

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin	6.57	195800927	198957010.7	3156083.71	1.59
Endrin aldehyde	6.92	642295.992			
Endrin ketone	7.63	2513787.715			

Column #2

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin #2	5.78	1085241845	1112231636	26989790.8	2.43
Endrin aldehyde #2	6.25	9551952.382			
Endrin ketone #2	6.98	17437838.39			

DDT BREAK DOWN

Column #1

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT	7.02	364771708.3	367822517.1	3050808.84	0.83
4,4'-DDE	6.20	669534.489			
4,4'-DDD	6.70	2381274.353			

Column #2

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT #2	6.18	1984665033	2003214267	18549234.1	0.93
4,4'-DDE #2	5.37	2329969.565			
4,4'-DDD #2	5.93	16219264.57			

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 10:47
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEM

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 08/01/2025
 Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 07:05:25 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.878	50972762	348.2E6	20.665	21.988
28)	SA Decachlor...	9.070	8.068	80035568	443.4E6	21.537	22.084
Target Compounds							
2)	A alpha-BHC	3.997	3.390	48629241	283.5E6	9.817	11.664
3)	MA gamma-BHC...	4.328	3.726	47886972	263.6E6	10.076	11.702
6)	B beta-BHC	4.514	4.022	19846516	114.3E6	10.759	11.842
12)	B 4,4'-DDE	6.196	5.371	669534	2329970	0.180m	0.110m#
14)	MA Endrin	6.572	5.785	195.8E6	1085.2E6	54.728	54.466
16)	A 4,4'-DDD	6.703	5.926	2381274	16219265	0.795	0.920m
17)	MA 4,4'-DDT	7.020	6.179	364.8E6	1984.7E6	108.555	108.023
18)	B Endrin al...	6.915	6.253	642296	9551952	0.257	0.739 #
20)	A Methoxychlor	7.491	6.750	463.0E6	2323.4E6	258.926	237.192
21)	B Endrin ke...	7.627	6.985	2513788	17437838	0.677m	0.869m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 10:47
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PEM

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 08/01/2025
Supervised By :mohammad ahmed 08/01/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:05:25 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

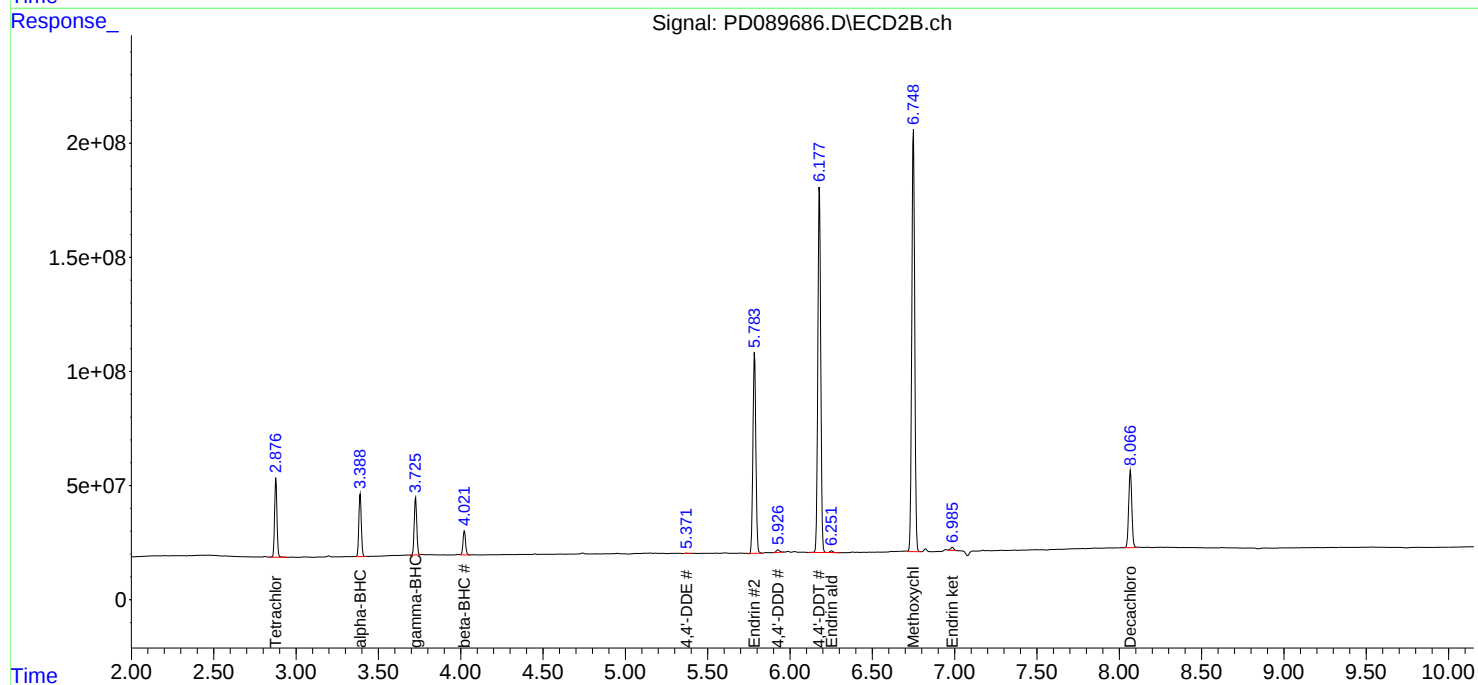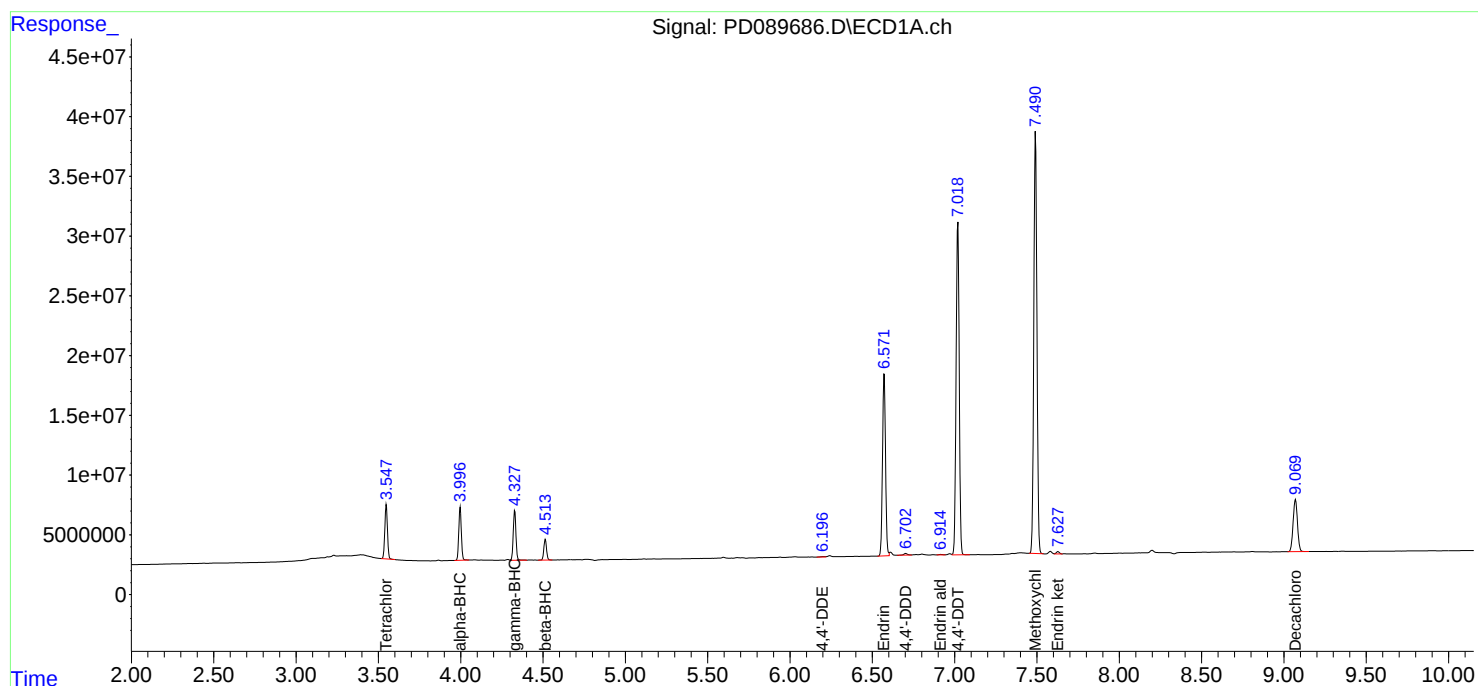

PESTICIDE CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

GC Column: ZB-MR1 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No. (PEM): PEM - PD089809.D Date Analyzed: 08/08/2025

Lab Sample No.(PEM): PEM Time Analyzed: 11:10

PEM COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	9.066	8.970	9.170	22.450	20.000	12.3
Tetrachloro-m-xylene	3.547	3.500	3.600	23.610	20.000	18.1
alpha-BHC	3.996	3.950	4.050	11.230	10.000	12.3
beta-BHC	4.513	4.460	4.560	12.370	10.000	23.7
gamma-BHC (Lindane)	4.327	4.280	4.380	11.720	10.000	17.2
Endrin	6.570	6.500	6.640	53.250	50.000	6.5
4,4'-DDT	7.017	6.950	7.090	97.430	100.000	-2.6
Methoxychlor	7.489	7.420	7.560	219.750	250.000	-12.1

GC Column: ZB-MR2 ID: 0.32 (mm) Initi. Calib. Date(s): 07/31/2025 07/31/2025

Client Sample No. (PEM): PEM - PD089809.D Date Analyzed: 08/08/2025

Lab Sample No.(PEM): PEM Time Analyzed: 11:10

PEM COMPOUND	RT	RT WINDOW		CALC AMOUNT(ng)	NOM AMOUNT(ng)	%D
		FROM	TO			
Decachlorobiphenyl	8.064	7.960	8.160	20.370	20.000	1.9
Tetrachloro-m-xylene	2.877	2.830	2.930	25.360	20.000	26.8
alpha-BHC	3.389	3.340	3.440	13.870	10.000	38.7
beta-BHC	4.021	3.970	4.070	13.880	10.000	38.8
gamma-BHC (Lindane)	3.725	3.670	3.780	13.660	10.000	36.6
Endrin	5.783	5.710	5.850	56.660	50.000	13.3
4,4'-DDT	6.177	6.110	6.250	109.020	100.000	9.0
Methoxychlor	6.748	6.680	6.820	210.340	250.000	-15.9

PEM
 Data File: PD089809.D Date Acquired 8/8/2025 11:10
 Operator: AR\AJ

ENDRIN BREAK DOWN

Column #1

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin	6.57	190501921.4	202599463	12097541.6	5.97
Endrin aldehyde	6.91	2918965.689			
Endrin ketone	7.63	9178575.952			

Column #2

Name	RT	Response	Response [E+EA+EK]	Response [EA+EK]	% Break Down
Endrin #2	5.78	1128923689	1229939118	101015430	8.21
Endrin aldehyde #2	6.25	23900436.66			
Endrin ketone #2	6.98	77114993.03			

DDT BREAK DOWN

Column #1

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT	7.02	327385575.2	343431573.7	16045998.5	4.67
4,4'-DDE	6.19	594995.688			
4,4'-DDD	6.70	15451002.79			

Column #2

Name	RT	Response	Response [DDT+DDE+DDD]	Response [DDE+DDD]	% Break Down
4,4'-DDT #2	6.18	2002935628	2111215270	108279642	5.13
4,4'-DDE #2	5.37	3960300.075			
4,4'-DDD #2	5.92	104319342.3			

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089809.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 11:10
 Operator : AR\AJ
 Sample : PEM
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PEM

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:33:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	58246714	401.6E6	23.614	25.358
28)	SA Decachlor...	9.066	8.064	83415937	408.9E6	22.446	20.365
Target Compounds							
2)	A alpha-BHC	3.996	3.389	55613989	337.1E6	11.227	13.868
3)	MA gamma-BHC...	4.327	3.725	55719510	307.7E6	11.725	13.662
6)	B beta-BHC	4.513	4.021	22817545	134.0E6	12.369	13.883
12)	B 4,4'-DDE	6.190	5.371	594996	3960300	0.160m	0.187
14)	MA Endrin	6.570	5.783	190.5E6	1128.9E6	53.247	56.658
16)	A 4,4'-DDD	6.701	5.923	15451003	104.3E6	5.159	5.916
17)	MA 4,4'-DDT	7.017	6.177	327.4E6	2002.9E6	97.429	109.017
18)	B Endrin al...	6.912	6.252	2918966	23900437	1.170	1.850 #
20)	A Methoxychlor	7.489	6.748	392.9E6	2060.4E6	219.748	210.344
21)	B Endrin ke...	7.626	6.985	9178576	77114993	2.471	3.843 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089809.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 11:10
Operator : AR\AJ
Sample : PEM
Misc :
ALS Vial : 3 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
PEM

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 08/11/2025
Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:33:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

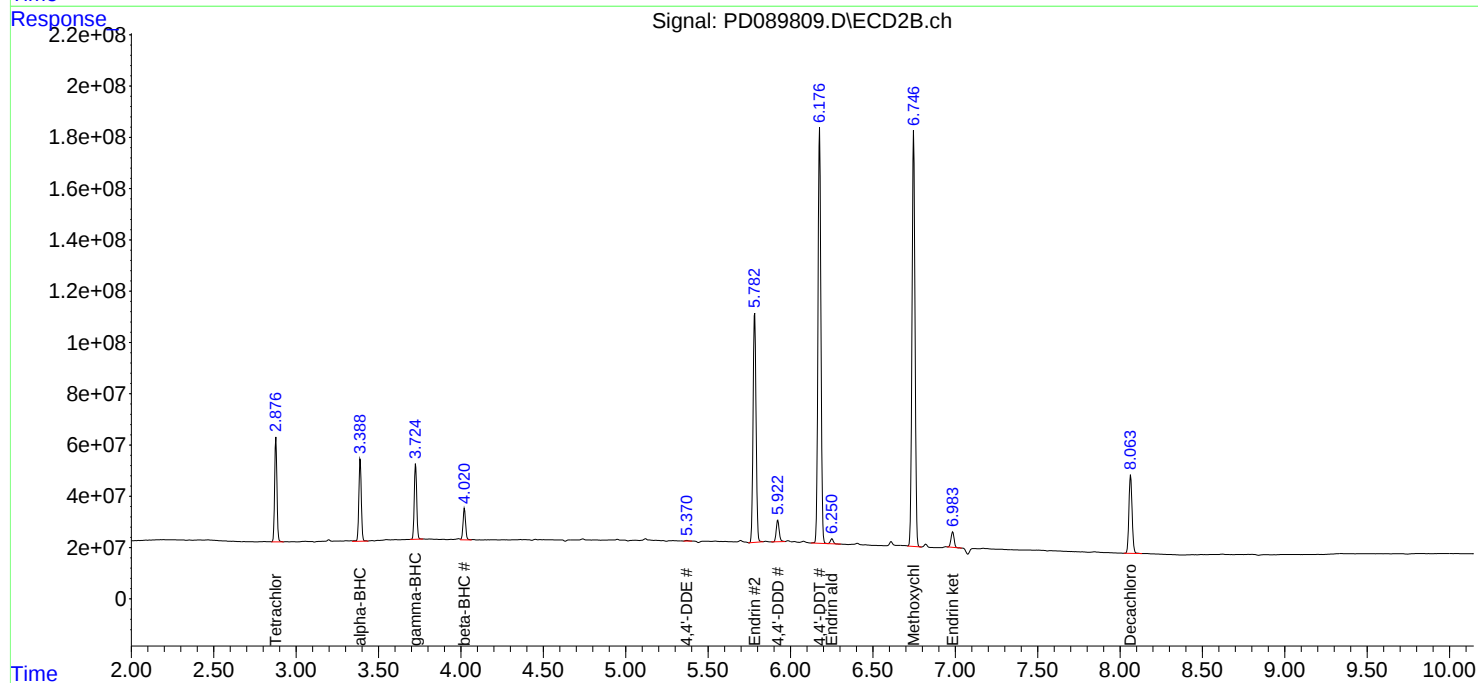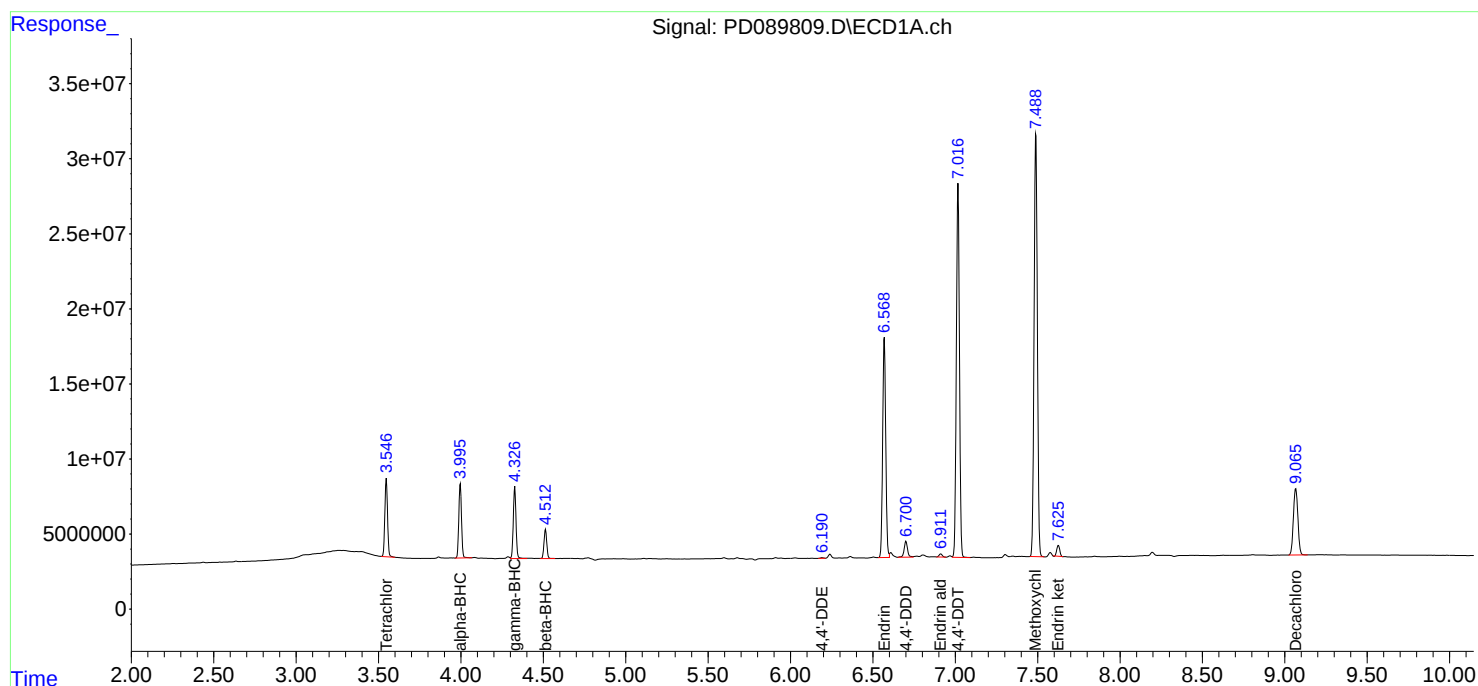

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089687.D
Acq On : 31 Jul 2025 11:34
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e

Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Title : GC Extractables
Last Update : Fri Aug 01 07:03:58 2025
Integrator: ChemStation

RT#1	RT#2	Resolution
3.555	5.952	100.00%
5.952	6.080	100.00%
6.080	6.202	100.00%
6.202	6.353	100.00%
6.353	7.156	100.00%
7.156	7.501	100.00%
7.501	7.637	100.00%
7.637	9.080	100.00%

Signal #2

2.877	5.123	100.00%
5.123	5.243	100.00%
5.243	5.372	100.00%
5.372	5.510	100.00%
5.510	6.480	100.00%
6.480	6.752	100.00%
6.752	6.989	100.00%
6.989	8.070	100.00%

PD073125.M Fri Aug 01 08:58:30 2025

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
 Data File : PD089687.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Jul 2025 11:34
 Operator : AR\AJ
 Sample : RESCHK
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 RESCHK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 07:05:37 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.877	43497342	289.6E6	17.635	18.287
28)	SA Decachlor...	9.080	8.070	68540687	368.9E6	18.443	18.373
Target Compounds							
9)	A Endosulfan I	6.080	5.243	32929310	180.8E6	8.308	9.250
10)	B gamma-Chl...	5.952	5.123	36168921	212.0E6	8.655	9.788
12)	B 4,4'-DDE	6.202	5.372	65872916	408.9E6	17.661	19.345
13)	MA Dieldrin	6.353	5.510	73492529	408.2E6	17.401	18.863
19)	B Endosulfa...	7.156	6.480	62490576	353.7E6	18.008	19.054
20)	A Methoxychlor	7.501	6.752	158.7E6	839.7E6	88.775	85.727
21)	B Endrin ke...	7.637	6.989	66017266	381.6E6	17.775	19.017



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089687.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 11:34
Operator : AR\AJ
Sample : RESCHK
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
RESCHK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:05:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

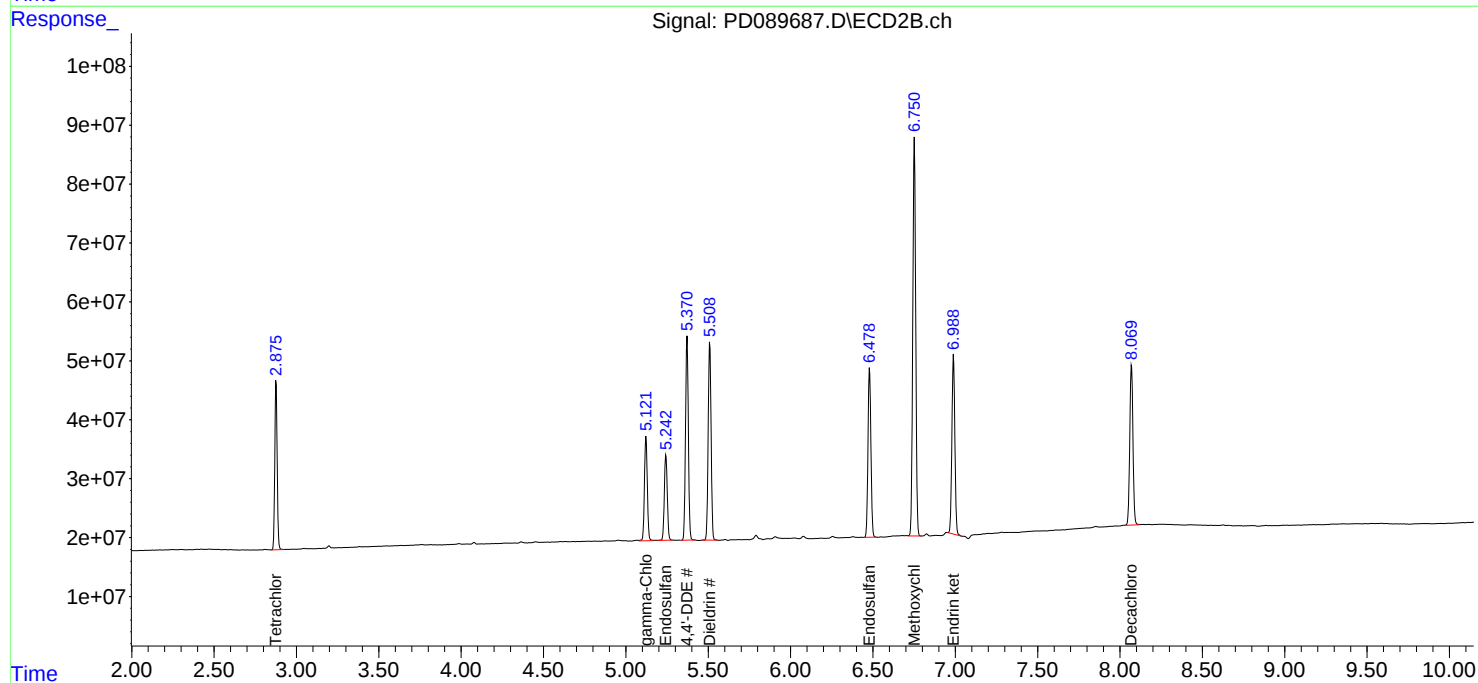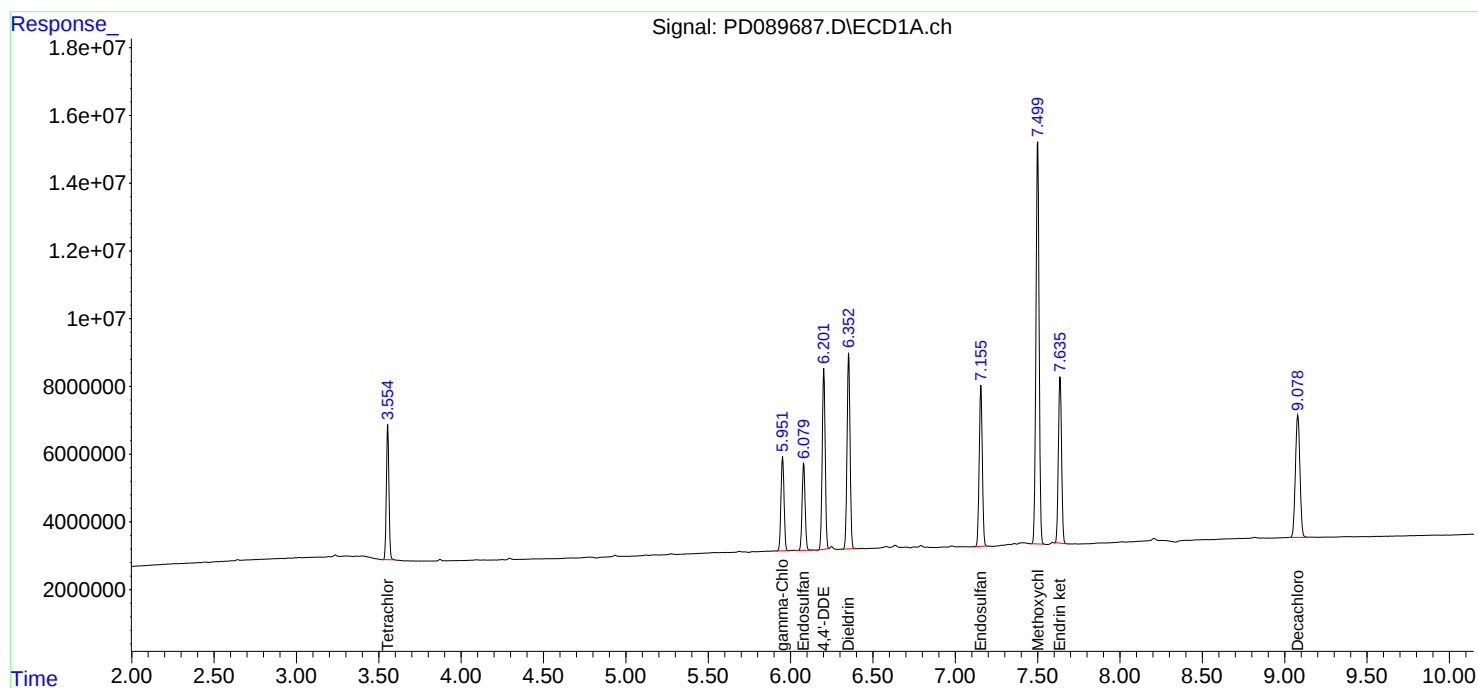

Analytical Sequence

Client: Kleinfelder

SDG No.: Q2795

Project: Girard school

Instrument ID: ECD_D

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 07/31/2025 07/31/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	07/31/2025	10:33	PD089685.D	9.08	3.56
PEM	PEM	07/31/2025	10:47	PD089686.D	9.07	3.55
RESCHK	RESCHK	07/31/2025	11:34	PD089687.D	9.08	3.56
PSTDICC100	PSTDICC100	07/31/2025	11:47	PD089688.D	9.07	3.55
PSTDICC075	PSTDICC075	07/31/2025	12:01	PD089689.D	9.07	3.55
PSTDICC050	PSTDICC050	07/31/2025	12:14	PD089690.D	9.07	3.55
PSTDICC025	PSTDICC025	07/31/2025	12:28	PD089691.D	9.07	3.55
PSTDICC005	PSTDICC005	07/31/2025	12:41	PD089692.D	9.07	3.55
PCHLORICC500	PCHLORICC500	07/31/2025	13:23	PD089695.D	9.07	3.55
PTOXICC500	PTOXICC500	07/31/2025	14:31	PD089700.D	9.07	3.55
IBLK	IBLK	08/08/2025	10:57	PD089808.D	9.07	3.55
PEM	PEM	08/08/2025	11:10	PD089809.D	9.07	3.55
PSTDCCC050	PSTDCCC050	08/08/2025	13:53	PD089810.D	9.07	3.55
PB169173BL	PB169173BL	08/08/2025	14:51	PD089811.D	9.08	3.56
PB169173BS	PB169173BS	08/08/2025	15:18	PD089812.D	9.08	3.55
IBLK	IBLK	08/08/2025	17:29	PD089820.D	9.07	3.55
PSTDCCC050	PSTDCCC050	08/08/2025	17:43	PD089821.D	9.07	3.55
COMP-1	Q2795-01	08/08/2025	18:10	PD089822.D	9.07	3.55
COMP-1MS	Q2795-01MS	08/08/2025	18:24	PD089823.D	9.07	3.55
COMP-1MSD	Q2795-01MSD	08/08/2025	18:37	PD089824.D	9.07	3.55
COMP-2	Q2795-02	08/08/2025	18:51	PD089825.D	9.07	3.55
COMP-3	Q2795-03	08/08/2025	19:05	PD089826.D	9.07	3.55
IBLK	IBLK	08/08/2025	19:32	PD089828.D	9.07	3.55
PSTDCCC050	PSTDCCC050	08/08/2025	19:46	PD089829.D	9.07	3.55

Analytical Sequence

Client: Kleinfelder

SDG No.: Q2795

Project: Girard school

Instrument ID: ECD_D

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 07/31/2025

07/31/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES,
AND STANDARDS IS GIVEN BELOW:

CLIENT ID	LAB SAMPLE ID	DATE ANALYZED	TIME ANALYZED	DATAFILE	DCB RT #	TCX RT #
IBLK	IBLK	07/31/2025	10:33	PD089685.D	8.07	2.88
PEM	PEM	07/31/2025	10:47	PD089686.D	8.07	2.88
RESCHK	RESCHK	07/31/2025	11:34	PD089687.D	8.07	2.88
PSTDICC100	PSTDICC100	07/31/2025	11:47	PD089688.D	8.07	2.88
PSTDICC075	PSTDICC075	07/31/2025	12:01	PD089689.D	8.07	2.88
PSTDICC050	PSTDICC050	07/31/2025	12:14	PD089690.D	8.07	2.88
PSTDICC025	PSTDICC025	07/31/2025	12:28	PD089691.D	8.07	2.88
PSTDICC005	PSTDICC005	07/31/2025	12:41	PD089692.D	8.07	2.88
PCHLORICC500	PCHLORICC500	07/31/2025	13:23	PD089695.D	8.07	2.88
PTOXICC500	PTOXICC500	07/31/2025	14:31	PD089700.D	8.07	2.88
IBLK	IBLK	08/08/2025	10:57	PD089808.D	8.07	2.88
PEM	PEM	08/08/2025	11:10	PD089809.D	8.06	2.88
PSTDCCC050	PSTDCCC050	08/08/2025	13:53	PD089810.D	8.07	2.88
PB169173BL	PB169173BL	08/08/2025	14:51	PD089811.D	8.07	2.88
PB169173BS	PB169173BS	08/08/2025	15:18	PD089812.D	8.07	2.88
IBLK	IBLK	08/08/2025	17:29	PD089820.D	8.07	2.88
PSTDCCC050	PSTDCCC050	08/08/2025	17:43	PD089821.D	8.07	2.88
COMP-1	Q2795-01	08/08/2025	18:10	PD089822.D	8.07	2.88
COMP-1MS	Q2795-01MS	08/08/2025	18:24	PD089823.D	8.07	2.88
COMP-1MSD	Q2795-01MSD	08/08/2025	18:37	PD089824.D	8.07	2.88
COMP-2	Q2795-02	08/08/2025	18:51	PD089825.D	8.07	2.88
COMP-3	Q2795-03	08/08/2025	19:05	PD089826.D	8.07	2.88
IBLK	IBLK	08/08/2025	19:32	PD089828.D	8.07	2.88
PSTDCCC050	PSTDCCC050	08/08/2025	19:46	PD089829.D	8.07	2.88

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

COMP-1MS

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Lab Sample ID: Q2795-01MS

Date(s) Analyzed: 08/08/2025 08/08/2025

Instrument ID (1): ECD_D

Instrument ID (2): ECD_D

GC Column: (1): ZB-MR1

ID: 0.32 (mm)

GC Column:(2): ZB-MR2

ID: 0.32 (mm)

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
4,4'-DDD	1	6.70	6.65	6.75	19.7	11.5
	2	5.92	5.87	5.97	22.1	
4,4'-DDT	1	7.02	6.97	7.07	13.8	27
	2	6.18	6.13	6.23	18.1	
Aldrin	1	5.27	5.22	5.32	20.2	11.2
	2	4.36	4.31	4.41	22.6	
4,4'-DDE	1	6.19	6.14	6.24	19.2	15.8
	2	5.37	5.32	5.42	22.5	
Dieldrin	1	6.34	6.29	6.39	17.6	17.1
	2	5.51	5.46	5.56	20.9	

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

COMP-1MSD

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Lab Sample ID: Q2795-01MSD

Date(s) Analyzed: 08/08/2025 08/08/2025

Instrument ID (1): ECD_D

Instrument ID (2): ECD_D

GC Column: (1): ZB-MR1

ID: 0.32 (mm)

GC Column:(2): ZB-MR2

ID: 0.32 (mm)

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
4,4'-DDD	1	6.70	6.65	6.75	19.9	10
	2	5.93	5.88	5.98	22.0	
4,4'-DDT	1	7.02	6.97	7.07	15.5	23.9
	2	6.18	6.13	6.23	19.7	
Aldrin	1	5.27	5.22	5.32	20.1	11.7
	2	4.36	4.31	4.41	22.6	
4,4'-DDE	1	6.19	6.14	6.24	19.5	13.4
	2	5.37	5.32	5.42	22.3	
Dieldrin	1	6.34	6.29	6.39	18.7	15.8
	2	5.51	5.46	5.56	21.9	

COMPOUND DETECTION SUMMARY

CLIENT SAMPLE NO.

PB169173BS

Lab Name: Alliance

Contract: POWE02

Lab Code: ACE

SDG NO.: Q2795

Lab Sample ID: PB169173BS

Date(s) Analyzed: 08/08/2025 08/08/2025

Instrument ID (1): ECD_D

Instrument ID (2): ECD_D

GC Column: (1): ZB-MR1

ID: 0.32 (mm)

GC Column:(2): ZB-MR2

ID: 0.32 (mm)

ANALYTE	COL	RT	RT WINDOW		CONCENTRATION	%RPD
			FROM	TO		
4,4'-DDD	1	6.71	6.66	6.76	15.9	15.1
	2	5.93	5.88	5.98	18.5	
4,4'-DDE	1	6.20	6.15	6.25	15.6	12.6
	2	5.37	5.32	5.42	17.7	
4,4'-DDT	1	7.03	6.98	7.08	13.8	17.2
	2	6.18	6.13	6.23	16.4	
Aldrin	1	5.28	5.23	5.33	16.0	10.1
	2	4.36	4.31	4.41	17.7	
Dieldrin	1	6.35	6.30	6.40	15.5	12.7
	2	5.51	5.46	5.56	17.6	



QC SAMPLE DATA

Report of Analysis

Client:	Kleinfelder	Date Collected:	
Project:	Girard school	Date Received:	
Client Sample ID:	PB169173BL	SDG No.:	Q2795
Lab Sample ID:	PB169173BL	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	100 Decanted:
Sample Wt/Vol:	30.02 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089811.D	1	08/08/25 08:43	08/08/25 14:51	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	0.12	U	0.12	1.70	ug/kg
60-57-1	Dieldrin	0.14	U	0.14	1.70	ug/kg
72-55-9	4,4-DDE	0.14	U	0.14	1.70	ug/kg
72-54-8	4,4-DDD	0.15	U	0.15	1.70	ug/kg
50-29-3	4,4-DDT	0.14	U	0.14	1.70	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	18.9		20 - 144	95%	SPK: 20
877-09-8	Tetrachloro-m-xylene	21.8		19 - 148	109%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089811.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 14:51
 Operator : AR\AJ
 Sample : PB169173BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB169173BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:34:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.877	45692738	345.3E6	18.525	21.803
28)	SA Decachlor...	9.078	8.068	68432234	379.9E6	18.414	18.922

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089811.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 14:51
Operator : AR\AJ
Sample : PB169173BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PB169173BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:34:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

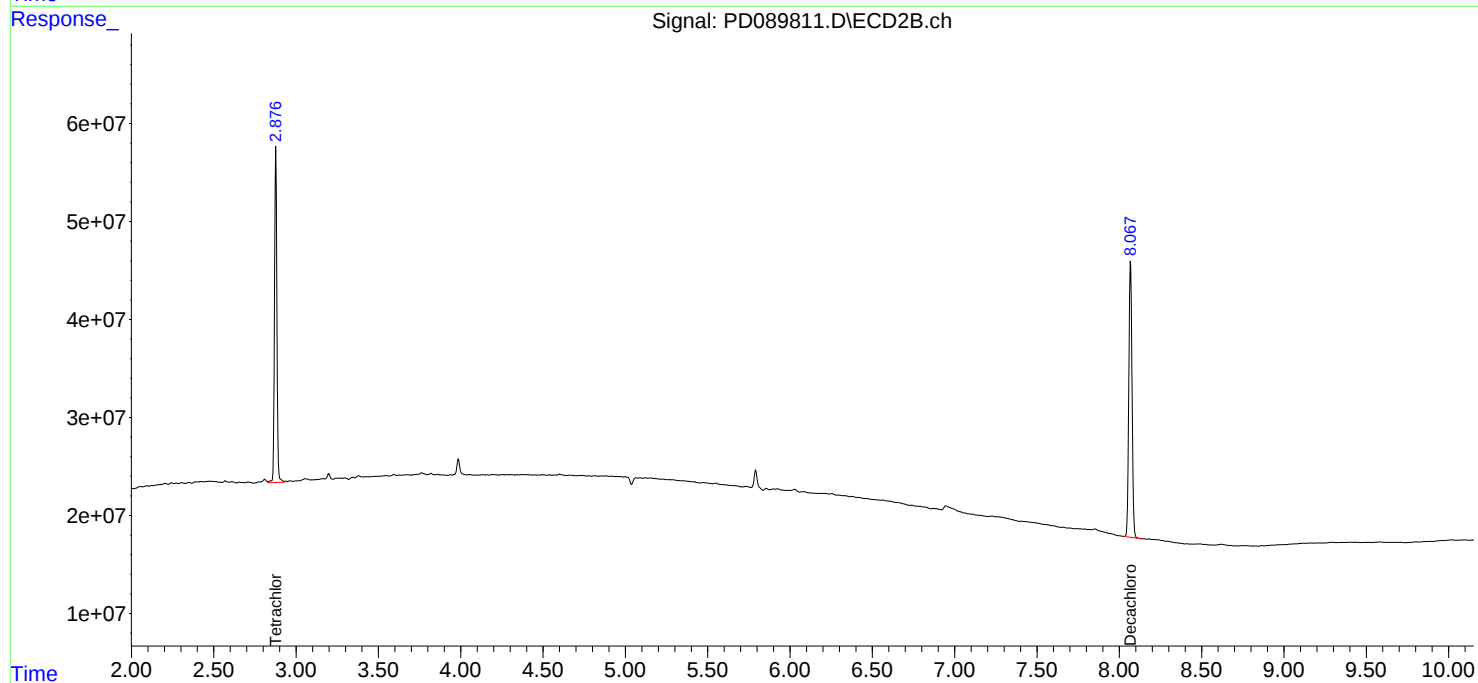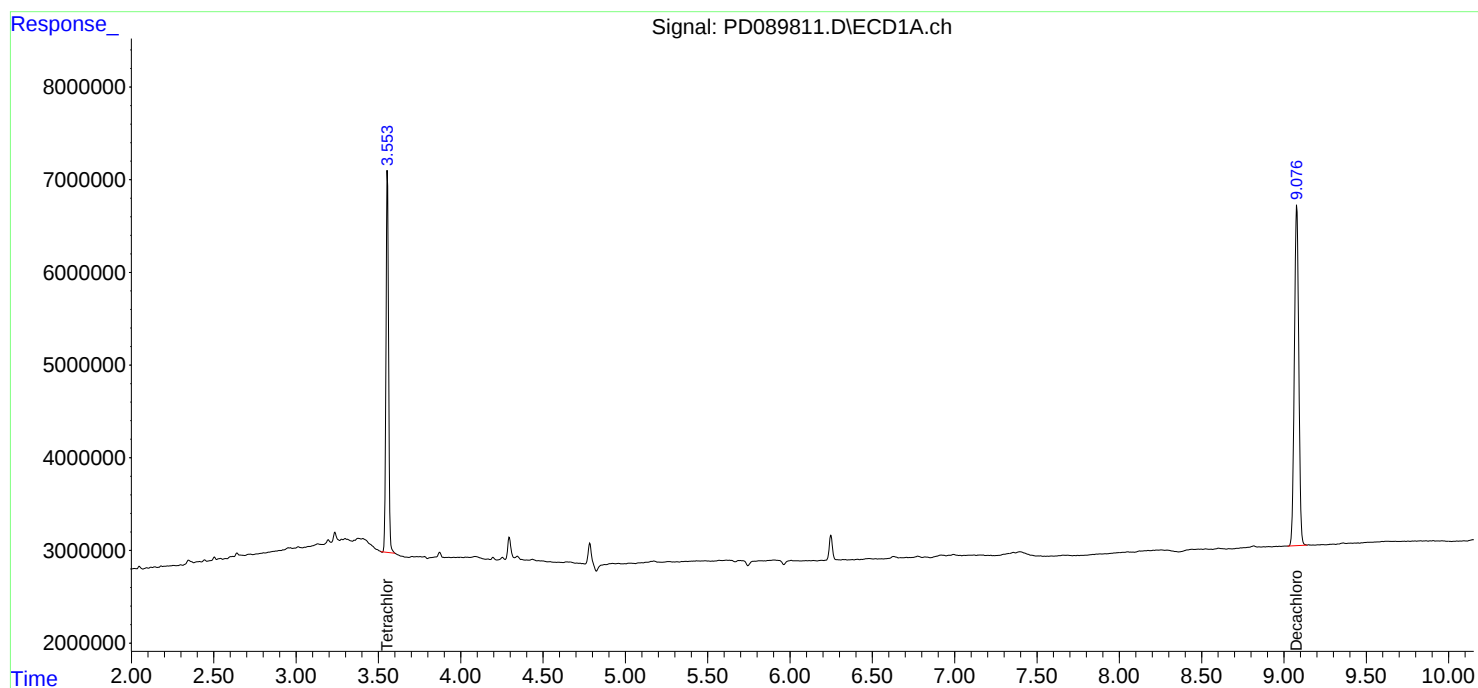


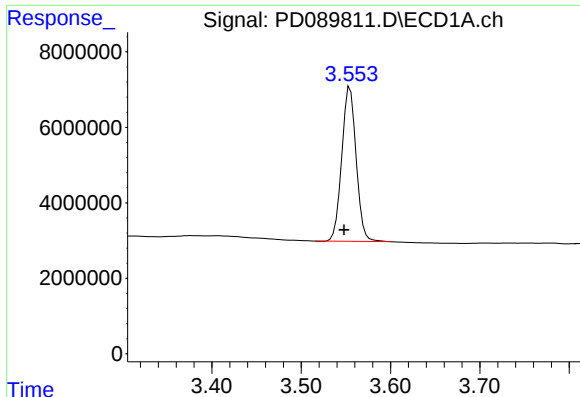

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.007 min
Response: 45692738
Conc: 18.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PB169173BL

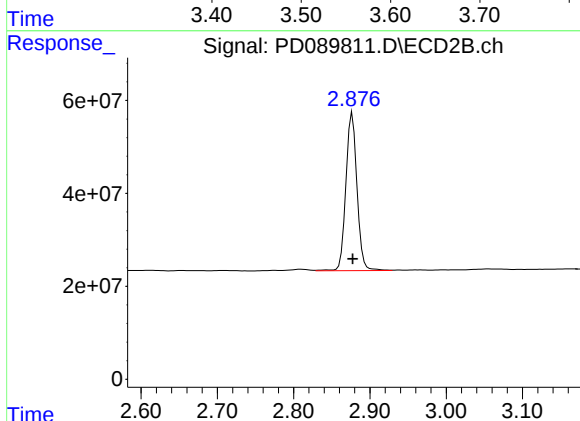


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 345319716
Conc: 21.80 ng/ml

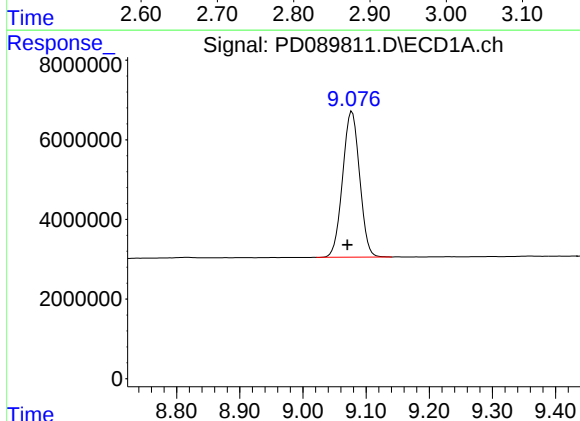

#28 Decachlorobiphenyl

R.T.: 9.078 min
Delta R.T.: 0.007 min
Response: 68432234
Conc: 18.41 ng/ml

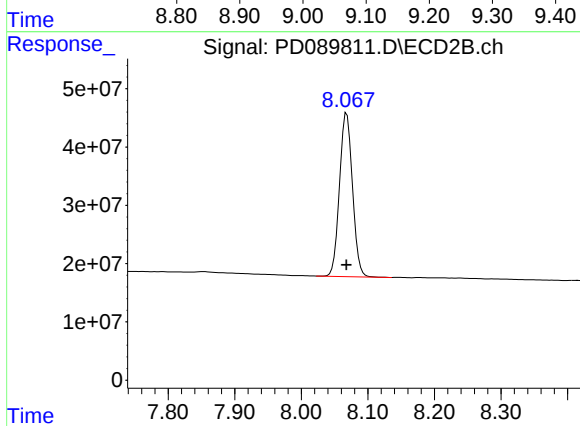

#28 Decachlorobiphenyl

R.T.: 8.068 min
Delta R.T.: 0.000 min
Response: 379922141
Conc: 18.92 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	07/31/25
Project:	Girard school	Date Received:	07/31/25
Client Sample ID:	PIBLK-PD089685.D	SDG No.:	Q2795
Lab Sample ID:	I.BLK-PD089685.D	Matrix:	WATER
Analytical Method:	8081B	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PESTICIDE Group1
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089685.D	1		07/31/25	pd073125

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
309-00-2	Aldrin	0.0036	U	0.0036	0.050	ug/L
60-57-1	Dieldrin	0.0036	U	0.0036	0.050	ug/L
72-55-9	4,4-DDE	0.0037	U	0.0037	0.050	ug/L
72-54-8	4,4-DDD	0.0071	U	0.0071	0.050	ug/L
50-29-3	4,4-DDT	0.0035	U	0.0035	0.050	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	20.9		57 - 171	104%	SPK: 20
877-09-8	Tetrachloro-m-xylene	20.4		61 - 148	102%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 10:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:05:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.555	2.877	48438502	323.8E6	19.638	20.442
28)	SA Decachlor...	9.080	8.070	77499630	419.1E6	20.854	20.872

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD073125\
Data File : PD089685.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Jul 2025 10:33
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 07:05:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

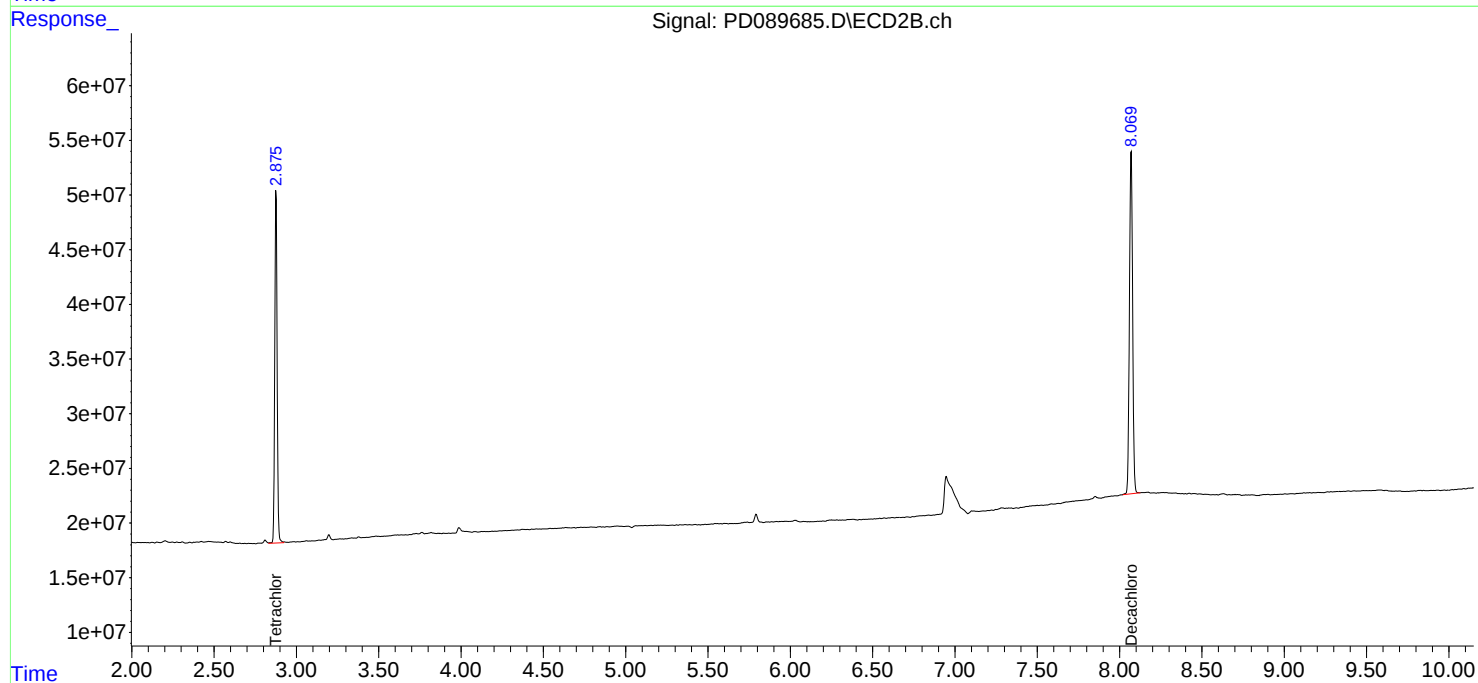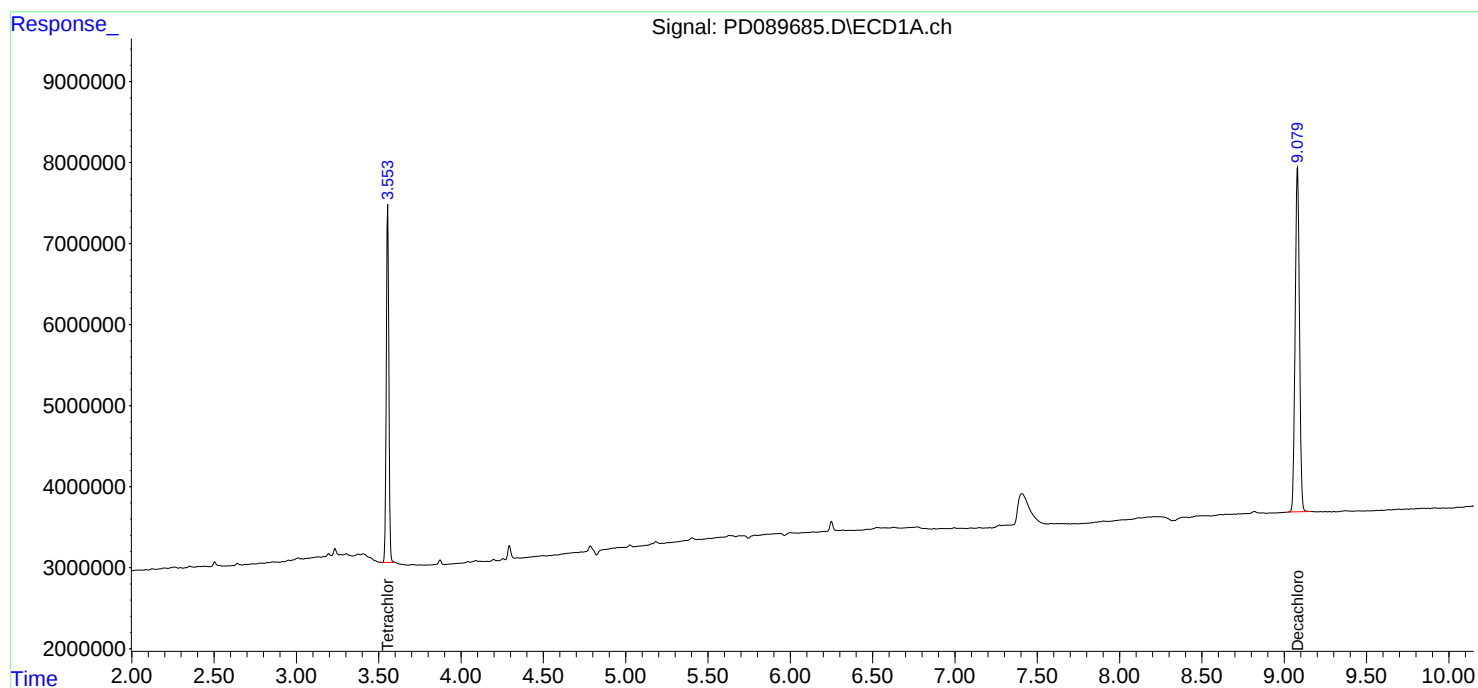


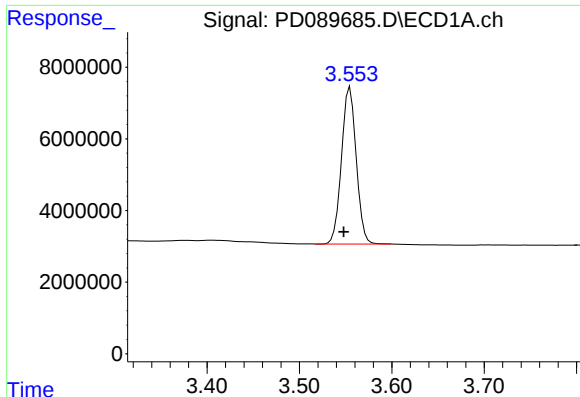

#1 Tetrachloro-m-xylene


R.T.: 3.555 min
Delta R.T.: 0.007 min
Response: 48438502
Conc: 19.64 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

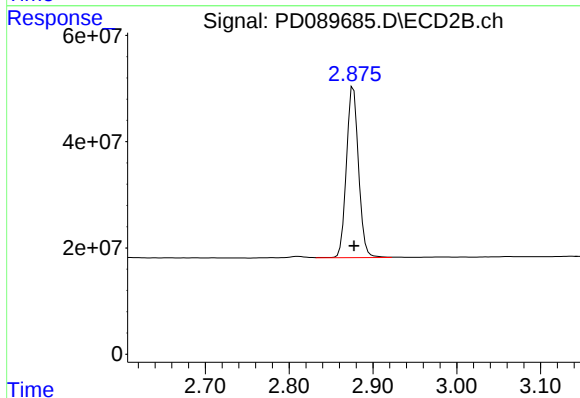


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 323764927
Conc: 20.44 ng/ml

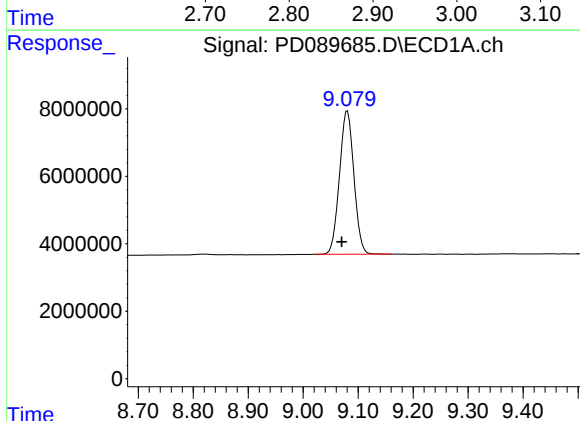

#28 Decachlorobiphenyl

R.T.: 9.080 min
Delta R.T.: 0.010 min
Response: 77499630
Conc: 20.85 ng/ml

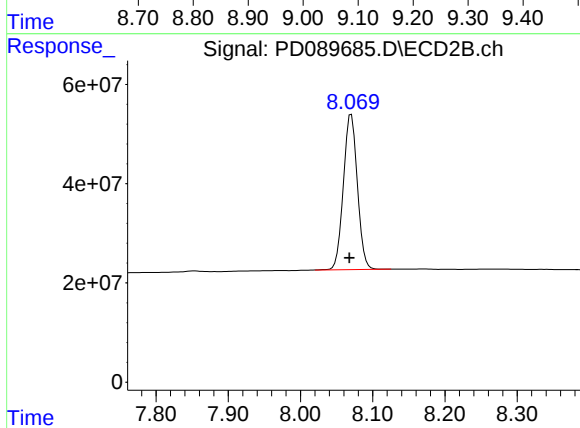

#28 Decachlorobiphenyl

R.T.: 8.070 min
Delta R.T.: 0.003 min
Response: 419071996
Conc: 20.87 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/08/25
Project:	Girard school	Date Received:	08/08/25
Client Sample ID:	PIBLK-PD089808.D	SDG No.:	Q2795
Lab Sample ID:	I.BLK-PD089808.D	Matrix:	WATER
Analytical Method:	8081B	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089808.D	1		08/08/25	pd080925

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
309-00-2	Aldrin	0.0036	U	0.0036	0.050	ug/L
60-57-1	Dieldrin	0.0036	U	0.0036	0.050	ug/L
72-55-9	4,4-DDE	0.0037	U	0.0037	0.050	ug/L
72-54-8	4,4-DDD	0.0071	U	0.0071	0.050	ug/L
50-29-3	4,4-DDT	0.0035	U	0.0035	0.050	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	23.2		57 - 171	116%	SPK: 20
877-09-8	Tetrachloro-m-xylene	26.1		61 - 148	130%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 10:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:33:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.548	2.877	56530727	413.2E6	22.919	26.087
28)	SA Decachlor...	9.068	8.066	86140219	417.6E6	23.179	20.800

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089808.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 10:57
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:33:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

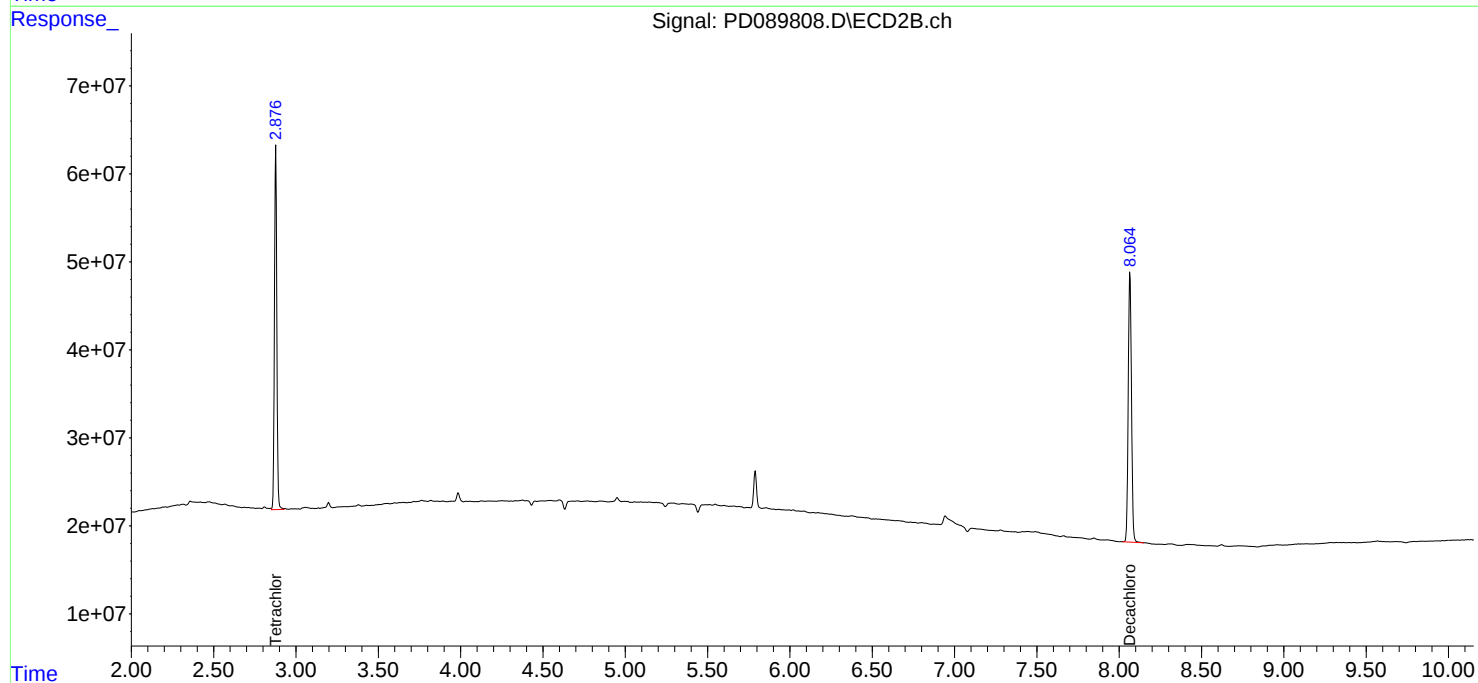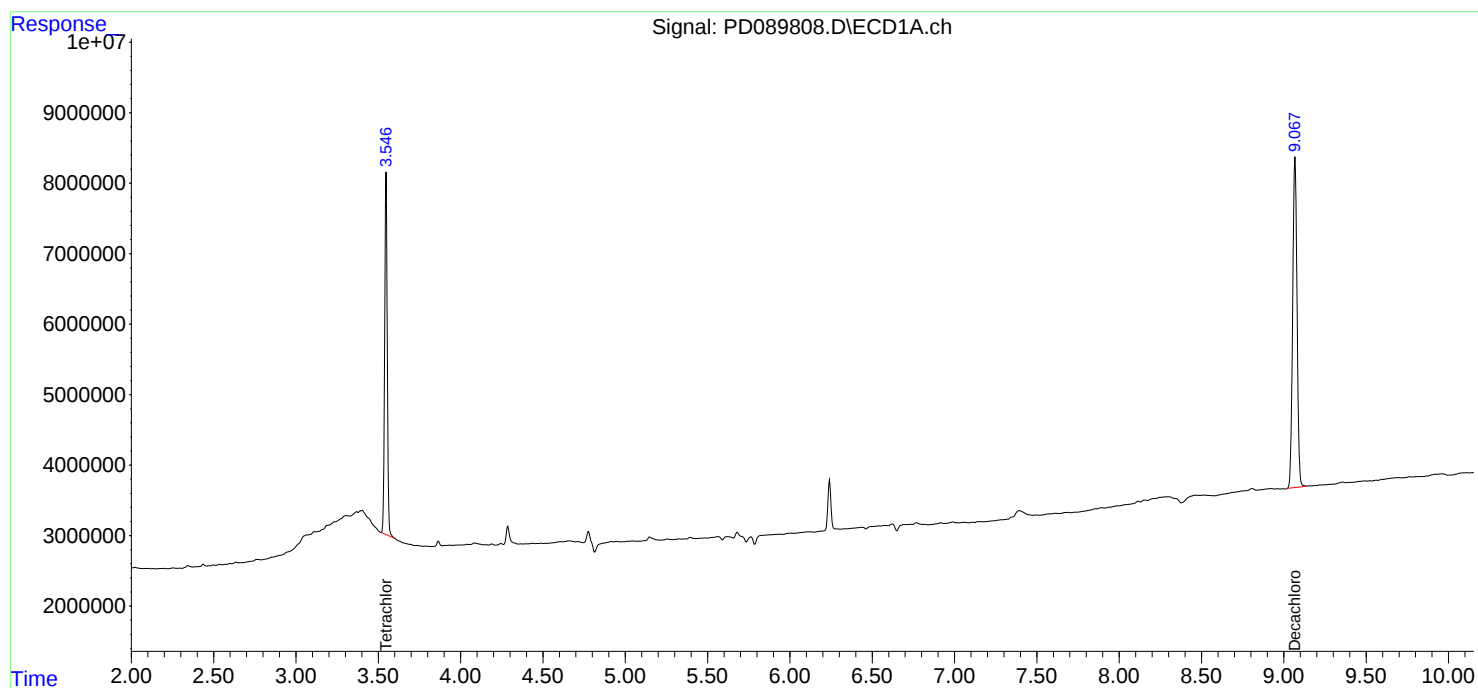


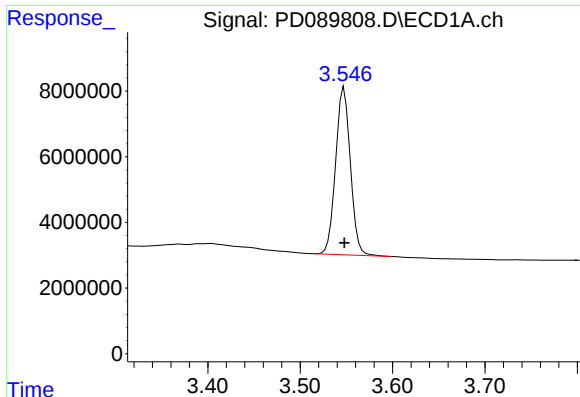

#1 Tetrachloro-m-xylene


R.T.: 3.548 min
Delta R.T.: 0.000 min
Response: 56530727
Conc: 22.92 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

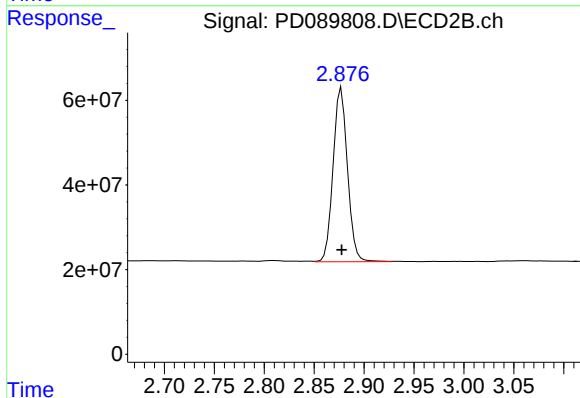


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 413159495
Conc: 26.09 ng/ml

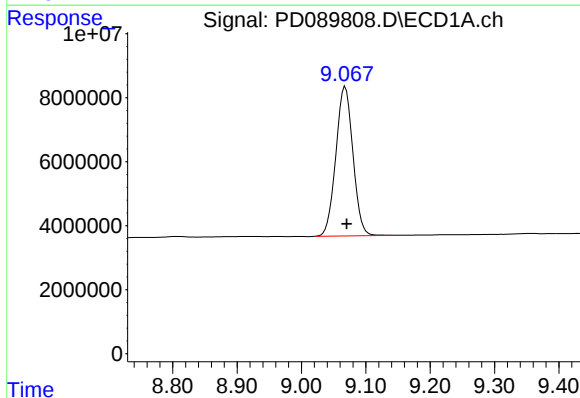

#28 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: -0.003 min
Response: 86140219
Conc: 23.18 ng/ml

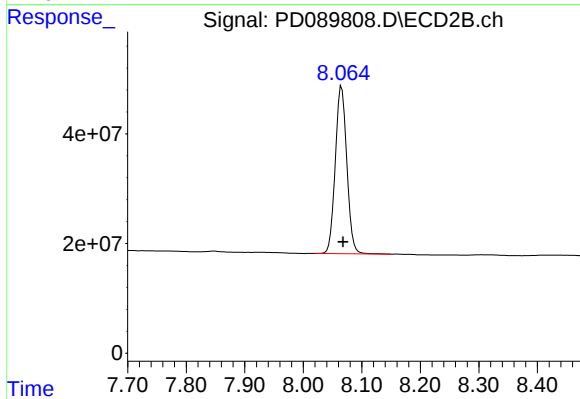

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 417613146
Conc: 20.80 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/08/25
Project:	Girard school	Date Received:	08/08/25
Client Sample ID:	PIBLK-PD089820.D	SDG No.:	Q2795
Lab Sample ID:	I.BLK-PD089820.D	Matrix:	WATER
Analytical Method:	8081B	% Solid:	0
Sample Wt/Vol:	1000	Units:	mL
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PESTICIDE Group1
GPC Factor :	1.0	PH :	
Prep Method :	3510C	Injection Volume :	

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089820.D	1		08/08/25	pd080925

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
309-00-2	Aldrin	0.0036	U	0.0036	0.050	ug/L
60-57-1	Dieldrin	0.0036	U	0.0036	0.050	ug/L
72-55-9	4,4-DDE	0.0037	U	0.0037	0.050	ug/L
72-54-8	4,4-DDD	0.0071	U	0.0071	0.050	ug/L
50-29-3	4,4-DDT	0.0035	U	0.0035	0.050	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	22.2		57 - 171	111%	SPK: 20
877-09-8	Tetrachloro-m-xylene	26.1		61 - 148	131%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 17:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:35:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.877	55104319	413.5E6	22.340	26.106
28)	SA Decachlor...	9.067	8.066	78753451	446.6E6	21.192	22.241

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089820.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 17:29
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:35:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

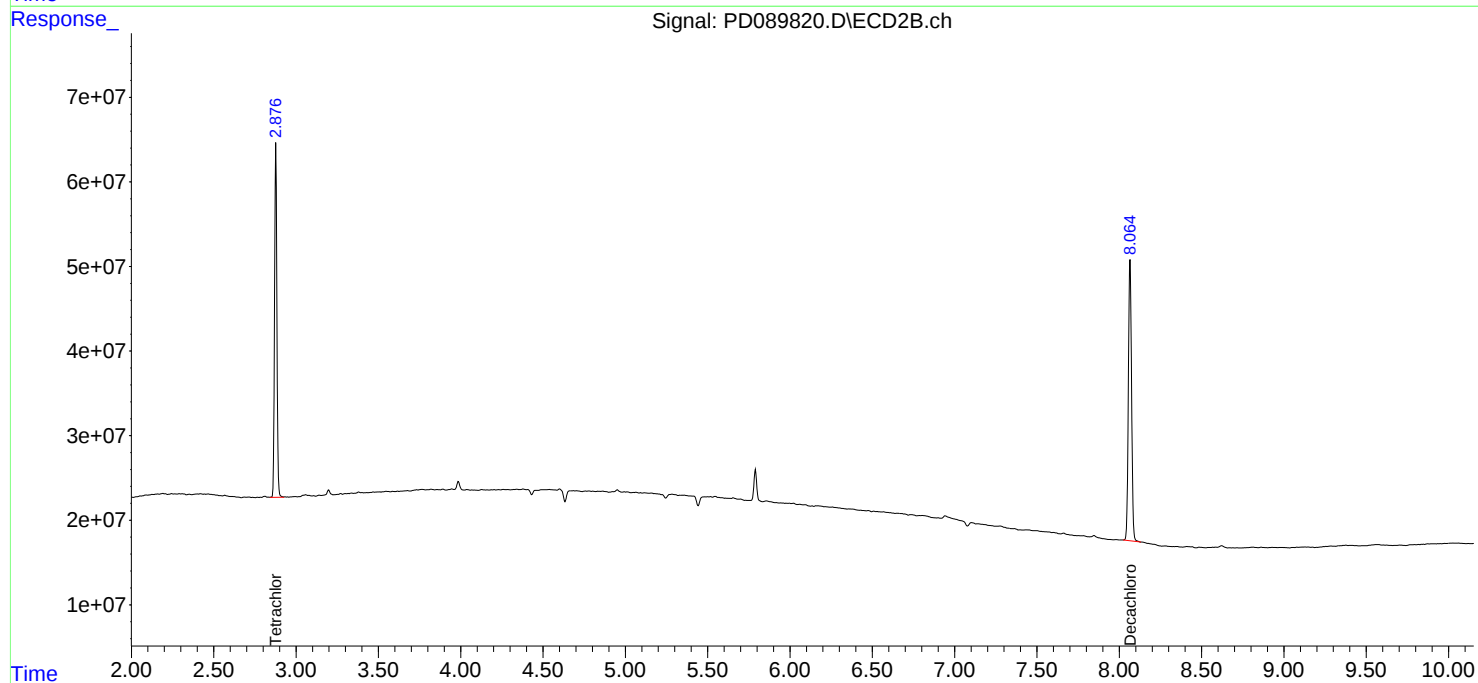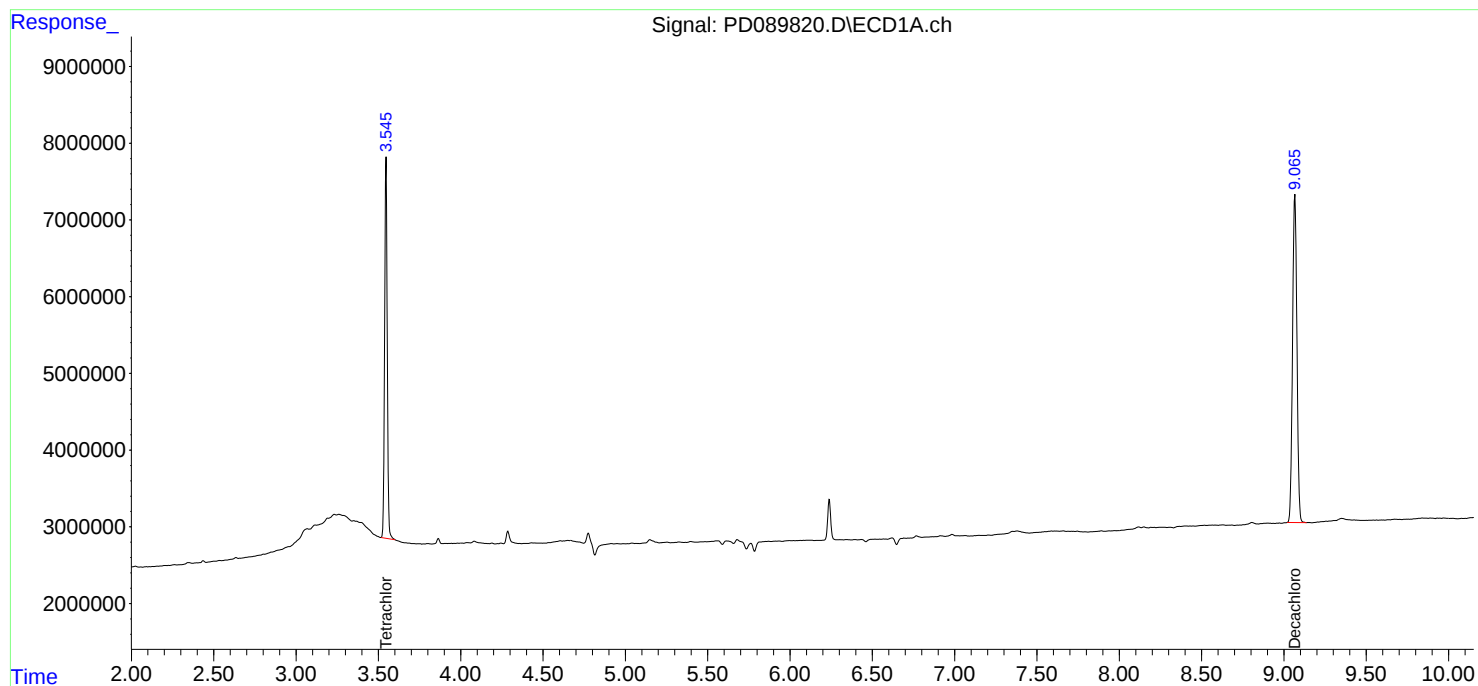


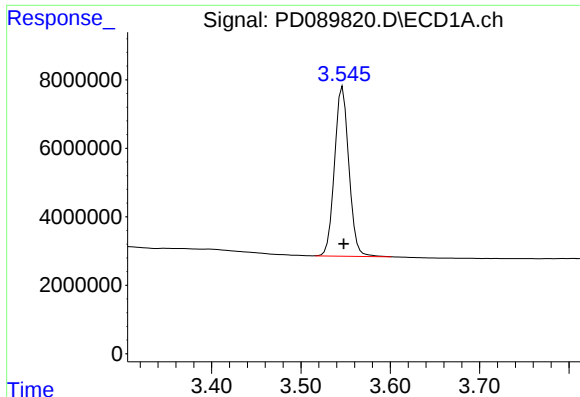

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: -0.001 min
Response: 55104319
Conc: 22.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

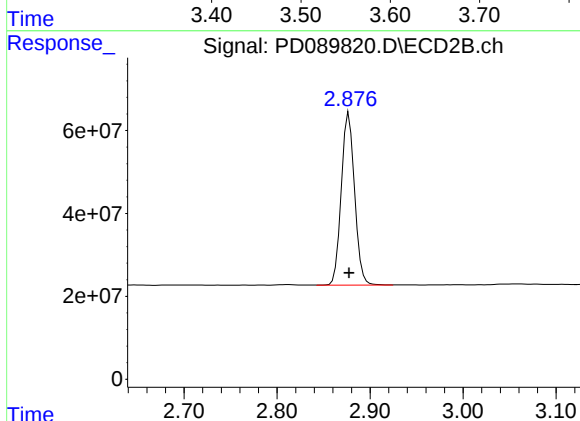


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 413468269
Conc: 26.11 ng/ml

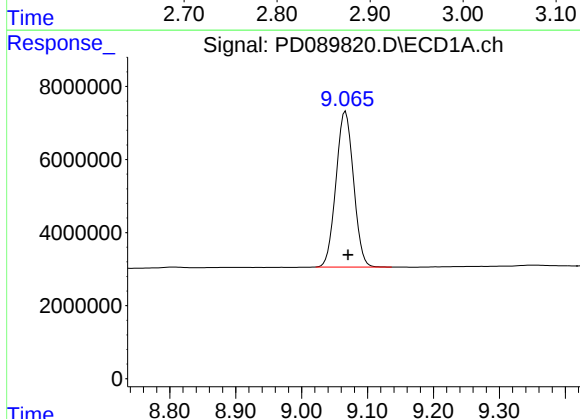

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: -0.004 min
Response: 78753451
Conc: 21.19 ng/ml

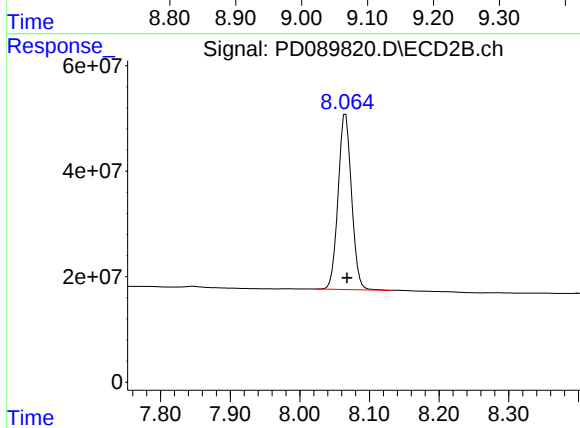

#28 Decachlorobiphenyl

R.T.: 8.066 min
Delta R.T.: -0.002 min
Response: 446559177
Conc: 22.24 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/08/25
Project:	Girard school	Date Received:	08/08/25
Client Sample ID:	PIBLK-PD089828.D	SDG No.:	Q2795
Lab Sample ID:	I.BLK-PD089828.D	Matrix:	WATER
Analytical Method:	8081B	% Solid:	0 Decanted:
Sample Wt/Vol:	1000 Units: mL	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	3510C		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089828.D	1		08/08/25	pd080925

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units
TARGETS						
309-00-2	Aldrin	0.0036	U	0.0036	0.050	ug/L
60-57-1	Dieldrin	0.0036	U	0.0036	0.050	ug/L
72-55-9	4,4-DDE	0.0037	U	0.0037	0.050	ug/L
72-54-8	4,4-DDD	0.0071	U	0.0071	0.050	ug/L
50-29-3	4,4-DDT	0.0035	U	0.0035	0.050	ug/L
SURROGATES						
2051-24-3	Decachlorobiphenyl	21.1		57 - 171	106%	SPK: 20
877-09-8	Tetrachloro-m-xylene	26.6		61 - 148	133%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 19:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:36:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.878	55427261	421.0E6	22.471	26.582
28)	SA Decachlor...	9.066	8.065	77885689	424.6E6	20.958	21.148

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089828.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 19:32
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:36:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

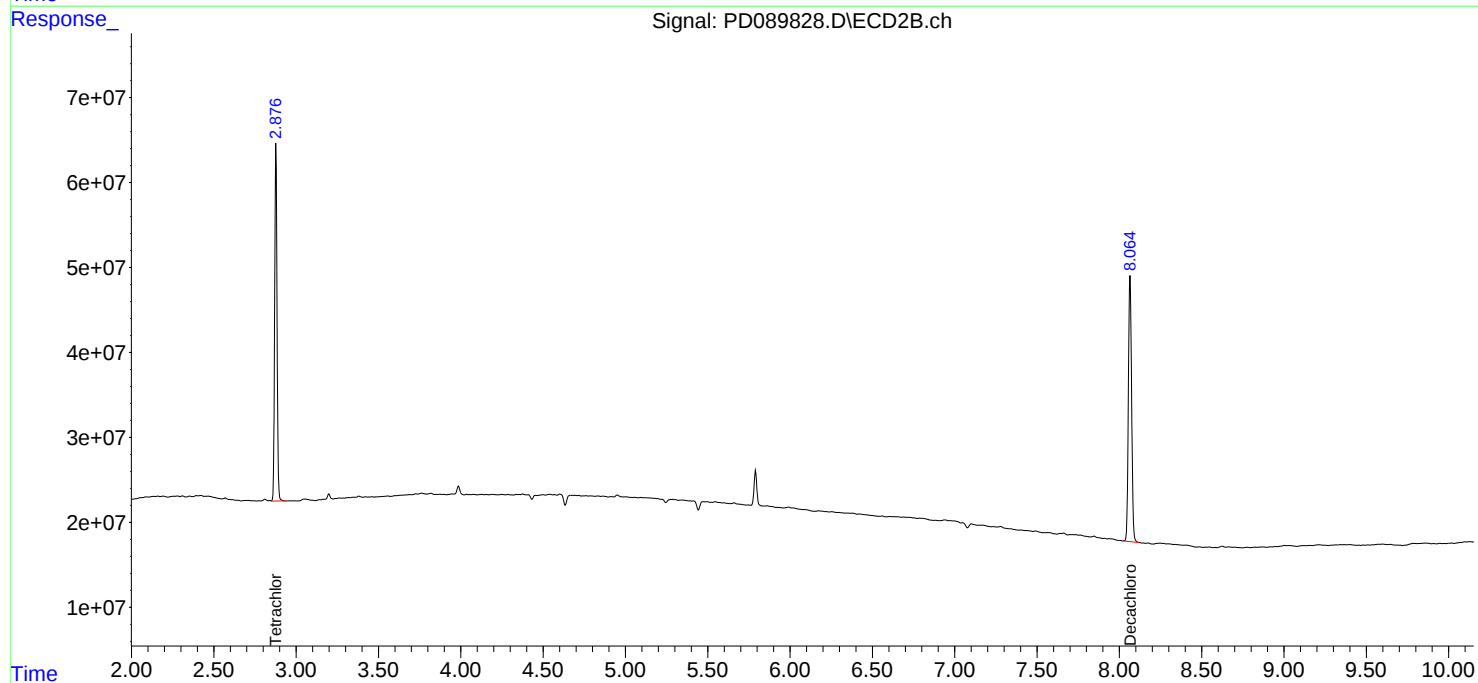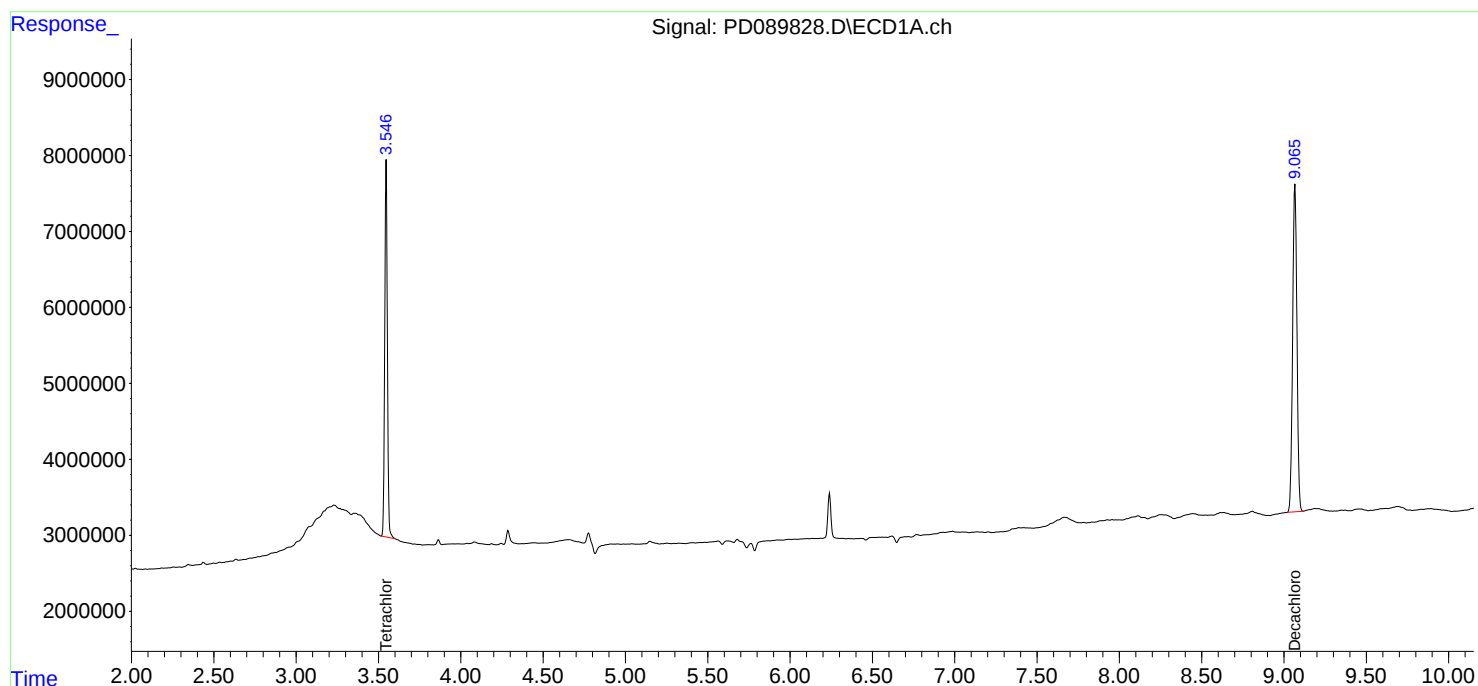


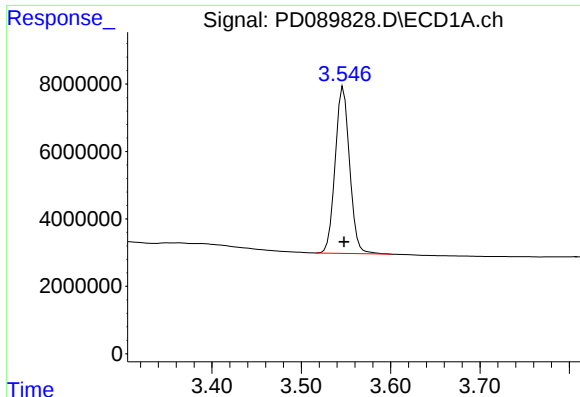

#1 Tetrachloro-m-xylene


R.T.: 3.547 min
Delta R.T.: 0.000 min
Response: 55427261
Conc: 22.47 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

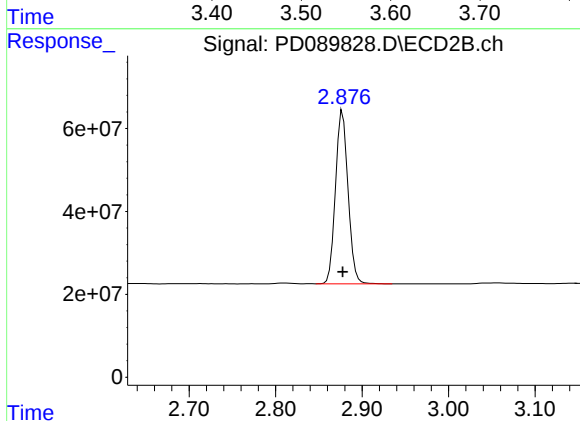


#1 Tetrachloro-m-xylene

R.T.: 2.878 min
Delta R.T.: 0.000 min
Response: 421007889
Conc: 26.58 ng/ml

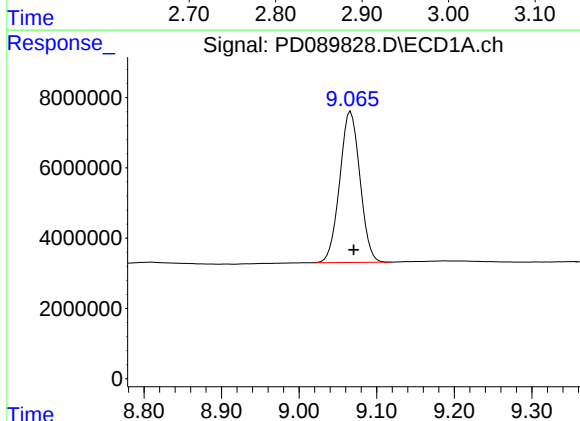

#28 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: -0.004 min
Response: 77885689
Conc: 20.96 ng/ml

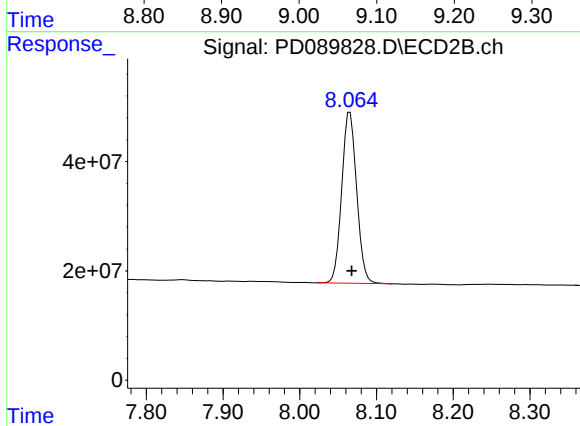

#28 Decachlorobiphenyl

R.T.: 8.065 min
Delta R.T.: -0.003 min
Response: 424600809
Conc: 21.15 ng/ml

Report of Analysis

Client:	Kleinfelder	Date Collected:	
Project:	Girard school	Date Received:	
Client Sample ID:	PB169173BS	SDG No.:	Q2795
Lab Sample ID:	PB169173BS	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	100 Decanted:
Sample Wt/Vol:	30.01 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089812.D	1	08/08/25 08:43	08/08/25 15:18	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	17.7		0.12	1.70	ug/kg
60-57-1	Dieldrin	17.6		0.14	1.70	ug/kg
72-55-9	4,4-DDE	17.7		0.14	1.70	ug/kg
72-54-8	4,4-DDD	18.5		0.15	1.70	ug/kg
50-29-3	4,4-DDT	16.4		0.14	1.70	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	19.5		20 - 144	98%	SPK: 20
877-09-8	Tetrachloro-m-xylene	22.2		19 - 148	111%	SPK: 20

Comments:

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 E = Value Exceeds Calibration Range
 P = Indicates >25% difference for detected concentrations between the two GC columns
 Q = indicates LCS control criteria did not meet requirements
 M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 N = Presumptive Evidence of a Compound
 * = Values outside of QC limits
 D = Dilution
 S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.
 () = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089812.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 15:18
 Operator : AR\AJ
 Sample : PB169173BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PB169173BS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:34:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.554	2.877	45600905	352.1E6	18.487	22.232
28)	SA Decachlor...	9.076	8.067	69294723	391.5E6	18.646	19.498
Target Compounds							
2)	A alpha-BHC	4.004	3.389	241.8E6	1294.6E6	48.806	53.265
3)	MA gamma-BHC...	4.335	3.726	229.3E6	1197.3E6	48.257	53.156
4)	MA Heptachlor	4.933	4.079	223.2E6	1182.8E6	46.389	50.962
5)	MB Aldrin	5.275	4.364	219.7E6	1185.1E6	48.134	53.260
6)	B beta-BHC	4.521	4.022	88040092	509.3E6	47.727	52.778
7)	B delta-BHC	4.768	4.258	227.6E6	1209.1E6	49.617m	53.228
8)	B Heptachlo...	5.695	4.868	197.2E6	1073.8E6	47.160	52.255
9)	A Endosulfan I	6.079	5.242	184.6E6	1022.3E6	46.571	52.298
10)	B gamma-Chl...	5.951	5.121	197.7E6	1153.4E6	47.316	53.269
11)	B alpha-Chl...	6.032	5.186	195.9E6	1105.1E6	46.608	53.073
12)	B 4,4'-DDE	6.201	5.370	174.2E6	1119.9E6	46.702	52.984
13)	MA Dieldrin	6.352	5.508	196.4E6	1140.4E6	46.507	52.700
14)	MA Endrin	6.579	5.785	151.9E6	963.6E6	42.460	48.361
15)	B Endosulfa...	6.791	6.077	165.9E6	987.0E6	45.203	52.500
16)	A 4,4'-DDD	6.710	5.925	143.0E6	978.5E6	47.756	55.492
17)	MA 4,4'-DDT	7.026	6.179	139.1E6	905.4E6	41.387	49.280
18)	B Endrin al...	6.920	6.255	128.0E6	761.2E6	51.290	58.912
19)	B Endosulfa...	7.155	6.478	155.1E6	952.4E6	44.701	51.301
20)	A Methoxychlor	7.499	6.750	69997285	454.8E6	39.149	46.428
21)	B Endrin ke...	7.635	6.988	164.2E6	1046.9E6	44.219	52.165
22)	Mirex	8.117	7.181	114.8E6	739.7E6	41.188	48.599

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089812.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 15:18
Operator : AR\AJ
Sample : PB169173BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

PB169173BS

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 08/11/2025

Supervised By :mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:34:09 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

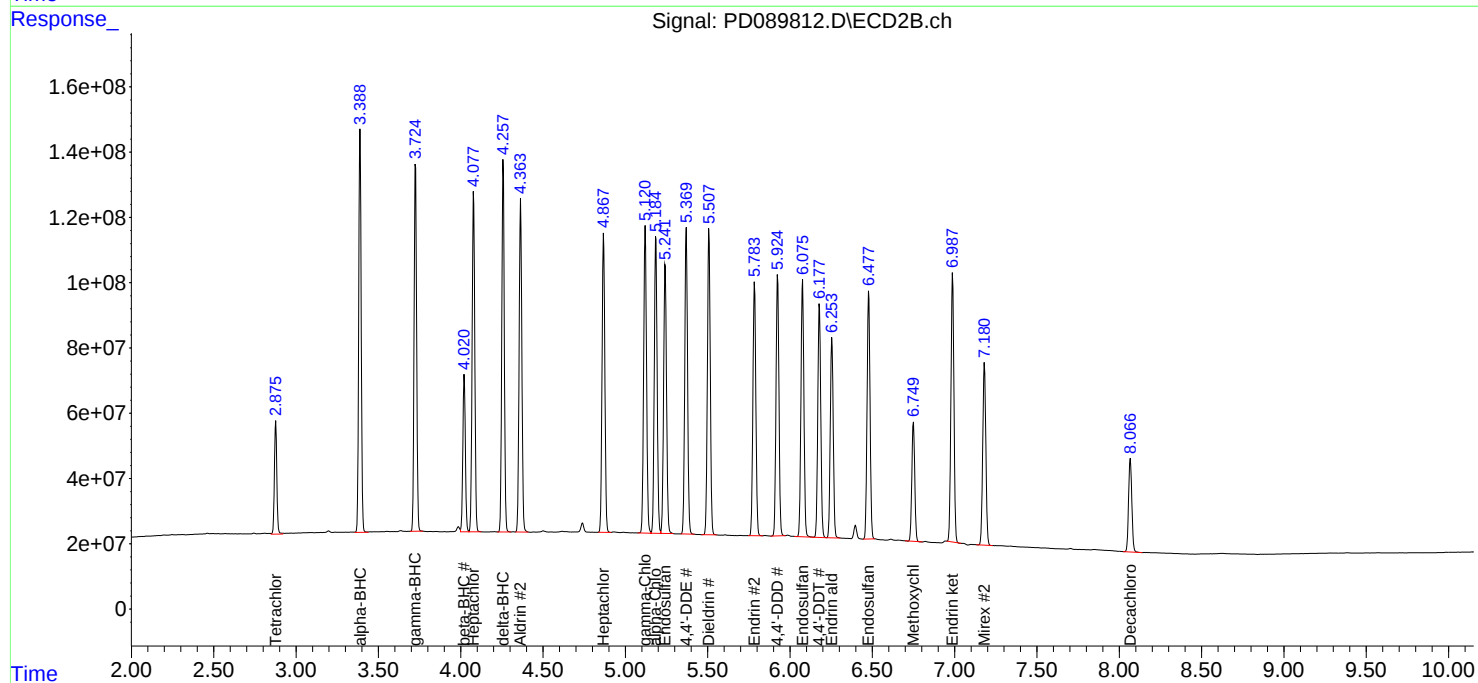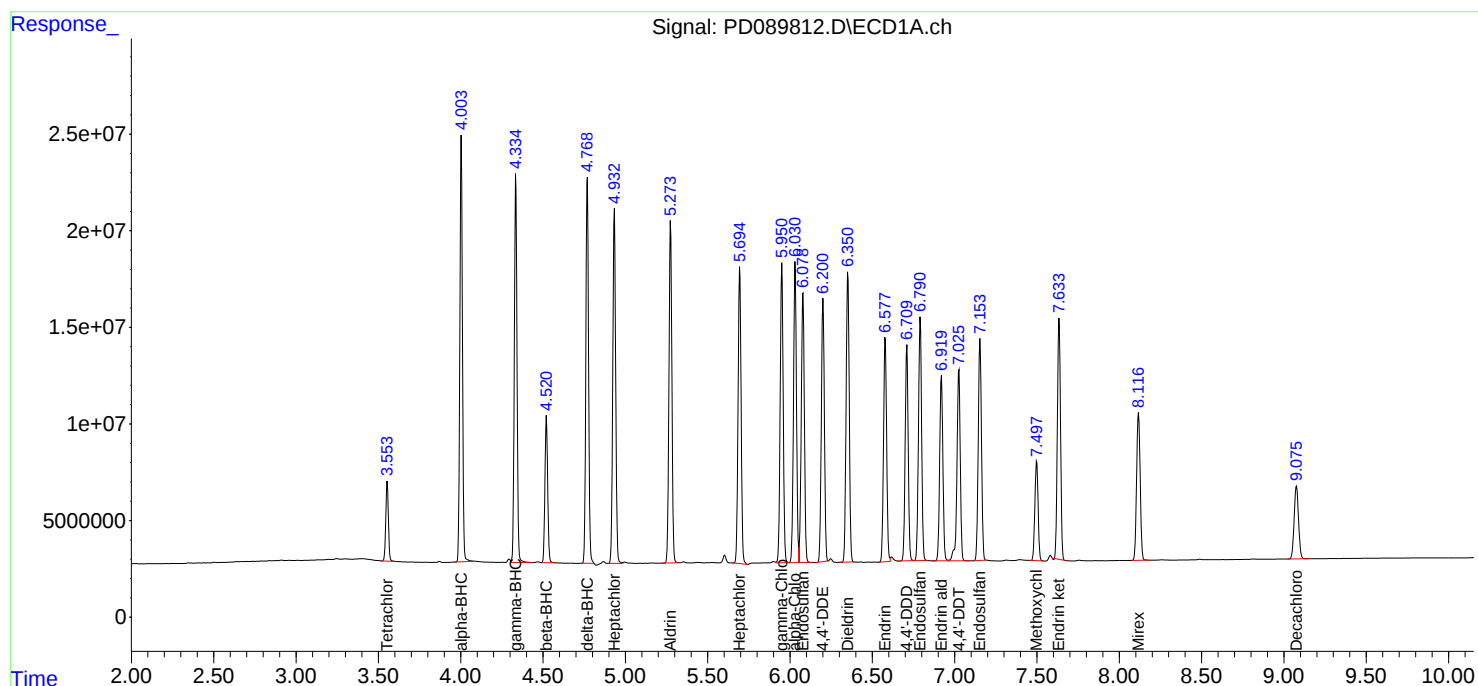

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/06/25
Project:	Girard school	Date Received:	08/07/25
Client Sample ID:	COMP-1MS	SDG No.:	Q2795
Lab Sample ID:	Q2795-01MS	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	82.5
Sample Wt/Vol:	30.06	Units:	g
Soil Aliquot Vol:			uL
Extraction Type:		Test:	PESTICIDE Group1
GPC Factor :	1.0	Injection Volume :	
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089823.D	1	08/08/25 08:43	08/08/25 18:24	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	22.6		0.15	2.10	ug/kg
60-57-1	Dieldrin	20.9		0.17	2.10	ug/kg
72-55-9	4,4-DDE	22.5		0.17	2.10	ug/kg
72-54-8	4,4-DDD	22.1		0.18	2.10	ug/kg
50-29-3	4,4-DDT	18.1		0.17	2.10	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	13.4		20 - 144	67%	SPK: 20
877-09-8	Tetrachloro-m-xylene	19.2		19 - 148	96%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089823.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 18:24
 Operator : AR\AJ
 Sample : Q2795-01MS
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 COMP-1MS

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 08/11/2025
 Supervised By : mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:35:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.876	40109693	304.0E6	16.261	19.195m
28)	SA Decachlor...	9.066	8.066	47615523	268.4E6	12.813	13.368
Target Compounds							
2)	A alpha-BHC	3.996	3.388	253.2E6	1368.4E6	51.120	56.303m
3)	MA gamma-BHC...	4.327	3.726	251.8E6	1253.8E6	52.988	55.664
4)	MA Heptachlor	4.926	4.079	210.2E6	1161.0E6	43.684	50.023
5)	MB Aldrin	5.267	4.364	228.8E6	1248.3E6	50.127	56.100
6)	B beta-BHC	4.513	4.022	90529851	564.6E6	49.076	58.519
7)	B delta-BHC	4.762	4.258	251.2E6	1272.2E6	54.778	56.007
8)	B Heptachlo...	5.687	4.868	199.2E6	1123.4E6	47.656	54.668
9)	A Endosulfan I	6.070	5.242	179.5E6	968.4E6	45.298	49.538
10)	B gamma-Chl...	5.942	5.120	201.8E6	1232.6E6	48.298	56.926
11)	B alpha-Chl...	6.023	5.185	201.8E6	1165.0E6	47.996	55.949
12)	B 4,4'-DDE	6.192	5.370	177.3E6	1179.7E6	47.546	55.812
13)	MA Dieldrin	6.343	5.507	184.3E6	1119.3E6	43.638	51.726
14)	MA Endrin	6.571	5.784	140.9E6	946.2E6	39.391	47.486
15)	B Endosulfa...	6.782	6.074	154.3E6	949.0E6	42.045	50.481m
16)	A 4,4'-DDD	6.702	5.924	146.5E6	967.1E6	48.918	54.847
17)	MA 4,4'-DDT	7.017	6.178	115.0E6	825.3E6	34.235	44.918 #
18)	B Endrin al...	6.911	6.254	107.1E6	686.5E6	42.902	53.137
19)	B Endosulfa...	7.146	6.477	141.4E6	874.1E6	40.756	47.084
20)	A Methoxychlor	7.489	6.748	53887836	377.1E6	30.139	38.493 #
21)	B Endrin ke...	7.626	6.985	143.2E6	914.2E6	38.560	45.555
22)	Mirex	8.109	7.179	115.6E6	782.0E6	41.461	51.374

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089823.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 18:24
Operator : AR\AJ
Sample : Q2795-01MS
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

COMP-1MS

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 08/11/2025

Supervised By :mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:35:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

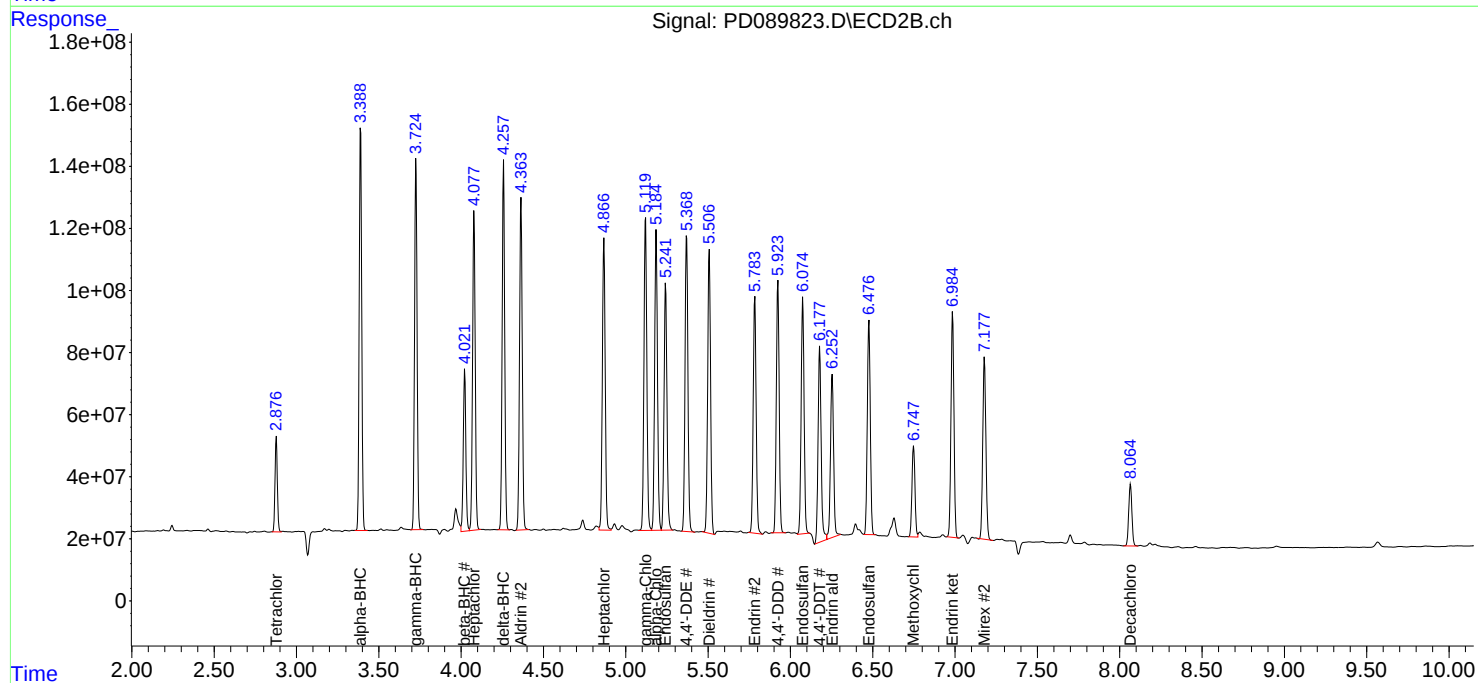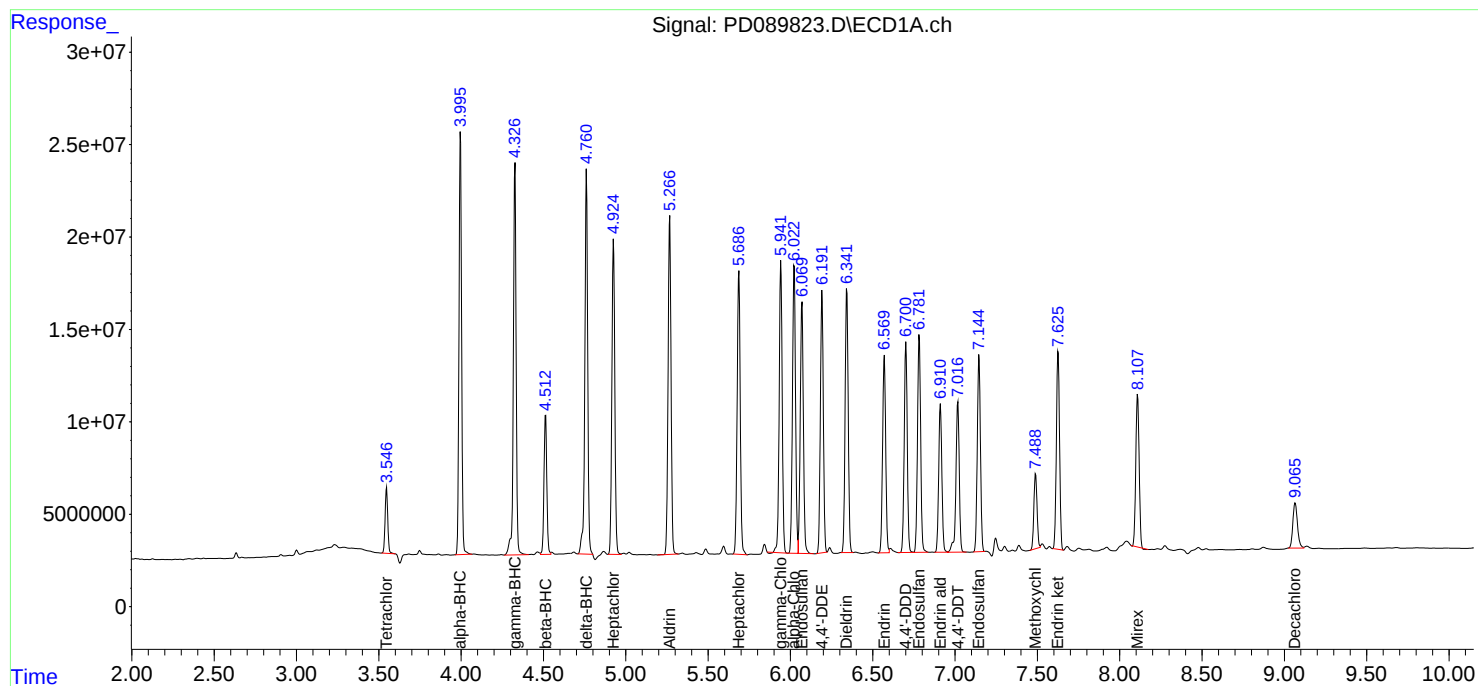

Report of Analysis

Client:	Kleinfelder	Date Collected:	08/06/25
Project:	Girard school	Date Received:	08/07/25
Client Sample ID:	COMP-1MSD	SDG No.:	Q2795
Lab Sample ID:	Q2795-01MSD	Matrix:	SOIL
Analytical Method:	8081B	% Solid:	82.5 Decanted:
Sample Wt/Vol:	30.04 Units: g	Final Vol:	10000 uL
Soil Aliquot Vol:	uL	Test:	PESTICIDE Group1
Extraction Type:		Injection Volume :	
GPC Factor :	1.0 PH :		
Prep Method :	SW3541B		

File ID/Qc Batch:	Dilution:	Prep Date	Date Analyzed	Prep Batch ID
PD089824.D	1	08/08/25 08:43	08/08/25 18:37	PB169173

CAS Number	Parameter	Conc.	Qualifier	MDL	LOQ / CRQL	Units(Dry Weight)
TARGETS						
309-00-2	Aldrin	22.6		0.15	2.10	ug/kg
60-57-1	Dieldrin	21.9		0.17	2.10	ug/kg
72-55-9	4,4-DDE	22.3		0.17	2.10	ug/kg
72-54-8	4,4-DDD	22.0		0.18	2.10	ug/kg
50-29-3	4,4-DDT	19.7		0.17	2.10	ug/kg
SURROGATES						
2051-24-3	Decachlorobiphenyl	13.2		20 - 144	66%	SPK: 20
877-09-8	Tetrachloro-m-xylene	19.2		19 - 148	96%	SPK: 20

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
 Data File : PD089824.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Aug 2025 18:37
 Operator : AR\AJ
 Sample : Q2795-01MSD
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

COMP-1MSD

Manual Integrations

APPROVED

Reviewed By :Abdul Mirza 08/11/2025

Supervised By :mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 11 01:36:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
 Quant Title : GC Extractables
 QLast Update : Fri Aug 01 07:03:58 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.547	2.876	39857997	304.5E6	16.159	19.227m
28)	SA Decachlor...	9.067	8.066	47848826	264.0E6	12.876	13.147
Target Compounds							
2)	A alpha-BHC	3.996	3.389	252.6E6	1374.0E6	50.993	56.530m
3)	MA gamma-BHC...	4.327	3.726	251.1E6	1260.7E6	52.831	55.973
4)	MA Heptachlor	4.926	4.079	217.5E6	1203.1E6	45.198	51.836
5)	MB Aldrin	5.267	4.364	227.1E6	1247.4E6	49.750	56.061
6)	B beta-BHC	4.514	4.022	89708718	563.4E6	48.631	58.389
7)	B delta-BHC	4.762	4.258	239.8E6	1273.8E6	52.287	56.078
8)	B Heptachlo...	5.687	4.868	200.4E6	1127.3E6	47.934	54.855
9)	A Endosulfan I	6.071	5.243	188.6E6	1008.7E6	47.577	51.599
10)	B gamma-Chl...	5.943	5.119	200.1E6	1210.5E6	47.870	55.904m
11)	B alpha-Chl...	6.023	5.185	200.9E6	1157.0E6	47.783	55.568
12)	B 4,4'-DDE	6.193	5.370	180.7E6	1165.9E6	48.441	55.160
13)	MA Dieldrin	6.343	5.508	195.4E6	1175.5E6	46.275	54.322
14)	MA Endrin	6.570	5.784	157.9E6	1029.4E6	44.136	51.661
15)	B Endosulfa...	6.783	6.074	163.3E6	1004.6E6	44.514	53.435m
16)	A 4,4'-DDD	6.701	5.925	147.7E6	960.5E6	49.333	54.476
17)	MA 4,4'-DDT	7.017	6.178	129.0E6	898.7E6	38.391	48.914 #
18)	B Endrin al...	6.911	6.254	120.2E6	754.1E6	48.160	58.364
19)	B Endosulfa...	7.146	6.477	151.8E6	934.5E6	43.757	50.335
20)	A Methoxychlor	7.490	6.749	62877452	426.5E6	35.167	43.545
21)	B Endrin ke...	7.627	6.986	158.0E6	986.6E6	42.545	49.164
22)	Mirex	8.109	7.180	116.4E6	775.7E6	41.729	50.963

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD080925\
Data File : PD089824.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Aug 2025 18:37
Operator : AR\AJ
Sample : Q2795-01MSD
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :

ECD_D

ClientSampleId :

COMP-1MSD

Manual Integrations



APPROVED

Reviewed By :Abdul Mirza 08/11/2025

Supervised By :mohammad ahmed 08/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 11 01:36:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD073125.M
Quant Title : GC Extractables
QLast Update : Fri Aug 01 07:03:58 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

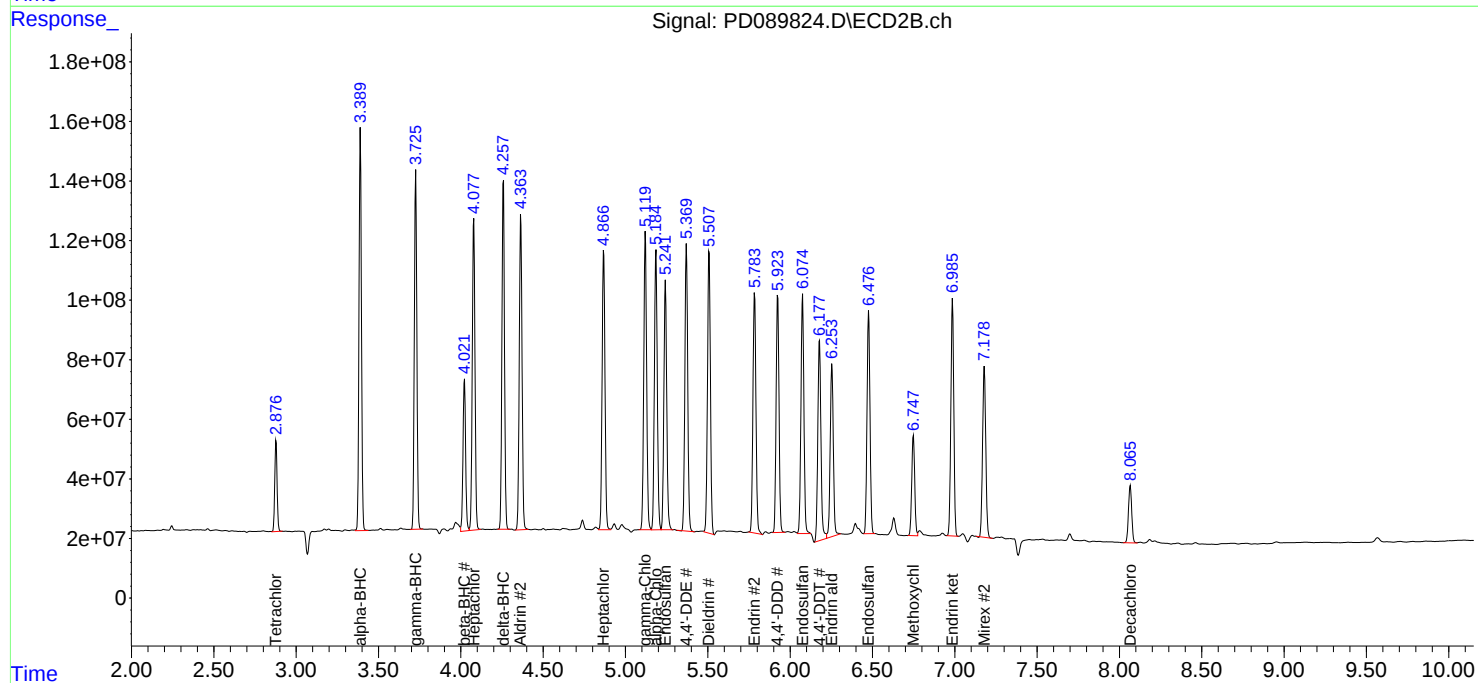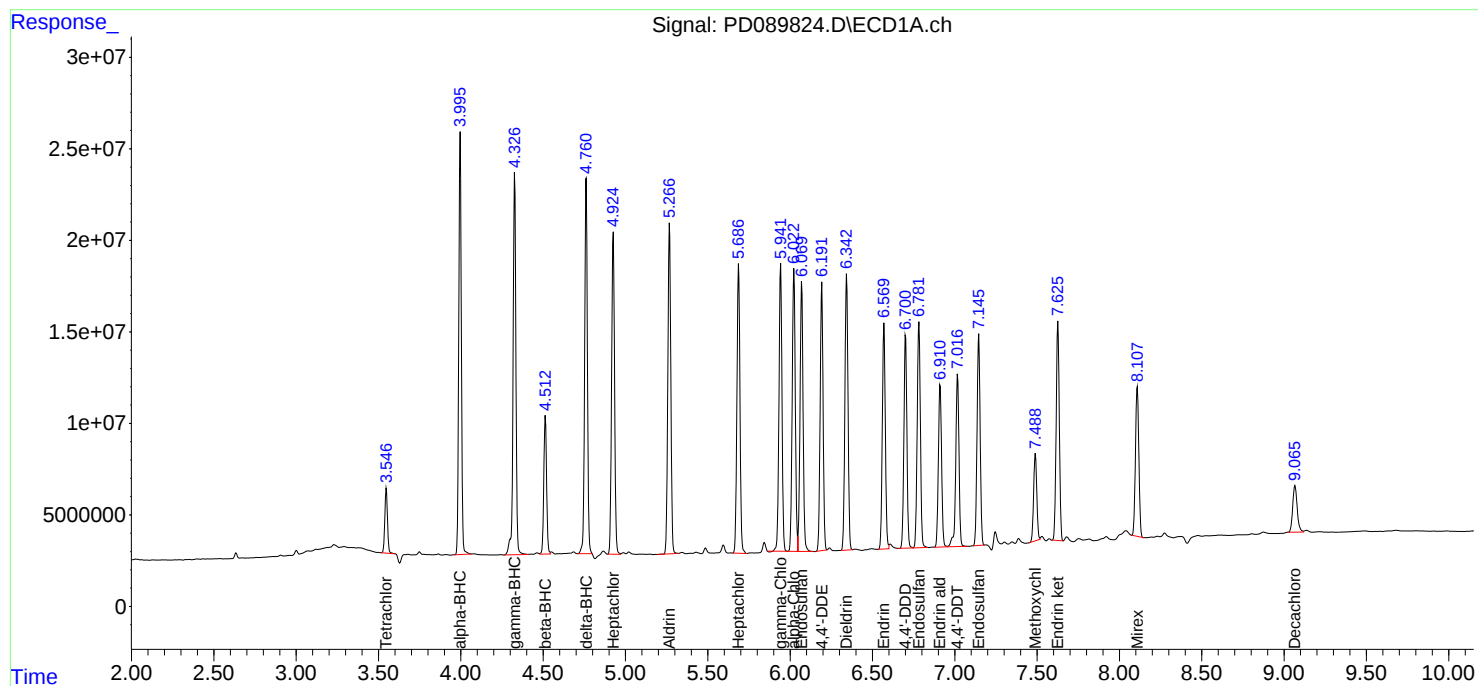

Manual Integration Report

Sequence:

pd073125

Instrument

ECD_d

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PEM	PD089686.D	4,4"-DDD #2	Abdul	8/1/2025 9:25:47 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PEM	PD089686.D	4,4"-DDE	Abdul	8/1/2025 9:25:47 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PEM	PD089686.D	4,4"-DDE #2	Abdul	8/1/2025 9:25:47 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PEM	PD089686.D	Endrin ketone	Abdul	8/1/2025 9:25:47 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PEM	PD089686.D	Endrin ketone #2	Abdul	8/1/2025 9:25:47 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PSTDICC075	PD089689.D	gamma-BHC (Lindane)	Abdul	8/1/2025 8:28:32 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PSTDICC005	PD089692.D	4,4"-DDE #2	Abdul	8/1/2025 8:28:35 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software
PSTDICC005	PD089692.D	Endrin aldehyde	Abdul	8/1/2025 8:28:35 AM	mohammad	8/1/2025 9:27:16	Peak Integrated by Software

Manual Integration Report

Sequence:	pd080925	Instrument	ECD_d
-----------	----------	------------	-------

Sample ID	File ID	Parameter	Review By	Review On	Supervised By	Supervised On	Reason
PEM	PD089809.D	4,4"-DDE	Abdul	8/11/2025 12:47:20 PM	 	 	Peak Integrated by Software
PB169173BS	PD089812.D	delta-BHC	Abdul	8/11/2025 12:47:38 PM	 	 	Peak Integrated by Software
Q2795-01	PD089822.D	Tetrachloro-m-xylene #2	Abdul	8/11/2025 12:47:58 PM	 	 	Peak Integrated by Software
Q2795-01MS	PD089823.D	alpha-BHC #2	Abdul	8/11/2025 12:48:02 PM	 	 	Peak Integrated by Software
Q2795-01MS	PD089823.D	Endosulfan II #2	Abdul	8/11/2025 12:48:02 PM	 	 	Peak Integrated by Software
Q2795-01MS	PD089823.D	Tetrachloro-m-xylene #2	Abdul	8/11/2025 12:48:02 PM	 	 	Peak Integrated by Software
Q2795-01MSD	PD089824.D	alpha-BHC #2	Abdul	8/11/2025 12:48:06 PM	 	 	Peak Integrated by Software
Q2795-01MSD	PD089824.D	Endosulfan II #2	Abdul	8/11/2025 12:48:06 PM	 	 	Peak Integrated by Software
Q2795-01MSD	PD089824.D	gamma-Chlordane #2	Abdul	8/11/2025 12:48:06 PM	 	 	Peak Integrated by Software
Q2795-01MSD	PD089824.D	Tetrachloro-m-xylene #2	Abdul	8/11/2025 12:48:06 PM	 	 	Peak Integrated by Software
Q2795-02	PD089825.D	Tetrachloro-m-xylene #2	Abdul	8/11/2025 12:48:38 PM	 	 	Peak Integrated by Software
Q2795-03	PD089826.D	Tetrachloro-m-xylene #2	Abdul	8/11/2025 12:48:28 PM	 	 	Peak Integrated by Software
PSTDCCC050	PD089829.D	4,4"-DDT	Abdul	8/11/2025 12:48:15 PM	 	 	Peak Integrated by Software



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

Manual Integration Report

Sequence:

pd080925

Instrument

ECD_d

Sample ID

File ID

Parameter

Review By

Review On

Supervised
By

Supervised On

Reason

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD073125

Review By	Abdul	Review On	8/1/2025 8:29:12 AM
Supervise By	mohammad	Supervise On	8/1/2025 9:27:16 AM
SubDirectory	PD073125	HP Acquire Method	HP Processing Method pd073125 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP24433,PP24651		
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,PP24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284		
CCC	PP24261,PP24273,PP24279,PP24284		
Internal Standard/PEM			
ICV/I.BLK	PP24273,PP24279,PP24284		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	Sampleld	Data File Name	Date-Time	Operator	Status
1	HEXANE	PD089684.D	31 Jul 2025 09:13	AR\AJ	Ok
2	I.BLK	PD089685.D	31 Jul 2025 10:33	AR\AJ	Ok
3	PEM	PD089686.D	31 Jul 2025 10:47	AR\AJ	Ok,M
4	RESCHK	PD089687.D	31 Jul 2025 11:34	AR\AJ	Ok
5	PSTDICC100	PD089688.D	31 Jul 2025 11:47	AR\AJ	Ok
6	PSTDICC075	PD089689.D	31 Jul 2025 12:01	AR\AJ	Ok,M
7	PSTDICC050	PD089690.D	31 Jul 2025 12:14	AR\AJ	Ok
8	PSTDICC025	PD089691.D	31 Jul 2025 12:28	AR\AJ	Ok
9	PSTDICC005	PD089692.D	31 Jul 2025 12:41	AR\AJ	Ok,M
10	PCHLORICC1000	PD089693.D	31 Jul 2025 12:56	AR\AJ	Ok
11	PCHLORICC750	PD089694.D	31 Jul 2025 13:09	AR\AJ	Ok
12	PCHLORICC500	PD089695.D	31 Jul 2025 13:23	AR\AJ	Ok
13	PCHLORICC250	PD089696.D	31 Jul 2025 13:36	AR\AJ	Ok
14	PCHLORICC050	PD089697.D	31 Jul 2025 13:50	AR\AJ	Ok
15	PTOXICC1000	PD089698.D	31 Jul 2025 14:03	AR\AJ	Ok
16	PTOXICC750	PD089699.D	31 Jul 2025 14:17	AR\AJ	Ok
17	PTOXICC500	PD089700.D	31 Jul 2025 14:31	AR\AJ	Ok
18	PTOXICC250	PD089701.D	31 Jul 2025 14:44	AR\AJ	Ok,M
19	PTOXICC100	PD089702.D	31 Jul 2025 14:58	AR\AJ	Ok,M
20	PSTDICV050	PD089703.D	31 Jul 2025 15:11	AR\AJ	Ok
21	PCHLORICV500	PD089704.D	31 Jul 2025 15:25	AR\AJ	Ok

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD073125

Review By	Abdul	Review On	8/1/2025 8:29:12 AM
Supervise By	mohammad	Supervise On	8/1/2025 9:27:16 AM
SubDirectory	PD073125	HP Acquire Method	HP Processing Method pd073125 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP24433,PP24651		
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,PP24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284		
CCC	PP24261,PP24273,PP24279,PP24284		
Internal Standard/PEM			
ICV/I.BLK	PP24273,PP24279,PP24284		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	PTOXICV500	PD089705.D	31 Jul 2025 15:39	AR\AJ	Ok
----	------------	------------	-------------------	-------	----

M : Manual Integration

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD080925

Review By	Abdul	Review On	8/11/2025 12:49:00 PM
Supervise By		Supervise On	
SubDirectory	PD080925	HP Acquire Method	HP Processing Method pd073125 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP24433,PP24651		
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,PP24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284		
CCC	PP24261,PP24273,PP24279,PP24284		
Internal Standard/PEM			
ICV/I.BLK	PP24273,PP24279,PP24284		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

Sr#	SampleId	Data File Name	Date-Time	Operator	Status
1	HEXANE	PD089807.D	08 Aug 2025 10:43	AR\AJ	Ok
2	I.BLK	PD089808.D	08 Aug 2025 10:57	AR\AJ	Ok
3	PEM	PD089809.D	08 Aug 2025 11:10	AR\AJ	Ok,NS
4	PSTDCCC050	PD089810.D	08 Aug 2025 13:53	AR\AJ	Ok
5	PB169173BL	PD089811.D	08 Aug 2025 14:51	AR\AJ	Ok
6	PB169173BS	PD089812.D	08 Aug 2025 15:18	AR\AJ	Ok,NS
7	Q2793-01	PD089813.D	08 Aug 2025 15:55	AR\AJ	Ok,NS
8	Q2800-01	PD089814.D	08 Aug 2025 16:08	AR\AJ	Ok,NS
9	Q2801-01	PD089815.D	08 Aug 2025 16:22	AR\AJ	Ok,NS
10	Q2759-04	PD089816.D	08 Aug 2025 16:35	AR\AJ	Not Ok
11	PB169174BL	PD089817.D	08 Aug 2025 16:49	AR\AJ	Ok
12	PB169174BS	PD089818.D	08 Aug 2025 17:02	AR\AJ	Not Ok
13	PB169174BSD	PD089819.D	08 Aug 2025 17:16	AR\AJ	Not Ok
14	I.BLK	PD089820.D	08 Aug 2025 17:29	AR\AJ	Ok
15	PSTDCCC050	PD089821.D	08 Aug 2025 17:43	AR\AJ	Ok
16	Q2795-01	PD089822.D	08 Aug 2025 18:10	AR\AJ	Ok,NS
17	Q2795-01MS	PD089823.D	08 Aug 2025 18:24	AR\AJ	Ok,NS
18	Q2795-01MSD	PD089824.D	08 Aug 2025 18:37	AR\AJ	Ok,NS
19	Q2795-02	PD089825.D	08 Aug 2025 18:51	AR\AJ	Ok,NS
20	Q2795-03	PD089826.D	08 Aug 2025 19:05	AR\AJ	Ok,NS
21	Q2798-01	PD089827.D	08 Aug 2025 19:18	AR\AJ	Ok,NS

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD080925

Review By	Abdul	Review On	8/11/2025 12:49:00 PM
Supervise By		Supervise On	
SubDirectory	PD080925	HP Acquire Method	HP Processing Method pd073125 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP24433,PP24651		
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,PP24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284		
CCC	PP24261,PP24273,PP24279,PP24284		
Internal Standard/PEM			
ICV/I.BLK	PP24273,PP24279,PP24284		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

22	I.BLK	PD089828.D	08 Aug 2025 19:32	AR\AJ	Ok
23	PSTDCCC050	PD089829.D	08 Aug 2025 19:46	AR\AJ	Ok,NS

M : Manual Integration

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD073125

Review By	Abdul	Review On	8/1/2025 8:29:12 AM
Supervise By	mohammad	Supervise On	8/1/2025 9:27:16 AM
SubDirectory	PD073125	HP Acquire Method	HP Processing Method pd073125 8081

STD. NAME	STD REF.#
Tune/Reschk	PP24433,PP24651
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,P P24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284
CCC	PP24261,PP24273,PP24279,PP24284
Internal Standard/PEM	
ICV/I.BLK	PP24273,PP24279,PP24284
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleID	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PD089684.D	31 Jul 2025 09:13		AR\AJ	Ok
2	I.BLK	I.BLK	PD089685.D	31 Jul 2025 10:33		AR\AJ	Ok
3	PEM	PEM	PD089686.D	31 Jul 2025 10:47		AR\AJ	Ok,M
4	RESCHK	RESCHK	PD089687.D	31 Jul 2025 11:34		AR\AJ	Ok
5	PSTDICC100	PSTDICC100	PD089688.D	31 Jul 2025 11:47		AR\AJ	Ok
6	PSTDICC075	PSTDICC075	PD089689.D	31 Jul 2025 12:01		AR\AJ	Ok,M
7	PSTDICC050	PSTDICC050	PD089690.D	31 Jul 2025 12:14		AR\AJ	Ok
8	PSTDICC025	PSTDICC025	PD089691.D	31 Jul 2025 12:28		AR\AJ	Ok
9	PSTDICC005	PSTDICC005	PD089692.D	31 Jul 2025 12:41		AR\AJ	Ok,M
10	PCHLORICC1000	PCHLORICC1000	PD089693.D	31 Jul 2025 12:56		AR\AJ	Ok
11	PCHLORICC750	PCHLORICC750	PD089694.D	31 Jul 2025 13:09		AR\AJ	Ok
12	PCHLORICC500	PCHLORICC500	PD089695.D	31 Jul 2025 13:23		AR\AJ	Ok
13	PCHLORICC250	PCHLORICC250	PD089696.D	31 Jul 2025 13:36		AR\AJ	Ok
14	PCHLORICC050	PCHLORICC050	PD089697.D	31 Jul 2025 13:50		AR\AJ	Ok
15	PTOXICC1000	PTOXICC1000	PD089698.D	31 Jul 2025 14:03		AR\AJ	Ok
16	PTOXICC750	PTOXICC750	PD089699.D	31 Jul 2025 14:17		AR\AJ	Ok
17	PTOXICC500	PTOXICC500	PD089700.D	31 Jul 2025 14:31		AR\AJ	Ok
18	PTOXICC250	PTOXICC250	PD089701.D	31 Jul 2025 14:44		AR\AJ	Ok,M

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD073125

Review By	Abdul	Review On	8/1/2025 8:29:12 AM
Supervise By	mohammad	Supervise On	8/1/2025 9:27:16 AM
SubDirectory	PD073125	HP Acquire Method	HP Processing Method pd073125 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP24433,PP24651		
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,P P24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284		
CCC	PP24261,PP24273,PP24279,PP24284		
Internal Standard/PEM			
ICV/I.BLK	PP24273,PP24279,PP24284		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

19	PTOXICC100	PTOXICC100	PD089702.D	31 Jul 2025 14:58		AR\AJ	Ok,M
20	PSTDICV050	ICVPD073125	PD089703.D	31 Jul 2025 15:11		AR\AJ	Ok
21	PCHLORICV500	ICVPD073125CHLOR	PD089704.D	31 Jul 2025 15:25		AR\AJ	Ok
22	PTOXICV500	ICVPD073125TOX	PD089705.D	31 Jul 2025 15:39		AR\AJ	Ok

M : Manual Integration

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD080925

Review By	Abdul	Review On	8/11/2025 12:49:00 PM
Supervise By		Supervise On	
SubDirectory	PD080925	HP Acquire Method	HP Processing Method pd073125 8081

STD. NAME	STD REF.#
Tune/Reschk	PP24433,PP24651
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,P P24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284
CCC	PP24261,PP24273,PP24279,PP24284
Internal Standard/PEM	
ICV/I.BLK	PP24273,PP24279,PP24284
Surrogate Standard	
MS/MSD Standard	
LCS Standard	

Sr#	SampleId	ClientID	Data File Name	Date-Time	Comment	Operator	Status
1	HEXANE	HEXANE	PD089807.D	08 Aug 2025 10:43		AR\AJ	Ok
2	I.BLK	I.BLK	PD089808.D	08 Aug 2025 10:57		AR\AJ	Ok
3	PEM	PEM	PD089809.D	08 Aug 2025 11:10		AR\AJ	Ok,NS
4	PSTDCCC050	PSTDCCC050	PD089810.D	08 Aug 2025 13:53		AR\AJ	Ok
5	PB169173BL	PB169173BL	PD089811.D	08 Aug 2025 14:51		AR\AJ	Ok
6	PB169173BS	PB169173BS	PD089812.D	08 Aug 2025 15:18		AR\AJ	Ok,NS
7	Q2793-01	VNJ-231	PD089813.D	08 Aug 2025 15:55		AR\AJ	Ok,NS
8	Q2800-01	VNJ-222	PD089814.D	08 Aug 2025 16:08		AR\AJ	Ok,NS
9	Q2801-01	TR-04-080725	PD089815.D	08 Aug 2025 16:22		AR\AJ	Ok,NS
10	Q2759-04	LIQUID-DRUM	PD089816.D	08 Aug 2025 16:35	Both surrogate low in both column	AR\AJ	Not Ok
11	PB169174BL	PB169174BL	PD089817.D	08 Aug 2025 16:49		AR\AJ	Ok
12	PB169174BS	PB169174BS	PD089818.D	08 Aug 2025 17:02	Comp#17,20 recovery fail	AR\AJ	Not Ok
13	PB169174BSD	PB169174BSD	PD089819.D	08 Aug 2025 17:16	Comp#17,20 recovery fail	AR\AJ	Not Ok
14	I.BLK	I.BLK	PD089820.D	08 Aug 2025 17:29		AR\AJ	Ok
15	PSTDCCC050	PSTDCCC050	PD089821.D	08 Aug 2025 17:43		AR\AJ	Ok
16	Q2795-01	COMP-1	PD089822.D	08 Aug 2025 18:10		AR\AJ	Ok,NS
17	Q2795-01MS	COMP-1MS	PD089823.D	08 Aug 2025 18:24		AR\AJ	Ok,NS

Instrument ID: ECD_D

Daily Analysis Runlog For Sequence/QC Batch ID # PD080925

Review By	Abdul	Review On	8/11/2025 12:49:00 PM
Supervise By		Supervise On	
SubDirectory	PD080925	HP Acquire Method	HP Processing Method pd073125 8081
STD. NAME	STD REF.#		
Tune/Reschk	PP24433,PP24651		
Initial Calibration Stds	PP24260,PP24261,PP24262,PP24269,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,P P24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284		
CCC	PP24261,PP24273,PP24279,PP24284		
Internal Standard/PEM			
ICV/I.BLK	PP24273,PP24279,PP24284		
Surrogate Standard			
MS/MSD Standard			
LCS Standard			

18	Q2795-01MSD	COMP-1MSD	PD089824.D	08 Aug 2025 18:37		AR\AJ	Ok,NS
19	Q2795-02	COMP-2	PD089825.D	08 Aug 2025 18:51		AR\AJ	Ok,NS
20	Q2795-03	COMP-3	PD089826.D	08 Aug 2025 19:05		AR\AJ	Ok,NS
21	Q2798-01	TP-6	PD089827.D	08 Aug 2025 19:18		AR\AJ	Ok,NS
22	I.BLK	I.BLK	PD089828.D	08 Aug 2025 19:32		AR\AJ	Ok
23	PSTDCCC050	PSTDCCC050	PD089829.D	08 Aug 2025 19:46	Comp#20 low in 1st column	AR\AJ	Ok,NS

M : Manual Integration



PERCENT SOLID

Supervisor: Iwona
Analyst: jignesh
Date: 8/8/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:10
In Date: 08/07/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:17
Out Date: 08/08/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % SOLID-OVEN

QC:LB136742

Lab ID	Client SampleID	Dish #	Dish Wt(g) (A)	Sample Wt(g)	Dish + Sample Wt(g) (B)	Dish+Dry Sample Wt(g) (C)	% Solid	Comments
Q2793-01	VNJ-231	1	1.15	10.43	11.58	10.82	92.7	
Q2793-02	VNJ-231	2	1.19	10.40	11.59	11.12	95.5	
Q2795-01	COMP-1	3	1.15	10.60	11.75	9.9	82.5	
Q2795-02	COMP-2	4	1.19	10.17	11.36	9.41	80.8	
Q2795-03	COMP-3	5	1.13	10.86	11.99	10.03	82.0	
Q2798-01	TP-6	6	1.18	10.17	11.35	10.25	89.2	
Q2798-02	TP-6-EPH	7	1.18	10.51	11.69	10.04	84.3	
Q2798-03	TP-6-VOC	8	1.18	10.21	11.39	10.06	87.0	
Q2800-01	VNJ-222	12	1.16	10.57	11.73	10.99	93.0	
Q2801-01	TR-04-080725	13	1.17	10.36	11.53	11.05	95.4	
Q2801-02	TR-04-080725-E2	14	1.14	10.41	11.55	10.71	91.9	
Q2802-01	S-1A	9	1.15	10.84	11.99	10.96	90.5	
Q2802-02	S-1B	10	1.16	10.20	11.36	9.04	77.3	
Q2802-03	S-2	11	1.15	10.84	11.99	10.4	85.3	

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

136742

WorkList Name : %1-080725

WorkList ID : 191140

Department : Wet-Chemistry

Date : 08-07-2025 07:55:24

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2793-01	VNJ-231	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/07/2025	Chemtech -SO
Q2793-02	VNJ-231	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/07/2025	Chemtech -SO
Q2795-01	COMP-1	Solid	Percent Solids	Cool 4 deg C	POWE02	D31	08/06/2025	Chemtech -SO
Q2795-02	COMP-2	Solid	Percent Solids	Cool 4 deg C	POWE02	D31	08/06/2025	Chemtech -SO
Q2795-03	COMP-3	Solid	Percent Solids	Cool 4 deg C	POWE02	D31	08/06/2025	Chemtech -SO
Q2798-01	TP-6	Solid	Percent Solids	Cool 4 deg C	PSEG03	D21	08/07/2025	Chemtech -SO
Q2798-02	TP-6-EPH	Solid	Percent Solids	Cool 4 deg C	PSEG03	D21	08/07/2025	Chemtech -SO
Q2798-03	TP-6-VOC	Solid	Percent Solids	Cool 4 deg C	PSEG03	D21	08/07/2025	Chemtech -SO
Q2800-01	VNJ-222	Solid	Percent Solids	Cool 4 deg C	PSEG03	D31	08/07/2025	Chemtech -SO
Q2801-01	TR-04-080725	Solid	Percent Solids	Cool 4 deg C	PSEG05	D21	08/07/2025	Chemtech -SO
Q2801-02	TR-04-080725-E2	Solid	Percent Solids	Cool 4 deg C	PSEG05	D21	08/07/2025	Chemtech -SO
Q2802-01	S-1A	Solid	Percent Solids	Cool 4 deg C	EARTH03	J13	08/07/2025	Chemtech -SO
Q2802-02	S-1B	Solid	Percent Solids	Cool 4 deg C	EARTH03	J13	08/07/2025	Chemtech -SO
Q2802-03	S-2	Solid	Percent Solids	Cool 4 deg C	EARTH03	J13	08/07/2025	Chemtech -SO

08/07/25

08/07/25 15:30

Date/Time

Raw Sample Received by:

Raw Sample Relinquished by:

08/07/25

Date/Time

Raw Sample Received by:

Raw Sample Relinquished by:

15:30

08/07/25

08/07/25

SOP ID: M3541-ASE Extraction-15

Clean Up SOP #: Florisil

Matrix : Solid

Weigh By: RJ

Balance check: RJ

Balance ID: EX-SC-2

pH Strip Lot#: N/A

Extraction By: RJ

Filter By: RJ

pH Meter ID: N/A

Hood ID: 3,7

Extraction Start Date : 08/08/2025

Extraction Start Time : 08:43

Extraction End Date : 08/08/2025

Extraction End Time : 11:45

Concentration By: RS

Supervisor By : RUPESH

Extraction Method: ☐ Separatory Funnel ☐ Continuous Liquid/Liquid ☐ Sonication ☐ Waste Dilution ☒ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	500 PPB	PP24627
Surrogate	1.0ML	200 PPB	PP24663
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Hexane/Acetone/1:1	N/A	EP2627
Baked Na2SO4	N/A	EP2629
Sand	N/A	E3951
Hexane	N/A	E3962
Florisil	N/A	E3927
9:1 Hexane:Acetone Mixture	N/A	EP2596
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

40ML Vial Lot # 03-40BTS721.

KD Bath ID: N/A

Envap ID: NE VAP-02

KD Bath Temperature: N/A

Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
8/8/25	RS (Ext Lab)	RS (Ext Lab)
11:50	Preparation Group	Analysis Group

Analytical Method: M3541-ASE Extraction-15

Concentration Date: 08/08/2025

Sample ID	Client Sample ID	Test	g / mL	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB169173BL	PBLK173	Pesticide-TCL	30.02	N/A	ritesh	RUPESH	10			U6-1
PB169173BS	PLCS173	Pesticide-TCL	30.01	N/A	ritesh	RUPESH	10			2
Q2793-01	VNJ-231	Pesticide-TCL	30.07	N/A	ritesh	RUPESH	10	E		3
Q2795-01	COMP-1	PESTICIDE Group1	30.10	N/A	ritesh	RUPESH	10	E		4
Q2795-01MS	COMP-1MS	PESTICIDE Group1	30.06	N/A	ritesh	RUPESH	10	E		5
Q2795-01MS D	COMP-1MSD	PESTICIDE Group1	30.04	N/A	ritesh	RUPESH	10	E		6
Q2795-02	COMP-2	PESTICIDE Group1	30.04	N/A	ritesh	RUPESH	10	E		U1-1
Q2795-03	COMP-3	PESTICIDE Group1	30.08	N/A	ritesh	RUPESH	10	E		2
Q2798-01	TP-6	Pesticide-TCL	30.03	N/A	ritesh	RUPESH	10	E		3
Q2800-01	VNJ-222	Pesticide-TCL	30.07	N/A	ritesh	RUPESH	10	E		4
Q2801-01	TR-04-080725	Pesticide-TCL	30.08	N/A	ritesh	RUPESH	10	E		5

Rs
8/8

16977
8:43

WORKLIST(Hardcopy Internal Chain)

WorkList Name : Q2793P WorkList ID : 191174 Department : Extraction Date : 08-08-2025 08:38:28

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2793-01	VNJ-231	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	D31	08/07/2025	8081B
Q2795-01	COMP-1	Solid	PESTICIDE Group1	Cool 4 deg C	POWE02	D31	08/06/2025	8081B
Q2795-02	COMP-2	Solid	PESTICIDE Group1	Cool 4 deg C	POWE02	D31	08/06/2025	8081B
Q2795-03	COMP-3	Solid	PESTICIDE Group1	Cool 4 deg C	POWE02	D31	08/06/2025	8081B
Q2798-01	TP-6	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	D21	08/07/2025	8081B
Q2800-01	VNJ-222	Solid	Pesticide-TCL	Cool 4 deg C	PSEG03	D31	08/07/2025	8081B
Q2801-01	TR-04-080725	Solid	Pesticide-TCL	Cool 4 deg C	PSEG05	D21	08/07/2025	8081B

Date/Time 08/08/25 8:38
Raw Sample Received by: RJ (EAT-UCH)
Raw Sample Relinquished by: CP SM

Date/Time 08/08/25 8:55
Raw Sample Received by: CP SM
Raw Sample Relinquished by: RJ (EAT-Kab)

Prep Standard - Chemical Standard Summary

Order ID : Q2795
Test : PESTICIDE Group1
Prepbatch ID : PB169173,
Sequence ID/Qc Batch ID: pd080925,

Standard ID :

EP2627,EP2629,PP24255,PP24256,PP24257,PP24258,PP24259,PP24260,PP24261,PP24262,PP24266,PP24267,PP24268,PP24269,PP24270,PP24271,PP24272,PP24273,PP24274,PP24275,PP24277,PP24278,PP24279,PP24280,PP24281,PP24282,PP24283,PP24284,PP24329,PP24433,PP24627,PP24651,PP24663,

Chemical ID :

E3875,E3877,E3914,E3927,E3937,E3941,E3944,E3949,E3950,E3951,E3962,P12603,P12611,P13037,P13040,P13195,P13246,P13356,P13405,P13785,P13786,P13861,P9052,W3177,

Extractions STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
230	1:1ACETONE/HEXANE	EP2627	07/15/2025	01/15/2026	RUPESHKUMAR SHAH	None	None	Riteshkumar Patel
07/15/2025								

FROM 4000.00000ml of E3949 + 4000.00000ml of E3950 = Final Quantity: 8000.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3923	Baked Sodium Sulfate	EP2629	07/28/2025	01/28/2026	RUPESHKUMAR SHAH	Extraction_SC ALE_2	None	Riteshkumar Patel
(EX-SC-2)								

FROM 4000.00000gram of E3875 = Final Quantity: 4000.000 gram

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24255	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 1.00000ml of P13785 + 9.00000ml of E3877 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3629	20 PPM PEST stock Solution 1st source(RESTEK)	PP24256	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 1.00000ml of P13040 + 9.00000ml of E3877 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1472	20 PPM Pest Stock Solution 2nd Source	PP24257	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 1.00000ml of P13037 + 9.00000ml of E3877 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
1273	20 PPM Mirex Stock (Primary Source)	PP24258	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.20000ml of P9052 + 9.80000ml of E3877 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3663	20 PPM MIREX Stock STD (Secondary source)	PP24259	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani 03/12/2025

FROM 0.20000ml of P13195 + 9.80000ml of E3877 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3630	100/100 PPB PEST Working std.1st Source(RESTEK)	PP24260	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani 03/12/2025

FROM 98.50000ml of E3877 + 0.50000ml of PP24255 + 0.50000ml of PP24256 + 0.50000ml of PP24258 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
80	100/100 PPB Pesticide Working Solution 2nd Source	PP24261	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 98.50000ml of E3877 + 0.50000ml of PP24255 + 0.50000ml of PP24257 + 0.50000ml of PP24259 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
386	1000/100 PPB Chlordane STD (Restek)	PP24262	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.10000ml of P12603 + 99.40000ml of E3877 + 0.50000ml of PP24255 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3746	1000/100 ppb Chlordane STD-RESTEK 2ND SOURCE	PP24266	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani 03/12/2025

FROM 0.10000ml of P12611 + 99.40000ml of E3877 + 0.50000ml of PP24255 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
383	1000/100 PPB Toxaphene STD (Restek)	PP24267	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani 03/12/2025

FROM 0.10000ml of P13405 + 99.40000ml of E3877 + 0.50000ml of PP24255 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3669	1000/100 PPB TOXAPHENE STD 2nd source (RESTEK)	PP24268	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.10000ml of P13861 + 99.40000ml of E3877 + 0.50000ml of PP24255 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3631	75 PPB ICAL PEST STD(RESTEK)	PP24269	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.75000ml of E3877 + 0.25000ml of PP24260 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3632	50 PPB ICAL PEST STD(RESTEK)	PP24270	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.50000ml of E3877 + 0.50000ml of PP24260 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3633	25 PPB ICAL PEST STD(RESTEK)	PP24271	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.75000ml of E3877 + 0.25000ml of PP24260 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3634	5 PPB ICAL PEST STD(RESTEK)	PP24272	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.90000ml of E3877 + 0.10000ml of PP24270 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3988	50 PPB PEST ICV STD(RESTEK)	PP24273	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.50000ml of E3877 + 0.50000ml of PP24261 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
528	CHLOR 750 PPB STD	PP24274	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.25000ml of E3877 + 0.75000ml of PP24262 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
529	CHLOR 500 PPB STD	PP24275	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.50000ml of E3877 + 0.50000ml of PP24262 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
530	CHLOR 250 PPB STD	PP24277	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.75000ml of E3877 + 0.25000ml of PP24262 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3408	CHLOR 50 PPB STD	PP24278	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.90000ml of E3877 + 0.10000ml of PP24275 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
532	CHLOR 500 PPB ICV STD	PP24279	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.50000ml of E3877 + 0.50000ml of PP24266 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
533	TOX 750 PPB STD	PP24280	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.25000ml of E3877 + 0.75000ml of PP24267 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
534	TOX 500 PPB STD	PP24281	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.50000ml of E3877 + 0.50000ml of PP24267 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
535	TOX 250 PPB STD	PP24282	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.75000ml of E3877 + 0.25000ml of PP24267 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2217	TOX 100 PPB STD	PP24283	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.90000ml of E3877 + 0.10000ml of PP24267 = Final Quantity: 1.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3670	TOX 500 PPB ICV std (RESTEK)	PP24284	03/11/2025	08/12/2025	Abdul Mirza	None	None	Ankita Jodhani
								03/12/2025

FROM 0.50000ml of E3877 + 0.50000ml of PP24268 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
84	Pest/PCB Surrogate Stock 20 PPM	PP24329	03/18/2025	08/22/2025	Yogesh Patel	None	None	Abdul Mirza
								04/03/2025

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
518	Pest/PCB I.BLK 20 PPB	PP24433	03/31/2025	08/22/2025	Abdul Mirza	None	None	Yogesh Patel
								04/02/2025

FROM 99.90000ml of E3914 + 0.10000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
79	500 PPB Pesticide Spike Solution	PP24627	06/10/2025	08/12/2025	Abdul Mirza	None	None	Yogesh Patel
								06/11/2025

FROM 95.00000ml of E3937 + 2.50000ml of PP24257 + 2.50000ml of PP24259 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4027	Pesticide resolution Check Mixture 8081	PP24651	06/16/2025	12/11/2025	Abdul Mirza	None	None	Yogesh Patel
								07/22/2025

FROM 1.00000ml of P13246 + 99.00000ml of E3941 = Final Quantity: 100.000 ml



<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
465	200 PPB Pest/PCB Surrogate Spike	PP24663	06/24/2025	12/24/2025	Abdul Mirza	None	None	Yogesh Patel 07/21/2025
<u>FROM</u> 1.00000ml of P13786 + 999.00000ml of E3944 = Final Quantity: 1000.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
PCI Scientific Supply, Inc.	PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1	417203	01/28/2026	07/28/2025 / RUPESH	01/29/2025 / Rajesh	E3875

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	08/12/2025	02/12/2025 / Rajesh	02/12/2025 / Rajesh	E3877

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	09/19/2025	03/19/2025 / RUPESH	03/13/2025 / RUPESH	E3914

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
phenomenex	FS0006 / Cleanert SPE Silica, 1000 mg/6ml	Z0830QB1	04/18/2026	05/30/2025 / RUPESH	03/13/2025 / RUPESH	E3927

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	11/22/2025	05/22/2025 / RUPESH	05/14/2025 / RUPESH	E3937

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	243570	12/11/2025	06/11/2025 / Rajesh	06/04/2025 / Rajesh	E3941

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H1462005	05/24/2027	06/20/2025 / RUPESH	05/14/2025 / RUPESH	E3944

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9254-03 / Acetone, Ultra Resi (cs/4x4L)	24H2762008	04/18/2027	07/08/2025 / RITESHKUMAR	07/03/2025 / RUPESH	E3949

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	07/08/2025 / RITESHKUMAR	07/03/2025 / RUPESH	E3950

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-3382-05 / Sand, Purified (cs/4x2.5kg)	25A2756718	12/31/2028	07/09/2025 / RUPESH	04/28/2020 / RUPESH	E3951

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	25C0362005	04/30/2026	08/05/2025 / RUPESH	07/30/2025 / RUPESH	E3962

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Chlordane Std.	A0197993	09/11/2025	03/10/2025 / Abdul	07/03/2023 / Abdul	P12603

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32021 / Chlordane Std.	A0193299	09/09/2025	03/10/2025 / Abdul	07/03/2023 / Abdul	P12611

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0200423	09/10/2025	03/10/2025 / Abdul	12/26/2023 / Abdul	P13037

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32291 / Pesticide Mix, CLP method, organochlorine Std AB#1, 200ug/mL, hexane/toluene, 1mL/ampul	A0199099	09/10/2025	03/10/2025 / Abdul	12/26/2023 / Abdul	P13040

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	042022	09/10/2025	03/10/2025 / Abdul	01/17/2024 / Abdul	P13195

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	19161 / 8081 pesticide resolution check mixture	013124	12/17/2025	06/17/2025 / Abdul	02/09/2024 / Abdul	P13246

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0206810	09/18/2025	03/18/2025 / yogesh	04/22/2024 / Abdul	P13356

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0203038	09/09/2025	03/10/2025 / Abdul	05/15/2024 / Abdul	P13405

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	09/10/2025	03/10/2025 / Abdul	11/19/2024 / Ankita	P13785

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL	A0214495	12/24/2025	06/24/2025 / Abdul	11/19/2024 / Ankita	P13786

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Restek	32005 / Toxaphene Standard	A0210240	09/10/2025	03/10/2025 / Abdul	12/09/2024 / Abdul	P13861

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	79136 / Mirex, 1000 ug/ml	112018	09/10/2025	03/10/2025 / Abdul	11/01/2019 / Stephen	P9052

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L)	24G1962003	08/22/2025	02/03/2025 / jignesh	01/31/2025 / jignesh	W3177



**PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.**

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 67 67
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

PRODUCT :	SODIUM SULFATE CRYSTALS ANHYDROUS		
QUALITY :	ACS (CODE RMB3375)	FORMULA :	Na ₂ SO ₄
SPECIFICATION NUMBER:	6399	RELEASE DATE:	MAY/23/2024
LOT NUMBER :	417203		

TEST	SPECIFICATIONS	LOT VALUES
Assay (Na ₂ SO ₄)	Min. 99.0%	99.8 %
pH of a 5% solution at 25°C	5.2 - 9.2	6.2
Insoluble matter	Max. 0.01%	0.001 %
Loss on ignition	Max. 0.5%	0.1 %
Chloride (Cl)	Max. 0.001%	<0.001 %
Nitrogen compounds (as N)	Max. 5 ppm	<5 ppm
Phosphate (PO ₄)	Max. 0.001%	<0.001 %
Heavy metals (as Pb)	Max. 5 ppm	<5 ppm
Iron (Fe)	Max. 0.001%	<0.001 %
Calcium (Ca)	Max. 0.01%	0.001 %
Magnesium (Mg)	Max. 0.005%	0.001 %
Potassium (K)	Max. 0.008%	0.001 %
Extraction-concentration suitability	Passes test	Passes test
Appearance	Passes test	Passes test
Identification	Passes test	Passes test
Solubility and foreign matter	Passes test	Passes test
Retained on US Standard No. 10 sieve	Max. 1%	0.2 %
Retained on US Standard No. 60 sieve	Min. 94%	96.2 %
Through US Standard No. 60 sieve	Max. 5%	3.5 %
Through US Standard No. 100 sieve	Max. 10%	0.1 %

COMMENTS

QC: PhC Irma Belmares

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd. by RP on 2/12/25

 E3877

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT - 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001

Recd by RS on 3/14/25



E3914

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
 If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Cleanert Florisil

1g/6ml 30/pkg

LOT#: Z0830QB1

MFG#: G01256

CAT# FS0006



Agela Technologies

Made in China

固相萃取产品

E3927



Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3937

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Certificate of Analysis

1 Reagent Lane
 Fair Lawn, NJ 07410
 201.796.7100 tel
 201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System
 Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

Catalog Number	H303	Quality Test / Release Date	11/07/2024
Lot Number	243570		
Description	HEXANES - OPTIMA		
Country of Origin	United States	Suggested Retest Date	Nov/2029
Chemical Origin	Organic - non animal		
BSE/TSE Comment	No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product.		

N/A			
Result Name	Units	Specifications	Test Value
APPEARANCE		REPORT	Clear, colorless liquid
ASSAY (N-HEXANE)	%	>= 60	69
ASSAY (SUM C6 HYDROCARBONS)	%	>= 99.9	>99.9
COLOR	APHA	<= 5	<5
DENSITY AT 25 DEGREES C	GM/ML	Inclusive Between 0.653 - 0.673	0.669
EVAPORATION RESIDUE	ppm	<= 1	<1
FLUORESCENCE BACKGROUND	ppb	<= 1	<1
IDENTIFICATION	PASS/FAIL	= PASS TEST	PASS TEST
OPTICAL ABS AT 195 NM	ABS. UNITS	<= 1	0.74
OPTICAL ABS AT 210 NM	ABS. UNITS	<= 0.25	0.17
OPTICAL ABS AT 220 NM	ABS. UNITS	<= 0.07	0.05
OPTICAL ABS AT 254 NM	ABS. UNITS	<= 0.005	0.001
PESTICIDE RESIDUE ANALYSIS	NG/L	<= 10	<10
REFRACTIVE INDEX @ 25 DEG C		Inclusive Between 1.375 - 1.385	1.379
SUITABILITY FOR GC/MS		= PASS TEST	PASS TEST
SULFUR COMPOUNDS	%	<= 0.005	<0.005
THIOPHENE	PASS/FAIL	= PASS TEST	PASS TEST
WATER (H2O)	%	<= 0.01	<0.01
WATER-SOLUBLE TITRABLE ACID	MEQ/G	<= 0.0003	0.0001



Recd. by RI on 6/11/25

E3941

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.
 If there are any questions with this certificate, please call at (800) 227-6701.
 *Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

avantor™



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	99.8 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.2 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (μeq/g)	<= 0.3	0.2
Titration Base (μeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	0.2 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	<1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3944

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis

Avantor™



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay ((CH ₃) ₂ CO) (by GC, corrected for water)	>= 99.4 %	100.0 %
Color (APHA)	<= 10	5
Residue after Evaporation	<= 1.0 ppm	0.0 ppm
Substances Reducing Permanganate	Passes Test	Passes Test
Titration Acid (µeq/g)	<= 0.3	0.2
Titration Base (µeq/g)	<= 0.6	<0.1
Water (H ₂ O)	<= 0.5 %	<0.1 %
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	<= 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	<= 10	1

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Reel on 7/2/25

E3949

J. Croak

Jamie Croak

Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Avantor Performance Materials LLC

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03

Batch No.: 25C0362005

Manufactured Date: 2025-01-29

Expiration Date: 2026-04-30

Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

3950

Recd on 7/02/25

Jamie Croak
Director Quality Operations, Bioscience Production



Material	BDH9274-2.5KG
Material Description	BDH SAND STDD OTTAWA W+I 2.5KG
Grade	NOT APPLICABLE
Batch	25A2756718
Reassay Date	12/31/2028
CAS Number	14808-60-7
Molecular Formula	SiO ₂
Molecular Mass	60.09
Date of Manufacture	12/05/2024
Storage	Room Temperature

Characteristics	Specifications	Measured Values
Appearance	Beige granules.	Beige granules.
Moisture	<= 0.1 %	0.1 %
Particle Size 30-40 mesh	>= 80 %	99 %
CUSTOMER PART # BDH9274-2.5KG		

Received on 1/12/25.

E3951

Internal ID #: 793

Signature

We certify that this batch conforms to the specifications listed above.

This document has been electronically produced and is valid without a signature.

Leona Edwardson, Quality Control Sr. Manager - Solon
VWR Chemicals, LLC.
28600 Fountain Parkway, Solon OH 44139 USA

Additional Information

Analysis may have been rounded to significant digits in specification limits

Product meets analytical specifications of the grades listed.

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	1
ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL)	≤ 10	6
ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL)	≤ 5	5
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	100.0 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	100 %
Color (APHA)	≤ 10	10
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	$< 0.01 \%$

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/30/25

E3962

Jamie Croak
Director Quality Operations, Bioscience Production

RESTEK

110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis
chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32021 **Lot No.:** A0193299
Description : Chlordane Standard
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL **Pkg Amt:** > 1 mL
Expiration Date : April 30, 2029 **Storage:** 10°C or colder
Ship: Ambient

P12616
↓
P12615
Five
7/3/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Chlordane 10% trans-Chlordane; 9% cis-Chlordane; 81% other isomers	57-74-9	978545	—%	1,010.0 µg/mL	+/- 56.0475

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

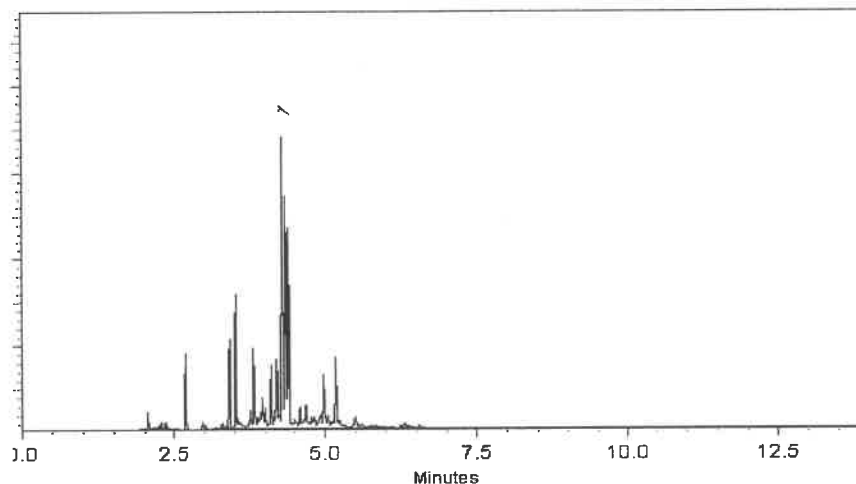

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Bryan Snyder
Bryan Snyder - Operations Tech I

Date Mixed: 06-Jan-2023

Balance Serial # B442140311

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Jan-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

CRm
P 12611
↓
P 12615
⑤
CRout
7/3/2023



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 Lot No.: A0199099

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL Pkg Amt: > 1 mL

Expiration Date : June 30, 2027 Storage: 10°C or colder

Ship: Ambient

P130397 5
↓
P13043 1
✓
12-26-2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	alpha-BHC	319-84-6	14434500	99%	200.0 µg/mL	+/- 8.9732
2	gamma-BHC (Lindane)	58-89-9	14184400	98%	200.1 µg/mL	+/- 8.9762
3	beta-BHC	319-85-7	BCCC6425	99%	200.3 µg/mL	+/- 8.9844
4	delta-BHC	319-86-8	14450800	98%	200.0 µg/mL	+/- 8.9740
5	Heptachlor	76-44-8	813251	99%	200.1 µg/mL	+/- 8.9754
6	Aldrin	309-00-2	14389400	98%	200.0 µg/mL	+/- 8.9718
7	Heptachlor epoxide (isomer B)	1024-57-3	14448800	99%	200.1 µg/mL	+/- 8.9754
8	trans-Chlordane	5103-74-2	32943	98%	199.9 µg/mL	+/- 8.9696
9	cis-Chlordane	5103-71-9	31766	98%	200.1 µg/mL	+/- 8.9762
10	Endosulfan I	959-98-8	BCCF4060	99%	200.1 µg/mL	+/- 8.9754
11	4,4'-DDE	72-55-9	GHYQG	99%	200.1 µg/mL	+/- 8.9777
12	Dieldrin	60-57-1	11129900	98%	200.0 µg/mL	+/- 8.9718
13	Endrin	72-20-8	14123200	98%	199.9 µg/mL	+/- 8.9696
14	4,4'-DDD	72-54-8	HAN02	99%	200.1 µg/mL	+/- 8.9777
15	Endosulfan II	33213-65-9	14374700	99%	200.0 µg/mL	+/- 8.9732
16	4,4'-DDT	50-29-3	230410JLMA	98%	200.0 µg/mL	+/- 8.9718

17	Endrin aldehyde	7421-93-4	30720	98%	200.1	µg/mL	+/- 8.9784
18	Endosulfan sulfate	1031-07-8	BCCH9010	99%	200.0	µg/mL	+/- 8.9732
19	Methoxychlor	72-43-5	13668200	99%	200.1	µg/mL	+/- 8.9777
20	Endrin ketone	53494-70-5	1-ABS-16-7	98%	200.0	µg/mL	+/- 8.9740

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane/Toluene (50:50)
CAS # 110-54-3/108-88-3
Purity 99%

P13039
 ↓
 P13043
 5
 1
 JAW
 12/26/23

Quality Confirmation Test

Column:
 30m x .25mm x .2um
 Rtx-CLP II (cat.# 11323)

Carrier Gas:
 helium-constant pressure 20 psi.

Temp. Program:
 150°C to 300°C
 @ 4°C/min. (hold 5 min.)


Inj. Temp:
 200°C

Det. Temp:
 300°C

Det. Type:
 ECD

Split Vent:
 Split ratio 50:1

Inj. Vol
 1µl

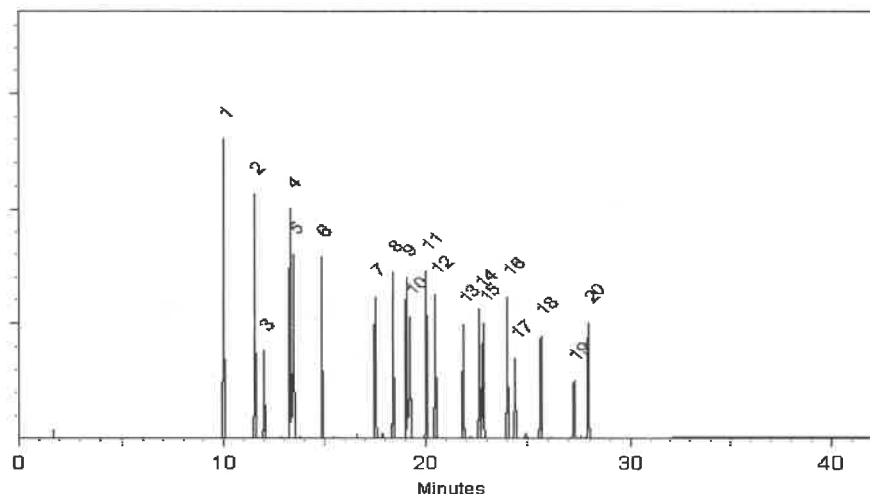

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Josh McCloskey
 Josh McCloskey - Operations Technician I

Date Mixed: 19-Jun-2023

Balance Serial # 1128360905

Jennifer Pollino
 Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 23-Jun-2023

Manufactured under Restek's ISO 9001:2015
 Registered Quality System
 Certificate #FM 80397



CERTIFIED WEIGHT REPORT

Part Number: 79136
Lot Number: 042022
Description: Mirex

Solvent(s): Acetone
Lot# 81025

Expiration Date: 04/2027
Recommended Storage: Refrigerate (4 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 6UTB

SE-05 Balance Uncertainty
0.006 Flask Uncertainty



Weight(s) shown below were combined and diluted to (mL):

Formulated By:	<i>Prashant Chauhan</i>	DATE	04/2022
Reviewed By:	<i>Pedro L. Renteria</i>	DATE	04/2022

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty Purity	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (±) (µg/mL)	CAS#	OSHA PEL (TWA)	LD50

1. Mirex 437 9492400 1000 99.4 0.5 0.05034 0.05040 1001.1 10.3 2385-85-5 N/A or-rel:306mg/kg

Method GC7MSD-1.M: Column: SPB-608 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 150°C (4min.), Temp 2 = 290°C (13.5 min.), Rate = 8°C/min., Injector B = 200°C, Detector B = 290°C. Split Ratio = 100:1, Scan Rate = 2. Analysis performed by Candice Warren.

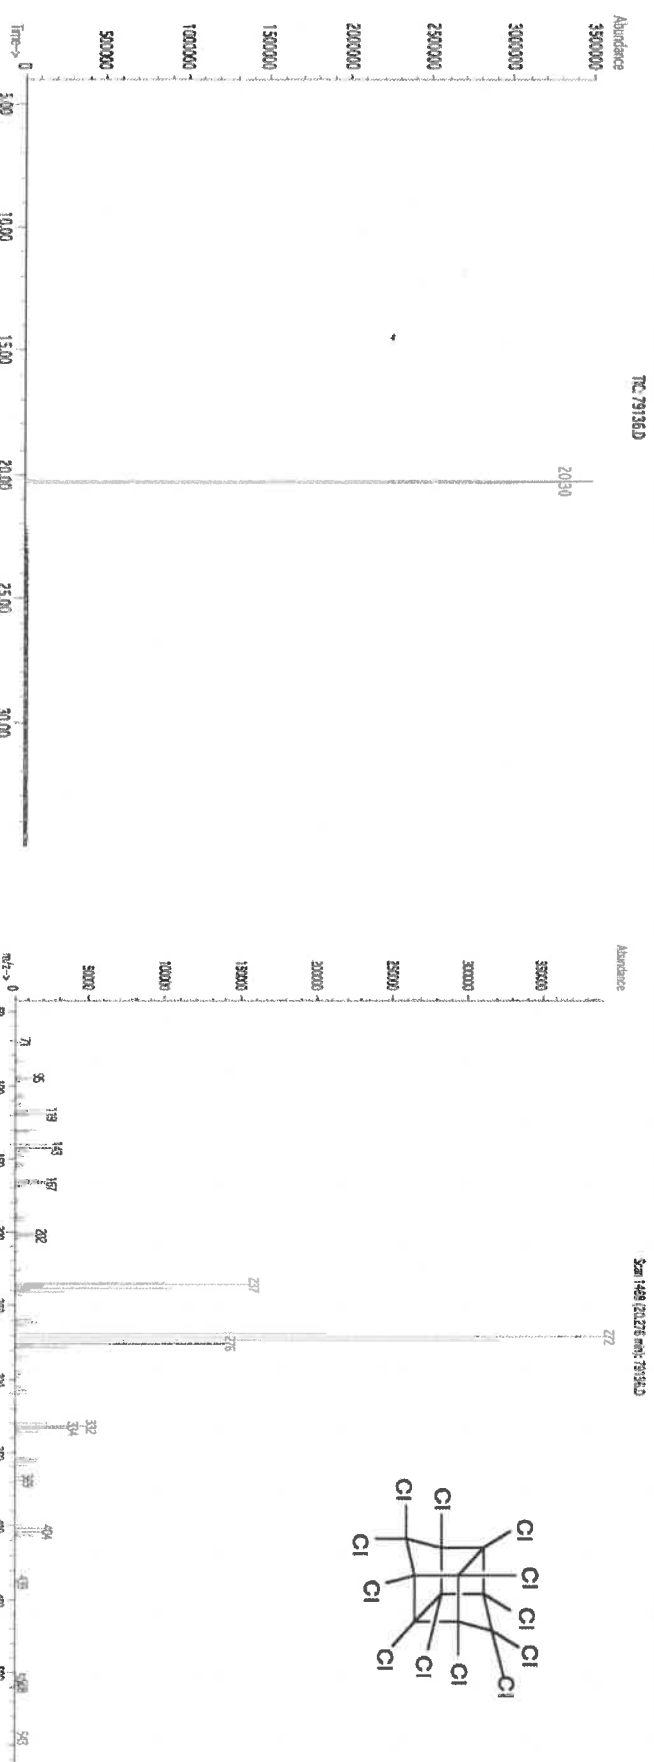

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening, sample, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N., and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Handwritten notes:
P13195
P13199
5
01/17/2024

01/17/2024
JALIN

5



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32021 Lot No.: A0197993
Description : Chlordane Standard
Chlordane Standard 1000µg/mL, Hexane, 1mL/ampul
Container Size : 2 mL Pkg Amt: > 1 mL
Expiration Date : August 31, 2029 Storage: 10°C or colder
Ship: Ambient

P 12603
↓
P 12605
3
Kauf
7/3/2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Chlordane 10% trans-Chlordane; 9% cis-Chlordane; 81% other isomers	57-74-9	978545	----%	1,005.0 µg/mL	+/- 55.7700

Solvent: Hexane
CAS # 110-54-3
Purity 99%

* Expanded Uncertainty displayed in same units as Grav. Conc.

Tech Tips:

CAS #57-74-9 nomenclature is based on EPA method 8081B.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

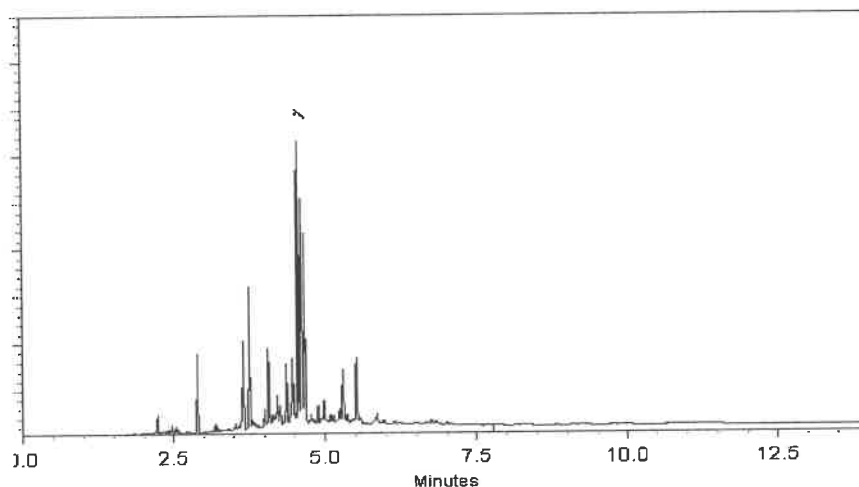

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Morgan Craighead - Mix Technician


Date Mixed: 11-May-2023

Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-May-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 12603 } (3)
↓
P 12605

7/3/2023



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32291 **Lot No.:** A0200423

Description : Organochlorine Pesticide Mix AB #1

Organochlorine Pesticide Mix AB #1 200µg/mL, Hexane/Toluene(50:50), 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2027 **Storage:** 10°C or colder

Ship: Ambient

P 13034
↓
P 13038
12.26.2023

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	alpha-BHC	319-84-6	14434500	99%	200.5 µg/mL	+/- 8.9956
2	gamma-BHC (Lindane)	58-89-9	14184400	98%	199.9 µg/mL	+/- 8.9696
3	beta-BHC	319-85-7	BCCC6425	99%	200.0 µg/mL	+/- 8.9732
4	delta-BHC	319-86-8	14450800	98%	199.9 µg/mL	+/- 8.9696
5	Heptachlor	76-44-8	813251	99%	202.0 µg/mL	+/- 9.0629
6	Aldrin	309-00-2	14389400	98%	200.9 µg/mL	+/- 9.0136
7	Heptachlor epoxide (isomer B)	1024-57-3	14448800	99%	200.0 µg/mL	+/- 8.9732
8	trans-Chlordane	5103-74-2	34616	99%	200.5 µg/mL	+/- 8.9956
9	cis-Chlordane	5103-71-9	31766	98%	201.4 µg/mL	+/- 9.0356
10	Endosulfan I	959-98-8	BCCF4060	99%	200.0 µg/mL	+/- 8.9732
11	4,4'-DDE	72-55-9	GHYQG	99%	201.5 µg/mL	+/- 9.0405
12	Dieldrin	60-57-1	14515000	98%	199.9 µg/mL	+/- 8.9696
13	Endrin	72-20-8	14485300	98%	200.4 µg/mL	+/- 8.9916
14	4,4'-DDD	72-54-8	HAN02	99%	200.5 µg/mL	+/- 8.9956
15	Endosulfan II	33213-65-9	14374700	99%	200.0 µg/mL	+/- 8.9732
16	4,4'-DDT	50-29-3	230410JLMA	98%	201.9 µg/mL	+/- 9.0575

17	Endrin aldehyde	7421-93-4	30720	98%	201.4 µg/mL	+/- 9.0356
18	Endosulfan sulfate	1031-07-8	BCCH9010	99%	200.5 µg/mL	+/- 8.9956
19	Methoxychlor	72-43-5	14563200	98%	200.9 µg/mL	+/- 9.0136
20	Endrin ketone	53494-70-5	14537700	98%	199.9 µg/mL	+/- 8.9696

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane/Toluene (50:50)
CAS # 110-54-3/108-88-3
Purity 99%

P13034
P13038
1
5
12/26/2023

Quality Confirmation Test

Column:
30m x .25mm x .2µm
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
150°C to 300°C
@ 4°C/min. (hold 5 min.)


Inj. Temp:
200°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
Split ratio 50:1

Inj. Vol
1µl

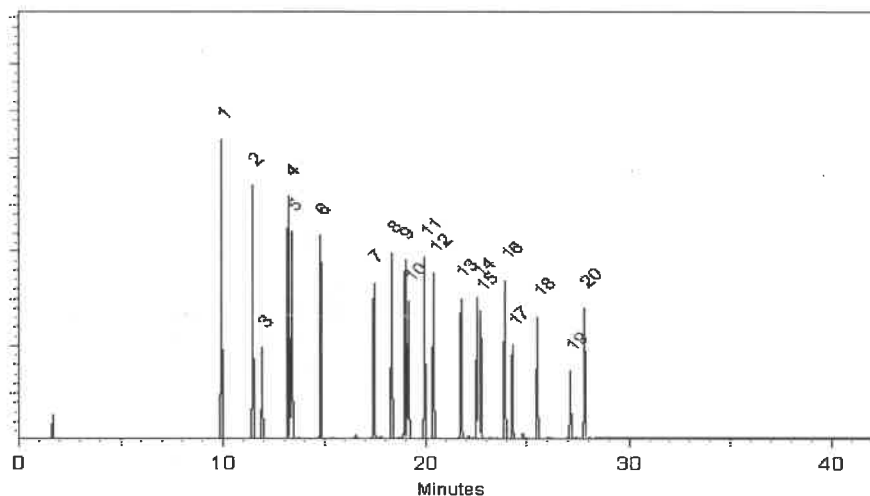

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Sam Moodler
Sam Moodler - Operations Tech I

Date Mixed: 31-Jul-2023 **Balance Serial #** B442140311

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 03-Aug-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0206810

Description : Pesticide Surrogate Mix
Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : April 30, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P13348
↓
P13357
10
DAUF
04/25/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.3 µg/mL	+/- 11.1143
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30638	99%	200.6 µg/mL	+/- 11.1298

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:


10 ml/min.

Inj. Vol

1µl

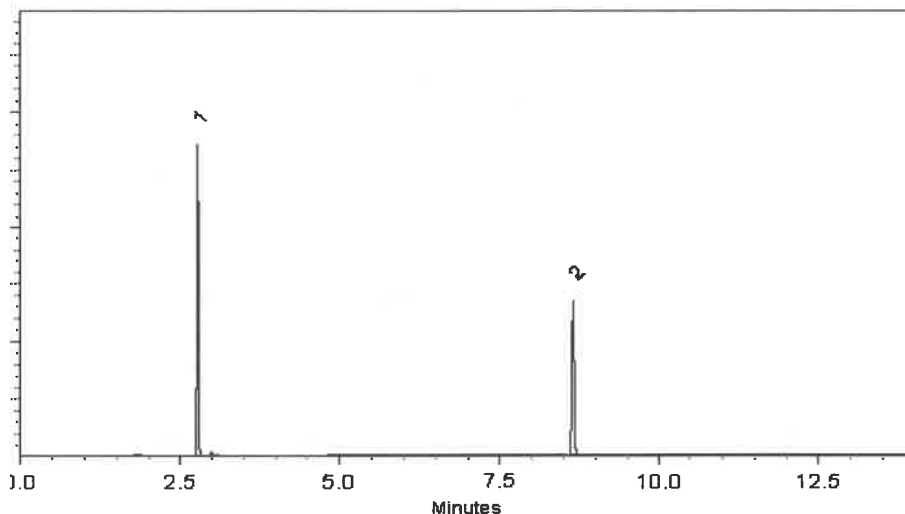


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Jan-2024


Balance Serial # 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
10


SAUF
04/25/2025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32005 **Lot No.:** A0203038

Description : Toxaphene Standard
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : January 31, 2028 **Storage:** 10°C or colder
Ship: Ambient

P13402
P13406
5/22/2024

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Toxaphene	8001-35-2	1051817	---%	1,009.0 µg/mL	+/- 55.9920

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

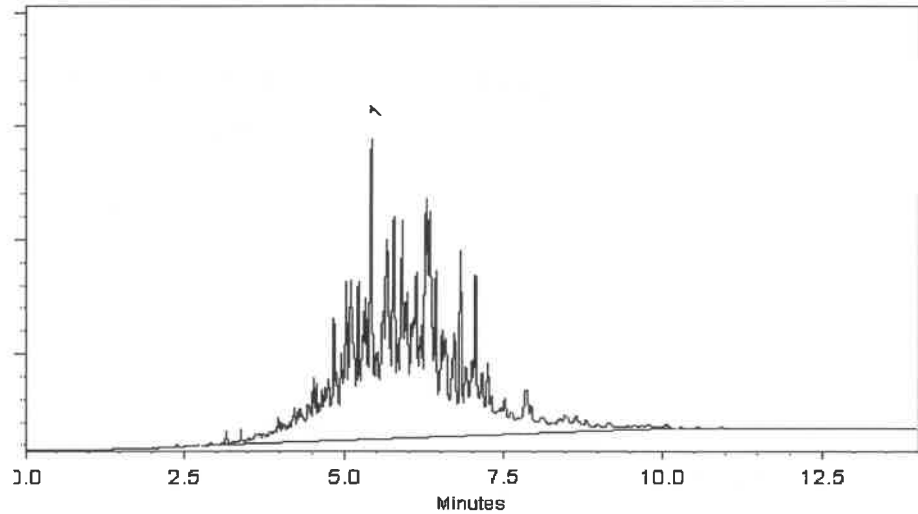


This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Dakota Parson - Operations Technician I

Date Mixed: 10-Oct-2023

Balance Serial # 1128353505


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 16-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13402
↓
P13406 } (5)

5/22/2024




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785
AJ
11/19/24
P19789

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:
30m x 25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
10 ml/min.

Inj. Vol
1µl

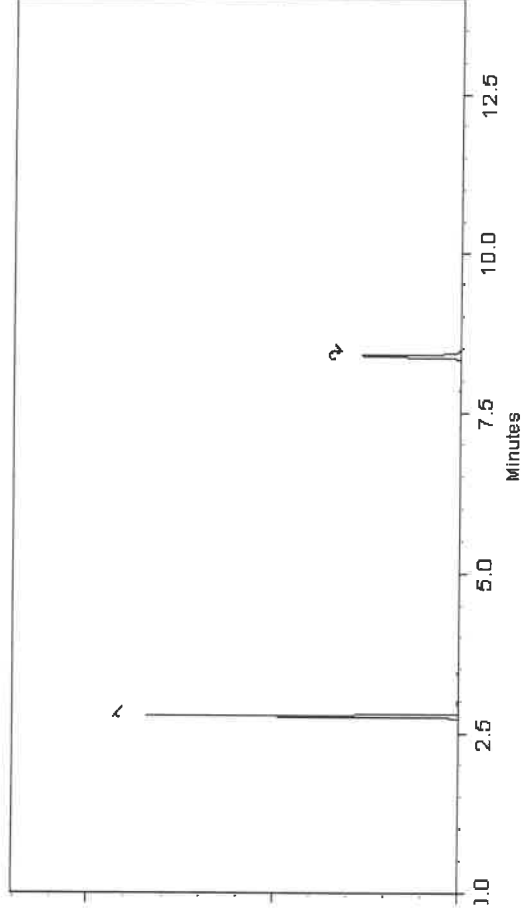

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. P.
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 **Balance Serial #** B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397




110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000 **Lot No.:** A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : October 31, 2030 **Storage:** 10°C or colder

Handling: Contains PCBs - sonicate prior to use. **Ship:** Ambient

P19785
AJ
11/19/24
P19789

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	2,4,5,6-Tetrachloro-m-xylene	877-09-8	RP220407	99%	200.2 µg/mL	+/- 11.1087
2	Decachlorobiphenyl (BZ# 209)	2051-24-3	30679	99%	201.4 µg/mL	+/- 11.1753

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone
CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isooctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:
30m x 25mm x 2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:
helium-constant pressure 20 psi.

Temp. Program:
200°C to 300°C
@ 25°C/min. (hold 10 min.)


Inj. Temp:
250°C

Det. Temp:
300°C

Det. Type:
ECD

Split Vent:
10 ml/min.

Inj. Vol
1µl

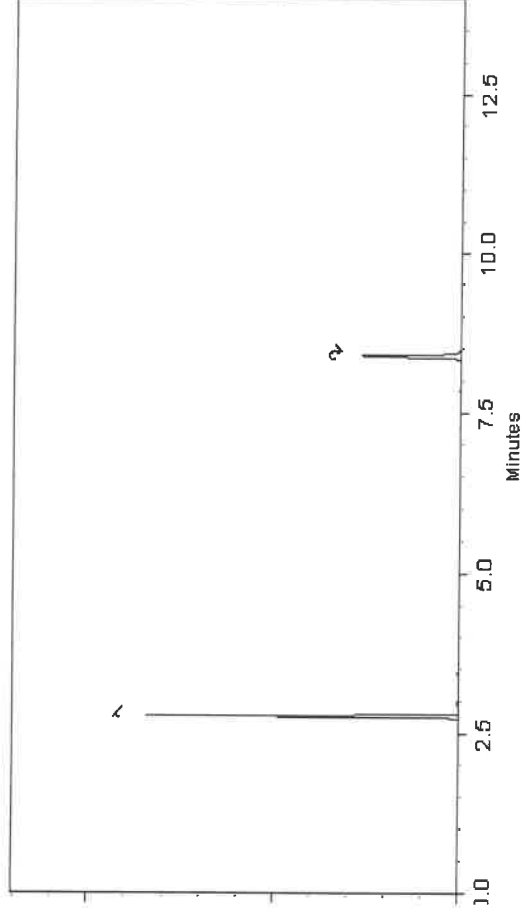

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

A. O. P.
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 Balance Serial # B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32005 **Lot No.:** A0210240

Description : Toxaphene Standard
Toxaphene Standard 1000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL **Pkg Amt:** > 1 mL

Expiration Date : July 31, 2028 **Storage:** 10°C or colder

Ship: Ambient

CERTIFIED VALUES

Elution Order	Compound	CAS #	Lot #	Purity	Grav. Conc. (weight/volume)	Expanded Uncertainty * (95% C.L.; K=2)
1	Toxaphene	8001-35-2	1051817	----%	1,009.3 µg/mL	+/- 56.0105

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P13861
P13862

12/9/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

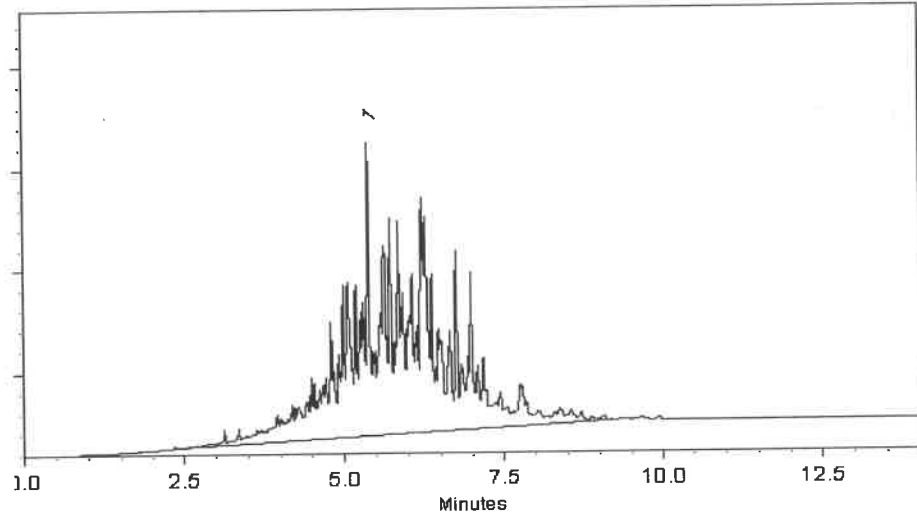

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Amanda Miller - Operations Tech III - ARM QC

Date Mixed: 11-Apr-2024

Balance Serial # B442140311



Christie Mills - Operations Lead Tech - ARM QC

Date Passed: 26-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13861 } ②
P13862 }


12/9/2024



CERTIFIED WEIGHT REPORT


Part Number: 72072
Lot Number: 112018
Description: n-Tetracosane-d50
Expiration Date: 112028
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test ID#: 2684186
Weight(s) shown below were combined and diluted to (mL): 200.0

Solvent(s): Lot#
Methylene chloride 102669
Received by
SG on 11/11/19
p9044-p9053
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Prashant Chauhan	112018	DATE
Reviewed By:	Pedro Rentas	112018	DATE

Compound	RM#	Lot Number	Nominal Conc (µg/mL)	Purity (%)	Uncertainty	Target Weight (g)	Actual Weight (g)	Actual Conc (µg/mL)	Expanded Uncertainty (+/-) (µg/mL)	SDS Information (Solvent Safety Info. On Attached pg.)
1. n-Tetracosane-d50	2072	PR-17753/09216TC1	1000	98	0.2	0.20411	0.20415	1000.2	4.2	18416-32-3 N/A
Method GC8MSD-3.M: Column:SPB-5 (30m X 0.25mm ID X 0.25µm film thickness) Temp 1 = 50°C (1min.), Temp 2 = 300°C (9min.), Rate = 10°C/min., Injector B= 250°C, Detector B = 275°C, Split Ratio = 100:1, Scan Rate = 2. Analysis performed by: Candice Warren.										

TC 720720

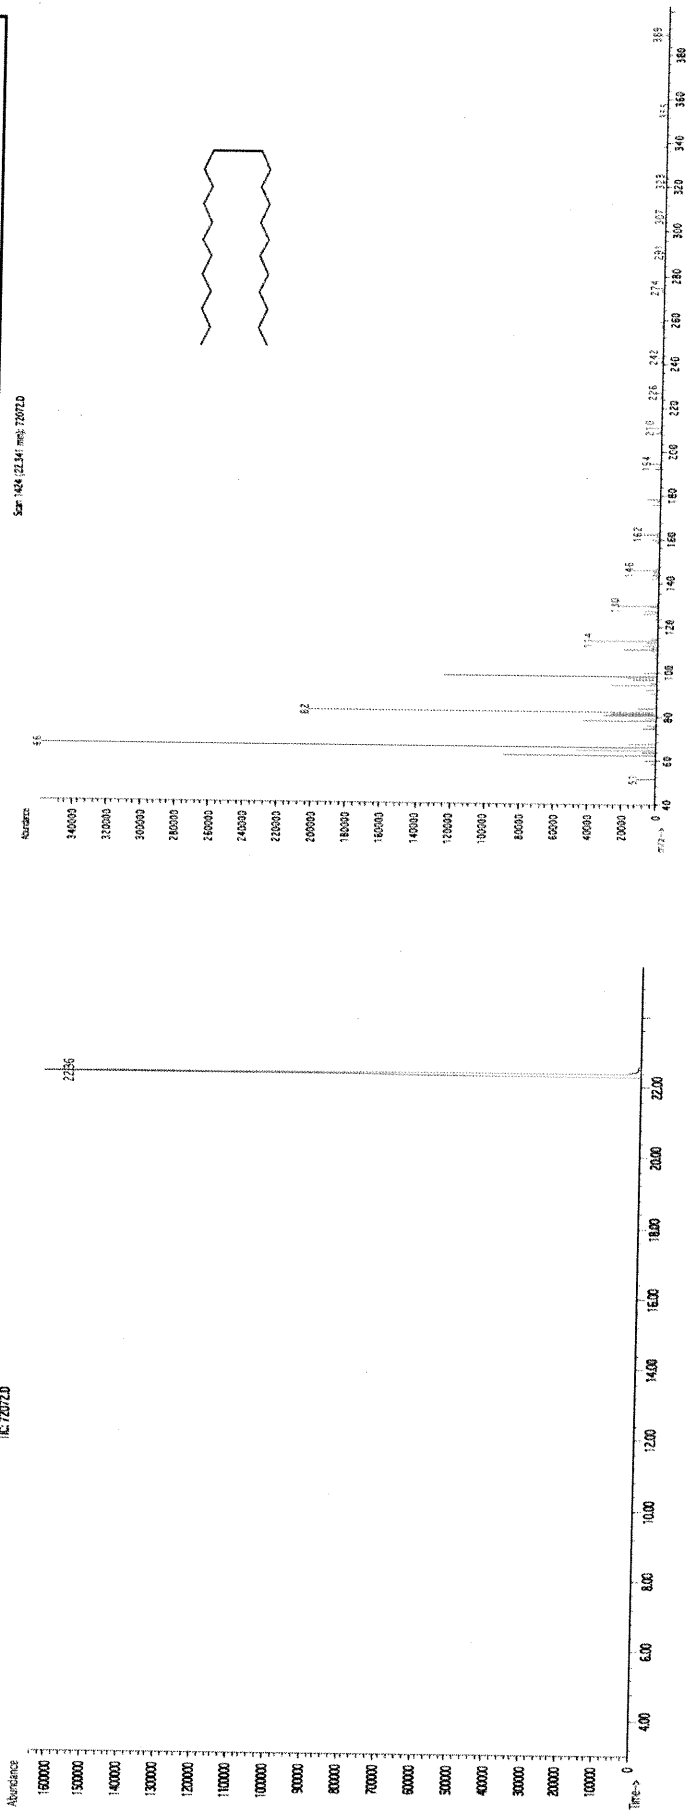

The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
• Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
• All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
• Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).



Run 40, "P72072 L112018 [1000µg/mL in MeCl2]"

Run Length: 35.00 min, 20999 points at 10 points/second.

Created: Thu, Nov 22, 2018 at 7:23:18 AM.

Sampled: Sequence "112018-GC4M1", Method "GC4-M1".

Analyzed using Method "GC4-M1".

Comments

GC4-M1 Analysis by Melissa Stonier


Column ID SPB5 L#60062-01A : 30 meter x 0.53mm x 1.5µm Film Thickness

Flow rates: Total Flow = 300 mL/min, Helium (carrier) = 6.5 mL, Helium (make-up) = 25 mL, Hydrogen (detector) = 30 mL, Air (detector) = 360 mL

Oven Temp 1 = 50°C (1 min), Rate = 10°C/min, Oven Temp 2 = 300°C (9 min), Total Run Time = 35 Minutes.

Injector Temp = 200°C, FID Temp = 300°C, FID Signal = eDAQ Channel 1.

Gas Chromatograph = HP 5890, Auto Sampler = HP 7673, Standard Injection = 0.5 µL, Range = 3

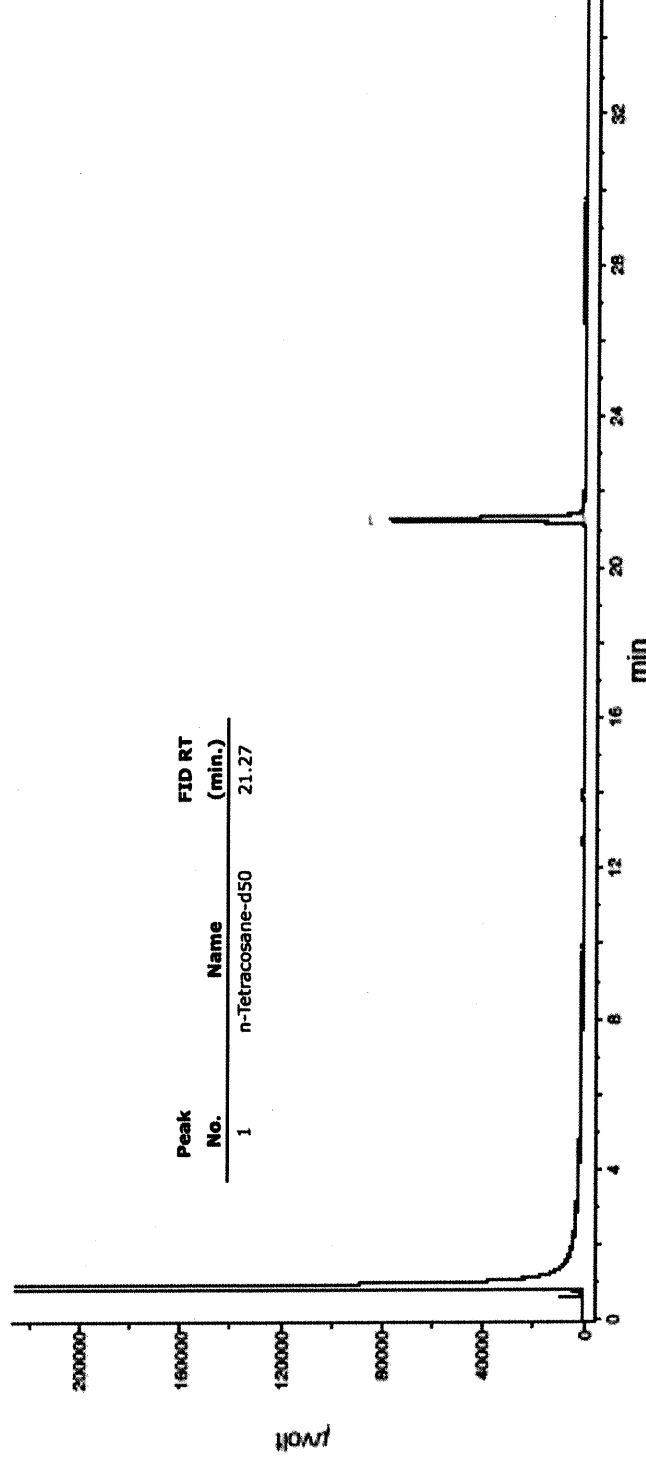

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL)	≤ 5	3
ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL)	≤ 10	1
ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL)	≤ 5	1
Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water)	$\geq 99.5 \%$	99.7 %
Assay (as n-Hexane) (by GC, corrected for water)	$\geq 95 \%$	98 %
Color (APHA)	≤ 10	5
Residue after Evaporation	≤ 1.0 ppm	0.1 ppm
Substances Darkened by H ₂ SO ₄	Passes Test	Passes Test
Water (by KF, coulometric)	$\leq 0.05 \%$	< 0.01 %

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak
Director Quality Operations, Bioscience Production



SHIPPING DOCUMENTS

CLIENT INFORMATION

REPORT TO BE SENT TO:
COMPANY: Kleinfelder
ADDRESS: 180 Sheree Blvd. Suite 3800
CITY: Exton STATE: PA ZIP: 19341
ATTENTION: Mark Warchol
PHONE: 484-883-3892 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Girard School
PROJECT NO.: 26001558.001A LOCATION: Philadelphia
PROJECT MANAGER: Mark Warchol
e-mail: mwarchol@kleinfelder.com
PHONE: 484-883-3892 FAX:

CLIENT BILLING INFORMATION

BILL TO: PO#: Same
ADDRESS:
CITY: STATE: ZIP:
ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) 5 DAYS*
HARDCOPY (DATA PACKAGE): 5 DAYS*
EDD: 5 DAYS*
*TO BE APPROVED BY CHEMTECH
STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☒ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☐ EDD FORMAT

PAVED Historic
Cleaner Hold

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS	
			COMP	GRAB	DATE	TIME		E	E								← Specify Preservatives	
1.	COMP-1	Soil	✓		8/6/25	10:20	4	✓									A-HCl	D-NaOH
2.	COMP-2					11:25	1	↓									B-HNO3	E-ICE
3.	COMP-3		↓			12:20	1	↓									C-H2SO4	F-OTHER
4.	SB-1			✓		9:40	1		✓									
5.	SB-2					9:50	1		↓									
6.	SB-3					10:00	1		↓									
7.	SB-4					10:15	1		↓									
8.	SB-5					10:35	1		↓									
9.	SB-6					10:50	1		↓									
10.	SB-7		↓	↓		11:00	1		↓									

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. [Signature]	DATE/TIME: 8/6/25	RECEIVED BY: 1. [Signature]	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP
RELINQUISHED BY SAMPLER: 2. [Signature]	DATE/TIME: 11:28 8/7/25	RECEIVED BY: 2. [Signature]	Comments: Hold grab samples SB-1 thru SB-12 2.8"
RELINQUISHED BY SAMPLER: 3. [Signature]	DATE/TIME:	RECEIVED BY: 3. [Signature]	IF Gun #1

Page 1 of 2 CLIENT: ☐ Hand Delivered ☒ Other FedEx Shipment Complete ☐ YES ☐ NO

CLIENT INFORMATION

COMPANY: Kleinfelder
ADDRESS: 180 Saeree Blvd. Suite 3800
CITY: Exton STATE: PA ZIP: 19341
ATTENTION: Mark Warchol
PHONE: 484-883-3892 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: Girard School
PROJECT NO.: 1600/558-001A LOCATION: Philadelphia
PROJECT MANAGER: Mark Warchol
e-mail: mwarchol@kleinfelder.com
PHONE: 484-883-3892 FAX:

CLIENT BILLING INFORMATION

BILL TO: PO#: Same
ADDRESS: Same
CITY: STATE: ZIP:
ATTENTION: PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) 5 DAYS*
HARDCOPY (DATA PACKAGE): 5 DAYS*
EDD: 5 DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

☐ Level 1 (Results Only) ☐ Level 4 (QC + Full Raw Data)
☒ Level 2 (Results + QC) ☐ NJ Reduced ☐ US EPA CLP
☐ Level 3 (Results + QC) ☐ NYS ASP A ☐ NYS ASP B
+ Raw Data ☐ Other
☐ EDD FORMAT

PRESERVATIVES

COMMENTS

ALLIANCE SAMPLE ID	PROJECT SAMPLE IDENTIFICATION	SAMPLE MATRIX	SAMPLE TYPE		SAMPLE COLLECTION		# OF BOTTLES	PRESERVATIVES									COMMENTS ← Specify Preservatives A-HCl D-NaOH B-HNO3 E-ICE C-H2SO4 F-OTHER
			COMP	GRAB	DATE	TIME		1	2	3	4	5	6	7	8	9	
1.	SB-8	Soil		✓	8/6/25	11:20	1		✓								
2.	SB-9	↓		↓	↓	11:50	↓		↓								
3.	SB-10	↓		↓	↓	12:00	↓		↓								
4.	SB-11	↓		↓	↓	12:10	↓		↓								
5.	SB-12	↓		↓	↓	12:15	↓		↓								
6.																	
7.																	
8.																	
9.																	
10.																	

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

RELINQUISHED BY SAMPLER: 1. <i>[Signature]</i>	DATE/TIME: 8/6/25	RECEIVED BY: 1. <i>[Signature]</i>	Conditions of bottles or coolers at receipt: ☐ COMPLIANT ☐ NON COMPLIANT ☐ COOLER TEMP 28 °C Comments: <i>[Signature]</i> Page 2 of 2
RELINQUISHED BY SAMPLER: 2. <i>[Signature]</i>	DATE/TIME: 1128 8/7/25	RECEIVED BY: 2. <i>[Signature]</i>	
RELINQUISHED BY SAMPLER: 3. <i>[Signature]</i>	DATE/TIME:	RECEIVED BY: 3. <i>[Signature]</i>	

CLIENT: ☐ Hand Delivered ☒ Other FedEx
Shipment Complete
☐ YES ☐ NO

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q2795	POWE02	Order Date : 8/7/2025 11:57:00 AM	Project Mgr :
Client Name : Kleinfelder		Project Name : Girad School	Report Type : Results+QC
Client Contact : Mark Warchol		Receive DateTime : 8/7/2025 11:28:00 AM	EDD Type : EXCEL NOCLEANUP
Invoice Name : Kleinfelder		Purchase Order :	Hard Copy Date :
Invoice Contact : Mark Warchol			Date Signoff :

LAB ID	CLIENT ID	MATRIX	SAMPLE DATE	SAMPLE TIME	TEST	TEST GROUP	METHOD	FAX DATE	DUE DATES
Q2795-01	COMP-1	Solid	08/06/2025	10:20		VOCMS Group1	8260D		5 Bus. Days
Q2795-02	COMP-2	Solid	08/06/2025	11:25		VOCMS Group1	8260D		5 Bus. Days
Q2795-03	COMP-3	Solid	08/06/2025	12:20		VOCMS Group1	8260D		5 Bus. Days

Relinquished By :

Date / Time :

CP
8/7/25 1240

Received By :

Date / Time :

Sam
8/7/25 12:40 *11-4-6*
F 22

Storage Area : VOA Refridgerator Room