
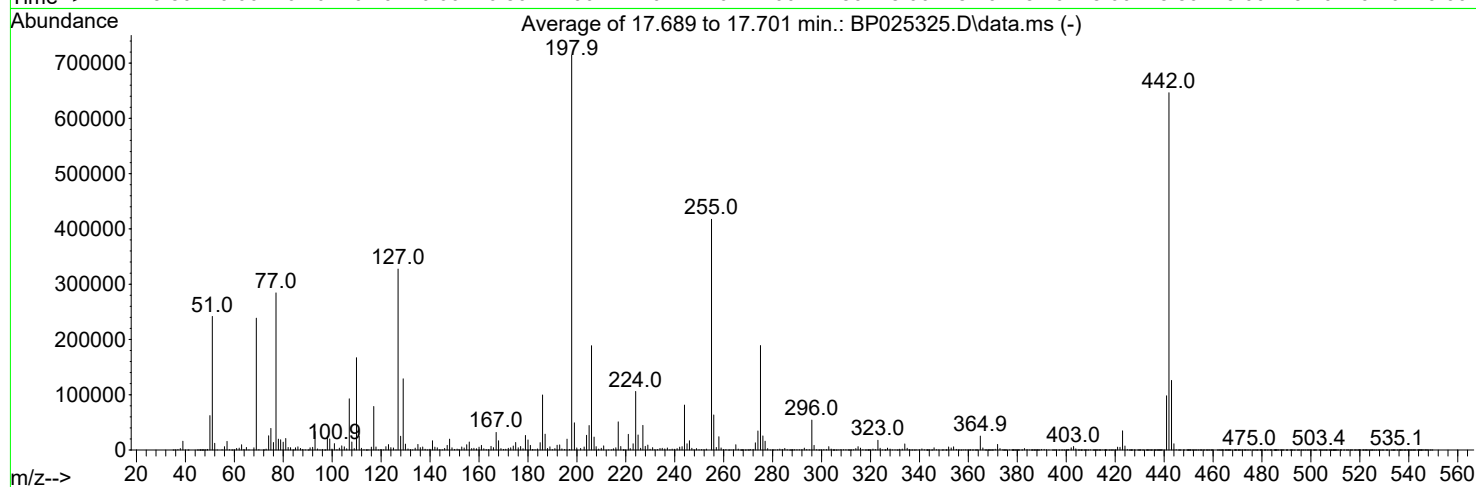


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080825\
Data File : BP025325.D
Acq On : 08 Aug 2025 09:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 06 06:41:44 2025

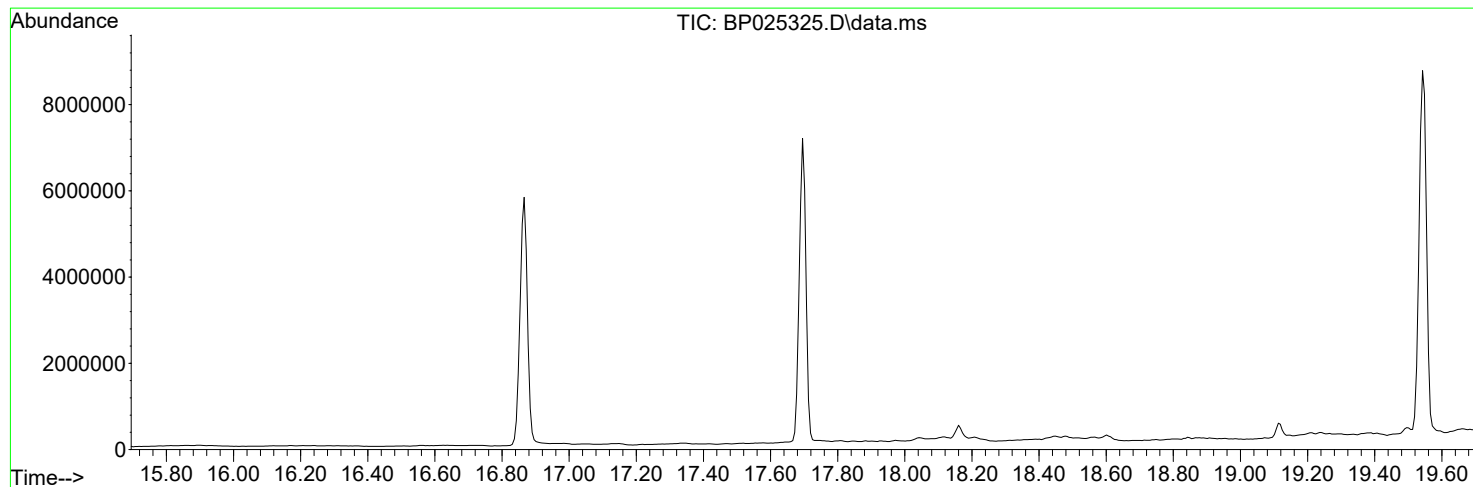

AutoFind: Scans 2508, 2509, 2510; Background Corrected with Scan 2497

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3981	PASS
69	69	100	100	100.0	238631	PASS
70	69	0.00	2	0.3	750	PASS
197	198	0.00	2	0.2	1112	PASS
198	198	100	100	100.0	714318	PASS
199	198	5	9	6.9	49360	PASS
365	198	1	100	3.5	25223	PASS
441	443	0.01	150	78.0	98129	PASS
442	442	100	100	100.0	646400	PASS
443	442	15	24	19.5	125821	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/7/2025	BNA_P	<u>BP025308.D</u>
Compound Name	Response	Retention Time
DDT	2373589	20.836
DDD	55464	20.383
DDE	2522	19.954
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
57986	2431575	2.38

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 07 12:25:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

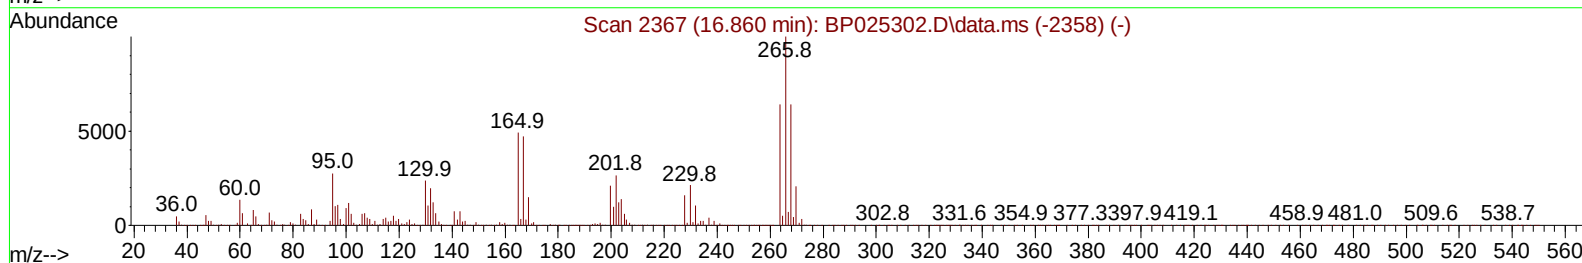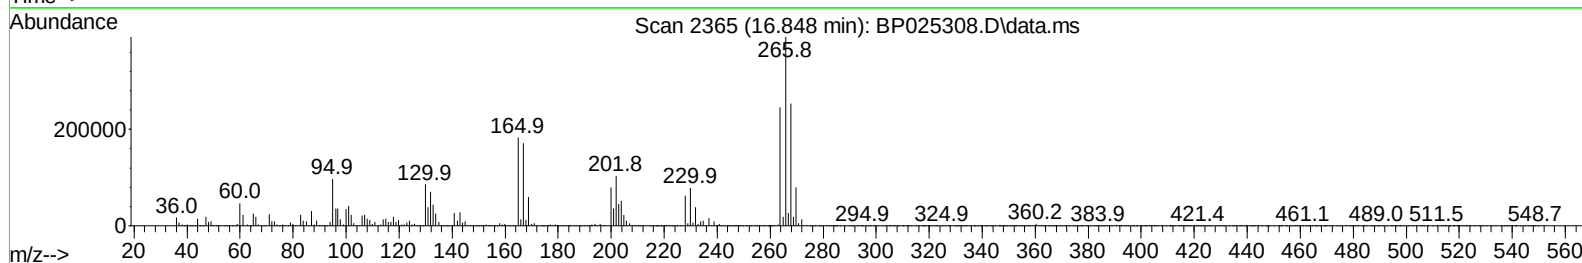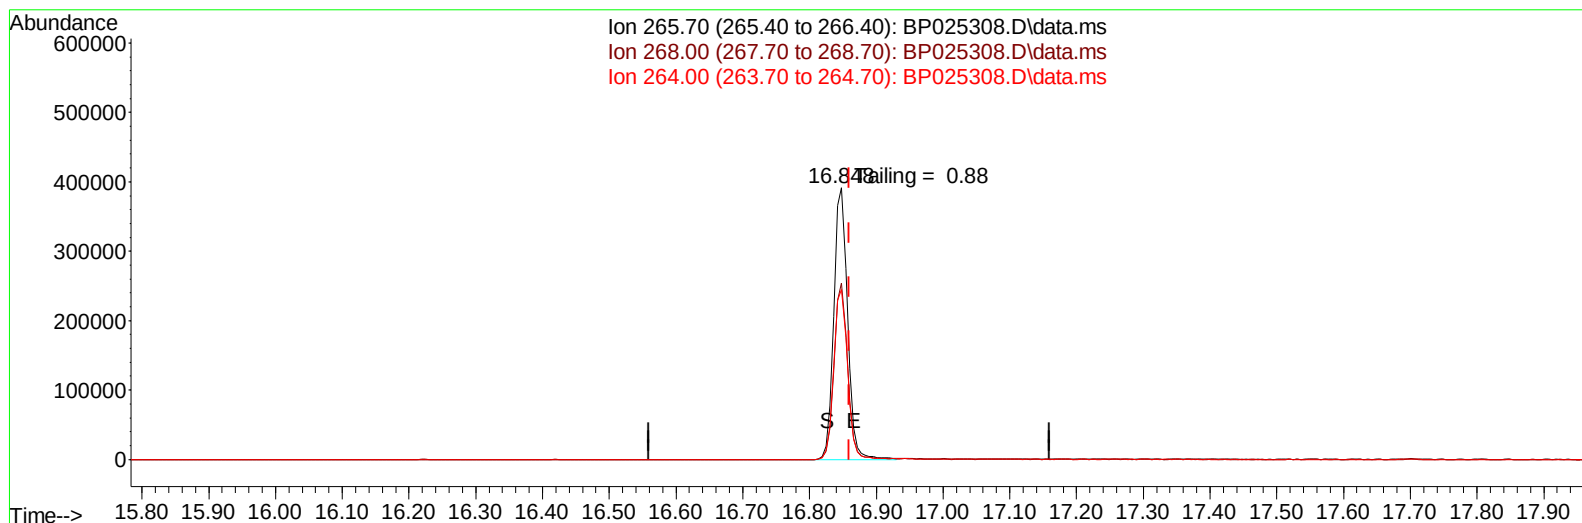

TIC: BP025308.D\data.ms

(70) Pentachlorophenol (C)

16.848min (-0.012) 12862.36 ng




response 556675

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	64.89
264.00	63.90	62.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP080725\
Data File : BP025308.D
Acq On : 07 Aug 2025 11:00
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 07 12:25:20 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

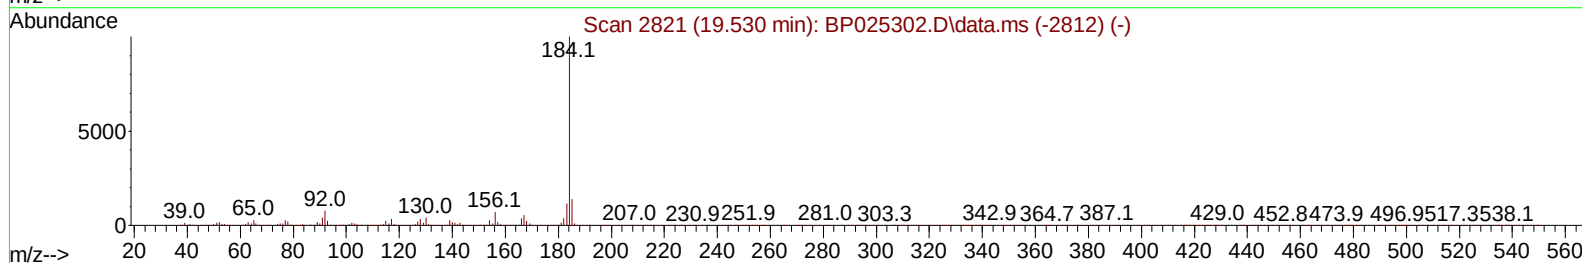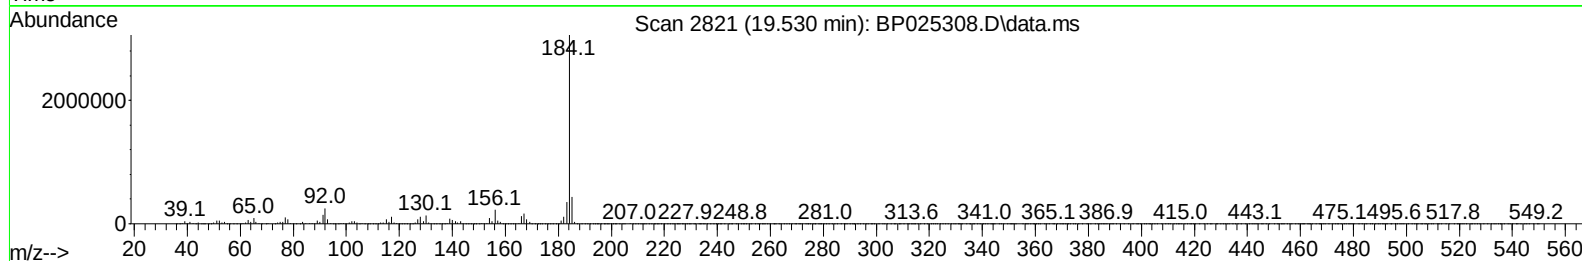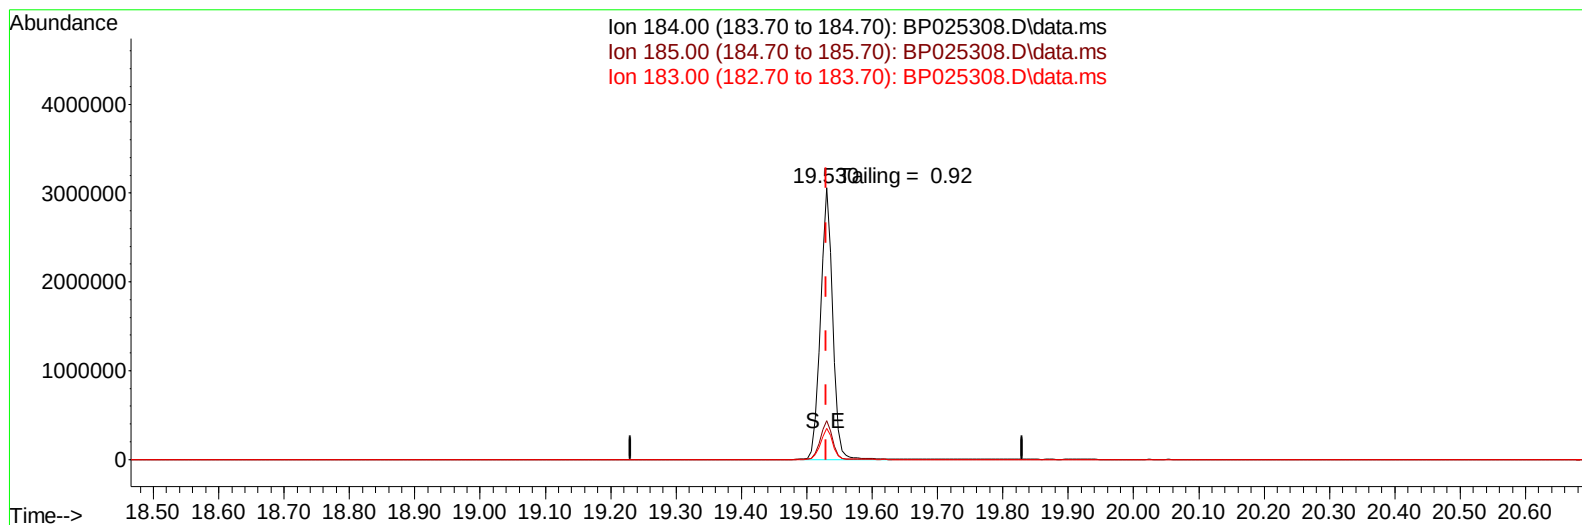

TIC: BP025308.D\data.ms

(77) Benzidine

19.530min (+ 0.000) 8796.27 ng

response 3944680

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.29
183.00	11.50	11.56
0.00	0.00	0.00