
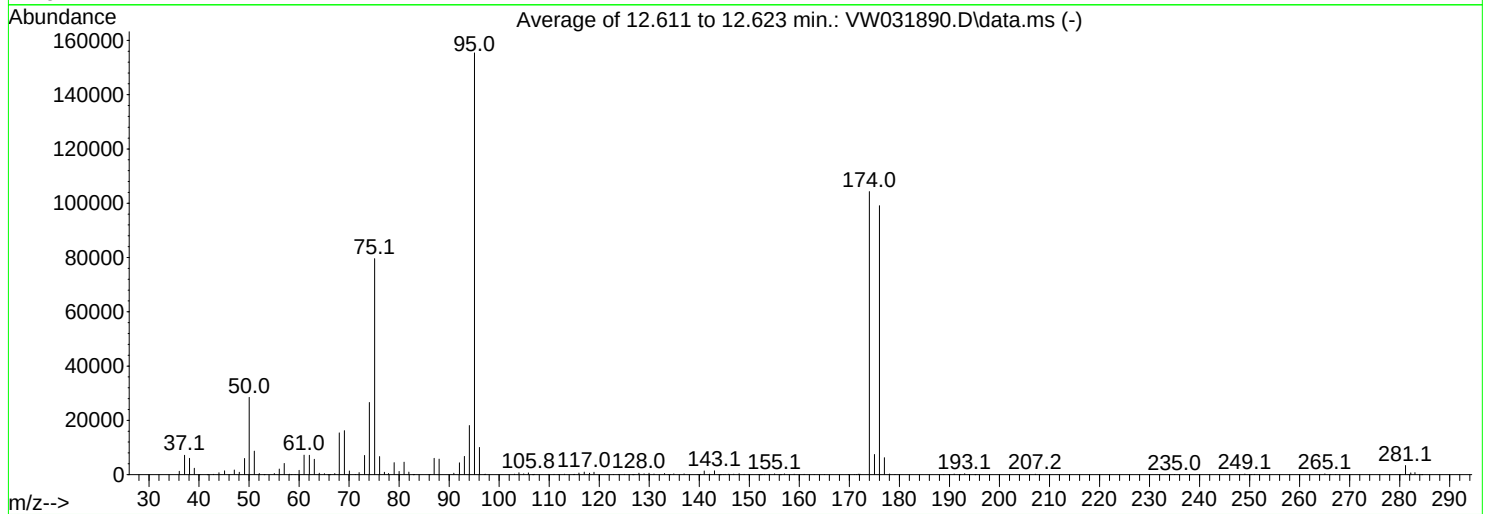


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW072225\
Data File : VW031890.D
Acq On : 22 Jul 2025 08:14
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W072225S.M
Title : SW846 8260
Last Update : Wed Jul 23 08:18:46 2025

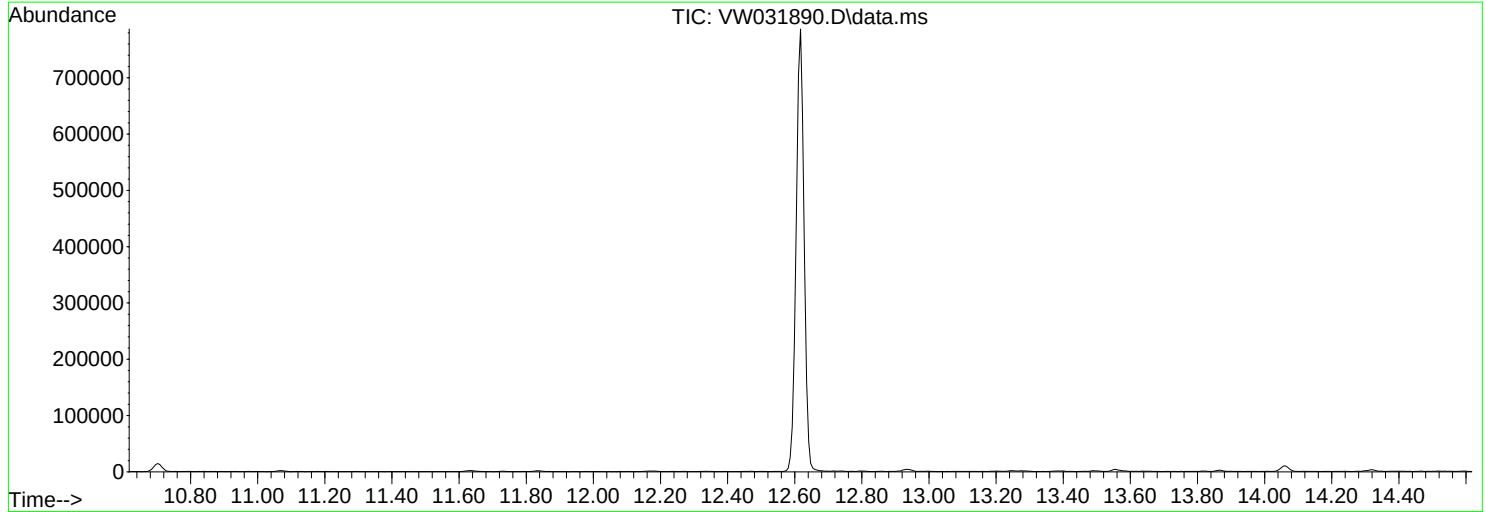

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	28475	PASS
75	95	30	60	51.2	79621	PASS
95	95	100	100	100.0	155413	PASS
96	95	5	9	6.4	10008	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	67.1	104317	PASS
175	174	5	9	7.1	7429	PASS
176	174	95	101	95.0	99120	PASS
177	176	5	9	6.3	6263	PASS