
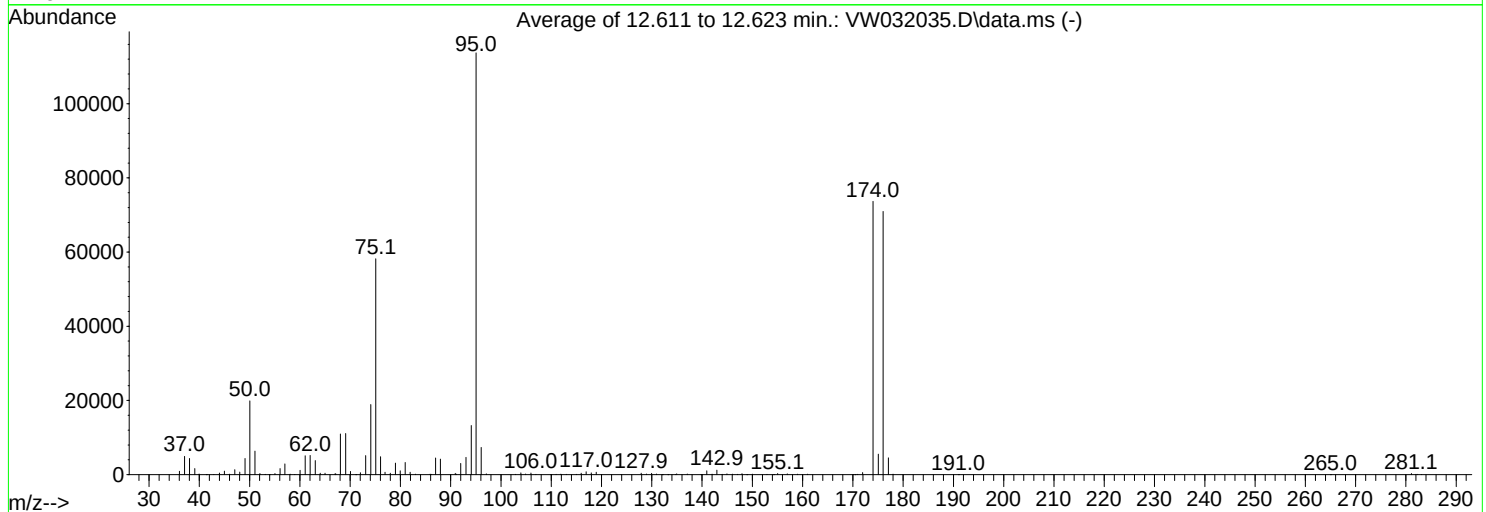


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW080725\
Data File : VW032035.D
Acq On : 07 Aug 2025 08:05
Operator : SY/MD
Sample : BFB
Misc : 5.00g/5mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W072225S.M
Title : SW846 8260
Last Update : Wed Jul 23 08:18:46 2025

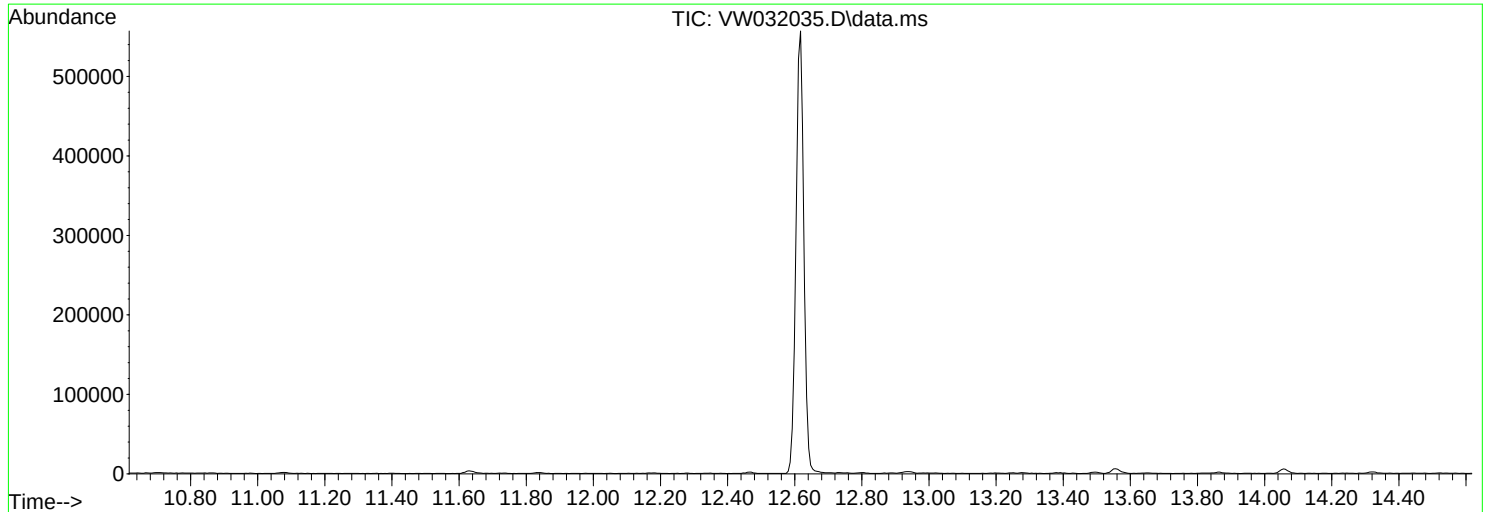

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	19886	PASS
75	95	30	60	51.2	58192	PASS
95	95	100	100	100.0	113712	PASS
96	95	5	9	6.4	7317	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	64.8	73664	PASS
175	174	5	9	7.5	5506	PASS
176	174	95	101	96.3	70952	PASS
177	176	5	9	6.4	4545	PASS