

DATA PACKAGE METALS

PROJECT NAME : NWIRP BETHPAGE 112G08005-WE13

TETRA TECH NUS, INC.

661 Andersen Drive

Suite 200

Pittsburgh, PA - 15220-2745

Phone No: 412-921-7090

ORDER ID : Q2805

ATTENTION : Ernie Wu



Laboratory Certification ID # 20012



1) METALS DATA	2
2) Signature Page	4
3) Case Narrative	5
4) Qualifier Page	6
5) Conformance/Non Conformance	7
6) QA Checklist	8
7) Chronicle	9
8) Hit Summary	10
9) Sample Data	11
9.1) RW8-SP100-20250807	12
9.2) RW8-SP303-20250807	13
10) METALS CALIBRATION DATA	14
10.1) Initial and Continuing Calibration Verification	15
10.2) CRDL Standard For AA & ICP	18
10.3) Initial and Continuing Calibration Blank Summary	19
10.4) Preparation Blank Summary	21
10.5) Interference Check Sample	22
11) METALS QC DATA	23
11.1) Matrix Spike Summary	24
11.2) Post Digest Spike Summary	26
11.3) Duplicate Sample Summary	27
11.4) Laboratory Control Sample Summary	29
11.5) ICP Serial Dilutions	30
12) METALS PREPARATION & INSTRUMENT DATA	31
12.1) ICP Interelement Correction Factors	32
13) PREPARATION & ANALYTICAL SUMMARY	37
13.1) Sample Preparation Summary	38
13.2) Analysis Run Log	39
14) METALS RAW DATA	40
14.1) METALS RAW DATA - ANALYTICAL	41
14.2) LB136779	41
14.3) METALS RAW DATA - PREP	157
14.3.1) PB169154	157
15) Analytical Runlogs	160
16) Standard Prep Logs	163

Table Of Contents for Q2805

17) Shipping Document	318
17.1) Chain Of Custody	319
17.2) Lab Certificate	320

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17

Cover Page

Order ID : Q2805

Project ID : NWIRP Bethpage 112G08005-WE13

Client : Tetra Tech NUS, Inc.

Lab Sample Number

Q2805-01
Q2805-02

Client Sample Number

RW8-SP100-20250807
RW8-SP303-20250807

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature :

APPROVED

By Nimisha Pandya, QA/QC Supervisor at 12:39 pm, Aug 19, 2025

Date: 8/14/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

CASE NARRATIVE

Tetra Tech NUS, Inc.

Project Name: NWIRP Bethpage 112G08005-WE13

Project Manager : Ernie Wu

Order ID # Q2805

Test Name: Metals Group4

A. Number of Samples and Date of Receipt:

1 Water sample was received on 08/08/2025.

B. Parameters:

According to the Chain of Custody document, the following analyses were requested: Metals Group4, SVOC-SIMGroup1, TDS and TSS. This data package contains results for Metals Group4.

C. Analytical Techniques:

The analysis of Metals Group4 was based on method 6010D and digestion based on method 3010 (waters).

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Blank Spike met requirements for all compounds.

The Duplicate analysis met criteria for all compounds.

The Matrix Spike analysis met criteria for all compounds.

The Matrix Spike Duplicate analysis met criteria for all compounds.

The Blank analysis did not indicate the presence of lab contamination.

The Calibration met the requirements.

The Serial Dilution met the acceptable requirements.

E. Additional Comments:

The laboratory certifies that the all-electronic diskette deliverable exactly match the data summary forms (i.e. Form Is).

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

APPROVED

By Nimisha Pandya, QA/QC Supervisor at 12:39 pm, Aug 19, 2025

DATA REPORTING QUALIFIERS- INORGANIC

For reporting results, the following “ Results Qualifiers” are used:

J	Indicates the reported value was obtained from a reading that was less than the Contract Required Detection Limit (CRDL), but greater than or equal to the Instrument Detection Limit (IDL).
U	Indicates the analyte was analyzed for, but not detected.
ND	Indicates the analyte was analyzed for, but not detected
E	Indicates the reported value is estimated because of the presence of interference
M	Indicates Duplicate injection precision not met.
N	Indicates the spiked sample recovery is not within control limits.
S	Indicates the reported value was determined by the Method of Standard Addition (MSA).
*	Indicates that the duplicate analysis is not within control limits.
+	Indicates the correlation coefficient for the MSA is less than 0.995.
D	Indicates the reported value is from a secondary analysis with a dilution factor. The original analysis exceeded the calibration range.
M	Method qualifiers “P” for ICP instrument “PM” for ICP when Microwave Digestion is used “CV” for Manual Cold Vapor AA “AV” for automated Cold Vapor AA “CA” for MIDI-Distillation Spectrophotometric “AS” for Semi -Automated Spectrophotometric “C” for Manual Spectrophotometric “T” for Titrimetric “NR” for analyte not required to be analyzed
OR	Indicates the analyte’s concentration exceeds the calibrated range of the instrument for that specific analysis.
Q	Indicates the LCS did not meet the control limits requirements
H	Sample Analysis Out Of Hold Time

METALS CONFORMANCE/NON-CONFORMANCE SUMMARY

ORDER ID: Q2805

MATRIX: Water

METHOD: 6010D

	NA	NO	YES
1. Calibration Summary met criteria.			✓
2. ICP Interference Check Sample Results Summary Submitted.			✓
3. Serial Dilution Summary (if applicable) Submitted.			✓
4. Laboratory Control Sample Summary (if applicable) Submitted.			✓
5. Blank Contamination - If yes, list compounds and concentrations in each blank:		✓	
6. Matrix Spike/Matrix Spike Duplicate Recoveries Met Criteria If not met, list those compounds and their recoveries which fall outside the acceptable range.			✓
7. Sample Duplicate Analysis Met QC Criteria If not met, list those compounds and their recoveries which fall outside the acceptable range.			✓
8. Digestion Holding Time Met If not met, list number of days exceeded for each sample:			✓
9. Analysis Holding Time Met If not met, list those compounds and their recoveries which fall outside the acceptable range.			✓

ADDITIONAL COMMENTS:

The laboratory certifies that the all-electronic diskette deliverable exactly match the data summary forms (i.e. Form Is).

QA REVIEW

REVIEWED

Sohil Jodhani, QA/QC Director , 8/19/2025, 10:30:48 AM

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2805

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication,airbill, sample management lab chronicle, login page)

✓

Check chain-of-custody for proper relinquish/return of samples

✓

Is the chain of custody signed and complete

✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts

✓

Collect information for each project id from server. Were all requirements followed

✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page

✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody

✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results

✓

Do requested analyses on Chain of Custody agree with the log-in page

✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Custody

✓

Were the samples received within hold time

✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle

✓

ANALYTICAL:

Was method requirement followed?

✓

Was client requirement followed?

✓

Does the case narrative summarize all QC failure?

✓

All runlogs and manual integration are reviewed for requirements

✓

All manual calculations and /or hand notations verified

✓

QA Review Signature: SOHIL JODHANI

Date: 08/14/2025

LAB CHRONICLE

OrderID:	Q2805	OrderDate:	8/8/2025 9:48:00 AM
Client:	Tetra Tech NUS, Inc.	Project:	NWIRP Bethpage 112G08005-WE13
Contact:	Ernie Wu	Location:	J22

LabID	ClientID	Matrix	Test	Method	Sample Date	Prep Date	Anal Date	Received
Q2805-01	RW8-SP100-2025080 7	Water			08/07/25			08/08/25
			Metals Group4	6010D		08/08/25	08/11/25	
Q2805-02	RW8-SP303-2025080 7	Water			08/07/25			08/08/25
			Metals Group4	6010D		08/08/25	08/11/25	

Hit Summary Sheet
SW-846

SDG No.:	Q2805	Order ID:	Q2805
Client:	Tetra Tech NUS, Inc.	Project ID:	NWIRP Bethpage 112G08005-WE13

Sample ID	Client ID	Matrix	Parameter	Concentration	C	MDL	LOD	RDL	Units
Client ID : RW8-SP100-20250807									
Q2805-01	RW8-SP100-20250807	Water	Iron	599		11.7	40.0	50.0	ug/L
Client ID : RW8-SP303-20250807									
Q2805-02	RW8-SP303-20250807	Water	Iron	33.3	J	11.7	40.0	50.0	ug/L



SAMPLE DATA

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Report of Analysis

Client:	Tetra Tech NUS, Inc.	Date Collected:	08/07/25
Project:	NWIRP Bethpage 112G08005-WE13	Date Received:	08/08/25
Client Sample ID:	RW8-SP100-20250807	SDG No.:	Q2805
Lab Sample ID:	Q2805-01	Matrix:	Water
Level (low/med):	low	% Solid:	0

Cas	Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.	Prep Met.
7439-89-6	Iron	599		1	11.7	40.0	50.0	ug/L	08/08/25 11:10	08/11/25 18:05	6010D	SW3010

Color Before:	Colorless	Clarity Before:	Clear	Texture:
Color After:	Colorless	Clarity After:	Clear	Artifacts:
Comments:	Metals Group4			

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 D = Dilution
 Q = indicates LCS control criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 * = indicates the duplicate analysis is not within control limits.
 E = Indicates the reported value is estimated because of the presence of interference.
 OR = Over Range
 N =Spiked sample recovery not within control limits

Report of Analysis

Client:	Tetra Tech NUS, Inc.	Date Collected:	08/07/25
Project:	NWIRP Bethpage 112G08005-WE13	Date Received:	08/08/25
Client Sample ID:	RW8-SP303-20250807	SDG No.:	Q2805
Lab Sample ID:	Q2805-02	Matrix:	Water
Level (low/med):	low	% Solid:	0

Cas	Parameter	Conc.	Qua.	DF	MDL	LOD	LOQ / CRQL	Units	Prep Date	Date Ana.	Ana Met.	Prep Met.
7439-89-6	Iron	33.3	J	1	11.7	40.0	50.0	ug/L	08/08/25 11:10	08/11/25 18:09	6010D	SW3010

Color Before:	Colorless	Clarity Before:	Clear	Texture:
Color After:	Colorless	Clarity After:	Clear	Artifacts:
Comments:	Metals Group4			

U = Not Detected
 LOQ = Limit of Quantitation
 MDL = Method Detection Limit
 LOD = Limit of Detection
 D = Dilution
 Q = indicates LCS control criteria did not meet requirements

J = Estimated Value
 B = Analyte Found in Associated Method Blank
 * = indicates the duplicate analysis is not within control limits.
 E = Indicates the reported value is estimated because of the presence of interference.
 OR = Over Range
 N =Spiked sample recovery not within control limits



METAL CALIBRATION DATA

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Metals

- 2a -

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Initial Calibration Source: EPA

Continuing Calibration Source: Inorganic Ventures

Sample ID	Analyte	Result ug/L	True Value	% Recovery	Acceptance Window (%R)	M	Analysis Date	Analysis Time	Run Number
ICV01	Iron	3930	4000	98	90 - 110	P	08/11/2025	16:44	LB136779

Metals

- 2a -

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Client: Tetra Tech NUS, Inc.
Contract: TETR06
Initial Calibration Source: EPA
Continuing Calibration Source: Inorganic Ventures

SDG No.: Q2805
Lab Code: ACE

Sample ID	Analyte	Result ug/L	True Value	% Recovery	Acceptance Window (%R)	M	Analysis Date	Analysis Time	Run Number
LLICV01	Iron	84.3	100	84	80 - 120	P	08/11/2025	16:49	LB136779

Metals

- 2a -

INITIAL AND CONTINUING CALIBRATION VERIFICATION

Client:	<u>Tetra Tech NUS, Inc.</u>	SDG No.:	<u>Q2805</u>
Contract:	<u>TETR06</u>	Lab Code:	<u>ACE</u>
Initial Calibration Source:	<u>EPA</u>		
Continuing Calibration Source:	<u>Inorganic Ventures</u>		

Sample ID	Analyte	Result ug/L	True Value	% Recovery	Acceptance Window (%R)	M	Analysis Date	Analysis Time	Run Number
CCV01	Iron	4850	5000	97	90 - 110	P	08/11/2025	17:19	LB136779
CCV02	Iron	4960	5000	99	90 - 110	P	08/11/2025	17:44	LB136779
CCV03	Iron	4910	5000	98	90 - 110	P	08/11/2025	18:26	LB136779
CCV04	Iron	4970	5000	99	90 - 110	P	08/11/2025	18:59	LB136779



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Metals

- 2b -

CRDL STANDARD FOR AA & ICP

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Initial Calibration Source: _____

Continuing Calibration Source: _____

Sample ID	Analyte	Result ug/L	True Value ug/L	% Recovery	Acceptance Window (%R)	M	Analysis Date	Analysis Time	Run Number
CRI01	Iron	83.7	100	84	65 - 135	P	08/11/2025	16:58	LB136779



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Metals

- 3a -

INITIAL AND CONTINUING CALIBRATION BLANK SUMMARY

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Sample ID	Analyte	Result ug/L	Acceptance Limit	Conc Qual	LOD	CRQL	M	Analysis Date	Analysis Time	Run Number
ICB01	Iron	23.4	+/-50	U	80.0	100	P	08/11/2025	16:54	LB136779

Metals

- 3a -

INITIAL AND CONTINUING CALIBRATION BLANK SUMMARY

Client: Tetra Tech NUS, Inc. **SDG No.:** Q2805
Contract: TETR06 **Lab Code:** ACE

Sample ID	Analyte	Result ug/L	Acceptance Limit	Conc Qual	LOD	CRQL	M	Analysis Date	Analysis Time	Run Number
CCB01	Iron	23.4	+/-50	U	80.0	100	P	08/11/2025	17:23	LB136779
CCB02	Iron	23.4	+/-50	U	80.0	100	P	08/11/2025	17:48	LB136779
CCB03	Iron	23.4	+/-50	U	80.0	100	P	08/11/2025	18:30	LB136779
CCB04	Iron	23.4	+/-50	U	80.0	100	P	08/11/2025	19:03	LB136779

Metals
- 3b -
PREPARATION BLANK SUMMARY

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Instrument: P4

Sample ID	Analyte	Result (ug/L)	Acceptance Limit	Conc Qual	LOD ug/L	CRQL ug/L	M	Analysis Date	Analysis Time	Run
PB169154BL		WATER		Batch Number:		PB169154		Prep Date:	08/08/2025	
	Iron	11.7	<25	U	40.0	50.0	P	08/11/2025	17:52	LB136779

Metals
- 4 -
INTERFERENCE CHECK SAMPLE

Client: Tetra Tech NUS, Inc. **SDG No.:** Q2805
Contract: TETR06 **Lab Code:** ACE
ICS Source: EPA **Instrument ID:** P4

Sample ID	Analyte	Result ug/L	True Value ug/L	% Recovery	Low Limit (ug/L)	High Limit (ug/L)	Analysis Date	Analysis Time	Run Number
ICSA01	Iron	97400	101000	96	85600	116500	08/11/2025	17:02	LB136779
ICSAB01	Iron	97900	99300	99	84400	114500	08/11/2025	17:06	LB136779



METAL QC DATA

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

metals
- 5a -
MATRIX SPIKE SUMMARY

client: <u>Tetra Tech NUS, Inc.</u>	level: <u>low</u>	sdg no.: <u>Q2805</u>
contract: <u>TETR06</u>		lab code: <u>ACE</u>
matrix: <u>Water</u>	sample id: <u>Q2805-02</u>	client id: <u>RW8-SP303-20250807MS</u>
Percent Solids for Sample: <u>NA</u>	Spiked ID: <u>Q2805-02MS</u>	Percent Solids for Spike Sample: <u>NA</u>

Analyte	Units	Acceptance Limit %R	Spiked Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M
Iron	ug/L	87 - 115	1540		33.3	J	1500	100		P

metals
- 5a -
MATRIX SPIKE DUPLICATE SUMMARY

client:	Tetra Tech NUS, Inc.		level:	low		sdg no.:	Q2805				
contract:	TETR06					lab code:	ACE				
matrix:	Water		sample id:	Q2805-02		client id:	RW8-SP303-20250807MSD				
Percent Solids for Sample:		NA		Spiked ID:		Q2805-02MSD		Percent Solids for Spike Sample:		NA	
Analyte	Units	Acceptance Limit %R	MSD Result	C	Sample Result	C	Spike Added	% Recovery	Qual	M	
Iron	ug/L	87 - 115	1510		33.3	J	1500	98		P	



- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11**
- 12
- 13
- 14
- 15
- 16
- 17

Sample ID: _____ **Spiked ID:** _____

Metals

- 6 -

DUPLICATE SAMPLE SUMMARY

Client:	<u>Tetra Tech NUS, Inc.</u>	Level:	<u>LOW</u>	SDG No.:	<u>Q2805</u>
Contract:	<u>TETR06</u>			Lab Code:	<u>ACE</u>
Matrix:	<u>Water</u>	Sample ID:	<u>Q2805-02</u>	Client ID:	<u>RW8-SP303-20250807DUP</u>
Percent Solids for Sample:	NA	Duplicate ID	Q2805-02DUP	Percent Solids for Spike Sample:	NA

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Iron	ug/L	20	33.3	J	34.9	J	5		P

“A control limit of $\pm 20\%$ RPD for each matrix applies for sample values greater than 10 times Detection Limit”

Metals

- 6 -

DUPLICATE SAMPLE SUMMARY

Client:	<u>Tetra Tech NUS, Inc.</u>	Level:	<u>LOW</u>	SDG No.:	<u>Q2805</u>
Contract:	<u>TETR06</u>			Lab Code:	<u>ACE</u>
Matrix:	<u>Water</u>	Sample ID:	<u>Q2805-02MS</u>	Client ID:	<u>RW8-SP303-20250807MSD</u>
Percent Solids for Sample:	NA	Duplicate ID	Q2805-02MSD	Percent Solids for Spike Sample:	NA

Analyte	Units	Acceptance Limit	Sample Result	C	Duplicate Result	C	RPD	Qual	M
Iron	ug/L	20	1540		1510		2		P

“A control limit of $\pm 20\%$ RPD for each matrix applies for sample values greater than 10 times Detection Limit”

Metals

- 7 -

LABORATORY CONTROL SAMPLE SUMMARY

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Analyte	Units	True Value	Result	C	% Recovery	Acceptance Limits	M
PB169154BS Iron	ug/L	1500	1500		100	87 - 115	P

Metals
-9 -
ICP SERIAL DILUTIONS

SAMPLE NO.

RW8-SP303-20250807L

Lab Name: Alliance **Contract:** TETR06
Lab Code: ACE **Lb No.:** lb136779 **Lab Sample ID :** Q2805-02L **SDG No.:** Q2805
Matrix (soil/water): Water **Level (low/med):** LOW
Concentration Units: ug/L

Analyte	Initial Sample Result (I)		Serial Dilution Result (S)		% Differ- ence	Q	M
Iron	33.3	J	250	U	100.0		P



METAL PREPARATION & INSTRUMENT DATA

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17

Metals

- 11 -

ICP INTERELEMENT CORRECTION FACTORS

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Instrument ID:

Date:

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Analyte	Wave- Length (nm)	ICP Interelement Correction Factors For:				
		Al	Ca	Fe	Mg	Ag
Iron	240.488	0.0000000	0.0000000	0.0000000	0.0000000	0.0000000

Metals

- 11 -

ICP INTERELEMENT CORRECTION FACTORS

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Instrument ID:

Date:

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Analyte	Wave- Length (nm)	ICP Interelement Correction Factors For:				
		As	Ba	Be	Cd	Co
Iron	240.488	0.0000000	0.0000000	0.0000000	0.0000000	-0.0039600

Metals

- 11 -

ICP INTERELEMENT CORRECTION FACTORS

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Instrument ID:

Date:

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Analyte	Wave- Length (nm)	ICP Interelement Correction Factors For:				
		Cr	Cu	K	Mn	Mo
Iron	240.488	0.0000000	0.0000000	0.0000730	0.0000000	-0.0015250

Metals

- 11 -

ICP INTERELEMENT CORRECTION FACTORS

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Instrument ID:

Date:

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Analyte	Wave- Length (nm)	ICP Interement Correction Factors For:				
		Na	Ni	Pb	Sb	Se
Iron	240.488	0.0000000	-0.0017000	0.0000000	0.0000000	0.0000000

Metals

- 11 -

ICP INTERELEMENT CORRECTION FACTORS

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Instrument ID:

Date:

Interelement Correction Factors (apparent ppb analyte/ppm interferent)

Analyte	Wave- Length (nm)	ICP Interement Correction Factors For:				
		Sn	Ti	Tl	V	Zn
Iron	240.488	0.0000000	0.0000000	0.0000000	0.0000000	0.0000000

METAL PREPARATION & ANALYICAL SUMMARY

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17

Metals
- 13 -

SAMPLE PREPARATION SUMMARY

Client: Tetra Tech NUS, Inc.

SDG No.: Q2805

Contract: TETR06

Lab Code: ACE

Method: _____

Sample ID	Client ID	Sample Type	Matrix	Prep Date	Initial Sample Size(mL)	Final Sample Volume (mL)	Percent Solids
Batch Number: PB169154							
PB169154BL	PB169154BL	MB	WATER	08/08/2025	50.0	25.0	
PB169154BS	PB169154BS	LCS	WATER	08/08/2025	50.0	25.0	
Q2805-01	RW8-SP100-20250807	SAM	WATER	08/08/2025	50.0	25.0	
Q2805-02	RW8-SP303-20250807	SAM	WATER	08/08/2025	50.0	25.0	
Q2805-02DUP	RW8-SP303-20250807DUP	DUP	WATER	08/08/2025	50.0	25.0	
Q2805-02MS	RW8-SP303-20250807MS	MS	WATER	08/08/2025	50.0	25.0	
Q2805-02MSD	RW8-SP303-20250807MSD	MSD	WATER	08/08/2025	50.0	25.0	

metals
- 14 -
ANALYSIS RUN LOG

Client: Tetra Tech NUS, Inc.

Contract: TETR06

Lab code: ACE

Sdg no.: Q2805

Instrument id number: _____

Method: _____

Run number: LB136779

Start date: 08/11/2025


End date: 08/11/2025


Lab sample id.	Client Sample Id	d/f	Time	Parameter list
S0	S0	1	1619	Fe
S1	S1	1	1623	Fe
S2	S2	1	1627	Fe
S3	S3	1	1631	Fe
S4	S4	1	1636	Fe
S5	S5	1	1640	Fe
ICV01	ICV01	1	1644	Fe
LLICV01	LLICV01	1	1649	Fe
ICB01	ICB01	1	1654	Fe
CRI01	CRI01	1	1658	Fe
ICSA01	ICSA01	1	1702	Fe
ICSAB01	ICSAB01	1	1706	Fe
CCV01	CCV01	1	1719	Fe
CCB01	CCB01	1	1723	Fe
CCV02	CCV02	1	1744	Fe
CCB02	CCB02	1	1748	Fe
PB169154BL	PB169154BL	1	1752	Fe
PB169154BS	PB169154BS	1	1757	Fe
Q2805-01	RW8-SP100-20250807	1	1805	Fe
Q2805-02	RW8-SP303-20250807	1	1809	Fe
Q2805-02DUP	RW8-SP303-20250807DUP	1	1814	Fe
Q2805-02L	RW8-SP303-20250807L	5	1818	Fe
Q2805-02MS	RW8-SP303-20250807MS	1	1822	Fe
CCV03	CCV03	1	1826	Fe
CCB03	CCB03	1	1830	Fe
Q2805-02MSD	RW8-SP303-20250807MSD	1	1835	Fe
CCV04	CCV04	1	1859	Fe
CCB04	CCB04	1	1903	Fe





METAL RAW DATA


- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

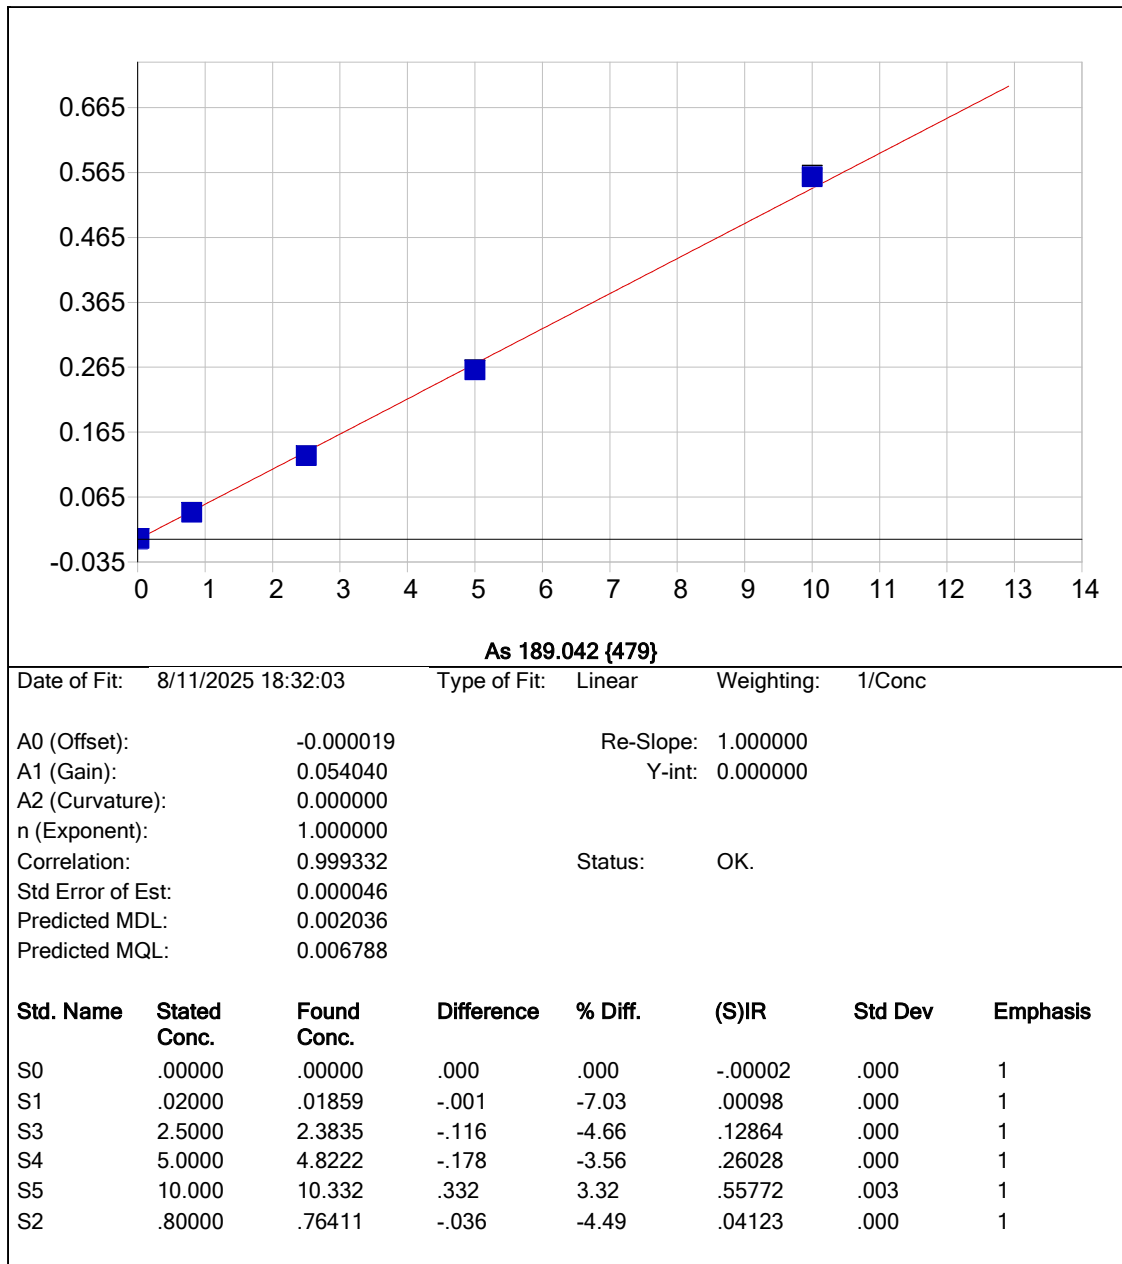


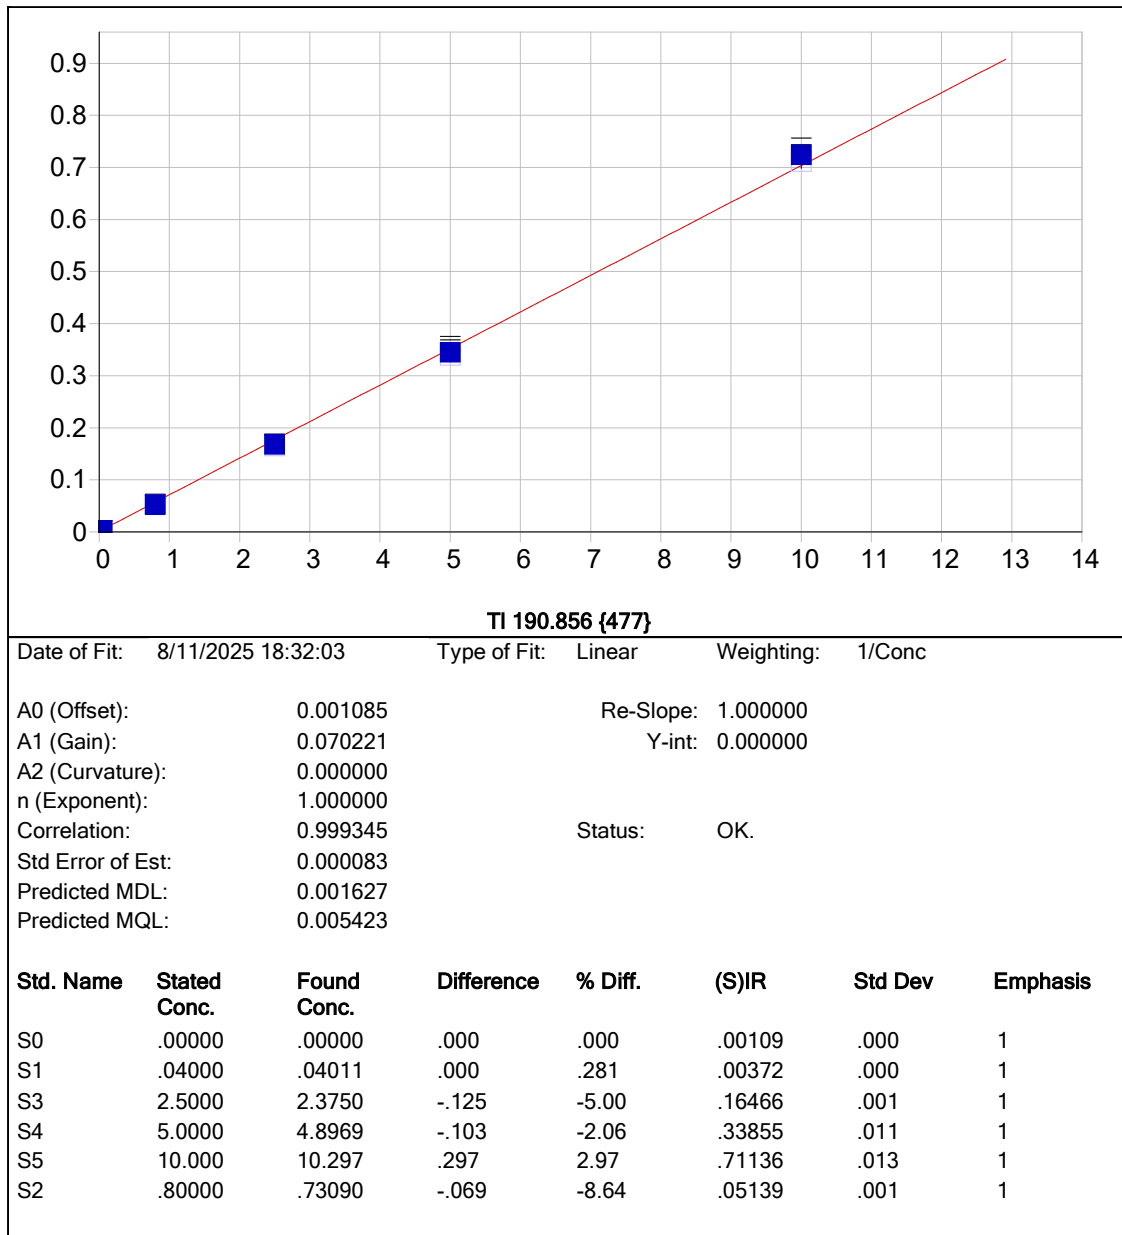


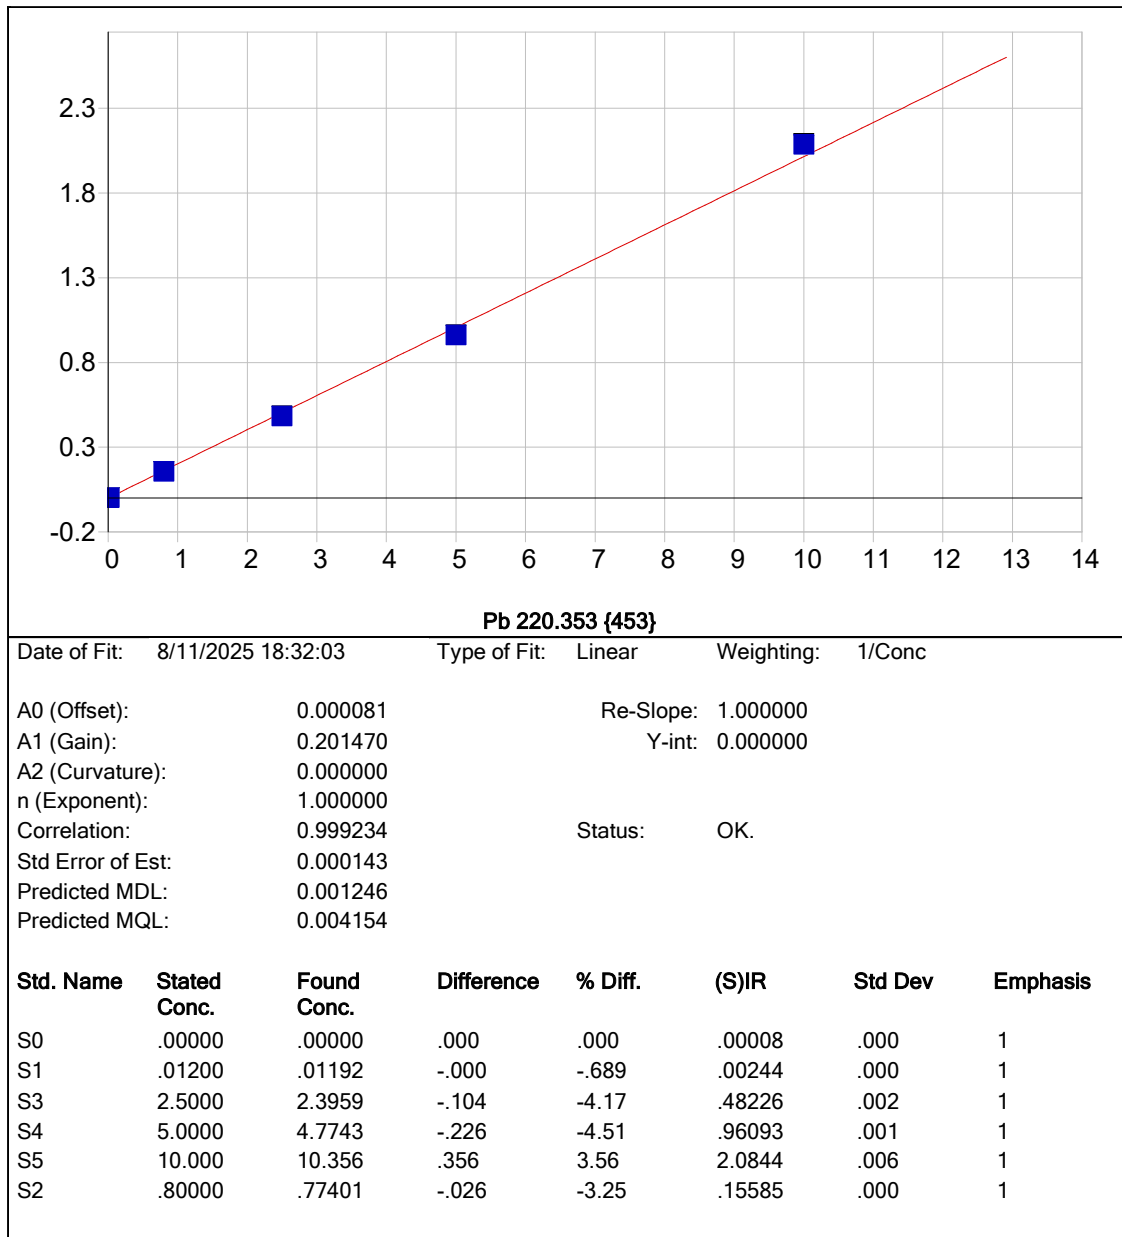


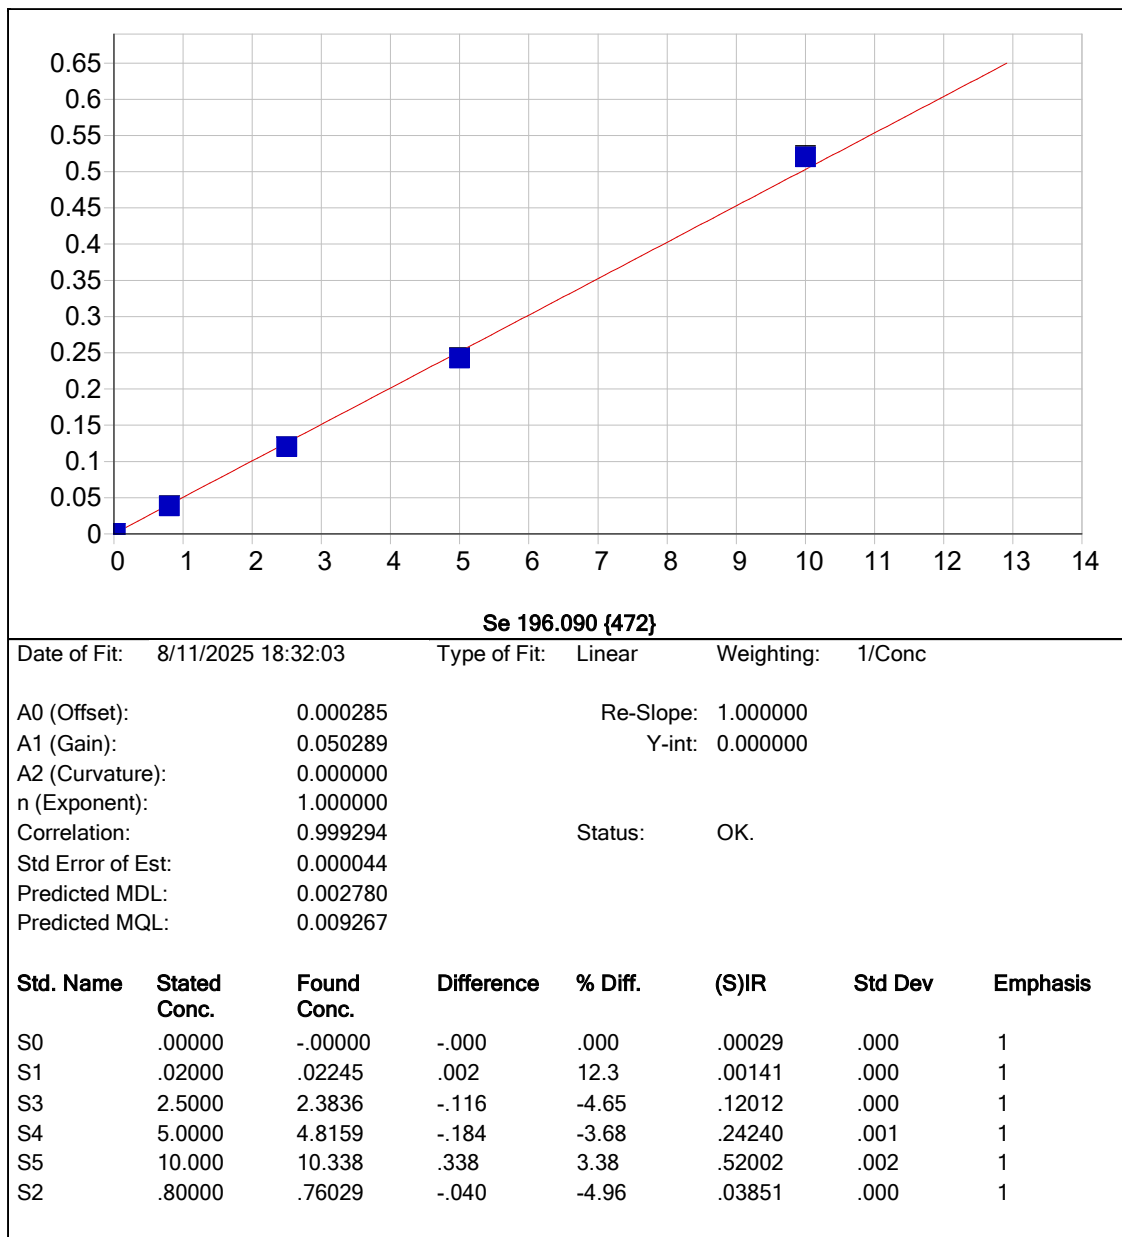


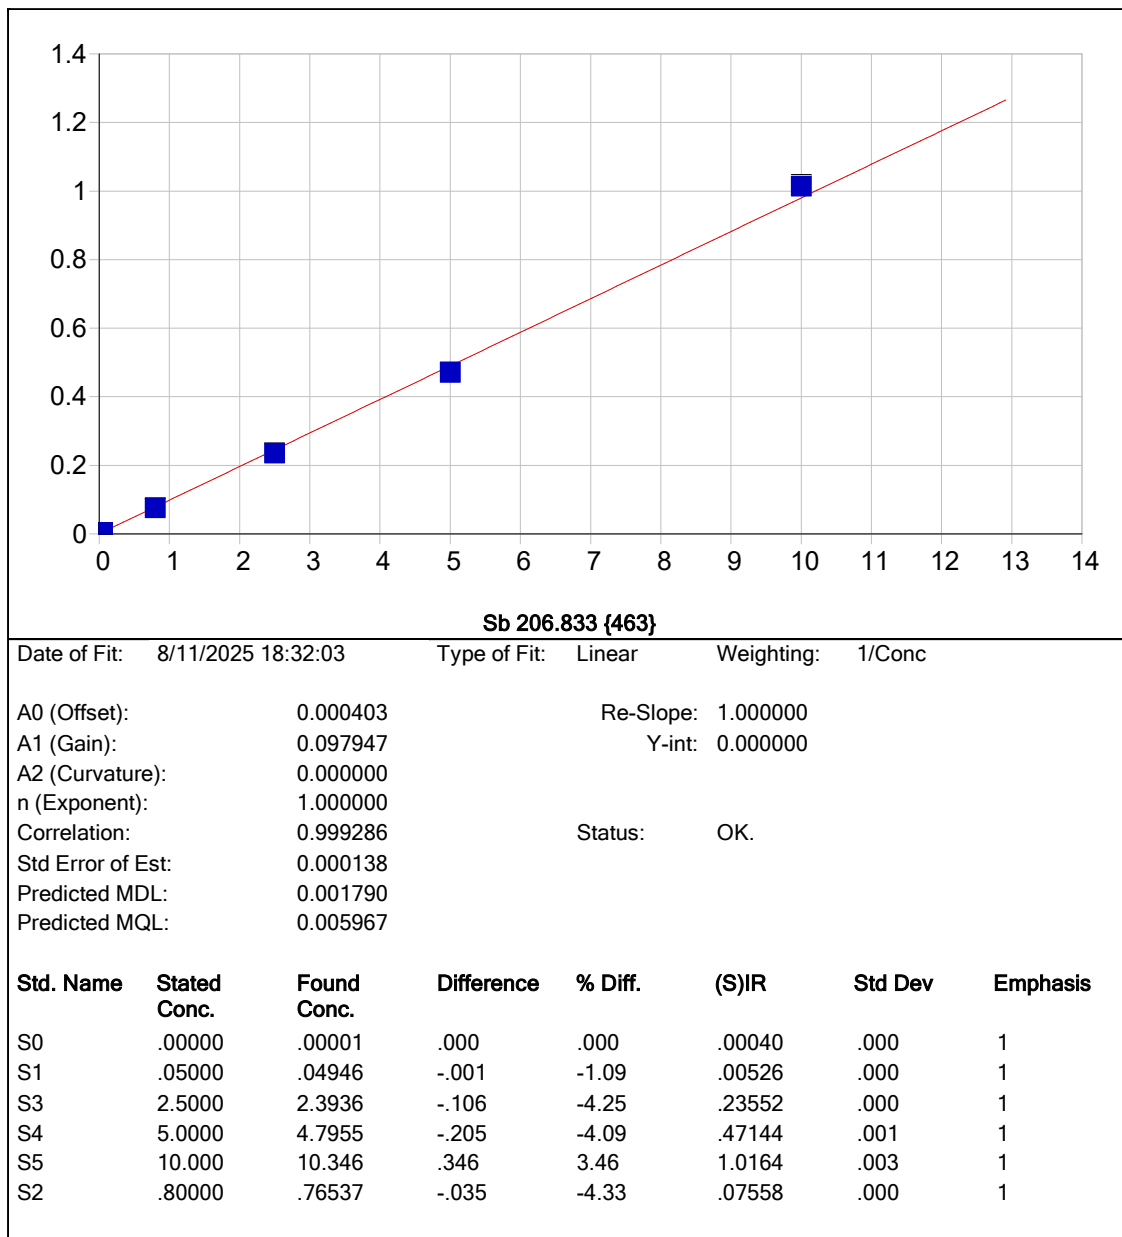

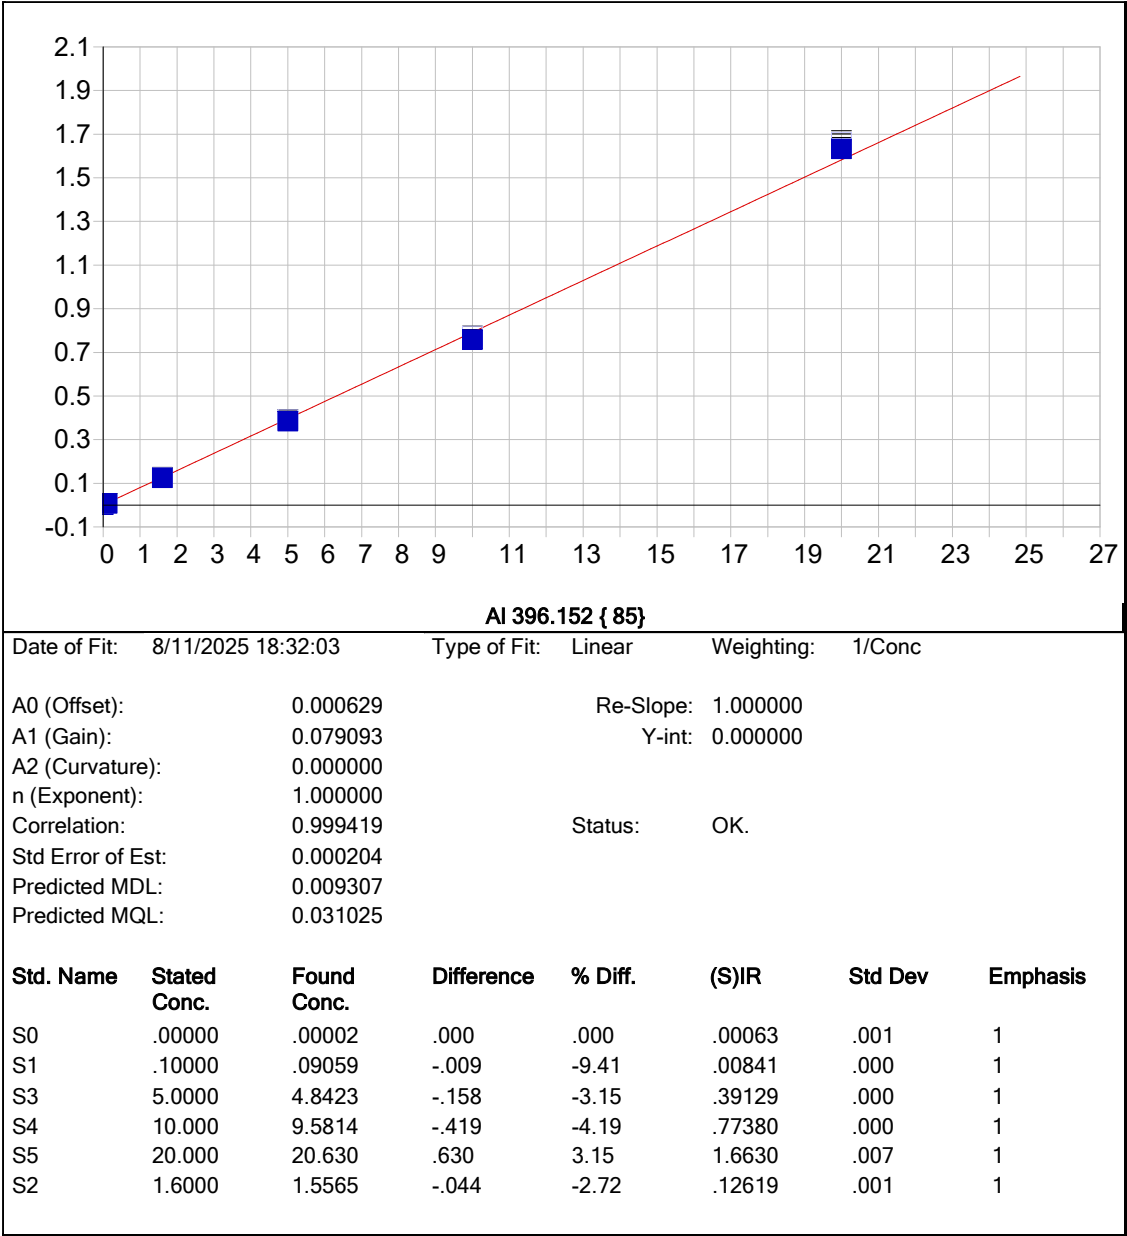


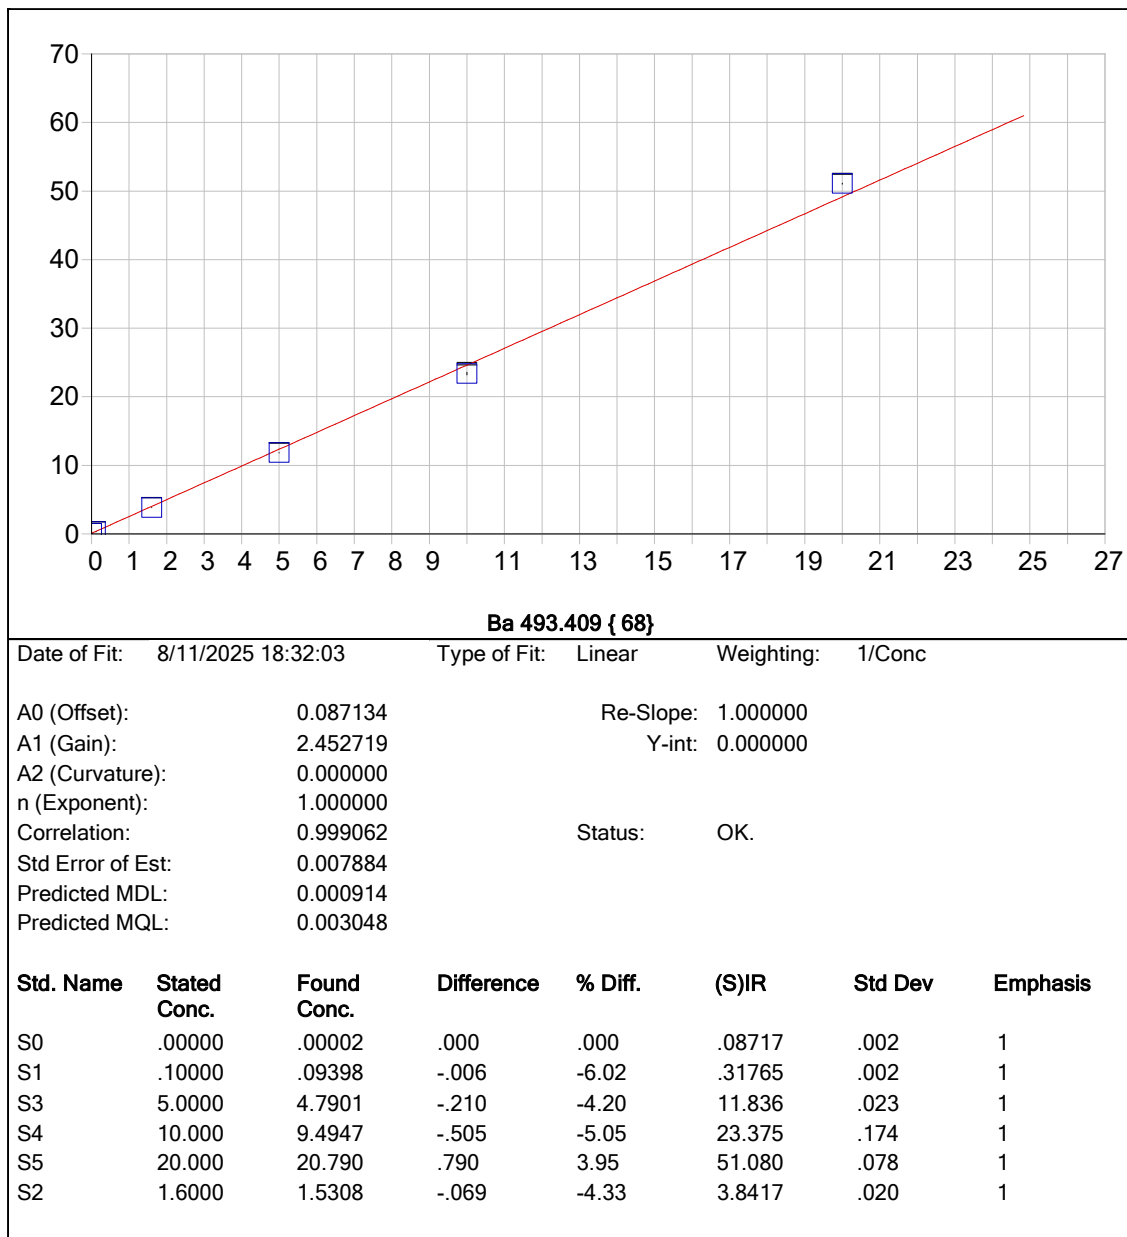


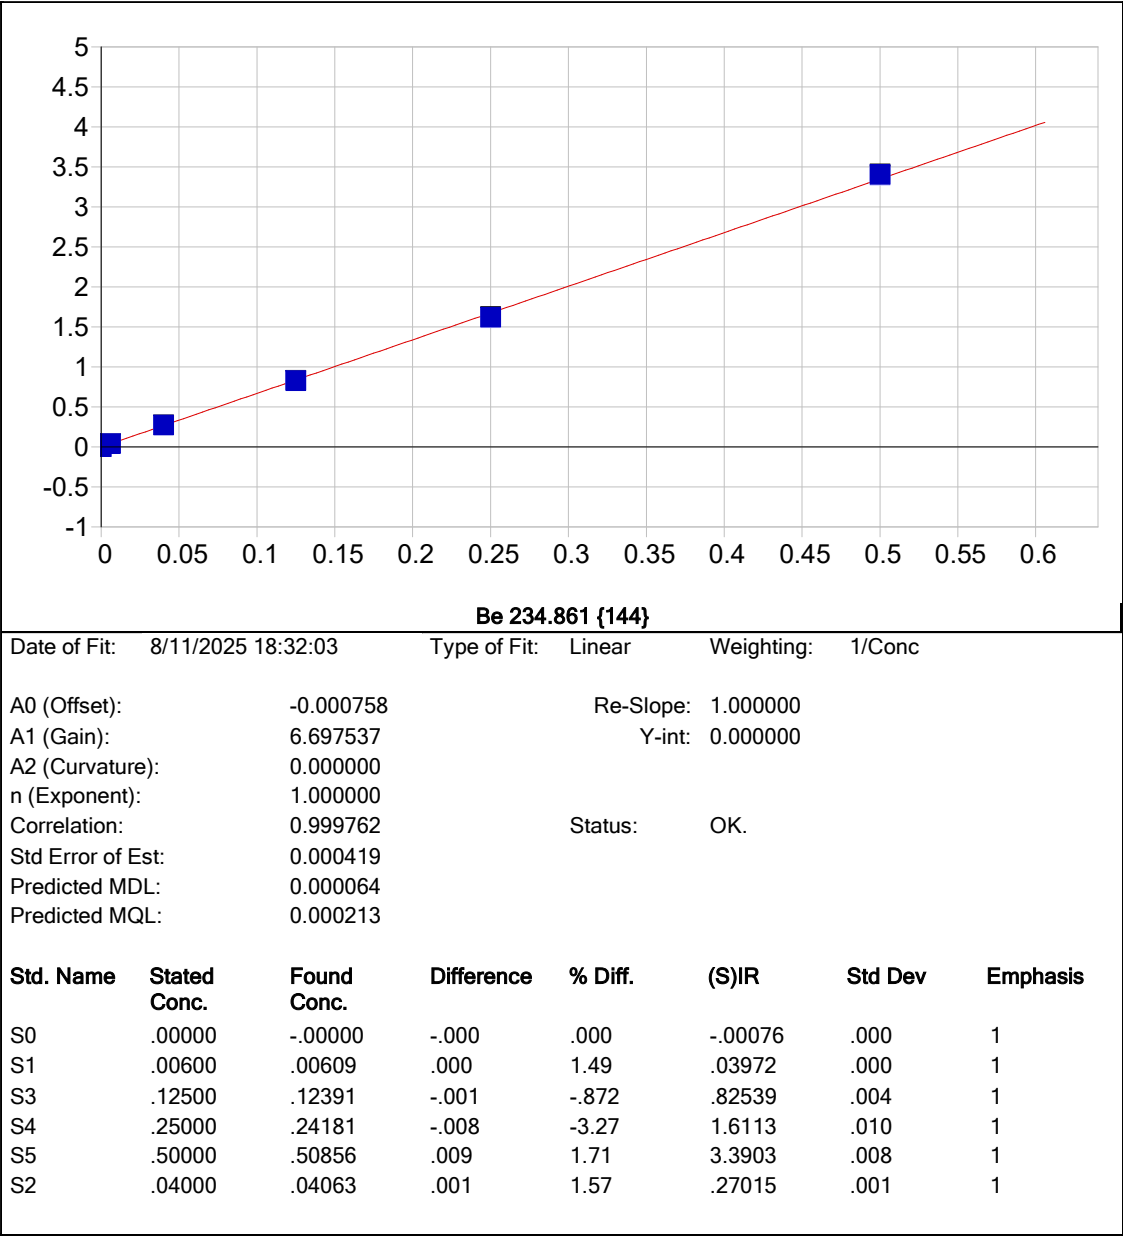


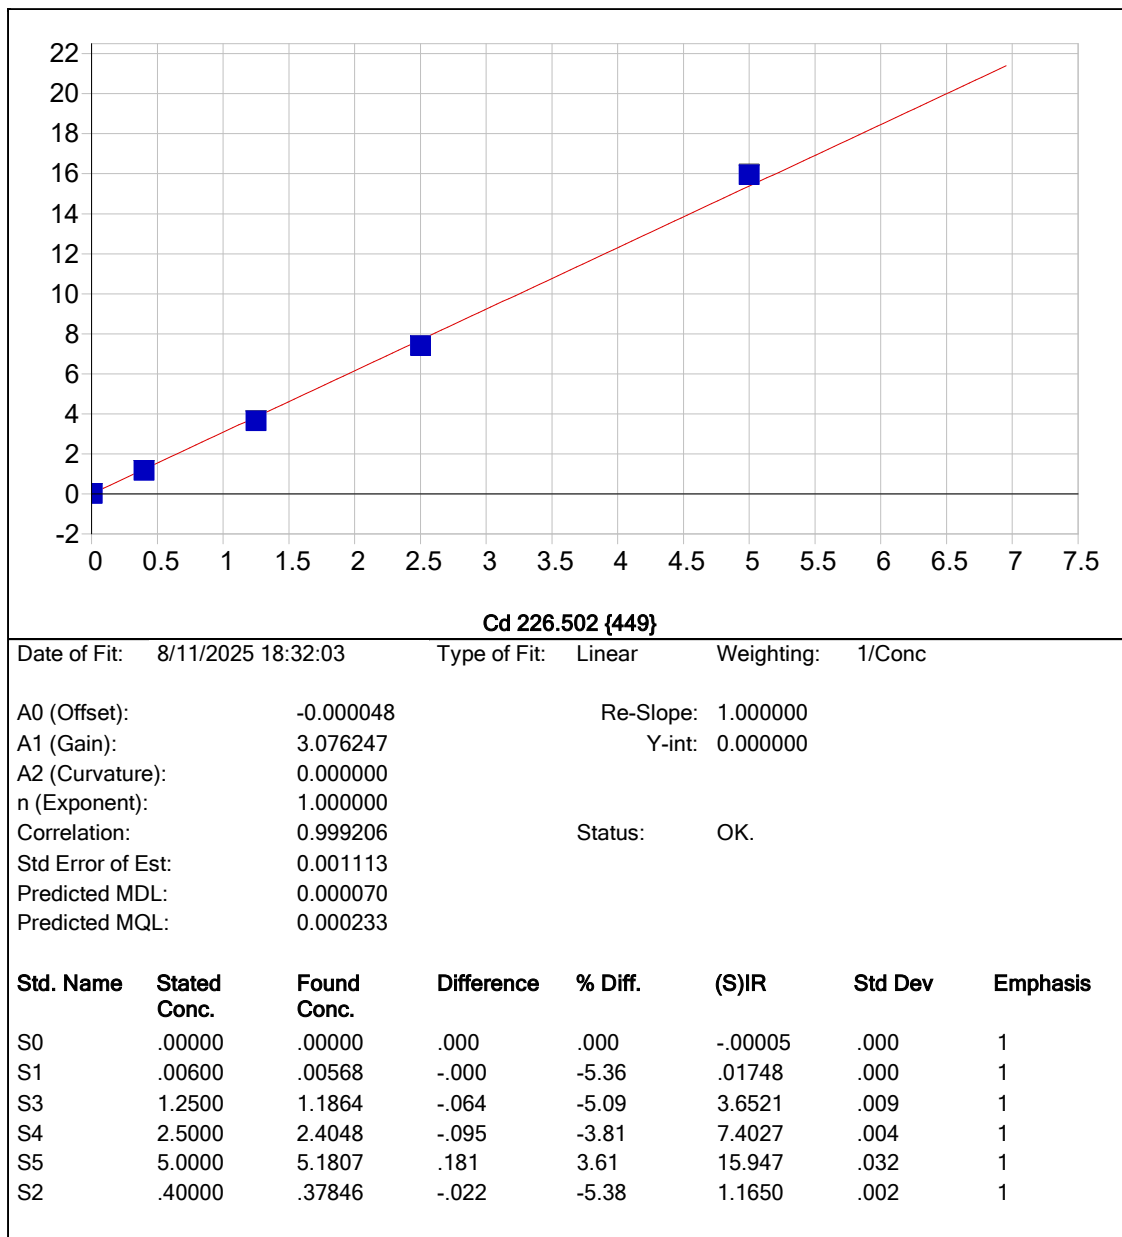



- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

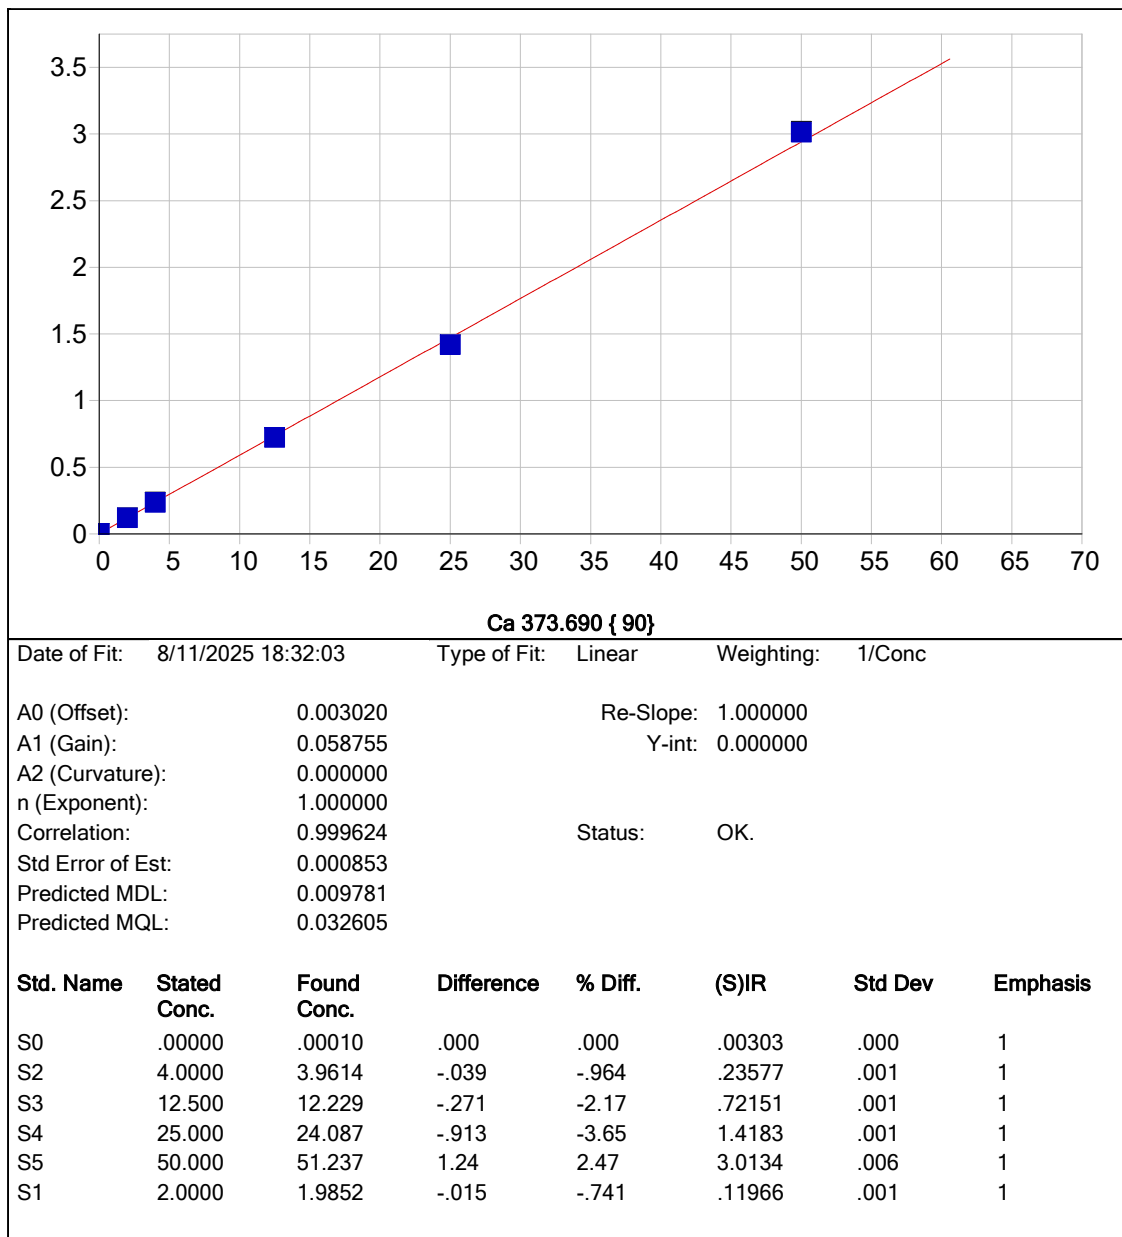


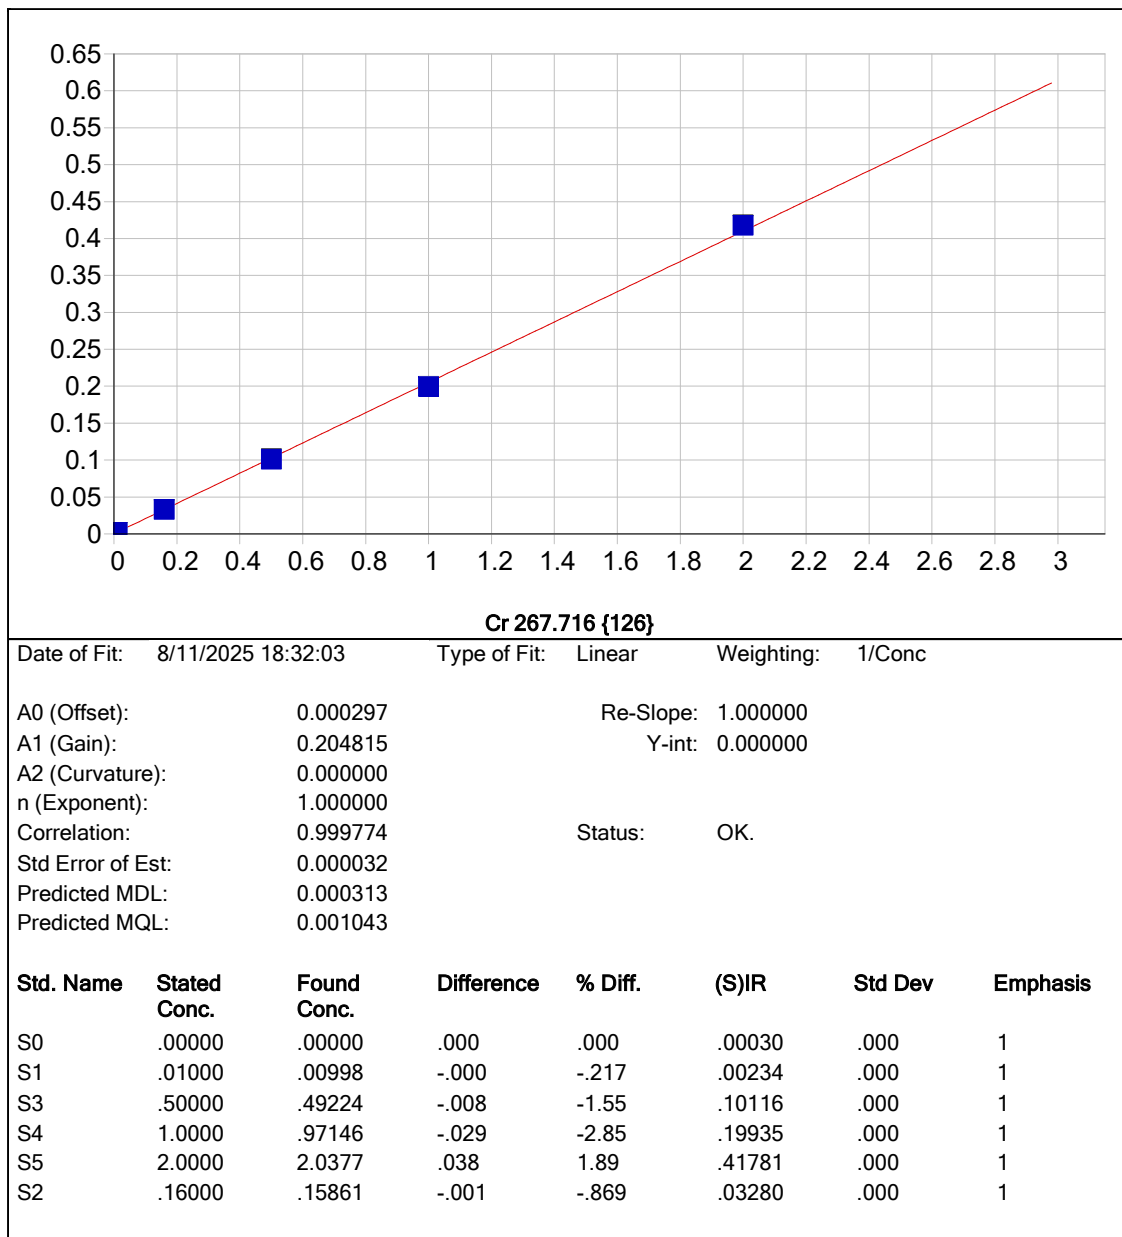


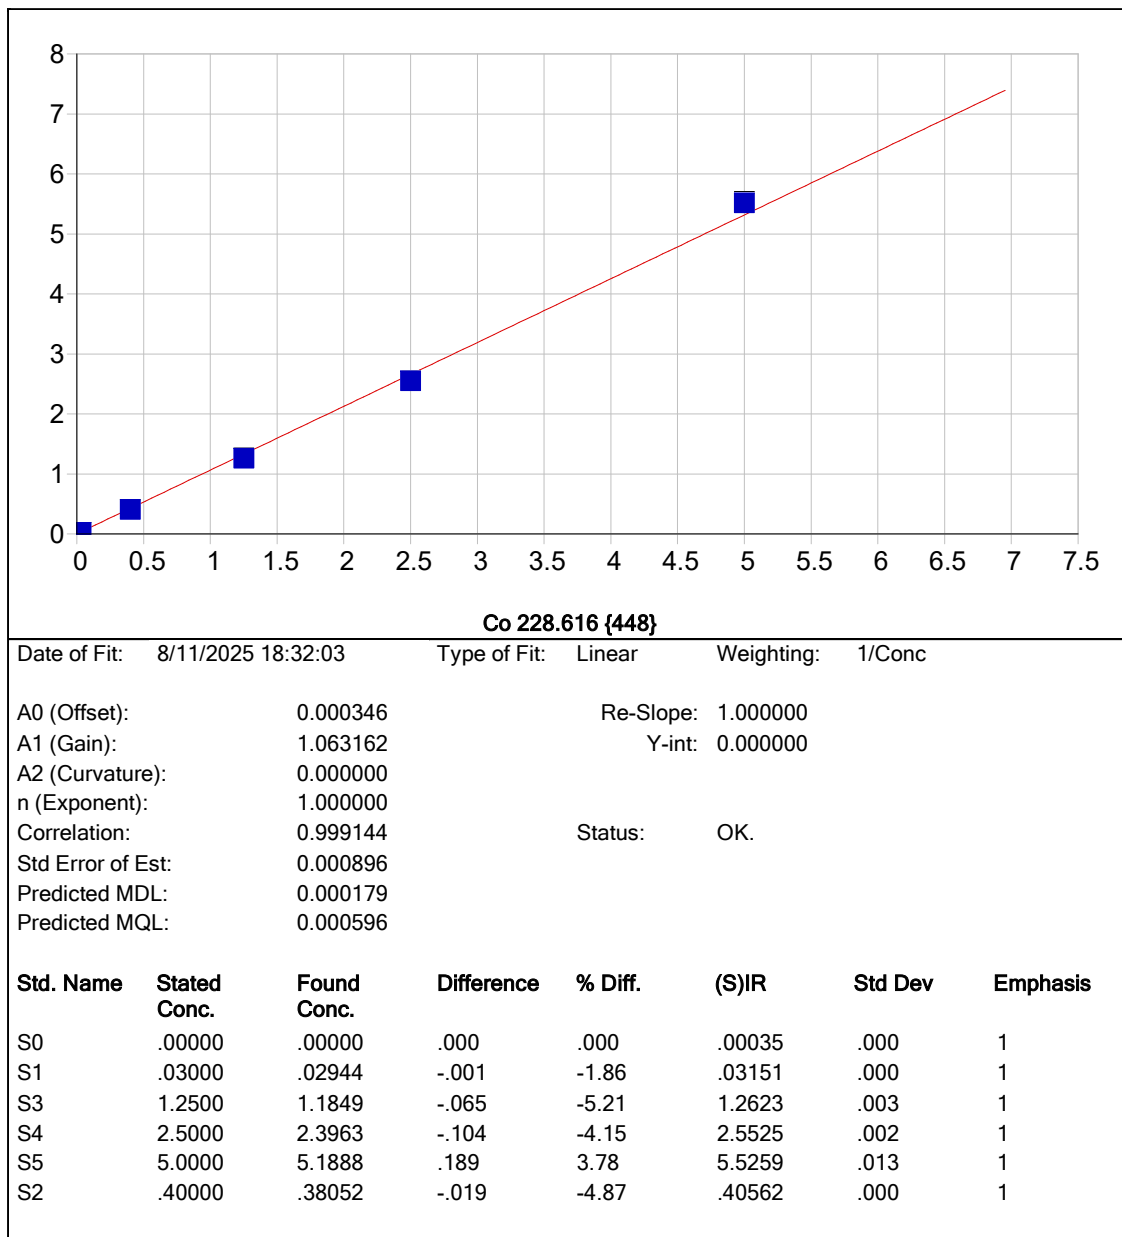


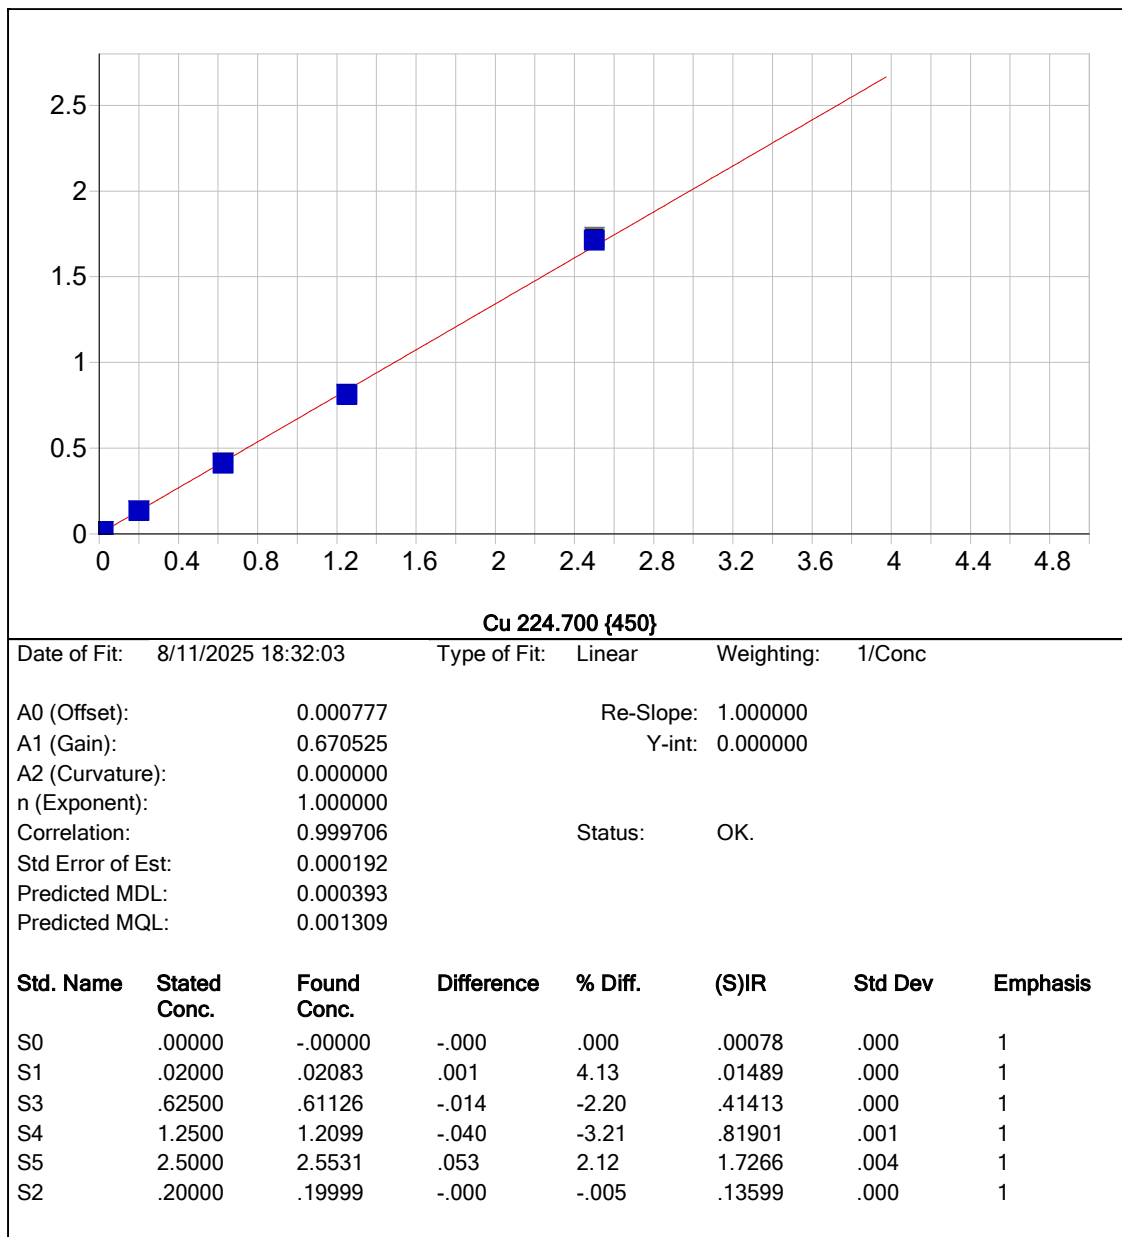


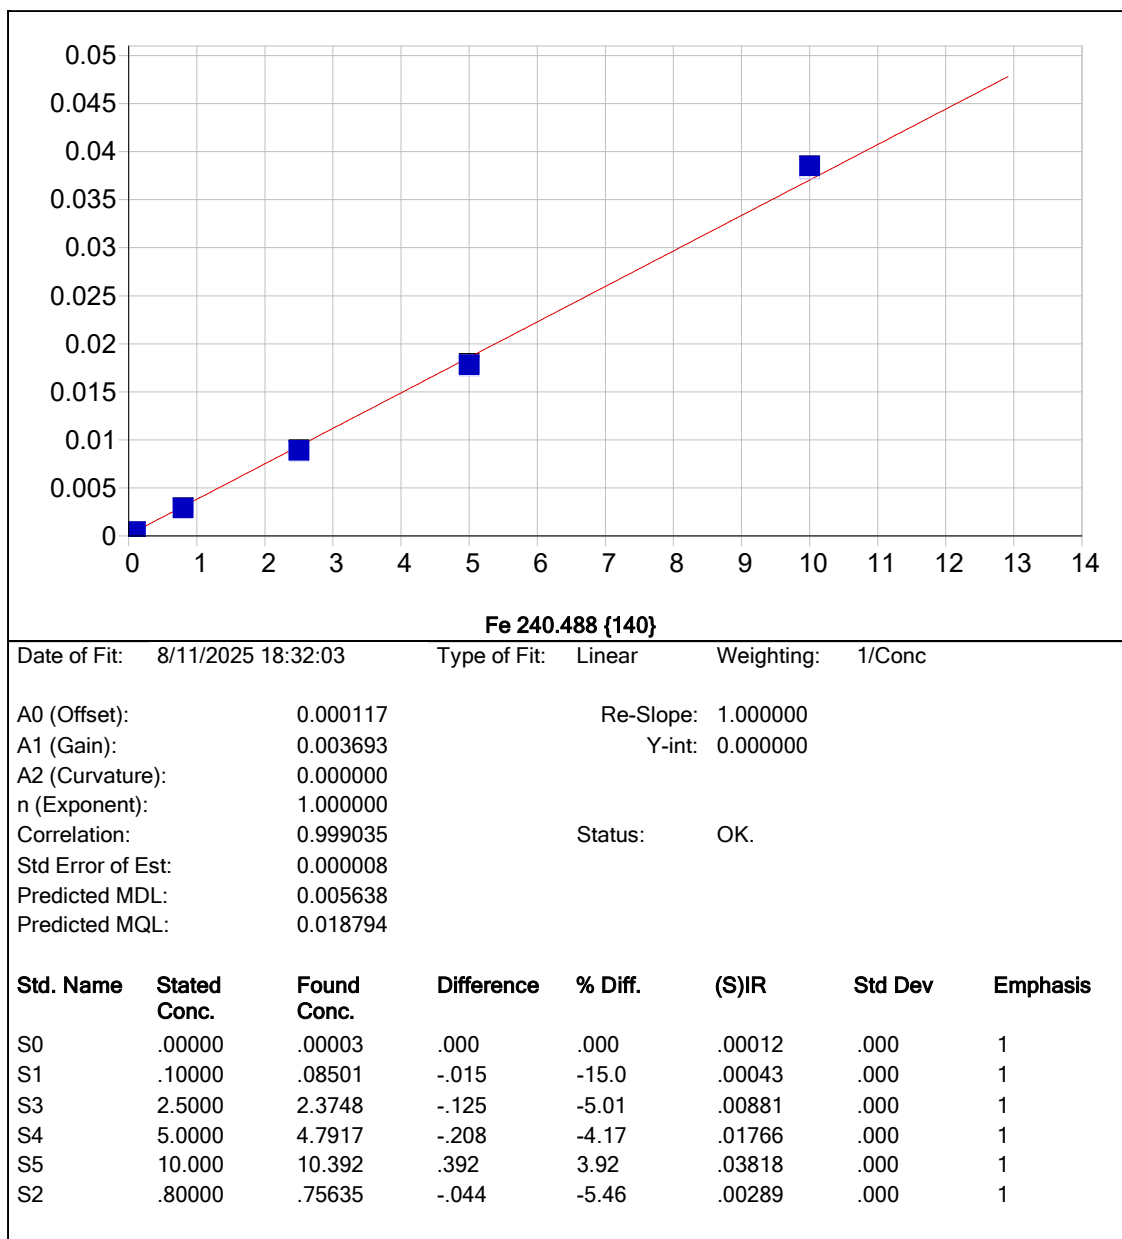


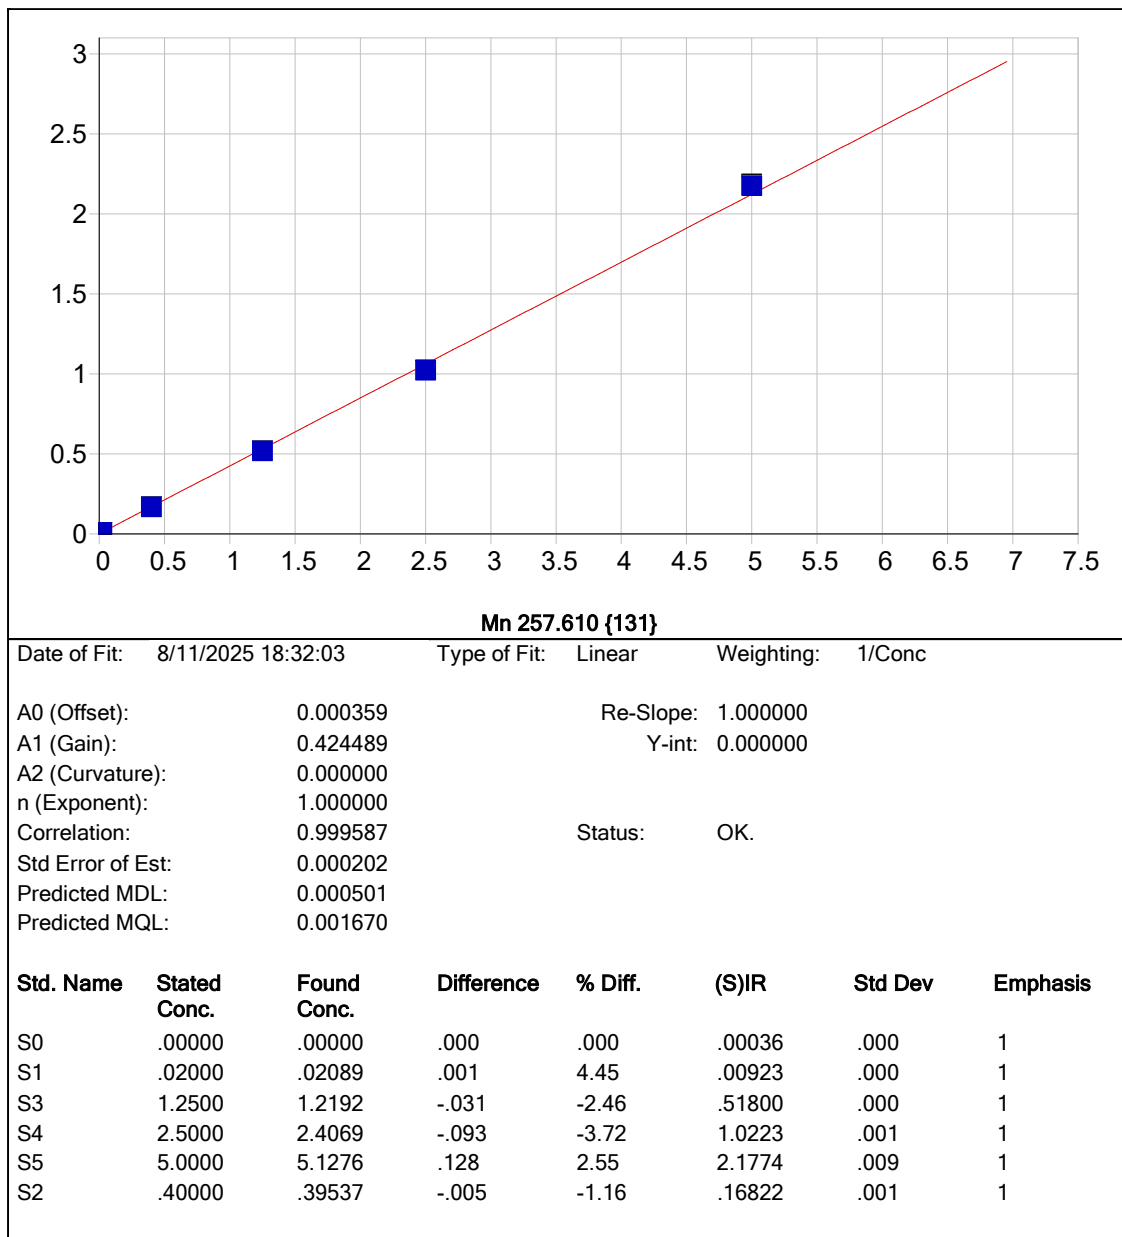


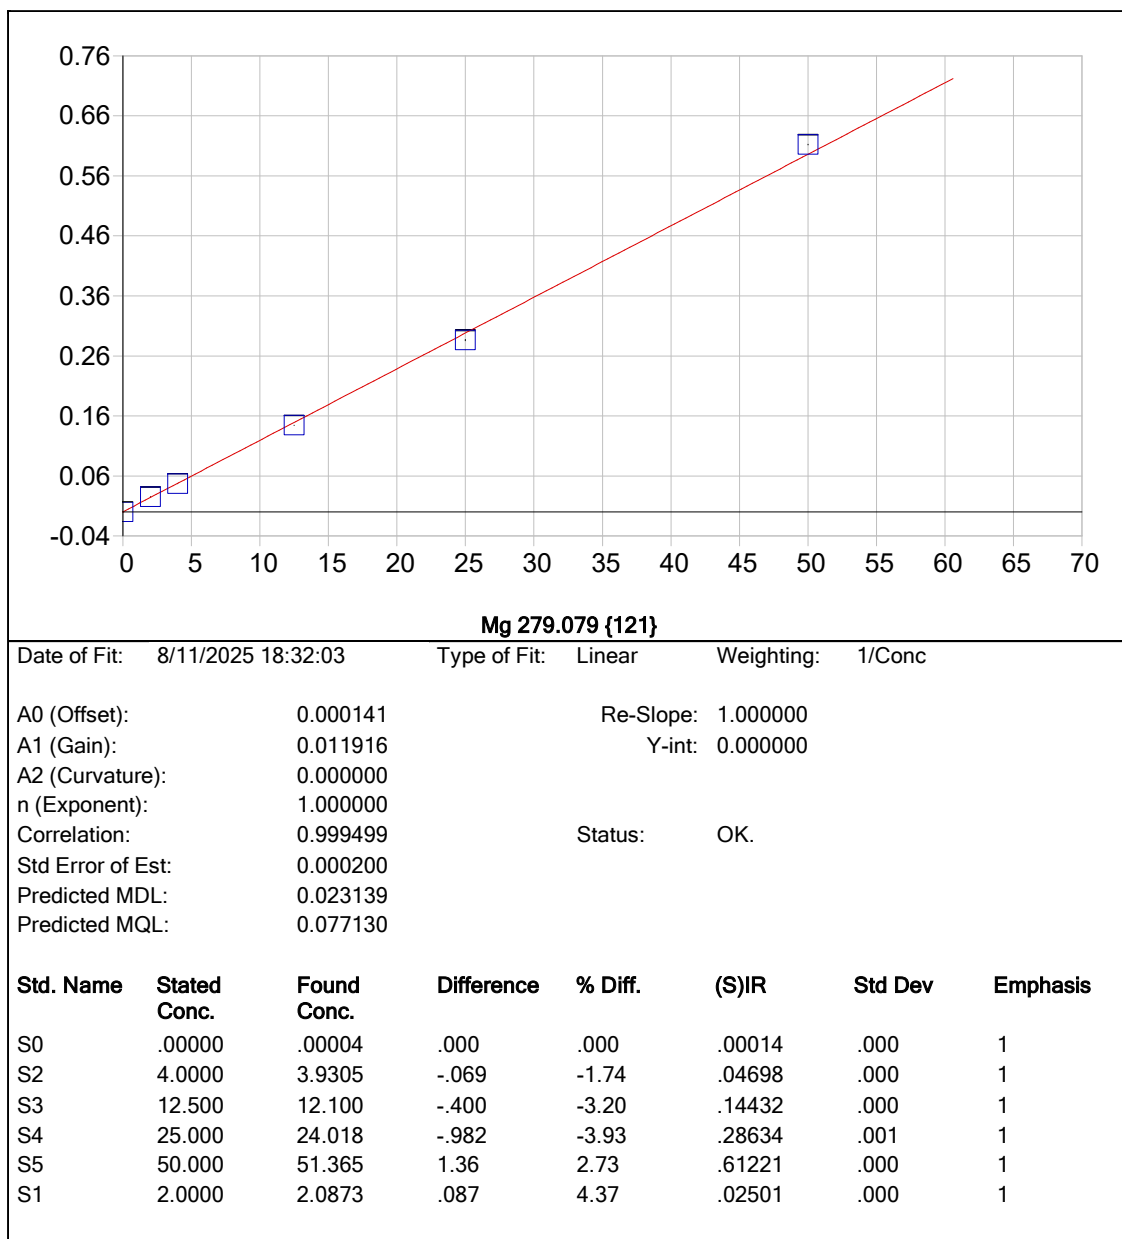


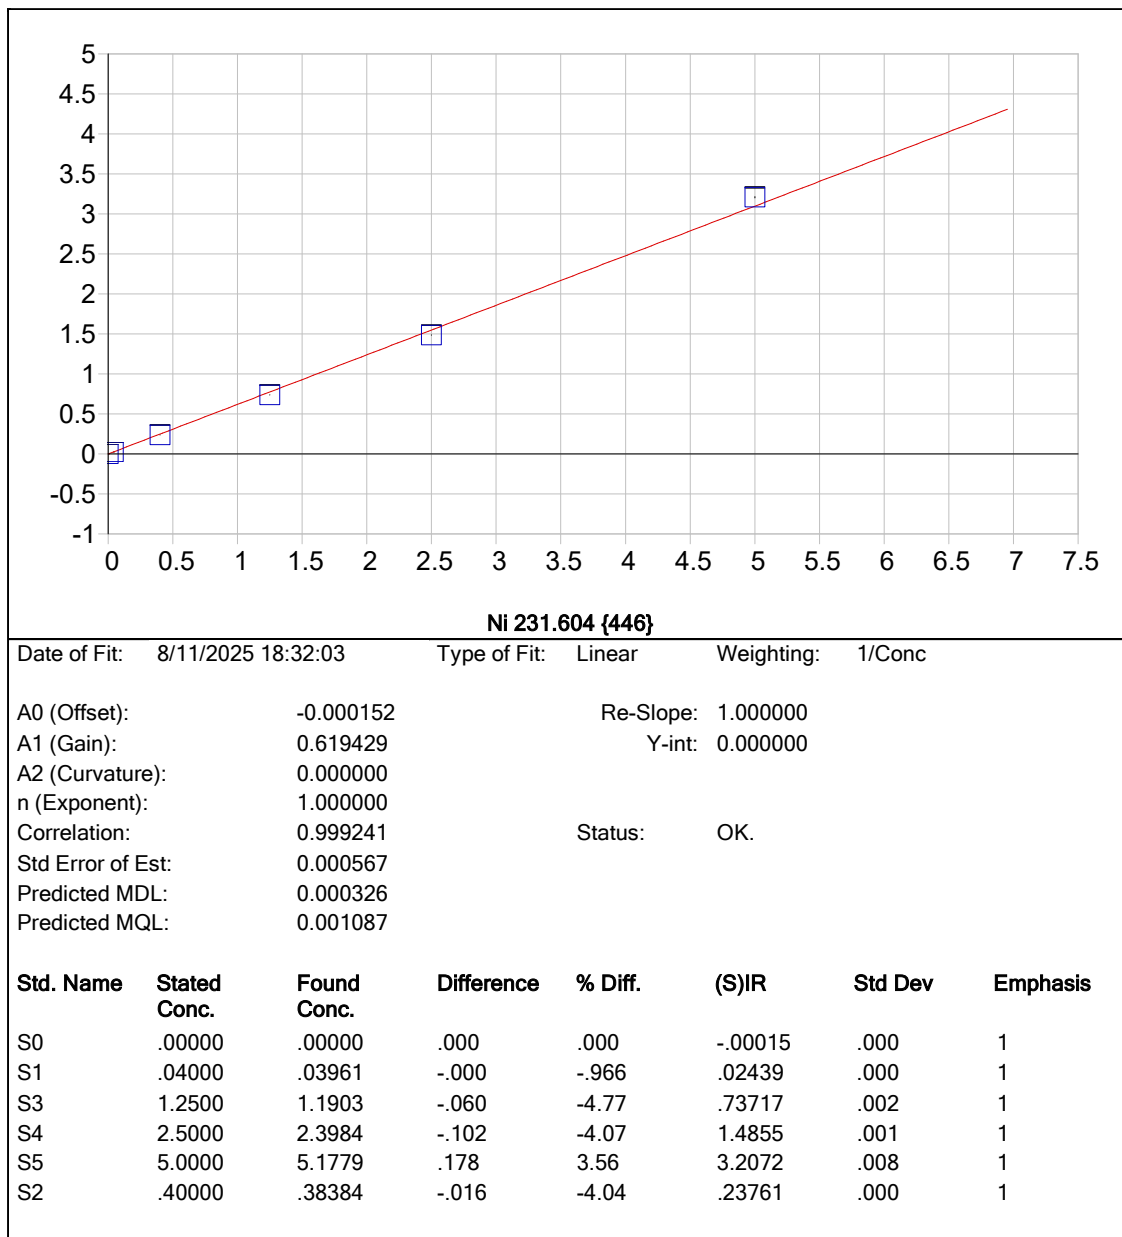


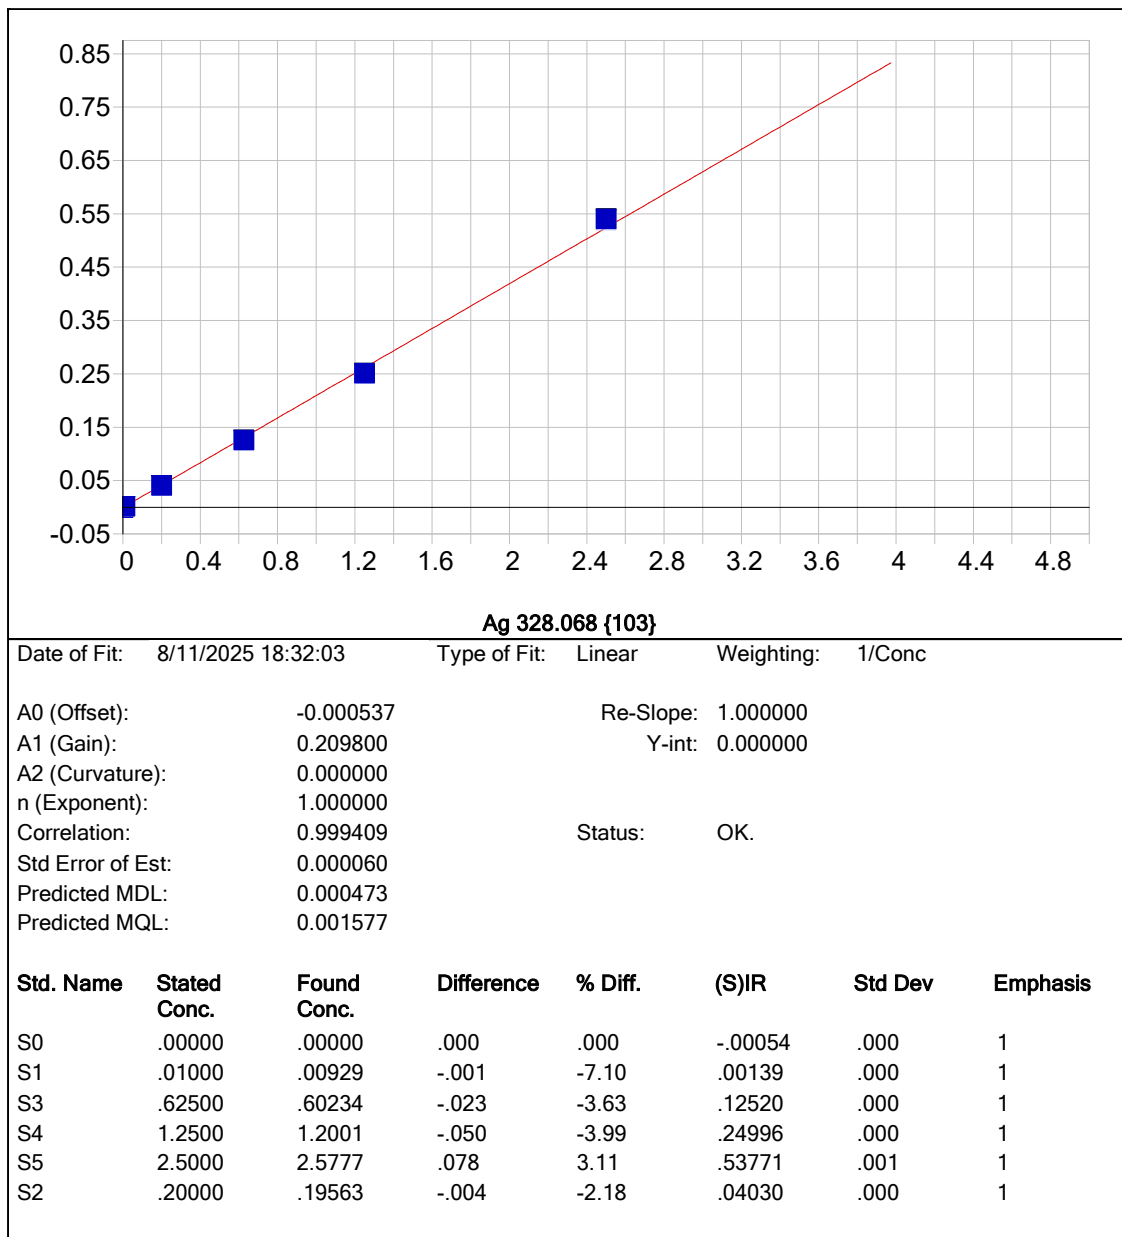


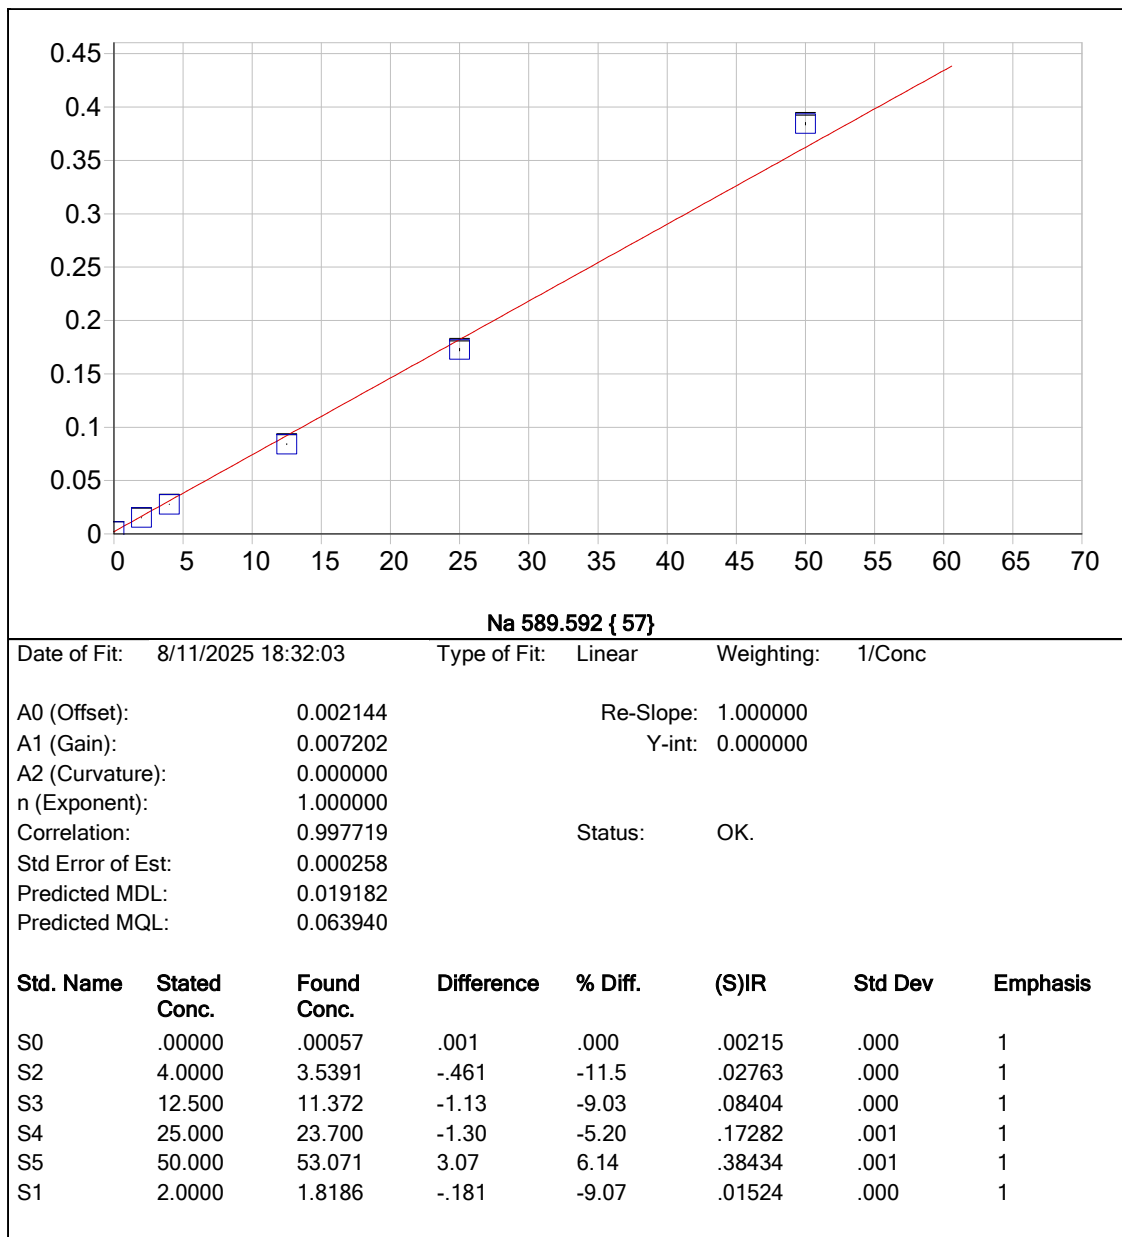


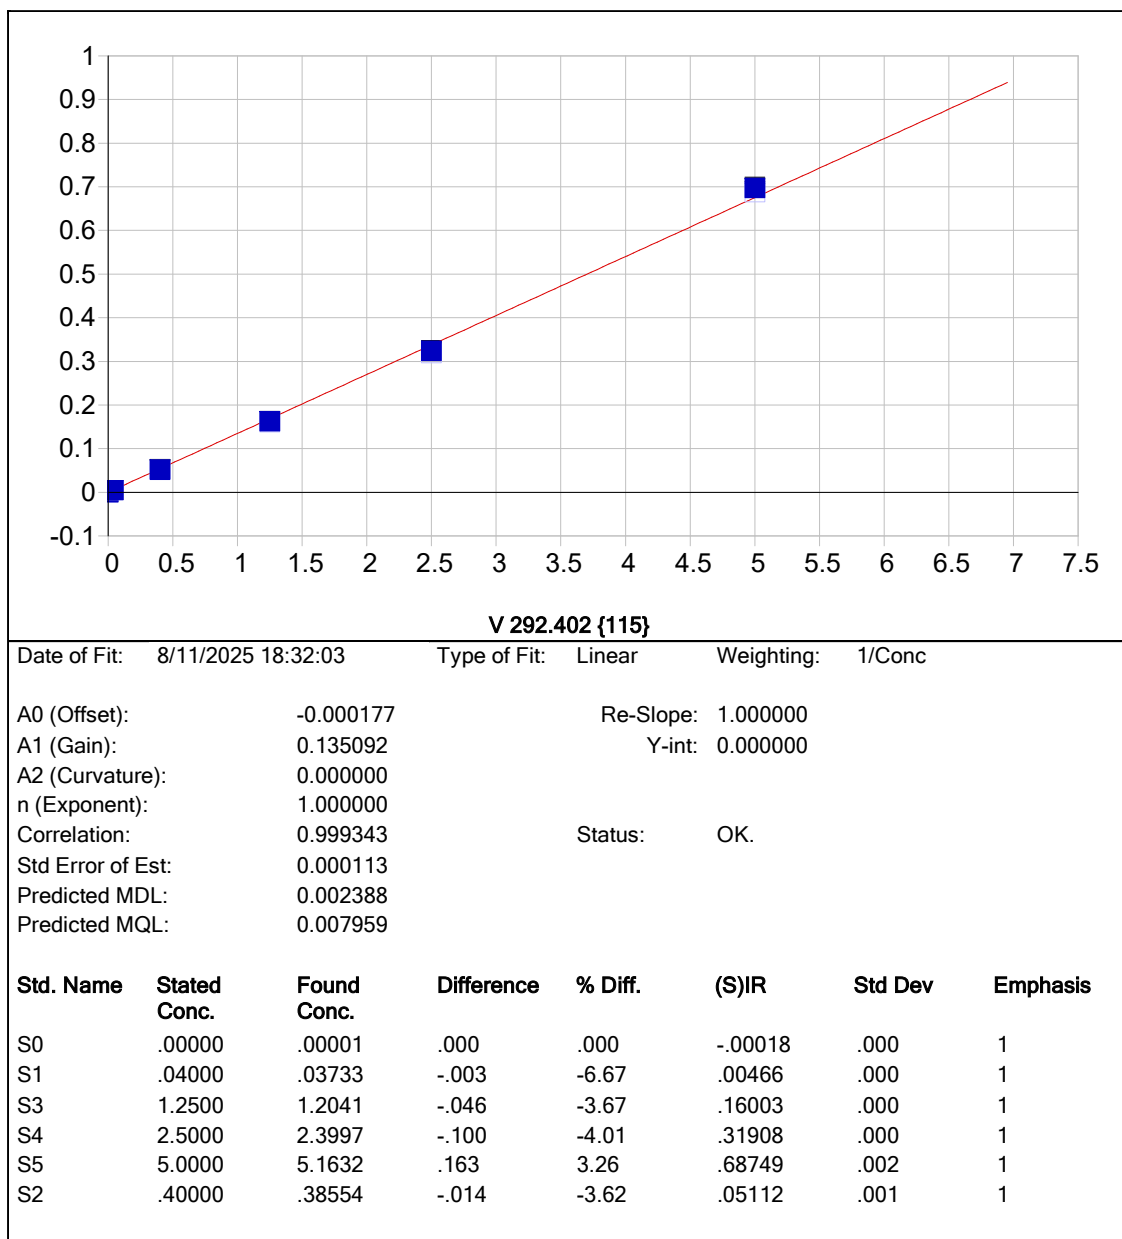


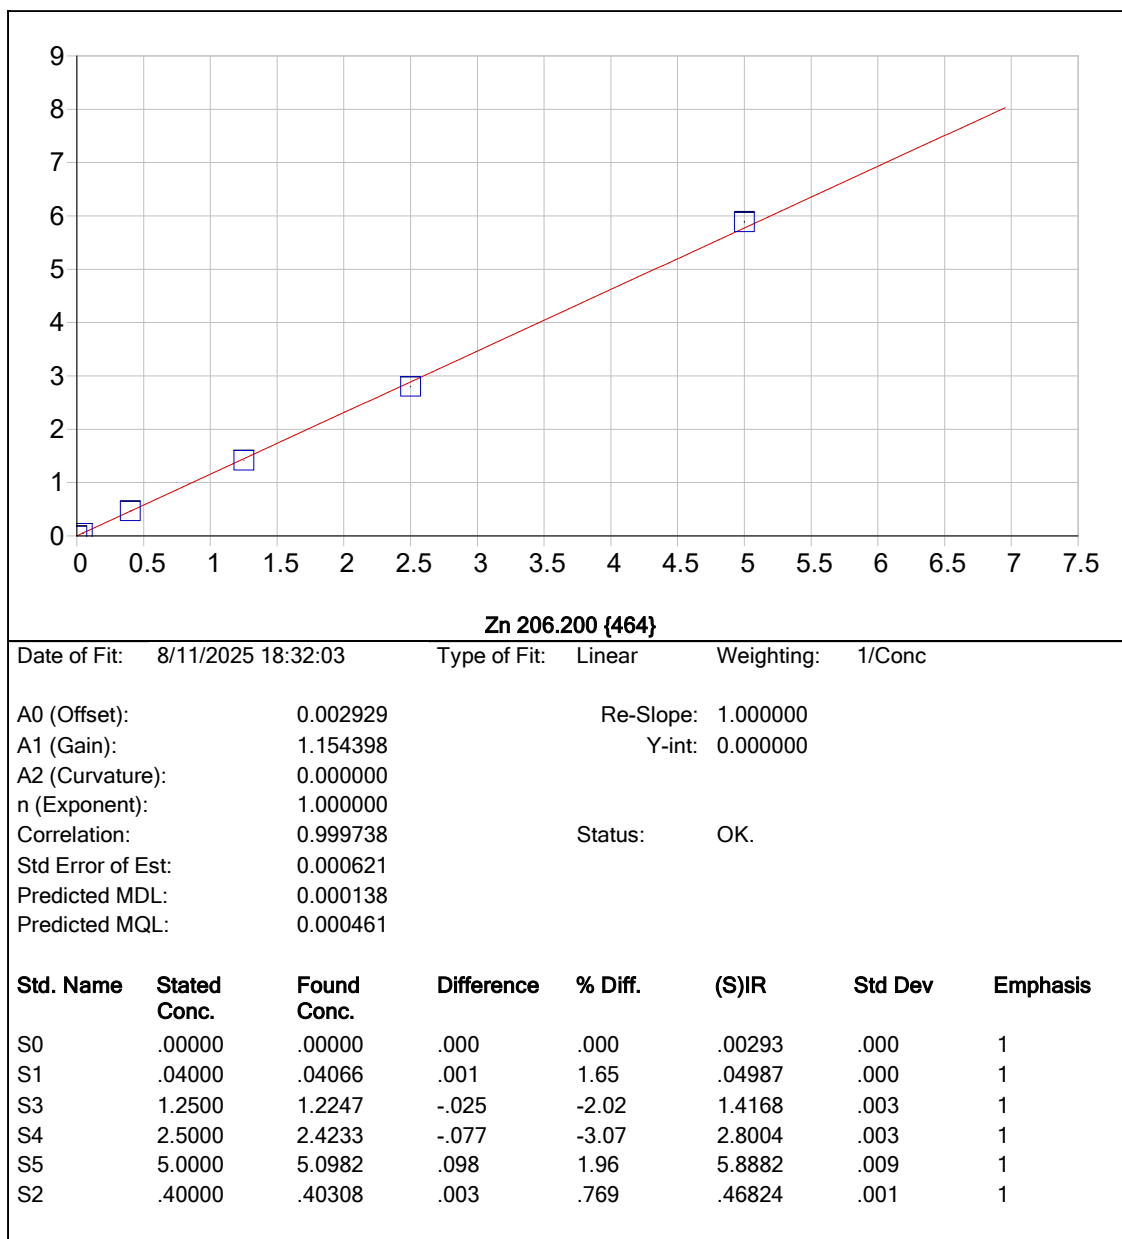


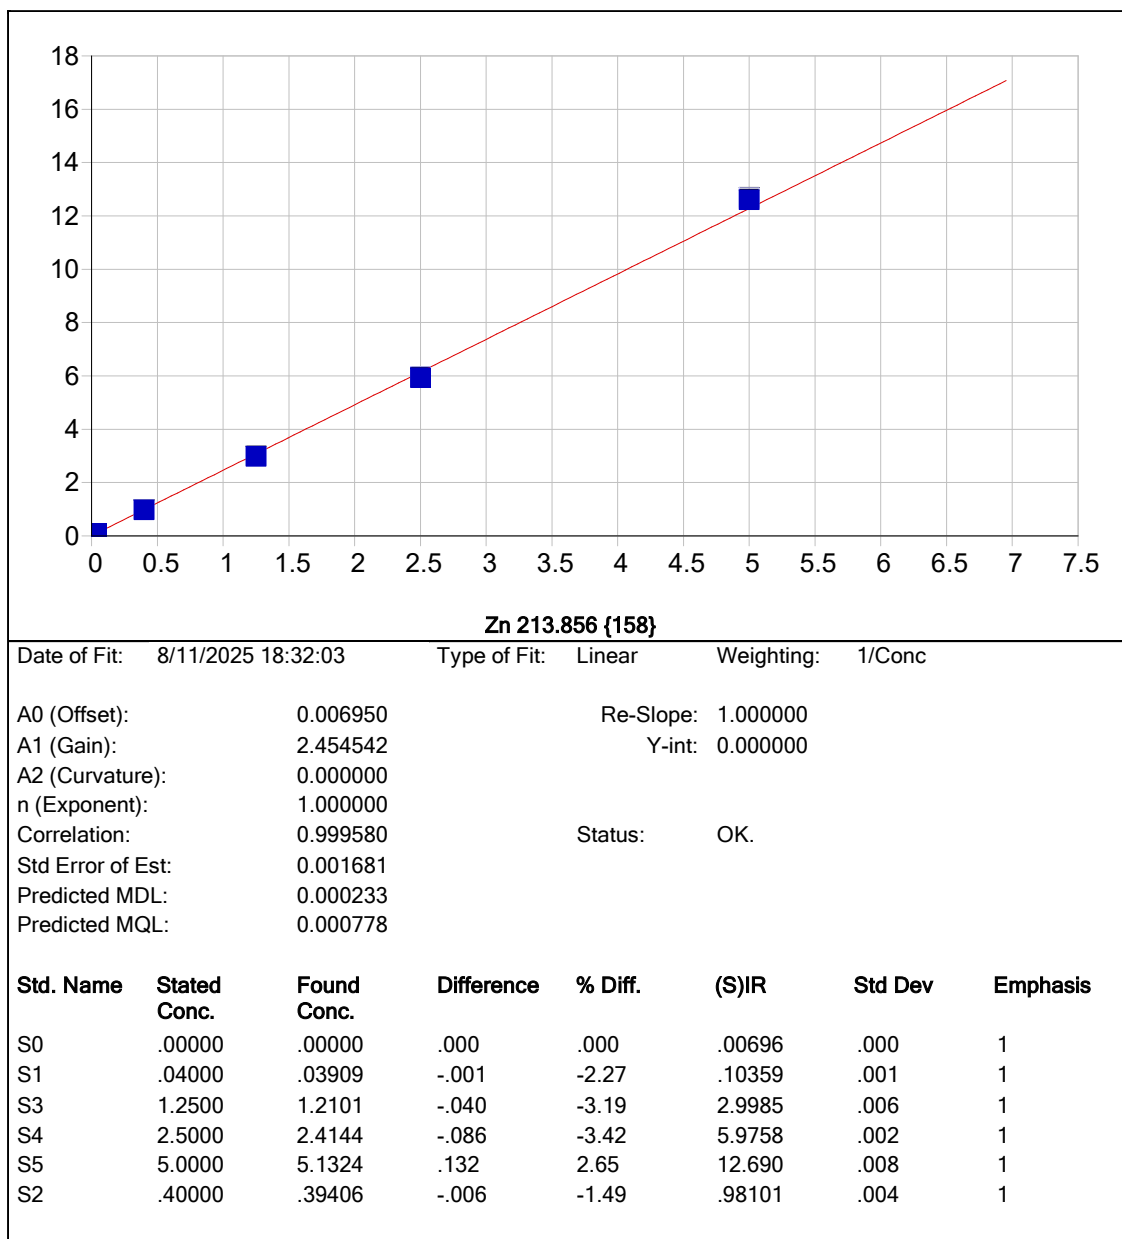


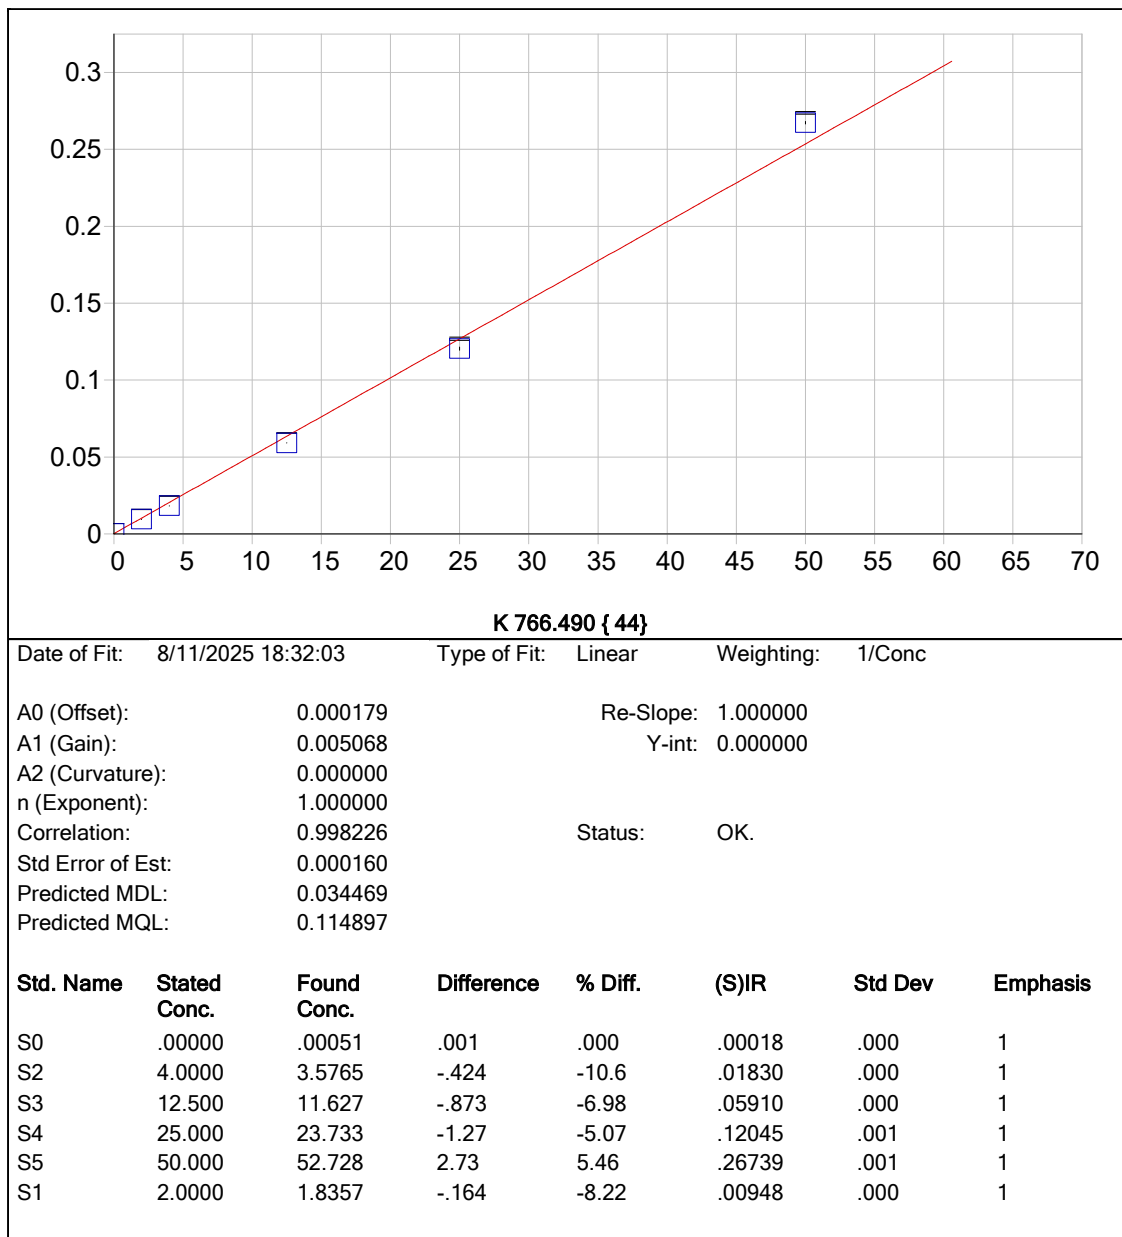


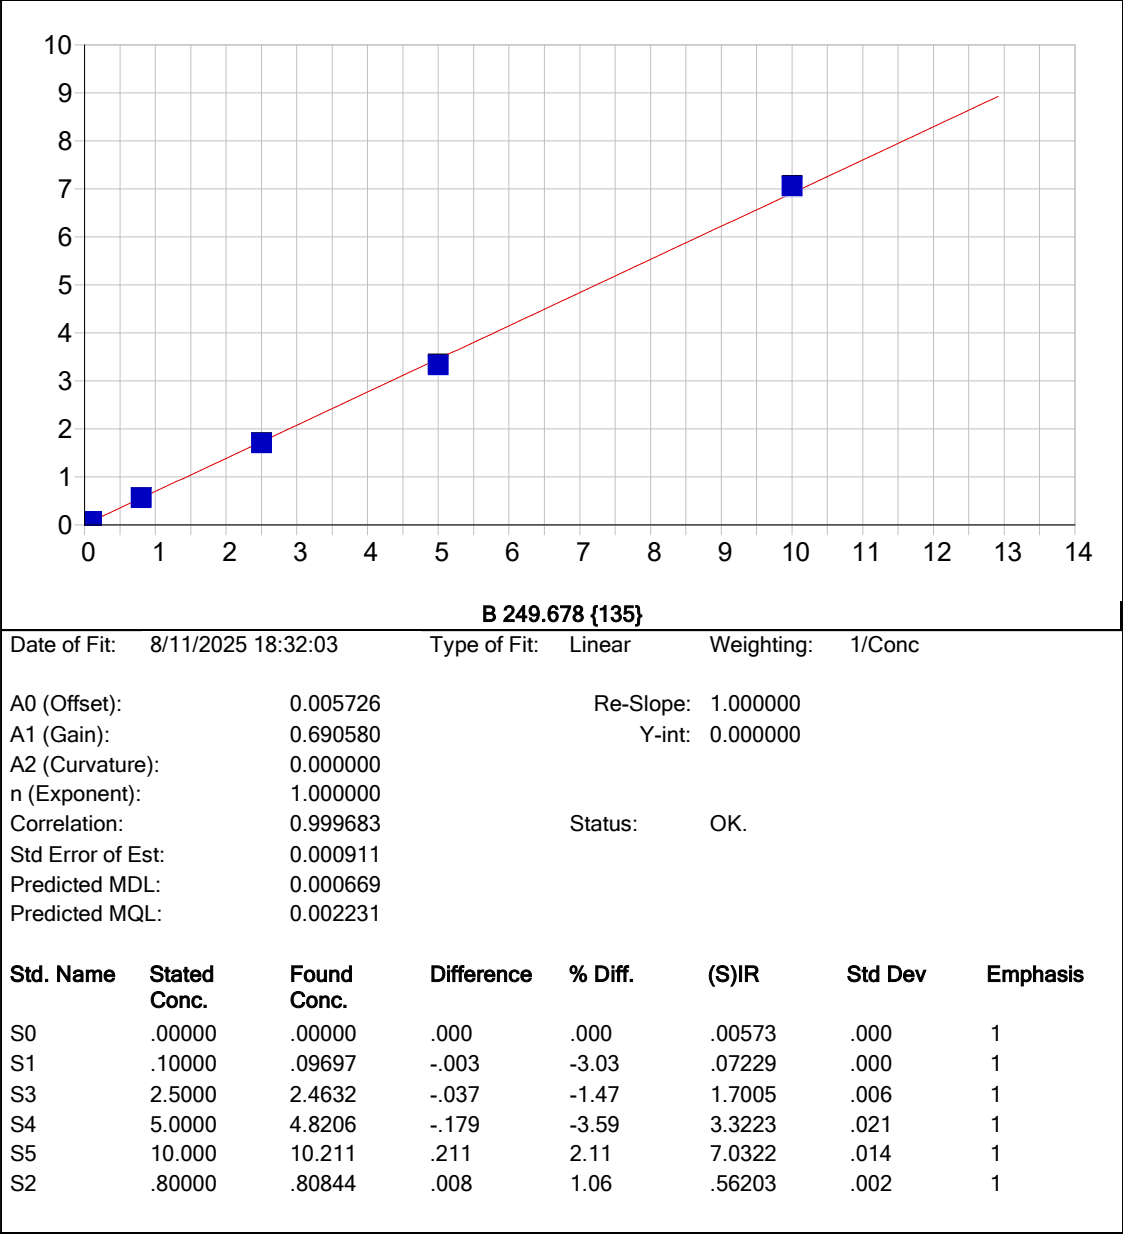


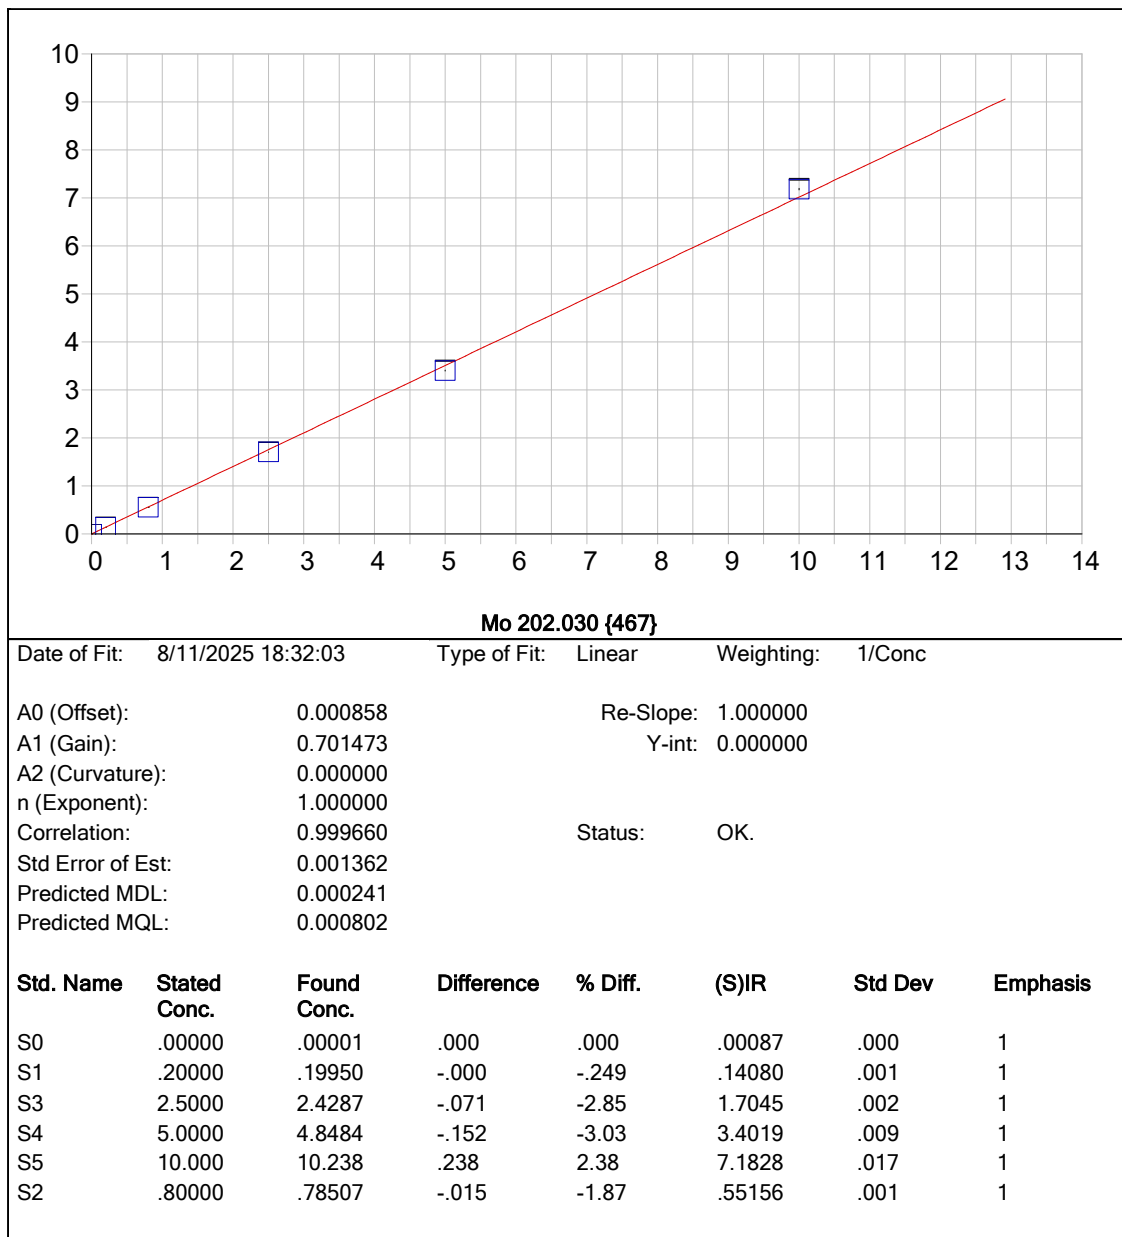


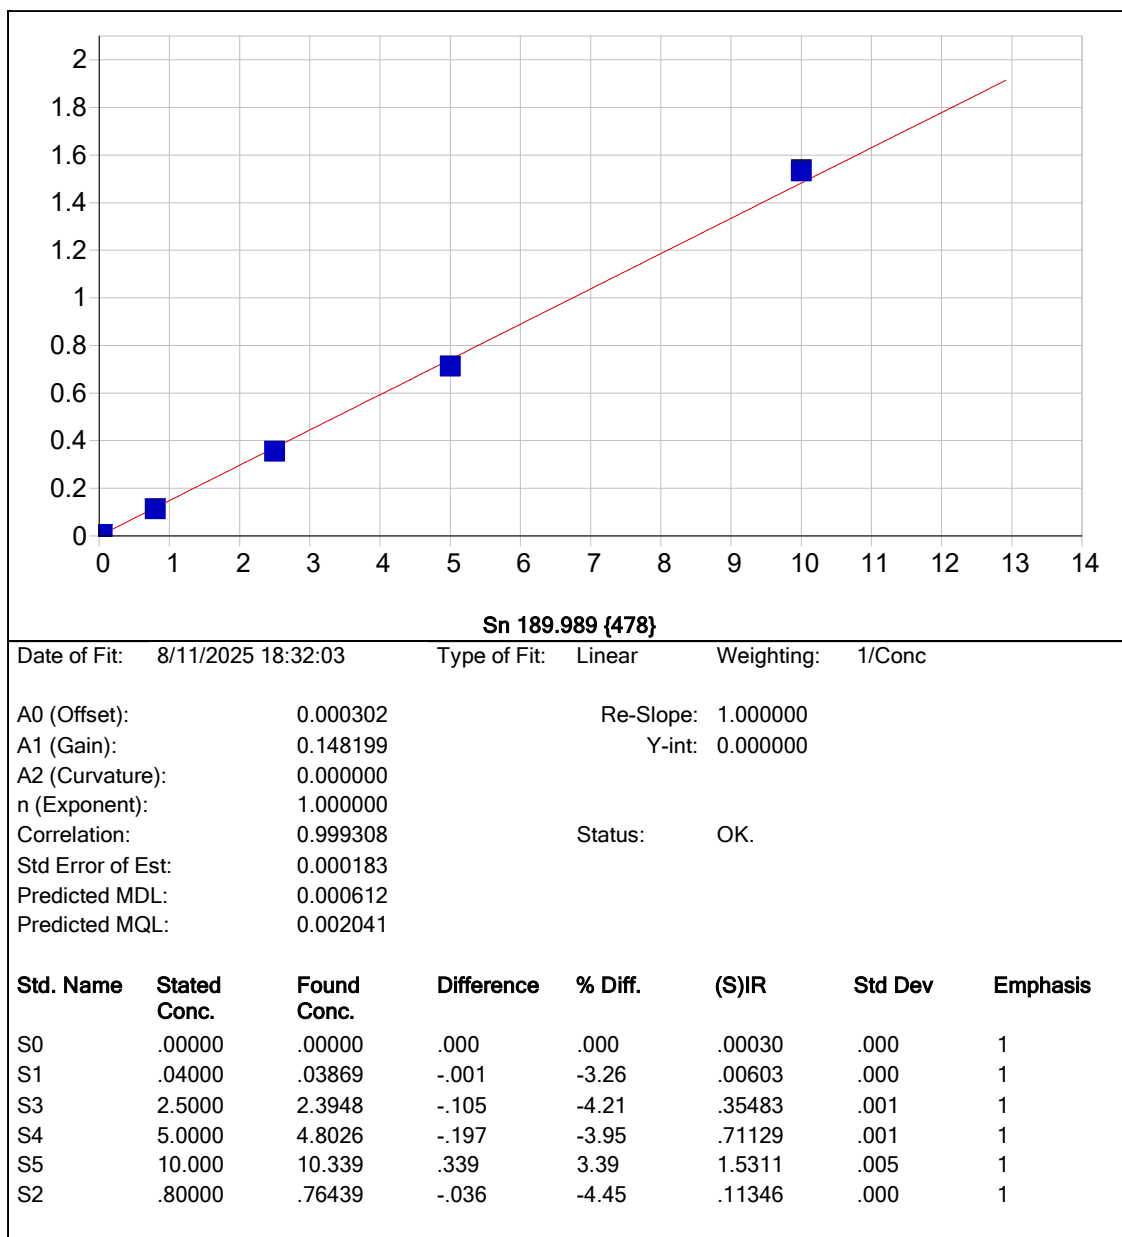


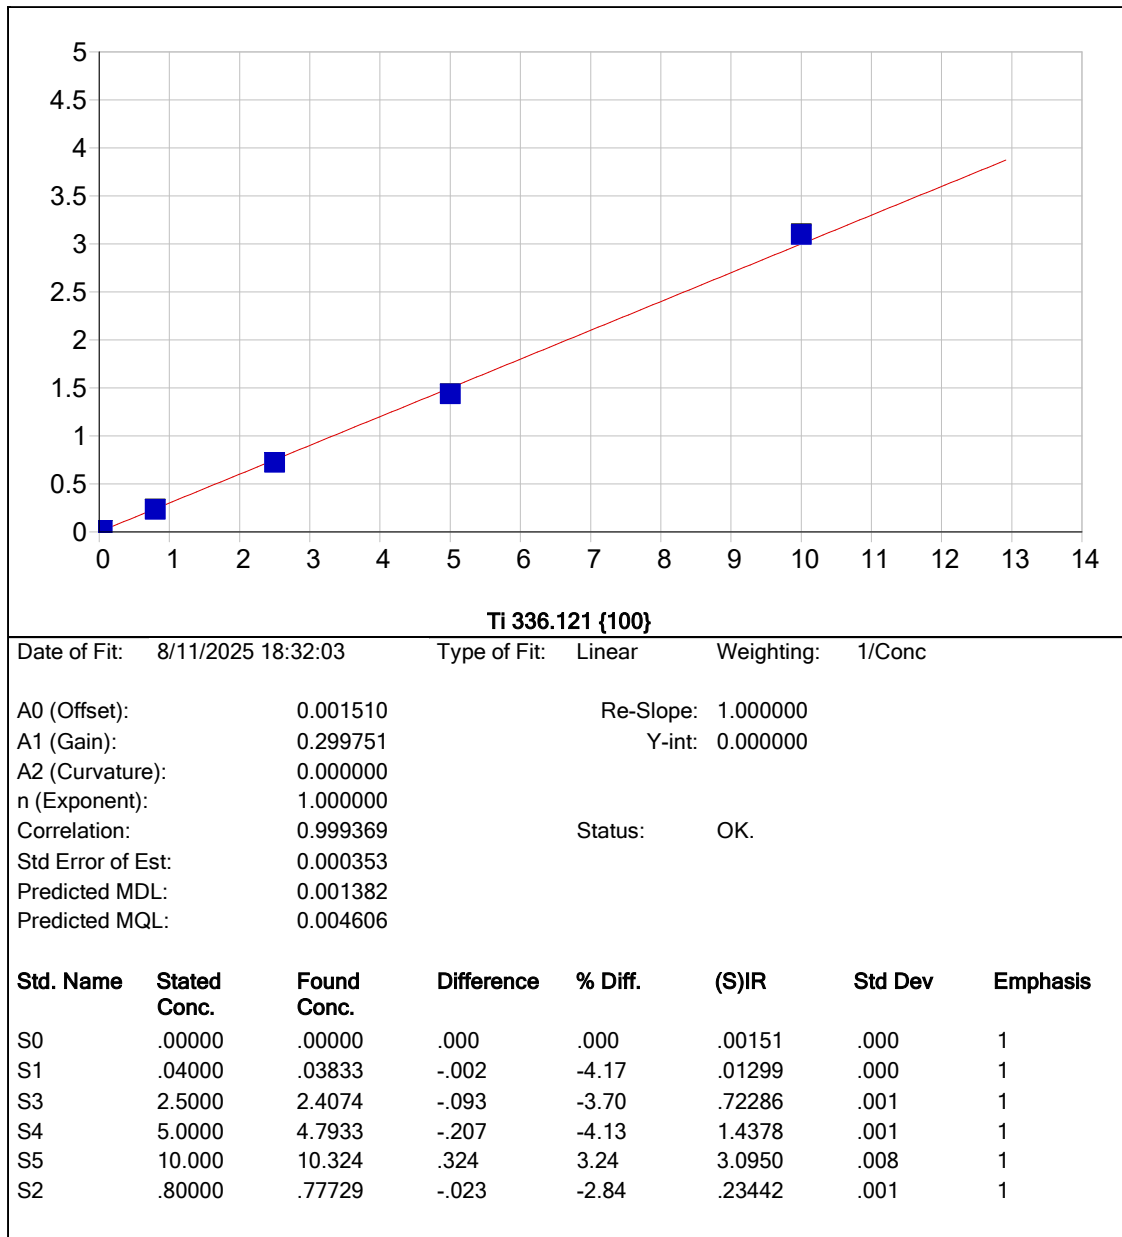


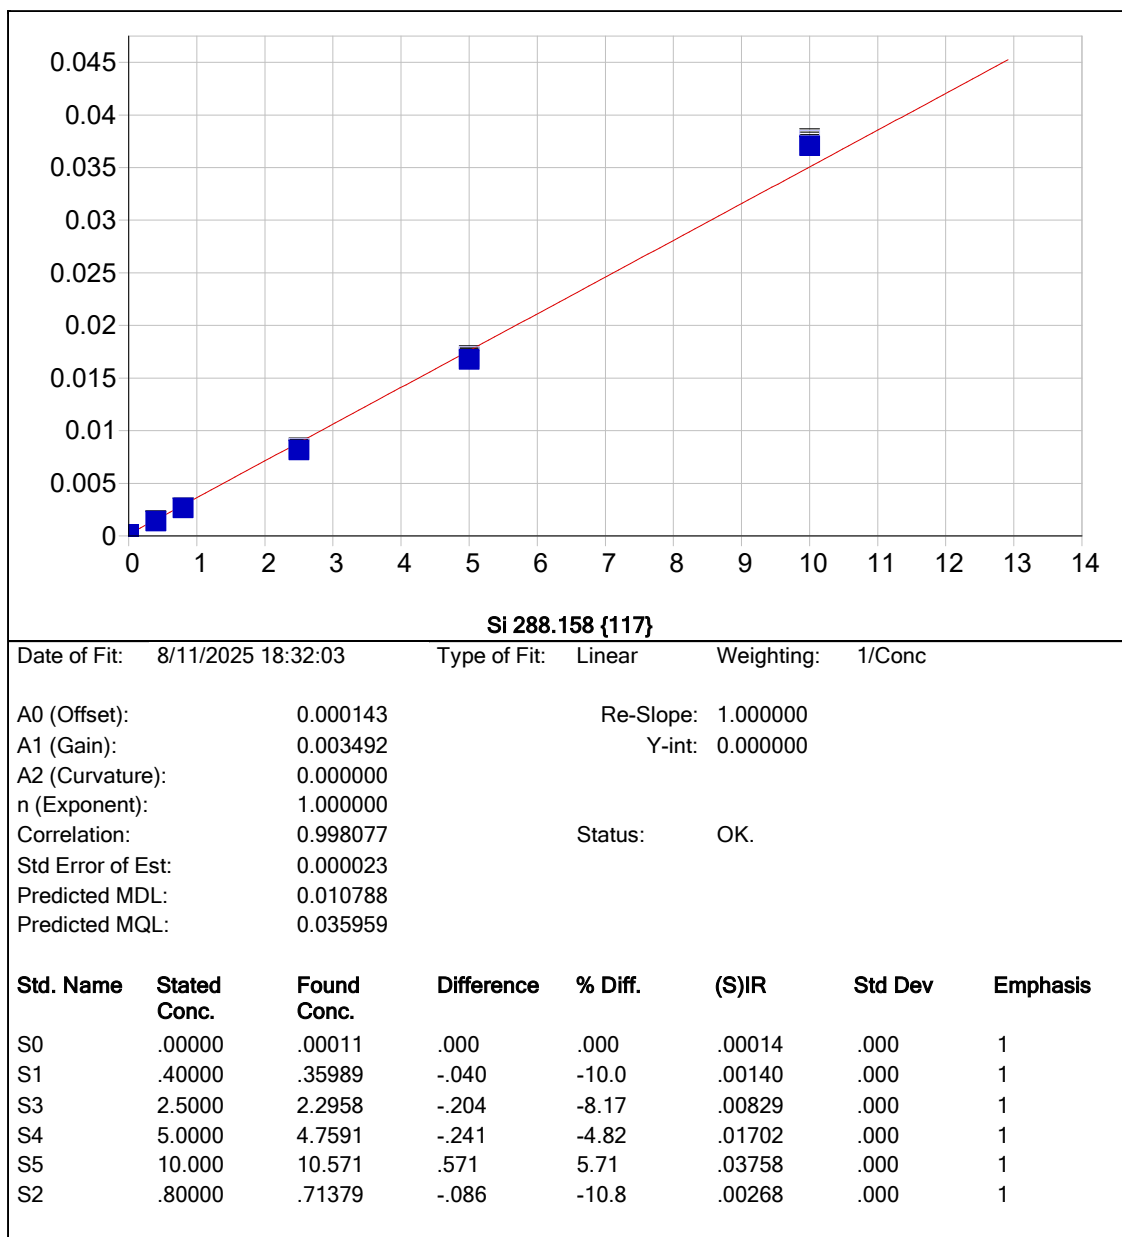


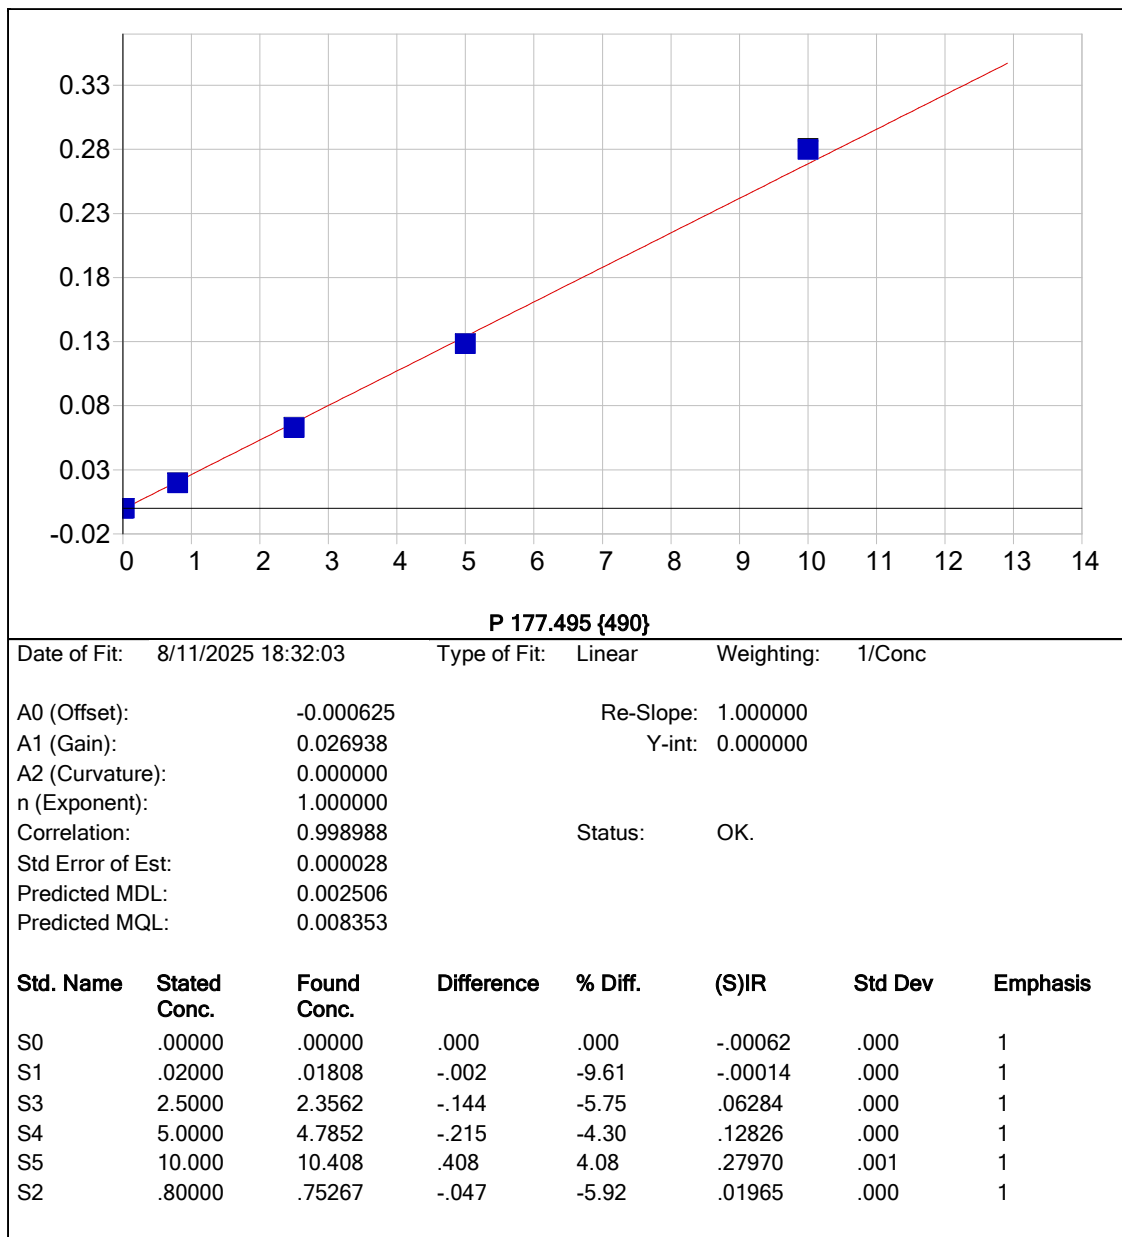

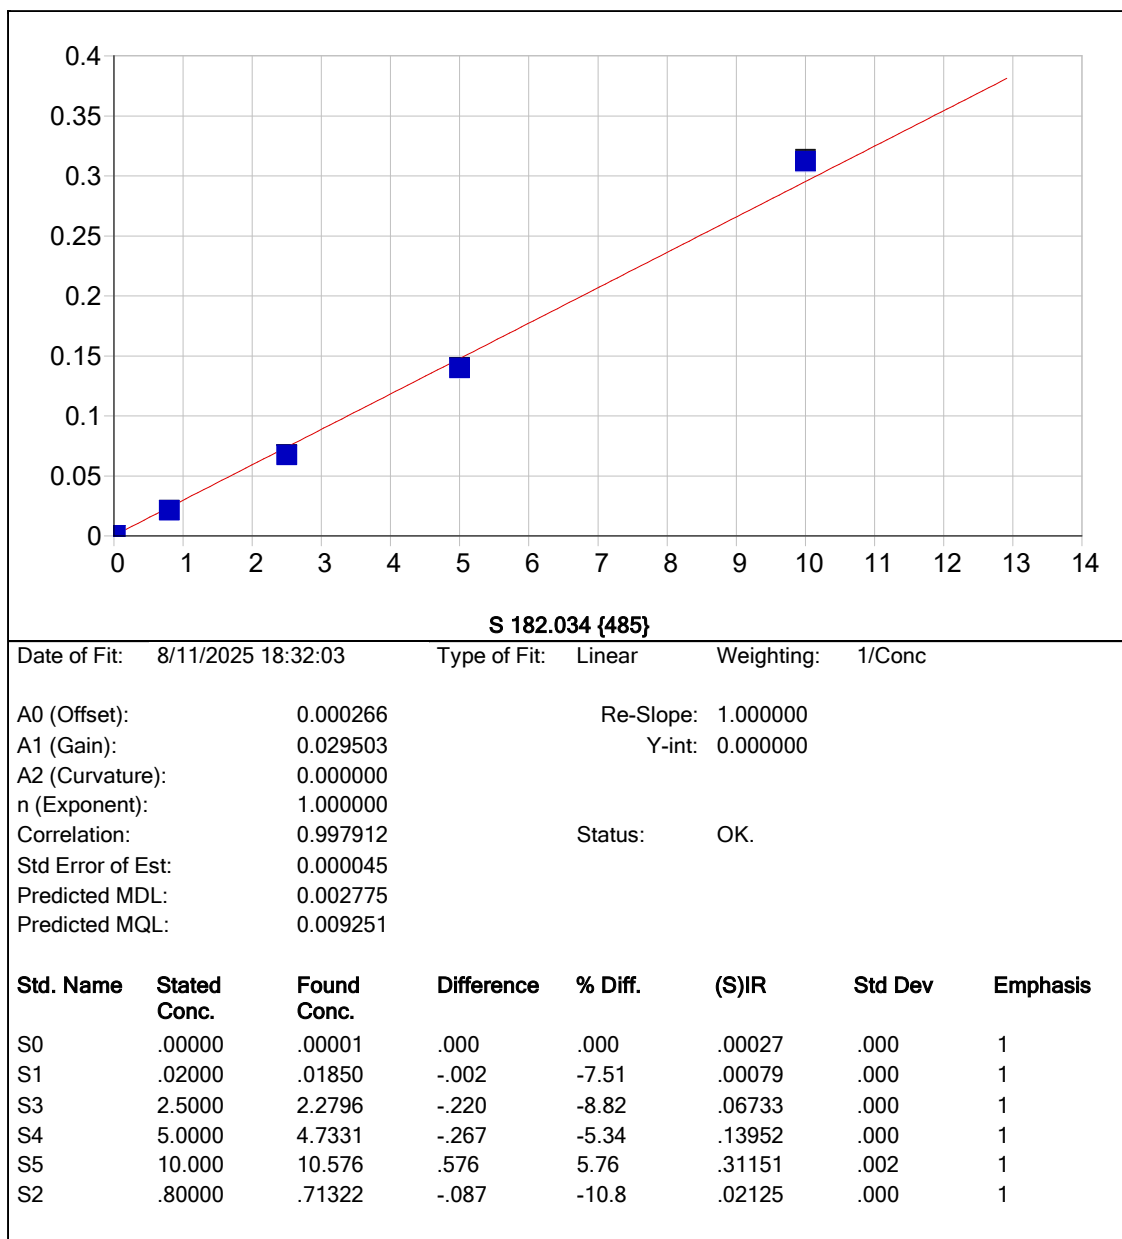


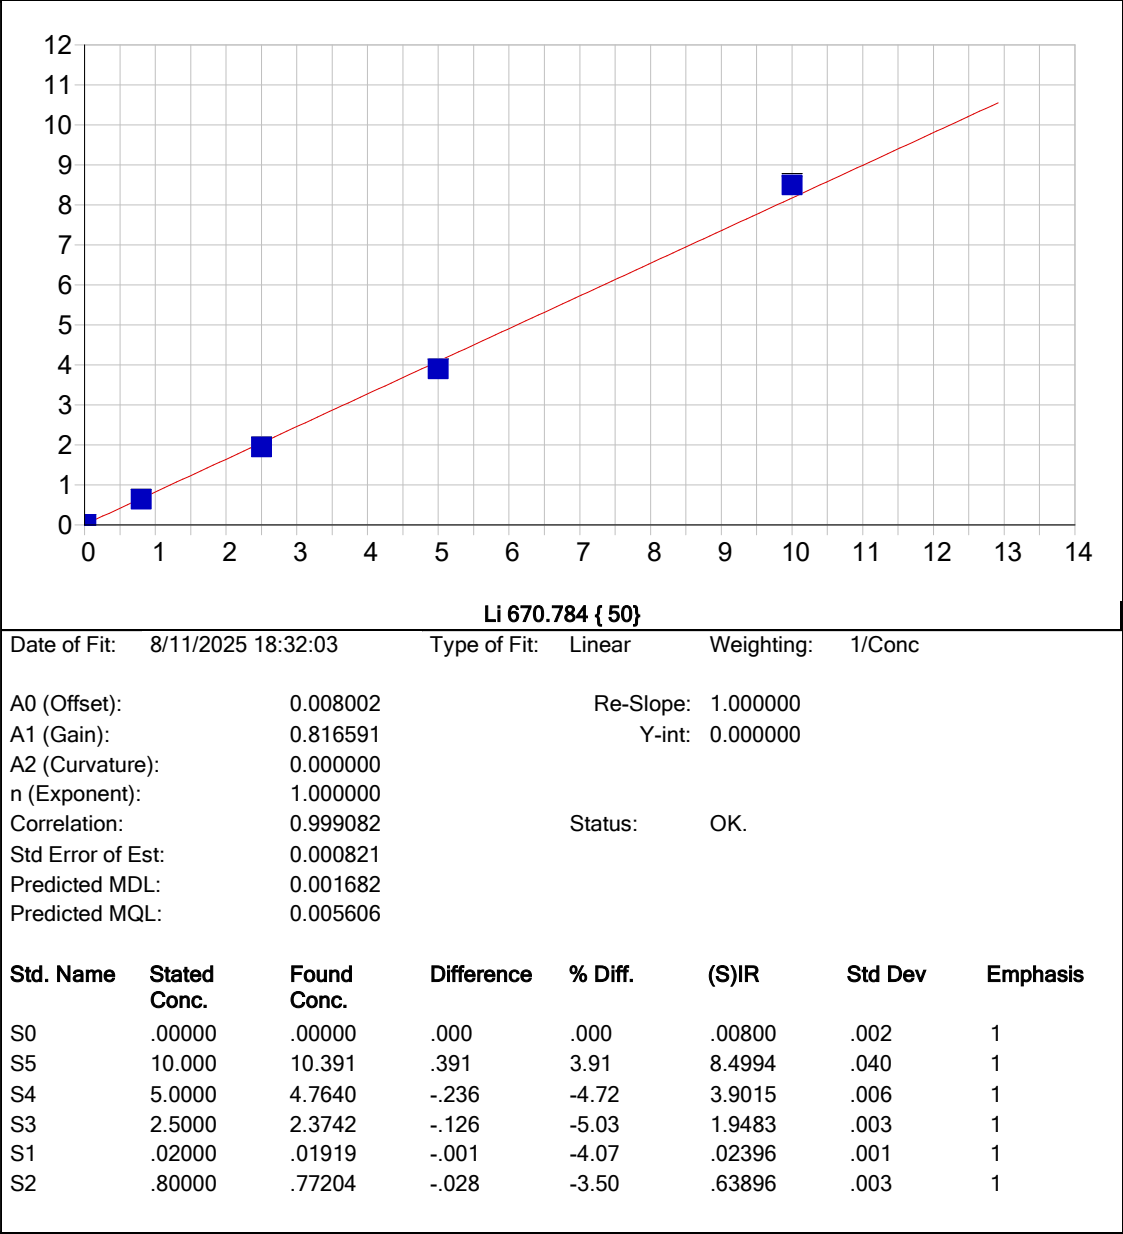

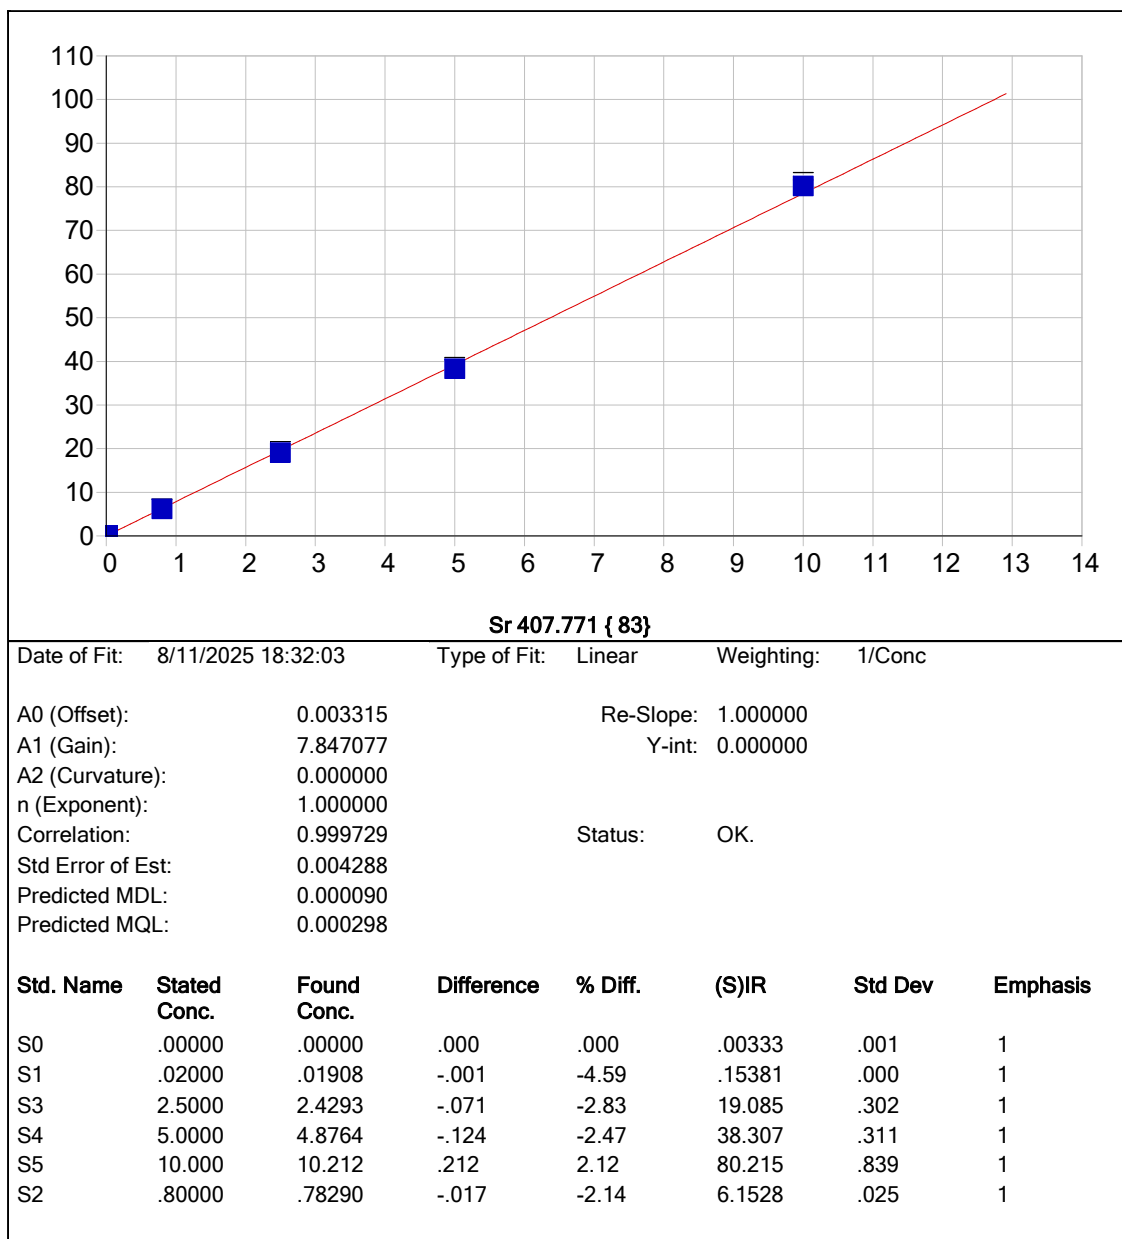


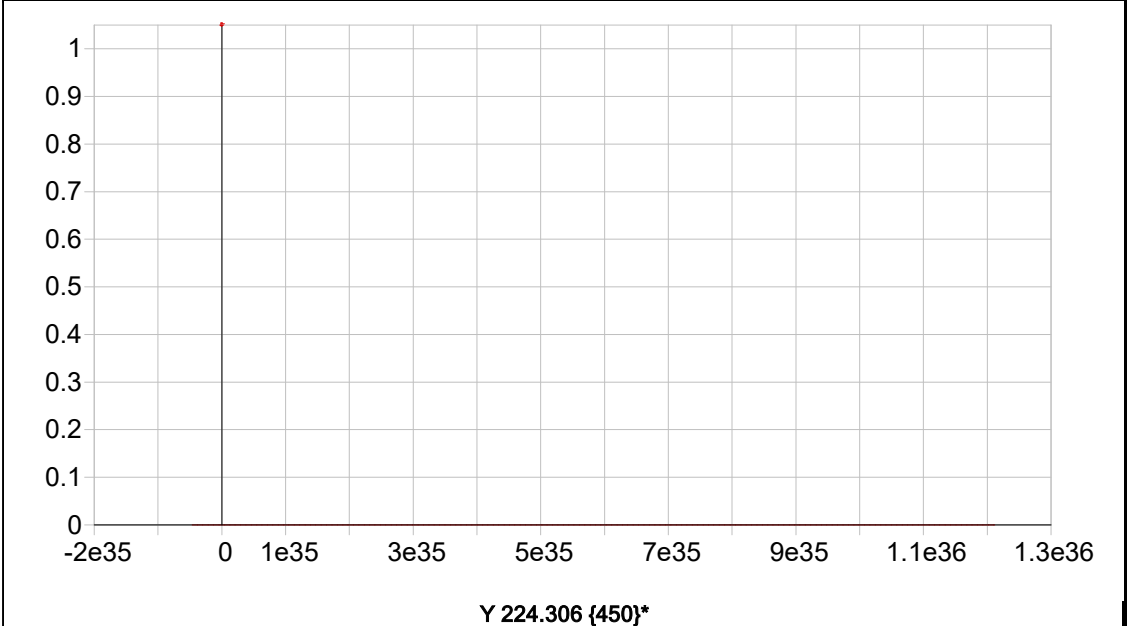


Date of Fit:	8/11/2025 18:32:03	Type of Fit:	Linear	Weighting:	1/Conc
A0 (Offset):	0.000000	Re-Slope:	1.000000		
A1 (Gain):	0.000000	Y-int:	0.000000		
A2 (Curvature):	0.000000				
n (Exponent):	1.000000				
Correlation:	0.000000	Status:	Warning	Zero Gain	
Std Error of Est:	0.000000				
Predicted MDL:	n/a				
Predicted MQL:	n/a				

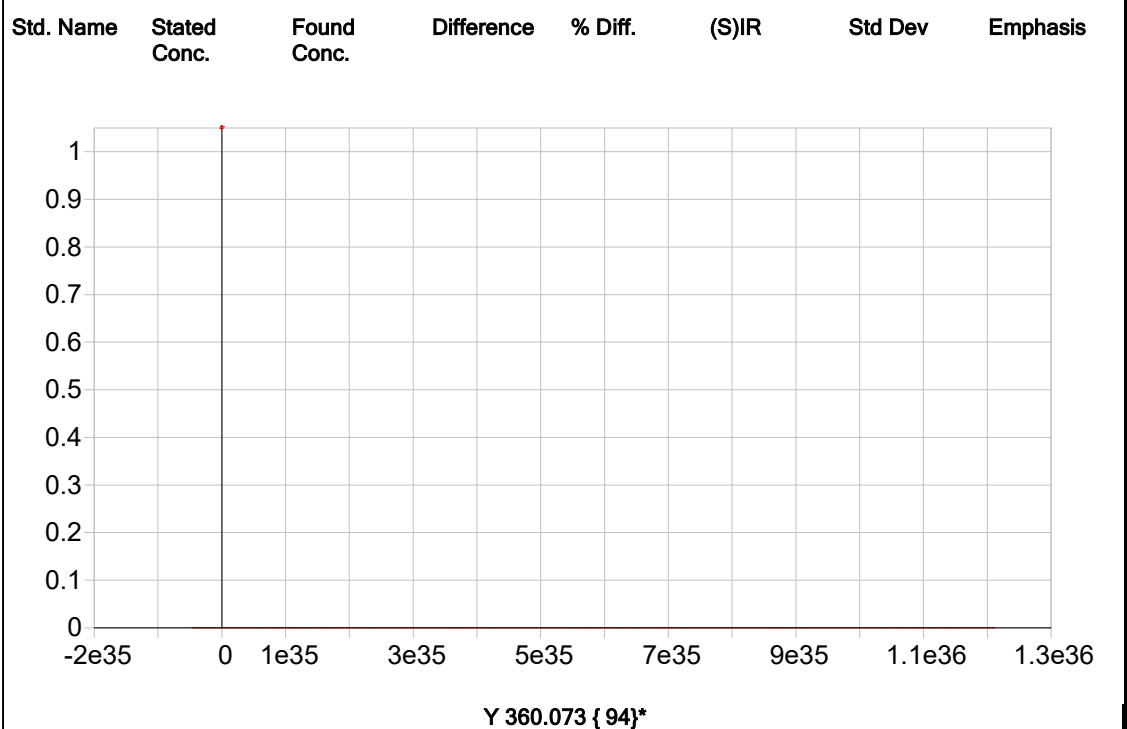


Date of Fit:	<not fit>	Type of Fit:	Linear	Weighting:	1/Conc
A0 (Offset):	0.000000	Re-Slope:	1.000000		
A1 (Gain):	0.000000	Y-int:	0.000000		

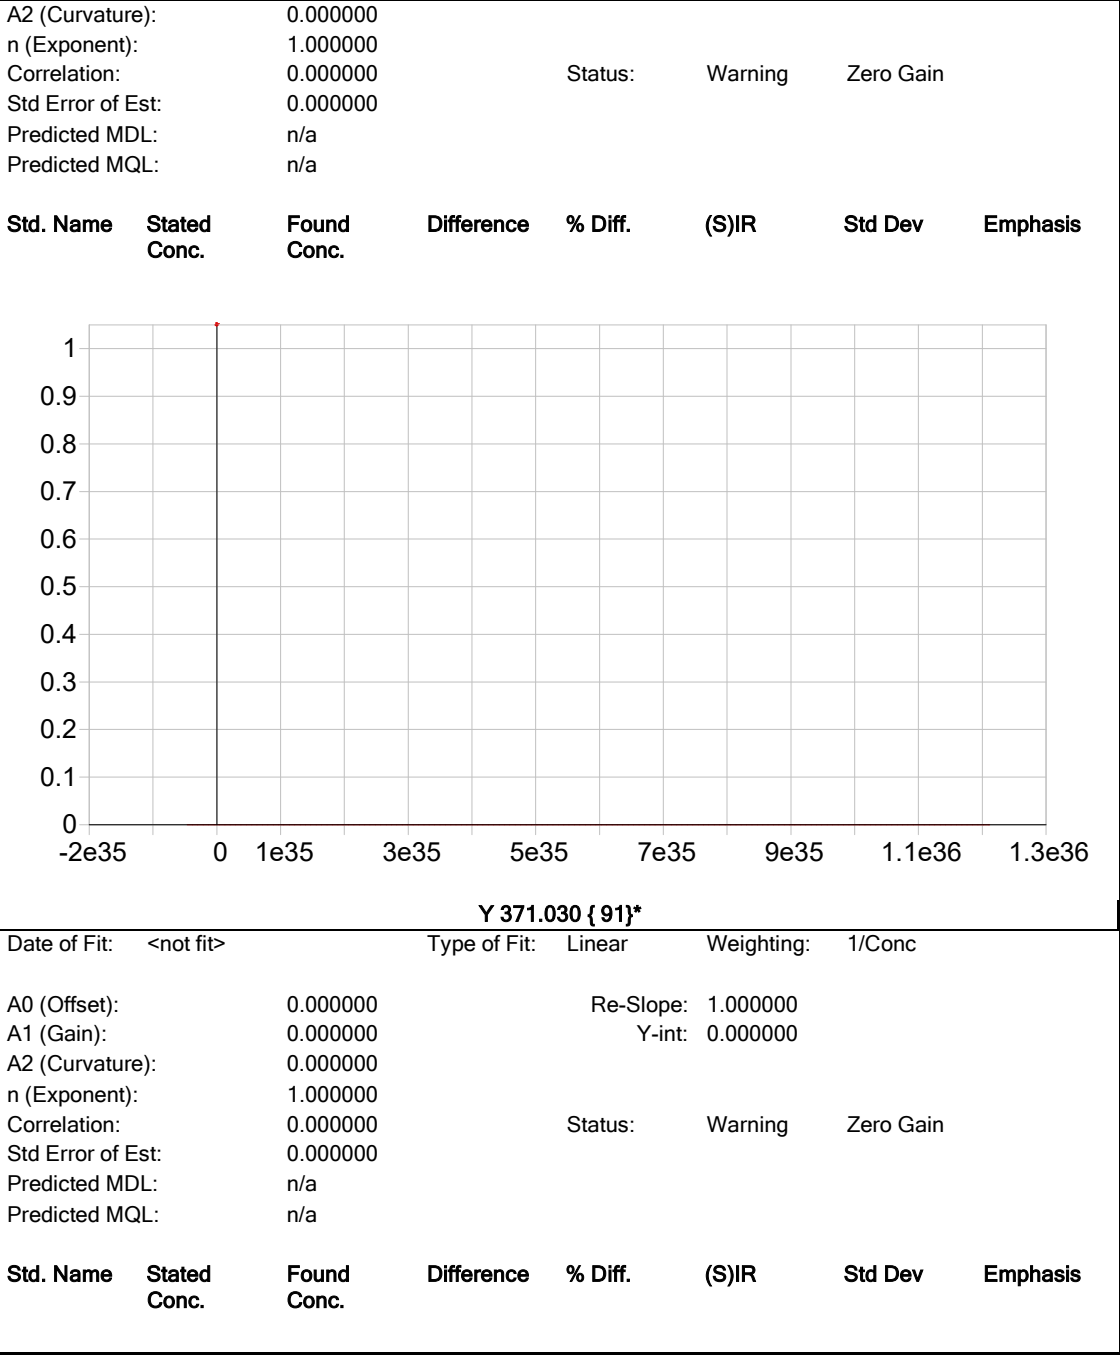

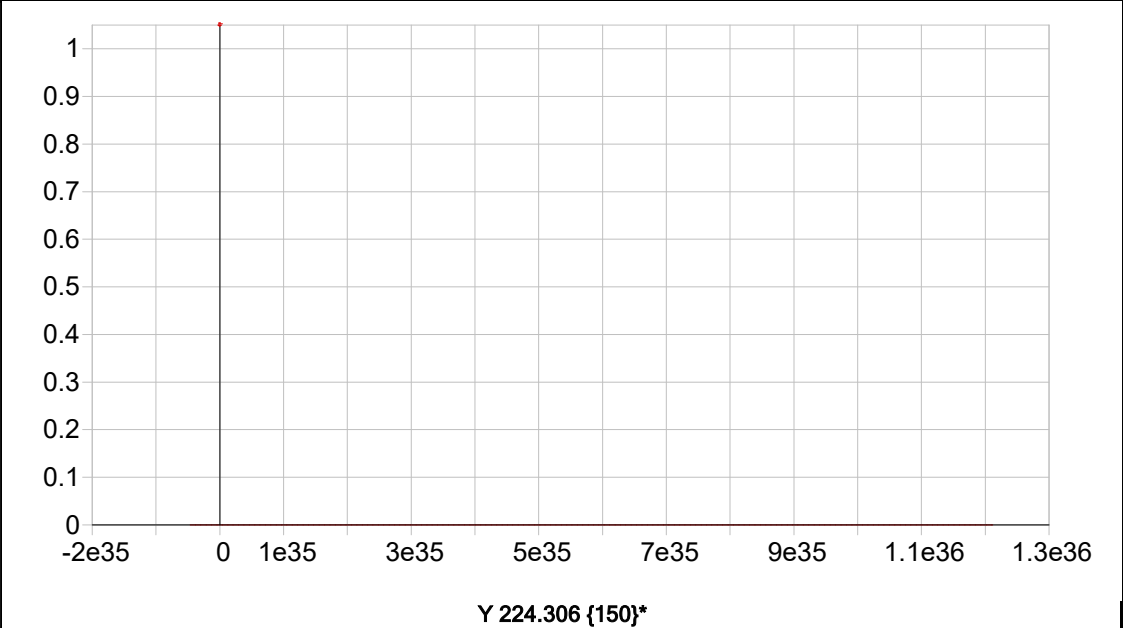

Date of Fit:	<not fit>	Type of Fit:	Linear	Weighting:	1/Conc
A0 (Offset):	0.000000		Re-Slope:	1.000000	
A1 (Gain):	0.000000		Y-int:	0.000000	
A2 (Curvature):	0.000000				
n (Exponent):	1.000000				
Correlation:	0.000000		Status:	Warning	Zero Gain
Std Error of Est:	0.000000				
Predicted MDL:	n/a				
Predicted MQL:	n/a				

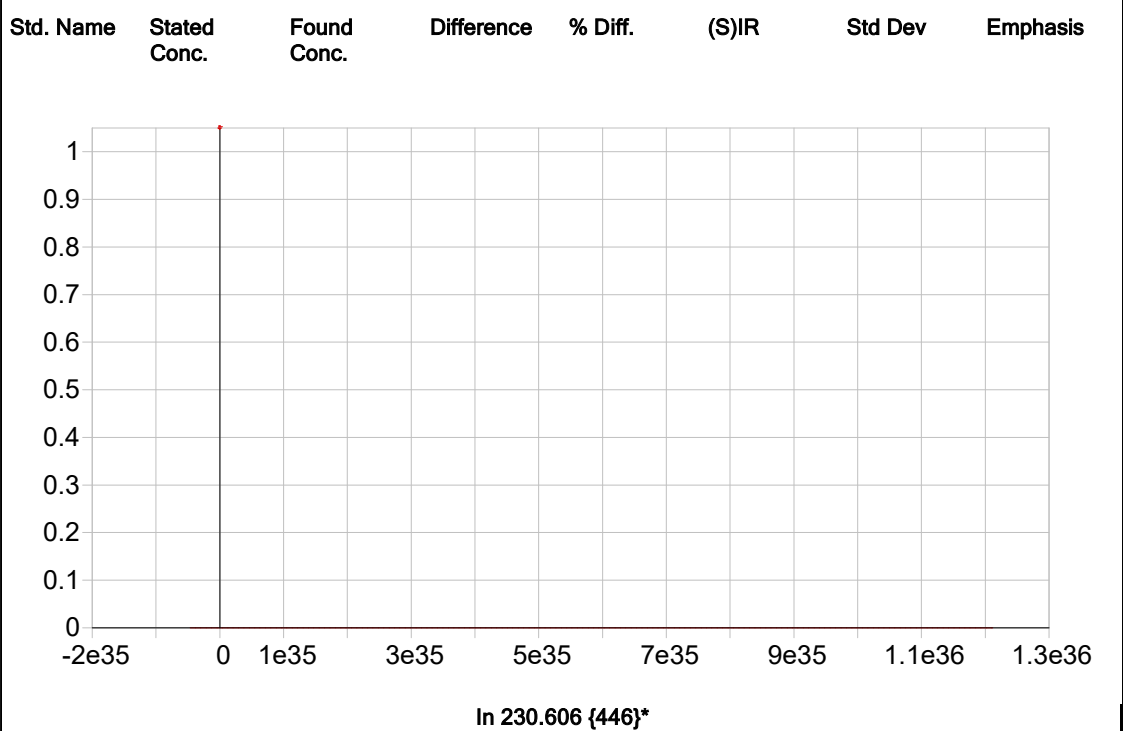

Date of Fit:	<not fit>	Type of Fit:	Linear	Weighting:	1/Conc
A0 (Offset):	0.000000	Re-Slope:	1.000000		
A1 (Gain):	0.000000	Y-int:	0.000000		

A2 (Curvature):		0.000000					
n (Exponent):		1.000000					
Correlation:		0.000000		Status:	Warning	Zero Gain	
Std Error of Est:		0.000000					
Predicted MDL:		n/a					
Predicted MQL:		n/a					
Std. Name	Stated Conc.	Found Conc.	Difference	% Diff.	(S)IR	Std Dev	Emphasis

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

Sample Name: S0 Acquired: 8/11/2025 16:19:09 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	-.00002	.00109	.00008	.00029	.00040	.00063	.08717	-.00076
Stddev	.00003	.00008	.00009	.00005	.00010	.00070	.00152	.00007
%RSD	180.00	7.8287	112.74	17.298	25.130	111.59	1.7462	9.7381
#1	-.00005	.00102	.00013	.00029	.00051	.00119	.08873	-.00067
#2	.00001	.00106	-.00002	.00023	.00040	.00085	.08709	-.00081
#3	-.00002	.00118	.00014	.00033	.00030	-.00016	.08569	-.00079
Elem	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	-.00005	.00303	.00030	.00035	.00078	.00012	.00036	.00014
Stddev	.00013	.00032	.00002	.00010	.00020	.00001	.00013	.00028
%RSD	280.09	10.599	7.6296	29.671	25.379	7.5625	36.859	195.35
#1	.00010	.00267	.00032	.00027	.00095	.00013	.00037	.00006
#2	-.00011	.00330	.00028	.00031	.00056	.00011	.00048	.00045
#3	-.00013	.00310	.00029	.00047	.00081	.00012	.00022	-.00009
Elem	Ni2316	Ag3280	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	-.00015	-.00054	.00215	-.00018	.00696	.00018	.00573	.00087
Stddev	.00012	.00004	.00010	.00027	.00047	.00006	.00010	.00004
%RSD	82.151	7.5290	4.7615	153.67	6.7955	35.225	1.8000	4.6192
#1	-.00002	-.00049	.00214	.00014	.00737	.00011	.00584	.00082
#2	-.00016	-.00055	.00205	-.00033	.00706	.00020	.00570	.00088
#3	-.00026	-.00057	.00225	-.00033	.00644	.00023	.00564	.00090
Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707	Sr4077	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.00030	.00151	.00014	-.00062	.00027	.00800	.00333	
Stddev	.00008	.00034	.00001	.00002	.00006	.00227	.00065	
%RSD	27.080	22.555	8.0708	2.7057	22.796	28.312	19.513	
#1	.00030	.00175	.00014	-.00061	.00032	.00735	.00395	
#2	.00022	.00167	.00016	-.00064	.00020	.01053	.00339	
#3	.00039	.00112	.00013	-.00063	.00028	.00614	.00266	

Sample Name: S0 Acquired: 8/11/2025 16:19:09 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5963.9	103970.	11328.	4515.9	7585.9
Stddev	7.1	143.	29.	9.9	15.9
%RSD	.11890	.13706	.26038	.21833	.20975
#1	5956.0	103940.	11295.	4505.0	7567.9
#2	5965.8	103850.	11351.	4524.2	7598.3
#3	5969.8	104130.	11339.	4518.5	7591.4

Sample Name: S1 Acquired: 8/11/2025 16:23:31 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.00098	.00372	.00244	.00141	.00526	.00841	.31765	.03972
Stddev	.00004	.00006	.00006	.00005	.00005	.00014	.00214	.00019
%RSD	4.0816	1.7160	2.6413	3.5248	.86966	1.7161	.67286	.48013
#1	.00099	.00373	.00239	.00144	.00531	.00847	.31955	.03958
#2	.00102	.00366	.00240	.00136	.00522	.00851	.31533	.03965
#3	.00094	.00378	.00251	.00145	.00524	.00824	.31805	.03994
Elem	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.01748	.11966	.00234	.03151	.01489	.00043	.00923	.02501
Stddev	.00017	.00082	.00001	.00010	.00013	.00002	.00012	.00033
%RSD	.97505	.68744	.55590	.31358	.84321	3.8919	1.2583	1.3000
#1	.01767	.12031	.00234	.03162	.01491	.00041	.00930	.02488
#2	.01742	.11994	.00235	.03143	.01476	.00043	.00930	.02478
#3	.01735	.11873	.00233	.03148	.01500	.00044	.00910	.02539
Elem	Ni2316	Ag3280	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.02439	.00139	.01524	.00466	.10359	.00948	.07229	.14080
Stddev	.00013	.00003	.00018	.00022	.00073	.00010	.00041	.00054
%RSD	.54416	2.0974	1.2064	4.6137	.70786	1.0545	.56239	.38220
#1	.02425	.00141	.01534	.00486	.10428	.00947	.07245	.14070
#2	.02452	.00136	.01536	.00470	.10367	.00939	.07182	.14032
#3	.02439	.00141	.01503	.00443	.10282	.00959	.07259	.14138
Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707	Sr4077	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.00603	.01299	.00140	-.00014	.00079	.02396	.15381	
Stddev	.00012	.00030	.00004	.00005	.00002	.00066	.00031	
%RSD	1.9323	2.3287	2.6206	34.063	2.2565	2.7702	.19963	
#1	.00613	.01307	.00140	-.00014	.00080	.02468	.15415	
#2	.00590	.01266	.00137	-.00009	.00077	.02337	.15373	
#3	.00606	.01325	.00144	-.00018	.00079	.02381	.15355	

Sample Name: S1 Acquired: 8/11/2025 16:23:31 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5809.3	101330.	11249.	4450.5	7190.8
Stddev	6.0	427.	51.	8.1	3.8
%RSD	.10390	.42138	.44895	.18224	.05288
#1	5805.2	101710.	11235.	4459.0	7186.8
#2	5816.3	100870.	11305.	4442.9	7191.1
#3	5806.6	101420.	11207.	4449.5	7194.4

Sample Name: S2 Acquired: 8/11/2025 16:27:53 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.04123	.05139	.15585	.03851	.07558	.12619	3.8417	.27015
Stddev	.00008	.00117	.00037	.00022	.00012	.00074	.0203	.00100
%RSD	.19515	2.2723	.23604	.56679	.16469	.58945	.52891	.37006
#1	.04130	.05262	.15601	.03875	.07557	.12705	3.8205	.26921
#2	.04125	.05125	.15543	.03844	.07546	.12573	3.8610	.27120
#3	.04114	.05029	.15612	.03833	.07571	.12579	3.8434	.27003
Elem	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	1.1650	.23577	.03280	.40562	.13599	.00289	.16822	.04698
Stddev	.0019	.00105	.00010	.00030	.00022	.00001	.00116	.00023
%RSD	.16013	.44629	.30254	.07427	.16171	.40409	.68912	.48014
#1	1.1651	.23456	.03268	.40536	.13619	.00288	.16688	.04685
#2	1.1631	.23641	.03286	.40555	.13575	.00288	.16890	.04724
#3	1.1668	.23635	.03284	.40595	.13604	.00290	.16888	.04685
Elem	Ni2316	Ag3280	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.23761	.04030	.02763	.05112	.98101	.01830	.56203	.55156
Stddev	.00041	.00004	.00018	.00069	.00440	.00011	.00200	.00065
%RSD	.17214	.10671	.64133	1.3443	.44813	.60128	.35578	.11787
#1	.23716	.04027	.02748	.05047	.97743	.01819	.56044	.55218
#2	.23772	.04028	.02783	.05104	.98592	.01841	.56427	.55088
#3	.23796	.04035	.02759	.05184	.97969	.01831	.56137	.55163
Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707	Sr4077	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.11346	.23442	.00268	.01965	.02125	.63896	6.1528	
Stddev	.00025	.00079	.00002	.00013	.00014	.00252	.0248	
%RSD	.22157	.33547	.75605	.66206	.68132	.39394	.40352	
#1	.11339	.23351	.00266	.01975	.02141	.63616	6.1265	
#2	.11325	.23483	.00267	.01950	.02116	.63969	6.1758	
#3	.11374	.23491	.00270	.01970	.02116	.64104	6.1562	

Sample Name: S2 Acquired: 8/11/2025 16:27:53 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5929.4	102250.	11117.	4464.1	7329.5
Stddev	6.6	164.	18.	12.6	11.1
%RSD	.11155	.16020	.16379	.28334	.15137
#1	5936.6	102310.	11133.	4468.7	7341.3
#2	5928.0	102370.	11097.	4473.8	7327.9
#3	5923.7	102060.	11120.	4449.8	7319.3

Sample Name: S3 Acquired: 8/11/2025 16:31:58 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Ti1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.12864	.16466	.48226	.12012	.23552	.39129	11.836	.82539
Stddev	.00009	.00137	.00167	.00019	.00018	.00033	.023	.00363
%RSD	.07212	.83190	.34710	.15416	.07824	.08483	.19440	.44021
#1	.12854	.16602	.48126	.11991	.23534	.39100	11.846	.82720
#2	.12865	.16328	.48132	.12025	.23571	.39123	11.810	.82776
#3	.12873	.16468	.48419	.12020	.23551	.39165	11.852	.82120
Elem	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3.6521	.72151	.10116	1.2623	.41413	.00881	.51800	.14432
Stddev	.0085	.00136	.00027	.0027	.00033	.00007	.00023	.00041
%RSD	.23280	.18898	.26712	.20977	.07897	.78837	.04491	.28275
#1	3.6478	.72290	.10107	1.2611	.41406	.00881	.51813	.14388
#2	3.6466	.72018	.10094	1.2606	.41384	.00874	.51773	.14439
#3	3.6619	.72144	.10146	1.2654	.41449	.00888	.51814	.14469
Elem	Ni2316	Ag3280	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.73717	.12520	.08404	.16003	2.9985	.05910	1.7005	1.7045
Stddev	.00155	.00016	.00047	.00036	.0059	.00011	.0058	.0018
%RSD	.20999	.12413	.55637	.22761	.19566	.18745	.34027	.10703
#1	.73605	.12516	.08397	.16017	2.9994	.05899	1.7013	1.7030
#2	.73651	.12507	.08361	.16030	2.9922	.05910	1.7059	1.7040
#3	.73893	.12537	.08454	.15961	3.0038	.05921	1.6944	1.7065
Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707	Sr4077	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.35483	.72286	.00829	.06284	.06733	1.9483	19.085	
Stddev	.00056	.00075	.00008	.00025	.00028	.0034	.302	
%RSD	.15918	.10398	.93836	.40437	.41102	.17422	1.5835	
#1	.35422	.72344	.00825	.06309	.06743	1.9512	18.968	
#2	.35495	.72201	.00824	.06259	.06702	1.9446	19.429	
#3	.35533	.72312	.00838	.06283	.06754	1.9493	18.859	

Sample Name: S3 Acquired: 8/11/2025 16:31:58 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5885.3	100480.	11207.	4381.5	7148.8
Stddev	2.1	224.	44.	18.8	7.5
%RSD	.03604	.22314	.39257	.42992	.10526
#1	5887.5	100250.	11177.	4370.5	7155.5
#2	5883.3	100690.	11187.	4403.3	7150.3
#3	5885.1	100510.	11257.	4370.8	7140.6

Sample Name: S4 Acquired: 8/11/2025 16:36:01 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.26028	.33855	.96093	.24240	.47144	.77380	23.375	1.6113
Stddev	.00030	.01124	.00107	.00071	.00100	.00021	.174	.0100
%RSD	.11355	3.3190	.11142	.29338	.21111	.02728	.74648	.61925
#1	.25994	.32597	.96072	.24160	.47032	.77378	23.363	1.6223
#2	.26041	.34208	.95998	.24297	.47178	.77359	23.207	1.6029
#3	.26049	.34760	.96209	.24262	.47222	.77401	23.555	1.6086
Elem	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	7.4027	1.4183	.19935	2.5525	.81901	.01766	1.0223	.28634
Stddev	.0040	.0015	.00036	.0015	.00053	.00013	.0013	.00090
%RSD	.05405	.10373	.18236	.06087	.06428	.75351	.12457	.31314
#1	7.4020	1.4200	.19906	2.5539	.81854	.01750	1.0230	.28734
#2	7.3991	1.4175	.19923	2.5508	.81958	.01772	1.0208	.28560
#3	7.4070	1.4173	.19976	2.5528	.81890	.01774	1.0230	.28609
Elem	Ni2316	Ag3280	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	1.4855	.24996	.17282	.31908	5.9758	.12045	3.3223	3.4019
Stddev	.0007	.00014	.00122	.00028	.0019	.00103	.0207	.0088
%RSD	.04967	.05564	.70802	.08688	.03126	.85203	.62440	.25927
#1	1.4863	.24981	.17141	.31883	5.9748	.11931	3.3439	3.3917
#2	1.4848	.25000	.17362	.31904	5.9747	.12130	3.3025	3.4074
#3	1.4853	.25008	.17343	.31938	5.9780	.12075	3.3205	3.4066
Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707	Sr4077	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	.71129	1.4378	.01702	.12826	.13952	3.9015	38.307	
Stddev	.00134	.0008	.00010	.00013	.00045	.0061	.311	
%RSD	.18801	.05262	.57814	.10097	.32357	.15670	.81286	
#1	.71049	1.4384	.01691	.12840	.13905	3.8997	38.638	
#2	.71055	1.4380	.01706	.12815	.13956	3.9083	38.020	
#3	.71283	1.4369	.01710	.12823	.13995	3.8965	38.262	

Sample Name: S4 Acquired: 8/11/2025 16:36:01 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5781.1	99607.	11280.	4332.8	6880.8
Stddev	10.3	71.	71.	7.7	8.2
%RSD	.17892	.07136	.62755	.17875	.11900
#1	5783.1	99688.	11200.	4327.1	6878.7
#2	5770.0	99573.	11335.	4329.6	6873.9
#3	5790.4	99559.	11304.	4341.6	6889.8

Sample Name: S5 Acquired: 8/11/2025 16:40:13 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934	Be2348
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	.55772	.71136	2.0844	.52002	1.0164	1.6630	51.080	3.3903
Stddev	.00268	.01314	.0056	.00188	.0030	.0070	.078	.0076
%RSD	.48001	1.8472	.26870	.36195	.29705	.42262	.15303	.22392

#1	.55584	.71799	2.0791	.51957	1.0143	1.6550	51.031	3.3816
#2	.55653	.69622	2.0840	.51840	1.0152	1.6658	51.039	3.3943
#3	.56078	.71986	2.0902	.52208	1.0199	1.6682	51.170	3.3951

Elem	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404	Mn2576	Mg2790
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	15.947	3.0134	.41781	5.5259	1.7266	.03818	2.1774	.61221
Stddev	.032	.0056	.00031	.0134	.0039	.00002	.0088	.00044
%RSD	.20294	.18736	.07317	.24151	.22787	.06000	.40403	.07140

#1	15.923	3.0077	.41806	5.5162	1.7238	.03819	2.1679	.61174
#2	15.934	3.0189	.41747	5.5205	1.7249	.03820	2.1852	.61259
#3	15.984	3.0137	.41791	5.5412	1.7311	.03815	2.1792	.61231

Elem	Ni2316	Ag3280	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	3.2072	.53771	.38434	.68749	12.690	.26739	7.0322	7.1828
Stddev	.0080	.00080	.00121	.00188	.008	.00083	.0135	.0167
%RSD	.24790	.14839	.31606	.27324	.06540	.31011	.19219	.23194

#1	3.2005	.53783	.38294	.68534	12.683	.26645	7.0169	7.1807
#2	3.2050	.53686	.38511	.68826	12.687	.26801	7.0373	7.1672
#3	3.2160	.53844	.38498	.68885	12.699	.26772	7.0424	7.2003

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707	Sr4077	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	1.5311	3.0950	.03758	.27970	.31151	8.4994	80.215	
Stddev	.0051	.0076	.00014	.00078	.00171	.0396	.839	
%RSD	.33352	.24686	.37923	.27811	.54891	.46585	1.0458	

#1	1.5275	3.0866	.03744	.27906	.31155	8.4569	79.371	
#2	1.5288	3.1015	.03759	.27947	.30978	8.5353	81.049	
#3	1.5369	3.0968	.03772	.28057	.31320	8.5062	80.226	

Sample Name: S5 Acquired: 8/11/2025 16:40:13 Type: Cal
Method: 6010-200.7 NEW(v90) Mode: IR Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5581.1	97017.	11140.	4166.5	6477.0
Stddev	10.6	81.	7.	6.4	14.9
%RSD	.19046	.08393	.06077	.15430	.22959
#1	5587.1	96938.	11148.	4161.3	6488.1
#2	5587.3	97101.	11138.	4173.7	6482.8
#3	5568.8	97011.	11135.	4164.5	6460.1

Sample Name: ICV01 Acquired: 8/11/2025 16:44:24 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICV01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	3.823189	3.792754	3.968291	3.827125	3.949102	7.639916
Stddev	.004363	.078914	.003669	.011574	.015067	.020970
%RSD	.1141107	2.080643	.0924479	.3024219	.3815332	.2744838
#1	3.819608	3.883789	3.971727	3.822847	3.933006	7.655758
#2	3.821912	3.750674	3.968717	3.818299	3.951430	7.647854
#3	3.828048	3.743799	3.964427	3.840229	3.962869	7.616135
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	7.522548	1.1895714	1.896124	19.12728	7.7925741	1.934916
Stddev	.101933	.0012036	.001723	.08426	.0030118	.002669
%RSD	1.355035	.6348990	.0908522	.4405150	.3800016	.1379643
#1	7.623967	.1906288	1.897721	19.21544	.7891738	1.933376
#2	7.523569	.1898237	1.894299	19.11886	.7949062	1.933375
#3	7.420108	.1882617	1.896352	19.04756	.7936423	1.937999
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.9893958	3.929059	1.912762	19.11862	1.936929	1.029706
Stddev	.0017566	.015034	.008450	.07914	.001231	.002096
%RSD	.1775385	.3826234	.4417557	.4139657	.0635367	.2035276
#1	.9877143	3.914289	1.915157	19.20234	1.936373	1.027307
#2	.9892544	3.928546	1.919755	19.10848	1.936075	1.030632
#3	.9912188	3.944342	1.903373	19.04503	1.938340	1.031179
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	18.66091	1.920981	1.923605	19.05108	3.711200	3.913688
Stddev	.14307	.006125	.008742	.08600	.030687	.007820
%RSD	.7666677	.3188588	.4544744	.4514103	.8268651	.1998132
#1	18.49574	1.919584	1.918599	18.95312	3.743895	3.907803
#2	18.74602	1.927684	1.918516	19.08596	3.706684	3.910699
#3	18.74098	1.915675	1.933700	19.11415	3.683022	3.922561

Sample Name: ICV01 Acquired: 8/11/2025 16:44:24 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICV01 Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	3.804580	3.807039	3.646245	F .0038440	F .0297571	F .0030459
Stddev	.006030	.010813	.031005	.0038407	.0003582	.0010927
%RSD	.1584799	.2840327	.8503301	99.91490	1.203877	35.87484

#1	3.811431	3.812774	3.610450	.0011339	.0300639	.0036296
#2	3.802231	3.813777	3.664723	.0082393	.0298440	.0017853
#3	3.800080	3.794567	3.663563	.0021589	.0293634	.0037227

Elem	Sr4077
Units	ppm
Avg	F -.003531
Stddev	.000095
%RSD	2.685642

#1	-.003439
#2	-.003526
#3	-.003629

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5765.850	100030.6	11576.04	4324.791	6953.299
Stddev	23.489	67.4	96.80	10.785	18.249
%RSD	.4073848	.0674157	.8362184	.2493650	.2624443

#1	5792.201	100048.3	11470.33	4335.482	6974.033
#2	5758.239	100087.4	11597.44	4324.975	6946.183
#3	5747.110	99956.1	11660.35	4313.915	6939.680

Sample Name: LLICV01 Acquired: 8/11/2025 16:49:25 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: LLICV01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0193272	.0406581	.0124613	.0221933	.0515041	.1002061	.0963659
Stddev	.0018406	.0005332	.0007658	.0020868	.0021034	.0049519	.0003656
%RSD	9.523323	1.311497	6.145780	9.402980	4.083863	4.941730	.3793446

#1	.0214142	.0408590	.0121075	.0198082	.0533743	.0953502	.0967207
#2	.0179360	.0410617	.0133401	.0236833	.0519109	.1052488	.0959905
#3	.0186313	.0400536	.0119363	.0230882	.0492271	.1000192	.0963866

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0059922	.0059431	2.026263	.0098523	.0295654	.0213329	.0843103
Stddev	.0000844	.0000640	.004156	.0001319	.0000495	.0002140	.0021735
%RSD	1.407938	1.076233	.2050829	1.338988	.1672718	1.003138	2.577925

#1	.0060560	.0059076	2.022928	.0099941	.0296218	.0212931	.0818882
#2	.0058966	.0060169	2.030918	.0098297	.0295296	.0211416	.0849521
#3	.0060241	.0059048	2.024943	.0097331	.0295447	.0215640	.0860906

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0226124	2.122581	.0399246	.0099431	1.768894	.0389164	.0412362
Stddev	.0005082	.014512	.0000867	.0002459	.027452	.0016335	.0003953
%RSD	2.247422	.6837055	.2170732	2.473445	1.551907	4.197496	.9586220

#1	.0226032	2.105885	.0398858	.0097826	1.747923	.0370356	.0416912
#2	.0231252	2.129689	.0400239	.0102263	1.799965	.0399801	.0409766
#3	.0221089	2.132169	.0398640	.0098205	1.758795	.0397336	.0410409

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1.789570	.1014961	.2017666	.0393101	.0386195	.3525602	.0185759
Stddev	.028009	.0013993	.0005481	.0001611	.0013346	.0070291	.0016554
%RSD	1.565134	1.378680	.2716324	.4098126	3.455723	1.993736	8.911446

#1	1.760329	.1027239	.2011413	.0392188	.0401526	.3450142	.0166967
#2	1.816158	.0999726	.2021635	.0394961	.0377170	.3589220	.0198186
#3	1.792223	.1017918	.2019950	.0392154	.0379890	.3537444	.0192123

Sample Name: LLICV01 Acquired: 8/11/2025 16:49:25 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: LLICV01 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.0180102	.0178187	.0203393
Stddev	.0014000	.0009549	.0000951
%RSD	7.773313	5.359008	.4678239

#1	.0165308	.0186436	.0203406
#2	.0181857	.0180398	.0204338
#3	.0193142	.0167726	.0202435

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5906.822	104132.7	11488.24	4424.157	7432.558
Stddev	14.779	430.5	119.47	15.396	10.506
%RSD	.2501987	.4134033	1.039936	.3480032	.1413578

#1	5905.730	104627.8	11382.09	4440.841	7430.274
#2	5892.619	103846.6	11617.62	4410.497	7423.381
#3	5922.116	103923.6	11465.00	4421.132	7444.018

Sample Name: ICB01 Acquired: 8/11/2025 16:54:03 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICB01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000520	-.000038	.0000604	.0012899	.0015037	-.002667	-.002541
Stddev	.000245	.002863	.0002289	.0012565	.0012094	.004581	.001442
%RSD	47.07807	7480.295	378.7093	97.40873	80.42677	171.7822	56.74654
#1	-.000239	-.002604	-.000054	-.000151	.0002091	.000708	-.002220
#2	-.000686	-.000560	.000324	.002161	.0016976	-.000827	-.001287
#3	-.000635	.003050	-.000089	.001860	.0026044	-.007882	-.004117
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000536	-.000008	.0025129	-.000239	-.000012	-.000056	-.014539
Stddev	.0000449	.000035	.0042596	.000217	.000104	.000260	.004326
%RSD	83.75706	439.7006	169.5048	90.55513	859.4020	462.2146	29.75574
#1	.0000211	.000030	-.000654	-.000484	-.000100	.000126	-.017264
#2	.0000349	-.000040	.007356	-.000162	.000102	-.000354	-.016802
#3	.0001049	-.000014	.000837	-.000071	-.000038	.000059	-.009550
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0003491	-.010603	.0002320	.0001146	-.018527	-.000232	.0022770
Stddev	.0001967	.009470	.0002396	.0004510	.025663	.000857	.0002796
%RSD	56.33323	89.31120	103.2808	393.6321	138.5170	369.3476	12.27755
#1	.0005545	-.016631	.0000791	.0004831	-.016510	.000741	.0023552
#2	.0001626	-.015491	.0005081	-.000388	-.045138	-.000877	.0019667
#3	.0003302	.000312	.0001088	.000249	.006068	-.000560	.0025092
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0016430	.0030079	-.000040	.0011136	-.000855	.0043241	-.000560
Stddev	.0176730	.0009519	.000127	.0002437	.000755	.0025418	.000445
%RSD	1075.674	31.64822	314.0131	21.88248	88.37515	58.78228	79.41840
#1	.0101870	.0039906	-.000030	.0012594	-.001111	.0044422	-.001070
#2	-.018678	.0029431	-.000172	.0012491	-.000005	.0068048	-.000367
#3	.013420	.0020900	.000081	.0008323	-.001449	.0017253	-.000245

Sample Name: ICB01 Acquired: 8/11/2025 16:54:03 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICB01 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.0025385	-.000194	-.000174
Stddev	.0008382	.000986	.000039
%RSD	33.02009	509.0201	22.65132

#1	.0018575	.000509	-.000206
#2	.0034746	-.001320	-.000185
#3	.0022833	.000230	-.000130

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5859.195	103450.6	11449.42	4449.047	7384.583
Stddev	6.614	320.8	76.35	11.014	14.926
%RSD	.1128803	.3100867	.6668413	.2475527	.2021193

#1	5852.388	103080.8	11368.80	4439.609	7367.760
#2	5859.597	103653.3	11458.82	4461.148	7389.752
#3	5865.598	103617.8	11520.63	4446.383	7396.238

Sample Name: CRI01 Acquired: 8/11/2025 16:58:22 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CRI01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0182384	.0382725	.0114338	.0216939	.0493698	.0931926	.0924075
Stddev	.0027281	.0009497	.0006480	.0009877	.0005665	.0050581	.0002981
%RSD	14.95811	2.481474	5.667226	4.553066	1.147460	5.427611	.3226374
#1	.0160164	.0393682	.0121598	.0225437	.0489455	.0966298	.0925180
#2	.0174155	.0377624	.0112277	.0206102	.0500131	.0873845	.0920699
#3	.0212832	.0376867	.0109140	.0219278	.0491507	.0955634	.0926347
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0059574	.0055529	1.986173	.0096312	.0289639	.0206728	.0836677
Stddev	.0000492	.0000274	.010138	.0002254	.0001553	.0005389	.0048134
%RSD	.8256057	.4930048	.5104253	2.339930	.5362582	2.606898	5.753032
#1	.0059857	.0055284	1.993840	.0097336	.0291305	.0212796	.0792756
#2	.0059006	.0055824	1.990000	.0093728	.0288230	.0202497	.0888136
#3	.0059859	.0055477	1.974679	.0097871	.0289382	.0204892	.0829139
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0210481	2.072771	.0389875	.0096452	1.782345	.0361439	.0394225
Stddev	.0002058	.006730	.0003168	.0004830	.012140	.0003056	.0001005
%RSD	.9780122	.3246639	.8126958	5.007261	.6811475	.8454621	.2548290
#1	.0208351	2.066271	.0393326	.0096014	1.776105	.0364366	.0395068
#2	.0210634	2.072335	.0389203	.0091857	1.774594	.0361683	.0394495
#3	.0212459	2.079709	.0387097	.0101486	1.796337	.0358269	.0393114
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1.846688	.0990964	.2013851	.0381085	.0361847	.3578565	.0171538
Stddev	.041973	.0005097	.0006534	.0003496	.0016184	.0082294	.0026957
%RSD	2.272899	.5143140	.3244379	.9173071	4.472611	2.299650	15.71507
#1	1.810123	.0994815	.2006826	.0382094	.0346360	.3657718	.0171331
#2	1.892521	.0985184	.2019746	.0383965	.0378648	.3584524	.0144685
#3	1.837420	.0992892	.2014982	.0377195	.0360535	.3493453	.0198598

Sample Name: CRI01 Acquired: 8/11/2025 16:58:22 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CRI01 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.0148011	.0172413	.0192393
Stddev	.0008029	.0000088	.0000465
%RSD	5.424848	.0512400	.2415815
#1	.0153536	.0172411	.0192527
#2	.0138800	.0172325	.0192776
#3	.0151697	.0172502	.0191876

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5903.184	103679.5	11551.17	4437.507	7412.635
Stddev	9.746	106.7	14.57	10.141	7.254
%RSD	.1651013	.1028855	.1261275	.2285272	.0978627
#1	5902.185	103786.8	11567.98	4436.900	7411.485
#2	5893.976	103678.4	11542.07	4447.937	7406.024
#3	5913.391	103573.4	11543.47	4427.683	7420.395

Sample Name: ICSA01 Acquired: 8/11/2025 17:02:36 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSA01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0099573	.0033407	-.006749	.0051938	-.002608	237.7428
Stddev	.0033044	.0012849	.001751	.0029487	.002443	.0564
%RSD	33.18527	38.46280	25.95109	56.77287	93.70599	.0237329
#1	.0135362	.0041117	-.005931	.0021719	-.003144	237.8013
#2	.0070222	.0018574	-.005555	.0053461	-.004738	237.6887
#3	.0093136	.0040531	-.008759	.0080633	.000059	237.7384
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001520	.0012859	.0019152	227.2125	.0568422	.0017036
Stddev	.001170	.0000806	.0000460	.3107	.0001140	.0002566
%RSD	76.94480	6.271361	2.402711	.1367367	.2004948	15.06515
#1	-.000608	.0011966	.0019555	227.4382	.0568630	.0014308
#2	-.002839	.0013075	.0018651	226.8581	.0567192	.0017396
#3	-.001113	.0013535	.0019252	227.3412	.0569443	.0019402
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000680	97.44913	.0091276	239.7171	.0052475	.0017682
Stddev	.000611	.50975	.0002534	.7434	.0005755	.0008170
%RSD	89.86909	.5230945	2.775909	.3101147	10.96662	46.20330
#1	-.000853	97.06539	.0094057	239.6987	.0053596	.0012422
#2	-.001185	98.02753	.0090673	238.9831	.0046242	.0027094
#3	-.000001	97.25448	.0089099	240.4696	.0057586	.0013530
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1031196	.0021542	.0021372	.0923462	.0318949	.0004408
Stddev	.0098228	.0014696	.0002453	.0235304	.0017460	.0004258
%RSD	9.525594	68.22038	11.47871	25.48065	5.474302	96.60422
#1	.0926794	.0030294	.0018651	.0732772	.0304386	.0004253
#2	.1045008	.0004575	.0023415	.0851189	.0338305	.0008742
#3	.1121787	.0029756	.0022050	.1186426	.0314155	.0000230

Sample Name: ICSA01 Acquired: 8/11/2025 17:02:36 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSA01 Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.002795	-.006344	.0200433	.0080835	-.007840	F -.027224
Stddev	.000571	.000734	.0047415	.0043914	.002593	.000773
%RSD	20.43297	11.57358	23.65643	54.32591	33.07200	2.837667

#1	-.003190	-.006215	.0221798	.0104739	-.009137	-.026438
#2	-.003056	-.005682	.0146094	.0030154	-.009528	-.027251
#3	-.002140	-.007134	.0233406	.0107612	-.004854	-.027983

Elem	Sr4077
Units	ppm
Avg	.0005467
Stddev	.0003728
%RSD	68.19632

#1	.0009768
#2	.0003167
#3	.0003465

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5290.170	90894.40	11215.83	3988.409	6082.158
Stddev	3.470	104.35	67.16	10.222	2.048
%RSD	.0655971	.1148002	.5987856	.2563011	.0336694

#1	5286.237	91009.23	11164.23	3979.865	6080.231
#2	5292.802	90868.58	11291.76	3999.734	6081.935
#3	5291.470	90805.38	11191.49	3985.628	6084.308

Sample Name: ICSAB01 Acquired: 8/11/2025 17:06:48 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSAB01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1034765	.1076761	.0388756	.0511823	.5794260	236.1917
Stddev	.0028345	.0022113	.0019500	.0019333	.0031403	.5368
%RSD	2.739320	2.053682	5.016107	3.777202	.5419668	.2272874
#1	.1008360	.1095907	.0370135	.0522174	.5776436	235.9845
#2	.1064717	.1081819	.0387101	.0523775	.5830519	235.7894
#3	.1031217	.1052557	.0409031	.0489518	.5775824	236.8013
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4641960	.4636596	.9450663	225.3088	.5343433	.4768355
Stddev	.0011805	.0021975	.0017952	.4620	.0010219	.0009953
%RSD	.2543192	.4739504	.1899566	.2050508	.1912374	.2087212
#1	.4652381	.4641686	.9431366	225.5470	.5350621	.4757302
#2	.4629139	.4612523	.9453756	224.7763	.5331735	.4771155
#3	.4644360	.4655580	.9466869	225.6031	.5347943	.4776607
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.4633547	97.86339	.4707643	238.1925	.9491282	.2067365
Stddev	.0007017	.30566	.0018809	.5710	.0023873	.0007015
%RSD	.1514333	.3123303	.3995390	.2397220	.2515277	.3393244
#1	.4625609	98.21597	.4703113	238.3879	.9463723	.2073076
#2	.4636112	97.67314	.4691512	237.5495	.9504535	.2059535
#3	.4638921	97.70106	.4728303	238.6402	.9505589	.2069486
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0457270	.4584531	.9871384	-.010287	F .8230100	.9136288
Stddev	.0206094	.0024336	.0011767	.032250	.0078853	.0189011
%RSD	45.07051	.5308268	.1192008	313.4861	.9581061	2.068797
#1	.0549830	.4573373	.9859291	.009502	.8166283	.8943359
#2	.0221124	.4567775	.9872066	.007137	.8205765	.9144385
#3	.0600856	.4612445	.9882795	-.047501	.8318252	.9321121

Sample Name: ICSAB01 Acquired: 8/11/2025 17:06:48 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSAB01 Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.8975367	F .8210786	.8507475	F .0074286	F -.002678	F -.029091
Stddev	.0191125	.0038317	.0084853	.0006996	.004532	.000905
%RSD	2.129437	.4666634	.9973917	9.417573	169.2471	3.111346
#1	.8783846	.8212774	.8605156	.0072205	-.001577	-.030126
#2	.8976161	.8171514	.8452012	.0068567	-.007658	-.028449
#3	.9166093	.8248070	.8465257	.0082086	.001203	-.028697

Elem	Sr4077
Units	ppm
Avg	F -.000346
Stddev	.000041
%RSD	11.78951
#1	-.000310
#2	-.000390
#3	-.000338

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5326.826	91282.33	11345.62	3973.606	6140.512
Stddev	6.704	217.12	49.94	18.182	9.965
%RSD	.1258465	.2378568	.4402013	.4575805	.1622852
#1	5326.305	91181.12	11339.14	3954.684	6139.918
#2	5320.398	91531.58	11398.48	3990.946	6130.857
#3	5333.775	91134.29	11299.22	3975.187	6150.761

Sample Name: ICSADLX20 Acquired: 8/11/2025 17:10:49 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSA01DLX20 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001248	.0011226	-.000487	.0015372	.0008572	11.68747	-.003012
Stddev	.002073	.0008944	.001038	.0006863	.0013250	.01628	.001111
%RSD	166.1369	79.67901	213.0094	44.64758	154.5763	.1392995	36.89408

#1	-.000540	.0020581	.000638	.0010395	.0021959	11.68334	-.001734
#2	-.003582	.0010338	-.000693	.0012519	-.000454	11.67365	-.003551
#3	.000379	.0002758	-.001407	.0023202	.000829	11.70542	-.003750

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0001739	.0000189	11.63884	.0026164	-.000080	-.000030	4.579321
Stddev	.0000628	.0000484	.02697	.0001025	.000161	.000218	.015531
%RSD	36.13704	256.5368	.2317325	3.917270	200.9253	737.1601	.3391489

#1	.0001723	-.000035	11.64299	.0027248	.000104	-.000115	4.566911
#2	.0002376	.000032	11.66350	.0025210	-.000147	.000218	4.596737
#3	.0001119	.000059	11.61004	.0026034	-.000197	-.000192	4.574315

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0002943	12.11622	-.000006	-.000117	-.060678	.0001500	-.000122
Stddev	.0001766	.01062	.000297	.000341	.004176	.0009814	.000095
%RSD	59.98459	.0876119	5187.746	292.4703	6.881905	654.1319	78.15937

#1	.0002488	12.12761	-.000349	-.000121	-.058743	.0007373	-.000105
#2	.0001450	12.10659	.000173	-.000455	-.057821	-.000983	-.000224
#3	.0004892	12.11447	.000159	.000227	-.065471	.000696	-.000036

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.123113	-.002659	-.000290	.0000991	-.000738	.0092011	-.001659
Stddev	.027191	.000392	.000135	.0001667	.001078	.0102568	.001654
%RSD	22.08594	14.75246	46.52607	168.1299	145.9490	111.4737	99.72776

#1	-.118870	-.003028	-.000261	.0000652	.000103	.0142715	-.000252
#2	-.152176	-.002247	-.000436	-.000048	-.001953	.0159353	-.003481
#3	-.098293	-.002704	-.000172	.000280	-.000365	-.002603	-.001244

Sample Name: ICSADLX20 Acquired: 8/11/2025 17:10:49 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSA01DLX20 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	-.002221	-.006089	-.000118
Stddev	.000472	.000736	.000023
%RSD	21.27008	12.08143	19.39951

#1	-.001841	-.006880	-.000094
#2	-.002072	-.005425	-.000120
#3	-.002750	-.005964	-.000139

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5796.107	101535.5	11339.13	4391.200	7189.125
Stddev	13.673	251.6	25.38	11.067	5.826
%RSD	.2359067	.2478044	.2238702	.2520367	.0810397

#1	5805.052	101373.2	11331.03	4399.596	7194.039
#2	5802.901	101408.0	11367.58	4395.345	7190.646
#3	5780.367	101825.3	11318.79	4378.658	7182.689

Sample Name: ICSABDLX20 Acquired: 8/11/2025 17:15:06 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSAB01DLX20 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0055474	.0067206	.0014606	.0034784	.0284537	11.73579	.0196463
Stddev	.0011881	.0018351	.0005407	.0027422	.0005182	.04349	.0009423
%RSD	21.41774	27.30550	37.02096	78.83676	1.821264	.3705721	4.796298
#1	.0056974	.0051875	.0012553	.0057534	.0280354	11.71257	.0207337
#2	.0042914	.0062204	.0020740	.0004335	.0282923	11.70883	.0190692
#3	.0066534	.0087539	.0010527	.0042482	.0290334	11.78596	.0191361
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0242692	.0468542	11.68817	.0274859	.0235315	.0248518	4.679591
Stddev	.0001604	.0000254	.06766	.0004995	.0002276	.0003117	.014598
%RSD	.6608943	.0541779	.5788596	1.817405	.9669905	1.254166	.3119403
#1	.0244354	.0468380	11.70385	.0271109	.0235478	.0244925	4.669524
#2	.0242569	.0468412	11.61405	.0272937	.0232963	.0250134	4.672917
#3	.0241153	.0468835	11.74661	.0280529	.0237505	.0250495	4.696333
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0246960	12.15209	.0475960	.0097140	-.084464	.0217290	.0478598
Stddev	.0002873	.04054	.0000578	.0003173	.008106	.0012473	.0001816
%RSD	1.163506	.3335861	.1213646	3.266735	9.596382	5.740287	.3794344
#1	.0250048	12.13677	.0476601	.0099758	-.089762	.0203913	.0479654
#2	.0246467	12.12144	.0475481	.0098052	-.088497	.0228602	.0476501
#3	.0244365	12.19805	.0475798	.0093611	-.075133	.0219354	.0479639
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.134821	.0478687	.0529165	.0504367	.0501527	.0614446	.0007121
Stddev	.032970	.0007336	.0003849	.0005855	.0013647	.0076584	.0007621
%RSD	24.45447	1.532533	.7274532	1.160921	2.721141	12.46393	107.0189
#1	-.168192	.0479099	.0531230	.0510891	.0517088	.0629402	.0009609
#2	-.102268	.0471153	.0524724	.0499568	.0495898	.0682449	.0013187
#3	-.134001	.0485808	.0531541	.0502642	.0491593	.0531488	-.000143

Sample Name: ICSABDLX20 Acquired: 8/11/2025 17:15:06 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: ICSAB01DLX20 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	-.003488	-.006014	-.000195
Stddev	.000918	.001815	.000063
%RSD	26.31610	30.17123	32.30954

#1	-.003039	-.005392	-.000227
#2	-.004544	-.004593	-.000123
#3	-.002881	-.008059	-.000237

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5771.992	100032.4	11421.83	4373.293	7124.314
Stddev	8.323	307.6	81.72	23.545	11.967
%RSD	.1441993	.3074866	.7154563	.5383725	.1679724

#1	5772.291	100116.7	11352.74	4346.506	7125.371
#2	5780.161	100289.1	11512.03	4390.709	7135.718
#3	5763.523	99691.5	11400.71	4382.665	7111.854

Sample Name: CCV01 Acquired: 8/11/2025 17:19:18 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCV01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.945025	4.884199	4.839102	4.946836	4.890499	9.604358	9.490171
Stddev	.022663	.045931	.015596	.017432	.011721	.022124	.174457
%RSD	.4583054	.9404014	.3222858	.3523845	.2396750	.2303581	1.838288

#1	4.926435	4.832930	4.833249	4.927363	4.881242	9.580856	9.418851
#2	4.938369	4.921593	4.827278	4.952159	4.886576	9.624783	9.688989
#3	4.970271	4.898073	4.856777	4.960986	4.903678	9.607435	9.362674

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2388714	2.444038	23.98855	.9720986	2.428213	1.237712	4.850584
Stddev	.0026331	.005247	.02954	.0024159	.005514	.002741	.065593
%RSD	1.102294	.2146930	.1231613	.2485224	.2270839	.2214729	1.352264

#1	.2358389	2.442898	23.96669	.9738998	2.426138	1.236727	4.924263
#2	.2405785	2.439455	24.02216	.9693532	2.424036	1.235599	4.798548
#3	.2401967	2.449762	23.97679	.9730427	2.434463	1.240809	4.828940

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.400595	23.85160	2.443374	1.206454	24.11335	2.409314	2.436321
Stddev	.006448	.11428	.005661	.001271	.33419	.006662	.006301
%RSD	.2686004	.4791438	.2316864	.1053125	1.385918	.2765092	.2586370

#1	2.401733	23.73038	2.440877	1.206189	24.48113	2.403469	2.438618
#2	2.393654	23.95737	2.439392	1.205337	23.82828	2.416568	2.441152
#3	2.406398	23.86706	2.449855	1.207836	24.03064	2.407906	2.429194

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	23.99550	4.763648	4.911540	4.876549	4.797872	4.840254	4.898428
Stddev	.26998	.054717	.010815	.013527	.006357	.033477	.017660
%RSD	1.125132	1.148643	.2201890	.2773917	.1324913	.6916458	.3605168

#1	24.30627	4.700952	4.903524	4.872127	4.803779	4.876774	4.917329
#2	23.81881	4.801770	4.907255	4.865786	4.791145	4.811019	4.895603
#3	23.86142	4.788222	4.923840	4.891734	4.798691	4.832971	4.882351

Sample Name: CCV01 Acquired: 8/11/2025 17:19:18 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCV01 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	4.868460	4.747737	4.880364
Stddev	.014747	.014377	.097554
%RSD	.3029081	.3028177	1.998900

#1	4.858468	4.755685	4.772026
#2	4.861516	4.731140	4.961250
#3	4.885398	4.756384	4.907817

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5632.981	99676.91	11494.16	4286.208	6690.036
Stddev	8.708	386.01	89.30	12.291	7.936
%RSD	.1545814	.3872661	.7768881	.2867592	.1186226

#1	5637.459	99235.47	11594.37	4273.096	6693.362
#2	5638.537	99844.19	11423.02	4288.060	6695.766
#3	5622.945	99951.06	11465.09	4297.468	6680.978

Sample Name: CCB01 Acquired: 8/11/2025 17:23:29 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCB01 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001829	-.000749	.0001979	.0022283	.0018598	-.001315	-.002363
Stddev	.001132	.001339	.0004917	.0013459	.0018671	.005923	.001076
%RSD	61.91280	178.7523	248.4526	60.40192	100.3933	450.5960	45.51647
#1	-.001302	-.002290	.0006587	.0007219	.0001561	-.001689	-.003131
#2	-.001056	-.000085	-.000320	.0033125	.0015674	.004787	-.002824
#3	-.003128	.000128	.000255	.0026505	.0038558	-.007042	-.001134
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000414	-.000020	-.012283	-.000061	.0001416	.0000030	-.018980
Stddev	.0000598	.000045	.015590	.000166	.0000888	.0002044	.004806
%RSD	144.3247	221.7071	126.9275	270.7191	62.69759	6927.256	25.31930
#1	.0001080	.000013	-.005809	.000129	.0000607	.0002078	-.024505
#2	.0000237	-.000002	-.000972	-.000175	.0001275	-.000201	-.015766
#3	-.000008	-.000072	-.030067	-.000138	.0002366	.000002	-.016670
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0005051	-.009190	-.000255	-.000408	-.062701	.0002620	.0018188
Stddev	.0002637	.017463	.000314	.000649	.004001	.0023268	.0000452
%RSD	52.19956	190.0251	123.3356	159.1412	6.380700	887.9869	2.482255
#1	.0002365	.008827	-.000166	-.000766	-.061112	.0023041	.0018445
#2	.0007635	-.026040	.000006	-.000799	-.059738	.0007531	.0018452
#3	.0005153	-.010356	-.000603	.000341	-.067252	-.002271	.0017667
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.071942	.0011578	.0001851	.0009690	-.000396	-.003240	.0006094
Stddev	.036271	.0002827	.0001349	.0004084	.000581	.006167	.0013210
%RSD	50.41672	24.41440	72.87328	42.14847	146.8279	190.3153	216.7776
#1	-.110467	.0011486	.0000811	.0007043	-.000330	.003852	.0012335
#2	-.066908	.0014450	.0001367	.0014394	.000150	-.006239	-.000908
#3	-.038452	.0008799	.0003375	.0007633	-.001007	-.007334	.001503

Sample Name: CCB01 Acquired: 8/11/2025 17:23:29 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCB01 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.0016294	-.001350	-.000063
Stddev	.0025332	.001559	.000028
%RSD	155.4661	115.5244	43.82799

#1	.0029856	-.001095	-.000084
#2	.0031959	-.003020	-.000032
#3	-.001293	.000066	-.000074

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5803.046	103396.4	11316.01	4402.324	7308.170
Stddev	9.312	507.0	61.77	22.562	6.339
%RSD	.1604750	.4903493	.5458274	.5125059	.0867413

#1	5792.296	103152.5	11365.43	4381.908	7303.793
#2	5808.223	103979.2	11335.82	4426.548	7315.439
#3	5808.620	103057.4	11246.76	4398.516	7305.276

Sample Name: Q2759-04 Acquired: 8/11/2025 17:27:48 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0122297	.0003199	2.623958	.0093891	.0124143	2.686036
Stddev	.0022953	.0010591	.001560	.0018267	.0008257	.018942
%RSD	18.76818	331.0746	.0594631	19.45557	6.651290	.7052184
#1	.0113363	-.000549	2.623385	.0086958	.0131067	2.697531
#2	.0148373	.000009	2.625724	.0114610	.0115004	2.664172
#3	.0105154	.001500	2.622766	.0080106	.0126356	2.696404
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.015043	.0004049	.0081061	54.90299	.0470783	.0179909
Stddev	.005300	.0000214	.0000828	.14611	.0002222	.0002917
%RSD	.1320140	5.290907	1.021499	.2661202	.4719753	1.621554
#1	4.016572	.0004124	.0080106	54.94989	.0473178	.0183224
#2	4.019410	.0003807	.0081505	54.73919	.0468788	.0178773
#3	4.009146	.0004215	.0081573	55.01989	.0470384	.0177731
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.3062656	15.96943	.3343975	9.422921	.0143961	.0016231
Stddev	.0006509	.14492	.0008869	.057125	.0000854	.0005380
%RSD	.2125277	.9074601	.2652147	.6062294	.5932396	33.14670
#1	.3059005	16.00825	.3346475	9.370929	.0143336	.0011164
#2	.3058792	16.09099	.3351326	9.413764	.0144935	.0021878
#3	.3070171	15.80906	.3334125	9.484071	.0143614	.0015652
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	124.7202	.0238523	5.313314	12.45731	.1046051	.0097386
Stddev	1.4293	.0007836	.007160	.11564	.0010616	.0000482
%RSD	1.146004	3.285102	.1347603	.9282532	1.014815	.4947438
#1	124.9562	.0247249	5.320407	12.45794	.1055761	.0096833
#2	126.0168	.0236232	5.313447	12.57263	.1034717	.0097718
#3	123.1876	.0232089	5.306089	12.34136	.1047675	.0097607

Sample Name: Q2759-04 Acquired: 8/11/2025 17:27:48 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0079020	.1168695	F 27.41097	1.472296	F 46.06726	.0269881
Stddev	.0002632	.0015378	.24575	.008766	.20648	.0013864
%RSD	3.331314	1.315826	.8965538	.5954211	.4482048	5.137016

#1	.0077727	.1176652	27.41204	1.467433	45.85801	.0281383
#2	.0077285	.1178464	27.65618	1.467040	46.07293	.0254487
#3	.0082049	.1150968	27.16468	1.482416	46.27084	.0273774

Elem	Sr4077
Units	ppm
Avg	.3307083
Stddev	.0001671
%RSD	.0505338

#1	.3309011
#2	.3306200
#3	.3306039

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5729.140	100264.1	11974.89	4260.727	6916.023
Stddev	14.609	189.8	113.76	18.104	12.377
%RSD	.2550030	.1893436	.9499757	.4249125	.1789559

#1	5725.671	100325.3	11994.30	4243.562	6909.566
#2	5745.172	100051.2	12077.70	4258.977	6930.292
#3	5716.577	100415.8	11852.68	4279.643	6908.209

Sample Name: Q2801-01 Acquired: 8/11/2025 17:31:56 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0976600	-.026349	.1868467	.0053580	-.008709	97.41938	.4586247
Stddev	.0002628	.002802	.0006070	.0034800	.002372	.22798	.0010803
%RSD	.2690768	10.63330	.3248692	64.95058	27.24101	.2340203	.2355569

#1	.0976672	-.029083	.1861462	.0026724	-.011345	97.18952	.4573787
#2	.0979191	-.026481	.1871781	.0041121	-.008038	97.64543	.4593004
#3	.0973937	-.023484	.1872160	.0092895	-.006745	97.42319	.4591949

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0089387	.0057063	36.17534	.1786454	.0873436	.1567014	232.5924
Stddev	.0000594	.0002041	.06401	.0006685	.0003783	.0002633	1.7564
%RSD	.6640372	3.577182	.1769571	.3742323	.4331368	.1680321	.7551280

#1	.0089730	.0058436	36.10998	.1788348	.0874429	.1569613	231.7905
#2	.0089730	.0058034	36.23792	.1779026	.0869255	.1567082	231.3801
#3	.0088702	.0054717	36.17814	.1791988	.0876623	.1564348	234.6066

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.760727	23.15933	.1313916	.0066072	5.780353	.2729826	.5070678
Stddev	.004862	.03081	.0007440	.0007841	.047647	.0014420	.0010759
%RSD	.1761281	.1330564	.5662293	11.86719	.8242966	.5282398	.2121875

#1	2.755156	23.13806	.1306870	.0059500	5.757959	.2713301	.5071583
#2	2.762907	23.14528	.1313183	.0063964	5.748028	.2736318	.5080956
#3	2.764118	23.19467	.1321696	.0074751	5.835072	.2739859	.5059495

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	7.999712	.0714830	.0043690	.0087928	1.407182	7.499674	5.328404
Stddev	.011950	.0091081	.0001450	.0003267	.003119	.050333	.011158
%RSD	.1493748	12.74164	3.319831	3.715842	.2216612	.6711397	.2094056

#1	7.990290	.0711750	.0044653	.0090843	1.403729	7.468042	5.332700
#2	7.995693	.0625327	.0044396	.0084396	1.408023	7.473264	5.315737
#3	8.013153	.0807411	.0042022	.0088544	1.409795	7.557715	5.336776

Sample Name: Q2801-01 Acquired: 8/11/2025 17:31:56 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	2.000809	.1057545	-.098782
Stddev	.002196	.0006947	.001630
%RSD	.1097356	.6569202	1.649859
#1	2.003198	.1049536	-.098047
#2	1.998881	.1061151	-.097649
#3	2.000347	.1061948	-.100650

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	6267.075	110158.5	13091.51	4736.570	6693.845
Stddev	10.767	420.6	39.64	34.691	7.585
%RSD	.1718074	.3818270	.3027949	.7324136	.1133087
#1	6259.148	110137.2	13071.45	4757.068	6694.285
#2	6279.334	110589.3	13065.92	4756.127	6701.201
#3	6262.743	109748.9	13137.18	4696.516	6686.050

Sample Name: Q2769-01 Acquired: 8/11/2025 17:35:58 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001704	.0007168	.0106700	.0023212	.0021095	.5135598
Stddev	.001383	.0002992	.0007462	.0023369	.0014848	.0063455
%RSD	81.14623	41.74918	6.993115	100.6764	70.38751	1.235599
#1	-.000572	.0004407	.0098920	.0000022	.0024601	.5172288
#2	-.001295	.0010348	.0113796	.0046757	.0033875	.5172179
#3	-.003246	.0006748	.0107383	.0022858	.0004807	.5062326
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0427228	-.000054	.0000222	32.77423	.0019273	.0006655
Stddev	.0009133	.000045	.0000311	.11944	.0001144	.0001288
%RSD	2.137719	83.00324	140.1409	.3644334	5.937690	19.34938
#1	.0436768	-.000023	.0000354	32.86690	.0020381	.0007201
#2	.0426350	-.000034	.0000445	32.81637	.0019344	.0005184
#3	.0418566	-.000106	-.000013	32.63944	.0018095	.0007579
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0770305	4.007773	.1417740	4.089413	.0026991	.0002137
Stddev	.0004351	.031300	.0005339	.030733	.0002645	.0001909
%RSD	.5648935	.7809797	.3765878	.7515257	9.801144	89.35007
#1	.0765387	3.981796	.1423491	4.113289	.0024023	.0000770
#2	.0773656	3.999000	.1412941	4.100213	.0029100	.0004319
#3	.0771873	4.042524	.1416788	4.054738	.0027849	.0001322
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	26.63763	.0004388	.1610330	4.351313	.0248940	.0011231
Stddev	.25578	.0005649	.0006841	.060769	.0010192	.0001229
%RSD	.9602027	128.7369	.4247940	1.396568	4.094214	10.93819
#1	26.45944	.0003156	.1614192	4.287993	.0249467	.0009912
#2	26.52275	-.000054	.1602432	4.356786	.0258859	.0011438
#3	26.93070	.001055	.1614367	4.409161	.0238495	.0012343

Sample Name: Q2769-01 Acquired: 8/11/2025 17:35:58 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001428	.0220507	4.013189	1.987842	F 330.6181	-.010571
Stddev	.000406	.0013716	.033371	.007721	1.6741	.001456
%RSD	28.41009	6.220326	.8315267	.3884055	.5063696	13.77769

#1	-.001896	.0235358	4.002179	1.996003	330.9991	-.012139
#2	-.001217	.0208314	3.986715	1.980653	328.7863	-.009260
#3	-.001172	.0217850	4.050674	1.986872	332.0689	-.010316

Elem	Sr4077
Units	ppm
Avg	.0950643
Stddev	.0002045
%RSD	.2151414

#1	.0953000
#2	.0949349
#3	.0949578

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5714.003	100918.1	11742.70	4393.599	7014.123
Stddev	2.717	211.3	143.97	12.910	8.460
%RSD	.0475492	.2093285	1.226045	.2938416	.1206206

#1	5710.924	101131.1	11623.37	4392.135	7010.736
#2	5716.064	100914.3	11702.14	4407.179	7023.752
#3	5715.020	100708.7	11902.60	4381.483	7007.880

Sample Name: Q2769-04 Acquired: 8/11/2025 17:40:09 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.002404	.0000902	.0083761	.0058270	.0014044	.4443004
Stddev	.000480	.0008218	.0019099	.0011232	.0008921	.0038130
%RSD	19.94994	910.7935	22.80179	19.27510	63.52192	.8581954
#1	-.001861	.0008448	.0062614	.0049331	.0017762	.4485996
#2	-.002768	-.000785	.0099754	.0054601	.0020504	.4429734
#3	-.002582	.000211	.0088916	.0070877	.0003865	.4413282
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0376731	-.000042	-.000034	30.69747	.0019775	.0004708
Stddev	.0006280	.000041	.000046	.11337	.0001817	.0000584
%RSD	1.666994	98.75760	136.8293	.3693202	9.188193	12.40512
#1	.0376209	.000005	.000019	30.57345	.0019683	.0004067
#2	.0383255	-.000055	-.000058	30.79578	.0018005	.0005211
#3	.0370727	-.000074	-.000062	30.72317	.0021636	.0004847
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0755328	3.492748	.1342291	3.826377	.0027041	.0003210
Stddev	.0002707	.005716	.0005669	.016246	.0003810	.0002062
%RSD	.3584435	.1636459	.4223361	.4245729	14.08809	64.23041
#1	.0753678	3.486321	.1335791	3.808609	.0023695	.0003436
#2	.0758453	3.494661	.1344877	3.840472	.0031187	.0001045
#3	.0753854	3.497261	.1346207	3.830050	.0026241	.0005150
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	25.46170	.0017730	.1334184	4.042790	.0213035	.0006426
Stddev	.08888	.0006611	.0002974	.039706	.0004380	.0000068
%RSD	.3490549	37.28466	.2228881	.9821333	2.056071	1.053059
#1	25.39812	.0016624	.1337460	4.009284	.0215528	.0006443
#2	25.56326	.0024823	.1331656	4.032440	.0207978	.0006484
#3	25.42373	.0011742	.1333435	4.086646	.0215600	.0006352

Sample Name: Q2769-04 Acquired: 8/11/2025 17:40:09 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001623	.0190695	3.711661	1.871732	F 415.1617	-.010796
Stddev	.000264	.0007386	.058919	.005368	1.0319	.000432
%RSD	16.29441	3.873060	1.587391	.2867913	.2485640	4.000082

#1	-.001502	.0194548	3.654006	1.870737	414.8581	-.010734
#2	-.001926	.0182180	3.709210	1.877528	416.3113	-.011255
#3	-.001441	.0195357	3.771767	1.866931	414.3155	-.010398

Elem	Sr4077
Units	ppm
Avg	.0908429
Stddev	.0002304
%RSD	.2536306

#1	.0907862
#2	.0910964
#3	.0906462

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5825.789	103668.9	11726.08	4404.253	7230.403
Stddev	16.190	267.3	40.46	6.855	14.009
%RSD	.2779005	.2577943	.3450312	.1556417	.1937522

#1	5812.637	103867.8	11729.30	4403.168	7222.896
#2	5820.859	103365.1	11684.11	4398.005	7221.746
#3	5843.871	103773.7	11764.83	4411.585	7246.565

Sample Name: CCV02 Acquired: 8/11/2025 17:44:21 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	5.006457	4.951226	4.898658	5.008915	4.926567	9.699463	9.566084
Stddev	.014048	.035846	.006554	.024888	.021124	.016827	.227935
%RSD	.2805990	.7239849	.1337845	.4968697	.4287840	.1734860	2.382740
#1	5.003136	4.910490	4.893210	5.008953	4.918400	9.693158	9.506764
#2	4.994367	4.965240	4.896833	4.984009	4.910744	9.686699	9.373674
#3	5.021868	4.977948	4.905930	5.033785	4.950555	9.718532	9.817815
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2420508	2.478587	24.30289	.9923645	2.453650	1.252653	4.964633
Stddev	.0022801	.003400	.05514	.0012368	.003441	.002604	.053919
%RSD	.9419801	.1371926	.2268882	.1246304	.1402257	.2078403	1.086072
#1	.2403261	2.476261	24.33794	.9920008	2.451907	1.253197	5.004136
#2	.2411905	2.477009	24.23933	.9937423	2.451430	1.249820	4.986559
#3	.2446359	2.482489	24.33139	.9913503	2.457613	1.254941	4.903205
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.427348	24.25168	2.473153	1.217158	24.38404	2.442333	2.453562
Stddev	.002819	.09470	.004328	.000855	.24054	.009693	.003474
%RSD	.1161215	.3904818	.1749892	.0702649	.9864649	.3968644	.1416050
#1	2.428455	24.25894	2.470721	1.218105	24.60173	2.432778	2.456078
#2	2.424144	24.15356	2.470589	1.216442	24.42460	2.442064	2.449598
#3	2.429445	24.34254	2.478150	1.216926	24.12580	2.452158	2.455011
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	24.57616	4.778070	4.949616	4.927408	4.867334	4.943393	4.959487
Stddev	.21891	.038290	.015467	.007533	.006187	.035159	.006483
%RSD	.8907345	.8013619	.3124867	.1528819	.1271108	.7112285	.1307165
#1	24.75276	4.752129	4.948067	4.922532	4.869698	4.919534	4.952015
#2	24.64448	4.760033	4.934982	4.923608	4.860314	4.983769	4.962834
#3	24.33124	4.822047	4.965800	4.936085	4.871991	4.926877	4.963613

Sample Name: CCV02 Acquired: 8/11/2025 17:44:21 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.065606	4.820333	4.837342
Stddev	.007005	.007230	.042907
%RSD	.1382852	.1499896	.8869942
#1	5.067445	4.828666	4.816493
#2	5.057865	4.815729	4.886689
#3	5.071509	4.816603	4.808843

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5539.570	97250.85	11303.33	4224.763	6569.535
Stddev	15.362	296.28	63.34	15.892	9.550
%RSD	.2773097	.3046558	.5603256	.3761538	.1453747
#1	5537.221	96972.16	11334.37	4206.428	6571.381
#2	5555.970	97218.36	11345.15	4233.288	6578.028
#3	5525.517	97562.04	11230.46	4234.572	6559.196

Sample Name: CCB02 Acquired: 8/11/2025 17:48:31 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0009300	.0004870	.0007278	.0030211	.0006524	-.006299
Stddev	.0018776	.0005111	.0007208	.0011995	.0008727	.002592
%RSD	201.9031	104.9608	99.03368	39.70360	133.7737	41.13875
#1	.0029390	.0003119	.0003437	.0020113	.0014651	-.003585
#2	-.000780	.0000864	.0015592	.0043470	-.000270	-.006565
#3	.000631	.0010627	.0002804	.0027051	.000762	-.008748
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.002336	-.000004	-.000010	-.009464	-.000082	-.000087
Stddev	.000913	.000024	.000030	.001227	.000248	.000130
%RSD	39.09874	627.2542	306.9752	12.96887	300.7700	149.9617
#1	-.002769	.000022	.000016	-.009092	.000120	-.000206
#2	-.001287	-.000006	-.000002	-.008466	-.000358	-.000106
#3	-.002952	-.000027	-.000043	-.010835	-.000008	.000052
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0005587	-.020447	-.000002	.0017262	-.000230	-.000339
Stddev	.0004747	.002949	.000295	.0153278	.000304	.000180
%RSD	84.96988	14.42174	16489.75	887.9685	132.4342	53.11890
#1	.0002189	-.022904	.000337	-.004346	-.000377	-.000516
#2	.0003561	-.017177	-.000201	-.009635	-.000432	-.000156
#3	.0011012	-.021261	-.000142	.019160	.000120	-.000345
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0239435	.0003754	.0023575	.0420501	.0006719	.0000565
Stddev	.0163529	.0006902	.0001437	.0228510	.0003675	.0001837
%RSD	68.29786	183.8608	6.096377	54.34234	54.69336	325.1185
#1	.0080502	.0009312	.0022708	.0281618	.0003483	.0002029
#2	.0230602	.0005921	.0025234	.0684237	.0010715	.0001162
#3	.0407203	-.000397	.0022783	.0295647	.0005960	-.000150

Sample Name: CCB02 Acquired: 8/11/2025 17:48:31 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0011052	.0001367	.0040119	.0010518	F .0467610	.0018476
Stddev	.0001261	.0004882	.0090632	.0016190	.0017724	.0020671
%RSD	11.41069	357.0684	225.9091	153.9253	3.790313	111.8785
#1	.0010094	.0004983	.0137578	-.000351	.0488015	.0028615
#2	.0012480	.0003305	-.004163	.000682	.0456040	.0032120
#3	.0010580	-.000419	.002441	.002824	.0458776	-.000531
Elem	Sr4077					
Units	ppm					
Avg	-.000102					
Stddev	.000069					
%RSD	67.92844					
#1	-.000043					
#2	-.000084					
#3	-.000178					
Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306	
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S	
Avg	5871.944	102232.1	11284.31	4402.888	7464.451	
Stddev	11.580	100.7	100.67	16.418	7.025	
%RSD	.1972083	.0985228	.8921168	.3728998	.0941112	
#1	5859.664	102117.1	11169.56	4384.162	7459.653	
#2	5882.666	102304.6	11357.76	4414.816	7472.514	
#3	5873.503	102274.6	11325.60	4409.685	7461.185	

Sample Name: PB169154BL Acquired: 8/11/2025 17:52:50 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000287	-.000579	.0002594	-.000021	.0018189	-.016421
Stddev	.001060	.000671	.0002860	.001615	.0013968	.002218
%RSD	368.9300	115.8729	110.2501	7783.323	76.79486	13.50821
#1	-.000030	-.000657	.0001465	.001700	.0002300	-.017880
#2	.000620	.000128	.0000471	-.000258	.0028536	-.017516
#3	-.001452	-.001207	.0005846	-.001504	.0023729	-.013869
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.003186	.0000043	-.000024	-.017772	-.000098	-.000043
Stddev	.000672	.0000556	.000049	.004532	.000091	.000092
%RSD	21.08483	1302.050	206.2964	25.50230	92.76451	213.4024
#1	-.002476	-.000055	-.000011	-.016212	-.000014	.000060
#2	-.003811	.000055	.000018	-.022878	-.000086	-.000071
#3	-.003270	.000012	-.000078	-.014226	-.000195	-.000119
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0003827	-.017395	.0003389	-.013452	-.000190	-.000034
Stddev	.0002566	.002661	.0002069	.010653	.000166	.000231
%RSD	67.06034	15.29992	61.06745	79.19451	87.28527	683.7979
#1	.0002762	-.014811	.0004454	-.003476	-.000086	-.000288
#2	.0006754	-.020127	.0004708	-.012205	-.000382	.000024
#3	.0001964	-.017247	.0001004	-.024673	-.000103	.000163
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.038621	.0005878	-.000012	-.047373	-.001378	-.000244
Stddev	.020437	.0017878	.000308	.029808	.000583	.000087
%RSD	52.91825	304.1453	2631.830	62.92254	42.29321	35.51822
#1	-.050687	-.001444	.000092	-.062680	-.001540	-.000344
#2	-.050151	.001287	-.000359	-.013021	-.001863	-.000201
#3	-.015024	.001920	.000231	-.066417	-.000731	-.000187

Sample Name: PB169154BL Acquired: 8/11/2025 17:52:50 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0005474	.0000143	.0010358	-.000621	F .0253663	-.002123
Stddev	.0003866	.0002104	.0014086	.000473	.0031034	.000647
%RSD	70.61850	1475.861	135.9859	76.15557	12.23454	30.46825

#1	.0001227	.0000130	-.000004	-.000076	.0251417	-.001381
#2	.0008788	.0002252	.000472	-.000921	.0285760	-.002566
#3	.0006409	-.000196	.002639	-.000866	.0223813	-.002423

Elem	Sr4077
Units	ppm
Avg	-.000157
Stddev	.000030
%RSD	19.21257

#1	-.000175
#2	-.000173
#3	-.000122

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5926.095	103668.5	11490.65	4437.124	7563.785
Stddev	5.721	88.9	79.33	6.932	11.160
%RSD	.0965403	.0857284	.6903529	.1562240	.1475486

#1	5920.112	103566.1	11509.42	4435.604	7551.963
#2	5931.512	103714.2	11558.91	4431.079	7574.139
#3	5926.660	103725.2	11403.62	4444.690	7565.253

Sample Name: PB169154BS Acquired: 8/11/2025 17:57:10 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.7888088	2.049425	.9773392	1.980233	.8076173	2.036599
Stddev	.0039378	.028063	.0016041	.007066	.0016198	.002624
%RSD	.4992110	1.369331	.1641265	.3568172	.2005652	.1288303
#1	.7910990	2.068894	.9765941	1.981418	.8093498	2.033749
#2	.7842618	2.017257	.9762431	1.972650	.8061407	2.038914
#3	.7910656	2.062124	.9791803	1.986632	.8073614	2.037136
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1972325	.2066358	.1953458	1.054010	.4131542	.2000243
Stddev	.0007506	.0015636	.0001917	.005734	.0020228	.0003295
%RSD	.3805472	.7567068	.0981362	.5440232	.4896026	.1647254
#1	.1977614	.2059120	.1952170	1.058904	.4112445	.1999625
#2	.1975626	.2055653	.1952544	1.047701	.4152738	.1997300
#3	.1963734	.2084302	.1955661	1.055424	.4129442	.2003803
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.3136384	3.009835	.2088746	2.064130	.5028271	.0755410
Stddev	.0005799	.026422	.0000766	.030031	.0012591	.0003641
%RSD	.1848893	.8778415	.0366778	1.454918	.2504075	.4820497
#1	.3129692	3.004668	.2088720	2.082075	.5021236	.0751650
#2	.3139531	3.038458	.2089524	2.029460	.5020770	.0758920
#3	.3139929	2.986378	.2087993	2.080855	.5042808	.0755660
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.821685	.3085190	.2103328	9.636212	.3003463	.4148858
Stddev	.046923	.0019817	.0005454	.092990	.0019699	.0002637
%RSD	1.662929	.6423188	.2593148	.9650081	.6558767	.0635650
#1	2.825486	.3075382	.2106049	9.598624	.2997686	.4147898
#2	2.866592	.3107998	.2097049	9.742113	.2987299	.4146835
#3	2.772978	.3072190	.2106886	9.567900	.3025405	.4151841

Sample Name: PB169154BS Acquired: 8/11/2025 17:57:10 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.6943689	.1987789	.8671045	5.678360	F .0227369	.2062828
Stddev	.0020100	.0007219	.0048246	.020468	.0002053	.0028599
%RSD	.2894655	.3631647	.5564015	.3604649	.9026995	1.386388

#1	.6946128	.1988752	.8710046	5.674830	.0226125	.2073010
#2	.6922481	.1980137	.8685997	5.659886	.0226244	.2084943
#3	.6962457	.1994479	.8617094	5.700363	.0229738	.2030532

Elem	Sr4077
Units	ppm
Avg	.1986715
Stddev	.0007960
%RSD	.4006622

#1	.1982230
#2	.1995906
#3	.1982010

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5925.656	102067.9	11321.49	4439.047	7399.206
Stddev	9.602	352.3	68.88	7.193	.936
%RSD	.1620416	.3451588	.6083645	.1620322	.0126541

#1	5930.686	102264.9	11345.07	4438.206	7399.768
#2	5914.584	101661.1	11375.48	4446.623	7399.725
#3	5931.698	102277.6	11243.92	4432.311	7398.125

Sample Name: Q2804-01 Acquired: 8/11/2025 18:01:09 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.003198	.0063692	.0019551	.0064309	.0024371	5.559984
Stddev	.001650	.0015798	.0020391	.0022325	.0015516	.006218
%RSD	51.60930	24.80311	104.2990	34.71552	63.66682	.1118279
#1	-.005100	.0063190	.0016585	.0039996	.0041682	5.559201
#2	-.002152	.0079734	.0041263	.0069045	.0019716	5.554194
#3	-.002341	.0048151	.0000805	.0083886	.0011715	5.566556
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000175	-.000072	-.000190	24.70793	.1379793	.0015456
Stddev	.001505	.000033	.000040	.05081	.0006822	.0001666
%RSD	861.6600	45.32953	20.82590	.2056614	.4944081	10.78157
#1	.001557	-.000107	-.000160	24.76616	.1382510	.0013544
#2	-.000911	-.000068	-.000175	24.67260	.1372031	.0016224
#3	-.001169	-.000042	-.000235	24.68503	.1384838	.0016600
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0197378	.1539382	.0197763	2.988859	.0411273	-.000127
Stddev	.0002395	.0023384	.0006512	.021872	.0002097	.000442
%RSD	1.213564	1.519032	3.292888	.7317937	.5097710	349.1379
#1	.0199388	.1516328	.0196178	3.009186	.0412549	-.000617
#2	.0194728	.1563082	.0192190	2.965715	.0408854	.000243
#3	.0198019	.1538737	.0204922	2.991675	.0412417	-.000007
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1885.262	.0009570	.3527686	248.6550	6.073417	.0186380
Stddev	4.321	.0012604	.0007884	1.2776	.053103	.0000581
%RSD	.2291929	131.7039	.2234942	.5138025	.8743537	.3119872
#1	1884.258	.0019131	.3536108	247.2286	6.119553	.0186237
#2	1881.531	.0014293	.3526467	249.6942	6.015370	.0185883
#3	1889.996	-.000471	.3520482	249.0422	6.085328	.0187019

Sample Name: Q2804-01 Acquired: 8/11/2025 18:01:09 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0014616	-.001606	.7940629	.8587108	F 933.4881	-.004197
Stddev	.0001885	.000210	.0047878	.0043609	2.3666	.001789
%RSD	12.89600	13.05304	.6029497	.5078430	.2535191	42.63557

#1	.0014120	-.001447	.7955806	.8544962	931.9815	-.003144
#2	.0013029	-.001527	.7979080	.8632046	936.2158	-.006263
#3	.0016700	-.001844	.7887002	.8584317	932.2670	-.003184

Elem	Sr4077
Units	ppm
Avg	.1043147
Stddev	.0003194
%RSD	.3061511

#1	.1046298
#2	.1039913
#3	.1043230

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	4864.925	82903.90	11509.10	3592.794	5386.475
Stddev	22.517	260.09	127.49	15.394	17.592
%RSD	.4628487	.3137282	1.107696	.4284609	.3265873

#1	4885.608	82767.75	11403.34	3588.528	5399.431
#2	4868.229	83203.81	11650.66	3609.870	5393.547
#3	4840.939	82740.15	11473.31	3579.983	5366.449

Sample Name: Q2805-01 Acquired: 8/11/2025 18:05:32 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.002289	.0003335	.0074625	.0028466	.0007337	.0423873	-.000757
Stddev	.001308	.0020529	.0006858	.0009297	.0001444	.0052725	.000838
%RSD	57.13334	615.6682	9.189807	32.66096	19.68181	12.43884	110.7507
#1	-.001597	.0005461	.0078517	.0021475	.0008933	.0417255	.000206
#2	-.003798	-.001818	.0078651	.0024907	.0006121	.0374770	-.001327
#3	-.001473	.002272	.0066706	.0039018	.0006956	.0479595	-.001149
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000107	-.000100	4.016347	-.000298	.0064136	.2438973	1.198475
Stddev	.000066	.000026	.013336	.000184	.0000590	.0001576	.013721
%RSD	61.89342	25.77523	.3320523	61.72690	.9196367	.0646321	1.144883
#1	-.000154	-.000071	4.002712	-.000500	.0064811	.2438447	1.214190
#2	-.000136	-.000119	4.016968	-.000140	.0063881	.2440745	1.192362
#3	-.000031	-.000112	4.029363	-.000255	.0063717	.2437727	1.188873
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0161555	1.582014	.0083104	-.000337	13.37643	-.000514	.0354821
Stddev	.0001001	.015084	.0001101	.000531	.04455	.002748	.0002596
%RSD	.6196683	.9534537	1.324533	157.4043	.3330175	534.3095	.7316572
#1	.0161434	1.564636	.0084066	-.000186	13.37417	.002032	.0357653
#2	.0162612	1.591721	.0083343	-.000928	13.33306	-.003427	.0352553
#3	.0160621	1.589684	.0081904	.000102	13.42207	-.000148	.0354259
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.8870003	.0068555	-.000301	.0003154	-.000088	5.638648	.0054823
Stddev	.0332081	.0002757	.000438	.0001207	.000564	.023652	.0008138
%RSD	3.743867	4.020913	145.6151	38.28353	643.1153	.4194683	14.84383
#1	.8563602	.0069155	.000203	.0001814	-.000423	5.617683	.0050220
#2	.8823537	.0065548	-.000589	.0004157	-.000403	5.633971	.0050031
#3	.9222870	.0070962	-.000516	.0003491	.000563	5.664289	.0064219

Sample Name: Q2805-01 Acquired: 8/11/2025 18:05:32 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.180590	-.011200	.0202808
Stddev	.008602	.000417	.0001207
%RSD	.1660413	3.719473	.5950517

#1	5.179758	-.011026	.0201427
#2	5.172435	-.010899	.0203657
#3	5.189578	-.011676	.0203342

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	6070.233	107716.1	12092.30	4587.079	7667.423
Stddev	6.985	216.3	8.16	16.863	19.404
%RSD	.1150726	.2008321	.0674752	.3676137	.2530766

#1	6070.572	107602.9	12083.02	4576.938	7670.715
#2	6077.043	107965.5	12098.36	4606.544	7684.971
#3	6063.085	107579.8	12095.53	4577.754	7646.583

Sample Name: Q2805-02 Acquired: 8/11/2025 18:09:47 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.003337	.0007644	.0064376	.0019874	.0010854	.0376928	.0005584
Stddev	.001199	.0003116	.0009094	.0008680	.0010611	.0049294	.0021024
%RSD	35.92920	40.76521	14.12666	43.67458	97.76345	13.07771	376.4961

#1	-.002348	.0004696	.0069480	.0017262	-.000074	.0327856	-.001862
#2	-.004671	.0010905	.0053877	.0029561	.001321	.0426440	.001928
#3	-.002992	.0007333	.0069773	.0012801	.002009	.0376490	.001610

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000092	-.000102	4.230027	-.000611	.0068215	.0122177	.0666347
Stddev	.000050	.000069	.009941	.000250	.0001984	.0002904	.0024701
%RSD	54.86238	68.27082	.2350110	40.90510	2.908409	2.376987	3.706881

#1	-.000064	-.000029	4.218906	-.000681	.0066303	.0120003	.0637972
#2	-.000061	-.000168	4.238049	-.000333	.0068079	.0121054	.0678034
#3	-.000149	-.000108	4.233127	-.000817	.0070264	.0125475	.0683036

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0185156	1.644050	.0073891	-.000043	13.79133	.0002253	.0591355
Stddev	.0003776	.023134	.0002319	.000311	.07640	.0015727	.0001230
%RSD	2.039441	1.407138	3.137883	719.2973	.5539696	697.9341	.2079491

#1	.0182716	1.620150	.0075808	-.000027	13.81924	-.000132	.0590540
#2	.0189506	1.645667	.0071314	.000259	13.84984	.001946	.0592770
#3	.0183247	1.666333	.0074551	-.000362	13.70490	-.001138	.0590757

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.8696572	.0053287	-.000435	-.000881	-.000764	5.770488	.0062110
Stddev	.0296212	.0004939	.000148	.000401	.000770	.015795	.0032126
%RSD	3.406083	9.269377	34.02076	45.47899	100.7417	.2737255	51.72359

#1	.8565159	.0056296	-.000366	-.000715	-.001024	5.769791	.0031203
#2	.9035756	.0055978	-.000334	-.001338	-.001370	5.755053	.0059799
#3	.8488801	.0047586	-.000605	-.000590	.000102	5.786621	.0095329

Sample Name: Q2805-02 Acquired: 8/11/2025 18:09:47 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.322404	-.011395	.0225922
Stddev	.009006	.001152	.0001412
%RSD	.1692068	10.10632	.6251718

#1	5.325849	-.012661	.0226466
#2	5.312184	-.011115	.0226981
#3	5.329179	-.010410	.0224318

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5930.717	105106.7	11663.42	4488.666	7488.938
Stddev	10.340	174.0	51.85	5.178	16.054
%RSD	.1743540	.1655772	.4445475	.1153539	.2143716

#1	5929.905	105192.5	11698.90	4494.523	7493.052
#2	5941.439	104906.4	11603.92	4486.777	7502.534
#3	5920.806	105221.1	11687.44	4484.697	7471.227

Sample Name: Q2805-02DUP Acquired: 8/11/2025 18:14:02 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.002656	-.000374	.0064464	.0028197	.0013656	.0383547	.0009187
Stddev	.001525	.000538	.0005549	.0016157	.0012571	.0081999	.0006020
%RSD	57.39578	143.6593	8.607836	57.30096	92.06037	21.37911	65.52661
#1	-.004357	-.000995	.0070715	.0025606	.0028171	.0342652	.0008010
#2	-.001412	-.000047	.0062558	.0045493	.0006237	.0330039	.0015708
#3	-.002200	-.000081	.0060120	.0013492	.0006559	.0477951	.0003842
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000097	-.000134	4.254516	-.000259	.0068441	.0122050	.0698195
Stddev	.000047	.000001	.006021	.000049	.0000972	.0001780	.0034618
%RSD	48.47675	.9775919	.1415181	18.99141	1.420418	1.458737	4.958253
#1	-.000118	-.000136	4.261381	-.000208	.0069562	.0122542	.0728632
#2	-.000129	-.000134	4.252037	-.000306	.0067826	.0120076	.0705419
#3	-.000043	-.000133	4.250130	-.000264	.0067936	.0123533	.0660535
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0180726	1.688706	.0077206	-.000169	14.08353	-.000078	.0603006
Stddev	.0002139	.029715	.0001965	.000397	.03856	.000613	.0003941
%RSD	1.183320	1.759624	2.545553	234.6679	.2738104	782.2040	.6535940
#1	.0181195	1.721970	.0075766	-.000614	14.04981	-.000608	.0598754
#2	.0182591	1.679360	.0079445	.000148	14.07520	-.000220	.0606536
#3	.0178392	1.664788	.0076407	-.000041	14.12557	.000593	.0603727
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.8608619	.0041940	-.000540	-.000546	-.000623	5.945531	.0066380
Stddev	.0099467	.0002889	.000205	.000565	.000898	.013887	.0014004
%RSD	1.155435	6.887603	38.01681	103.4003	144.0661	.2335654	21.09653
#1	.8722208	.0043241	-.000641	-.001171	-.000845	5.938323	.0050559
#2	.8537097	.0043949	-.000304	-.000072	.000365	5.961540	.0077185
#3	.8566553	.0038630	-.000676	-.000396	-.001390	5.936731	.0071396

Sample Name: Q2805-02DUP Acquired: 8/11/2025 18:14:02 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.310099	-.010491	.0228787
Stddev	.016387	.000670	.0001253
%RSD	.3085936	6.381863	.5478302

#1	5.327478	-.009964	.0228203
#2	5.294929	-.010266	.0227933
#3	5.307889	-.011244	.0230226

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5997.695	104901.8	11777.87	4491.628	7636.611
Stddev	7.688	241.6	62.09	7.827	7.748
%RSD	.1281767	.2303062	.5272045	.1742554	.1014603

#1	6006.433	104837.3	11735.62	4482.633	7645.517
#2	5991.972	105169.1	11849.16	4495.365	7632.894
#3	5994.679	104699.0	11748.82	4496.886	7631.422

Sample Name: Q2805-02LX5 Acquired: 8/11/2025 18:18:17 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000436	.0000770	.0003330	.0017647	.0018291	.0021814	-.003418
Stddev	.000457	.0013100	.0005338	.0011110	.0019523	.0015899	.001120
%RSD	104.8357	1701.067	160.2858	62.95501	106.7336	72.88807	32.77876

#1	-.000868	-.000246	.0000578	.0009979	.0040269	.0025775	-.002140
#2	-.000482	.001518	-.000007	.0030387	.0011648	.0004308	-.004230
#3	.000042	-.001041	.000948	.0012574	.0002957	.0035358	-.003884

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000352	-.000121	.9241958	-.000094	.0012188	.0027170	.0031233
Stddev	.0000433	.000039	.0038674	.000073	.0001312	.0001669	.0013574
%RSD	123.1429	32.07357	.4184575	77.63010	10.76740	6.142386	43.46094

#1	.0000840	-.000132	.9285806	-.000047	.0011252	.0027593	.0026213
#2	.0000013	-.000078	.9212709	-.000057	.0013688	.0028586	.0020884
#3	.0000202	-.000153	.9227359	-.000178	.0011624	.0025330	.0046602

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0038965	.3562560	.0013195	-.000016	3.809058	-.000927	.0126927
Stddev	.0005376	.0134298	.0002226	.000261	.036441	.001945	.0003223
%RSD	13.79658	3.769700	16.86696	1638.616	.9567032	209.8360	2.538916

#1	.0032762	.3703637	.0015760	.000106	3.840857	.000759	.0128939
#2	.0041863	.3547780	.0012050	.000162	3.817023	-.003054	.0123210
#3	.0042269	.3436264	.0011776	-.000316	3.769292	-.000486	.0128631

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1.104155	-.001413	-.000365	-.000424	.0003461	1.268186	.0019221
Stddev	.033743	.000383	.000034	.000453	.0009847	.015494	.0023636
%RSD	3.056011	27.12738	9.343052	106.6522	284.5410	1.221733	122.9737

#1	1.088291	-.001654	-.000380	-.000779	.0009541	1.282415	-.000298
#2	1.142907	-.001614	-.000390	.000085	.0008741	1.270465	.001657
#3	1.081268	-.000971	-.000327	-.000580	-.000790	1.251679	.004407

Sample Name: Q2805-02LX5 Acquired: 8/11/2025 18:18:17 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	1.251095	.0357747	.0047272
Stddev	.029560	.0012661	.0000532
%RSD	2.362760	3.539212	1.125326
#1	1.279502	.0365895	.0047630
#2	1.253281	.0364187	.0047526
#3	1.220503	.0343161	.0046661

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5861.936	103843.2	11496.46	4415.172	7383.714
Stddev	8.096	304.2	51.19	8.537	9.084
%RSD	.1381045	.2929009	.4452772	.1933654	.1230255
#1	5860.156	103798.1	11522.36	4412.039	7373.377
#2	5870.774	103564.0	11529.53	4408.643	7390.422
#3	5854.879	104167.3	11437.49	4424.833	7387.344

Sample Name: Q2805-02MS Acquired: 8/11/2025 18:22:36 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.8050562	1.845197	.9530809	1.974839	.7954043	2.033544	.1956985
Stddev	.0007534	.079953	.0023663	.012264	.0035180	.003376	.0007791
%RSD	.0935840	4.333024	.2482821	.6210221	.4422887	.1659945	.3981050
#1	.8043103	1.759399	.9536139	1.961273	.7913423	2.030938	.1952261
#2	.8050414	1.858576	.9504935	1.978100	.7974763	2.037357	.1965977
#3	.8058169	1.917617	.9551352	1.985142	.7973942	2.032337	.1952716
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1934103	.1944441	5.360428	.4120335	.2064372	.3239334	3.070923
Stddev	.0003545	.0005110	.013802	.0006666	.0007756	.0010531	.010263
%RSD	.1833058	.2628035	.2574840	.1617902	.3757111	.3251076	.3342041
#1	.1937991	.1941454	5.349731	.4118443	.2061400	.3235420	3.064900
#2	.1931049	.1941527	5.376008	.4114819	.2058541	.3231320	3.082773
#3	.1933270	.1950341	5.355544	.4127743	.2073174	.3251262	3.065095
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2199721	3.693870	.5084017	.0717221	17.27293	.3016616	.2646648
Stddev	.0009584	.014472	.0010247	.0003302	.06089	.0017643	.0016938
%RSD	.4356726	.3917771	.2015501	.4603550	.3524905	.5848547	.6399931
#1	.2191159	3.708848	.5082895	.0720816	17.22697	.3024150	.2659912
#2	.2210074	3.679965	.5074378	.0716521	17.34198	.3029240	.2652463
#3	.2197930	3.692796	.5094779	.0714325	17.24983	.2996456	.2627568
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	10.42717	.2676255	.4256438	.6894914	.1958611	6.923918	5.656023
Stddev	.03067	.0013700	.0016906	.0034652	.0013385	.020863	.023267
%RSD	.2941617	.5119047	.3971953	.5025677	.6833999	.3013167	.4113692
#1	10.39218	.2684813	.4239521	.6864078	.1959203	6.901843	5.629993
#2	10.44939	.2660454	.4256460	.6888252	.1971689	6.926601	5.663280
#3	10.43995	.2683497	.4273334	.6932414	.1944939	6.943309	5.674798

Sample Name: Q2805-02MS Acquired: 8/11/2025 18:22:36 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.787454	.1878176	.2147257
Stddev	.049550	.0008109	.0007455
%RSD	.8561588	.4317289	.3472016

#1	5.732717	.1885237	.2146666
#2	5.800399	.1879971	.2154991
#3	5.829247	.1869320	.2140115

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5733.459	104178.7	11685.46	4426.300	7091.574
Stddev	5.742	166.1	4.75	15.492	8.847
%RSD	.1001493	.1594830	.0406387	.3499890	.1247517

#1	5727.252	104360.9	11687.38	4424.651	7084.899
#2	5734.545	104035.5	11688.95	4411.698	7088.215
#3	5738.581	104139.8	11680.06	4442.550	7101.608

Sample Name: CCV03 Acquired: 8/11/2025 18:26:32 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCV03 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.935707	4.516350	4.847941	4.905764	4.889308	9.606692	9.550967
Stddev	.004781	.112774	.008900	.013735	.012344	.026807	.109511
%RSD	.0968588	2.497014	.1835792	.2799678	.2524658	.2790410	1.146595

#1	4.930239	4.390656	4.842791	4.890161	4.879798	9.576365	9.433425
#2	4.939102	4.608672	4.842814	4.916026	4.884868	9.627224	9.650119
#3	4.937778	4.549722	4.858217	4.911105	4.903258	9.616486	9.569356

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2397229	2.447100	24.08516	.9766219	2.432228	1.237469	4.911653
Stddev	.0008858	.002771	.06415	.0034734	.005023	.001153	.007479
%RSD	.3695253	.1132248	.2663637	.3556587	.2065122	.0931428	.1522712

#1	.2387870	2.445852	24.07114	.9749066	2.430369	1.238379	4.920288
#2	.2405482	2.445172	24.15516	.9743398	2.428400	1.236173	4.907208
#3	.2398336	2.450275	24.02917	.9806193	2.437916	1.237855	4.907464

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.409755	23.93978	2.447964	1.211163	23.29523	2.426905	2.448761
Stddev	.004866	.10103	.002599	.000790	.13104	.004567	.001789
%RSD	.2019323	.4219999	.1061675	.0652304	.5625259	.1881683	.0730530

#1	2.410002	23.93800	2.446244	1.211794	23.44088	2.421646	2.446846
#2	2.414493	24.04168	2.446694	1.210277	23.18688	2.429877	2.449048
#3	2.404770	23.83965	2.450954	1.211417	23.25794	2.429191	2.450389

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	24.26302	4.787473	4.911981	4.849141	4.823334	4.848674	4.918430
Stddev	.02781	.023021	.012622	.006182	.007971	.007764	.005985
%RSD	.1146199	.4808556	.2569647	.1274889	.1652617	.1601173	.1216866

#1	24.29356	4.764809	4.899350	4.842535	4.828501	4.855425	4.912402
#2	24.23915	4.810835	4.912000	4.850101	4.827347	4.850406	4.924371
#3	24.25636	4.786775	4.924594	4.854787	4.814154	4.840191	4.918516

Sample Name: CCV03 Acquired: 8/11/2025 18:26:32 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCV03 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	4.873484	4.758742	4.805836
Stddev	.007292	.006245	.019504
%RSD	.1496177	.1312343	.4058488

#1	4.865481	4.763375	4.799158
#2	4.879750	4.761212	4.827803
#3	4.875222	4.751640	4.790549

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5594.305	98744.41	11408.61	4214.360	6656.565
Stddev	6.802	95.41	47.02	12.860	9.293
%RSD	.1215792	.0966269	.4121834	.3051475	.1396095

#1	5595.429	98759.46	11461.41	4222.133	6656.514
#2	5600.475	98831.41	11371.24	4221.430	6665.884
#3	5587.011	98642.37	11393.18	4199.516	6647.297

Sample Name: CCB03 Acquired: 8/11/2025 18:30:44 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCB03 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0011673	.0008458	.0014888	.0025540	.0020116	.0092982
Stddev	.0003436	.0023395	.0010988	.0013494	.0012268	.0057989
%RSD	29.43158	276.6045	73.80344	52.83585	60.98550	62.36571
#1	.0014990	.0035187	.0018087	.0016126	.0018976	.0056139
#2	.0008130	-.000152	.0002656	.0041001	.0032914	.0062982
#3	.0011899	-.000829	.0023922	.0019494	.0008458	.0159825
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001407	.0001018	.0004192	.0238179	.0000347	.0003996
Stddev	.000844	.0000202	.0000320	.0049066	.0001754	.0000545
%RSD	60.02768	19.88558	7.624378	20.60053	504.7167	13.65223
#1	-.001229	.0000784	.0003870	.0188077	.0001888	.0003763
#2	-.000665	.0001135	.0004198	.0286139	-.000156	.0004619
#3	-.002325	.0001134	.0004509	.0240320	.000072	.0003605
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0003902	-.003664	.0015153	-.005548	.0004849	.0004269
Stddev	.0001652	.004040	.0004002	.003769	.0001743	.0001711
%RSD	42.33388	110.2820	26.41109	67.93303	35.95026	40.08227
#1	.0002370	.000676	.0018929	-.007232	.0006464	.0003009
#2	.0005652	-.004351	.0015573	-.001231	.0003001	.0006217
#3	.0003683	-.007317	.0010958	-.008183	.0005081	.0003580
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.3538804	-.000806	.0048738	.3323623	.0018311	.0010814
Stddev	.0169342	.000994	.0000795	.0196714	.0006682	.0001751
%RSD	4.785297	123.2294	1.630199	5.918671	36.49110	16.19576
#1	.3607072	-.001951	.0047966	.3506964	.0022310	.0011198
#2	.3663356	-.000162	.0048694	.3348082	.0010597	.0012341
#3	.3345983	-.000307	.0049553	.3115823	.0022026	.0008902

Sample Name: CCB03 Acquired: 8/11/2025 18:30:44 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCB03 Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0015745	.0009059	.0003613	.0011329	F .0363948	F .0114244
Stddev	.0008110	.0012821	.0093120	.0022963	.0029769	.0018514
%RSD	51.51097	141.5349	2577.288	202.6893	8.179484	16.20603

#1	.0025110	.0000501	-.006782	.0013835	.0370922	.0104785
#2	.0011105	.0002875	-.003027	.0032936	.0389610	.0102369
#3	.0011021	.0023799	.010893	-.001278	.0331311	.0135577

Elem	Sr4077
Units	ppm
Avg	.0007929
Stddev	.0000202
%RSD	2.548341

#1	.0008133
#2	.0007729
#3	.0007926

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5816.884	103220.6	11419.72	4402.356	7372.781
Stddev	10.047	8.7	41.80	6.820	5.036
%RSD	.1727286	.0083986	.3660543	.1549178	.0683048

#1	5823.260	103224.6	11371.49	4401.837	7378.327
#2	5822.091	103226.4	11445.66	4395.811	7371.521
#3	5805.302	103210.6	11442.00	4409.421	7368.494

Sample Name: Q2805-02MSD Acquired: 8/11/2025 18:35:03 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.7610666	1.706963	.9052272	1.862378	.7774441	2.002311	.1924367
Stddev	.0006277	.059215	.0034777	.004653	.0034287	.006970	.0004516
%RSD	.0824764	3.469014	.3841766	.2498188	.4410252	.3480775	.2346764
#1	.7604733	1.674622	.9026551	1.860091	.7750913	2.000143	.1928828
#2	.7617238	1.670961	.9038425	1.859312	.7758628	2.010106	.1924475
#3	.7610028	1.775305	.9091839	1.867732	.7813781	1.996682	.1919798
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1898116	.1828238	5.314589	.4067438	.1968392	.3089842	3.016568
Stddev	.0016644	.0002843	.024130	.0010305	.0001298	.0007397	.022875
%RSD	.8768677	.1555284	.4540333	.2533531	.0659359	.2393944	.7583273
#1	.1910083	.1827886	5.339511	.4071241	.1968433	.3091827	3.007569
#2	.1905155	.1825586	5.312918	.4055772	.1967074	.3081655	2.999560
#3	.1879109	.1831241	5.291338	.4075301	.1969669	.3096044	3.042574
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2169100	3.641165	.4810952	.0698002	17.23879	.2962605	.2609507
Stddev	.0012666	.018390	.0008478	.0002194	.15161	.0031670	.0008585
%RSD	.5839113	.5050504	.1762302	.3143577	.8794735	1.069007	.3290001
#1	.2183097	3.657083	.4807773	.0695497	17.11520	.2937514	.2602587
#2	.2165772	3.645378	.4804522	.0698929	17.19322	.2998191	.2619114
#3	.2158430	3.621034	.4820560	.0699581	17.40797	.2952111	.2606820
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	10.31474	.2636905	.4202418	.6550954	.1944270	6.912458	5.171481
Stddev	.05836	.0026491	.0015752	.0027035	.0010864	.074587	.002596
%RSD	.5657815	1.004619	.3748307	.4126814	.5587604	1.079019	.0502070
#1	10.24851	.2661171	.4195383	.6534716	.1944389	6.847880	5.168570
#2	10.33705	.2640901	.4191410	.6535983	.1955073	6.895397	5.173557
#3	10.35865	.2608643	.4220462	.6582162	.1933347	6.994097	5.172316

Sample Name: Q2805-02MSD Acquired: 8/11/2025 18:35:03 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.352761	.1840268	.2119805
Stddev	.034488	.0009702	.0001250
%RSD	.6443058	.5271847	.0589512

#1	5.322277	.1851064	.2120932
#2	5.345812	.1837459	.2120021
#3	5.390195	.1832281	.2118461

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5960.245	104315.0	11730.15	4436.343	7535.527
Stddev	.992	111.0	140.06	21.597	4.565
%RSD	.0166409	.1064167	1.193978	.4868267	.0605751

#1	5960.522	104226.0	11623.30	4419.333	7539.296
#2	5961.069	104279.7	11678.43	4429.054	7536.834
#3	5959.144	104439.4	11888.70	4460.642	7530.452

Sample Name: Q2805-02A Acquired: 8/11/2025 18:38:59 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.7437939	1.728982	.8862764	1.838658	.7475062	2.001589	.1818867
Stddev	.0051248	.023905	.0035728	.002970	.0006995	.006985	.0013538
%RSD	.6890011	1.382634	.4031261	.1615559	.0935852	.3489960	.7443188
#1	.7441874	1.719046	.8842102	1.835444	.7483039	1.995144	.1807873
#2	.7384837	1.756253	.8842172	1.839228	.7469973	2.009012	.1814739
#3	.7487105	1.711647	.8904020	1.841302	.7472174	2.000612	.1833988
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1802455	.1797186	5.129785	.3847974	.1909007	.3006305	2.897741
Stddev	.0018307	.0005466	.028205	.0005938	.0009132	.0009401	.005954
%RSD	1.015658	.3041352	.5498330	.1543204	.4783784	.3126951	.2054865
#1	.1785565	.1791925	5.099894	.3841329	.1903266	.3000342	2.897752
#2	.1799891	.1796797	5.133531	.3849834	.1904218	.3001432	2.903690
#3	.1821908	.1802836	5.155930	.3852760	.1919538	.3017142	2.891782
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2071126	3.490375	.4717930	.0666558	16.73332	.2845767	.2505626
Stddev	.0016147	.046479	.0013962	.0003036	.06640	.0018620	.0009599
%RSD	.7796195	1.331629	.2959444	.4555516	.3968319	.6543058	.3830922
#1	.2056707	3.439173	.4706038	.0669816	16.72822	.2843827	.2507553
#2	.2068098	3.529907	.4714449	.0663806	16.80213	.2865281	.2495209
#3	.2088572	3.502045	.4733304	.0666052	16.66962	.2828193	.2514115
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.915086	.2510499	.3978325	.6391590	.1818689	6.704695	5.152744
Stddev	.048048	.0026712	.0007013	.0032408	.0012772	.055582	.029191
%RSD	.4845909	1.063990	.1762809	.5070363	.7022417	.8290006	.5665065
#1	9.942038	.2499509	.3980347	.6367136	.1804901	6.740614	5.130612
#2	9.943607	.2491036	.3970524	.6379286	.1821051	6.732797	5.141792
#3	9.859613	.2540953	.3984105	.6428348	.1830114	6.640673	5.185826

Sample Name: Q2805-02A Acquired: 8/11/2025 18:38:59 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	5.407496	.1771257	.2033542
Stddev	.020209	.0006922	.0008972
%RSD	.3737199	.3907886	.4411949
#1	5.405854	.1767264	.2023595
#2	5.388158	.1767258	.2036010
#3	5.428476	.1779250	.2041022

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5825.659	103760.9	11749.00	4421.136	7255.279
Stddev	5.747	137.0	129.47	20.250	4.846
%RSD	.0986468	.1320798	1.101954	.4580267	.0667887
#1	5819.167	103722.0	11845.74	4408.220	7251.677
#2	5827.718	103913.2	11799.34	4444.475	7260.788
#3	5830.094	103647.6	11601.93	4410.714	7253.372

Sample Name: Q2807-01 Acquired: 8/11/2025 18:42:57 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1108499	-.033978	.6027179	.0111225	-.012529	184.8862	1.391072
Stddev	.0003056	.001054	.0019565	.0029044	.001513	1.6319	.011891
%RSD	.2757073	3.101920	.3246192	26.11318	12.07735	.8826426	.8548319
#1	.1105507	-.034227	.6033043	.0111558	-.014259	185.7877	1.402662
#2	.1111615	-.034885	.6043141	.0082015	-.011875	183.0025	1.391655
#3	.1108376	-.032822	.6005352	.0140101	-.011452	185.8685	1.378900
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0151371	.0189248	37.48221	.3481350	.2111992	.3594804	432.5326
Stddev	.0001037	.0002699	.05844	.0015777	.0000825	.0025684	4.7635
%RSD	.6849340	1.426076	.1559008	.4531783	.0390572	.7144854	1.101314
#1	.0151915	.0186495	37.47363	.3487335	.2111647	.3565473	437.5058
#2	.0150175	.0191890	37.54447	.3463456	.2112934	.3613274	428.0108
#3	.0152022	.0189358	37.42854	.3493258	.2111397	.3605663	432.0811
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	6.370298	54.73960	.2240669	.0150360	205.6263	.6349088	1.095433
Stddev	.036682	.16743	.0002121	.0016595	.8276	.0023563	.001440
%RSD	.5758345	.3058741	.0946769	11.03660	.4024970	.3711287	.1314697
#1	6.393238	54.54656	.2238581	.0168247	206.5556	.6354415	1.094508
#2	6.389666	54.82685	.2242823	.0135465	205.3548	.6369533	1.097093
#3	6.327991	54.84538	.2240604	.0147368	204.9686	.6323318	1.094699
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	34.86444	^ *****	.0128417	.0554657	9.214843	9.332751	12.01229
Stddev	.20665	-----	.0001013	.0014079	.042316	.006453	.03600
%RSD	.5927248	-----	.7887418	2.538335	.4592172	.0691487	.2997155
#1	35.07639	^ -----	.0127599	.0550141	9.241664	9.338135	11.98189
#2	34.85339	^ -----	.0128103	.0543390	9.236803	9.334520	12.00293
#3	34.66354	^ -----	.0129550	.0570440	9.166061	9.325598	12.05205

Sample Name: Q2807-01 Acquired: 8/11/2025 18:42:57 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.6101081	.1990748	-.263144
Stddev	.0052354	.0005608	.004367
%RSD	.8581142	.2817228	1.659609
#1	.6144981	.1997149	-.267146
#2	.6115127	.1986695	-.258486
#3	.6043137	.1988401	-.263801

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	6848.045	117347.4	14604.75	5047.349	6026.907
Stddev	11.668	354.0	13.54	27.554	15.752
%RSD	.1703849	.3017038	.0927297	.5459036	.2613608
#1	6835.402	116941.8	14592.33	5025.863	6010.146
#2	6850.333	117594.4	14619.19	5037.770	6029.170
#3	6858.399	117506.0	14602.72	5078.414	6041.405

Sample Name: Q2807-02 Acquired: 8/11/2025 18:47:18 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0980740	-.022750	1.496777	.0047918	-.005490	140.7855
Stddev	.0025245	.003113	.004504	.0018819	.002444	.1100
%RSD	2.574027	13.68512	.3009338	39.27266	44.51348	.0781512
#1	.0962885	-.020637	1.494718	.0032095	-.002669	140.6584
#2	.1009622	-.026325	1.493670	.0042932	-.006939	140.8509
#3	.0969713	-.021288	1.501942	.0068728	-.006863	140.8470
Elem	Ba4934	Be2348	Cd2265	Ca3736	Cr2677	Co2286
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	1.131300	.0124802	.0116504	69.13174	.2573287	.1213649
Stddev	.006460	.0001465	.0002384	.08905	.0010498	.0003305
%RSD	.5710252	1.173488	2.046184	.1288184	.4079777	.2723286
#1	1.124017	.0126384	.0117533	69.03973	.2576838	.1210060
#2	1.133547	.0124530	.0118200	69.21751	.2561473	.1214320
#3	1.136337	.0123493	.0113778	69.13798	.2581549	.1216567
Elem	Cu2247	Fe2404	Mn2576	Mg2790	Ni2316	Ag3280
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.3431650	258.6557	4.825046	26.88820	.1790902	.0120614
Stddev	.0008781	3.0610	.015005	.01158	.0001053	.0011613
%RSD	.2558867	1.183426	.3109734	.0430710	.0587907	9.628282
#1	.3441775	257.0122	4.807786	26.88861	.1790021	.0112012
#2	.3426121	256.7674	4.834990	26.87642	.1790616	.0116006
#3	.3427053	262.1874	4.832360	26.89957	.1792068	.0133824
Elem	Na5895	V_2924	Zn2138	K_7664	B_2496	Mo2020
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.172080	.3908042	.7401354	9.890993	.0648427	.0110478
Stddev	.065036	.0022627	.0034783	.123337	.0160975	.0002393
%RSD	1.558840	.5789862	.4699578	1.246963	24.82543	2.165962
#1	4.127643	.3899634	.7397073	9.795277	.0589256	.0107979
#2	4.141872	.3933669	.7438080	9.847522	.0525411	.0110706
#3	4.246727	.3890823	.7368910	10.03018	.0830613	.0112748

Sample Name: Q2807-02 Acquired: 8/11/2025 18:47:18 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	Sn1899	Ti3361	Si2881	P_1774	S_1820	Li6707
Units	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1171978	2.795537	9.471390	F 25.22585	1.082487	.1436860
Stddev	.0011143	.011486	.072658	.03682	.007029	.0005091
%RSD	.9507733	.4108674	.7671331	.1459428	.6493671	.3543447

#1	.1159671	2.782415	9.457180	25.18463	1.090585	.1431760
#2	.1181381	2.800430	9.406887	25.23744	1.077954	.1436878
#3	.1174883	2.803766	9.550104	25.25547	1.078922	.1441943

Elem	Sr4077
Units	ppm
Avg	.1129306
Stddev	.0025490
%RSD	2.257119

#1	.1120000
#2	.1158141
#3	.1109776

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	7188.621	125290.6	15099.51	5387.307	6541.057
Stddev	9.860	348.5	124.73	18.026	6.102
%RSD	.1371678	.2781306	.8260689	.3346078	.0932818

#1	7181.320	125203.2	15035.60	5398.155	6541.662
#2	7184.704	125674.5	15019.69	5366.498	6534.676
#3	7199.838	124994.2	15243.25	5397.268	6546.834

Sample Name: Q2807-03 Acquired: 8/11/2025 18:51:22 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1253347	-.027299	1.566073	.0014320	-.006905	178.9124	1.188666
Stddev	.0016480	.001824	.002941	.0015255	.003392	.0710	.000516
%RSD	1.314859	6.680544	.1877643	106.5288	49.12045	.0396902	.0434097
#1	.1259348	-.025603	1.564594	.0003133	-.010536	178.8473	1.189176
#2	.1265985	-.029228	1.569460	.0008130	-.006362	178.9881	1.188144
#3	.1234707	-.027066	1.564166	.0031697	-.003818	178.9018	1.188678
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0141598	.0121955	41.96396	.3223990	.1071492	.2176486	308.2119
Stddev	.0001072	.0001037	.01651	.0011219	.0002916	.0013841	1.2587
%RSD	.7572150	.8504515	.0393477	.3479730	.2721051	.6359160	.4083839
#1	.0142632	.0123072	41.98222	.3236271	.1068303	.2183392	306.8943
#2	.0140491	.0121023	41.95009	.3214279	.1074021	.2185515	308.3393
#3	.0141671	.0121769	41.95956	.3221420	.1072153	.2160552	309.4020
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	3.756024	34.20763	.1726686	.0084746	4.544905	.4662627	.7256465
Stddev	.006802	.07540	.0006478	.0003338	.015331	.0039984	.0020142
%RSD	.1810889	.2204049	.3751782	3.939125	.3373149	.8575496	.2775665
#1	3.761610	34.25919	.1720964	.0080920	4.527890	.4646778	.7278204
#2	3.748450	34.12110	.1733719	.0086256	4.549183	.4632996	.7238438
#3	3.758011	34.24259	.1725373	.0087063	4.557643	.4708106	.7252753
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	9.784065	.0651888	.0118390	.0714060	2.601023	9.564550	13.95825
Stddev	.041557	.0052367	.0000165	.0012871	.002269	.044083	.03402
%RSD	.4247400	8.033086	.1390063	1.802512	.0872475	.4609011	.2437619
#1	9.736194	.0592166	.0118474	.0721818	2.602629	9.516411	13.91933
#2	9.810871	.0689949	.0118497	.0721159	2.602012	9.574293	13.97310
#3	9.805131	.0673548	.0118201	.0699203	2.598427	9.602947	13.98233

Sample Name: Q2807-03 Acquired: 8/11/2025 18:51:22 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.8807389	.1415339	-.078882
Stddev	.0042353	.0007700	.001368
%RSD	.4808831	.5440651	1.733969

#1	.8773420	.1420230	-.077401
#2	.8854843	.1419324	-.079148
#3	.8793905	.1406463	-.080098

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	7001.349	121868.2	14646.81	5283.253	6482.693
Stddev	12.516	278.6	43.61	14.110	10.821
%RSD	.1787668	.2286306	.2977676	.2670773	.1669187

#1	6986.897	122122.3	14599.71	5295.808	6470.199
#2	7008.487	121912.0	14685.79	5285.970	6488.867
#3	7008.662	121570.2	14654.92	5267.982	6489.014

Sample Name: Q2798-01 Acquired: 8/11/2025 18:55:26 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0567554	-.021048	.3119161	.0030985	-.008229	121.5032	.5865916
Stddev	.0005650	.002021	.0015531	.0011222	.002694	.1728	.0017731
%RSD	.9955194	9.599799	.4979265	36.21802	32.73391	.1422462	.3022700
#1	.0571195	-.022811	.3129006	.0039178	-.005473	121.3086	.5878514
#2	.0570422	-.018843	.3101257	.0018194	-.008358	121.5623	.5873593
#3	.0561045	-.021491	.3127220	.0035582	-.010856	121.6387	.5845640
Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0089001	.0107983	76.55458	.2710227	.1780160	.5987648	299.1266
Stddev	.0000342	.0002029	.15671	.0004849	.0004105	.0011196	1.4335
%RSD	.3847396	1.879025	.2047077	.1788987	.2305958	.1869837	.4792195
#1	.0088685	.0106082	76.50276	.2715299	.1778804	.5982982	300.7533
#2	.0089365	.0110119	76.43034	.2705639	.1776904	.5979540	298.0484
#3	.0088953	.0107747	76.73064	.2709743	.1784771	.6000422	298.5781
Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.713334	61.70351	.3270116	.0097780	13.25385	.4627519	.6155131
Stddev	.012266	.32421	.0002275	.0001706	.14096	.0014365	.0010932
%RSD	.2602445	.5254306	.0695545	1.745172	1.063565	.3104281	.1775995
#1	4.723341	61.52514	.3268445	.0098972	13.40173	.4611822	.6164153
#2	4.699650	61.50766	.3269197	.0095825	13.23884	.4640011	.6158266
#3	4.717011	62.07774	.3272707	.0098543	13.12100	.4630723	.6142975
Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	8.007612	.1279309	.0034750	.0193731	7.850077	3.202025	6.093593
Stddev	.051641	.0023814	.0002434	.0011745	.010200	.014160	.009524
%RSD	.6449044	1.861468	7.004294	6.062437	.1299308	.4422314	.1562923
#1	8.060495	.1305480	.0033454	.0180208	7.856991	3.217566	6.096068
#2	8.005031	.1258916	.0033238	.0201381	7.854877	3.198658	6.083077
#3	7.957309	.1273530	.0037558	.0199604	7.838363	3.189852	6.101636

Sample Name: Q2798-01 Acquired: 8/11/2025 18:55:26 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	3.137075	.1057094	-.056412
Stddev	.014656	.0006105	.001433
%RSD	.4671949	.5775205	2.540999
#1	3.135666	.1054595	-.057541
#2	3.123175	.1052635	-.054799
#3	3.152385	.1064052	-.056897

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	6573.862	115068.0	14044.91	4967.470	6527.179
Stddev	13.806	224.7	55.90	1.041	13.328
%RSD	.2100113	.1952768	.3980047	.0209528	.2041943
#1	6588.538	114930.1	14092.08	4968.416	6538.247
#2	6571.917	115327.3	14059.49	4966.355	6530.906
#3	6561.133	114946.6	13983.17	4967.637	6512.384

Sample Name: CCV04 Acquired: 8/11/2025 18:59:28 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCV04 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	4.887759	4.646670	4.807711	4.867973	4.868434	9.621884	9.590706
Stddev	.006060	.117257	.005988	.020437	.005825	.016578	.096874
%RSD	.1239804	2.523453	.1245410	.4198345	.1196406	.1722981	1.010087

#1	4.891151	4.541126	4.800798	4.856248	4.871685	9.629410	9.524603
#2	4.880763	4.625995	4.811119	4.856099	4.861709	9.602877	9.701908
#3	4.891364	4.772889	4.811217	4.891572	4.871907	9.633363	9.545608

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.2391652	2.422165	24.20188	.9794150	2.415304	1.226087	4.968076
Stddev	.0006487	.003145	.02036	.0015008	.003023	.001056	.034102
%RSD	.2712439	.1298330	.0841410	.1532325	.1251629	.0861225	.6864228

#1	.2398478	2.418589	24.19664	.9784038	2.412996	1.227287	4.928714
#2	.2385568	2.423403	24.18465	.9811394	2.414190	1.225303	4.986815
#3	.2390910	2.424501	24.22435	.9787018	2.418726	1.225669	4.988700

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	2.428748	24.03210	2.428036	1.209113	24.05300	2.434358	2.436601
Stddev	.004824	.03593	.001946	.000480	.07162	.009130	.008812
%RSD	.1986405	.1495266	.0801386	.0396690	.2977453	.3750413	.3616514

#1	2.426274	23.99452	2.425805	1.209302	23.97587	2.430759	2.446731
#2	2.425663	24.03565	2.429380	1.209469	24.11739	2.427575	2.432362
#3	2.434308	24.06612	2.428924	1.208568	24.06574	2.444738	2.430709

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	24.46848	4.745603	4.906743	4.823027	4.860585	4.899271	4.791966
Stddev	.14380	.017595	.011027	.008685	.004985	.016831	.007528
%RSD	.5876953	.3707720	.2247373	.1800678	.1025517	.3435511	.1570965

#1	24.31239	4.758097	4.898496	4.813411	4.855827	4.882427	4.783286
#2	24.59556	4.725481	4.902463	4.830299	4.860160	4.916090	4.795896
#3	24.49750	4.753231	4.919268	4.825372	4.865769	4.899296	4.796716

Sample Name: CCV04 Acquired: 8/11/2025 18:59:28 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCV04 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	4.750098	4.792677	4.844850
Stddev	.018458	.011171	.020220
%RSD	.3885717	.2330927	.4173538

#1	4.732215	4.783599	4.821543
#2	4.748998	4.789281	4.855314
#3	4.769081	4.805153	4.857695

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5704.466	98897.80	11506.32	4293.282	6803.481
Stddev	3.595	81.68	44.40	13.100	9.177
%RSD	.0630164	.0825872	.3858636	.3051314	.1348853

#1	5706.175	98972.22	11469.02	4279.877	6814.030
#2	5706.888	98810.42	11555.43	4306.054	6799.078
#3	5700.336	98910.75	11494.50	4293.915	6797.335

Sample Name: CCB04 Acquired: 8/11/2025 19:03:38 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCB04 Custom ID2: Custom ID3:
Comment:

Elem	As1890	Tl1908	Pb2203	Se1960	Sb2068	Al3961	Ba4934
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.001924	-.000510	-.000689	.0030955	.0008607	-.003448	-.003492
Stddev	.000131	.000505	.000802	.0011903	.0016924	.004257	.000608
%RSD	6.834025	98.95641	116.3904	38.45249	196.6318	123.4387	17.41838

#1	-.001848	-.000835	-.000605	.0044541	.0002092	-.007628	-.003561
#2	-.001847	.000072	.000068	.0022356	.0027820	-.003598	-.004063
#3	-.002076	-.000768	-.001529	.0025969	-.000409	.000881	-.002853

Elem	Be2348	Cd2265	Ca3736	Cr2677	Co2286	Cu2247	Fe2404
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.0000260	-.000081	-.019833	-.000247	-.000102	-.000446	-.019730
Stddev	.0000689	.000003	.002584	.000143	.000032	.000351	.004046
%RSD	264.6554	3.757070	13.03036	57.86986	31.03214	78.81899	20.50842

#1	.0000644	-.000080	-.022656	-.000110	-.000099	-.000850	-.021507
#2	-.000054	-.000078	-.019258	-.000396	-.000135	-.000208	-.022584
#3	.000067	-.000084	-.017584	-.000235	-.000072	-.000280	-.015100

Elem	Mn2576	Mg2790	Ni2316	Ag3280	Na5895	V_2924	Zn2138
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	-.000562	-.002805	-.000479	-.000037	.1491444	-.000069	-.000838
Stddev	.000312	.014434	.000079	.000317	.0154086	.002252	.000071
%RSD	55.46012	514.6193	16.58979	856.2835	10.33137	3287.085	8.416660

#1	-.000737	.008448	-.000436	-.000076	.1664830	-.002653	-.000902
#2	-.000202	.002216	-.000571	-.000333	.1439329	.001473	-.000848
#3	-.000747	-.019078	-.000430	.000298	.1370173	.000974	-.000763

Elem	K_7664	B_2496	Mo2020	Sn1899	Ti3361	Si2881	P_1774
Units	ppm	ppm	ppm	ppm	ppm	ppm	ppm
Avg	.1215116	-.000424	-.000053	.0007691	-.000655	.0027929	-.000164
Stddev	.0342705	.000235	.000072	.0005007	.001155	.0069410	.001710
%RSD	28.20349	55.47775	136.6771	65.10108	176.3413	248.5201	1045.510

#1	.1610264	-.000533	-.000088	.0006276	-.000103	-.005221	-.001941
#2	.0999079	-.000585	.000030	.0013253	-.001983	.006913	-.000020
#3	.1036007	-.000154	-.000100	.0003544	.000120	.006686	.001470

Sample Name: CCB04 Acquired: 8/11/2025 19:03:38 Type: Unk
Method: 6010-200.7 NEW(v90) Mode: CONC Corr. Factor: 1.000000
User: Jaswal Custom ID1: CCB04 Custom ID2: Custom ID3:
Comment:

Elem	S_1820	Li6707	Sr4077
Units	ppm	ppm	ppm
Avg	.0069289	.0018638	-.000251
Stddev	.0016868	.0007685	.000062
%RSD	24.34491	41.23430	24.51429

#1	.0082506	.0009814	-.000240
#2	.0050290	.0022235	-.000196
#3	.0075072	.0023866	-.000317

Int. Std.	Y_2243	Y_3600	Y_3710	Y_2243	In2306
Units	Cts/S	Cts/S	Cts/S	Cts/S	Cts/S
Avg	5909.247	102961.4	11326.71	4449.439	7567.643
Stddev	3.750	59.9	41.74	14.083	7.167
%RSD	.0634537	.0581454	.3685140	.3165077	.0947063

#1	5904.949	102897.2	11371.24	4434.525	7560.866
#2	5911.846	103015.7	11320.40	4462.509	7566.917
#3	5910.947	102971.3	11288.48	4451.283	7575.145

SOP ID : M3010A-Digestion-17

SDG No : N/A

Matrix : WATER

Pipette ID: ICP A

Balance ID : N/A

Filter paper ID : N/A

pH Strip ID : M6069

Hood ID : #3

Block ID: 1. HOT BLOCK #1 2. N/A

Start Digest Date: 08/08/2025 Time : 11:10 Temp : 96 °C

End Digest Date: 08/08/2025 Time : 14:12 Temp : 96 °C

Digestion tube ID: M5595

Block thermometer ID: MET-DIG. #1

Dig Technician Signature: *S123*

Supervisor Signature: *Jerp*

Temp : 1. 96°C 2. N/A

Standard Name	MLS USED	STD REF. # FROM LOG
LFS-1	0.25	M6180
LFS-2	0.25	M6181
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
CONC: HNO3	3.00	M6158
1:1 HCL	5.00	MP85156
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

HOT BLOCK#1 CELL#50 96C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
08/08/25 15:12	<i>S123 met lab</i>	<i>Jerp / Metlab</i>
	Preparation Group	Analysis Group

Lab Sample ID	Client Sample ID	pH	Initial Vol (ml)	Final Vol (ml)	Color Before	Color After	Clarity Before	Clarity After	Comment	Prep Pos
PB169154BL	PBW154	<2	50	25	Colorless	Colorless	Clear	Clear	N/A	1
PB169154BS	LCS154	<2	50	25	Colorless	Colorless	Clear	Clear	M6180,M6181	2
Q2759-04	LIQUID-DRUM	<2	5.00	25	Colorless	Colorless	Clear	Clear	N/A	3
Q2804-01	WATER-TREATMENT DISCHARGE	<2	50	25	Colorless	Colorless	Clear	Clear	N/A	4
Q2805-01	RW8-SP100-20250807	<2	50	25	Colorless	Colorless	Clear	Clear	N/A	5
Q2805-02	RW8-SP303-20250807	<2	50	25	Colorless	Colorless	Clear	Clear	N/A	6
Q2805-02MS	RW8-SP303-20250807MS	<2	50	25	Colorless	Colorless	Clear	Clear	M6180,M6181	8
Q2805-02MSD	RW8-SP303-20250807MSD	<2	50	25	Colorless	Colorless	Clear	Clear	M6180,M6181	9
Q2805-02DUP	RW8-SP303-20250807DUP	<2	50	25	Colorless	Colorless	Clear	Clear	N/A	7

WORKLIST(Hardcopy Internal Chain)

WorkList Name : PB169154

WorkList ID : 191149

Department : Digestion

Date : 08-07-2025 08:34:49

Sample	Customer Sample	Matrix	Test	Preservative	Customer	Raw Sample Storage Location	Collect Date	Method
Q2805-01	RW8-SP100-20250807	Water	Metals Group4	1:1 HNO3 to pH < 2	TETR06	J22	08/07/2025	6010D
Q2805-02	RW8-SP303-20250807	Water	Metals Group4	1:1 HNO3 to pH < 2	TETR06	J22	08/07/2025	6010D
Q2759-04	LIQUID-DRUM	Water	Metals PSEG Group2	1:1 HNO3 to pH < 2	PSEG03	D31	08/04/2025	6010D
Q2804-01	WATER-TREATMENT DISCHAI	Water	Metals Group4	1:1 HNO3 to pH < 2	VERI01	J22	08/07/2025	6010D

Date/Time 08/07/25 10:53
Raw Sample Received by: SKS met dip
Raw Sample Relinquished by: Crcan

Date/Time 08/08/25 11:23
Raw Sample Received by: Crcan
Raw Sample Relinquished by: SKS met dip

Instrument ID: P4

Daily Analysis Runlog For Sequence/QC Batch ID # LB136779

Review By	Janvi	Review On	8/13/2025 10:17:16 AM
Supervise By	jaswal	Supervise On	8/13/2025 4:06:52 PM
STD. NAME	STD REF.#		
ICAL Standard	MP86640,MP86656,MP86653,MP86643,MP86642,MP86641		
ICV Standard	MP86752,MP86656		
CCV Standard	MP86646		
ICSA Standard	MP86651,MP86753		
CRI Standard	MP86656		
LCS Standard			
Chk Standard	MP86647,MP86648		

Sr#	SampleId	ClientID	QcType	Date	Comment	Operator	Status
1	S0	S0	CAL1	08/11/25 16:19		Jaswal	OK
2	S1	S1	CAL2	08/11/25 16:23		Jaswal	OK
3	S2	S2	CAL3	08/11/25 16:27		Jaswal	OK
4	S3	S3	CAL4	08/11/25 16:31		Jaswal	OK
5	S4	S4	CAL5	08/11/25 16:36		Jaswal	OK
6	S5	S5	CAL6	08/11/25 16:40		Jaswal	OK
7	ICV01	ICV01	ICV	08/11/25 16:44		Jaswal	OK
8	LLICV01	LLICV01	LLICV	08/11/25 16:49		Jaswal	OK
9	ICB01	ICB01	ICB	08/11/25 16:54		Jaswal	OK
10	CRI01	CRI01	CRDL	08/11/25 16:58		Jaswal	OK
11	ICSA01	ICSA01	ICSA	08/11/25 17:02		Jaswal	OK
12	ICSAB01	ICSAB01	ICSAB	08/11/25 17:06		Jaswal	OK
13	ICSADL	ICSADL	ICSA	08/11/25 17:10		Jaswal	OK
14	ICSABDL	ICSABDL	ICSAB	08/11/25 17:15		Jaswal	OK
15	CCV01	CCV01	CCV	08/11/25 17:19		Jaswal	OK
16	CCB01	CCB01	CCB	08/11/25 17:23		Jaswal	OK
17	Q2759-04	LIQUID-DRUM	SAM	08/11/25 17:27		Jaswal	OK
18	Q2801-01	TR-04-080725	SAM	08/11/25 17:31		Jaswal	OK

Instrument ID: P4

Daily Analysis Runlog For Sequence/QC Batch ID # LB136779

Review By	Janvi	Review On	8/13/2025 10:17:16 AM
Supervise By	jaswal	Supervise On	8/13/2025 4:06:52 PM

STD. NAME	STD REF.#
ICAL Standard	MP86640,MP86656,MP86653,MP86643,MP86642,MP86641
ICV Standard	MP86752,MP86656
CCV Standard	MP86646
ICSA Standard	MP86651,MP86753
CRI Standard	MP86656
LCS Standard	
Chk Standard	MP86647,MP86648

19	Q2769-01	001-WILLETS-PT-BLV	SAM	08/11/25 17:35		Jaswal	OK
20	Q2769-04	002-35TH-AVE(AUG)	SAM	08/11/25 17:40		Jaswal	OK
21	CCV02	CCV02	CCV	08/11/25 17:44		Jaswal	OK
22	CCB02	CCB02	CCB	08/11/25 17:48		Jaswal	OK
23	PB169154BL	PB169154BL	MB	08/11/25 17:52		Jaswal	OK
24	PB169154BS	PB169154BS	LCS	08/11/25 17:57		Jaswal	OK
25	Q2804-01	WATER-TREATMENT	SAM	08/11/25 18:01		Jaswal	OK
26	Q2805-01	RW8-SP100-2025080	SAM	08/11/25 18:05		Jaswal	OK
27	Q2805-02	RW8-SP303-2025080	SAM	08/11/25 18:09		Jaswal	OK
28	Q2805-02DUP	RW8-SP303-2025080	DUP	08/11/25 18:14		Jaswal	OK
29	Q2805-02L	RW8-SP303-2025080	SD	08/11/25 18:18		Jaswal	OK
30	Q2805-02MS	RW8-SP303-2025080	MS	08/11/25 18:22		Jaswal	OK
31	CCV03	CCV03	CCV	08/11/25 18:26		Jaswal	OK
32	CCB03	CCB03	CCB	08/11/25 18:30		Jaswal	OK
33	Q2805-02MSD	RW8-SP303-2025080	MSD	08/11/25 18:35		Jaswal	OK
34	Q2805-02A	RW8-SP303-2025080	PS	08/11/25 18:38	0.1ML OF EACH M6004 AND M6017	Jaswal	OK
35	Q2807-01	COMP-4	SAM	08/11/25 18:42		Jaswal	OK
36	Q2807-02	COMP-5	SAM	08/11/25 18:47		Jaswal	OK
37	Q2807-03	COMP-6	SAM	08/11/25 18:51		Jaswal	OK

Instrument ID: P4

Daily Analysis Runlog For Sequence/QC Batch ID # LB136779

Review By	Janvi	Review On	8/13/2025 10:17:16 AM
Supervise By	jaswal	Supervise On	8/13/2025 4:06:52 PM

STD. NAME	STD REF.#
ICAL Standard	MP86640,MP86656,MP86653,MP86643,MP86642,MP86641
ICV Standard	MP86752,MP86656
CCV Standard	MP86646
ICSA Standard	MP86651,MP86753
CRI Standard	MP86656
LCS Standard	
Chk Standard	MP86647,MP86648

38	Q2798-01	TP-6	SAM	08/11/25 18:55		Jaswal	OK
39	CCV04	CCV04	CCV	08/11/25 18:59		Jaswal	OK
40	CCB04	CCB04	CCB	08/11/25 19:03		Jaswal	OK

Prep Standard - Chemical Standard Summary

Order ID : Q2805

Test : Metals Group4

Prepbatch ID : PB169154,

Sequence ID/Qc Batch ID: LB136779, LB136779,

Standard ID :

MP85156, MP86640, MP86641, MP86642, MP86643, MP86646, MP86647, MP86648, MP86651, MP86653, MP86655, MP86656, MP86752, MP86753,

Chemical ID :

M5467, M5658, M5697, M5748, M5798, M5799, M5800, M5801, M5805, M5814, M5816, M5820, M5962, M5969, M5970, M5979, M5985, M5998, M6021, M6023, M6027, M6028, M6030, M6032, M6058, M6076, M6077, M6086, M6128, M6137, M6140, M6142, M6144, M6145, M6146, M6151, M6158, M6159, M6162, M6163, M6164, M6165, M6171, M6174, M6176, M6177, M6178, M6179, M6180, M6181, M6182, M6184, W3112,

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
170	1:1HCL	MP85156	04/07/2025	09/06/2025	Kareem Khairalla	None	None	Sarabjit Jaswal 04/07/2025

FROM 1250.00000ml of M6151 + 1250.00000ml of W3112 = Final Quantity: 2500.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
902	ICP AES CAL BLK (SO/ICB/CCB)	MP86640	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025

FROM 125.00000ml of M6151 + 2350.00000ml of W3112 + 25.00000ml of M6162 = Final Quantity: 2500.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
907	ICP AES STD S (S5)	MP86641	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025
FROM 5.00000ml of M5467 + 5.00000ml of M5820 + 5.00000ml of M5969 + 5.00000ml of M5970 + 5.00000ml of M5998 + 5.00000ml of M6077 + 5.00000ml of M6146 + 5.00000ml of M6174 + 5.00000ml of M6176 + 455.00000ml of MP86640 = Final Quantity: 500.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
910	ICP AES STD S4	MP86642	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025
FROM 50.00000ml of MP86640 + 50.00000ml of MP86641 = Final Quantity: 100.000 ml								

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
909	ICP AES STD S3	MP86643	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP	Sarabjit Jaswal

A)

FROM 25.00000ml of MP86641 + 75.00000ml of MP86640 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
911	ICP AES CCV SOLN	MP86646	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP	Sarabjit Jaswal

A)

FROM 50.00000ml of MP86640 + 50.00000ml of MP86641 = Final Quantity: 100.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
919	ICP AES INTERNAL STD	MP86647	08/06/2025	08/27/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025
FROM 1.00000ml of M6179 + 10.00000ml of M5985 + 1969.00000ml of W3112 + 20.00000ml of M6162 = Final Quantity: 2000.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
903	ICP AES RINSE SOLN	MP86648	08/06/2025	08/27/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025
FROM 200.00000ml of M6162 + 9800.00000ml of W3112 = Final Quantity: 10000.000 ml								

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
904	ICP AES ICSA SOLN	MP86651	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP	Sarabjit Jaswal

A)

FROM 5.00000ml of M6182 + 45.00000ml of MP86640 = Final Quantity: 50.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3913	ICP AES STD S2	MP86653	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP	Sarabjit Jaswal

A)

FROM 4.00000ml of MP86641 + 46.00000ml of MP86640 = Final Quantity: 50.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2950	ICP AES S1/CRI STOCK STD	MP86655	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025

FROM 0.00000ml of M5748 + 0.00000ml of M5805 + 0.03000ml of M5798 + 0.03000ml of M6028 + 0.05000ml of M5658 + 0.05000ml of M6030 + 0.05000ml of M6140 + 0.05000ml of M6159 + 0.06000ml of M6177 + 0.10000ml of M5697 + 0.10000ml of M5801 + 0.10000ml of M5816 + 0.10000ml of M5820 + 0.10000ml of M5962 + 0.10000ml of M5970 + 0.10000ml of M6128 + 0.10000ml of M6176 + 0.15000ml of M5800 + 0.20000ml of M5799 + 0.20000ml of M5979 + 0.20000ml of M6021 + 0.20000ml of M6023 + 0.20000ml of M6027 + 0.20000ml of M6145 + 0.25000ml of M5467 + 0.25000ml of M6146 + 0.50000ml of M5814 + 0.50000ml of M6032 + 1.00000ml of M6086 + 1.00000ml of M6142 + 1.00000ml of M6144 + 1.00000ml of M6171 + 1.00000ml of M6178 + 2.00000ml of M6137 + 89.03000ml of MP86640 = Final Quantity: 100.000 ml

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
2951	ICP AES S1/CRI WORK STD	MP86656	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/07/2025

FROM 1.00000ml of MP86655 + 49.00000ml of MP86640 = Final Quantity: 50.000 ml

Metals STANDARD PREPARATION LOG

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
4163	NEW ICV-060925	MP86752	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/14/2025
FROM 0.20000ml of M6058 + 0.40000ml of M6163 + 0.40000ml of M6164 + 0.40000ml of M6165 + 48.60000ml of MP86640 = Final Quantity: 50.000 ml								

<u>Recipe ID</u>	<u>NAME</u>	<u>NO.</u>	<u>Prep Date</u>	<u>Expiration Date</u>	<u>Prepared By</u>	<u>ScaleID</u>	<u>PipetteID</u>	<u>Supervised By</u>
3494	ICP AES ICSAB SOLN-1	MP86753	08/06/2025	08/18/2025	Janvi Patel	None	METALS_PIPETTE_1 (ICP A)	Sarabjit Jaswal 08/14/2025
FROM 0.05000ml of M6076 + 5.00000ml of M6182 + 5.00000ml of M6184 + 39.95000ml of MP86640 = Final Quantity: 100.000 ml								

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57058 / Cerium, 1000PPM, 100ML	020623	02/06/2026	03/06/2023 / bin	03/01/2023 / bin	M5467

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58024 / Chromium, Cr, 500 ml, 1000 PPM	060523	06/05/2026	08/28/2023 / jaswal	08/25/2023 / jaswal	M5658

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58029 / Cu, 1000 PPM, 500 ml	102523	10/25/2026	04/03/2024 / jaswal	10/27/2023 / jaswal	M5697

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Nickel (Ni) 1000PPM	091223	09/12/2026	01/02/2024 / bin	12/20/2023 / jaswal	M5748

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57004 / Be, 1000 PPM, 125 ml	102523	10/25/2026	02/09/2024 / bin	02/09/2024 / bin	M5798

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57050 / Sn, 1000 PPM, 125 ml	071123	07/11/2026	02/09/2024 / bin	02/09/2024 / bin	M5799

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57027 / CO, 1000 PPM, 125 ml	091923	09/19/2026	05/31/2024 / bin	02/09/2024 / bin	M5800

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57033 / As, 1000 PPM, 125 ml	111323	11/13/2026	02/09/2024 / bin	02/09/2024 / bin	M5801

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58120 / Ca, 10000 PPM, 500 ml	122223	12/22/2026	04/17/2025 / Janvi	01/03/2024 / jaswal	M5805

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57005 / B, 1000 PPM, 125 ml	071123	07/11/2026	03/26/2024 / Sohil	01/03/2024 / jaswal	M5814

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57016 / S, 1000 PPM, 125 ml	122923	12/29/2026	05/20/2024 / Jaswal	02/09/2024 / jaswal	M5816

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57015 / P, 1000 PPM, 125 ml	091123	09/11/2026	05/01/2024 / jaswal	02/09/2024 / jaswal	M5820

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57034 / Se, 1000 PPM, 125 ml	060624	06/06/2027	07/02/2024 / Jaswal	06/14/2024 / Jaswal	M5962

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57016 / S, 1000 PPM, 125 ml	122923	03/31/2026	03/31/2025 / kareem	06/11/2024 / Jaswal	M5969

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57003 / Li, 1000 PPM, 125 ml	061224	06/21/2027	07/01/2024 / Jaswal	07/01/2024 / Jaswal	M5970

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGTI1-1 / TITANIUM 125mL 1000ug/mL	T2-TI719972	08/05/2026	08/06/2025 / Janvi	02/22/2024 / Jaswal	M5979

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGIN10-5 / INDIUM 1 x 500 ml	U2-IN729349	02/21/2028	10/08/2024 / Jaswal	06/14/2024 / Jaswal	M5985

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CLPP-CAL-3 / CLP CAL SOLUTION #3, 125mL	T2-MEB727800	07/30/2026	07/30/2025 / Janvi	02/22/2024 / kareem	M5998

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57023 / V, 1000 PPM, 125 ml	062424	06/24/2027	09/28/2024 / jaswal	08/05/2024 / Jaswal	M6021

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57081 / TI, 1000 PPM, 125 ml	0624724	06/27/2027	08/05/2024 / kareem	08/05/2024 / Jaswal	M6023

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57028 / Ni, 1000 PPM, 125 ml	062024	06/20/2027	06/04/2025 / Janvi	08/05/2024 / Jaswal	M6027

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57048 / Cd, 1000 PPM, 125 ml	070124	07/01/2027	08/05/2024 / kareem	08/05/2024 / Jaswal	M6028

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57047 / Ag, 1000 PPM, 125 ml	122823	12/28/2026	08/05/2024 / kareem	08/05/2024 / Jaswal	M6030

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57056 / Ba, 1000 PPM, 125 ml	010924	01/09/2027	01/14/2025 / Jaswal	08/05/2024 / Jaswal	M6032

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CHEM-QC-4 / CHEM-QC-4, Second Source, 1000 ug/ml, B, Mo, Si, Sn, Ti	V2-MEB746173	01/29/2026	01/29/2025 / JANVI	08/22/2024 / Jaswal	M6058

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	Z9651Q / CHEM-CLP-4/.25L	V2-MEB746762	01/01/2026	01/01/2025 / kareem	09/19/2024 / kareem	M6076

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	Z9651Q / CHEM-CLP-4/.25L	V2-MEB746762	09/06/2029	01/23/2025 / kareem	09/19/2024 / kareem	M6077

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58120 / Calcium, 500 ml, 10000 PPM	082324	08/23/2027	03/06/2025 / JANVI	10/14/2024 / jaswal	M6086

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58025 / Mn, 1000 PPM, 500 ml	101124	10/11/2027	01/13/2025 / kareem	01/13/2025 / kareem	M6128

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGSI1-1 / SILICON 125mL 1000ug/mL	V2-SI744713	07/10/2029	01/14/2025 / Jaswal	10/03/2024 / Jaswal	M6137

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58126 / Fe, 10000 PPM, 500 ml	011025	01/10/2028	06/25/2025 / Janvi	01/13/2025 / Jaswal	M6140

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58119 / K, 10000 PPM, 500 ml	103024	10/30/2027	05/06/2025 / JANVI	01/13/2025 / Jaswal	M6142

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58111 / Na, 10000 PPM, 500 ml	072424	07/24/2027	01/23/2025 / kareem	01/13/2025 / Jaswal	M6144

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58030 / Zinc, Zn, 500 ml, 1000 PPM	121724	12/17/2027	02/04/2025 / jaswal	01/13/2025 / Jaswal	M6145

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57051 / Sb, 1000 PPM, 125 ml	071724	07/17/2027	01/31/2025 / kareem	10/18/2024 / kareem	M6146

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9530-33 / Hydrochloric Acid, Instra-Analyzed (cs/6x2.5L)	22G2862015	08/17/2025	02/18/2025 / Sagar	01/15/2025 / Sagar	M6151

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9598-34 / Nitric Acid, Instra-Analyzed (cs/4x2.5L)	24D1062002	09/09/2025	03/10/2025 / Eman	02/02/2025 / Sagar	M6158

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58113 / Al, 10000 PPM, 500 ml	011325	03/18/2026	03/18/2025 / kareem	02/09/2025 / kareem	M6159

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	BA-9598-34 / Nitric Acid, Instra-Analyzed (cs/4x2.5L)	24H0162012	11/27/2025	05/27/2025 / Sagar	04/27/2025 / Sagar	M6162

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	QCP-CICV-1-125ML / EPA CLP ICP Verification Standard1	V2-MEB744107	06/08/2026	06/09/2025 / jaswal	06/06/2025 / jaswal	M6163

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	QCP-CICV-2-125ML / EPA CLP ICP Verification Standard2	U2-MEB733713	06/08/2026	06/09/2025 / jaswal	06/09/2025 / jaswal	M6164

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	QCP-CICV-3-125ML / EPA CLP ICP Verification Standard3	V2-MEB749572	06/08/2026	06/09/2025 / jaswal	06/09/2025 / jaswal	M6165

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	58112 / Mg, 10000 PPM, 500 ml	011525	01/15/2028	07/15/2025 / jaswal	02/13/2025 / Janvi	M6171

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CLPP-CAL-1 / CLP CAL SOLUTION #1, 125mL	V2-MEB742428	07/31/2026	07/31/2025 / Janvi	05/05/2025 / Janvi	M6174

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57038 / Sr, 1000 PPM, 125 ml	092724	09/27/2027	08/06/2025 / Janvi	08/06/2025 / Janvi	M6176

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	/ Lead (Pb) 1000PPM	031525	03/15/2028	08/06/2025 / Janvi	08/06/2025 / Janvi	M6177

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Absolute Standards, Inc.	57042 / Mo, 1000 PPM, 125 ml	080528	08/05/2028	08/06/2025 / Janvi	08/06/2025 / Janvi	M6178

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	CGY10-1 / YTTRIUM 125mL 10,000ug/mL	V2-Y740548	08/05/2026	08/06/2025 / Janvi	06/02/2024 / Janvi	M6179

CHEMICAL RECEIPT LOG BOOK

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	WW-LFS-1 / Laboratory Fortified Stock Solution 1, 125 ml	W2-MEB752149	02/05/2026	08/06/2025 / Janvi	07/22/2025 / Janvi	M6180

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Inorganic Ventures	WW-LFS-2 / Laboratory Fortified Stock Solution 2, 125 ml	V2-MEB7433480	02/05/2026	08/06/2025 / Janvi	07/22/2025 / Janvi	M6181

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
EPA	PART A / ICSA (ICP) STOCK SOLN	ICSA-1211	02/05/2026	08/06/2025 / Janvi	03/06/2024 / Janvi	M6182

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
EPA	PART B / ICSAB (ICP) STOCK SOLN	ICSB-0710	02/05/2026	08/06/2025 / Janvi	03/06/2024 / Janvi	M6184

Supplier	ItemCode / ItemName	Lot #	Expiration Date	Date Opened / Opened By	Received Date / Received By	Chemtech Lot #
Seidler Chemical	DIW / DI Water	Daily Lab-Certified	07/03/2029	07/03/2024 / Iwona	07/03/2024 / Iwona	W3112



M6032




CERTIFIED WEIGHT REPORT:

Part Number: 57056
Lot Number: 010924
Description: Barium (Ba)
Solvent: Nitric Acid
Lot #
Expiration Date: 010927
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 2000.02
Balance Uncertainty: 5E-05
Flask Uncertainty: 0.058

Giovanni Caporaso	
Formulated By:	Giovanni Esposito
	010924
Reviewed By:	Pedro L. Renteria
	010924

SDS Information									
Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)
1. Barium nitrate (Ba)	IN023	BA0022019A1	1000	99.999	0.10	52.3	3.82417	3.82441	1000.1

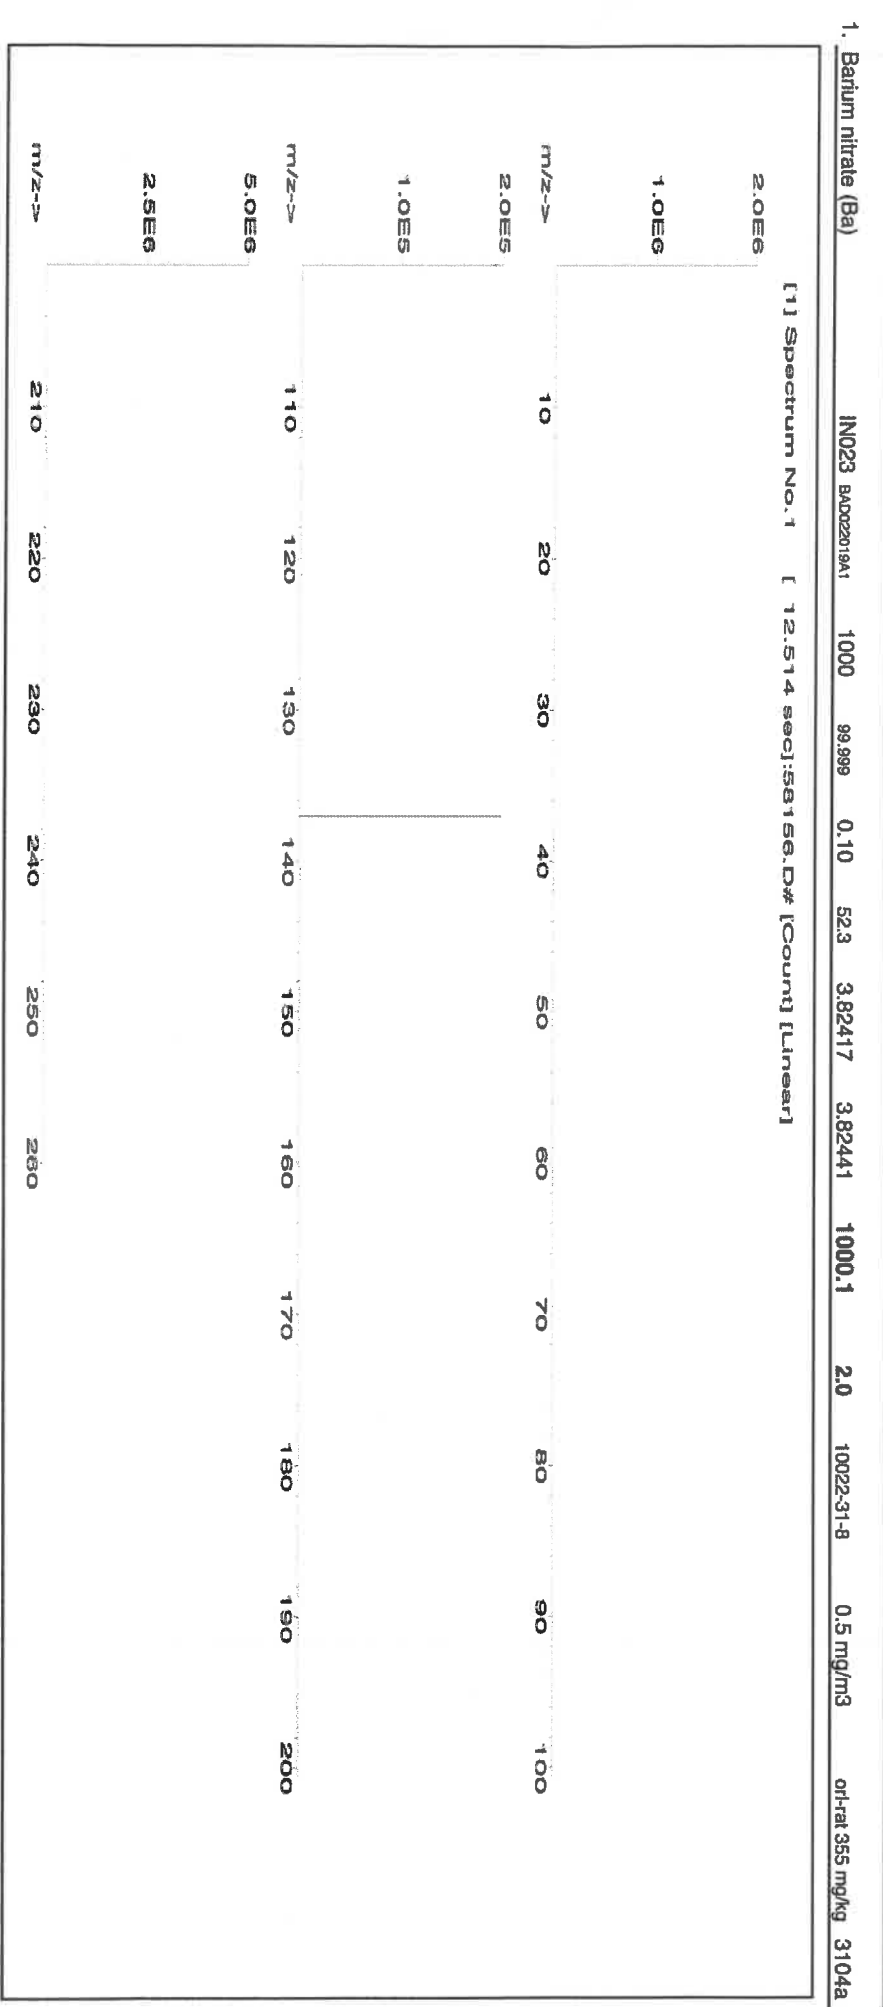



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	T	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number: 58120
Lot Number: 122223
Description: Calcium (Ca)

Solvent: 24002546 Nitric Acid

Lot #

Expiration Date: 122226

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 10000

NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 4000.0

5E-05 Balance Uncertainty
0.06 Flask Uncertainty

2% 80.0 mL Nitric Acid


Giovanni Caporaso	
Formulated By:	Giovanni Esposito
	122223
Reviewed By:	Pedro L. Renteria
	122223

Compound

Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Expanded	SDS Information	NIST
RM#	Number	Conc. (µg/mL)	(%)	Purity (%)	Weight (g)	Weight (g)	Conc. (µg/mL)	+/- (µg/mL)	(Solvent Safety Info. On Attached pg.)	SRM

1. Calcium carbonate (Ca) IN014 CAD0302383 10000 99.999 0.10 39.9 100.2525 100.2670 10001.4 20.0 471.34-1 5 mg/m3 off-ral >2000mg/kg 3109a

[1] Spectrum No.1 [12.514 sec]:58120.D# [Count] [Linear]

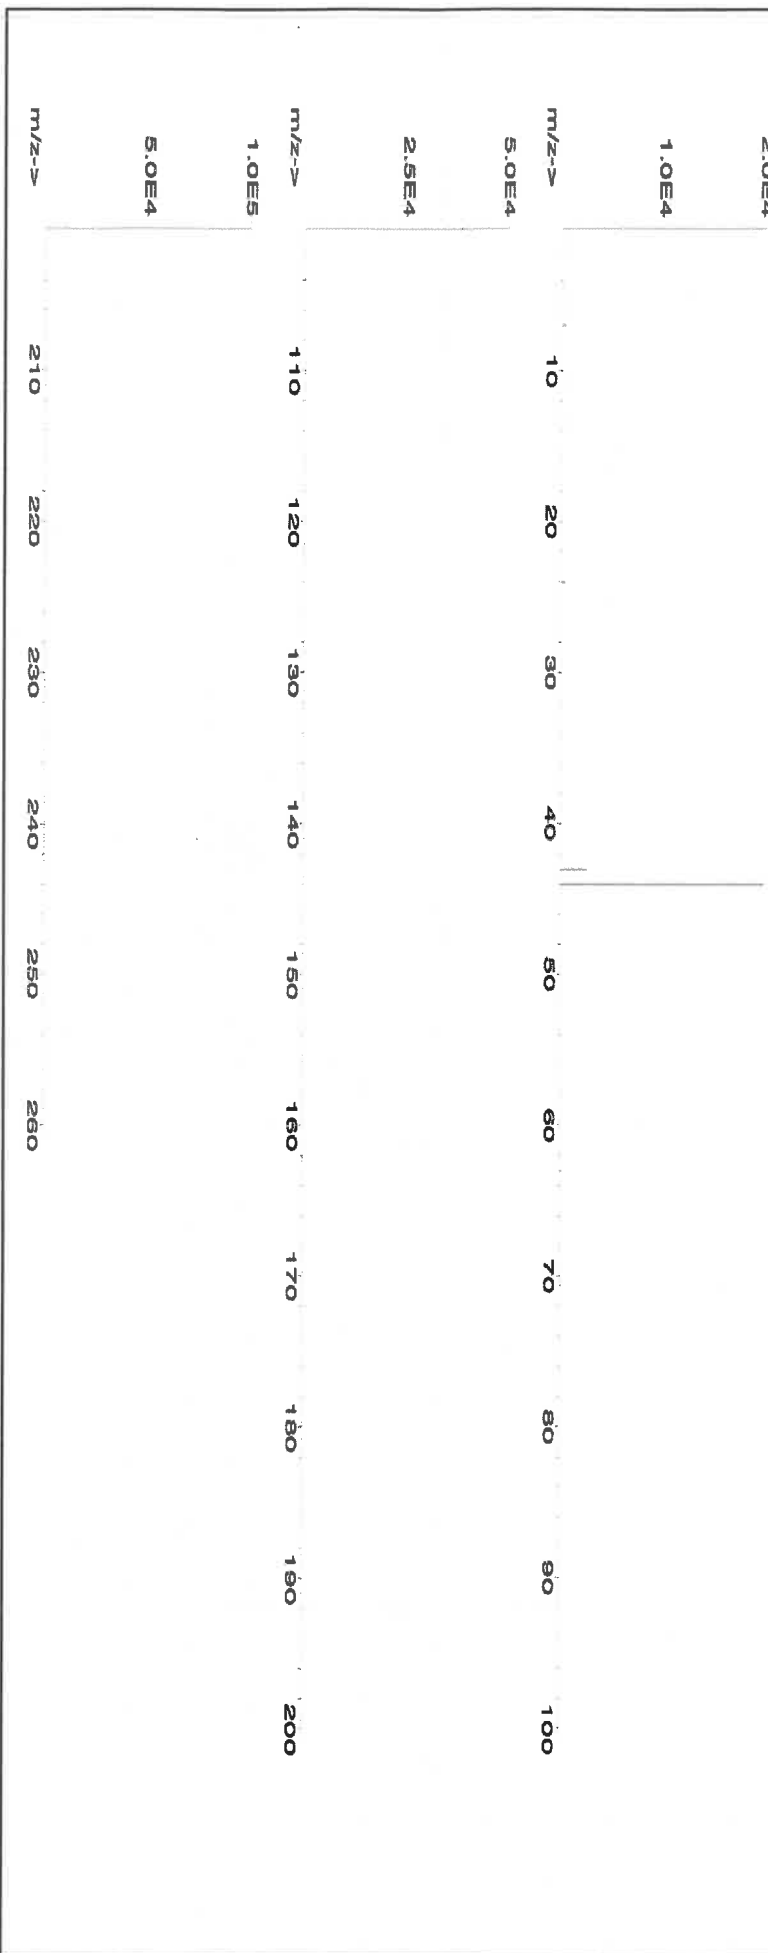



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	T	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Ti	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	30	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pr	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



Rev'd 2/10/14/2021 M6085 / M6086 / M6087

CERTIFIED WEIGHT REPORT:

Part Number: 58120
Lot Number: 082324
Description: Calcium (Ca)

Solvent: 24002546 Nitric Acid

Lot #

2% 80.0 (mL) Nitric Acid

Expiration Date: 082327

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 10000

NIST Test Number: 6UTB

Weight shown below was diluted to (mL): 4000.1 0.15 Flask Uncertainty


<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
Reviewed By:	Pedro L. Rentas
	082324

SDS Information

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-----	------------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Calcium carbonate (Ca) IN014 CAD03202383 10000 99.999 0.10 39.9 100.2537 100.2656 10001.2 20.0 471-34-1 5 mg/m3 or-rel >2000mg/kg 3109a

[1] Spectrum No. 1 [12.514 sec]:58120.D* [Count] [Linear]

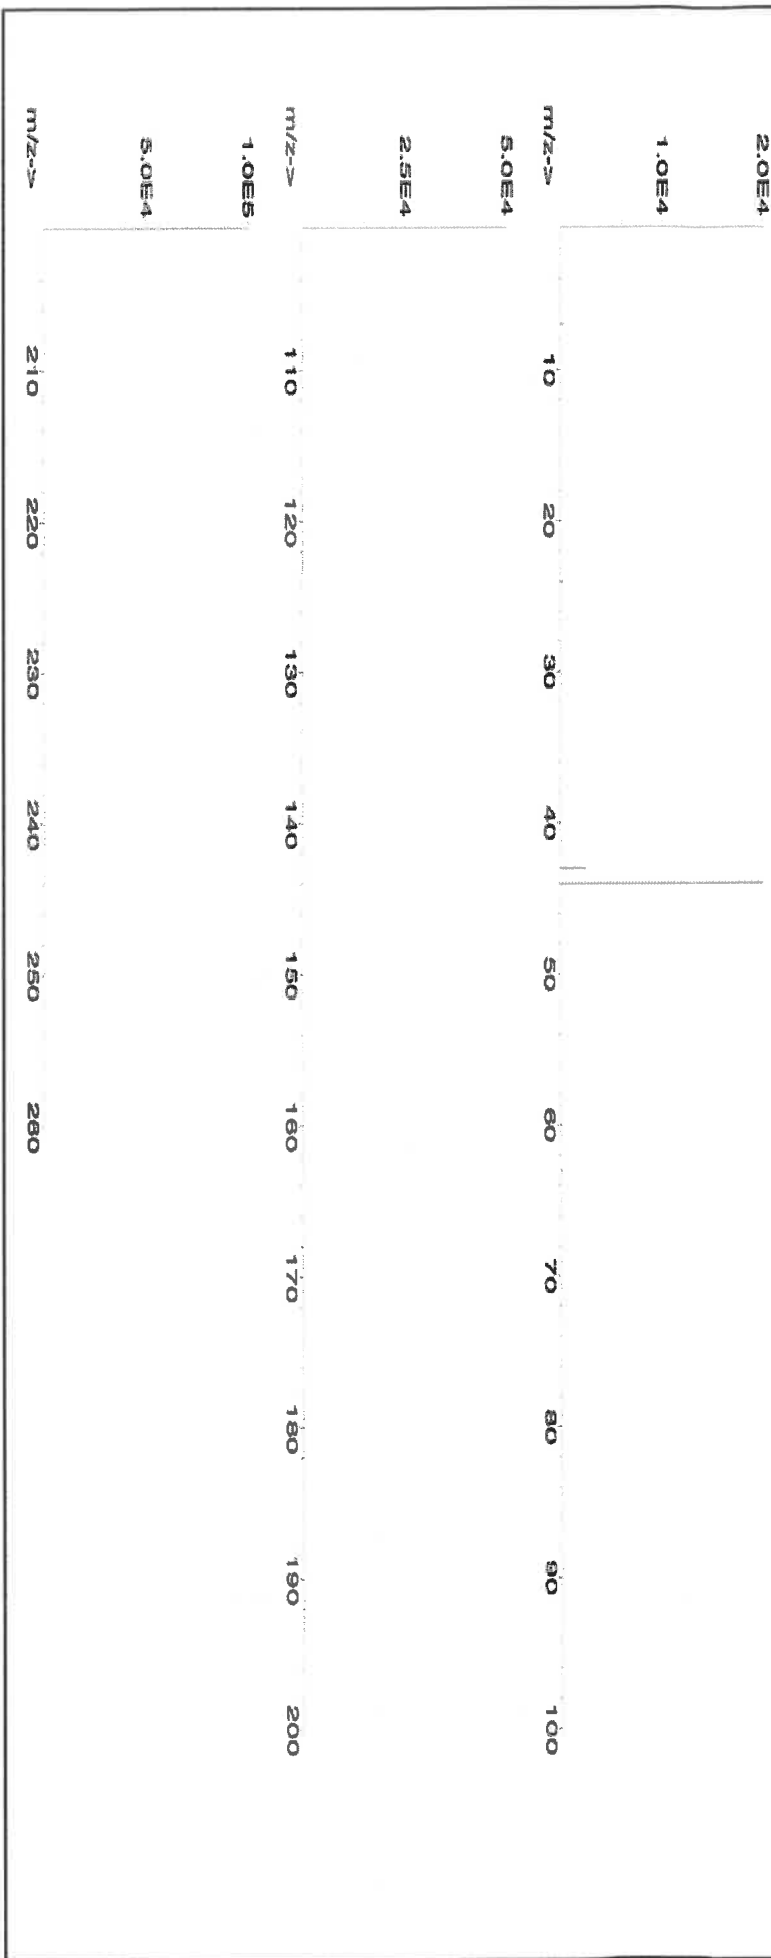



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	T	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	30	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Su	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



M6028



CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57048
070124
Cadmium (Cd)

Lot #
Solvent: 24002546 Nitric Acid

2% 40.0 (mL) Nitric Acid

Expiration Date:

070127

Recommended Storage:
Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

Weight shown below was diluted to (mL):

2000.07

SE-05 Balance Uncertainty
0.100 Flask Uncertainty

<i>Aleah O'Brady</i>	
Formulated By:	Aleah O'Brady
	070124
<i>Pedro L. Rentas</i>	
Reviewed By:	Pedro L. Rentas
	070124

Compound

Lot
Number
Nominal
Conc. (µg/mL)
Purity (%)
Uncertainty (%)
Assay (%)

Target
Weight (g)
Actual
Weight (g)
Actual
Conc. (µg/mL)

Expanded
Uncertainty
+/- (µg/mL)
CAS#
OSHA PEL (TWA)


SDS Information

(Solvent Safety Info. On Attached pg.)

NIST
SRM

1. Cadmium nitrate tetrahydrate (Cd) IN024 CDM09221A1 1000 99.999 0.10 36.5 5.4797 5.4804 1000.1 2.0 10022-68-1 0.01 mg/m3 or-rat 60.2mg/kg 3108

[1] Spectrum No.1 [12.514 sec]:\$8148.D# [Count] [Linear]

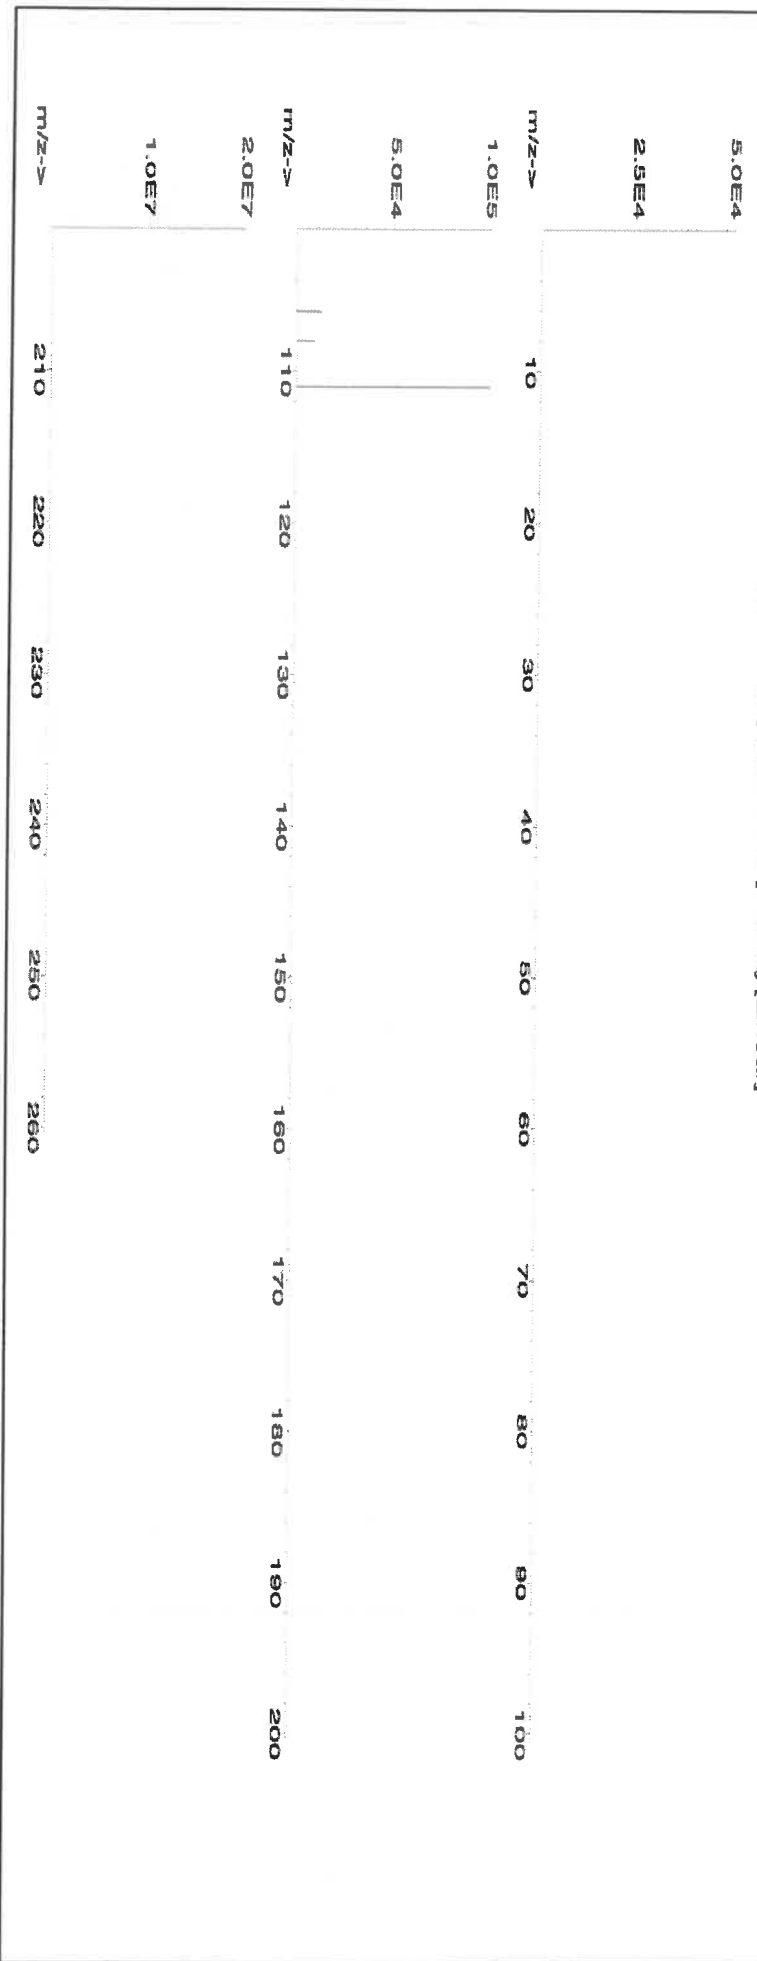



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.2	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Ba	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Cd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pr	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



N5467 R: 03/01/23 (14)

CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57058
020623
Cerium (Ce)

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):
NIST Test Number:

020626
Ambient (20 °C)
1000
6UTB

Weight shown below was diluted to (mL):

1000.12

5E-05 Balance Uncertainty

0.058 Flask Uncertainty

Lot #


Solvent: 21110221 Nitric Acid

2% 20.0 Nitric Acid (mL)

Formulated By:	Lawrence Barry
Reviewed By:	Pedro L. Rentas

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	SDS Information		
										(Solvent Safety Info. On Attached pg.)	CAS#	LD50
1. Cerium nitrate hexahydrate (Ce)	IN146	Z512CEB1	1000	99.999	0.10	32.8	3.04919	3.04921	1000.0	2.0	10294-41-4	NA
											NA	NA

[1] Spectrum No.1 [43.472 sec]58158.D# [Count] [Linear]

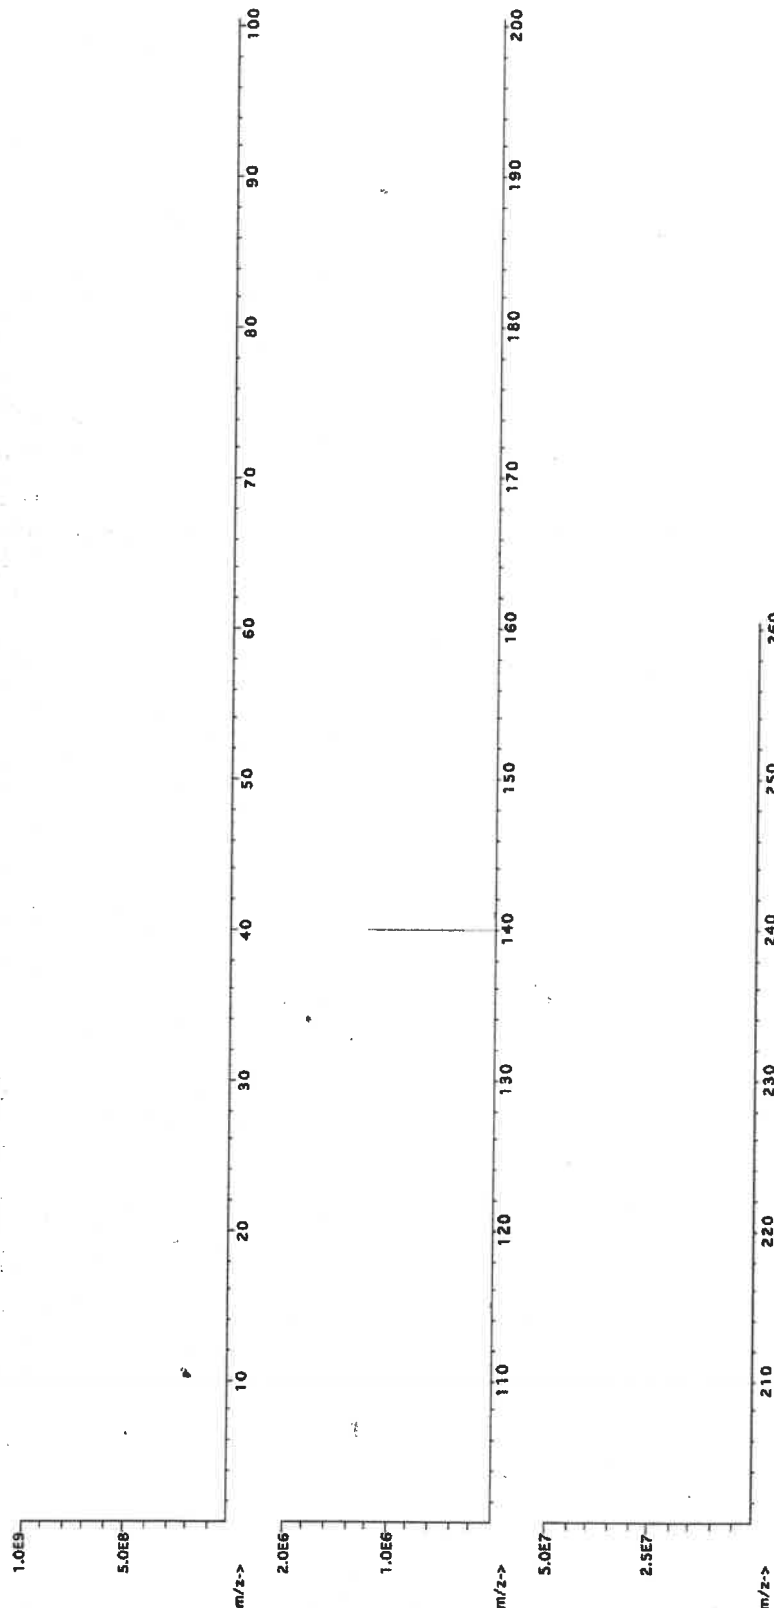



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	La	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.2	Ce	T	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T)= Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58024
Lot Number: 060523
Description: Chromium (Cr)

Lot # 21110221
Solvent: Nitric Acid


Formulated By:	Lawrence Barry
	060523
Reviewed By:	Pedro L. Ruelas
	060523

Expiration Date: 060526
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Volume shown below was diluted to (mL): 2000.02 0.058 Balance Uncertainty
Flask Uncertainty

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Chromium(III) nitrate nonahydrate (Cr) 58124 071122 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 7789-02-8 0.5 mg(Cr)/m3 or rat 3250 mg/kg 3112a

[1] Spectrum No.1 [31.393 sec]:57024.D# [Count] [Linear]

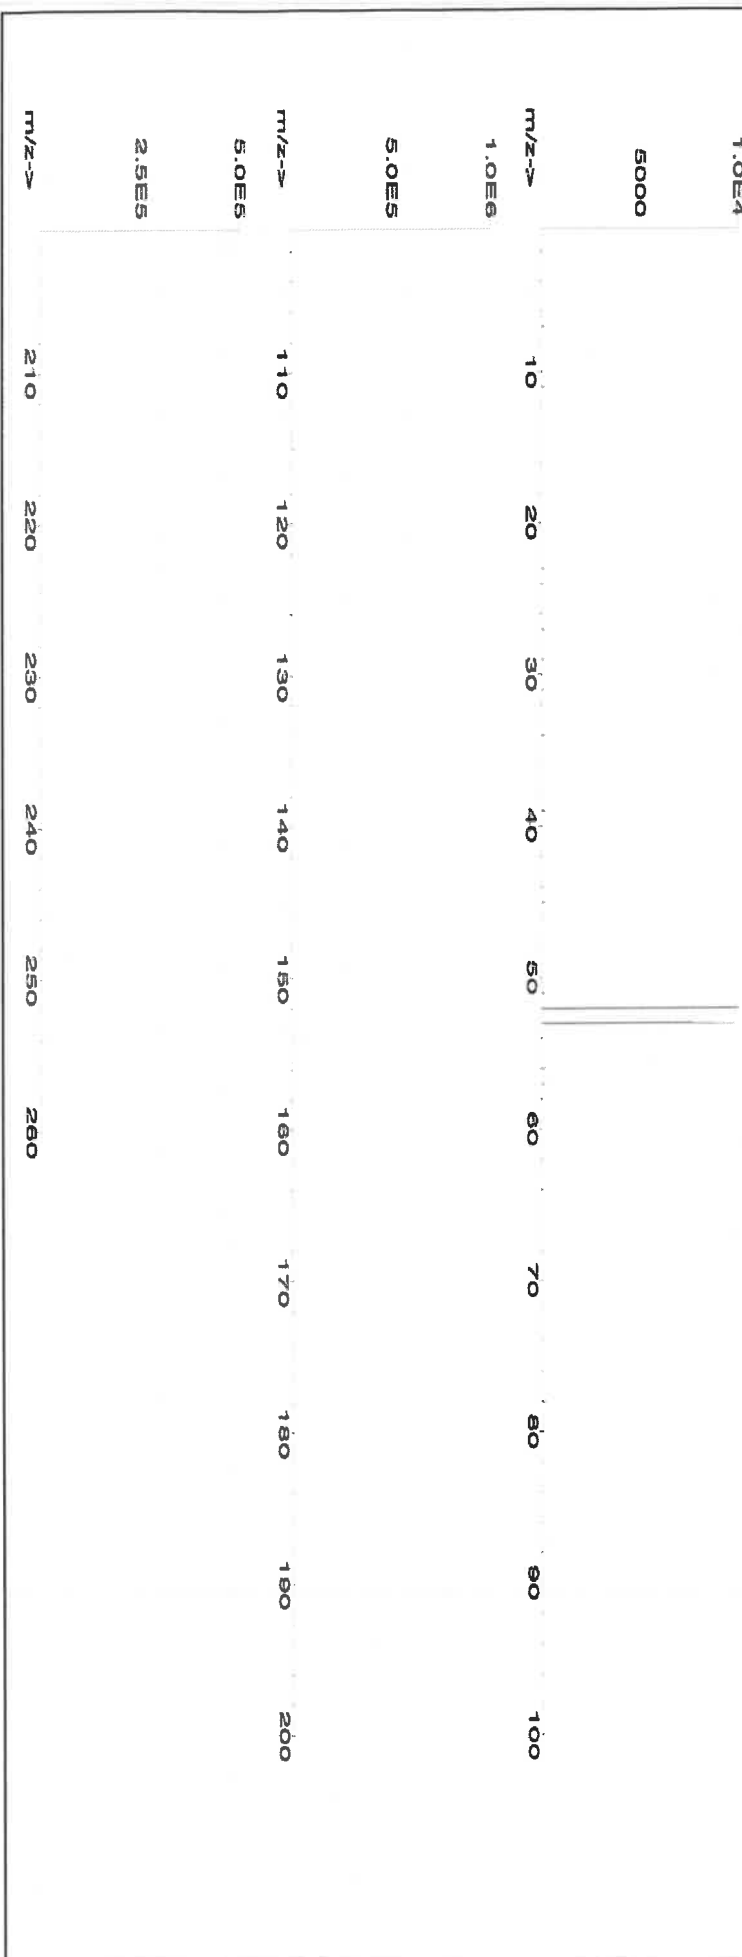



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	T	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58029
Lot Number: 102523
Description: Copper (Cu)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date: 102526
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Volume shown below was diluted to (mL): 2000.02
Balance Uncertainty: 5E-05
Flask Uncertainty: 0.058


Formulated By:	Benson Chan
Reviewed By:	Pedro L. Rentas

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Copper(II) nitrate trihydrate (Cu) 58129 100223 0.1000 200.0 0.084 1000 10000.1 1000.0 2.2 10031-43-3 1 mg/m3 or-rat 794 mg/kg 3114

[1] Spectrum No.1 [33.422 sec]:58029.D# [Count] [Linear]

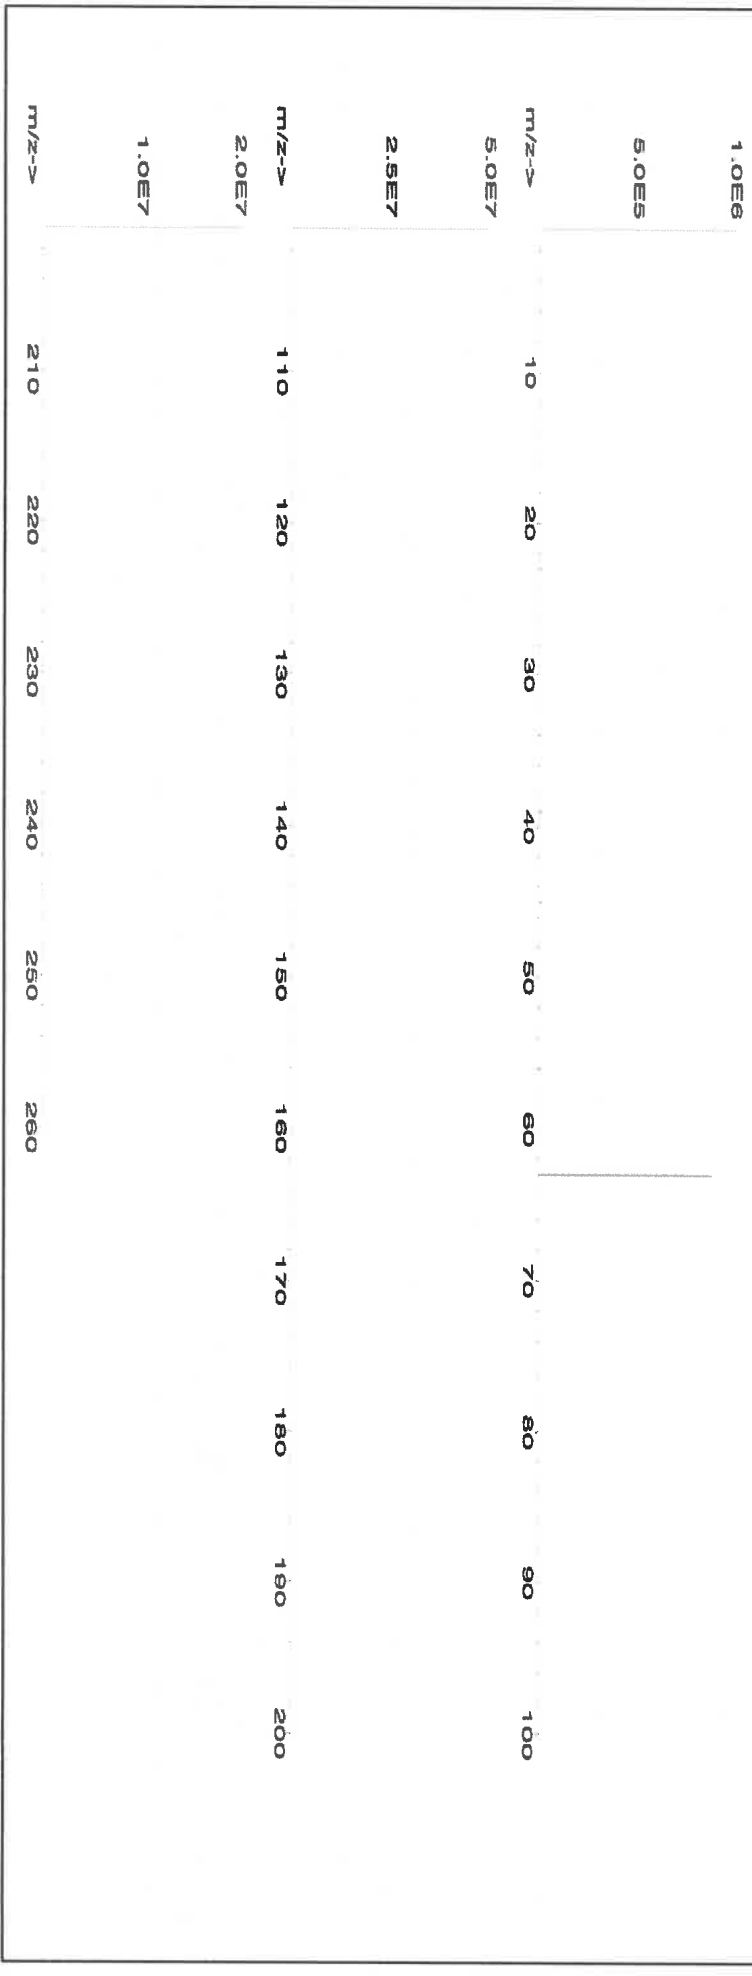



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Trace Metals Verification by ICP-MS (µg/mL)																			
Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Si	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

[Signature]

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
 - * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
 - * All standard containers are meticulously cleaned prior to use.
 - * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
 - * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
 - * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57028
Lot Number: 091223
Description: Nickel (NI)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date: 091226
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6U7B

2.0% 40.0 (mL) Nitric Acid


Volume shown below was diluted to (mL): 2000.02
5E-05 Balance Uncertainty
0.056 Flask Uncertainty

Formulated By:	Lawrence Barry	091223
Reviewed By:	Pedro L. Renteria	091223

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty (mL)	Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	------------------	--------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Nickel(II) nitrate hexahydrate (NI) 58128 062023 0.1000 200.0 0.084 1000 10000.4 1000.0 2.2 13478-00-7 1 mg/m3 or-rel 1620 mg/kg 3136

[1] Spectrum No.1 [9.135 sec]:56026.D# [Count] [Linear]

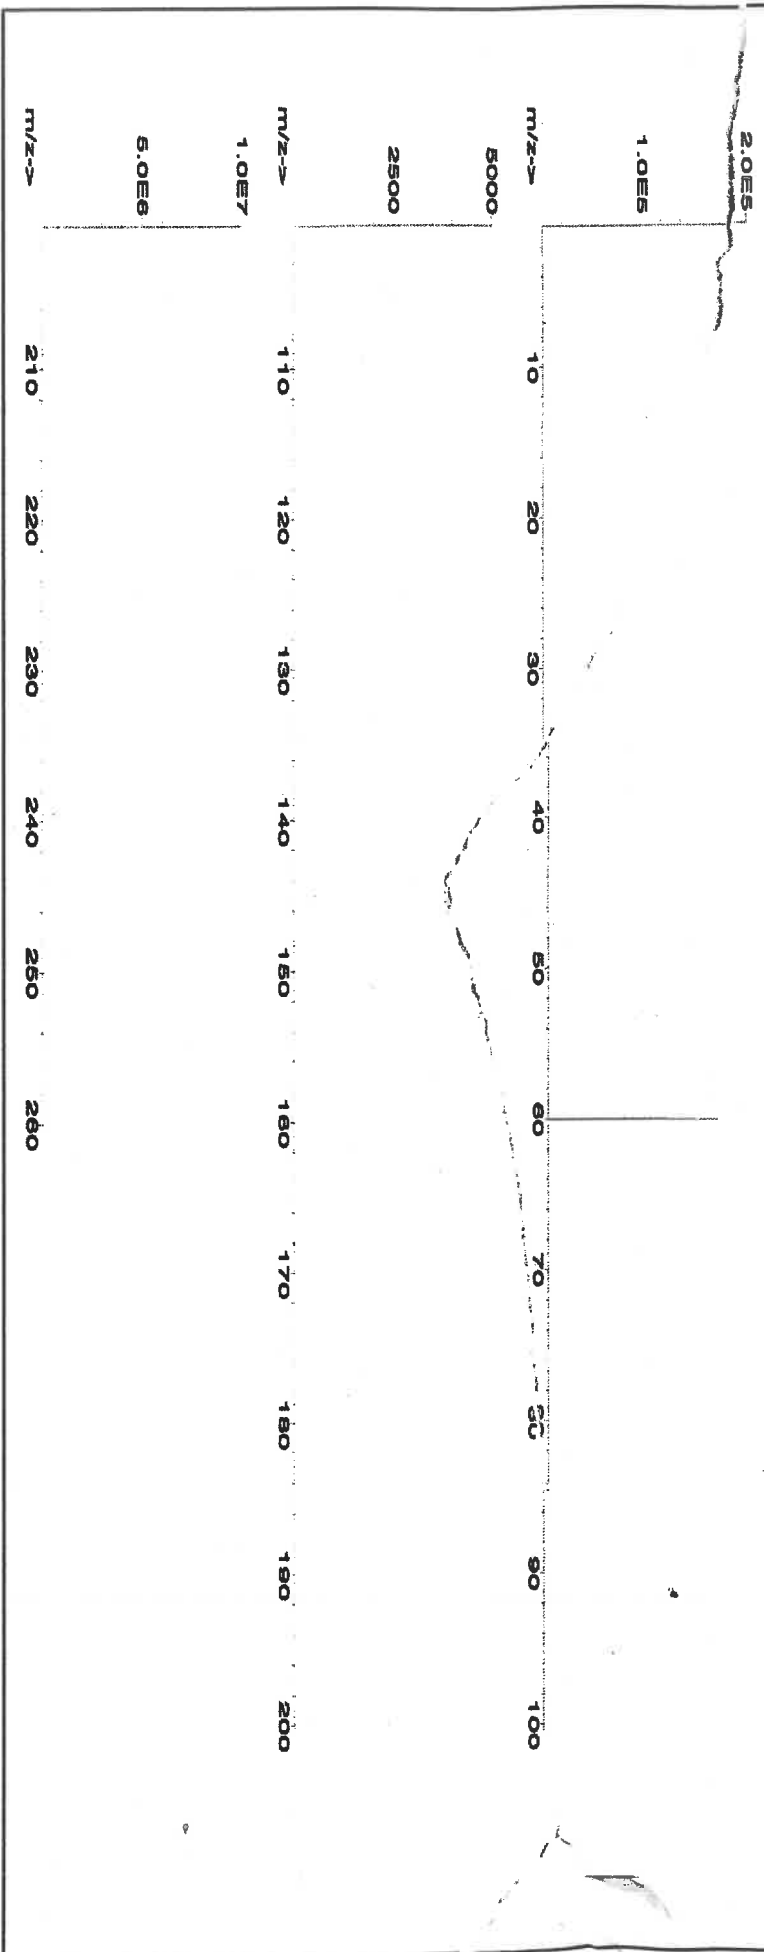



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	T	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Tb	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57004
Lot Number: 102523
Description: Beryllium (Be)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date:

102526

2.0%

40.0 (mL)

Nitric Acid

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

Volume shown below was diluted to (mL): 2000.02


5E-05 Balance Uncertainty
0.058 Flask Uncertainty

Formulated By:	Benson Chan
Reviewed By:	Pedro L. Rentas

SDS Information

Compound	Part Number	Lot	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	-----	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Beryllium nitrate (Be)	58104	091423	0.1000	200.0	0.084	1000	10001.5	1000.0	2.2	13597-99-4	0.2µg/m3	intrinsc-rat 3.16mg/kg	NA
---------------------------	-------	--------	--------	-------	-------	------	---------	--------	-----	------------	----------	------------------------	----

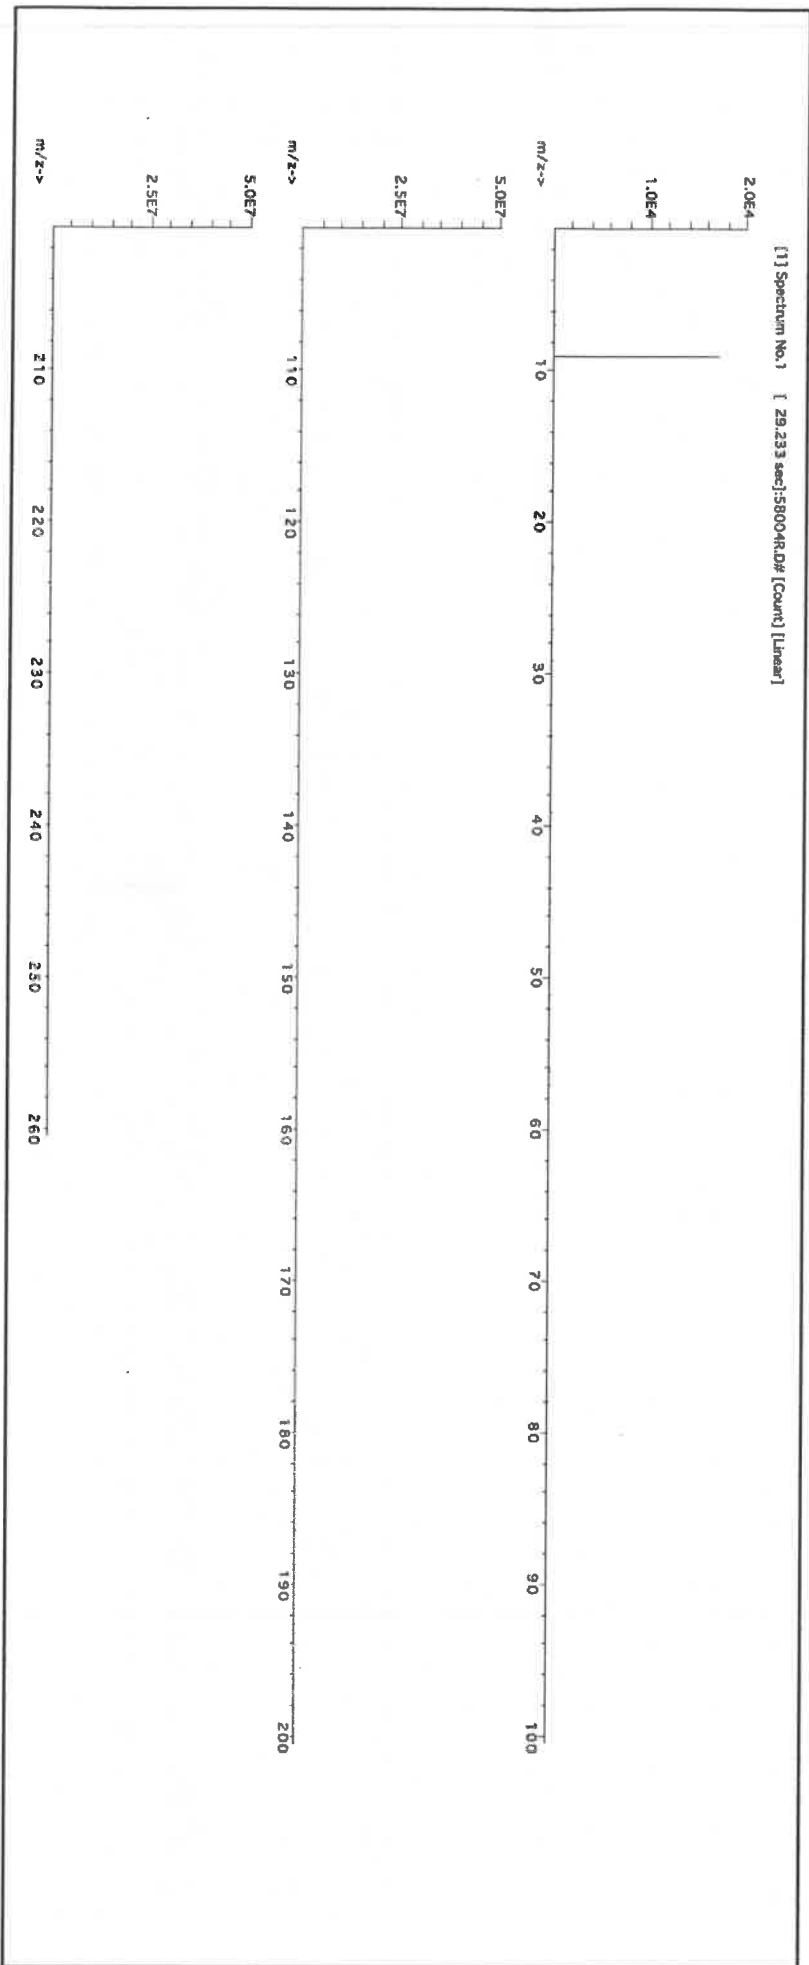



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.02	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Ti	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.02	Th	<0.02	Yb	<0.02
Be	T	Cr	<0.02	Ga	<0.02	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Ta	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.02	Sc	<0.02	Ta	<0.02	Tl	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E. "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

CERTIFIED WEIGHT REPORT:

Part Number: 57050
Lot Number: 071123
Description: Tin (Sn)

Solvents: 21110221 Nitric Acid
22D0562008 Hydrochloric acid

Expiration Date: 071126
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000

2% 10.0 Nitric Acid
6% 30.0 Hydrochloric acid
(mL)

NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 499.93


5E-05 Balance Uncertainty
0.0058 Flask Uncertainty

<i>[Signature]</i>	
Formulated By:	Benson Chan
	071123
Reviewed By:	Pedro L. Rientas
	071123

SDS Information															NIST
Solvent Safety Info. On Attached pg.)															
Compound	Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Expanded						
										RM#	Number	Conc. (µg/mL)	(%)	Purity (%)	

1. Ammonium hexafluoroantimonate(V) (Sn) IN010 SMD042023A1 1000 99.999 0.10 44.2 1.13107 1.13286 1001.6 2.0 16919-24-7 7 mg/m3 NA 3161a

[1] Spectrum No. 1 [15.034 sec]:56150.D# [Count] [Linear]

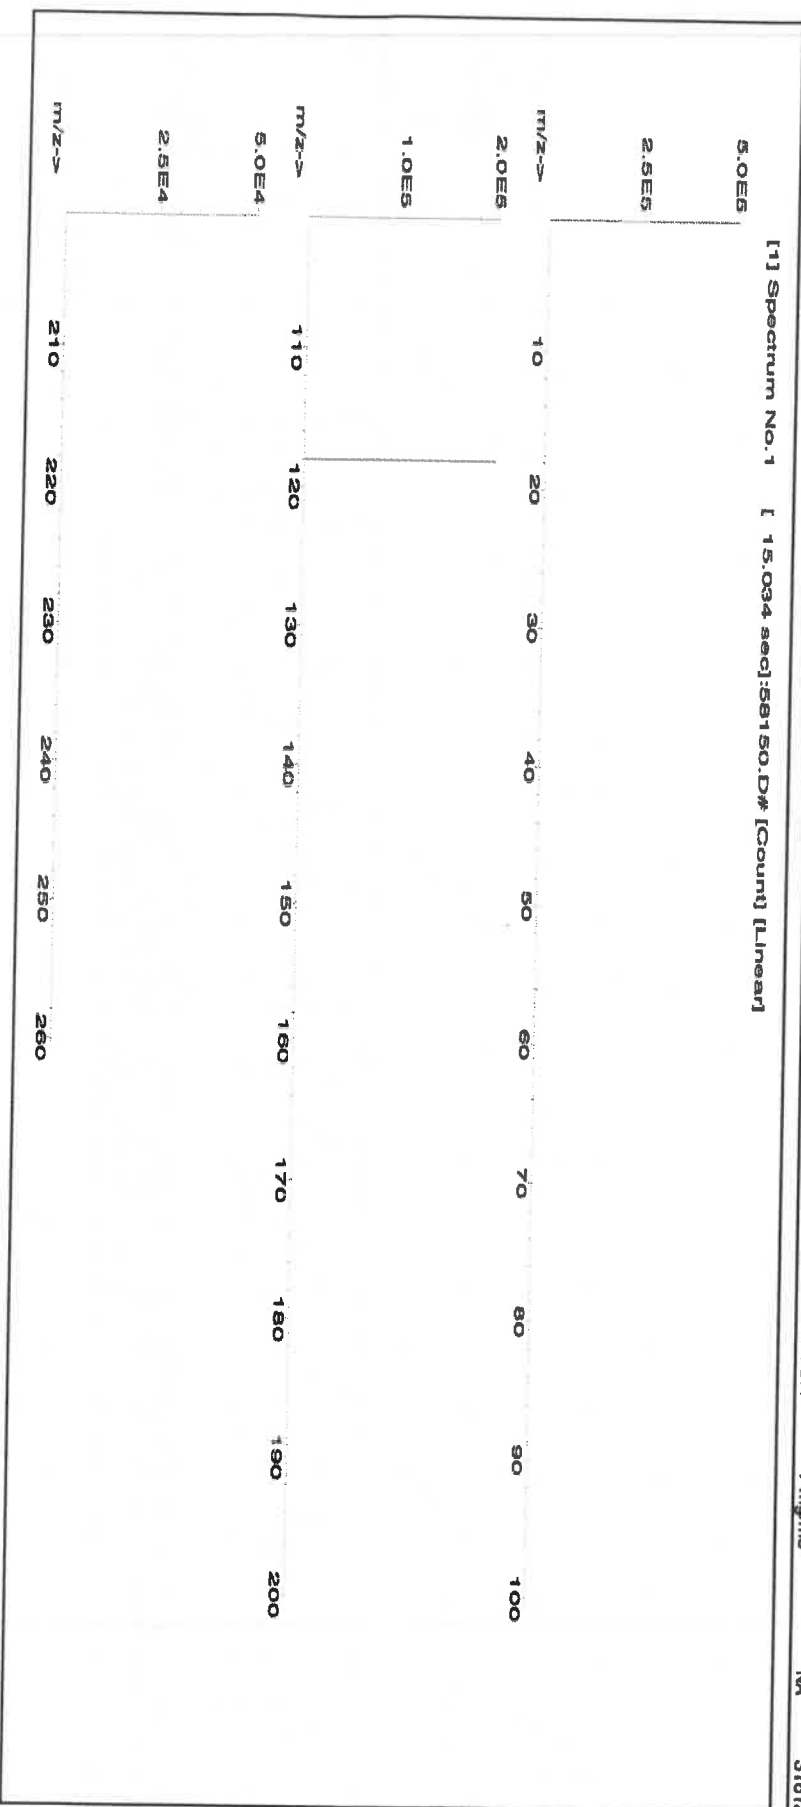



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<500	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Ta	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R: 02/09/24 115800 (54)

CERTIFIED WEIGHT REPORT:

Part Number: 57027
Lot Number: 091923
Description: Cobalt (Co)

Expiration Date: 091926
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Volume shown below was diluted to (mL): 2000.02

Lot # 24002546
Solvent: Nitric Acid


Formulated By:	Lawrence Barry	091923
Reviewed By:	Pedro L. Rentas	091923

SDS Information

Expanded Uncertainty +/- (µg/mL)
(Solvent Safety Info. On Attached pg.)
NIST SRM
CAS# OSHA PEL (TWA) LD50

1. Cobalt(II) nitrate hexahydrate (Co) 58127 050923 0.1000 200.0 0.084 1000 10000.0 1000.0 2.2 10026-22-9 0.02 mg/m3 orl-rat 691 mg/kg 3113

[1] Spectrum No.1 [34.243 sec]:58027.D# [Count] [Linear]

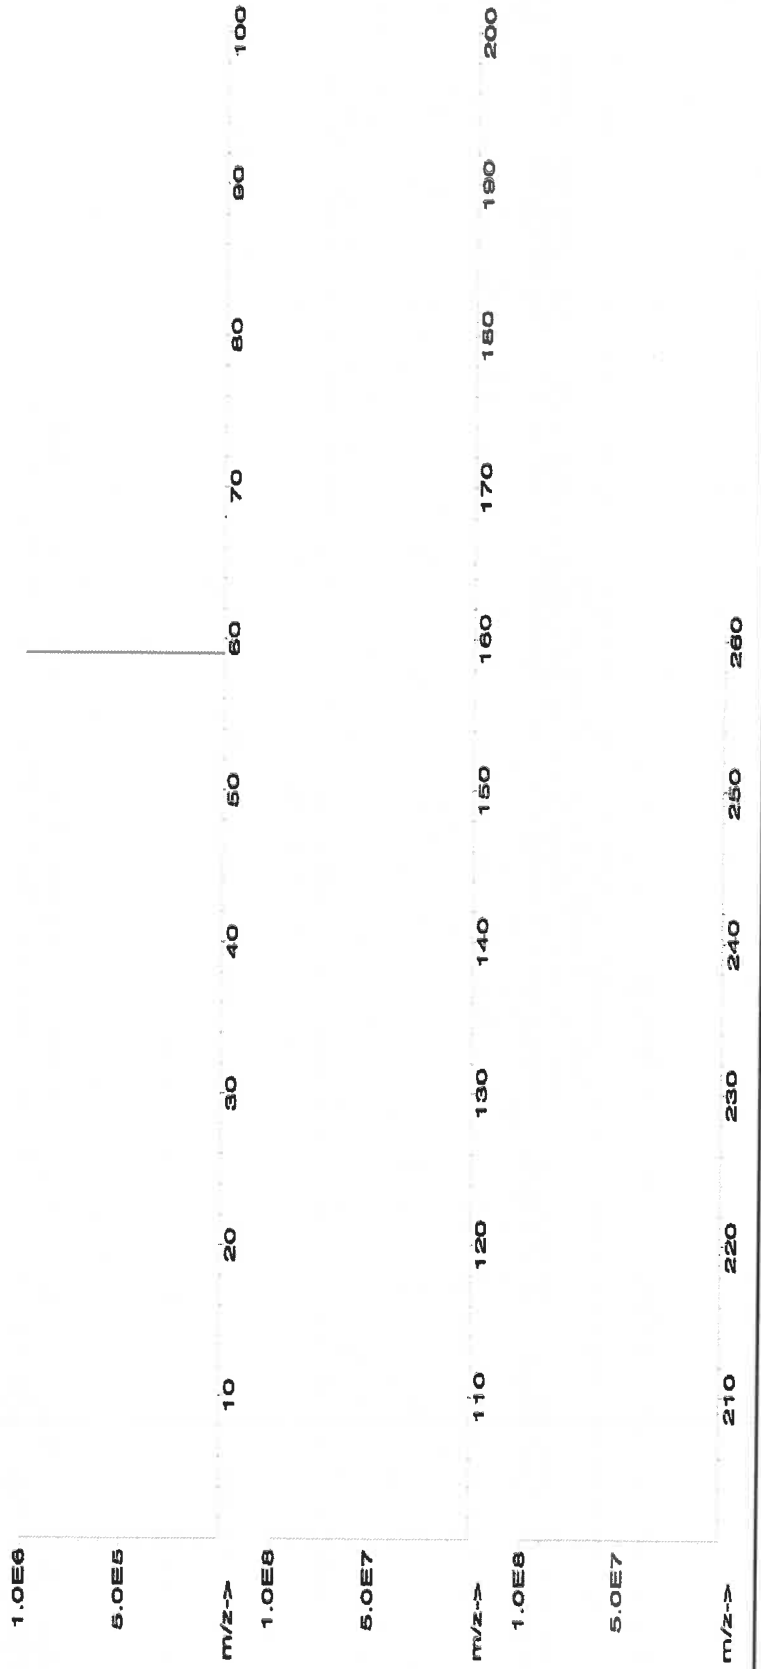



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS ($\mu\text{g/mL}$)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.02	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Gé	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.2	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

Ben. H. R.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

AR: 02/09/24

M5801

BA



CERTIFIED WEIGHT REPORT:

Part Number: 57033
Lot Number: 111323
Description: Arsenic (As)

Lot # 24002546
Solvent: Nitric Acid

Expiration Date: 111326

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL): 1000

NIST Test Number: 6LUTB

Volume shown below was diluted to (mL): 4000.0

Balance Uncertainty: 5E-05
Flask Uncertainty: 0.06

2.0%

80.0 (mL)


Nitric Acid

Formulated By:	Lawrence Barry	111323
Reviewed By:	Pedro L. Rendas	111323

SDS Information									
Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)
1. Arsenic (As)	58133	020522	0.1000	400.0	0.084	1000	10001.0	1000.0	2.0

(Solvent Safety Info. On Attached pg.) CAS# OSHA PEL (TWA) LD50 NIST SRM

[1] Spectrum No. 1 [34.433 sec]:57033.D# [Count] [Linear]

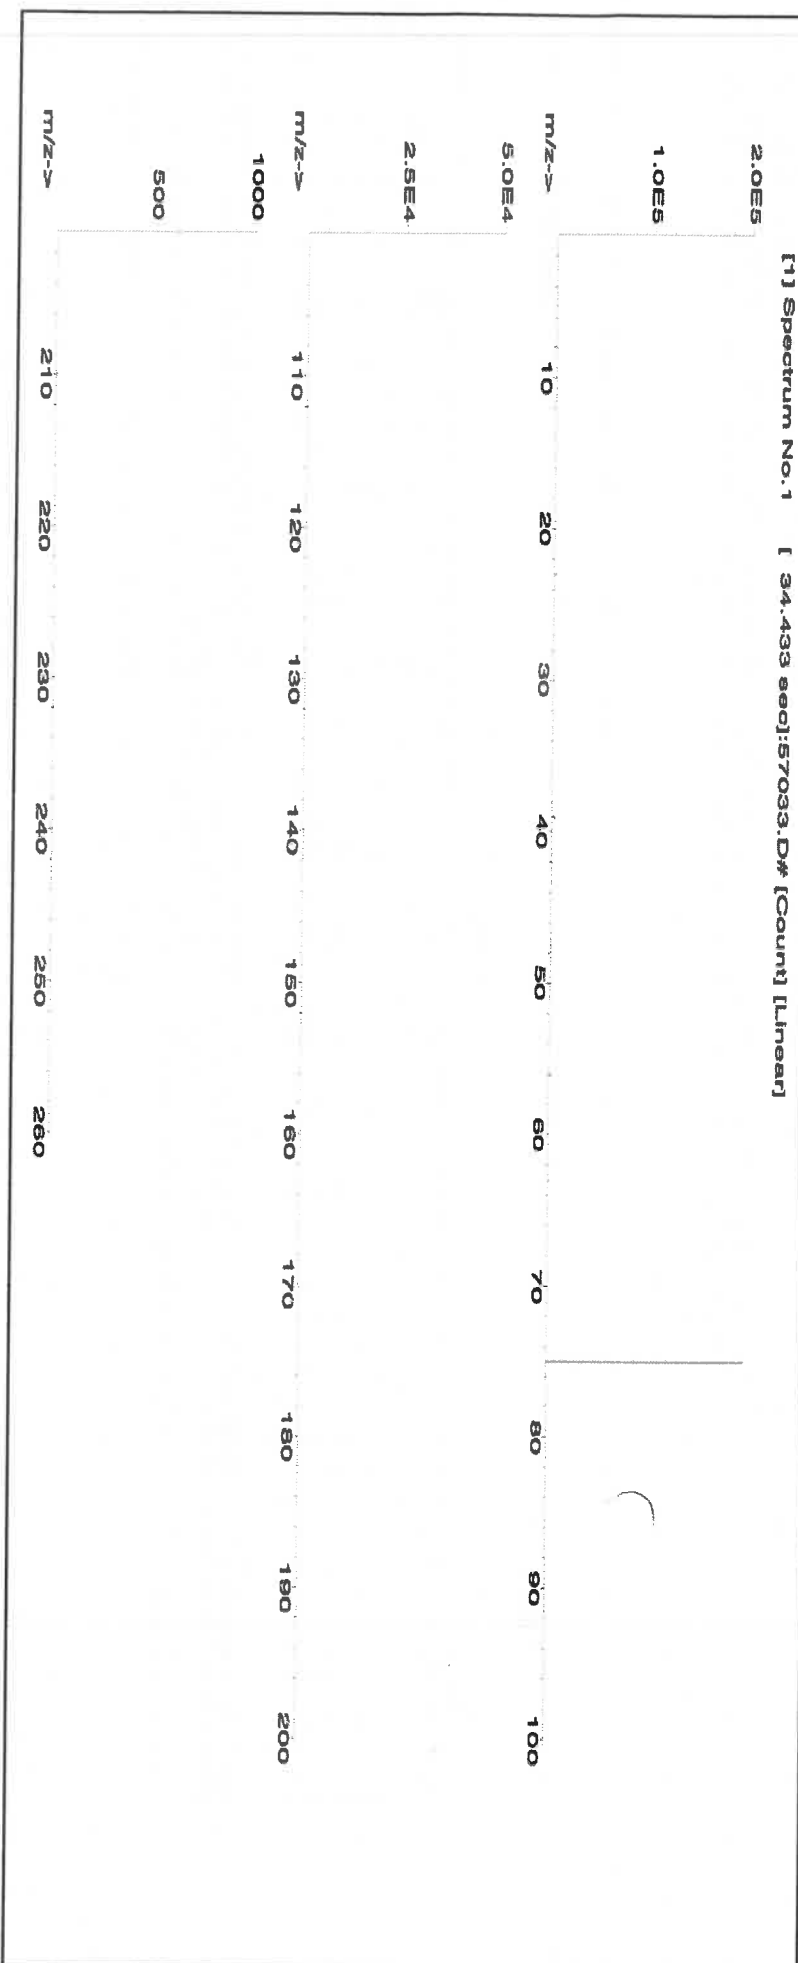



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	T	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Tl _h	<0.02	Yb	<0.02
Bc	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	S	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge [*]	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	Ta	<0.02	Sa	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02			Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: **57005**
Lot Number: **071123**
Description: **Boron (B)**

Solvent: MKB0857V Ammonium hydroxide

Lot #

AI: 021009124 M5814

Expiration Date: 071126
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB

2.0% 40.0 Ammonium hydroxide (mL)


Weight shown below was diluted to (mL): 1999.48 0.058 Balance Uncertainty Flask Uncertainty

Formulated By:	Benson Chan
071123	
Reviewed By:	Pedro L. Rientas
071123	

SDS Information

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-----	------------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Boric acid (B) IN018 BV082018A1 1000 99.999 0.10 17.3 11.55772 11.56201 1000.4 2.0 10043-35-3 2 mg/m3 or-nat 2660 mg/kg 3107

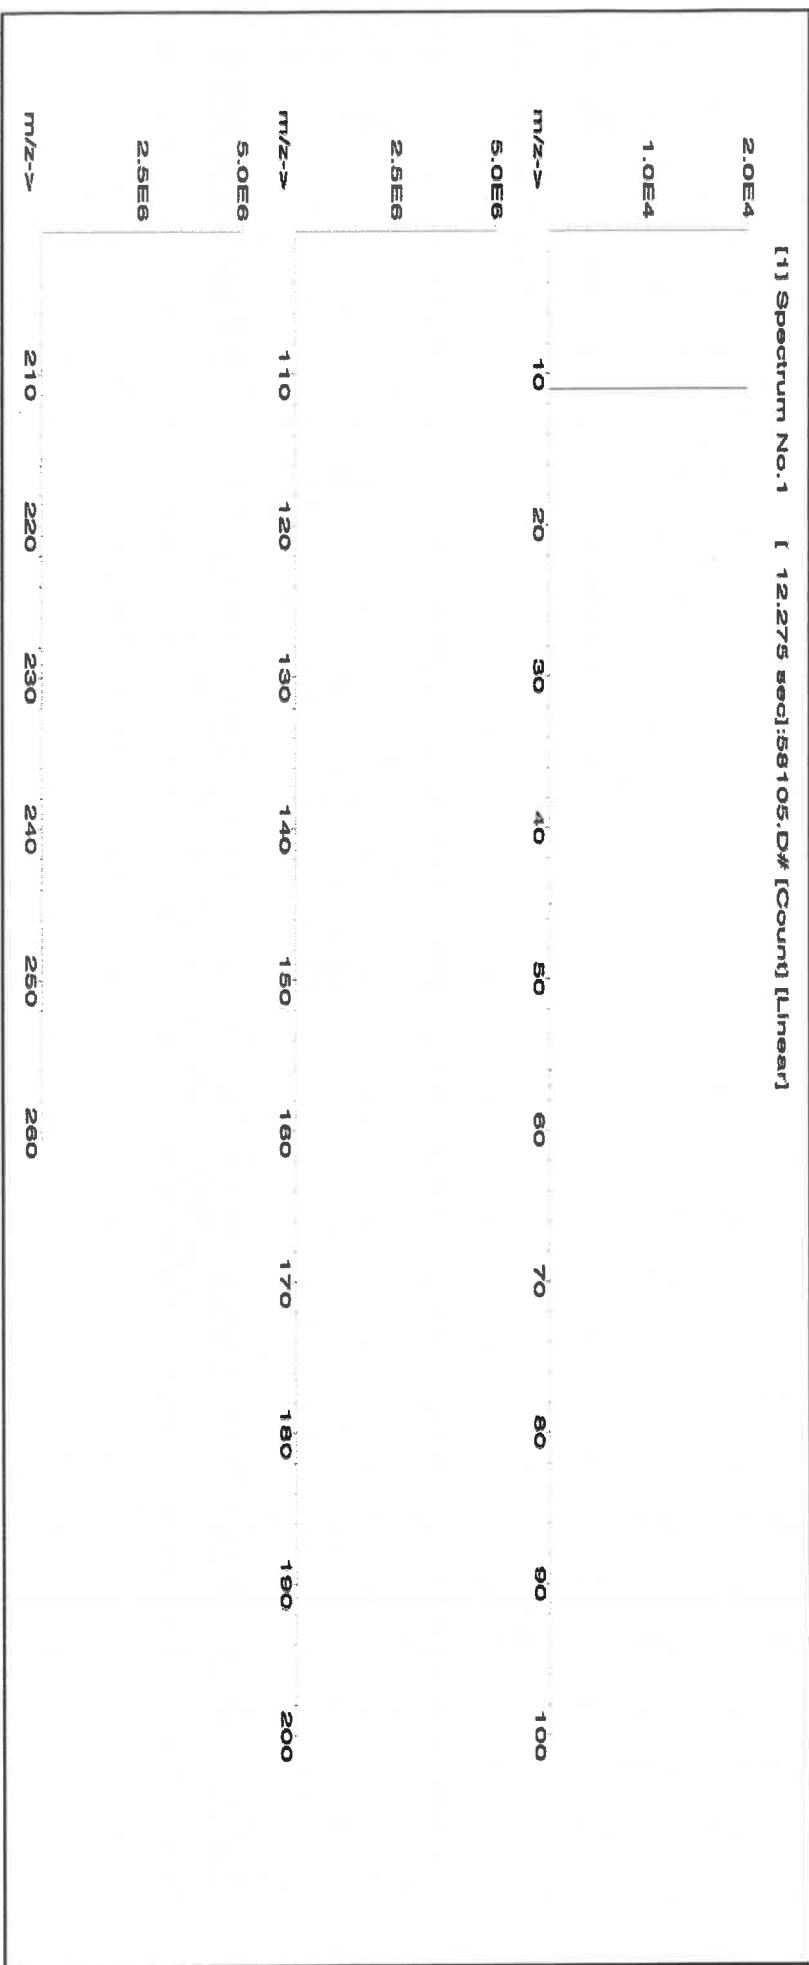



Instrumental Analysis by Inductively Coupled Plasma Mass Spectroscopy (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	T	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 57016
Lot Number: 122923
Description: Sulfur (S)


Solvent: 122923
ASTM Type 1 Water

Formulated By:	Benson Chan
122923	
Reviewed By:	Pedro L. Rentas
122923	

Expiration Date: 122926
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6L7B
Weight shown below was diluted to (mL): 4000.0
SE-05 Balance Uncertainty
0.06 Flask Uncertainty

SDS Information																
Expanded (Solvent Safety Info. On Attached pg.)																
Compound	RM#	Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Expanded	CAS#	OSHA PEL (TWA)	LD50	NIST	SRM	
		Number	Conc. (µg/mL)	(%)	Purity (%)	(%)	Weight (g)	Weight (g)	Conc. (µg/mL)	+/- (µg/mL)						

1. Ammonium sulfate (S) IN117 SLBR225V 1000 99.9 0.10 24.3 16.4979 16.4980 1000.0 2.0 7783-20-2 NA or-rel 4250mg/kg 3181

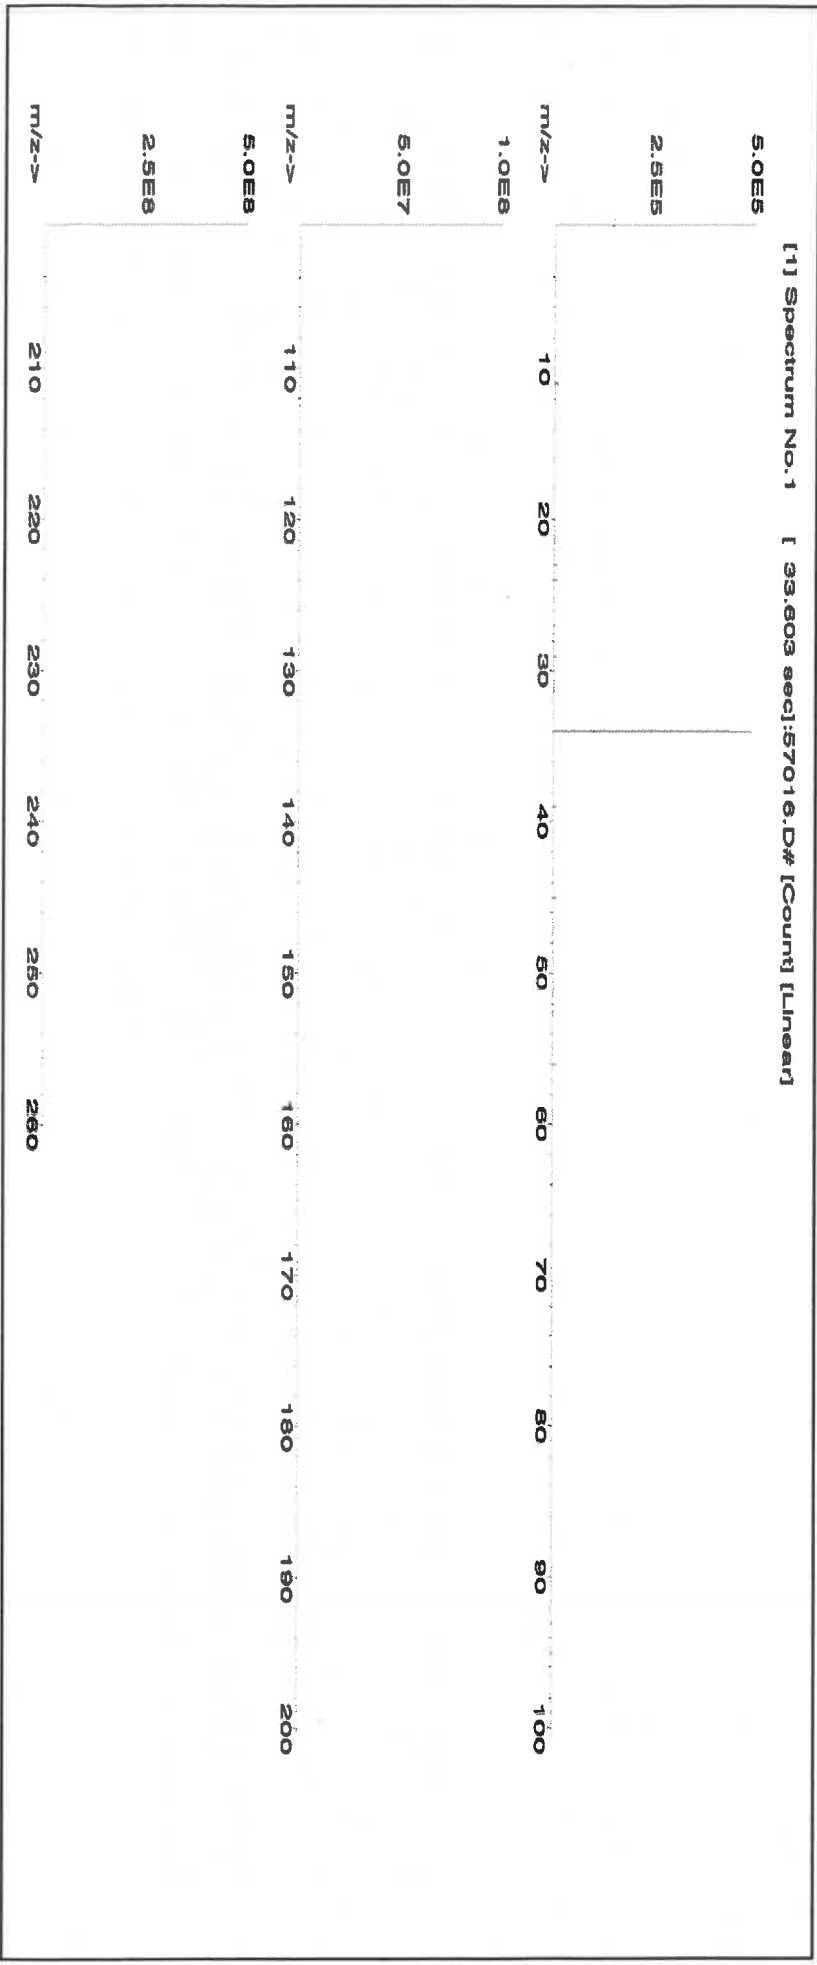



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	La	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Ba	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	S	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	Ta	<0.02	Ti	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Certified by:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number: 57015
Lot Number: 091123
Description: Phosphorous (P)

Solvent: 24002546 Nitric Acid

Lot #

Formulated By: Lawrence Barry
Reviewed By: Pedro L. Rentas

091123

2% 40.0 (mL) Nitric Acid


Expiration Date: 091126
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6LUTB
Weight shown below was diluted to (mL): 2000.02
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

SDS Information

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-----	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Ammonium dihydrogen phosphate (P) IN008 PVO62019A1 1000 99.999 0.10 27.5 7.2729 7.2730 1000.0 2.0 7722-76-1 5 mg/m3 xH-rat >2000mg/kg 3186

[1] Spectrum No.1 [12.074 sec]:58115.D# [Count] [Linear]

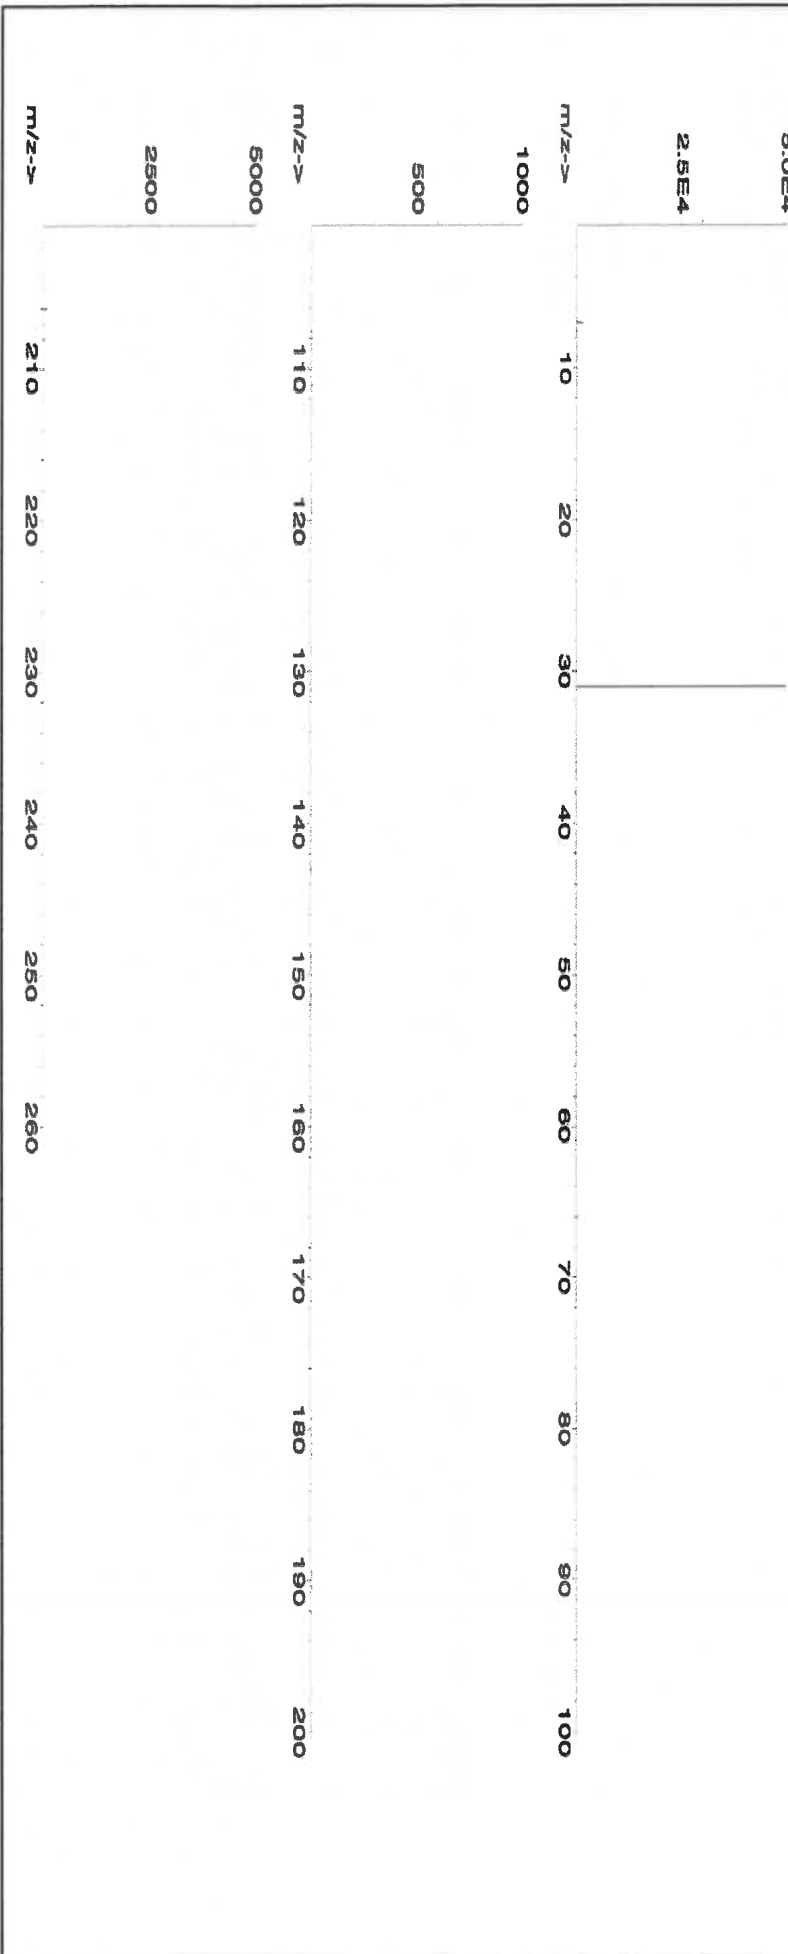



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	T	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sa	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Absolute Standards, Inc.

800-368-1131
www.absolutestandards.com



Certified Reference Material CRM



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
<https://AbsoluteStandards.com>

CERTIFIED WEIGHT REPORT:

Part Number:

57034

Lot Number:

060624

Description:

Selenium (Se)

Lot # Solvent:

24002546

Nitric Acid

2.0%

40.0 (mL)

Nitric Acid

Formulated By:

Benson Chan

060624

Expiration Date:

060627

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

Volume shown below was diluted to (mL):

2000.07

SE-05 Balance Uncertainty
0.100 Flask Uncertainty

Reviewed By:

Pedro L. Rantas


060624

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	(Solvent Safety Info. On Attached pg.)	CAS#	OSHA PEL (TWA)	LDSO	NIST SRM
----------	-------------	------------	-----------------	-------------------	--------------	-----------------------	-----------------------	---------------------	----------------------------------	--	------	----------------	------	----------

1. Selenium (Se)	58134	071223	0.1000	200.0	0.084	1000	10002.5	1000.0	2.2	7782-49-2	0.2 mg/m3	or-tral 6700 mg/kg	3149
------------------	-------	--------	--------	-------	-------	------	---------	--------	-----	-----------	-----------	--------------------	------

[1] Spectrum No. 1 [33.702 sec]:58034.D# [Count] [Linear]

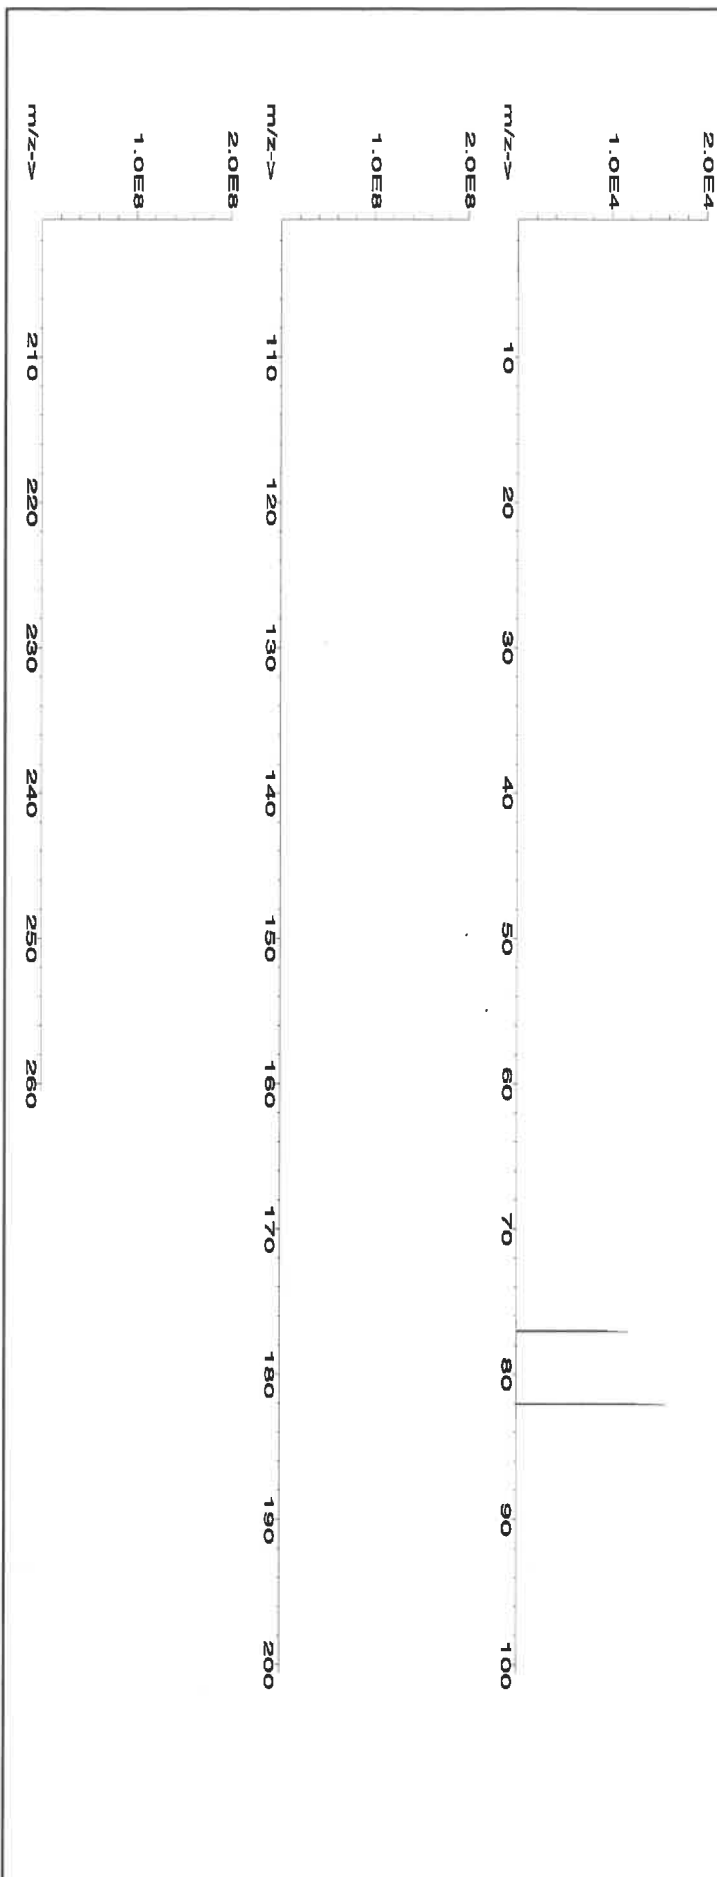

Absolute Standards, Inc.
800-368-1131
www.absolutestandards.com



Certified Reference Material CRM



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
<https://AbsoluteStandards.com>

Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	T	Tb	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Th	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	S	<0.02	Tm	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	Ta	<0.02	Sn	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02		<0.02	Ti	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
https://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT:

Part Number: **57016**
Lot Number: **122923**
Description: **Sulfur (S)**


Lot #
Solvent: **122923** ASTM Type 1 Water

Formulated By:	Benson Chan
122923	
Reviewed By:	Pedro L. Rentas
122923	

Expiration Date: **122926**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test Number: **6UTB**
Weight shown below was diluted to (mL): **4000.0** **5E-05** Balance Uncertainty
0.06 Flask Uncertainty

Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty			NIST SRM
									SDS information			
									(Solvent Safety Info. On Attached pg.)			
RM#									± (µg/mL)	CAS#	OSHA PEL (TWA)	LD50

1. Ammonium sulfate (S) IN117 SLBR725V 1000 99.9 0.10 24.3 16.4979 16.4980 1000.0 2.0 7783-20-2 NA or-rel 4250mg/kg 3181

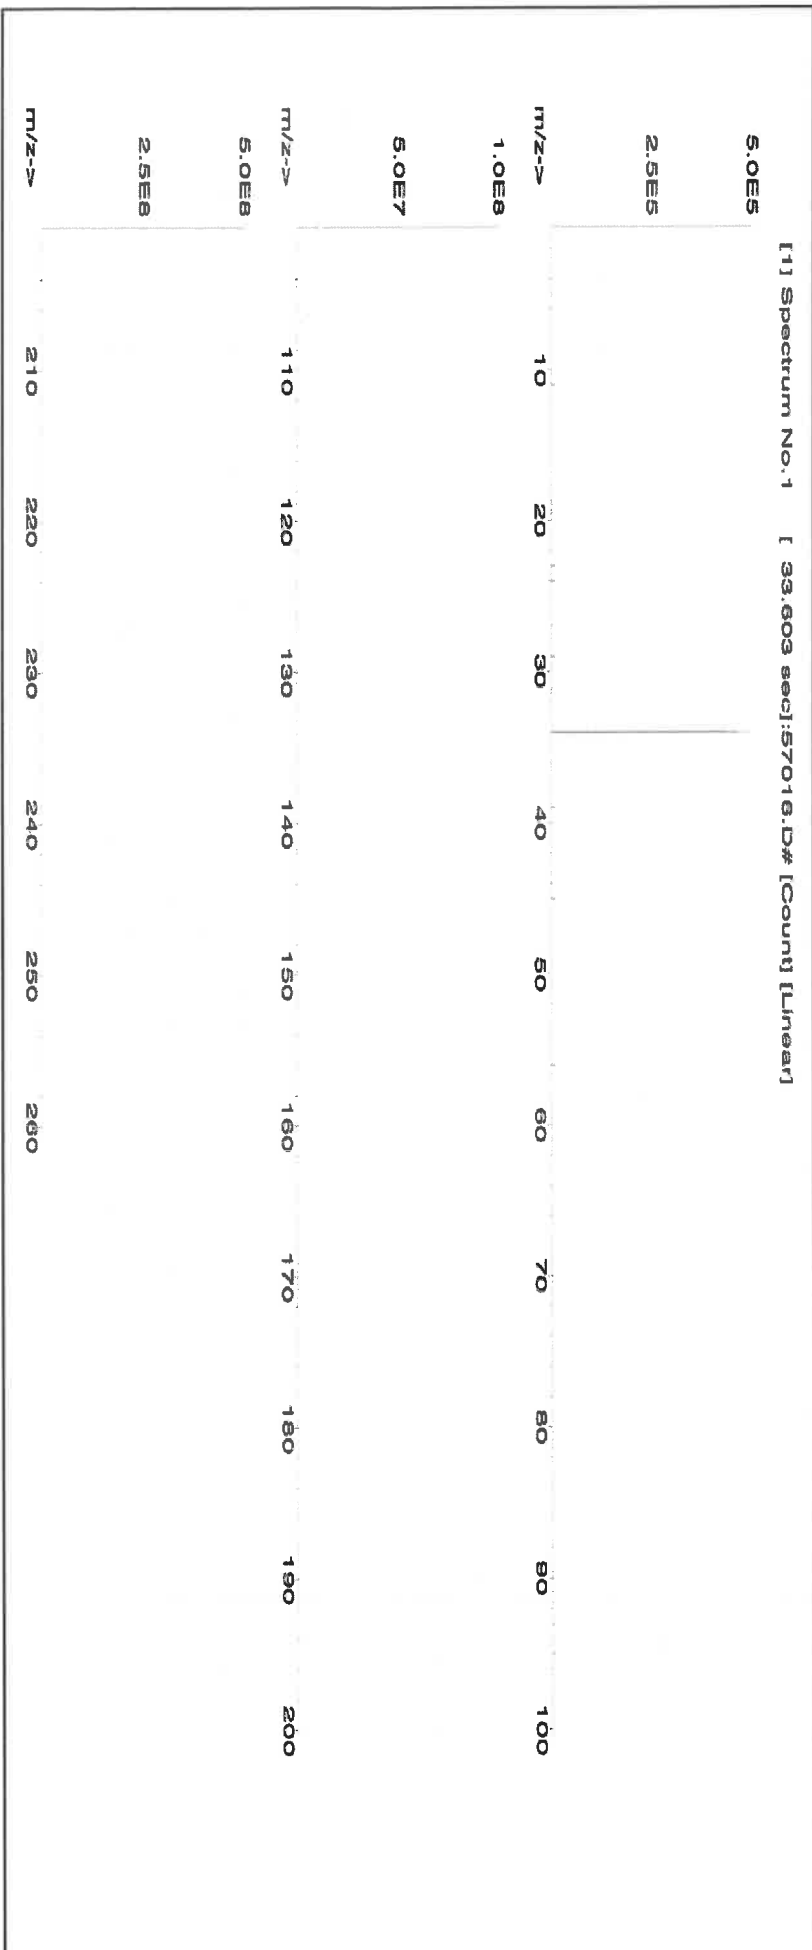

Absolute Standards, Inc.
800-368-1131
www.absolute-standards.com



Certified Reference Material CRM
M5970 M5971 R1 710124



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
https://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT:


Part Number: 57003
Lot Number: 062124
Description: Lithium (Li)
Expiration Date: 06/21/27
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Volume shown below was diluted to (mL): 250.11

Lot # 24002546
Solvent: Nitric Acid
Balance Uncertainty: SE-05
Flask Uncertainty: 0.016
Conc. (µg/mL): 2.0%
Initial Conc. (µg/mL): 5.0 (mL)
Final Conc. (µg/mL): Nitric Acid

Microvite Capable	
Formulated By:	062124
Reviewed By: <i>[Signature]</i>	
Petro L. Parias	

Compound		SDS Information												Expanded (Solvent Safety Info. On Attachment pg.)		CAS# OSHA PEL (TWA) LD50		NEST SM																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																				
		Part	Lot	Dilution	Initial	Uncertainty	Nominal	Initial	Final	Uncertainty	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)							Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																																
Number	Factor	Number	Factor	Vol. (mL)	Pipette (mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg/mL)	Conc. (µg

1. Lithium nitrate (Li) 58103 070622 0.1000 25.0 0.004 1000 10000.4 1000.0 2.0 7790-68-4 5 mg/m3 or-hal 1428 mg/kg NA

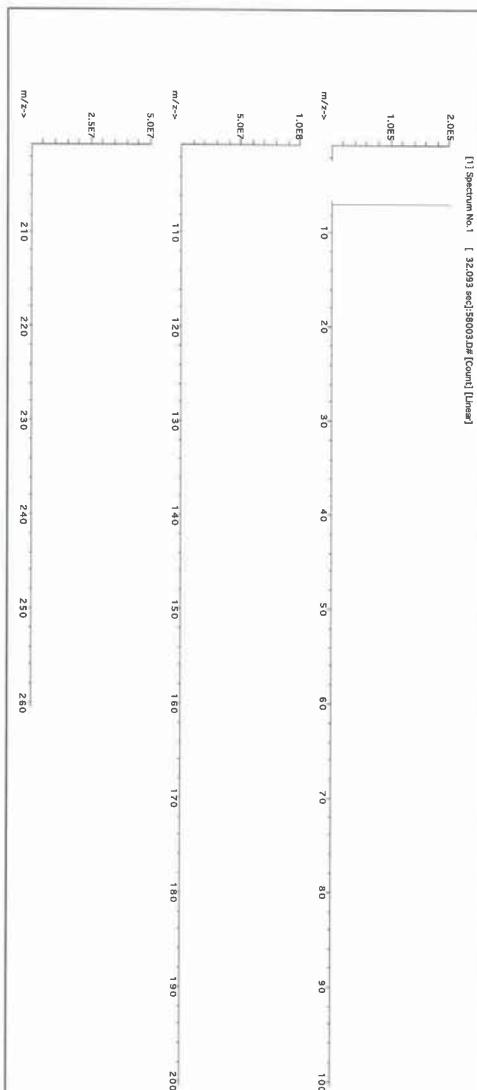

Part # 57003 Lot # 062124

1 of 2

Printed: 6/24/2024, 11:20:08 PM



Redefine your results. Redefine your industry.

Certificate of Analysis

M5978, M5979

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com



INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).

1.0 ACCREDITATION / REGISTRATION

2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution

Catalog Number: CGT1

Lot Number: T2-T1719972

Matrix: 2% (v/v) HNO₃

Value / Analyte(s): tr. HF

Starting Material: 1 000 µg/mL ea.

Starting Material: Titanium

Starting Material: Ti Metal

Starting Material Lot#: 2094

Starting Material Purity: 99.9975%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 1002 ± 5 µg/mL

Density: 1.012 g/mL (measured at 20 ± 4 °C)

Assay Method #1

1002 ± 4 µg/mL

ICP Assay NIST SRM 3162a Lot Number: 130925

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$X_{CRM/RM} = (k_p / v_{char,p})$

k_p = mean of Assay Method A with

$v_{char,p}$ = the standard uncertainty of characterization Method A

k = coverage factor = 2

$v_{char,p} = [(2/v_p)^2 (v_{CRM/RM})^2 + v_{char,p}^2 + v_{rep}^2 + v_{lab}^2 + v_{stb}^2]^{1/2}$

$v_{char,p}$ = the mean of Assay Method A with

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

$v_{char,p}$ = the standard uncertainty of characterization Method A

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0

TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an UHPA-filtered Clean Room. An UHPA-filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000536	M	Eu	<	0.000268	O	Na	<	0.032670	M	Se	<	0.001204	O	Zn	<	0.003267
M	Al	<	0.000872	O	Fe	<	0.003225	O	Nb	<	0.043560	O	Si	<	0.004735	O	Zr	<	0.043560
M	As	<	0.008586	M	Ga	<	0.000268	M	Nd	<	0.000268	M	Sm	<	0.000268				
M	Au	<	0.004577	M	Gd	<	0.000268	O	Ni	<	0.010890	M	Sn	<	0.000986				
O	B	<	0.008929	M	Ge	<	0.002146	M	Os	<	0.000269	O	Sr	<	0.000986				
M	Ba	<	0.002683	M	Hf	<	0.002161	O	P	<	0.054450	M	Ta	<	0.010560				
M	Be	<	0.005366	M	Hg	<	0.003231	M	Pb	<	0.001073	M	Tb	<	0.000268				
M	Bi	<	0.001609	M	Ho	<	0.000268	M	Pd	<	0.000268	M	Te	<	0.001341				
O	Ca	<	0.000676	M	In	<	0.002683	M	Pr	<	0.000268	M	Th	<	0.053663				
M	Cd	<	0.000268	M	Ir	<	0.000269	M	Pt	<	0.000536	s	Ti	<	<				
M	Ce	<	0.000268	M	K	<	0.001172	M	Rb	<	0.000268	M	Tl	<	0.000268				
M	Co	<	0.004293	M	La	<	0.000268	M	Rc	<	0.000268	M	Tm	<	0.000268				
M	Cr	<	0.000752	O	Li	<	0.027225	M	Rh	<	0.000268	M	U	<	0.000268				
M	Cs	<	0.000268	M	Lu	<	0.000268	M	Ru	<	0.000269	M	V	<	0.019855				
O	Cu	<	0.010890	O	Mg	<	0.005445	I	S	<	0.006976	M	W	<	0.000473				
M	Dy	<	0.000268	O	Mn	<	0.003267	M	Sb	<	0.006976	M	Y	<	0.002146				
M	Er	<	0.000268	M	Mo	<	0.000774	O	Sc	<	0.004900	M	Yb	<	0.000536				

6.0 INTENDED USE

- For the calibration of analytical instruments and validation of analytical methods as appropriate.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence: Soluble in concentrated HCl, HF, H3PO4 H2SO4 and HNO3. Avoid neutral to basic media. Unstable at ppm levels with metals that would pull F- away (i.e. Do not mix with Alkaline or Rare Earths or high levels of transition elements unless they are fluorinated). Stable with most inorganic anions with a tendency to hydrolyze forming the hydrated oxide in all dilute acids except HF.

Stability: - 2-100 ppb levels stable (Alone or mixed with all other metals) as the Ti(F)-6-2 for months in 1% HNO3 / LDPE container. - 1-10,000 ppm single element solutions as the Ti(F)-6-2 chemically stable for years in 2-5% HNO3 / trace HF in an LDPE container.

Ti Containing Samples (Preparation and Solution) - Metal (Soluble in H2O / HF caution - powder reacts violently): Oxide - low temperature history anatase or rutile (Dissolved by heating in 1:1:1 H2O / HF / H2SO4); K2S2O7 - no KF if silica not present); Organic Matrices (Dry ash at 450EC in P10 and dissolve by heating with 1:1:1 H2O / HF / H2SO4 or fuse ash with pyrosulfate if oxide is as plastic pigment and likely in brookite crystaline form).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 48 amu	14 ppt	N/A	32S16O, 32S14N,
ICP-OES 323.452 nm	0.0054 / 0.00092 µg/mL	1	14N17N2, 36Ar12C,
ICP-OES 334.941 nm	0.0038 / 0.00028 µg/mL	1	48Ca, 196X=2
ICP-OES 336.121 nm	0.0053 / 0.00034 µg/mL	1	(where X = Zr, Mo, W, Mo, Co Nb, Ta, Cr, U Ce, Ar, Ni Ru))

HAZARDOUS INFORMATION

HF Note: This standard should not be prepared or stored in glass.

HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

Reference Material Producer - Accredited / AZLA Certificate Number 883.02
Inorganic Ventures, 300 Technology Drive, Chesapeake, VA 24073, USA; Telephone: 800.868.6786; 540.565.3030; Fax: 540.565.3012; info@inorganicventures.com

11.0

CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

June 17, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- June 17, 2027

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0

NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozlikowski
Manager, Quality Control

TD978L

Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director

Paul R. Gaines

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

M5985
R: 6/14/24

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGIN10
Lot Number: U2-IN729349
Matrix: 5% (v/v) HNO₃
Value / Analyte(s): 10 000 µg/mL ea:
Indium
Starting Material: Indium Metal
Starting Material Lot#: 2511
Starting Material Purity: 99.9995%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 10022 ± 30 µg/mL
Density: 1.044 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1	10021 ± 56 µg/mL ICP Assay NIST SRM 3124a Lot Number: 110516
Assay Method #2	10035 ± 25 µg/mL EDTA NIST SRM 928 Lot Number: 928
Assay Method #3	10001 ± 33 µg/mL Calculated NIST SRM Lot Number: See Sec. 4.2

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum(1/u_{char j}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k(u_{char}^2 + u_{bb}^2 + u_{ts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum(w_i)^2(u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{ts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a)(u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (k) = U_{CRM/RM} = k(u_{char a}^2 + u_{bb}^2 + u_{ts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{ts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000760	M	Eu	<	0.000760	O	Na	0.012771	M	Se	<	0.023000	M	Zn	<	0.006100
M	Al	0.003385	O	Fe	0.004462	M	Nb	<	0.000760	O	Si	0.024619	M	Zr	<	0.000760		
M	As	<	0.004600	M	Ga	<	0.000760	M	Nd	<	0.000760	M	Sm	<	0.000760			
M	Au	<	0.002300	M	Gd	<	0.000760	O	Ni	<	0.005100	M	Sn	<	0.000760			
O	B	0.003692	M	Ge	<	0.001600	M	Os	<	0.000760	O	Sr	<	0.000610				
M	Ba	<	0.001600	M	Hf	<	0.000760	n	P	<		M	Ta	<	0.000760			
O	Be	<	0.000130	M	Hg	<	0.003100	M	Pb	0.001400	M	Tb	<	0.000760				
M	Bi	<	0.000760	M	Ho	<	0.000760	M	Pd	<	0.001600	M	Te	<	0.000760			
O	Ca	0.004616	s	In	<			M	Pr	<	0.000760	M	Th	<	0.000760			
M	Cd	<	0.000760	M	Ir	<	0.000760	M	Pt	<	0.000760	O	Ti	<	0.001100			
M	Ce	<	0.000760	O	K	0.007078	M	Rb	<	0.000760	M	Tl	<	0.000760				
M	Co	<	0.000760	M	La	<	0.000760	M	Re	<	0.000760	M	Tm	<	0.000760			
O	Cr	<	0.001300	O	Li	<	0.000130	M	Rh	<	0.000760	M	U	<	0.000760			
M	Cs	<	0.000760	M	Lu	<	0.000760	M	Ru	<	0.000760	M	V	<	0.001600			
M	Cu	<	0.003800	O	Mg	0.000707	n	S	<		M	W	<	0.001600				
M	Dy	<	0.000760	O	Mn	0.000149	M	Sb	<	0.000760	M	Y	<	0.000760				
M	Er	<	0.000760	M	Mo	<	0.002300	M	Sc	<	0.000760	M	Yb	<	0.000760			

M - Checked by ICP-MS

O - Checked by ICP-OES

i - Spectral Interference

n - Not Checked For

s - Solution Standard Element

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form In Solution - 114.82 +3 6 In(H₂O)₆+3

Chemical Compatibility -Soluble in HCl, HNO₃, and H₂SO₄. Avoid neutral and basic media. Stable with most metals and inorganic anions. The oxalate, sulfide, carbonate, hydroxide and phosphate are insoluble in water.

Stability - 2-100 ppb levels stable for months in 1% HNO₃ / LDPE container. 1-10,000 ppm solutions chemically stable for years in 2-5% HNO₃ / LDPE container.

In Containing Samples (Preparation and Solution) -Metal (Best dissolved in HCl / HNO₃); Oxide (Soluble in mineral acids); Ores (Carbonate fusion in PtO followed by HCl dissolution); Organic Matrices (Sulfuric/peroxide digestion or dry ash and dissolution in dilute HCl).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 115 amu	1 ppt	n/a	115Sn, 99Ru16O
ICP-OES 158.583 nm	0.05 / 0.002 µg/mL	1	
ICP-OES 230.606 nm	0.1 / 0.03 µg/mL	1	Ni, Os
ICP-OES 325.609 nm	0.2 / 0.05 µg/mL	1	Mn, Mo, Th

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; Info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

February 21, 2023

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- February 21, 2028

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

R: 2/22/24
MS997

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: CLPP-CAL-3
Lot Number: T2-MEB727800
Matrix: 7% (v/v) HNO₃
Value / Analyte(s):
1 000 µg/mL ea:
Arsenic, Lead,
Selenium, Thallium,
500 µg/mL ea:
Cadmium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Arsenic, As	1 000 ± 7 µg/mL	Cadmium, Cd	500.0 ± 2.2 µg/mL
Lead, Pb	1 000 ± 4 µg/mL	Selenium, Se	1 000 ± 6 µg/mL
Thallium, Tl	1 000 ± 7 µg/mL		

Density: 1.042 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
As	ICP Assay	3103a	100818
As	Calculated		See Sec. 4.2
Cd	ICP Assay	3108	130116
Cd	EDTA	928	928
Pb	ICP Assay	3128	101026
Pb	EDTA	928	928
Se	ICP Assay	3149	100901
Tl	ICP Assay	3158	151215

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum (1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty (k)} = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{ts}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum (w_i)^2 (u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{ts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty (k)} = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{ts}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{ts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

December 21, 2022

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **December 21, 2027**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



Certificate of Analysis

R: 08/22/24 M6058, M6059

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: CHEM-CLP-4
Lot Number: V2-MEB746172
Matrix: 3% (v/v) HNO₃
3% (v/v) HF
Value / Analyte(s): 1 000 µg/mL ea:
Boron, Molybdenum,
Silicon, Tin,
Titanium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Boron, B	1 000 ± 5 µg/mL	Molybdenum, Mo	1 000 ± 5 µg/mL
Silicon, Si	1 000 ± 7 µg/mL	Tin, Sn	1 000 ± 5 µg/mL
Titanium, Ti	1 000 ± 6 µg/mL		

Density: 1.032 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
B	ICP Assay	3107	190605
B	Calculated		See Sec. 4.2
Mo	ICP Assay	traceable to 3134	U2-MO739068
Si	ICP Assay	Traceable to 3150	S2-SI702546
Sn	ICP Assay	3161a	140917
Ti	ICP Assay	traceable to 3162a	T2-TI725816

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2 (u_{\text{char } i})^2]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™)

see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale).

<https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

August 12, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **August 12, 2029**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Joseph Burns
Custom VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

Certificate of Analysis

M6074
M6075
M6076
M6077

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

EXP: 9/6/2029

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: CHEM-CLP-4
Lot Number: V2-MEB746762
Matrix: 3% (v/v) HNO₃
3% (v/v) HF
Value / Analyte(s): 1 000 µg/mL ea:
Boron, Molybdenum,
Silicon, Tin,
Titanium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Boron, B	1 000 ± 5 µg/mL	Molybdenum, Mo	1 000 ± 5 µg/mL
Silicon, Si	1 000 ± 7 µg/mL	Tin, Sn	1 000 ± 5 µg/mL
Titanium, Ti	1 000 ± 6 µg/mL		

Density: 1.033 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
B	ICP Assay	3107	190605
B	Calculated		See Sec. 4.2
Mo	ICP Assay	traceable to 3134	U2-MO739068
Si	ICP Assay	Traceable to 3150	S2-SI702546
Sn	ICP Assay	3161a	140917
Ti	ICP Assay	traceable to 3162a	T2-TI725816

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

September 06, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- September 06, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Joseph Burns
Custom VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

Certificate of Analysis

M6074
M6075
M6076
M6077

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

EXP: 9/6/2029

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: CHEM-CLP-4
Lot Number: V2-MEB746762
Matrix: 3% (v/v) HNO₃
3% (v/v) HF
Value / Analyte(s): 1 000 µg/mL ea:
Boron, Molybdenum,
Silicon, Tin,
Titanium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Boron, B	1 000 ± 5 µg/mL	Molybdenum, Mo	1 000 ± 5 µg/mL
Silicon, Si	1 000 ± 7 µg/mL	Tin, Sn	1 000 ± 5 µg/mL
Titanium, Ti	1 000 ± 6 µg/mL		

Density: 1.033 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
B	ICP Assay	3107	190605
B	Calculated		See Sec. 4.2
Mo	ICP Assay	traceable to 3134	U2-MO739068
Si	ICP Assay	Traceable to 3150	S2-SI702546
Sn	ICP Assay	3161a	140917
Ti	ICP Assay	traceable to 3162a	T2-TI725816

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2(u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a)(u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k(u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

September 06, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- September 06, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Joseph Burns
Custom VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number: **58025**
Lot Number: **101124**
Description: **Manganese (Mn)**

R-71113128

Lot #: **24002546**
Solvent: **Nitric Acid**

Expiration Date: **101127**

Recommended Storage: **Ambient (20 °C)**

Nominal Concentration (µg/mL): **1000**

NIST Test Number: **6UTB**

Weight shown below was diluted to (mL): **4000.2**

0.10 Flask Uncertainty

2% **80.0** Nitric Acid (mL)

<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
Reviewed By:	<i>Pedro L. Renteria</i>
	101124

Compound

RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty ± (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
-----	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	--------------------------------	------	----------------	------	----------

1. Manganese(II) nitrate hydrate (Mn) IN031 MMN02020A1 1000 99.999 0.10 20.8 19.2322 19.2344 **1000.1** **2.0** 15710-66-4 5 mg/m3 or-rel >300mg/kg 3132

[1] Spectrum No.1 [34.243 sec]:57025.D# [Count] [Linear]

5.0E6													
2.5E6													
m/z->	10	20	30	40	50	60	70	80	90	100			
1.0E6													
5.0E7													
m/z->	110	120	130	140	150	160	170	180	190	200			
1.0E6													
5.0E7													
m/z->	210	220	230	240	250	260							



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	T	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

M6137
R-71013124

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGSI1
Lot Number: V2-SI744713
Matrix: tr. HNO₃
tr. HF
Value / Analyte(s): 1 000 µg/mL ea:
Silicon
Starting Material: Silica
Starting Material Lot#: 1771
Starting Material Purity: 99.9981%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 999 ± 6 µg/mL
Density: 1.003 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1	999 ± 5 µg/mL ICP Assay NIST SRM Traceable to 3150 Lot Number: S2-SI702546
Assay Method #2	1000 ± 7 µg/mL Calculated NIST SRM Lot Number: See Sec. 4.2

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char\ i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char\ i})^2 / (\sum (1/(u_{char\ i})^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i)^2 (u_{char\ i})^2]^{1/2}$ where $u_{char\ i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char\ a})$$

X_a = mean of Assay Method A with

$u_{char\ a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char\ a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char\ a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.000310	M	Eu	<	0.000310	O	Na		0.001656	M	Se	<	0.022000	M	Zn	<	0.002500
M	Al		0.010787	M	Fe	<	0.027000	M	Nb	<	0.001300	s	Si	<		O	Zr	<	0.001900
M	As	<	0.001900	M	Ga	<	0.001300	M	Nd	<	0.000310	M	Sm	<	0.000310				
M	Au	<	0.000910	M	Gd	<	0.000310	M	Ni	<	0.005500	M	Sn		0.000096				
M	B		0.016180	M	Ge	<	0.001900	M	Os	<	0.000610	O	Sr		0.000092				
M	Ba		0.000096	M	Hf		0.000423	i	P	<		M	Ta		0.002542				
O	Be	<	0.000570	M	Hg	<	0.000610	M	Pb	<	0.000310	M	Tb	<	0.000310				
M	Bi	<	0.000310	M	Ho	<	0.000610	M	Pd	<	0.000610	M	Te	<	0.000910				
O	Ca		0.011557	M	In	<	0.000310	M	Pr	<	0.000310	M	Th	<	0.001900				
M	Cd	<	0.000310	M	Ir	<	0.000310	M	Pt	<	0.000310	M	Ti		0.001078				
M	Ce	<	0.000610	O	K		0.000577	M	Rb	<	0.009100	M	Tl	<	0.000310				
M	Co	<	0.001600	M	La	<	0.000310	M	Re	<	0.000310	M	Tm	<	0.000310				
M	Cr	<	0.010000	O	Li	<	0.000460	M	Rh	<	0.000310	M	U	<	0.000310				
M	Cs	<	0.000310	M	Lu	<	0.000310	M	Ru	<	0.000310	O	V	<	0.001300				
M	Cu	<	0.002500	O	Mg		0.001348	O	S	<	0.570000	M	W	<	0.001900				
M	Dy	<	0.000310	M	Mn	<	0.002500	M	Sb	<	0.000310	M	Y	<	0.000310				
M	Er	<	0.000310	M	Mo	<	0.000310	O	Sc	<	0.000590	M	Yb	<	0.000310				

M - Checked by ICP-MS

O - Checked by ICP-OES

i - Spectral Interference

n - Not Checked For

s - Solution Standard Element

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale, <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form In Solution - 28.09 +4 6 Si(OH)x(F)y2-

Chemical Compatibility -Soluble in HCl, HF, H3PO4 H2SO4 and HNO3 as the Si(OH)x(F)y2-. Avoid neutral to basic media. Unstable at ppm levels with metals that would pull F- away (i.e. Do not mix with Alkaline or Rare Earths, or high levels of transition elements unless they are fluorinated. Stable with most inorganic anions with a tendency to hydrolyze forming silicic acid (silicic acid is soluble up to ∼100 ppm in water) in all dilute acids except HF.

Stability - 2-100 ppb levels - stability unknown - (alone or mixed with all other metals) as the Si(OH)x(F)y2-. 1-10,000 ppm single element solutions as the Si(OH)x(F)y2- chemically stable for years in 2-5 % HNO3 / trace HF in a LDPE container.

Si Containing Samples (Preparation and Solution) -Metal (Soluble in 1:1:1 H2O / HF / HNO3); Oxide - SiO2, amorphous (dissolve by heating in 1:1:1 H2O / HF / HNO3); Oxide - quartz (fuse in Pt0 with Na2CO3); Geological Samples(fuse in Pt0with Na2CO3 followed by HCl solution of the fuseate); Organic Matrices containing silicates and non volatile silicon compounds (dry ash at 4500C in Pt0 and dissolve by gently warming with 1:1:1 H2O / HF / H2SO4 or fuse / ash with Na2CO3 and dissolve fuseate with HCl / H2O); Silicone Oils - dimethyl silicones depolymerize to form volatile monomer units when heated (Measure directly in alcoholic KOH / xylene mixture where sample is treated first with the KOH at 60-1000C to "unzip" the Si- O-Si polymeric structure or digest with conc. H2SO4 / H2O2 followed by cooling and dissolution of the dehydrated silica with HF.) Note that the direct analysis of silicone oils in an organic solvent will result in false high results due to high vapor pressure of volatile monomer units like hexamethylcyclotrisiloxane. The KOH forms the K2+Si(CH3)2O= salt which is not volatile at room temperature.

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 28 amu	4000 - 8000 ppt	N/A	N2, 12C16O
ICP-OES 212.412 nm	0.02/0.01 µg/mL	1	Hf, Os, Mo, Ta
ICP-OES 251.611 nm	0.012/0.003 µg/mL	1	Ta, U, Zn, Th
ICP-OES 288.158 nm	0.03/0.004 µg/mL	1	Ta, Ce, Cr, Cd, Th

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; Inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

July 10, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- July 10, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Custom Processing Supervisor



Certificate Approved By:

Muzzammil Khan
Stock Laboratory Supervisor



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

58126
011025
Iron (Fe)

R-113125
M6140

Lot #
Solvent: 24012496 Nitric Acid

Expiration Date:

011028

2% 40.0 (mL)

Nitric Acid

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

10000

NIST Test Number:

6U7B

5E-05 Balance Uncertainty

Weight shown below was diluted to (mL):

2000.07

0.100 Flask Uncertainty

Formulated By:	Benson Chan	011025
Reviewed By:	Pedro L. Renteria	011025

Compound

Lot
Number

Nominal
Conc. (µg/mL)

Purity
(%)

Uncertainty
(%)

Assay
(%)

Target
Weight (g)

Actual
Weight (g)

Actual
Conc. (µg/mL)

Expanded
Uncertainty
± (µg/mL)

CAS#

OSHA PEL (TWA)

LDSO

NIST

SFM

SDS Information
(Solvent Safety Info. On Attached pg.)

1 mg/m³

or-rel 3250mg/kg 3126A

1. Iron(III) nitrate nonahydrate (Fe)

IN028 FED082023A1

10000

99.999

0.10

13.0

153.8534

#####

10000.2


20.0

7782-61-8

1 mg/m³

or-rel 3250mg/kg 3126A

[1] Spectrum No.1 [30.763 sec]58126.D# [Count] [Linear]

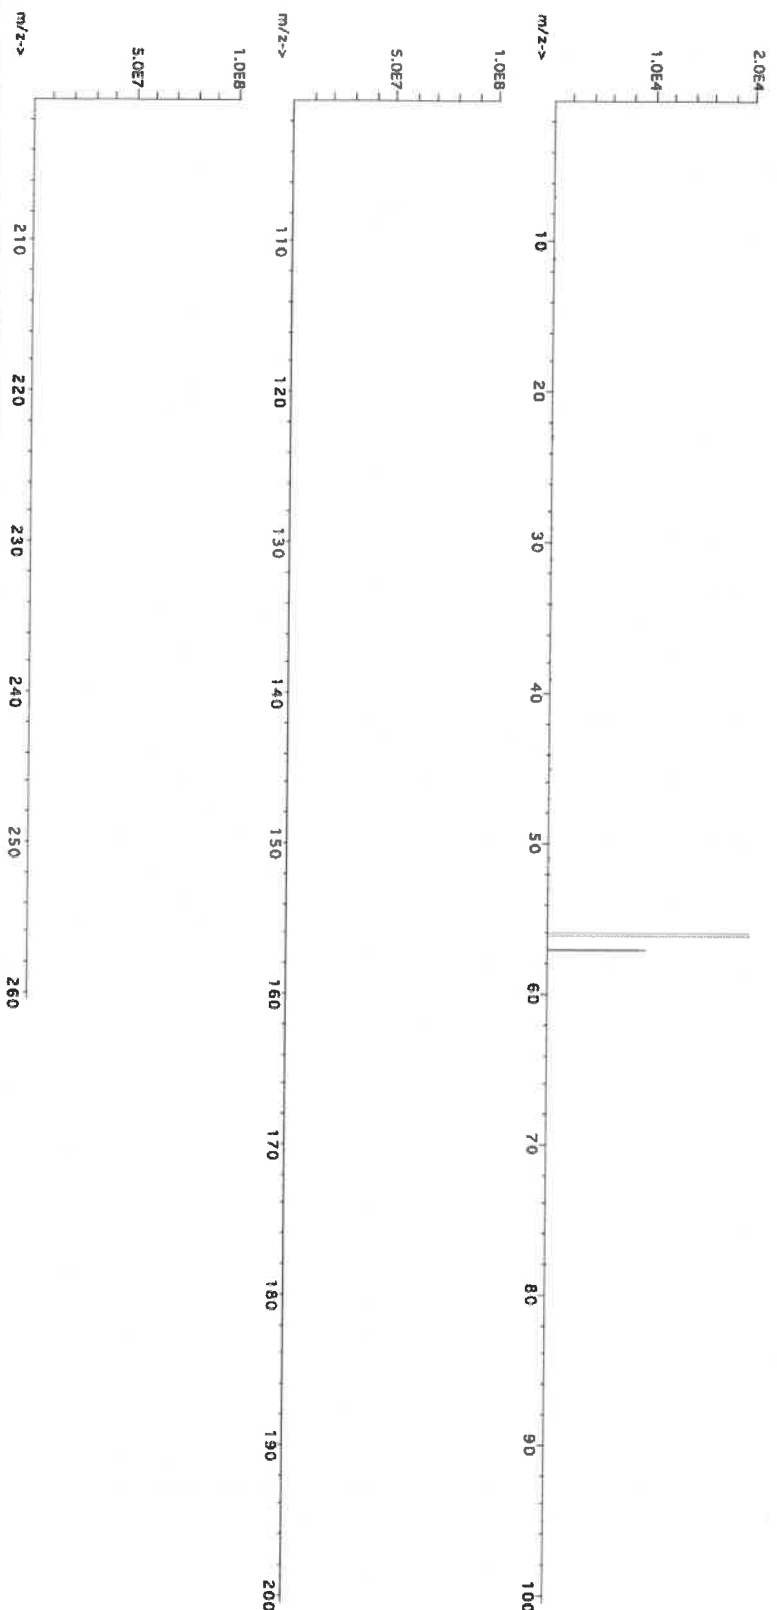



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS ($\mu\text{g/mL}$)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	T	Hg	<0.2	P	<0.02	Sr	<0.02		<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

Har. P. A.

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57119
103024
Potassium (K)

R-21113125

Solvent: 24002546 Nitric Acid
Lot #

<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
Reviewed By:	Pedro L. Renteria
	103024

Expiration Date:
Recommended Storage:
Nominal Concentration (µg/mL):

103027
Ambient (20 °C)
10000

M6141
M6142
M6143

2%
80.0
(mL)
Nitric Acid


Weight shown below was diluted to (mL):

4000.1
0.15
Flask Uncertainty

Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM

1. Potassium nitrate (K) IN034 KD062022A1 10000 99.999 0.10 37.7 106.1040 ##### 10001.1 20.0 7757-79-1 5 mg/m3 orl-rat 3750 mg/kg 3141a

[1] Spectrum No. 1 [35.763 sec]:58119.D# [Count] [Linear]

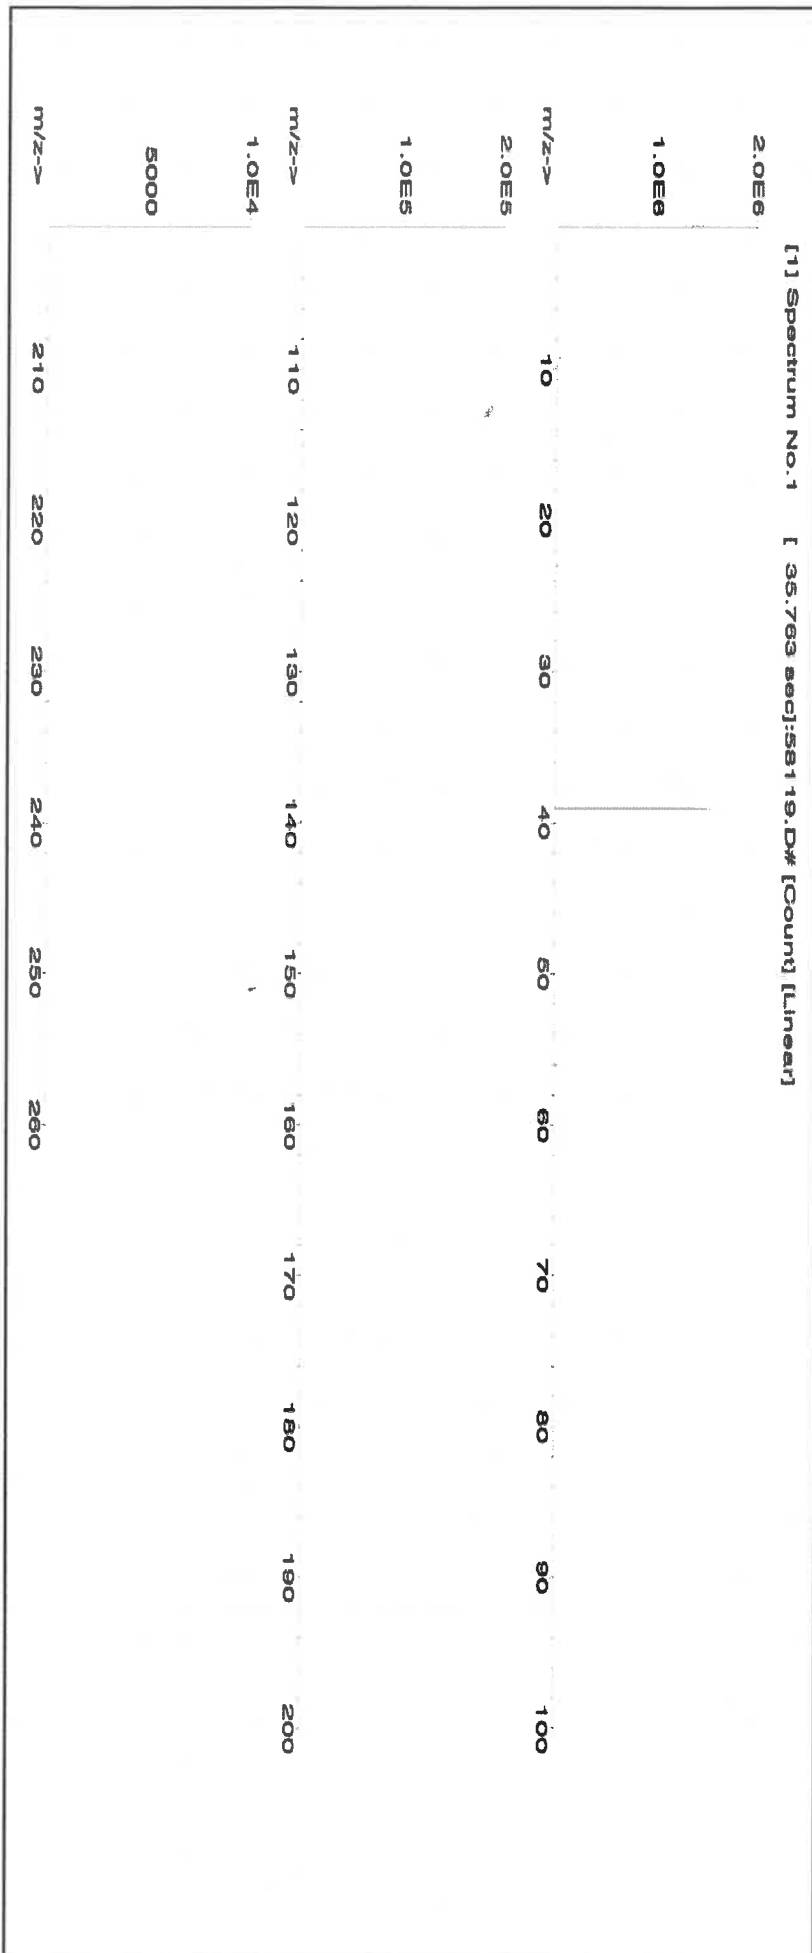



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	T	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



CERTIFIED WEIGHT REPORT:

Part Number: 58111 **Lot #** R-1113/25
Lot Number: 072424 **Solvent:** Nitric Acid
Description: Sodium (Na)

Expiration Date: 072427 **2%** **80.0** **Nitric Acid**
Recommended Storage: Ambient (20 °C) (mL)

Nominal Concentration (µg/mL): 10000

NIST Test Number: 6UTB **5E-05** **Balance Uncertainty**

Weight shown below was diluted to (mL): 4000.2 **0.10** **Flask Uncertainty**


Formulated By:	Benson Chan	072424
Reviewed By:	Pedro L. Renteria	072424

SDS Information

Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	------------	-----------------------	------------	------------------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Sodium nitrate (Na) IN036 NAV01201511 10000 99.999 0.10 26.9 148.7096 ##### 10000.0 20.0 7631-99-4 5 mg/m3 orl-rat 3430 mg/kg 3152a

[1] Spectrum No. 1 [8.935 sec]: 58111.D# [Count] [Linear]

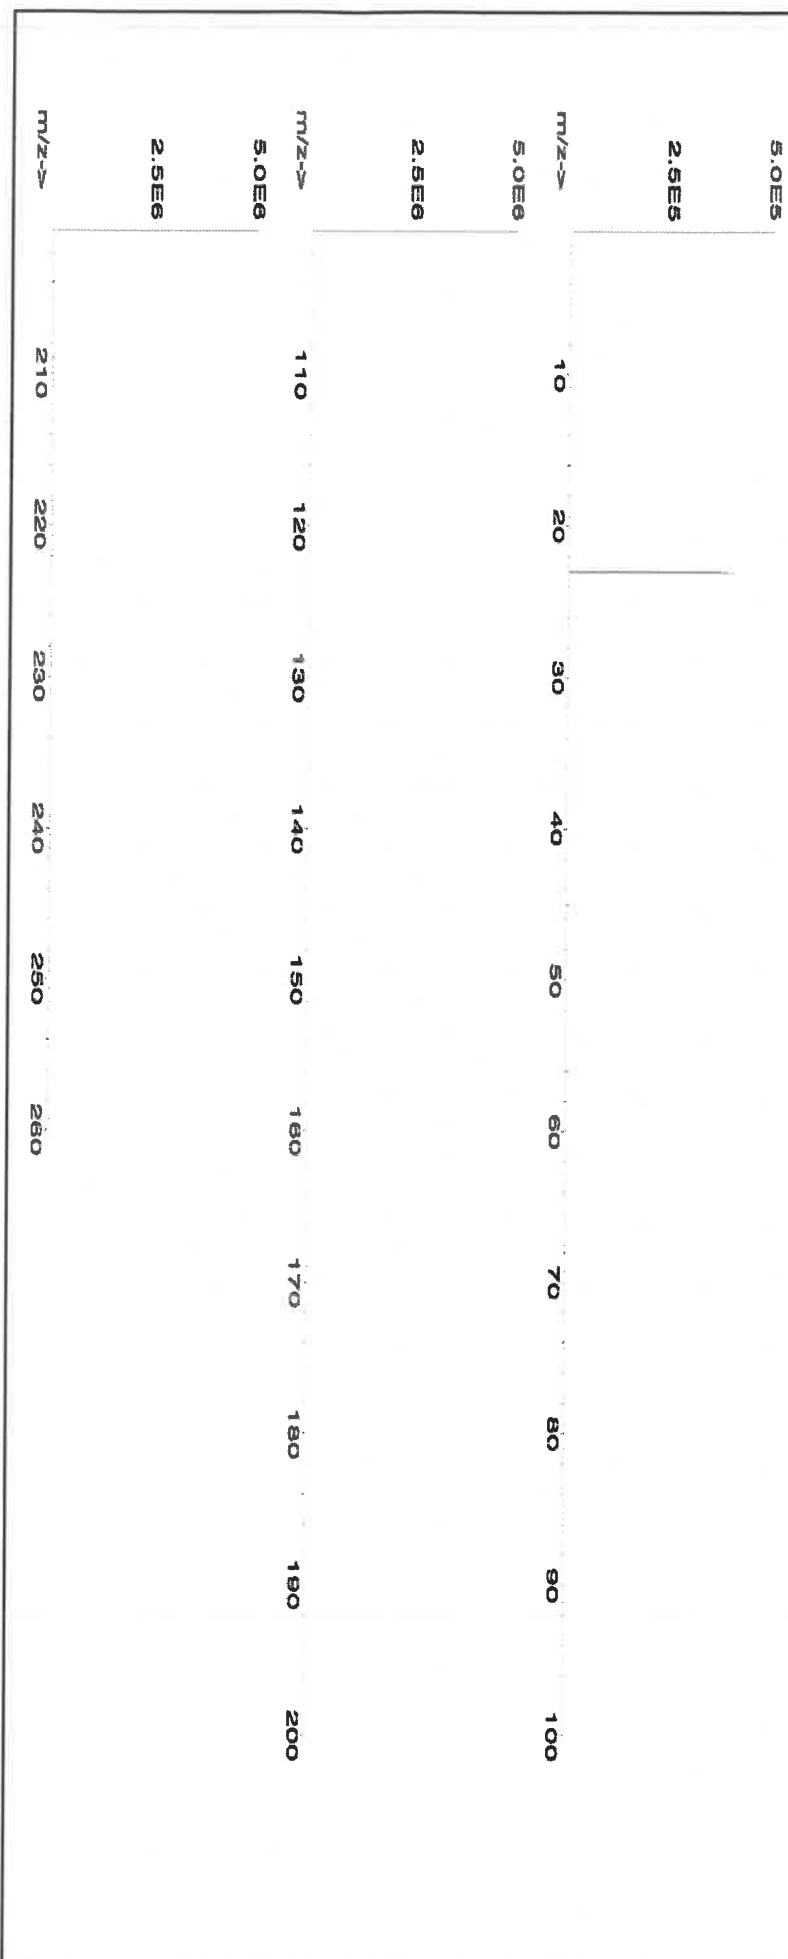



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	T	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).




CERTIFIED WEIGHT REPORT:

Part Number: 58030
Lot Number: 121724
Description: Zinc (Zn)
Expiration Date: 121727
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 2000.1
Balance Uncertainty: 5E-05
Flask Uncertainty: 0.10

Lot # 24012496
Nitric Acid
2%
40.0 (mL)
Nitric Acid

Aleah O'Brady
Formulated By: Aleah O'Brady
Reviewed By: Pedro L. Rentias
121724

SDS Information									
Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty Purity (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)
1. Zinc nitrate hexahydrate (Zn)	IN016	ZNE032021A1	1000	99.999	0.10	24.3	8.2308	8.2311	1000.0
							2.0	10196-18-6	1 mg/m3
									or-rat 1190mg/kg 3168

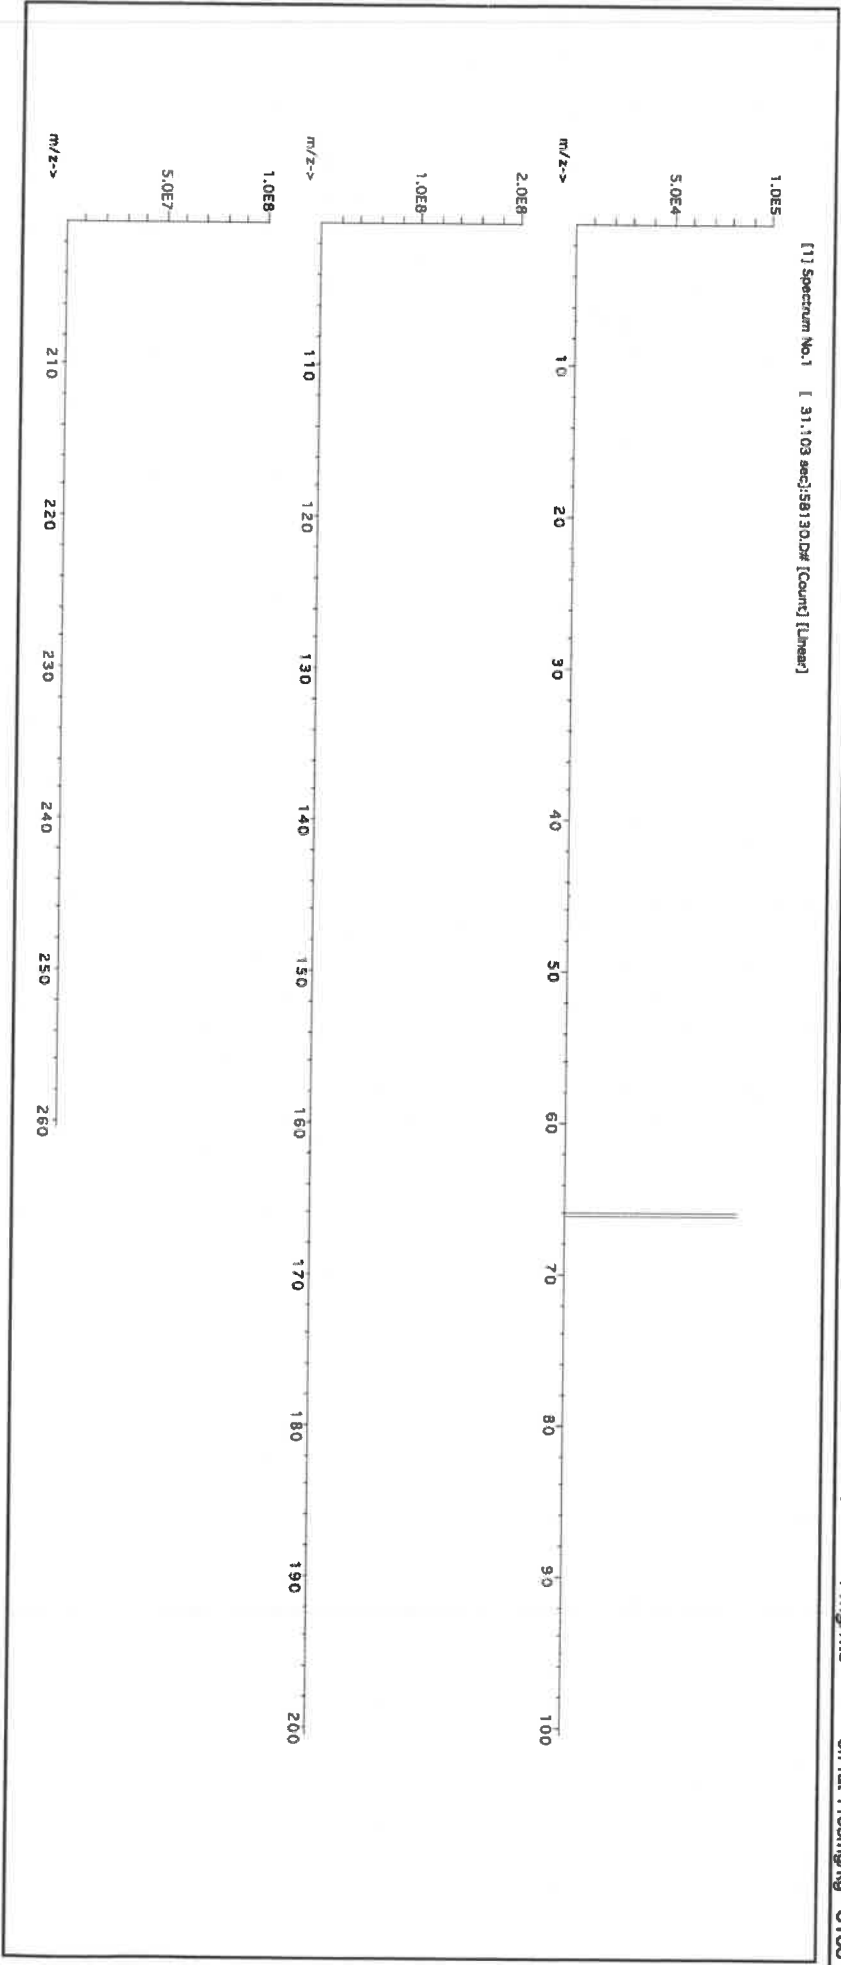



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis

avantor™



M6151

R → 11/15/25

Material No.: 9530-33
Batch No.: 22G2862015
Manufactured Date: 2022-06-15
Retest Date: 2027-06-14
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
ACS – Assay (as HCl) (by acid–base titrn)	36.5 – 38.0 %	37.9 %
ACS – Color (APHA)	≤ 10	5
ACS – Residue after Ignition	≤ 3 ppm	< 1 ppm
ACS – Specific Gravity at 60°/60°F	1.185 – 1.192	1.191
ACS – Bromide (Br)	≤ 0.005 %	< 0.005 %
ACS – Extractable Organic Substances	≤ 5 ppm	< 1 ppm
ACS – Free Chlorine (as Cl ₂)	≤ 0.5 ppm	< 0.5 ppm
Phosphate (PO ₄)	≤ 0.05 ppm	< 0.03 ppm
Sulfate (SO ₄)	≤ 0.5 ppm	< 0.3 ppm
Sulfite (SO ₃)	≤ 0.8 ppm	0.3 ppm
Ammonium (NH ₄)	≤ 3 ppm	< 1 ppm
Trace Impurities – Arsenic (As)	≤ 0.010 ppm	< 0.003 ppm
Trace Impurities – Aluminum (Al)	≤ 10.0 ppb	1.3 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 3.0 ppb
Trace Impurities – Barium (Ba)	≤ 1.0 ppb	0.2 ppb
Trace Impurities – Beryllium (Be)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Bismuth (Bi)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Boron (B)	≤ 20.0 ppb	< 5.0 ppb
Trace Impurities – Cadmium (Cd)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Calcium (Ca)	≤ 50.0 ppb	163.0 ppb
Trace Impurities – Chromium (Cr)	≤ 1.0 ppb	0.7 ppb
Trace Impurities – Cobalt (Co)	≤ 1.0 ppb	< 0.3 ppb
Trace Impurities – Copper (Cu)	≤ 1.0 ppb	< 0.1 ppb
Trace Impurities – Gallium (Ga)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Germanium (Ge)	≤ 3.0 ppb	< 2.0 ppb
Trace Impurities – Gold (Au)	≤ 4.0 ppb	0.6 ppb
Heavy Metals (as Pb)	≤ 100 ppb	< 50 ppb
Trace Impurities – Iron (Fe)	≤ 15 ppb	6 ppb

>>> Continued on page 2 >>>

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis



Material No.: 9530-33
Batch No.: 22G2862015

Test	Specification	Result
Trace Impurities – Lead (Pb)	≤ 1.0 ppb	< 0.5 ppb
Trace Impurities – Lithium (Li)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Magnesium (Mg)	≤ 10.0 ppb	2.9 ppb
Trace Impurities – Manganese (Mn)	≤ 1.0 ppb	< 0.4 ppb
Trace Impurities – Mercury (Hg)	≤ 0.5 ppb	0.1 ppb
Trace Impurities – Molybdenum (Mo)	≤ 10.0 ppb	< 3.0 ppb
Trace Impurities – Nickel (Ni)	≤ 4.0 ppb	< 0.3 ppb
Trace Impurities – Niobium (Nb)	≤ 1.0 ppb	0.8 ppb
Trace Impurities – Potassium (K)	≤ 9.0 ppb	< 2.0 ppb
Trace Impurities – Selenium (Se), For Information Only		< 1.0 ppb
Trace Impurities – Silicon (Si)	≤ 100.0 ppb	< 10.0 ppb
Trace Impurities – Silver (Ag)	≤ 1.0 ppb	0.5 ppb
Trace Impurities – Sodium (Na)	≤ 100.0 ppb	2.3 ppb
Trace Impurities – Strontium (Sr)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Tantalum (Ta)	≤ 1.0 ppb	1.6 ppb
Trace Impurities – Thallium (Tl)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities – Tin (Sn)	≤ 5.0 ppb	4.0 ppb
Trace Impurities – Titanium (Ti)	≤ 1.0 ppb	1.5 ppb
Trace Impurities – Vanadium (V)	≤ 1.0 ppb	< 0.2 ppb
Trace Impurities – Zinc (Zn)	≤ 5.0 ppb	0.8 ppb
Trace Impurities – Zirconium (Zr)	≤ 1.0 ppb	0.3 ppb

>>> Continued on page 3 >>>

Hydrochloric Acid, 36.5–38.0%
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis

 **avantor**™




Material No.: 9530-33
Batch No.: 22G2862015

Test	Specification	Result
------	---------------	--------

For Laboratory, Research, or Manufacturing Use
Product Information (not specifications):
Appearance (clear, fuming liquid)
Meets ACS Specifications
Storage Condition: Store below 25 °C.

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC


Jamie Ethier
Vice President Global Quality

Nitric Acid 69%
CMOS



R- 0210212025

m - 6158

Material No.: 9606-03
Batch No.: 24D1062002
Manufactured Date: 2024-03-26
Retest Date: 2029-03-25
Revision No.: 0

Certificate of Analysis

Test	Specification	Result
Assay (HNO ₃)	69.0 - 70.0 %	69.7 %
Appearance	Passes Test	Passes Test
Color (APHA)	≤ 10	5
Residue after Ignition	≤ 2 ppm	1 ppm
Chloride (Cl)	≤ 0.08 ppm	< 0.03 ppm
Phosphate (PO ₄)	≤ 0.10 ppm	< 0.03 ppm
Sulfate (SO ₄)	≤ 0.2 ppm	< 0.2 ppm
Trace Impurities - Aluminum (Al)	≤ 40.0 ppb	< 1.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities - Barium (Ba)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Bismuth (Bi)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities - Boron (B)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities - Cadmium (Cd)	≤ 50 ppb	< 1 ppb
Trace Impurities - Calcium (Ca)	≤ 50.0 ppb	2.3 ppb
Trace Impurities - Chromium (Cr)	≤ 30.0 ppb	< 1.0 ppb
Trace Impurities - Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Germanium (Ge)	≤ 20 ppb	< 10 ppb
Trace Impurities - Gold (Au)	≤ 20 ppb	< 5 ppb
Heavy Metals (as Pb)	≤ 100 ppb	100 ppb
Trace Impurities - Iron (Fe)	≤ 40.0 ppb	< 1.0 ppb
Trace Impurities - Lead (Pb)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities - Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities - Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities - Nickel (Ni)	≤ 20.0 ppb	< 5.0 ppb

>>> Continued on page 2 >>>

Nitric Acid 69%
CMOS

avantor™



Material No.: 9606-03
Batch No.: 24D1062002

Test	Specification	Result
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 50 ppb	16 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	< 10 ppb
Trace Impurities – Silver (Ag)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 150.0 ppb	< 5.0 ppb
Trace Impurities – Strontium (Sr)	≤ 30.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 5.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 10.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater	≤ 60 par/ml	10 par/ml
Particle Count – 1.0 µm and greater	≤ 10 par/ml	3 par/ml

>>> Continued on page 3 >>>

Nitric Acid 69%
CMOS



m-6162

Material No.: 9606-03
Batch No.: 24H0162012
Manufactured Date: 2024-06-28
Retest Date: 2029-06-27
Revision No.: 0

R. Date :- 04/27/2025

Certificate of Analysis

Test	Specification	Result
Assay (HNO ₃)	69.0 – 70.0 %	69.7 %
Appearance	Passes Test	Passes Test
Color (APHA)	≤ 10	5
Residue after Ignition	≤ 2 ppm	< 1 ppm
Chloride (Cl)	≤ 0.08 ppm	0.03 ppm
Phosphate (PO ₄)	≤ 0.10 ppm	< 0.03 ppm
Sulfate (SO ₄)	≤ 0.2 ppm	< 0.2 ppm
Trace Impurities – Aluminum (Al)	≤ 40.0 ppb	< 1.0 ppb
Arsenic and Antimony (as As)	≤ 5.0 ppb	< 2.0 ppb
Trace Impurities – Barium (Ba)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Beryllium (Be)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Bismuth (Bi)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Boron (B)	≤ 10.0 ppb	0.1 ppb
Trace Impurities – Cadmium (Cd)	≤ 50 ppb	< 1 ppb
Trace Impurities – Calcium (Ca)	≤ 50.0 ppb	0.3 ppb
Trace Impurities – Chromium (Cr)	≤ 30.0 ppb	0.1 ppb
Trace Impurities – Cobalt (Co)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Copper (Cu)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Gallium (Ga)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Germanium (Ge)	≤ 20 ppb	< 1 ppb
Trace Impurities – Gold (Au)	≤ 20 ppb	< 1 ppb
Heavy Metals (as Pb)	≤ 100 ppb	< 50 ppb
Trace Impurities – Iron (Fe)	≤ 40.0 ppb	< 1.0 ppb
Trace Impurities – Lead (Pb)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Lithium (Li)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Magnesium (Mg)	≤ 20 ppb	< 1 ppb
Trace Impurities – Manganese (Mn)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Nickel (Ni)	≤ 20.0 ppb	< 1.0 ppb

>>> Continued on page 2 >>>

Nitric Acid 69%
CMOS

avantor™



Material No.: 9606-03
Batch No.: 24H0162012

Test	Specification	Result
Trace Impurities – Niobium (Nb)	≤ 50.0 ppb	< 1.0 ppb
Trace Impurities – Potassium (K)	≤ 50 ppb	< 1 ppb
Trace Impurities – Silicon (Si)	≤ 50 ppb	1 ppb
Trace Impurities – Silver (Ag)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Sodium (Na)	≤ 150.0 ppb	< 1.0 ppb
Trace Impurities – Strontium (Sr)	≤ 30.0 ppb	< 1.0 ppb
Trace Impurities – Tantalum (Ta)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Thallium (Tl)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Tin (Sn)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Titanium (Ti)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Vanadium (V)	≤ 10.0 ppb	< 1.0 ppb
Trace Impurities – Zinc (Zn)	≤ 20.0 ppb	< 1.0 ppb
Trace Impurities – Zirconium (Zr)	≤ 10.0 ppb	< 1.0 ppb
Particle Count – 0.5 µm and greater	≤ 60 par/ml	13 par/ml
Particle Count – 1.0 µm and greater	≤ 10 par/ml	5 par/ml

>>> Continued on page 3 >>>



300 Technology Drive
 Christiansburg, VA 24073 USA
 inorganicventures.com

P: 800-669-6799/540-585-3030
 F: 540-585-3012
 info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code:	Multi Analyte Custom Grade Solution		
Catalog Number:	QCP-CICV-1		
Lot Number:	V2-MEB744107		
Matrix:	7% (v/v) HNO ₃		
Value / Analyte(s):	2 500 µg/mL ea:		
	Calcium,	Potassium,	
	Magnesium,	Sodium,	
	1 000 µg/mL ea:		
	Aluminum,	Barium,	
	500 µg/mL ea:		
	Iron,		
	250 µg/mL ea:		
	Nickel,	Vanadium,	
	Zinc,	Cobalt,	
	Manganese,		
	125 µg/mL ea:		
	Silver,	Copper,	
	100 µg/mL ea:		
	Chromium,		
	25 µg/mL ea:		
	Beryllium		

Second Source: Whenever possible, this solution was manufactured from a second set of concentrates in our manufacturing facility.

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Aluminum, Al	1 000 ± 4 µg/mL	Barium, Ba	1 000 ± 6 µg/mL
Beryllium, Be	24.98 ± 0.12 µg/mL	Calcium, Ca	2 500 ± 8 µg/mL
Chromium, Cr	99.9 ± 0.6 µg/mL	Cobalt, Co	250.2 ± 1.2 µg/mL
Copper, Cu	125.0 ± 0.5 µg/mL	Iron, Fe	500.0 ± 2.2 µg/mL
Magnesium, Mg	2 500 ± 11 µg/mL	Manganese, Mn	249.9 ± 1.1 µg/mL
Nickel, Ni	250.0 ± 1.2 µg/mL	Potassium, K	2 500 ± 11 µg/mL
Silver, Ag	125.0 ± 0.6 µg/mL	Sodium, Na	2 500 ± 11 µg/mL
Vanadium, V	250.0 ± 1.1 µg/mL	Zinc, Zn	249.9 ± 1.1 µg/mL

Density: 1.081 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Ag	ICP Assay	3151	160729
Ag	Volhard	999c	999c
Al	ICP Assay	3101a	140903
Al	EDTA	928	928
Ba	ICP Assay	3104a	140909
Ba	Gravimetric		See Sec. 4.2
Be	ICP Assay	3105a	090514
Be	Calculated		See Sec. 4.2
Ca	ICP Assay	3109a	130213
Ca	EDTA	928	928
Co	ICP Assay	3113	190630
Co	EDTA	928	928
Cr	ICP Assay	3112a	170630
Cu	ICP Assay	3114	120618
Cu	EDTA	928	928
Fe	ICP Assay	3126a	140812
Fe	EDTA	928	928
K	ICP Assay	3141a	140813
K	Gravimetric		See Sec. 4.2
Mg	ICP Assay	3131a	140110
Mg	EDTA	928	928
Mn	ICP Assay	3132	050429
Mn	EDTA	928	928
Na	ICP Assay	3152a	200413
Na	Gravimetric		See Sec. 4.2
Ni	ICP Assay	3136	120619
Ni	EDTA	928	928
V	ICP Assay	3165	160906
V	EDTA	928	928
Zn	ICP Assay	3168a	120629
Zn	EDTA	928	928

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum(1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum(w_i)^2 (u_{\text{char } i})^2]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale), <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Note: This solution contains Silver (Ag), please refer to our Sample Preparation Guide for more information (<https://www.inorganicventures.com/sample-preparation-guide/samples-containing-silver>)

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

May 22, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **May 22, 2029**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Justin Dirico
Stock Processing Supervisor



Certificate Approved By:

Jodie Wall
Stock VSM Coordinator



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: QCP-CICV-2
Lot Number: U2-MEB733713
Matrix: 3% (w/v) Tartaric acid
1% (v/v) HNO₃
Value / Analyte(s): 500 µg/mL ea:
Antimony

Second Source: Whenever possible, this solution was manufactured from a second set of concentrates in our manufacturing facility.

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Antimony, Sb	500.0 ± 2.8 µg/mL		

Density: 1.017 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Sb	ICP Assay	3102a	140911

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum(w_i)(X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char i}^2) / (\sum(1/u_{char i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k(u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

u_{char} = $[\sum(w_i)^2(u_{char i}^2)]^{1/2}$ where $u_{char i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a)(u_{char a})$$

X_a = mean of Assay Method A with

$u_{char a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k(u_{char a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale). <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

June 01, 2023

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- June 01, 2028

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Approved By:

Thomas Kozikowski
Manager, Quality Control



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
 Christiansburg, VA 24073 USA
 inorganicventures.com

P: 800-669-6799/540-585-3030
 F: 540-585-3012
 info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
 Catalog Number: QCP-CICV-3
 Lot Number: V2-MEB749572
 Matrix: 7% (v/v) HNO₃
 Value / Analyte(s):
 500 µg/mL ea:
 Arsenic, Lead,
 Selenium, Thallium,
 250 µg/mL ea:
 Cadmium

Second Source: Whenever possible, this solution was manufactured from a second set of concentrates in our manufacturing facility.

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Arsenic, As	500.0 ± 3.1 µg/mL	Cadmium, Cd	250.1 ± 1.1 µg/mL
Lead, Pb	500.0 ± 2.3 µg/mL	Selenium, Se	500.0 ± 3.2 µg/mL
Thallium, Tl	500.0 ± 3.0 µg/mL		

Density: 1.040 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
As	ICP Assay	3103a	100818
Cd	ICP Assay	3108	130116
Cd	EDTA	928	928
Pb	ICP Assay	3128	101026
Pb	EDTA	928	928
Se	ICP Assay	3149	100901
Tl	ICP Assay	3158	151215

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum (1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum (w_i)^2 (u_{\text{char } i})^2]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale), <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

January 02, 2025

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **January 02, 2030**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Justin Dirico
Stock Processing Supervisor



Certificate Approved By:

Jodie Wall
Stock VSM Coordinator



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





Certified Reference Material CRM



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
<https://AbsoluteStandards.com>


CERTIFIED WEIGHT REPORT:

Part Number: 58112 **Lot #** M 6171
Lot Number: 011525 **Solvent:** 24012496 Nitric Acid
Description: Magnesium (Mg)
Expiration Date: 011528 2% 40.0 Nitric Acid
Recommended Storage: Ambient (20 °C) (mL)
Nominal Concentration (µg/mL): 10000
NIST Test Number: 6UTB 5E-05 Balance Uncertainty
Weight shown below was diluted to (mL): 2000.07 0.100 Flask Uncertainty

Formulated By:	Benson Chan	011525
Reviewed By:	Pedro L. Rentas	011525

Compound

1. Magnesium nitrate hexahydrate (Mg) IN030 MGD05023A1 10000 99.999 0.10 8.51 234.9183 234.9195 10000.1 20.0 13446-18-9 NA off-ret 5440 mg/kg 3131a

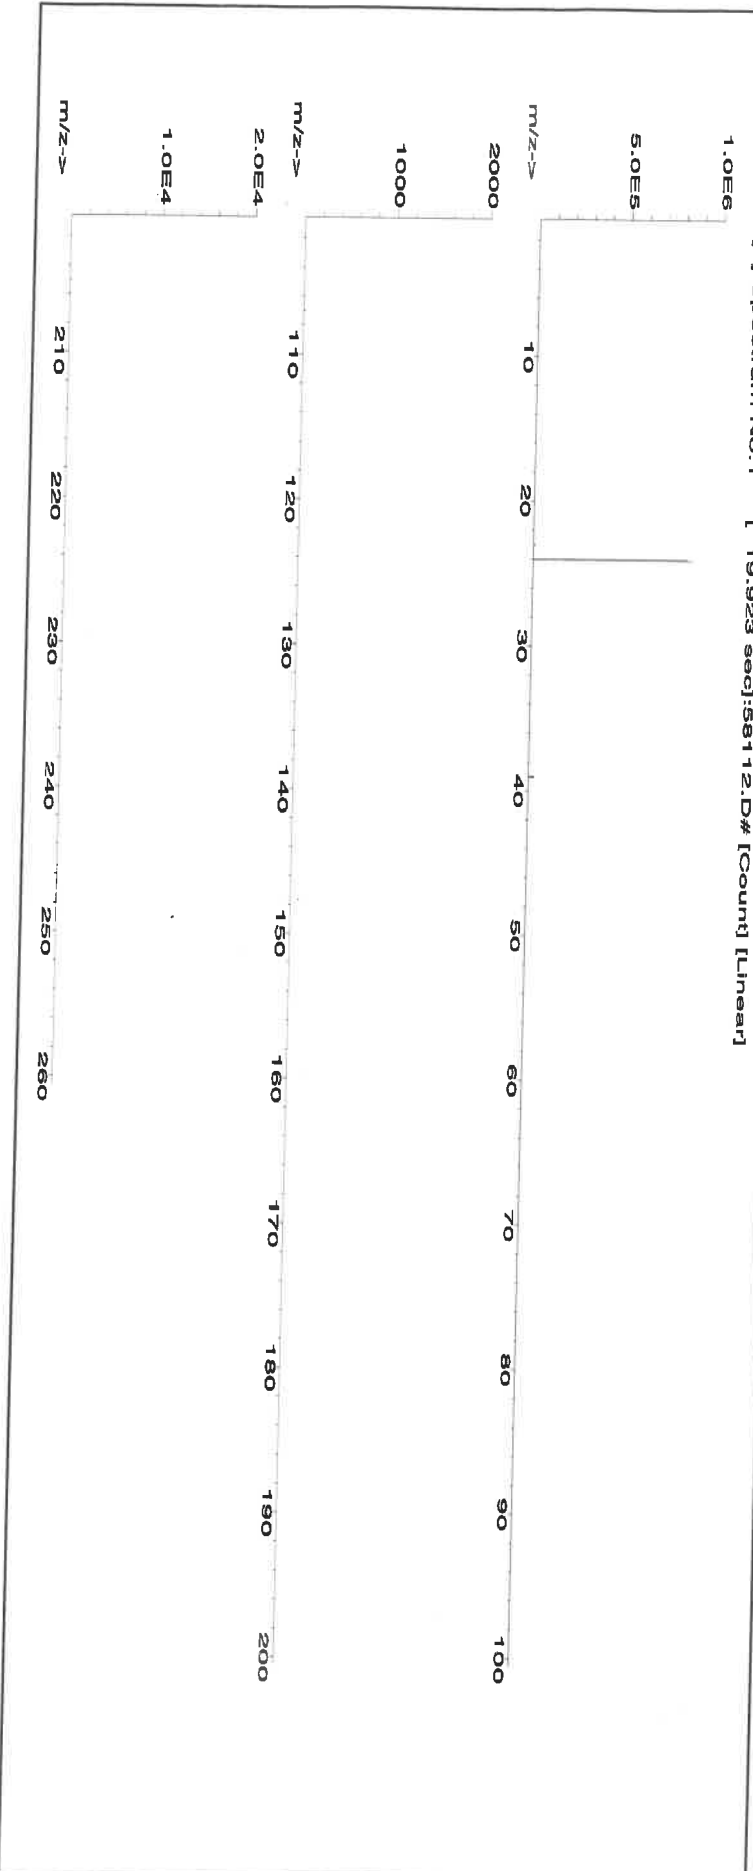



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	T	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ku	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

Certificate of Analysis

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030

F: 540-585-3012

info@inorganicventures.com

M6174
R → S1/S124

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code:	Multi Analyte Custom Grade Solution	
Catalog Number:	CLPP-CAL-1	
Lot Number:	V2-MEB742428	
Matrix:	5% (v/v) HNO ₃	
Value / Analyte(s):	5 000 µg/mL ea:	
	Calcium,	Potassium,
	Magnesium,	Sodium,
	2 000 µg/mL ea:	
	Aluminum,	Barium,
	1 000 µg/mL ea:	
	Iron,	
	500 µg/mL ea:	
	Nickel,	Vanadium,
	Zinc,	Cobalt,
	Manganese,	
	250 µg/mL ea:	
	Silver,	Copper,
	200 µg/mL ea:	
	Chromium,	
	50 µg/mL ea:	
	Beryllium	

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Aluminum, Al	2 000 ± 7 µg/mL	Barium, Ba	2 000 ± 9 µg/mL
Beryllium, Be	50.03 ± 0.30 µg/mL	Calcium, Ca	5 000 ± 16 µg/mL
Chromium, Cr	200.0 ± 1.1 µg/mL	Cobalt, Co	500.0 ± 2.3 µg/mL
Copper, Cu	250.0 ± 1.1 µg/mL	Iron, Fe	1 000 ± 4 µg/mL
Magnesium, Mg	5 000 ± 22 µg/mL	Manganese, Mn	499.9 ± 2.2 µg/mL
Nickel, Ni	500.1 ± 2.3 µg/mL	Potassium, K	5 000 ± 22 µg/mL
Silver, Ag	250.0 ± 1.1 µg/mL	Sodium, Na	5 000 ± 22 µg/mL
Vanadium, V	500.0 ± 2.2 µg/mL	Zinc, Zn	500.0 ± 2.2 µg/mL

Density: 1.117 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Ag	ICP Assay	3151	160729
Ag	Volhard	999c	999c
Al	ICP Assay	3101a	140903
Al	EDTA	928	928
Ba	ICP Assay	3104a	140909
Ba	Gravimetric		See Sec. 4.2
Be	ICP Assay	3105a	090514
Ca	ICP Assay	3109a	130213
Ca	EDTA	928	928
Co	ICP Assay	3113	190630
Co	EDTA	928	928
Cr	ICP Assay	3112a	170630
Cu	ICP Assay	3114	120618
Cu	EDTA	928	928
Fe	ICP Assay	3126a	140812
Fe	EDTA	928	928
K	ICP Assay	3141a	140813
K	Gravimetric		See Sec. 4.2
Mg	ICP Assay	3131a	140110
Mg	EDTA	928	928
Mn	ICP Assay	3132	050429
Mn	EDTA	928	928
Na	ICP Assay	3152a	200413
Na	Gravimetric		See Sec. 4.2
Ni	ICP Assay	3136	120619
Ni	EDTA	928	928
V	ICP Assay	3165	160906
V	EDTA	928	928
Zn	ICP Assay	3168a	120629
Zn	EDTA	928	928

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i})^2 / (\sum (1/u_{\text{char } i})^2)$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum (w_i)^2 (u_{\text{char } i})^2]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale). <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Note: This solution contains Silver (Ag), please refer to our Sample Preparation Guide for more information (<https://www.inorganicventures.com/sample-preparation-guide/samples-containing-silver>)

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; info@inorganicventures.com;
www.inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

March 22, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- **March 22, 2029**

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Custom Processing Supervisor



Certificate Approved By:

Jodie Wall
Stock VSM Coordinator



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





CERTIFIED WEIGHT REPORT:


Part Number: 57038 **Lot #** 24002546 **Solvent:** Nitric Acid
Lot Number: 092724
Description: Strontium (Sr)
Expiration Date: 092727
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 8UTB
Weight shown below was diluted to (mL): 2000.07
5E-05 Balance Uncertainty 0.100 **Flask Uncertainty**

R-5816125
M 6/76

Formulated By:	Benson Chan	092724
Reviewed By:	Pedro L. Rentas	092724

Compound	Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Expanded	SDS Information	NIST
	Number	Conc. (µg/mL)	(%)	Purity (%)	(%)	Weight (g)	Weight (g)	Conc. (µg/mL)	Uncertainty	(Solvent Safety Info. On Attached pg.)	
									± (µg/mL)	CAS#	LD50
										OSHA PEL (TWA)	SRM

1. Strontium nitrate (Sr) IN017 SR2022018A1 1000 99.997 0.10 41.2 4.85470 4.85481 1000.0 2.0 10042-76-9 NA or-rel >2000mg/kg 3153a

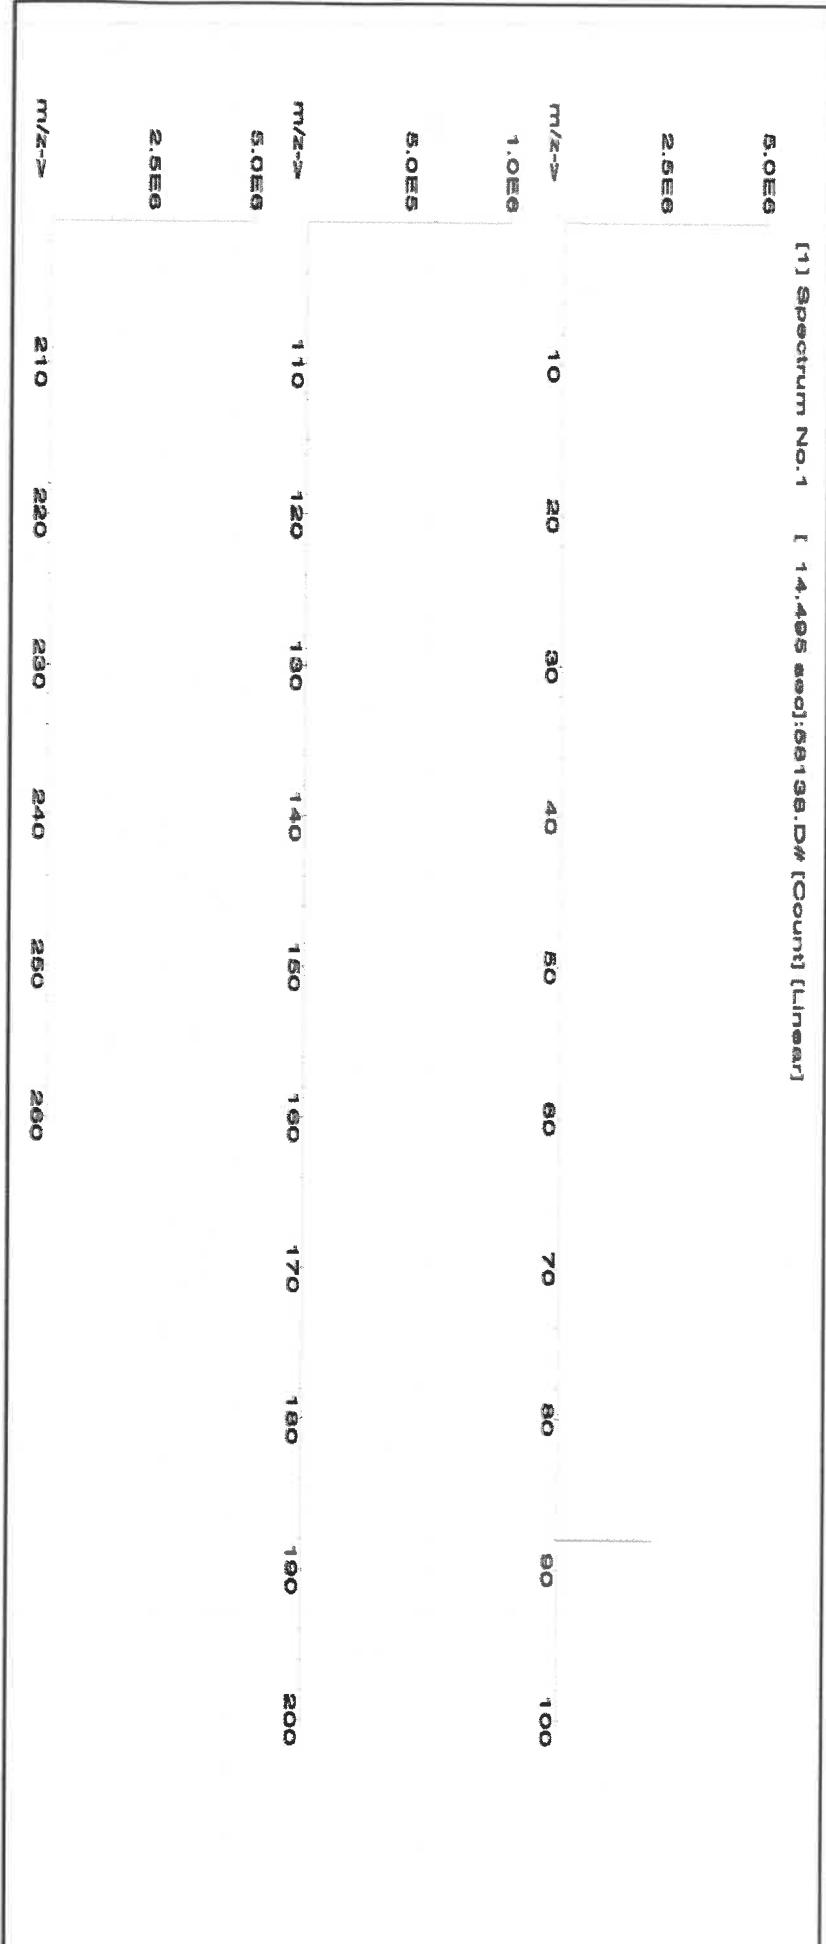



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	T	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
https://AbsoluteStandards.com

CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57042
080525
Molybdenum (Mo)

US#
MKP08697V
080525
Solvent
Ammonium hydroxide
ASTM Type 1 Water

Expiration Date:

080528

Recommended Storage:

Ambient (15 - 30 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

Volume shown below was diluted to (mL):

1999.41

5E-05

Balance Uncertainty

0.058

Fork Uncertainty

R → 8/6/25
M6177


0.5%
10.0
Ammonium hydroxide

Formulated By:	Benson Chan	080525
Reviewed By:	Pedro L. Renteria	080525

Compound		Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty ± (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	--	-------------	------------	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	--------------------------------	------	----------------	------	----------

1. Ammonium molybdate (Mo) 58142 112322 0.1000 200.0 0.084 1000 10001.4 1000.5 2.2 13106-76-8 5 mg(Mo)/mL 0.1-0.3 333 mg/kg 3134

[1] Spectrum No. 1 [8.594 sec]:57042.D# [Count] [Linear]

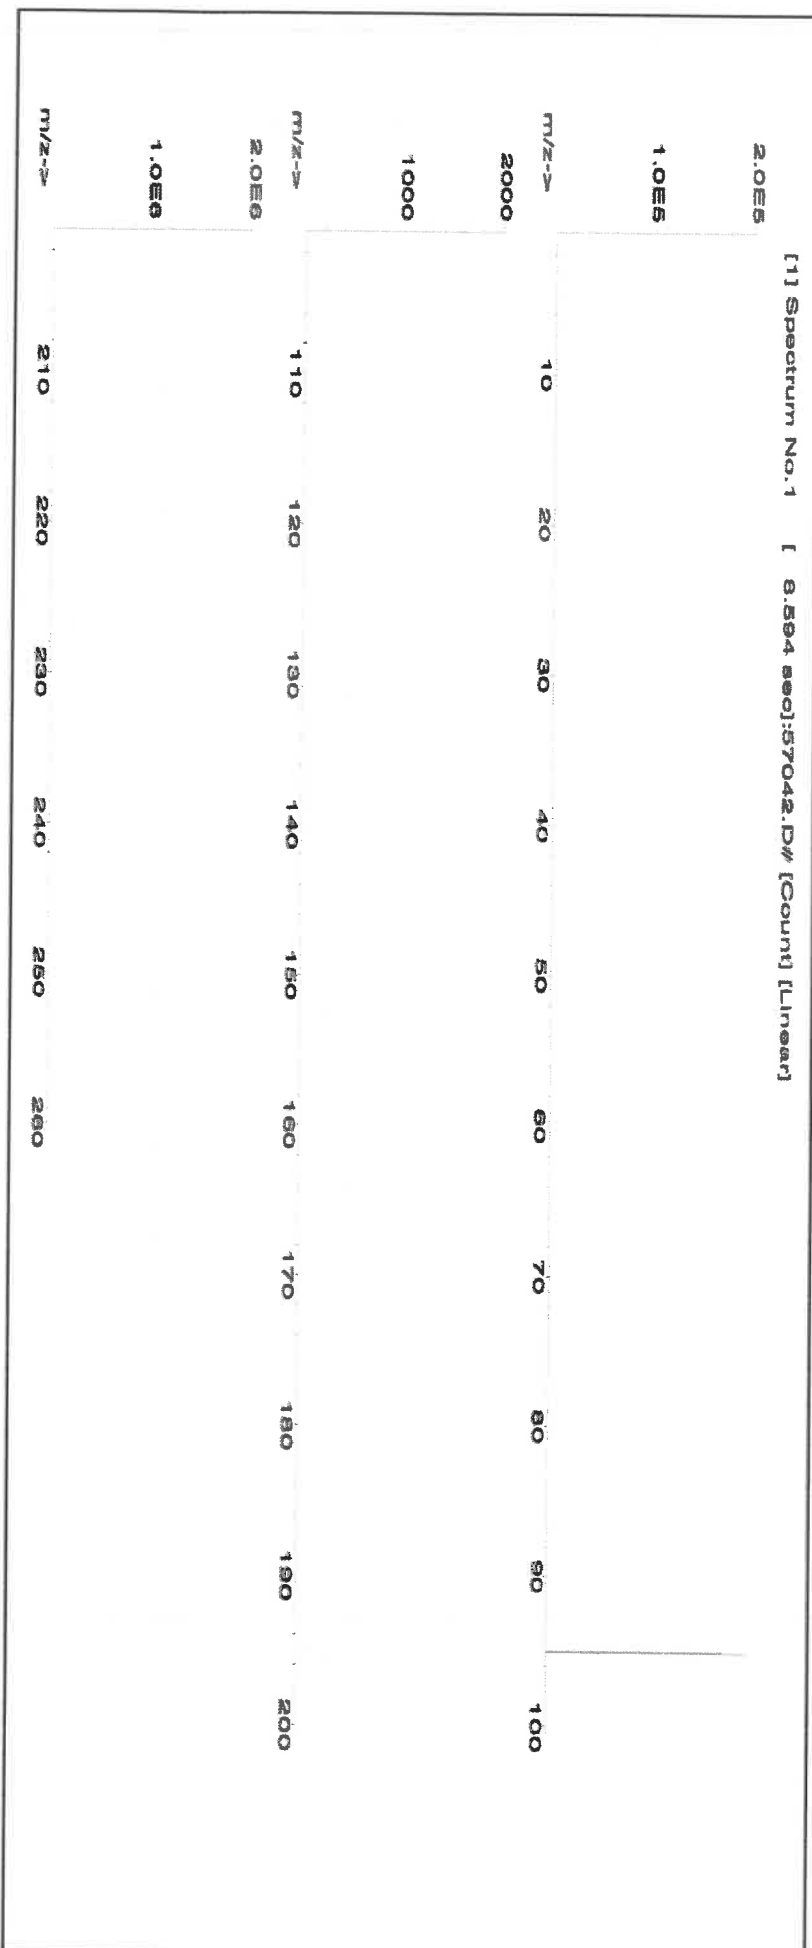



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)															
Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pr	<0.02	Se	<0.2
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02
Ba	<0.02	Ce	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	T	Pt	<0.02	Sm	<0.02	S	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Te	<0.02
														Tb	<0.02
														Ti	<0.02
														Th	<0.02
														Tm	<0.02
														Sn	<0.02
														Tl	<0.02
														U	<0.02
														V	<0.02
														Yb	<0.02
														Y	<0.02
														Zn	<0.02
														Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

[Signature]

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware, and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated by an ISO17025 certified organization with weights traceable through NIST to the SI kilogram (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).
- Rev 1.0, 2/25/2025



CERTIFIED WEIGHT REPORT:

Part Number:
Lot Number:
Description:

57082
031525
Lead (Pb)

Lot #

Nitric Acid

Expiration Date:

031528

Recommended Storage:

Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

SE-05 Balance Uncertainty

Weight shown below was diluted to (mL): 2000.07 0.10 Flask Uncertainty

2%

40.0 (mL)

Nitric Acid

Formulated By:

Giovanni Esposito

031525

Reviewed By:

Pedro L. Renteria

031525

SDS Information


Compound

Lot	Nominal	Purity	Uncertainty	Assay	Target	Actual	Actual	Uncertainty	(Solvent Safety Info. On Attached pg.)			NIST
PM#	Number	Conc. (µg/mL)	(%)	Purity (%)	Weight (g)	Weight (g)	Conc. (µg/mL)	+/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	SRM

1. Lead(II) nitrate (Pb)

IN029	PBD122016A1	1000	99.999	0.10	62.5	3.20015	3.20067	1000.2	2.0	10099-74-8	0.05 mg/m3	Intramuscular 93 mg/kg 3128
-------	-------------	------	--------	------	------	---------	---------	--------	-----	------------	------------	-----------------------------

[1] Spectrum No. 1 [14.144 sec]:58082.D# [Count] [Linear]

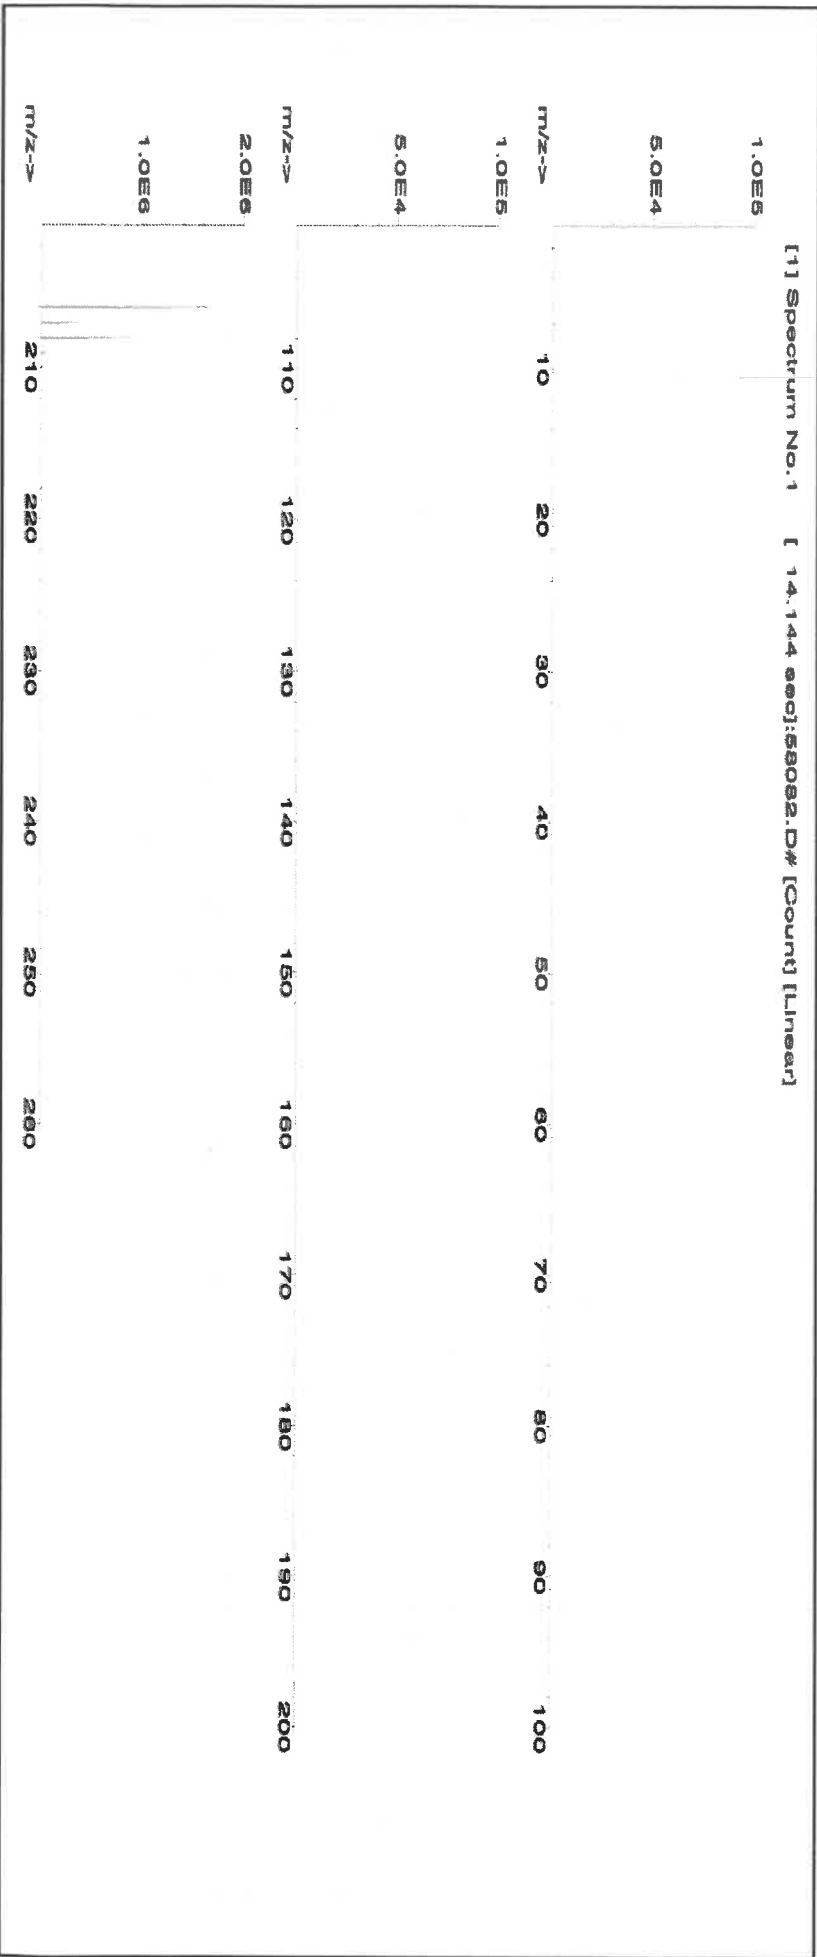



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Sc	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Tc	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Bu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Se	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).

300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

M6179
R → 612/24

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Single Analyte Custom Grade Solution
Catalog Number: CGY10
Lot Number: V2-Y740548
Matrix: 2% (v/v) HNO₃
Value / Analyte(s): 10 000 µg/mL ea:
Yttrium
Starting Material: Yttrium Oxide
Starting Material Lot#: 2661 and 06230520YL
Starting Material Purity: 99.9984%

3.0 CERTIFIED VALUES AND UNCERTAINTIES

Certified Value: 10000 ± 30 µg/mL
Density: 1.032 g/mL (measured at 20 ± 4 °C)

Assay Information:

Assay Method #1	10011 ± 25 µg/mL EDTA NIST SRM 928 Lot Number: 928
Assay Method #2	9997 ± 50 µg/mL ICP Assay NIST SRM 3167a Lot Number: 190730
Assay Method #3	9984 ± 31 µg/mL Calculated NIST SRM Lot Number: See Sec. 4.2

- The Calculated Value is a value calculated from the weight of a starting material that has been certified directly vs. a National Institute of Standards and Technology (NIST) SRM/RM. See Sec 4.2 for balance traceability.

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{CRM/RM}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{CRM/RM} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{char\ i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{char\ i}^2) / (\sum (1/u_{char\ i}^2))$$

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char} = [\sum (w_i)^2 (u_{char\ i}^2)]^{1/2}$ where $u_{char\ i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{CRM/RM}$, where one method of characterization is used is the mean of individual results:

$$X_{CRM/RM} = (X_a) (u_{char\ a})$$

X_a = mean of Assay Method A with

$u_{char\ a}$ = the standard uncertainty of characterization Method A

$$CRM/RM \text{ Expanded Uncertainty } (\pm) = U_{CRM/RM} = k (u_{char\ a}^2 + u_{bb}^2 + u_{lts}^2 + u_{ts}^2)^{1/2}$$

k = coverage factor = 2

$u_{char\ a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{lts} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

CRM/RMs are tested for trace metallic impurities by Axial ICP-OES and ICP-MS. The result from the most sensitive method for each element, is reported below. Solutions tested by ICP-MS were analyzed in an ULPA-Filtered Clean Room. An ULPA-Filter is 99.9985% efficient for the removal of particles down to 0.3 µm.

M	Ag	<	0.004600	M	Eu	0.009037	M	Na	0.086360	M	Se	<	0.005200	M	Zn	0.030125	
M	Al		0.014862	O	Fe	0.002410	M	Nb	<	0.000570	O	Si	0.024100	O	Zr	<	0.002600
M	As	<	0.003500	M	Ga	<	0.000570	M	Nd	0.000923	M	Sm	0.000461				
M	Au	<	0.001700	M	Gd	<	0.003500	M	Ni	<	0.005700	M	Sn	<	0.002300		
O	B		0.002209	M	Ge	<	0.005200	M	Os	<	0.001200	M	Sr	<	0.004600		
O	Ba	<	0.002500	M	Hf	<	0.000570	n	P	<		M	Ta	<	0.000570		
O	Be	<	0.001400	M	Hg	<	0.000570	M	Pb	0.005020	M	Tb	0.001044				
M	Bi	<	0.003500	M	Ho	0.009037	M	Pd	<	0.005100	M	Te	<	0.002300			
O	Ca		0.009841	M	In	<	0.002300	M	Pr	<	0.002300	M	Th	<	0.000570		
M	Cd	<	0.000570	M	Ir	<	0.000570	M	Pt	<	0.000570	M	Ti	<	0.003500		
M	Ce	<	0.002300	O	K	0.018677	M	Rb	<	0.000570	M	Tl	<	0.000570			
M	Co	<	0.000570	M	La	0.000461	M	Re	<	0.000570	M	Tm	<	0.003500			
M	Cr	<	0.004000	O	Li	<	0.009300	M	Rh	<	0.008000	M	U	<	0.000570		
M	Cs	<	0.000570	M	Lu	0.000582	M	Ru	<	0.000570	M	V	0.001265				
M	Cu		0.002610	O	Mg	0.001486	n	S	<		M	W	<	0.002300			
M	Dy		0.003815	M	Mn	0.000582	M	Sb	0.005422	s	Y	<					
M	Er		0.003615	M	Mo	<	0.005700	M	Sc	<	0.001200	M	Yb	0.001827			

M - Checked by ICP-MS

O - Checked by ICP-OES

i - Spectral Interference

n - Not Checked For

s - Solution Standard Element

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale). <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.
- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.
- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Atomic Weight; Valence; Coordination Number; Chemical Form In Solution - 88.91 +3 6 Y(OH)(H₂O)_{x+2}

Chemical Compatibility -Soluble in HCl, H₂SO₄ and HNO₃. Avoid HF, H₃PO₄ and neutral to basic media. Stable with most metals and inorganic anions forming an insoluble carbonate, oxide, oxalate, and fluoride. Avoid mixing with elements / solutions containing moderate amounts of fluoride.

Stability - 2-100 ppb levels stable for months in 1% HNO₃ / LDPE container. 1-10,000 ppm solutions chemically stable for years in 2-5% HNO₃ / LDPE container.

Y Containing Samples (Preparation and Solution) - Metal (Soluble in acids); Oxide (Dissolve by heating in H₂O / HNO₃); Ores (Carbonate fusion in PtO followed by HCl dissolution); Organic Matrices (Dry ash and dissolve in 1:1 H₂O / HCl or HNO₃).

Atomic Spectroscopic Information (ICP-OES D.L.s are given as radial/axial view):

Technique/Line	Estimated D.L.	Order	Interferences (underlined indicates severe)
ICP-MS 89 amu	0.8 ppt	N/A	73Ge16O, 178Hf+2
ICP-OES 360.073 nm	0.005 / 0.000036 µg/mL	1	Ce, Th
ICP-OES 371.030 nm	0.004 / 0.00007 µg/mL	1	Ce
ICP-OES 377.433 nm	0.005 / 0.0009 µg/mL	1	Ta, Th

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

February 20, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- February 20, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Uyen Truong
Custom Processing Supervisor



Certificate Approved By:

Muzzammil Khan
Stock Laboratory Supervisor



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: WW-LFS-1
Lot Number: W2-MEB752149
Matrix: 5% (v/v) HNO₃

M6180
R-37/22/23

Value / Analyte(s):	
1 000 µg/mL ea:	
Potassium,	
600 µg/mL ea:	
Phosphorus,	
300 µg/mL ea:	
Sodium,	Iron,
200 µg/mL ea:	
Magnesium,	Aluminum,
Cerium,	Selenium,
Thallium,	
100 µg/mL ea:	
Lead,	Calcium,
80 µg/mL ea:	
Arsenic,	
70 µg/mL ea:	
Mercury,	
50 µg/mL ea:	
Nickel,	
40 µg/mL ea:	
Chromium,	
30 µg/mL ea:	
Copper,	Boron,
Vanadium,	
20 µg/mL ea:	
Zinc,	Strontium,
Barium,	Beryllium,
Cadmium,	Cobalt,
Manganese,	Lithium,
7.5 µg/mL ea:	
Silver	

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Aluminum, Al	200.2 ± 0.7 µg/mL	Arsenic, As	80.1 ± 0.5 µg/mL
Barium, Ba	20.02 ± 0.12 µg/mL	Beryllium, Be	20.02 ± 0.11 µg/mL
Boron, B	30.02 ± 0.15 µg/mL	Cadmium, Cd	20.04 ± 0.09 µg/mL
Calcium, Ca	100.1 ± 0.3 µg/mL	Cerium, Ce	200.2 ± 1.0 µg/mL
Chromium, Cr	40.02 ± 0.26 µg/mL	Cobalt, Co	20.03 ± 0.09 µg/mL
Copper, Cu	30.03 ± 0.13 µg/mL	Iron, Fe	300.3 ± 1.3 µg/mL
Lead, Pb	100.1 ± 0.5 µg/mL	Lithium, Li	20.03 ± 0.09 µg/mL
Magnesium, Mg	200.2 ± 0.9 µg/mL	Manganese, Mn	19.99 ± 0.09 µg/mL
Mercury, Hg	70.0 ± 0.3 µg/mL	Nickel, Ni	50.05 ± 0.22 µg/mL
Phosphorus, P	600.5 ± 2.9 µg/mL	Potassium, K	1 001 ± 4 µg/mL
Selenium, Se	200.2 ± 1.1 µg/mL	Silver, Ag	7.52 ± 0.03 µg/mL
Sodium, Na	300.3 ± 1.3 µg/mL	Strontium, Sr	20.02 ± 0.10 µg/mL
Thallium, Tl	200.2 ± 1.0 µg/mL	Vanadium, V	30.02 ± 0.13 µg/mL
Zinc, Zn	20.05 ± 0.09 µg/mL		

Density: 1.037 g/mL (measured at 20 ± 5 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Ag	ICP Assay	3151	160729
Ag	Volhard	999c	999c
Al	ICP Assay	3101a	140903
Al	EDTA	928	928
As	ICP Assay	3103a	100818
B	ICP Assay	3107	190605
B	Calculated		See Sec. 4.2
Ba	ICP Assay	3104a	140909
Ba	Gravimetric		See Sec. 4.2
Be	ICP Assay	3105a	090514
Ca	ICP Assay	3109a	130213
Ca	EDTA	928	928
Cd	ICP Assay	3108	130116
Cd	EDTA	928	928
Ce	ICP Assay	3110	160830
Ce	EDTA	928	928
Co	ICP Assay	3113	190630
Co	EDTA	928	928
Cr	ICP Assay	3112a	170630
Cu	ICP Assay	3114	120618
Cu	EDTA	928	928
Fe	ICP Assay	3126a	140812
Fe	EDTA	928	928
Hg	ICP Assay	3133	160921
Hg	EDTA	928	928
K	ICP Assay	3141a	140813
K	Gravimetric		See Sec. 4.2
Li	ICP Assay	3129a	100714
Li	Gravimetric		See Sec. 4.2
Mg	ICP Assay	3131a	140110
Mg	EDTA	928	928
Mn	ICP Assay	3132	050429
Mn	EDTA	928	928
Na	ICP Assay	3152a	200413
Na	Gravimetric		See Sec. 4.2
Ni	ICP Assay	3136	120619
Ni	EDTA	928	928
P	ICP Assay	3139a	060717
P	Acidimetric	84L	84L
Pb	ICP Assay	3128	101026
Pb	EDTA	928	928
Se	ICP Assay	3149	100901
Sr	EDTA	928	928
Sr	ICP Assay	Traceable to 3153a	K2-SR650985
Tl	ICP Assay	3158	151215
V	ICP Assay	3165	160906
V	EDTA	928	928
Zn	ICP Assay	3168a	120629
Zn	EDTA	928	928

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of $k = 2$.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i}^2) / (\sum (1/u_{\text{char } i}^2))$$

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{ITS}}^2 + u_{\text{TS}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum (w_i)^2 (u_{\text{char } i}^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{ITS} = long term stability standard uncertainty (storage)

u_{TS} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty } (\pm) = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{ITS}}^2 + u_{\text{TS}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{ITS} = long term stability standard uncertainty (storage)

u_{TS} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures [Terms and Conditions of Sale](https://www.inorganicventures.com/terms-and-conditions-sale). <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 25° C to minimize the effects of transpiration. Use at 20° ± 5° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

Note: This solution contains Silver (Ag), please refer to our Sample Preparation Guide for more information (<https://www.inorganicventures.com/sample-preparation-guide/samples-containing-silver>)

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; Info@inorganicventures.com;

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

April 08, 2025

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- April 08, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Justin Dirico
Stock Processing Supervisor



Certificate Approved By:

Jodie Wall
Stock VSM Coordinator



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director



300 Technology Drive
Christiansburg, VA 24073 USA
inorganicventures.com

Certificate of Analysis

P: 800-669-6799/540-585-3030
F: 540-585-3012
info@inorganicventures.com

M6181
R → 7/22/28

1.0 ACCREDITATION / REGISTRATION

INORGANIC VENTURES is accredited to ISO 17034, "General Requirements for the Competence of Reference Material Producers" and ISO/IEC 17025, "General Requirements for the Competence of Testing and Calibration Laboratories". Inorganic Ventures is also an ISO 9001 registered manufacturer (QSR Certificate Number QSR-1034).



2.0 PRODUCT DESCRIPTION

Product Code: Multi Analyte Custom Grade Solution
Catalog Number: WW-LFS-2
Lot Number: V2-MEB743480
Matrix: 5% (v/v) HNO₃
tr. HF
Value / Analyte(s):
200 µg/mL ea:
Silica,
80 µg/mL ea:
Antimony,
70 µg/mL ea:
Tin,
40 µg/mL ea:
Molybdenum,
20 µg/mL ea:
Titanium

3.0 CERTIFIED VALUES AND UNCERTAINTIES

ANALYTE	CERTIFIED VALUE	ANALYTE	CERTIFIED VALUE
Antimony, Sb	80.1 ± 0.5 µg/mL	Molybdenum, Mo	40.05 ± 0.22 µg/mL
Silica, SiO ₂	200.3 ± 1.4 µg/mL	Tin, Sn	70.1 ± 0.4 µg/mL
Titanium, Ti	20.03 ± 0.12 µg/mL		

Density: 1.025 g/mL (measured at 20 ± 4 °C)

Assay Information:

ANALYTE	METHOD	NIST SRM#	SRM LOT#
Mo	ICP Assay	3134	130418
Sb	ICP Assay	3102a	140911
SiO ₂	Calculated		See Sec. 4.2
Sn	ICP Assay	3161a	140917
Ti	ICP Assay	traceable to 3162a	T2-TI725816

The following equations are used in the calculation of the certified value and the uncertainty. Reported uncertainties represent expanded uncertainties expressed at approximately the 95% confidence level using a coverage factor of k = 2.

Characterization of CRM/RM by Two or More Methods

Certified Value, $X_{\text{CRM/RM}}$, where two or more methods of characterization are used is the weighted mean of the results:

$$X_{\text{CRM/RM}} = \sum (w_i) (X_i)$$

X_i = mean of Assay Method i with standard uncertainty $u_{\text{char } i}$

w_i = the weighting factors for each method calculated using the inverse square of the variance:

$$w_i = (1/u_{\text{char } i})^2 / (\sum (1/u_{\text{char } i})^2)$$

$$\text{CRM/RM Expanded Uncertainty (z)} = U_{\text{CRM/RM}} = k (u_{\text{char}}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char}} = [\sum ((w_i)^2 (u_{\text{char } i})^2)]^{1/2}$ where $u_{\text{char } i}$ are the errors from each characterization method

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

Characterization of CRM/RM by One Method

Certified Value, $X_{\text{CRM/RM}}$, where one method of characterization is used is the mean of individual results:

$$X_{\text{CRM/RM}} = (X_a) (u_{\text{char } a})$$

X_a = mean of Assay Method A with

$u_{\text{char } a}$ = the standard uncertainty of characterization Method A

$$\text{CRM/RM Expanded Uncertainty (z)} = U_{\text{CRM/RM}} = k (u_{\text{char } a}^2 + u_{\text{bb}}^2 + u_{\text{Its}}^2 + u_{\text{ts}}^2)^{1/2}$$

k = coverage factor = 2

$u_{\text{char } a}$ = the errors from characterization

u_{bb} = bottle to bottle homogeneity standard uncertainty

u_{Its} = long term stability standard uncertainty (storage)

u_{ts} = transport stability standard uncertainty

4.0 TRACEABILITY TO NIST

- This product is traceable to NIST via an unbroken chain of comparisons. The uncertainties for each certified value are reported, taking into account the SRM/RM uncertainty error and the measurement, weighing and volume dilution errors. In rare cases where no NIST SRM/RM are available, the term 'in-house std.' is specified.

4.1 Thermometer Calibration

- All thermometers are NIST traceable through thermometers that are calibrated by an accredited calibration laboratory.

4.2 Balance Calibration

- All analytical balances are calibrated by an accredited calibration laboratory and procedure. The weights used for testing are annually compared to master weights and are traceable to NIST.

4.3 Glassware Calibration

- An in-house procedure is used to calibrate all Class A glassware used in the manufacturing and quality control of CRM/RMs.

5.0 TRACE METALLIC IMPURITIES (TMI) DETERMINED BY ICP-MS AND ICP-OES (µg/mL)

N/A

6.0 INTENDED USE

6.1 This standard is intended for the calibration of analytical instruments and validation of analytical methods as appropriate. This CRM may be used in connection with EPA Methods 6010, 6020 (all versions), Standard Methods 3120 B and USP <232> / ICH Q3D.

6.2 For products attaining traceability through Inorganic Ventures' Primary Certified Reference Materials (PCRM™) see the Limited License to Use PCRM™ in the Inorganic Ventures Terms and Conditions of Sale. <https://www.inorganicventures.com/terms-and-conditions-sale>. The Terms and Conditions contain information on the use of materials traceable to PCRM™ certified reference materials. This Limited License agreement is especially pertinent for laboratories accredited under ISO:17034.

7.0 INSTRUCTIONS FOR THE CORRECT USE OF THIS REFERENCE MATERIAL

7.1 Storage and Handling Recommendations

- Store between approximately 4° - 30° C while in sealed TCT bag.

- While stored in the sealed TCT bag, transpiration of this CRM/RM is negligible. After opening the sealed TCT bag transpiration of the CRM/RM will occur, resulting in a gradual increase in the analyte concentration(s). It is the responsibility of the user to account for this effect. When the bottle is weighed both before and after being placed in storage, the mass difference observed will be a measure of transpiration mass loss.

- After opening the sealed TCT bag, keep cap tightly sealed when not in use and store between 4° - 24° C to minimize the effects of transpiration. Use at 20° ± 4° C to minimize volumetric dilution error when using the reported density. Do not pipette from the container. Do not return removed aliquots to container.

- For more information, visit www.inorganicventures.com/TCT

HF Note: This standard should not be prepared or stored in glass.

8.0 HAZARDOUS INFORMATION

- Please refer to the Safety Data Sheet for information regarding this CRM/RM.

9.0 HOMOGENEITY

- This solution was mixed according to an in-house procedure and is guaranteed to be homogeneous. Homogeneity data indicate that the end user should take a minimum sample size of 0.2 mL to assure homogeneity.

10.0 QUALITY STANDARD DOCUMENTATION

10.1 ISO 9001 Quality Management System Registration

- QSR Certificate Number QSR-1034

10.2 ISO/IEC 17025 "General Requirements for the Competence of Testing and Calibration Laboratories"

- Chemical Testing - Accredited / A2LA Certificate Number 883.01

10.3 ISO 17034 "General Requirements for the Competence of Reference Material Producers"

- Reference Material Producer - Accredited / A2LA Certificate Number 883.02

Inorganic Ventures, 300 Technology Drive, Christiansburg, Va. 24073, USA; Telephone: 800.669.6799; 540.585.3030, Fax: 540.585.3012; inorganicventures.com; info@inorganicventures.com

11.0 CERTIFICATION, LOT EXPIRATION AND PERIOD OF VALIDITY

11.1 Certification Issue Date

May 07, 2024

- The certification is valid within the measurement uncertainty specified provided the CRM/RM is stored and handled in accordance with instructions given in Sec 7.1. This certification is nullified if instructions in Sec 7.1 are not followed or if the CRM/RM is damaged, contaminated, or otherwise modified.

11.2 Lot Expiration Date

- May 07, 2029

- The date after which this CRM/RM should not be used.

- The lot expiration date reflects the period of time that the stability of a CRM/RM can be supported by long term stability studies conducted on properly stored and handled CRM/RMs. Lot expiration is limited primarily by transpiration (loss of water from the solution) and infrequently by chemical stability.

11.3 Period of Validity

- Sealed TCT Bag Open Date: _____

- This CRM/RM should not be used longer than one year (or six months in the case of a 30 mL bottle) from the date of opening the aluminized bag or after the date given in Sec. 11.2, whichever comes first. This is contingent upon the CRM/RM being stored and handled in accordance with the instructions given in Sec. 7.1.

12.0 NAMES AND SIGNATURES OF CERTIFYING OFFICERS

Certificate Prepared By:

Justin Dirico
Stock Processing Supervisor



Certificate Approved By:

Thomas Kozikowski
Stock VS Manager



Certifying Officer:

Paul Gaines
Chairman / Senior Technical Director





Instructions for QATS Reference Material: ICP-AES ICS

QATS LABORATORY INORGANIC REFERENCE MATERIAL
INTERFERENCE CHECK SAMPLE SET FOR ICP-AES (ICSA WITH ICSB)

NOTE: These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

APPLICATION: For use with the CLP SFAM01.0 SOW and revisions.

CAUTION: Read instructions carefully before opening bottle(s) and proceeding with the analyses.



M6182

(A) **SAMPLE DESCRIPTION**

Enclosed is a set of one (1) or more bottles of Aqueous Reference Material, each composed of metals at various concentrations and prepared with nitrate salts and oxy-acids of the respective elements in a 5% nitric acid matrix. **For the reference material source in reporting ICSA and ICSAB mixture use "USEPA". For the reference material lot number for the ICSA use "ICSA-1211" and for the ICSAB mixture use "ICSA-1211+ICSB-0710".**

CAUTION: The bottle(s) should be protected from light during storage to ensure the stability of silver which is contained in the ICSB solution. The bottle(s) should be stored at room temperature. **Do not allow the solution(s) to freeze.**

(B) **BREAKAGE OR MISSING ITEMS**

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY
APTIM Federal Services, LLC
2700 Chandler Avenue - Building C
Las Vegas, NV 89120

(C) **ANALYSIS OF SAMPLES**

The interference check sample set is to be used to verify inter-element and background correction factors of inductively-coupled plasma (ICP) spectrometers. This reference material set consists of two (2) concentrated solutions. The ICSA solution contains the four (4) interferent elements: Al, Ca, Fe, and Mg. The ICSB solution contains the analytes: Ag, As, Sb, Ba, Be,





Instructions for QATS Reference Material: ICP-AES ICS

Cd, Co, Cr, Cu, Mn, Ni, Pb, Tl, Se, V, and Zn. This instruction sheet provides the nominal values for ICP-AES Part A and Part B target analytes when diluted as directed.

Using Class "A" glassware, preparation and analysis must be performed according to the following instructions:

ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSA solution by ICP-AES.

ICSB-0710, Analytes, mixed with ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution and 10 mL of the ICSB solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSAB solution by ICP-AES.

(D) "CERTIFIED VALUE" CONCENTRATIONS OF QATS ICP-AES ICS SOLUTION(S)

The "Certified Value" concentrations of the elements, listed in Table 1 below, were derived from statistically pooled analysis results from the following sources, if available: QATS Laboratory, CLP laboratories, Quarterly Blind (QB)/Proficiency Testing (PT) events, CLP pre-award events, and external referee laboratories.

Table 1. "CERTIFIED VALUES" FOR INTERFERENCE CHECK SAMPLE ICP-AES ICSA-1211, AND ICSA-1211 MIXED WITH ICSB-0710

Element	CRQL	Part A (µg/L)	Low Limit (µg/L)	High Limit (µg/L)	Part A +Part B (µg/L)	Low Limit (µg/L)	High Limit (µg/L)
Al	200	255000	216000	294000	247000	209000	285000
Sb	60	(0.0)	-60.0	60.0	618	525	711
As	10	(0.0)	-10.0	10.0	104	88.4	120
Ba	200	(6.0)	-194	206	(537)	337	737
Be	5.0	(0.0)	-5.0	5.0	495	420	570
Cd	5.0	(1.0)	-4.0	6.0	972	826	1120
Ca	5000	245000	208000	282000	235000	199000	271000
Cr	10	(52.0)	42.0	62.0	542	460	624
Co	50	(0.0)	-50.0	50.0	476	404	548
Cu	25	(2.0)	-23.0	27.0	511	434	588
Fe	100	101000	85600	116500	99300	84400	114500
Pb	10	(0.0)	-10.0	10.0	(49.0)	39.0	59.0
Mg	5000	255000	216000	294000	248000	210000	286000
Mn	15	(7.0)	-8.0	22.0	507	430	584
Ni	40	(2.0)	-38.0	42.0	954	810	1100
Se	35	(0.0)	-35.0	35.0	(46.0)	11.0	81.0
Ag	10	(0.0)	-10.0	10.0	201	170	232
Tl	25	(0.0)	-25.0	25.0	(108)	83.0	133
V	50	(0.0)	-50.0	50.0	491	417	565
Zn	60	(0.0)	-60.0	60.0	952	809	1095

The acceptance ranges for all analytes in parentheses in the above table were determined using the listed certified value ± 1 times the associated CLP SOW CRQL. The acceptance ranges for all other analytes were determined using the certified value ± 15 percent of the listed certified value.




Instructions for QATS Reference Material: ICP-AES ICS

QATS LABORATORY INORGANIC REFERENCE MATERIAL
INTERFERENCE CHECK SAMPLE SET FOR ICP-AES (ICSA WITH ICSB)

NOTE: These instructions are for advisory purposes only. If any apparent conflict exists between these instructions and the analytical protocol or your contract, disregard these instructions.

APPLICATION: For use with the CLP SFAM01.0 SOW and revisions.

CAUTION: Read instructions carefully before opening bottle(s) and proceeding with the analyses.

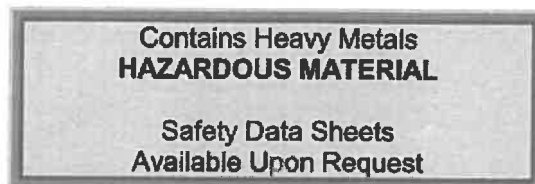

M6184

(A) **SAMPLE DESCRIPTION**

Enclosed is a set of one (1) or more bottles of Aqueous Reference Material, each composed of metals at various concentrations and prepared with nitrate salts and oxy-acids of the respective elements in a 5% nitric acid matrix. **For the reference material source in reporting ICSA and ICSAB mixture use "USEPA". For the reference material lot number for the ICSA use "ICSA-1211" and for the ICSAB mixture use "ICSA-1211+ICSB-0710".**

CAUTION: The bottle(s) should be protected from light during storage to ensure the stability of silver which is contained in the ICSB solution. The bottle(s) should be stored at room temperature. **Do not allow the solution(s) to freeze.**

(B) **BREAKAGE OR MISSING ITEMS**

Check the contents of the shipment carefully for any broken, leaking, or missing items. Check that the seal is intact on each bottle. Refer to the enclosed chain of custody record. Report any problems to Mr. Keith Strout, APTIM Federal Services, LLC, at (702) 895-8722. If requested, return the chain-of-custody record with appropriate annotations and signatures to the address provided below.

QUALITY ASSURANCE TECHNICAL SUPPORT LABORATORY
APTIM Federal Services, LLC
2700 Chandler Avenue - Building C
Las Vegas, NV 89120

(C) **ANALYSIS OF SAMPLES**

The interference check sample set is to be used to verify inter-element and background correction factors of inductively-coupled plasma (ICP) spectrometers. This reference material set consists of two (2) concentrated solutions. The ICSA solution contains the four (4) interferent elements: Al, Ca, Fe, and Mg. The ICSB solution contains the analytes: Ag, As, Sb, Ba, Be,





Instructions for QATS Reference Material: ICP-AES ICS

Cd, Co, Cr, Cu, Mn, Ni, Pb, Tl, Se, V, and Zn. This instruction sheet provides the nominal values for ICP-AES Part A and Part B target analytes when diluted as directed.

Using Class "A" glassware, preparation and analysis must be performed according to the following instructions:

ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSA solution by ICP-AES.

ICSB-0710, Analytes, mixed with ICSA-1211, Interferents: Pipet 10 mL of the ICSA solution and 10 mL of the ICSB solution into a 100 mL volumetric flask and dilute to volume with 2% v/v HNO₃. Analyze this ICSAB solution by ICP-AES.

(D) "CERTIFIED VALUE" CONCENTRATIONS OF QATS ICP-AES ICS SOLUTION(S)

The "Certified Value" concentrations of the elements, listed in Table 1 below, were derived from statistically pooled analysis results from the following sources, if available: QATS Laboratory, CLP laboratories, Quarterly Blind (QB)/Proficiency Testing (PT) events, CLP pre-award events, and external referee laboratories.

Table 1. "CERTIFIED VALUES" FOR INTERFERENCE CHECK SAMPLE ICP-AES ICSA-1211, AND ICSA-1211 MIXED WITH ICSB-0710

Element	CRQL	Part A (µg/L)	Low Limit (µg/L)	High Limit (µg/L)	Part A +Part B (µg/L)	Low Limit (µg/L)	High Limit (µg/L)
Al	200	255000	216000	294000	247000	209000	285000
Sb	60	(0.0)	-60.0	60.0	618	525	711
As	10	(0.0)	-10.0	10.0	104	88.4	120
Ba	200	(6.0)	-194	206	(537)	337	737
Be	5.0	(0.0)	-5.0	5.0	495	420	570
Cd	5.0	(1.0)	-4.0	6.0	972	826	1120
Ca	5000	245000	208000	282000	235000	199000	271000
Cr	10	(52.0)	42.0	62.0	542	460	624
Co	50	(0.0)	-50.0	50.0	476	404	548
Cu	25	(2.0)	-23.0	27.0	511	434	588
Fe	100	101000	85600	116500	99300	84400	114500
Pb	10	(0.0)	-10.0	10.0	(49.0)	39.0	59.0
Mg	5000	255000	216000	294000	248000	210000	286000
Mn	15	(7.0)	-8.0	22.0	507	430	584
Ni	40	(2.0)	-38.0	42.0	954	810	1100
Se	35	(0.0)	-35.0	35.0	(46.0)	11.0	81.0
Ag	10	(0.0)	-10.0	10.0	201	170	232
Tl	25	(0.0)	-25.0	25.0	(108)	83.0	133
V	50	(0.0)	-50.0	50.0	491	417	565
Zn	60	(0.0)	-60.0	60.0	952	809	1095

The acceptance ranges for all analytes in parentheses in the above table were determined using the listed certified value ± 1 times the associated CLP SOW CRQL. The acceptance ranges for all other analytes were determined using the certified value ± 15 percent of the listed certified value.



Certified Reference Material CRM

M6027



CERTIFIED WEIGHT REPORT:

Part Number: **57028**
Lot Number: **062024**
Description: **Nickel (NI)**


Lot # **24002546**
Solvent: **Nitric Acid**

Formulated By:	Benson Chan
062024	
Reviewed By:	Pedro L. Rentes
062024	

Expiration Date: **062027**
Recommended Storage: **Ambient (20 °C)**
Nominal Concentration (µg/mL): **1000**
NIST Test Number: **6UTB**
Volume shown below was diluted to (mL): **2000.07**
5E-05 Balance Uncertainty
0.100 Flask Uncertainty

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pippet (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM

1. Nickel(II) nitrate hexahydrate (NI) 58128 062023 0.1000 200.0 0.084 1000 10000.4 1000.0 2.2 13478-00-7 1 mg/m3 orl-rat 1620 mg/kg 3136

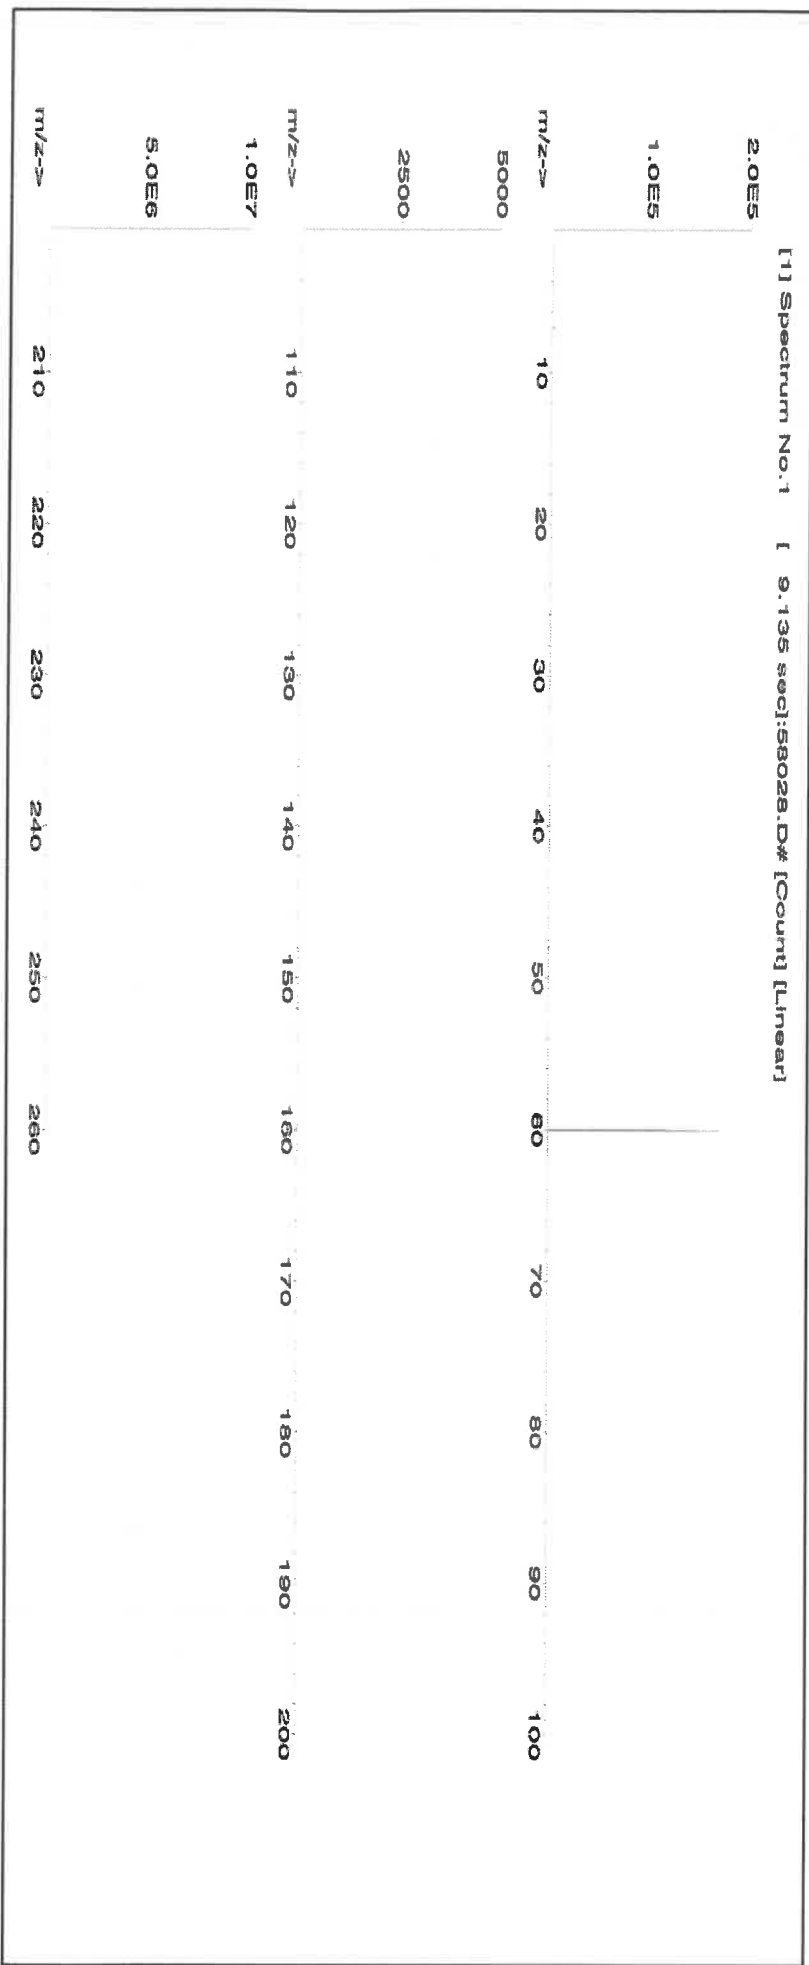



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	T	Pr	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

M6030



ANAB ISO 17034 Accredited
AR-1539 Certificate Number
<https://absolutestandards.com>

CERTIFIED WEIGHT REPORT:

Part Number: **57047**
Lot Number: **122823**
Description: **Silver (Ag)**

Solvent: 24002546 Nitric Acid
Lot #


Formulated By:	Benson Chan
Reviewed By:	Pedro L. Rentas
	122823

Expiration Date: 122826
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB
Weight shown below was diluted to (mL): 4000.30
5E-05 Balance Uncertainty
0.058 Flask Uncertainty

SDS Information									
Compound	RM#	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)
1. Silver nitrate (Ag)	IN035	J0612AGAI	1000.0	99.999	0.10	63.7	6.27992	6.27998	1000.0

Expanded Uncertainty +/- (µg/mL) 2.0 7761-88-8 10 µg/mL3 NA 3151

[1] Spectrum No. 1 [14.044 sec]:58147.D# [Count] [Linear]

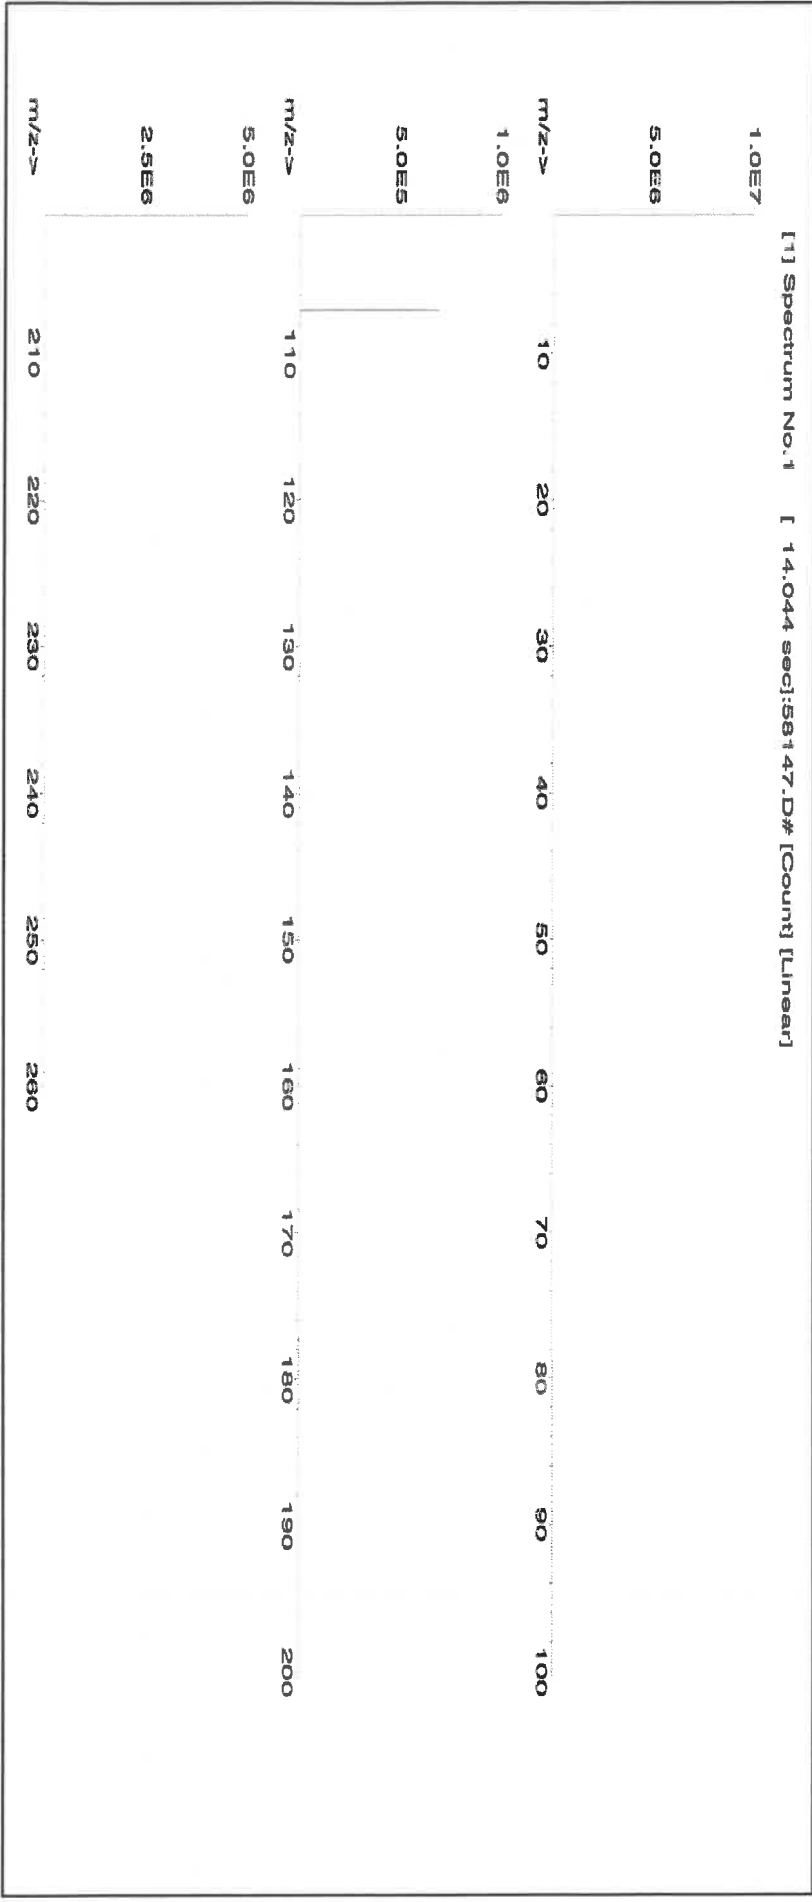



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	T	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02	Ta	<0.02	Ti	<0.02	Zr	<0.02

Physical Characterization:

(T)= Target analyte

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 meqohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



R: 10/18/24
Certified Reference Material CRM



CERTIFIED WEIGHT REPORT:

Part Number: **57051**

Lot Number: **071724**

Description: **Antimony (Sb)**

Lot # **24002546**
Solvent: **Nitric Acid**

Expiration Date: **071727**

Recommended Storage: **Ambient (20 °C)**

Nominal Concentration (µg/mL): **1000**

NIST Test Number: **6LJB**

Volume shown below was diluted to (mL): **2000.26**

5E-05 Balance Uncertainty
0.058 Flask Uncertainty


2.0% 40.0 (mL) Nitric Acid

<i>Giovanni Esposito</i>	
Formulated By:	Giovanni Esposito
	071724
<i>Pedro L. Rentas</i>	
Reviewed By:	Pedro L. Rentas
	071724

SDS Information

Compound	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	-------------	------------	-----------------	-------------------	--------------------------	-----------------------	-----------------------	---------------------	----------------------------------	------	----------------	------	----------

1. Antimony (Sb)	58151	060324	0.1000	200.0	0.084	1000	10001.4	1000.0	2.2	7440-36-0	0.5 mg/m3	or-rat 7000 mg/kg	3102a
------------------	-------	--------	--------	-------	-------	------	---------	--------	-----	-----------	-----------	-------------------	-------

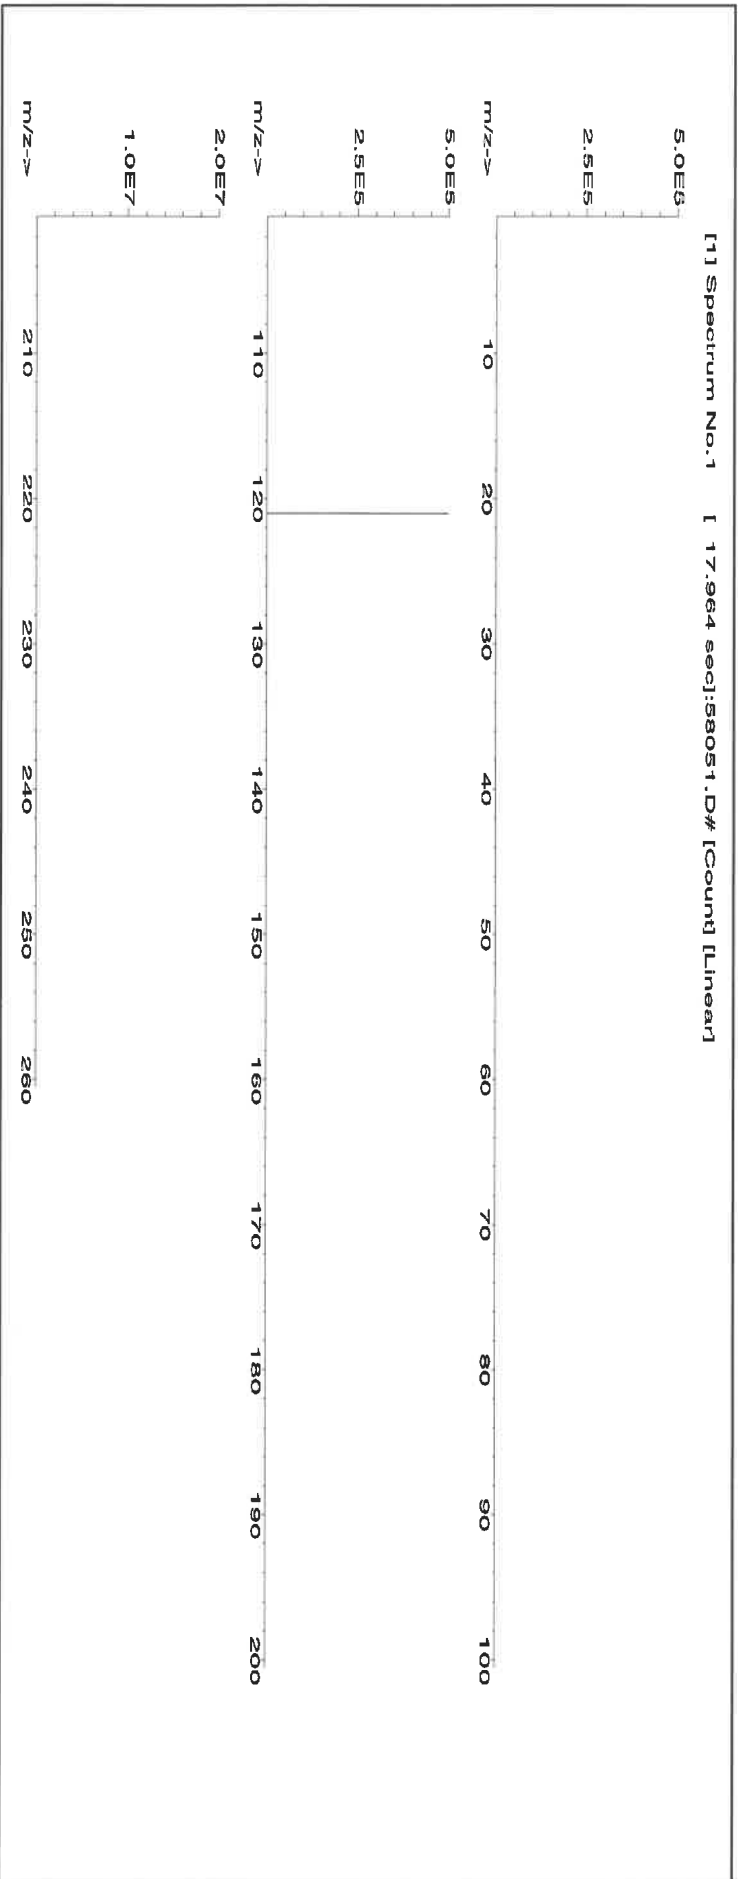

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17



CERTIFIED WEIGHT REPORT:

Part Number: 57081
Lot Number: 062724
Description: Thallium (TI)

Lot #

Solvent: 24002546 Nitric Acid

Aliah O'Brady
Formulated By: Aliah O'Brady 062724

Expiration Date:

062727

2%

40.0

Nitric Acid

Recommended Storage: Ambient (20 °C)

Nominal Concentration (µg/mL):

1000

NIST Test Number:

6UTB

5E-05 Balance Uncertainty

Weight shown below was diluted to (mL):

2000.1

0.10 Flask Uncertainty


Pedro L. Renteria
Reviewed By: Pedro L. Renterias 062724

SDS Information

Compound	Lot Number	Nominal Conc. (µg/mL)	Purity (%)	Uncertainty (%)	Assay (%)	Target Weight (g)	Actual Weight (g)	Actual Conc. (µg/mL)	Expanded Uncertainty +/- (µg/mL)	CAS#	OSHA PEL (TWA)	LD50	NIST SRM
----------	------------	-----------------------	------------	-----------------	-----------	-------------------	-------------------	----------------------	----------------------------------	------	----------------	------	----------

1. Thallium nitrate (TI) IN037 BCCF4399 1000 99.999 0.10 77.0 2.5975 2.5977 1000.1 2.0 10102-45-1 0.1 mg/m3 or-mus 15mg/kg 3158

[1] Spectrum No.1 [14.044 sec]:57081.D# [Count] [Linear]

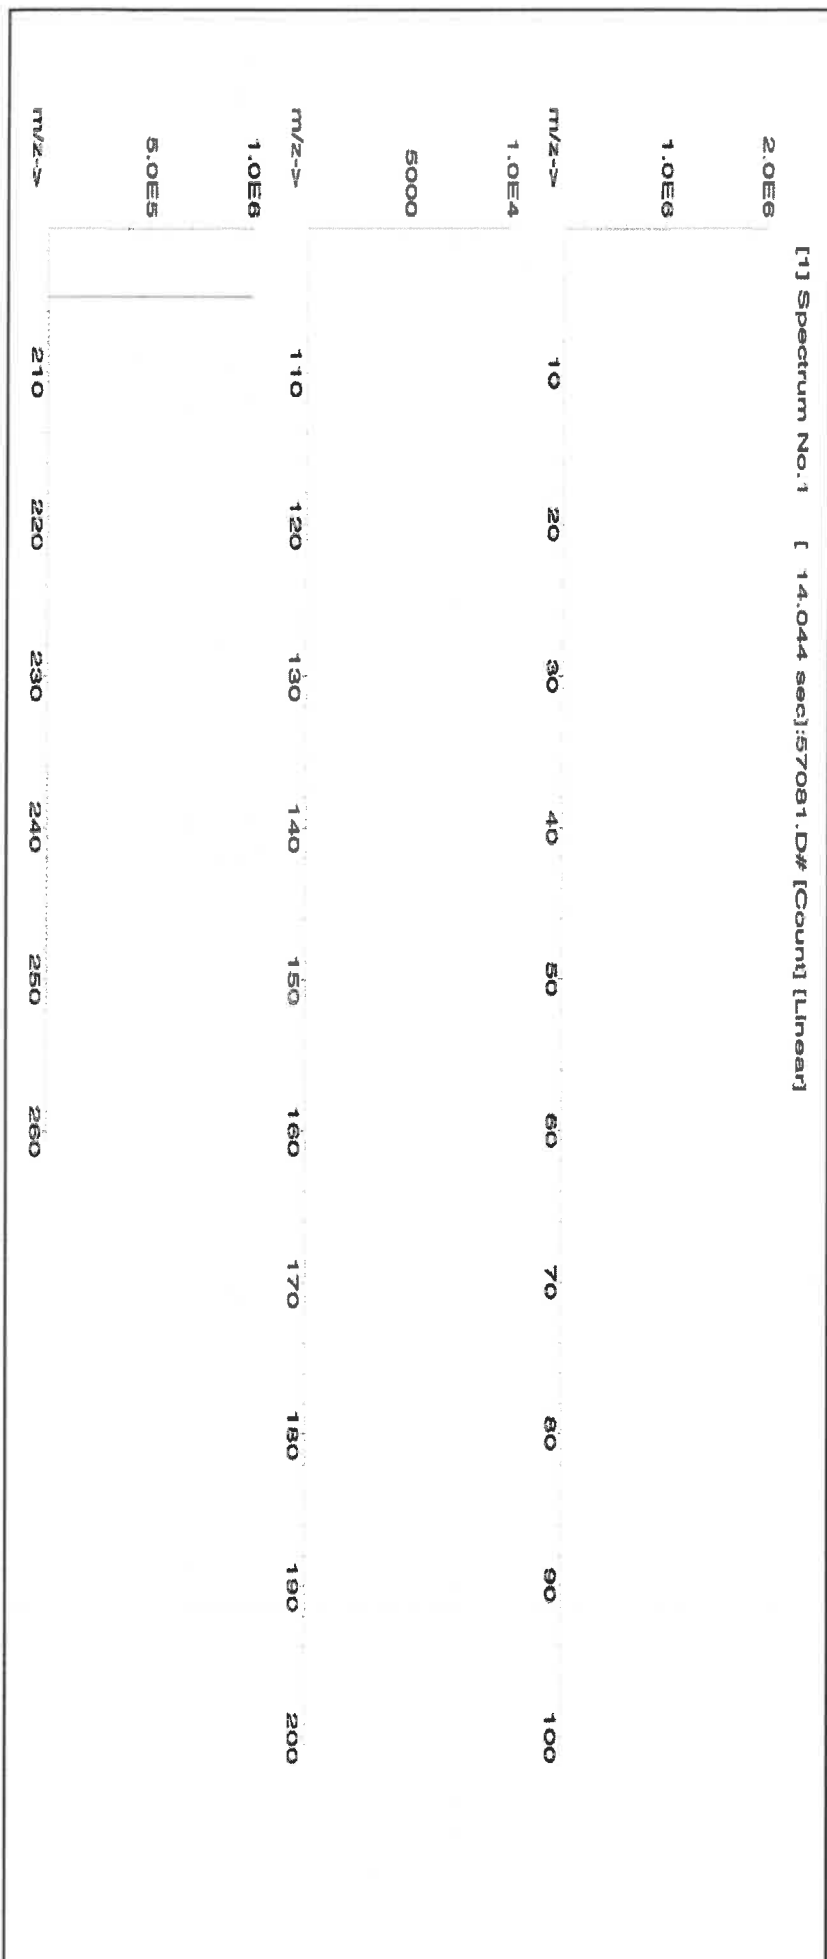



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Sc	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	T	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Rb	<0.02	Na	<0.2	Tm	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Ru	<0.02	Sr	<0.02	Sn	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	S	<0.02	Ti	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Se	<0.02	Ta	<0.02			Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



Certified Reference Material CRM

M6021



CERTIFIED WEIGHT REPORT:

Part Number: 57023
Lot Number: 062424
Description: Vanadium (V)

Lot # 24002546
Solvent: Nitric Acid

<i>Aleah O Brady</i>	
Formulated By:	Aleah O Brady
Reviewed By:	<i>Pedro L. Rantas</i>
	Pedro L. Rantas
	062424

Expiration Date: 062427
Recommended Storage: Ambient (20 °C)
Nominal Concentration (µg/mL): 1000
NIST Test Number: 6UTB


2.0% 40.0 (mL) Nitric Acid

Volume shown below was diluted to (mL): 2000.3

5E-05 Balance Uncertainty
0.06 Flask Uncertainty

Compound	SDS Information										
	Expanded									NIST SRM	
	Part Number	Lot Number	Dilution Factor	Initial Vol. (mL)	Uncertainty Pipette (mL)	Nominal Conc. (µg/mL)	Initial Conc. (µg/mL)	Final Conc. (µg/mL)	Uncertainty +/- (µg/mL)		
									(Solvent Safety Info. On Attached pg.)	CAS#	
										OSHA PEL (TWA)	LD50

[1] Spectrum No.1 [34.243 sec]:58023.D# [Count] [Linear]

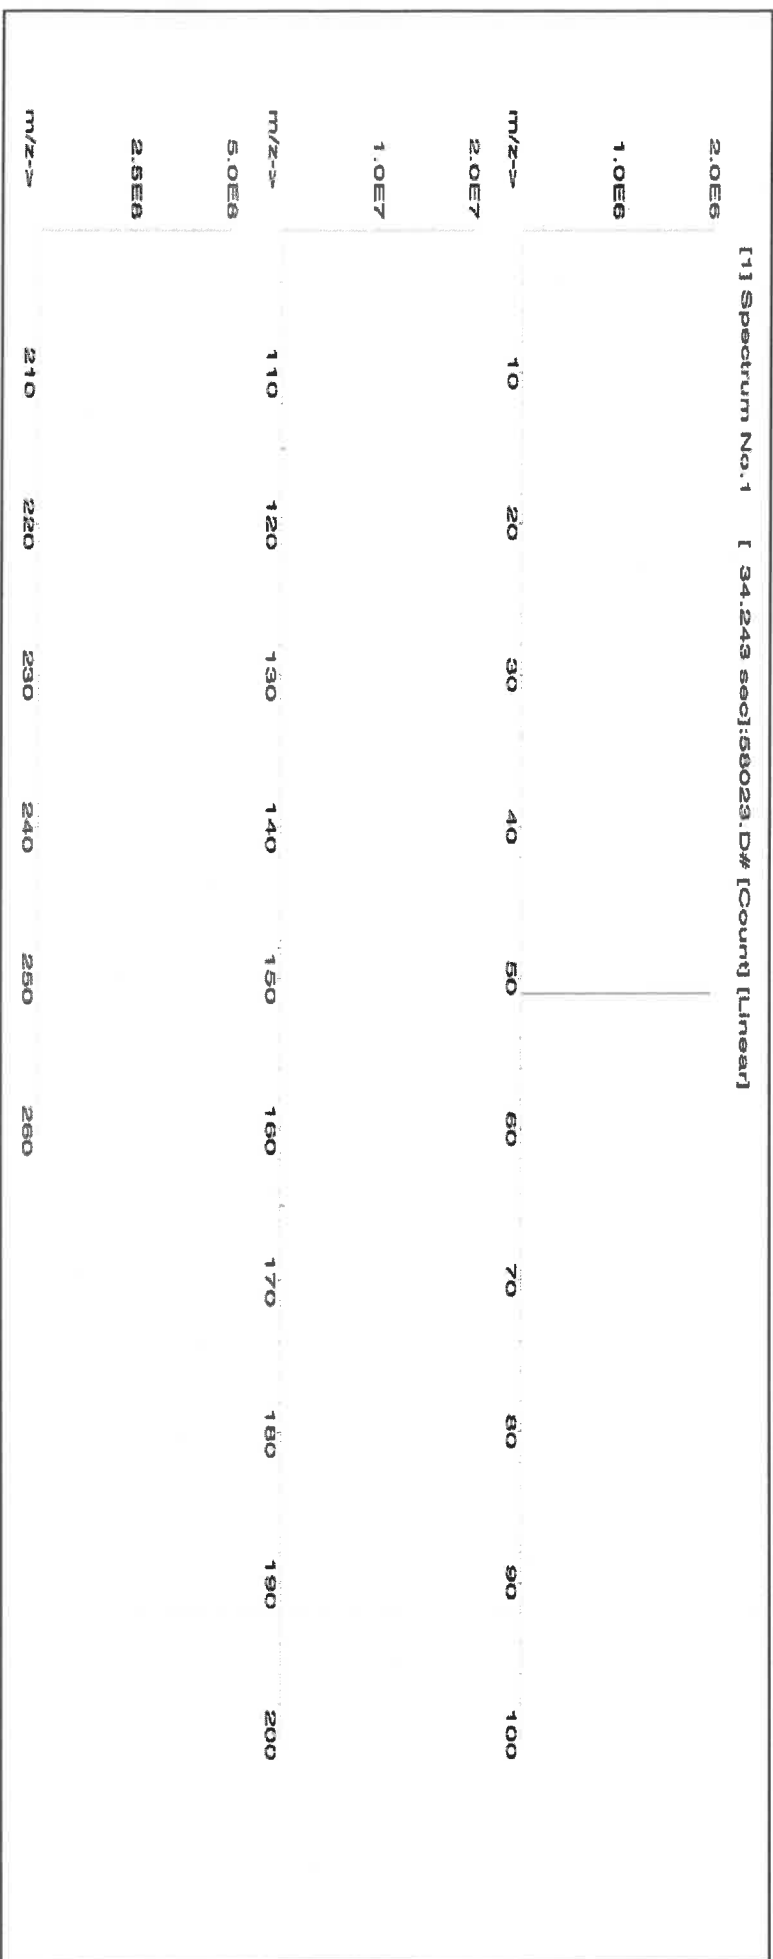



Instrumental Analysis by Inductively Coupled Plasma Mass Spectrometry (ICP-MS):

Trace Metals Verification by ICP-MS (µg/mL)

Al	<0.02	Cd	<0.02	Dy	<0.02	Hf	<0.02	Li	<0.02	Ni	<0.02	Pt	<0.02	Se	<0.2	Tb	<0.02	W	<0.02
Sb	<0.02	Ca	<0.2	Er	<0.02	Ho	<0.02	Lu	<0.02	Nb	<0.02	Re	<0.02	Si	<0.02	Te	<0.02	U	<0.02
As	<0.2	Ce	<0.02	Eu	<0.02	In	<0.02	Mg	<0.01	Os	<0.02	Rh	<0.02	Ag	<0.02	Tl	<0.02	V	<0.02
Ba	<0.02	Cs	<0.02	Gd	<0.02	Ir	<0.02	Mn	<0.02	Pd	<0.02	Ru	<0.02	Na	<0.2	Th	<0.02	Yb	<0.02
Be	<0.01	Cr	<0.02	Ga	<0.02	Fe	<0.2	Hg	<0.2	P	<0.02	Sr	<0.02	S	<0.02	Tm	<0.02	Y	<0.02
Bi	<0.02	Co	<0.02	Ge	<0.02	La	<0.02	Mo	<0.02	Pt	<0.02	Sm	<0.02	Ta	<0.02	Sn	<0.02	Zn	<0.02
B	<0.02	Cu	<0.02	Au	<0.02	Pb	<0.02	Nd	<0.02	K	<0.2	Sc	<0.02			Ti	<0.02	Zr	<0.02

(T) = Target analyte

Physical Characterization:

Homogeneity: No heterogeneity was observed in the preparation of this standard.

Certified by:

- * The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- * Purified acids, 18.2 megohm deionized water, calibrated Class A glassware and the highest purity raw materials are used in the preparation of all standards.
- * All standard containers are meticulously cleaned prior to use.
- * Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- * Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- * All Standards should be stored with caps tight and under appropriate laboratory conditions.
- * Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, D.C. (1994).



SHIPPING DOCUMENTS

- 1
- 2
- 3
- 4
- 5
- 6
- 7
- 8
- 9
- 10
- 11
- 12
- 13
- 14
- 15
- 16
- 17

CHEMTECH CHAIN OF CUSTODY RECORD		284 Sheffield Street, Mountainside, NJ 07092 (908) 789-8900 Fax: (908) 78-8922 www.chemtech.net		Chemtech Project Number: 22805															
COC Number:																			
CLIENT INFORMATION		PROJECT INFORMATION		BILLING INFORMATION															
COMPANY: Tetra Tech		PROJECT NAME: NWIRP Bethpage		BILL TO:		PO#													
ADDRESS: 4433 Corporation Ln, Suite 300		PROJECT #: 112G08005-WE13 LOCATION: RW8		ADDRESS:															
CITY: Virginia Beach STATE: VA ZIP: 23462		PROJECT MANAGER: Ernie Wu		CITY:		STATE: ZIP:													
ATTENTION: Ernie Wu		E-MAIL: ernie.wu@tetratech.com		ATTENTION:		PHONE:													
PHONE: 757-466-4901 FAX: 757-461-4148		PHONE: 757-466-4901 FAX: 757-461-4148		ANALYSIS															
DATA TURNAROUND INFORMATION		DATA DELIVERABLE INFORMATION		1,4-Dioxane SW846 8270 SIM Iron, Total TSS TDS 1 2 3 4 5 6 7 8 9															
FAX: 10 DAYS* HARD COPY: 10 DAYS* EDD: 10 DAYS* * TO BE APPROVED BY CHEMTECH STANDARD TURNAROUND TIME IS 10 BUSINESS DAYS		☐ RESEULTS ONLY ☐ USEPA CLP ☐ RESULTS + QC ☐ New York State ASP "B" ☐ New Jersey REDUCED ☐ New York State ASP "A" ☐ New Jersey CLP ☐ Other _____ ☐ EDD Format _____																	
CHEMTECH SAMPLE ID		PROJECT SAMPLE IDENTIFICATION		SAMPLE MATRIX		SAMPLE TYPE		SAMPLE COLLECTION		# of Bottles		PRESERVATIVES				COMMENTS			
						COMP GRAB		DATE TIME				1 2 3 4 5 6 7 8 9				Specify Preservatives A-HCl B-HNO3 C-H2SO4 D-NaOH E-ICE F-Other			
1.		RW8-SP100-20250807		GW		X		8/7/25 13:05		2		X X				pH 1.3			
2.		RW8-SP303-20250807		GW		X		8/7/25 13:13		4		X X X X				pH 1.3			
3.																			
4.																			
5.																			
6.																			
7.																			
8.																			
9.																			
10.																			
SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE PROSESSION INCLUDING COURIER DELIVERY																			
RELINQUISHED BY SAMPLER		DATE/TIME		RECEIVED BY		Conditions of bottles or coolers at receipt: ☐ Compliant ☐ Non Compliant ☐ Cooler Temp 2.1C MeOH extraction requires an additional 4oz. Jar for percent solid Comments:													
1. [Signature]		8/7/25/2025		1. [Signature]															
RELINQUISHED BY		DATE/TIME		RECEIVED BY															
2. [Signature]		8/8/25		2. [Signature]															
RELINQUISHED BY		DATE/TIME		RECEIVED FOR LAB BY															
3. [Signature]				3. [Signature]															
Page _____ of _____						SHIPPED VIA: CLIENT: ☐ Hand Delivered ☐ Overnight CHEMTECH: ☐ Picked Up ☐ Overnight						Shipment Complete ☐ YES ☐ NO							
WHITE - CHEMTECH COPYFOR RETURN TO CLIENT YELLOW - CHEMTECH COPY PINK - SAMPLER COPY																			

Laboratory Certification

Certified By	License No.
CAS EPA CLP Contract	68HERH20D0011
Connecticut	PH-0830
DOD ELAP (ANAB)	L2219
Maine	2024021
Maryland	296
New Hampshire	255424 Rev 1
New Jersey	20012
New York	11376
Pennsylvania	68-00548
Soil Permit	525-24-234-08441
Texas	T104704488