
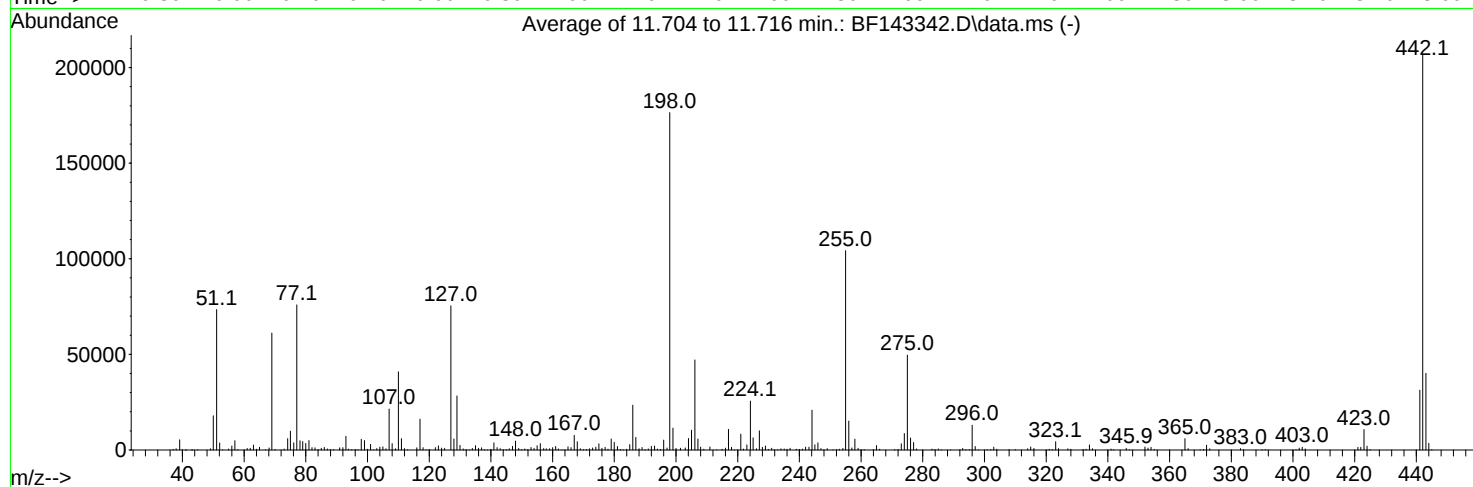


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081225\
Data File : BF143342.D
Acq On : 12 Aug 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 12 13:25:39 2025

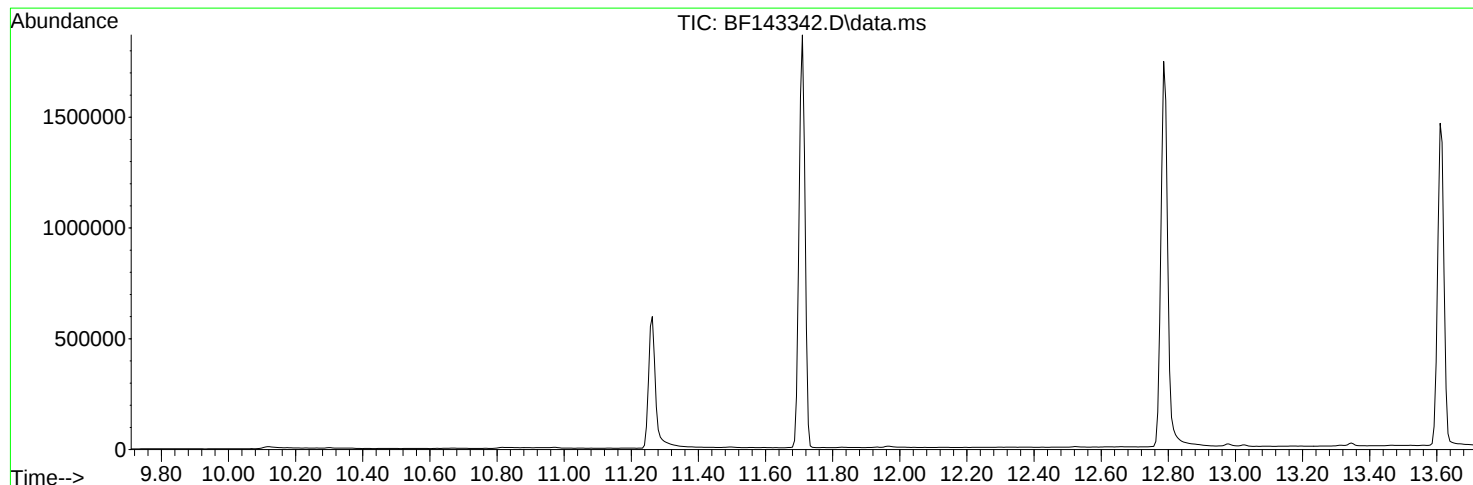

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.8	1075	PASS
69	69	100	100	100.0	61205	PASS
70	69	0.00	2	0.5	326	PASS
197	198	0.00	2	0.6	1092	PASS
198	198	100	100	100.0	176469	PASS
199	198	5	9	6.5	11438	PASS
365	198	1	100	3.4	5927	PASS
441	443	0.01	150	77.9	31269	PASS
442	442	100	100	100.0	206464	PASS
443	442	15	24	19.4	40120	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/12/2025	BNA_F	<u>BF143342.D</u>
Compound Name	Response	Retention Time
DDT	266385	13.61
DDD	3780	13.345
DDE	3356	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7136	273521	2.61

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081225\
Data File : BF143342.D
Acq On : 12 Aug 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 13:28:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

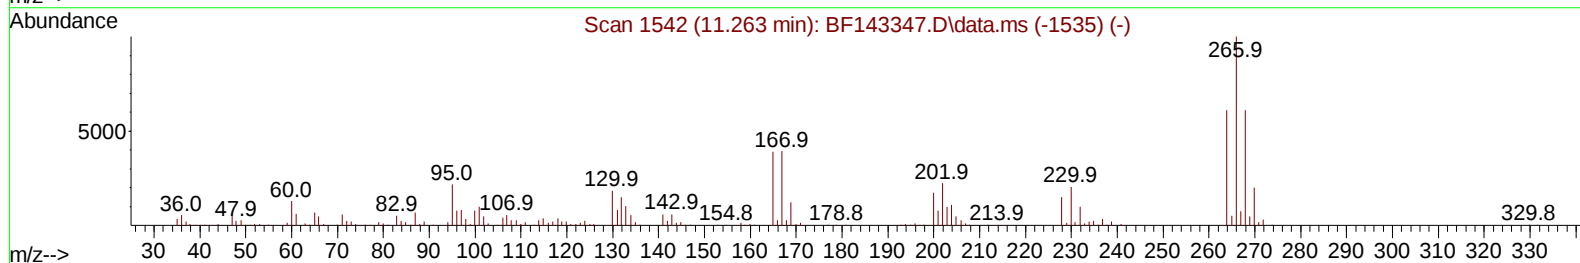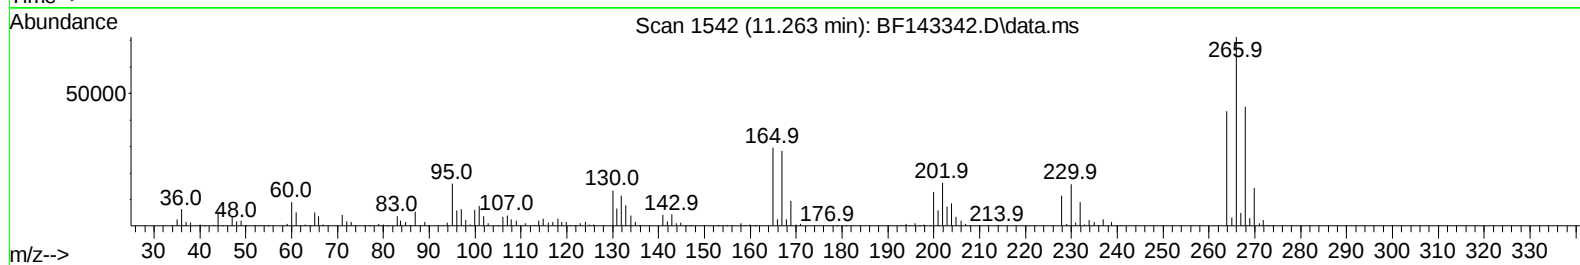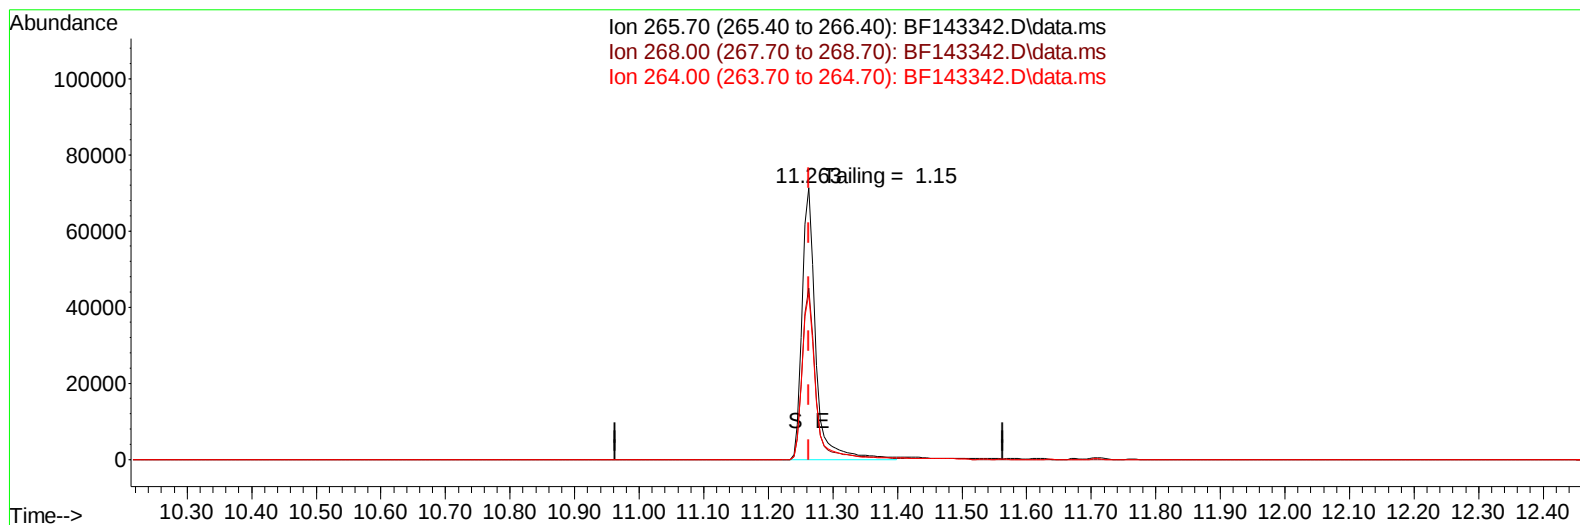

TIC: BF143342.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.000) 127995.01 ng




response 106759

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.14
264.00	61.00	60.85
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081225\
Data File : BF143342.D
Acq On : 12 Aug 2025 08:34
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 12 13:28:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

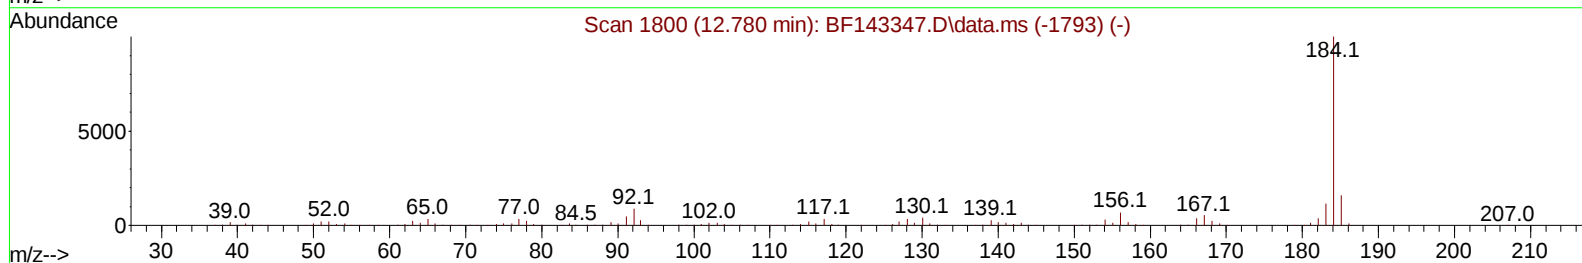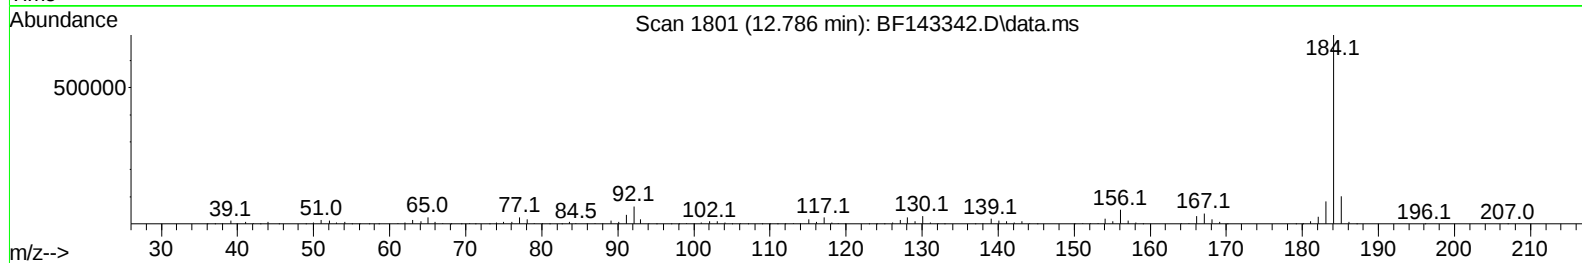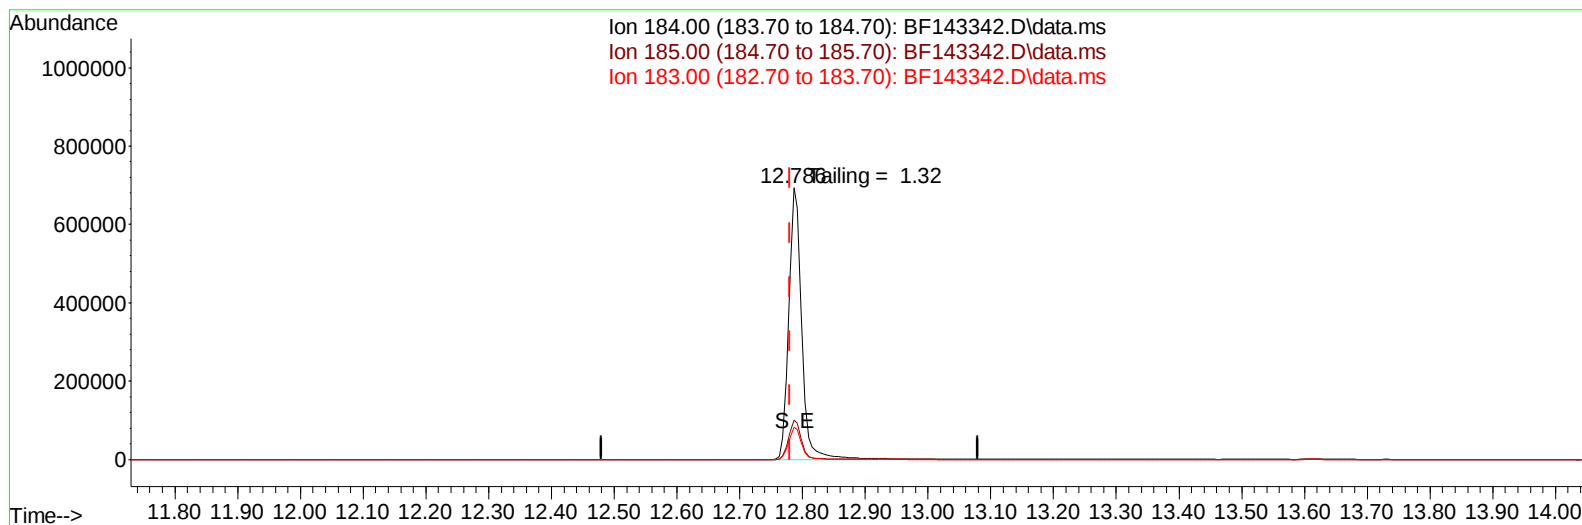

TIC: BF143342.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 1006924

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.63
183.00	11.60	11.87
0.00	0.00	0.00