
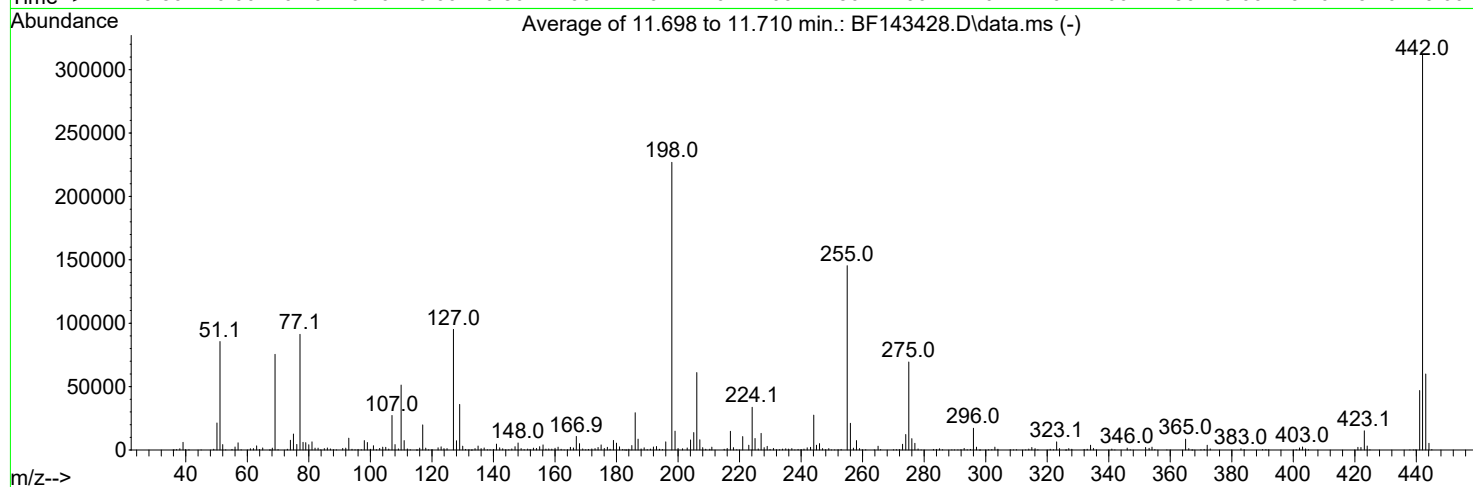


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081825\
Data File : BF143428.D
Acq On : 18 Aug 2025 08:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 18 04:40:19 2025

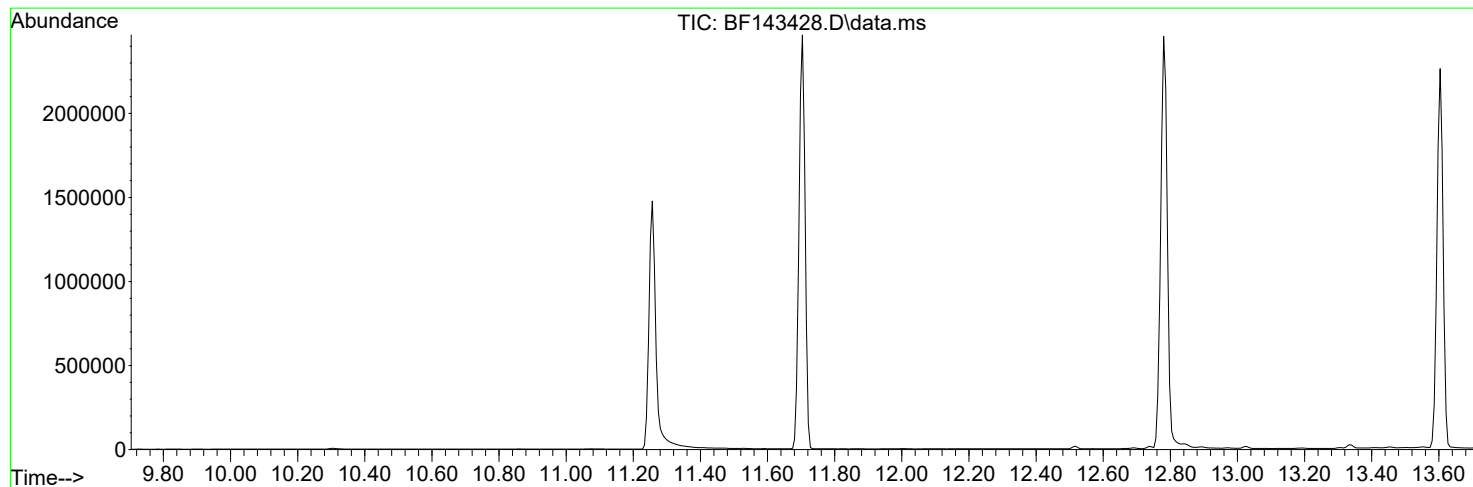

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1609

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	2.0	1498	PASS
69	69	100	100	100.0	75440	PASS
70	69	0.00	2	0.5	389	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	226987	PASS
199	198	5	9	6.6	14870	PASS
365	198	1	100	3.8	8602	PASS
441	443	0.01	150	78.5	46984	PASS
442	442	100	100	100.0	311424	PASS
443	442	15	24	19.2	59888	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/18/2025	BNA_F	<u>BF143428.D</u>
Compound Name	Response	Retention Time
DDT	555192	13.604
DDD	7876	13.333
DDE	2112	12.969
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9988	565180	1.77

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081825\
Data File : BF143428.D
Acq On : 18 Aug 2025 08:37
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 12:01:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

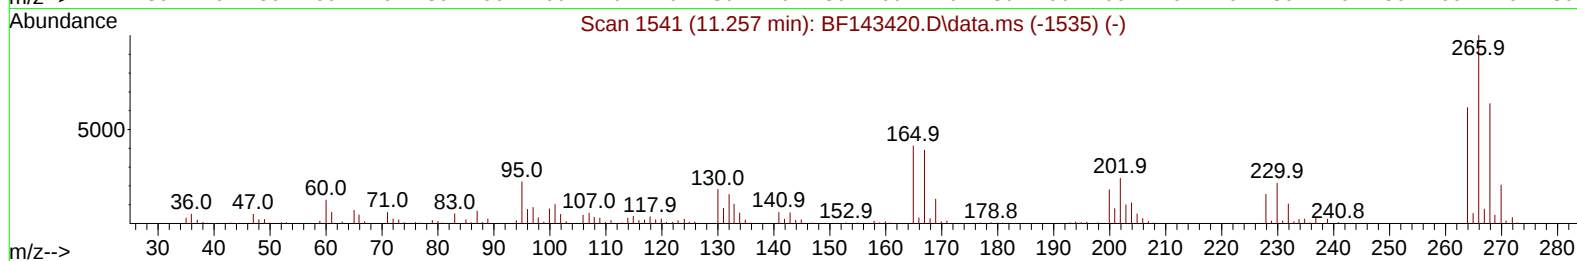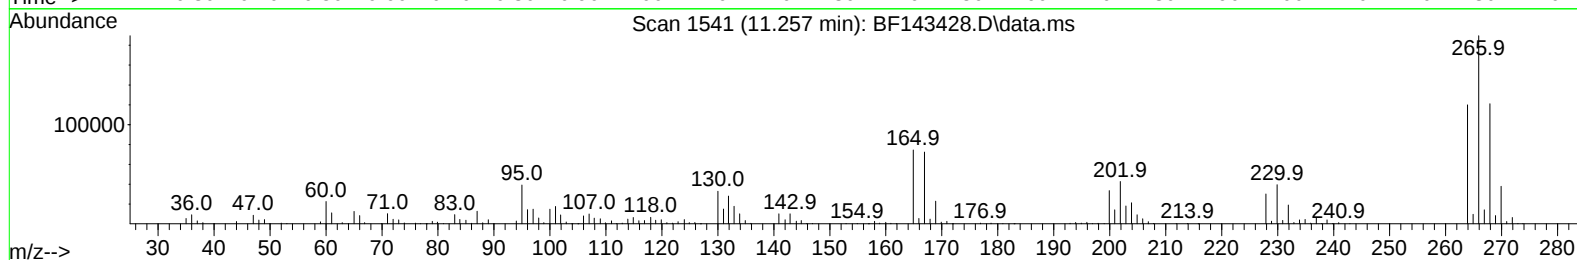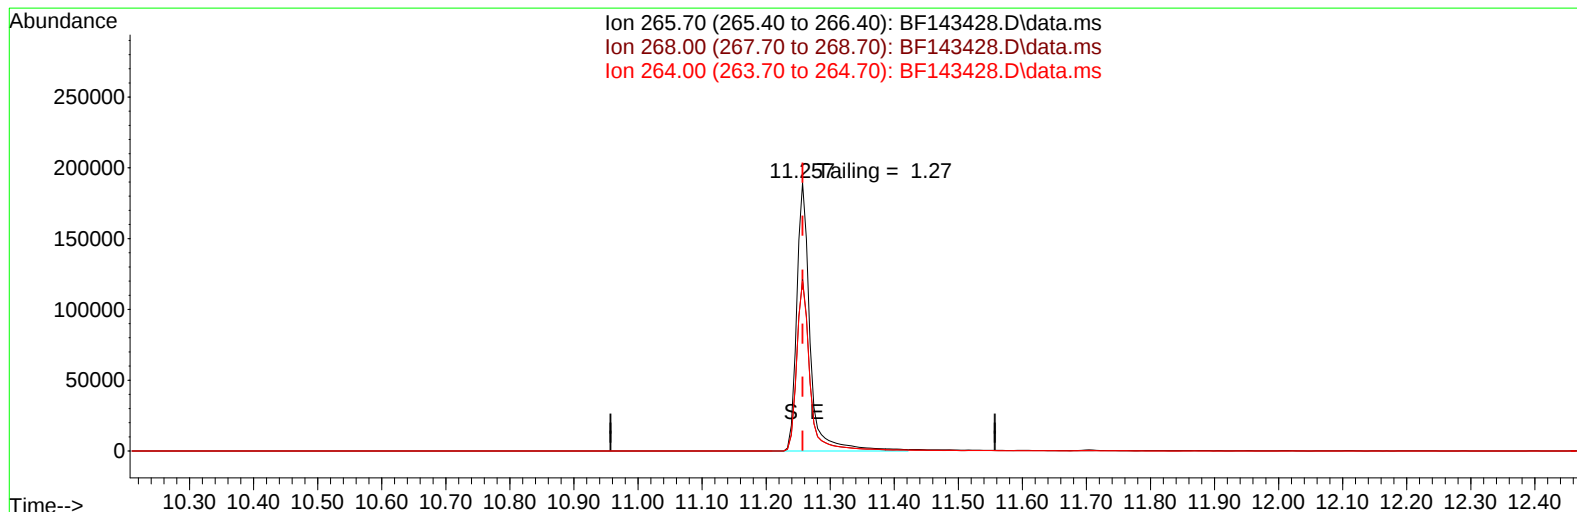

TIC: BF143428.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 817352.89 ng

response 279770

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.80	63.84
264.00	61.60	63.23
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 18 12:01:43 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 18 04:40:19 2025
Response via : Initial Calibration

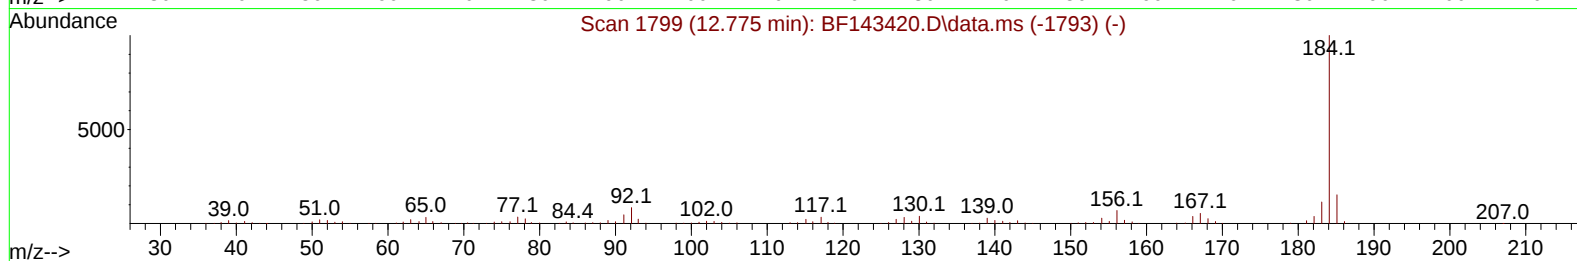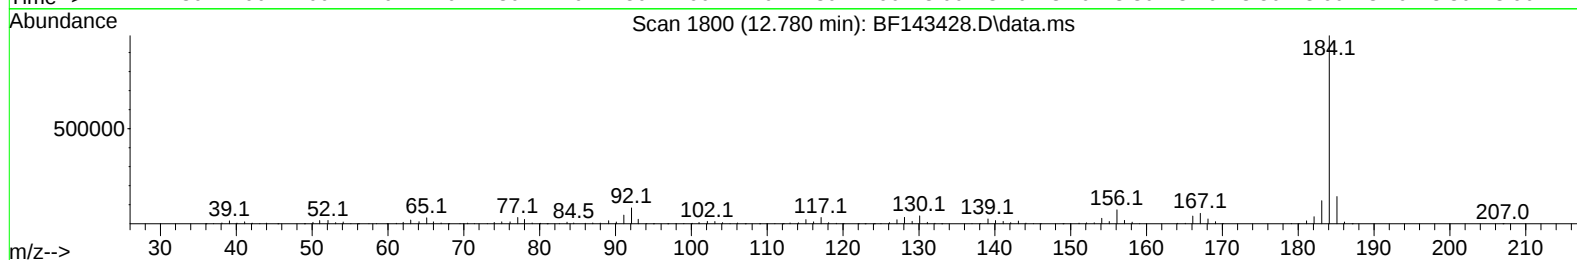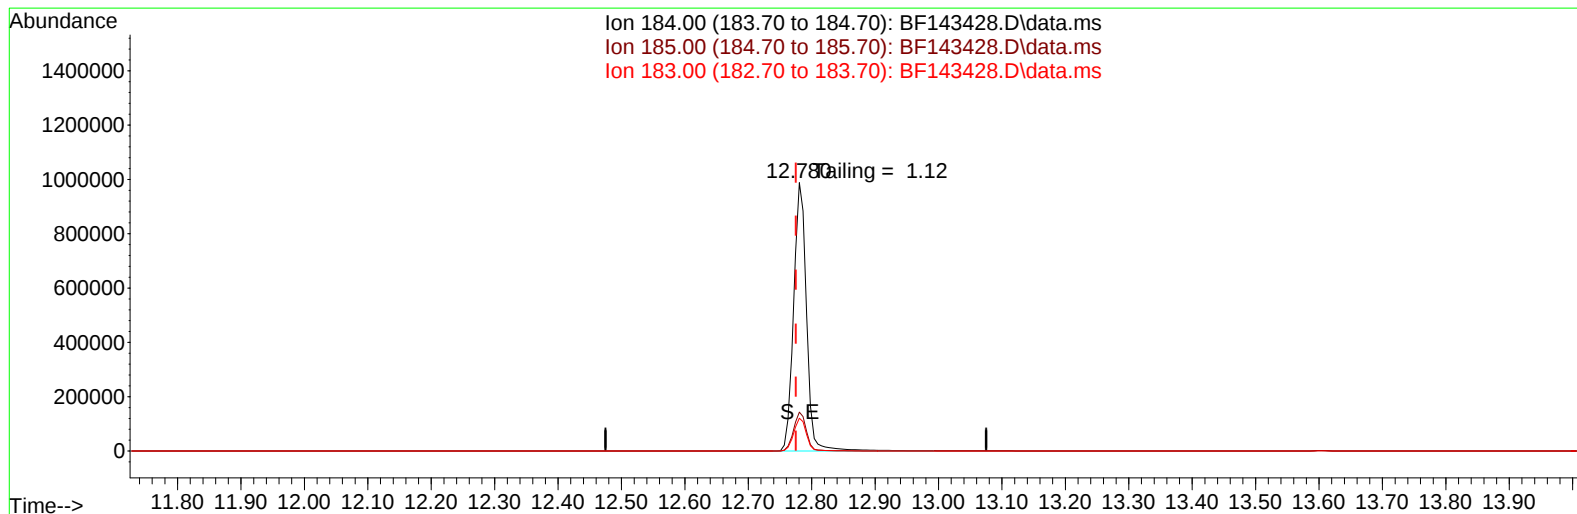

TIC: BF143428.D\data.ms

(77) Benzidine

12.780min (+ 0.005) 0.00 ng

response 1404146

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.49
183.00	11.50	12.23
0.00	0.00	0.00