

SOP ID: M625.1-BNA-21

Clean Up SOP #: N/A

Matrix : Water

Weigh By: N/A

Balance check: N/A

Balance ID: N/A

pH Strip Lot#: E3880

Extraction By: RS

Filter By: RS

pH Meter ID: N/A

Hood ID: 4,6,7

Extraction Start Date : 08/14/2025

Extraction Start Time : 10:35

Extraction End Date : 08/14/2025

Extraction End Time : 15:25

Concentration By: EH

Supervisor By : RUPESH

Extraction Method: ☒ Separatory Funnel

☐ Continious Liquid/Liquid

☐ Sonication

☐ Waste Dilution

☐ Soxhlet

Standard Name	MLS USED	Concentration ug/mL	STD REF. # FROM LOG
Spike Sol 1	1.0ML	50/100 PPM	SP6849
Surrogate	1.0ML	100 PPM	SP6759
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A
N/A	N/A	N/A	N/A

Chemical Used	ML/SAMPLE USED	Lot Number
Methylene Chloride	N/A	E3954
Baked Na2SO4	N/A	EP2632
10N NaoH	N/A	EP2609
H2SO4 1:1	N/A	EP2610
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A
N/A	N/A	N/A

Extraction Conformance/Non-Conformance Comments:

1.5 ML Vial lot# 2210443. pH Adjusted<2 with 1:1 H2SO4 & >11 with10N NaOH.

KD Bath ID: Water bath -01

Envap ID: NEVAP-02

KD Bath Temperature: 60 °C


Envap Temperature: 40 °C

Date / Time	Prepped Sample Relinquished By/Location	Received By/Location
8/14/25 15:30	RS (Ext Lab) Preparation Group	RL/svoc Analysis Group

Analytical Method: M625.1-BNA-21

Concentration Date: 08/14/2025

Sample ID	Client Sample ID	Test	g / (mL)	PH	Surr/Spike By:		Final Vol. (mL)	JarID	Comments	Prep Pos
					AddedBy	VerifiedBy				
PB169256BL	SBLK256	SVOCMS Group1	1000	6	RUPESH	ritesh	1			SEP-1
PB169256BS	SLCS256	SVOCMS Group1	1000	6	RUPESH	ritesh	1			2
PB169256BS D	SLCSD256	SVOCMS Group1	1000	6	RUPESH	ritesh	1			3
Q2811-02	EFF-WASTE WATER	SVOCMS Group1	960	6	RUPESH	ritesh	1	C		4

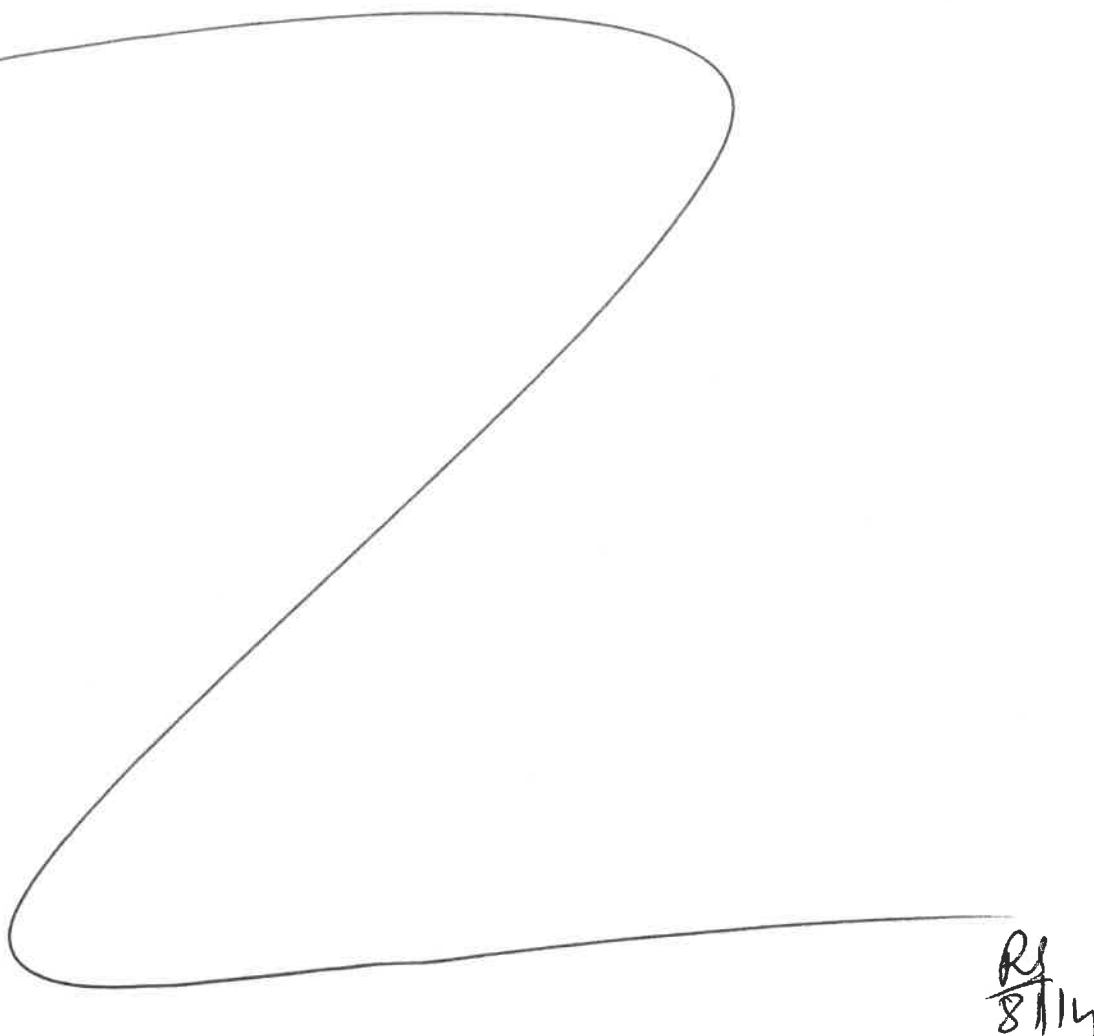

Rs
8/14