


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143376.D
Acq On : 14 Aug 2025 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Aug 12 13:25:39 2025

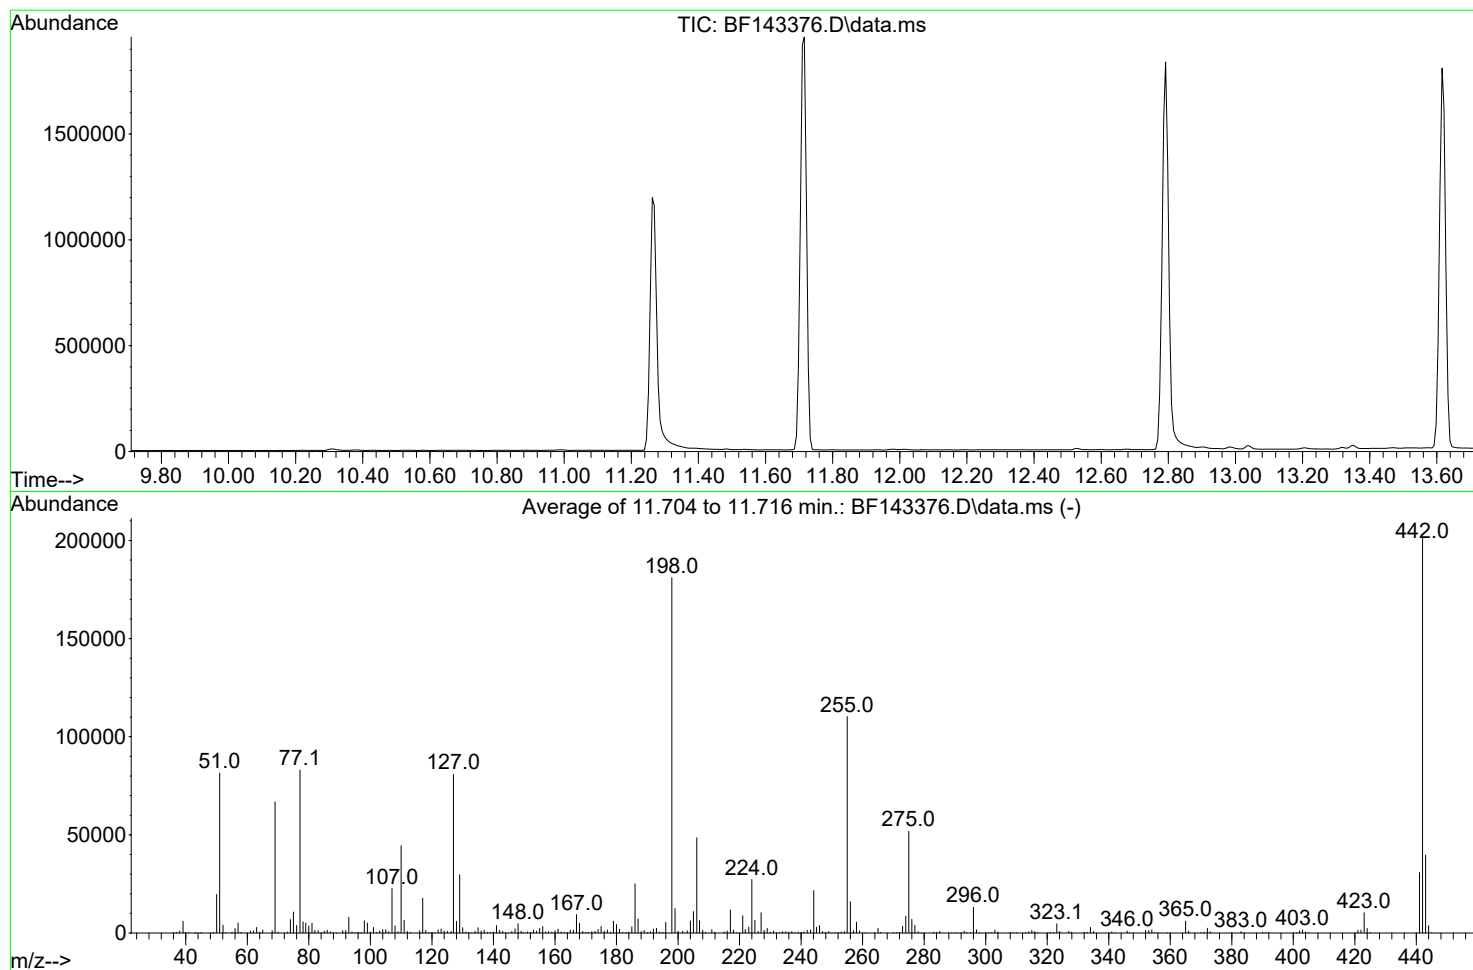

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.8	1210	PASS
69	69	100	100	100.0	66827	PASS
70	69	0.00	2	0.6	419	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	180963	PASS
199	198	5	9	6.9	12493	PASS
365	198	1	100	3.3	6022	PASS
441	443	0.01	150	77.7	30860	PASS
442	442	100	100	100.0	201176	PASS
443	442	15	24	19.8	39741	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/14/2025	BNA_F	<u>BF143376.D</u>
Compound Name	Response	Retention Time
DDT	444870	13.616
DDD	6873	13.351
DDE	3527	12.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10400	455270	2.28

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143376.D
Acq On : 14 Aug 2025 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 12:58:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

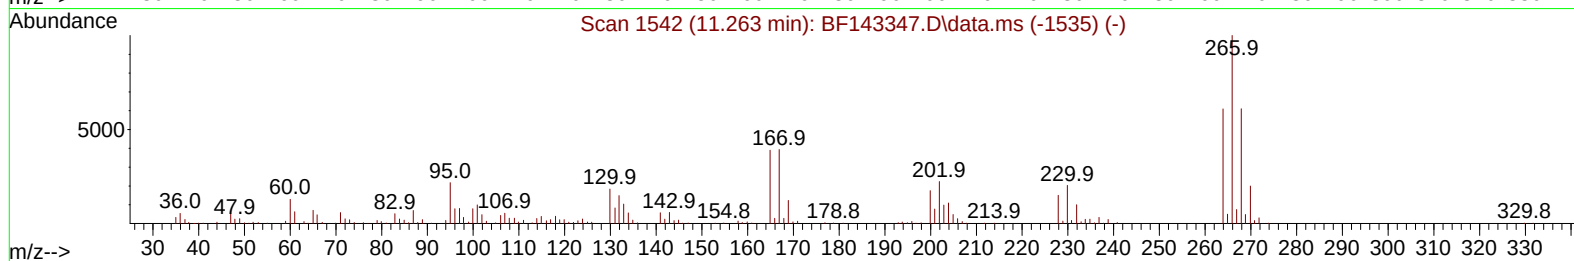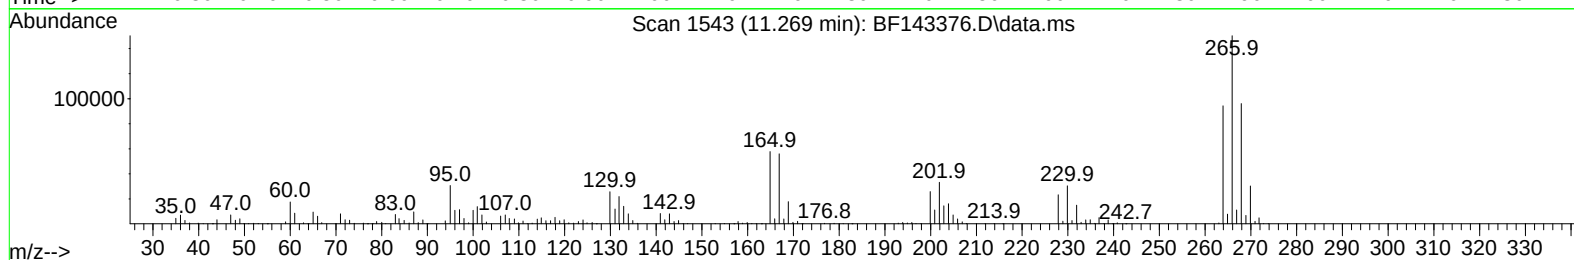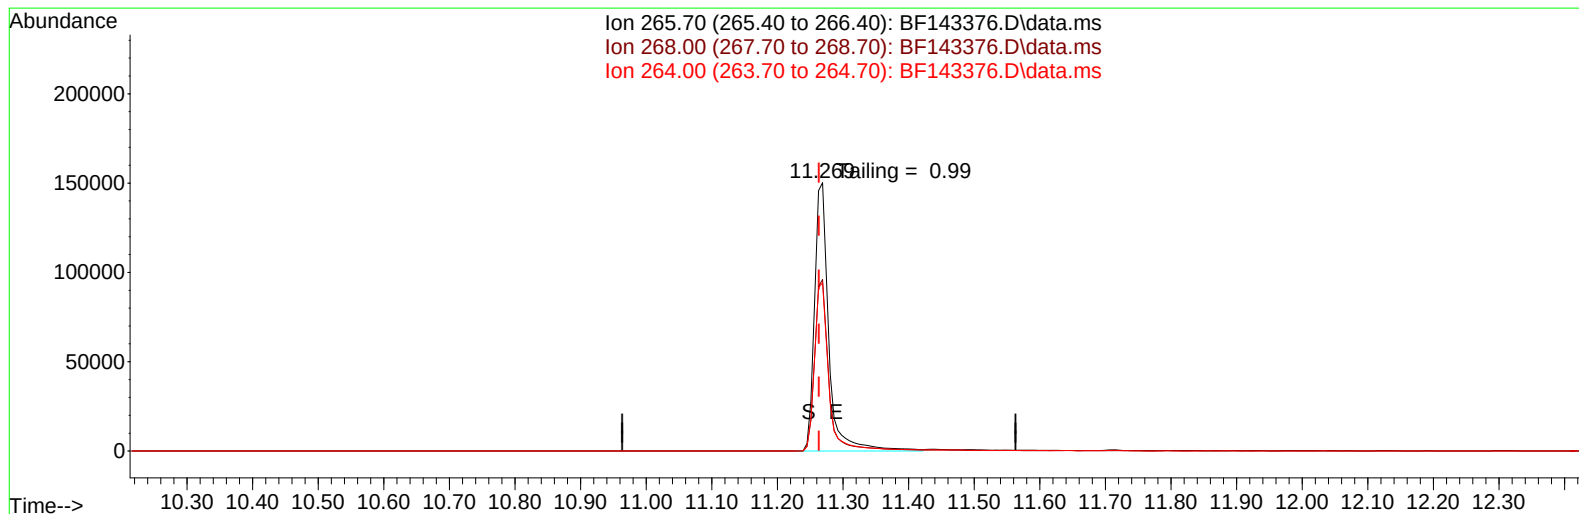

TIC: BF143376.D\data.ms

(70) Pentachlorophenol (C)

11.269min (+ 0.006) 295541.56 ng




response 227255

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.00	63.95
264.00	61.00	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143376.D
Acq On : 14 Aug 2025 11:55
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 14 12:58:39 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration

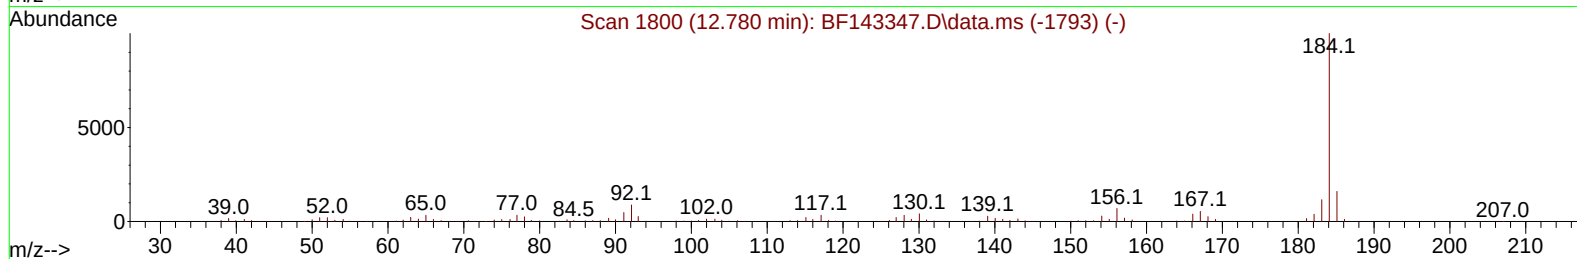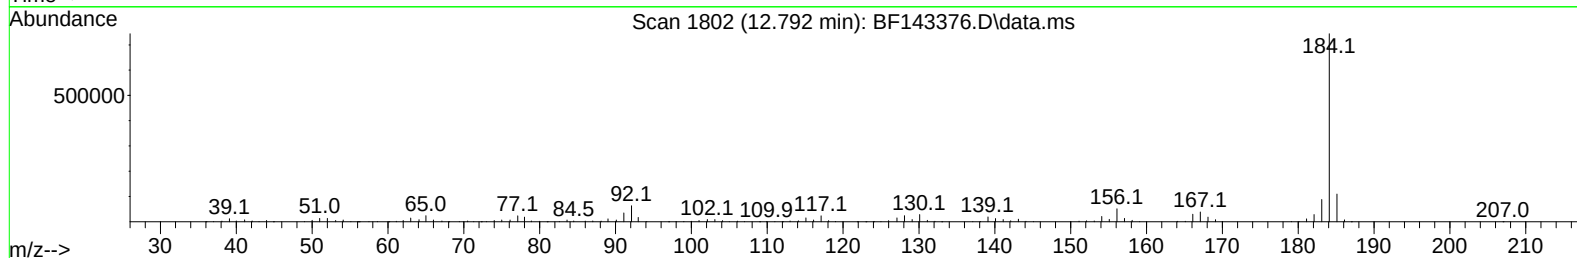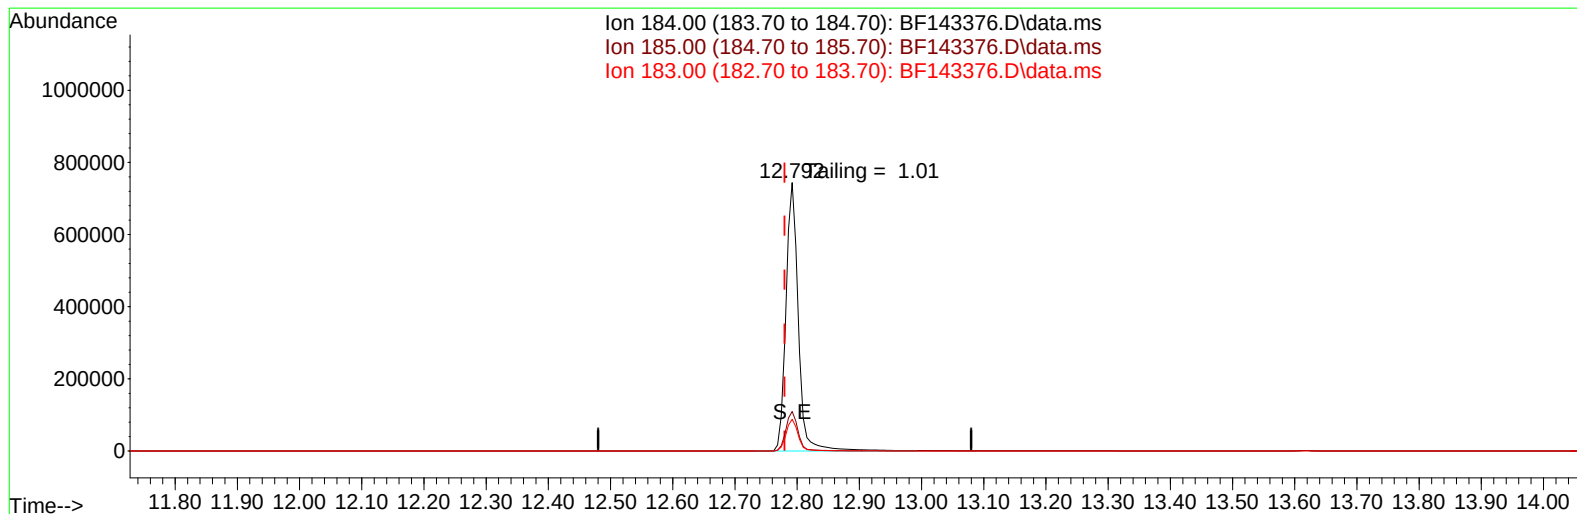

TIC: BF143376.D\data.ms

(77) Benzidine

12.792min (+ 0.012) 0.00 ng

response 1039955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	16.00	14.73
183.00	11.60	11.82
0.00	0.00	0.00