
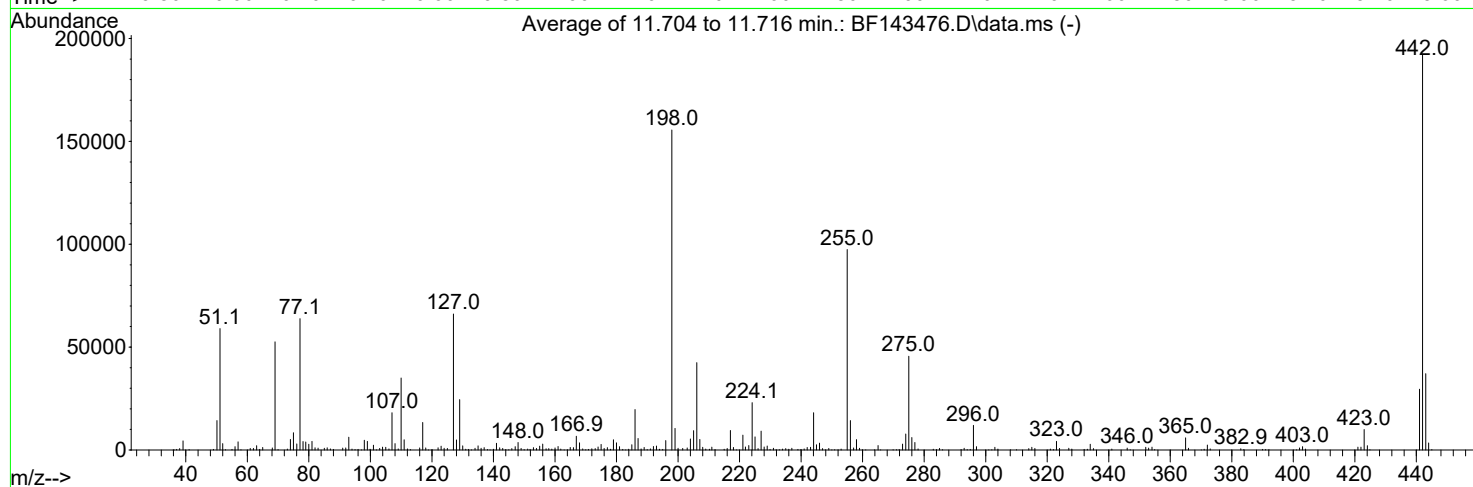


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082025\
Data File : BF143476.D
Acq On : 20 Aug 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 21 06:12:21 2025

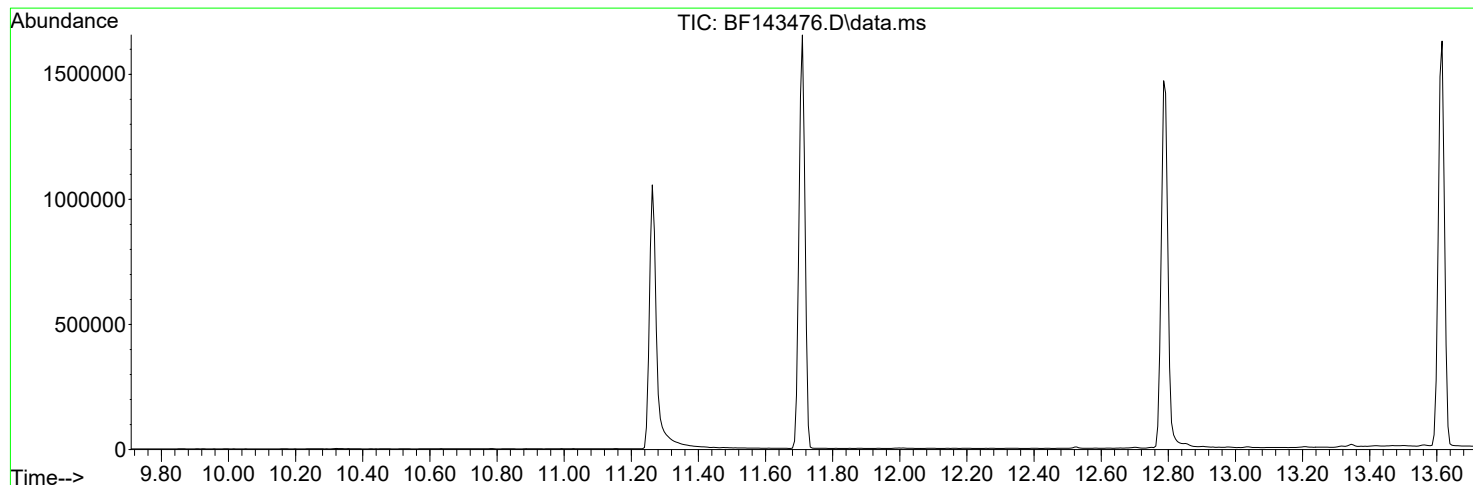

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.9	985	PASS
69	69	100	100	100.0	52563	PASS
70	69	0.00	2	0.5	276	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	155509	PASS
199	198	5	9	6.8	10536	PASS
365	198	1	100	3.8	5904	PASS
441	443	0.01	150	79.6	29523	PASS
442	442	100	100	100.0	191893	PASS
443	442	15	24	19.3	37093	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_F	<u>BF143476.D</u>
Compound Name	Response	Retention Time
DDT	414933	13.616
DDD	4692	13.345
DDE	1143	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5835	420768	1.39

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082025\
Data File : BF143476.D
Acq On : 20 Aug 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 20 16:18:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 20 15:07:46 2025
Response via : Initial Calibration

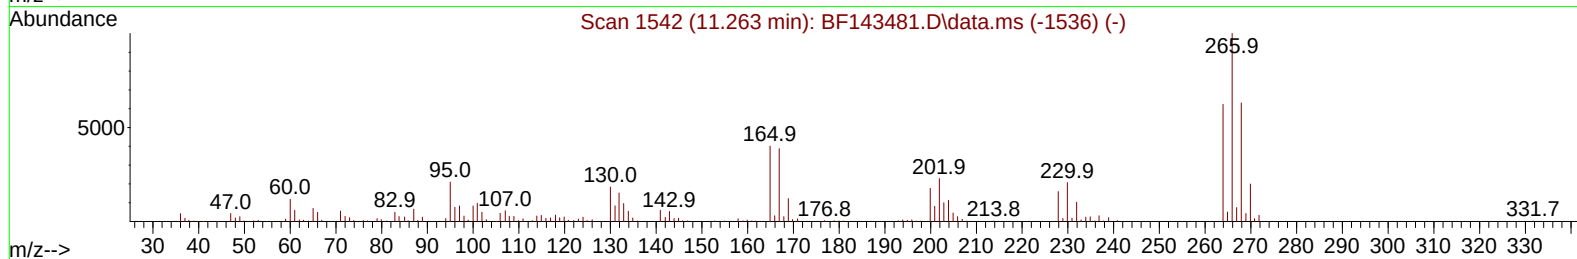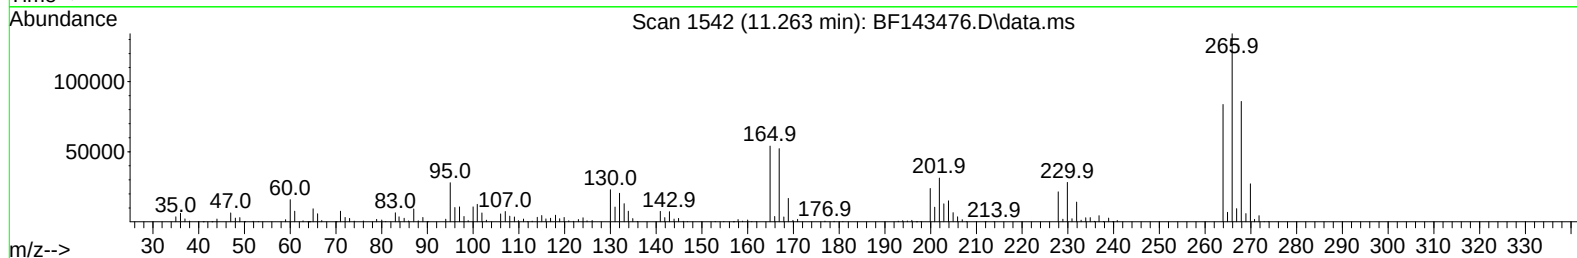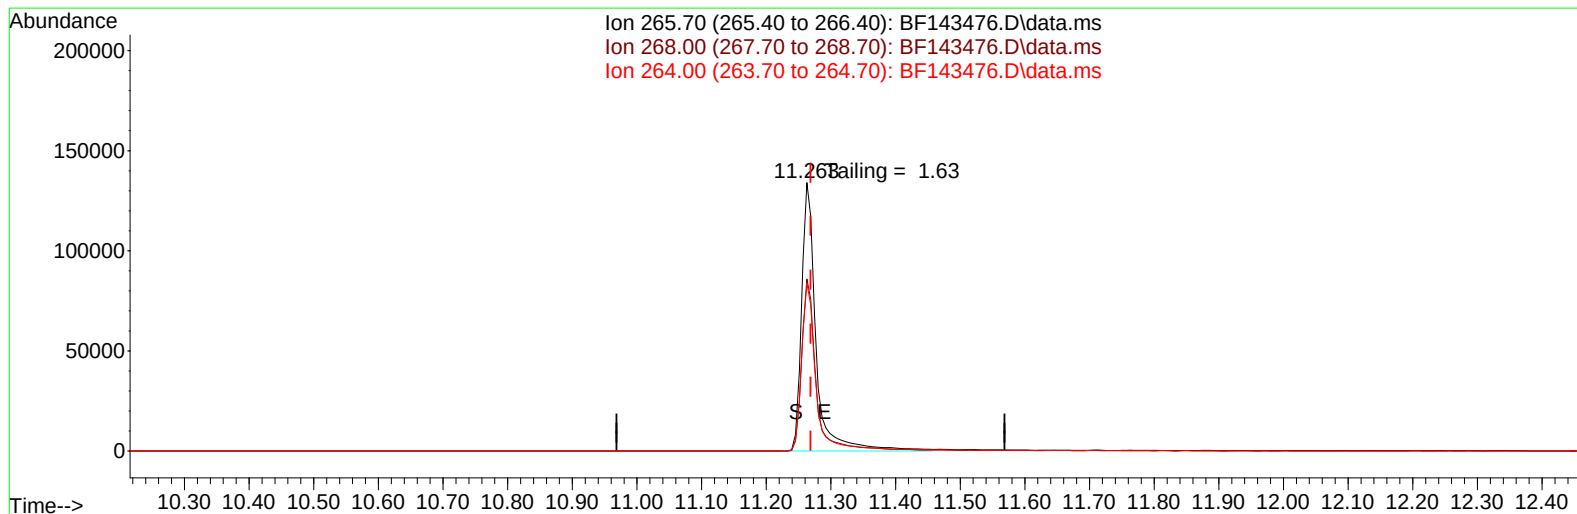

TIC: BF143476.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 46358.19 ng




response 211078

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.07
264.00	62.30	62.45
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082025\
Data File : BF143476.D
Acq On : 20 Aug 2025 10:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 20 16:18:41 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 20 15:07:46 2025
Response via : Initial Calibration

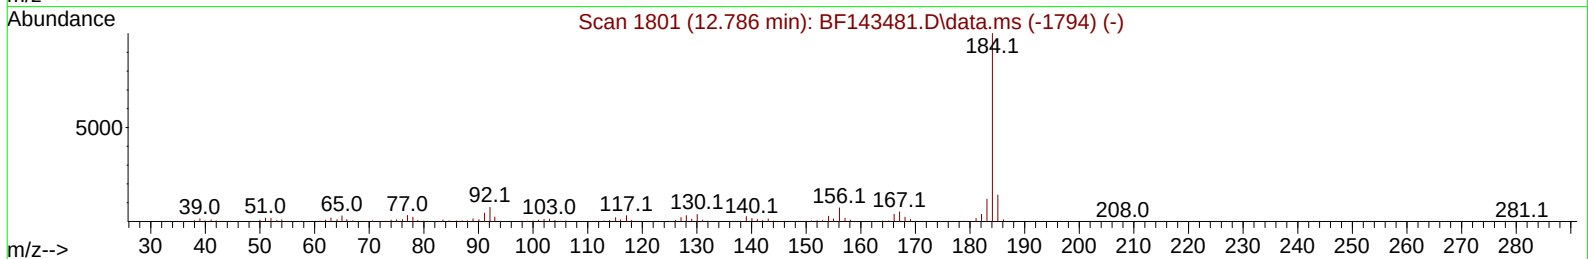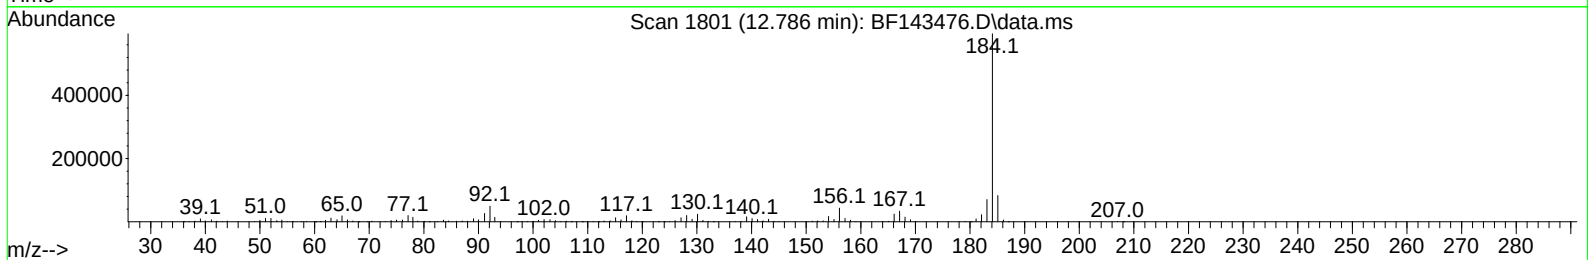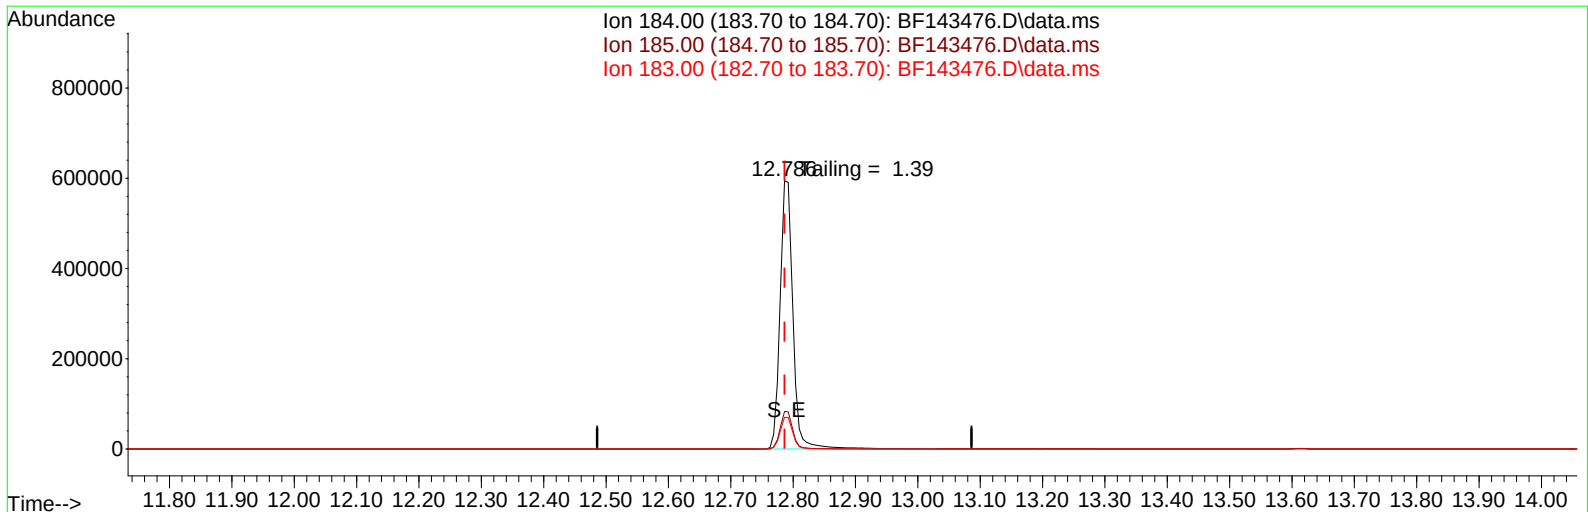

TIC: BF143476.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 0.00 ng

response 857686

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.00
183.00	11.90	11.84
0.00	0.00	0.00