
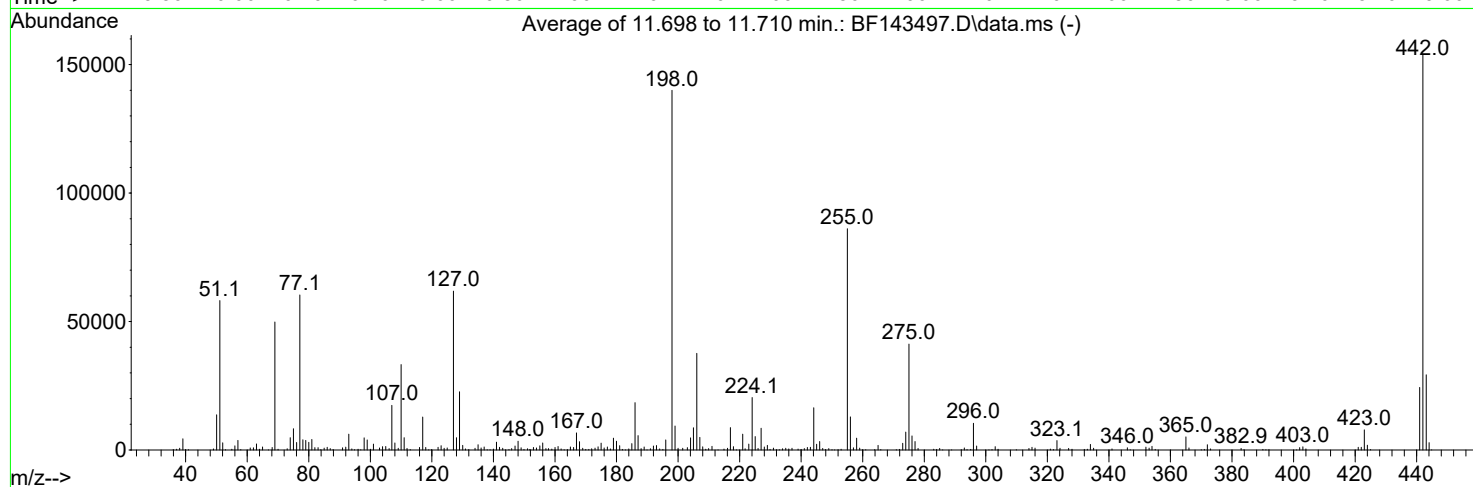


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082025\
 Data File : BF143497.D
 Acq On : 20 Aug 2025 21:36
 Operator : RC/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Aug 21 06:12:21 2025

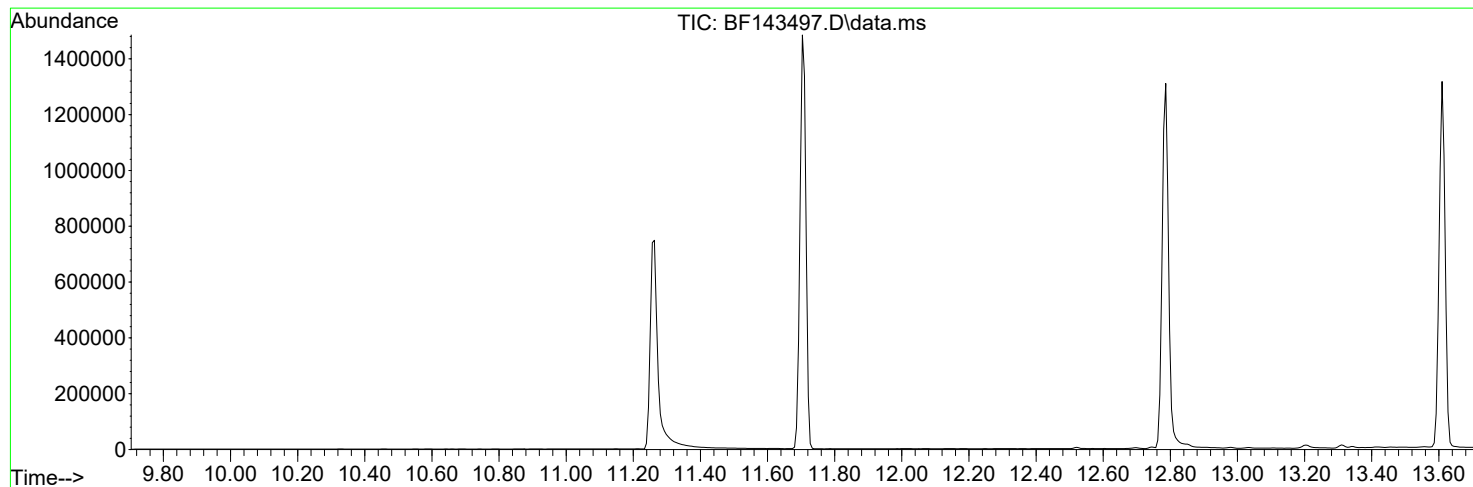

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	2.0	984	PASS
69	69	100	100	100.0	49792	PASS
70	69	0.00	2	0.6	289	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	139989	PASS
199	198	5	9	6.7	9329	PASS
365	198	1	100	3.6	5107	PASS
441	443	0.01	150	83.2	24347	PASS
442	442	100	100	100.0	153672	PASS
443	442	15	24	19.0	29261	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_F	<u>BF143497.D</u>
Compound Name	Response	Retention Time
DDT	312124	13.61
DDD	5317	13.31
DDE	1164	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6481	318605	2.03

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082025\
Data File : BF143497.D
Acq On : 20 Aug 2025 21:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 02:56:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 20 15:07:46 2025
Response via : Initial Calibration

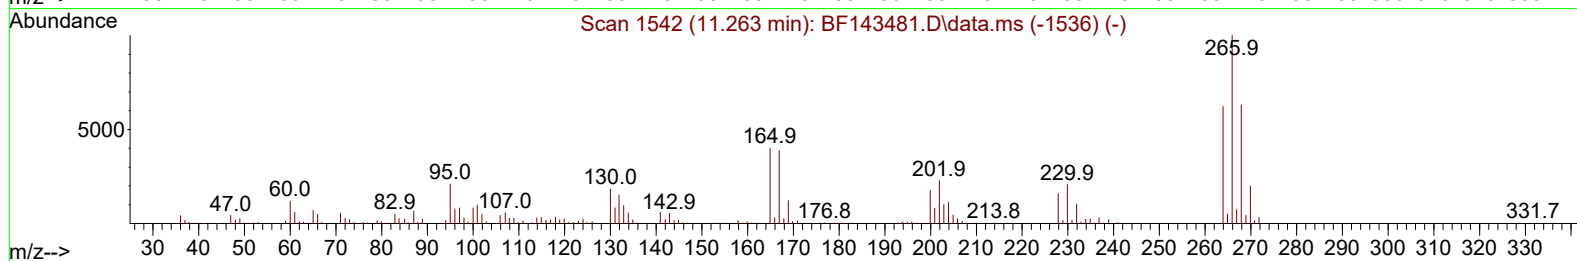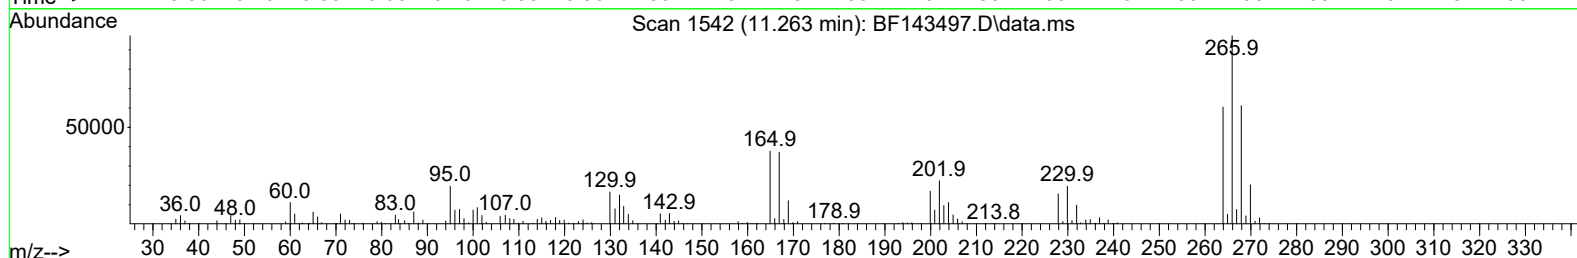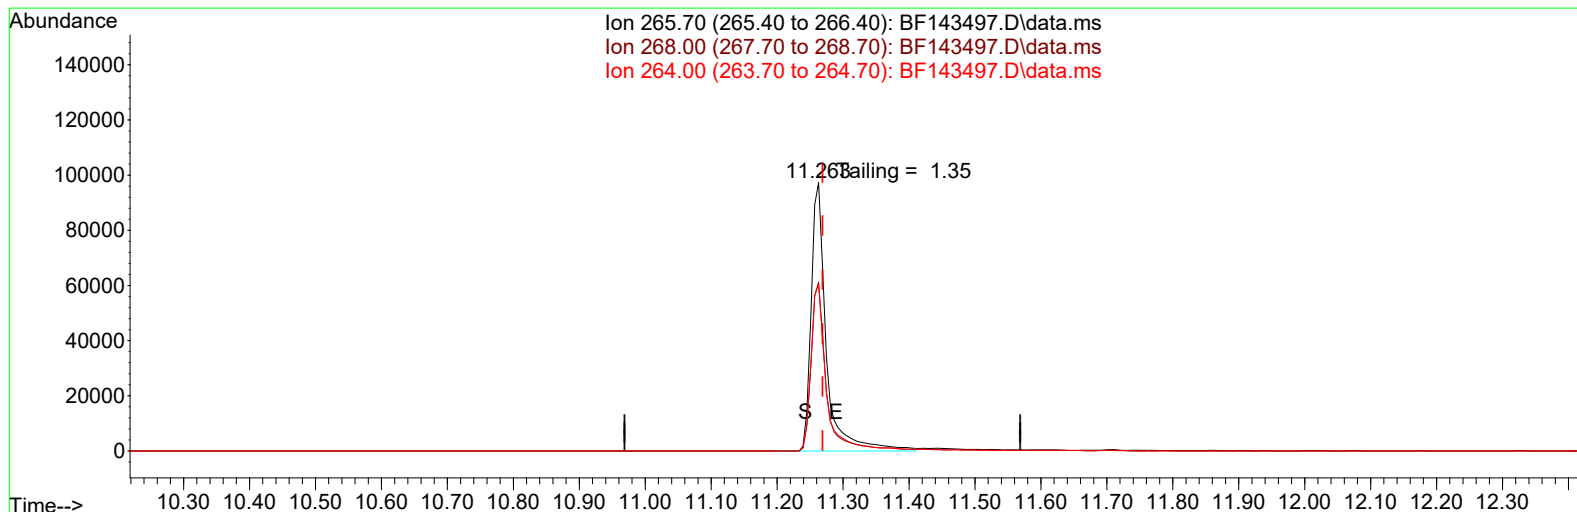

TIC: BF143497.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 130789.27 ng


response 157159

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	62.88
264.00	62.30	62.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082025\
Data File : BF143497.D
Acq On : 20 Aug 2025 21:36
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 02:56:15 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 20 15:07:46 2025
Response via : Initial Calibration

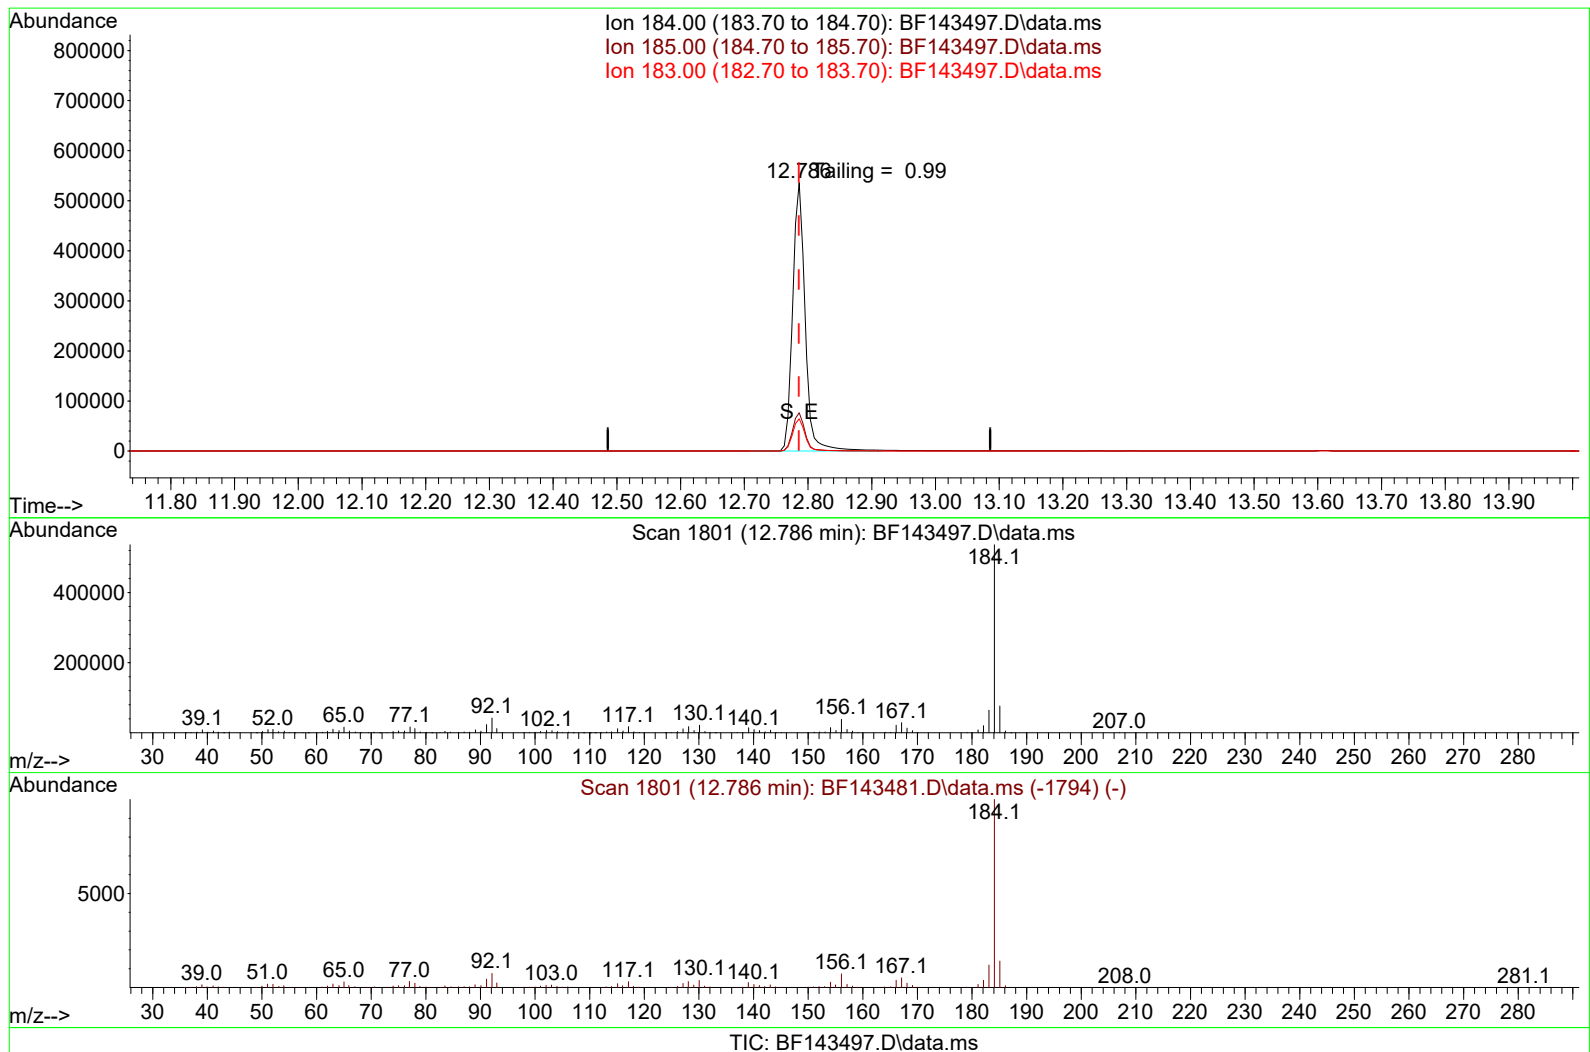

TIC: BF143497.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 0.00 ng

response 737567

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.26
183.00	11.90	12.02
0.00	0.00	0.00