

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
 Data File : BF143382.D
 Acq On : 14 Aug 2025 15:26
 Operator : RC/JU
 Sample : Q2814-04
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TW-82H-N

Quant Time: Aug 14 16:16:53 2025
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 12 13:25:39 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.934	152	152831	20.000	ng	0.00
21) Naphthalene-d8	8.210	136	587688	20.000	ng	0.00
39) Acenaphthene-d10	9.969	164	317654	20.000	ng	0.00
64) Phenanthrene-d10	11.457	188	484666	20.000	ng	0.00
76) Chrysene-d12	14.098	240	294954	20.000	ng	0.00
86) Perylene-d12	15.592	264	316888	20.000	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.569	112	677807	76.693	ng	0.00
7) Phenol-d6	6.563	99	685455	60.480	ng	0.00
23) Nitrobenzene-d5	7.493	82	841229	89.140	ng	0.00
42) 2,4,6-Tribromophenol	10.757	330	360426	155.257	ng	0.00
45) 2-Fluorobiphenyl	9.287	172	1502587	80.214	ng	0.00
79) Terphenyl-d14	13.039	244	1407470	85.193	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF081425\
Data File : BF143382.D
Acq On : 14 Aug 2025 15:26
Operator : RC/JU
Sample : Q2814-04
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TW-82H-N

Quant Time: Aug 14 16:16:53 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF081225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 12 13:25:39 2025
Response via : Initial Calibration




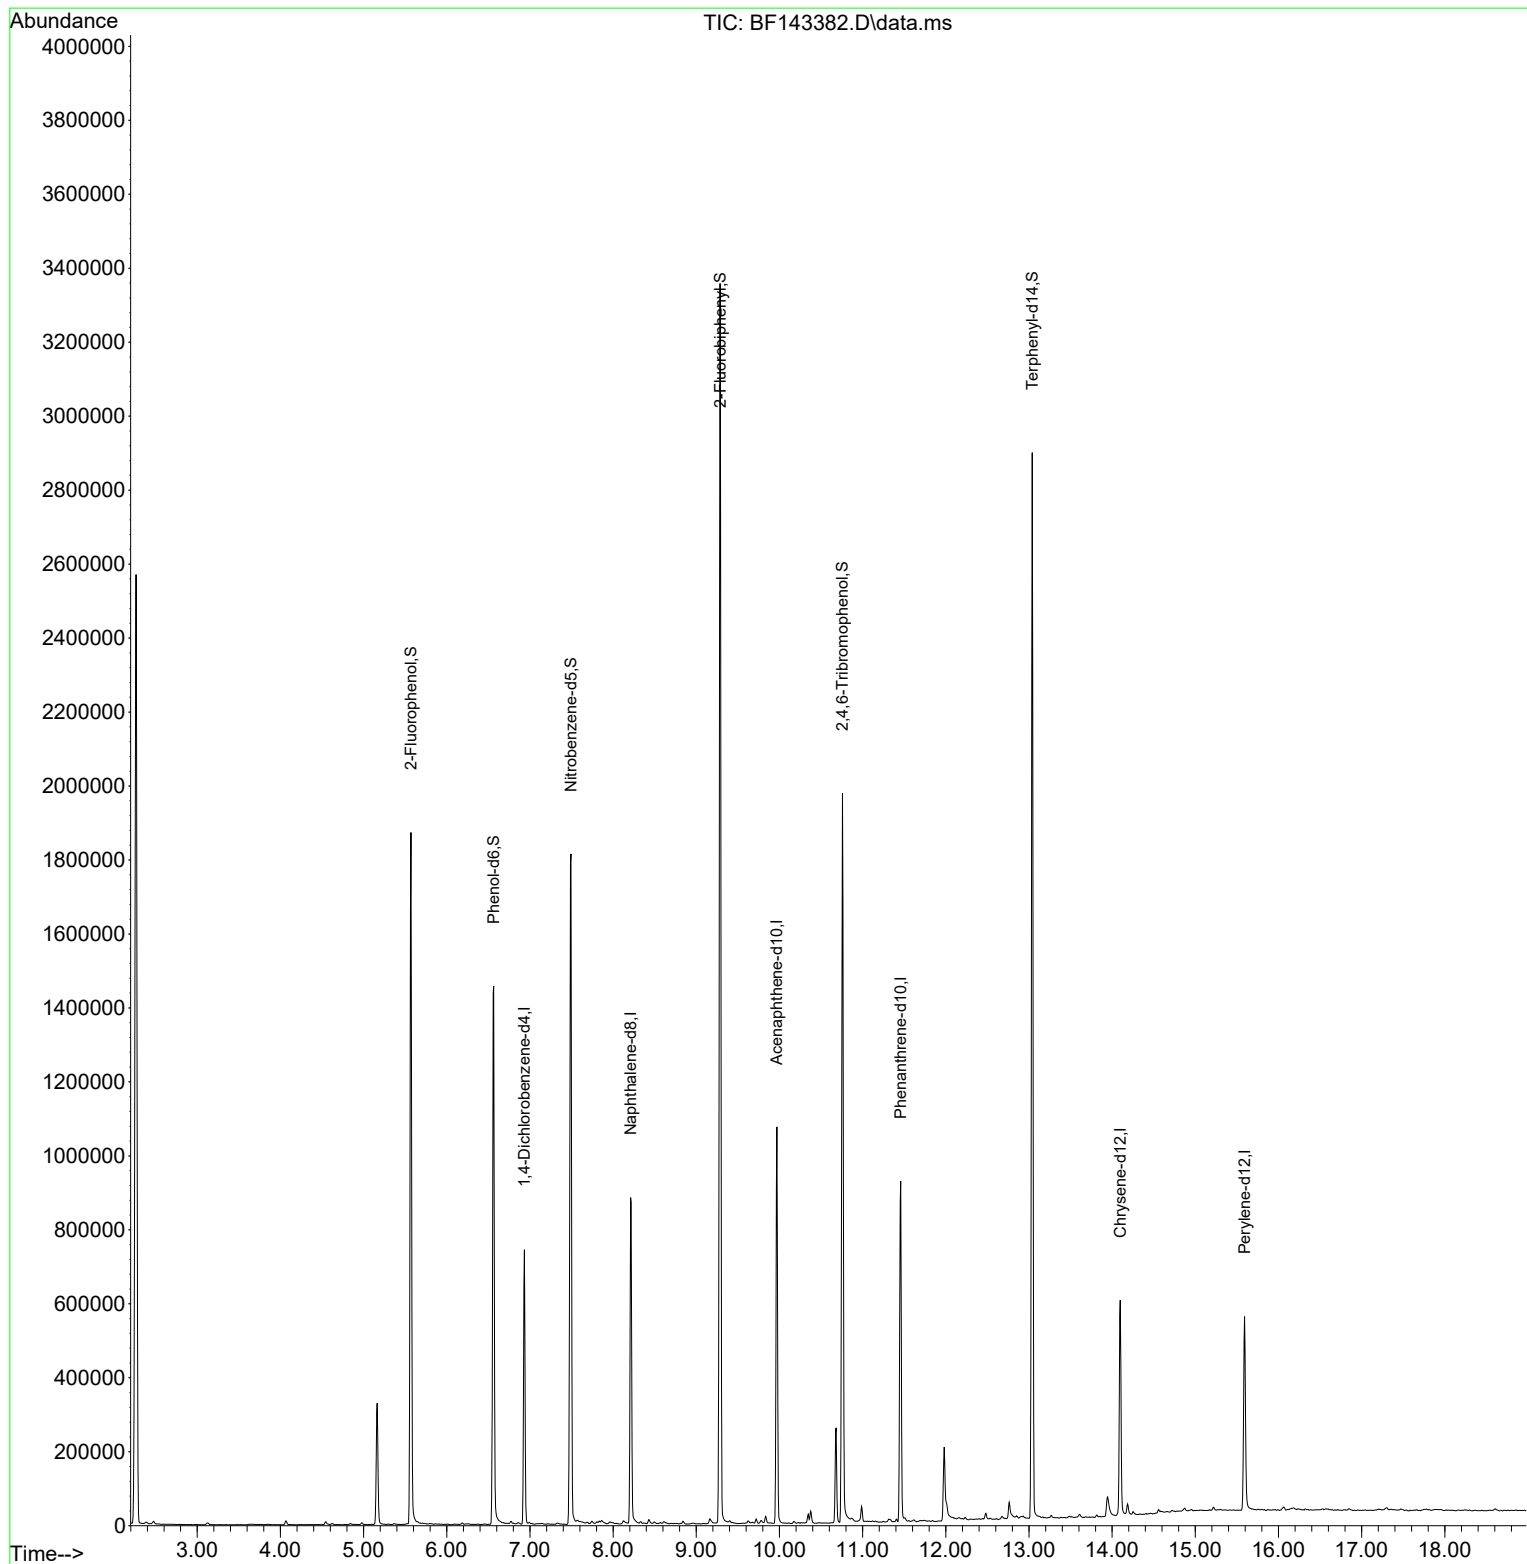


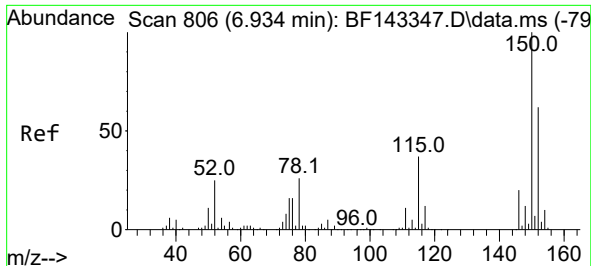

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.934 min Scan# 806
Delta R.T. -0.000 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26




Instrument :
BNA_F
ClientSampleId :
TW-82H-N


Tgt Ion:152 Resp: 152831
Ion Ratio Lower Upper
152 100
150 155.4 129.8 194.8
115 59.2 47.8 71.8

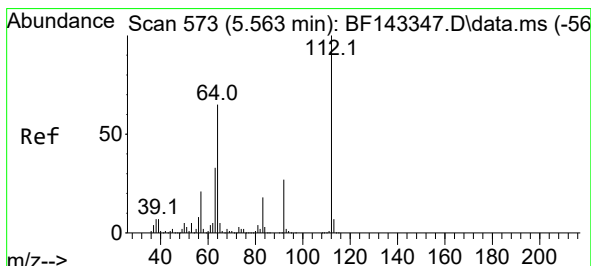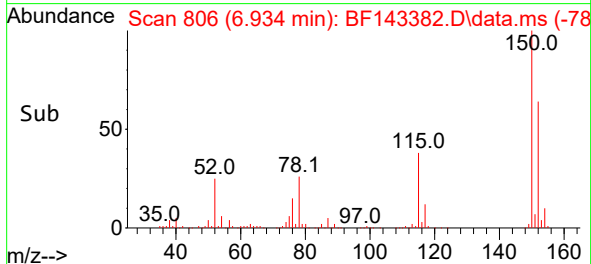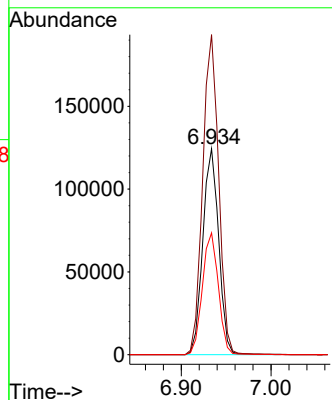

#5
2-Fluorophenol
Concen: 76.693 ng
RT: 5.569 min Scan# 574
Delta R.T. 0.006 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26

Tgt Ion:112 Resp: 677807
Ion Ratio Lower Upper
112 100
64 65.2 52.1 78.1
63 33.5 26.6 39.8



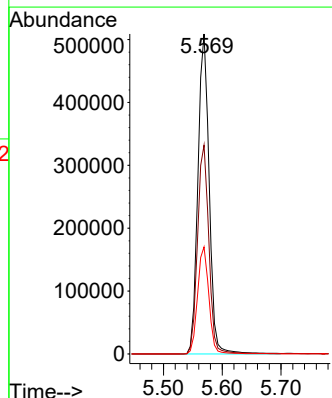
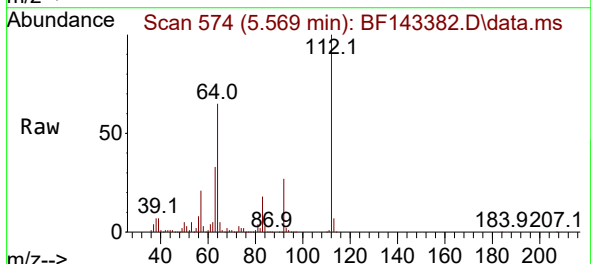


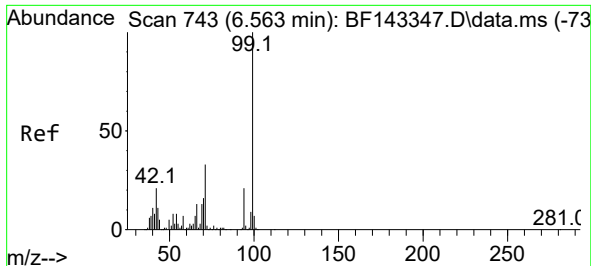

#7
Phenol-d6
Concen: 60.480 ng
RT: 6.563 min Scan# 743
Delta R.T. 0.000 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26




Instrument :
BNA_F
ClientSampleId :
TW-82H-N

Tgt Ion: 99 Resp: 685455
Ion Ratio Lower Upper
99 100
42 20.6 16.6 25.0
71 32.7 26.2 39.2

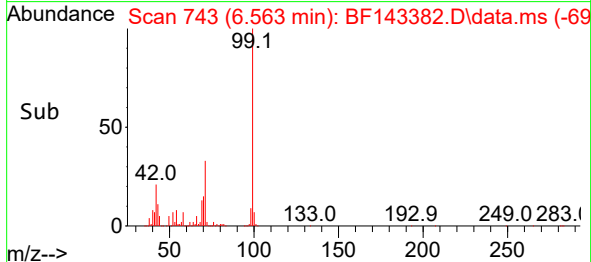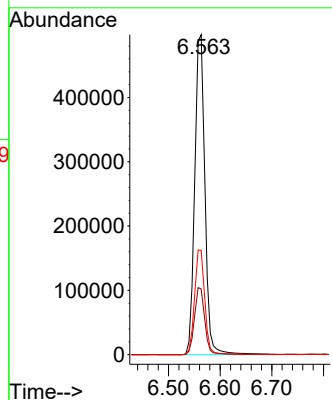

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.210 min Scan# 1023
Delta R.T. 0.000 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26

Tgt Ion: 136 Resp: 587688
Ion Ratio Lower Upper
136 100
137 10.9 8.6 13.0
54 10.3 8.4 12.6
68 7.1 5.9 8.9

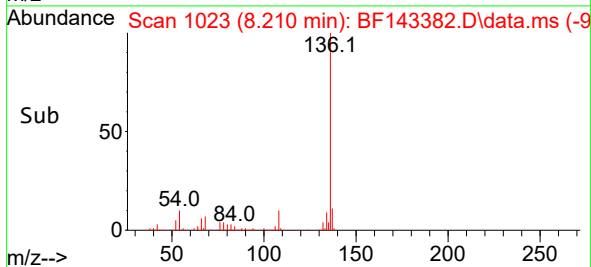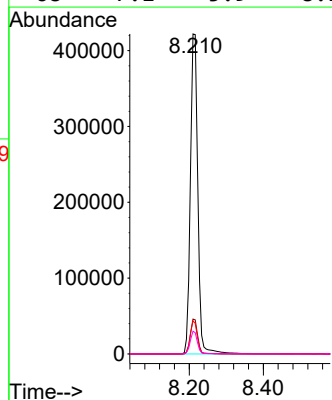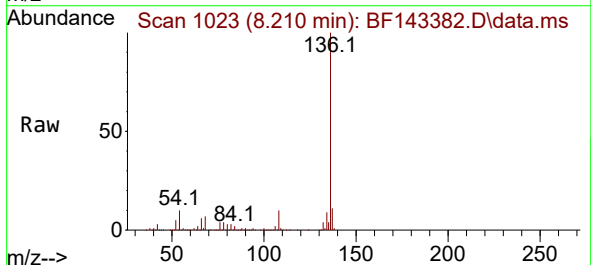



#23

Nitrobenzene-d5

Concen: 89.140 ng

RT: 7.493 min Scan# 901

Delta R.T. 0.000 min

Lab File: BF143382.D

Acq: 14 Aug 2025 15:26

Instrument :

BNA_F

ClientSampleId :

TW-82H-N





Tgt Ion: 82 Resp: 841229

Ion Ratio Lower Upper

82 100

128 44.2 33.5 50.3

54 58.1 46.7 70.1

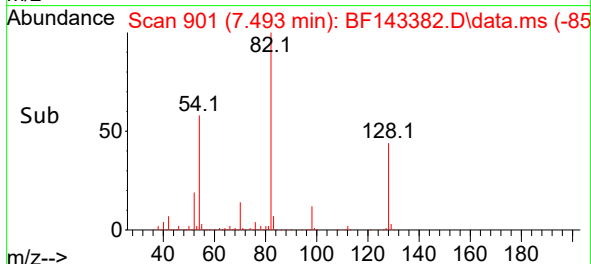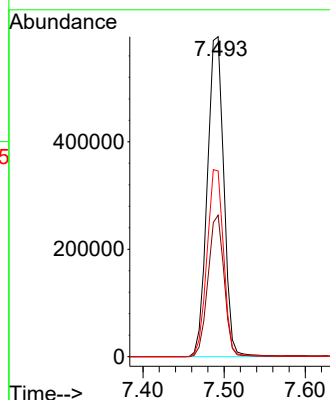

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.969 min Scan# 1322

Delta R.T. -0.000 min

Lab File: BF143382.D

Acq: 14 Aug 2025 15:26




Tgt Ion:164 Resp: 317654


Ion Ratio Lower Upper

164 100

162 97.2 78.6 118.0

160 42.5 34.4 51.6


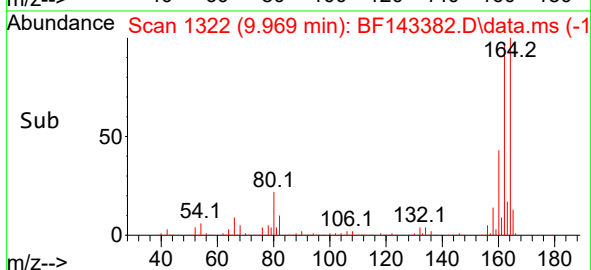
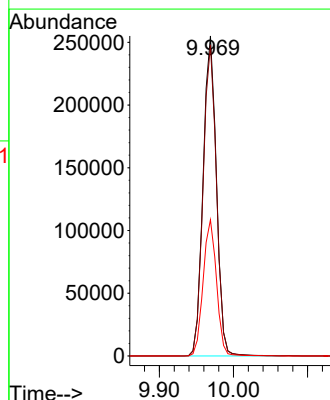
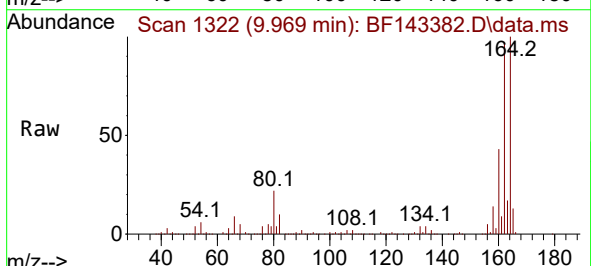


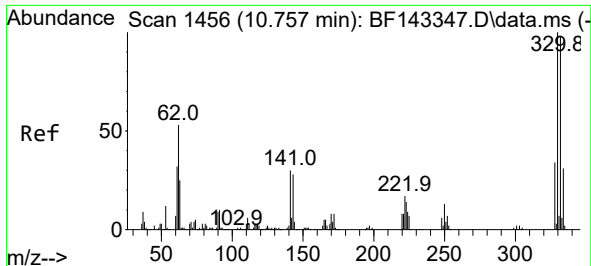

#42
2,4,6-Tribromophenol
Concen: 155.257 ng
RT: 10.757 min Scan# 1456
Delta R.T. 0.000 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26




Instrument :
BNA_F
ClientSampleId :
TW-82H-N


Tgt Ion:330 Resp: 360426
Ion Ratio Lower Upper
330 100
332 95.7 78.1 117.1
141 28.0 25.4 38.0

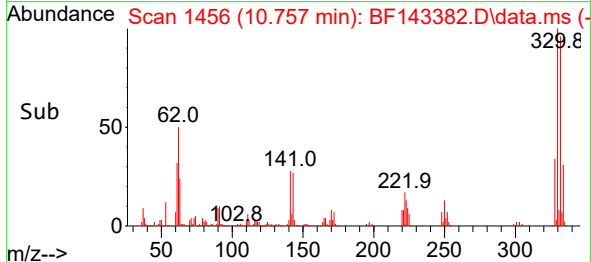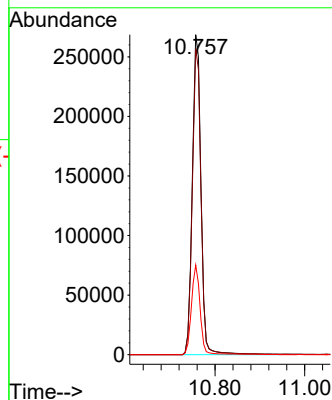

#45
2-Fluorobiphenyl
Concen: 80.214 ng
RT: 9.287 min Scan# 1206
Delta R.T. 0.000 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26

Tgt Ion:172 Resp: 1502587
Ion Ratio Lower Upper
172 100
171 35.6 28.4 42.6
170 23.7 19.1 28.7


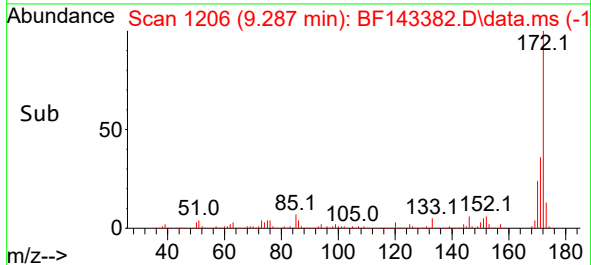
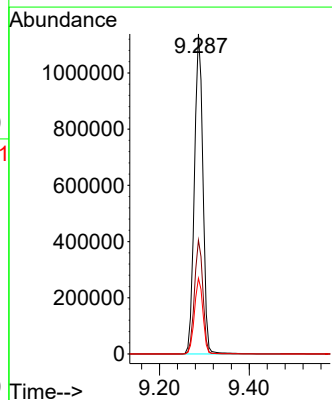
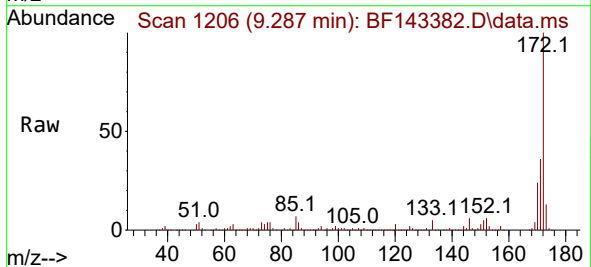


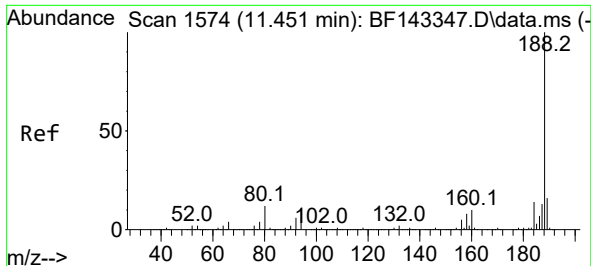

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.457 min Scan# 11
Delta R.T. 0.006 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26




Instrument :
BNA_F
ClientSampleId :
TW-82H-N


Tgt Ion:188 Resp: 484666
Ion Ratio Lower Upper
188 100
94 10.4 8.8 13.2
80 11.1 9.7 14.5

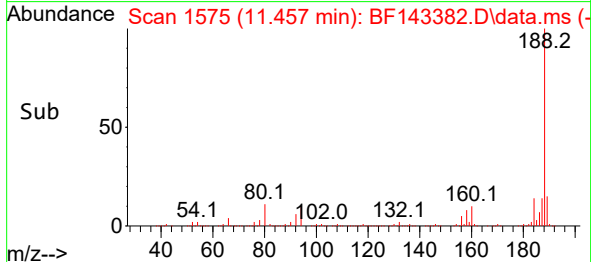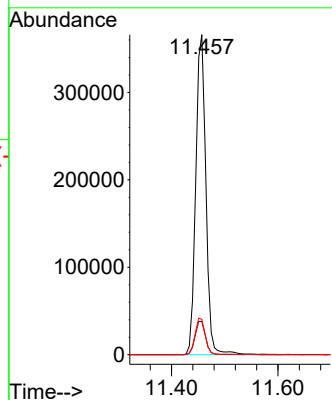

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.098 min Scan# 2024
Delta R.T. 0.006 min
Lab File: BF143382.D
Acq: 14 Aug 2025 15:26

Tgt Ion:240 Resp: 294954
Ion Ratio Lower Upper
240 100
120 11.2 9.0 13.6
236 24.8 19.9 29.9

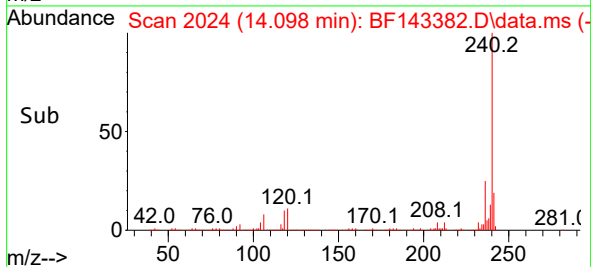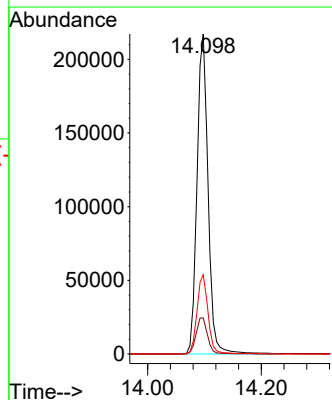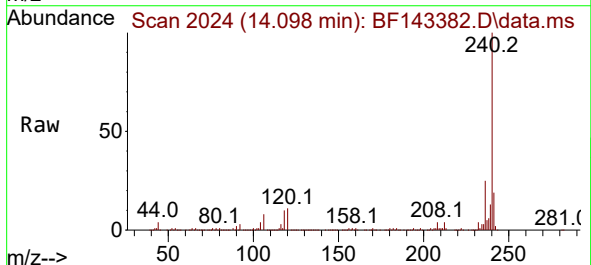



#79

Terphenyl-d14

Concen: 85.193 ng

RT: 13.039 min Scan# 1843

Delta R.T. 0.006 min

Lab File: BF143382.D

Acq: 14 Aug 2025 15:26

Instrument :

BNA_F

ClientSampleId :

TW-82H-N





Tgt Ion:244 Resp: 1407470

Ion Ratio Lower Upper

244 100

212 6.6 5.1 7.7

122 10.7 8.9 13.3

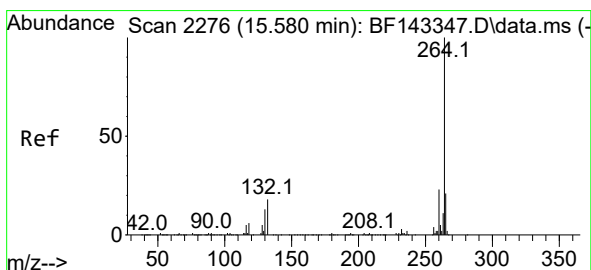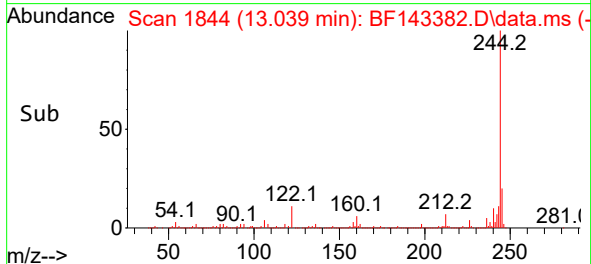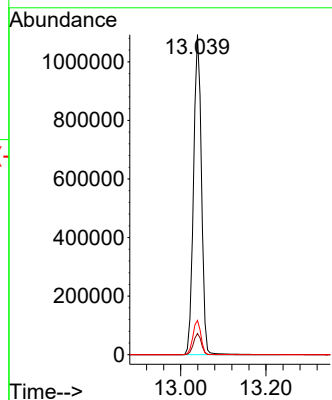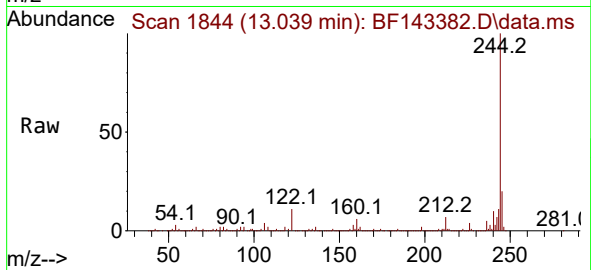

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.592 min Scan# 2278

Delta R.T. 0.012 min

Lab File: BF143382.D

Acq: 14 Aug 2025 15:26

Tgt Ion:264 Resp: 316888

Ion Ratio Lower Upper

264 100

260 23.3 18.7 28.1

265 21.7 17.2 25.8

