

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081225\
 Data File : VX047287.D
 Acq On : 12 Aug 2025 11:17
 Operator : JC/MD
 Sample : VX0812WBL02
 Misc : 5.0mL/MSVOA_X/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_X
 ClientSampleId :
 VX0812WBL02

Quant Time: Aug 13 01:17:04 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
 Quant Title : SW846 8260
 QLast Update : Tue Jul 22 03:59:51 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	5.562	168	346553	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	6.763	114	664166	50.000	ug/l	0.00
63) Chlorobenzene-d5	10.055	117	641288	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.018	152	313492	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	5.964	65	241016	55.830	ug/l	0.00
Spiked Amount	50.000	Range	78 - 117	Recovery	=	111.660%
35) Dibromofluoromethane	5.391	113	202875	49.472	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.940%
50) Toluene-d8	8.647	98	731358	55.071	ug/l	0.00
Spiked Amount	50.000	Range	92 - 112	Recovery	=	110.140%
62) 4-Bromofluorobenzene	11.079	95	304518	53.209	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	106.420%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081225\
Data File : VX047287.D
Acq On : 12 Aug 2025 11:17
Operator : JC/MD
Sample : VX0812WBL02
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
VX0812WBL02

Quant Time: Aug 13 01:17:04 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Quant Title : SW846 8260
QLast Update : Tue Jul 22 03:59:51 2025
Response via : Initial Calibration




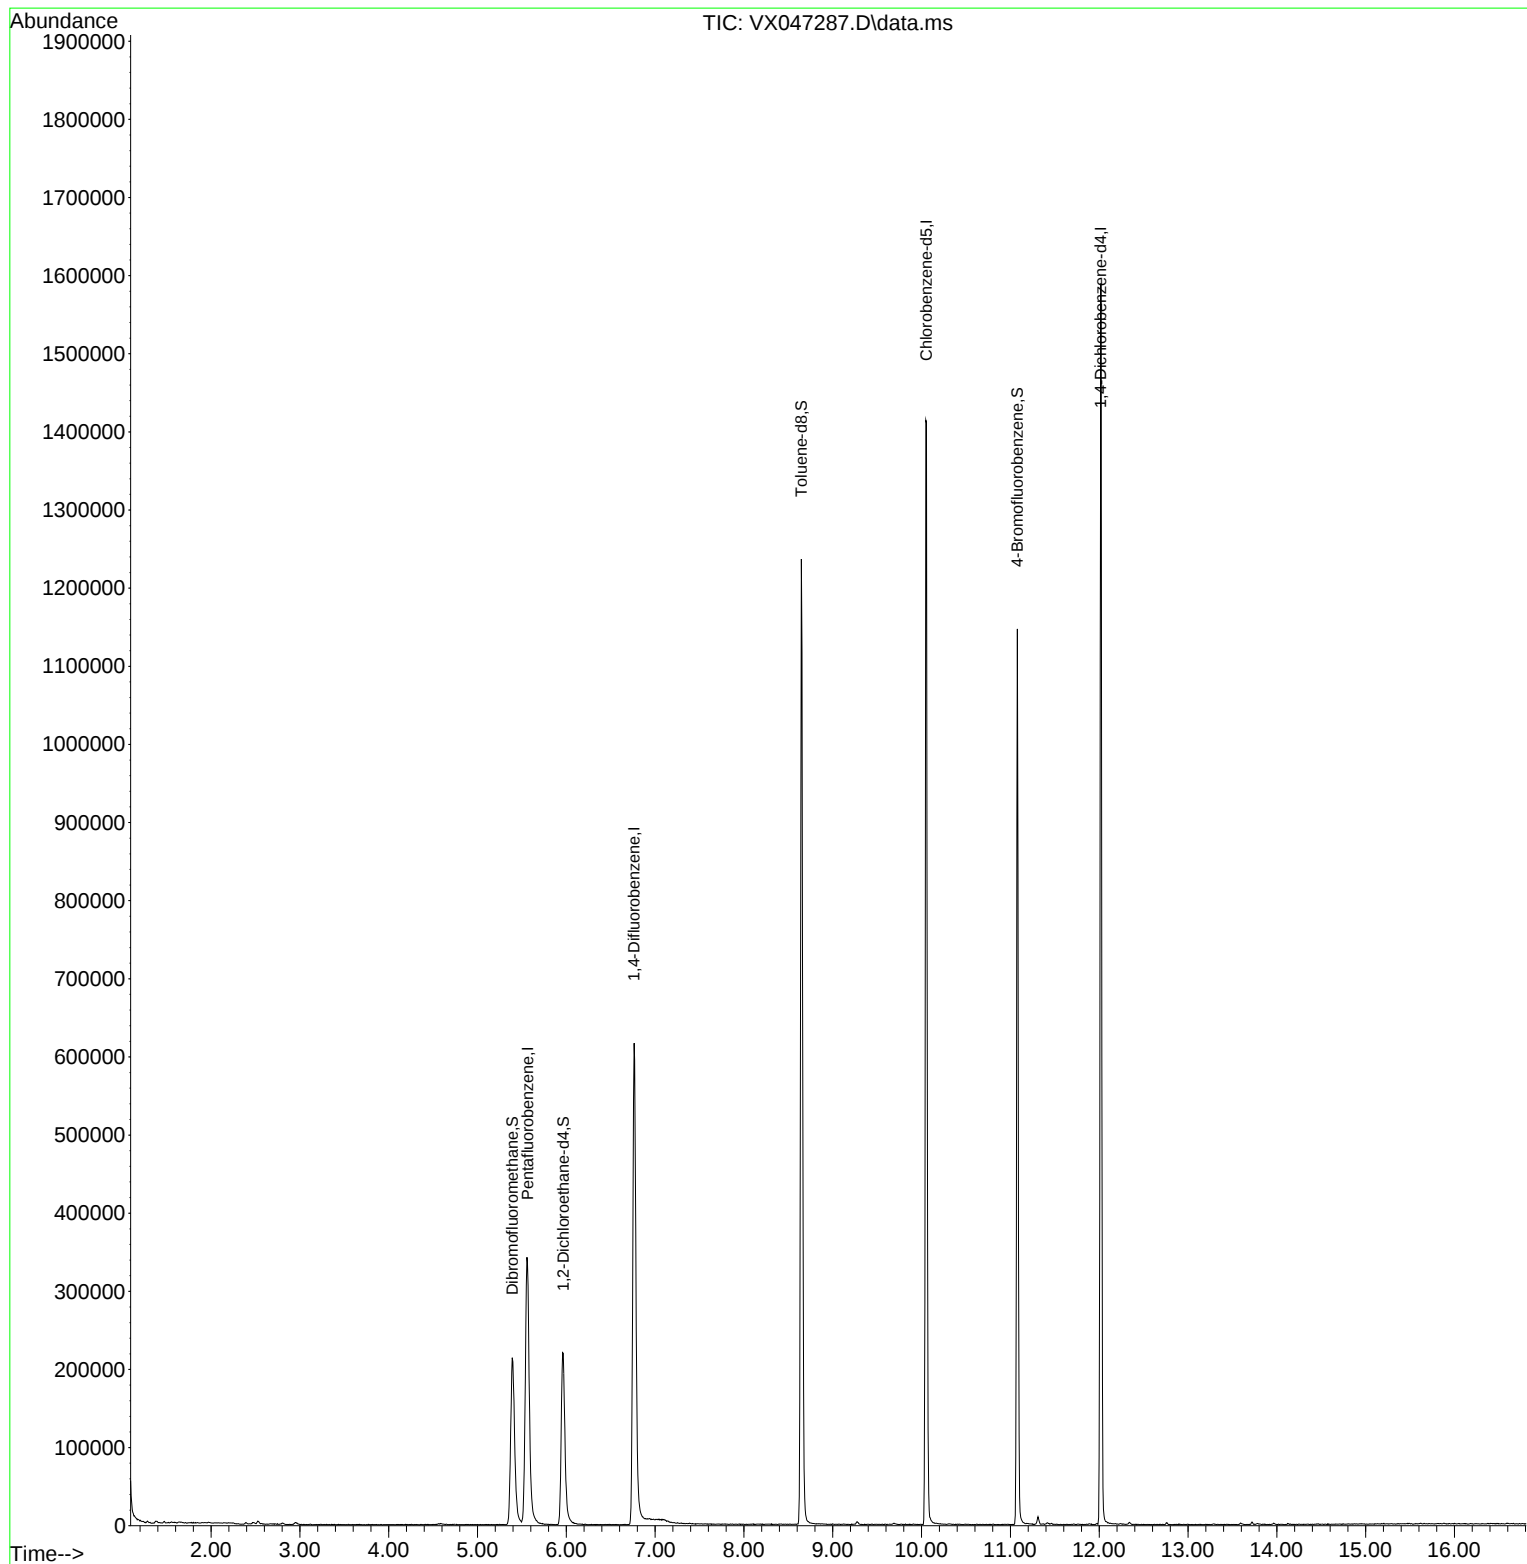


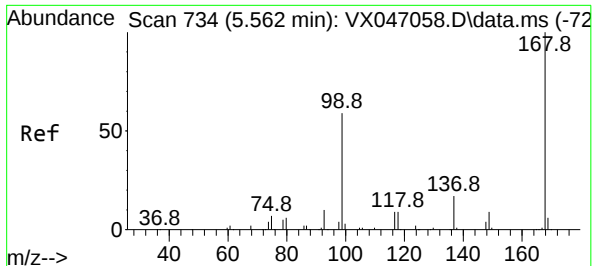

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 5.562 min Scan# 71
Delta R.T. 0.000 min
Lab File: VX047287.D
Acq: 12 Aug 2025 11:17




Instrument :
MSVOA_X
ClientSampleId :
VX0812WBL02


Tgt Ion:168 Resp: 346553
Ion Ratio Lower Upper
168 100
99 60.4 48.0 72.0

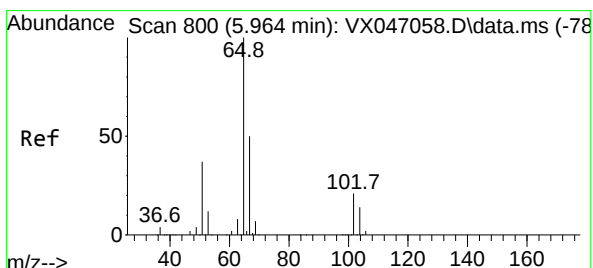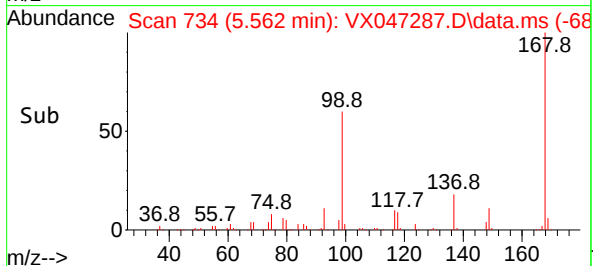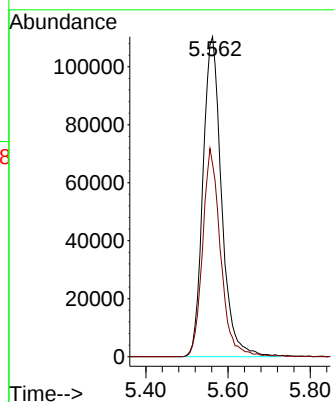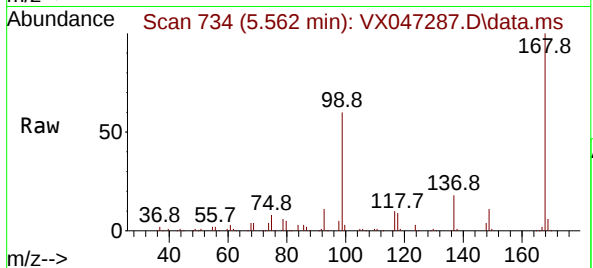

#33
1,2-Dichloroethane-d4
Concen: 55.830 ug/l
RT: 5.964 min Scan# 800
Delta R.T. 0.000 min
Lab File: VX047287.D
Acq: 12 Aug 2025 11:17


Tgt Ion: 65 Resp: 241016
Ion Ratio Lower Upper
65 100
67 51.1 0.0 104.8

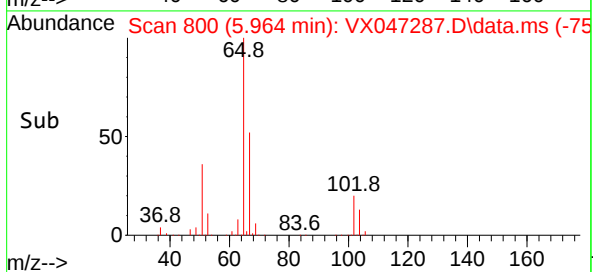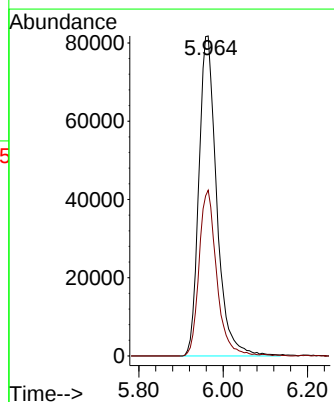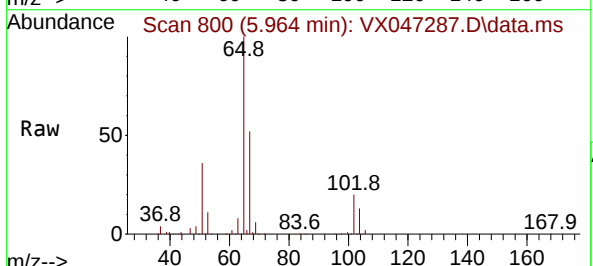



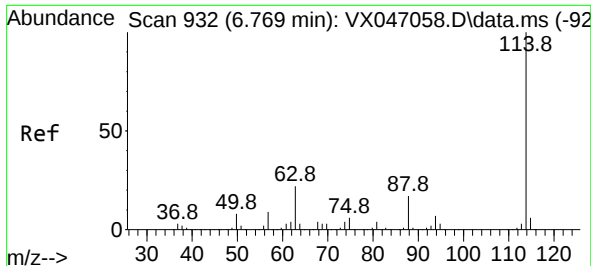


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 6.763 min Scan# 91
Delta R.T. -0.006 min
Lab File: VX047287.D
Acq: 12 Aug 2025 11:17


Instrument :
MSVOA_X
ClientSampleId :
VX0812WBL02

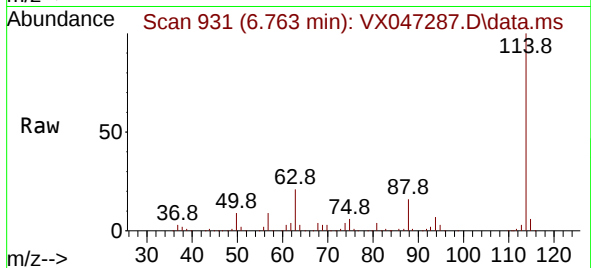



Tgt Ion:114 Resp: 664166
Ion Ratio Lower Upper
114 100
63 21.5 0.0 43.2
88 16.1 0.0 33.8

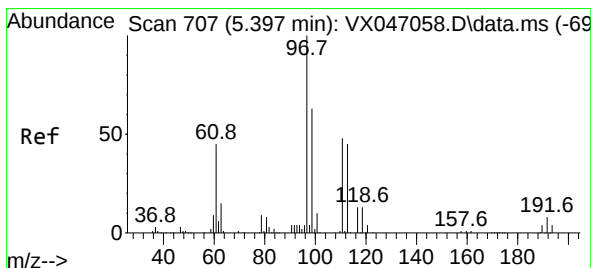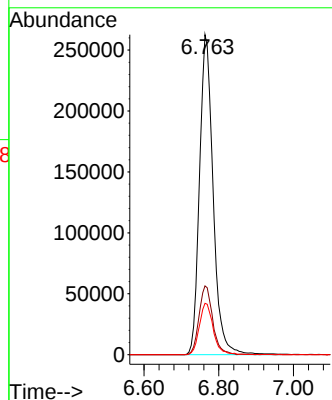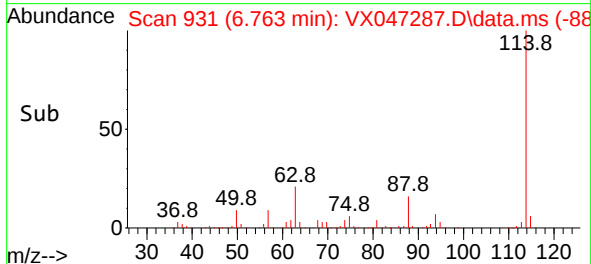


#35
Dibromofluoromethane
Concen: 49.472 ug/l
RT: 5.391 min Scan# 706
Delta R.T. -0.006 min
Lab File: VX047287.D
Acq: 12 Aug 2025 11:17

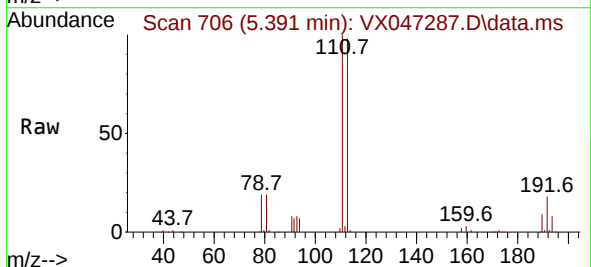

Tgt Ion:113 Resp: 202875
Ion Ratio Lower Upper
113 100
111 102.8 82.6 124.0
192 18.1 14.9 22.3



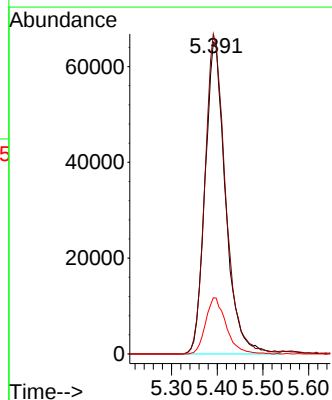
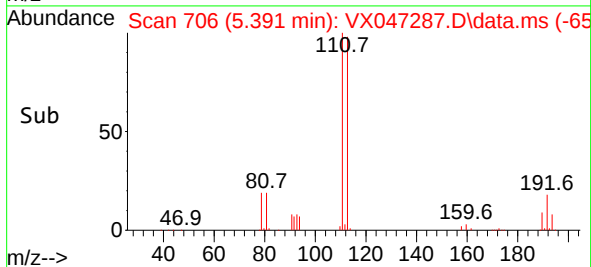


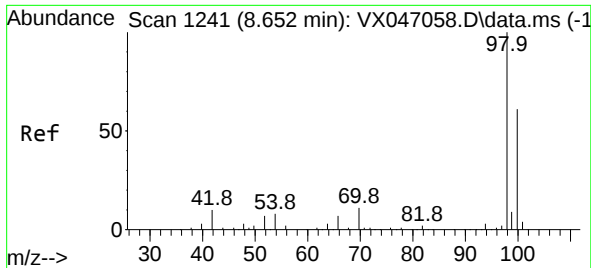

#50
Toluene-d8
Concen: 55.071 ug/l
RT: 8.647 min Scan# 11
Delta R.T. -0.006 min
Lab File: VX047287.D
Acq: 12 Aug 2025 11:17




Instrument :
MSVOA_X
ClientSampleId :
VX0812WBL02


Tgt Ion: 98 Resp: 731358
Ion Ratio Lower Upper
98 100
100 66.7 53.3 79.9

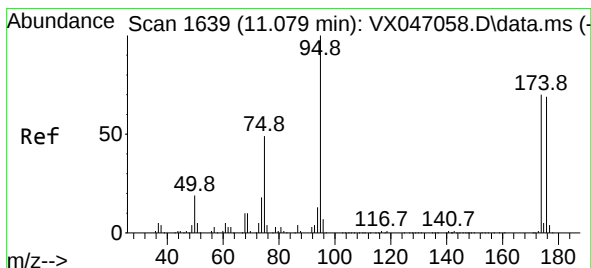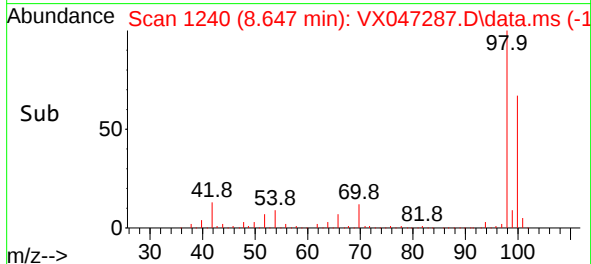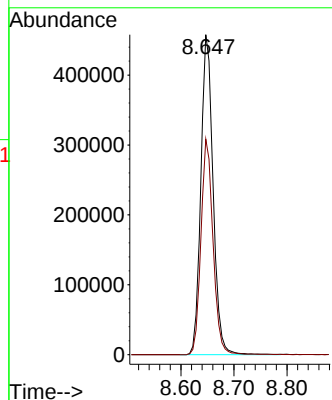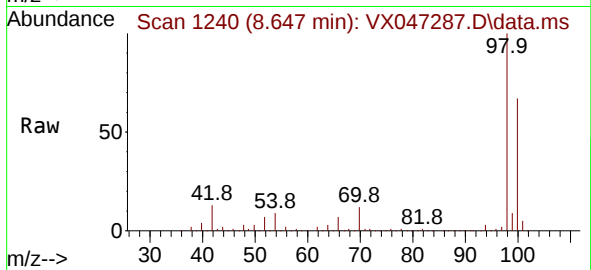

#62
4-Bromofluorobenzene
Concen: 53.209 ug/l
RT: 11.079 min Scan# 1639
Delta R.T. 0.000 min
Lab File: VX047287.D
Acq: 12 Aug 2025 11:17

Tgt Ion: 95 Resp: 304518
Ion Ratio Lower Upper
95 100
174 73.2 0.0 144.6
176 70.9 0.0 139.6

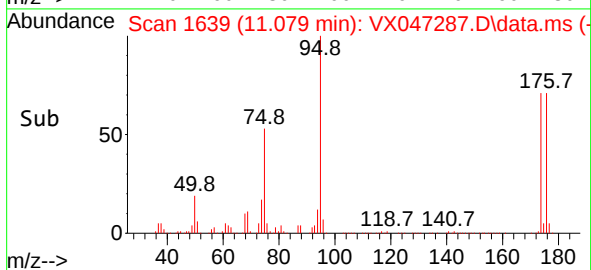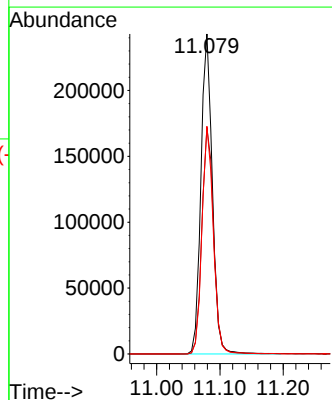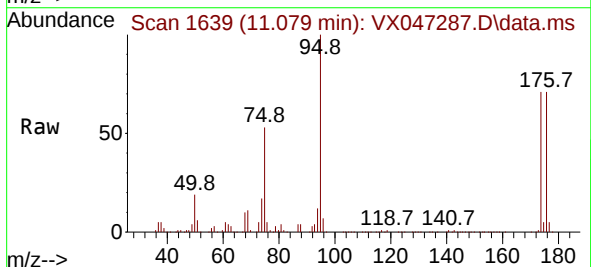

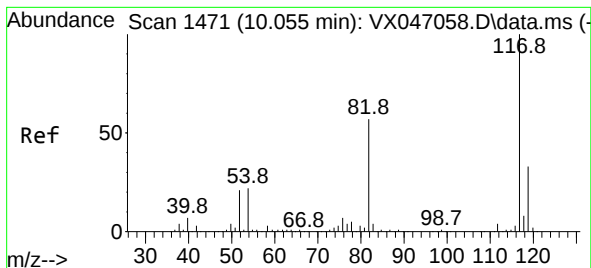

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 10.055 min Scan# 1471

Delta R.T. 0.000 min

Lab File: VX047287.D

Acq: 12 Aug 2025 11:17

Instrument :

MSVOA_X

ClientSampleId :

VX0812WBL02





Tgt Ion:117 Resp: 641288

Ion Ratio Lower Upper

117 100

82 56.1 45.4 68.2

119 32.4 26.1 39.1

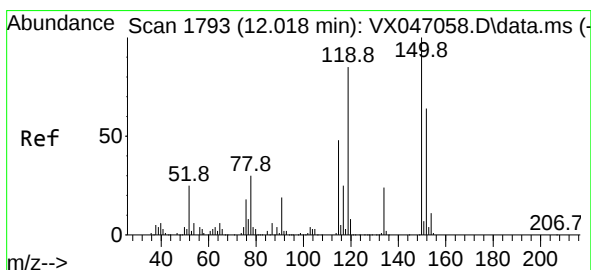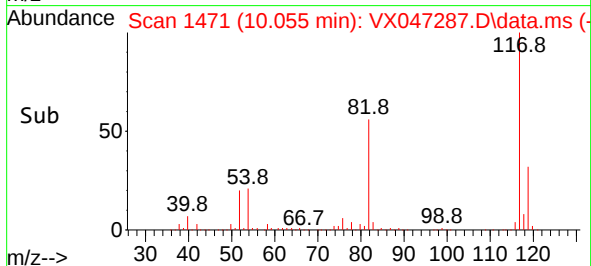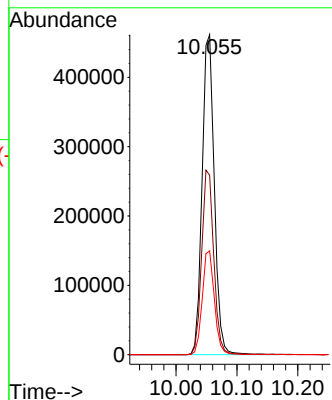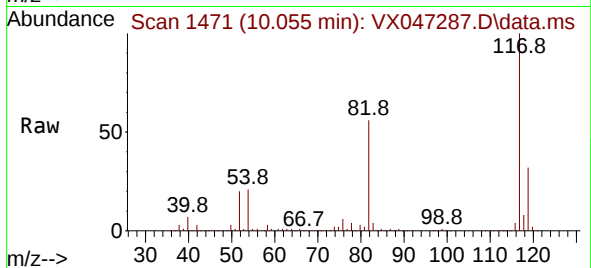

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 12.018 min Scan# 1793

Delta R.T. 0.000 min

Lab File: VX047287.D

Acq: 12 Aug 2025 11:17

Tgt Ion:152 Resp: 313492

Ion Ratio Lower Upper

152 100

115 63.0 45.6 136.7

150 157.9 0.0 354.6

