
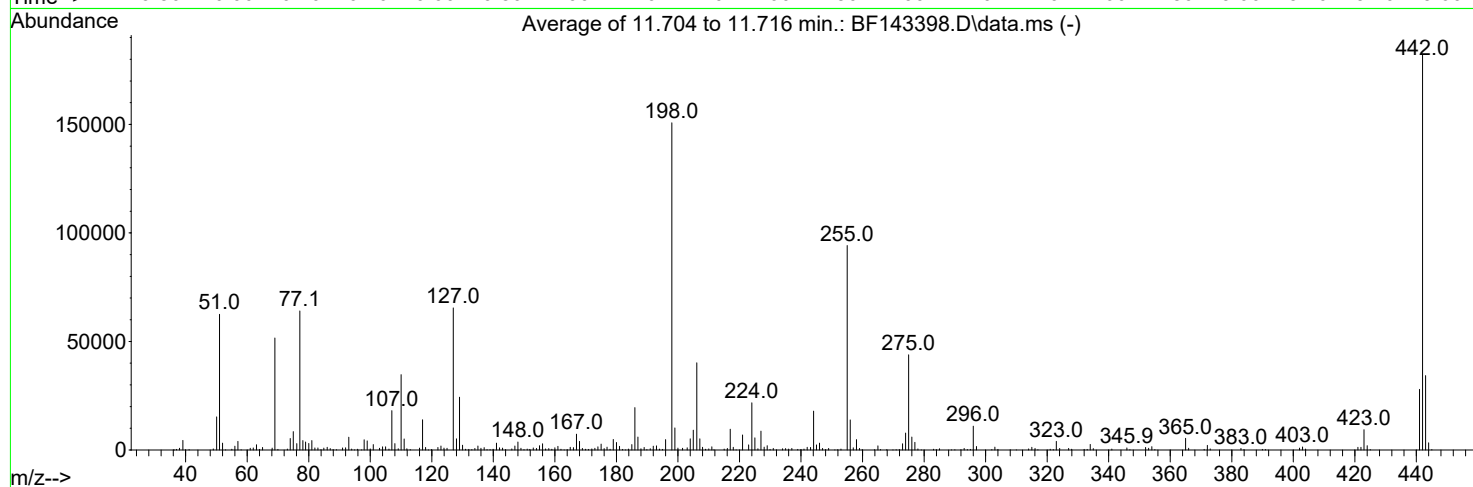


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081425\  
Data File : BF143398.D  
Acq On : 15 Aug 2025 01:26  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081225.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Aug 12 13:25:39 2025

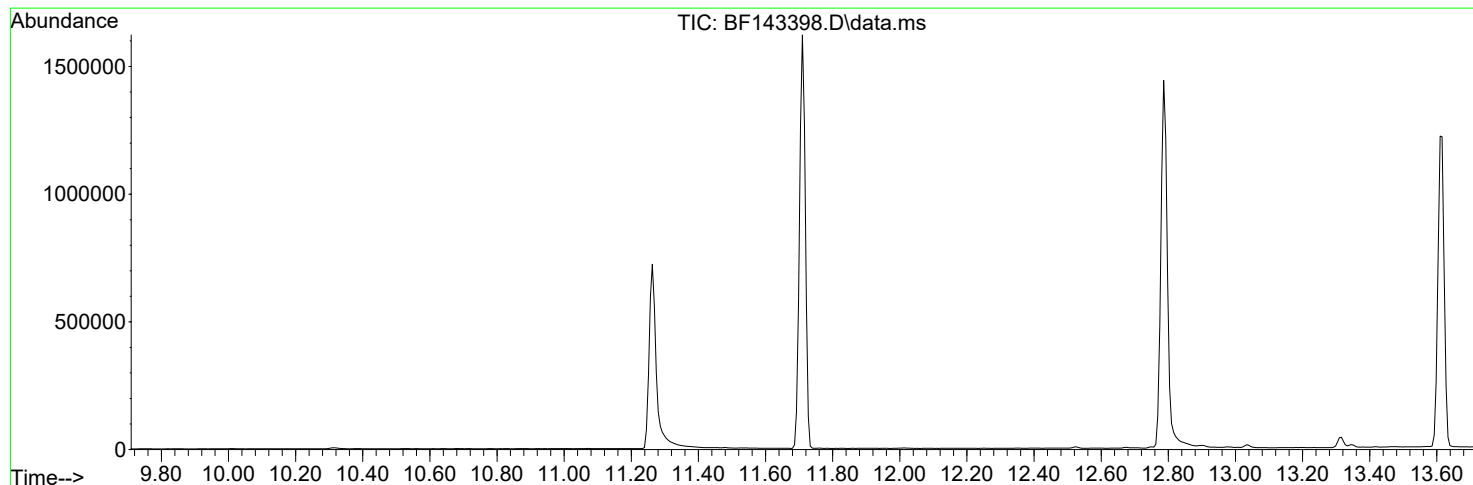

AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw    | Result    |
|--------|---------|--------|--------|-------|--------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn    | Pass/Fail |
| 68     | 69      | 0.00   | 2      | 1.7   | 886    | PASS      |
| 69     | 69      | 100    | 100    | 100.0 | 51568  | PASS      |
| 70     | 69      | 0.00   | 2      | 0.6   | 319    | PASS      |
| 197    | 198     | 0.00   | 2      | 0.0   | 0      | PASS      |
| 198    | 198     | 100    | 100    | 100.0 | 150741 | PASS      |
| 199    | 198     | 5      | 9      | 6.8   | 10206  | PASS      |
| 365    | 198     | 1      | 100    | 3.6   | 5358   | PASS      |
| 441    | 443     | 0.01   | 150    | 81.5  | 27955  | PASS      |
| 442    | 442     | 100    | 100    | 100.0 | 181899 | PASS      |
| 443    | 442     | 15     | 24     | 18.8  | 34285  | PASS      |

# DDT Breakdown




| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 8/14/2025     | BNA_F            | <u>BF143398.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 317573           | 13.619             |
| DDD           | 15212            | 13.316             |
| DDE           | 914              | 12.98              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 16126         | 333699           | 4.83               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081425\  
Data File : BF143398.D  
Acq On : 15 Aug 2025 01:26  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 15 03:37:49 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 12 13:25:39 2025  
Response via : Initial Calibration

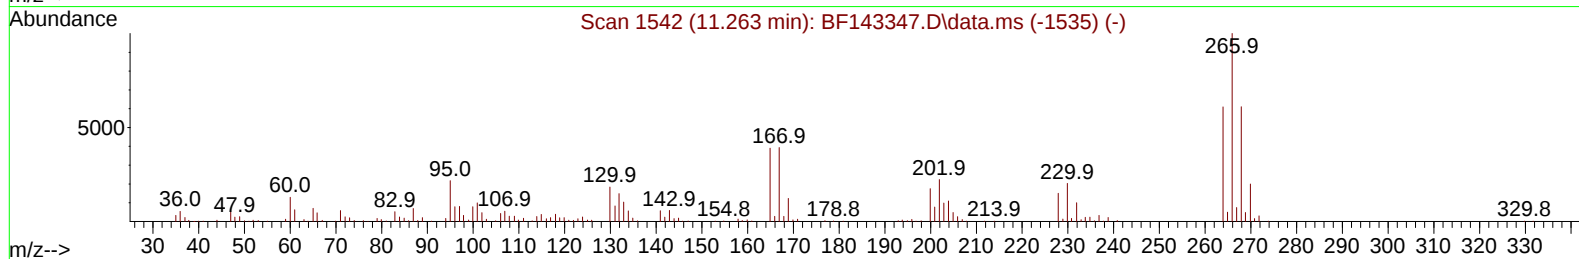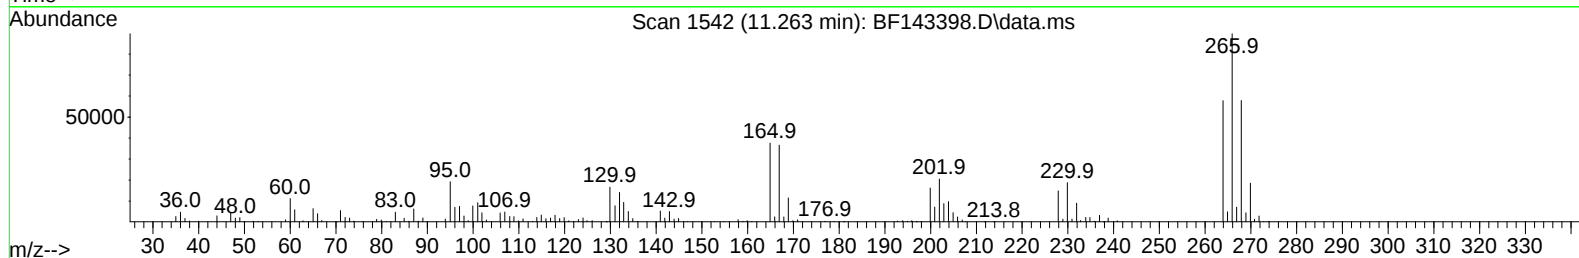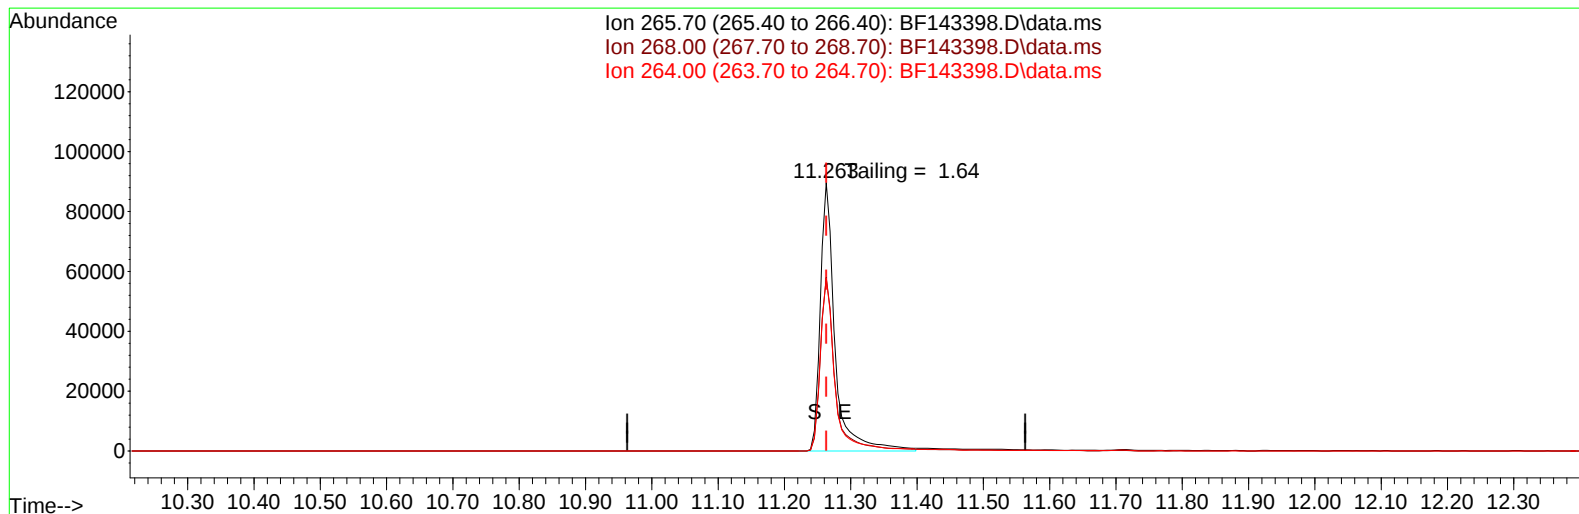

TIC: BF143398.D\data.ms

**(70) Pentachlorophenol (C)**

**11.263min (-0.000) 83327.89 ng**




**response 139002**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.00  | 64.61  |
| 264.00 | 61.00  | 64.47  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF081425\  
Data File : BF143398.D  
Acq On : 15 Aug 2025 01:26  
Operator : RC/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Aug 15 03:37:49 2025  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF081225.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Aug 12 13:25:39 2025  
Response via : Initial Calibration

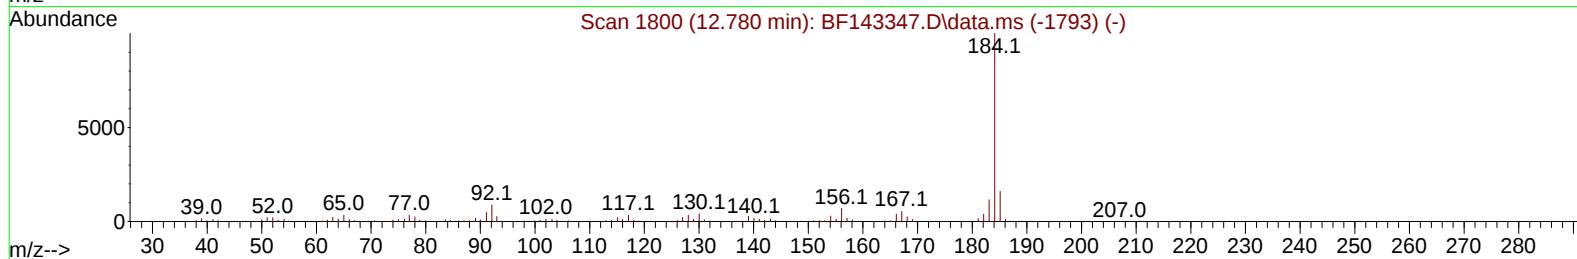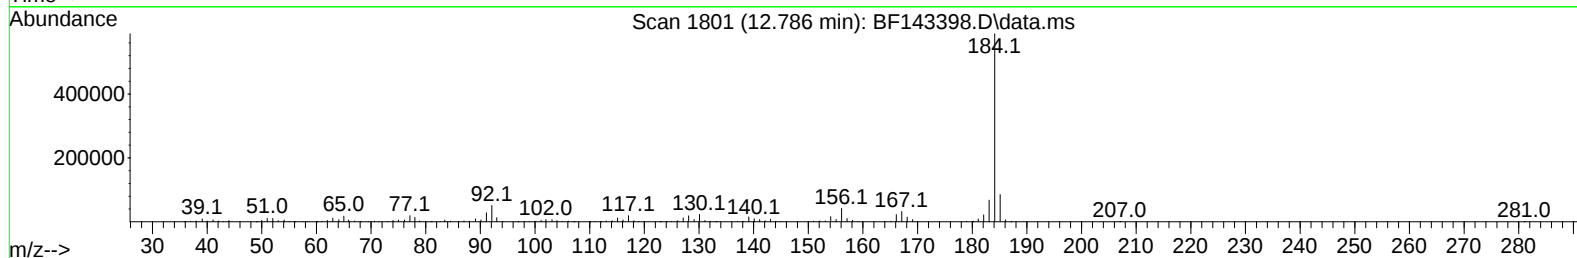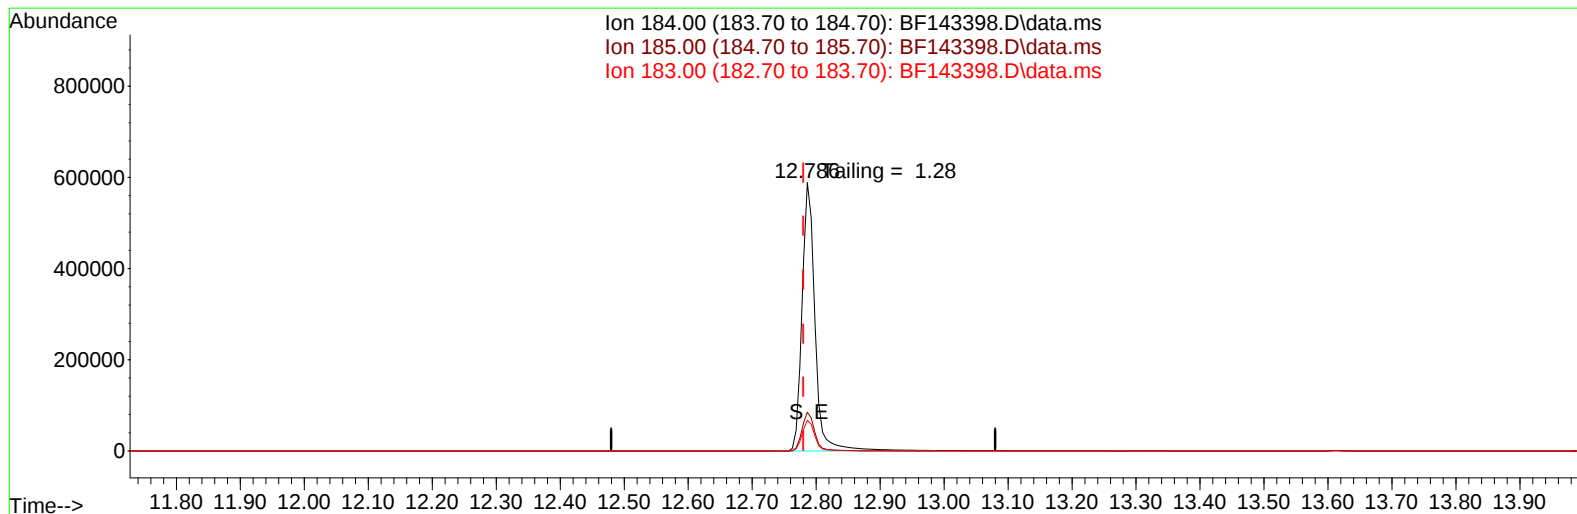

TIC: BF143398.D\data.ms

**(77) Benzidine**

**12.786min (+ 0.006) 0.00 ng**

**response 830815**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 16.00  | 14.46  |
| 183.00 | 11.60  | 11.48  |
| 0.00   | 0.00   | 0.00   |