


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143517.D
Acq On : 21 Aug 2025 08:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 21 06:12:21 2025

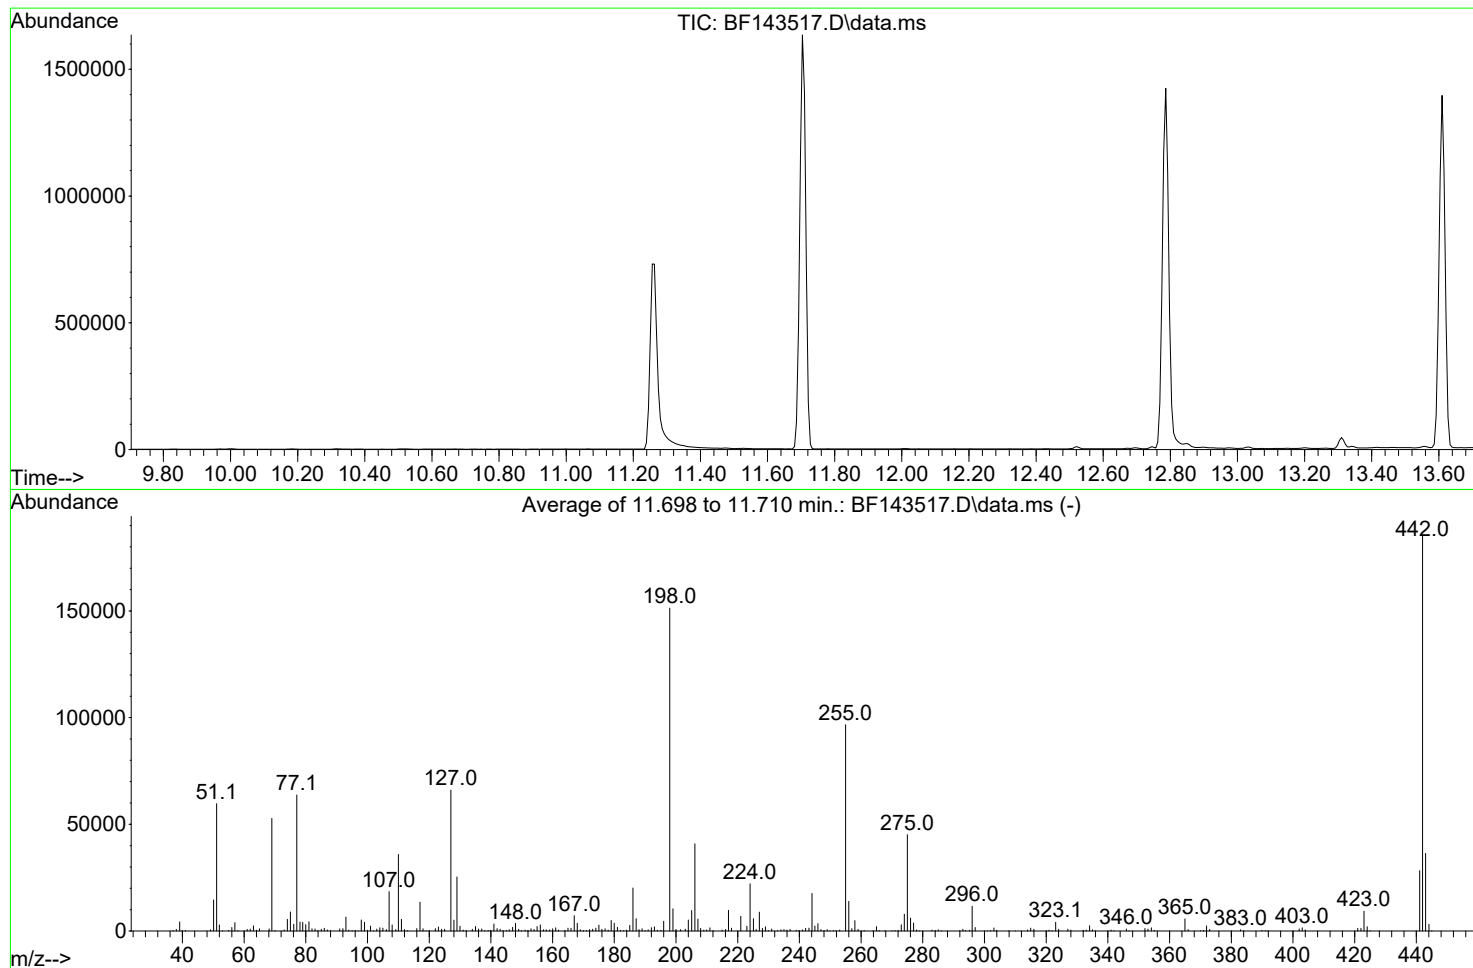

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.9	984	PASS
69	69	100	100	100.0	52787	PASS
70	69	0.00	2	0.6	326	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	151288	PASS
199	198	5	9	6.9	10453	PASS
365	198	1	100	3.8	5742	PASS
441	443	0.01	150	77.6	28243	PASS
442	442	100	100	100.0	185035	PASS
443	442	15	24	19.7	36395	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
8/21/2025	BNA_F	<u>BF143517.D</u>
Compound Name	Response	Retention Time
DDT	346568	13.61
DDD	14042	13.31
DDE	896	12.974
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14938	361506	4.13

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143517.D
Acq On : 21 Aug 2025 08:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 08:42:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

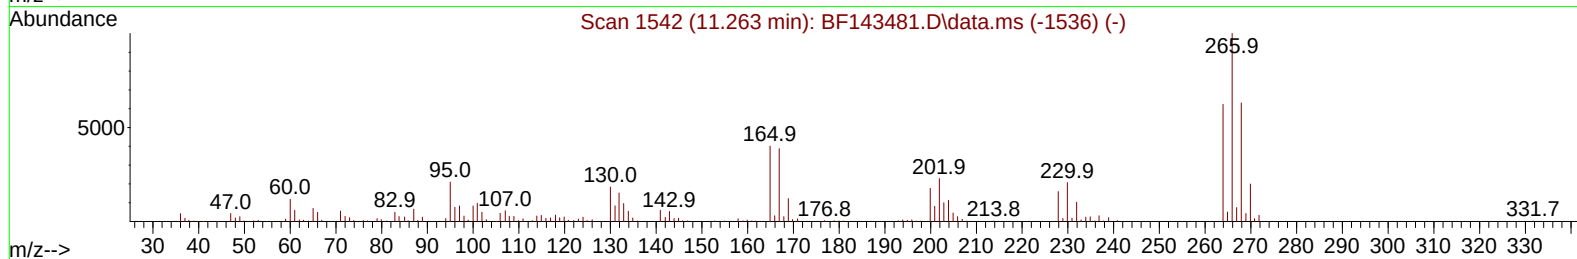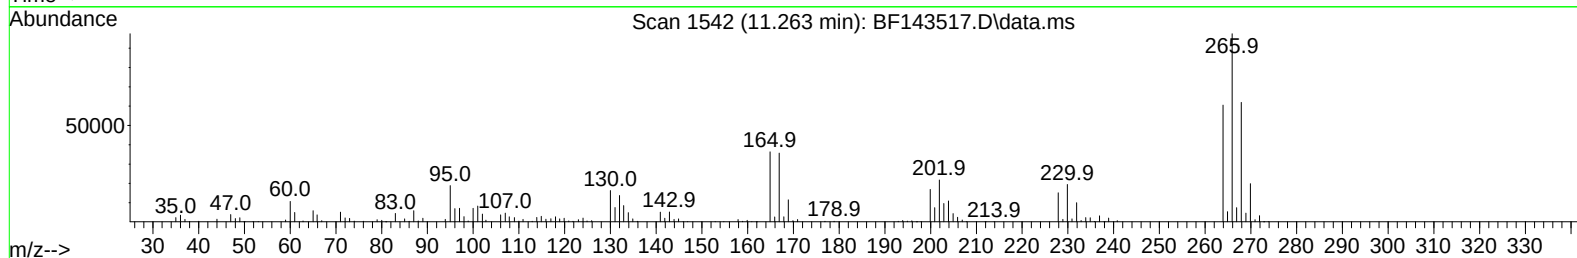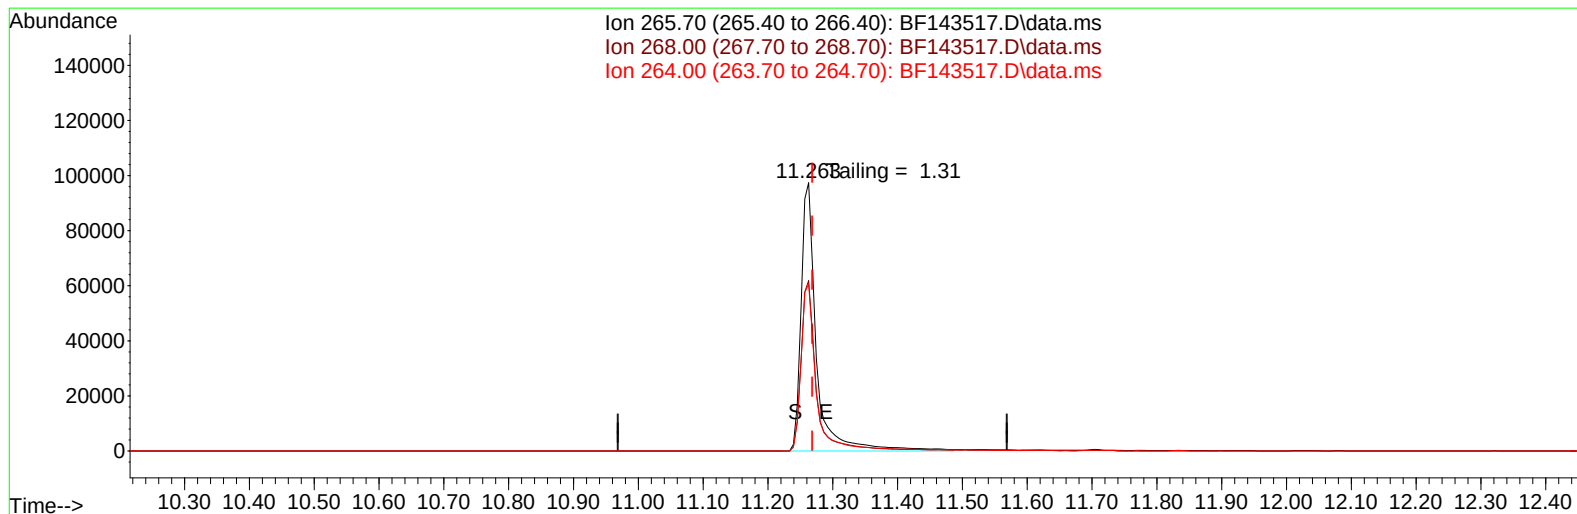

TIC: BF143517.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 27043.48 ng




response 160887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.52
264.00	62.30	62.15
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF082125\
Data File : BF143517.D
Acq On : 21 Aug 2025 08:20
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 21 08:42:13 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF082025.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 21 06:12:21 2025
Response via : Initial Calibration

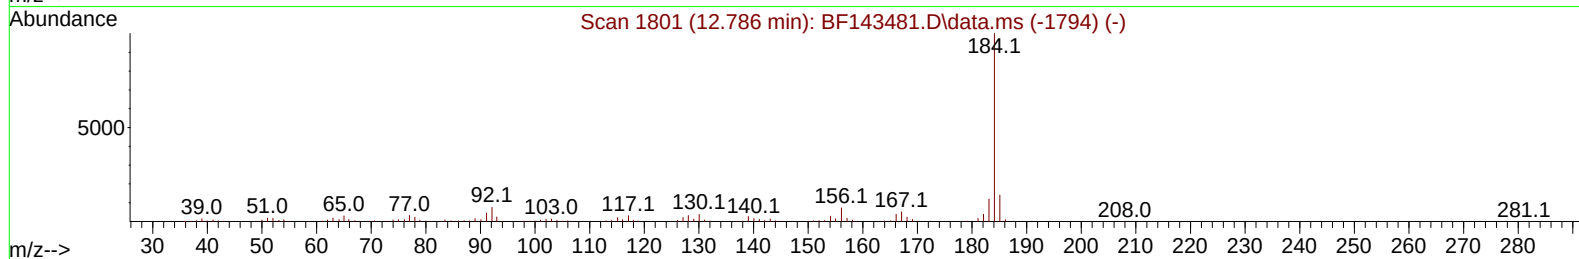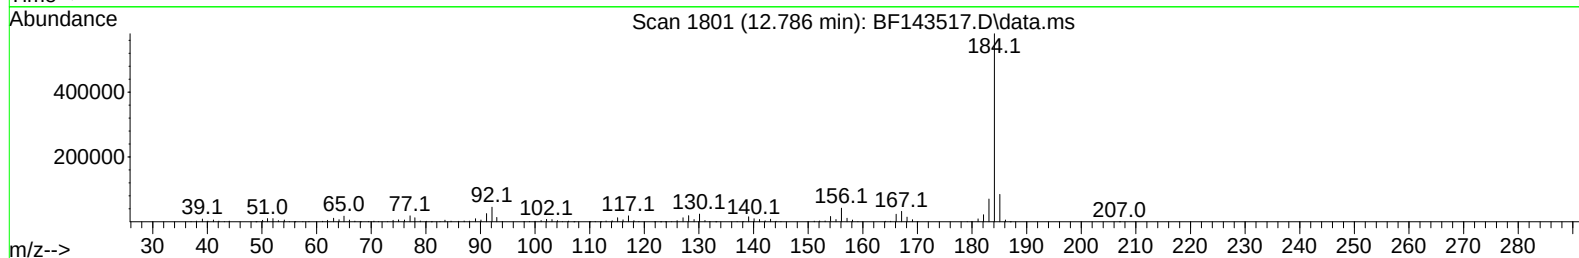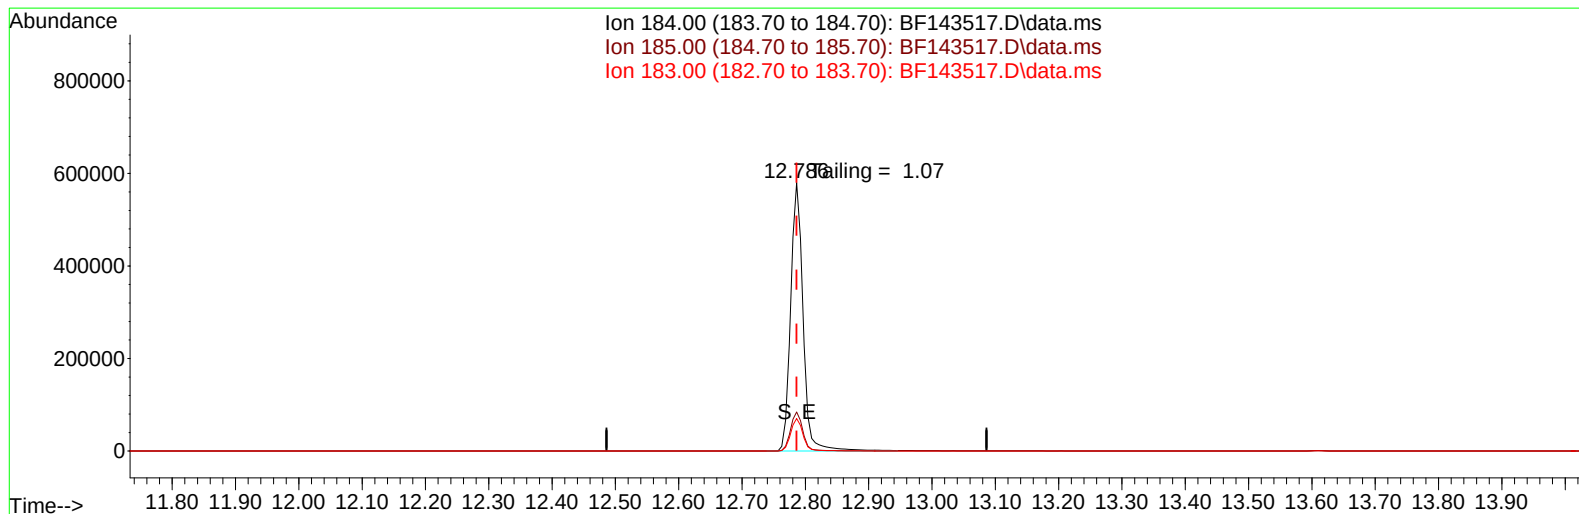

TIC: BF143517.D\data.ms

(77) Benzidine

12.786min (+ 0.000) 116738.94 ng

response 796205

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.54
183.00	11.90	12.13
0.00	0.00	0.00