
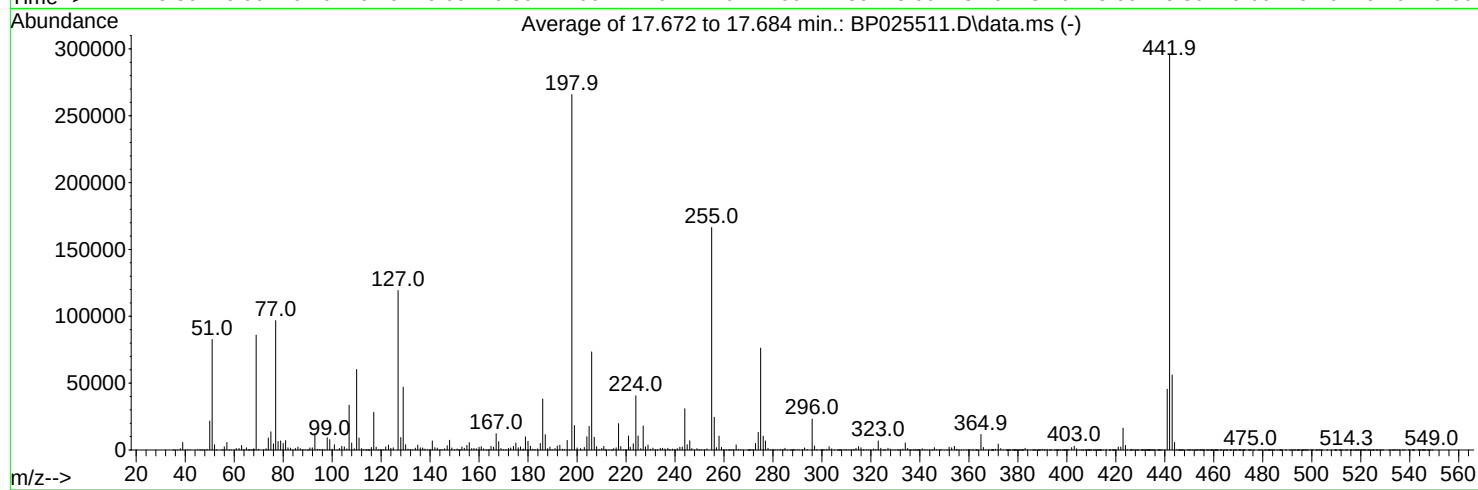


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025511.D
Acq On : 20 Aug 2025 17:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Aug 14 18:14:31 2025

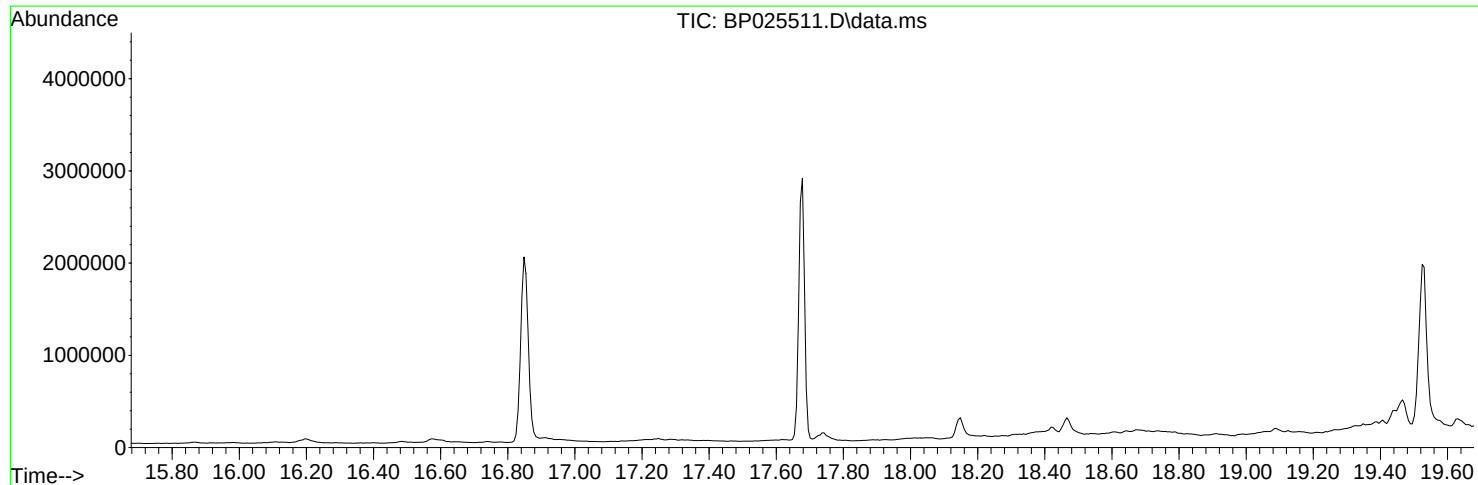




AutoFind: Scans 2505, 2506, 2507; Background Corrected with Scan 2494

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
68	69	0.00	2	1.1	967	PASS
69	69	100	100	100.0	85970	PASS
70	69	0.00	2	0.7	593	PASS
197	198	0.00	2	0.2	540	PASS
198	198	100	100	100.0	265973	PASS
199	198	5	9	6.9	18267	PASS
365	198	1	100	4.4	11643	PASS
441	443	0.01	150	80.9	45462	PASS
442	442	100	100	100.0	295314	PASS
443	442	15	24	19.0	56176	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025511.D
Acq On : 20 Aug 2025 17:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 21 01:41:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

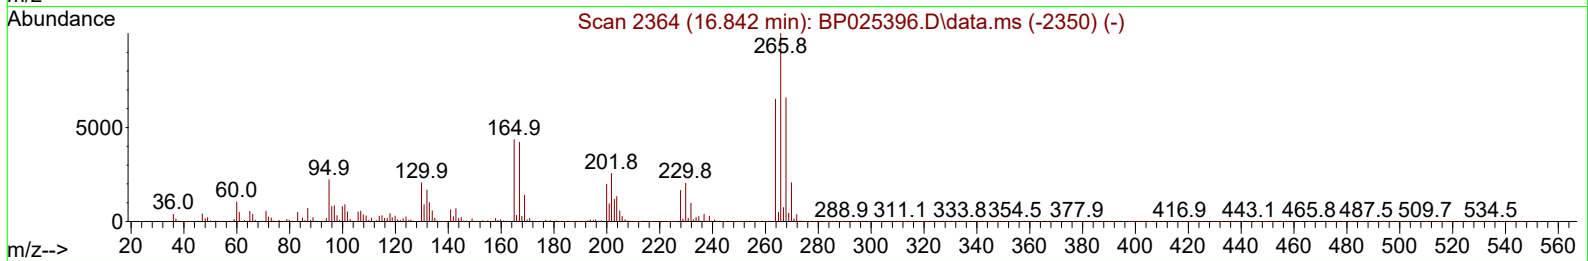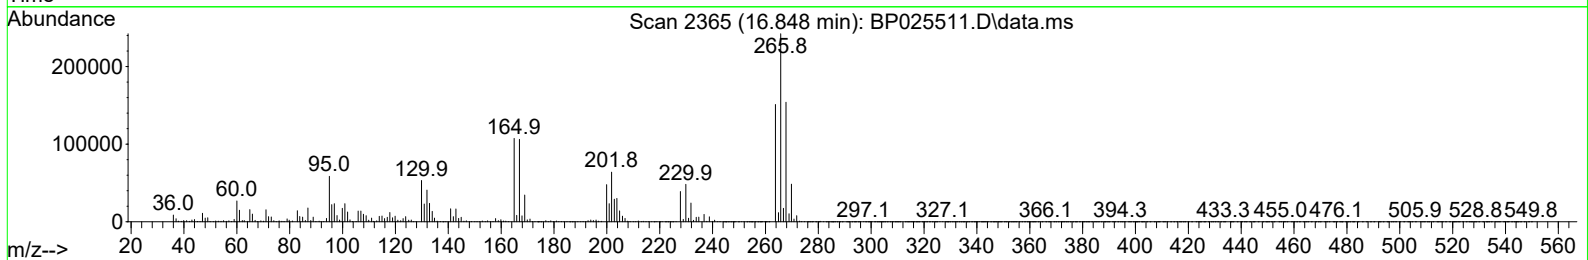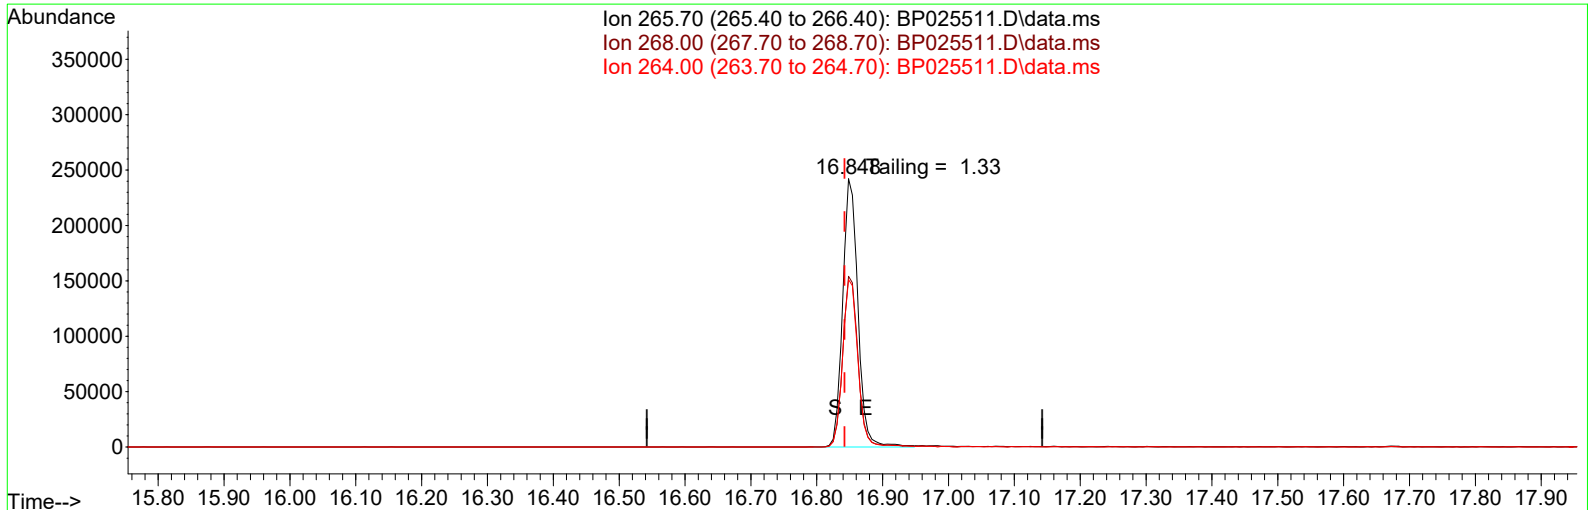

TIC: BP025511.D\data.ms

(70) Pentachlorophenol (C)

16.848min (+ 0.006) 19981.54 ng




response 390285

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	63.60
264.00	65.00	62.36
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP082025\
Data File : BP025511.D
Acq On : 20 Aug 2025 17:04
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 21 01:41:40 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP081425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Aug 14 18:14:31 2025
Response via : Initial Calibration

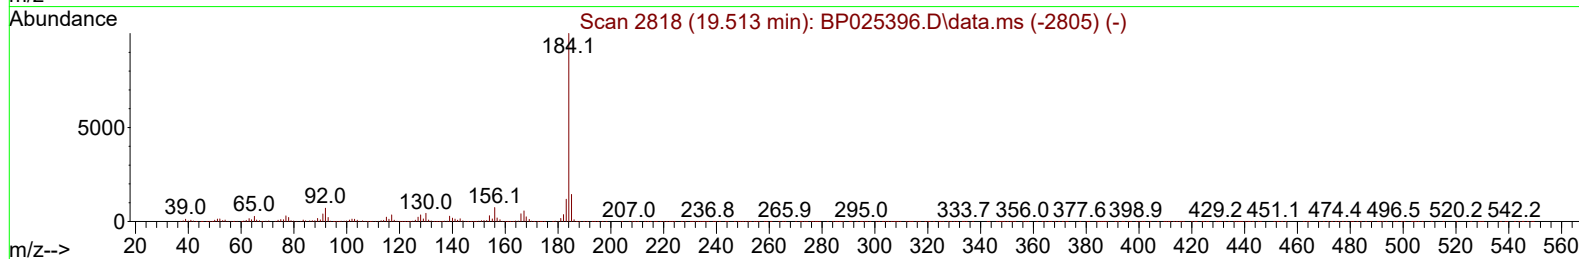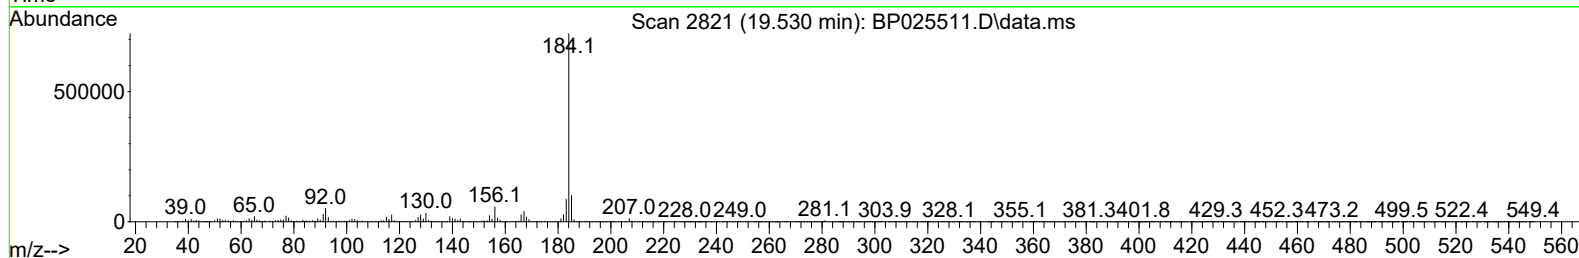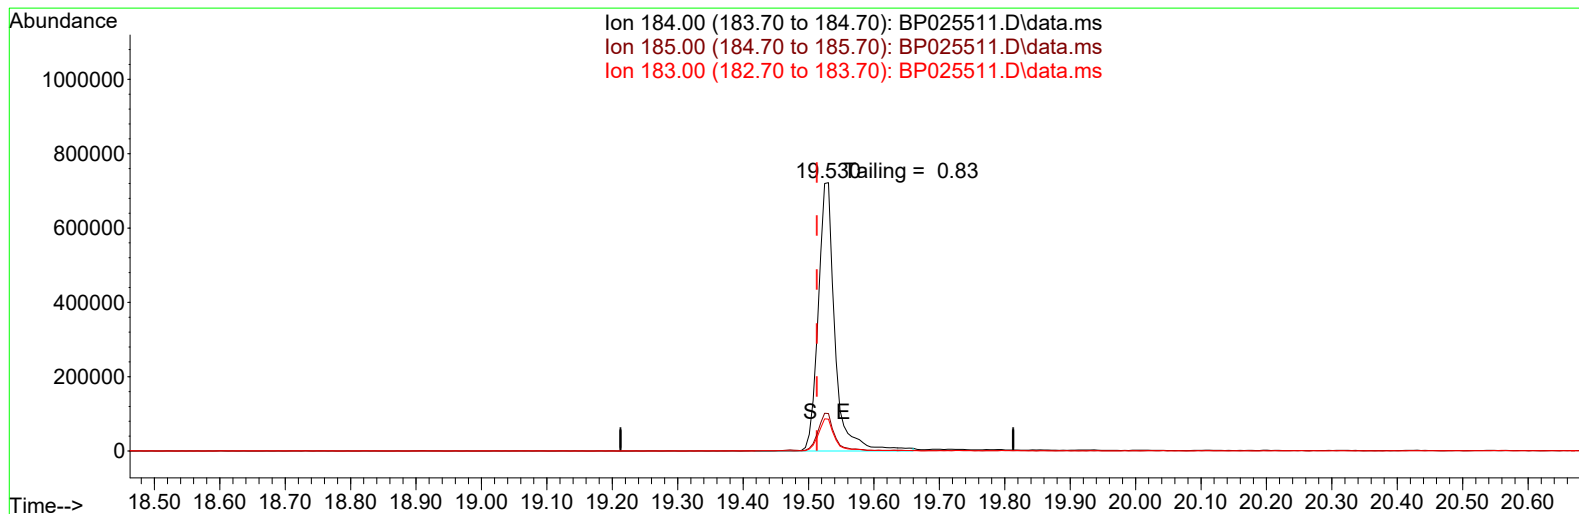

TIC: BP025511.D\data.ms

(77) Benzidine

19.530min (+ 0.018) 12499.23 ng

response 1286969

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.98
183.00	11.80	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/20/2025	BNA_P	<u>BP025511.D</u>
Compound Name	Response	Retention Time
DDT	1084945	20.825
DDD	23682	20.366
DDE	2473	19.836
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
26155	1111100	2.35

Instrument :
BNA_P
ClientSampleId :
DFTPP