


BFB

Data Path : Z:\voasrv\HPCHEM1\MSVOA_X\Data\VX081325\
Data File : VX047308.D
Acq On : 13 Aug 2025 08:30
Operator : JC/MD
Sample : BFB
Misc : 5.0mL/MSVOA_X/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_X
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_X\Method\82X072125W.M
Title : SW846 8260
Last Update : Tue Jul 22 03:59:51 2025

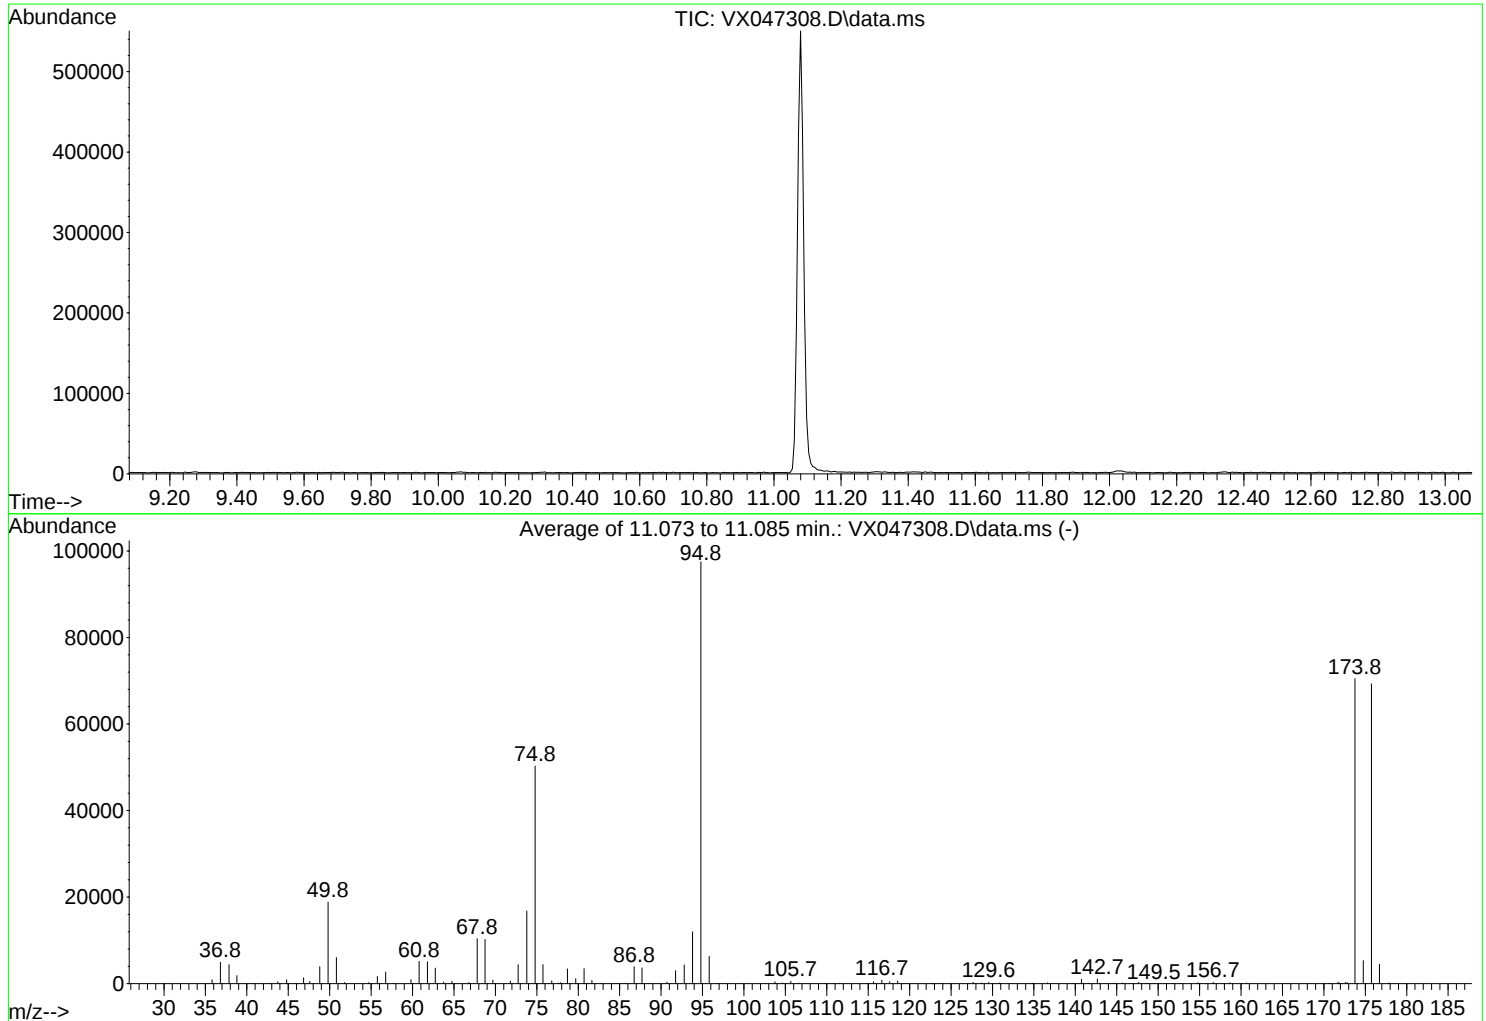

AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1632

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	18818	PASS
75	95	30	60	51.6	50309	PASS
95	95	100	100	100.0	97485	PASS
96	95	5	9	6.5	6306	PASS
173	174	0.00	2	0.4	267	PASS
174	95	50	100	72.3	70472	PASS
175	174	5	9	7.6	5338	PASS
176	174	95	101	98.4	69315	PASS
177	176	5	9	6.4	4463	PASS