
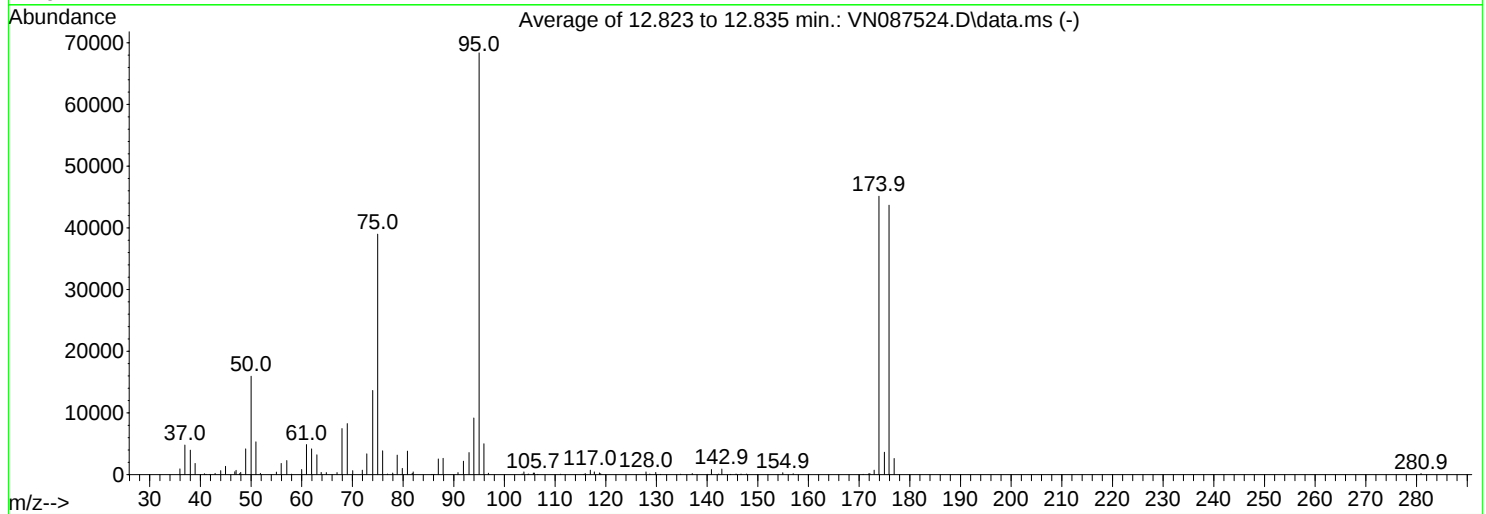


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN081325\
Data File : VN087524.D
Acq On : 13 Aug 2025 09:04
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N071625W.M
Title : SW846 8260
Last Update : Thu Jul 17 02:56:13 2025

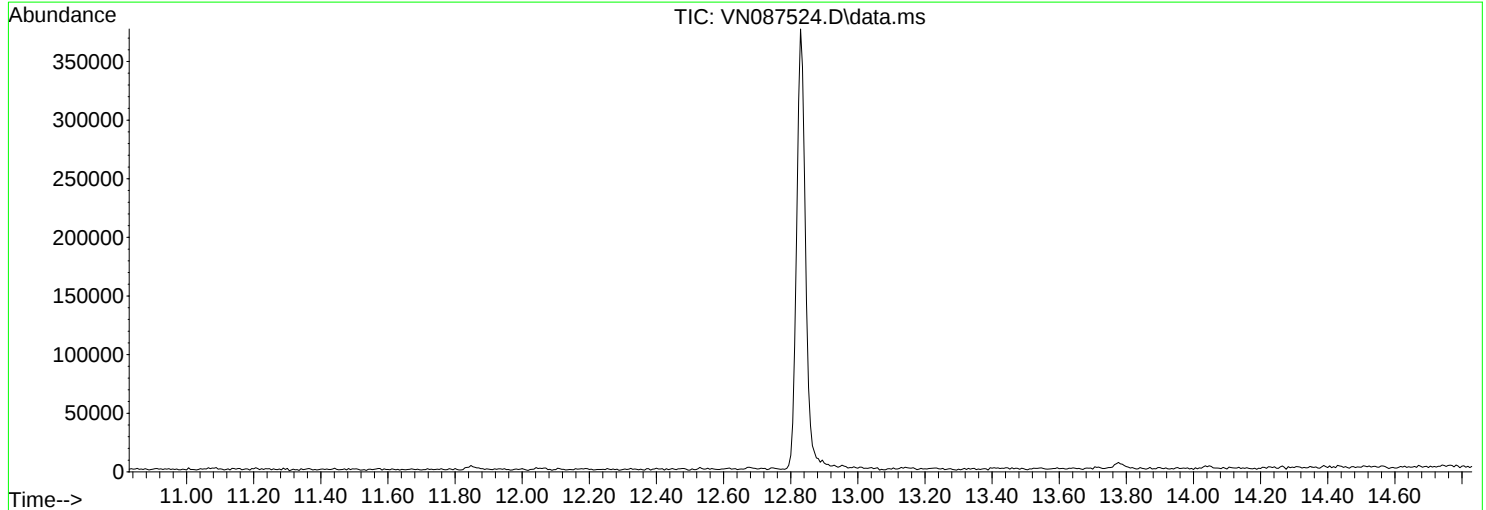

AutoFind: Scans 1848, 1849, 1850; Background Corrected with Scan 1840

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.3	15951	PASS
75	95	30	60	57.0	38971	PASS
95	95	100	100	100.0	68368	PASS
96	95	5	9	7.3	5004	PASS
173	174	0.00	2	1.6	725	PASS
174	95	50	100	66.0	45131	PASS
175	174	5	9	8.0	3631	PASS
176	174	95	101	96.8	43667	PASS
177	176	5	9	6.0	2620	PASS

Average of 12.823 to 12.835 min.: VN087524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	939	47.05	695	60.00	820	72.85	337
36.95	4796	47.70	146	60.95	4890	74.00	1363
38.00	3964	47.95	354	61.95	4189	75.00	3897
38.95	1822	48.95	4174	63.00	3227	75.95	385
40.80	160	50.00	15951	63.85	366	76.90	119
41.10	62	50.95	5325	64.85	333	77.95	271
41.90	66	51.85	201	66.95	342	78.85	3161
42.90	198	55.00	429	67.95	7476	79.85	1018
44.00	659	55.95	1827	69.00	8286	80.85	3806
44.95	1347	57.05	2293	70.05	640	81.80	206
46.80	478	58.00	88	71.95	719	82.00	441

Average of 12.823 to 12.835 min.: VN087524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.70	58	103.50	117	117.75	452	142.30	102
86.10	64	103.85	440	118.75	282	142.90	923
86.95	2549	104.60	61	119.00	170	144.60	58
87.90	2655	104.80	94	127.95	455	145.70	103
90.85	343	105.70	266	128.70	112	146.70	92
91.90	2172	105.90	249	129.85	354	147.80	110
93.00	3581	106.60	53	130.80	57	154.95	303
93.95	9181	111.10	71	134.80	76	157.00	148
95.00	68368	115.70	58	137.05	180	170.80	61
95.95	5004	115.95	192	140.10	67	171.90	139
96.85	227	116.95	716	140.85	824	172.10	184

Average of 12.823 to 12.835 min.: VN087524.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.95	725						
173.90	45131						
175.00	3631						
175.90	43667						
176.90	2620						
280.90	179						