
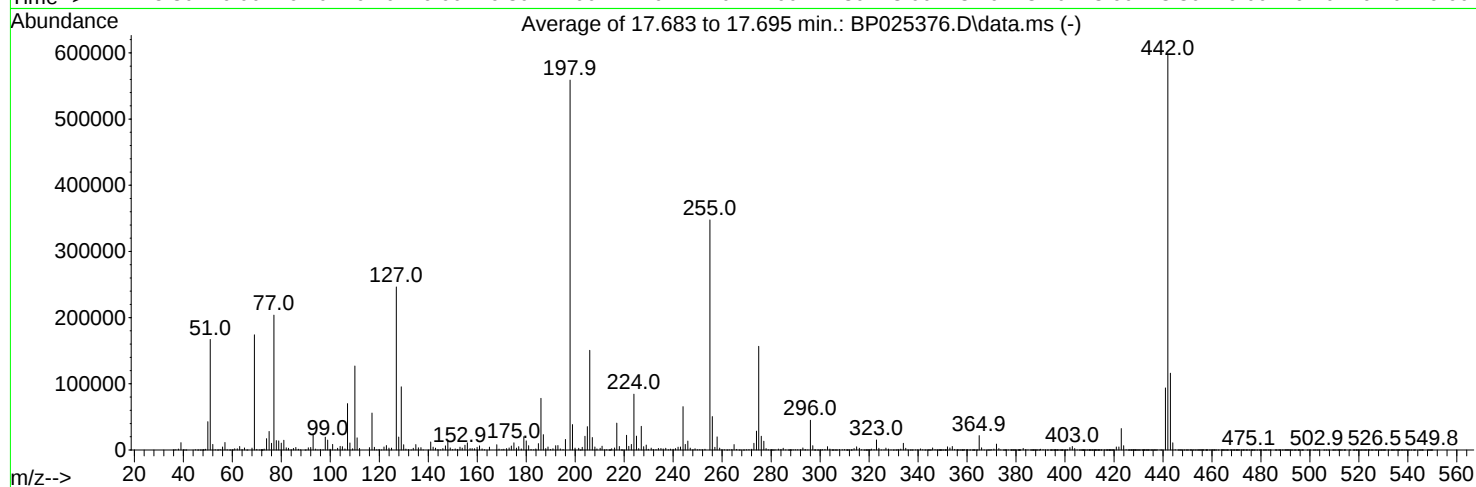


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081325\
Data File : BP025376.D
Acq On : 13 Aug 2025 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Aug 06 06:41:44 2025

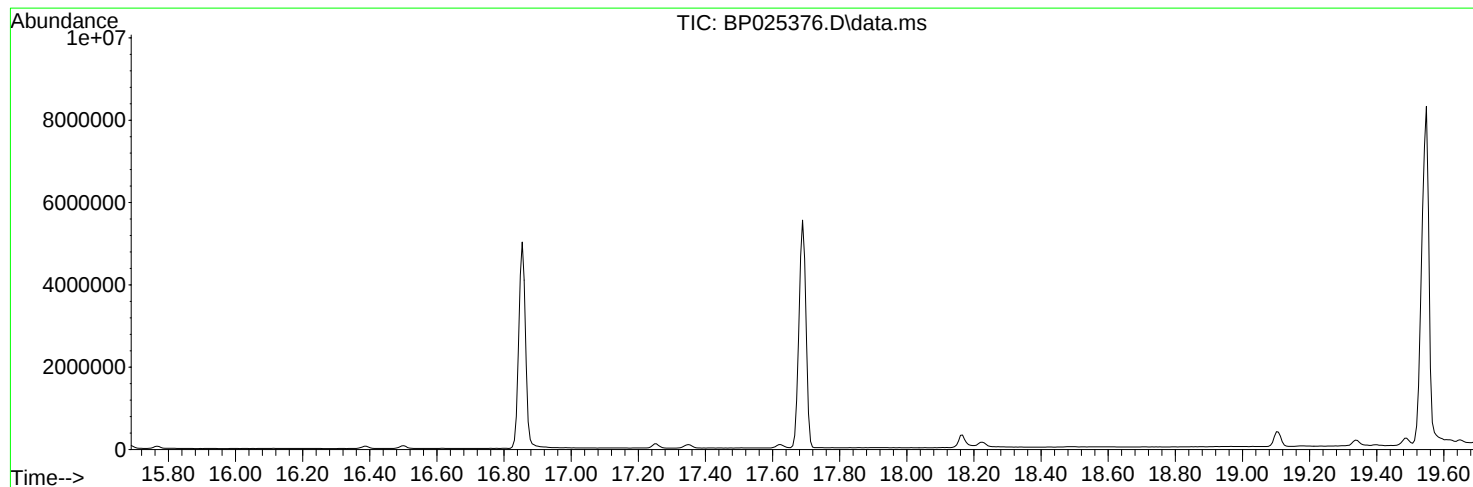




AutoFind: Scans 2507, 2508, 2509; Background Corrected with Scan 2496

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
68	69	0.00	2	1.7	3000	PASS
69	69	100	100	100.0	174059	PASS
70	69	0.00	2	0.5	948	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	559040	PASS
199	198	5	9	6.9	38448	PASS
365	198	1	100	3.9	21719	PASS
441	443	0.01	150	80.7	93704	PASS
442	442	100	100	100.0	596565	PASS
443	442	15	24	19.5	116141	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081325\
Data File : BP025376.D
Acq On : 13 Aug 2025 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 13 10:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

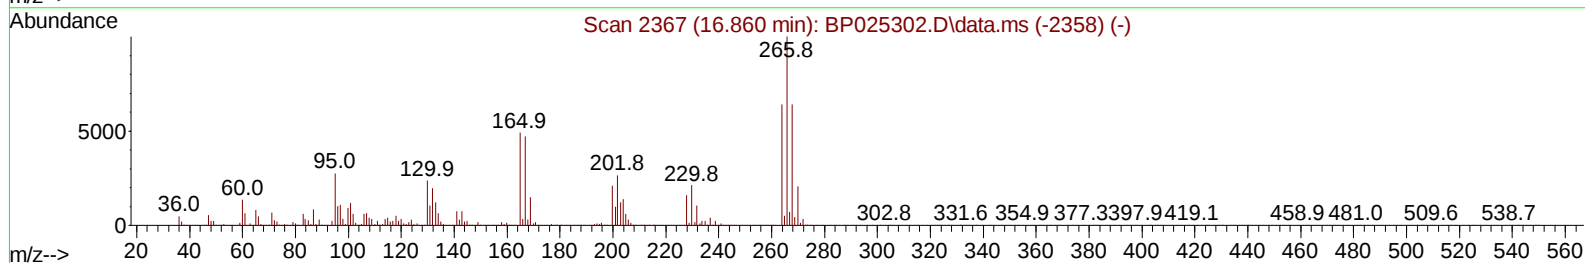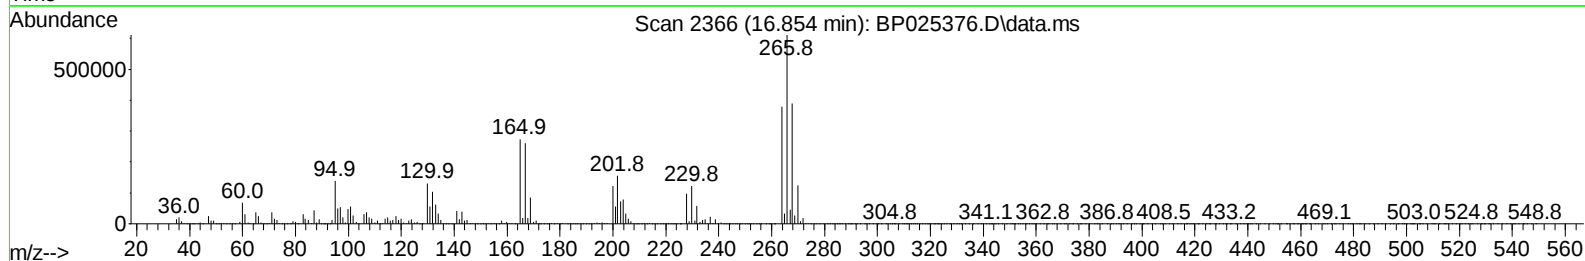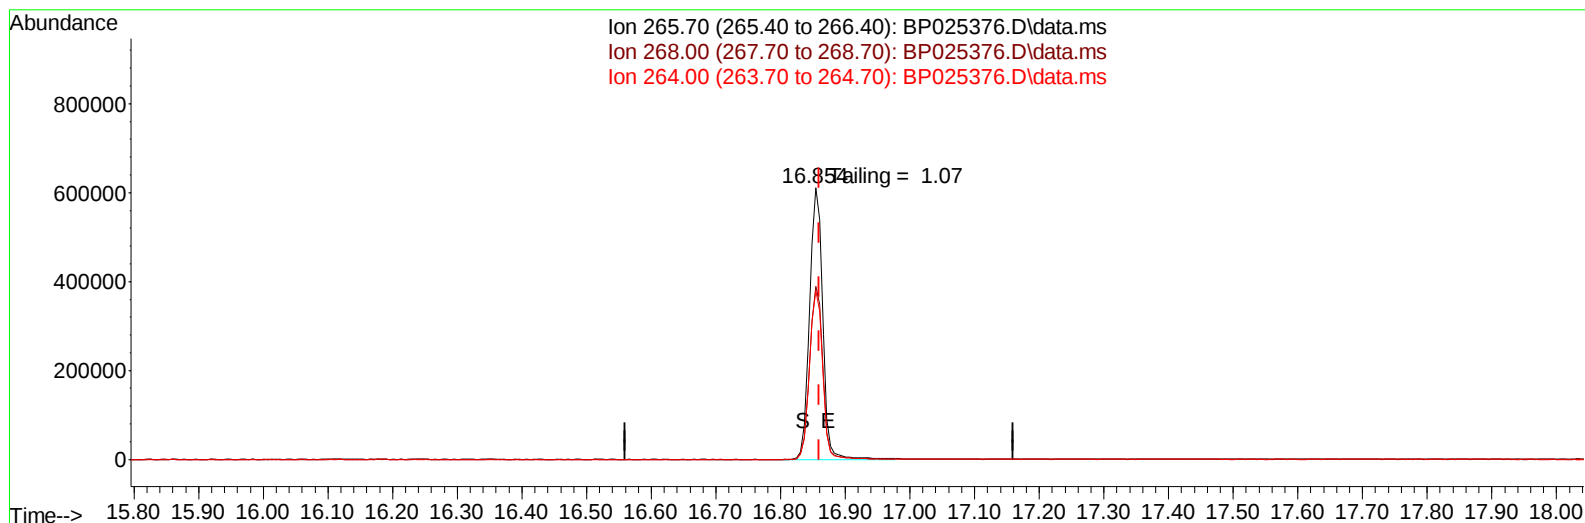

TIC: BP025376.D\data.ms

(70) Pentachlorophenol (C)

16.854min (-0.006) 72054.22 ng




response 872257

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.20	63.77
264.00	63.90	62.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP081325\
Data File : BP025376.D
Acq On : 13 Aug 2025 09:10
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Aug 13 10:45:46 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP080525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 06 06:41:44 2025
Response via : Initial Calibration

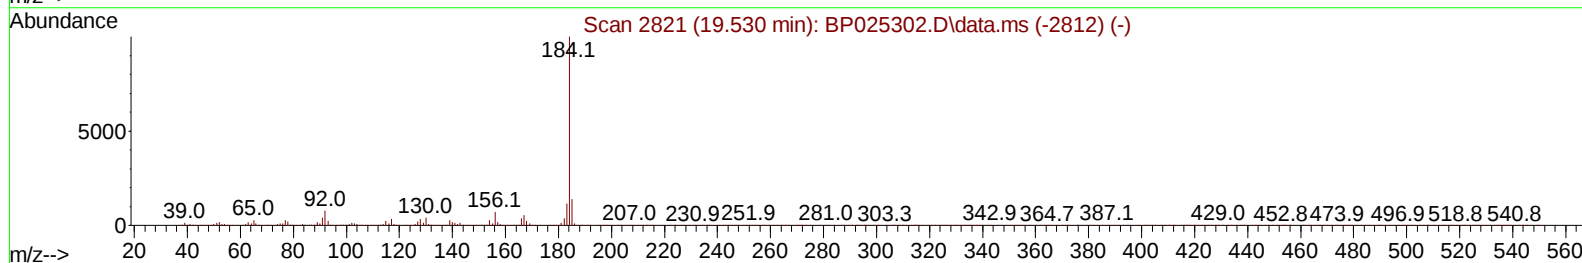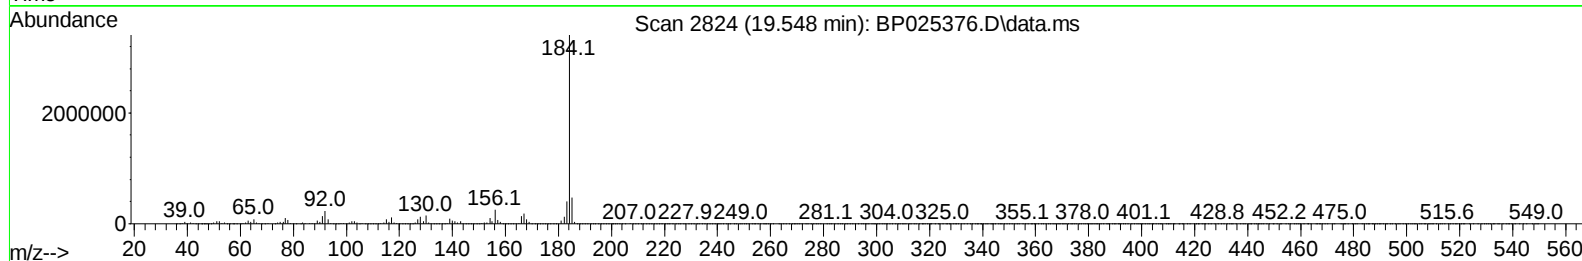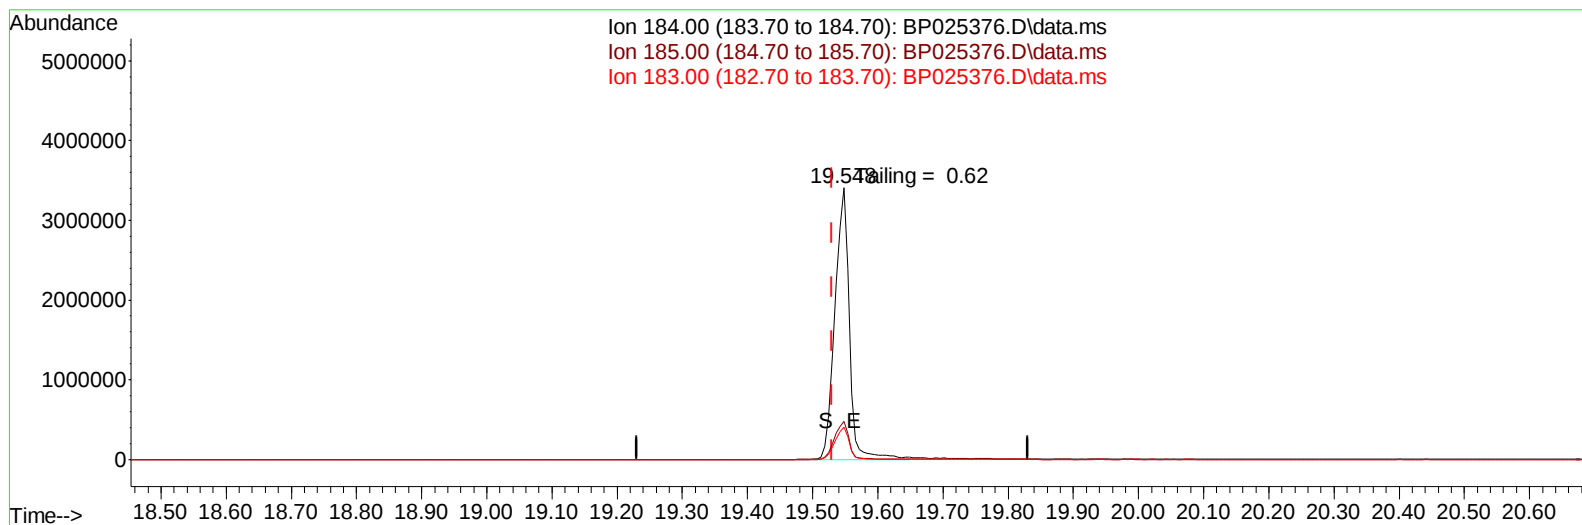

TIC: BP025376.D\data.ms

(77) Benzidine

19.548min (+ 0.018) 57458.25 ng

response 5292761

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.80	14.00
183.00	11.50	11.99
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/13/2025	BNA_P	<u>BP025376.D</u>
Compound Name	Response	Retention Time
DDT	2483175	20.842
DDD	51260	20.372
DDE	5330	19.848
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
56590	2539765	2.23

Instrument :
BNA_P
ClientSampleId :
DFTPP