

**DATA PACKAGE
GC SEMI-VOLATILES**

PROJECT NAME : USACE018-44 DOD

FIRST ENVIRONMENT, INC.

10 Park Place, Bldg 1A, Suite 504

Butler, NJ - 07405

Phone No: 973-334-0003

ORDER ID : Q2819

ATTENTION : Al Smith



Laboratory Certification ID # 20012

| | |
|--|------------|
| 1) PCB Data | 2 |
| 2) Signature Page | 4 |
| 3) Case Narrative | 5 |
| 4) Qualifier Page | 7 |
| 5) Conformance/Non Conformance | 8 |
| 6) QA Checklist | 10 |
| 7) Chronicle | 11 |
| 8) Hit Summary | 12 |
| 9) QC Data Summary For PCB | 13 |
| 9.1) Deuterated Monitoring Compound Summary | 14 |
| 9.2) MS/MSD Summary | 16 |
| 9.3) LCS/LCSD Summary | 18 |
| 9.4) Method Blank Summary | 19 |
| 10) Sample Data | 20 |
| 10.1) 11M-S | 21 |
| 10.2) 84SB-W | 25 |
| 10.3) 17M-W | 29 |
| 11) Calibration Data Summary | 33 |
| 11.1) Initial Calibration Data | 34 |
| 11.1.1) PO072325 | 34 |
| 11.1.2) PP080125 | 253 |
| 11.2) Continued Calibration Data | 408 |
| 11.2.1) PO112850.D | 408 |
| 11.2.2) PO112865.D | 420 |
| 11.2.3) PP074302.D | 432 |
| 11.2.4) PP074316.D | 444 |
| 11.3) Analytical Seq | 456 |
| 12) Compound Detection Summary | 460 |
| 13) QC Sample Data | 463 |
| 13.1) Method Blank Data | 464 |
| 13.2) PIBLK Data | 468 |
| 13.3) LCS Data | 492 |
| 13.4) MS Data | 501 |
| 13.5) MSD Data | 510 |
| 14) Manual Integration | 519 |



Table Of Contents for Q2819

| | | |
|------------------------|-----|----|
| 15) Analytical Runlogs | 530 | 1 |
| 16) Percent Solid | 548 | 2 |
| 17) Extraction Logs | 555 | 3 |
| 17.1) PB169205.pdf | 555 | 4 |
| 17.2) PB169205IC.pdf | 557 | 5 |
| 18) Standard Prep Logs | 558 | 6 |
| 19) Shipping Document | 644 | 7 |
| 19.1) Chain Of Custody | 645 | 8 |
| 19.2) Lab Certificate | 647 | 9 |
| 19.3) Internal COC | 648 | 10 |
| 20) Not Reviewed Data | 651 | 11 |
| | | 12 |
| | | 13 |
| | | 14 |
| | | 15 |
| | | 16 |
| | | 17 |
| | | 18 |
| | | 19 |
| | | 20 |

Cover Page

Order ID : Q2819

Project ID : USACE018-44 DOD

Client : First Environment, Inc.

Lab Sample Number

Q2819-01
Q2819-02
Q2819-03
Q2819-04
Q2819-05
Q2819-06
Q2819-07
Q2819-08
Q2819-09
Q2819-10
Q2819-11
Q2819-12
Q2819-13
Q2819-14
Q2819-15
Q2819-16
Q2819-17
Q2819-18
Q2819-19
Q2819-20

Client Sample Number

22BP-N
22BP-E
22BP-W
22BP-S
11M-W
11M-S
11M-N
11M-E
84SB-E
84SB-S
84SB-W
17M-S
17M-E
17M-W
17M-N
38M-S
38M-N
38M-W
38M-E
82H-E

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. Release of the data contained in this hard copy data package has been authorized by the laboratory manager or his designee, as verified by the following signature.

Signature : _____

Date: 8/18/2025

NYDOH CERTIFICATION NO - 11376

NJDEP CERTIFICATION NO - 20012

CASE NARRATIVE

First Environment, Inc.

Project Name: USACE018-44 DOD

Project # N/A

Order ID # Q2819

Test Name: PCB

A. Number of Samples and Date of Receipt:

20 Solid samples were received on 08/08/2025.

B. Parameters

According to the Chain of Custody document, the following analyses were requested:
PCB. This data package contains results for PCB.

C. Analytical Techniques:

The analyses were performed on instrument GCECD_P. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analyses were performed on instrument GCECD_O. The front column is ZB-MR1 which is 30 meters, 0.32 mm ID, 0.5 um df, Catalogue # 7HM-G016-17. The rear column is ZB-MR2 which is 30 meters, 0.32 mm ID, 0.25 µm; Catalogue # 7HM-G017-11. The analysis of PCBs was based on method 8082A and extraction was done based on method 3541.

D. QA/ QC Samples:

The Holding Times were met for all analysis.

The Surrogate recoveries were met for all analysis except for 84SB-W [Decachlorobiphenyl(1)59%]AS per method one surrogate allowed to fail to meet the criteria per column, No further corrective action was taken.

The Retention Times were met for all analysis.

The MS recoveries met the requirements for all compounds.

The MSD recoveries met the requirements for all compounds.

The RPD were met for all analysis.

The Blank Spike met requirements for all compounds.

The Blank analysis did not indicate the presence of lab contamination.

The Initial Calibration met the requirements.

The Continuous Calibration File ID PO112850.D met the requirements except for Aroclor-1016(Peak-01),Tetrachloro-m-xylene is failing in 1st column however it is passing in 2nd column therefore no corrective action taken.



284 Sheffield Street, Mountainside, NJ 07092
Phone: 908 789 8900 Fax: 908 789 8922

The Continuous Calibration File ID PP074302.D met the requirements except for Aroclor-1016(Peak-02),Tetrachloro-m-xylene is failing in 2nd column however it is passing in 1st column therefore no corrective action taken.

E. Additional Comments:

The not QT review data is reported in the Miscellaneous.

The soil samples results are based on a dry weight basis.

F. Manual Integration Comments:

Please refer to the Manual integration Report included with the Run Logs for information on the manual integrations performed.

I certify that the data package is in compliance with the terms and conditions of the contract, both technically and for completeness, for other than the conditions detailed above. The laboratory manager or his designee, as verified by the following signature has authorized release of the data contained in this hard copy data package.

Signature_____

DATA REPORTING QUALIFIERS- ORGANIC

For reporting results, the following "Results Qualifiers" are used:

- Value** If the result is a value greater than or equal to the detection limit, report the value
- U** Indicates the compound was analyzed for but was not detected. Report the minimum detection limit for the sample with the U, i.e. "10 U". This is not necessarily the instrument detection limit attainable for this particular sample based on any concentration or dilution that may have been required.
- ND** Indicates the analyte was analyzed for, but not detected
- J** Indicates an estimated value. This flag is used:
(1) When estimating a concentration for a tentatively identified compound (library search hits, where a 1:1 response is assumed.)
(2) When the mass spectral data indicated the identification, however the result was less than the specified detection limit greater than zero. If the detection limit was 10ug/L and a concentration of 3 ug/L was calculated report as 3 J. This flag is used when similar situation arise on any organic parameter i.e. Pest, PCB and others.
- B** Indicates the analyte was found in the blank as well as the sample report as "12 B".
- E** Indicates the analyte's concentration exceeds the calibrated range of the instrument for that specific analysis.
- D** This flag identifies all compounds identified in an analysis at a secondary dilution factor.
- P** This flag is used for Pesticide/PCB target analyte when there is >25% difference for detected concentrations between the two GC columns. The lower of the two values is reported on Form 1 and flagged with a "P".
- N** This flag indicates presumptive evidence of a compound. This is only used for tentatively identified compounds (TICs), where the identification is based on a mass spectral library search. It applies to all TIC results. For generic characterization of a TIC, such as chlorinated hydrocarbon, the flag is not used.
- A** This flag indicates that a Tentatively Identified Compound is a suspected aldol-condensation product.
- Q** Indicates the LCS did not meet the control limits requirements



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY

ORDER ID: Q2819

MATRIX: Solid

METHOD: 8082A/3541

| | NA | NO | YES |
|---|----|----|-----|
| 1. Chromatograms Labeled/Compounds Identified. | | | ✓ |
| 2. Standard Summary Submitted. | | | ✓ |
| 3. Calibration - Initial Calibration performed within 30 days before sample analysis and continuing calibration performed within 24 hours of sample analysis, 12 HOURS IF 8000 SERIES METHOD. | | | ✓ |

The Initial Calibration met the requirements.

The Continuous Calibration File ID PO112850.D met the requirements except for Aroclor-1016(Peak-01),Tetrachloro-m-xylene is failing in 1st column however it is passing in 2nd column therefore no corrective action taken.

The Continuous Calibration File ID PP074302.D met the requirements except for Aroclor-1016(Peak-02),Tetrachloro-m-xylene is failing in 2nd column however it is passing in 1st column therefore no corrective action taken.

| | |
|---|---|
| 4. Blank Contamination - If yes, list compounds and concentrations in each blank: | ✓ |
| 5. Surrogate Recoveries Meet Criteria | ✓ |

If not met, list those compounds and their recoveries which fall outside the acceptable ranges.

The Surrogate recoveries were met for all analysis except for 84SB-W [Decachlorobiphenyl(1)59%]AS per method one surrogate allowed to fail to meet the criteria per column, No further corrective action was taken.

| | |
|--|---|
| 6. Matrix Spike/Matrix Spike Duplicate Recoveries Meet Criteria | ✓ |
| If not met, list those compounds and their recoveries which fall outside the acceptable range. | |

The MS recoveries met the requirements for all compounds.

The MSD recoveries met the requirements for all compounds.

The Blank Spike met requirements for all compounds.

The RPD were met for all analysis.

| | |
|---|---|
| 7. Retention Time Shift Meet Criteria (if applicable) | ✓ |
| Comments: | |



284 Sheffield Street, Mountainside, NJ 07092 Phone: 908 789 8900 Fax: 908 789 8922

GC ANALYSIS CONFORMANCE/NON-CONFORMANCE SUMMARY (CONTINUED)

| | NA | NO | YES |
|--|----|----|-----|
| 8. Extraction Holding Time Met | | | ✓ |
| If not met, list number of days exceeded for each sample: | | | |
| 9. Analysis Holding Time Met | | | ✓ |
| If not met, list those compounds and their recoveries which fall outside the acceptable range. | | | |

ADDITIONAL COMMENTS:

The not QT review data is reported in the Miscellaneous.

The soil samples results are based on a dry weight basis.

QA REVIEW

Date

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

APPENDIX A

QA REVIEW GENERAL DOCUMENTATION

Project #: Q2819

Completed

For thorough review, the report must have the following:

GENERAL:

Are all original paperwork present (chain of custody, record of communication, airbill, sample management lab chronicle, login page) ✓

Check chain-of-custody for proper relinquish/return of samples ✓

Is the chain of custody signed and complete ✓

Check internal chain-of-custody for proper relinquish/return of samples /sample extracts ✓

Collect information for each project id from server. Were all requirements followed ✓

COVER PAGE:

Do numbers of samples correspond to the number of samples in the Chain of Custody on login page ✓

Do lab numbers and client Ids on cover page agree with the Chain of Custody ✓

CHAIN OF CUSTODY:

Do requested analyses on Chain of Custody agree with form I results ✓

Do requested analyses on Chain of Custody agree with the log-in page ✓

Were the correct method log-in for analysis according to the Analytical Request and Chain of Castody ✓

Were the samples received within hold time ✓

Were any problems found with the samples at arrival recorded in the Sample Management Laboratory Chronicle ✓

ANALYTICAL:

Was method requirement followed? ✓

Was client requirement followed? ✓

Does the case narrative summarize all QC failure? ✓

All runlogs and manual integration are reviewed for requirements ✓

All manual calculations and /or hand notations verified ✓

QA Review Signature: SOHIL JODHANI

Date: 08/18/2025

LAB CHRONICLE

| | | | |
|-----------------|-------------------------|-------------------|-----------------------|
| OrderID: | Q2819 | OrderDate: | 8/11/2025 12:06:00 PM |
| Client: | First Environment, Inc. | Project: | USACE018-44 DOD |
| Contact: | Al Smith | Location: | D31,VOA Ref. #2 Soil |

| LabID | ClientID | Matrix | Test | Method | Sample Date | Prep Date | Anal Date | Received |
|----------|----------|--------|------|--------|-------------|-----------|-----------|----------|
| Q2819-06 | 11M-S | SOIL | | | 08/05/25 | | | 08/08/25 |
| | | | PCB | 8082A | | 08/12/25 | 08/12/25 | |
| Q2819-11 | 84SB-W | SOIL | | | 08/05/25 | | | 08/08/25 |
| | | | PCB | 8082A | | 08/12/25 | 08/12/25 | |
| Q2819-14 | 17M-W | SOIL | | | 08/05/25 | | | 08/08/25 |
| | | | PCB | 8082A | | 08/12/25 | 08/12/25 | |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Hit Summary Sheet
SW-846

SDG No.: Q2819

Order ID: Q2819

Client: First Environment, Inc.

Project ID: USACE018-44 DOD

| Sample ID | Client ID | Matrix | Parameter | Concentration | C | MDL | LOD | RDL | Units |
|-----------|-----------|--------|-----------|---------------|---|-----|-----|-----|-------|
|-----------|-----------|--------|-----------|---------------|---|-----|-----|-----|-------|

Client ID :

Total Concentration: 0.000

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



QC

SUMMARY

Surrogate Summary

SDG No.: Q2819

Client: First Environment, Inc.

Analytical Method: 8082A

| Lab Sample ID | Client ID | Parameter | Column | Spike | Result | Recovery(%) | Qual | Limits(%) | |
|------------------|--------------------------|-------------------|--------|-------|--------|-------------|------|-----------|------|
| | | | | | | | | Low | High |
| I.BLK-PO112413.D | PIBLK-PO112413.D | Tetrachloro-m-xyl | 1 | 20 | 19.1 | 95 | | 60 | 140 |
| | | Decachlorobiphen | 1 | 20 | 20.0 | 100 | | 60 | 140 |
| | | Tetrachloro-m-xyl | 2 | 20 | 19.5 | 98 | | 60 | 140 |
| | | Decachlorobiphen | 2 | 20 | 20.4 | 102 | | 60 | 140 |
| I.BLK-PO112854.D | PIBLK-PO112854.D | Tetrachloro-m-xyl | 1 | 20 | 20.9 | 105 | | 60 | 140 |
| | | Decachlorobiphen | 1 | 20 | 17.2 | 86 | | 60 | 140 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.5 | 102 | | 60 | 140 |
| | | Decachlorobiphen | 2 | 20 | 20.4 | 102 | | 60 | 140 |
| Q2819-06 | 11M-S | Tetrachloro-m-xyl | 1 | 20 | 21.6 | 108 | | 44 | 130 |
| | | Decachlorobiphen | 1 | 20 | 12.8 | 64 | | 60 | 125 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.6 | 103 | | 44 | 130 |
| | | Decachlorobiphen | 2 | 20 | 15.2 | 76 | | 60 | 125 |
| Q2819-11 | 84SB-W | Tetrachloro-m-xyl | 1 | 20 | 21.4 | 107 | | 44 | 130 |
| | | Decachlorobiphen | 1 | 20 | 11.9 | 59 | * | 60 | 125 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.5 | 103 | | 44 | 130 |
| | | Decachlorobiphen | 2 | 20 | 14.2 | 71 | | 60 | 125 |
| Q2819-14 | 17M-W | Tetrachloro-m-xyl | 1 | 20 | 21.4 | 107 | | 44 | 130 |
| | | Decachlorobiphen | 1 | 20 | 12.4 | 62 | | 60 | 125 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.4 | 102 | | 44 | 130 |
| | | Decachlorobiphen | 2 | 20 | 13.8 | 69 | | 60 | 125 |
| I.BLK-PO112869.D | PIBLK-PO112869.D | Tetrachloro-m-xyl | 1 | 20 | 20.7 | 103 | | 60 | 140 |
| | | Decachlorobiphen | 1 | 20 | 19.2 | 96 | | 60 | 140 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.3 | 102 | | 60 | 140 |
| | | Decachlorobiphen | 2 | 20 | 20.5 | 103 | | 60 | 140 |
| I.BLK-PP074167.D | PIBLK-PP074167.D | Tetrachloro-m-xyl | 1 | 20 | 19.1 | 95 | | 60 | 140 |
| | | Decachlorobiphen | 1 | 20 | 19.7 | 98 | | 60 | 140 |
| | | Tetrachloro-m-xyl | 2 | 20 | 17.3 | 86 | | 60 | 140 |
| | | Decachlorobiphen | 2 | 20 | 18.7 | 93 | | 60 | 140 |
| I.BLK-PP074305.D | PIBLK-PP074305.D | Tetrachloro-m-xyl | 1 | 20 | 22.0 | 110 | | 60 | 140 |
| | | Decachlorobiphen | 1 | 20 | 21.1 | 105 | | 60 | 140 |
| | | Tetrachloro-m-xyl | 2 | 20 | 19.7 | 98 | | 60 | 140 |
| | | Decachlorobiphen | 2 | 20 | 18.5 | 93 | | 60 | 140 |
| PB169205BL | PB169205BL | Tetrachloro-m-xyl | 1 | 20 | 23.1 | 116 | | 44 | 130 |
| | | Decachlorobiphen | 1 | 20 | 22.2 | 111 | | 60 | 125 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.1 | 101 | | 44 | 130 |
| | | Decachlorobiphen | 2 | 20 | 20.1 | 100 | | 60 | 125 |
| PB169205BS | PB169205BS | Tetrachloro-m-xyl | 1 | 20 | 24.3 | 121 | | 44 | 130 |
| | | Decachlorobiphen | 1 | 20 | 22.5 | 112 | | 60 | 125 |
| | | Tetrachloro-m-xyl | 2 | 20 | 20.8 | 104 | | 44 | 130 |
| | | Decachlorobiphen | 2 | 20 | 20.0 | 100 | | 60 | 125 |
| Q2830-01MS | BIN0009-DRIVEWAY-TP-SOUT | Tetrachloro-m-xyl | 1 | 20 | 23.5 | 117 | | 44 | 130 |

Surrogate Summary

SDG No.: **Q2819**

Client: **First Environment, Inc.**

Analytical Method: **8082A**

| Lab Sample ID | Client ID | Parameter | Column | Spike | Result | Recovery(%) | Qual | Limits(%) | Low | High |
|------------------|--------------------------|-------------------|--------|-------|--------|-------------|------|-----------|-----|------|
| Q2830-01MS | BIN0009-DRIVEWAY-TP-SOUT | Decachlorobiphen | 1 | 20 | 19.9 | 100 | | 60 | 125 | |
| | | Tetrachloro-m-xyl | 2 | 20 | 22.0 | 110 | | 44 | 130 | |
| | | Decachlorobiphen | 2 | 20 | 17.5 | 87 | | 60 | 125 | |
| Q2830-01MSD | BIN0009-DRIVEWAY-TP-SOUT | Tetrachloro-m-xyl | 1 | 20 | 23.3 | 116 | | 44 | 130 | |
| | | Decachlorobiphen | 1 | 20 | 19.9 | 99 | | 60 | 125 | |
| | | Tetrachloro-m-xyl | 2 | 20 | 22.1 | 111 | | 44 | 130 | |
| | | Decachlorobiphen | 2 | 20 | 17.9 | 89 | | 60 | 125 | |
| I.BLK-PP074319.D | PIBLK-PP074319.D | Tetrachloro-m-xyl | 1 | 20 | 22.9 | 115 | | 60 | 140 | |
| | | Decachlorobiphen | 1 | 20 | 21.7 | 109 | | 60 | 140 | |
| | | Tetrachloro-m-xyl | 2 | 20 | 19.8 | 99 | | 60 | 140 | |
| | | Decachlorobiphen | 2 | 20 | 19.8 | 99 | | 60 | 140 | |

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q2819
Client: First Environment, Inc.

Analytical Method: 8082A
DataFile : PP074311.D

| | Parameter | Spike | Sample Result | Result | Units | Rec | Rec Qual | RPD | RPD Qual | Limits Low | Limits High | RPD |
|-----------------------|----------------------------------|-------|--------------------------|-----------------------------|-------|-----|----------|-----|----------|------------|-------------|-----|
| Lab Sample ID: | Q2830-01MS (Column 1) | | Client Sample ID: | BIN0009-DRIVEWAY-TP- | | | | | | | | |
| | AR1016 | 191.7 | 0 | 201 | ug/kg | 105 | | | | 47 | 134 | |
| | AR1260 | 191.7 | 0 | 173 | ug/kg | 90 | | | | 53 | 140 | |
| Lab Sample ID: | Q2830-01MS (Column 2) | | Client Sample ID: | BIN0009-DRIVEWAY-TP- | | | | | | | | |
| | AR1016 | 191.7 | 0 | 213 | ug/kg | 111 | | | | 47 | 134 | |
| | AR1260 | 191.7 | 0 | 181 | ug/kg | 94 | | | | 53 | 140 | |

Matrix Spike/Matrix Spike Duplicate Summary

SW-846

SDG No.: Q2819
Client: First Environment, Inc.

Analytical Method: 8082A
DataFile : PP074312.D

| | Parameter | Spike | Sample Result | Result | Units | Rec | Rec Qual | RPD | RPD Qual | Limits | Low | High | RPD |
|-----------------------|-----------------------------------|-------|--------------------------|-----------------------------|-------|-----|----------|-----|----------|--------|-----|------|-----|
| Lab Sample ID: | Q2830-01MSD (Column 1) | | Client Sample ID: | BIN0009-DRIVEWAY-TP- | | | | | | | | | |
| | AR1016 | 191.6 | 0 | 213 | ug/kg | 111 | | 6 | | 47 | 134 | 20 | |
| | AR1260 | 191.6 | 0 | 177 | ug/kg | 92 | | 2 | | 53 | 140 | 20 | |
| Lab Sample ID: | Q2830-01MSD (Column 2) | | Client Sample ID: | BIN0009-DRIVEWAY-TP- | | | | | | | | | |
| | AR1016 | 191.6 | 0 | 219 | ug/kg | 114 | | 3 | | 47 | 134 | 20 | |
| | AR1260 | 191.6 | 0 | 188 | ug/kg | 98 | | 4 | | 53 | 140 | 20 | |

Laboratory Control Sample/Laboratory Control Sample Duplicate Summary

SW-846

SDG No.: Q2819

Analytical Method: 8082A

Client: First Environment, Inc.

Datafile : PP074309.D

| Lab Sample ID | Parameter | Spike | Result | Units | Rec | RPD | RPD | | Limits | | |
|--------------------------|-----------|-------|--------|-------|-----|-----|------|------|--------|------|--|
| | | | | | | | Qual | Qual | Low | High | |
| PB169205BS (Column 1) | AR1016 | 166.6 | 185 | ug/kg | 111 | | | | 47 | 134 | |
| | AR1260 | 166.6 | 165 | ug/kg | 99 | | | | 53 | 140 | |
| PB169205BS (Column 2) | AR1016 | 166.6 | 183 | ug/kg | 110 | | | | 47 | 134 | |
| | AR1260 | 166.6 | 180 | ug/kg | 108 | | | | 53 | 140 | |

4C

PESTICIDE METHOD BLANK SUMMARY

Client ID

PB169205BL

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Lab Sample ID: PB169205BL

Lab File ID: PP074308.D

Matrix: (soil/water) Solid

Extraction: (Type) SOXH

Sulfur Cleanup: (Y/N) N

Date Extracted: 08/12/2025

Date Analyzed (1): 08/12/2025

Date Analyzed (2): 08/12/2025

Time Analyzed (1): 12:48

Time Analyzed (2): 12:48

Instrument ID (1): ECD_P

Instrument ID (2): ECD_P

GC Column (1): ZB-MR1 ID: 0.32 (mm) GC Column (2): ZB-MR2 ID: 0.32 (mm)

THIS METHOD BLANK APPLIES TO THE FOLLOWING SAMPLES, MS AND MSD:

| EPA SAMPLE NO. | LAB SAMPLE ID | LAB FILE ID | DATE ANALYZED 1 | DATE ANALYZED 2 |
|-----------------------------------|------------------|----------------|--------------------|--------------------|
| 11M-S | Q2819-06 | PO112860.D | 08/12/2025 | 08/12/2025 |
| 84SB-W | Q2819-11 | PO112861.D | 08/12/2025 | 08/12/2025 |
| 17M-W | Q2819-14 | PO112862.D | 08/12/2025 | 08/12/2025 |
| PB169205BS | PB169205BS | PP074309.D | 08/12/2025 | 08/12/2025 |
| BIN0009-DRIVEWAY-TP-SOUTH-EASTMS | Q2830-01MS | PP074311.D | 08/12/2025 | 08/12/2025 |
| BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD | Q2830-01MSD | PP074312.D | 08/12/2025 | 08/12/2025 |

COMMENTS:



SAMPLE

DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | |
|--------------------|-------------------------|--------|---|--------------------|----------|-----------|
| Client: | First Environment, Inc. | | | Date Collected: | 08/05/25 | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/08/25 | |
| Client Sample ID: | 11M-S | | | SDG No.: | Q2819 | |
| Lab Sample ID: | Q2819-06 | | | Matrix: | SOIL | |
| Analytical Method: | 8082A | | | % Solid: | 90.5 | Decanted: |
| Sample Wt/Vol: | 30.05 | Units: | g | Final Vol: | 10000 | uL |
| Soil Aliquot Vol: | uL | | | Test: | PCB | |
| Extraction Type: | | | | Injection Volume : | | |
| GPC Factor : | 1.0 | PH : | | | | |
| Prep Method : | SW3541B | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PO112860.D | 1 | 08/12/25 08:15 | 08/12/25 13:26 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 9.20 | U | 4.40 | 9.20 | 18.8 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 14.3 | U | 4.40 | 14.3 | 18.8 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 9.20 | U | 4.10 | 9.20 | 18.8 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 9.20 | U | 4.40 | 9.20 | 18.8 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 14.3 | U | 6.50 | 14.3 | 18.8 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 9.20 | U | 3.50 | 9.20 | 18.8 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 14.3 | U | 5.50 | 14.3 | 18.8 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 9.20 | U | 4.00 | 9.20 | 18.8 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 9.20 | U | 3.60 | 9.20 | 18.8 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 21.6 | | 44 - 130 | | 108% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 15.2 | | 60 - 125 | | 76% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:26
 Operator : YP/AJ
 Sample : Q2819-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
11M-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:43:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.664 | 3.658 | 175.2E6 | 102.2E6 | 21.546 | 20.572 |
| 2) SA Decachlor... | 8.685 | 8.632 | 93732262 | 26876447 | 12.819 | 15.209 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112860.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:26
 Operator : YP/AJ
 Sample : Q2819-06
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 11M-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:43:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

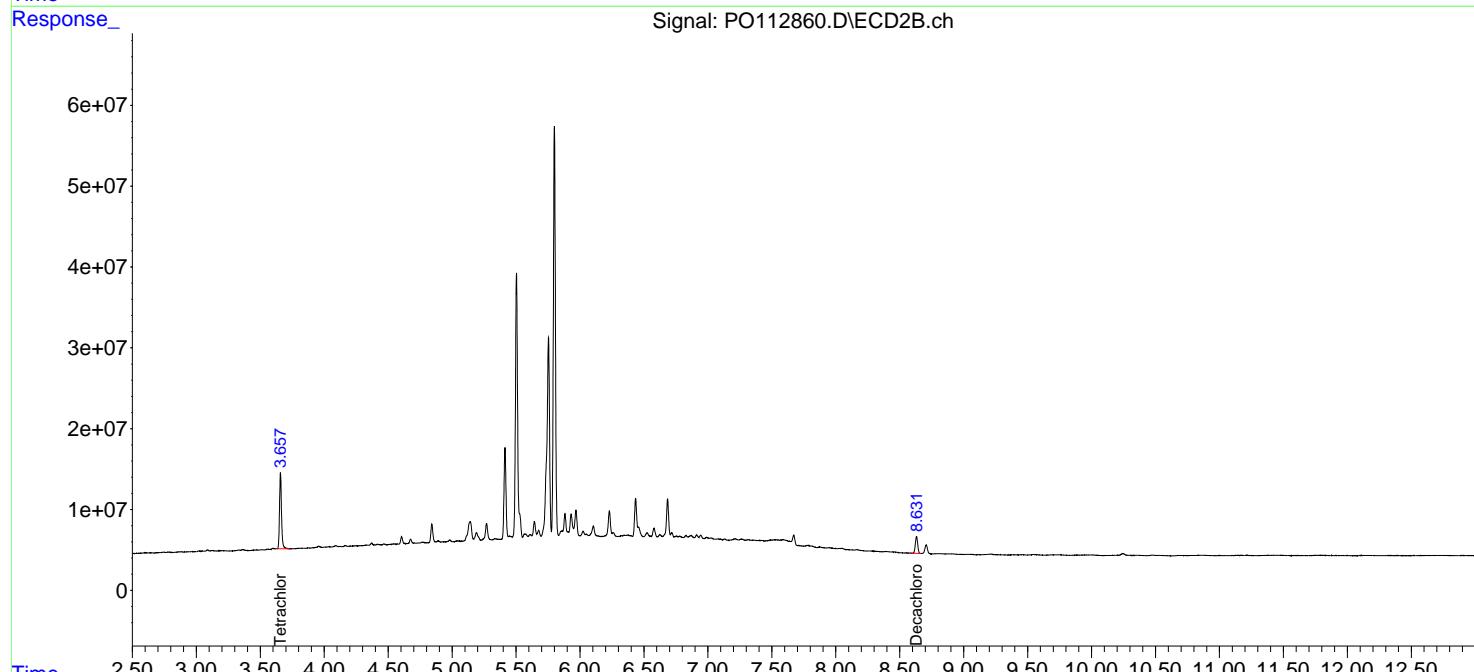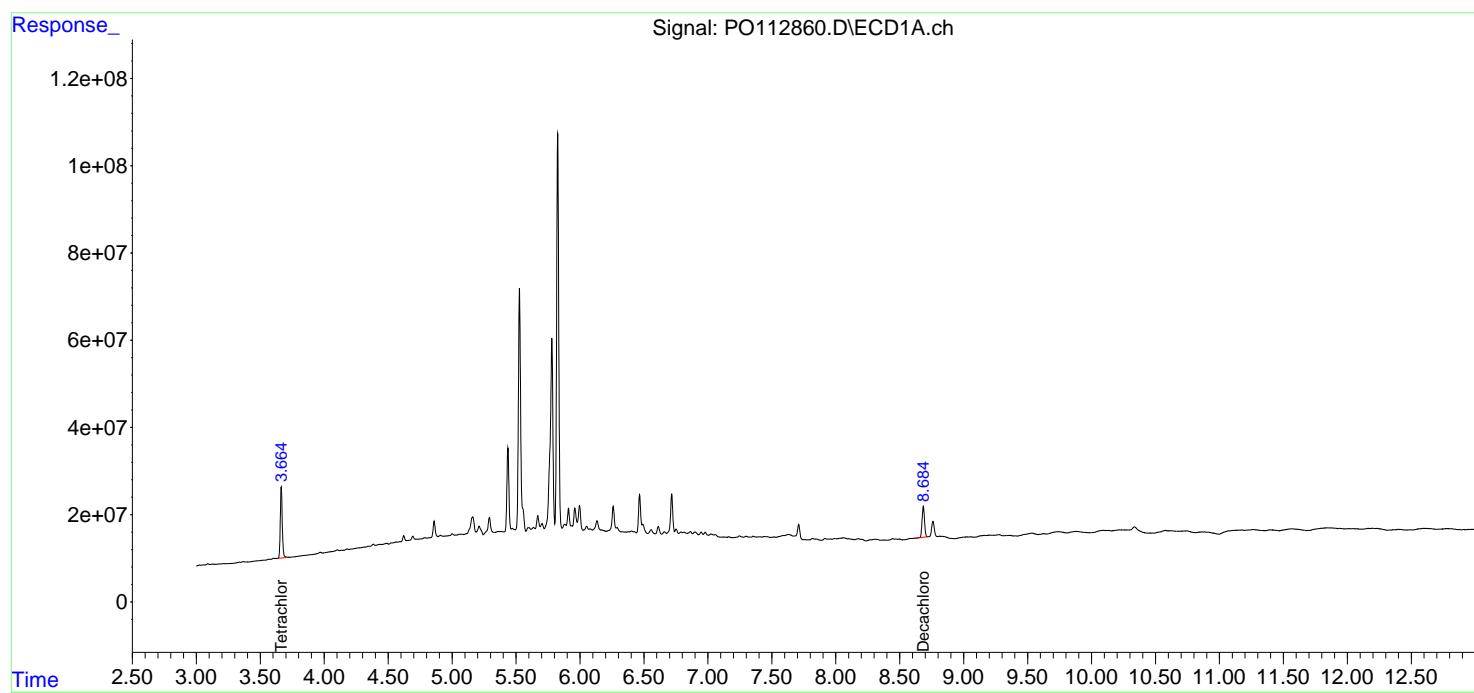

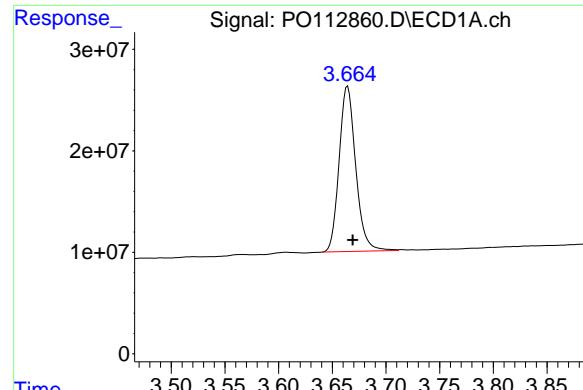

#1 Tetrachloro-m-xylene

R.T.: 3.664 min

Delta R.T.: -0.005 min

Response: 175203369


Conc: 21.55 ng/ml

Instrument:

ECD_O

ClientSampleId :

11M-S

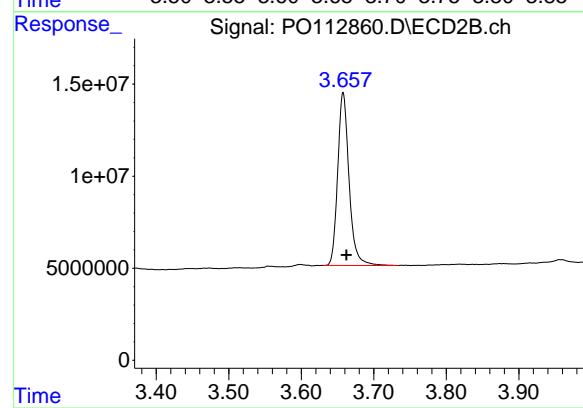


#1 Tetrachloro-m-xylene

R.T.: 3.658 min

Delta R.T.: -0.005 min

Response: 102226840

Conc: 20.57 ng/ml

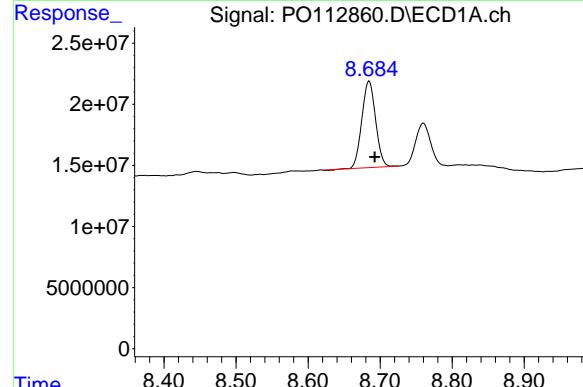


#2 Decachlorobiphenyl

R.T.: 8.685 min

Delta R.T.: -0.008 min

Response: 93732262

Conc: 12.82 ng/ml

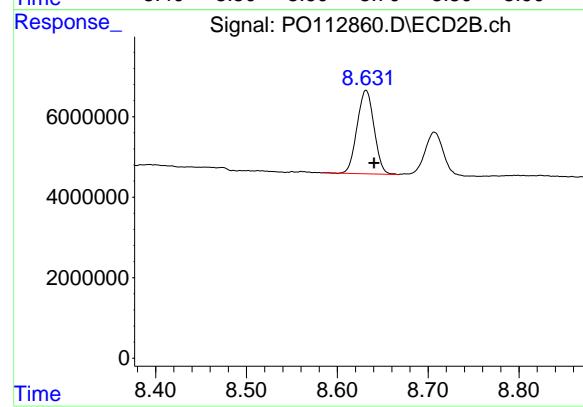

#2 Decachlorobiphenyl

R.T.: 8.632 min

Delta R.T.: -0.009 min

Response: 26876447

Conc: 15.21 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | |
|--------------------|-------------------------|--------|---|--------------------|----------|-----------|
| Client: | First Environment, Inc. | | | Date Collected: | 08/05/25 | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/08/25 | |
| Client Sample ID: | 84SB-W | | | SDG No.: | Q2819 | |
| Lab Sample ID: | Q2819-11 | | | Matrix: | SOIL | |
| Analytical Method: | 8082A | | | % Solid: | 86.8 | Decanted: |
| Sample Wt/Vol: | 30.02 | Units: | g | Final Vol: | 10000 | uL |
| Soil Aliquot Vol: | uL | | | Test: | PCB | |
| Extraction Type: | | | | Injection Volume : | | |
| GPC Factor : | 1.0 | PH : | | | | |
| Prep Method : | SW3541B | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PO112861.D | 1 | 08/12/25 08:15 | 08/12/25 13:43 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 9.60 | U | 4.50 | 9.60 | 19.6 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 15.0 | U | 4.60 | 15.0 | 19.6 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 9.60 | U | 4.30 | 9.60 | 19.6 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 9.60 | U | 4.60 | 9.60 | 19.6 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 15.0 | U | 6.80 | 15.0 | 19.6 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 9.60 | U | 3.70 | 9.60 | 19.6 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 15.0 | U | 5.80 | 15.0 | 19.6 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 9.60 | U | 4.10 | 9.60 | 19.6 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 9.60 | U | 3.70 | 9.60 | 19.6 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 21.4 | | 44 - 130 | | 107% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 14.2 | | 60 - 125 | | 71% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:43
 Operator : YP/AJ
 Sample : Q2819-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
84SB-W

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:43:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.665 | 3.658 | 173.6E6 | 101.9E6 | 21.347 | 20.515 |
| 2) SA Decachlor... | 8.684 | 8.631 | 86836801 | 25023931 | 11.876 | 14.161 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112861.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:43
 Operator : YP/AJ
 Sample : Q2819-11
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
84SB-W

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:43:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

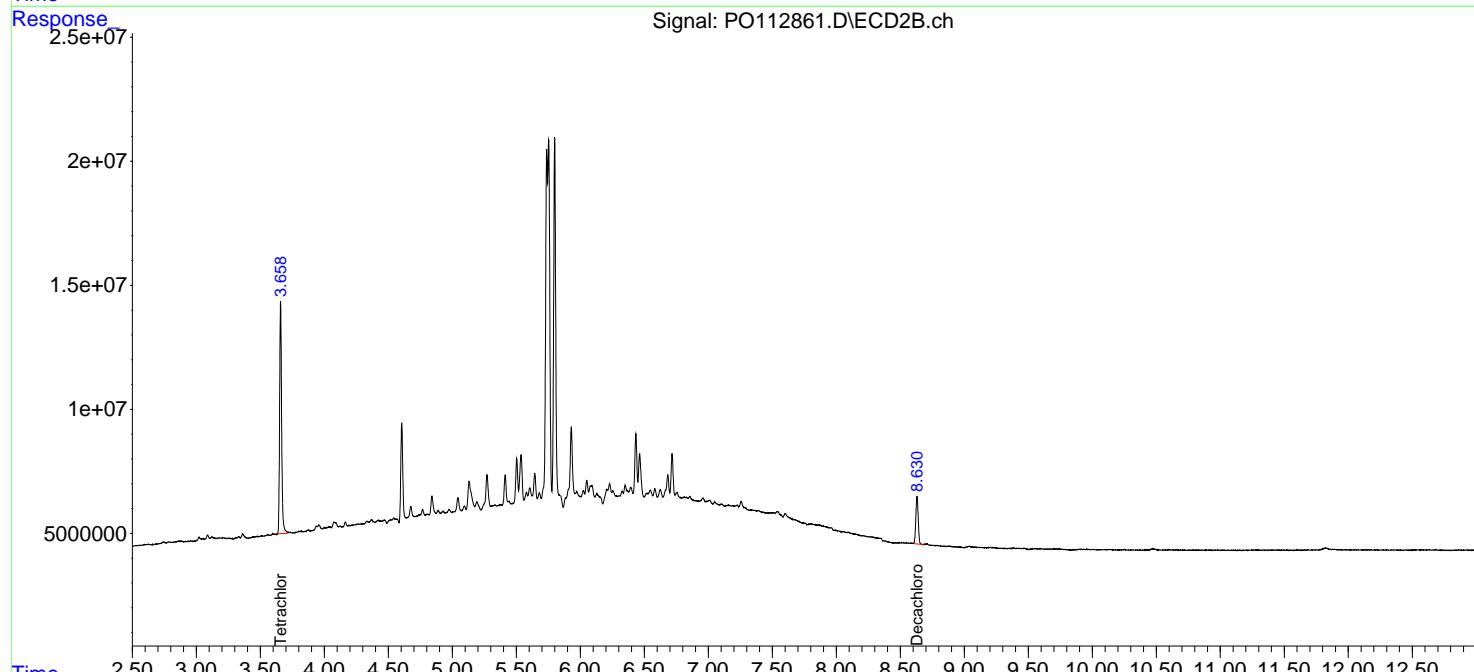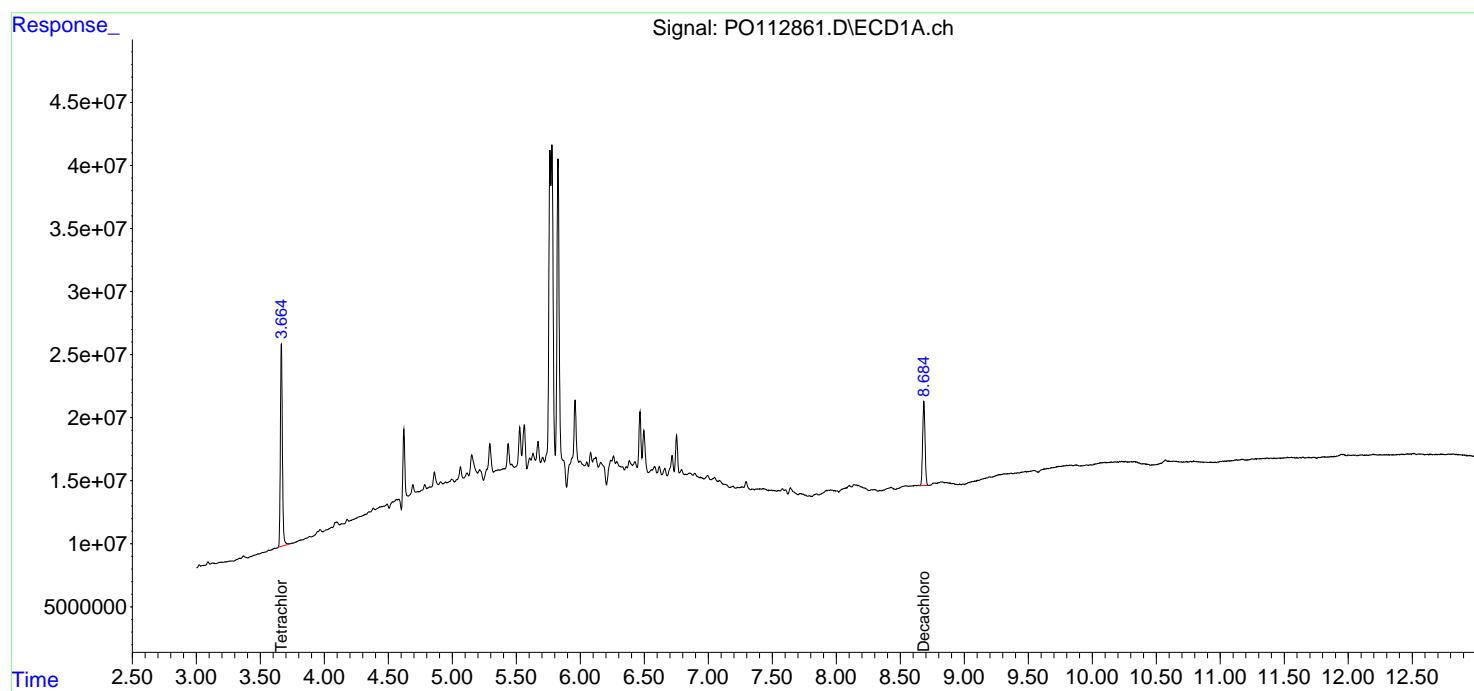



#1 Tetrachloro-m-xylene


R.T.: 3.665 min

Delta R.T.: -0.004 min

Instrument: ECD_O

Response: 173587400

Conc: 21.35 ng/ml

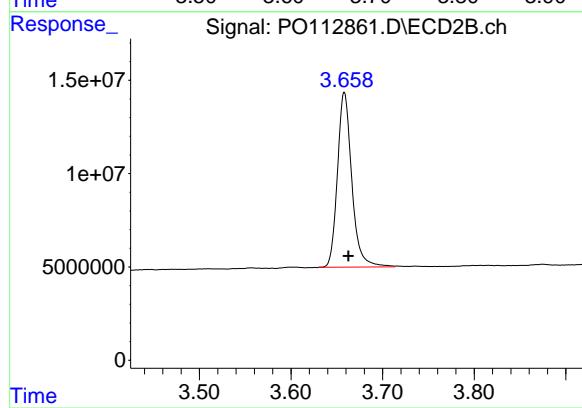


#1 Tetrachloro-m-xylene

R.T.: 3.658 min

Delta R.T.: -0.004 min

Response: 101945115

Conc: 20.52 ng/ml

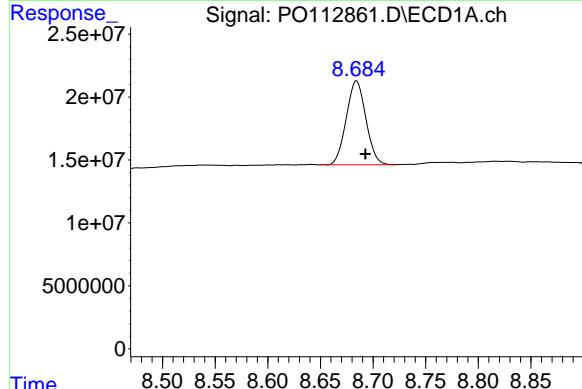


#2 Decachlorobiphenyl

R.T.: 8.684 min

Delta R.T.: -0.008 min

Response: 86836801

Conc: 11.88 ng/ml

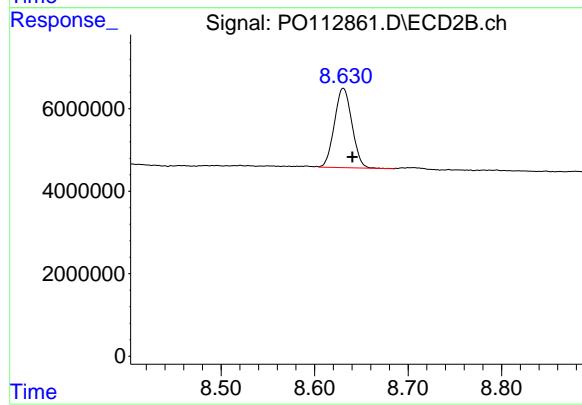

#2 Decachlorobiphenyl

R.T.: 8.631 min

Delta R.T.: -0.010 min

Response: 25023931

Conc: 14.16 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | |
|--------------------|-------------------------|--------|---|--------------------|----------|-----------|
| Client: | First Environment, Inc. | | | Date Collected: | 08/05/25 | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/08/25 | |
| Client Sample ID: | 17M-W | | | SDG No.: | Q2819 | |
| Lab Sample ID: | Q2819-14 | | | Matrix: | SOIL | |
| Analytical Method: | 8082A | | | % Solid: | 85.6 | Decanted: |
| Sample Wt/Vol: | 30.08 | Units: | g | Final Vol: | 10000 | uL |
| Soil Aliquot Vol: | uL | | | Test: | PCB | |
| Extraction Type: | | | | Injection Volume : | | |
| GPC Factor : | 1.0 | PH : | | | | |
| Prep Method : | SW3541B | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PO112862.D | 1 | 08/12/25 08:15 | 08/12/25 14:01 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 9.70 | U | 4.60 | 9.70 | 19.8 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 15.1 | U | 4.70 | 15.1 | 19.8 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 9.70 | U | 4.30 | 9.70 | 19.8 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 9.70 | U | 4.70 | 9.70 | 19.8 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 15.1 | U | 6.90 | 15.1 | 19.8 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 9.70 | U | 3.70 | 9.70 | 19.8 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 15.1 | U | 5.80 | 15.1 | 19.8 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 9.70 | U | 4.20 | 9.70 | 19.8 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 9.70 | U | 3.80 | 9.70 | 19.8 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 21.4 | | 44 - 130 | | 107% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 13.8 | | 60 - 125 | | 69% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 14:01
 Operator : YP/AJ
 Sample : Q2819-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
17M-W

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:43:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.666 | 3.659 | 173.6E6 | 101.6E6 | 21.351 | 20.451 |
| 2) SA Decachlor... | 8.687 | 8.634 | 90484172 | 24480483 | 12.375 | 13.853 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112862.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 14:01
 Operator : YP/AJ
 Sample : Q2819-14
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 17M-W

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:43:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

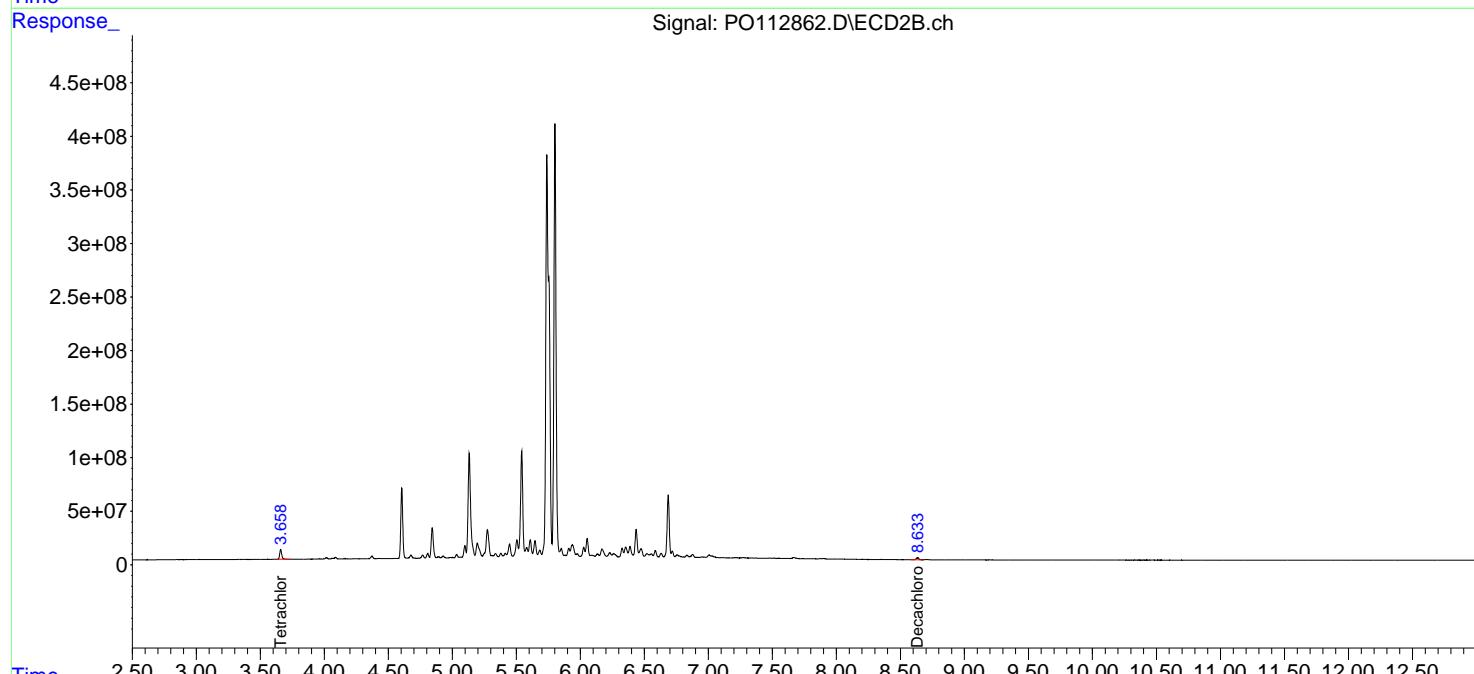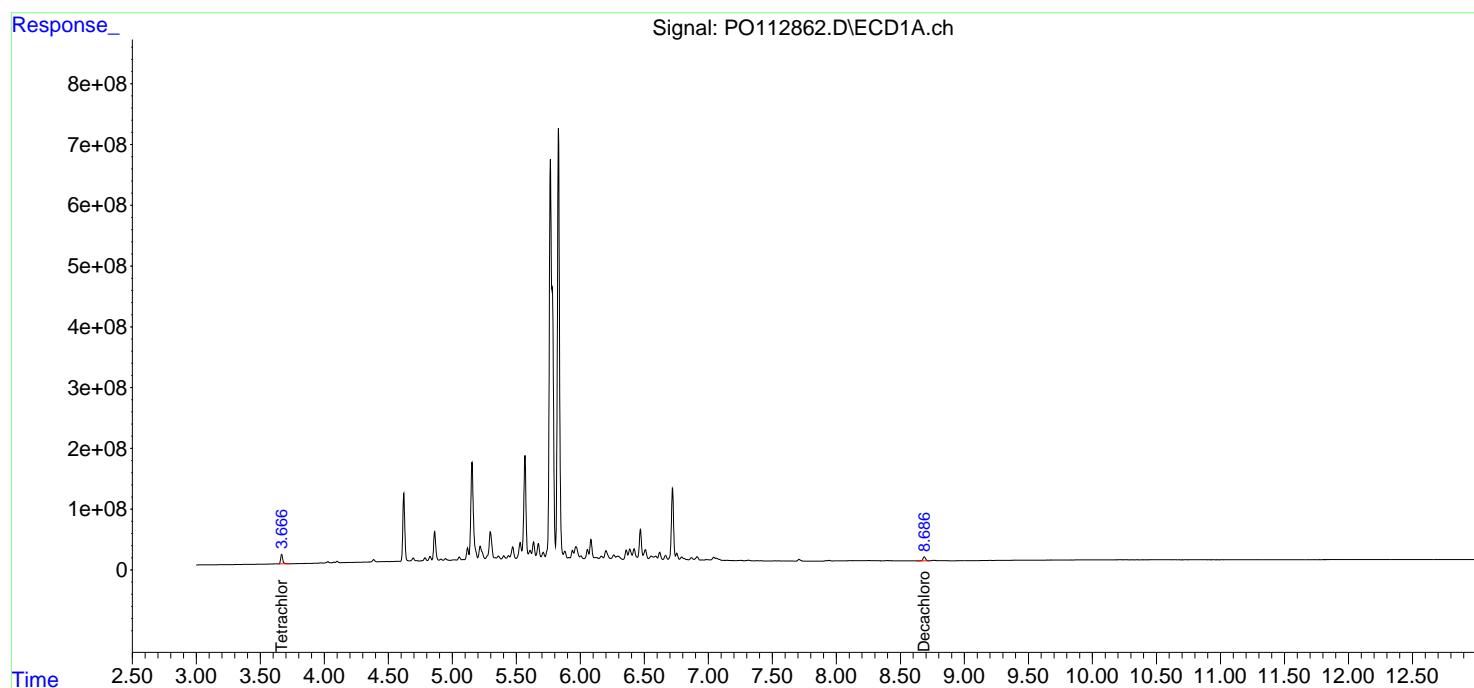



#1 Tetrachloro-m-xylene

R.T.: 3.666 min

Delta R.T.: -0.003 min

Response: 173620830


Conc: 21.35 ng/ml

Instrument:

ECD_O

ClientSampleId :

17M-W

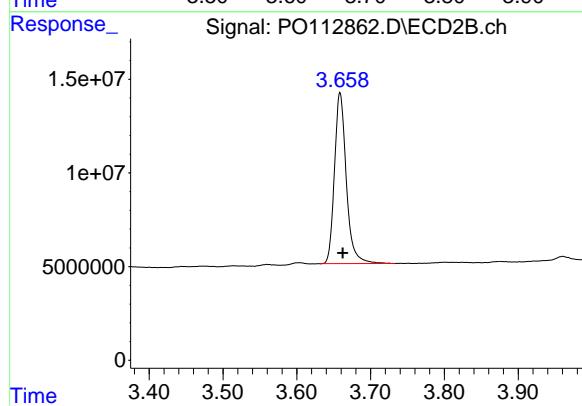


#1 Tetrachloro-m-xylene

R.T.: 3.659 min

Delta R.T.: -0.004 min

Response: 101625470

Conc: 20.45 ng/ml

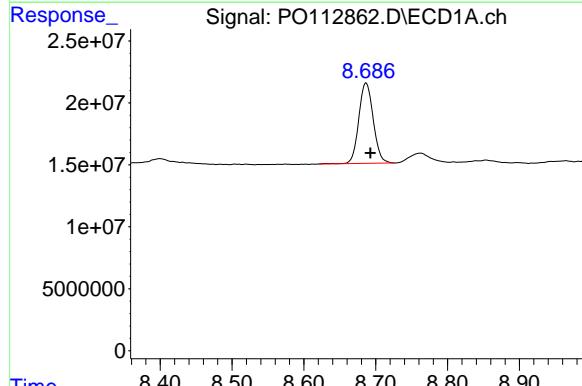


#2 Decachlorobiphenyl

R.T.: 8.687 min

Delta R.T.: -0.006 min

Response: 90484172

Conc: 12.38 ng/ml

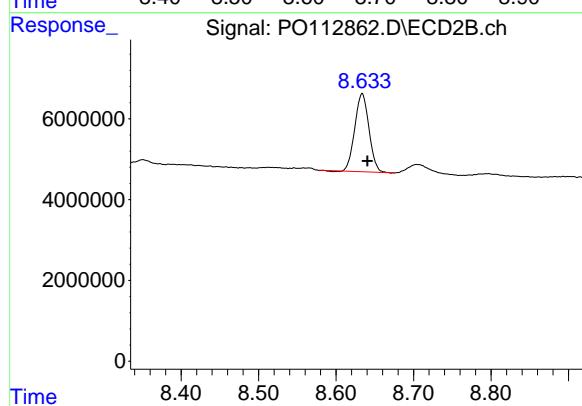

#2 Decachlorobiphenyl

R.T.: 8.634 min

Delta R.T.: -0.007 min

Response: 24480483

Conc: 13.85 ng/ml



CALIBRATION

SUMMARY



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

| | | | |
|----------------|----------|----------------------|------------------|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| Instrument ID: | ECD_O | Calibration Date(s): | 07/23/2025 |
| | | Calibration Times: | 11:32 19:47 |

GC Column: ZB-MR1 ID: 0.32 (mm)

| | | |
|--------------|--|---------------------|
| LAB FILE ID: | RT 1000 = PO112414.D | RT 750 = PO112415.D |
| | RT 500 = PO112416.D RT 250 = PO112417.D | RT 050 = PO112418.D |

| COMPOUND | RT 1000 | RT 750 | RT 500 | RT 250 | RT 050 | MEAN RT | RT WINDOW FROM | RT WINDOW TO |
|----------------------|---------|--------|--------|--------|--------|---------|----------------|--------------|
| Aroclor-1016-1 (1) | 4.76 | 4.75 | 4.76 | 4.76 | 4.76 | 4.76 | 4.66 | 4.86 |
| Aroclor-1016-2 (2) | 4.78 | 4.77 | 4.77 | 4.77 | 4.77 | 4.77 | 4.67 | 4.87 |
| Aroclor-1016-3 (3) | 4.83 | 4.83 | 4.83 | 4.83 | 4.83 | 4.83 | 4.73 | 4.93 |
| Aroclor-1016-4 (4) | 4.95 | 4.95 | 4.95 | 4.95 | 4.95 | 4.95 | 4.85 | 5.05 |
| Aroclor-1016-5 (5) | 5.21 | 5.21 | 5.21 | 5.21 | 5.21 | 5.21 | 5.11 | 5.31 |
| Aroclor-1260-1 (1) | 6.25 | 6.24 | 6.25 | 6.24 | 6.25 | 6.24 | 6.14 | 6.34 |
| Aroclor-1260-2 (2) | 6.44 | 6.43 | 6.43 | 6.43 | 6.43 | 6.43 | 6.33 | 6.53 |
| Aroclor-1260-3 (3) | 6.80 | 6.80 | 6.80 | 6.80 | 6.80 | 6.80 | 6.70 | 6.90 |
| Aroclor-1260-4 (4) | 7.06 | 7.06 | 7.06 | 7.06 | 7.06 | 7.06 | 6.96 | 7.16 |
| Aroclor-1260-5 (5) | 7.30 | 7.30 | 7.30 | 7.30 | 7.30 | 7.30 | 7.20 | 7.40 |
| Decachlorobiphenyl | 8.70 | 8.69 | 8.69 | 8.69 | 8.69 | 8.69 | 8.59 | 8.79 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.57 | 3.77 |
| Aroclor-1242-1 (1) | 4.76 | 4.76 | 4.76 | 4.76 | 4.76 | 4.76 | 4.66 | 4.86 |
| Aroclor-1242-2 (2) | 4.78 | 4.77 | 4.77 | 4.77 | 4.78 | 4.78 | 4.68 | 4.88 |
| Aroclor-1242-3 (3) | 4.83 | 4.83 | 4.83 | 4.83 | 4.83 | 4.83 | 4.73 | 4.93 |
| Aroclor-1242-4 (4) | 4.95 | 4.95 | 4.95 | 4.95 | 4.95 | 4.95 | 4.85 | 5.05 |
| Aroclor-1242-5 (5) | 5.60 | 5.60 | 5.60 | 5.60 | 5.60 | 5.60 | 5.50 | 5.70 |
| Decachlorobiphenyl | 8.69 | 8.69 | 8.69 | 8.69 | 8.70 | 8.69 | 8.59 | 8.79 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.57 | 3.77 |
| Aroclor-1248-1 (1) | 4.76 | 4.76 | 4.75 | 4.76 | 4.76 | 4.76 | 4.66 | 4.86 |
| Aroclor-1248-2 (2) | 4.99 | 4.99 | 4.99 | 4.99 | 5.00 | 4.99 | 4.89 | 5.09 |
| Aroclor-1248-3 (3) | 5.21 | 5.21 | 5.21 | 5.21 | 5.21 | 5.21 | 5.11 | 5.31 |
| Aroclor-1248-4 (4) | 5.56 | 5.56 | 5.56 | 5.56 | 5.56 | 5.56 | 5.46 | 5.66 |
| Aroclor-1248-5 (5) | 5.60 | 5.60 | 5.60 | 5.60 | 5.60 | 5.60 | 5.50 | 5.70 |
| Decachlorobiphenyl | 8.69 | 8.69 | 8.69 | 8.70 | 8.69 | 8.69 | 8.59 | 8.79 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.57 | 3.77 |
| Aroclor-1254-1 (1) | 5.56 | 5.56 | 5.56 | 5.56 | 5.56 | 5.56 | 5.46 | 5.66 |
| Aroclor-1254-2 (2) | 5.71 | 5.71 | 5.71 | 5.71 | 5.71 | 5.71 | 5.61 | 5.81 |
| Aroclor-1254-3 (3) | 6.11 | 6.11 | 6.11 | 6.11 | 6.11 | 6.11 | 6.01 | 6.21 |
| Aroclor-1254-4 (4) | 6.34 | 6.34 | 6.34 | 6.34 | 6.34 | 6.34 | 6.24 | 6.44 |
| Aroclor-1254-5 (5) | 6.76 | 6.76 | 6.76 | 6.76 | 6.76 | 6.76 | 6.66 | 6.86 |
| Decachlorobiphenyl | 8.69 | 8.69 | 8.70 | 8.69 | 8.69 | 8.69 | 8.59 | 8.79 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.57 | 3.77 |
| Aroclor-1268-1 (1) | 7.59 | 7.59 | 7.59 | 7.58 | 7.59 | 7.59 | 7.49 | 7.69 |
| Aroclor-1268-2 (2) | 7.65 | 7.65 | 7.65 | 7.65 | 7.65 | 7.65 | 7.55 | 7.75 |
| Aroclor-1268-3 (3) | 7.86 | 7.86 | 7.86 | 7.86 | 7.86 | 7.86 | 7.76 | 7.96 |
| Aroclor-1268-4 (4) | 8.15 | 8.15 | 8.15 | 8.14 | 8.15 | 8.15 | 8.05 | 8.25 |
| Aroclor-1268-5 (5) | 8.44 | 8.44 | 8.44 | 8.44 | 8.44 | 8.44 | 8.34 | 8.54 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

| | | | | | | | | | |
|----------------------|------|------|------|------|------|------|------|------|---|
| Decachlorobiphenyl | 8.70 | 8.70 | 8.70 | 8.69 | 8.70 | 8.70 | 8.60 | 8.80 | 1 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.67 | 3.57 | 3.77 | 2 |

3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

| | | | |
|----------------|----------|----------------------|------------------|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| Instrument ID: | ECD_O | Calibration Date(s): | 07/23/2025 |
| | | Calibration Times: | 11:32 19:47 |

GC Column: ZB-MR2 ID: 0.32 (mm)

| | | |
|--------------|--|---------------------|
| LAB FILE ID: | RT 1000 = PO112414.D | RT 750 = PO112415.D |
| | RT 500 = PO112416.D RT 250 = PO112417.D | RT 050 = PO112418.D |

| COMPOUND | RT 1000 | RT 750 | RT 500 | RT 250 | RT 050 | MEAN RT | RT WINDOW FROM | RT WINDOW TO |
|----------------------|---------|--------|--------|--------|--------|---------|----------------|--------------|
| Aroclor-1016-1 (1) | 4.74 | 4.74 | 4.74 | 4.74 | 4.74 | 4.74 | 4.64 | 4.84 |
| Aroclor-1016-2 (2) | 4.76 | 4.76 | 4.76 | 4.76 | 4.76 | 4.76 | 4.66 | 4.86 |
| Aroclor-1016-3 (3) | 4.93 | 4.93 | 4.93 | 4.93 | 4.93 | 4.93 | 4.83 | 5.03 |
| Aroclor-1016-4 (4) | 4.97 | 4.97 | 4.97 | 4.97 | 4.97 | 4.97 | 4.87 | 5.07 |
| Aroclor-1016-5 (5) | 5.19 | 5.19 | 5.19 | 5.19 | 5.19 | 5.19 | 5.09 | 5.29 |
| Aroclor-1260-1 (1) | 6.21 | 6.21 | 6.21 | 6.21 | 6.21 | 6.21 | 6.11 | 6.31 |
| Aroclor-1260-2 (2) | 6.40 | 6.40 | 6.40 | 6.40 | 6.40 | 6.40 | 6.30 | 6.50 |
| Aroclor-1260-3 (3) | 6.55 | 6.55 | 6.55 | 6.55 | 6.55 | 6.55 | 6.45 | 6.65 |
| Aroclor-1260-4 (4) | 7.02 | 7.02 | 7.02 | 7.02 | 7.02 | 7.02 | 6.92 | 7.12 |
| Aroclor-1260-5 (5) | 7.27 | 7.26 | 7.26 | 7.26 | 7.27 | 7.26 | 7.16 | 7.36 |
| Decachlorobiphenyl | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.54 | 8.74 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.56 | 3.76 |
| Aroclor-1242-1 (1) | 4.74 | 4.74 | 4.74 | 4.74 | 4.74 | 4.74 | 4.64 | 4.84 |
| Aroclor-1242-2 (2) | 4.76 | 4.76 | 4.76 | 4.76 | 4.76 | 4.76 | 4.66 | 4.86 |
| Aroclor-1242-3 (3) | 4.93 | 4.93 | 4.93 | 4.93 | 4.93 | 4.93 | 4.83 | 5.03 |
| Aroclor-1242-4 (4) | 5.02 | 5.02 | 5.02 | 5.02 | 5.02 | 5.02 | 4.92 | 5.12 |
| Aroclor-1242-5 (5) | 5.53 | 5.53 | 5.53 | 5.53 | 5.54 | 5.53 | 5.43 | 5.63 |
| Decachlorobiphenyl | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.54 | 8.74 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.56 | 3.76 |
| Aroclor-1248-1 (1) | 4.74 | 4.74 | 4.74 | 4.74 | 4.74 | 4.74 | 4.64 | 4.84 |
| Aroclor-1248-2 (2) | 4.97 | 4.97 | 4.97 | 4.97 | 4.97 | 4.97 | 4.87 | 5.07 |
| Aroclor-1248-3 (3) | 5.02 | 5.02 | 5.02 | 5.02 | 5.02 | 5.02 | 4.92 | 5.12 |
| Aroclor-1248-4 (4) | 5.19 | 5.19 | 5.19 | 5.19 | 5.19 | 5.19 | 5.09 | 5.29 |
| Aroclor-1248-5 (5) | 5.58 | 5.58 | 5.58 | 5.58 | 5.58 | 5.58 | 5.48 | 5.68 |
| Decachlorobiphenyl | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.54 | 8.74 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.56 | 3.76 |
| Aroclor-1254-1 (1) | 5.54 | 5.54 | 5.54 | 5.53 | 5.53 | 5.54 | 5.44 | 5.64 |
| Aroclor-1254-2 (2) | 5.68 | 5.68 | 5.68 | 5.68 | 5.68 | 5.68 | 5.58 | 5.78 |
| Aroclor-1254-3 (3) | 6.08 | 6.08 | 6.08 | 6.08 | 6.08 | 6.08 | 5.98 | 6.18 |
| Aroclor-1254-4 (4) | 6.31 | 6.31 | 6.31 | 6.31 | 6.31 | 6.31 | 6.21 | 6.41 |
| Aroclor-1254-5 (5) | 6.73 | 6.73 | 6.73 | 6.73 | 6.73 | 6.73 | 6.63 | 6.83 |
| Decachlorobiphenyl | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.54 | 8.74 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.56 | 3.76 |
| Aroclor-1268-1 (1) | 7.55 | 7.55 | 7.55 | 7.55 | 7.55 | 7.55 | 7.45 | 7.65 |
| Aroclor-1268-2 (2) | 7.61 | 7.61 | 7.61 | 7.61 | 7.61 | 7.61 | 7.51 | 7.71 |
| Aroclor-1268-3 (3) | 7.82 | 7.82 | 7.82 | 7.82 | 7.82 | 7.82 | 7.72 | 7.92 |
| Aroclor-1268-4 (4) | 8.10 | 8.10 | 8.10 | 8.10 | 8.10 | 8.10 | 8.00 | 8.20 |
| Aroclor-1268-5 (5) | 8.39 | 8.39 | 8.39 | 8.39 | 8.39 | 8.39 | 8.29 | 8.49 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

| | | | | | | | | | |
|----------------------|------|------|------|------|------|------|------|------|---|
| Decachlorobiphenyl | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.64 | 8.54 | 8.74 | 1 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.66 | 3.56 | 3.76 | 2 |

3

4

5

6

7

8

9

10

11

12

13

14

15

16

17

18

19

20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

| | | | |
|----------------|----------|----------------------|------------|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| Instrument ID: | ECD_O | Calibration Date(s): | 07/23/2025 |
| | | Calibration Times: | 11:32 |
| | | | 19:47 |

GC Column: ZB-MR1 ID: 0.32 (mm)

| LAB FILE ID: | CF 1000 = | <u>PO112414.D</u> | CF 750 = | <u>PO112415.D</u> | CF | % RSD |
|----------------------|------------|-------------------|------------|-------------------|------------|---------------|
| | CF 500 = | <u>PO112416.D</u> | CF 250 = | <u>PO112417.D</u> | | |
| COMPOUND | CF 1000 | CF 750 | CF 500 | CF 250 | CF 050 | |
| Aroclor-1016-1 (1) | 281481703 | 285148303 | 290849518 | 279501268 | 204848240 | 268365806 13 |
| Aroclor-1016-2 (2) | 418001550 | 431852928 | 433849136 | 420704900 | 326178800 | 406117463 11 |
| Aroclor-1016-3 (3) | 263638281 | 273794351 | 273610504 | 262887848 | 234438940 | 261673985 6 |
| Aroclor-1016-4 (4) | 216165184 | 219268720 | 223332708 | 213740540 | 186700200 | 211841470 6 |
| Aroclor-1016-5 (5) | 221113370 | 228268088 | 233867428 | 235369996 | 178734160 | 219470608 10 |
| Aroclor-1260-1 (1) | 431773857 | 450001749 | 476240286 | 447612572 | 391026880 | 439331069 7 |
| Aroclor-1260-2 (2) | 673380136 | 698254531 | 722944530 | 686506064 | 658383800 | 687893812 3 |
| Aroclor-1260-3 (3) | 611274773 | 627246767 | 610311884 | 614713140 | 476551180 | 588019549 10 |
| Aroclor-1260-4 (4) | 447285263 | 461047633 | 473248904 | 505121600 | 368319820 | 451004644 11 |
| Aroclor-1260-5 (5) | 1262689005 | 1283961461 | 1337121492 | 1347466800 | 964454900 | 1239138732 12 |
| Decachlorobiphenyl | 7456684020 | 7676252293 | 7829495380 | 7672255680 | 5924316000 | 7311800675 11 |
| Tetrachloro-m-xylene | 8554863660 | 8750848067 | 8754072420 | 8314620000 | 6283438800 | 8131568589 13 |
| Aroclor-1242-1 (1) | 256299409 | 259568919 | 260660454 | 265097176 | 196334180 | 247592028 11 |
| Aroclor-1242-2 (2) | 381137122 | 387088803 | 391556862 | 393536916 | 295648160 | 369793573 11 |
| Aroclor-1242-3 (3) | 241769617 | 246476011 | 248315054 | 252195680 | 194532760 | 236657824 10 |
| Aroclor-1242-4 (4) | 195717021 | 198363989 | 201564902 | 203398396 | 172348620 | 194278586 6 |
| Aroclor-1242-5 (5) | 215656431 | 220174447 | 229182990 | 229543836 | 175020200 | 213915581 10 |
| Decachlorobiphenyl | 8000645330 | 8037989413 | 8087967020 | 8086832920 | 6389983800 | 7720683697 10 |
| Tetrachloro-m-xylene | 9125652230 | 9195232120 | 9219491440 | 9207437080 | 6341808000 | 8617924174 15 |
| Aroclor-1248-1 (1) | 189314500 | 193406379 | 198364040 | 203445536 | 151513120 | 187208715 10 |
| Aroclor-1248-2 (2) | 257058197 | 266019899 | 270572928 | 278752472 | 203158020 | 255112303 11 |
| Aroclor-1248-3 (3) | 329824745 | 342687100 | 350417966 | 364320620 | 331255900 | 343701266 4 |
| Aroclor-1248-4 (4) | 503150480 | 523568551 | 540549606 | 563745892 | 409374460 | 508077798 11 |
| Aroclor-1248-5 (5) | 346508966 | 363261911 | 374337920 | 392493440 | 271353380 | 349591123 13 |
| Decachlorobiphenyl | 7900018490 | 8086308400 | 8195171040 | 8262080520 | 6143274400 | 7717370570 12 |
| Tetrachloro-m-xylene | 8946590960 | 9189061507 | 9273186240 | 9357342160 | 6567561400 | 8666748453 14 |
| Aroclor-1254-1 (1) | 525205609 | 551869540 | 568048078 | 599161796 | 500508140 | 548958633 7 |
| Aroclor-1254-2 (2) | 467389736 | 490253857 | 501431616 | 531267632 | 439250900 | 485918748 7 |
| Aroclor-1254-3 (3) | 736681841 | 765368536 | 778116616 | 788008044 | 653257120 | 744286431 7 |
| Aroclor-1254-4 (4) | 537295054 | 560529123 | 571244926 | 572391952 | 507057560 | 549703723 5 |
| Aroclor-1254-5 (5) | 713157717 | 729355651 | 738947588 | 743850736 | 613809420 | 707824222 7 |
| Decachlorobiphenyl | 7810644110 | 7988158653 | 8118440840 | 8069654680 | 6321650600 | 7661709777 10 |
| Tetrachloro-m-xylene | 8477893750 | 8928798520 | 9019842540 | 9077508800 | 7004909800 | 8501790682 10 |
| Aroclor-1268-1 (1) | 1805209287 | 1836925397 | 1850534848 | 1852730580 | 1410311920 | 1751142406 10 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

| | | | | | | | | |
|----------------------|-----|-------------|-------------|-------------|-------------|-------------|-------------|----|
| Aroclor-1268-2 | (2) | 1523811042 | 1548194379 | 1559255960 | 1566806172 | 1167050180 | 1473023547 | 11 |
| Aroclor-1268-3 | (3) | 1298638460 | 1316156257 | 1333295814 | 1329215988 | 983852920 | 1252231888 | 11 |
| Aroclor-1268-4 | (4) | 502325303 | 515160189 | 514467028 | 515975792 | 361392800 | 481864222 | 13 |
| Aroclor-1268-5 | (5) | 3537850645 | 3568750916 | 3561527908 | 3536594816 | 2581136540 | 3357172165 | 12 |
| Decachlorobiphenyl | | 14538757830 | 14683927053 | 14777305700 | 14801547680 | 10962984400 | 13952904533 | 12 |
| Tetrachloro-m-xylene | | 8916461140 | 9229914440 | 9271431040 | 9355148600 | 6516020600 | 8657795164 | 14 |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

| | | | |
|----------------|----------|----------------------|------------|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| Instrument ID: | ECD_O | Calibration Date(s): | 07/23/2025 |
| | | Calibration Times: | 11:32 |
| | | | 19:47 |
| GC Column: | ZB-MR2 | ID: | 0.32 (mm) |

| LAB FILE ID: | CF 1000 = | CF 750 = | CF 500 = | CF 250 = | CF 050 = | CF | % RSD |
|----------------------|-------------------|-------------------|-------------------|-------------------|-------------------|------------|-------|
| | <u>PO112414.D</u> | <u>PO112415.D</u> | <u>PO112416.D</u> | <u>PO112417.D</u> | <u>PO112418.D</u> | | |
| COMPOUND | CF 1000 | CF 750 | CF 500 | CF 250 | CF 050 | CF | % RSD |
| Aroclor-1016-1 (1) | 171399488 | 177928739 | 180256326 | 179838608 | 165612060 | 175007044 | 3 |
| Aroclor-1016-2 (2) | 254283756 | 266059885 | 273532534 | 272267680 | 236331280 | 260495027 | 6 |
| Aroclor-1016-3 (3) | 134555314 | 139369485 | 142347070 | 141007248 | 122553240 | 135966471 | 6 |
| Aroclor-1016-4 (4) | 106915956 | 111683577 | 115661150 | 118698688 | 102464540 | 111084782 | 6 |
| Aroclor-1016-5 (5) | 139169322 | 144750759 | 147937312 | 152336452 | 132321220 | 143303013 | 5 |
| Aroclor-1260-1 (1) | 240286237 | 254043527 | 261134446 | 258041412 | 229050000 | 248511124 | 5 |
| Aroclor-1260-2 (2) | 317223235 | 329626419 | 335041102 | 340620804 | 324956000 | 329493512 | 3 |
| Aroclor-1260-3 (3) | 256241072 | 262701627 | 269297872 | 275910760 | 220454080 | 256921082 | 8 |
| Aroclor-1260-4 (4) | 185740526 | 193469844 | 197255514 | 200936168 | 179151380 | 191310686 | 4 |
| Aroclor-1260-5 (5) | 419199446 | 421594747 | 433075366 | 434815624 | 352283180 | 412193673 | 8 |
| Decachlorobiphenyl | 1753295660 | 1820833173 | 1877801640 | 1892185680 | 1491444000 | 1767112031 | 9 |
| Tetrachloro-m-xylene | 5169666700 | 5314856493 | 5330554580 | 5111206560 | 3919594600 | 4969175787 | 12 |
| Aroclor-1242-1 (1) | 153645977 | 158282413 | 162201976 | 169125204 | 148714620 | 158394038 | 5 |
| Aroclor-1242-2 (2) | 230553136 | 236233123 | 241816698 | 253231308 | 206497880 | 233666429 | 7 |
| Aroclor-1242-3 (3) | 120997871 | 124593004 | 126633224 | 130347852 | 103373540 | 121189098 | 8 |
| Aroclor-1242-4 (4) | 116921071 | 120755713 | 124229780 | 129097232 | 122693120 | 122739383 | 3 |
| Aroclor-1242-5 (5) | 154482444 | 160907067 | 167116390 | 163960092 | 158390400 | 160971279 | 3 |
| Decachlorobiphenyl | 1831604040 | 1871840933 | 1924104720 | 1967119920 | 1579850400 | 1834904003 | 8 |
| Tetrachloro-m-xylene | 5483238770 | 5543459253 | 5573552360 | 5630865680 | 4061456200 | 5258514453 | 13 |
| Aroclor-1248-1 (1) | 116797575 | 121746903 | 126835386 | 132022196 | 110144520 | 121509316 | 7 |
| Aroclor-1248-2 (2) | 161755092 | 168905528 | 175846314 | 185366264 | 154525280 | 169279696 | 7 |
| Aroclor-1248-3 (3) | 170672394 | 178220732 | 184519824 | 194073912 | 160748960 | 177647164 | 7 |
| Aroclor-1248-4 (4) | 202462025 | 210645355 | 219142380 | 229572292 | 179950700 | 208354550 | 9 |
| Aroclor-1248-5 (5) | 207118457 | 216119221 | 227433754 | 242834452 | 180319280 | 214765033 | 10 |
| Decachlorobiphenyl | 1836524820 | 1878481893 | 1941164520 | 1982063240 | 1517022000 | 1831051295 | 10 |
| Tetrachloro-m-xylene | 5362990180 | 5502770333 | 5558036420 | 5629888520 | 4177350800 | 5246207251 | 12 |
| Aroclor-1254-1 (1) | 308086628 | 324598995 | 339171148 | 360746064 | 310502200 | 328621007 | 6 |
| Aroclor-1254-2 (2) | 269579969 | 283423153 | 295499466 | 318260532 | 280690420 | 289490708 | 6 |
| Aroclor-1254-3 (3) | 411643535 | 427646563 | 444183030 | 462345912 | 391487940 | 427461396 | 6 |
| Aroclor-1254-4 (4) | 256982627 | 269810957 | 279068642 | 286892132 | 272060980 | 272963068 | 4 |
| Aroclor-1254-5 (5) | 324913084 | 333876627 | 346327314 | 357344936 | 307636300 | 334019652 | 5 |
| Decachlorobiphenyl | 1794065640 | 1872151533 | 1910898600 | 1948005080 | 1573949600 | 1819814091 | 8 |
| Tetrachloro-m-xylene | 5135321880 | 5340323933 | 5419556800 | 5524764520 | 4404208000 | 5164835027 | 9 |
| Aroclor-1268-1 (1) | 514567345 | 516695037 | 532735372 | 551455976 | 473857920 | 517862330 | 5 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

| | | | | | | | | |
|----------------------|-----|------------|------------|------------|------------|------------|------------|----|
| Aroclor-1268-2 | (2) | 421574479 | 425971267 | 436618852 | 454509592 | 386645480 | 425063934 | 6 |
| Aroclor-1268-3 | (3) | 318758782 | 324505707 | 331241876 | 345977680 | 285851460 | 321267101 | 7 |
| Aroclor-1268-4 | (4) | 111516853 | 115705837 | 114796592 | 121616720 | 92841800 | 111295560 | 9 |
| Aroclor-1268-5 | (5) | 742715083 | 756736297 | 758808540 | 780432416 | 619995020 | 731737471 | 8 |
| Decachlorobiphenyl | | 3224484190 | 3300929360 | 3351395200 | 3481054400 | 2726789400 | 3216930510 | 9 |
| Tetrachloro-m-xylene | | 5326223920 | 5511724707 | 5541913900 | 5672741280 | 4190979000 | 5248716561 | 12 |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

| | | | |
|----------------|-----------------|-------------------|-------------------|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| Instrument ID: | <u>ECD_O</u> | Date(s) Analyzed: | <u>07/23/2025</u> |
| GC Column: | <u>ZB-MR1</u> | ID: | <u>0.32</u> (mm) |

| COMPOUND | AMOUNT (ng) | PEAK | RT | RT WINDOW | | CALIBRATION FACTOR |
|--------------|----------------|------|------|-----------|------|-----------------------|
| | | | | FROM | TO | |
| Aroclor-1221 | 500 | 1 | 3.88 | 3.78 | 3.98 | 96659600 |
| | | 2 | 3.97 | 3.87 | 4.07 | 71862000 |
| | | 3 | 4.04 | 3.94 | 4.14 | 237712000 |
| | | 4 | 0.00 | | | 0 |
| | | 5 | 0.00 | | | 0 |
| Aroclor-1232 | 500 | 1 | 4.04 | 3.94 | 4.14 | 186979000 |
| | | 2 | 4.54 | 4.44 | 4.64 | 107625000 |
| | | 3 | 4.78 | 4.68 | 4.88 | 206800000 |
| | | 4 | 4.95 | 4.85 | 5.05 | 104740000 |
| | | 5 | 4.99 | 4.89 | 5.09 | 67880800 |
| Aroclor-1262 | 500 | 1 | 6.80 | 6.70 | 6.90 | 929208000 |
| | | 2 | 7.30 | 7.20 | 7.40 | 1487020000 |
| | | 3 | 7.59 | 7.49 | 7.69 | 590252000 |
| | | 4 | 7.65 | 7.55 | 7.75 | 994166000 |
| | | 5 | 8.15 | 8.05 | 8.25 | 434062000 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

| | | | |
|----------------|-----------------|-------------------|-------------------|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| Instrument ID: | <u>ECD_O</u> | Date(s) Analyzed: | <u>07/23/2025</u> |
| GC Column: | <u>ZB-MR2</u> | ID: | <u>0.32</u> (mm) |

| COMPOUND | AMOUNT (ng) | PEAK | RT | RT WINDOW | | CALIBRATION FACTOR |
|--------------|----------------|------|------|-----------|------|-----------------------|
| | | | | FROM | TO | |
| Aroclor-1221 | 500 | 1 | 3.87 | 3.77 | 3.97 | 67265800 |
| | | 2 | 3.96 | 3.86 | 4.06 | 50728000 |
| | | 3 | 4.03 | 3.93 | 4.13 | 158529000 |
| | | 4 | 0.00 | | | 0 |
| | | 5 | 0.00 | | | 0 |
| Aroclor-1232 | 500 | 1 | 4.03 | 3.93 | 4.13 | 126550000 |
| | | 2 | 4.76 | 4.66 | 4.86 | 131155000 |
| | | 3 | 4.93 | 4.83 | 5.03 | 67196800 |
| | | 4 | 5.02 | 4.92 | 5.12 | 59829000 |
| | | 5 | 5.19 | 5.09 | 5.29 | 65203000 |
| Aroclor-1262 | 500 | 1 | 6.77 | 6.67 | 6.87 | 414828000 |
| | | 2 | 7.27 | 7.17 | 7.37 | 515546000 |
| | | 3 | 7.55 | 7.45 | 7.65 | 186525000 |
| | | 4 | 7.61 | 7.51 | 7.71 | 288104000 |
| | | 5 | 8.10 | 8.00 | 8.20 | 99503400 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 11:32
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:31:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:24:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 855.5E6 | 517.0E6 | 98.849 | 98.468 |
| 2) SA Decachlor... | 8.695 | 8.641 | 745.7E6 | 175.3E6 | 97.561 | 96.571 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|---------|
| 3) L1 AR-1016-1 | 4.756 | 4.738 | 281.5E6 | 171.4E6 | 983.632 | 974.814 |
| 4) L1 AR-1016-2 | 4.775 | 4.756 | 418.0E6 | 254.3E6 | 981.396 | 963.531 |
| 5) L1 AR-1016-3 | 4.832 | 4.931 | 263.6E6 | 134.6E6 | 981.438 | 971.861 |
| 6) L1 AR-1016-4 | 4.951 | 4.974 | 216.2E6 | 106.9E6 | 983.692 | 960.709 |
| 7) L1 AR-1016-5 | 5.208 | 5.186 | 221.1E6 | 139.2E6 | 971.968 | 969.461 |
| 31) L7 AR-1260-1 | 6.245 | 6.214 | 431.8E6 | 240.3E6 | 951.029 | 958.422 |
| 32) L7 AR-1260-2 | 6.435 | 6.402 | 673.4E6 | 317.2E6 | 964.504 | 972.683 |
| 33) L7 AR-1260-3 | 6.801 | 6.554 | 611.3E6 | 256.2E6 | 1000.788 | 975.155 |
| 34) L7 AR-1260-4 | 7.061 | 7.023 | 447.3E6 | 185.7E6 | 971.795 | 969.934 |
| 35) L7 AR-1260-5 | 7.304 | 7.265 | 1262.7E6 | 419.2E6 | 971.370 | 983.719 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112414.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 11:32
 Operator : YP/AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:31:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:24:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

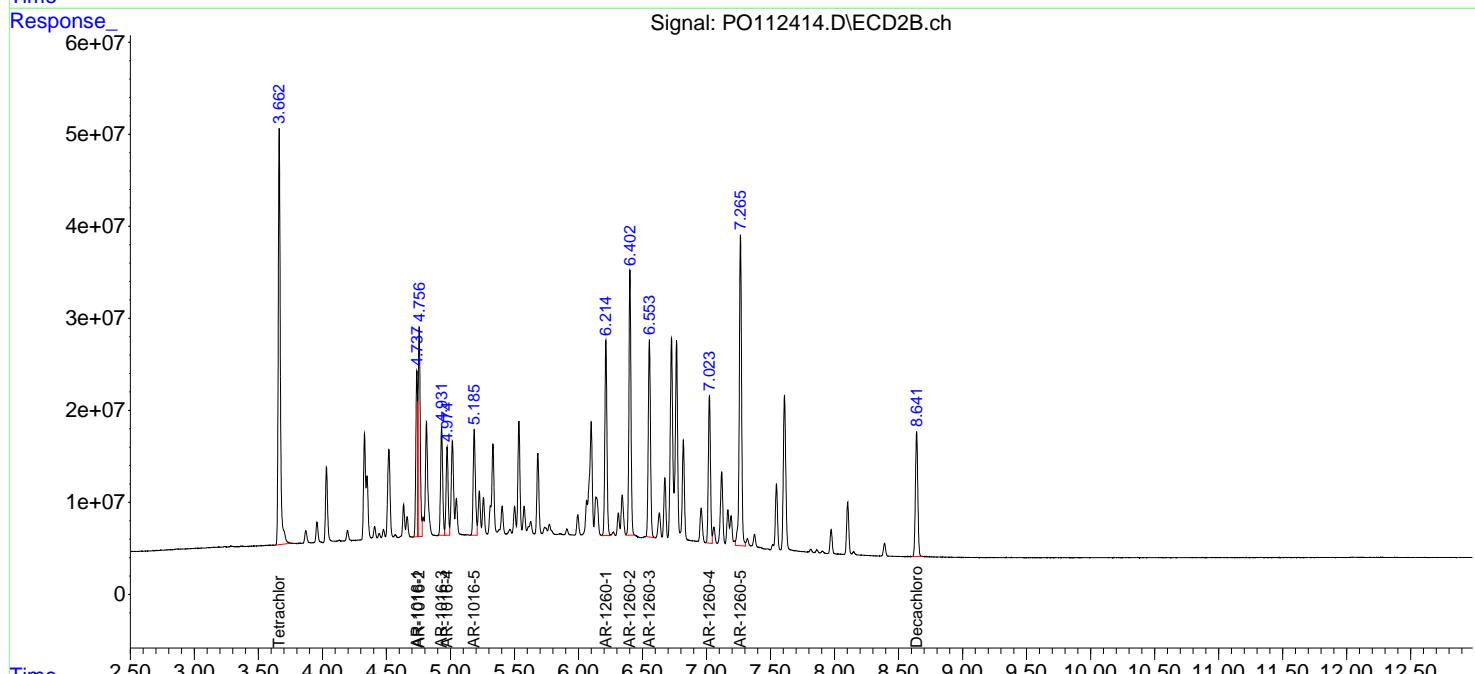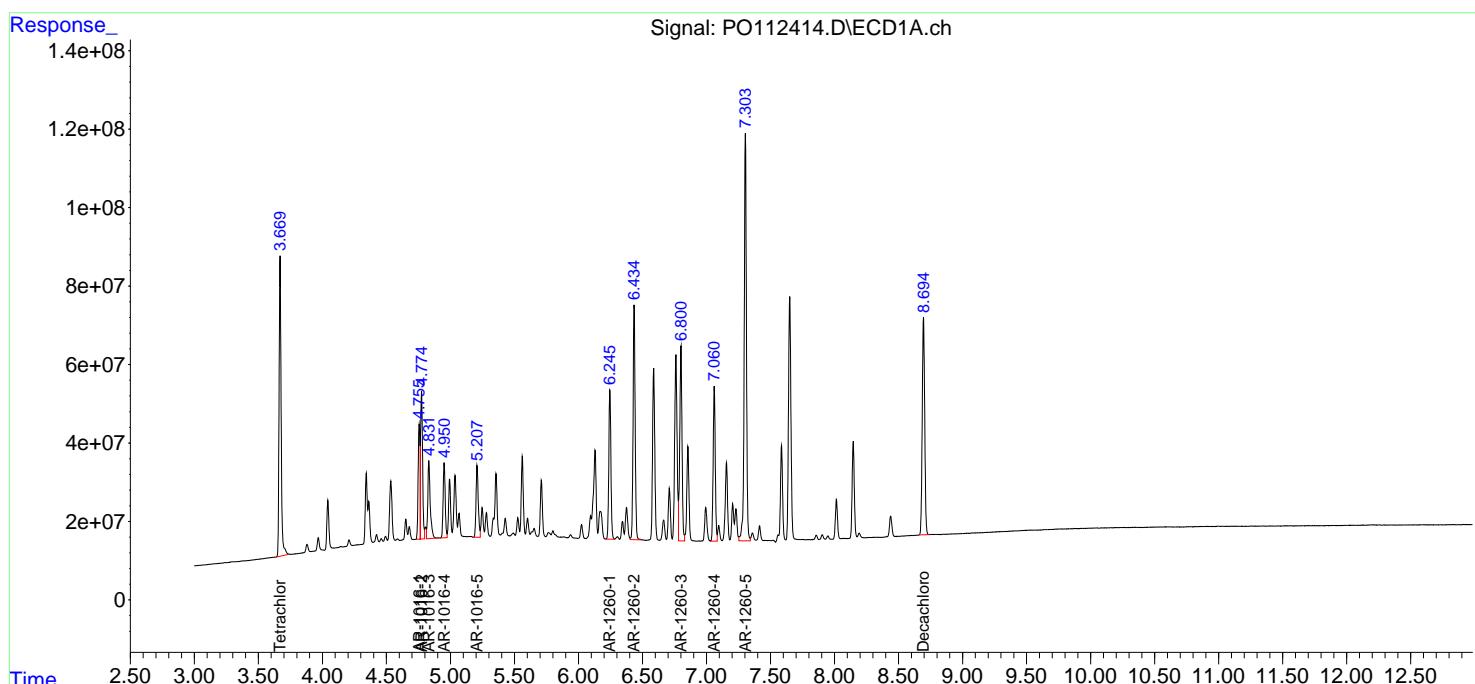

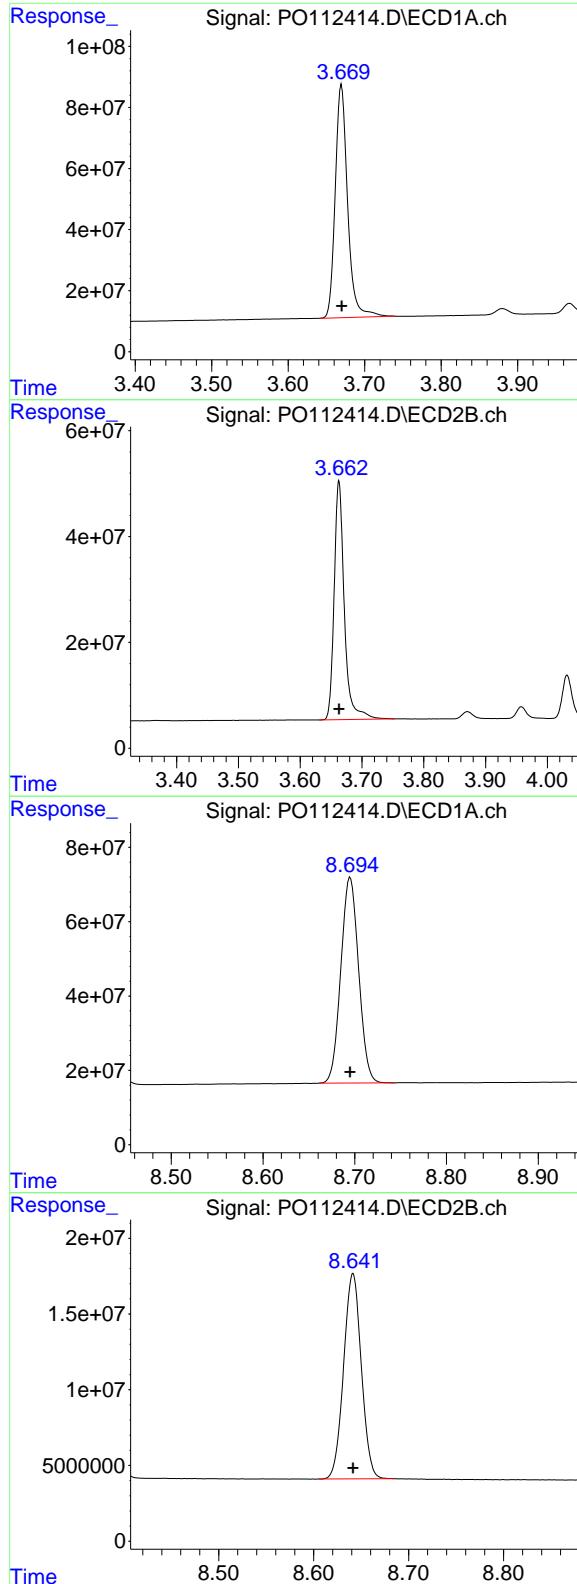

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 855486366
Conc: 98.85 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 516966670
Conc: 98.47 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 745668402
Conc: 97.56 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 175329566
Conc: 96.57 ng/ml

#3 AR-1016-1


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 281481703
 Conc: 983.63 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000




#3 AR-1016-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 171399488
 Conc: 974.81 ng/ml

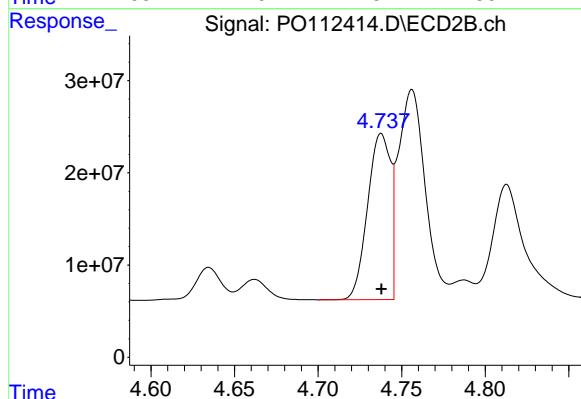


#4 AR-1016-2

R.T.: 4.775 min
 Delta R.T.: 0.000 min
 Response: 418001550
 Conc: 981.40 ng/ml

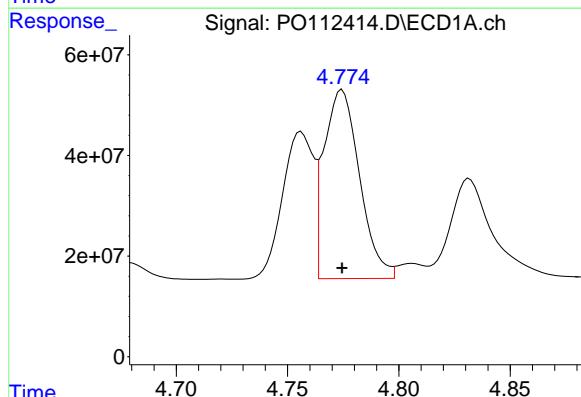

#4 AR-1016-2


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 254283756
 Conc: 963.53 ng/ml

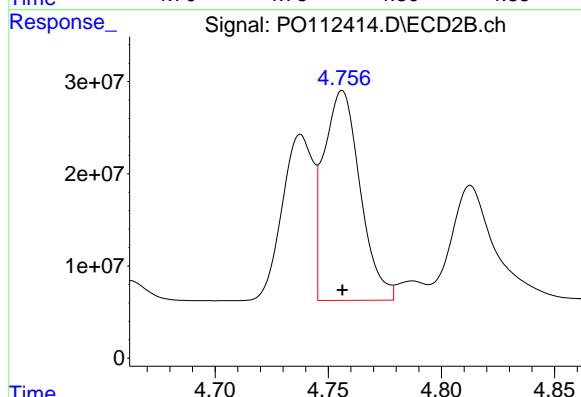

#5 AR-1016-3


R.T.: 4.832 min
 Delta R.T.: 0.000 min
 Response: 263638281
 Conc: 981.44 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

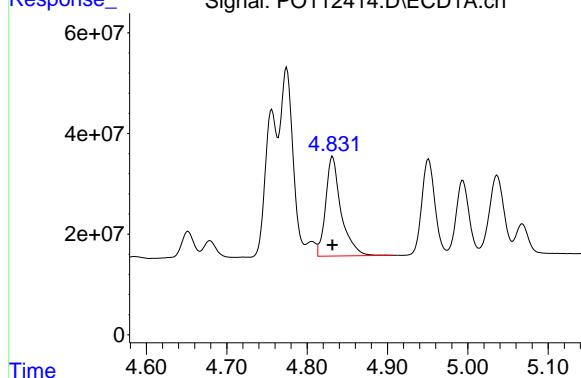


#5 AR-1016-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 134555314
 Conc: 971.86 ng/ml

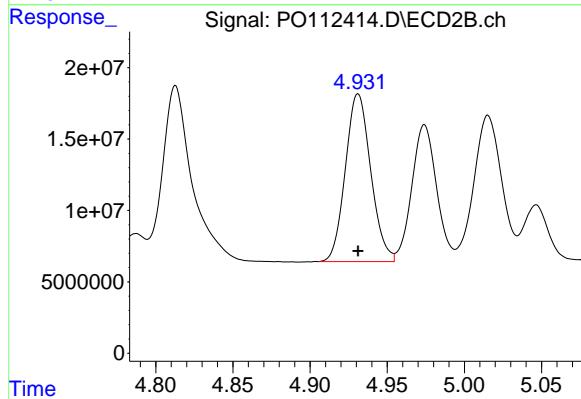


#6 AR-1016-4





R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 216165184
 Conc: 983.69 ng/ml

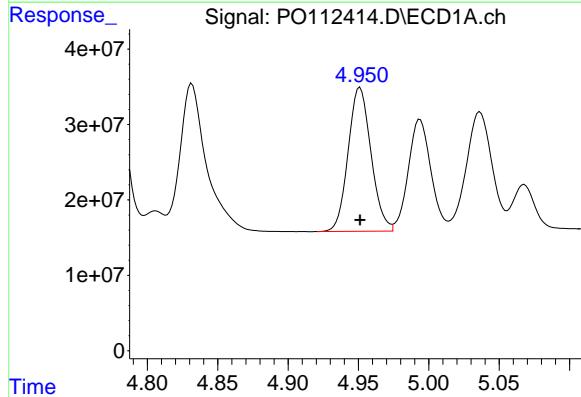

#6 AR-1016-4

R.T.: 4.974 min
 Delta R.T.: 0.000 min
 Response: 106915956
 Conc: 960.71 ng/ml

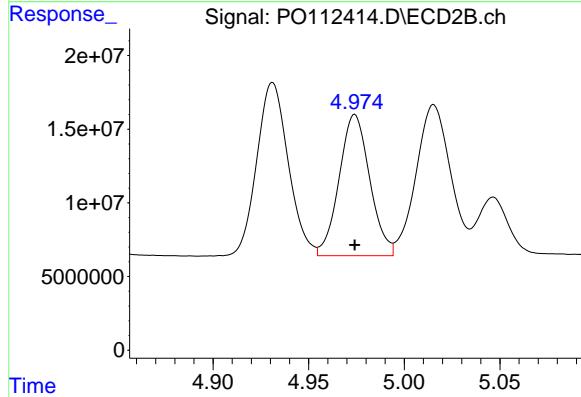

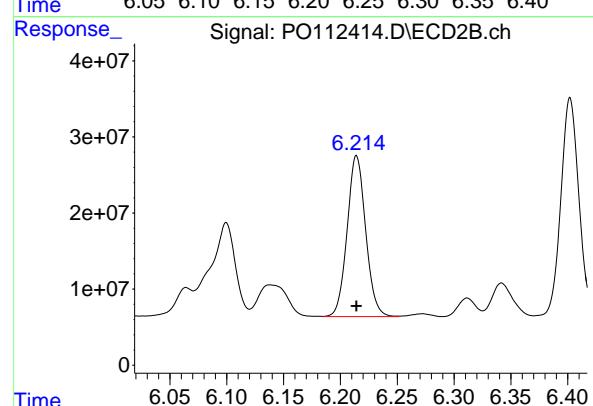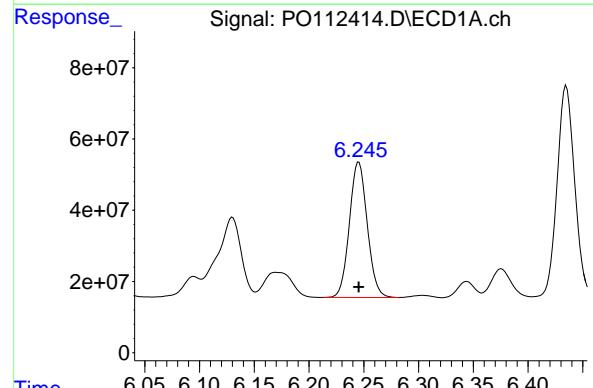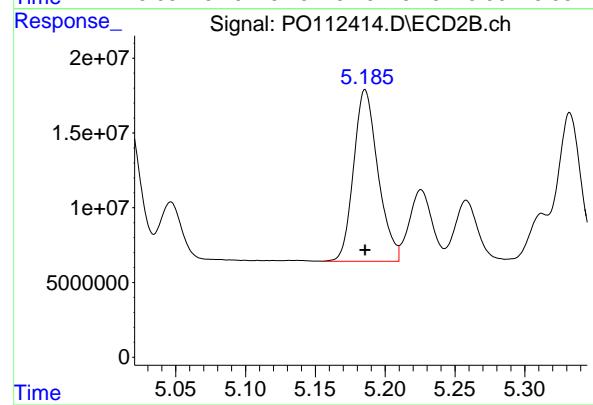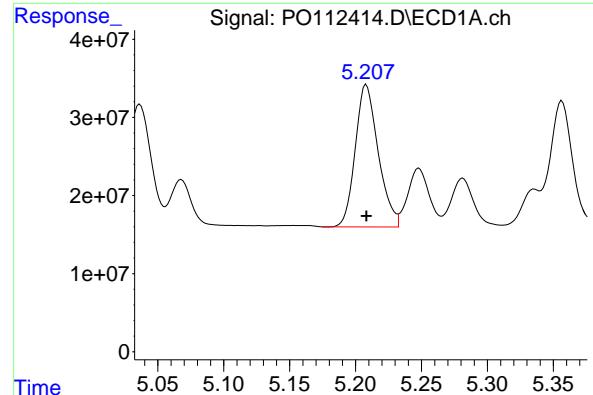

#7 AR-1016-5

R.T.: 5.208 min
 Delta R.T.: 0.000 min
 Response: 221113370
 Conc: 971.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC1000

#7 AR-1016-5

R.T.: 5.186 min
 Delta R.T.: 0.000 min
 Response: 139169322
 Conc: 969.46 ng/ml

#31 AR-1260-1

R.T.: 6.245 min
 Delta R.T.: 0.000 min
 Response: 431773857
 Conc: 951.03 ng/ml





#31 AR-1260-1

R.T.: 6.214 min
 Delta R.T.: 0.000 min
 Response: 240286237
 Conc: 958.42 ng/ml

#32 AR-1260-2

R.T.: 6.435 min
 Delta R.T.: 0.000 min
 Response: 673380136
 Conc: 964.50 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

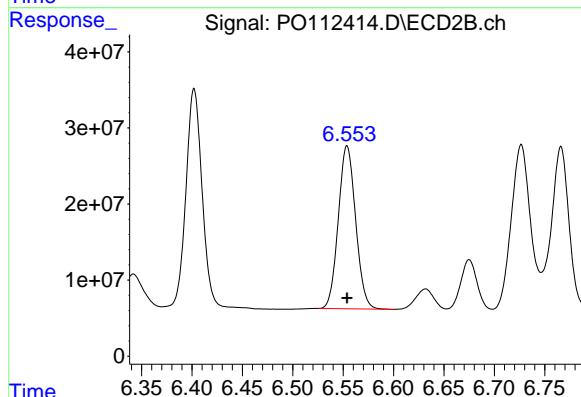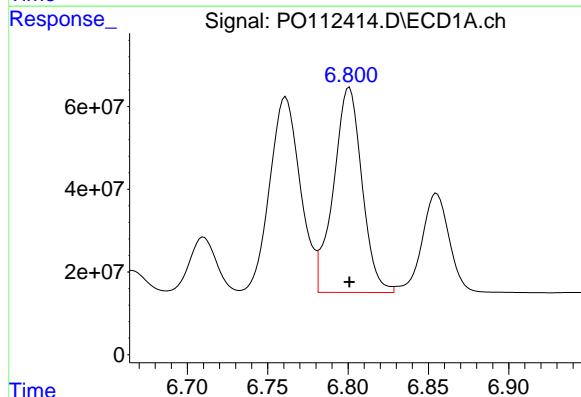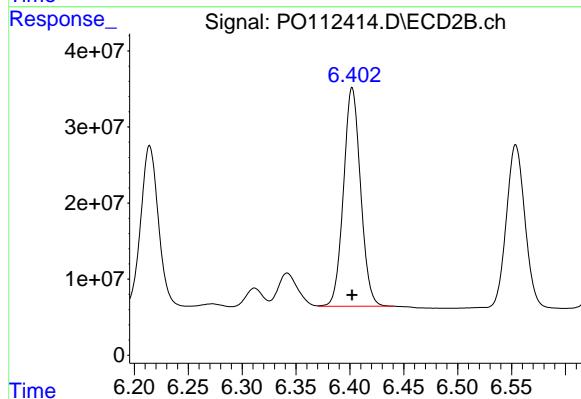

#32 AR-1260-2


R.T.: 6.402 min
 Delta R.T.: 0.000 min
 Response: 317223235
 Conc: 972.68 ng/ml

#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: 0.000 min
 Response: 611274773
 Conc: 1000.79 ng/ml

#33 AR-1260-3

R.T.: 6.554 min
 Delta R.T.: 0.000 min
 Response: 256241072
 Conc: 975.16 ng/ml

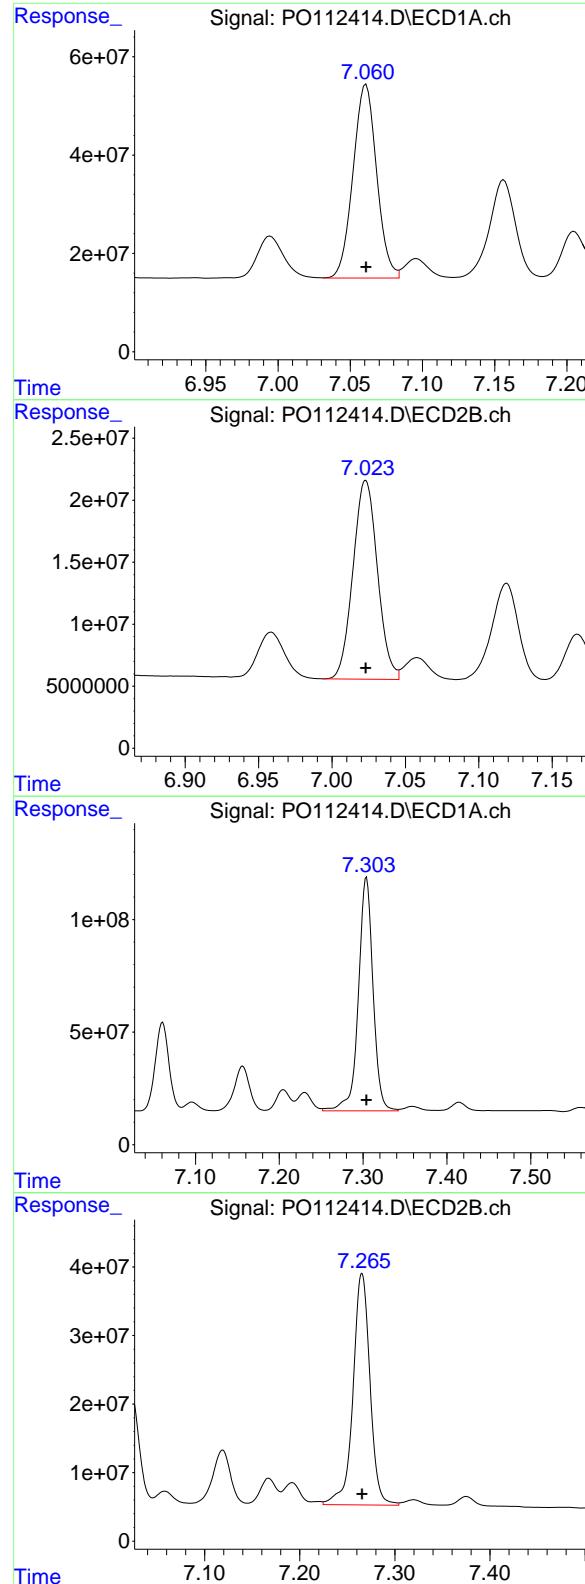

#34 AR-1260-4

R.T.: 7.061 min
Delta R.T.: 0.000 min
Response: 447285263
Conc: 971.80 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC1000

#34 AR-1260-4

R.T.: 7.023 min
Delta R.T.: 0.000 min
Response: 185740526
Conc: 969.93 ng/ml

#35 AR-1260-5

R.T.: 7.304 min
Delta R.T.: 0.000 min
Response: 1262689005
Conc: 971.37 ng/ml

#35 AR-1260-5

R.T.: 7.265 min
Delta R.T.: 0.000 min
Response: 419199446
Conc: 983.72 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 11:50
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:34:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:24:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.668 | 3.662 | 656.3E6 | 398.6E6 | 75.555 | 75.614 |
| 2) SA Decachlor... | 8.692 | 8.640 | 575.7E6 | 136.6E6 | 75.217 | 75.145 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 3) L1 AR-1016-1 | 4.754 | 4.738 | 213.9E6 | 133.4E6 | 748.220 | 755.950 |
| 4) L1 AR-1016-2 | 4.772 | 4.756 | 323.9E6 | 199.5E6 | 756.926 | 754.066 |
| 5) L1 AR-1016-3 | 4.829 | 4.931 | 205.3E6 | 104.5E6 | 759.562 | 753.309 |
| 6) L1 AR-1016-4 | 4.949 | 4.973 | 164.5E6 | 83762683 | 748.907 | 751.773 |
| 7) L1 AR-1016-5 | 5.206 | 5.185 | 171.2E6 | 108.6E6 | 751.707 | 754.159 |
| 31) L7 AR-1260-1 | 6.243 | 6.213 | 337.5E6 | 190.5E6 | 745.576 | 756.618 |
| 32) L7 AR-1260-2 | 6.433 | 6.401 | 523.7E6 | 247.2E6 | 750.066 | 755.338 |
| 33) L7 AR-1260-3 | 6.798 | 6.553 | 470.4E6 | 197.0E6 | 763.349 | 749.871 |
| 34) L7 AR-1260-4 | 7.058 | 7.022 | 345.8E6 | 145.1E6 | 750.847 | 755.131 |
| 35) L7 AR-1260-5 | 7.301 | 7.264 | 963.0E6 | 316.2E6 | 743.842 | 744.651 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 11:50
 Operator : YP/AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:34:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:24:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

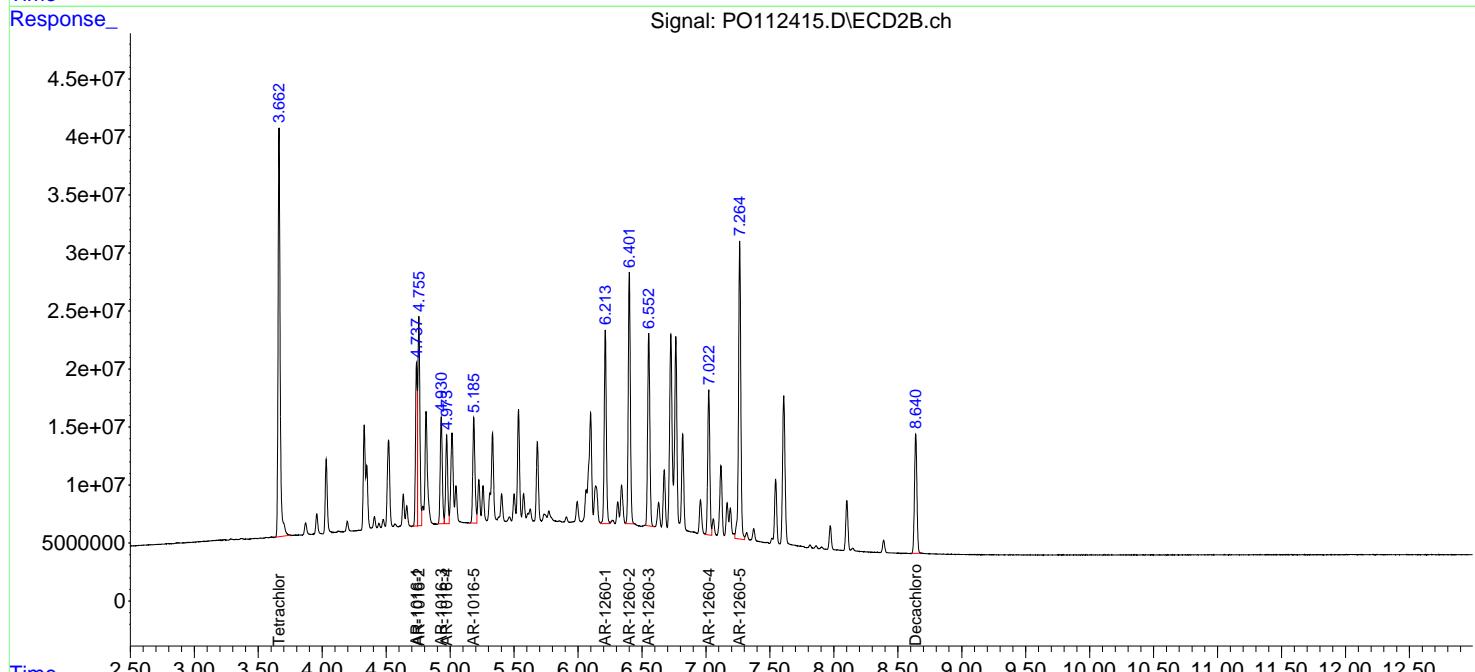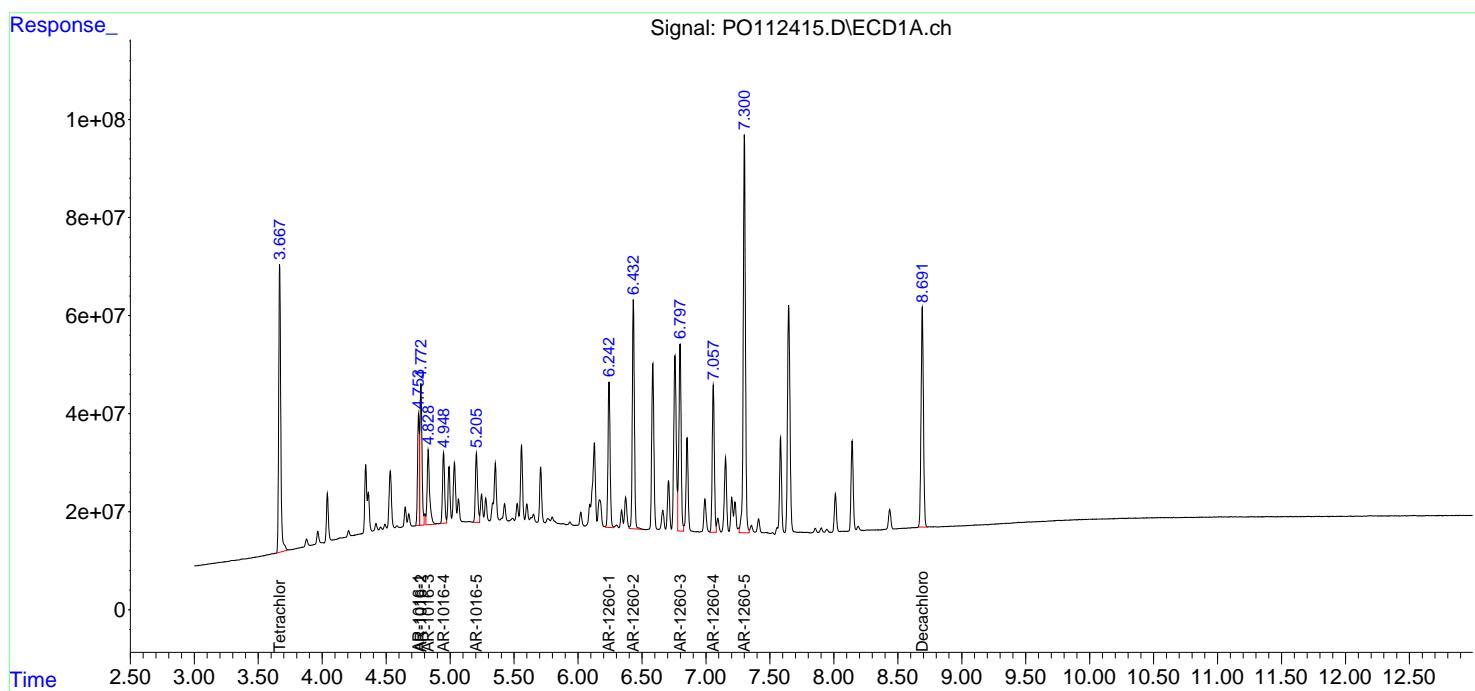

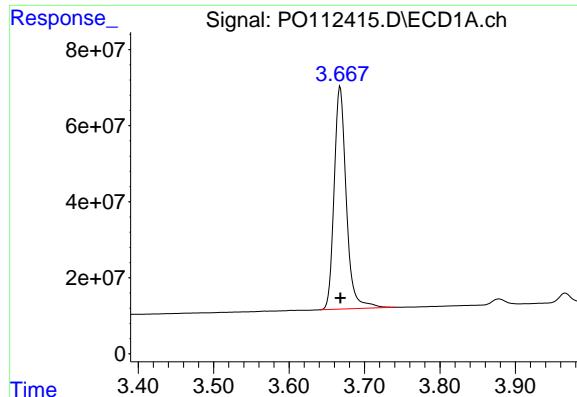

#1 Tetrachloro-m-xylene


R.T.: 3.668 min

Delta R.T.: 0.000 min

Instrument: ECD_O

Response: 656313605

Conc: 75.55 ng/ml

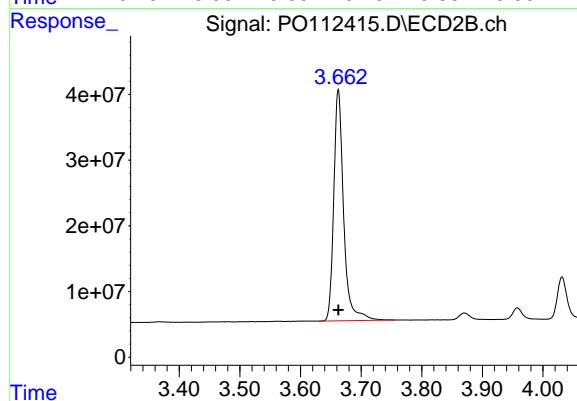


#1 Tetrachloro-m-xylene

R.T.: 3.662 min

Delta R.T.: 0.000 min

Response: 398614237

Conc: 75.61 ng/ml

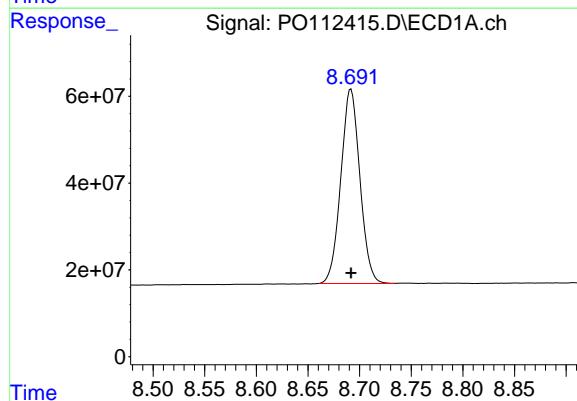


#2 Decachlorobiphenyl

R.T.: 8.692 min

Delta R.T.: 0.000 min

Response: 575718922

Conc: 75.22 ng/ml

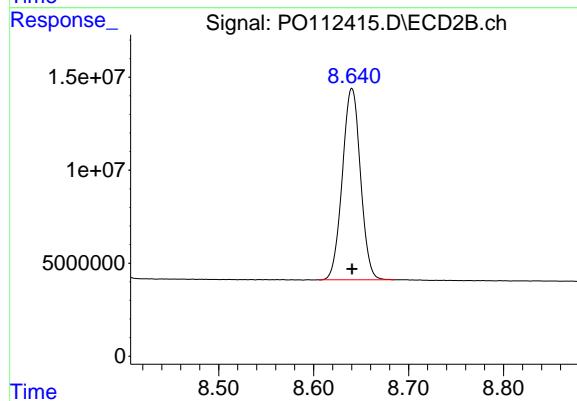

#2 Decachlorobiphenyl

R.T.: 8.640 min

Delta R.T.: 0.000 min


Response: 136562488

Conc: 75.15 ng/ml

#3 AR-1016-1


R.T.: 4.754 min
 Delta R.T.: 0.000 min
 Response: 213861227
 Conc: 748.22 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

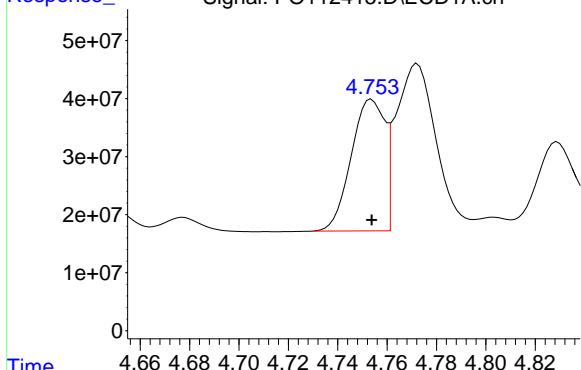


#3 AR-1016-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 133446554
 Conc: 755.95 ng/ml

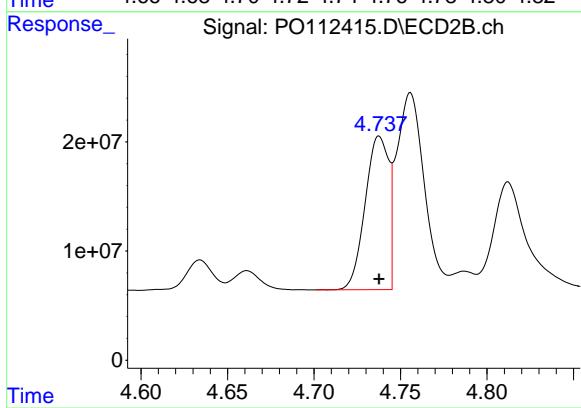


#4 AR-1016-2

R.T.: 4.772 min
 Delta R.T.: 0.000 min
 Response: 323889696
 Conc: 756.93 ng/ml



#4 AR-1016-2





R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 199544914
 Conc: 754.07 ng/ml

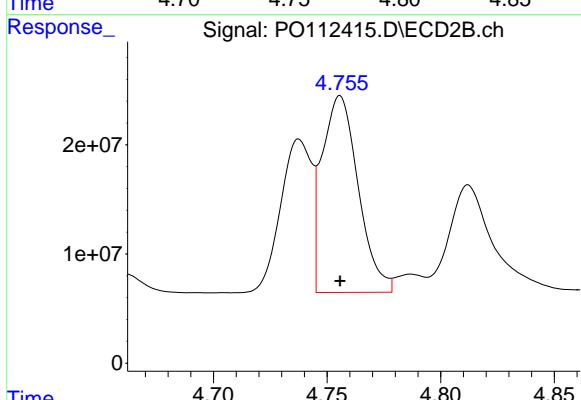

#5 AR-1016-3

R.T.: 4.829 min
 Delta R.T.: 0.000 min
 Response: 205345763
 Conc: 759.56 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

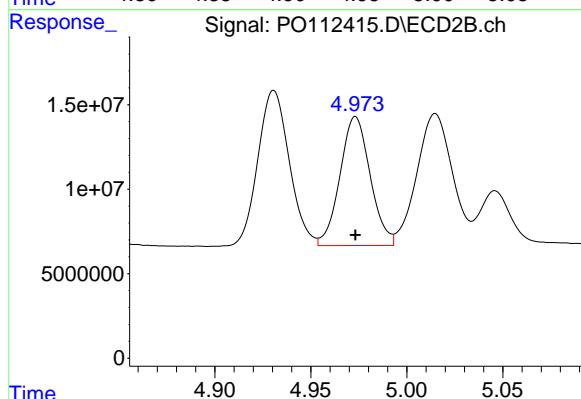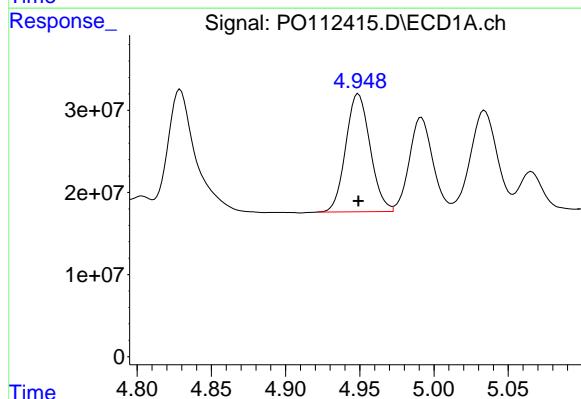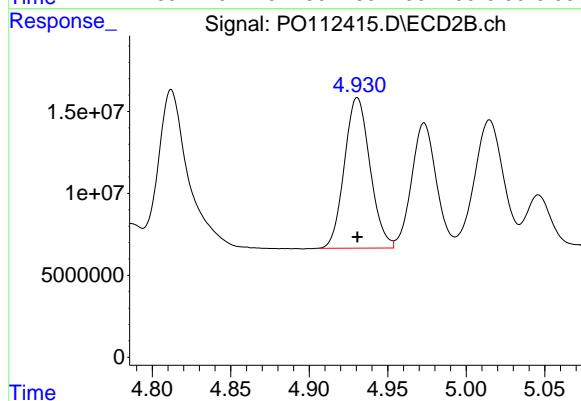

#5 AR-1016-3


R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 104527114
 Conc: 753.31 ng/ml

#6 AR-1016-4

R.T.: 4.949 min
 Delta R.T.: 0.000 min
 Response: 164451540
 Conc: 748.91 ng/ml

#6 AR-1016-4

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 83762683
 Conc: 751.77 ng/ml

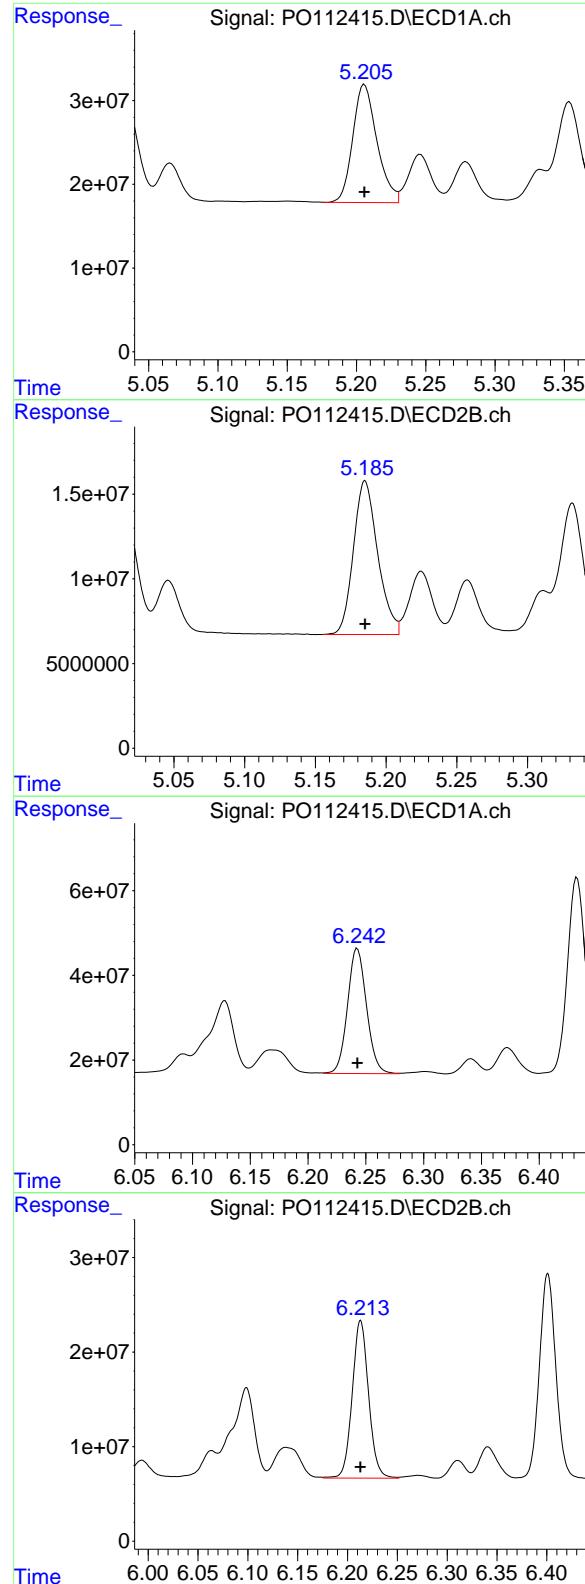

#7 AR-1016-5

R.T.: 5.206 min
 Delta R.T.: 0.000 min
 Response: 171201066
 Conc: 751.71 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC750

#7 AR-1016-5

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 108563069
 Conc: 754.16 ng/ml

#31 AR-1260-1

R.T.: 6.243 min
 Delta R.T.: 0.000 min
 Response: 337501312
 Conc: 745.58 ng/ml


#31 AR-1260-1

R.T.: 6.213 min
 Delta R.T.: 0.000 min
 Response: 190532645
 Conc: 756.62 ng/ml

#32 AR-1260-2


R.T.: 6.433 min
 Delta R.T.: 0.000 min
 Response: 523690898
 Conc: 750.07 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750

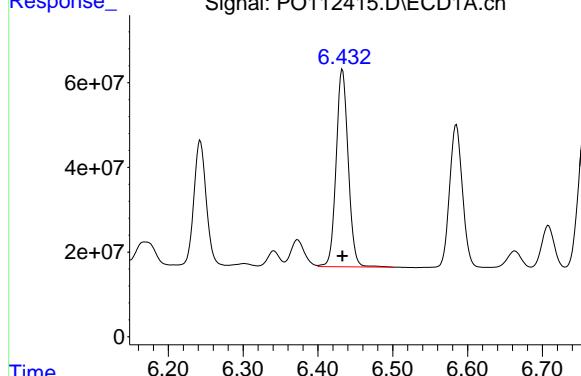


#32 AR-1260-2

R.T.: 6.401 min
 Delta R.T.: 0.000 min
 Response: 247219814
 Conc: 755.34 ng/ml

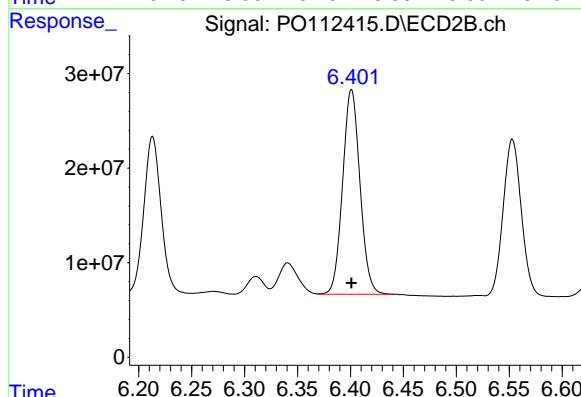


#33 AR-1260-3

R.T.: 6.798 min
 Delta R.T.: 0.000 min
 Response: 470435075
 Conc: 763.35 ng/ml

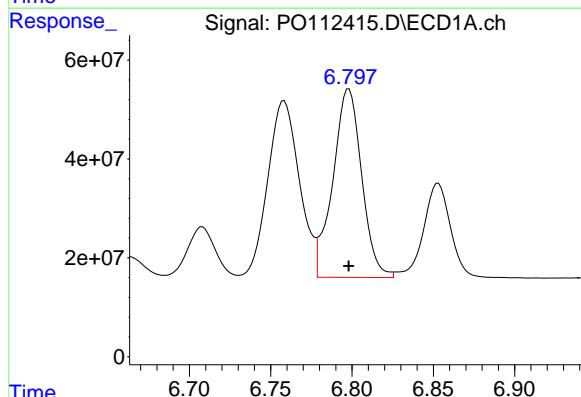

#33 AR-1260-3


R.T.: 6.553 min
 Delta R.T.: 0.000 min
 Response: 197026220
 Conc: 749.87 ng/ml

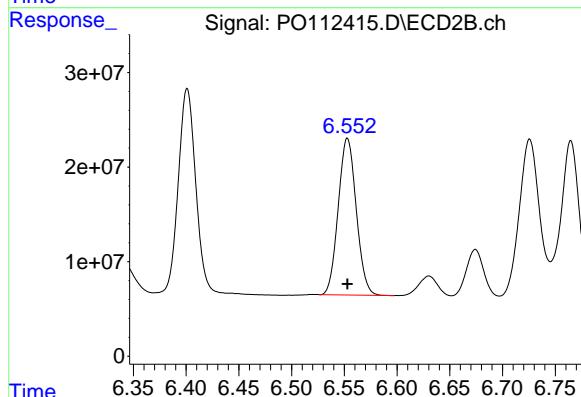

#34 AR-1260-4


R.T.: 7.058 min
 Delta R.T.: 0.000 min
 Response: 345785725
 Conc: 750.85 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC750




#34 AR-1260-4

R.T.: 7.022 min
 Delta R.T.: 0.000 min
 Response: 145102383
 Conc: 755.13 ng/ml

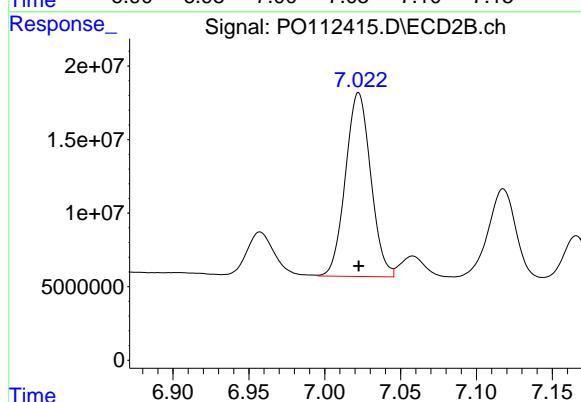


#35 AR-1260-5

R.T.: 7.301 min
 Delta R.T.: 0.000 min
 Response: 962971096
 Conc: 743.84 ng/ml

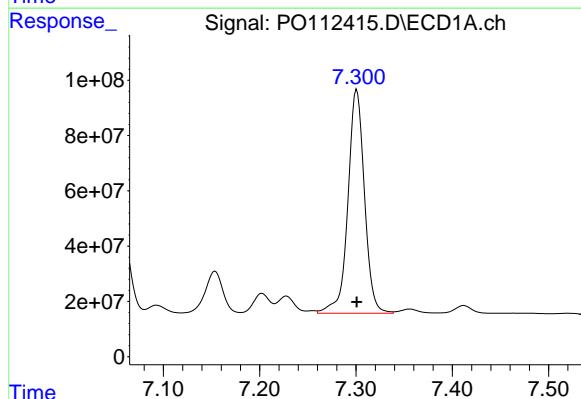

#35 AR-1260-5

R.T.: 7.264 min
 Delta R.T.: 0.000 min
 Response: 316196060
 Conc: 744.65 ng/ml

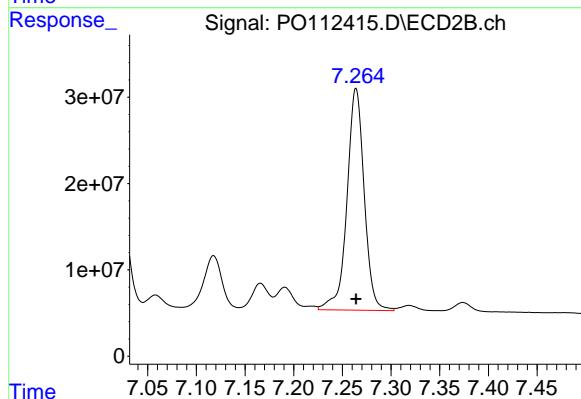

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:08
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:27:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:24:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 437.7E6 | 266.5E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.693 | 8.640 | 391.5E6 | 93890082 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 3) L1 AR-1016-1 | 4.755 | 4.738 | 145.4E6 | 90128163 | 500.000 | 500.000 |
| 4) L1 AR-1016-2 | 4.774 | 4.756 | 216.9E6 | 136.8E6 | 500.000 | 500.000 |
| 5) L1 AR-1016-3 | 4.831 | 4.931 | 136.8E6 | 71173535 | 500.000 | 500.000 |
| 6) L1 AR-1016-4 | 4.951 | 4.973 | 111.7E6 | 57830575 | 500.000 | 500.000 |
| 7) L1 AR-1016-5 | 5.208 | 5.185 | 116.9E6 | 73968656 | 500.000 | 500.000 |
| 31) L7 AR-1260-1 | 6.245 | 6.213 | 238.1E6 | 130.6E6 | 500.000 | 500.000 |
| 32) L7 AR-1260-2 | 6.433 | 6.402 | 361.5E6 | 167.5E6 | 500.000 | 500.000 |
| 33) L7 AR-1260-3 | 6.800 | 6.553 | 305.2E6 | 134.6E6 | 500.000 | 500.000 |
| 34) L7 AR-1260-4 | 7.059 | 7.023 | 236.6E6 | 98627757 | 500.000 | 500.000 |
| 35) L7 AR-1260-5 | 7.303 | 7.264 | 668.6E6 | 216.5E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:08
 Operator : YP/AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:27:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:24:33 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

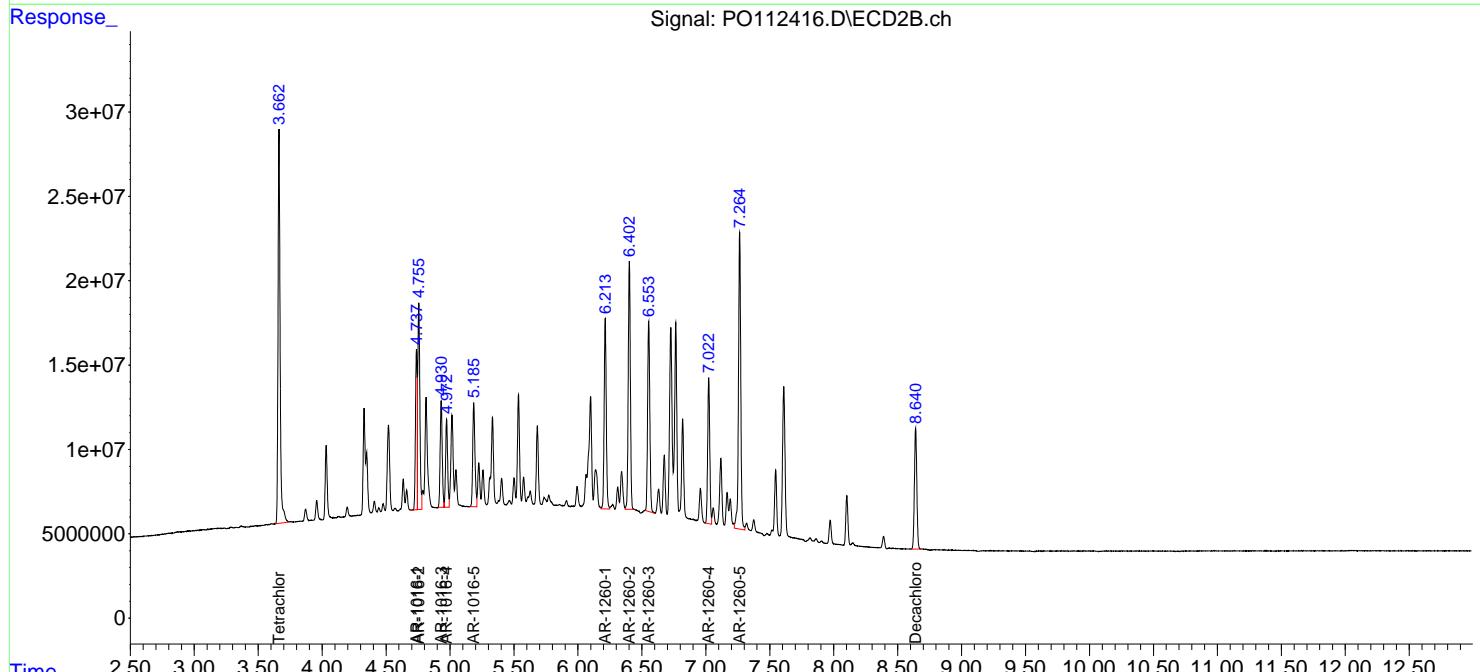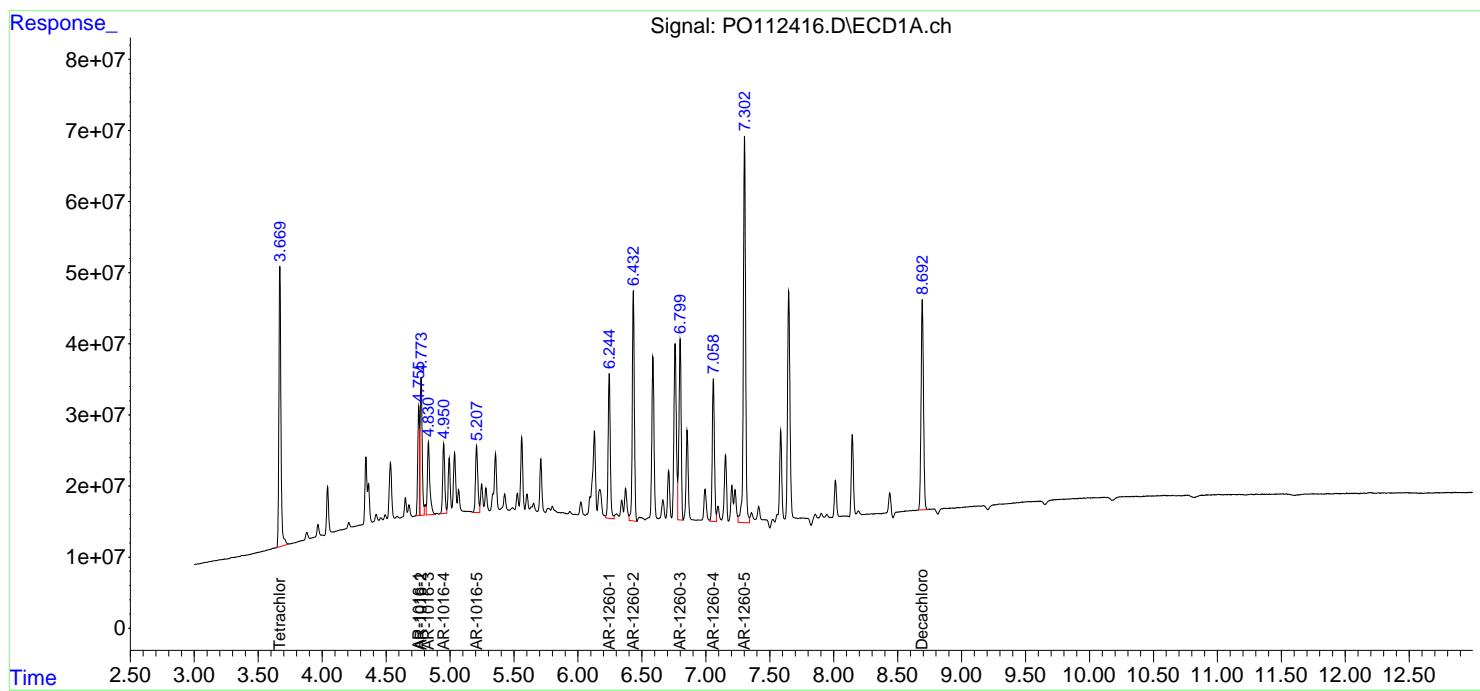

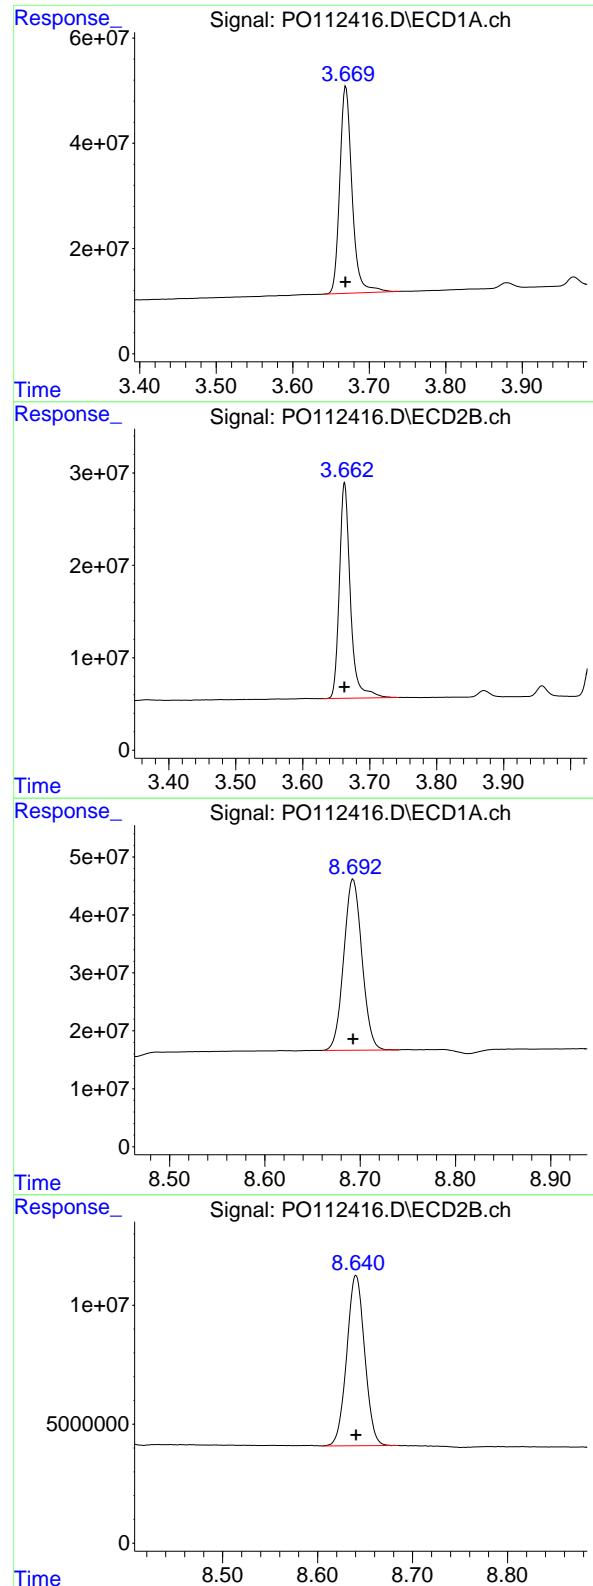

#1 Tetrachloro-m-xylene

R.T.: 3.669 min
 Delta R.T.: 0.000 min
 Response: 437703621
 Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.662 min
 Delta R.T.: 0.000 min
 Response: 266527729
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.693 min
 Delta R.T.: 0.000 min
 Response: 391474769
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
 Delta R.T.: 0.000 min
 Response: 93890082
 Conc: 50.00 ng/ml

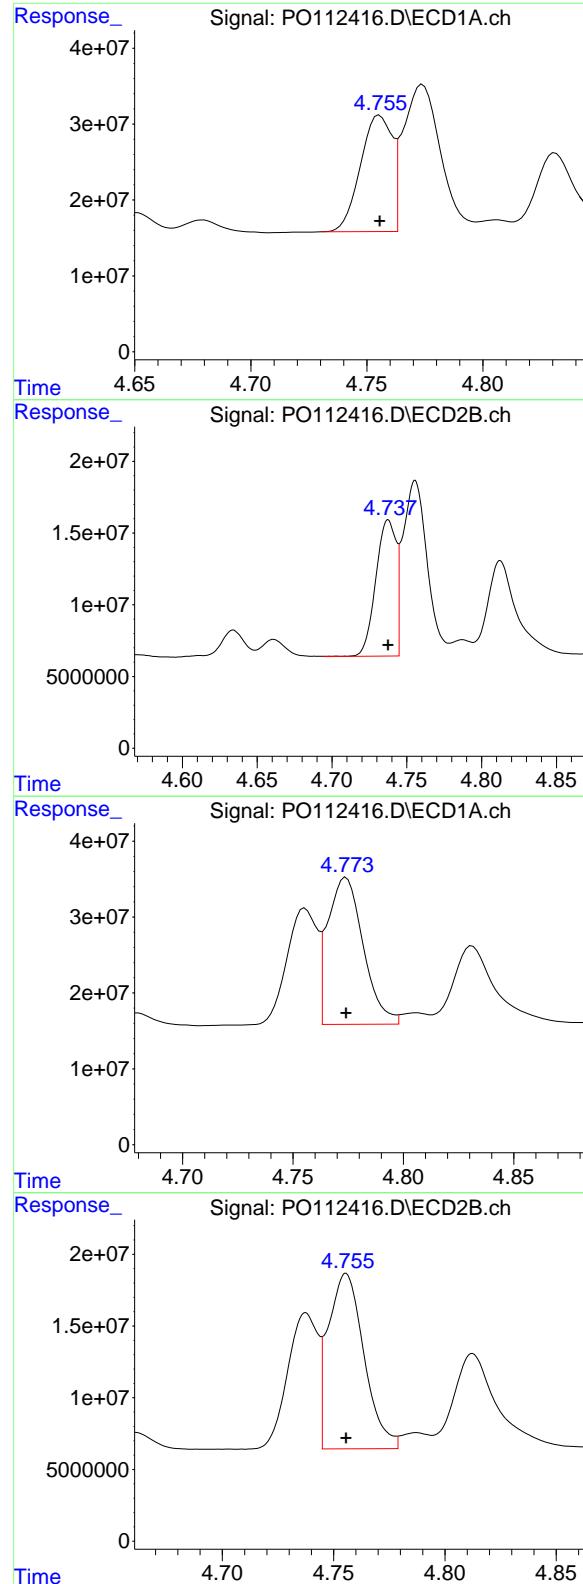

#3 AR-1016-1

R.T.: 4.755 min
 Delta R.T.: 0.000 min
 Response: 145424759
 Conc: 500.00 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC500

#3 AR-1016-1





R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 90128163
 Conc: 500.00 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 216924568
 Conc: 500.00 ng/ml

#4 AR-1016-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 136766267
 Conc: 500.00 ng/ml

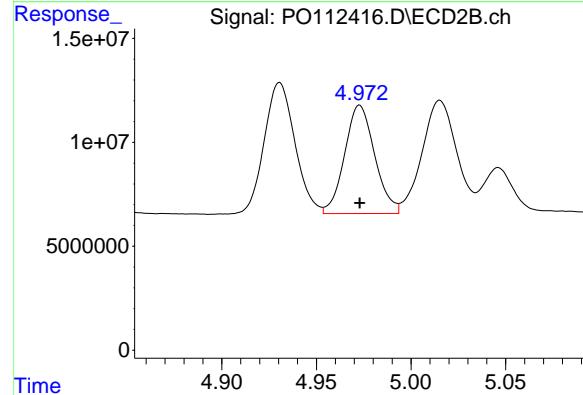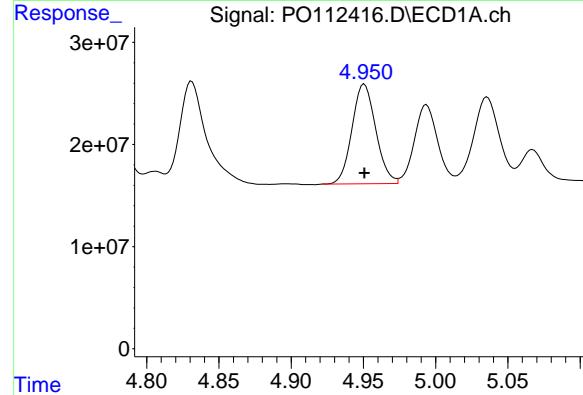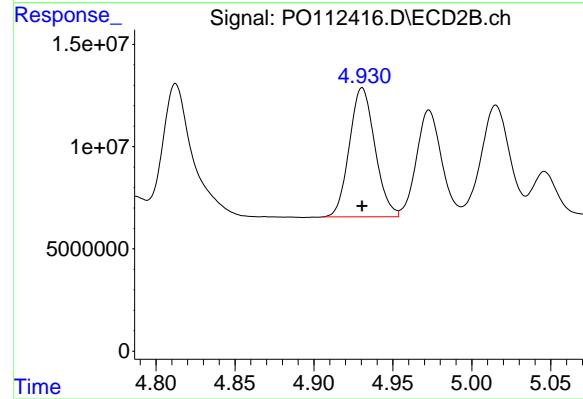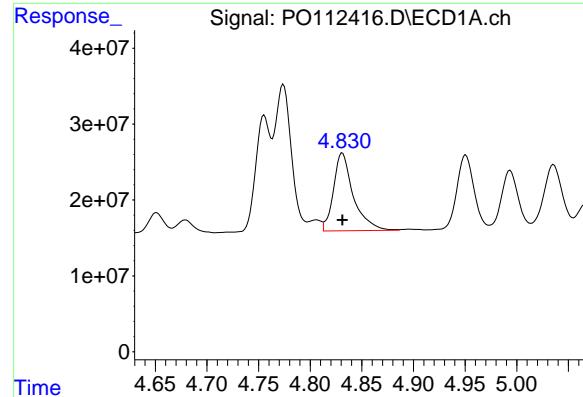

#5 AR-1016-3

R.T.: 4.831 min
 Delta R.T.: 0.000 min
 Response: 136805252
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

#5 AR-1016-3


R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 71173535
 Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 111666354
 Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 57830575
 Conc: 500.00 ng/ml

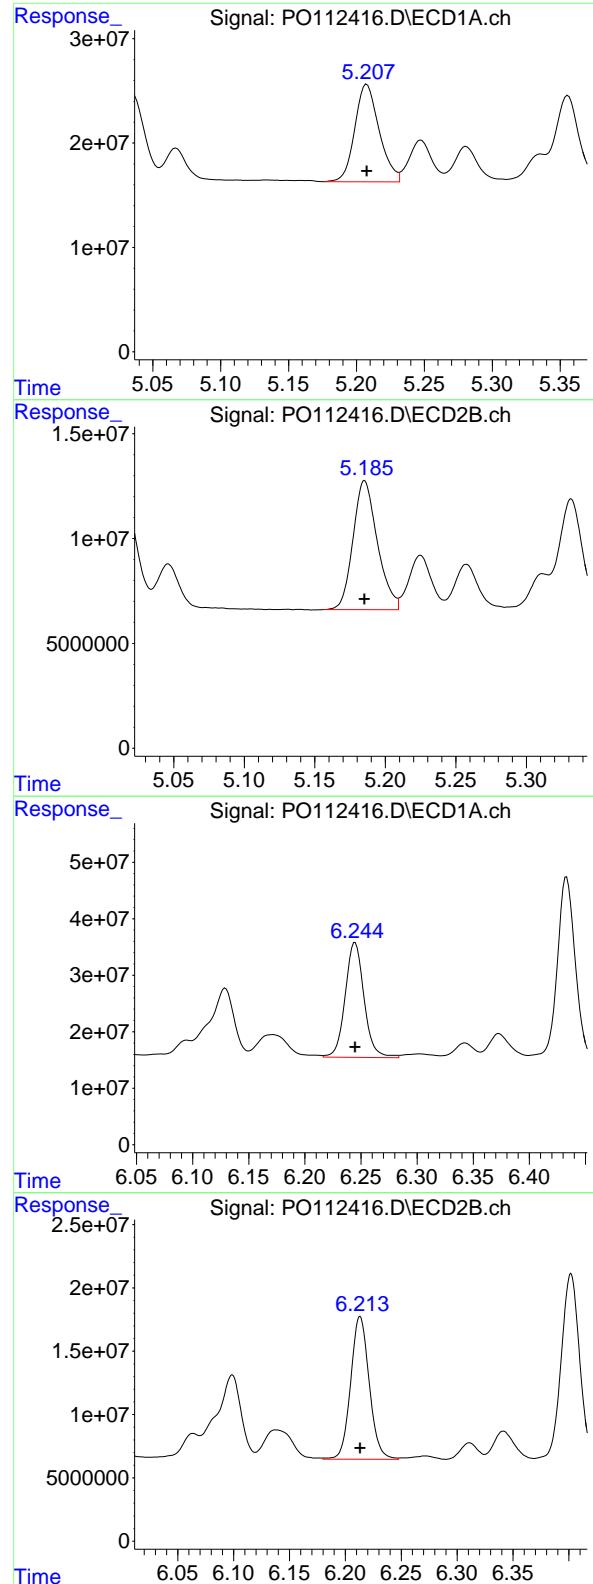

#7 AR-1016-5

R.T.: 5.208 min
 Delta R.T.: 0.000 min
 Response: 116933714
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

#7 AR-1016-5

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 73968656
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 6.245 min
 Delta R.T.: 0.000 min
 Response: 238120143
 Conc: 500.00 ng/ml


#31 AR-1260-1

R.T.: 6.213 min
 Delta R.T.: 0.000 min
 Response: 130567223
 Conc: 500.00 ng/ml

#32 AR-1260-2


R.T.: 6.433 min
 Delta R.T.: 0.000 min
 Response: 361472265
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500




#32 AR-1260-2

R.T.: 6.402 min
 Delta R.T.: 0.000 min
 Response: 167520551
 Conc: 500.00 ng/ml

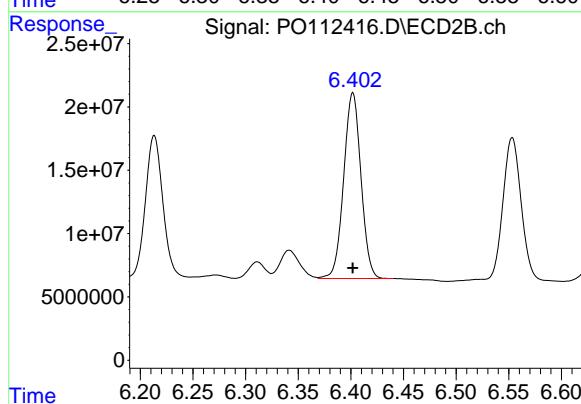


#33 AR-1260-3

R.T.: 6.800 min
 Delta R.T.: 0.000 min
 Response: 305155942
 Conc: 500.00 ng/ml

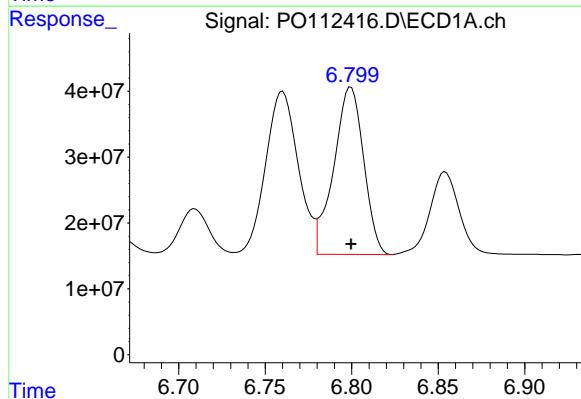

#33 AR-1260-3


R.T.: 6.553 min
 Delta R.T.: 0.000 min
 Response: 134648936
 Conc: 500.00 ng/ml

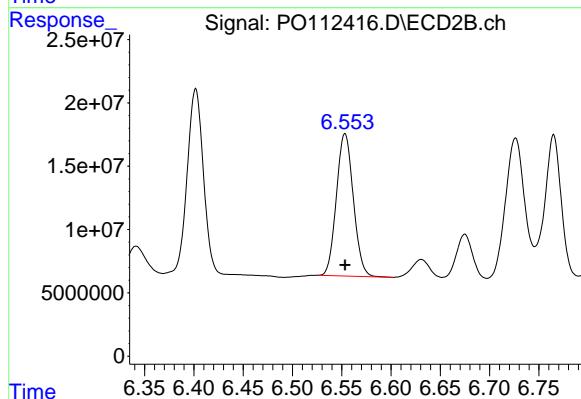

#34 AR-1260-4


R.T.: 7.059 min
 Delta R.T.: 0.000 min
 Response: 236624452
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC500

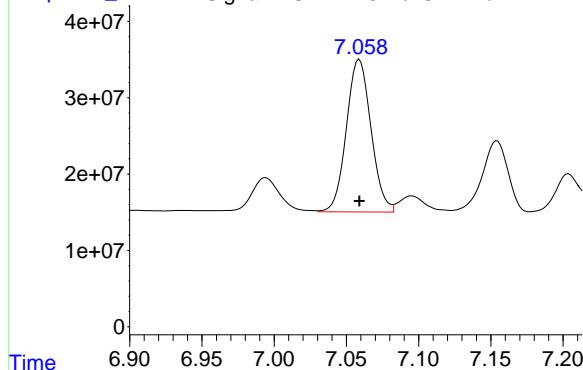


#34 AR-1260-4

R.T.: 7.023 min
 Delta R.T.: 0.000 min
 Response: 98627757
 Conc: 500.00 ng/ml

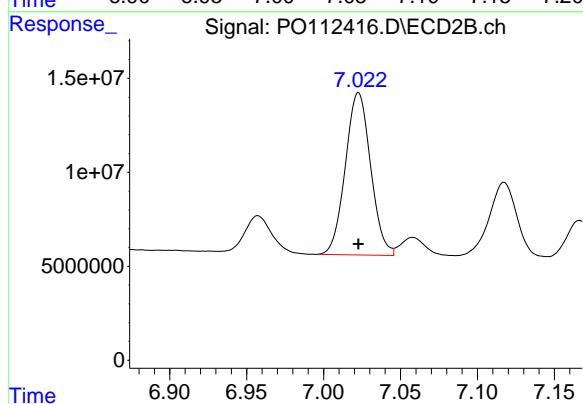


#35 AR-1260-5

R.T.: 7.303 min
 Delta R.T.: 0.000 min
 Response: 668560746
 Conc: 500.00 ng/ml

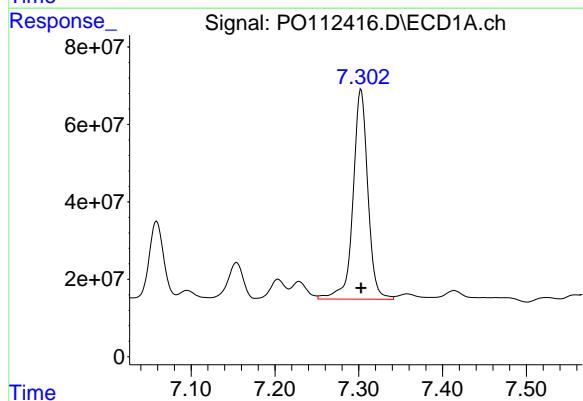

#35 AR-1260-5

R.T.: 7.264 min
 Delta R.T.: 0.000 min
 Response: 216537683
 Conc: 500.00 ng/ml

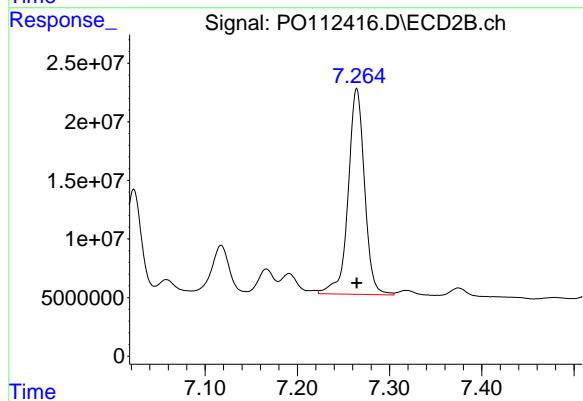

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:27
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:41:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:41:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 207.9E6 | 127.8E6 | 24.188 | 24.425 |
| 2) SA Decachlor... | 8.693 | 8.639 | 191.8E6 | 47304642 | 25.044 | 25.765 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|----------|
| 3) L1 AR-1016-1 | 4.756 | 4.737 | 69875317 | 44959652 | 245.828 | 253.500 |
| 4) L1 AR-1016-2 | 4.774 | 4.756 | 105.2E6 | 68066920 | 246.833 | 255.376 |
| 5) L1 AR-1016-3 | 4.831 | 4.931 | 65721962 | 35251812 | 244.790 | 253.028 |
| 6) L1 AR-1016-4 | 4.951 | 4.973 | 53435135 | 29674672 | 244.973 | 262.052 |
| 7) L1 AR-1016-5 | 5.207 | 5.185 | 58842499 | 38084113 | 256.222 | 260.764 |
| 31) L7 AR-1260-1 | 6.243 | 6.213 | 111.9E6 | 64510353 | 248.096m | 249.850m |
| 32) L7 AR-1260-2 | 6.433 | 6.401 | 171.6E6 | 85155201 | 247.077m | 257.556 |
| 33) L7 AR-1260-3 | 6.800 | 6.552 | 153.7E6 | 68977690 | 249.524 | 262.028m |
| 34) L7 AR-1260-4 | 7.059 | 7.022 | 126.3E6 | 50234042 | 267.727 | 258.471 |
| 35) L7 AR-1260-5 | 7.302 | 7.264 | 336.9E6 | 108.7E6 | 257.581 | 254.474 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:27
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:41:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:41:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660ICC250

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

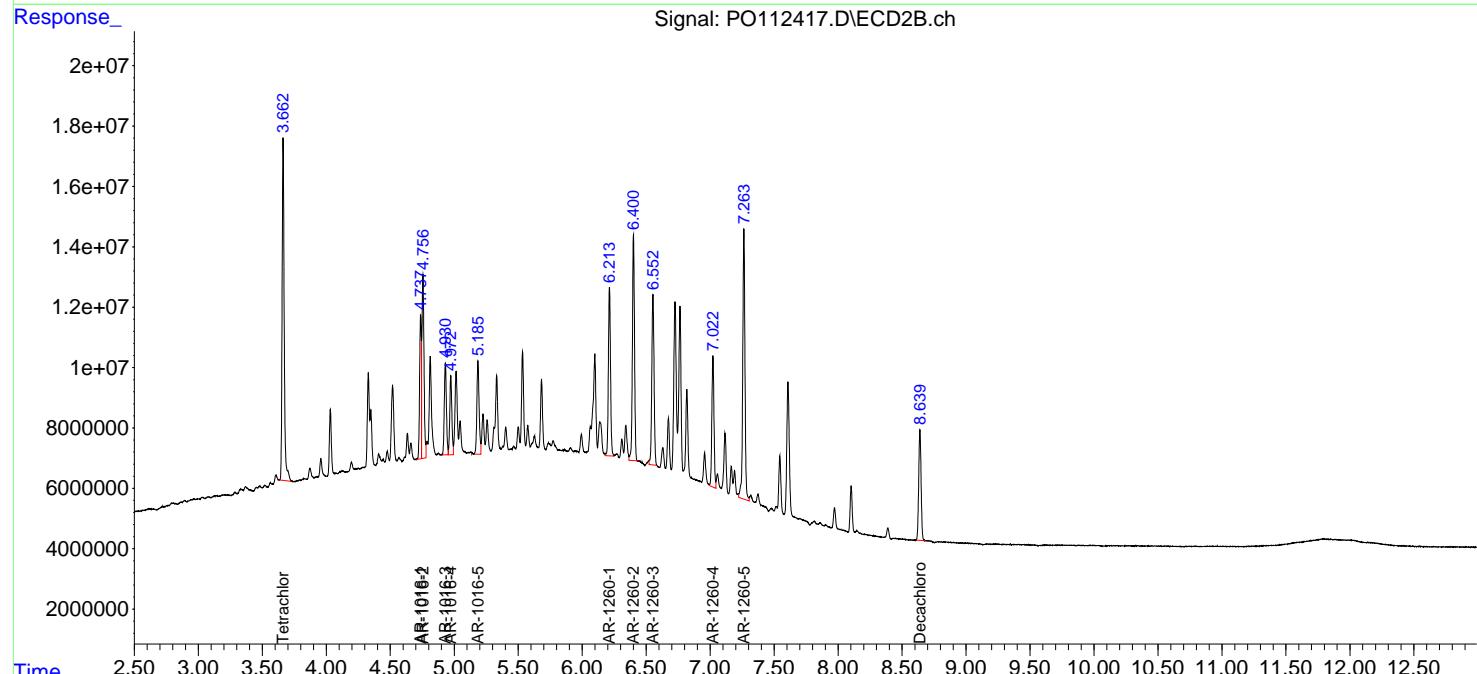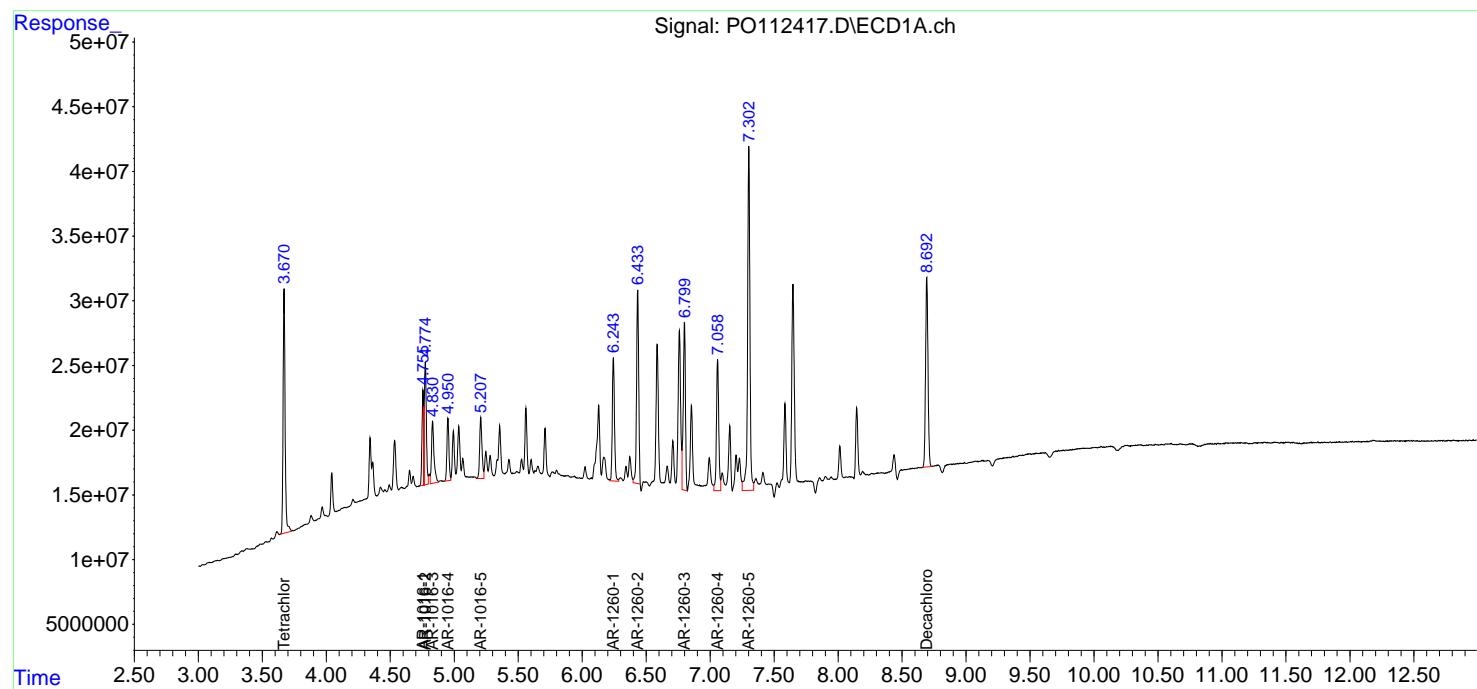

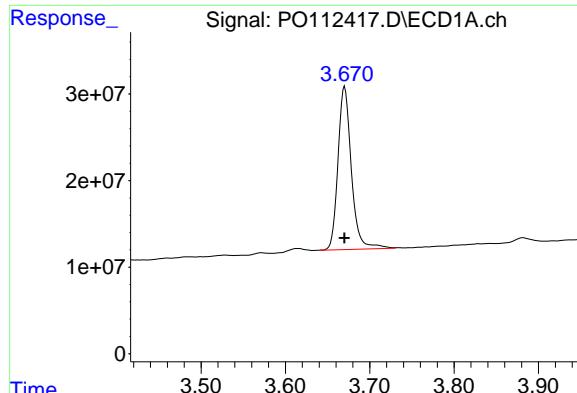


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 207865500
Conc: 24.19 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

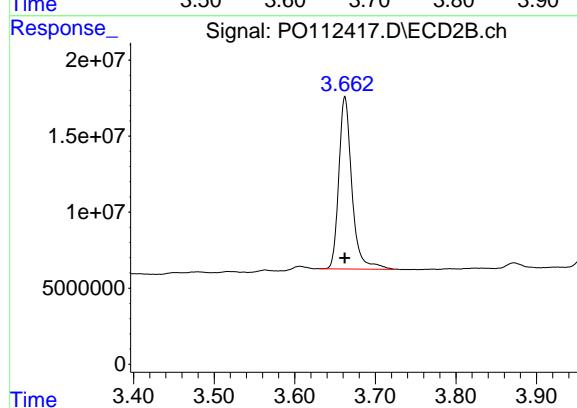


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 127780164
Conc: 24.42 ng/ml

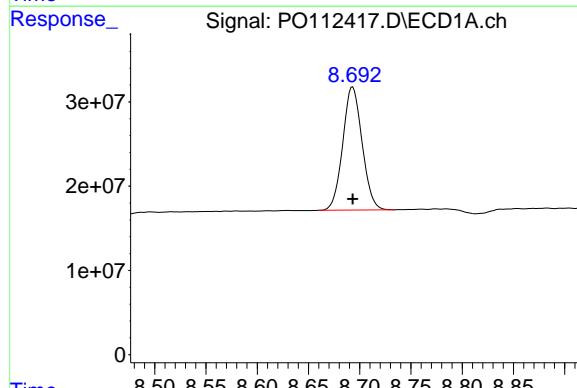


#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 191806392
Conc: 25.04 ng/ml

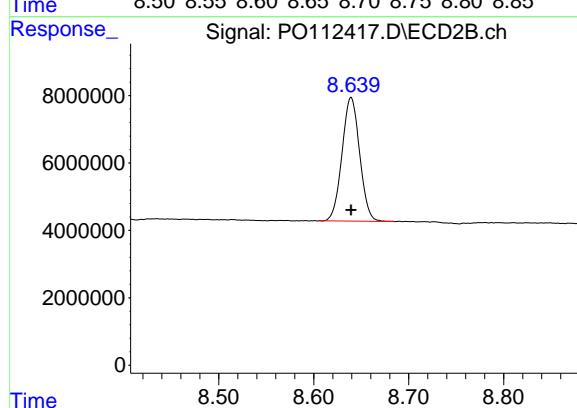

#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 47304642
Conc: 25.76 ng/ml

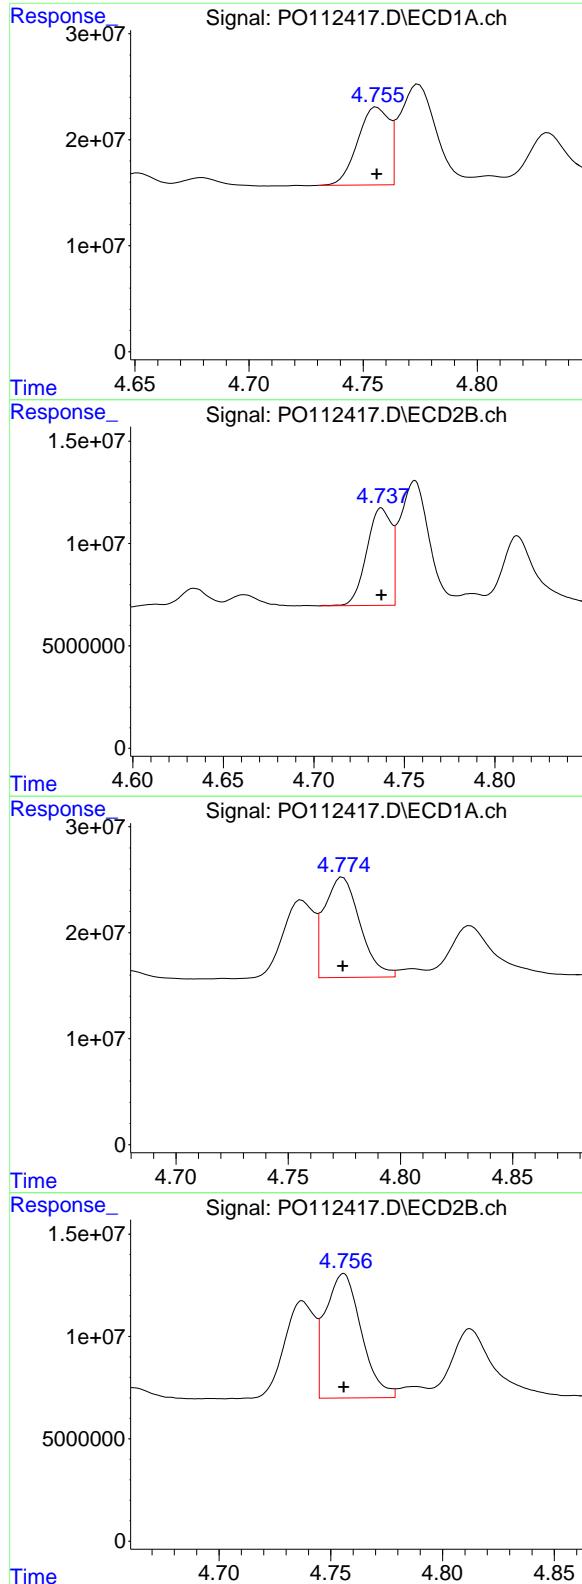

#3 AR-1016-1

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 69875317
Conc: 245.83 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

#3 AR-1016-1


R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 44959652
Conc: 253.50 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 105176225
Conc: 246.83 ng/ml

#4 AR-1016-2

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 68066920
Conc: 255.38 ng/ml

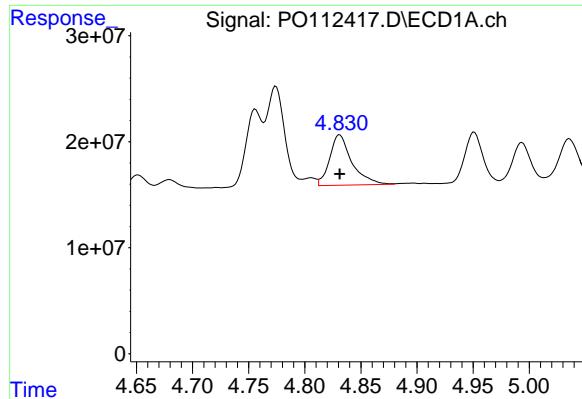


#5 AR-1016-3

R.T.: 4.831 min
Delta R.T.: 0.000 min
Response: 65721962
Conc: 244.79 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

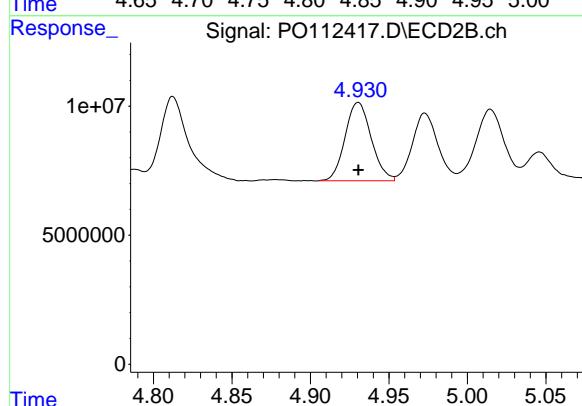


#5 AR-1016-3

R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 35251812
Conc: 253.03 ng/ml

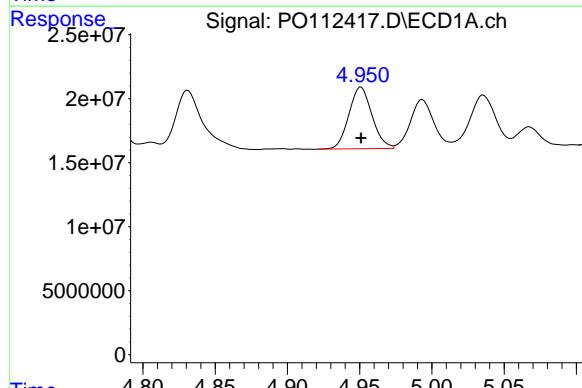


#6 AR-1016-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 53435135
Conc: 244.97 ng/ml

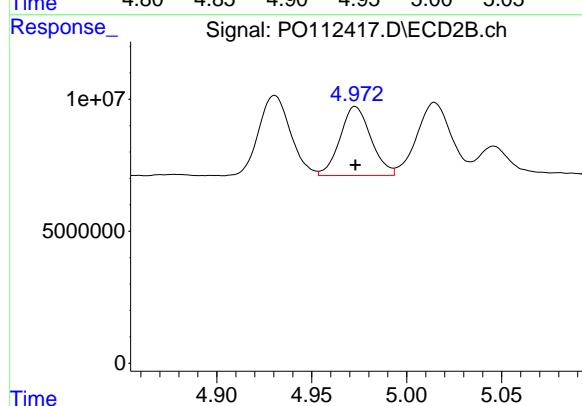

#6 AR-1016-4

R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 29674672
Conc: 262.05 ng/ml

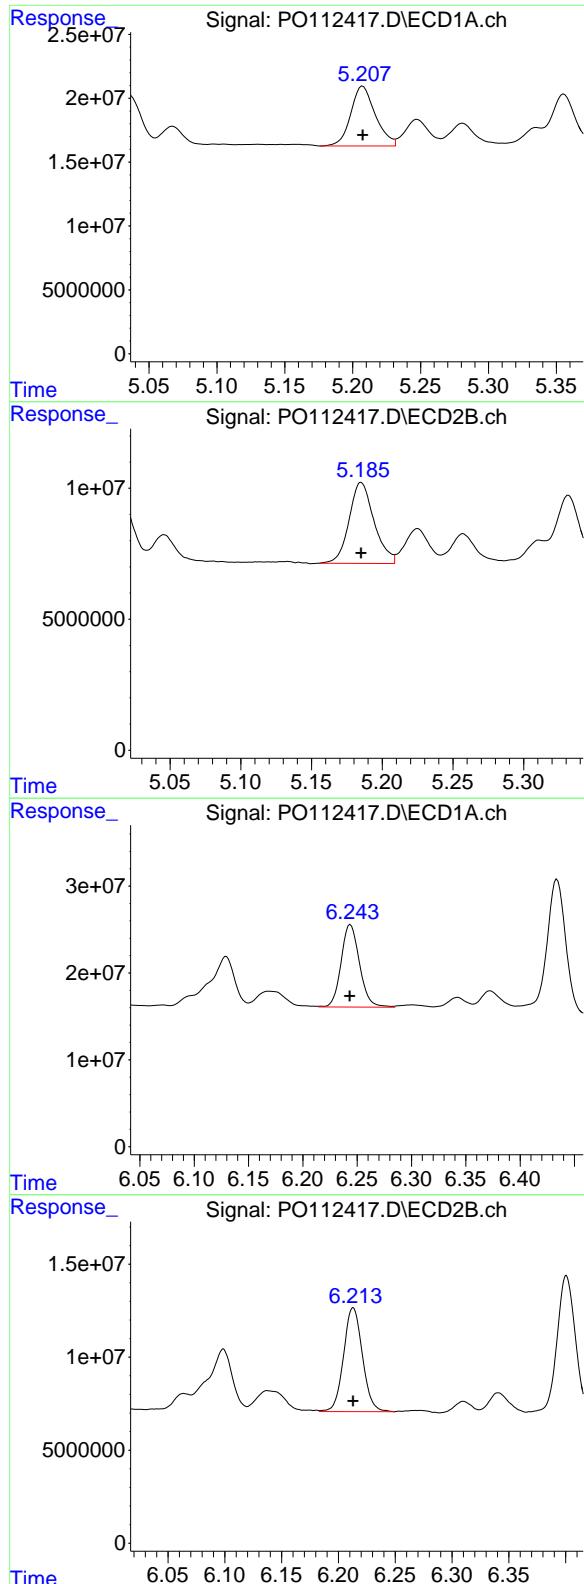

#7 AR-1016-5

R.T.: 5.207 min
 Delta R.T.: 0.000 min
 Response: 58842499
 Conc: 256.22 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#7 AR-1016-5

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 38084113
 Conc: 260.76 ng/ml

#31 AR-1260-1

R.T.: 6.243 min
 Delta R.T.: 0.000 min
 Response: 111903143
 Conc: 248.10 ng/ml

#31 AR-1260-1

R.T.: 6.213 min
 Delta R.T.: 0.000 min
 Response: 64510353
 Conc: 249.85 ng/ml

#32 AR-1260-2

R.T.: 6.433 min
 Delta R.T.: 0.000 min
 Response: 171626516
 Conc: 247.08 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#32 AR-1260-2


R.T.: 6.401 min
 Delta R.T.: 0.000 min
 Response: 85155201
 Conc: 257.56 ng/ml

#33 AR-1260-3

R.T.: 6.800 min
 Delta R.T.: 0.000 min
 Response: 153678285
 Conc: 249.52 ng/ml

#33 AR-1260-3

R.T.: 6.552 min
 Delta R.T.: 0.000 min
 Response: 68977690
 Conc: 262.03 ng/ml

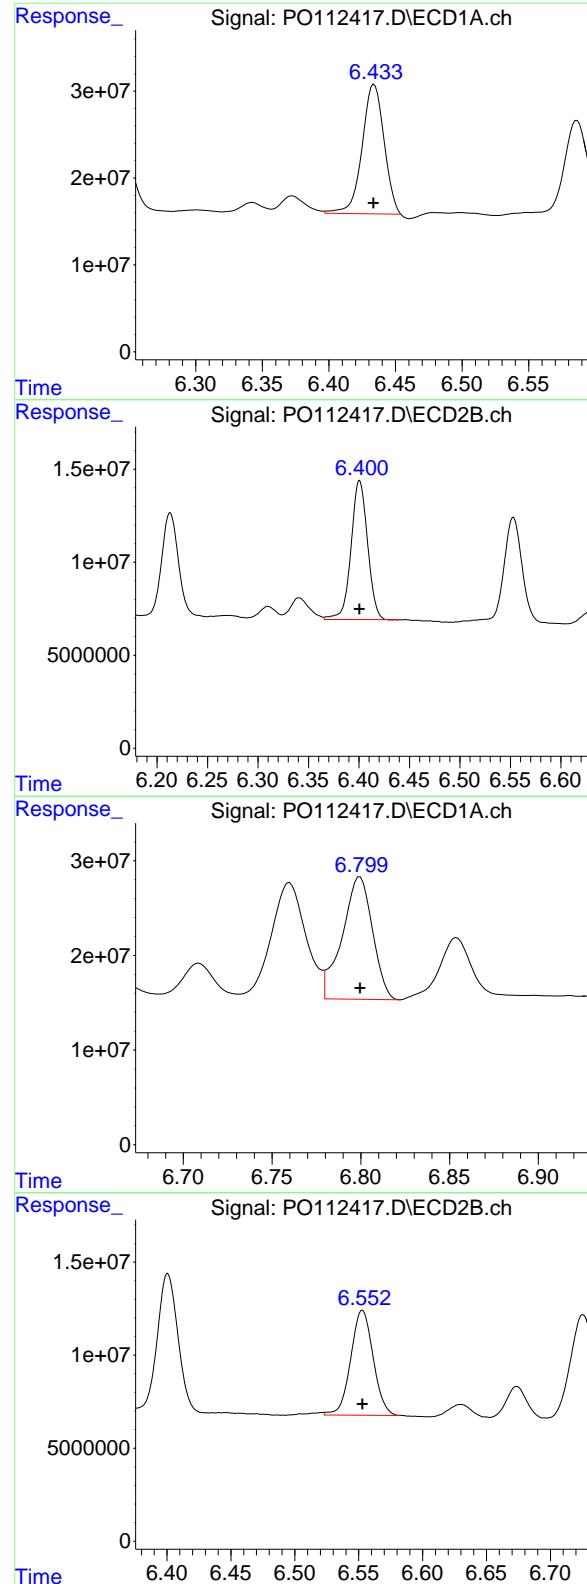

#34 AR-1260-4

R.T.: 7.059 min

Delta R.T.: 0.000 min

Response: 126280400

Conc: 267.73 ng/ml

Instrument:

ECD_O





ClientSampleId :

AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025

Supervised By :mohammad ahmed 07/25/2025

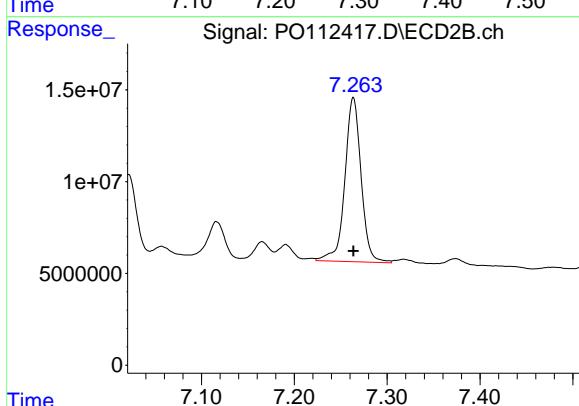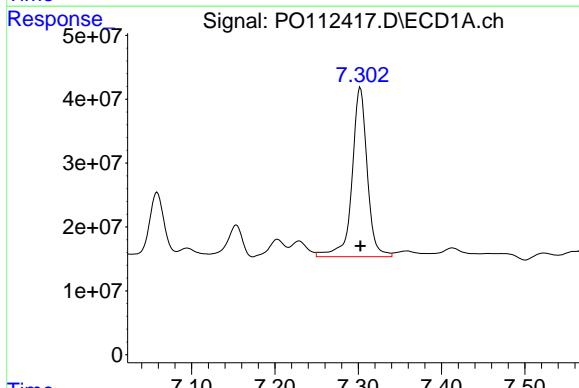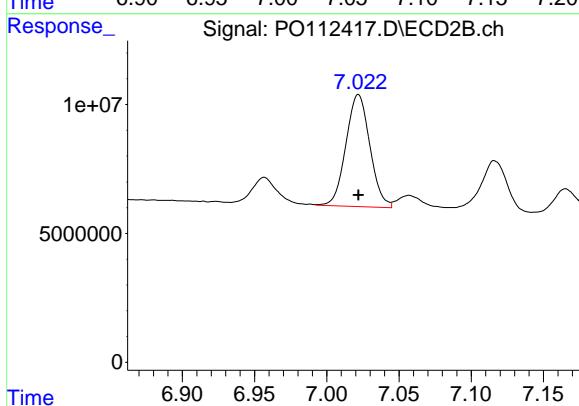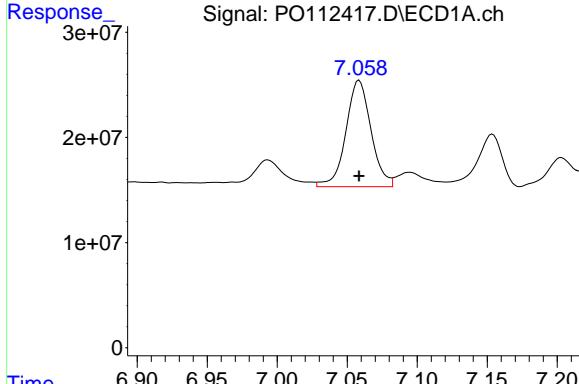

#34 AR-1260-4

R.T.: 7.022 min

Delta R.T.: 0.000 min

Response: 50234042

Conc: 258.47 ng/ml

#35 AR-1260-5

R.T.: 7.302 min

Delta R.T.: 0.000 min

Response: 336866700

Conc: 257.58 ng/ml

#35 AR-1260-5

R.T.: 7.264 min

Delta R.T.: 0.000 min

Response: 108703906

Conc: 254.47 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:45
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:01:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 13:01:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 31417194 | 19597973 | 3.883 | 3.906 |
| 2) SA Decachlor... | 8.693 | 8.640 | 29621580 | 7457220 | 4.051 | 4.220 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 4.756 | 4.737 | 10242412 | 8280603 | 38.166 | 47.316 |
| 4) L1 AR-1016-2 | 4.774 | 4.756 | 16308940 | 11816564 | 40.158 | 45.362 |
| 5) L1 AR-1016-3 | 4.832 | 4.931 | 11721947 | 6127662 | 44.796 | 45.067 |
| 6) L1 AR-1016-4 | 4.951 | 4.973 | 9335010 | 5123227 | 44.066 | 46.120 |
| 7) L1 AR-1016-5 | 5.207 | 5.185 | 8936708 | 6616061 | 41.260m | 46.488m |
| 31) L7 AR-1260-1 | 6.245 | 6.213 | 19551344 | 11452500 | 44.503 | 44.442m |
| 32) L7 AR-1260-2 | 6.434 | 6.402 | 32919190 | 16247800 | 47.855 | 49.311 |
| 33) L7 AR-1260-3 | 6.801 | 6.553 | 23827559 | 11022704 | 40.522 | 43.782m |
| 34) L7 AR-1260-4 | 7.060 | 7.022 | 18415991 | 8957569 | 40.833 | 46.822 |
| 35) L7 AR-1260-5 | 7.303 | 7.265 | 48222745 | 17614159 | 38.916 | 42.733 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:45
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:01:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 13:01:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

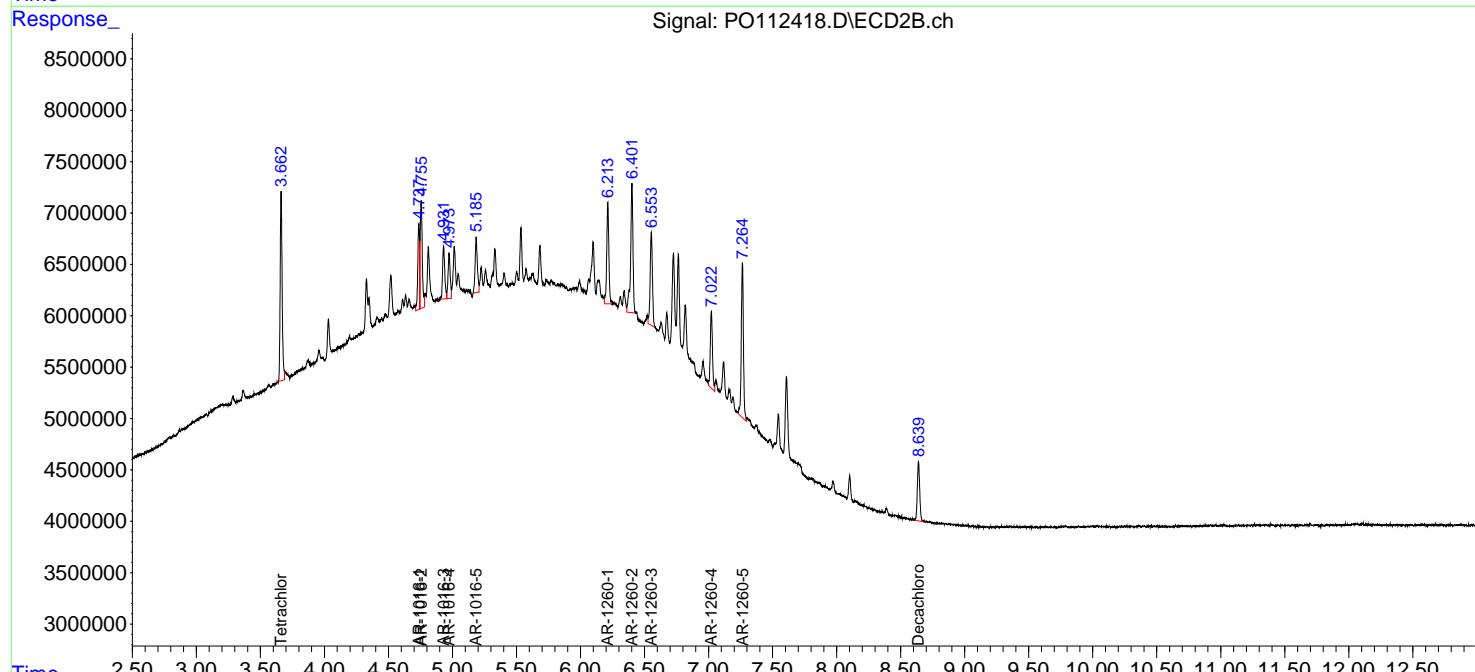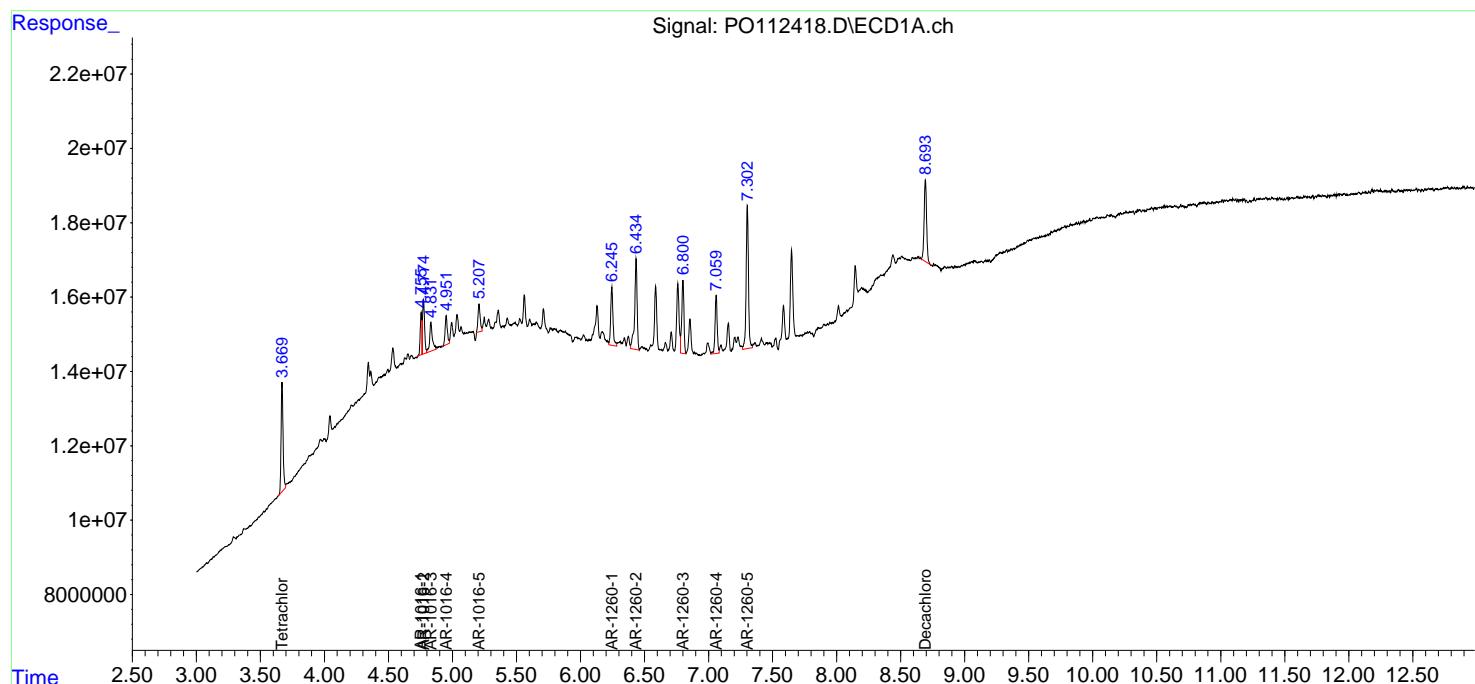

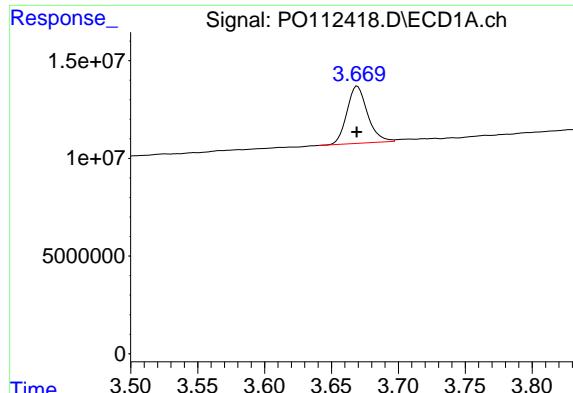


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 31417194
Conc: 3.88 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

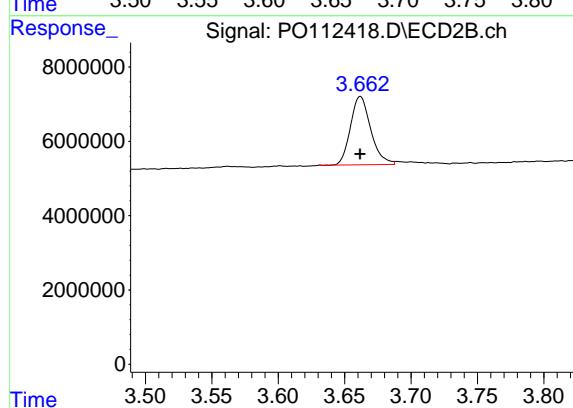


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 19597973
Conc: 3.91 ng/ml

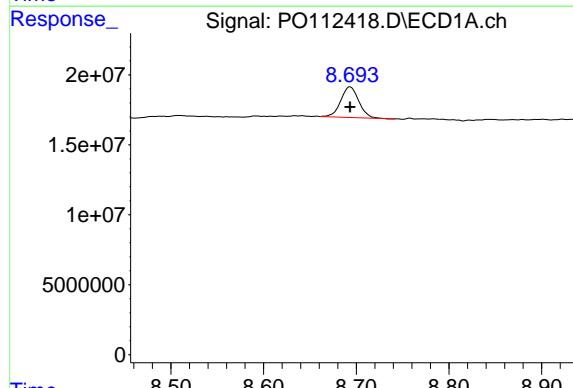





#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 29621580
Conc: 4.05 ng/ml

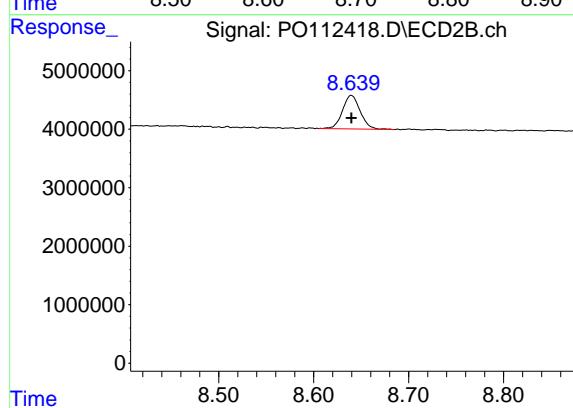

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 7457220
Conc: 4.22 ng/ml

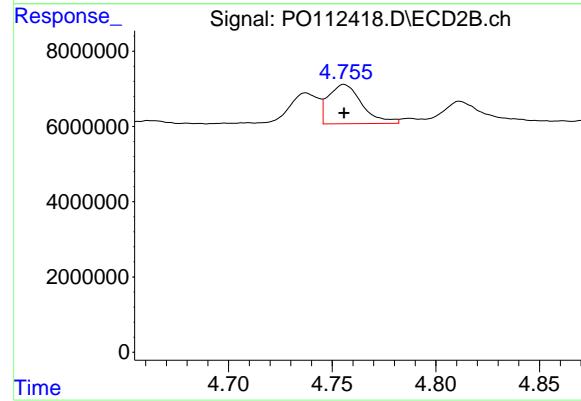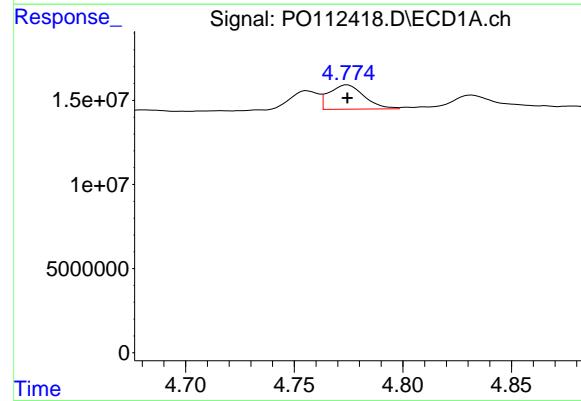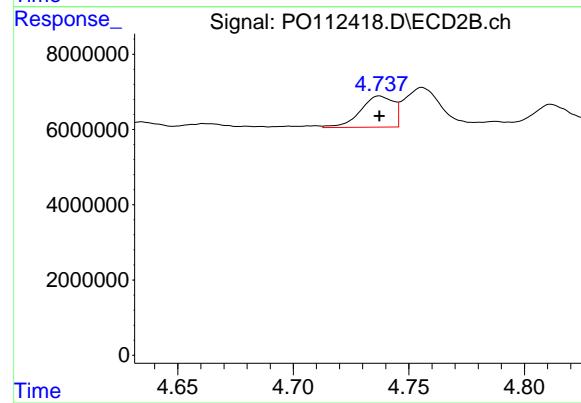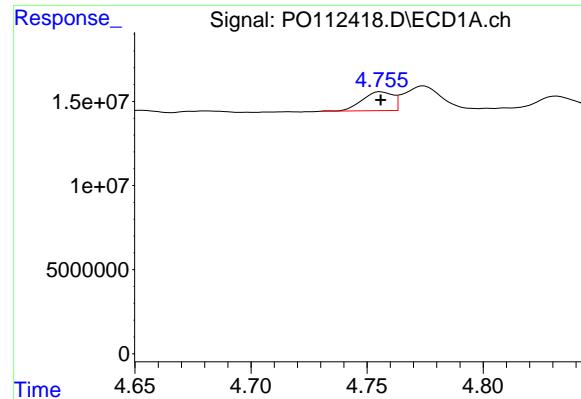




#3 AR-1016-1

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 10242412
Conc: 38.17 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

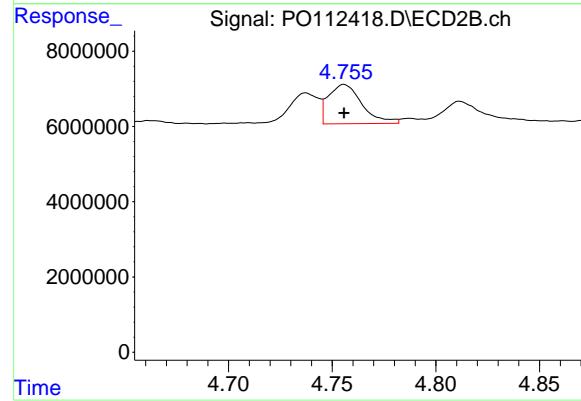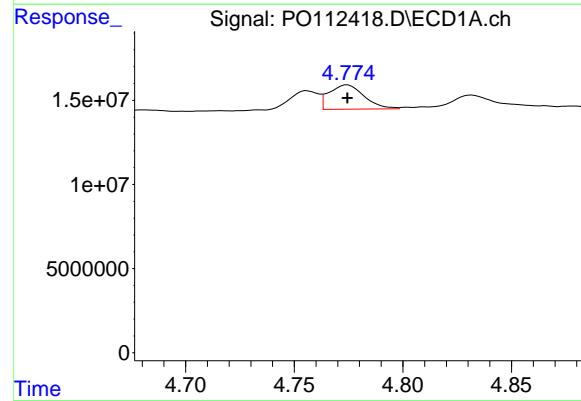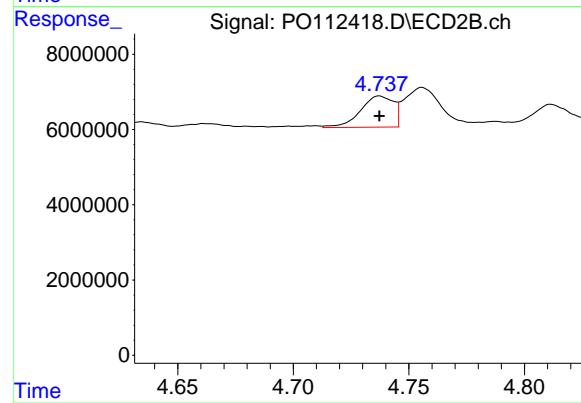

#3 AR-1016-1





R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 8280603
Conc: 47.32 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 16308940
Conc: 40.16 ng/ml

#4 AR-1016-2

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 11816564
Conc: 45.36 ng/ml

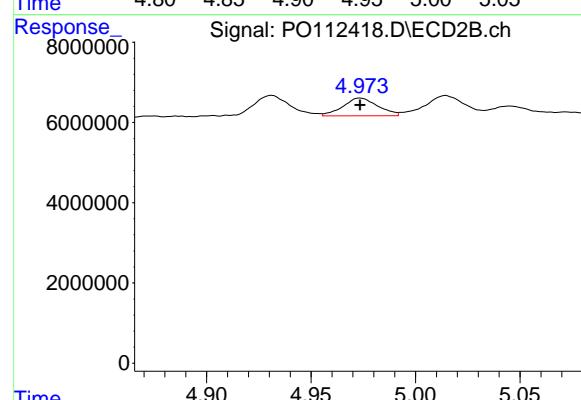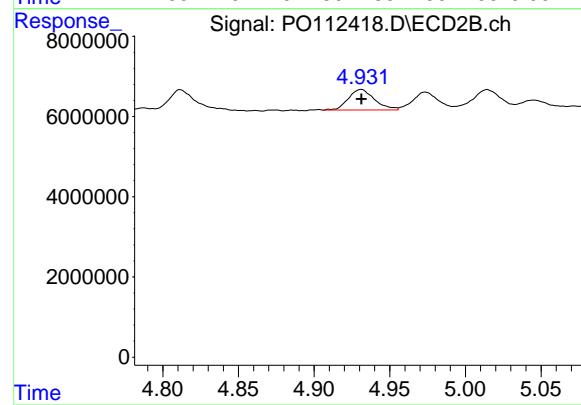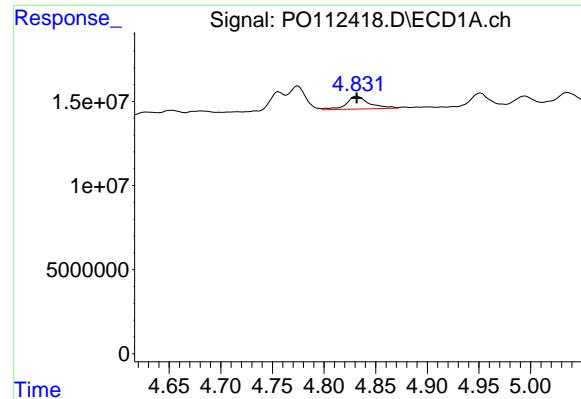




#5 AR-1016-3

R.T.: 4.832 min
Delta R.T.: 0.000 min
Response: 11721947
Conc: 44.80 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

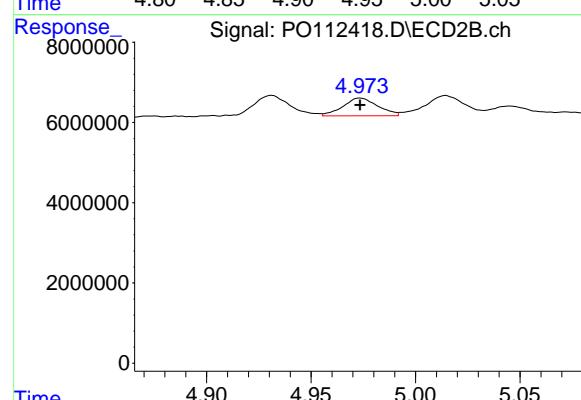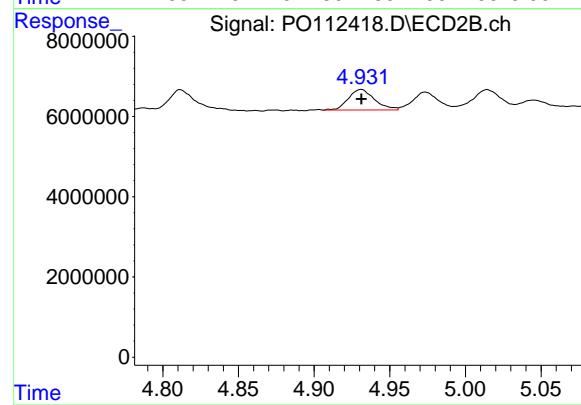

#5 AR-1016-3


R.T.: 4.931 min
Delta R.T.: 0.000 min
Response: 6127662
Conc: 45.07 ng/ml

#6 AR-1016-4

R.T.: 4.951 min
Delta R.T.: 0.000 min
Response: 9335010
Conc: 44.07 ng/ml

#6 AR-1016-4

R.T.: 4.973 min
Delta R.T.: 0.000 min
Response: 5123227
Conc: 46.12 ng/ml

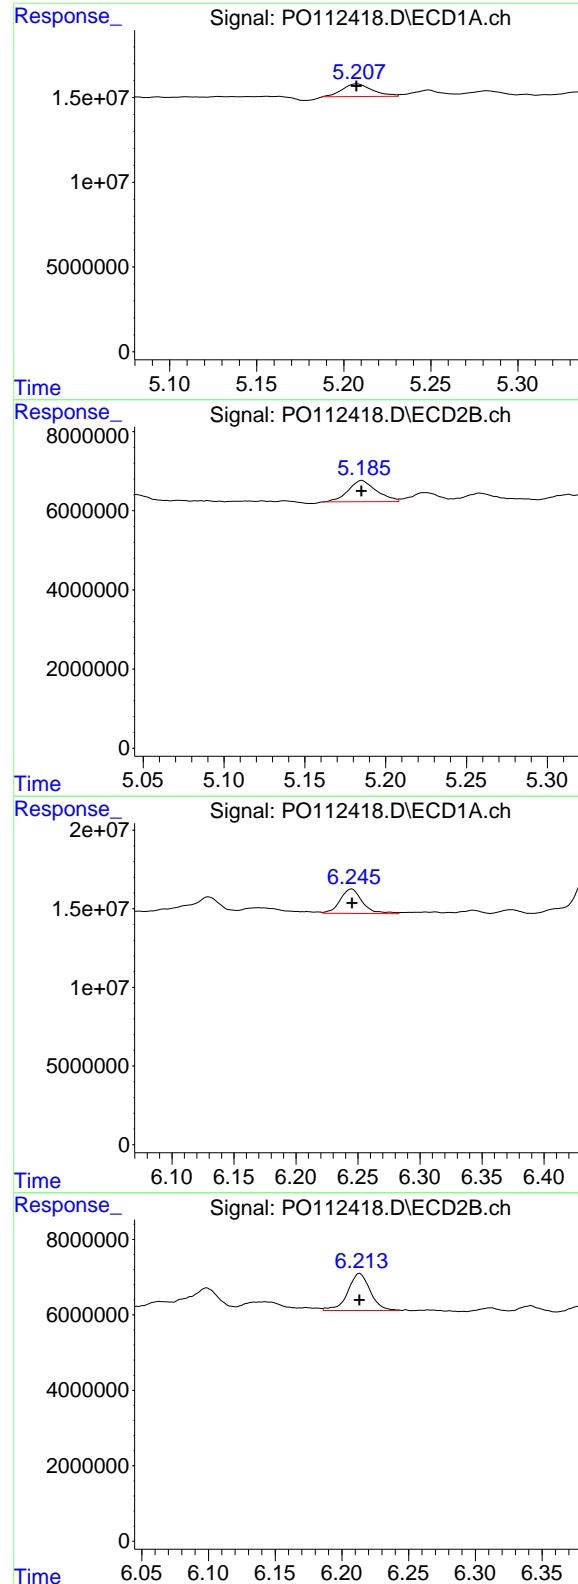

#7 AR-1016-5

R.T.: 5.207 min
 Delta R.T.: 0.000 min
 Response: 8936708
 Conc: 41.26 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#7 AR-1016-5


R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 6616061
 Conc: 46.49 ng/ml

#31 AR-1260-1

R.T.: 6.245 min
 Delta R.T.: 0.000 min
 Response: 19551344
 Conc: 44.50 ng/ml

#31 AR-1260-1

R.T.: 6.213 min
 Delta R.T.: 0.000 min
 Response: 11452500
 Conc: 44.44 ng/ml

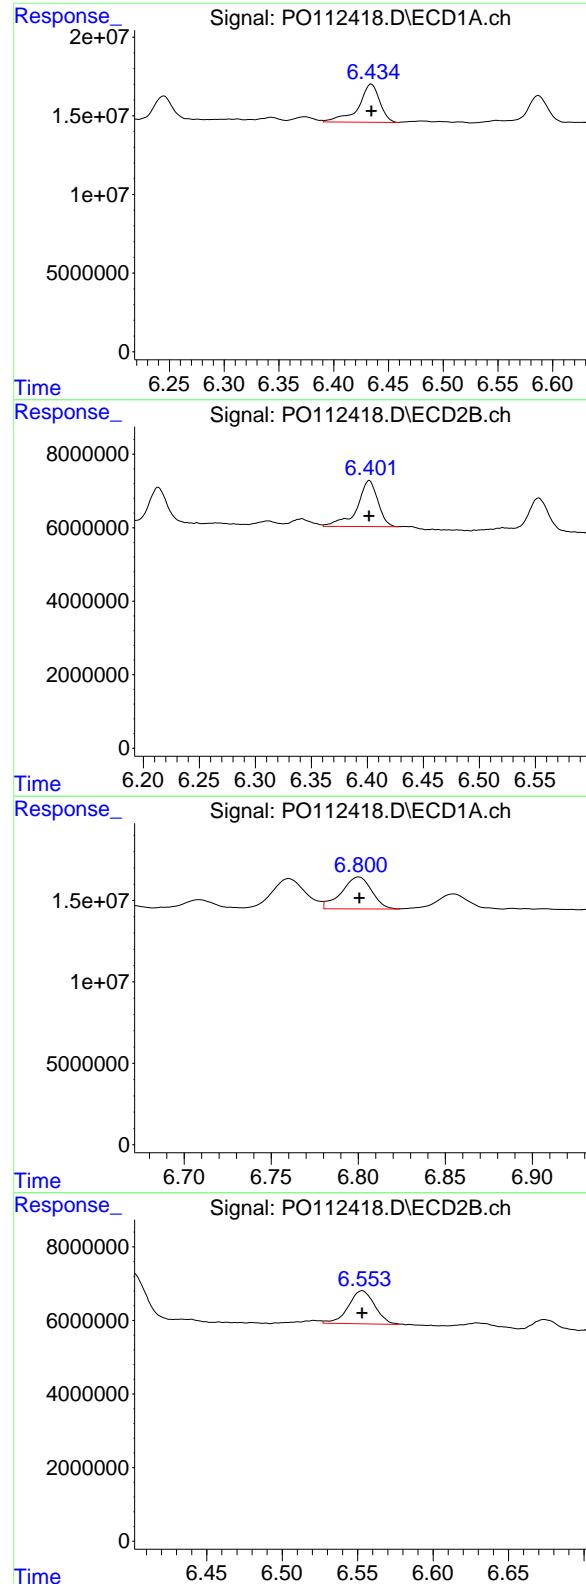

#32 AR-1260-2

R.T.: 6.434 min
 Delta R.T.: 0.000 min
 Response: 32919190
 Conc: 47.86 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#32 AR-1260-2

R.T.: 6.402 min
 Delta R.T.: 0.000 min
 Response: 16247800
 Conc: 49.31 ng/ml

#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: 0.000 min
 Response: 23827559
 Conc: 40.52 ng/ml

#33 AR-1260-3

R.T.: 6.553 min
 Delta R.T.: 0.000 min
 Response: 11022704
 Conc: 43.78 ng/ml





#34 AR-1260-4

R.T.: 7.060 min
 Delta R.T.: 0.000 min
 Response: 18415991
 Conc: 40.83 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

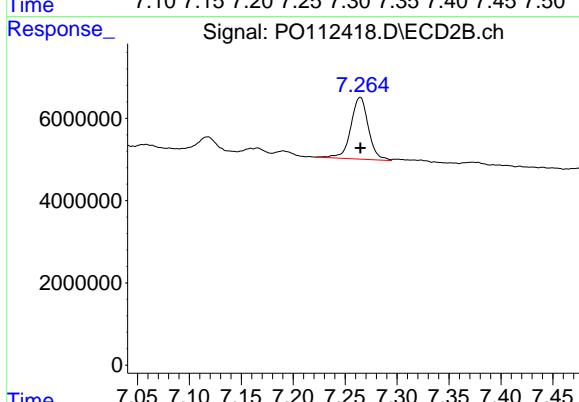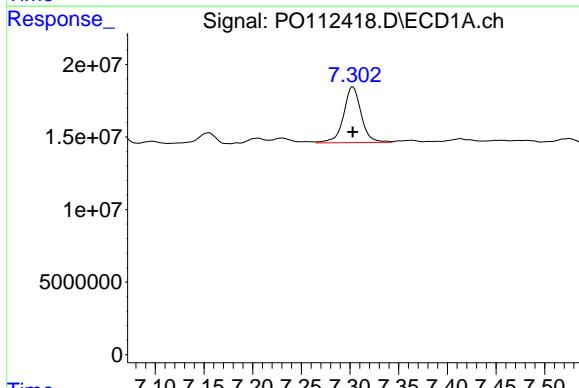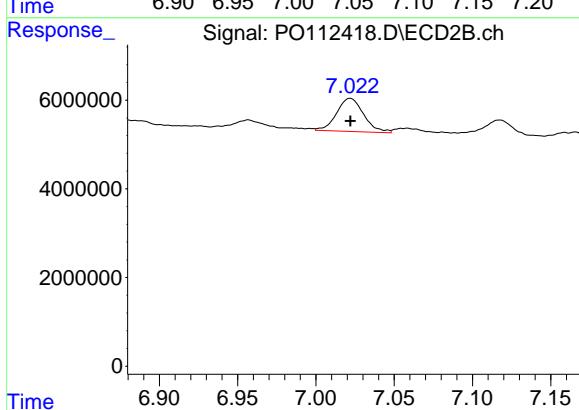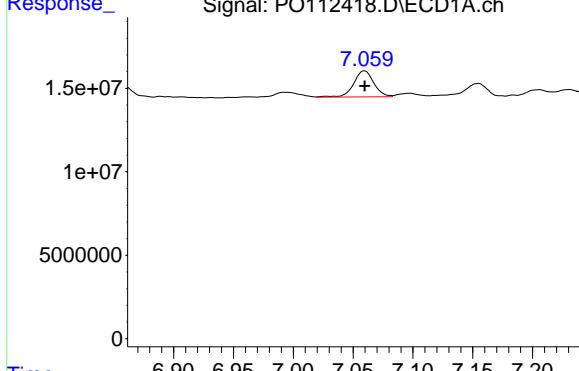

#34 AR-1260-4

R.T.: 7.022 min
 Delta R.T.: 0.000 min
 Response: 8957569
 Conc: 46.82 ng/ml

#35 AR-1260-5

R.T.: 7.303 min
 Delta R.T.: 0.000 min
 Response: 48222745
 Conc: 38.92 ng/ml

#35 AR-1260-5

R.T.: 7.265 min
 Delta R.T.: 0.000 min
 Response: 17614159
 Conc: 42.73 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:03
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:39:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 13:39:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 423.2E6 | 251.3E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.694 | 8.641 | 374.2E6 | 89450396 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 8) L2 AR-1221-1 | 3.882 | 3.872 | 48329823 | 33632938 | 500.000 | 500.000 |
| 9) L2 AR-1221-2 | 3.967 | 3.958 | 35930990 | 25363994 | 500.000 | 500.000 |
| 10) L2 AR-1221-3 | 4.044 | 4.032 | 118.9E6 | 79264688 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:03
 Operator : YP/AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:39:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 13:39:21 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

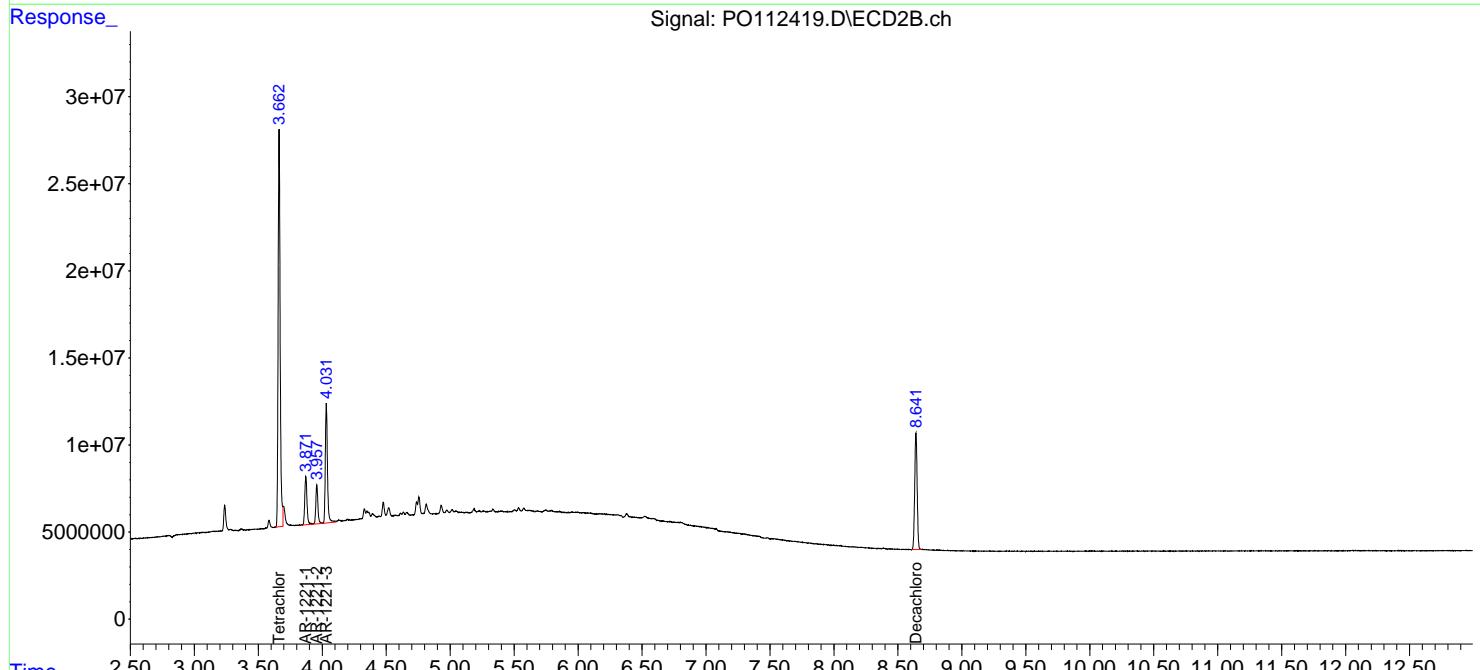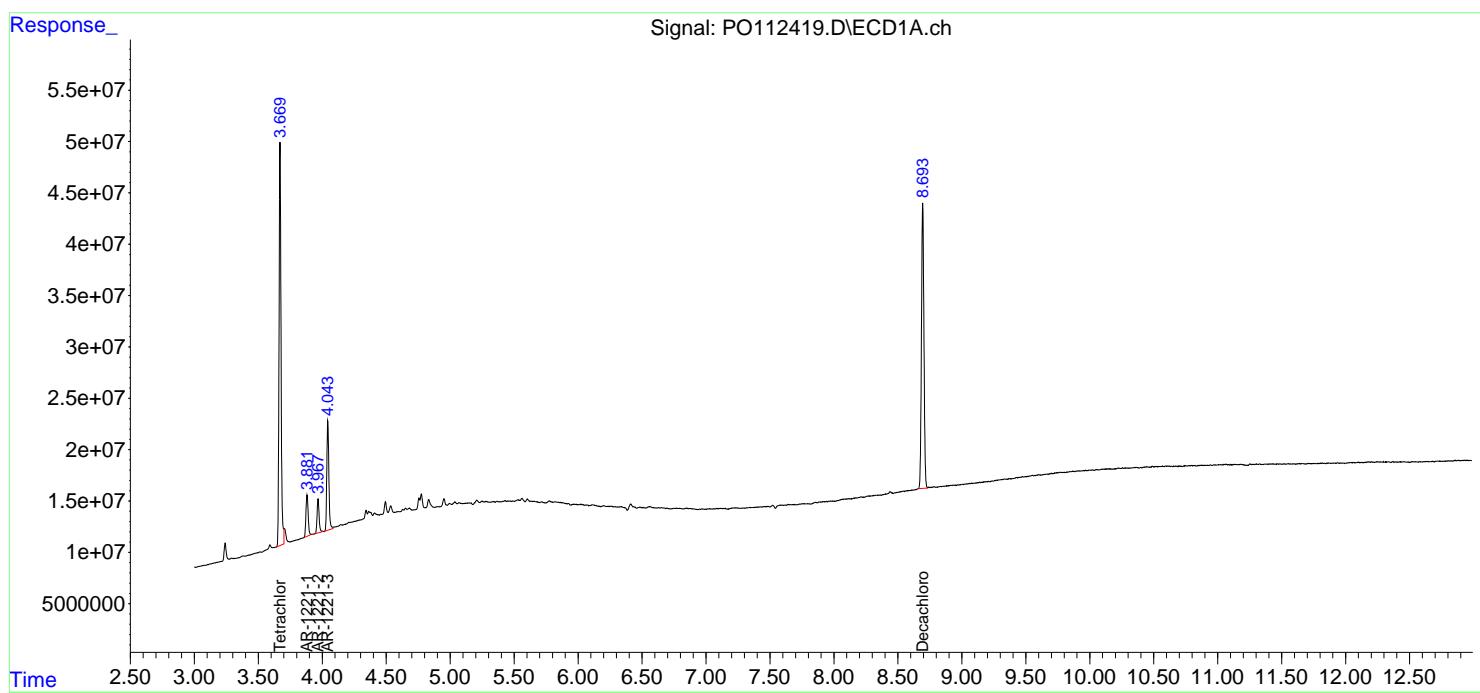

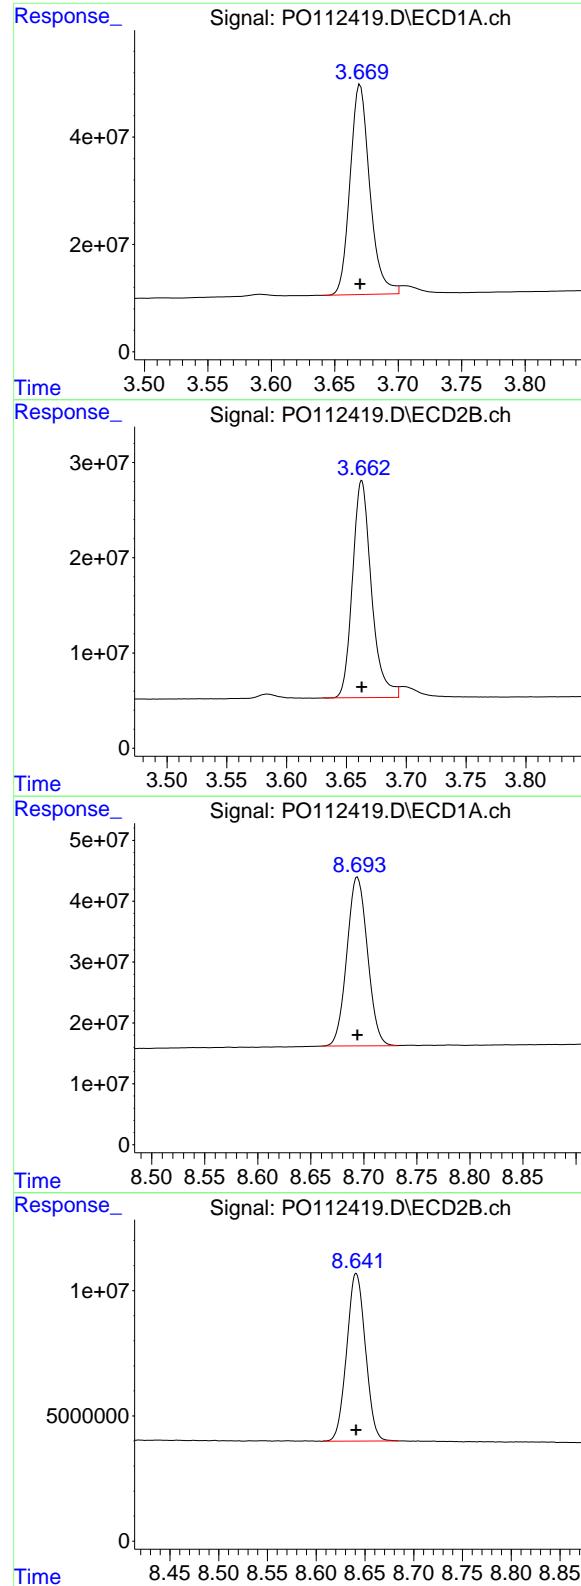

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: 0.000 min
 Response: 423227865
 Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1221ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
 Delta R.T.: 0.000 min
 Response: 251317595
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
 Delta R.T.: 0.000 min
 Response: 374163837
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
 Delta R.T.: 0.000 min
 Response: 89450396
 Conc: 50.00 ng/ml

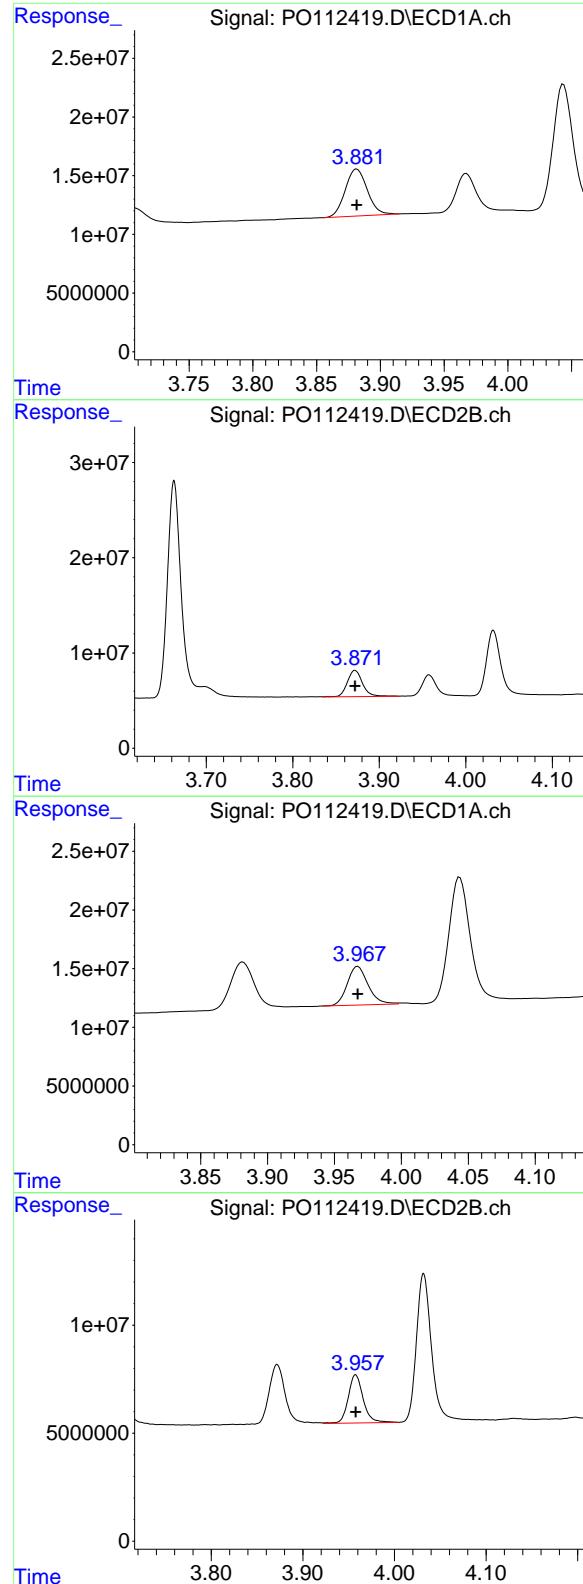

#8 AR-1221-1

R.T.: 3.882 min
 Delta R.T.: 0.000 min
 Response: 48329823
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1221ICC500

#8 AR-1221-1

R.T.: 3.872 min
 Delta R.T.: 0.000 min
 Response: 33632938
 Conc: 500.00 ng/ml


#9 AR-1221-2

R.T.: 3.967 min
 Delta R.T.: 0.000 min
 Response: 35930990
 Conc: 500.00 ng/ml

#9 AR-1221-2

R.T.: 3.958 min
 Delta R.T.: 0.000 min
 Response: 25363994
 Conc: 500.00 ng/ml

#10 AR-1221-3

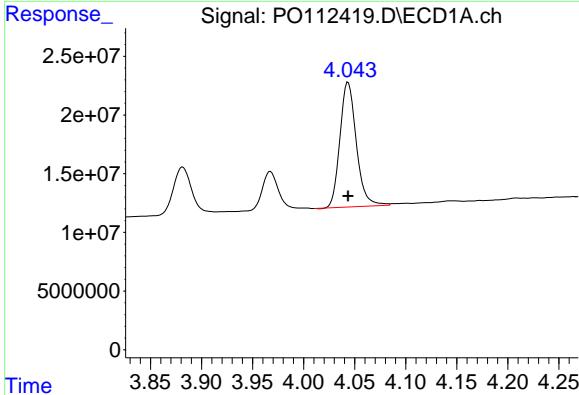


R.T.: 4.044 min
Delta R.T.: 0.000 min
Response: 118855573
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1221ICC500

#10 AR-1221-3

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 79264688
Conc: 500.00 ng/ml

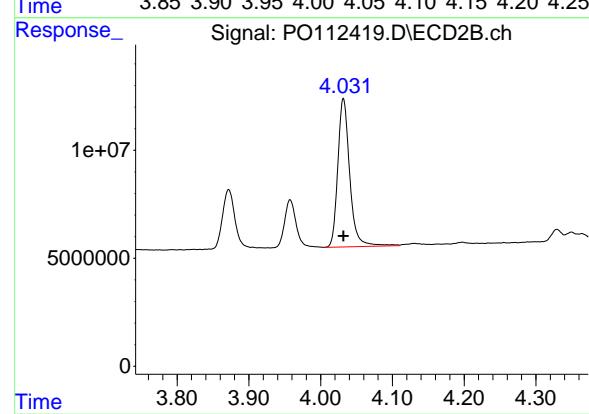

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:22
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:21:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:21:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 456.9E6 | 277.1E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.694 | 8.641 | 397.2E6 | 95040741 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 11) L3 AR-1232-1 | 4.043 | 4.031 | 93489328 | 63274969 | 500.000 | 500.000 |
| 12) L3 AR-1232-2 | 4.535 | 4.756 | 53812362 | 65577392 | 500.000 | 500.000 |
| 13) L3 AR-1232-3 | 4.775 | 4.931 | 103.4E6 | 33598402 | 500.000 | 500.000 |
| 14) L3 AR-1232-4 | 4.951 | 5.015 | 52370149 | 29914546 | 500.000 | 500.000 |
| 15) L3 AR-1232-5 | 4.994 | 5.185 | 33940444 | 32601518 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:22
 Operator : YP/AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:21:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:21:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

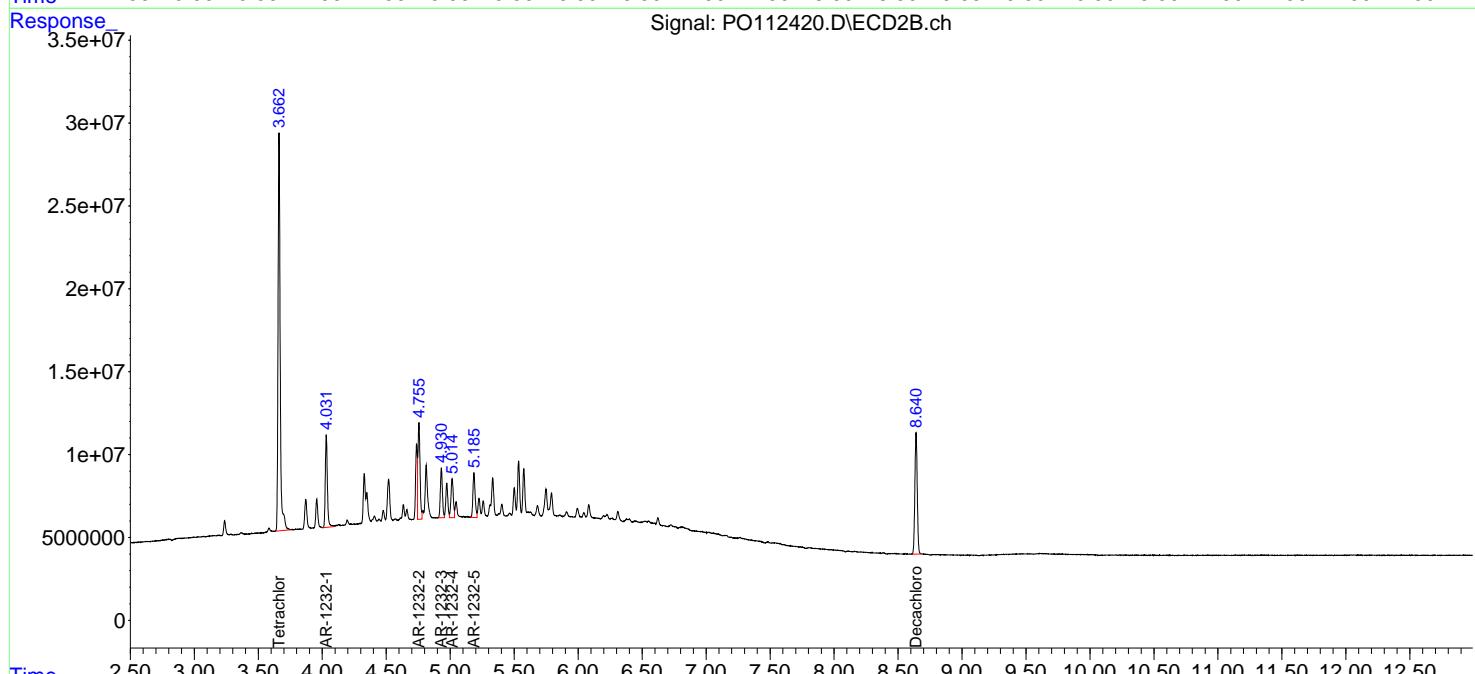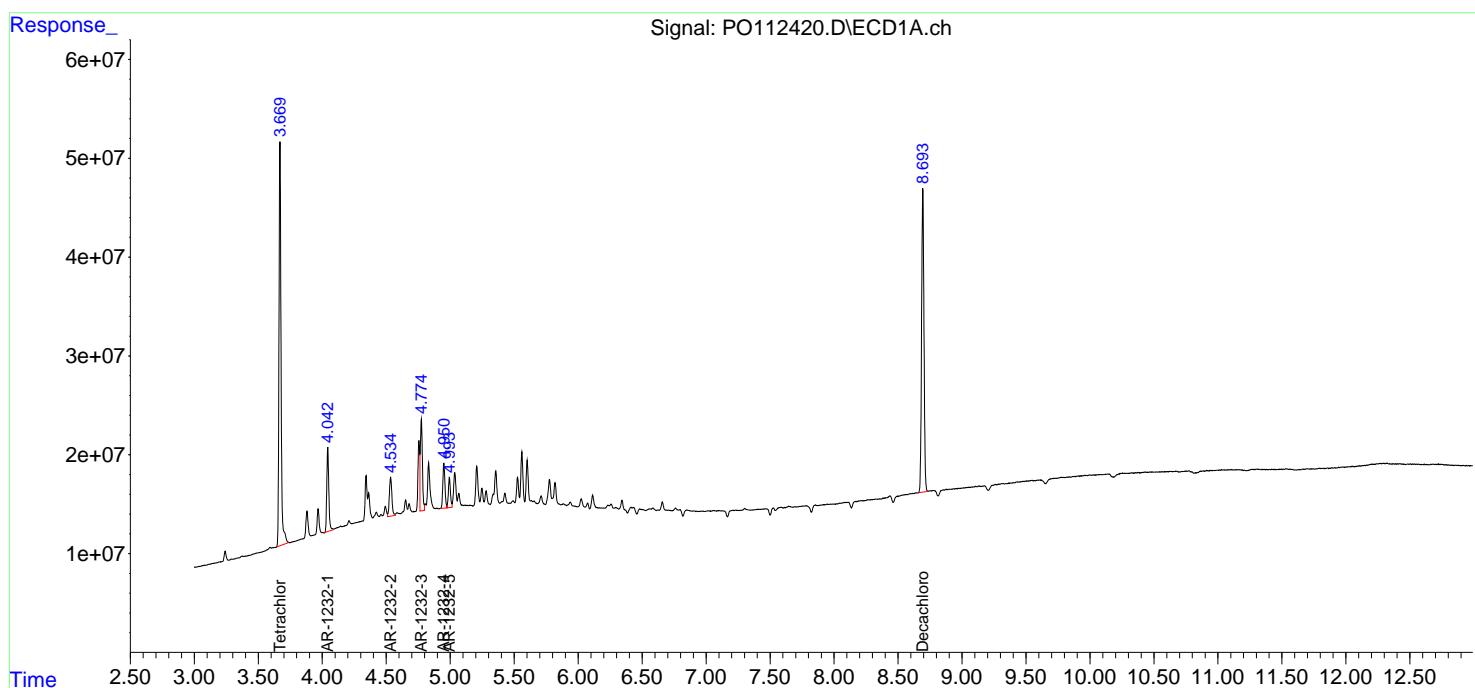


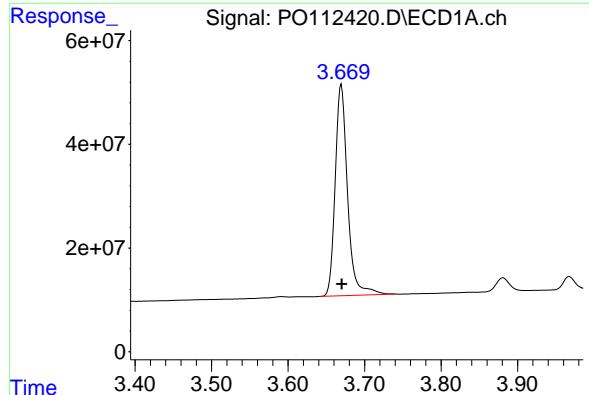

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 456891808
Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500

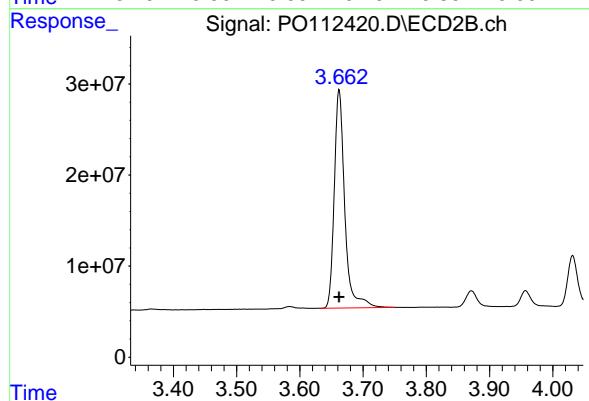


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 277117760
Conc: 50.00 ng/ml

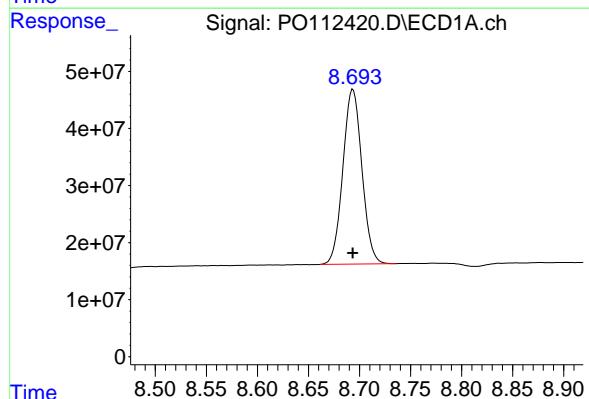


#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 397152757
Conc: 50.00 ng/ml

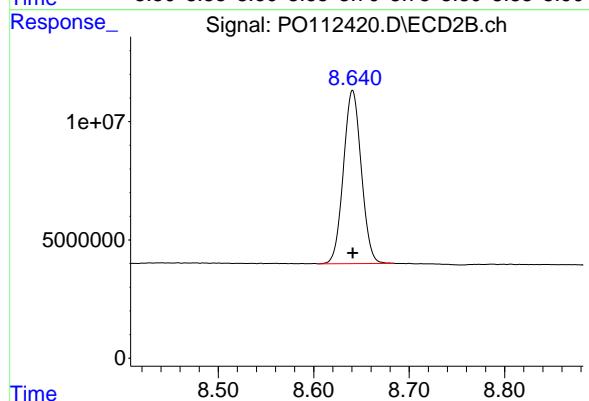

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 95040741
Conc: 50.00 ng/ml

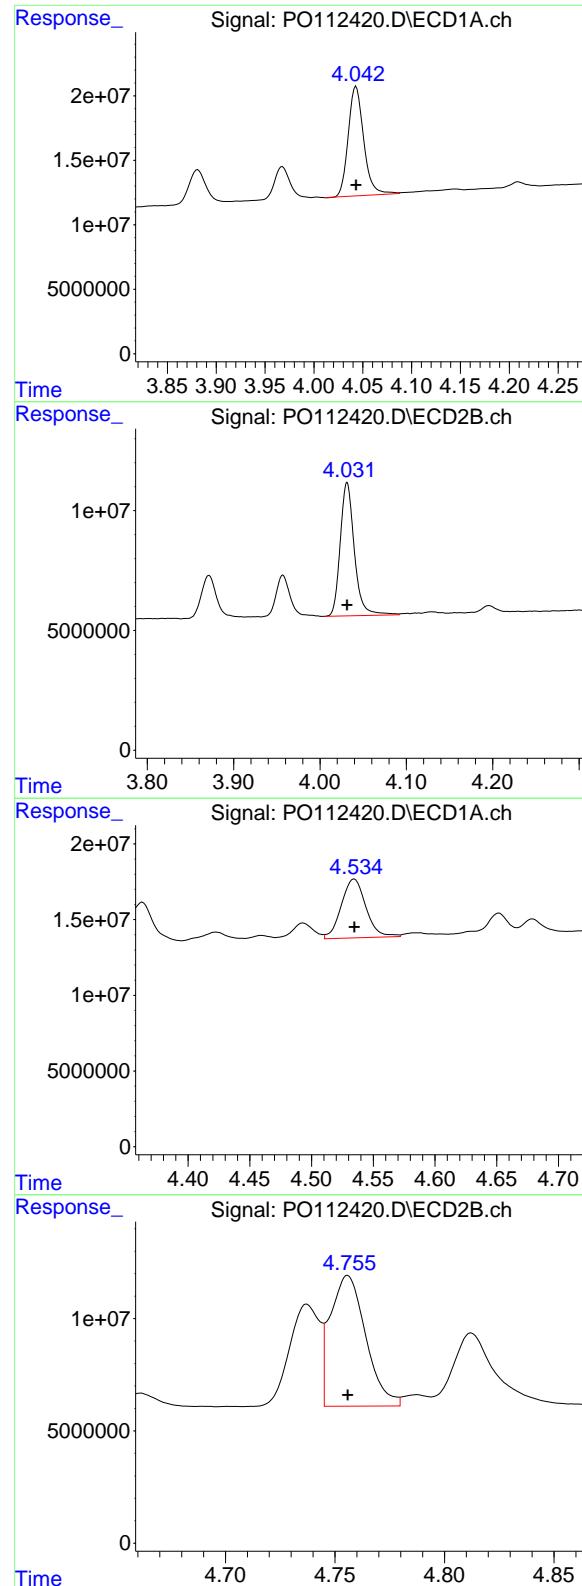

#11 AR-1232-1

R.T.: 4.043 min
 Delta R.T.: 0.000 min
 Response: 93489328
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500

#11 AR-1232-1

R.T.: 4.031 min
 Delta R.T.: 0.000 min
 Response: 63274969
 Conc: 500.00 ng/ml

#12 AR-1232-2

R.T.: 4.535 min
 Delta R.T.: 0.000 min
 Response: 53812362
 Conc: 500.00 ng/ml


#12 AR-1232-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 65577392
 Conc: 500.00 ng/ml

#13 AR-1232-3


R.T.: 4.775 min
 Delta R.T.: 0.000 min
 Response: 103399628
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500

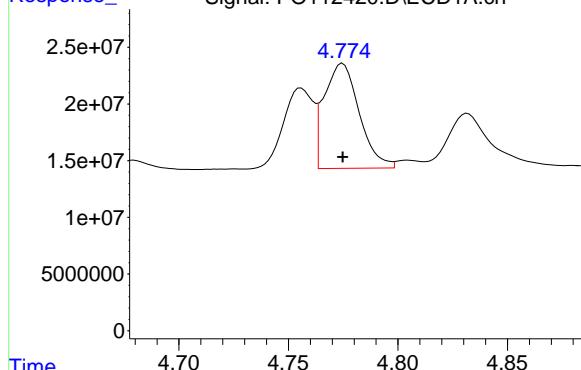


#13 AR-1232-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 33598402
 Conc: 500.00 ng/ml

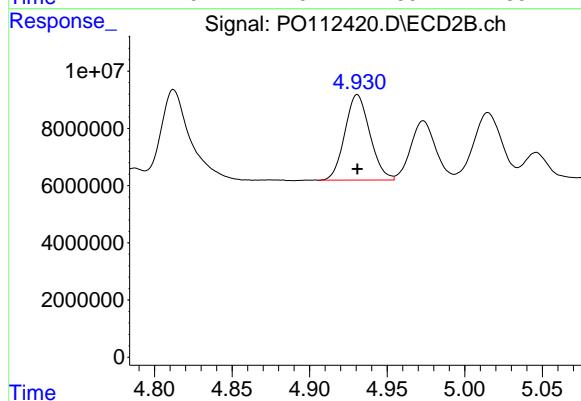


#14 AR-1232-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 52370149
 Conc: 500.00 ng/ml



#14 AR-1232-4



R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 29914546
 Conc: 500.00 ng/ml

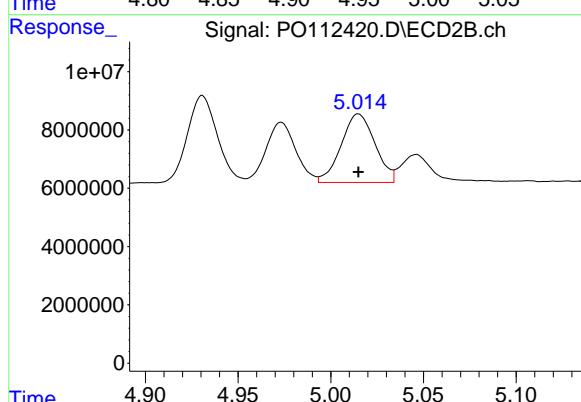

#15 AR-1232-5

R.T.: 4.994 min
Delta R.T.: 0.000 min
Response: 33940444
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1232ICC500

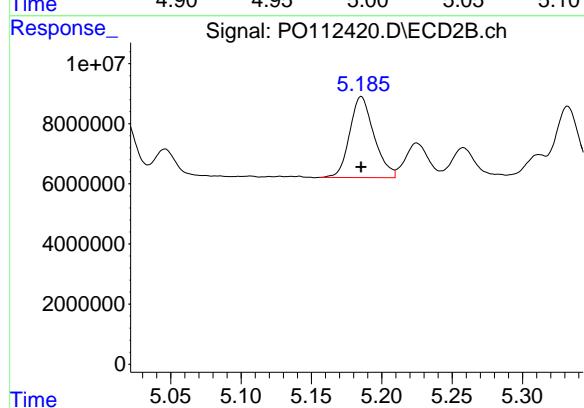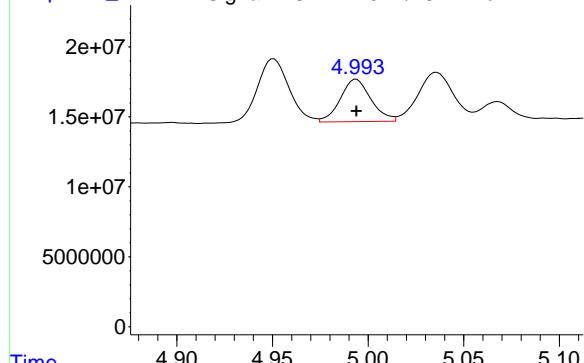

#15 AR-1232-5

R.T.: 5.185 min
Delta R.T.: 0.000 min
Response: 32601518
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:40
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:43:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:40:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 912.6E6 | 548.3E6 | 99.488 | 99.183 |
| 2) SA Decachlor... | 8.694 | 8.641 | 800.1E6 | 183.2E6 | 99.457 | 97.537 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|---------|---------|---------|
| 16) L4 AR-1242-1 | 4.755 | 4.738 | 256.3E6 | 153.6E6 | 991.564 | 972.911 |
| 17) L4 AR-1242-2 | 4.775 | 4.756 | 381.1E6 | 230.6E6 | 986.515 | 976.155 |
| 18) L4 AR-1242-3 | 4.832 | 4.931 | 241.8E6 | 121.0E6 | 986.644 | 977.243 |
| 19) L4 AR-1242-4 | 4.951 | 5.015 | 195.7E6 | 116.9E6 | 985.280 | 969.692 |
| 20) L4 AR-1242-5 | 5.602 | 5.534 | 215.7E6 | 154.5E6 | 969.592 | 960.715 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:40
 Operator : YP/AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:43:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:40:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

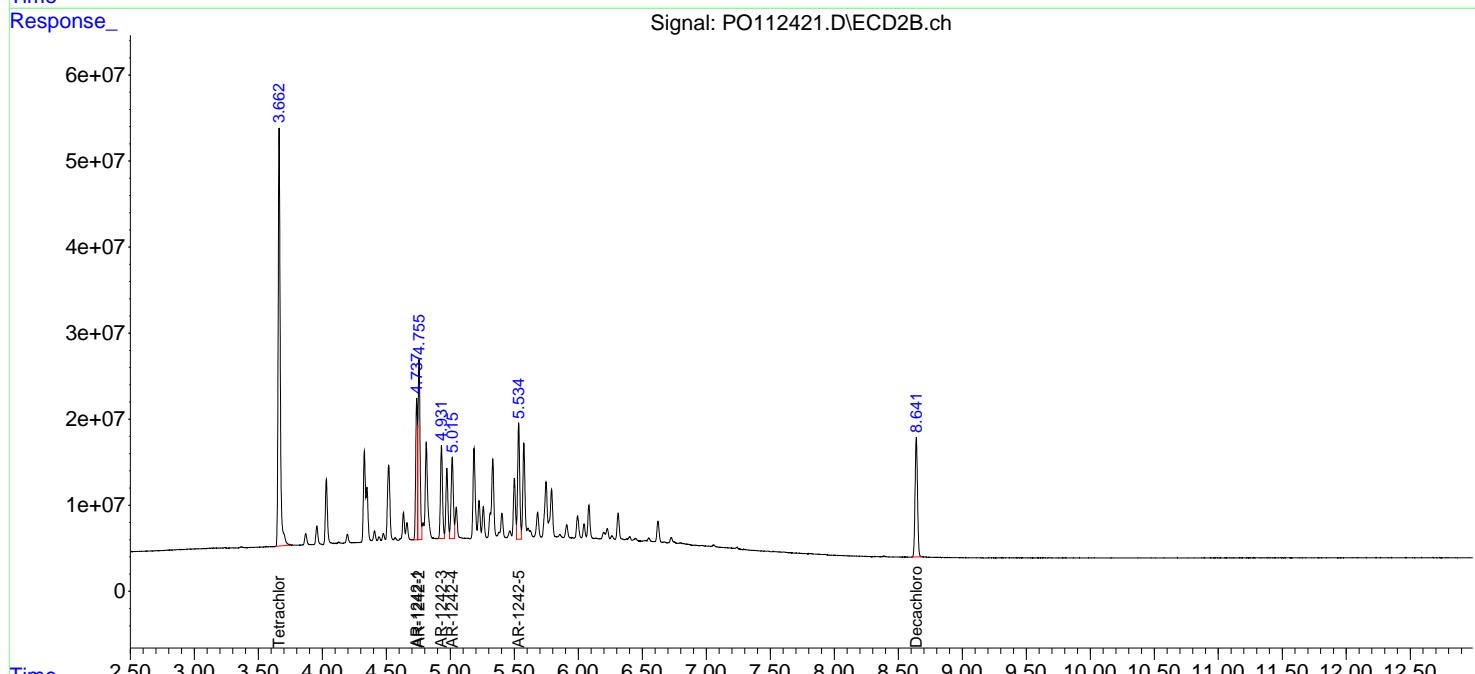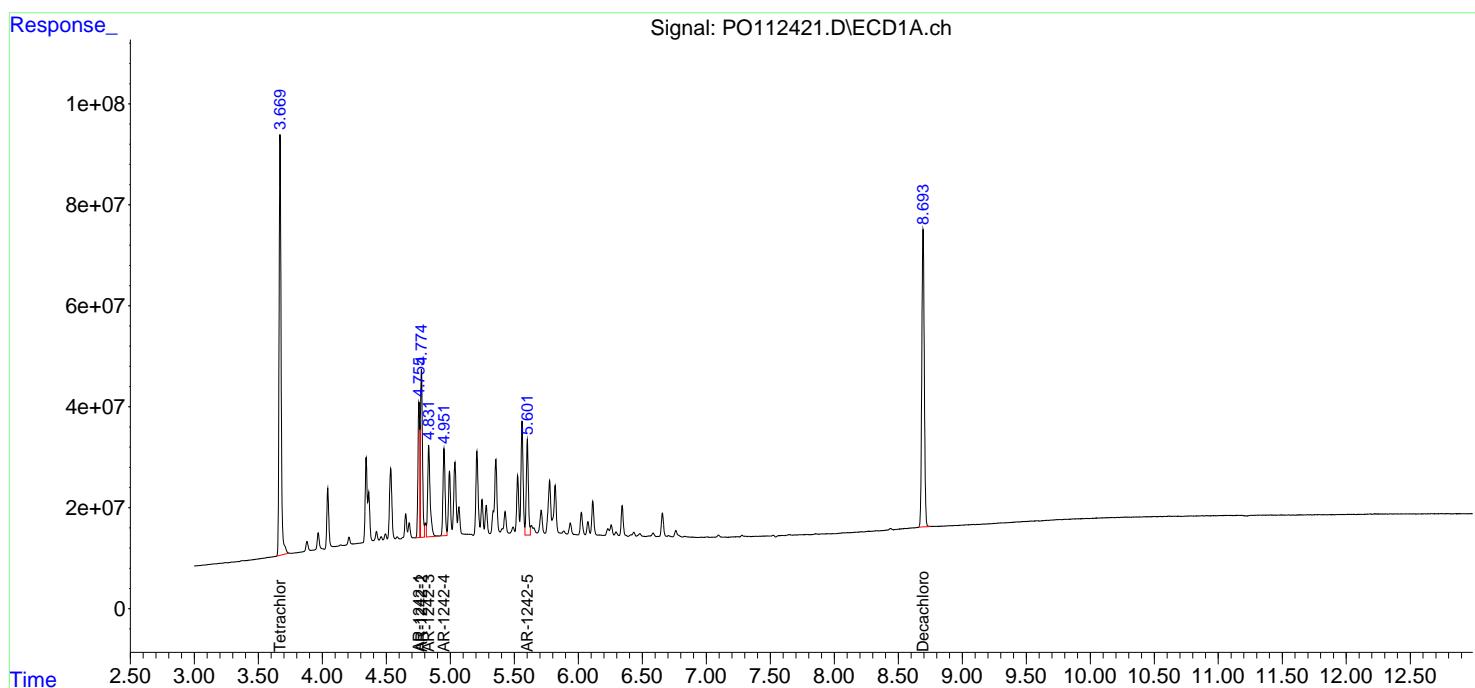

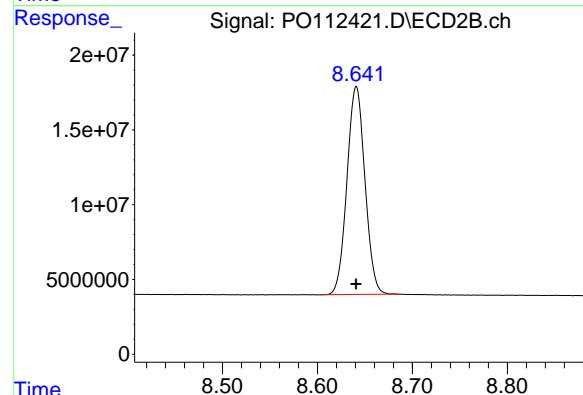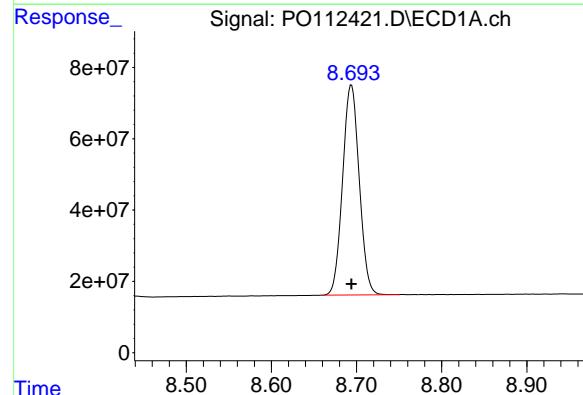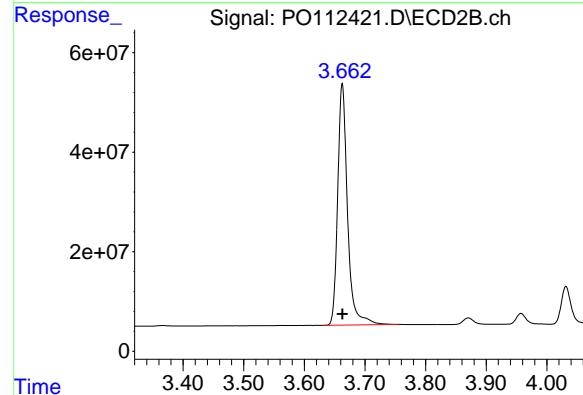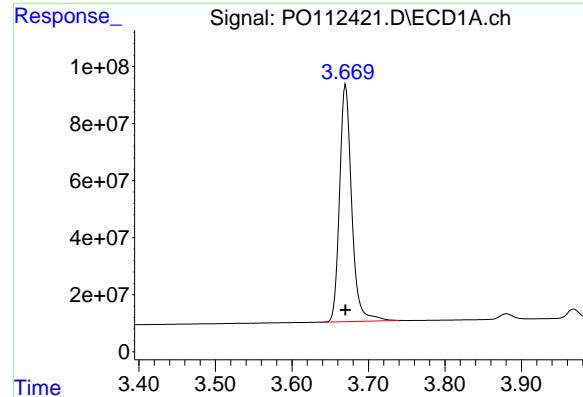

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 912565223
Conc: 99.49 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 548323877
Conc: 99.18 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 800064533
Conc: 99.46 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 183160404
Conc: 97.54 ng/ml

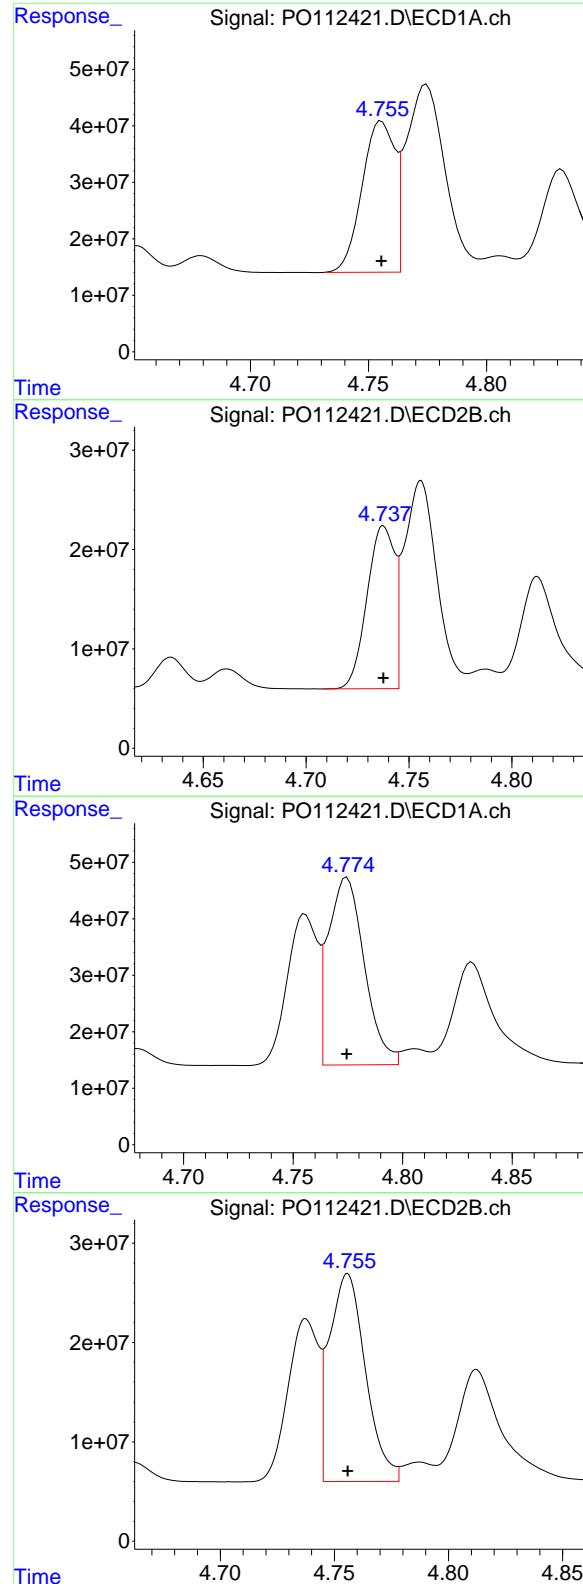

#16 AR-1242-1

R.T.: 4.755 min
 Delta R.T.: 0.000 min
 Response: 256299409
 Conc: 991.56 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC1000

#16 AR-1242-1


R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 153645977
 Conc: 972.91 ng/ml

#17 AR-1242-2

R.T.: 4.775 min
 Delta R.T.: 0.000 min
 Response: 381137122
 Conc: 986.52 ng/ml

#17 AR-1242-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 230553136
 Conc: 976.16 ng/ml

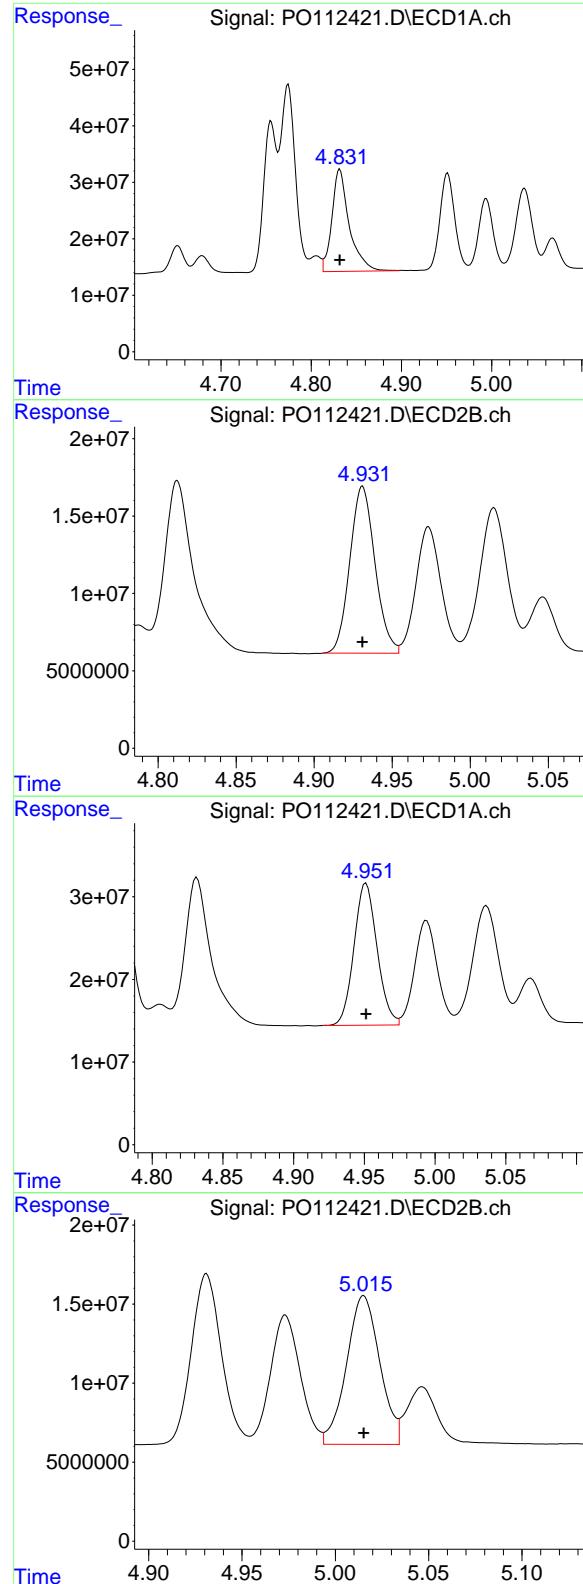

#18 AR-1242-3

R.T.: 4.832 min
 Delta R.T.: 0.000 min
 Response: 241769617
 Conc: 986.64 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC1000

#18 AR-1242-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 120997871
 Conc: 977.24 ng/ml

#19 AR-1242-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 195717021
 Conc: 985.28 ng/ml



#19 AR-1242-4

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 116921071
 Conc: 969.69 ng/ml

#20 AR-1242-5

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 215656431
Conc: 969.59 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC1000

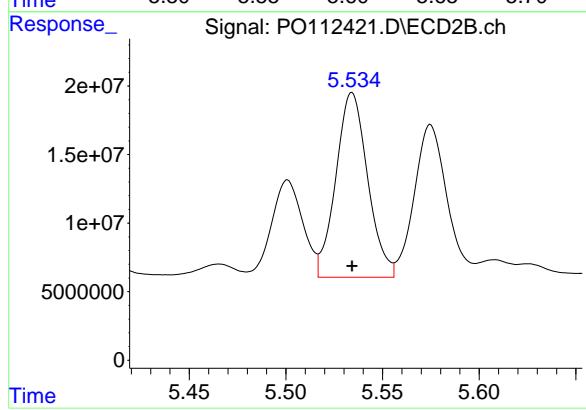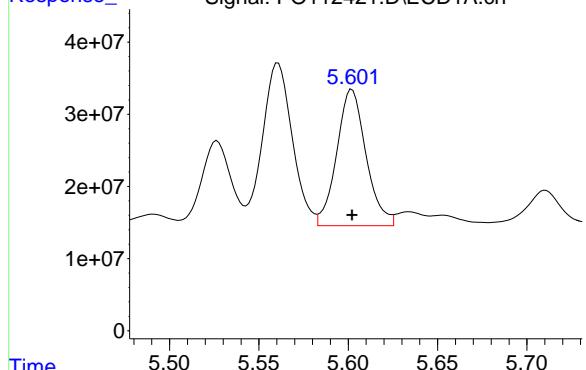

#20 AR-1242-5

R.T.: 5.534 min
Delta R.T.: 0.000 min
Response: 154482444
Conc: 960.72 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:59
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:46:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:40:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 689.6E6 | 415.8E6 | 75.123 | 75.136 |
| 2) SA Decachlor... | 8.694 | 8.641 | 602.8E6 | 140.4E6 | 74.961 | 74.840 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 16) L4 AR-1242-1 | 4.756 | 4.738 | 194.7E6 | 118.7E6 | 752.104 | 751.134 |
| 17) L4 AR-1242-2 | 4.774 | 4.756 | 290.3E6 | 177.2E6 | 750.959 | 750.102 |
| 18) L4 AR-1242-3 | 4.831 | 4.931 | 184.9E6 | 93444753 | 752.920 | 753.133 |
| 19) L4 AR-1242-4 | 4.951 | 5.015 | 148.8E6 | 90566785 | 749.303 | 750.747 |
| 20) L4 AR-1242-5 | 5.602 | 5.534 | 165.1E6 | 120.7E6 | 744.936 | 750.335 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 13:59
 Operator : YP/AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:46:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:40:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

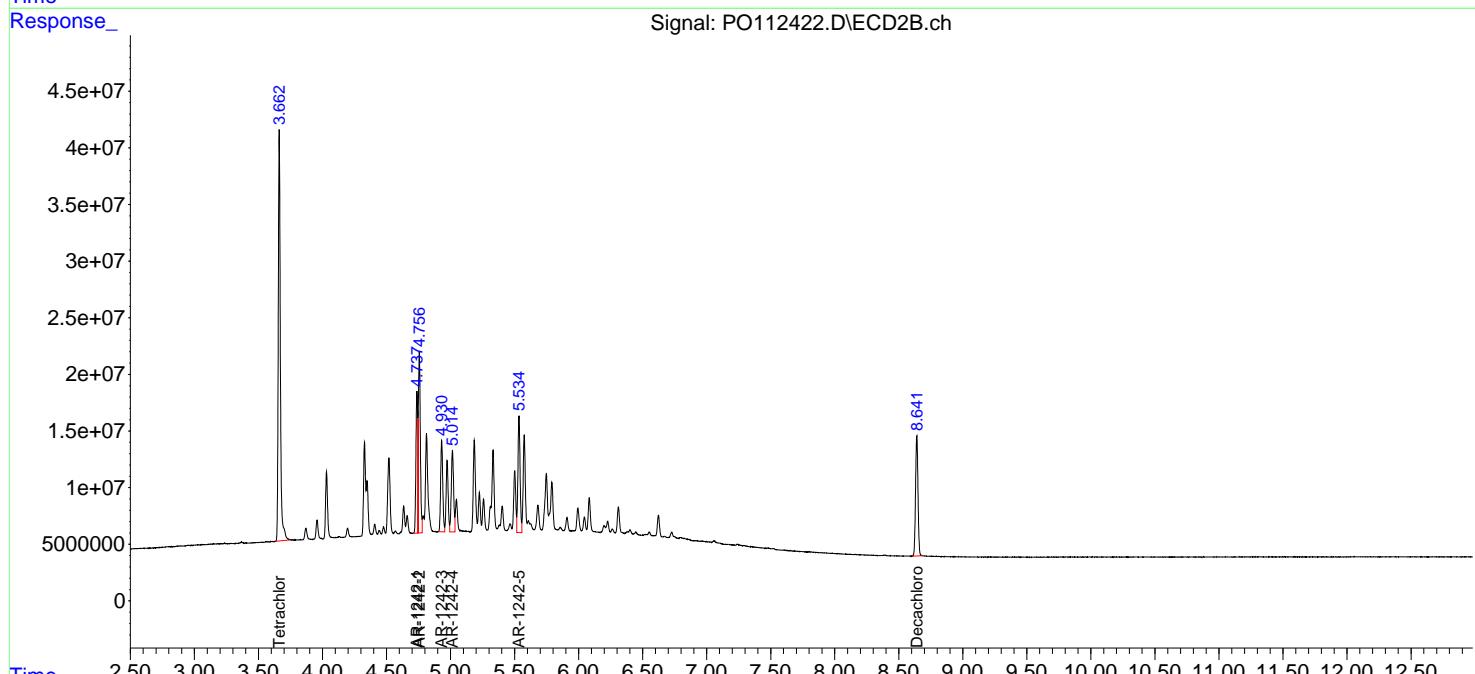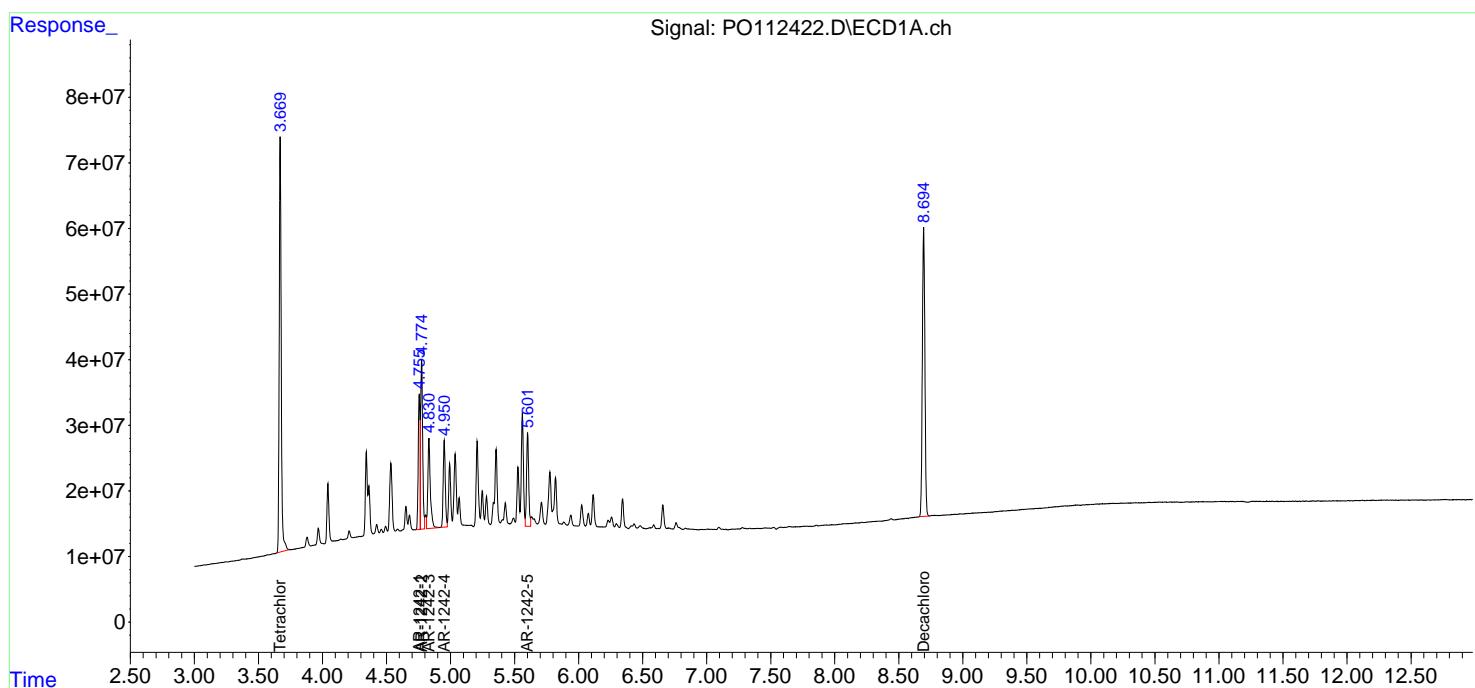

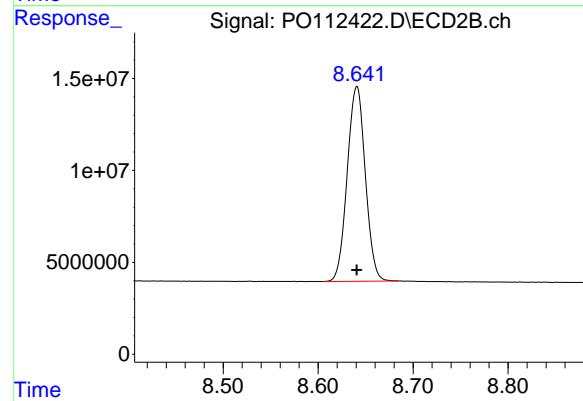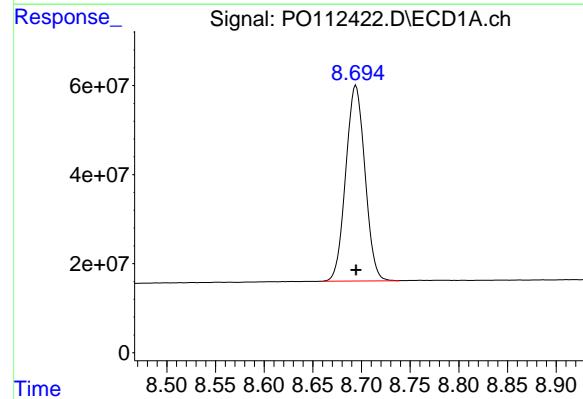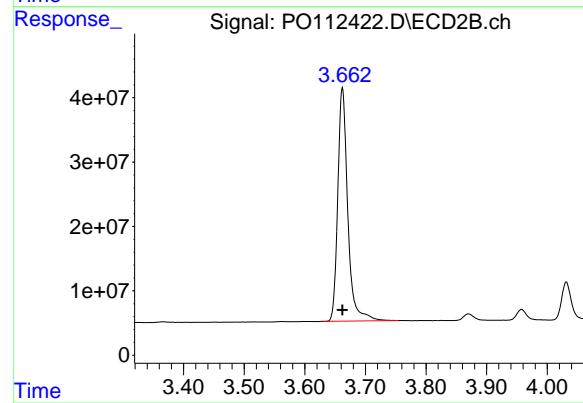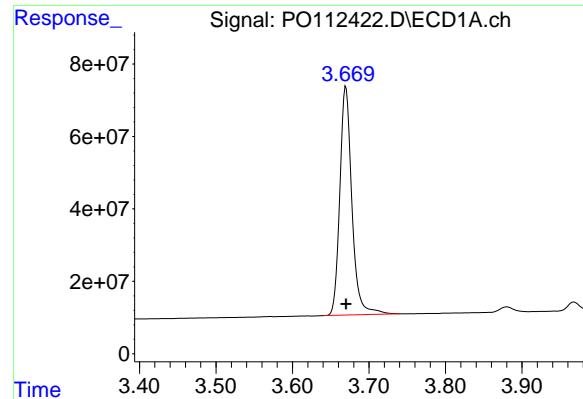

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: 0.000 min
 Response: 689642409
 Conc: 75.12 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1242ICC750

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
 Delta R.T.: 0.000 min
 Response: 415759444
 Conc: 75.14 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
 Delta R.T.: 0.000 min
 Response: 602849206
 Conc: 74.96 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.641 min
 Delta R.T.: 0.000 min
 Response: 140388070
 Conc: 74.84 ng/ml

#16 AR-1242-1


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 194676689
 Conc: 752.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC750

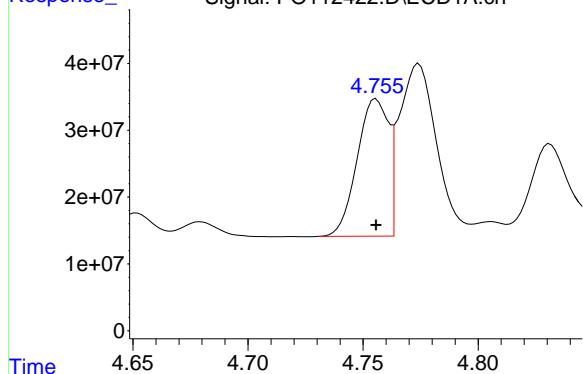


#16 AR-1242-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 118711810
 Conc: 751.13 ng/ml

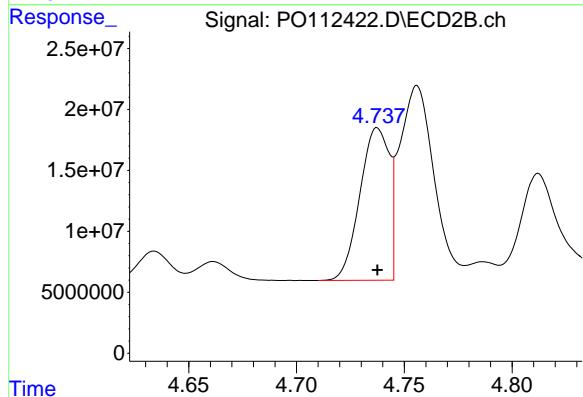


#17 AR-1242-2


R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 290316602
 Conc: 750.96 ng/ml

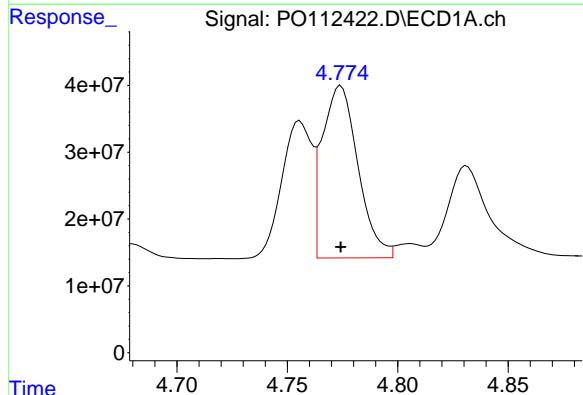

#17 AR-1242-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 177174842
 Conc: 750.10 ng/ml

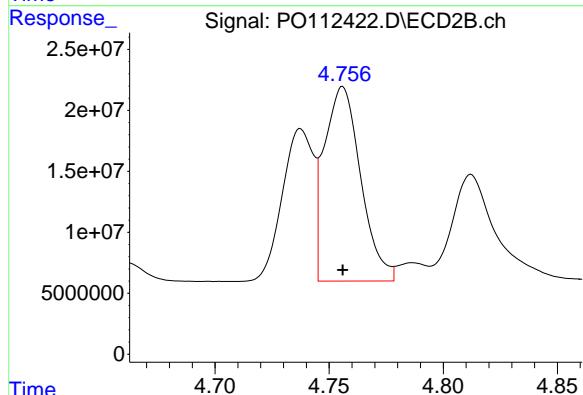

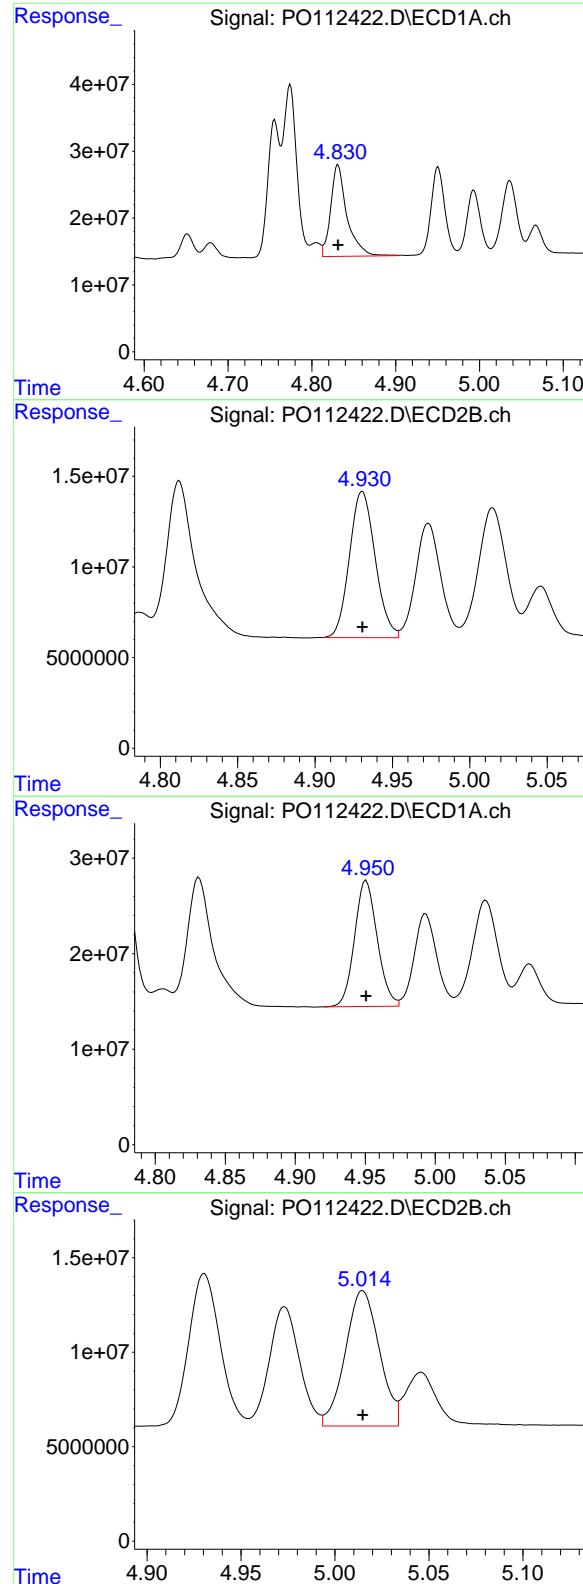

#18 AR-1242-3

R.T.: 4.831 min
 Delta R.T.: 0.000 min
 Response: 184857008
 Conc: 752.92 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC750

#18 AR-1242-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 93444753
 Conc: 753.13 ng/ml

#19 AR-1242-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 148772992
 Conc: 749.30 ng/ml



#19 AR-1242-4

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 90566785
 Conc: 750.75 ng/ml

#20 AR-1242-5

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 165130835
Conc: 744.94 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC750

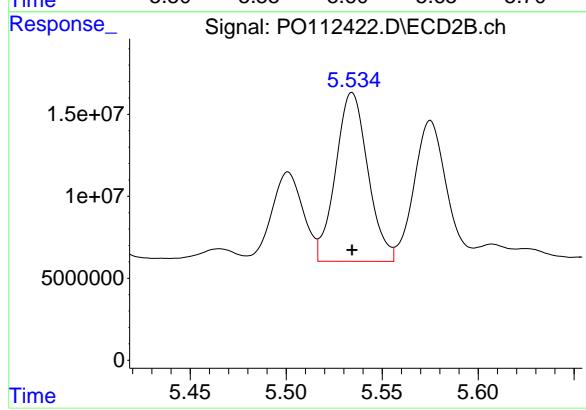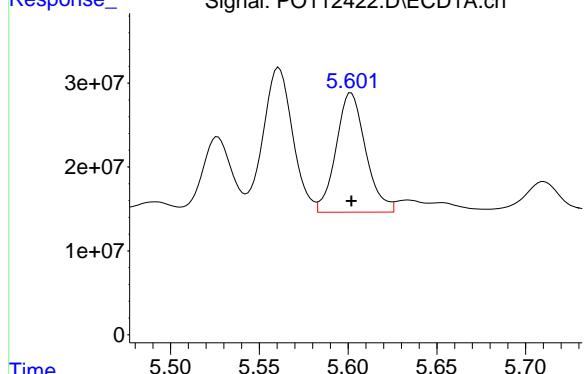

#20 AR-1242-5

R.T.: 5.534 min
Delta R.T.: 0.000 min
Response: 120680300
Conc: 750.33 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:17
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:40:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:40:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 461.0E6 | 278.7E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.693 | 8.641 | 404.4E6 | 96205236 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 16) L4 AR-1242-1 | 4.755 | 4.737 | 130.3E6 | 81100988 | 500.000 | 500.000 |
| 17) L4 AR-1242-2 | 4.774 | 4.755 | 195.8E6 | 120.9E6 | 500.000 | 500.000 |
| 18) L4 AR-1242-3 | 4.831 | 4.931 | 124.2E6 | 63316612 | 500.000 | 500.000 |
| 19) L4 AR-1242-4 | 4.951 | 5.015 | 100.8E6 | 62114890 | 500.000 | 500.000 |
| 20) L4 AR-1242-5 | 5.602 | 5.534 | 114.6E6 | 83558195 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:17
 Operator : YP/AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:40:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:40:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

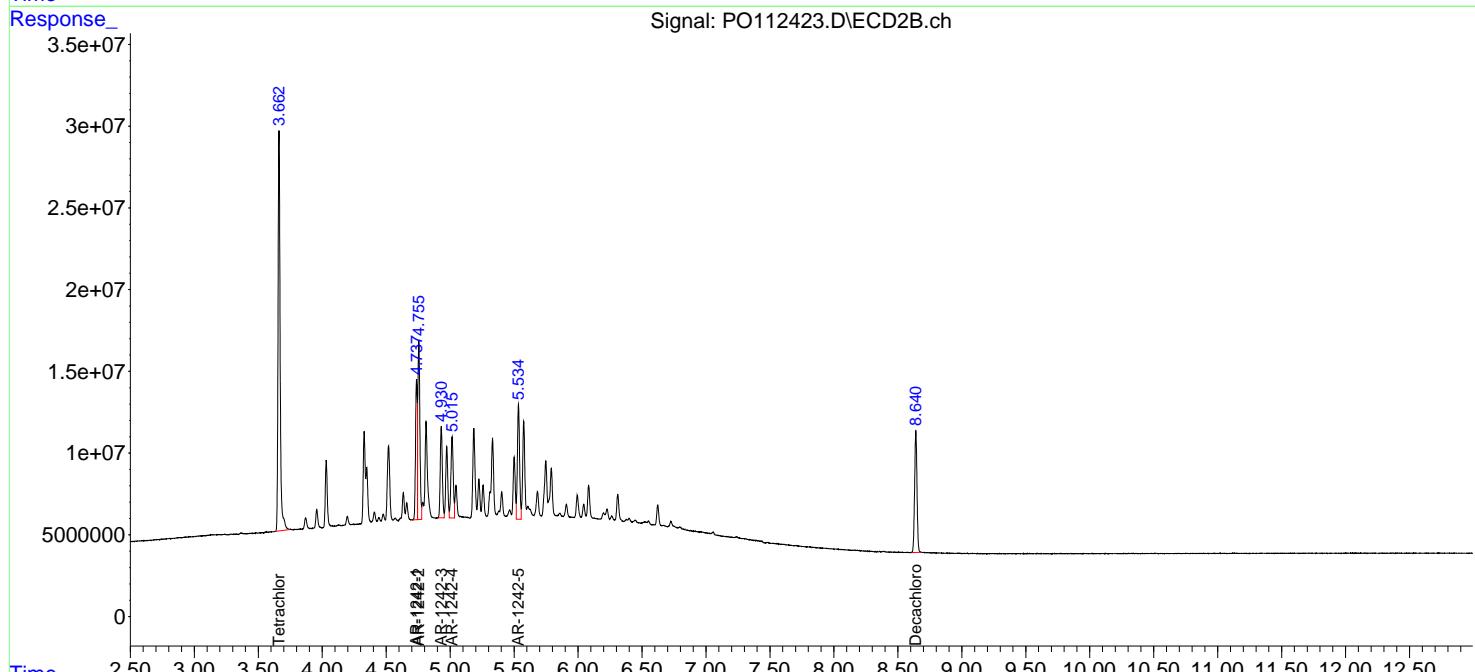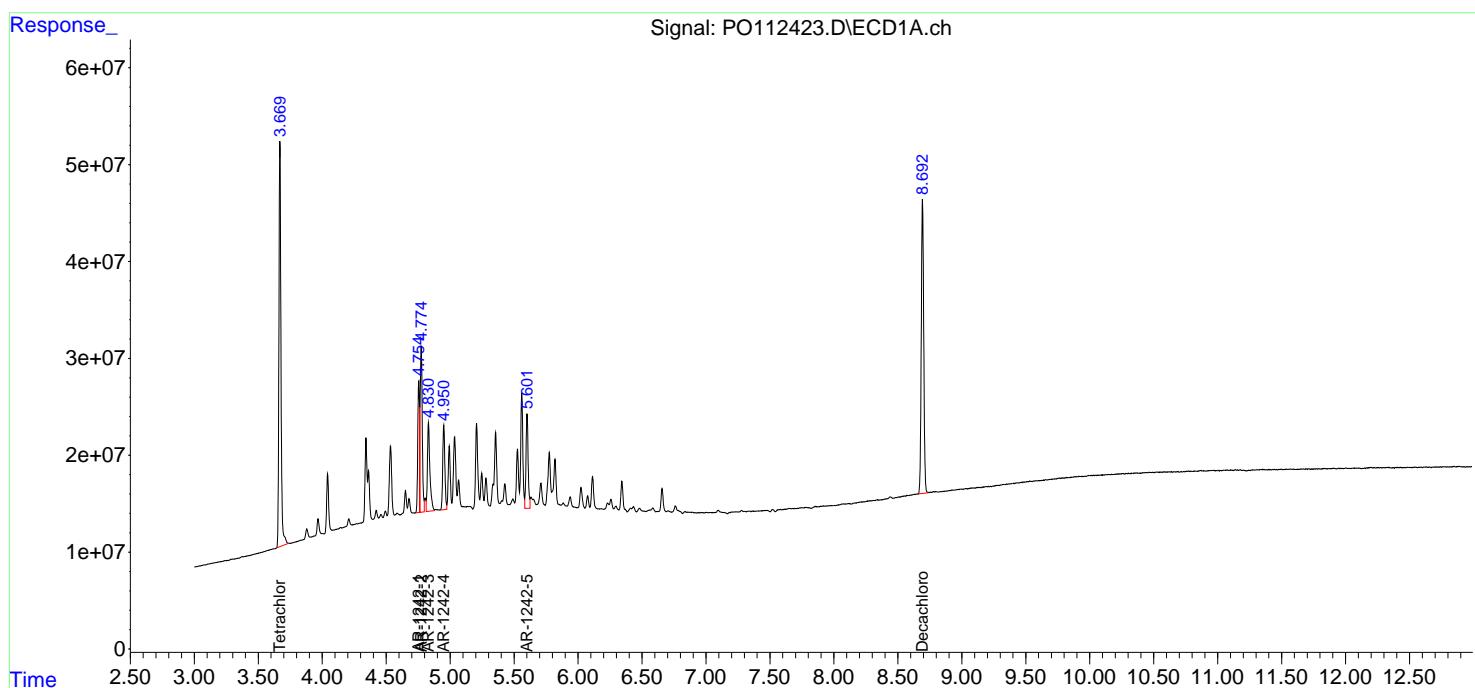

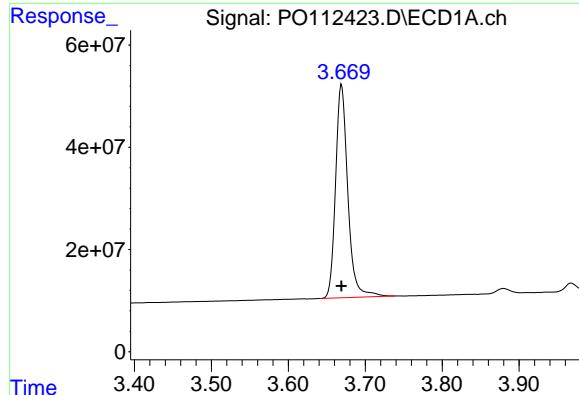

#1 Tetrachloro-m-xylene

R.T.: 3.669 min

Delta R.T.: 0.000 min

Response: 460974572


Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1242ICC500

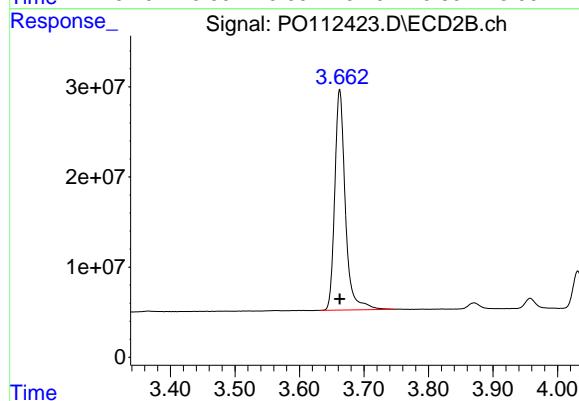


#1 Tetrachloro-m-xylene

R.T.: 3.662 min

Delta R.T.: 0.000 min

Response: 278677618

Conc: 50.00 ng/ml

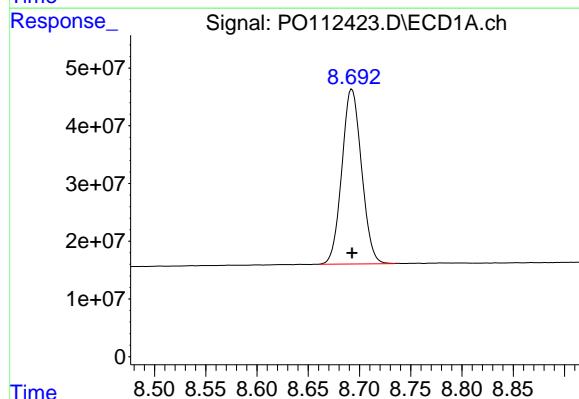


#2 Decachlorobiphenyl

R.T.: 8.693 min

Delta R.T.: 0.000 min

Response: 404398351

Conc: 50.00 ng/ml

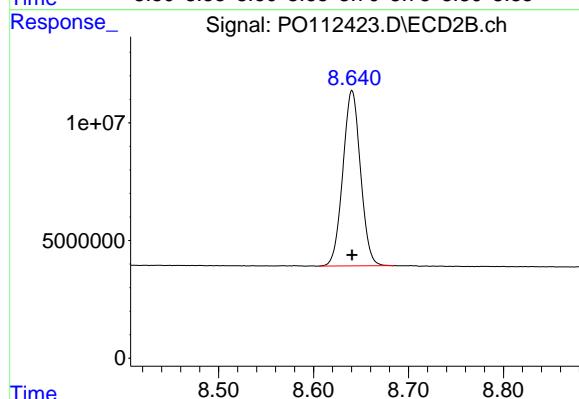


#2 Decachlorobiphenyl

R.T.: 8.641 min

Delta R.T.: 0.000 min

Response: 96205236

Conc: 50.00 ng/ml

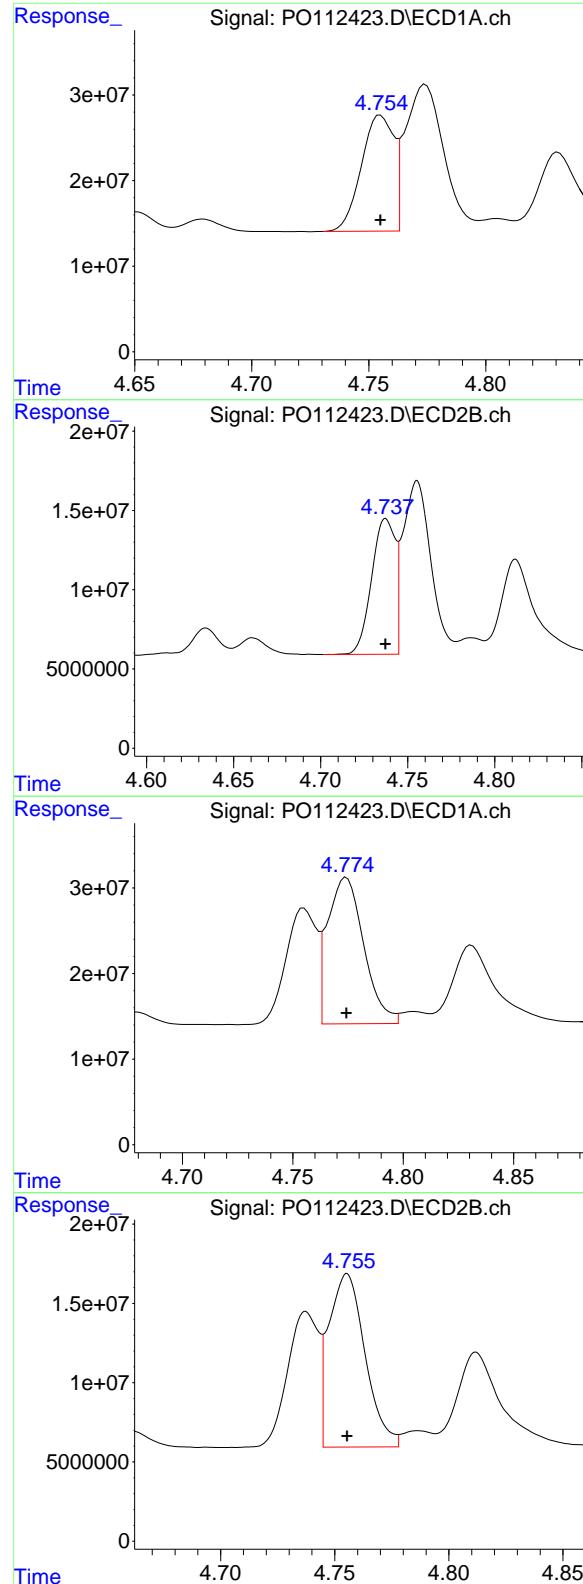

#16 AR-1242-1

R.T.: 4.755 min
 Delta R.T.: 0.000 min
 Response: 130330227
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC500

#16 AR-1242-1

R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 81100988
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 195778431
 Conc: 500.00 ng/ml





#17 AR-1242-2

R.T.: 4.755 min
 Delta R.T.: 0.000 min
 Response: 120908349
 Conc: 500.00 ng/ml

#18 AR-1242-3

R.T.: 4.831 min
 Delta R.T.: 0.000 min
 Response: 124157527
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC500

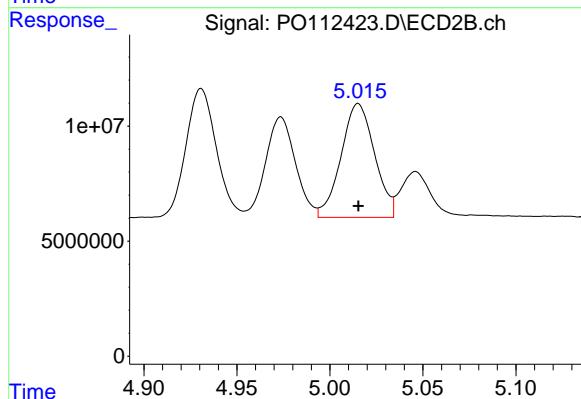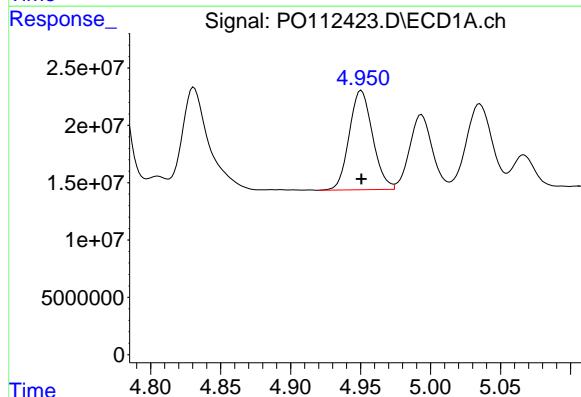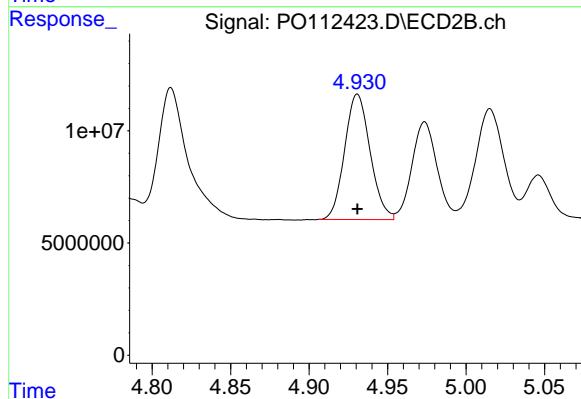

#18 AR-1242-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 63316612
 Conc: 500.00 ng/ml

#19 AR-1242-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 100782451
 Conc: 500.00 ng/ml

#19 AR-1242-4

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 62114890
 Conc: 500.00 ng/ml

#20 AR-1242-5


R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 114591495
Conc: 500.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1242ICC500

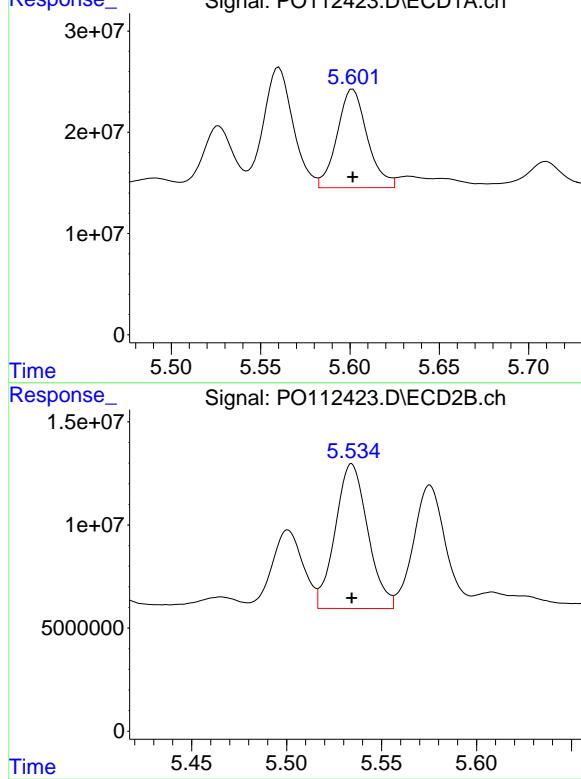

#20 AR-1242-5

R.T.: 5.534 min
Delta R.T.: 0.000 min
Response: 83558195
Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:36
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:50:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:50:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 230.2E6 | 140.8E6 | 25.056 | 25.329 |
| 2) SA Decachlor... | 8.692 | 8.640 | 202.2E6 | 49177998 | 25.104 | 25.901 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|----------|
| 16) L4 AR-1242-1 | 4.756 | 4.737 | 66274294 | 42281301 | 254.503 | 262.921 |
| 17) L4 AR-1242-2 | 4.774 | 4.756 | 98384229 | 63307827 | 253.352 | 263.280 |
| 18) L4 AR-1242-3 | 4.830 | 4.930 | 63048920 | 32586963 | 255.064 | 259.362 |
| 19) L4 AR-1242-4 | 4.951 | 5.015 | 50849599 | 32274308 | 254.552 | 262.925 |
| 20) L4 AR-1242-5 | 5.601 | 5.534 | 57385959 | 40990023 | 262.483m | 253.808m |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:36
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:50:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:50:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation





Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
ClientSampleId :
 AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

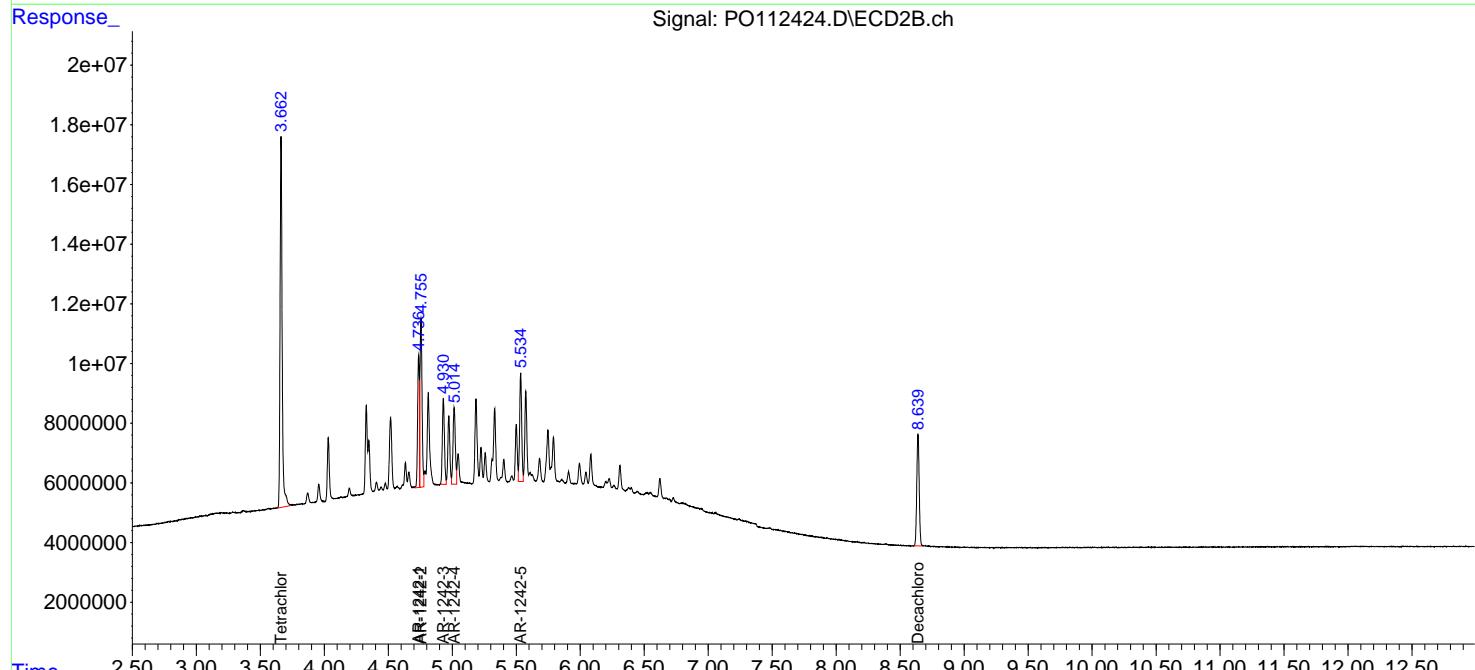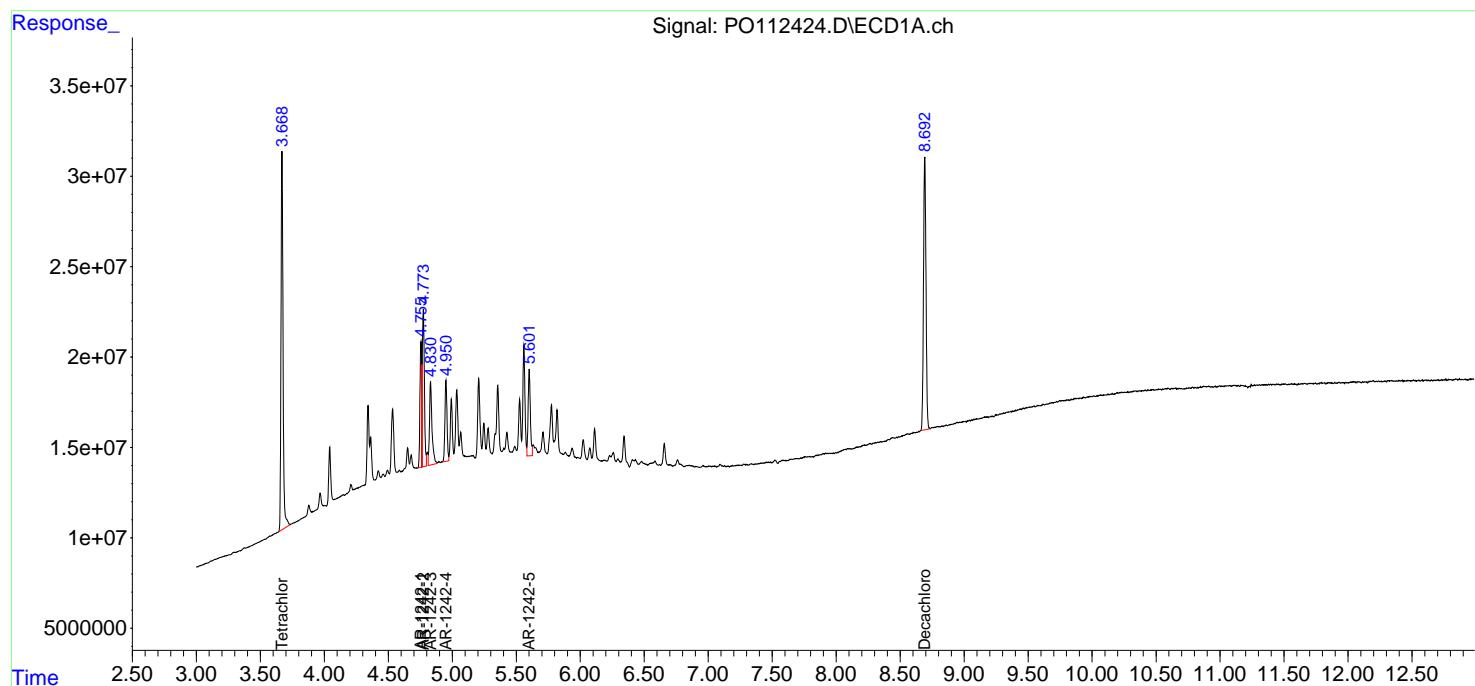

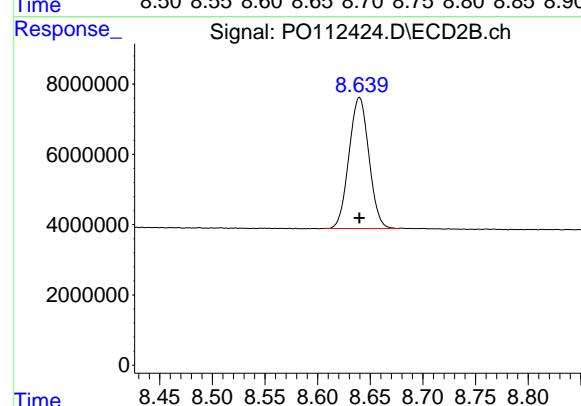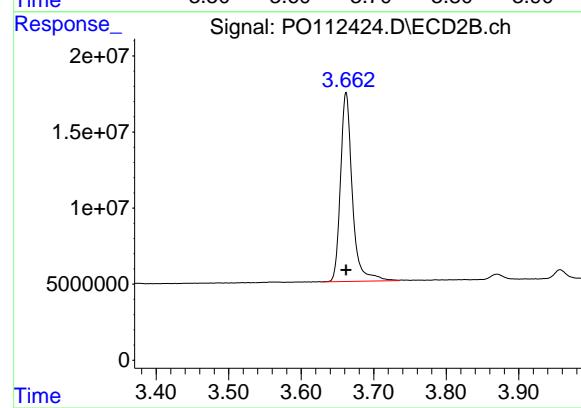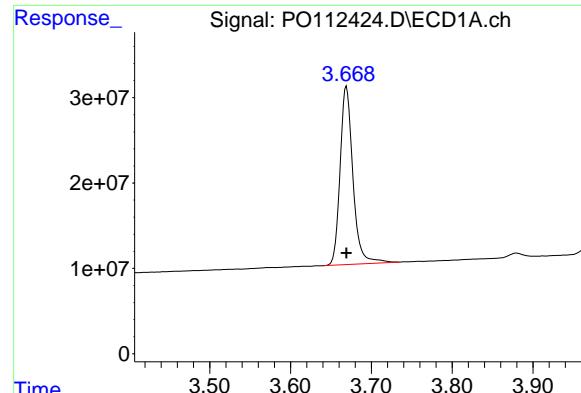

#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 230185927
Conc: 25.06 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

#1 Tetrachloro-m-xylene





R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 140771642
Conc: 25.33 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: 0.000 min
Response: 202170823
Conc: 25.10 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 49177998
Conc: 25.90 ng/ml

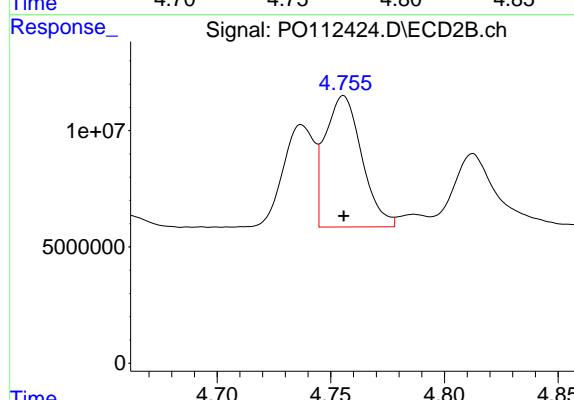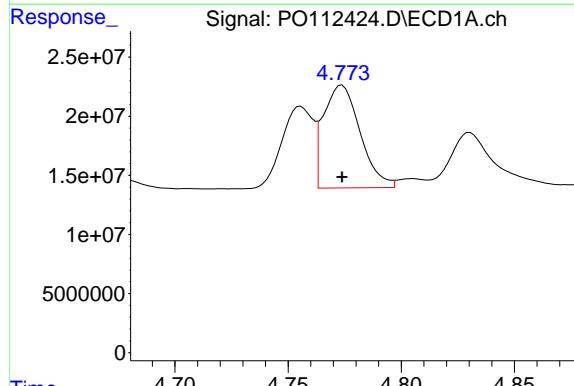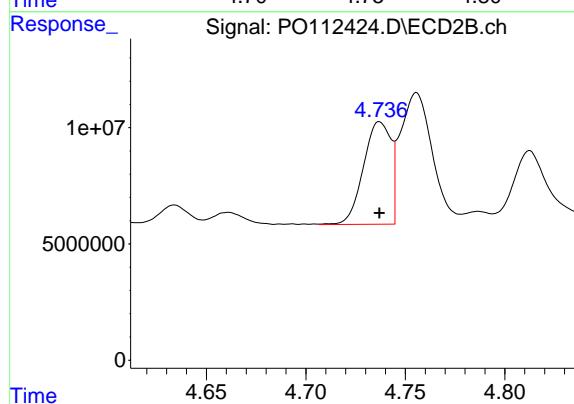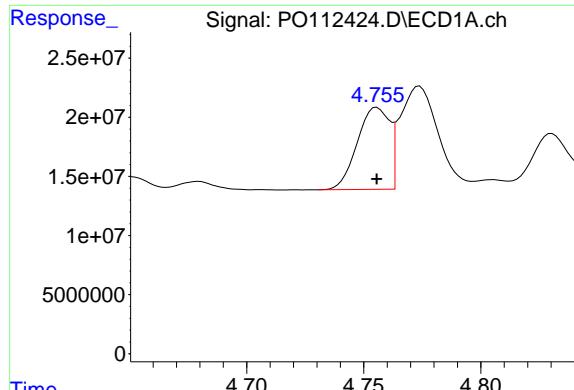

#16 AR-1242-1

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 66274294
Conc: 254.50 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

#16 AR-1242-1

R.T.: 4.737 min
Delta R.T.: 0.000 min
Response: 42281301
Conc: 262.92 ng/ml

#17 AR-1242-2

R.T.: 4.774 min
Delta R.T.: 0.000 min
Response: 98384229
Conc: 253.35 ng/ml

#17 AR-1242-2

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 63307827
Conc: 263.28 ng/ml

#18 AR-1242-3

R.T.: 4.830 min
 Delta R.T.: 0.000 min
 Response: 63048920
 Conc: 255.06 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#18 AR-1242-3





R.T.: 4.930 min
 Delta R.T.: 0.000 min
 Response: 32586963
 Conc: 259.36 ng/ml

#19 AR-1242-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 50849599
 Conc: 254.55 ng/ml

#19 AR-1242-4

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 32274308
 Conc: 262.93 ng/ml

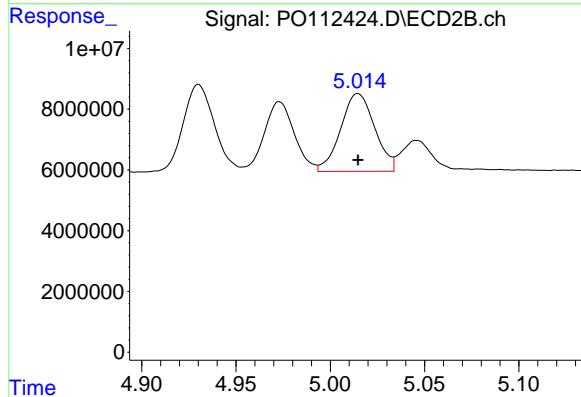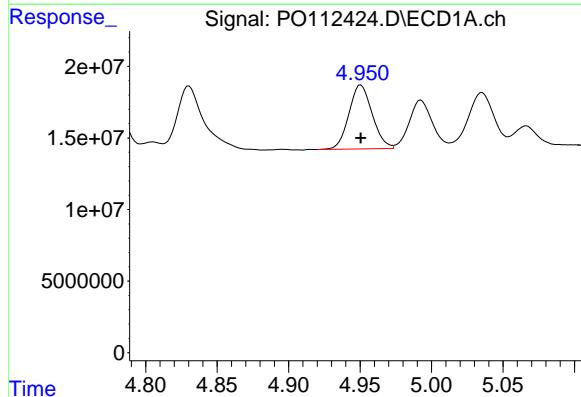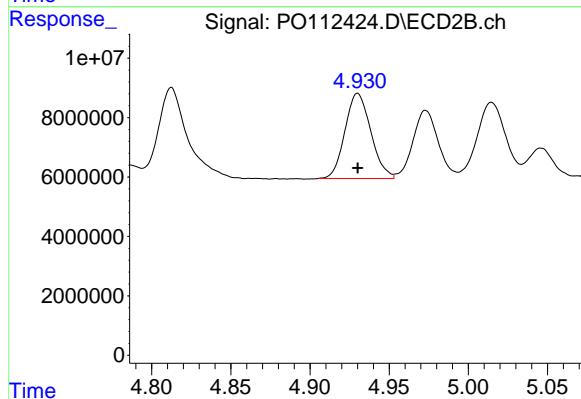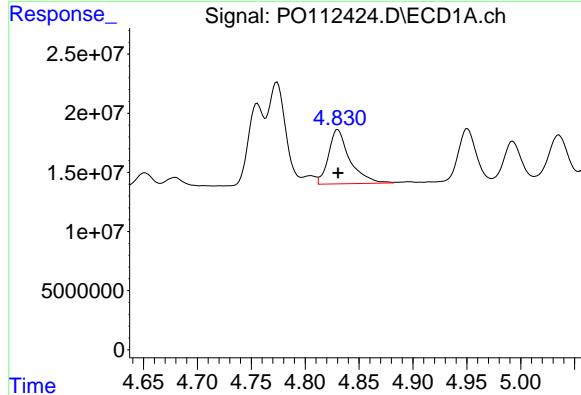



#20 AR-1242-5

R.T.: 5.601 min
 Delta R.T.: 0.000 min
 Response: 57385959
 Conc: 262.48 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

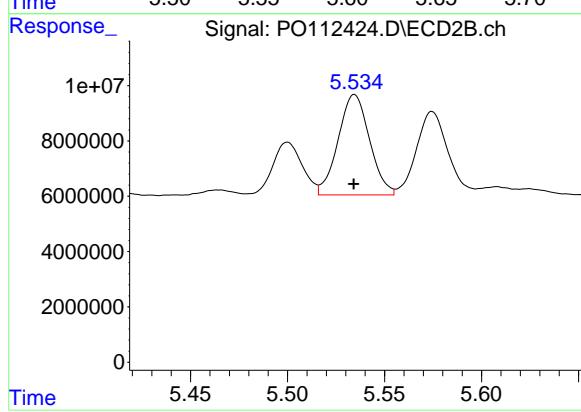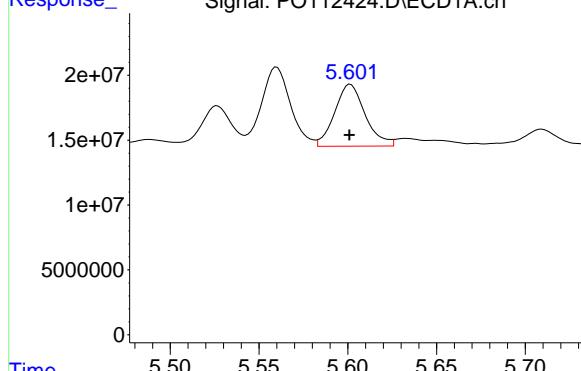

#20 AR-1242-5

R.T.: 5.534 min
 Delta R.T.: 0.000 min
 Response: 40990023
 Conc: 253.81 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:54
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 15:07:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 15:07:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 31709040 | 20307281 | 3.679 | 3.861m |
| 2) SA Decachlor... | 8.695 | 8.640 | 31949919 | 7899252 | 4.138 | 4.305 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 16) L4 AR-1242-1 | 4.757 | 4.738 | 9816709 | 7435731 | 39.649 | 46.945 |
| 17) L4 AR-1242-2 | 4.776 | 4.756 | 14782408 | 10324894 | 39.975 | 44.186 |
| 18) L4 AR-1242-3 | 4.833 | 4.932 | 9726638 | 5168677 | 41.100 | 42.650 |
| 19) L4 AR-1242-4 | 4.952 | 5.016 | 8617431 | 6134656 | 44.356 | 49.981 |
| 20) L4 AR-1242-5 | 5.603 | 5.535 | 8751010 | 7919520 | 41.522m | 48.545m |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:54
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 15:07:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 15:07:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

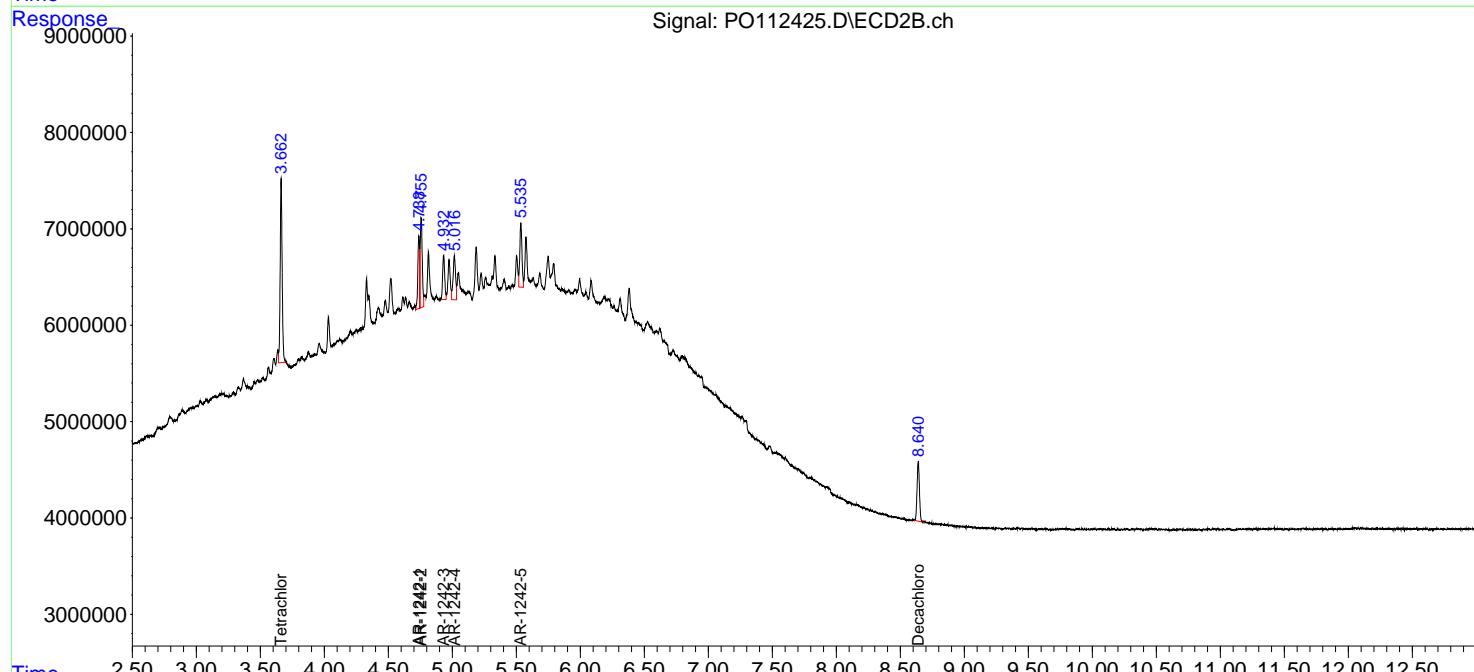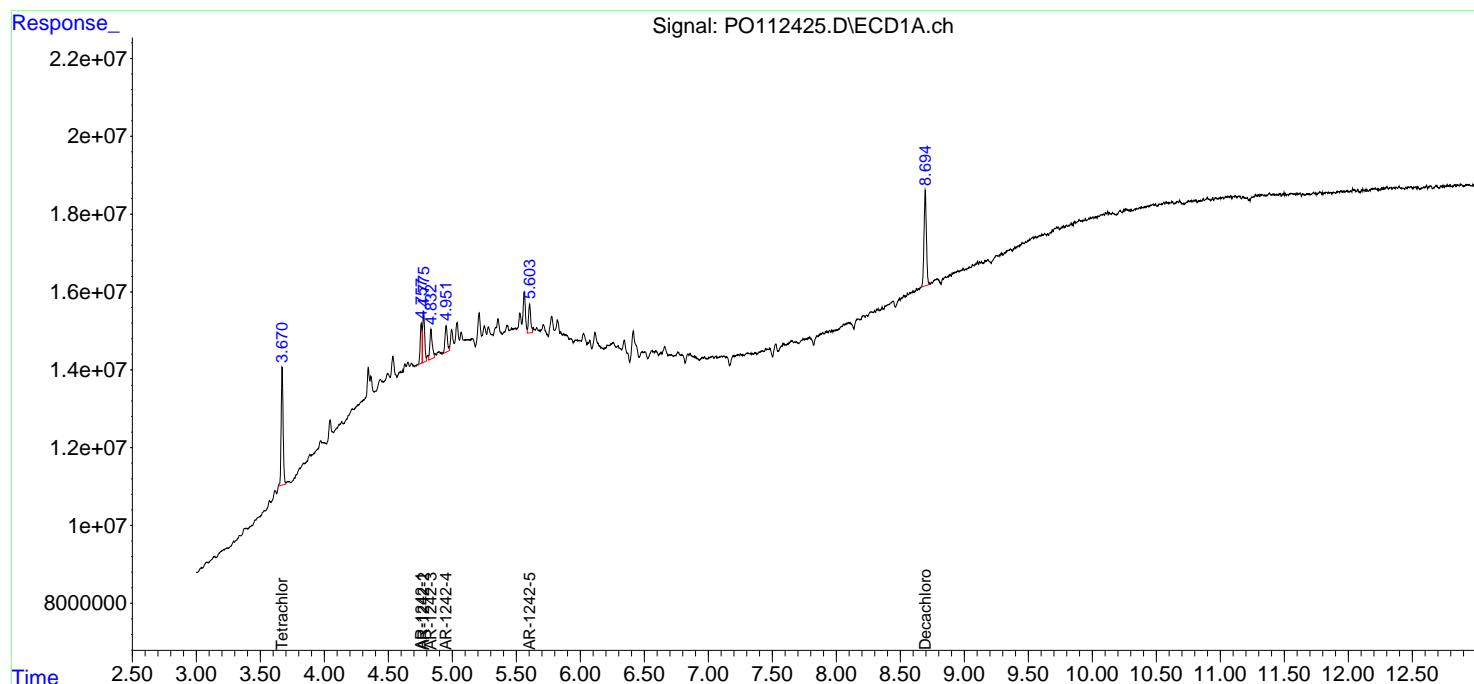

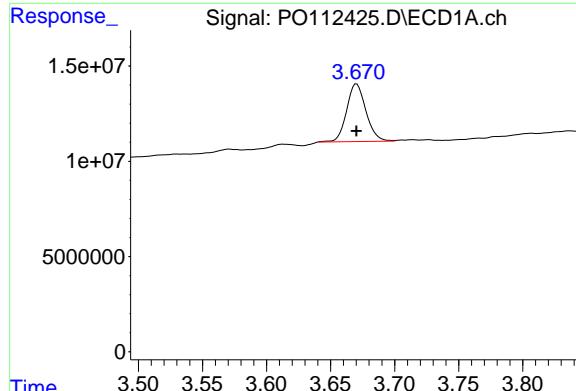


#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 31709040
Conc: 3.68 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

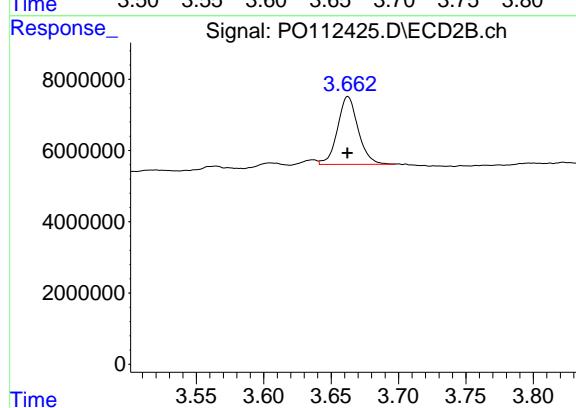


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 20307281
Conc: 3.86 ng/ml

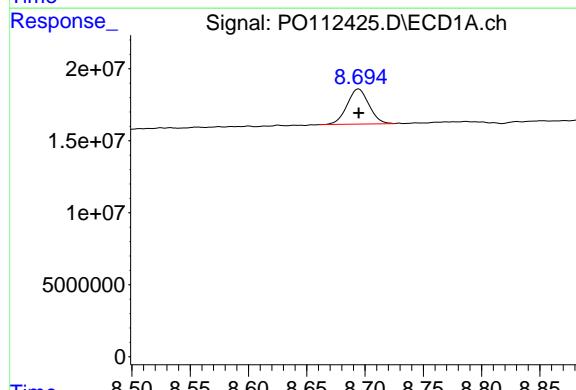


#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 31949919
Conc: 4.14 ng/ml

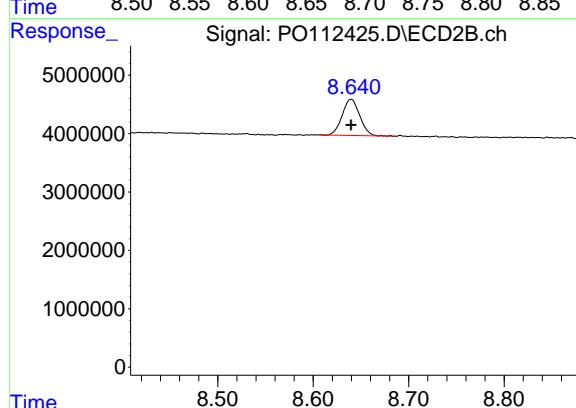

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 7899252
Conc: 4.30 ng/ml

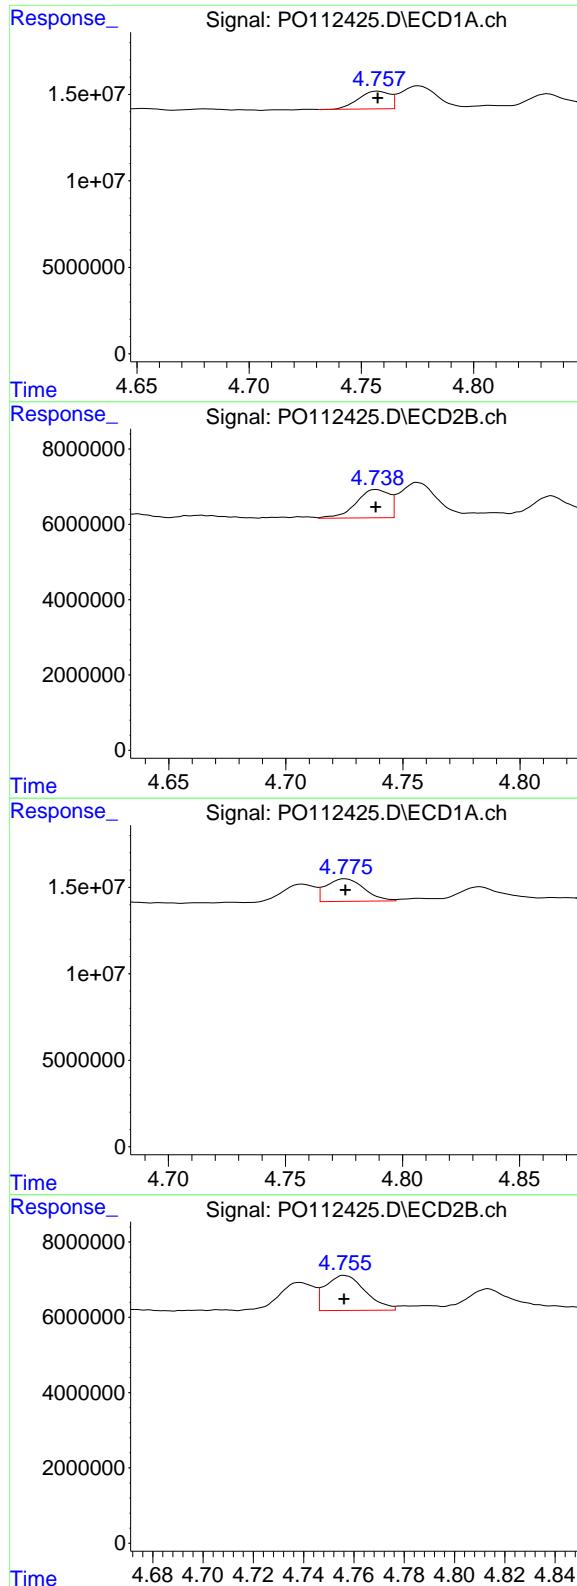

#16 AR-1242-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 9816709
 Conc: 39.65 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#16 AR-1242-1


R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 7435731
 Conc: 46.94 ng/ml

#17 AR-1242-2

R.T.: 4.776 min
 Delta R.T.: 0.000 min
 Response: 14782408
 Conc: 39.97 ng/ml

#17 AR-1242-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 10324894
 Conc: 44.19 ng/ml

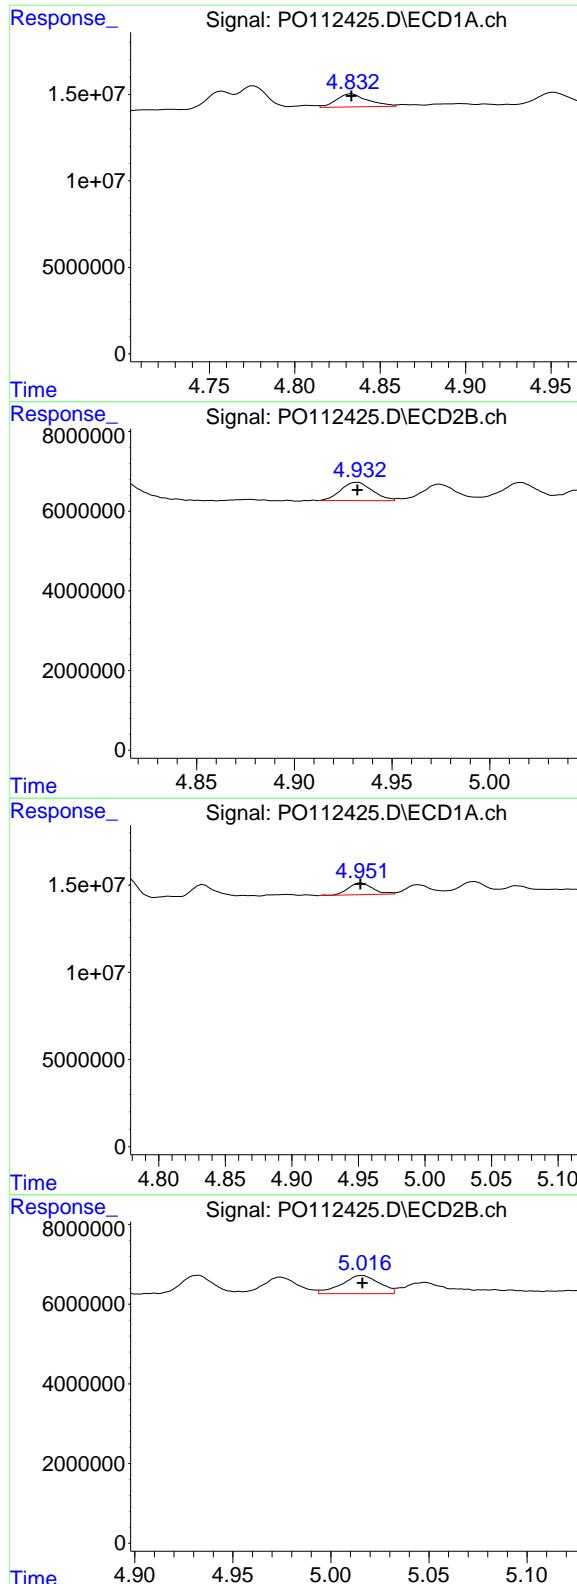

#18 AR-1242-3

R.T.: 4.833 min
 Delta R.T.: 0.000 min
 Response: 9726638
 Conc: 41.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#18 AR-1242-3

R.T.: 4.932 min
 Delta R.T.: 0.000 min
 Response: 5168677
 Conc: 42.65 ng/ml

#19 AR-1242-4

R.T.: 4.952 min
 Delta R.T.: 0.000 min
 Response: 8617431
 Conc: 44.36 ng/ml

#19 AR-1242-4

R.T.: 5.016 min
 Delta R.T.: 0.000 min
 Response: 6134656
 Conc: 49.98 ng/ml



#20 AR-1242-5

R.T.: 5.603 min
 Delta R.T.: 0.000 min
 Response: 8751010
 Conc: 41.52 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

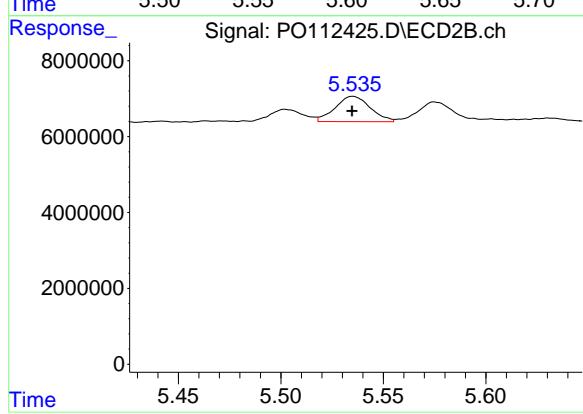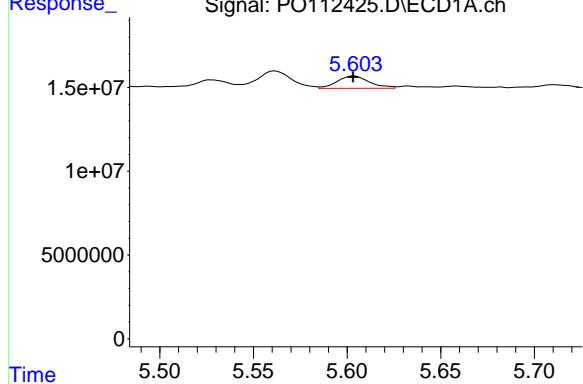

#20 AR-1242-5

R.T.: 5.535 min
 Delta R.T.: 0.000 min
 Response: 7919520
 Conc: 48.54 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:13
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:42:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 894.7E6 | 536.3E6 | 98.207 | 98.214 |
| 2) SA Decachlor... | 8.694 | 8.642 | 790.0E6 | 183.7E6 | 98.166 | 97.230 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|---------|---------|---------|
| 21) L5 AR-1248-1 | 4.756 | 4.738 | 189.3E6 | 116.8E6 | 976.657 | 958.799 |
| 22) L5 AR-1248-2 | 4.994 | 4.974 | 257.1E6 | 161.8E6 | 974.386 | 958.261 |
| 23) L5 AR-1248-3 | 5.208 | 5.015 | 329.8E6 | 170.7E6 | 969.727 | 961.014 |
| 24) L5 AR-1248-4 | 5.561 | 5.185 | 503.2E6 | 202.5E6 | 964.167 | 960.436 |
| 25) L5 AR-1248-5 | 5.602 | 5.576 | 346.5E6 | 207.1E6 | 961.394 | 953.250 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112426.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:13
 Operator : YP/AJ
 Sample : AR1248ICC1000
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:42:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

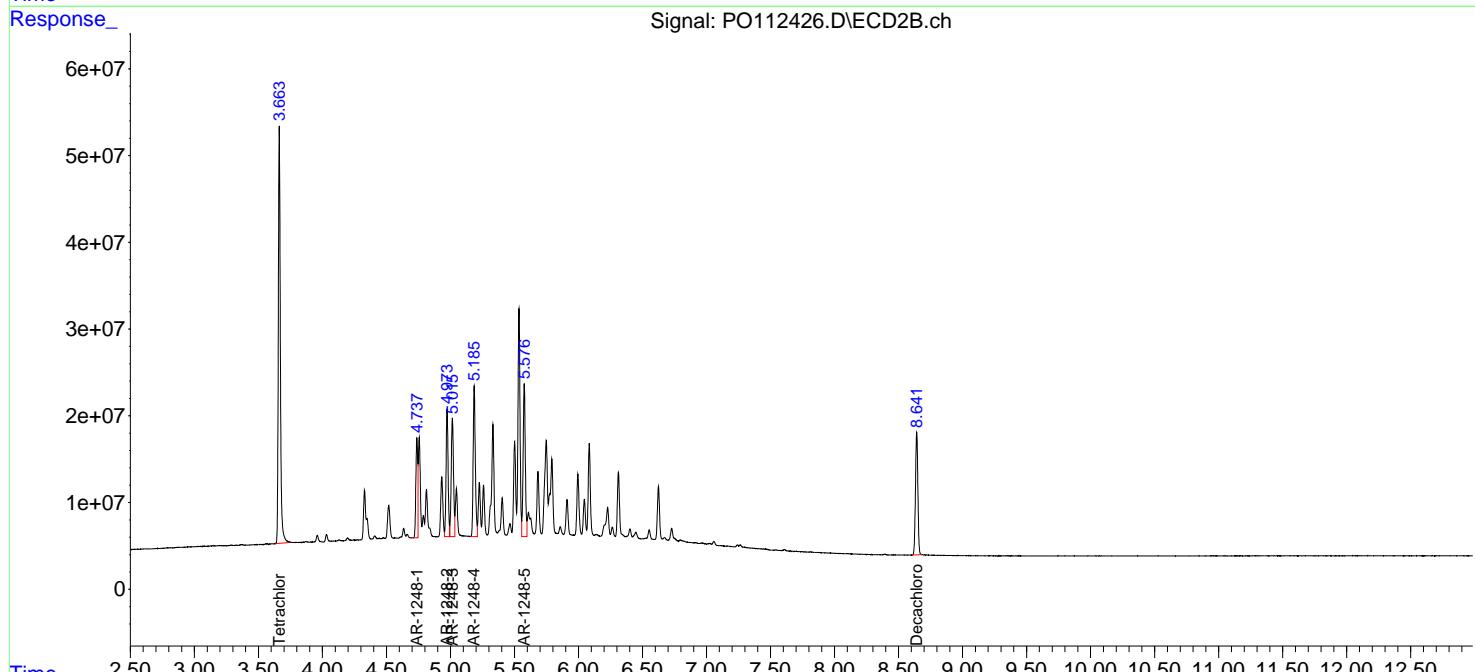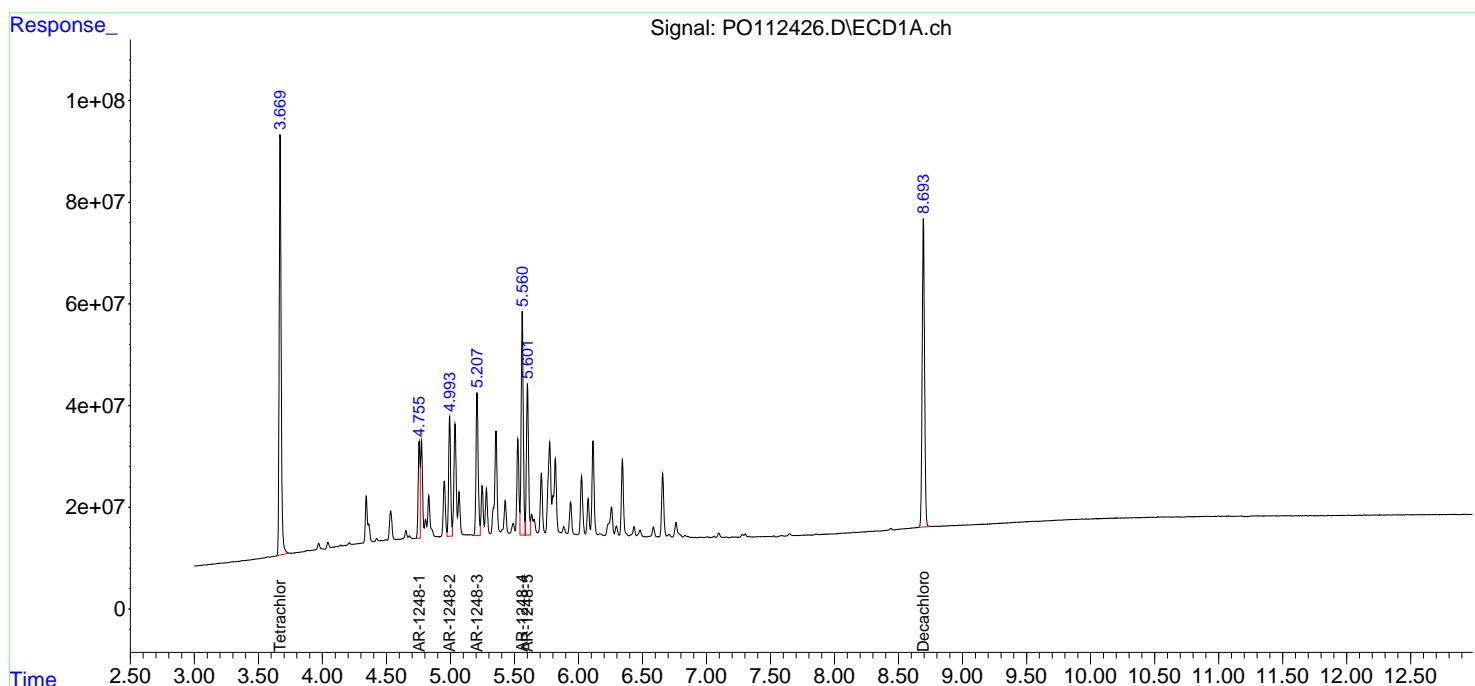

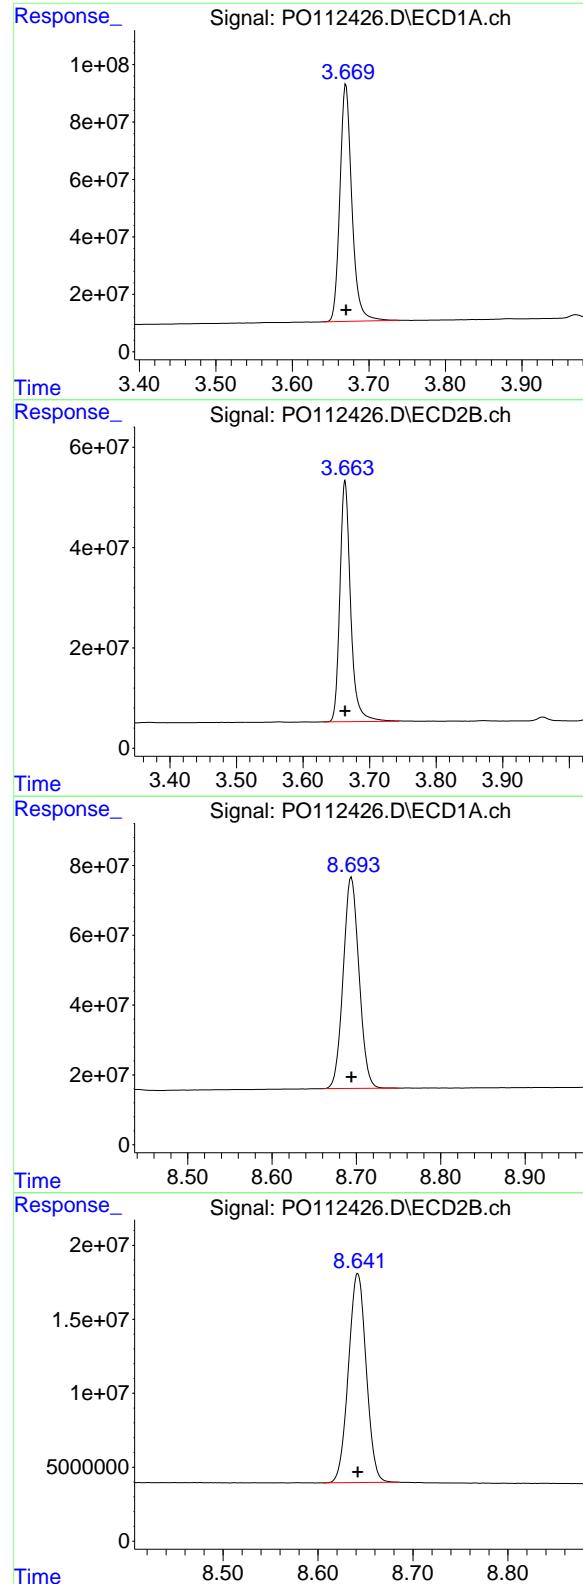

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 894659096
Conc: 98.21 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1248ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 536299018
Conc: 98.21 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 790001849
Conc: 98.17 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.642 min
Delta R.T.: 0.000 min
Response: 183652482
Conc: 97.23 ng/ml

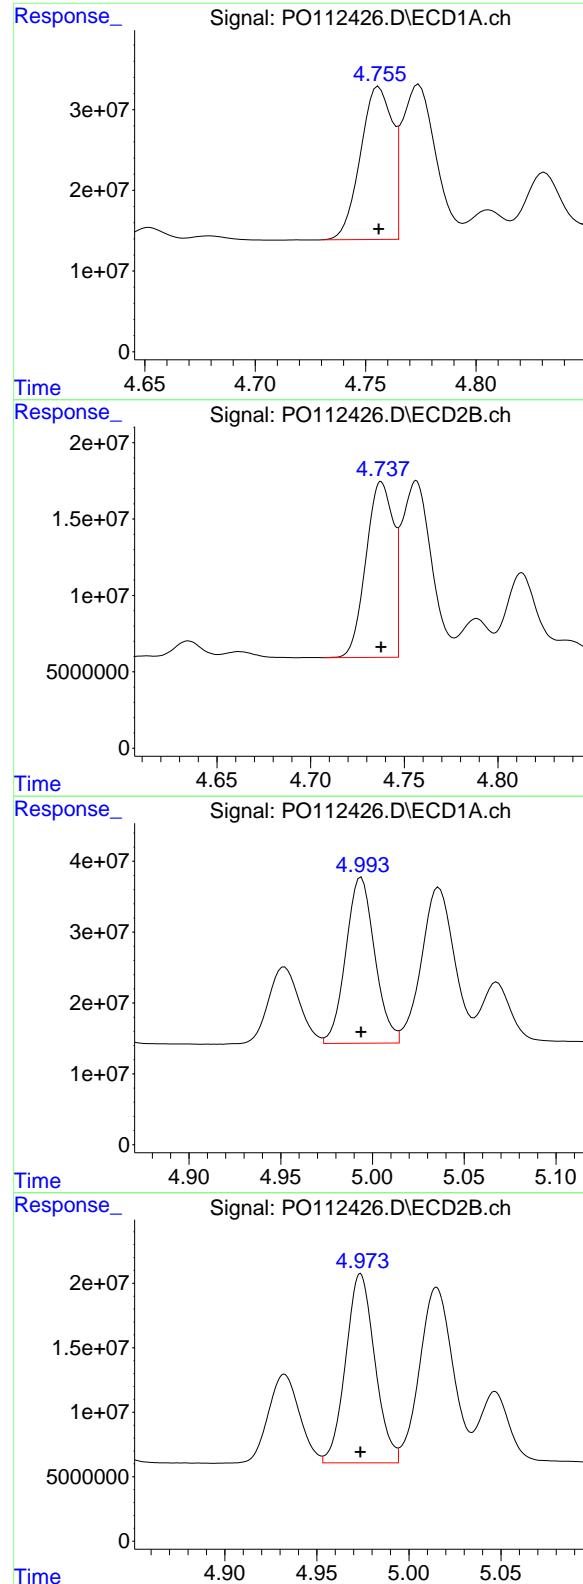

#21 AR-1248-1

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 189314500
 Conc: 976.66 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC1000

#21 AR-1248-1


R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 116797575
 Conc: 958.80 ng/ml

#22 AR-1248-2

R.T.: 4.994 min
 Delta R.T.: 0.000 min
 Response: 257058197
 Conc: 974.39 ng/ml

#22 AR-1248-2

R.T.: 4.974 min
 Delta R.T.: 0.000 min
 Response: 161755092
 Conc: 958.26 ng/ml

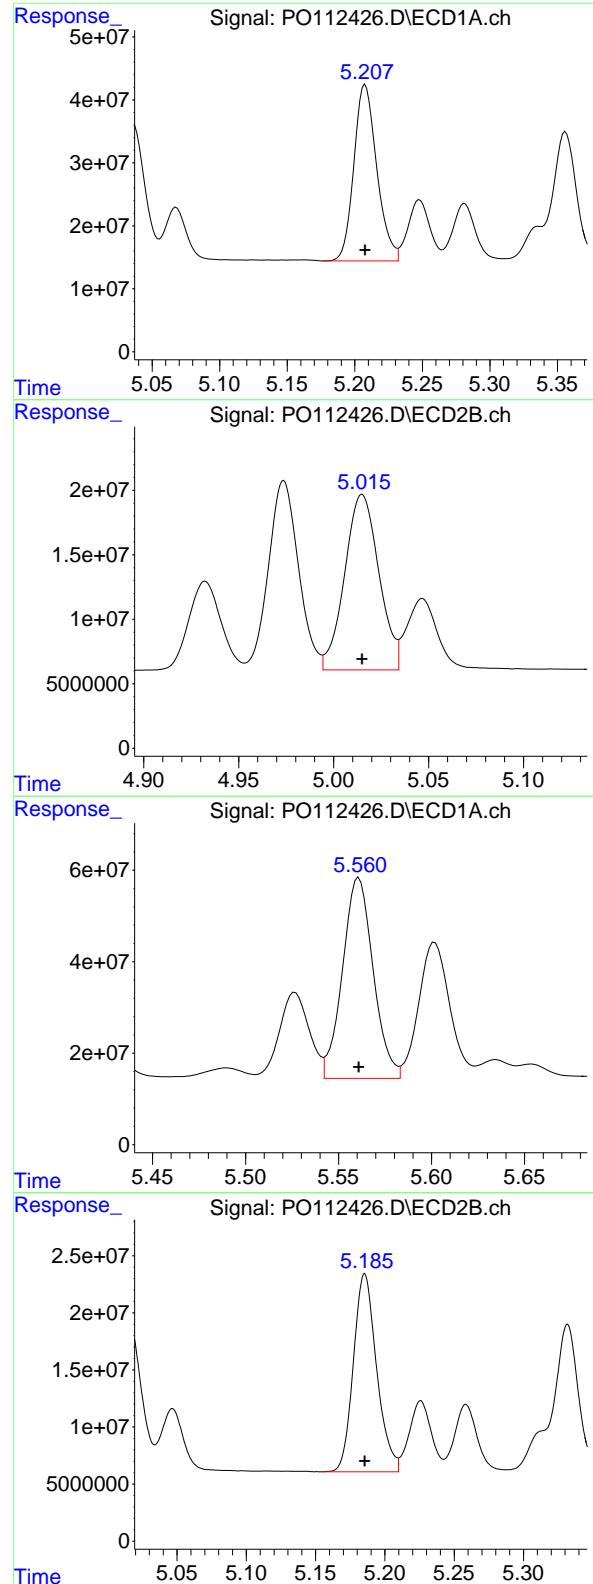

#23 AR-1248-3

R.T.: 5.208 min
 Delta R.T.: 0.000 min
 Response: 329824745
 Conc: 969.73 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC1000

#23 AR-1248-3

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 170672394
 Conc: 961.01 ng/ml

#24 AR-1248-4

R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 503150480
 Conc: 964.17 ng/ml



#24 AR-1248-4

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 202462025
 Conc: 960.44 ng/ml

#25 AR-1248-5

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 346508966
Conc: 961.39 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC1000

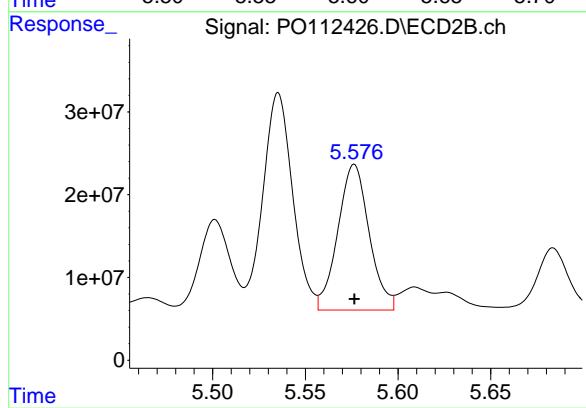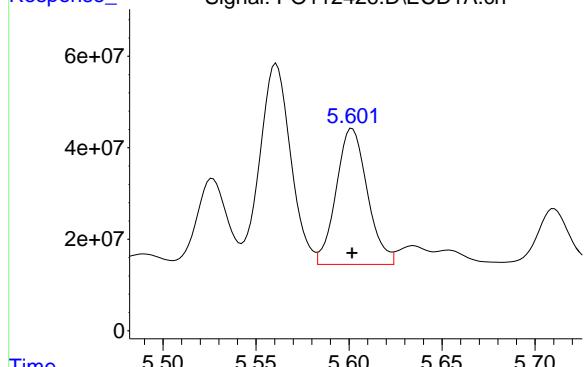

#25 AR-1248-5

R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 207118457
Conc: 953.25 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:31
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:46:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 689.2E6 | 412.7E6 | 75.433 | 75.386 |
| 2) SA Decachlor... | 8.694 | 8.640 | 606.5E6 | 140.9E6 | 75.240 | 74.725 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 21) L5 AR-1248-1 | 4.755 | 4.737 | 145.1E6 | 91310177 | 748.883 | 749.714 |
| 22) L5 AR-1248-2 | 4.993 | 4.973 | 199.5E6 | 126.7E6 | 754.166 | 750.310 |
| 23) L5 AR-1248-3 | 5.207 | 5.015 | 257.0E6 | 133.7E6 | 753.762 | 751.756 |
| 24) L5 AR-1248-4 | 5.560 | 5.185 | 392.7E6 | 158.0E6 | 751.645 | 749.628 |
| 25) L5 AR-1248-5 | 5.601 | 5.575 | 272.4E6 | 162.1E6 | 753.927 | 747.333 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112427.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:31
 Operator : YP/AJ
 Sample : AR1248ICC750
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:46:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

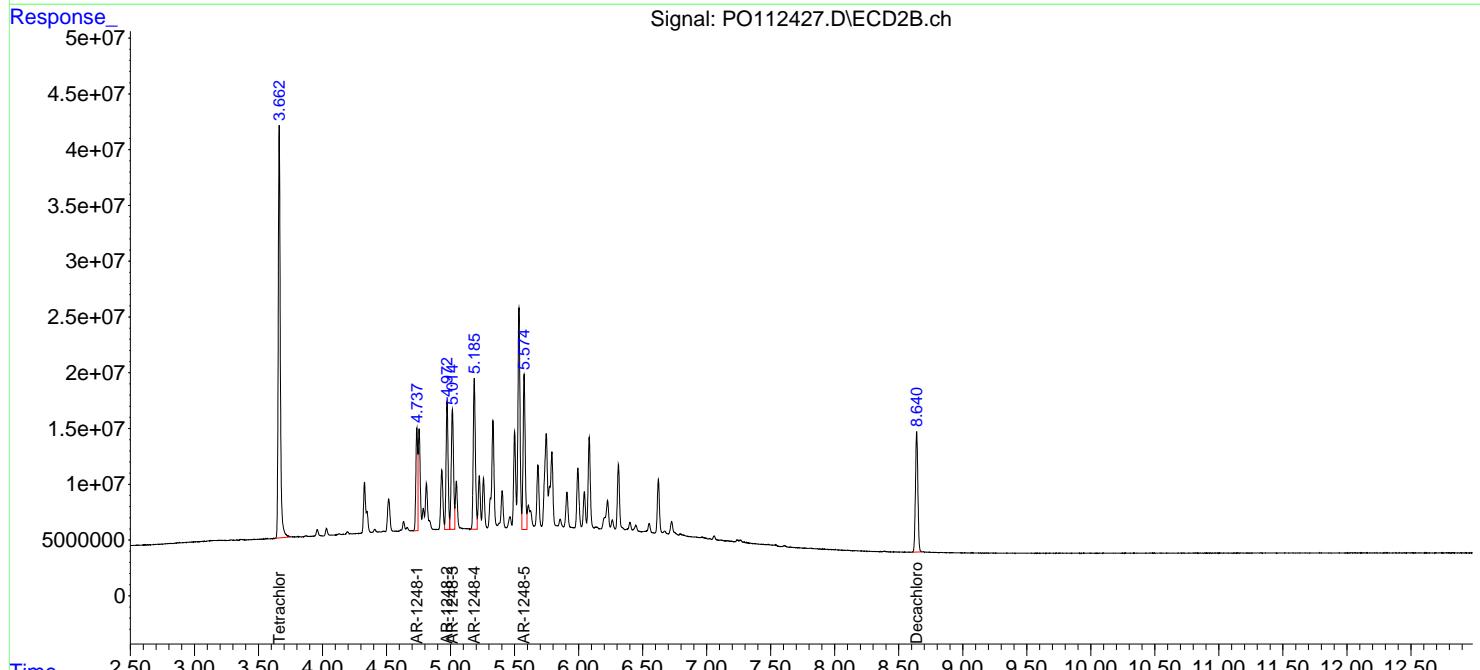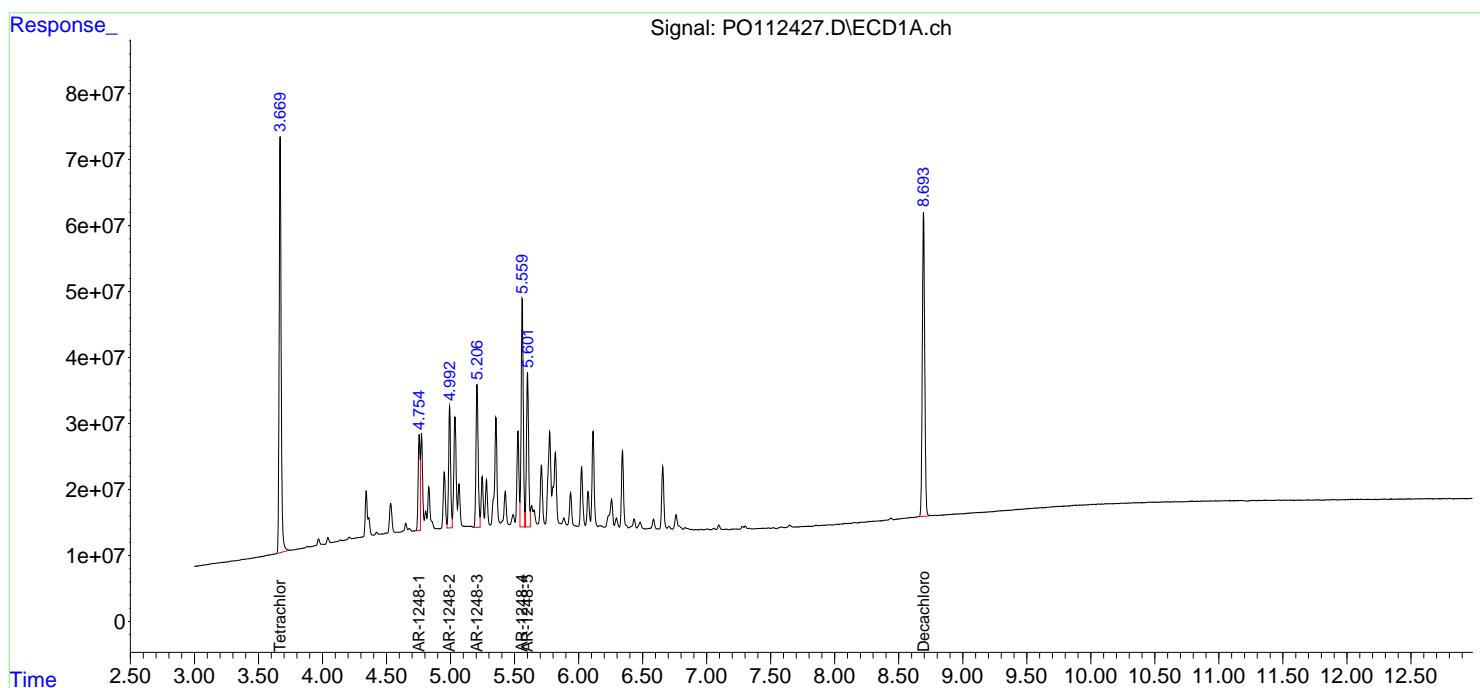

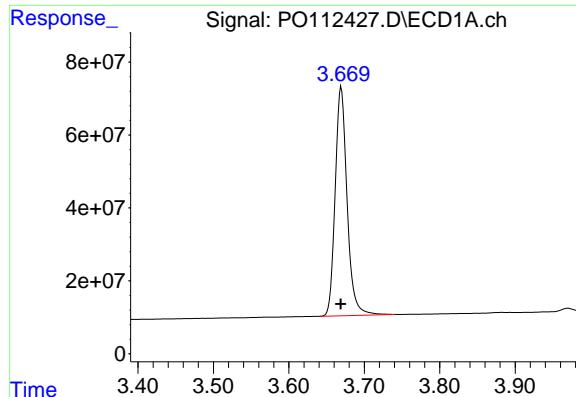

#1 Tetrachloro-m-xylene

R.T.: 3.669 min

Delta R.T.: 0.000 min

Instrument:


Response: 689179613

ECD_O

Conc: 75.43 ng/ml

ClientSampleId :

AR1248ICC750

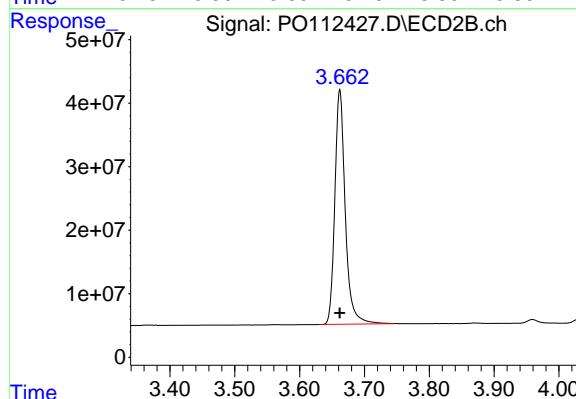


#1 Tetrachloro-m-xylene

R.T.: 3.662 min

Delta R.T.: 0.000 min

Response: 412707775

Conc: 75.39 ng/ml

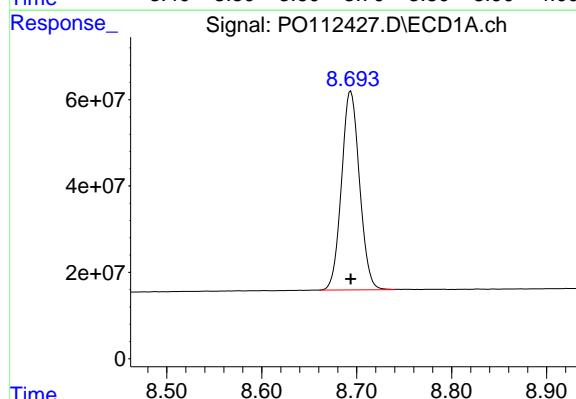


#2 Decachlorobiphenyl

R.T.: 8.694 min

Delta R.T.: 0.000 min

Response: 606473130

Conc: 75.24 ng/ml

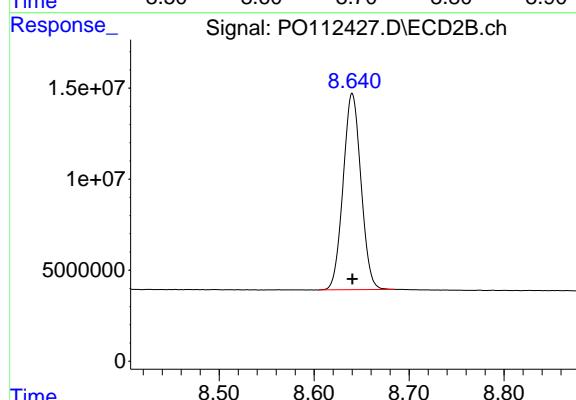





#2 Decachlorobiphenyl

R.T.: 8.640 min

Delta R.T.: 0.000 min

Response: 140886142

Conc: 74.73 ng/ml

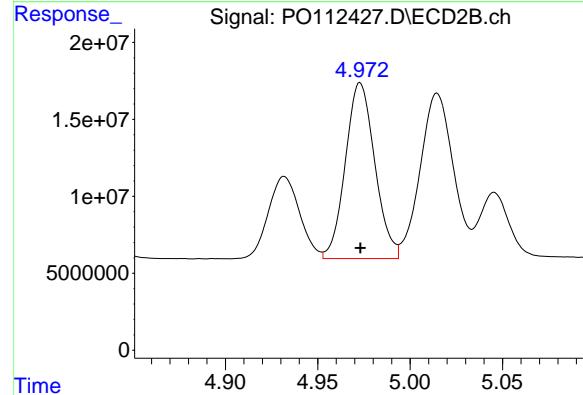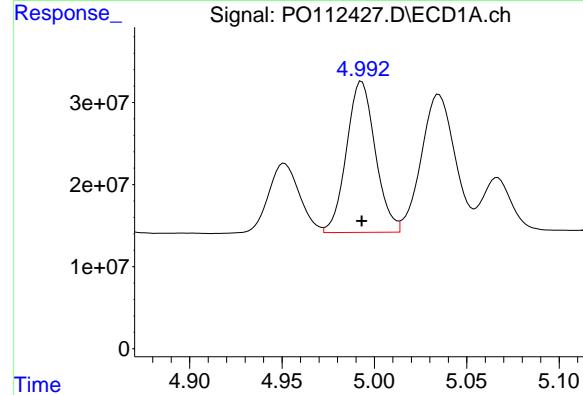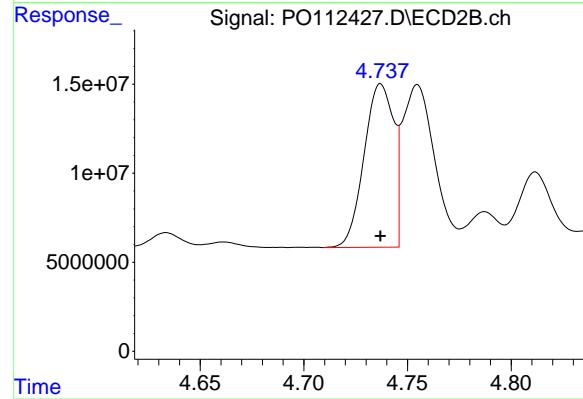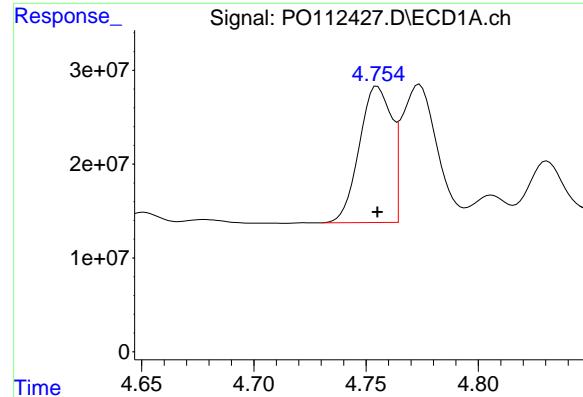

#21 AR-1248-1

R.T.: 4.755 min
 Delta R.T.: 0.000 min
 Response: 145054784
 Conc: 748.88 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750

#21 AR-1248-1


R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 91310177
 Conc: 749.71 ng/ml

#22 AR-1248-2

R.T.: 4.993 min
 Delta R.T.: 0.000 min
 Response: 199514924
 Conc: 754.17 ng/ml

#22 AR-1248-2

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 126679146
 Conc: 750.31 ng/ml

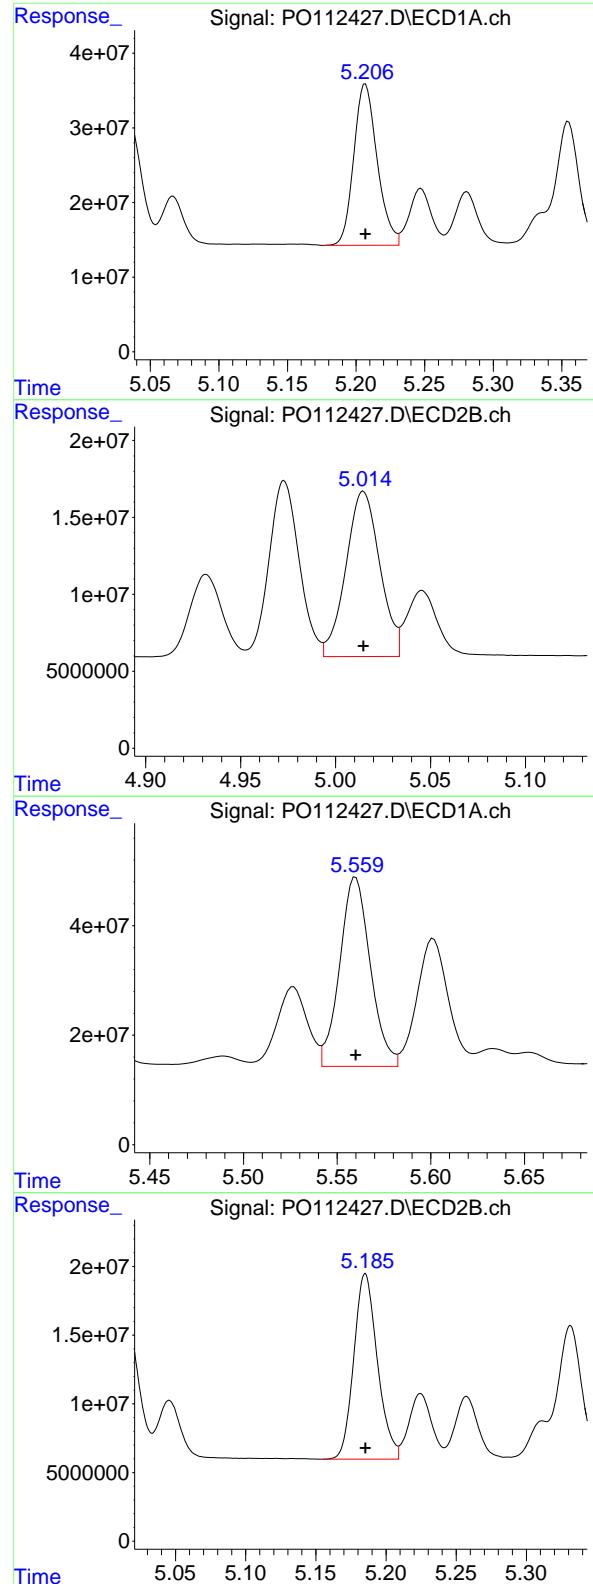

#23 AR-1248-3

R.T.: 5.207 min
 Delta R.T.: 0.000 min
 Response: 257015325
 Conc: 753.76 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750

#23 AR-1248-3

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 133665549
 Conc: 751.76 ng/ml

#24 AR-1248-4

R.T.: 5.560 min
 Delta R.T.: 0.000 min
 Response: 392676413
 Conc: 751.64 ng/ml


#24 AR-1248-4

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 157984016
 Conc: 749.63 ng/ml

#25 AR-1248-5

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 272446433
Conc: 753.93 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC750

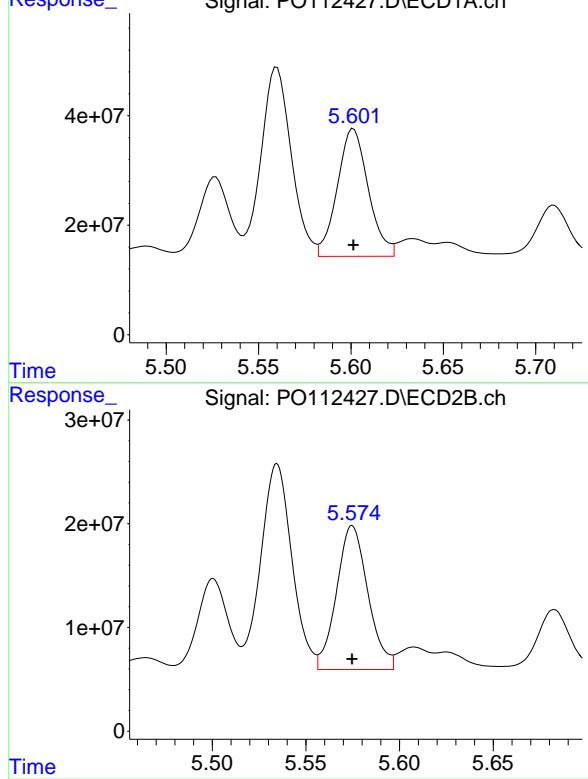

#25 AR-1248-5

R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 162089416
Conc: 747.33 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:48
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:39:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.668 | 3.662 | 463.7E6 | 277.9E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.692 | 8.640 | 409.8E6 | 97058226 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 21) L5 AR-1248-1 | 4.754 | 4.737 | 99182020 | 63417693 | 500.000 | 500.000 |
| 22) L5 AR-1248-2 | 4.992 | 4.973 | 135.3E6 | 87923157 | 500.000 | 500.000 |
| 23) L5 AR-1248-3 | 5.205 | 5.015 | 175.2E6 | 92259912 | 500.000 | 500.000 |
| 24) L5 AR-1248-4 | 5.559 | 5.185 | 270.3E6 | 109.6E6 | 500.000 | 500.000 |
| 25) L5 AR-1248-5 | 5.599 | 5.575 | 187.2E6 | 113.7E6 | 500.000 | 500.000 |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 15:48
 Operator : YP/AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:39:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

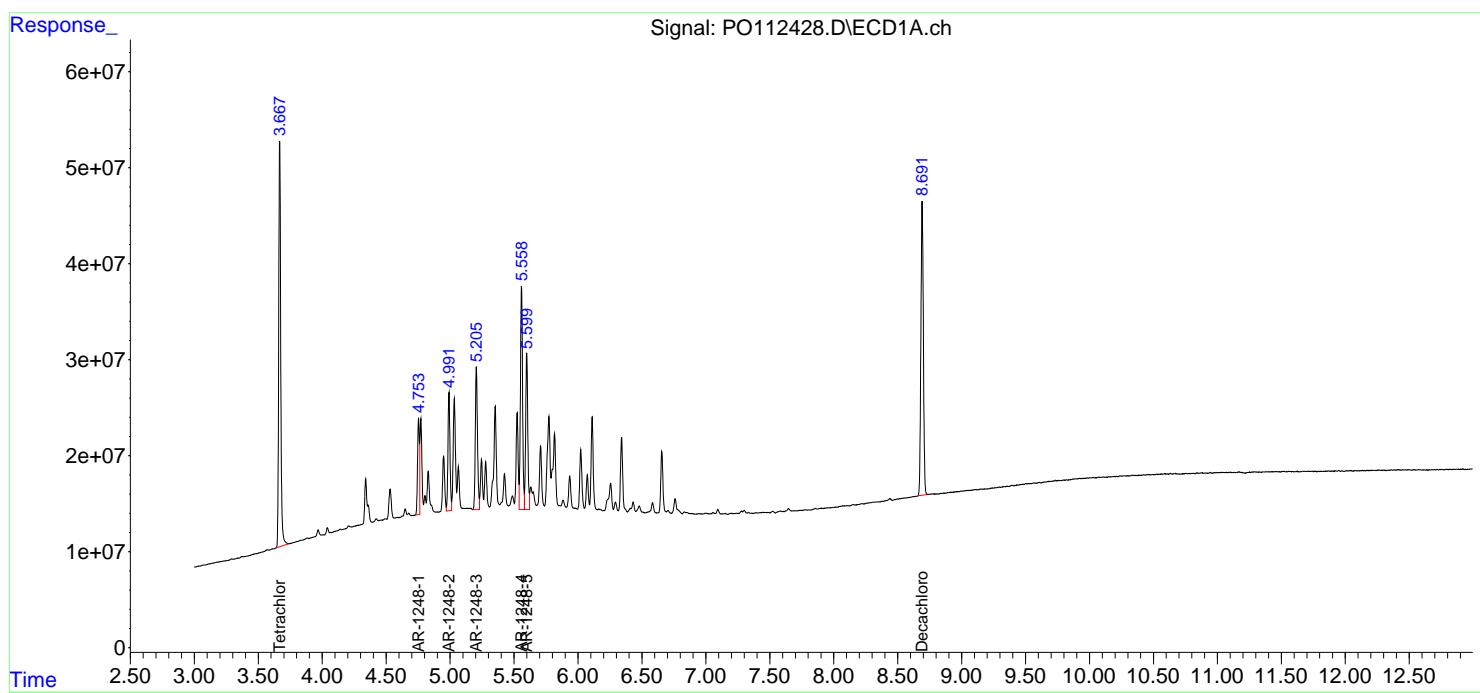

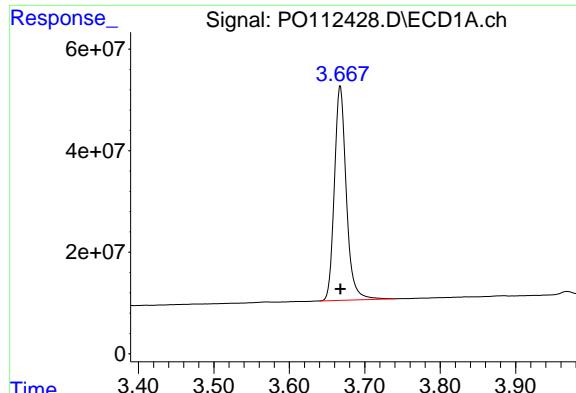

#1 Tetrachloro-m-xylene


R.T.: 3.668 min

Delta R.T.: 0.000 min

Instrument: ECD_O

Response: 463659312

Conc: 50.00 ng/ml

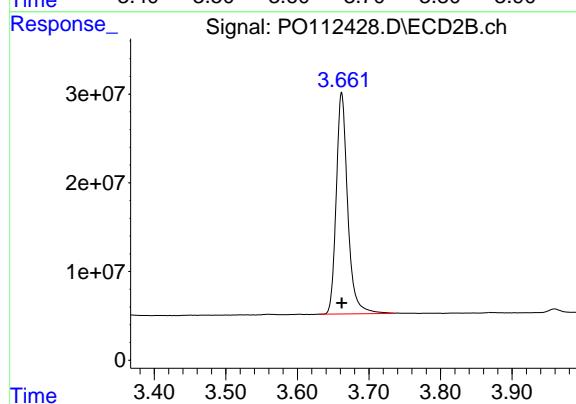


#1 Tetrachloro-m-xylene

R.T.: 3.662 min

Delta R.T.: 0.000 min

Response: 277901821

Conc: 50.00 ng/ml

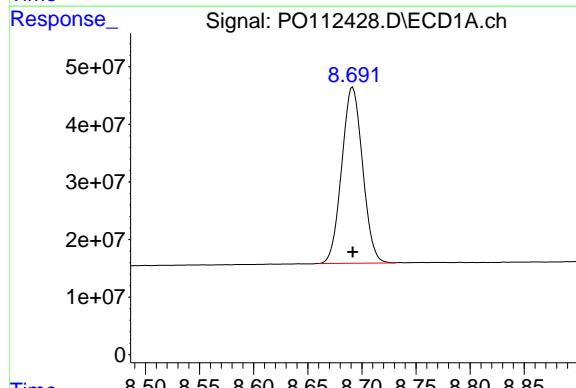


#2 Decachlorobiphenyl

R.T.: 8.692 min

Delta R.T.: 0.000 min

Response: 409758552

Conc: 50.00 ng/ml

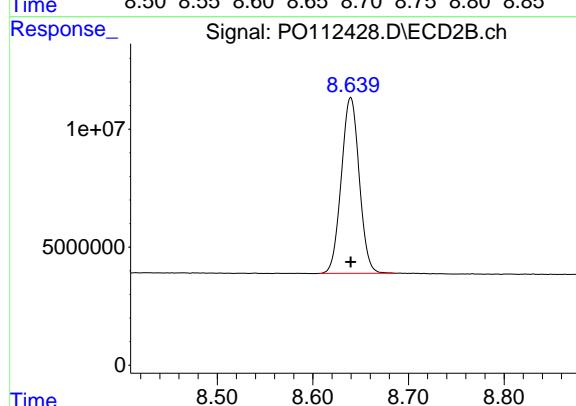

#2 Decachlorobiphenyl

R.T.: 8.640 min

Delta R.T.: 0.000 min


Response: 97058226

Conc: 50.00 ng/ml

#21 AR-1248-1


R.T.: 4.754 min
 Delta R.T.: 0.000 min
 Response: 99182020
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC500




#21 AR-1248-1

R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 63417693
 Conc: 500.00 ng/ml

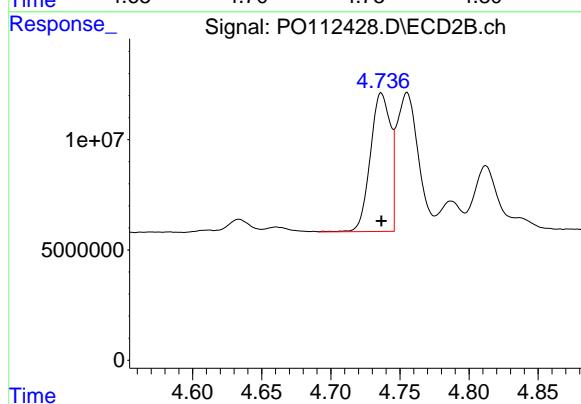


#22 AR-1248-2


R.T.: 4.992 min
 Delta R.T.: 0.000 min
 Response: 135286464
 Conc: 500.00 ng/ml

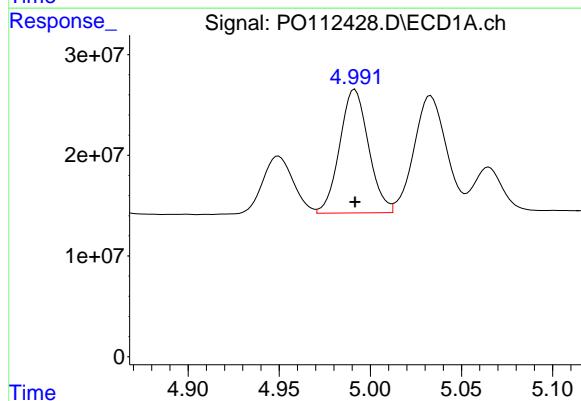

#22 AR-1248-2

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 87923157
 Conc: 500.00 ng/ml

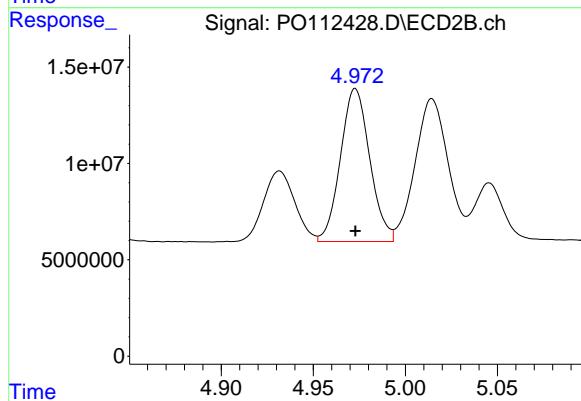

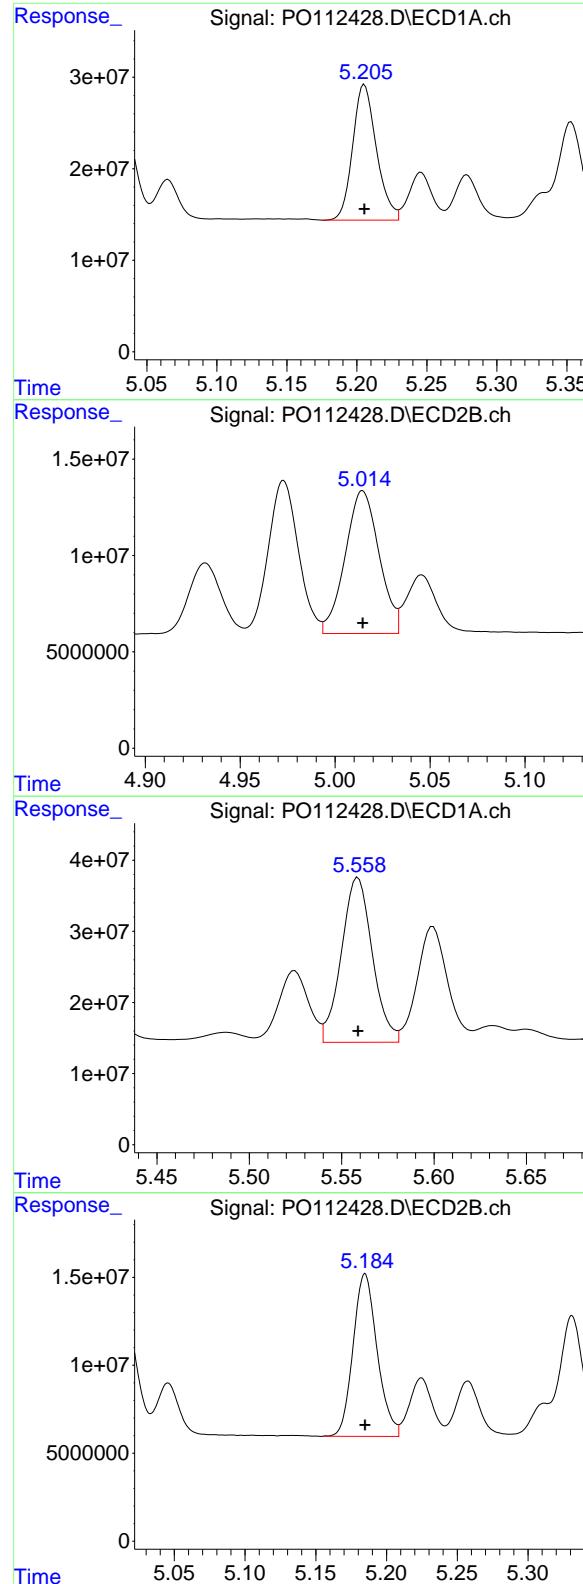

#23 AR-1248-3

R.T.: 5.205 min
 Delta R.T.: 0.000 min
 Response: 175208983
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC500

#23 AR-1248-3

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 92259912
 Conc: 500.00 ng/ml

#24 AR-1248-4

R.T.: 5.559 min
 Delta R.T.: 0.000 min
 Response: 270274803
 Conc: 500.00 ng/ml



#24 AR-1248-4

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 109571190
 Conc: 500.00 ng/ml

#25 AR-1248-5

R.T.: 5.599 min
Delta R.T.: 0.000 min
Response: 187168960
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC500

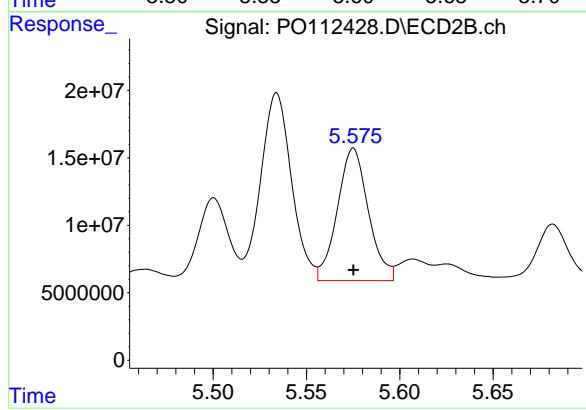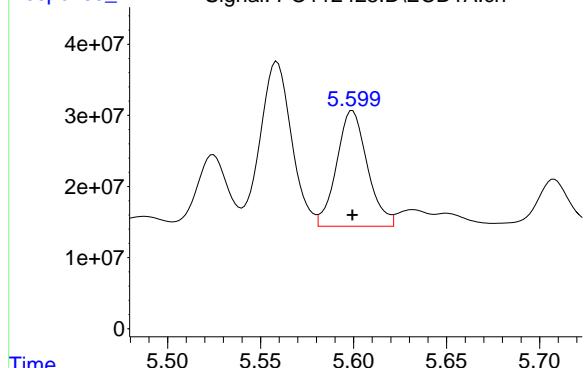

#25 AR-1248-5

R.T.: 5.575 min
Delta R.T.: 0.000 min
Response: 113716877
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:07
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:49:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 233.9E6 | 140.7E6 | 25.451 | 25.528 |
| 2) SA Decachlor... | 8.695 | 8.641 | 206.6E6 | 49551581 | 25.466 | 25.949 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 21) L5 AR-1248-1 | 4.756 | 4.738 | 50861384 | 33005549 | 259.321 | 265.423 |
| 22) L5 AR-1248-2 | 4.994 | 4.974 | 69688118 | 46341566 | 259.932 | 267.919 |
| 23) L5 AR-1248-3 | 5.208 | 5.016 | 91080155 | 48518478 | 262.621 | 266.773 |
| 24) L5 AR-1248-4 | 5.561 | 5.186 | 140.9E6 | 57393073 | 264.543 | 266.380 |
| 25) L5 AR-1248-5 | 5.602 | 5.576 | 98123360 | 60708613 | 265.809 | 271.777 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:07
 Operator : YP/AJ
 Sample : AR1248ICC250
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:49:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

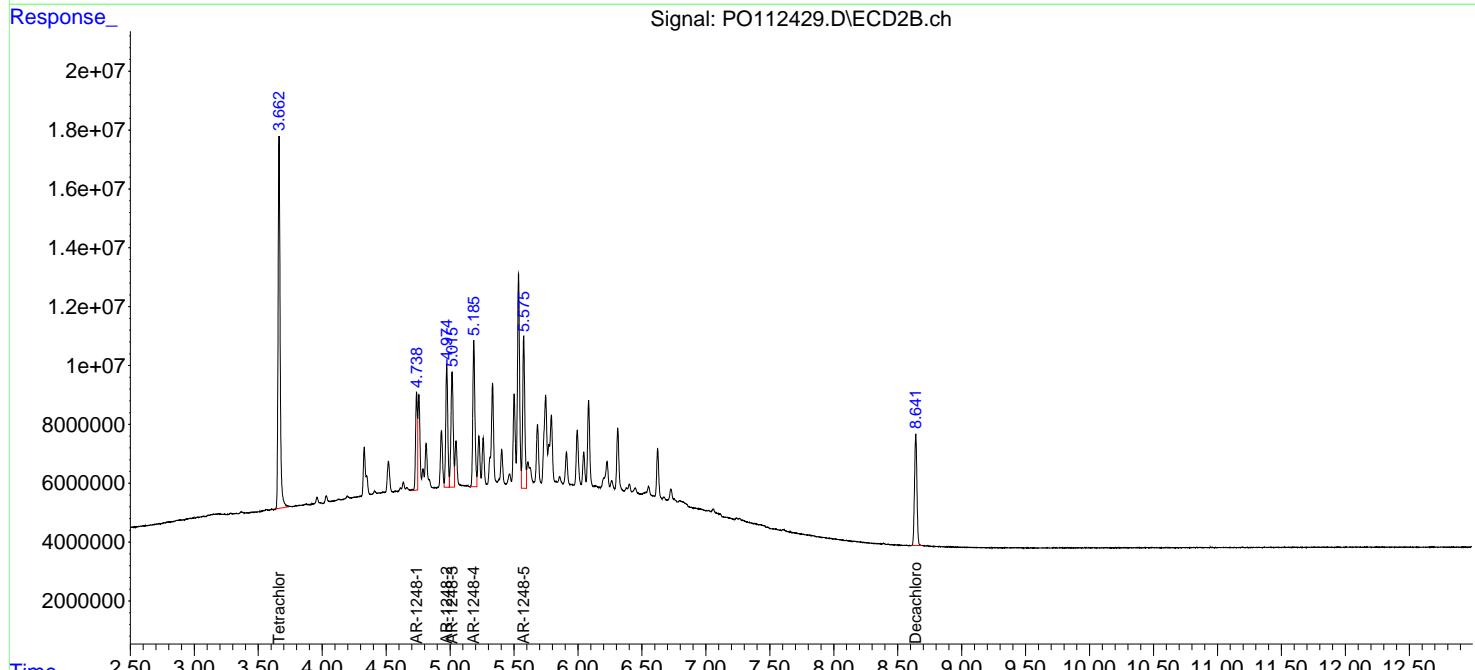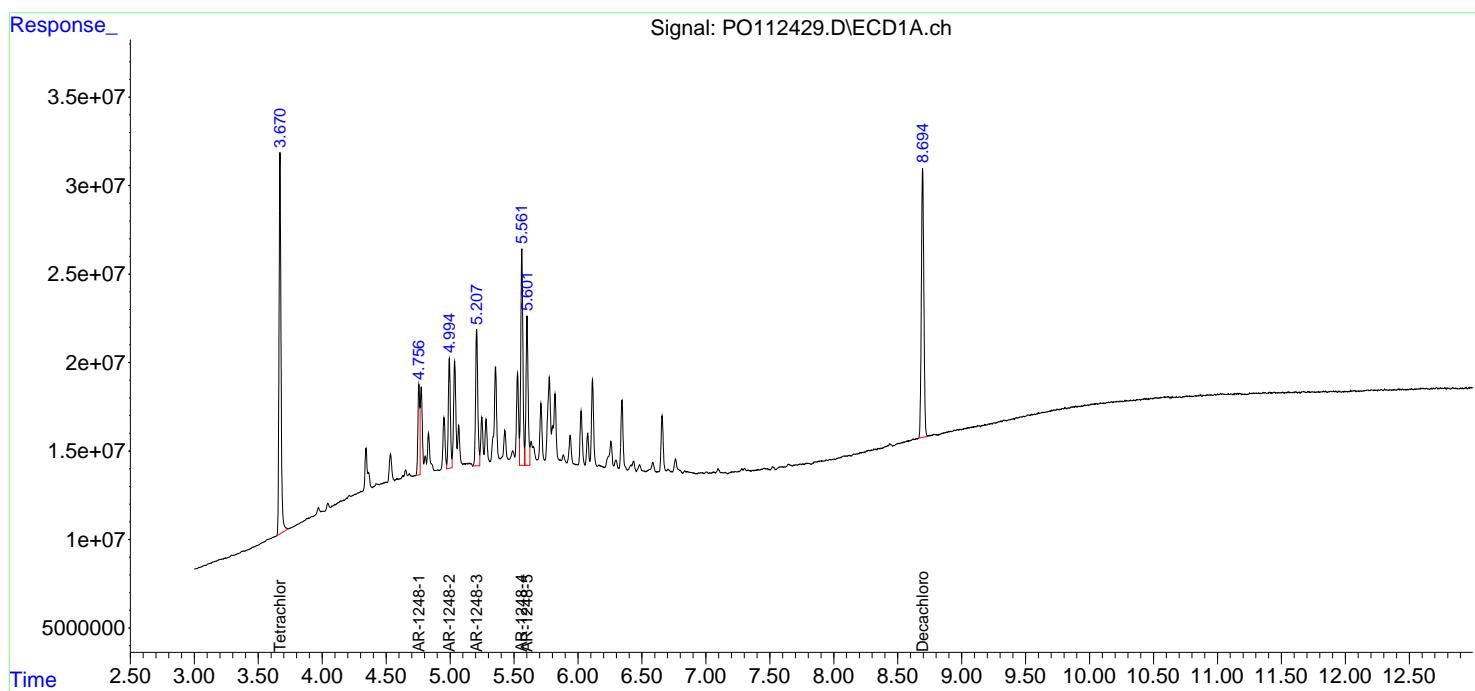

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
 Delta R.T.: 0.000 min
 Response: 233933554
 Conc: 25.45 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC250

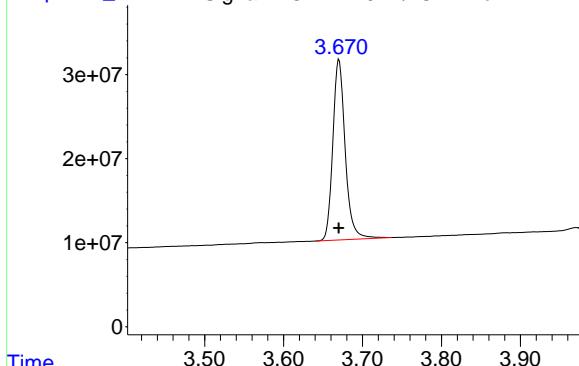


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
 Delta R.T.: 0.000 min
 Response: 140747213
 Conc: 25.53 ng/ml

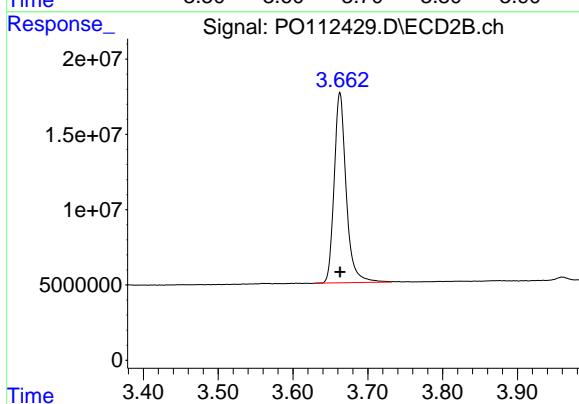


#2 Decachlorobiphenyl

R.T.: 8.695 min
 Delta R.T.: 0.000 min
 Response: 206552013
 Conc: 25.47 ng/ml

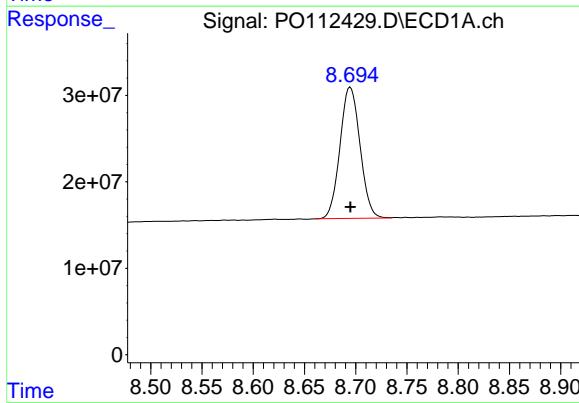

#2 Decachlorobiphenyl


R.T.: 8.641 min
 Delta R.T.: 0.000 min
 Response: 49551581
 Conc: 25.95 ng/ml

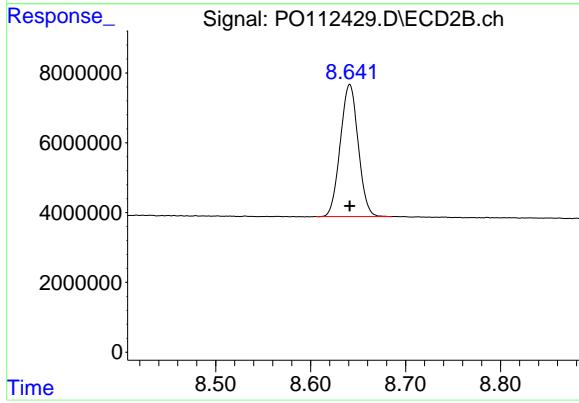

#21 AR-1248-1


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 50861384
 Conc: 259.32 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC250




#21 AR-1248-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 33005549
 Conc: 265.42 ng/ml

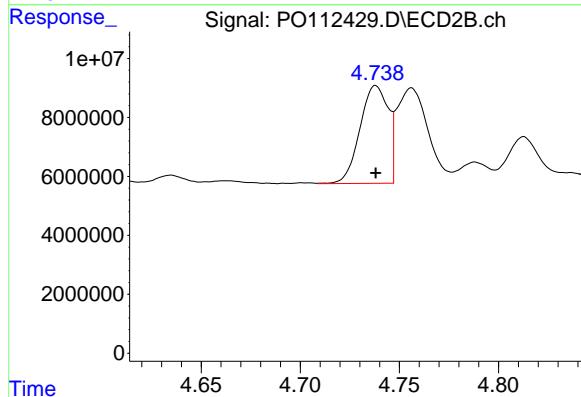


#22 AR-1248-2

R.T.: 4.994 min
 Delta R.T.: 0.000 min
 Response: 69688118
 Conc: 259.93 ng/ml

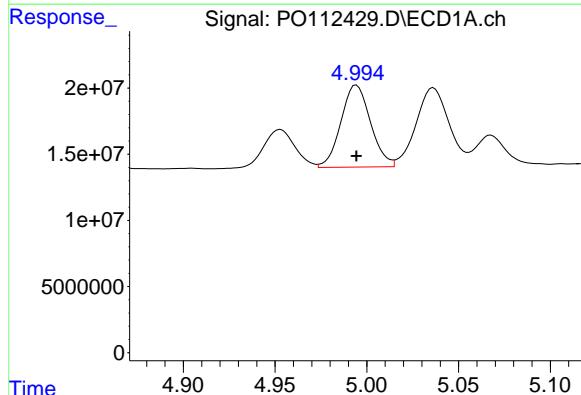

#22 AR-1248-2


R.T.: 4.974 min
 Delta R.T.: 0.000 min
 Response: 46341566
 Conc: 267.92 ng/ml

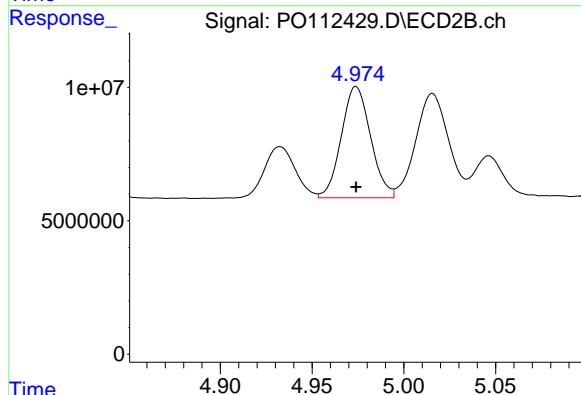

#23 AR-1248-3


R.T.: 5.208 min
 Delta R.T.: 0.000 min
 Response: 91080155
 Conc: 262.62 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC250




#23 AR-1248-3

R.T.: 5.016 min
 Delta R.T.: 0.000 min
 Response: 48518478
 Conc: 266.77 ng/ml

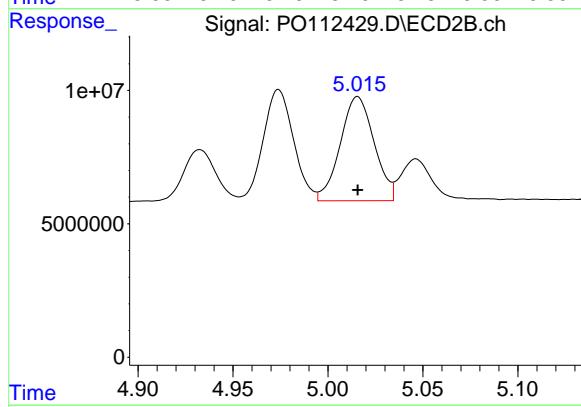


#24 AR-1248-4

R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 140936473
 Conc: 264.54 ng/ml

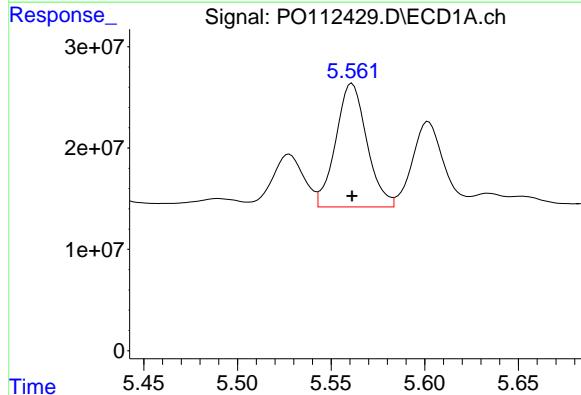

#24 AR-1248-4



R.T.: 5.186 min
 Delta R.T.: 0.000 min
 Response: 57393073
 Conc: 266.38 ng/ml

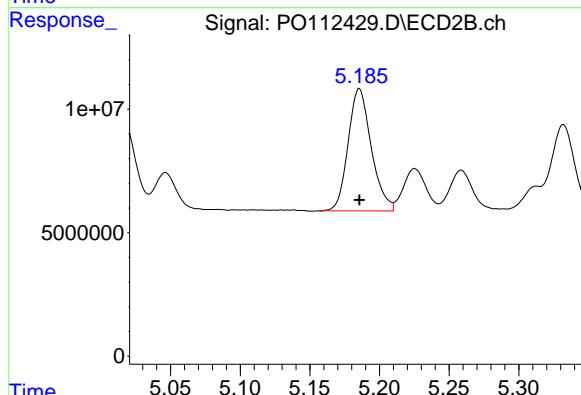

#25 AR-1248-5

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 98123360
Conc: 265.81 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC250

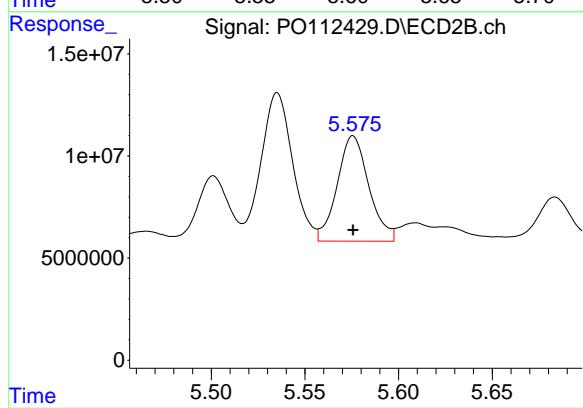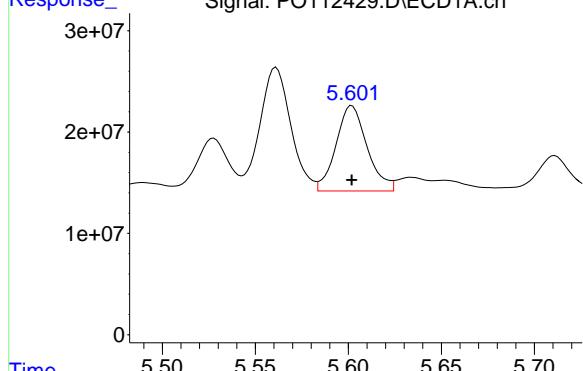

#25 AR-1248-5

R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 60708613
Conc: 271.78 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:25
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:53:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 32837807 | 20886754 | 3.789 | 3.981 |
| 2) SA Decachlor... | 8.694 | 8.641 | 30716372 | 7585110 | 3.980 | 4.142 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|---------|---------|
| 21) L5 AR-1248-1 | 4.757 | 4.738 | 7575656 | 5507226 | 40.466 | 45.323 |
| 22) L5 AR-1248-2 | 4.995 | 4.973 | 10157901 | 7726264 | 39.817 | 45.642 |
| 23) L5 AR-1248-3 | 5.208 | 5.015 | 16562795 | 8037448 | 48.190 | 45.244 |
| 24) L5 AR-1248-4 | 5.561 | 5.185 | 20468723 | 8997535 | 40.302m | 43.063m |
| 25) L5 AR-1248-5 | 5.602 | 5.575 | 13567669 | 9015964 | 38.853m | 41.910m |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:25
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1



Instrument :
 ECD_O
 ClientSampleId :
 AR1248ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:53:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

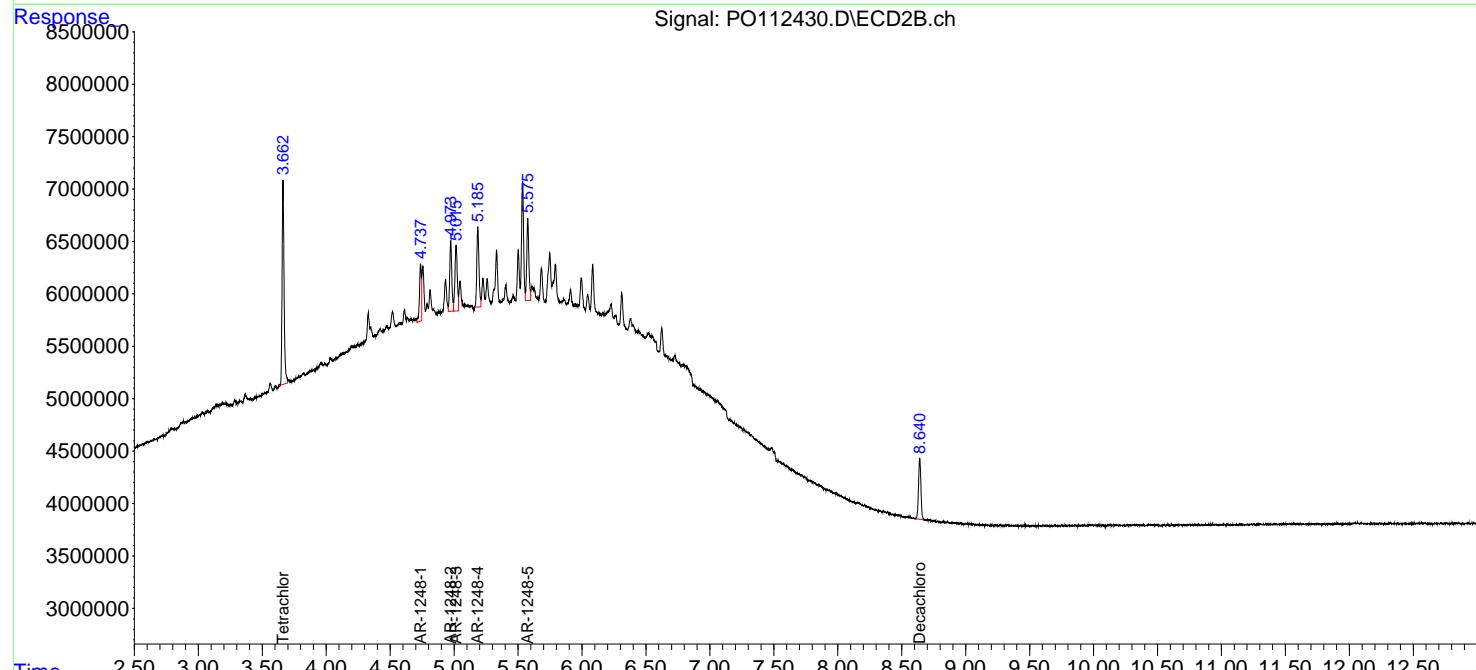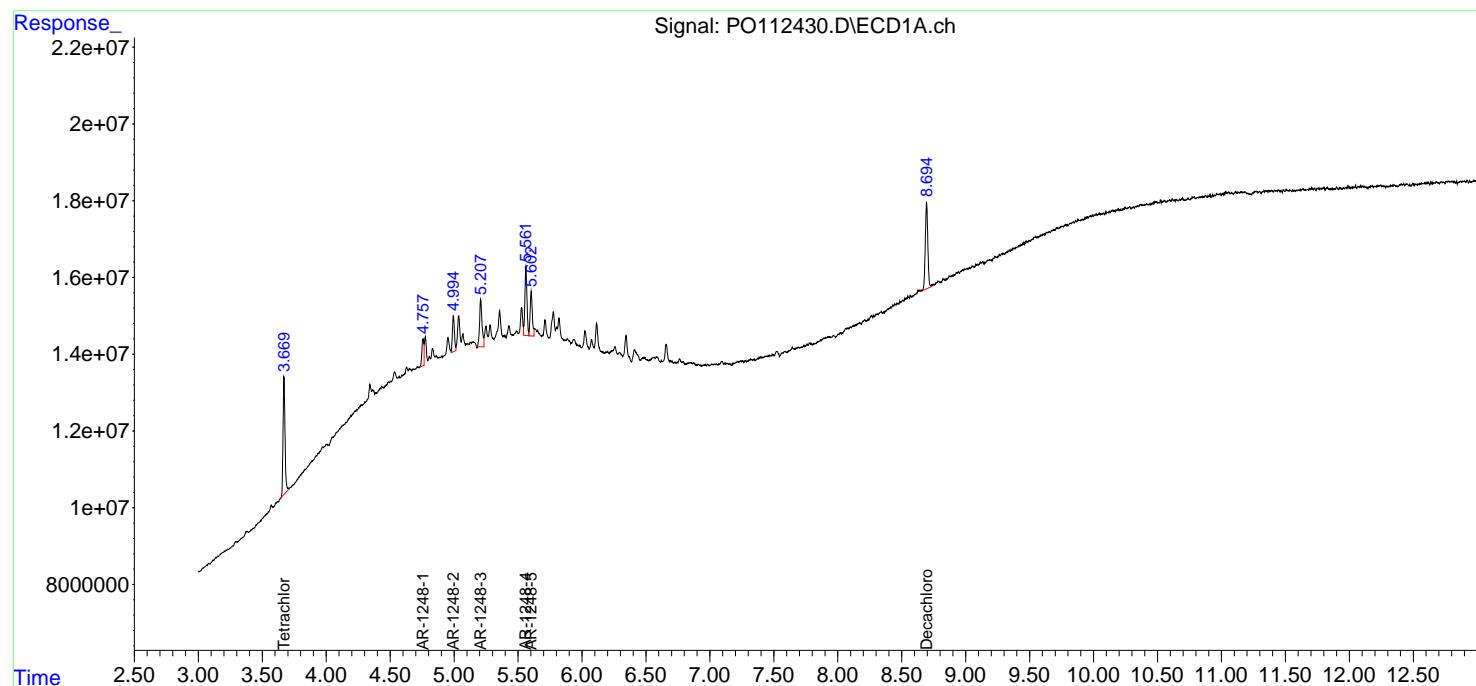

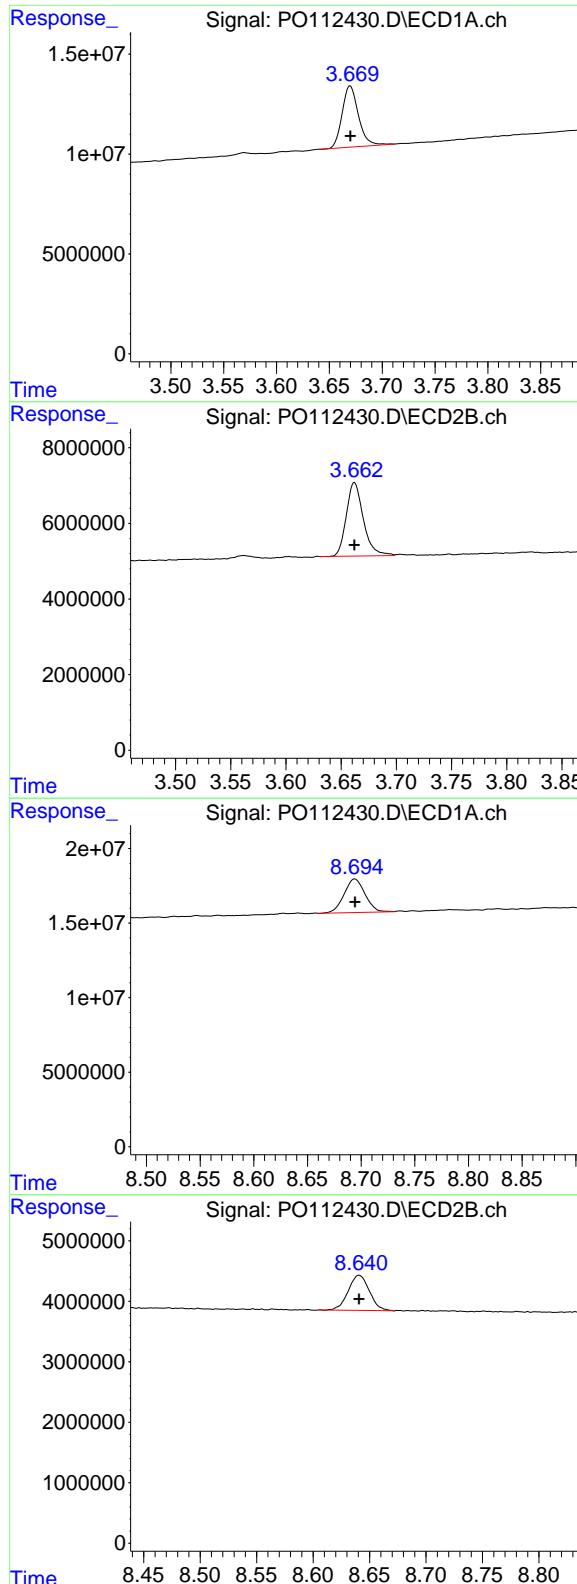

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 32837807
Conc: 3.79 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

#1 Tetrachloro-m-xylene





R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 20886754
Conc: 3.98 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 30716372
Conc: 3.98 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 7585110
Conc: 4.14 ng/ml

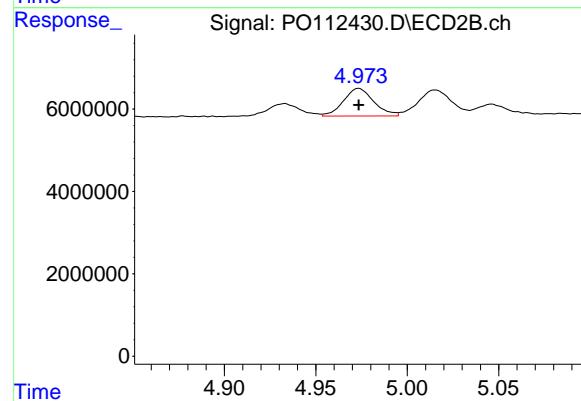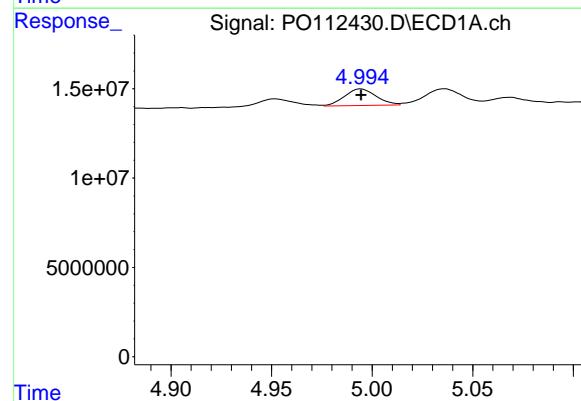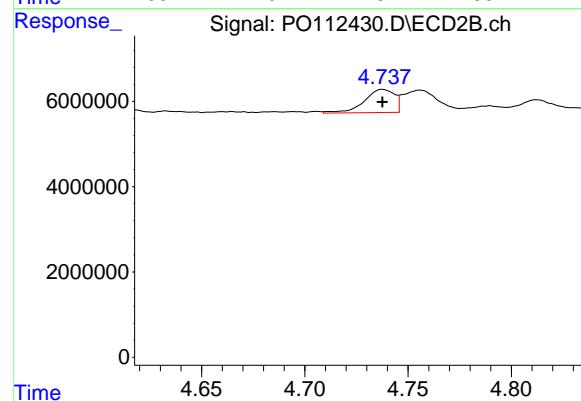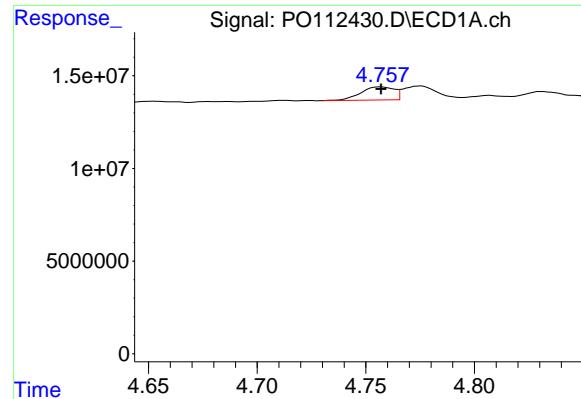



#21 AR-1248-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 7575656
 Conc: 40.47 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

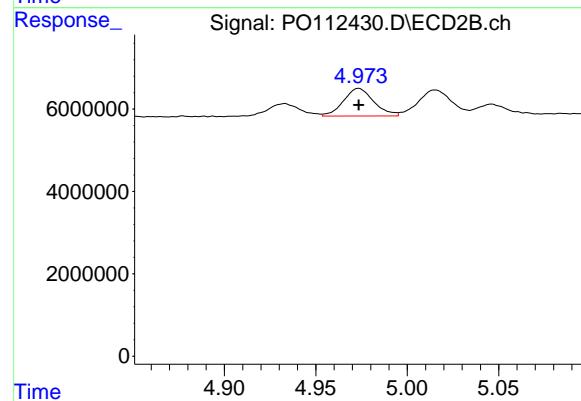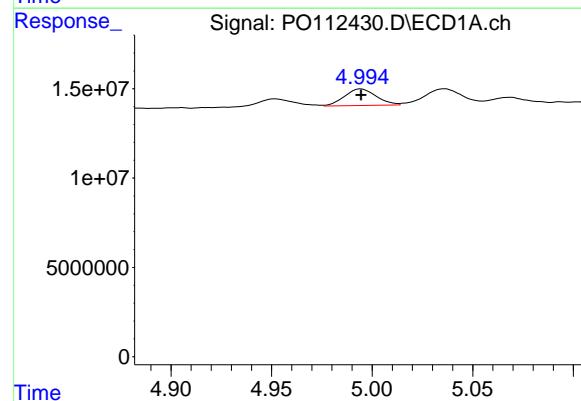

#21 AR-1248-1





R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 5507226
 Conc: 45.32 ng/ml

#22 AR-1248-2

R.T.: 4.995 min
 Delta R.T.: 0.000 min
 Response: 10157901
 Conc: 39.82 ng/ml

#22 AR-1248-2

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 7726264
 Conc: 45.64 ng/ml

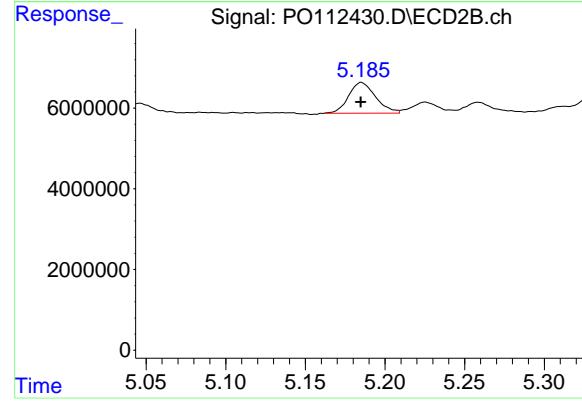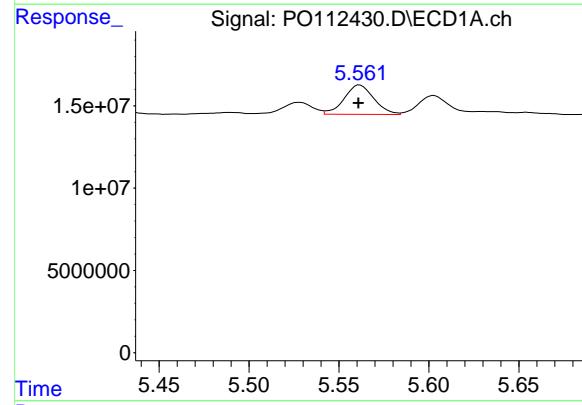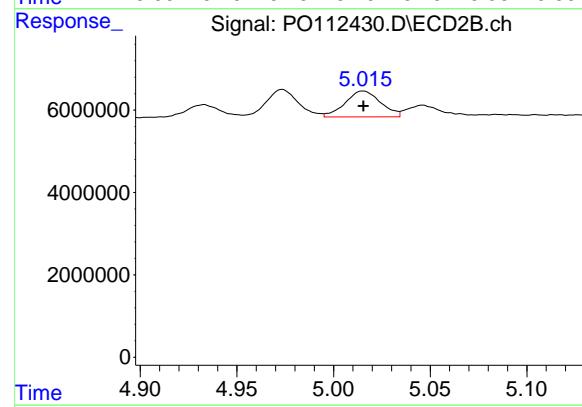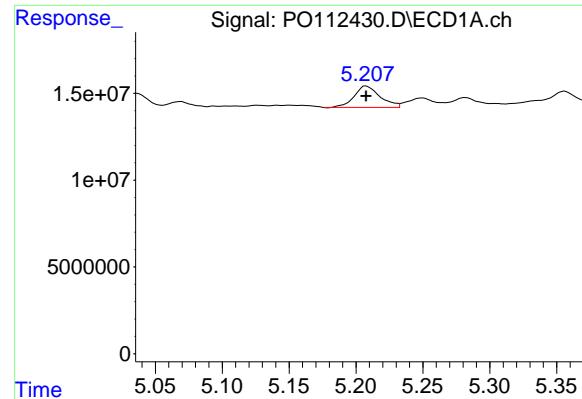

#23 AR-1248-3

R.T.: 5.208 min
 Delta R.T.: 0.000 min
 Response: 16562795
 Conc: 48.19 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#23 AR-1248-3

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 8037448
 Conc: 45.24 ng/ml

#24 AR-1248-4

R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 20468723
 Conc: 40.30 ng/ml

#24 AR-1248-4

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 8997535
 Conc: 43.06 ng/ml



#25 AR-1248-5

R.T.: 5.602 min
 Delta R.T.: 0.000 min
 Response: 13567669
 Conc: 38.85 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

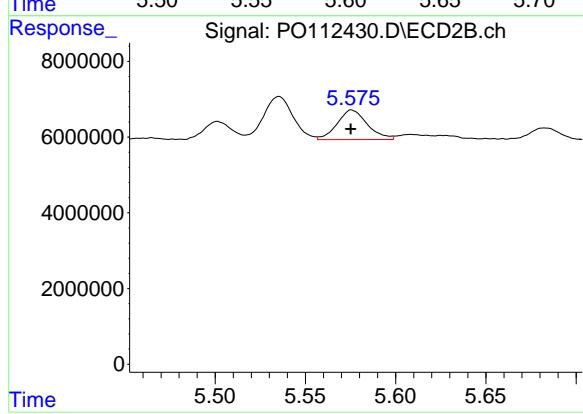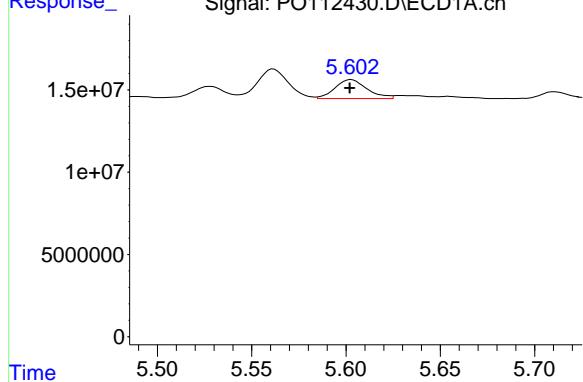

#25 AR-1248-5

R.T.: 5.575 min
 Delta R.T.: 0.000 min
 Response: 9015964
 Conc: 41.91 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:44
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:03:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 847.8E6 | 513.5E6 | 96.903 | 97.307 |
| 2) SA Decachlor... | 8.694 | 8.640 | 781.1E6 | 179.4E6 | 98.068 | 96.847 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|---------|---------|---------|
| 26) L6 AR-1254-1 | 5.561 | 5.535 | 525.2E6 | 308.1E6 | 960.812 | 951.975 |
| 27) L6 AR-1254-2 | 5.710 | 5.682 | 467.4E6 | 269.6E6 | 964.863 | 954.131 |
| 28) L6 AR-1254-3 | 6.114 | 6.083 | 736.7E6 | 411.6E6 | 972.647 | 961.979 |
| 29) L6 AR-1254-4 | 6.343 | 6.311 | 537.3E6 | 257.0E6 | 969.374 | 958.799 |
| 30) L6 AR-1254-5 | 6.762 | 6.727 | 713.2E6 | 324.9E6 | 982.240 | 968.098 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112431.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:44
 Operator : YP/AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:03:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

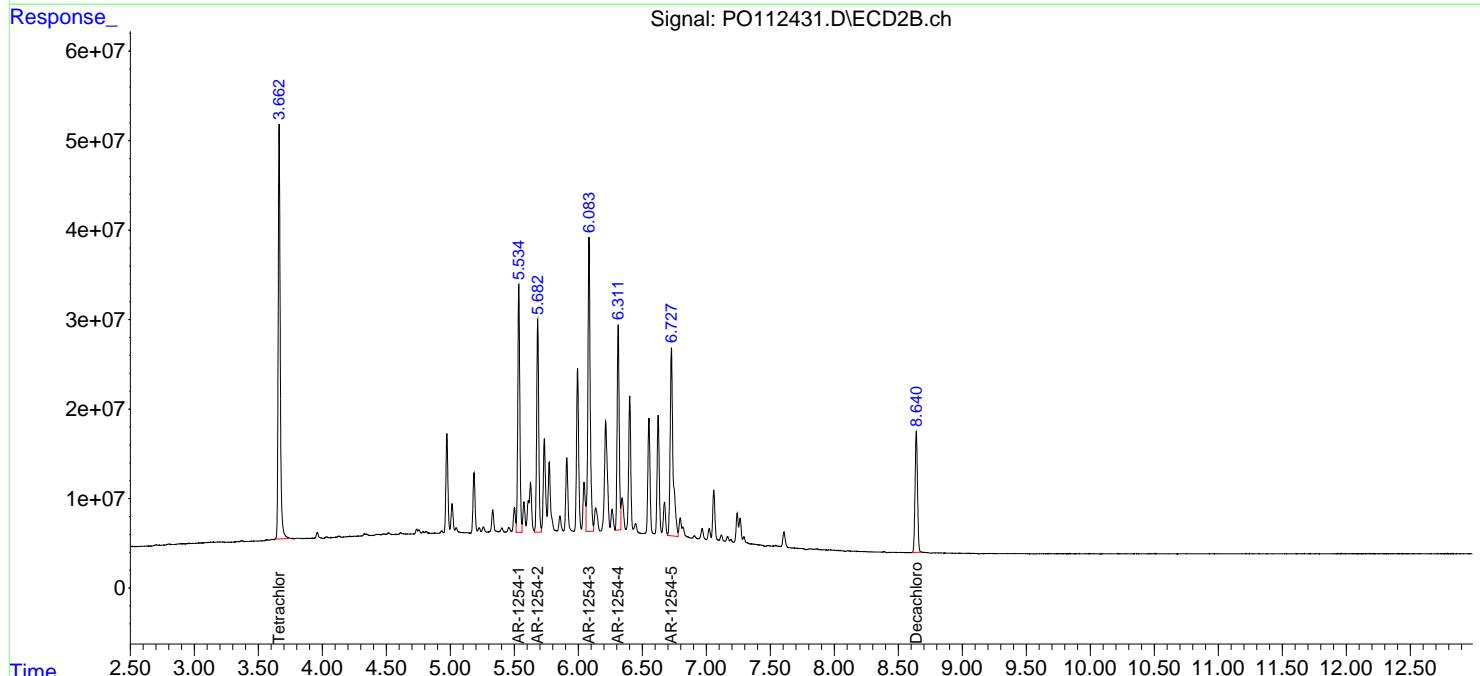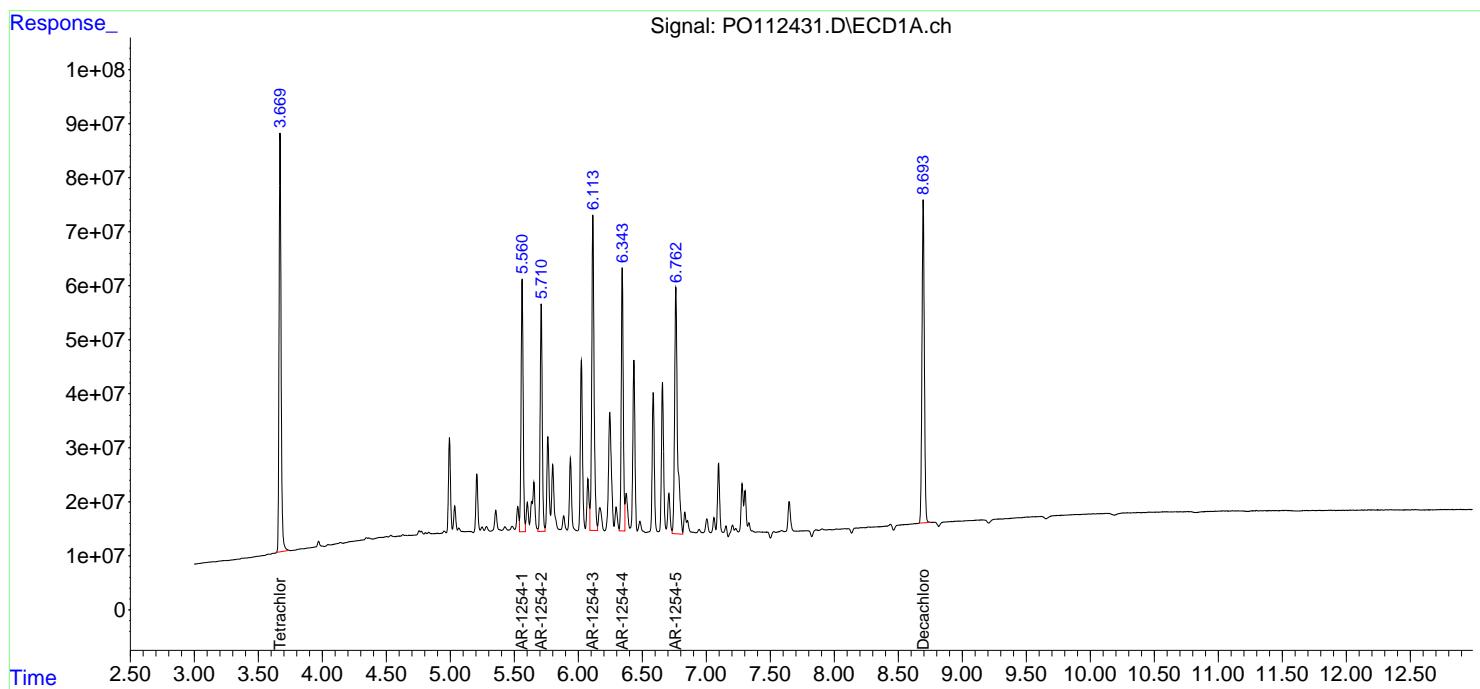

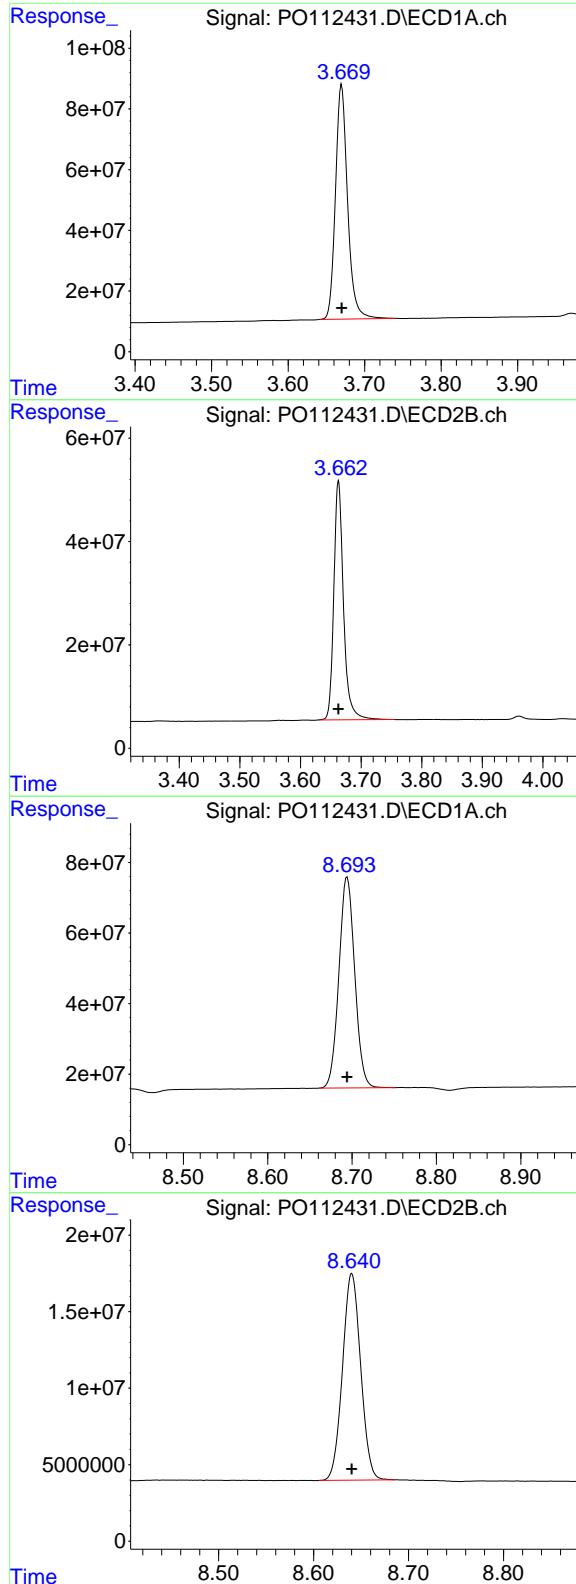

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: 0.000 min
 Response: 847789375
 Conc: 96.90 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1254ICC1000

#1 Tetrachloro-m-xylene

R.T.: 3.663 min
 Delta R.T.: 0.000 min
 Response: 513532188
 Conc: 97.31 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
 Delta R.T.: 0.000 min
 Response: 781064411
 Conc: 98.07 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.640 min
 Delta R.T.: 0.000 min
 Response: 179406564
 Conc: 96.85 ng/ml

#26 AR-1254-1


R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 525205609
 Conc: 960.81 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

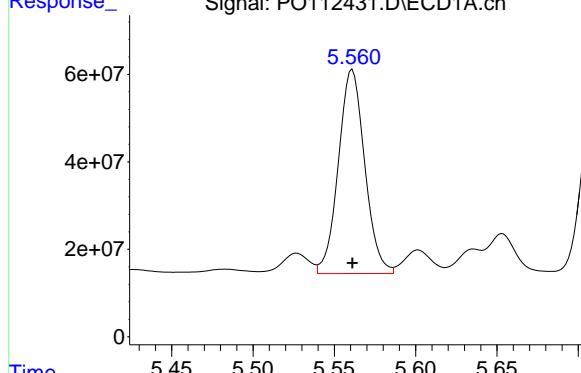


#26 AR-1254-1

R.T.: 5.535 min
 Delta R.T.: 0.000 min
 Response: 308086628
 Conc: 951.98 ng/ml

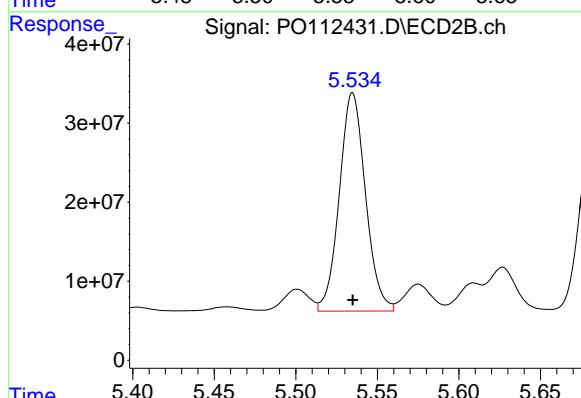


#27 AR-1254-2





R.T.: 5.710 min
 Delta R.T.: 0.000 min
 Response: 467389736
 Conc: 964.86 ng/ml

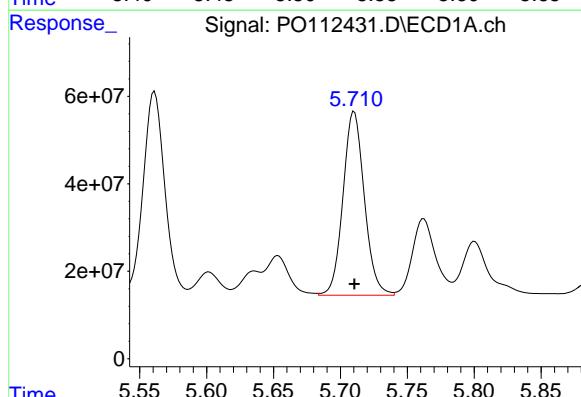

#27 AR-1254-2

R.T.: 5.682 min
 Delta R.T.: 0.000 min
 Response: 269579969
 Conc: 954.13 ng/ml

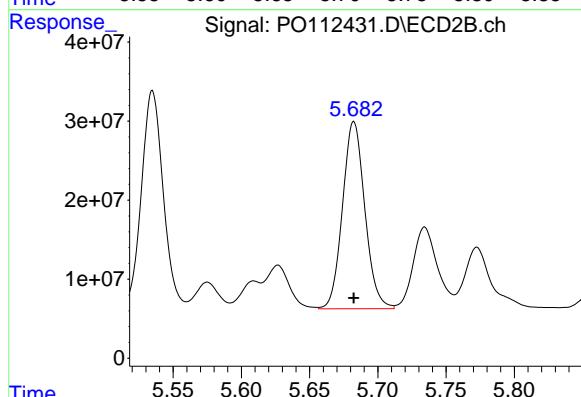

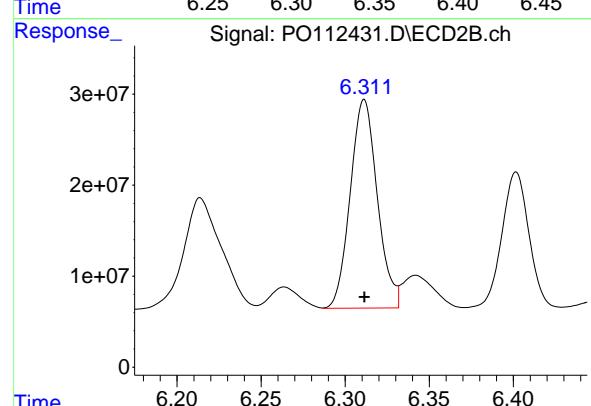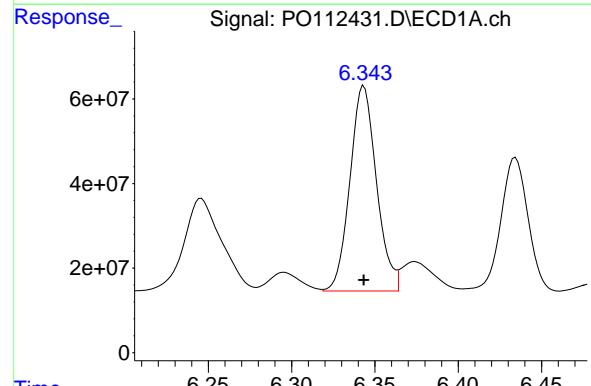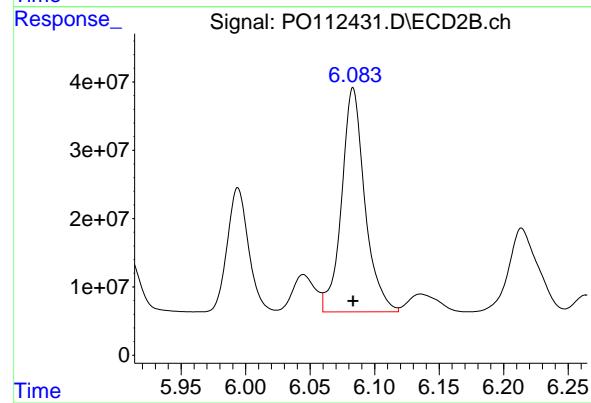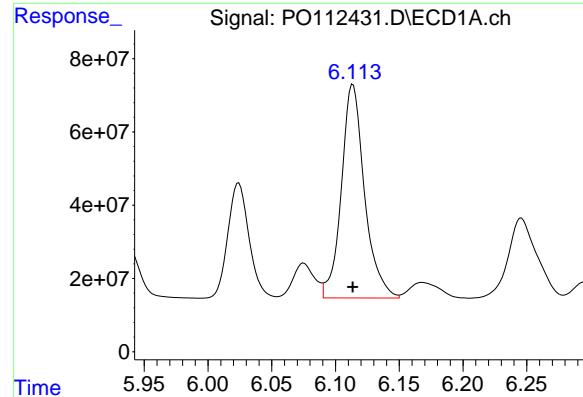

#28 AR-1254-3

R.T.: 6.114 min
 Delta R.T.: 0.000 min
 Response: 736681841
 Conc: 972.65 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

#28 AR-1254-3

R.T.: 6.083 min
 Delta R.T.: 0.000 min
 Response: 411643535
 Conc: 961.98 ng/ml

#29 AR-1254-4

R.T.: 6.343 min
 Delta R.T.: 0.000 min
 Response: 537295054
 Conc: 969.37 ng/ml



#29 AR-1254-4

R.T.: 6.311 min
 Delta R.T.: 0.000 min
 Response: 256982627
 Conc: 958.80 ng/ml

#30 AR-1254-5

R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 713157717
Conc: 982.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC1000

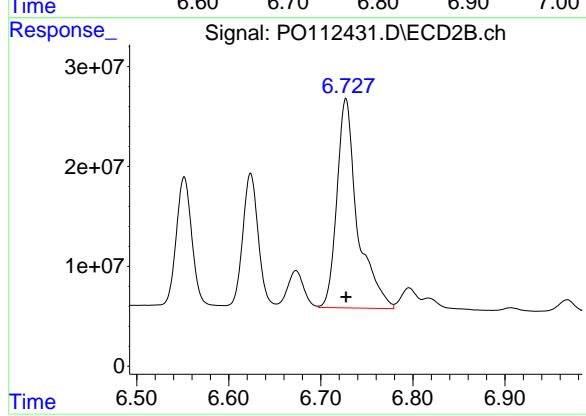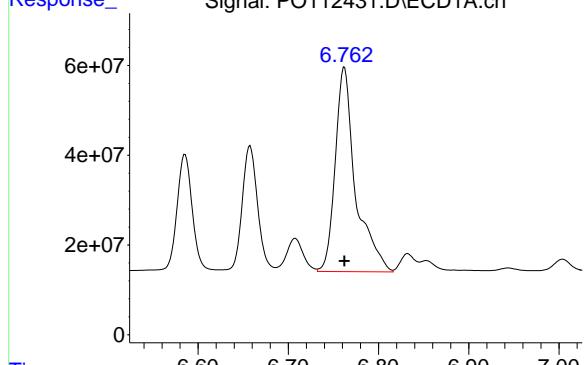

#30 AR-1254-5

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 324913084
Conc: 968.10 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:02
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:06:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 669.7E6 | 400.5E6 | 76.021 | 75.593 |
| 2) SA Decachlor... | 8.694 | 8.640 | 599.1E6 | 140.4E6 | 75.148 | 75.529 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|---------|---------|---------|
| 26) L6 AR-1254-1 | 5.561 | 5.535 | 413.9E6 | 243.4E6 | 754.780 | 751.497 |
| 27) L6 AR-1254-2 | 5.710 | 5.683 | 367.7E6 | 212.6E6 | 756.007 | 751.562 |
| 28) L6 AR-1254-3 | 6.113 | 6.084 | 574.0E6 | 320.7E6 | 755.243 | 749.688 |
| 29) L6 AR-1254-4 | 6.343 | 6.311 | 420.4E6 | 202.4E6 | 755.625 | 753.323 |
| 30) L6 AR-1254-5 | 6.762 | 6.728 | 547.0E6 | 250.4E6 | 752.271 | 747.398 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:02
 Operator : YP/AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:06:16 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

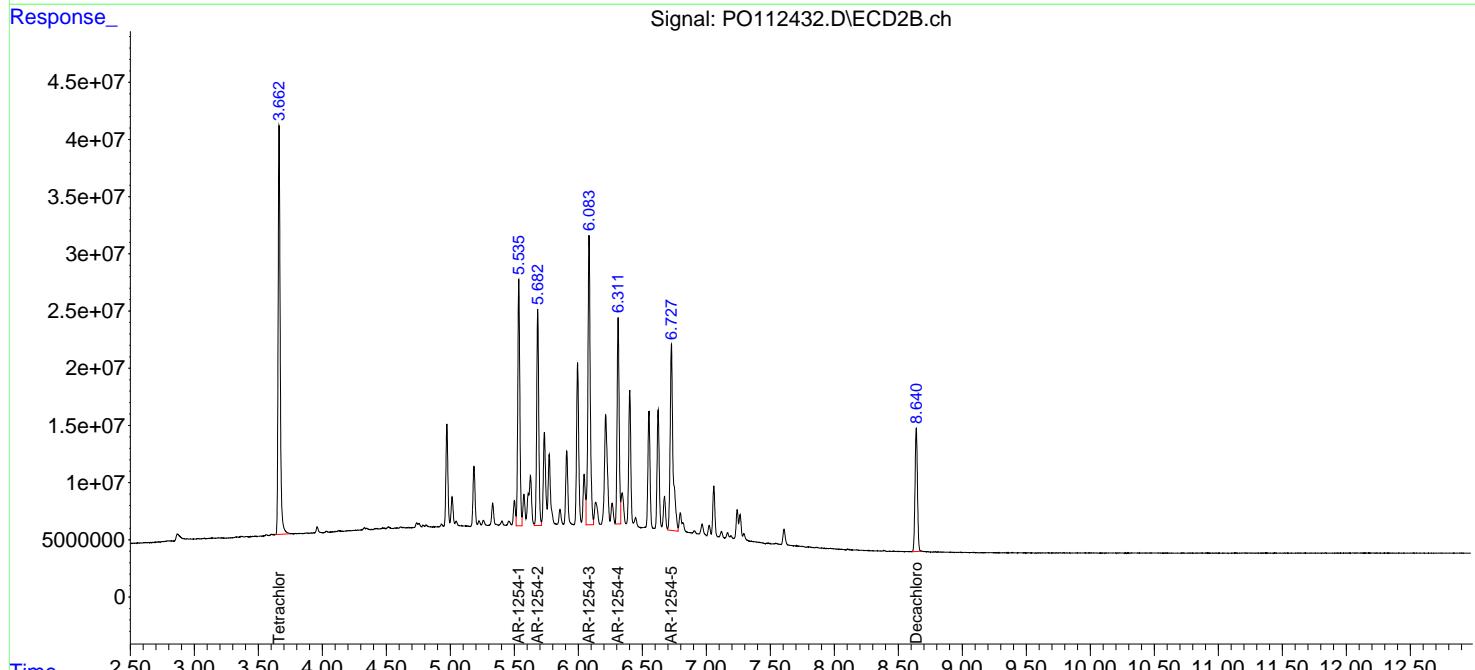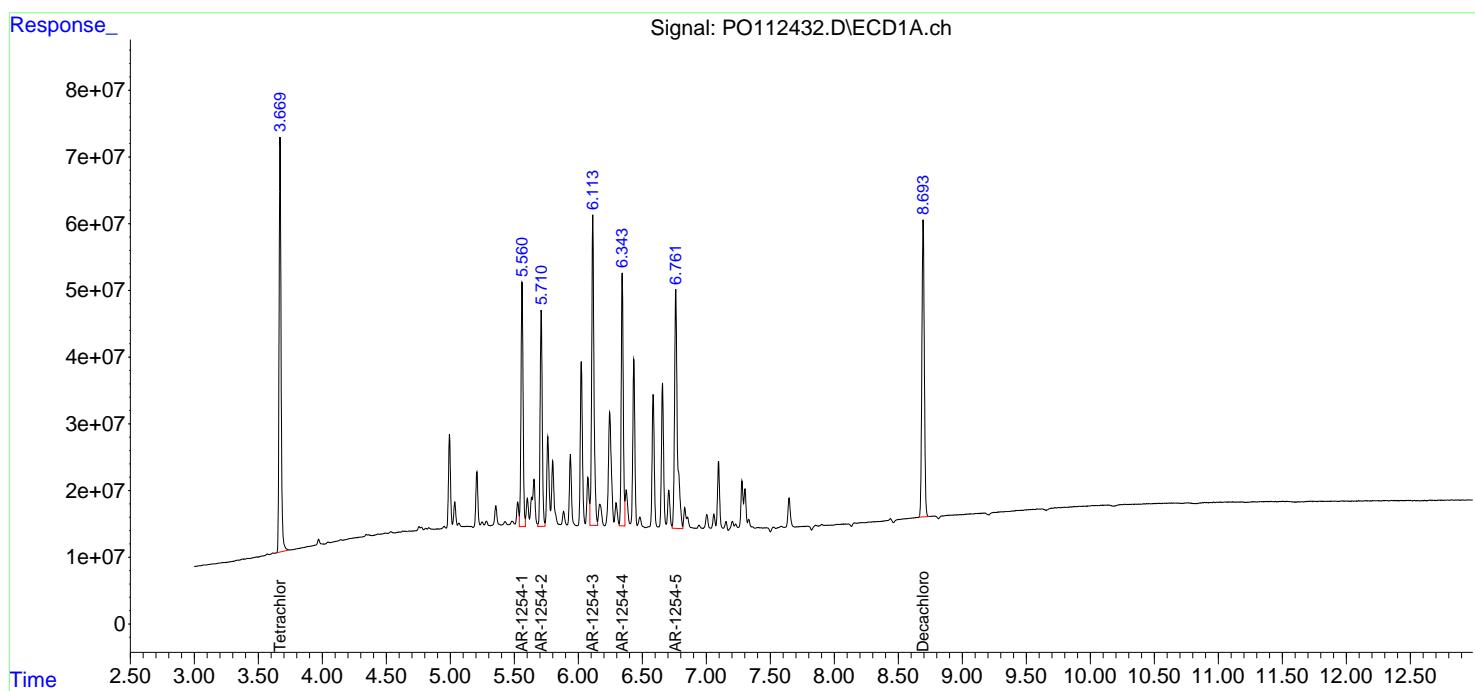

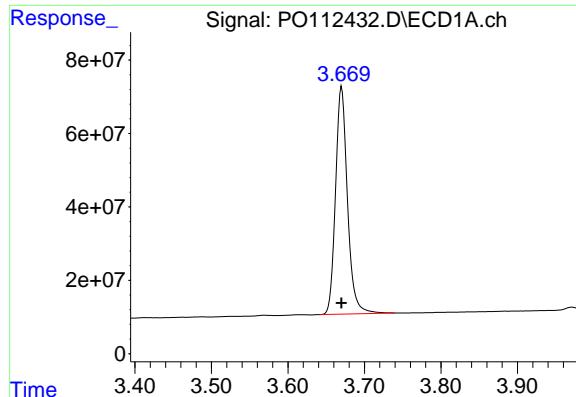

#1 Tetrachloro-m-xylene


R.T.: 3.670 min

Delta R.T.: 0.000 min

Instrument: ECD_O

Response: 669659889

Conc: 76.02 ng/ml

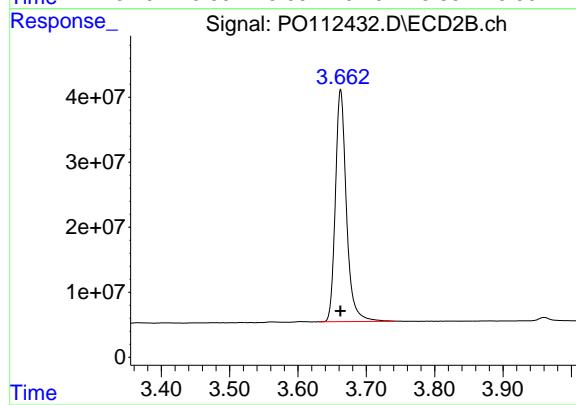


#1 Tetrachloro-m-xylene

R.T.: 3.662 min

Delta R.T.: 0.000 min

Response: 400524295

Conc: 75.59 ng/ml

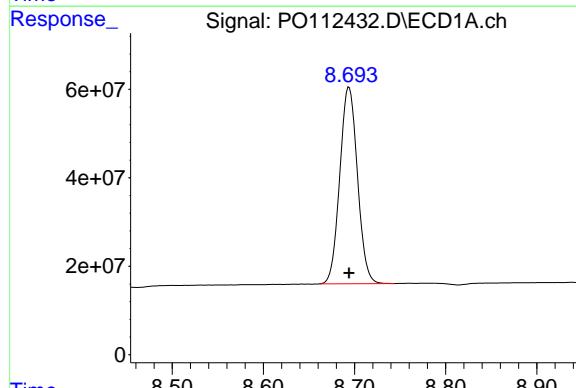


#2 Decachlorobiphenyl

R.T.: 8.694 min

Delta R.T.: 0.000 min

Response: 599111899

Conc: 75.15 ng/ml

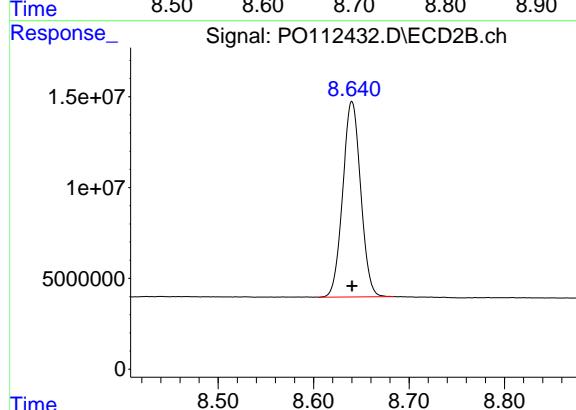


#2 Decachlorobiphenyl

R.T.: 8.640 min

Delta R.T.: 0.000 min

Response: 140411365

Conc: 75.53 ng/ml

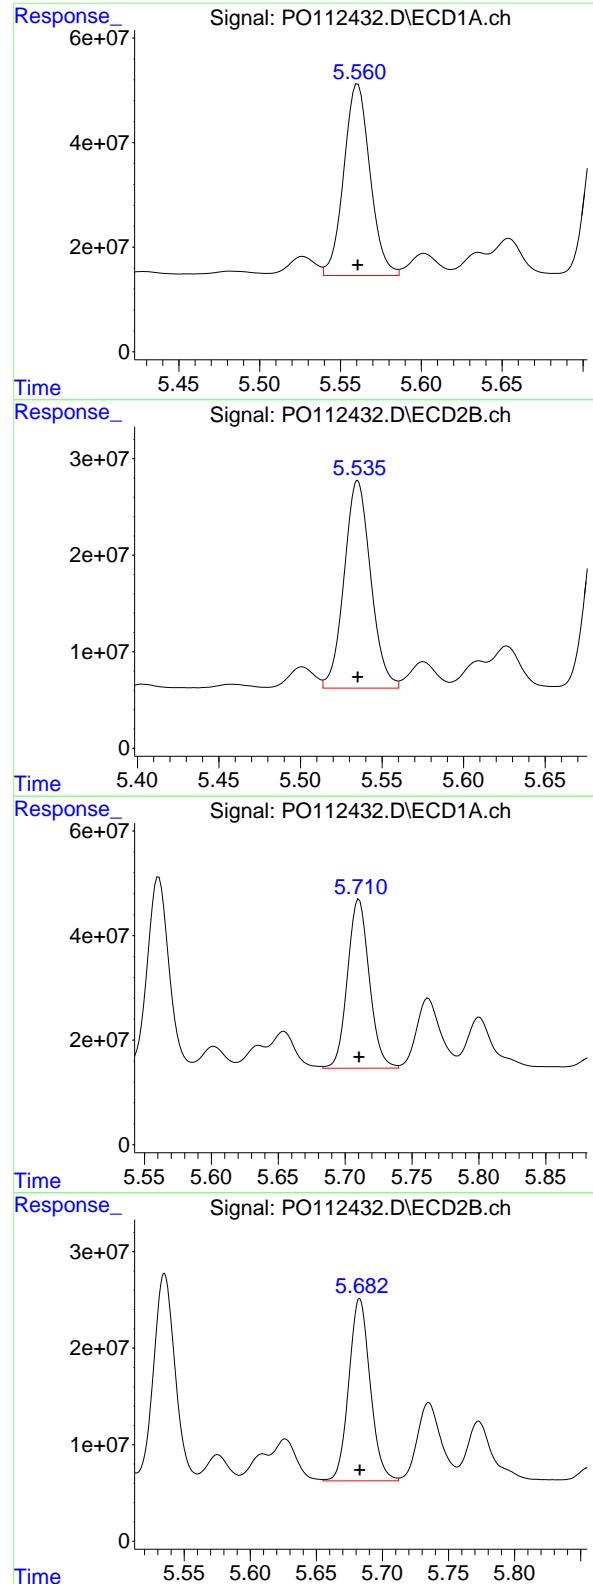

#26 AR-1254-1

R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 413902155
 Conc: 754.78 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1254ICC750

#26 AR-1254-1


R.T.: 5.535 min
 Delta R.T.: 0.000 min
 Response: 243449246
 Conc: 751.50 ng/ml

#27 AR-1254-2

R.T.: 5.710 min
 Delta R.T.: 0.000 min
 Response: 367690393
 Conc: 756.01 ng/ml

#27 AR-1254-2

R.T.: 5.683 min
 Delta R.T.: 0.000 min
 Response: 212567365
 Conc: 751.56 ng/ml

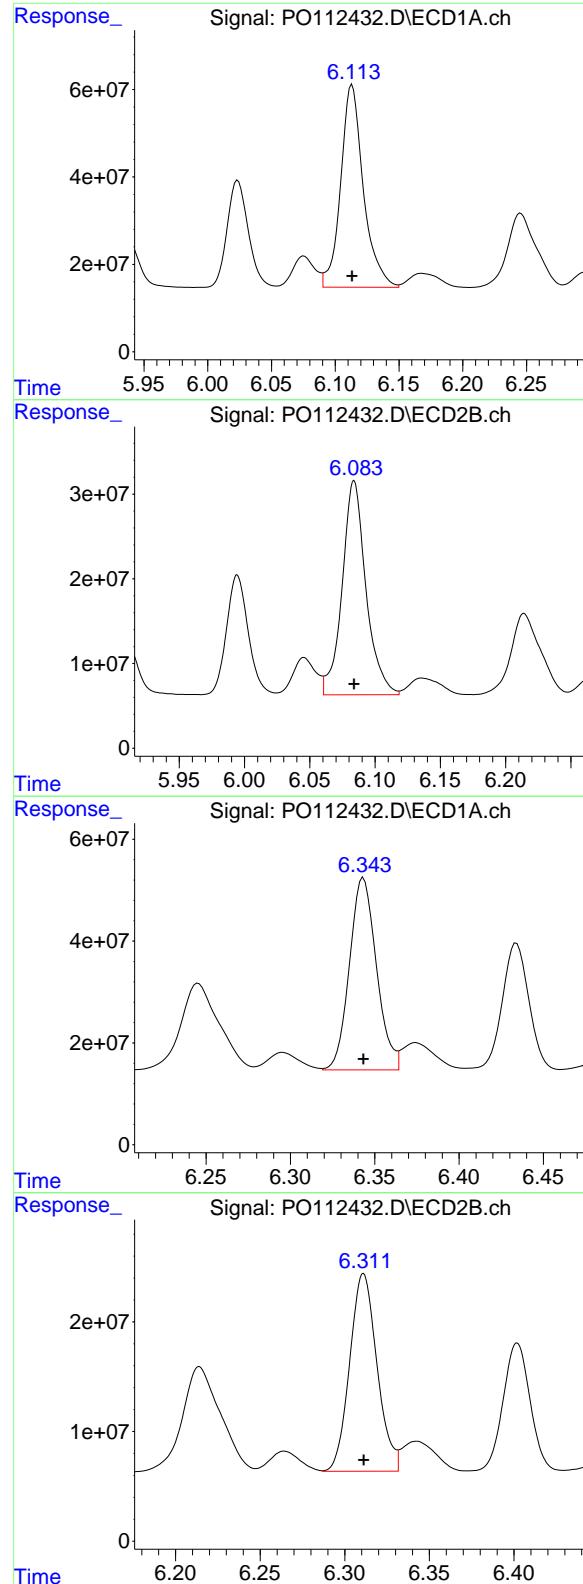

#28 AR-1254-3

R.T.: 6.113 min
 Delta R.T.: 0.000 min
 Response: 574026402
 Conc: 755.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC750

#28 AR-1254-3


R.T.: 6.084 min
 Delta R.T.: 0.000 min
 Response: 320734922
 Conc: 749.69 ng/ml

#29 AR-1254-4

R.T.: 6.343 min
 Delta R.T.: 0.000 min
 Response: 420396842
 Conc: 755.63 ng/ml

#29 AR-1254-4

R.T.: 6.311 min
 Delta R.T.: 0.000 min
 Response: 202358218
 Conc: 753.32 ng/ml

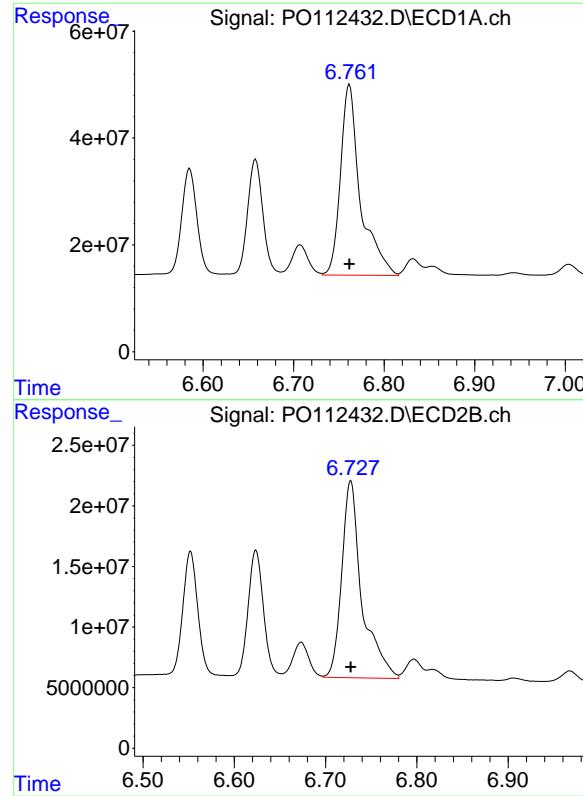

#30 AR-1254-5

R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 547016738
Conc: 752.27 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC750

#30 AR-1254-5

R.T.: 6.728 min
Delta R.T.: 0.000 min
Response: 250407470
Conc: 747.40 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:21
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:00:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 451.0E6 | 271.0E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.695 | 8.641 | 405.9E6 | 95544930 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|---------|---------|---------|
| 26) L6 AR-1254-1 | 5.561 | 5.535 | 284.0E6 | 169.6E6 | 500.000 | 500.000 |
| 27) L6 AR-1254-2 | 5.711 | 5.683 | 250.7E6 | 147.7E6 | 500.000 | 500.000 |
| 28) L6 AR-1254-3 | 6.114 | 6.084 | 389.1E6 | 222.1E6 | 500.000 | 500.000 |
| 29) L6 AR-1254-4 | 6.344 | 6.311 | 285.6E6 | 139.5E6 | 500.000 | 500.000 |
| 30) L6 AR-1254-5 | 6.762 | 6.727 | 369.5E6 | 173.2E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112433.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:21
 Operator : YP/AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:00:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

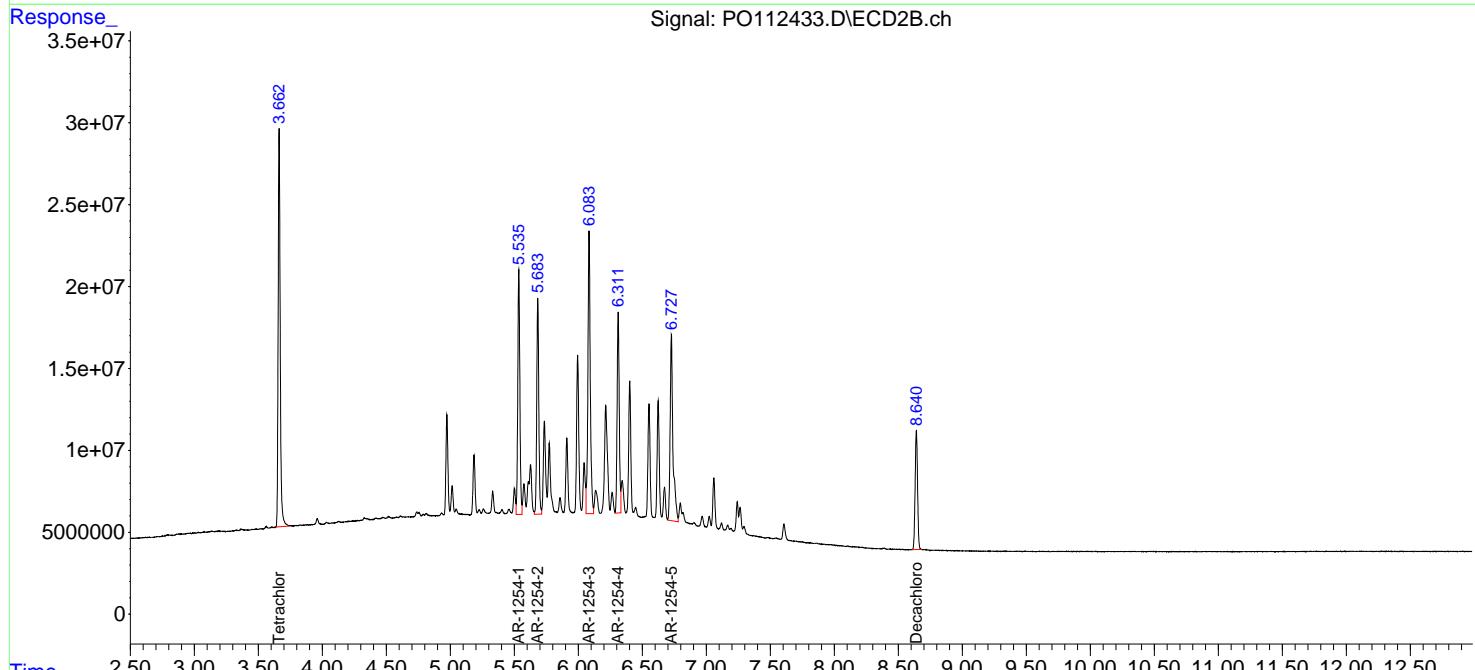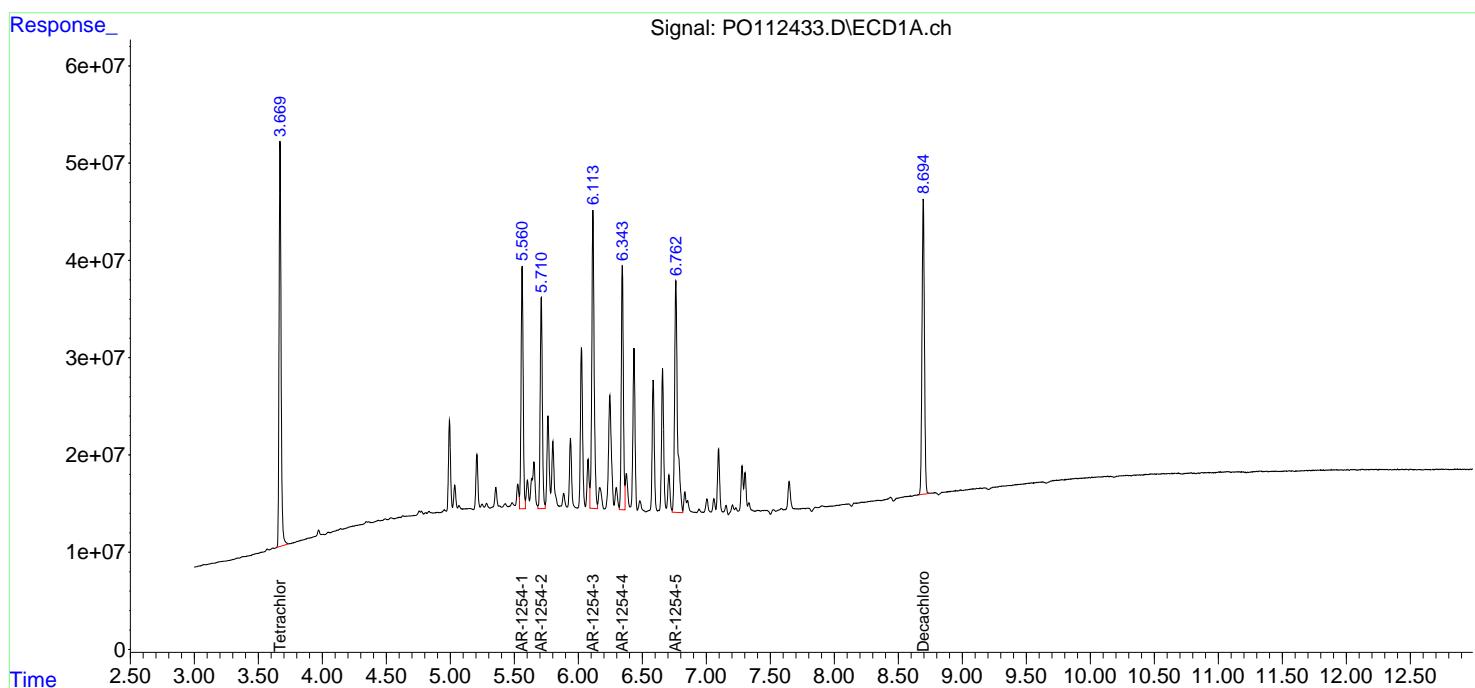


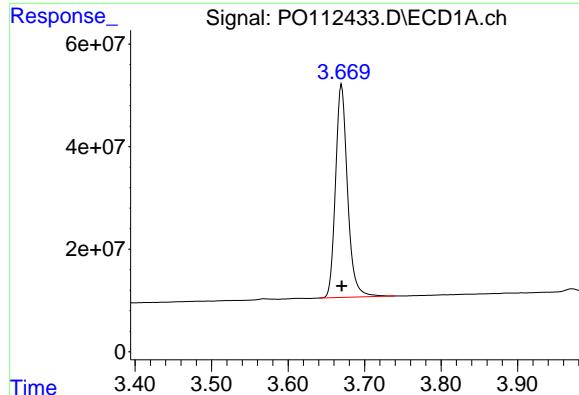

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 450992127
Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC500

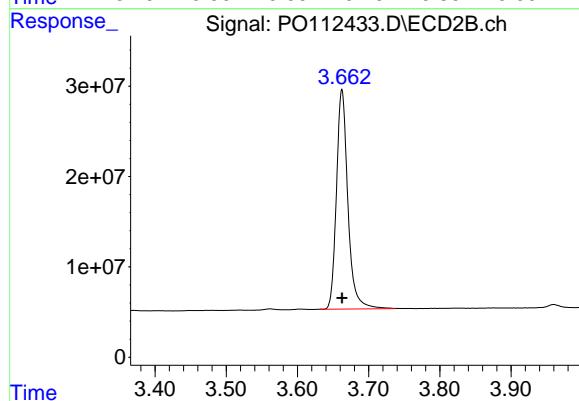


#1 Tetrachloro-m-xylene

R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 270977840
Conc: 50.00 ng/ml

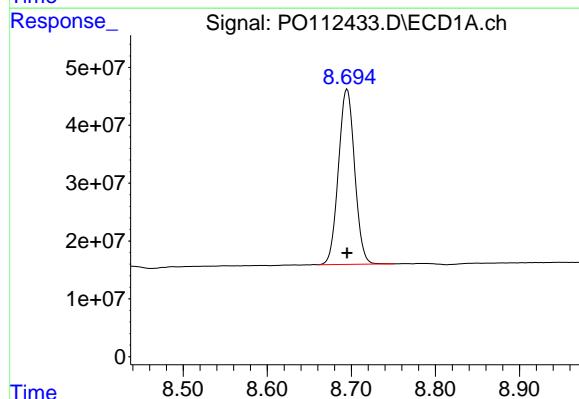

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 405922042
Conc: 50.00 ng/ml

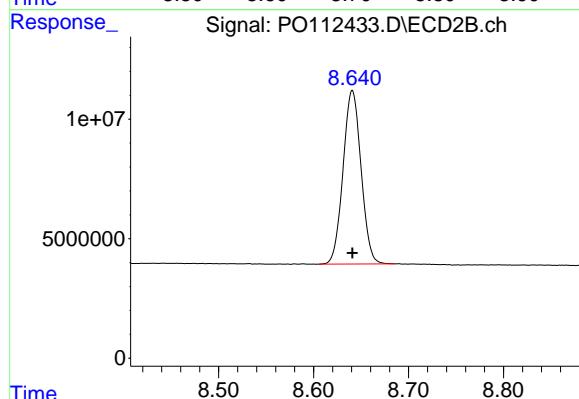





#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 95544930
Conc: 50.00 ng/ml

#26 AR-1254-1

R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 284024039
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC500

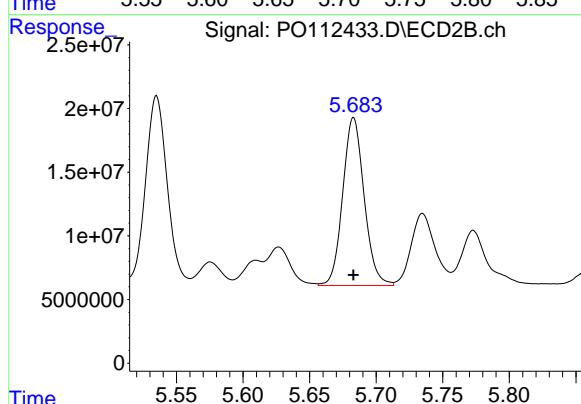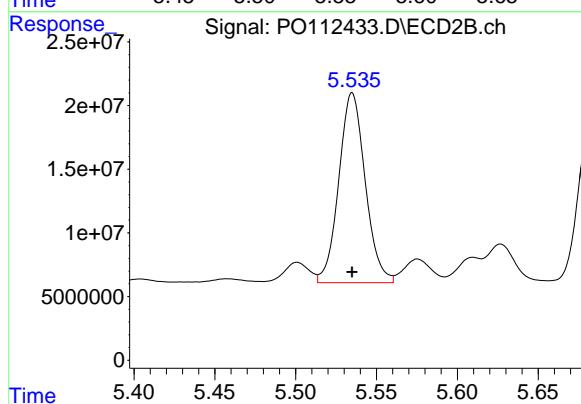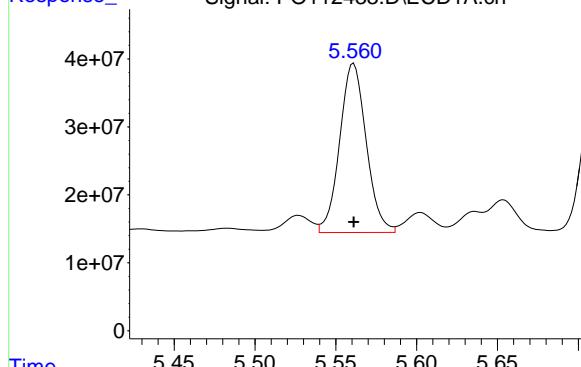

#26 AR-1254-1


R.T.: 5.535 min
 Delta R.T.: 0.000 min
 Response: 169585574
 Conc: 500.00 ng/ml

#27 AR-1254-2

R.T.: 5.711 min
 Delta R.T.: 0.000 min
 Response: 250715808
 Conc: 500.00 ng/ml

#27 AR-1254-2

R.T.: 5.683 min
 Delta R.T.: 0.000 min
 Response: 147749733
 Conc: 500.00 ng/ml

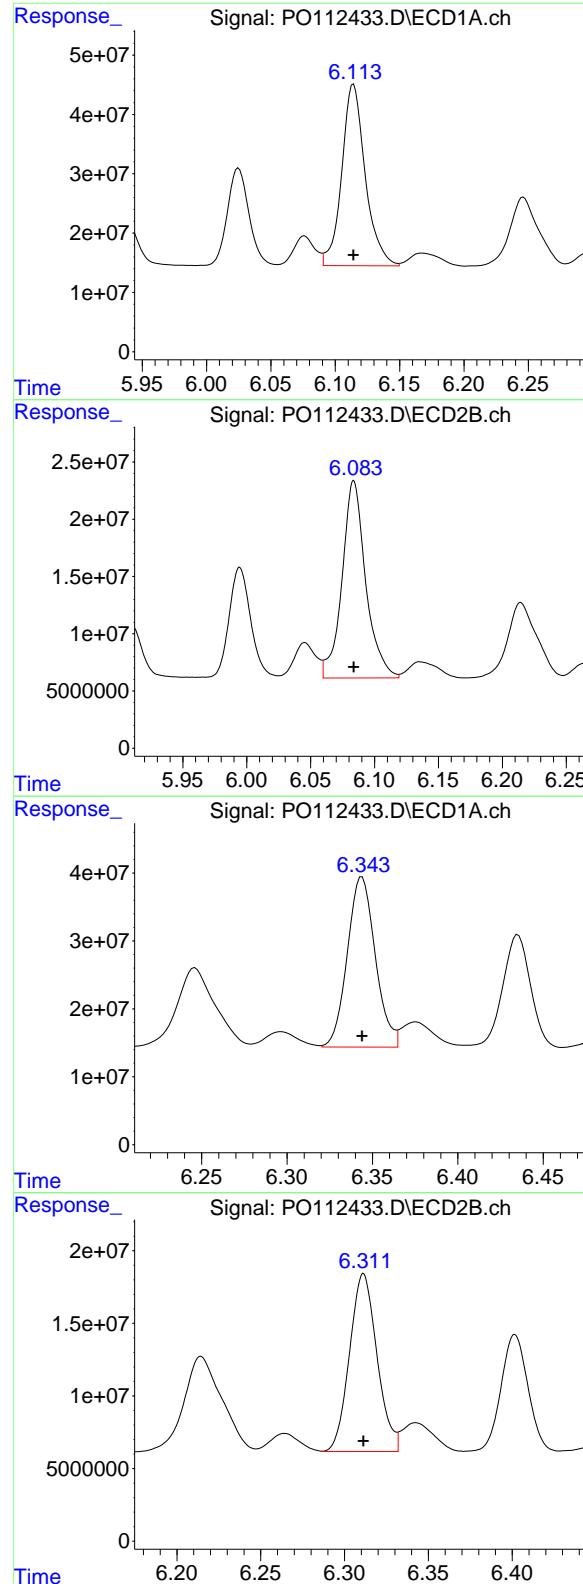

#28 AR-1254-3

R.T.: 6.114 min
 Delta R.T.: 0.000 min
 Response: 389058308
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC500

#28 AR-1254-3

R.T.: 6.084 min
 Delta R.T.: 0.000 min
 Response: 222091515
 Conc: 500.00 ng/ml

#29 AR-1254-4

R.T.: 6.344 min
 Delta R.T.: 0.000 min
 Response: 285622463
 Conc: 500.00 ng/ml



#29 AR-1254-4

R.T.: 6.311 min
 Delta R.T.: 0.000 min
 Response: 139534321
 Conc: 500.00 ng/ml

#30 AR-1254-5

R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 369473794
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC500

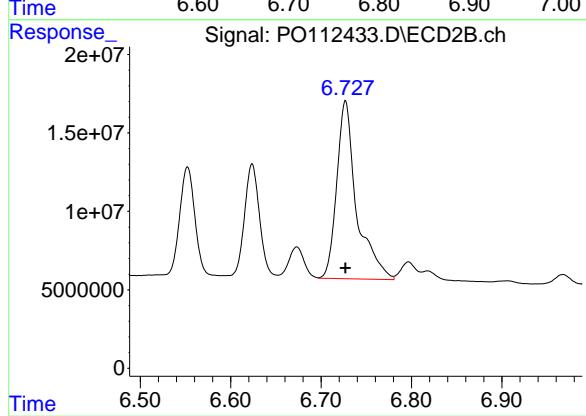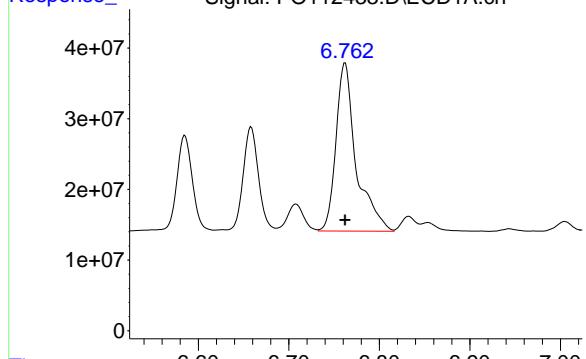

#30 AR-1254-5

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 173163657
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:39
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:10:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 226.9E6 | 138.1E6 | 25.568 | 25.793 |
| 2) SA Decachlor... | 8.694 | 8.640 | 201.7E6 | 48700127 | 25.228 | 25.887 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 26) L6 AR-1254-1 | 5.561 | 5.534 | 149.8E6 | 90186516 | 266.972 | 270.708 |
| 27) L6 AR-1254-2 | 5.709 | 5.682 | 132.8E6 | 79565133 | 266.923 | 272.772 |
| 28) L6 AR-1254-3 | 6.113 | 6.083 | 197.0E6 | 115.6E6 | 256.833 | 264.830 |
| 29) L6 AR-1254-4 | 6.343 | 6.311 | 143.1E6 | 71723033 | 255.366 | 262.540 |
| 30) L6 AR-1254-5 | 6.761 | 6.727 | 186.0E6 | 89336234 | 254.281 | 262.279 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112434.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:39
 Operator : YP/AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:10:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

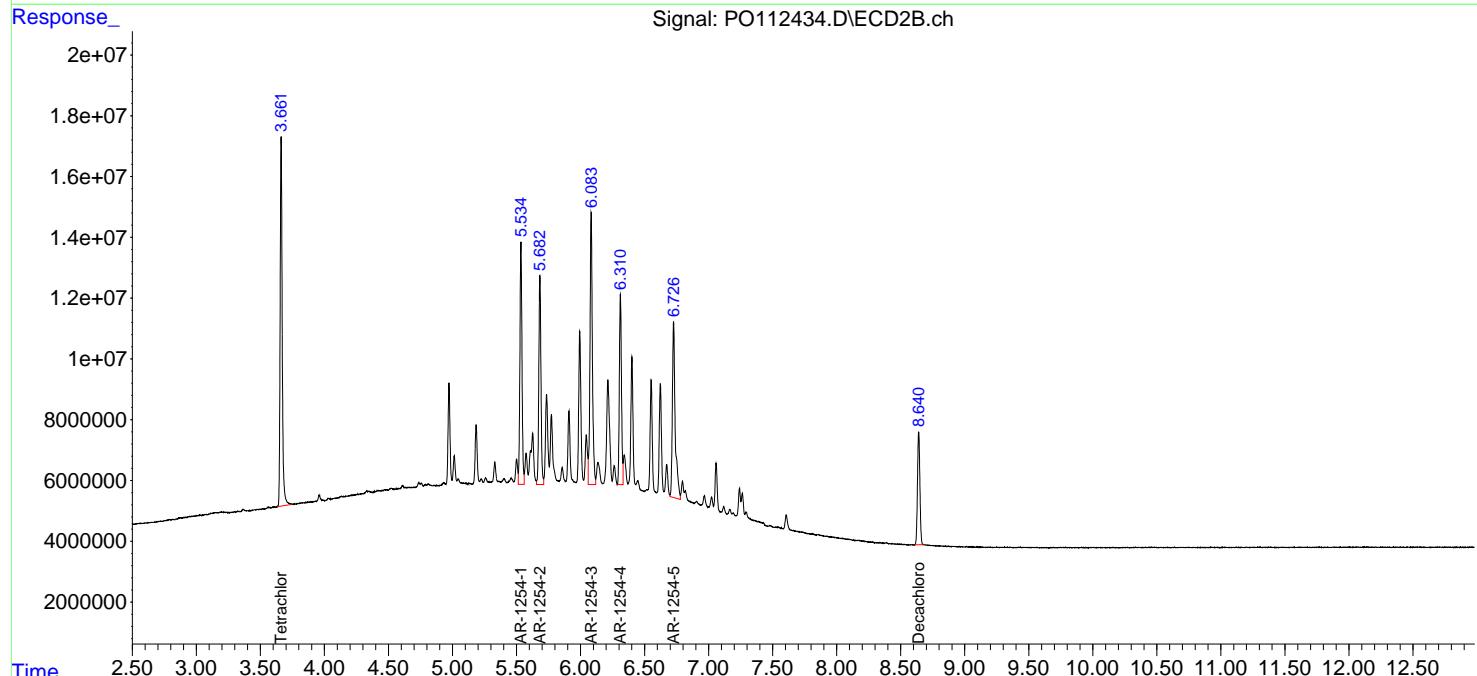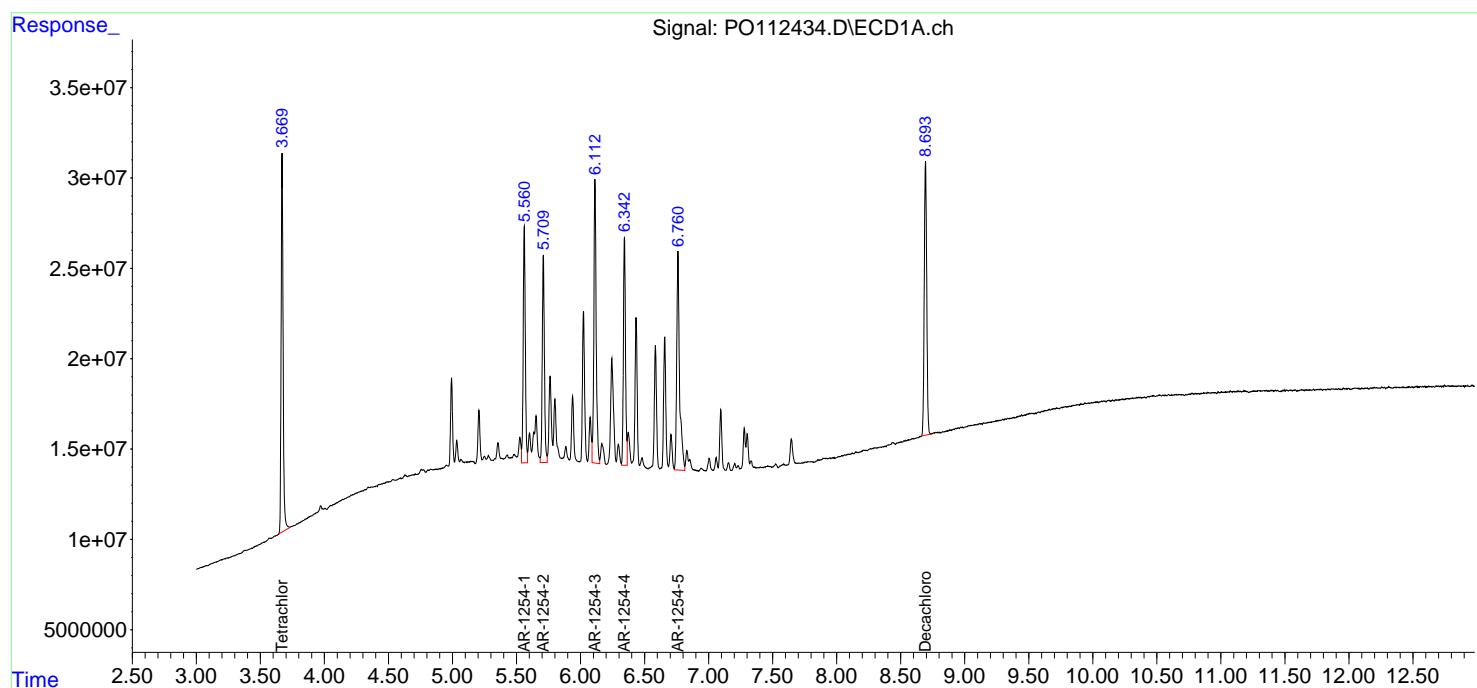

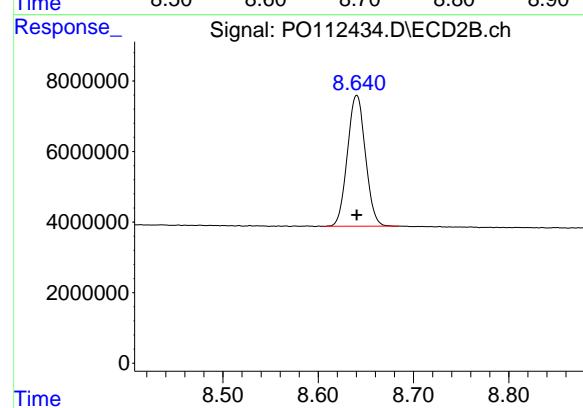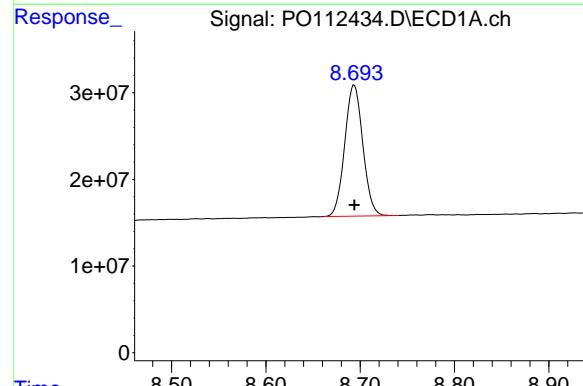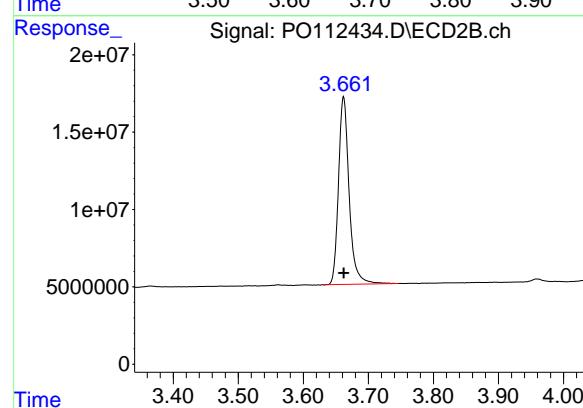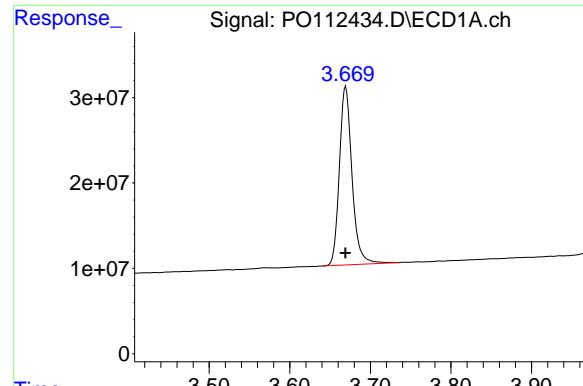

#1 Tetrachloro-m-xylene

R.T.: 3.669 min
 Delta R.T.: 0.000 min
 Response: 226937720
 Conc: 25.57 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
 Delta R.T.: 0.000 min
 Response: 138119113
 Conc: 25.79 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
 Delta R.T.: 0.000 min
 Response: 201741367
 Conc: 25.23 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.640 min
 Delta R.T.: 0.000 min
 Response: 48700127
 Conc: 25.89 ng/ml

#26 AR-1254-1


R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 149790449
 Conc: 266.97 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

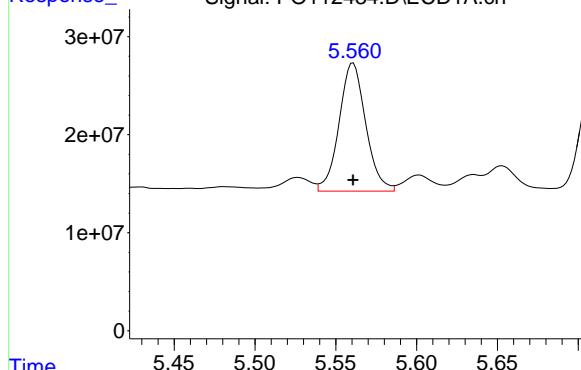


#26 AR-1254-1

R.T.: 5.534 min
 Delta R.T.: 0.000 min
 Response: 90186516
 Conc: 270.71 ng/ml

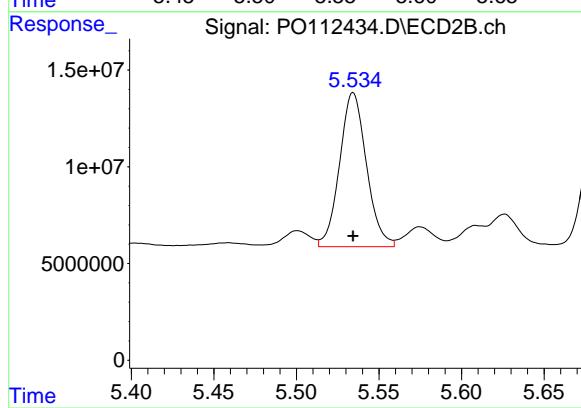


#27 AR-1254-2

R.T.: 5.709 min
 Delta R.T.: 0.000 min
 Response: 132816908
 Conc: 266.92 ng/ml



#27 AR-1254-2





R.T.: 5.682 min
 Delta R.T.: 0.000 min
 Response: 79565133
 Conc: 272.77 ng/ml

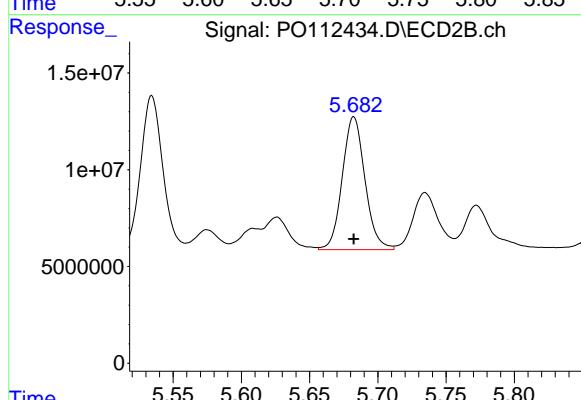

#28 AR-1254-3

R.T.: 6.113 min
 Delta R.T.: 0.000 min
 Response: 197002011
 Conc: 256.83 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

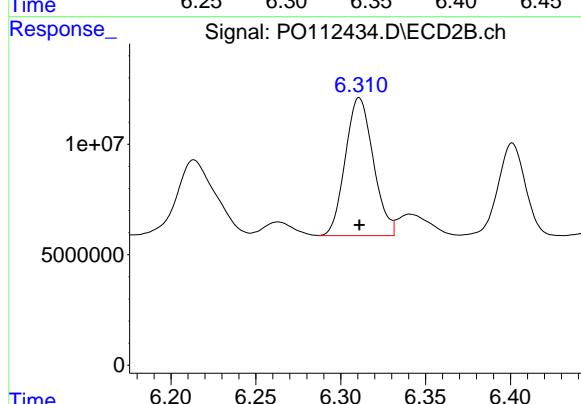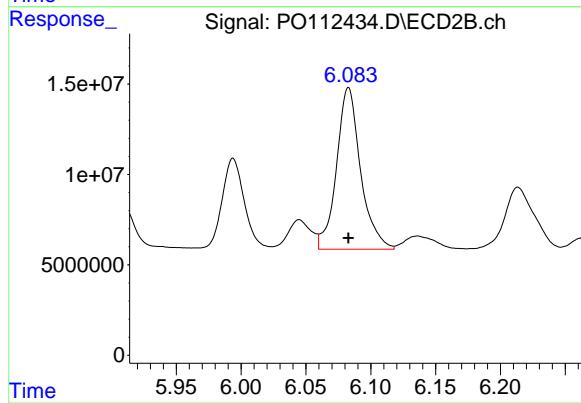

#28 AR-1254-3

R.T.: 6.083 min
 Delta R.T.: 0.000 min
 Response: 115586478
 Conc: 264.83 ng/ml

#29 AR-1254-4

R.T.: 6.343 min
 Delta R.T.: 0.000 min
 Response: 143097988
 Conc: 255.37 ng/ml



#29 AR-1254-4

R.T.: 6.311 min
 Delta R.T.: 0.000 min
 Response: 71723033
 Conc: 262.54 ng/ml

#30 AR-1254-5

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 185962684
Conc: 254.28 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC250

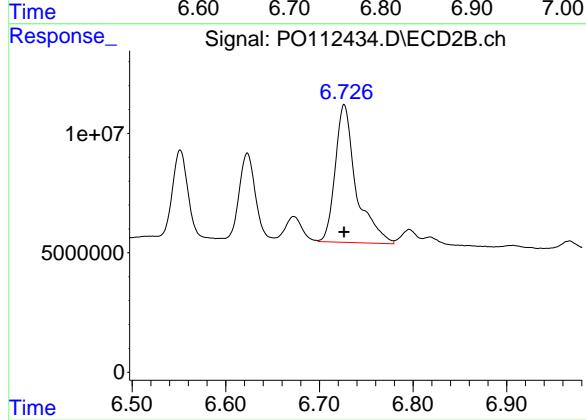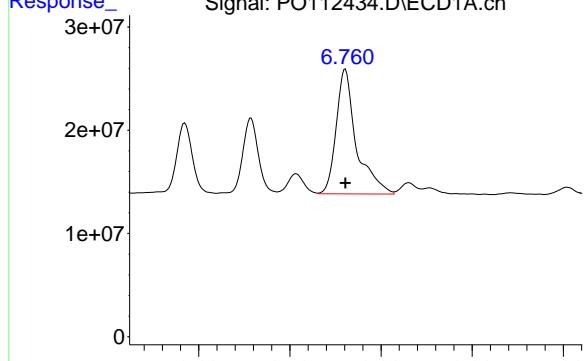

#30 AR-1254-5

R.T.: 6.727 min
Delta R.T.: 0.000 min
Response: 89336234
Conc: 262.28 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:57
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:14:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.669 | 3.661 | 35024549 | 22021040 | 4.120 | 4.264 |
| 2) SA Decachlor... | 8.694 | 8.640 | 31608253 | 7869748 | 4.125 | 4.324 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 26) L6 AR-1254-1 | 5.560 | 5.534 | 25025407 | 15525110 | 45.951m | 47.285m |
| 27) L6 AR-1254-2 | 5.710 | 5.682 | 21962545 | 14034521 | 45.717m | 48.955m |
| 28) L6 AR-1254-3 | 6.114 | 6.082 | 32662856 | 19574397 | 43.885 | 45.822m |
| 29) L6 AR-1254-4 | 6.344 | 6.311 | 25352878 | 13603049 | 46.121 | 50.646 |
| 30) L6 AR-1254-5 | 6.762 | 6.726 | 30690471 | 15381815 | 43.359 | 46.051 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:57
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_O
ClientSampleId :
AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:14:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

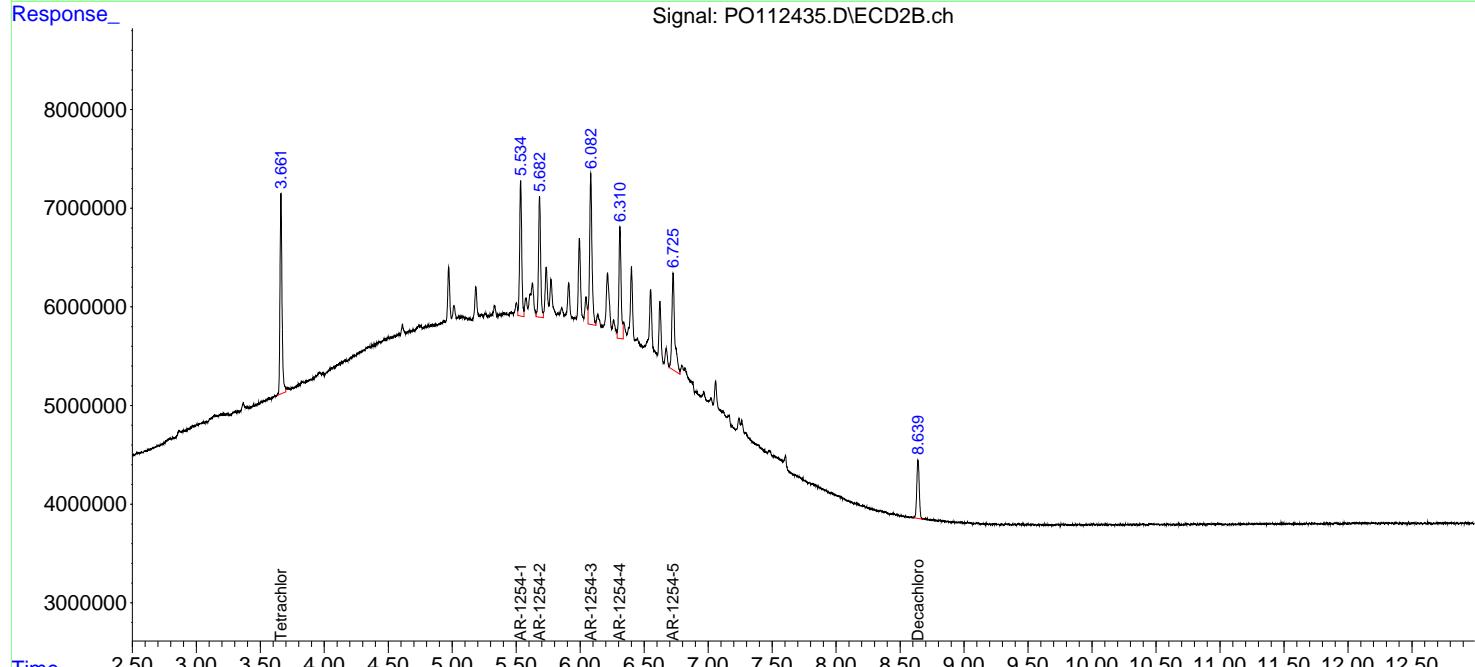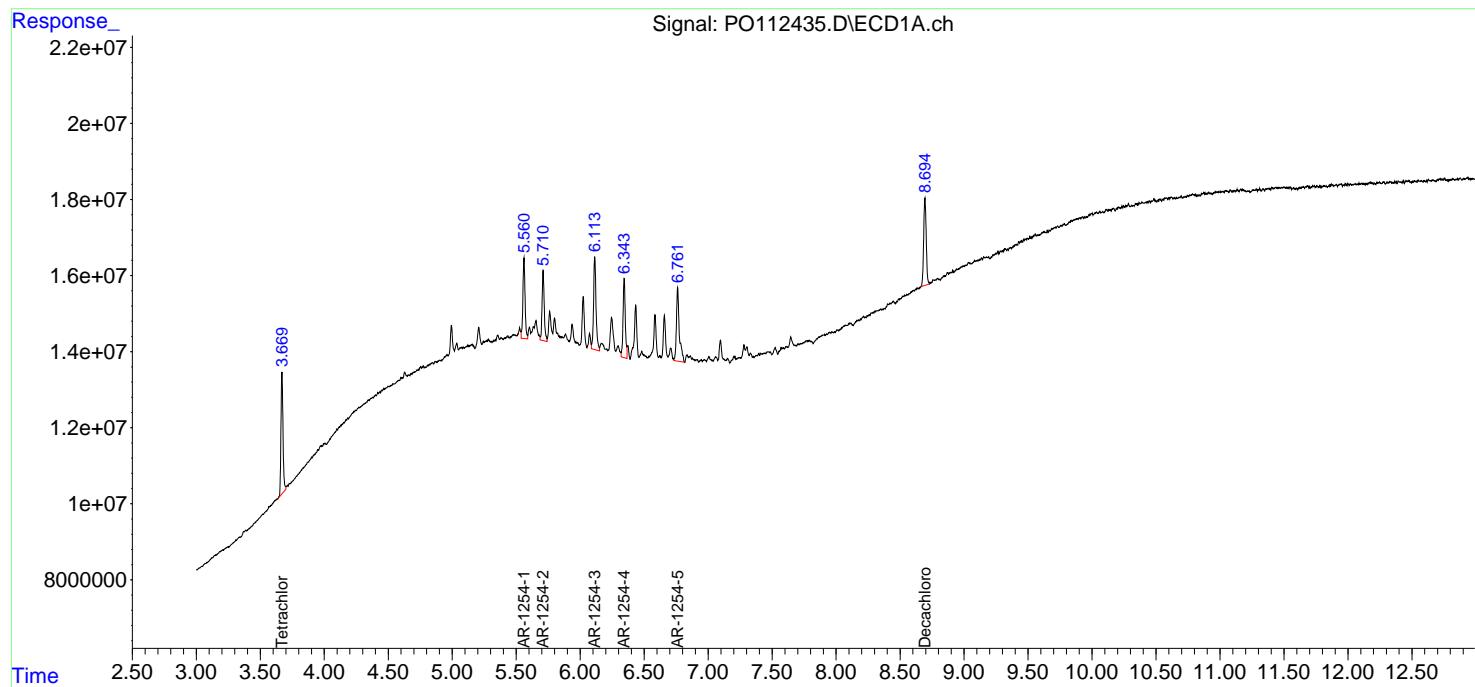

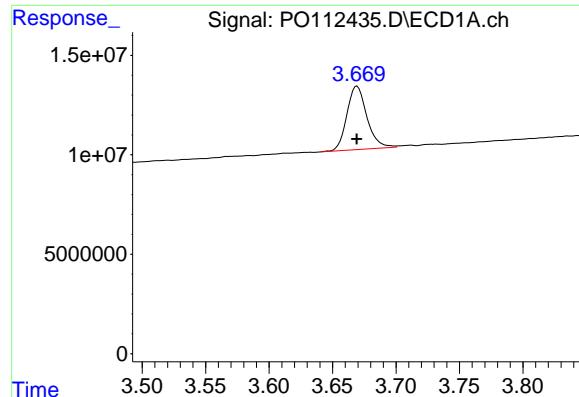


#1 Tetrachloro-m-xylene

R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 35024549
Conc: 4.12 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
Supervised By :mohammad ahmed 07/25/2025

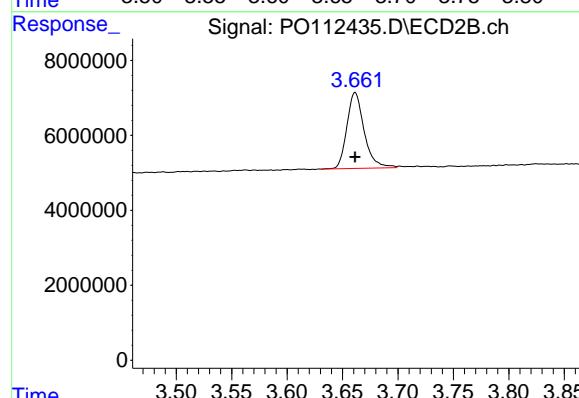


#1 Tetrachloro-m-xylene

R.T.: 3.661 min
Delta R.T.: 0.000 min
Response: 22021040
Conc: 4.26 ng/ml

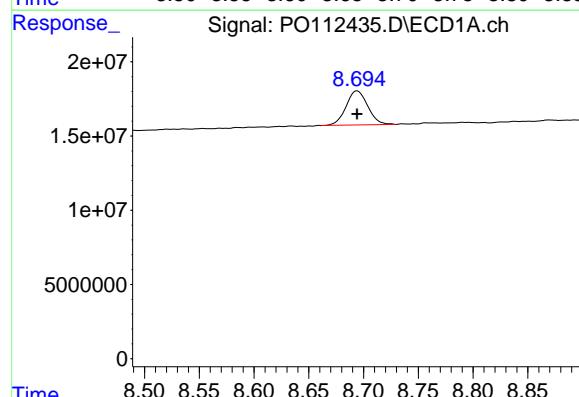

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 31608253
Conc: 4.13 ng/ml

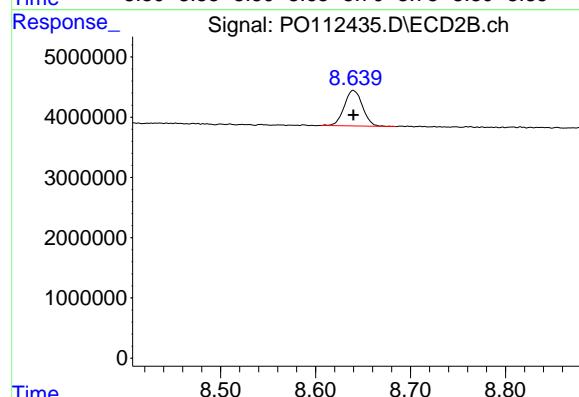

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 7869748
Conc: 4.32 ng/ml

#26 AR-1254-1

R.T.: 5.560 min
 Delta R.T.: 0.000 min
 Response: 25025407
 Conc: 45.95 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#26 AR-1254-1





R.T.: 5.534 min
 Delta R.T.: 0.000 min
 Response: 15525110
 Conc: 47.28 ng/ml

#27 AR-1254-2

R.T.: 5.710 min
 Delta R.T.: 0.000 min
 Response: 21962545
 Conc: 45.72 ng/ml

#27 AR-1254-2

R.T.: 5.682 min
 Delta R.T.: 0.000 min
 Response: 14034521
 Conc: 48.95 ng/ml

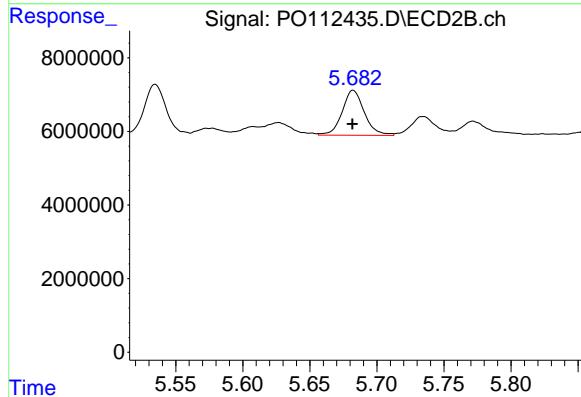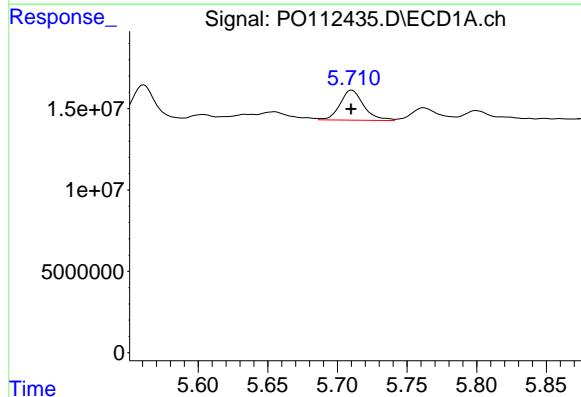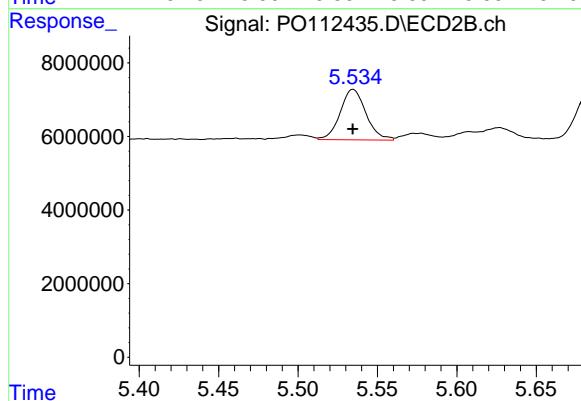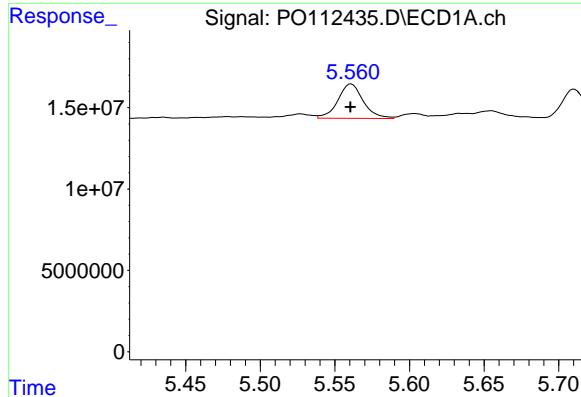

#28 AR-1254-3

R.T.: 6.114 min
 Delta R.T.: 0.000 min
 Response: 32662856
 Conc: 43.88 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

#28 AR-1254-3





R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 19574397
 Conc: 45.82 ng/ml

#29 AR-1254-4

R.T.: 6.344 min
 Delta R.T.: 0.000 min
 Response: 25352878
 Conc: 46.12 ng/ml

#29 AR-1254-4

R.T.: 6.311 min
 Delta R.T.: 0.000 min
 Response: 13603049
 Conc: 50.65 ng/ml

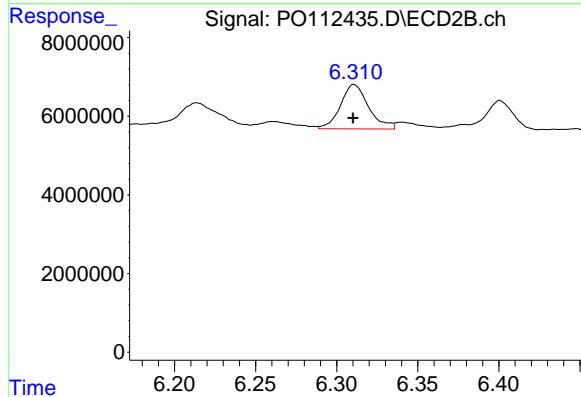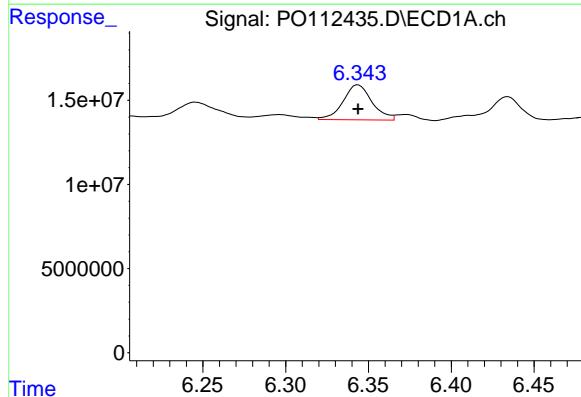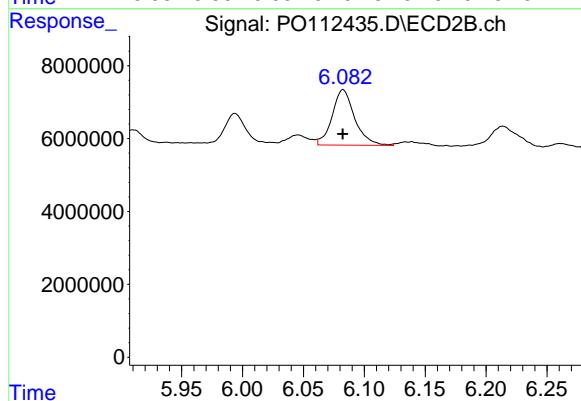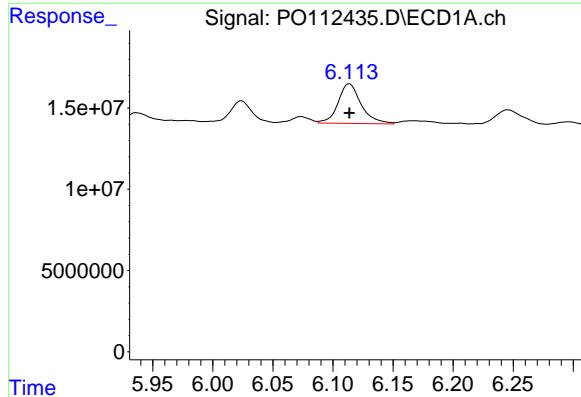



#30 AR-1254-5

R.T.: 6.762 min
 Delta R.T.: 0.000 min
 Response: 30690471
 Conc: 43.36 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 07/24/2025
 Supervised By :mohammad ahmed 07/25/2025

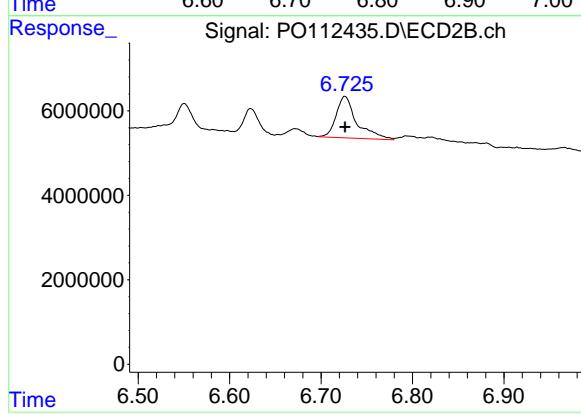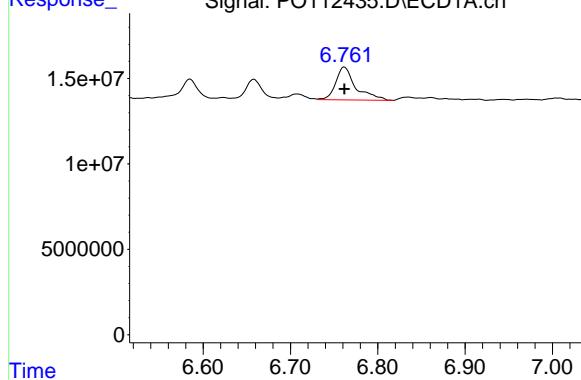

#30 AR-1254-5

R.T.: 6.726 min
 Delta R.T.: 0.000 min
 Response: 15381815
 Conc: 46.05 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 18:16
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:23:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:22:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 431.0E6 | 259.6E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.695 | 8.640 | 390.0E6 | 91817563 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 36) L8 AR-1262-1 | 6.801 | 6.766 | 464.6E6 | 207.4E6 | 500.000 | 500.000 |
| 37) L8 AR-1262-2 | 7.303 | 7.265 | 743.5E6 | 257.8E6 | 500.000 | 500.000 |
| 38) L8 AR-1262-3 | 7.586 | 7.546 | 295.1E6 | 93262624 | 500.000 | 500.000 |
| 39) L8 AR-1262-4 | 7.650 | 7.611 | 497.1E6 | 144.1E6 | 500.000 | 500.000 |
| 40) L8 AR-1262-5 | 8.146 | 8.103 | 217.0E6 | 49751686 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112436.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 18:16
 Operator : YP/AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_O
ClientSampleId :
 AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:23:57 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:22:29 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

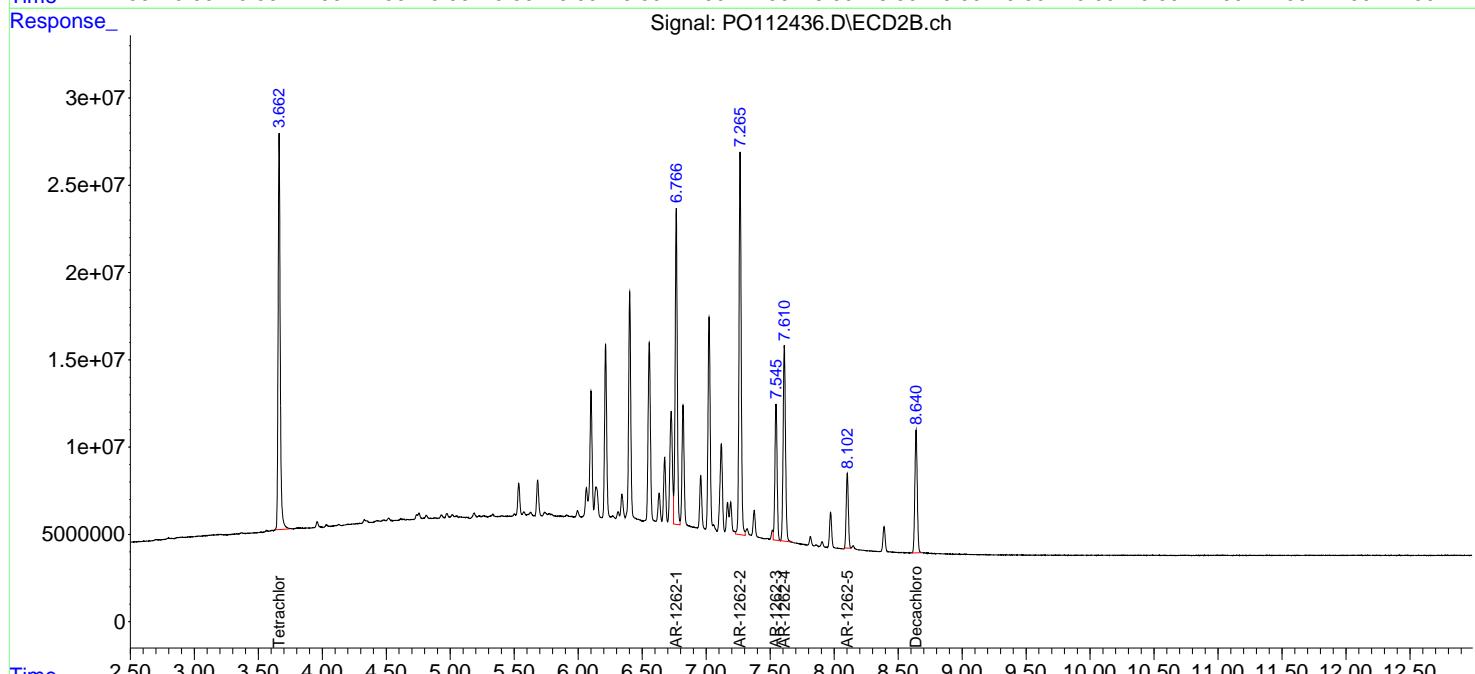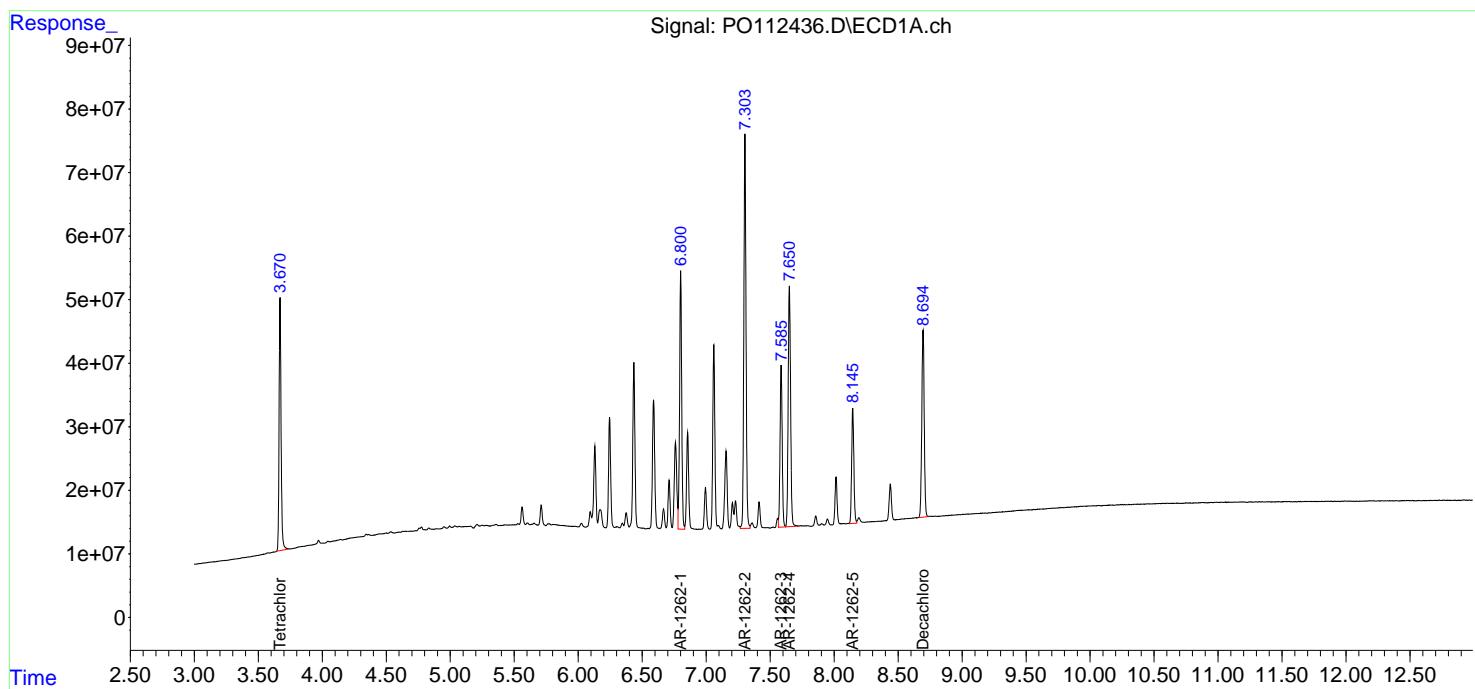

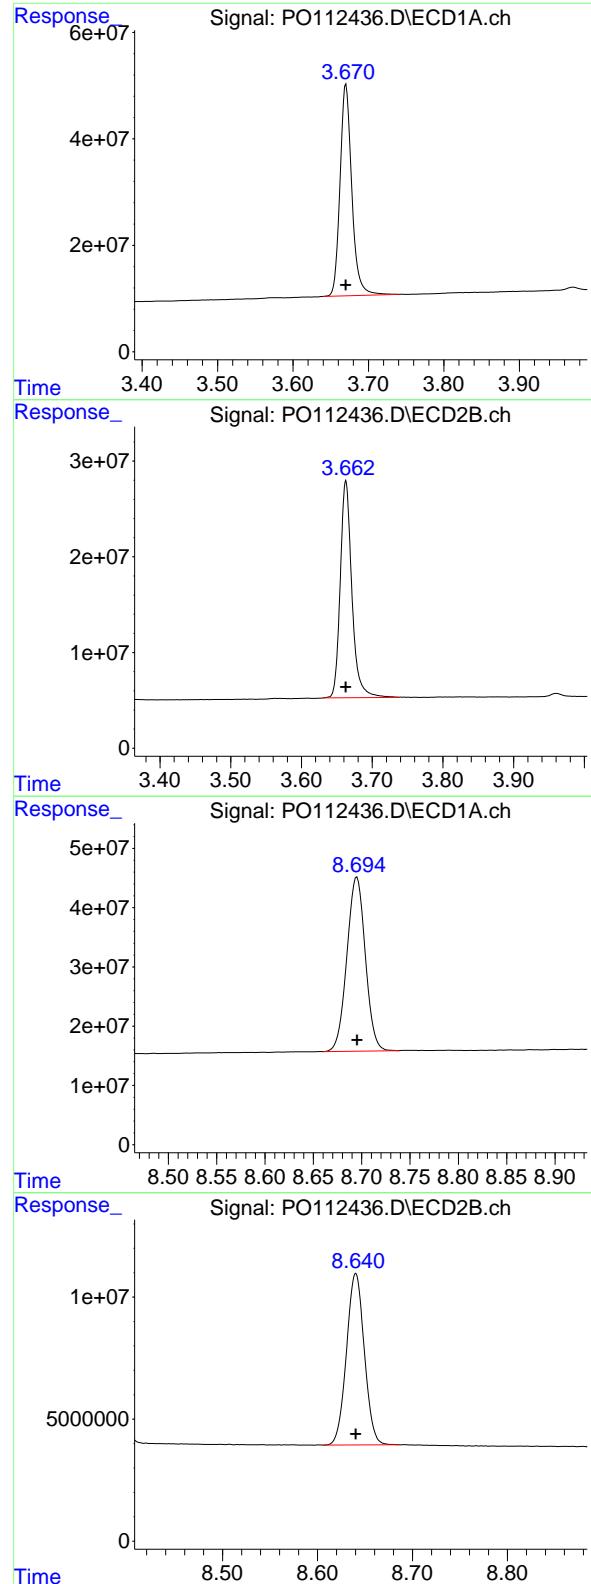

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 431047231
Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
Delta R.T.: 0.000 min
Response: 259634200
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 390011550
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 91817563
Conc: 50.00 ng/ml

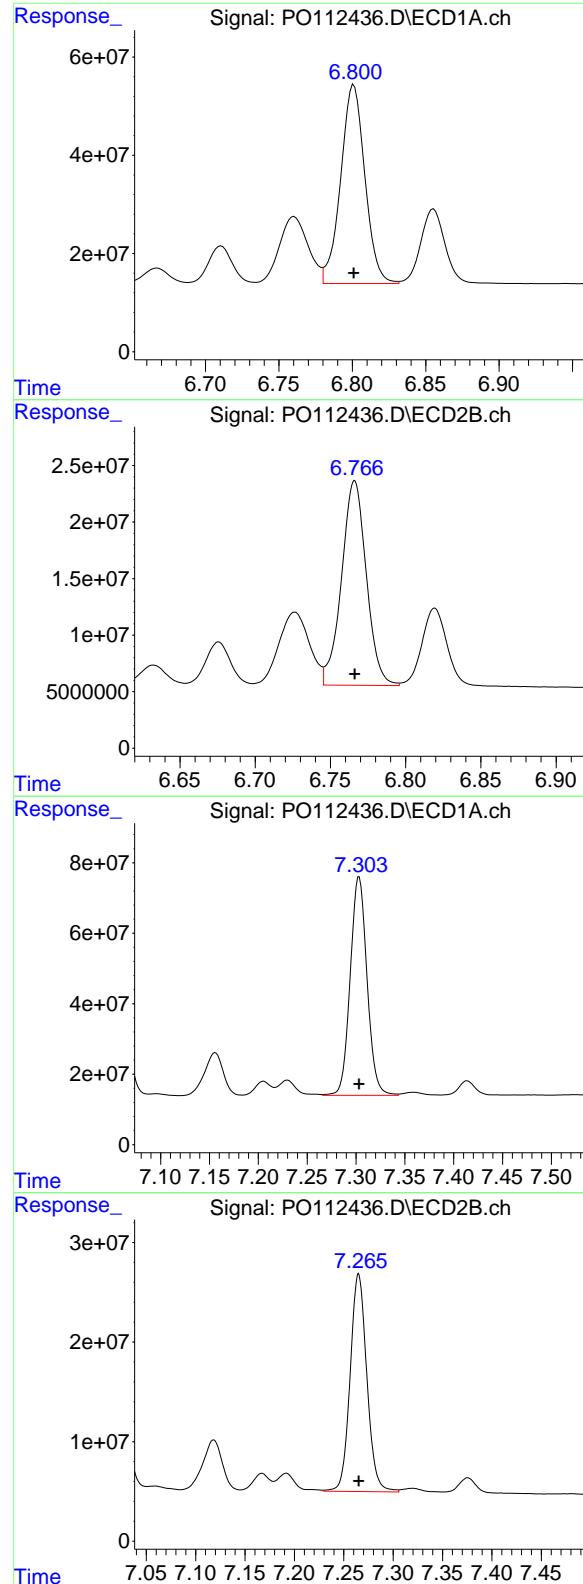

#36 AR-1262-1

R.T.: 6.801 min
 Delta R.T.: 0.000 min
 Response: 464603934
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

#36 AR-1262-1

R.T.: 6.766 min
 Delta R.T.: 0.000 min
 Response: 207413976
 Conc: 500.00 ng/ml

#37 AR-1262-2

R.T.: 7.303 min
 Delta R.T.: 0.000 min
 Response: 743508813
 Conc: 500.00 ng/ml


#37 AR-1262-2

R.T.: 7.265 min
 Delta R.T.: 0.000 min
 Response: 257772904
 Conc: 500.00 ng/ml

#38 AR-1262-3


R.T.: 7.586 min
 Delta R.T.: 0.000 min
 Response: 295126335
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

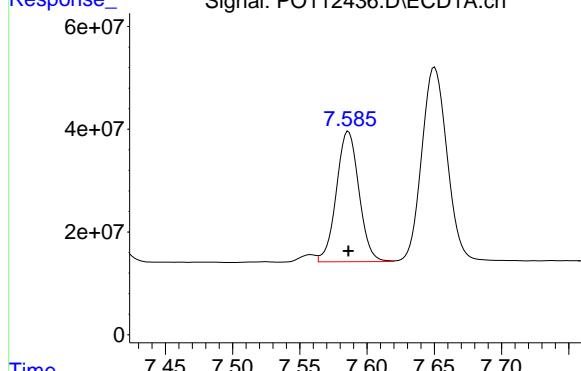


#38 AR-1262-3

R.T.: 7.546 min
 Delta R.T.: 0.000 min
 Response: 93262624
 Conc: 500.00 ng/ml

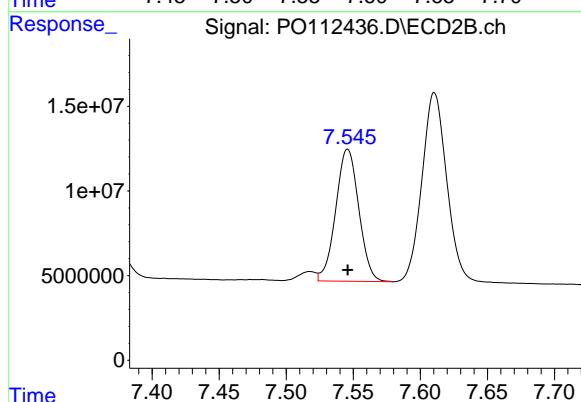


#39 AR-1262-4

R.T.: 7.650 min
 Delta R.T.: 0.000 min
 Response: 497083193
 Conc: 500.00 ng/ml

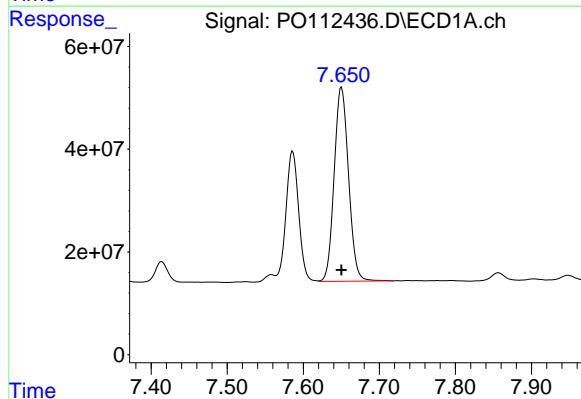

#39 AR-1262-4



R.T.: 7.611 min
 Delta R.T.: 0.000 min
 Response: 144051747
 Conc: 500.00 ng/ml

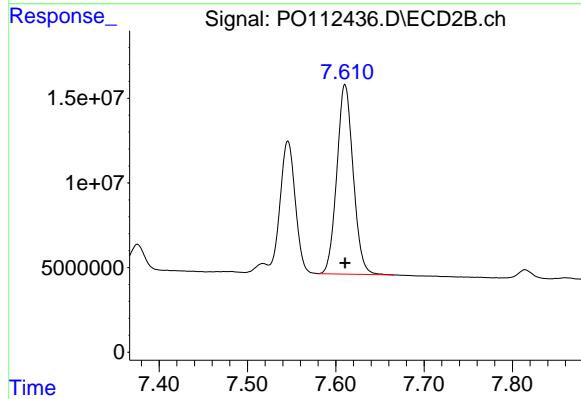

#40 AR-1262-5

R.T.: 8.146 min
Delta R.T.: 0.000 min
Response: 217030539
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1262ICC500

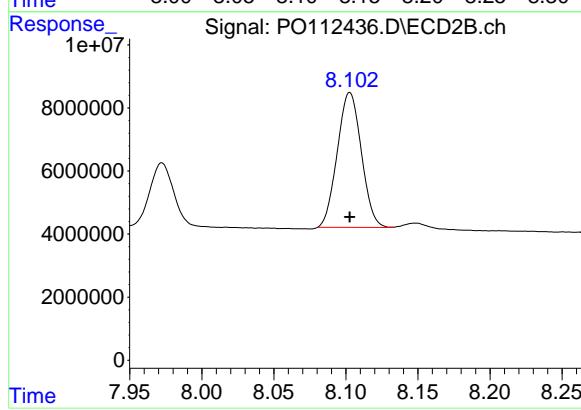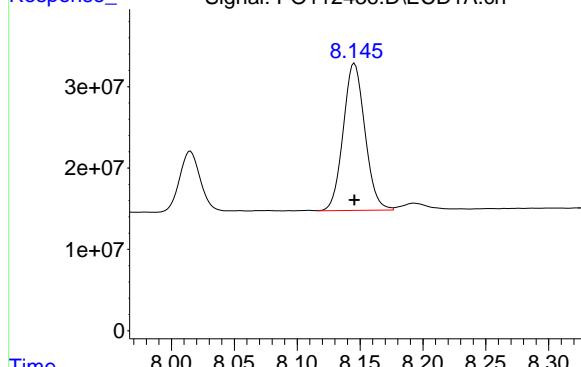

#40 AR-1262-5

R.T.: 8.103 min
Delta R.T.: 0.000 min
Response: 49751686
Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 18:34
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:26:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 891.6E6 | 532.6E6 | 96.171 | 96.108 |
| 2) SA Decachlor... | 8.695 | 8.642 | 1453.9E6 | 322.4E6 | 98.386 | 96.213 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|---------|---------|
| 41) L9 AR-1268-1 | 7.587 | 7.547 | 1805.2E6 | 514.6E6 | 975.507 | 965.897 |
| 42) L9 AR-1268-2 | 7.652 | 7.613 | 1523.8E6 | 421.6E6 | 977.268 | 965.543 |
| 43) L9 AR-1268-3 | 7.858 | 7.817 | 1298.6E6 | 318.8E6 | 974.006 | 962.314 |
| 44) L9 AR-1268-4 | 8.147 | 8.103 | 502.3E6 | 111.5E6 | 976.399 | 971.430 |
| 45) L9 AR-1268-5 | 8.440 | 8.392 | 3537.9E6 | 742.7E6 | 993.352 | 978.791 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 18:34
 Operator : YP/AJ
 Sample : AR1268ICC1000
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:26:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

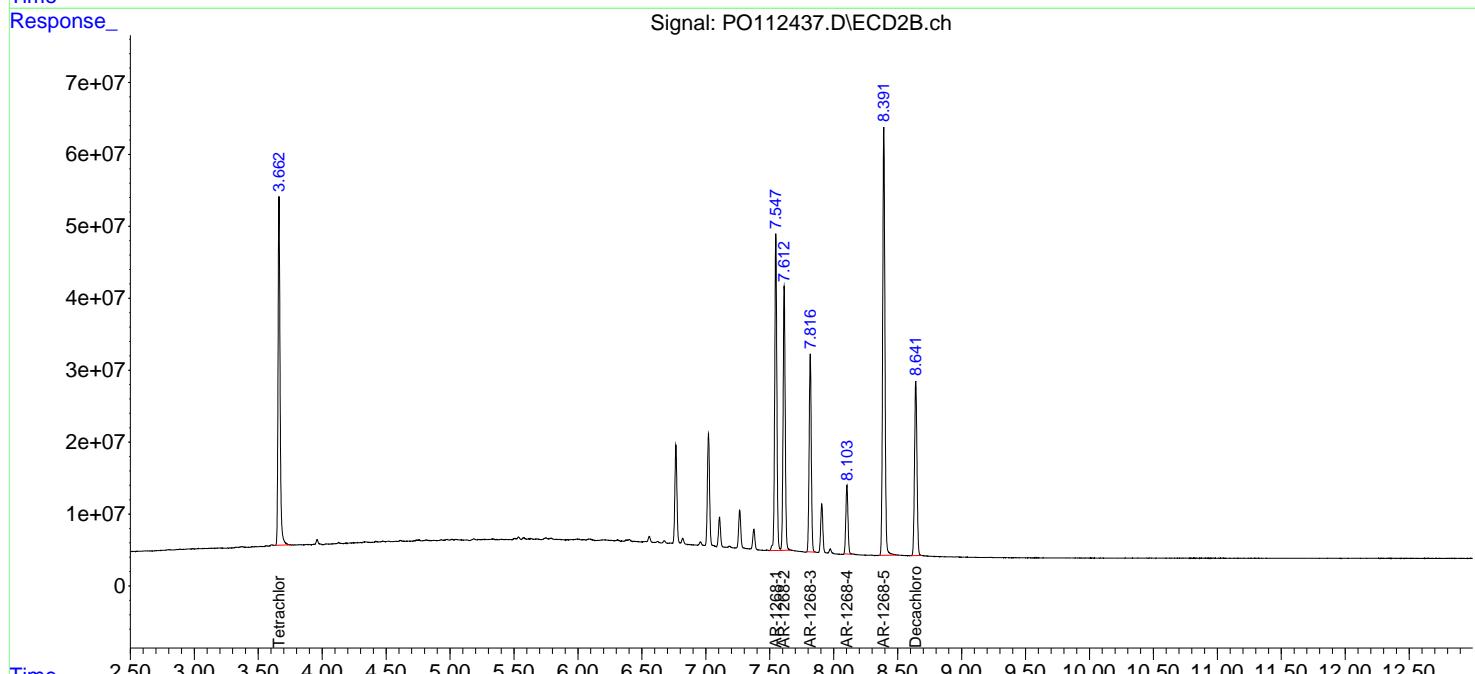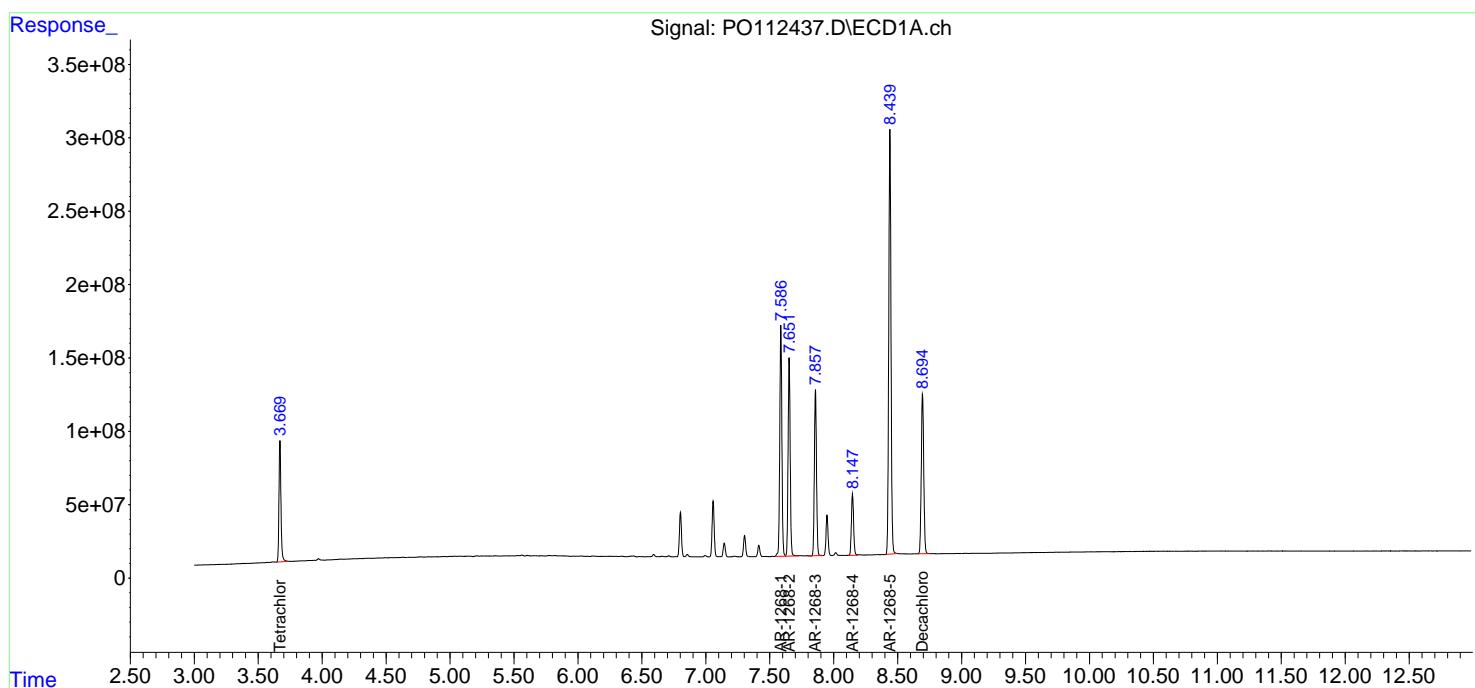

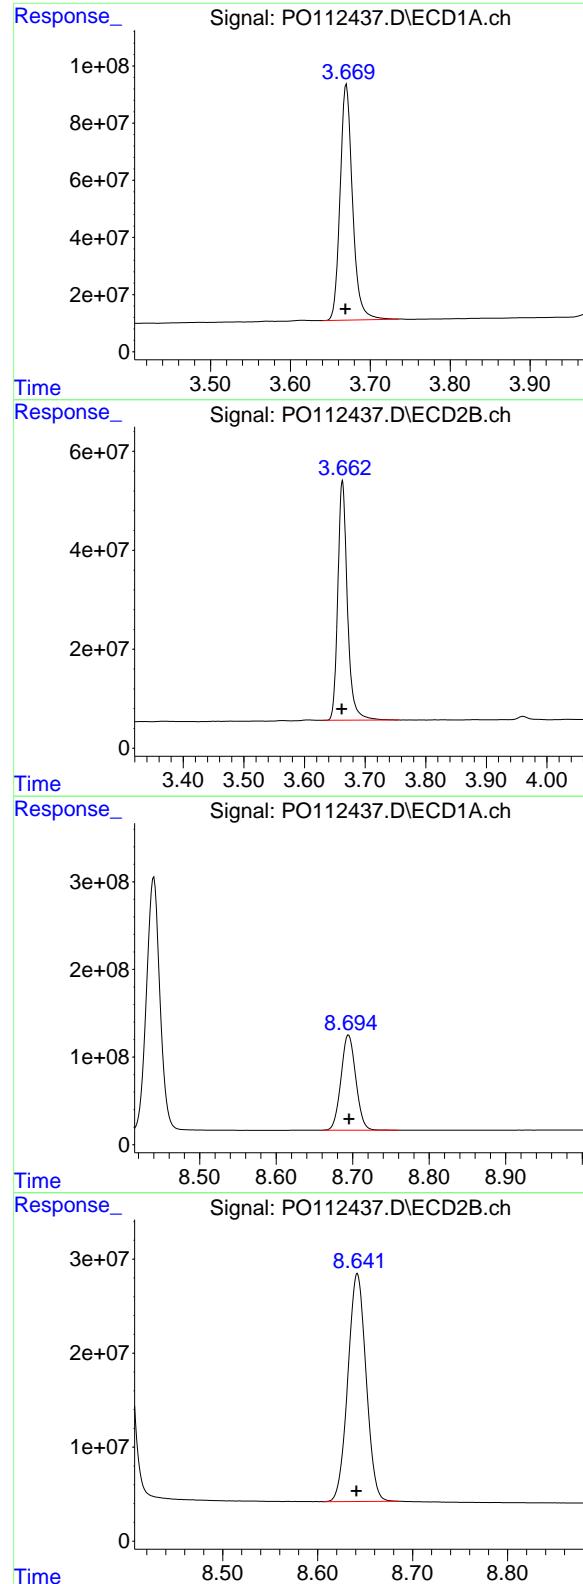

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: 0.001 min
 Response: 891646114
 Conc: 96.17 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1268ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
 Delta R.T.: 0.001 min
 Response: 532622392
 Conc: 96.11 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
 Delta R.T.: 0.000 min
 Response: 1453875783
 Conc: 98.39 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.642 min
 Delta R.T.: 0.001 min
 Response: 322448419
 Conc: 96.21 ng/ml

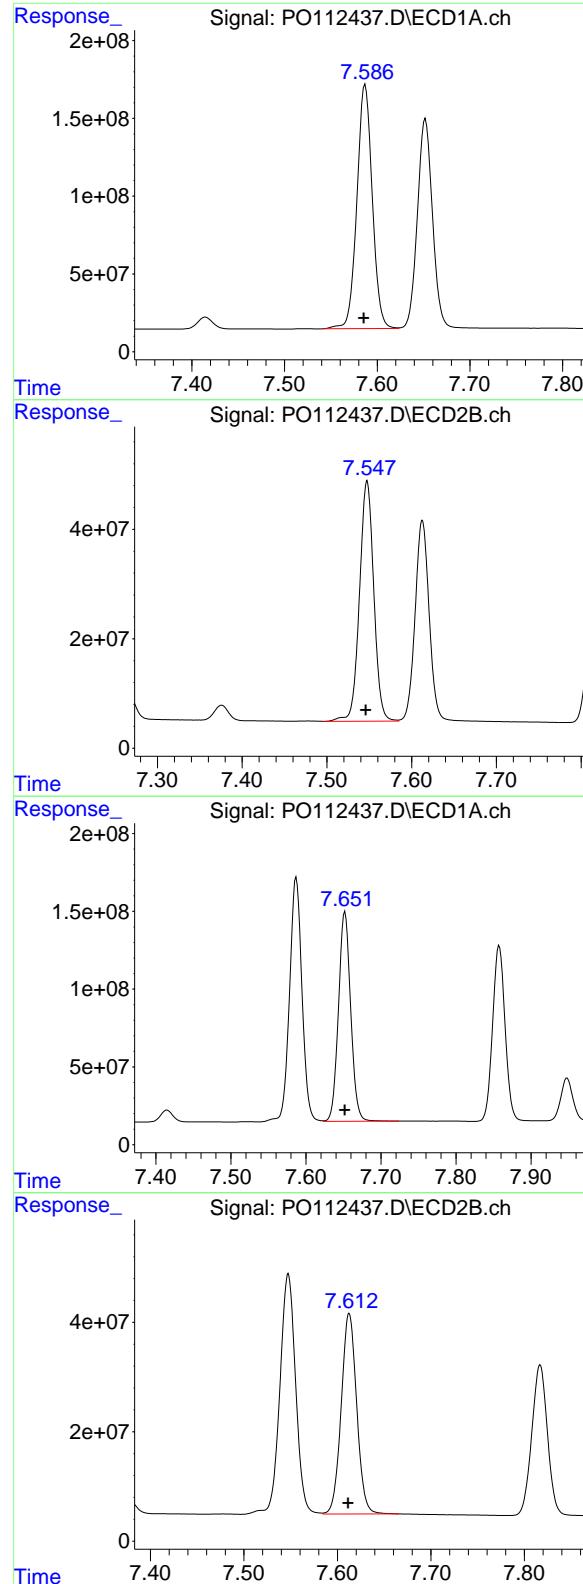

#41 AR-1268-1

R.T.: 7.587 min
 Delta R.T.: 0.001 min
 Response: 1805209287
 Conc: 975.51 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC1000

#41 AR-1268-1

R.T.: 7.547 min
 Delta R.T.: 0.002 min
 Response: 514567345
 Conc: 965.90 ng/ml

#42 AR-1268-2





R.T.: 7.652 min
 Delta R.T.: 0.000 min
 Response: 1523811042
 Conc: 977.27 ng/ml

#42 AR-1268-2

R.T.: 7.613 min
 Delta R.T.: 0.001 min
 Response: 421574479
 Conc: 965.54 ng/ml

#43 AR-1268-3

R.T.: 7.858 min
 Delta R.T.: 0.000 min
Instrument:
 Response: 1298638460 ECD_O
 Conc: 974.01 ng/ml ClientSampleId :
 AR1268ICC1000

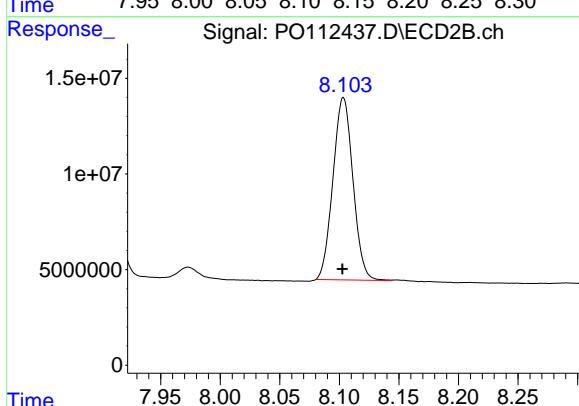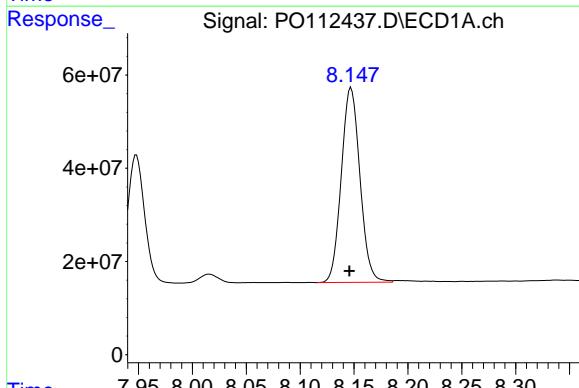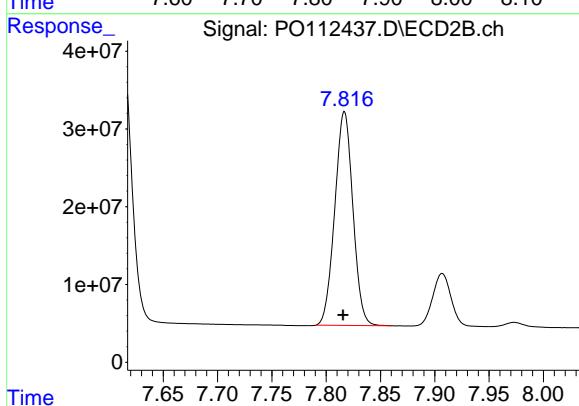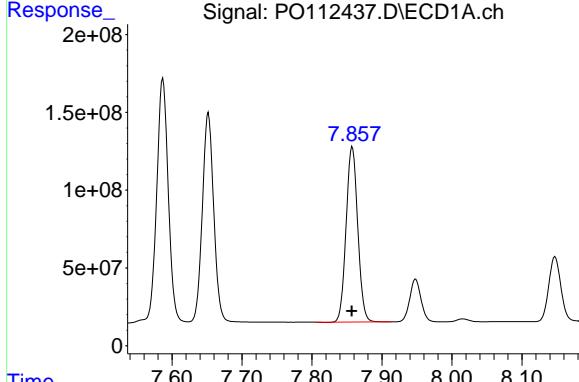

#43 AR-1268-3

R.T.: 7.817 min
 Delta R.T.: 0.001 min
 Response: 318758782
 Conc: 962.31 ng/ml

#44 AR-1268-4

R.T.: 8.147 min
 Delta R.T.: 0.001 min
 Response: 502325303
 Conc: 976.40 ng/ml



#44 AR-1268-4

R.T.: 8.103 min
 Delta R.T.: 0.000 min
 Response: 111516853
 Conc: 971.43 ng/ml

#45 AR-1268-5

R.T.: 8.440 min
Delta R.T.: 0.000 min
Response: 3537850645
Conc: 993.35 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC1000

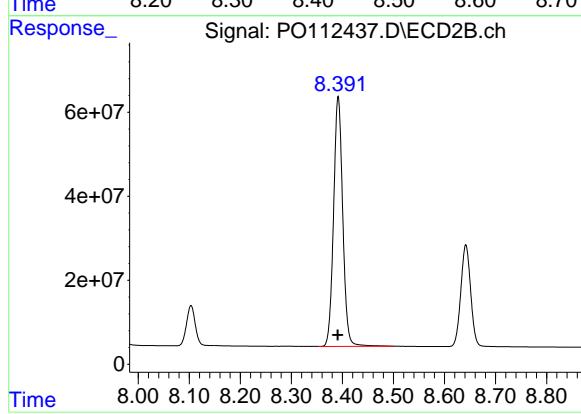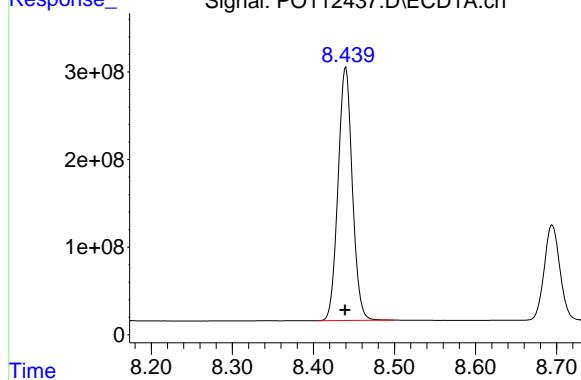

#45 AR-1268-5

R.T.: 8.392 min
Delta R.T.: 0.000 min
Response: 742715083
Conc: 978.79 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 18:53
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 692.2E6 | 413.4E6 | 74.664 | 74.591 |
| 2) SA Decachlor... | 8.695 | 8.641 | 1101.3E6 | 247.6E6 | 74.526 | 73.871 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 41) L9 AR-1268-1 | 7.586 | 7.547 | 1377.7E6 | 387.5E6 | 744.484 | 727.418 |
| 42) L9 AR-1268-2 | 7.652 | 7.613 | 1161.1E6 | 319.5E6 | 744.679 | 731.710 |
| 43) L9 AR-1268-3 | 7.857 | 7.816 | 987.1E6 | 243.4E6 | 740.359 | 734.748 |
| 44) L9 AR-1268-4 | 8.147 | 8.103 | 386.4E6 | 86779378 | 751.011 | 755.940 |
| 45) L9 AR-1268-5 | 8.439 | 8.391 | 2676.6E6 | 567.6E6 | 751.521 | 747.952 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 18:53
 Operator : YP/AJ
 Sample : AR1268ICC750
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

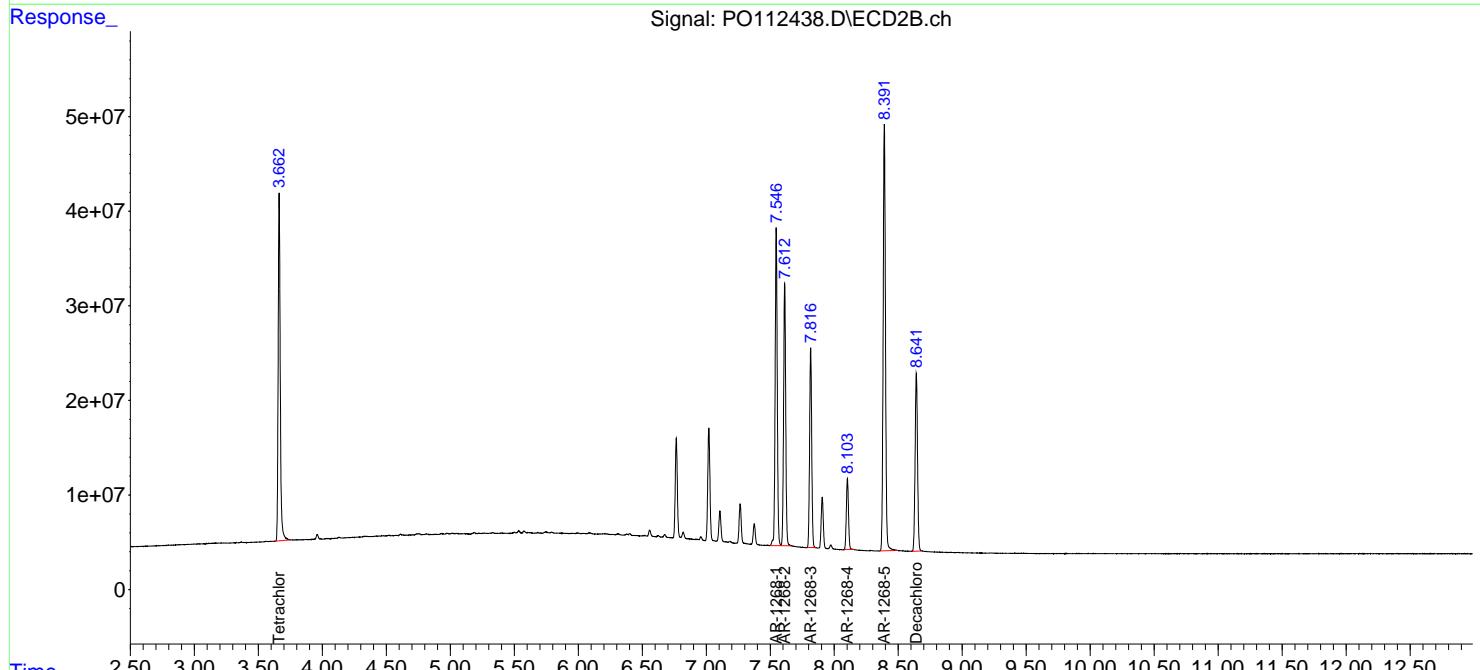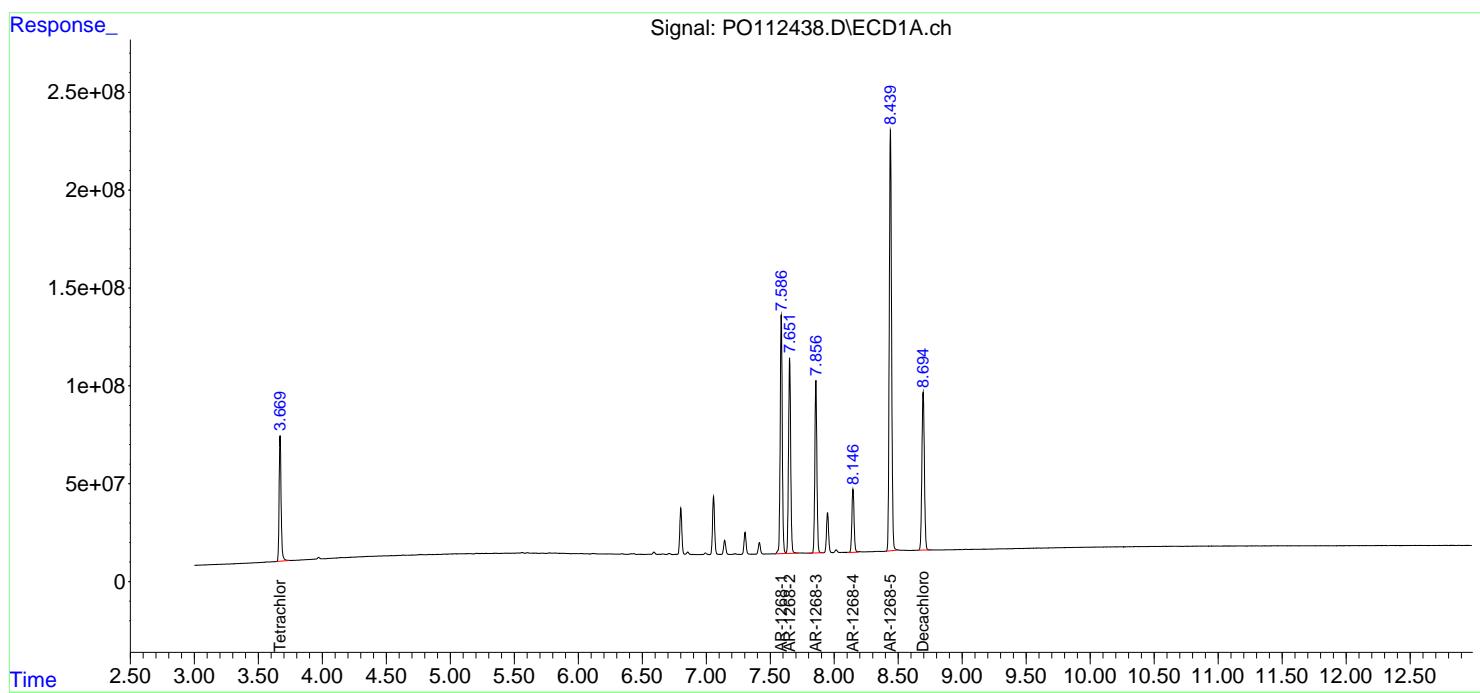

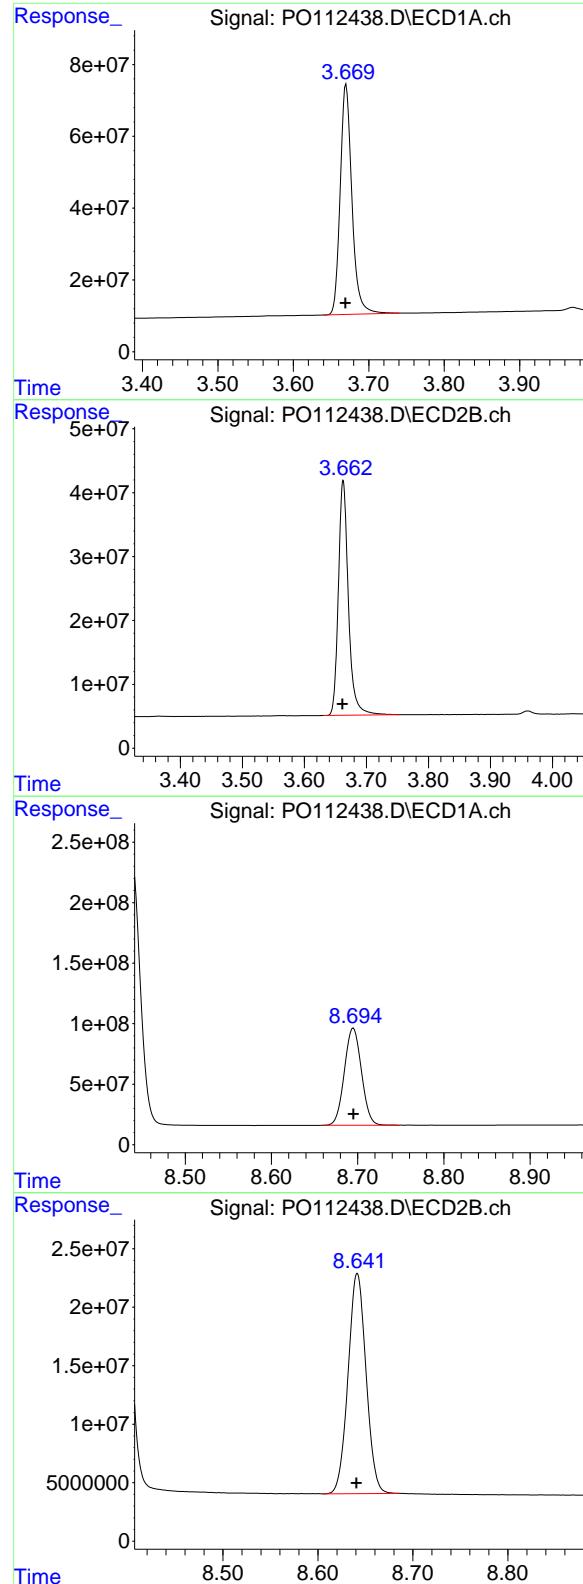

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 692243583
Conc: 74.66 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1268ICC750

#1 Tetrachloro-m-xylene


R.T.: 3.663 min
Delta R.T.: 0.001 min
Response: 413379353
Conc: 74.59 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 1101294529
Conc: 74.53 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 247569702
Conc: 73.87 ng/ml

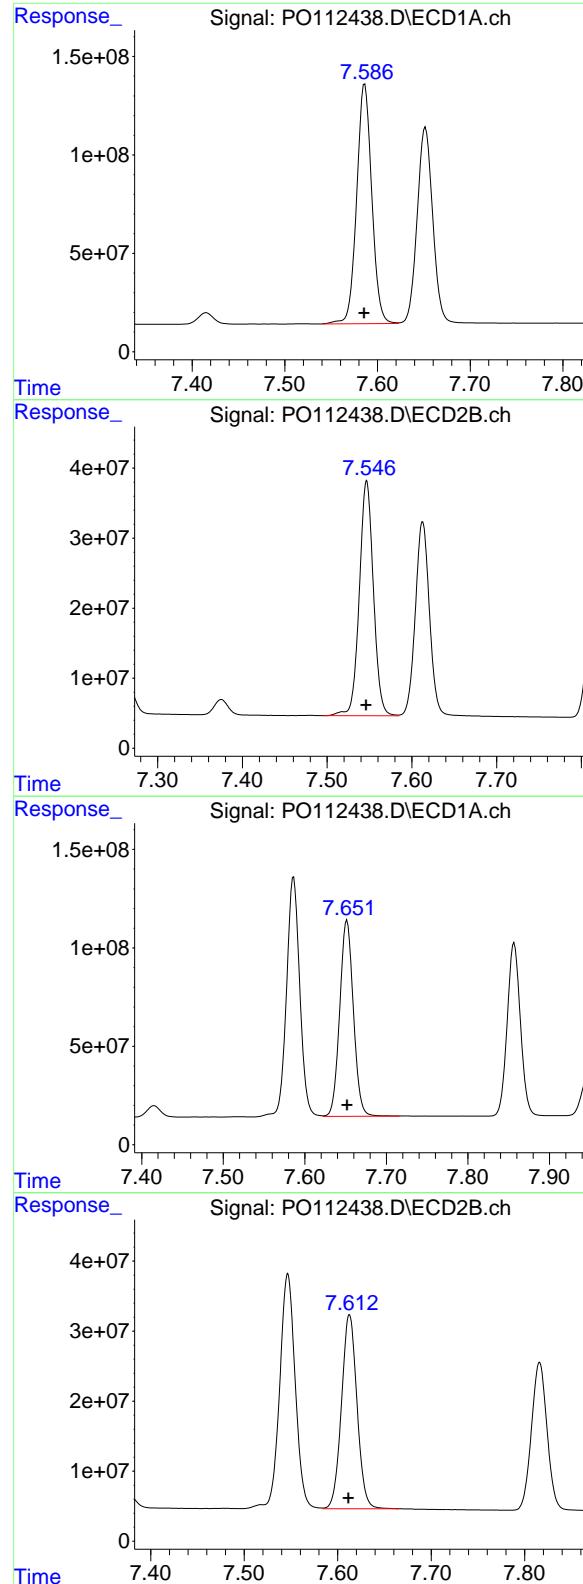

#41 AR-1268-1

R.T.: 7.586 min
Delta R.T.: 0.000 min
Instrument: ECD_O
Response: 1377694048
Conc: 744.48 ng/ml
ClientSampleId : AR1268ICC750

#41 AR-1268-1


R.T.: 7.547 min
Delta R.T.: 0.000 min
Response: 387521278
Conc: 727.42 ng/ml

#42 AR-1268-2

R.T.: 7.652 min
Delta R.T.: 0.000 min
Response: 1161145784
Conc: 744.68 ng/ml

#42 AR-1268-2

R.T.: 7.613 min
Delta R.T.: 0.001 min
Response: 319478450
Conc: 731.71 ng/ml

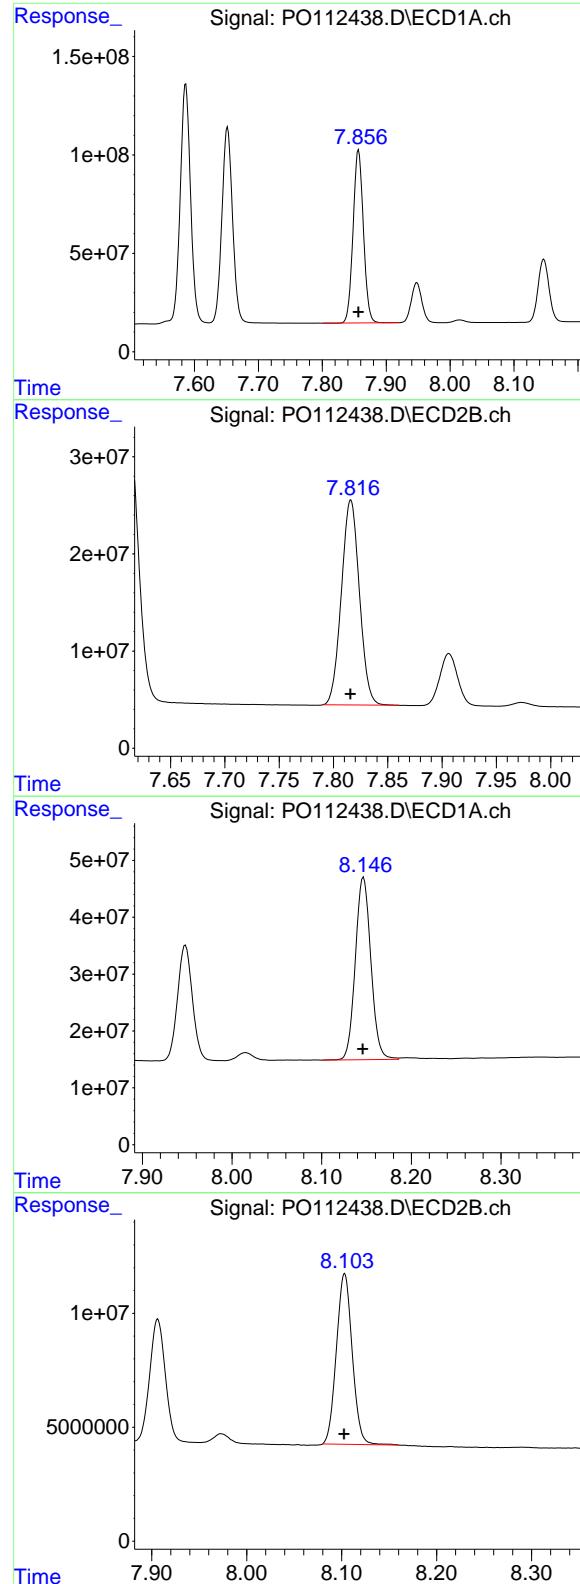

#43 AR-1268-3

R.T.: 7.857 min
 Delta R.T.: 0.000 min
 Response: 987117193
 Conc: 740.36 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC750

#43 AR-1268-3

R.T.: 7.816 min
 Delta R.T.: 0.000 min
 Response: 243379280
 Conc: 734.75 ng/ml

#44 AR-1268-4

R.T.: 8.147 min
 Delta R.T.: 0.000 min
 Response: 386370142
 Conc: 751.01 ng/ml



#44 AR-1268-4

R.T.: 8.103 min
 Delta R.T.: 0.000 min
 Response: 86779378
 Conc: 755.94 ng/ml

#45 AR-1268-5

R.T.: 8.439 min
Delta R.T.: 0.000 min
Response: 2676563187
Conc: 751.52 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC750

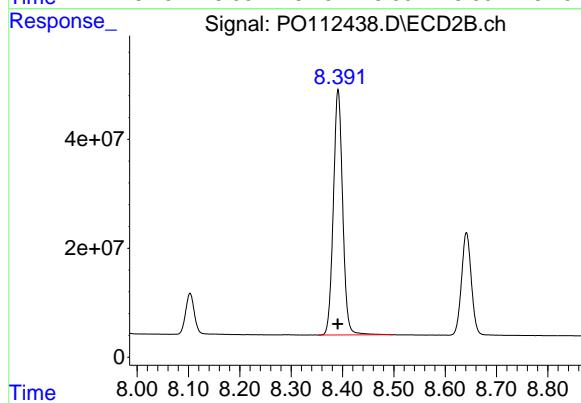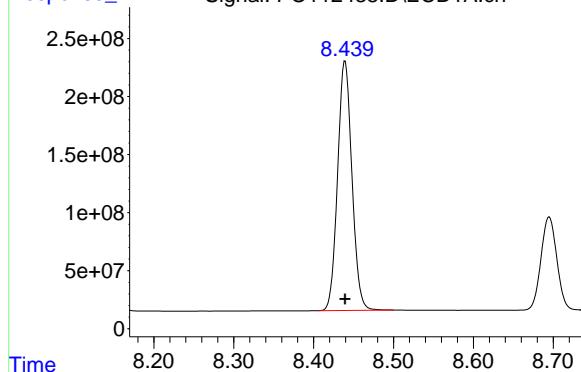

#45 AR-1268-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 567552223
Conc: 747.95 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 19:11
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.661 | 463.6E6 | 277.1E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 8.695 | 8.641 | 738.9E6 | 167.6E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 41) L9 AR-1268-1 | 7.586 | 7.546 | 925.3E6 | 266.4E6 | 500.000 | 500.000 |
| 42) L9 AR-1268-2 | 7.652 | 7.611 | 779.6E6 | 218.3E6 | 500.000 | 500.000 |
| 43) L9 AR-1268-3 | 7.857 | 7.816 | 666.6E6 | 165.6E6 | 500.000 | 500.000 |
| 44) L9 AR-1268-4 | 8.146 | 8.103 | 257.2E6 | 57398296 | 500.000 | 500.000 |
| 45) L9 AR-1268-5 | 8.439 | 8.391 | 1780.8E6 | 379.4E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 19:11
 Operator : YP/AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

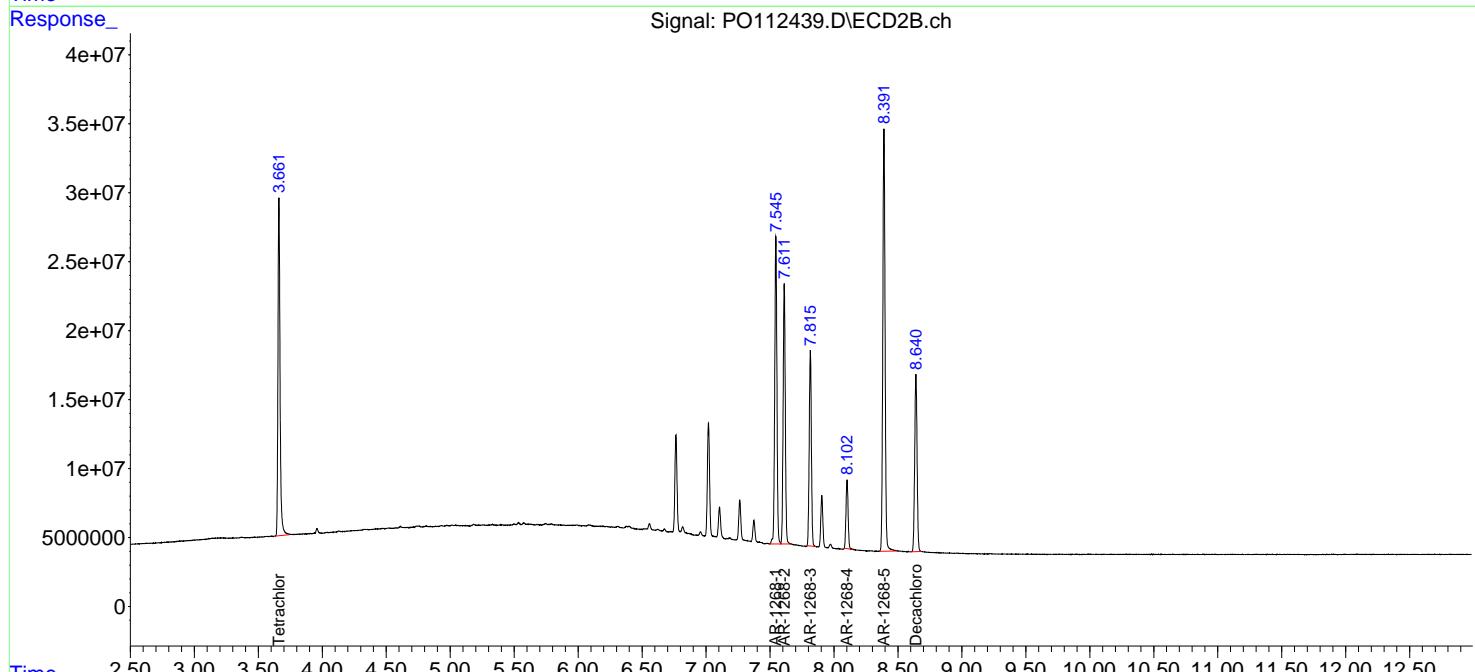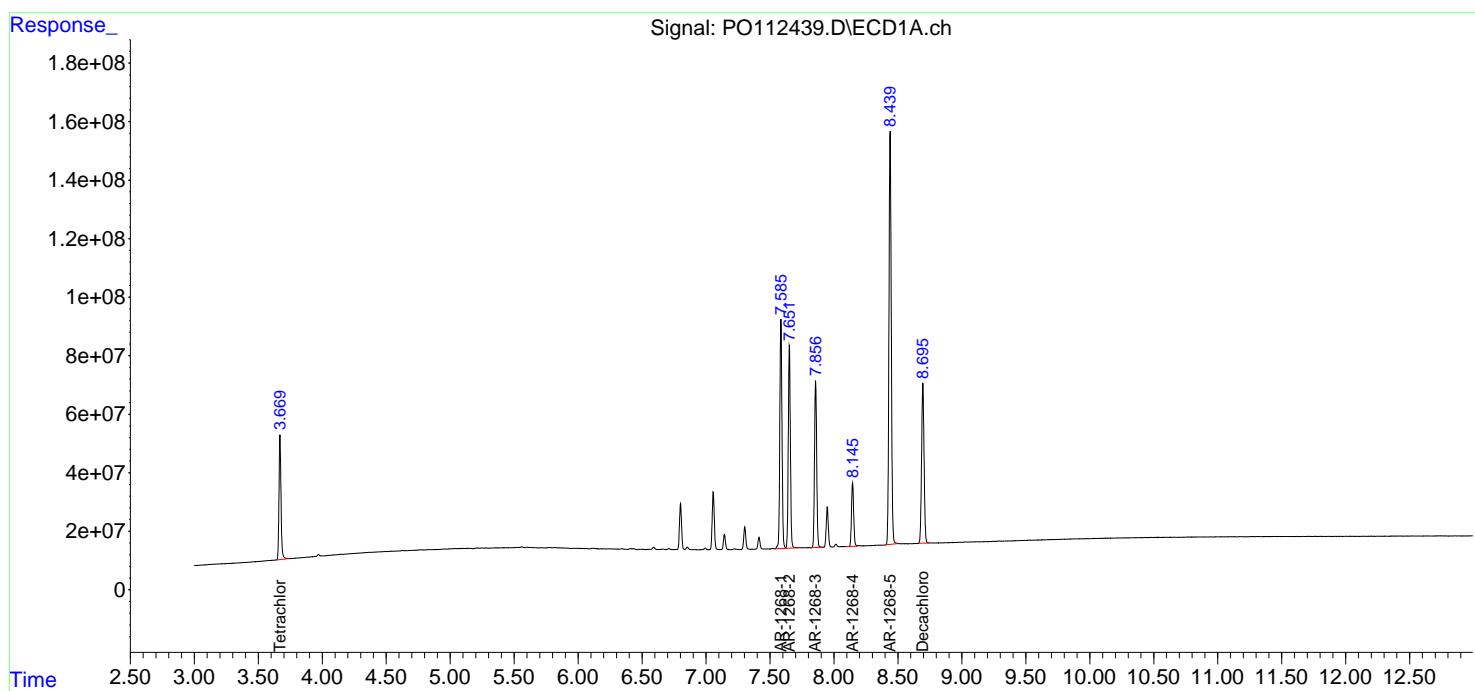

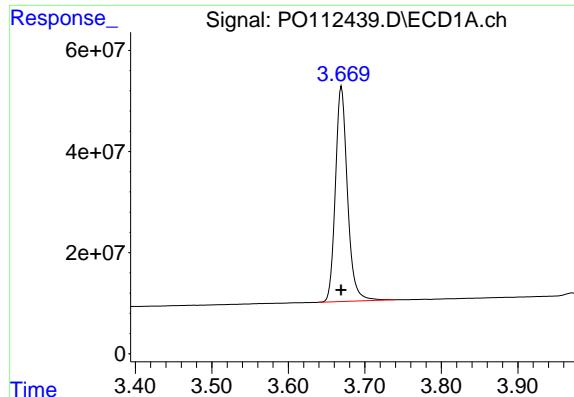

#1 Tetrachloro-m-xylene

R.T.: 3.669 min

Delta R.T.: 0.000 min

Response: 463571552


Conc: 50.00 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1268ICC500

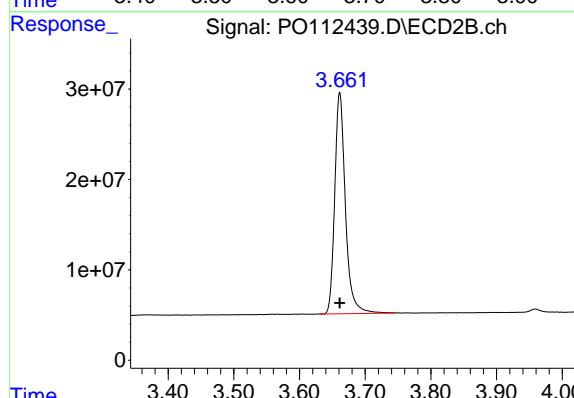


#1 Tetrachloro-m-xylene

R.T.: 3.661 min

Delta R.T.: 0.000 min

Response: 277095695

Conc: 50.00 ng/ml

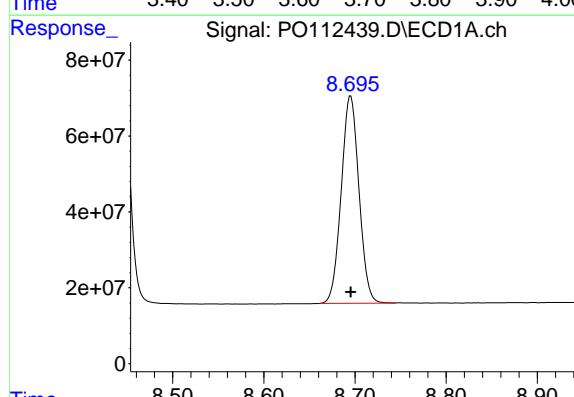


#2 Decachlorobiphenyl

R.T.: 8.695 min

Delta R.T.: 0.000 min

Response: 738865285

Conc: 50.00 ng/ml

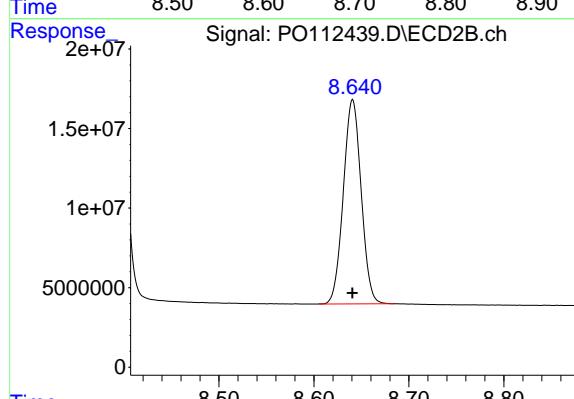

#2 Decachlorobiphenyl

R.T.: 8.641 min

Delta R.T.: 0.000 min


Response: 167569760

Conc: 50.00 ng/ml

#41 AR-1268-1


R.T.: 7.586 min
 Delta R.T.: 0.000 min
 Response: 925267424
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

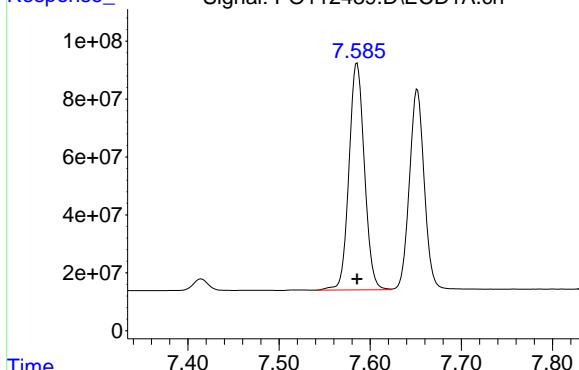


#41 AR-1268-1

R.T.: 7.546 min
 Delta R.T.: 0.000 min
 Response: 266367686
 Conc: 500.00 ng/ml

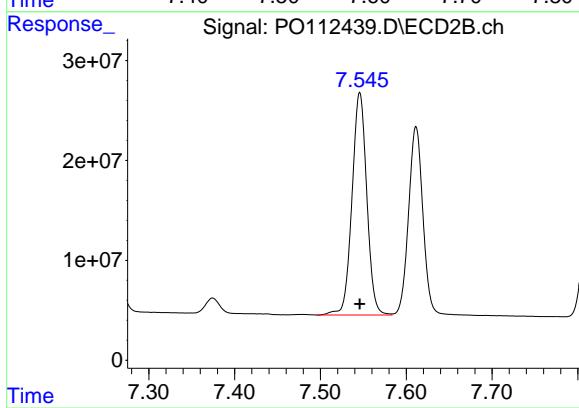


#42 AR-1268-2

R.T.: 7.652 min
 Delta R.T.: 0.000 min
 Response: 779627980
 Conc: 500.00 ng/ml

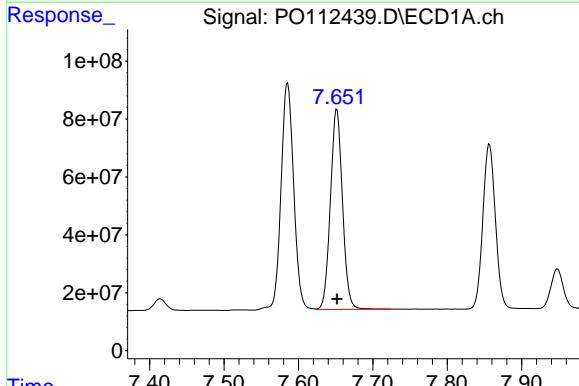

#42 AR-1268-2


R.T.: 7.611 min
 Delta R.T.: 0.000 min
 Response: 218309426
 Conc: 500.00 ng/ml

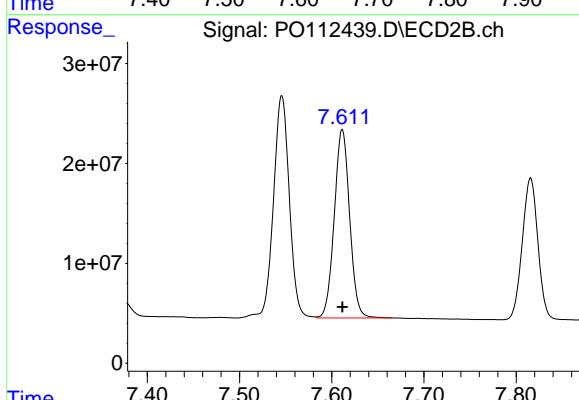

#43 AR-1268-3


R.T.: 7.857 min
 Delta R.T.: 0.000 min
 Response: 666647907
 Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

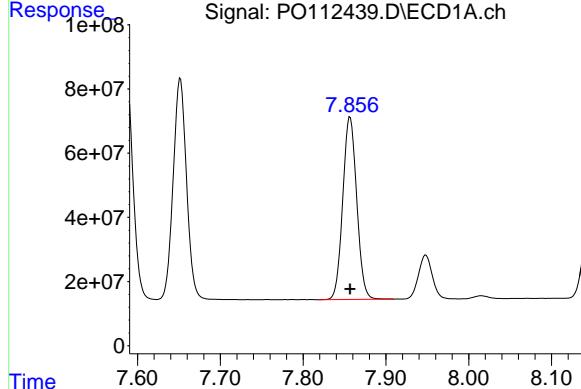


#43 AR-1268-3

R.T.: 7.816 min
 Delta R.T.: 0.000 min
 Response: 165620938
 Conc: 500.00 ng/ml

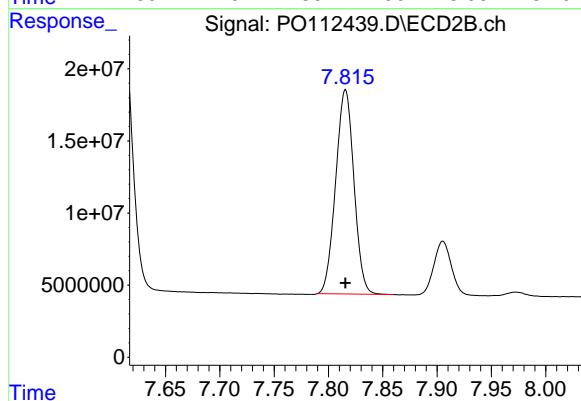


#44 AR-1268-4

R.T.: 8.146 min
 Delta R.T.: 0.000 min
 Response: 257233514
 Conc: 500.00 ng/ml

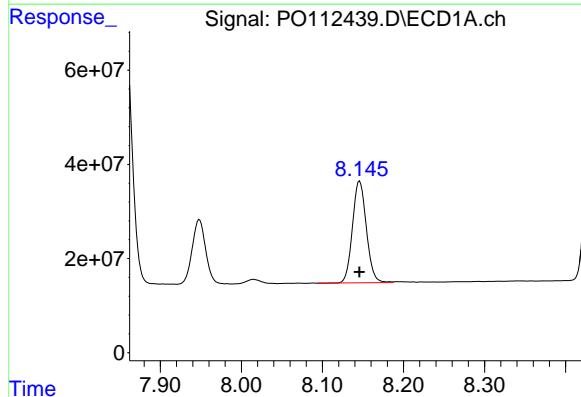

#44 AR-1268-4


R.T.: 8.103 min
 Delta R.T.: 0.000 min
 Response: 57398296
 Conc: 500.00 ng/ml

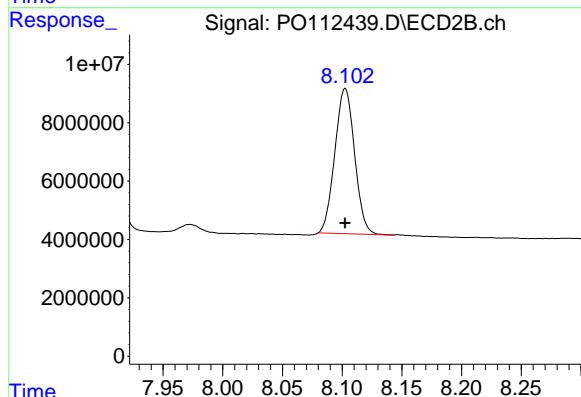

#45 AR-1268-5

R.T.: 8.439 min
Delta R.T.: 0.000 min
Response: 1780763954
Conc: 500.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC500

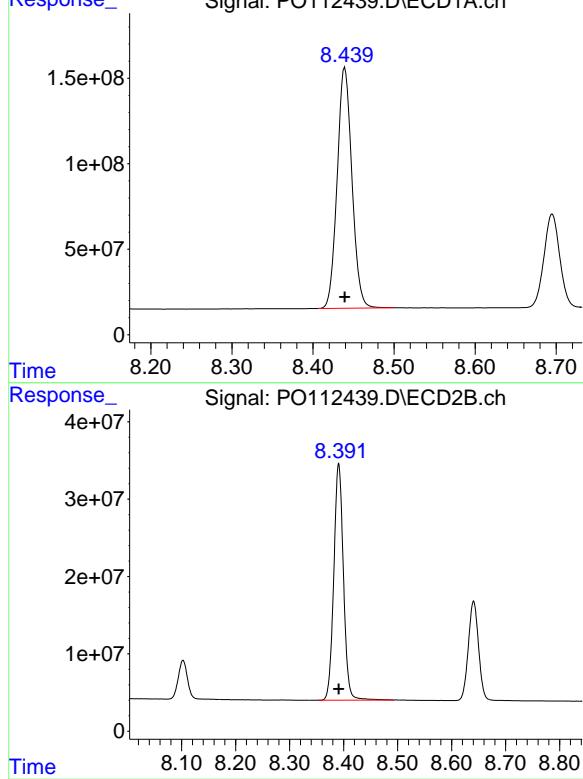

#45 AR-1268-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 379404270
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 19:28
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.668 | 3.663 | 233.9E6 | 141.8E6 | 25.226 | 25.590 |
| 2) SA Decachlor... | 8.693 | 8.640 | 370.0E6 | 87026360 | 25.041 | 25.967 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 41) L9 AR-1268-1 | 7.584 | 7.546 | 463.2E6 | 137.9E6 | 250.297 | 258.785 |
| 42) L9 AR-1268-2 | 7.649 | 7.611 | 391.7E6 | 113.6E6 | 251.211 | 260.244 |
| 43) L9 AR-1268-3 | 7.855 | 7.815 | 332.3E6 | 86494420 | 249.235 | 261.122 |
| 44) L9 AR-1268-4 | 8.144 | 8.102 | 129.0E6 | 30404180 | 250.733 | 264.853 |
| 45) L9 AR-1268-5 | 8.438 | 8.390 | 884.1E6 | 195.1E6 | 248.250 | 257.124 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 19:28
 Operator : YP/AJ
 Sample : AR1268ICC250
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:32 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

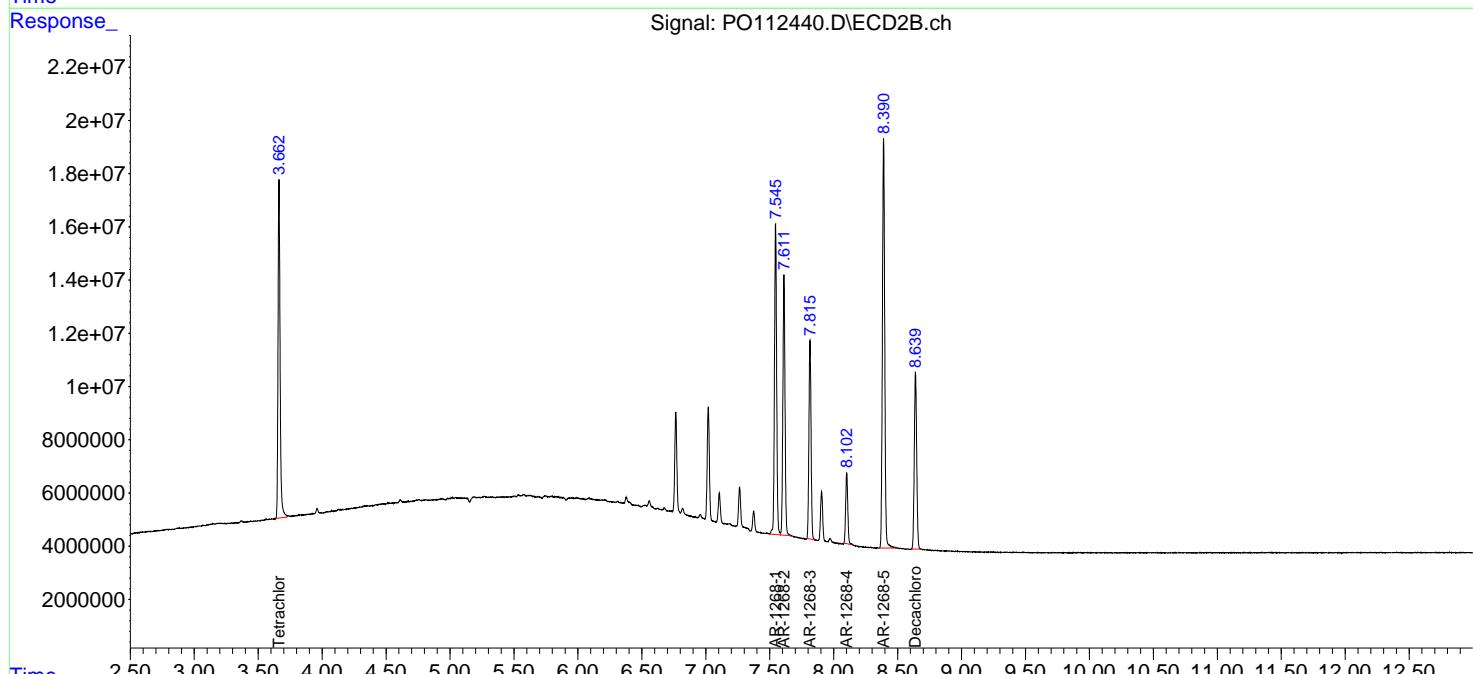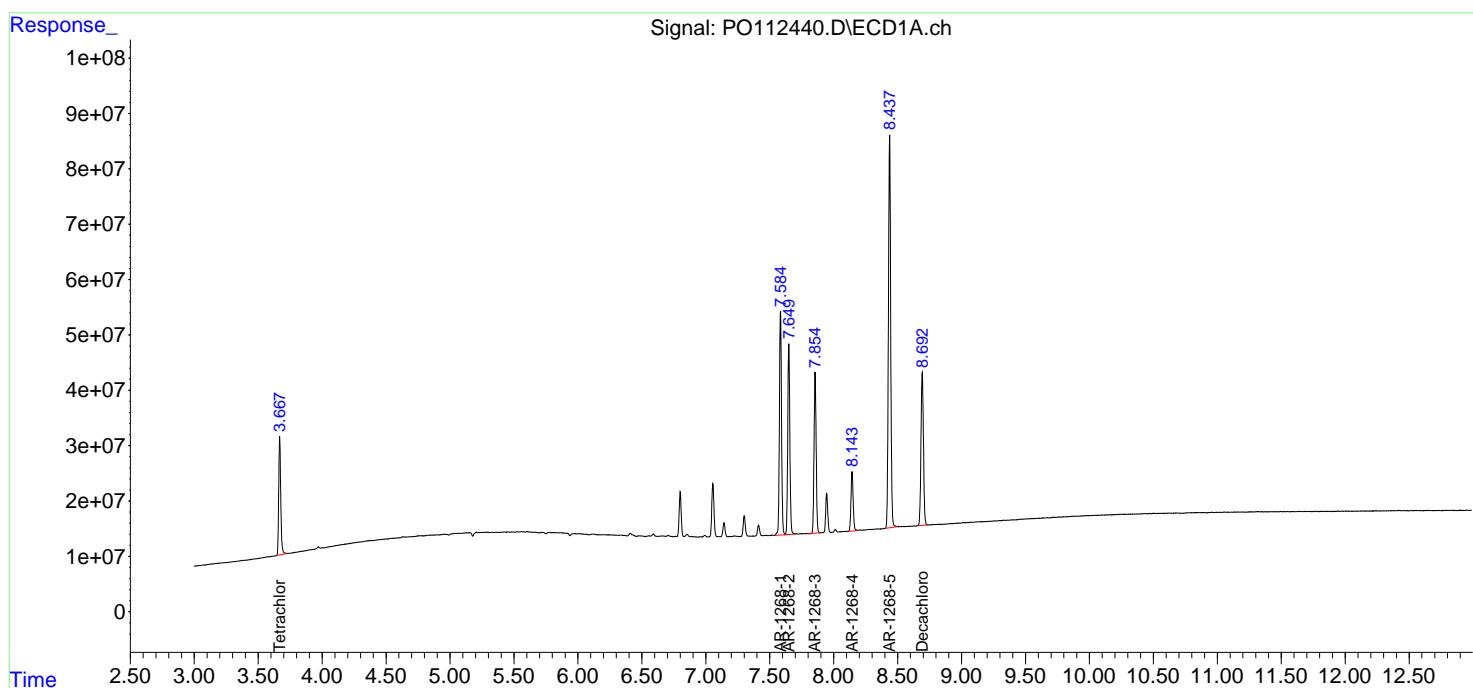

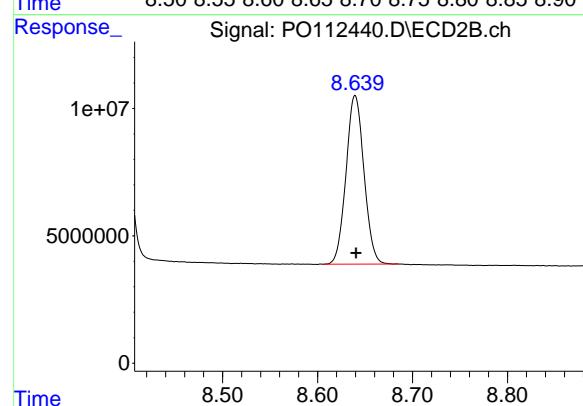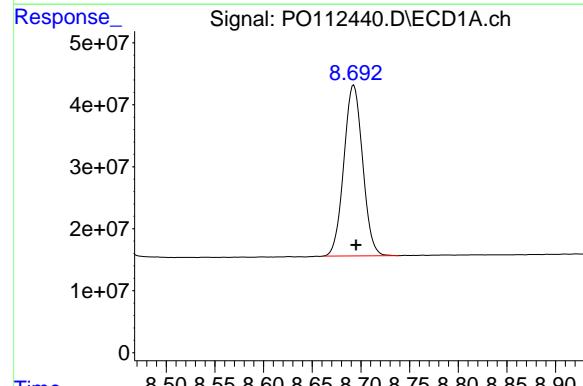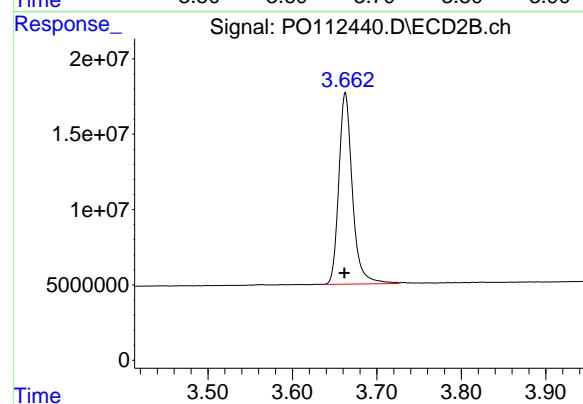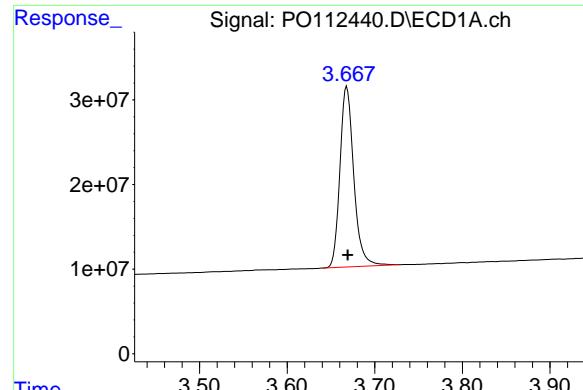

#1 Tetrachloro-m-xylene

R.T.: 3.668 min
Delta R.T.: 0.000 min
Response: 233878715
Conc: 25.23 ng/ml

Instrument: ECD_O
ClientSampleId : AR1268ICC250

#1 Tetrachloro-m-xylene





R.T.: 3.663 min
Delta R.T.: 0.001 min
Response: 141818532
Conc: 25.59 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: -0.003 min
Response: 370038692
Conc: 25.04 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: -0.001 min
Response: 87026360
Conc: 25.97 ng/ml

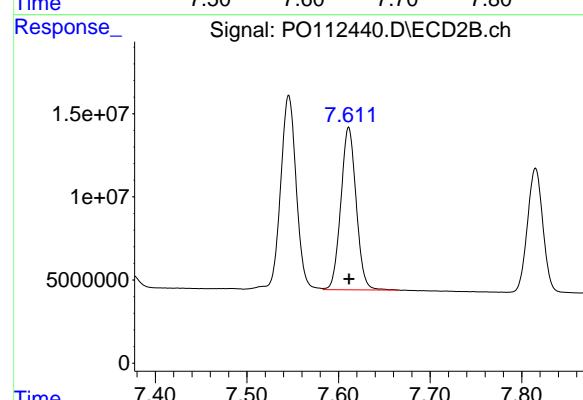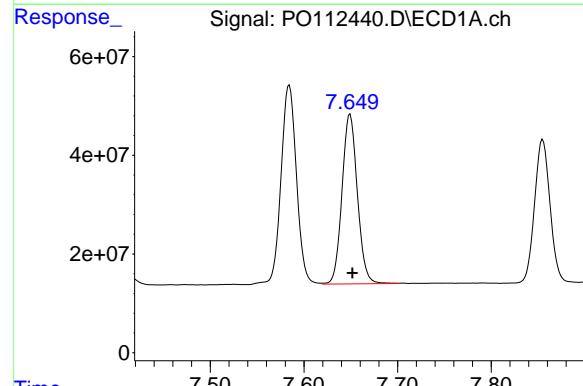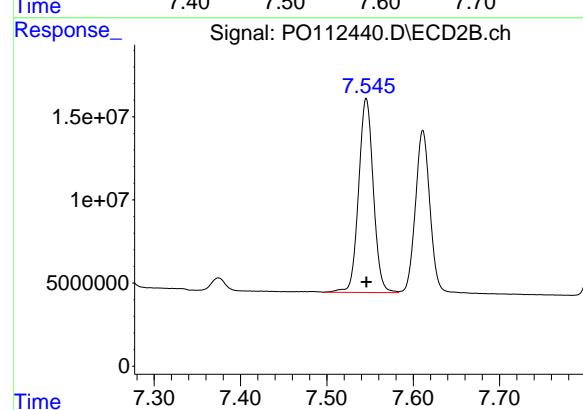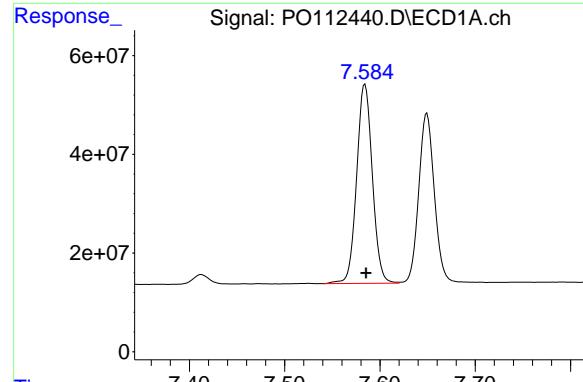

#41 AR-1268-1

R.T.: 7.584 min
 Delta R.T.: -0.001 min
 Response: 463182645
 Conc: 250.30 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1268ICC250

#41 AR-1268-1

R.T.: 7.546 min
 Delta R.T.: 0.000 min
 Response: 137863994
 Conc: 258.79 ng/ml

#42 AR-1268-2

R.T.: 7.649 min
 Delta R.T.: -0.002 min
 Response: 391701543
 Conc: 251.21 ng/ml





#42 AR-1268-2

R.T.: 7.611 min
 Delta R.T.: 0.000 min
 Response: 113627398
 Conc: 260.24 ng/ml

#43 AR-1268-3

R.T.: 7.855 min
 Delta R.T.: -0.002 min
 Response: 332303997
 Conc: 249.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC250

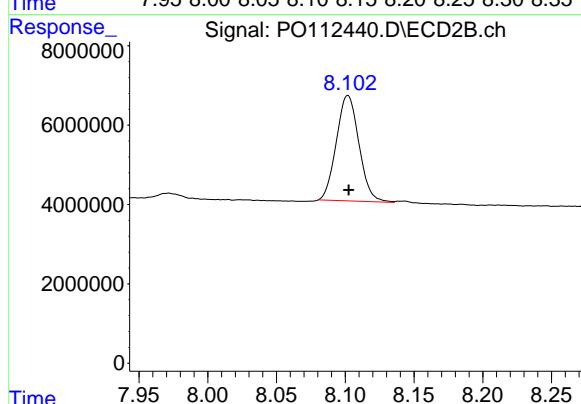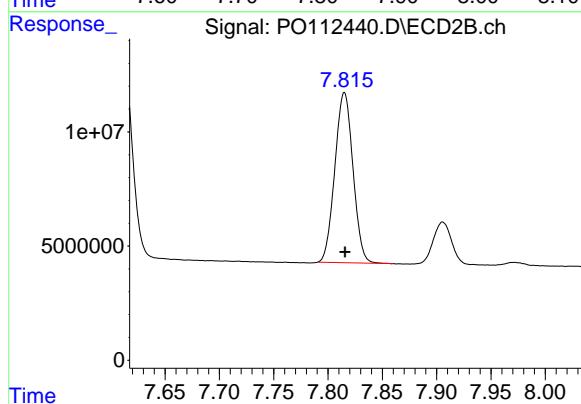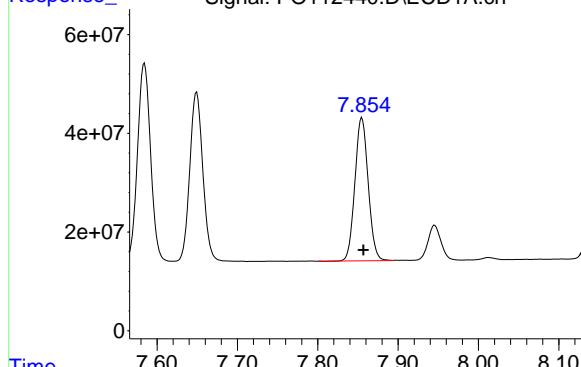

#43 AR-1268-3

R.T.: 7.815 min
 Delta R.T.: 0.000 min
 Response: 86494420
 Conc: 261.12 ng/ml

#44 AR-1268-4

R.T.: 8.144 min
 Delta R.T.: -0.002 min
 Response: 128993948
 Conc: 250.73 ng/ml



#44 AR-1268-4

R.T.: 8.102 min
 Delta R.T.: 0.000 min
 Response: 30404180
 Conc: 264.85 ng/ml

#45 AR-1268-5

R.T.: 8.438 min
Delta R.T.: -0.002 min
Response: 884148704
Conc: 248.25 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC250

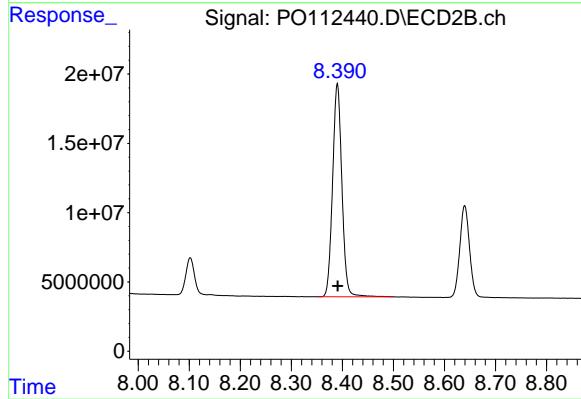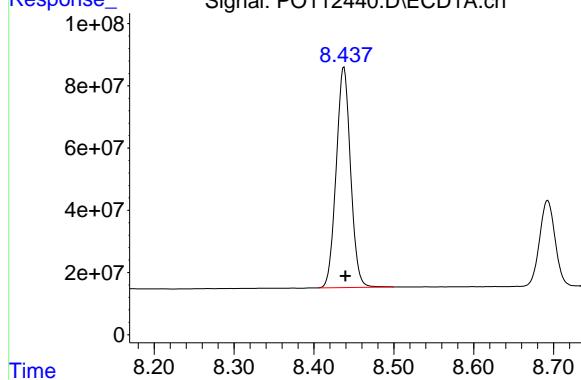

#45 AR-1268-5

R.T.: 8.390 min
Delta R.T.: 0.000 min
Response: 195108104
Conc: 257.12 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 19:47
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 32580103 | 20954895 | 3.514 | 3.781 |
| 2) SA Decachlor... | 8.695 | 8.641 | 54814922 | 13633947 | 3.709 | 4.068 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|--------|--------|
| 41) L9 AR-1268-1 | 7.587 | 7.546 | 70515596 | 23692896 | 38.106 | 44.474 |
| 42) L9 AR-1268-2 | 7.653 | 7.612 | 58352509 | 19332274 | 37.423 | 44.277 |
| 43) L9 AR-1268-3 | 7.857 | 7.816 | 49192646 | 14292573 | 36.896 | 43.148 |
| 44) L9 AR-1268-4 | 8.148 | 8.103 | 18069640 | 4642090 | 35.123 | 40.438 |
| 45) L9 AR-1268-5 | 8.441 | 8.391 | 129.1E6 | 30999751 | 36.236 | 40.853 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112441.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 19:47
 Operator : YP/AJ
 Sample : AR1268ICC050
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1268ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:27:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:26:17 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

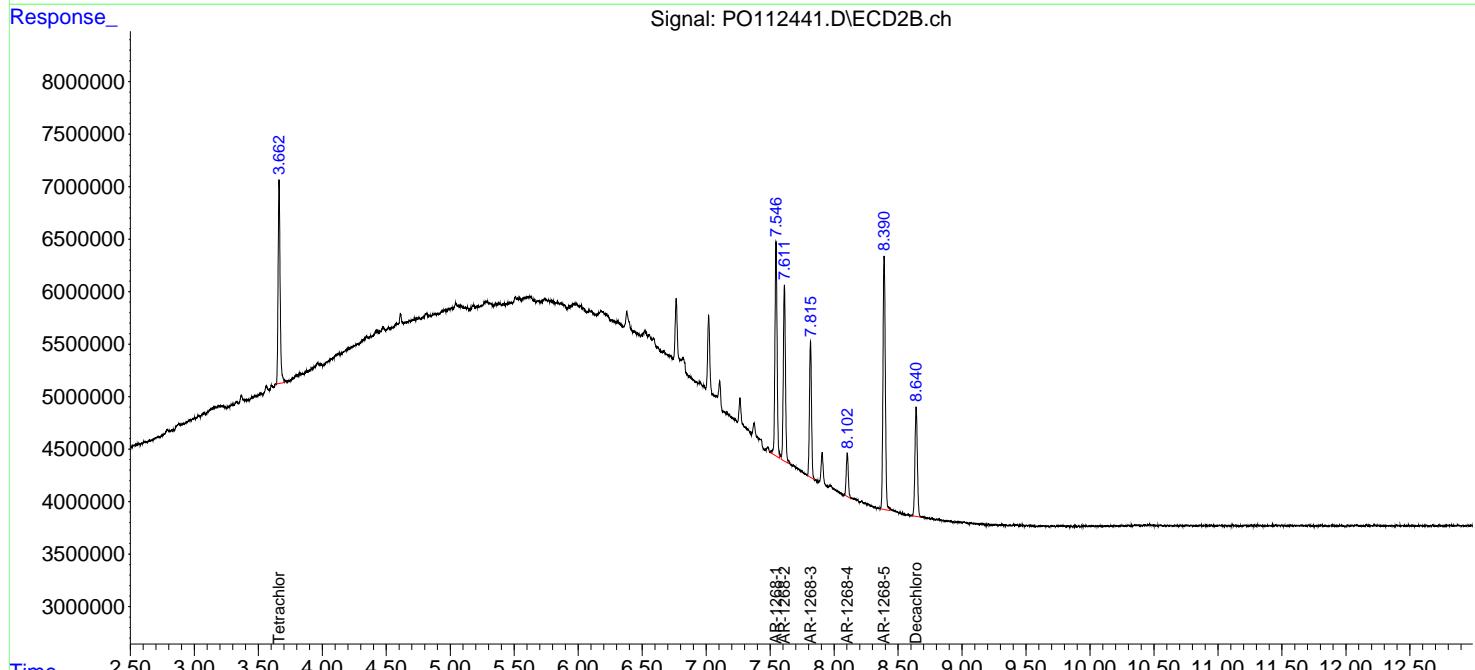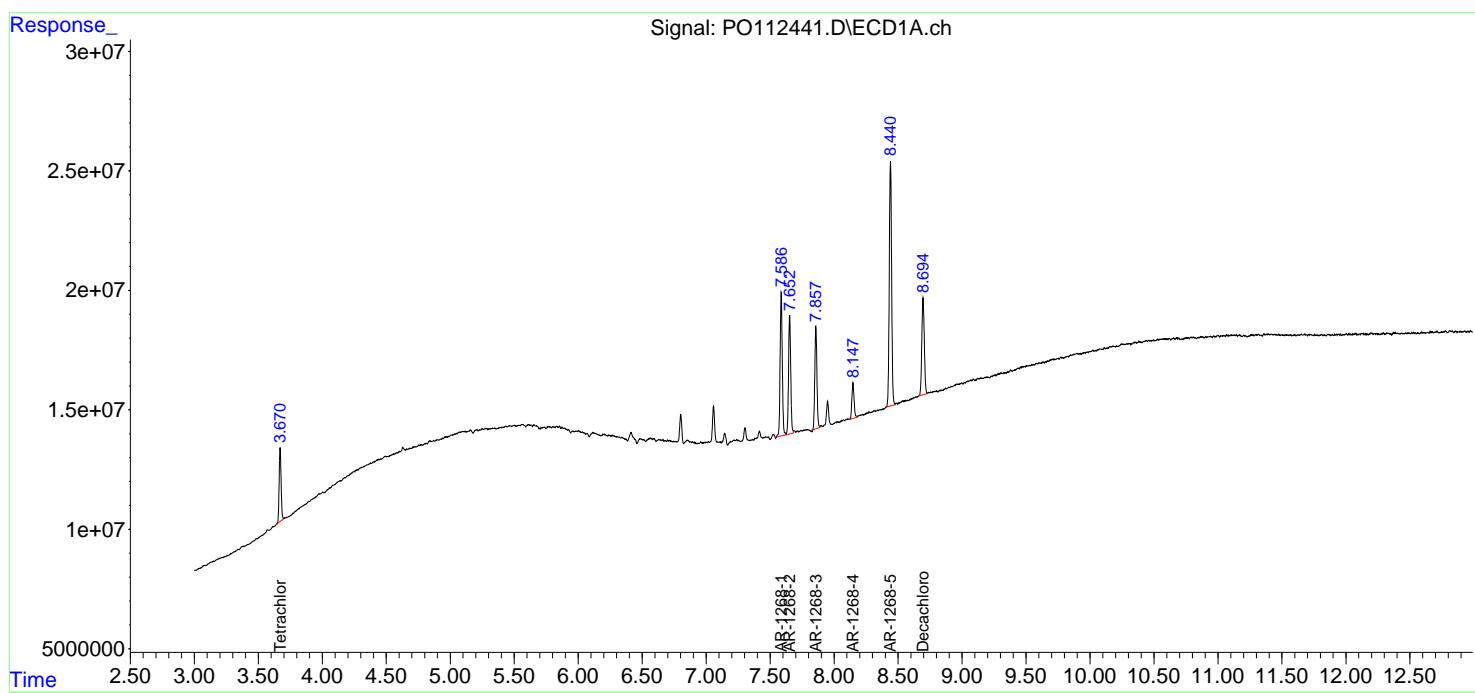

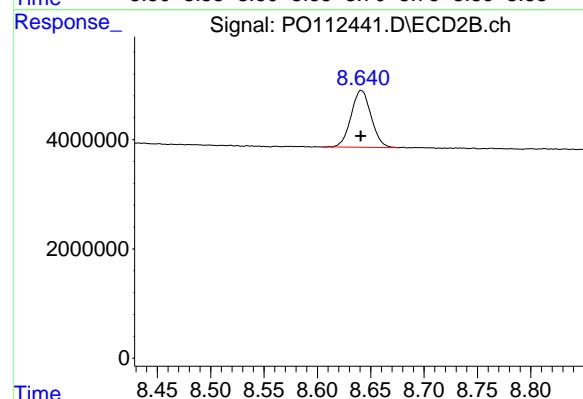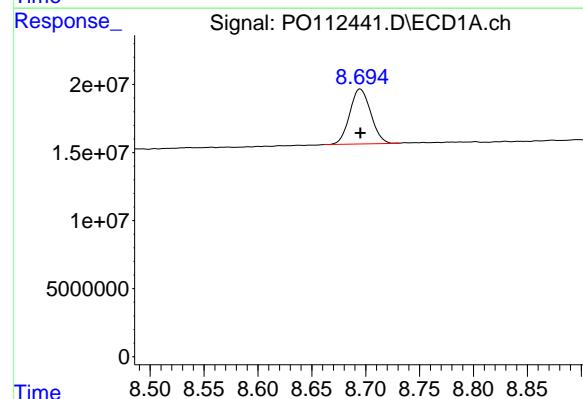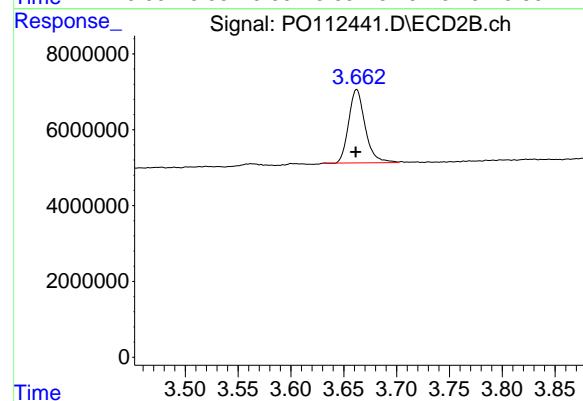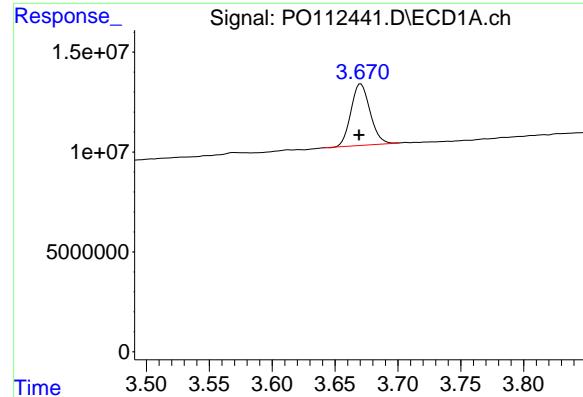

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.001 min
Response: 32580103
Conc: 3.51 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1268ICC050

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 20954895
Conc: 3.78 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 54814922
Conc: 3.71 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 13633947
Conc: 4.07 ng/ml

#41 AR-1268-1


R.T.: 7.587 min
 Delta R.T.: 0.001 min
 Response: 70515596
 Conc: 38.11 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050




#41 AR-1268-1

R.T.: 7.546 min
 Delta R.T.: 0.000 min
 Response: 23692896
 Conc: 44.47 ng/ml

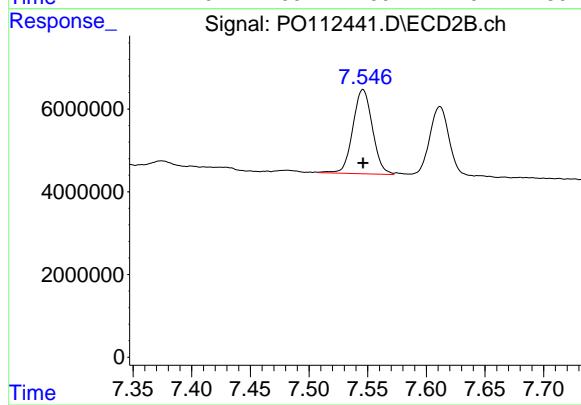


#42 AR-1268-2


R.T.: 7.653 min
 Delta R.T.: 0.001 min
 Response: 58352509
 Conc: 37.42 ng/ml



#42 AR-1268-2

R.T.: 7.612 min
 Delta R.T.: 0.000 min
 Response: 19332274
 Conc: 44.28 ng/ml

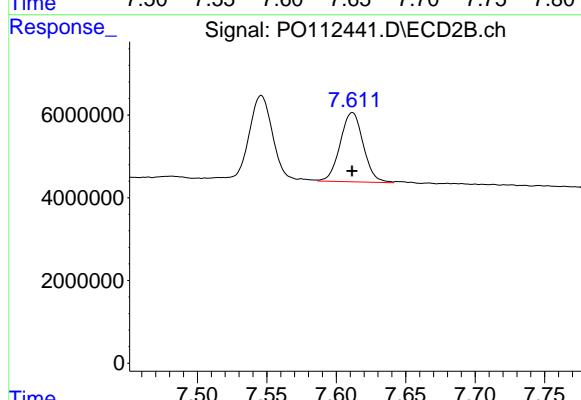

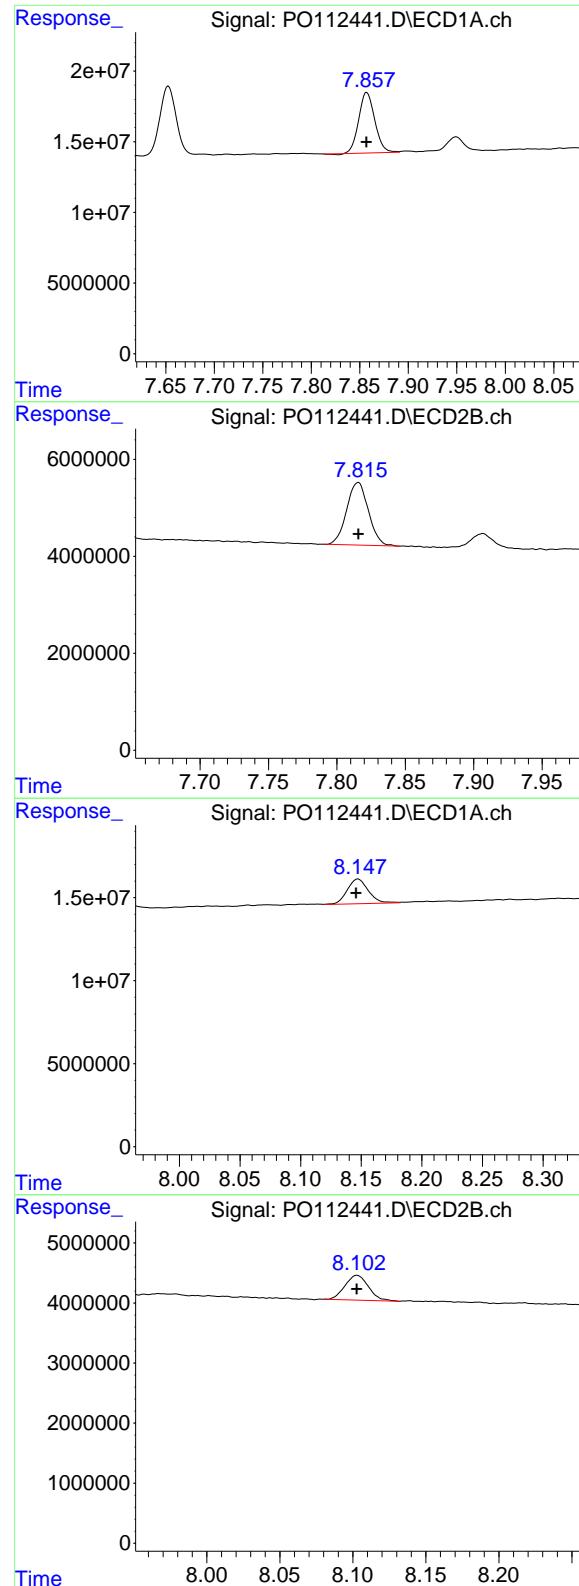

#43 AR-1268-3

R.T.: 7.857 min
 Delta R.T.: 0.000 min
 Response: 49192646
 Conc: 36.90 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1268ICC050

#43 AR-1268-3


R.T.: 7.816 min
 Delta R.T.: 0.000 min
 Response: 14292573
 Conc: 43.15 ng/ml

#44 AR-1268-4

R.T.: 8.148 min
 Delta R.T.: 0.002 min
 Response: 18069640
 Conc: 35.12 ng/ml

#44 AR-1268-4

R.T.: 8.103 min
 Delta R.T.: 0.000 min
 Response: 4642090
 Conc: 40.44 ng/ml

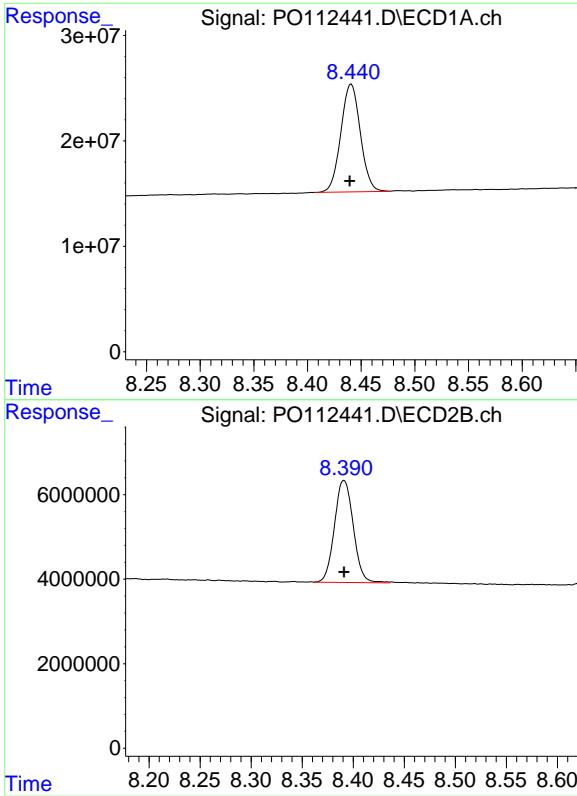

#45 AR-1268-5

R.T.: 8.441 min
Delta R.T.: 0.002 min
Response: 129056827
Conc: 36.24 ng/ml

Instrument: ECD_O
ClientSampleId: AR1268ICC050

#45 AR-1268-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 30999751
Conc: 40.85 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 20:05
 Operator : YP/AJ
 Sample : P0072325ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:04:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 429.5E6 | 257.8E6 | 52.813 | 51.889 |
| 2) SA Decachlor... | 8.695 | 8.640 | 375.0E6 | 87671423 | 51.286 | 49.613 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|---------|
| 3) L1 AR-1016-1 | 4.756 | 4.737 | 141.9E6 | 87193424 | 528.782 | 498.228 |
| 4) L1 AR-1016-2 | 4.774 | 4.756 | 214.8E6 | 130.5E6 | 528.864 | 500.904 |
| 5) L1 AR-1016-3 | 4.832 | 4.931 | 137.7E6 | 68749292 | 526.111 | 505.634 |
| 6) L1 AR-1016-4 | 4.951 | 4.973 | 109.7E6 | 56111590 | 517.883 | 505.124 |
| 7) L1 AR-1016-5 | 5.208 | 5.186 | 116.9E6 | 72935368 | 532.523 | 508.959 |
| 31) L7 AR-1260-1 | 6.245 | 6.214 | 222.6E6 | 126.1E6 | 506.590 | 507.535 |
| 32) L7 AR-1260-2 | 6.435 | 6.402 | 342.3E6 | 162.4E6 | 497.536 | 492.983 |
| 33) L7 AR-1260-3 | 6.800 | 6.553 | 311.1E6 | 133.0E6 | 528.992 | 517.596 |
| 34) L7 AR-1260-4 | 7.059 | 7.023 | 226.3E6 | 98281247 | 501.824 | 513.726 |
| 35) L7 AR-1260-5 | 7.303 | 7.265 | 621.4E6 | 214.6E6 | 501.504 | 520.509 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 20:05
 Operator : YP/AJ
 Sample : P0072325ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_O
ClientSampleId :
 ICVPO072325

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:04:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

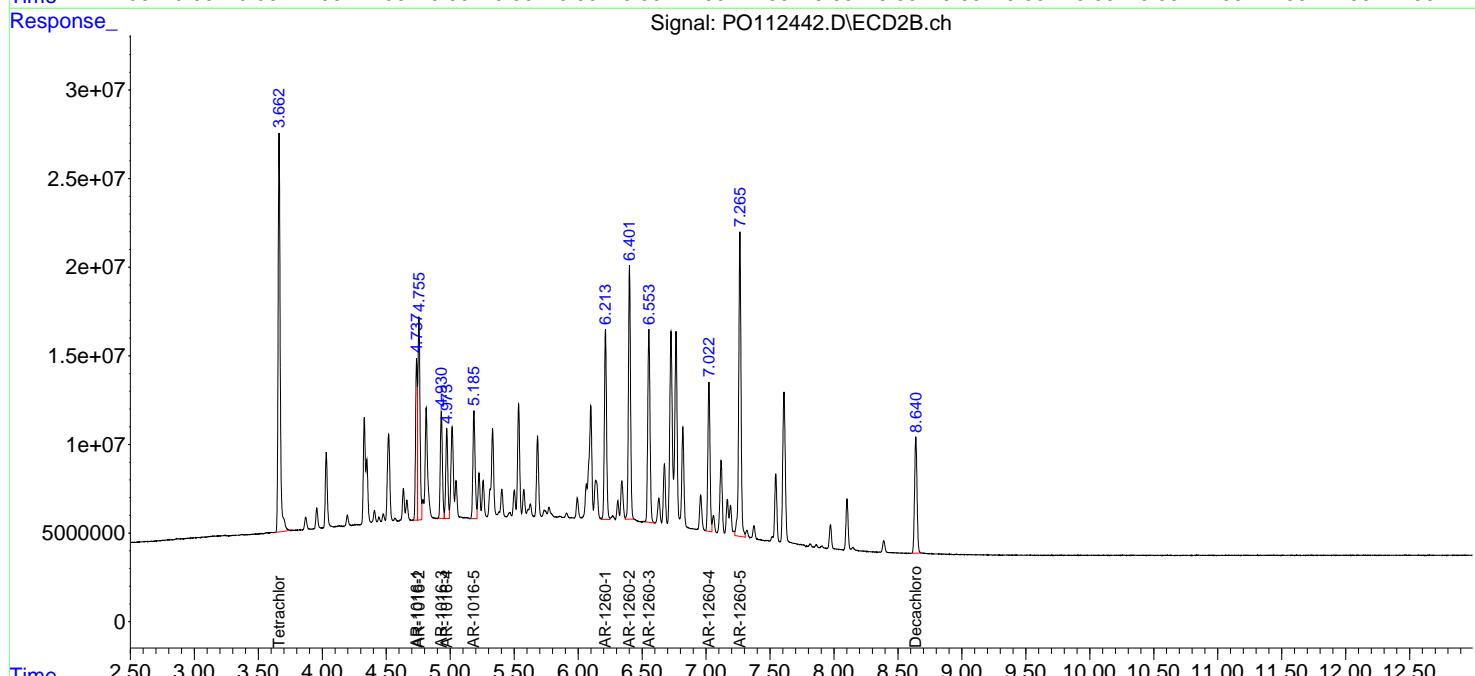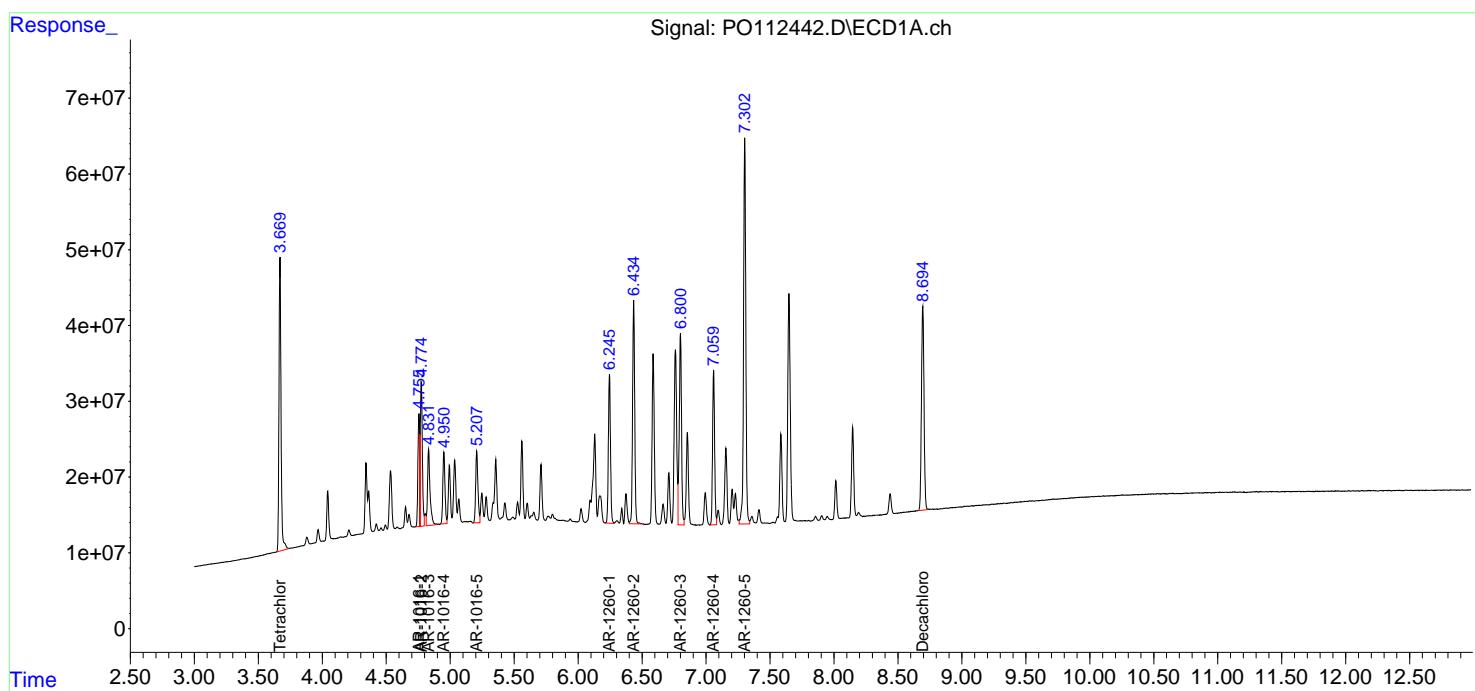

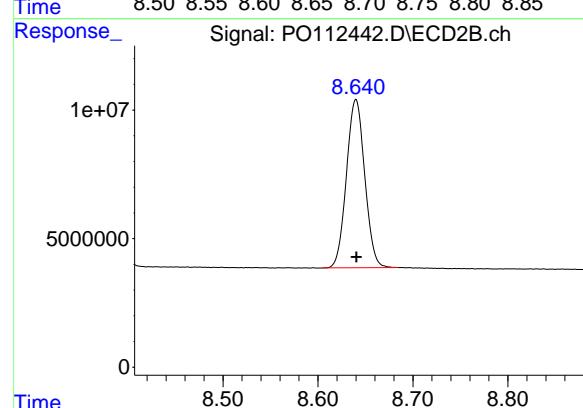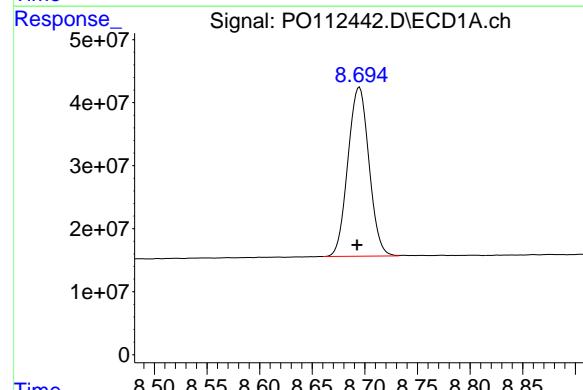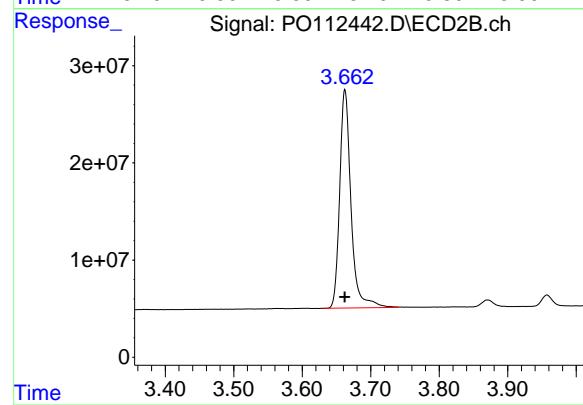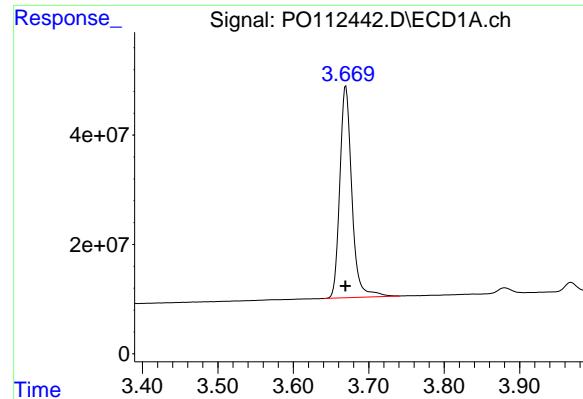

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 429455402
Conc: 52.81 ng/ml

Instrument:

ECD_O

ClientSampleId :

ICVPO072325

#1 Tetrachloro-m-xylene


R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 257845809
Conc: 51.89 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.002 min
Response: 374991509
Conc: 51.29 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 87671423
Conc: 49.61 ng/ml

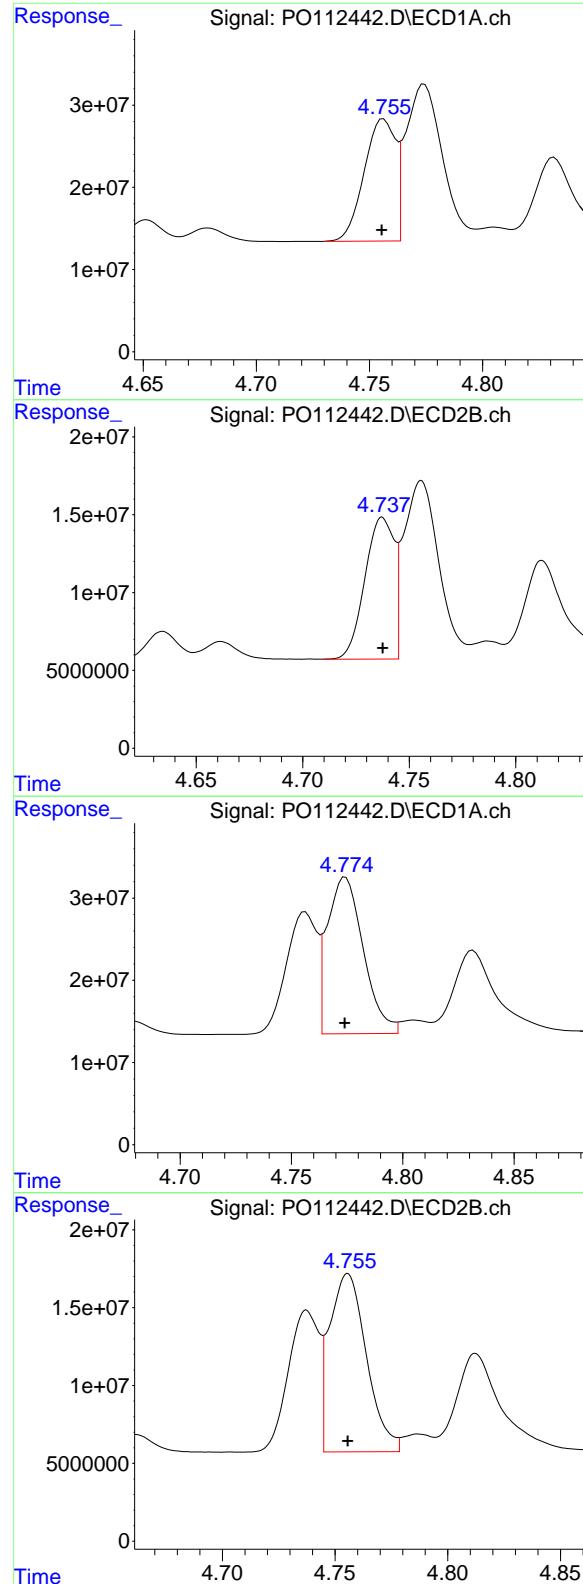

#3 AR-1016-1

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 141906938
 Conc: 528.78 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO072325

#3 AR-1016-1

R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 87193424
 Conc: 498.23 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 214780855
 Conc: 528.86 ng/ml





#4 AR-1016-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 130482985
 Conc: 500.90 ng/ml

#5 AR-1016-3

R.T.: 4.832 min
 Delta R.T.: 0.000 min
 Response: 137669441
 Conc: 526.11 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325

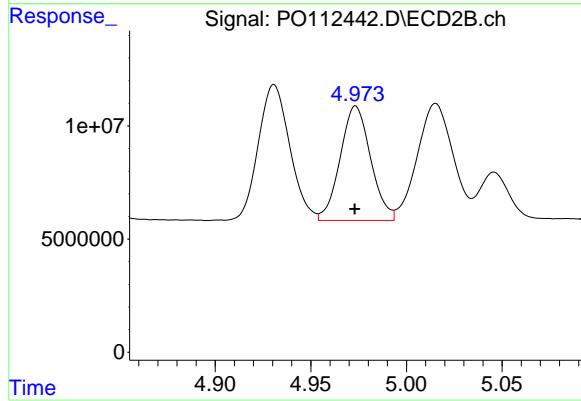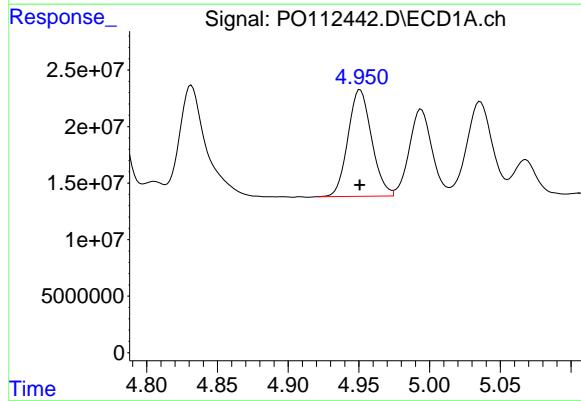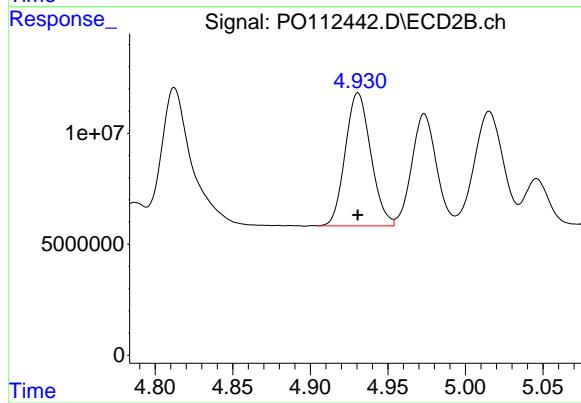

#5 AR-1016-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 68749292
 Conc: 505.63 ng/ml

#6 AR-1016-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 109709153
 Conc: 517.88 ng/ml


#6 AR-1016-4

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 56111590
 Conc: 505.12 ng/ml

#7 AR-1016-5


R.T.: 5.208 min
 Delta R.T.: 0.000 min
 Response: 116873095
 Conc: 532.52 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO072325




#7 AR-1016-5

R.T.: 5.186 min
 Delta R.T.: 0.000 min
 Response: 72935368
 Conc: 508.96 ng/ml

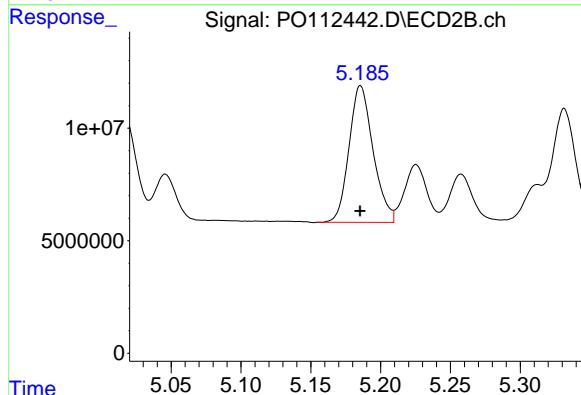


#31 AR-1260-1

R.T.: 6.245 min
 Delta R.T.: 0.000 min
 Response: 222560513
 Conc: 506.59 ng/ml

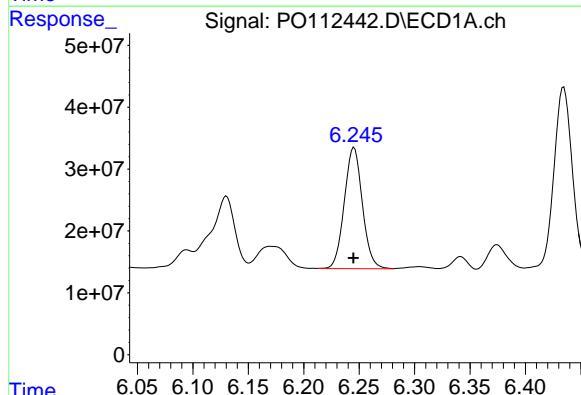

#31 AR-1260-1





R.T.: 6.214 min
 Delta R.T.: 0.000 min
 Response: 126128146
 Conc: 507.54 ng/ml

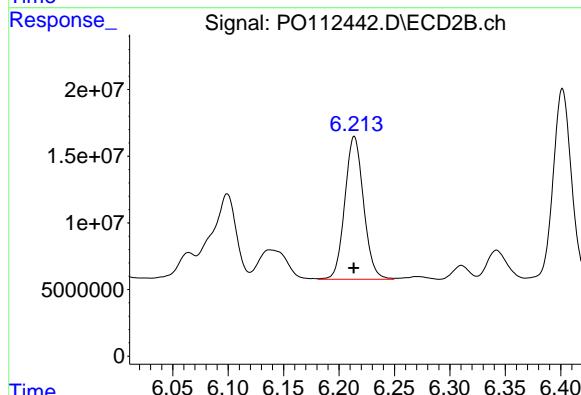

#32 AR-1260-2

R.T.: 6.435 min
 Delta R.T.: 0.001 min
 Response: 342251594
 Conc: 497.54 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325

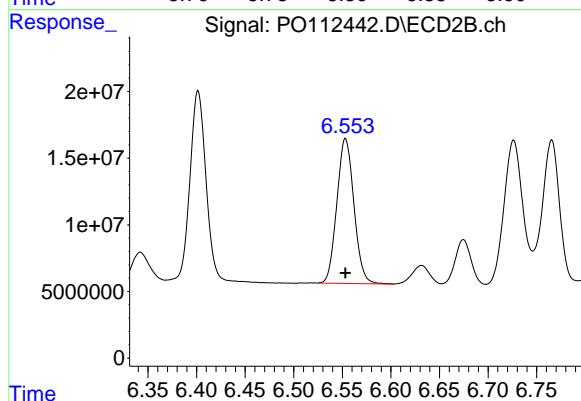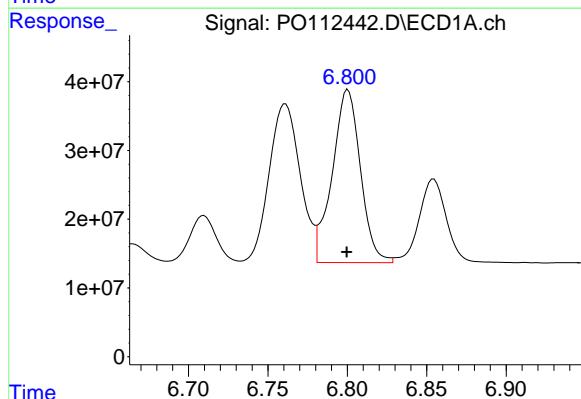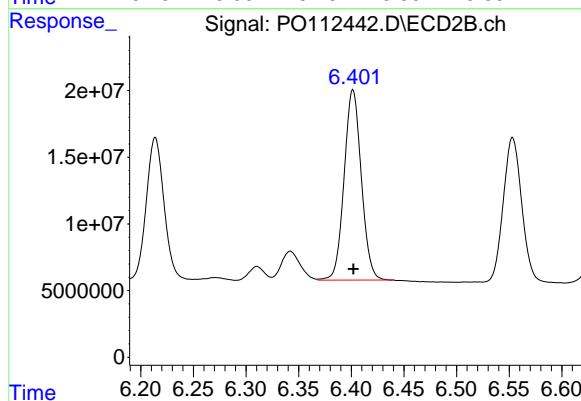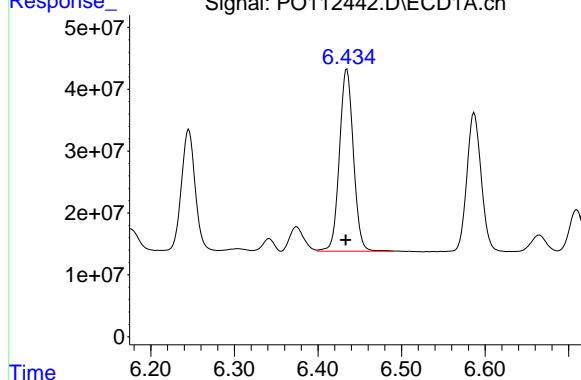

#32 AR-1260-2


R.T.: 6.402 min
 Delta R.T.: 0.000 min
 Response: 162434681
 Conc: 492.98 ng/ml

#33 AR-1260-3

R.T.: 6.800 min
 Delta R.T.: 0.000 min
 Response: 311057482
 Conc: 528.99 ng/ml

#33 AR-1260-3

R.T.: 6.553 min
 Delta R.T.: 0.000 min
 Response: 132981251
 Conc: 517.60 ng/ml

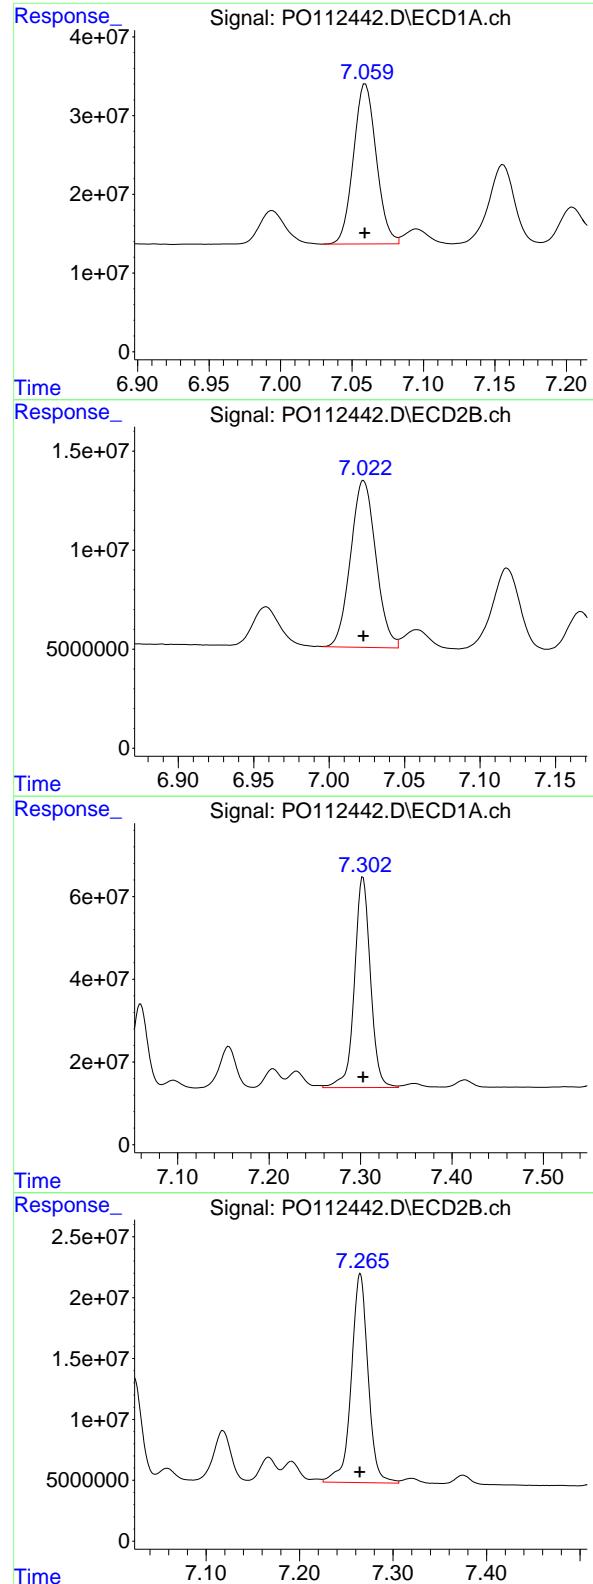

#34 AR-1260-4

R.T.: 7.059 min
 Delta R.T.: 0.000 min
 Response: 226325062
 Conc: 501.82 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO072325

#34 AR-1260-4

R.T.: 7.023 min
 Delta R.T.: 0.000 min
 Response: 98281247
 Conc: 513.73 ng/ml

#35 AR-1260-5

R.T.: 7.303 min
 Delta R.T.: 0.000 min
 Response: 621432684
 Conc: 501.50 ng/ml

#35 AR-1260-5

R.T.: 7.265 min
 Delta R.T.: 0.000 min
 Response: 214550458
 Conc: 520.51 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 20:42
 Operator : YP/AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:04:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.663 | 460.7E6 | 275.9E6 | 56.651 | 55.526 |
| 2) SA Decachlor... | 8.694 | 8.640 | 401.5E6 | 93838611 | 54.911 | 53.103 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 16) L4 AR-1242-1 | 4.756 | 4.738 | 129.0E6 | 80174107 | 521.171 | 506.169 |
| 17) L4 AR-1242-2 | 4.776 | 4.756 | 194.8E6 | 118.6E6 | 526.705 | 507.457 |
| 18) L4 AR-1242-3 | 4.832 | 4.931 | 123.7E6 | 62408526 | 522.828 | 514.968 |
| 19) L4 AR-1242-4 | 4.952 | 5.015 | 99083869 | 61266680 | 510.009 | 499.161 |
| 20) L4 AR-1242-5 | 5.603 | 5.535 | 107.3E6 | 81609556 | 501.589 | 506.982 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 20:42
 Operator : YP/AJ
 Sample : AR12421ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:04:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

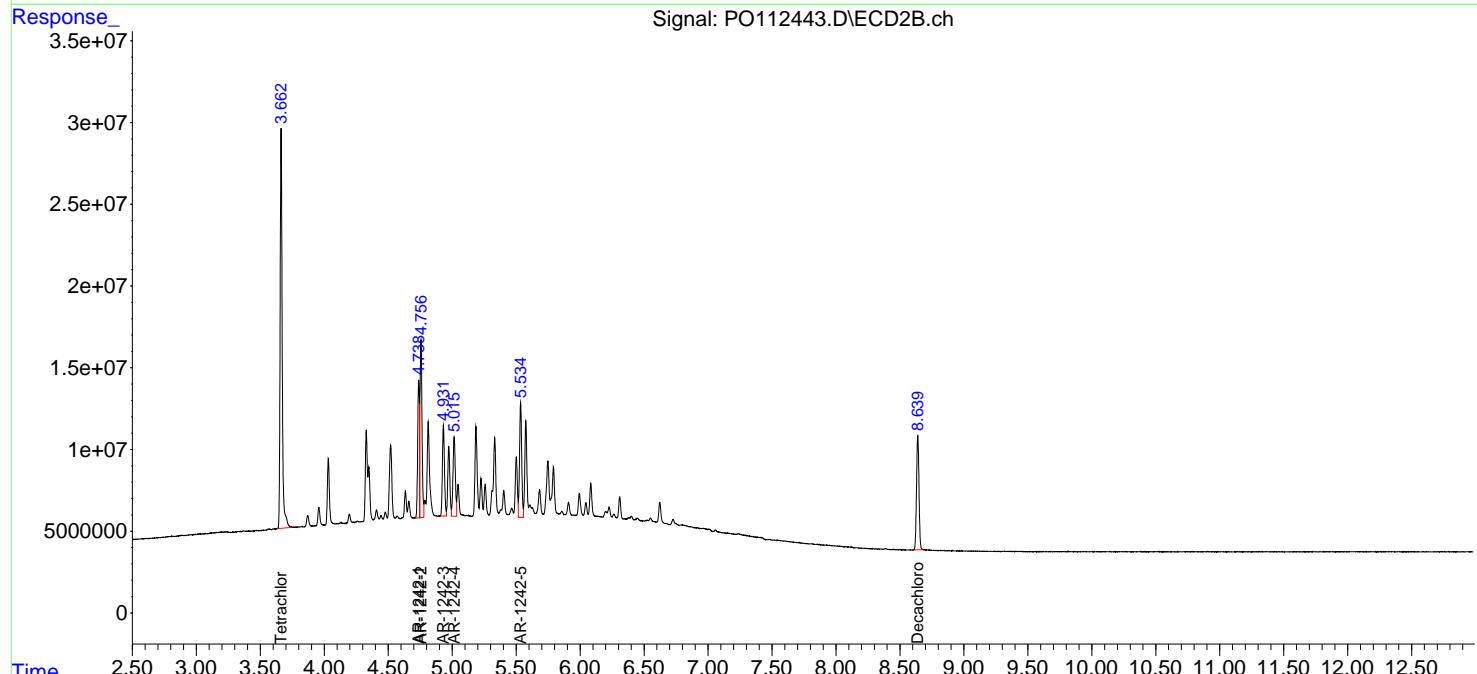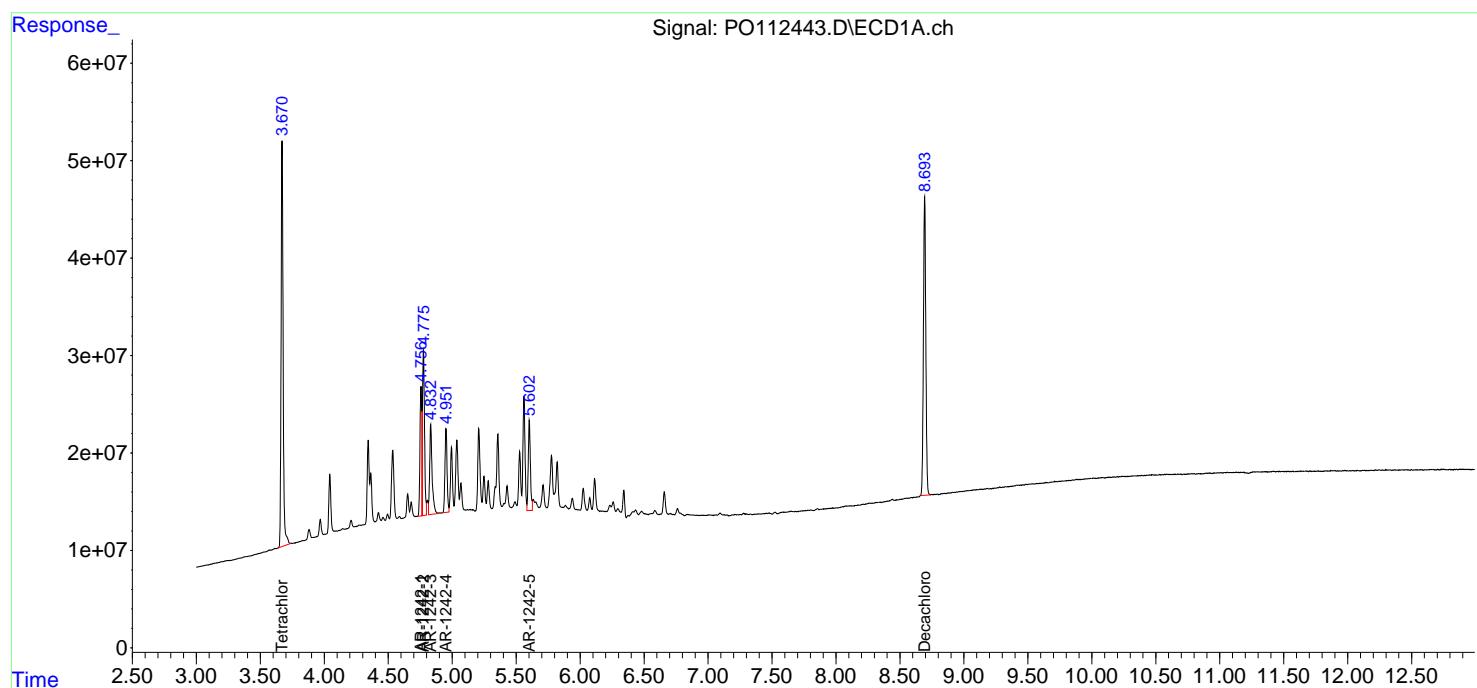

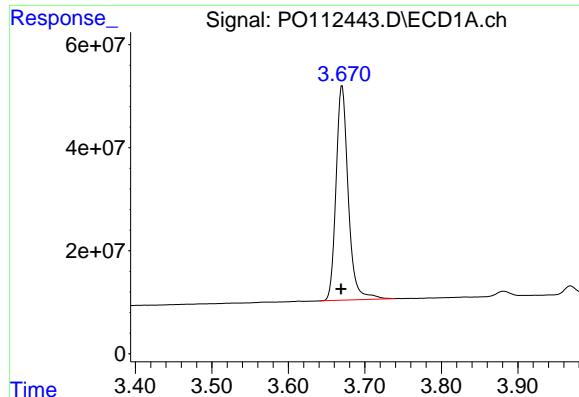


#1 Tetrachloro-m-xylene

R.T.: 3.670 min

Delta R.T.: 0.001 min

Response: 460660306

Conc: 56.65 ng/ml

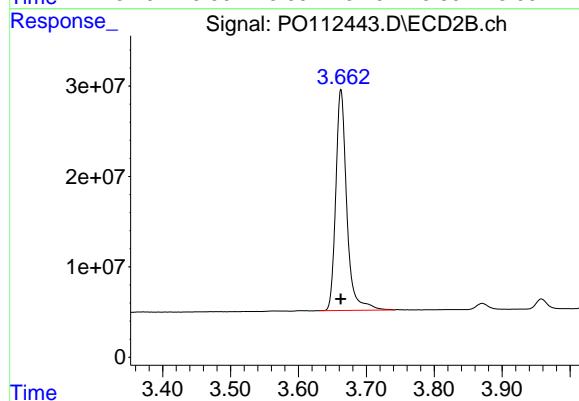Instrument:
ECD_O
ClientSampleId :
ICVPO072325AR1242


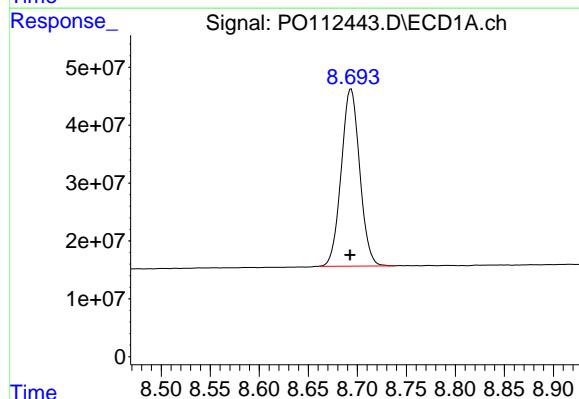
#1 Tetrachloro-m-xylene

R.T.: 3.663 min

Delta R.T.: 0.000 min

Response: 275918957

Conc: 55.53 ng/ml




#2 Decachlorobiphenyl

R.T.: 8.694 min

Delta R.T.: 0.000 min

Response: 401498785

Conc: 54.91 ng/ml

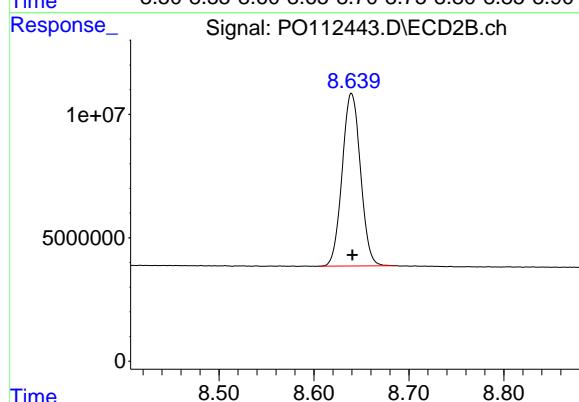





#2 Decachlorobiphenyl

R.T.: 8.640 min

Delta R.T.: 0.000 min

Response: 93838611

Conc: 53.10 ng/ml

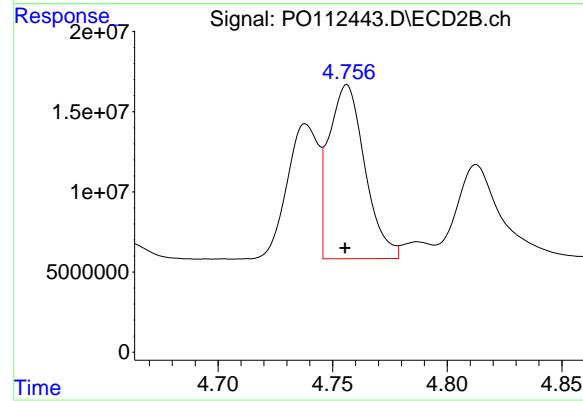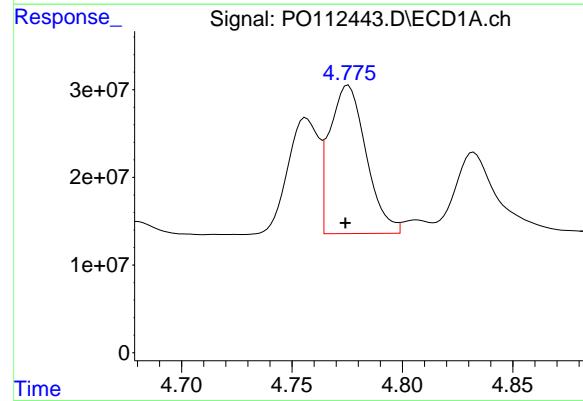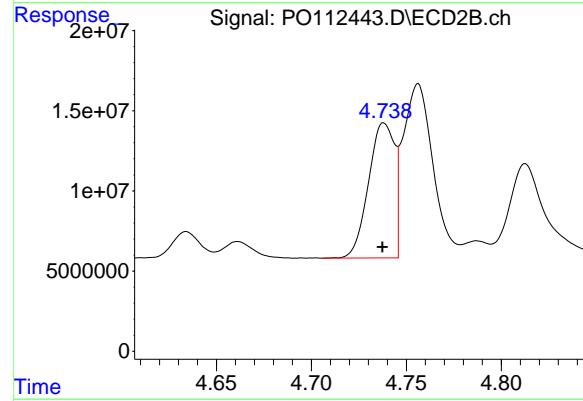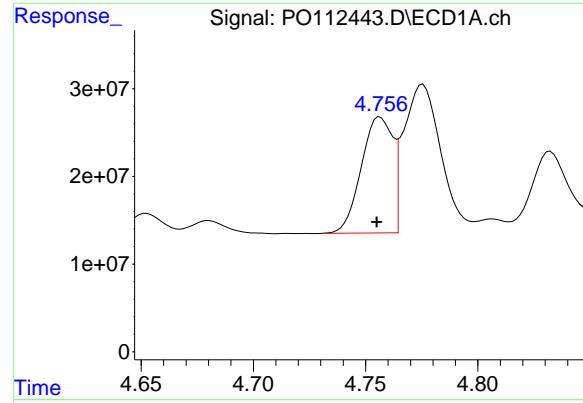

#16 AR-1242-1

R.T.: 4.756 min
 Delta R.T.: 0.001 min
 Response: 129037672
 Conc: 521.17 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1242

#16 AR-1242-1

R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 80174107
 Conc: 506.17 ng/ml

#17 AR-1242-2

R.T.: 4.776 min
 Delta R.T.: 0.001 min
 Response: 194771971
 Conc: 526.70 ng/ml


#17 AR-1242-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 118575765
 Conc: 507.46 ng/ml

#18 AR-1242-3


R.T.: 4.832 min
 Delta R.T.: 0.002 min
 Response: 123731413
 Conc: 522.83 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1242

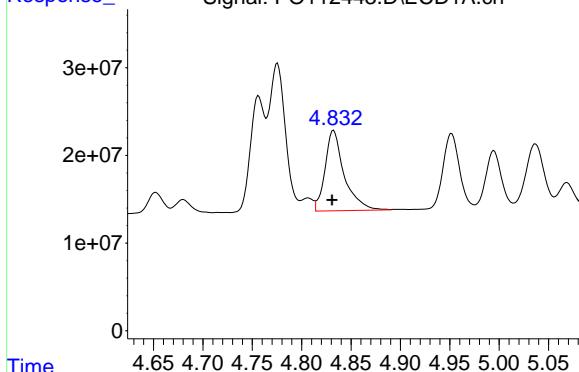


#18 AR-1242-3

R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 62408526
 Conc: 514.97 ng/ml

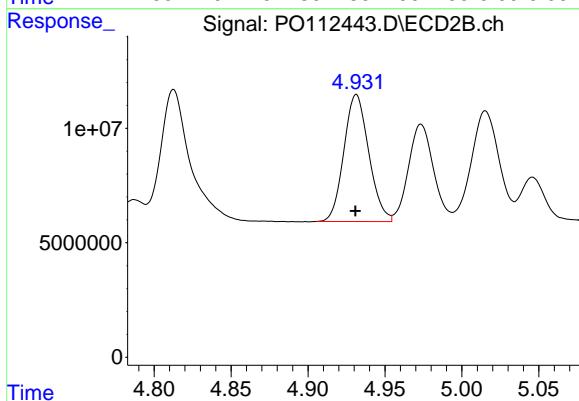


#19 AR-1242-4


R.T.: 4.952 min
 Delta R.T.: 0.001 min
 Response: 99083869
 Conc: 510.01 ng/ml

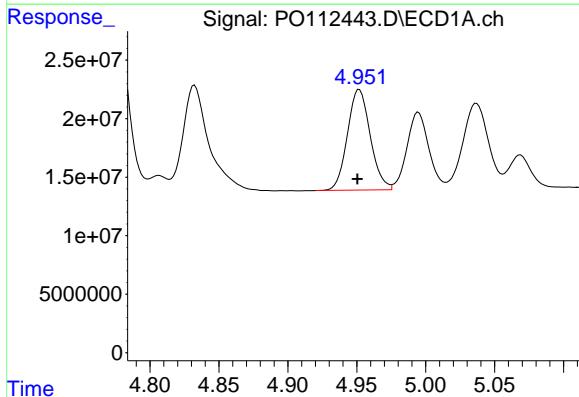

#19 AR-1242-4

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 61266680
 Conc: 499.16 ng/ml

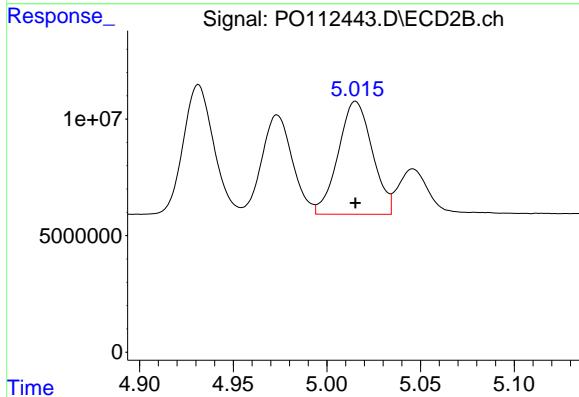

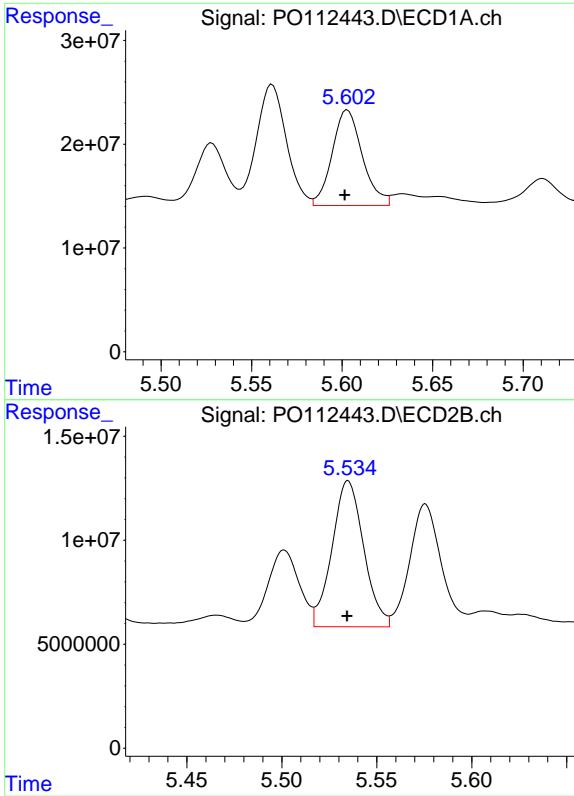

#20 AR-1242-5

R.T.: 5.603 min
Delta R.T.: 0.001 min
Response: 107297707
Conc: 501.59 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1242

#20 AR-1242-5

R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 81609556
Conc: 506.98 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 21:18
 Operator : YP/AJ
 Sample : AR1248ICV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:04:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 452.2E6 | 269.7E6 | 55.615 | 54.268 |
| 2) SA Decachlor... | 8.694 | 8.641 | 403.2E6 | 94089624 | 55.141 | 53.245 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 21) L5 AR-1248-1 | 4.755 | 4.737 | 96403586 | 60735474 | 514.952 | 499.842 |
| 22) L5 AR-1248-2 | 4.994 | 4.973 | 132.8E6 | 84845389 | 520.457 | 501.214 |
| 23) L5 AR-1248-3 | 5.207 | 5.015 | 170.0E6 | 89430727 | 494.627 | 503.418 |
| 24) L5 AR-1248-4 | 5.560 | 5.185 | 261.6E6 | 105.8E6 | 514.800 | 507.962 |
| 25) L5 AR-1248-5 | 5.602 | 5.576 | 177.0E6 | 109.0E6 | 506.243 | 507.656 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112444.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 21:18
 Operator : YP/AJ
 Sample : AR12481CV500
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1248

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:04:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

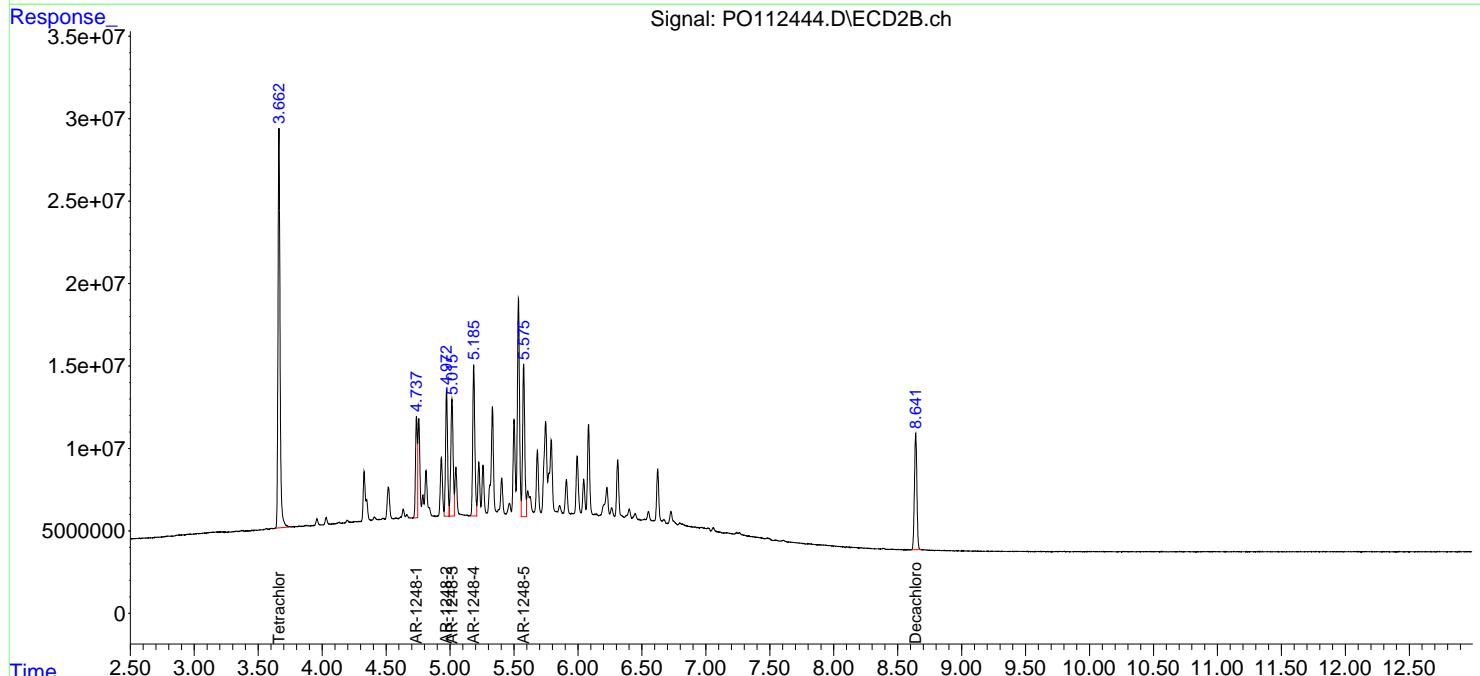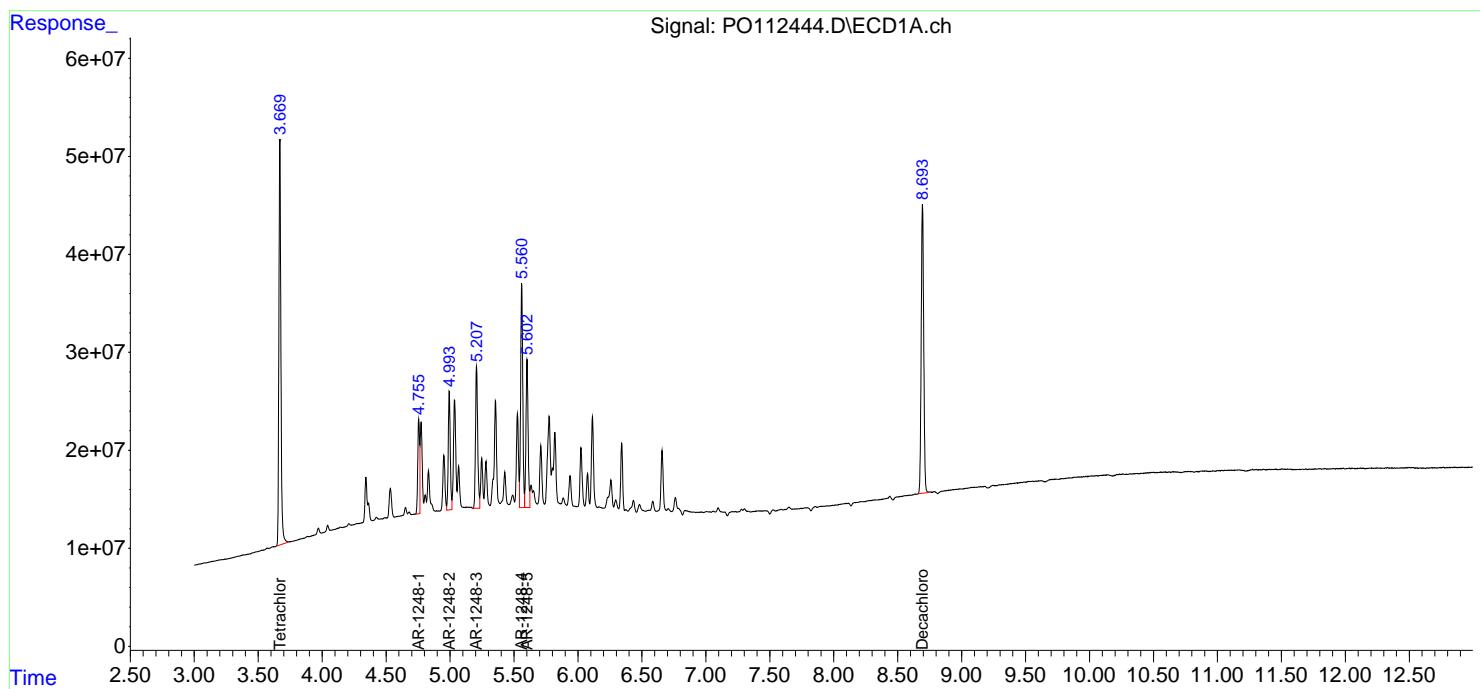


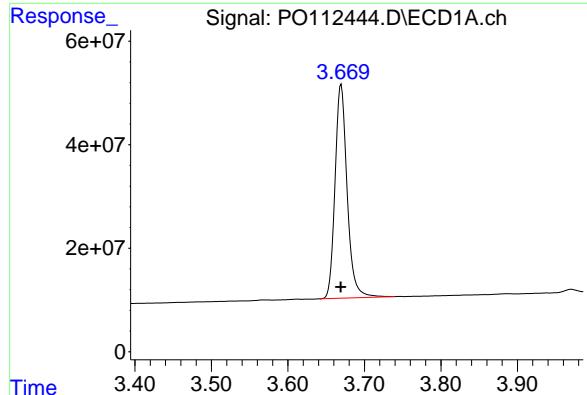

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 452237643
Conc: 55.62 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1248

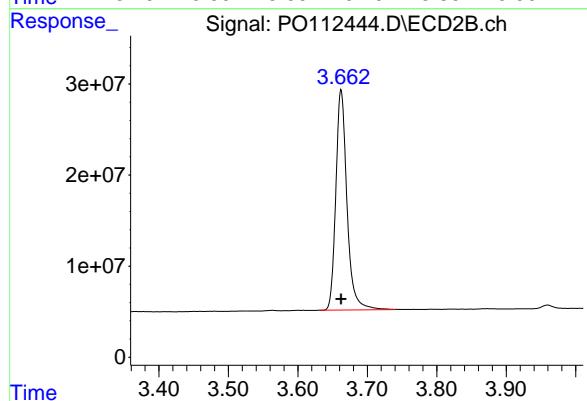


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 269667822
Conc: 54.27 ng/ml

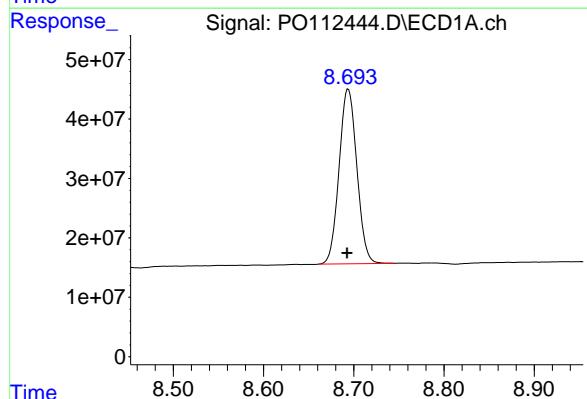





#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.001 min
Response: 403182686
Conc: 55.14 ng/ml

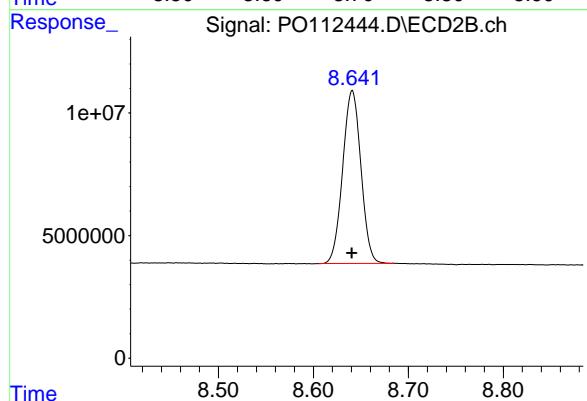

#2 Decachlorobiphenyl

R.T.: 8.641 min
Delta R.T.: 0.000 min
Response: 94089624
Conc: 53.24 ng/ml

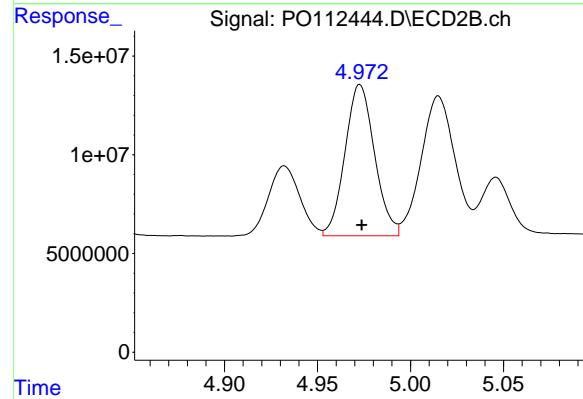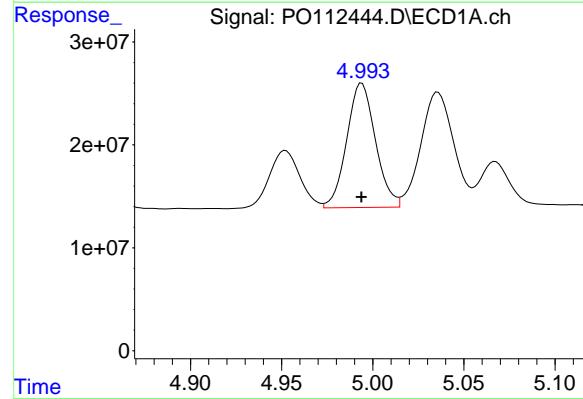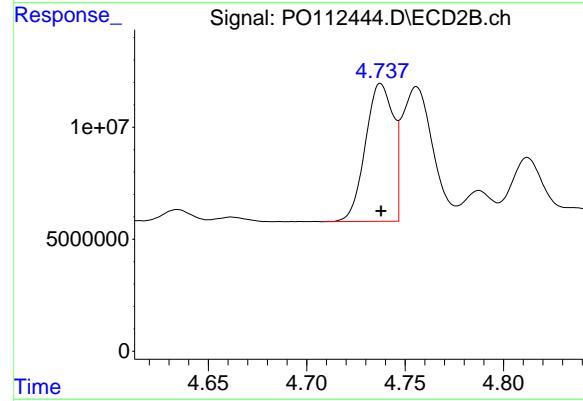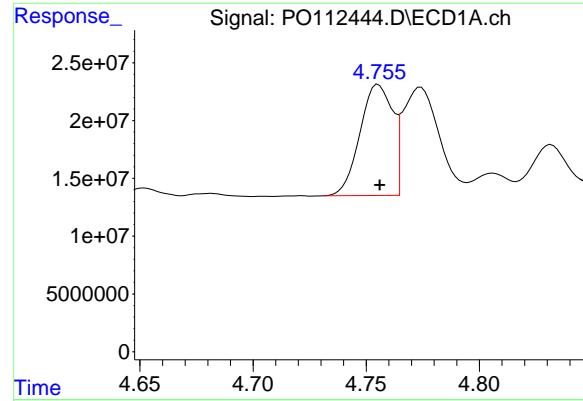

#21 AR-1248-1

R.T.: 4.755 min
 Delta R.T.: 0.000 min
 Response: 96403586
 Conc: 514.95 ng/ml

Instrument: ECD_O
 ClientSampleId: ICVPO072325AR1248

#21 AR-1248-1


R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 60735474
 Conc: 499.84 ng/ml

#22 AR-1248-2

R.T.: 4.994 min
 Delta R.T.: 0.000 min
 Response: 132775009
 Conc: 520.46 ng/ml

#22 AR-1248-2

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 84845389
 Conc: 501.21 ng/ml

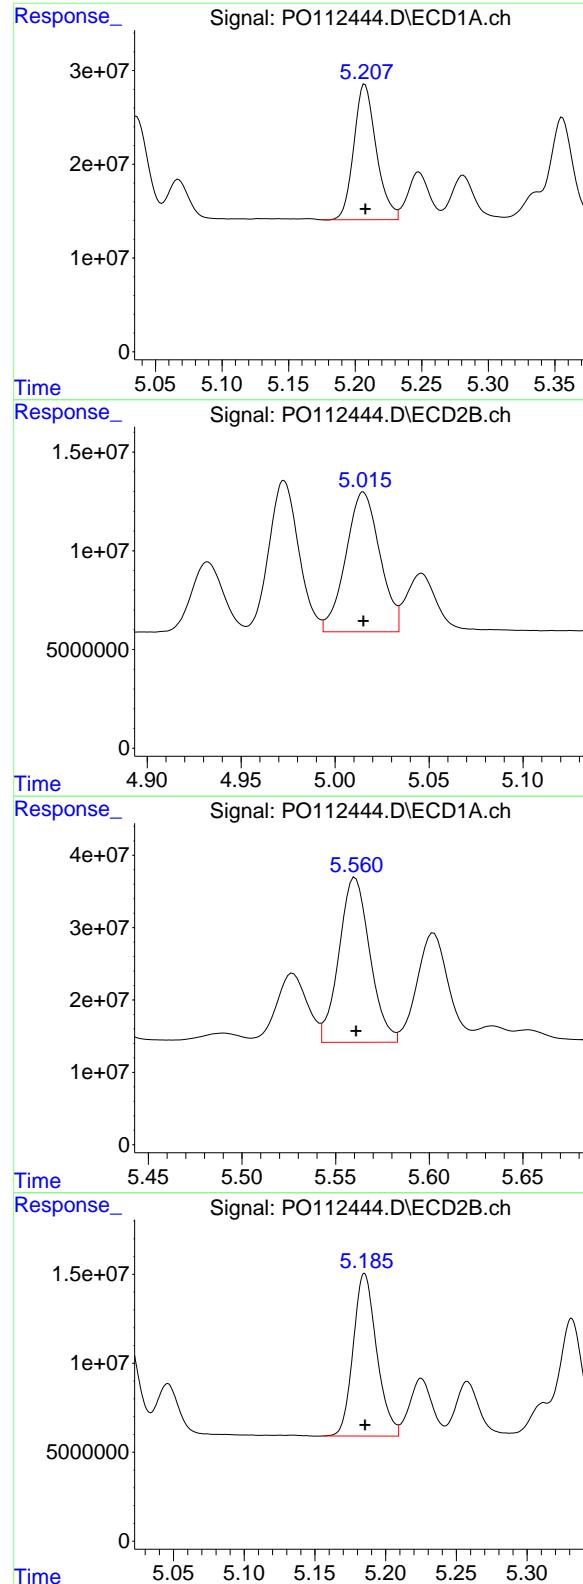

#23 AR-1248-3

R.T.: 5.207 min
 Delta R.T.: 0.000 min
 Response: 170003864
 Conc: 494.63 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1248

#23 AR-1248-3

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 89430727
 Conc: 503.42 ng/ml

#24 AR-1248-4

R.T.: 5.560 min
 Delta R.T.: 0.000 min
 Response: 261558200
 Conc: 514.80 ng/ml



#24 AR-1248-4

R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 105836252
 Conc: 507.96 ng/ml

#25 AR-1248-5

R.T.: 5.602 min
Delta R.T.: 0.000 min
Response: 176978025
Conc: 506.24 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1248

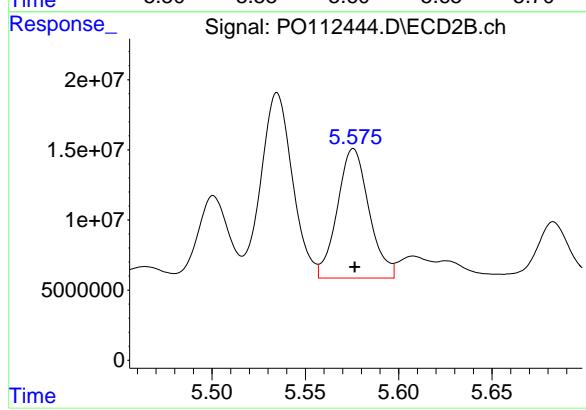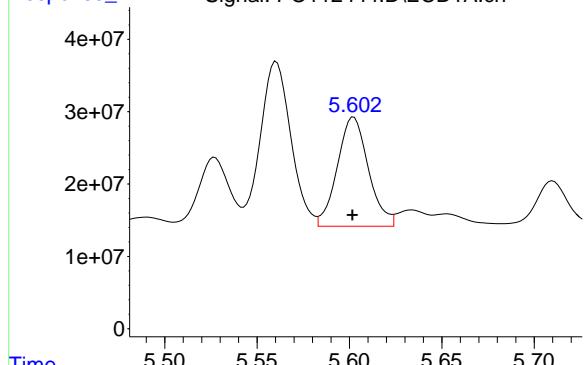

#25 AR-1248-5

R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 109026784
Conc: 507.66 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 21:54
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:05:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 445.4E6 | 266.6E6 | 54.778 | 53.658 |
| 2) SA Decachlor... | 8.693 | 8.639 | 391.6E6 | 91844886 | 53.551 | 51.975 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|---------|---------|---------|
| 26) L6 AR-1254-1 | 5.561 | 5.534 | 276.3E6 | 163.9E6 | 503.299 | 498.849 |
| 27) L6 AR-1254-2 | 5.711 | 5.683 | 249.7E6 | 144.3E6 | 513.931 | 498.389 |
| 28) L6 AR-1254-3 | 6.114 | 6.083 | 379.5E6 | 213.7E6 | 509.918 | 499.814 |
| 29) L6 AR-1254-4 | 6.342 | 6.310 | 247.0E6 | 123.1E6 | 449.340 | 450.950 |
| 30) L6 AR-1254-5 | 6.761 | 6.726 | 356.3E6 | 167.5E6 | 503.357 | 501.388 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112445.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 21:54
 Operator : YP/AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:05:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

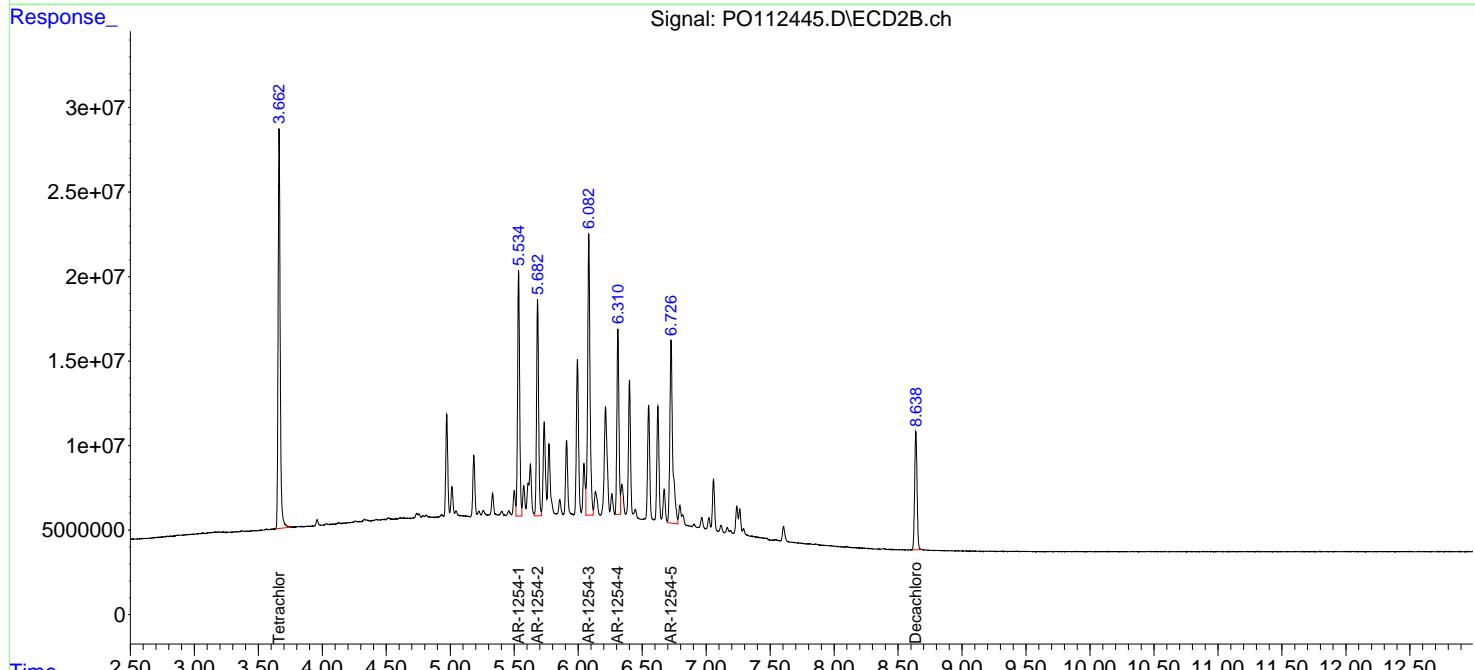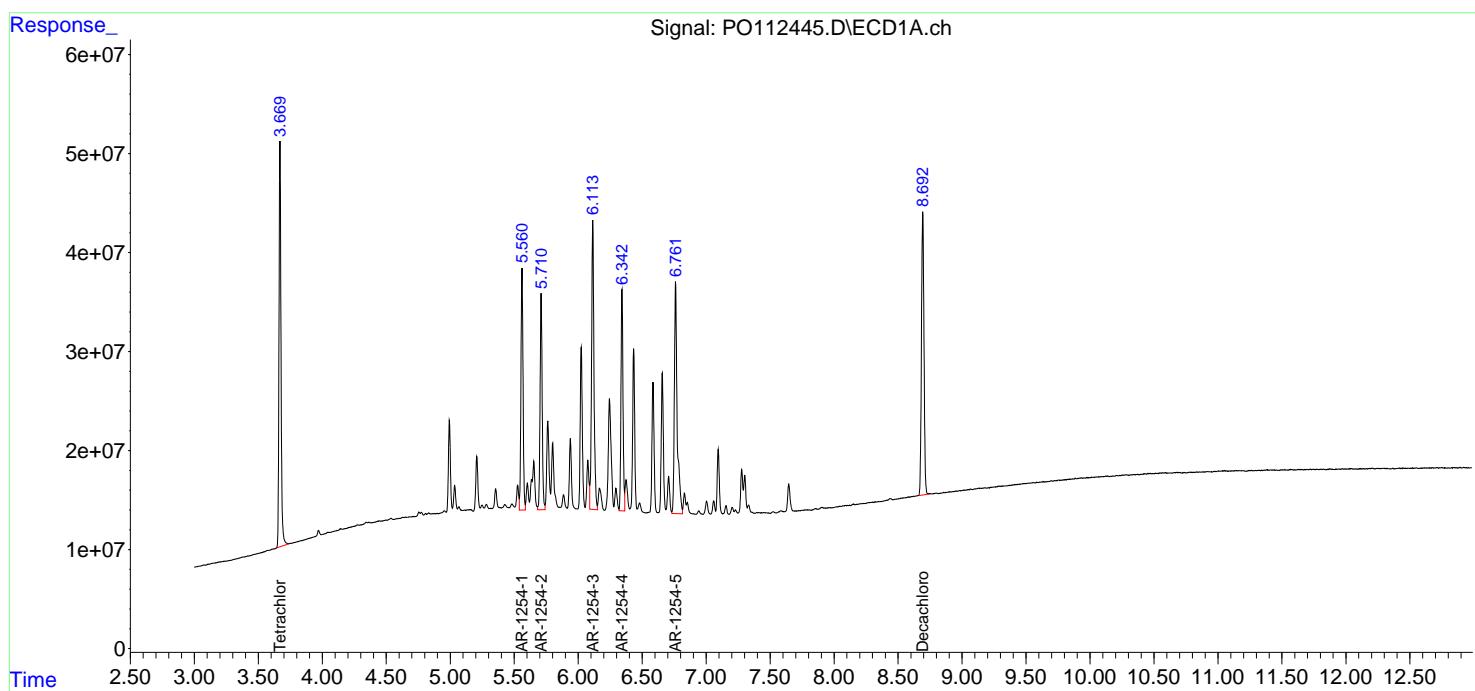


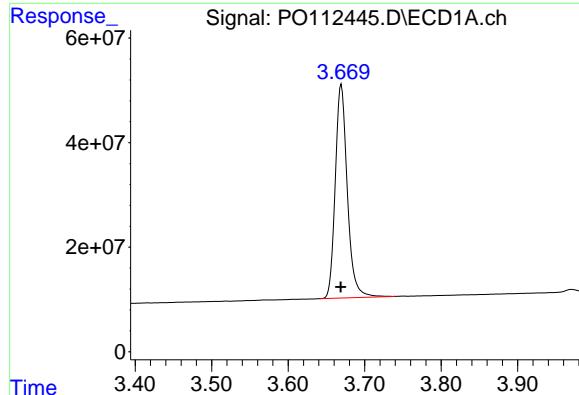

#1 Tetrachloro-m-xylene


R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 445431862
Conc: 54.78 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1254

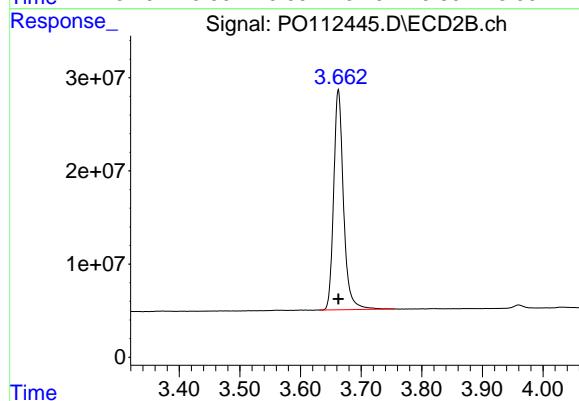


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 266634238
Conc: 53.66 ng/ml

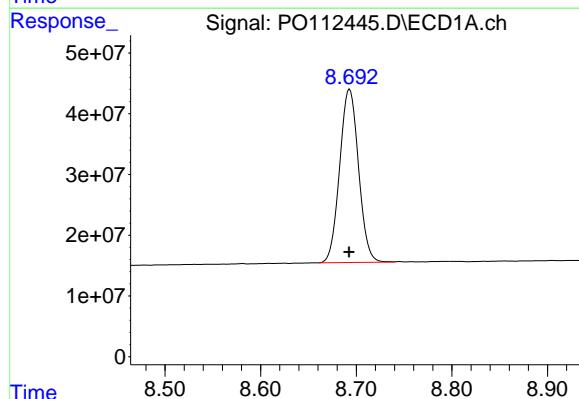

#2 Decachlorobiphenyl

R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 391557477
Conc: 53.55 ng/ml

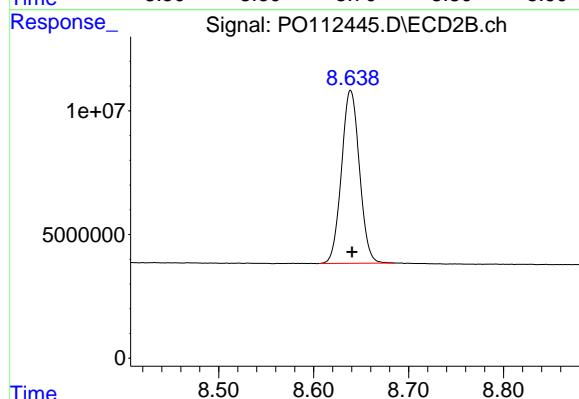


#2 Decachlorobiphenyl

R.T.: 8.639 min
Delta R.T.: -0.002 min
Response: 91844886
Conc: 51.97 ng/ml

#26 AR-1254-1


R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 276290556
 Conc: 503.30 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1254

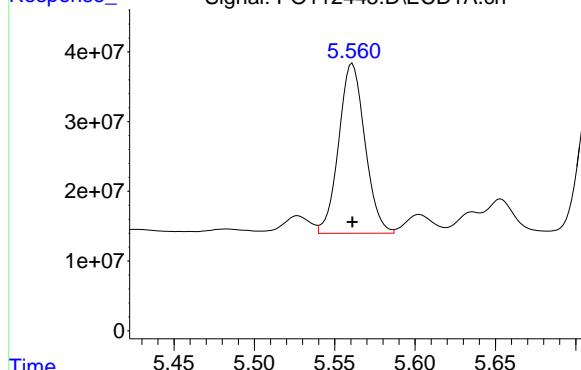


#26 AR-1254-1

R.T.: 5.534 min
 Delta R.T.: 0.000 min
 Response: 163932118
 Conc: 498.85 ng/ml

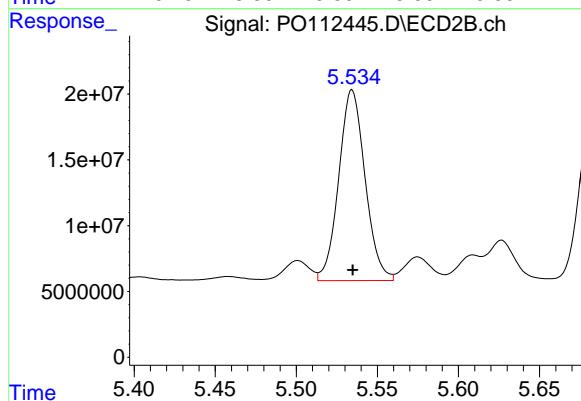


#27 AR-1254-2

R.T.: 5.711 min
 Delta R.T.: 0.000 min
 Response: 249728799
 Conc: 513.93 ng/ml

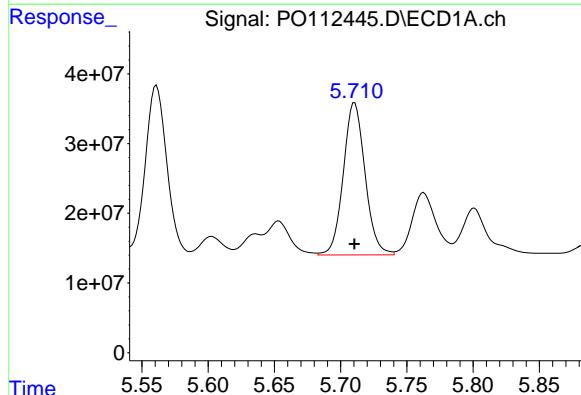

#27 AR-1254-2


R.T.: 5.683 min
 Delta R.T.: 0.000 min
 Response: 144278870
 Conc: 498.39 ng/ml

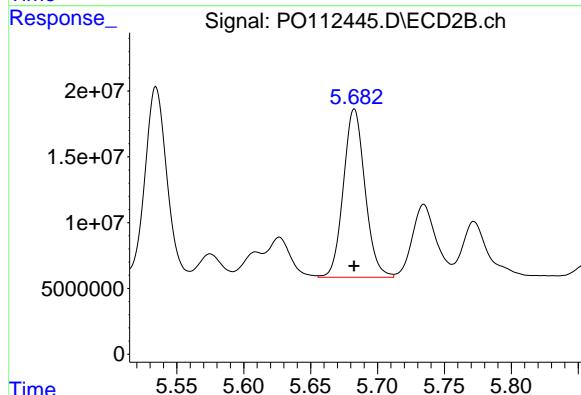

#28 AR-1254-3


R.T.: 6.114 min
 Delta R.T.: 0.000 min
 Response: 379525107
 Conc: 509.92 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1254

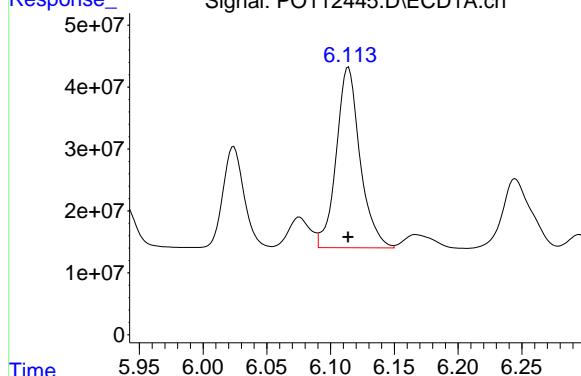


#28 AR-1254-3

R.T.: 6.083 min
 Delta R.T.: 0.000 min
 Response: 213651018
 Conc: 499.81 ng/ml

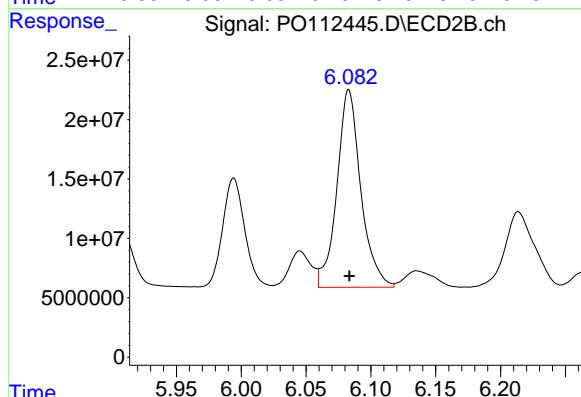


#29 AR-1254-4

R.T.: 6.342 min
 Delta R.T.: 0.000 min
 Response: 247003787
 Conc: 449.34 ng/ml

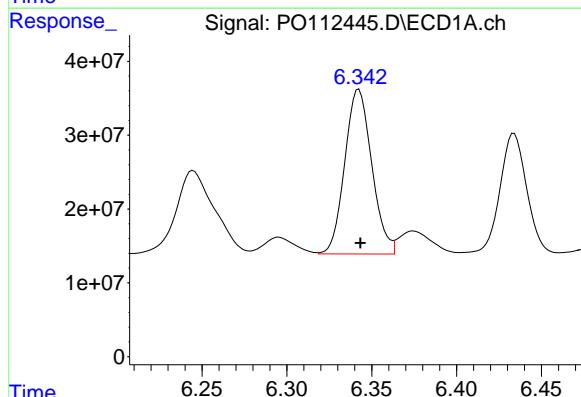

#29 AR-1254-4



R.T.: 6.310 min
 Delta R.T.: 0.000 min
 Response: 123092792
 Conc: 450.95 ng/ml

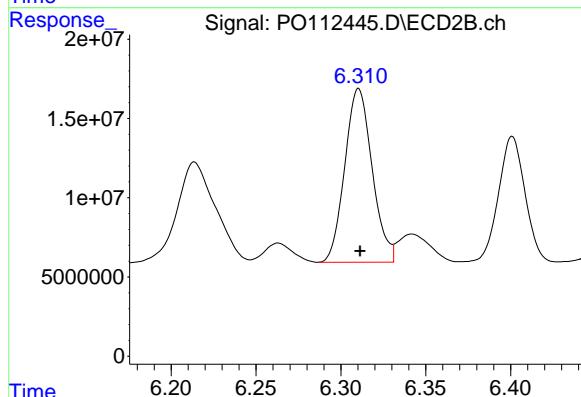

#30 AR-1254-5

R.T.: 6.761 min
Delta R.T.: 0.000 min
Response: 356288489
Conc: 503.36 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1254

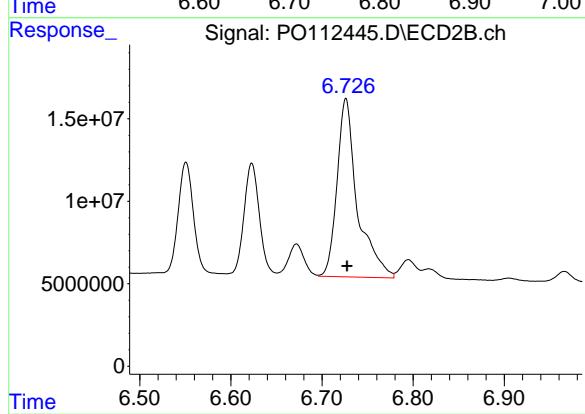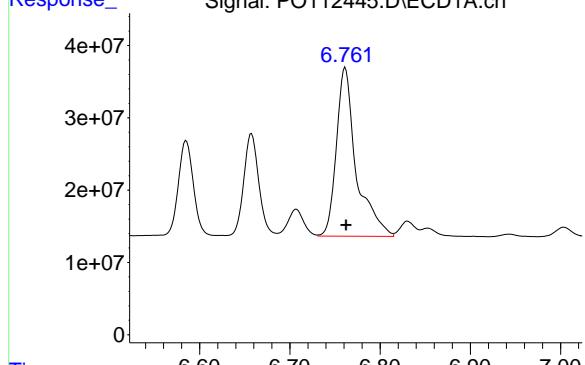

#30 AR-1254-5

R.T.: 6.726 min
Delta R.T.: -0.001 min
Response: 167473534
Conc: 501.39 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 22:31
 Operator : YP/AJ
 Sample : AR1268ICV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:54:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:52:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|---------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 460.9E6 | 275.4E6 | 53.238 | 52.473 |
| 2) SA Decachlor... | 8.694 | 8.640 | 731.3E6 | 166.7E6 | 52.412 | 51.834 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 41) L9 AR-1268-1 | 7.586 | 7.546 | 910.3E6 | 250.7E6 | 519.844 | 484.189 |
| 42) L9 AR-1268-2 | 7.651 | 7.611 | 767.0E6 | 207.2E6 | 520.717 | 487.400 |
| 43) L9 AR-1268-3 | 7.856 | 7.815 | 656.2E6 | 158.5E6 | 524.050 | 493.242 |
| 44) L9 AR-1268-4 | 8.146 | 8.102 | 253.2E6 | 55462942 | 525.396 | 498.339 |
| 45) L9 AR-1268-5 | 8.439 | 8.391 | 1754.5E6 | 373.2E6 | 522.622 | 509.970 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112446.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 22:31
 Operator : YP/AJ
 Sample : AR12681CV500
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
ICVPO072325AR1268

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 04:54:33 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:52:41 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

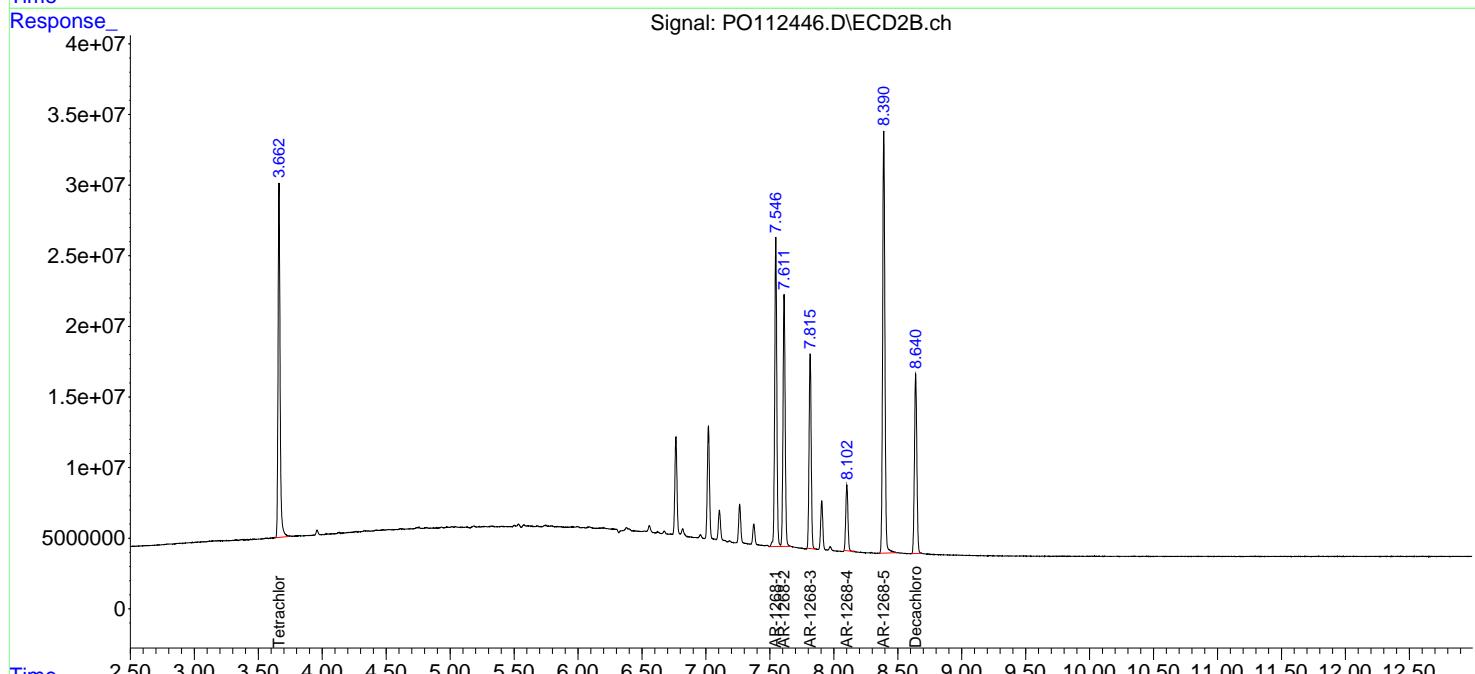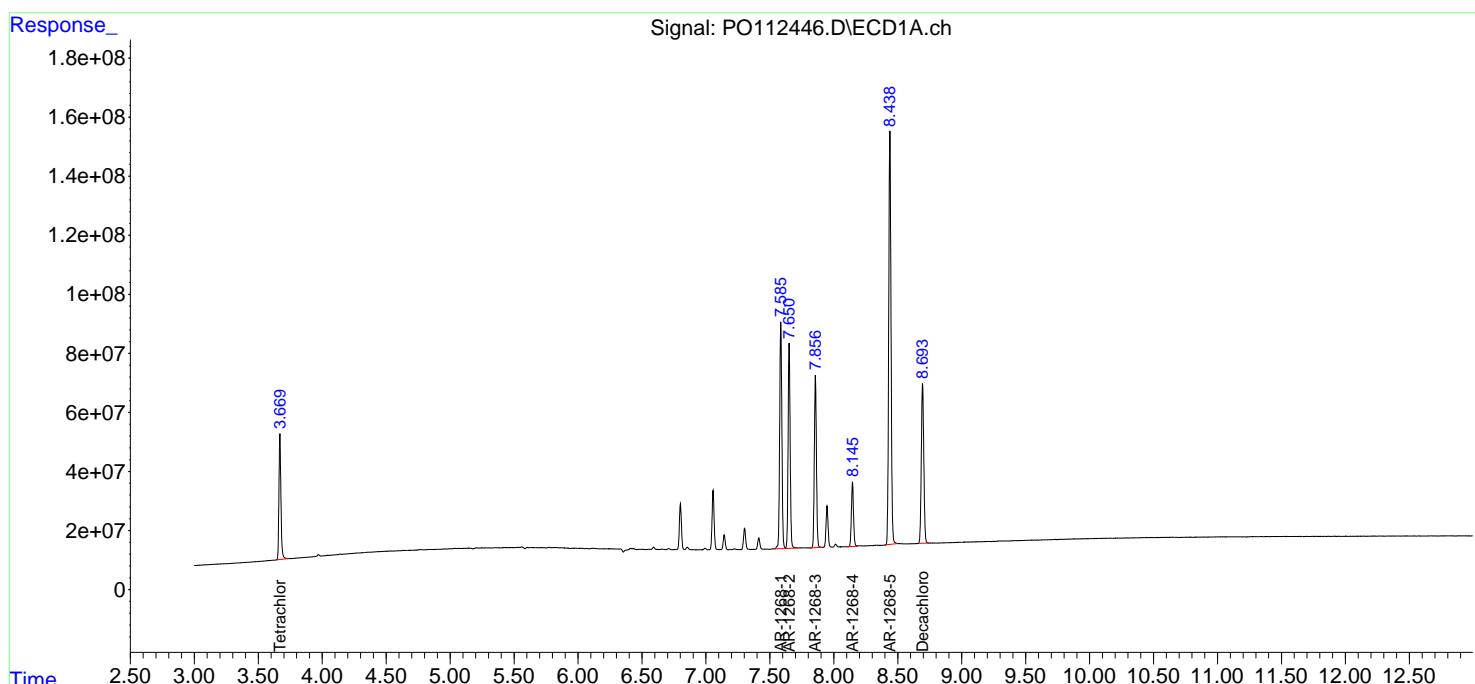

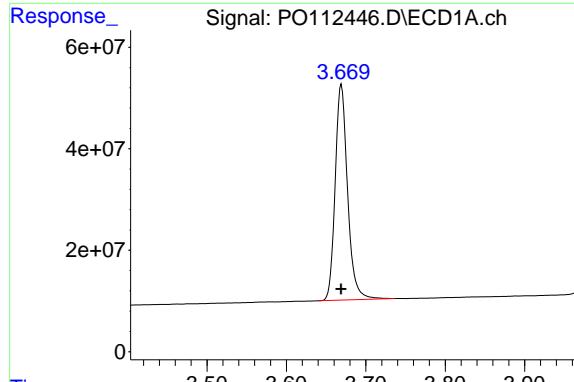

#1 Tetrachloro-m-xylene

R.T.: 3.669 min

Delta R.T.: 0.000 min

Response: 460923763


Conc: 53.24 ng/ml

Instrument:

ECD_O

ClientSampleId :

ICVPO072325AR1268

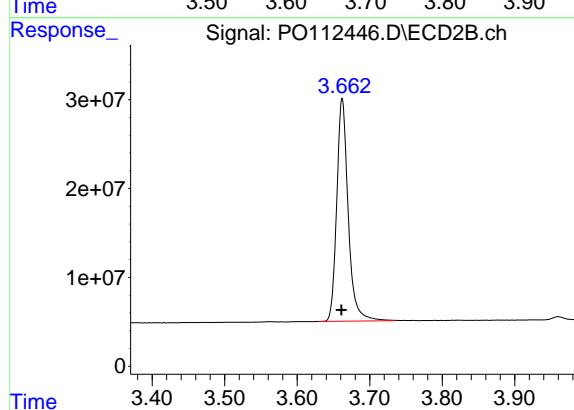


#1 Tetrachloro-m-xylene

R.T.: 3.662 min

Delta R.T.: 0.000 min

Response: 275414210

Conc: 52.47 ng/ml

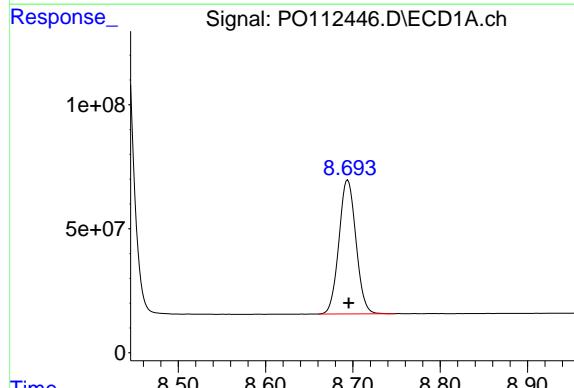


#2 Decachlorobiphenyl

R.T.: 8.694 min

Delta R.T.: -0.001 min

Response: 731296278

Conc: 52.41 ng/ml

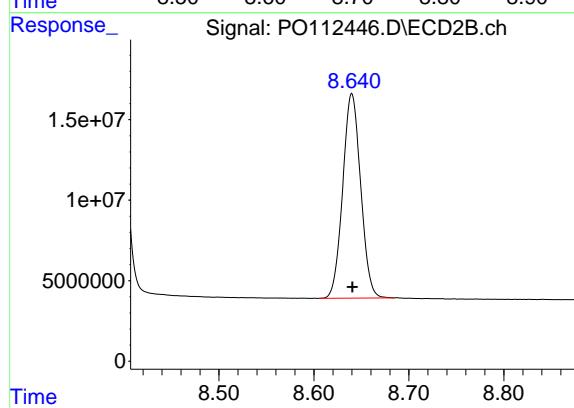


#2 Decachlorobiphenyl

R.T.: 8.640 min

Delta R.T.: 0.000 min

Response: 166747338

Conc: 51.83 ng/ml

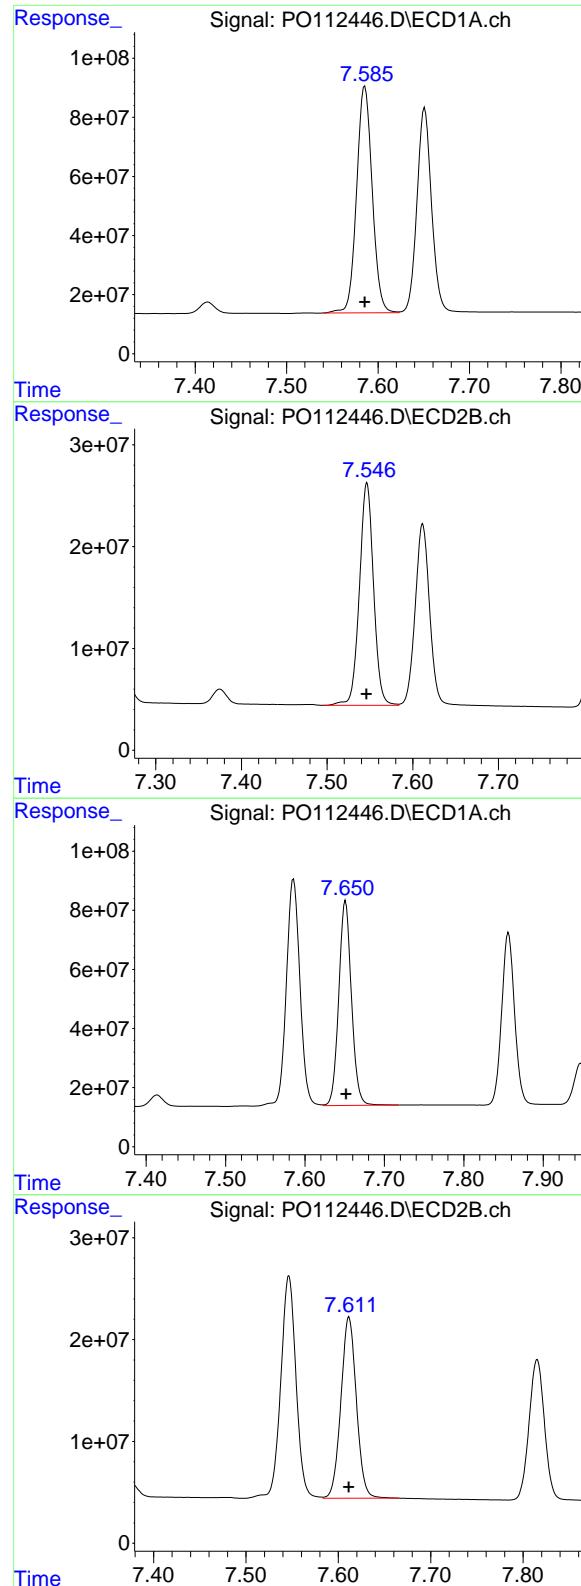

#41 AR-1268-1

R.T.: 7.586 min
Delta R.T.: 0.000 min
Response: 910320699
Conc: 519.84 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1268

#41 AR-1268-1

R.T.: 7.546 min
Delta R.T.: 0.000 min
Response: 250743260
Conc: 484.19 ng/ml

#42 AR-1268-2

R.T.: 7.651 min
Delta R.T.: 0.000 min
Response: 767028892
Conc: 520.72 ng/ml





#42 AR-1268-2

R.T.: 7.611 min
Delta R.T.: 0.000 min
Response: 207176092
Conc: 487.40 ng/ml

#43 AR-1268-3

R.T.: 7.856 min
 Delta R.T.: 0.000 min
 Response: 656231584
 Conc: 524.05 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1268

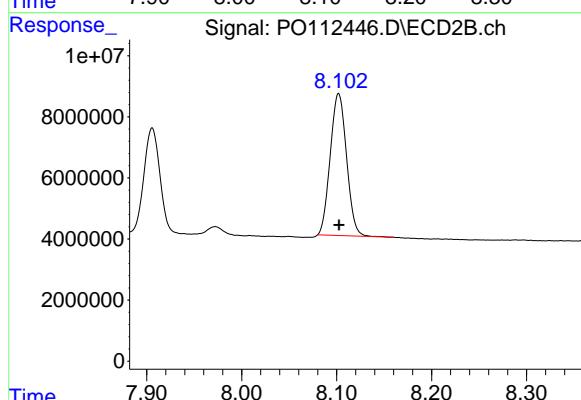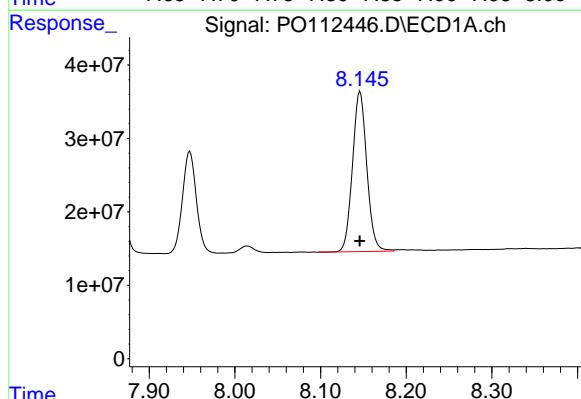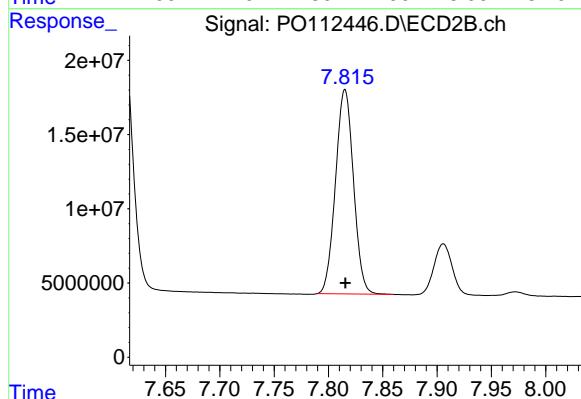

#43 AR-1268-3

R.T.: 7.815 min
 Delta R.T.: 0.000 min
 Response: 158462268
 Conc: 493.24 ng/ml

#44 AR-1268-4

R.T.: 8.146 min
 Delta R.T.: 0.000 min
 Response: 253169344
 Conc: 525.40 ng/ml



#44 AR-1268-4

R.T.: 8.102 min
 Delta R.T.: 0.000 min
 Response: 55462942
 Conc: 498.34 ng/ml

#45 AR-1268-5

R.T.: 8.439 min
Delta R.T.: 0.000 min
Response: 1754531841
Conc: 522.62 ng/ml

Instrument: ECD_O
ClientSampleId: ICVPO072325AR1268

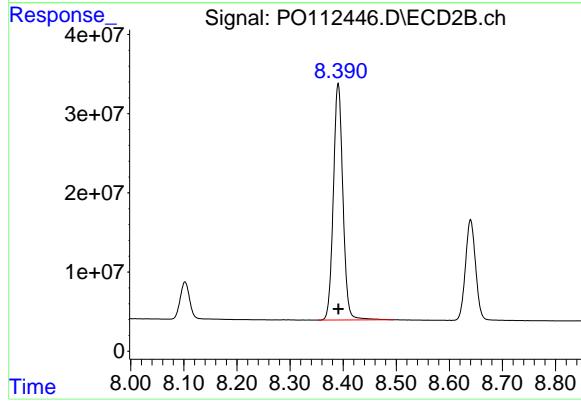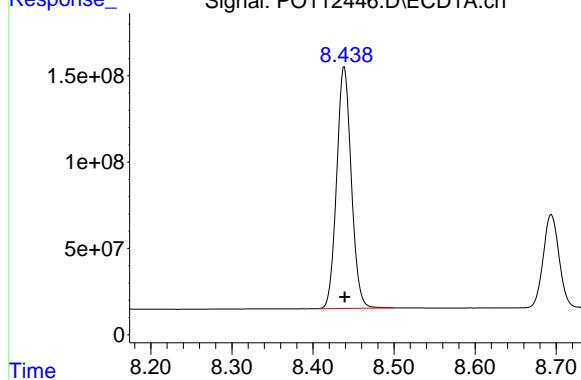

#45 AR-1268-5

R.T.: 8.391 min
Delta R.T.: 0.000 min
Response: 373164428
Conc: 509.97 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

| | | | |
|-----------------------|-----------------|-----------------------------|-------------------------------------|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| Instrument ID: | <u>ECD_P</u> | Calibration Date(s): | <u>08/01/2025</u> <u>08/01/2025</u> |
| | | Calibration Times: | <u>12:05</u> <u>20:28</u> |

GC Column: ZB-MR1 ID: 0.32 (mm)

| | | |
|---------------------|-----------------------------|----------------------------|
| LAB FILE ID: | RT 1000 = <u>PP074168.D</u> | RT 750 = <u>PP074169.D</u> |
| | RT 500 = <u>PP074170.D</u> | RT 250 = <u>PP074171.D</u> |
| | | RT 050 = <u>PP074172.D</u> |

| COMPOUND | RT 1000 | RT 750 | RT 500 | RT 250 | RT 050 | MEAN RT | RT WINDOW FROM | TO |
|----------------------|---------|--------|--------|--------|--------|---------|----------------|-------|
| Aroclor-1016-1 (1) | 5.81 | 5.81 | 5.81 | 5.81 | 5.81 | 5.81 | 5.71 | 5.91 |
| Aroclor-1016-2 (2) | 5.83 | 5.84 | 5.83 | 5.83 | 5.84 | 5.83 | 5.73 | 5.93 |
| Aroclor-1016-3 (3) | 5.90 | 5.90 | 5.90 | 5.90 | 5.90 | 5.90 | 5.80 | 6.00 |
| Aroclor-1016-4 (4) | 5.99 | 6.00 | 5.99 | 5.99 | 5.99 | 5.99 | 5.89 | 6.09 |
| Aroclor-1016-5 (5) | 6.29 | 6.29 | 6.29 | 6.28 | 6.29 | 6.29 | 6.19 | 6.39 |
| Aroclor-1260-1 (1) | 7.40 | 7.41 | 7.40 | 7.40 | 7.40 | 7.40 | 7.30 | 7.50 |
| Aroclor-1260-2 (2) | 7.66 | 7.66 | 7.66 | 7.65 | 7.66 | 7.66 | 7.56 | 7.76 |
| Aroclor-1260-3 (3) | 8.01 | 8.02 | 8.01 | 8.01 | 8.02 | 8.01 | 7.91 | 8.11 |
| Aroclor-1260-4 (4) | 8.24 | 8.24 | 8.24 | 8.24 | 8.24 | 8.24 | 8.14 | 8.34 |
| Aroclor-1260-5 (5) | 8.57 | 8.57 | 8.57 | 8.57 | 8.57 | 8.57 | 8.47 | 8.67 |
| Decachlorobiphenyl | 10.44 | 10.44 | 10.44 | 10.44 | 10.44 | 10.44 | 10.34 | 10.54 |
| Tetrachloro-m-xylene | 4.66 | 4.66 | 4.66 | 4.66 | 4.66 | 4.66 | 4.56 | 4.76 |
| Aroclor-1242-1 (1) | 5.81 | 5.81 | 5.81 | 5.81 | 5.81 | 5.81 | 5.71 | 5.91 |
| Aroclor-1242-2 (2) | 5.83 | 5.84 | 5.83 | 5.83 | 5.83 | 5.83 | 5.73 | 5.93 |
| Aroclor-1242-3 (3) | 5.90 | 5.90 | 5.89 | 5.90 | 5.90 | 5.90 | 5.80 | 6.00 |
| Aroclor-1242-4 (4) | 5.99 | 6.00 | 5.99 | 5.99 | 5.99 | 5.99 | 5.89 | 6.09 |
| Aroclor-1242-5 (5) | 6.72 | 6.72 | 6.72 | 6.72 | 6.72 | 6.72 | 6.62 | 6.82 |
| Decachlorobiphenyl | 10.44 | 10.44 | 10.43 | 10.44 | 10.43 | 10.44 | 10.34 | 10.54 |
| Tetrachloro-m-xylene | 4.66 | 4.66 | 4.66 | 4.66 | 4.66 | 4.66 | 4.56 | 4.76 |
| Aroclor-1254-1 (1) | 6.66 | 6.66 | 6.66 | 6.66 | 6.66 | 6.66 | 6.56 | 6.76 |
| Aroclor-1254-2 (2) | 6.88 | 6.87 | 6.87 | 6.87 | 6.87 | 6.87 | 6.77 | 6.97 |
| Aroclor-1254-3 (3) | 7.24 | 7.24 | 7.24 | 7.24 | 7.23 | 7.24 | 7.14 | 7.34 |
| Aroclor-1254-4 (4) | 7.52 | 7.52 | 7.52 | 7.52 | 7.52 | 7.52 | 7.42 | 7.62 |
| Aroclor-1254-5 (5) | 7.93 | 7.93 | 7.93 | 7.93 | 7.93 | 7.93 | 7.83 | 8.03 |
| Decachlorobiphenyl | 10.43 | 10.43 | 10.43 | 10.43 | 10.43 | 10.43 | 10.33 | 10.53 |
| Tetrachloro-m-xylene | 4.66 | 4.66 | 4.66 | 4.66 | 4.66 | 4.66 | 4.56 | 4.76 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

RETENTION TIMES OF INITIAL CALIBRATION

| | | | |
|----------------|-----------------|----------------------|-------------------|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| Instrument ID: | <u>ECD_P</u> | Calibration Date(s): | <u>08/01/2025</u> |
| | | Calibration Times: | <u>12:05</u> |

GC Column: ZB-MR2 ID: 0.32 (mm)

| | | |
|--------------|-----------------------------|----------------------------|
| LAB FILE ID: | RT 1000 = <u>PP074168.D</u> | RT 750 = <u>PP074169.D</u> |
| | RT 500 = <u>PP074170.D</u> | RT 250 = <u>PP074171.D</u> |

| COMPOUND | RT 1000 | RT 750 | RT 500 | RT 250 | RT 050 | MEAN RT | RT WINDOW FROM | TO |
|----------------------|---------|--------|--------|--------|--------|---------|----------------|------|
| Aroclor-1016-1 (1) | 4.91 | 4.90 | 4.91 | 4.91 | 4.91 | 4.91 | 4.81 | 5.01 |
| Aroclor-1016-2 (2) | 4.96 | 4.96 | 4.96 | 4.97 | 4.97 | 4.96 | 4.86 | 5.06 |
| Aroclor-1016-3 (3) | 5.08 | 5.08 | 5.08 | 5.09 | 5.08 | 5.08 | 4.98 | 5.18 |
| Aroclor-1016-4 (4) | 5.12 | 5.12 | 5.12 | 5.13 | 5.12 | 5.12 | 5.02 | 5.22 |
| Aroclor-1016-5 (5) | 5.34 | 5.34 | 5.34 | 5.34 | 5.34 | 5.34 | 5.24 | 5.44 |
| Aroclor-1260-1 (1) | 6.56 | 6.55 | 6.56 | 6.56 | 6.56 | 6.56 | 6.46 | 6.66 |
| Aroclor-1260-2 (2) | 6.71 | 6.71 | 6.71 | 6.71 | 6.71 | 6.71 | 6.61 | 6.81 |
| Aroclor-1260-3 (3) | 6.92 | 6.92 | 6.92 | 6.92 | 6.92 | 6.92 | 6.82 | 7.02 |
| Aroclor-1260-4 (4) | 7.18 | 7.18 | 7.18 | 7.18 | 7.18 | 7.18 | 7.08 | 7.28 |
| Aroclor-1260-5 (5) | 7.42 | 7.42 | 7.42 | 7.42 | 7.42 | 7.42 | 7.32 | 7.52 |
| Decachlorobiphenyl | 8.83 | 8.83 | 8.83 | 8.83 | 8.83 | 8.83 | 8.73 | 8.93 |
| Tetrachloro-m-xylene | 3.81 | 3.80 | 3.81 | 3.81 | 3.80 | 3.81 | 3.71 | 3.91 |
| Aroclor-1242-1 (1) | 4.91 | 4.90 | 4.91 | 4.91 | 4.90 | 4.91 | 4.81 | 5.01 |
| Aroclor-1242-2 (2) | 4.96 | 4.96 | 4.96 | 4.96 | 4.96 | 4.96 | 4.86 | 5.06 |
| Aroclor-1242-3 (3) | 5.08 | 5.08 | 5.08 | 5.08 | 5.08 | 5.08 | 4.98 | 5.18 |
| Aroclor-1242-4 (4) | 5.16 | 5.16 | 5.16 | 5.17 | 5.16 | 5.16 | 5.06 | 5.26 |
| Aroclor-1242-5 (5) | 5.69 | 5.69 | 5.69 | 5.69 | 5.69 | 5.69 | 5.59 | 5.79 |
| Decachlorobiphenyl | 8.83 | 8.82 | 8.83 | 8.82 | 8.82 | 8.82 | 8.72 | 8.92 |
| Tetrachloro-m-xylene | 3.80 | 3.80 | 3.81 | 3.81 | 3.80 | 3.80 | 3.70 | 3.90 |
| Aroclor-1254-1 (1) | 5.69 | 5.69 | 5.69 | 5.69 | 5.69 | 5.69 | 5.59 | 5.79 |
| Aroclor-1254-2 (2) | 5.84 | 5.84 | 5.83 | 5.83 | 5.84 | 5.84 | 5.74 | 5.94 |
| Aroclor-1254-3 (3) | 6.24 | 6.24 | 6.24 | 6.24 | 6.24 | 6.24 | 6.14 | 6.34 |
| Aroclor-1254-4 (4) | 6.46 | 6.46 | 6.46 | 6.46 | 6.46 | 6.46 | 6.36 | 6.56 |
| Aroclor-1254-5 (5) | 6.88 | 6.88 | 6.88 | 6.88 | 6.88 | 6.88 | 6.78 | 6.98 |
| Decachlorobiphenyl | 8.82 | 8.82 | 8.82 | 8.82 | 8.82 | 8.82 | 8.72 | 8.92 |
| Tetrachloro-m-xylene | 3.81 | 3.80 | 3.80 | 3.80 | 3.80 | 3.80 | 3.70 | 3.90 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

| | | | |
|----------------|----------|----------------------|-----------------------|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| Instrument ID: | ECD_P | Calibration Date(s): | 08/01/2025 08/01/2025 |
| | | Calibration Times: | 12:05 20:28 |

GC Column: ZB-MR1 ID: 0.32 (mm)

| LAB FILE ID: | CF 1000 = | PP074168.D | CF 750 = | PP074169.D | CF | % RSD |
|----------------------|------------|------------|------------|------------|------------|---------------|
| | CF 500 = | PP074170.D | CF 250 = | PP074171.D | | |
| COMPOUND | CF 1000 | CF 750 | CF 500 | CF 250 | CF 050 | % RSD |
| Aroclor-1016-1 (1) | 35273925 | 37423669 | 39112938 | 43859036 | 50614460 | 41256806 14 |
| Aroclor-1016-2 (2) | 51795728 | 55199127 | 58347288 | 64689960 | 73676540 | 60741729 13 |
| Aroclor-1016-3 (3) | 33422245 | 35685564 | 37869938 | 42702196 | 48622620 | 39660513 14 |
| Aroclor-1016-4 (4) | 27792815 | 29586895 | 31487664 | 35862436 | 37992560 | 32544474 12 |
| Aroclor-1016-5 (5) | 27690329 | 29450228 | 31441930 | 35606544 | 38151200 | 32468046 13 |
| Aroclor-1260-1 (1) | 47709498 | 50888675 | 54142460 | 59119820 | 69919860 | 56356063 15 |
| Aroclor-1260-2 (2) | 56508230 | 60166887 | 63913596 | 71401348 | 88771760 | 68152364 18 |
| Aroclor-1260-3 (3) | 45067030 | 48123128 | 50650728 | 57005548 | 65633220 | 53295931 14 |
| Aroclor-1260-4 (4) | 54035441 | 57066597 | 60264502 | 66664376 | 75043960 | 62614975 13 |
| Aroclor-1260-5 (5) | 97992993 | 102942959 | 107738868 | 117332464 | 140517260 | 113304909 14 |
| Decachlorobiphenyl | 852434670 | 894679120 | 940440840 | 1016872040 | 1151380600 | 971161454 12 |
| Tetrachloro-m-xylene | 994587660 | 1038636867 | 1076051520 | 1154524400 | 1327726000 | 1118305289 12 |
| Aroclor-1242-1 (1) | 31512428 | 33419607 | 35918512 | 39696020 | 45782500 | 37265813 14 |
| Aroclor-1242-2 (2) | 47421171 | 49356251 | 53063334 | 57890692 | 64313200 | 54408930 12 |
| Aroclor-1242-3 (3) | 30290298 | 32076312 | 34724744 | 38188808 | 43399140 | 35735860 14 |
| Aroclor-1242-4 (4) | 25177060 | 26633319 | 28691812 | 30950152 | 34640880 | 29218645 12 |
| Aroclor-1242-5 (5) | 29128304 | 32087727 | 34406488 | 38696772 | 43470800 | 35558018 15 |
| Decachlorobiphenyl | 880786000 | 919506067 | 984418560 | 1056643120 | 1205252000 | 1009321149 13 |
| Tetrachloro-m-xylene | 1043240650 | 1075688493 | 1133074840 | 1202593000 | 1370780600 | 1165075517 11 |
| Aroclor-1254-1 (1) | 49559228 | 49811068 | 53907260 | 53993024 | 55934640 | 52641044 5 |
| Aroclor-1254-2 (2) | 70079706 | 72686637 | 78166692 | 86577056 | 90012700 | 79504558 10 |
| Aroclor-1254-3 (3) | 76495408 | 79340601 | 84479860 | 93420496 | 102844700 | 87316213 12 |
| Aroclor-1254-4 (4) | 57834344 | 59926583 | 63428804 | 69599176 | 68258480 | 63809477 8 |
| Aroclor-1254-5 (5) | 73335985 | 76078215 | 80654566 | 88040632 | 87614400 | 81144760 8 |
| Decachlorobiphenyl | 901613940 | 929059080 | 979122040 | 1057269880 | 1005303000 | 974473588 6 |
| Tetrachloro-m-xylene | 1055318110 | 1070331613 | 1114290760 | 1189360720 | 1187072000 | 1123274641 6 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION FACTOR OF INITIAL CALIBRATION

| | | | |
|----------------|----------|----------------------|-----------------------|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| Instrument ID: | ECD_P | Calibration Date(s): | 08/01/2025 08/01/2025 |
| | | Calibration Times: | 12:05 20:28 |
| GC Column: | ZB-MR2 | ID: | 0.32 (mm) |

| LAB FILE ID: | CF 1000 = | PP074168.D | CF 750 = | PP074169.D | CF | % RSD |
|----------------------|------------|------------|------------|------------|------------|---------------|
| | CF 500 = | PP074170.D | CF 250 = | PP074171.D | | |
| COMPOUND | CF 1000 | CF 750 | CF 500 | CF 250 | CF 050 | % RSD |
| Aroclor-1016-1 (1) | 401748995 | 398824608 | 399912360 | 403735356 | 390215520 | 398887368 1 |
| Aroclor-1016-2 (2) | 186854426 | 192495525 | 187577416 | 198284052 | 173833620 | 187809008 5 |
| Aroclor-1016-3 (3) | 104048217 | 106580327 | 106062448 | 114925596 | 98731580 | 106069634 5 |
| Aroclor-1016-4 (4) | 102945349 | 106576167 | 111089380 | 109624088 | 115865320 | 109220061 4 |
| Aroclor-1016-5 (5) | 116097268 | 118066511 | 118643196 | 118883084 | 113126240 | 116963260 2 |
| Aroclor-1260-1 (1) | 398303416 | 397444124 | 405725820 | 438106428 | 380206020 | 403957162 5 |
| Aroclor-1260-2 (2) | 301304557 | 308158192 | 308266150 | 305734868 | 340030740 | 312698901 5 |
| Aroclor-1260-3 (3) | 408378449 | 417603121 | 404068616 | 383320072 | 357221180 | 394118288 6 |
| Aroclor-1260-4 (4) | 295359710 | 299954812 | 306136602 | 280781712 | 272663920 | 290979351 4 |
| Aroclor-1260-5 (5) | 811772813 | 805780147 | 794112086 | 732491376 | 642892660 | 757409816 9 |
| Decachlorobiphenyl | 6091085760 | 6145498480 | 6064775080 | 5991469080 | 5775302800 | 6013626240 2 |
| Tetrachloro-m-xylene | 4204747790 | 4209506627 | 3997167900 | 3658659200 | 3102045200 | 3834425343 12 |
| Aroclor-1242-1 (1) | 341272725 | 348537165 | 356175586 | 358260688 | 321457320 | 345140697 4 |
| Aroclor-1242-2 (2) | 162660327 | 171629959 | 165033416 | 168697644 | 148866940 | 163377657 5 |
| Aroclor-1242-3 (3) | 93075141 | 96957855 | 92088854 | 97223352 | 81897380 | 92248516 6 |
| Aroclor-1242-4 (4) | 117292839 | 116784915 | 126377070 | 120581608 | 116071680 | 119421622 3 |
| Aroclor-1242-5 (5) | 140731652 | 152438257 | 148354640 | 155481924 | 150793560 | 149560007 4 |
| Decachlorobiphenyl | 6182103300 | 6198353267 | 6343202860 | 6254049920 | 5638925600 | 6123326989 5 |
| Tetrachloro-m-xylene | 4380731720 | 4319851627 | 4244718880 | 3977934440 | 3138312200 | 4012309773 13 |
| Aroclor-1254-1 (1) | 384557283 | 361450625 | 385081202 | 377494716 | 322325960 | 366181957 7 |
| Aroclor-1254-2 (2) | 284389782 | 276601852 | 284135592 | 290728916 | 255228600 | 278216948 5 |
| Aroclor-1254-3 (3) | 520239168 | 520693099 | 508814756 | 526662268 | 369647720 | 489211402 13 |
| Aroclor-1254-4 (4) | 378053305 | 389619320 | 377098978 | 394351108 | 298703960 | 367565334 10 |
| Aroclor-1254-5 (5) | 425051302 | 410967521 | 398226716 | 393575444 | 298014540 | 385167105 12 |
| Decachlorobiphenyl | 6206832720 | 6179384467 | 6118770460 | 6279475360 | 4842174000 | 5925327401 10 |
| Tetrachloro-m-xylene | 4358828150 | 4220486587 | 4040036280 | 3680489520 | 2529500800 | 3765868267 20 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

| | | | |
|----------------|-----------------|-------------------|-------------------------------------|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| Instrument ID: | <u>ECD_P</u> | Date(s) Analyzed: | <u>08/01/2025</u> <u>08/01/2025</u> |
| GC Column: | <u>ZB-MR1</u> | ID: | <u>0.32</u> (mm) |

| COMPOUND | AMOUNT (ng) | PEAK | RT | RT WINDOW | | CALIBRATION FACTOR |
|--------------|----------------|------|-------|-----------|-------|-----------------------|
| | | | | FROM | TO | |
| Aroclor-1221 | 500 | 1 | 4.86 | 4.76 | 4.96 | 16763600 |
| | | 2 | 4.94 | 4.84 | 5.04 | 12601100 |
| | | 3 | 5.02 | 4.92 | 5.12 | 36635200 |
| | | 4 | 0.00 | | | 0 |
| | | 5 | 0.00 | | | 0 |
| Aroclor-1232 | 500 | 1 | 5.02 | 4.92 | 5.12 | 29037400 |
| | | 2 | 5.55 | 5.45 | 5.65 | 15042700 |
| | | 3 | 5.83 | 5.73 | 5.93 | 29001800 |
| | | 4 | 5.99 | 5.89 | 6.09 | 15468800 |
| | | 5 | 6.08 | 5.98 | 6.18 | 11716000 |
| Aroclor-1248 | 500 | 1 | 5.81 | 5.71 | 5.91 | 28382600 |
| | | 2 | 6.08 | 5.98 | 6.18 | 40187600 |
| | | 3 | 6.28 | 6.18 | 6.38 | 44640800 |
| | | 4 | 6.68 | 6.58 | 6.78 | 51582200 |
| | | 5 | 6.72 | 6.62 | 6.82 | 53240200 |
| Aroclor-1262 | 500 | 1 | 8.24 | 8.14 | 8.34 | 75789600 |
| | | 2 | 8.56 | 8.46 | 8.66 | 130430000 |
| | | 3 | 8.89 | 8.79 | 8.99 | 94070800 |
| | | 4 | 8.97 | 8.87 | 9.07 | 72851600 |
| | | 5 | 9.65 | 9.55 | 9.75 | 50922600 |
| Aroclor-1268 | 500 | 1 | 8.88 | 8.78 | 8.98 | 158028000 |
| | | 2 | 8.98 | 8.88 | 9.08 | 146028000 |
| | | 3 | 9.22 | 9.12 | 9.32 | 121402000 |
| | | 4 | 9.64 | 9.54 | 9.74 | 59648200 |
| | | 5 | 10.08 | 9.98 | 10.18 | 357940000 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

INITIAL CALIBRATION OF MULTICOMPONENT ANALYTES

| | | | |
|----------------|-----------------|-------------------|-------------------|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| Instrument ID: | <u>ECD_P</u> | Date(s) Analyzed: | <u>08/01/2025</u> |
| GC Column: | <u>ZB-MR2</u> | ID: | <u>0.32</u> (mm) |

| COMPOUND | AMOUNT (ng) | PEAK | RT | RT WINDOW | | CALIBRATION FACTOR |
|--------------|----------------|------|------|-----------|------|-----------------------|
| | | | | FROM | TO | |
| Aroclor-1221 | 500 | 1 | 4.02 | 3.92 | 4.12 | 49085200 |
| | | 2 | 4.10 | 4.00 | 4.20 | 35889400 |
| | | 3 | 4.18 | 4.08 | 4.28 | 135225000 |
| | | 4 | 0.00 | | | 0 |
| | | 5 | 0.00 | | | 0 |
| Aroclor-1232 | 500 | 1 | 4.18 | 4.08 | 4.28 | 101362000 |
| | | 2 | 4.90 | 4.80 | 5.00 | 174266000 |
| | | 3 | 5.08 | 4.98 | 5.18 | 45816600 |
| | | 4 | 5.16 | 5.06 | 5.26 | 58010800 |
| | | 5 | 5.34 | 5.24 | 5.44 | 46979400 |
| Aroclor-1248 | 500 | 1 | 4.90 | 4.80 | 5.00 | 223628000 |
| | | 2 | 5.12 | 5.02 | 5.22 | 147770000 |
| | | 3 | 5.16 | 5.06 | 5.26 | 179546000 |
| | | 4 | 5.34 | 5.24 | 5.44 | 167057000 |
| | | 5 | 5.73 | 5.63 | 5.83 | 302782000 |
| Aroclor-1262 | 500 | 1 | 6.92 | 6.82 | 7.02 | 563142000 |
| | | 2 | 7.18 | 7.08 | 7.28 | 401024000 |
| | | 3 | 7.70 | 7.60 | 7.80 | 359470000 |
| | | 4 | 7.76 | 7.66 | 7.86 | 666922000 |
| | | 5 | 8.26 | 8.16 | 8.36 | 283268000 |
| Aroclor-1268 | 500 | 1 | 7.70 | 7.60 | 7.80 | 1169220000 |
| | | 2 | 7.76 | 7.66 | 7.86 | 1148130000 |
| | | 3 | 7.97 | 7.87 | 8.07 | 891866000 |
| | | 4 | 8.26 | 8.16 | 8.36 | 329470000 |
| | | 5 | 8.56 | 8.46 | 8.66 | 2772300000 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:05
 Operator : YP\AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:05:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|---------|
| 1) SA Tetrachlor... | 4.660 | 3.805 | 99458766 | 420.5E6 | 96.066 | 102.531 |
| 2) SA Decachlor... | 10.437 | 8.826 | 85243467 | 609.1E6 | 95.091 | 100.216 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|---------|----------|
| 3) L1 AR-1016-1 | 5.812 | 4.905 | 35273925 | 401.7E6 | 948.391 | 1002.291 |
| 4) L1 AR-1016-2 | 5.833 | 4.963 | 51795728 | 186.9E6 | 940.518 | 998.069 |
| 5) L1 AR-1016-3 | 5.896 | 5.083 | 33422245 | 104.0E6 | 937.613 | 990.413 |
| 6) L1 AR-1016-4 | 5.993 | 5.124 | 27792815 | 102.9E6 | 937.672 | 961.950 |
| 7) L1 AR-1016-5 | 6.285 | 5.338 | 27690329 | 116.1E6 | 936.556 | 989.154 |
| 31) L7 AR-1260-1 | 7.403 | 6.555 | 47709498 | 398.3E6 | 936.840 | 990.768 |
| 32) L7 AR-1260-2 | 7.656 | 6.711 | 56508230 | 301.3E6 | 938.505 | 988.580 |
| 33) L7 AR-1260-3 | 8.013 | 6.921 | 45067030 | 408.4E6 | 941.665 | 1005.305 |
| 34) L7 AR-1260-4 | 8.241 | 7.180 | 54035441 | 295.4E6 | 945.503 | 982.083 |
| 35) L7 AR-1260-5 | 8.567 | 7.419 | 97992993 | 811.8E6 | 952.628 | 1010.998 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074168.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:05
 Operator : YP\AJ
 Sample : AR1660ICC1000
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:05:03 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

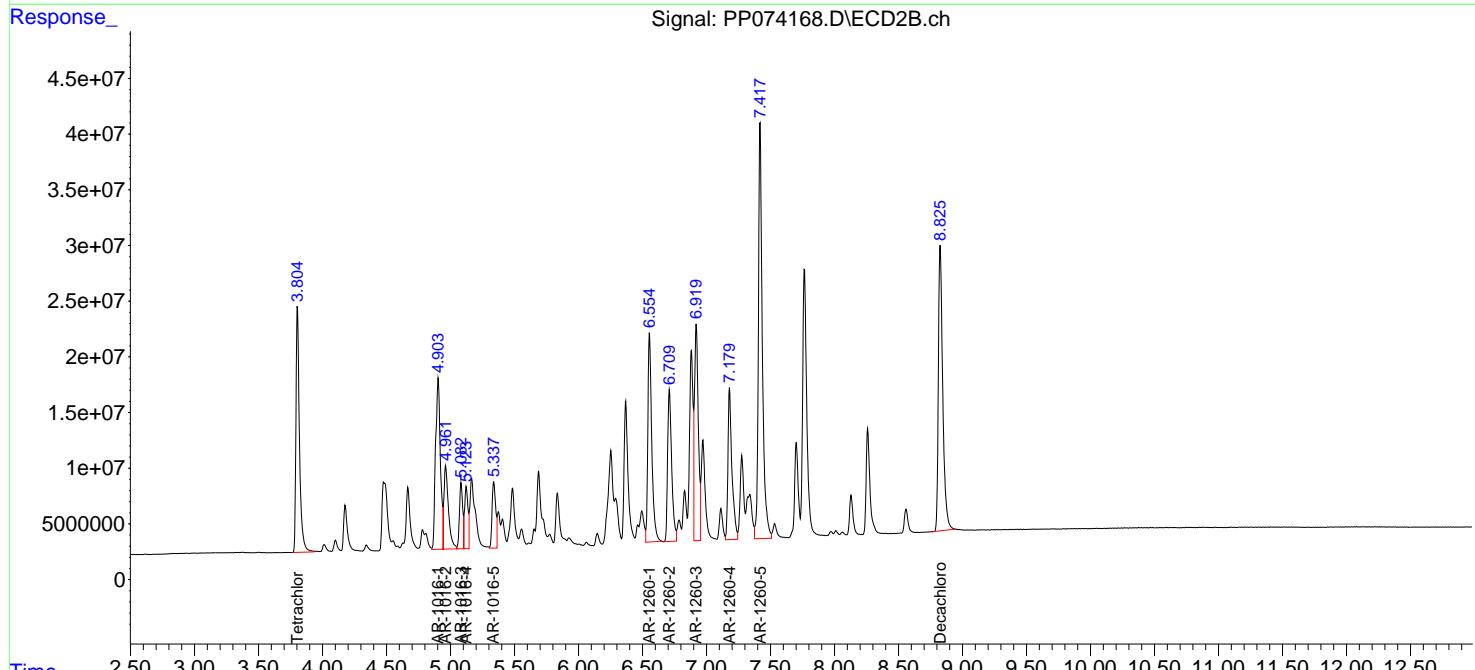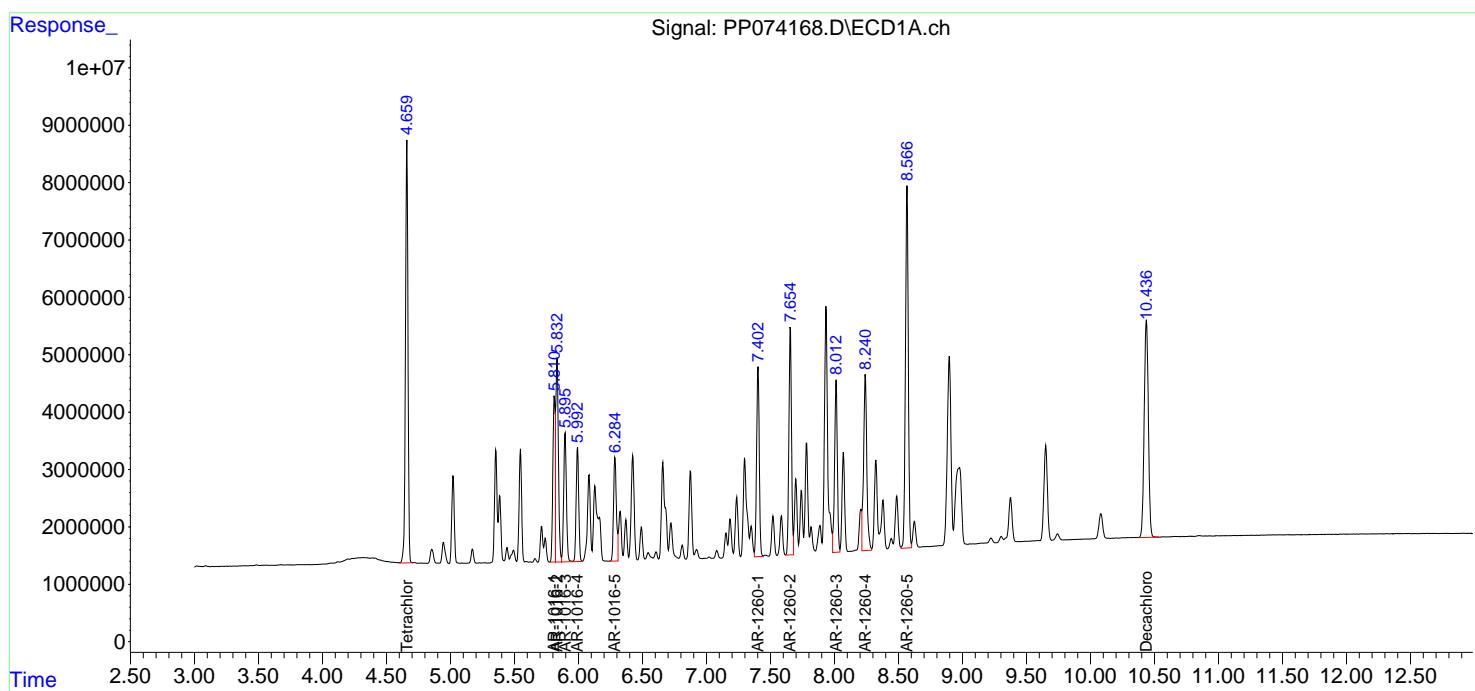


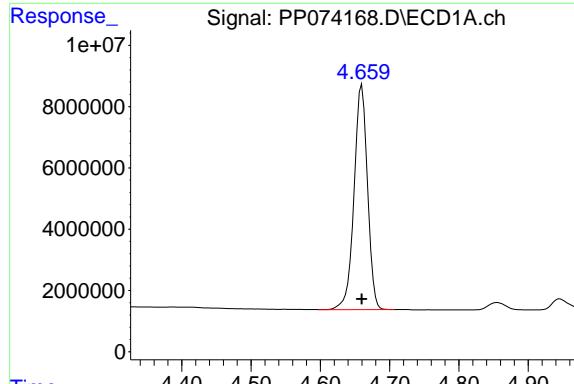

#1 Tetrachloro-m-xylene


R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 99458766
Conc: 96.07 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

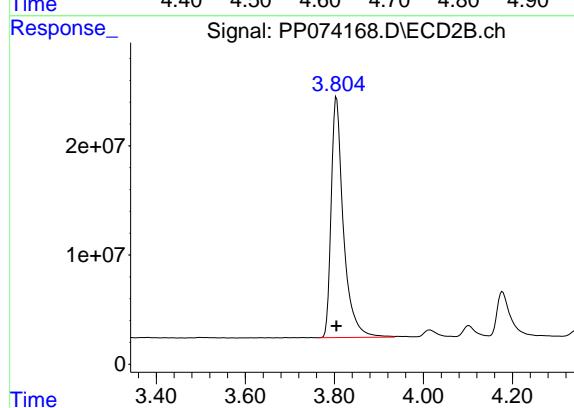


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 420474779
Conc: 102.53 ng/ml

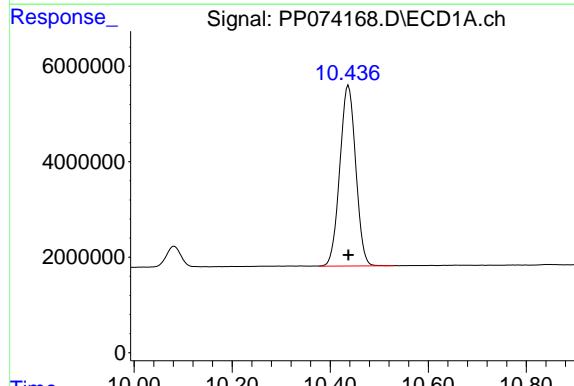


#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 85243467
Conc: 95.09 ng/ml

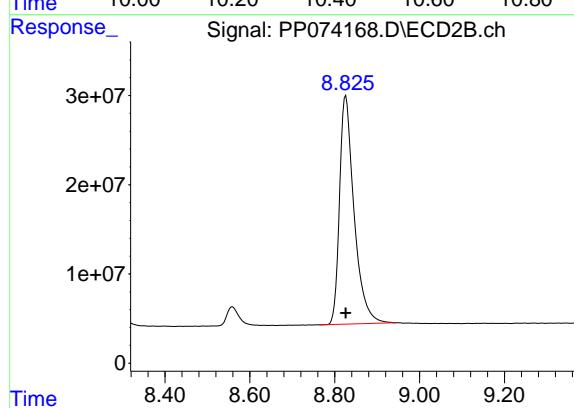

#2 Decachlorobiphenyl

R.T.: 8.826 min
Delta R.T.: 0.000 min
Response: 609108576
Conc: 100.22 ng/ml

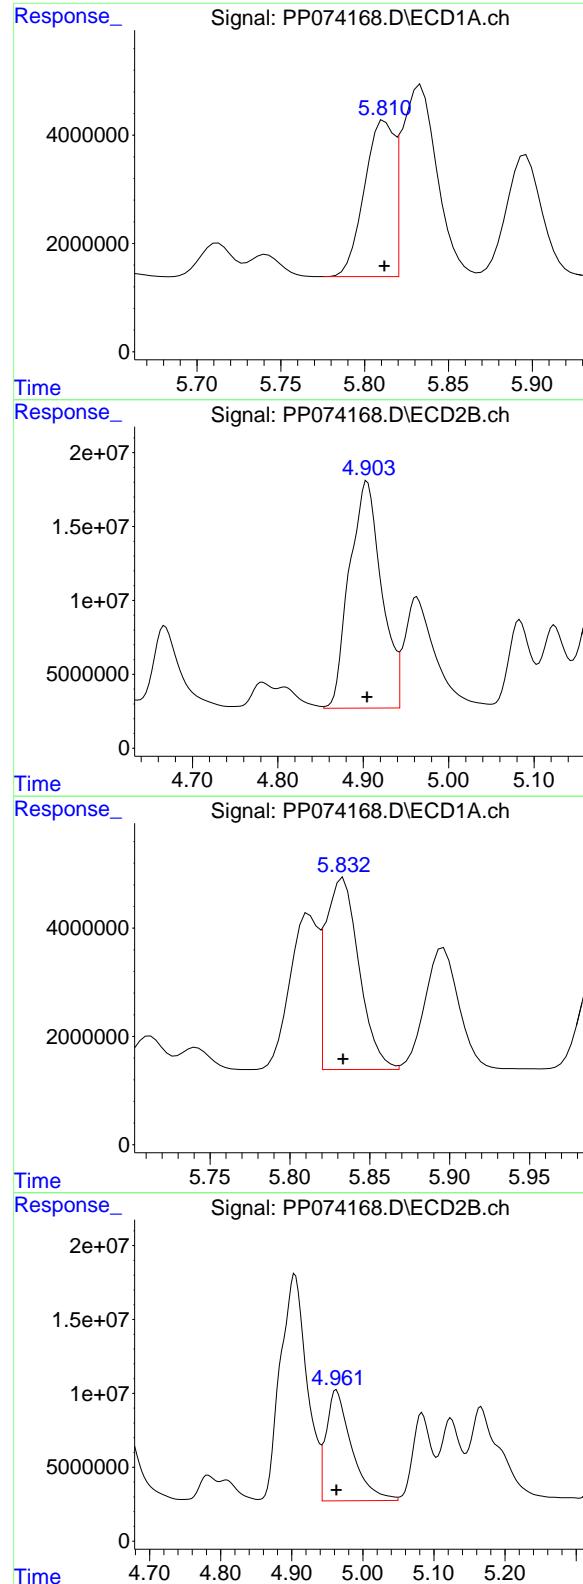

#3 AR-1016-1

R.T.: 5.812 min
 Delta R.T.: 0.000 min
 Response: 35273925
 Conc: 948.39 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC1000

#3 AR-1016-1





R.T.: 4.905 min
 Delta R.T.: 0.000 min
 Response: 401748995
 Conc: 1002.29 ng/ml

#4 AR-1016-2

R.T.: 5.833 min
 Delta R.T.: 0.000 min
 Response: 51795728
 Conc: 940.52 ng/ml

#4 AR-1016-2

R.T.: 4.963 min
 Delta R.T.: 0.000 min
 Response: 186854426
 Conc: 998.07 ng/ml

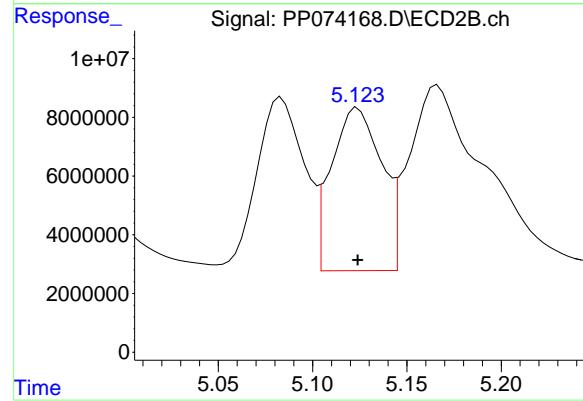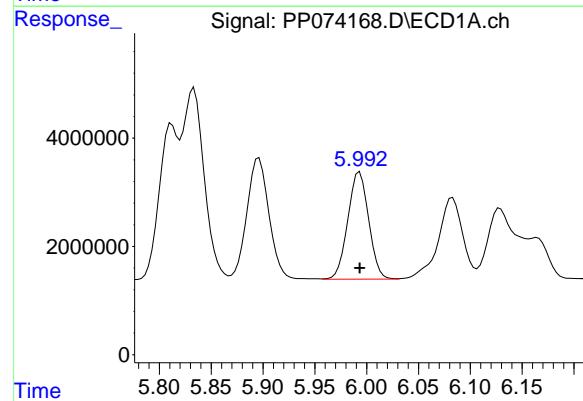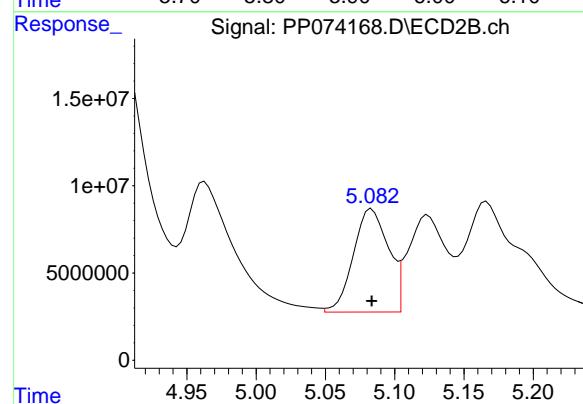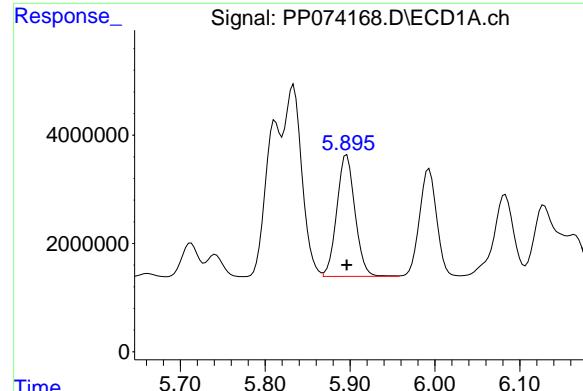

#5 AR-1016-3

R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 33422245
Conc: 937.61 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

#5 AR-1016-3





R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 104048217
Conc: 990.41 ng/ml

#6 AR-1016-4

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 27792815
Conc: 937.67 ng/ml

#6 AR-1016-4

R.T.: 5.124 min
Delta R.T.: 0.000 min
Response: 102945349
Conc: 961.95 ng/ml

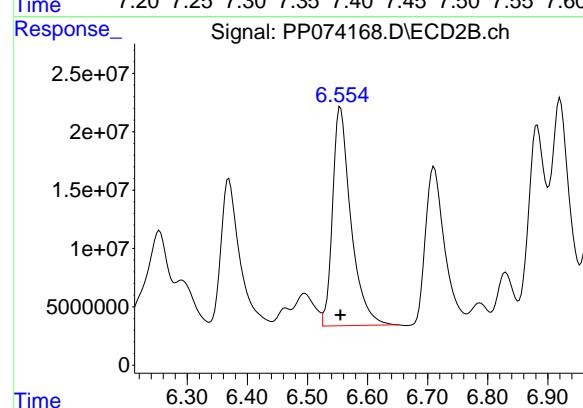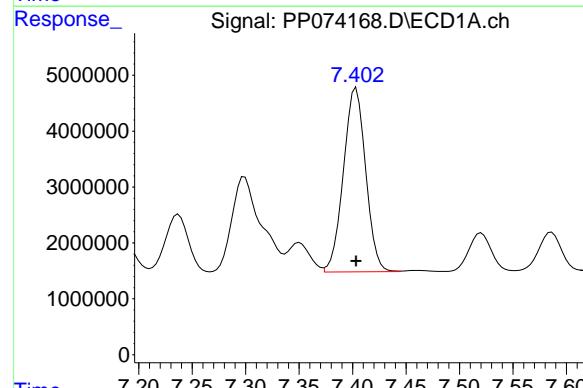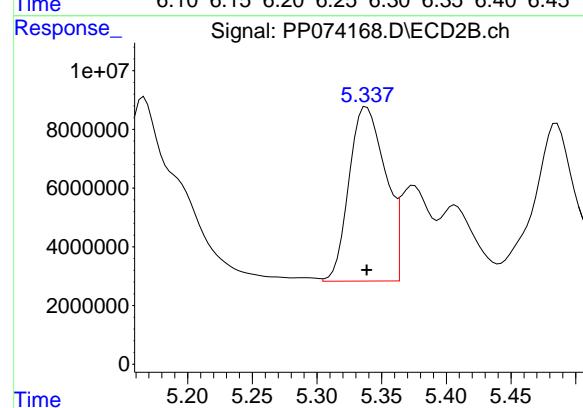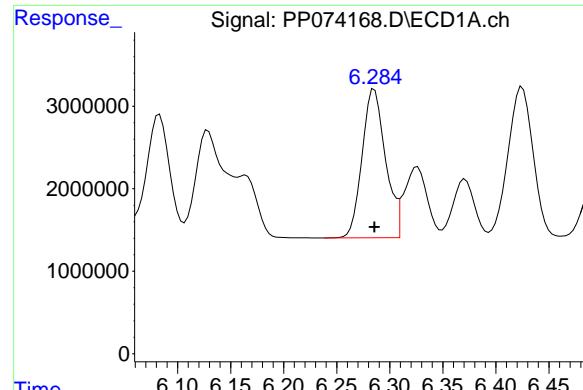

#7 AR-1016-5

R.T.: 6.285 min
 Delta R.T.: 0.000 min
 Response: 27690329
 Conc: 936.56 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC1000

#7 AR-1016-5

R.T.: 5.338 min
 Delta R.T.: 0.000 min
 Response: 116097268
 Conc: 989.15 ng/ml

#31 AR-1260-1

R.T.: 7.403 min
 Delta R.T.: 0.000 min
 Response: 47709498
 Conc: 936.84 ng/ml





#31 AR-1260-1

R.T.: 6.555 min
 Delta R.T.: 0.000 min
 Response: 398303416
 Conc: 990.77 ng/ml

#32 AR-1260-2

R.T.: 7.656 min
 Delta R.T.: 0.000 min
 Response: 56508230
 Conc: 938.50 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

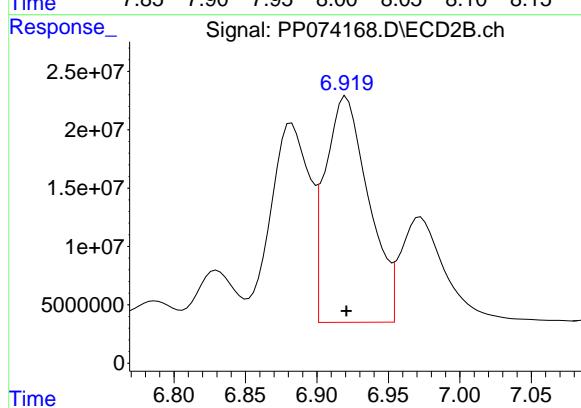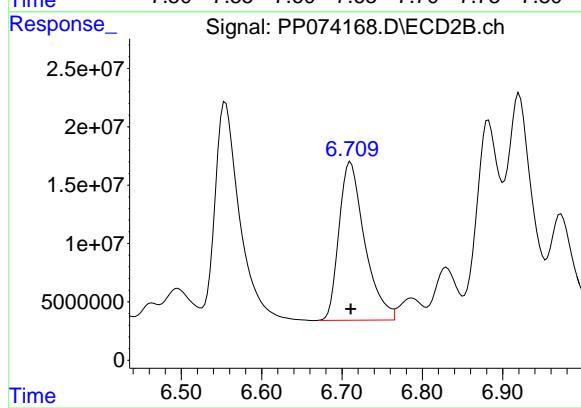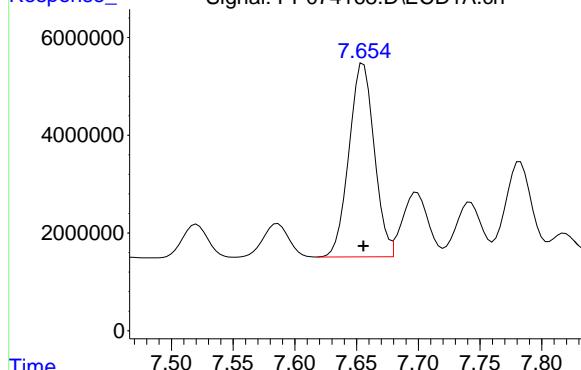

#32 AR-1260-2

R.T.: 6.711 min
 Delta R.T.: 0.000 min
 Response: 301304557
 Conc: 988.58 ng/ml

#33 AR-1260-3

R.T.: 8.013 min
 Delta R.T.: 0.000 min
 Response: 45067030
 Conc: 941.66 ng/ml





#33 AR-1260-3

R.T.: 6.921 min
 Delta R.T.: 0.000 min
 Response: 408378449
 Conc: 1005.30 ng/ml

#34 AR-1260-4

R.T.: 8.241 min
 Delta R.T.: 0.000 min
 Response: 54035441
 Conc: 945.50 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC1000

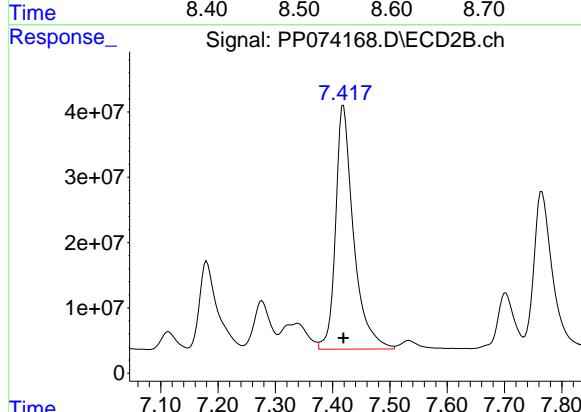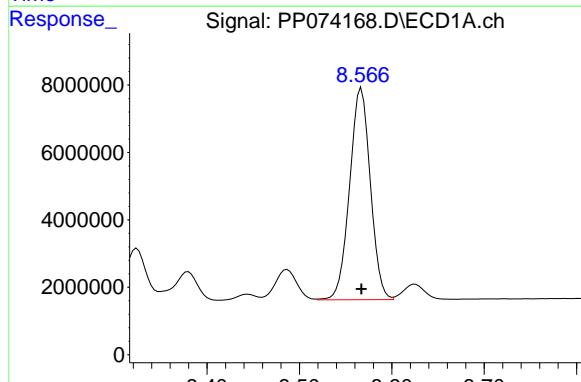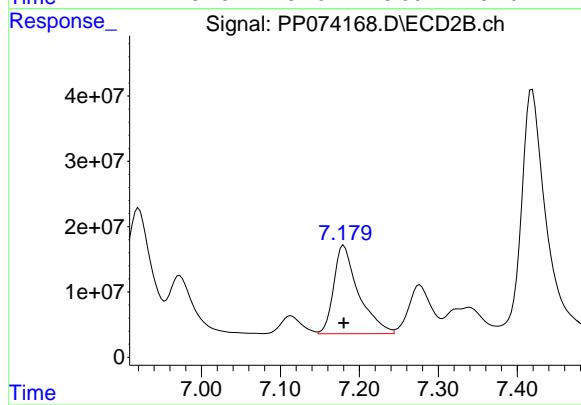

#34 AR-1260-4

R.T.: 7.180 min
 Delta R.T.: 0.000 min
 Response: 295359710
 Conc: 982.08 ng/ml

#35 AR-1260-5

R.T.: 8.567 min
 Delta R.T.: 0.000 min
 Response: 97992993
 Conc: 952.63 ng/ml

#35 AR-1260-5

R.T.: 7.419 min
 Delta R.T.: 0.000 min
 Response: 811772813
 Conc: 1011.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:22
 Operator : YP\AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:07:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.662 | 3.804 | 77897765 | 315.7E6 | 75.160 | 76.312 |
| 2) SA Decachlor... | 10.440 | 8.825 | 67100934 | 460.9E6 | 74.902 | 75.554 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 5.814 | 4.904 | 28067752 | 299.1E6 | 753.089 | 747.493 |
| 4) L1 AR-1016-2 | 5.836 | 4.962 | 41399345 | 144.4E6 | 751.158 | 763.969 |
| 5) L1 AR-1016-3 | 5.898 | 5.082 | 26764173 | 79935245 | 750.553 | 757.223 |
| 6) L1 AR-1016-4 | 5.995 | 5.122 | 22190171 | 79932125 | 749.100 | 747.936 |
| 7) L1 AR-1016-5 | 6.288 | 5.337 | 22087671 | 88549883 | 748.037 | 752.960 |
| 31) L7 AR-1260-1 | 7.405 | 6.554 | 38166506 | 298.1E6 | 749.634 | 744.294 |
| 32) L7 AR-1260-2 | 7.658 | 6.709 | 45125165 | 231.1E6 | 749.634 | 755.513 |
| 33) L7 AR-1260-3 | 8.016 | 6.919 | 36092346 | 313.2E6 | 752.756 | 763.877 |
| 34) L7 AR-1260-4 | 8.244 | 7.178 | 42799948 | 225.0E6 | 749.270 | 748.680 |
| 35) L7 AR-1260-5 | 8.569 | 7.417 | 77207219 | 604.3E6 | 750.374 | 751.765 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074169.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:22
 Operator : YP\AJ
 Sample : AR1660ICC750
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:07:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

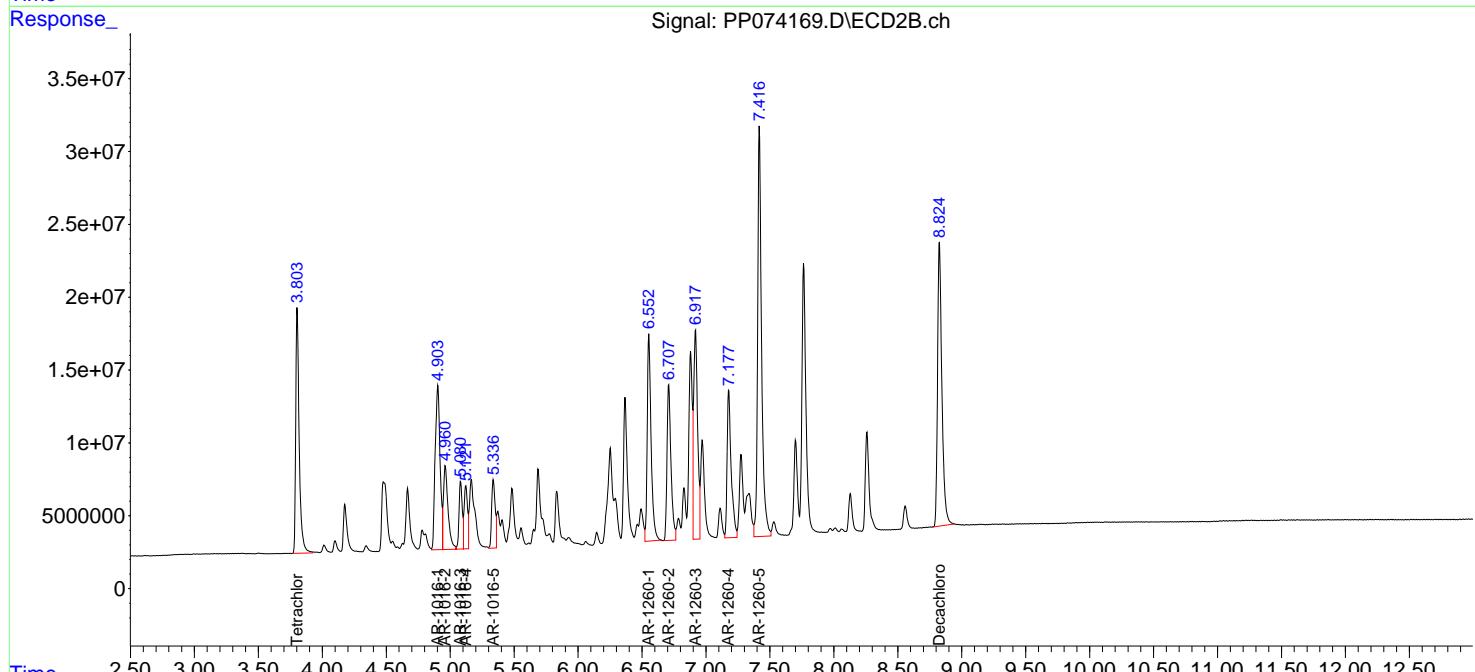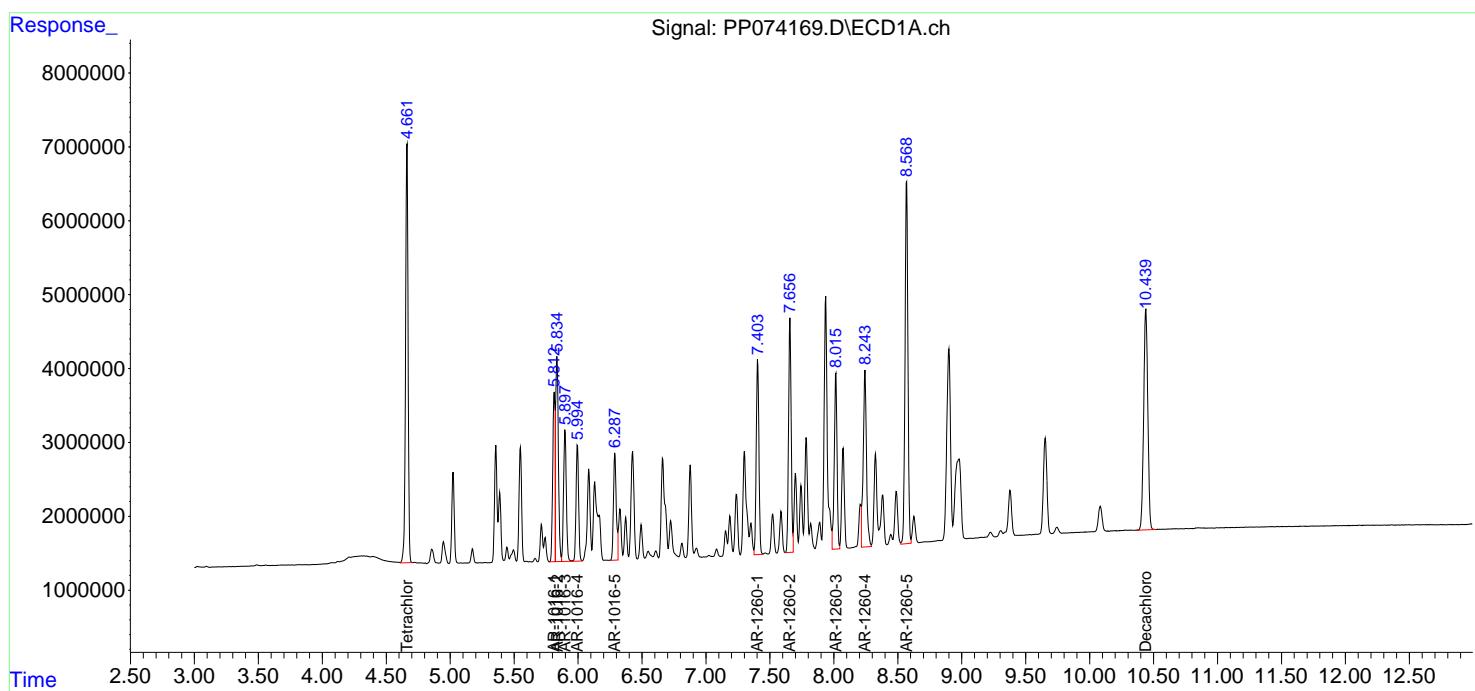


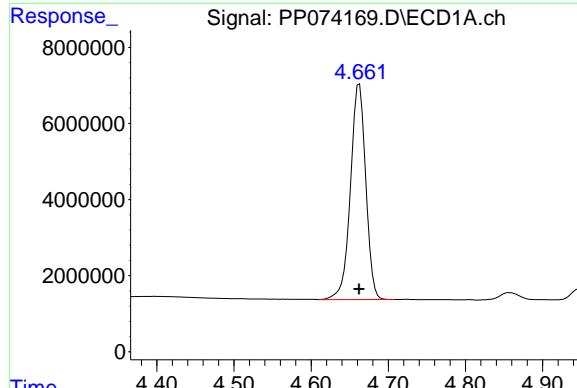

#1 Tetrachloro-m-xylene


R.T.: 4.662 min
Delta R.T.: 0.000 min
Response: 77897765
Conc: 75.16 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

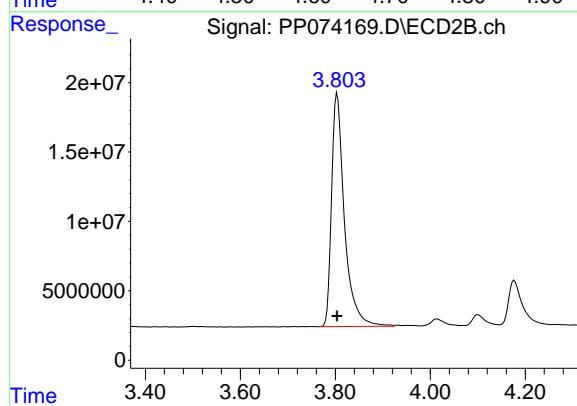


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 315712997
Conc: 76.31 ng/ml

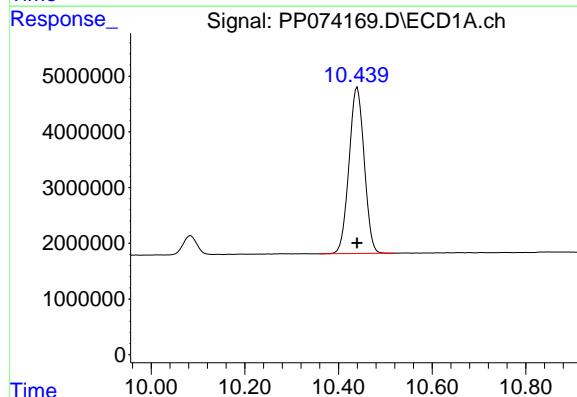

#2 Decachlorobiphenyl

R.T.: 10.440 min
Delta R.T.: 0.000 min
Response: 67100934
Conc: 74.90 ng/ml

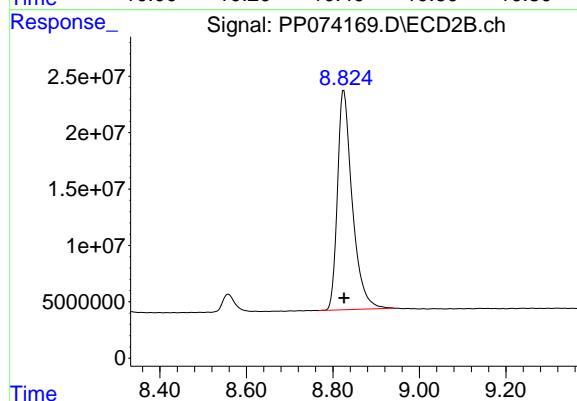


#2 Decachlorobiphenyl

R.T.: 8.825 min
Delta R.T.: 0.000 min
Response: 460912386
Conc: 75.55 ng/ml

#3 AR-1016-1


R.T.: 5.814 min
 Delta R.T.: 0.000 min
 Response: 28067752
 Conc: 753.09 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC750

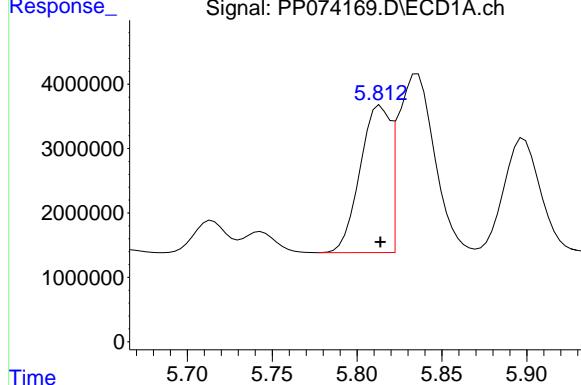


#3 AR-1016-1

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 299118456
 Conc: 747.49 ng/ml

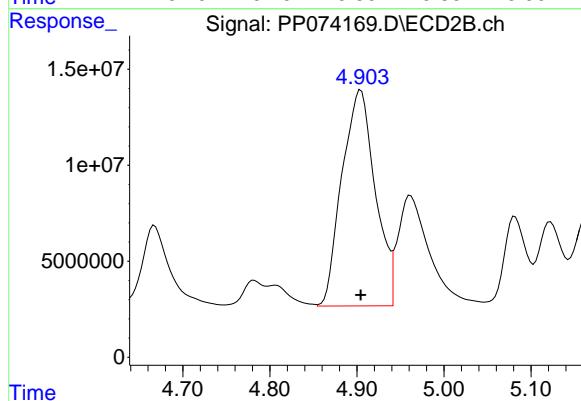


#4 AR-1016-2

R.T.: 5.836 min
 Delta R.T.: 0.000 min
 Response: 41399345
 Conc: 751.16 ng/ml



#4 AR-1016-2


R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 144371644
 Conc: 763.97 ng/ml

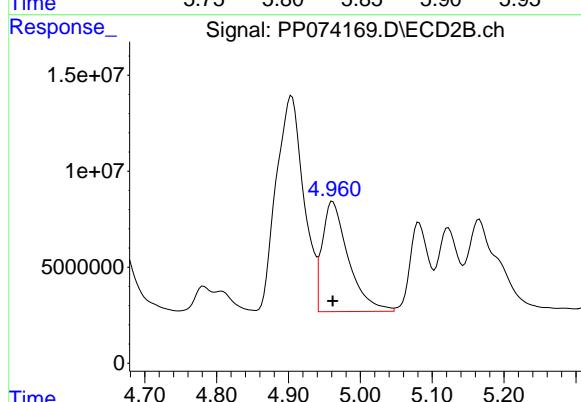

#5 AR-1016-3


R.T.: 5.898 min
 Delta R.T.: 0.000 min
 Response: 26764173
 Conc: 750.55 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

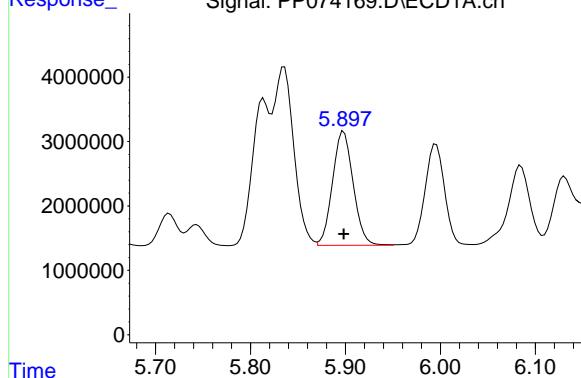

#5 AR-1016-3

R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 79935245
 Conc: 757.22 ng/ml

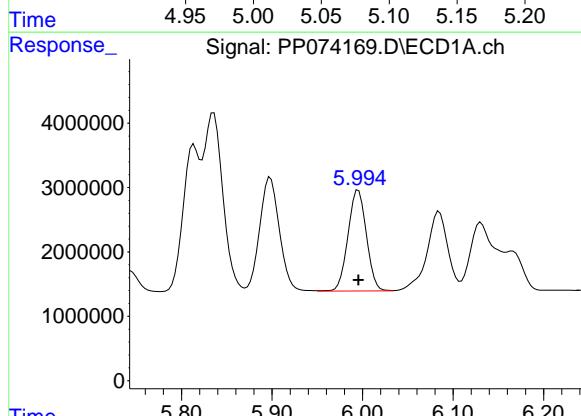


#6 AR-1016-4

R.T.: 5.995 min
 Delta R.T.: 0.000 min
 Response: 22190171
 Conc: 749.10 ng/ml

#6 AR-1016-4

R.T.: 5.122 min
 Delta R.T.: 0.000 min
 Response: 79932125
 Conc: 747.94 ng/ml

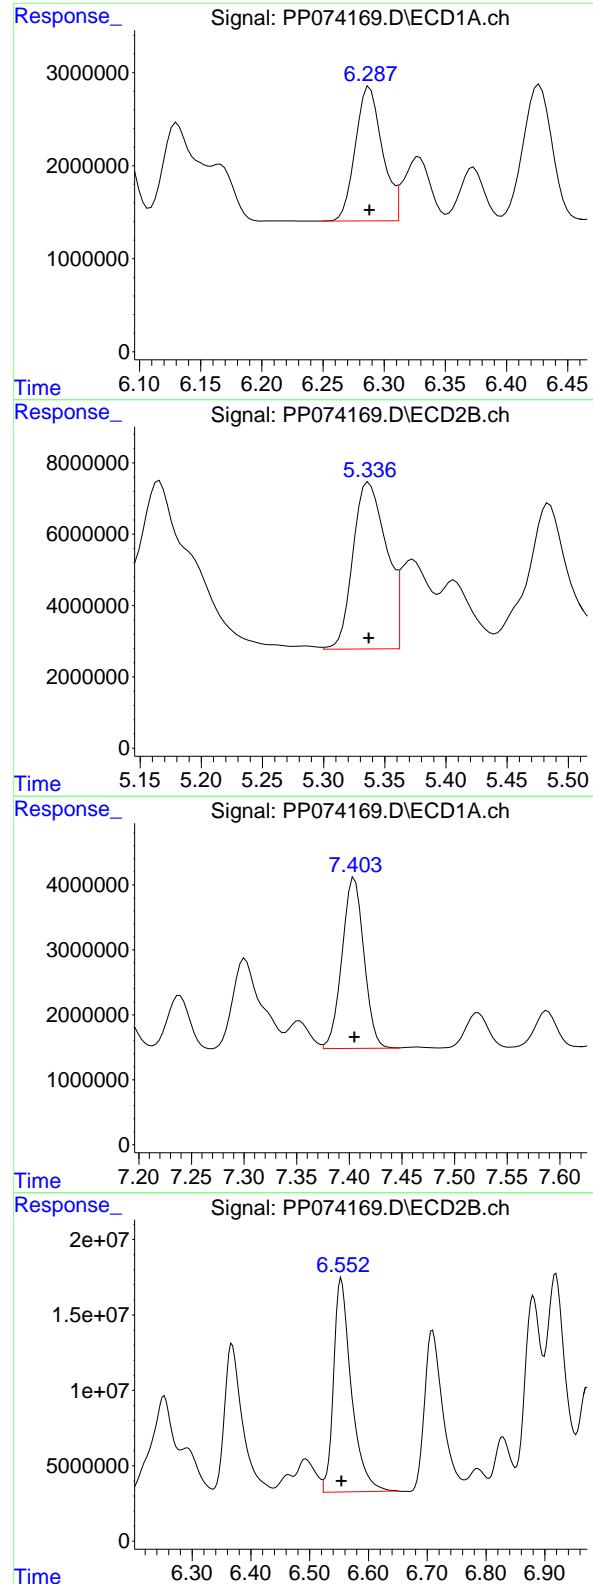

#7 AR-1016-5

R.T.: 6.288 min
 Delta R.T.: 0.000 min
 Response: 22087671
 Conc: 748.04 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC750

#7 AR-1016-5

R.T.: 5.337 min
 Delta R.T.: 0.000 min
 Response: 88549883
 Conc: 752.96 ng/ml

#31 AR-1260-1

R.T.: 7.405 min
 Delta R.T.: 0.000 min
 Response: 38166506
 Conc: 749.63 ng/ml


#31 AR-1260-1

R.T.: 6.554 min
 Delta R.T.: 0.000 min
 Response: 298083093
 Conc: 744.29 ng/ml

#32 AR-1260-2


R.T.: 7.658 min
 Delta R.T.: 0.000 min
 Response: 45125165
 Conc: 749.63 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

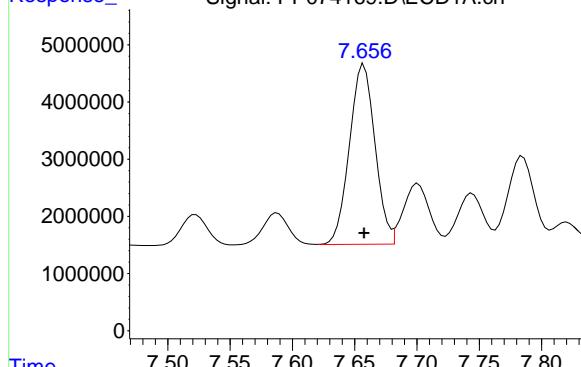


#32 AR-1260-2

R.T.: 6.709 min
 Delta R.T.: 0.000 min
 Response: 231118644
 Conc: 755.51 ng/ml

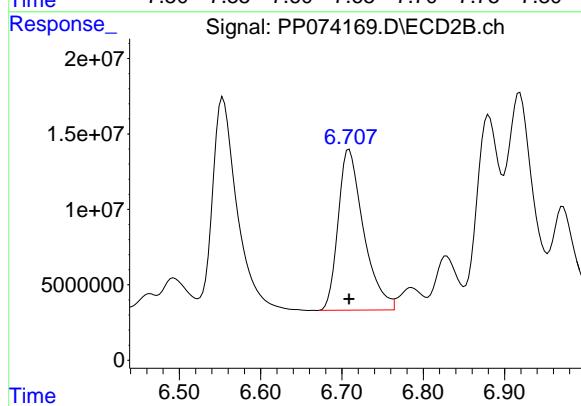


#33 AR-1260-3

R.T.: 8.016 min
 Delta R.T.: 0.000 min
 Response: 36092346
 Conc: 752.76 ng/ml



#33 AR-1260-3





R.T.: 6.919 min
 Delta R.T.: 0.000 min
 Response: 313202341
 Conc: 763.88 ng/ml

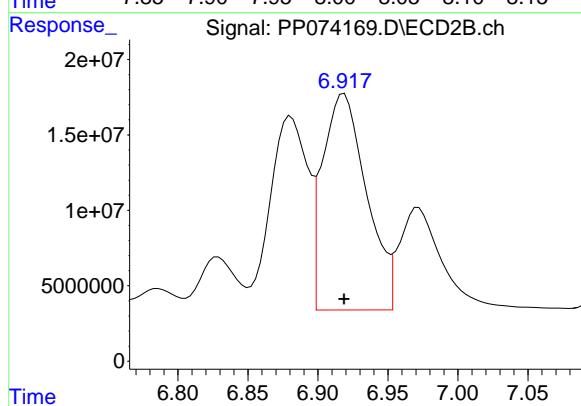

#34 AR-1260-4

R.T.: 8.244 min
 Delta R.T.: 0.000 min
 Response: 42799948
 Conc: 749.27 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC750

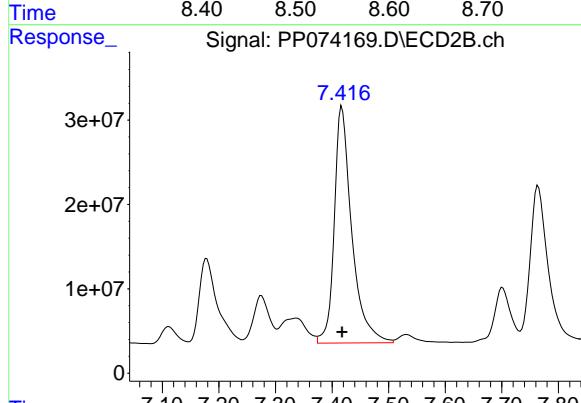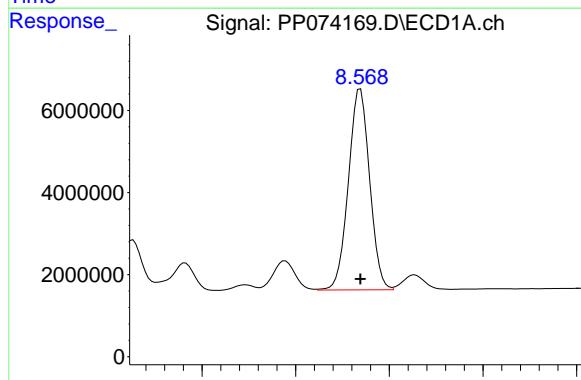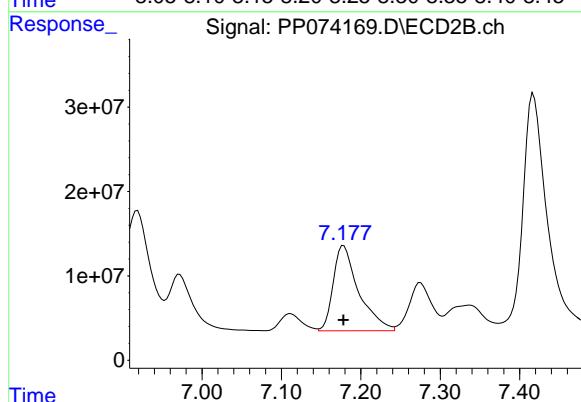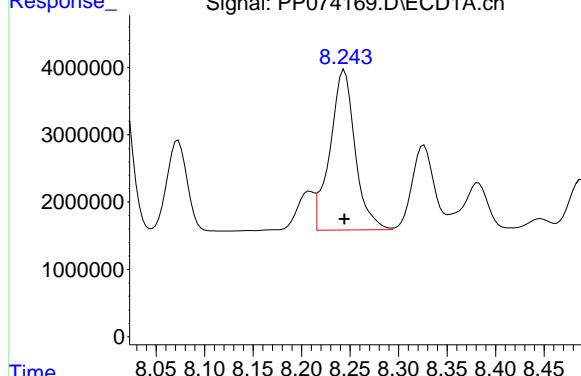

#34 AR-1260-4

R.T.: 7.178 min
 Delta R.T.: 0.000 min
 Response: 224966109
 Conc: 748.68 ng/ml

#35 AR-1260-5

R.T.: 8.569 min
 Delta R.T.: 0.000 min
 Response: 77207219
 Conc: 750.37 ng/ml

#35 AR-1260-5

R.T.: 7.417 min
 Delta R.T.: 0.000 min
 Response: 604335110
 Conc: 751.76 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:38
 Operator : YP\AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:02:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.660 | 3.805 | 53802576 | 199.9E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.438 | 8.826 | 47022042 | 303.2E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 5.812 | 4.906 | 19556469 | 200.0E6 | 500.000 | 500.000 |
| 4) L1 AR-1016-2 | 5.833 | 4.963 | 29173644 | 93788708 | 500.000 | 500.000 |
| 5) L1 AR-1016-3 | 5.896 | 5.083 | 18934969 | 53031224 | 500.000 | 500.000 |
| 6) L1 AR-1016-4 | 5.993 | 5.123 | 15743832 | 55544690 | 500.000 | 500.000 |
| 7) L1 AR-1016-5 | 6.286 | 5.339 | 15720965 | 59321598 | 500.000 | 500.000 |
| 31) L7 AR-1260-1 | 7.403 | 6.555 | 27071230 | 202.9E6 | 500.000 | 500.000 |
| 32) L7 AR-1260-2 | 7.655 | 6.709 | 31956798 | 154.1E6 | 500.000 | 500.000 |
| 33) L7 AR-1260-3 | 8.013 | 6.919 | 25325364 | 202.0E6 | 500.000 | 500.000 |
| 34) L7 AR-1260-4 | 8.242 | 7.179 | 30132251 | 153.1E6 | 500.000 | 500.000 |
| 35) L7 AR-1260-5 | 8.568 | 7.418 | 53869434 | 397.1E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:38
 Operator : YP\AJ
 Sample : AR1660ICC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:02:29 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

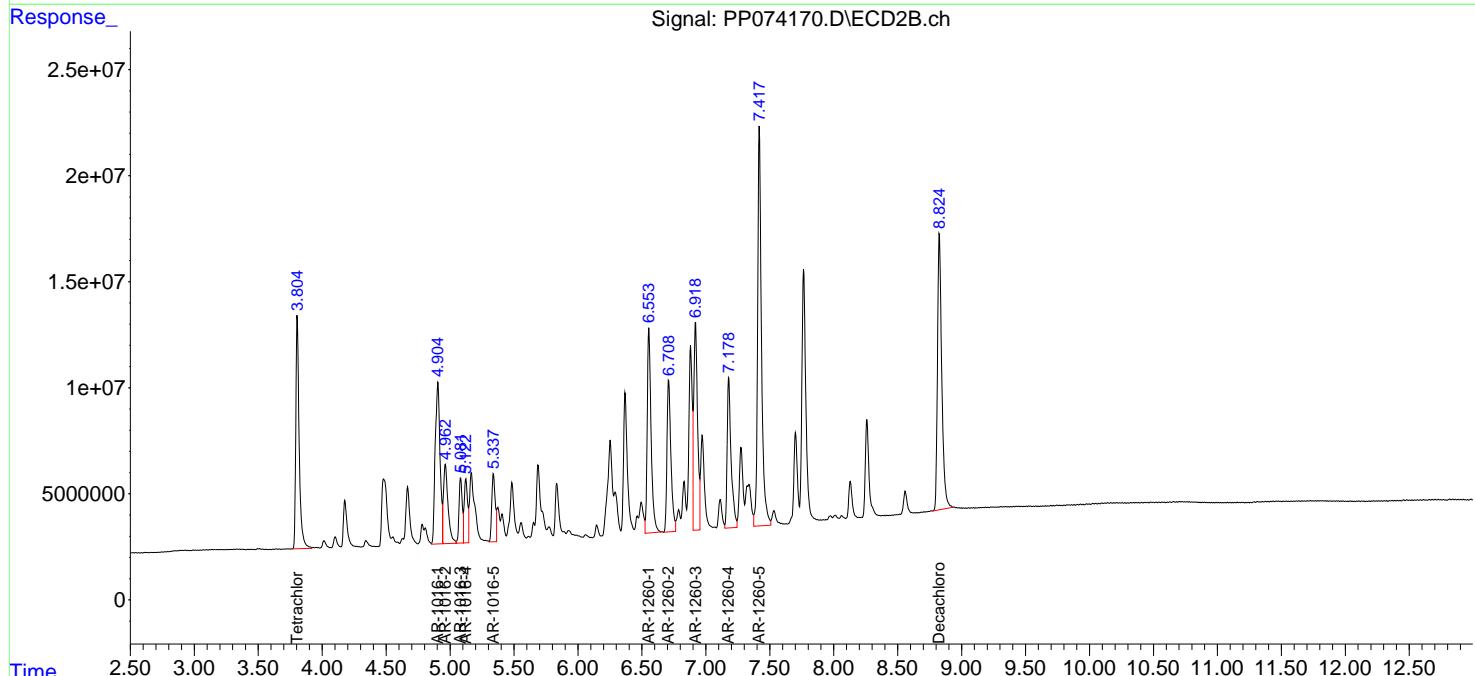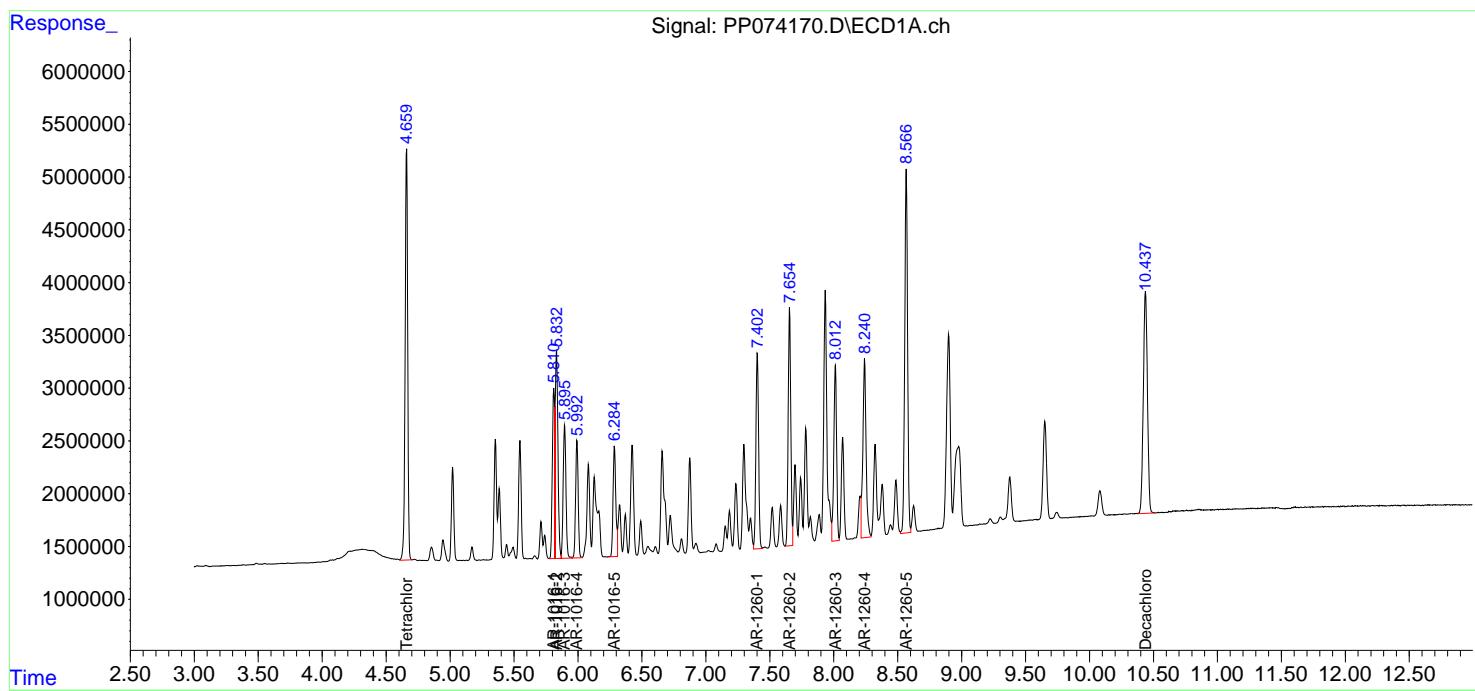

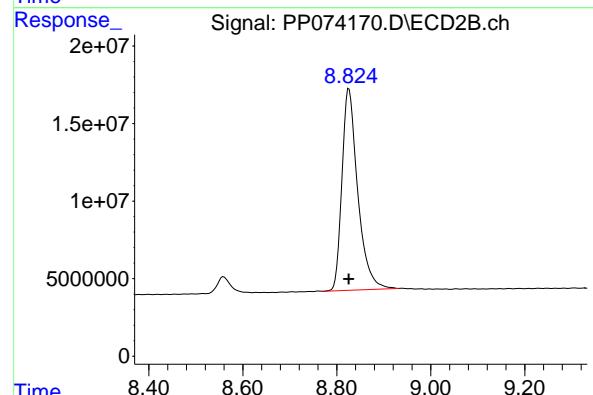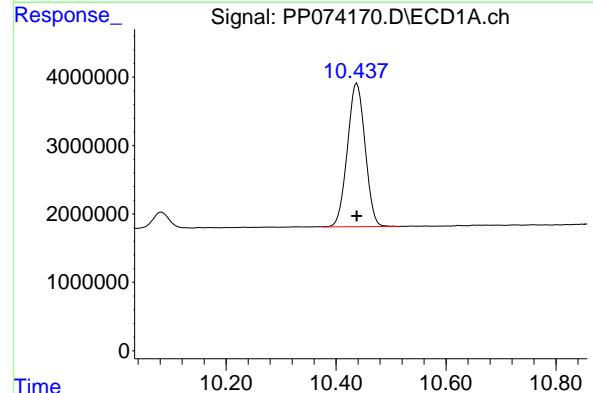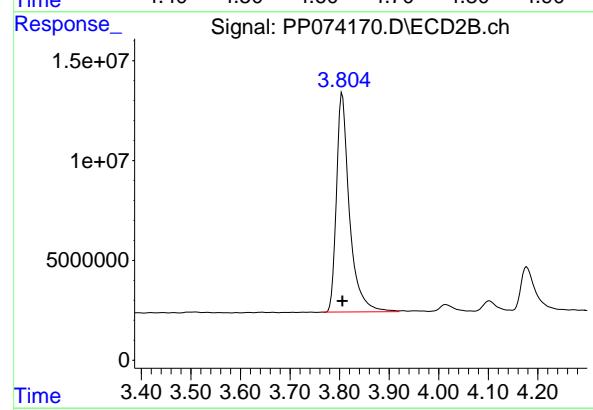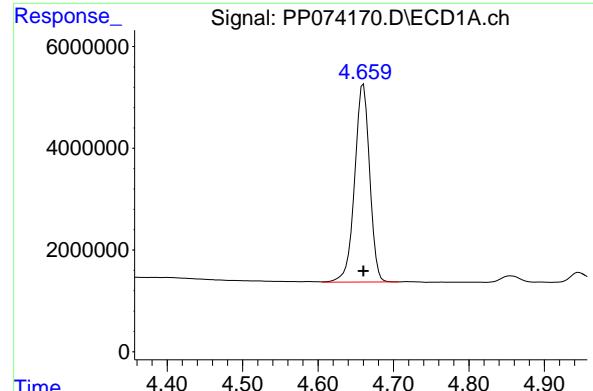

#1 Tetrachloro-m-xylene

R.T.: 4.660 min
 Delta R.T.: 0.000 min
 Response: 53802576
 Conc: 50.00 ng/ml

Instrument: ECD_P
 ClientSampleId : AR1660ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.805 min
 Delta R.T.: 0.000 min
 Response: 199858395
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.438 min
 Delta R.T.: 0.000 min
 Response: 47022042
 Conc: 50.00 ng/ml


#2 Decachlorobiphenyl

R.T.: 8.826 min
 Delta R.T.: 0.000 min
 Response: 303238754
 Conc: 50.00 ng/ml

#3 AR-1016-1


R.T.: 5.812 min
 Delta R.T.: 0.000 min
 Response: 19556469
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

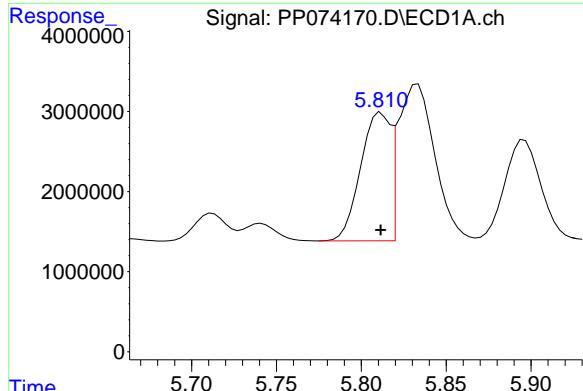


#3 AR-1016-1

R.T.: 4.906 min
 Delta R.T.: 0.000 min
 Response: 199956180
 Conc: 500.00 ng/ml

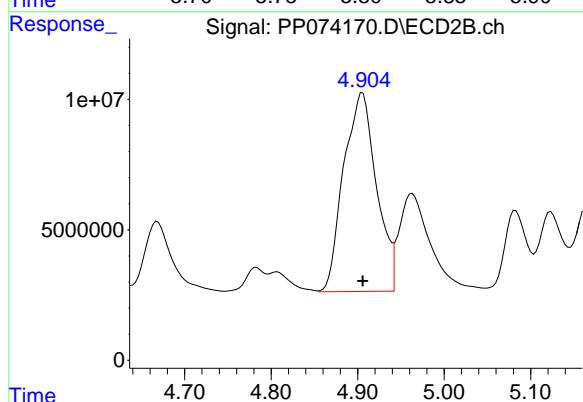


#4 AR-1016-2





R.T.: 5.833 min
 Delta R.T.: 0.000 min
 Response: 29173644
 Conc: 500.00 ng/ml

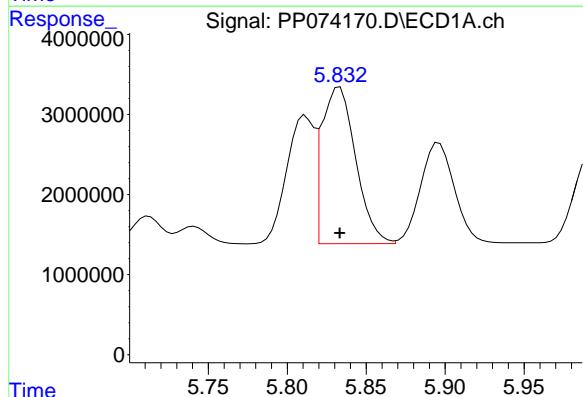

#4 AR-1016-2

R.T.: 4.963 min
 Delta R.T.: 0.000 min
 Response: 93788708
 Conc: 500.00 ng/ml

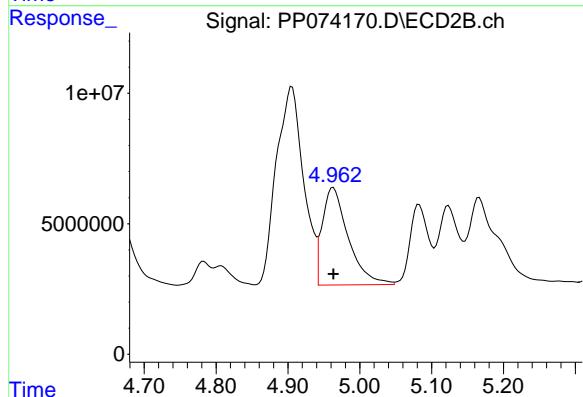

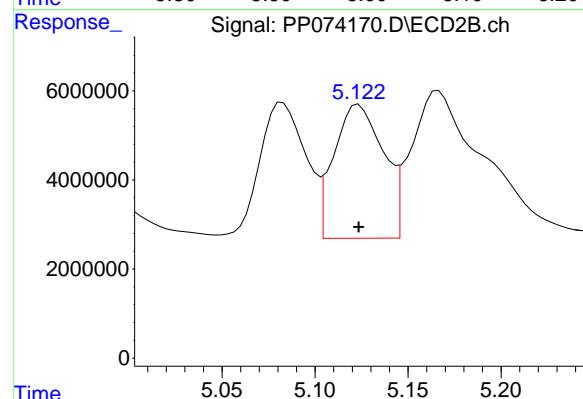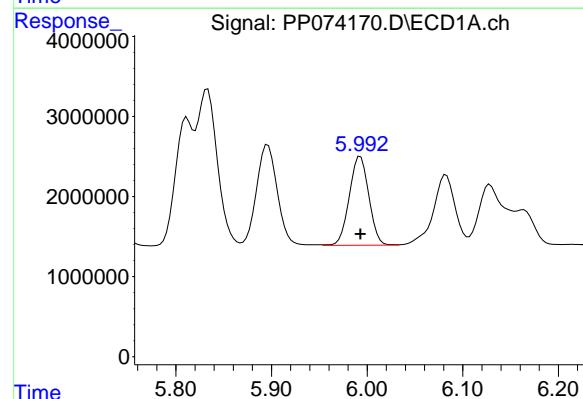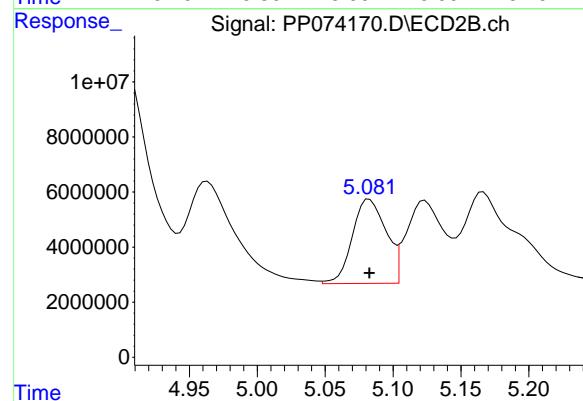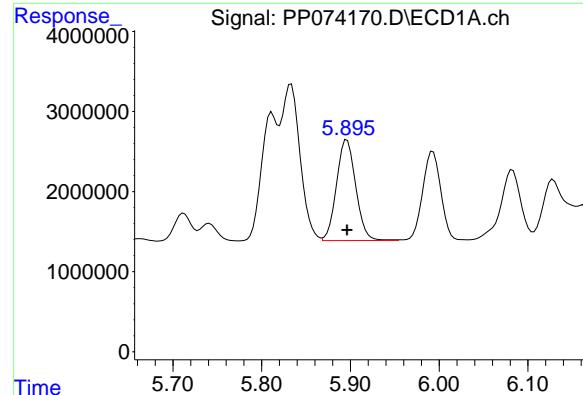

#5 AR-1016-3

R.T.: 5.896 min
Delta R.T.: 0.000 min
Response: 18934969
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

#5 AR-1016-3

R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 53031224
Conc: 500.00 ng/ml

#6 AR-1016-4

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 15743832
Conc: 500.00 ng/ml





#6 AR-1016-4

R.T.: 5.123 min
Delta R.T.: 0.000 min
Response: 55544690
Conc: 500.00 ng/ml

#7 AR-1016-5

R.T.: 6.286 min
 Delta R.T.: 0.000 min
 Response: 15720965
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

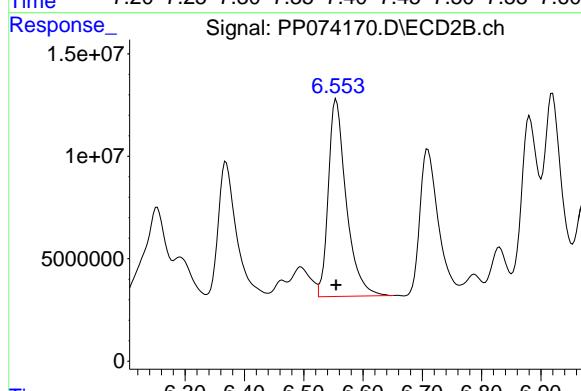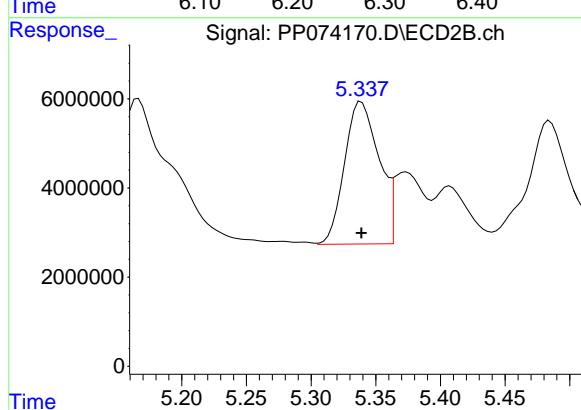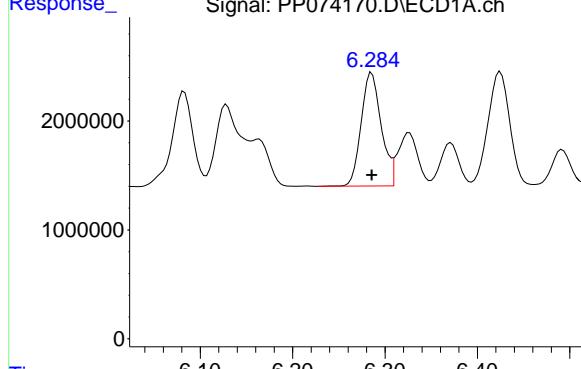

#7 AR-1016-5

R.T.: 5.339 min
 Delta R.T.: 0.000 min
 Response: 59321598
 Conc: 500.00 ng/ml

#31 AR-1260-1

R.T.: 7.403 min
 Delta R.T.: 0.000 min
 Response: 27071230
 Conc: 500.00 ng/ml





#31 AR-1260-1

R.T.: 6.555 min
 Delta R.T.: 0.000 min
 Response: 202862910
 Conc: 500.00 ng/ml

#32 AR-1260-2

R.T.: 7.655 min
 Delta R.T.: 0.000 min
 Response: 31956798
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

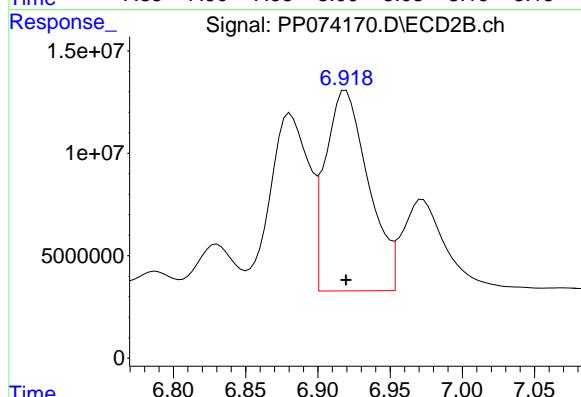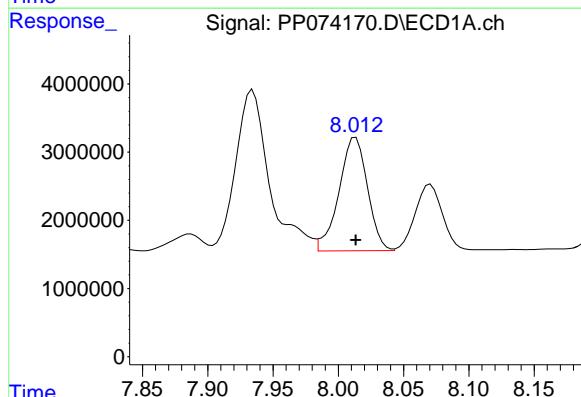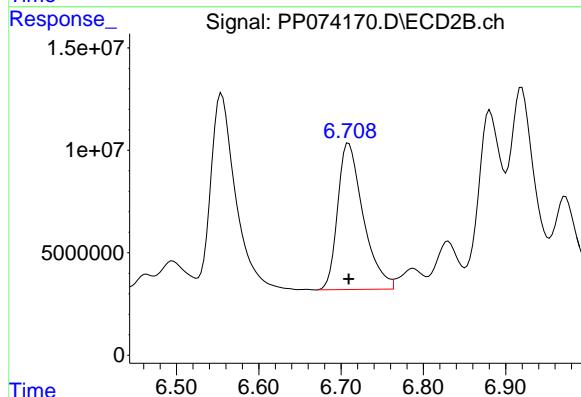

#32 AR-1260-2

R.T.: 6.709 min
 Delta R.T.: 0.000 min
 Response: 154133075
 Conc: 500.00 ng/ml

#33 AR-1260-3

R.T.: 8.013 min
 Delta R.T.: 0.000 min
 Response: 25325364
 Conc: 500.00 ng/ml


#33 AR-1260-3

R.T.: 6.919 min
 Delta R.T.: 0.000 min
 Response: 202034308
 Conc: 500.00 ng/ml

#34 AR-1260-4


R.T.: 8.242 min
 Delta R.T.: 0.000 min
 Response: 30132251
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC500

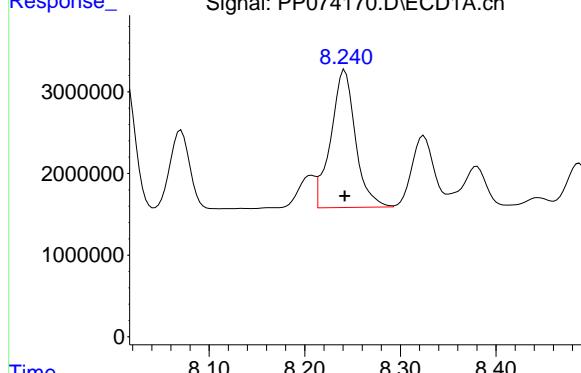


#34 AR-1260-4

R.T.: 7.179 min
 Delta R.T.: 0.000 min
 Response: 153068301
 Conc: 500.00 ng/ml

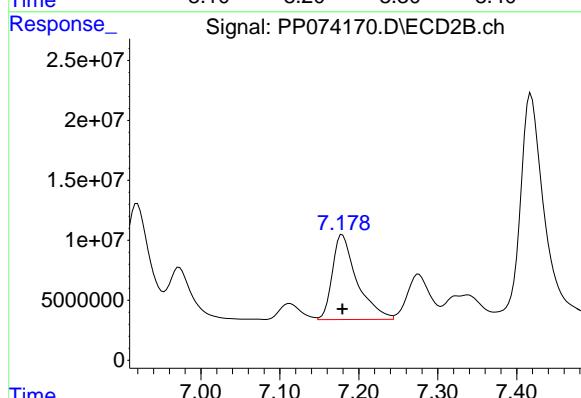


#35 AR-1260-5

R.T.: 8.568 min
 Delta R.T.: 0.000 min
 Response: 53869434
 Conc: 500.00 ng/ml

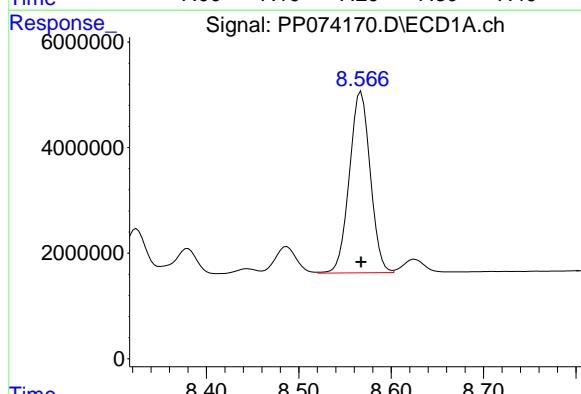

#35 AR-1260-5

R.T.: 7.418 min
 Delta R.T.: 0.000 min
 Response: 397056043
 Conc: 500.00 ng/ml

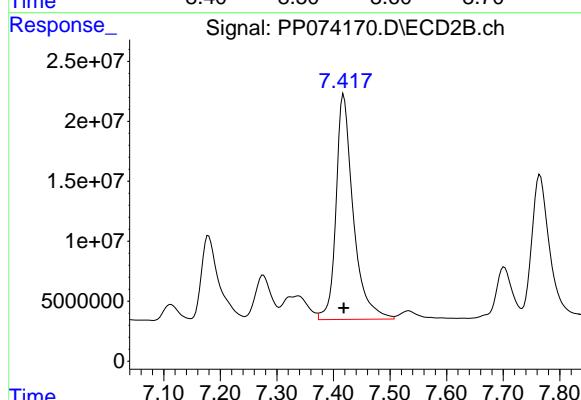

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:54
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:10:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.807 | 28863110 | 91466480 | 27.077 | 22.767 |
| 2) SA Decachlor... | 10.435 | 8.827 | 25421801 | 149.8E6 | 27.450 | 24.664 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|---------|
| 3) L1 AR-1016-1 | 5.810 | 4.907 | 10964759 | 100.9E6 | 281.744 | 251.671 |
| 4) L1 AR-1016-2 | 5.832 | 4.965 | 16172490 | 49571013 | 281.221 | 259.123 |
| 5) L1 AR-1016-3 | 5.895 | 5.085 | 10675549 | 28731399 | 285.290 | 266.268 |
| 6) L1 AR-1016-4 | 5.991 | 5.126 | 8965609 | 27406022 | 287.521 | 254.800 |
| 7) L1 AR-1016-5 | 6.282 | 5.340 | 8901636 | 29720771 | 287.291m | 252.036 |
| 31) L7 AR-1260-1 | 7.399 | 6.557 | 14779955 | 109.5E6 | 277.879m | 267.207 |
| 32) L7 AR-1260-2 | 7.652 | 6.711 | 17850337 | 76433717 | 284.356m | 249.893 |
| 33) L7 AR-1260-3 | 8.011 | 6.922 | 14251387 | 95830018 | 283.827 | 237.590 |
| 34) L7 AR-1260-4 | 8.240 | 7.182 | 16666094 | 70195428 | 280.066 | 237.501 |
| 35) L7 AR-1260-5 | 8.565 | 7.421 | 29333116 | 183.1E6 | 275.424 | 232.969 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:54
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:10:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

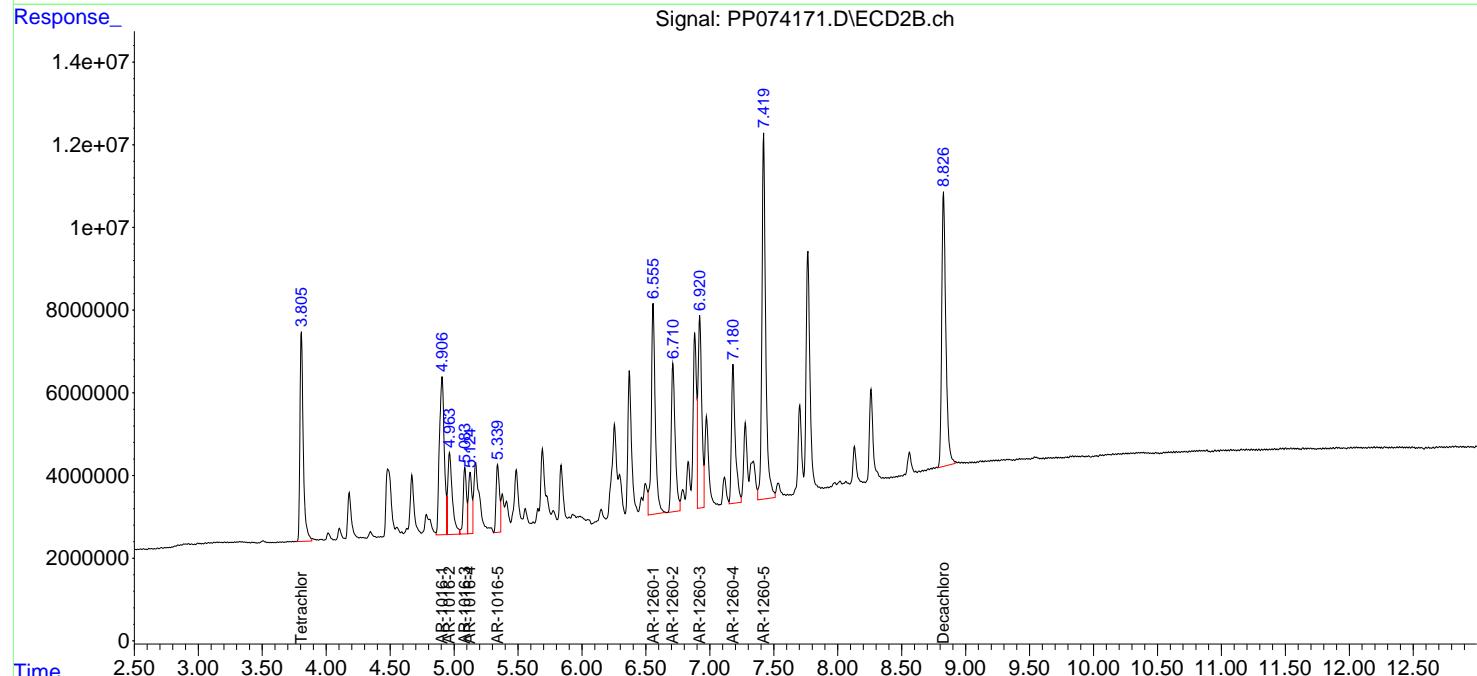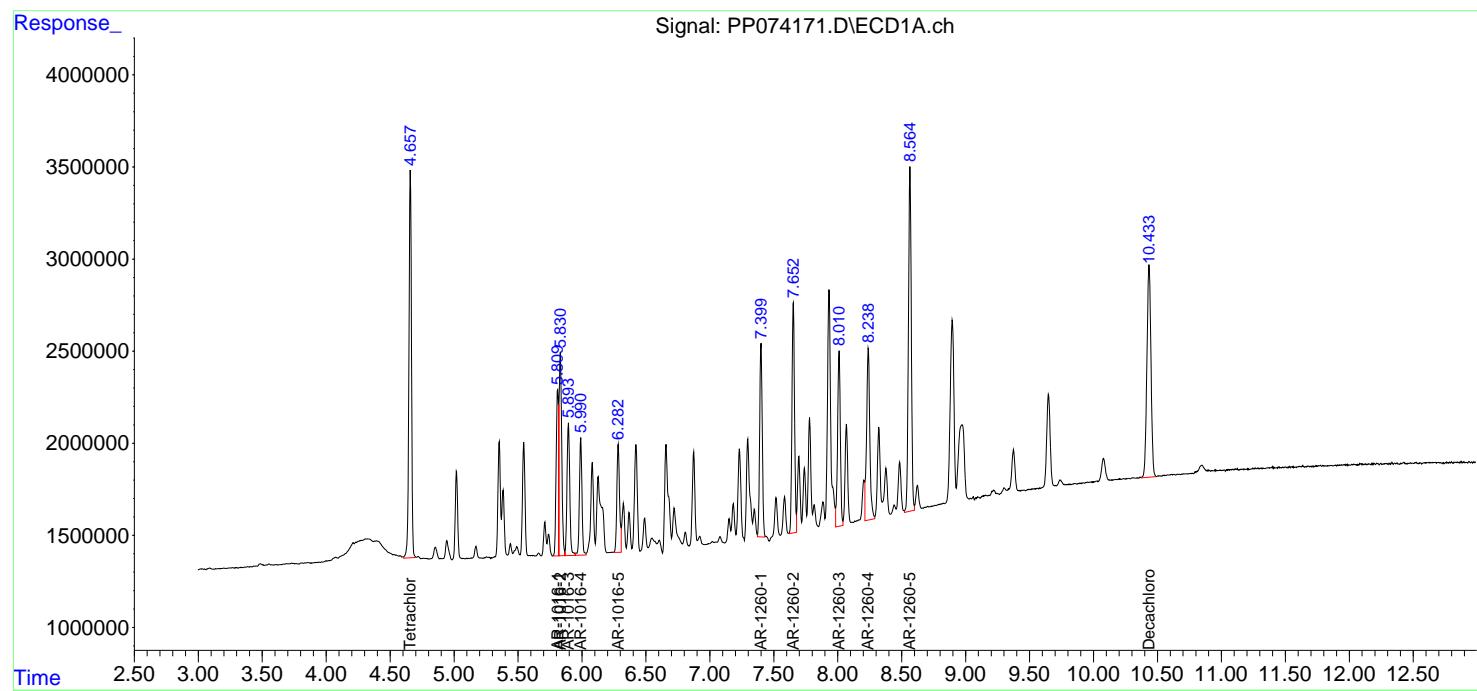

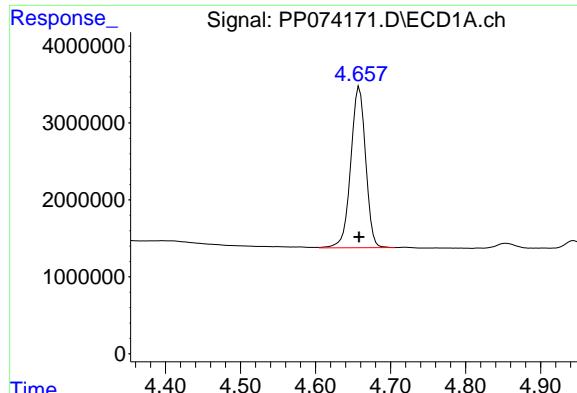


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: 0.000 min
Response: 28863110
Conc: 27.08 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

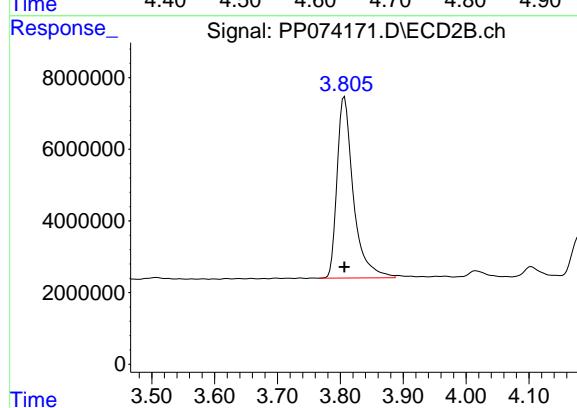


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 91466480
Conc: 22.77 ng/ml

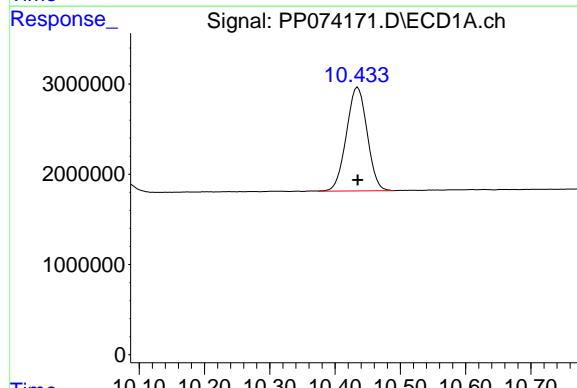

#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.000 min
Response: 25421801
Conc: 27.45 ng/ml

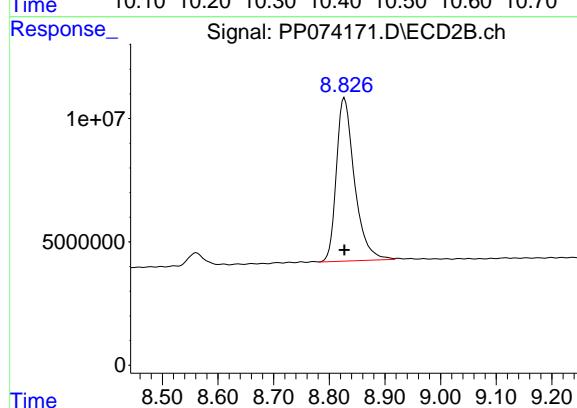

#2 Decachlorobiphenyl

R.T.: 8.827 min
Delta R.T.: 0.000 min
Response: 149786727
Conc: 24.66 ng/ml





#3 AR-1016-1

R.T.: 5.810 min
 Delta R.T.: 0.000 min
 Response: 10964759
 Conc: 281.74 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

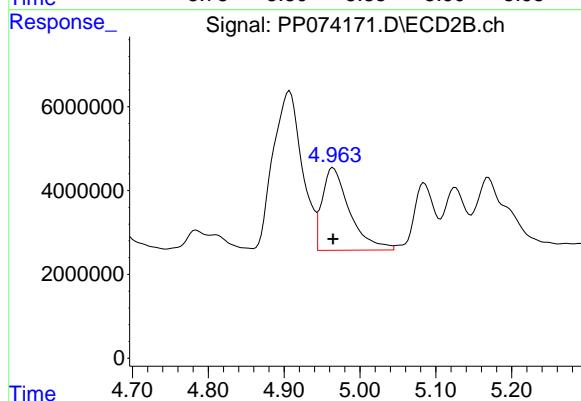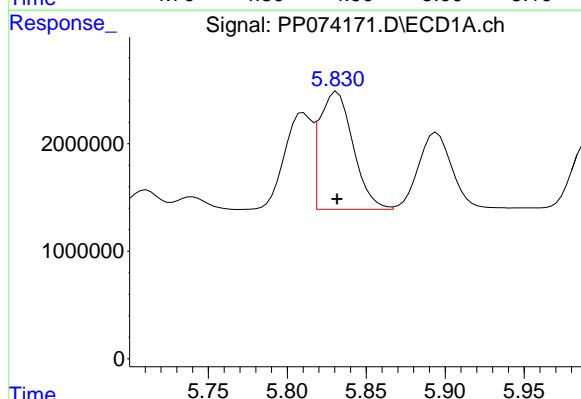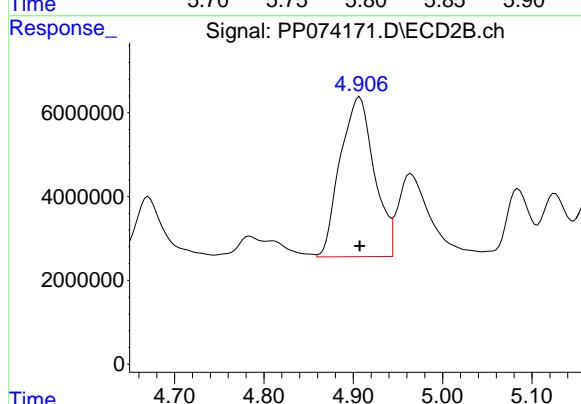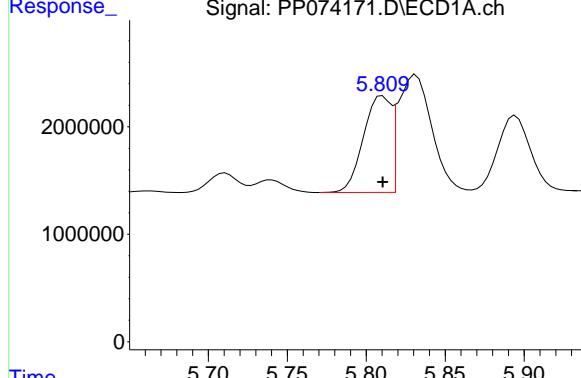

#3 AR-1016-1

R.T.: 4.907 min
 Delta R.T.: 0.000 min
 Response: 100933839
 Conc: 251.67 ng/ml

#4 AR-1016-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 16172490
 Conc: 281.22 ng/ml

#4 AR-1016-2

R.T.: 4.965 min
 Delta R.T.: 0.000 min
 Response: 49571013
 Conc: 259.12 ng/ml





#5 AR-1016-3

R.T.: 5.895 min
 Delta R.T.: 0.000 min
 Response: 10675549
 Conc: 285.29 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

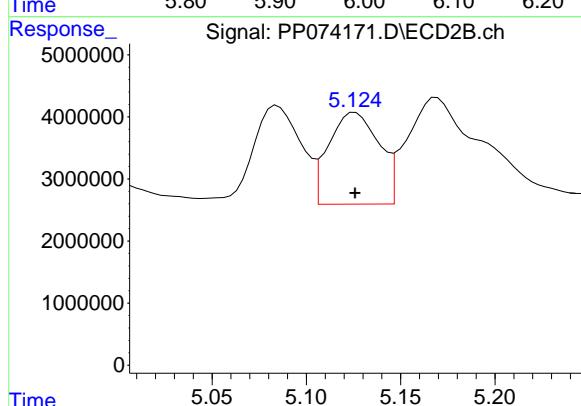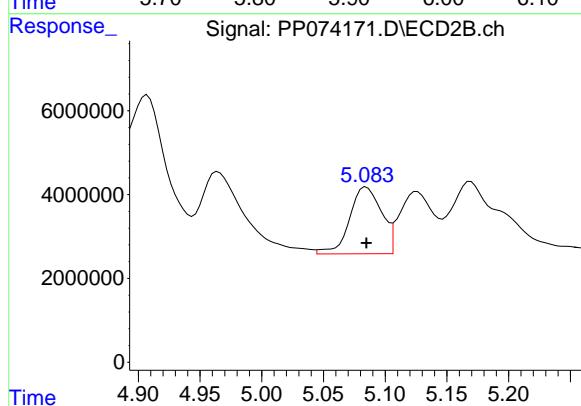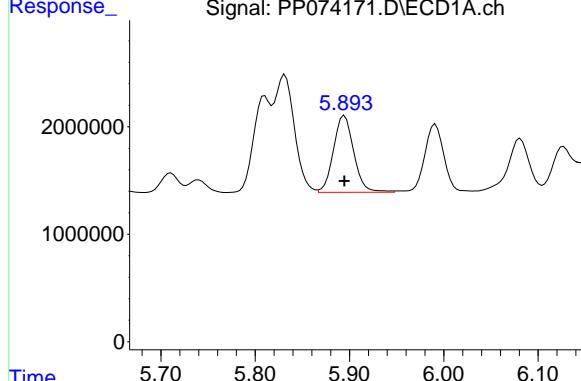

#5 AR-1016-3


R.T.: 5.085 min
 Delta R.T.: 0.000 min
 Response: 28731399
 Conc: 266.27 ng/ml

#6 AR-1016-4

R.T.: 5.991 min
 Delta R.T.: 0.000 min
 Response: 8965609
 Conc: 287.52 ng/ml

#6 AR-1016-4

R.T.: 5.126 min
 Delta R.T.: 0.000 min
 Response: 27406022
 Conc: 254.80 ng/ml

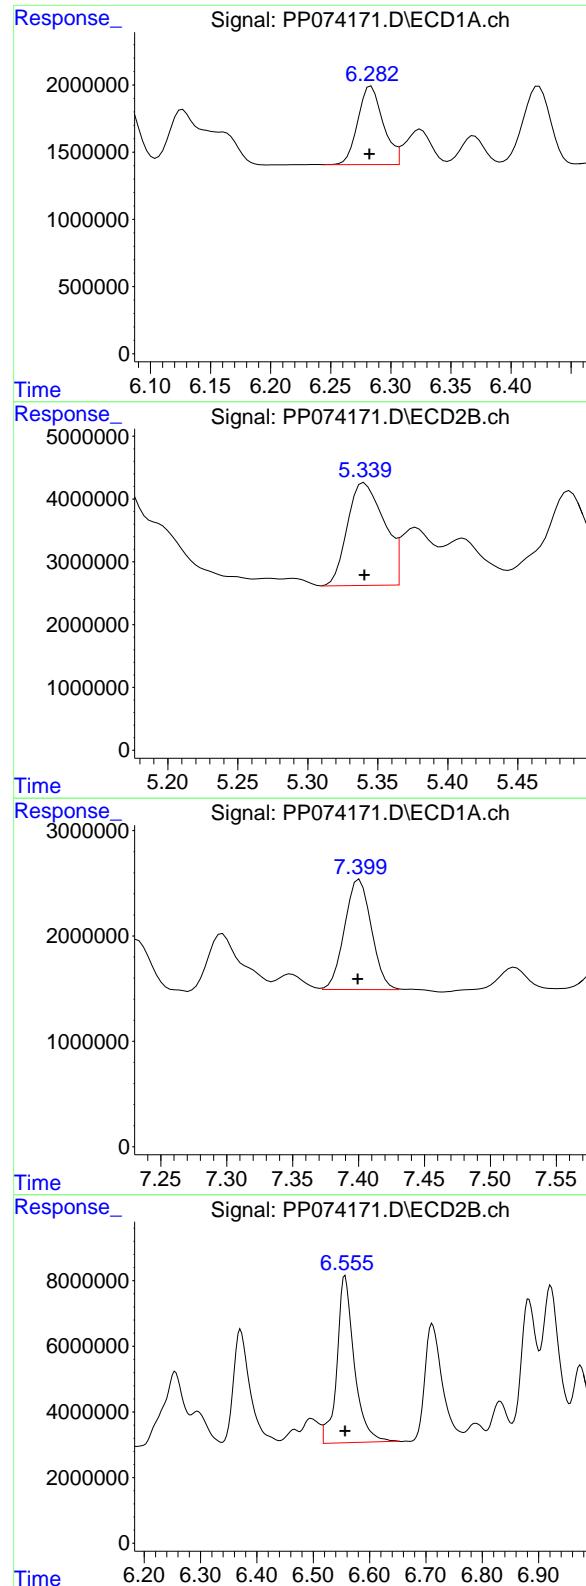

#7 AR-1016-5

R.T.: 6.282 min
 Delta R.T.: 0.000 min
 Response: 8901636
 Conc: 287.29 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#7 AR-1016-5

R.T.: 5.340 min
 Delta R.T.: 0.000 min
 Response: 29720771
 Conc: 252.04 ng/ml

#31 AR-1260-1

R.T.: 7.399 min
 Delta R.T.: 0.000 min
 Response: 14779955
 Conc: 277.88 ng/ml

#31 AR-1260-1

R.T.: 6.557 min
 Delta R.T.: 0.000 min
 Response: 109526607
 Conc: 267.21 ng/ml

#32 AR-1260-2

R.T.: 7.652 min
 Delta R.T.: 0.000 min
 Response: 17850337
 Conc: 284.36 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#32 AR-1260-2





R.T.: 6.711 min
 Delta R.T.: 0.000 min
 Response: 76433717
 Conc: 249.89 ng/ml


#33 AR-1260-3

R.T.: 8.011 min
 Delta R.T.: 0.000 min
 Response: 14251387
 Conc: 283.83 ng/ml

#33 AR-1260-3

R.T.: 6.922 min
 Delta R.T.: 0.000 min
 Response: 95830018
 Conc: 237.59 ng/ml

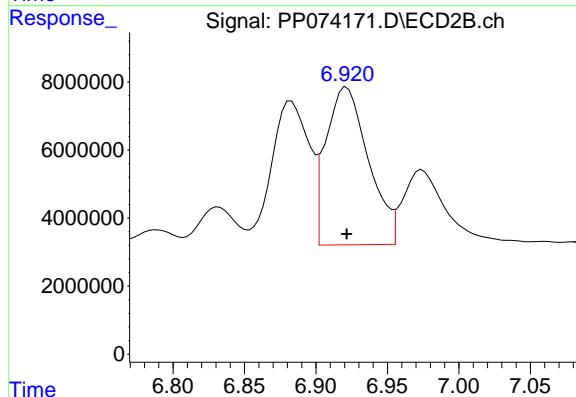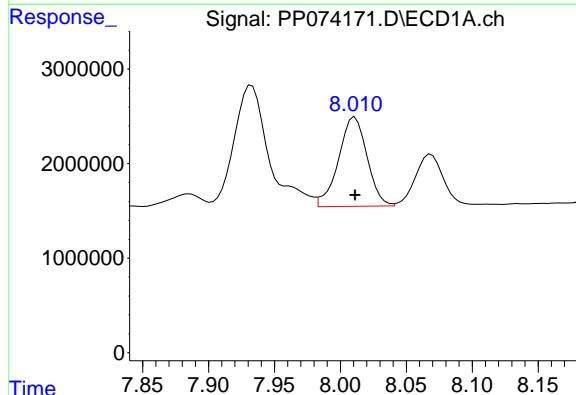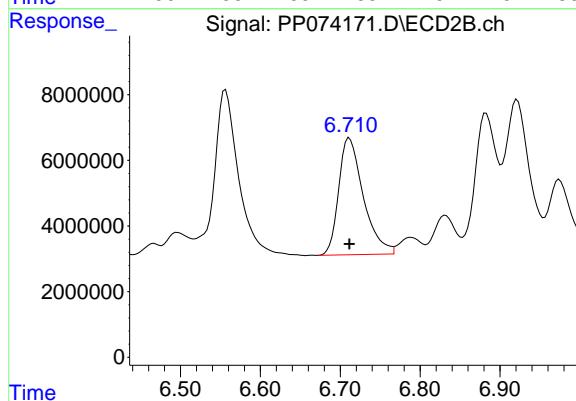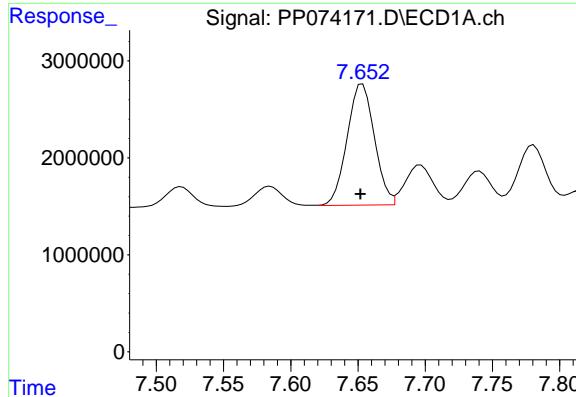

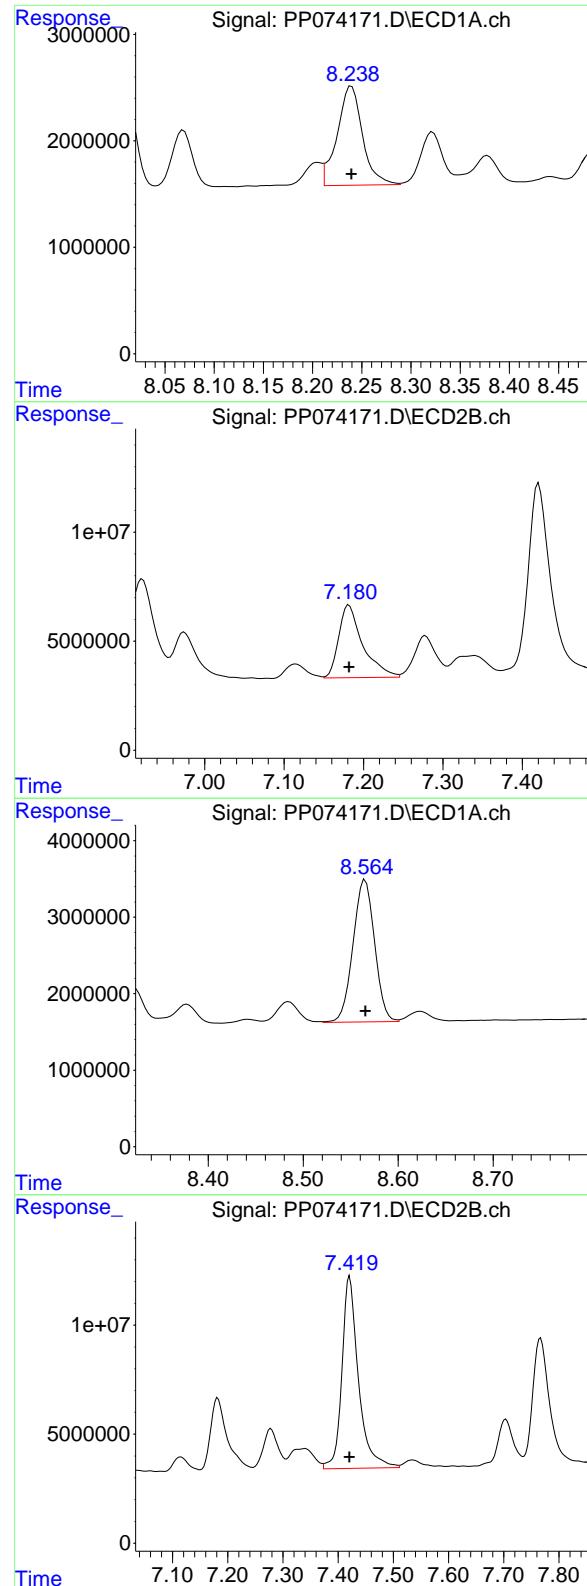

#34 AR-1260-4

R.T.: 8.240 min
 Delta R.T.: 0.000 min
 Response: 16666094
 Conc: 280.07 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#34 AR-1260-4

R.T.: 7.182 min
 Delta R.T.: 0.000 min
 Response: 70195428
 Conc: 237.50 ng/ml

#35 AR-1260-5

R.T.: 8.565 min
 Delta R.T.: 0.000 min
 Response: 29333116
 Conc: 275.42 ng/ml

#35 AR-1260-5

R.T.: 7.421 min
 Delta R.T.: 0.000 min
 Response: 183122844
 Conc: 232.97 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 13:42
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:58:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:58:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|---------|----------|--------|---------|
| 1) SA Tetrachlor... | 4.660 | 3.804 | 6638630 | 15510226 | 5.935m | 4.043m# |
| 2) SA Decachlor... | 10.437 | 8.827 | 5756903 | 28876514 | 5.928 | 4.802 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|----------|
| 3) L1 AR-1016-1 | 5.813 | 4.906 | 2530723 | 19510776 | 61.341 | 48.913 |
| 4) L1 AR-1016-2 | 5.835 | 4.966 | 3683827 | 8691681 | 60.647 | 46.279 |
| 5) L1 AR-1016-3 | 5.897 | 5.084 | 2431131 | 4936579 | 61.299 | 46.541 |
| 6) L1 AR-1016-4 | 5.994 | 5.124 | 1899628 | 5793266 | 58.370 | 53.042 |
| 7) L1 AR-1016-5 | 6.287 | 5.341 | 1907560 | 5656312 | 58.752 | 48.360 |
| 31) L7 AR-1260-1 | 7.404 | 6.556 | 3495993 | 19010301 | 62.034 | 47.060 |
| 32) L7 AR-1260-2 | 7.656 | 6.709 | 4438588 | 17001537 | 64.615m | 54.991m |
| 33) L7 AR-1260-3 | 8.015 | 6.920 | 3281661 | 17861059 | 61.574 | 45.319 # |
| 34) L7 AR-1260-4 | 8.242 | 7.180 | 3752198 | 13633196 | 59.829m | 46.853 |
| 35) L7 AR-1260-5 | 8.568 | 7.418 | 7025863 | 32144633 | 62.008 | 42.440 # |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 13:42
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 50 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:58:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:58:39 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

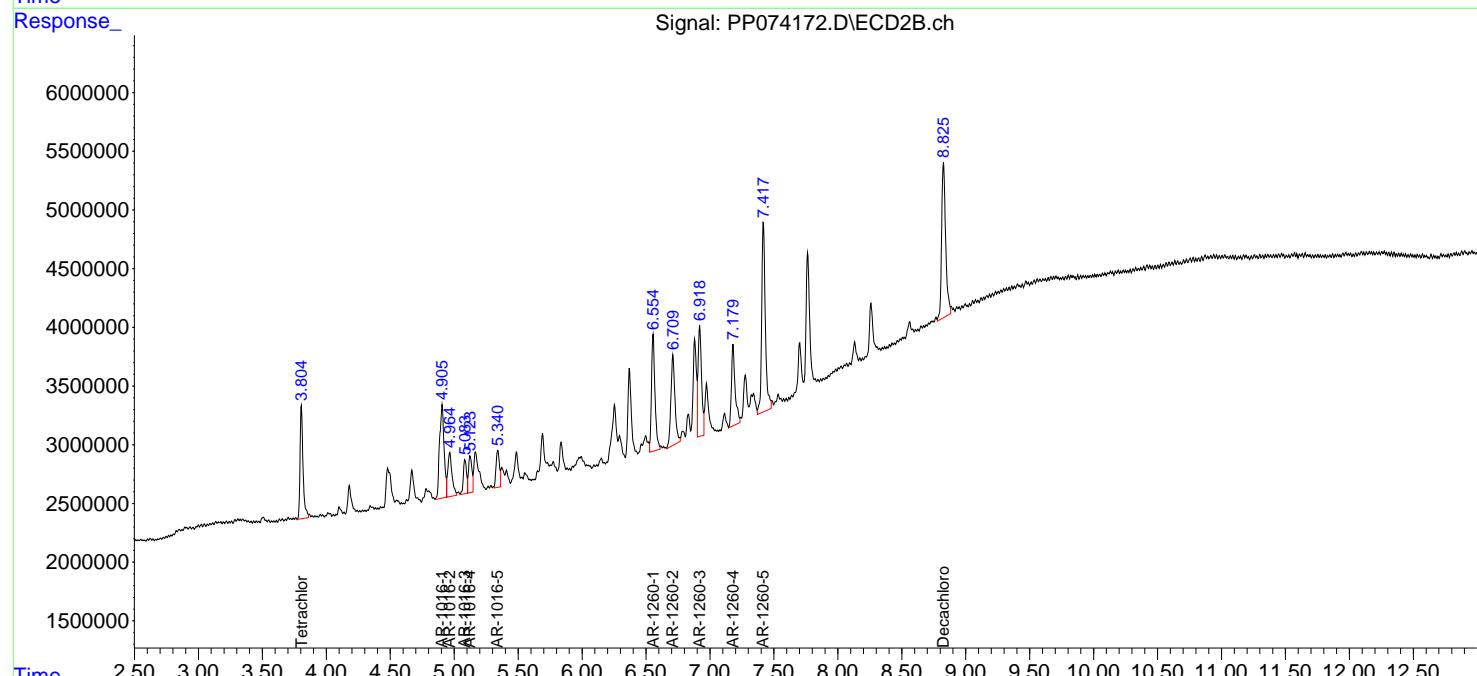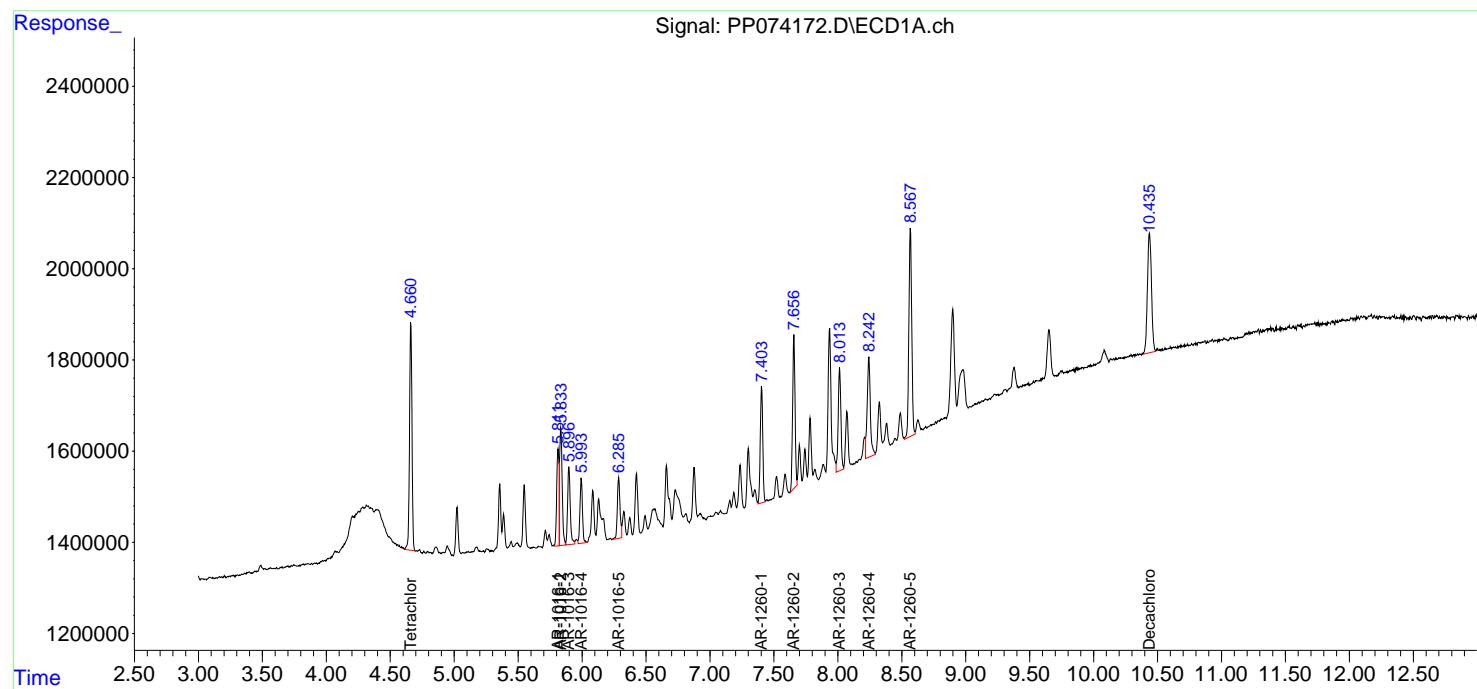

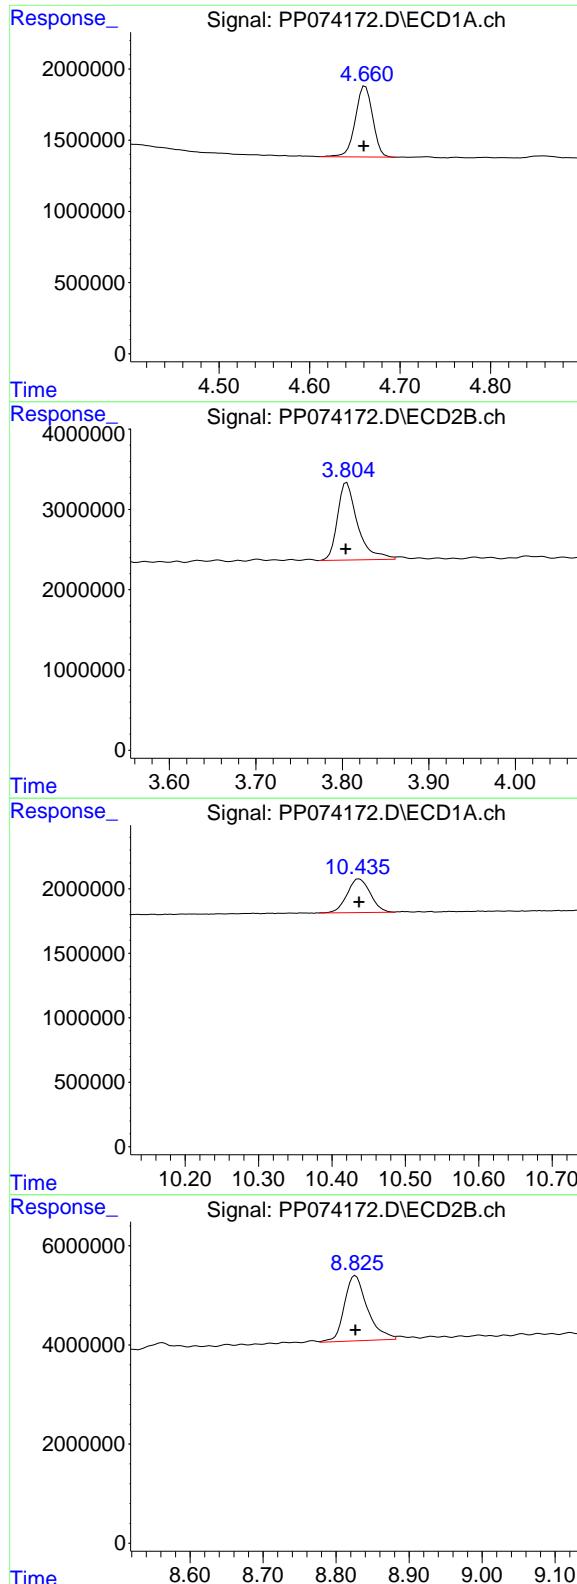

#1 Tetrachloro-m-xylene

R.T.: 4.660 min
 Delta R.T.: 0.000 min
 Response: 6638630
 Conc: 5.93 ng/ml

Instrument: ECD_P
 ClientSampleId : AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#1 Tetrachloro-m-xylene


R.T.: 3.804 min
 Delta R.T.: 0.000 min
 Response: 15510226
 Conc: 4.04 ng/ml m

#2 Decachlorobiphenyl

R.T.: 10.437 min
 Delta R.T.: 0.000 min
 Response: 5756903
 Conc: 5.93 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.827 min
 Delta R.T.: 0.000 min
 Response: 28876514
 Conc: 4.80 ng/ml

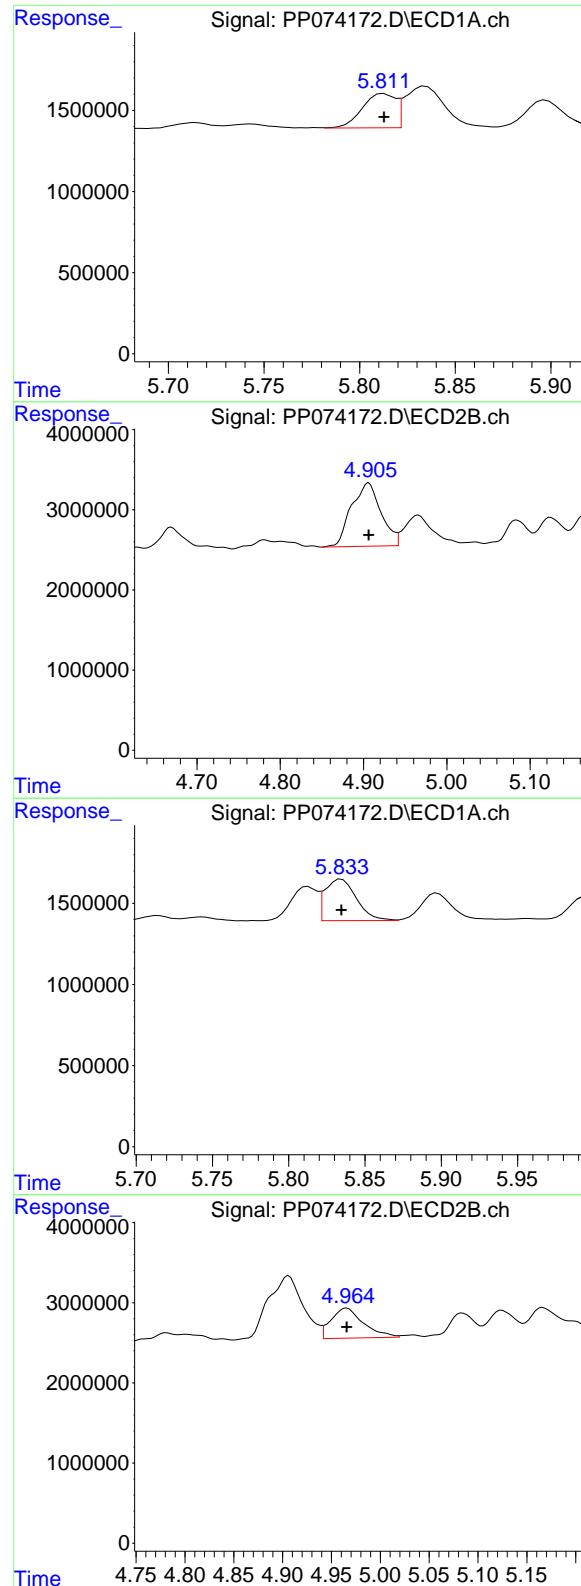

#3 AR-1016-1

R.T.: 5.813 min
 Delta R.T.: 0.000 min
 Response: 2530723
 Conc: 61.34 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#3 AR-1016-1

R.T.: 4.906 min
 Delta R.T.: 0.000 min
 Response: 19510776
 Conc: 48.91 ng/ml

#4 AR-1016-2

R.T.: 5.835 min
 Delta R.T.: 0.000 min
 Response: 3683827
 Conc: 60.65 ng/ml

#4 AR-1016-2

R.T.: 4.966 min
 Delta R.T.: 0.000 min
 Response: 8691681
 Conc: 46.28 ng/ml





#5 AR-1016-3

R.T.: 5.897 min
 Delta R.T.: 0.000 min
 Response: 2431131
 Conc: 61.30 ng/ml

Instrument: ECD_P
ClientSampleId : AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

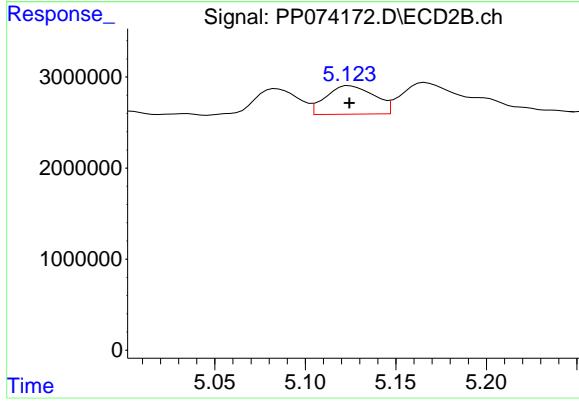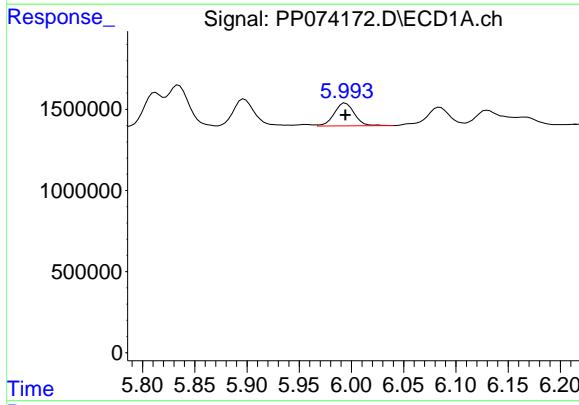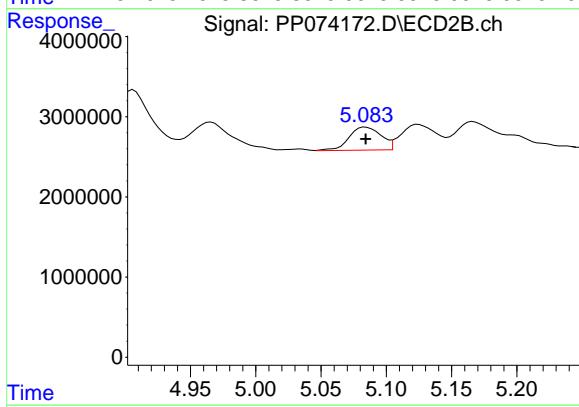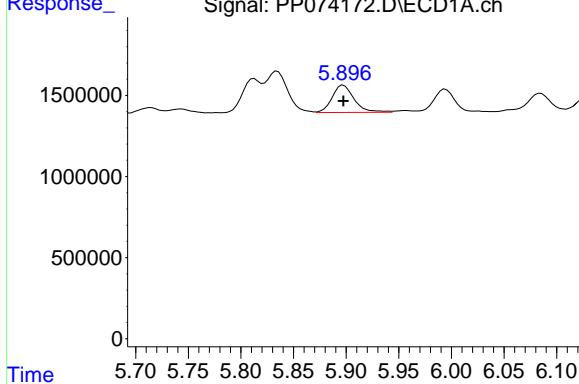

#5 AR-1016-3


R.T.: 5.084 min
 Delta R.T.: 0.000 min
 Response: 4936579
 Conc: 46.54 ng/ml

#6 AR-1016-4

R.T.: 5.994 min
 Delta R.T.: 0.000 min
 Response: 1899628
 Conc: 58.37 ng/ml

#6 AR-1016-4

R.T.: 5.124 min
 Delta R.T.: 0.000 min
 Response: 5793266
 Conc: 53.04 ng/ml

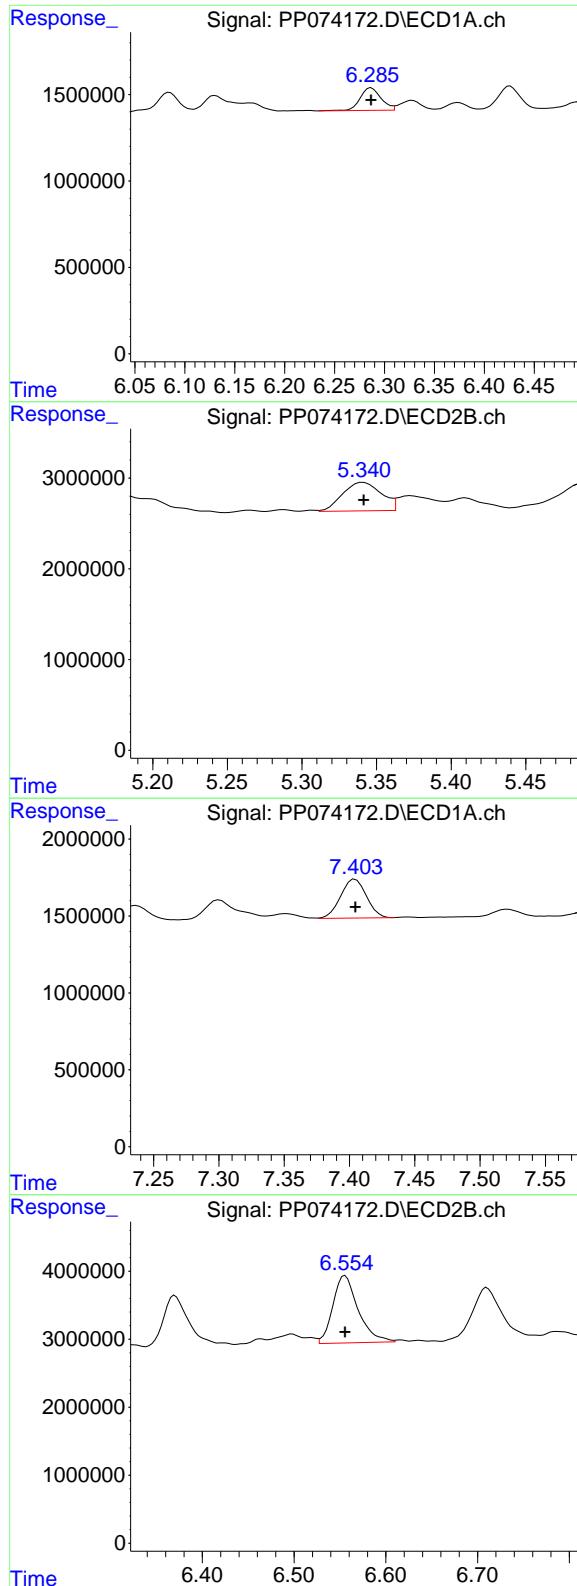

#7 AR-1016-5

R.T.: 6.287 min
 Delta R.T.: 0.000 min
 Response: 1907560
 Conc: 58.75 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#7 AR-1016-5

R.T.: 5.341 min
 Delta R.T.: 0.000 min
 Response: 5656312
 Conc: 48.36 ng/ml

#31 AR-1260-1

R.T.: 7.404 min
 Delta R.T.: 0.000 min
 Response: 3495993
 Conc: 62.03 ng/ml

#31 AR-1260-1

R.T.: 6.556 min
 Delta R.T.: 0.000 min
 Response: 19010301
 Conc: 47.06 ng/ml

#32 AR-1260-2

R.T.: 7.656 min
 Delta R.T.: 0.000 min
 Response: 4438588
 Conc: 64.62 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#32 AR-1260-2





R.T.: 6.709 min
 Delta R.T.: -0.001 min
 Response: 17001537
 Conc: 54.99 ng/ml

#33 AR-1260-3

R.T.: 8.015 min
 Delta R.T.: 0.000 min
 Response: 3281661
 Conc: 61.57 ng/ml

#33 AR-1260-3

R.T.: 6.920 min
 Delta R.T.: 0.000 min
 Response: 17861059
 Conc: 45.32 ng/ml

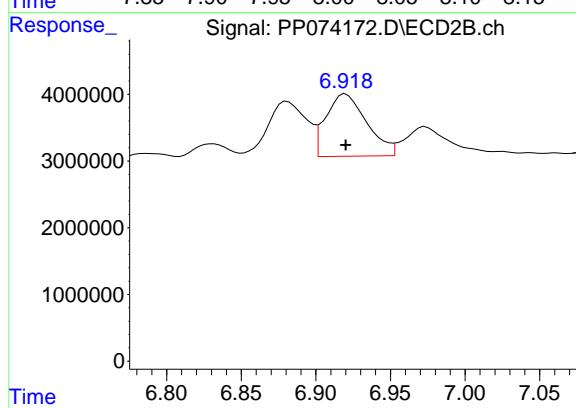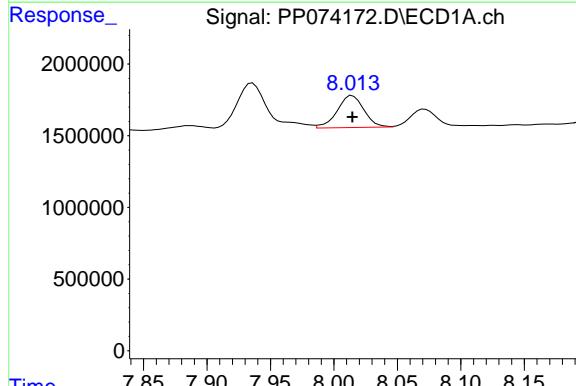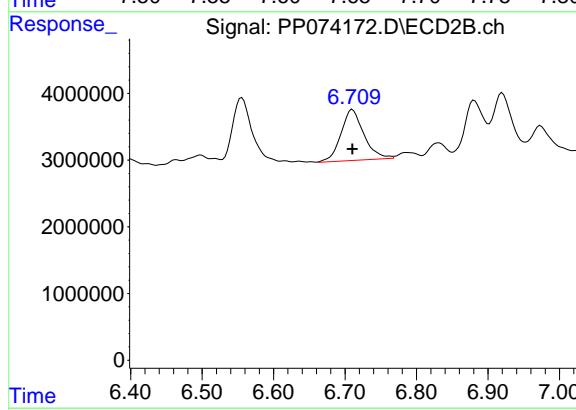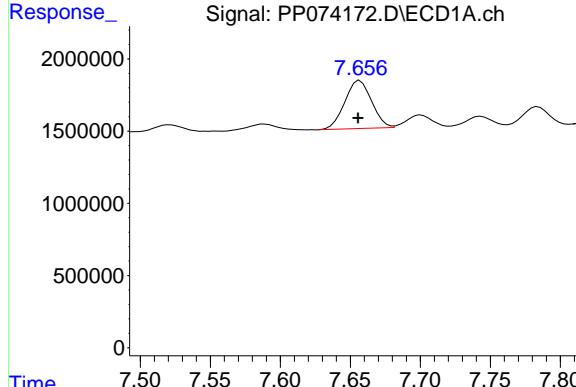





#34 AR-1260-4

R.T.: 8.242 min
 Delta R.T.: 0.000 min
 Response: 3752198
 Conc: 59.83 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

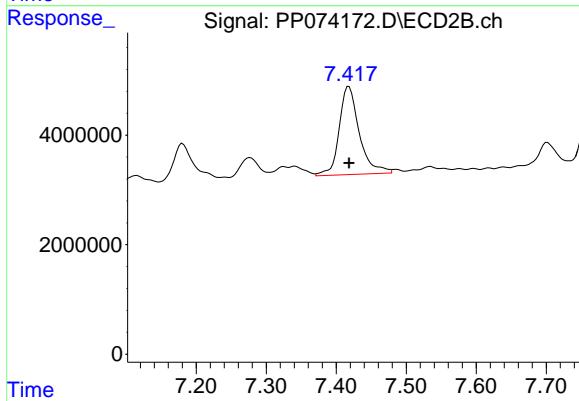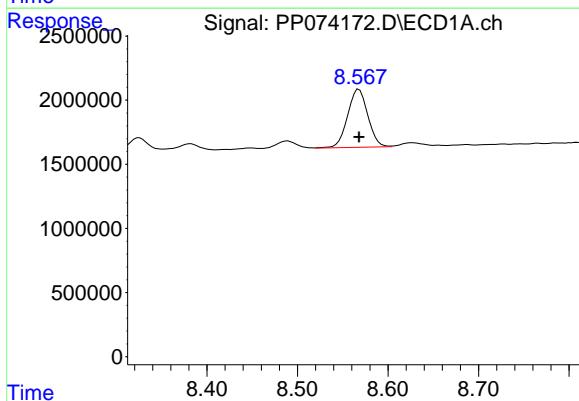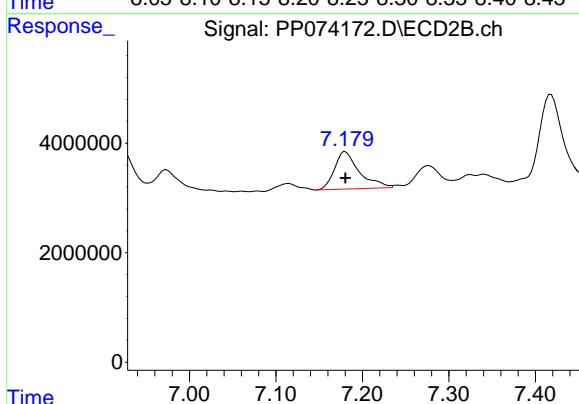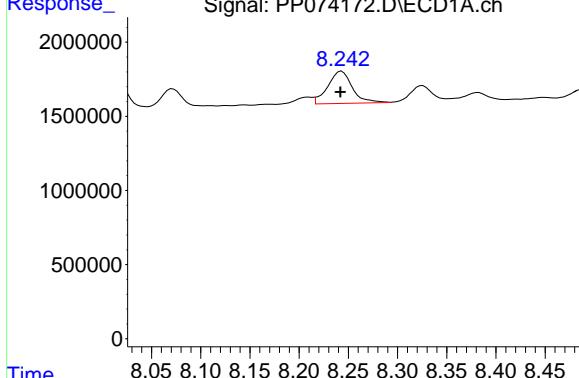

#34 AR-1260-4

R.T.: 7.180 min
 Delta R.T.: 0.000 min
 Response: 13633196
 Conc: 46.85 ng/ml

#35 AR-1260-5

R.T.: 8.568 min
 Delta R.T.: 0.000 min
 Response: 7025863
 Conc: 62.01 ng/ml

#35 AR-1260-5

R.T.: 7.418 min
 Delta R.T.: 0.000 min
 Response: 32144633
 Conc: 42.44 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 13:58
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:14:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:13:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 54821028 | 195.8E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.435 | 8.825 | 46278402 | 298.9E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 8) L2 AR-1221-1 | 4.858 | 4.015 | 8381808 | 24542587 | 500.000 | 500.000 |
| 9) L2 AR-1221-2 | 4.944 | 4.100 | 6300527 | 17944660 | 500.000 | 500.000 |
| 10) L2 AR-1221-3 | 5.019 | 4.176 | 18317605 | 67612277 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074173.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 13:58
 Operator : YP\AJ
 Sample : AR1221ICC500
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1221ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:14:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:13:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

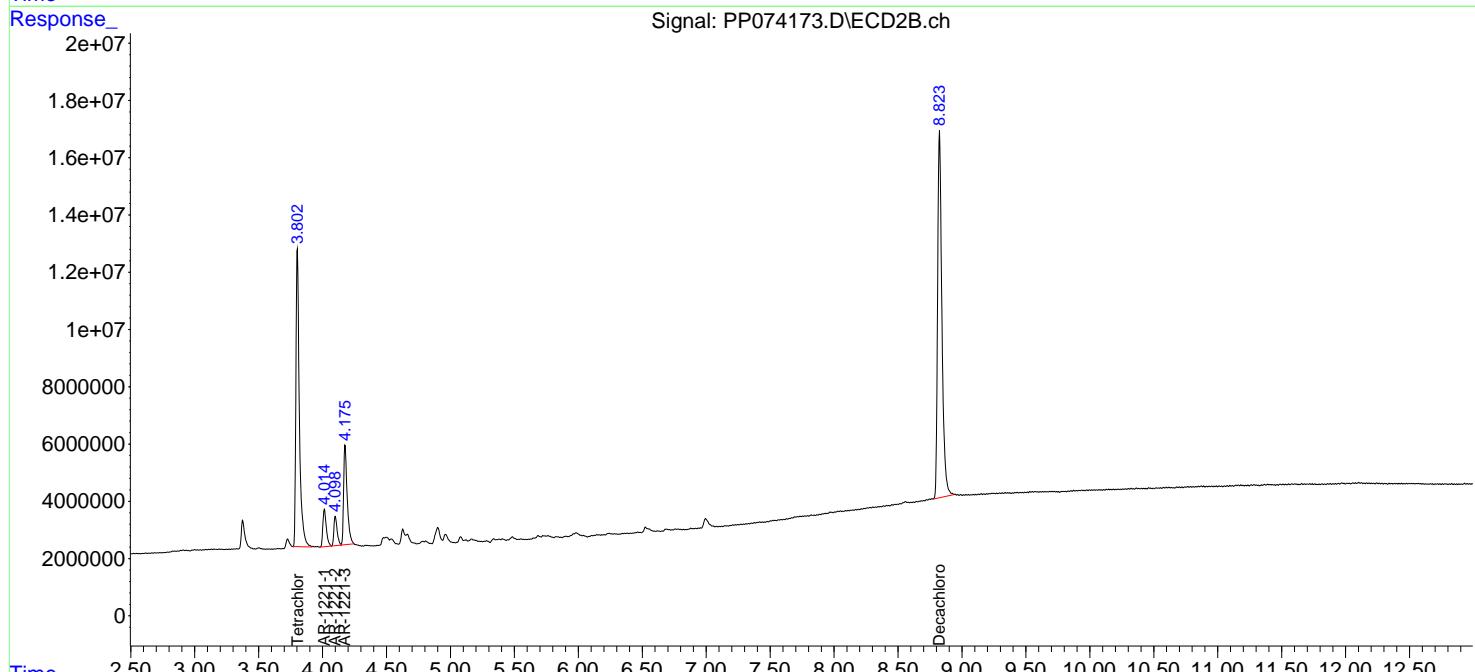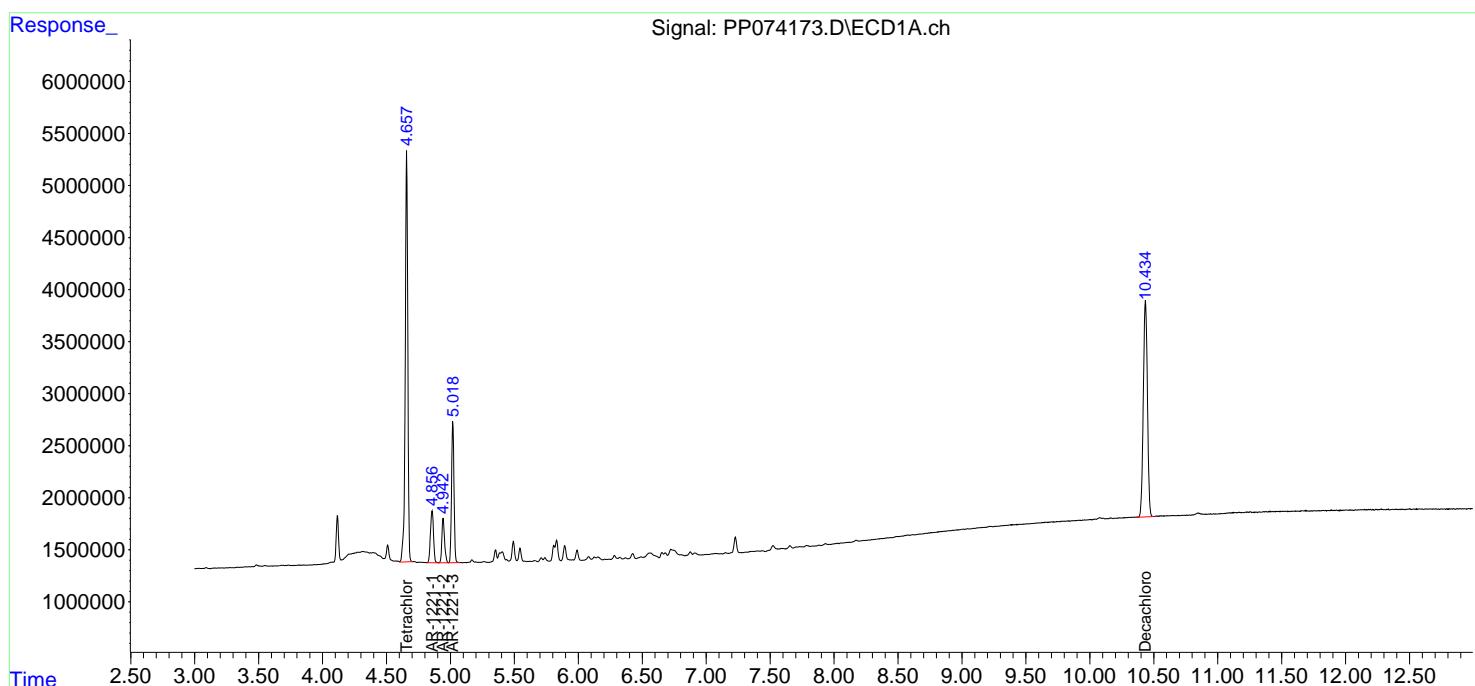

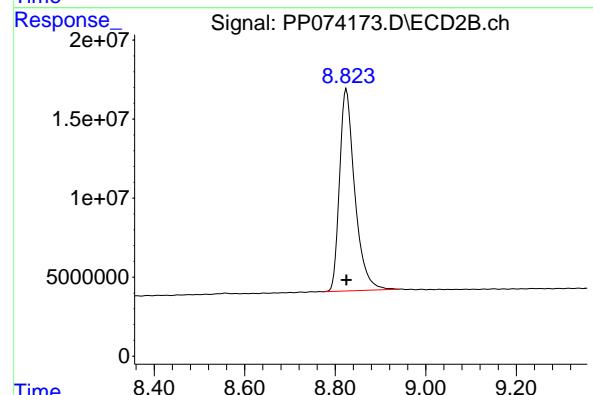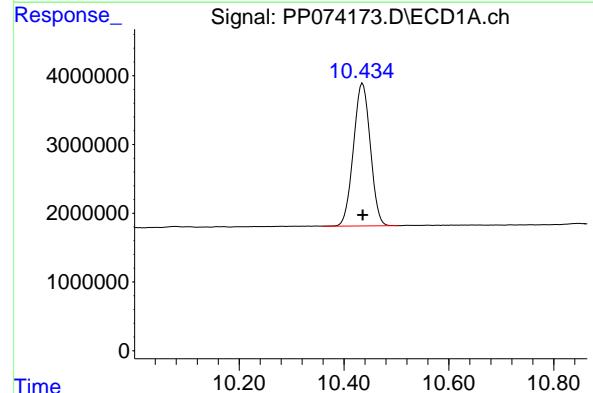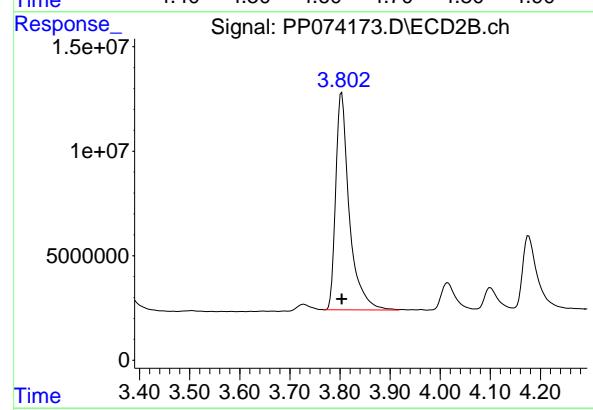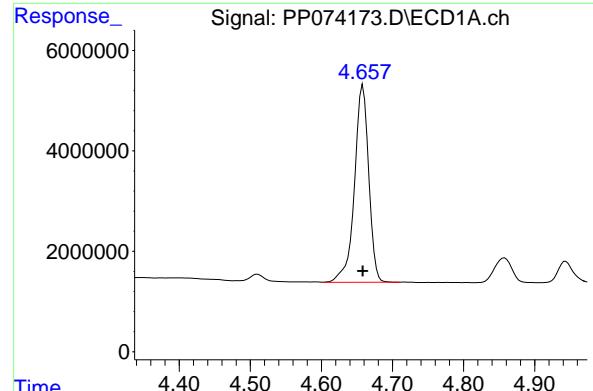

#1 Tetrachloro-m-xylene

R.T.: 4.658 min
 Delta R.T.: 0.000 min
 Response: 54821028
 Conc: 50.00 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1221ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.803 min
 Delta R.T.: 0.000 min
 Response: 195798506
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl


R.T.: 10.435 min
 Delta R.T.: 0.000 min
 Response: 46278402
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.825 min
 Delta R.T.: 0.000 min
 Response: 298854739
 Conc: 50.00 ng/ml


#8 AR-1221-1

R.T.: 4.858 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 8381808 ECD_P
 Conc: 500.00 ng/ml **ClientSampleId :**
 AR1221ICC500

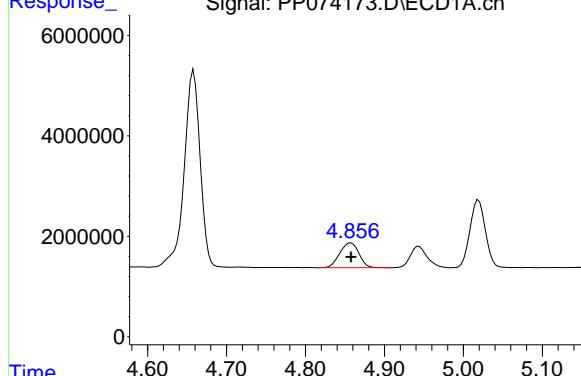


#8 AR-1221-1

R.T.: 4.015 min
 Delta R.T.: 0.000 min
 Response: 24542587
 Conc: 500.00 ng/ml

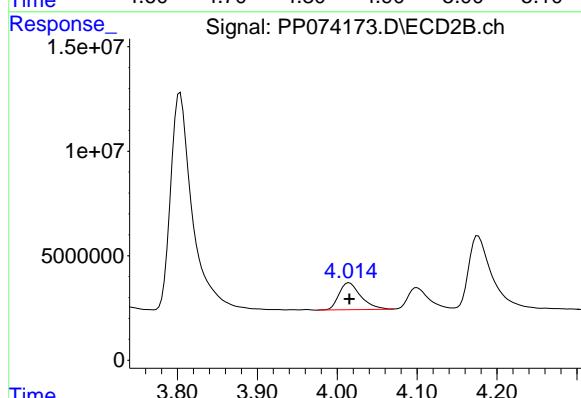


#9 AR-1221-2

R.T.: 4.944 min
 Delta R.T.: 0.000 min
 Response: 6300527
 Conc: 500.00 ng/ml

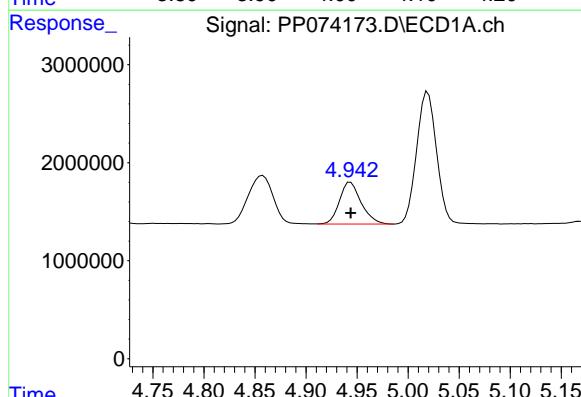

#9 AR-1221-2



R.T.: 4.100 min
 Delta R.T.: 0.000 min
 Response: 17944660
 Conc: 500.00 ng/ml

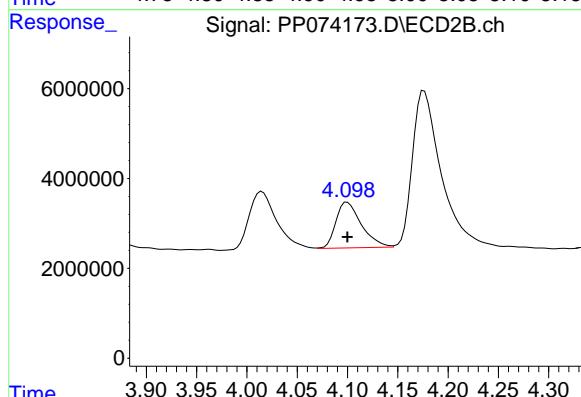

#10 AR-1221-3

R.T.: 5.019 min
Delta R.T.: 0.000 min
Response: 18317605
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1221ICC500

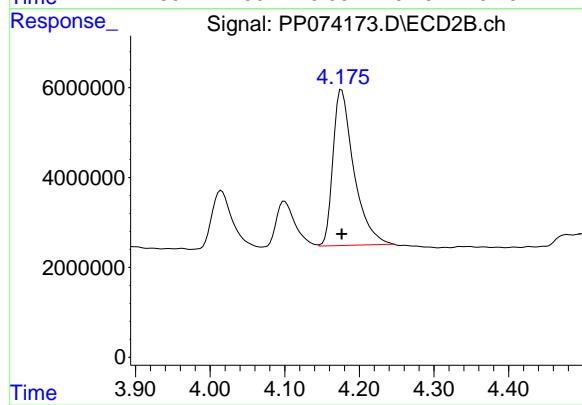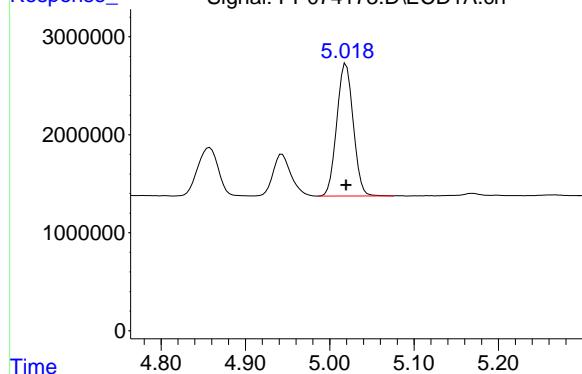

#10 AR-1221-3

R.T.: 4.176 min
Delta R.T.: 0.000 min
Response: 67612277
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:15
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:17:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:13:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.660 | 3.804 | 54684846 | 201.8E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.437 | 8.826 | 47117835 | 301.0E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 11) L3 AR-1232-1 | 5.020 | 4.177 | 14518661 | 50681220 | 500.000 | 500.000 |
| 12) L3 AR-1232-2 | 5.546 | 4.904 | 7521357 | 87133099 | 500.000 | 500.000 |
| 13) L3 AR-1232-3 | 5.832 | 5.081 | 14500854 | 22908311 | 500.000 | 500.000 |
| 14) L3 AR-1232-4 | 5.993 | 5.164 | 7734413 | 29005356 | 500.000 | 502.399m |
| 15) L3 AR-1232-5 | 6.082 | 5.338 | 5858006 | 23489726 | 500.000 | 500.000 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:15
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1



Instrument :
 ECD_P
 ClientSampleId :
 AR1232ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:17:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:13:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

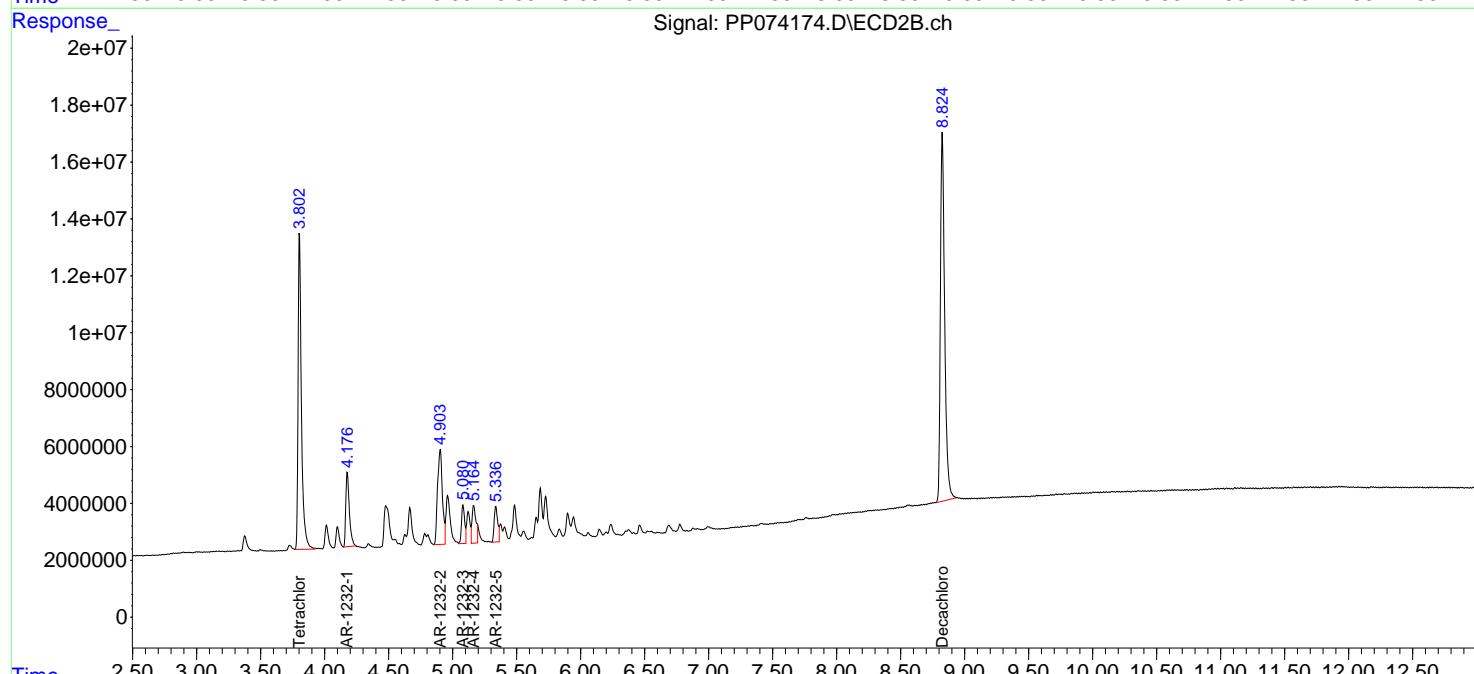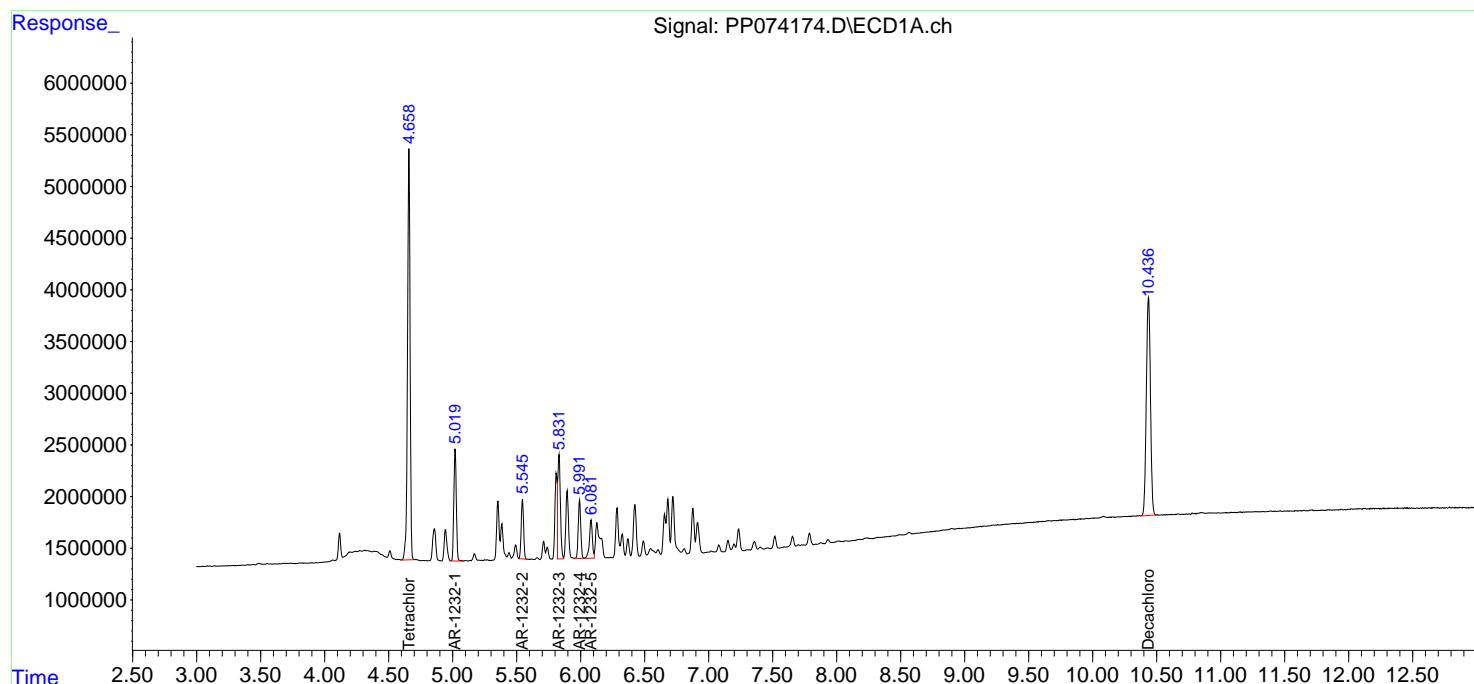

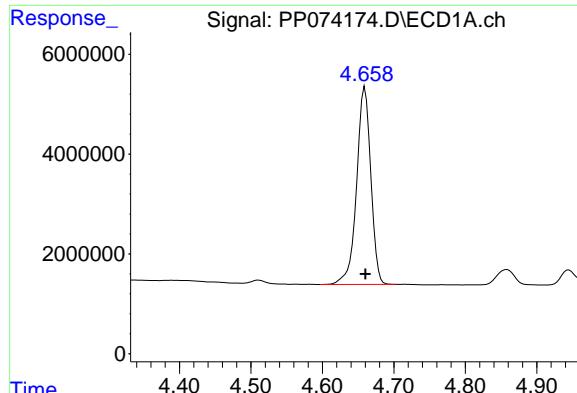


#1 Tetrachloro-m-xylene

R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 54684846
Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

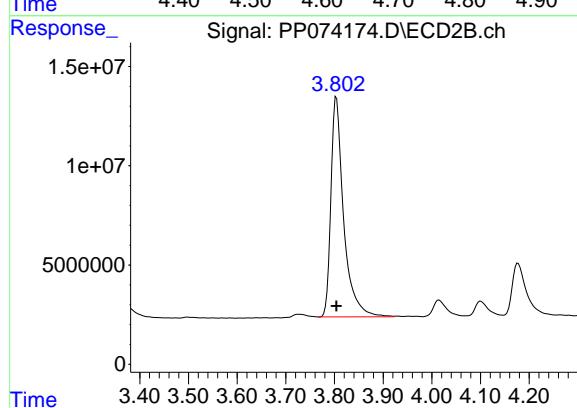


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 201821673
Conc: 50.00 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 47117835
Conc: 50.00 ng/ml

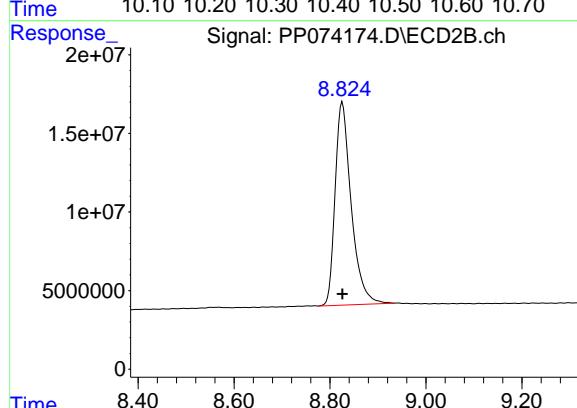

#2 Decachlorobiphenyl

R.T.: 8.826 min
Delta R.T.: 0.000 min
Response: 300994205
Conc: 50.00 ng/ml

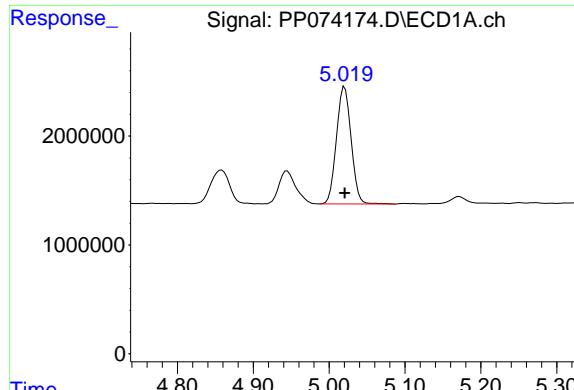


#11 AR-1232-1

R.T.: 5.020 min
Delta R.T.: 0.000 min
Response: 14518661
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

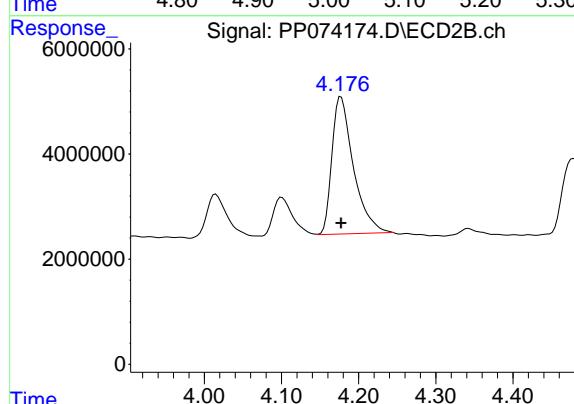


#11 AR-1232-1

R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 50681220
Conc: 500.00 ng/ml

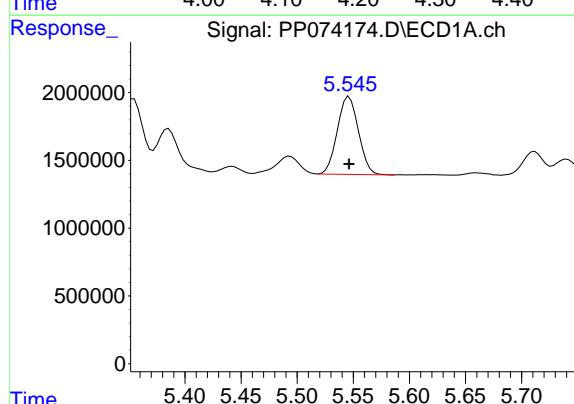


#12 AR-1232-2

R.T.: 5.546 min
Delta R.T.: 0.000 min
Response: 7521357
Conc: 500.00 ng/ml

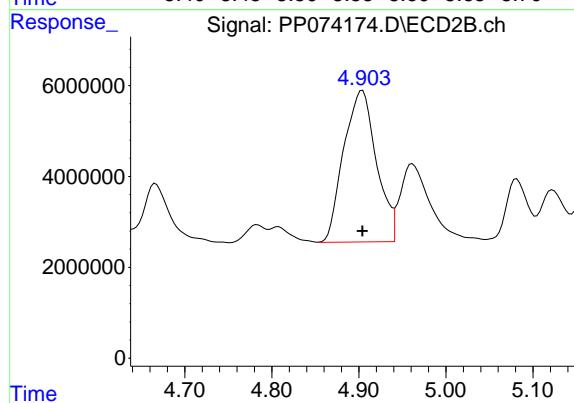

#12 AR-1232-2

R.T.: 4.904 min
Delta R.T.: 0.000 min
Response: 87133099
Conc: 500.00 ng/ml

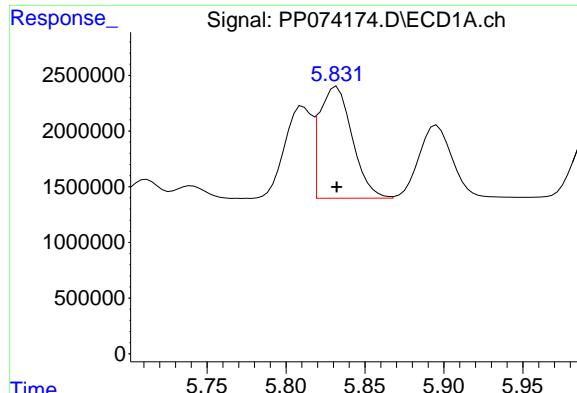


#13 AR-1232-3

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 14500854
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

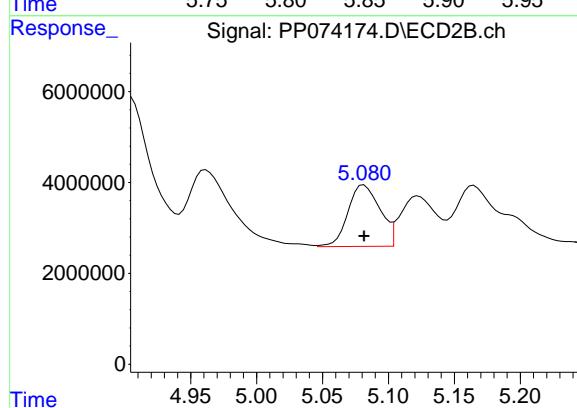


#13 AR-1232-3

R.T.: 5.081 min
Delta R.T.: 0.000 min
Response: 22908311
Conc: 500.00 ng/ml

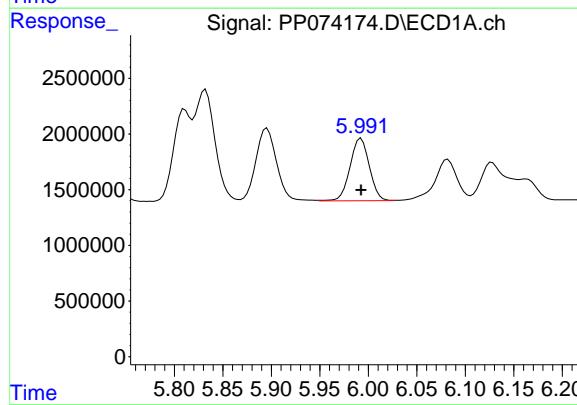

#14 AR-1232-4

R.T.: 5.993 min
Delta R.T.: 0.000 min
Response: 7734413
Conc: 500.00 ng/ml

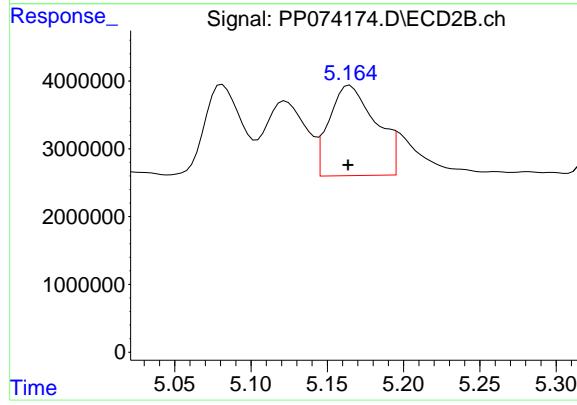

#14 AR-1232-4

R.T.: 5.164 min
Delta R.T.: 0.000 min
Response: 29005356
Conc: 502.40 ng/ml



#15 AR-1232-5

R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 5858006
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

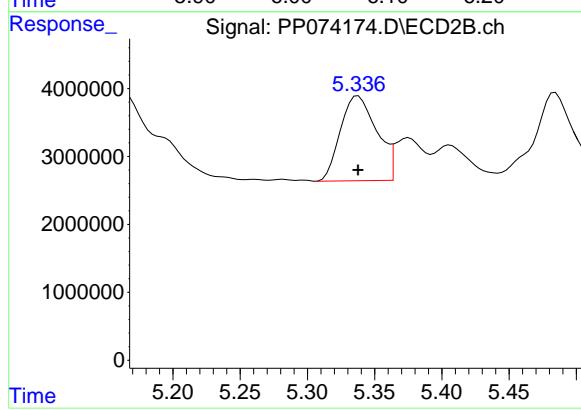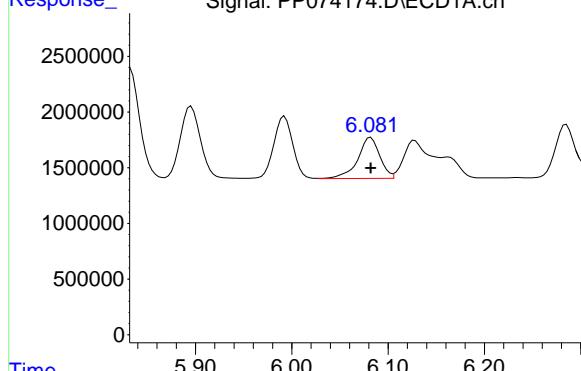

#15 AR-1232-5

R.T.: 5.338 min
 Delta R.T.: 0.000 min
 Response: 23489726
 Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:31
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:23:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|---------|
| 1) SA Tetrachlor... | 4.659 | 3.804 | 104.3E6 | 438.1E6 | 95.872 | 101.577 |
| 2) SA Decachlor... | 10.436 | 8.825 | 88078600 | 618.2E6 | 94.444 | 98.714 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 16) L4 AR-1242-1 | 5.811 | 4.905 | 31512428 | 341.3E6 | 934.658 | 978.632 |
| 17) L4 AR-1242-2 | 5.832 | 4.962 | 47421171 | 162.7E6 | 943.850 | 992.758 |
| 18) L4 AR-1242-3 | 5.896 | 5.082 | 30290298 | 93075141 | 931.794 | 1005.327 |
| 19) L4 AR-1242-4 | 5.992 | 5.164 | 25177060 | 117.3E6 | 934.754 | 940.884m |
| 20) L4 AR-1242-5 | 6.721 | 5.686 | 29128304 | 140.7E6 | 916.924 | 973.631 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:31
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1


Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:23:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1242ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

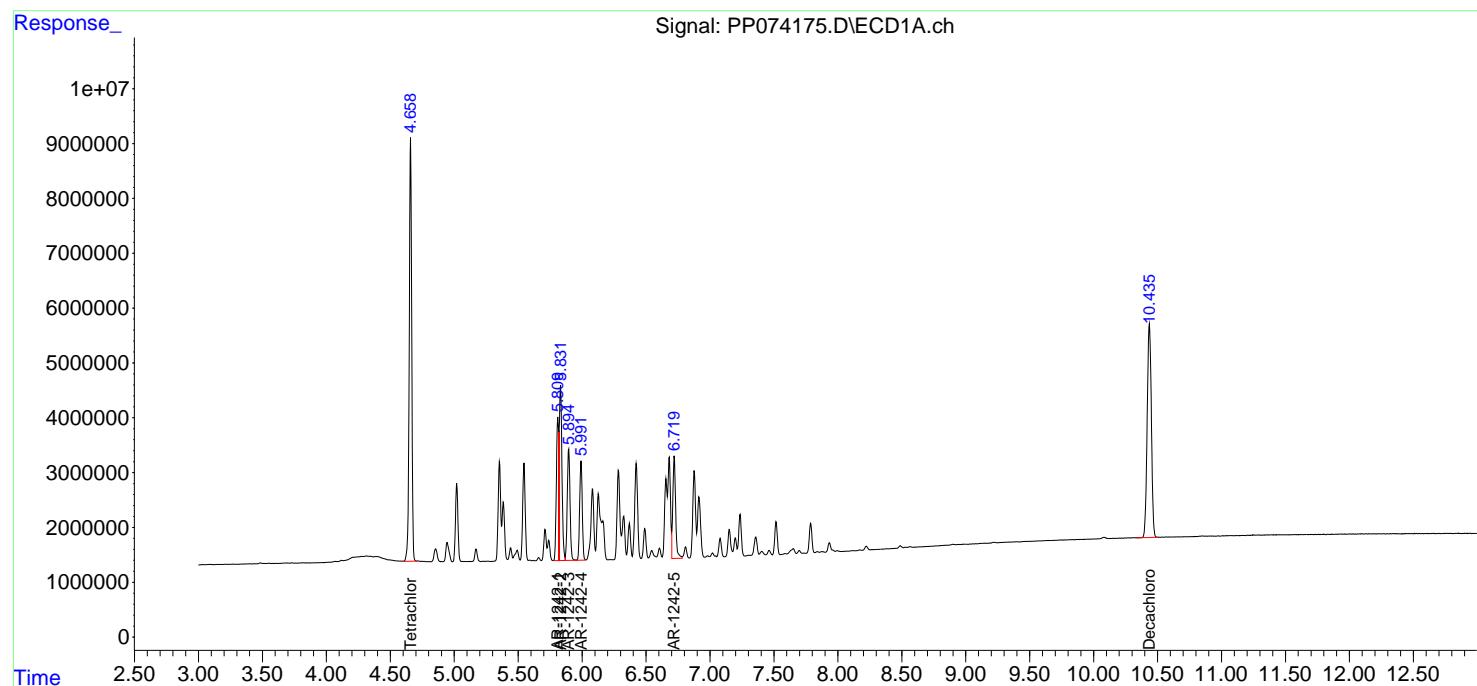




#1 Tetrachloro-m-xylene

R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 104324065
Conc: 95.87 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

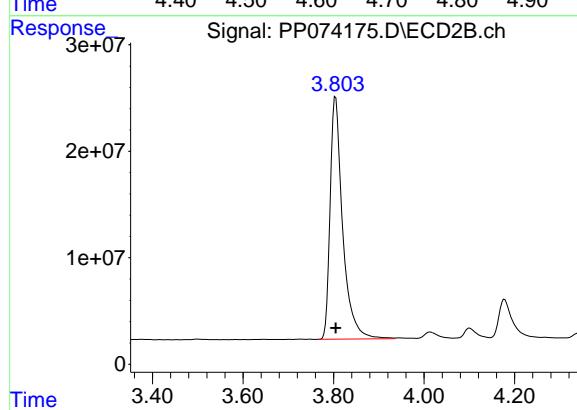


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 438073172
Conc: 101.58 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.000 min
Response: 88078600
Conc: 94.44 ng/ml

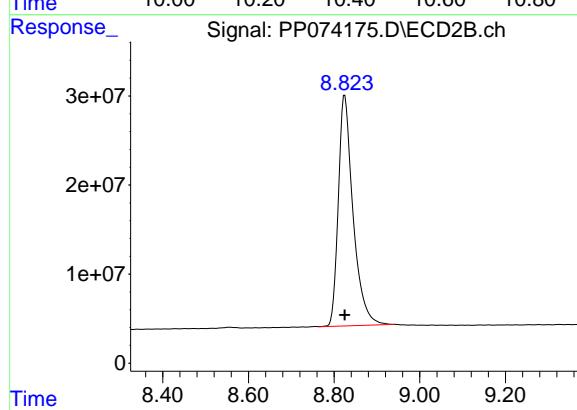

#2 Decachlorobiphenyl

R.T.: 8.825 min
Delta R.T.: 0.000 min
Response: 618210330
Conc: 98.71 ng/ml





#16 AR-1242-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 31512428
 Conc: 934.66 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

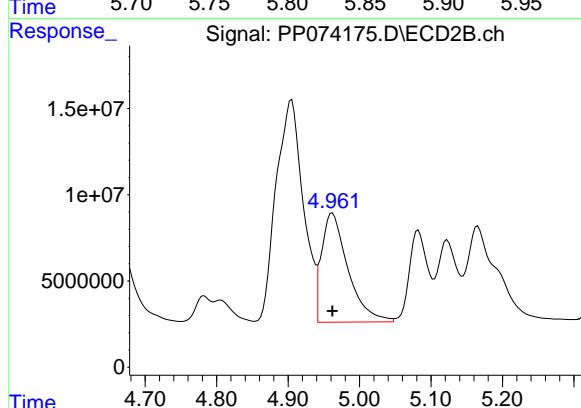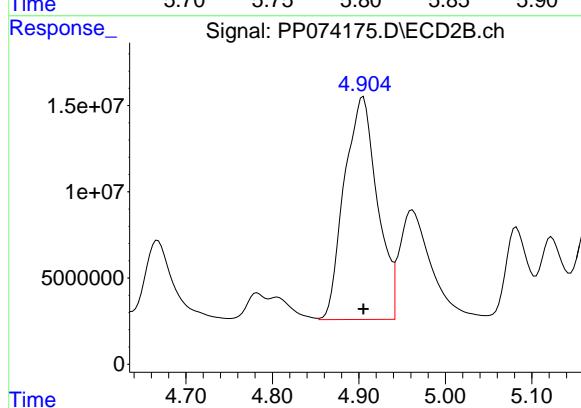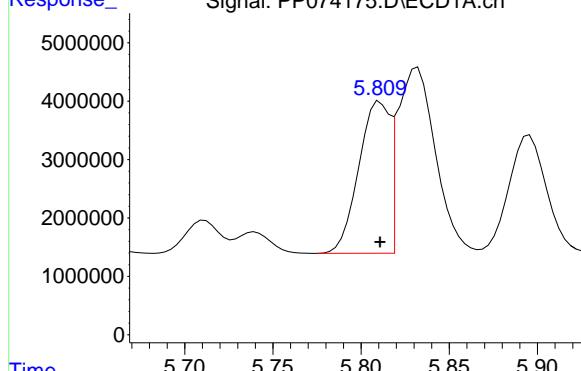

#16 AR-1242-1

R.T.: 4.905 min
 Delta R.T.: 0.000 min
 Response: 341272725
 Conc: 978.63 ng/ml

#17 AR-1242-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 47421171
 Conc: 943.85 ng/ml

#17 AR-1242-2

R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 162660327
 Conc: 992.76 ng/ml

#18 AR-1242-3

R.T.: 5.896 min
 Delta R.T.: 0.000 min
 Response: 30290298
 Conc: 931.79 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#18 AR-1242-3





R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 93075141
 Conc: 1005.33 ng/ml

#19 AR-1242-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 25177060
 Conc: 934.75 ng/ml

#19 AR-1242-4

R.T.: 5.164 min
 Delta R.T.: 0.000 min
 Response: 117292839
 Conc: 940.88 ng/ml

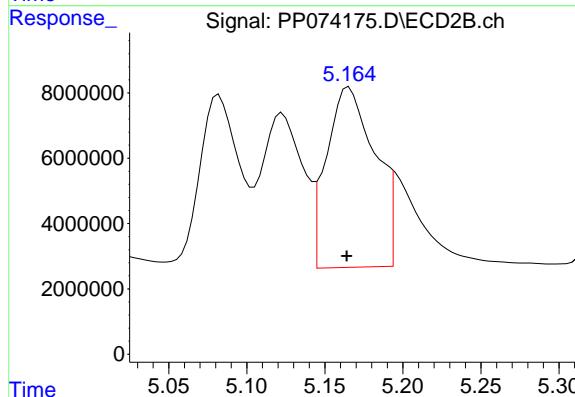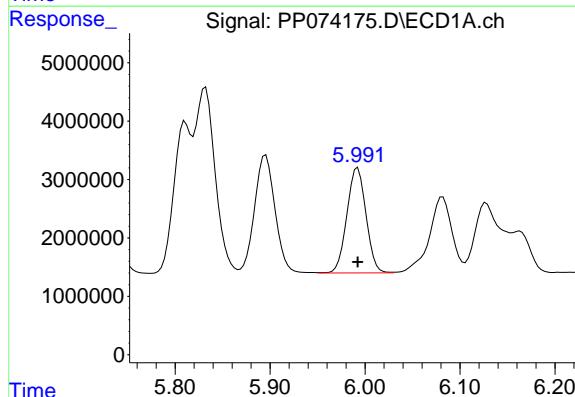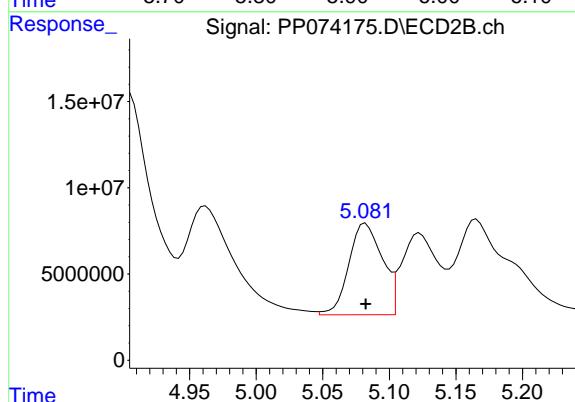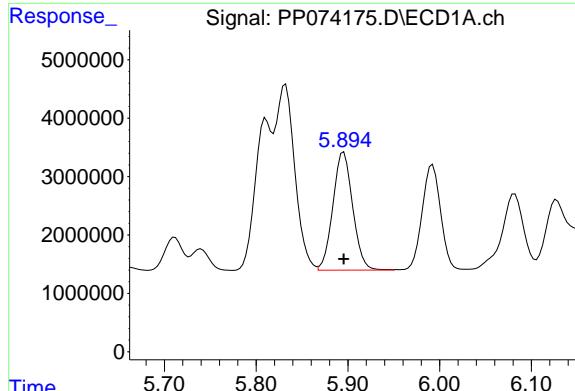



#20 AR-1242-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 29128304
 Conc: 916.92 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

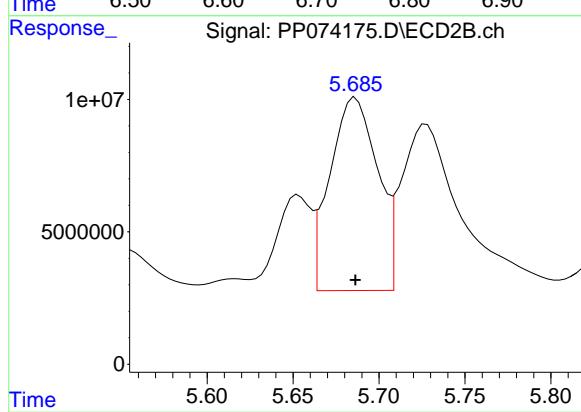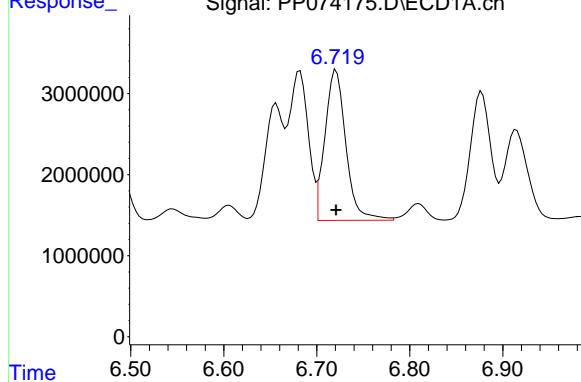

#20 AR-1242-5

R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 140731652
 Conc: 973.63 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:47
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:26:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.662 | 3.803 | 80676637 | 324.0E6 | 74.425 | 75.083 |
| 2) SA Decachlor... | 10.438 | 8.824 | 68962955 | 464.9E6 | 74.295 | 74.485 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 16) L4 AR-1242-1 | 5.813 | 4.904 | 25064705 | 261.4E6 | 745.599 | 749.732 |
| 17) L4 AR-1242-2 | 5.835 | 4.960 | 37017188 | 128.7E6 | 741.131 | 773.381 |
| 18) L4 AR-1242-3 | 5.898 | 5.081 | 24057234 | 72718391 | 743.338 | 773.266 |
| 19) L4 AR-1242-4 | 5.995 | 5.163 | 19974989 | 87588686 | 744.389 | 713.205m |
| 20) L4 AR-1242-5 | 6.724 | 5.685 | 24065795 | 114.3E6 | 755.025 | 776.822 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:47
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:26:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1242ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

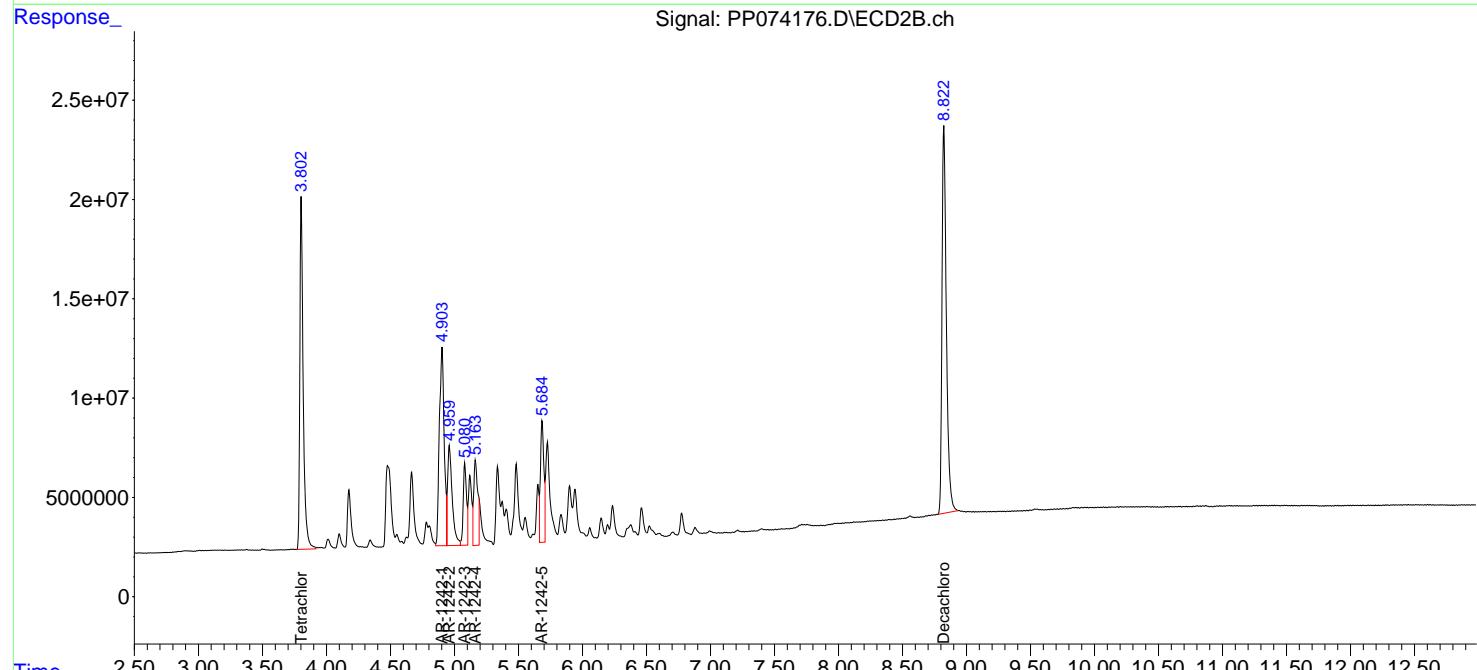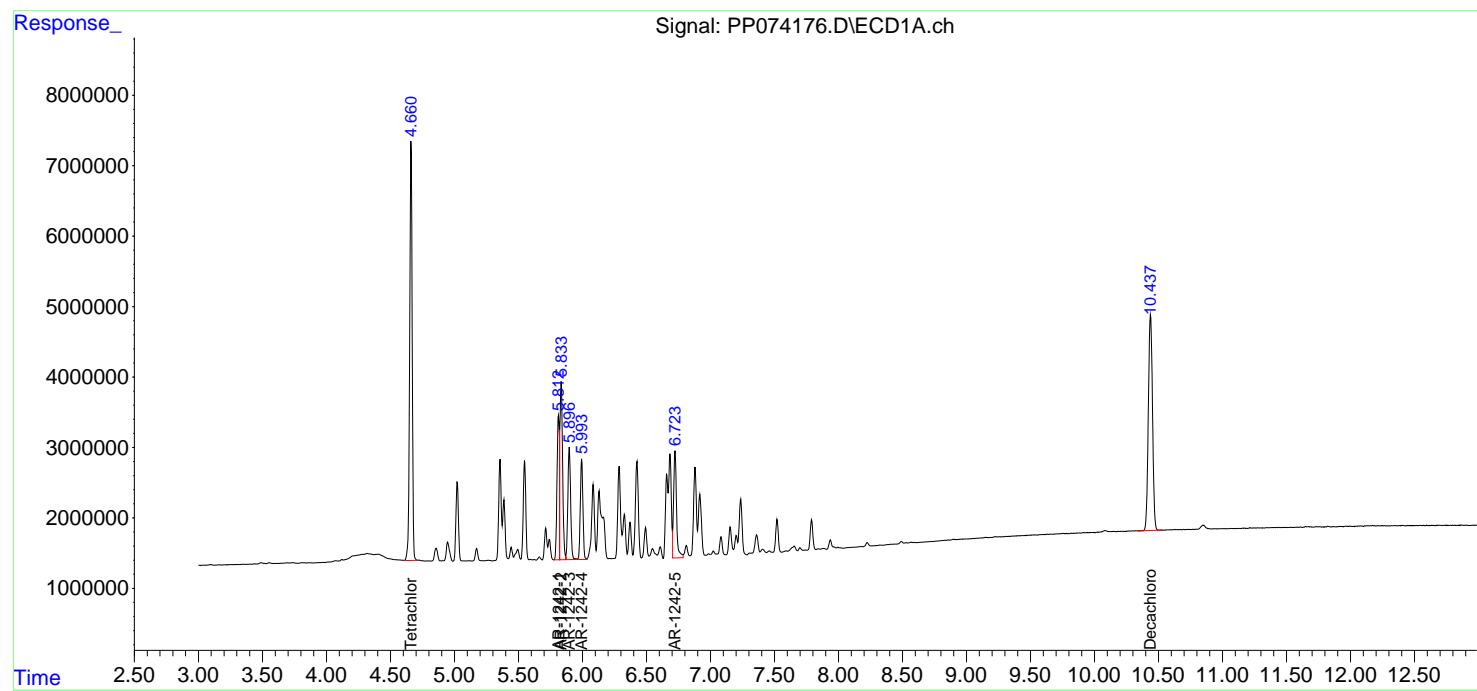

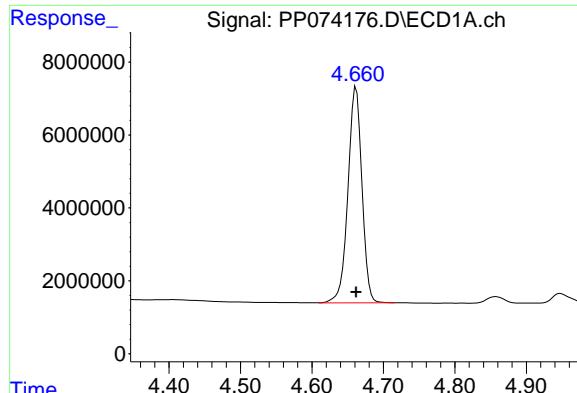


#1 Tetrachloro-m-xylene

R.T.: 4.662 min
Delta R.T.: 0.000 min
Response: 80676637
Conc: 74.42 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

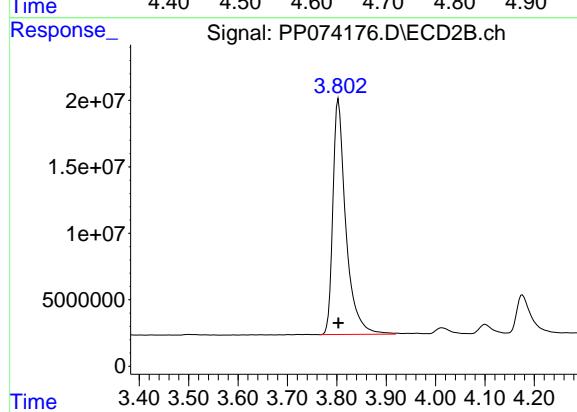


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 323988872
Conc: 75.08 ng/ml







#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.000 min
Response: 68962955
Conc: 74.29 ng/ml

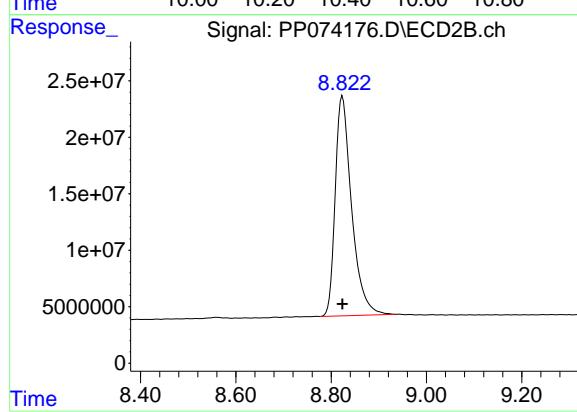

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 464876495
Conc: 74.48 ng/ml

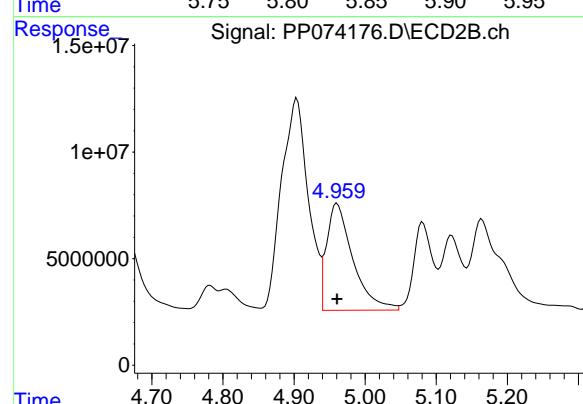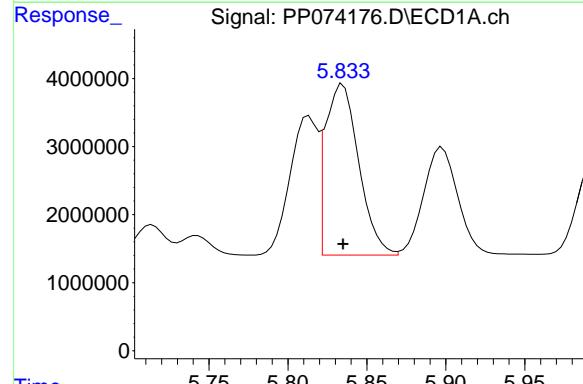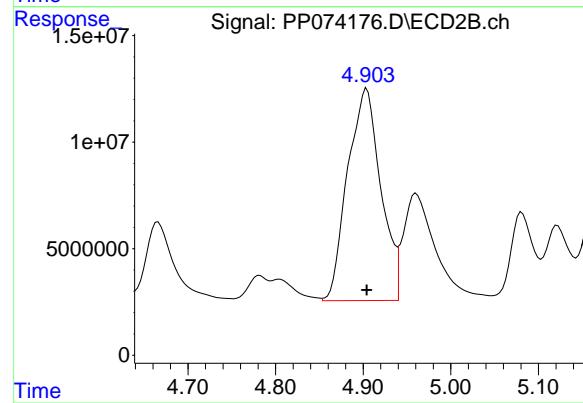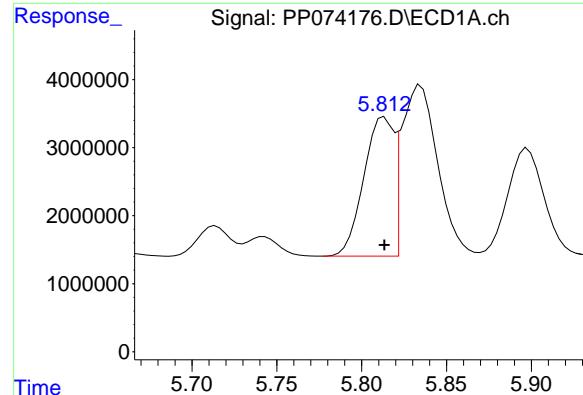

#16 AR-1242-1

R.T.: 5.813 min
 Delta R.T.: 0.000 min
 Response: 25064705
 Conc: 745.60 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#16 AR-1242-1

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 261402874
 Conc: 749.73 ng/ml

#17 AR-1242-2

R.T.: 5.835 min
 Delta R.T.: 0.000 min
 Response: 37017188
 Conc: 741.13 ng/ml

#17 AR-1242-2

R.T.: 4.960 min
 Delta R.T.: 0.000 min
 Response: 128722469
 Conc: 773.38 ng/ml





#18 AR-1242-3

R.T.: 5.898 min
 Delta R.T.: 0.000 min
 Response: 24057234
 Conc: 743.34 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

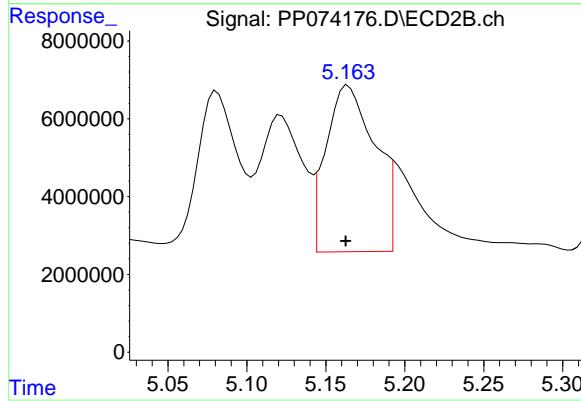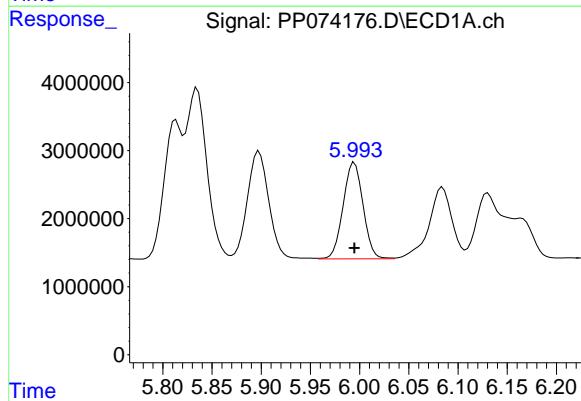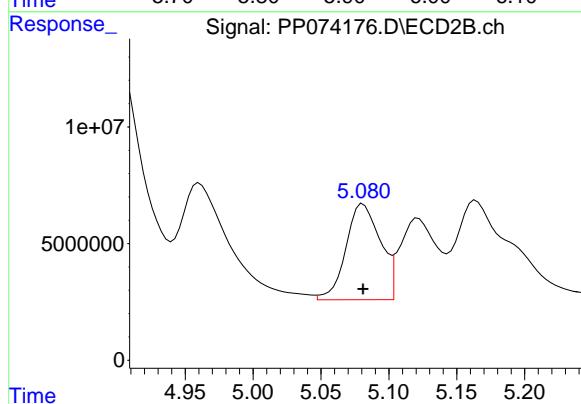

#18 AR-1242-3

R.T.: 5.081 min
 Delta R.T.: 0.000 min
 Response: 72718391
 Conc: 773.27 ng/ml

#19 AR-1242-4

R.T.: 5.995 min
 Delta R.T.: 0.000 min
 Response: 19974989
 Conc: 744.39 ng/ml

#19 AR-1242-4

R.T.: 5.163 min
 Delta R.T.: 0.000 min
 Response: 87588686
 Conc: 713.20 ng/ml



#20 AR-1242-5

R.T.: 6.724 min
 Delta R.T.: 0.000 min
 Response: 24065795
 Conc: 755.02 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

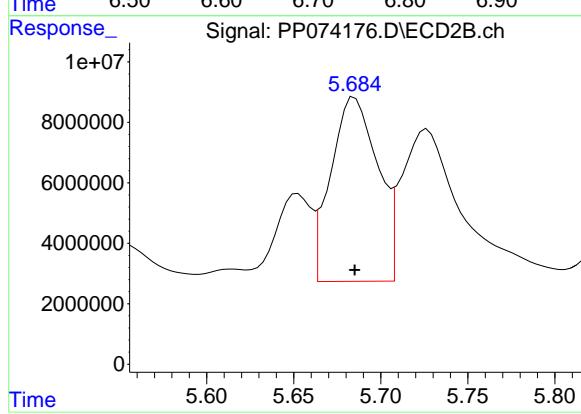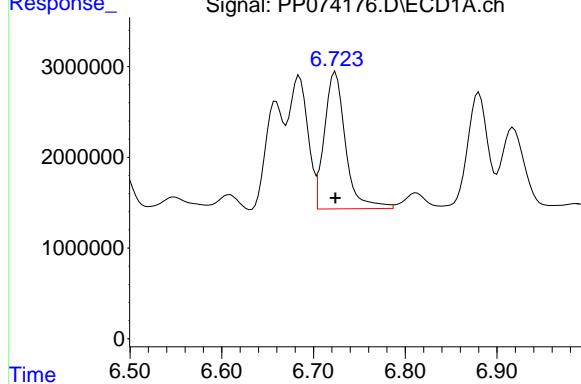

#20 AR-1242-5

R.T.: 5.685 min
 Delta R.T.: 0.000 min
 Response: 114328693
 Conc: 776.82 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:03
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:21:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.805 | 56653742 | 212.2E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.434 | 8.826 | 49220928 | 317.2E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 16) L4 AR-1242-1 | 5.808 | 4.905 | 17959256 | 178.1E6 | 500.000 | 500.000 |
| 17) L4 AR-1242-2 | 5.830 | 4.963 | 26531667 | 82516708 | 500.000 | 500.000 |
| 18) L4 AR-1242-3 | 5.893 | 5.084 | 17362372 | 46044427 | 500.000 | 500.000 |
| 19) L4 AR-1242-4 | 5.990 | 5.164 | 14345906 | 63188535 | 500.000 | 505.329m |
| 20) L4 AR-1242-5 | 6.719 | 5.687 | 17203244 | 74177320 | 500.000 | 500.000 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:03
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:21:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1242ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

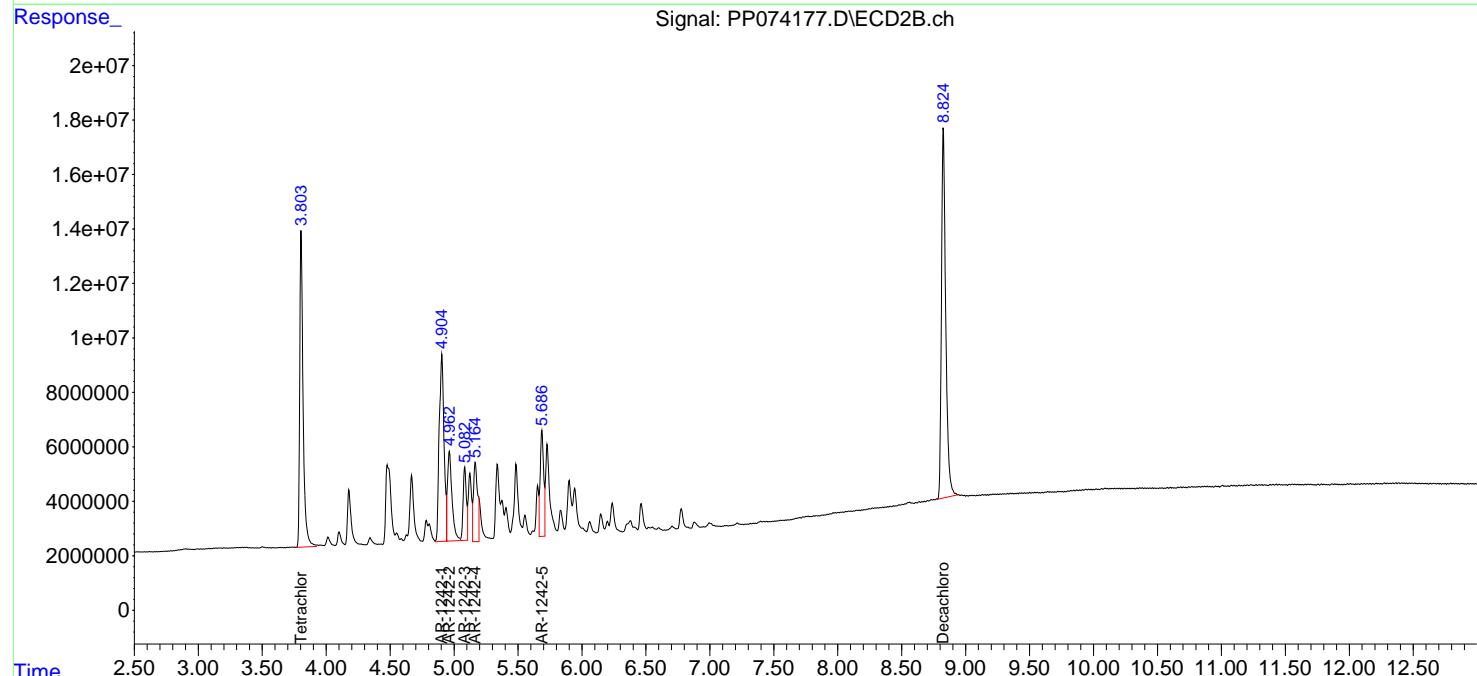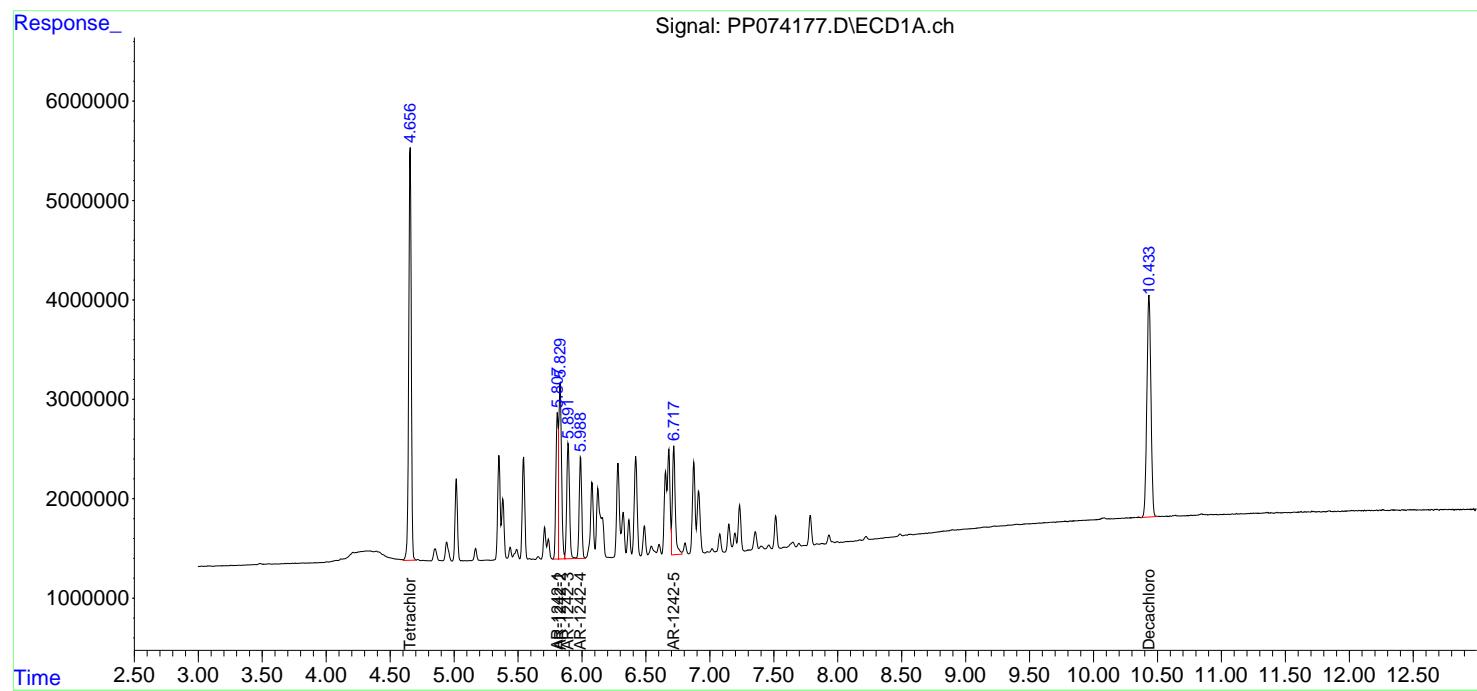

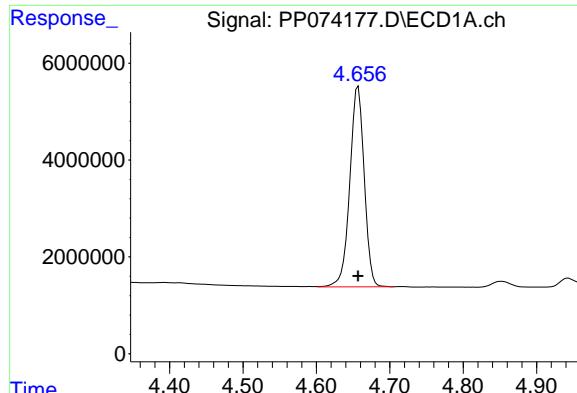


#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 56653742
Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

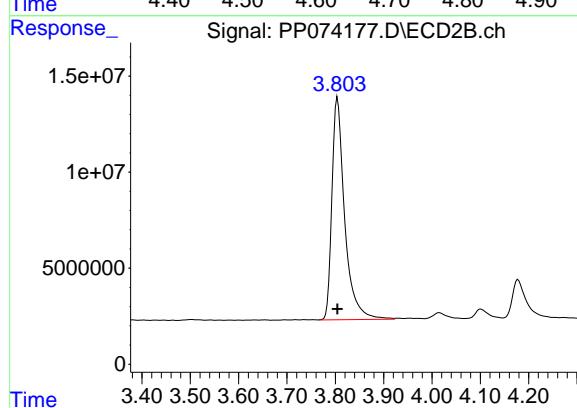


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 212235944
Conc: 50.00 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.000 min
Response: 49220928
Conc: 50.00 ng/ml

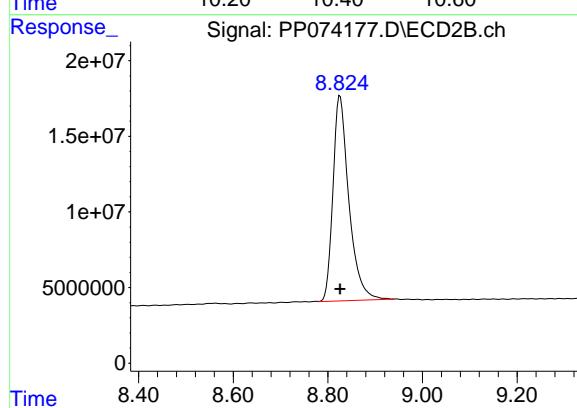

#2 Decachlorobiphenyl

R.T.: 8.826 min
Delta R.T.: 0.000 min
Response: 317160143
Conc: 50.00 ng/ml





#16 AR-1242-1

R.T.: 5.808 min
 Delta R.T.: 0.000 min
 Response: 17959256
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

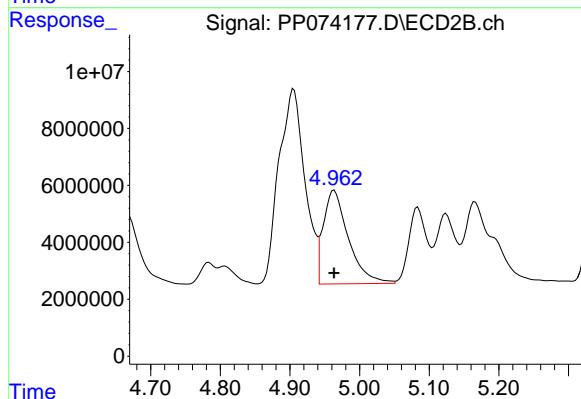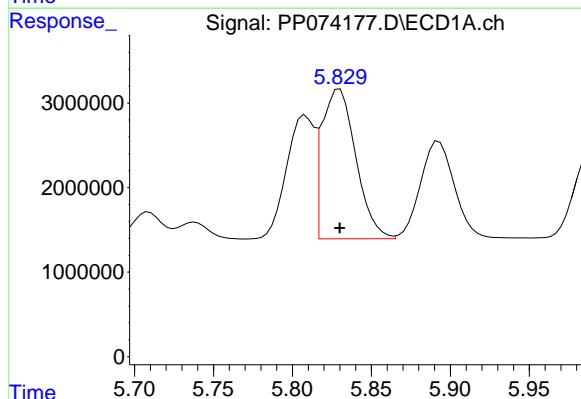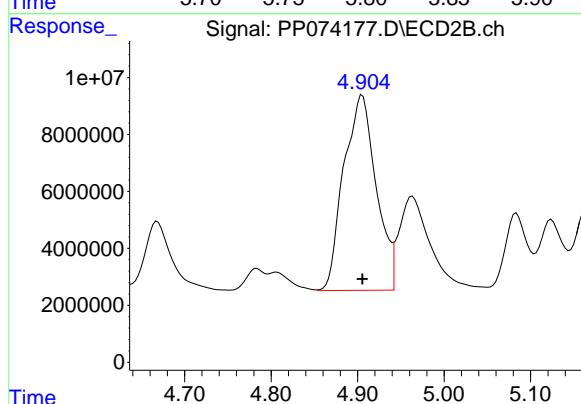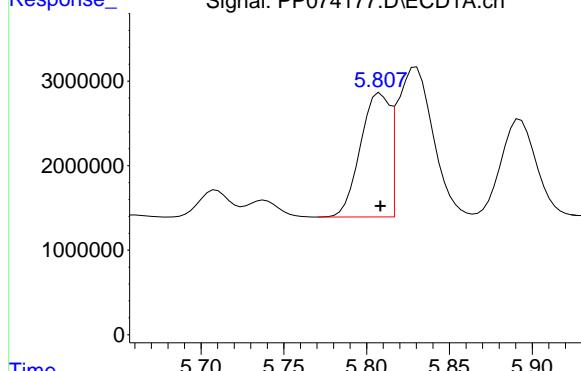

#16 AR-1242-1

R.T.: 4.905 min
 Delta R.T.: 0.000 min
 Response: 178087793
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 5.830 min
 Delta R.T.: 0.000 min
 Response: 26531667
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 4.963 min
 Delta R.T.: 0.000 min
 Response: 82516708
 Conc: 500.00 ng/ml

#18 AR-1242-3

R.T.: 5.893 min
 Delta R.T.: 0.000 min
 Response: 17362372
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#18 AR-1242-3





R.T.: 5.084 min
 Delta R.T.: 0.000 min
 Response: 46044427
 Conc: 500.00 ng/ml


#19 AR-1242-4

R.T.: 5.990 min
 Delta R.T.: 0.000 min
 Response: 14345906
 Conc: 500.00 ng/ml

#19 AR-1242-4

R.T.: 5.164 min
 Delta R.T.: 0.000 min
 Response: 63188535
 Conc: 505.33 ng/ml

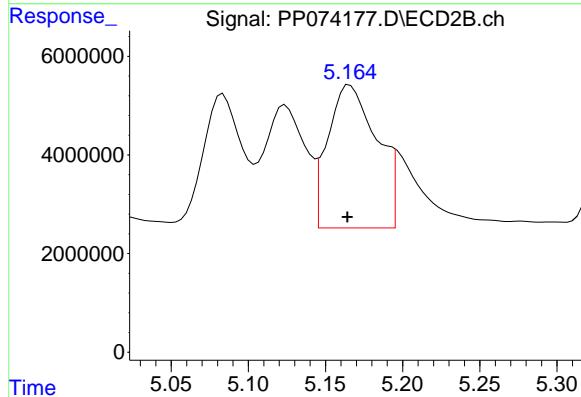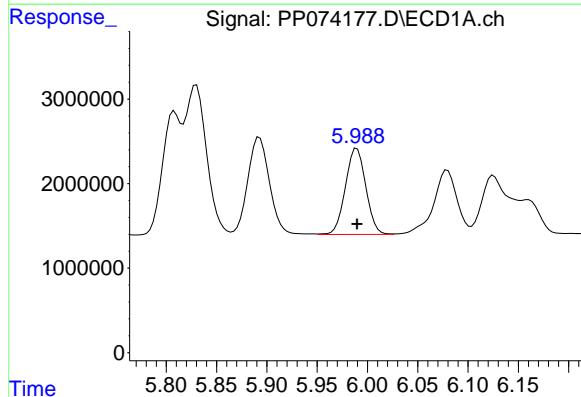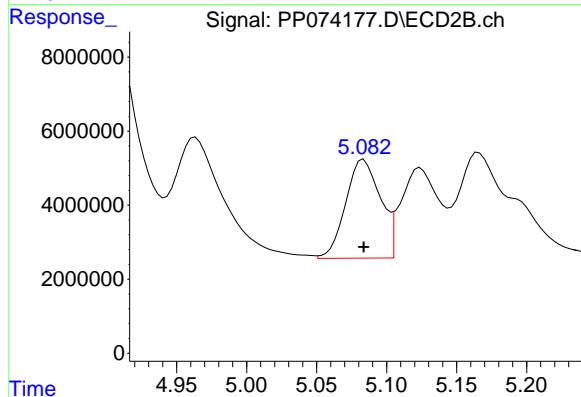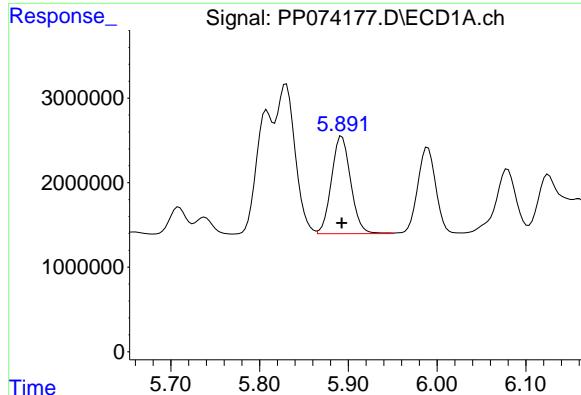

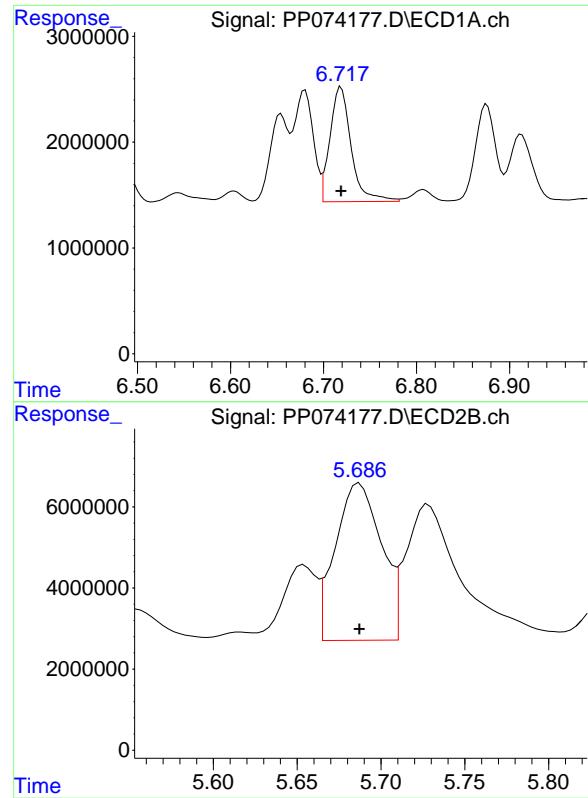

#20 AR-1242-5

R.T.: 6.719 min
 Delta R.T.: 0.000 min
 Response: 17203244
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#20 AR-1242-5

R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 74177320
 Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:19
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:30:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.662 | 3.805 | 30064825 | 99448361 | 26.997 | 23.506 |
| 2) SA Decachlor... | 10.436 | 8.824 | 26416078 | 156.4E6 | 27.507 | 25.039 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|----------|
| 16) L4 AR-1242-1 | 5.812 | 4.906 | 9924005 | 89565172 | 282.440 | 255.127 |
| 17) L4 AR-1242-2 | 5.834 | 4.964 | 14472673 | 42174411 | 278.680 | 252.533 |
| 18) L4 AR-1242-3 | 5.897 | 5.084 | 9547202 | 24305838 | 282.294 | 256.293 |
| 19) L4 AR-1242-4 | 5.994 | 5.165 | 7737538 | 30145402 | 277.699 | 249.527m |
| 20) L4 AR-1242-5 | 6.721 | 5.687 | 9674193 | 38870481 | 289.648m | 260.436 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:19
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1



Instrument :
 ECD_P
ClientSampleId :
 AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:30:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

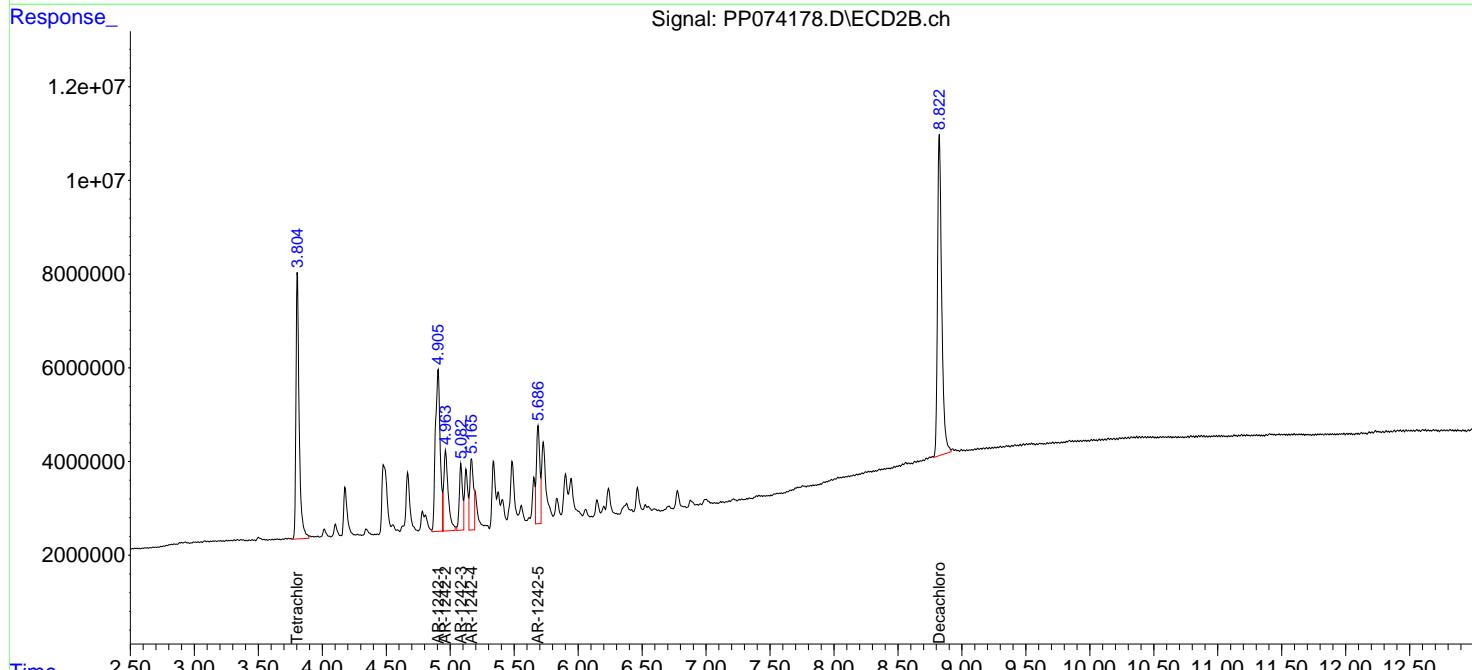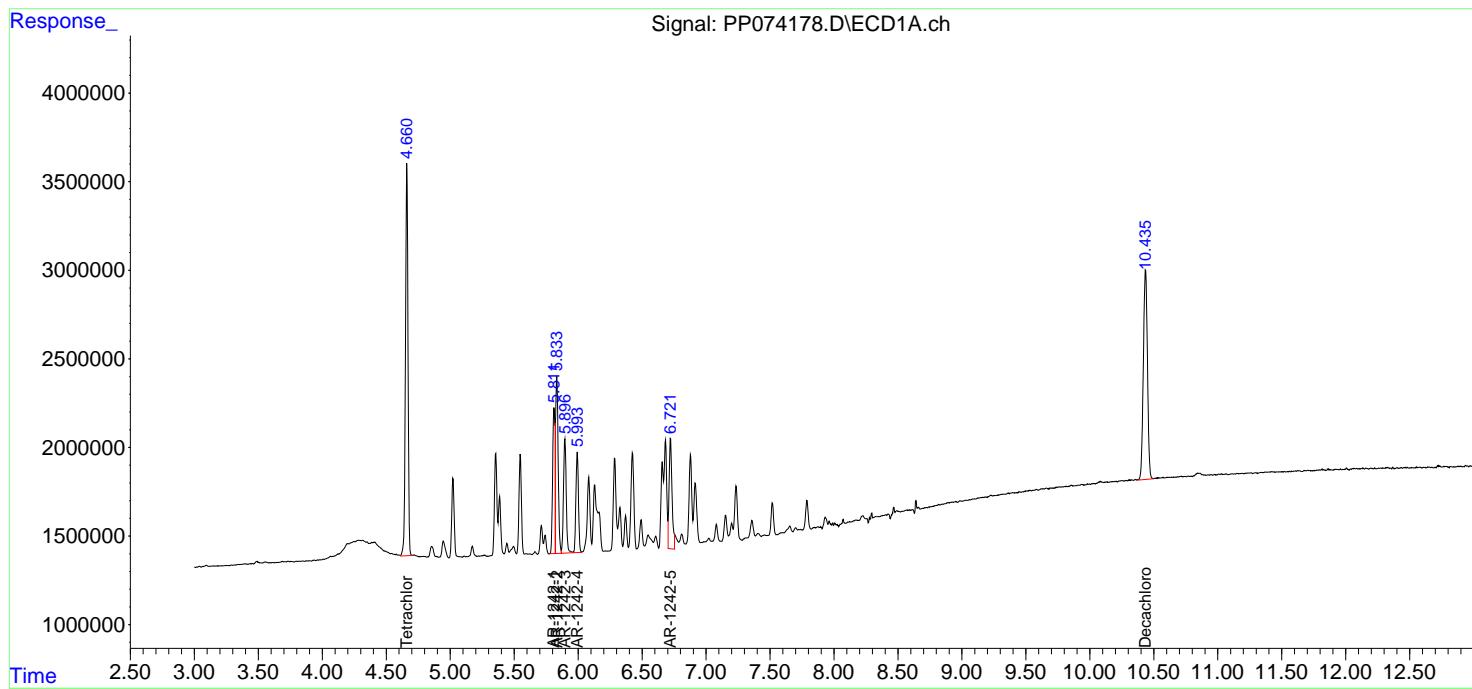

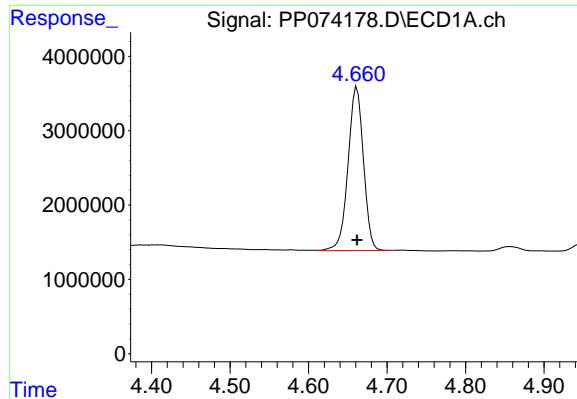


#1 Tetrachloro-m-xylene

R.T.: 4.662 min
Delta R.T.: 0.000 min
Response: 30064825
Conc: 27.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

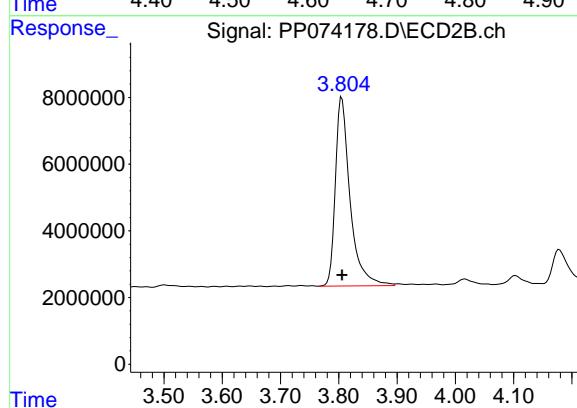


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 99448361
Conc: 23.51 ng/ml

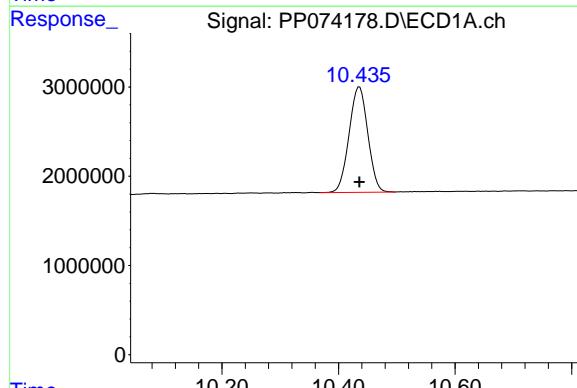



#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.000 min
Response: 26416078
Conc: 27.51 ng/ml

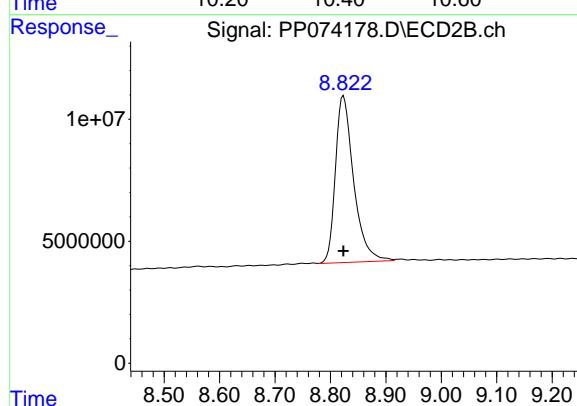

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 156351248
Conc: 25.04 ng/ml

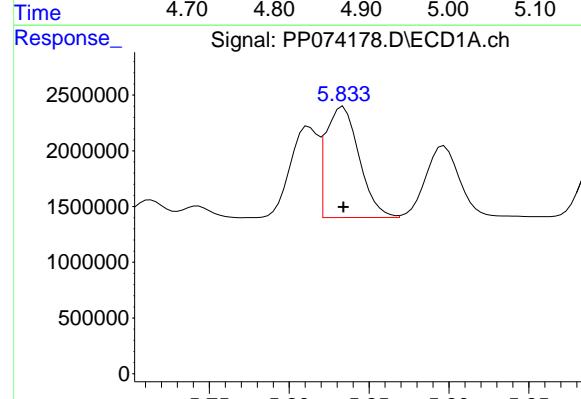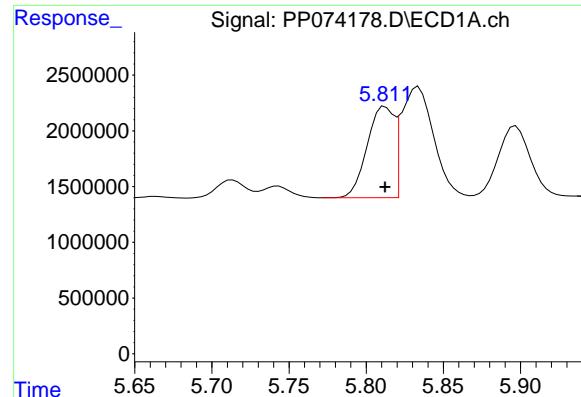

#16 AR-1242-1

R.T.: 5.812 min
 Delta R.T.: 0.000 min
 Response: 9924005
 Conc: 282.44 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#16 AR-1242-1


R.T.: 4.906 min
 Delta R.T.: 0.000 min
 Response: 89565172
 Conc: 255.13 ng/ml

#17 AR-1242-2

R.T.: 5.834 min
 Delta R.T.: 0.000 min
 Response: 14472673
 Conc: 278.68 ng/ml

#17 AR-1242-2

R.T.: 4.964 min
 Delta R.T.: 0.000 min
 Response: 42174411
 Conc: 252.53 ng/ml

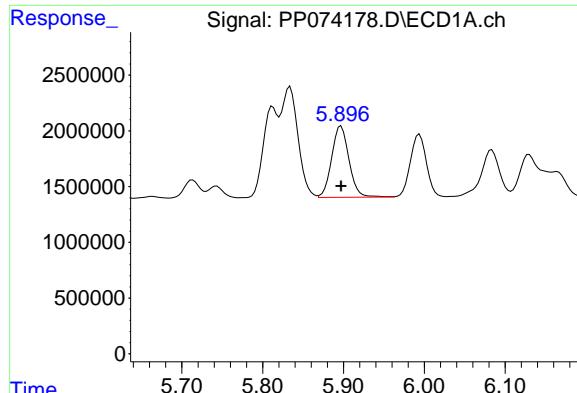


#18 AR-1242-3

R.T.: 5.897 min
Delta R.T.: 0.000 min
Response: 9547202
Conc: 282.29 ng/ml

Instrument: ECD_P
ClientSampleId : AR1242ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

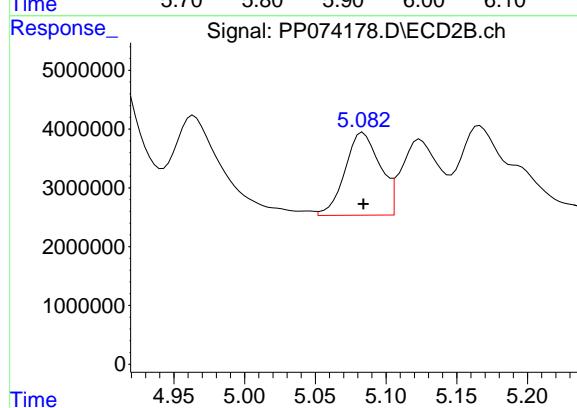


#18 AR-1242-3

R.T.: 5.084 min
Delta R.T.: 0.000 min
Response: 24305838
Conc: 256.29 ng/ml

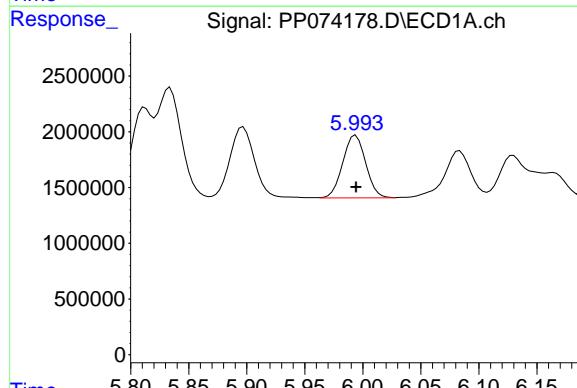

#19 AR-1242-4

R.T.: 5.994 min
Delta R.T.: 0.000 min
Response: 7737538
Conc: 277.70 ng/ml

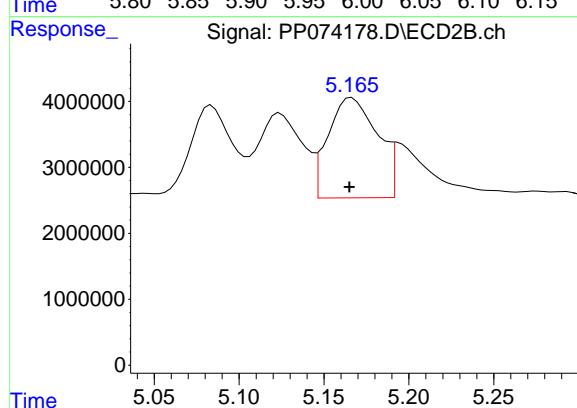

#19 AR-1242-4

R.T.: 5.165 min
Delta R.T.: 0.000 min
Response: 30145402
Conc: 249.53 ng/ml



#20 AR-1242-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 9674193
 Conc: 289.65 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

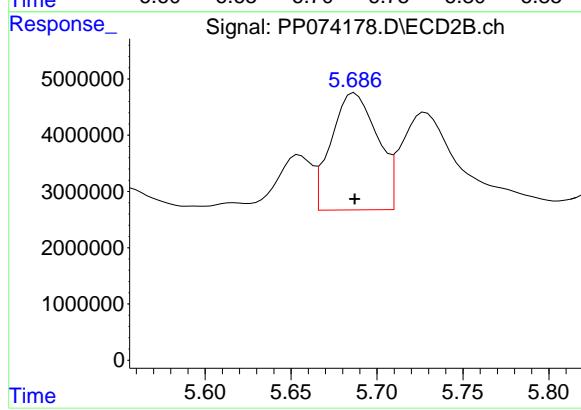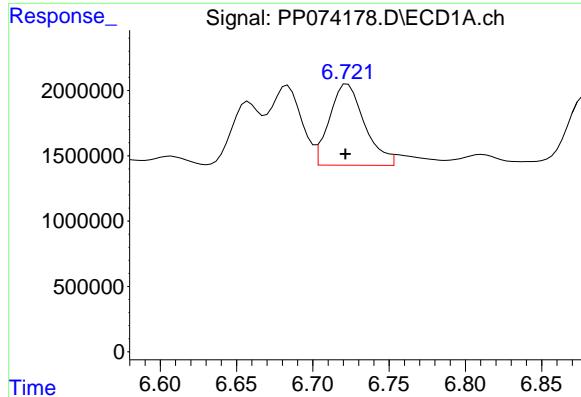

#20 AR-1242-5

R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 38870481
 Conc: 260.44 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:36
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:58:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:57:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|---------|----------|--------|---------|
| 1) SA Tetrachlor... | 4.657 | 3.802 | 6853903 | 15691561 | 5.892m | 3.915m# |
| 2) SA Decachlor... | 10.432 | 8.821 | 6026260 | 28194628 | 5.971 | 4.604 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|----------|
| 16) L4 AR-1242-1 | 5.810 | 4.903 | 2289125 | 16072866 | 61.427 | 46.569 |
| 17) L4 AR-1242-2 | 5.832 | 4.962 | 3215660 | 7443347 | 59.102 | 45.559 |
| 18) L4 AR-1242-3 | 5.895 | 5.082 | 2169957 | 4094869 | 60.722 | 44.390 # |
| 19) L4 AR-1242-4 | 5.991 | 5.163 | 1732044 | 5803584 | 59.279 | 48.597 |
| 20) L4 AR-1242-5 | 6.720 | 5.686 | 2173540 | 7539678 | 56.364m | 50.412 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:36
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:58:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:57:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

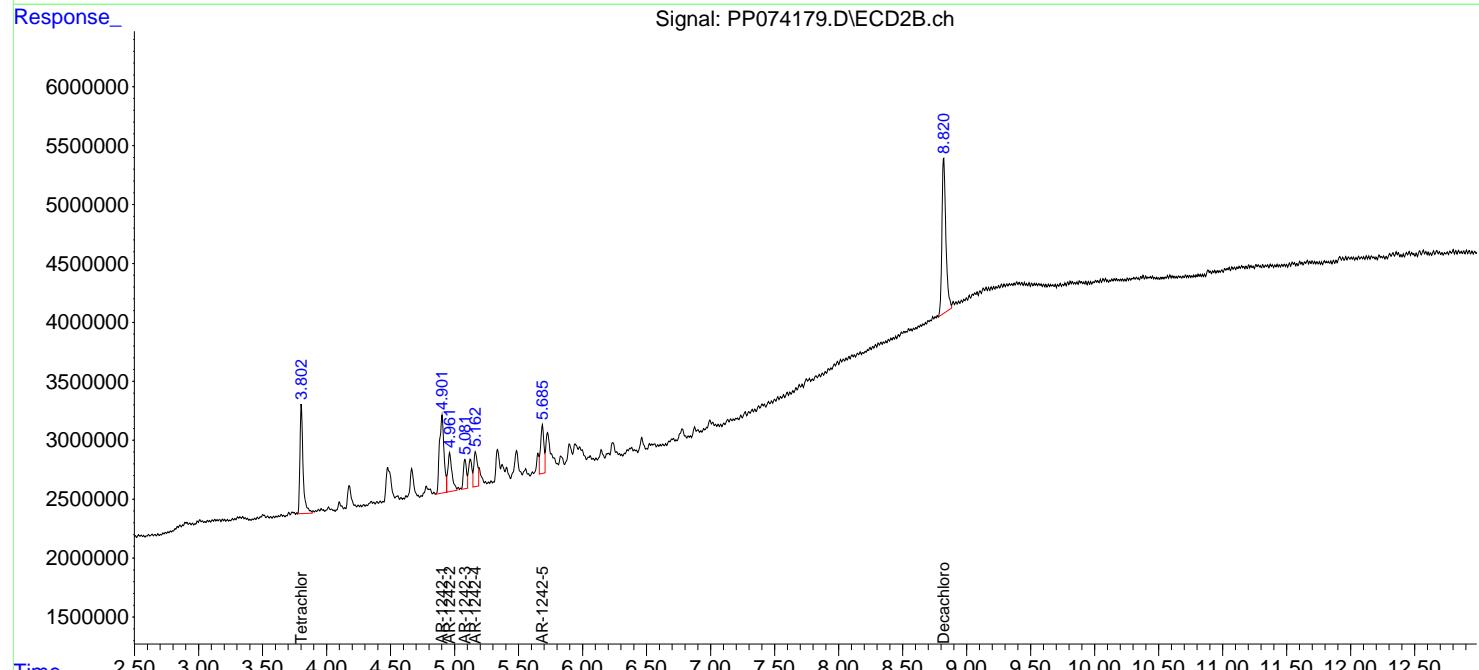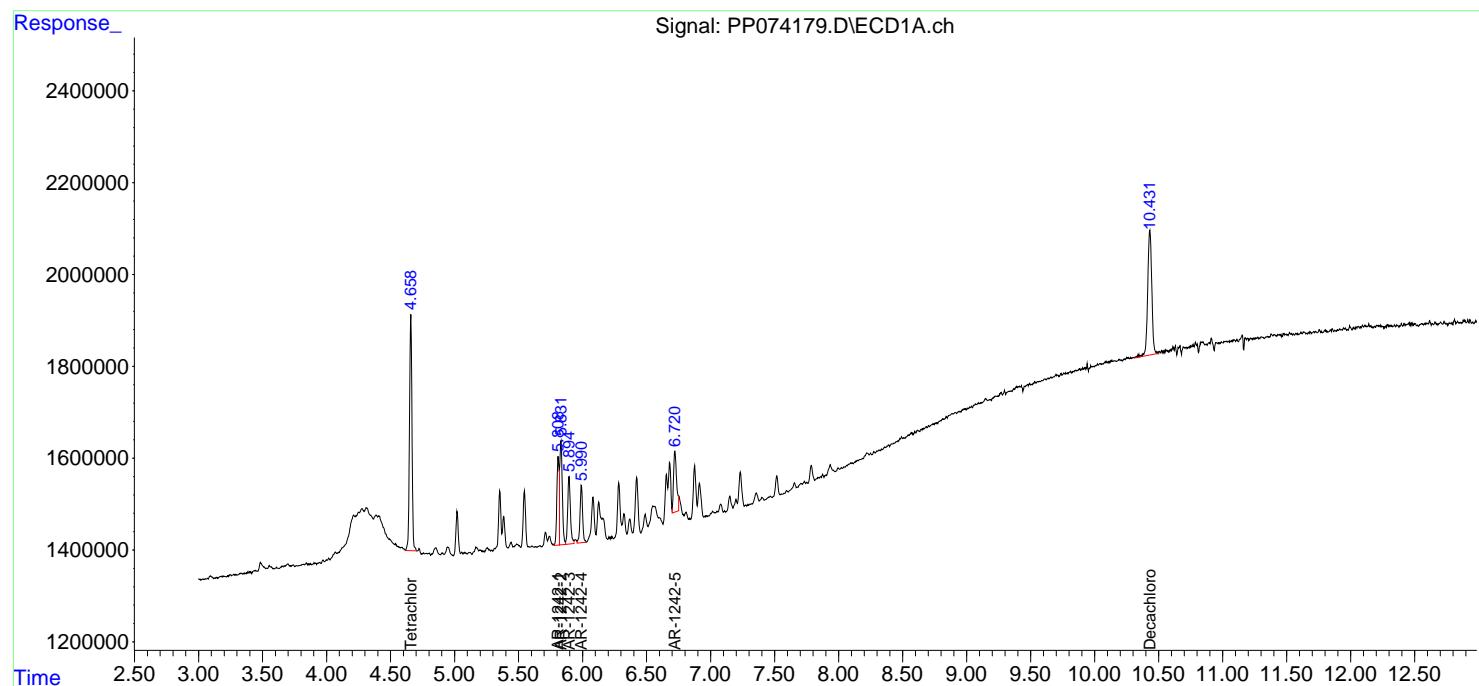

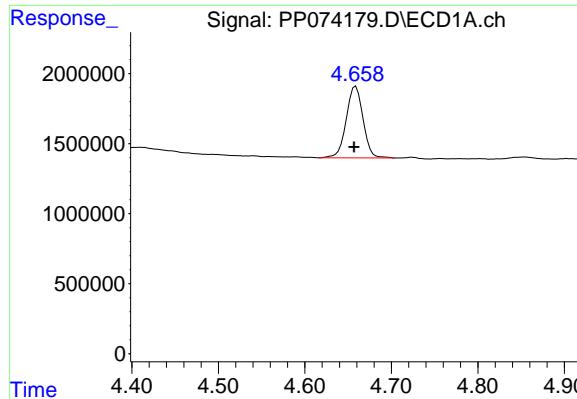


#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 6853903
Conc: 5.89 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

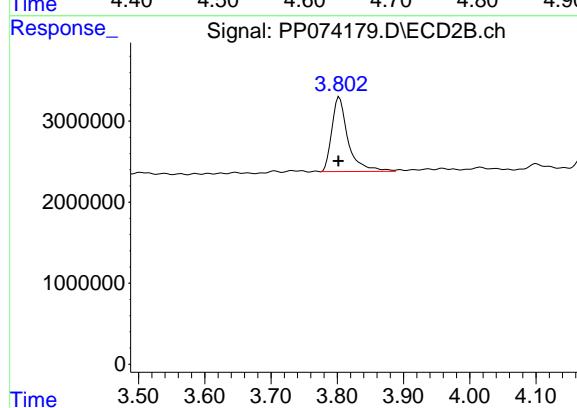


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: 0.000 min
Response: 15691561
Conc: 3.91 ng/ml

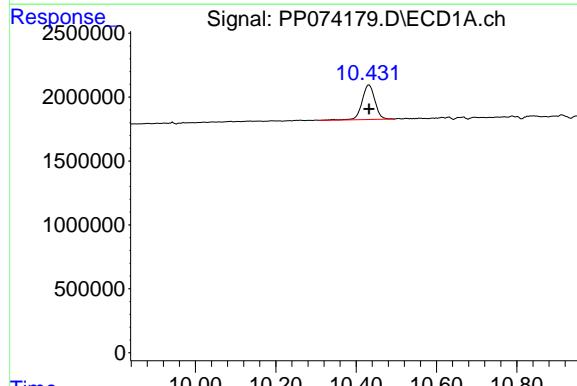





#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 6026260
Conc: 5.97 ng/ml

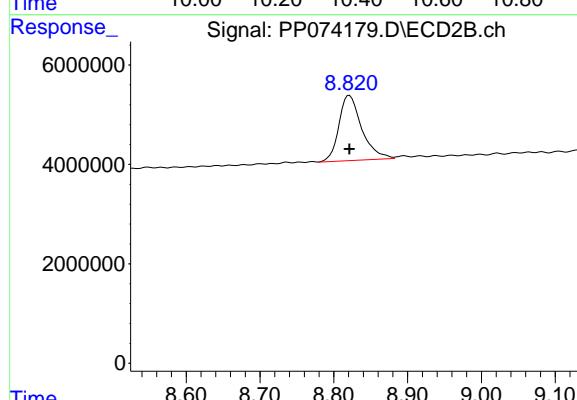

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: 0.000 min
Response: 28194628
Conc: 4.60 ng/ml

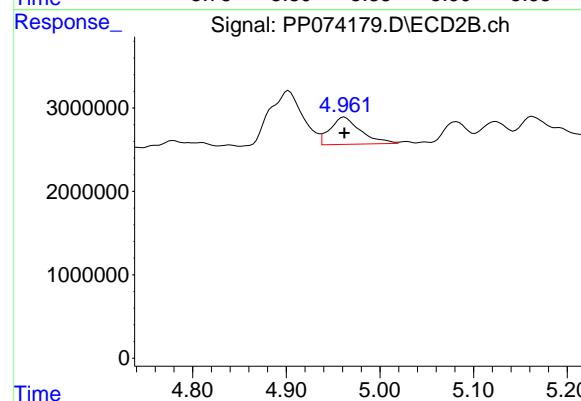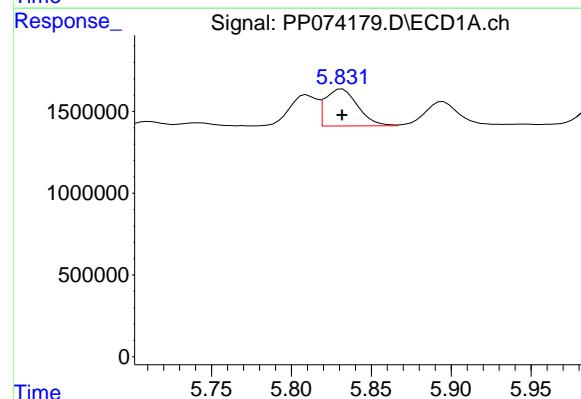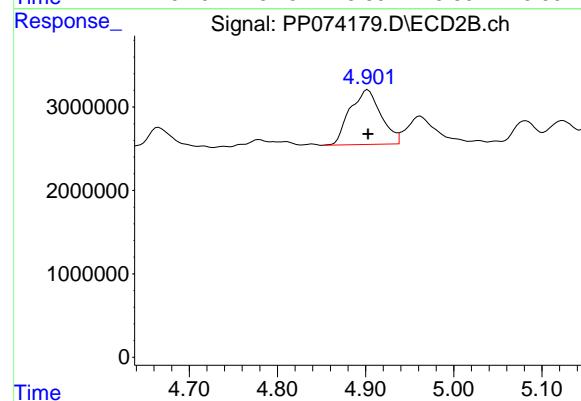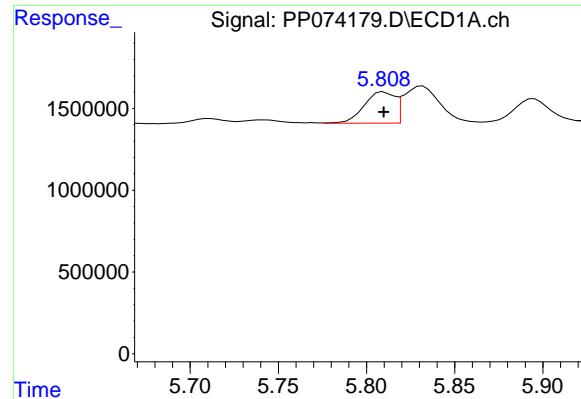





#16 AR-1242-1

R.T.: 5.810 min
 Delta R.T.: 0.000 min
 Response: 2289125
 Conc: 61.43 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

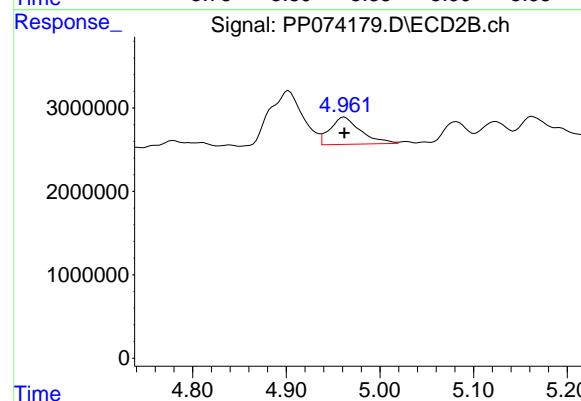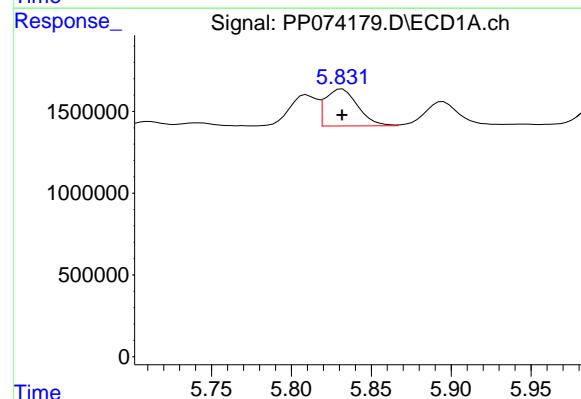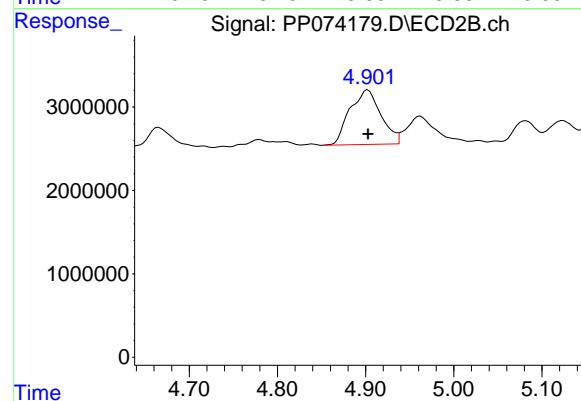

#18 AR-1242-3

R.T.: 5.895 min
 Delta R.T.: 0.000 min
 Response: 2169957
 Conc: 60.72 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#18 AR-1242-3





R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 4094869
 Conc: 44.39 ng/ml


#19 AR-1242-4

R.T.: 5.991 min
 Delta R.T.: 0.000 min
 Response: 1732044
 Conc: 59.28 ng/ml

#19 AR-1242-4

R.T.: 5.163 min
 Delta R.T.: 0.000 min
 Response: 5803584
 Conc: 48.60 ng/ml

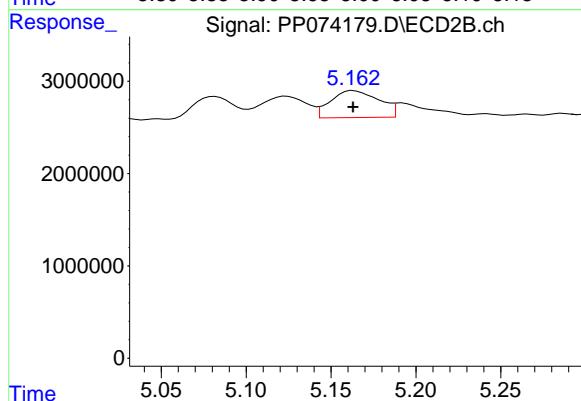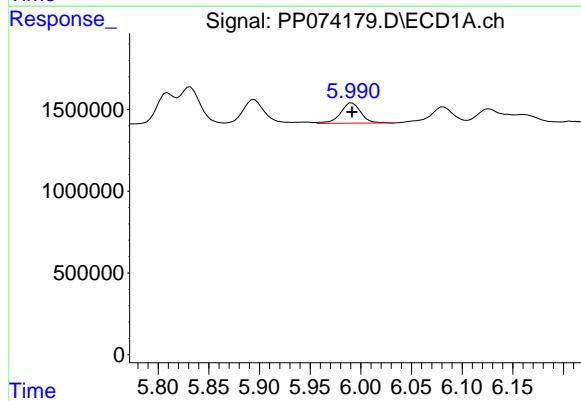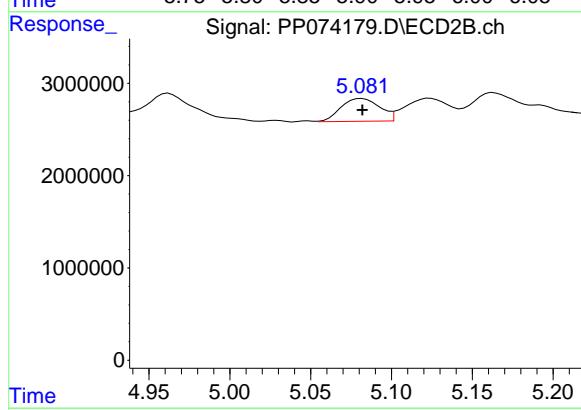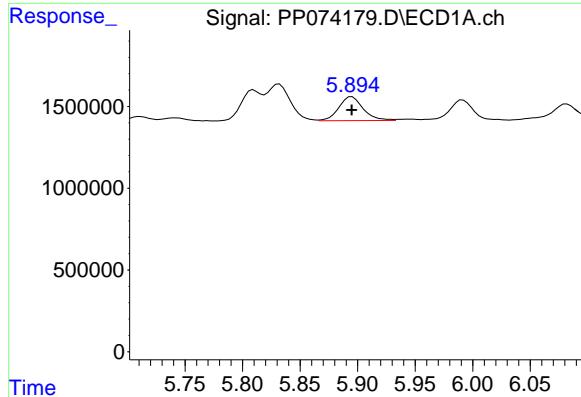

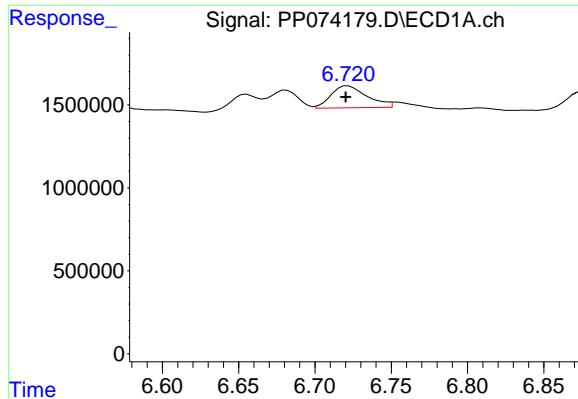


#20 AR-1242-5

R.T.: 6.720 min
 Delta R.T.: 0.000 min
 Response: 2173540
 Conc: 56.36 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

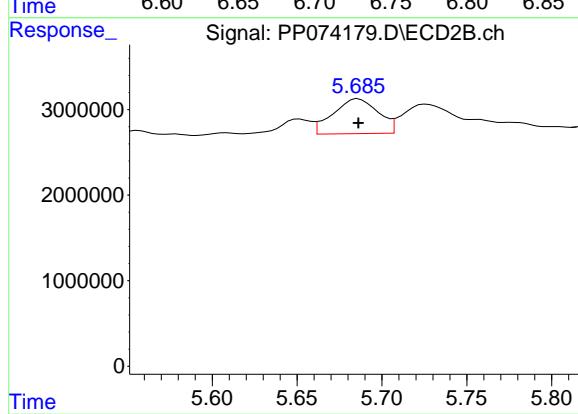

#20 AR-1242-5

R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 7539678
 Conc: 50.41 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 16:57
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 23:35:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 23:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.660 | 3.805 | 54922987 | 197.2E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.433 | 8.824 | 48401219 | 304.7E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 21) L5 AR-1248-1 | 5.810 | 4.903 | 14191296 | 111.8E6 | 500.000 | 500.000 |
| 22) L5 AR-1248-2 | 6.082 | 5.124 | 20093773 | 73885161 | 500.000 | 500.000 |
| 23) L5 AR-1248-3 | 6.284 | 5.164 | 22320416 | 89773071 | 500.000 | 477.333m |
| 24) L5 AR-1248-4 | 6.682 | 5.338 | 25791080 | 83528426 | 500.000 | 500.000 |
| 25) L5 AR-1248-5 | 6.721 | 5.727 | 26620059 | 151.4E6 | 500.000 | 500.000 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 16:57
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 23:35:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 23:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1248ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

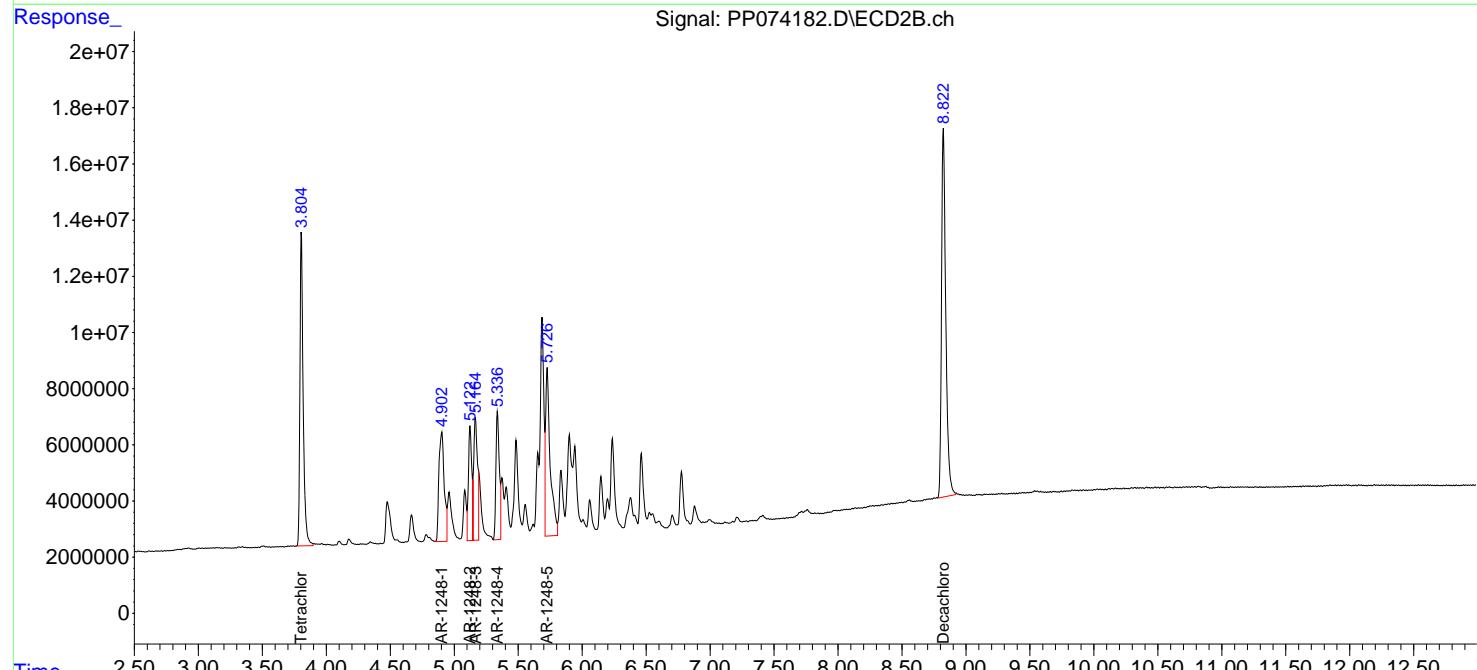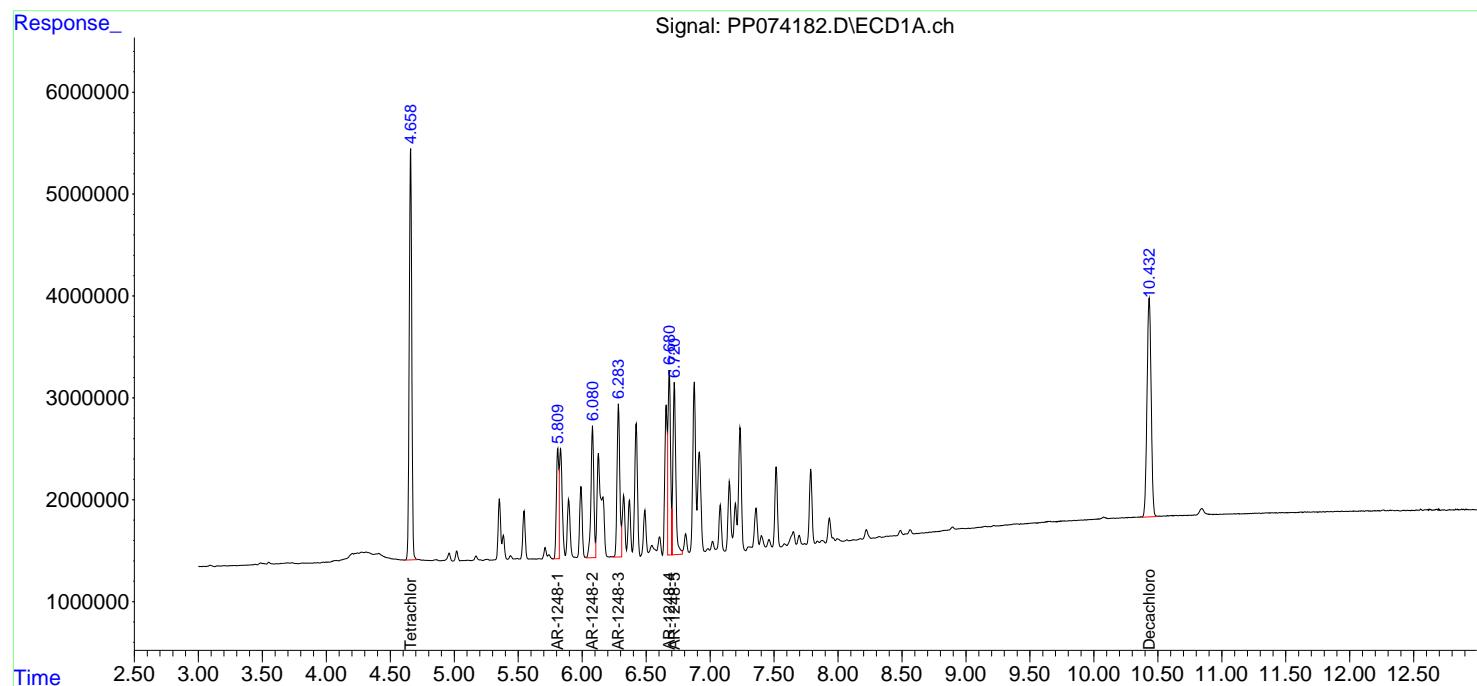

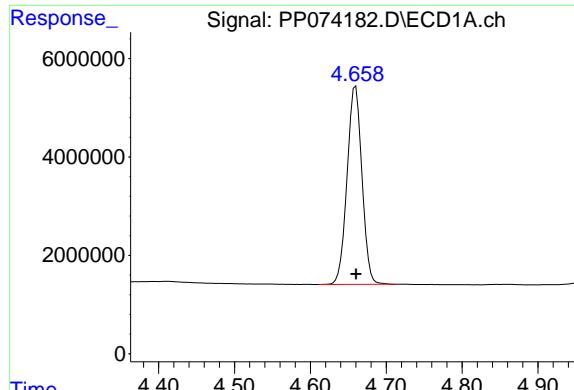


#1 Tetrachloro-m-xylene

R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 54922987
Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

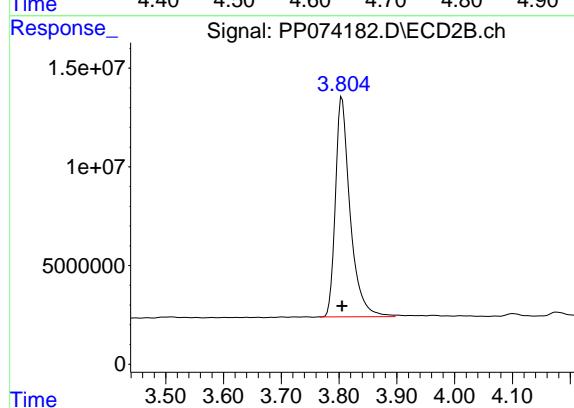


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 197242850
Conc: 50.00 ng/ml

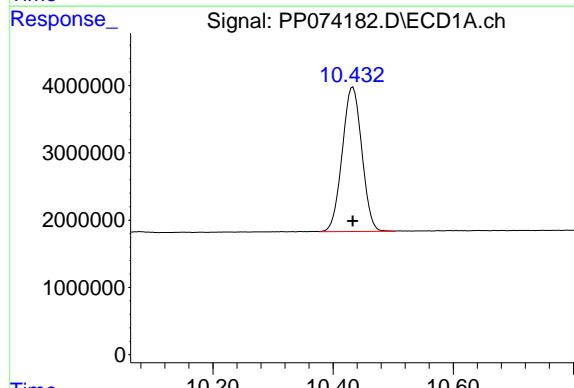


#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.000 min
Response: 48401219
Conc: 50.00 ng/ml

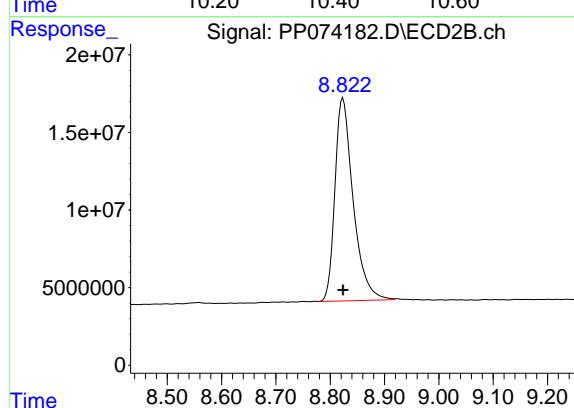

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 304735949
Conc: 50.00 ng/ml

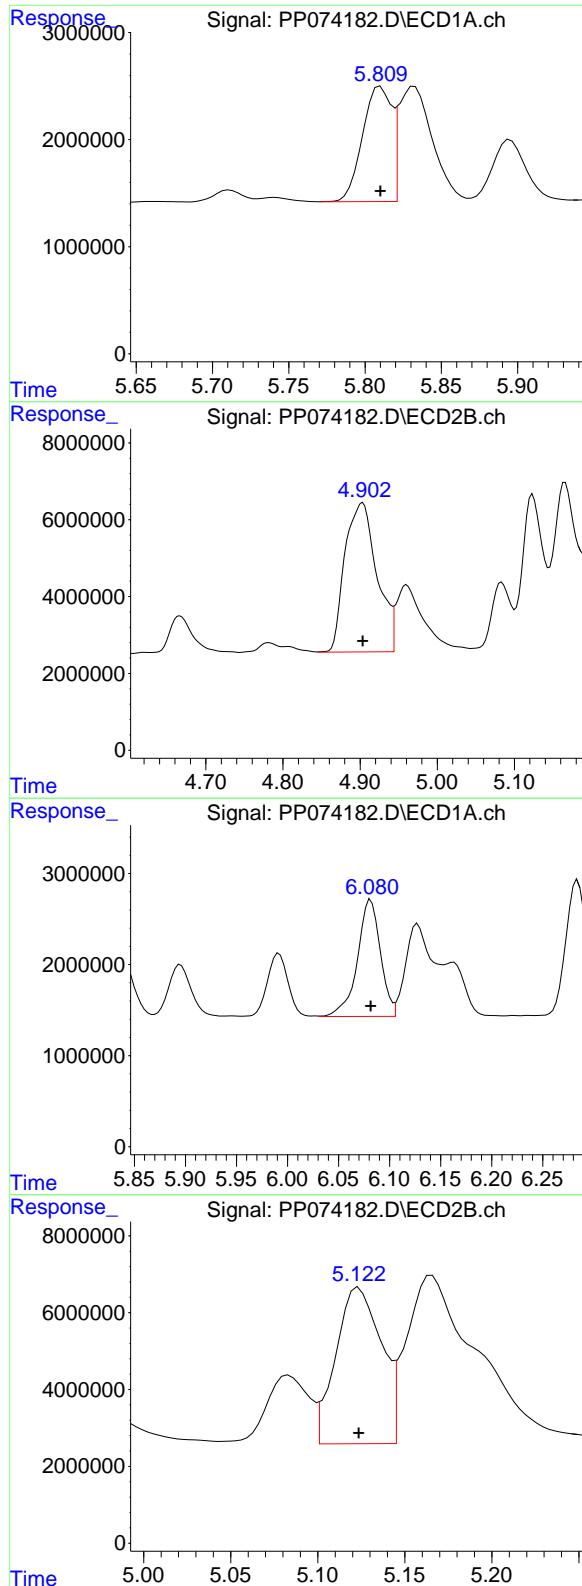

#21 AR-1248-1

R.T.: 5.810 min
 Delta R.T.: 0.000 min
 Response: 14191296
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#21 AR-1248-1


R.T.: 4.903 min
 Delta R.T.: 0.000 min
 Response: 111814459
 Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 20093773
 Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 5.124 min
 Delta R.T.: 0.000 min
 Response: 73885161
 Conc: 500.00 ng/ml




#23 AR-1248-3

R.T.: 6.284 min
 Delta R.T.: 0.000 min
 Response: 22320416
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

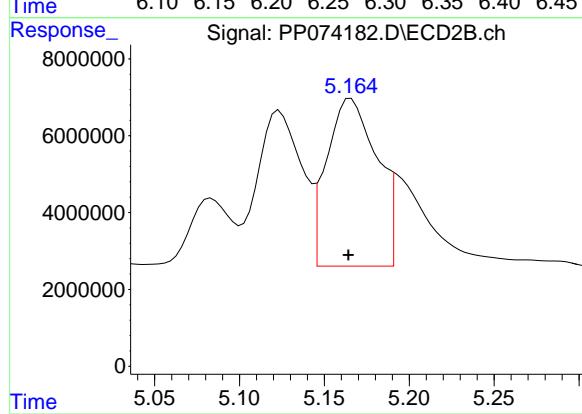


#23 AR-1248-3

R.T.: 5.164 min
 Delta R.T.: 0.000 min
 Response: 89773071
 Conc: 477.33 ng/ml

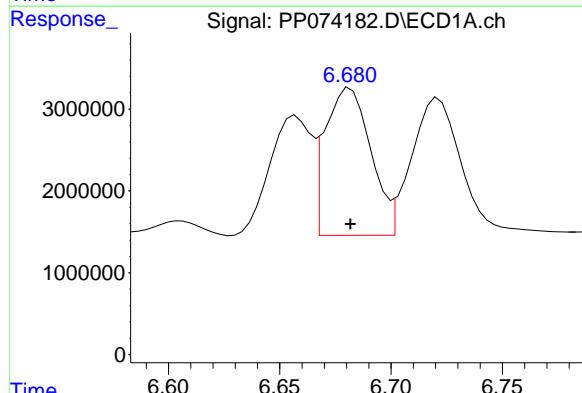

#24 AR-1248-4

R.T.: 6.682 min
 Delta R.T.: 0.000 min
 Response: 25791080
 Conc: 500.00 ng/ml

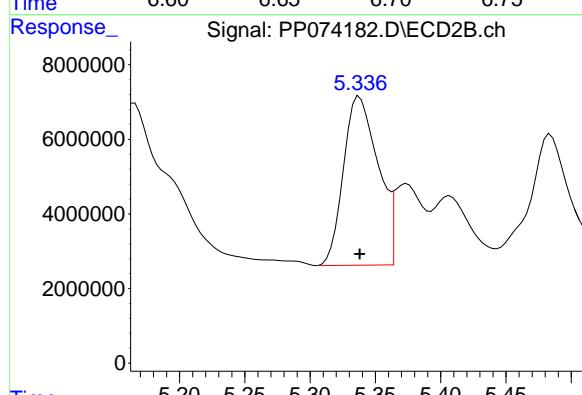

#24 AR-1248-4

R.T.: 5.338 min
 Delta R.T.: 0.000 min
 Response: 83528426
 Conc: 500.00 ng/ml



#25 AR-1248-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 26620059
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1248ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

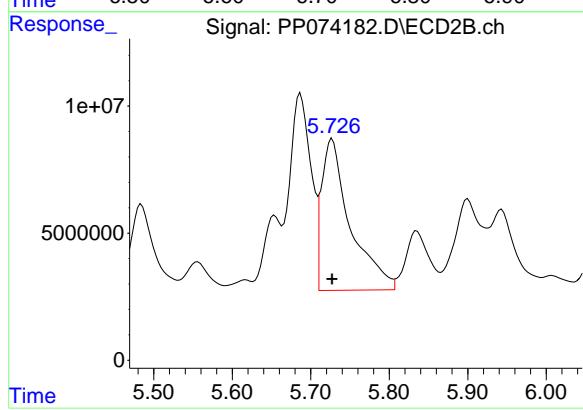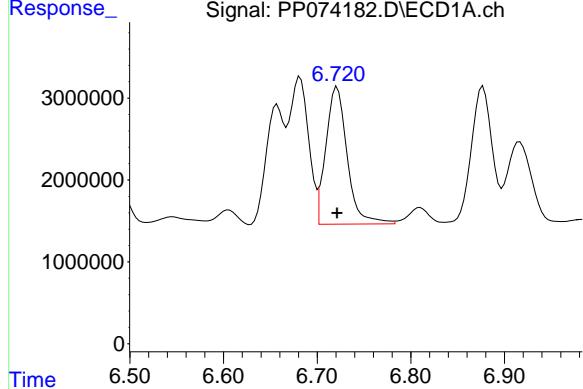

#25 AR-1248-5

R.T.: 5.727 min
 Delta R.T.: 0.000 min
 Response: 151391354
 Conc: 500.00 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:02
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|---------|
| 1) SA Tetrachlor... | 4.660 | 3.805 | 105.5E6 | 435.9E6 | 94.708 | 107.891 |
| 2) SA Decachlor... | 10.433 | 8.824 | 90161394 | 620.7E6 | 92.084 | 101.439 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|-----------|
| 26) L6 AR-1254-1 | 6.658 | 5.689 | 49559228 | 384.6E6 | 913.982m | 998.639 |
| 27) L6 AR-1254-2 | 6.875 | 5.835 | 70079706 | 284.4E6 | 896.542 | 1000.895 |
| 28) L6 AR-1254-3 | 7.237 | 6.238 | 76495408 | 520.2E6 | 905.487 | 1022.453 |
| 29) L6 AR-1254-4 | 7.518 | 6.464 | 57834344 | 378.1E6 | 911.799 | 1002.531 |
| 30) L6 AR-1254-5 | 7.934 | 6.880 | 73335985 | 425.1E6 | 909.260 | 1067.360m |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:02
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1254ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

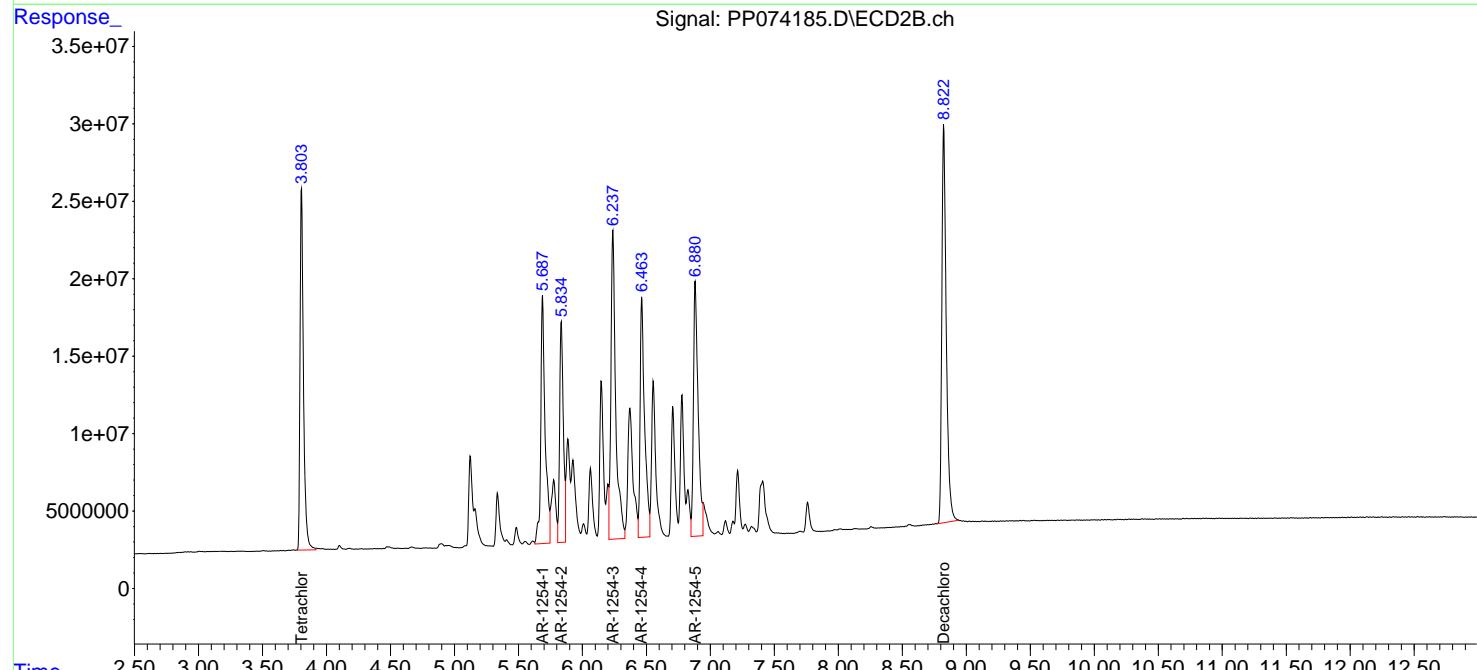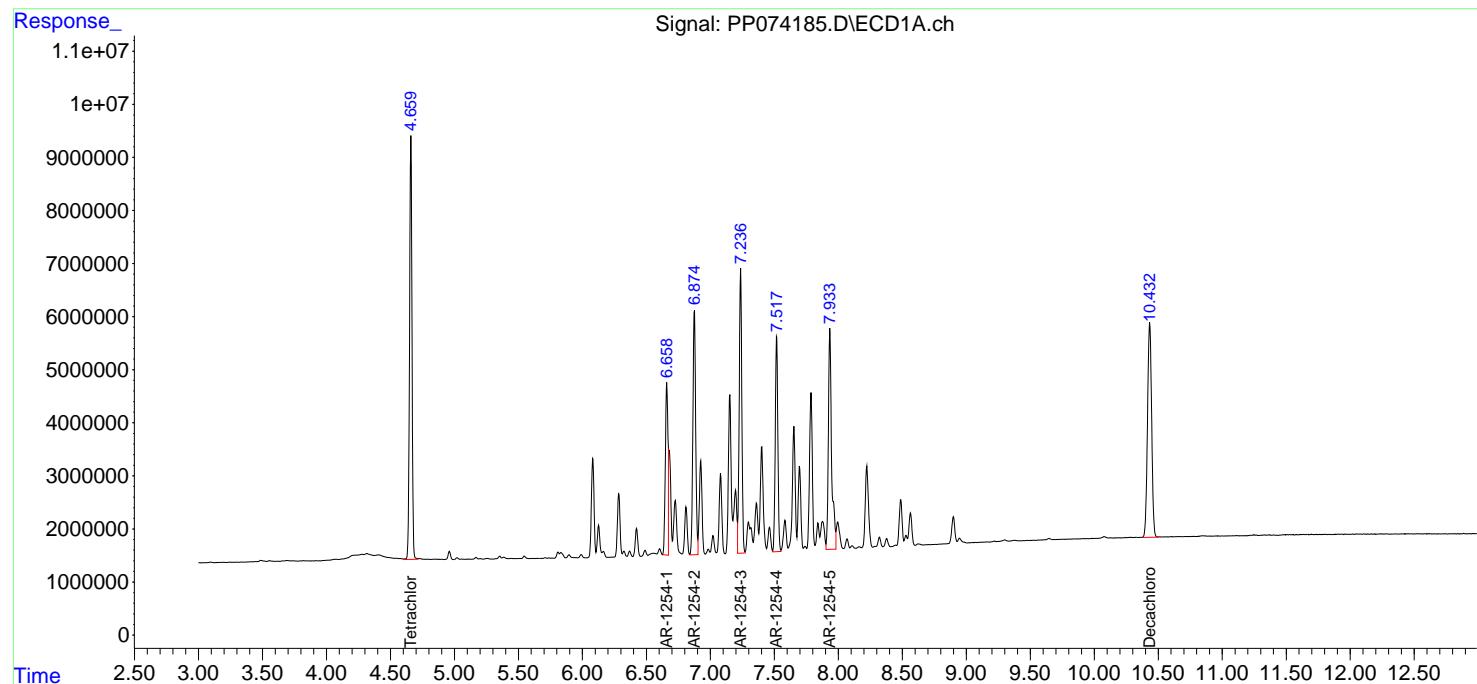

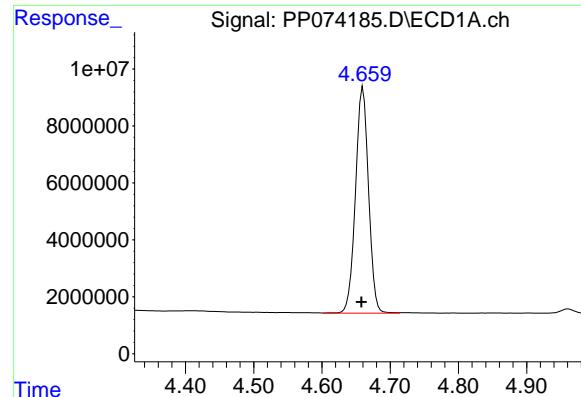


#1 Tetrachloro-m-xylene

R.T.: 4.660 min
Delta R.T.: 0.002 min
Response: 105531811
Conc: 94.71 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC1000


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

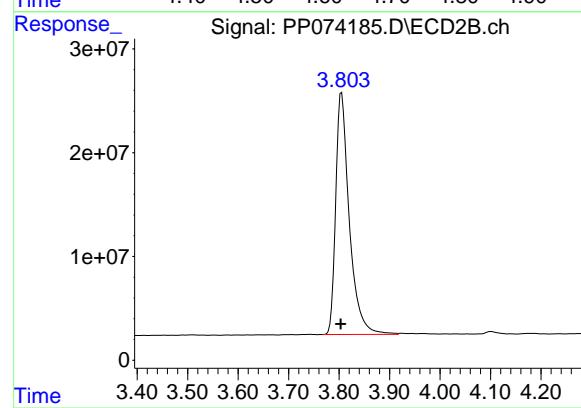


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.002 min
Response: 435882815
Conc: 107.89 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.001 min
Response: 90161394
Conc: 92.08 ng/ml

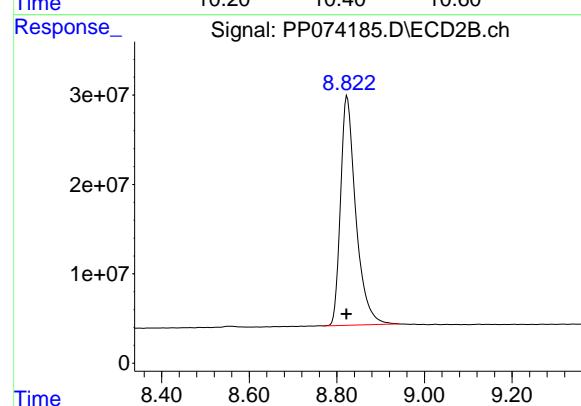

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.002 min
Response: 620683272
Conc: 101.44 ng/ml

#26 AR-1254-1

R.T.: 6.658 min
 Delta R.T.: 0.001 min
 Response: 49559228
 Conc: 913.98 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#26 AR-1254-1





R.T.: 5.689 min
 Delta R.T.: 0.001 min
 Response: 384557283
 Conc: 998.64 ng/ml


#27 AR-1254-2

R.T.: 6.875 min
 Delta R.T.: 0.002 min
 Response: 70079706
 Conc: 896.54 ng/ml

#27 AR-1254-2

R.T.: 5.835 min
 Delta R.T.: 0.001 min
 Response: 284389782
 Conc: 1000.89 ng/ml

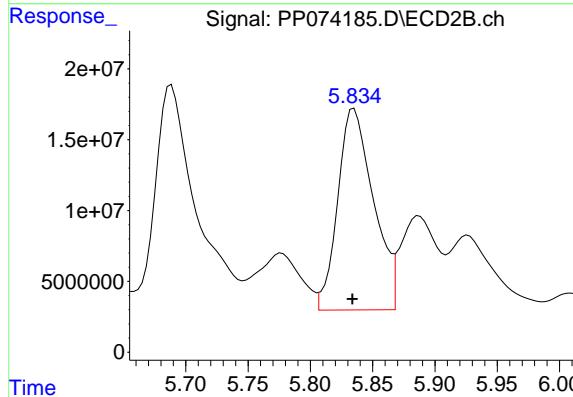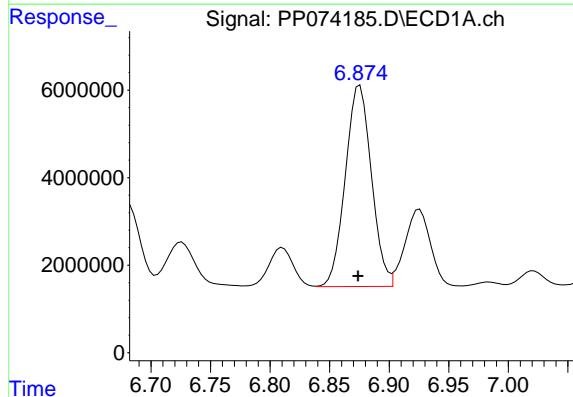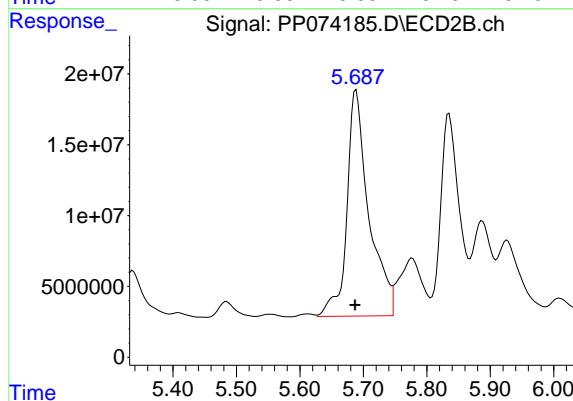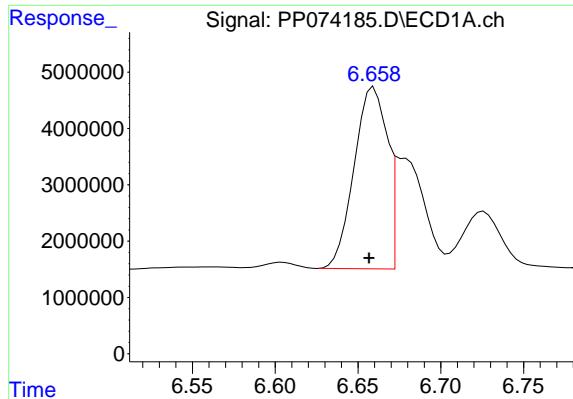

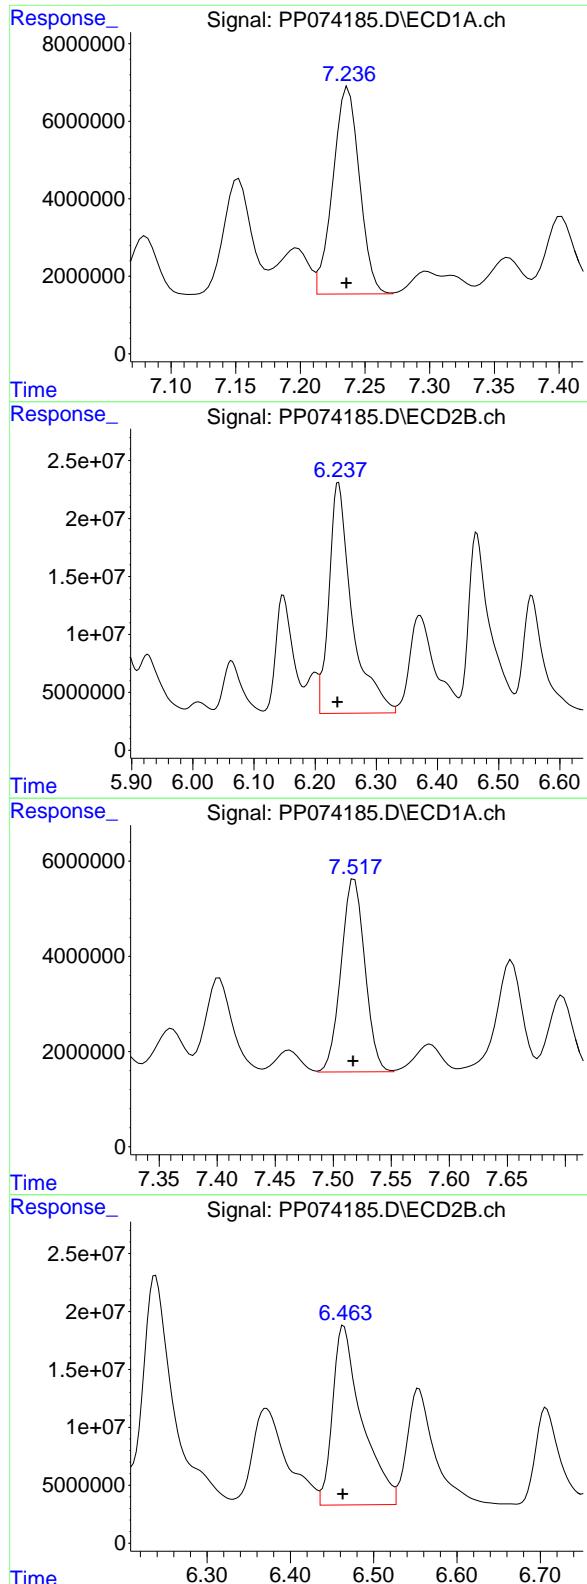

#28 AR-1254-3

R.T.: 7.237 min
 Delta R.T.: 0.002 min
 Response: 76495408
 Conc: 905.49 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#28 AR-1254-3

R.T.: 6.238 min
 Delta R.T.: 0.002 min
 Response: 520239168
 Conc: 1022.45 ng/ml


#29 AR-1254-4

R.T.: 7.518 min
 Delta R.T.: 0.001 min
 Response: 57834344
 Conc: 911.80 ng/ml

#29 AR-1254-4

R.T.: 6.464 min
 Delta R.T.: 0.001 min
 Response: 378053305
 Conc: 1002.53 ng/ml

#30 AR-1254-5

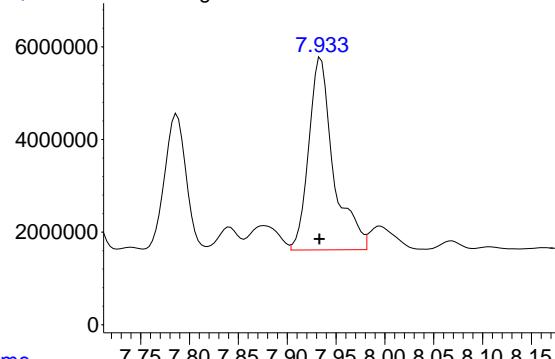

R.T.: 7.934 min
Delta R.T.: 0.002 min
Response: 73335985
Conc: 909.26 ng/ml


Instrument: ECD_P
ClientSampleId: AR1254ICC1000

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

#30 AR-1254-5

R.T.: 6.880 min
Delta R.T.: 0.000 min
Response: 425051302
Conc: 1067.36 ng/ml

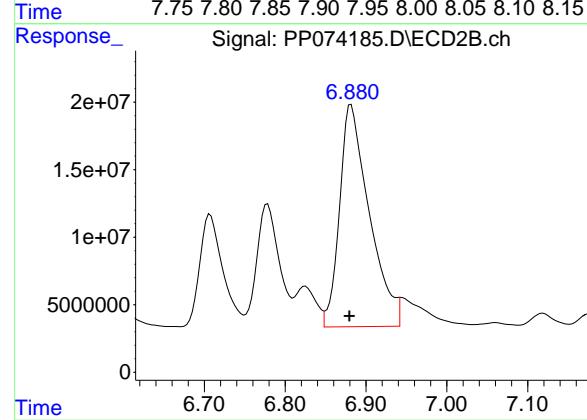

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:18
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.659 | 3.804 | 80274871 | 316.5E6 | 72.041 | 78.350 |
| 2) SA Decachlor... | 10.433 | 8.823 | 69679431 | 463.5E6 | 71.165 | 75.743 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|---------|
| 26) L6 AR-1254-1 | 6.657 | 5.688 | 37358301 | 271.1E6 | 688.970m | 703.976 |
| 27) L6 AR-1254-2 | 6.874 | 5.835 | 54514978 | 207.5E6 | 697.420 | 730.114 |
| 28) L6 AR-1254-3 | 7.236 | 6.237 | 59505451 | 390.5E6 | 704.374 | 767.509 |
| 29) L6 AR-1254-4 | 7.517 | 6.464 | 44944937 | 292.2E6 | 708.589 | 774.901 |
| 30) L6 AR-1254-5 | 7.933 | 6.881 | 57058661 | 308.2E6 | 707.445 | 773.995 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:18
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC750

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

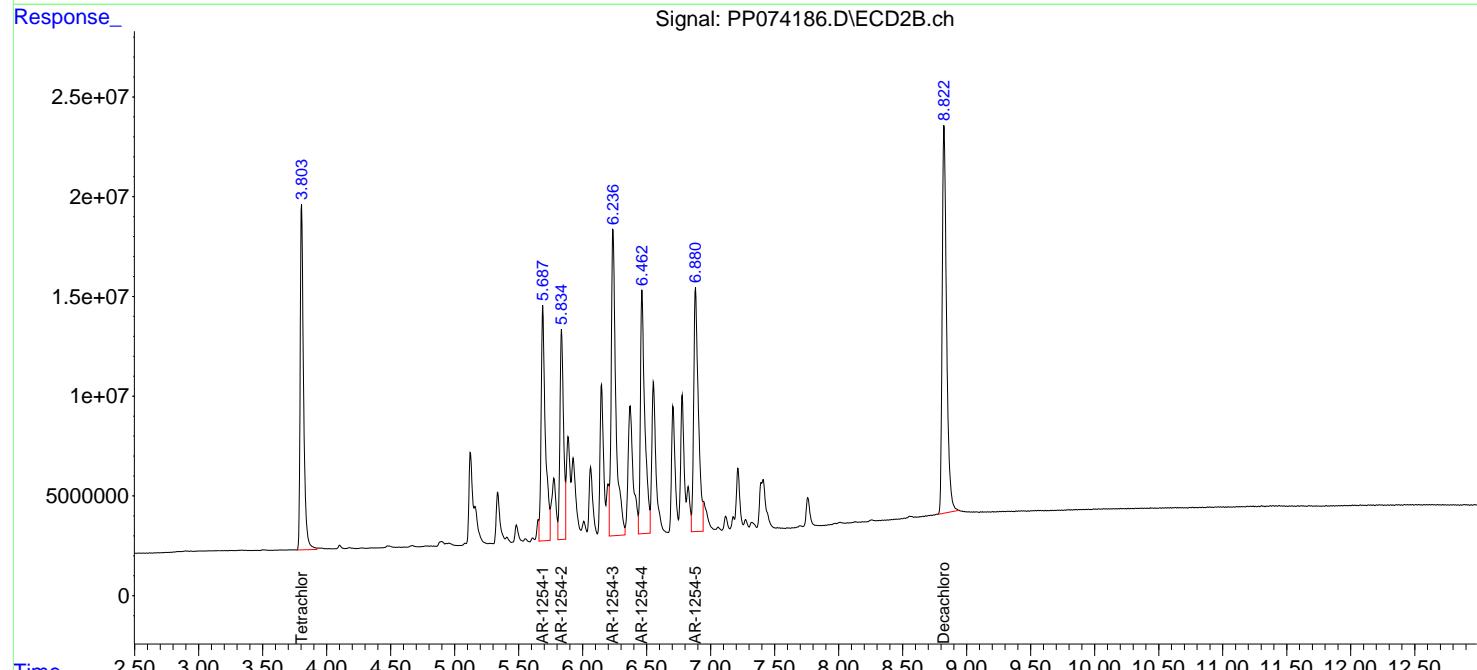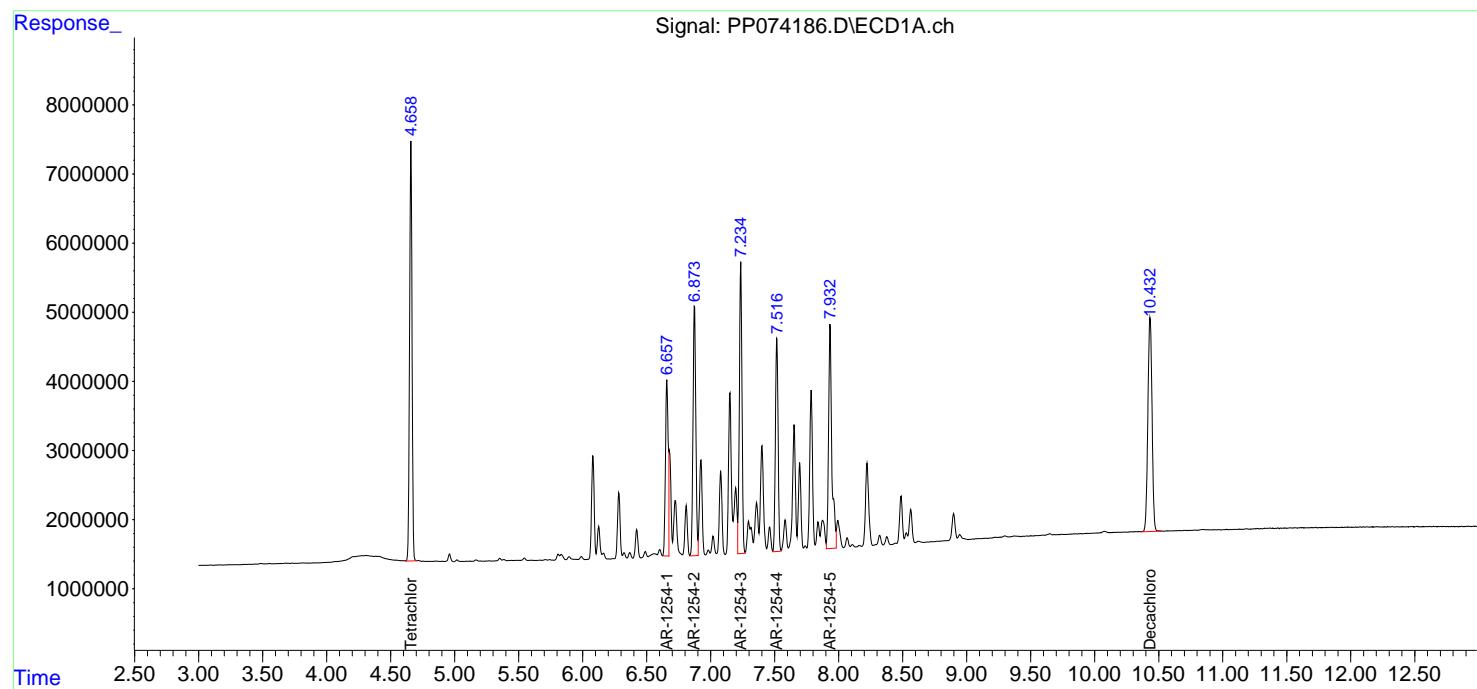

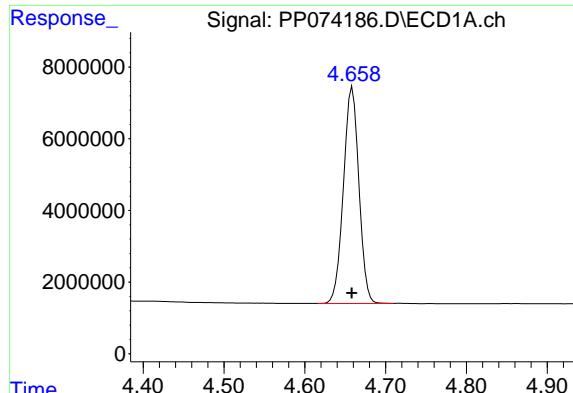


#1 Tetrachloro-m-xylene

R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 80274871
Conc: 72.04 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

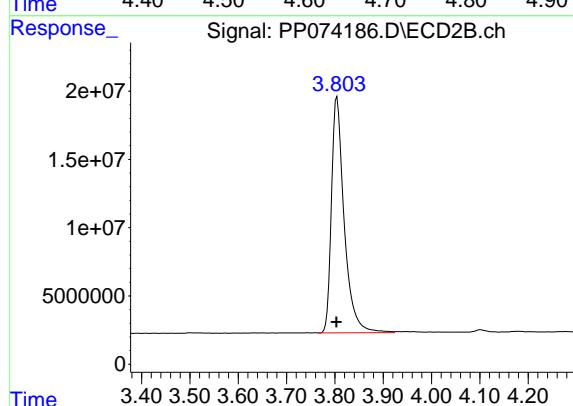


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.001 min
Response: 316536494
Conc: 78.35 ng/ml

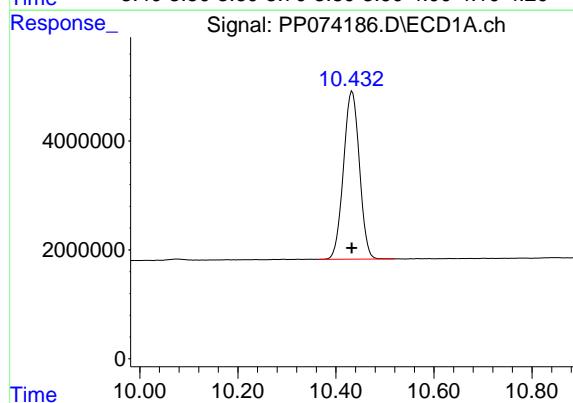

#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.000 min
Response: 69679431
Conc: 71.17 ng/ml

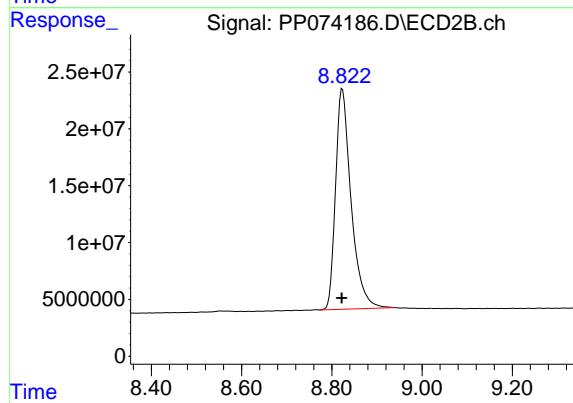

#2 Decachlorobiphenyl

R.T.: 8.823 min
Delta R.T.: 0.001 min
Response: 463453835
Conc: 75.74 ng/ml





#26 AR-1254-1

R.T.: 6.657 min
 Delta R.T.: 0.000 min
 Response: 37358301
 Conc: 688.97 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

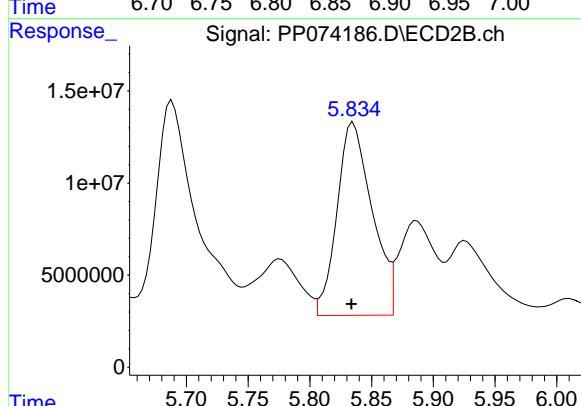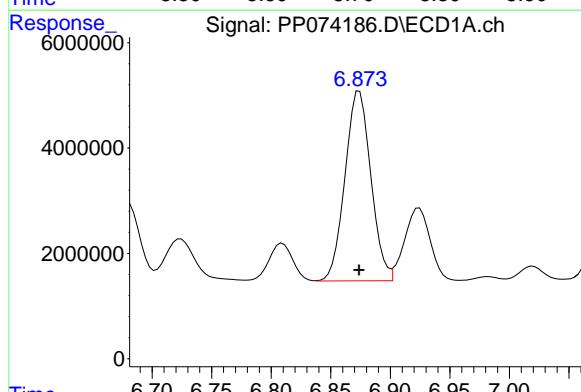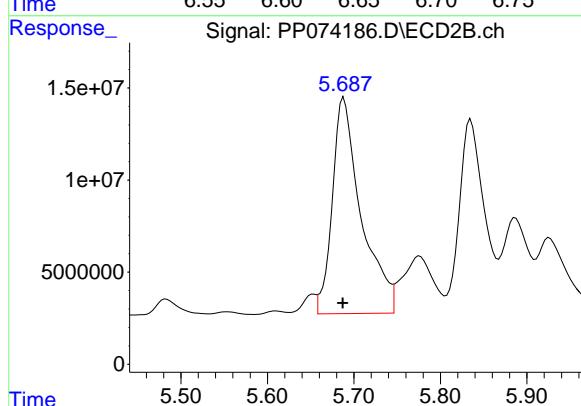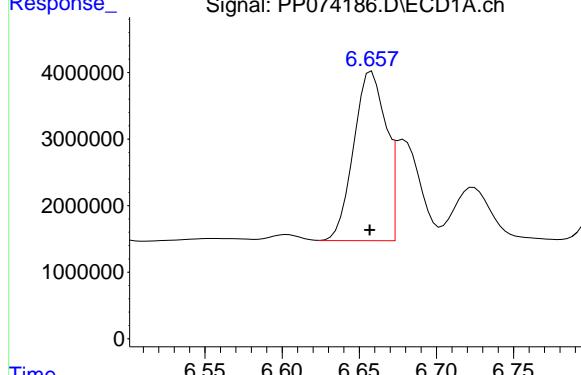

#26 AR-1254-1


R.T.: 5.688 min
 Delta R.T.: 0.001 min
 Response: 271087969
 Conc: 703.98 ng/ml

#27 AR-1254-2

R.T.: 6.874 min
 Delta R.T.: 0.000 min
 Response: 54514978
 Conc: 697.42 ng/ml

#27 AR-1254-2

R.T.: 5.835 min
 Delta R.T.: 0.001 min
 Response: 207451389
 Conc: 730.11 ng/ml

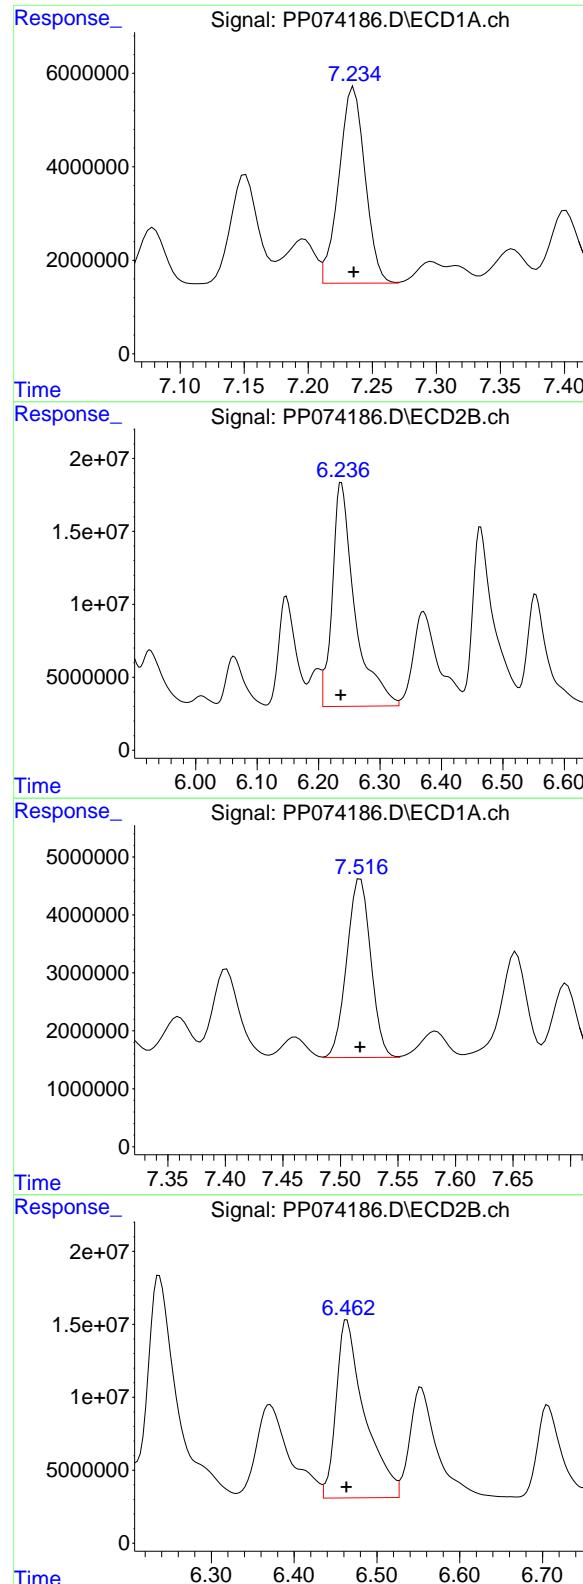

#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: 0.000 min
 Response: 59505451
 Conc: 704.37 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#28 AR-1254-3

R.T.: 6.237 min
 Delta R.T.: 0.000 min
 Response: 390519824
 Conc: 767.51 ng/ml

#29 AR-1254-4

R.T.: 7.517 min
 Delta R.T.: 0.000 min
 Response: 44944937
 Conc: 708.59 ng/ml

#29 AR-1254-4

R.T.: 6.464 min
 Delta R.T.: 0.000 min
 Response: 292214490
 Conc: 774.90 ng/ml

#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: 0.000 min
 Response: 57058661
 Conc: 707.44 ng/ml


Instrument: ECD_P
ClientSampleId: AR1254ICC750

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#30 AR-1254-5

R.T.: 6.881 min
 Delta R.T.: 0.002 min
 Response: 308225641
 Conc: 774.00 ng/ml

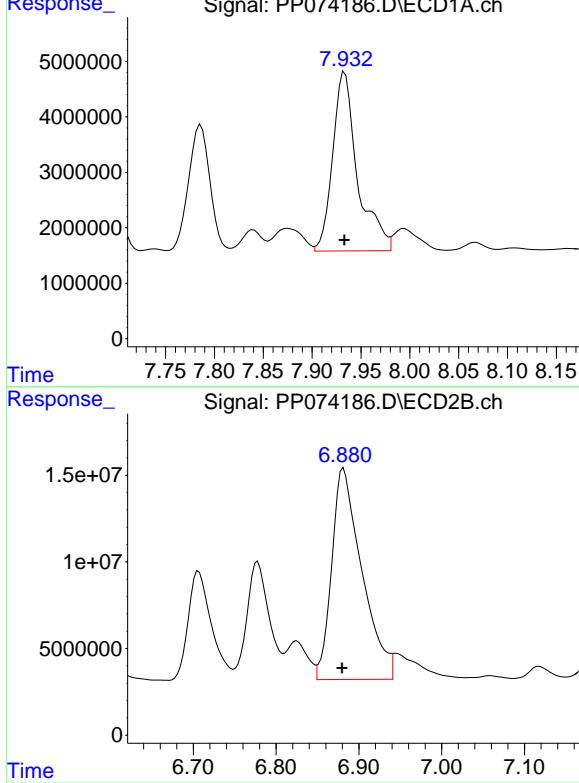

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:34
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 55714538 | 202.0E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.432 | 8.822 | 48956102 | 305.9E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|---------|
| 26) L6 AR-1254-1 | 6.657 | 5.687 | 26953630 | 192.5E6 | 497.085m | 500.000 |
| 27) L6 AR-1254-2 | 6.874 | 5.834 | 39083346 | 142.1E6 | 500.000 | 500.000 |
| 28) L6 AR-1254-3 | 7.236 | 6.237 | 42239930 | 254.4E6 | 500.000 | 500.000 |
| 29) L6 AR-1254-4 | 7.517 | 6.463 | 31714402 | 188.5E6 | 500.000 | 500.000 |
| 30) L6 AR-1254-5 | 7.933 | 6.880 | 40327283 | 199.1E6 | 500.000 | 500.000 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:34
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

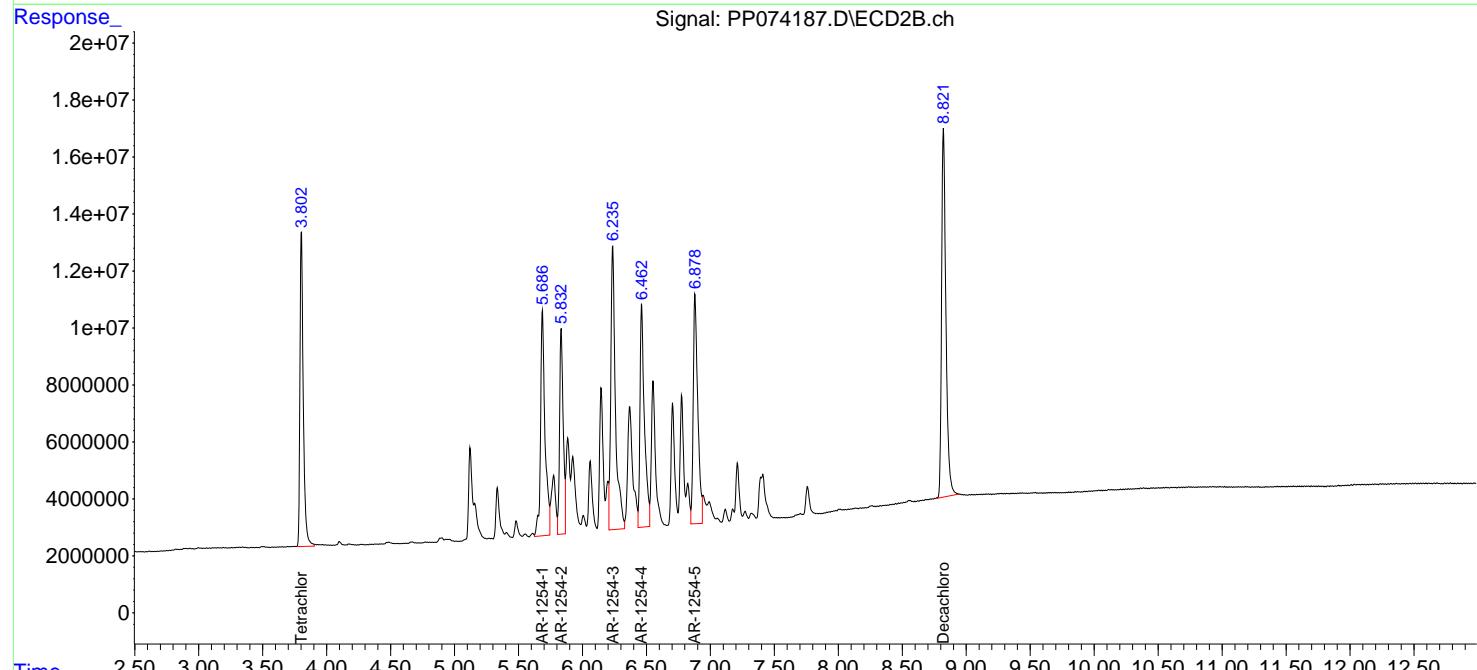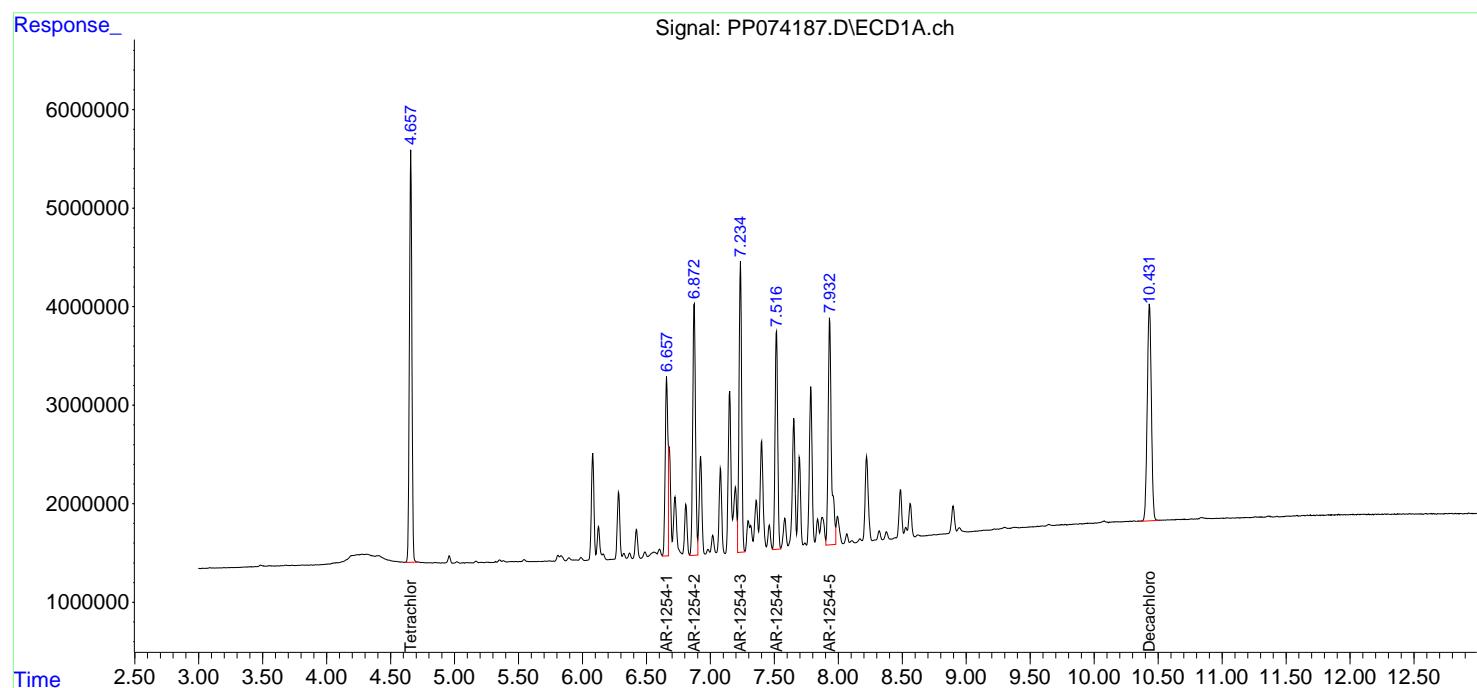

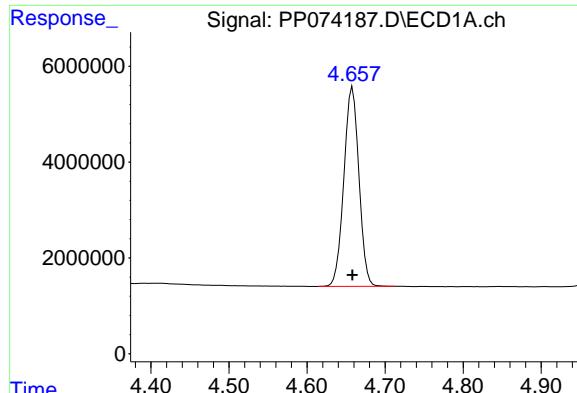


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: 0.000 min
Response: 55714538
Conc: 50.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

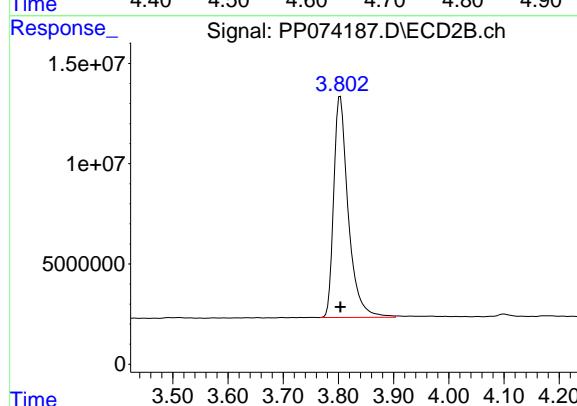


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 202001814
Conc: 50.00 ng/ml

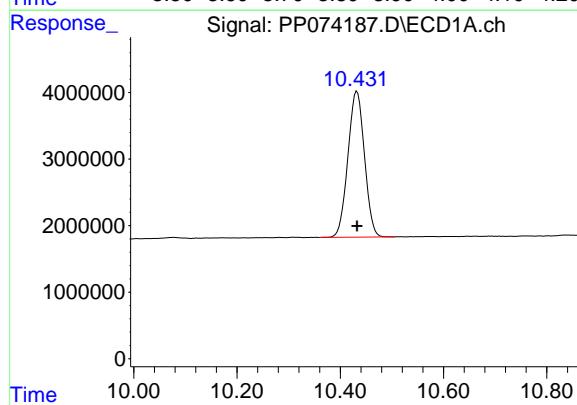

#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 48956102
Conc: 50.00 ng/ml

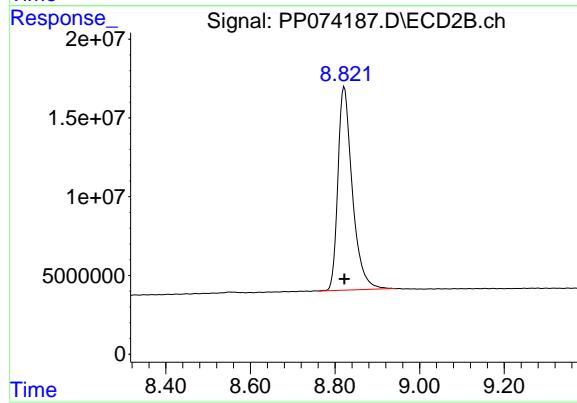

#2 Decachlorobiphenyl

R.T.: 8.822 min
Delta R.T.: 0.000 min
Response: 305938523
Conc: 50.00 ng/ml





#26 AR-1254-1

R.T.: 6.657 min
 Delta R.T.: 0.000 min
 Response: 26953630
 Conc: 497.08 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

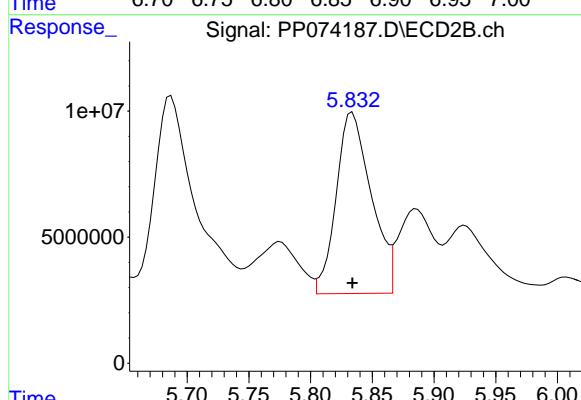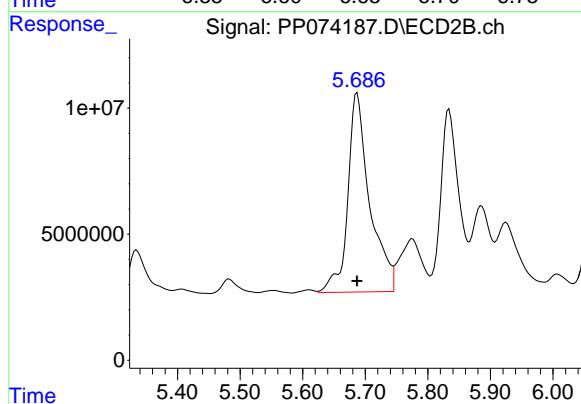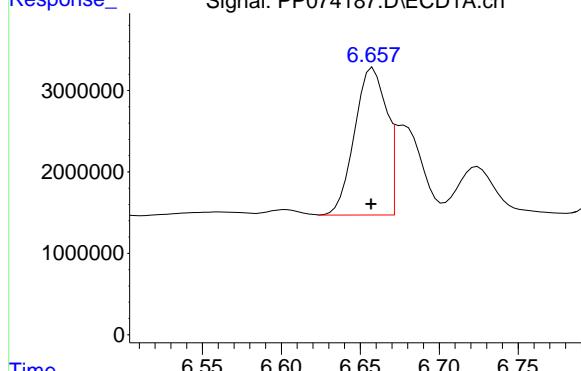

#26 AR-1254-1


R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 192540601
 Conc: 500.00 ng/ml

#27 AR-1254-2

R.T.: 6.874 min
 Delta R.T.: 0.000 min
 Response: 39083346
 Conc: 500.00 ng/ml

#27 AR-1254-2

R.T.: 5.834 min
 Delta R.T.: 0.000 min
 Response: 142067796
 Conc: 500.00 ng/ml

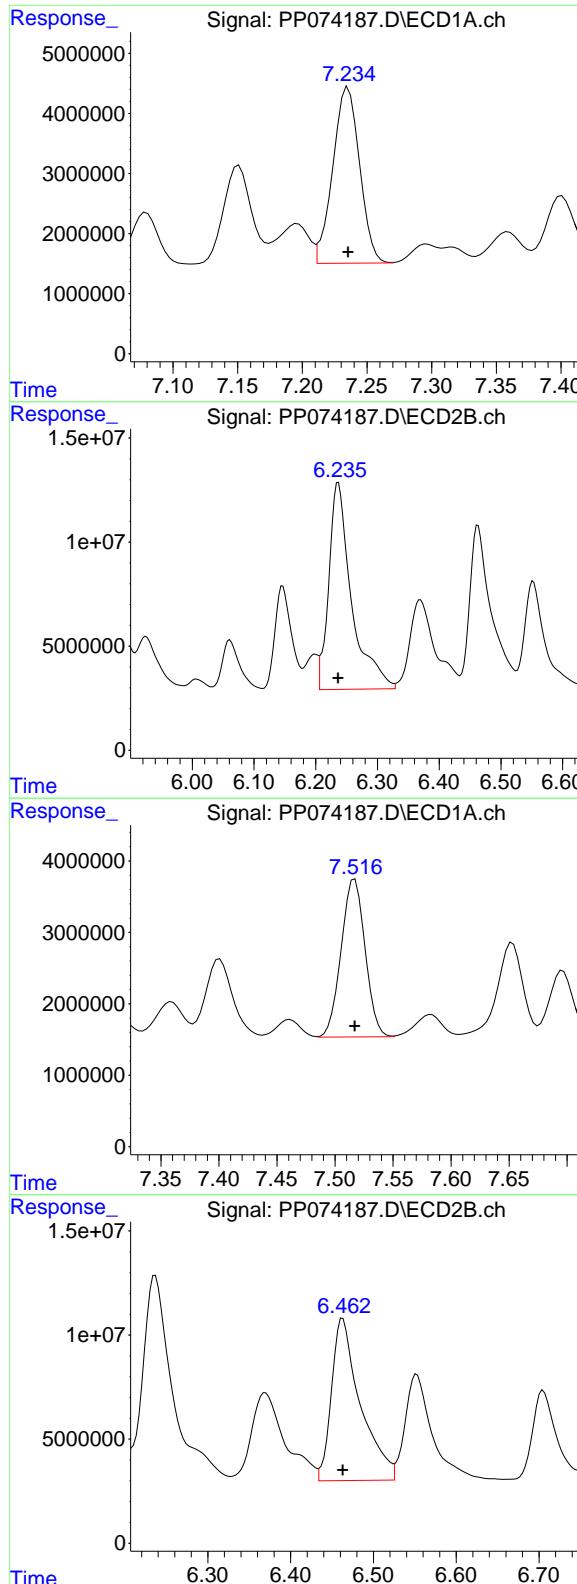

#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: 0.000 min
 Response: 42239930
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#28 AR-1254-3

R.T.: 6.237 min
 Delta R.T.: 0.000 min
 Response: 254407378
 Conc: 500.00 ng/ml


#29 AR-1254-4

R.T.: 7.517 min
 Delta R.T.: 0.000 min
 Response: 31714402
 Conc: 500.00 ng/ml

#29 AR-1254-4

R.T.: 6.463 min
 Delta R.T.: 0.000 min
 Response: 188549489
 Conc: 500.00 ng/ml

#30 AR-1254-5

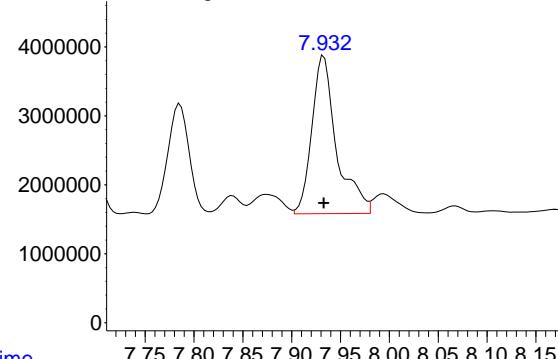

R.T.: 7.933 min
 Delta R.T.: 0.000 min
 Response: 40327283
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#30 AR-1254-5

R.T.: 6.880 min
 Delta R.T.: 0.000 min
 Response: 199113358
 Conc: 500.00 ng/ml

5

6

7

8

9

10

11

12

13

14

15

16

17

18

19

20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:50
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 29734018 | 92012238 | 26.684 | 22.775 |
| 2) SA Decachlor... | 10.431 | 8.821 | 26431747 | 157.0E6 | 26.995 | 25.657 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|---------|
| 26) L6 AR-1254-1 | 6.656 | 5.687 | 13498256 | 94373679 | 248.938m | 245.075 |
| 27) L6 AR-1254-2 | 6.873 | 5.834 | 21644264 | 72682229 | 276.899 | 255.801 |
| 28) L6 AR-1254-3 | 7.235 | 6.236 | 23355124 | 131.7E6 | 276.458 | 258.769 |
| 29) L6 AR-1254-4 | 7.516 | 6.462 | 17399794 | 98587777 | 274.320 | 261.437 |
| 30) L6 AR-1254-5 | 7.932 | 6.879 | 22010158 | 98393861 | 272.894 | 247.080 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:50
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1254ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

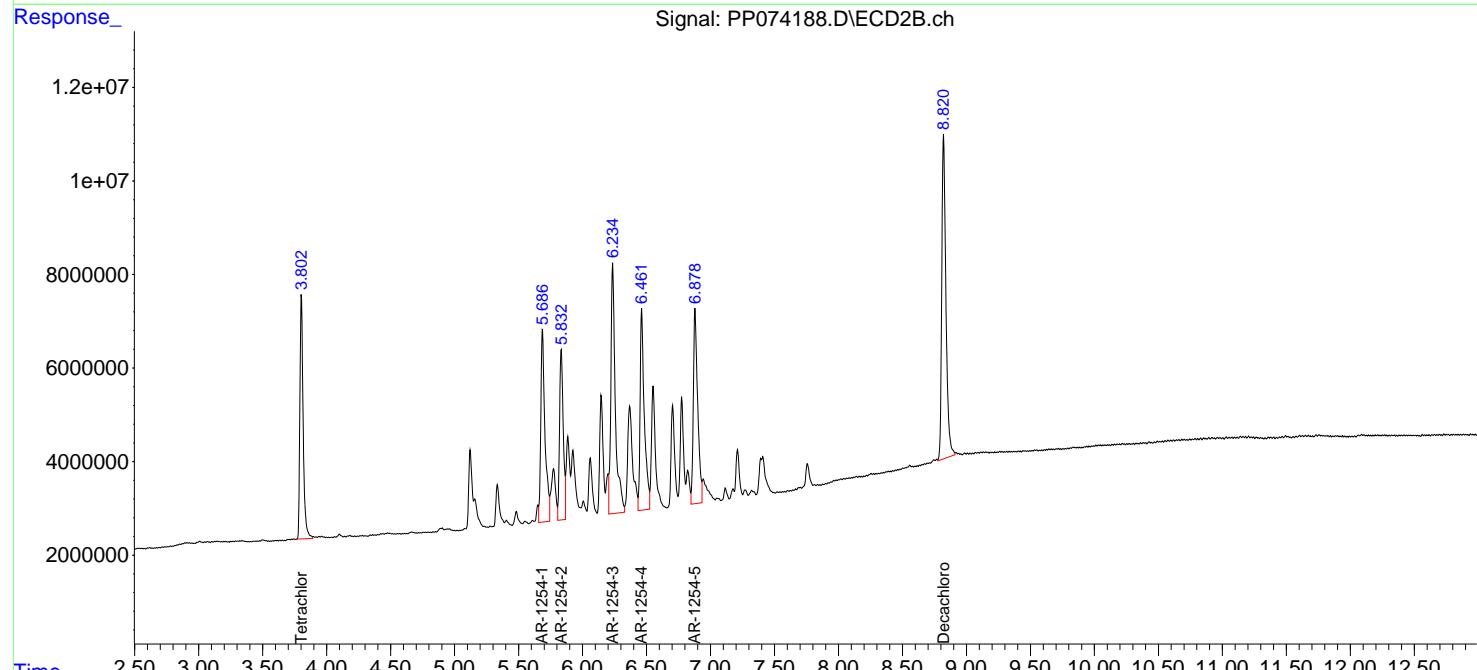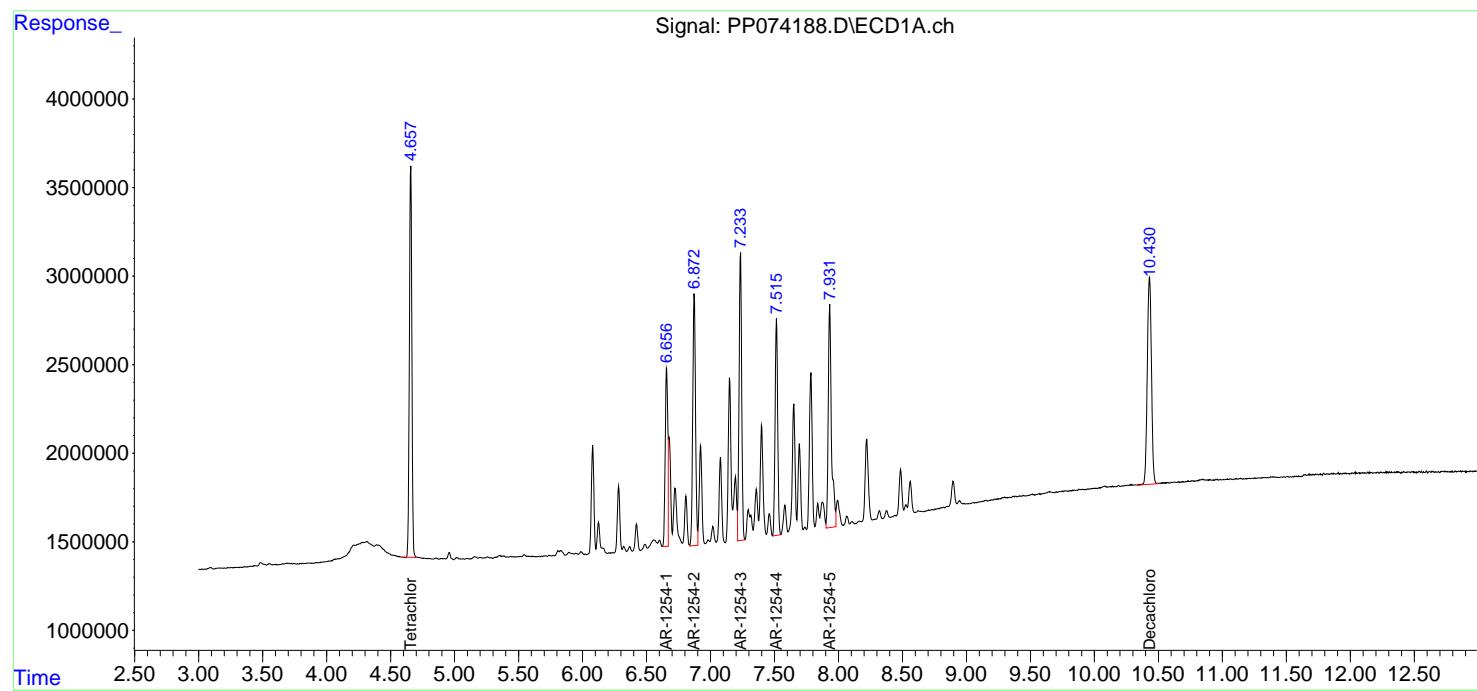

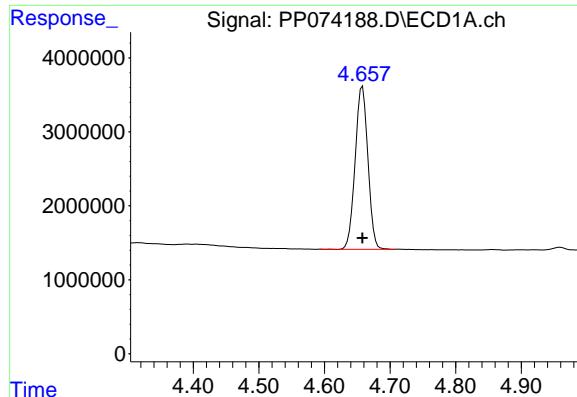


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: 0.000 min
Response: 29734018
Conc: 26.68 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

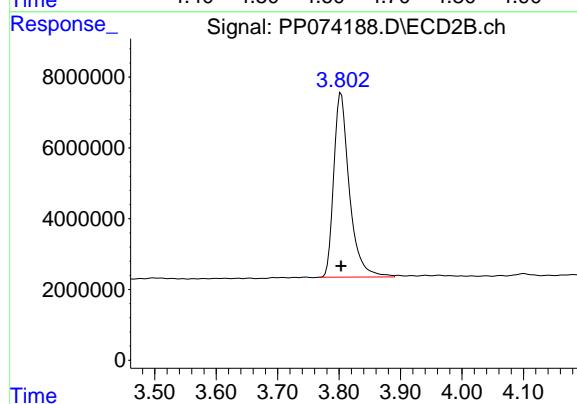


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 92012238
Conc: 22.78 ng/ml

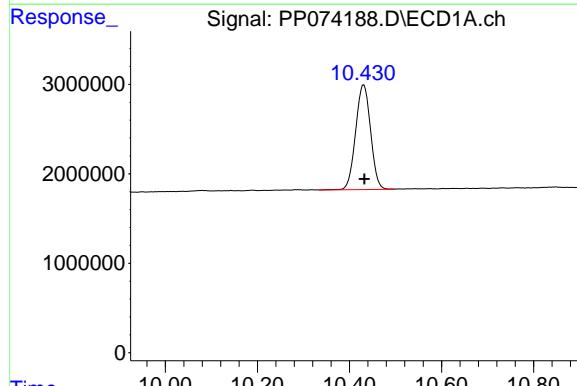

#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: -0.001 min
Response: 26431747
Conc: 27.00 ng/ml

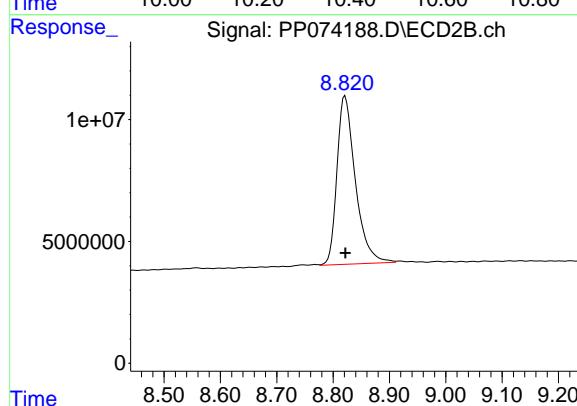

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: 0.000 min
Response: 156986884
Conc: 25.66 ng/ml

#26 AR-1254-1

R.T.: 6.656 min
 Delta R.T.: 0.000 min
 Response: 13498256
 Conc: 248.94 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#26 AR-1254-1





R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 94373679
 Conc: 245.07 ng/ml





#27 AR-1254-2

R.T.: 6.873 min
 Delta R.T.: 0.000 min
 Response: 21644264
 Conc: 276.90 ng/ml

#27 AR-1254-2

R.T.: 5.834 min
 Delta R.T.: 0.000 min
 Response: 72682229
 Conc: 255.80 ng/ml

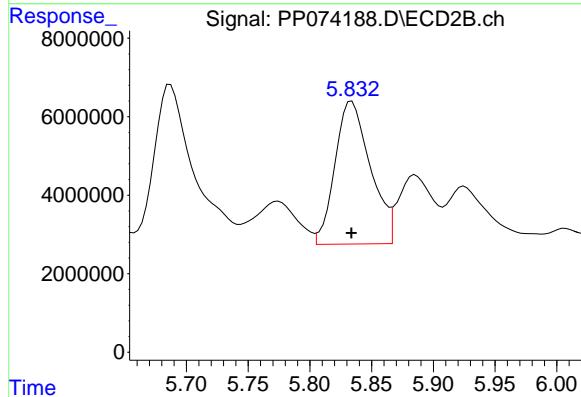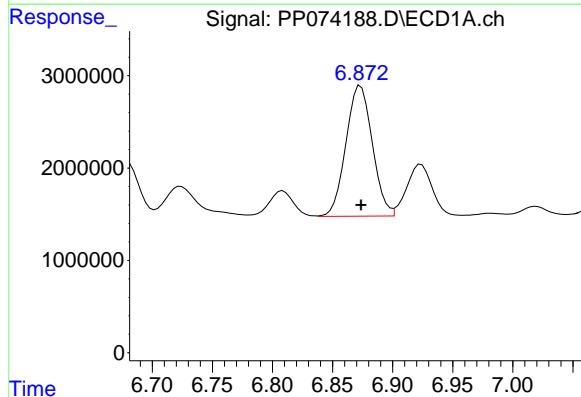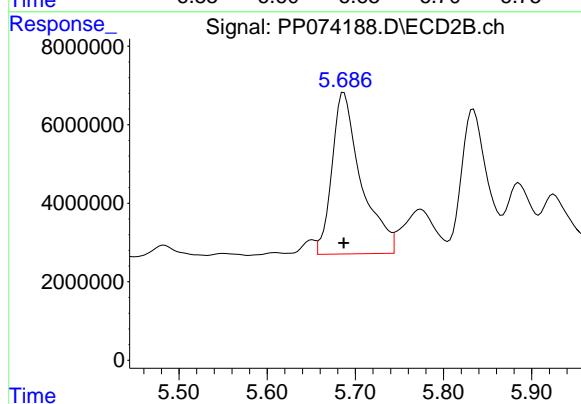

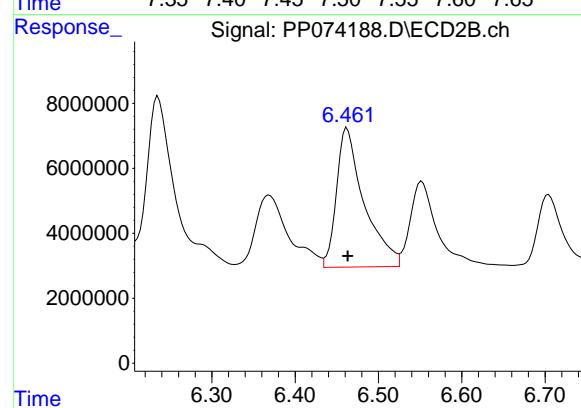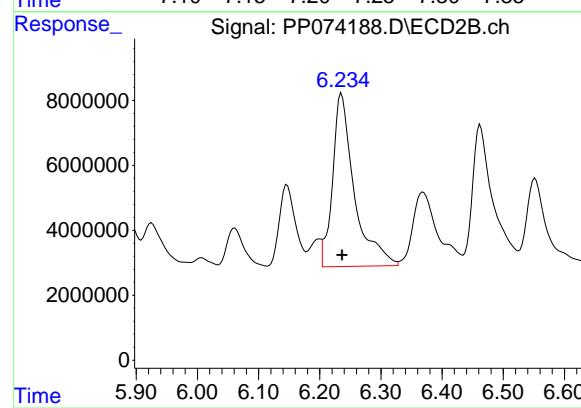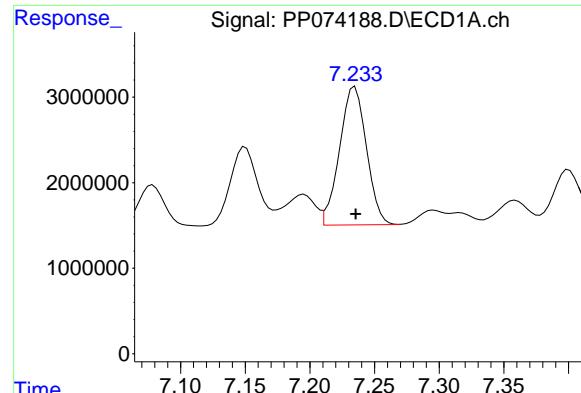




#28 AR-1254-3

R.T.: 7.235 min
 Delta R.T.: 0.000 min
 Response: 23355124
 Conc: 276.46 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

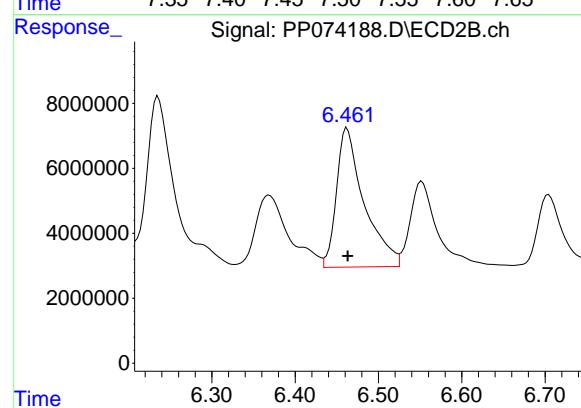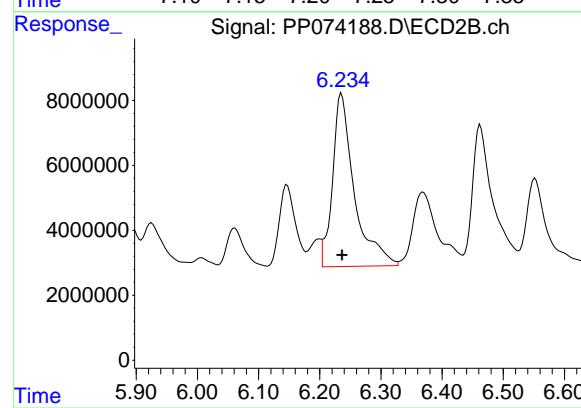

#28 AR-1254-3

R.T.: 6.236 min
 Delta R.T.: -0.001 min
 Response: 131665567
 Conc: 258.77 ng/ml

#29 AR-1254-4

R.T.: 7.516 min
 Delta R.T.: 0.000 min
 Response: 17399794
 Conc: 274.32 ng/ml

#29 AR-1254-4

R.T.: 6.462 min
 Delta R.T.: 0.000 min
 Response: 98587777
 Conc: 261.44 ng/ml



#30 AR-1254-5

R.T.: 7.932 min
 Delta R.T.: 0.000 min
 Response: 22010158
 Conc: 272.89 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

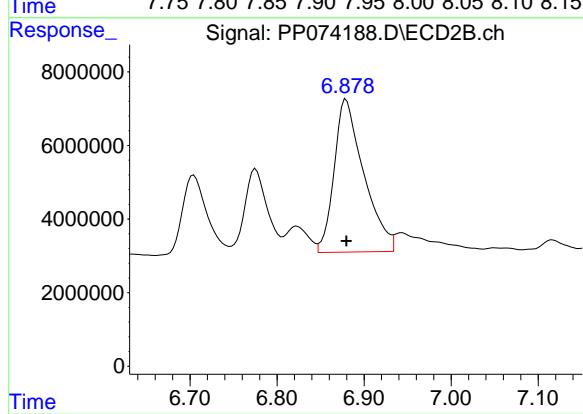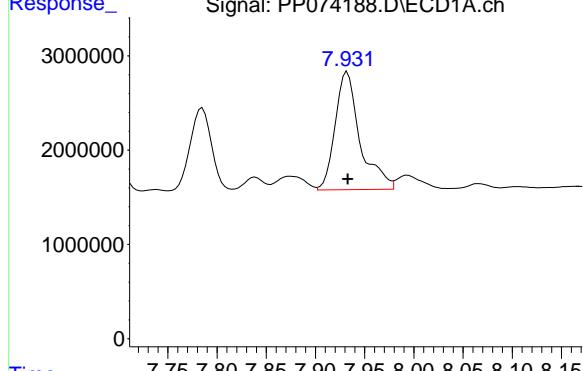

#30 AR-1254-5

R.T.: 6.879 min
 Delta R.T.: 0.000 min
 Response: 98393861
 Conc: 247.08 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 19:23
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:03:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:03:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|---------|----------|-------|---------|
| 1) SA Tetrachlor... | 4.657 | 3.804 | 5935360 | 12647504 | 5.284 | 3.358 # |
| 2) SA Decachlor... | 10.430 | 8.823 | 5026515 | 24210870 | 5.158 | 4.086 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|----------|
| 26) L6 AR-1254-1 | 6.655 | 5.689 | 2796732 | 16116298 | 51.810m | 44.012 |
| 27) L6 AR-1254-2 | 6.872 | 5.836 | 4500635 | 12761430 | 56.609 | 45.869 |
| 28) L6 AR-1254-3 | 7.234 | 6.237 | 5142235 | 18482386 | 58.892 | 37.780 # |
| 29) L6 AR-1254-4 | 7.515 | 6.464 | 3412924 | 14935198 | 53.486 | 40.633 |
| 30) L6 AR-1254-5 | 7.931 | 6.881 | 4380720 | 14900727 | 53.986 | 37.906 # |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 19:23
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 48 Sample Multiplier: 1


Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:03:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:03:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

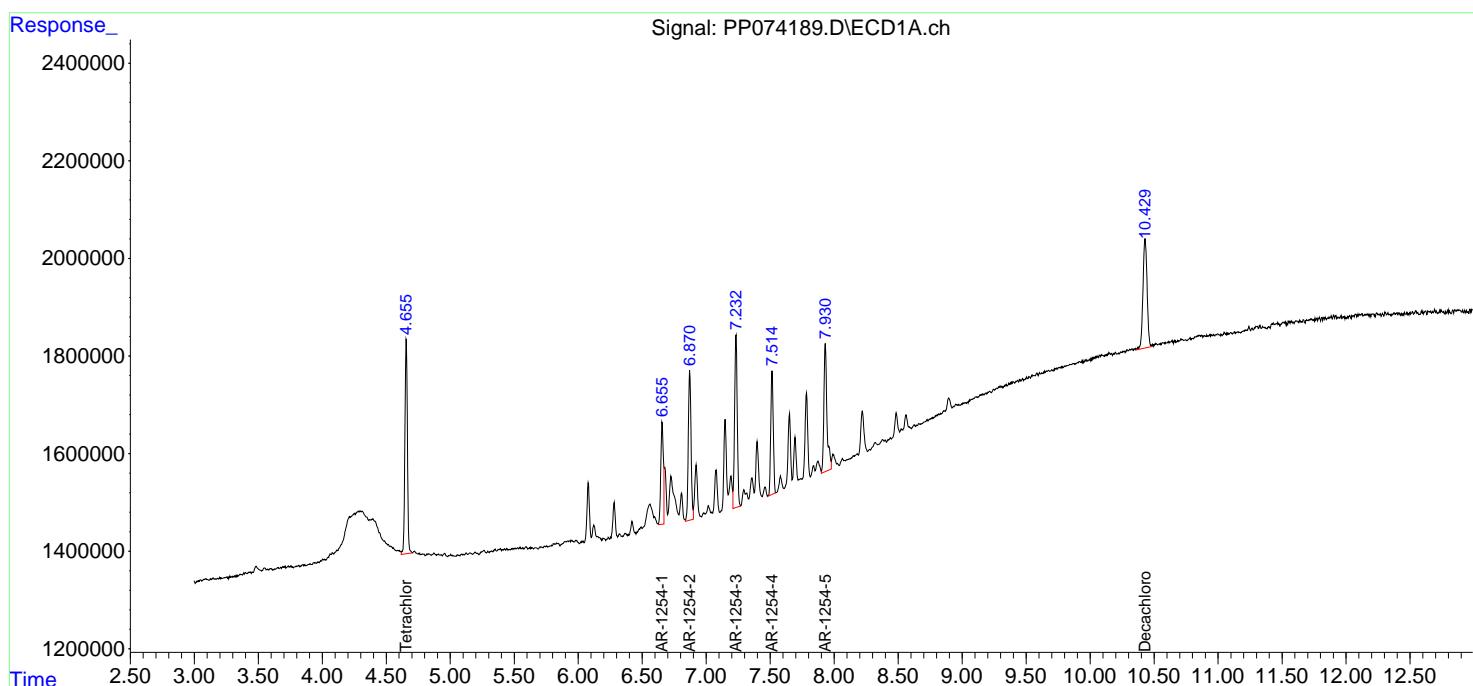

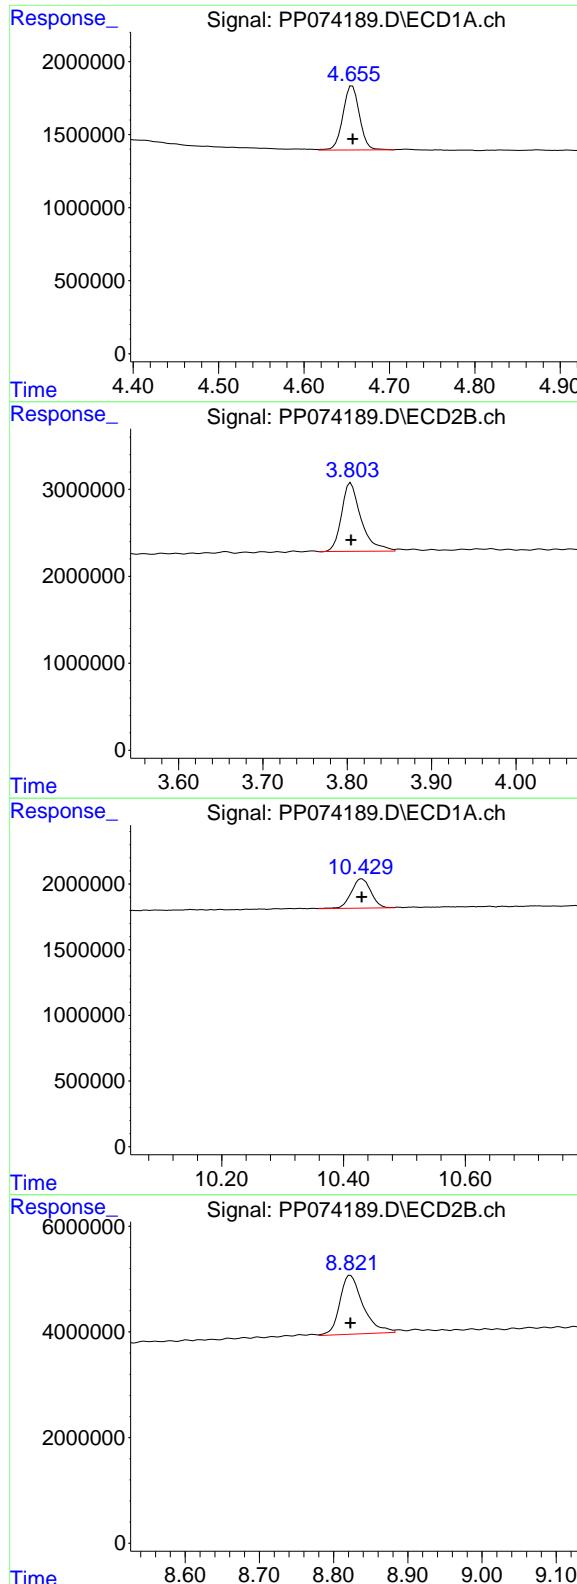

#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 5935360
Conc: 5.28 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 12647504
Conc: 3.36 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: 0.000 min
Response: 5026515
Conc: 5.16 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.823 min
Delta R.T.: 0.000 min
Response: 24210870
Conc: 4.09 ng/ml

#26 AR-1254-1

R.T.: 6.655 min
 Delta R.T.: 0.000 min
 Response: 2796732
 Conc: 51.81 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#26 AR-1254-1





R.T.: 5.689 min
 Delta R.T.: 0.000 min
 Response: 16116298
 Conc: 44.01 ng/ml


#27 AR-1254-2

R.T.: 6.872 min
 Delta R.T.: 0.000 min
 Response: 4500635
 Conc: 56.61 ng/ml

#27 AR-1254-2

R.T.: 5.836 min
 Delta R.T.: 0.000 min
 Response: 12761430
 Conc: 45.87 ng/ml

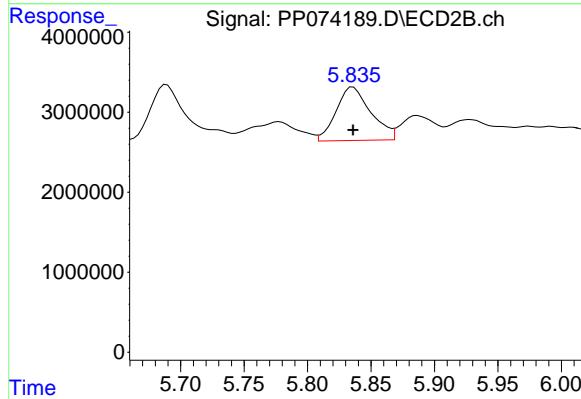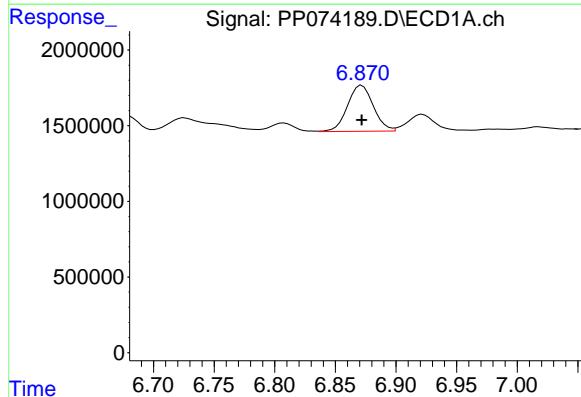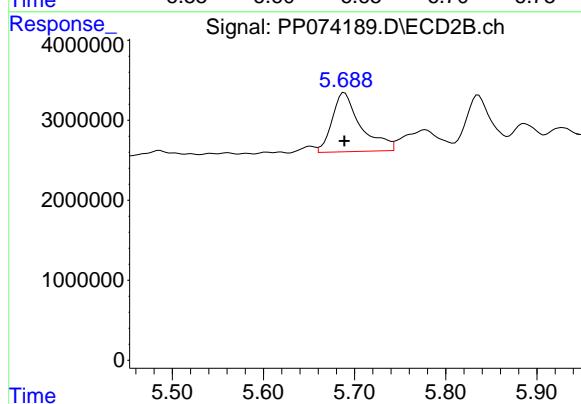

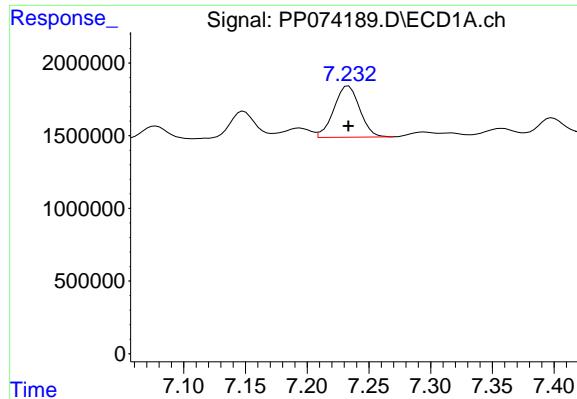


#28 AR-1254-3

R.T.: 7.234 min
 Delta R.T.: 0.000 min
 Response: 5142235
 Conc: 58.89 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC050


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

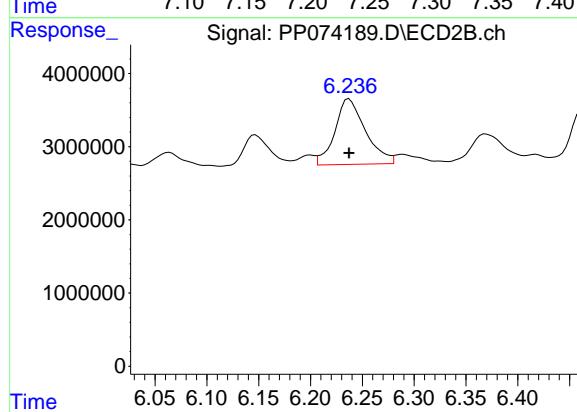


#28 AR-1254-3

R.T.: 6.237 min
 Delta R.T.: 0.000 min
 Response: 18482386
 Conc: 37.78 ng/ml

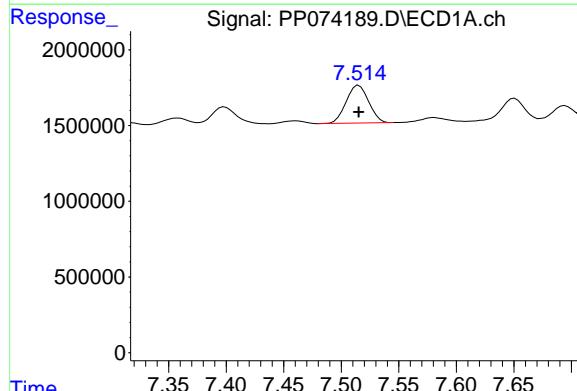


#29 AR-1254-4

R.T.: 7.515 min
 Delta R.T.: 0.000 min
 Response: 3412924
 Conc: 53.49 ng/ml

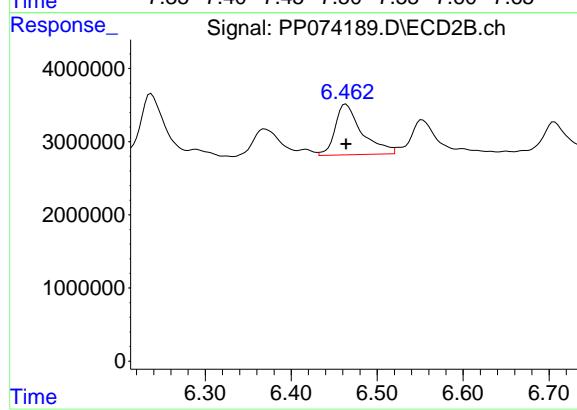

#29 AR-1254-4

R.T.: 6.464 min
 Delta R.T.: 0.000 min
 Response: 14935198
 Conc: 40.63 ng/ml

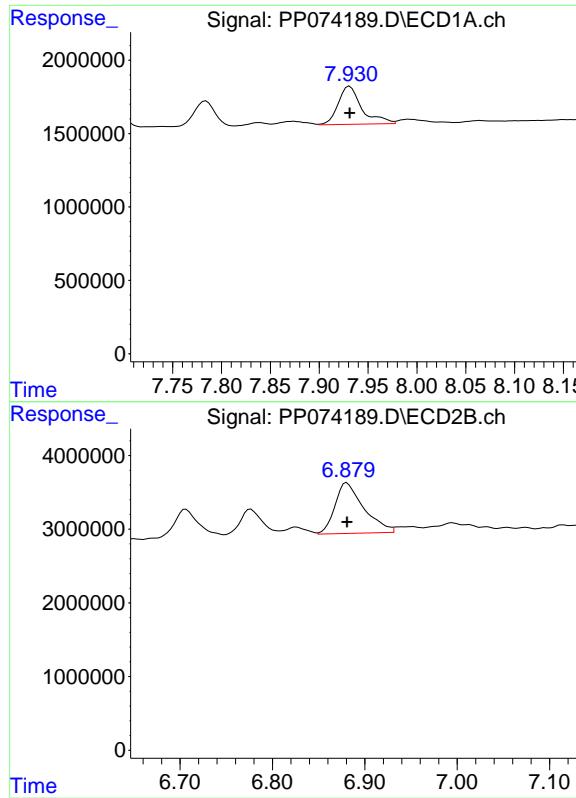

#30 AR-1254-5

R.T.: 7.931 min
 Delta R.T.: 0.000 min
 Response: 4380720
 Conc: 53.99 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#30 AR-1254-5

R.T.: 6.881 min
 Delta R.T.: 0.000 min
 Response: 14900727
 Conc: 37.91 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 19:39
 Operator : YP\AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:10:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:10:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.802 | 54354703 | 199.7E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.430 | 8.820 | 48321379 | 306.6E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|---------|---------|
| 36) L8 AR-1262-1 | 8.237 | 6.917 | 37894848 | 281.6E6 | 500.000 | 500.000 |
| 37) L8 AR-1262-2 | 8.562 | 7.176 | 65215013 | 200.5E6 | 500.000 | 500.000 |
| 38) L8 AR-1262-3 | 8.888 | 7.698 | 47035440 | 179.7E6 | 500.000 | 500.000 |
| 39) L8 AR-1262-4 | 8.974 | 7.761 | 36425846 | 333.5E6 | 500.000 | 500.000 |
| 40) L8 AR-1262-5 | 9.645 | 8.255 | 25461320 | 141.6E6 | 500.000 | 500.000 |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074190.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 19:39
 Operator : YP\AJ
 Sample : AR1262ICC500
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1262ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:10:39 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:10:03 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

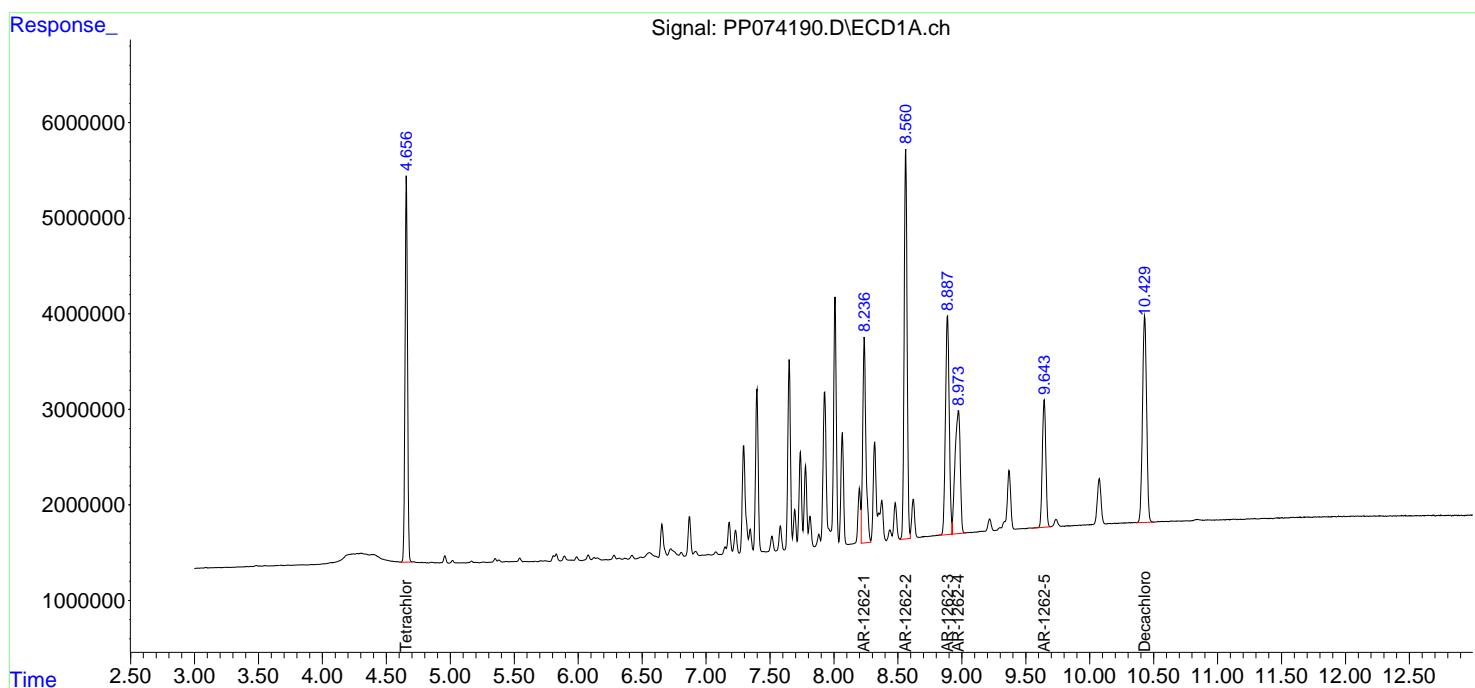

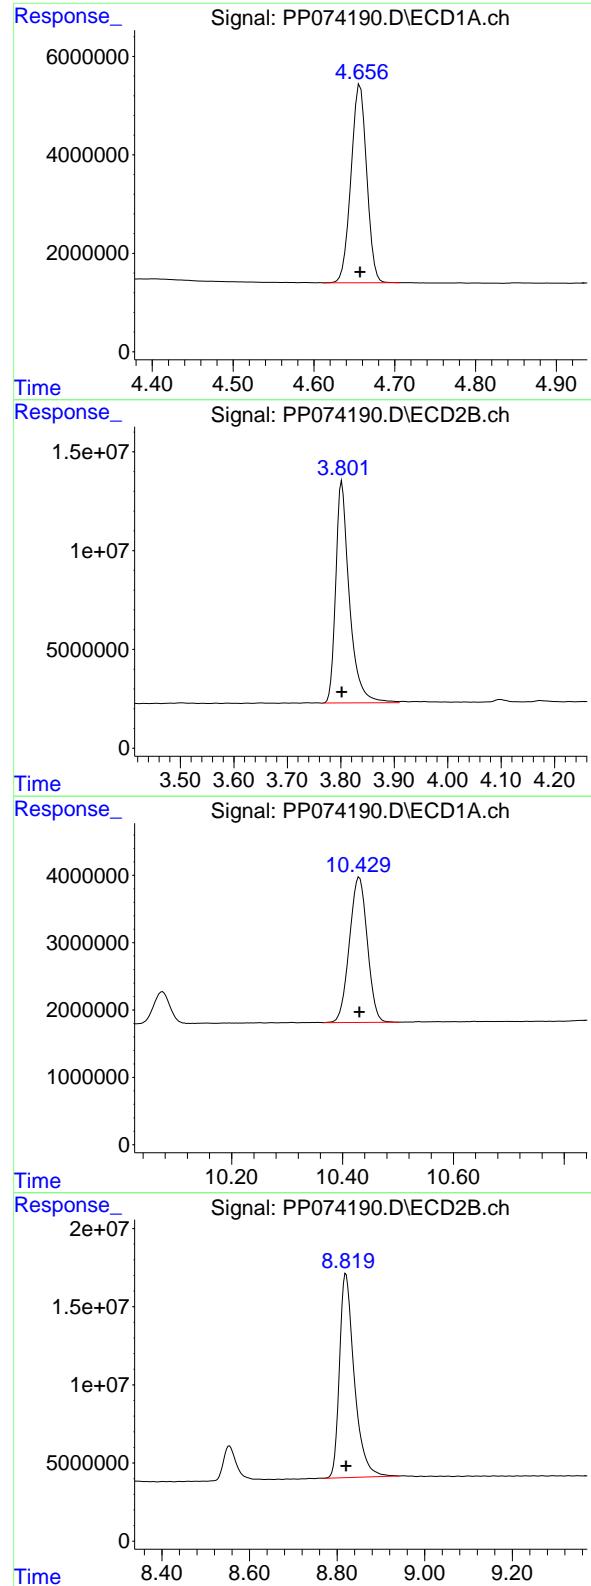

#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 54354703
Conc: 50.00 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1262ICC500

#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: 0.000 min
Response: 199655972
Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: 0.000 min
Response: 48321379
Conc: 50.00 ng/ml





#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: 0.000 min
Response: 306598020
Conc: 50.00 ng/ml

#36 AR-1262-1

R.T.: 8.237 min
 Delta R.T.: 0.000 min
 Response: 37894848
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1262ICC500

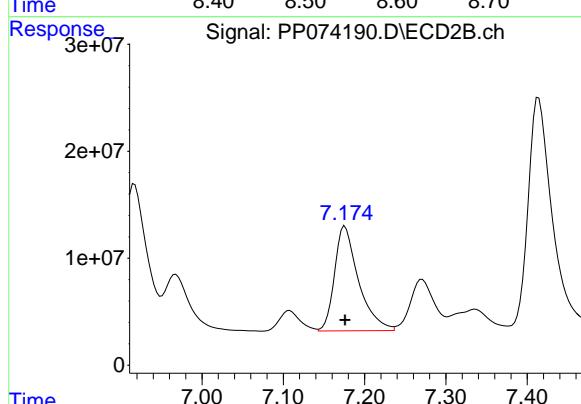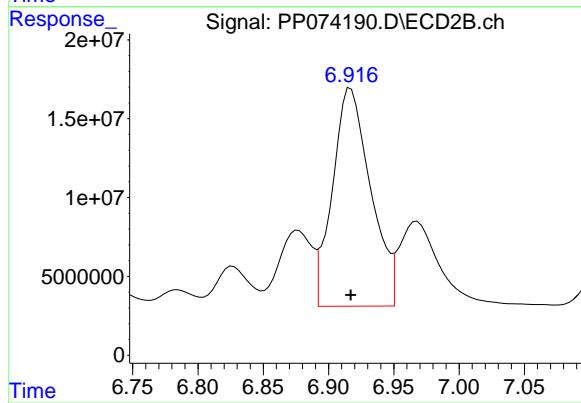

#36 AR-1262-1

R.T.: 6.917 min
 Delta R.T.: 0.000 min
 Response: 281571248
 Conc: 500.00 ng/ml

#37 AR-1262-2

R.T.: 8.562 min
 Delta R.T.: 0.000 min
 Response: 65215013
 Conc: 500.00 ng/ml





#37 AR-1262-2

R.T.: 7.176 min
 Delta R.T.: 0.000 min
 Response: 200511630
 Conc: 500.00 ng/ml

#38 AR-1262-3

R.T.: 8.888 min
 Delta R.T.: 0.000 min
 Response: 47035440
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1262ICC500

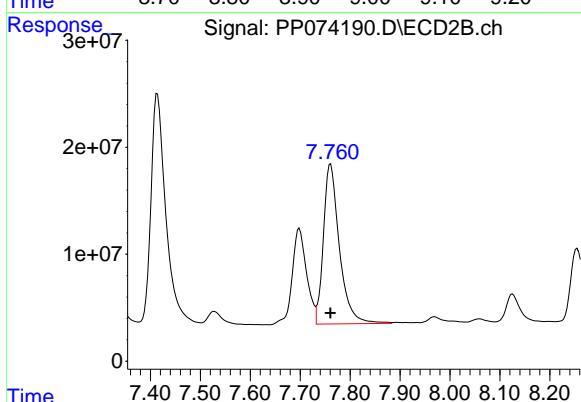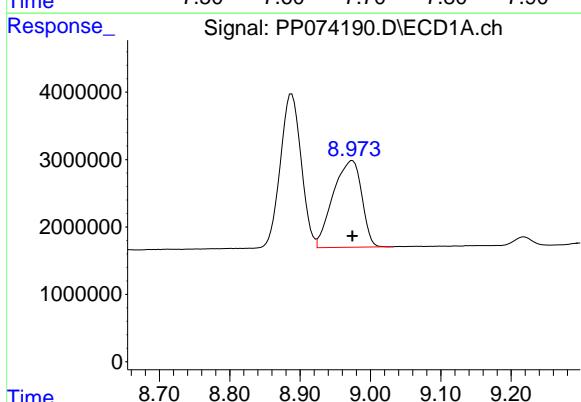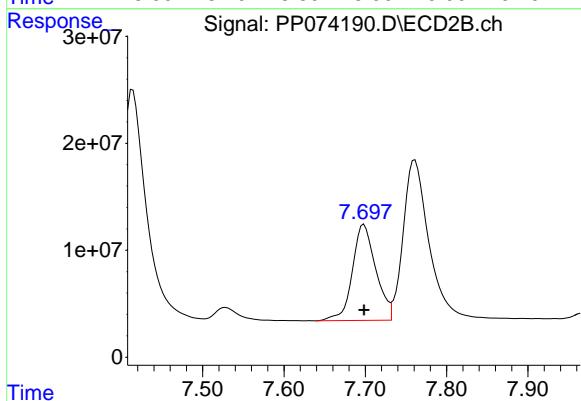

#38 AR-1262-3

R.T.: 7.698 min
 Delta R.T.: 0.000 min
 Response: 179734932
 Conc: 500.00 ng/ml

#39 AR-1262-4

R.T.: 8.974 min
 Delta R.T.: 0.000 min
 Response: 36425846
 Conc: 500.00 ng/ml



#39 AR-1262-4

R.T.: 7.761 min
 Delta R.T.: 0.000 min
 Response: 333460882
 Conc: 500.00 ng/ml

#40 AR-1262-5

R.T.: 9.645 min
Delta R.T.: 0.000 min
Response: 25461320
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1262ICC500

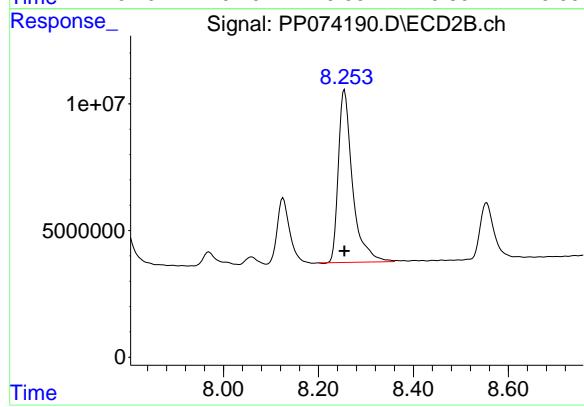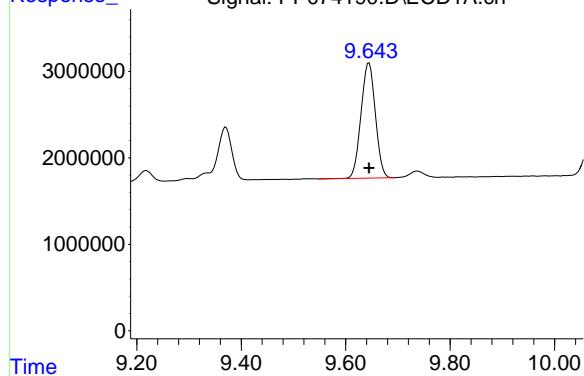

#40 AR-1262-5

R.T.: 8.255 min
Delta R.T.: 0.000 min
Response: 141634065
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 20:28
 Operator : YP\AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:15:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:13:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.656 | 3.801 | 58418637 | 219.4E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.429 | 8.820 | 86270477 | 592.0E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|--------|-------|----------|----------|---------|---------|
| 41) L9 AR-1268-1 | 8.883 | 7.698 | 79013824 | 584.6E6 | 500.000 | 500.000 |
| 42) L9 AR-1268-2 | 8.978 | 7.762 | 73014004 | 574.1E6 | 500.000 | 500.000 |
| 43) L9 AR-1268-3 | 9.218 | 7.970 | 60700868 | 445.9E6 | 500.000 | 500.000 |
| 44) L9 AR-1268-4 | 9.644 | 8.255 | 29824069 | 164.7E6 | 500.000 | 500.000 |
| 45) L9 AR-1268-5 | 10.075 | 8.556 | 179.0E6 | 1386.1E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074193.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 20:28
 Operator : YP\AJ
 Sample : AR1268ICC500
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1268ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:15:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:13:43 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

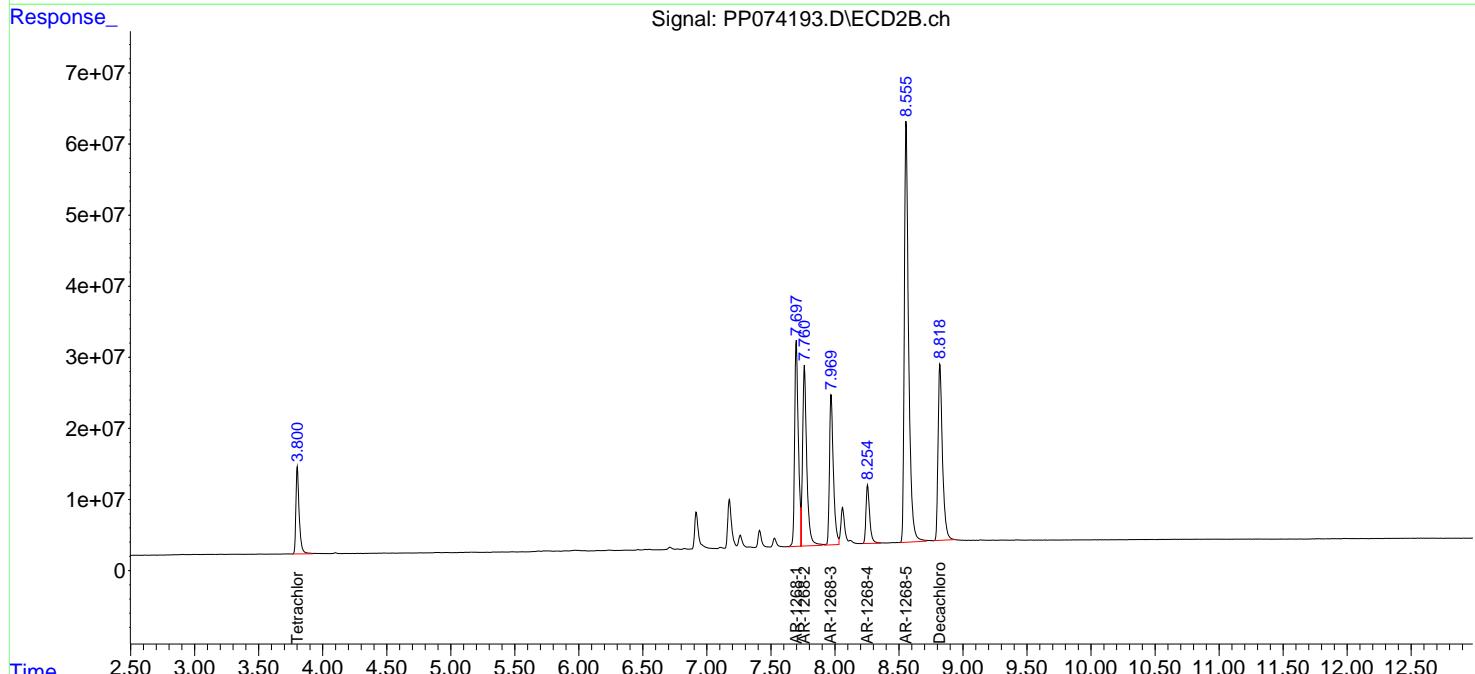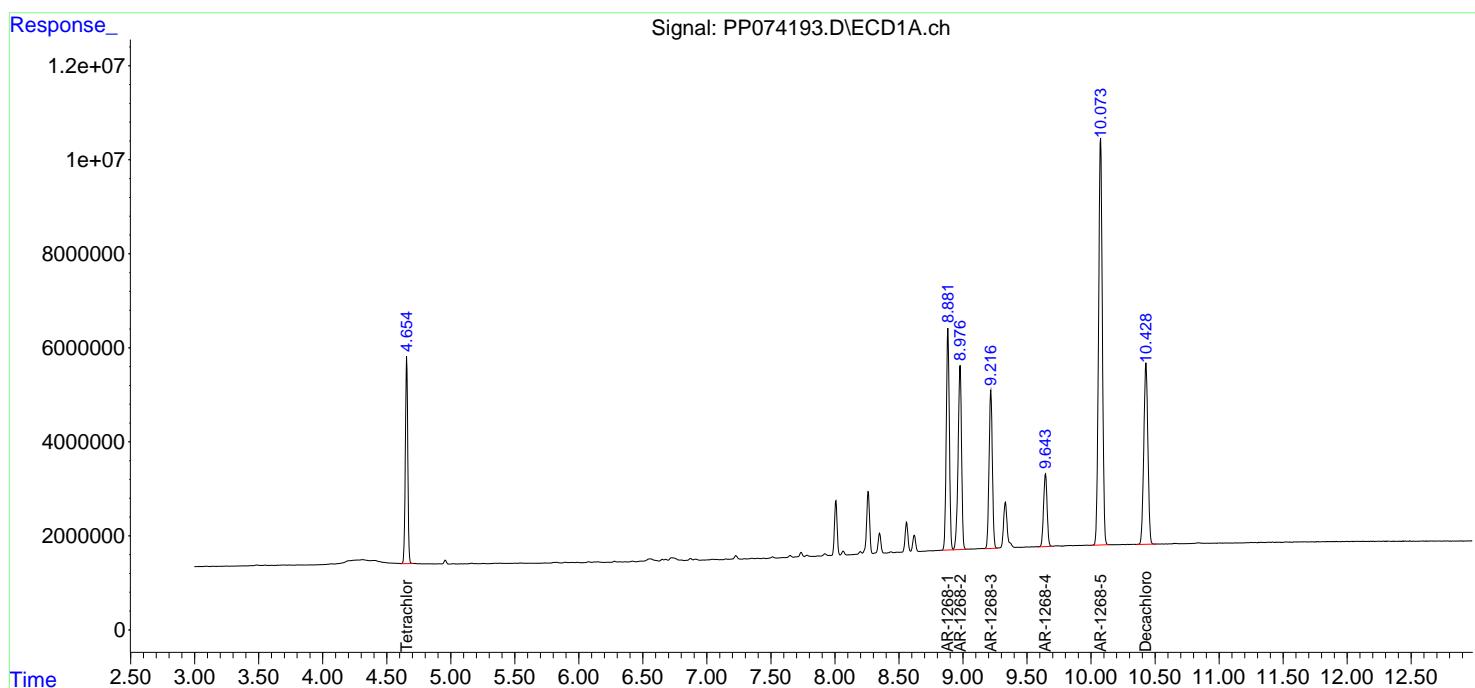

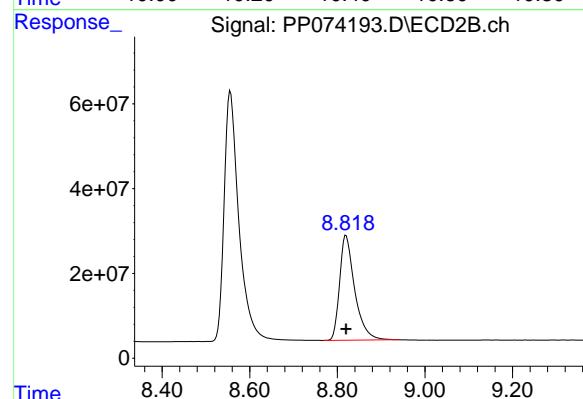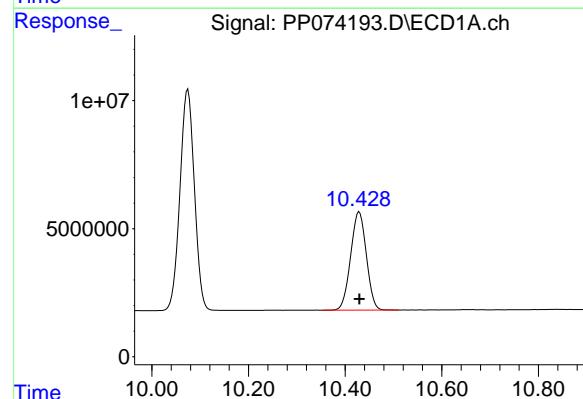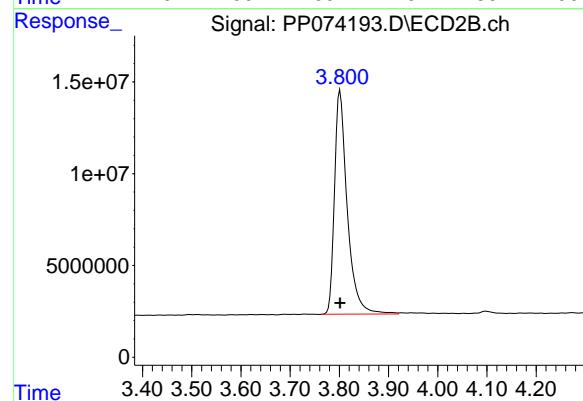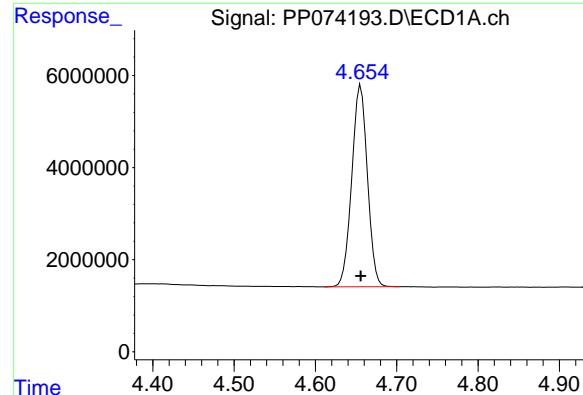

#1 Tetrachloro-m-xylene

R.T.: 4.656 min
 Delta R.T.: 0.000 min
 Response: 58418637
 Conc: 50.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1268ICC500

#1 Tetrachloro-m-xylene





R.T.: 3.801 min
 Delta R.T.: 0.000 min
 Response: 219400957
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.429 min
 Delta R.T.: 0.000 min
 Response: 86270477
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.820 min
 Delta R.T.: 0.000 min
 Response: 591964965
 Conc: 50.00 ng/ml

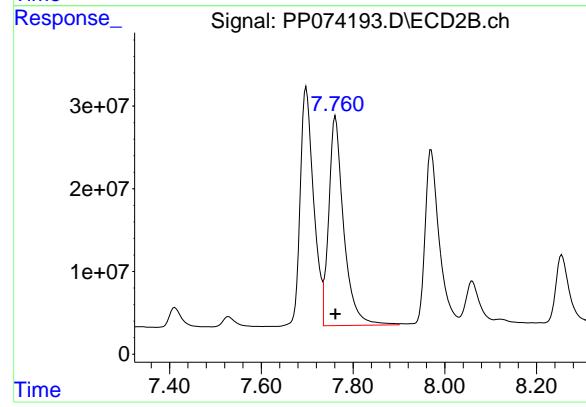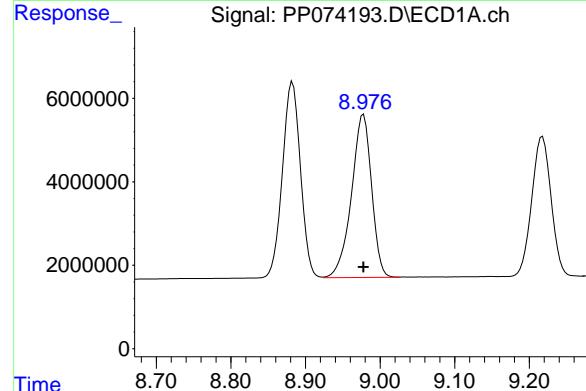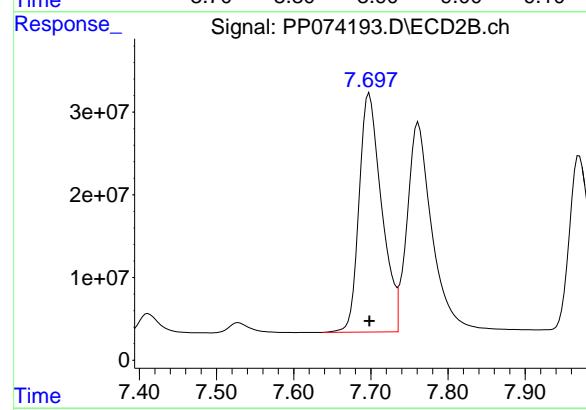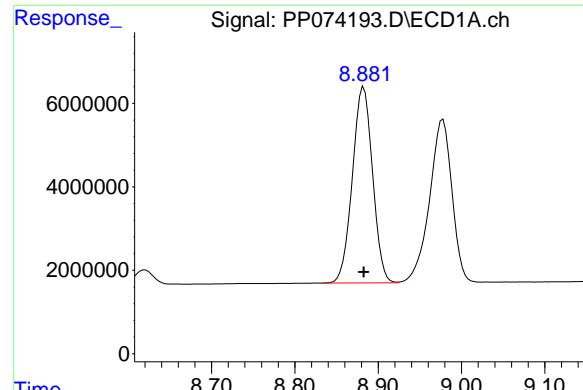

#41 AR-1268-1

R.T.: 8.883 min
Delta R.T.: 0.000 min
Response: 79013824
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

#41 AR-1268-1

R.T.: 7.698 min
Delta R.T.: 0.000 min
Response: 584610148
Conc: 500.00 ng/ml

#42 AR-1268-2

R.T.: 8.978 min
Delta R.T.: 0.000 min
Response: 73014004
Conc: 500.00 ng/ml





#42 AR-1268-2

R.T.: 7.762 min
Delta R.T.: 0.000 min
Response: 574066353
Conc: 500.00 ng/ml

#43 AR-1268-3

R.T.: 9.218 min
 Delta R.T.: 0.000 min
 Response: 60700868
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

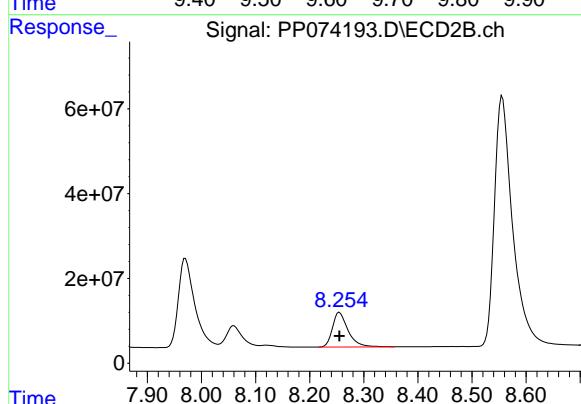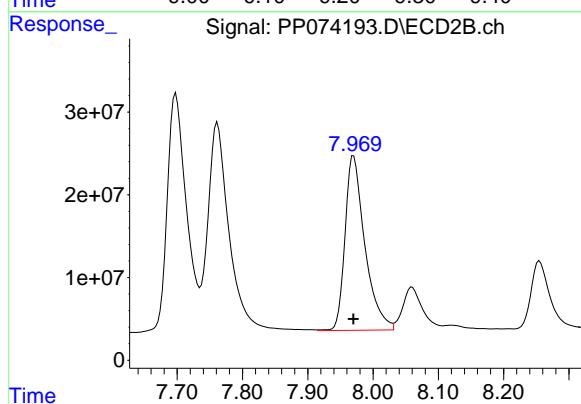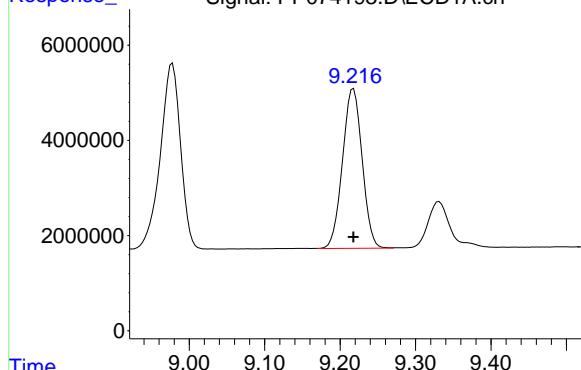

#43 AR-1268-3

R.T.: 7.970 min
 Delta R.T.: 0.000 min
 Response: 445933310
 Conc: 500.00 ng/ml

#44 AR-1268-4

R.T.: 9.644 min
 Delta R.T.: 0.000 min
 Response: 29824069
 Conc: 500.00 ng/ml



#44 AR-1268-4

R.T.: 8.255 min
 Delta R.T.: 0.000 min
 Response: 164734669
 Conc: 500.00 ng/ml

#45 AR-1268-5

R.T.: 10.075 min
Delta R.T.: 0.000 min
Response: 178970338
Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1268ICC500

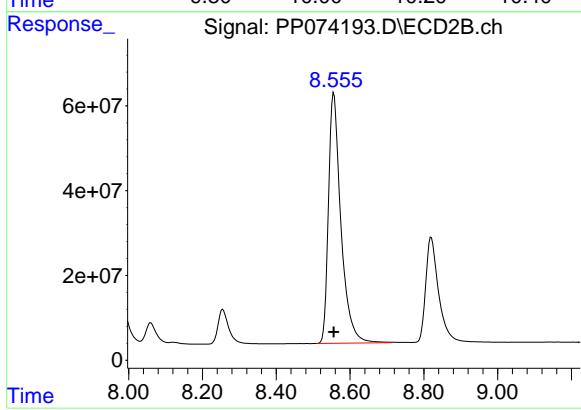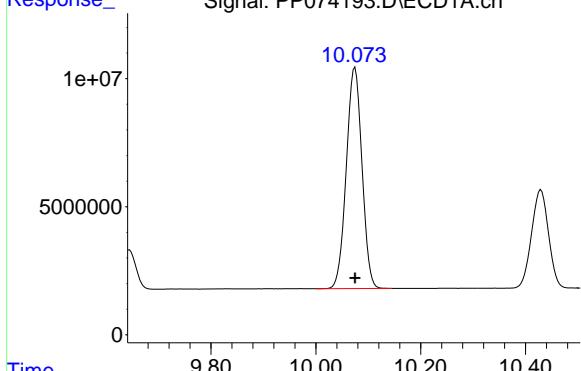

#45 AR-1268-5

R.T.: 8.556 min
Delta R.T.: 0.000 min
Response: 1386149287
Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 21:16
 Operator : YP\AJ
 Sample : PP080125ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:35:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.659 | 3.806 | 53809613 | 192.5E6 | 48.117 | 50.193 |
| 2) SA Decachlor... | 10.433 | 8.823 | 46918201 | 290.2E6 | 48.311 | 48.263 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 5.810 | 4.906 | 19711119 | 191.3E6 | 477.766 | 479.651 |
| 4) L1 AR-1016-2 | 5.831 | 4.963 | 29290082 | 90085682 | 482.207 | 479.666 |
| 5) L1 AR-1016-3 | 5.894 | 5.083 | 19171615 | 49893167 | 483.393 | 470.381 |
| 6) L1 AR-1016-4 | 5.991 | 5.124 | 15834175 | 51335124 | 486.540 | 470.016 |
| 7) L1 AR-1016-5 | 6.283 | 5.338 | 15788703 | 57011251 | 486.284 | 487.429 |
| 31) L7 AR-1260-1 | 7.400 | 6.554 | 27159073 | 192.5E6 | 481.919 | 476.633 |
| 32) L7 AR-1260-2 | 7.653 | 6.708 | 31876376 | 149.4E6 | 467.722 | 477.644 |
| 33) L7 AR-1260-3 | 8.010 | 6.918 | 25282960 | 196.9E6 | 474.388 | 499.492 |
| 34) L7 AR-1260-4 | 8.239 | 7.178 | 29964985 | 140.7E6 | 478.559 | 483.661 |
| 35) L7 AR-1260-5 | 8.563 | 7.417 | 53436862 | 370.6E6 | 471.620 | 489.248 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074196.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 21:16
 Operator : YP\AJ
 Sample : PP080125ICV500
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:35:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

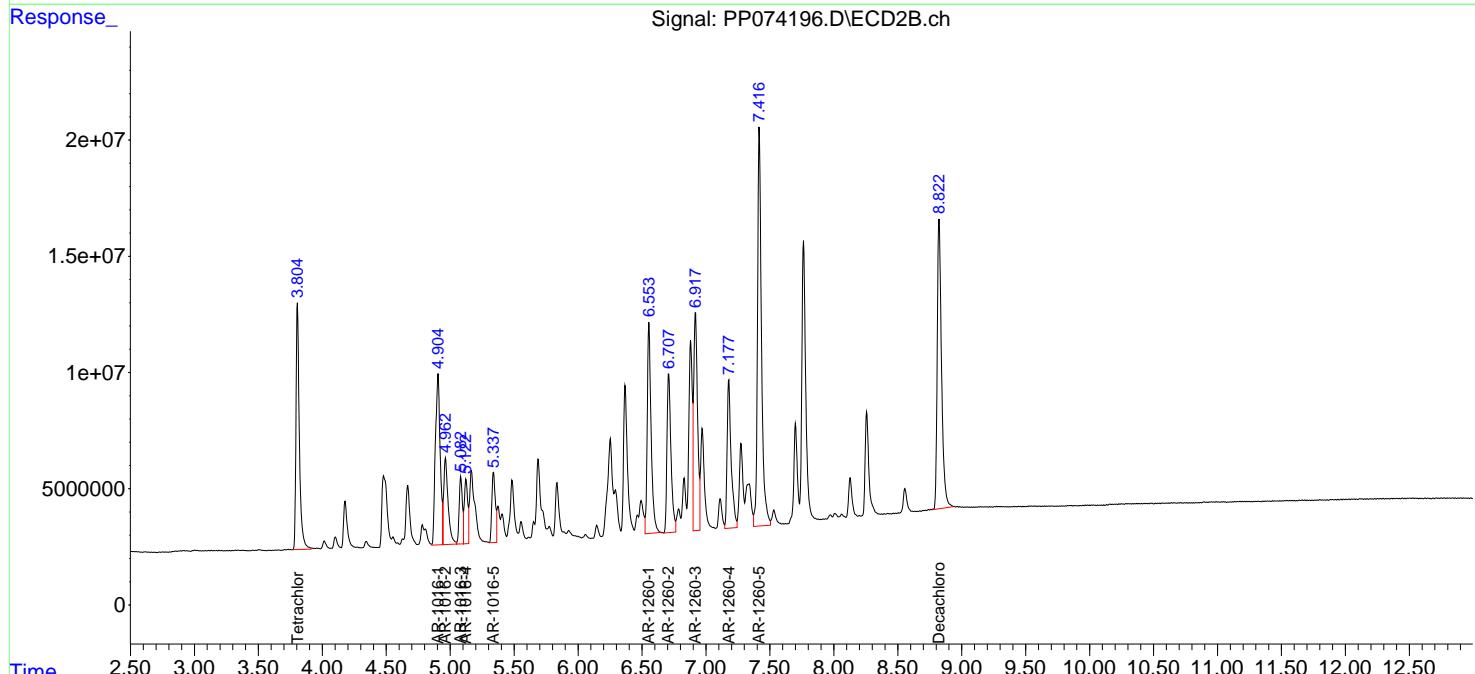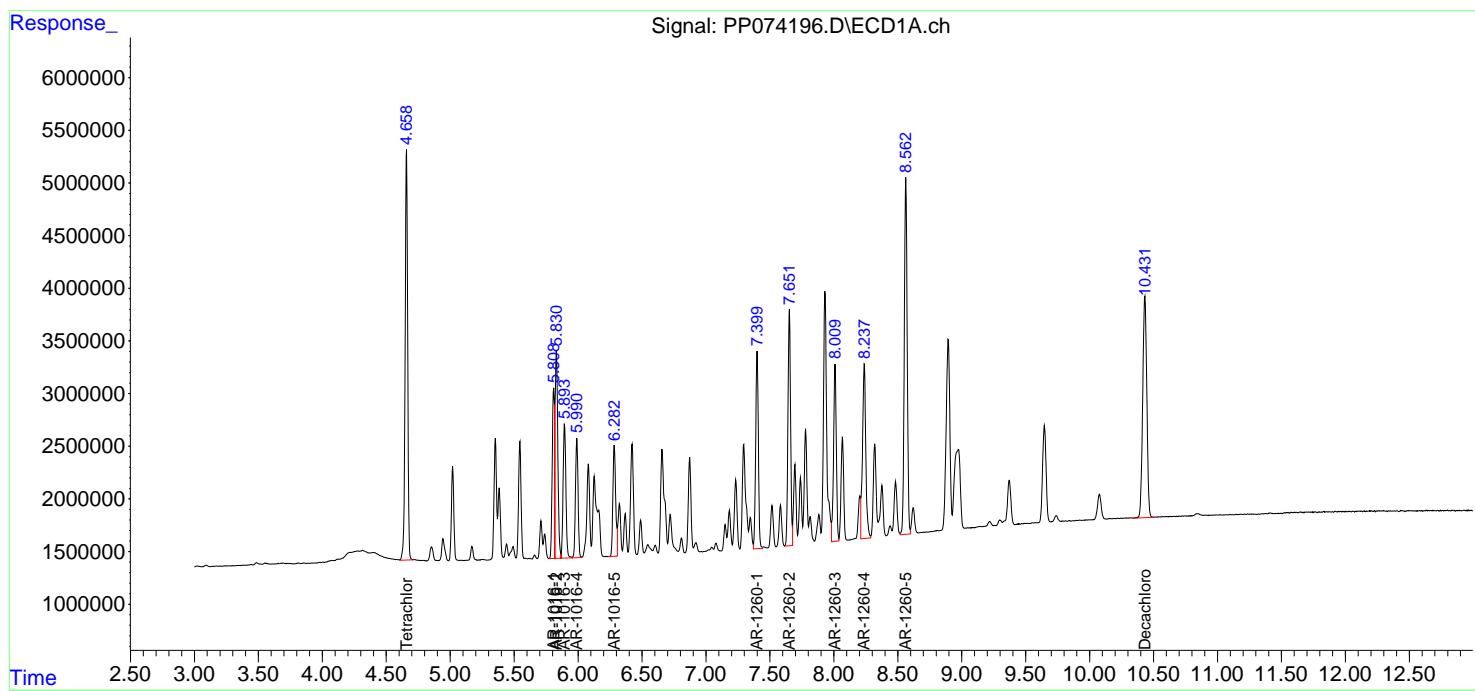


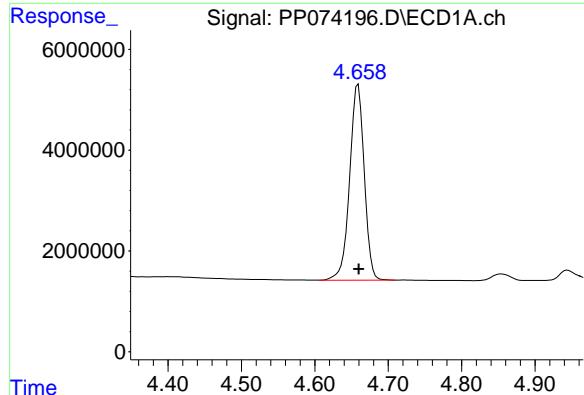

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 53809613
Conc: 48.12 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125

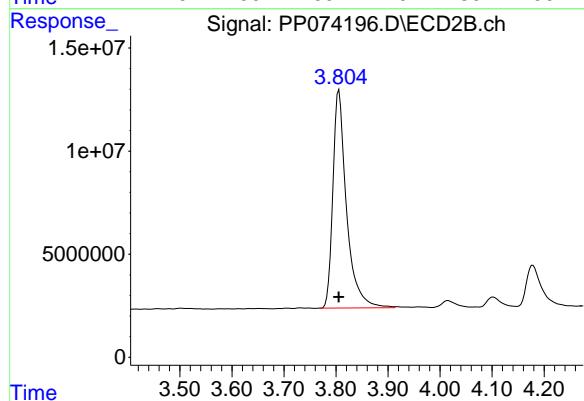


#1 Tetrachloro-m-xylene

R.T.: 3.806 min
Delta R.T.: 0.000 min
Response: 192460994
Conc: 50.19 ng/ml

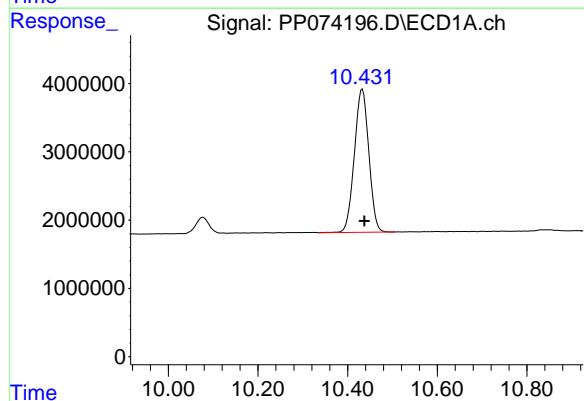


#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: -0.004 min
Response: 46918201
Conc: 48.31 ng/ml

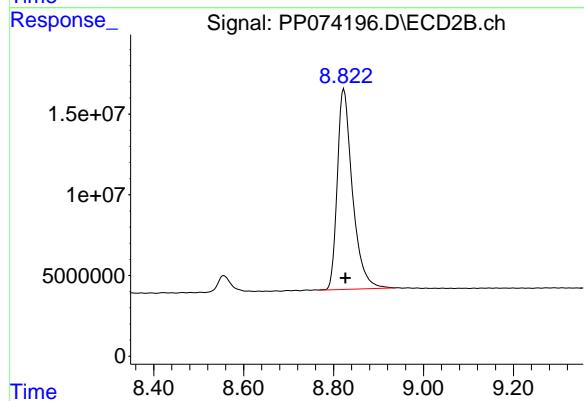

#2 Decachlorobiphenyl

R.T.: 8.823 min
Delta R.T.: -0.003 min
Response: 290236674
Conc: 48.26 ng/ml

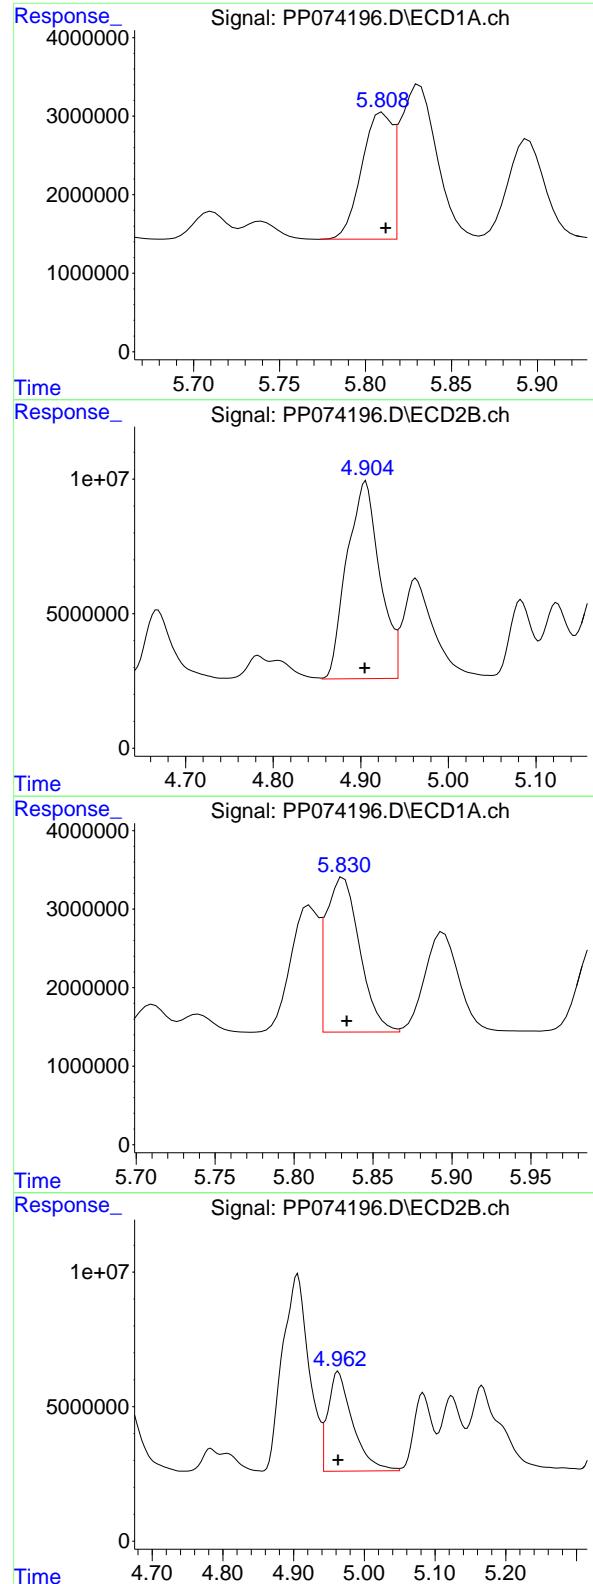

#3 AR-1016-1

R.T.: 5.810 min
 Delta R.T.: -0.002 min
 Response: 19711119
 Conc: 477.77 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125

#3 AR-1016-1





R.T.: 4.906 min
 Delta R.T.: 0.001 min
 Response: 191326645
 Conc: 479.65 ng/ml

#4 AR-1016-2

R.T.: 5.831 min
 Delta R.T.: -0.002 min
 Response: 29290082
 Conc: 482.21 ng/ml

#4 AR-1016-2

R.T.: 4.963 min
 Delta R.T.: 0.000 min
 Response: 90085682
 Conc: 479.67 ng/ml

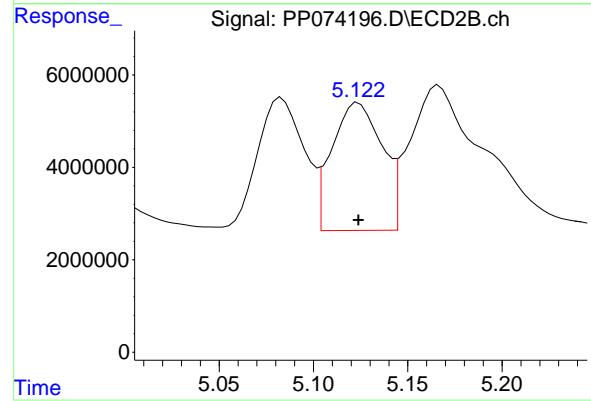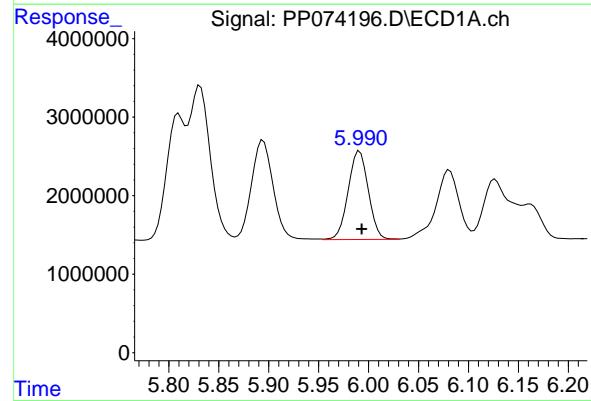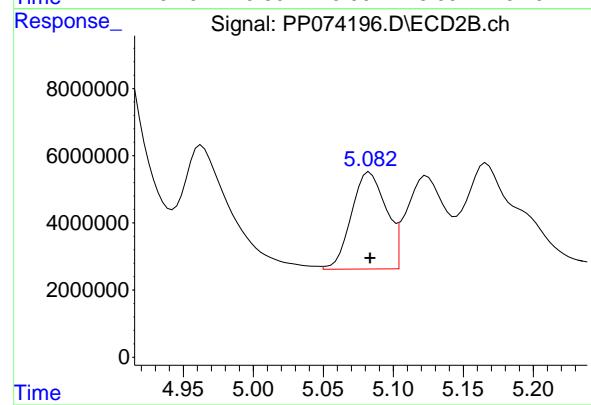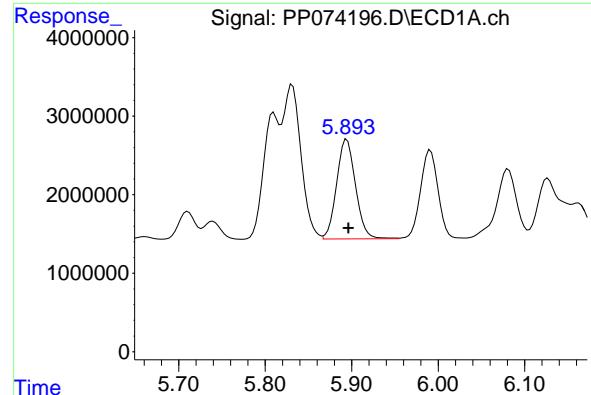

#5 AR-1016-3

R.T.: 5.894 min
Delta R.T.: -0.002 min
Response: 19171615
Conc: 483.39 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125

#5 AR-1016-3


R.T.: 5.083 min
Delta R.T.: 0.000 min
Response: 49893167
Conc: 470.38 ng/ml

#6 AR-1016-4

R.T.: 5.991 min
Delta R.T.: -0.002 min
Response: 15834175
Conc: 486.54 ng/ml

#6 AR-1016-4

R.T.: 5.124 min
Delta R.T.: 0.000 min
Response: 51335124
Conc: 470.02 ng/ml

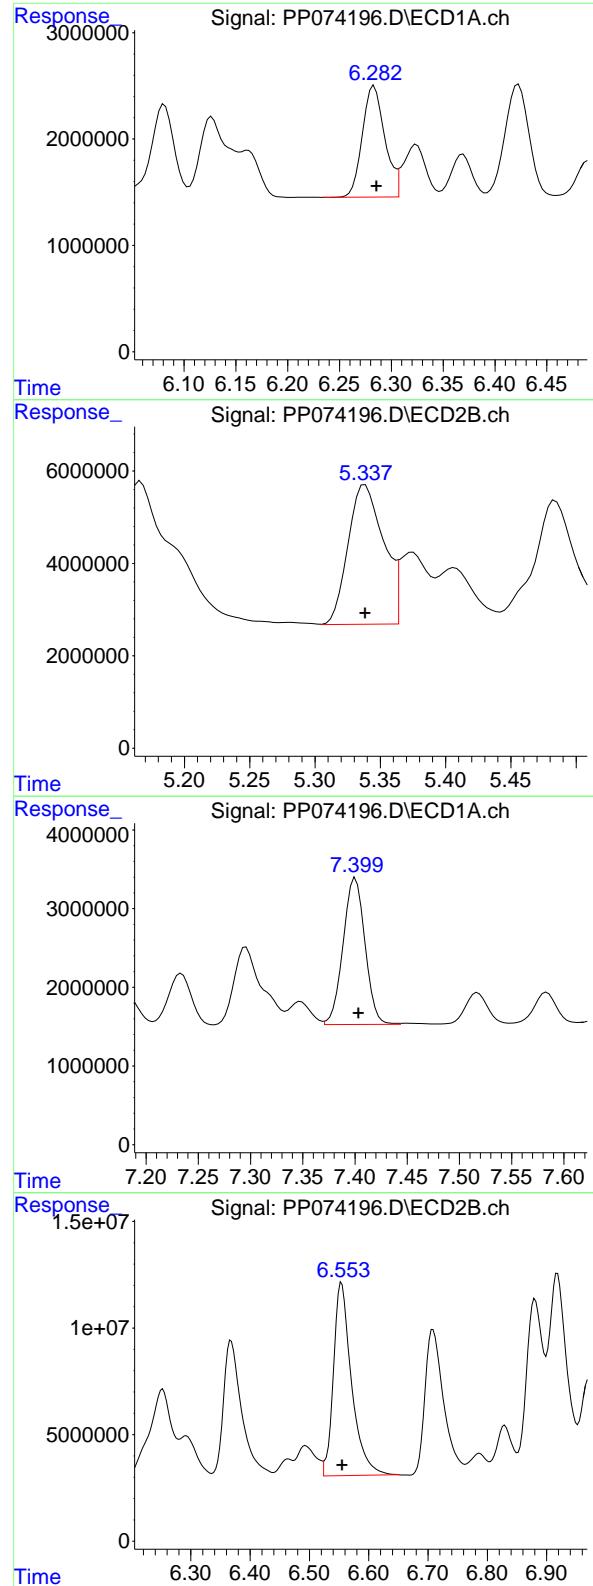

#7 AR-1016-5

R.T.: 6.283 min
 Delta R.T.: -0.002 min
 Response: 15788703
 Conc: 486.28 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125

#7 AR-1016-5

R.T.: 5.338 min
 Delta R.T.: 0.000 min
 Response: 57011251
 Conc: 487.43 ng/ml

#31 AR-1260-1

R.T.: 7.400 min
 Delta R.T.: -0.003 min
 Response: 27159073
 Conc: 481.92 ng/ml





#31 AR-1260-1

R.T.: 6.554 min
 Delta R.T.: 0.000 min
 Response: 192539458
 Conc: 476.63 ng/ml

#32 AR-1260-2

R.T.: 7.653 min
 Delta R.T.: -0.003 min
 Response: 31876376
 Conc: 467.72 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125

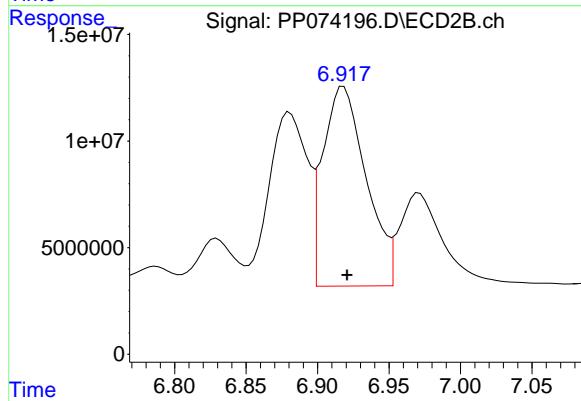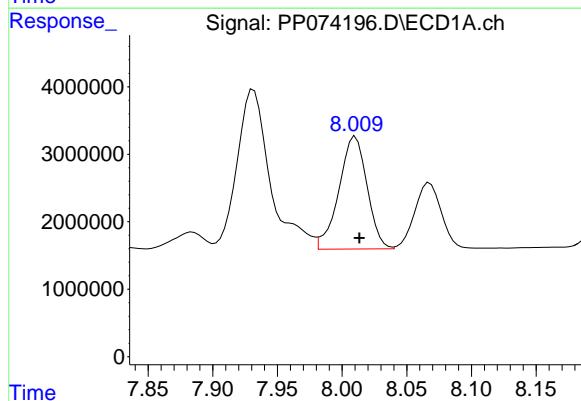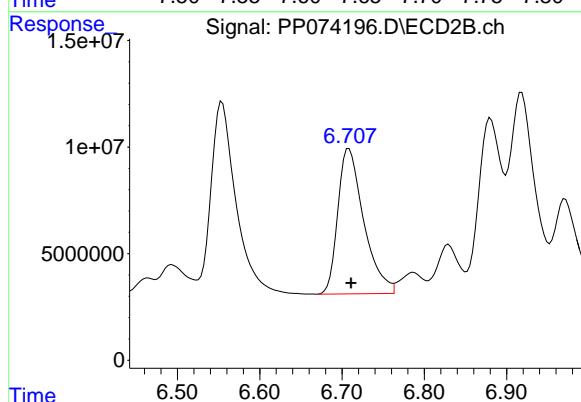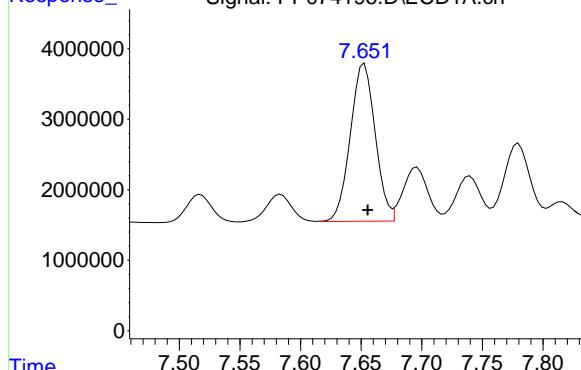

#32 AR-1260-2

R.T.: 6.708 min
 Delta R.T.: -0.002 min
 Response: 149358620
 Conc: 477.64 ng/ml

#33 AR-1260-3

R.T.: 8.010 min
 Delta R.T.: -0.003 min
 Response: 25282960
 Conc: 474.39 ng/ml





#33 AR-1260-3

R.T.: 6.918 min
 Delta R.T.: -0.002 min
 Response: 196859105
 Conc: 499.49 ng/ml

#34 AR-1260-4

R.T.: 8.239 min
 Delta R.T.: -0.003 min
 Response: 29964985
 Conc: 478.56 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125

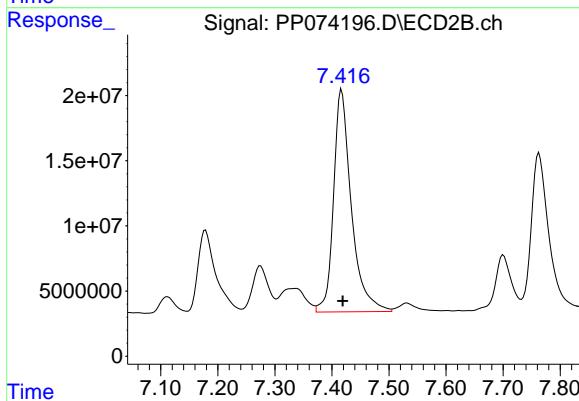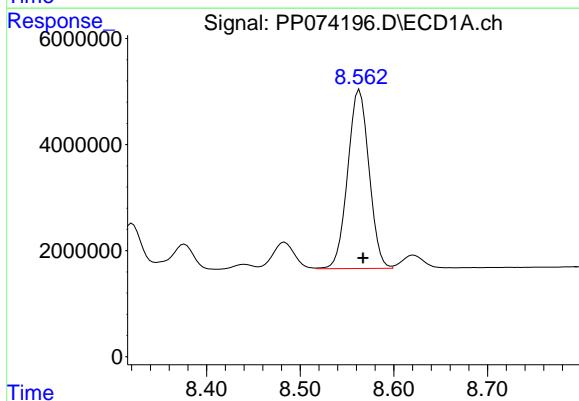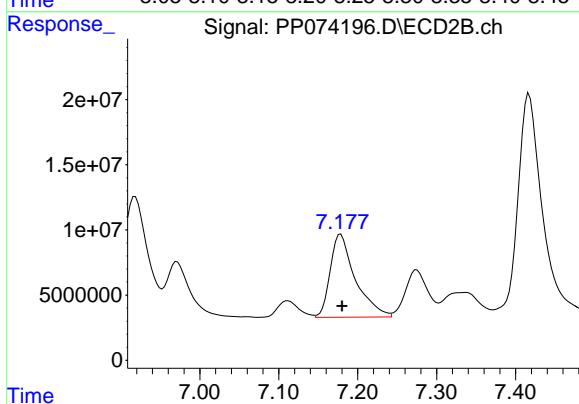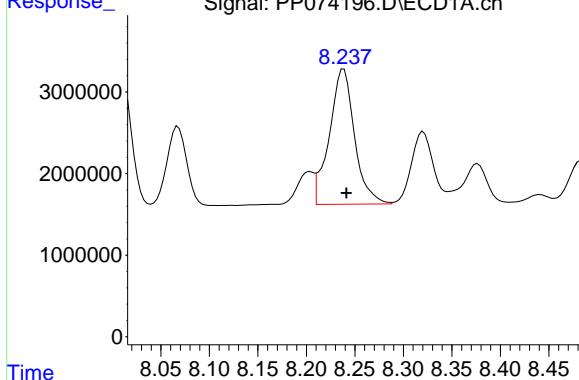

#34 AR-1260-4

R.T.: 7.178 min
 Delta R.T.: -0.002 min
 Response: 140735248
 Conc: 483.66 ng/ml

#35 AR-1260-5

R.T.: 8.563 min
 Delta R.T.: -0.004 min
 Response: 53436862
 Conc: 471.62 ng/ml

#35 AR-1260-5

R.T.: 7.417 min
 Delta R.T.: -0.002 min
 Response: 370561588
 Conc: 489.25 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 22:05
 Operator : YP\AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1242

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:36:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.655 | 3.804 | 55143327 | 198.9E6 | 49.310 | 51.866 |
| 2) SA Decachlor... | 10.427 | 8.822 | 47800939 | 295.6E6 | 49.220 | 49.156 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 16) L4 AR-1242-1 | 5.806 | 4.904 | 17499270 | 167.4E6 | 469.580 | 484.954 |
| 17) L4 AR-1242-2 | 5.827 | 4.962 | 25894594 | 77861664 | 475.925 | 476.575 |
| 18) L4 AR-1242-3 | 5.890 | 5.082 | 17050061 | 43676713 | 477.113 | 473.468 |
| 19) L4 AR-1242-4 | 5.987 | 5.164 | 14124012 | 56465948 | 483.390 | 472.829m |
| 20) L4 AR-1242-5 | 6.716 | 5.686 | 16823190 | 70286035 | 473.119 | 469.952 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 22:05
 Operator : YP\AJ
 Sample : AR12421ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:36:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 ICVPP080125AR1242

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

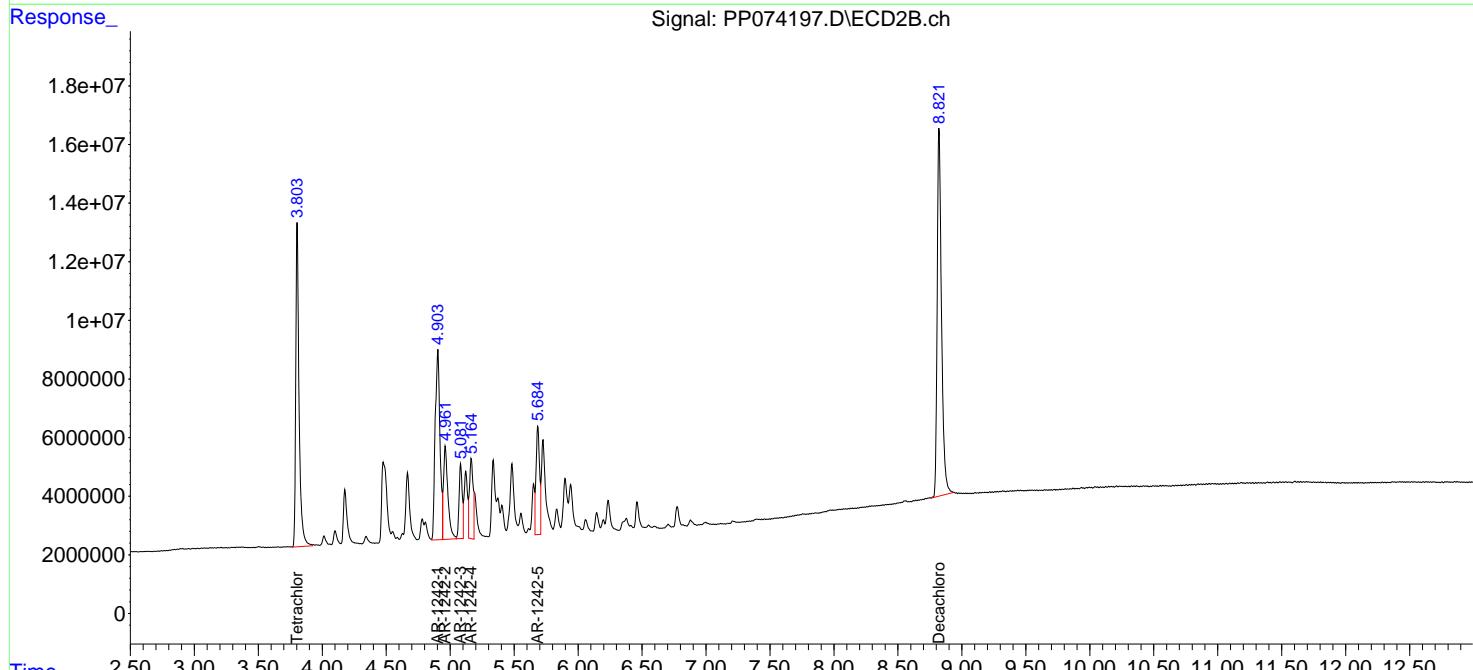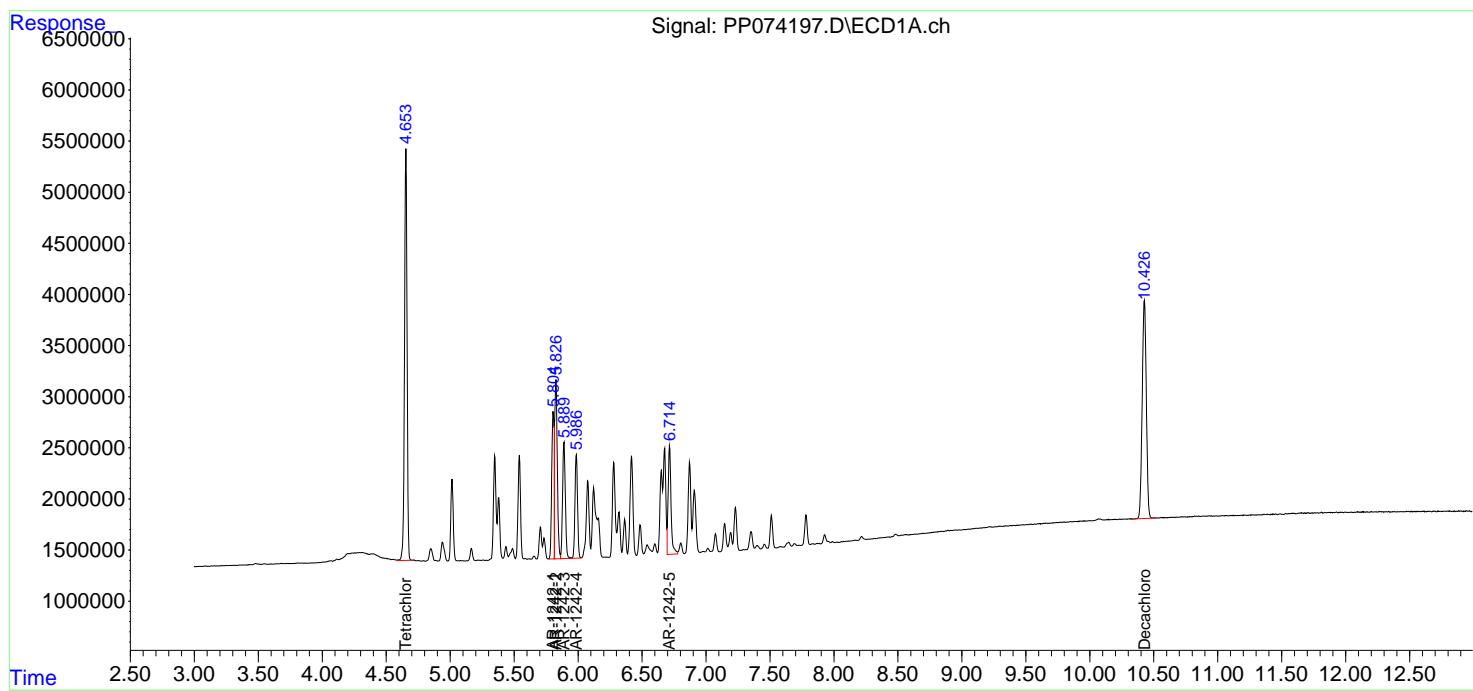

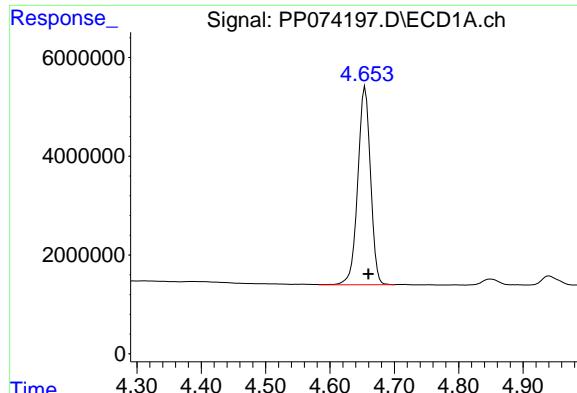


#1 Tetrachloro-m-xylene

R.T.: 4.655 min
Delta R.T.: -0.005 min
Response: 55143327
Conc: 49.31 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
Supervised By :mohammad ahmed 08/08/2025

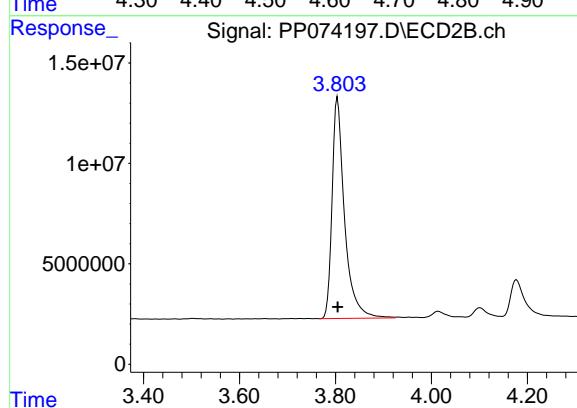


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 198876613
Conc: 51.87 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: -0.010 min
Response: 47800939
Conc: 49.22 ng/ml

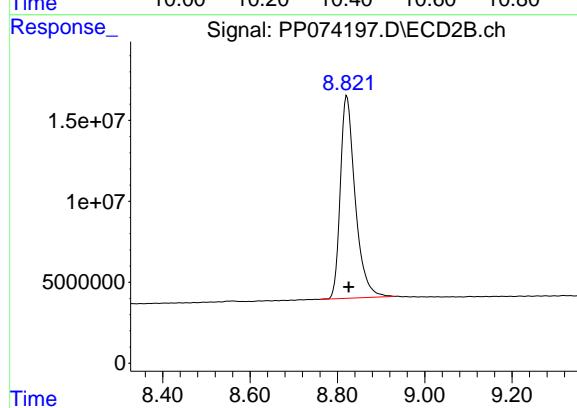

#2 Decachlorobiphenyl

R.T.: 8.822 min
Delta R.T.: -0.004 min
Response: 295607088
Conc: 49.16 ng/ml





#16 AR-1242-1

R.T.: 5.806 min
 Delta R.T.: -0.005 min
 Response: 17499270
 Conc: 469.58 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

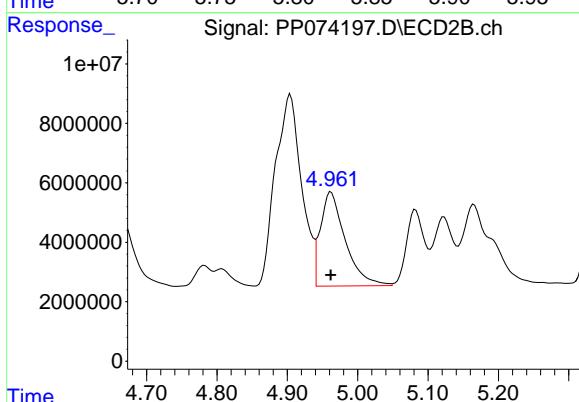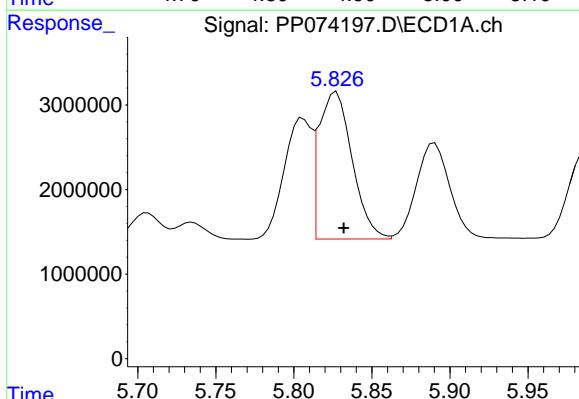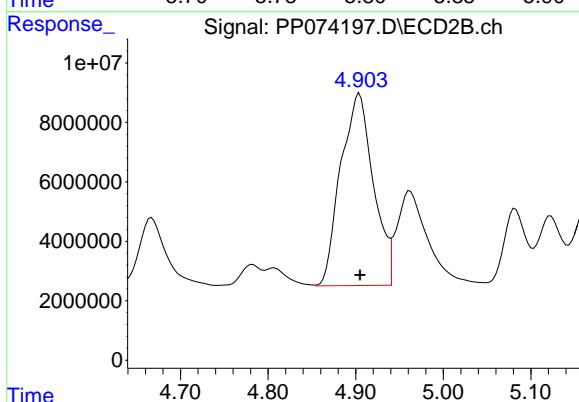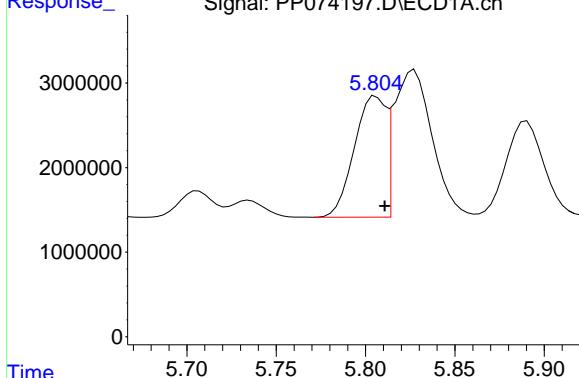

#16 AR-1242-1

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 167377399
 Conc: 484.95 ng/ml

#17 AR-1242-2

R.T.: 5.827 min
 Delta R.T.: -0.005 min
 Response: 25894594
 Conc: 475.93 ng/ml

#17 AR-1242-2

R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 77861664
 Conc: 476.57 ng/ml





#18 AR-1242-3

R.T.: 5.890 min
 Delta R.T.: -0.005 min
 Response: 17050061
 Conc: 477.11 ng/ml

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP080125AR1242

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

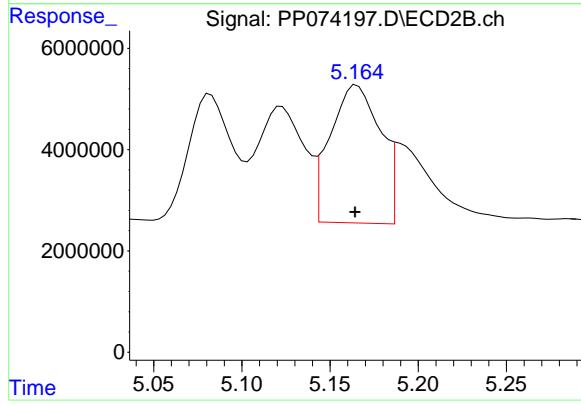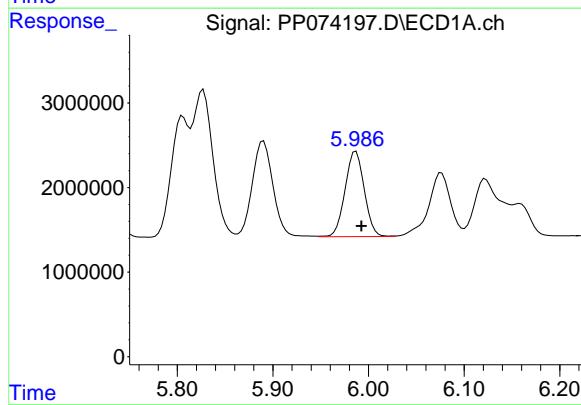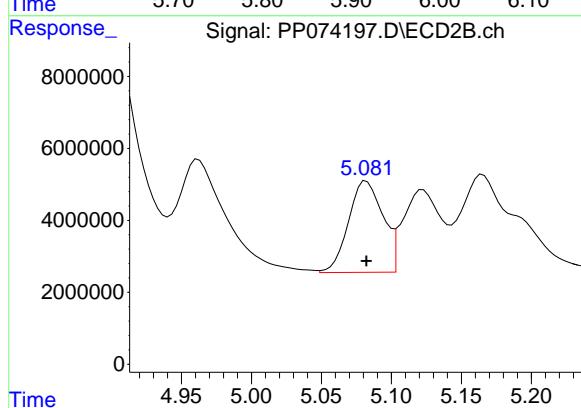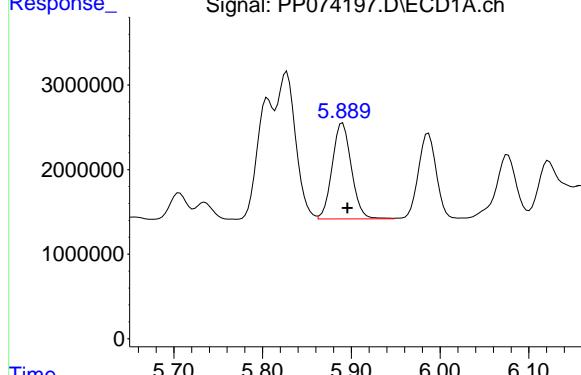

#18 AR-1242-3


R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 43676713
 Conc: 473.47 ng/ml

#19 AR-1242-4

R.T.: 5.987 min
 Delta R.T.: -0.006 min
 Response: 14124012
 Conc: 483.39 ng/ml

#19 AR-1242-4

R.T.: 5.164 min
 Delta R.T.: 0.000 min
 Response: 56465948
 Conc: 472.83 ng/ml

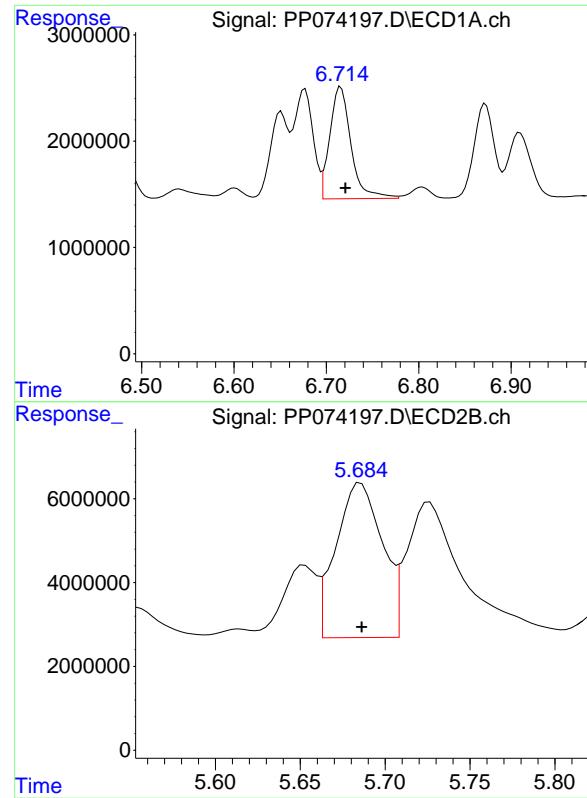

#20 AR-1242-5

R.T.: 6.716 min
 Delta R.T.: -0.005 min
 Response: 16823190
 Conc: 473.12 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/05/2025
 Supervised By :mohammad ahmed 08/08/2025

#20 AR-1242-5

R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 70286035
 Conc: 469.95 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 23:10
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1254

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
 Supervised By :mohammad ahmed 08/08/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 11:04:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.656 | 3.803 | 53831323 | 191.6E6 | 48.137 | 49.971 |
| 2) SA Decachlor... | 10.430 | 8.820 | 47450930 | 299.2E6 | 48.860 | 49.761 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|---------|
| 26) L6 AR-1254-1 | 6.654 | 5.686 | 27290919 | 178.5E6 | 518.434m | 487.493 |
| 27) L6 AR-1254-2 | 6.871 | 5.833 | 37599140 | 134.8E6 | 472.918 | 484.650 |
| 28) L6 AR-1254-3 | 7.233 | 6.235 | 40597005 | 245.2E6 | 464.942 | 501.115 |
| 29) L6 AR-1254-4 | 7.514 | 6.462 | 30708926 | 181.0E6 | 481.260 | 492.525 |
| 30) L6 AR-1254-5 | 7.930 | 6.878 | 38809795 | 188.2E6 | 478.279 | 488.601 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 23:10
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 04 11:04:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
ClientSampleId :
 ICVPP080125AR1254

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
 Supervised By :mohammad ahmed 08/08/2025

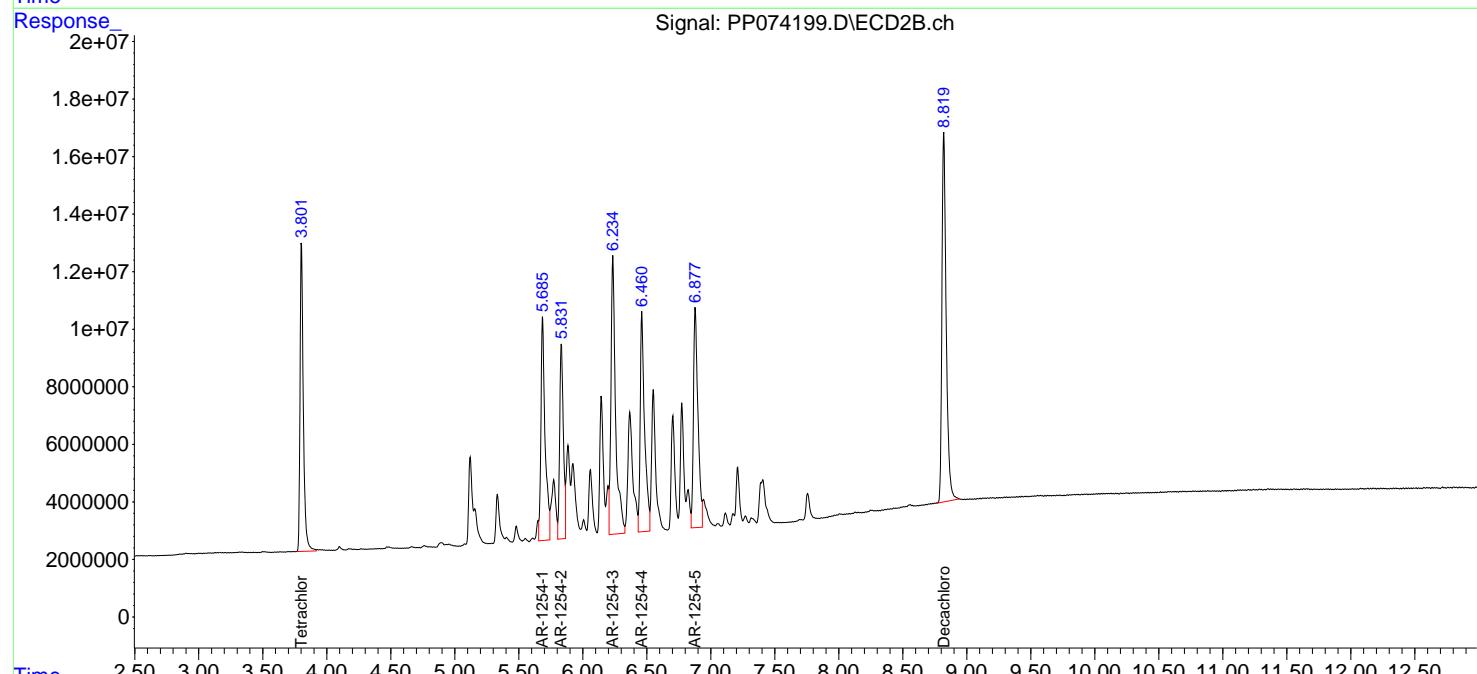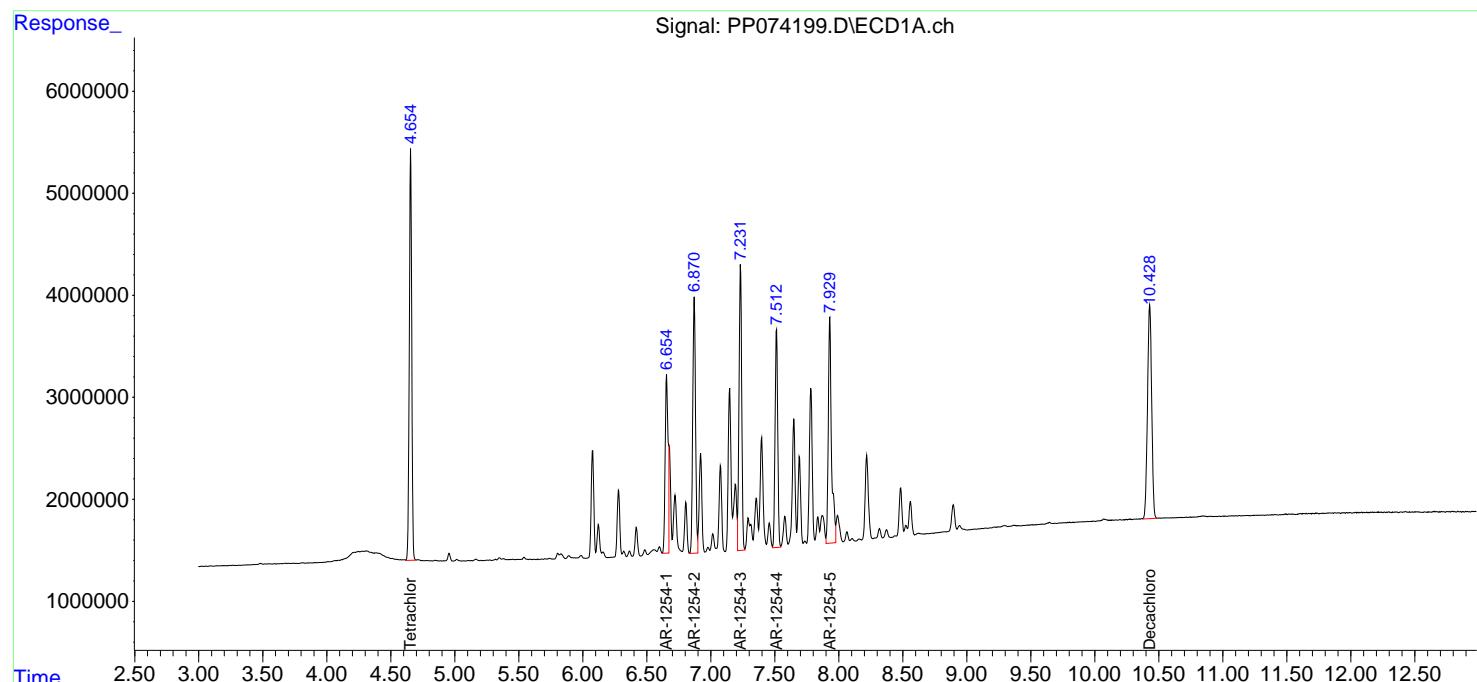

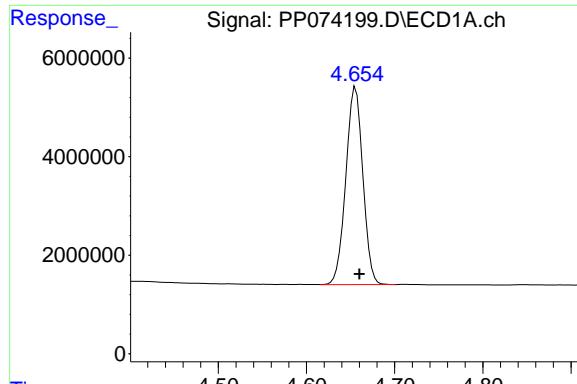


#1 Tetrachloro-m-xylene

R.T.: 4.656 min
Delta R.T.: -0.004 min
Response: 53831323
Conc: 48.14 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
Supervised By :mohammad ahmed 08/08/2025

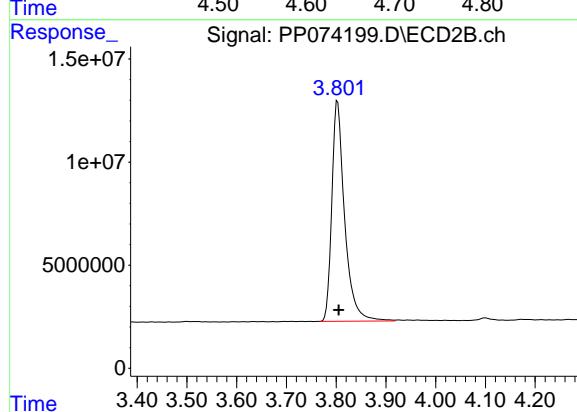


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: -0.003 min
Response: 191609515
Conc: 49.97 ng/ml



#2 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: -0.008 min
Response: 47450930
Conc: 48.86 ng/ml

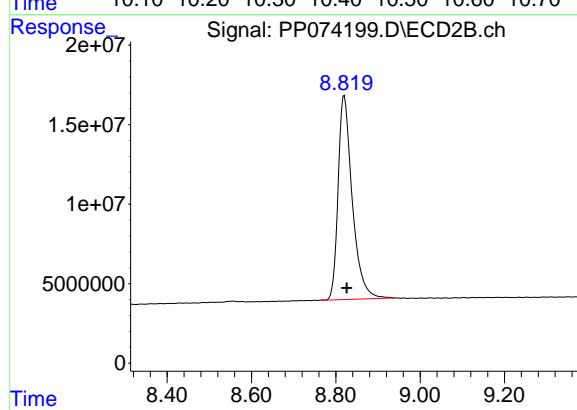

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 299243051
Conc: 49.76 ng/ml





#26 AR-1254-1

R.T.: 6.654 min
 Delta R.T.: -0.004 min
 Response: 27290919
 Conc: 518.43 ng/ml

Instrument : ECD_P
ClientSampleId : ICVPP080125AR1254

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
 Supervised By :mohammad ahmed 08/08/2025

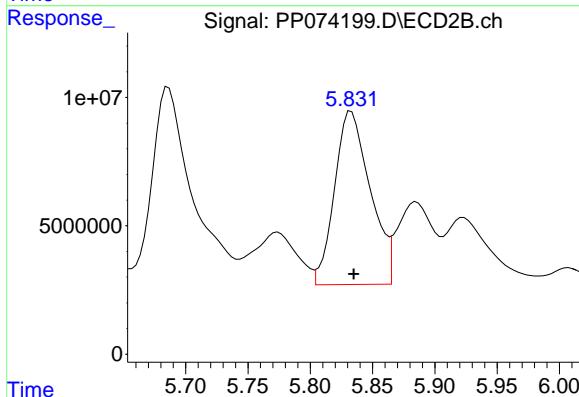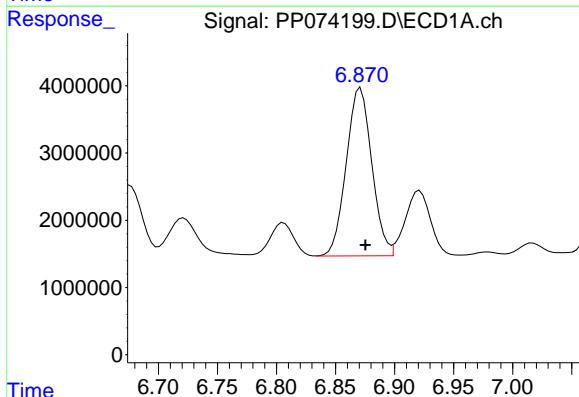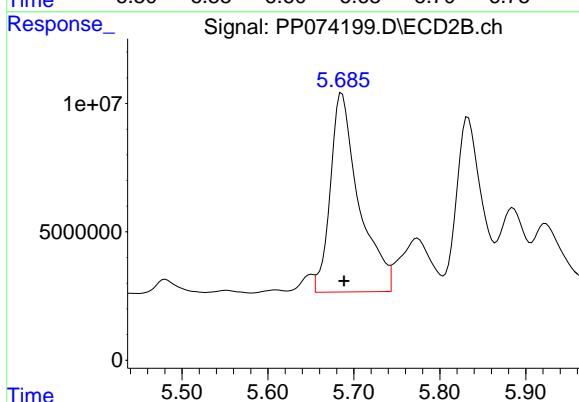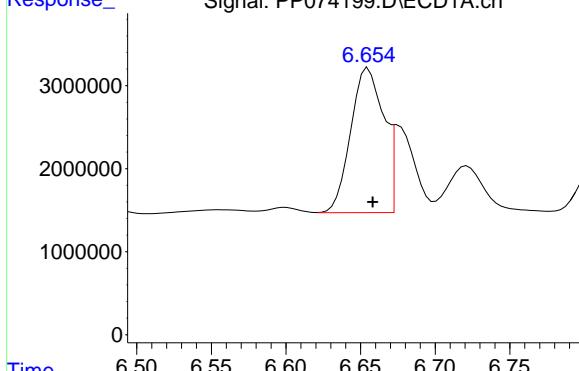

#26 AR-1254-1


R.T.: 5.686 min
 Delta R.T.: -0.002 min
 Response: 178511104
 Conc: 487.49 ng/ml

#27 AR-1254-2

R.T.: 6.871 min
 Delta R.T.: -0.004 min
 Response: 37599140
 Conc: 472.92 ng/ml

#27 AR-1254-2

R.T.: 5.833 min
 Delta R.T.: -0.002 min
 Response: 134837969
 Conc: 484.65 ng/ml

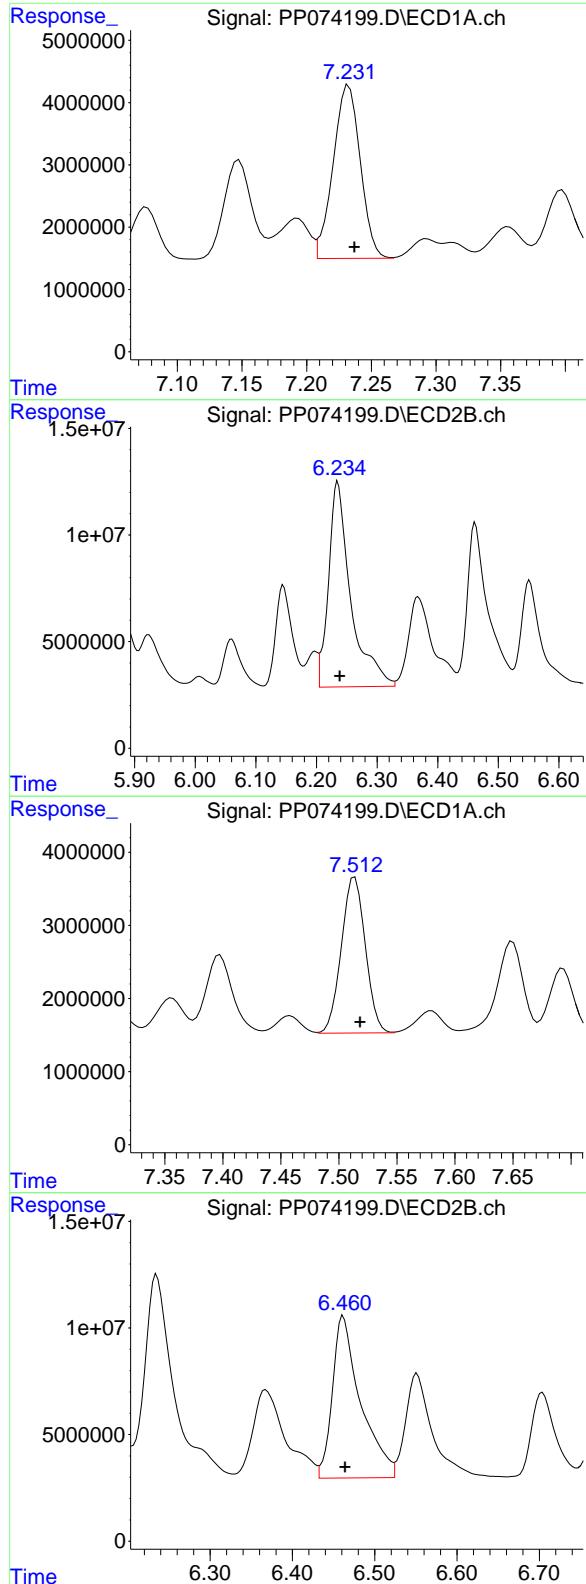

#28 AR-1254-3

R.T.: 7.233 min
 Delta R.T.: -0.004 min
 Response: 40597005
 Conc: 464.94 ng/ml

Instrument : ECD_P
 ClientSampleId : ICP080125AR1254

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
 Supervised By :mohammad ahmed 08/08/2025

#28 AR-1254-3

R.T.: 6.235 min
 Delta R.T.: -0.003 min
 Response: 245151099
 Conc: 501.11 ng/ml

#29 AR-1254-4

R.T.: 7.514 min
 Delta R.T.: -0.005 min
 Response: 30708926
 Conc: 481.26 ng/ml

#29 AR-1254-4

R.T.: 6.462 min
 Delta R.T.: -0.002 min
 Response: 181035006
 Conc: 492.52 ng/ml



#30 AR-1254-5

R.T.: 7.930 min
 Delta R.T.: -0.004 min
 Response: 38809795
 Conc: 478.28 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/08/2025
 Supervised By :mohammad ahmed 08/08/2025

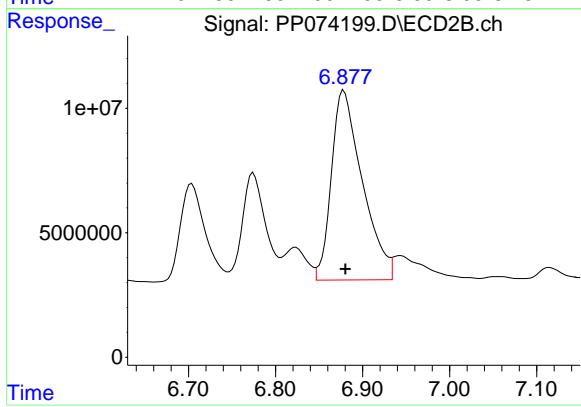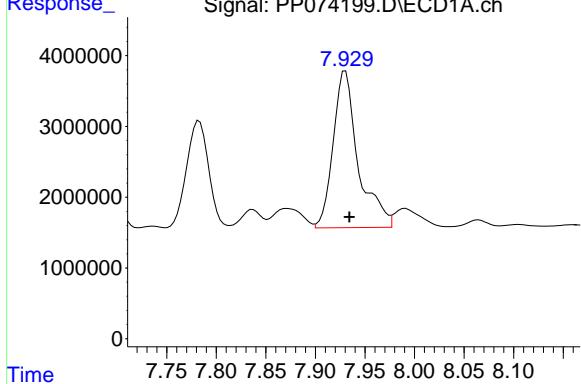

#30 AR-1254-5

R.T.: 6.878 min
 Delta R.T.: -0.002 min
 Response: 188193102
 Conc: 488.60 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 07/23/2025

07/23/2025

Continuing Calib Time: 08:54

Initial Calibration Time(s): 11:32

19:47

GC Column: ZB-MR1

ID: 0.32 (mm)

| COMPOUND | CCAL RT | AVG RT | RT WINDOW FROM | TO | DIFF RT |
|----------------------|---------|--------|----------------|------|---------|
| Aroclor-1016-1 (1) | 4.75 | 4.76 | 4.66 | 4.86 | 0.01 |
| Aroclor-1016-2 (2) | 4.77 | 4.77 | 4.67 | 4.87 | 0.00 |
| Aroclor-1016-3 (3) | 4.83 | 4.83 | 4.73 | 4.93 | 0.00 |
| Aroclor-1016-4 (4) | 4.95 | 4.95 | 4.85 | 5.05 | 0.00 |
| Aroclor-1016-5 (5) | 5.20 | 5.21 | 5.11 | 5.31 | 0.01 |
| Aroclor-1260-1 (1) | 6.24 | 6.25 | 6.15 | 6.35 | 0.01 |
| Aroclor-1260-2 (2) | 6.43 | 6.43 | 6.33 | 6.53 | 0.00 |
| Aroclor-1260-3 (3) | 6.79 | 6.80 | 6.70 | 6.90 | 0.01 |
| Aroclor-1260-4 (4) | 7.05 | 7.06 | 6.96 | 7.16 | 0.01 |
| Aroclor-1260-5 (5) | 7.30 | 7.30 | 7.20 | 7.40 | 0.00 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.57 | 3.77 | 0.01 |
| Decachlorobiphenyl | 8.69 | 8.69 | 8.59 | 8.79 | 0.00 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 07/23/2025

07/23/2025

Continuing Calib Time: 08:54

Initial Calibration Time(s): 11:32

19:47

GC Column: ZB-MR2

ID: 0.32 (mm)

| COMPOUND | CCAL RT | AVG RT | RT WINDOW FROM | TO | DIFF RT |
|----------------------|---------|--------|----------------|------|---------|
| Aroclor-1016-1 (1) | 4.73 | 4.74 | 4.64 | 4.84 | 0.01 |
| Aroclor-1016-2 (2) | 4.75 | 4.76 | 4.66 | 4.86 | 0.01 |
| Aroclor-1016-3 (3) | 4.92 | 4.93 | 4.83 | 5.03 | 0.01 |
| Aroclor-1016-4 (4) | 4.97 | 4.97 | 4.87 | 5.07 | 0.00 |
| Aroclor-1016-5 (5) | 5.18 | 5.19 | 5.09 | 5.29 | 0.01 |
| Aroclor-1260-1 (1) | 6.21 | 6.21 | 6.11 | 6.31 | 0.00 |
| Aroclor-1260-2 (2) | 6.39 | 6.40 | 6.30 | 6.50 | 0.01 |
| Aroclor-1260-3 (3) | 6.55 | 6.55 | 6.45 | 6.65 | 0.00 |
| Aroclor-1260-4 (4) | 7.02 | 7.02 | 6.92 | 7.12 | 0.01 |
| Aroclor-1260-5 (5) | 7.26 | 7.26 | 7.16 | 7.36 | 0.00 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.56 | 3.76 | 0.00 |
| Decachlorobiphenyl | 8.63 | 8.64 | 8.54 | 8.74 | 0.01 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|-----------------|----------------------|--|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| GC Column: | <u>ZB-MR1</u> | ID: <u>0.32</u> (mm) | Initi. Calib. Date(s): <u>07/23/2025</u> <u>07/23/2025</u> |

| | | | |
|--------------------|---------------------|----------------|-------------------|
| Client Sample No.: | <u>CCAL01</u> | Date Analyzed: | <u>08/12/2025</u> |
| Lab Sample No.: | <u>AR1660CCC500</u> | Data File : | <u>PO112850.D</u> |
| | | Time Analyzed: | <u>08:54</u> |

| COMPOUND | RT | RT WINDOW FROM | TO | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|-------|-------------------|-------|--------------------|-------------------|------|
| Aroclor-1016-1 | 4.750 | 4.655 | 4.855 | 651.000 | 500.000 | 30.2 |
| Aroclor-1016-2 | 4.769 | 4.674 | 4.874 | 549.480 | 500.000 | 9.9 |
| Aroclor-1016-3 | 4.826 | 4.731 | 4.931 | 565.780 | 500.000 | 13.2 |
| Aroclor-1016-4 | 4.945 | 4.851 | 5.051 | 571.540 | 500.000 | 14.3 |
| Aroclor-1016-5 | 5.202 | 5.108 | 5.308 | 574.860 | 500.000 | 15.0 |
| Aroclor-1260-1 | 6.238 | 6.145 | 6.345 | 579.220 | 500.000 | 15.8 |
| Aroclor-1260-2 | 6.428 | 6.333 | 6.533 | 547.500 | 500.000 | 9.5 |
| Aroclor-1260-3 | 6.794 | 6.700 | 6.900 | 528.750 | 500.000 | 5.8 |
| Aroclor-1260-4 | 7.053 | 6.959 | 7.159 | 498.850 | 500.000 | -0.2 |
| Aroclor-1260-5 | 7.296 | 7.203 | 7.403 | 553.130 | 500.000 | 10.6 |
| Decachlorobiphenyl | 8.686 | 8.593 | 8.793 | 46.550 | 50.000 | -6.9 |
| Tetrachloro-m-xylene | 3.665 | 3.569 | 3.769 | 60.080 | 50.000 | 20.2 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|-----------------|----------------------|--|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| GC Column: | <u>ZB-MR2</u> | ID: <u>0.32</u> (mm) | Initi. Calib. Date(s): <u>07/23/2025</u> <u>07/23/2025</u> |

| | | | |
|--------------------|---------------------|----------------|-------------------|
| Client Sample No.: | <u>CCAL01</u> | Date Analyzed: | <u>08/12/2025</u> |
| Lab Sample No.: | <u>AR1660CCC500</u> | Data File : | <u>PO112850.D</u> |
| | | Time Analyzed: | <u>08:54</u> |

| COMPOUND | RT | RT WINDOW FROM | TO | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|-------|-------------------|-------|--------------------|-------------------|------|
| Aroclor-1016-1 | 4.731 | 4.638 | 4.838 | 532.580 | 500.000 | 6.5 |
| Aroclor-1016-2 | 4.749 | 4.656 | 4.856 | 524.330 | 500.000 | 4.9 |
| Aroclor-1016-3 | 4.924 | 4.831 | 5.031 | 531.470 | 500.000 | 6.3 |
| Aroclor-1016-4 | 4.966 | 4.873 | 5.073 | 529.880 | 500.000 | 6.0 |
| Aroclor-1016-5 | 5.179 | 5.085 | 5.285 | 523.970 | 500.000 | 4.8 |
| Aroclor-1260-1 | 6.206 | 6.113 | 6.313 | 535.240 | 500.000 | 7.0 |
| Aroclor-1260-2 | 6.394 | 6.302 | 6.502 | 538.810 | 500.000 | 7.8 |
| Aroclor-1260-3 | 6.545 | 6.453 | 6.653 | 559.410 | 500.000 | 11.9 |
| Aroclor-1260-4 | 7.015 | 6.923 | 7.123 | 530.130 | 500.000 | 6.0 |
| Aroclor-1260-5 | 7.257 | 7.164 | 7.364 | 549.900 | 500.000 | 10.0 |
| Decachlorobiphenyl | 8.631 | 8.540 | 8.740 | 52.550 | 50.000 | 5.1 |
| Tetrachloro-m-xylene | 3.658 | 3.562 | 3.762 | 56.390 | 50.000 | 12.8 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 08:54
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:01:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.665 | 3.658 | 488.6E6 | 280.2E6 | 60.081 | 56.386 |
| 2) SA Decachlor... | 8.686 | 8.631 | 340.4E6 | 92854815 | 46.549 | 52.546 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|----------|----------|
| 3) L1 AR-1016-1 | 4.750 | 4.731 | 174.7E6 | 93205664 | 650.999m | 532.582 |
| 4) L1 AR-1016-2 | 4.769 | 4.749 | 223.2E6 | 136.6E6 | 549.476m | 524.330 |
| 5) L1 AR-1016-3 | 4.826 | 4.924 | 148.1E6 | 72262042 | 565.785 | 531.470m |
| 6) L1 AR-1016-4 | 4.945 | 4.966 | 121.1E6 | 58861848 | 571.539 | 529.882m |
| 7) L1 AR-1016-5 | 5.202 | 5.179 | 126.2E6 | 75085975 | 574.857 | 523.966 |
| 31) L7 AR-1260-1 | 6.238 | 6.206 | 254.5E6 | 133.0E6 | 579.224 | 535.236 |
| 32) L7 AR-1260-2 | 6.428 | 6.394 | 376.6E6 | 177.5E6 | 547.504 | 538.814 |
| 33) L7 AR-1260-3 | 6.794 | 6.545 | 310.9E6 | 143.7E6 | 528.746 | 559.414m |
| 34) L7 AR-1260-4 | 7.053 | 7.015 | 225.0E6 | 101.4E6 | 498.852 | 530.125 |
| 35) L7 AR-1260-5 | 7.296 | 7.257 | 685.4E6 | 226.7E6 | 553.135 | 549.898 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 08:54
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:01:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

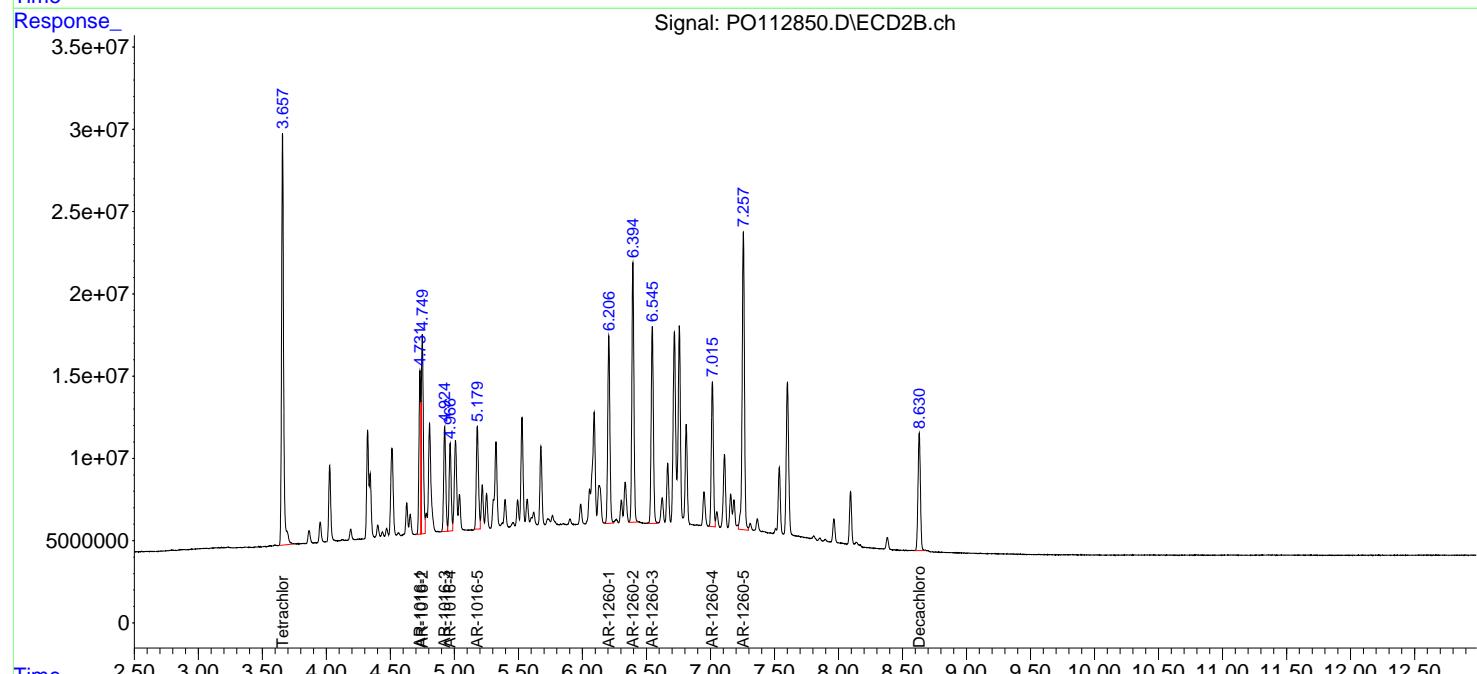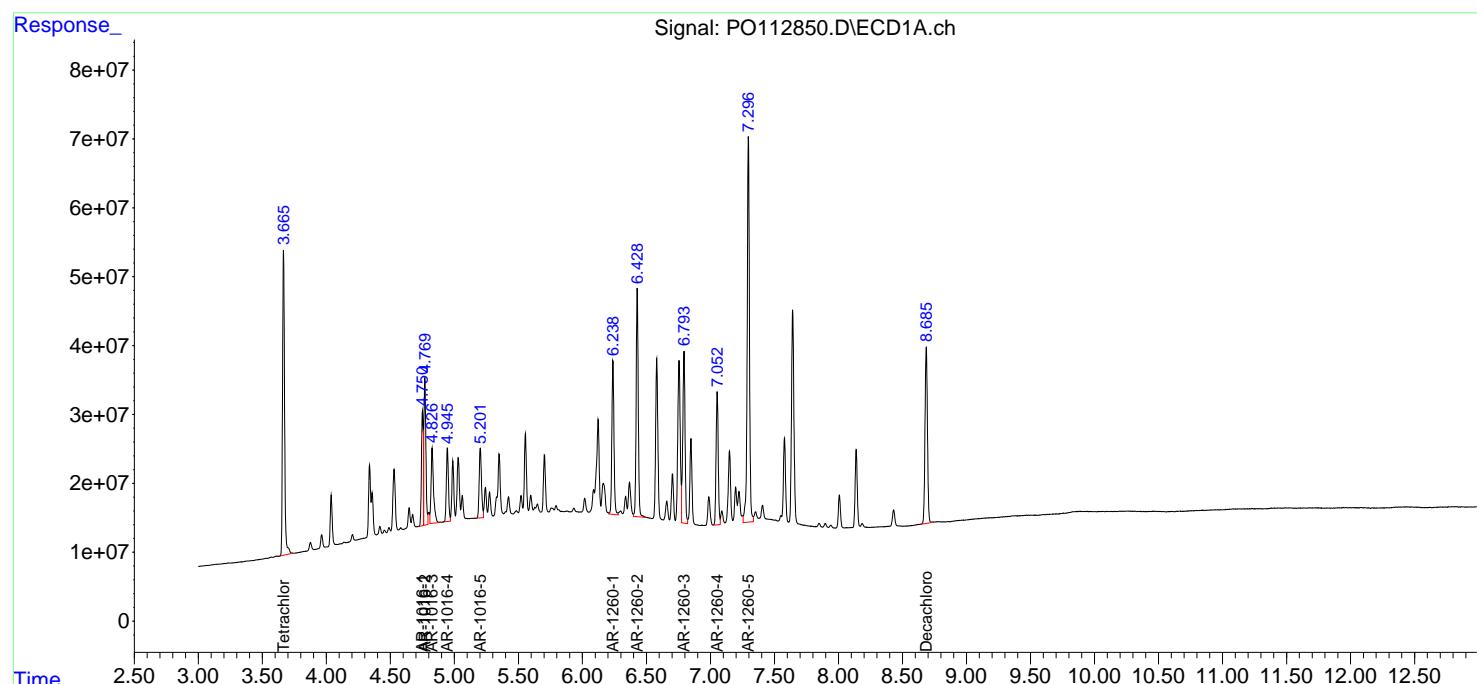

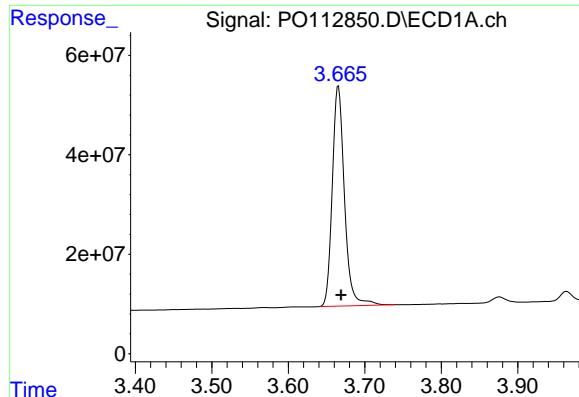


#1 Tetrachloro-m-xylene

R.T.: 3.665 min
Delta R.T.: -0.004 min
Response: 488550662
Conc: 60.08 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

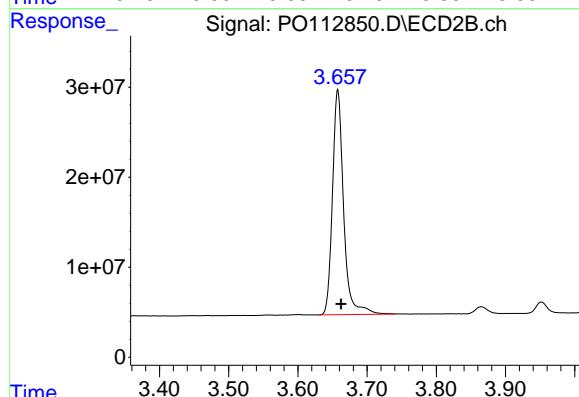


#1 Tetrachloro-m-xylene

R.T.: 3.658 min
Delta R.T.: -0.005 min
Response: 280189739
Conc: 56.39 ng/ml

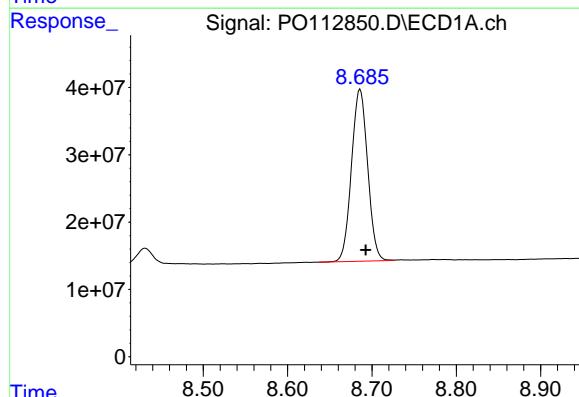


#2 Decachlorobiphenyl

R.T.: 8.686 min
Delta R.T.: -0.007 min
Response: 340356409
Conc: 46.55 ng/ml

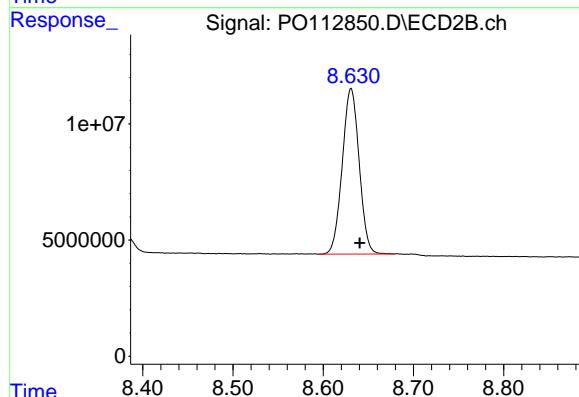

#2 Decachlorobiphenyl

R.T.: 8.631 min
Delta R.T.: -0.010 min
Response: 92854815
Conc: 52.55 ng/ml

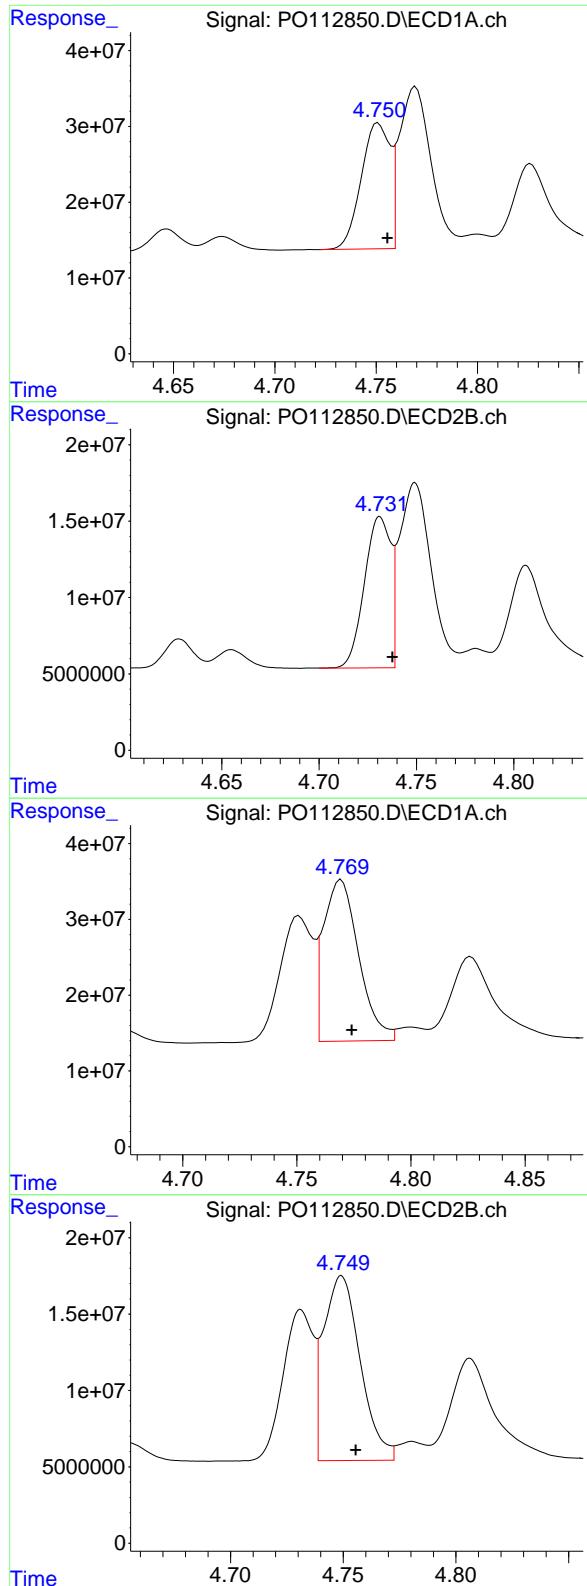

#3 AR-1016-1

R.T.: 4.750 min
 Delta R.T.: -0.005 min
 Response: 174705980
 Conc: 651.00 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#3 AR-1016-1


R.T.: 4.731 min
 Delta R.T.: -0.006 min
 Response: 93205664
 Conc: 532.58 ng/ml

#4 AR-1016-2

R.T.: 4.769 min
 Delta R.T.: -0.005 min
 Response: 223151755
 Conc: 549.48 ng/ml

#4 AR-1016-2

R.T.: 4.749 min
 Delta R.T.: -0.006 min
 Response: 136585485
 Conc: 524.33 ng/ml




#5 AR-1016-3

R.T.: 4.826 min
Delta R.T.: -0.005 min
Response: 148051145
Conc: 565.78 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

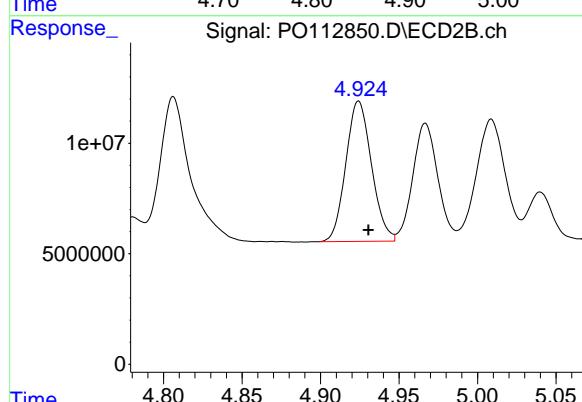


#5 AR-1016-3

R.T.: 4.924 min
Delta R.T.: -0.007 min
Response: 72262042
Conc: 531.47 ng/ml

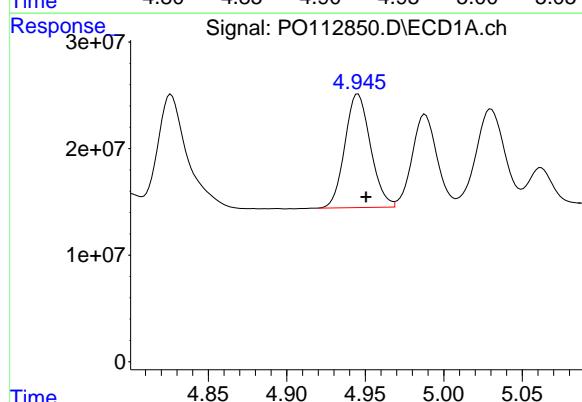


#6 AR-1016-4

R.T.: 4.945 min
Delta R.T.: -0.005 min
Response: 121075575
Conc: 571.54 ng/ml

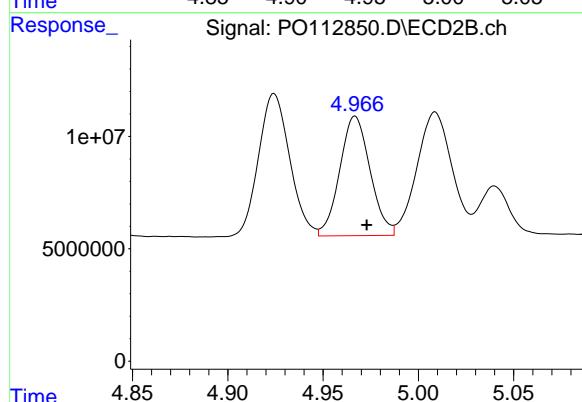

#6 AR-1016-4

R.T.: 4.966 min
Delta R.T.: -0.006 min
Response: 58861848
Conc: 529.88 ng/ml

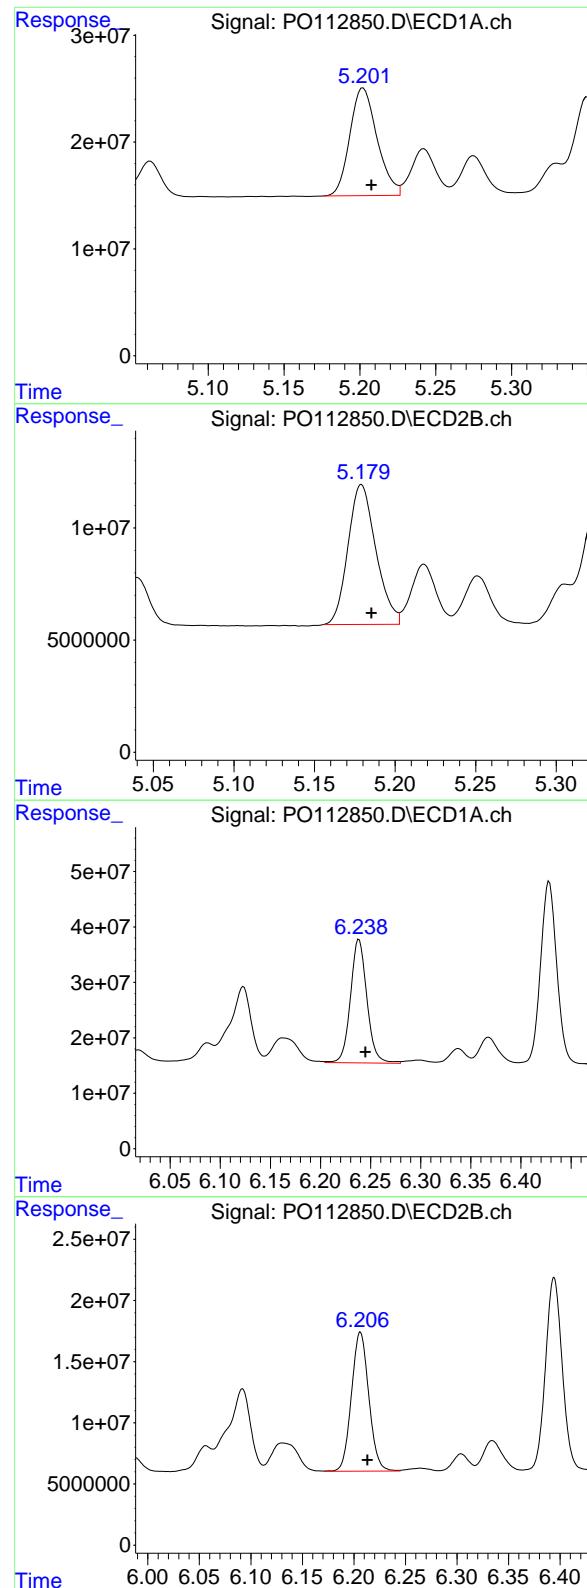

#7 AR-1016-5

R.T.: 5.202 min
 Delta R.T.: -0.005 min
 Response: 126164306
 Conc: 574.86 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#7 AR-1016-5


R.T.: 5.179 min
 Delta R.T.: -0.006 min
 Response: 75085975
 Conc: 523.97 ng/ml

#31 AR-1260-1

R.T.: 6.238 min
 Delta R.T.: -0.006 min
 Response: 254471304
 Conc: 579.22 ng/ml

#31 AR-1260-1

R.T.: 6.206 min
 Delta R.T.: -0.007 min
 Response: 133012078
 Conc: 535.24 ng/ml

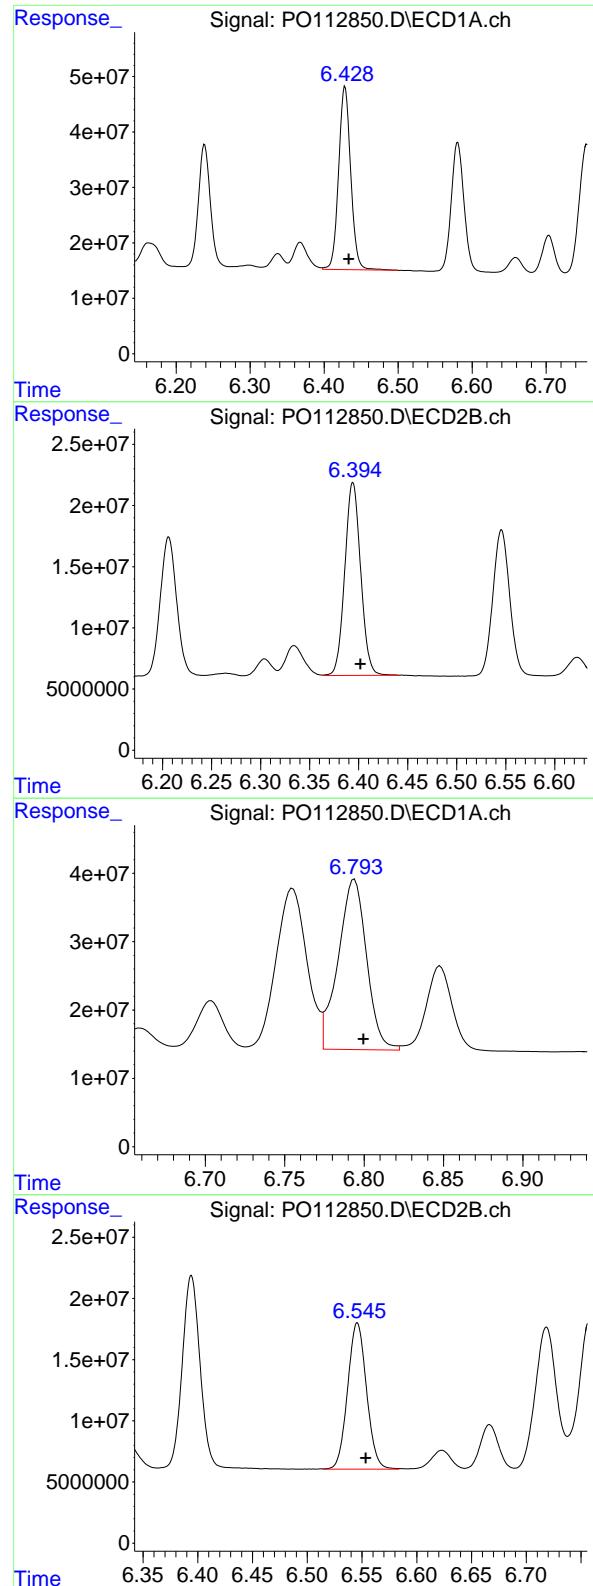

#32 AR-1260-2

R.T.: 6.428 min
 Delta R.T.: -0.005 min
 Response: 376624885
 Conc: 547.50 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#32 AR-1260-2





R.T.: 6.394 min
 Delta R.T.: -0.008 min
 Response: 177535660
 Conc: 538.81 ng/ml

#33 AR-1260-3

R.T.: 6.794 min
 Delta R.T.: -0.006 min
 Response: 310912948
 Conc: 528.75 ng/ml

#33 AR-1260-3

R.T.: 6.545 min
 Delta R.T.: -0.008 min
 Response: 143725245
 Conc: 559.41 ng/ml

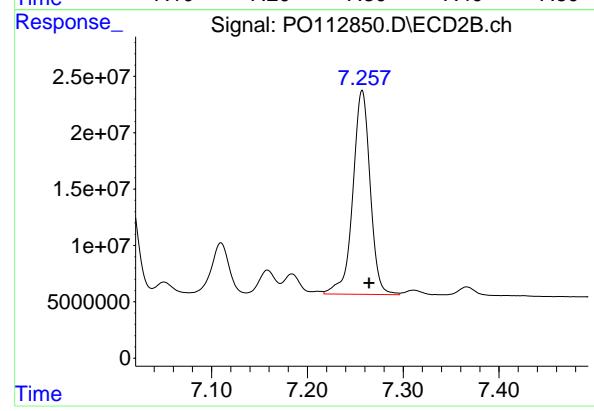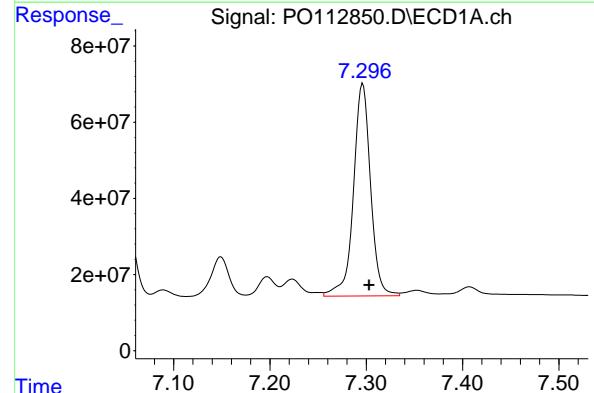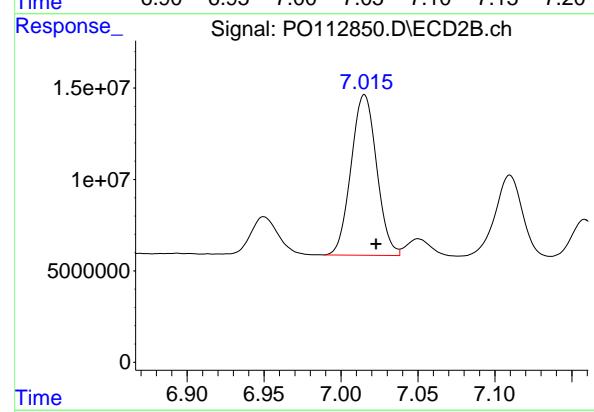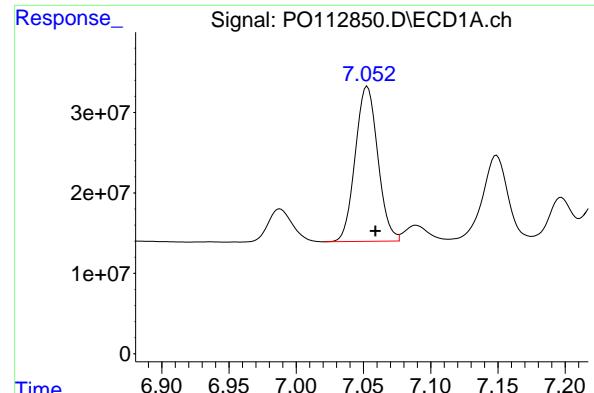

#34 AR-1260-4

R.T.: 7.053 min
 Delta R.T.: -0.006 min
 Response: 224984392
 Conc: 498.85 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#34 AR-1260-4

R.T.: 7.015 min
 Delta R.T.: -0.007 min
 Response: 101418669
 Conc: 530.13 ng/ml

#35 AR-1260-5

R.T.: 7.296 min
 Delta R.T.: -0.006 min
 Response: 685410891
 Conc: 553.13 ng/ml

#35 AR-1260-5

R.T.: 7.257 min
 Delta R.T.: -0.007 min
 Response: 226664288
 Conc: 549.90 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 07/23/2025

07/23/2025

Continuing Calib Time: 15:50

Initial Calibration Time(s): 11:32

19:47

GC Column: ZB-MR1

ID: 0.32 (mm)

| COMPOUND | CCAL RT | Avg RT | RT Window From | TO | Diff RT |
|----------------------|---------|--------|----------------|------|---------|
| Aroclor-1016-1 (1) | 4.75 | 4.76 | 4.66 | 4.86 | 0.01 |
| Aroclor-1016-2 (2) | 4.77 | 4.77 | 4.67 | 4.87 | 0.00 |
| Aroclor-1016-3 (3) | 4.83 | 4.83 | 4.73 | 4.93 | 0.00 |
| Aroclor-1016-4 (4) | 4.95 | 4.95 | 4.85 | 5.05 | 0.00 |
| Aroclor-1016-5 (5) | 5.20 | 5.21 | 5.11 | 5.31 | 0.01 |
| Aroclor-1260-1 (1) | 6.24 | 6.25 | 6.15 | 6.35 | 0.01 |
| Aroclor-1260-2 (2) | 6.43 | 6.43 | 6.33 | 6.53 | 0.00 |
| Aroclor-1260-3 (3) | 6.80 | 6.80 | 6.70 | 6.90 | 0.00 |
| Aroclor-1260-4 (4) | 7.06 | 7.06 | 6.96 | 7.16 | 0.01 |
| Aroclor-1260-5 (5) | 7.30 | 7.30 | 7.20 | 7.40 | 0.00 |
| Tetrachloro-m-xylene | 3.67 | 3.67 | 3.57 | 3.77 | 0.00 |
| Decachlorobiphenyl | 8.69 | 8.69 | 8.59 | 8.79 | 0.00 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 07/23/2025

07/23/2025

Continuing Calib Time: 15:50

Initial Calibration Time(s): 11:32

19:47

GC Column: ZB-MR2

ID: 0.32 (mm)

| COMPOUND | CCAL RT | AVG RT | RT WINDOW FROM | TO | DIFF RT |
|----------------------|---------|--------|----------------|------|---------|
| Aroclor-1016-1 (1) | 4.73 | 4.74 | 4.64 | 4.84 | 0.01 |
| Aroclor-1016-2 (2) | 4.75 | 4.76 | 4.66 | 4.86 | 0.01 |
| Aroclor-1016-3 (3) | 4.93 | 4.93 | 4.83 | 5.03 | 0.00 |
| Aroclor-1016-4 (4) | 4.97 | 4.97 | 4.87 | 5.07 | 0.00 |
| Aroclor-1016-5 (5) | 5.18 | 5.19 | 5.09 | 5.29 | 0.01 |
| Aroclor-1260-1 (1) | 6.21 | 6.21 | 6.11 | 6.31 | 0.00 |
| Aroclor-1260-2 (2) | 6.40 | 6.40 | 6.30 | 6.50 | 0.00 |
| Aroclor-1260-3 (3) | 6.55 | 6.55 | 6.45 | 6.65 | 0.00 |
| Aroclor-1260-4 (4) | 7.02 | 7.02 | 6.92 | 7.12 | 0.00 |
| Aroclor-1260-5 (5) | 7.26 | 7.26 | 7.16 | 7.36 | 0.00 |
| Tetrachloro-m-xylene | 3.66 | 3.66 | 3.56 | 3.76 | 0.00 |
| Decachlorobiphenyl | 8.63 | 8.64 | 8.54 | 8.74 | 0.01 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|----------|---------------|--|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| GC Column: | ZB-MR1 | ID: 0.32 (mm) | Initi. Calib. Date(s): 07/23/2025 07/23/2025 |

| | | | |
|--------------------|--------------|----------------|------------|
| Client Sample No.: | CCAL02 | Date Analyzed: | 08/12/2025 |
| Lab Sample No.: | AR1660CCC500 | Data File : | PO112865.D |
| | | Time Analyzed: | 15:50 |

| COMPOUND | RT | RT WINDOW FROM TO | | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|-------|----------------------|-------|--------------------|-------------------|------|
| Aroclor-1016-1 | 4.751 | 4.655 | 4.855 | 524.640 | 500.000 | 4.9 |
| Aroclor-1016-2 | 4.769 | 4.674 | 4.874 | 553.430 | 500.000 | 10.7 |
| Aroclor-1016-3 | 4.827 | 4.731 | 4.931 | 551.220 | 500.000 | 10.2 |
| Aroclor-1016-4 | 4.947 | 4.851 | 5.051 | 550.720 | 500.000 | 10.1 |
| Aroclor-1016-5 | 5.203 | 5.108 | 5.308 | 584.150 | 500.000 | 16.8 |
| Aroclor-1260-1 | 6.240 | 6.145 | 6.345 | 550.350 | 500.000 | 10.1 |
| Aroclor-1260-2 | 6.430 | 6.333 | 6.533 | 543.410 | 500.000 | 8.7 |
| Aroclor-1260-3 | 6.795 | 6.700 | 6.900 | 570.950 | 500.000 | 14.2 |
| Aroclor-1260-4 | 7.055 | 6.959 | 7.159 | 542.260 | 500.000 | 8.5 |
| Aroclor-1260-5 | 7.297 | 7.203 | 7.403 | 529.970 | 500.000 | 6.0 |
| Decachlorobiphenyl | 8.687 | 8.593 | 8.793 | 48.970 | 50.000 | -2.1 |
| Tetrachloro-m-xylene | 3.667 | 3.569 | 3.769 | 57.760 | 50.000 | 15.5 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|----------|---------------|--|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| GC Column: | ZB-MR2 | ID: 0.32 (mm) | Initi. Calib. Date(s): 07/23/2025 07/23/2025 |

| | | | |
|--------------------|--------------|----------------|------------|
| Client Sample No.: | CCAL02 | Date Analyzed: | 08/12/2025 |
| Lab Sample No.: | AR1660CCC500 | Data File : | PO112865.D |
| | | Time Analyzed: | 15:50 |

| COMPOUND | RT | RT WINDOW FROM TO | | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|-------|----------------------|-------|--------------------|-------------------|------|
| Aroclor-1016-1 | 4.734 | 4.638 | 4.838 | 522.080 | 500.000 | 4.4 |
| Aroclor-1016-2 | 4.751 | 4.656 | 4.856 | 517.090 | 500.000 | 3.4 |
| Aroclor-1016-3 | 4.926 | 4.831 | 5.031 | 516.260 | 500.000 | 3.3 |
| Aroclor-1016-4 | 4.969 | 4.873 | 5.073 | 515.840 | 500.000 | 3.2 |
| Aroclor-1016-5 | 5.181 | 5.085 | 5.285 | 527.110 | 500.000 | 5.4 |
| Aroclor-1260-1 | 6.208 | 6.113 | 6.313 | 523.960 | 500.000 | 4.8 |
| Aroclor-1260-2 | 6.396 | 6.302 | 6.502 | 531.850 | 500.000 | 6.4 |
| Aroclor-1260-3 | 6.547 | 6.453 | 6.653 | 550.200 | 500.000 | 10.0 |
| Aroclor-1260-4 | 7.017 | 6.923 | 7.123 | 543.780 | 500.000 | 8.8 |
| Aroclor-1260-5 | 7.260 | 7.164 | 7.364 | 560.820 | 500.000 | 12.2 |
| Decachlorobiphenyl | 8.633 | 8.540 | 8.740 | 53.180 | 50.000 | 6.4 |
| Tetrachloro-m-xylene | 3.659 | 3.562 | 3.762 | 55.270 | 50.000 | 10.5 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:50
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:39:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.667 | 3.659 | 469.7E6 | 274.6E6 | 57.765 | 55.269 |
| 2) SA Decachlor... | 8.687 | 8.633 | 358.1E6 | 93971024 | 48.973 | 53.178 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|----------|----------|
| 3) L1 AR-1016-1 | 4.751 | 4.734 | 140.8E6 | 91367071 | 524.643m | 522.077 |
| 4) L1 AR-1016-2 | 4.769 | 4.751 | 224.8E6 | 134.7E6 | 553.429m | 517.092 |
| 5) L1 AR-1016-3 | 4.827 | 4.926 | 144.2E6 | 70193896 | 551.218 | 516.259 |
| 6) L1 AR-1016-4 | 4.947 | 4.969 | 116.7E6 | 57301939 | 550.721 | 515.840 |
| 7) L1 AR-1016-5 | 5.203 | 5.181 | 128.2E6 | 75537038 | 584.153 | 527.114 |
| 31) L7 AR-1260-1 | 6.240 | 6.208 | 241.8E6 | 130.2E6 | 550.345 | 523.958 |
| 32) L7 AR-1260-2 | 6.430 | 6.396 | 373.8E6 | 175.2E6 | 543.411 | 531.849 |
| 33) L7 AR-1260-3 | 6.795 | 6.547 | 335.7E6 | 141.4E6 | 570.949 | 550.198m |
| 34) L7 AR-1260-4 | 7.055 | 7.017 | 244.6E6 | 104.0E6 | 542.265 | 543.785 |
| 35) L7 AR-1260-5 | 7.297 | 7.260 | 656.7E6 | 231.2E6 | 529.972 | 560.820 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:50
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:39:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

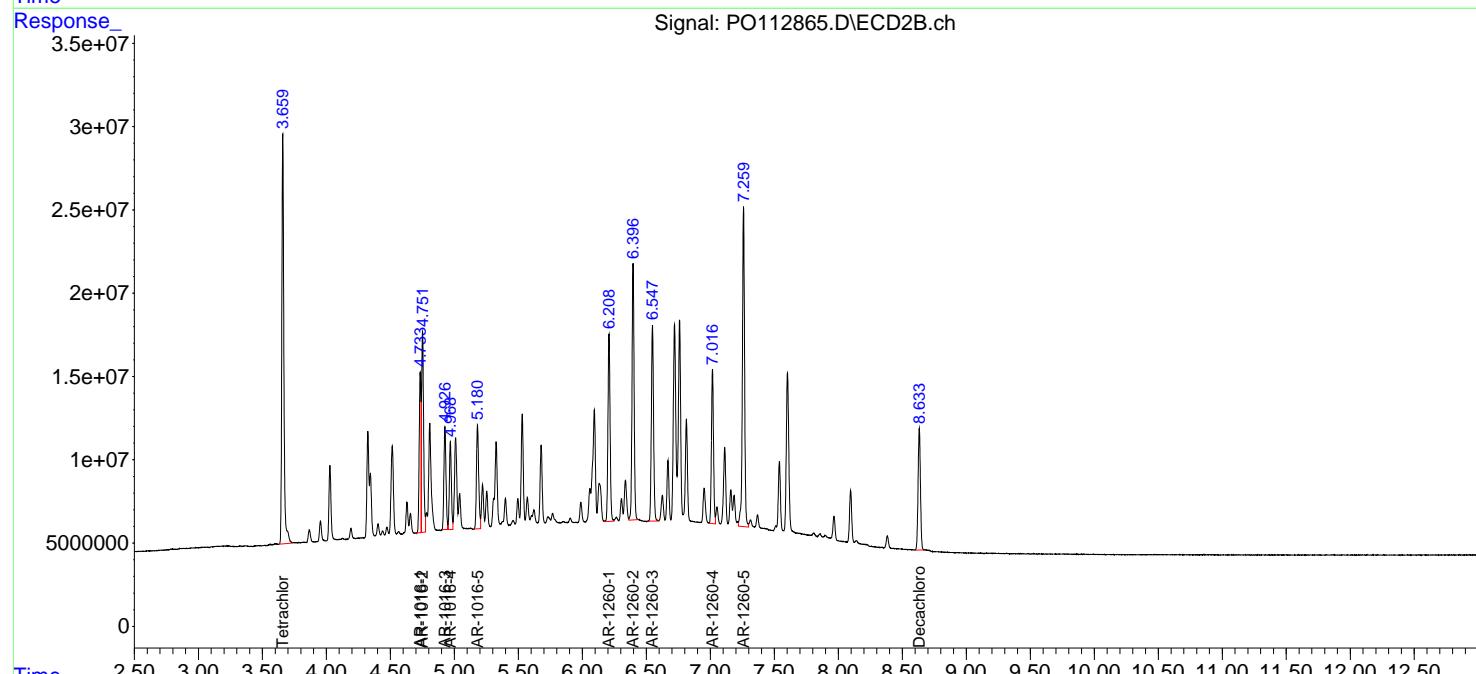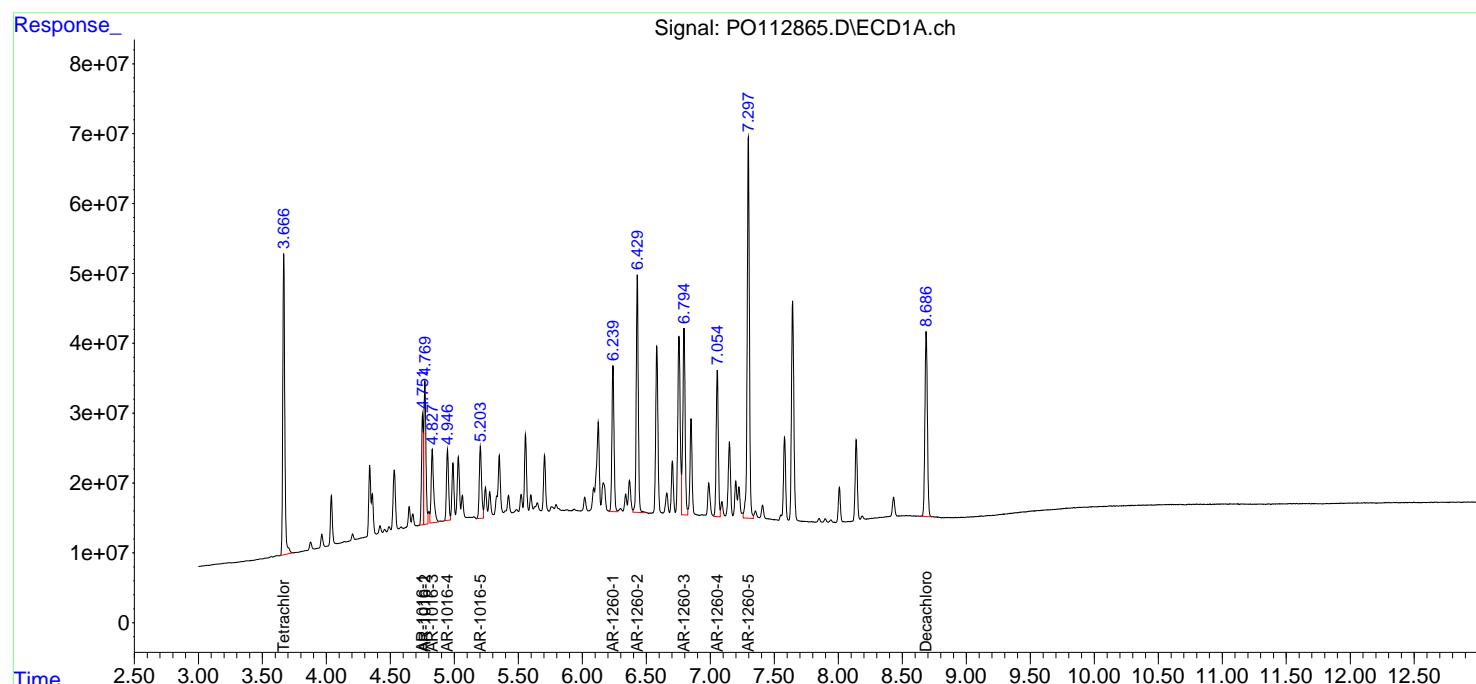

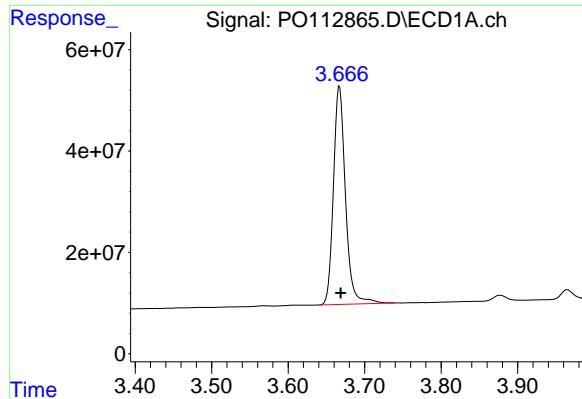


#1 Tetrachloro-m-xylene

R.T.: 3.667 min
Delta R.T.: -0.002 min
Response: 469719514
Conc: 57.76 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

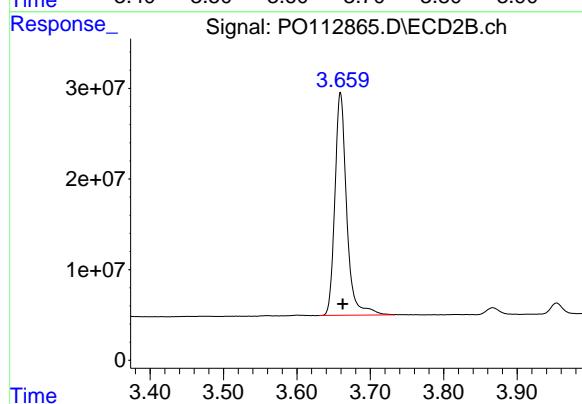


#1 Tetrachloro-m-xylene

R.T.: 3.659 min
Delta R.T.: -0.003 min
Response: 274642690
Conc: 55.27 ng/ml

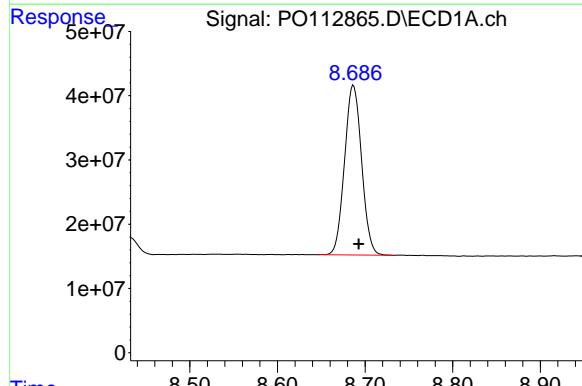


#2 Decachlorobiphenyl

R.T.: 8.687 min
Delta R.T.: -0.006 min
Response: 358077397
Conc: 48.97 ng/ml

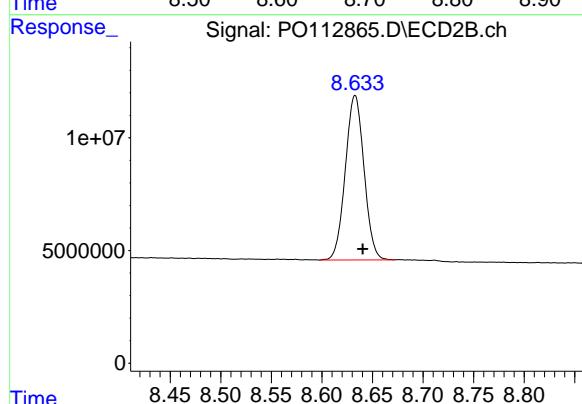

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.008 min
Response: 93971024
Conc: 53.18 ng/ml

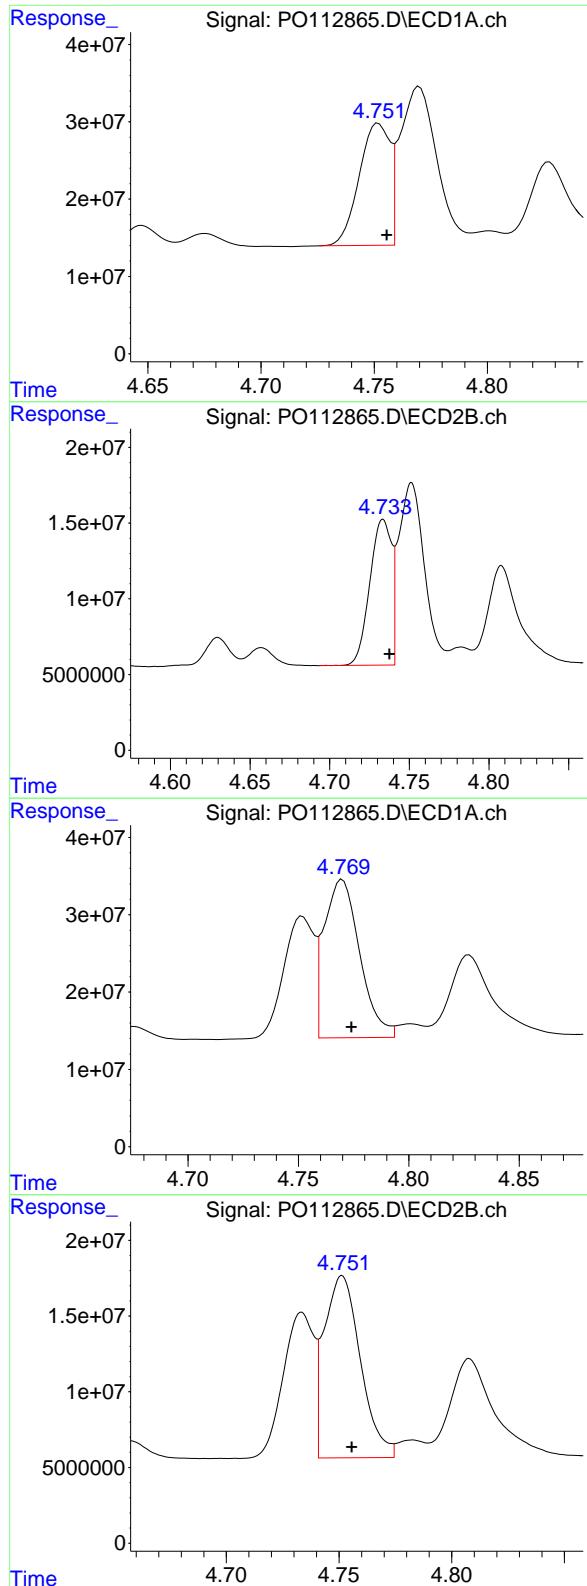

#3 AR-1016-1

R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 140796148
 Conc: 524.64 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#3 AR-1016-1


R.T.: 4.734 min
 Delta R.T.: -0.004 min
 Response: 91367071
 Conc: 522.08 ng/ml

#4 AR-1016-2

R.T.: 4.769 min
 Delta R.T.: -0.005 min
 Response: 224757096
 Conc: 553.43 ng/ml

#4 AR-1016-2

R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 134699953
 Conc: 517.09 ng/ml

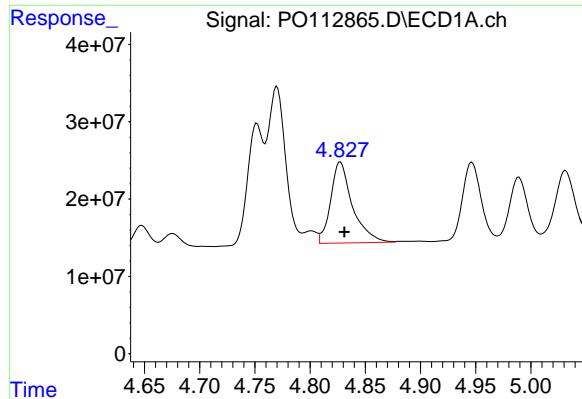


#5 AR-1016-3

R.T.: 4.827 min
Delta R.T.: -0.004 min
Response: 144239367
Conc: 551.22 ng/ml

Instrument:
ECD_O
ClientSampleId :
AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

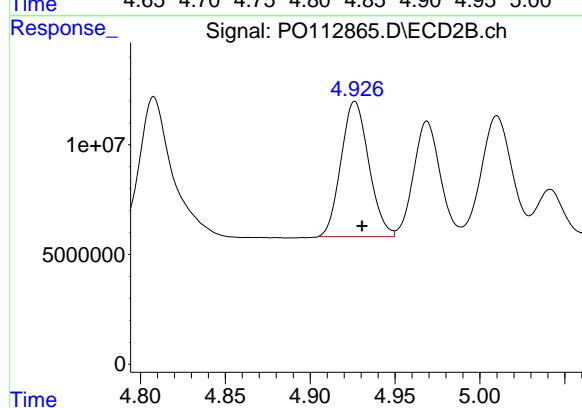


#5 AR-1016-3

R.T.: 4.926 min
Delta R.T.: -0.004 min
Response: 70193896
Conc: 516.26 ng/ml

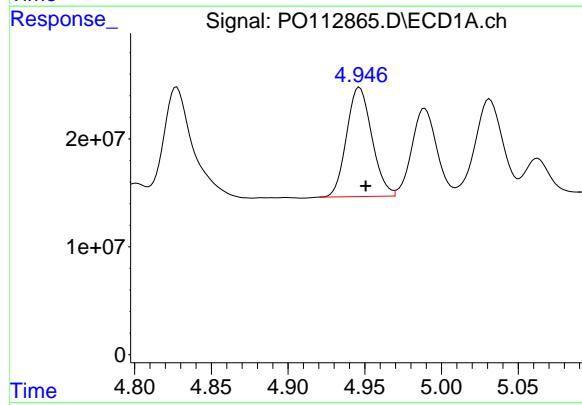


#6 AR-1016-4

R.T.: 4.947 min
Delta R.T.: -0.004 min
Response: 116665542
Conc: 550.72 ng/ml

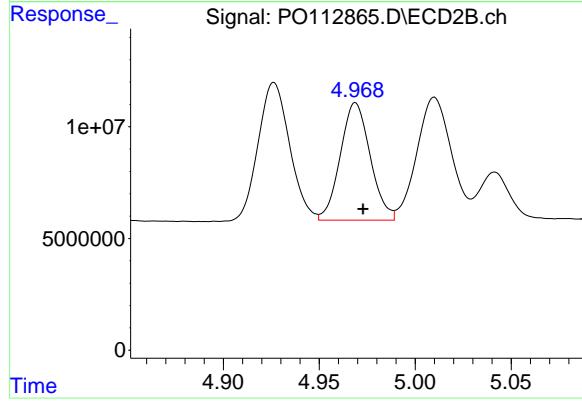

#6 AR-1016-4

R.T.: 4.969 min
Delta R.T.: -0.004 min
Response: 57301939
Conc: 515.84 ng/ml

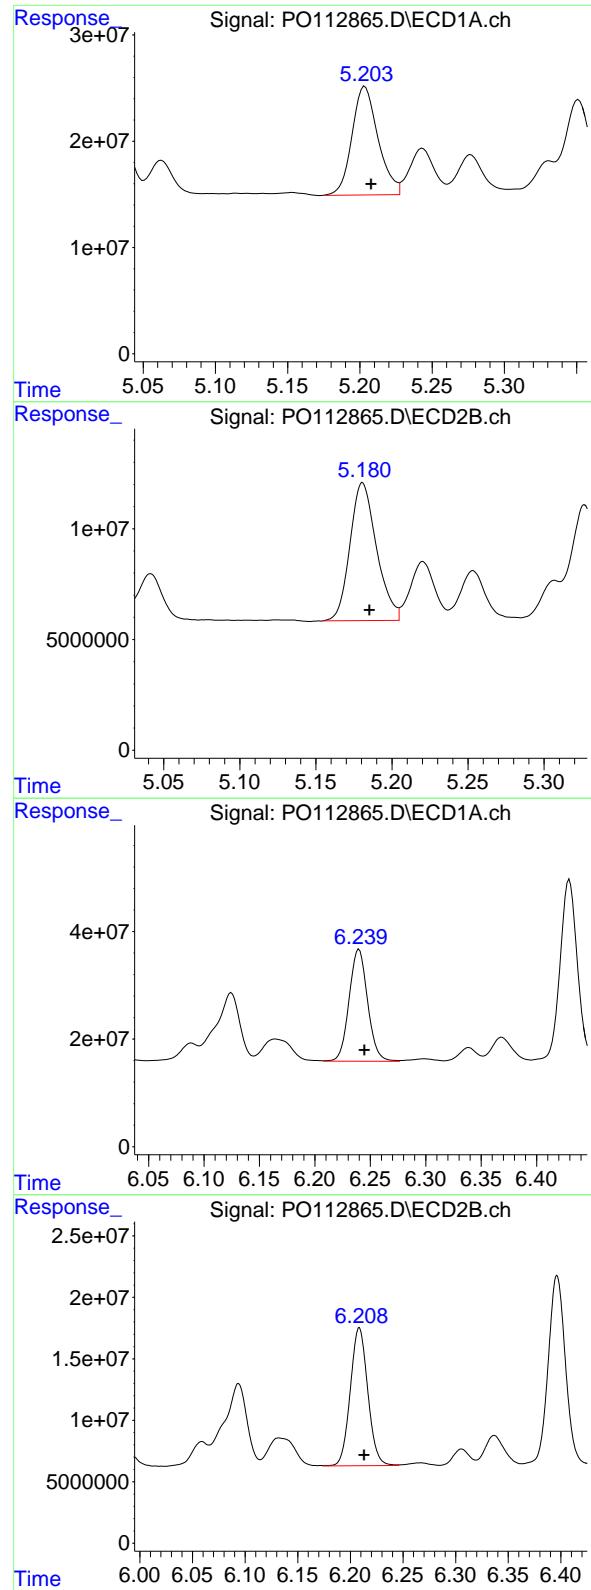

#7 AR-1016-5

R.T.: 5.203 min
 Delta R.T.: -0.004 min
 Response: 128204484
 Conc: 584.15 ng/ml

Instrument:
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#7 AR-1016-5


R.T.: 5.181 min
 Delta R.T.: -0.005 min
 Response: 75537038
 Conc: 527.11 ng/ml

#31 AR-1260-1

R.T.: 6.240 min
 Delta R.T.: -0.005 min
 Response: 241783854
 Conc: 550.35 ng/ml

#31 AR-1260-1

R.T.: 6.208 min
 Delta R.T.: -0.005 min
 Response: 130209411
 Conc: 523.96 ng/ml

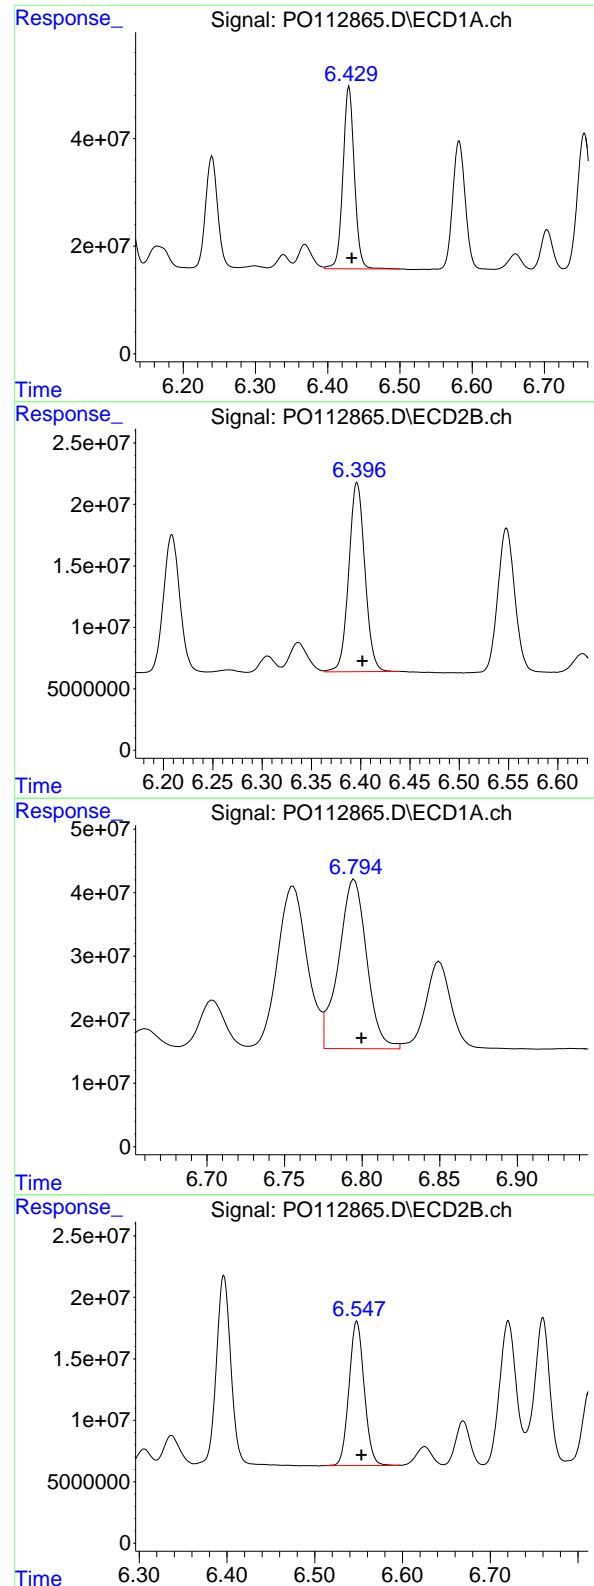

#32 AR-1260-2

R.T.: 6.430 min
 Delta R.T.: -0.004 min
 Response: 373809275
 Conc: 543.41 ng/ml

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#32 AR-1260-2


R.T.: 6.396 min
 Delta R.T.: -0.006 min
 Response: 175240912
 Conc: 531.85 ng/ml

#33 AR-1260-3

R.T.: 6.795 min
 Delta R.T.: -0.005 min
 Response: 335729402
 Conc: 570.95 ng/ml

#33 AR-1260-3

R.T.: 6.547 min
 Delta R.T.: -0.006 min
 Response: 141357365
 Conc: 550.20 ng/ml

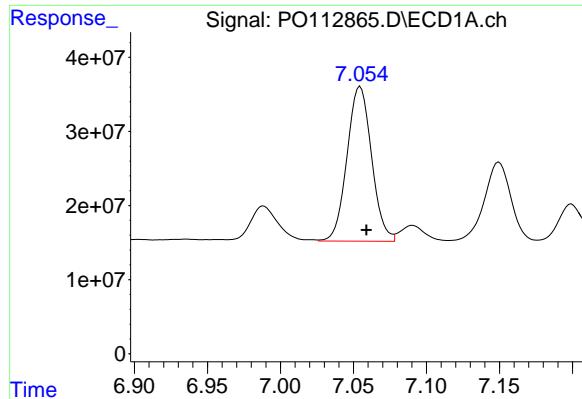


#34 AR-1260-4

R.T.: 7.055 min
Delta R.T.: -0.004 min
Response: 244563892
Conc: 542.26 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

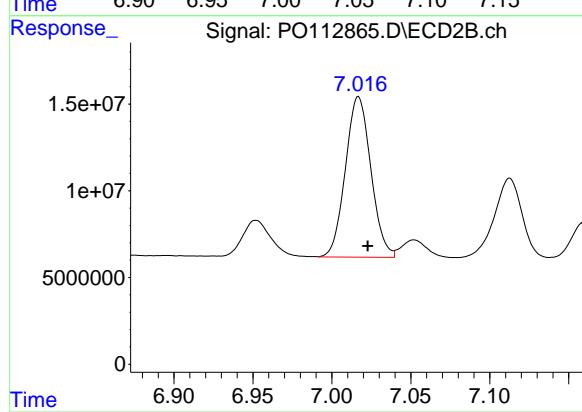


#34 AR-1260-4

R.T.: 7.017 min
Delta R.T.: -0.006 min
Response: 104031834
Conc: 543.78 ng/ml

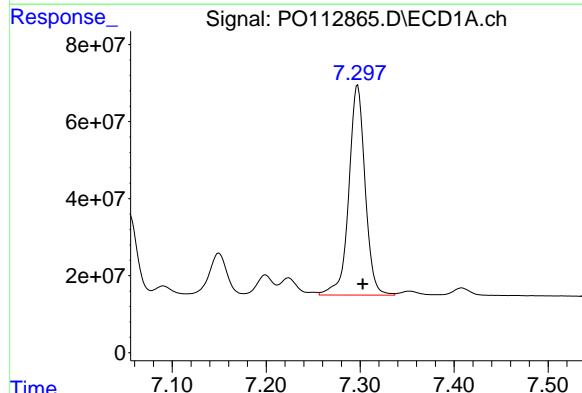

#35 AR-1260-5

R.T.: 7.297 min
Delta R.T.: -0.005 min
Response: 656708588
Conc: 529.97 ng/ml

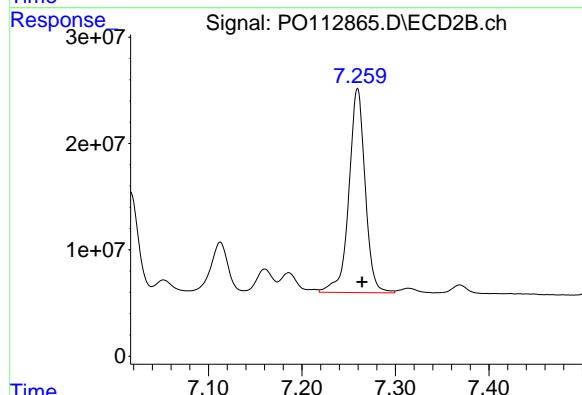

#35 AR-1260-5

R.T.: 7.260 min
Delta R.T.: -0.005 min
Response: 231166363
Conc: 560.82 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 08/01/2025

08/01/2025

Continuing Calib Time: 09:51

Initial Calibration Time(s): 12:05

20:28

GC Column: ZB-MR1

ID: 0.32 (mm)

| COMPOUND | CCAL RT | Avg RT | RT Window From | TO | Diff RT |
|----------------------|---------|--------|----------------|-------|---------|
| Aroclor-1016-1 (1) | 5.81 | 5.81 | 5.71 | 5.91 | 0.00 |
| Aroclor-1016-2 (2) | 5.83 | 5.83 | 5.73 | 5.93 | 0.00 |
| Aroclor-1016-3 (3) | 5.89 | 5.90 | 5.80 | 6.00 | 0.01 |
| Aroclor-1016-4 (4) | 5.99 | 5.99 | 5.89 | 6.09 | 0.00 |
| Aroclor-1016-5 (5) | 6.28 | 6.29 | 6.19 | 6.39 | 0.01 |
| Aroclor-1260-1 (1) | 7.40 | 7.40 | 7.30 | 7.50 | 0.00 |
| Aroclor-1260-2 (2) | 7.65 | 7.66 | 7.56 | 7.76 | 0.01 |
| Aroclor-1260-3 (3) | 8.01 | 8.01 | 7.91 | 8.11 | 0.00 |
| Aroclor-1260-4 (4) | 8.24 | 8.24 | 8.14 | 8.34 | 0.00 |
| Aroclor-1260-5 (5) | 8.56 | 8.57 | 8.47 | 8.67 | 0.01 |
| Tetrachloro-m-xylene | 4.66 | 4.66 | 4.56 | 4.76 | 0.00 |
| Decachlorobiphenyl | 10.43 | 10.44 | 10.34 | 10.54 | 0.01 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 08/01/2025

08/01/2025

Continuing Calib Time: 09:51

Initial Calibration Time(s): 12:05

20:28

GC Column: ZB-MR2

ID: 0.32 (mm)

| COMPOUND | CCAL RT | AVG RT | RT WINDOW FROM | TO | DIFF RT |
|----------------------|---------|--------|----------------|------|---------|
| Aroclor-1016-1 (1) | 4.90 | 4.91 | 4.81 | 5.01 | 0.01 |
| Aroclor-1016-2 (2) | 4.96 | 4.96 | 4.86 | 5.06 | 0.00 |
| Aroclor-1016-3 (3) | 5.08 | 5.08 | 4.98 | 5.18 | 0.00 |
| Aroclor-1016-4 (4) | 5.12 | 5.12 | 5.02 | 5.22 | 0.00 |
| Aroclor-1016-5 (5) | 5.34 | 5.34 | 5.24 | 5.44 | 0.00 |
| Aroclor-1260-1 (1) | 6.55 | 6.56 | 6.46 | 6.66 | 0.01 |
| Aroclor-1260-2 (2) | 6.71 | 6.71 | 6.61 | 6.81 | 0.01 |
| Aroclor-1260-3 (3) | 6.92 | 6.92 | 6.82 | 7.02 | 0.01 |
| Aroclor-1260-4 (4) | 7.17 | 7.18 | 7.08 | 7.28 | 0.01 |
| Aroclor-1260-5 (5) | 7.41 | 7.42 | 7.32 | 7.52 | 0.01 |
| Tetrachloro-m-xylene | 3.80 | 3.81 | 3.71 | 3.91 | 0.01 |
| Decachlorobiphenyl | 8.82 | 8.83 | 8.73 | 8.93 | 0.01 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|----------|---------------|--|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| GC Column: | ZB-MR1 | ID: 0.32 (mm) | Initi. Calib. Date(s): 08/01/2025 08/01/2025 |

| | | | |
|--------------------|--------------|----------------|------------|
| Client Sample No.: | CCAL03 | Date Analyzed: | 08/12/2025 |
| Lab Sample No.: | AR1660CCC500 | Data File : | PP074302.D |
| | | Time Analyzed: | 09:51 |

| COMPOUND | RT | RT WINDOW FROM TO | | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|--------|----------------------|--------|--------------------|-------------------|------|
| Aroclor-1016-1 | 5.809 | 5.712 | 5.912 | 541.110 | 500.000 | 8.2 |
| Aroclor-1016-2 | 5.830 | 5.733 | 5.933 | 542.210 | 500.000 | 8.4 |
| Aroclor-1016-3 | 5.894 | 5.796 | 5.996 | 546.140 | 500.000 | 9.2 |
| Aroclor-1016-4 | 5.990 | 5.893 | 6.093 | 549.740 | 500.000 | 9.9 |
| Aroclor-1016-5 | 6.283 | 6.186 | 6.386 | 547.590 | 500.000 | 9.5 |
| Aroclor-1260-1 | 7.400 | 7.303 | 7.503 | 520.400 | 500.000 | 4.1 |
| Aroclor-1260-2 | 7.653 | 7.555 | 7.755 | 502.220 | 500.000 | 0.4 |
| Aroclor-1260-3 | 8.010 | 7.913 | 8.113 | 510.120 | 500.000 | 2.0 |
| Aroclor-1260-4 | 8.239 | 8.142 | 8.342 | 508.850 | 500.000 | 1.8 |
| Aroclor-1260-5 | 8.564 | 8.468 | 8.668 | 488.630 | 500.000 | -2.3 |
| Decachlorobiphenyl | 10.432 | 10.338 | 10.538 | 50.860 | 50.000 | 1.7 |
| Tetrachloro-m-xylene | 4.657 | 4.560 | 4.760 | 56.700 | 50.000 | 13.4 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|-----------------|----------------------|--|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| GC Column: | <u>ZB-MR2</u> | ID: <u>0.32</u> (mm) | Initi. Calib. Date(s): <u>08/01/2025</u> <u>08/01/2025</u> |

| | | | |
|--------------------|---------------------|----------------|-------------------|
| Client Sample No.: | <u>CCAL03</u> | Date Analyzed: | <u>08/12/2025</u> |
| Lab Sample No.: | <u>AR1660CCC500</u> | Data File : | <u>PP074302.D</u> |
| | | Time Analyzed: | <u>09:51</u> |

| COMPOUND | RT | RT WINDOW FROM | | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|-------|-------------------|-------|--------------------|-------------------|------|
| | | TO | | | | |
| Aroclor-1016-1 | 4.901 | 4.806 | 5.006 | 583.180 | 500.000 | 16.6 |
| Aroclor-1016-2 | 4.958 | 4.863 | 5.063 | 601.820 | 500.000 | 20.4 |
| Aroclor-1016-3 | 5.080 | 4.983 | 5.183 | 578.000 | 500.000 | 15.6 |
| Aroclor-1016-4 | 5.120 | 5.023 | 5.223 | 590.230 | 500.000 | 18.0 |
| Aroclor-1016-5 | 5.335 | 5.239 | 5.439 | 592.640 | 500.000 | 18.5 |
| Aroclor-1260-1 | 6.551 | 6.455 | 6.655 | 550.000 | 500.000 | 10.0 |
| Aroclor-1260-2 | 6.705 | 6.609 | 6.809 | 554.960 | 500.000 | 11.0 |
| Aroclor-1260-3 | 6.915 | 6.819 | 7.019 | 569.790 | 500.000 | 14.0 |
| Aroclor-1260-4 | 7.174 | 7.079 | 7.279 | 581.890 | 500.000 | 16.4 |
| Aroclor-1260-5 | 7.413 | 7.318 | 7.518 | 587.660 | 500.000 | 17.5 |
| Decachlorobiphenyl | 8.818 | 8.726 | 8.926 | 52.860 | 50.000 | 5.7 |
| Tetrachloro-m-xylene | 3.802 | 3.705 | 3.905 | 61.630 | 50.000 | 23.3 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 09:51
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:29:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.802 | 63412779 | 236.3E6 | 56.704 | 61.629 |
| 2) SA Decachlor... | 10.432 | 8.818 | 49396168 | 317.9E6 | 50.863 | 52.859 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 5.809 | 4.901 | 22324389 | 232.6E6 | 541.108 | 583.175 |
| 4) L1 AR-1016-2 | 5.830 | 4.958 | 32934644 | 113.0E6 | 542.208 | 601.822 |
| 5) L1 AR-1016-3 | 5.894 | 5.080 | 21660183 | 61308172 | 546.140 | 577.999 |
| 6) L1 AR-1016-4 | 5.990 | 5.120 | 17890857 | 64465367 | 549.736 | 590.234 |
| 7) L1 AR-1016-5 | 6.283 | 5.335 | 17779139 | 69316623 | 547.589 | 592.636 |
| 31) L7 AR-1260-1 | 7.400 | 6.551 | 29327545 | 222.2E6 | 520.397 | 549.999 |
| 32) L7 AR-1260-2 | 7.653 | 6.705 | 34227789 | 173.5E6 | 502.225 | 554.959 |
| 33) L7 AR-1260-3 | 8.010 | 6.915 | 27187361 | 224.6E6 | 510.121 | 569.795 |
| 34) L7 AR-1260-4 | 8.239 | 7.174 | 31861536 | 169.3E6 | 508.848 | 581.890 |
| 35) L7 AR-1260-5 | 8.564 | 7.413 | 55364530 | 445.1E6 | 488.633 | 587.662 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074302.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 09:51
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:29:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

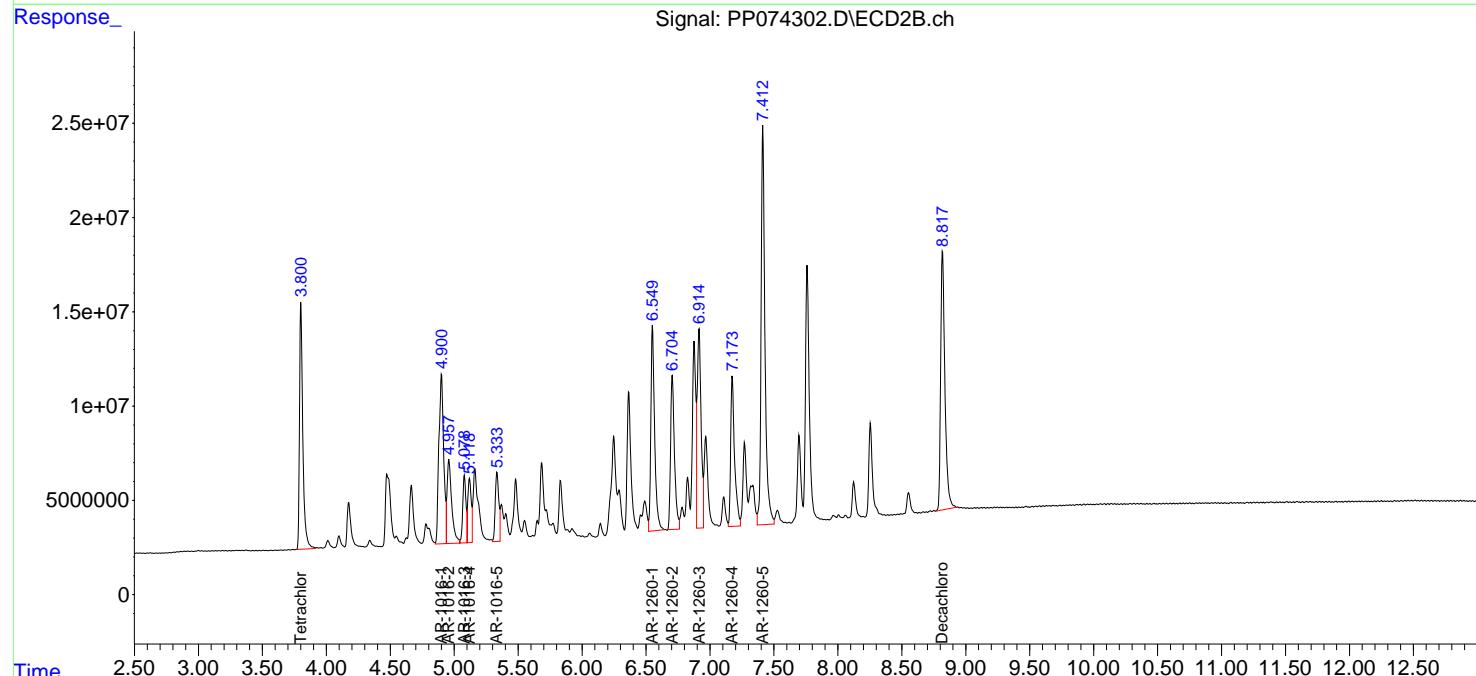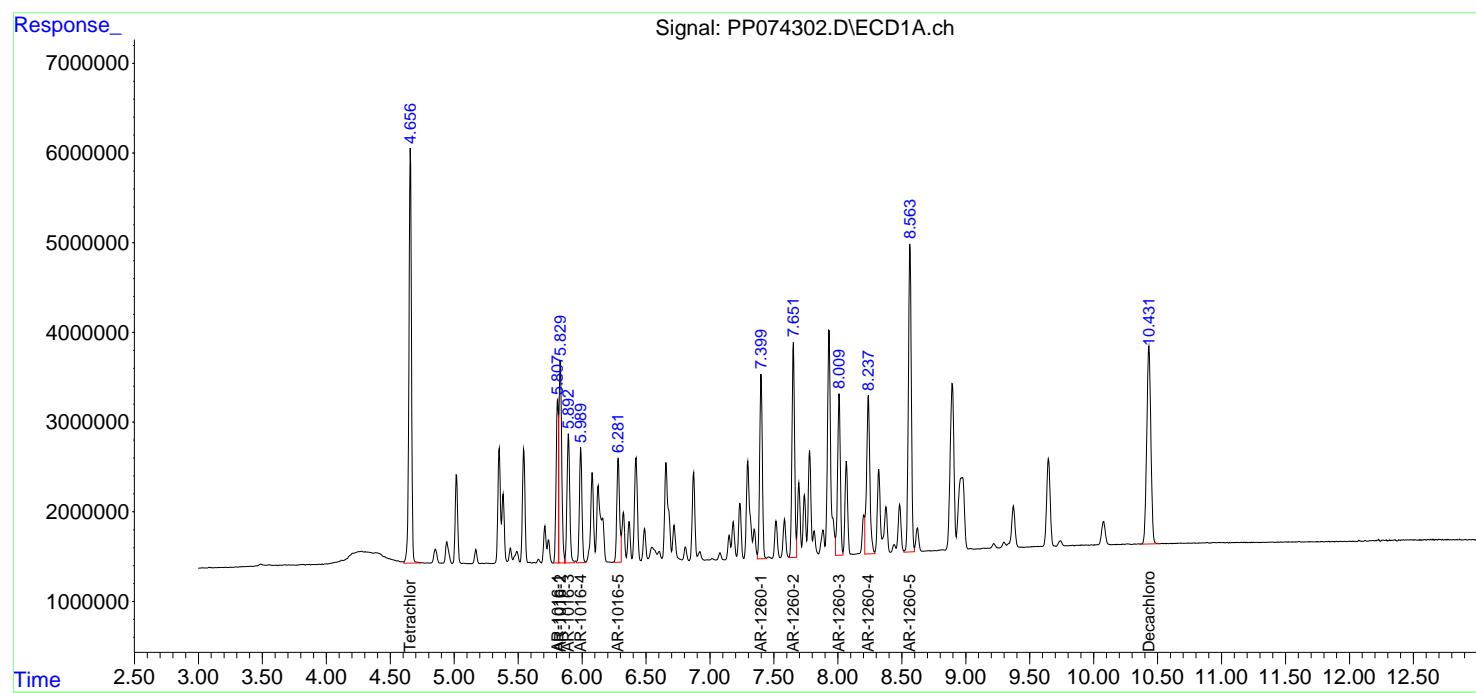

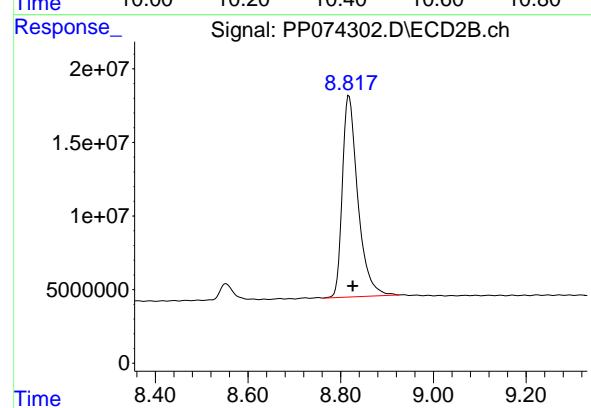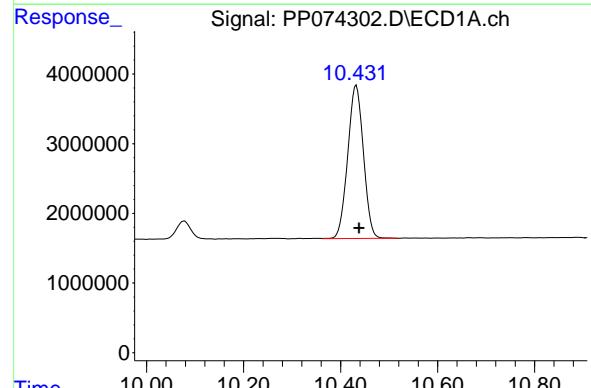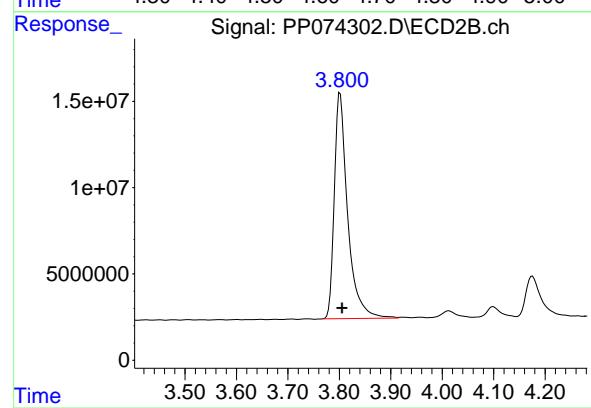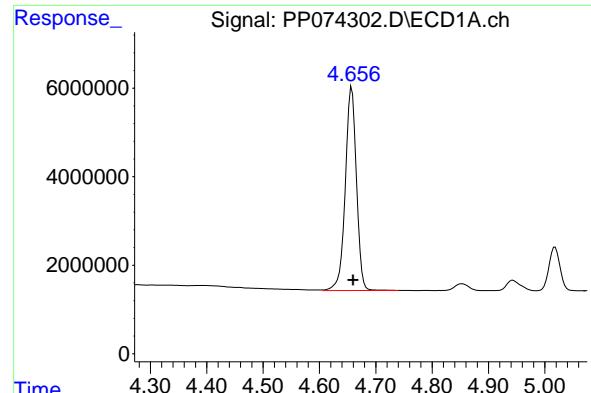

#1 Tetrachloro-m-xylene

R.T.: 4.657 min
 Delta R.T.: -0.003 min
 Response: 63412779
 Conc: 56.70 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1660CCC500

#1 Tetrachloro-m-xylene


R.T.: 3.802 min
 Delta R.T.: -0.004 min
 Response: 236312344
 Conc: 61.63 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.432 min
 Delta R.T.: -0.006 min
 Response: 49396168
 Conc: 50.86 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.818 min
 Delta R.T.: -0.008 min
 Response: 317876418
 Conc: 52.86 ng/ml

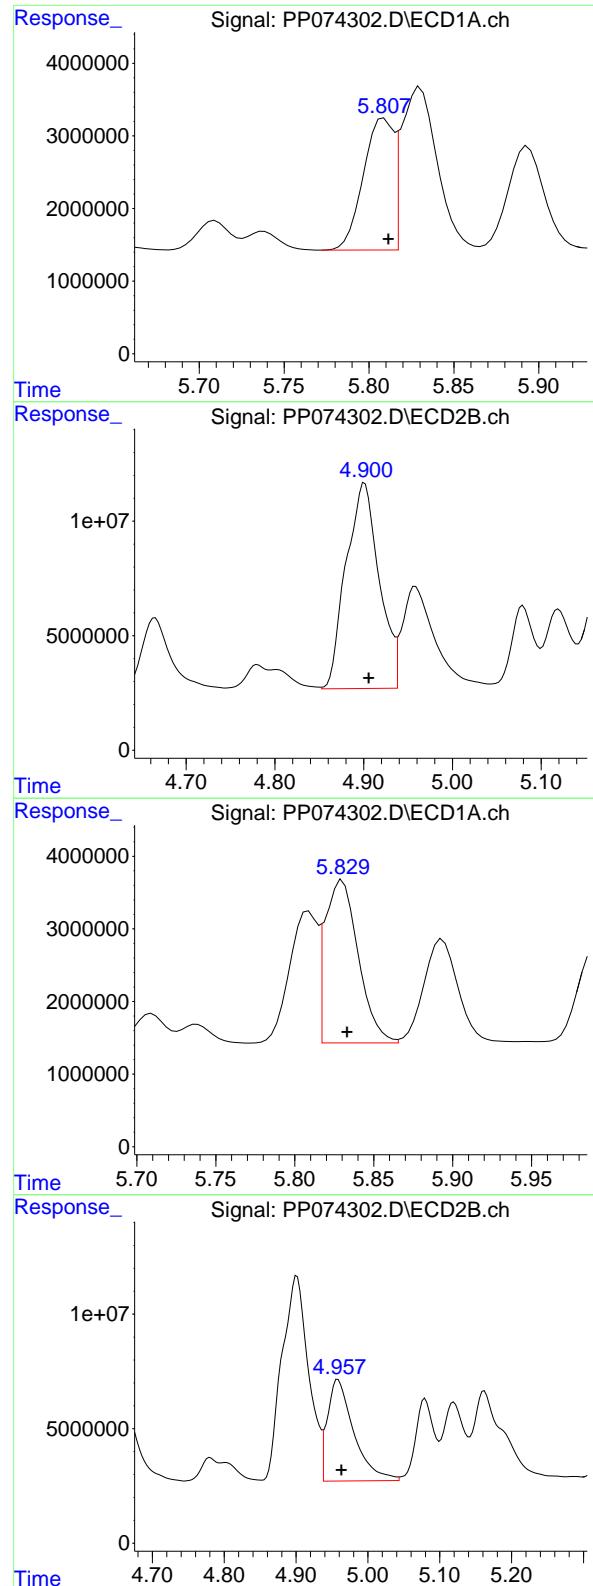

#3 AR-1016-1

R.T.: 5.809 min
 Delta R.T.: -0.003 min
 Response: 22324389
 Conc: 541.11 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#3 AR-1016-1





R.T.: 4.901 min
 Delta R.T.: -0.005 min
 Response: 232621277
 Conc: 583.18 ng/ml

#4 AR-1016-2

R.T.: 5.830 min
 Delta R.T.: -0.003 min
 Response: 32934644
 Conc: 542.21 ng/ml

#4 AR-1016-2

R.T.: 4.958 min
 Delta R.T.: -0.005 min
 Response: 113027618
 Conc: 601.82 ng/ml

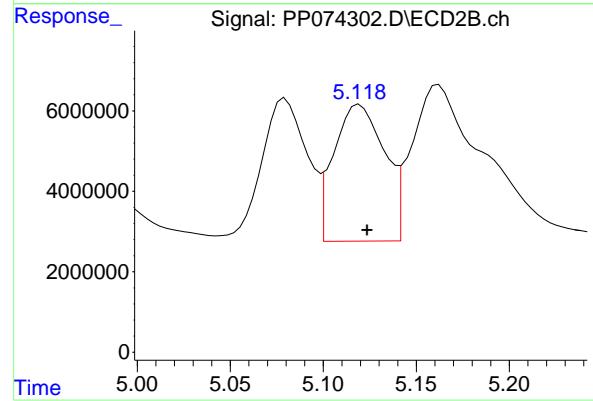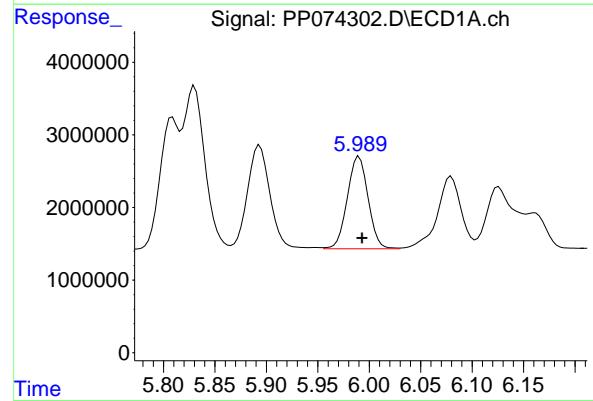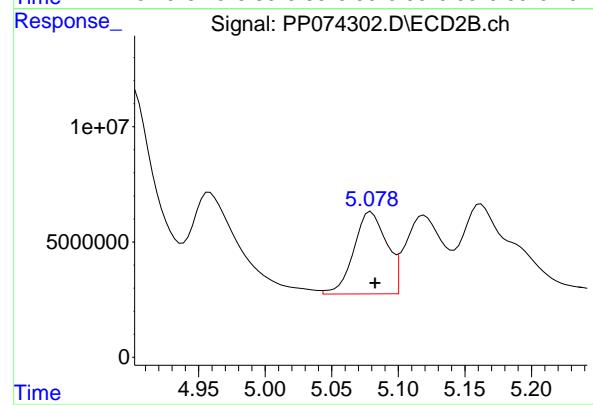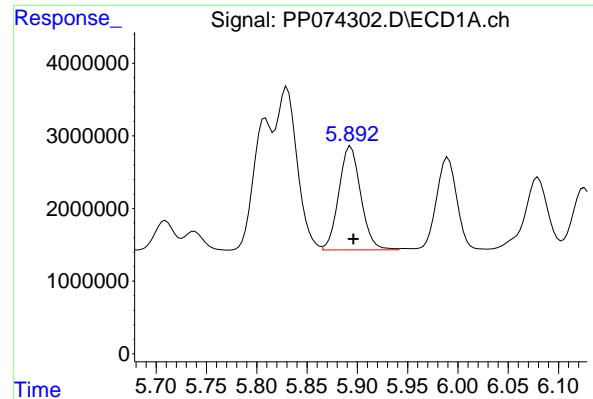

#5 AR-1016-3

R.T.: 5.894 min
 Delta R.T.: -0.003 min
 Response: 21660183
 Conc: 546.14 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#5 AR-1016-3





R.T.: 5.080 min
 Delta R.T.: -0.003 min
 Response: 61308172
 Conc: 578.00 ng/ml

#6 AR-1016-4

R.T.: 5.990 min
 Delta R.T.: -0.003 min
 Response: 17890857
 Conc: 549.74 ng/ml

#6 AR-1016-4

R.T.: 5.120 min
 Delta R.T.: -0.004 min
 Response: 64465367
 Conc: 590.23 ng/ml

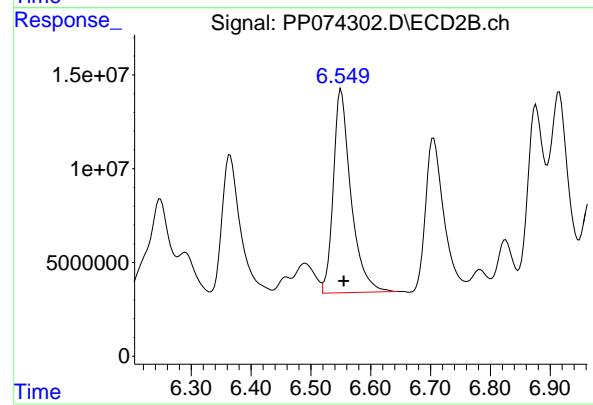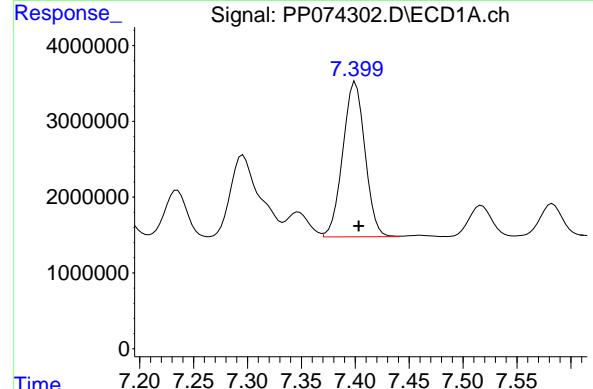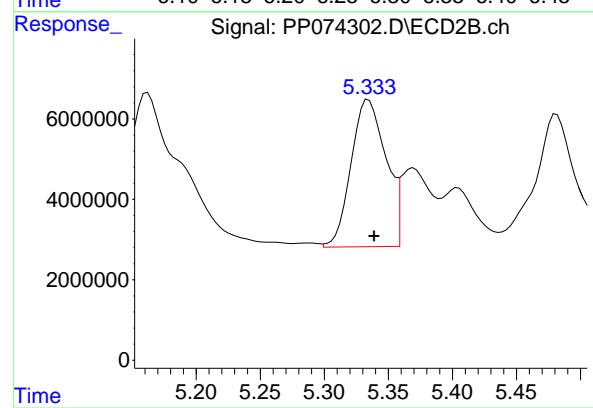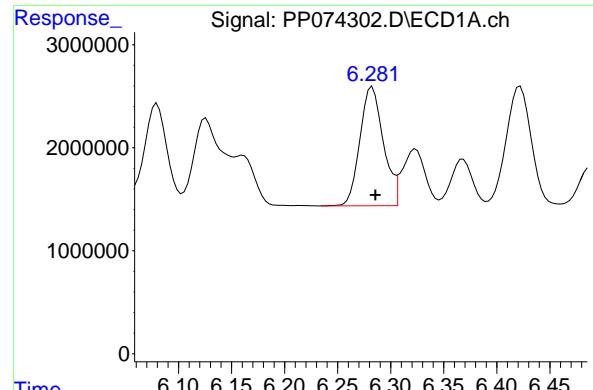

#7 AR-1016-5

R.T.: 6.283 min
 Delta R.T.: -0.003 min
 Response: 17779139
 Conc: 547.59 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#7 AR-1016-5

R.T.: 5.335 min
 Delta R.T.: -0.004 min
 Response: 69316623
 Conc: 592.64 ng/ml

#31 AR-1260-1

R.T.: 7.400 min
 Delta R.T.: -0.003 min
 Response: 29327545
 Conc: 520.40 ng/ml





#31 AR-1260-1

R.T.: 6.551 min
 Delta R.T.: -0.004 min
 Response: 222175958
 Conc: 550.00 ng/ml

#32 AR-1260-2

R.T.: 7.653 min
 Delta R.T.: -0.003 min
 Response: 34227789
 Conc: 502.22 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

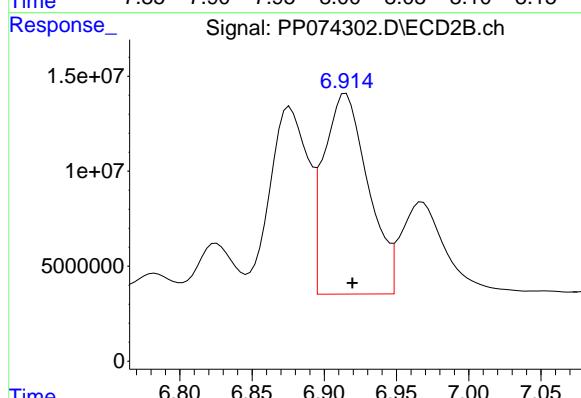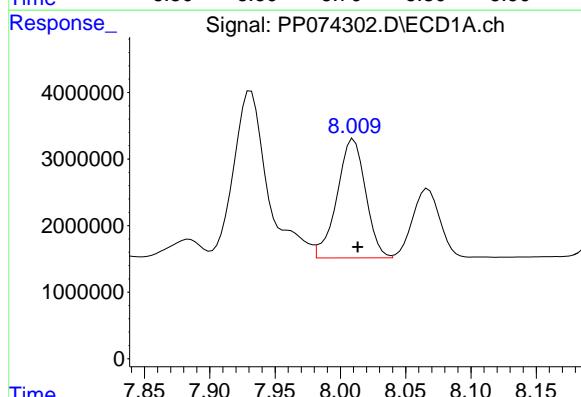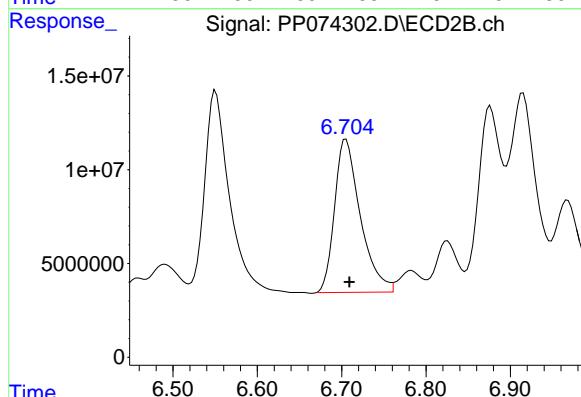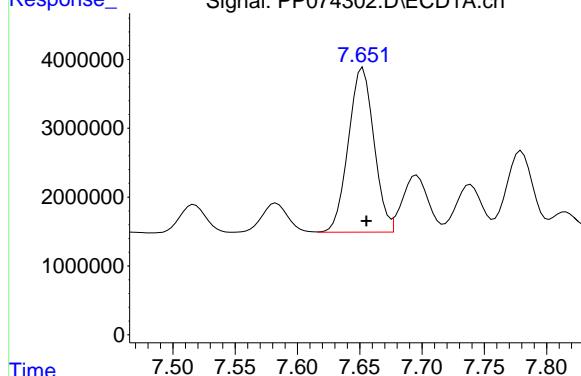

#32 AR-1260-2

R.T.: 6.705 min
 Delta R.T.: -0.004 min
 Response: 173534930
 Conc: 554.96 ng/ml

#33 AR-1260-3

R.T.: 8.010 min
 Delta R.T.: -0.003 min
 Response: 27187361
 Conc: 510.12 ng/ml





#33 AR-1260-3

R.T.: 6.915 min
 Delta R.T.: -0.004 min
 Response: 224566541
 Conc: 569.79 ng/ml

#34 AR-1260-4

R.T.: 8.239 min
 Delta R.T.: -0.003 min
 Response: 31861536
 Conc: 508.85 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

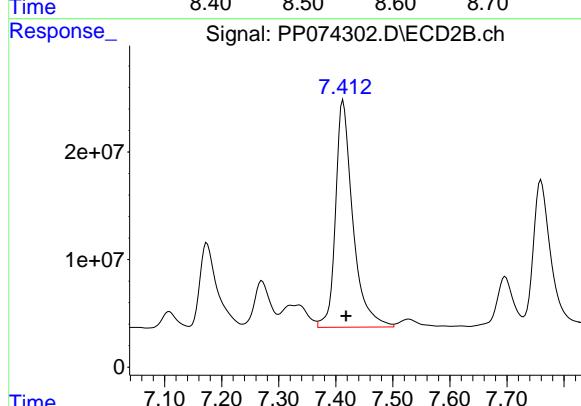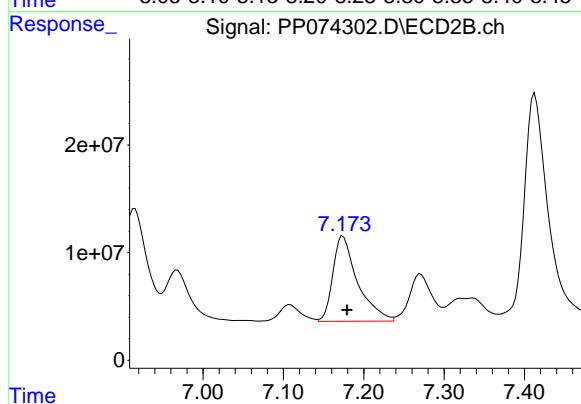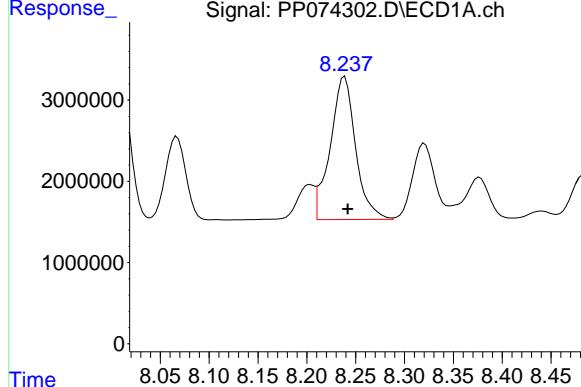

#34 AR-1260-4

R.T.: 7.174 min
 Delta R.T.: -0.005 min
 Response: 169318007
 Conc: 581.89 ng/ml

#35 AR-1260-5

R.T.: 8.564 min
 Delta R.T.: -0.003 min
 Response: 55364530
 Conc: 488.63 ng/ml

#35 AR-1260-5

R.T.: 7.413 min
 Delta R.T.: -0.005 min
 Response: 445101278
 Conc: 587.66 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 08/01/2025

08/01/2025

Continuing Calib Time: 15:48

Initial Calibration Time(s): 12:05

20:28

GC Column: ZB-MR1

ID: 0.32 (mm)

| COMPOUND | CCAL RT | Avg RT | RT Window From | TO | Diff RT |
|----------------------|---------|--------|----------------|-------|---------|
| Aroclor-1016-1 (1) | 5.81 | 5.81 | 5.71 | 5.91 | 0.00 |
| Aroclor-1016-2 (2) | 5.83 | 5.83 | 5.73 | 5.93 | 0.00 |
| Aroclor-1016-3 (3) | 5.90 | 5.90 | 5.80 | 6.00 | 0.01 |
| Aroclor-1016-4 (4) | 5.99 | 5.99 | 5.89 | 6.09 | 0.00 |
| Aroclor-1016-5 (5) | 6.28 | 6.29 | 6.19 | 6.39 | 0.01 |
| Aroclor-1260-1 (1) | 7.40 | 7.40 | 7.30 | 7.50 | 0.00 |
| Aroclor-1260-2 (2) | 7.65 | 7.66 | 7.56 | 7.76 | 0.01 |
| Aroclor-1260-3 (3) | 8.01 | 8.01 | 7.91 | 8.11 | 0.00 |
| Aroclor-1260-4 (4) | 8.24 | 8.24 | 8.14 | 8.34 | 0.00 |
| Aroclor-1260-5 (5) | 8.57 | 8.57 | 8.47 | 8.67 | 0.01 |
| Tetrachloro-m-xylene | 4.66 | 4.66 | 4.56 | 4.76 | 0.00 |
| Decachlorobiphenyl | 10.44 | 10.44 | 10.34 | 10.54 | 0.00 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

Lab Name: Alliance

Contract: FIRS02

Lab Code: ACE

SDG NO.: Q2819

Continuing Calib Date: 08/12/2025

Initial Calibration Date(s): 08/01/2025

08/01/2025

Continuing Calib Time: 15:48

Initial Calibration Time(s): 12:05

20:28

GC Column: ZB-MR2

ID: 0.32 (mm)

| COMPOUND | CCAL RT | AVG RT | RT WINDOW FROM | TO | DIFF RT |
|----------------------|---------|--------|----------------|------|---------|
| Aroclor-1016-1 (1) | 4.90 | 4.91 | 4.81 | 5.01 | 0.01 |
| Aroclor-1016-2 (2) | 4.96 | 4.96 | 4.86 | 5.06 | 0.00 |
| Aroclor-1016-3 (3) | 5.08 | 5.08 | 4.98 | 5.18 | 0.00 |
| Aroclor-1016-4 (4) | 5.12 | 5.12 | 5.02 | 5.22 | 0.00 |
| Aroclor-1016-5 (5) | 5.33 | 5.34 | 5.24 | 5.44 | 0.01 |
| Aroclor-1260-1 (1) | 6.55 | 6.56 | 6.46 | 6.66 | 0.01 |
| Aroclor-1260-2 (2) | 6.71 | 6.71 | 6.61 | 6.81 | 0.00 |
| Aroclor-1260-3 (3) | 6.92 | 6.92 | 6.82 | 7.02 | 0.00 |
| Aroclor-1260-4 (4) | 7.18 | 7.18 | 7.08 | 7.28 | 0.00 |
| Aroclor-1260-5 (5) | 7.41 | 7.42 | 7.32 | 7.52 | 0.01 |
| Tetrachloro-m-xylene | 3.80 | 3.81 | 3.71 | 3.91 | 0.01 |
| Decachlorobiphenyl | 8.82 | 8.83 | 8.73 | 8.93 | 0.01 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|----------|---------------|--|
| Lab Name: | Alliance | Contract: | FIRS02 |
| Lab Code: | ACE | SDG NO.: | Q2819 |
| GC Column: | ZB-MR1 | ID: 0.32 (mm) | Initi. Calib. Date(s): 08/01/2025 08/01/2025 |

| | | | |
|--------------------|--------------|----------------|------------|
| Client Sample No.: | CCAL04 | Date Analyzed: | 08/12/2025 |
| Lab Sample No.: | AR1660CCC500 | Data File : | PP074316.D |
| | | Time Analyzed: | 15:48 |

| COMPOUND | RT | RT WINDOW FROM TO | | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|--------|----------------------|--------|--------------------|-------------------|------|
| Aroclor-1016-1 | 5.811 | 5.712 | 5.912 | 556.880 | 500.000 | 11.4 |
| Aroclor-1016-2 | 5.832 | 5.733 | 5.933 | 550.560 | 500.000 | 10.1 |
| Aroclor-1016-3 | 5.895 | 5.796 | 5.996 | 559.440 | 500.000 | 11.9 |
| Aroclor-1016-4 | 5.992 | 5.893 | 6.093 | 563.510 | 500.000 | 12.7 |
| Aroclor-1016-5 | 6.284 | 6.186 | 6.386 | 554.850 | 500.000 | 11.0 |
| Aroclor-1260-1 | 7.401 | 7.303 | 7.503 | 536.530 | 500.000 | 7.3 |
| Aroclor-1260-2 | 7.654 | 7.555 | 7.755 | 517.500 | 500.000 | 3.5 |
| Aroclor-1260-3 | 8.012 | 7.913 | 8.113 | 522.830 | 500.000 | 4.6 |
| Aroclor-1260-4 | 8.240 | 8.142 | 8.342 | 532.940 | 500.000 | 6.6 |
| Aroclor-1260-5 | 8.565 | 8.468 | 8.668 | 506.790 | 500.000 | 1.4 |
| Decachlorobiphenyl | 10.436 | 10.338 | 10.538 | 52.310 | 50.000 | 4.6 |
| Tetrachloro-m-xylene | 4.659 | 4.560 | 4.760 | 57.560 | 50.000 | 15.1 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900, Fax : 908 789 8922

CALIBRATION VERIFICATION SUMMARY

| | | | |
|------------|-----------------|----------------------|--|
| Lab Name: | <u>Alliance</u> | Contract: | <u>FIRS02</u> |
| Lab Code: | <u>ACE</u> | SDG NO.: | <u>Q2819</u> |
| GC Column: | <u>ZB-MR2</u> | ID: <u>0.32</u> (mm) | Initi. Calib. Date(s): <u>08/01/2025</u> <u>08/01/2025</u> |

| | | | |
|--------------------|---------------------|----------------|-------------------|
| Client Sample No.: | <u>CCAL04</u> | Date Analyzed: | <u>08/12/2025</u> |
| Lab Sample No.: | <u>AR1660CCC500</u> | Data File : | <u>PP074316.D</u> |
| | | Time Analyzed: | <u>15:48</u> |

| COMPOUND | RT | RT WINDOW FROM | | CALC AMOUNT(ng) | NOM AMOUNT(ng) | %D |
|----------------------|-------|-------------------|-------|--------------------|-------------------|------|
| | | TO | | | | |
| Aroclor-1016-1 | 4.903 | 4.806 | 5.006 | 585.540 | 500.000 | 17.1 |
| Aroclor-1016-2 | 4.958 | 4.863 | 5.063 | 555.580 | 500.000 | 11.1 |
| Aroclor-1016-3 | 5.081 | 4.983 | 5.183 | 591.090 | 500.000 | 18.2 |
| Aroclor-1016-4 | 5.122 | 5.023 | 5.223 | 595.870 | 500.000 | 19.2 |
| Aroclor-1016-5 | 5.334 | 5.239 | 5.439 | 590.590 | 500.000 | 18.1 |
| Aroclor-1260-1 | 6.552 | 6.455 | 6.655 | 580.600 | 500.000 | 16.1 |
| Aroclor-1260-2 | 6.706 | 6.609 | 6.809 | 568.790 | 500.000 | 13.8 |
| Aroclor-1260-3 | 6.917 | 6.819 | 7.019 | 594.280 | 500.000 | 18.9 |
| Aroclor-1260-4 | 7.175 | 7.079 | 7.279 | 583.960 | 500.000 | 16.8 |
| Aroclor-1260-5 | 7.414 | 7.318 | 7.518 | 585.850 | 500.000 | 17.2 |
| Decachlorobiphenyl | 8.820 | 8.726 | 8.926 | 55.460 | 50.000 | 10.9 |
| Tetrachloro-m-xylene | 3.802 | 3.705 | 3.905 | 59.630 | 50.000 | 19.3 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:48
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:54:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|---------|
| 1) SA Tetrachlor... | 4.659 | 3.802 | 64369772 | 228.6E6 | 57.560 | 59.625m |
| 2) SA Decachlor... | 10.436 | 8.820 | 50800485 | 333.5E6 | 52.309 | 55.456 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|----------|
| 3) L1 AR-1016-1 | 5.811 | 4.903 | 22974987 | 233.6E6 | 556.877 | 585.544 |
| 4) L1 AR-1016-2 | 5.832 | 4.958 | 33441672 | 104.3E6 | 550.555 | 555.579m |
| 5) L1 AR-1016-3 | 5.895 | 5.081 | 22187737 | 62696370 | 559.442 | 591.087 |
| 6) L1 AR-1016-4 | 5.992 | 5.122 | 18339102 | 65081402 | 563.509 | 595.874 |
| 7) L1 AR-1016-5 | 6.284 | 5.334 | 18014922 | 69076982 | 554.851 | 590.587m |
| 31) L7 AR-1260-1 | 7.401 | 6.552 | 30236790 | 234.5E6 | 536.531 | 580.596 |
| 32) L7 AR-1260-2 | 7.654 | 6.706 | 35268906 | 177.9E6 | 517.501 | 568.793 |
| 33) L7 AR-1260-3 | 8.012 | 6.917 | 27864737 | 234.2E6 | 522.830 | 594.283 |
| 34) L7 AR-1260-4 | 8.240 | 7.175 | 33370027 | 169.9E6 | 532.940 | 583.961 |
| 35) L7 AR-1260-5 | 8.565 | 7.414 | 57421797 | 443.7E6 | 506.790 | 585.848 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:48
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:54:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 AR1660CCC500

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

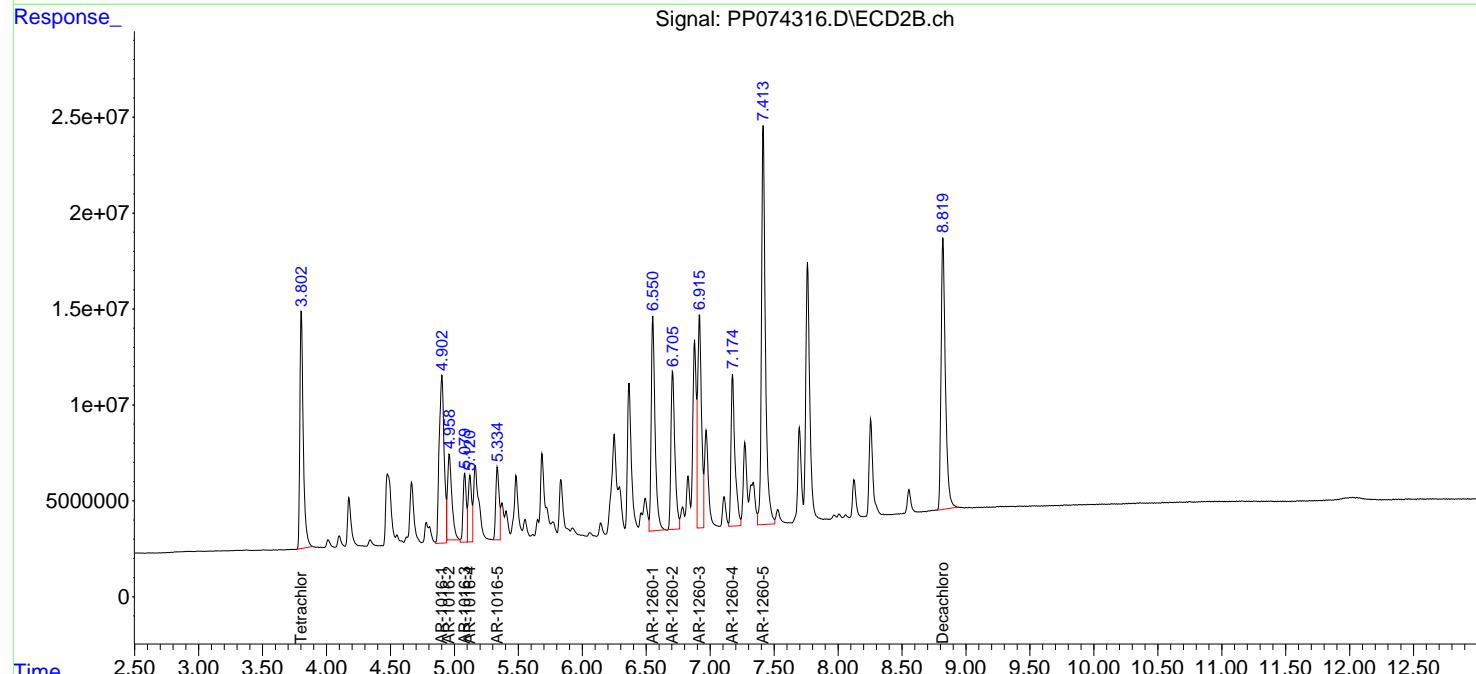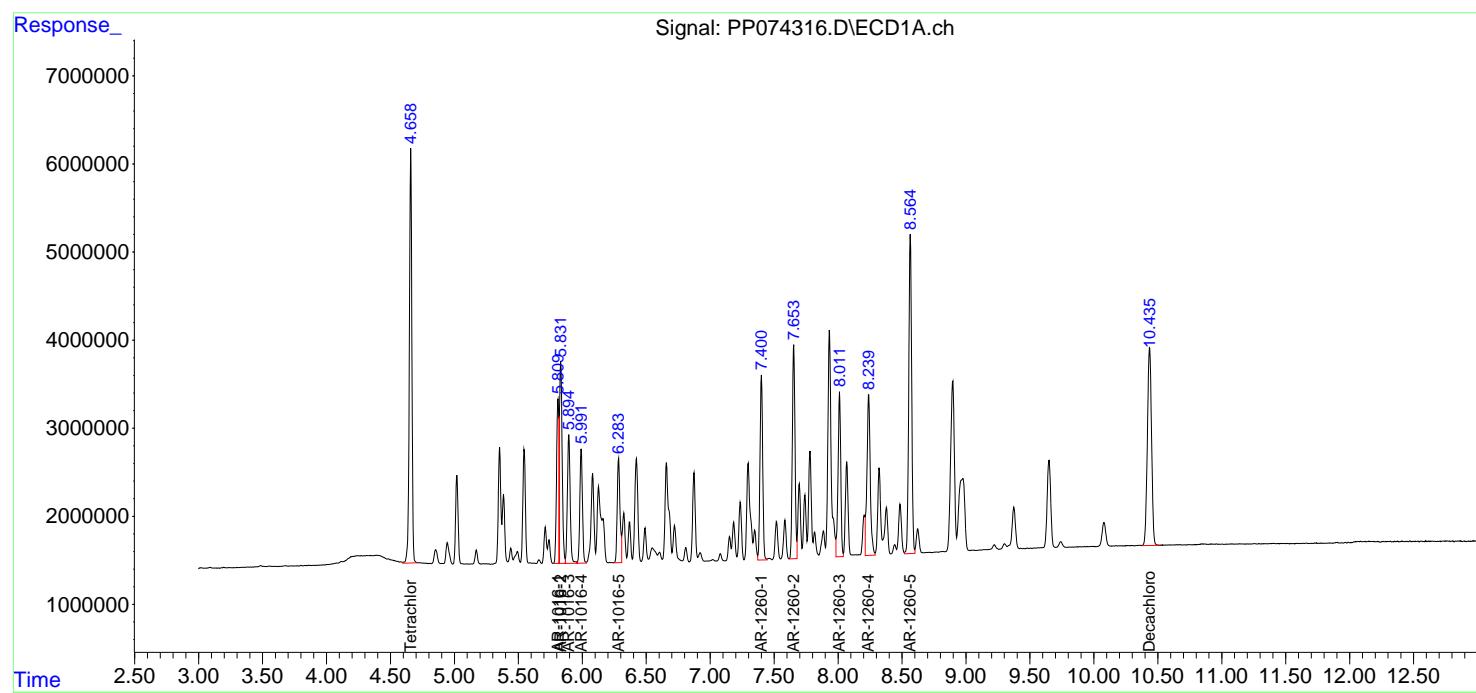

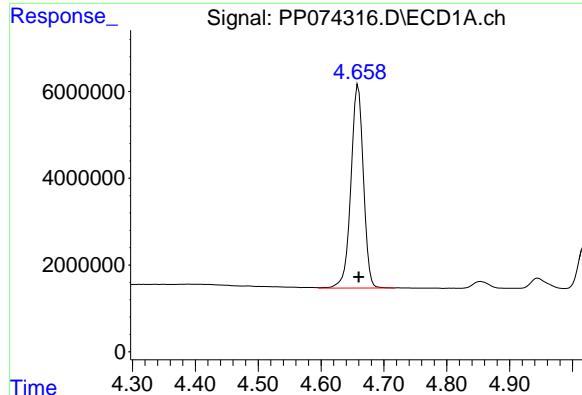


#1 Tetrachloro-m-xylene

R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 64369772
Conc: 57.56 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

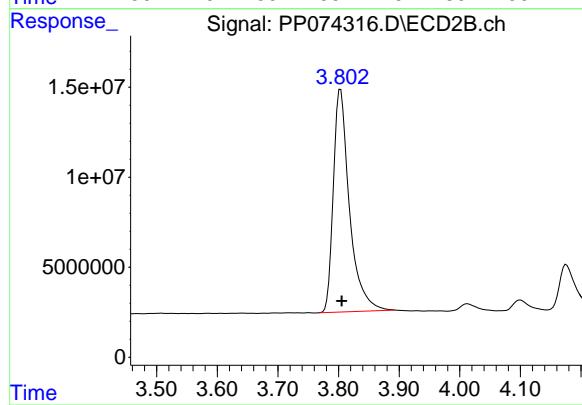


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: -0.003 min
Response: 228628471
Conc: 59.63 ng/ml

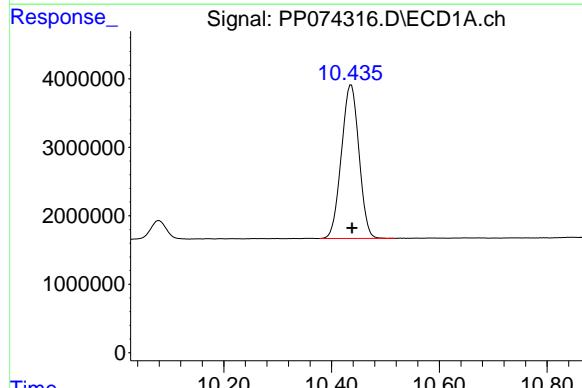


#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: -0.002 min
Response: 50800485
Conc: 52.31 ng/ml

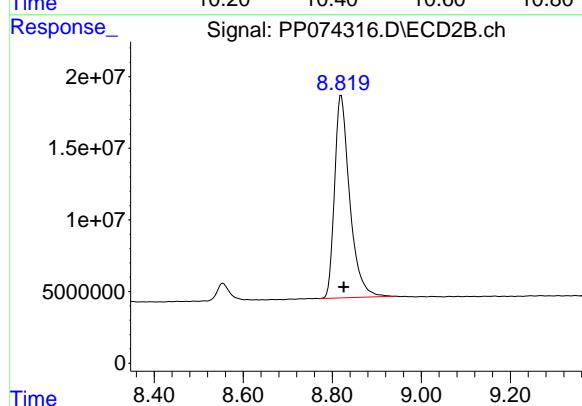

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 333491572
Conc: 55.46 ng/ml

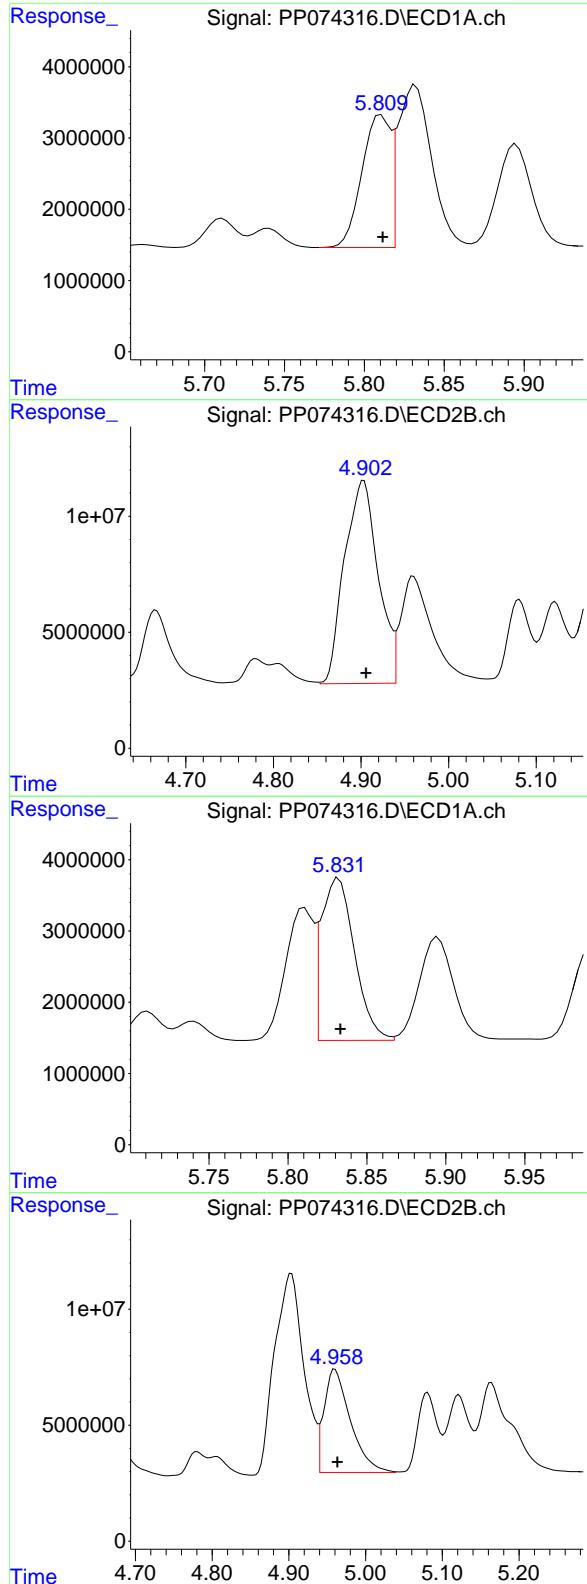

#3 AR-1016-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 22974987
 Conc: 556.88 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#3 AR-1016-1


R.T.: 4.903 min
 Delta R.T.: -0.003 min
 Response: 233566270
 Conc: 585.54 ng/ml

#4 AR-1016-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 33441672
 Conc: 550.56 ng/ml

#4 AR-1016-2

R.T.: 4.958 min
 Delta R.T.: -0.005 min
 Response: 104342798
 Conc: 555.58 ng/ml

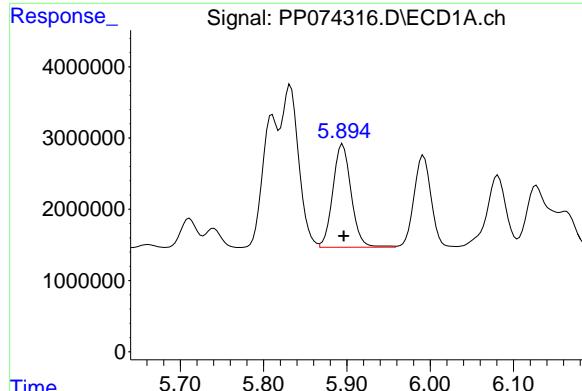


#5 AR-1016-3

R.T.: 5.895 min
Delta R.T.: -0.001 min
Response: 22187737
Conc: 559.44 ng/ml

Instrument: ECD_P
ClientSampleId : AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

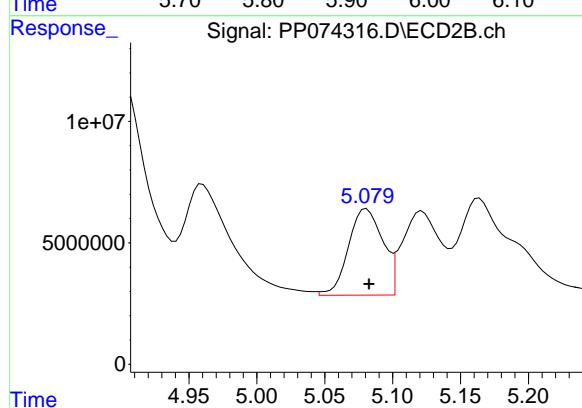


#5 AR-1016-3

R.T.: 5.081 min
Delta R.T.: -0.002 min
Response: 62696370
Conc: 591.09 ng/ml




#6 AR-1016-4

R.T.: 5.992 min
Delta R.T.: 0.000 min
Response: 18339102
Conc: 563.51 ng/ml

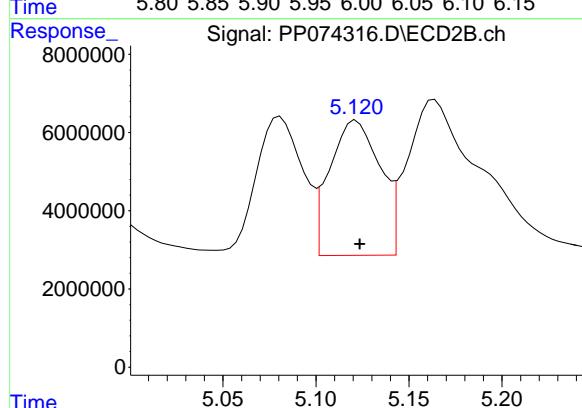

#6 AR-1016-4

R.T.: 5.122 min
Delta R.T.: -0.002 min
Response: 65081402
Conc: 595.87 ng/ml

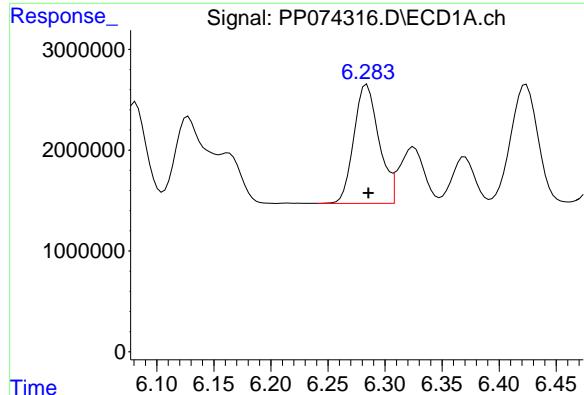


#7 AR-1016-5

R.T.: 6.284 min
Delta R.T.: -0.002 min
Response: 18014922
Conc: 554.85 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

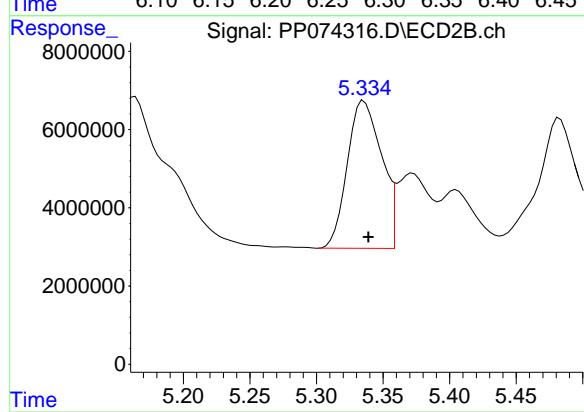


#7 AR-1016-5

R.T.: 5.334 min
Delta R.T.: -0.005 min
Response: 69076982
Conc: 590.59 ng/ml

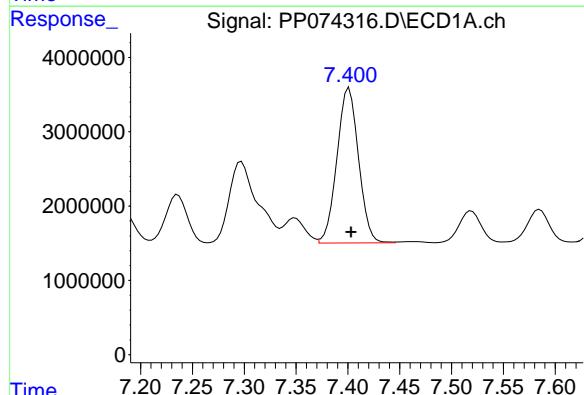


#31 AR-1260-1

R.T.: 7.401 min
Delta R.T.: -0.002 min
Response: 30236790
Conc: 536.53 ng/ml

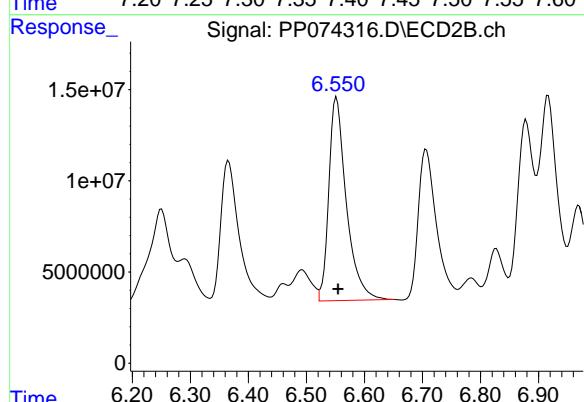

#31 AR-1260-1

R.T.: 6.552 min
Delta R.T.: -0.003 min
Response: 234535731
Conc: 580.60 ng/ml

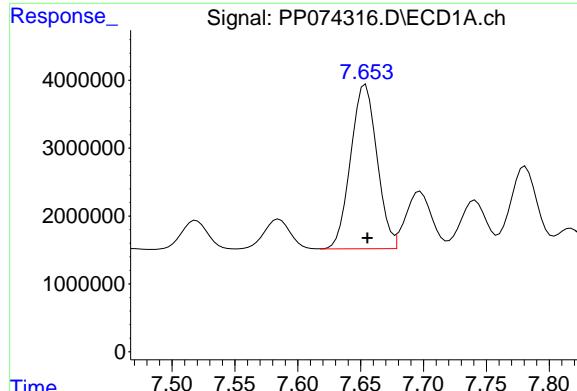


#32 AR-1260-2

R.T.: 7.654 min
 Delta R.T.: -0.001 min
 Response: 35268906
 Conc: 517.50 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

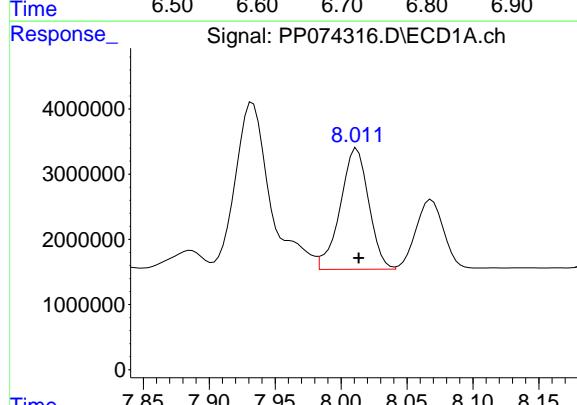

#32 AR-1260-2

R.T.: 6.706 min
 Delta R.T.: -0.003 min
 Response: 177860970
 Conc: 568.79 ng/ml

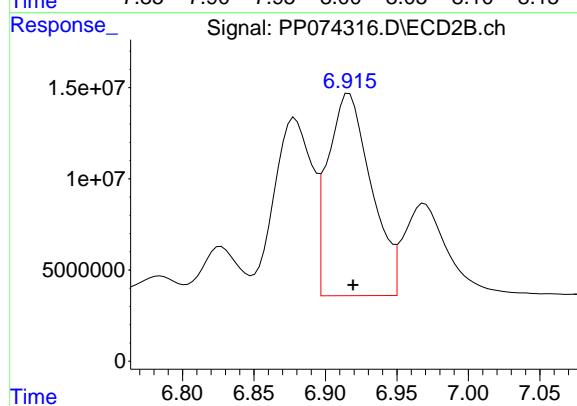


#33 AR-1260-3

R.T.: 8.012 min
 Delta R.T.: -0.001 min
 Response: 27864737
 Conc: 522.83 ng/ml

#33 AR-1260-3

R.T.: 6.917 min
 Delta R.T.: -0.003 min
 Response: 234217922
 Conc: 594.28 ng/ml

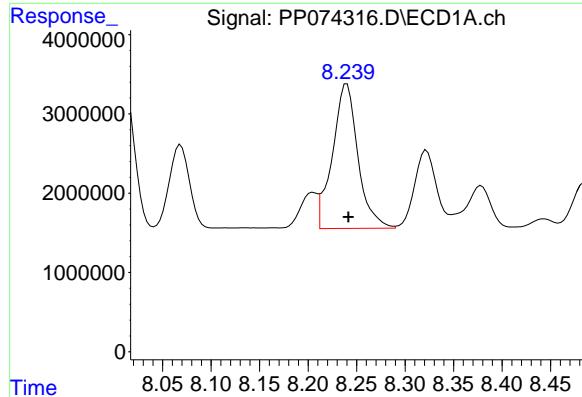


#34 AR-1260-4

R.T.: 8.240 min
Delta R.T.: -0.002 min
Response: 33370027
Conc: 532.94 ng/ml

Instrument:
ECD_P
ClientSampleId :
AR1660CCC500


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

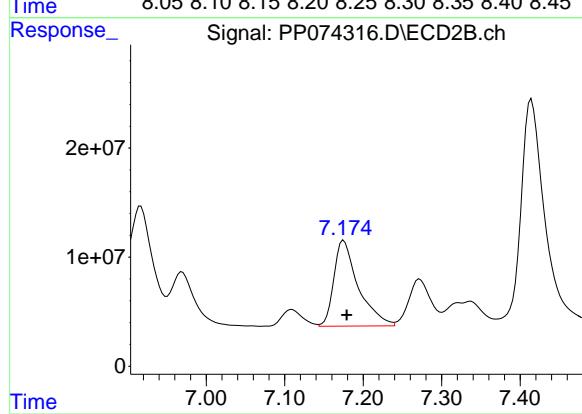


#34 AR-1260-4

R.T.: 7.175 min
Delta R.T.: -0.004 min
Response: 169920550
Conc: 583.96 ng/ml

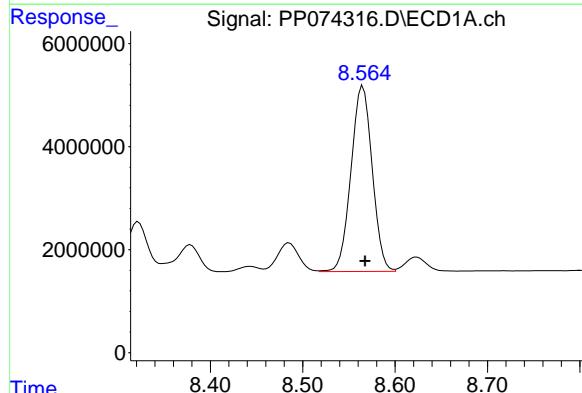

#35 AR-1260-5

R.T.: 8.565 min
Delta R.T.: -0.002 min
Response: 57421797
Conc: 506.79 ng/ml

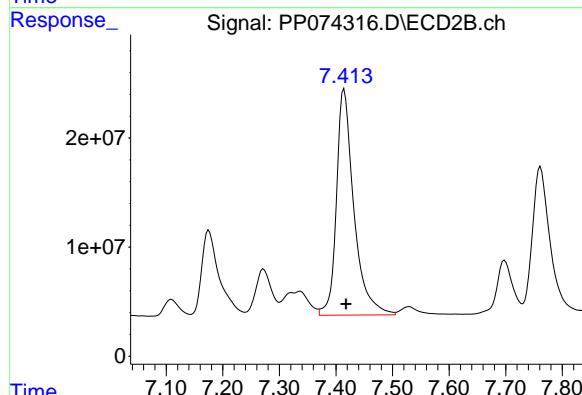

#35 AR-1260-5

R.T.: 7.414 min
Delta R.T.: -0.004 min
Response: 443727135
Conc: 585.85 ng/ml

Analytical Sequence

Client: First Environment, Inc.

SDG No.: Q2819

Project: USACE018-44 DOD

Instrument ID: ECD_O

GC Column: ZB-MR1

ID: 0.32 (mm)

Inst. Calib. Date(s): 07/23/2025 07/23/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

| CLIENT ID | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | DATAFILE | DCB RT # | TCX RT # |
|---------------|---------------|---------------|---------------|------------|----------|----------|
| I.BLK | I.BLK | 07/23/2025 | 11:14 | PO112413.D | 8.69 | 3.67 |
| AR1660ICC1000 | AR1660ICC1000 | 07/23/2025 | 11:32 | PO112414.D | 8.70 | 3.67 |
| AR1660ICC750 | AR1660ICC750 | 07/23/2025 | 11:50 | PO112415.D | 8.69 | 3.67 |
| AR1660ICC500 | AR1660ICC500 | 07/23/2025 | 12:08 | PO112416.D | 8.69 | 3.67 |
| AR1660ICC250 | AR1660ICC250 | 07/23/2025 | 12:27 | PO112417.D | 8.69 | 3.67 |
| AR1660ICC050 | AR1660ICC050 | 07/23/2025 | 12:45 | PO112418.D | 8.69 | 3.67 |
| AR1221ICC500 | AR1221ICC500 | 07/23/2025 | 13:03 | PO112419.D | 8.69 | 3.67 |
| AR1232ICC500 | AR1232ICC500 | 07/23/2025 | 13:22 | PO112420.D | 8.69 | 3.67 |
| AR1242ICC1000 | AR1242ICC1000 | 07/23/2025 | 13:40 | PO112421.D | 8.69 | 3.67 |
| AR1242ICC750 | AR1242ICC750 | 07/23/2025 | 13:59 | PO112422.D | 8.69 | 3.67 |
| AR1242ICC500 | AR1242ICC500 | 07/23/2025 | 14:17 | PO112423.D | 8.69 | 3.67 |
| AR1242ICC250 | AR1242ICC250 | 07/23/2025 | 14:36 | PO112424.D | 8.69 | 3.67 |
| AR1242ICC050 | AR1242ICC050 | 07/23/2025 | 14:54 | PO112425.D | 8.70 | 3.67 |
| AR1248ICC1000 | AR1248ICC1000 | 07/23/2025 | 15:13 | PO112426.D | 8.69 | 3.67 |
| AR1248ICC750 | AR1248ICC750 | 07/23/2025 | 15:31 | PO112427.D | 8.69 | 3.67 |
| AR1248ICC500 | AR1248ICC500 | 07/23/2025 | 15:48 | PO112428.D | 8.69 | 3.67 |
| AR1248ICC250 | AR1248ICC250 | 07/23/2025 | 16:07 | PO112429.D | 8.70 | 3.67 |
| AR1248ICC050 | AR1248ICC050 | 07/23/2025 | 16:25 | PO112430.D | 8.69 | 3.67 |
| AR1254ICC1000 | AR1254ICC1000 | 07/23/2025 | 16:44 | PO112431.D | 8.69 | 3.67 |
| AR1254ICC750 | AR1254ICC750 | 07/23/2025 | 17:02 | PO112432.D | 8.69 | 3.67 |
| AR1254ICC500 | AR1254ICC500 | 07/23/2025 | 17:21 | PO112433.D | 8.70 | 3.67 |
| AR1254ICC250 | AR1254ICC250 | 07/23/2025 | 17:39 | PO112434.D | 8.69 | 3.67 |
| AR1254ICC050 | AR1254ICC050 | 07/23/2025 | 17:57 | PO112435.D | 8.69 | 3.67 |
| AR1262ICC500 | AR1262ICC500 | 07/23/2025 | 18:16 | PO112436.D | 8.70 | 3.67 |
| AR1268ICC1000 | AR1268ICC1000 | 07/23/2025 | 18:34 | PO112437.D | 8.70 | 3.67 |
| AR1268ICC750 | AR1268ICC750 | 07/23/2025 | 18:53 | PO112438.D | 8.70 | 3.67 |
| AR1268ICC500 | AR1268ICC500 | 07/23/2025 | 19:11 | PO112439.D | 8.70 | 3.67 |
| AR1268ICC250 | AR1268ICC250 | 07/23/2025 | 19:28 | PO112440.D | 8.69 | 3.67 |
| AR1268ICC050 | AR1268ICC050 | 07/23/2025 | 19:47 | PO112441.D | 8.70 | 3.67 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 08:54 | PO112850.D | 8.69 | 3.67 |
| I.BLK | I.BLK | 08/12/2025 | 10:05 | PO112854.D | 8.69 | 3.66 |
| 11M-S | Q2819-06 | 08/12/2025 | 13:26 | PO112860.D | 8.69 | 3.66 |
| 84SB-W | Q2819-11 | 08/12/2025 | 13:43 | PO112861.D | 8.68 | 3.67 |
| 17M-W | Q2819-14 | 08/12/2025 | 14:01 | PO112862.D | 8.69 | 3.67 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 15:50 | PO112865.D | 8.69 | 3.67 |
| I.BLK | I.BLK | 08/12/2025 | 17:00 | PO112869.D | 8.69 | 3.67 |
| I.BLK | I.BLK | 08/01/2025 | 11:49 | PP074167.D | 10.44 | 4.66 |
| AR1660ICC1000 | AR1660ICC1000 | 08/01/2025 | 12:05 | PP074168.D | 10.44 | 4.66 |
| AR1660ICC750 | AR1660ICC750 | 08/01/2025 | 12:22 | PP074169.D | 10.44 | 4.66 |
| AR1660ICC500 | AR1660ICC500 | 08/01/2025 | 12:38 | PP074170.D | 10.44 | 4.66 |
| AR1660ICC250 | AR1660ICC250 | 08/01/2025 | 12:54 | PP074171.D | 10.44 | 4.66 |
| AR1660ICC050 | AR1660ICC050 | 08/01/2025 | 13:42 | PP074172.D | 10.44 | 4.66 |

Analytical Sequence

| | | | | | | |
|--------------------------------|---------------|------------|-------|------------|-------|------|
| AR1221ICC500 | AR1221ICC500 | 08/01/2025 | 13:58 | PP074173.D | 10.44 | 4.66 |
| AR1232ICC500 | AR1232ICC500 | 08/01/2025 | 14:15 | PP074174.D | 10.44 | 4.66 |
| AR1242ICC1000 | AR1242ICC1000 | 08/01/2025 | 14:31 | PP074175.D | 10.44 | 4.66 |
| AR1242ICC750 | AR1242ICC750 | 08/01/2025 | 14:47 | PP074176.D | 10.44 | 4.66 |
| AR1242ICC500 | AR1242ICC500 | 08/01/2025 | 15:03 | PP074177.D | 10.43 | 4.66 |
| AR1242ICC250 | AR1242ICC250 | 08/01/2025 | 15:19 | PP074178.D | 10.44 | 4.66 |
| AR1242ICC050 | AR1242ICC050 | 08/01/2025 | 15:36 | PP074179.D | 10.43 | 4.66 |
| AR1248ICC500 | AR1248ICC500 | 08/01/2025 | 16:57 | PP074182.D | 10.43 | 4.66 |
| AR1254ICC1000 | AR1254ICC1000 | 08/01/2025 | 18:02 | PP074185.D | 10.43 | 4.66 |
| AR1254ICC750 | AR1254ICC750 | 08/01/2025 | 18:18 | PP074186.D | 10.43 | 4.66 |
| AR1254ICC500 | AR1254ICC500 | 08/01/2025 | 18:34 | PP074187.D | 10.43 | 4.66 |
| AR1254ICC250 | AR1254ICC250 | 08/01/2025 | 18:50 | PP074188.D | 10.43 | 4.66 |
| AR1254ICC050 | AR1254ICC050 | 08/01/2025 | 19:23 | PP074189.D | 10.43 | 4.66 |
| AR1262ICC500 | AR1262ICC500 | 08/01/2025 | 19:39 | PP074190.D | 10.43 | 4.66 |
| AR1268ICC500 | AR1268ICC500 | 08/01/2025 | 20:28 | PP074193.D | 10.43 | 4.66 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 09:51 | PP074302.D | 10.43 | 4.66 |
| L.BLK | L.BLK | 08/12/2025 | 10:43 | PP074305.D | 10.44 | 4.66 |
| PB169205BL | PB169205BL | 08/12/2025 | 12:48 | PP074308.D | 10.44 | 4.66 |
| PB169205BS | PB169205BS | 08/12/2025 | 13:05 | PP074309.D | 10.44 | 4.66 |
| BIN0009-DRIVEWAY-TP-SOUTH-EAST | Q2830-01MS | 08/12/2025 | 13:37 | PP074311.D | 10.44 | 4.66 |
| BIN0009-DRIVEWAY-TP-SOUTH-EAST | Q2830-01MSD | 08/12/2025 | 13:53 | PP074312.D | 10.44 | 4.66 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 15:48 | PP074316.D | 10.44 | 4.66 |
| L.BLK | L.BLK | 08/12/2025 | 16:53 | PP074319.D | 10.43 | 4.66 |

Analytical Sequence

Client: First Environment, Inc.

SDG No.: Q2819

Project: USACE018-44 DOD

Instrument ID: ECD_O

GC Column: ZB-MR2

ID: 0.32 (mm)

Inst. Calib. Date(s): 07/23/2025 07/23/2025

THE ANALYTICAL SEQUENCE OF PERFORMANCE EVALUATION MIXTURES, BLANKS, SAMPLES, AND STANDARDS IS GIVEN BELOW:

| CLIENT ID | LAB SAMPLE ID | DATE ANALYZED | TIME ANALYZED | DATAFILE | DCB RT # | TCX RT # |
|---------------|---------------|---------------|---------------|------------|----------|----------|
| I.BLK | I.BLK | 07/23/2025 | 11:14 | PO112413.D | 8.64 | 3.66 |
| AR1660ICC1000 | AR1660ICC1000 | 07/23/2025 | 11:32 | PO112414.D | 8.64 | 3.66 |
| AR1660ICC750 | AR1660ICC750 | 07/23/2025 | 11:50 | PO112415.D | 8.64 | 3.66 |
| AR1660ICC500 | AR1660ICC500 | 07/23/2025 | 12:08 | PO112416.D | 8.64 | 3.66 |
| AR1660ICC250 | AR1660ICC250 | 07/23/2025 | 12:27 | PO112417.D | 8.64 | 3.66 |
| AR1660ICC050 | AR1660ICC050 | 07/23/2025 | 12:45 | PO112418.D | 8.64 | 3.66 |
| AR1221ICC500 | AR1221ICC500 | 07/23/2025 | 13:03 | PO112419.D | 8.64 | 3.66 |
| AR1232ICC500 | AR1232ICC500 | 07/23/2025 | 13:22 | PO112420.D | 8.64 | 3.66 |
| AR1242ICC1000 | AR1242ICC1000 | 07/23/2025 | 13:40 | PO112421.D | 8.64 | 3.66 |
| AR1242ICC750 | AR1242ICC750 | 07/23/2025 | 13:59 | PO112422.D | 8.64 | 3.66 |
| AR1242ICC500 | AR1242ICC500 | 07/23/2025 | 14:17 | PO112423.D | 8.64 | 3.66 |
| AR1242ICC250 | AR1242ICC250 | 07/23/2025 | 14:36 | PO112424.D | 8.64 | 3.66 |
| AR1242ICC050 | AR1242ICC050 | 07/23/2025 | 14:54 | PO112425.D | 8.64 | 3.66 |
| AR1248ICC1000 | AR1248ICC1000 | 07/23/2025 | 15:13 | PO112426.D | 8.64 | 3.66 |
| AR1248ICC750 | AR1248ICC750 | 07/23/2025 | 15:31 | PO112427.D | 8.64 | 3.66 |
| AR1248ICC500 | AR1248ICC500 | 07/23/2025 | 15:48 | PO112428.D | 8.64 | 3.66 |
| AR1248ICC250 | AR1248ICC250 | 07/23/2025 | 16:07 | PO112429.D | 8.64 | 3.66 |
| AR1248ICC050 | AR1248ICC050 | 07/23/2025 | 16:25 | PO112430.D | 8.64 | 3.66 |
| AR1254ICC1000 | AR1254ICC1000 | 07/23/2025 | 16:44 | PO112431.D | 8.64 | 3.66 |
| AR1254ICC750 | AR1254ICC750 | 07/23/2025 | 17:02 | PO112432.D | 8.64 | 3.66 |
| AR1254ICC500 | AR1254ICC500 | 07/23/2025 | 17:21 | PO112433.D | 8.64 | 3.66 |
| AR1254ICC250 | AR1254ICC250 | 07/23/2025 | 17:39 | PO112434.D | 8.64 | 3.66 |
| AR1254ICC050 | AR1254ICC050 | 07/23/2025 | 17:57 | PO112435.D | 8.64 | 3.66 |
| AR1262ICC500 | AR1262ICC500 | 07/23/2025 | 18:16 | PO112436.D | 8.64 | 3.66 |
| AR1268ICC1000 | AR1268ICC1000 | 07/23/2025 | 18:34 | PO112437.D | 8.64 | 3.66 |
| AR1268ICC750 | AR1268ICC750 | 07/23/2025 | 18:53 | PO112438.D | 8.64 | 3.66 |
| AR1268ICC500 | AR1268ICC500 | 07/23/2025 | 19:11 | PO112439.D | 8.64 | 3.66 |
| AR1268ICC250 | AR1268ICC250 | 07/23/2025 | 19:28 | PO112440.D | 8.64 | 3.66 |
| AR1268ICC050 | AR1268ICC050 | 07/23/2025 | 19:47 | PO112441.D | 8.64 | 3.66 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 08:54 | PO112850.D | 8.63 | 3.66 |
| I.BLK | I.BLK | 08/12/2025 | 10:05 | PO112854.D | 8.63 | 3.66 |
| 11M-S | Q2819-06 | 08/12/2025 | 13:26 | PO112860.D | 8.63 | 3.66 |
| 84SB-W | Q2819-11 | 08/12/2025 | 13:43 | PO112861.D | 8.63 | 3.66 |
| 17M-W | Q2819-14 | 08/12/2025 | 14:01 | PO112862.D | 8.63 | 3.66 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 15:50 | PO112865.D | 8.63 | 3.66 |
| I.BLK | I.BLK | 08/12/2025 | 17:00 | PO112869.D | 8.63 | 3.66 |
| I.BLK | I.BLK | 08/01/2025 | 11:49 | PP074167.D | 8.83 | 3.80 |
| AR1660ICC1000 | AR1660ICC1000 | 08/01/2025 | 12:05 | PP074168.D | 8.83 | 3.81 |
| AR1660ICC750 | AR1660ICC750 | 08/01/2025 | 12:22 | PP074169.D | 8.83 | 3.80 |
| AR1660ICC500 | AR1660ICC500 | 08/01/2025 | 12:38 | PP074170.D | 8.83 | 3.81 |
| AR1660ICC250 | AR1660ICC250 | 08/01/2025 | 12:54 | PP074171.D | 8.83 | 3.81 |
| AR1660ICC050 | AR1660ICC050 | 08/01/2025 | 13:42 | PP074172.D | 8.83 | 3.80 |

Analytical Sequence

| | | | | | | |
|--------------------------------|---------------|------------|-------|------------|------|------|
| AR1221ICC500 | AR1221ICC500 | 08/01/2025 | 13:58 | PP074173.D | 8.83 | 3.80 |
| AR1232ICC500 | AR1232ICC500 | 08/01/2025 | 14:15 | PP074174.D | 8.83 | 3.80 |
| AR1242ICC1000 | AR1242ICC1000 | 08/01/2025 | 14:31 | PP074175.D | 8.83 | 3.80 |
| AR1242ICC750 | AR1242ICC750 | 08/01/2025 | 14:47 | PP074176.D | 8.82 | 3.80 |
| AR1242ICC500 | AR1242ICC500 | 08/01/2025 | 15:03 | PP074177.D | 8.83 | 3.81 |
| AR1242ICC250 | AR1242ICC250 | 08/01/2025 | 15:19 | PP074178.D | 8.82 | 3.81 |
| AR1242ICC050 | AR1242ICC050 | 08/01/2025 | 15:36 | PP074179.D | 8.82 | 3.80 |
| AR1248ICC500 | AR1248ICC500 | 08/01/2025 | 16:57 | PP074182.D | 8.82 | 3.81 |
| AR1254ICC1000 | AR1254ICC1000 | 08/01/2025 | 18:02 | PP074185.D | 8.82 | 3.81 |
| AR1254ICC750 | AR1254ICC750 | 08/01/2025 | 18:18 | PP074186.D | 8.82 | 3.80 |
| AR1254ICC500 | AR1254ICC500 | 08/01/2025 | 18:34 | PP074187.D | 8.82 | 3.80 |
| AR1254ICC250 | AR1254ICC250 | 08/01/2025 | 18:50 | PP074188.D | 8.82 | 3.80 |
| AR1254ICC050 | AR1254ICC050 | 08/01/2025 | 19:23 | PP074189.D | 8.82 | 3.80 |
| AR1262ICC500 | AR1262ICC500 | 08/01/2025 | 19:39 | PP074190.D | 8.82 | 3.80 |
| AR1268ICC500 | AR1268ICC500 | 08/01/2025 | 20:28 | PP074193.D | 8.82 | 3.80 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 09:51 | PP074302.D | 8.82 | 3.80 |
| L.BLK | L.BLK | 08/12/2025 | 10:43 | PP074305.D | 8.82 | 3.81 |
| PB169205BL | PB169205BL | 08/12/2025 | 12:48 | PP074308.D | 8.82 | 3.80 |
| PB169205BS | PB169205BS | 08/12/2025 | 13:05 | PP074309.D | 8.82 | 3.80 |
| BIN0009-DRIVEWAY-TP-SOUTH-EAST | Q2830-01MS | 08/12/2025 | 13:37 | PP074311.D | 8.82 | 3.80 |
| BIN0009-DRIVEWAY-TP-SOUTH-EAST | Q2830-01MSD | 08/12/2025 | 13:53 | PP074312.D | 8.82 | 3.80 |
| AR1660CCC500 | AR1660CCC500 | 08/12/2025 | 15:48 | PP074316.D | 8.82 | 3.80 |
| L.BLK | L.BLK | 08/12/2025 | 16:53 | PP074319.D | 8.82 | 3.80 |



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES

SAMPLE NO.

PB169205BS

Lab Name: Alliance Contract: FIRS02
Lab Code: ACE SDG NO.: Q2819
Lab Sample ID: PB169205BS Date(s) Analyzed: 08/12/2025 08/12/2025
Instrument ID (1): ECD_P Instrument ID (2): ECD_P
GC Column: (1): ZB-MR1 ID: 0.32 (mm) GC Column: (2): ZB-MR2 ID: 0.32 (mm)
Data file PP074309.D

| ANALYTE | COL | RT | RT WINDOW FROM | TO | CONCENTRATION | MEAN CONCENTRATION | %RPD | |
|--------------|-----|-------|-------------------|-------|---------------|-----------------------|------|--|
| Aroclor-1016 | 1 | 5.809 | 5.759 | 5.859 | 183 | 185 | 1.09 | |
| | 2 | 5.83 | 5.78 | 5.88 | 187 | | | |
| | 3 | 5.893 | 5.843 | 5.943 | 187 | | | |
| | 4 | 5.99 | 5.94 | 6.04 | 188 | | | |
| | 5 | 6.283 | 6.233 | 6.333 | 180 | | | |
| | 1 | 4.902 | 4.852 | 4.952 | 191 | 183 | | |
| | 2 | 4.959 | 4.909 | 5.009 | 185 | | | |
| | 3 | 5.08 | 5.03 | 5.13 | 176 | | | |
| | 4 | 5.121 | 5.071 | 5.171 | 172 | | | |
| | 5 | 5.334 | 5.284 | 5.384 | 191 | | | |
| Aroclor-1260 | 1 | 7.401 | 7.351 | 7.451 | 183 | 165 | 8.7 | |
| | 2 | 7.653 | 7.603 | 7.703 | 176 | | | |
| | 3 | 8.012 | 7.962 | 8.062 | 152 | | | |
| | 4 | 8.238 | 8.188 | 8.288 | 165 | | | |
| | 5 | 8.566 | 8.516 | 8.616 | 150 | | | |
| | 1 | 6.551 | 6.501 | 6.601 | 195 | 180 | | |
| | 2 | 6.706 | 6.656 | 6.756 | 195 | | | |
| | 3 | 6.915 | 6.865 | 6.965 | 173 | | | |
| | 4 | 7.175 | 7.125 | 7.225 | 171 | | | |
| | 5 | 7.415 | 7.365 | 7.465 | 168 | | | |

**IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES**

SAMPLE NO.

BIN0009-DRIVEWAY-TP.

| | | | | | | | |
|--------------------|------------|--------------------|-----------------------|-----------------|--------|-----|-----------|
| Lab Name: | Alliance | Contract: | FIRS02 | | | | |
| Lab Code: | ACE | SDG NO.: | Q2819 | | | | |
| Lab Sample ID: | Q2830-01MS | Date(s) Analyzed: | 08/12/2025 08/12/2025 | | | | |
| Instrument ID (1): | ECD_P | Instrument ID (2): | ECD_P | | | | |
| GC Column: (1): | ZB-MR1 | ID: | 0.32 (mm) | GC Column: (2): | ZB-MR2 | ID: | 0.32 (mm) |
| Data file | PP074311.D | | | | | | |

| ANALYTE | COL | RT | RT WINDOW | | CONCENTRATION | MEAN CONCENTRATION | %RPD | |
|--------------|-----|-------|-----------|-------|---------------|--------------------|------|--|
| | | | FROM | TO | | | | |
| Aroclor-1016 | 1 | 5.809 | 5.759 | 5.859 | 200 | 201 | 5.8 | |
| | 2 | 5.831 | 5.781 | 5.881 | 201 | | | |
| | 3 | 5.894 | 5.844 | 5.944 | 200 | | | |
| | 4 | 5.991 | 5.941 | 6.041 | 209 | | | |
| | 5 | 6.283 | 6.233 | 6.333 | 195 | | | |
| | 1 | 4.901 | 4.851 | 4.951 | 213 | 213 | | |
| | 2 | 4.958 | 4.908 | 5.008 | 215 | | | |
| | 3 | 5.079 | 5.029 | 5.129 | 219 | | | |
| | 4 | 5.119 | 5.069 | 5.169 | 206 | | | |
| | 5 | 5.334 | 5.284 | 5.384 | 212 | | | |
| Aroclor-1260 | 1 | 7.4 | 7.35 | 7.45 | 191 | 173 | 4.52 | |
| | 2 | 7.653 | 7.603 | 7.703 | 183 | | | |
| | 3 | 8.012 | 7.962 | 8.062 | 157 | | | |
| | 4 | 8.238 | 8.188 | 8.288 | 181 | | | |
| | 5 | 8.566 | 8.516 | 8.616 | 155 | | | |
| | 1 | 6.55 | 6.5 | 6.6 | 196 | 181 | | |
| | 2 | 6.704 | 6.654 | 6.754 | 193 | | | |
| | 3 | 6.914 | 6.864 | 6.964 | 172 | | | |
| | 4 | 7.175 | 7.125 | 7.225 | 175 | | | |
| | 5 | 7.413 | 7.363 | 7.463 | 170 | | | |

**IDENTIFICATION SUMMARY
FOR MULTICOMPONENT ANALYTES**

SAMPLE NO.

BIN0009-DRIVEWAY-TP.

| | | | | | | | |
|--------------------|-------------|--------------------|-----------------------|-----------------|--------|-----|-----------|
| Lab Name: | Alliance | Contract: | FIRS02 | | | | |
| Lab Code: | ACE | SDG NO.: | Q2819 | | | | |
| Lab Sample ID: | Q2830-01MSD | Date(s) Analyzed: | 08/12/2025 08/12/2025 | | | | |
| Instrument ID (1): | ECD_P | Instrument ID (2): | ECD_P | | | | |
| GC Column: (1): | ZB-MR1 | ID: | 0.32 (mm) | GC Column: (2): | ZB-MR2 | ID: | 0.32 (mm) |
| Data file | PP074312.D | | | | | | |

| ANALYTE | COL | RT | RT WINDOW | | CONCENTRATION | MEAN CONCENTRATION | %RPD | |
|--------------|-----|-------|-----------|-------|---------------|--------------------|------|--|
| | | | FROM | TO | | | | |
| Aroclor-1016 | 1 | 5.811 | 5.761 | 5.861 | 205 | 213 | 2.78 | |
| | 2 | 5.832 | 5.782 | 5.882 | 202 | | | |
| | 3 | 5.895 | 5.845 | 5.945 | 204 | | | |
| | 4 | 5.992 | 5.942 | 6.042 | 256 | | | |
| | 5 | 6.284 | 6.234 | 6.334 | 199 | | | |
| | 1 | 4.904 | 4.854 | 4.954 | 220 | 219 | | |
| | 2 | 4.961 | 4.911 | 5.011 | 222 | | | |
| | 3 | 5.081 | 5.031 | 5.131 | 215 | | | |
| | 4 | 5.122 | 5.072 | 5.172 | 218 | | | |
| | 5 | 5.337 | 5.287 | 5.387 | 219 | | | |
| Aroclor-1260 | 1 | 7.402 | 7.352 | 7.452 | 197 | 177 | 6.03 | |
| | 2 | 7.654 | 7.604 | 7.704 | 186 | | | |
| | 3 | 8.012 | 7.962 | 8.062 | 160 | | | |
| | 4 | 8.239 | 8.189 | 8.289 | 183 | | | |
| | 5 | 8.565 | 8.515 | 8.615 | 159 | | | |
| | 1 | 6.552 | 6.502 | 6.602 | 206 | 188 | | |
| | 2 | 6.707 | 6.657 | 6.757 | 201 | | | |
| | 3 | 6.916 | 6.866 | 6.966 | 178 | | | |
| | 4 | 7.176 | 7.126 | 7.226 | 180 | | | |
| | 5 | 7.415 | 7.365 | 7.465 | 176 | | | |



QC SAMPLE

DATA



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | |
|--------------------|-------------------------|--------|----|--------------------|---------------|
| Client: | First Environment, Inc. | | | Date Collected: | |
| Project: | USACE018-44 DOD | | | Date Received: | |
| Client Sample ID: | PB169205BL | | | SDG No.: | Q2819 |
| Lab Sample ID: | PB169205BL | | | Matrix: | SOIL |
| Analytical Method: | 8082A | | | % Solid: | 100 Decanted: |
| Sample Wt/Vol: | 30.03 | Units: | g | Final Vol: | 10000 uL |
| Soil Aliquot Vol: | | | uL | Test: | PCB |
| Extraction Type: | | | | Injection Volume : | |
| GPC Factor : | 1.0 | PH : | | | |
| Prep Method : | SW3541B | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PP074308.D | 1 | 08/12/25 08:15 | 08/12/25 12:48 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 8.30 | U | 3.90 | 8.30 | 17.0 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 13.0 | U | 4.00 | 13.0 | 17.0 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 8.30 | U | 3.70 | 8.30 | 17.0 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 8.30 | U | 4.00 | 8.30 | 17.0 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 13.0 | U | 5.90 | 13.0 | 17.0 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 8.30 | U | 3.20 | 8.30 | 17.0 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 13.0 | U | 5.00 | 13.0 | 17.0 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 8.30 | U | 3.60 | 8.30 | 17.0 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 8.30 | U | 3.20 | 8.30 | 17.0 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 23.1 | | 44 - 130 | | 116% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 22.2 | | 60 - 125 | | 111% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 12:48
Operator : YP\AJ
Sample : PB169205BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB169205BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 13:31:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.656 | 3.798 | 25834612 | 77167851 | 23.102 | 20.125 |
| 2) SA Decachlor... | 10.439 | 8.817 | 21524564 | 120.6E6 | 22.164 | 20.052 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 12:48
 Operator : YP\AJ
 Sample : PB169205BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB169205BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 13:31:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

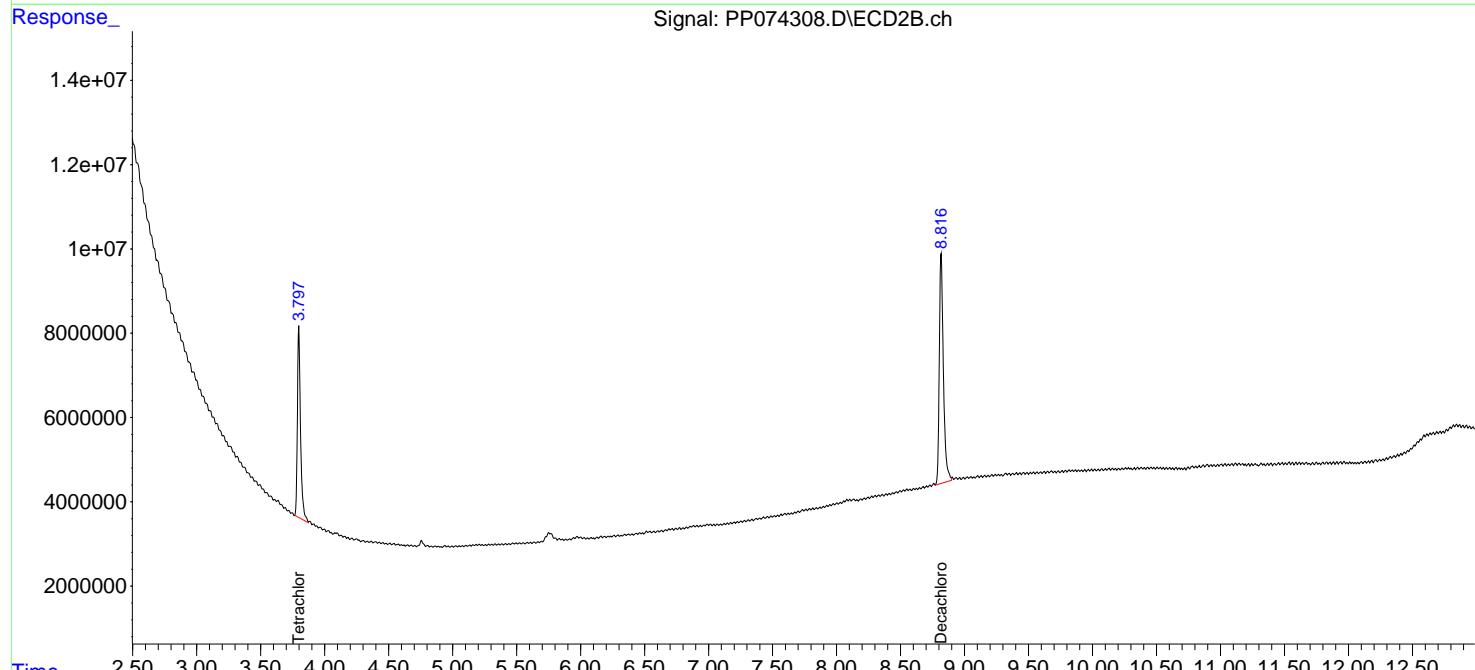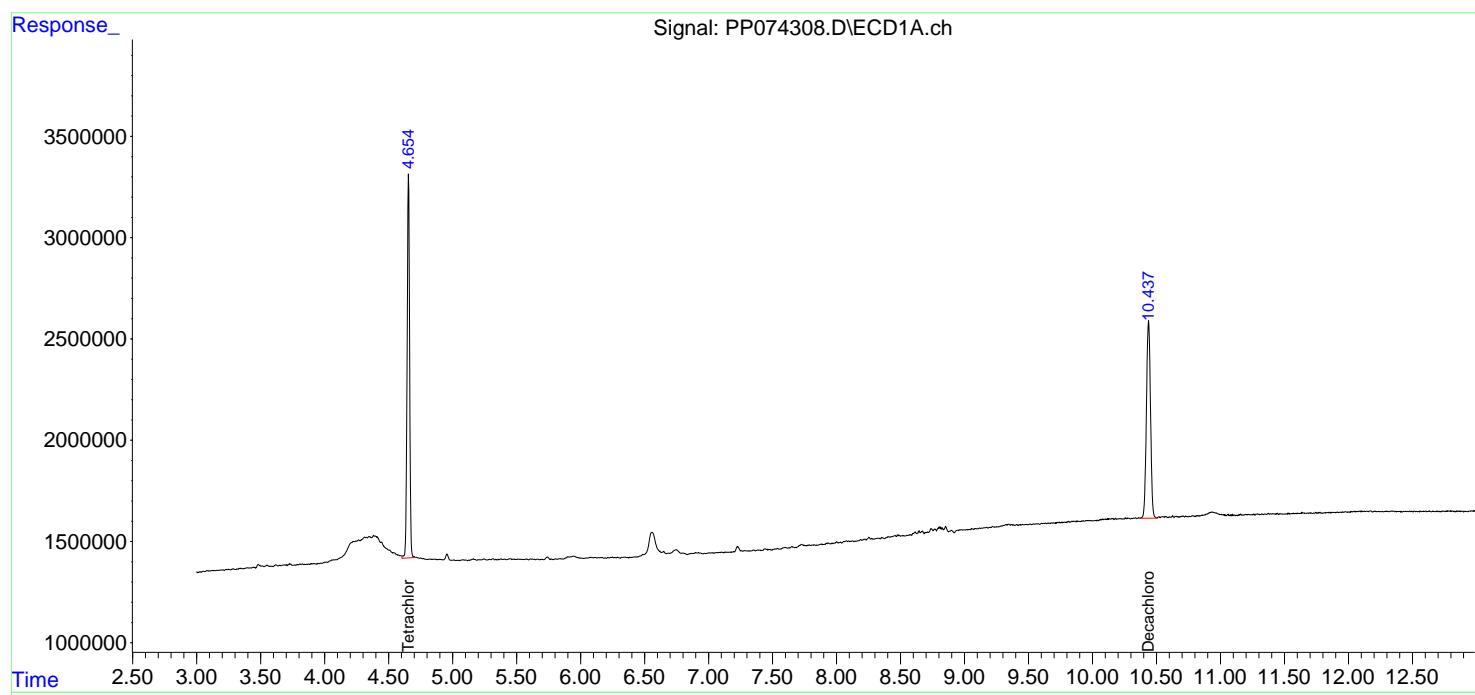

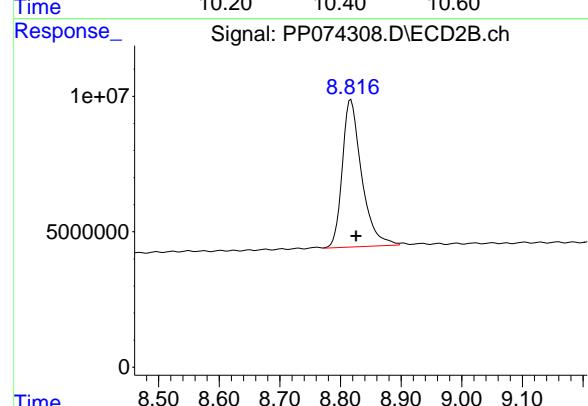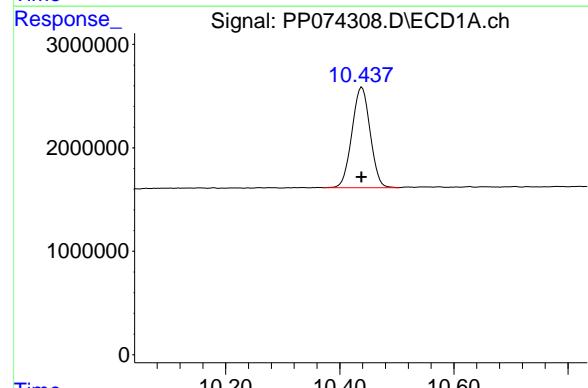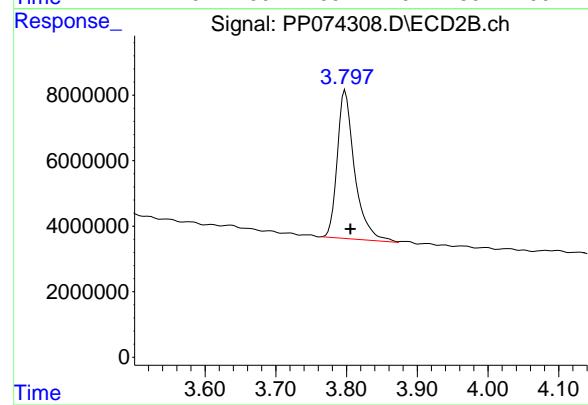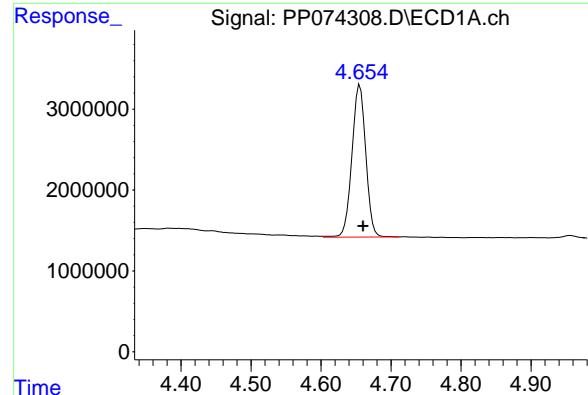

#1 Tetrachloro-m-xylene

R.T.: 4.656 min
 Delta R.T.: -0.004 min
 Response: 25834612
 Conc: 23.10 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BL

#1 Tetrachloro-m-xylene

R.T.: 3.798 min
 Delta R.T.: -0.007 min
 Response: 77167851
 Conc: 20.13 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.439 min
 Delta R.T.: 0.000 min
 Response: 21524564
 Conc: 22.16 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.817 min
 Delta R.T.: -0.009 min
 Response: 120583654
 Conc: 20.05 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | | | |
|--------------------|-------------------------|--------|----|--------------------|----------|-----------|--|--|
| Client: | First Environment, Inc. | | | Date Collected: | 07/23/25 | | | |
| Project: | USACE018-44 DOD | | | Date Received: | 07/23/25 | | | |
| Client Sample ID: | PIBLK-PO112413.D | | | SDG No.: | Q2819 | | | |
| Lab Sample ID: | I.BLK-PO112413.D | | | Matrix: | WATER | | | |
| Analytical Method: | 8082A | | | % Solid: | 0 | Decanted: | | |
| Sample Wt/Vol: | 1000 | Units: | mL | Final Vol: | 10000 | uL | | |
| Soil Aliquot Vol: | uL | | | Test: | PCB | | | |
| Extraction Type: | | | | Injection Volume : | | | | |
| GPC Factor : | 1.0 | PH : | | | | | | |
| Prep Method : | 5030 | | | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|-----------|---------------|---------------|
| PO112413.D | 1 | | 07/23/25 | PO072325 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units |
|-------------------|----------------------|-------|-----------|----------|------|------------|---------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 0.25 | U | 0.097 | 0.25 | 0.50 | ug/L |
| 11104-28-2 | Aroclor-1221 | 0.40 | U | 0.13 | 0.40 | 0.50 | ug/L |
| 11141-16-5 | Aroclor-1232 | 0.25 | U | 0.096 | 0.25 | 0.50 | ug/L |
| 53469-21-9 | Aroclor-1242 | 0.25 | U | 0.12 | 0.25 | 0.50 | ug/L |
| 12672-29-6 | Aroclor-1248 | 0.25 | U | 0.071 | 0.25 | 0.50 | ug/L |
| 11097-69-1 | Aroclor-1254 | 0.25 | U | 0.094 | 0.25 | 0.50 | ug/L |
| 11096-82-5 | Aroclor-1260 | 0.25 | U | 0.081 | 0.25 | 0.50 | ug/L |
| 37324-23-5 | Aroclor-1262 | 0.40 | U | 0.14 | 0.40 | 0.50 | ug/L |
| 11100-14-4 | Aroclor-1268 | 0.25 | U | 0.11 | 0.25 | 0.50 | ug/L |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 19.1 | | 60 - 140 | | 95% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 20.0 | | 60 - 140 | | 100% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
Data File : P0112413.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Jul 2025 11:14
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jul 24 05:03:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 155.1E6 | 97072114 | 19.073 | 19.535 |
| 2) SA Decachlor... | 8.694 | 8.640 | 146.0E6 | 36122645 | 19.970 | 20.442 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.





Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112413.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 11:14
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 24 05:03:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

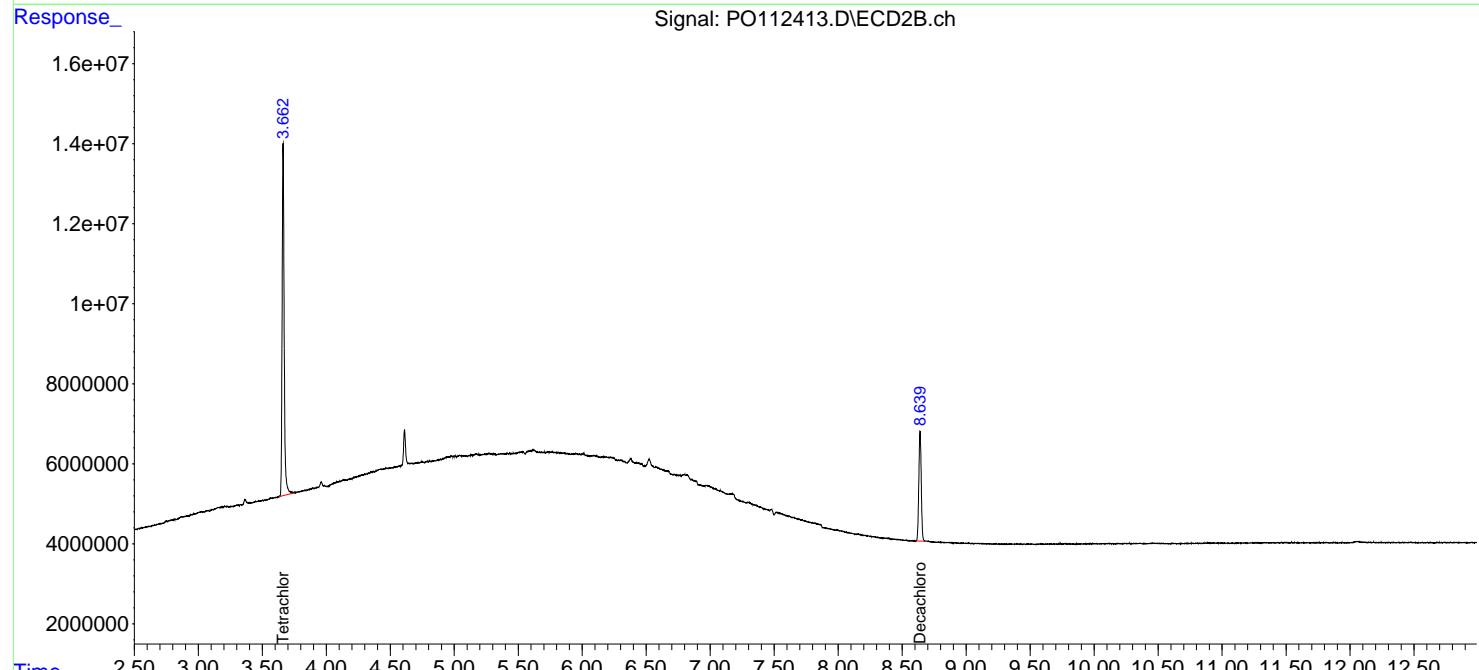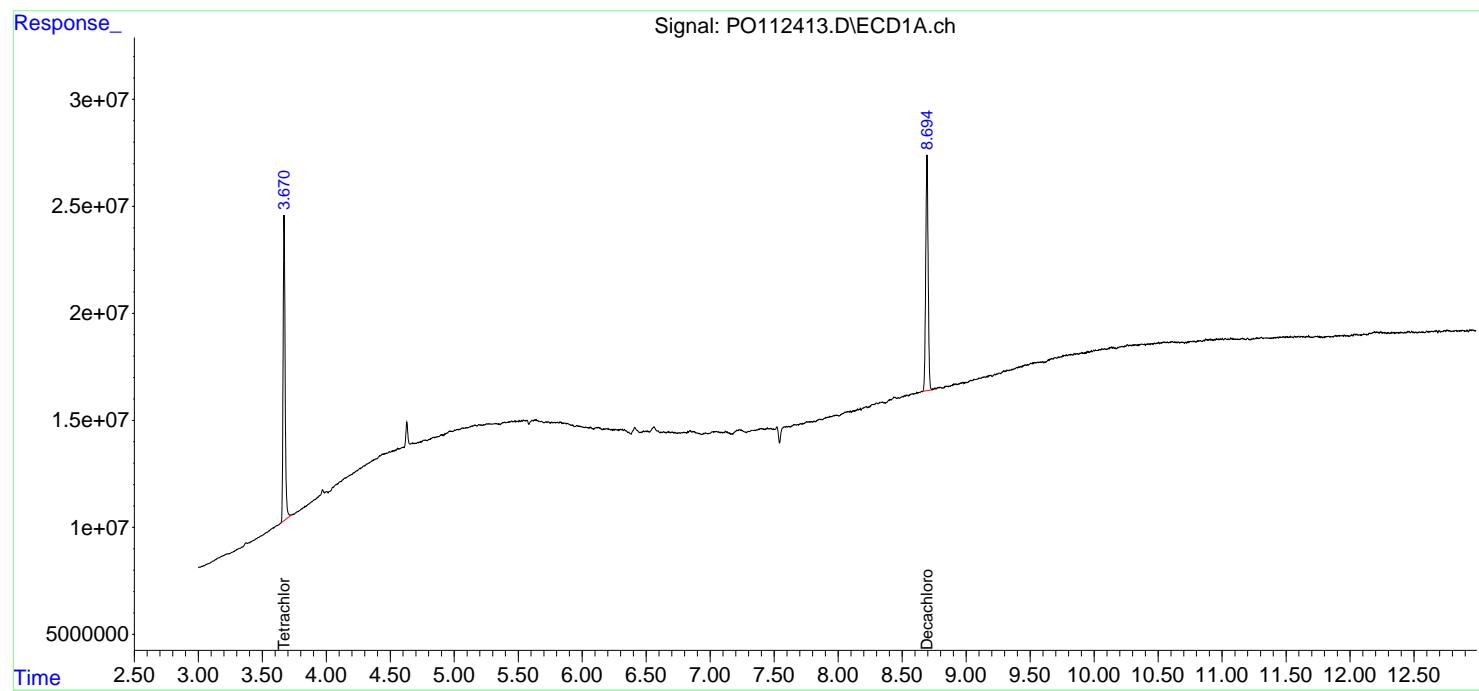

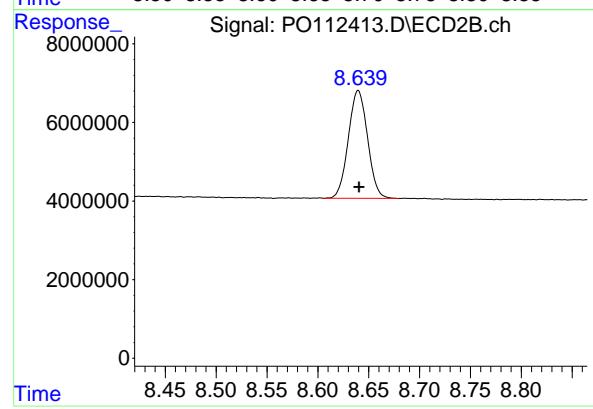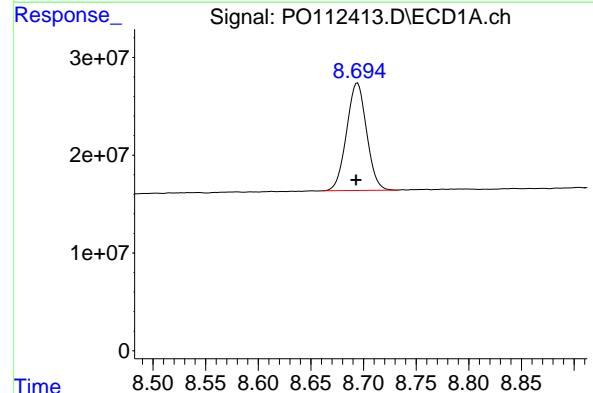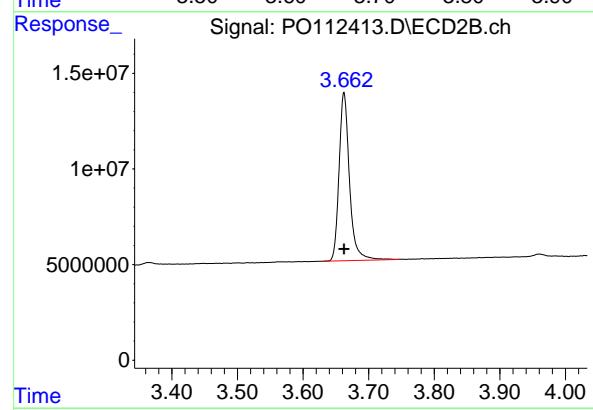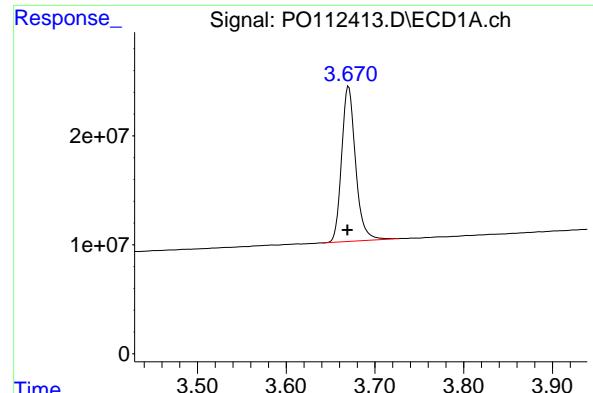

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
Delta R.T.: 0.001 min
Response: 155090113
Conc: 19.07 ng/ml

Instrument:

ECD_O

ClientSampleId :

I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 97072114
Conc: 19.53 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
Delta R.T.: 0.001 min
Response: 146014518
Conc: 19.97 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 36122645
Conc: 20.44 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | | | |
|--------------------|-------------------------|--------|----|--------------------|----------|-----------|--|--|
| Client: | First Environment, Inc. | | | Date Collected: | 08/12/25 | | | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/12/25 | | | |
| Client Sample ID: | PIBLK-PO112854.D | | | SDG No.: | Q2819 | | | |
| Lab Sample ID: | I.BLK-PO112854.D | | | Matrix: | WATER | | | |
| Analytical Method: | 8082A | | | % Solid: | 0 | Decanted: | | |
| Sample Wt/Vol: | 1000 | Units: | mL | Final Vol: | 10000 | uL | | |
| Soil Aliquot Vol: | uL | | | Test: | PCB | | | |
| Extraction Type: | | | | Injection Volume : | | | | |
| GPC Factor : | 1.0 | PH : | | | | | | |
| Prep Method : | 5030 | | | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|-----------|---------------|---------------|
| PO112854.D | 1 | | 08/12/25 | PO081225 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units |
|-------------------|----------------------|-------|-----------|----------|------|------------|---------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 0.25 | U | 0.097 | 0.25 | 0.50 | ug/L |
| 11104-28-2 | Aroclor-1221 | 0.40 | U | 0.13 | 0.40 | 0.50 | ug/L |
| 11141-16-5 | Aroclor-1232 | 0.25 | U | 0.096 | 0.25 | 0.50 | ug/L |
| 53469-21-9 | Aroclor-1242 | 0.25 | U | 0.12 | 0.25 | 0.50 | ug/L |
| 12672-29-6 | Aroclor-1248 | 0.25 | U | 0.071 | 0.25 | 0.50 | ug/L |
| 11097-69-1 | Aroclor-1254 | 0.25 | U | 0.094 | 0.25 | 0.50 | ug/L |
| 11096-82-5 | Aroclor-1260 | 0.25 | U | 0.081 | 0.25 | 0.50 | ug/L |
| 37324-23-5 | Aroclor-1262 | 0.40 | U | 0.14 | 0.40 | 0.50 | ug/L |
| 11100-14-4 | Aroclor-1268 | 0.25 | U | 0.11 | 0.25 | 0.50 | ug/L |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 20.5 | | 60 - 140 | | 102% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 17.2 | | 60 - 140 | | 86% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 10:05
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:05:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.664 | 3.658 | 170.0E6 | 101.6E6 | 20.911 | 20.456 |
| 2) SA Decachlor... | 8.685 | 8.632 | 126.0E6 | 36010722 | 17.231 | 20.378 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 10:05
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:05:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

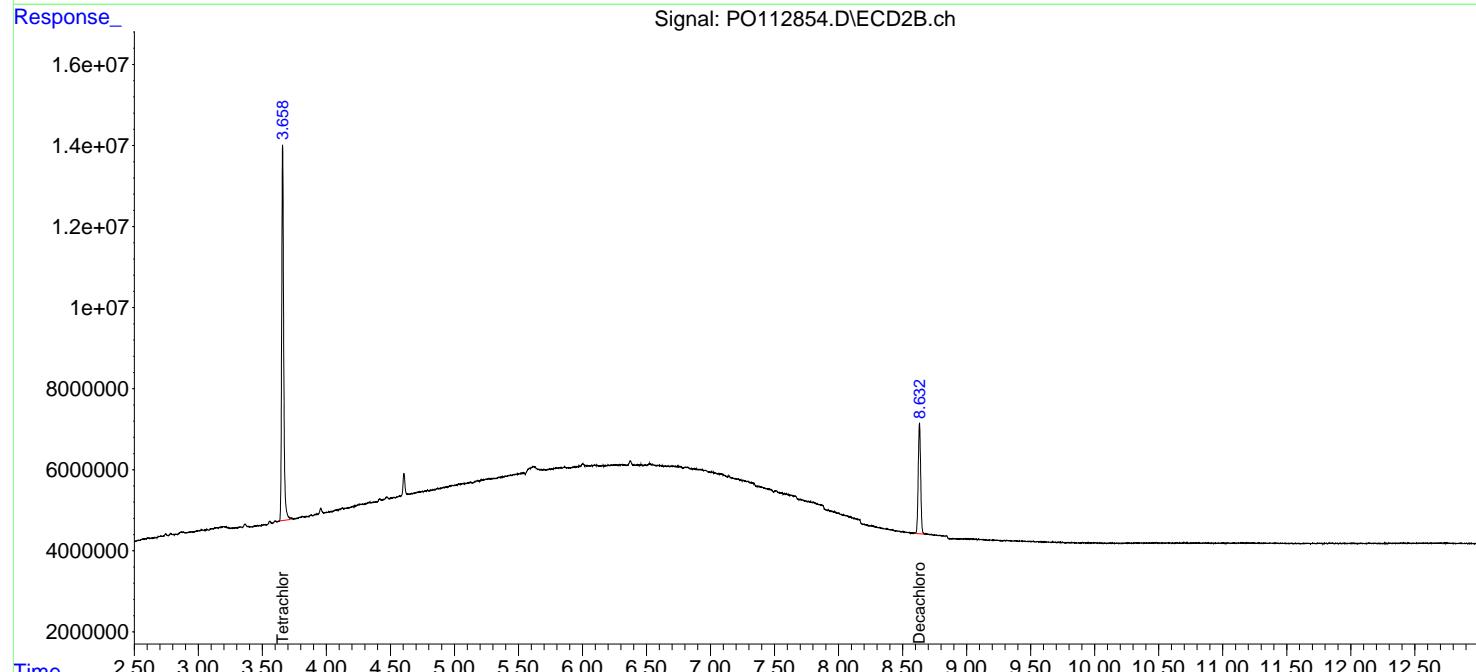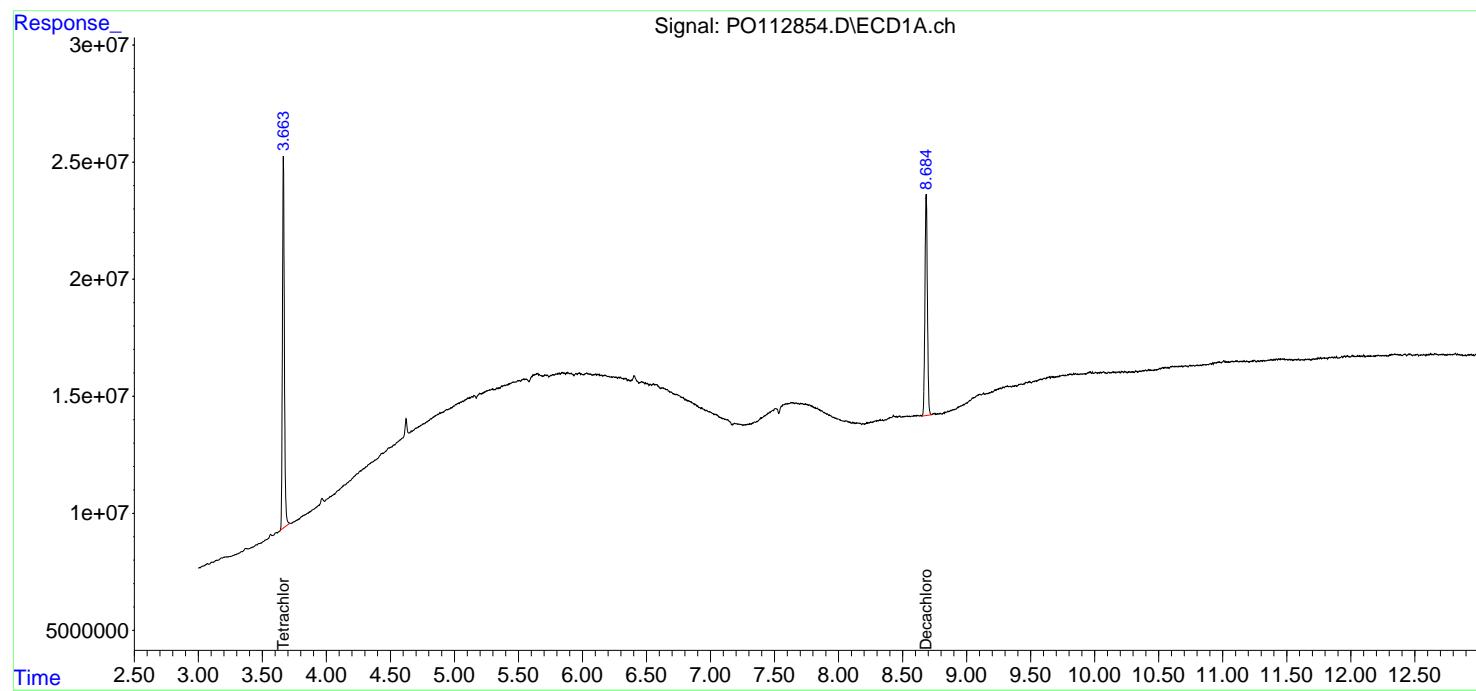

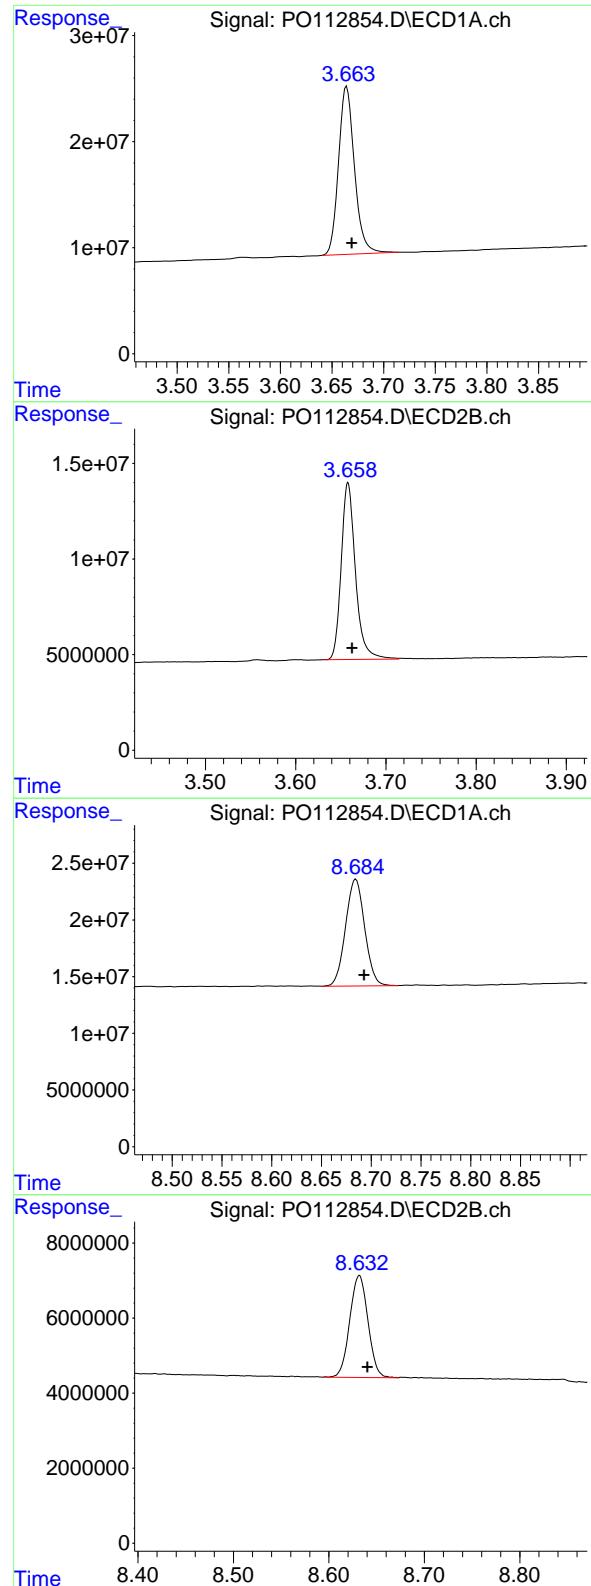

#1 Tetrachloro-m-xylene

R.T.: 3.664 min
 Delta R.T.: -0.005 min
 Response: 170038746
 Conc: 20.91 ng/ml

Instrument: ECD_O
 ClientSampleId: I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.658 min
 Delta R.T.: -0.004 min
 Response: 101647548
 Conc: 20.46 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.685 min
 Delta R.T.: -0.008 min
 Response: 125986606
 Conc: 17.23 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.632 min
 Delta R.T.: -0.008 min
 Response: 36010722
 Conc: 20.38 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | |
|--------------------|-------------------------|--------|----|--------------------|----------|-----------|
| Client: | First Environment, Inc. | | | Date Collected: | 08/12/25 | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/12/25 | |
| Client Sample ID: | PIBLK-PO112869.D | | | SDG No.: | Q2819 | |
| Lab Sample ID: | I.BLK-PO112869.D | | | Matrix: | WATER | |
| Analytical Method: | 8082A | | | % Solid: | 0 | Decanted: |
| Sample Wt/Vol: | 1000 | Units: | mL | Final Vol: | 10000 | uL |
| Soil Aliquot Vol: | uL | | | Test: | PCB | |
| Extraction Type: | | | | Injection Volume : | | |
| GPC Factor : | 1.0 | PH : | | | | |
| Prep Method : | 5030 | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|-----------|---------------|---------------|
| PO112869.D | 1 | | 08/12/25 | po081225 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units |
|-------------------|----------------------|-------|-----------|----------|------|------------|---------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 0.25 | U | 0.097 | 0.25 | 0.50 | ug/L |
| 11104-28-2 | Aroclor-1221 | 0.40 | U | 0.13 | 0.40 | 0.50 | ug/L |
| 11141-16-5 | Aroclor-1232 | 0.25 | U | 0.096 | 0.25 | 0.50 | ug/L |
| 53469-21-9 | Aroclor-1242 | 0.25 | U | 0.12 | 0.25 | 0.50 | ug/L |
| 12672-29-6 | Aroclor-1248 | 0.25 | U | 0.071 | 0.25 | 0.50 | ug/L |
| 11097-69-1 | Aroclor-1254 | 0.25 | U | 0.094 | 0.25 | 0.50 | ug/L |
| 11096-82-5 | Aroclor-1260 | 0.25 | U | 0.081 | 0.25 | 0.50 | ug/L |
| 37324-23-5 | Aroclor-1262 | 0.40 | U | 0.14 | 0.40 | 0.50 | ug/L |
| 11100-14-4 | Aroclor-1268 | 0.25 | U | 0.11 | 0.25 | 0.50 | ug/L |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 20.3 | | 60 - 140 | | 102% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 19.2 | | 60 - 140 | | 96% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
Data File : P0112869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 17:00
Operator : YP/AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:40:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Jul 24 04:54:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.667 | 3.660 | 168.1E6 | 101.0E6 | 20.674 | 20.323 |
| 2) SA Decachlor... | 8.688 | 8.633 | 140.3E6 | 36246288 | 19.192 | 20.512 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 17:00
 Operator : YP/AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:40:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

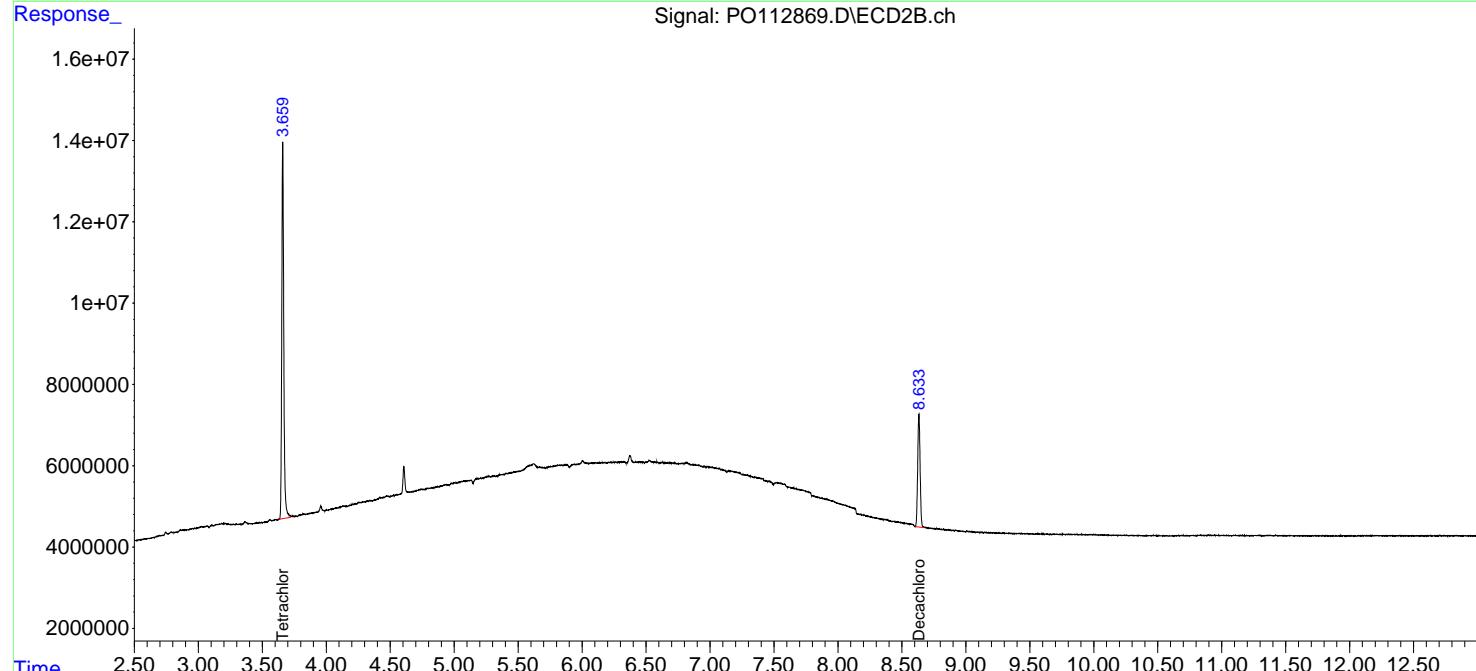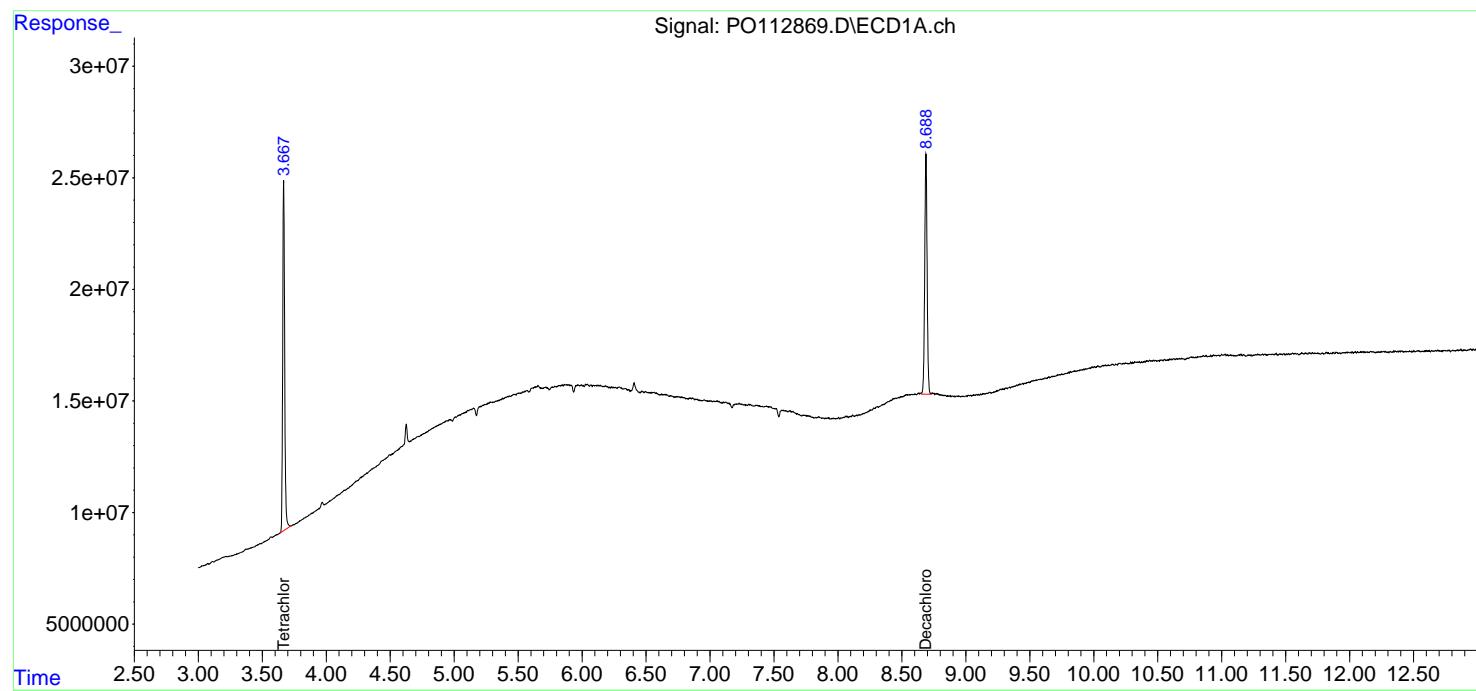

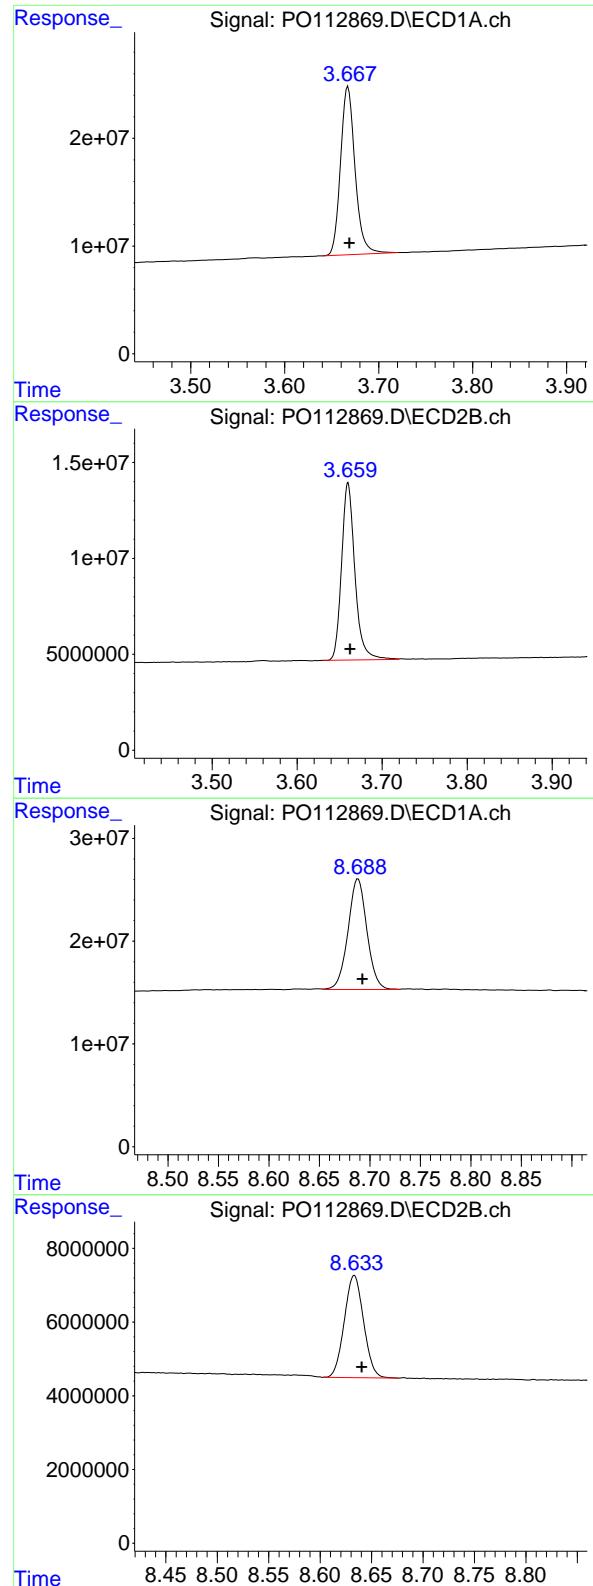

#1 Tetrachloro-m-xylene

R.T.: 3.667 min
Delta R.T.: -0.002 min
Response: 168114131
Conc: 20.67 ng/ml

Instrument:

ECD_O

ClientSampleId:
I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.660 min
Delta R.T.: -0.003 min
Response: 100987501
Conc: 20.32 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.688 min
Delta R.T.: -0.004 min
Response: 140325611
Conc: 19.19 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: -0.007 min
Response: 36246288
Conc: 20.51 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | | | |
|--------------------|-------------------------|--------|----|--------------------|----------|-----------|--|--|
| Client: | First Environment, Inc. | | | Date Collected: | 08/01/25 | | | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/01/25 | | | |
| Client Sample ID: | PIBLK-PP074167.D | | | SDG No.: | Q2819 | | | |
| Lab Sample ID: | I.BLK-PP074167.D | | | Matrix: | WATER | | | |
| Analytical Method: | 8082A | | | % Solid: | 0 | Decanted: | | |
| Sample Wt/Vol: | 1000 | Units: | mL | Final Vol: | 10000 | uL | | |
| Soil Aliquot Vol: | uL | | | Test: | PCB | | | |
| Extraction Type: | | | | Injection Volume : | | | | |
| GPC Factor : | 1.0 | PH : | | | | | | |
| Prep Method : | 5030 | | | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|-----------|---------------|---------------|
| PP074167.D | 1 | | 08/01/25 | PP080125 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units |
|-------------------|----------------------|-------|-----------|----------|------|------------|---------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 0.25 | U | 0.097 | 0.25 | 0.50 | ug/L |
| 11104-28-2 | Aroclor-1221 | 0.40 | U | 0.13 | 0.40 | 0.50 | ug/L |
| 11141-16-5 | Aroclor-1232 | 0.25 | U | 0.096 | 0.25 | 0.50 | ug/L |
| 53469-21-9 | Aroclor-1242 | 0.25 | U | 0.12 | 0.25 | 0.50 | ug/L |
| 12672-29-6 | Aroclor-1248 | 0.25 | U | 0.071 | 0.25 | 0.50 | ug/L |
| 11097-69-1 | Aroclor-1254 | 0.25 | U | 0.094 | 0.25 | 0.50 | ug/L |
| 11096-82-5 | Aroclor-1260 | 0.25 | U | 0.081 | 0.25 | 0.50 | ug/L |
| 37324-23-5 | Aroclor-1262 | 0.40 | U | 0.14 | 0.40 | 0.50 | ug/L |
| 11100-14-4 | Aroclor-1268 | 0.25 | U | 0.11 | 0.25 | 0.50 | ug/L |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 17.3 | | 60 - 140 | | 86% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 18.7 | | 60 - 140 | | 93% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 11:49
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:35:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 21300659 | 66146859 | 19.047 | 17.251 |
| 2) SA Decachlor... | 10.435 | 8.825 | 19096192 | 112.2E6 | 19.663 | 18.655 |

Target Compounds


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074167.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 11:49
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:35:26 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

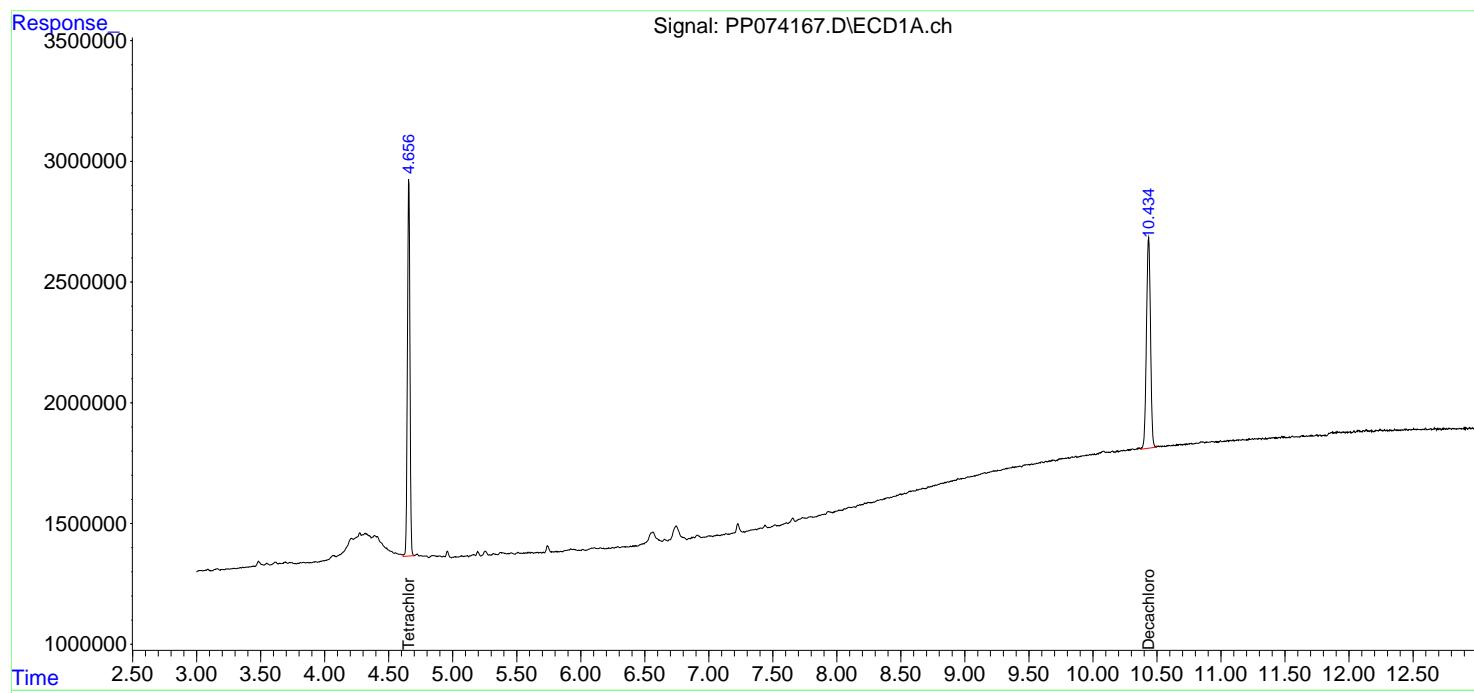

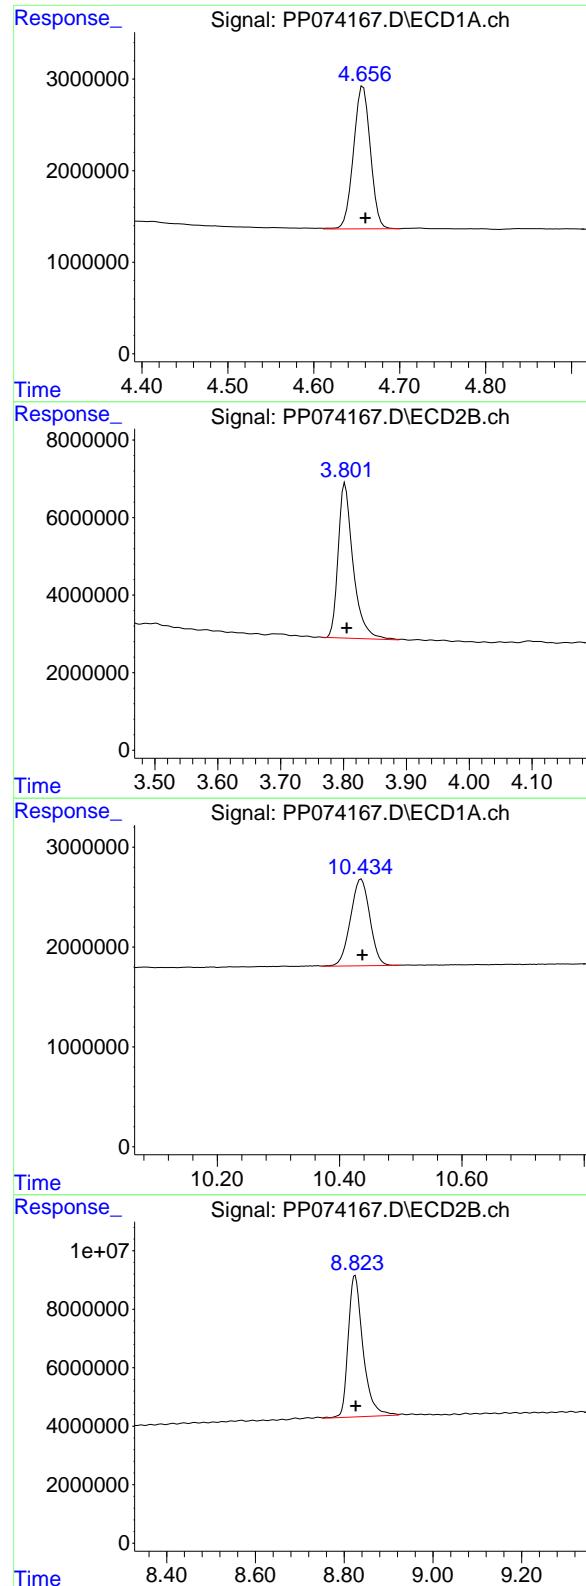

#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: -0.002 min
Response: 21300659
Conc: 19.05 ng/ml

Instrument : ECD_P

ClientSampleId : I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: -0.002 min
Response: 66146859
Conc: 17.25 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: -0.002 min
Response: 19096192
Conc: 19.66 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.825 min
Delta R.T.: -0.002 min
Response: 112184396
Conc: 18.66 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | | | |
|--------------------|-------------------------|--------|----|--------------------|----------|-----------|--|--|
| Client: | First Environment, Inc. | | | Date Collected: | 08/12/25 | | | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/12/25 | | | |
| Client Sample ID: | PIBLK-PP074305.D | | | SDG No.: | Q2819 | | | |
| Lab Sample ID: | I.BLK-PP074305.D | | | Matrix: | WATER | | | |
| Analytical Method: | 8082A | | | % Solid: | 0 | Decanted: | | |
| Sample Wt/Vol: | 1000 | Units: | mL | Final Vol: | 10000 | uL | | |
| Soil Aliquot Vol: | uL | | | Test: | PCB | | | |
| Extraction Type: | | | | Injection Volume : | | | | |
| GPC Factor : | 1.0 | PH : | | | | | | |
| Prep Method : | 5030 | | | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|-----------|---------------|---------------|
| PP074305.D | 1 | | 08/12/25 | PP081225 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units |
|-------------------|----------------------|-------|-----------|----------|------|------------|---------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 0.25 | U | 0.097 | 0.25 | 0.50 | ug/L |
| 11104-28-2 | Aroclor-1221 | 0.40 | U | 0.13 | 0.40 | 0.50 | ug/L |
| 11141-16-5 | Aroclor-1232 | 0.25 | U | 0.096 | 0.25 | 0.50 | ug/L |
| 53469-21-9 | Aroclor-1242 | 0.25 | U | 0.12 | 0.25 | 0.50 | ug/L |
| 12672-29-6 | Aroclor-1248 | 0.25 | U | 0.071 | 0.25 | 0.50 | ug/L |
| 11097-69-1 | Aroclor-1254 | 0.25 | U | 0.094 | 0.25 | 0.50 | ug/L |
| 11096-82-5 | Aroclor-1260 | 0.25 | U | 0.081 | 0.25 | 0.50 | ug/L |
| 37324-23-5 | Aroclor-1262 | 0.40 | U | 0.14 | 0.40 | 0.50 | ug/L |
| 11100-14-4 | Aroclor-1268 | 0.25 | U | 0.11 | 0.25 | 0.50 | ug/L |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 19.7 | | 60 - 140 | | 98% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 18.5 | | 60 - 140 | | 93% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074305.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 10:43
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 11:31:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.661 | 3.805 | 24597780 | 75474847 | 21.996 | 19.683 |
| 2) SA Decachlor... | 10.437 | 8.822 | 20447388 | 111.5E6 | 21.055 | 18.538 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074305.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 10:43
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 11:31:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

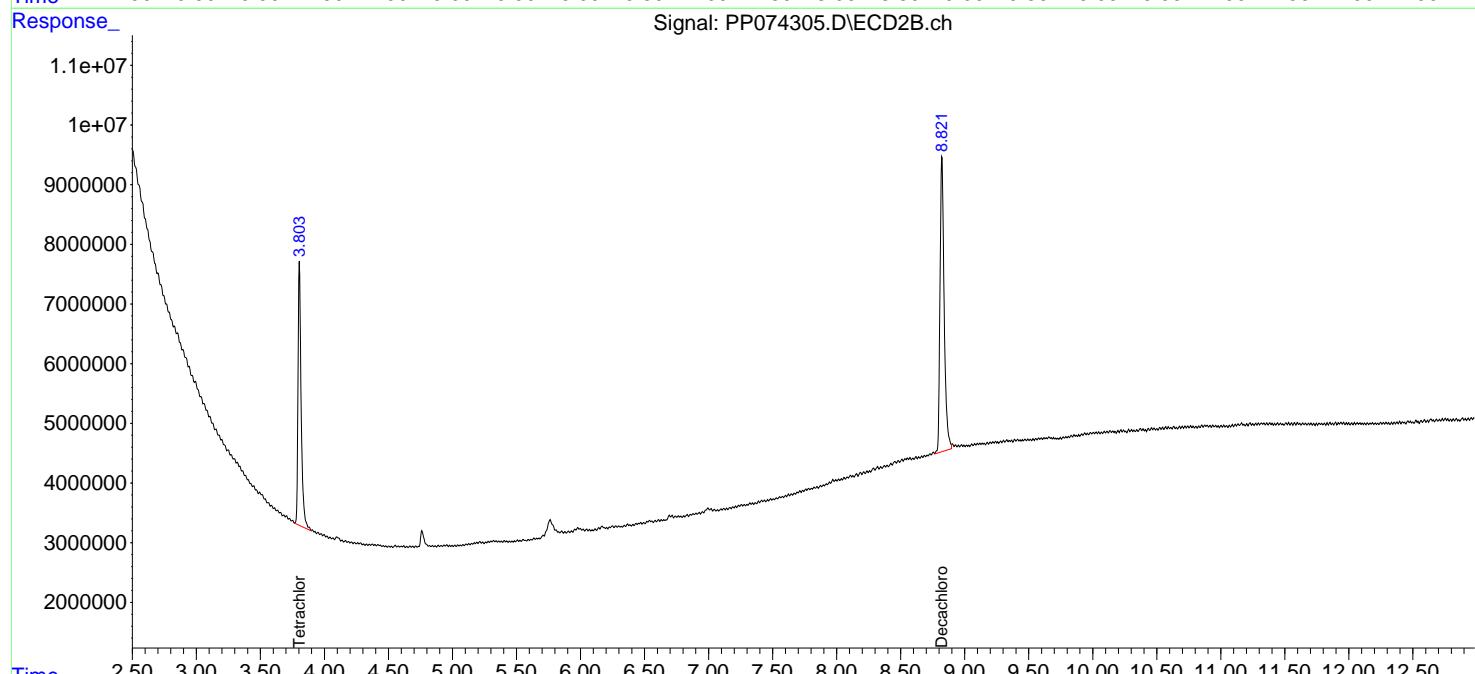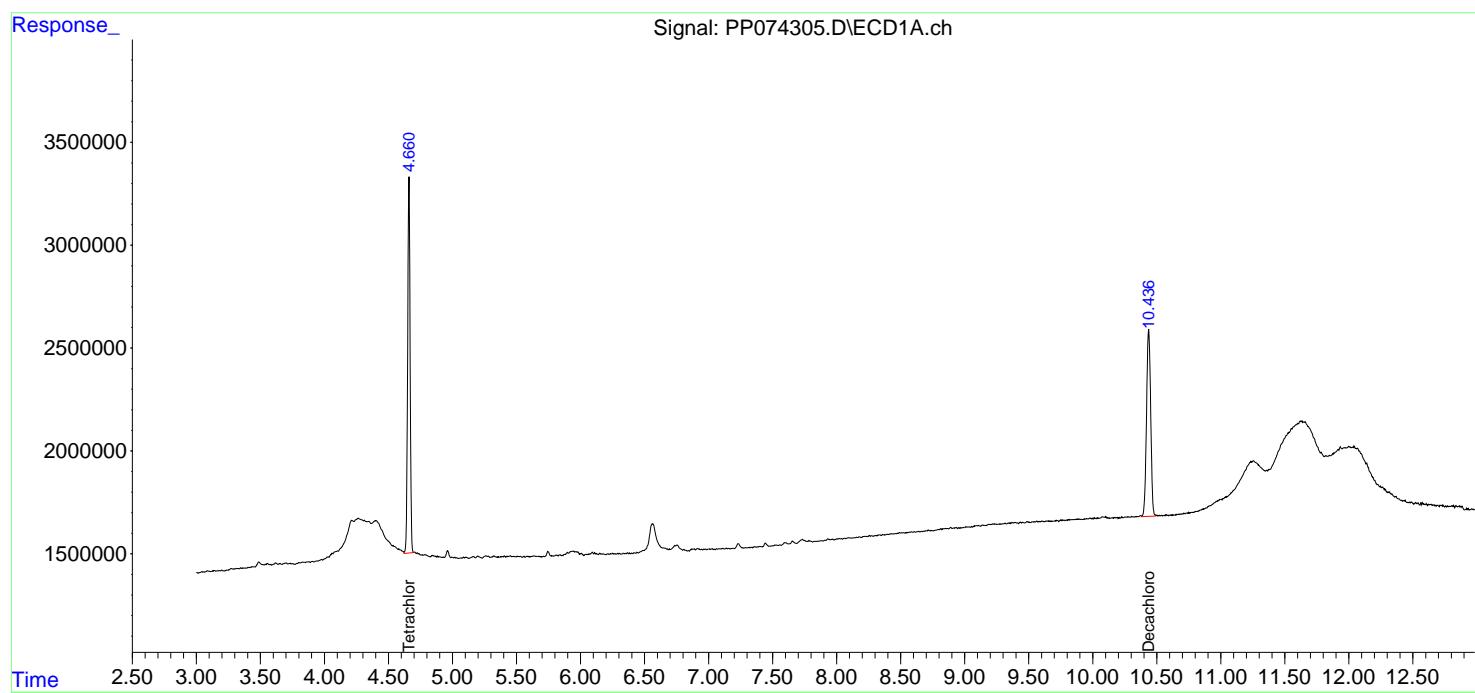

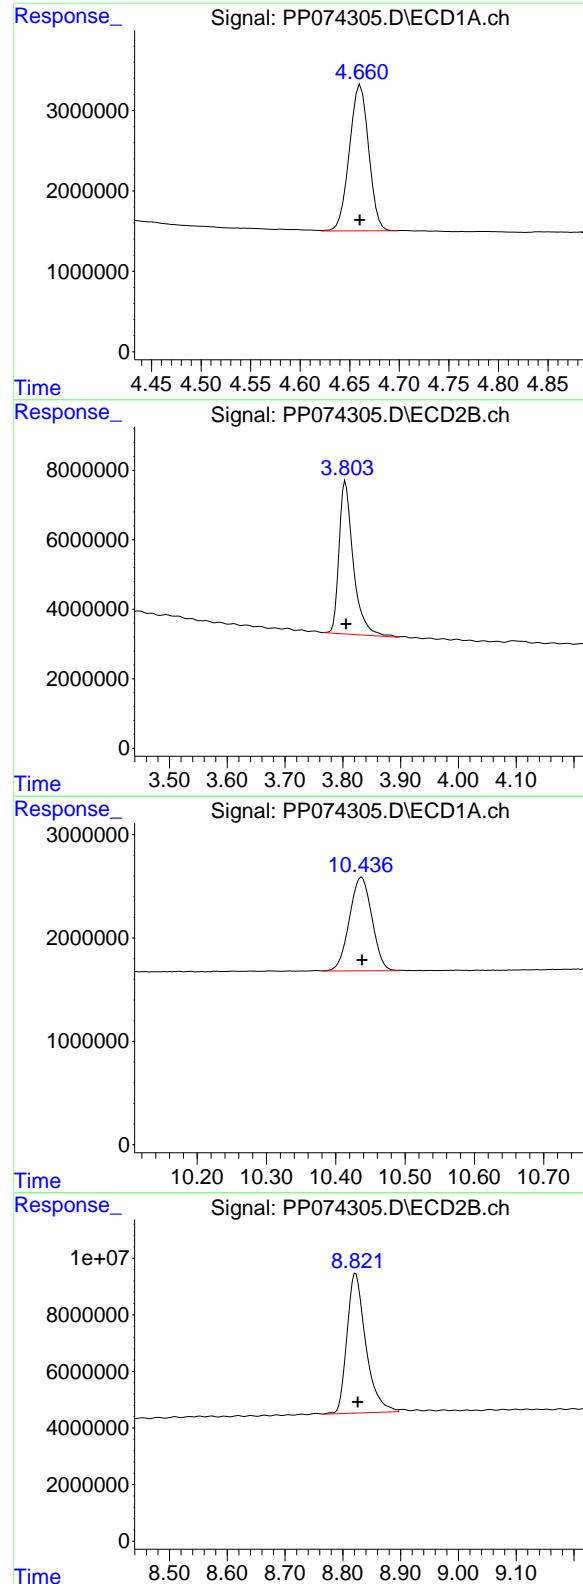

#1 Tetrachloro-m-xylene

R.T.: 4.661 min
 Delta R.T.: 0.000 min
 Response: 24597780
 Conc: 22.00 ng/ml

Instrument: ECD_P

ClientSampleId: I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.805 min
 Delta R.T.: 0.000 min
 Response: 75474847
 Conc: 19.68 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.437 min
 Delta R.T.: 0.000 min
 Response: 20447388
 Conc: 21.05 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.822 min
 Delta R.T.: -0.004 min
 Response: 111481904
 Conc: 18.54 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | | | |
|--------------------|-------------------------|--------|----|--------------------|----------|-----------|--|--|
| Client: | First Environment, Inc. | | | Date Collected: | 08/12/25 | | | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/12/25 | | | |
| Client Sample ID: | PIBLK-PP074319.D | | | SDG No.: | Q2819 | | | |
| Lab Sample ID: | I.BLK-PP074319.D | | | Matrix: | WATER | | | |
| Analytical Method: | 8082A | | | % Solid: | 0 | Decanted: | | |
| Sample Wt/Vol: | 1000 | Units: | mL | Final Vol: | 10000 | uL | | |
| Soil Aliquot Vol: | uL | | | Test: | PCB | | | |
| Extraction Type: | | | | Injection Volume : | | | | |
| GPC Factor : | 1.0 | PH : | | | | | | |
| Prep Method : | 5030 | | | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|-----------|---------------|---------------|
| PP074319.D | 1 | | 08/12/25 | pp081225 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units |
|-------------------|----------------------|-------|-----------|----------|------|------------|---------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 0.25 | U | 0.097 | 0.25 | 0.50 | ug/L |
| 11104-28-2 | Aroclor-1221 | 0.40 | U | 0.13 | 0.40 | 0.50 | ug/L |
| 11141-16-5 | Aroclor-1232 | 0.25 | U | 0.096 | 0.25 | 0.50 | ug/L |
| 53469-21-9 | Aroclor-1242 | 0.25 | U | 0.12 | 0.25 | 0.50 | ug/L |
| 12672-29-6 | Aroclor-1248 | 0.25 | U | 0.071 | 0.25 | 0.50 | ug/L |
| 11097-69-1 | Aroclor-1254 | 0.25 | U | 0.094 | 0.25 | 0.50 | ug/L |
| 11096-82-5 | Aroclor-1260 | 0.25 | U | 0.081 | 0.25 | 0.50 | ug/L |
| 37324-23-5 | Aroclor-1262 | 0.40 | U | 0.14 | 0.40 | 0.50 | ug/L |
| 11100-14-4 | Aroclor-1268 | 0.25 | U | 0.11 | 0.25 | 0.50 | ug/L |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 19.8 | | 60 - 140 | | 99% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 19.8 | | 60 - 140 | | 99% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 16:53
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:54:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.800 | 25617664 | 75726237 | 22.908 | 19.749 |
| 2) SA Decachlor... | 10.433 | 8.818 | 21108609 | 119.3E6 | 21.735 | 19.843 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074319.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 16:53
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:54:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

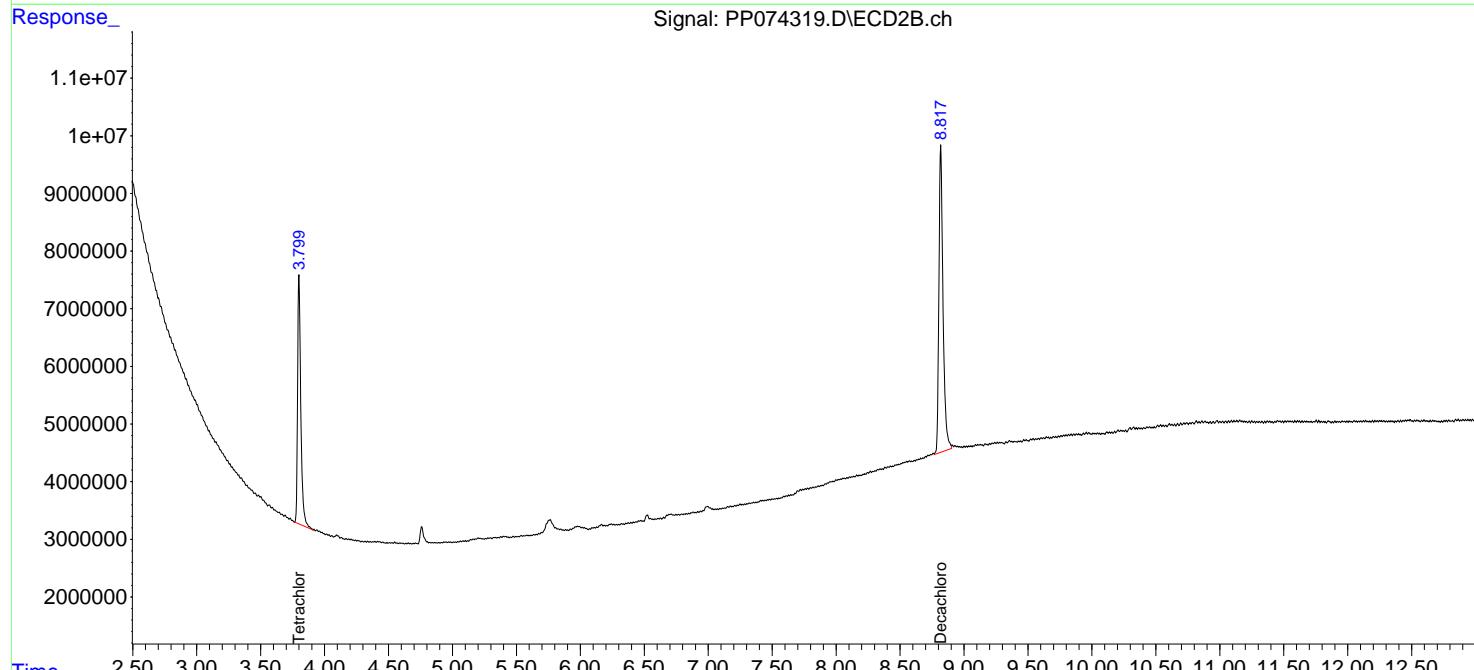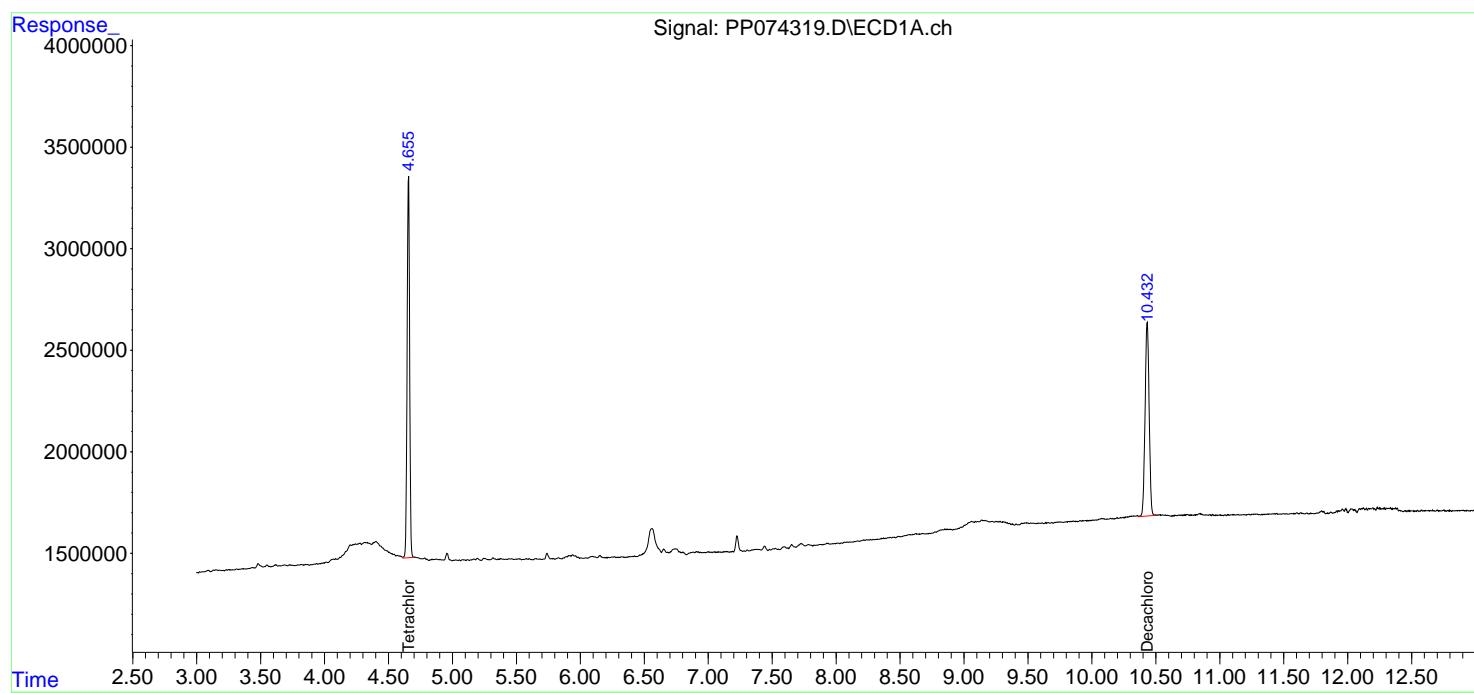

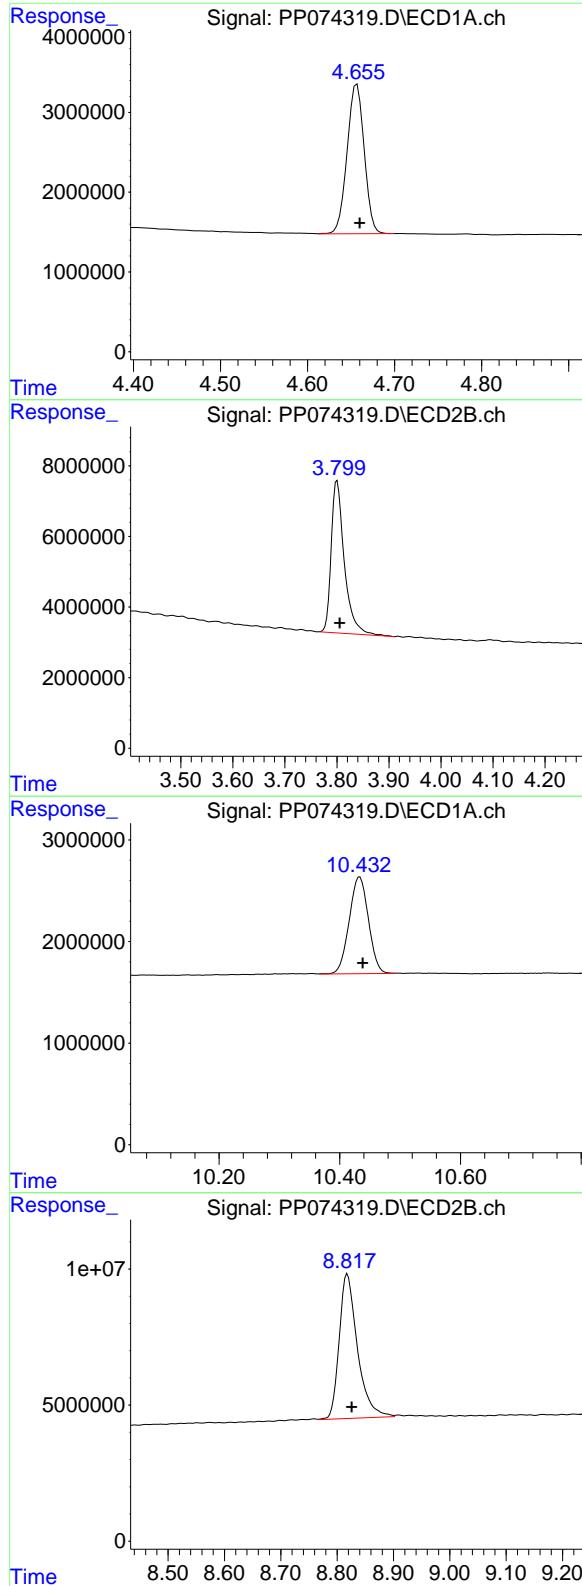

#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: -0.003 min
Response: 25617664
Conc: 22.91 ng/ml

Instrument : ECD_P

ClientSampleId : I.BLK

#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: -0.005 min
Response: 75726237
Conc: 19.75 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: -0.005 min
Response: 21108609
Conc: 21.74 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.818 min
Delta R.T.: -0.008 min
Response: 119328926
Conc: 19.84 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | |
|--------------------|-------------------------|--------|----|--------------------|---------------|
| Client: | First Environment, Inc. | | | Date Collected: | |
| Project: | USACE018-44 DOD | | | Date Received: | |
| Client Sample ID: | PB169205BS | | | SDG No.: | Q2819 |
| Lab Sample ID: | PB169205BS | | | Matrix: | SOIL |
| Analytical Method: | 8082A | | | % Solid: | 100 Decanted: |
| Sample Wt/Vol: | 30.01 | Units: | g | Final Vol: | 10000 uL |
| Soil Aliquot Vol: | | | uL | Test: | PCB |
| Extraction Type: | | | | Injection Volume : | |
| GPC Factor : | 1.0 | PH : | | | |
| Prep Method : | SW3541B | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PP074309.D | 1 | 08/12/25 08:15 | 08/12/25 13:05 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 185 | | 3.90 | 8.30 | 17.0 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 13.0 | U | 4.00 | 13.0 | 17.0 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 8.30 | U | 3.70 | 8.30 | 17.0 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 8.30 | U | 4.00 | 8.30 | 17.0 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 13.0 | U | 5.90 | 13.0 | 17.0 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 8.30 | U | 3.20 | 8.30 | 17.0 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 13.0 | U | 5.00 | 13.0 | 17.0 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 8.30 | U | 3.60 | 8.30 | 17.0 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 180 | | 3.20 | 8.30 | 17.0 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 24.3 | | 44 - 130 | | 121% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 22.5 | | 60 - 125 | | 112% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:05
 Operator : YP\AJ
 Sample : PB169205BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB169205BS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 13:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.801 | 27178701 | 79780335 | 24.303 | 20.806 |
| 2) SA Decachlor... | 10.438 | 8.821 | 21836747 | 120.3E6 | 22.485 | 20.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|---------|
| 3) L1 AR-1016-1 | 5.809 | 4.902 | 22669527 | 228.6E6 | 549.474 | 573.187 |
| 4) L1 AR-1016-2 | 5.830 | 4.959 | 34110297 | 104.5E6 | 561.563 | 556.666 |
| 5) L1 AR-1016-3 | 5.893 | 5.080 | 22276842 | 56001049 | 561.688 | 527.965 |
| 6) L1 AR-1016-4 | 5.990 | 5.121 | 18317589 | 56446484 | 562.848 | 516.814 |
| 7) L1 AR-1016-5 | 6.283 | 5.334 | 17574695 | 66942868 | 541.292 | 572.341 |
| 31) L7 AR-1260-1 | 7.401 | 6.551 | 31033148 | 236.1E6 | 550.662 | 584.486 |
| 32) L7 AR-1260-2 | 7.653 | 6.706 | 36070118 | 182.5E6 | 529.257 | 583.716 |
| 33) L7 AR-1260-3 | 8.012 | 6.915 | 24314378 | 204.9E6 | 456.215 | 519.977 |
| 34) L7 AR-1260-4 | 8.238 | 7.175 | 30953569 | 149.4E6 | 494.348m | 513.385 |
| 35) L7 AR-1260-5 | 8.566 | 7.415 | 51128845 | 382.8E6 | 451.250 | 505.423 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:05
 Operator : YP\AJ
 Sample : PB169205BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 13:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument :
 ECD_P
 ClientSampleId :
 PB169205BS

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

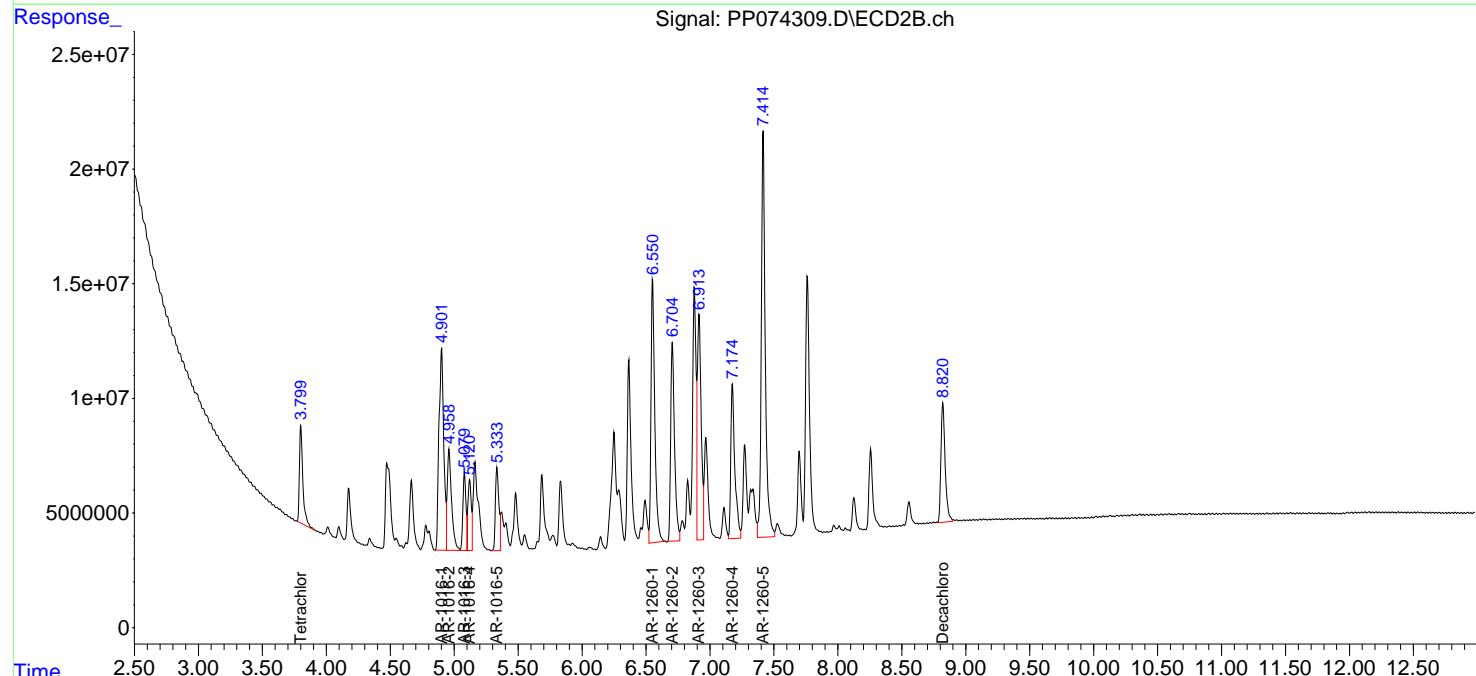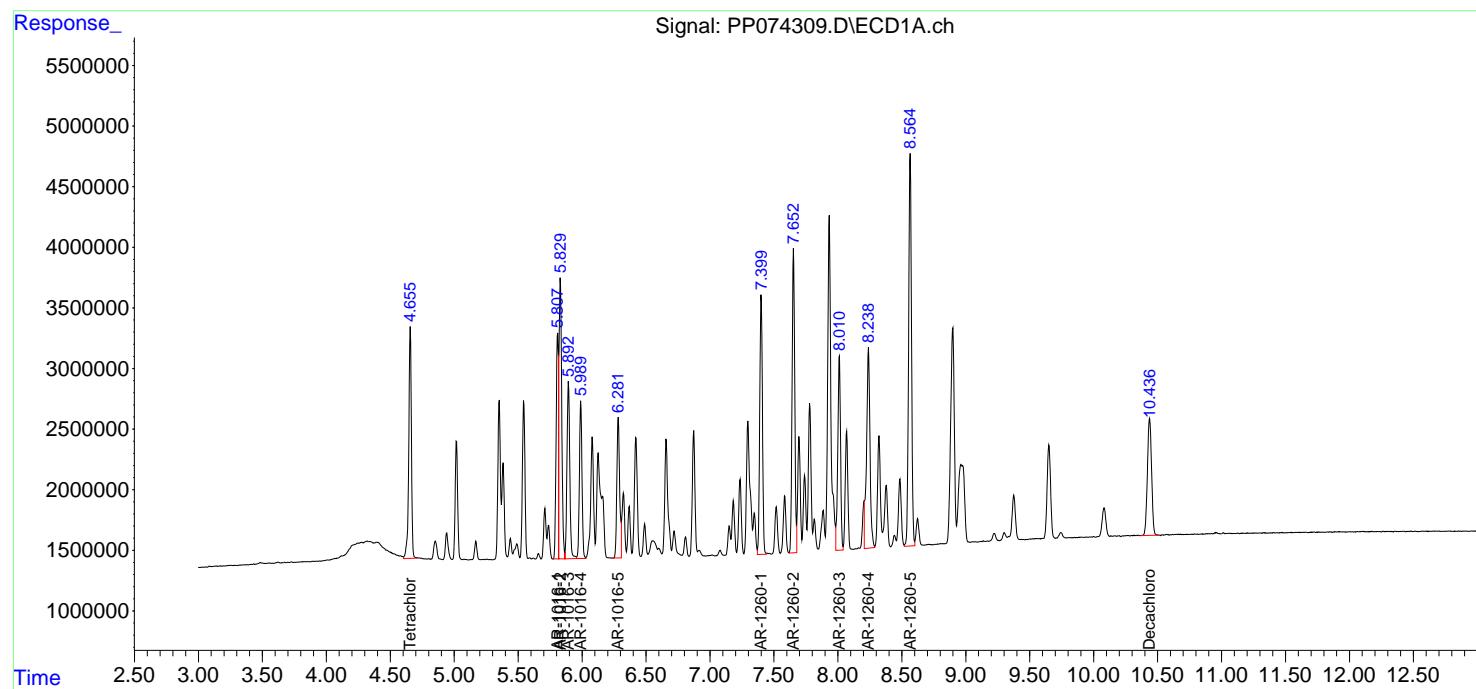

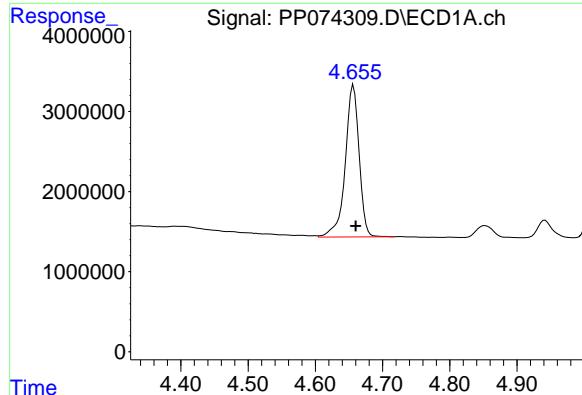


#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: -0.003 min
Response: 27178701
Conc: 24.30 ng/ml

Instrument : ECD_P
ClientSampleId : PB169205BS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

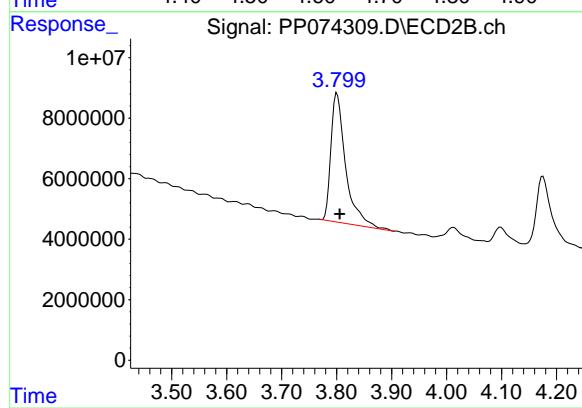


#1 Tetrachloro-m-xylene

R.T.: 3.801 min
Delta R.T.: -0.005 min
Response: 79780335
Conc: 20.81 ng/ml

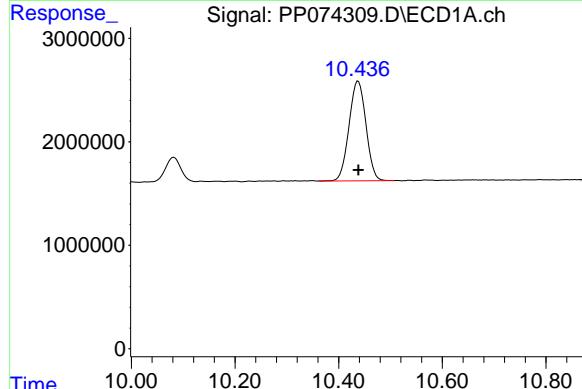


#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.000 min
Response: 21836747
Conc: 22.49 ng/ml

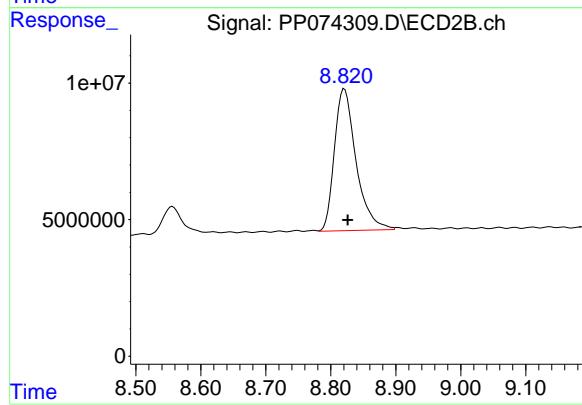

#2 Decachlorobiphenyl

R.T.: 8.821 min
Delta R.T.: -0.005 min
Response: 120271397
Conc: 20.00 ng/ml




#3 AR-1016-1

R.T.: 5.809 min
Delta R.T.: -0.003 min
Response: 22669527
Conc: 549.47 ng/ml

Instrument: ECD_P
ClientSampleId: PB169205BS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

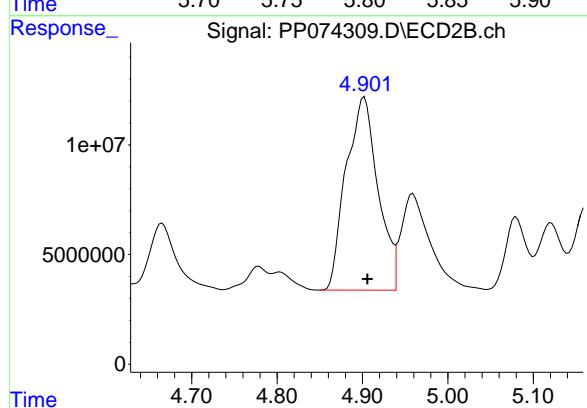


#3 AR-1016-1

R.T.: 4.902 min
Delta R.T.: -0.003 min
Response: 228636880
Conc: 573.19 ng/ml

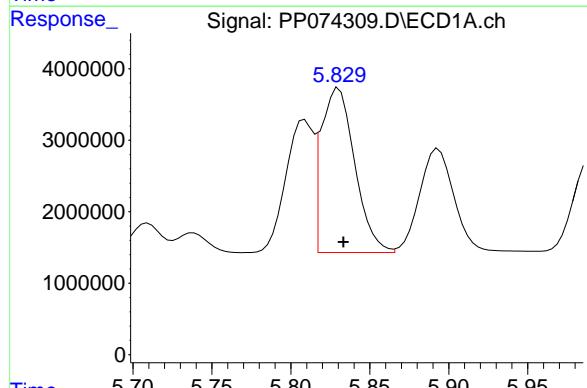


#4 AR-1016-2

R.T.: 5.830 min
Delta R.T.: -0.003 min
Response: 34110297
Conc: 561.56 ng/ml

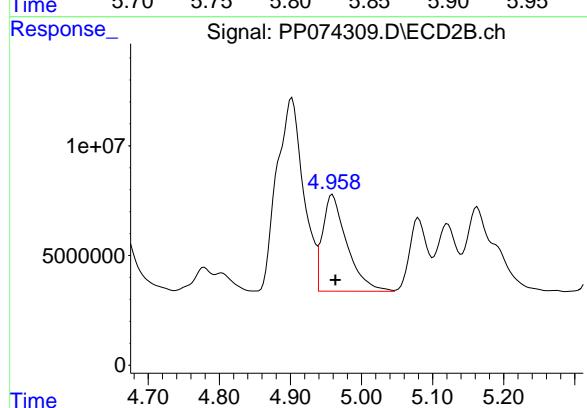

#4 AR-1016-2

R.T.: 4.959 min
Delta R.T.: -0.004 min
Response: 104546878
Conc: 556.67 ng/ml

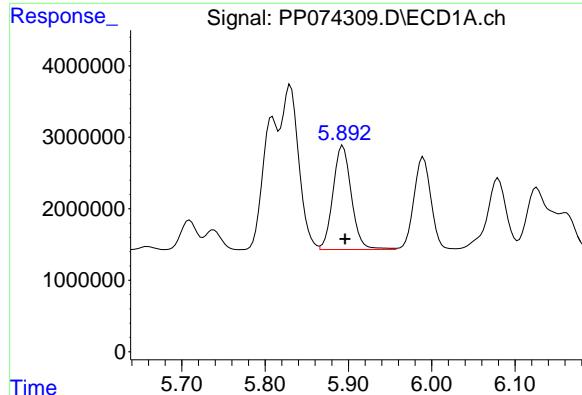


#5 AR-1016-3

R.T.: 5.893 min
Delta R.T.: -0.003 min
Response: 22276842
Conc: 561.69 ng/ml

Instrument: ECD_P
ClientSampleId: PB169205BS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

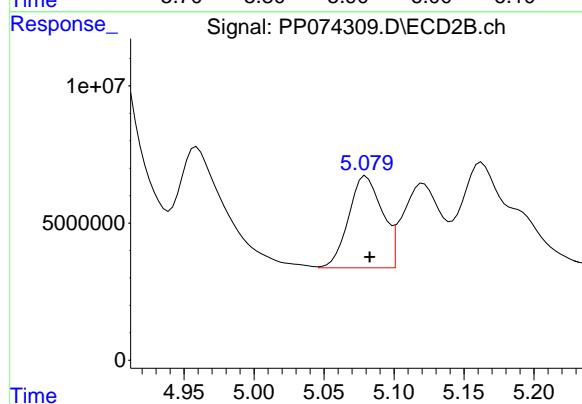


#5 AR-1016-3

R.T.: 5.080 min
Delta R.T.: -0.003 min
Response: 56001049
Conc: 527.96 ng/ml

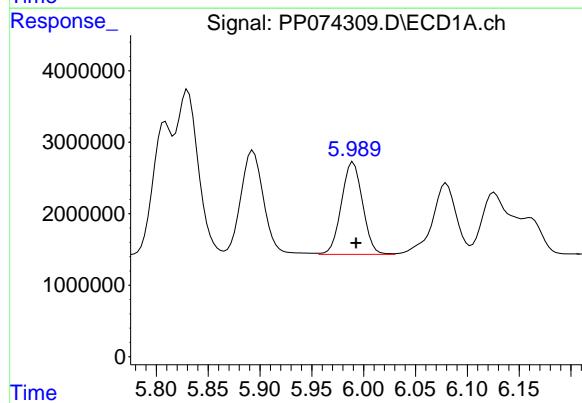


#6 AR-1016-4

R.T.: 5.990 min
Delta R.T.: -0.003 min
Response: 18317589
Conc: 562.85 ng/ml

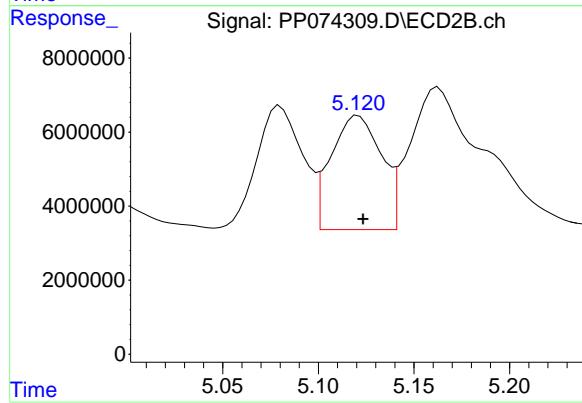

#6 AR-1016-4

R.T.: 5.121 min
Delta R.T.: -0.002 min
Response: 56446484
Conc: 516.81 ng/ml

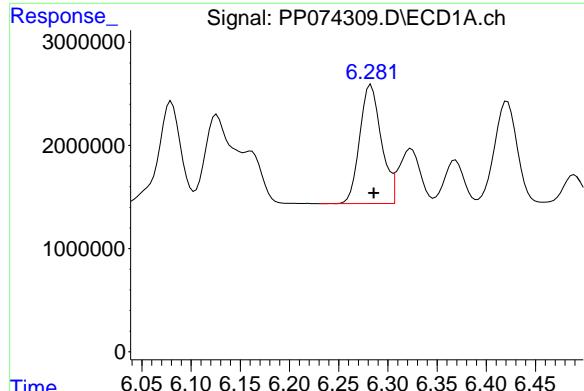


#7 AR-1016-5

R.T.: 6.283 min
 Delta R.T.: -0.003 min
 Response: 17574695
 Conc: 541.29 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

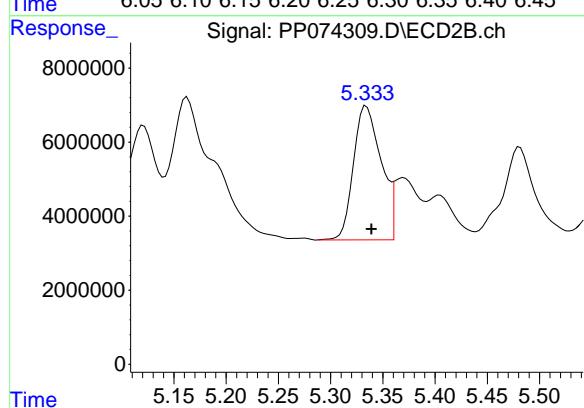


#7 AR-1016-5

R.T.: 5.334 min
 Delta R.T.: -0.005 min
 Response: 66942868
 Conc: 572.34 ng/ml

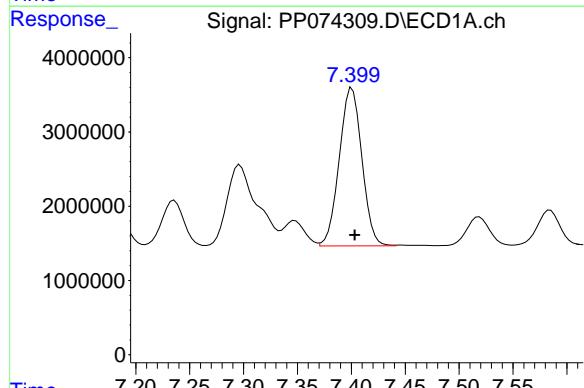



#31 AR-1260-1

R.T.: 7.401 min
 Delta R.T.: -0.002 min
 Response: 31033148
 Conc: 550.66 ng/ml

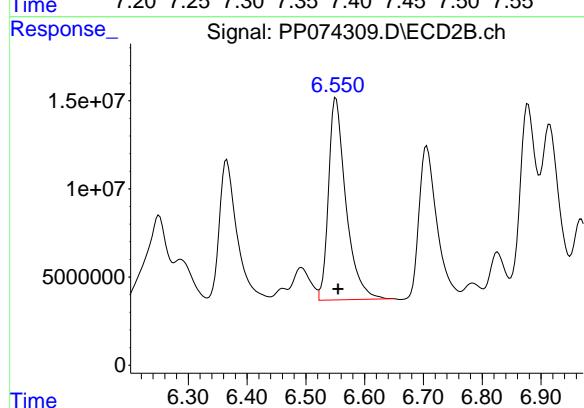

#31 AR-1260-1

R.T.: 6.551 min
 Delta R.T.: -0.004 min
 Response: 236107273
 Conc: 584.49 ng/ml

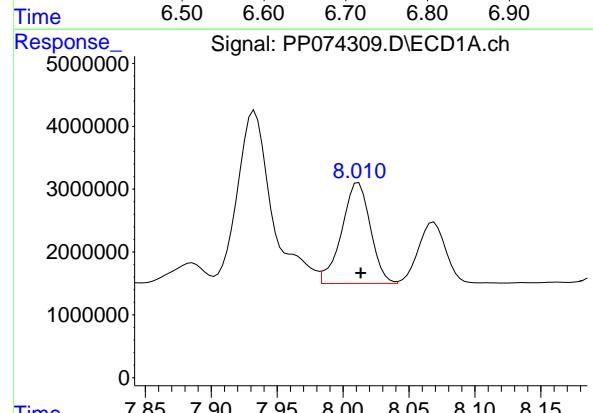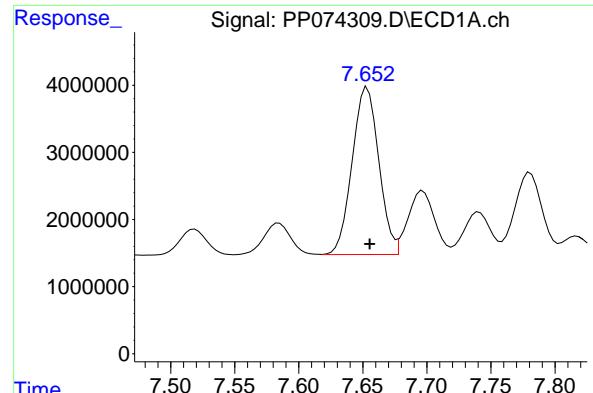

#32 AR-1260-2

R.T.: 7.653 min
 Delta R.T.: -0.002 min
 Response: 36070118
 Conc: 529.26 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#32 AR-1260-2


R.T.: 6.706 min
 Delta R.T.: -0.004 min
 Response: 182527346
 Conc: 583.72 ng/ml

#33 AR-1260-3

R.T.: 8.012 min
 Delta R.T.: -0.002 min
 Response: 24314378
 Conc: 456.21 ng/ml

#33 AR-1260-3

R.T.: 6.915 min
 Delta R.T.: -0.005 min
 Response: 204932581
 Conc: 519.98 ng/ml

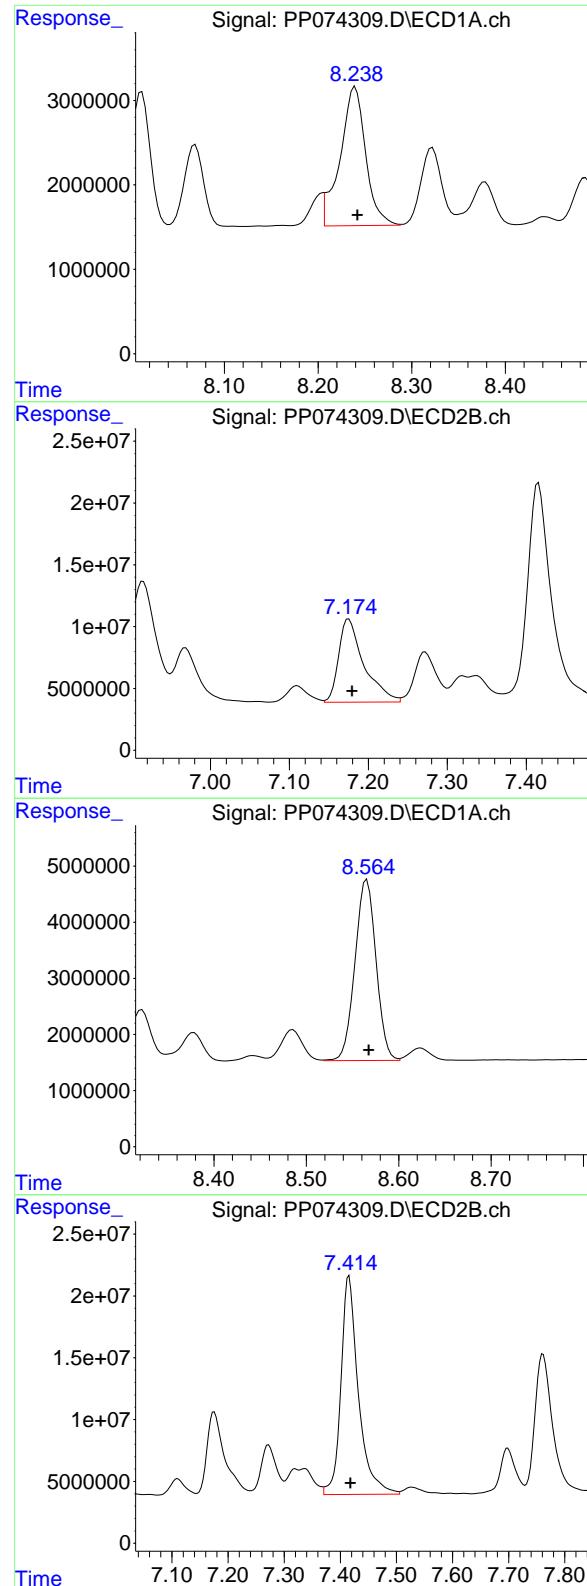

#34 AR-1260-4

R.T.: 8.238 min
 Delta R.T.: -0.004 min
 Response: 30953569
 Conc: 494.35 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

#34 AR-1260-4

R.T.: 7.175 min
 Delta R.T.: -0.004 min
 Response: 149384307
 Conc: 513.38 ng/ml

#35 AR-1260-5

R.T.: 8.566 min
 Delta R.T.: -0.002 min
 Response: 51128845
 Conc: 451.25 ng/ml

#35 AR-1260-5

R.T.: 7.415 min
 Delta R.T.: -0.003 min
 Response: 382812137
 Conc: 505.42 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | |
|--------------------|----------------------------------|--------|---|--------------------|----------|-----------|
| Client: | First Environment, Inc. | | | Date Collected: | 08/11/25 | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/11/25 | |
| Client Sample ID: | BIN0009-DRIVEWAY-TP-SOUTH-EASTMS | | | SDG No.: | Q2819 | |
| Lab Sample ID: | Q2830-01MS | | | Matrix: | SOIL | |
| Analytical Method: | 8082A | | | % Solid: | 86.9 | Decanted: |
| Sample Wt/Vol: | 30.01 | Units: | g | Final Vol: | 10000 | uL |
| Soil Aliquot Vol: | uL | | | Test: | PCB | |
| Extraction Type: | | | | Injection Volume : | | |
| GPC Factor : | 1.0 | PH : | | | | |
| Prep Method : | SW3541B | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PP074311.D | 1 | 08/12/25 08:15 | 08/12/25 13:37 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 213 | | 4.50 | 9.50 | 19.6 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 15.0 | U | 4.60 | 15.0 | 19.6 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 9.50 | U | 4.30 | 9.50 | 19.6 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 9.50 | U | 4.60 | 9.50 | 19.6 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 15.0 | U | 6.80 | 15.0 | 19.6 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 9.50 | U | 3.70 | 9.50 | 19.6 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 15.0 | U | 5.80 | 15.0 | 19.6 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 9.50 | U | 4.10 | 9.50 | 19.6 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 181 | | 3.70 | 9.50 | 19.6 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 23.5 | | 44 - 130 | | 117% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 19.9 | | 60 - 125 | | 100% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:37
 Operator : YP\AJ
 Sample : Q2830-01MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|---------|--------|
| 1) SA Tetrachlor... | 4.655 | 3.800 | 26250208 | 84433109 | 23.473m | 22.020 |
| 2) SA Decachlor... | 10.437 | 8.820 | 19335273 | 105.2E6 | 19.909 | 17.488 |

Target Compounds



| | | | | | | |
|------------------|-------|-------|----------|----------|----------|---------|
| 3) L1 AR-1016-1 | 5.809 | 4.901 | 21480557 | 221.4E6 | 520.655 | 555.093 |
| 4) L1 AR-1016-2 | 5.831 | 4.958 | 31794685 | 105.4E6 | 523.441 | 561.178 |
| 5) L1 AR-1016-3 | 5.894 | 5.079 | 20638950 | 60560553 | 520.390 | 570.951 |
| 6) L1 AR-1016-4 | 5.991 | 5.119 | 17736155 | 58694992 | 544.982 | 537.401 |
| 7) L1 AR-1016-5 | 6.283 | 5.334 | 16474757 | 64653966 | 507.414 | 552.772 |
| 31) L7 AR-1260-1 | 7.400 | 6.550 | 28140334 | 207.0E6 | 499.331 | 512.404 |
| 32) L7 AR-1260-2 | 7.653 | 6.704 | 32575808 | 157.6E6 | 477.985 | 503.902 |
| 33) L7 AR-1260-3 | 8.012 | 6.914 | 21771827 | 176.5E6 | 408.508 | 447.876 |
| 34) L7 AR-1260-4 | 8.238 | 7.175 | 29533684 | 132.7E6 | 471.671m | 455.876 |
| 35) L7 AR-1260-5 | 8.566 | 7.413 | 45863963 | 335.1E6 | 404.784 | 442.376 |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 13:37
Operator : YP\AJ
Sample : Q2830-01MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

```
Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 14:50:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title  : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation
```

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

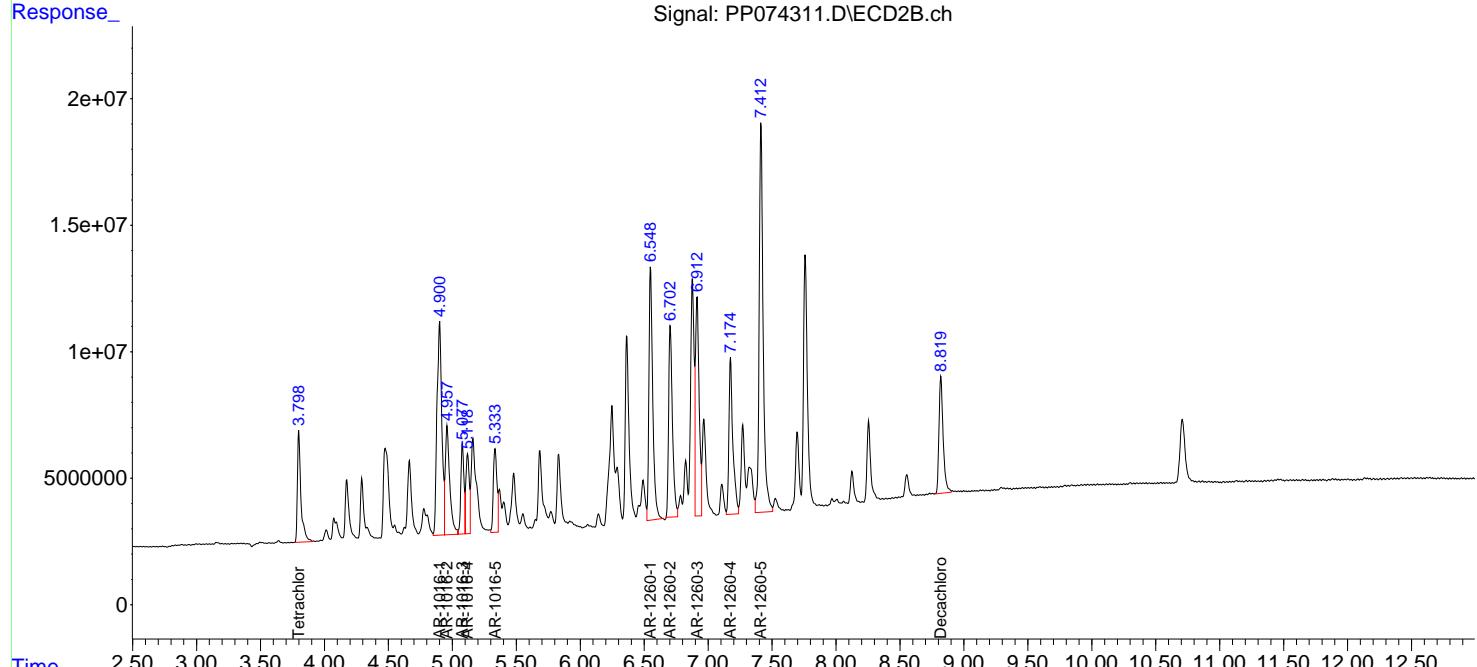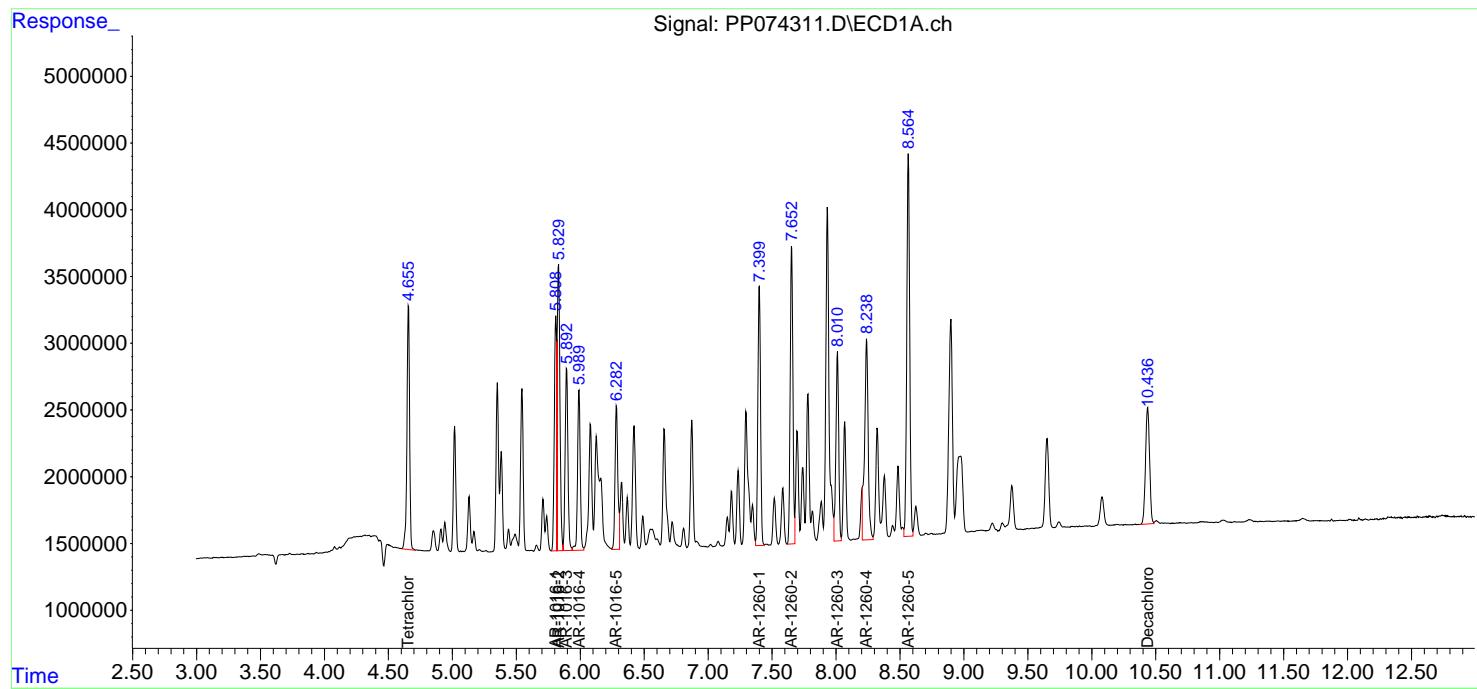

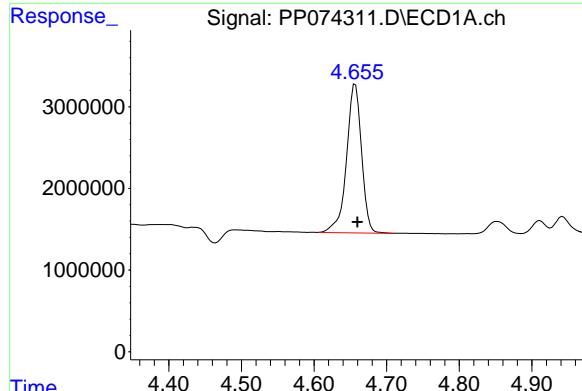


#1 Tetrachloro-m-xylene

R.T.: 4.655 min
Delta R.T.: -0.005 min
Response: 26250208
Conc: 23.47 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

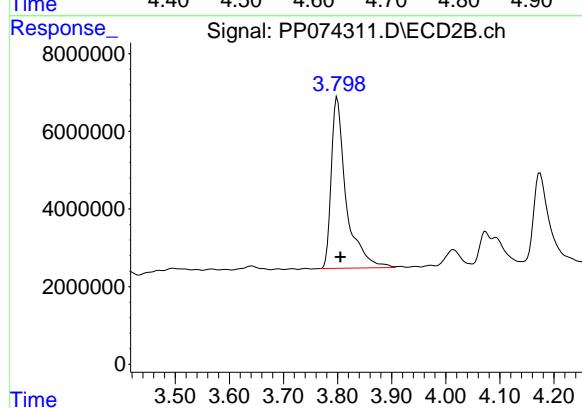


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: -0.006 min
Response: 84433109
Conc: 22.02 ng/ml

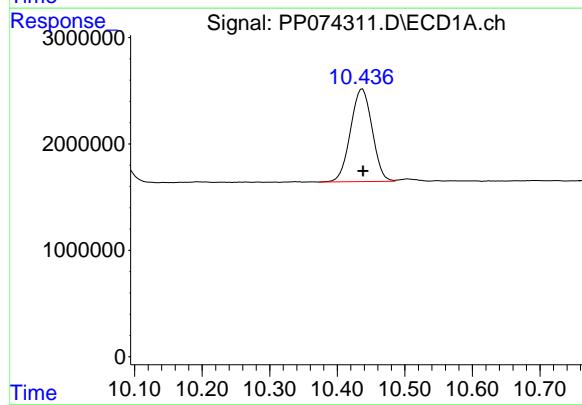


#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 19335273
Conc: 19.91 ng/ml

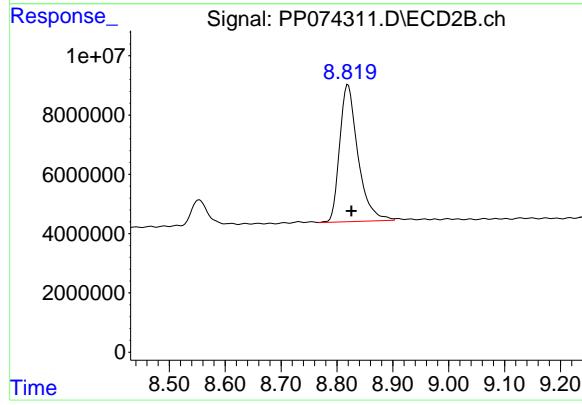

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 105164574
Conc: 17.49 ng/ml

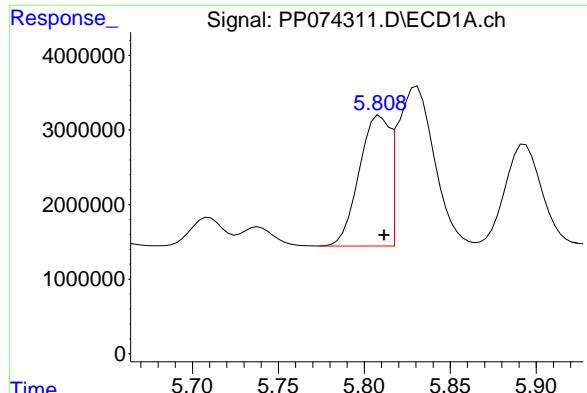


#3 AR-1016-1

R.T.: 5.809 min
Delta R.T.: -0.002 min
Response: 21480557
Conc: 520.65 ng/ml

Instrument: ECD_P
ClientSampleId: BIN009-DRIVEWAY-TP-SOUTH-EASTMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

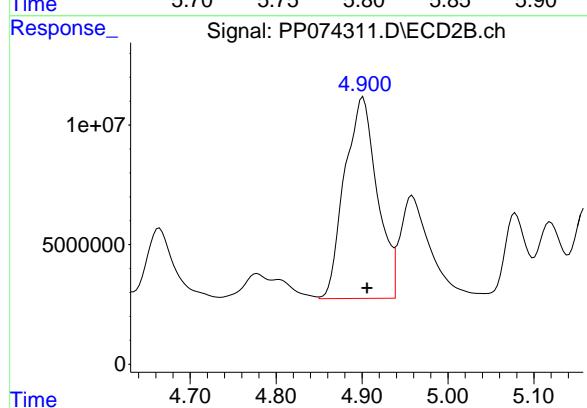


#3 AR-1016-1

R.T.: 4.901 min
Delta R.T.: -0.004 min
Response: 221419556
Conc: 555.09 ng/ml




#4 AR-1016-2

R.T.: 5.831 min
Delta R.T.: -0.003 min
Response: 31794685
Conc: 523.44 ng/ml

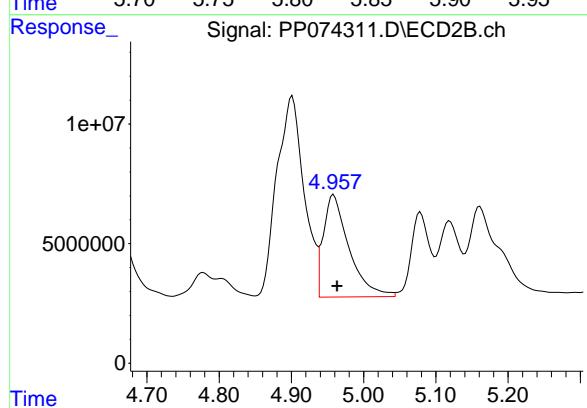

#4 AR-1016-2

R.T.: 4.958 min
Delta R.T.: -0.005 min
Response: 105394294
Conc: 561.18 ng/ml

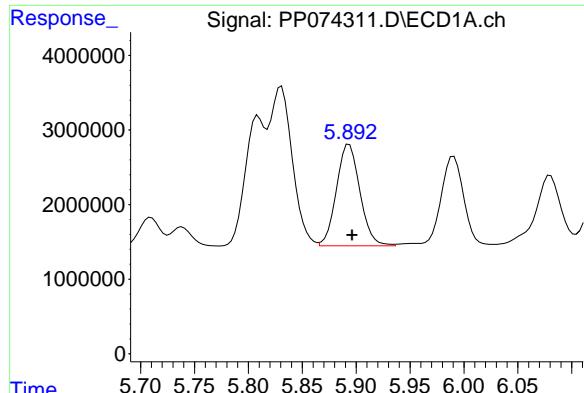


#5 AR-1016-3

R.T.: 5.894 min
Delta R.T.: -0.003 min
Response: 20638950
Conc: 520.39 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

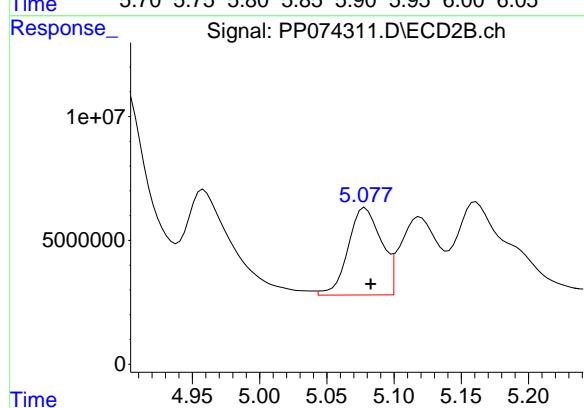


#5 AR-1016-3

R.T.: 5.079 min
Delta R.T.: -0.004 min
Response: 60560553
Conc: 570.95 ng/ml

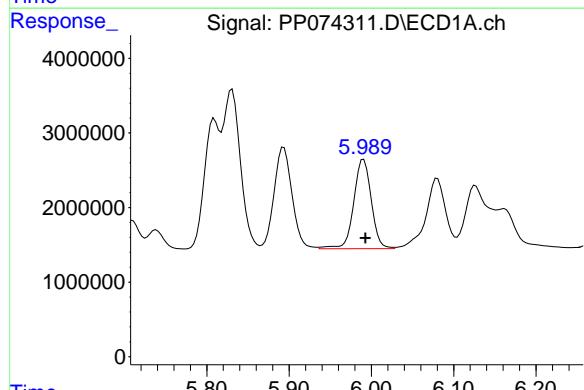


#6 AR-1016-4

R.T.: 5.991 min
Delta R.T.: -0.002 min
Response: 17736155
Conc: 544.98 ng/ml

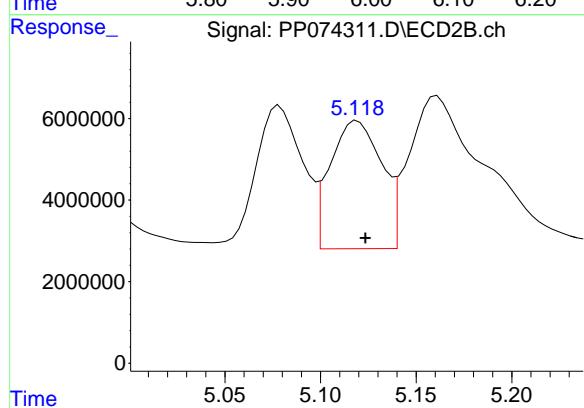

#6 AR-1016-4

R.T.: 5.119 min
Delta R.T.: -0.004 min
Response: 58694992
Conc: 537.40 ng/ml

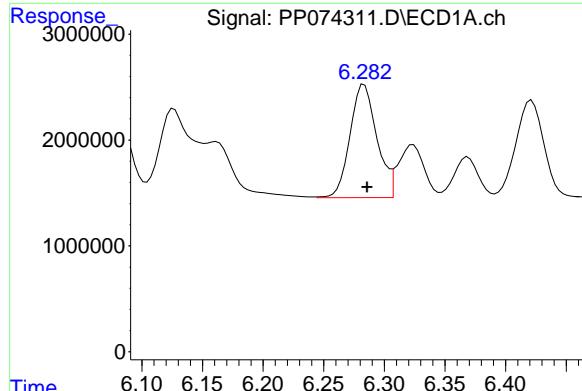


#7 AR-1016-5

R.T.: 6.283 min
Delta R.T.: -0.002 min
Response: 16474757
Conc: 507.41 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

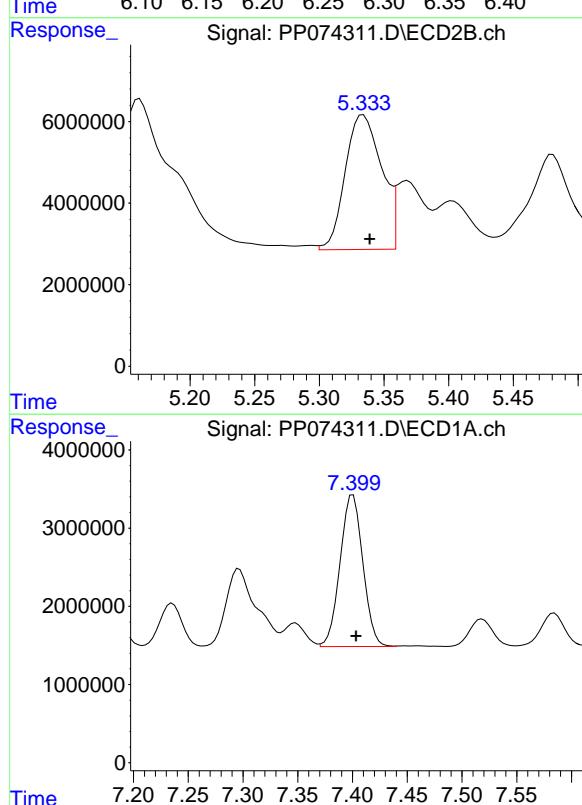

#7 AR-1016-5


R.T.: 5.334 min
Delta R.T.: -0.005 min
Response: 64653966
Conc: 552.77 ng/ml

#31 AR-1260-1

R.T.: 7.400 min
Delta R.T.: -0.003 min
Response: 28140334
Conc: 499.33 ng/ml

#31 AR-1260-1

R.T.: 6.550 min
Delta R.T.: -0.005 min
Response: 206989419
Conc: 512.40 ng/ml

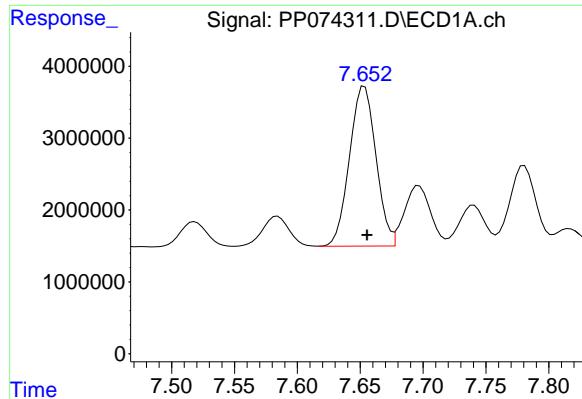


#32 AR-1260-2

R.T.: 7.653 min
Delta R.T.: -0.002 min
Response: 32575808
Conc: 477.98 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

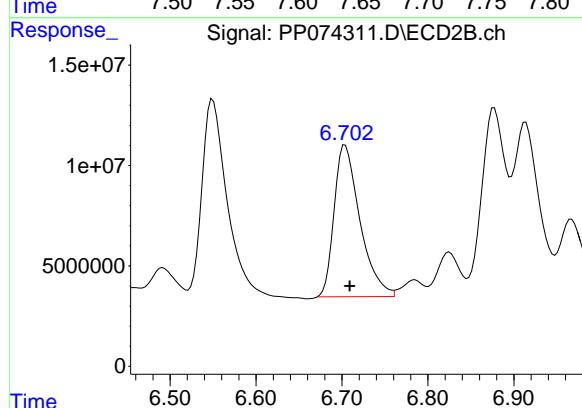


#32 AR-1260-2

R.T.: 6.704 min
Delta R.T.: -0.005 min
Response: 157569693
Conc: 503.90 ng/ml

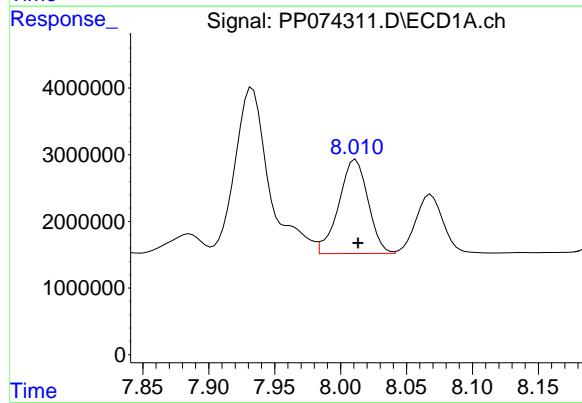





#33 AR-1260-3

R.T.: 8.012 min
Delta R.T.: -0.002 min
Response: 21771827
Conc: 408.51 ng/ml

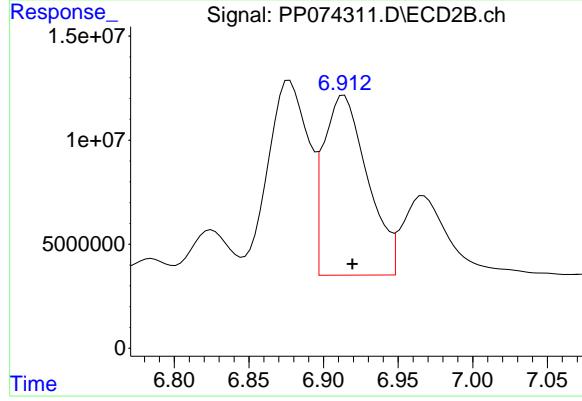

#33 AR-1260-3

R.T.: 6.914 min
Delta R.T.: -0.006 min
Response: 176516117
Conc: 447.88 ng/ml

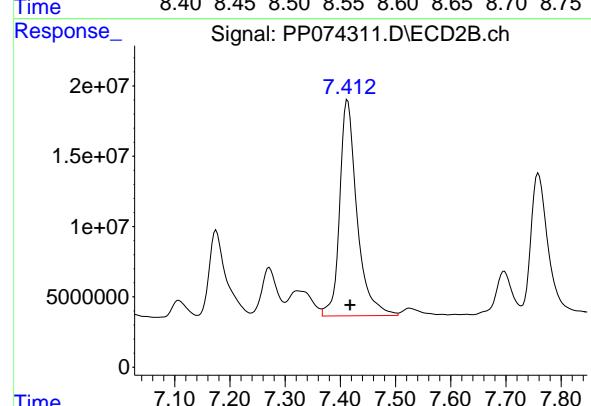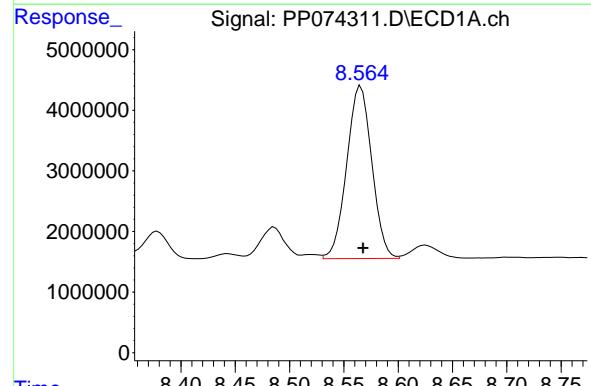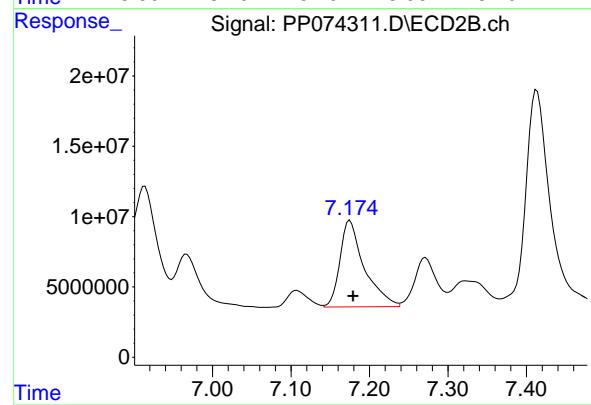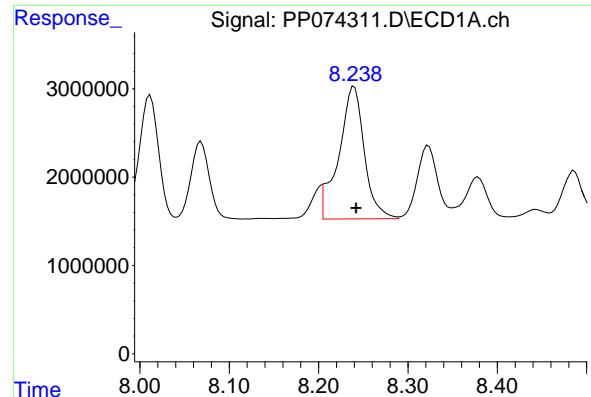





#34 AR-1260-4

R.T.: 8.238 min
 Delta R.T.: -0.003 min
 Response: 29533684
 Conc: 471.67 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

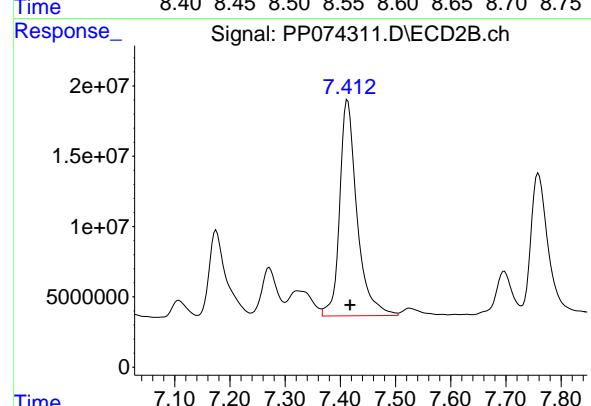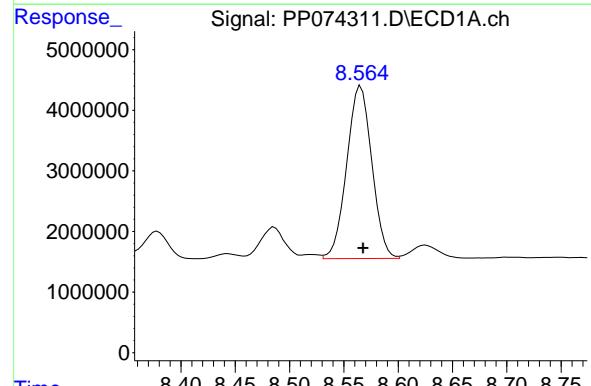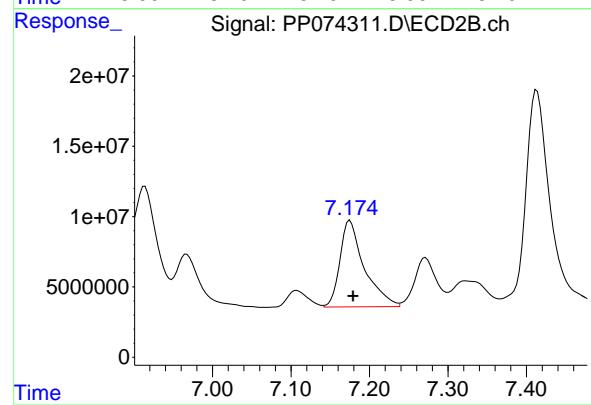

#34 AR-1260-4

R.T.: 7.175 min
 Delta R.T.: -0.004 min
 Response: 132650496
 Conc: 455.88 ng/ml

#35 AR-1260-5

R.T.: 8.566 min
 Delta R.T.: -0.002 min
 Response: 45863963
 Conc: 404.78 ng/ml

#35 AR-1260-5

R.T.: 7.413 min
 Delta R.T.: -0.005 min
 Response: 335060197
 Conc: 442.38 ng/ml



284 Sheffield Street, Mountainside, New Jersey 07092, Phone : 908 789 8900,
Fax : 908 789 8922

Report of Analysis

| | | | | | | |
|--------------------|-----------------------------------|--------|---|--------------------|----------|-----------|
| Client: | First Environment, Inc. | | | Date Collected: | 08/11/25 | |
| Project: | USACE018-44 DOD | | | Date Received: | 08/11/25 | |
| Client Sample ID: | BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD | | | SDG No.: | Q2819 | |
| Lab Sample ID: | Q2830-01MSD | | | Matrix: | SOIL | |
| Analytical Method: | 8082A | | | % Solid: | 86.9 | Decanted: |
| Sample Wt/Vol: | 30.03 | Units: | g | Final Vol: | 10000 | uL |
| Soil Aliquot Vol: | uL | | | Test: | PCB | |
| Extraction Type: | | | | Injection Volume : | | |
| GPC Factor : | 1.0 | PH : | | | | |
| Prep Method : | SW3541B | | | | | |

| File ID/Qc Batch: | Dilution: | Prep Date | Date Analyzed | Prep Batch ID |
|-------------------|-----------|----------------|----------------|---------------|
| PP074312.D | 1 | 08/12/25 08:15 | 08/12/25 13:53 | PB169205 |

| CAS Number | Parameter | Conc. | Qualifier | MDL | LOD | LOQ / CRQL | Units(Dry Weight) |
|-------------------|----------------------|-------|-----------|----------|------|------------|-------------------|
| TARGETS | | | | | | | |
| 12674-11-2 | Aroclor-1016 | 219 | | 4.50 | 9.50 | 19.5 | ug/kg |
| 11104-28-2 | Aroclor-1221 | 14.9 | U | 4.60 | 14.9 | 19.5 | ug/kg |
| 11141-16-5 | Aroclor-1232 | 9.50 | U | 4.30 | 9.50 | 19.5 | ug/kg |
| 53469-21-9 | Aroclor-1242 | 9.50 | U | 4.60 | 9.50 | 19.5 | ug/kg |
| 12672-29-6 | Aroclor-1248 | 14.9 | U | 6.80 | 14.9 | 19.5 | ug/kg |
| 11097-69-1 | Aroclor-1254 | 9.50 | U | 3.70 | 9.50 | 19.5 | ug/kg |
| 37324-23-5 | Aroclor-1262 | 14.9 | U | 5.80 | 14.9 | 19.5 | ug/kg |
| 11100-14-4 | Aroclor-1268 | 9.50 | U | 4.10 | 9.50 | 19.5 | ug/kg |
| 11096-82-5 | Aroclor-1260 | 188 | | 3.70 | 9.50 | 19.5 | ug/kg |
| SURROGATES | | | | | | | |
| 877-09-8 | Tetrachloro-m-xylene | 23.3 | | 44 - 130 | | 116% | SPK: 20 |
| 2051-24-3 | Decachlorobiphenyl | 19.9 | | 60 - 125 | | 99% | SPK: 20 |

Comments:

U = Not Detected

LOQ = Limit of Quantitation

MDL = Method Detection Limit

LOD = Limit of Detection

E = Value Exceeds Calibration Range

P = Indicates >25% difference for detected concentrations between the two GC columns

Q = indicates LCS control criteria did not meet requirements

M = MS/MSD acceptance criteria did not meet requirements

J = Estimated Value

B = Analyte Found in Associated Method Blank

N = Presumptive Evidence of a Compound

* = Values outside of QC limits

D = Dilution

S = Indicates estimated value where valid five-point calibration was not performed prior to analyte detection in sample.

() = Laboratory InHouse Limit

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:53
 Operator : YP\AJ
 Sample : Q2830-01MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|---------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 26034862 | 84782674 | 23.281m | 22.111 |
| 2) SA Decachlor... | 10.435 | 8.820 | 19291425 | 107.3E6 | 19.864m | 17.849 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|---------|
| 3) L1 AR-1016-1 | 5.811 | 4.904 | 22025300 | 229.5E6 | 533.859 | 575.363 |
| 4) L1 AR-1016-2 | 5.832 | 4.961 | 31957321 | 109.0E6 | 526.118 | 580.403 |
| 5) L1 AR-1016-3 | 5.895 | 5.081 | 21162376 | 59483478 | 533.588 | 560.796 |
| 6) L1 AR-1016-4 | 5.992 | 5.122 | 21722805 | 62077143 | 667.481 | 568.368 |
| 7) L1 AR-1016-5 | 6.284 | 5.337 | 16835913 | 66799585 | 518.538 | 571.116 |
| 31) L7 AR-1260-1 | 7.402 | 6.552 | 28910383 | 216.7E6 | 512.995 | 536.408 |
| 32) L7 AR-1260-2 | 7.654 | 6.707 | 33152517 | 164.0E6 | 486.447 | 524.348 |
| 33) L7 AR-1260-3 | 8.012 | 6.916 | 22216794 | 183.6E6 | 416.857 | 465.809 |
| 34) L7 AR-1260-4 | 8.239 | 7.176 | 29914044 | 137.0E6 | 477.746m | 470.828 |
| 35) L7 AR-1260-5 | 8.565 | 7.415 | 47018435 | 347.3E6 | 414.973 | 458.490 |

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:53
 Operator : YP\AJ
 Sample : Q2830-01MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1



Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

Instrument : ECD_P
 ClientSampleId : BIN009-DRIVEWAY-TP-SOUTH-EASTMSD

Manual Integrations APPROVED

Reviewed By :Yogesh Patel 08/13/2025
 Supervised By :mohammad ahmed 08/14/2025

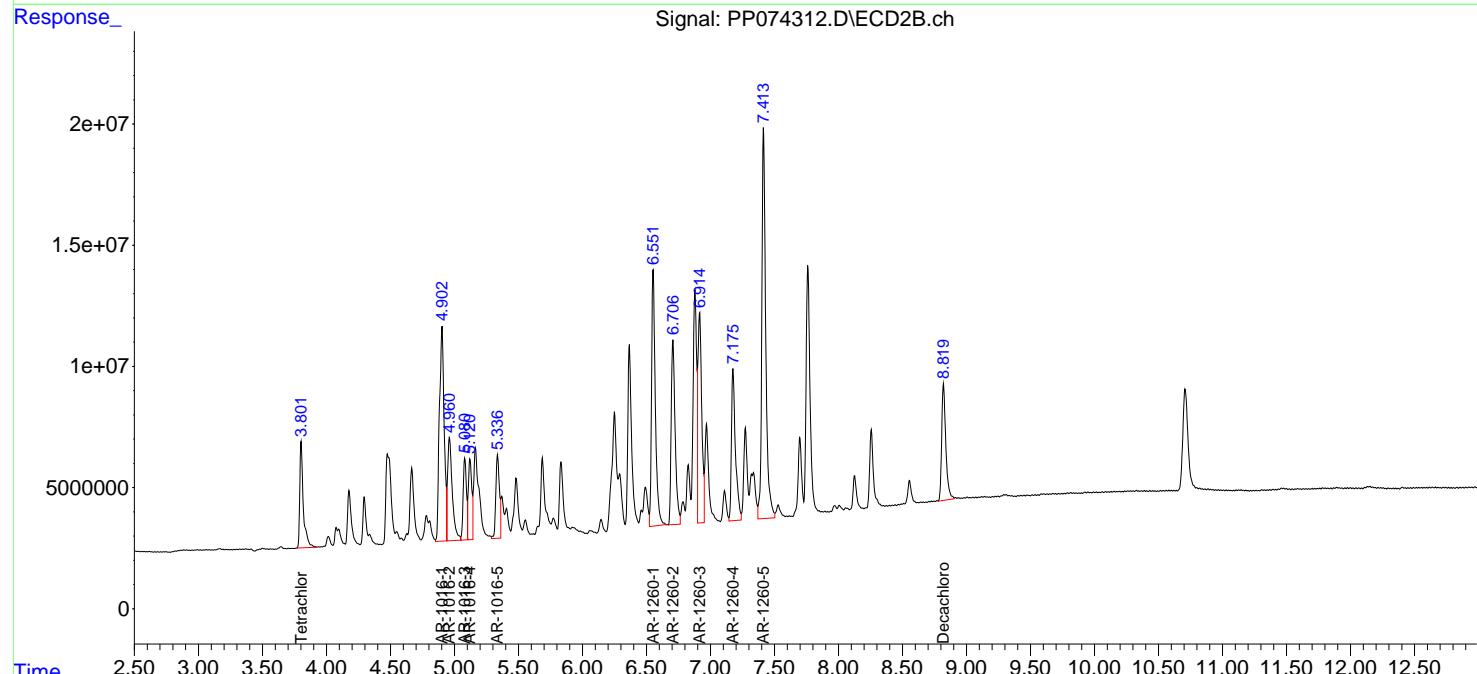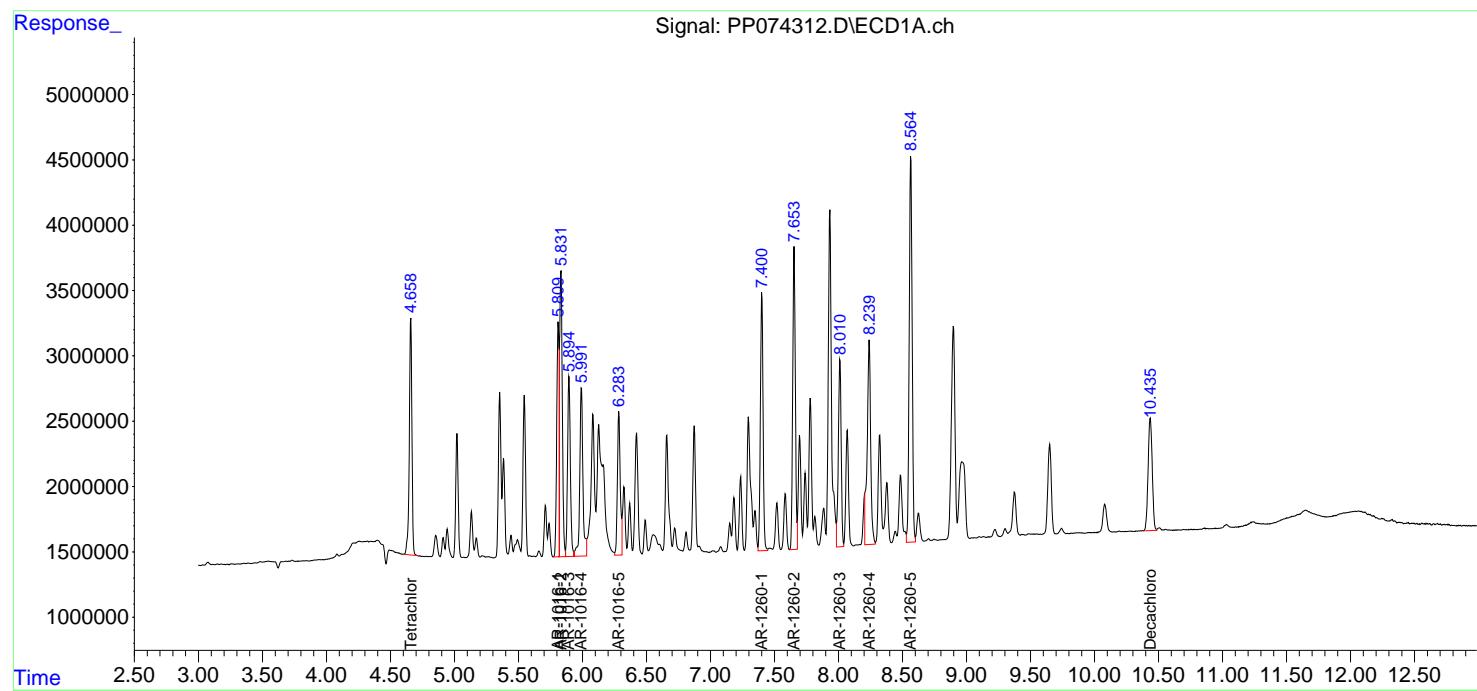

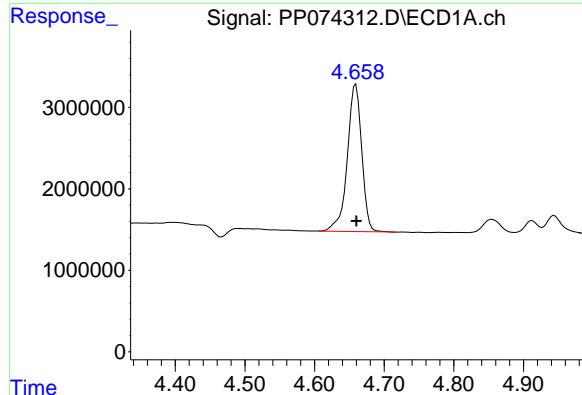


#1 Tetrachloro-m-xylene

R.T.: 4.658 min
Delta R.T.: -0.002 min
Response: 26034862
Conc: 23.28 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

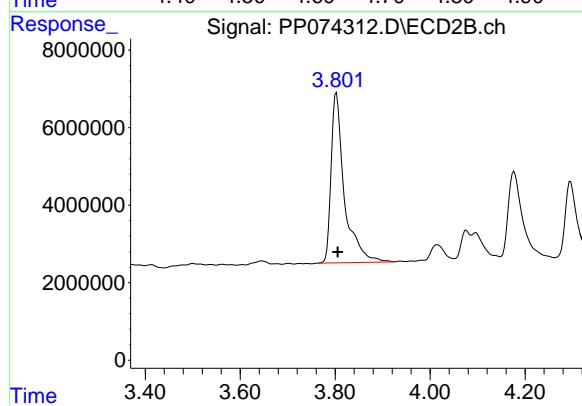


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: -0.003 min
Response: 84782674
Conc: 22.11 ng/ml

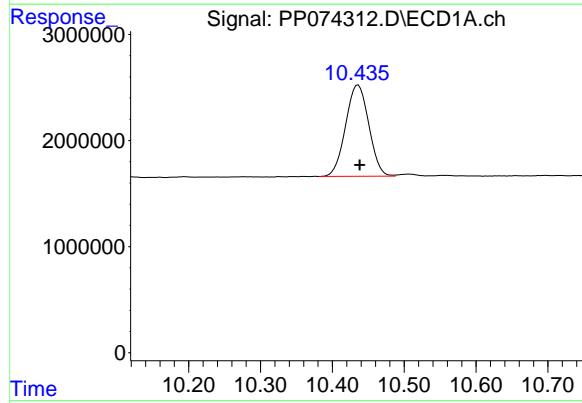


#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: -0.003 min
Response: 19291425
Conc: 19.86 ng/ml

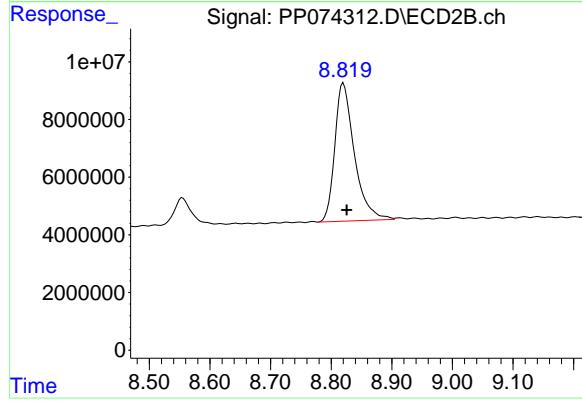

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 107334950
Conc: 17.85 ng/ml

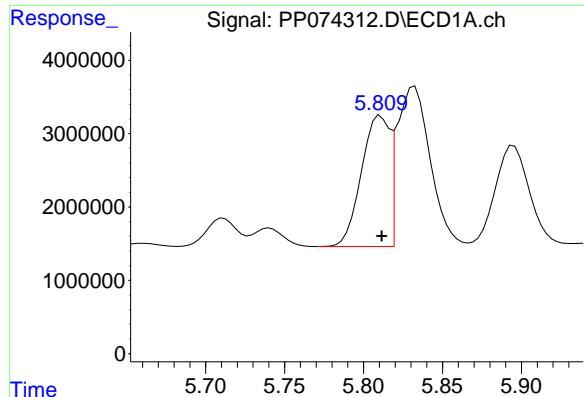


#3 AR-1016-1

R.T.: 5.811 min
Delta R.T.: 0.000 min
Response: 22025300
Conc: 533.86 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

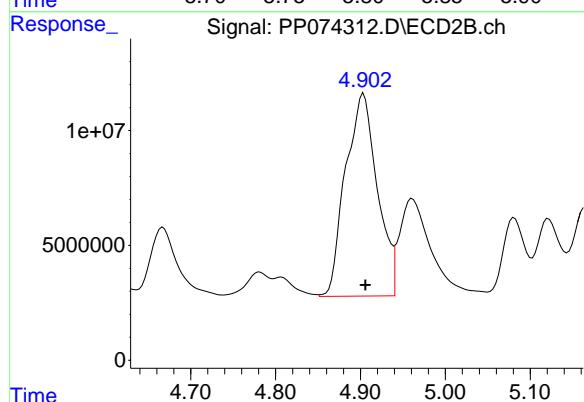


#3 AR-1016-1

R.T.: 4.904 min
Delta R.T.: -0.002 min
Response: 229504954
Conc: 575.36 ng/ml

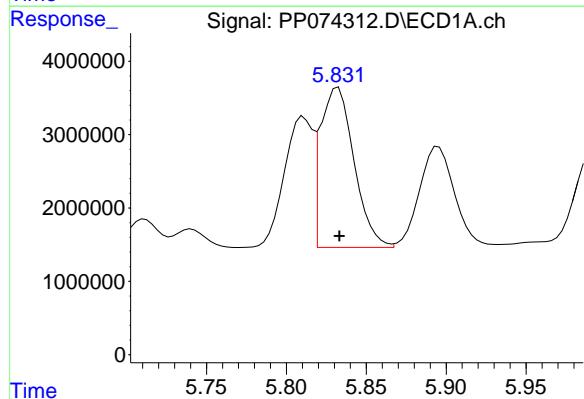


#4 AR-1016-2

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 31957321
Conc: 526.12 ng/ml

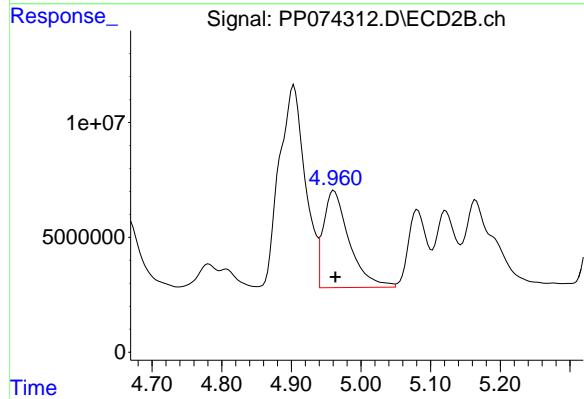

#4 AR-1016-2

R.T.: 4.961 min
Delta R.T.: -0.002 min
Response: 109004993
Conc: 580.40 ng/ml

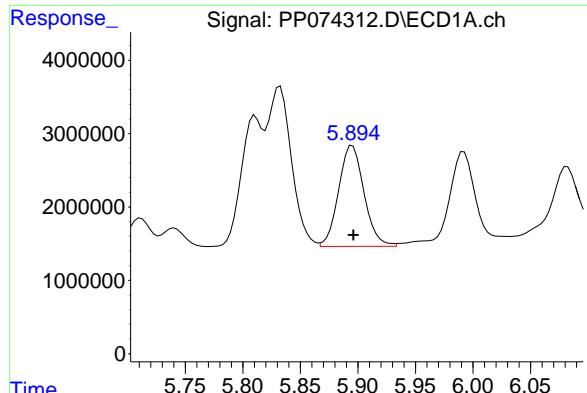


#5 AR-1016-3

R.T.: 5.895 min
Delta R.T.: 0.000 min
Response: 21162376
Conc: 533.59 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

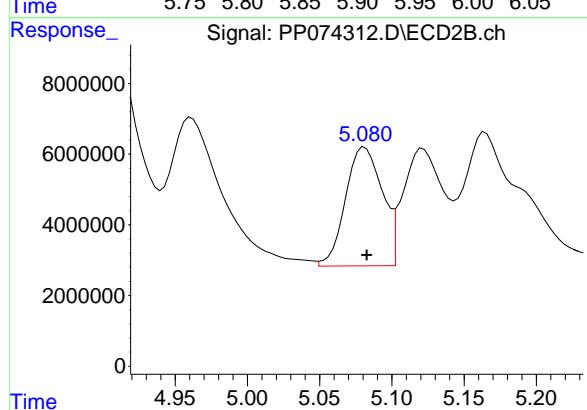


#5 AR-1016-3

R.T.: 5.081 min
Delta R.T.: -0.001 min
Response: 59483478
Conc: 560.80 ng/ml

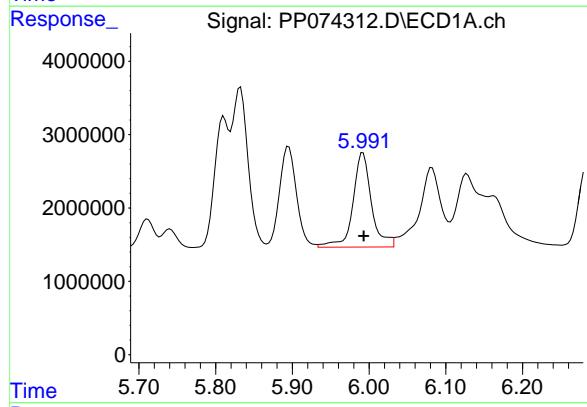


#6 AR-1016-4

R.T.: 5.992 min
Delta R.T.: 0.000 min
Response: 21722805
Conc: 667.48 ng/ml

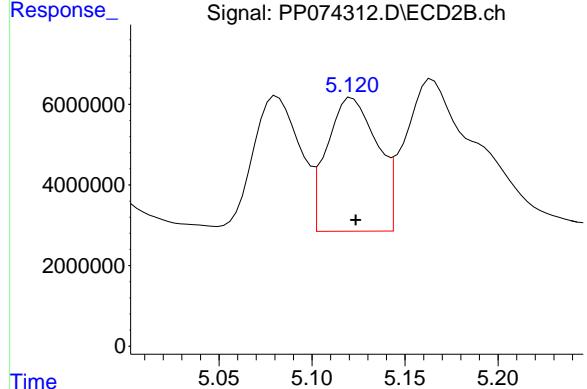

#6 AR-1016-4

R.T.: 5.122 min
Delta R.T.: -0.002 min
Response: 62077143
Conc: 568.37 ng/ml

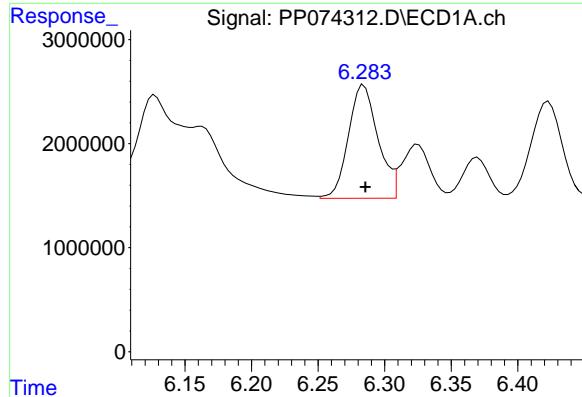


#7 AR-1016-5

R.T.: 6.284 min
Delta R.T.: -0.001 min
Response: 16835913
Conc: 518.54 ng/ml

Instrument: ECD_P
ClientSampleId: BIN009-DRIVEWAY-TP-SOUTH-EASTMSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

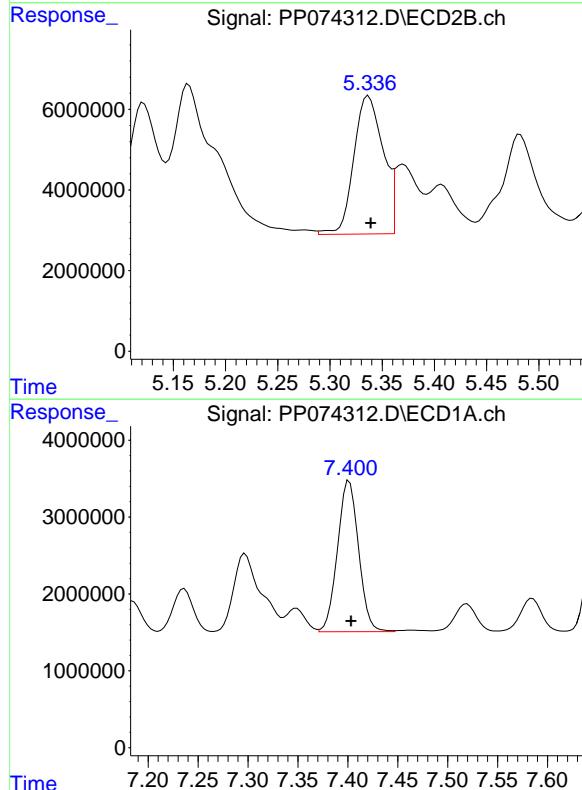

#7 AR-1016-5


R.T.: 5.337 min
Delta R.T.: -0.002 min
Response: 66799585
Conc: 571.12 ng/ml

#31 AR-1260-1

R.T.: 7.402 min
Delta R.T.: -0.002 min
Response: 28910383
Conc: 513.00 ng/ml

#31 AR-1260-1

R.T.: 6.552 min
Delta R.T.: -0.002 min
Response: 216685736
Conc: 536.41 ng/ml

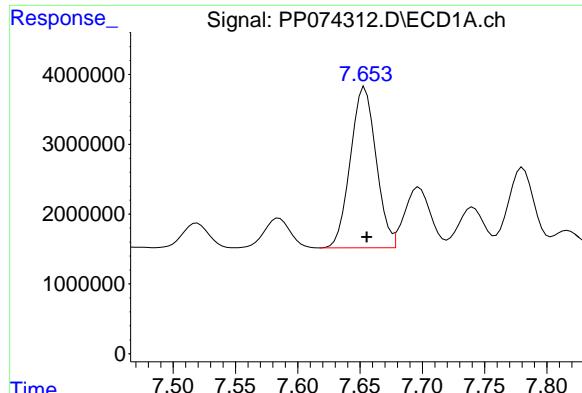


#32 AR-1260-2

R.T.: 7.654 min
Delta R.T.: -0.002 min
Response: 33152517
Conc: 486.45 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

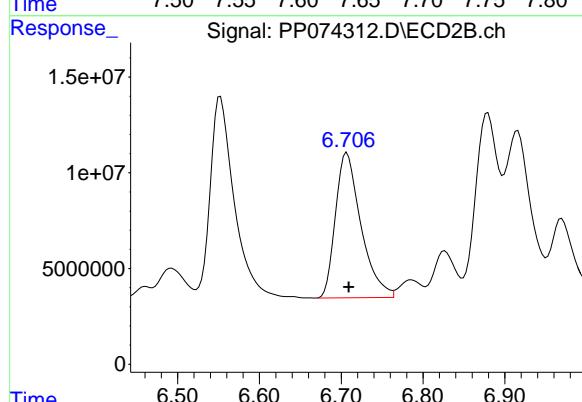


#32 AR-1260-2

R.T.: 6.707 min
Delta R.T.: -0.002 min
Response: 163962965
Conc: 524.35 ng/ml

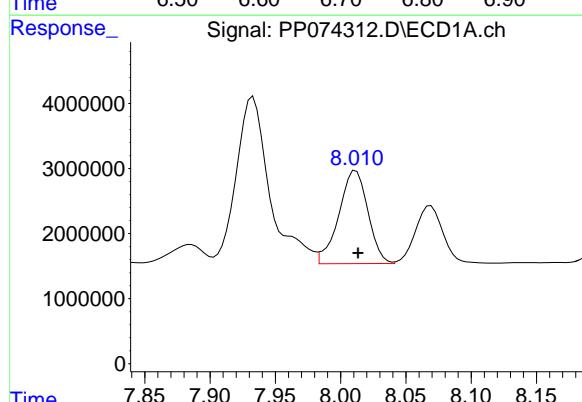





#33 AR-1260-3

R.T.: 8.012 min
Delta R.T.: -0.002 min
Response: 22216794
Conc: 416.86 ng/ml

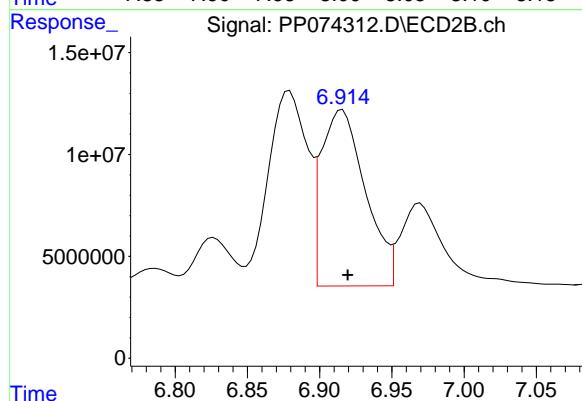

#33 AR-1260-3

R.T.: 6.916 min
Delta R.T.: -0.004 min
Response: 183583696
Conc: 465.81 ng/ml

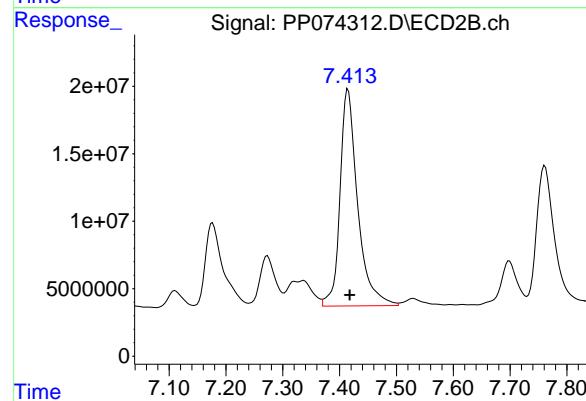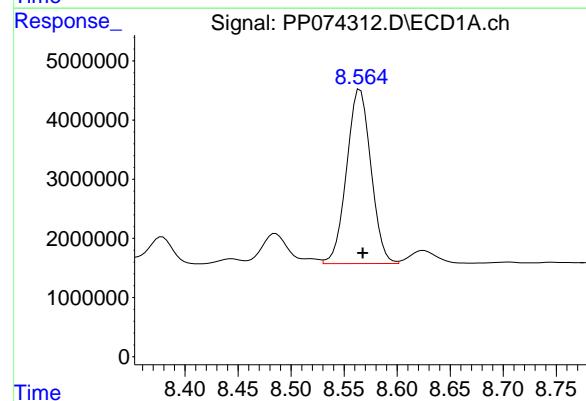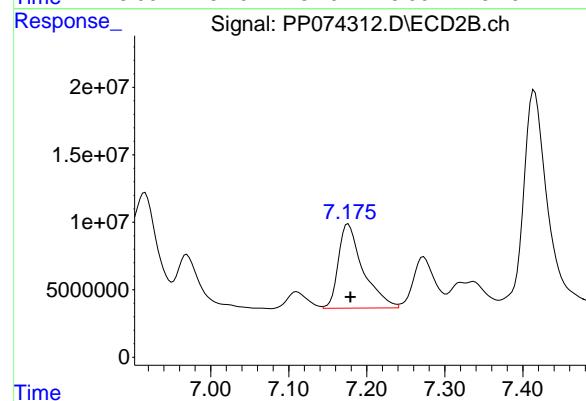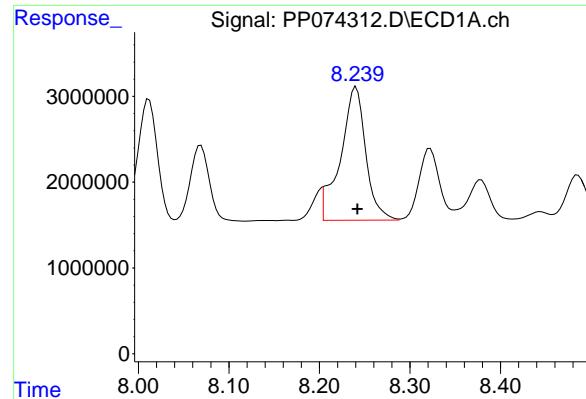





#34 AR-1260-4

R.T.: 8.239 min
Delta R.T.: -0.003 min
Response: 29914044
Conc: 477.75 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 08/13/2025
Supervised By :mohammad ahmed 08/14/2025

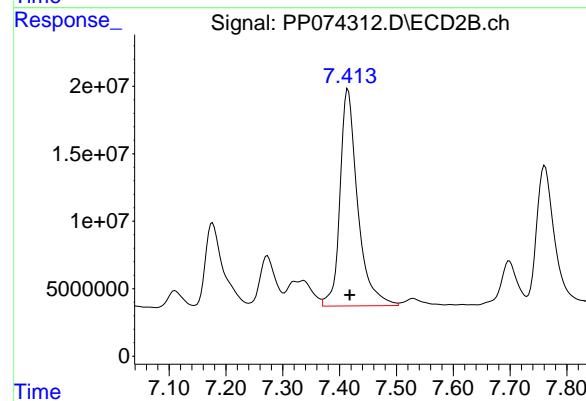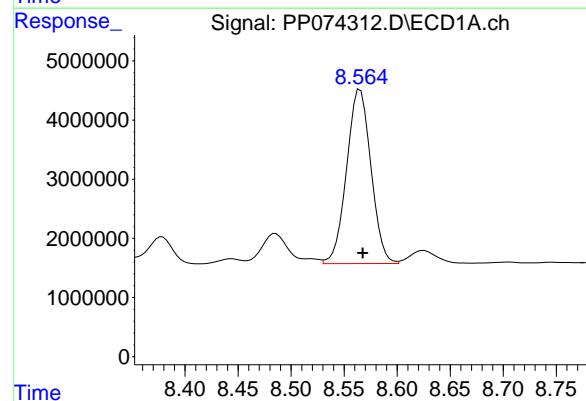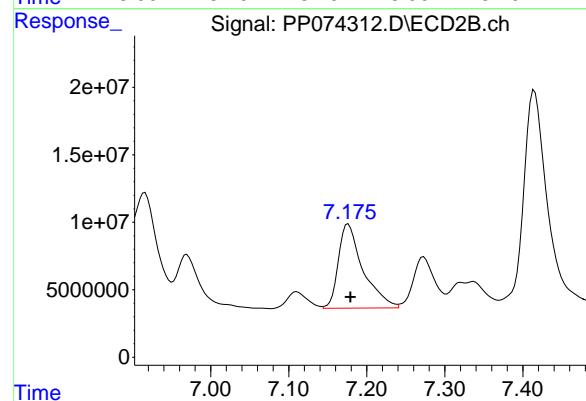

#34 AR-1260-4

R.T.: 7.176 min
Delta R.T.: -0.003 min
Response: 137001180
Conc: 470.83 ng/ml

#35 AR-1260-5

R.T.: 8.565 min
Delta R.T.: -0.002 min
Response: 47018435
Conc: 414.97 ng/ml

#35 AR-1260-5

R.T.: 7.415 min
Delta R.T.: -0.003 min
Response: 347264975
Conc: 458.49 ng/ml

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PO072325 | Instrument | ECD_o |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|-------------------------|-----------|----------------------|---------------|-------------------|-----------------------------|
| AR1660ICC250 | PO112417.D | AR-1260-1 | yogesh | 7/24/2025 7:42:50 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC250 | PO112417.D | AR-1260-1 #2 | yogesh | 7/24/2025 7:42:50 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC250 | PO112417.D | AR-1260-2 | yogesh | 7/24/2025 7:42:50 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC250 | PO112417.D | AR-1260-3 #2 | yogesh | 7/24/2025 7:42:50 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC050 | PO112418.D | AR-1016-5 | yogesh | 7/24/2025 7:42:52 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC050 | PO112418.D | AR-1016-5 #2 | yogesh | 7/24/2025 7:42:52 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC050 | PO112418.D | AR-1260-1 #2 | yogesh | 7/24/2025 7:42:52 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1660ICC050 | PO112418.D | AR-1260-3 #2 | yogesh | 7/24/2025 7:42:52 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1242ICC250 | PO112424.D | AR-1242-5 | yogesh | 7/24/2025 7:42:53 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1242ICC250 | PO112424.D | AR-1242-5 #2 | yogesh | 7/24/2025 7:42:53 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1242ICC050 | PO112425.D | AR-1242-5 | yogesh | 7/24/2025 7:42:55 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1242ICC050 | PO112425.D | AR-1242-5 #2 | yogesh | 7/24/2025 7:42:55 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1242ICC050 | PO112425.D | Tetrachloro-m-xylene #2 | yogesh | 7/24/2025 7:42:55 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PO072325 | Instrument | ECD_o |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|--------------|-----------|----------------------|---------------|-------------------|-----------------------------|
| AR1248ICC050 | PO112430.D | AR-1248-4 | yogesh | 7/24/2025 7:42:57 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1248ICC050 | PO112430.D | AR-1248-4 #2 | yogesh | 7/24/2025 7:42:57 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1248ICC050 | PO112430.D | AR-1248-5 | yogesh | 7/24/2025 7:42:57 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1248ICC050 | PO112430.D | AR-1248-5 #2 | yogesh | 7/24/2025 7:42:57 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1254ICC050 | PO112435.D | AR-1254-1 | yogesh | 7/24/2025 7:42:59 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1254ICC050 | PO112435.D | AR-1254-1 #2 | yogesh | 7/24/2025 7:42:59 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1254ICC050 | PO112435.D | AR-1254-2 | yogesh | 7/24/2025 7:42:59 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1254ICC050 | PO112435.D | AR-1254-2 #2 | yogesh | 7/24/2025 7:42:59 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |
| AR1254ICC050 | PO112435.D | AR-1254-3 #2 | yogesh | 7/24/2025 7:42:59 AM | mohammad | 7/25/2025 3:53:10 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PO081225 | Instrument | ECD_o |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|--------------|-----------|--------------------------|---------------|-------------------|-----------------------------|
| AR1660CCC500 | PO112850.D | AR-1016-1 | yogesh | 8/13/2025 11:49:43 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112850.D | AR-1016-2 | yogesh | 8/13/2025 11:49:43 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112850.D | AR-1016-3 #2 | yogesh | 8/13/2025 11:49:43 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112850.D | AR-1016-4 #2 | yogesh | 8/13/2025 11:49:43 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112850.D | AR-1260-3 #2 | yogesh | 8/13/2025 11:49:43 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112851.D | AR-1242-1 | yogesh | 8/13/2025 11:49:45 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112851.D | AR-1242-2 | yogesh | 8/13/2025 11:49:45 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112851.D | AR-1242-3 #2 | yogesh | 8/13/2025 11:49:45 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1248CCC500 | PO112852.D | AR-1248-1 | yogesh | 8/13/2025 11:49:47 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112865.D | AR-1016-1 | yogesh | 8/13/2025 11:49:48 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112865.D | AR-1016-2 | yogesh | 8/13/2025 11:49:48 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112865.D | AR-1260-3 #2 | yogesh | 8/13/2025 11:49:48 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112866.D | AR-1242-1 | yogesh | 8/13/2025 11:49:52 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PO081225 | Instrument | ECD_o |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|--------------|-----------|--------------------------|---------------|-------------------|-----------------------------|
| AR1242CCC500 | PO112866.D | AR-1242-2 | yogesh | 8/13/2025 11:49:52 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112866.D | AR-1242-3 #2 | yogesh | 8/13/2025 11:49:52 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112880.D | AR-1016-1 | yogesh | 8/13/2025 11:49:56 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112880.D | AR-1016-2 | yogesh | 8/13/2025 11:49:56 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112880.D | AR-1260-3 #2 | yogesh | 8/13/2025 11:49:56 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112881.D | AR-1242-1 | yogesh | 8/13/2025 11:49:58 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112881.D | AR-1242-2 | yogesh | 8/13/2025 11:49:58 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112890.D | AR-1016-1 | yogesh | 8/13/2025 11:50:01 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1660CCC500 | PO112890.D | AR-1016-2 | yogesh | 8/13/2025 11:50:01 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112891.D | AR-1242-1 | yogesh | 8/13/2025 11:50:03 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112891.D | AR-1242-2 | yogesh | 8/13/2025 11:50:03 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112891.D | AR-1242-3 #2 | yogesh | 8/13/2025 11:50:03 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1242CCC500 | PO112891.D | AR-1242-4 #2 | yogesh | 8/13/2025 11:50:03 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PO081225 | Instrument | ECD_o |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|-----------|-----------|----------------------|---------------|-------------------|-----------------------------|
| AR1254CCC500 | PO112893.D | AR-1254-1 | yogesh | 8/13/2025 7:36:58 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |
| AR1254CCC500 | PO112893.D | AR-1254-2 | yogesh | 8/13/2025 7:36:58 AM | mohammad | 8/14/2025 1:21:40 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PP080125 | Instrument | ECD_p |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|-------------------------|-----------|---------------------|---------------|------------------|-----------------------------|
| AR1660ICC250 | PP074171.D | AR-1016-5 | yogesh | 8/5/2025 7:23:21 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC250 | PP074171.D | AR-1260-1 | yogesh | 8/5/2025 7:23:21 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC250 | PP074171.D | AR-1260-2 | yogesh | 8/5/2025 7:23:21 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC050 | PP074172.D | AR-1260-2 | yogesh | 8/5/2025 7:22:19 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC050 | PP074172.D | AR-1260-2 #2 | yogesh | 8/5/2025 7:22:19 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC050 | PP074172.D | AR-1260-4 | yogesh | 8/5/2025 7:22:19 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC050 | PP074172.D | Tetrachloro-m-xylene | yogesh | 8/5/2025 7:22:19 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1660ICC050 | PP074172.D | Tetrachloro-m-xylene #2 | yogesh | 8/5/2025 7:22:19 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1232ICC500 | PP074174.D | AR-1232-4 #2 | yogesh | 8/5/2025 7:22:20 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC100 | PP074175.D | AR-1242-4 #2 | yogesh | 8/5/2025 7:22:22 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC750 | PP074176.D | AR-1242-4 #2 | yogesh | 8/5/2025 7:22:24 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC500 | PP074177.D | AR-1242-4 #2 | yogesh | 8/5/2025 7:22:27 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC250 | PP074178.D | AR-1242-4 #2 | yogesh | 8/5/2025 7:22:29 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PP080125 | Instrument | ECD_p |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|-------------------------|-----------|---------------------|---------------|------------------|-----------------------------|
| AR1242ICC250 | PP074178.D | AR-1242-5 | yogesh | 8/5/2025 7:22:29 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC050 | PP074179.D | AR-1242-5 | yogesh | 8/5/2025 7:22:32 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC050 | PP074179.D | Tetrachloro-m-xylene | yogesh | 8/5/2025 7:22:32 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICC050 | PP074179.D | Tetrachloro-m-xylene #2 | yogesh | 8/5/2025 7:22:32 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1248ICC500 | PP074182.D | AR-1248-3 #2 | yogesh | 8/5/2025 7:22:38 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1254ICC100 | PP074185.D | AR-1254-1 | yogesh | 8/5/2025 7:22:44 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1254ICC100 | PP074185.D | AR-1254-5 #2 | yogesh | 8/5/2025 7:22:44 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1254ICC750 | PP074186.D | AR-1254-1 | yogesh | 8/5/2025 7:22:45 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1254ICC500 | PP074187.D | AR-1254-1 | yogesh | 8/5/2025 7:22:47 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1254ICC250 | PP074188.D | AR-1254-1 | yogesh | 8/5/2025 7:22:49 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1254ICC050 | PP074189.D | AR-1254-1 | yogesh | 8/5/2025 7:22:51 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1242ICV500 | PP074197.D | AR-1242-4 #2 | yogesh | 8/5/2025 7:22:52 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |
| AR1248ICV500 | PP074198.D | AR-1248-3 #2 | yogesh | 8/5/2025 7:22:54 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PP080125 | Instrument | ECD_p |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|-----------|-----------|---------------------|---------------|------------------|-----------------------------|
| AR1254ICV500 | PP074199.D | AR-1254-1 | yogesh | 8/8/2025 7:32:21 AM | mohammad | 8/8/2025 7:37:53 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PP081225 | Instrument | ECD_p |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|----------------------|-----------|----------------------|---------------|-------------------|-----------------------------|
| AR1242CCC500 | PP074303.D | AR-1242-3 #2 | yogesh | 8/13/2025 7:35:08 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074303.D | AR-1242-4 #2 | yogesh | 8/13/2025 7:35:08 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074304.D | AR-1254-1 | yogesh | 8/13/2025 7:35:10 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074304.D | AR-1254-1 #2 | yogesh | 8/13/2025 7:35:10 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074304.D | AR-1254-3 #2 | yogesh | 8/13/2025 7:35:10 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| PB169205BS | PP074309.D | AR-1260-4 | yogesh | 8/13/2025 7:35:14 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| Q2830-01MS | PP074311.D | AR-1260-4 | yogesh | 8/13/2025 7:35:18 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| Q2830-01MS | PP074311.D | Tetrachloro-m-xylene | yogesh | 8/13/2025 7:35:18 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| Q2830-01MSD | PP074312.D | AR-1260-4 | yogesh | 8/13/2025 7:35:19 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| Q2830-01MSD | PP074312.D | Decachlorobiphenyl | yogesh | 8/13/2025 7:35:19 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| Q2830-01MSD | PP074312.D | Tetrachloro-m-xylene | yogesh | 8/13/2025 7:35:19 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1660CCC500 | PP074316.D | AR-1016-2 #2 | yogesh | 8/13/2025 7:35:23 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1660CCC500 | PP074316.D | AR-1016-5 #2 | yogesh | 8/13/2025 7:35:23 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |

 1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PP081225 | Instrument | ECD_p |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|-------------------------|-----------|----------------------|---------------|-------------------|-----------------------------|
| AR1660CCC500 | PP074316.D | Tetrachloro-m-xylene #2 | yogesh | 8/13/2025 7:35:23 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074317.D | AR-1242-2 #2 | yogesh | 8/13/2025 7:35:24 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074317.D | AR-1242-3 #2 | yogesh | 8/13/2025 7:35:24 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074317.D | AR-1242-4 #2 | yogesh | 8/13/2025 7:35:24 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074318.D | AR-1254-1 | yogesh | 8/13/2025 7:35:26 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074318.D | AR-1254-1 #2 | yogesh | 8/13/2025 7:35:26 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074318.D | AR-1254-2 #2 | yogesh | 8/13/2025 7:35:26 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074318.D | AR-1254-3 #2 | yogesh | 8/13/2025 7:35:26 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074318.D | AR-1254-4 #2 | yogesh | 8/13/2025 7:35:26 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074318.D | AR-1254-5 #2 | yogesh | 8/13/2025 7:35:26 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074330.D | AR-1242-2 #2 | yogesh | 8/13/2025 7:35:40 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074330.D | AR-1242-3 #2 | yogesh | 8/13/2025 7:35:40 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1242CCC500 | PP074330.D | AR-1242-4 #2 | yogesh | 8/13/2025 7:35:40 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Manual Integration Report

| | | | |
|-----------|----------|------------|-------|
| Sequence: | PP081225 | Instrument | ECD_p |
|-----------|----------|------------|-------|

| Sample ID | File ID | Parameter | Review By | Review On | Supervised By | Supervised On | Reason |
|--------------|------------|--------------|-----------|----------------------|---------------|-------------------|-----------------------------|
| AR1254CCC500 | PP074331.D | AR-1254-1 | yogesh | 8/13/2025 7:35:42 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074331.D | AR-1254-2 #2 | yogesh | 8/13/2025 7:35:42 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074331.D | AR-1254-3 #2 | yogesh | 8/13/2025 7:35:42 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074331.D | AR-1254-4 #2 | yogesh | 8/13/2025 7:35:42 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |
| AR1254CCC500 | PP074331.D | AR-1254-5 #2 | yogesh | 8/13/2025 7:35:42 AM | mohammad | 8/14/2025 1:21:51 | Peak Integrated by Software |

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072325

| Review By | yogesh | Review On | 7/23/2025 3:39:31 PM |
|---|--|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 7/25/2025 3:53:10 AM |
| SubDirectory | PO072325 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | |

| Sr# | SampleId | Data File Name | Date-Time | Operator | Status |
|-----|---------------|----------------|-------------------|----------|--------|
| 1 | HEXANE | PO112412.D | 23 Jul 2025 10:56 | YP/AJ | Ok |
| 2 | I.BLK | PO112413.D | 23 Jul 2025 11:14 | YP/AJ | Ok |
| 3 | AR1660ICC1000 | PO112414.D | 23 Jul 2025 11:32 | YP/AJ | Ok |
| 4 | AR1660ICC750 | PO112415.D | 23 Jul 2025 11:50 | YP/AJ | Ok |
| 5 | AR1660ICC500 | PO112416.D | 23 Jul 2025 12:08 | YP/AJ | Ok |
| 6 | AR1660ICC250 | PO112417.D | 23 Jul 2025 12:27 | YP/AJ | Ok,M |
| 7 | AR1660ICC050 | PO112418.D | 23 Jul 2025 12:45 | YP/AJ | Ok,M |
| 8 | AR1221ICC500 | PO112419.D | 23 Jul 2025 13:03 | YP/AJ | Ok |
| 9 | AR1232ICC500 | PO112420.D | 23 Jul 2025 13:22 | YP/AJ | Ok |
| 10 | AR1242ICC1000 | PO112421.D | 23 Jul 2025 13:40 | YP/AJ | Ok |
| 11 | AR1242ICC750 | PO112422.D | 23 Jul 2025 13:59 | YP/AJ | Ok |
| 12 | AR1242ICC500 | PO112423.D | 23 Jul 2025 14:17 | YP/AJ | Ok |
| 13 | AR1242ICC250 | PO112424.D | 23 Jul 2025 14:36 | YP/AJ | Ok,M |
| 14 | AR1242ICC050 | PO112425.D | 23 Jul 2025 14:54 | YP/AJ | Ok,M |
| 15 | AR1248ICC1000 | PO112426.D | 23 Jul 2025 15:13 | YP/AJ | Ok |
| 16 | AR1248ICC750 | PO112427.D | 23 Jul 2025 15:31 | YP/AJ | Ok |
| 17 | AR1248ICC500 | PO112428.D | 23 Jul 2025 15:48 | YP/AJ | Ok |
| 18 | AR1248ICC250 | PO112429.D | 23 Jul 2025 16:07 | YP/AJ | Ok |
| 19 | AR1248ICC050 | PO112430.D | 23 Jul 2025 16:25 | YP/AJ | Ok,M |
| 20 | AR1254ICC1000 | PO112431.D | 23 Jul 2025 16:44 | YP/AJ | Ok |
| 21 | AR1254ICC750 | PO112432.D | 23 Jul 2025 17:02 | YP/AJ | Ok |

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072325

| Review By | yogesh | Review On | 7/23/2025 3:39:31 PM | | |
|---|--|-------------------|----------------------|----------------------|----------|
| Supervise By | mohammad | Supervise On | 7/25/2025 3:53:10 AM | | |
| SubDirectory | PO072325 | HP Acquire Method | | HP Processing Method | PO072325 |
| STD. NAME | STD REF.# | | | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | | | |

| | | | | | |
|----|----------------|------------|-------------------|-------|------|
| 22 | AR1254ICC500 | PO112433.D | 23 Jul 2025 17:21 | YP/AJ | Ok |
| 23 | AR1254ICC250 | PO112434.D | 23 Jul 2025 17:39 | YP/AJ | Ok |
| 24 | AR1254ICC050 | PO112435.D | 23 Jul 2025 17:57 | YP/AJ | Ok,M |
| 25 | AR1262ICC500 | PO112436.D | 23 Jul 2025 18:16 | YP/AJ | Ok |
| 26 | AR1268ICC1000 | PO112437.D | 23 Jul 2025 18:34 | YP/AJ | Ok |
| 27 | AR1268ICC750 | PO112438.D | 23 Jul 2025 18:53 | YP/AJ | Ok |
| 28 | AR1268ICC500 | PO112439.D | 23 Jul 2025 19:11 | YP/AJ | Ok |
| 29 | AR1268ICC250 | PO112440.D | 23 Jul 2025 19:28 | YP/AJ | Ok |
| 30 | AR1268ICC050 | PO112441.D | 23 Jul 2025 19:47 | YP/AJ | Ok |
| 31 | PO072325ICV500 | PO112442.D | 23 Jul 2025 20:05 | YP/AJ | Ok |
| 32 | AR1242ICV500 | PO112443.D | 23 Jul 2025 20:42 | YP/AJ | Ok |
| 33 | AR1248ICV500 | PO112444.D | 23 Jul 2025 21:18 | YP/AJ | Ok |
| 34 | AR1254ICV500 | PO112445.D | 23 Jul 2025 21:54 | YP/AJ | Ok |
| 35 | AR1268ICV500 | PO112446.D | 23 Jul 2025 22:31 | YP/AJ | Ok |
| 36 | DDT ANALOG | PO112447.D | 23 Jul 2025 23:07 | YP/AJ | Ok |

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO081225

| Review By | yogesh | Review On | 8/12/2025 10:12:49 AM |
|---|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:40 AM |
| SubDirectory | PO081225 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | |

| Sr# | SampleId | Data File Name | Date-Time | Operator | Status |
|-----|--------------|----------------|-------------------|----------|--------|
| 1 | HEXANE | PO112849.D | 12 Aug 2025 08:35 | YP/AJ | Ok |
| 2 | AR1660CCC500 | PO112850.D | 12 Aug 2025 08:54 | YP/AJ | Ok,M |
| 3 | AR1242CCC500 | PO112851.D | 12 Aug 2025 09:12 | YP/AJ | Ok,M |
| 4 | AR1248CCC500 | PO112852.D | 12 Aug 2025 09:29 | YP/AJ | Ok,M |
| 5 | AR1254CCC500 | PO112853.D | 12 Aug 2025 09:48 | YP/AJ | Ok |
| 6 | I.BLK | PO112854.D | 12 Aug 2025 10:05 | YP/AJ | Ok |
| 7 | DDT ANALOG | PO112855.D | 12 Aug 2025 10:24 | YP/AJ | Ok |
| 8 | Q2808-01DL | PO112856.D | 12 Aug 2025 10:42 | YP/AJ | Ok,M |
| 9 | Q2807-02 | PO112857.D | 12 Aug 2025 11:01 | YP/AJ | Ok |
| 10 | Q2818-01 | PO112858.D | 12 Aug 2025 12:50 | YP/AJ | Ok,M |
| 11 | Q2818-02 | PO112859.D | 12 Aug 2025 13:08 | YP/AJ | Ok |
| 12 | Q2819-06 | PO112860.D | 12 Aug 2025 13:26 | YP/AJ | Ok |
| 13 | Q2819-11 | PO112861.D | 12 Aug 2025 13:43 | YP/AJ | Ok |
| 14 | Q2819-14 | PO112862.D | 12 Aug 2025 14:01 | YP/AJ | Ok |
| 15 | Q2820-09 | PO112863.D | 12 Aug 2025 14:20 | YP/AJ | ReRun |
| 16 | Q2820-10 | PO112864.D | 12 Aug 2025 14:38 | YP/AJ | Ok |
| 17 | AR1660CCC500 | PO112865.D | 12 Aug 2025 15:50 | YP/AJ | Ok,M |
| 18 | AR1242CCC500 | PO112866.D | 12 Aug 2025 16:07 | YP/AJ | Ok,M |
| 19 | AR1248CCC500 | PO112867.D | 12 Aug 2025 16:25 | YP/AJ | Ok |
| 20 | AR1254CCC500 | PO112868.D | 12 Aug 2025 16:42 | YP/AJ | Ok |
| 21 | I.BLK | PO112869.D | 12 Aug 2025 17:00 | YP/AJ | Ok |

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO081225

| Review By | yogesh | Review On | 8/12/2025 10:12:49 AM | | |
|---|---|-------------------|-----------------------|----------------------|----------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:40 AM | | |
| SubDirectory | PO081225 | HP Acquire Method | | HP Processing Method | PO072325 |
| STD. NAME | STD REF.# | | | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | | | |

| | | | | | |
|----|--------------|------------|-------------------|-------|----------|
| 22 | Q2820-24 | PO112870.D | 12 Aug 2025 17:19 | YP/AJ | Ok |
| 23 | Q2823-01 | PO112871.D | 12 Aug 2025 17:37 | YP/AJ | Ok,M |
| 24 | Q2826-01 | PO112872.D | 12 Aug 2025 17:56 | YP/AJ | Ok |
| 25 | Q2827-01 | PO112873.D | 12 Aug 2025 18:14 | YP/AJ | Dilution |
| 26 | Q2827-05 | PO112874.D | 12 Aug 2025 18:31 | YP/AJ | Ok |
| 27 | Q2830-03 | PO112875.D | 12 Aug 2025 18:49 | YP/AJ | Ok |
| 28 | Q2839-01 | PO112876.D | 12 Aug 2025 19:06 | YP/AJ | Ok,M |
| 29 | Q2839-02 | PO112877.D | 12 Aug 2025 19:24 | YP/AJ | Ok,M |
| 30 | Q2839-03 | PO112878.D | 12 Aug 2025 19:42 | YP/AJ | Ok |
| 31 | Q2839-04 | PO112879.D | 12 Aug 2025 19:59 | YP/AJ | Ok,M |
| 32 | AR1660CCC500 | PO112880.D | 12 Aug 2025 21:09 | YP/AJ | Ok,M |
| 33 | AR1242CCC500 | PO112881.D | 12 Aug 2025 22:02 | YP/AJ | Ok,M |
| 34 | AR1248CCC500 | PO112882.D | 12 Aug 2025 22:21 | YP/AJ | Ok |
| 35 | AR1254CCC500 | PO112883.D | 12 Aug 2025 22:38 | YP/AJ | Ok |
| 36 | I.BLK | PO112884.D | 12 Aug 2025 22:56 | YP/AJ | Ok |
| 37 | Q2839-05 | PO112885.D | 12 Aug 2025 23:15 | YP/AJ | Ok |
| 38 | Q2839-06 | PO112886.D | 12 Aug 2025 23:33 | YP/AJ | Ok |
| 39 | Q2839-07 | PO112887.D | 12 Aug 2025 23:51 | YP/AJ | Ok,M |
| 40 | Q2839-08 | PO112888.D | 13 Aug 2025 00:09 | YP/AJ | Ok,M |
| 41 | Q2839-09 | PO112889.D | 13 Aug 2025 00:27 | YP/AJ | Ok |
| 42 | AR1660CCC500 | PO112890.D | 13 Aug 2025 01:41 | YP/AJ | Ok,M |
| 43 | AR1242CCC500 | PO112891.D | 13 Aug 2025 02:34 | YP/AJ | Ok,M |
| 44 | AR1248CCC500 | PO112892.D | 13 Aug 2025 02:52 | YP/AJ | Ok |

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO081225

| Review By | yogesh | Review On | 8/12/2025 10:12:49 AM |
|--------------------------|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:40 AM |
| SubDirectory | PO081225 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk | | | |
| Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | |
| CCC | PP24332,PP24347,PP24352,PP24357 | | |
| Internal Standard/PEM | | | |
| ICV/I.BLK | PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | |
| Surrogate Standard | | | |
| MS/MSD Standard | | | |
| LCS Standard | | | |

| | | | | | |
|----|--------------|------------|-------------------|-------|------|
| 45 | AR1254CCC500 | PO112893.D | 13 Aug 2025 03:11 | YP/AJ | Ok,M |
| 46 | I.BLK | PO112894.D | 13 Aug 2025 03:29 | YP/AJ | Ok |

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP080125

| Review By | yogesh | Review On | 8/1/2025 3:30:36 PM |
|--------------------------|---|-------------------|------------------------------------|
| Supervise By | mohammad | Supervise On | 8/8/2025 7:37:53 AM |
| SubDirectory | PP080125 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk | | | |
| Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | |
| CCC | PP24332,PP24347,PP24352,PP24357 | | |
| Internal Standard/PEM | | | |
| ICV/I.BLK | PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | |
| Surrogate Standard | | | |
| MS/MSD Standard | | | |
| LCS Standard | | | |

| Sr# | SampleId | Data File Name | Date-Time | Operator | Status |
|-----|---------------|----------------|-------------------|----------|--------|
| 1 | HEXANE | PP074166.D | 01 Aug 2025 11:33 | YP\AJ | Ok |
| 2 | I.BLK | PP074167.D | 01 Aug 2025 11:49 | YP\AJ | Ok |
| 3 | AR1660ICC1000 | PP074168.D | 01 Aug 2025 12:05 | YP\AJ | Ok |
| 4 | AR1660ICC750 | PP074169.D | 01 Aug 2025 12:22 | YP\AJ | Ok |
| 5 | AR1660ICC500 | PP074170.D | 01 Aug 2025 12:38 | YP\AJ | Ok |
| 6 | AR1660ICC250 | PP074171.D | 01 Aug 2025 12:54 | YP\AJ | Ok,M |
| 7 | AR1660ICC050 | PP074172.D | 01 Aug 2025 13:42 | YP\AJ | Ok,M |
| 8 | AR1221ICC500 | PP074173.D | 01 Aug 2025 13:58 | YP\AJ | Ok |
| 9 | AR1232ICC500 | PP074174.D | 01 Aug 2025 14:15 | YP\AJ | Ok,M |
| 10 | AR1242ICC1000 | PP074175.D | 01 Aug 2025 14:31 | YP\AJ | Ok,M |
| 11 | AR1242ICC750 | PP074176.D | 01 Aug 2025 14:47 | YP\AJ | Ok,M |
| 12 | AR1242ICC500 | PP074177.D | 01 Aug 2025 15:03 | YP\AJ | Ok,M |
| 13 | AR1242ICC250 | PP074178.D | 01 Aug 2025 15:19 | YP\AJ | Ok,M |
| 14 | AR1242ICC050 | PP074179.D | 01 Aug 2025 15:36 | YP\AJ | Ok,M |
| 15 | AR1248ICC1000 | PP074180.D | 01 Aug 2025 16:24 | YP\AJ | Not Ok |
| 16 | AR1248ICC750 | PP074181.D | 01 Aug 2025 16:41 | YP\AJ | Not Ok |
| 17 | AR1248ICC500 | PP074182.D | 01 Aug 2025 16:57 | YP\AJ | Ok,M |
| 18 | AR1248ICC250 | PP074183.D | 01 Aug 2025 17:13 | YP\AJ | Not Ok |
| 19 | AR1248ICC050 | PP074184.D | 01 Aug 2025 17:45 | YP\AJ | Not Ok |
| 20 | AR1254ICC1000 | PP074185.D | 01 Aug 2025 18:02 | YP\AJ | Ok,M |
| 21 | AR1254ICC750 | PP074186.D | 01 Aug 2025 18:18 | YP\AJ | Ok,M |

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP080125

| Review By | yogesh | Review On | 8/1/2025 3:30:36 PM | | |
|--------------------------|---|-------------------|---------------------|----------------------|----------|
| Supervise By | mohammad | Supervise On | 8/8/2025 7:37:53 AM | | |
| SubDirectory | PP080125 | HP Acquire Method | | HP Processing Method | PP080125 |
| STD. NAME | STD REF.# | | | | |
| Tune/Reschk | | | | | |
| Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344 ,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP2435 9,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | | | |
| CCC | PP24332,PP24347,PP24352,PP24357 | | | | |
| Internal Standard/PEM | | | | | |
| ICV/I.BLK | PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | | | |
| Surrogate Standard | | | | | |
| MS/MSD Standard | | | | | |
| LCS Standard | | | | | |

| | | | | | |
|----|----------------|------------|-------------------|-------|--------|
| 22 | AR1254ICC500 | PP074187.D | 01 Aug 2025 18:34 | YP\AJ | Ok,M |
| 23 | AR1254ICC250 | PP074188.D | 01 Aug 2025 18:50 | YP\AJ | Ok,M |
| 24 | AR1254ICC050 | PP074189.D | 01 Aug 2025 19:23 | YP\AJ | Ok,M |
| 25 | AR1262ICC500 | PP074190.D | 01 Aug 2025 19:39 | YP\AJ | Ok |
| 26 | AR1268ICC1000 | PP074191.D | 01 Aug 2025 19:55 | YP\AJ | Not Ok |
| 27 | AR1268ICC750 | PP074192.D | 01 Aug 2025 20:11 | YP\AJ | Not Ok |
| 28 | AR1268ICC500 | PP074193.D | 01 Aug 2025 20:28 | YP\AJ | Ok |
| 29 | AR1268ICC250 | PP074194.D | 01 Aug 2025 20:44 | YP\AJ | Not Ok |
| 30 | AR1268ICC050 | PP074195.D | 01 Aug 2025 21:00 | YP\AJ | Not Ok |
| 31 | PP080125ICV500 | PP074196.D | 01 Aug 2025 21:16 | YP\AJ | Ok |
| 32 | AR1242ICV500 | PP074197.D | 01 Aug 2025 22:05 | YP\AJ | Ok,M |
| 33 | AR1248ICV500 | PP074198.D | 01 Aug 2025 22:37 | YP\AJ | Not Ok |
| 34 | AR1254ICV500 | PP074199.D | 01 Aug 2025 23:10 | YP\AJ | Ok,M |
| 35 | AR1268ICV500 | PP074200.D | 01 Aug 2025 23:42 | YP\AJ | Not Ok |
| 36 | DDT ANALOG | PP074201.D | 02 Aug 2025 00:15 | YP\AJ | Ok |

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP081225

| Review By | yogesh | Review On | 8/12/2025 10:13:41 AM |
|--------------------------|---|-------------------|------------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:51 AM |
| SubDirectory | PP081225 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk | | | |
| Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | |
| CCC | PP24332,PP24347,PP24352,PP24357 | | |
| Internal Standard/PEM | | | |
| ICV/I.BLK | PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | |
| Surrogate Standard | | | |
| MS/MSD Standard | | | |
| LCS Standard | | | |

| Sr# | SampleId | Data File Name | Date-Time | Operator | Status |
|-----|--------------|----------------|-------------------|----------|--------|
| 1 | HEXANE | PP074301.D | 12 Aug 2025 09:35 | YP\AJ | Ok |
| 2 | AR1660CCC500 | PP074302.D | 12 Aug 2025 09:51 | YP\AJ | Ok |
| 3 | AR1242CCC500 | PP074303.D | 12 Aug 2025 10:11 | YP\AJ | Ok,M |
| 4 | AR1254CCC500 | PP074304.D | 12 Aug 2025 10:27 | YP\AJ | Ok,M |
| 5 | I.BLK | PP074305.D | 12 Aug 2025 10:43 | YP\AJ | Ok |
| 6 | DDT ANALOG | PP074306.D | 12 Aug 2025 10:59 | YP\AJ | Ok |
| 7 | PP24799 | PP074307.D | 12 Aug 2025 11:16 | YP\AJ | Ok,M |
| 8 | PB169205BL | PP074308.D | 12 Aug 2025 12:48 | YP\AJ | Ok |
| 9 | PB169205BS | PP074309.D | 12 Aug 2025 13:05 | YP\AJ | Ok,M |
| 10 | Q2830-01 | PP074310.D | 12 Aug 2025 13:21 | YP\AJ | Ok,M |
| 11 | Q2830-01MS | PP074311.D | 12 Aug 2025 13:37 | YP\AJ | Ok,M |
| 12 | Q2830-01MSD | PP074312.D | 12 Aug 2025 13:53 | YP\AJ | Ok,M |
| 13 | Q2830-05 | PP074313.D | 12 Aug 2025 14:10 | YP\AJ | Ok |
| 14 | Q2830-07 | PP074314.D | 12 Aug 2025 14:26 | YP\AJ | Ok,M |
| 15 | Q2831-01 | PP074315.D | 12 Aug 2025 14:42 | YP\AJ | Ok |
| 16 | AR1660CCC500 | PP074316.D | 12 Aug 2025 15:48 | YP\AJ | Ok,M |
| 17 | AR1242CCC500 | PP074317.D | 12 Aug 2025 16:20 | YP\AJ | Ok,M |
| 18 | AR1254CCC500 | PP074318.D | 12 Aug 2025 16:37 | YP\AJ | Ok,M |
| 19 | I.BLK | PP074319.D | 12 Aug 2025 16:53 | YP\AJ | Ok |
| 20 | PB169220BL | PP074320.D | 12 Aug 2025 17:26 | YP\AJ | Ok |
| 21 | PB169220BS | PP074321.D | 12 Aug 2025 17:42 | YP\AJ | Ok |

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP081225

| Review By | yogesh | Review On | 8/12/2025 10:13:41 AM |
|--------------------------|---|-------------------|------------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:51 AM |
| SubDirectory | PP081225 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk | | | |
| Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | |
| CCC | PP24332,PP24347,PP24352,PP24357 | | |
| Internal Standard/PEM | | | |
| ICV/I.BLK | PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP2 | | |
| Surrogate Standard | | | |
| MS/MSD Standard | | | |
| LCS Standard | | | |

| | | | | | |
|----|--------------|------------|-------------------|-------|------|
| 22 | Q2839-10 | PP074322.D | 12 Aug 2025 17:58 | YP\AJ | Ok,M |
| 23 | Q2839-11 | PP074323.D | 12 Aug 2025 18:14 | YP\AJ | Ok,M |
| 24 | Q2839-12 | PP074324.D | 12 Aug 2025 18:31 | YP\AJ | Ok,M |
| 25 | Q2839-13 | PP074325.D | 12 Aug 2025 18:47 | YP\AJ | Ok,M |
| 26 | Q2839-14 | PP074326.D | 12 Aug 2025 19:03 | YP\AJ | Ok,M |
| 27 | Q2839-15 | PP074327.D | 12 Aug 2025 19:20 | YP\AJ | Ok,M |
| 28 | Q2839-16 | PP074328.D | 12 Aug 2025 19:36 | YP\AJ | Ok,M |
| 29 | AR1660CCC500 | PP074329.D | 12 Aug 2025 20:41 | YP\AJ | Ok |
| 30 | AR1242CCC500 | PP074330.D | 12 Aug 2025 21:30 | YP\AJ | Ok,M |
| 31 | AR1254CCC500 | PP074331.D | 12 Aug 2025 21:46 | YP\AJ | Ok,M |
| 32 | I.BLK | PP074332.D | 12 Aug 2025 22:02 | YP\AJ | Ok |

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072325

| Review By | yogesh | Review On | 7/23/2025 3:39:31 PM |
|---|--|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 7/25/2025 3:53:10 AM |
| SubDirectory | PO072325 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| Sr# | SampleId | ClientID | Data File Name | Date-Time | Comment | Operator | Status |
|-----|---------------|---------------|----------------|-------------------|---------|----------|--------|
| 1 | HEXANE | HEXANE | PO112412.D | 23 Jul 2025 10:56 | | YP/AJ | Ok |
| 2 | I.BLK | I.BLK | PO112413.D | 23 Jul 2025 11:14 | | YP/AJ | Ok |
| 3 | AR1660ICC1000 | AR1660ICC1000 | PO112414.D | 23 Jul 2025 11:32 | | YP/AJ | Ok |
| 4 | AR1660ICC750 | AR1660ICC750 | PO112415.D | 23 Jul 2025 11:50 | | YP/AJ | Ok |
| 5 | AR1660ICC500 | AR1660ICC500 | PO112416.D | 23 Jul 2025 12:08 | | YP/AJ | Ok |
| 6 | AR1660ICC250 | AR1660ICC250 | PO112417.D | 23 Jul 2025 12:27 | | YP/AJ | Ok,M |
| 7 | AR1660ICC050 | AR1660ICC050 | PO112418.D | 23 Jul 2025 12:45 | | YP/AJ | Ok,M |
| 8 | AR1221ICC500 | AR1221ICC500 | PO112419.D | 23 Jul 2025 13:03 | | YP/AJ | Ok |
| 9 | AR1232ICC500 | AR1232ICC500 | PO112420.D | 23 Jul 2025 13:22 | | YP/AJ | Ok |
| 10 | AR1242ICC1000 | AR1242ICC1000 | PO112421.D | 23 Jul 2025 13:40 | | YP/AJ | Ok |
| 11 | AR1242ICC750 | AR1242ICC750 | PO112422.D | 23 Jul 2025 13:59 | | YP/AJ | Ok |
| 12 | AR1242ICC500 | AR1242ICC500 | PO112423.D | 23 Jul 2025 14:17 | | YP/AJ | Ok |
| 13 | AR1242ICC250 | AR1242ICC250 | PO112424.D | 23 Jul 2025 14:36 | | YP/AJ | Ok,M |
| 14 | AR1242ICC050 | AR1242ICC050 | PO112425.D | 23 Jul 2025 14:54 | | YP/AJ | Ok,M |
| 15 | AR1248ICC1000 | AR1248ICC1000 | PO112426.D | 23 Jul 2025 15:13 | | YP/AJ | Ok |
| 16 | AR1248ICC750 | AR1248ICC750 | PO112427.D | 23 Jul 2025 15:31 | | YP/AJ | Ok |
| 17 | AR1248ICC500 | AR1248ICC500 | PO112428.D | 23 Jul 2025 15:48 | | YP/AJ | Ok |
| 18 | AR1248ICC250 | AR1248ICC250 | PO112429.D | 23 Jul 2025 16:07 | | YP/AJ | Ok |

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO072325

| Review By | yogesh | Review On | 7/23/2025 3:39:31 PM |
|---|--|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 7/25/2025 3:53:10 AM |
| SubDirectory | PO072325 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| | | | | | | | |
|----|----------------|-------------------|------------|-------------------|--|-------|------|
| 19 | AR1248ICC050 | AR1248ICC050 | PO112430.D | 23 Jul 2025 16:25 | | YP/AJ | Ok,M |
| 20 | AR1254ICC1000 | AR1254ICC1000 | PO112431.D | 23 Jul 2025 16:44 | | YP/AJ | Ok |
| 21 | AR1254ICC750 | AR1254ICC750 | PO112432.D | 23 Jul 2025 17:02 | | YP/AJ | Ok |
| 22 | AR1254ICC500 | AR1254ICC500 | PO112433.D | 23 Jul 2025 17:21 | | YP/AJ | Ok |
| 23 | AR1254ICC250 | AR1254ICC250 | PO112434.D | 23 Jul 2025 17:39 | | YP/AJ | Ok |
| 24 | AR1254ICC050 | AR1254ICC050 | PO112435.D | 23 Jul 2025 17:57 | | YP/AJ | Ok,M |
| 25 | AR1262ICC500 | AR1262ICC500 | PO112436.D | 23 Jul 2025 18:16 | | YP/AJ | Ok |
| 26 | AR1268ICC1000 | AR1268ICC1000 | PO112437.D | 23 Jul 2025 18:34 | | YP/AJ | Ok |
| 27 | AR1268ICC750 | AR1268ICC750 | PO112438.D | 23 Jul 2025 18:53 | | YP/AJ | Ok |
| 28 | AR1268ICC500 | AR1268ICC500 | PO112439.D | 23 Jul 2025 19:11 | | YP/AJ | Ok |
| 29 | AR1268ICC250 | AR1268ICC250 | PO112440.D | 23 Jul 2025 19:28 | | YP/AJ | Ok |
| 30 | AR1268ICC050 | AR1268ICC050 | PO112441.D | 23 Jul 2025 19:47 | | YP/AJ | Ok |
| 31 | PO072325ICV500 | ICVPO072325 | PO112442.D | 23 Jul 2025 20:05 | | YP/AJ | Ok |
| 32 | AR1242ICV500 | ICVPO072325AR1242 | PO112443.D | 23 Jul 2025 20:42 | | YP/AJ | Ok |
| 33 | AR1248ICV500 | ICVPO072325AR1248 | PO112444.D | 23 Jul 2025 21:18 | | YP/AJ | Ok |
| 34 | AR1254ICV500 | ICVPO072325AR1254 | PO112445.D | 23 Jul 2025 21:54 | | YP/AJ | Ok |
| 35 | AR1268ICV500 | ICVPO072325AR1268 | PO112446.D | 23 Jul 2025 22:31 | | YP/AJ | Ok |
| 36 | DDT ANALOG | DDT ANALOG | PO112447.D | 23 Jul 2025 23:07 | | YP/AJ | Ok |

M : Manual Integration

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO081225

| Review By | yogesh | Review On | 8/12/2025 10:12:49 AM | |
|--|---|-------------------|-----------------------|----------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:40 AM | |
| SubDirectory | PO081225 | HP Acquire Method | HP Processing Method | PO072325 |
| STD. NAME | STD REF.# | | | |
| Tune/Reschk Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | | |
| CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | | |

| Sr# | SampleId | ClientID | Data File Name | Date-Time | Comment | Operator | Status |
|-----|--------------|--------------|----------------|-------------------|-----------------------|----------|--------|
| 1 | HEXANE | HEXANE | PO112849.D | 12 Aug 2025 08:35 | | YP/AJ | Ok |
| 2 | AR1660CCC500 | AR1660CCC500 | PO112850.D | 12 Aug 2025 08:54 | | YP/AJ | Ok,M |
| 3 | AR1242CCC500 | AR1242CCC500 | PO112851.D | 12 Aug 2025 09:12 | | YP/AJ | Ok,M |
| 4 | AR1248CCC500 | AR1248CCC500 | PO112852.D | 12 Aug 2025 09:29 | | YP/AJ | Ok,M |
| 5 | AR1254CCC500 | AR1254CCC500 | PO112853.D | 12 Aug 2025 09:48 | | YP/AJ | Ok |
| 6 | I.BLK | I.BLK | PO112854.D | 12 Aug 2025 10:05 | | YP/AJ | Ok |
| 7 | DDT ANALOG | DDT ANALOG | PO112855.D | 12 Aug 2025 10:24 | | YP/AJ | Ok |
| 8 | Q2808-01DL | TP-7DL | PO112856.D | 12 Aug 2025 10:42 | AR1242 + 1254 Hit | YP/AJ | Ok,M |
| 9 | Q2807-02 | COMP-5 | PO112857.D | 12 Aug 2025 11:01 | | YP/AJ | Ok |
| 10 | Q2818-01 | B-2-5-1 | PO112858.D | 12 Aug 2025 12:50 | | YP/AJ | Ok,M |
| 11 | Q2818-02 | B-3-5-2 | PO112859.D | 12 Aug 2025 13:08 | | YP/AJ | Ok |
| 12 | Q2819-06 | 11M-S | PO112860.D | 12 Aug 2025 13:26 | | YP/AJ | Ok |
| 13 | Q2819-11 | 84SB-W | PO112861.D | 12 Aug 2025 13:43 | DCB low in 1ST column | YP/AJ | Ok |
| 14 | Q2819-14 | 17M-W | PO112862.D | 12 Aug 2025 14:01 | | YP/AJ | Ok |
| 15 | Q2820-09 | 705R-S | PO112863.D | 12 Aug 2025 14:20 | DCB low both column | YP/AJ | ReRun |
| 16 | Q2820-10 | SOIL-DUP-2 | PO112864.D | 12 Aug 2025 14:38 | | YP/AJ | Ok |
| 17 | AR1660CCC500 | AR1660CCC500 | PO112865.D | 12 Aug 2025 15:50 | | YP/AJ | Ok,M |
| 18 | AR1242CCC500 | AR1242CCC500 | PO112866.D | 12 Aug 2025 16:07 | | YP/AJ | Ok,M |

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO081225

| Review By | yogesh | Review On | 8/12/2025 10:12:49 AM |
|---|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:40 AM |
| SubDirectory | PO081225 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| | | | | | | | |
|----|--------------|--------------------|------------|-------------------|--|-------|----------|
| 19 | AR1248CCC500 | AR1248CCC500 | PO112867.D | 12 Aug 2025 16:25 | | YP/AJ | Ok |
| 20 | AR1254CCC500 | AR1254CCC500 | PO112868.D | 12 Aug 2025 16:42 | TCMX high in 1st column | YP/AJ | Ok |
| 21 | I.BLK | I.BLK | PO112869.D | 12 Aug 2025 17:00 | | YP/AJ | Ok |
| 22 | Q2820-24 | 22M-S | PO112870.D | 12 Aug 2025 17:19 | | YP/AJ | Ok |
| 23 | Q2823-01 | SU-04-081125 | PO112871.D | 12 Aug 2025 17:37 | | YP/AJ | Ok,M |
| 24 | Q2826-01 | WC1 | PO112872.D | 12 Aug 2025 17:56 | AR1254 Hit | YP/AJ | Ok |
| 25 | Q2827-01 | TP-8 | PO112873.D | 12 Aug 2025 18:14 | AR1248 & AR1260 Hit , Need 2x dilution | YP/AJ | Dilution |
| 26 | Q2827-05 | TP-9 | PO112874.D | 12 Aug 2025 18:31 | AR1260 Hit | YP/AJ | Ok |
| 27 | Q2830-03 | BIN0009-DRIVEWAY-T | PO112875.D | 12 Aug 2025 18:49 | DCB high in 2nd column | YP/AJ | Ok |
| 28 | Q2839-01 | BC274436-1-1 | PO112876.D | 12 Aug 2025 19:06 | | YP/AJ | Ok,M |
| 29 | Q2839-02 | BC274436-1-2 | PO112877.D | 12 Aug 2025 19:24 | | YP/AJ | Ok,M |
| 30 | Q2839-03 | BC151973-1-1 | PO112878.D | 12 Aug 2025 19:42 | | YP/AJ | Ok |
| 31 | Q2839-04 | BC151973-1-2 | PO112879.D | 12 Aug 2025 19:59 | AR1254 Hit | YP/AJ | Ok,M |
| 32 | AR1660CCC500 | AR1660CCC500 | PO112880.D | 12 Aug 2025 21:09 | | YP/AJ | Ok,M |
| 33 | AR1242CCC500 | AR1242CCC500 | PO112881.D | 12 Aug 2025 22:02 | | YP/AJ | Ok,M |
| 34 | AR1248CCC500 | AR1248CCC500 | PO112882.D | 12 Aug 2025 22:21 | | YP/AJ | Ok |
| 35 | AR1254CCC500 | AR1254CCC500 | PO112883.D | 12 Aug 2025 22:38 | TCMX high in 1st column | YP/AJ | Ok |
| 36 | I.BLK | I.BLK | PO112884.D | 12 Aug 2025 22:56 | | YP/AJ | Ok |
| 37 | Q2839-05 | BC271336-1-1 | PO112885.D | 12 Aug 2025 23:15 | | YP/AJ | Ok |

Instrument ID: ECD_O

Daily Analysis Runlog For Sequence/QCBatch ID # PO081225

| Review By | yogesh | Review On | 8/12/2025 10:12:49 AM |
|---|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:40 AM |
| SubDirectory | PO081225 | HP Acquire Method | HP Processing Method PO072325 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,P P24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP 24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| | | | | | | | |
|----|--------------|--------------|------------|-------------------|-------------------------|-------|------|
| 38 | Q2839-06 | BC271336-1-2 | PO112886.D | 12 Aug 2025 23:33 | | YP/AJ | Ok |
| 39 | Q2839-07 | BC271242-1-1 | PO112887.D | 12 Aug 2025 23:51 | AR1254 Hit | YP/AJ | Ok,M |
| 40 | Q2839-08 | BC271242-1-2 | PO112888.D | 13 Aug 2025 00:09 | | YP/AJ | Ok,M |
| 41 | Q2839-09 | BC271242-2-1 | PO112889.D | 13 Aug 2025 00:27 | | YP/AJ | Ok |
| 42 | AR1660CCC500 | AR1660CCC500 | PO112890.D | 13 Aug 2025 01:41 | | YP/AJ | Ok,M |
| 43 | AR1242CCC500 | AR1242CCC500 | PO112891.D | 13 Aug 2025 02:34 | | YP/AJ | Ok,M |
| 44 | AR1248CCC500 | AR1248CCC500 | PO112892.D | 13 Aug 2025 02:52 | | YP/AJ | Ok |
| 45 | AR1254CCC500 | AR1254CCC500 | PO112893.D | 13 Aug 2025 03:11 | TCMX high in 1st column | YP/AJ | Ok,M |
| 46 | I.BLK | I.BLK | PO112894.D | 13 Aug 2025 03:29 | | YP/AJ | Ok |

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP080125

| Review By | yogesh | Review On | 8/1/2025 3:30:36 PM |
|--|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/8/2025 7:37:53 AM |
| SubDirectory | PP080125 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | |
| CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| Sr# | SampleId | ClientID | Data File Name | Date-Time | Comment | Operator | Status |
|-----|---------------|---------------|----------------|-------------------|---------|----------|--------|
| 1 | HEXANE | HEXANE | PP074166.D | 01 Aug 2025 11:33 | | YPAJ | Ok |
| 2 | I.BLK | I.BLK | PP074167.D | 01 Aug 2025 11:49 | | YPAJ | Ok |
| 3 | AR1660ICC1000 | AR1660ICC1000 | PP074168.D | 01 Aug 2025 12:05 | | YPAJ | Ok |
| 4 | AR1660ICC750 | AR1660ICC750 | PP074169.D | 01 Aug 2025 12:22 | | YPAJ | Ok |
| 5 | AR1660ICC500 | AR1660ICC500 | PP074170.D | 01 Aug 2025 12:38 | | YPAJ | Ok |
| 6 | AR1660ICC250 | AR1660ICC250 | PP074171.D | 01 Aug 2025 12:54 | | YPAJ | Ok,M |
| 7 | AR1660ICC050 | AR1660ICC050 | PP074172.D | 01 Aug 2025 13:42 | | YPAJ | Ok,M |
| 8 | AR1221ICC500 | AR1221ICC500 | PP074173.D | 01 Aug 2025 13:58 | | YPAJ | Ok |
| 9 | AR1232ICC500 | AR1232ICC500 | PP074174.D | 01 Aug 2025 14:15 | | YPAJ | Ok,M |
| 10 | AR1242ICC1000 | AR1242ICC1000 | PP074175.D | 01 Aug 2025 14:31 | | YPAJ | Ok,M |
| 11 | AR1242ICC750 | AR1242ICC750 | PP074176.D | 01 Aug 2025 14:47 | | YPAJ | Ok,M |
| 12 | AR1242ICC500 | AR1242ICC500 | PP074177.D | 01 Aug 2025 15:03 | | YPAJ | Ok,M |
| 13 | AR1242ICC250 | AR1242ICC250 | PP074178.D | 01 Aug 2025 15:19 | | YPAJ | Ok,M |
| 14 | AR1242ICC050 | AR1242ICC050 | PP074179.D | 01 Aug 2025 15:36 | | YPAJ | Ok,M |
| 15 | AR1248ICC1000 | AR1248ICC1000 | PP074180.D | 01 Aug 2025 16:24 | Not Use | YPAJ | Not Ok |
| 16 | AR1248ICC750 | AR1248ICC750 | PP074181.D | 01 Aug 2025 16:41 | Not Use | YPAJ | Not Ok |
| 17 | AR1248ICC500 | AR1248ICC500 | PP074182.D | 01 Aug 2025 16:57 | | YPAJ | Ok,M |
| 18 | AR1248ICC250 | AR1248ICC250 | PP074183.D | 01 Aug 2025 17:13 | Not Use | YPAJ | Not Ok |

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP080125

| Review By | yogesh | Review On | 8/1/2025 3:30:36 PM |
|---|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/8/2025 7:37:53 AM |
| SubDirectory | PP080125 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| | | | | | | | |
|----|----------------|-------------------|------------|-------------------|---------|------|--------|
| 19 | AR1248ICC050 | AR1248ICC050 | PP074184.D | 01 Aug 2025 17:45 | Not Use | YPAJ | Not Ok |
| 20 | AR1254ICC1000 | AR1254ICC1000 | PP074185.D | 01 Aug 2025 18:02 | | YPAJ | Ok,M |
| 21 | AR1254ICC750 | AR1254ICC750 | PP074186.D | 01 Aug 2025 18:18 | | YPAJ | Ok,M |
| 22 | AR1254ICC500 | AR1254ICC500 | PP074187.D | 01 Aug 2025 18:34 | | YPAJ | Ok,M |
| 23 | AR1254ICC250 | AR1254ICC250 | PP074188.D | 01 Aug 2025 18:50 | | YPAJ | Ok,M |
| 24 | AR1254ICC050 | AR1254ICC050 | PP074189.D | 01 Aug 2025 19:23 | | YPAJ | Ok,M |
| 25 | AR1262ICC500 | AR1262ICC500 | PP074190.D | 01 Aug 2025 19:39 | | YPAJ | Ok |
| 26 | AR1268ICC1000 | AR1268ICC1000 | PP074191.D | 01 Aug 2025 19:55 | Not Use | YPAJ | Not Ok |
| 27 | AR1268ICC750 | AR1268ICC750 | PP074192.D | 01 Aug 2025 20:11 | Not Use | YPAJ | Not Ok |
| 28 | AR1268ICC500 | AR1268ICC500 | PP074193.D | 01 Aug 2025 20:28 | | YPAJ | Ok |
| 29 | AR1268ICC250 | AR1268ICC250 | PP074194.D | 01 Aug 2025 20:44 | Not Use | YPAJ | Not Ok |
| 30 | AR1268ICC050 | AR1268ICC050 | PP074195.D | 01 Aug 2025 21:00 | Not Use | YPAJ | Not Ok |
| 31 | PP080125ICV500 | ICVPP080125 | PP074196.D | 01 Aug 2025 21:16 | | YPAJ | Ok |
| 32 | AR1242ICV500 | ICVPP080125AR1242 | PP074197.D | 01 Aug 2025 22:05 | | YPAJ | Ok,M |
| 33 | AR1248ICV500 | ICVPP080125AR1248 | PP074198.D | 01 Aug 2025 22:37 | Not Use | YPAJ | Not Ok |
| 34 | AR1254ICV500 | ICVPP080125AR1254 | PP074199.D | 01 Aug 2025 23:10 | | YPAJ | Ok,M |
| 35 | AR1268ICV500 | ICVPP080125AR1268 | PP074200.D | 01 Aug 2025 23:42 | Not Use | YPAJ | Not Ok |
| 36 | DDT ANALOG | DDT ANALOG | PP074201.D | 02 Aug 2025 00:15 | | YPAJ | Ok |

M : Manual Integration

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP081225

| Review By | yogesh | Review On | 8/12/2025 10:13:41 AM |
|--|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:51 AM |
| SubDirectory | PP081225 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 | | |
| CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| Sr# | SampleId | ClientID | Data File Name | Date-Time | Comment | Operator | Status |
|-----|--------------|--------------------|----------------|-------------------|------------------------------------|----------|--------|
| 1 | HEXANE | HEXANE | PP074301.D | 12 Aug 2025 09:35 | | YPAJ | Ok |
| 2 | AR1660CCC500 | AR1660CCC500 | PP074302.D | 12 Aug 2025 09:51 | AR1016-02& TCMX high in sec column | YPAJ | Ok |
| 3 | AR1242CCC500 | AR1242CCC500 | PP074303.D | 12 Aug 2025 10:11 | TCMX high in sec column | YPAJ | Ok,M |
| 4 | AR1254CCC500 | AR1254CCC500 | PP074304.D | 12 Aug 2025 10:27 | TCMX high in sec column | YPAJ | Ok,M |
| 5 | I.BLK | I.BLK | PP074305.D | 12 Aug 2025 10:43 | | YPAJ | Ok |
| 6 | DDT ANALOG | DDT ANALOG | PP074306.D | 12 Aug 2025 10:59 | | YPAJ | Ok |
| 7 | PP24799 | PP24799 | PP074307.D | 12 Aug 2025 11:16 | | YPAJ | Ok,M |
| 8 | PB169205BL | PB169205BL | PP074308.D | 12 Aug 2025 12:48 | | YPAJ | Ok |
| 9 | PB169205BS | PB169205BS | PP074309.D | 12 Aug 2025 13:05 | | YPAJ | Ok,M |
| 10 | Q2830-01 | BIN0009-DRIVeway-T | PP074310.D | 12 Aug 2025 13:21 | | YPAJ | Ok,M |
| 11 | Q2830-01MS | BIN0009-DRIVeway-T | PP074311.D | 12 Aug 2025 13:37 | | YPAJ | Ok,M |
| 12 | Q2830-01MSD | BIN0009-DRIVeway-T | PP074312.D | 12 Aug 2025 13:53 | | YPAJ | Ok,M |
| 13 | Q2830-05 | BIN0009-DRIVeway-T | PP074313.D | 12 Aug 2025 14:10 | | YPAJ | Ok |
| 14 | Q2830-07 | BIN0009-DRIVeway-T | PP074314.D | 12 Aug 2025 14:26 | | YPAJ | Ok,M |
| 15 | Q2831-01 | VNJ-238 | PP074315.D | 12 Aug 2025 14:42 | | YPAJ | Ok |
| 16 | AR1660CCC500 | AR1660CCC500 | PP074316.D | 12 Aug 2025 15:48 | | YPAJ | Ok,M |
| 17 | AR1242CCC500 | AR1242CCC500 | PP074317.D | 12 Aug 2025 16:20 | TCMX high in 2nd column | YPAJ | Ok,M |

Instrument ID: ECD_P

Daily Analysis Runlog For Sequence/QCBatch ID # PP081225

| Review By | yogesh | Review On | 8/12/2025 10:13:41 AM |
|---|---|-------------------|-------------------------------|
| Supervise By | mohammad | Supervise On | 8/14/2025 1:21:51 AM |
| SubDirectory | PP081225 | HP Acquire Method | HP Processing Method PP080125 |
| STD. NAME | STD REF.# | | |
| Tune/Reschk Initial Calibration Stds CCC Internal Standard/PEM ICV/I.BLK Surrogate Standard MS/MSD Standard LCS Standard | PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369 PP24332,PP24347,PP24352,PP24357 PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387 | | |

| | | | | | | | |
|----|--------------|--------------|------------|-------------------|-------------------------|------|------|
| 18 | AR1254CCC500 | AR1254CCC500 | PP074318.D | 12 Aug 2025 16:37 | | YPAJ | Ok,M |
| 19 | I.BLK | I.BLK | PP074319.D | 12 Aug 2025 16:53 | | YPAJ | Ok |
| 20 | PB169220BL | PB169220BL | PP074320.D | 12 Aug 2025 17:26 | | YPAJ | Ok |
| 21 | PB169220BS | PB169220BS | PP074321.D | 12 Aug 2025 17:42 | | YPAJ | Ok |
| 22 | Q2839-10 | BC271242-2-2 | PP074322.D | 12 Aug 2025 17:58 | | YPAJ | Ok,M |
| 23 | Q2839-11 | BC226751-1-1 | PP074323.D | 12 Aug 2025 18:14 | | YPAJ | Ok,M |
| 24 | Q2839-12 | BC226751-1-2 | PP074324.D | 12 Aug 2025 18:31 | | YPAJ | Ok,M |
| 25 | Q2839-13 | BC226751-2-1 | PP074325.D | 12 Aug 2025 18:47 | AR1254 Hit | YPAJ | Ok,M |
| 26 | Q2839-14 | BC226751-2-2 | PP074326.D | 12 Aug 2025 19:03 | | YPAJ | Ok,M |
| 27 | Q2839-15 | JEC773V-1-1 | PP074327.D | 12 Aug 2025 19:20 | TCMX low in 2nd column | YPAJ | Ok,M |
| 28 | Q2839-16 | JEC773V-1-2 | PP074328.D | 12 Aug 2025 19:36 | | YPAJ | Ok,M |
| 29 | AR1660CCC500 | AR1660CCC500 | PP074329.D | 12 Aug 2025 20:41 | | YPAJ | Ok |
| 30 | AR1242CCC500 | AR1242CCC500 | PP074330.D | 12 Aug 2025 21:30 | TCMX high in 2nd column | YPAJ | Ok,M |
| 31 | AR1254CCC500 | AR1254CCC500 | PP074331.D | 12 Aug 2025 21:46 | TCMX high in 2nd column | YPAJ | Ok,M |
| 32 | I.BLK | I.BLK | PP074332.D | 12 Aug 2025 22:02 | | YPAJ | Ok |

M : Manual Integration

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/13/2025

OVENTEMP IN Celsius (°C): 107
Time IN: 17:30
In Date: 08/12/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius (°C): 104
Time OUT: 08:22
Out Date: 08/13/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % solids-oven

QC:LB136783

| Lab ID | Client SampleID | Dish # | Dish Wt(g) (A) | Sample Wt(g) | Dish + Sample Wt(g) (B) | Dish+Dry Sample Wt(g) (C) | % Solid | Comments |
|----------|-----------------|--------|----------------|--------------|-------------------------|---------------------------|---------|----------|
| Q2732-02 | WC-A7-01-C | 74 | 1.15 | 10.37 | 11.52 | 11.18 | 96.7 | |
| Q2819-01 | 22BP-N | 1 | 1.15 | 10.16 | 11.31 | 9.57 | 82.9 | |
| Q2819-02 | 22BP-E | 2 | 1.16 | 10.67 | 11.83 | 10.3 | 85.7 | |
| Q2819-03 | 22BP-W | 3 | 1.16 | 10.83 | 11.99 | 10.45 | 85.8 | |
| Q2819-04 | 22BP-S | 4 | 1.15 | 9.96 | 11.11 | 9.92 | 88.1 | |
| Q2819-05 | 11M-W | 5 | 1.14 | 10.45 | 11.59 | 10.7 | 91.5 | |
| Q2819-06 | 11M-S | 6 | 1.16 | 10.83 | 11.99 | 10.96 | 90.5 | |
| Q2819-07 | 11M-N | 7 | 1.16 | 10.81 | 11.97 | 9.37 | 75.9 | |
| Q2819-08 | 11M-E | 8 | 1.17 | 10.27 | 11.44 | 8.54 | 71.8 | |
| Q2819-09 | 84SB-E | 9 | 1.13 | 10.62 | 11.75 | 5.12 | 37.6 | |
| Q2819-10 | 84SB-S | 10 | 1.18 | 10.11 | 11.29 | 10.51 | 92.3 | |
| Q2819-11 | 84SB-W | 11 | 1.14 | 10.14 | 11.28 | 9.94 | 86.8 | |
| Q2819-12 | 17M-S | 12 | 1.19 | 118.66 | 119.85 | 11.15 | 8.4 | |
| Q2819-13 | 17M-E | 13 | 1.17 | 10.38 | 11.55 | 9.86 | 83.7 | |
| Q2819-14 | 17M-W | 14 | 1.15 | 10.46 | 11.61 | 10.1 | 85.6 | |
| Q2819-15 | 17M-N | 15 | 1.15 | 10.57 | 11.72 | 9.96 | 83.3 | |
| Q2819-16 | 38M-S | 16 | 1.15 | 10.77 | 11.92 | 11.1 | 92.4 | |
| Q2819-17 | 38M-N | 17 | 1.16 | 10.41 | 11.57 | 10.27 | 87.5 | |
| Q2819-18 | 38M-W | 18 | 1.14 | 10.66 | 11.8 | 10.34 | 86.3 | |
| Q2819-19 | 38M-E | 19 | 1.13 | 10.13 | 11.26 | 10.02 | 87.8 | |
| Q2819-20 | 82H-E | 20 | 1.17 | 10.64 | 11.81 | 9.38 | 77.2 | |
| Q2820-01 | 82H-S | 21 | 1.16 | 10.76 | 11.92 | 10.04 | 82.5 | |
| Q2820-02 | 82H-W | 22 | 1.15 | 11.21 | 12.36 | 10.51 | 83.5 | |
| Q2820-03 | 82H-N | 23 | 1.16 | 11.14 | 12.3 | 10.9 | 87.4 | |
| Q2820-04 | SOIL-DUP-1 | 24 | 1.16 | 10.83 | 11.99 | 10.56 | 86.8 | |
| Q2820-05 | 518R-E | 25 | 1.16 | 10.40 | 11.56 | 6.23 | 48.8 | |
| Q2820-06 | 518R-N | 26 | 1.18 | 10.55 | 11.73 | 9.35 | 77.4 | |
| Q2820-07 | 518R-S | 27 | 1.17 | 10.52 | 11.69 | 9.44 | 78.6 | |

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/13/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:30
In Date: 08/12/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:22
Out Date: 08/13/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % solids-oven

QC:LB136783

| Lab ID | Client SampleID | Dish # | Dish Wt(g) (A) | Sample Wt(g) | Dish + Sample Wt(g) (B) | Dish+Dry Sample Wt(g) (C) | % Solid | Comments |
|----------|-----------------|--------|----------------|--------------|-------------------------|---------------------------|---------|----------|
| Q2820-08 | 518R-W | 28 | 1.13 | 10.80 | 11.93 | 10.74 | 89.0 | |
| Q2820-09 | 705R-S | 29 | 1.14 | 10.59 | 11.73 | 7.05 | 55.8 | |
| Q2820-10 | SOIL-DUP-2 | 30 | 1.15 | 10.87 | 12.02 | 6.41 | 48.4 | |
| Q2820-11 | 10PC-W | 31 | 1.11 | 10.25 | 11.36 | 10.58 | 92.4 | |
| Q2820-12 | 10PC-S | 32 | 1.19 | 10.52 | 11.71 | 10.88 | 92.1 | |
| Q2820-13 | 10P-W | 33 | 1.14 | 10.09 | 11.23 | 10.34 | 91.2 | |
| Q2820-14 | 10P-E | 34 | 1.19 | 10.37 | 11.56 | 9.62 | 81.3 | |
| Q2820-15 | 10P-S | 35 | 1.18 | 10.21 | 11.39 | 10.22 | 88.5 | |
| Q2820-16 | 10P-N | 36 | 1.11 | 10.09 | 11.2 | 9.81 | 86.2 | |
| Q2820-17 | 88H-E | 37 | 1.16 | 10.42 | 11.58 | 9.77 | 82.6 | |
| Q2820-18 | 88H-N | 38 | 1.16 | 10.90 | 12.06 | 10.57 | 86.3 | |
| Q2820-19 | 88H-W | 39 | 1.18 | 10.66 | 11.84 | 10.62 | 88.6 | |
| Q2820-20 | 88H-S | 40 | 1.18 | 10.12 | 11.3 | 9.74 | 84.6 | |
| Q2820-21 | 22M-N | 41 | 1.14 | 11.06 | 12.2 | 11.34 | 92.2 | |
| Q2820-22 | 22M-W | 42 | 1.17 | 10.90 | 12.07 | 6.94 | 52.9 | |
| Q2820-23 | 22M-E | 43 | 1.17 | 10.27 | 11.44 | 4.66 | 34.0 | |
| Q2820-24 | 22M-S | 44 | 1.13 | 10.68 | 11.81 | 10.63 | 89.0 | |
| Q2832-01 | TG-S01 | 45 | 1.15 | 10.46 | 11.61 | 10.92 | 93.4 | |
| Q2832-03 | TG-S02 | 46 | 1.18 | 10.41 | 11.59 | 10.97 | 94.0 | |
| Q2832-05 | TG-S03 | 47 | 1.15 | 10.50 | 11.65 | 11.00 | 93.8 | |
| Q2832-07 | TG-S04 | 48 | 1.17 | 10.58 | 11.75 | 11.02 | 93.1 | |
| Q2832-09 | TG-S05 | 49 | 1.15 | 10.40 | 11.55 | 10.6 | 90.9 | |
| Q2836-02 | WC-A2-15-C | 75 | 1.18 | 10.38 | 11.56 | 9.67 | 81.8 | |
| Q2836-06 | WC-A2-16-C | 76 | 1.19 | 10.43 | 11.62 | 10.66 | 90.8 | |
| Q2836-10 | WC-A2-17-C | 77 | 1.19 | 10.48 | 11.67 | 10.96 | 93.2 | |
| Q2836-14 | WC-A5-02-C | 78 | 1.19 | 10.17 | 11.36 | 8.8 | 74.8 | |
| Q2838-01 | TP-11 | 50 | 1.14 | 10.60 | 11.74 | 10.44 | 87.7 | |
| Q2838-02 | TP-11-EPH | 51 | 1.14 | 10.85 | 11.99 | 9.57 | 77.7 | |

PERCENT SOLID

Supervisor: rubina
Analyst: jignesh
Date: 8/13/2025

OVENTEMP IN Celsius(°C): 107
Time IN: 17:30
In Date: 08/12/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
OvenID: M OVEN#1

OVENTEMP OUT Celsius(°C): 104
Time OUT: 08:22
Out Date: 08/13/2025
Weight Check 1.0g: 1.00
Weight Check 10g: 10.00
BalanceID: M SC-4
Thermometer ID: % solids-oven

QC:LB136783

| Lab ID | Client SampleID | Dish # | Dish Wt(g) (A) | Sample Wt(g) | Dish + Sample Wt(g) (B) | Dish+Dry Sample Wt(g) (C) | % Solid | Comments |
|----------|-----------------|--------|----------------|--------------|-------------------------|---------------------------|---------|----------|
| Q2838-03 | TP-11-VOC | 52 | 1.19 | 11.24 | 12.43 | 9.97 | 78.1 | |
| Q2838-05 | TP-10 | 53 | 1.14 | 11.08 | 12.22 | 10.75 | 86.7 | |
| Q2838-06 | TP-10-EPH | 54 | 1.18 | 10.42 | 11.6 | 7.63 | 61.9 | |
| Q2838-07 | TP-10-VOC | 55 | 1.18 | 10.50 | 11.68 | 8.68 | 71.4 | |
| Q2839-01 | BC274436-1-1 | 56 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-02 | BC274436-1-2 | 57 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-03 | BC151973-1-1 | 58 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-04 | BC151973-1-2 | 59 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-05 | BC271336-1-1 | 60 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-06 | BC271336-1-2 | 61 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-07 | BC271242-1-1 | 62 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-08 | BC271242-1-2 | 63 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-09 | BC271242-2-1 | 64 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-10 | BC271242-2-2 | 65 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-11 | BC226751-1-1 | 66 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-12 | BC226751-1-2 | 67 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-13 | BC226751-2-1 | 68 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-14 | BC226751-2-2 | 69 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-15 | JEC773V-1-1 | 70 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2839-16 | JEC773V-1-2 | 71 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | PILC |
| Q2840-01 | 0804-SOIL | 72 | 1.12 | 11.32 | 12.44 | 10.42 | 82.2 | |
| Q2840-02 | 0804-D | 73 | 1.00 | 1.00 | 2.00 | 2.00 | 100.0 | debris |

$$\% \text{ Solid} = \frac{(C-A) * 100}{(B-A)}$$

WORKLIST(Hardcopy Internal Chain)

| WorkList Name : | %1-081225 | WorkList ID : | 191210 | Department : | Wet-Chemistry | Date : | 08-12-2025 07:56:53 |
|-----------------|-----------------|---------------|----------------|--------------|---------------|-----------------------------|-------------------------|
| Sample | Customer Sample | Matrix | Test | Preservative | Customer | Raw Sample Storage Location | Collect Date Method |
| Q2820-06 | 518R-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 Chemtech -SO |
| Q2820-07 | 518R-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 Chemtech -SO |
| Q2820-08 | 518R-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 Chemtech -SO |
| Q2820-09 | 705R-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 Chemtech -SO |
| Q2820-10 | SOIL-DUP-2 | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 Chemtech -SO |
| Q2819-19 | 38M-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 Chemtech -SO |
| Q2819-20 | 82H-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2820-01 | 82H-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2820-02 | 82H-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2820-03 | 82H-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2820-04 | SOIL-DUP-1 | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2819-13 | 17M-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2819-14 | 17M-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2819-15 | 17M-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2819-16 | 38M-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 Chemtech -SO |
| Q2819-17 | 38M-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 Chemtech -SO |
| Q2819-18 | 38M-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2819-07 | 11M-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 Chemtech -SO |
| Q2819-08 | 11M-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/06/2025 Chemtech -SO |
| Q2819-09 | 84SB-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 Chemtech -SO |
| Q2819-10 | 84SB-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 Chemtech -SO |

08/12/15
CJ S

08/12/15
CJ S

Date/Time : 08/12/15
Raw Sample Received by: CJ S

Raw Sample Relinquished by:
CJ S

1135
CJ S

Raw Sample Relinquished by:
CJ S

1135
CJ S

Page 2 of 4
18
19
20

15
16
17
18
19
20

11
12
13

14
15
16

17
18
19

10
11
12

9
8
7

6
5
4

3
2
1

WorkList Name : %1-081225

WorkList ID : 191210

Department : WetChemistry

Date : 08-12-2025 07:56:53

WORKLIST(Hardcopy Internal Chain)

MB 136483

| Sample | Customer Sample | Matrix | Test | Preservative | Customer Location | Raw Sample Storage Location | Collect Date | Method |
|----------|-----------------|--------|----------------|--------------|-------------------|-----------------------------|--------------|--------------|
| Q2819-01 | 22BP-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/04/2025 | Chemtech -SO |
| Q2819-02 | 22BP-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/04/2025 | Chemtech -SO |
| Q2819-03 | 22BP-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/04/2025 | Chemtech -SO |
| Q2819-04 | 22BP-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/04/2025 | Chemtech -SO |
| Q2819-05 | 11M-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/04/2025 | Chemtech -SO |
| Q2819-06 | 11M-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 | Chemtech -SO |
| Q2820-23 | 22M-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 | Chemtech -SO |
| Q2820-24 | 22M-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-17 | 88H-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-18 | 88H-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-19 | 88H-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-20 | 88H-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-21 | 22M-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-22 | 22M-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-11 | 10PC-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/08/2025 | Chemtech -SO |
| Q2820-12 | 10PC-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 | Chemtech -SO |
| Q2820-13 | 10P-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 | Chemtech -SO |
| Q2820-14 | 10P-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 | Chemtech -SO |
| Q2820-15 | 10P-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 | Chemtech -SO |
| Q2820-16 | 10P-N | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 | Chemtech -SO |
| Q2820-05 | 518R-E | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/07/2025 | Chemtech -SO |

Date/Time 08/12/2025, 15:00

Raw Sample Received by: MB 136483

Raw Sample Relinquished by:

Date/Time 08/12/2025, 15:00

Raw Sample Received by: MB 136483

Raw Sample Relinquished by:

WORKLIST(Hardcopy Internal Chain)

WorkList Name : %1-081225

WorkList ID : 191210

Department : Wet-Chemistry

Date : 08-12-2025 07:56:53

| Sample | Customer Sample | Matrix | Test | Preservative | Customer | Raw Sample Storage Location | Collect Date | Method |
|----------|-----------------|--------|----------------|--------------|----------|-----------------------------|--------------|--------------|
| Q2839-04 | BC151973-1-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-05 | BC271336-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-06 | BC271336-1-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-07 | BC271242-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-08 | BC271242-1-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-09 | BC271242-2-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-10 | BC271242-2-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-11 | BC226751-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-12 | BC226751-1-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-13 | BC226751-2-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-14 | BC226751-2-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-15 | JEC773V-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-16 | JEC773V-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2840-01 | 0804-SOIL | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D31 | 08/12/2025 | Chemtech -SO |
| Q2840-02 | 0804-D | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D31 | 08/12/2025 | Chemtech -SO |

Date/Time 08/12/2025 14:35
 Raw Sample Received by: John Doe
 Raw Sample Relinquished by: John Doe

Date/Time 08/12/2025
 Raw Sample Received by:
 Raw Sample Relinquished by:

WORKLIST(Hardcopy Internal Chain)

WorkList Name : %1-081225

WorkList ID : 191210

Department : Wet-Chemistry

Date : 08-12-2025 07:56:53

| Sample | Customer Sample | Matrix | Test | Preservative | Customer Location | Raw Sample Storage Location | Collect Date | Method |
|----------|-----------------|--------|----------------|--------------|-------------------|-----------------------------|--------------|--------------|
| Q2819-11 | 84SB-W | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 | Chemtech -SO |
| Q2819-12 | 17M-S | Solid | Percent Solids | Cool 4 deg C | FIRS02 | D31 | 08/05/2025 | Chemtech -SO |
| Q2832-01 | TG-S01 | Solid | Percent Solids | Cool 4 deg C | PORT06 | J21 | 08/11/2025 | Chemtech -SO |
| Q2732-02 | WC-A7-01-C | Solid | Percent Solids | Cool 4 deg C | ENTA05 | J21 | 08/12/2025 | Chemtech -SO |
| Q2832-03 | TG-S02 | Solid | Percent Solids | Cool 4 deg C | PORT06 | J21 | 08/11/2025 | Chemtech -SO |
| Q2832-05 | TG-S03 | Solid | Percent Solids | Cool 4 deg C | PORT06 | J21 | 08/11/2025 | Chemtech -SO |
| Q2832-07 | TG-S04 | Solid | Percent Solids | Cool 4 deg C | PORT06 | J21 | 08/11/2025 | Chemtech -SO |
| Q2832-09 | TG-S05 | Solid | Percent Solids | Cool 4 deg C | PORT06 | J21 | 08/11/2025 | Chemtech -SO |
| Q2836-02 | WC-A2-15-C | Solid | Percent Solids | Cool 4 deg C | ENTA05 | J23 | 08/12/2025 | Chemtech -SO |
| Q2836-06 | WC-A2-16-C | Solid | Percent Solids | Cool 4 deg C | ENTA05 | J23 | 08/12/2025 | Chemtech -SO |
| Q2836-10 | WC-A2-17-C | Solid | Percent Solids | Cool 4 deg C | ENTA05 | J23 | 08/12/2025 | Chemtech -SO |
| Q2836-14 | WC-A5-02-C | Solid | Percent Solids | Cool 4 deg C | ENTA05 | J23 | 08/12/2025 | Chemtech -SO |
| Q2838-01 | TP-11 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D21 | 08/12/2025 | Chemtech -SO |
| Q2838-02 | TP-11-EPH | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D21 | 08/12/2025 | Chemtech -SO |
| Q2838-03 | TP-11-VOC | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D21 | 08/12/2025 | Chemtech -SO |
| Q2838-05 | TP-10 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D21 | 08/12/2025 | Chemtech -SO |
| Q2838-06 | TP-10-EPH | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D21 | 08/12/2025 | Chemtech -SO |
| Q2838-07 | TP-10-VOC | Solid | Percent Solids | Cool 4 deg C | PSEG03 | D21 | 08/12/2025 | Chemtech -SO |
| Q2839-01 | BC274436-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-02 | BC274436-1-2 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |
| Q2839-03 | BC151973-1-1 | Solid | Percent Solids | Cool 4 deg C | PSEG03 | L11 | 08/12/2025 | Chemtech -SO |

Date/Time 08/12/2025 15:00

Raw Sample Received by: John W C Date/Time 08/12/2025 14:15Raw Sample Relinquished by: John W C

Raw Sample Received by:

John W C

| | | | |
|--------------------|---|-------------------------|------------|
| SOP ID: | M3541-ASE Extraction-15 | | |
| Clean Up SOP #: | Acid Cleanup | Extraction Start Date : | 08/12/2025 |
| Matrix : | Solid | Extraction Start Time : | 08:15 |
| Weigh By: | RJ | Extraction End Date : | 08/12/2025 |
| Balance check: | RJ | Extraction End Time : | 11:30 |
| Balance ID: | EX-SC-2 | pH Meter ID: | N/A |
| pH Strip Lot#: | N/A | Hood ID: | 3,7 |
| Extraction Method: | <input type="checkbox"/> Separatory Funnel <input type="checkbox"/> Continous Liquid/Liquid <input type="checkbox"/> Sonication <input type="checkbox"/> Waste Dilution <input checked="" type="checkbox"/> Soxhlet | | |

| Standardized Name | MLS USED | Concentration ug/mL | STD REF. # FROM LOG |
|-------------------|----------|---------------------|---------------------|
| Spike Sol 1 | 1.0ML | 5000 PPB | PP24650 |
| Surrogate | 1.0ML | 200 PPB | PP24663 |
| N/A | N/A | N/A | N/A |
| N/A | N/A | N/A | N/A |
| N/A | N/A | N/A | N/A |

| Chemical Used | ML/SAMPLE USED | Lot Number |
|--------------------|----------------|------------|
| Hexane/Acetone/1:1 | N/A | EP2627 |
| Baked Na2SO4 | N/A | EP2632 |
| Sand | N/A | E3951 |
| Hexane | N/A | E3962 |
| H2SO4 1:1 | N/A | EP2610 |
| N/A | N/A | N/A |

Extraction Conformance/Non-Conformance Comments:

40ML Vial Lot # 03-40BTS721.

KD Bath ID: N/A Envap ID: NEVAP-02
KD Bath Temperature: N/A Envap Temperature: 40 °C

| Date / Time | Prepped Sample Relinquished By/Location | Received By/Location |
|-------------|---|----------------------|
| 8/12/25 | RJ (Ext Lab) | Y. P. Pest/PCB |
| 11:35 | Preparation Group | Analysis Group |

Analytical Method: N/A

Concentration Date: 08/12/2025

| Sample ID | Client Sample ID | Test | g/mL | PH | Surr/Spike By: | | Final Vol. (mL) | JarID | Comments | Prep Pos |
|-----------------|---------------------------------------|------|-------|-----|----------------|------------|-----------------|-------|----------------|----------|
| | | | | | AddedBy | VerifiedBy | | | | |
| PB169205BL | ABLK205 | PCB | 30.03 | N/A | ritesh | RUPESH | 10 | | | U1-1 |
| PB169205BS | ALCS205 | PCB | 30.01 | N/A | ritesh | RUPESH | 10 | | | 2 |
| Q2818-01 | B-2-5-1 | PCB | 30.07 | N/A | ritesh | RUPESH | 10 | B | | 3 |
| Q2818-02 | B-3-5-2 | PCB | 30.03 | N/A | ritesh | RUPESH | 10 | B | | 4 |
| Q2819-06 | 11M-S | PCB | 30.05 | N/A | ritesh | RUPESH | 10 | E | | 5 |
| Q2819-11 | 84SB-W | PCB | 30.02 | N/A | ritesh | RUPESH | 10 | E | | 6 |
| Q2819-14 | 17M-W | PCB | 30.08 | N/A | ritesh | RUPESH | 10 | E | | U2-1 |
| Q2820-09 | 705R-S | PCB | 30.06 | N/A | ritesh | RUPESH | 10 | E | | 2 |
| Q2820-10 | SOIL-DUP-2 | PCB | 30.09 | N/A | ritesh | RUPESH | 10 | E | | 3 |
| Q2820-24 | 22M-S | PCB | 30.01 | N/A | ritesh | RUPESH | 10 | E | | 4 |
| Q2823-01 | SU-04-081125 | PCB | 30.04 | N/A | ritesh | RUPESH | 10 | E | | 5 |
| Q2826-01 | WC1 | PCB | 30.08 | N/A | ritesh | RUPESH | 10 | | | 6 |
| Q2827-01 | TP-8 | PCB | 30.07 | N/A | ritesh | RUPESH | 10 | E | | U3-1 |
| Q2827-05 | TP-9 | PCB | 30.02 | N/A | ritesh | RUPESH | 10 | E | Gasoline Smell | 2 |
| Q2830-01 | BIN0009-DRIVEWAY-TP-S OUTH-EAST | PCB | 30.06 | N/A | ritesh | RUPESH | 10 | E | | 3 |
| Q2830-01MS | BIN0009-DRIVEWAY-TP-S OUTH-EASTMS | PCB | 30.01 | N/A | ritesh | RUPESH | 10 | E | | 4 |
| Q2830-01MS D | BIN0009-DRIVEWAY-TP-S OUTH-EASTMSD | PCB | 30.03 | N/A | ritesh | RUPESH | 10 | E | | 5 |
| Q2830-03 | BIN0009-DRIVEWAY-TP- WEST | PCB | 30.09 | N/A | ritesh | RUPESH | 10 | E | | 6 |
| Q2830-05 | BIN0009-DRIVEWAY-TP- WESTSIDE | PCB | 30.06 | N/A | ritesh | RUPESH | 10 | E | | U6-1 |
| Q2830-07 | BIN0009-DRIVEWAY-TP-E ASTSIDE | PCB | 30.04 | N/A | ritesh | RUPESH | 10 | E | | 2 |
| Q2831-01 | VNJ-238 | PCB | 30.08 | N/A | ritesh | RUPESH | 10 | B | | 3 |

RJ
8/12

* Extracts relinquished on the same date as received.

WORKLIST(Hardcopy Internal Chain)

| WorkList Name : | Q2818 | WorkList ID : | 191213 | Department : | Extraction | Raw Sample Storage Location | Collect Date | Date : |
|-----------------|---------------------------|---------------|--------|--------------|------------|-----------------------------|--------------|---------------------|
| Sample | Customer Sample | Matrix | Test | Preservative | Customer | | | 08-12-2025 08:10:04 |
| | | | | | | | | |
| Q2818-01 | B-2-5-1 | Solid | PCB | Cool 4 deg C | EARTH03 | 08/11/2025 | 8082A | |
| Q2818-02 | B-3-5-2 | Solid | PCB | Cool 4 deg C | EARTH03 | 08/11/2025 | 8082A | |
| Q2819-06 | 11M-S | Solid | PCB | Cool 4 deg C | FIRSO2 | D31 | 08/05/2025 | 8082A |
| Q2819-11 | 84SB-V | Solid | PCB | Cool 4 deg C | FIRSO2 | D31 | 08/05/2025 | 8082A |
| Q2819-14 | 17M-W | Solid | PCB | Cool 4 deg C | FIRSO2 | D31 | 08/05/2025 | 8082A |
| Q2820-09 | 705R-S | Solid | PCB | Cool 4 deg C | FIRSO2 | D31 | 08/07/2025 | 8082A |
| Q2820-10 | SOIL-DUP-2 | Solid | PCB | Cool 4 deg C | FIRSO2 | D31 | 08/07/2025 | 8082A |
| Q2820-24 | 22M-S | Solid | PCB | Cool 4 deg C | FIRSO2 | D31 | 08/08/2025 | 8082A |
| Q2823-01 | SU-04-081125 | Solid | PCB | Cool 4 deg C | PSEG05 | D31 | 08/11/2025 | 8082A |
| Q2826-01 | WC1 | Solid | PCB | Cool 4 deg C | GENV01 | D31 | 08/11/2025 | 8082A |
| Q2827-01 | TP-8 | Solid | PCB | Cool 4 deg C | PSEG03 | D31 | 08/11/2025 | 8082A |
| Q2827-05 | TP-9 | Solid | PCB | Cool 4 deg C | PSEG03 | D31 | 08/11/2025 | 8082A |
| Q2830-01 | BIN009-DRIVEWAY-TP-SOUTH | Solid | PCB | Cool 4 deg C | PSEG03 | D31 | 08/11/2025 | 8082A |
| Q2830-03 | BIN009-DRIVEWAY-TP-WEST | Solid | PCB | Cool 4 deg C | PSEG03 | D31 | 08/11/2025 | 8082A |
| Q2830-05 | BIN009-DRIVEWAY-TP-WEST | Solid | PCB | Cool 4 deg C | PSEG03 | D31 | 08/11/2025 | 8082A |
| Q2830-07 | BIN009-DRIVEWAY-TP-EAST'S | Solid | PCB | Cool 4 deg C | PSEG03 | D31 | 08/11/2025 | 8082A |
| Q2831-01 | VNJ-238 | Solid | PCB | Cool 4 deg C | PSEG03 | D21 | 08/11/2025 | 8082A |

Date/Time 08/11/2025 08:10
 Raw Sample Received by: RJ C (EPA - 126)
 Raw Sample Relinquished by: CR S

Date/Time

Raw Sample Received by:

Raw Sample Relinquished by:

08/11/2025 08:10
RJ C (EPA - 126)

Page 1 of 1

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Prep Standard - Chemical Standard Summary

Order ID : Q2819

Test : PCB

Prepbatch ID : PB169205,

Sequence ID/Qc Batch ID: PO081225,PP081225,

Standard ID :

EP2610,EP2627,EP2632,PP24329,PP24330,PP24331,PP24332,PP24333,PP24334,PP24335,PP24336,PP24337,PP24338,PP24339,PP24340,PP24341,PP24342,PP24343,PP24344,PP24345,PP24346,PP24347,PP24348,PP24349,PP24350,PP24351,PP24352,PP24353,PP24354,PP24355,PP24356,PP24357,PP24358,PP24359,PP24360,PP24361,PP24362,PP24363,PP24364,PP24365,PP24366,PP24367,PP24368,PP24369,PP24370,PP24371,PP24372,PP24373,PP24374,PP24375,PP24376,PP24377,PP24378,PP24379,PP24380,PP24381,PP24382,PP24384,PP24385,PP24386,PP24387,PP24650,PP24663,

Chemical ID :

E3804,E3875,E3877,E3940,E3944,E3949,E3950,E3951,E3962,M6157,P11522,P12699,P12702,P12931,P12936,P12949,P12950,P12957,P13356,P13373,P13381,P13589,P13591,P13697,P13702,P13786,P13830,P13878,P13883,W3112,W3177,

Extractions STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------|------------------------|------------------|------------------------|--------------------|----------------------------------|------------------|---------------------------------|
| 314 | 1.1 H2SO4 SOLN | EP2610 | 05/07/2025 | 11/07/2025 | RUPESHKUMA R SHAH | Extraction_SC ALE_2 (EX-SC-2) | None | Riteshkumar Patel 05/07/2025 |

FROM 1000.00000ml of M6157 + 1000.00000ml of W3112 = Final Quantity: 2000.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------------|
| 230 | 1:1ACETONE/HEXANE | EP2627 | 07/15/2025 | 01/15/2026 | RUPESHKUMA R SHAH | None | None | Riteshkumar Patel 07/15/2025 |

FROM 4000.00000ml of E3949 + 4000.00000ml of E3950 = Final Quantity: 8000.000 ml

Extractions STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------|------------------------|------------------|------------------------|--------------------|----------------------------------|------------------|---------------------------------|
| 3923 | Baked Sodium Sulfate | EP2632 | 08/11/2025 | 01/28/2026 | RUPESHKUMA R SHAH | Extraction_SC ALE_2 (EX-SC-2) | None | Riteshkumar Patel 08/11/2025 |

FROM 4000.00000gram of E3875 = Final Quantity: 4000.000 gram

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 84 | Pest/PCB Surrogate Stock 20 PPM | PP24329 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P13356 + 9.00000ml of W3177 = Final Quantity: 10.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 202 | AR1660 1000/100 ppb working solution 1st source | PP24330 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P13697 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 203 | AR1660 750 PPB STD | PP24331 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 204 | AR1660 500 PPB STD | PP24332 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24330 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 205 | AR1660 250 PPB STD | PP24333 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24330 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 206 | AR1660 50 PPB STD | PP24334 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24332 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 213 | AR1221 1000 PPB WORKING SOLUTION | PP24335 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P13702 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1079 | AR1221 750 PPB STD | PP24336 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24335 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 222 | AR1221 500 PPB STD | PP24337 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24335 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1080 | AR1221 250 PPB STD | PP24338 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24335 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1081 | AR1221 50 PPB STD | PP24339 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24337 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 214 | AR1232 1000 PPB WORKING SOLUTION | PP24340 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P13878 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1063 | AR1232 750 PPB STD | PP24341 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 223 | AR1232 500 PPB STD | PP24342 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24340 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1064 | AR1232 250 PPB STD | PP24343 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24340 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1065 | AR1232 50 PPB STD | PP24344 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24342 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 215 | AR1242 1000 PPB WORKING STD | PP24345 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P12931 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1067 | AR1242 750 PPB STD | PP24346 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.75000ml of PP24345 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 224 | AR1242 500 PPB STD | PP24347 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24345 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1068 | AR1242 250 PPB STD | PP24348 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24345 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1069 | AR1242 50 PPB STD | PP24349 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24347 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 216 | AR1248 1000 PPB WORKING STD | PP24350 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P12936 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1075 | AR1248 750 PPB STD | PP24351 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 225 | AR1248 500 PPB STD | PP24352 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24350 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1076 | AR1248 250 PPB STD | PP24353 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24350 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1077 | AR1248 50 PPB STD | PP24354 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24352 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 217 | AR1254 1000 PPB WORKING STD | PP24355 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P13830 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1071 | AR1254 750 PPB STD | PP24356 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24355 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 226 | AR1254 500 PPB STD | PP24357 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24355 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1072 | AR1254 250 PPB STD | PP24358 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24355 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1073 | AR1254 50 PPB STD | PP24359 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24357 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1529 | AR1262 1000 PPB Working Solution | PP24360 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P13883 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3753 | AR1262 750 PPB STD | PP24361 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1530 | AR1262 500 PPB STD | PP24362 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24360 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3754 | AR1262 250 PPB STD | PP24363 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24360 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3755 | AR1262 50 PPB STD | PP24364 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24362 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1532 | AR1268 1000 PPB Working Solution | PP24365 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.10000ml of P13381 + 99.40000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3820 | AR1268 750 PPB STD | PP24366 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.25000ml of W3177 + 0.75000ml of PP24365 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1533 | AR1268 500 PPB STD | PP24367 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24365 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3821 | AR1268 250 PPB STD | PP24368 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.75000ml of W3177 + 0.25000ml of PP24365 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3822 | AR1268 50 PPB STD | PP24369 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.90000ml of W3177 + 0.10000ml of PP24367 = Final Quantity: 1.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 404 | AR1660 100 PPM Stock Solution 2nd Source | PP24370 | 03/18/2025 | 09/18/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P12949 + 9.00000ml of E3804 = Final Quantity: 10.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|-----------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 405 | AR1660 1000/100 PPB ICV STD | PP24371 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 98.50000ml of W3177 + 0.50000ml of PP24329 + 1.00000ml of PP24370 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 406 | AR1660 500 PPB ICV | PP24372 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24371 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3789 | AR1221 1000 PPB WORKING SOL.2ND SOURCE(AGILENT) | PP24373 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P13373 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1886 | AR1221 500 PPB ICV | PP24374 | 03/18/2025 | 08/12/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of E3877 + 0.50000ml of W3177 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1887 | AR1232 1000 PPB Working Sol. 2nd Source | PP24375 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P12699 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1888 | AR1232 500 PPB ICV | PP24376 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24375 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1889 | AR1242 1000 PPB Working Sol. 2nd Source | PP24377 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P13589 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1891 | AR1242 500 PPB ICV | PP24378 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24377 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1890 | AR1248 1000 PPB Working Sol. 2nd Source | PP24379 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P13591 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1892 | AR1248 500 PPB ICV | PP24380 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24379 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1893 | AR1254 1000 PPB Working Sol. 2nd Source | PP24381 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P12957 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 1894 | AR1254 500 PPB ICV | PP24382 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24381 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3757 | AR1262 1000 PPB Working Solution second source | PP24384 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P12702 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3758 | AR1262 500 PPB STD ICV | PP24385 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24384 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|---|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3817 | AR1268 1000 ppb Working Soln. 2nd source | PP24386 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 1.00000ml of P11522 + 98.50000ml of W3177 + 0.50000ml of PP24329 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|---------------------------|
| 3823 | AR1268 500 PPB STD ICV | PP24387 | 03/18/2025 | 08/22/2025 | Yogesh Patel | None | None | Abdul Mirza 04/03/2025 |

FROM 0.50000ml of W3177 + 0.50000ml of PP24386 = Final Quantity: 1.000 ml

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|--|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------------|
| 3857 | 5000 PPB PCB SPIKE SOLUTION 2ND SOURCE | PP24650 | 06/16/2025 | 12/11/2025 | Abdul Mirza | None | None | Yogesh Patel 07/21/2025 |

FROM 0.50000ml of P12950 + 99.50000ml of E3940 = Final Quantity: 100.000 ml

Pest/Pcb STANDARD PREPARATION LOG

| <u>Recipe ID</u> | <u>NAME</u> | <u>NO.</u> | <u>Prep Date</u> | <u>Expiration Date</u> | <u>Prepared By</u> | <u>ScaleID</u> | <u>PipetteID</u> | <u>Supervised By</u> |
|------------------|----------------------------------|-------------------------|------------------|------------------------|--------------------|----------------|------------------|----------------------------|
| 465 | 200 PPB Pest/PCB Surrogate Spike | PP24663 | 06/24/2025 | 12/24/2025 | Abdul Mirza | None | None | Yogesh Patel 07/21/2025 |

FROM 1.00000ml of P13786 + 999.00000ml of E3944 = Final Quantity: 1000.000 ml

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|-----------------------------|--|--------------|------------------------|--------------------------------|------------------------------------|-----------------------|
| Seidler Chemical | 9005-05 / Acetone Ultra (cs/4x4L) | 24E0761004 | 11/05/2025 | 10/01/2024 / Rajesh | 09/25/2024 / Rajesh | E3804 |
| PCI Scientific Supply, Inc. | PC19631-100 / SODIUM SULFATE, ANHYDROUS, PEST GRADE, 1 | 417203 | 01/28/2026 | 07/28/2025 / RUPESH | 01/29/2025 / Rajesh | E3875 |
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 243570 | 08/12/2025 | 02/12/2025 / Rajesh | 02/12/2025 / Rajesh | E3877 |
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H1462005 | 12/11/2025 | 06/11/2025 / Rajesh | 06/04/2025 / Rajesh | E3940 |
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H1462005 | 05/24/2027 | 06/20/2025 / RUPESH | 05/14/2025 / RUPESH | E3944 |
| Seidler Chemical | BA-9254-03 / Acetone, Ultra Resi (cs/4x4L) | 24H2762008 | 04/18/2027 | 07/08/2025 / RITESHKUMAR | 07/03/2025 / RUPESH | E3949 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------------|---|------------|-----------------|--------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362005 | 04/30/2026 | 07/08/2025 / RITESHKUMAR | 07/03/2025 / RUPESH | E3950 |
| Seidler Chemical | BA-3382-05 / Sand, Purified (cs/4x2.5kg) | 25A2756718 | 12/31/2028 | 07/09/2025 / RUPESH | 04/28/2020 / RUPESH | E3951 |
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 25C0362005 | 04/30/2026 | 08/05/2025 / RUPESH | 07/30/2025 / RUPESH | E3962 |
| Seidler Chemical | BA-9673-33 / Sulfuric Acid, Instra-Analyzed (cs/6c2.5L) | 24i1262013 | 11/07/2025 | 05/07/2025 / RUPESH | 02/18/2025 / Mohan | M6157 |
| Agilent Technologies | PP-382-1 / Aroclor 1268 | 0006587800 | 09/18/2025 | 03/18/2025 / yogesh | 02/21/2022 / Ankita | P11522 |
| Absolute Standards,Inc | 91867 / Aroclor 1232 100 ug/mL | 020823 | 09/18/2025 | 03/18/2025 / yogesh | 08/07/2023 / Ankita | P12699 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|--------------------------|---|----------|-----------------|-------------------------|-----------------------------|----------------|
| Absolute Standards, Inc. | x9166 / Aroclor 1262 100 ug/mL | 060523 | 09/18/2025 | 03/18/2025 / yogesh | 08/07/2023 / Ankita | P12702 |
| Restek | 32009 / PCB Mix, Aroclor 1242, 1000ug/mL, Hexane, 1mL/ampul | a0203672 | 09/18/2025 | 03/18/2025 / yogesh | 12/07/2023 / Ankita | P12931 |
| Restek | 32010 / PCB Mix, Aroclor 1248, 1000ug/mL, Hexane, 1mL/ampul | a0202803 | 09/18/2025 | 03/18/2025 / yogesh | 12/07/2023 / Ankita | P12936 |
| Absolute Standards, Inc. | 20064 / Aroclor 1016/1260 | 022023 | 09/18/2025 | 03/18/2025 / yogesh | 12/20/2023 / Yogesh | P12949 |
| Absolute Standards, Inc. | 20064 / Aroclor 1016/1260 | 022023 | 12/16/2025 | 06/16/2025 / Abdul | 12/20/2023 / Yogesh | P12950 |
| Absolute Standards, Inc. | / Arochlor 1254 | 121823 | 04/03/2025 | 10/03/2024 / Ankita | 12/20/2023 / Yogesh | P12957 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|----------------------|--|------------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL | A0206810 | 09/18/2025 | 03/18/2025 / yogesh | 04/22/2024 / Abdul | P13356 |
| Agilent Technologies | PP-292-1 / Aroclor 1221 | 0006783205 | 09/18/2025 | 03/18/2025 / yogesh | 05/02/2024 / Ankita | P13373 |
| Restek | 32410 / PCB Stock Solution, Aroclor 1268 Std, 1mL, Hexane | A0207475 | 09/18/2025 | 03/18/2025 / yogesh | 05/03/2024 / Abdul | P13381 |
| Agilent Technologies | PP-312-1 / Aroclor 1242 | 0006665550 | 09/18/2025 | 03/18/2025 / yogesh | 10/14/2024 / Ankita | P13589 |
| Agilent Technologies | PP-342-1 / Aroclor 1248 | 0006726317 | 09/18/2025 | 03/18/2025 / yogesh | 10/14/2024 / Ankita | P13591 |
| Restek | 32039 / PCB Mix, Aroclor 1016/1260, 1000ug/mL, hexane, 1mL/ampul | A0210629 | 09/18/2025 | 03/18/2025 / yogesh | 10/17/2024 / yogesh | P13697 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|--|---------------------|-----------------|-------------------------|-----------------------------|----------------|
| Restek | 32007 / PCB Mix, Aroclor 1221, 1000ug/mL, Hexane, 1mL/ampul | A0215270 | 09/18/2025 | 03/18/2025 / yogesh | 10/17/2024 / yogesh | P13702 |
| Restek | 32000 / Pesticide Mix, CLP method, Pesticide Surrogate Mix, 200ug/mL, Acetone, 1mL | A0214495 | 12/24/2025 | 06/24/2025 / Abdul | 11/19/2024 / Ankita | P13786 |
| Restek | 32011 / PCB Mix, Aroclor 1254, 1000ug/mL, Hexane, 1mL/ampul | A0217391 | 09/18/2025 | 03/18/2025 / yogesh | 12/09/2024 / Ankita | P13830 |
| Restek | 32008 / PCB Mix, Aroclor 1232, 1000ug/mL, Hexane, 1mL/ampul | A0219655 | 09/18/2025 | 03/18/2025 / yogesh | 01/23/2025 / Ankita | P13878 |
| Restek | 32409 / PCB Stock Solution, Aroclor 1262 Std, 1mL, Hexane | A0220950 | 09/18/2025 | 03/18/2025 / yogesh | 01/23/2025 / Ankita | P13883 |
| Seidler Chemical | DIW / DI Water | Daily Lab-Certified | 07/03/2029 | 07/03/2024 / Iwona | 07/03/2024 / Iwona | W3112 |

CHEMICAL RECEIPT LOG BOOK

| Supplier | ItemCode / ItemName | Lot # | Expiration Date | Date Opened / Opened By | Received Date / Received By | Chemtech Lot # |
|------------------|---|------------|-----------------|-------------------------|-----------------------------|----------------|
| Seidler Chemical | BA-9262-03 / Hexane, Ultra-Resi (cs/4x4L) | 24G1962003 | 08/22/2025 | 02/03/2025 / jignesh | 01/31/2025 / jignesh | W3177 |

 1
 2
 3
 4
 5
 6
 7
 8
 9
 10
 11
 12
 13
 14
 15
 16
 17
 18
 19
 20

Material No.: 9005-05
Batch No.: 24E0761004
Manufactured Date: 2024-05-02
Retest Date: 2029-05-01
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | ≥ 99.5 % | 99.8 % |
| Color (APHA) | ≤ 10 | < 5 |
| Residue after Evaporation | ≤ 5 ppm | < 1 ppm |
| Titrable Acid (μeq/g) | ≤ 0.3 | 0.1 |
| Titrable Base (μeq/g) | ≤ 0.5 | 0.1 |
| Water (H ₂ O) | ≤ 0.5 % | 0.1 % |
| Solubility in H ₂ O | Passes Test | Passes Test |
| Chloride (Cl) | ≤ 0.2 ppm | < 0.2 ppm |
| Phosphate (PO ₄) | ≤ 0.05 ppm | < 0.05 ppm |
| Trace Impurities – Aluminum (Al) | ≤ 50.0 ppb | < 5.0 ppb |
| Arsenic and Antimony (as As) | ≤ 5.0 ppb | < 5.0 ppb |
| Trace Impurities – Barium (Ba) | ≤ 20.0 ppb | < 1.0 ppb |
| Trace Impurities – Beryllium (Be) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Bismuth (Bi) | ≤ 20.0 ppb | < 10.0 ppb |
| Trace Impurities – Boron (B) | ≤ 10.0 ppb | < 5.0 ppb |
| Trace Impurities – Cadmium (Cd) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Calcium (Ca) | ≤ 25.0 ppb | 3.6 ppb |
| Trace Impurities – Chromium (Cr) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Cobalt (Co) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Copper (Cu) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Gallium (Ga) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Germanium (Ge) | ≤ 10.0 ppb | < 10.0 ppb |
| Trace Impurities – Gold (Au) | ≤ 20 ppb | < 5 ppb |
| Trace Impurities – Iron (Fe) | ≤ 20.0 ppb | < 1.0 ppb |
| Trace Impurities – Lead (Pb) | ≤ 10.0 ppb | < 10.0 ppb |
| Trace Impurities – Lithium (Li) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Magnesium (Mg) | ≤ 20 ppb | < 1 ppb |
| Trace Impurities – Manganese (Mn) | ≤ 10.0 ppb | < 1.0 ppb |

Recd by RP on 9/25/24

E 3804

>>> Continued on page 2 >>>

Acetone
CMOS



Material No.: 9005-05
Batch No.: 24E0761004

| Test | Specification | Result |
|---|---------------|------------|
| Trace Impurities – Molybdenum (Mo) | ≤ 10.0 ppb | < 5.0 ppb |
| Trace Impurities – Nickel (Ni) | ≤ 10.0 ppb | < 5.0 ppb |
| Trace Impurities – Niobium (Nb) | ≤ 50.0 ppb | < 1.0 ppb |
| Trace Impurities – Potassium (K) | ≤ 10.0 ppb | < 10.0 ppb |
| Trace Impurities – Silicon (Si) | ≤ 50 ppb | < 10 ppb |
| Trace Impurities – Silver (Ag) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Sodium (Na) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Strontium (Sr) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Tantalum (Ta) | ≤ 50.0 ppb | < 5.0 ppb |
| Trace Impurities – Thallium (Tl) | ≤ 10.0 ppb | < 5.0 ppb |
| Trace Impurities – Tin (Sn) | ≤ 20.0 ppb | < 10.0 ppb |
| Trace Impurities – Titanium (Ti) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Vanadium (V) | ≤ 10.0 ppb | < 1.0 ppb |
| Trace Impurities – Zinc (Zn) | ≤ 20.0 ppb | 7.9 ppb |
| Trace Impurities – Zirconium (Zr) | ≤ 10.0 ppb | < 1.0 ppb |
| Particle Count – 0.5 µm and greater (Rion KS42AF) | ≤ 100 par/ml | 8 par/ml |
| Particle Count – 1.0 µm and greater (Rion KS42AF) | ≤ 8 par/ml | 2 par/ml |

>>> Continued on page 3 >>>

Acetone CMOS



Material No.: 9005-05
Batch No.: 24E0761004

For Microelectronic Use

**Country of Origin: USA
Packaging Site: Paris Mfg Ctr & DC**

Michelle Bales
Michelle Bales
Sr. Manager, Quality Assurance



PRODUCTOS
QUÍMICOS
MONTERREY, S.A. DE C.V.

MIRADOR 201, COL. MIRADOR
MONTERREY, N.L. MÉXICO
CP 64070
TEL +52 81 13 52 57 57
www.pqm.com.mx

CERTIFICATE OF ANALYSIS

| | | | |
|-----------------------|-----------------------------------|---------------|---------------------------------|
| PRODUCT : | SODIUM SULFATE CRYSTALS ANHYDROUS | | |
| QUALITY : | ACS (CODE RMB3375) | FORMULA : | Na ₂ SO ₄ |
| SPECIFICATION NUMBER: | 6399 | RELEASE DATE: | MAY/23/2024 |
| LOT NUMBER : | 417203 | | |

| TEST | SPECIFICATIONS | LOT VALUES |
|--|----------------|-------------|
| Assay (Na ₂ SO ₄) | Min. 99.0% | 99.8 % |
| pH of a 5% solution at 25°C | 5.2 - 9.2 | 6.2 |
| Insoluble matter | Max. 0.01% | 0.001 % |
| Loss on ignition | Max. 0.5% | 0.1 % |
| Chloride (Cl) | Max. 0.001% | <0.001 % |
| Nitrogen compounds (as N) | Max. 5 ppm | <5 ppm |
| Phosphate (PO ₄) | Max. 0.001% | <0.001 % |
| Heavy metals (as Pb) | Max. 5 ppm | <5 ppm |
| Iron (Fe) | Max. 0.001% | <0.001 % |
| Calcium (Ca) | Max. 0.01% | 0.001 % |
| Magnesium (Mg) | Max. 0.005% | 0.001 % |
| Potassium (K) | Max. 0.008% | 0.001 % |
| Extraction-concentration suitability | Passes test | Passes test |
| Appearance | Passes test | Passes test |
| Identification | Passes test | Passes test |
| Solubility and foreign matter | Passes test | Passes test |
| Retained on US Standard No. 10 sieve | Max. 1% | 0.2 % |
| Retained on US Standard No. 60 sieve | Min. 94% | 96.2 % |
| Through US Standard No. 60 sieve | Max. 5% | 3.5 % |
| Through US Standard No. 100 sieve | Max. 10% | 0.1 % |
| COMMENTS | | |
| | | |
| QC: PhC Irma Belmares | | |

If you need further details, please call our factory or contact our local distributor.

RE-02-01, Ed. 3

E 3875



Certificate of Analysis

1 Reagent Lane
Fair Lawn, NJ 07410
201.796.7100 tel
201.796.1329 fax

Thermo Fisher Scientific's Quality System has been found to conform to Quality Management System Standard ISO9001:2015 by SAI Global Certificate Number CERT – 0120633

This is to certify that units of the lot number below were tested and found to comply with the specifications of the grade listed. Certain data have been supplied by third parties. Thermo Fisher Scientific expressly disclaims all warranties, expressed or implied, including the implied warranties of merchantability and fitness for a particular purpose. Products are for research use or further manufacturing. Not for direct administration to humans or animals. It is the responsibility of the final formulator and end user to determine suitability based upon the intended use of the end product. Products are tested to meet the analytical requirements of the noted grade. The following information is the actual analytical results obtained.

| | | | |
|-------------------|---|-----------------------------|------------|
| Catalog Number | H303 | Quality Test / Release Date | 11/07/2024 |
| Lot Number | 243570 | | |
| Description | HEXANES - OPTIMA | | |
| Country of Origin | United States | Suggested Retest Date | Nov/2029 |
| Chemical Origin | Organic - non animal | | |
| BSE/TSE Comment | No animal products are used as starting raw material ingredients, or used in processing, including lubricants, processing aids, or any other material that might migrate to the finished product. | | |

N/A

| Result Name | Units | Specifications | Test Value |
|-----------------------------|------------|---------------------------------|-------------------------|
| APPEARANCE | | REPORT | Clear, colorless liquid |
| ASSAY (N-HEXANE) | % | >= 60 | 69 |
| ASSAY (SUM C6 HYDROCARBONS) | % | >= 99.9 | >99.9 |
| COLOR | APHA | <= 5 | <5 |
| DENSITY AT 25 DEGREES C | GM/ML | Inclusive Between 0.653 - 0.673 | 0.669 |
| EVAPORATION RESIDUE | ppm | <= 1 | <1 |
| FLUORESCENCE BACKGROUND | ppb | <= 1 | <1 |
| IDENTIFICATION | PASS/FAIL | = PASS TEST | PASS TEST |
| OPTICAL ABS AT 195 NM | ABS. UNITS | <= 1 | 0.74 |
| OPTICAL ABS AT 210 NM | ABS. UNITS | <= 0.25 | 0.17 |
| OPTICAL ABS AT 220 NM | ABS. UNITS | <= 0.07 | 0.05 |
| OPTICAL ABS AT 254 NM | ABS. UNITS | <= 0.005 | 0.001 |
| PESTICIDE RESIDUE ANALYSIS | NG/L | <= 10 | <10 |
| REFRACTIVE INDEX @ 25 DEG C | | Inclusive Between 1.375 - 1.385 | 1.379 |
| SUITABILITY FOR GC/MS | | = PASS TEST | PASS TEST |
| SULFUR COMPOUNDS | % | <= 0.005 | <0.005 |
| THIOPHENE | PASS/FAIL | = PASS TEST | PASS TEST |
| WATER (H2O) | % | <= 0.01 | <0.01 |
| WATER-SOLUBLE TITRABLE ACID | MEQ/G | <= 0.0003 | 0.0001 |

Recd - by RP on 2/12/25

 [E3877]

Harout Sahagian - Quality Control Manager - Fair Lawn

Note: The data listed is valid for all package sizes of this lot of this product, expressed as an extension of this catalog number listed above.

If there are any questions with this certificate, please call at (800) 227-6701.

*Based on suggested storage condition.

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | >= 99.4 % | 99.8 % |
| Color (APHA) | <= 10 | 5 |
| Residue after Evaporation | <= 1.0 ppm | 0.2 ppm |
| Substances Reducing Permanganate | Passes Test | Passes Test |
| Titrable Acid (μeq/g) | <= 0.3 | 0.2 |
| Titrable Base (μeq/g) | <= 0.6 | <0.1 |
| Water (H ₂ O) | <= 0.5 % | 0.2 % |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | <1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | <= 10 | 1 |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Recd by RP on 6/11/25

E3940

A handwritten signature in black ink that appears to read "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H1462005

Manufactured Date: 2024-05-24

Expiration Date: 2027-05-24

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | >= 99.4 % | 99.8 % |
| Color (APHA) | <= 10 | 5 |
| Residue after Evaporation | <= 1.0 ppm | 0.2 ppm |
| Substances Reducing Permanganate | Passes Test | Passes Test |
| Titrable Acid (μeq/g) | <= 0.3 | 0.2 |
| Titrable Base (μeq/g) | <= 0.6 | <0.1 |
| Water (H ₂ O) | <= 0.5 % | 0.2 % |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | <1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | <= 10 | 1 |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

E3944

A handwritten signature of the name 'Jamie Croak'.

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Acetone

BAKER RESI-ANALYZED® Reagent
For Organic Residue Analysis



Material No.: 9254-03

Batch No.: 24H2762008

Manufactured Date: 2024-04-18

Expiration Date: 2027-04-18

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| Assay ((CH ₃) ₂ CO) (by GC, corrected for water) | >= 99.4 % | 100.0 % |
| Color (APHA) | <= 10 | 5 |
| Residue after Evaporation | <= 1.0 ppm | 0.0 ppm |
| Substances Reducing Permanganate | Passes Test | Passes Test |
| Titrable Acid (μeq/g) | <= 0.3 | 0.2 |
| Titrable Base (μeq/g) | <= 0.6 | <0.1 |
| Water (H ₂ O) | <= 0.5 % | <0.1 % |
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | 1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | <= 10 | 1 |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

Reed on 7/2/25

E3949

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|---------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | 1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | <= 10 | 6 |
| ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL) | <= 5 | 5 |
| Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water) | >= 99.5 % | 100.0 % |
| Assay (as n-Hexane) (by GC, corrected for water) | >= 95 % | 100 % |
| Color (APHA) | <= 10 | 10 |
| Residue after Evaporation | <= 1.0 ppm | 0.1 ppm |
| Substances Darkened by H ₂ SO ₄ | Passes Test | Passes Test |
| Water (by KF, coulometric) | <= 0.05 % | <0.01 % |

For Laboratory, Research, or Manufacturing Use

MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

3950

Read on 7/02/25

Jamie Croak
Director Quality Operations, Bioscience Production



Certificate of Analysis

| | |
|----------------------|--------------------------------|
| Material | BDH9274-2.5KG |
| Material Description | BDH SAND STDD OTTAWA W+I 2.5KG |
| Grade | NOT APPLICABLE |
| Batch | 25A2756718 |
| Reassay Date | 12/31/2028 |
| CAS Number | 14808-60-7 |
| Molecular Formula | SiO ₂ |
| Molecular Mass | 60.09 |
| Date of Manufacture | 12/05/2024 |
| Storage | Room Temperature |

| Characteristics | Specifications | Measured Values |
|-------------------------------|-----------------|-----------------|
| Appearance | Beige granules. | Beige granules. |
| Moisture | <= 0.1 % | 0.1 % |
| Particle Size 30-40 mesh | >= 80 % | 99 % |
| CUSTOMER PART # BDH9274-2.5KG | | |

Received on 7/1/25.

E3951

Internal ID #: 793

| Signature | Additional Information |
|---|---|
| We certify that this batch conforms to the specifications listed above. This document has been electronically produced and is valid without a signature. Leona Edwardson, Quality Control Sr. Manager - Solon VWR Chemicals, LLC. 28600 Fountain Parkway, Solon OH 44139 USA | Analysis may have been rounded to significant digits in specification limits Product meets analytical specifications of the grades listed. |

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 25C0362005
Manufactured Date: 2025-01-29
Expiration Date: 2026-04-30
Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|--|---------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | <= 5 | 1 |
| ECD Sensitive Impurities (as HeptachlorEpoxide) Single Peak (pg/mL) | <= 10 | 6 |
| ECD-Sensitive Impurities (as EthyleneDibromide) - Single Impurity Peak (ng/mL) | <= 5 | 5 |
| Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water) | >= 99.5 % | 100.0 % |
| Assay (as n-Hexane) (by GC, corrected for water) | >= 95 % | 100 % |
| Color (APHA) | <= 10 | 10 |
| Residue after Evaporation | <= 1.0 ppm | 0.1 ppm |
| Substances Darkened by H ₂ SO ₄ | Passes Test | Passes Test |
| Water (by KF, coulometric) | <= 0.05 % | <0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: United States
Packaging Site: Phillipsburg Mfg Ctr & DC

Received on 7/30/25

E3962

Jamie Croak
Director Quality Operations, Bioscience Production

For questions on this Certificate of Analysis please contact Technical Services at 855.282.6867 or +1.610.386.1700

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium



M6157
B

Material No.: 9673-33

Batch No.: 24I1262013

Manufactured Date: 2024-08-07

Retest Date: 2029-08-06

Revision No.: 0

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| ACS - Assay (H ₂ SO ₄) | 95.0 – 98.0 % | 96.2 % |
| Appearance | Passes Test | Passes Test |
| ACS - Color (APHA) | <= 10 | 5 |
| ACS - Residue after Ignition | <= 3 ppm | <1 ppm |
| ACS - Substances Reducing Permanganate(as SO ₂) | <= 2 ppm | <2 ppm |
| Ammonium (NH ₄) | <= 1 ppm | <1 ppm |
| Chloride (Cl) | <= 0.1 ppm | <0.1 ppm |
| Nitrate (NO ₃) | <= 0.2 ppm | 0.1 ppm |
| Phosphate (PO ₄) | <= 0.5 ppm | <0.1 ppm |
| Trace Impurities - Aluminum (Al) | <= 30.0 ppb | <5.0 ppb |
| Arsenic & Antimony (as As) | <= 4.0 ppb | <2.0 ppb |
| Trace Impurities - Boron (B) | <= 10.0 ppb | <5.0 ppb |
| Trace Impurities - Cadmium (Cd) | <= 2.0 ppb | <1.0 ppb |
| Trace Impurities - Chromium (Cr) | <= 6.0 ppb | <1.0 ppb |
| Trace Impurities - Cobalt (Co) | <= 0.5 ppb | <0.3 ppb |
| Trace Impurities - Copper (Cu) | <= 1.0 ppb | <1.0 ppb |
| Trace Impurities - Gold (Au) | <= 10.0 ppb | <5.0 ppb |
| Heavy Metals (as Pb) | <= 500.0 ppb | <100.0 ppb |
| Trace Impurities - Iron (Fe) | <= 50.0 ppb | <1.0 ppb |
| Trace Impurities - Lead (Pb) | <= 0.5 ppb | <0.5 ppb |
| Trace Impurities - Magnesium (Mg) | <= 7.0 ppb | <1.0 ppb |
| Trace Impurities - Manganese (Mn) | <= 1.0 ppb | <1.0 ppb |
| Trace Impurities - Mercury (Hg) | <= 0.5 ppb | <0.1 ppb |
| Trace Impurities - Nickel (Ni) | <= 2.0 ppb | <0.3 ppb |
| Trace Impurities - Potassium (K) | <= 500.0 ppb | <10.0 ppb |
| Trace Impurities - Selenium (Se) | <= 50.0 ppb | 7.2 ppb |
| Trace Impurities - Silicon (Si) | <= 100.0 ppb | 12.8 ppb |
| Trace Impurities - Silver (Ag) | <= 1.0 ppb | <1.0 ppb |

Sulfuric Acid
BAKER INSTRA-ANALYZED® Reagent
For Trace Metal Analysis
Low Selenium



Material No.: 9673-33
Batch No.: 24I1262013

| Test | Specification | Result |
|-----------------------------------|---------------|----------|
| Trace Impurities – Sodium (Na) | <= 500.0 ppb | <5.0 ppb |
| Trace Impurities – Strontium (Sr) | <= 5.0 ppb | <1.0 ppb |
| Trace Impurities – Tin (Sn) | <= 5.0 ppb | 1.1 ppb |
| Trace Impurities – Zinc (Zn) | <= 5.0 ppb | <1.0 ppb |

For Laboratory, Research, or Manufacturing Use

Country of Origin: United States

Packaging Site: Phillipsburg Mfg Ctr & DC

A handwritten signature in black ink that reads "Jamie Croak".

Jamie Croak
Director Quality Operations, Bioscience Production



Certificate of Analysis

P11518
↓
P11522
02/21/22

Product Name: Aroclor 1268 Standard

Product Number: PP-382-1

Lot Issue Date: 09-Feb-2021

Lot Number: 0006587800

Expiration Date: 31-Mar-2029

Description:

This analytical reference material (RM) was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed below.

| Analyte | CAS# | Analyte Lot | Concentration ± Uncertainty |
|--------------|-------------|-------------|-----------------------------|
| Aroclor 1268 | 011100-14-4 | RM00937 | 100.0 ± 0.5 µg/mL |

Matrix: isoctane (2,2,4-trimethylpentane)

Storage Conditions: Store at Room Temperature (15° to 30°C).

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This RM was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Intended Use:

This RM is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Hazards:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this RM.

Expiration of Certification:

The certification of this RM is valid until the expiration date specified above, provided the RM is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the RM is damaged, contaminated, or otherwise modified.

Maintenance of Certification:

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with TUV USA Inc registered ISO 9001 Quality Management System. Cert # 56 100 18560026

Page: 1 of 1

www.agilent.com/quality/
CSD-QA-015.1



ISO 17025 Cert
No. AT-1937



CERTIFIED WEIGHT REPORT

| | | | | |
|--|-----------------------|---------------------|-------------------|----|
| Part Number: | <u>91867</u> | Solvent# | 10 | |
| Lot Number: | <u>020823</u> | Acet | 11 | |
| Description: | WP 037 - Aroclor 1232 | | 12 | |
| Expiration Date: | PCB Technical Mixture | | 13 | |
| Recommended Storage: | 020833 | | 14 | |
| Nominal Concentration ($\mu\text{g/mL}$): | Ambient (20 °C) | | 15 | |
| NIST Test ID#: | 100 | Balance Uncertainty | 16 | |
| Weight(s) shown below were combined and diluted to (mL): | 6UTB | 0.057 | Flask Uncertainty | 17 |
| | 100.0 | | | |

| Compound | RM# | Lot Number | Nominal Conc ($\mu\text{g/mL}$) | Purity (%) | Uncertainty Purity | Target Weight (g) |
|-----------------|-----|------------|-----------------------------------|------------|--------------------|-------------------|
| 1. Aroclor 1232 | 17 | 45-6A | 100 | 100 | 0.5 | 0.01000 |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurements," Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Storier

Column ID SPB-608 30 meter X 0.53mm X 5 μm film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min


Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min

Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1

Standard injection = 1.5 μL , Range=3

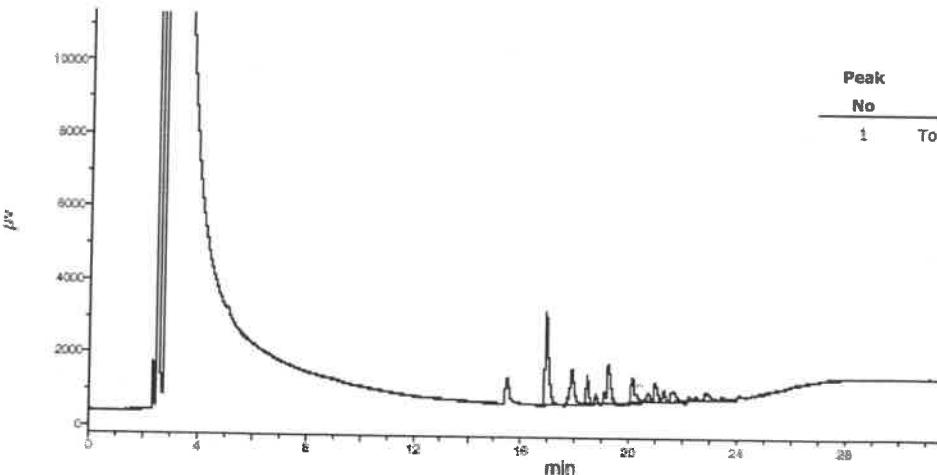



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32009

Lot No.: A0203672

p12928

Description : Aroclor® 1242 Standard

Aroclor® 1242 Standard 1,000 µg/mL, Hexane, 1mL/ampul

↓
P 12932

Container Size : 2 mL

Pkg Amt: > 1 mL

AJ
T2107123

Expiration Date : January 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|-------|--------|--------------------------------|---|
| 1 | Aroclor 1242 | 53469-21-9 | 01141 | ---% | 1,004.7 µg/mL | +/- 55.7515 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2µl

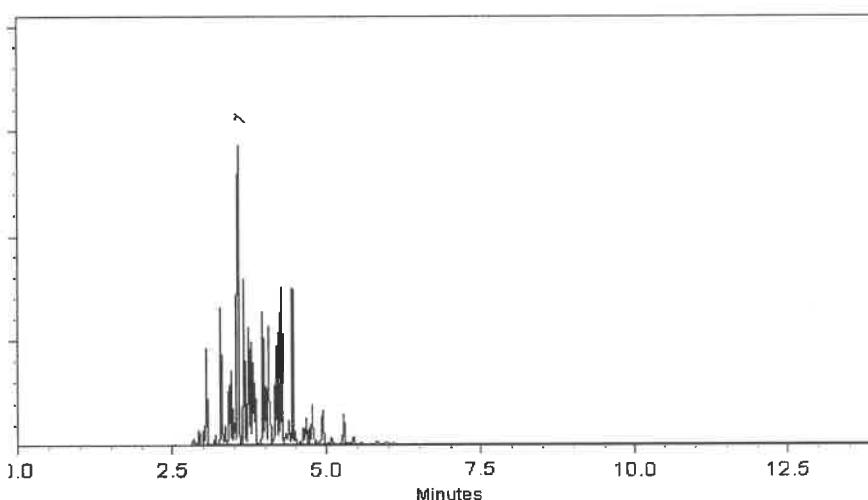

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Russ Bookhamer - Operations Technician I

Date Mixed: 26-Oct-2023 Balance Serial #: B442140311

Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 06-Nov-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32010

Lot No.: A0202803

Description : Aroclor® 1248 Standard

Aroclor® 1248 Standard 1,000 μ g/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

P12933
↓
P12937
AJ
12/07/23

C E R T I F I E D V A L U E S

| Elation Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|----------|--------|--------------------------------|---|
| 1 | Aroclor 1248 | 12672-29-6 | 13897600 | ---% | 1,001.7 μ g/mL | +/- 55.5850 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

0.2μl

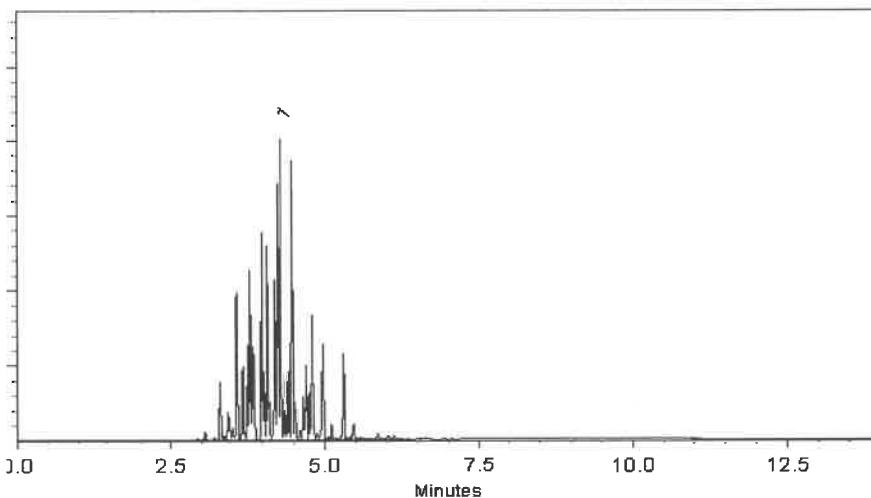

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician |

Date Mixed: 03-Oct-2023 Balance Serial #: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 09-Oct-2023

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



CERTIFIED WEIGHT REPORT

Part Number: 20064
 Lot Number: 022023
 Description: CLP PCB'S - Aroclor Mix
 Aroclors 1016 & 1260
 Expiration Date: 022033
 Recommended Storage: Ambient (20 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 1000
 NIST Test ID#: 6UTB
 5E-05 Balance Uncertainty
 Weight(s) shown below were combined and diluted to (mL): 200.0 0.010 Flask Uncertainty

| | |
|-------------------------------------|--------|
| <i>Benson Chan</i> | 022023 |
| Formulated By: <u>Benson Chan</u> | DATE |
| <i>Pedro L. Rentas</i> | 022023 |
| Reviewed By: <u>Pedro L. Rentas</u> | DATE |

P129h6 7/19
↓ 12/19/23
P129SS



CERTIFIED WEIGHT REPORT

Part Number: 20064 Solvent(s): Hexane Lot#: 273615
 Lot Number: 022023
 Description: CLP PCB'S - Aroclor Mix
Aroclors 1016 & 1260
 Expiration Date: 022033
 Recommended Storage: Ambient (20 °C)
 Nominal Concentration ($\mu\text{g/mL}$): 1000
 NIST Test ID#: 6UTB 5E-05 Balance Uncertainty
 Weight(s) shown below were combined and diluted to (mL): 200.0 0.010 Flask Uncertainty

| | |
|-------------------------------------|--------|
| | 022023 |
| Formulated By: <u>Benson Chan</u> | DATE |
| | 022023 |
| Reviewed By: <u>Pedro L. Rentas</u> | DATE |


P12946 7/19
↓
12/19/23
P12955

| Compound | RM# | Lot Number | Nominal Conc ($\mu\text{g/mL}$) | Purity (%) | Uncertainty Purity | Target Weight(g) | Actual Weight(g) | Actual Conc ($\mu\text{g/mL}$) | Expanded Uncertainty (+/-) ($\mu\text{g/mL}$) | SDS Information (Solvent Safety Info. On Attached pg.) | | |
|-----------------|-----|------------|-----------------------------------|------------|--------------------|------------------|------------------|----------------------------------|---|--|----------|--------------------|
| | | | | | | | | | | (+/-) ($\mu\text{g/mL}$) | CAS# | OSHA PEL (TWA) |
| 1. Aroclor 1016 | 15 | 020491JC | 1000 | 100 | 0.2 | 0.20004 | 0.20060 | 1002.8 | 4.0 | 12674-11-2 | N/A | N/A |
| 2. Aroclor 1260 | 21 | 020491JC | 1000 | 100 | 0.2 | 0.20004 | 0.20081 | 1003.9 | 4.0 | 11096-82-5 | 0.5mg/m3 | oral-rat 1315mg/kg |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stenier
 Column ID SPB-608 30 meter X 0.53mm X5 μm film thickness
 Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min
 Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min
 Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 290°C (Time 2 = 13.5 min)
 Rate = 8°C/min, Total run time = 35 min
 Injector temp. = 200°C, FID Temp. = 300°C. FID Signal = Edaq Channel 1
 Standard injection = 1.5 μL , Range=3

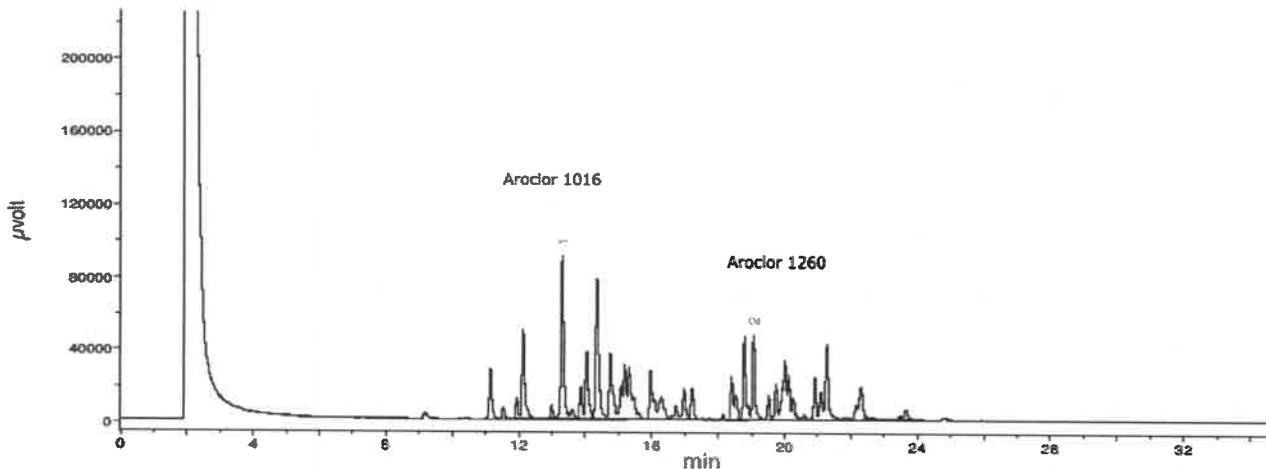



CERTIFIED WEIGHT REPORT

Part Number: 99139
Lot Number: 121823
Description: Aroclor 1254

Expiration Date: 121833
Recommended Storage: Ambient (20 °C)
Nominal Concentration ($\mu\text{g/mL}$): 100
NIST Test ID#: 6UTB

Volume(s) shown below were combined and diluted to (mL): 20.0

Note: Aroclor 1254 is a mix of isomers.

| Compound | Part Number | Lot Number | Dilution Factor | Initial Vol. (mL) | Uncertainty Pipette (mL) | Initial Conc. ($\mu\text{g/mL}$) | Final Conc. ($\mu\text{g/mL}$) | Expanded Uncertainty (+/-) ($\mu\text{g/mL}$) | SDS Information (Solvent Safety Info. On Attached pg.) | CAS# | OSHA PEL (TWA) | LD50 |
|-----------------|-------------|------------|-----------------|-------------------|--------------------------|------------------------------------|----------------------------------|---|--|------|----------------|------|
| 1. Aroclor 1254 | 79100 | 121823 | 0.10 | 2.00 | 0.017 | 1003.3 | 100.1 | 1.8 | 11097-69-1 0.5mg/m3 (skin) oral-rat 1295mg/kg | | | |

- The certified value is the concentration calculated from gravimetric and volumetric measurements unless otherwise stated.
- Standards are prepared gravimetrically using balances that are calibrated with weights traceable to NIST (see above).
- Standards are certified (+/-) 0.5% of the stated value, unless otherwise stated.
- All Standards, after opening ampule, should be stored with caps tight and under appropriate laboratory conditions.
- Uncertainty Reference: Taylor, B.N. and Kuyat, C.E., "Guidelines for Evaluating and Expressing the Uncertainty of NIST Measurement Result," NIST Technical Note 1297, U.S. Government Printing Office, Washington, DC, (1994).

Comments

GC3-M1 Analysis by Melissa Stonier

Column ID SPB-600 30 meter X 0.53mm X5µm film thickness

Flow rates: Helium (carrier) = 5mL/min, Helium (make-up) = 25mL/min

Hydrogen (make-up) = 30mL/min, Air (make-up) = 350mL/min


Oven Profile: Temp 1 = 150°C (Time 1 = 4 min), Temp 2 = 260°C (Time 2 = 13.5 min)

Rate = 8°C/min, Total run time = 35 min

Injector temp. = 200°C, FID Temp. = 300°C, FID Signal = Edaq Channel 1

Standard injection = 1.5µL, Range=3

| Peak No. | Name | FID RT (min.) |
|----------|--------------------|---------------|
| 1 | Total Aroclor 1254 | 18.12 |

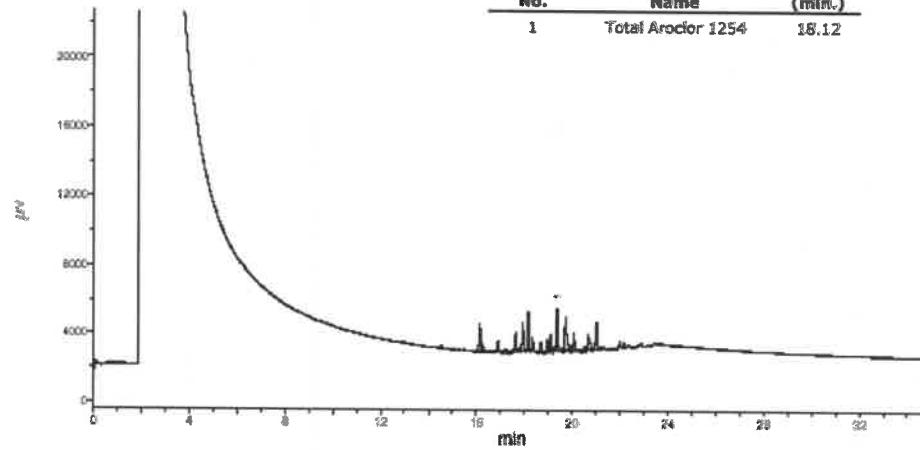



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32000

Lot No.: A0206810

Description: Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: April 30, 2030

Storage: 10°C or colder

Handling: Contains PCBs - sonicate prior to use.

Ship: Ambient

P13348
P13357
DAU
04/25/2024

CERTIFIED VALUES

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|-----------|----------|--------|--------------------------------|---|
| 1 | 2,4,5,6-Tetrachloro-m-xylene | 877-09-8 | RP220407 | 99% | 200.3 µg/mL | +/- 11.1143 |
| 2 | Decachlorobiphenyl (BZ# 209) | 2051-24-3 | 30638 | 99% | 200.6 µg/mL | +/- 11.1298 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone

CAS # 67-64-1
Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isoctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol


1µl

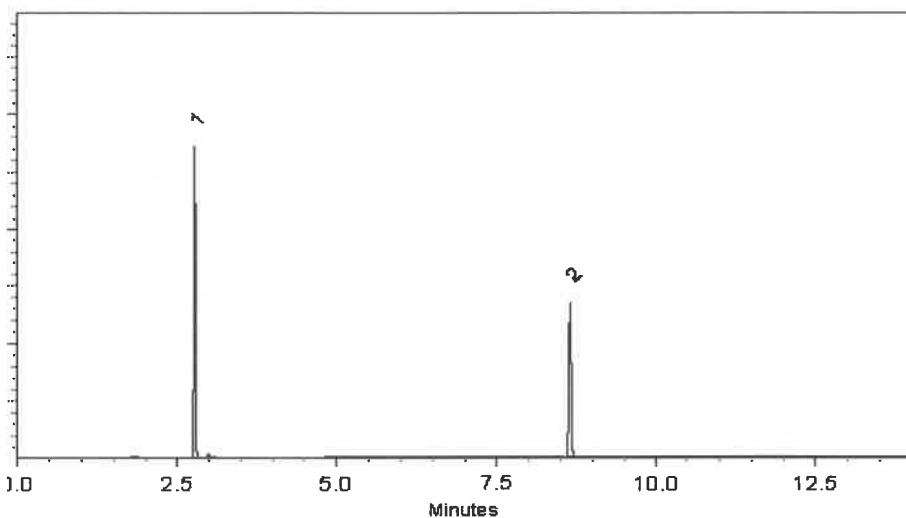

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I


Date Mixed: 22-Jan-2024 Balance Serial #: 1128360905


Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 24-Jan-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P 13348
↓
P 13357
↓
S-AWF
04/25/2025



Trusted Answers

ISO 17034

Reference Material Certificate

Product Information Sheet

| | | | |
|----------------------------|--|-------------------------|-------------|
| Product Name: | Aroclor 1221 Standard | Lot Number: | 0006783205 |
| Product Number: | PP-292-1 | Lot Issue Date: | 20-Feb-2024 |
| Storage Conditions: | Store at Room Temperature (15° to 30°C). | Expiration Date: | 31-Mar-2032 |

| Component Name | Concentration | Uncertainty | CAS# | Analyte Lot |
|----------------|-------------------|-------------|-------------|-------------|
| Aroclor 1221 | 100.3 ± 0.5 µg/mL | | 011104-28-2 | NT01017 |

Matrix: isoctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P133f2

↓

AJ
05/06/24

Page: 1 of 2

CSD-QA-015.2

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.2

ISO 17034
Cert No. AR-1936

ISO 17025
Cert No. AT-1937

250 Smith Street North Kingstown, Rhode Island 02852 www.agilent.com/quality



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32410

Lot No.: A0207475

Description: Aroclor® 1268 Standard

Aroclor® 1268 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: May 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|----------|--------|--------------------------------|---|
| 1 | Aroclor 1268 | 11100-14-4 | 10947000 | ----% | 1,000.0 µg/mL | +/- 55.4925 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

P 13386
P 13381
D 2015
05/01/2024

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

Split ratio 500:1

Inj. Vol

0.2µl

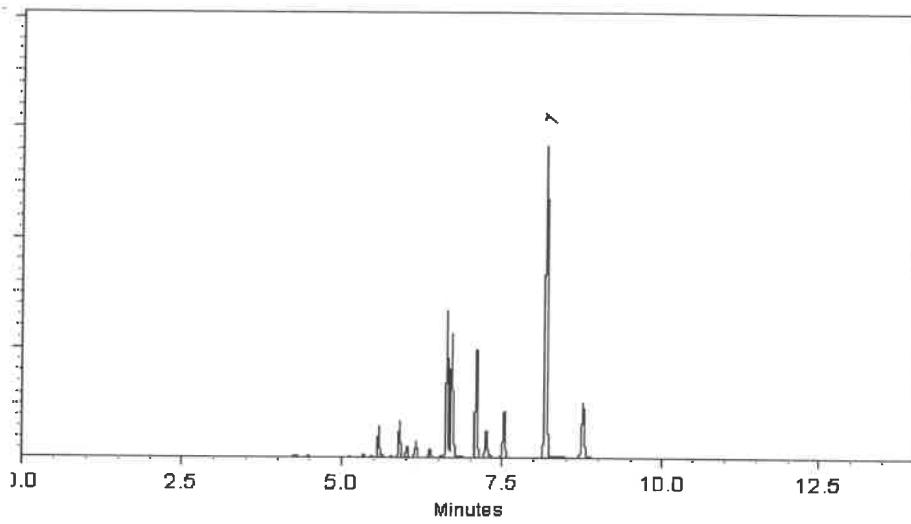

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I


Date Mixed: 06-Feb-2024 Balance Serial #: B442140311

Dillan Murphy
Dillan Murphy - Operations Technician I

Date Passed: 09-Feb-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

P13380
↓
P13381
②
05/6/2024



Reference Material Certificate

Product Name: Aroclor 1242 Standard **Lot Number:** 0006665550
Product Number: PP-312-1 **Lot Issue Date:** 08-Feb-2022
Storage Conditions: Store at Room Temperature (15° to 30°C). **Expiration Date:** 31-Jan-2027

| Component Name | CERTIFIED VALUES | | | CAS# | Analyte Lot |
|----------------|------------------|----------------------|--|-------------|-------------|
| | Concentration | Expanded Uncertainty | | | |
| Aroclor 1242 | 100.4 | ± 0.5 µg/mL | | 053469-21-9 | NT01020 |

Matrix: isoctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:


This analytical reference standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

P13589
↓
P13590

AJ
10/11/12/14

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:

Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO 9001:2015
Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/

CSD-QA-015.1



ISO 17025
Cert No. AT-

Reference Material Certificate
Product Information Sheet

Product Name: Aroclor 1248 Standard

Lot Number: 0006726317

Product Number: PP-342-1

Lot Issue Date: 27-Jan-2023

Storage Conditions: Store at Room Temperature (15° to 30°C).

Expiration Date: 28-Feb-2031

| Component Name | Concentration | Uncertainty | CAS# | Analyte Lot |
|----------------|---------------|-------------|-------------|-------------|
| Aroclor 1248 | 100.3 | ± 0.5 µg/mL | 012672-29-6 | NT01582 |

Matrix: isoctane (2,2,4-trimethylpentane)

Description:

This document is prepared in accordance with ISO 17034 and Guide 31. This analytical reference material (RM) standard was manufactured and verified in accordance with an ISO 9001 registered quality system and analyte concentrations were verified by an ISO 17025 accredited laboratory. The concentration and uncertainty value at the 95% confidence level for each analyte, determined gravimetrically, is listed above. Purity values are taken from approved vendor raw material certificates.

Traceability:

The balances used for these measurements are calibrated with weights traceable to NIST in compliance with ANSI/NCSL Z540.3, ISO 9001, ISO 17025, and ISO 17034. Calibrated Class A glassware is used for volumetric measurements. Thermometers are calibrated against a NIST traceable thermometer in accordance with NIST Special Publication 1088.

Homogeneity:

This analytical reference (RM) standard was unitized according to an in-house procedure and is guaranteed to be homogeneous. There is no minimum sub-sample size required.

Instructions for Use:

Sample aliquots for analysis should be withdrawn at 20°C to 25°C immediately after opening the container and should be processed without delay for the certified values to be valid within the stated uncertainties.

Safety:

Refer to the Safety Data Sheet on www.agilent.com for information regarding this analytical reference material.

Intended Use:

This analytical reference (RM) standard is intended for the preparation of working reference samples for use in routine laboratory analyses, calibration of instruments, validation of analytical methods, assessments of measurement methods, and continuing calibration verification.

Expiration of Certification:

The certification of this analytical reference standard (RM) is valid until the expiration date specified above, provided the material is handled and stored in accordance with the instructions given in this certificate. This certification is nullified if the material is damaged, contaminated, or otherwise modified.

p13591

↓


p13592

AJ
10/14/2024

**Maintenance of Certification:**

If substantive changes are noted that affect the certification before the expiration of this certificate, Agilent will notify the purchaser.

Sample lot approver:


Monica Bourgeois
QMS Representative



ISO 17034 Cert
No. AR-1936

RM was produced in accordance with the TUV/SUD registered ISO
9001:2015 Quality Management System. Cert# 951215321

Page: 2 of 2

www.agilent.com/quality/
CSD-QA-015.1

ISO 17025



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis *chromatographic plus*

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32039

Lot No.: A0210629

P13697
↓
P13701 } Y.P.
} 10/19/24

Description : Aroclor® 1016/1260 Mix

Aroclor® 1016/1260 Mix 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : July 31, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|---------|--------|-----------------------------|--|
| 1 | Aroclor 1016 | 12674-11-2 | 07 | ----% | 1,005.3 µg/mL | +/- 55.7809 |
| 2 | Aroclor 1260 | 11096-82-5 | 1320657 | ----% | 1,000.0 µg/mL | +/- 55.4850 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol


0.2µl

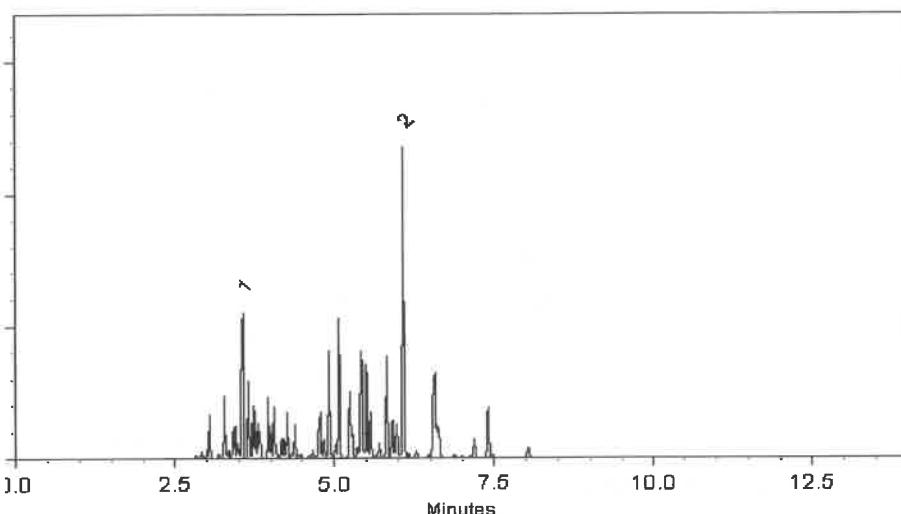

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Laith Clemente - Operations Technician I

Date Mixed: 22-Apr-2024 Balance Serial #: B442140311


Dillon Murphy - Operations Technician I

Date Passed: 24-Apr-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/ μ ECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus



FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32007

Lot No.: A0215270

Description: Aroclor® 1221 Standard

Aroclor® 1221 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size: 2 mL

Pkg Amt: > 1 mL

Expiration Date: November 30, 2030

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

P13902 }
P13903 } Y.P.
10/17/24

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|----------|--------|-----------------------------|--|
| 1 | Aroclor 1221 | 11104-28-2 | 14969200 | ----% | 1,005.0 µg/mL | +/- 55.7700 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane
CAS # 110-54-3
Purity 99%

Quality Confirmation Test

Column:

30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C
@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

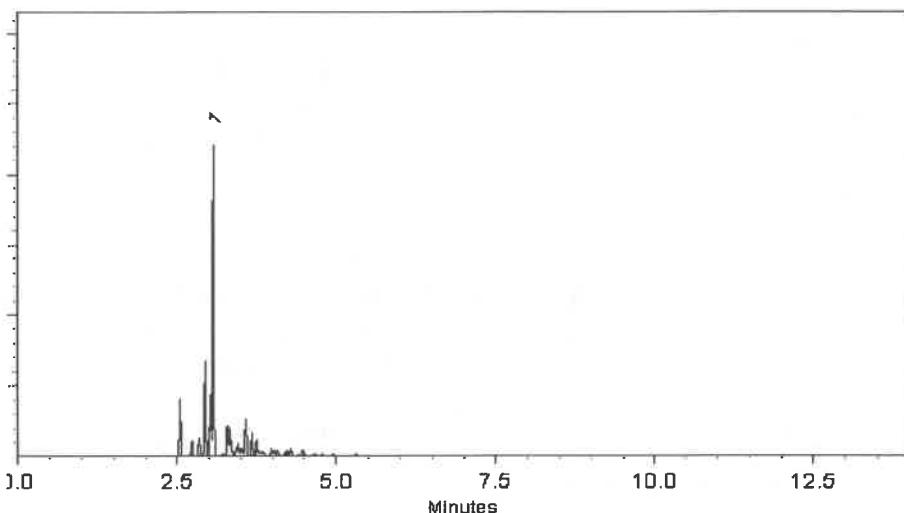

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I

Date Mixed: 16-Aug-2024 Balance Serial #: 1128360905

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 20-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

General Certified Reference Material Notes

Expiration Notes:

- Expiration date valid for unopened ampul stored in compliance with the recommended conditions.
- Uncertainty, concentration, and expiration of the CRM are based on the unopened product being stored according to the recommended condition found in the storage field.

Purity Notes:

- Purity and/or chemical identity are determined by one or more of the following techniques: GC/FID, HPLC, GC/μECD, GC/MS, LC/MS, RI, and/or melting point.
- Compounds with a listed purity of less than 99% have been weight corrected to compensate for impurities and/or salts. A correction factor is used to calculate the amount of compound necessary to achieve the desired concentration of the parent compound in solution.
- Purity of isomeric compounds is reported as the sum of the isomers.
- Purity values are rounded to the nearest whole number.

Certified Uncertainty Value Notes:

- The uncertainties are determined in accordance with ISO 17034 and Guide 35. The certified expanded uncertainty value includes gravimetric uncertainty, homogeneity between-ampul uncertainty, storage stability uncertainty and shipping stability uncertainty and were combined using the following formula:

$$U_{\text{combined uncertainty}} = k \sqrt{u_{\text{gravimetric}}^2 + u_{\text{homogeneity}}^2 + u_{\text{storage stability}}^2 + u_{\text{shipping stability}}^2}$$

k is a coverage factor of 2, which gives a level of confidence of approximately 95%.

- The packaged amount is the minimum sample size for which uncertainty is valid. The ampuls are over-filled to ensure that the minimum packaged amount can be sufficiently transferred.

Manufacturing Notes:

- Concentration is based upon gravimetric preparation using either a balance whose calibration has been verified daily using NIST traceable weights, and/or dilutions with Class A glassware.

Handling Notes:

- Stability of the unopened product, when stored in compliance with the recommended conditions, is guaranteed through the expiration displayed on the product label and certificate. Contact Restek for additional opened product stability information, with the knowledge/understanding that open product stability is subject to the specific handling and environmental conditions to which the product is exposed. For your convenience Restek supplies deactivated vials with most standards packed in 2mL ampuls. Larger volume deactivated vials are available through Restek as a custom ordered item. Additionally, Restek sells DMDCS for the purpose of glassware deactivation as catalog number 31861, which includes complete instructions.
- If any undissolved material is visible inside the ampul, sonicate the unopened ampul until the material is completely dissolved.



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32000

Lot No.: A0214495

Description : Pesticide Surrogate Mix

Pesticide Surrogate Mix 200 µg/mL, Acetone, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : October 31, 2030

Storage: 10°C or colder

Handling: Contains PCBs - sonicate prior to use.

Ship: Ambient

p19785

J

AJ
11/19/24

p19789

11/19/24

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|------------------------------|-----------|----------|--------|--------------------------------|---|
| 1 | 2,4,5,6-Tetrachloro-m-xylene | 877-09-8 | RP220407 | 99% | 200.2 µg/mL | +/- 11.1087 |
| 2 | Decachlorobiphenyl (BZ# 209) | 2051-24-3 | 30679 | 99% | 201.4 µg/mL | +/- 11.1753 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Acetone

CAS # 67-64-1

Purity 99%

Tech Tips:

Decachlorobiphenyl has poor solubility in most organic solvents. The maximum concentration that can be prepared in acetone, hexane, or isoctane is 200µg/mL. Temperature will affect the solubility as well. Storing solutions at reduced temperatures will cause decachlorobiphenyl to precipitate.

Products containing decachlorobiphenyl must be sonicated for a minimum of 10 minutes prior to opening the ampul. Because each ultrasonic bath operates at a different energy level, 10 minutes is a guideline only. Longer sonication time will not affect product quality.

These precautions apply to working solutions prepared in your laboratory as well. The amount of compound that precipitates depends on concentration AND temperature. If you store your standards at a temperature lower than 4°C (even dilute solutions), allow extra sonication time.

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1µl

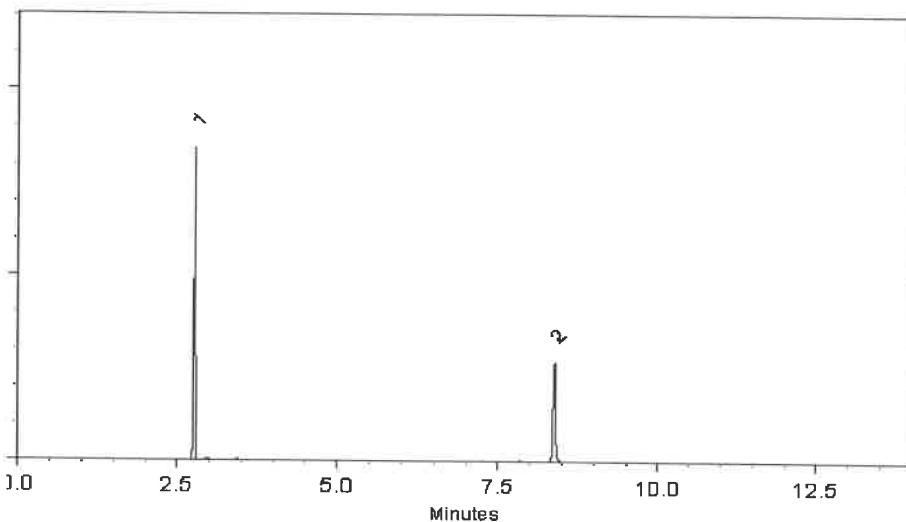

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

Aaron Enyart
Aaron Enyart - Operations Tech I

Date Mixed: 29-Jul-2024 Balance Serial #: B345965662

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 01-Aug-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL



21
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



22
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

Certificate of Analysis

chromatographic plus

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32011

Lot No.: A0217391

Description : Aroclor® 1254 Standard

Aroclor® 1254 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : January 31, 2031

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|-----------|--------|--------------------------------|---|
| 1 | Aroclor 1254 | 11097-69-1 | 124-191-B | ----% | 1,004.7 µg/mL | +/- 55.7515 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

P13830
↓
P13832 12/09/24 AJ

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

1µl

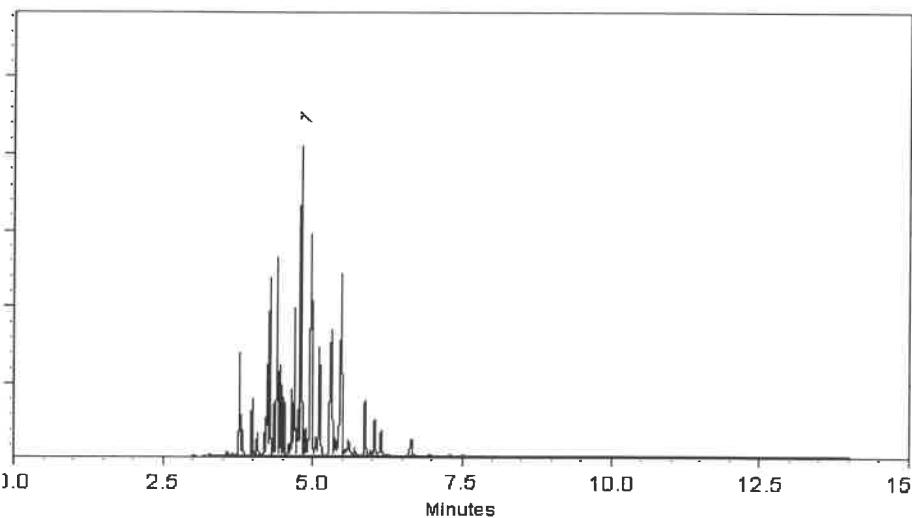

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I

Date Mixed: 02-Oct-2024 Balance Serial #: C322230531

Jennifer Pollino
Jennifer Pollino - Operations Tech III - ARM QC

Date Passed: 07-Oct-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No. : 32008

Lot No.: A0219655

Description : Aroclor® 1232 Standard

Aroclor® 1232 Standard 1,000 µg/mL, Hexane, 1mL/ampul

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : March 31, 2031

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|----------|--------|--------------------------------|---|
| 1 | Aroclor 1232 | 11141-16-5 | 15665-01 | ----% | 1,007.0 µg/mL | +/- 55.8810 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

p13878
↓
p13860

AJ
01/28/25

Quality Confirmation Test

Column:30m x .25mm x .2um
Rtx-CLP II (cat.# 11323)**Carrier Gas:**

helium-constant pressure 20 psi.

Temp. Program:200°C to 300°C
@ 25°C/min. (hold 10 min.)**Inj. Temp:**

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

10 ml/min.

Inj. Vol

1μl

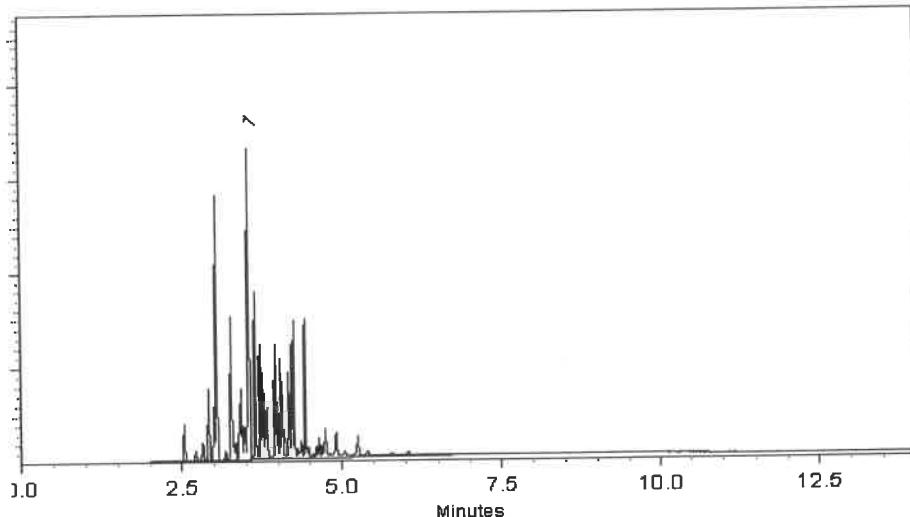

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.

michael maye
Michael Maye - Operations Tech I

Date Mixed: 02-Dec-2024 Balance Serial #: C322230531

Brittany Federinko
Brittany Federinko - Operations Tech I

Date Passed: 05-Dec-2024

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397



110 Benner Circle
Bellefonte, PA 16823-8812
Tel: 1-814-353-1300
Fax: 1-814-353-1309

www.restek.com

CERTIFIED REFERENCE MATERIAL

Certificate of Analysis

chromatographic plus



ILAC-MRA
ACCREDITED
ISO 17034 Accredited
Reference Material Producer
Certificate #3222.01



ILAC-MRA
ACCREDITED
ISO/IEC 17025 Accredited
Testing Laboratory
Certificate #3222.02

FOR LABORATORY USE ONLY-READ SDS PRIOR TO USE.

This Reference Material is intended for Laboratory Use Only as a standard for the qualitative and/or quantitative determination of the analyte(s) listed.

Catalog No.: 32409

Lot No.: A0220950

Description : Aroclor® 1262 Standard

Aroclor® 1262 Standard 1,000 µg/mL, 1mL/ampul, Hexane

Container Size : 2 mL

Pkg Amt: > 1 mL

Expiration Date : April 30, 2031

Storage: 25°C nominal

Handling: This product contains PCBs.

Ship: Ambient

C E R T I F I E D V A L U E S

| Elution Order | Compound | CAS # | Lot # | Purity | Grav. Conc. (weight/volume) | Expanded Uncertainty * (95% C.L.; K=2) |
|---------------|--------------|------------|----------|--------|-----------------------------|--|
| 1 | Aroclor 1262 | 37324-23-5 | 10849100 | ----% | 1,002.0 µg/mL | +/- 55.6035 |

* Expanded Uncertainty displayed in same units as Grav. Conc.

Solvent: Hexane

CAS # 110-54-3

Purity 99%

p13882

↓

AJ
01/28/25

p13883

Quality Confirmation Test

Column:

30m x .25mm x .2um

Rtx-CLP II (cat.# 11323)

Carrier Gas:

helium-constant pressure 20 psi.

Temp. Program:

200°C to 300°C

@ 25°C/min. (hold 10 min.)

Inj. Temp:

250°C

Det. Temp:

300°C

Det. Type:


ECD

Split Vent:

300 ml/min.

Inj. Vol

0.2µl

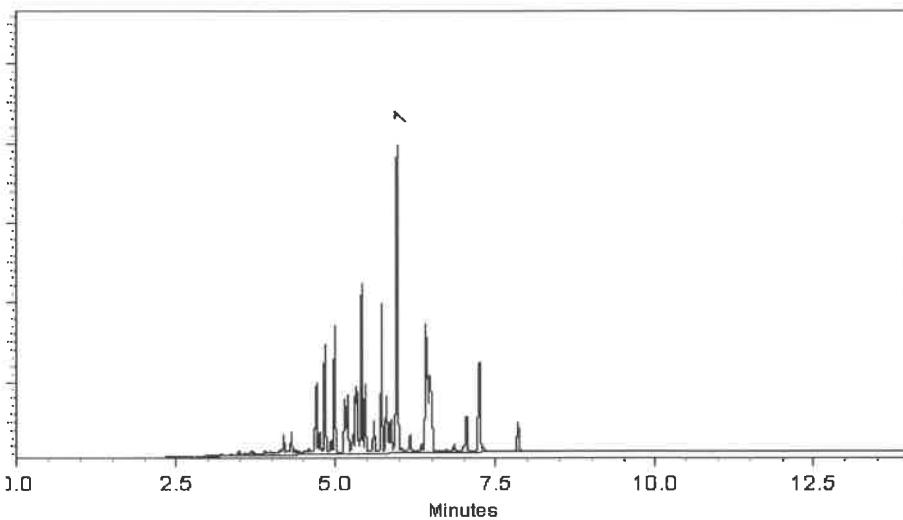

This chromatogram represents a general set of testing conditions chosen for product acceptance. For optimal results in your lab, conditions should be adjusted for your specific instrument, method, and application.


Tom Suckar - Mix Technician

Date Mixed: 09-Jan-2025 Balance Serial #: C322230531


Brittany Federinko - Operations Tech I

Date Passed: 14-Jan-2025

Manufactured under Restek's ISO 9001:2015
Registered Quality System
Certificate #FM 80397

n-Hexane 95%
ULTRA RESI-ANALYZED
For Organic Residue Analysis



Material No.: 9262-03
Batch No.: 24G1962003
Manufactured Date: 2024-05-23
Expiration Date: 2025-08-22
Revision No.: 0

W314X
W314X
CPLTE. 02/03/2023
SP

Certificate of Analysis

| Test | Specification | Result |
|---|---------------|-------------|
| FID-Sensitive Impurities (as 2-Octanol) Single Impurity Peak (ng/mL) | ≤ 5 | 3 |
| ECD Sensitive Impurities (as Heptachlor Epoxide) Single Peak (pg/mL) | ≤ 10 | 1 |
| ECD-Sensitive Impurities (as Ethylene Dibromide) - Single Impurity Peak (ng/mL) | ≤ 5 | 1 |
| Assay (Total Saturated C ₆ Isomers) (by GC, corrected for water) | ≥ 99.5 % | 99.7 % |
| Assay (as n-Hexane) (by GC, corrected for water) | ≥ 95 % | 98 % |
| Color (APHA) | ≤ 10 | 5 |
| Residue after Evaporation | ≤ 1.0 ppm | 0.1 ppm |
| Substances Darkened by H ₂ SO ₄ | Passes Test | Passes Test |
| Water (by KF, coulometric) | ≤ 0.05 % | < 0.01 % |

For Laboratory, Research, or Manufacturing Use
MEETS SPECIFICATIONS WITHIN THE EXPIRATION PERIOD

Country of Origin: USA
Packaging Site: Phillipsburg Mfg Ctr & DC

Jamie Croak

Director Quality Operations, Biosciences Division



SHIPPING DOCUMENTS

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20



284 Sheffield Street, Mountainside, NJ 07092
 (908) 789-8900 • Fax (908) 789-8922
www.chemtech.net

ALLIANCE PROJECT NO.

QUOTE NO.

COC Number

Q2819

2045329

CLIENT INFORMATION

REPORT TO BE SENT TO:

COMPANY: First Environment

ADDRESS: 10 Park Pl Bldg 1A Suite 504

CITY Butler STATE: NJ ZIP: 07405

ATTENTION: Al Smith

PHONE: 973-334-0003 FAX:

CLIENT PROJECT INFORMATION

PROJECT NAME: USACE FIMP

PROJECT NO.: USACE018-44 LOCATION: Long Island, NY

PROJECT MANAGER: Al Smith

e-mail: asmith@firstenvironment.com

PHONE: 973-334-0003

FAX::

CLIENT BILLING INFORMATION

BILL TO:

PO#:

ADDRESS:

CITY

STATE: ZIP:

ATTENTION:

PHONE:

ANALYSIS

DATA TURNAROUND INFORMATION

FAX (RUSH) _____ DAYS*

HARDCOPY (DATA PACKAGE): 10 DAYS*

EDD: 10 DAYS*

*TO BE APPROVED BY CHEMTECH

STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS

DATA DELIVERABLE INFORMATION

Level 1 (Results Only) Level 4 (QC + Full Raw Data)

Level 2 (Results + QC) NJ Reduced US EPA CLP

Level 3 (Results + QC + Raw Data) NYS ASP A NYS ASP B

Other _____

EDD FORMAT NYSDOC

NAC / SVOC
pest. / PCB
metals

1 2 3 4 5 6 7 8 9

PRESERVATIVES

COMMENTS

← Specify Preservatives

A-HCl D-NaOH

B-HN03 E-ICE

C-H2SO4 F-OTHER

| ALLIANCE SAMPLE ID | PROJECT SAMPLE IDENTIFICATION | SAMPLE MATRIX | SAMPLE TYPE | | SAMPLE COLLECTION | | # OF BOTTLES | PRESERVATIVES | | | | | | | | | COMMENTS |
|--------------------|-------------------------------|---------------|-------------|------|-------------------|------|--------------|---------------|---|---|---|---|---|---|---|---|----------|
| | | | CMP | GRAB | DATE | TIME | | 1 | 2 | 3 | 4 | 5 | 6 | 7 | 8 | 9 | |
| 1. | 22BP-N | S | | | 8/4/25 | 1500 | 5 | X | | | | | | | | | |
| 2. | 22BP-E | S | | | | 1434 | 5 | X | | | | | | | | | |
| 3. | 22BP-W | S | | | | 1418 | 5 | X | | | | | | | | | |
| 4. | 22BP-S | S | | | | 1427 | 5 | X | | | | | | | | | |
| 5. | IIM-W | S | | | 8/5/25 | 1015 | 5 | K | | | | | | | | | |
| 6. | IIM-S | S | | | | 0955 | 7 | K | X | X | | | | | | | |
| 7. | IIM-N | S | | | | 1100 | 5 | K | | | | | | | | | |
| 8. | IIM-E | S | | | | 1110 | 5 | X | | | | | | | | | |
| 9. | 84SB-E | S | | | | 1340 | 5 | X | | | | | | | | | |
| 10. | 84SB-S | S | | | | 1410 | 5 | X | | | | | | | | | |

SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY

| | | | |
|--------------------------|------------|--|--|
| RELINQUISHED BY SAMPLER: | DATE/TIME: | RECEIVED BY: | Conditions of bottles or coolers at receipt: <input type="checkbox"/> COMPLIANT <input type="checkbox"/> NON COMPLIANT <input checked="" type="checkbox"/> COOLER TEMP 3.8i °C |
| 1. GNC | 6:01 | 1. 8-8-25 | Comments: _____ |
| RELINQUISHED BY SAMPLER: | DATE/TIME: | RECEIVED BY: | |
| 2. | | 2. | |
| RELINQUISHED BY SAMPLER: | DATE/TIME: | RECEIVED BY: | |
| 3. | | 3. | |
| Page 1 of 5 | CLIENT: | <input type="checkbox"/> Hand Delivered <input type="checkbox"/> Other | Shipment Complete <input type="checkbox"/> YES <input type="checkbox"/> NO |

| CLIENT INFORMATION | | | CLIENT PROJECT INFORMATION | | | CLIENT BILLING INFORMATION | | | | | | | |
|--|---------------------|------------------------|--|--|-------------------|-------------------------------------|--|-------|--|--|--|--|--|
| REPORT TO BE SENT TO: | | | | | | | | | | | | | |
| COMPANY: <u>See page</u> | | | PROJECT NAME: _____ | | | BILL TO: _____ | | | | | | | |
| ADDRESS: _____ | | | PROJECT NO.: _____ LOCATION: _____ | | | PO#: _____ | | | | | | | |
| CITY: _____ | STATE: _____ | ZIP: _____ | PROJECT MANAGER: _____ | | | ADDRESS: _____ | | | | | | | |
| ATTENTION: _____ | | | e-mail: _____ | | | CITY: _____ STATE: _____ ZIP: _____ | | | | | | | |
| PHONE: _____ | | FAX: _____ | PHONE: _____ | | FAX: _____ | ATTENTION: _____ PHONE: _____ | | | | | | | |
| DATA TURNAROUND INFORMATION | | | | | | | | | | | | | |
| FAX (RUSH) _____ DAYS* | | | HARDCOPY (DATA PACKAGE): <u>10</u> DAYS* | | | EDD: <u>10</u> DAYS* | | | | | | | |
| *TO BE APPROVED BY CHEMTECH STANDARD HARDCOPY TURNAROUND TIME IS 10 BUSINESS | | | | | | | | | | | | | |
| PROJECT SAMPLE IDENTIFICATION | | | SAMPLE MATRIX | SAMPLE TYPE | SAMPLE COLLECTION | OF BOTTLES # | PRESERVATIVES | | | COMMENTS | | | |
| ALLIANCE SAMPLE ID | 1. <u>84 3B - W</u> | | | S C | 8/5/25 1400 | 7 | X X X | | | | ← Specify Preservatives A-HCl D-NaOH B-HNO3 E-ICE C-H2SO4 F-OTHER | | |
| | 2. <u>17M - S</u> | | | | | 1605 | 5 | X | | | | | |
| | 3. <u>17M - E</u> | | | | | 1700 | 5 | X | | | | | |
| | 4. <u>17M - W</u> | | | | | 1620 | 7 | X X X | | | | | |
| | 5. <u>17M - N</u> | | | | | 1640 | 5 | X | | | | | |
| | 6. <u>38M - S</u> | | | | | 8/6/25 0935 | 5 | X | | | | | |
| | 7. <u>38M - N</u> | | | | | 1005 | 5 | X | | | | | |
| | 8. <u>38M - W</u> | | | | | 0955 | 15 | X X X | | | | | |
| | 9. <u>38M - E</u> | | | | | 1020 | 5 | X | | | | | |
| | 10. <u>82H - E</u> | | | | | 1205 | 5 | X | | | | | |
| SAMPLE CUSTODY MUST BE DOCUMENTED BELOW EACH TIME SAMPLES CHANGE POSSESSION INCLUDING COURIER DELIVERY | | | | | | | | | | | | | |
| RELINQUISHED BY SAMPLER: 1. <u>Gme</u> | | DATE/TIME: <u>6:01</u> | RECEIVED BY: <u>R. J. 8.8.24</u> | Conditions of bottles or coolers at receipt: <input type="checkbox"/> COMPLIANT <input type="checkbox"/> NON COMPLIANT <input checked="" type="checkbox"/> COOLER TEMP <u>3.6 c</u> °C | | | Comments: _____ | | | | | | |
| RELINQUISHED BY SAMPLER: 2. | | DATE/TIME: | RECEIVED BY: | | | | | | | | | | |
| RELINQUISHED BY SAMPLER: 3. | | DATE/TIME: | RECEIVED BY: 3. | | | | CLIENT: <input type="checkbox"/> Hand Delivered <input type="checkbox"/> Other | | | Shipment Complete <input type="checkbox"/> YES <input type="checkbox"/> NO | | | |
| Page <u>2</u> of <u>5</u> | | | | | | | | | | | | | |

Laboratory Certification

| Certified By | License No. |
|----------------------|------------------|
| CAS EPA CLP Contract | 68HERH20D0011 |
| Connecticut | PH-0830 |
| DOD ELAP (ANAB) | L2219 |
| Maine | 2024021 |
| Maryland | 296 |
| New Hampshire | 255424 Rev 1 |
| New Jersey | 20012 |
| New York | 11376 |
| Pennsylvania | 68-00548 |
| Soil Permit | 525-24-234-08441 |
| Texas | T104704488 |

LOGIN REPORT/SAMPLE TRANSFER

| | | | |
|--|--------|--|-----------------------|
| Order ID : Q2819 | FIRS02 | Order Date : 8/11/2025 12:06:00 PM | Project Mgr : |
| Client Name : First Environment, Inc. | | Project Name : USACE018-44 DOD | Report Type : Level 4 |
| Client Contact : Al Smith | | Receive DateTime : 8/8/2025 6:01:00 PM | EDD Type : EQUIS |
| Invoice Name : First Environment, Inc. | | Purchase Order : | Hard Copy Date : |
| Invoice Contact : Al Smith | | | Date Signoff : |

| LAB ID | CLIENT ID | MATRIX | SAMPLE DATE | SAMPLE TIME | TEST | TEST GROUP | METHOD | FAX DATE | DUE DATES |
|----------|-----------|--------|-------------|-------------|---------------|------------|--------|--------------|-----------|
| Q2819-01 | 22BP-N | Solid | 08/04/2025 | 15:00 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-02 | 22BP-E | Solid | 08/04/2025 | 14:34 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-03 | 22BP-W | Solid | 08/04/2025 | 14:18 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-04 | 22BP-S | Solid | 08/04/2025 | 14:27 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-05 | 11M-W | Solid | 08/05/2025 | 10:15 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-06 | 11M-S | Solid | 08/05/2025 | 09:55 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-07 | 11M-N | Solid | 08/05/2025 | 11:00 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-08 | 11M-E | Solid | 08/05/2025 | 11:10 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |

DP 08/16/2025

LOGIN REPORT/SAMPLE TRANSFER

Order ID : Q2819 **FIRS02**

Order Date : 8/11/2025 12:06:00 PM

Project Mgr :

Client Name : First Environment, Inc.

Project Name : USACE018-44 DOD

Report Type : Level 4

Client Contact : Al Smith

Receive DateTime : 8/8/2025 6:01:00 PM

EDD Type : EQUIS

Invoice Name : First Environment, Inc.

Purchase Order :

Hard Copy Date :

Invoice Contact : Al Smith

Date Signoff :


| LAB ID | CLIENT ID | MATRIX | SAMPLE DATE | SAMPLE TIME | TEST | TEST GROUP | METHOD | FAX DATE | DU ^E DATES |
|----------|------------------------------|--------|-------------|-------------|---------------|------------|--------|--------------|-----------------------|
| Q2819-09 | 84SB-E 845SB-E | Solid | 08/05/2025 | 13:40 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-10 | 84SB-S 845SB-S | Solid | 08/05/2025 | 14:10 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-11 | 84SB-W 845SB-W | Solid | 08/05/2025 | 14:00 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-12 | 17M-S | Solid | 08/05/2025 | 16:05 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-13 | 17M-E | Solid | 08/05/2025 | 17:00 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-14 | 17M-W | Solid | 08/05/2025 | 16:20 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-15 | 17M-N | Solid | 08/05/2025 | 16:40 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |

LOGIN REPORT/SAMPLE TRANSFER

| | | | |
|--|--------|--|-----------------------|
| Order ID : Q2819 | FIRS02 | Order Date : 8/11/2025 12:06:00 PM | Project Mgr : |
| Client Name : First Environment, Inc. | | Project Name : USACE018-44 DOD | Report Type : Level 4 |
| Client Contact : Al Smith | | Receive DateTime : 8/8/2025 6:01:00 PM | EDD Type : EQUIS |
| Invoice Name : First Environment, Inc. | | Purchase Order : | Hard Copy Date : |
| Invoice Contact : Al Smith | | | Date Signoff : |


| LAB ID | CLIENT ID | MATRIX | SAMPLE DATE | SAMPLE TIME | TEST | TEST GROUP | METHOD | FAX DATE | DUE DATES |
|----------|-----------|--------|-------------|-------------|---------------|------------|--------|--------------|-----------|
| Q2819-16 | 38M-S | Solid | 08/06/2025 | 09:35 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-17 | 38M-N | Solid | 08/06/2025 | 10:05 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-18 | 38M-W | Solid | 08/06/2025 | 09:55 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-19 | 38M-E | Solid | 08/06/2025 | 10:20 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |
| Q2819-20 | 82H-E | Solid | 08/06/2025 | 12:05 | VOC-TCLVOA-10 | | 8260D | 10 Bus. Days | |

Relinquished By :

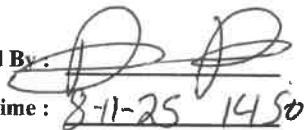

Date / Time : 8-11-25 14:50

Received By :



Date / Time :

8-11-25 14:50 Rg H 6
522

Storage Area : VOA Refrigerator Room

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:27
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:41:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:41:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 207.9E6 | 127.8E6 | 24.188 | 24.425 |
| 2) SA Decachlor... | 8.693 | 8.639 | 191.8E6 | 47304642 | 25.044 | 25.765 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 4.756 | 4.737 | 69875317 | 44959652 | 245.828 | 253.500 |
| 4) L1 AR-1016-2 | 4.774 | 4.756 | 105.2E6 | 68066920 | 246.833 | 255.376 |
| 5) L1 AR-1016-3 | 4.831 | 4.931 | 65721962 | 35251812 | 244.790 | 253.028 |
| 6) L1 AR-1016-4 | 4.951 | 4.973 | 53435135 | 29674672 | 244.973 | 262.052 |
| 7) L1 AR-1016-5 | 5.207 | 5.185 | 58842499 | 38084113 | 256.222 | 260.764 |
| 31) L7 AR-1260-1 | 6.244 | 6.213 | 125.2E6 | 69330497 | 277.528 | 268.518 |
| 32) L7 AR-1260-2 | 6.434 | 6.401 | 189.6E6 | 85155201 | 272.943 | 257.556 |
| 33) L7 AR-1260-3 | 6.800 | 6.553 | 153.7E6 | 66184896 | 249.524 | 251.419 |
| 34) L7 AR-1260-4 | 7.059 | 7.022 | 126.3E6 | 50234042 | 267.727 | 258.471 |
| 35) L7 AR-1260-5 | 7.302 | 7.264 | 336.9E6 | 108.7E6 | 257.581 | 254.474 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112417.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:27
 Operator : YP/AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 12:41:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 12:41:19 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

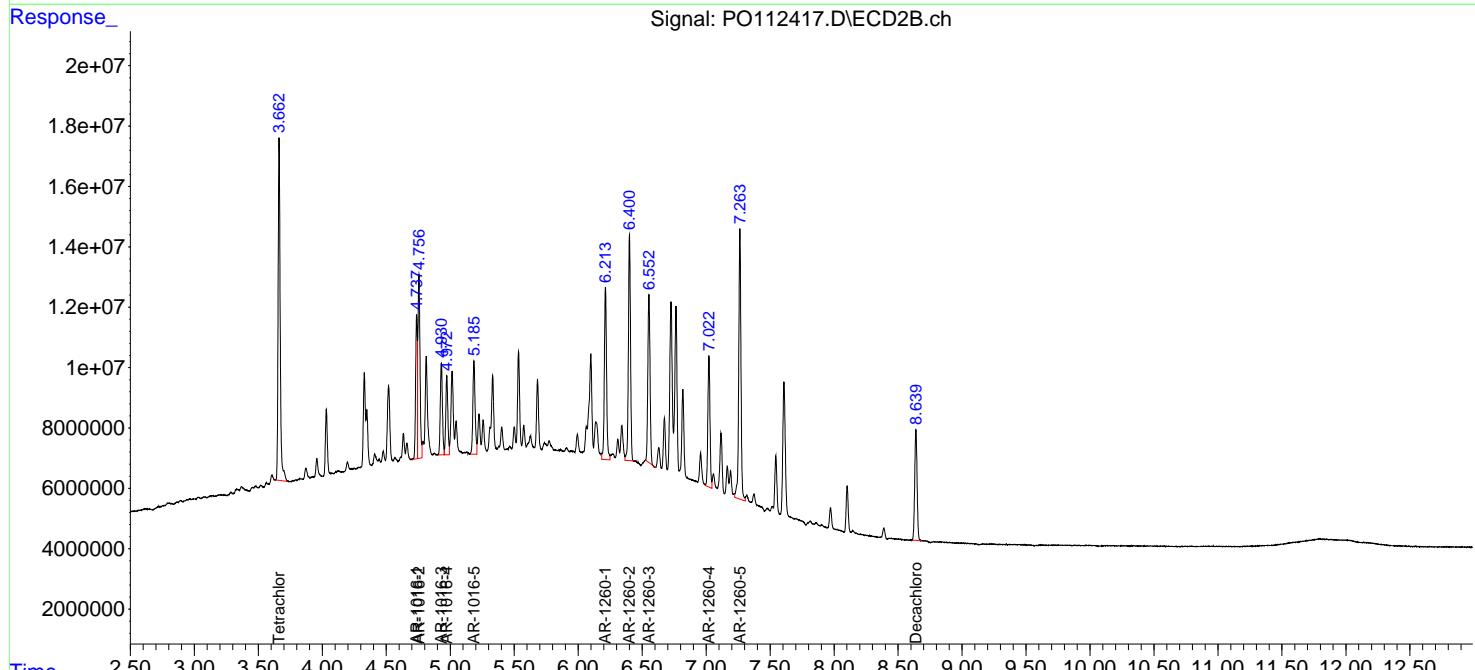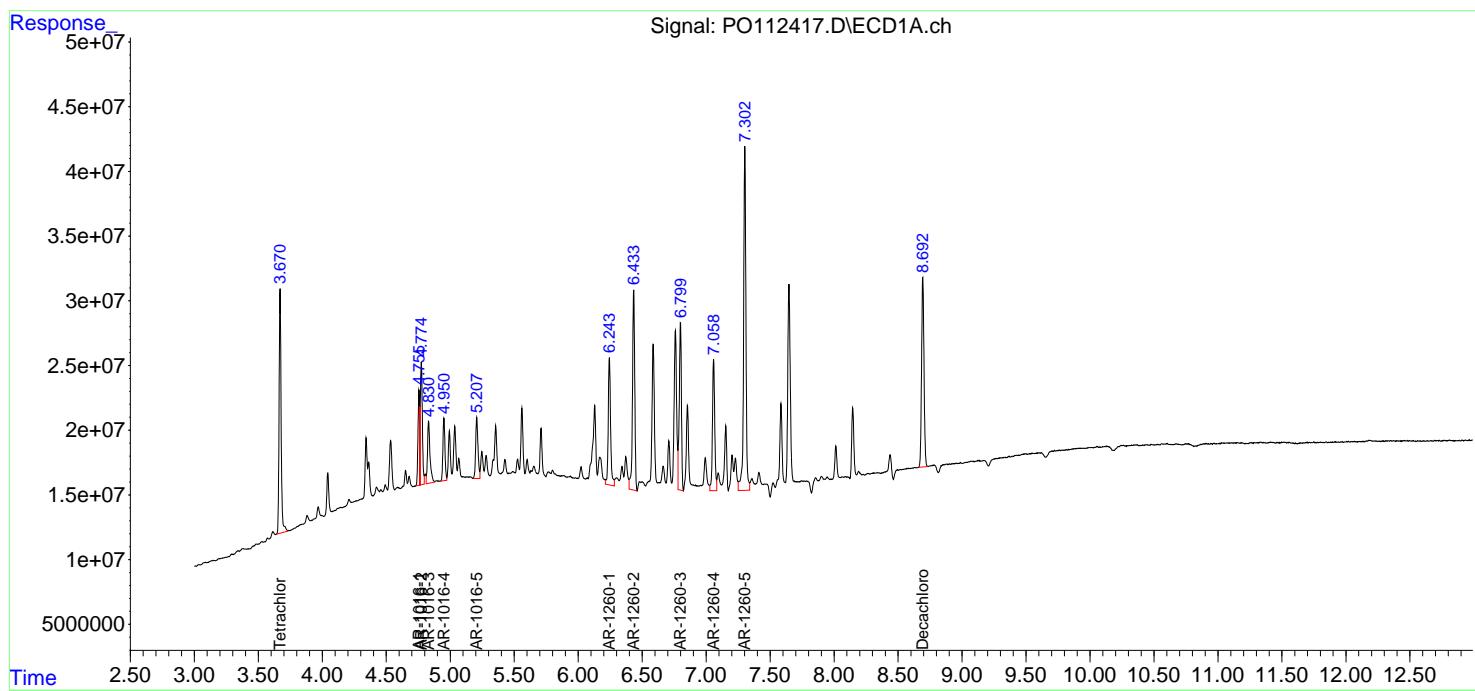

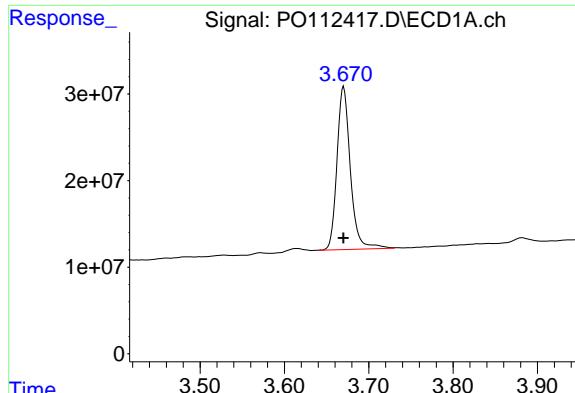


#1 Tetrachloro-m-xylene
R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 207865500
Conc: 24.19 ng/ml


Instrument: ECD_O
ClientSampleId: AR1660ICC250

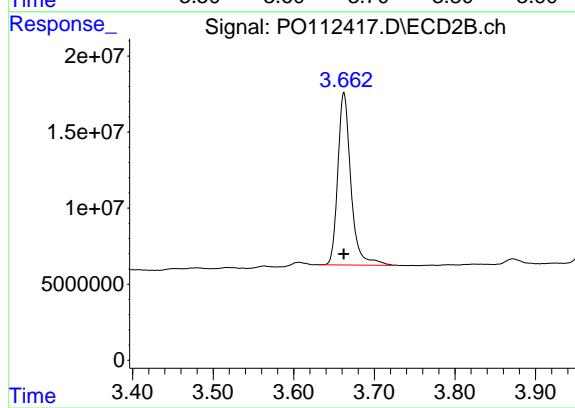


#1 Tetrachloro-m-xylene
R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 127780164
Conc: 24.42 ng/ml

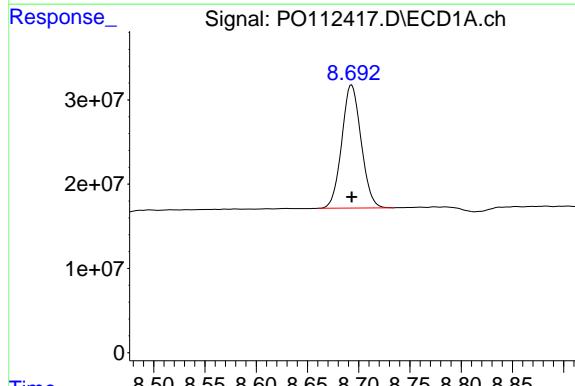

#2 Decachlorobiphenyl
R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 191806392
Conc: 25.04 ng/ml

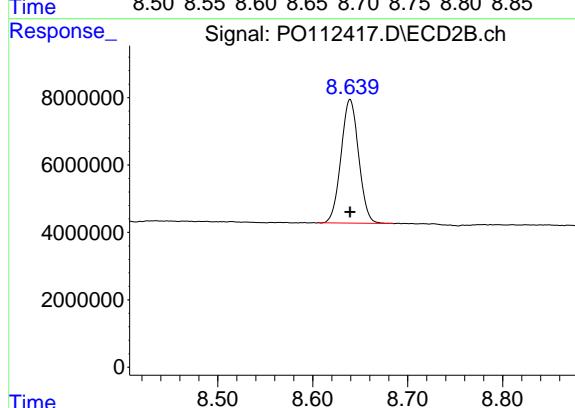

#2 Decachlorobiphenyl
R.T.: 8.639 min
Delta R.T.: 0.000 min
Response: 47304642
Conc: 25.76 ng/ml

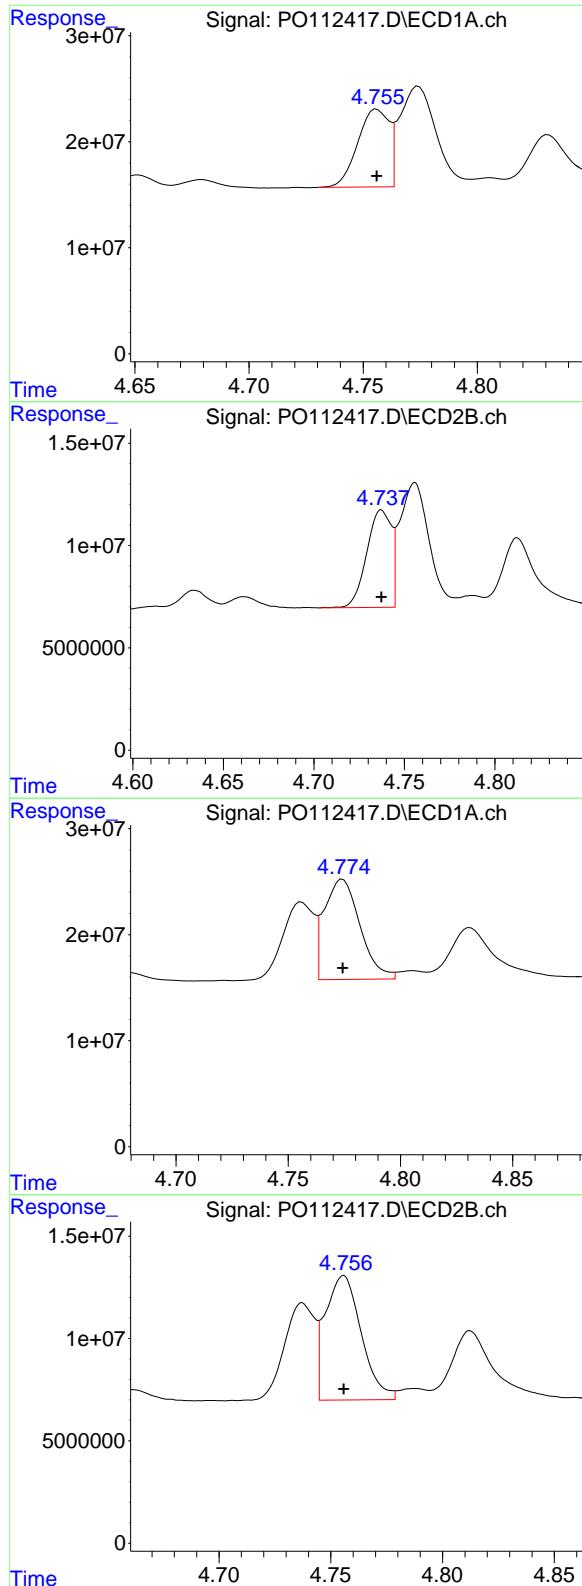

#3 AR-1016-1

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 69875317
 Conc: 245.83 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#3 AR-1016-1


R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 44959652
 Conc: 253.50 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 105176225
 Conc: 246.83 ng/ml

#4 AR-1016-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 68066920
 Conc: 255.38 ng/ml

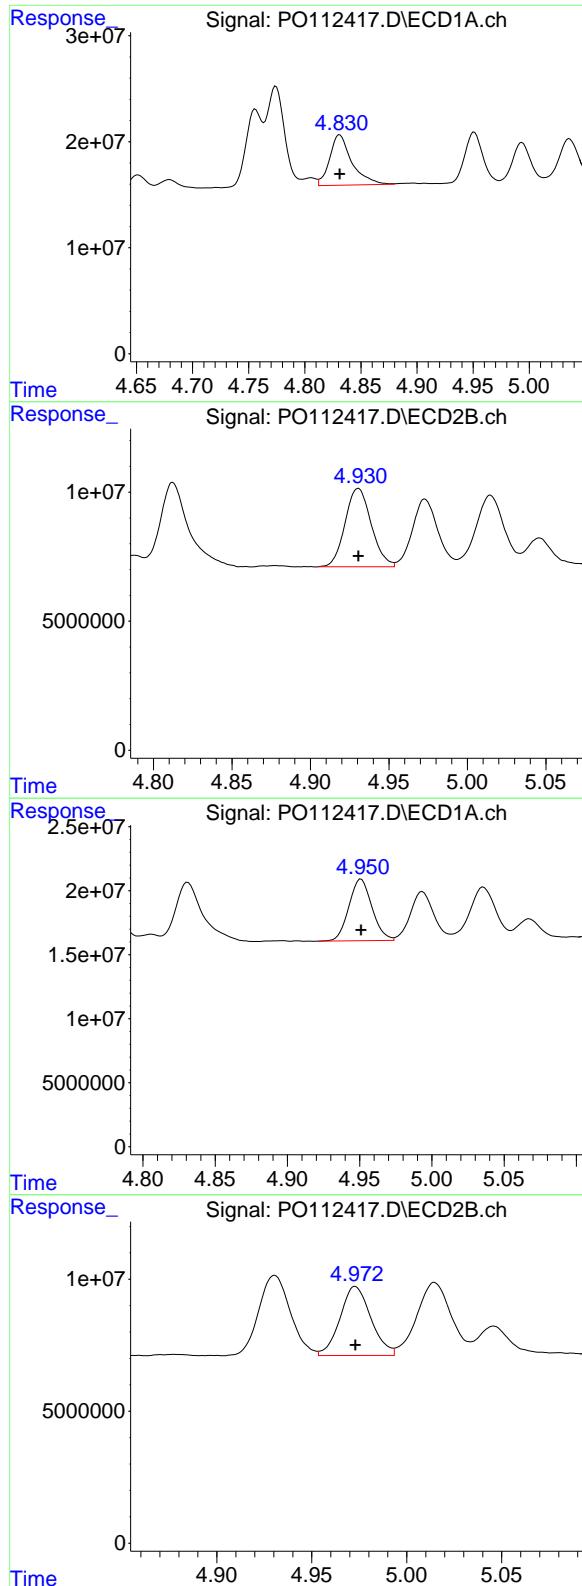

#5 AR-1016-3

R.T.: 4.831 min
 Delta R.T.: 0.000 min
 Response: 65721962
 Conc: 244.79 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#5 AR-1016-3


R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 35251812
 Conc: 253.03 ng/ml

#6 AR-1016-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 53435135
 Conc: 244.97 ng/ml

#6 AR-1016-4

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 29674672
 Conc: 262.05 ng/ml

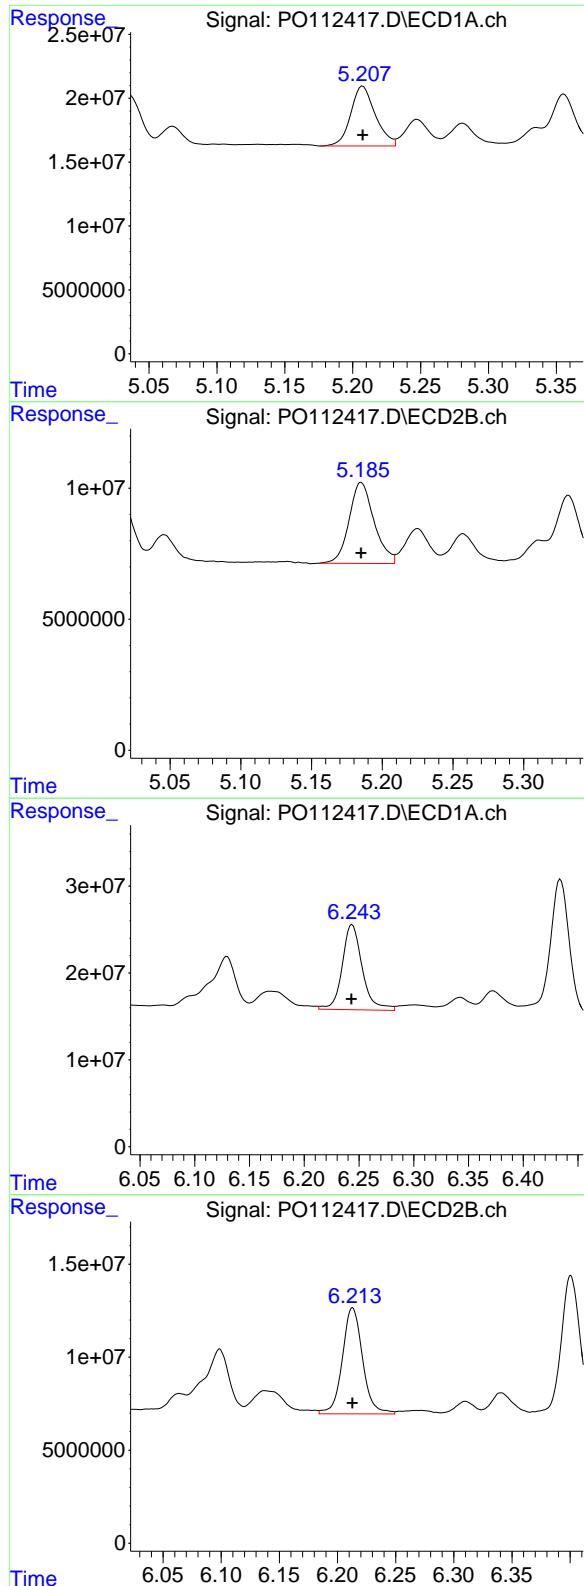

#7 AR-1016-5

R.T.: 5.207 min
 Delta R.T.: 0.000 min
 Response: 58842499
 Conc: 256.22 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#7 AR-1016-5


R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 38084113
 Conc: 260.76 ng/ml

#31 AR-1260-1

R.T.: 6.244 min
 Delta R.T.: 0.000 min
 Response: 125178335
 Conc: 277.53 ng/ml

#31 AR-1260-1


R.T.: 6.213 min
 Delta R.T.: 0.000 min
 Response: 69330497
 Conc: 268.52 ng/ml

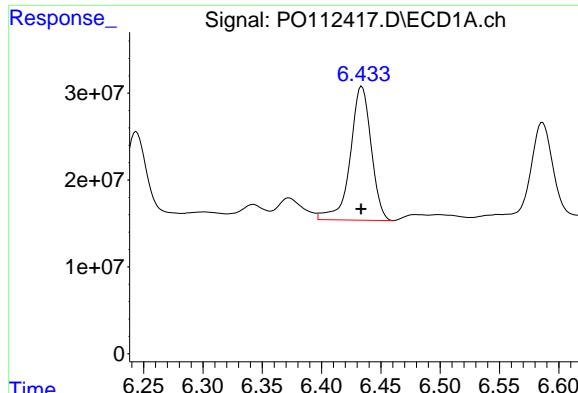

#32 AR-1260-2


R.T.: 6.434 min
 Delta R.T.: 0.000 min
 Response: 189593196
 Conc: 272.94 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

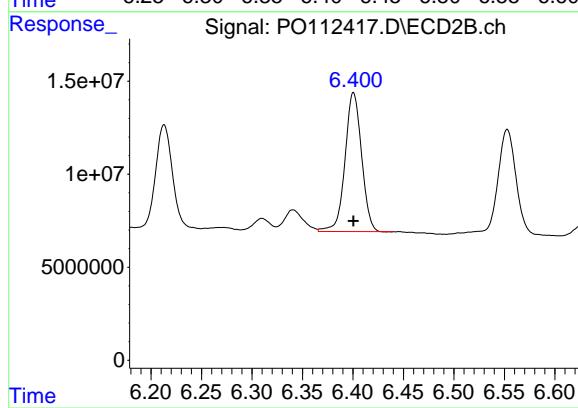


#32 AR-1260-2

R.T.: 6.401 min
 Delta R.T.: 0.000 min
 Response: 85155201
 Conc: 257.56 ng/ml

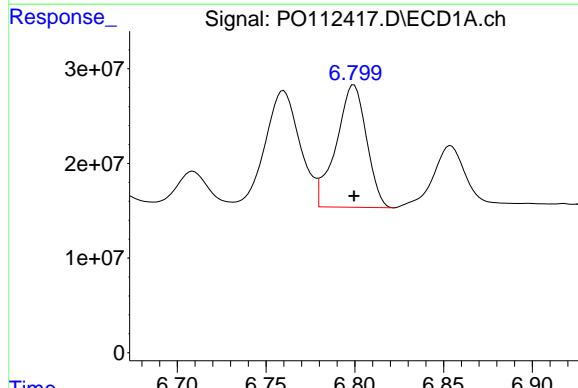


#33 AR-1260-3

R.T.: 6.800 min
 Delta R.T.: 0.000 min
 Response: 153678285
 Conc: 249.52 ng/ml

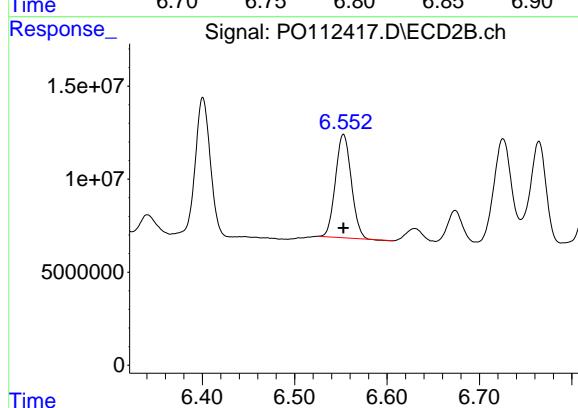

#33 AR-1260-3

R.T.: 6.553 min
 Delta R.T.: 0.000 min
 Response: 66184896
 Conc: 251.42 ng/ml

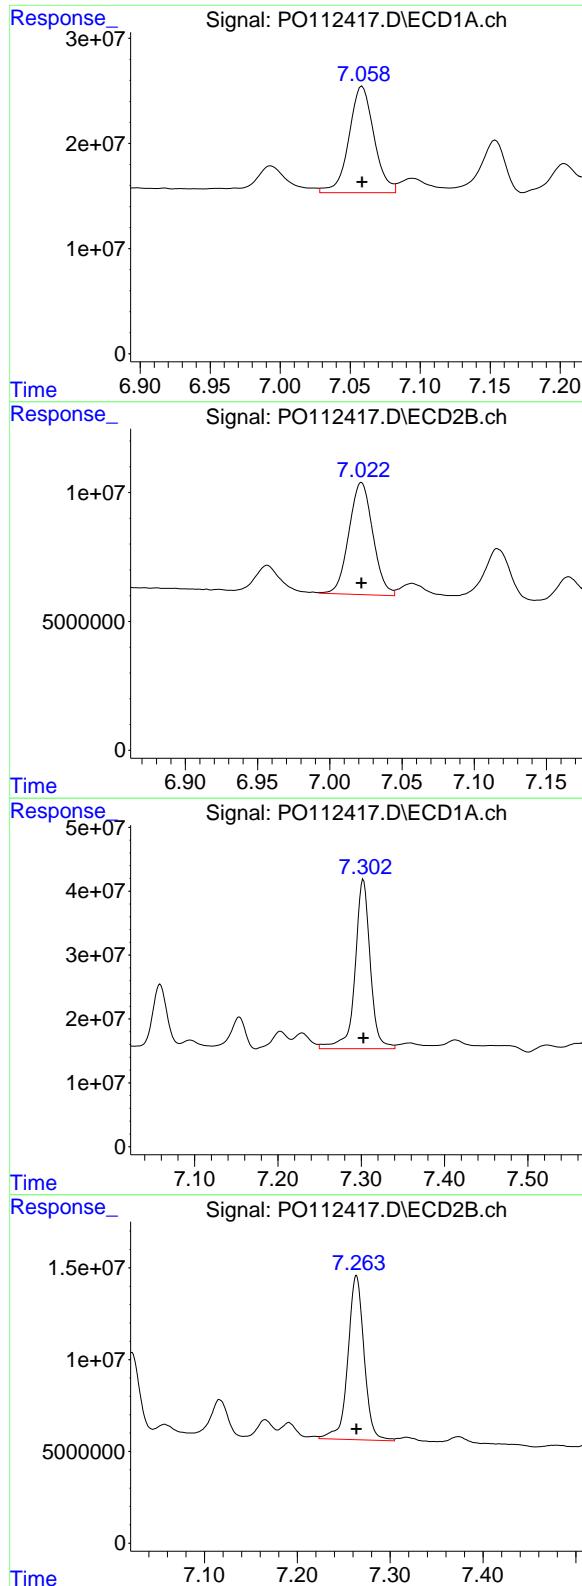

#34 AR-1260-4

R.T.: 7.059 min
 Delta R.T.: 0.000 min
 Response: 126280400
 Conc: 267.73 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC250

#34 AR-1260-4

R.T.: 7.022 min
 Delta R.T.: 0.000 min
 Response: 50234042
 Conc: 258.47 ng/ml

#35 AR-1260-5

R.T.: 7.302 min
 Delta R.T.: 0.000 min
 Response: 336866700
 Conc: 257.58 ng/ml

#35 AR-1260-5

R.T.: 7.264 min
 Delta R.T.: 0.000 min
 Response: 108703906
 Conc: 254.47 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:45
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:01:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 13:01:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 31417194 | 19597973 | 3.883 | 3.906 |
| 2) SA Decachlor... | 8.693 | 8.640 | 29621580 | 7457220 | 4.051 | 4.220 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|--------|--------|
| 3) L1 AR-1016-1 | 4.756 | 4.737 | 10242412 | 8280603 | 38.166 | 47.316 |
| 4) L1 AR-1016-2 | 4.774 | 4.756 | 16308940 | 11816564 | 40.158 | 45.362 |
| 5) L1 AR-1016-3 | 4.832 | 4.931 | 11721947 | 6127662 | 44.796 | 45.067 |
| 6) L1 AR-1016-4 | 4.951 | 4.973 | 9335010 | 5123227 | 44.066 | 46.120 |
| 7) L1 AR-1016-5 | 5.208 | 5.185 | 15148752 | 7917067 | 69.940 | 55.630 |
| 31) L7 AR-1260-1 | 6.245 | 6.213 | 19551344 | 13747865 | 44.503 | 53.350 |
| 32) L7 AR-1260-2 | 6.434 | 6.402 | 32919190 | 16247800 | 47.855 | 49.311 |
| 33) L7 AR-1260-3 | 6.801 | 6.553 | 23827559 | 9733666 | 40.522 | 38.662 |
| 34) L7 AR-1260-4 | 7.060 | 7.022 | 18415991 | 8957569 | 40.833 | 46.822 |
| 35) L7 AR-1260-5 | 7.303 | 7.265 | 48222745 | 17614159 | 38.916 | 42.733 |
| 36) L8 AR-1262-1 | 6.801 | 6.764 | 23827559 | 12127374 | 50.000 | 50.000 |
| 37) L8 AR-1262-2 | 7.303 | 7.265 | 48222745 | 17614159 | 50.000 | 50.000 |
| 38) L8 AR-1262-3 | 7.585 | 7.545 | 16287328 | 4284383 | 50.000 | 50.000 |
| 39) L8 AR-1262-4 | 7.649 | 7.608 | 35754287 | 10013446 | 50.000 | 50.000 |
| 40) L8 AR-1262-5 | 8.146 | 8.102 | 14312589 | 2665703 | 50.000 | 50.000 |
| 41) L9 AR-1268-1 | 7.585 | 7.545 | 16287328 | 4284383 | 50.000 | 50.000 |
| 42) L9 AR-1268-2 | 7.649 | 7.608 | 35754287 | 10013446 | 50.000 | 50.000 |
| 43) L9 AR-1268-3 | 7.855 | 7.818 | -141825 | -8046 | 50.000 | 50.000 |
| 44) L9 AR-1268-4 | 8.146 | 8.102 | 14312589 | 2665703 | 50.000 | 50.000 |
| 45) L9 AR-1268-5 | 8.440 | 8.387 | 3715372 | 692132 | 50.000 | 50.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 12:45
 Operator : YP/AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 13:01:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 13:01:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

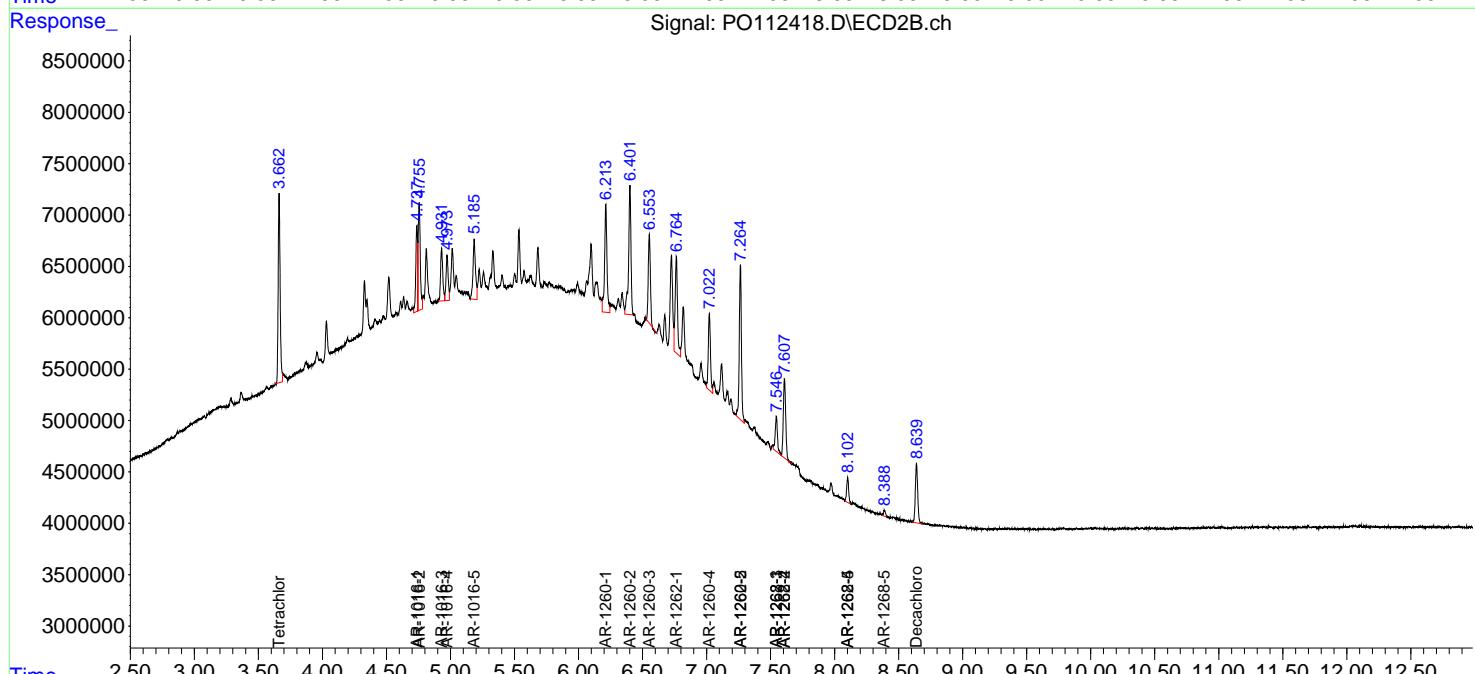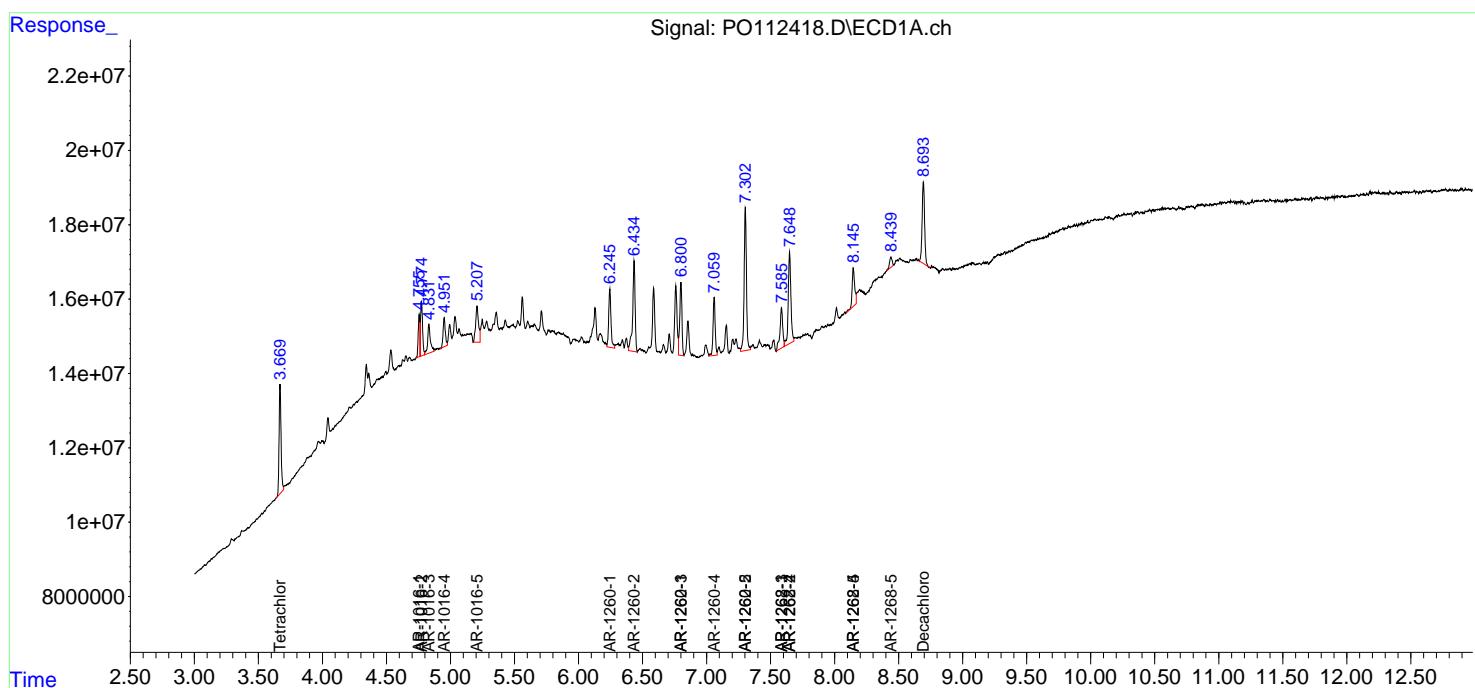

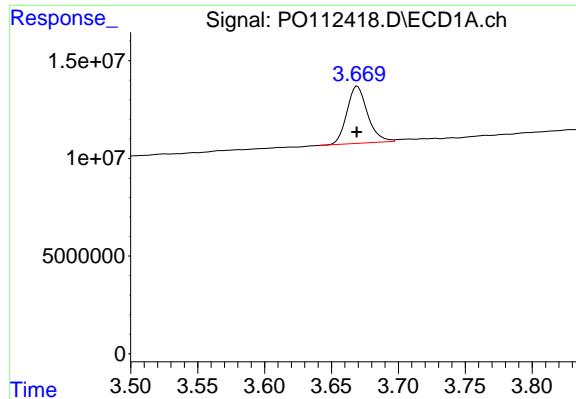


#1 Tetrachloro-m-xylene
R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 31417194
Conc: 3.88 ng/ml


Instrument: ECD_O
ClientSampleId: AR1660ICC050

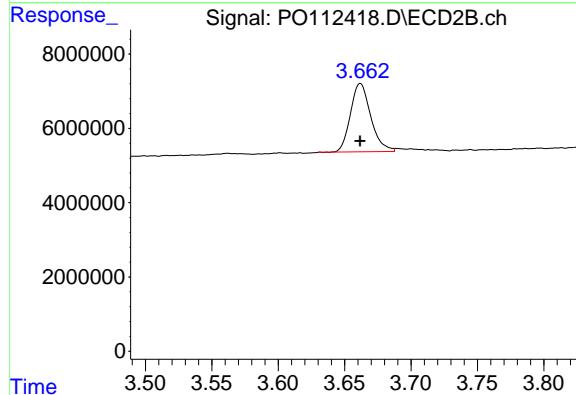


#1 Tetrachloro-m-xylene
R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 19597973
Conc: 3.91 ng/ml

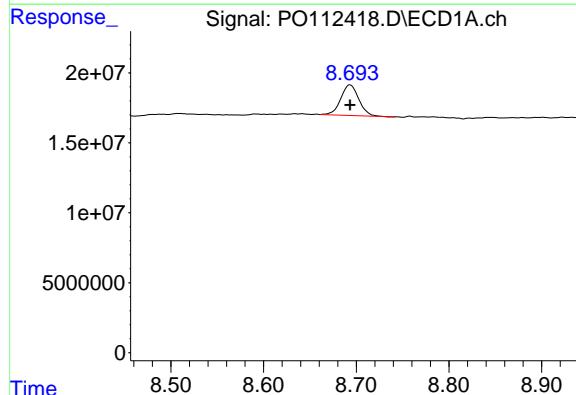

#2 Decachlorobiphenyl
R.T.: 8.693 min
Delta R.T.: 0.000 min
Response: 29621580
Conc: 4.05 ng/ml

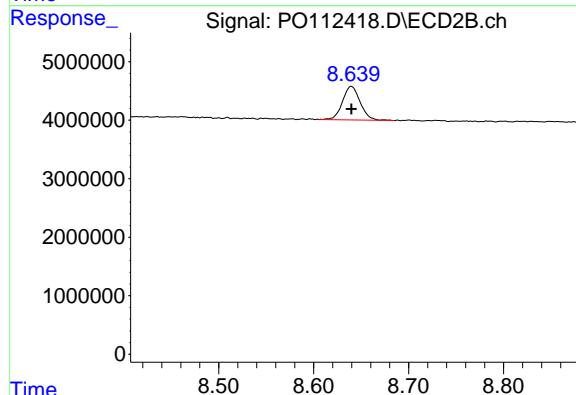

#2 Decachlorobiphenyl
R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 7457220
Conc: 4.22 ng/ml

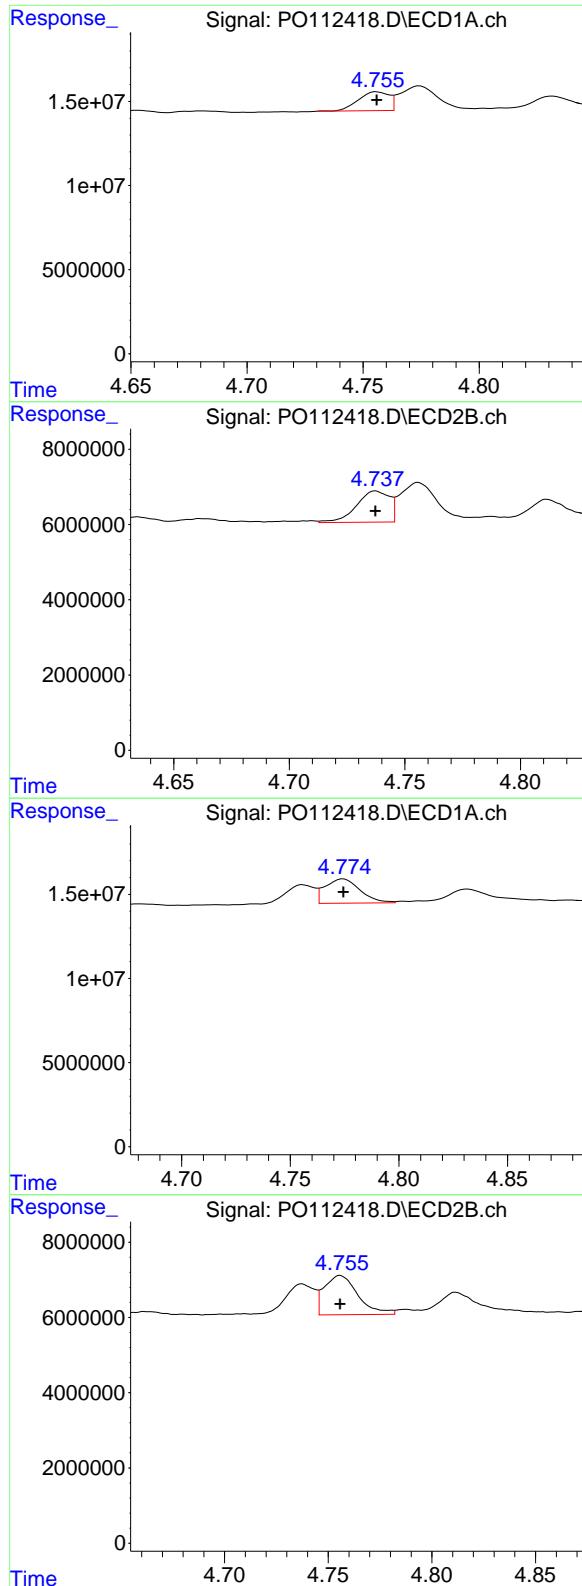

#3 AR-1016-1

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 10242412
 Conc: 38.17 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC050

#3 AR-1016-1


R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 8280603
 Conc: 47.32 ng/ml

#4 AR-1016-2

R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 16308940
 Conc: 40.16 ng/ml

#4 AR-1016-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 11816564
 Conc: 45.36 ng/ml

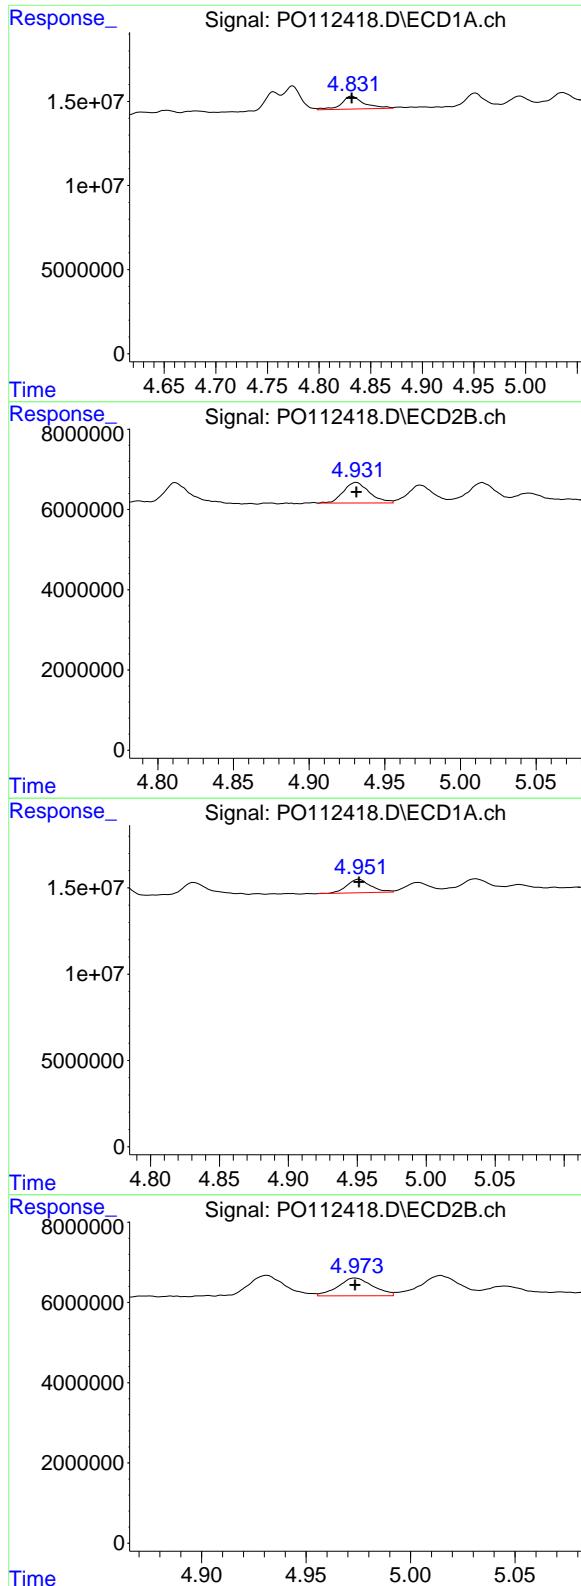

#5 AR-1016-3

R.T.: 4.832 min
 Delta R.T.: 0.000 min
 Response: 11721947
 Conc: 44.80 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

#5 AR-1016-3


R.T.: 4.931 min
 Delta R.T.: 0.000 min
 Response: 6127662
 Conc: 45.07 ng/ml

#6 AR-1016-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 9335010
 Conc: 44.07 ng/ml

#6 AR-1016-4

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 5123227
 Conc: 46.12 ng/ml

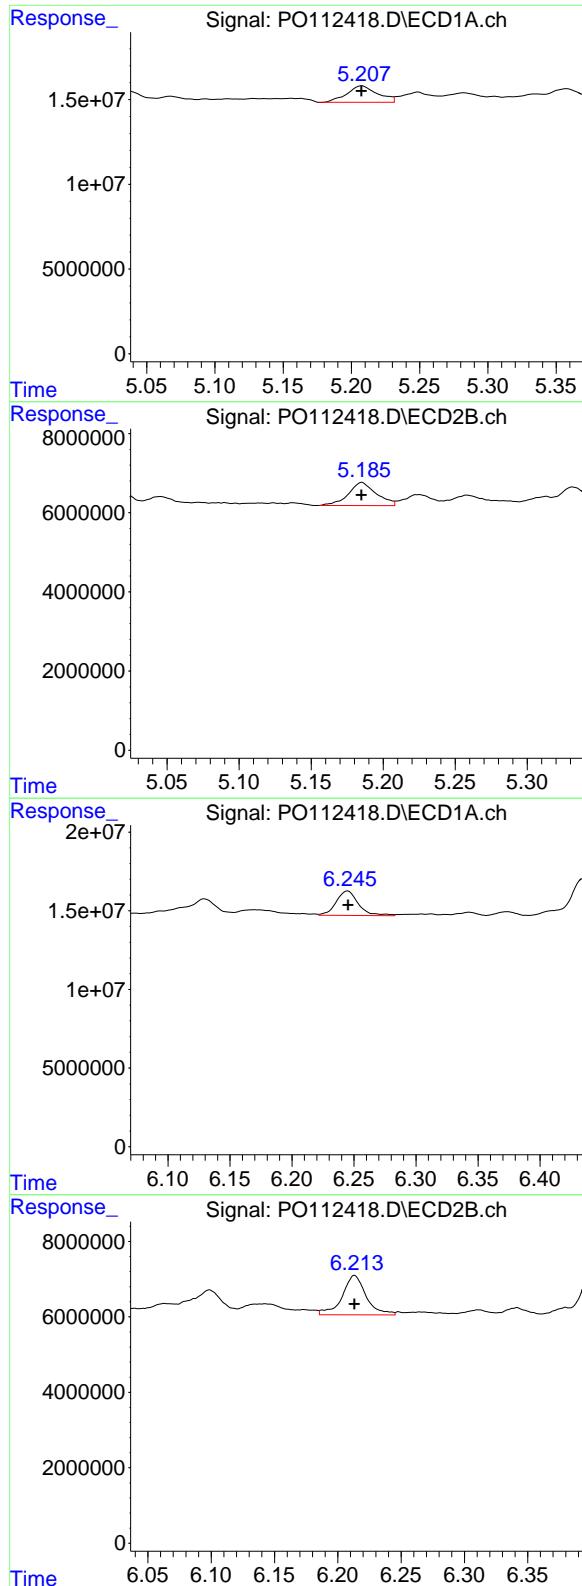

#7 AR-1016-5

R.T.: 5.208 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 15148752 ECD_O
 Conc: 69.94 ng/ml **ClientSampleId:**
 AR1660ICC050

#7 AR-1016-5


R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 7917067
 Conc: 55.63 ng/ml

#31 AR-1260-1

R.T.: 6.245 min
 Delta R.T.: 0.000 min
 Response: 19551344
 Conc: 44.50 ng/ml

#31 AR-1260-1

R.T.: 6.213 min
 Delta R.T.: 0.000 min
 Response: 13747865
 Conc: 53.35 ng/ml

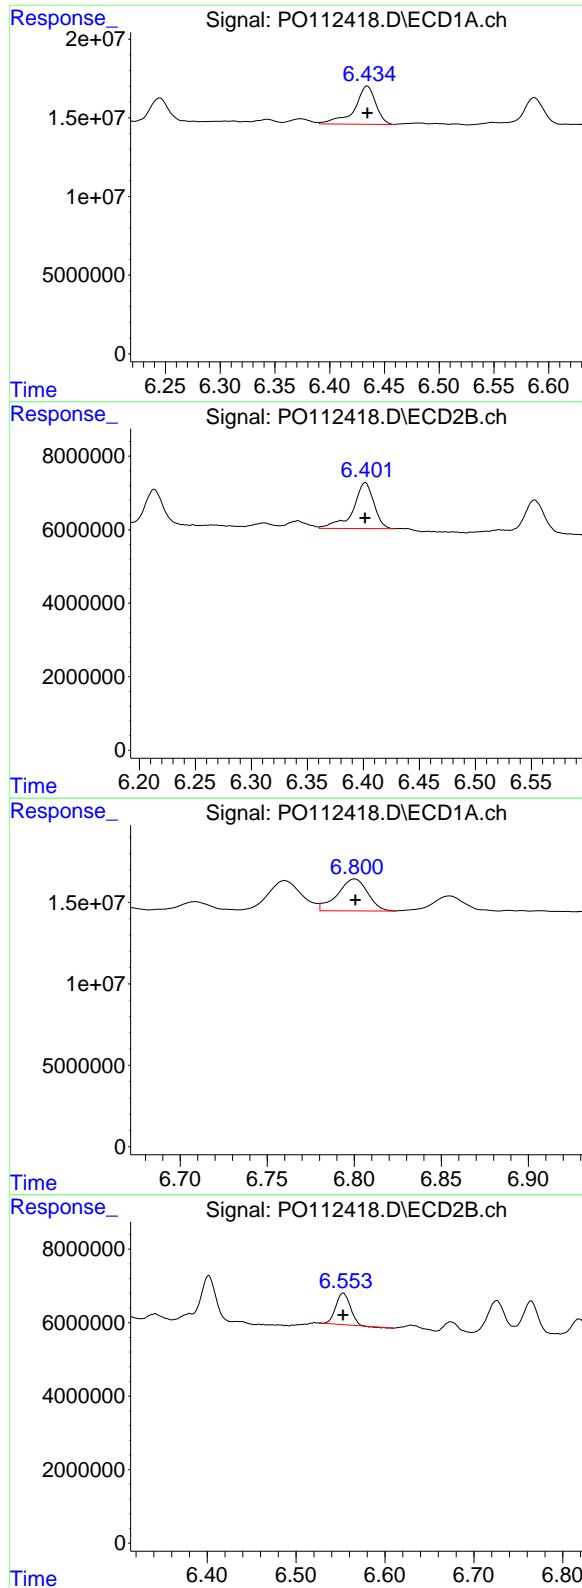

#32 AR-1260-2

R.T.: 6.434 min
 Delta R.T.: 0.000 min
 Response: 32919190
 Conc: 47.86 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC050

#32 AR-1260-2


R.T.: 6.402 min
 Delta R.T.: 0.000 min
 Response: 16247800
 Conc: 49.31 ng/ml

#33 AR-1260-3

R.T.: 6.801 min
 Delta R.T.: 0.000 min
 Response: 23827559
 Conc: 40.52 ng/ml

#33 AR-1260-3

R.T.: 6.553 min
 Delta R.T.: 0.000 min
 Response: 9733666
 Conc: 38.66 ng/ml

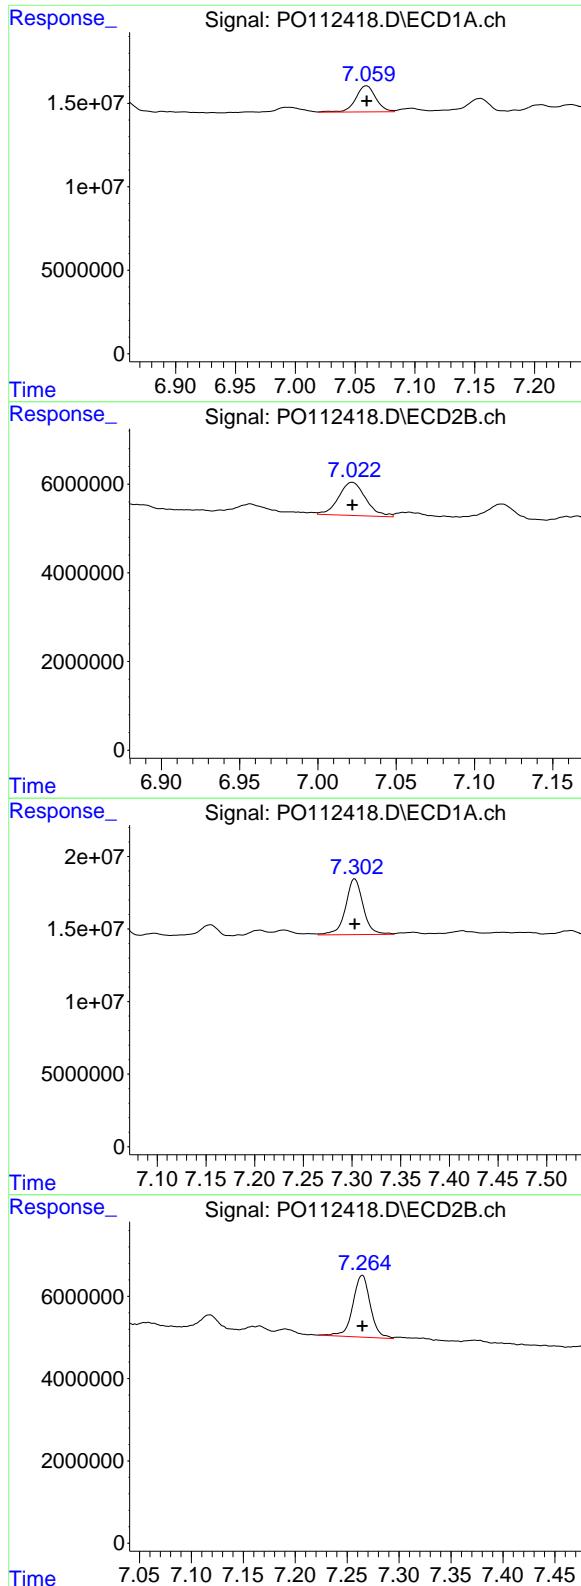

#34 AR-1260-4

R.T.: 7.060 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 18415991 ECD_O
 Conc: 40.83 ng/ml **ClientSampleId:**
 AR1660ICC050

#34 AR-1260-4


R.T.: 7.022 min
 Delta R.T.: 0.000 min
 Response: 8957569
 Conc: 46.82 ng/ml

#35 AR-1260-5

R.T.: 7.303 min
 Delta R.T.: 0.000 min
 Response: 48222745
 Conc: 38.92 ng/ml

#35 AR-1260-5


R.T.: 7.265 min
 Delta R.T.: 0.000 min
 Response: 17614159
 Conc: 42.73 ng/ml



#36 AR-1262-1


R.T.: 6.801 min
Delta R.T.: 0.000 min
Response: 23827559
Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

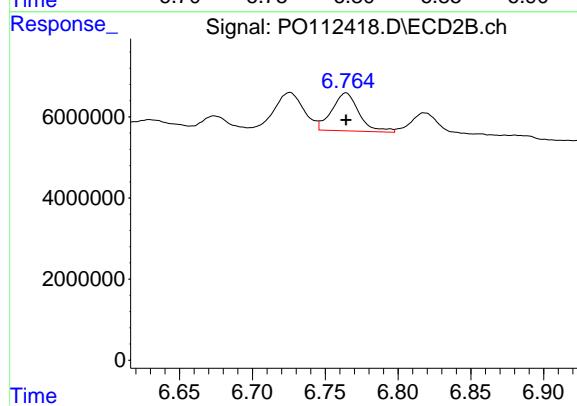


#36 AR-1262-1

R.T.: 6.764 min
Delta R.T.: 0.000 min
Response: 12127374
Conc: 50.00 ng/ml

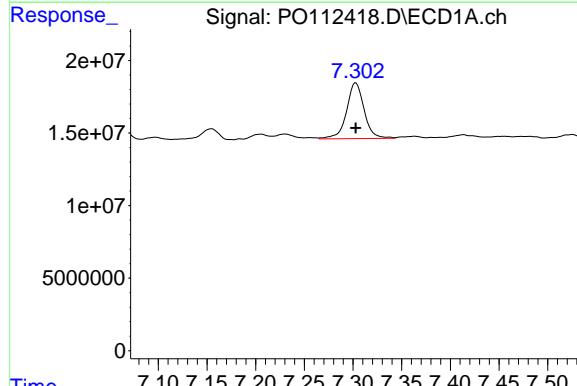


#37 AR-1262-2

R.T.: 7.303 min
Delta R.T.: 0.000 min
Response: 48222745
Conc: 50.00 ng/ml

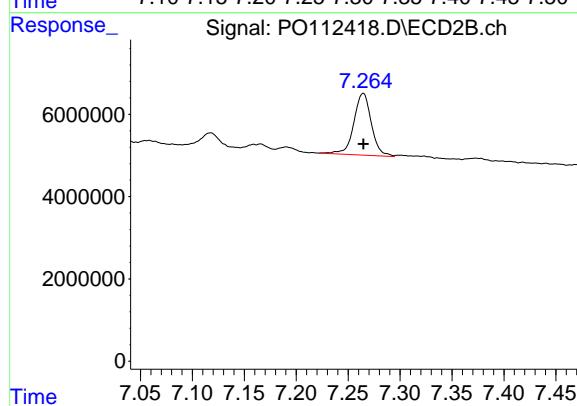

#37 AR-1262-2

R.T.: 7.265 min
Delta R.T.: 0.000 min
Response: 17614159
Conc: 50.00 ng/ml

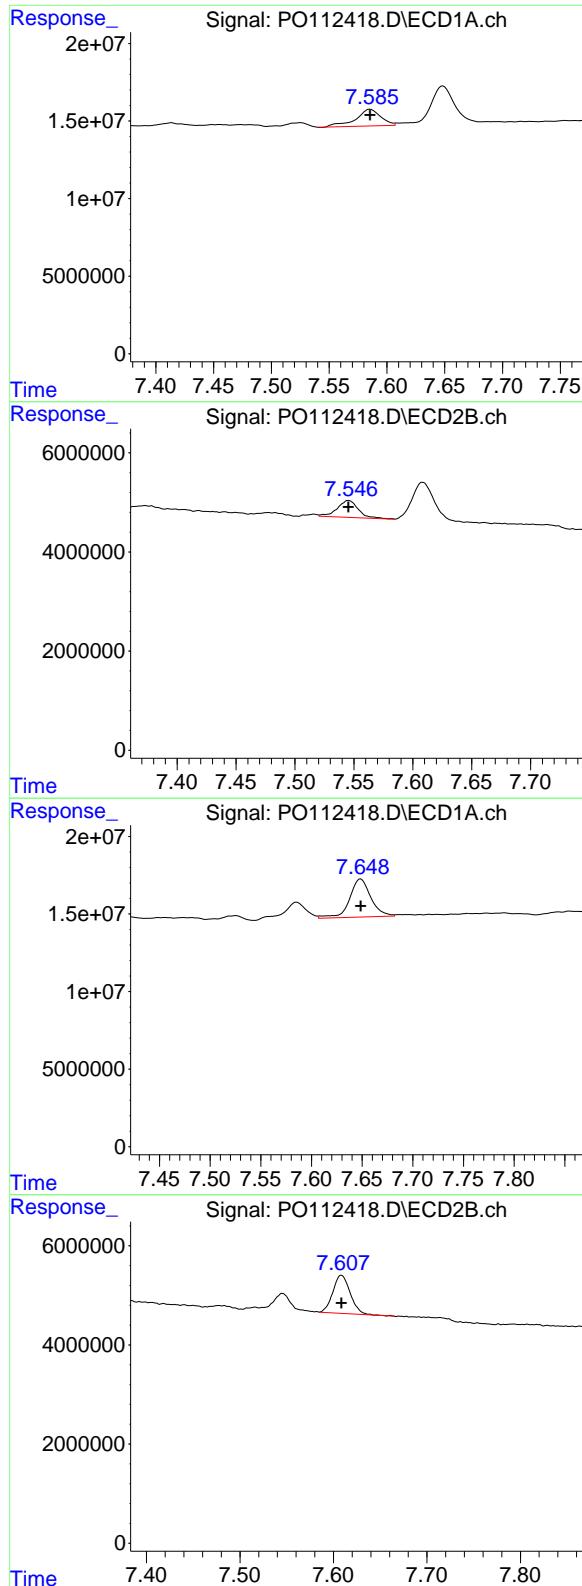

#38 AR-1262-3

R.T.: 7.585 min
 Delta R.T.: 0.000 min
 Response: 16287328
 Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

#38 AR-1262-3


R.T.: 7.545 min
 Delta R.T.: 0.000 min
 Response: 4284383
 Conc: 50.00 ng/ml

#39 AR-1262-4

R.T.: 7.649 min
 Delta R.T.: 0.000 min
 Response: 35754287
 Conc: 50.00 ng/ml

#39 AR-1262-4

R.T.: 7.608 min
 Delta R.T.: 0.000 min
 Response: 10013446
 Conc: 50.00 ng/ml

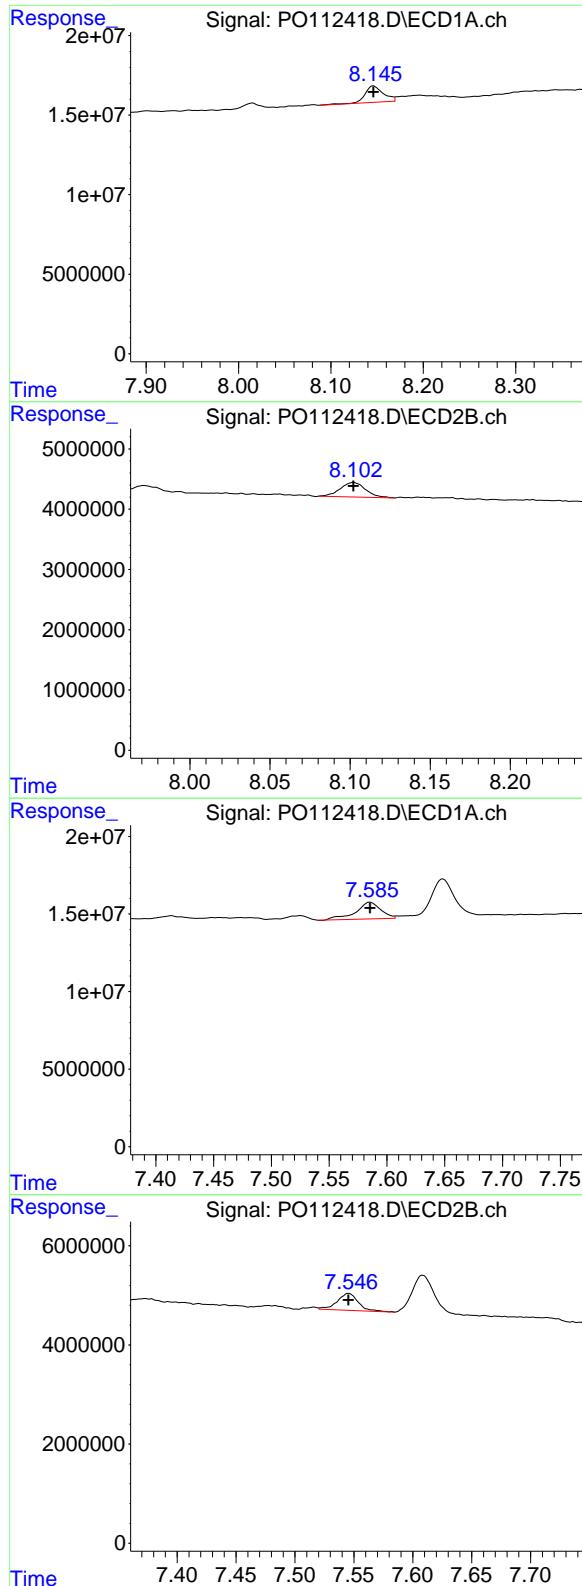

#40 AR-1262-5

R.T.: 8.146 min
 Delta R.T.: 0.000 min
 Response: 14312589
 Conc: 50.00 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660ICC050

#40 AR-1262-5


R.T.: 8.102 min
 Delta R.T.: 0.000 min
 Response: 2665703
 Conc: 50.00 ng/ml

#41 AR-1268-1

R.T.: 7.585 min
 Delta R.T.: 0.000 min
 Response: 16287328
 Conc: 50.00 ng/ml

#41 AR-1268-1

R.T.: 7.545 min
 Delta R.T.: 0.000 min
 Response: 4284383
 Conc: 50.00 ng/ml

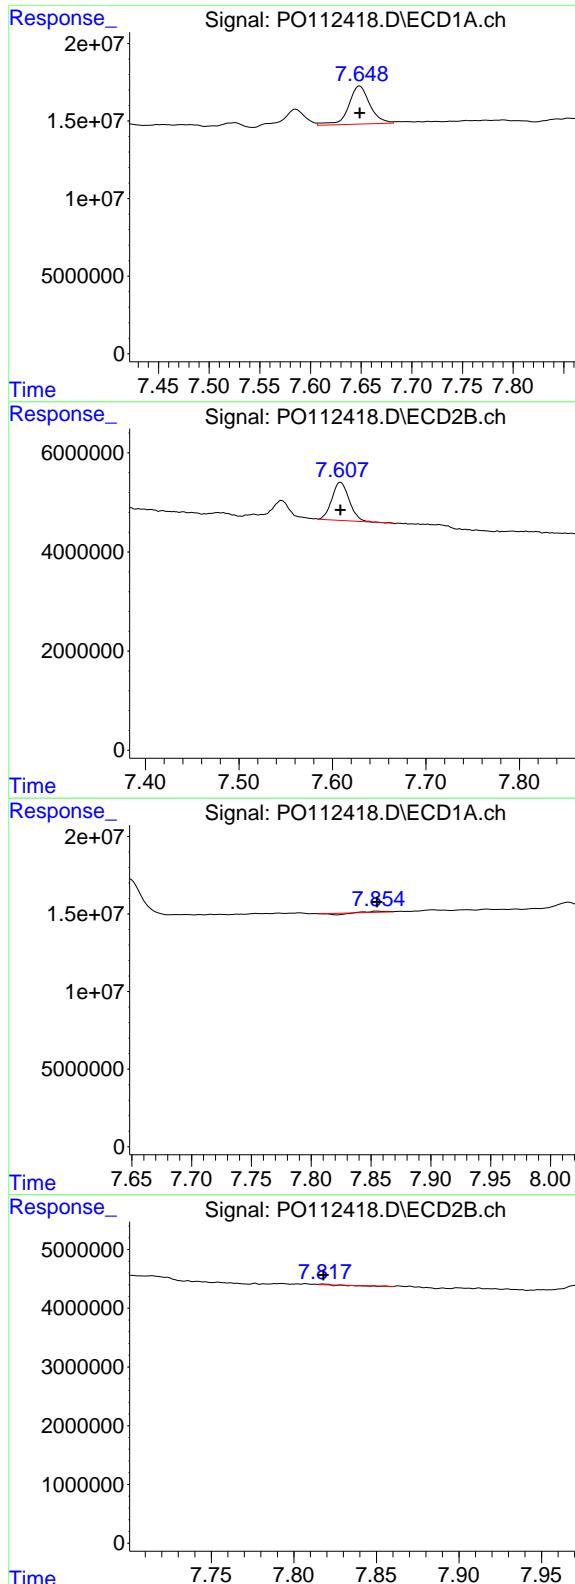

#42 AR-1268-2

R.T.: 7.649 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 35754287 ECD_O
 Conc: 50.00 ng/ml **ClientSampleId:**
 AR1660ICC050

#42 AR-1268-2


R.T.: 7.608 min
 Delta R.T.: 0.000 min
 Response: 10013446
 Conc: 50.00 ng/ml

#43 AR-1268-3

R.T.: 7.855 min
 Delta R.T.: 0.000 min
 Response: -141825
 Conc: 50.00 ng/ml

#43 AR-1268-3


R.T.: 7.818 min
 Delta R.T.: 0.000 min
 Response: -8046
 Conc: 50.00 ng/ml

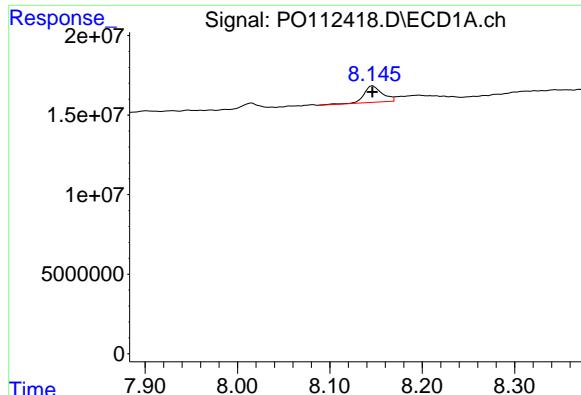

#44 AR-1268-4


R.T.: 8.146 min
Delta R.T.: 0.000 min
Response: 14312589
Conc: 50.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660ICC050

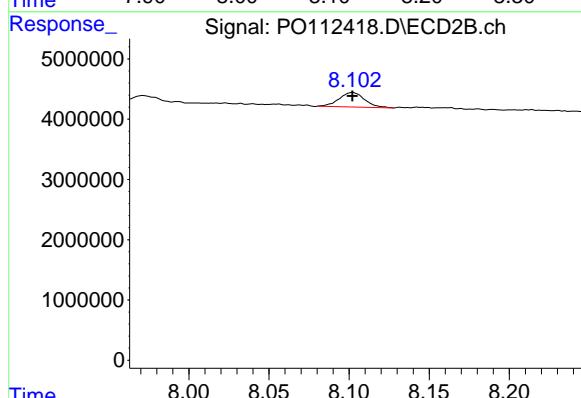


#44 AR-1268-4

R.T.: 8.102 min
Delta R.T.: 0.000 min
Response: 2665703
Conc: 50.00 ng/ml

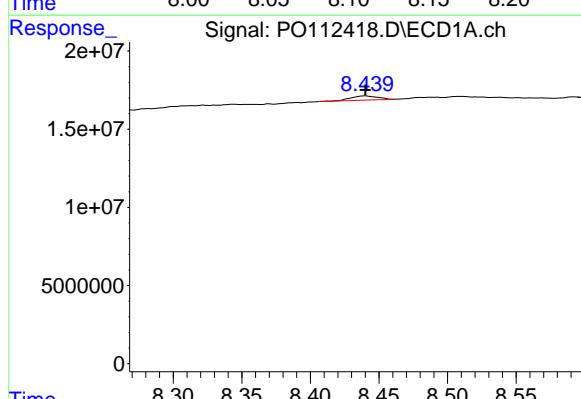

#45 AR-1268-5

R.T.: 8.440 min
Delta R.T.: 0.000 min
Response: 3715372
Conc: 50.00 ng/ml

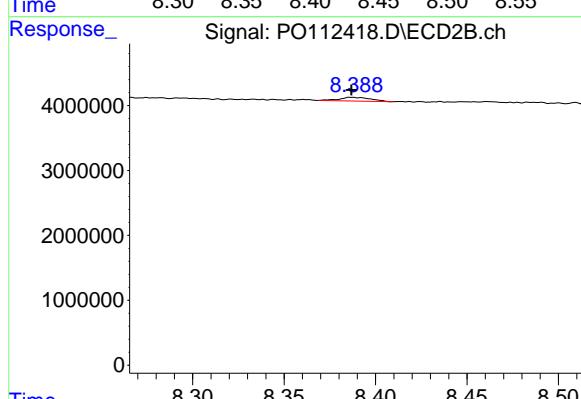

#45 AR-1268-5

R.T.: 8.387 min
Delta R.T.: 0.000 min
Response: 692132
Conc: 50.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:36
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:50:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:50:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.669 | 3.662 | 230.2E6 | 140.8E6 | 25.056 | 25.329 |
| 2) SA Decachlor... | 8.692 | 8.640 | 202.2E6 | 49177998 | 25.104 | 25.901 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 16) L4 AR-1242-1 | 4.756 | 4.737 | 66274294 | 42281301 | 254.503 | 262.921 |
| 17) L4 AR-1242-2 | 4.774 | 4.756 | 98384229 | 63307827 | 253.352 | 263.280 |
| 18) L4 AR-1242-3 | 4.830 | 4.930 | 63048920 | 32586963 | 255.064 | 259.362 |
| 19) L4 AR-1242-4 | 4.951 | 5.015 | 50849599 | 32274308 | 254.552 | 262.925 |
| 20) L4 AR-1242-5 | 5.601 | 5.535 | 60576839 | 45188557 | 277.078 | 279.805 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:36
 Operator : YP/AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 14:50:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 14:50:26 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

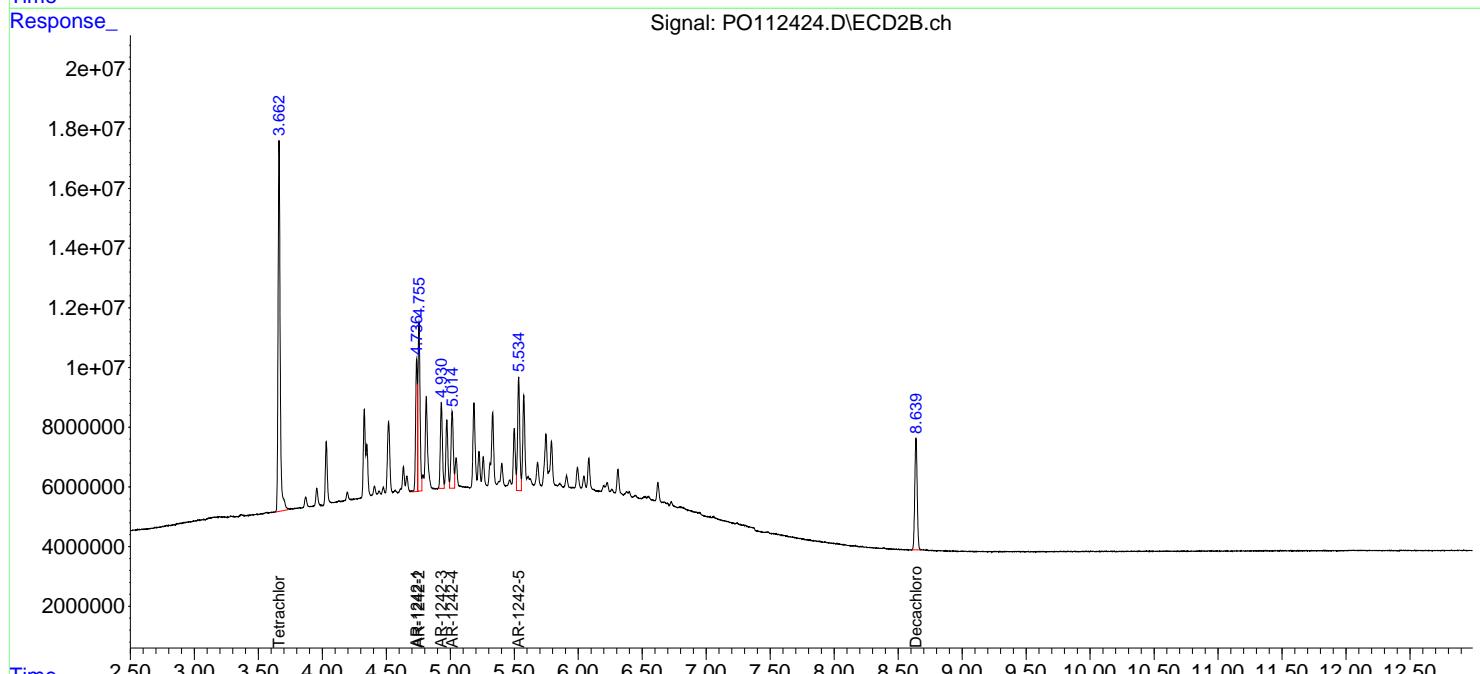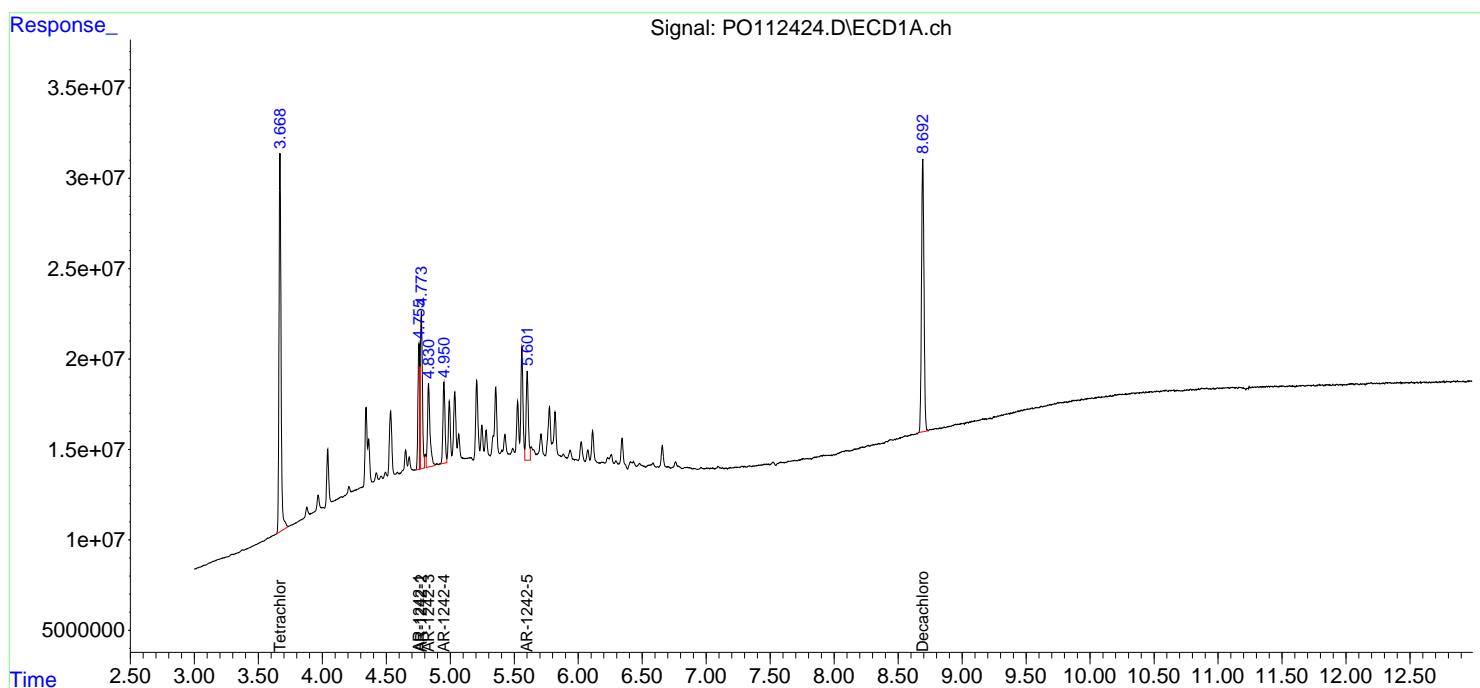



#1 Tetrachloro-m-xylene


R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 230185927
Conc: 25.06 ng/ml

Instrument:

ECD_O


ClientSampleId :

AR1242ICC250

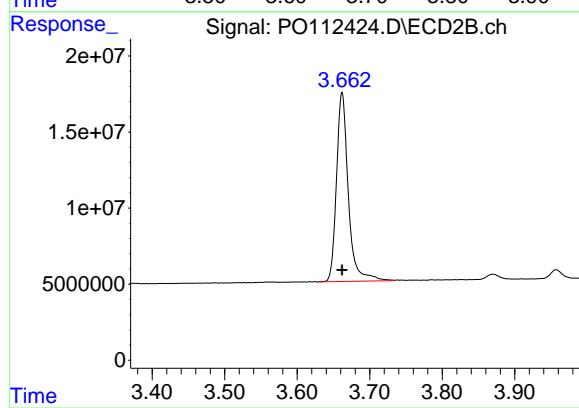


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 140771642
Conc: 25.33 ng/ml

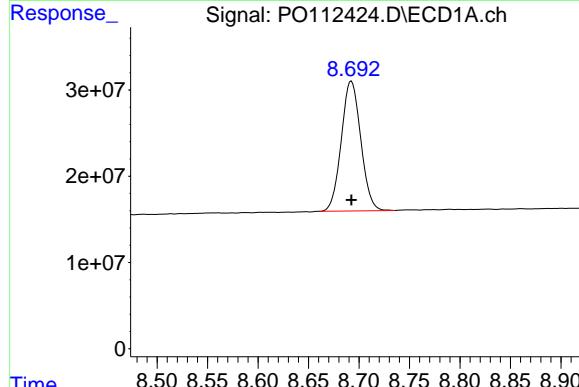


#2 Decachlorobiphenyl

R.T.: 8.692 min
Delta R.T.: 0.000 min
Response: 202170823
Conc: 25.10 ng/ml

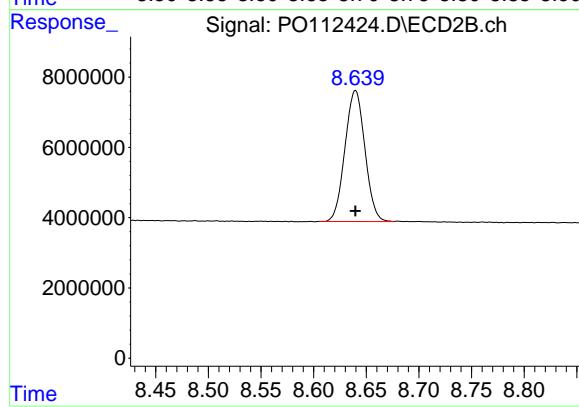

#2 Decachlorobiphenyl


R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 49177998
Conc: 25.90 ng/ml



#16 AR-1242-1


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 66274294
 Conc: 254.50 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC250

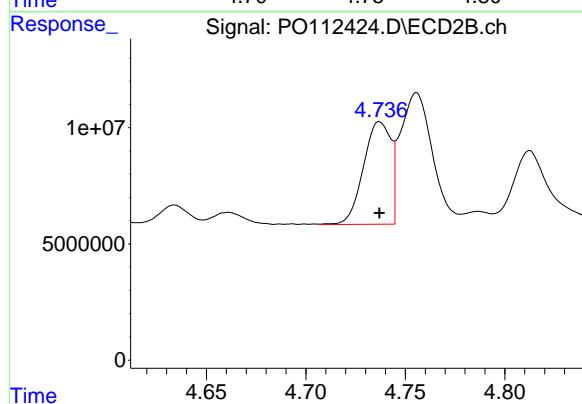


#16 AR-1242-1

R.T.: 4.737 min
 Delta R.T.: 0.000 min
 Response: 42281301
 Conc: 262.92 ng/ml

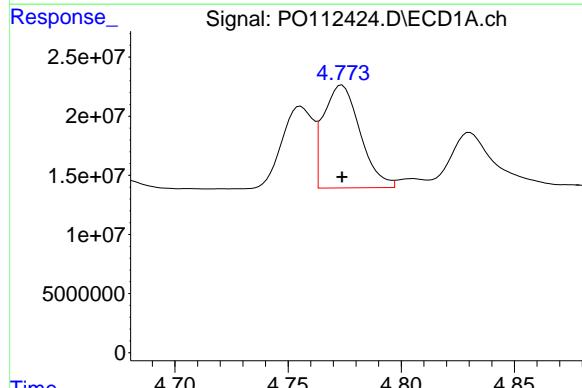


#17 AR-1242-2

R.T.: 4.774 min
 Delta R.T.: 0.000 min
 Response: 98384229
 Conc: 253.35 ng/ml

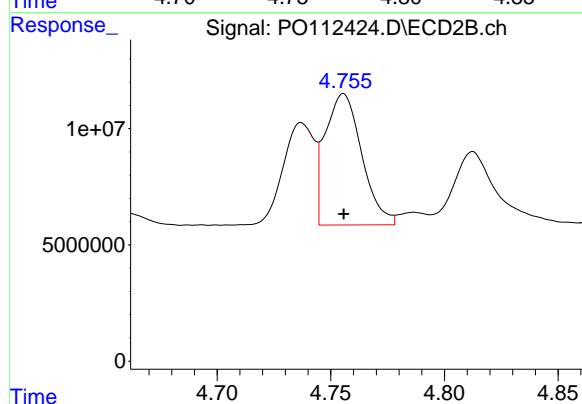

#17 AR-1242-2

R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 63307827
 Conc: 263.28 ng/ml

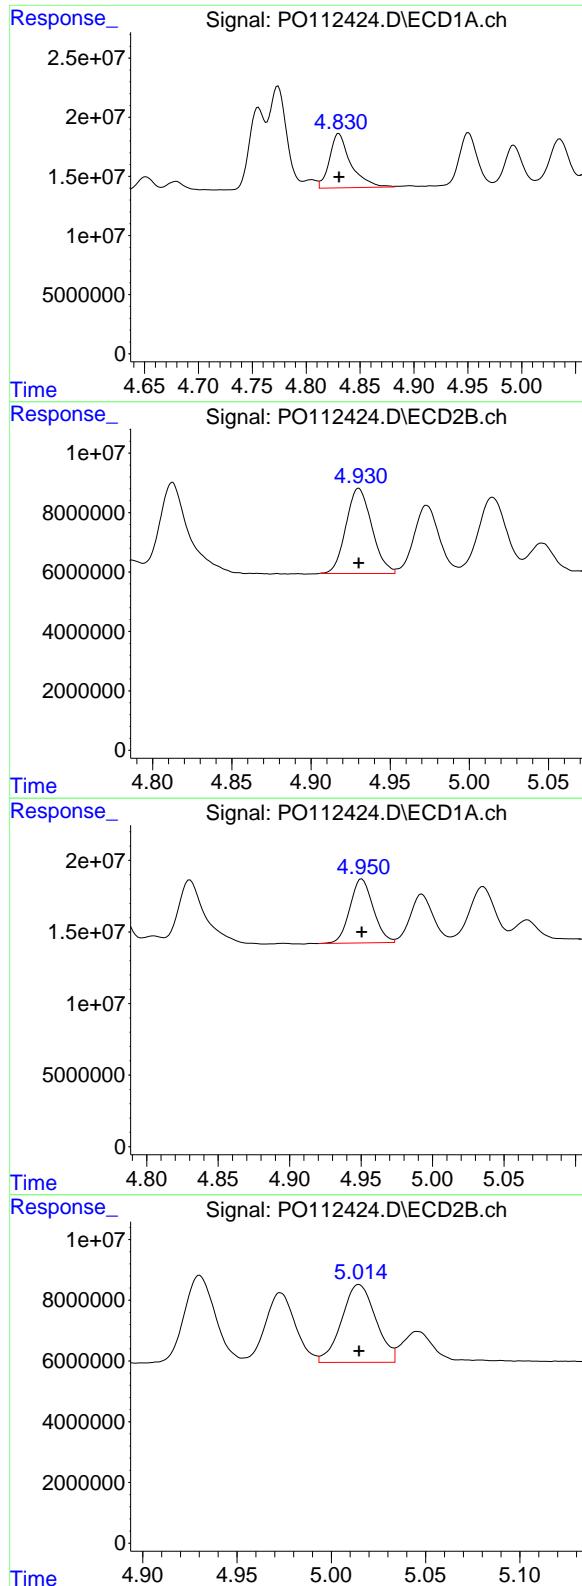

#18 AR-1242-3

R.T.: 4.830 min
 Delta R.T.: 0.000 min
 Response: 63048920
 Conc: 255.06 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC250

#18 AR-1242-3


R.T.: 4.930 min
 Delta R.T.: 0.000 min
 Response: 32586963
 Conc: 259.36 ng/ml

#19 AR-1242-4

R.T.: 4.951 min
 Delta R.T.: 0.000 min
 Response: 50849599
 Conc: 254.55 ng/ml

#19 AR-1242-4

R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 32274308
 Conc: 262.93 ng/ml

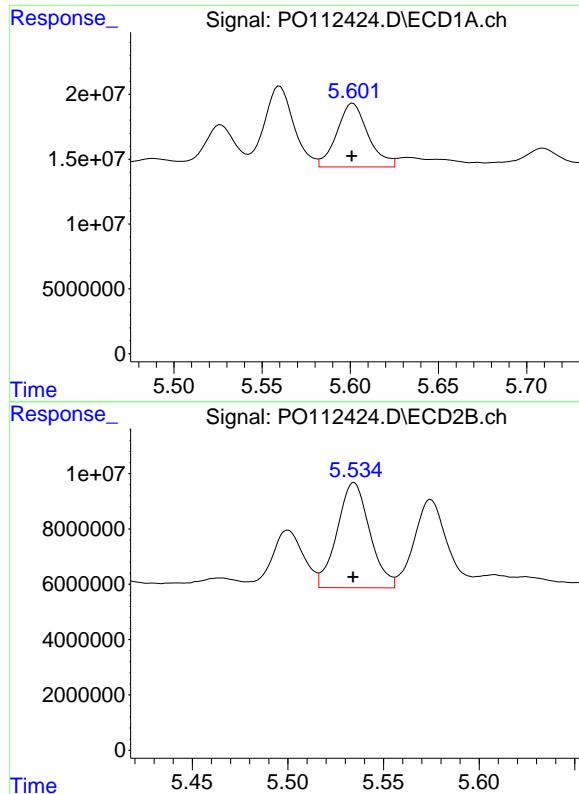

#20 AR-1242-5

R.T.: 5.601 min
Delta R.T.: 0.000 min
Response: 60576839
Conc: 277.08 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC250

#20 AR-1242-5

R.T.: 5.535 min
Delta R.T.: 0.000 min
Response: 45188557
Conc: 279.80 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:54
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 15:07:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 15:07:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 31709040 | 19454228 | 3.679 | 3.698 |
| 2) SA Decachlor... | 8.695 | 8.640 | 31949919 | 7899252 | 4.138 | 4.305 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|--------|--------|
| 16) L4 AR-1242-1 | 4.757 | 4.738 | 9816709 | 7435731 | 39.649 | 46.945 |
| 17) L4 AR-1242-2 | 4.776 | 4.756 | 14782408 | 10324894 | 39.975 | 44.186 |
| 18) L4 AR-1242-3 | 4.833 | 4.932 | 9726638 | 5168677 | 41.100 | 42.650 |
| 19) L4 AR-1242-4 | 4.952 | 5.016 | 8617431 | 6134656 | 44.356 | 49.981 |
| 20) L4 AR-1242-5 | 5.604 | 5.535 | 15882894 | 12714804 | 75.361 | 77.938 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112425.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 14:54
 Operator : YP/AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 15:07:13 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 15:07:00 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

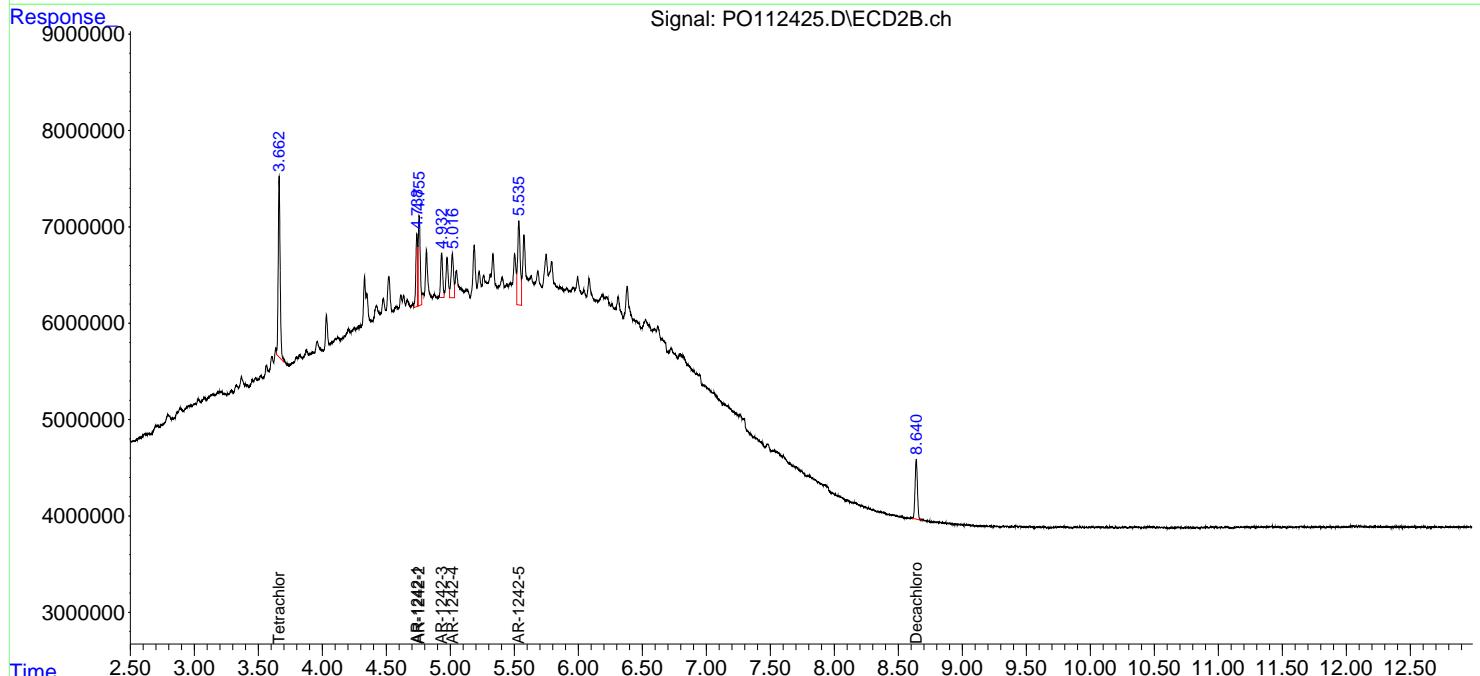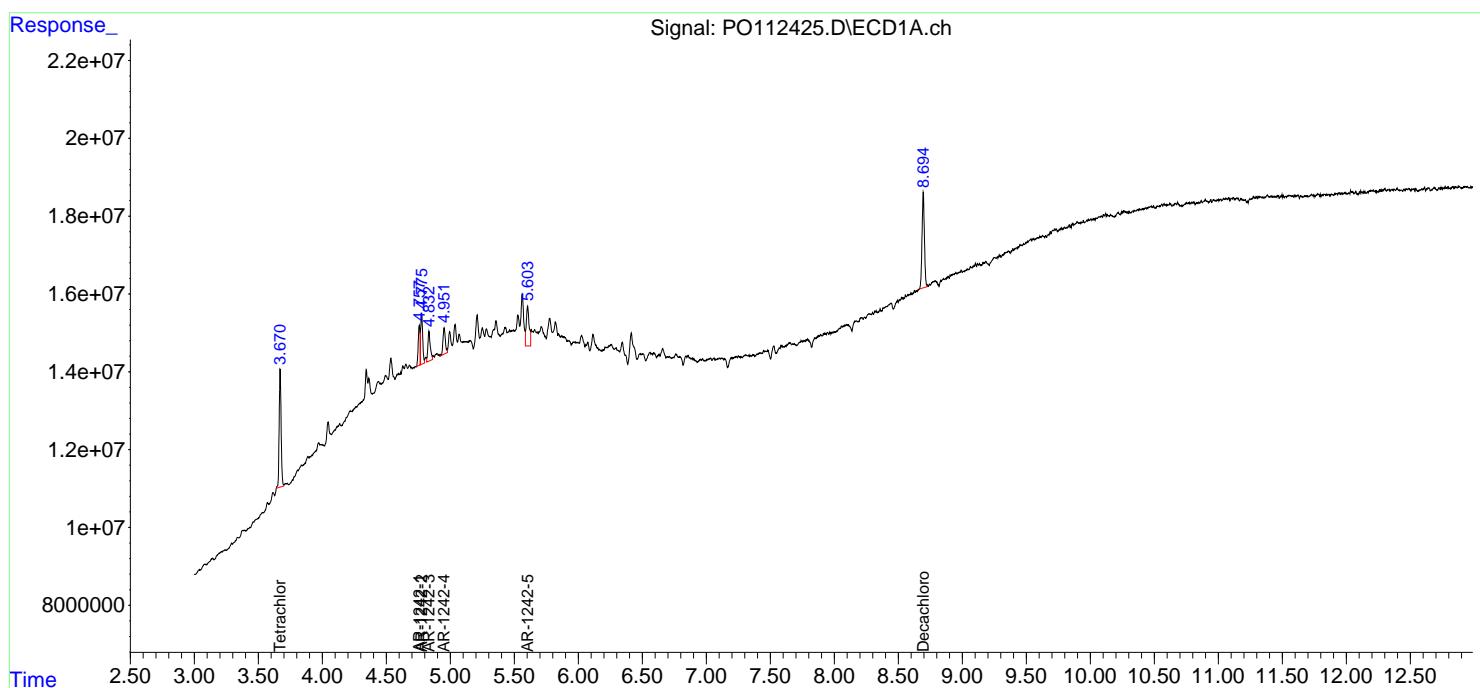


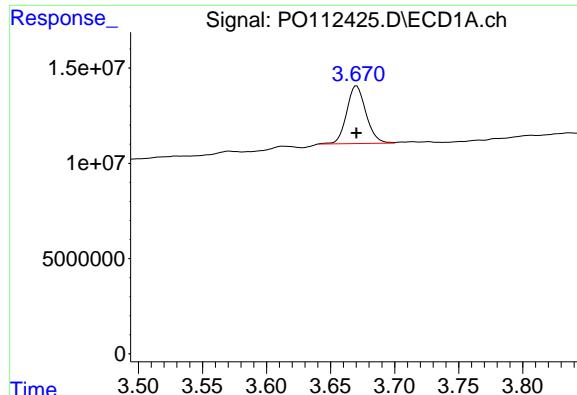

#1 Tetrachloro-m-xylene


R.T.: 3.670 min
Delta R.T.: 0.000 min
Response: 31709040
Conc: 3.68 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

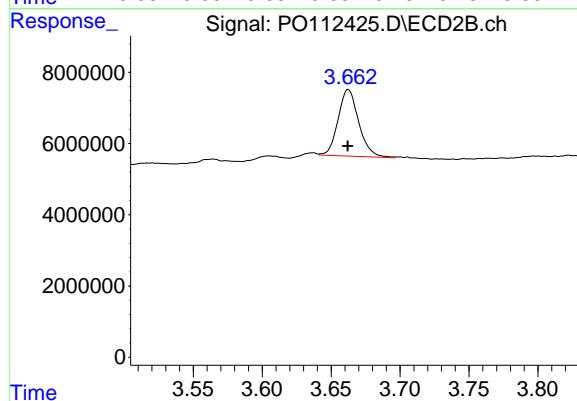


#1 Tetrachloro-m-xylene

R.T.: 3.662 min
Delta R.T.: 0.000 min
Response: 19454228
Conc: 3.70 ng/ml

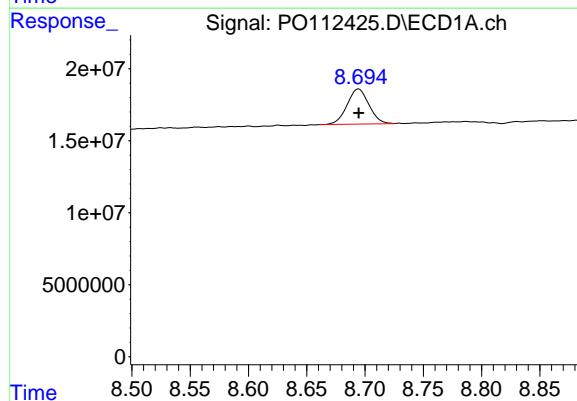


#2 Decachlorobiphenyl

R.T.: 8.695 min
Delta R.T.: 0.000 min
Response: 31949919
Conc: 4.14 ng/ml

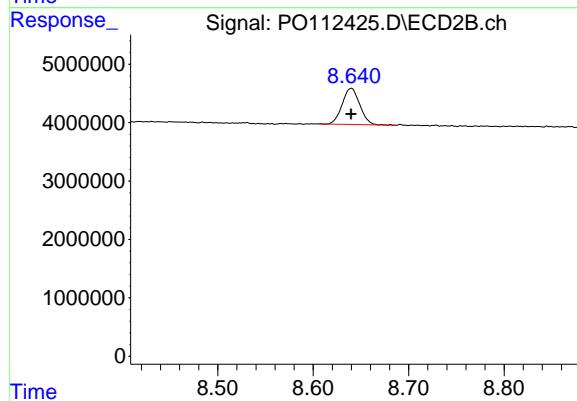

#2 Decachlorobiphenyl

R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 7899252
Conc: 4.30 ng/ml

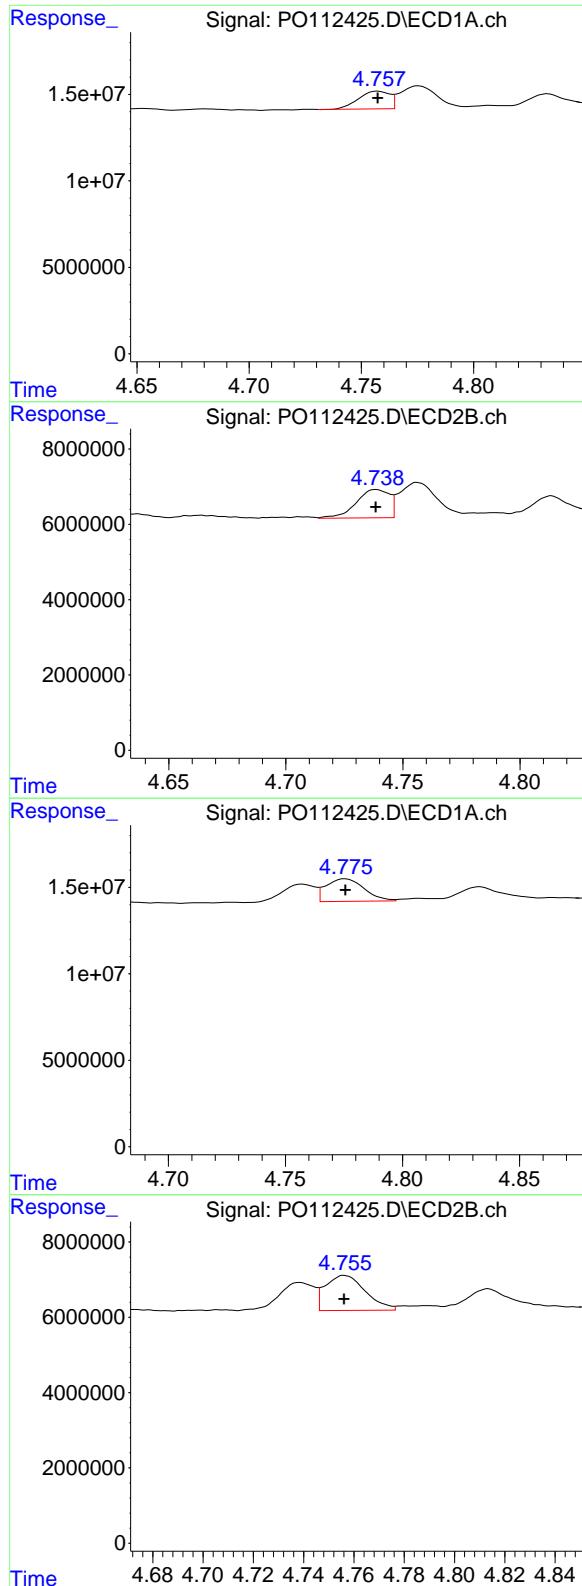

#16 AR-1242-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min
 Response: 9816709
 Conc: 39.65 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1242ICC050

#16 AR-1242-1


R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 7435731
 Conc: 46.94 ng/ml

#17 AR-1242-2

R.T.: 4.776 min
 Delta R.T.: 0.000 min
 Response: 14782408
 Conc: 39.97 ng/ml

#17 AR-1242-2


R.T.: 4.756 min
 Delta R.T.: 0.000 min
 Response: 10324894
 Conc: 44.19 ng/ml

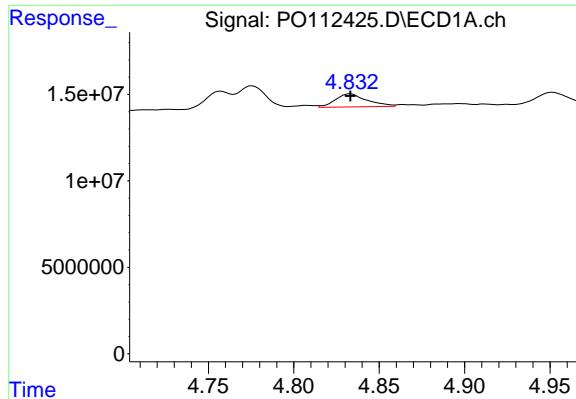

#18 AR-1242-3


R.T.: 4.833 min
Delta R.T.: 0.000 min
Response: 9726638
Conc: 41.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1242ICC050

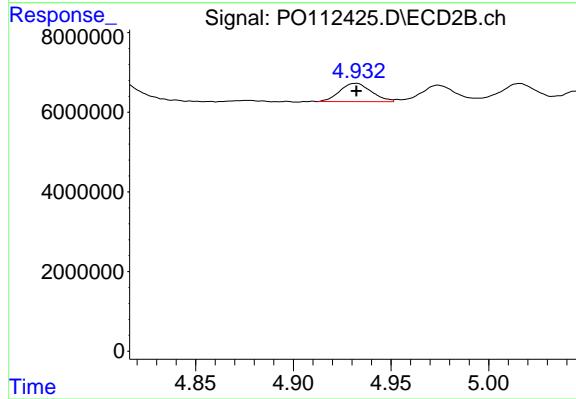


#18 AR-1242-3

R.T.: 4.932 min
Delta R.T.: 0.000 min
Response: 5168677
Conc: 42.65 ng/ml

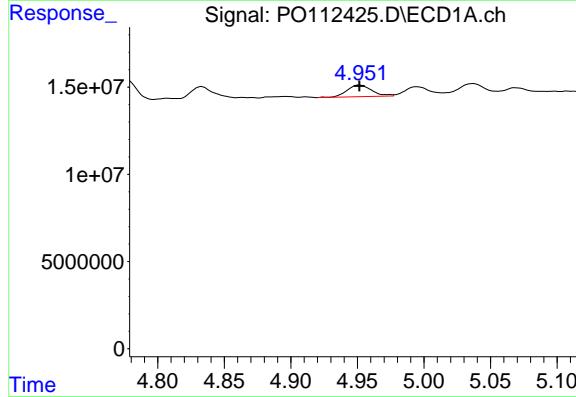


#19 AR-1242-4

R.T.: 4.952 min
Delta R.T.: 0.000 min
Response: 8617431
Conc: 44.36 ng/ml

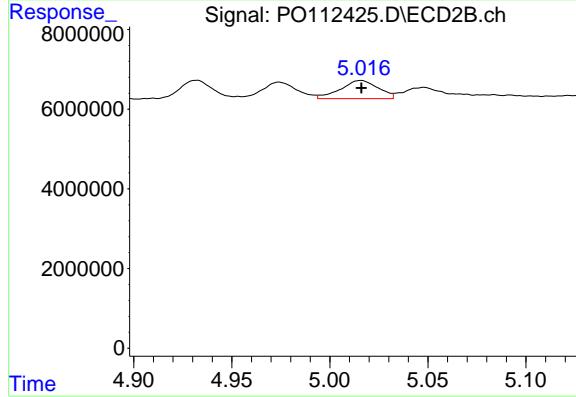

#19 AR-1242-4

R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 6134656
Conc: 49.98 ng/ml

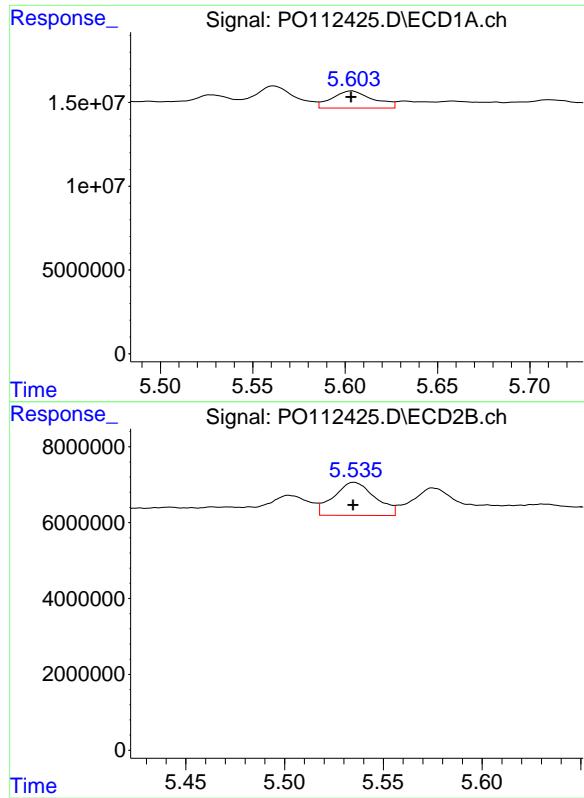

#20 AR-1242-5

R.T.: 5.604 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 15882894 ECD_O
 Conc: 75.36 ng/ml **ClientSampleId:**
 AR1242ICC050

#20 AR-1242-5

R.T.: 5.535 min
 Delta R.T.: 0.000 min
 Response: 12714804
 Conc: 77.94 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:25
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:53:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.670 | 3.662 | 32837807 | 20886754 | 3.789 | 3.981 |
| 2) SA Decachlor... | 8.694 | 8.641 | 30716372 | 7585110 | 3.980 | 4.142 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|--------|--------|
| 21) L5 AR-1248-1 | 4.757 | 4.738 | 7575656 | 5507226 | 40.466 | 45.323 |
| 22) L5 AR-1248-2 | 4.995 | 4.973 | 10157901 | 7726264 | 39.817 | 45.642 |
| 23) L5 AR-1248-3 | 5.208 | 5.015 | 16562795 | 8037448 | 48.190 | 45.244 |
| 24) L5 AR-1248-4 | 5.562 | 5.185 | 27935829 | 10008226 | 55.005 | 47.900 |
| 25) L5 AR-1248-5 | 5.603 | 5.576 | 21113477 | 13039110 | 60.462 | 60.611 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112430.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 16:25
 Operator : YP/AJ
 Sample : AR1248ICC050
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1248ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 17:53:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:39:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

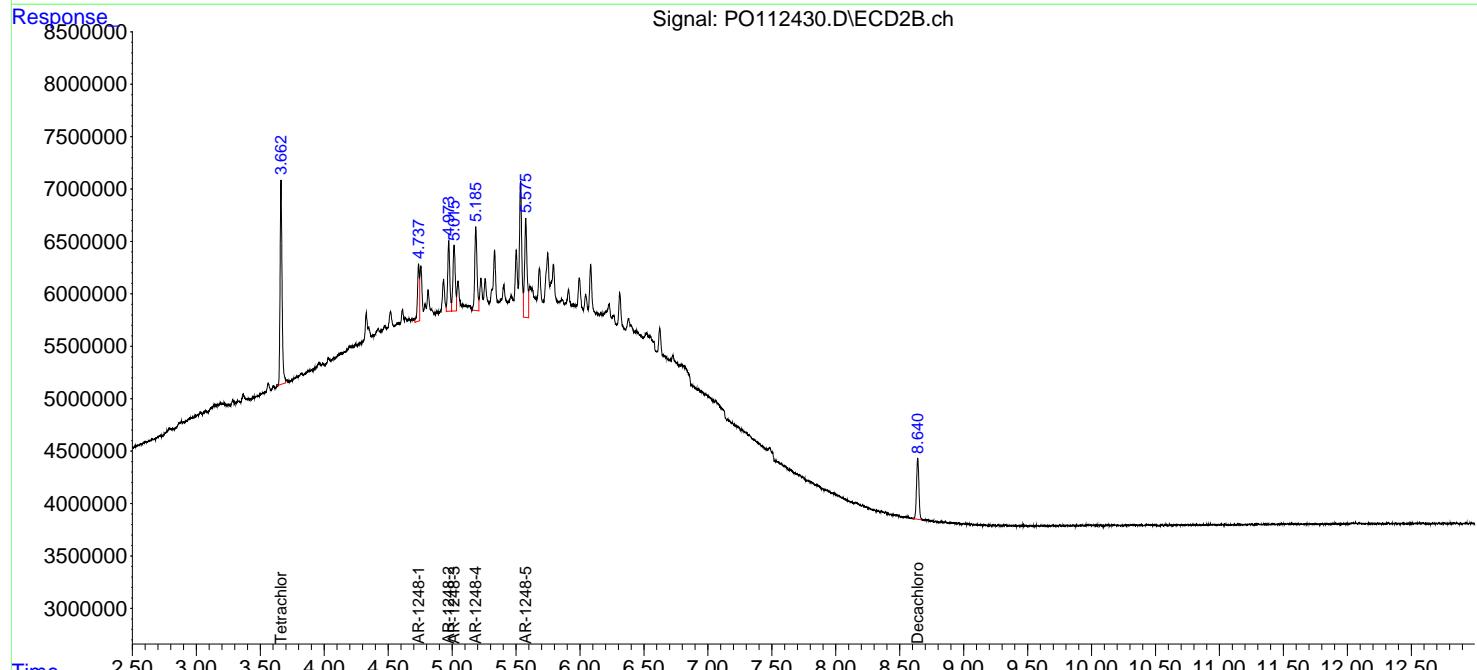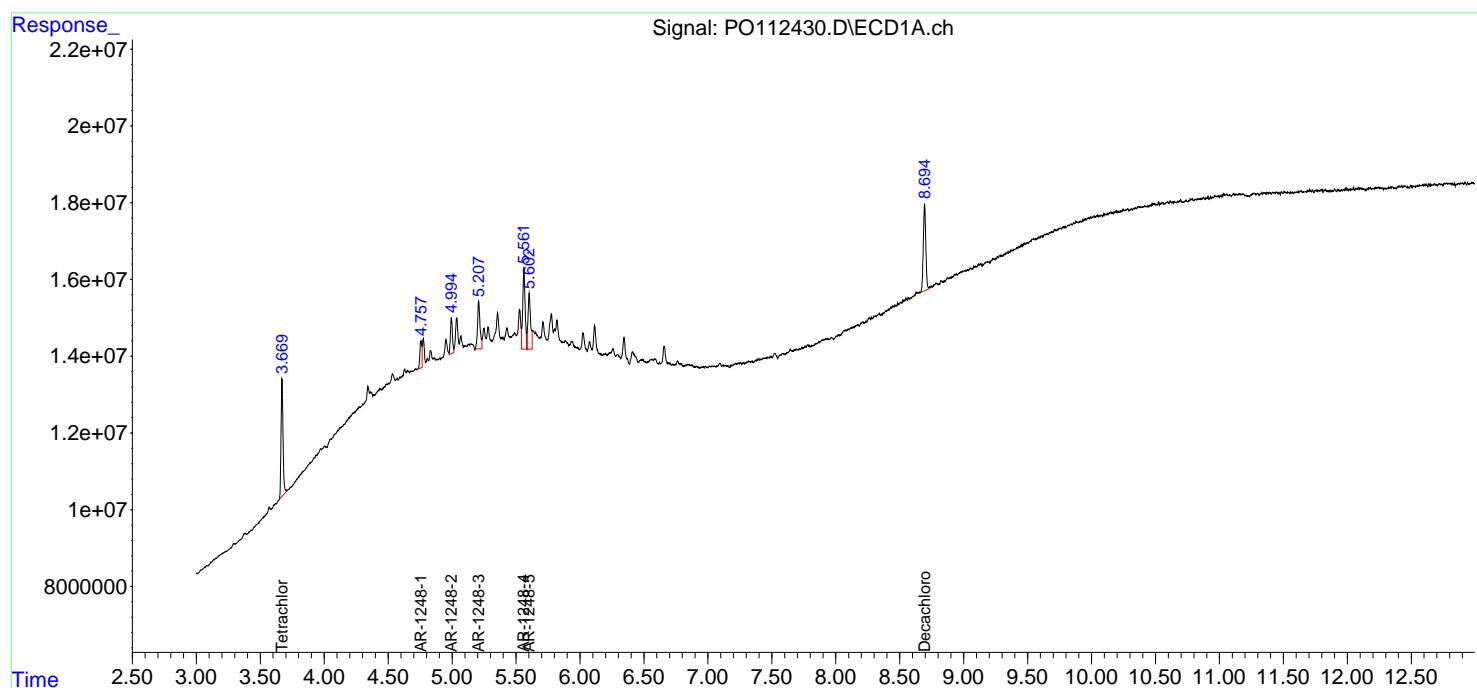

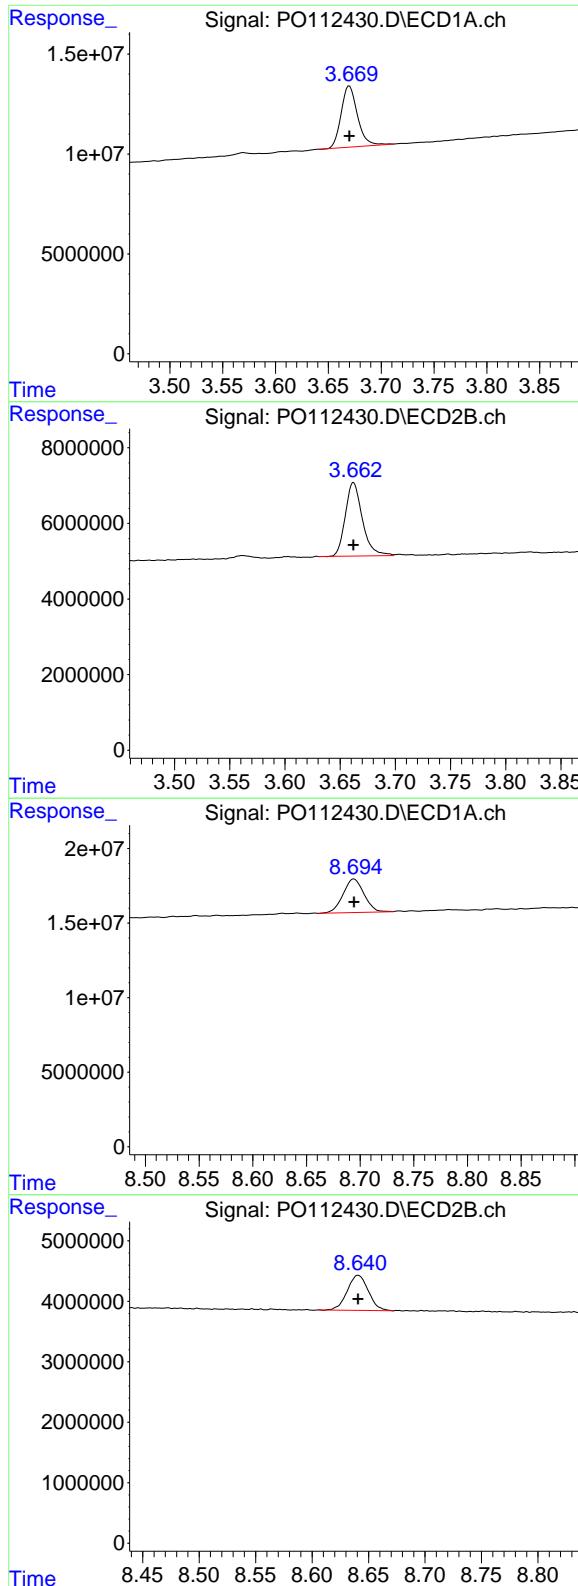

#1 Tetrachloro-m-xylene

R.T.: 3.670 min
 Delta R.T.: 0.000 min
 Response: 32837807
 Conc: 3.79 ng/ml

Instrument:

ECD_O

ClientSampleId :
 AR1248ICC050

#1 Tetrachloro-m-xylene


R.T.: 3.662 min
 Delta R.T.: 0.000 min
 Response: 20886754
 Conc: 3.98 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.694 min
 Delta R.T.: 0.000 min
 Response: 30716372
 Conc: 3.98 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.641 min
 Delta R.T.: 0.000 min
 Response: 7585110
 Conc: 4.14 ng/ml

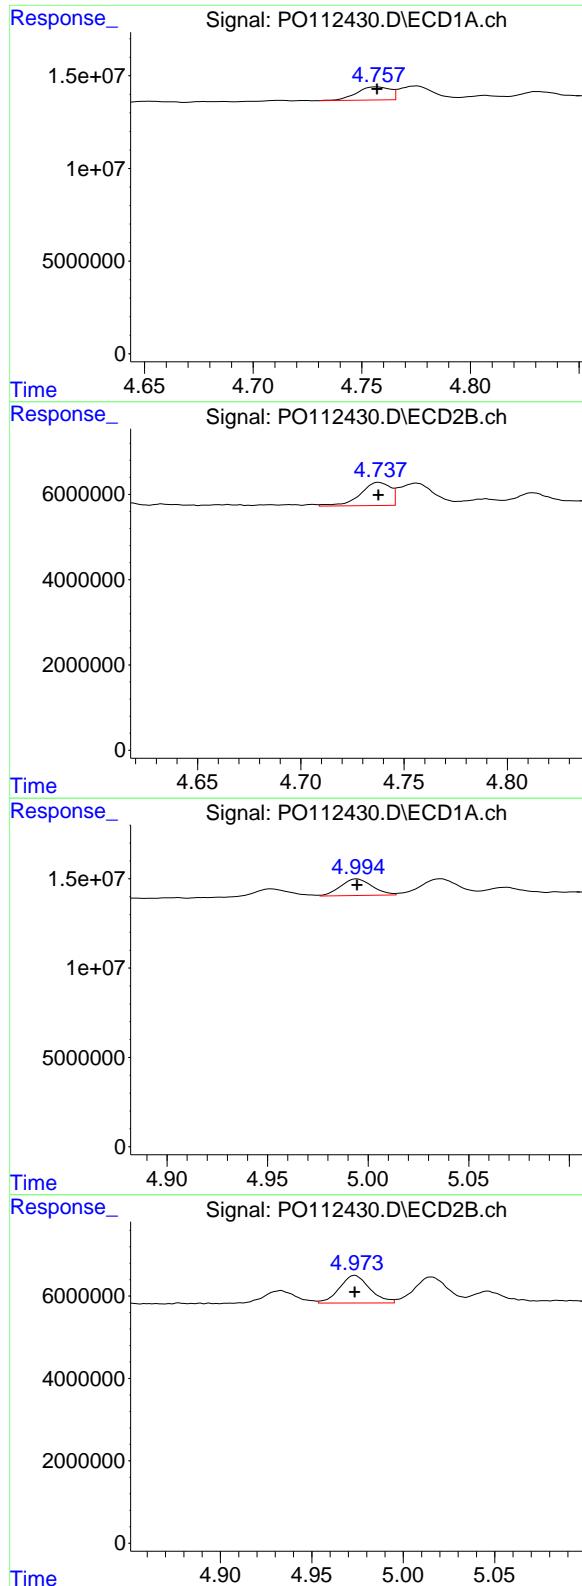

#21 AR-1248-1

R.T.: 4.757 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 7575656 ECD_O
 Conc: 40.47 ng/ml **ClientSampleId :**
 AR1248ICC050

#21 AR-1248-1


R.T.: 4.738 min
 Delta R.T.: 0.000 min
 Response: 5507226
 Conc: 45.32 ng/ml

#22 AR-1248-2

R.T.: 4.995 min
 Delta R.T.: 0.000 min
 Response: 10157901
 Conc: 39.82 ng/ml

#22 AR-1248-2

R.T.: 4.973 min
 Delta R.T.: 0.000 min
 Response: 7726264
 Conc: 45.64 ng/ml

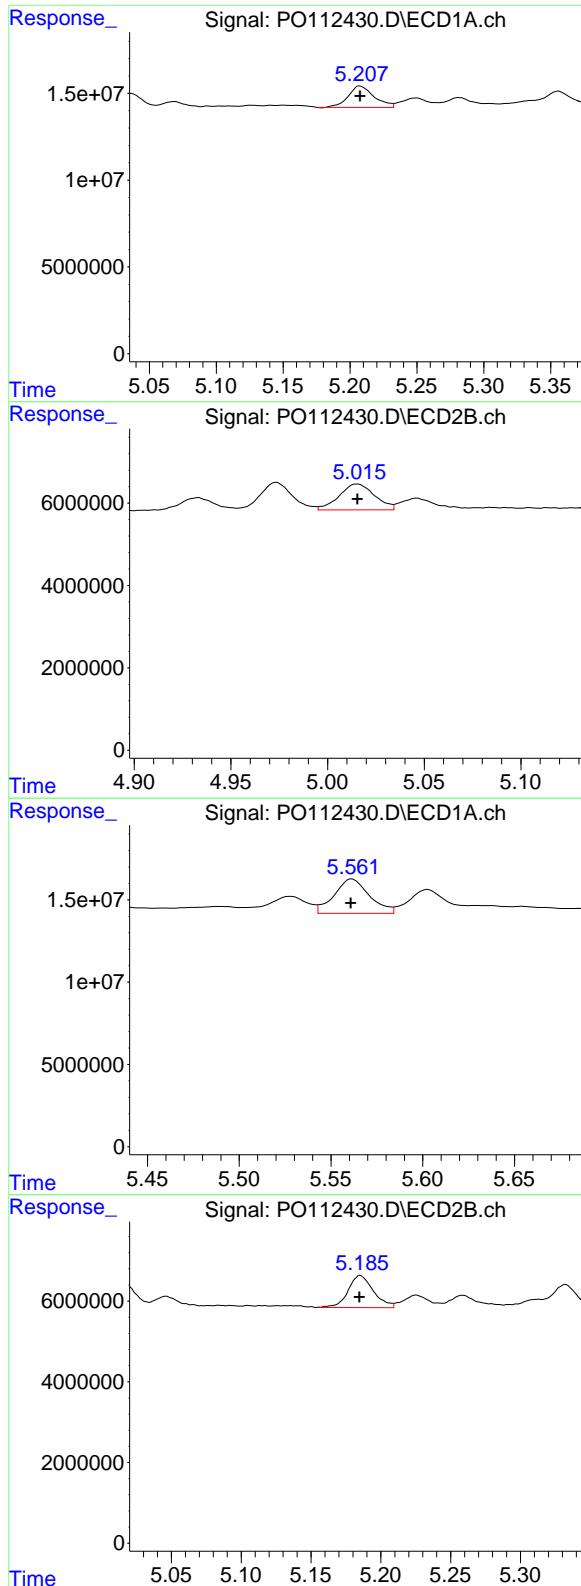

#23 AR-1248-3

R.T.: 5.208 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 16562795 ECD_O
 Conc: 48.19 ng/ml **ClientSampleId:**
 AR1248ICC050

#23 AR-1248-3


R.T.: 5.015 min
 Delta R.T.: 0.000 min
 Response: 8037448
 Conc: 45.24 ng/ml

#24 AR-1248-4

R.T.: 5.562 min
 Delta R.T.: 0.000 min
 Response: 27935829
 Conc: 55.00 ng/ml

#24 AR-1248-4


R.T.: 5.185 min
 Delta R.T.: 0.000 min
 Response: 10008226
 Conc: 47.90 ng/ml

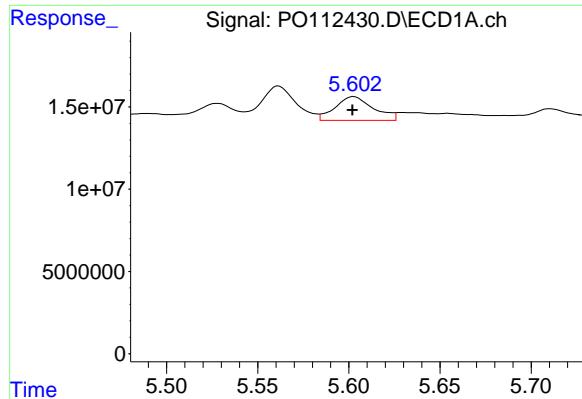

#25 AR-1248-5

R.T.: 5.603 min
Delta R.T.: 0.000 min
Response: 21113477
Conc: 60.46 ng/ml

Instrument: ECD_O
ClientSampleId: AR1248ICC050

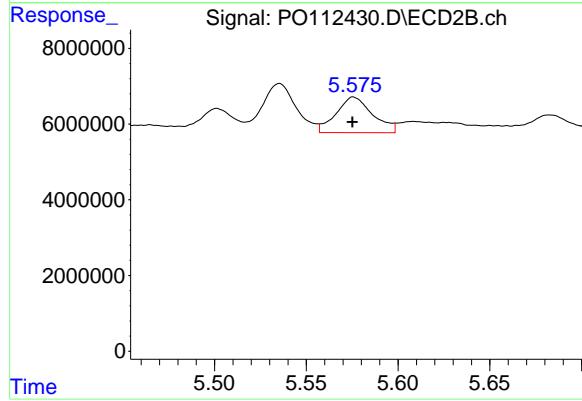

#25 AR-1248-5

R.T.: 5.576 min
Delta R.T.: 0.000 min
Response: 13039110
Conc: 60.61 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:57
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:14:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|----------|----------|-------|-------|
| 1) SA Tetrachlor... | 3.669 | 3.661 | 35024549 | 22021040 | 4.120 | 4.264 |
| 2) SA Decachlor... | 8.694 | 8.640 | 31608253 | 7869748 | 4.125 | 4.324 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|--------|----------|
| 26) L6 AR-1254-1 | 5.561 | 5.535 | 31620587 | 18445655 | 58.061 | 56.180 |
| 27) L6 AR-1254-2 | 5.710 | 5.682 | 26814044 | 17671717 | 55.816 | 61.642 |
| 28) L6 AR-1254-3 | 6.114 | 6.083 | 32662856 | 23495492 | 43.885 | 55.001 # |
| 29) L6 AR-1254-4 | 6.344 | 6.311 | 25352878 | 13603049 | 46.121 | 50.646 |
| 30) L6 AR-1254-5 | 6.762 | 6.726 | 30690471 | 15381815 | 43.359 | 46.051 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0072325\
 Data File : P0112435.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Jul 2025 17:57
 Operator : YP/AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jul 23 18:14:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Jul 23 17:59:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

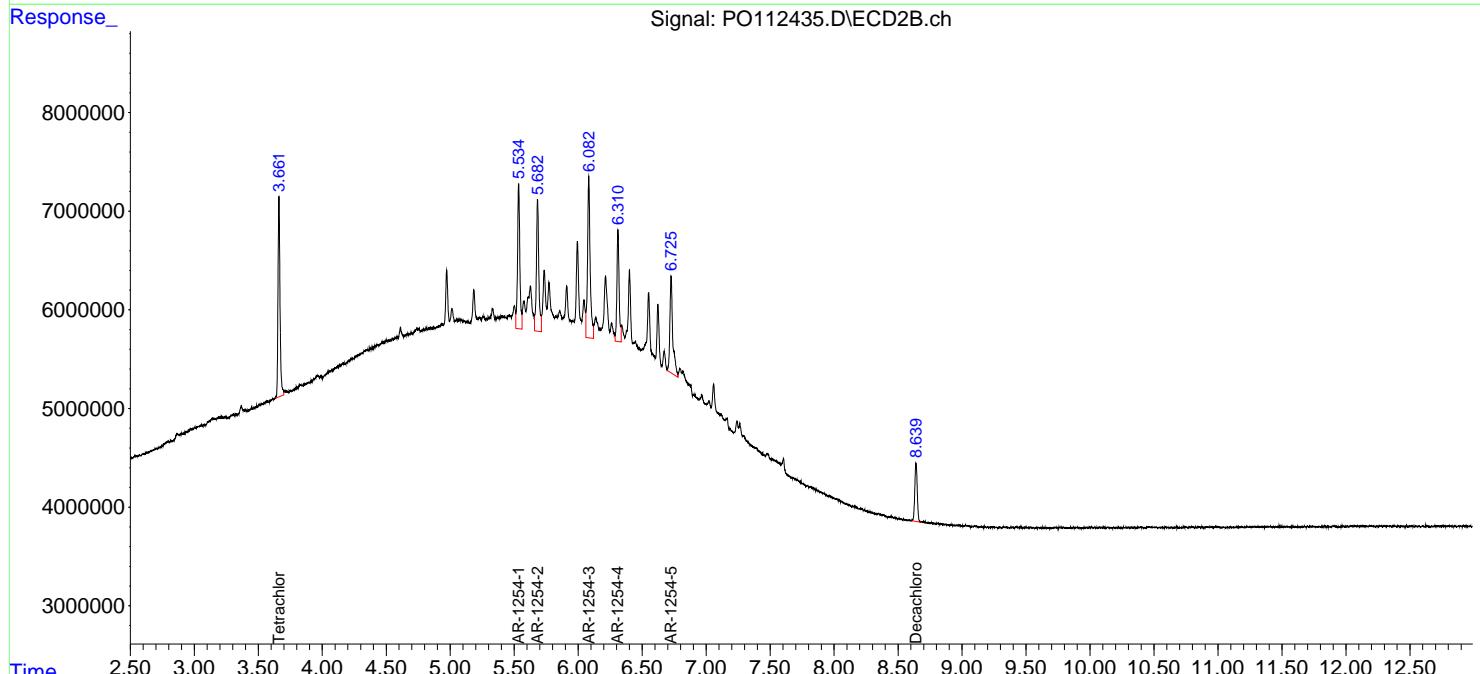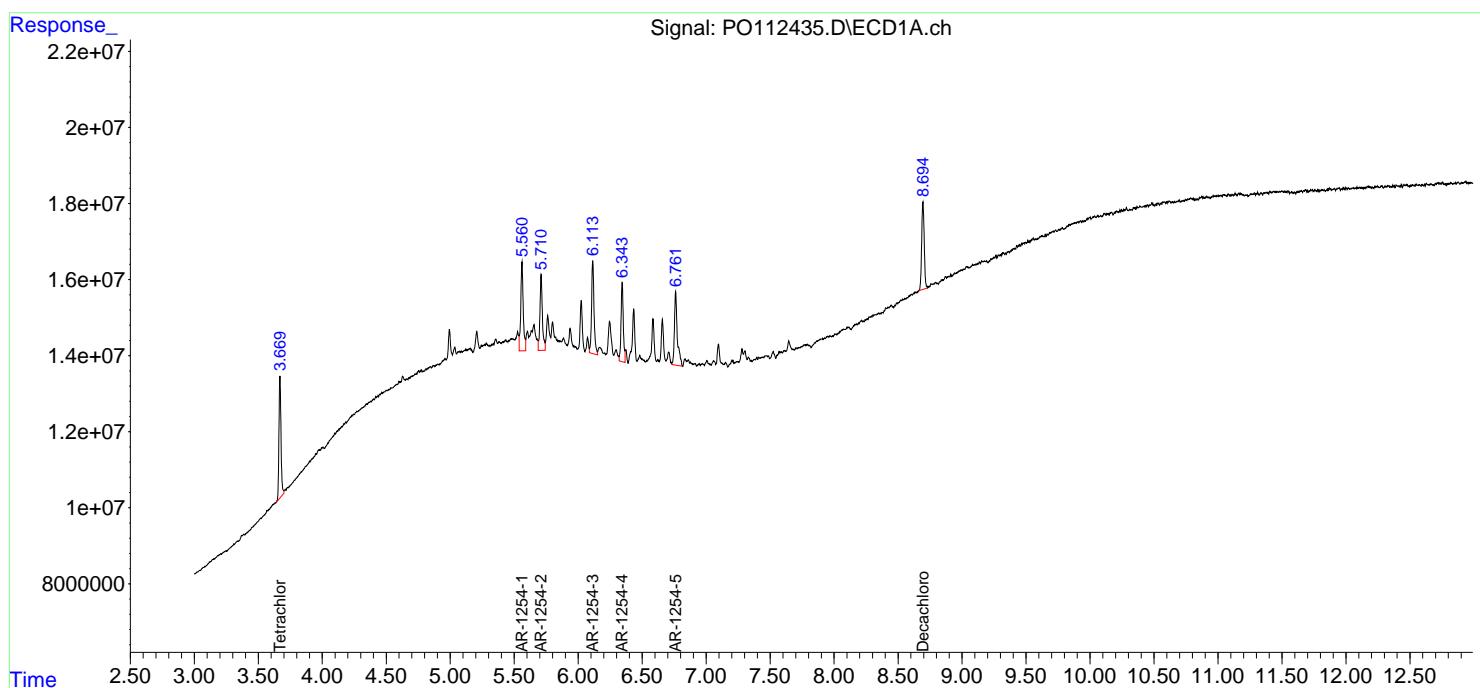

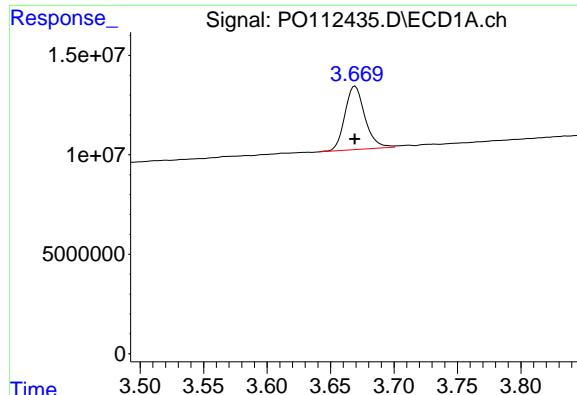


#1 Tetrachloro-m-xylene
R.T.: 3.669 min
Delta R.T.: 0.000 min
Response: 35024549
Conc: 4.12 ng/ml


Instrument: ECD_O
ClientSampleId: AR1254ICC050

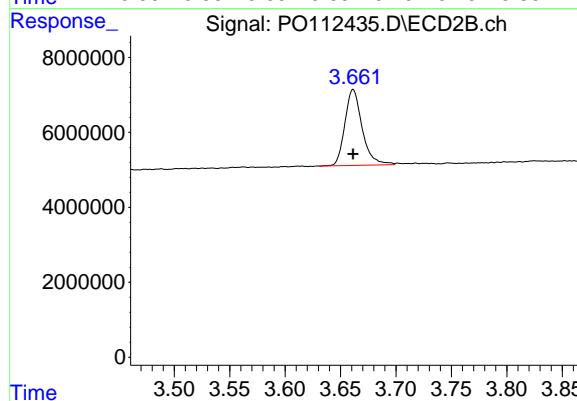


#1 Tetrachloro-m-xylene
R.T.: 3.661 min
Delta R.T.: 0.000 min
Response: 22021040
Conc: 4.26 ng/ml

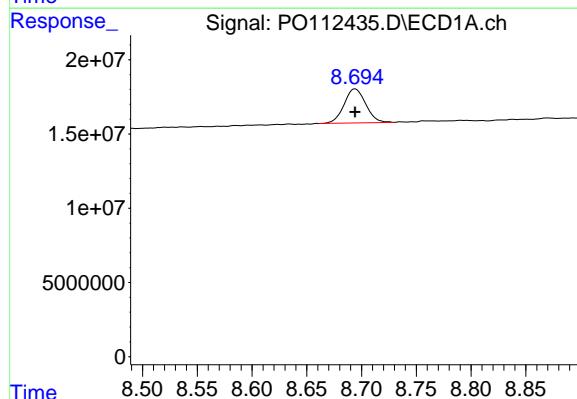

#2 Decachlorobiphenyl
R.T.: 8.694 min
Delta R.T.: 0.000 min
Response: 31608253
Conc: 4.13 ng/ml

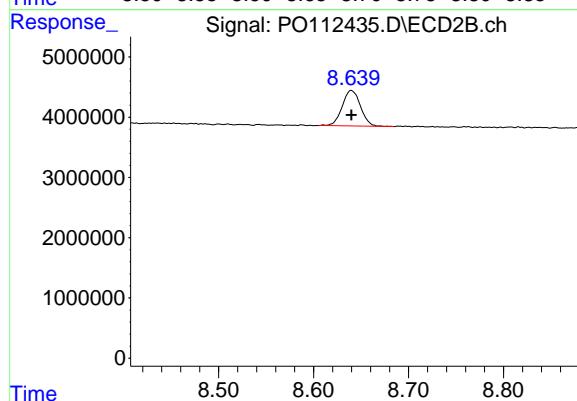

#2 Decachlorobiphenyl
R.T.: 8.640 min
Delta R.T.: 0.000 min
Response: 7869748
Conc: 4.32 ng/ml

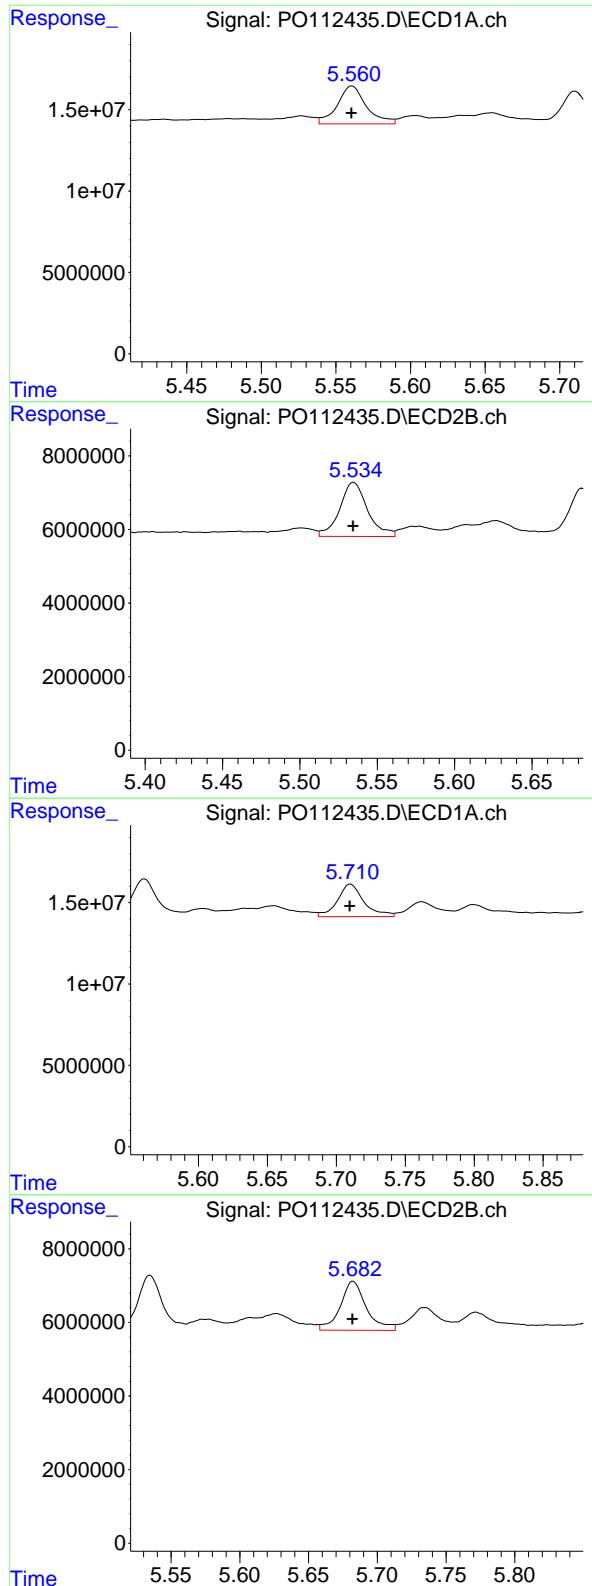

#26 AR-1254-1

R.T.: 5.561 min
 Delta R.T.: 0.000 min
 Response: 31620587
 Conc: 58.06 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

#26 AR-1254-1


R.T.: 5.535 min
 Delta R.T.: 0.000 min
 Response: 18445655
 Conc: 56.18 ng/ml

#27 AR-1254-2

R.T.: 5.710 min
 Delta R.T.: 0.000 min
 Response: 26814044
 Conc: 55.82 ng/ml

#27 AR-1254-2

R.T.: 5.682 min
 Delta R.T.: 0.000 min
 Response: 17671717
 Conc: 61.64 ng/ml

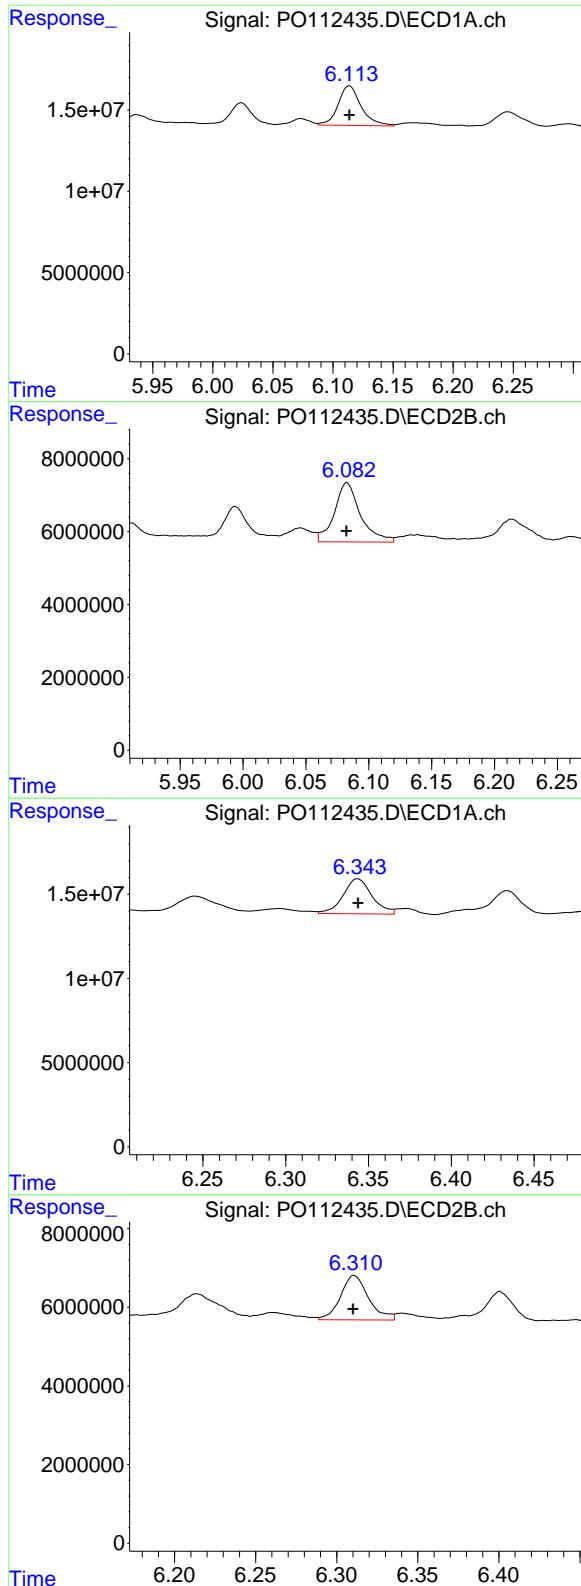

#28 AR-1254-3

R.T.: 6.114 min
 Delta R.T.: 0.000 min
 Response: 32662856
 Conc: 43.88 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1254ICC050

#28 AR-1254-3


R.T.: 6.083 min
 Delta R.T.: 0.000 min
 Response: 23495492
 Conc: 55.00 ng/ml

#29 AR-1254-4

R.T.: 6.344 min
 Delta R.T.: 0.000 min
 Response: 25352878
 Conc: 46.12 ng/ml

#29 AR-1254-4

R.T.: 6.311 min
 Delta R.T.: 0.000 min
 Response: 13603049
 Conc: 50.65 ng/ml

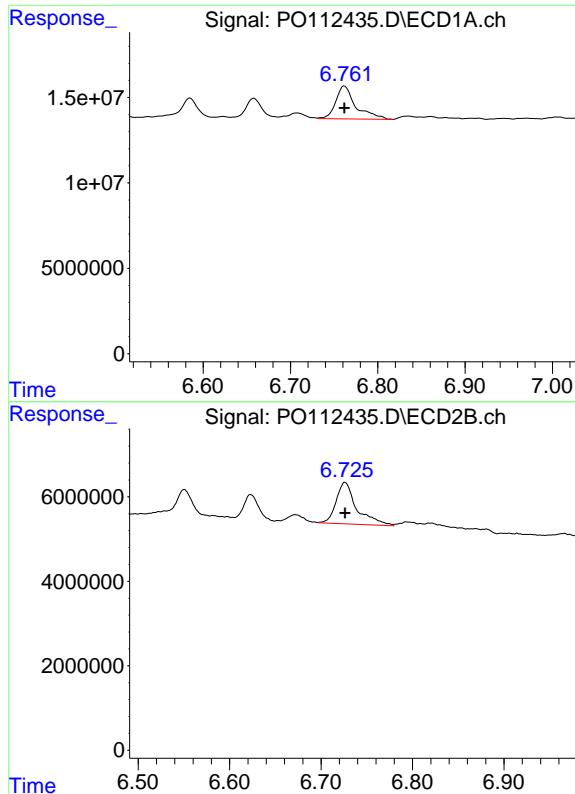

#30 AR-1254-5

R.T.: 6.762 min
Delta R.T.: 0.000 min
Response: 30690471
Conc: 43.36 ng/ml

Instrument: ECD_O
ClientSampleId: AR1254ICC050

#30 AR-1254-5

R.T.: 6.726 min
Delta R.T.: 0.000 min
Response: 15381815
Conc: 46.05 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 08:54
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:51:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.665 | 3.658 | 488.6E6 | 280.2E6 | 60.081 | 56.386 |
| 2) SA Decachlor... | 8.686 | 8.631 | 340.4E6 | 92854815 | 46.549 | 52.546 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|-----------|
| 3) L1 AR-1016-1 | 4.751 | 4.731 | 155.3E6 | 93205664 | 578.725 | 532.582 |
| 4) L1 AR-1016-2 | 4.769 | 4.749 | 233.9E6 | 136.6E6 | 575.978 | 524.330 |
| 5) L1 AR-1016-3 | 4.826 | 4.924 | 148.1E6 | 68284681 | 565.785 | 502.217 |
| 6) L1 AR-1016-4 | 4.945 | 4.967 | 121.1E6 | 56332621 | 571.539 | 507.114 |
| 7) L1 AR-1016-5 | 5.202 | 5.179 | 126.2E6 | 75085975 | 574.857 | 523.966 |
| 8) L2 AR-1221-1 | 3.876 | 3.865 | 13553752 | 9529395 | 140.221 | 141.668 |
| 9) L2 AR-1221-2 | 3.964 | 3.952 | 20985345 | 14408008 | 292.023 | 284.025 |
| 10) L2 AR-1221-3 | 4.038 | 4.026 | 79639699 | 51419673 | 335.027 | 324.354 |
| 11) L3 AR-1232-1 | 4.038 | 4.026 | 79639699 | 51419673 | 425.929 | 406.319 |
| 12) L3 AR-1232-2 | 4.529 | 4.749 | 118.7E6 | 136.6E6 | 1102.695 | 1041.407 |
| 13) L3 AR-1232-3 | 4.769 | 4.924 | 233.9E6 | 68284681 | 1131.120 | 1016.189 |
| 14) L3 AR-1232-4 | 4.945 | 5.009 | 121.1E6 | 68260248 | 1155.960 | 1140.921 |
| 15) L3 AR-1232-5 | 4.988 | 5.179 | 94920489 | 75085975 | 1398.339 | 1151.572 |
| 16) L4 AR-1242-1 | 4.751 | 4.731 | 155.3E6 | 93205664 | 627.282 | 588.442 |
| 17) L4 AR-1242-2 | 4.769 | 4.749 | 233.9E6 | 136.6E6 | 632.555 | 584.532 |
| 18) L4 AR-1242-3 | 4.826 | 4.924 | 148.1E6 | 68284681 | 625.592 | 563.456 |
| 19) L4 AR-1242-4 | 4.945 | 5.009 | 121.1E6 | 68260248 | 623.206 | 556.140 |
| 20) L4 AR-1242-5 | 5.597 | 5.528 | 36369268 | 77150754 | 170.017 | 479.283 # |
| 21) L5 AR-1248-1 | 4.751 | 4.731 | 155.3E6 | 93205664 | 829.608 | 767.066 |
| 22) L5 AR-1248-2 | 4.988 | 4.967 | 94920489 | 56332621 | 372.073 | 332.778 |
| 23) L5 AR-1248-3 | 5.202 | 5.009 | 126.2E6 | 68260248 | 367.075 | 384.246 |
| 24) L5 AR-1248-4 | 5.555 | 5.179 | 137.5E6 | 75085975 | 270.594 | 360.376 # |
| 25) L5 AR-1248-5 | 5.597 | 5.569 | 36369268 | 20206764 | 104.034 | 94.088 |
| 26) L6 AR-1254-1 | 5.555 | 5.528 | 137.5E6 | 77150754 | 250.443 | 234.771 |
| 27) L6 AR-1254-2 | 5.704 | 5.676 | 102.5E6 | 56225513 | 210.971 | 194.222 |
| 28) L6 AR-1254-3 | 6.123 | 6.092 | 202.0E6 | 105.5E6 | 271.395 | 246.703 |
| 29) L6 AR-1254-4 | 6.338 | 6.304 | 31938035 | 14309000 | 58.100 | 52.421 |
| 30) L6 AR-1254-5 | 6.755 | 6.718 | 317.3E6 | 158.6E6 | 448.328 | 474.727 |
| 31) L7 AR-1260-1 | 6.238 | 6.206 | 254.5E6 | 133.0E6 | 579.224 | 535.236 |
| 32) L7 AR-1260-2 | 6.428 | 6.394 | 376.6E6 | 177.5E6 | 547.504 | 538.814 |
| 33) L7 AR-1260-3 | 6.794 | 6.546 | 310.9E6 | 135.1E6 | 528.746 | 525.921 |
| 34) L7 AR-1260-4 | 7.053 | 7.015 | 225.0E6 | 101.4E6 | 498.852 | 530.125 |
| 35) L7 AR-1260-5 | 7.296 | 7.257 | 685.4E6 | 226.7E6 | 553.135 | 549.898 |
| 36) L8 AR-1262-1 | 6.794 | 6.757 | 310.9E6 | 150.6E6 | 334.600 | 363.000 |
| 37) L8 AR-1262-2 | 7.296 | 7.257 | 685.4E6 | 226.7E6 | 460.930 | 439.659 |
| 38) L8 AR-1262-3 | 7.578 | 7.538 | 136.5E6 | 46051874 | 231.184 | 246.894 |
| 39) L8 AR-1262-4 | 7.643 | 7.601 | 401.5E6 | 122.5E6 | 403.859 | 425.366 |
| 40) L8 AR-1262-5 | 8.139 | 8.094 | 132.3E6 | 27693523 | 304.690 | 278.317 |
| 41) L9 AR-1268-1 | 7.578 | 7.538 | 136.5E6 | 46051874 | 77.925 | 88.927 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 08:54
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:51:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|-------|-------|----------|----------|---------|----------|
| 42) L9 AR-1268-2 | 7.643 | 7.601 | 401.5E6 | 122.5E6 | 272.570 | 288.308 |
| 43) L9 AR-1268-3 | 7.849 | 7.807 | 6266792 | 2290388 | 5.004 | 7.129 # |
| 44) L9 AR-1268-4 | 8.139 | 8.094 | 132.3E6 | 27693523 | 274.463 | 248.829 |
| 45) L9 AR-1268-5 | 8.431 | 8.382 | 30321851 | 8645473 | 9.032 | 11.815 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 08:54
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 ECD_O
 ClientSampleId :
 AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 18 05:51:48 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

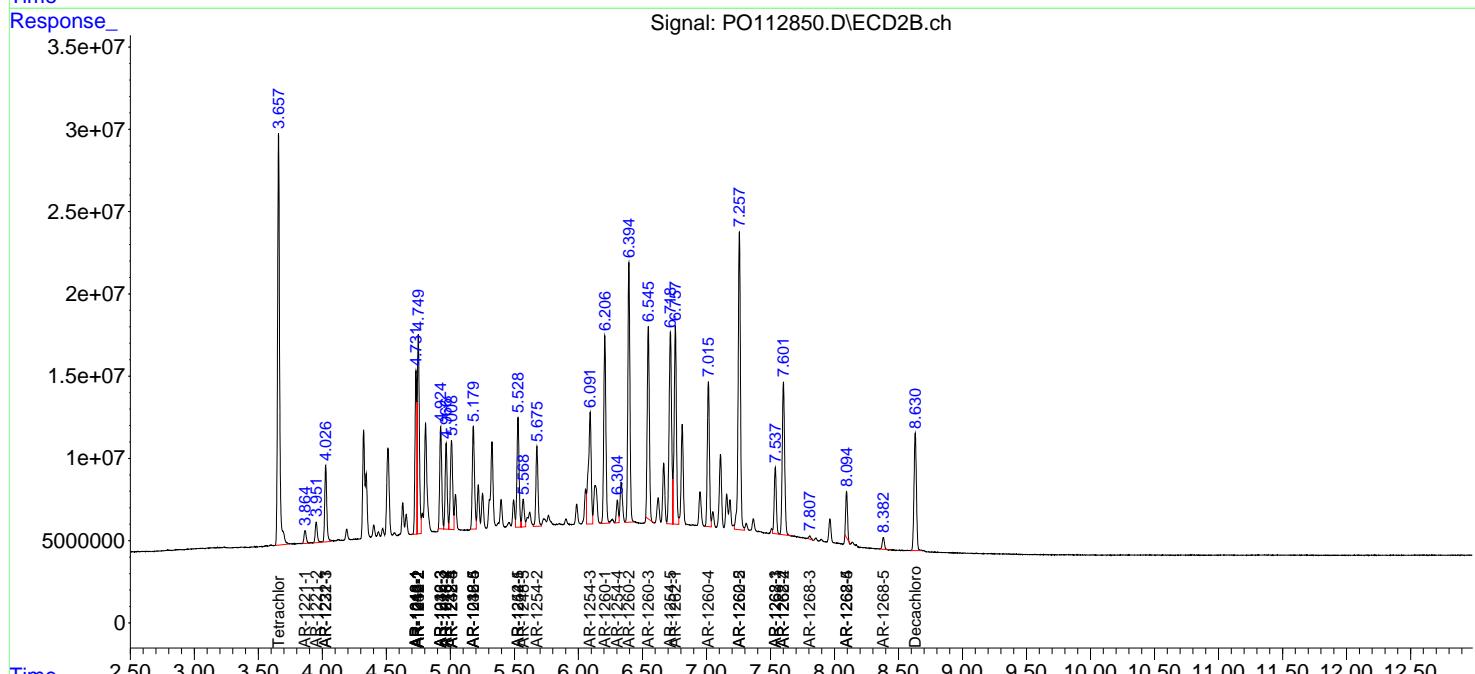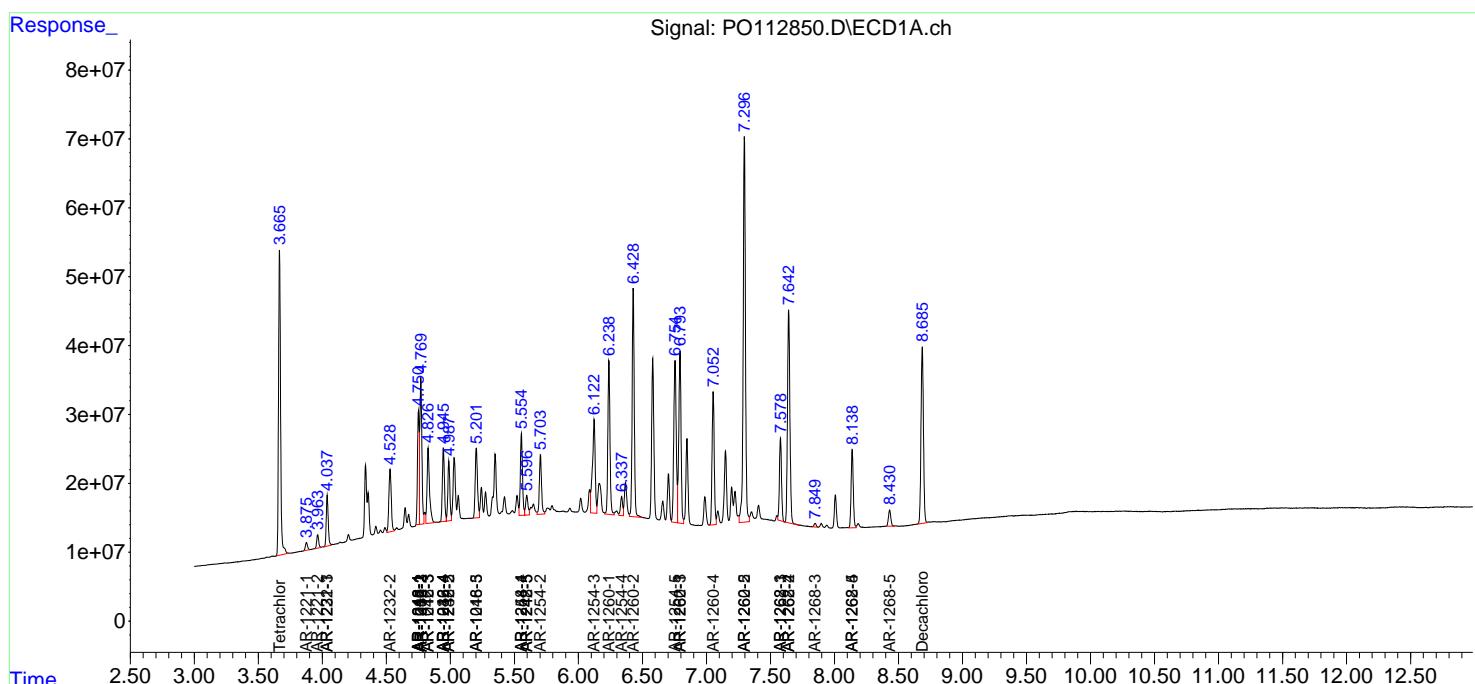

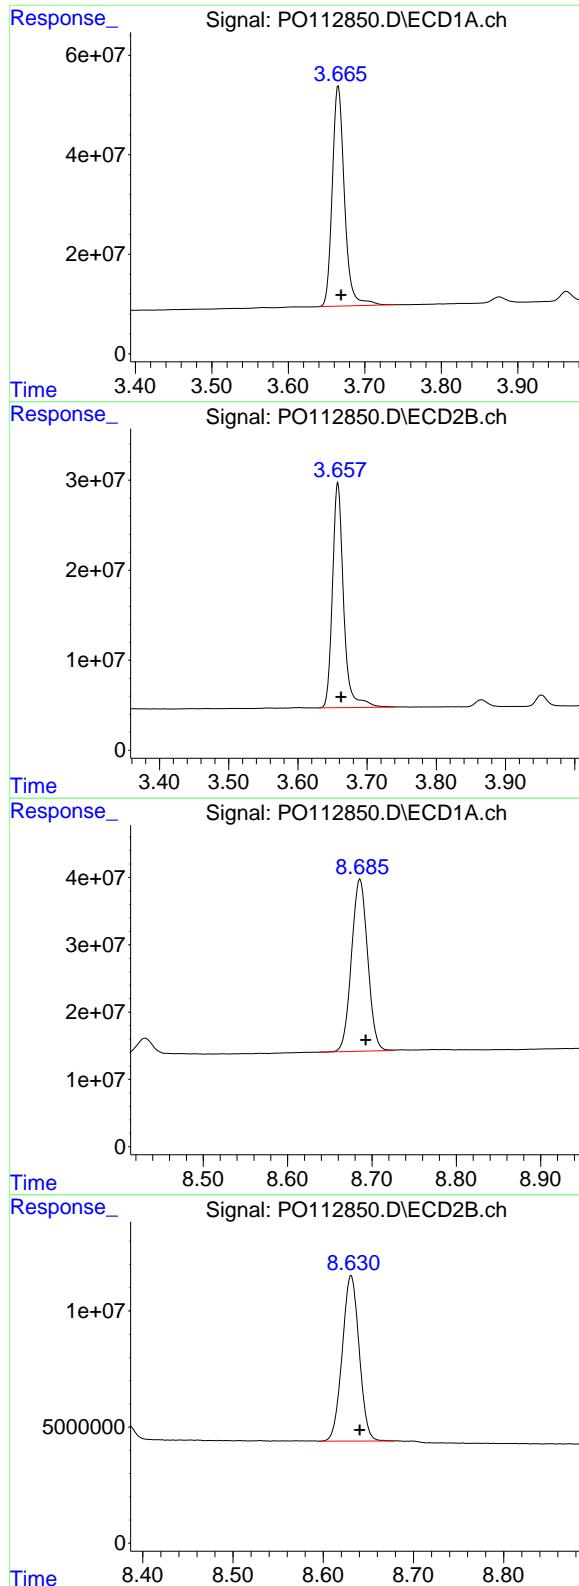

#1 Tetrachloro-m-xylene

R.T.: 3.665 min
 Delta R.T.: -0.004 min
 Response: 488550662
 Conc: 60.08 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1660CCC500

#1 Tetrachloro-m-xylene


R.T.: 3.658 min
 Delta R.T.: -0.005 min
 Response: 280189739
 Conc: 56.39 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.686 min
 Delta R.T.: -0.007 min
 Response: 340356409
 Conc: 46.55 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.631 min
 Delta R.T.: -0.010 min
 Response: 92854815
 Conc: 52.55 ng/ml

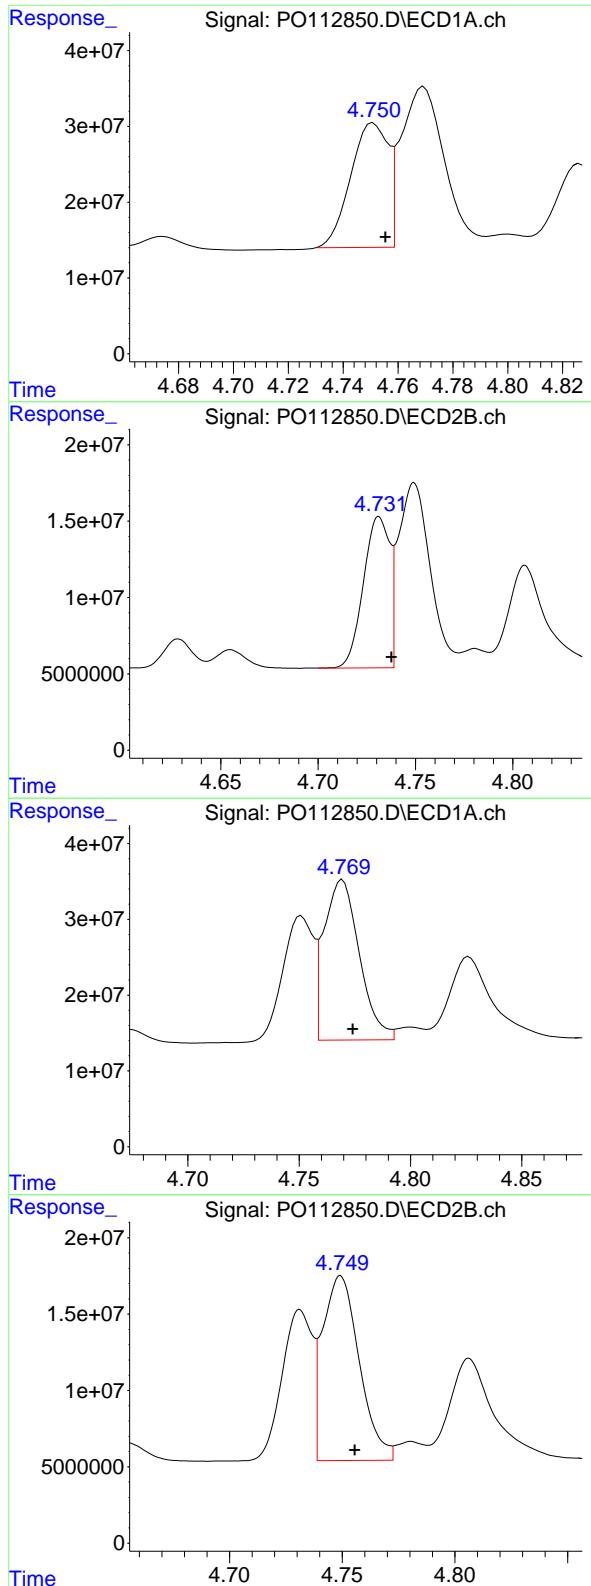

#3 AR-1016-1

R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 155309919
 Conc: 578.72 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.731 min
 Delta R.T.: -0.006 min
 Response: 93205664
 Conc: 532.58 ng/ml

#4 AR-1016-2

R.T.: 4.769 min
 Delta R.T.: -0.005 min
 Response: 233914683
 Conc: 575.98 ng/ml

#4 AR-1016-2

R.T.: 4.749 min
 Delta R.T.: -0.006 min
 Response: 136585485
 Conc: 524.33 ng/ml

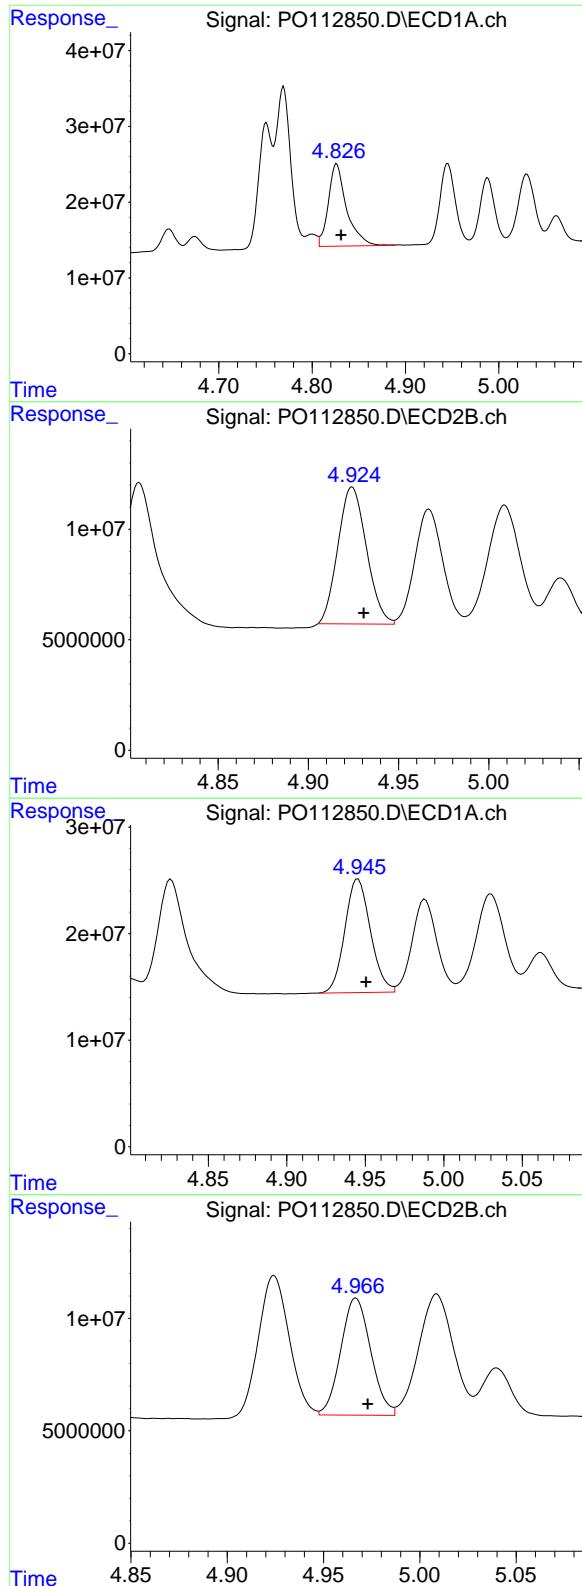

#5 AR-1016-3

R.T.: 4.826 min
 Delta R.T.: -0.005 min
 Response: 148051145
 Conc: 565.78 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 4.924 min
 Delta R.T.: -0.006 min
 Response: 68284681
 Conc: 502.22 ng/ml

#6 AR-1016-4

R.T.: 4.945 min
 Delta R.T.: -0.005 min
 Response: 121075575
 Conc: 571.54 ng/ml

#6 AR-1016-4

R.T.: 4.967 min
 Delta R.T.: -0.006 min
 Response: 56332621
 Conc: 507.11 ng/ml

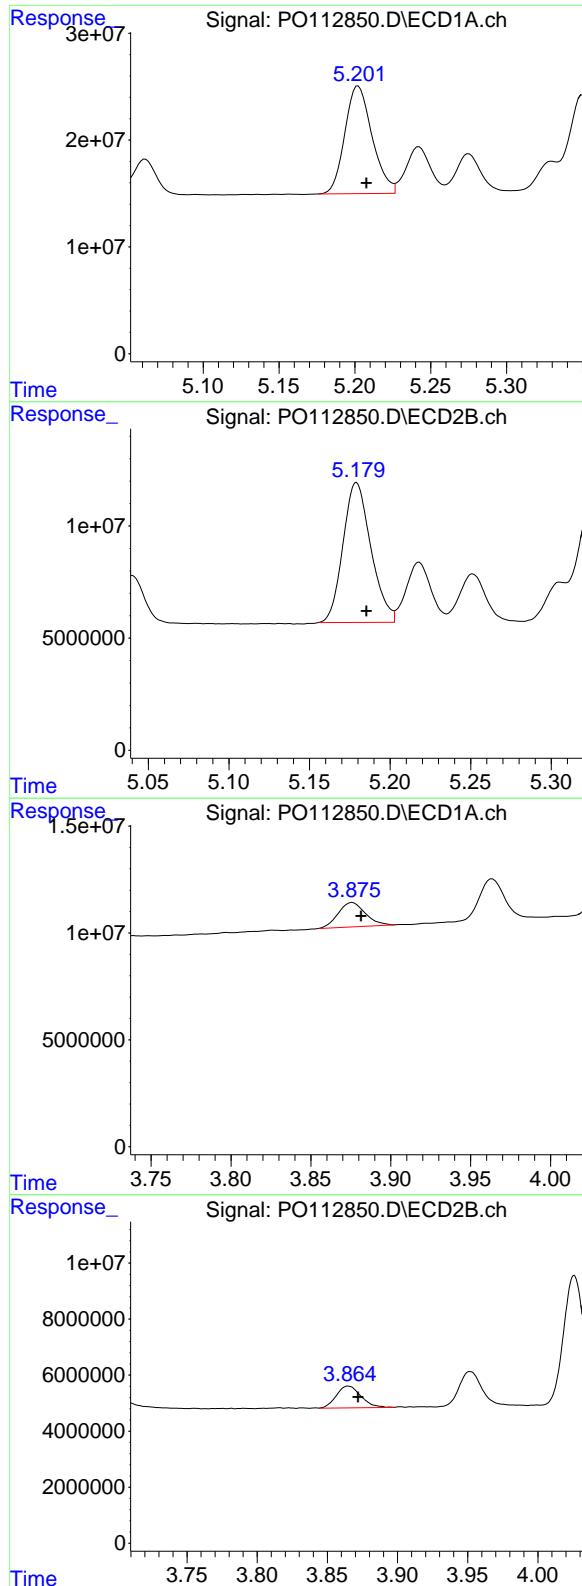

#7 AR-1016-5

R.T.: 5.202 min
 Delta R.T.: -0.005 min
 Response: 126164306
 Conc: 574.86 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.179 min
 Delta R.T.: -0.006 min
 Response: 75085975
 Conc: 523.97 ng/ml

#8 AR-1221-1

R.T.: 3.876 min
 Delta R.T.: -0.006 min
 Response: 13553752
 Conc: 140.22 ng/ml

#8 AR-1221-1

R.T.: 3.865 min
 Delta R.T.: -0.007 min
 Response: 9529395
 Conc: 141.67 ng/ml

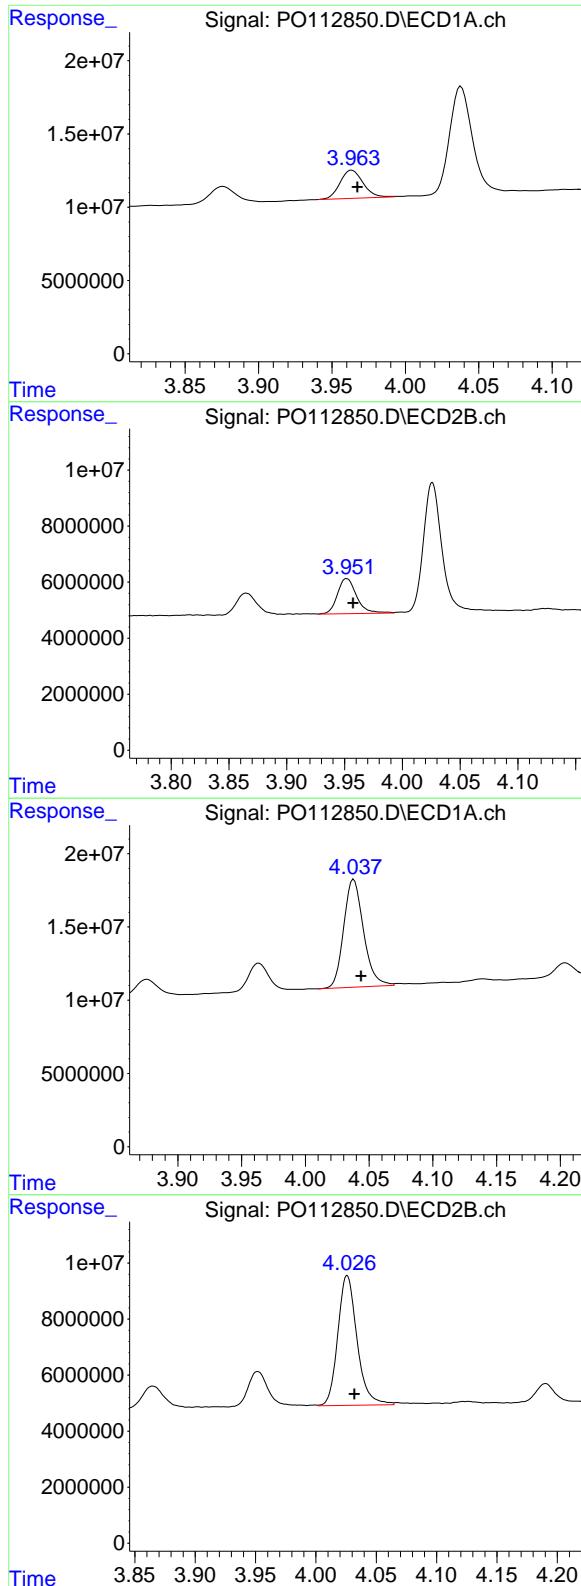

#9 AR-1221-2

R.T.: 3.964 min
 Delta R.T.: -0.004 min
 Response: 20985345
 Conc: 292.02 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 3.952 min
 Delta R.T.: -0.006 min
 Response: 14408008
 Conc: 284.02 ng/ml

#10 AR-1221-3

R.T.: 4.038 min
 Delta R.T.: -0.006 min
 Response: 79639699
 Conc: 335.03 ng/ml

#10 AR-1221-3

R.T.: 4.026 min
 Delta R.T.: -0.006 min
 Response: 51419673
 Conc: 324.35 ng/ml

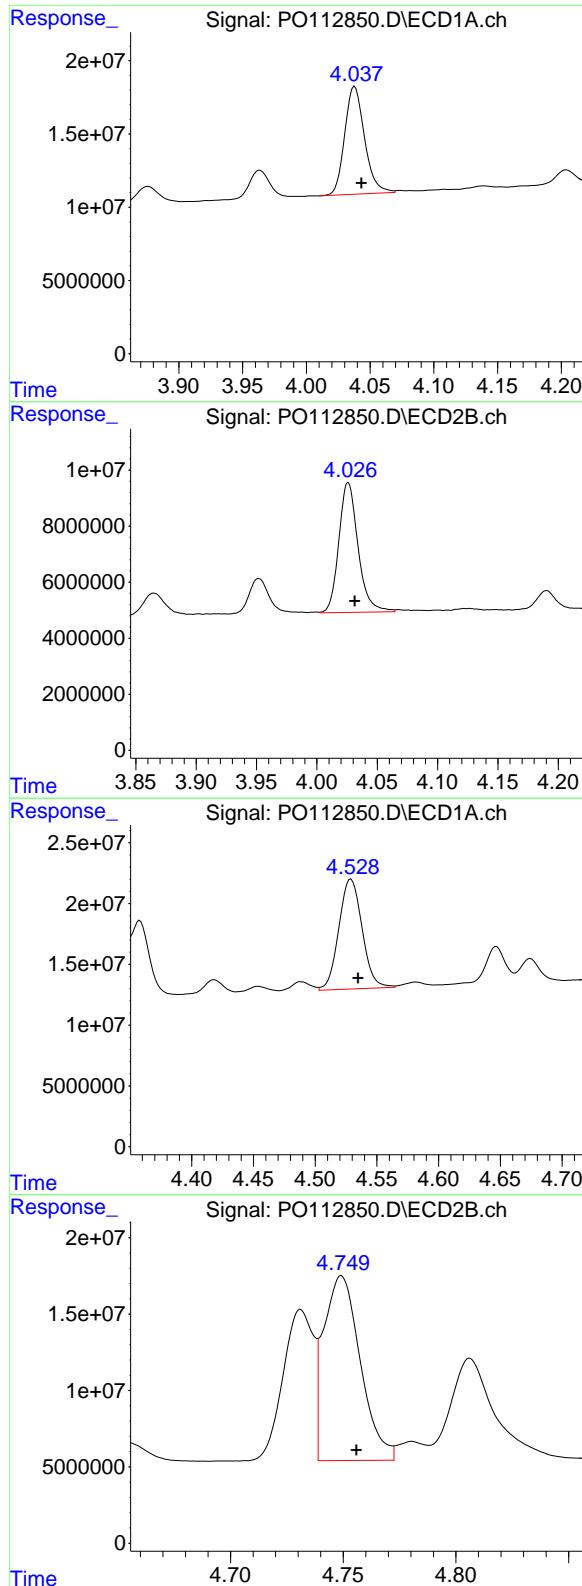

#11 AR-1232-1

R.T.: 4.038 min
 Delta R.T.: -0.005 min
 Response: 79639699
 Conc: 425.93 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.026 min
 Delta R.T.: -0.006 min
 Response: 51419673
 Conc: 406.32 ng/ml

#12 AR-1232-2

R.T.: 4.529 min
 Delta R.T.: -0.006 min
 Response: 118677283
 Conc: 1102.70 ng/ml

#12 AR-1232-2


R.T.: 4.749 min
 Delta R.T.: -0.007 min
 Response: 136585485
 Conc: 1041.41 ng/ml

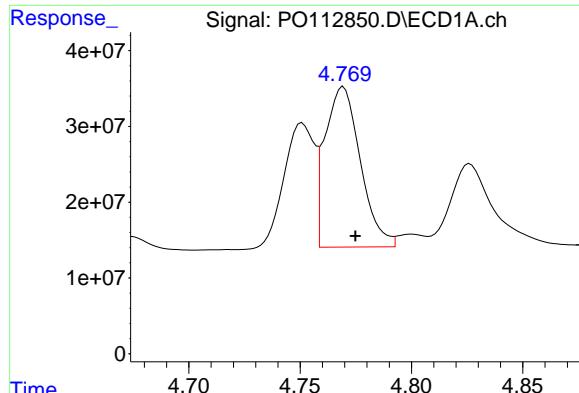

#13 AR-1232-3


R.T.: 4.769 min
 Delta R.T.: -0.005 min
 Response: 233914683
 Conc: 1131.12 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

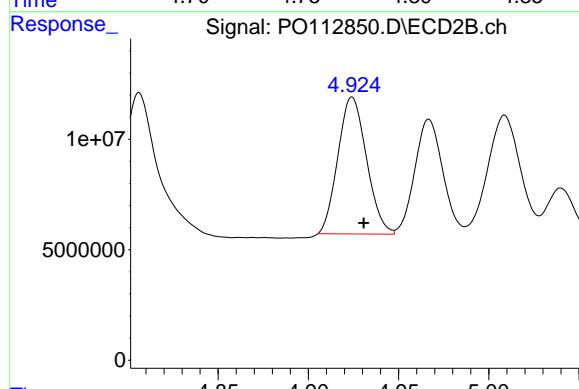


#13 AR-1232-3

R.T.: 4.924 min
 Delta R.T.: -0.006 min
 Response: 68284681
 Conc: 1016.19 ng/ml

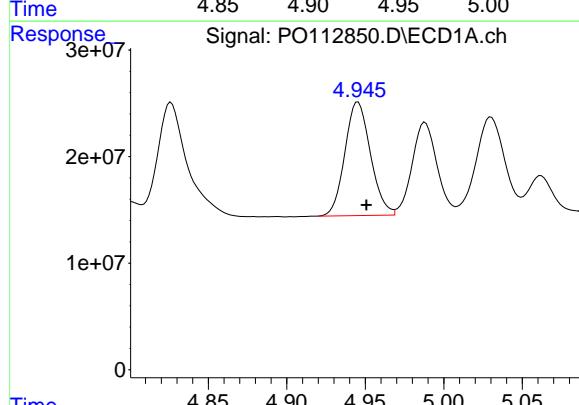


#14 AR-1232-4

R.T.: 4.945 min
 Delta R.T.: -0.005 min
 Response: 121075575
 Conc: 1155.96 ng/ml

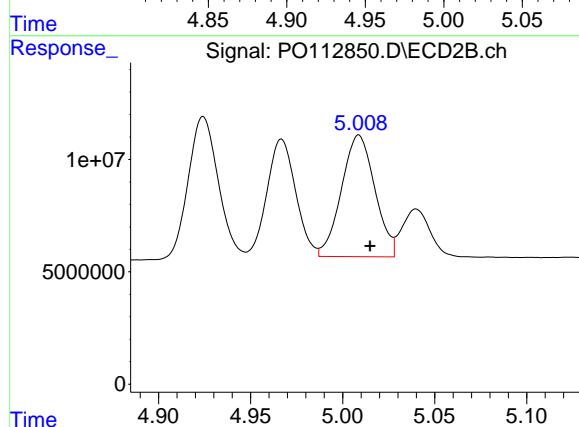

#14 AR-1232-4


R.T.: 5.009 min
 Delta R.T.: -0.006 min
 Response: 68260248
 Conc: 1140.92 ng/ml



#15 AR-1232-5


R.T.: 4.988 min
 Delta R.T.: -0.006 min
 Response: 94920489
 Conc: 1398.34 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

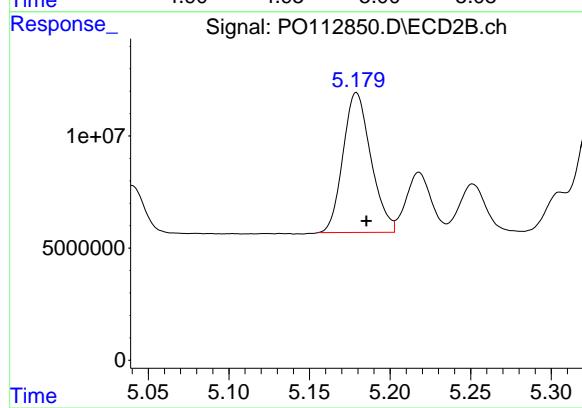


#15 AR-1232-5

R.T.: 5.179 min
 Delta R.T.: -0.006 min
 Response: 75085975
 Conc: 1151.57 ng/ml

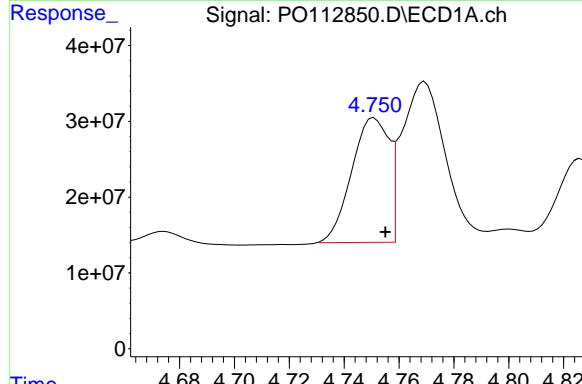


#16 AR-1242-1

R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 155309919
 Conc: 627.28 ng/ml

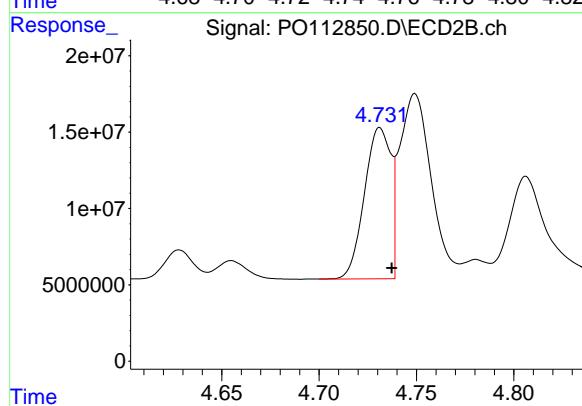

#16 AR-1242-1


R.T.: 4.731 min
 Delta R.T.: -0.006 min
 Response: 93205664
 Conc: 588.44 ng/ml



#17 AR-1242-2


R.T.: 4.769 min
 Delta R.T.: -0.005 min
 Response: 233914683
 Conc: 632.55 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

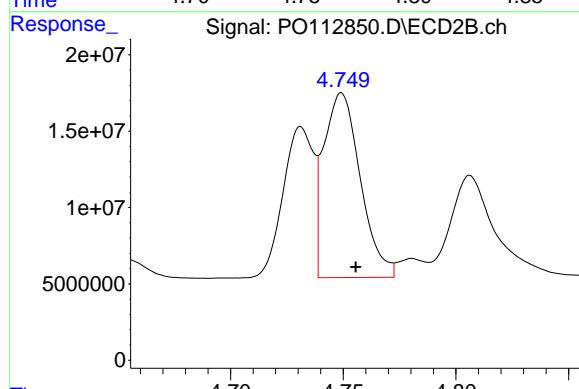


#17 AR-1242-2

R.T.: 4.749 min
 Delta R.T.: -0.006 min
 Response: 136585485
 Conc: 584.53 ng/ml

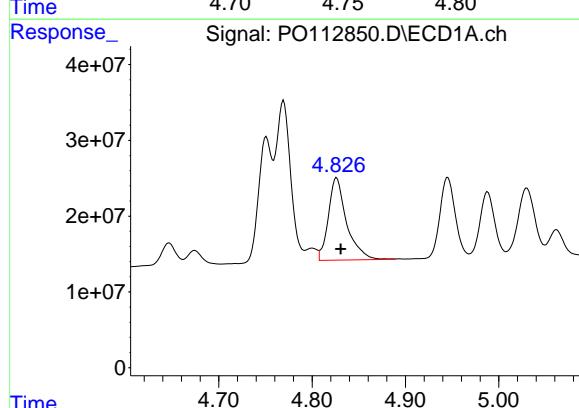


#18 AR-1242-3

R.T.: 4.826 min
 Delta R.T.: -0.005 min
 Response: 148051145
 Conc: 625.59 ng/ml

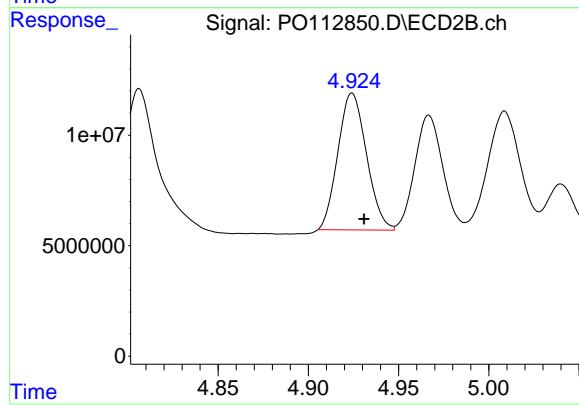

#18 AR-1242-3

R.T.: 4.924 min
 Delta R.T.: -0.006 min
 Response: 68284681
 Conc: 563.46 ng/ml

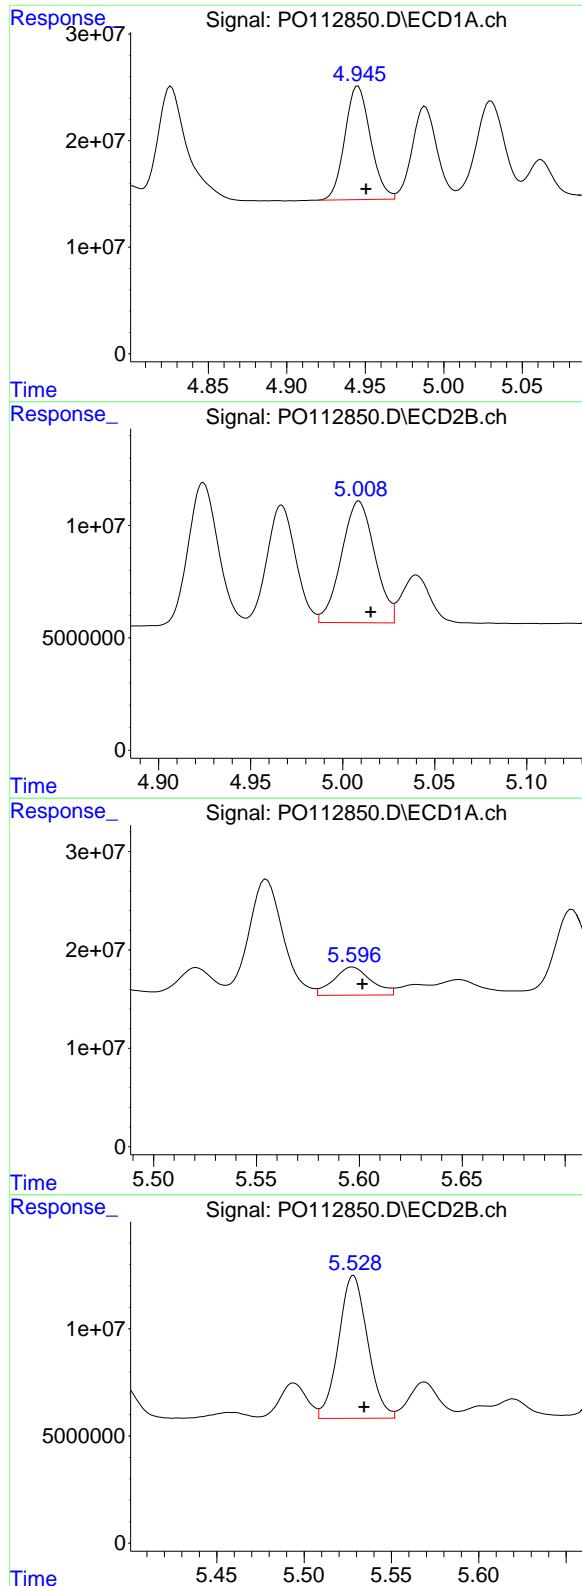

#19 AR-1242-4

R.T.: 4.945 min
 Delta R.T.: -0.005 min
 Response: 121075575
 Conc: 623.21 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.009 min
 Delta R.T.: -0.006 min
 Response: 68260248
 Conc: 556.14 ng/ml

#20 AR-1242-5

R.T.: 5.597 min
 Delta R.T.: -0.005 min
 Response: 36369268
 Conc: 170.02 ng/ml

#20 AR-1242-5

R.T.: 5.528 min
 Delta R.T.: -0.006 min
 Response: 77150754
 Conc: 479.28 ng/ml

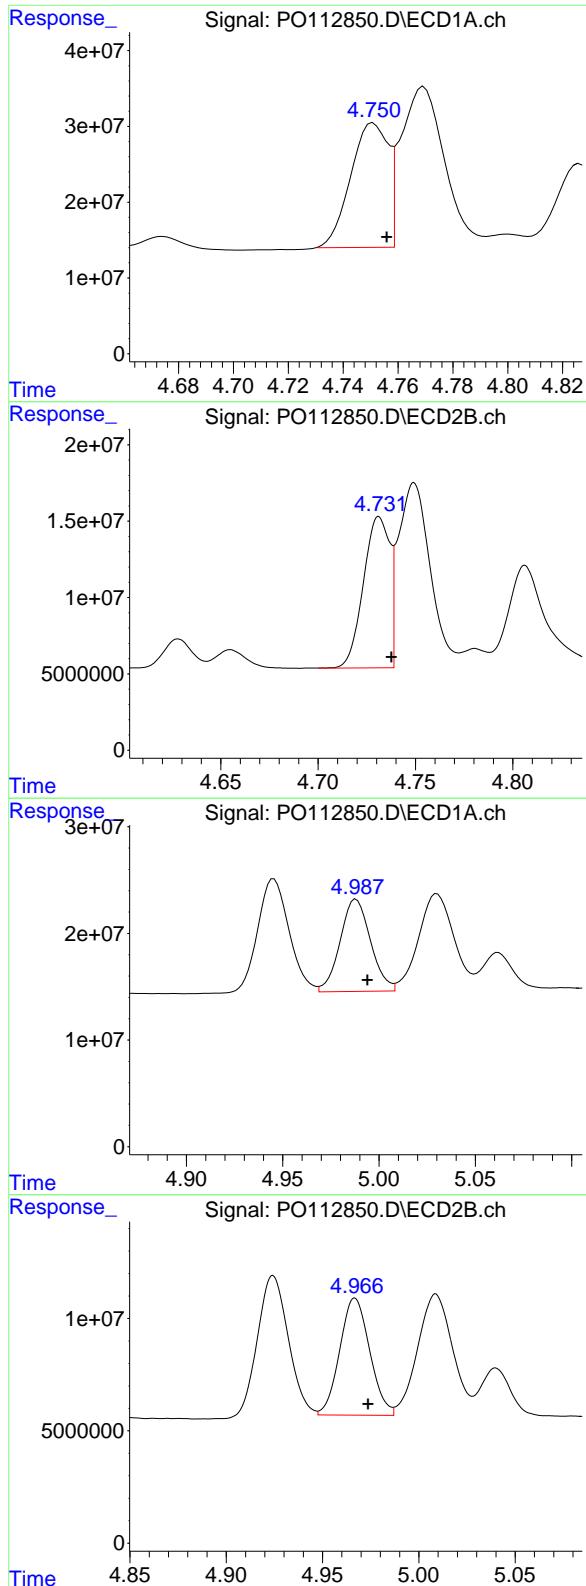

#21 AR-1248-1

R.T.: 4.751 min
 Delta R.T.: -0.005 min
 Response: 155309919
 Conc: 829.61 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#21 AR-1248-1


R.T.: 4.731 min
 Delta R.T.: -0.007 min
 Response: 93205664
 Conc: 767.07 ng/ml

#22 AR-1248-2

R.T.: 4.988 min
 Delta R.T.: -0.006 min
 Response: 94920489
 Conc: 372.07 ng/ml

#22 AR-1248-2

R.T.: 4.967 min
 Delta R.T.: -0.007 min
 Response: 56332621
 Conc: 332.78 ng/ml

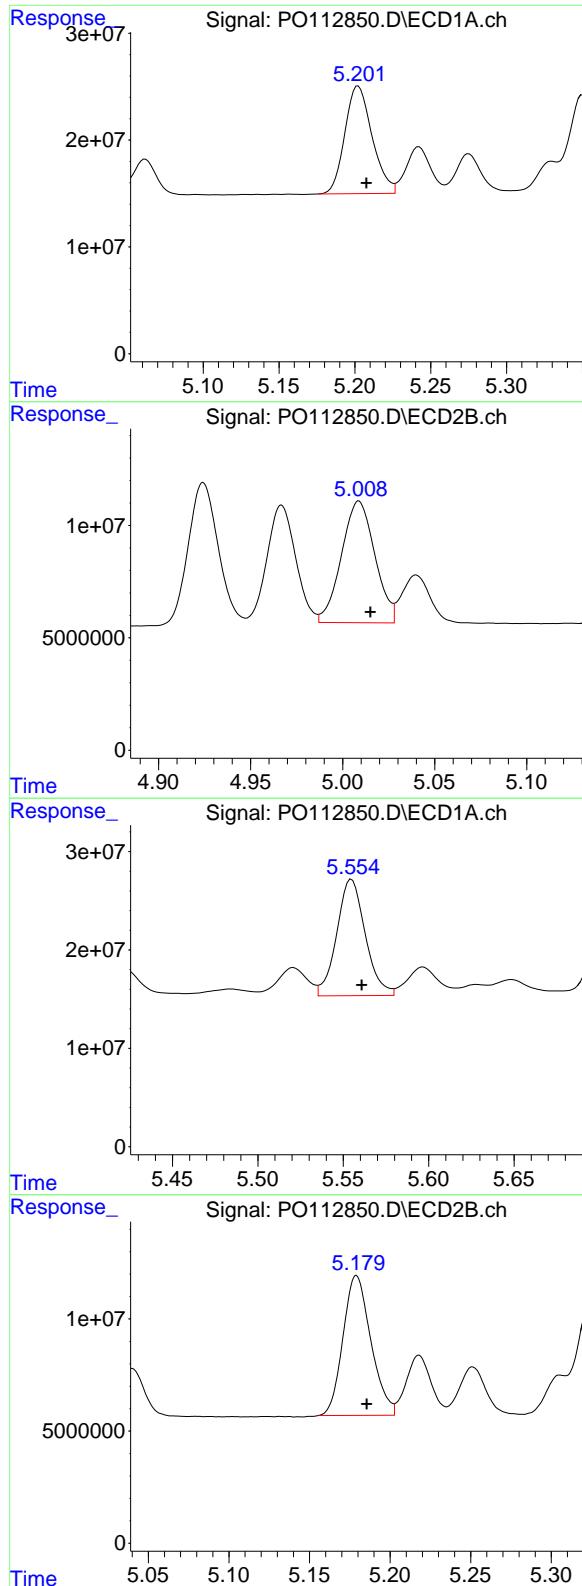

#23 AR-1248-3

R.T.: 5.202 min
 Delta R.T.: -0.005 min
 Response: 126164306
 Conc: 367.08 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.009 min
 Delta R.T.: -0.006 min
 Response: 68260248
 Conc: 384.25 ng/ml

#24 AR-1248-4

R.T.: 5.555 min
 Delta R.T.: -0.006 min
 Response: 137483056
 Conc: 270.59 ng/ml

#24 AR-1248-4

R.T.: 5.179 min
 Delta R.T.: -0.006 min
 Response: 75085975
 Conc: 360.38 ng/ml

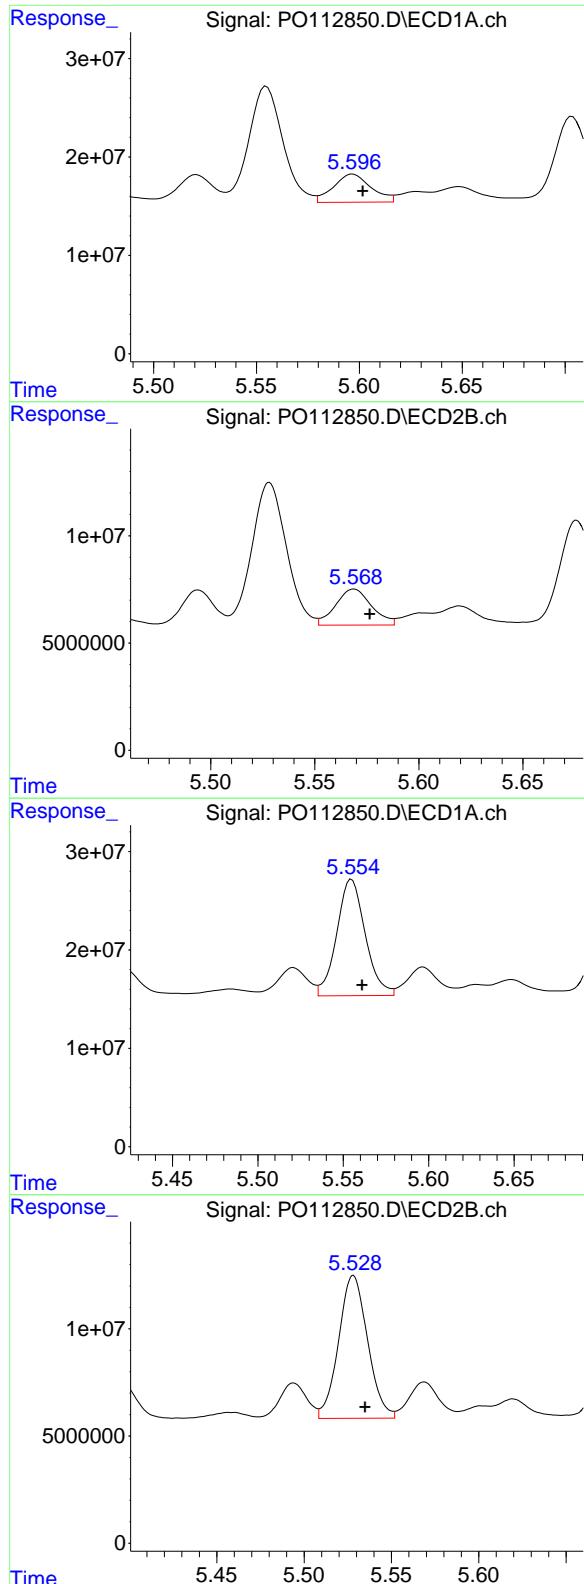

#25 AR-1248-5

R.T.: 5.597 min
 Delta R.T.: -0.005 min
 Response: 36369268
 Conc: 104.03 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.569 min
 Delta R.T.: -0.008 min
 Response: 20206764
 Conc: 94.09 ng/ml

#26 AR-1254-1

R.T.: 5.555 min
 Delta R.T.: -0.006 min
 Response: 137483056
 Conc: 250.44 ng/ml

#26 AR-1254-1


R.T.: 5.528 min
 Delta R.T.: -0.007 min
 Response: 77150754
 Conc: 234.77 ng/ml



#27 AR-1254-2


R.T.: 5.704 min
 Delta R.T.: -0.007 min
 Response: 102514866
 Conc: 210.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

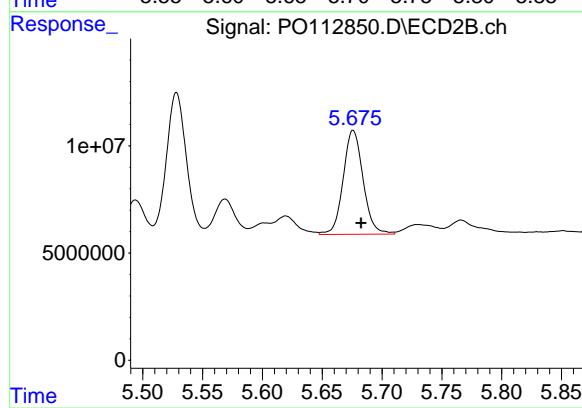


#27 AR-1254-2

R.T.: 5.676 min
 Delta R.T.: -0.007 min
 Response: 56225513
 Conc: 194.22 ng/ml

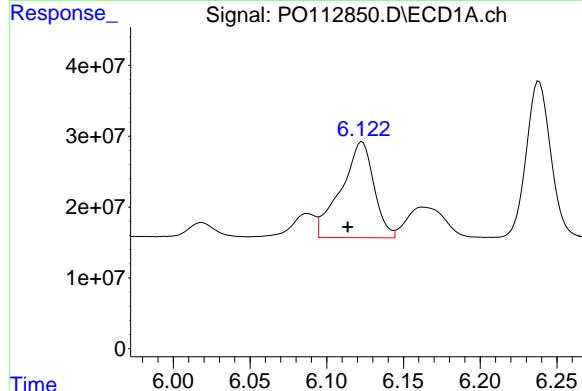


#28 AR-1254-3

R.T.: 6.123 min
 Delta R.T.: 0.009 min
 Response: 201995721
 Conc: 271.40 ng/ml

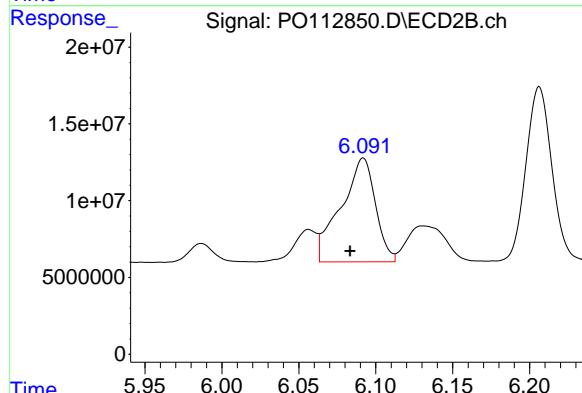

#28 AR-1254-3

R.T.: 6.092 min
 Delta R.T.: 0.009 min
 Response: 105456191
 Conc: 246.70 ng/ml

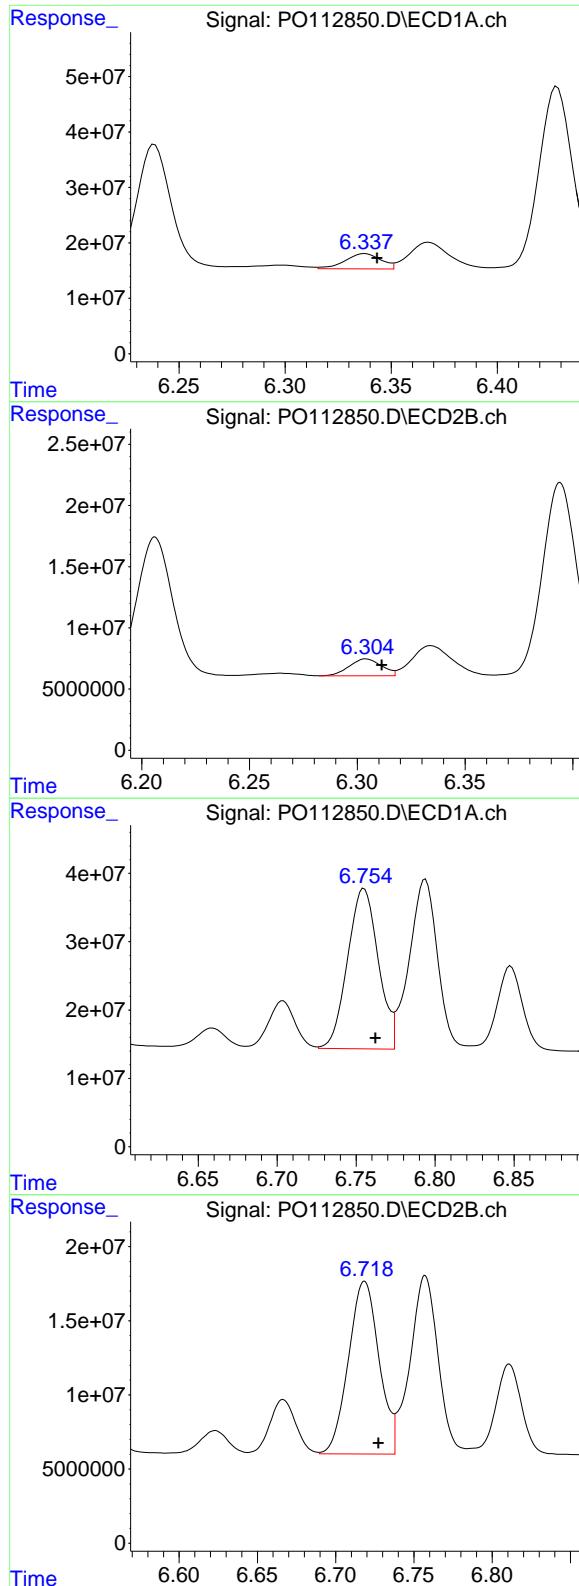

#29 AR-1254-4

R.T.: 6.338 min
 Delta R.T.: -0.006 min
 Response: 31938035
 Conc: 58.10 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.304 min
 Delta R.T.: -0.007 min
 Response: 14309000
 Conc: 52.42 ng/ml

#30 AR-1254-5

R.T.: 6.755 min
 Delta R.T.: -0.007 min
 Response: 317337305
 Conc: 448.33 ng/ml

#30 AR-1254-5

R.T.: 6.718 min
 Delta R.T.: -0.009 min
 Response: 158568170
 Conc: 474.73 ng/ml

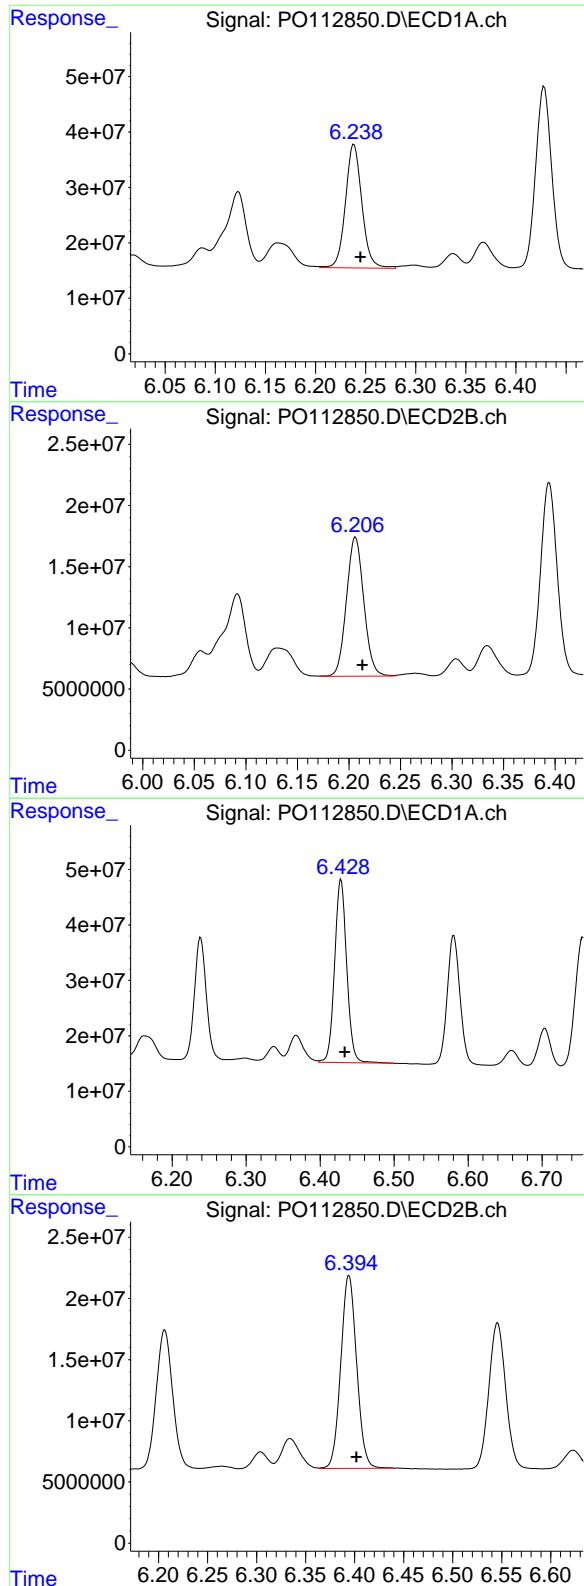

#31 AR-1260-1

R.T.: 6.238 min
 Delta R.T.: -0.006 min
 Response: 254471304
 Conc: 579.22 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#31 AR-1260-1


R.T.: 6.206 min
 Delta R.T.: -0.007 min
 Response: 133012078
 Conc: 535.24 ng/ml

#32 AR-1260-2

R.T.: 6.428 min
 Delta R.T.: -0.005 min
 Response: 376624885
 Conc: 547.50 ng/ml

#32 AR-1260-2

R.T.: 6.394 min
 Delta R.T.: -0.008 min
 Response: 177535660
 Conc: 538.81 ng/ml

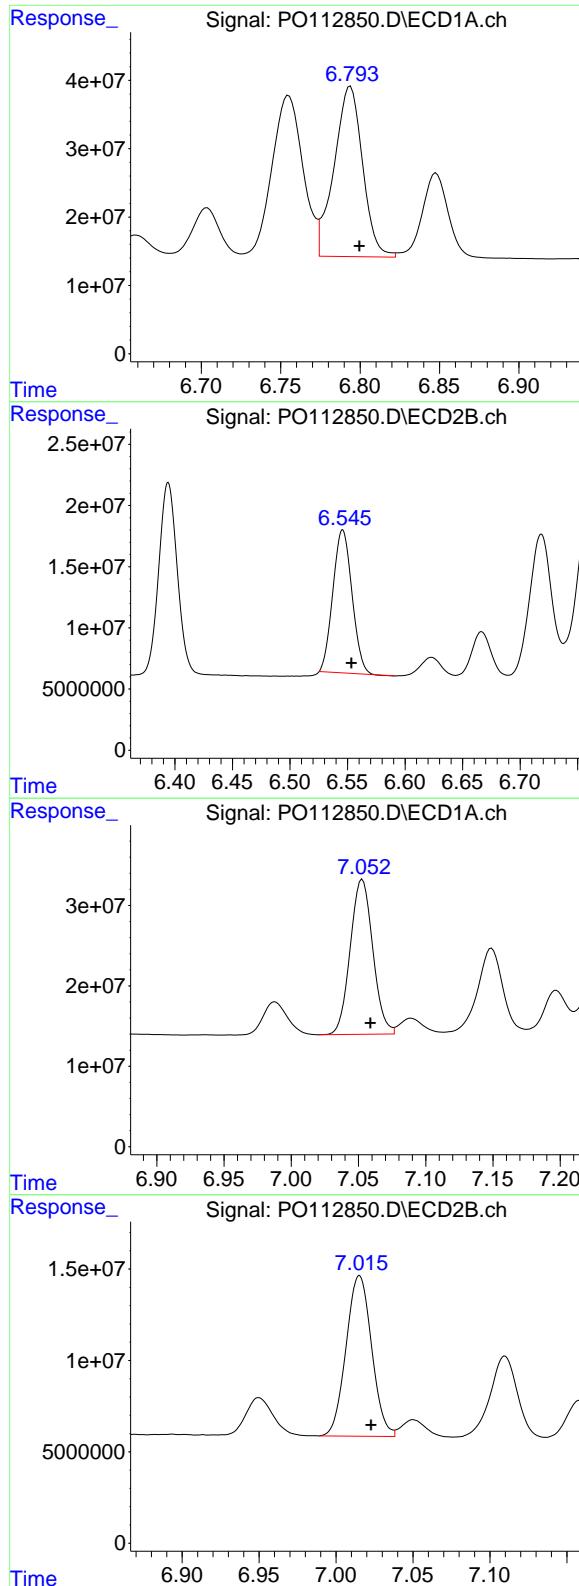

#33 AR-1260-3

R.T.: 6.794 min
 Delta R.T.: -0.006 min
 Response: 310912948
 Conc: 528.75 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#33 AR-1260-3


R.T.: 6.546 min
 Delta R.T.: -0.008 min
 Response: 135120158
 Conc: 525.92 ng/ml

#34 AR-1260-4

R.T.: 7.053 min
 Delta R.T.: -0.006 min
 Response: 224984392
 Conc: 498.85 ng/ml

#34 AR-1260-4

R.T.: 7.015 min
 Delta R.T.: -0.007 min
 Response: 101418669
 Conc: 530.13 ng/ml

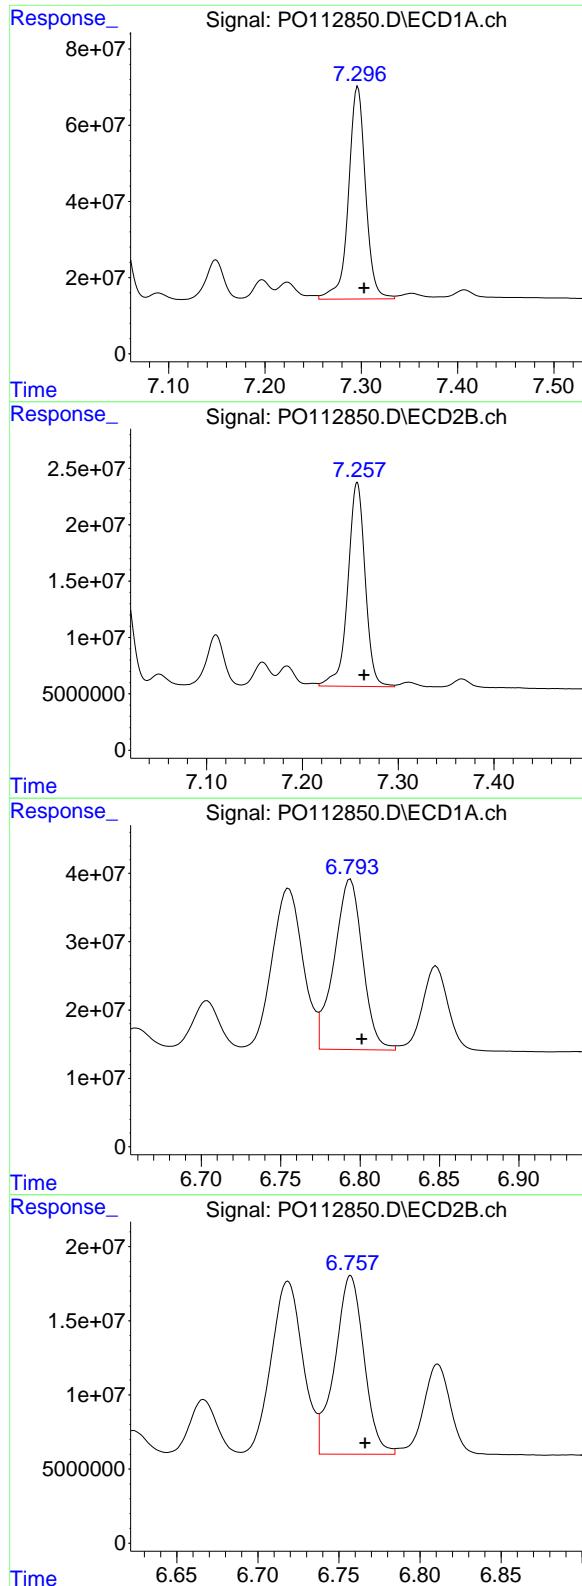

#35 AR-1260-5

R.T.: 7.296 min
Delta R.T.: -0.006 min
Response: 685410891
Conc: 553.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#35 AR-1260-5


R.T.: 7.257 min
Delta R.T.: -0.007 min
Response: 226664288
Conc: 549.90 ng/ml

#36 AR-1262-1

R.T.: 6.794 min
Delta R.T.: -0.007 min
Response: 310912948
Conc: 334.60 ng/ml

#36 AR-1262-1

R.T.: 6.757 min
Delta R.T.: -0.009 min
Response: 150582424
Conc: 363.00 ng/ml

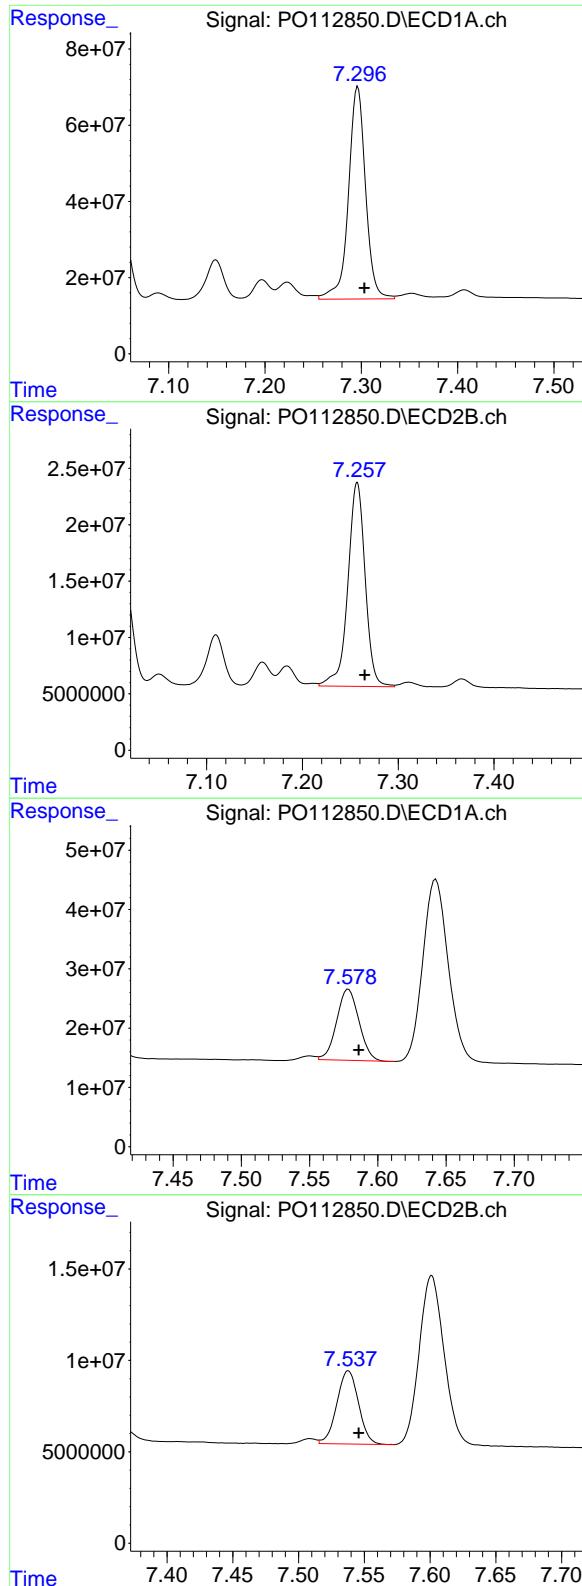

#37 AR-1262-2

R.T.: 7.296 min
Delta R.T.: -0.007 min
Response: 685410891
Conc: 460.93 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#37 AR-1262-2


R.T.: 7.257 min
Delta R.T.: -0.008 min
Response: 226664288
Conc: 439.66 ng/ml

#38 AR-1262-3

R.T.: 7.578 min
Delta R.T.: -0.008 min
Response: 136457043
Conc: 231.18 ng/ml

#38 AR-1262-3


R.T.: 7.538 min
Delta R.T.: -0.008 min
Response: 46051874
Conc: 246.89 ng/ml



#39 AR-1262-4


R.T.: 7.643 min
 Delta R.T.: -0.008 min
 Response: 401502752
 Conc: 403.86 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

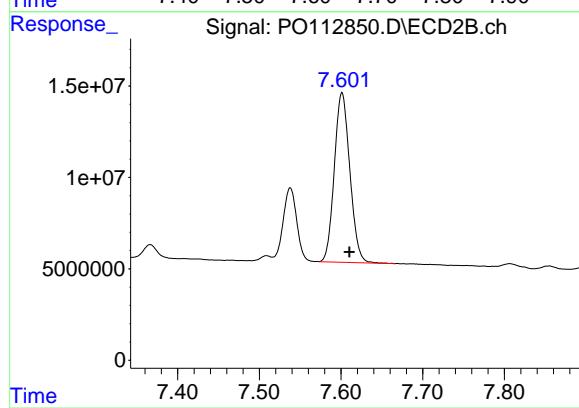


#39 AR-1262-4

R.T.: 7.601 min
 Delta R.T.: -0.009 min
 Response: 122549526
 Conc: 425.37 ng/ml

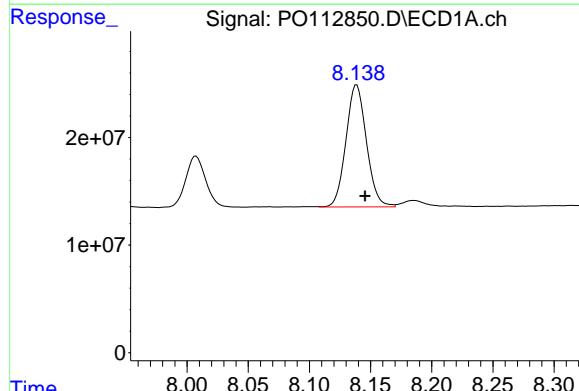


#40 AR-1262-5

R.T.: 8.139 min
 Delta R.T.: -0.007 min
 Response: 132253896
 Conc: 304.69 ng/ml

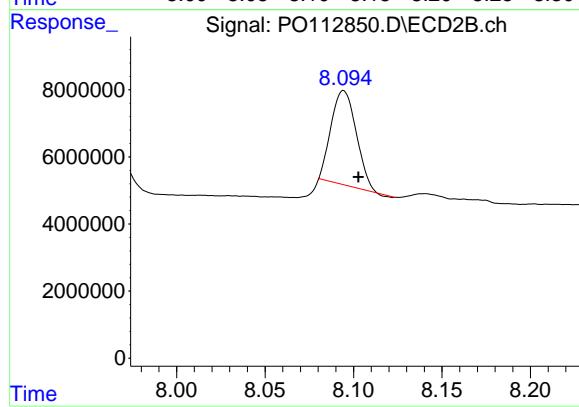

#40 AR-1262-5


R.T.: 8.094 min
 Delta R.T.: -0.008 min
 Response: 27693523
 Conc: 278.32 ng/ml



#41 AR-1268-1


R.T.: 7.578 min
 Delta R.T.: -0.007 min
 Response: 136457043
 Conc: 77.92 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

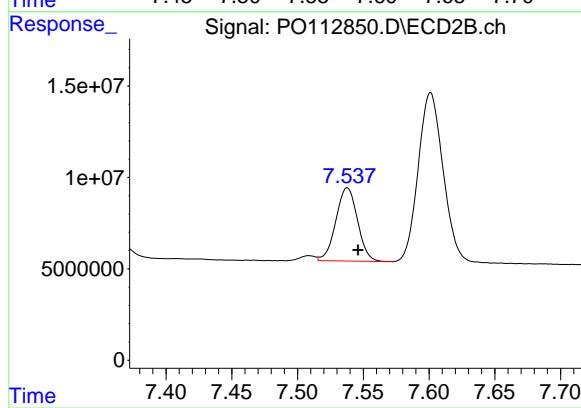


#41 AR-1268-1

R.T.: 7.538 min
 Delta R.T.: -0.008 min
 Response: 46051874
 Conc: 88.93 ng/ml




#42 AR-1268-2

R.T.: 7.643 min
 Delta R.T.: -0.009 min
 Response: 401502752
 Conc: 272.57 ng/ml

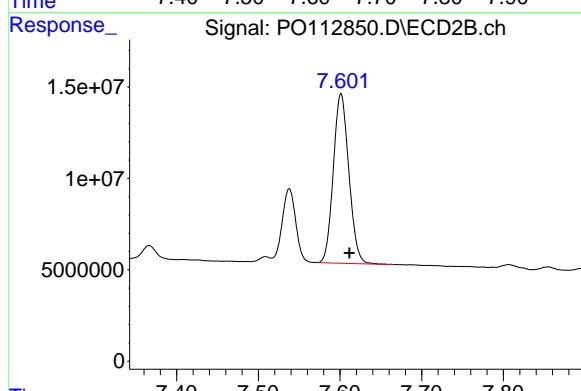

#42 AR-1268-2


R.T.: 7.601 min
 Delta R.T.: -0.010 min
 Response: 122549526
 Conc: 288.31 ng/ml



#43 AR-1268-3


R.T.: 7.849 min
Delta R.T.: -0.007 min
Response: 6266792
Conc: 5.00 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

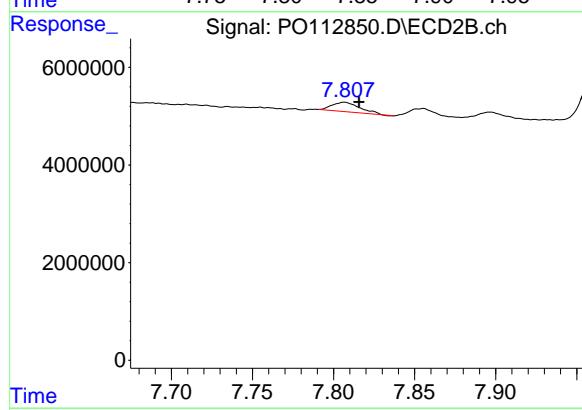


#43 AR-1268-3

R.T.: 7.807 min
Delta R.T.: -0.009 min
Response: 2290388
Conc: 7.13 ng/ml

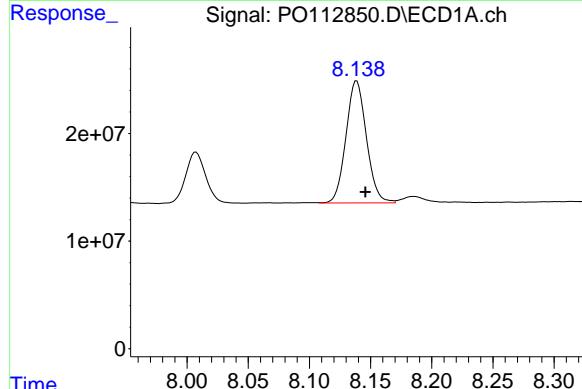


#44 AR-1268-4

R.T.: 8.139 min
Delta R.T.: -0.007 min
Response: 132253896
Conc: 274.46 ng/ml

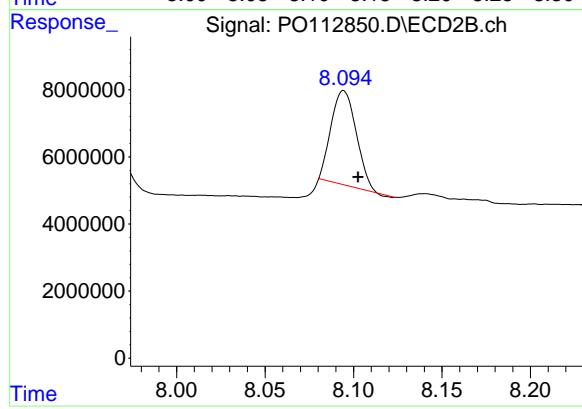

#44 AR-1268-4


R.T.: 8.094 min
Delta R.T.: -0.008 min
Response: 27693523
Conc: 248.83 ng/ml

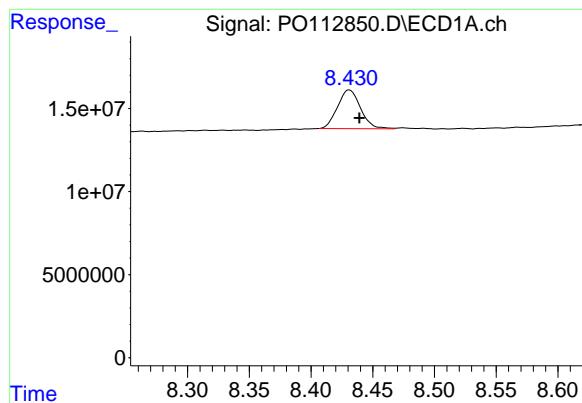

#45 AR-1268-5

R.T.: 8.431 min
Delta R.T.: -0.008 min
Response: 30321851
Conc: 9.03 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

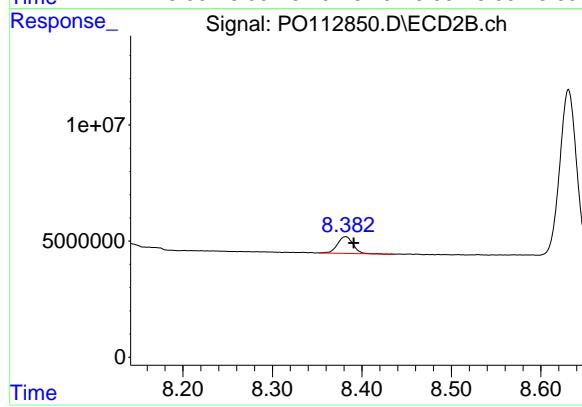

#45 AR-1268-5

R.T.: 8.382 min
Delta R.T.: -0.009 min
Response: 8645473
Conc: 11.81 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:50
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:39:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|-------|-------|---------|----------|--------|--------|
| 1) SA Tetrachlor... | 3.667 | 3.659 | 469.7E6 | 274.6E6 | 57.765 | 55.269 |
| 2) SA Decachlor... | 8.687 | 8.633 | 358.1E6 | 93971024 | 48.973 | 53.178 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|-----------|
| 3) L1 AR-1016-1 | 4.752 | 4.734 | 147.4E6 | 91367071 | 549.288 | 522.077 |
| 4) L1 AR-1016-2 | 4.770 | 4.751 | 229.3E6 | 134.7E6 | 564.529 | 517.092 |
| 5) L1 AR-1016-3 | 4.827 | 4.926 | 144.2E6 | 70193896 | 551.218 | 516.259 |
| 6) L1 AR-1016-4 | 4.947 | 4.969 | 116.7E6 | 57301939 | 550.721 | 515.840 |
| 7) L1 AR-1016-5 | 5.203 | 5.181 | 128.2E6 | 75537038 | 584.153 | 527.114 |
| 8) L2 AR-1221-1 | 3.877 | 3.867 | 13148124 | 9180422 | 136.025 | 136.480 |
| 9) L2 AR-1221-2 | 3.965 | 3.954 | 19963791 | 13995329 | 277.807 | 275.890 |
| 10) L2 AR-1221-3 | 4.039 | 4.028 | 77808137 | 50607541 | 327.322 | 319.231 |
| 11) L3 AR-1232-1 | 4.039 | 4.028 | 77808137 | 50607541 | 416.134 | 399.902 |
| 12) L3 AR-1232-2 | 4.531 | 4.751 | 115.3E6 | 134.7E6 | 1071.630 | 1027.030 |
| 13) L3 AR-1232-3 | 4.770 | 4.926 | 229.3E6 | 70193896 | 1108.636 | 1044.602 |
| 14) L3 AR-1232-4 | 4.947 | 5.010 | 116.7E6 | 68905552 | 1113.855 | 1151.706 |
| 15) L3 AR-1232-5 | 4.989 | 5.181 | 90857298 | 75537038 | 1338.481 | 1158.490 |
| 16) L4 AR-1242-1 | 4.752 | 4.734 | 147.4E6 | 91367071 | 595.376 | 576.834 |
| 17) L4 AR-1242-2 | 4.770 | 4.751 | 229.3E6 | 134.7E6 | 619.981 | 576.463 |
| 18) L4 AR-1242-3 | 4.827 | 4.926 | 144.2E6 | 70193896 | 609.485 | 579.210 |
| 19) L4 AR-1242-4 | 4.947 | 5.010 | 116.7E6 | 68905552 | 600.506 | 561.397 |
| 20) L4 AR-1242-5 | 5.598 | 5.530 | 35516814 | 76792861 | 166.032 | 477.059 # |
| 21) L5 AR-1248-1 | 4.752 | 4.734 | 147.4E6 | 91367071 | 787.411 | 751.935 |
| 22) L5 AR-1248-2 | 4.989 | 4.969 | 90857298 | 57301939 | 356.146 | 338.505 |
| 23) L5 AR-1248-3 | 5.203 | 5.010 | 128.2E6 | 68905552 | 373.011 | 387.879 |
| 24) L5 AR-1248-4 | 5.556 | 5.181 | 135.5E6 | 75537038 | 266.615 | 362.541 # |
| 25) L5 AR-1248-5 | 5.598 | 5.571 | 35516814 | 21481781 | 101.595 | 100.025 |
| 26) L6 AR-1254-1 | 5.556 | 5.530 | 135.5E6 | 76792861 | 246.761 | 233.682 |
| 27) L6 AR-1254-2 | 5.705 | 5.678 | 102.0E6 | 56804415 | 209.968 | 196.222 |
| 28) L6 AR-1254-3 | 6.125 | 6.094 | 191.3E6 | 103.5E6 | 257.015 | 242.166 |
| 29) L6 AR-1254-4 | 6.339 | 6.306 | 28484111 | 13812616 | 51.817 | 50.603 |
| 30) L6 AR-1254-5 | 6.756 | 6.721 | 340.1E6 | 156.7E6 | 480.427 | 469.129 |
| 31) L7 AR-1260-1 | 6.240 | 6.208 | 241.8E6 | 130.2E6 | 550.345 | 523.958 |
| 32) L7 AR-1260-2 | 6.430 | 6.396 | 373.8E6 | 175.2E6 | 543.411 | 531.849 |
| 33) L7 AR-1260-3 | 6.795 | 6.548 | 335.7E6 | 137.9E6 | 570.949 | 536.590 |
| 34) L7 AR-1260-4 | 7.055 | 7.017 | 244.6E6 | 104.0E6 | 542.265 | 543.785 |
| 35) L7 AR-1260-5 | 7.297 | 7.260 | 656.7E6 | 231.2E6 | 529.972 | 560.820 |
| 36) L8 AR-1262-1 | 6.795 | 6.760 | 335.7E6 | 149.6E6 | 361.307 | 360.738 |
| 37) L8 AR-1262-2 | 7.297 | 7.260 | 656.7E6 | 231.2E6 | 441.628 | 448.392 |
| 38) L8 AR-1262-3 | 7.580 | 7.540 | 135.6E6 | 47945338 | 229.672 | 257.045 |
| 39) L8 AR-1262-4 | 7.643 | 7.603 | 400.9E6 | 127.7E6 | 403.259 | 443.370 |
| 40) L8 AR-1262-5 | 8.140 | 8.096 | 139.2E6 | 31782749 | 320.641 | 319.414 |
| 41) L9 AR-1268-1 | 7.580 | 7.540 | 135.6E6 | 47945338 | 77.415 | 92.583 |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:50
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:39:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|-------|-------|----------|----------|---------|---------|
| 42) L9 AR-1268-2 | 7.643 | 7.603 | 400.9E6 | 127.7E6 | 272.166 | 300.511 |
| 43) L9 AR-1268-3 | 7.851 | 7.807 | 5704040 | 1601864 | 4.555 | 4.986 |
| 44) L9 AR-1268-4 | 8.140 | 8.096 | 139.2E6 | 31782749 | 288.832 | 285.571 |
| 45) L9 AR-1268-5 | 8.432 | 8.383 | 33094872 | 8792996 | 9.858 | 12.017 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_0\Data\P0081225\
 Data File : P0112865.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:50
 Operator : YP/AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_O
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:39:22 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_0\methods\P0072325.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Jul 24 04:54:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

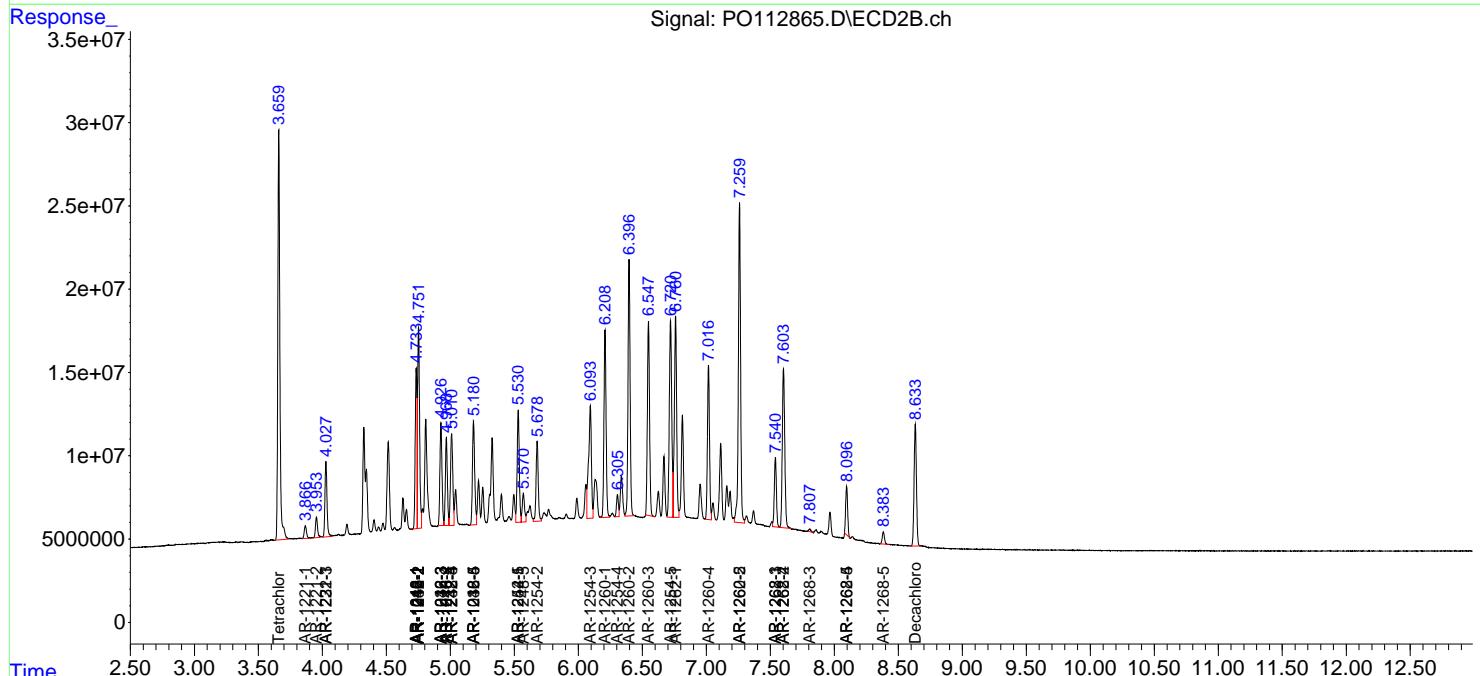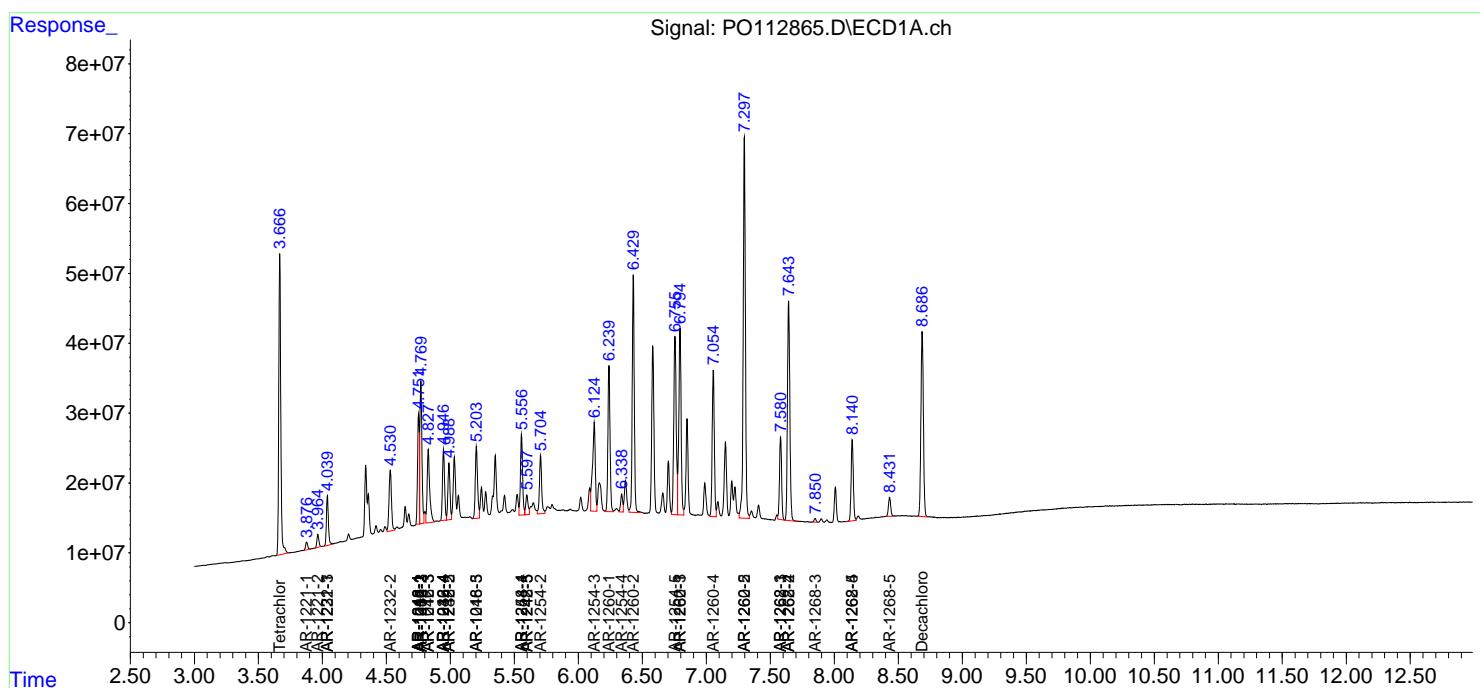

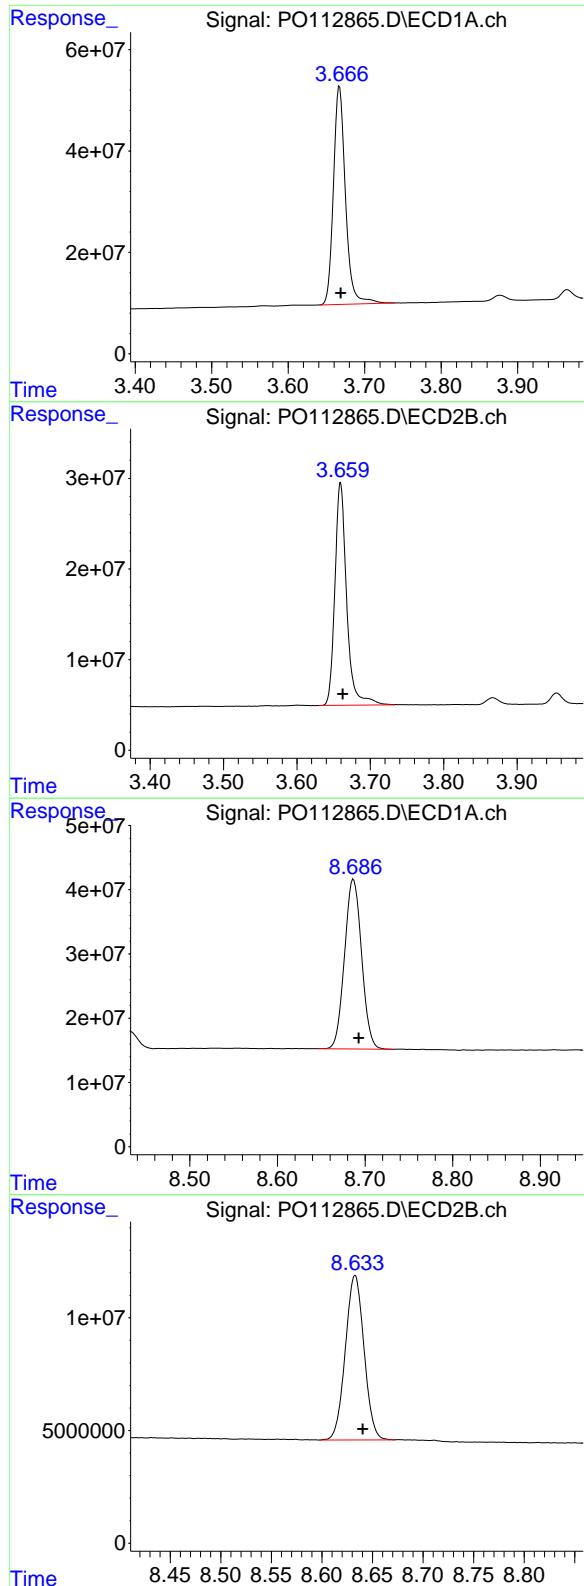

#1 Tetrachloro-m-xylene

R.T.: 3.667 min
 Delta R.T.: -0.002 min
 Response: 469719514
 Conc: 57.76 ng/ml

Instrument:

ECD_O

ClientSampleId :

AR1660CCC500

#1 Tetrachloro-m-xylene


R.T.: 3.659 min
 Delta R.T.: -0.003 min
 Response: 274642690
 Conc: 55.27 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.687 min
 Delta R.T.: -0.006 min
 Response: 358077397
 Conc: 48.97 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.633 min
 Delta R.T.: -0.008 min
 Response: 93971024
 Conc: 53.18 ng/ml

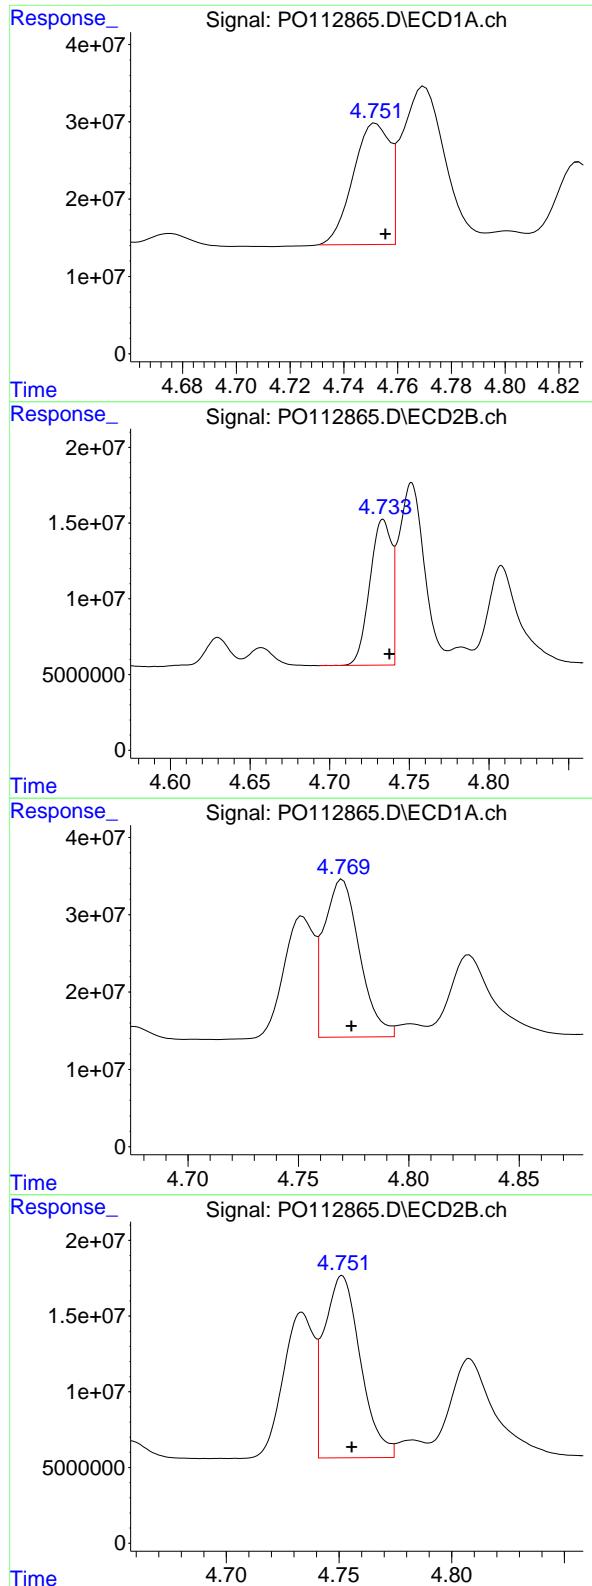

#3 AR-1016-1

R.T.: 4.752 min
 Delta R.T.: -0.004 min
 Response: 147410245
 Conc: 549.29 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#3 AR-1016-1


R.T.: 4.734 min
 Delta R.T.: -0.004 min
 Response: 91367071
 Conc: 522.08 ng/ml

#4 AR-1016-2

R.T.: 4.770 min
 Delta R.T.: -0.004 min
 Response: 229265156
 Conc: 564.53 ng/ml

#4 AR-1016-2

R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 134699953
 Conc: 517.09 ng/ml

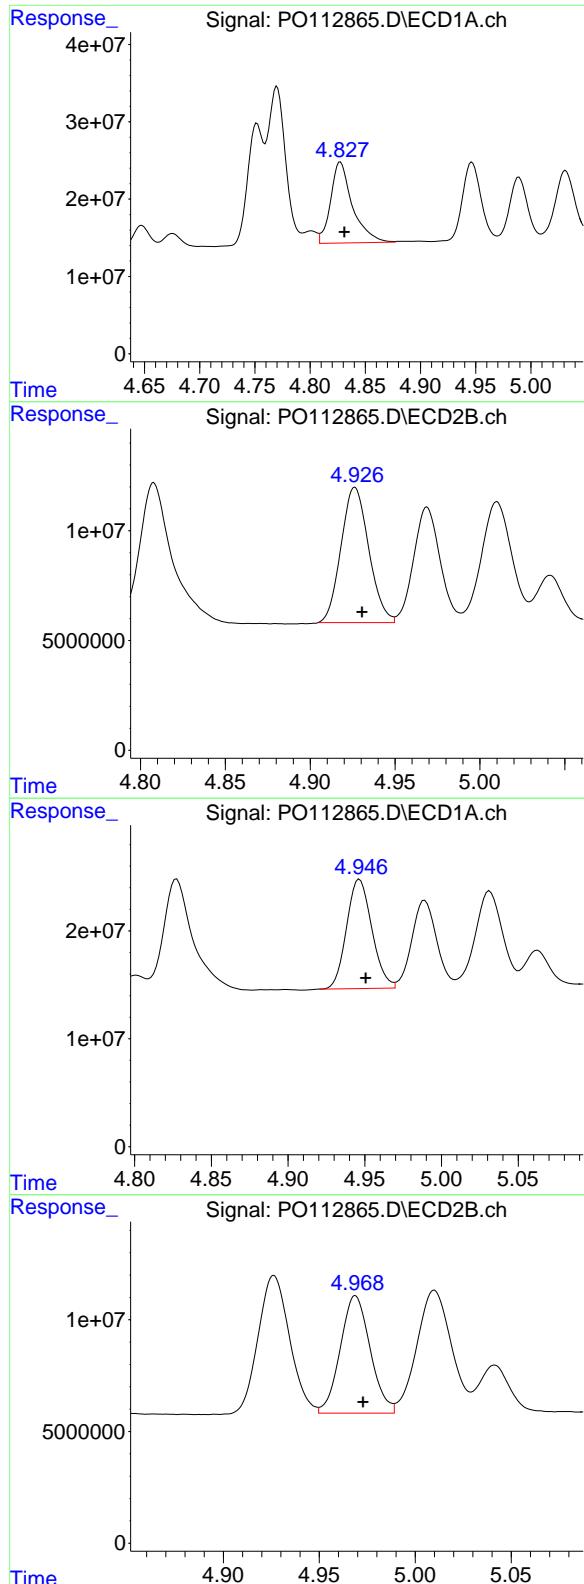

#5 AR-1016-3

R.T.: 4.827 min
 Delta R.T.: -0.004 min
 Response: 144239367
 Conc: 551.22 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#5 AR-1016-3


R.T.: 4.926 min
 Delta R.T.: -0.004 min
 Response: 70193896
 Conc: 516.26 ng/ml

#6 AR-1016-4

R.T.: 4.947 min
 Delta R.T.: -0.004 min
 Response: 116665542
 Conc: 550.72 ng/ml

#6 AR-1016-4

R.T.: 4.969 min
 Delta R.T.: -0.004 min
 Response: 57301939
 Conc: 515.84 ng/ml

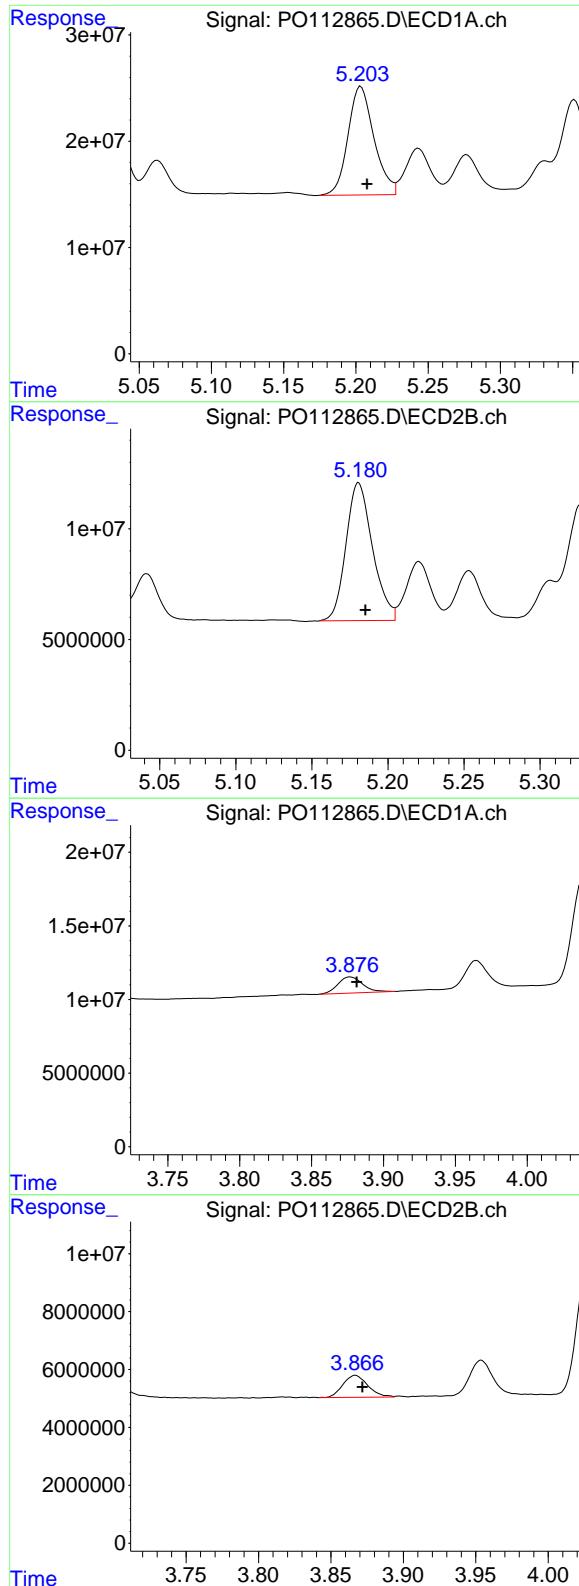

#7 AR-1016-5

R.T.: 5.203 min
 Delta R.T.: -0.004 min
 Response: 128204484
 Conc: 584.15 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#7 AR-1016-5


R.T.: 5.181 min
 Delta R.T.: -0.005 min
 Response: 75537038
 Conc: 527.11 ng/ml

#8 AR-1221-1

R.T.: 3.877 min
 Delta R.T.: -0.005 min
 Response: 13148124
 Conc: 136.02 ng/ml

#8 AR-1221-1

R.T.: 3.867 min
 Delta R.T.: -0.005 min
 Response: 9180422
 Conc: 136.48 ng/ml

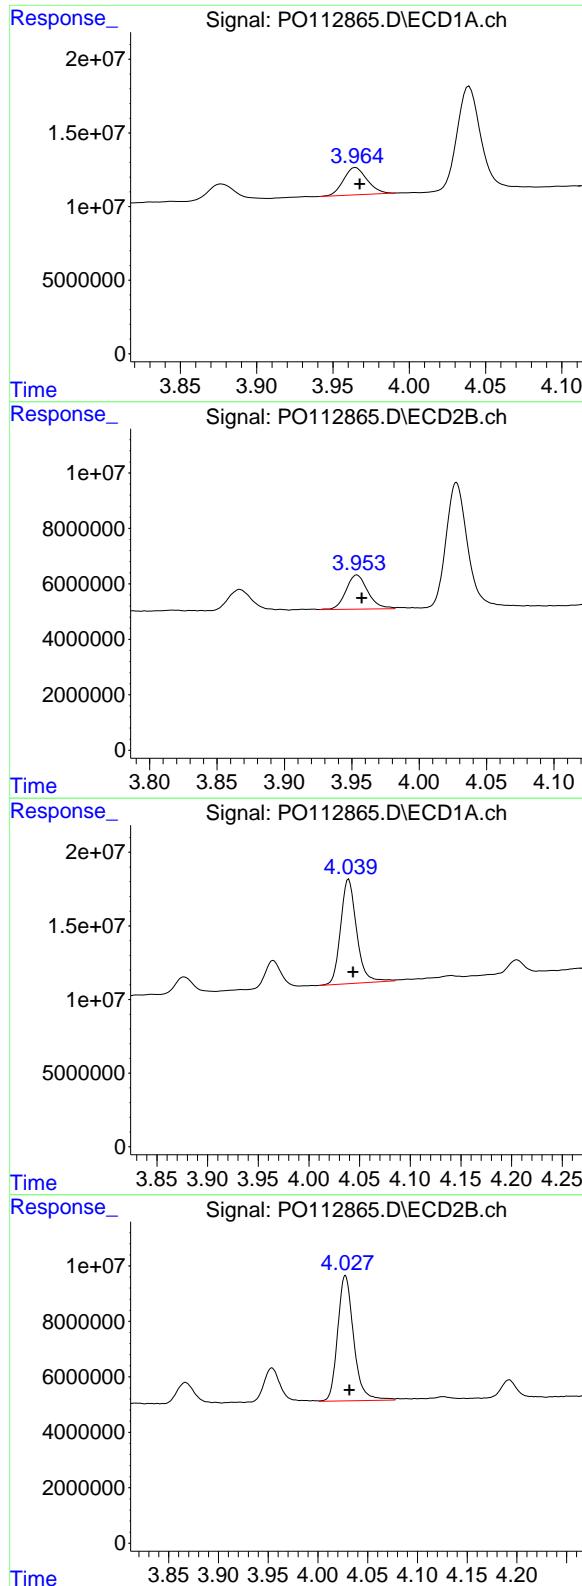

#9 AR-1221-2

R.T.: 3.965 min
 Delta R.T.: -0.003 min
 Response: 19963791
 Conc: 277.81 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 3.954 min
 Delta R.T.: -0.004 min
 Response: 13995329
 Conc: 275.89 ng/ml

#10 AR-1221-3

R.T.: 4.039 min
 Delta R.T.: -0.004 min
 Response: 77808137
 Conc: 327.32 ng/ml

#10 AR-1221-3

R.T.: 4.028 min
 Delta R.T.: -0.004 min
 Response: 50607541
 Conc: 319.23 ng/ml

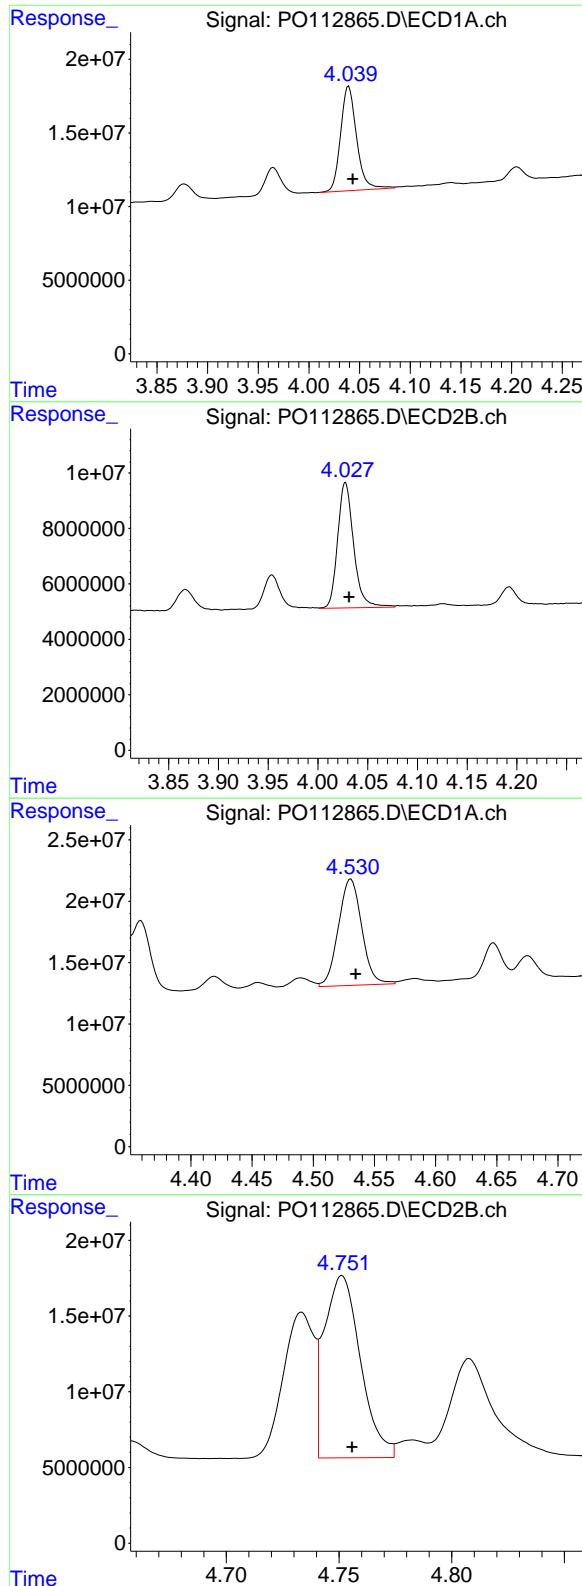

#11 AR-1232-1

R.T.: 4.039 min
 Delta R.T.: -0.004 min
 Response: 77808137
 Conc: 416.13 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.028 min
 Delta R.T.: -0.004 min
 Response: 50607541
 Conc: 399.90 ng/ml

#12 AR-1232-2

R.T.: 4.531 min
 Delta R.T.: -0.004 min
 Response: 115333904
 Conc: 1071.63 ng/ml

#12 AR-1232-2


R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 134699953
 Conc: 1027.03 ng/ml

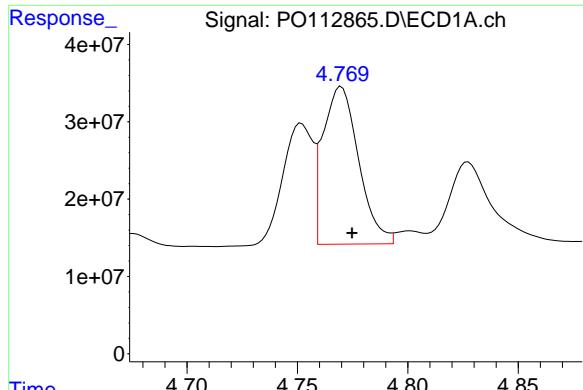

#13 AR-1232-3


R.T.: 4.770 min
 Delta R.T.: -0.005 min
 Response: 229265156
 Conc: 1108.64 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

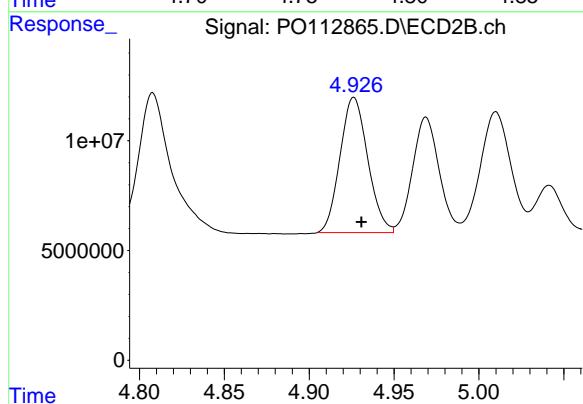


#13 AR-1232-3

R.T.: 4.926 min
 Delta R.T.: -0.004 min
 Response: 70193896
 Conc: 1044.60 ng/ml

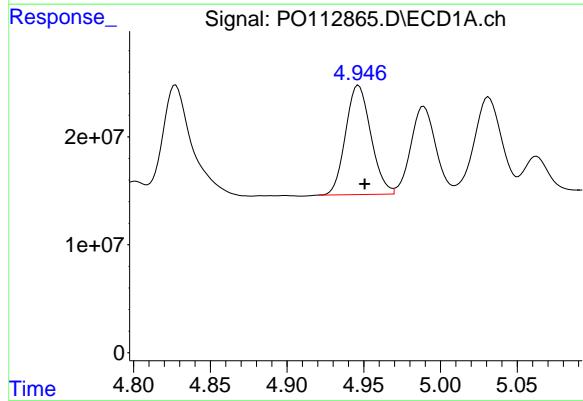


#14 AR-1232-4

R.T.: 4.947 min
 Delta R.T.: -0.004 min
 Response: 116665542
 Conc: 1113.86 ng/ml

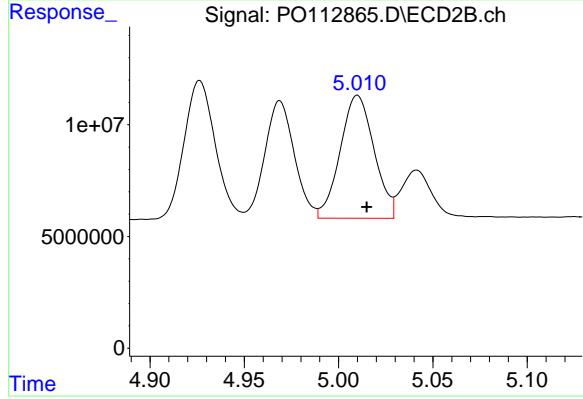

#14 AR-1232-4


R.T.: 5.010 min
 Delta R.T.: -0.005 min
 Response: 68905552
 Conc: 1151.71 ng/ml

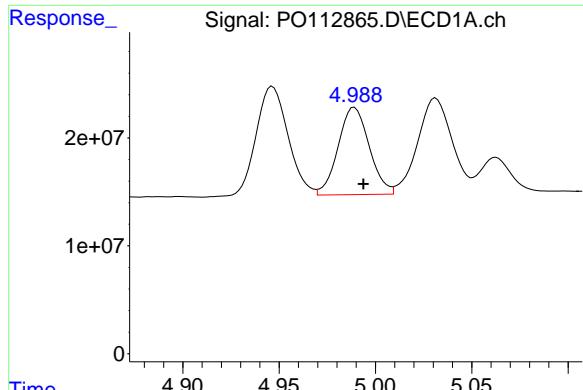

#15 AR-1232-5


R.T.: 4.989 min
 Delta R.T.: -0.005 min
 Response: 90857298
 Conc: 1338.48 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

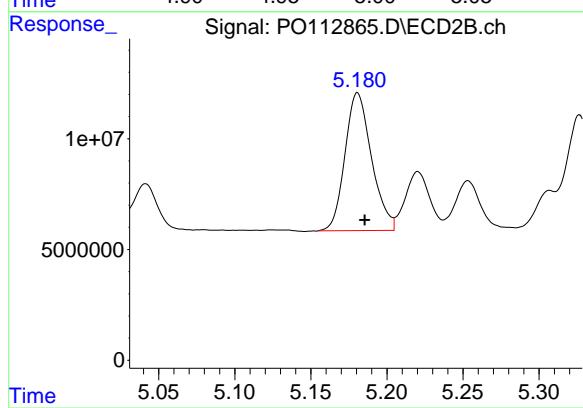


#15 AR-1232-5

R.T.: 5.181 min
 Delta R.T.: -0.005 min
 Response: 75537038
 Conc: 1158.49 ng/ml

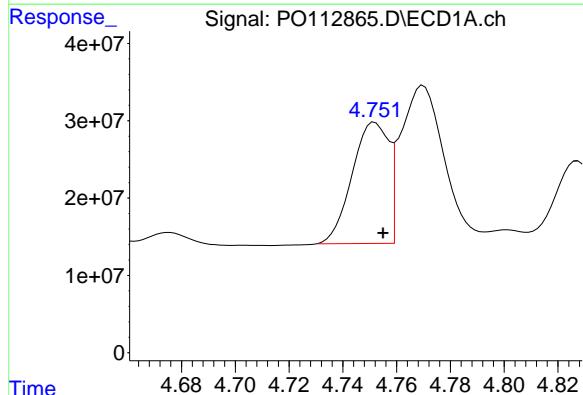


#16 AR-1242-1

R.T.: 4.752 min
 Delta R.T.: -0.003 min
 Response: 147410245
 Conc: 595.38 ng/ml

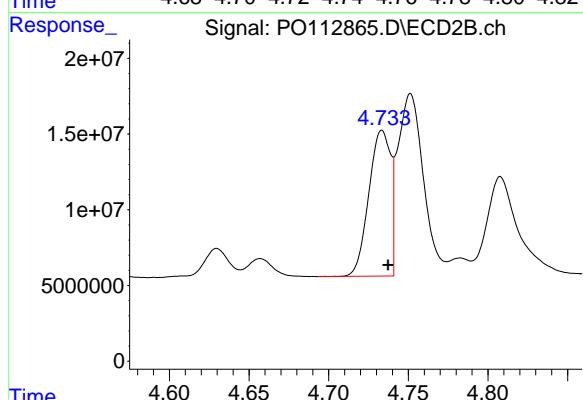

#16 AR-1242-1


R.T.: 4.734 min
 Delta R.T.: -0.004 min
 Response: 91367071
 Conc: 576.83 ng/ml



#17 AR-1242-2


R.T.: 4.770 min
 Delta R.T.: -0.004 min
 Response: 229265156
 Conc: 619.98 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

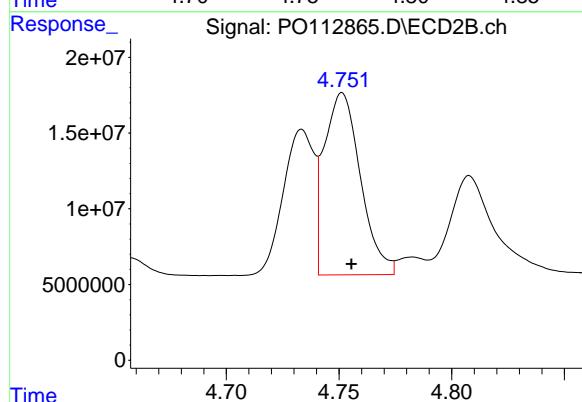


#17 AR-1242-2

R.T.: 4.751 min
 Delta R.T.: -0.004 min
 Response: 134699953
 Conc: 576.46 ng/ml

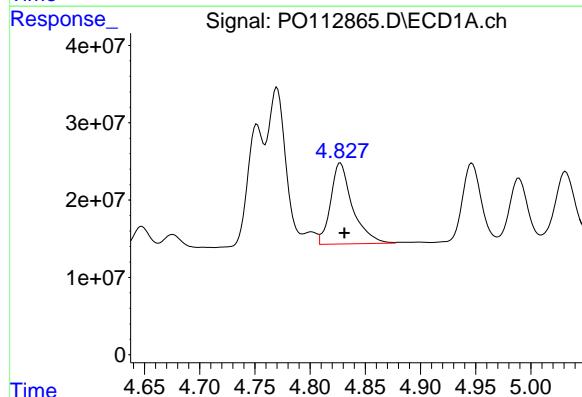


#18 AR-1242-3

R.T.: 4.827 min
 Delta R.T.: -0.003 min
 Response: 144239367
 Conc: 609.48 ng/ml

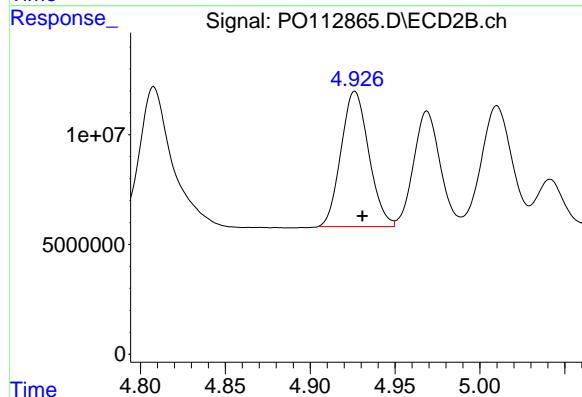

#18 AR-1242-3

R.T.: 4.926 min
 Delta R.T.: -0.004 min
 Response: 70193896
 Conc: 579.21 ng/ml

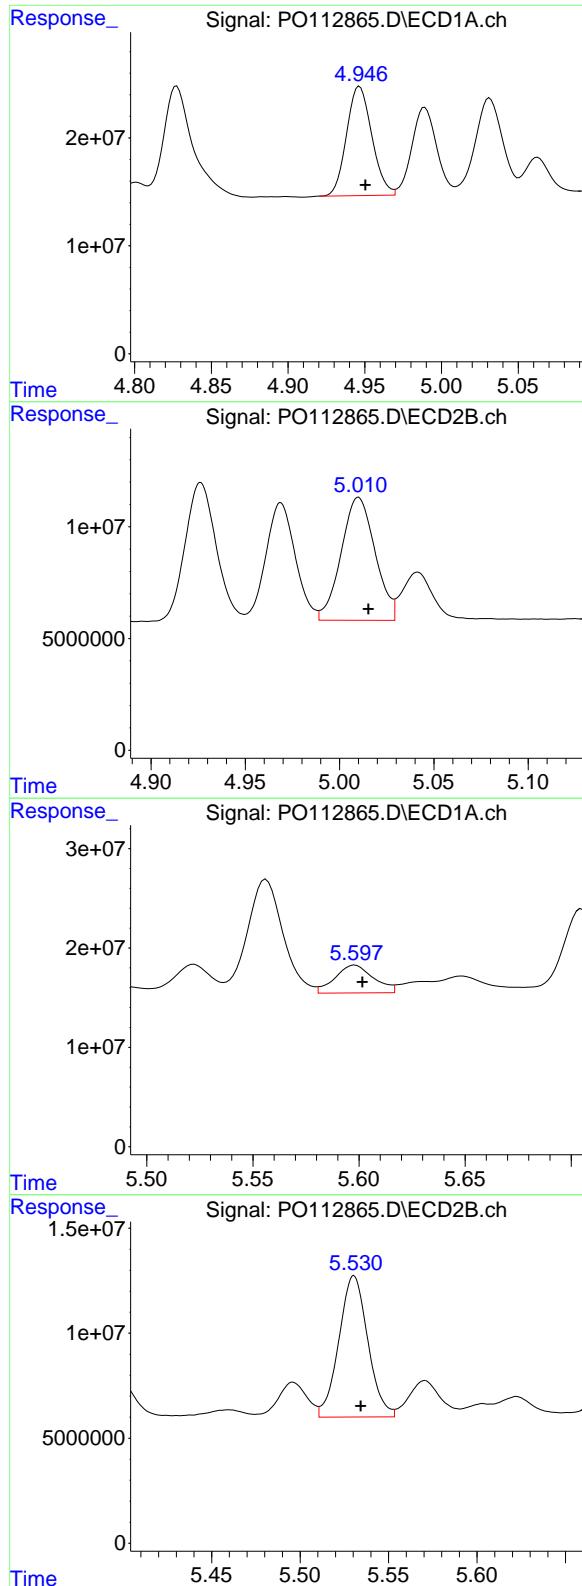

#19 AR-1242-4

R.T.: 4.947 min
 Delta R.T.: -0.004 min
 Response: 116665542
 Conc: 600.51 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#19 AR-1242-4


R.T.: 5.010 min
 Delta R.T.: -0.005 min
 Response: 68905552
 Conc: 561.40 ng/ml

#20 AR-1242-5

R.T.: 5.598 min
 Delta R.T.: -0.003 min
 Response: 35516814
 Conc: 166.03 ng/ml

#20 AR-1242-5

R.T.: 5.530 min
 Delta R.T.: -0.004 min
 Response: 76792861
 Conc: 477.06 ng/ml

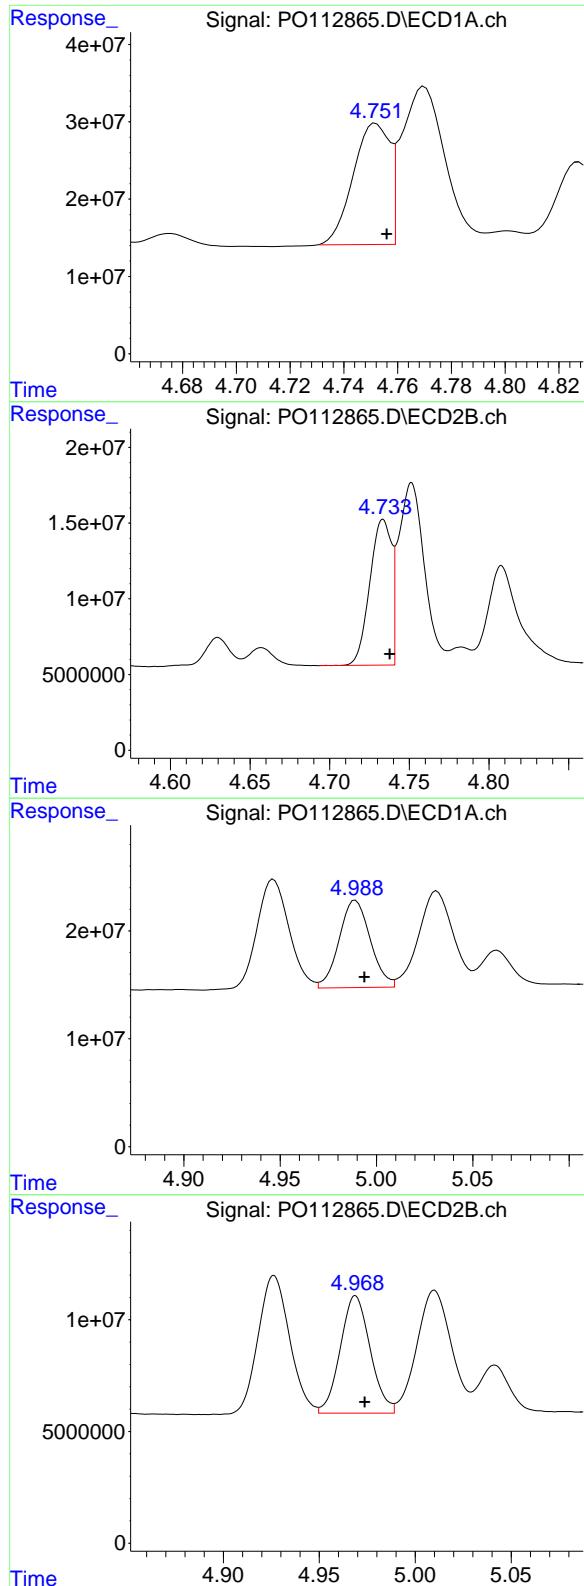

#21 AR-1248-1

R.T.: 4.752 min
 Delta R.T.: -0.004 min
 Response: 147410245
 Conc: 787.41 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#21 AR-1248-1


R.T.: 4.734 min
 Delta R.T.: -0.004 min
 Response: 91367071
 Conc: 751.93 ng/ml

#22 AR-1248-2

R.T.: 4.989 min
 Delta R.T.: -0.005 min
 Response: 90857298
 Conc: 356.15 ng/ml

#22 AR-1248-2

R.T.: 4.969 min
 Delta R.T.: -0.005 min
 Response: 57301939
 Conc: 338.50 ng/ml

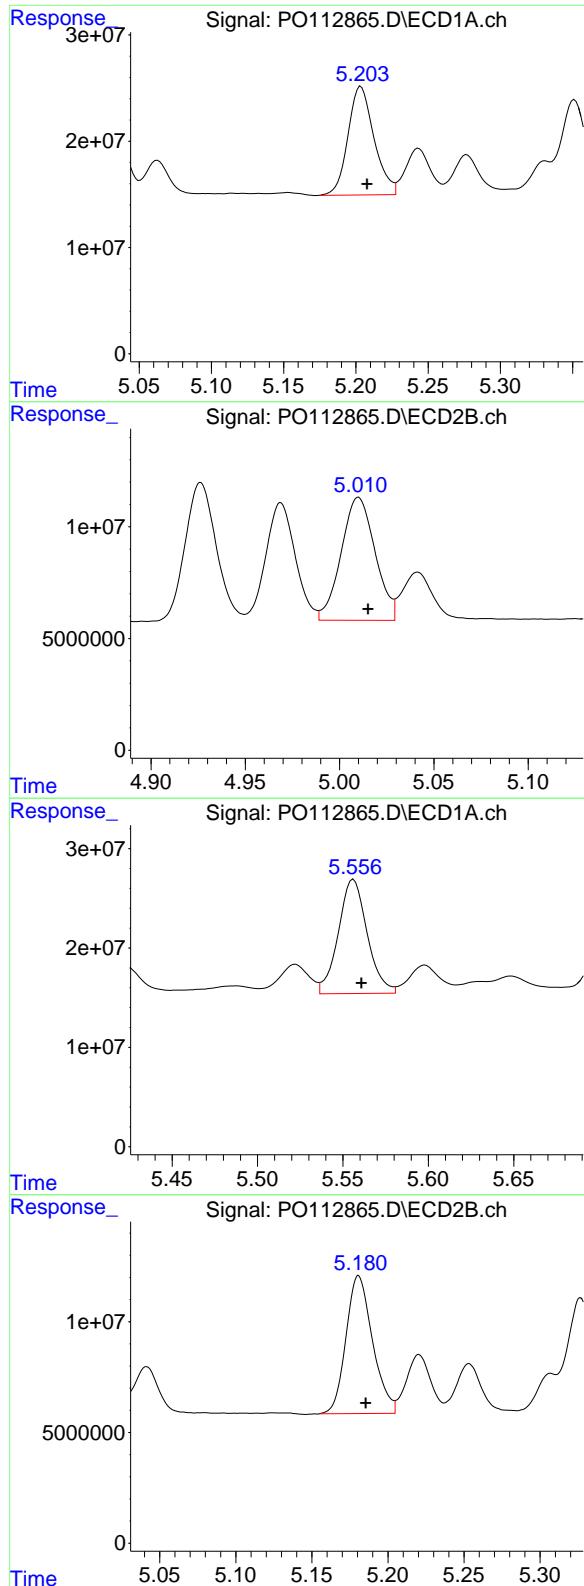

#23 AR-1248-3

R.T.: 5.203 min
 Delta R.T.: -0.004 min
 Response: 128204484
 Conc: 373.01 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#23 AR-1248-3


R.T.: 5.010 min
 Delta R.T.: -0.005 min
 Response: 68905552
 Conc: 387.88 ng/ml

#24 AR-1248-4

R.T.: 5.556 min
 Delta R.T.: -0.005 min
 Response: 135461406
 Conc: 266.62 ng/ml

#24 AR-1248-4

R.T.: 5.181 min
 Delta R.T.: -0.005 min
 Response: 75537038
 Conc: 362.54 ng/ml

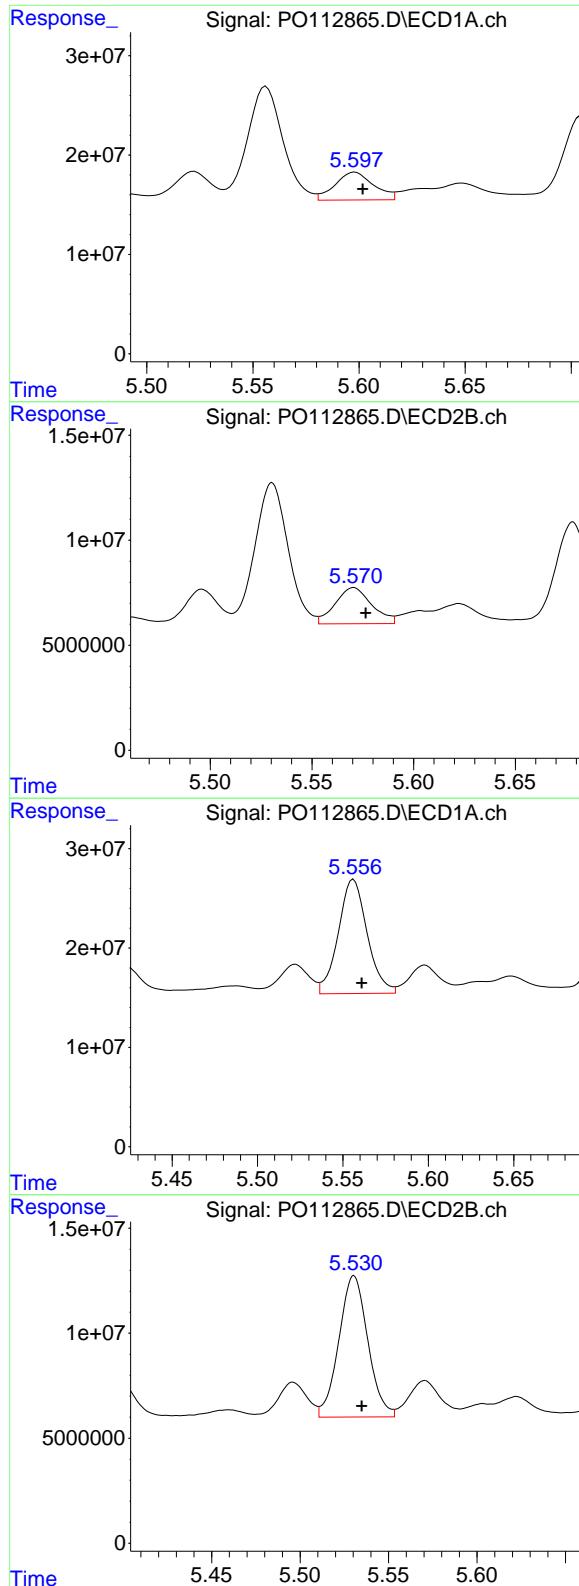

#25 AR-1248-5

R.T.: 5.598 min
 Delta R.T.: -0.004 min
 Response: 35516814
 Conc: 101.60 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#25 AR-1248-5


R.T.: 5.571 min
 Delta R.T.: -0.006 min
 Response: 21481781
 Conc: 100.02 ng/ml

#26 AR-1254-1

R.T.: 5.556 min
 Delta R.T.: -0.005 min
 Response: 135461406
 Conc: 246.76 ng/ml

#26 AR-1254-1


R.T.: 5.530 min
 Delta R.T.: -0.004 min
 Response: 76792861
 Conc: 233.68 ng/ml



#27 AR-1254-2


R.T.: 5.705 min
 Delta R.T.: -0.005 min
 Response: 102027337
 Conc: 209.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

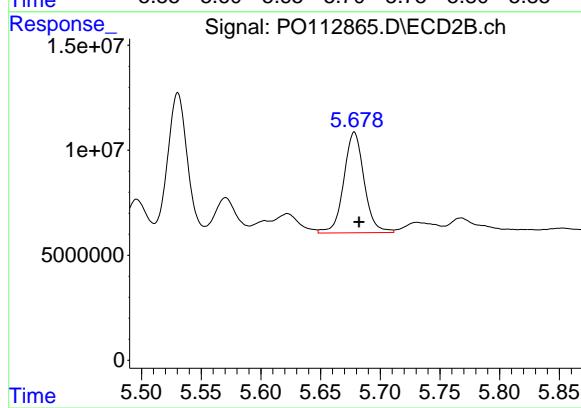


#27 AR-1254-2

R.T.: 5.678 min
 Delta R.T.: -0.004 min
 Response: 56804415
 Conc: 196.22 ng/ml

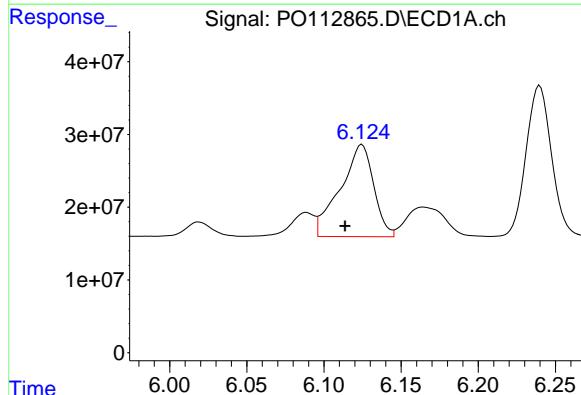


#28 AR-1254-3

R.T.: 6.125 min
 Delta R.T.: 0.011 min
 Response: 191292429
 Conc: 257.01 ng/ml

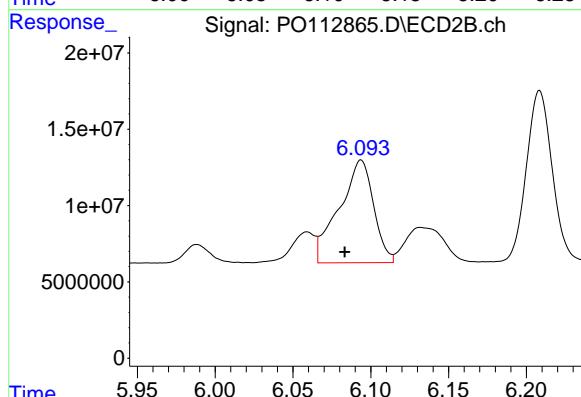

#28 AR-1254-3

R.T.: 6.094 min
 Delta R.T.: 0.010 min
 Response: 103516711
 Conc: 242.17 ng/ml

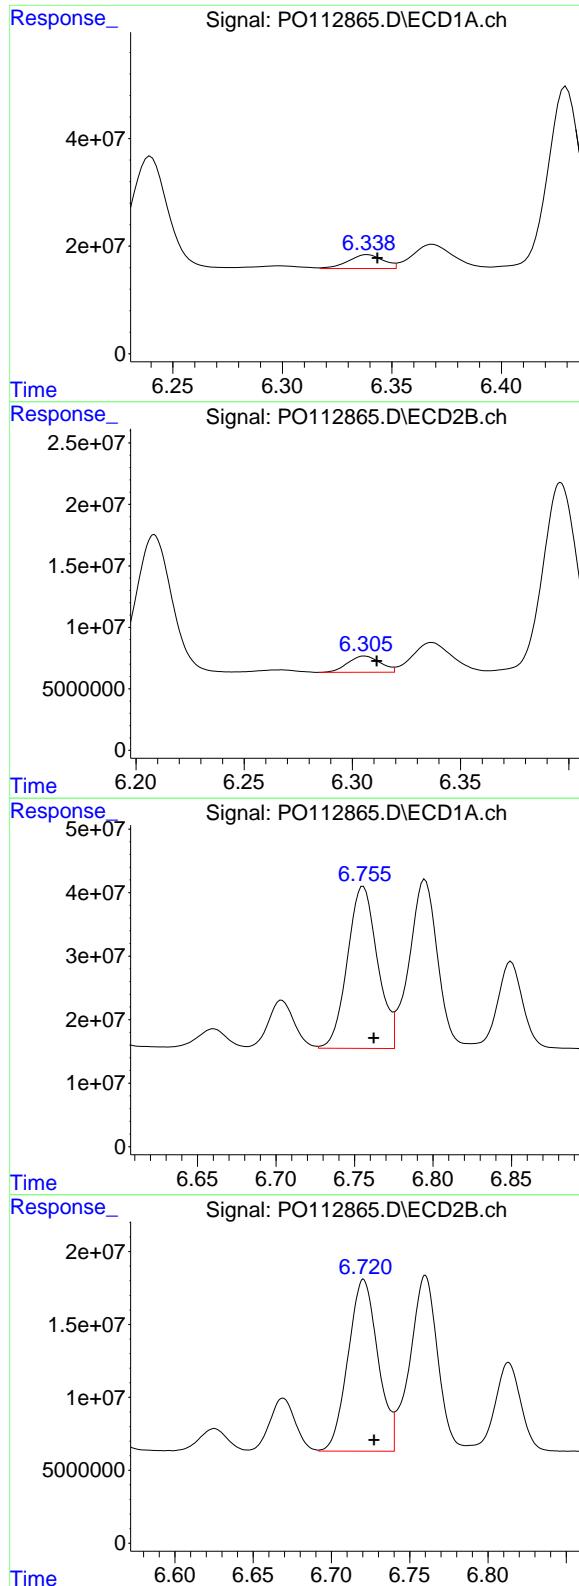

#29 AR-1254-4

R.T.: 6.339 min
 Delta R.T.: -0.004 min
 Response: 28484111
 Conc: 51.82 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#29 AR-1254-4


R.T.: 6.306 min
 Delta R.T.: -0.006 min
 Response: 13812616
 Conc: 50.60 ng/ml

#30 AR-1254-5

R.T.: 6.756 min
 Delta R.T.: -0.007 min
 Response: 340057594
 Conc: 480.43 ng/ml

#30 AR-1254-5

R.T.: 6.721 min
 Delta R.T.: -0.007 min
 Response: 156698403
 Conc: 469.13 ng/ml

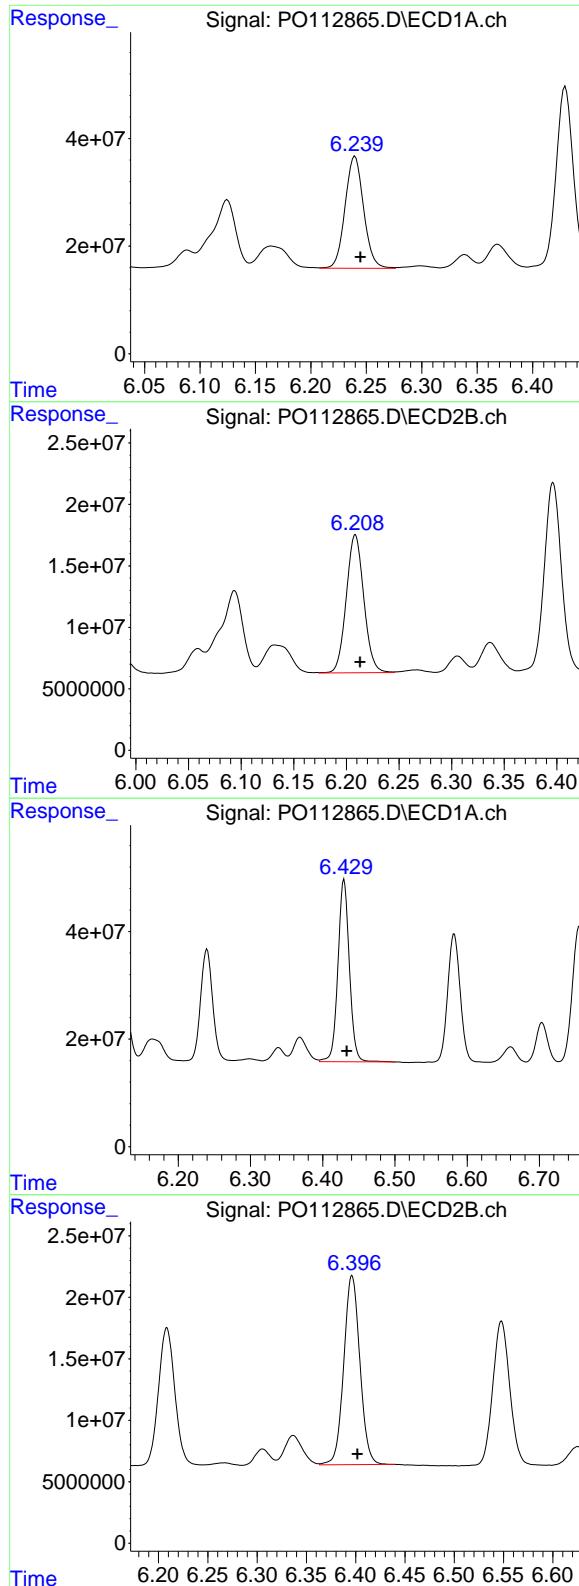

#31 AR-1260-1

R.T.: 6.240 min
 Delta R.T.: -0.005 min
 Response: 241783854
 Conc: 550.35 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#31 AR-1260-1


R.T.: 6.208 min
 Delta R.T.: -0.005 min
 Response: 130209411
 Conc: 523.96 ng/ml

#32 AR-1260-2

R.T.: 6.430 min
 Delta R.T.: -0.004 min
 Response: 373809275
 Conc: 543.41 ng/ml

#32 AR-1260-2

R.T.: 6.396 min
 Delta R.T.: -0.006 min
 Response: 175240912
 Conc: 531.85 ng/ml

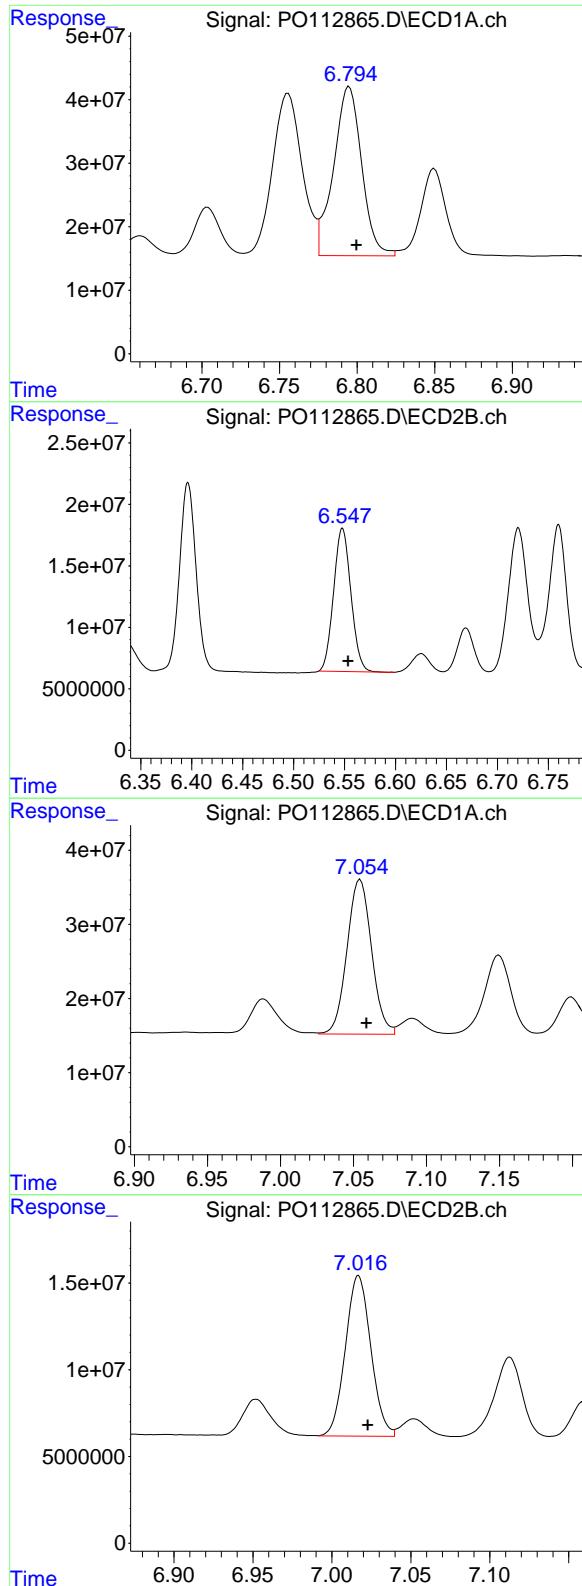

#33 AR-1260-3

R.T.: 6.795 min
 Delta R.T.: -0.005 min
 Response: 335729402
 Conc: 570.95 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#33 AR-1260-3


R.T.: 6.548 min
 Delta R.T.: -0.005 min
 Response: 137861384
 Conc: 536.59 ng/ml

#34 AR-1260-4

R.T.: 7.055 min
 Delta R.T.: -0.004 min
 Response: 244563892
 Conc: 542.26 ng/ml

#34 AR-1260-4

R.T.: 7.017 min
 Delta R.T.: -0.006 min
 Response: 104031834
 Conc: 543.78 ng/ml

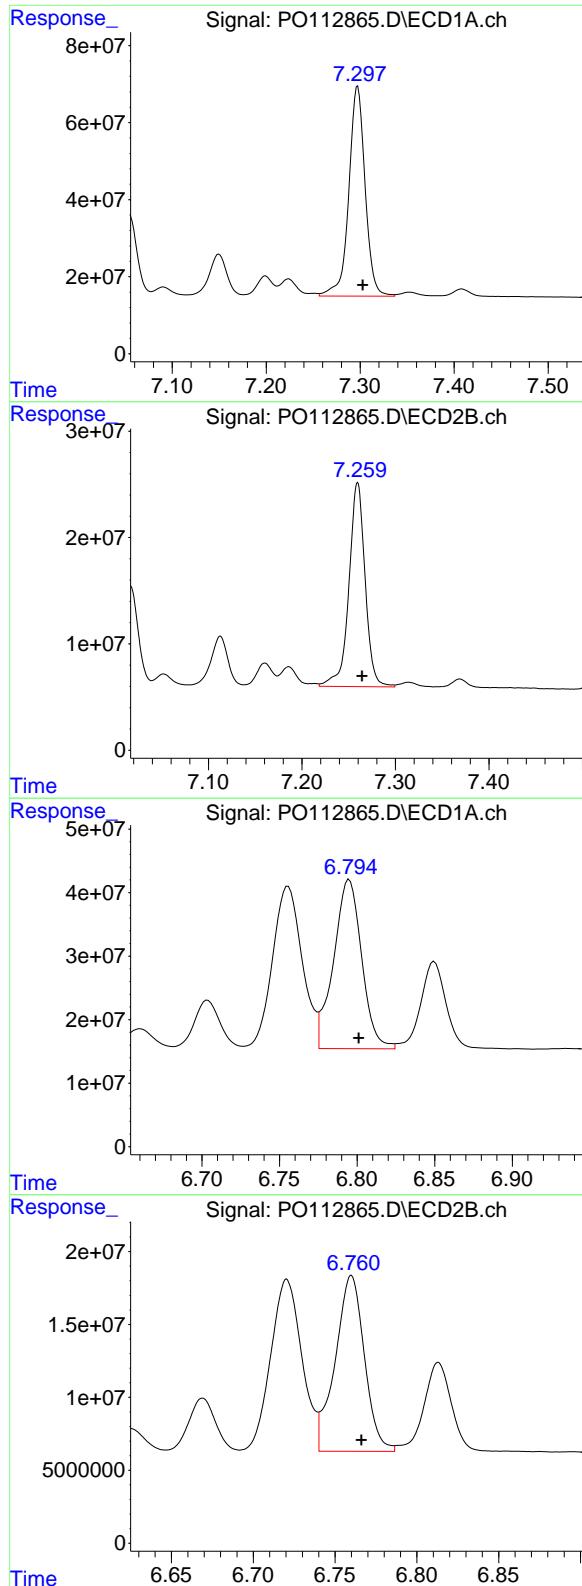

#35 AR-1260-5

R.T.: 7.297 min
 Delta R.T.: -0.005 min
 Response: 656708588
 Conc: 529.97 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

#35 AR-1260-5


R.T.: 7.260 min
 Delta R.T.: -0.005 min
 Response: 231166363
 Conc: 560.82 ng/ml

#36 AR-1262-1

R.T.: 6.795 min
 Delta R.T.: -0.006 min
 Response: 335729402
 Conc: 361.31 ng/ml

#36 AR-1262-1


R.T.: 6.760 min
 Delta R.T.: -0.006 min
 Response: 149644381
 Conc: 360.74 ng/ml

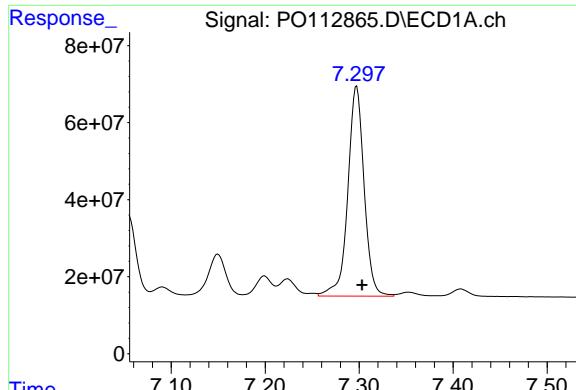

#37 AR-1262-2


R.T.: 7.297 min
 Delta R.T.: -0.006 min
 Response: 656708588
 Conc: 441.63 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

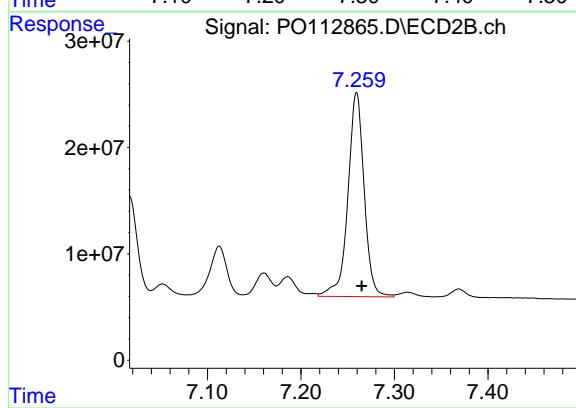


#37 AR-1262-2

R.T.: 7.260 min
 Delta R.T.: -0.005 min
 Response: 231166363
 Conc: 448.39 ng/ml

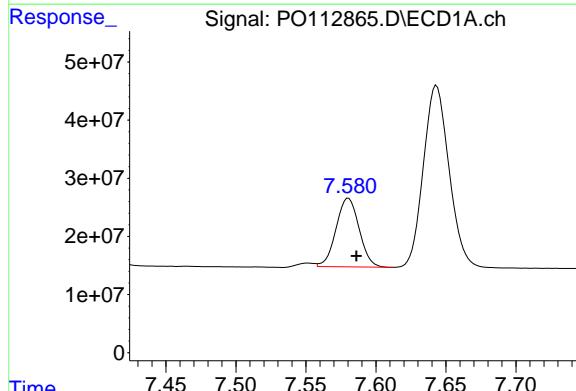


#38 AR-1262-3

R.T.: 7.580 min
 Delta R.T.: -0.006 min
 Response: 135564393
 Conc: 229.67 ng/ml

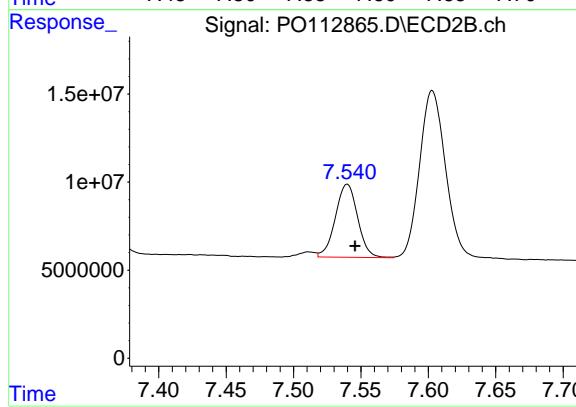

#38 AR-1262-3


R.T.: 7.540 min
 Delta R.T.: -0.006 min
 Response: 47945338
 Conc: 257.04 ng/ml

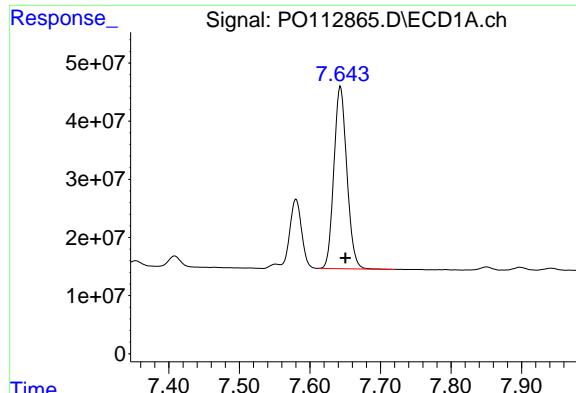

#39 AR-1262-4


R.T.: 7.643 min
 Delta R.T.: -0.007 min
 Response: 400906213
 Conc: 403.26 ng/ml

Instrument: ECD_O
 ClientSampleId: AR1660CCC500

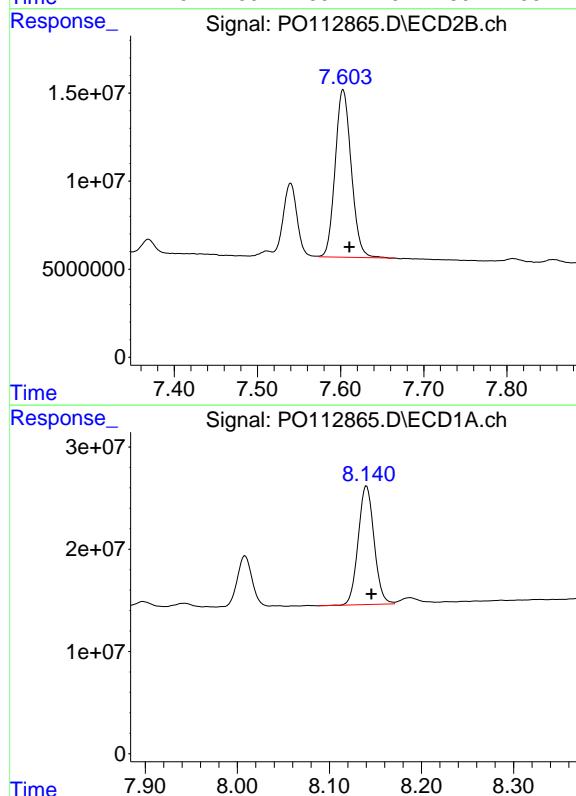


#40 AR-1262-5

R.T.: 8.140 min
 Delta R.T.: -0.005 min
 Response: 139177733
 Conc: 320.64 ng/ml

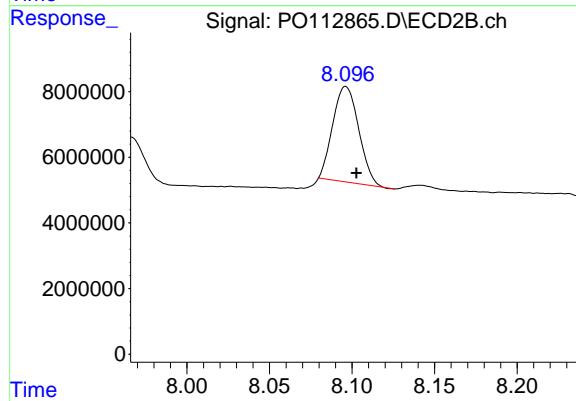

#40 AR-1262-5

R.T.: 8.096 min
 Delta R.T.: -0.007 min
 Response: 31782749
 Conc: 319.41 ng/ml

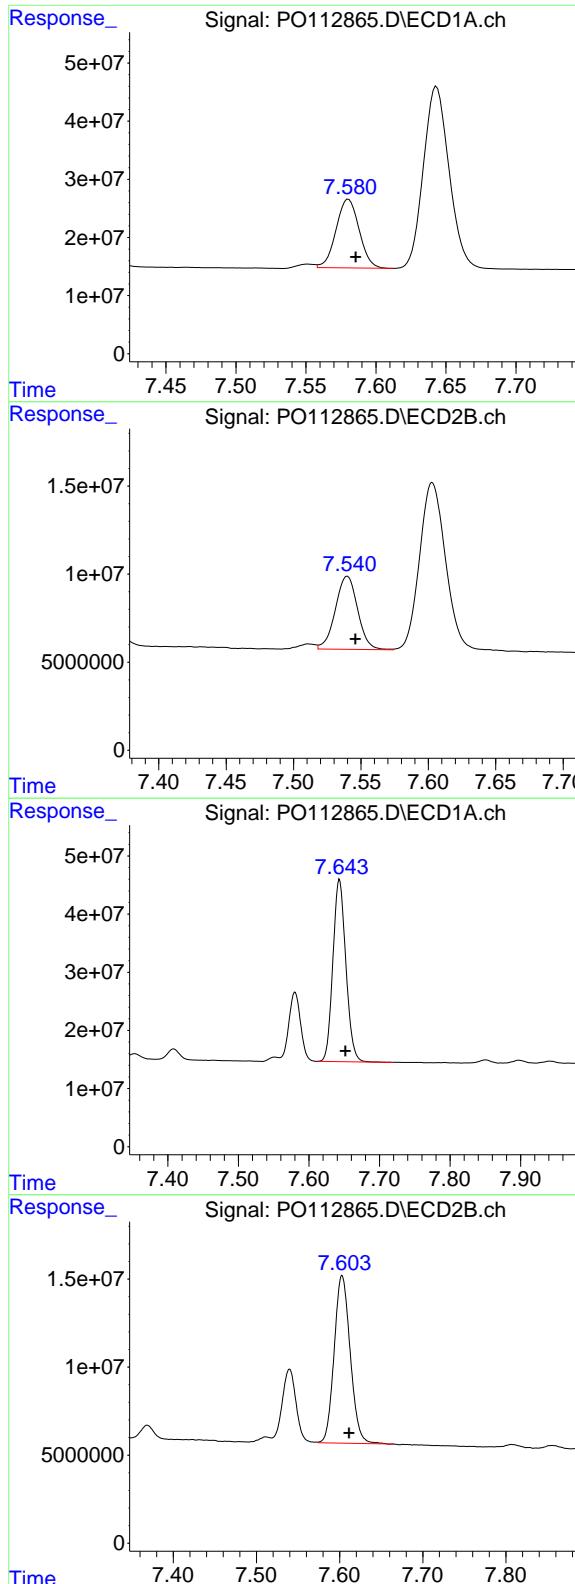

#41 AR-1268-1

R.T.: 7.580 min
 Delta R.T.: -0.005 min
 Response: 135564393
 Conc: 77.41 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#41 AR-1268-1


R.T.: 7.540 min
 Delta R.T.: -0.006 min
 Response: 47945338
 Conc: 92.58 ng/ml

#42 AR-1268-2

R.T.: 7.643 min
 Delta R.T.: -0.008 min
 Response: 400906213
 Conc: 272.17 ng/ml

#42 AR-1268-2


R.T.: 7.603 min
 Delta R.T.: -0.008 min
 Response: 127736391
 Conc: 300.51 ng/ml



#43 AR-1268-3


R.T.: 7.851 min
Delta R.T.: -0.006 min
Response: 5704040
Conc: 4.56 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

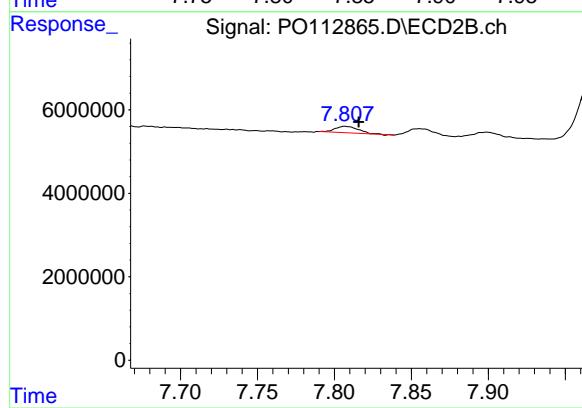


#43 AR-1268-3

R.T.: 7.807 min
Delta R.T.: -0.009 min
Response: 1601864
Conc: 4.99 ng/ml

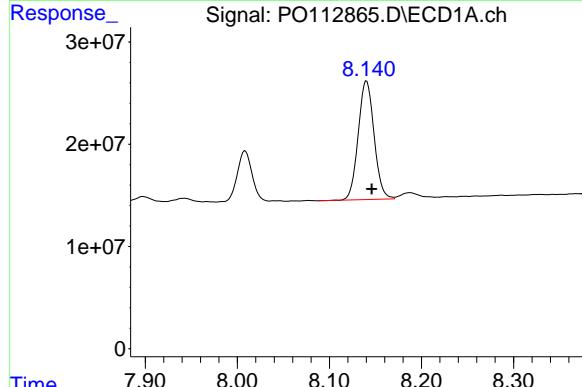


#44 AR-1268-4

R.T.: 8.140 min
Delta R.T.: -0.005 min
Response: 139177733
Conc: 288.83 ng/ml

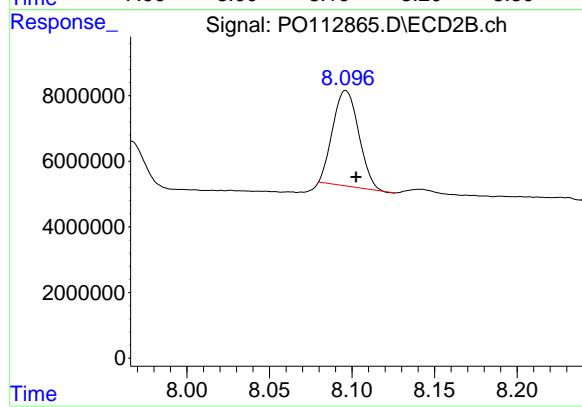

#44 AR-1268-4

R.T.: 8.096 min
Delta R.T.: -0.006 min
Response: 31782749
Conc: 285.57 ng/ml

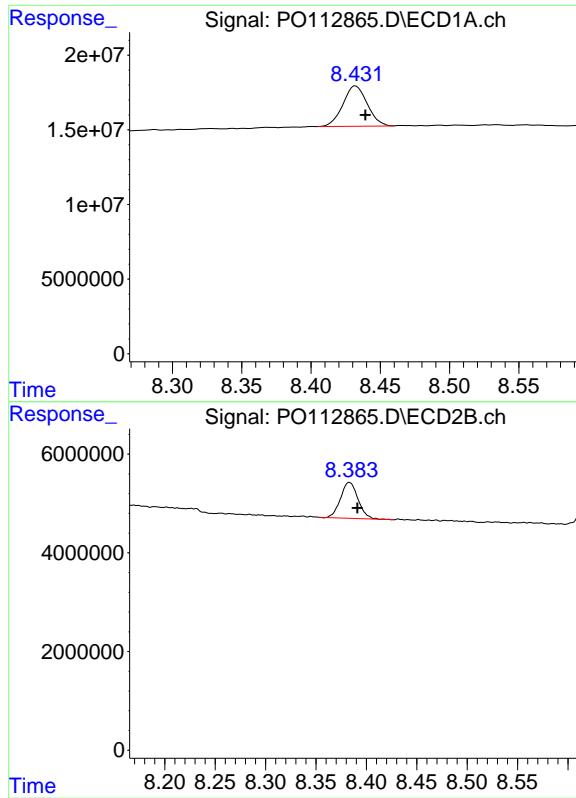

#45 AR-1268-5

R.T.: 8.432 min
Delta R.T.: -0.007 min
Response: 33094872
Conc: 9.86 ng/ml

Instrument: ECD_O
ClientSampleId: AR1660CCC500

#45 AR-1268-5

R.T.: 8.383 min
Delta R.T.: -0.008 min
Response: 8792996
Conc: 12.02 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:54
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:10:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.807 | 28863110 | 91466480 | 27.077 | 22.767 |
| 2) SA Decachlor... | 10.435 | 8.827 | 25421801 | 149.8E6 | 27.450 | 24.664 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|---------|
| 3) L1 AR-1016-1 | 5.810 | 4.907 | 10964759 | 100.9E6 | 281.744 | 251.671 |
| 4) L1 AR-1016-2 | 5.832 | 4.965 | 16172490 | 49571013 | 281.221 | 259.123 |
| 5) L1 AR-1016-3 | 5.895 | 5.085 | 10675549 | 28731399 | 285.290 | 266.268 |
| 6) L1 AR-1016-4 | 5.991 | 5.126 | 8965609 | 27406022 | 287.521 | 254.800 |
| 7) L1 AR-1016-5 | 6.284 | 5.340 | 9320877 | 29720771 | 300.822 | 252.036 |
| 31) L7 AR-1260-1 | 7.401 | 6.557 | 16203062 | 109.5E6 | 304.635 | 267.207 |
| 32) L7 AR-1260-2 | 7.653 | 6.711 | 18253217 | 76433717 | 290.773 | 249.893 |
| 33) L7 AR-1260-3 | 8.011 | 6.922 | 14251387 | 95830018 | 283.827 | 237.590 |
| 34) L7 AR-1260-4 | 8.240 | 7.182 | 16666094 | 70195428 | 280.066 | 237.501 |
| 35) L7 AR-1260-5 | 8.565 | 7.421 | 29333116 | 183.1E6 | 275.424 | 232.969 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074171.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 12:54
 Operator : YP\AJ
 Sample : AR1660ICC250
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:10:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:02:12 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

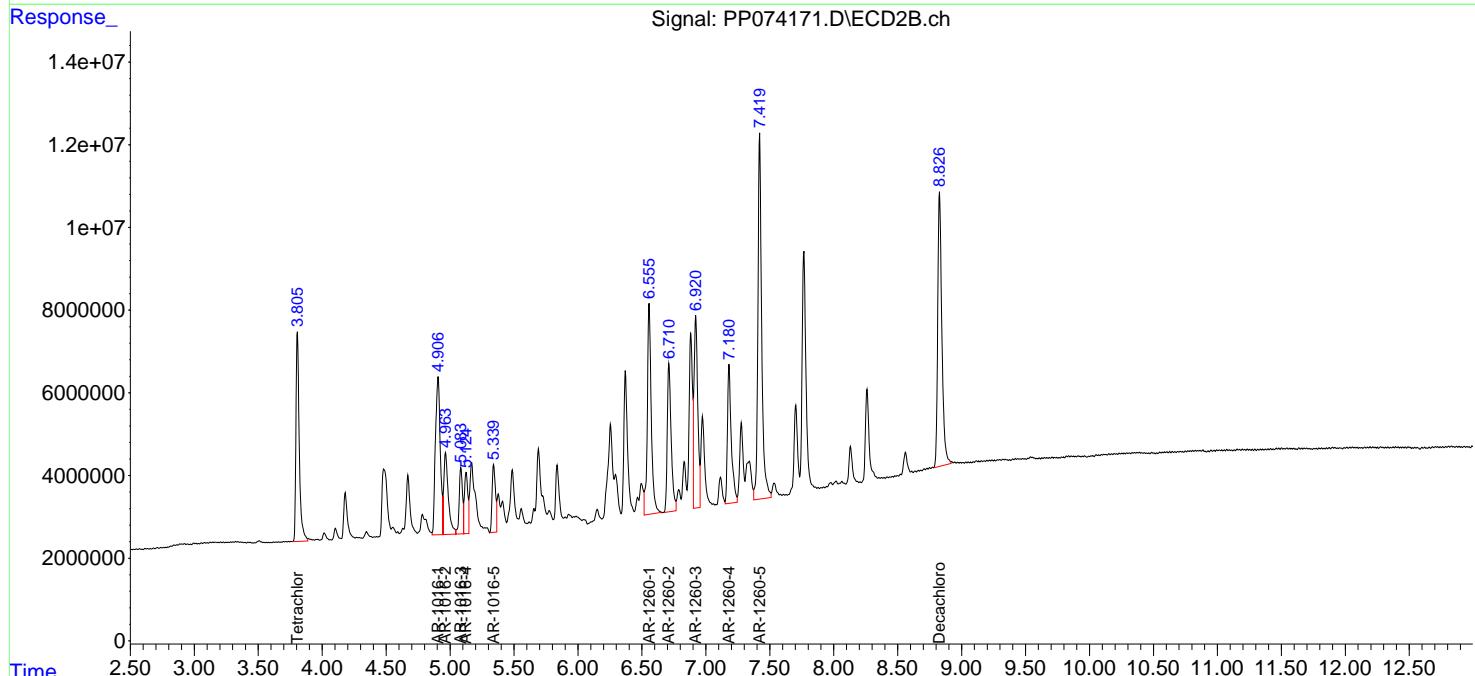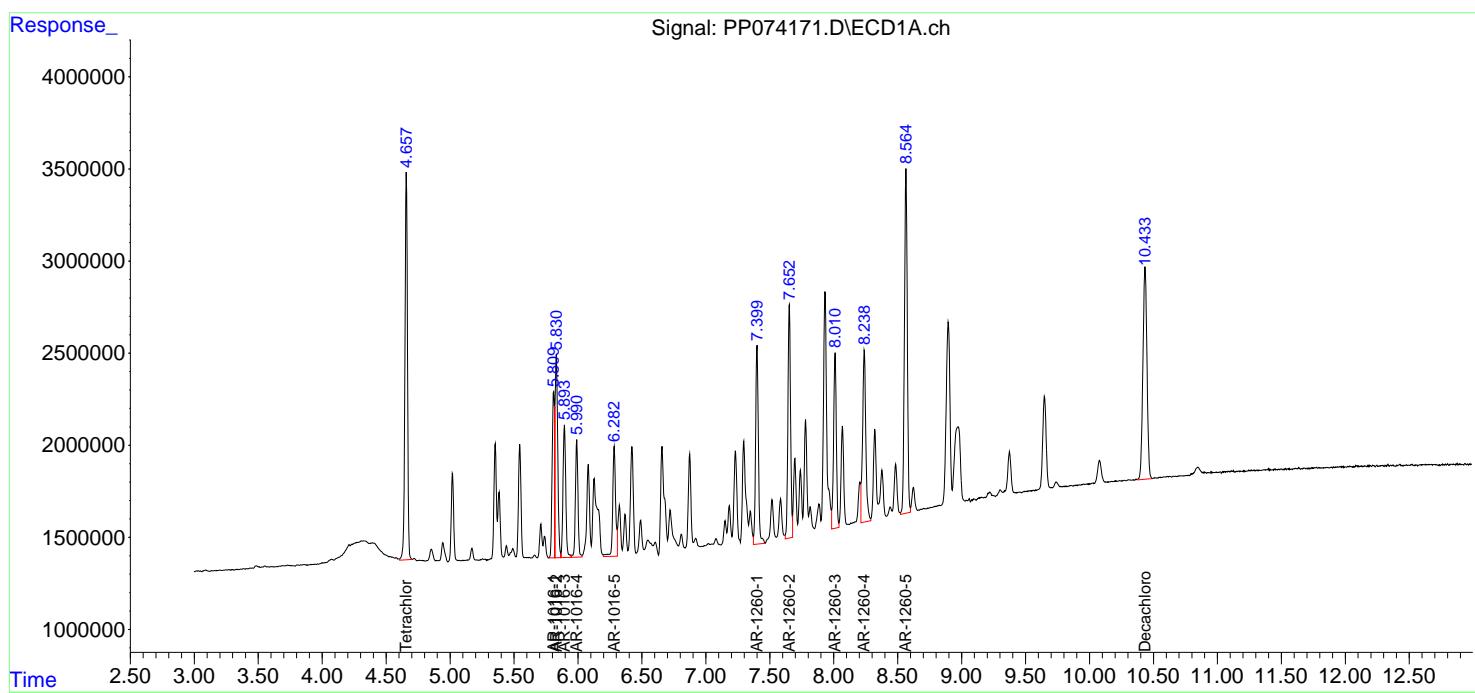

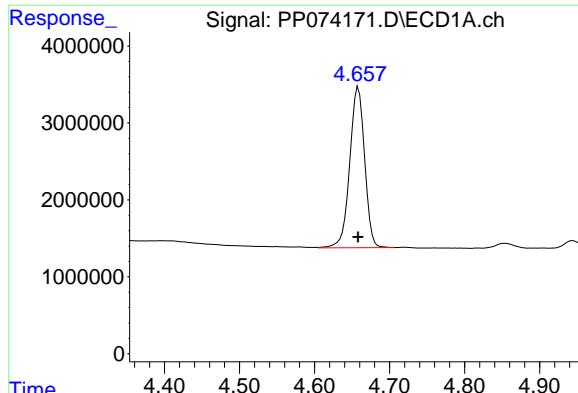

#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: 0.000 min
Response: 28863110
Conc: 27.08 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1660ICC250

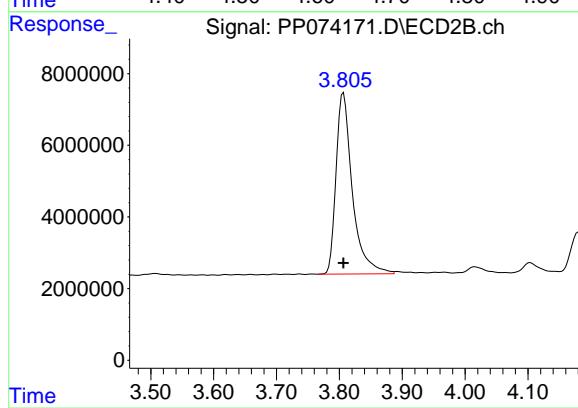


#1 Tetrachloro-m-xylene

R.T.: 3.807 min
Delta R.T.: 0.000 min
Response: 91466480
Conc: 22.77 ng/ml

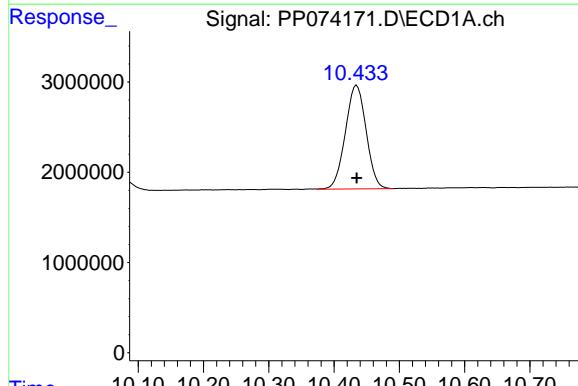


#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.000 min
Response: 25421801
Conc: 27.45 ng/ml

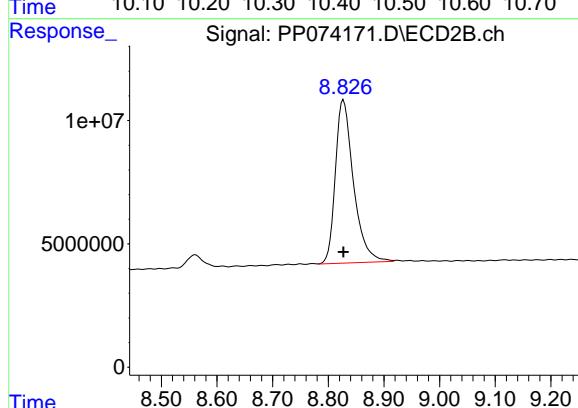

#2 Decachlorobiphenyl

R.T.: 8.827 min
Delta R.T.: 0.000 min
Response: 149786727
Conc: 24.66 ng/ml

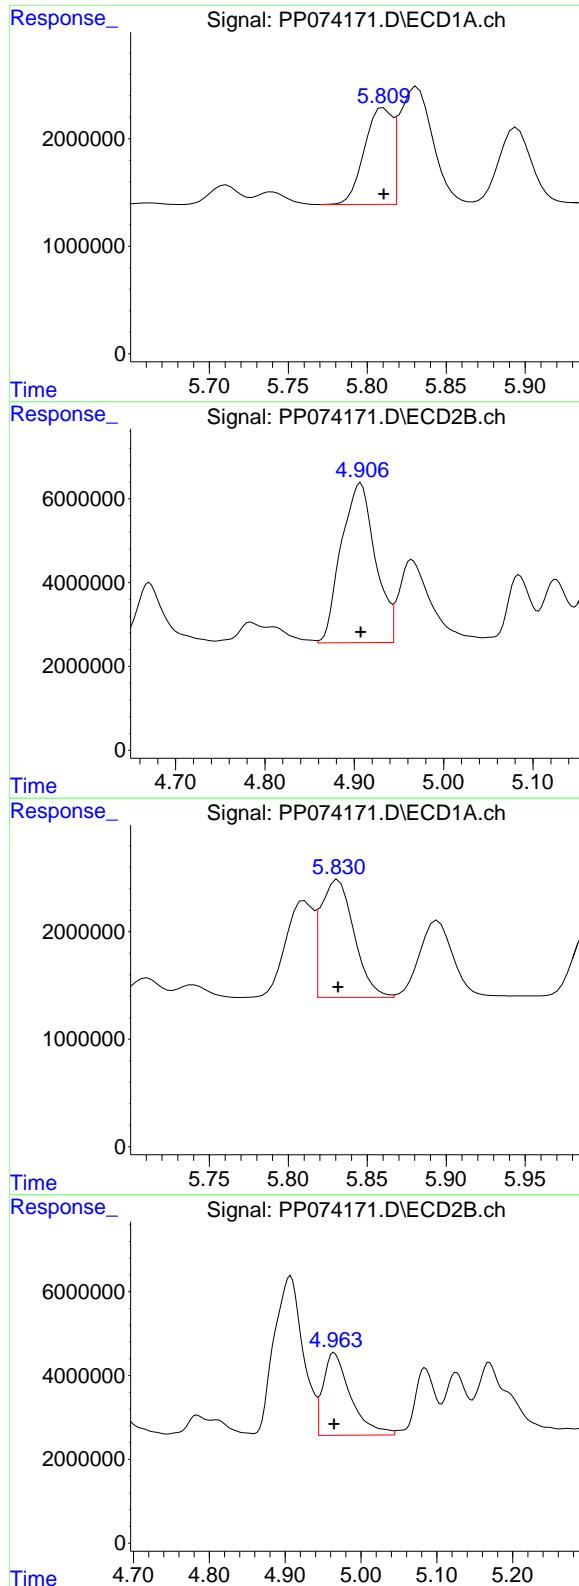

#3 AR-1016-1

R.T.: 5.810 min
Delta R.T.: 0.000 min **Instrument:**
Response: 10964759 ECD_P
Conc: 281.74 ng/ml **ClientSampleId:**
AR1660ICC250

#3 AR-1016-1


R.T.: 4.907 min
Delta R.T.: 0.000 min
Response: 100933839
Conc: 251.67 ng/ml

#4 AR-1016-2

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 16172490
Conc: 281.22 ng/ml


#4 AR-1016-2

R.T.: 4.965 min
Delta R.T.: 0.000 min
Response: 49571013
Conc: 259.12 ng/ml

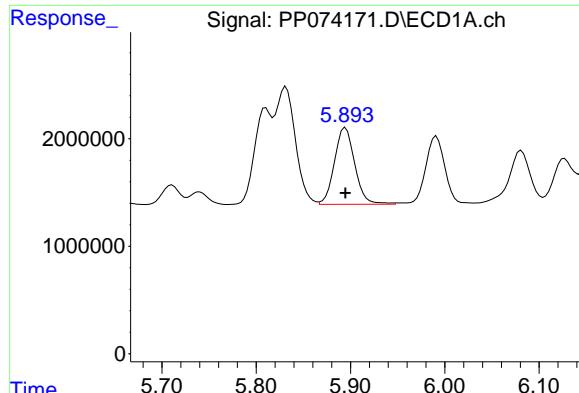


#5 AR-1016-3
R.T.: 5.895 min
Delta R.T.: 0.000 min
Response: 10675549
Conc: 285.29 ng/ml


Instrument: ECD_P
ClientSampleId: AR1660ICC250

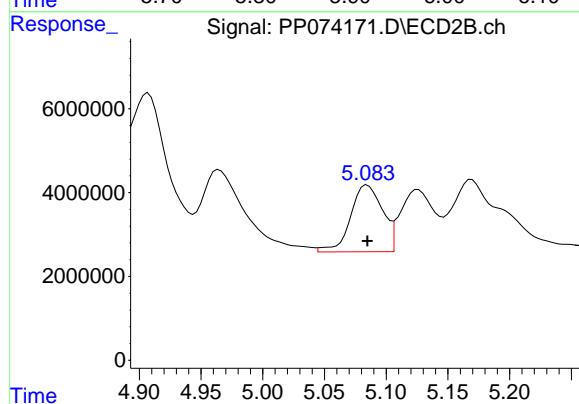


#5 AR-1016-3
R.T.: 5.085 min
Delta R.T.: 0.000 min
Response: 28731399
Conc: 266.27 ng/ml

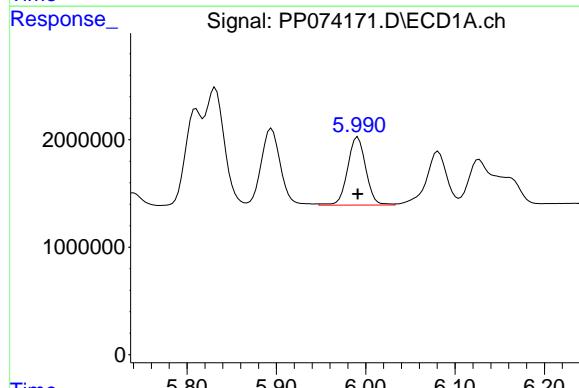

#6 AR-1016-4
R.T.: 5.991 min
Delta R.T.: 0.000 min
Response: 8965609
Conc: 287.52 ng/ml

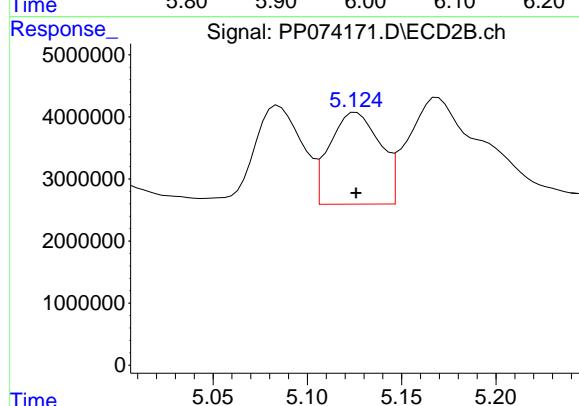

#6 AR-1016-4
R.T.: 5.126 min
Delta R.T.: 0.000 min
Response: 27406022
Conc: 254.80 ng/ml

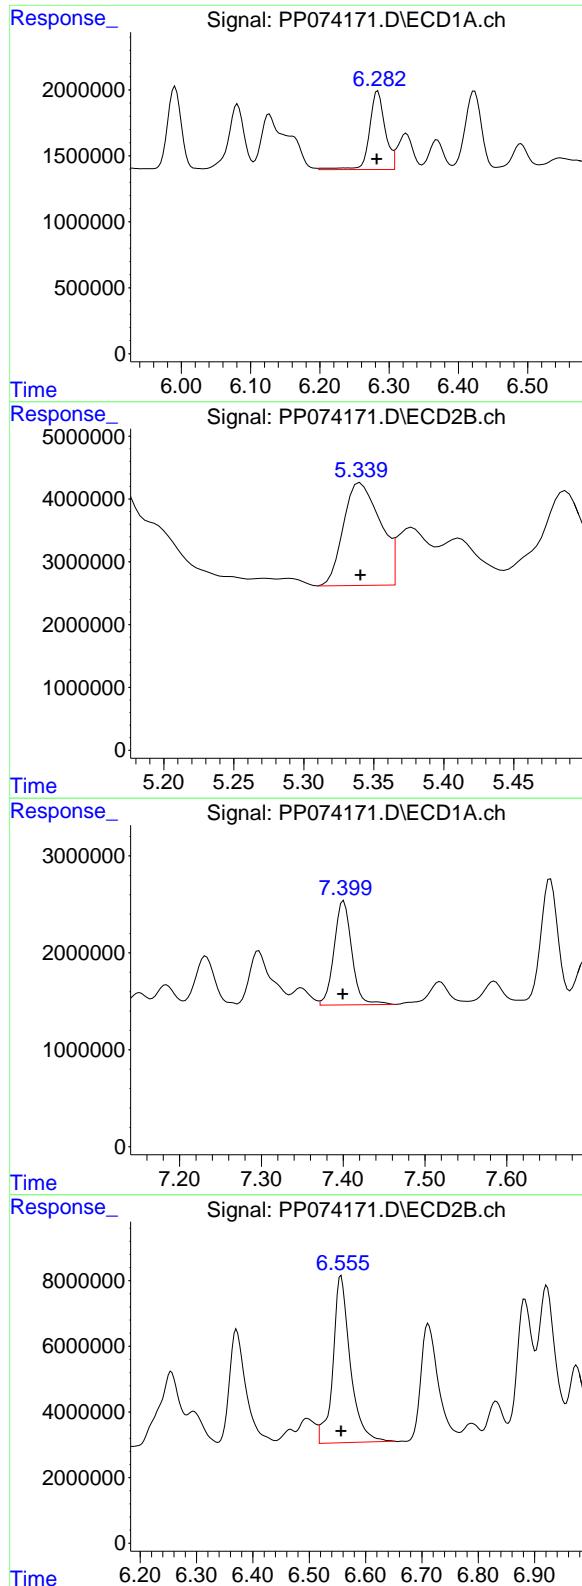

#7 AR-1016-5

R.T.: 6.284 min
 Delta R.T.: 0.001 min
 Response: 9320877
 Conc: 300.82 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC250

#7 AR-1016-5


R.T.: 5.340 min
 Delta R.T.: 0.000 min
 Response: 29720771
 Conc: 252.04 ng/ml

#31 AR-1260-1

R.T.: 7.401 min
 Delta R.T.: 0.001 min
 Response: 16203062
 Conc: 304.63 ng/ml

#31 AR-1260-1

R.T.: 6.557 min
 Delta R.T.: 0.000 min
 Response: 109526607
 Conc: 267.21 ng/ml

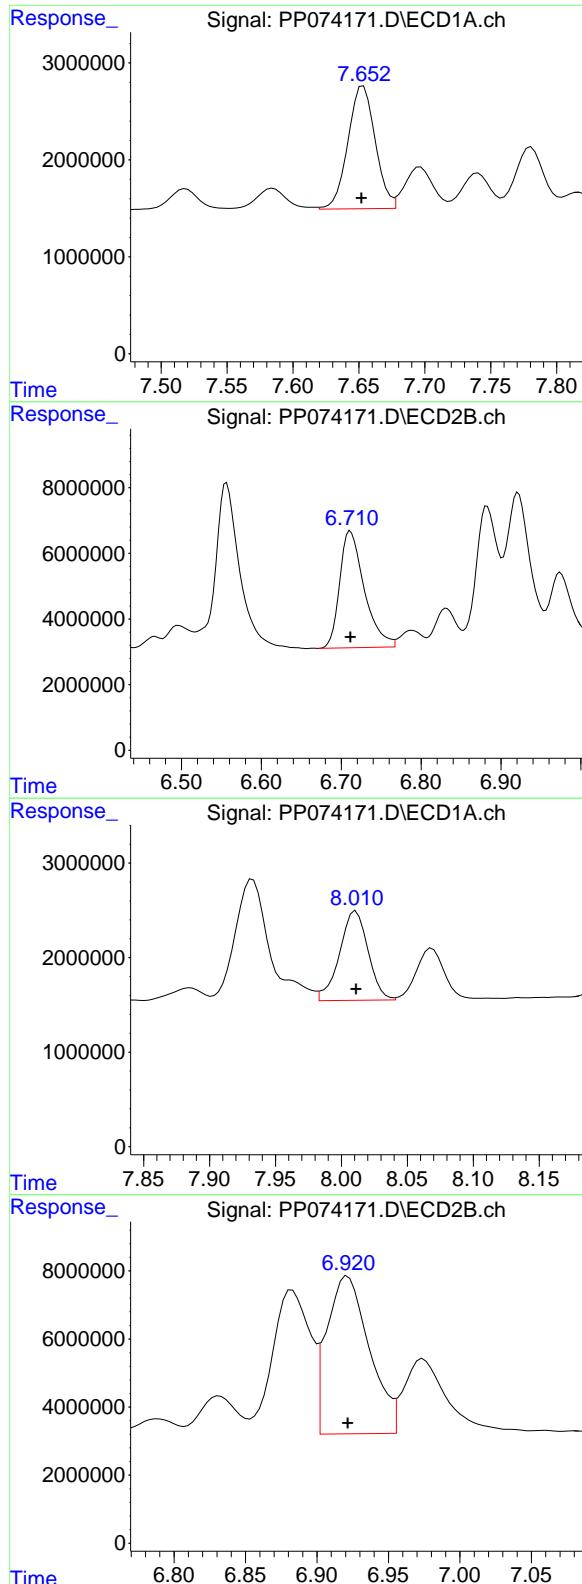

#32 AR-1260-2

R.T.: 7.653 min
 Delta R.T.: 0.001 min
 Response: 18253217
 Conc: 290.77 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC250

#32 AR-1260-2


R.T.: 6.711 min
 Delta R.T.: 0.000 min
 Response: 76433717
 Conc: 249.89 ng/ml

#33 AR-1260-3

R.T.: 8.011 min
 Delta R.T.: 0.000 min
 Response: 14251387
 Conc: 283.83 ng/ml

#33 AR-1260-3

R.T.: 6.922 min
 Delta R.T.: 0.000 min
 Response: 95830018
 Conc: 237.59 ng/ml

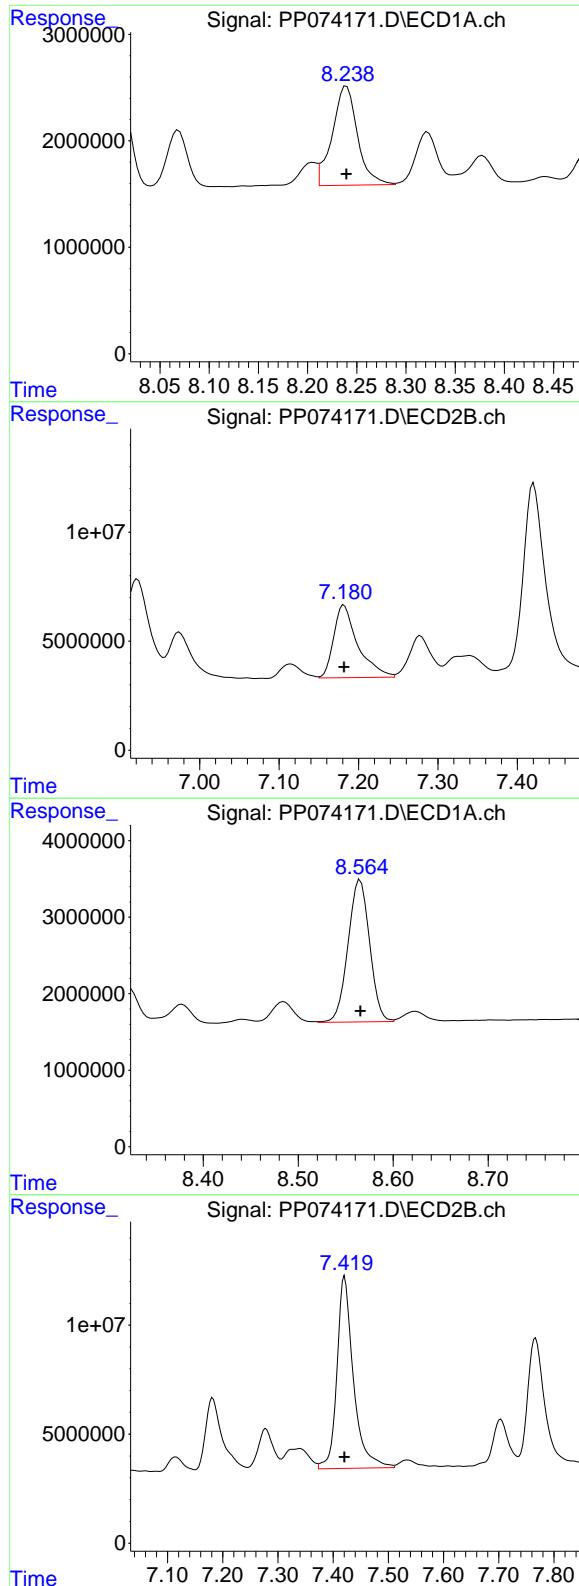

#34 AR-1260-4

R.T.: 8.240 min
 Delta R.T.: 0.000 min
 Response: 16666094
 Conc: 280.07 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC250

#34 AR-1260-4

R.T.: 7.182 min
 Delta R.T.: 0.000 min
 Response: 70195428
 Conc: 237.50 ng/ml

#35 AR-1260-5

R.T.: 8.565 min
 Delta R.T.: 0.000 min
 Response: 29333116
 Conc: 275.42 ng/ml

#35 AR-1260-5

R.T.: 7.421 min
 Delta R.T.: 0.000 min
 Response: 183122844
 Conc: 232.97 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 13:10
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:23:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:23:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|---------|----------|-------|---------|
| 1) SA Tetrachlor... | 4.659 | 3.802 | 5276522 | 10952936 | 4.987 | 2.999 # |
| 2) SA Decachlor... | 10.437 | 8.824 | 4796081 | 22193655 | 5.142 | 3.862 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|--------|----------|
| 3) L1 AR-1016-1 | 5.811 | 4.904 | 1988336 | 14775918 | 50.869 | 38.889 |
| 4) L1 AR-1016-2 | 5.833 | 4.962 | 2791158 | 7843665 | 48.821 | 42.532 |
| 5) L1 AR-1016-3 | 5.896 | 5.082 | 1878829 | 4619486 | 50.167 | 44.079 |
| 6) L1 AR-1016-4 | 5.992 | 5.122 | 1465464 | 4449408 | 47.568 | 42.847 |
| 7) L1 AR-1016-5 | 6.285 | 5.337 | 1456706 | 4779894 | 47.504 | 42.129 |
| 31) L7 AR-1260-1 | 7.402 | 6.554 | 2907384 | 16702003 | 53.839 | 42.313 |
| 32) L7 AR-1260-2 | 7.655 | 6.708 | 3290166 | 11775837 | 51.766 | 40.356 |
| 33) L7 AR-1260-3 | 8.012 | 6.918 | 2515483 | 13666247 | 50.078 | 36.217 # |
| 34) L7 AR-1260-4 | 8.241 | 7.178 | 2924100 | 9844627 | 49.308 | 35.692 # |
| 35) L7 AR-1260-5 | 8.566 | 7.417 | 5505858 | 24685436 | 51.349 | 33.928 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074172.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 13:10
 Operator : YP\AJ
 Sample : AR1660ICC050
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 13:23:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 13:23:09 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

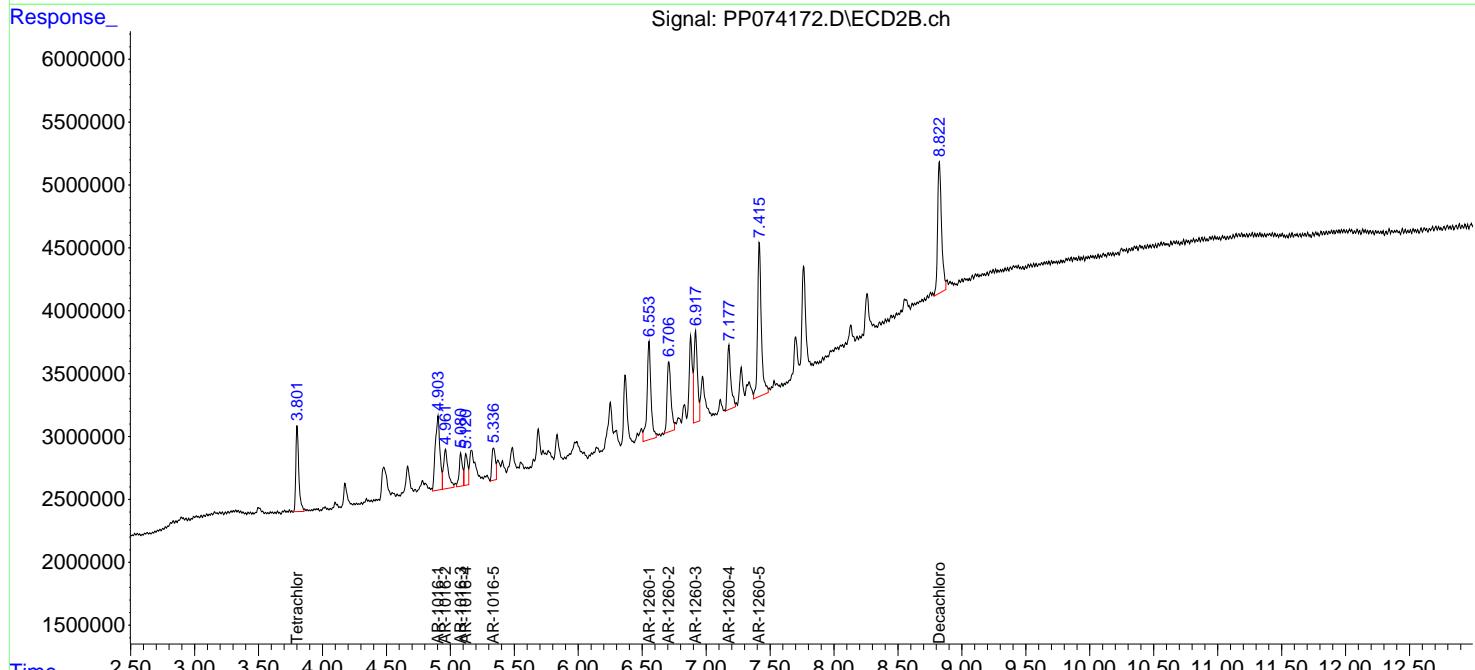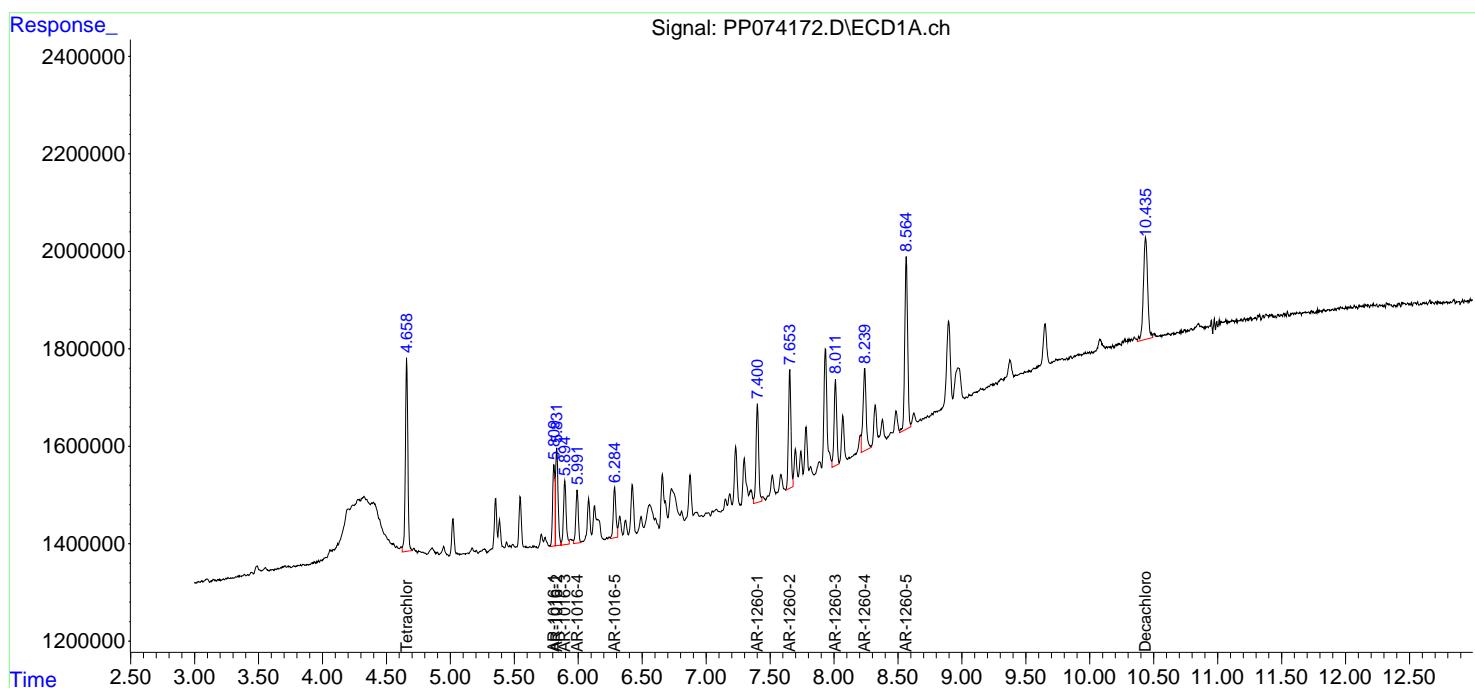

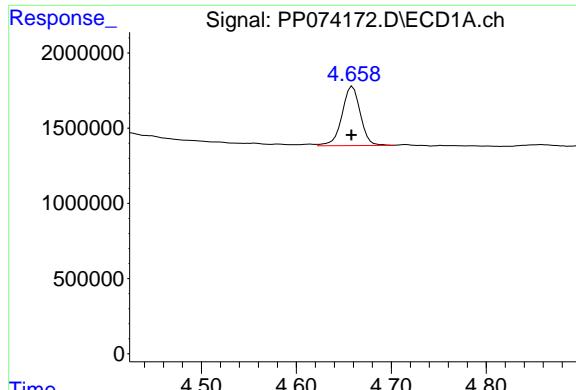

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.001 min
Response: 5276522
Conc: 4.99 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1660ICC050

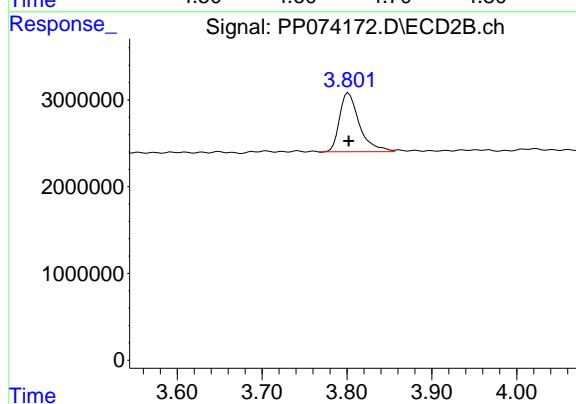


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: 0.000 min
Response: 10952936
Conc: 3.00 ng/ml

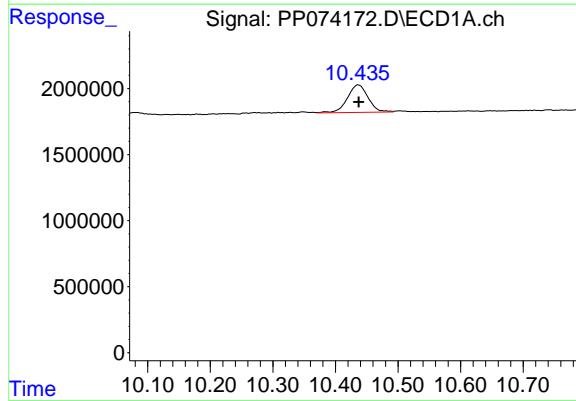


#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 4796081
Conc: 5.14 ng/ml

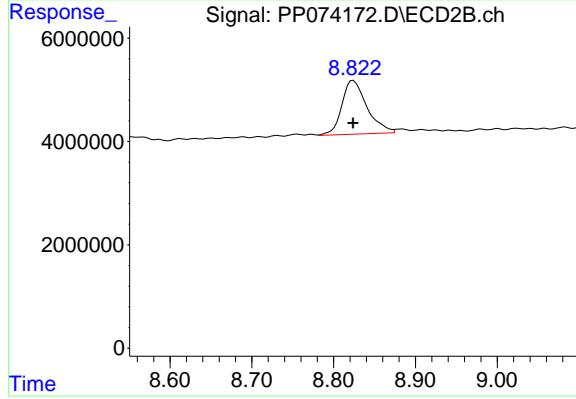

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 22193655
Conc: 3.86 ng/ml

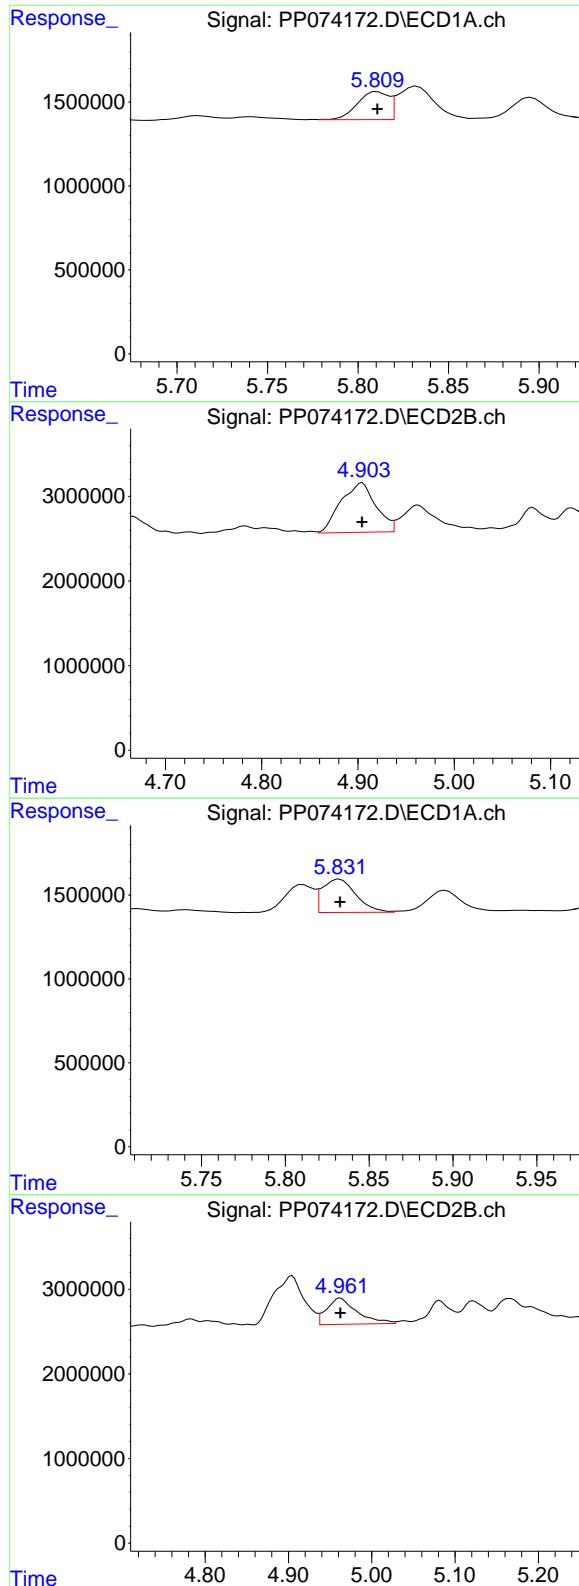

#3 AR-1016-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 1988336
 Conc: 50.87 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC050

#3 AR-1016-1


R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 14775918
 Conc: 38.89 ng/ml

#4 AR-1016-2

R.T.: 5.833 min
 Delta R.T.: 0.000 min
 Response: 2791158
 Conc: 48.82 ng/ml

#4 AR-1016-2

R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 7843665
 Conc: 42.53 ng/ml

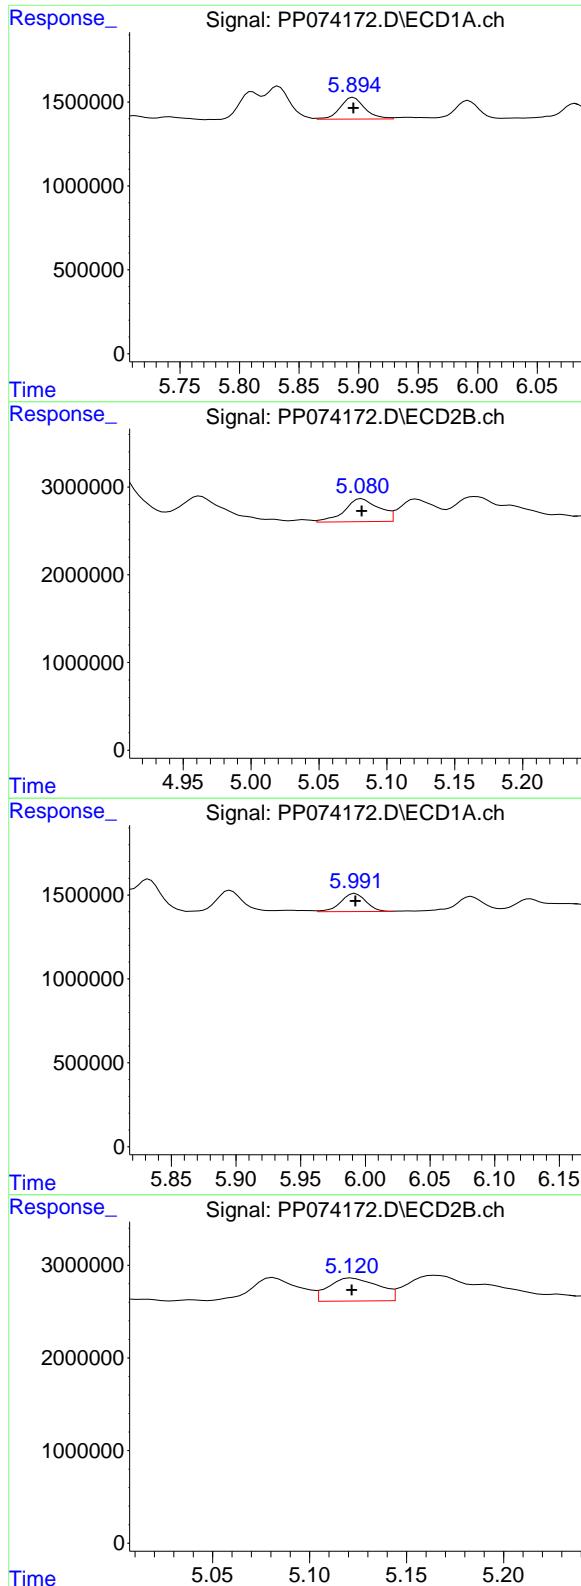

#5 AR-1016-3

R.T.: 5.896 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 1878829 ECD_P
 Conc: 50.17 ng/ml **ClientSampleId:**
 AR1660ICC050

#5 AR-1016-3


R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 4619486
 Conc: 44.08 ng/ml

#6 AR-1016-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 1465464
 Conc: 47.57 ng/ml

#6 AR-1016-4

R.T.: 5.122 min
 Delta R.T.: 0.000 min
 Response: 4449408
 Conc: 42.85 ng/ml

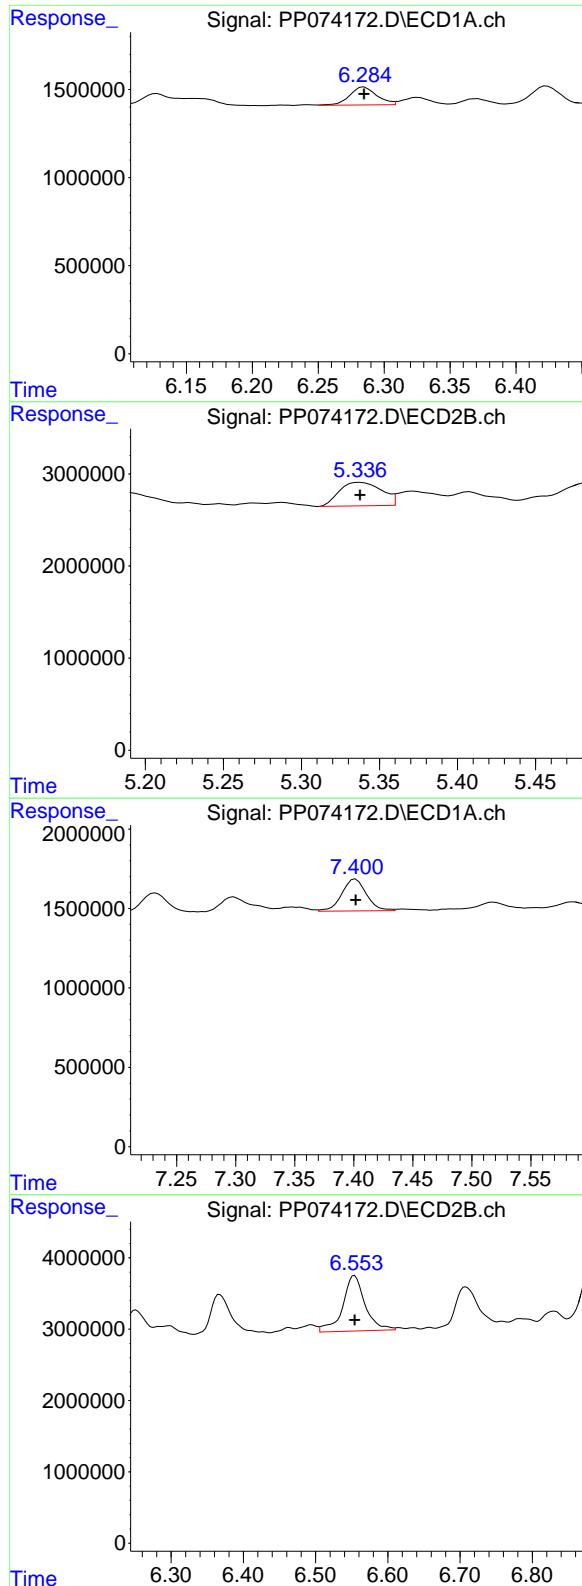

#7 AR-1016-5

R.T.: 6.285 min
 Delta R.T.: 0.000 min
 Response: 1456706
 Conc: 47.50 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660ICC050

#7 AR-1016-5


R.T.: 5.337 min
 Delta R.T.: 0.000 min
 Response: 4779894
 Conc: 42.13 ng/ml

#31 AR-1260-1

R.T.: 7.402 min
 Delta R.T.: 0.000 min
 Response: 2907384
 Conc: 53.84 ng/ml

#31 AR-1260-1

R.T.: 6.554 min
 Delta R.T.: 0.000 min
 Response: 16702003
 Conc: 42.31 ng/ml

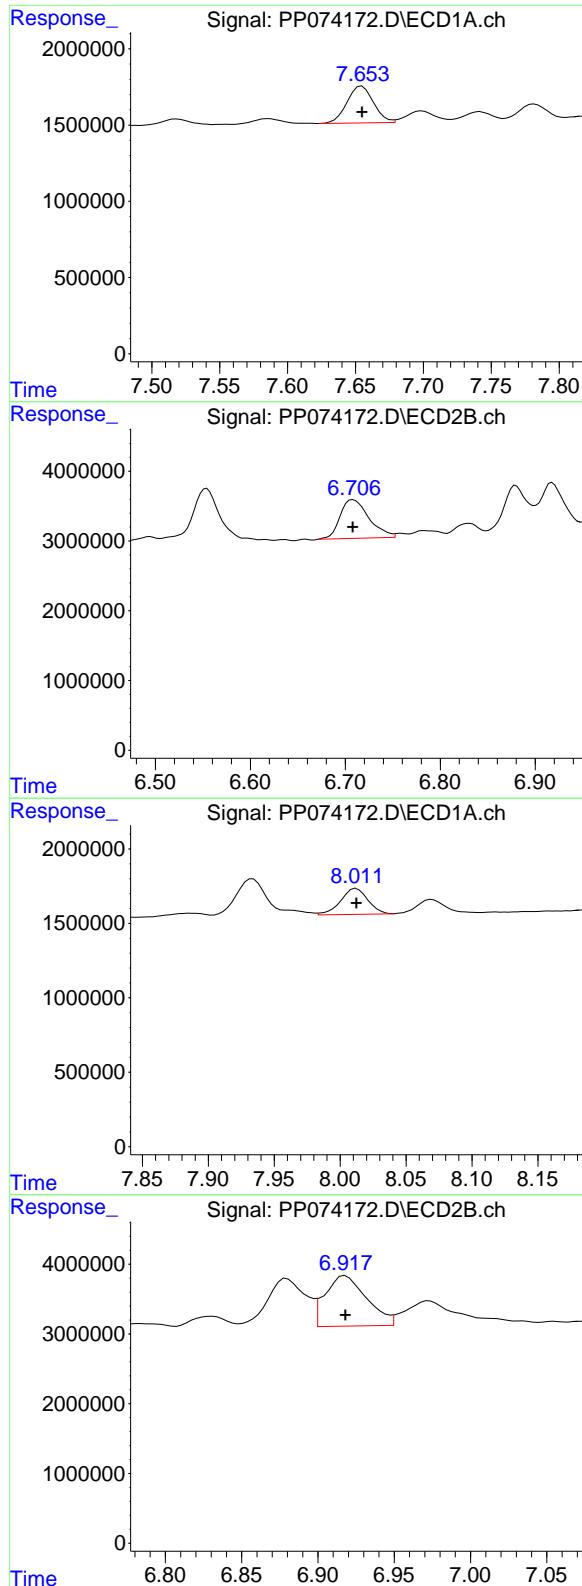

#32 AR-1260-2

R.T.: 7.655 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 3290166 ECD_P
 Conc: 51.77 ng/ml **ClientSampleId:**
 AR1660ICC050

#32 AR-1260-2


R.T.: 6.708 min
 Delta R.T.: 0.000 min
 Response: 11775837
 Conc: 40.36 ng/ml

#33 AR-1260-3

R.T.: 8.012 min
 Delta R.T.: 0.000 min
 Response: 2515483
 Conc: 50.08 ng/ml

#33 AR-1260-3

R.T.: 6.918 min
 Delta R.T.: 0.000 min
 Response: 13666247
 Conc: 36.22 ng/ml

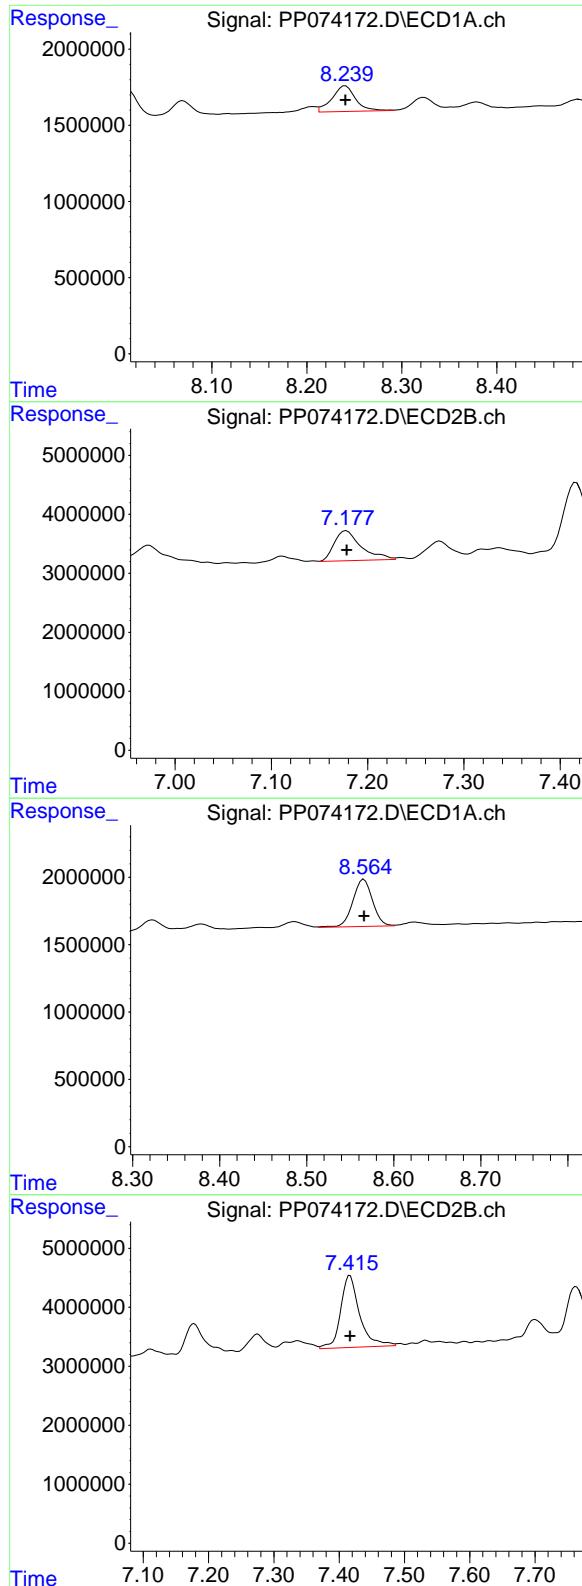

#34 AR-1260-4

R.T.: 8.241 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 2924100 ECD_P
 Conc: 49.31 ng/ml **ClientSampleId:**
 AR1660ICC050

#34 AR-1260-4

R.T.: 7.178 min
 Delta R.T.: 0.000 min
 Response: 9844627
 Conc: 35.69 ng/ml

#35 AR-1260-5

R.T.: 8.566 min
 Delta R.T.: 0.000 min
 Response: 5505858
 Conc: 51.35 ng/ml

#35 AR-1260-5

R.T.: 7.417 min
 Delta R.T.: 0.000 min
 Response: 24685436
 Conc: 33.93 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:15
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:17:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:13:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.660 | 3.804 | 54684846 | 201.8E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.437 | 8.826 | 47117835 | 301.0E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|-----------|
| 8) L2 AR-1221-1 | 4.858 | 4.015 | 5316620 | 14977475 | 317.152 | 305.132 |
| 9) L2 AR-1221-2 | 4.945 | 4.101 | 4648979 | 12599168 | 368.936 | 351.056 |
| 10) L2 AR-1221-3 | 5.020 | 4.177 | 14518661 | 50681220 | 396.303 | 374.793 |
| 11) L3 AR-1232-1 | 5.020 | 4.177 | 14518661 | 50681220 | 500.000 | 500.000 |
| 12) L3 AR-1232-2 | 5.546 | 4.904 | 7521357 | 87133099 | 500.000 | 500.000 |
| 13) L3 AR-1232-3 | 5.832 | 5.081 | 14500854 | 22908311 | 500.000 | 500.000 |
| 14) L3 AR-1232-4 | 5.993 | 5.165 | 7734413 | 36297070 | 500.000 | 628.698 # |
| 15) L3 AR-1232-5 | 6.082 | 5.338 | 5858006 | 23489726 | 500.000 | 500.000 |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074174.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:15
 Operator : YP\AJ
 Sample : AR1232ICC500
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1232ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:17:09 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:13:54 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

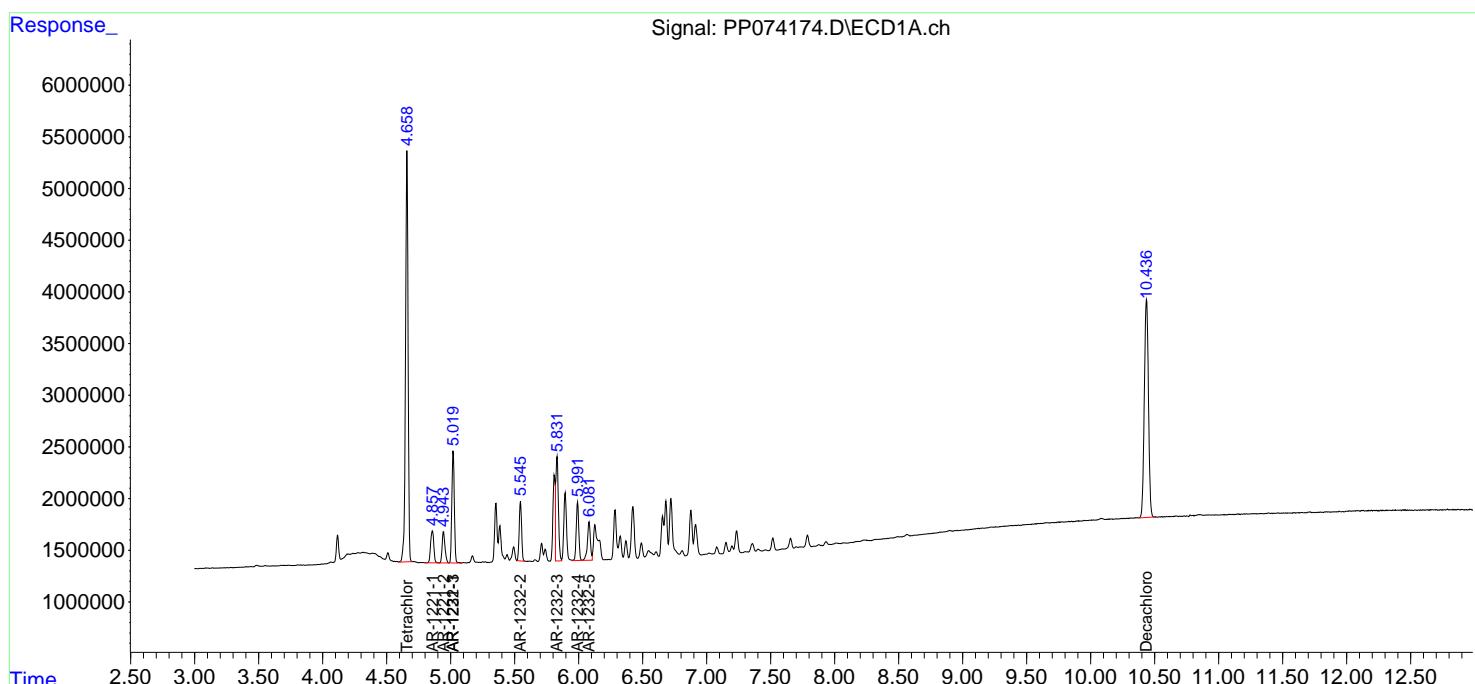




#1 Tetrachloro-m-xylene
R.T.: 4.660 min
Delta R.T.: 0.000 min
Response: 54684846
Conc: 50.00 ng/ml


Instrument: ECD_P
ClientSampleId: AR1232ICC500

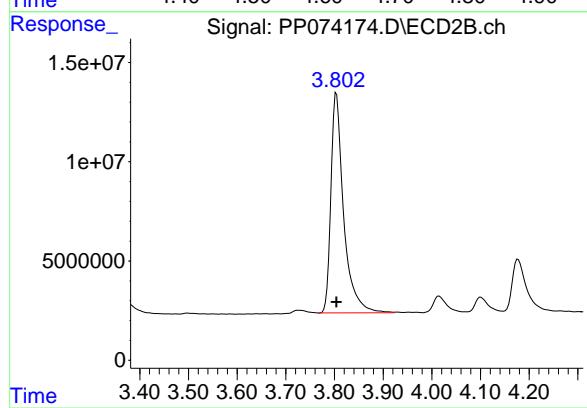


#1 Tetrachloro-m-xylene
R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 201821673
Conc: 50.00 ng/ml

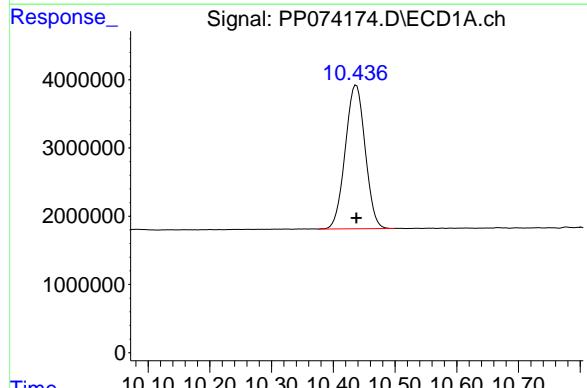

#2 Decachlorobiphenyl
R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 47117835
Conc: 50.00 ng/ml

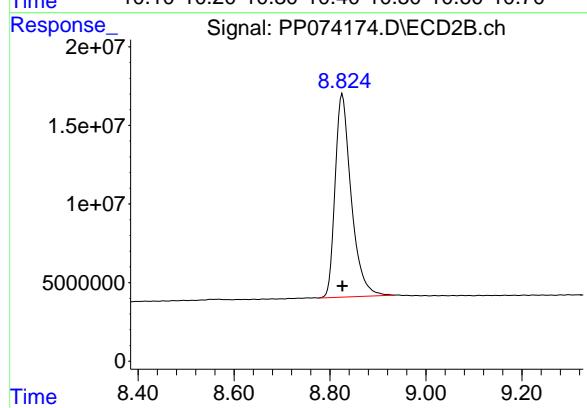


#2 Decachlorobiphenyl
R.T.: 8.826 min
Delta R.T.: 0.000 min
Response: 300994205
Conc: 50.00 ng/ml



#8 AR-1221-1


R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 5316620
Conc: 317.15 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

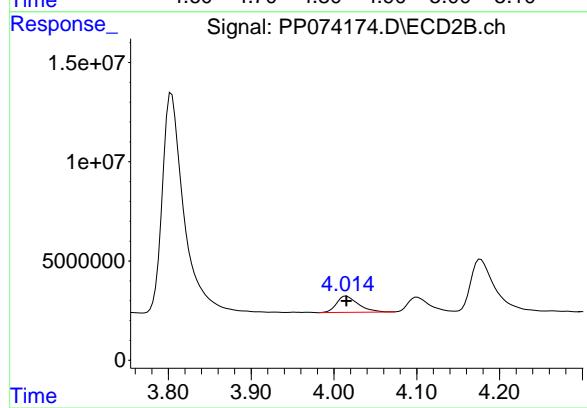


#8 AR-1221-1

R.T.: 4.015 min
Delta R.T.: 0.000 min
Response: 14977475
Conc: 305.13 ng/ml

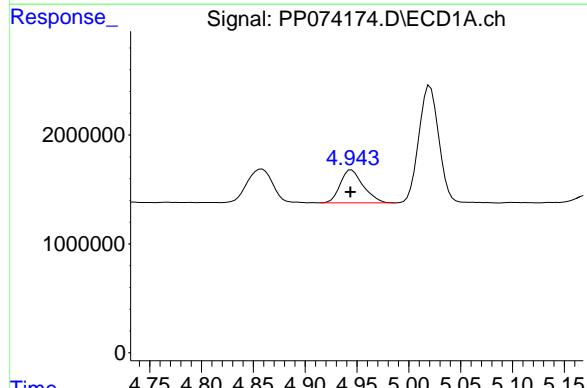


#9 AR-1221-2

R.T.: 4.945 min
Delta R.T.: 0.001 min
Response: 4648979
Conc: 368.94 ng/ml

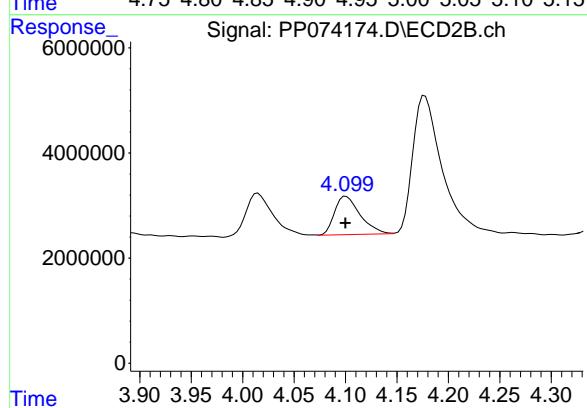

#9 AR-1221-2

R.T.: 4.101 min
Delta R.T.: 0.000 min
Response: 12599168
Conc: 351.06 ng/ml

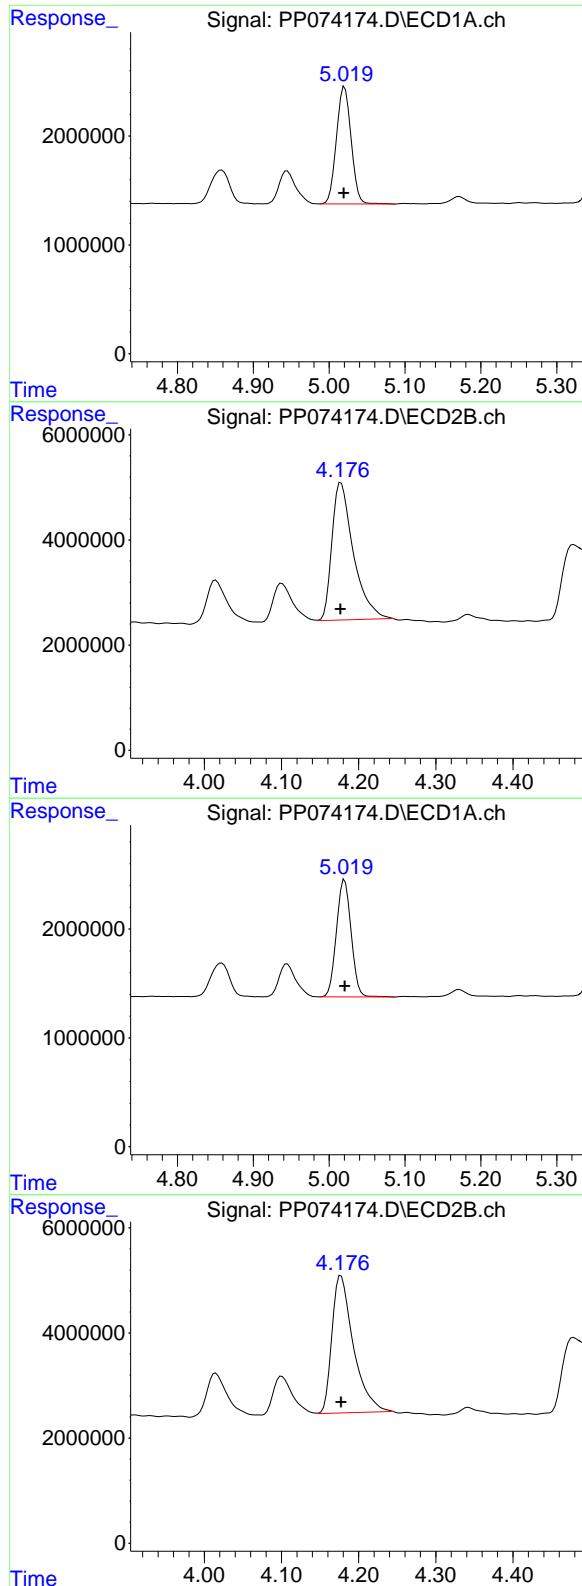

#10 AR-1221-3

R.T.: 5.020 min
 Delta R.T.: 0.001 min
 Response: 14518661
 Conc: 396.30 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1232ICC500

#10 AR-1221-3


R.T.: 4.177 min
 Delta R.T.: 0.000 min
 Response: 50681220
 Conc: 374.79 ng/ml

#11 AR-1232-1

R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 14518661
 Conc: 500.00 ng/ml

#11 AR-1232-1

R.T.: 4.177 min
 Delta R.T.: 0.000 min
 Response: 50681220
 Conc: 500.00 ng/ml

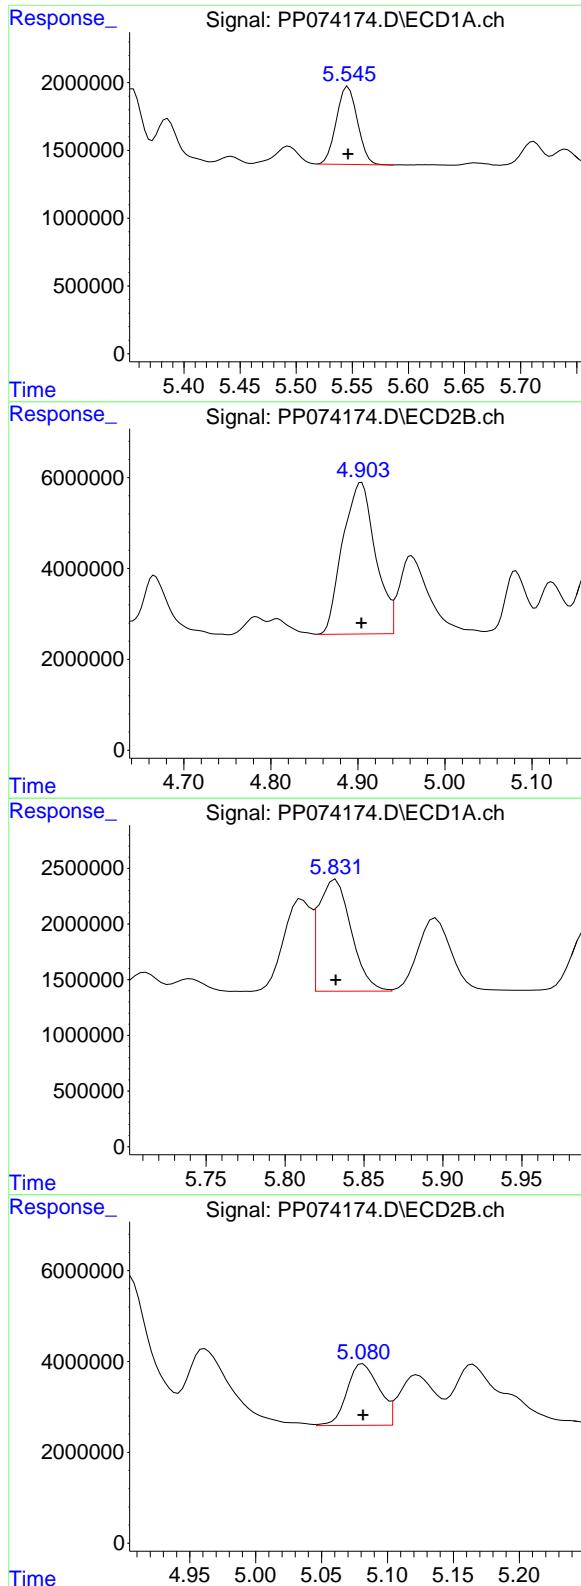

#12 AR-1232-2

R.T.: 5.546 min
 Delta R.T.: 0.000 min
 Response: 7521357
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1232ICC500

#12 AR-1232-2


R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 87133099
 Conc: 500.00 ng/ml

#13 AR-1232-3

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 14500854
 Conc: 500.00 ng/ml

#13 AR-1232-3


R.T.: 5.081 min
 Delta R.T.: 0.000 min
 Response: 22908311
 Conc: 500.00 ng/ml



#14 AR-1232-4


R.T.: 5.993 min
 Delta R.T.: 0.000 min
 Response: 7734413
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1232ICC500

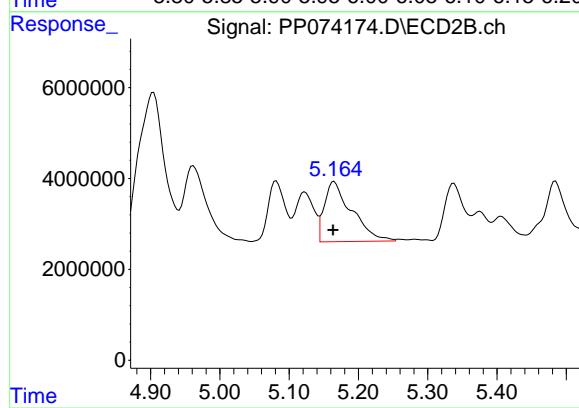


#14 AR-1232-4

R.T.: 5.165 min
 Delta R.T.: 0.001 min
 Response: 36297070
 Conc: 628.70 ng/ml

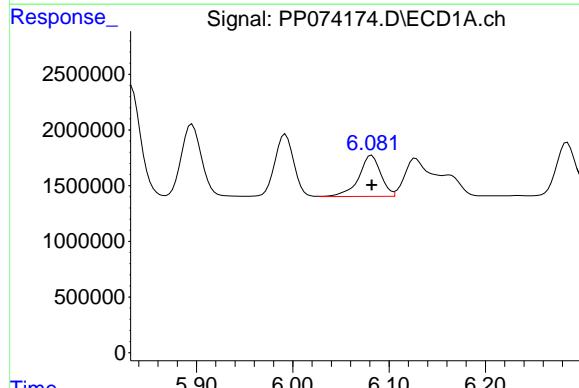

#15 AR-1232-5

R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 5858006
 Conc: 500.00 ng/ml

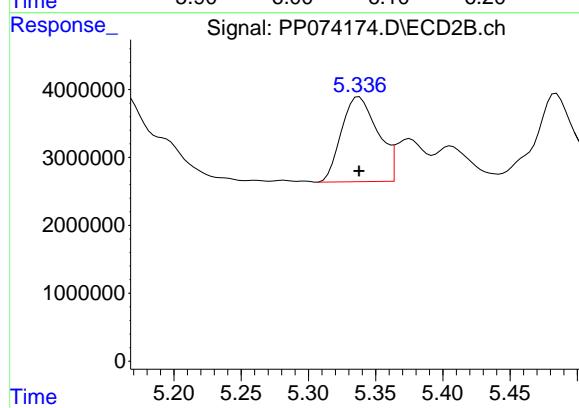

#15 AR-1232-5

R.T.: 5.338 min
 Delta R.T.: 0.000 min
 Response: 23489726
 Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:31
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:23:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|---------|
| 1) SA Tetrachlor... | 4.659 | 3.804 | 104.3E6 | 438.1E6 | 95.872 | 101.577 |
| 2) SA Decachlor... | 10.436 | 8.825 | 88078600 | 618.2E6 | 94.444 | 98.714 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|------------|
| 16) L4 AR-1242-1 | 5.811 | 4.905 | 31512428 | 341.3E6 | 934.658 | 978.632 |
| 17) L4 AR-1242-2 | 5.832 | 4.962 | 47421171 | 162.7E6 | 943.850 | 992.758 |
| 18) L4 AR-1242-3 | 5.896 | 5.082 | 30290298 | 93075141 | 931.794 | 1005.327 |
| 19) L4 AR-1242-4 | 5.992 | 5.165 | 25177060 | 162.5E6 | 934.754 | 1303.690 # |
| 20) L4 AR-1242-5 | 6.721 | 5.686 | 29128304 | 140.7E6 | 916.924 | 973.631 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074175.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:31
 Operator : YP\AJ
 Sample : AR1242ICC1000
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:23:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

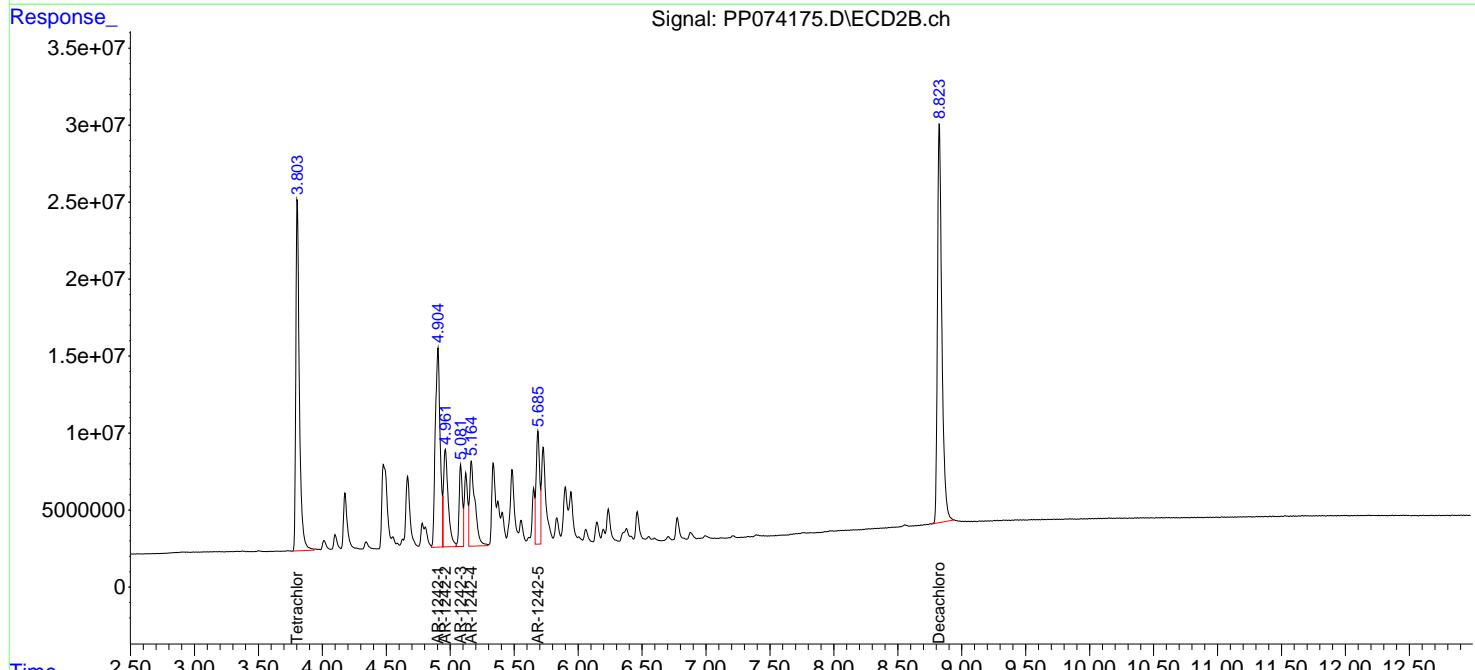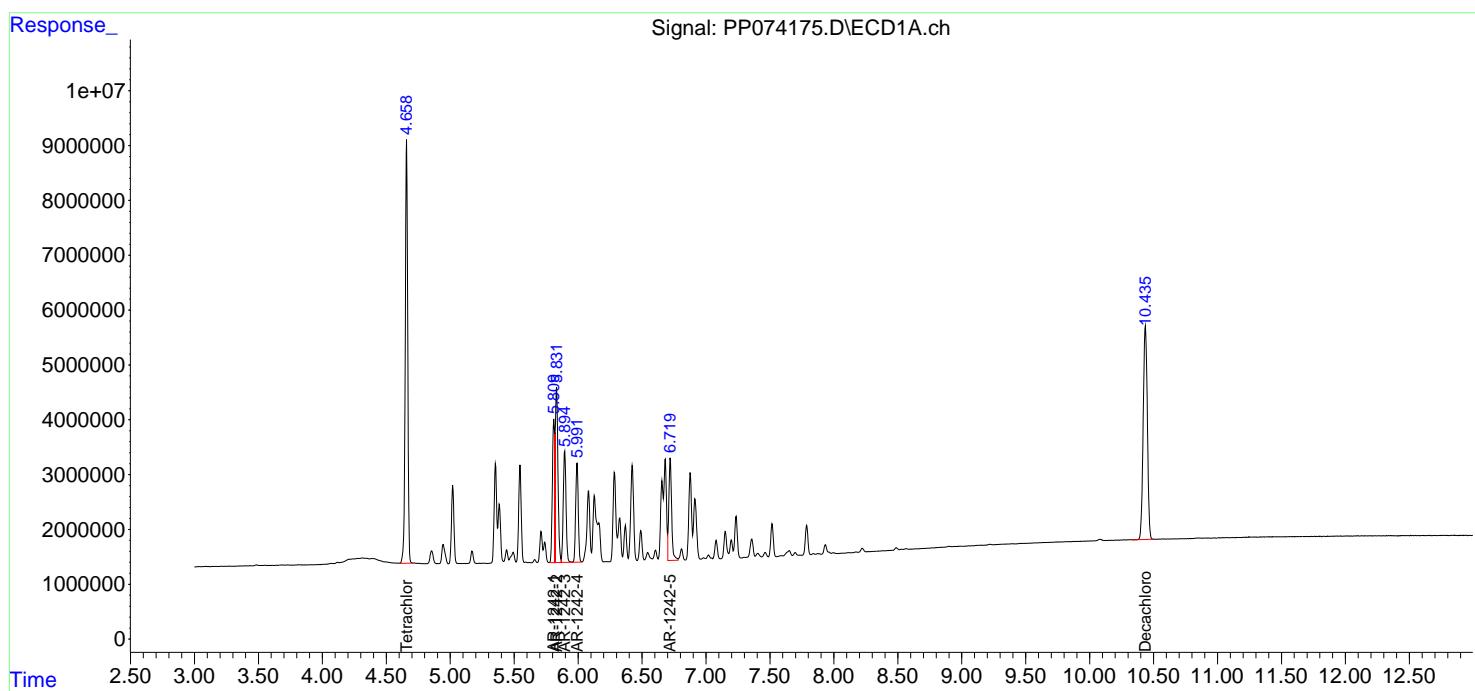




#1 Tetrachloro-m-xylene
R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 104324065
Conc: 95.87 ng/ml


Instrument: ECD_P
ClientSampleId: AR1242ICC1000

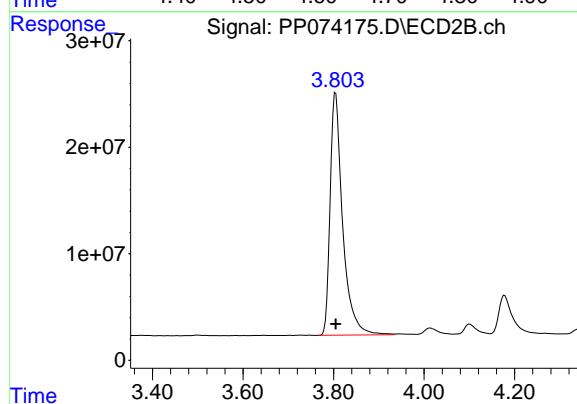


#1 Tetrachloro-m-xylene
R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 438073172
Conc: 101.58 ng/ml

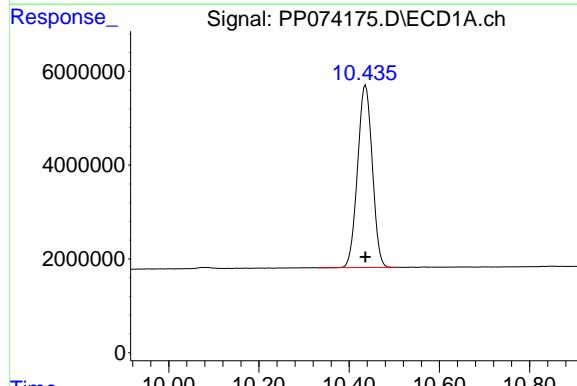

#2 Decachlorobiphenyl
R.T.: 10.436 min
Delta R.T.: 0.000 min
Response: 88078600
Conc: 94.44 ng/ml

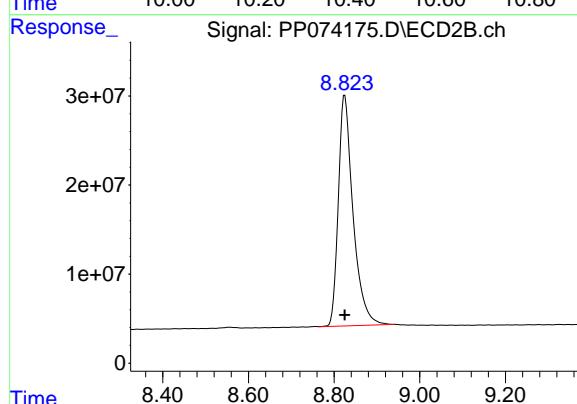


#2 Decachlorobiphenyl
R.T.: 8.825 min
Delta R.T.: 0.000 min
Response: 618210330
Conc: 98.71 ng/ml

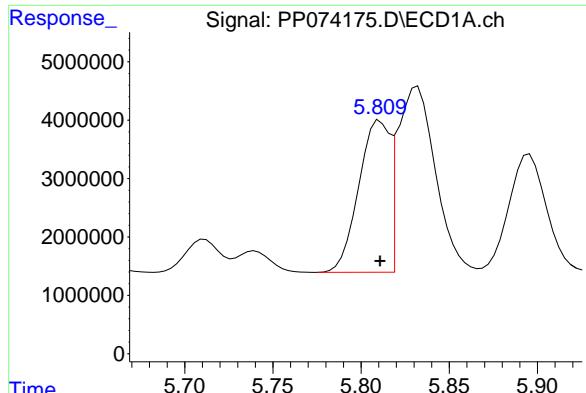

#16 AR-1242-1


R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 31512428
 Conc: 934.66 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC1000

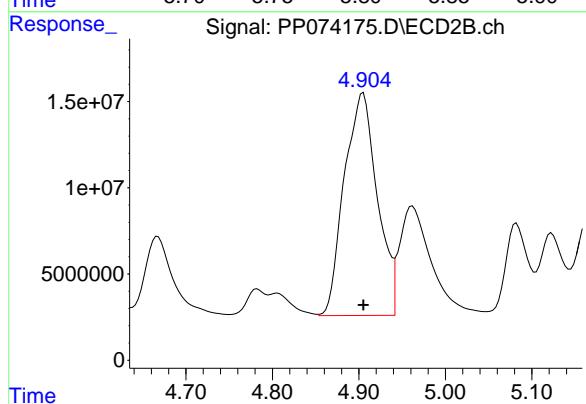


#16 AR-1242-1

R.T.: 4.905 min
 Delta R.T.: 0.000 min
 Response: 341272725
 Conc: 978.63 ng/ml

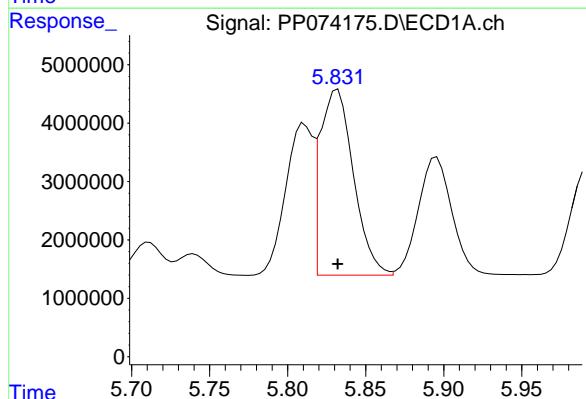


#17 AR-1242-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 47421171
 Conc: 943.85 ng/ml

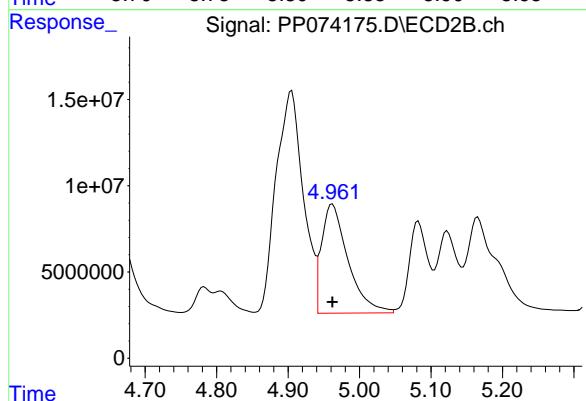

#17 AR-1242-2


R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 162660327
 Conc: 992.76 ng/ml

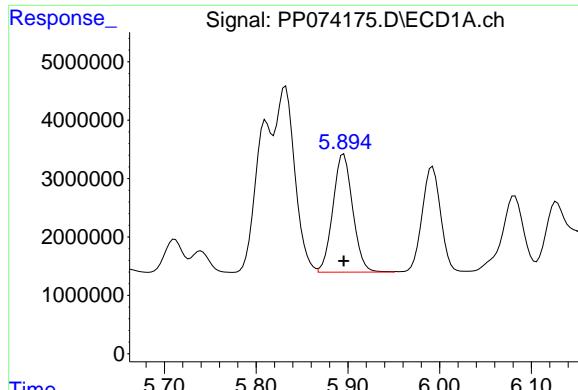

#18 AR-1242-3


R.T.: 5.896 min
 Delta R.T.: 0.000 min
 Response: 30290298
 Conc: 931.79 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC1000

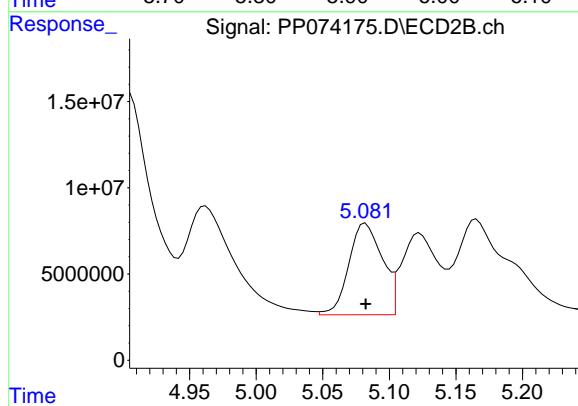


#18 AR-1242-3

R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 93075141
 Conc: 1005.33 ng/ml

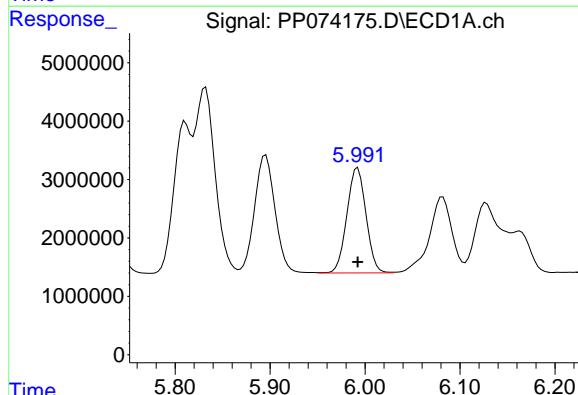


#19 AR-1242-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 25177060
 Conc: 934.75 ng/ml

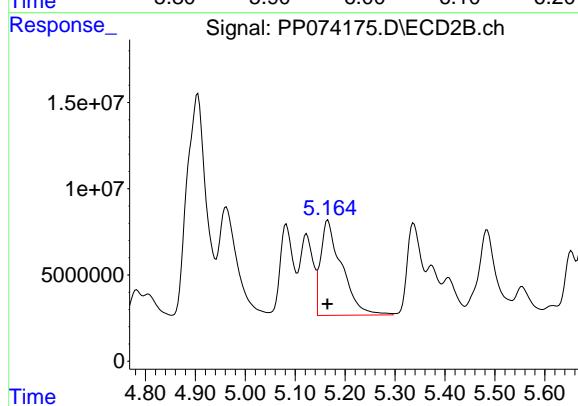

#19 AR-1242-4

R.T.: 5.165 min
 Delta R.T.: 0.001 min
 Response: 162521092
 Conc: 1303.69 ng/ml

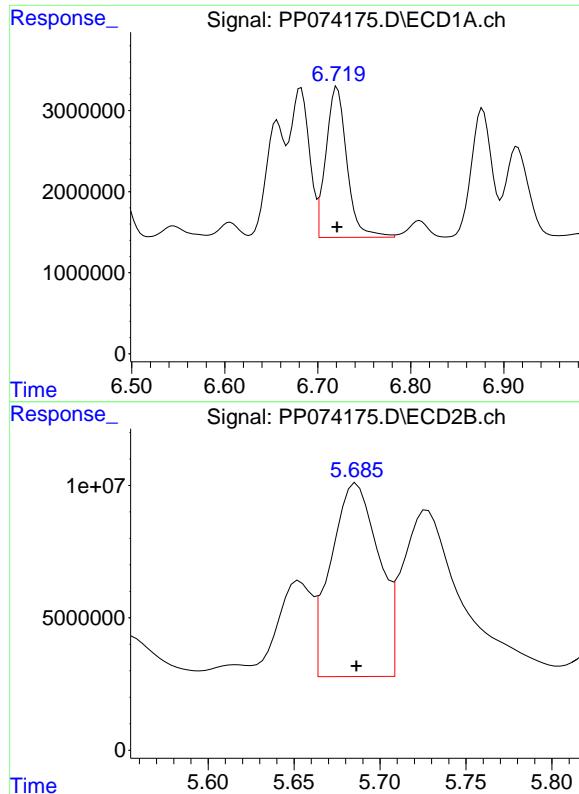

#20 AR-1242-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 29128304
 Conc: 916.92 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC1000

#20 AR-1242-5

R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 140731652
 Conc: 973.63 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:47
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:26:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.662 | 3.803 | 80676637 | 324.0E6 | 74.425 | 75.083 |
| 2) SA Decachlor... | 10.438 | 8.824 | 68962955 | 464.9E6 | 74.295 | 74.485 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|------------|
| 16) L4 AR-1242-1 | 5.813 | 4.904 | 25064705 | 261.4E6 | 745.599 | 749.732 |
| 17) L4 AR-1242-2 | 5.835 | 4.960 | 37017188 | 128.7E6 | 741.131 | 773.381 |
| 18) L4 AR-1242-3 | 5.898 | 5.081 | 24057234 | 72718391 | 743.338 | 773.266 |
| 19) L4 AR-1242-4 | 5.995 | 5.164 | 19974989 | 130.9E6 | 744.389 | 1065.577 # |
| 20) L4 AR-1242-5 | 6.724 | 5.685 | 24065795 | 114.3E6 | 755.025 | 776.822 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074176.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 14:47
 Operator : YP\AJ
 Sample : AR1242ICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:26:53 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

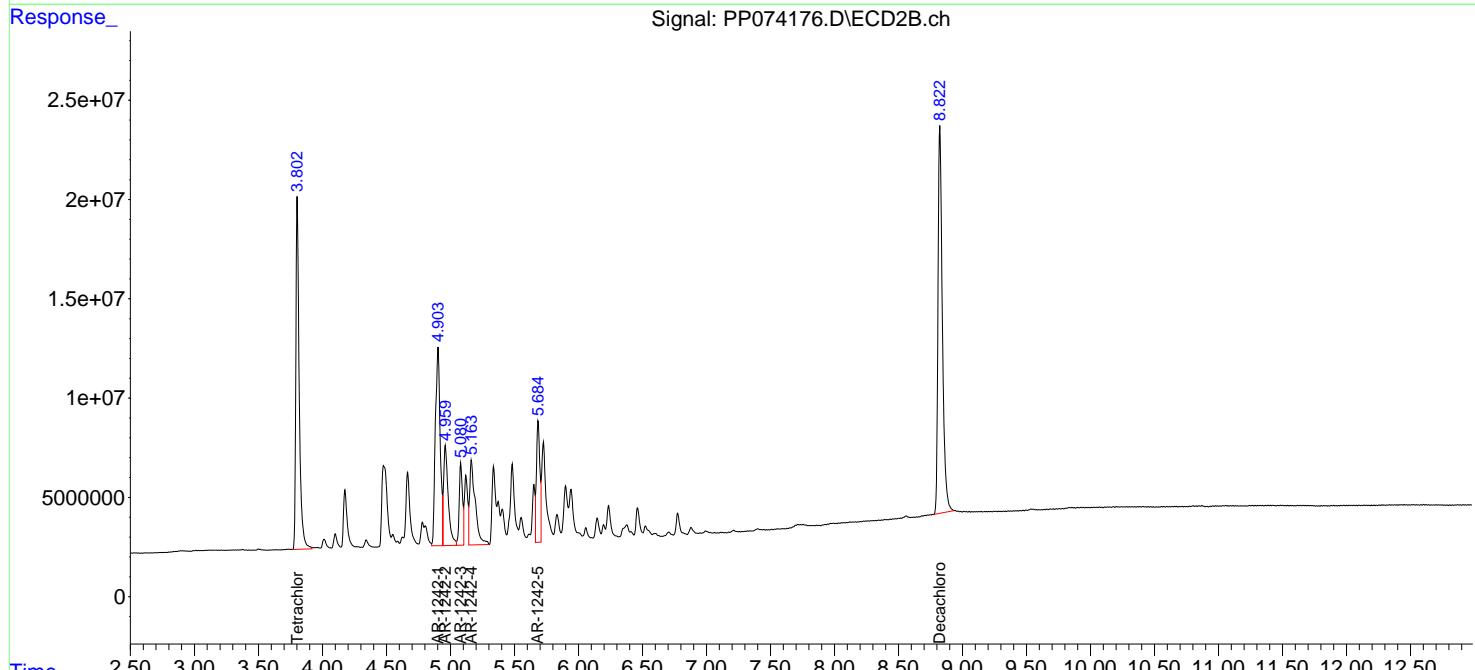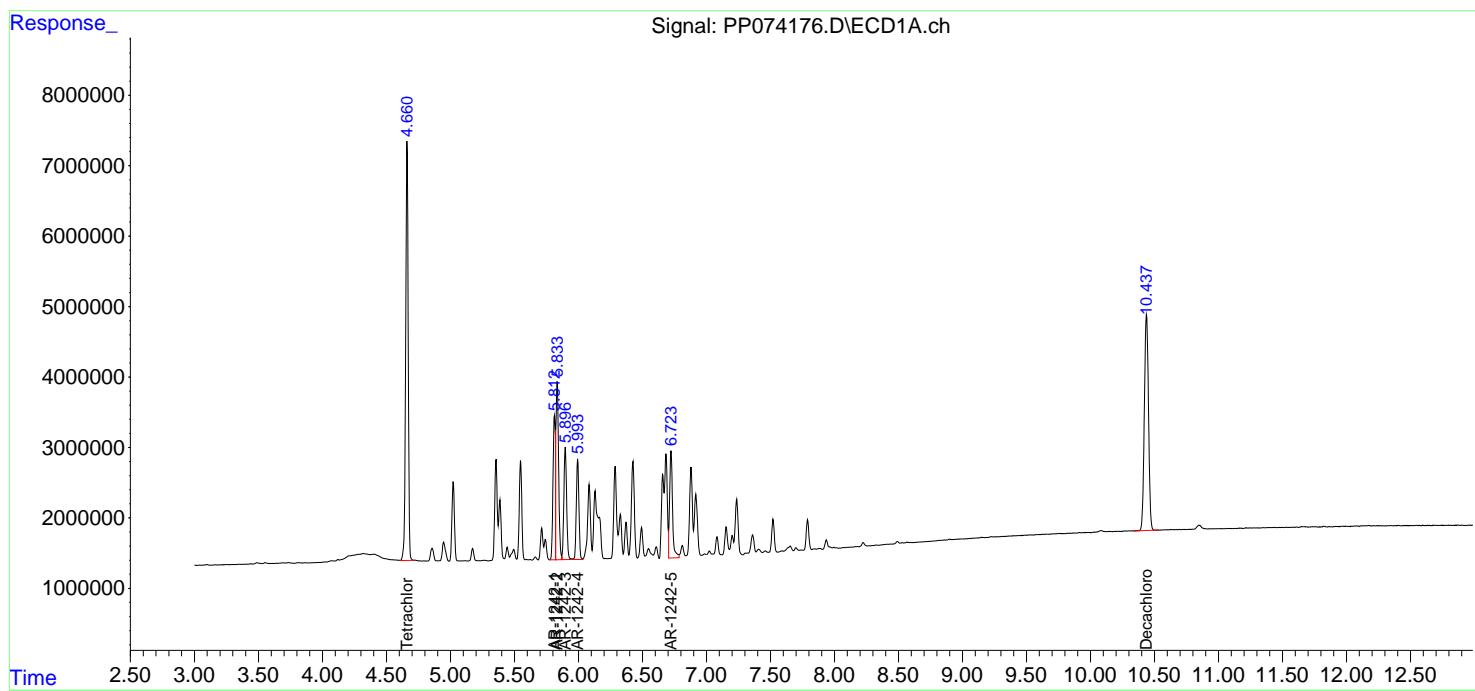

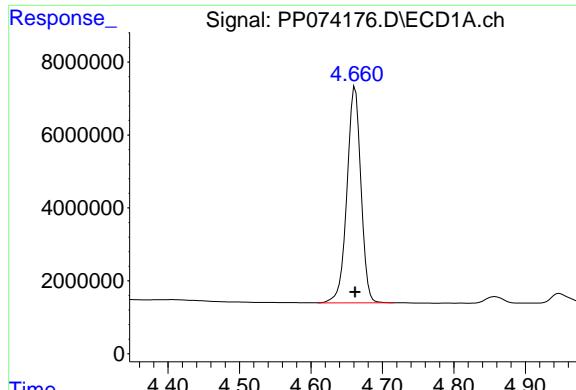

#1 Tetrachloro-m-xylene


R.T.: 4.662 min
Delta R.T.: 0.000 min
Response: 80676637
Conc: 74.42 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1242ICC750

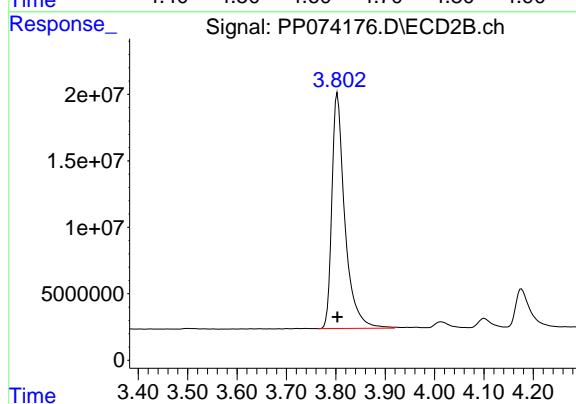


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 323988872
Conc: 75.08 ng/ml

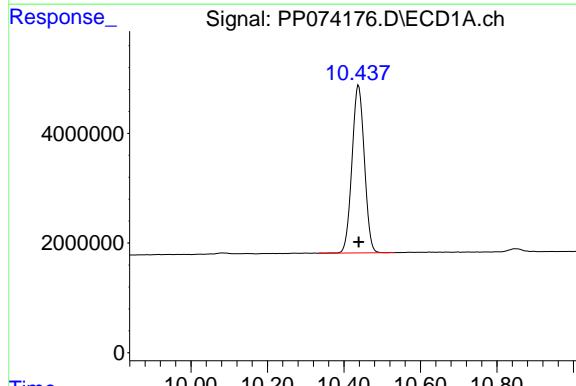


#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.000 min
Response: 68962955
Conc: 74.29 ng/ml

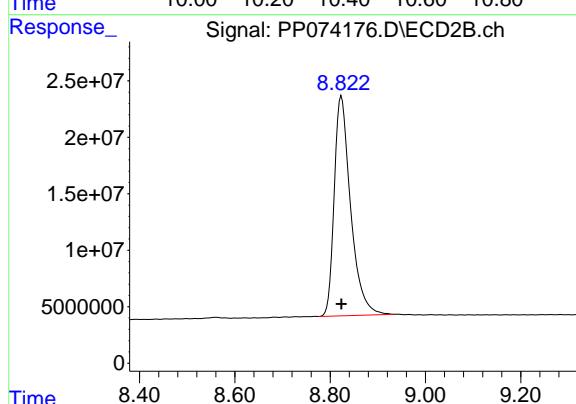

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 464876495
Conc: 74.48 ng/ml

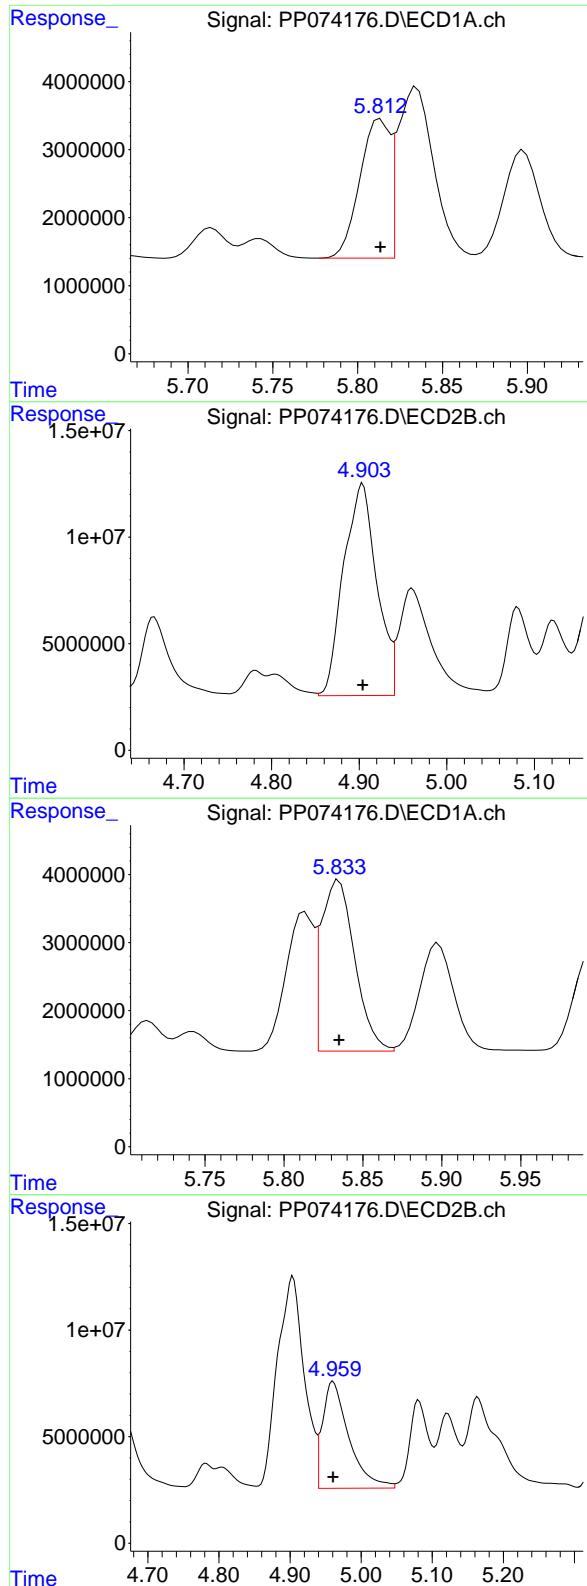

#16 AR-1242-1

R.T.: 5.813 min
 Delta R.T.: 0.000 min
 Response: 25064705
 Conc: 745.60 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC750

#16 AR-1242-1


R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 261402874
 Conc: 749.73 ng/ml

#17 AR-1242-2

R.T.: 5.835 min
 Delta R.T.: 0.000 min
 Response: 37017188
 Conc: 741.13 ng/ml

#17 AR-1242-2


R.T.: 4.960 min
 Delta R.T.: 0.000 min
 Response: 128722469
 Conc: 773.38 ng/ml



#18 AR-1242-3


R.T.: 5.898 min
 Delta R.T.: 0.000 min
 Response: 24057234
 Conc: 743.34 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC750

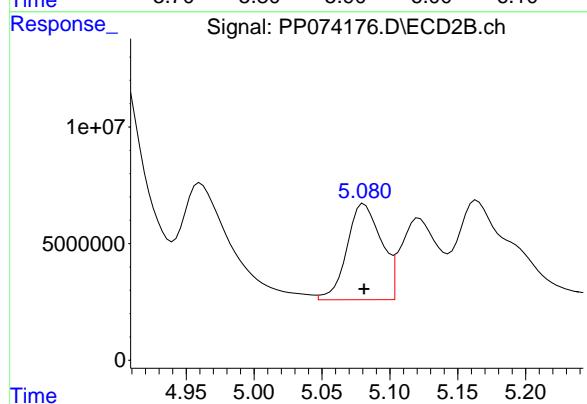


#18 AR-1242-3

R.T.: 5.081 min
 Delta R.T.: 0.000 min
 Response: 72718391
 Conc: 773.27 ng/ml

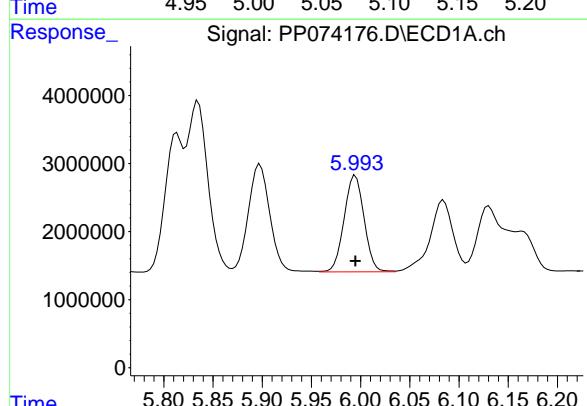


#19 AR-1242-4

R.T.: 5.995 min
 Delta R.T.: 0.000 min
 Response: 19974989
 Conc: 744.39 ng/ml

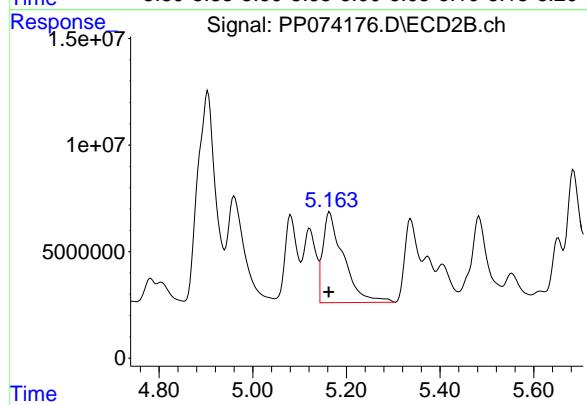

#19 AR-1242-4

R.T.: 5.164 min
 Delta R.T.: 0.001 min
 Response: 130863576
 Conc: 1065.58 ng/ml

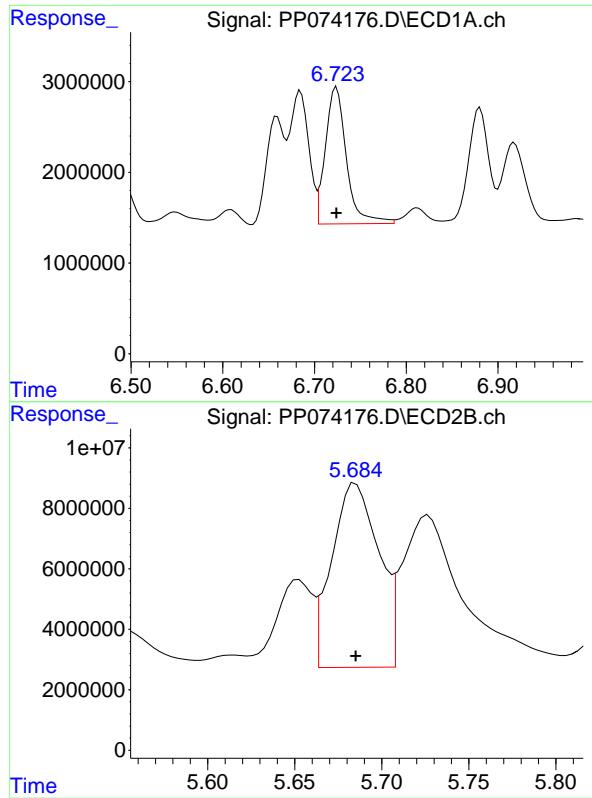

#20 AR-1242-5

R.T.: 6.724 min
Delta R.T.: 0.000 min
Response: 24065795
Conc: 755.02 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC750

#20 AR-1242-5

R.T.: 5.685 min
Delta R.T.: 0.000 min
Response: 114328693
Conc: 776.82 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:03
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:21:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.805 | 56653742 | 212.2E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.434 | 8.826 | 49220928 | 317.2E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|-----------|
| 16) L4 AR-1242-1 | 5.808 | 4.905 | 17959256 | 178.1E6 | 500.000 | 500.000 |
| 17) L4 AR-1242-2 | 5.830 | 4.963 | 26531667 | 82516708 | 500.000 | 500.000 |
| 18) L4 AR-1242-3 | 5.893 | 5.084 | 17362372 | 46044427 | 500.000 | 500.000 |
| 19) L4 AR-1242-4 | 5.990 | 5.166 | 14345906 | 81425101 | 500.000 | 651.170 # |
| 20) L4 AR-1242-5 | 6.719 | 5.687 | 17203244 | 74177320 | 500.000 | 500.000 |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074177.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:03
 Operator : YP\AJ
 Sample : AR1242ICC500
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:21:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

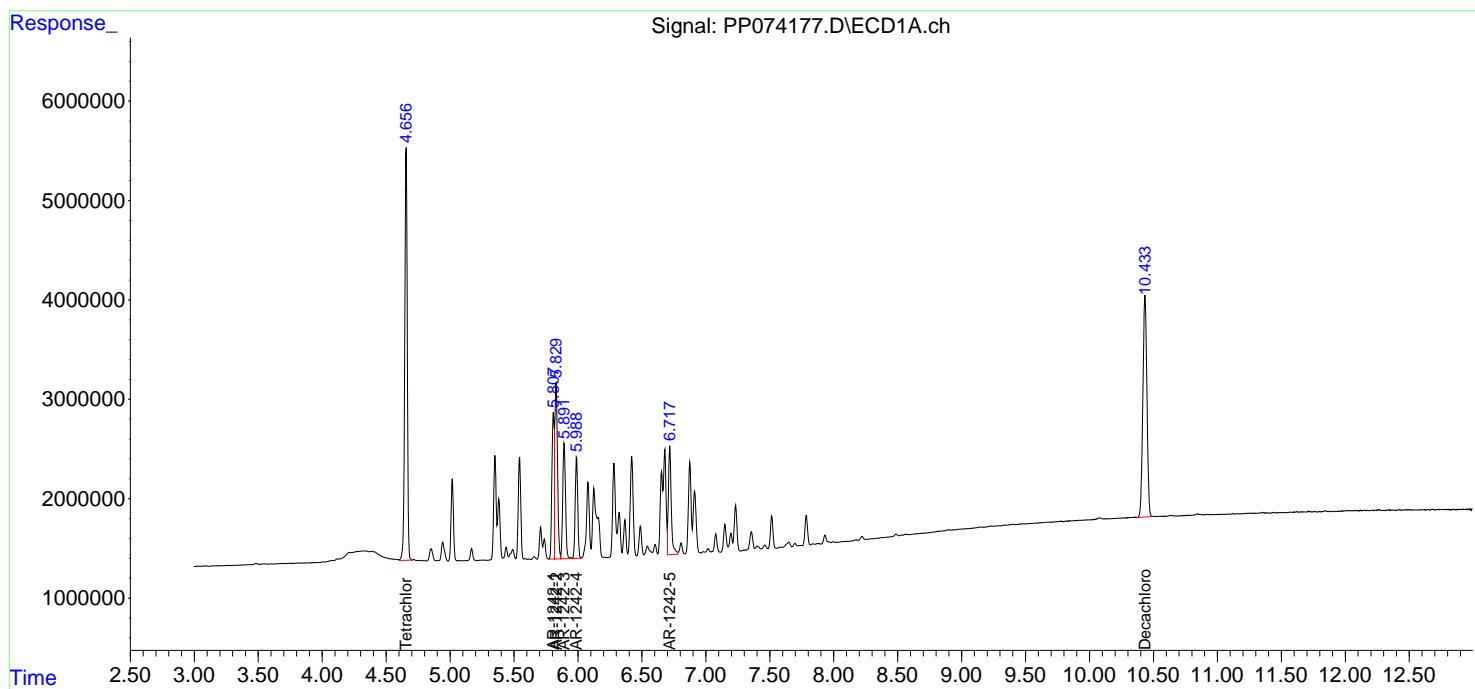



#1 Tetrachloro-m-xylene


R.T.: 4.657 min
Delta R.T.: 0.000 min
Response: 56653742
Conc: 50.00 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1242ICC500

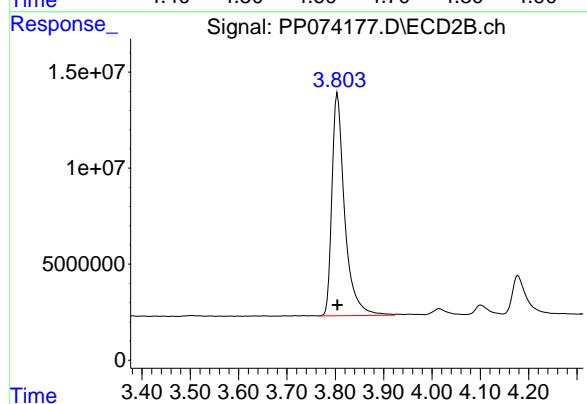


#1 Tetrachloro-m-xylene

R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 212235944
Conc: 50.00 ng/ml

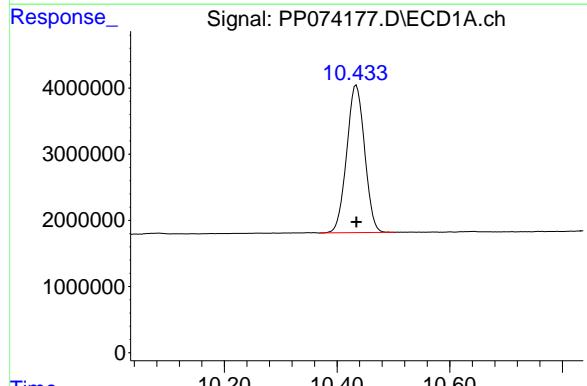


#2 Decachlorobiphenyl

R.T.: 10.434 min
Delta R.T.: 0.000 min
Response: 49220928
Conc: 50.00 ng/ml

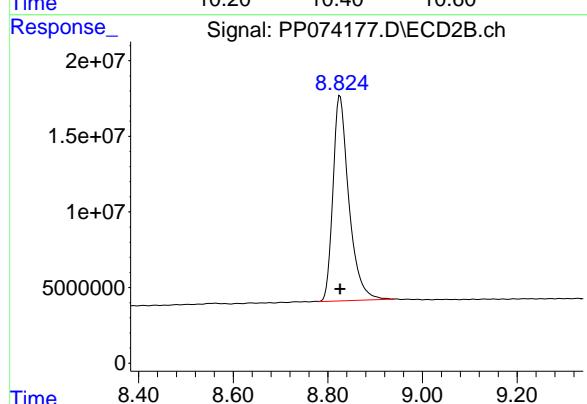

#2 Decachlorobiphenyl

R.T.: 8.826 min
Delta R.T.: 0.000 min
Response: 317160143
Conc: 50.00 ng/ml

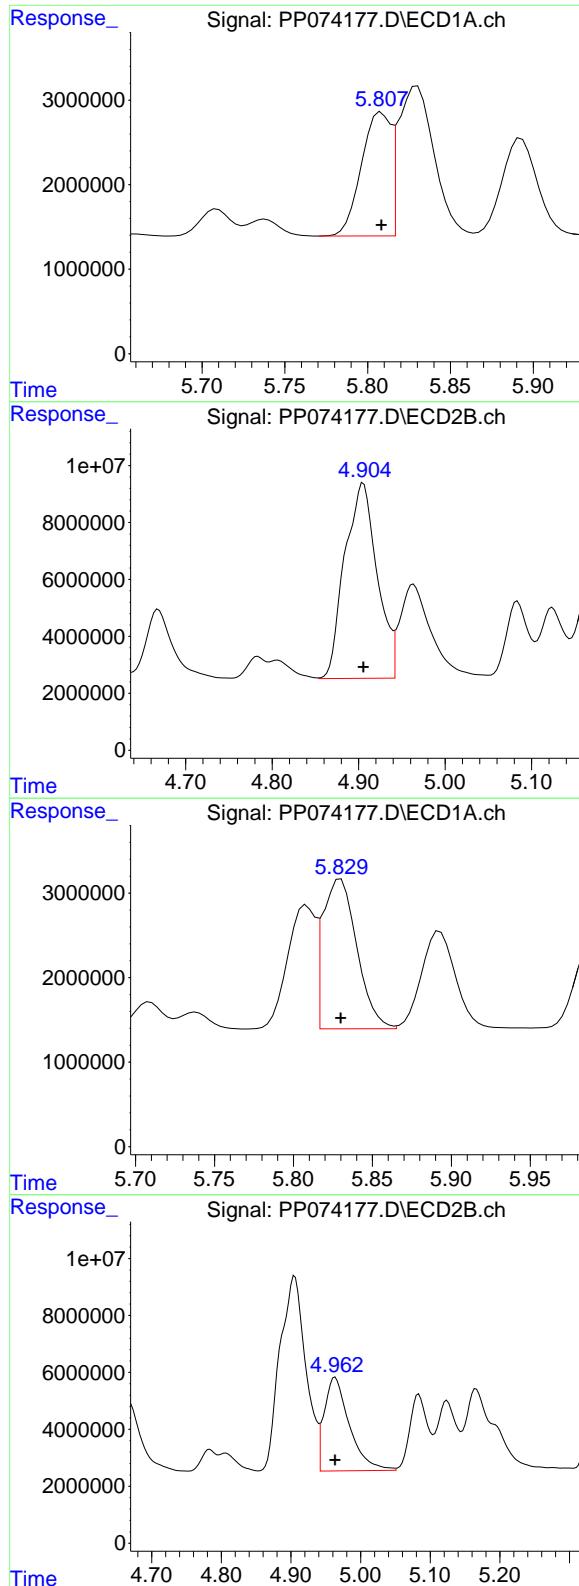

#16 AR-1242-1

R.T.: 5.808 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 17959256 ECD_P
 Conc: 500.00 ng/ml **ClientSampleId:**
 AR1242ICC500

#16 AR-1242-1


R.T.: 4.905 min
 Delta R.T.: 0.000 min
 Response: 178087793
 Conc: 500.00 ng/ml

#17 AR-1242-2

R.T.: 5.830 min
 Delta R.T.: 0.000 min
 Response: 26531667
 Conc: 500.00 ng/ml

#17 AR-1242-2


R.T.: 4.963 min
 Delta R.T.: 0.000 min
 Response: 82516708
 Conc: 500.00 ng/ml

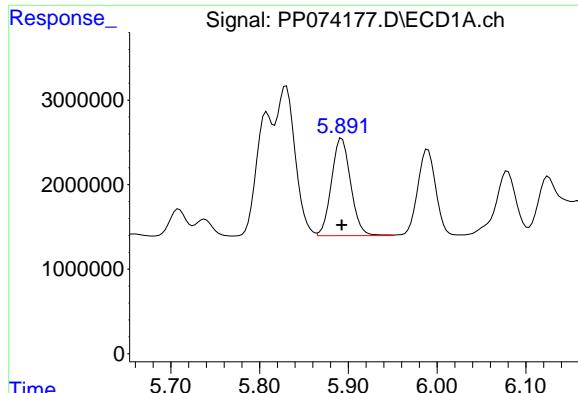

#18 AR-1242-3


R.T.: 5.893 min
 Delta R.T.: 0.000 min
 Response: 17362372
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC500

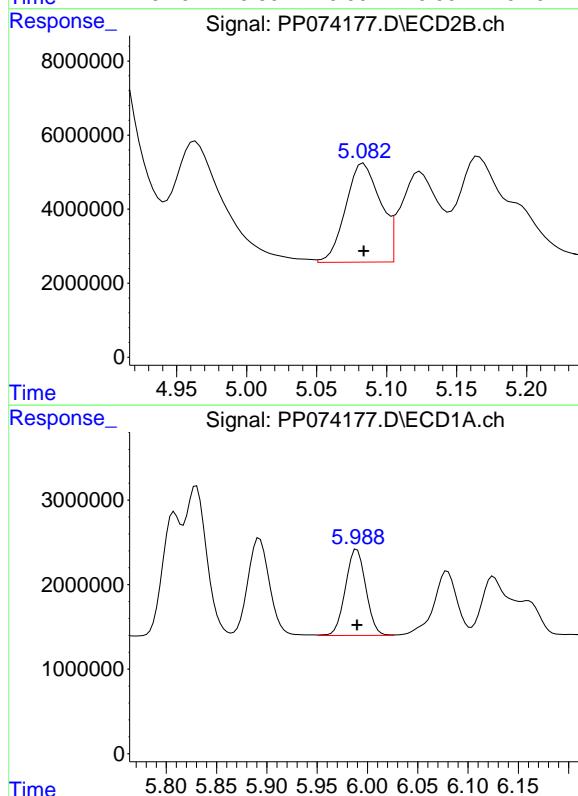


#19 AR-1242-4

R.T.: 5.990 min
 Delta R.T.: 0.000 min
 Response: 14345906
 Conc: 500.00 ng/ml

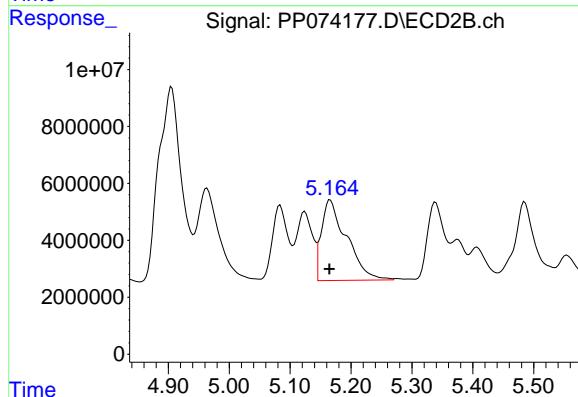

#19 AR-1242-4

R.T.: 5.166 min
 Delta R.T.: 0.002 min
 Response: 81425101
 Conc: 651.17 ng/ml

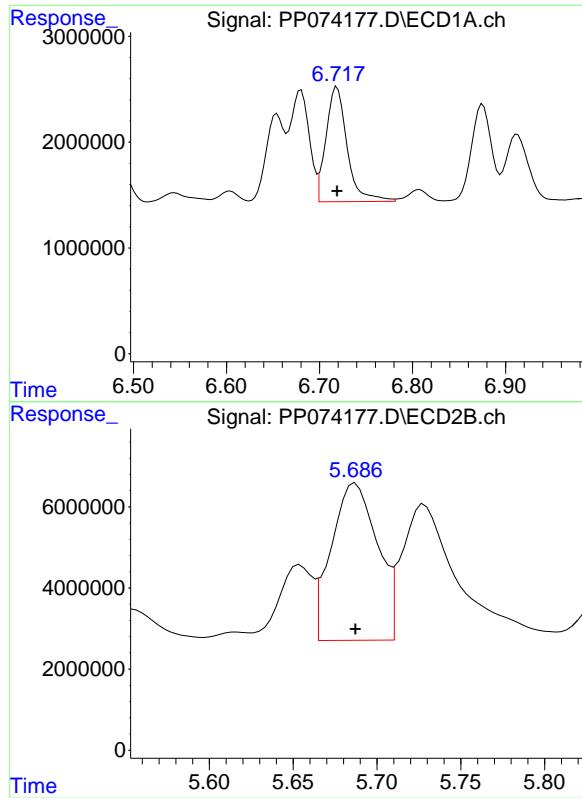

#20 AR-1242-5

R.T.: 6.719 min
 Delta R.T.: 0.000 min
 Response: 17203244
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC500

#20 AR-1242-5

R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 74177320
 Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:19
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:30:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.662 | 3.805 | 30064825 | 99448361 | 26.997 | 23.506 |
| 2) SA Decachlor... | 10.436 | 8.824 | 26416078 | 156.4E6 | 27.507 | 25.039 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|-----------|
| 16) L4 AR-1242-1 | 5.812 | 4.906 | 9924005 | 89565172 | 282.440 | 255.127 |
| 17) L4 AR-1242-2 | 5.834 | 4.964 | 14472673 | 42174411 | 278.680 | 252.533 |
| 18) L4 AR-1242-3 | 5.897 | 5.084 | 9547202 | 24305838 | 282.294 | 256.293 |
| 19) L4 AR-1242-4 | 5.994 | 5.166 | 7737538 | 43979753 | 277.699 | 364.040 # |
| 20) L4 AR-1242-5 | 6.723 | 5.687 | 10585475 | 38870481 | 316.932 | 260.436 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074178.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:19
 Operator : YP\AJ
 Sample : AR1242ICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:30:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:20:45 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

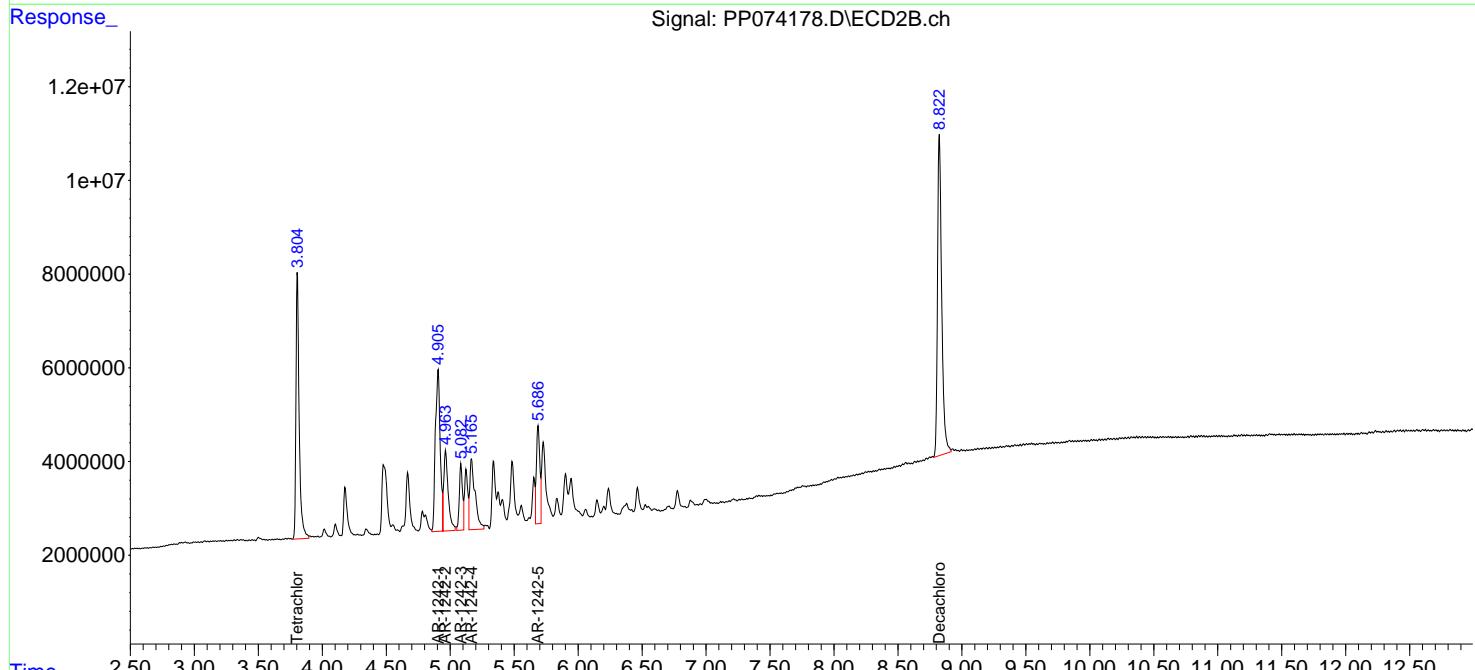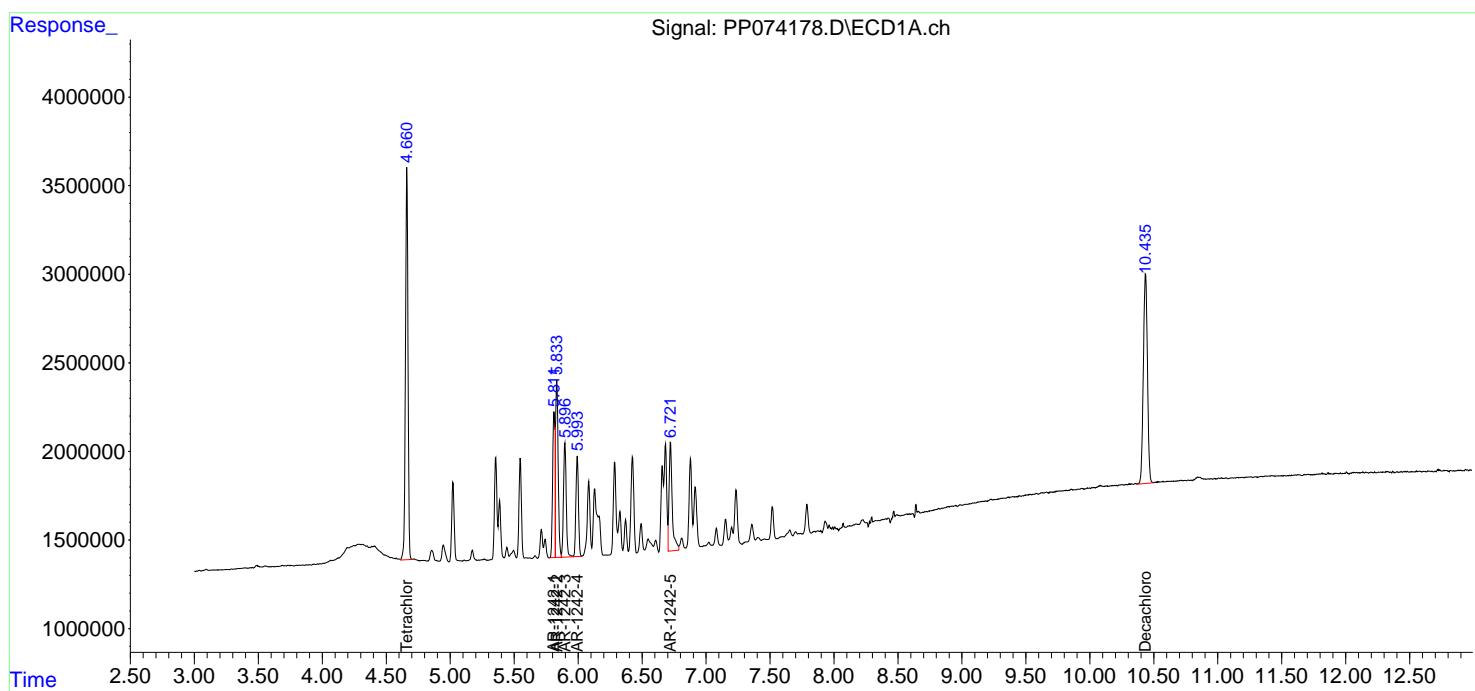

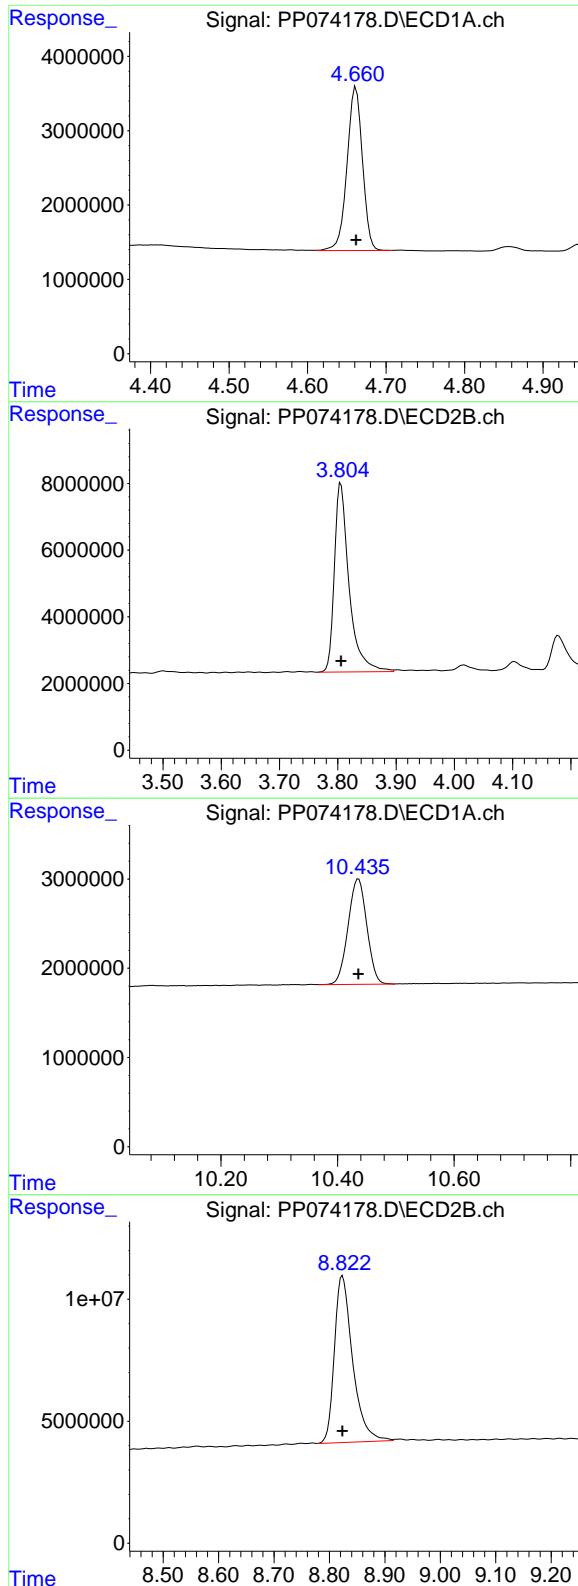

#1 Tetrachloro-m-xylene

R.T.: 4.662 min
Delta R.T.: 0.000 min
Response: 30064825
Conc: 27.00 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1242ICC250

#1 Tetrachloro-m-xylene


R.T.: 3.805 min
Delta R.T.: 0.000 min
Response: 99448361
Conc: 23.51 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.000 min
Response: 26416078
Conc: 27.51 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.824 min
Delta R.T.: 0.000 min
Response: 156351248
Conc: 25.04 ng/ml

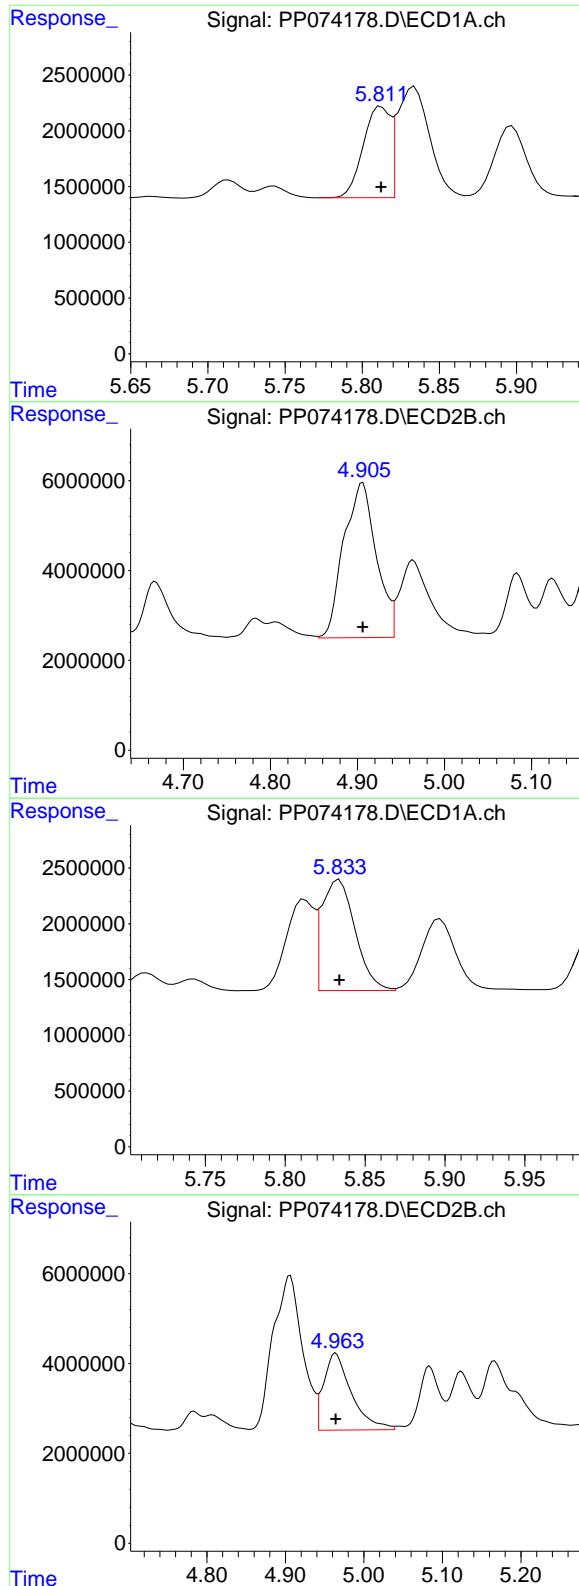

#16 AR-1242-1

R.T.: 5.812 min
 Delta R.T.: 0.000 min
 Response: 9924005
 Conc: 282.44 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC250

#16 AR-1242-1


R.T.: 4.906 min
 Delta R.T.: 0.000 min
 Response: 89565172
 Conc: 255.13 ng/ml

#17 AR-1242-2

R.T.: 5.834 min
 Delta R.T.: 0.000 min
 Response: 14472673
 Conc: 278.68 ng/ml

#17 AR-1242-2

R.T.: 4.964 min
 Delta R.T.: 0.000 min
 Response: 42174411
 Conc: 252.53 ng/ml

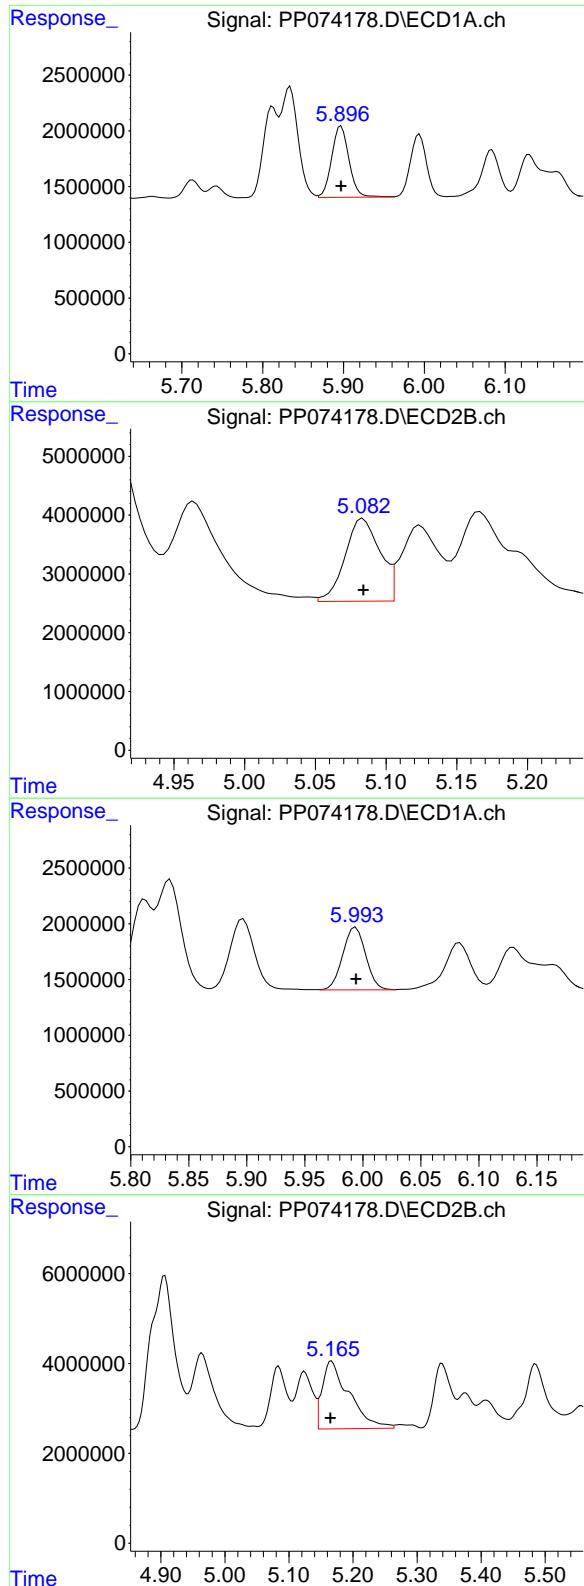

#18 AR-1242-3

R.T.: 5.897 min
 Delta R.T.: 0.000 min
 Response: 9547202
 Conc: 282.29 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC250

#18 AR-1242-3


R.T.: 5.084 min
 Delta R.T.: 0.000 min
 Response: 24305838
 Conc: 256.29 ng/ml

#19 AR-1242-4

R.T.: 5.994 min
 Delta R.T.: 0.000 min
 Response: 7737538
 Conc: 277.70 ng/ml

#19 AR-1242-4

R.T.: 5.166 min
 Delta R.T.: 0.001 min
 Response: 43979753
 Conc: 364.04 ng/ml

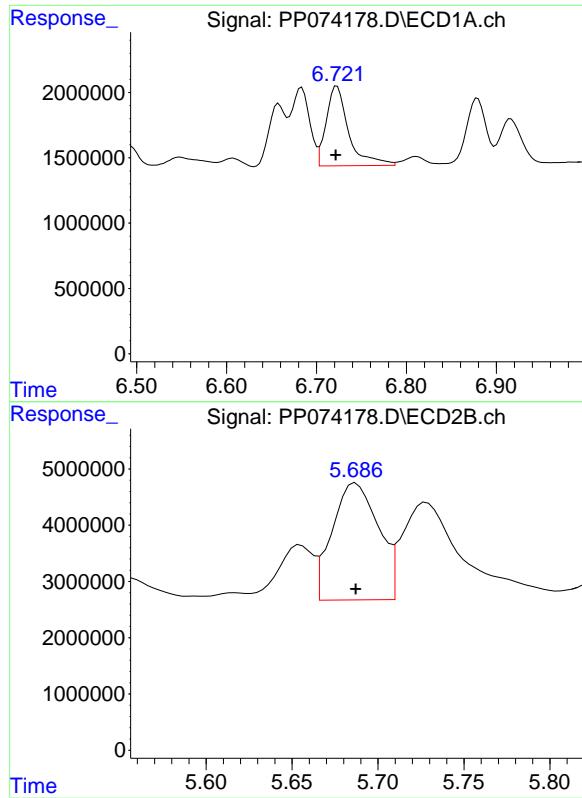

#20 AR-1242-5

R.T.: 6.723 min
Delta R.T.: 0.001 min
Response: 10585475
Conc: 316.93 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC250

#20 AR-1242-5

R.T.: 5.687 min
Delta R.T.: 0.000 min
Response: 38870481
Conc: 260.44 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074179.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 15:36
 Operator : YP\AJ
 Sample : AR1242ICC050
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 15:58:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 15:57:36 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|---------|----------|-------|---------|
| 1) SA Tetrachlor... | 4.659 | 3.803 | 6977861 | 15078408 | 5.999 | 3.762 # |
| 2) SA Decachlor... | 10.432 | 8.821 | 6026260 | 28194628 | 5.971 | 4.604 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|---------|----------|
| 16) L4 AR-1242-1 | 5.810 | 4.903 | 2289125 | 16072866 | 61.427 | 46.569 |
| 17) L4 AR-1242-2 | 5.832 | 4.962 | 3215660 | 7443347 | 59.102 | 45.559 |
| 18) L4 AR-1242-3 | 5.895 | 5.082 | 2169957 | 4094869 | 60.722 | 44.390 # |
| 19) L4 AR-1242-4 | 5.991 | 5.163 | 1732044 | 5803584 | 59.279 | 48.597 |
| 20) L4 AR-1242-5 | 6.722 | 5.686 | 3937933 | 7539678 | 102.119 | 50.412 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
Data File : PP074179.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2025 15:36
Operator : YP\AJ
Sample : AR1242ICC050
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1242ICC050

```
Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 01 15:58:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title  : GC EXTRACTABLES
QLast Update : Fri Aug 01 15:57:36 2025
Response via : Initial Calibration
Integrator: ChemStation
```

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

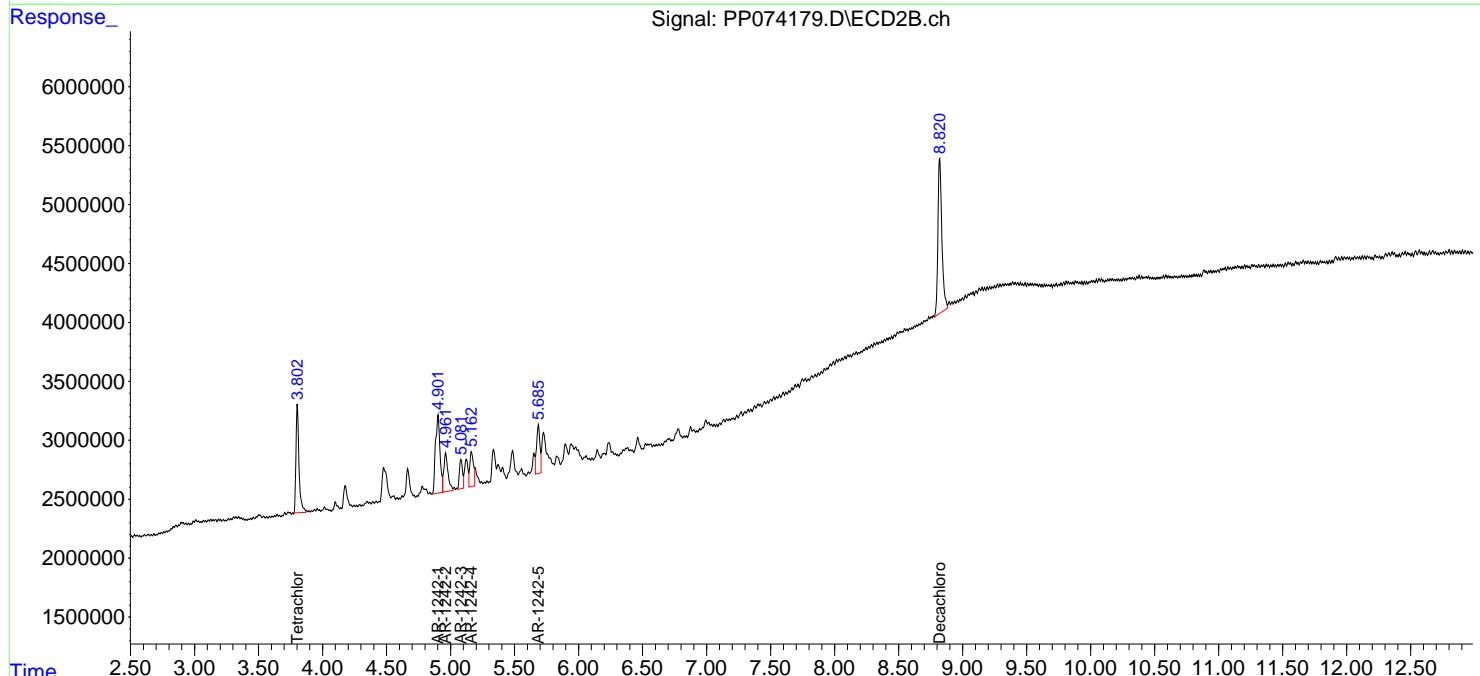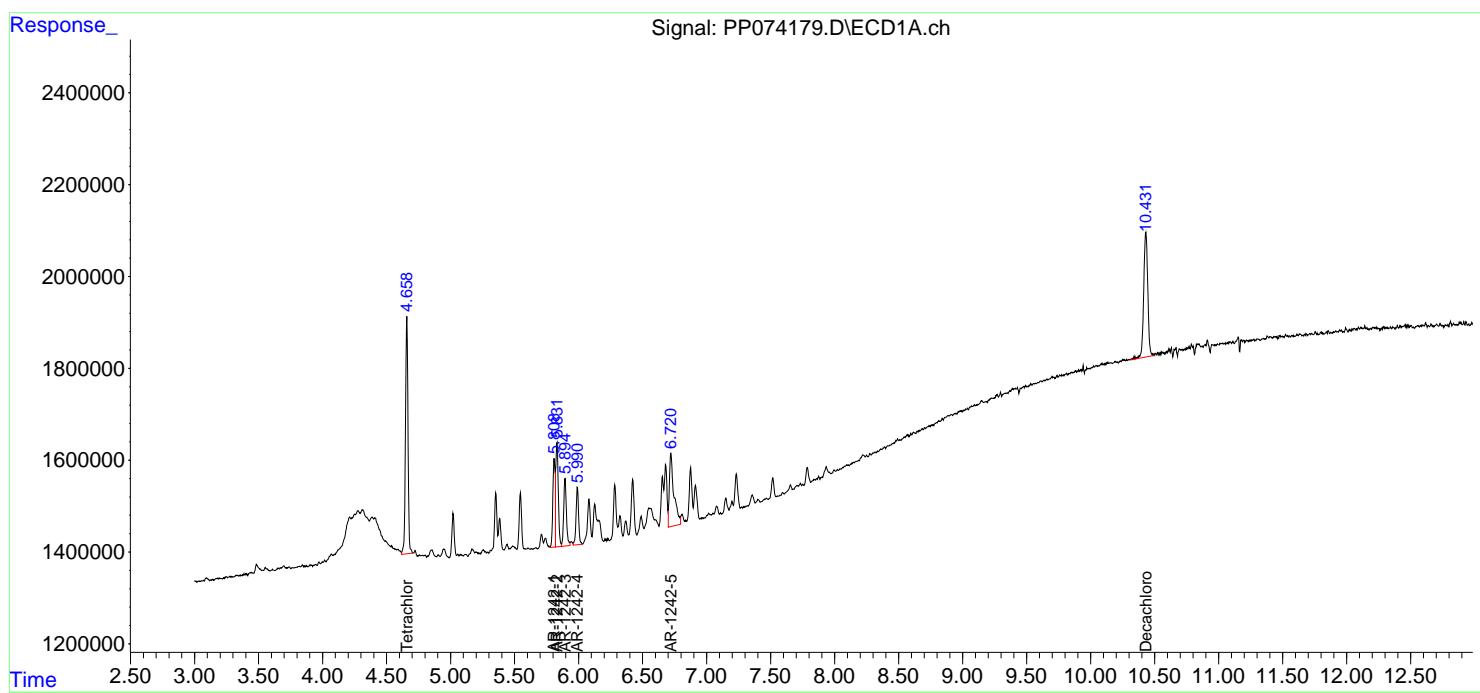

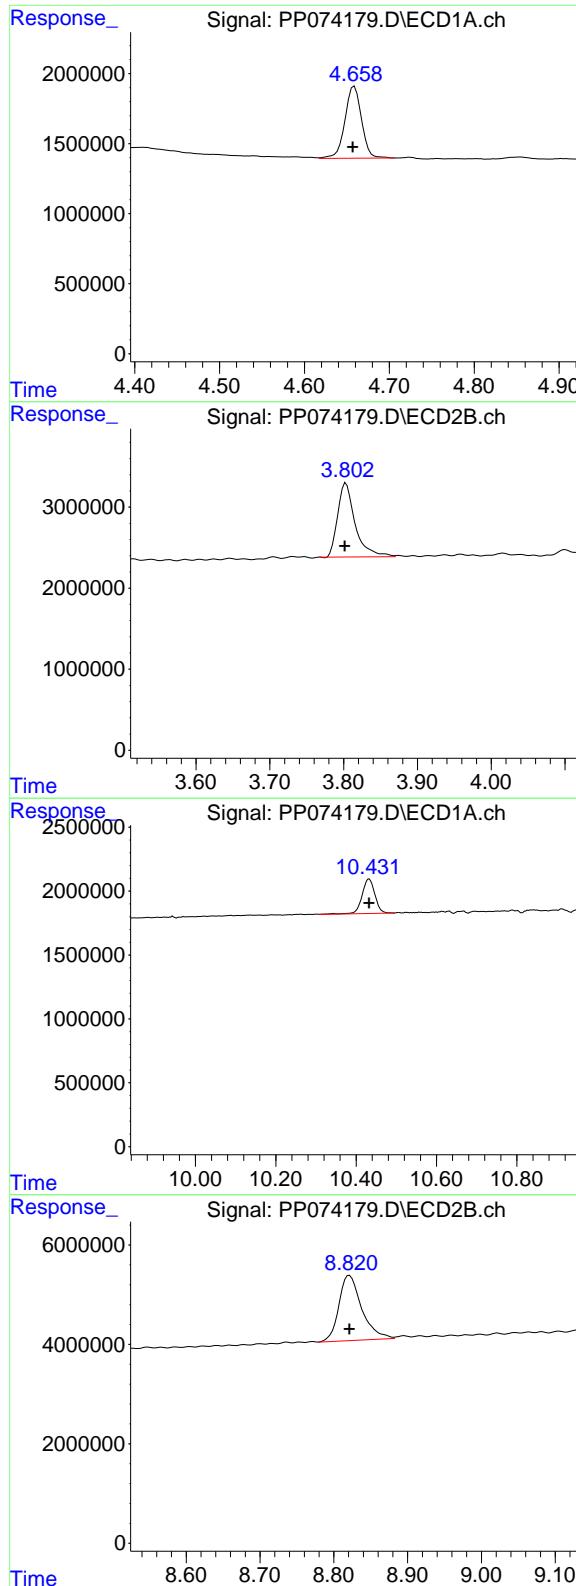

#1 Tetrachloro-m-xylene

R.T.: 4.659 min
 Delta R.T.: 0.002 min
 Response: 6977861
 Conc: 6.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC050

#1 Tetrachloro-m-xylene


R.T.: 3.803 min
 Delta R.T.: 0.001 min
 Response: 15078408
 Conc: 3.76 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.432 min
 Delta R.T.: 0.000 min
 Response: 6026260
 Conc: 5.97 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.821 min
 Delta R.T.: 0.000 min
 Response: 28194628
 Conc: 4.60 ng/ml

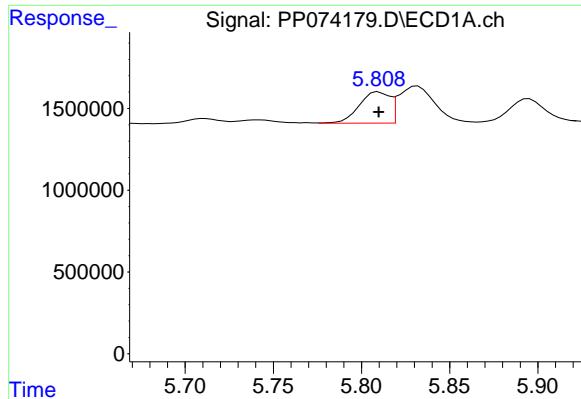

#16 AR-1242-1


R.T.: 5.810 min
Delta R.T.: 0.000 min
Response: 2289125
Conc: 61.43 ng/ml

Instrument: ECD_P
ClientSampleId: AR1242ICC050

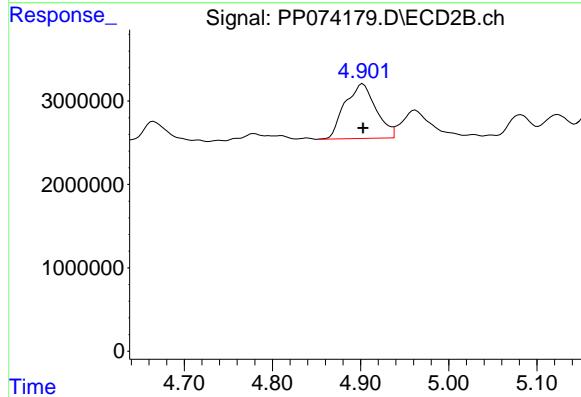


#16 AR-1242-1

R.T.: 4.903 min
Delta R.T.: 0.000 min
Response: 16072866
Conc: 46.57 ng/ml

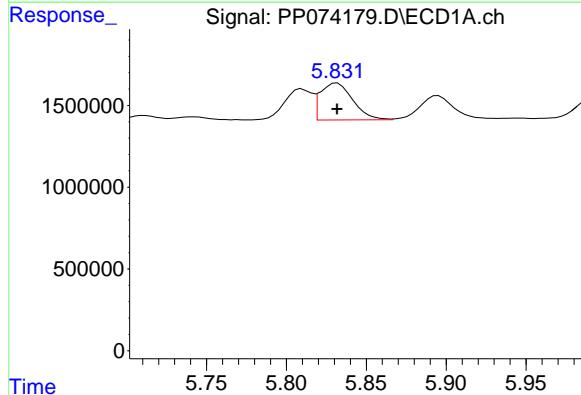


#17 AR-1242-2

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 3215660
Conc: 59.10 ng/ml

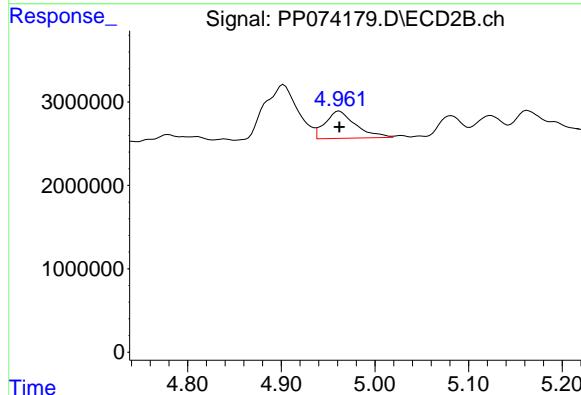

#17 AR-1242-2

R.T.: 4.962 min
Delta R.T.: 0.000 min
Response: 7443347
Conc: 45.56 ng/ml

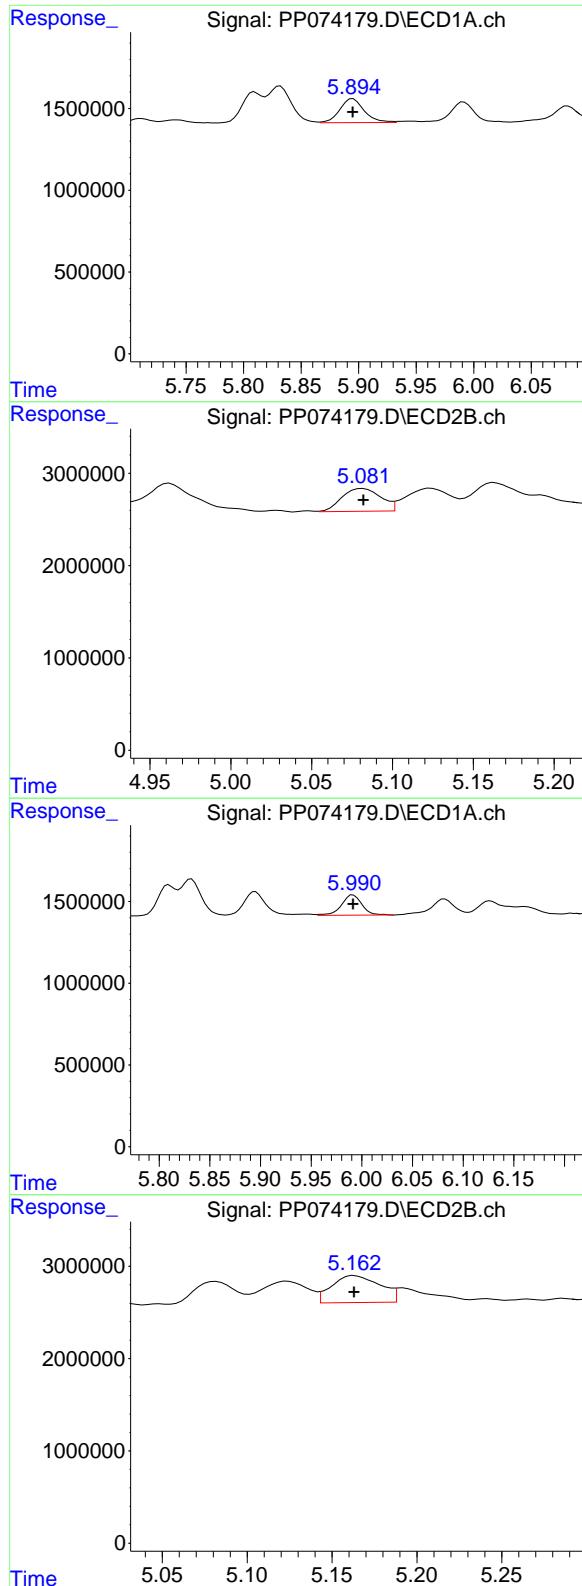

#18 AR-1242-3

R.T.: 5.895 min
 Delta R.T.: 0.000 min
 Response: 2169957
 Conc: 60.72 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC050

#18 AR-1242-3


R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 4094869
 Conc: 44.39 ng/ml

#19 AR-1242-4

R.T.: 5.991 min
 Delta R.T.: 0.000 min
 Response: 1732044
 Conc: 59.28 ng/ml

#19 AR-1242-4

R.T.: 5.163 min
 Delta R.T.: 0.000 min
 Response: 5803584
 Conc: 48.60 ng/ml

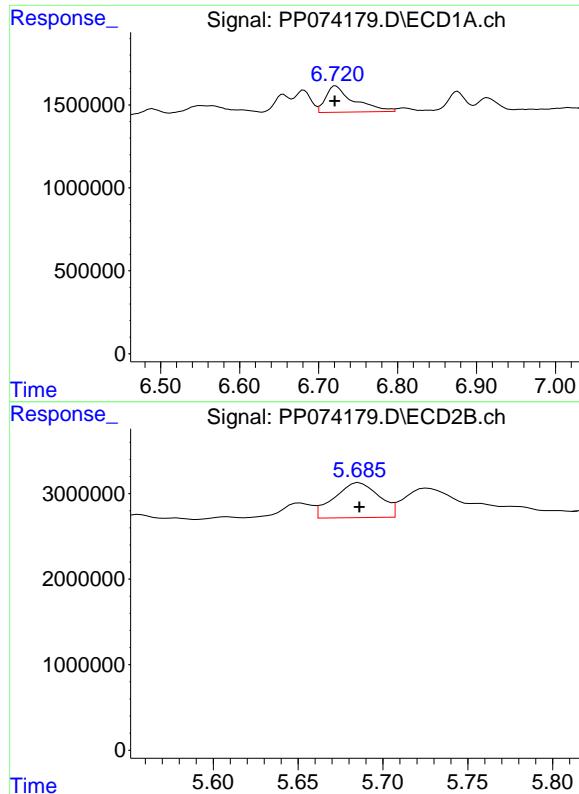

#20 AR-1242-5

R.T.: 6.722 min
 Delta R.T.: 0.001 min
 Response: 3937933
 Conc: 102.12 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1242ICC050

#20 AR-1242-5

R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 7539678
 Conc: 50.41 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 16:57
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 23:35:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 23:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.660 | 3.805 | 54922987 | 197.2E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.433 | 8.824 | 48401219 | 304.7E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|-----------|
| 21) L5 AR-1248-1 | 5.810 | 4.903 | 14191296 | 111.8E6 | 500.000 | 500.000 |
| 22) L5 AR-1248-2 | 6.082 | 5.124 | 20093773 | 73885161 | 500.000 | 500.000 |
| 23) L5 AR-1248-3 | 6.284 | 5.166 | 22320416 | 131.4E6 | 500.000 | 698.929 # |
| 24) L5 AR-1248-4 | 6.682 | 5.338 | 25791080 | 83528426 | 500.000 | 500.000 |
| 25) L5 AR-1248-5 | 6.721 | 5.727 | 26620059 | 151.4E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074182.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 16:57
 Operator : YP\AJ
 Sample : AR1248ICC500
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1248ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 01 23:35:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 01 23:33:57 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

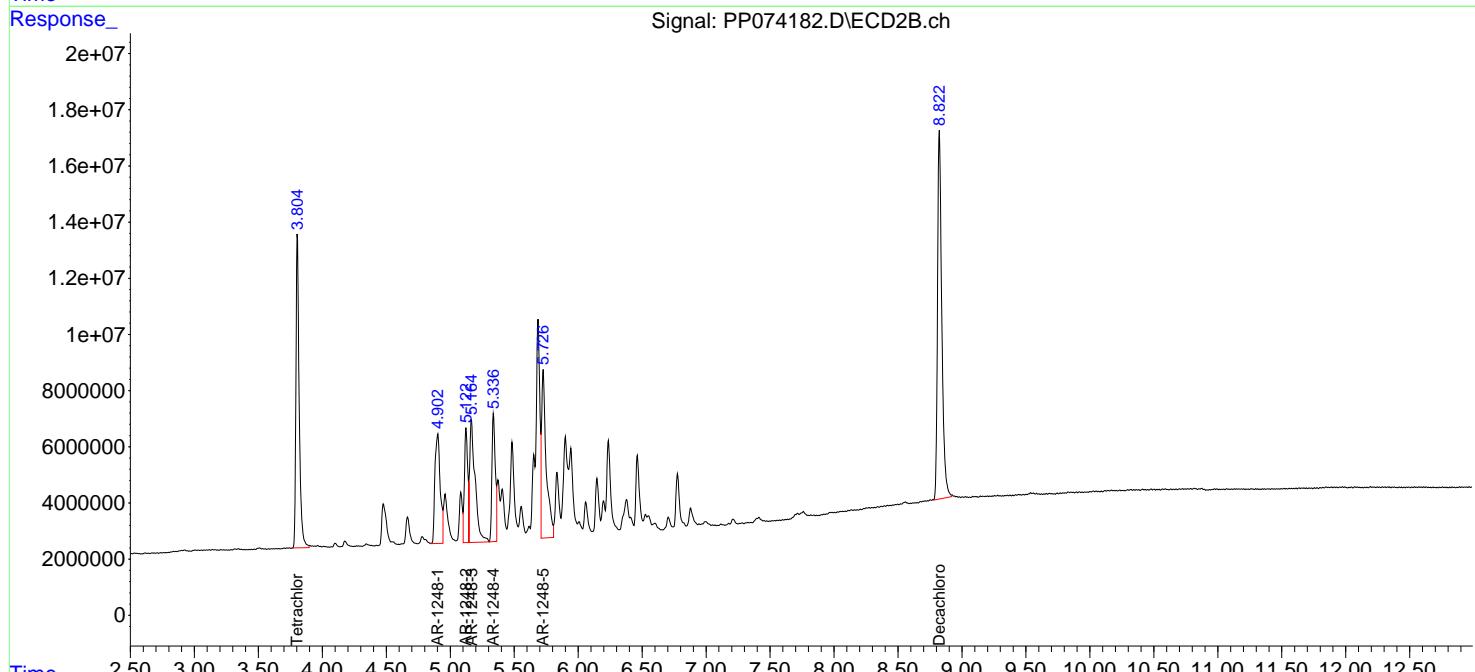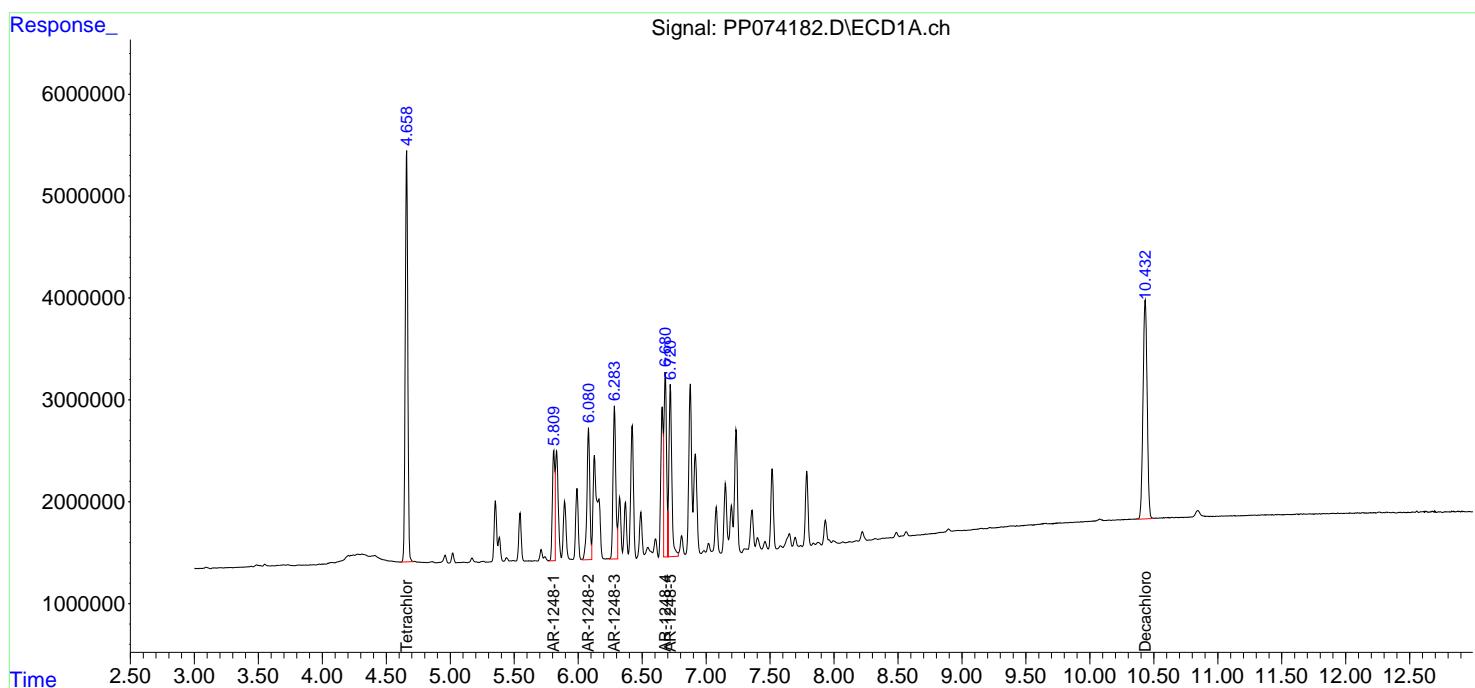

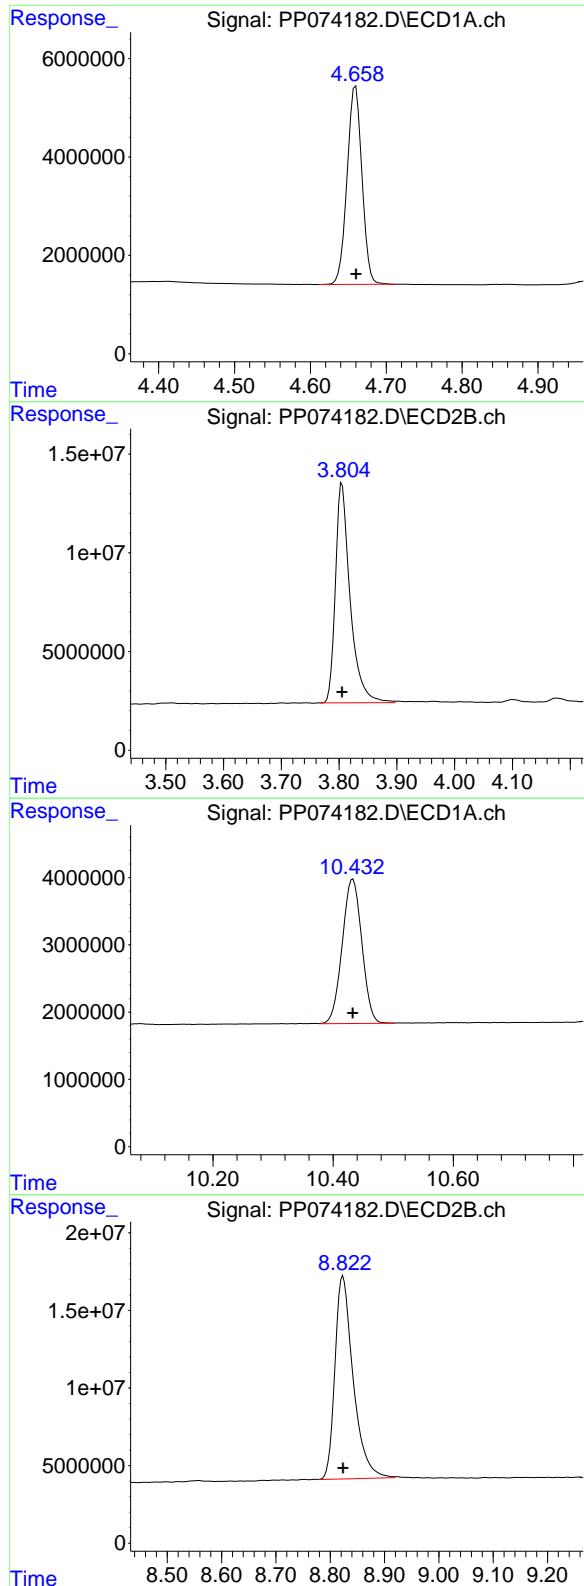

#1 Tetrachloro-m-xylene

R.T.: 4.660 min
 Delta R.T.: 0.000 min
 Response: 54922987
 Conc: 50.00 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1248ICC500

#1 Tetrachloro-m-xylene


R.T.: 3.805 min
 Delta R.T.: 0.000 min
 Response: 197242850
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.433 min
 Delta R.T.: 0.000 min
 Response: 48401219
 Conc: 50.00 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.824 min
 Delta R.T.: 0.000 min
 Response: 304735949
 Conc: 50.00 ng/ml

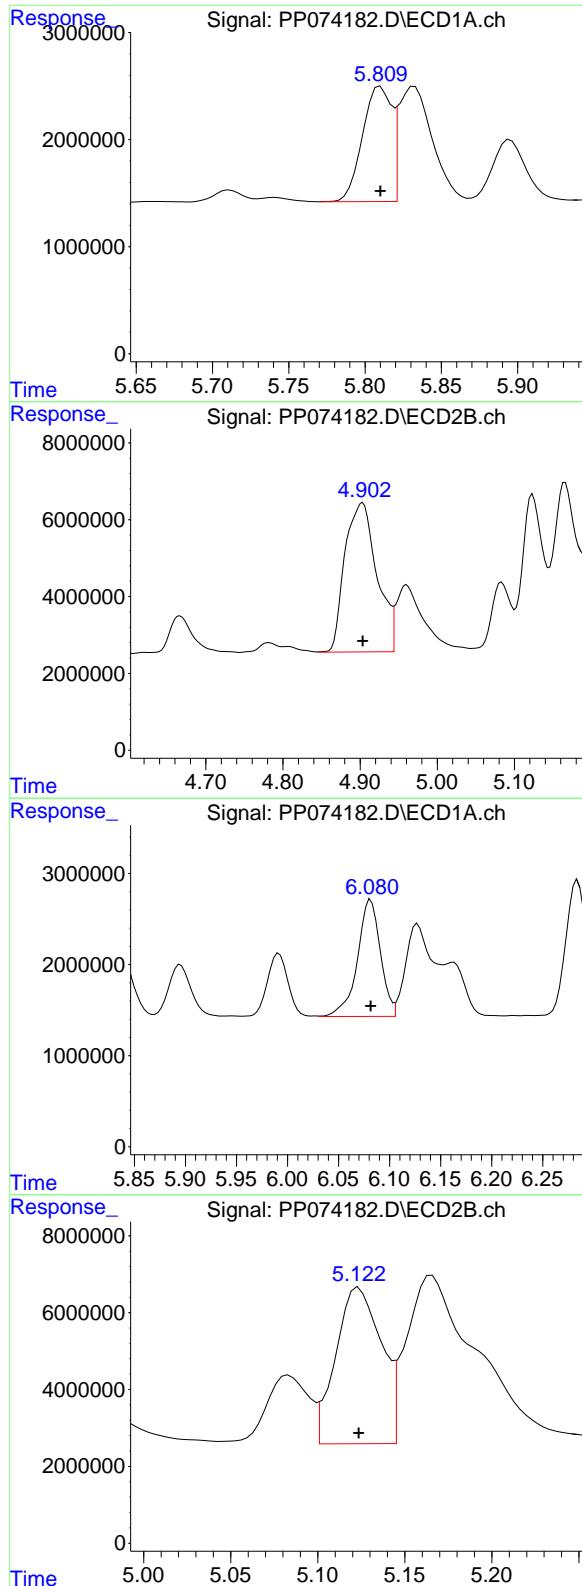

#21 AR-1248-1

R.T.: 5.810 min
 Delta R.T.: 0.000 min
 Response: 14191296
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC500

#21 AR-1248-1


R.T.: 4.903 min
 Delta R.T.: 0.000 min
 Response: 111814459
 Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 20093773
 Conc: 500.00 ng/ml

#22 AR-1248-2

R.T.: 5.124 min
 Delta R.T.: 0.000 min
 Response: 73885161
 Conc: 500.00 ng/ml

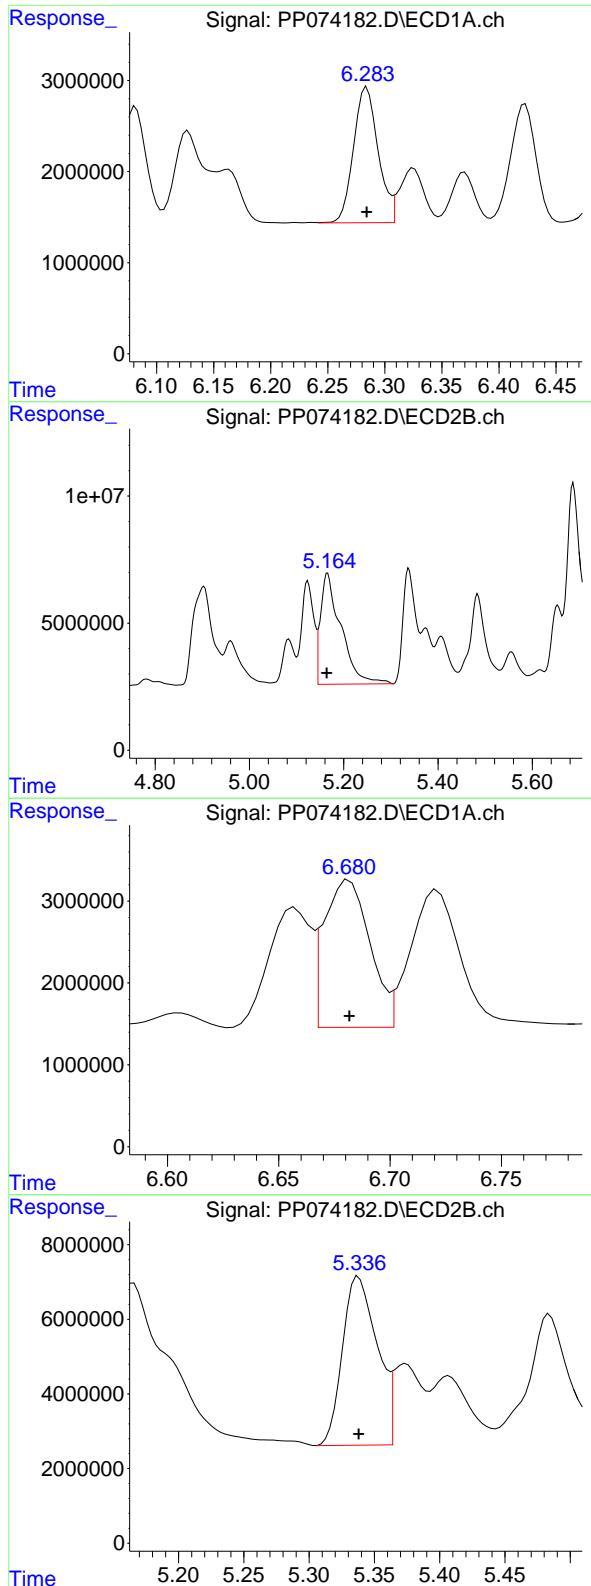

#23 AR-1248-3

R.T.: 6.284 min
 Delta R.T.: 0.000 min
 Response: 22320416
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC500

#23 AR-1248-3


R.T.: 5.166 min
 Delta R.T.: 0.002 min
 Response: 131449027
 Conc: 698.93 ng/ml

#24 AR-1248-4

R.T.: 6.682 min
 Delta R.T.: 0.000 min
 Response: 25791080
 Conc: 500.00 ng/ml

#24 AR-1248-4

R.T.: 5.338 min
 Delta R.T.: 0.000 min
 Response: 83528426
 Conc: 500.00 ng/ml

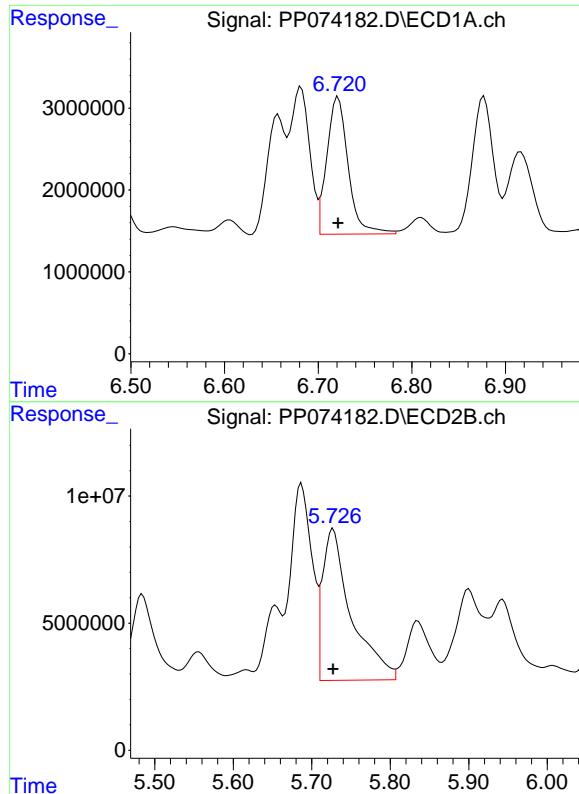

#25 AR-1248-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 26620059
 Conc: 500.00 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1248ICC500

#25 AR-1248-5

R.T.: 5.727 min
 Delta R.T.: 0.000 min
 Response: 151391354
 Conc: 500.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:02
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|---------|
| 1) SA Tetrachlor... | 4.660 | 3.805 | 105.5E6 | 435.9E6 | 94.708 | 107.891 |
| 2) SA Decachlor... | 10.433 | 8.824 | 90161394 | 620.7E6 | 92.084 | 101.439 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|------------|
| 26) L6 AR-1254-1 | 6.660 | 5.689 | 70203514 | 384.6E6 | 1294.709 | 998.639 |
| 27) L6 AR-1254-2 | 6.875 | 5.835 | 70079706 | 284.4E6 | 896.542 | 1000.895 |
| 28) L6 AR-1254-3 | 7.237 | 6.238 | 76495408 | 520.2E6 | 905.487 | 1022.453 |
| 29) L6 AR-1254-4 | 7.518 | 6.464 | 57834344 | 378.1E6 | 911.799 | 1002.531 |
| 30) L6 AR-1254-5 | 7.934 | 6.882 | 73335985 | 464.7E6 | 909.260 | 1166.896 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074185.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:02
 Operator : YP\AJ
 Sample : AR1254ICC1000
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC1000

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

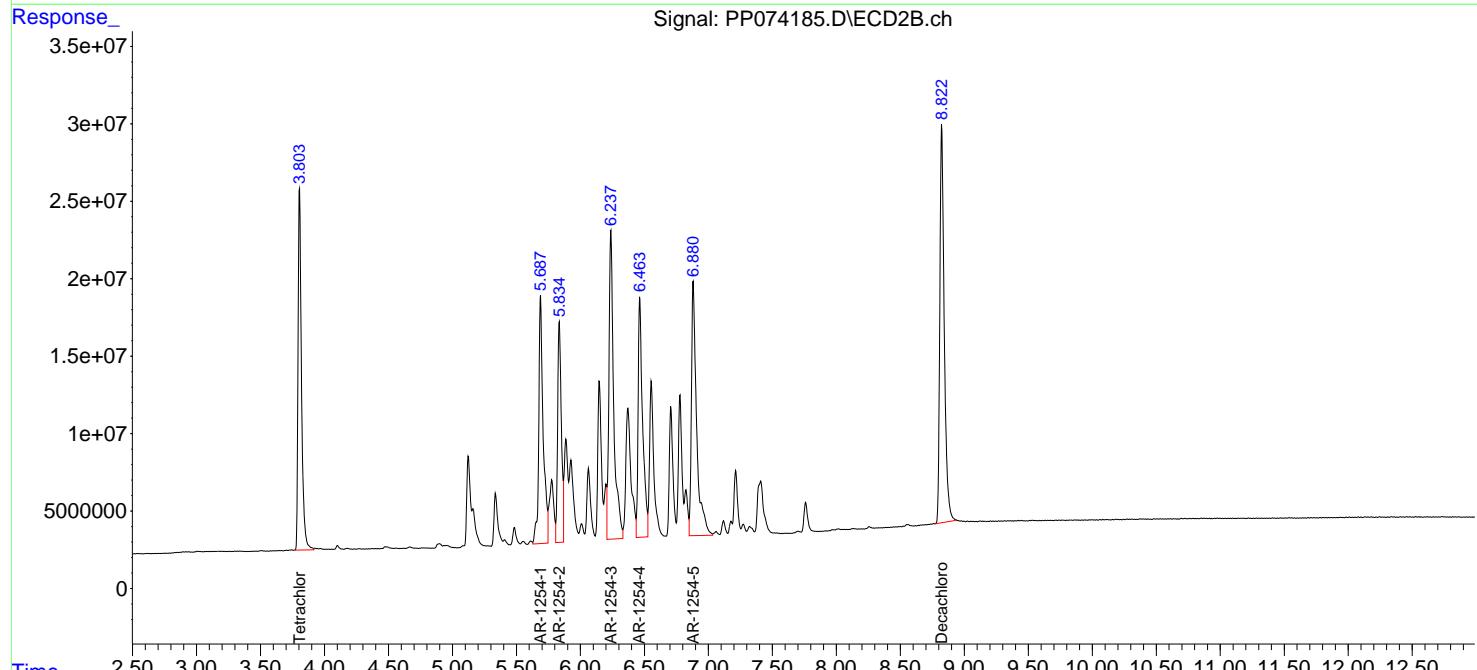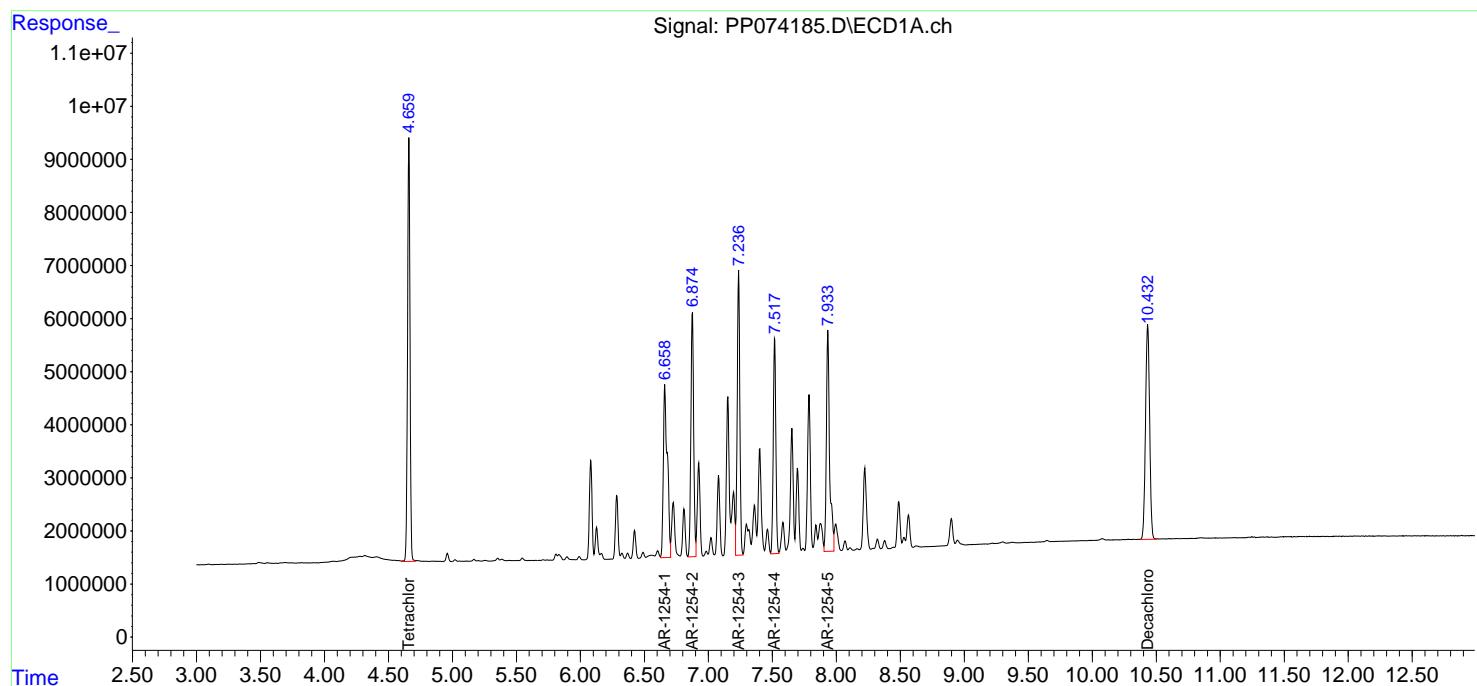

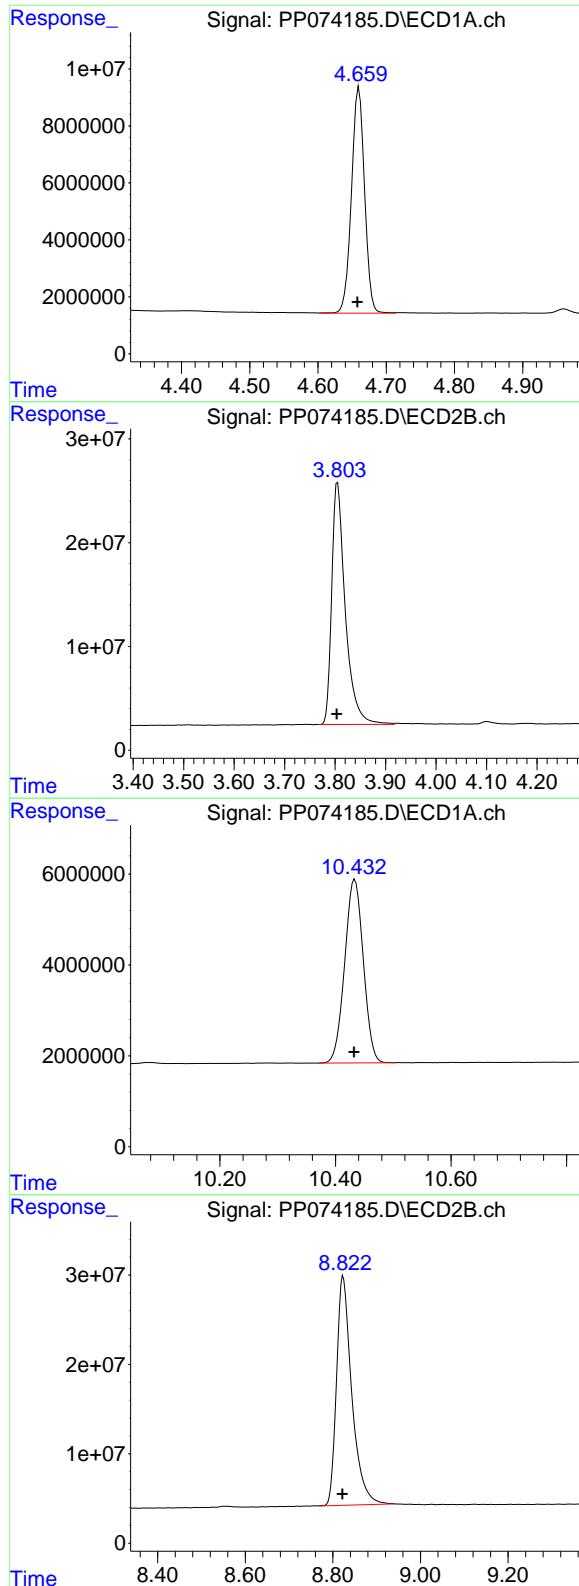

#1 Tetrachloro-m-xylene

R.T.: 4.660 min
 Delta R.T.: 0.002 min
 Response: 105531811
 Conc: 94.71 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1254ICC1000

#1 Tetrachloro-m-xylene


R.T.: 3.805 min
 Delta R.T.: 0.002 min
 Response: 435882815
 Conc: 107.89 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.433 min
 Delta R.T.: 0.001 min
 Response: 90161394
 Conc: 92.08 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.824 min
 Delta R.T.: 0.002 min
 Response: 620683272
 Conc: 101.44 ng/ml

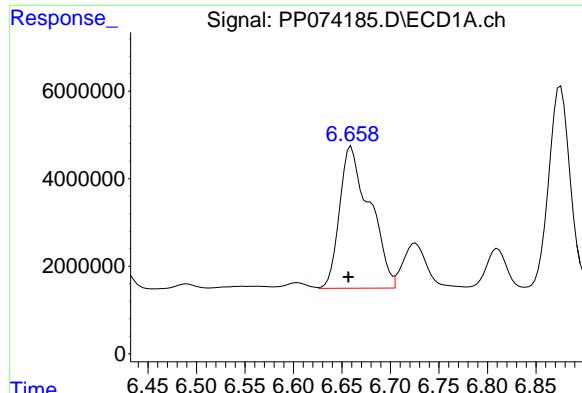

#26 AR-1254-1


R.T.: 6.660 min
 Delta R.T.: 0.003 min
 Response: 70203514
 Conc: 1294.71 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC1000

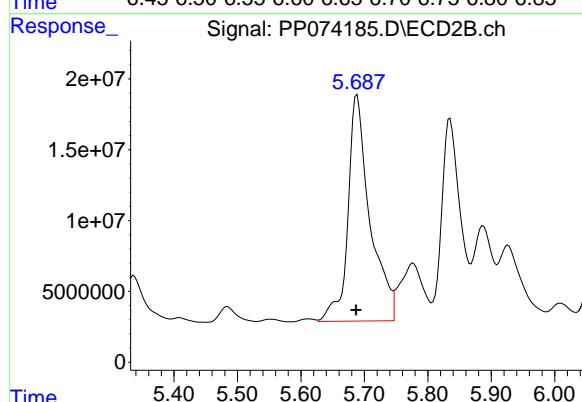


#26 AR-1254-1

R.T.: 5.689 min
 Delta R.T.: 0.001 min
 Response: 384557283
 Conc: 998.64 ng/ml

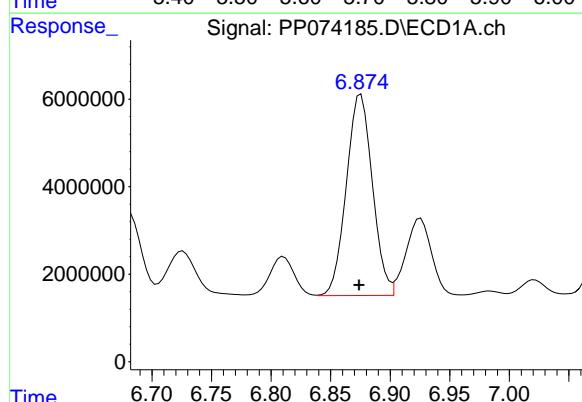


#27 AR-1254-2

R.T.: 6.875 min
 Delta R.T.: 0.002 min
 Response: 70079706
 Conc: 896.54 ng/ml

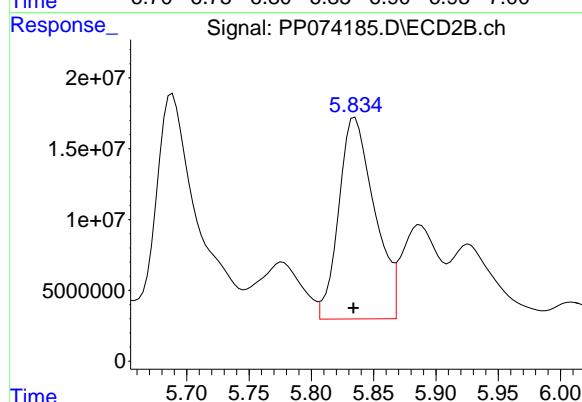

#27 AR-1254-2


R.T.: 5.835 min
 Delta R.T.: 0.001 min
 Response: 284389782
 Conc: 1000.89 ng/ml



#28 AR-1254-3


R.T.: 7.237 min
 Delta R.T.: 0.002 min
 Response: 76495408
 Conc: 905.49 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC1000

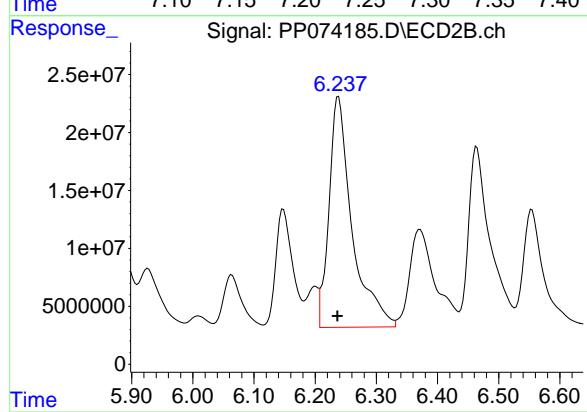


#28 AR-1254-3

R.T.: 6.238 min
 Delta R.T.: 0.002 min
 Response: 520239168
 Conc: 1022.45 ng/ml




#29 AR-1254-4

R.T.: 7.518 min
 Delta R.T.: 0.001 min
 Response: 57834344
 Conc: 911.80 ng/ml

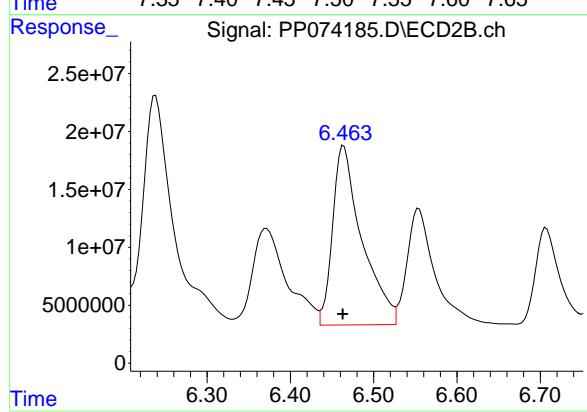

#29 AR-1254-4


R.T.: 6.464 min
 Delta R.T.: 0.001 min
 Response: 378053305
 Conc: 1002.53 ng/ml



#30 AR-1254-5

R.T.: 7.934 min
Delta R.T.: 0.002 min
Response: 73335985
Conc: 909.26 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC1000

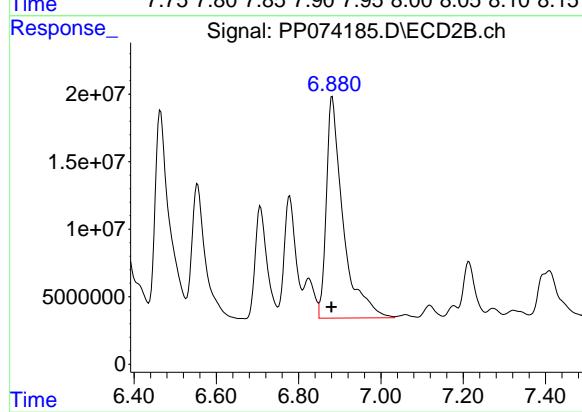

#30 AR-1254-5

R.T.: 6.882 min
Delta R.T.: 0.002 min
Response: 464689213
Conc: 1166.90 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:18
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.659 | 3.804 | 80274871 | 316.5E6 | 72.041 | 78.350 |
| 2) SA Decachlor... | 10.433 | 8.823 | 69679431 | 463.5E6 | 71.165 | 75.743 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|----------|-----------|
| 26) L6 AR-1254-1 | 6.658 | 5.688 | 55036391 | 271.1E6 | 1014.994 | 703.976 # |
| 27) L6 AR-1254-2 | 6.874 | 5.835 | 54514978 | 207.5E6 | 697.420 | 730.114 |
| 28) L6 AR-1254-3 | 7.236 | 6.237 | 59505451 | 390.5E6 | 704.374 | 767.509 |
| 29) L6 AR-1254-4 | 7.517 | 6.464 | 44944937 | 292.2E6 | 708.589 | 774.901 |
| 30) L6 AR-1254-5 | 7.933 | 6.881 | 57058661 | 308.2E6 | 707.445 | 773.995 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074186.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:18
 Operator : YP\AJ
 Sample : AR1254ICC750
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

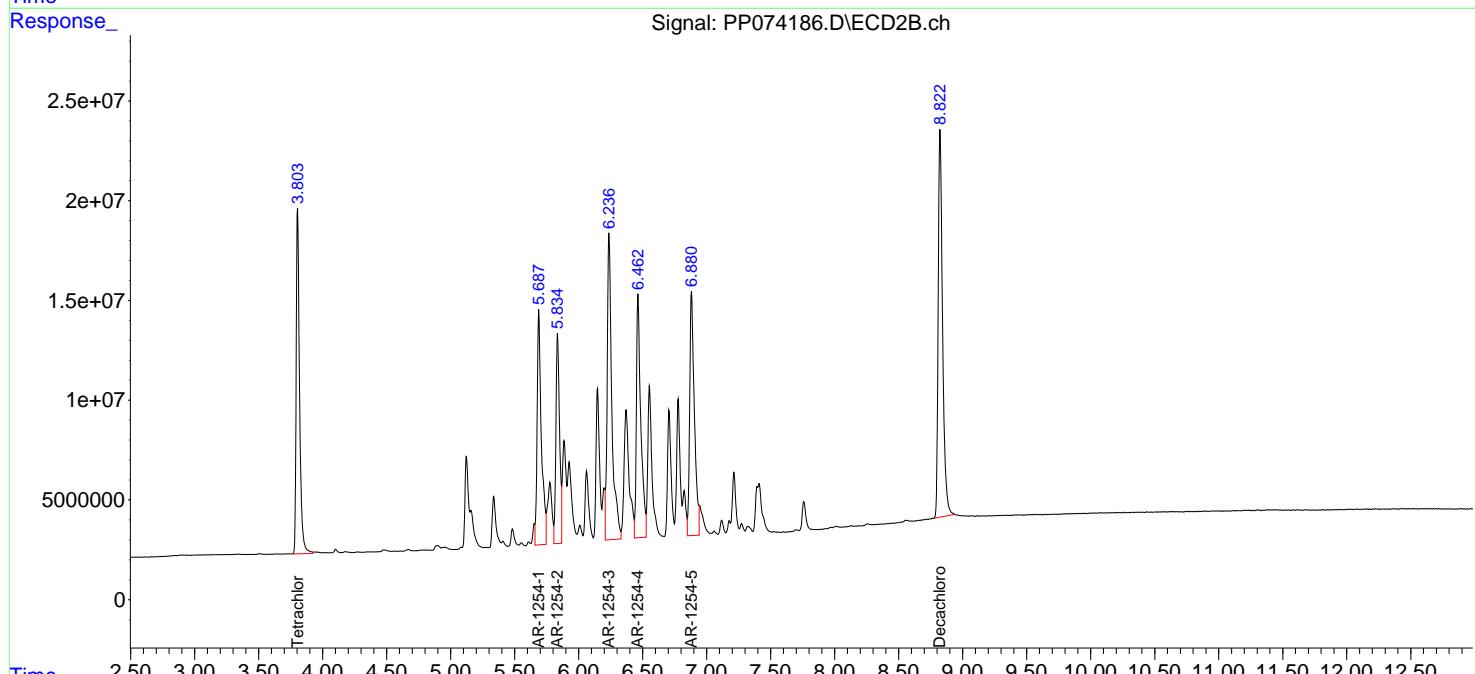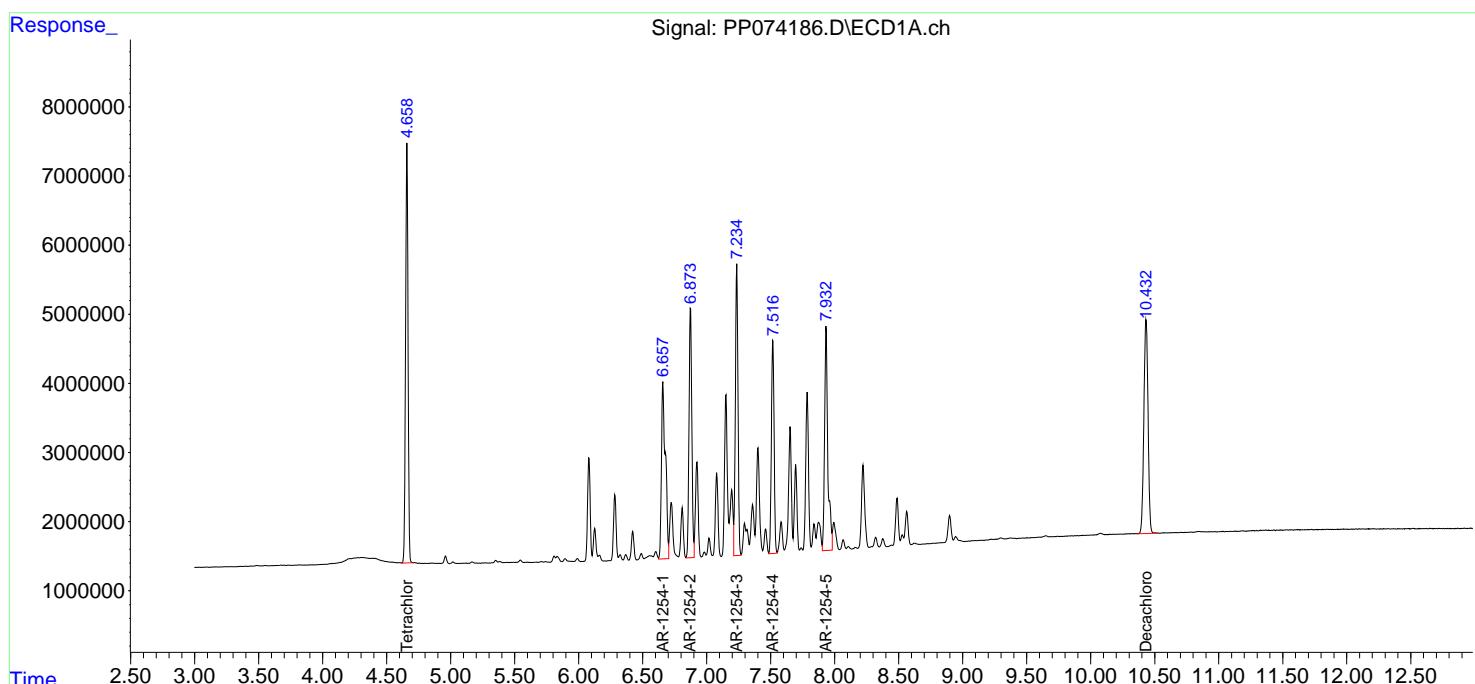

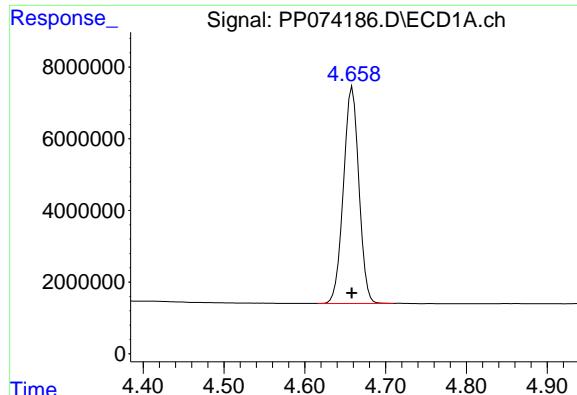

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 80274871
Conc: 72.04 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1254ICC750

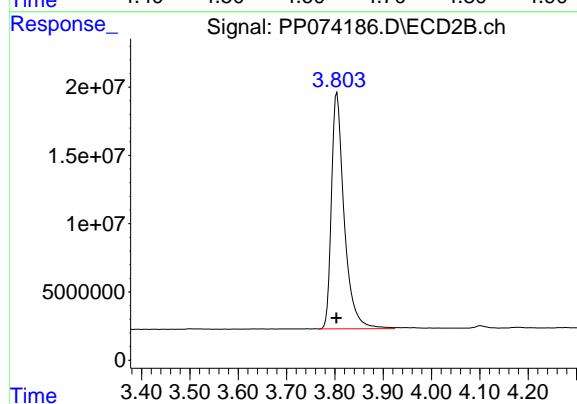


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.001 min
Response: 316536494
Conc: 78.35 ng/ml

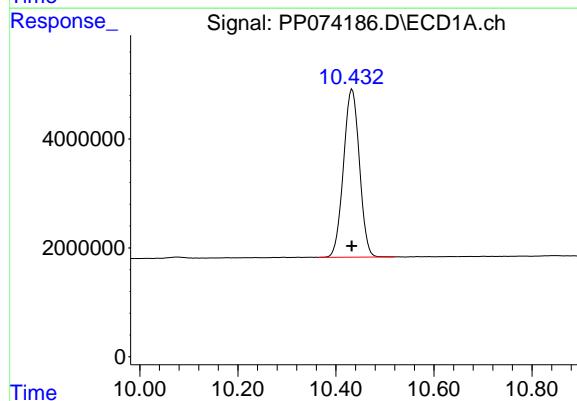


#2 Decachlorobiphenyl

R.T.: 10.433 min
Delta R.T.: 0.000 min
Response: 69679431
Conc: 71.17 ng/ml

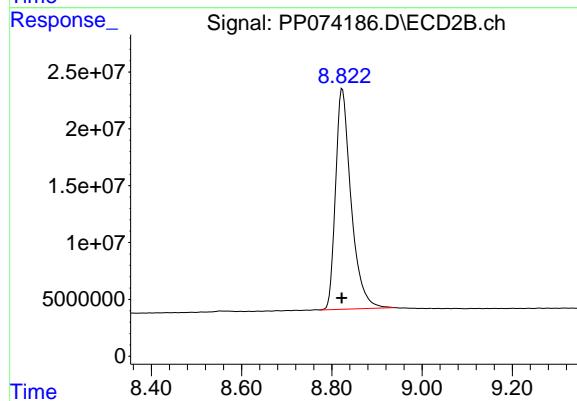

#2 Decachlorobiphenyl


R.T.: 8.823 min
Delta R.T.: 0.001 min
Response: 463453835
Conc: 75.74 ng/ml

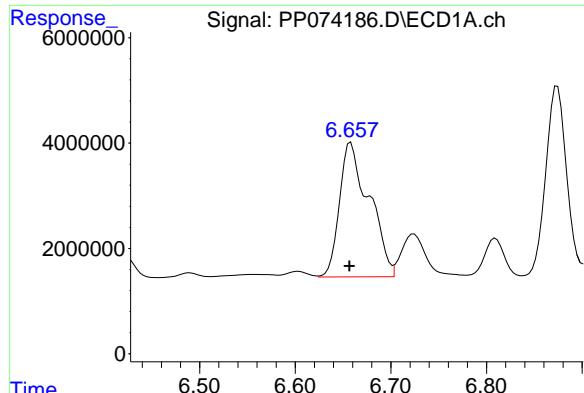

#26 AR-1254-1


R.T.: 6.658 min
Delta R.T.: 0.001 min
Response: 55036391
Conc: 1014.99 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC750

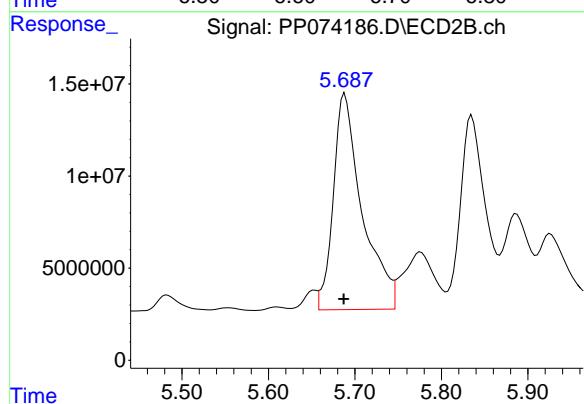


#26 AR-1254-1

R.T.: 5.688 min
Delta R.T.: 0.001 min
Response: 271087969
Conc: 703.98 ng/ml

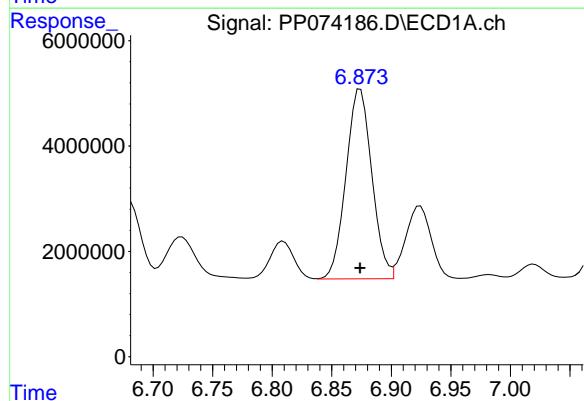


#27 AR-1254-2

R.T.: 6.874 min
Delta R.T.: 0.000 min
Response: 54514978
Conc: 697.42 ng/ml

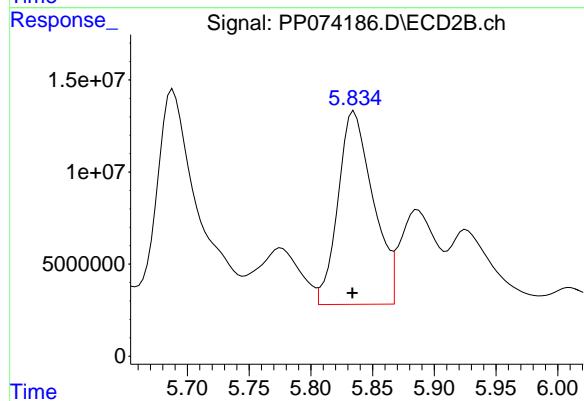

#27 AR-1254-2

R.T.: 5.835 min
Delta R.T.: 0.001 min
Response: 207451389
Conc: 730.11 ng/ml

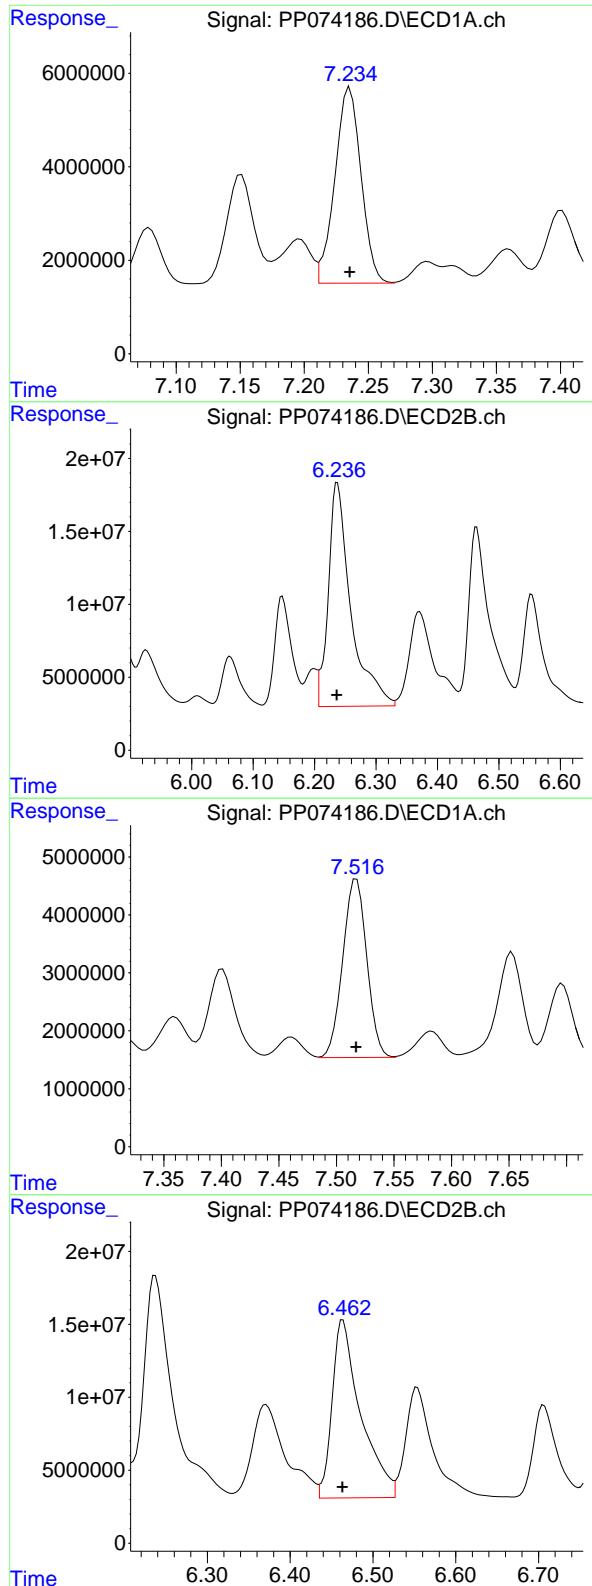

#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: 0.000 min
 Response: 59505451
 Conc: 704.37 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC750

#28 AR-1254-3


R.T.: 6.237 min
 Delta R.T.: 0.000 min
 Response: 390519824
 Conc: 767.51 ng/ml

#29 AR-1254-4

R.T.: 7.517 min
 Delta R.T.: 0.000 min
 Response: 44944937
 Conc: 708.59 ng/ml

#29 AR-1254-4

R.T.: 6.464 min
 Delta R.T.: 0.000 min
 Response: 292214490
 Conc: 774.90 ng/ml

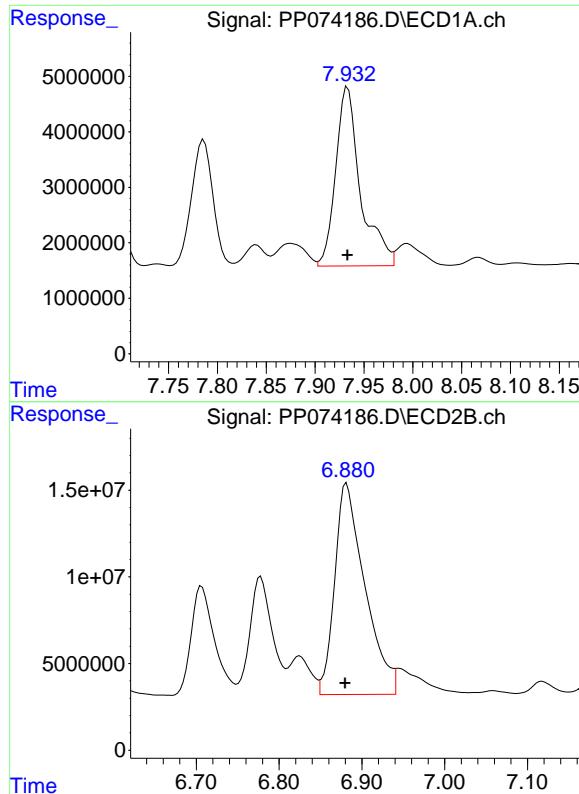

#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 57058661 ECD_P
 Conc: 707.44 ng/ml **ClientSampleId:**
 AR1254ICC750

#30 AR-1254-5

R.T.: 6.881 min
 Delta R.T.: 0.002 min
 Response: 308225641
 Conc: 774.00 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:34
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 55714538 | 202.0E6 | 50.000 | 50.000 |
| 2) SA Decachlor... | 10.432 | 8.822 | 48956102 | 305.9E6 | 50.000 | 50.000 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|---------|---------|-----------|
| 26) L6 AR-1254-1 | 6.658 | 5.687 | 39387303 | 192.5E6 | 726.390 | 500.000 # |
| 27) L6 AR-1254-2 | 6.874 | 5.834 | 39083346 | 142.1E6 | 500.000 | 500.000 |
| 28) L6 AR-1254-3 | 7.236 | 6.237 | 42239930 | 254.4E6 | 500.000 | 500.000 |
| 29) L6 AR-1254-4 | 7.517 | 6.463 | 31714402 | 188.5E6 | 500.000 | 500.000 |
| 30) L6 AR-1254-5 | 7.933 | 6.880 | 40327283 | 199.1E6 | 500.000 | 500.000 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074187.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:34
 Operator : YP\AJ
 Sample : AR1254ICC500
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

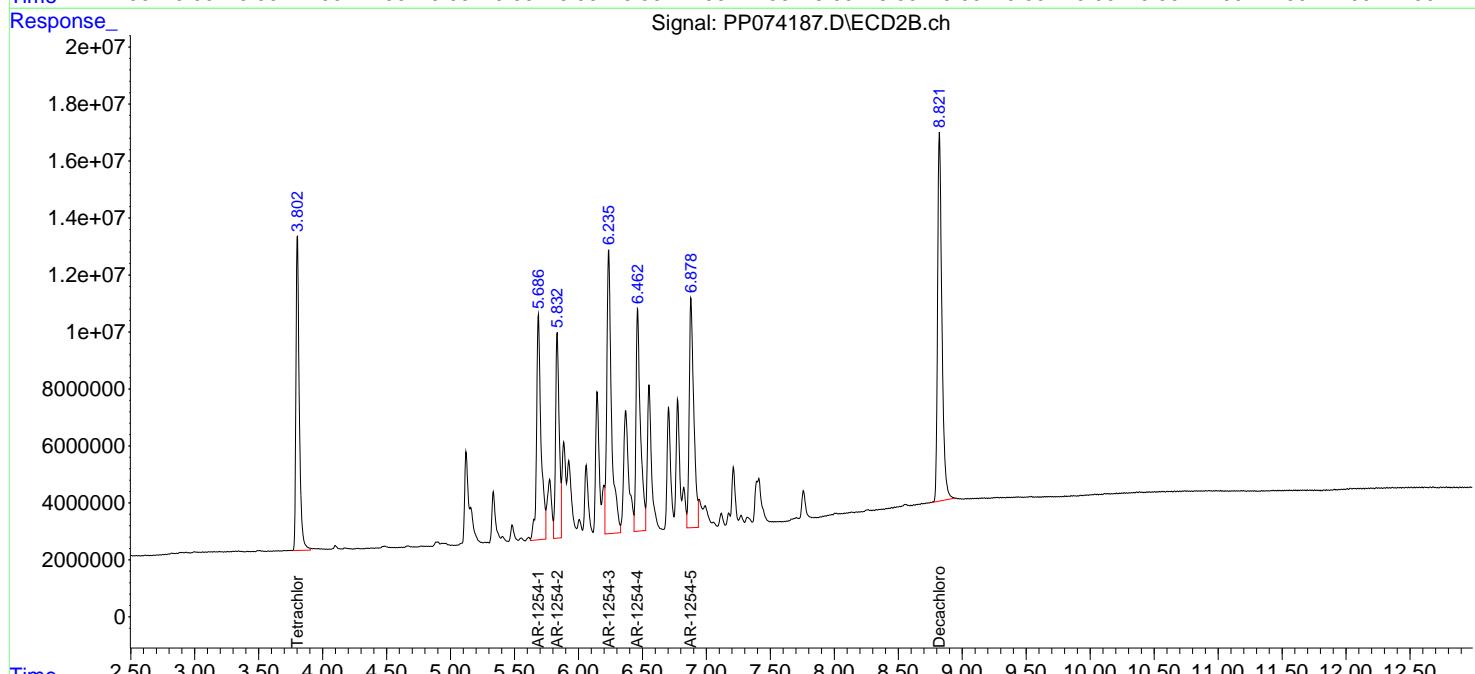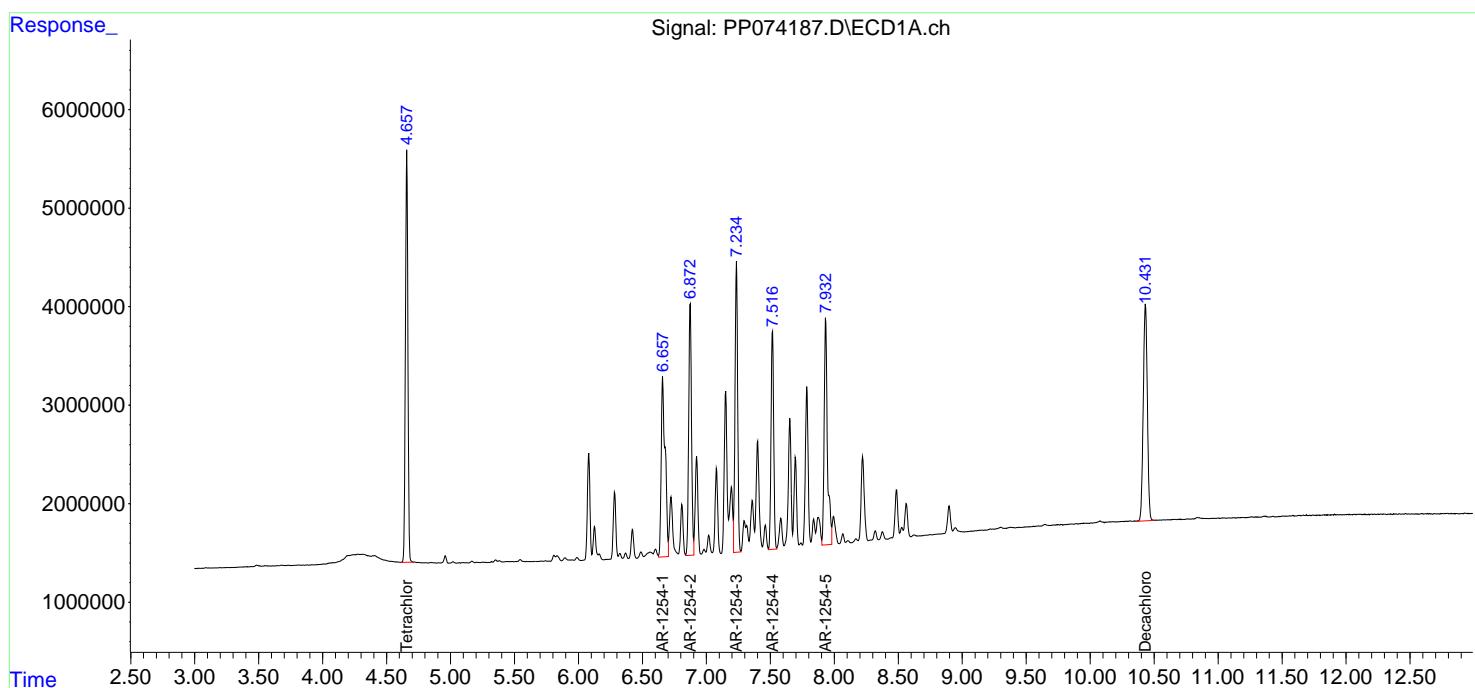



#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: 0.000 min
Response: 55714538
Conc: 50.00 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1254ICC500

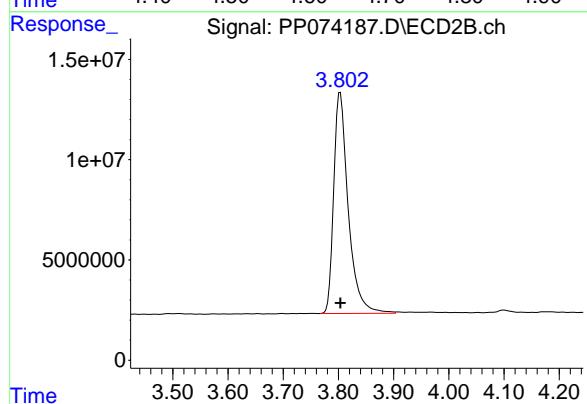


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 202001814
Conc: 50.00 ng/ml

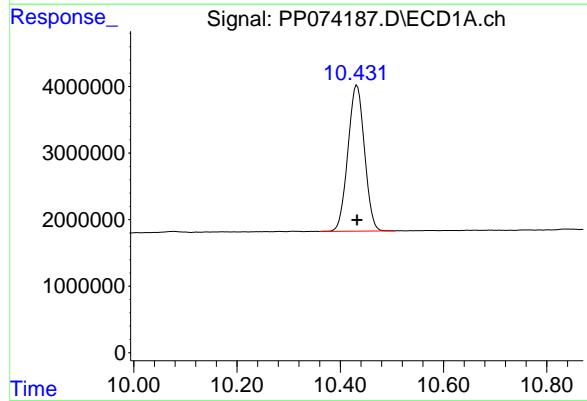


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.000 min
Response: 48956102
Conc: 50.00 ng/ml

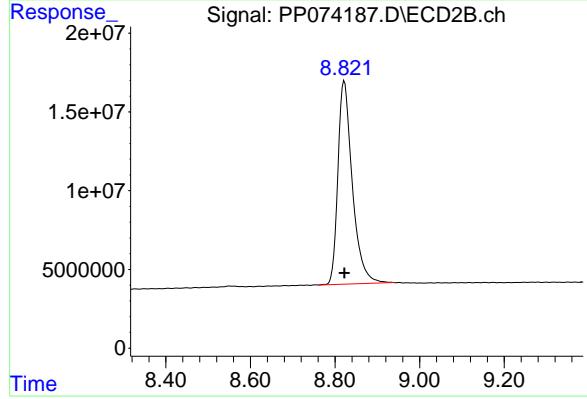

#2 Decachlorobiphenyl


R.T.: 8.822 min
Delta R.T.: 0.000 min
Response: 305938523
Conc: 50.00 ng/ml

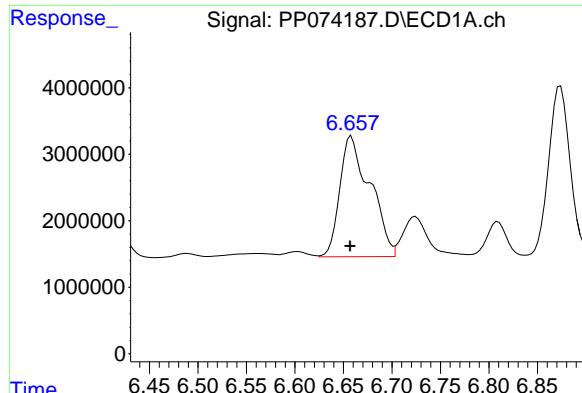

#26 AR-1254-1


R.T.: 6.658 min
 Delta R.T.: 0.001 min
 Response: 39387303
 Conc: 726.39 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC500

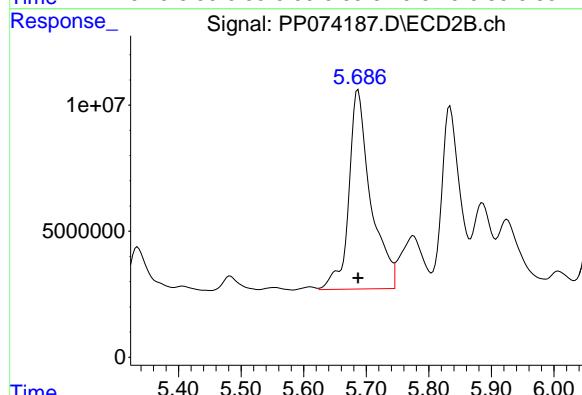


#26 AR-1254-1

R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 192540601
 Conc: 500.00 ng/ml

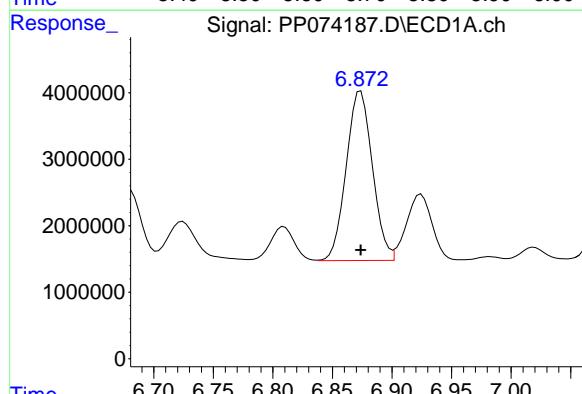


#27 AR-1254-2

R.T.: 6.874 min
 Delta R.T.: 0.000 min
 Response: 39083346
 Conc: 500.00 ng/ml

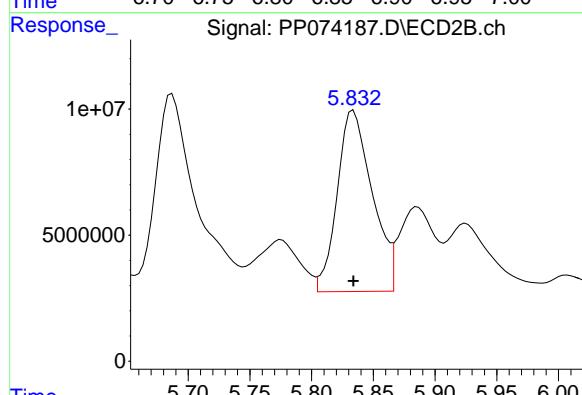

#27 AR-1254-2


R.T.: 5.834 min
 Delta R.T.: 0.000 min
 Response: 142067796
 Conc: 500.00 ng/ml



#28 AR-1254-3


R.T.: 7.236 min
 Delta R.T.: 0.000 min
 Response: 42239930
 Conc: 500.00 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC500

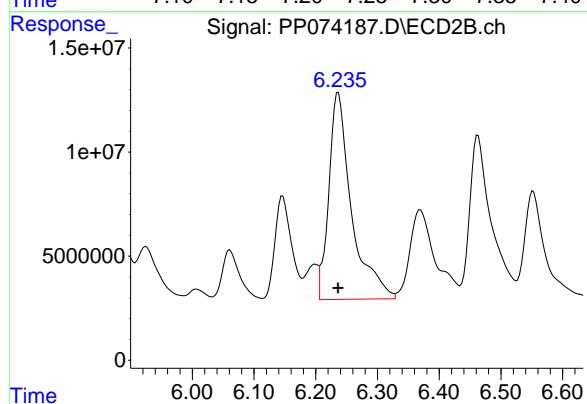


#28 AR-1254-3

R.T.: 6.237 min
 Delta R.T.: 0.000 min
 Response: 254407378
 Conc: 500.00 ng/ml

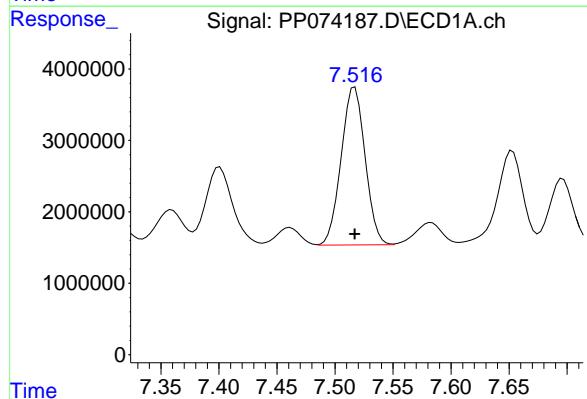


#29 AR-1254-4

R.T.: 7.517 min
 Delta R.T.: 0.000 min
 Response: 31714402
 Conc: 500.00 ng/ml

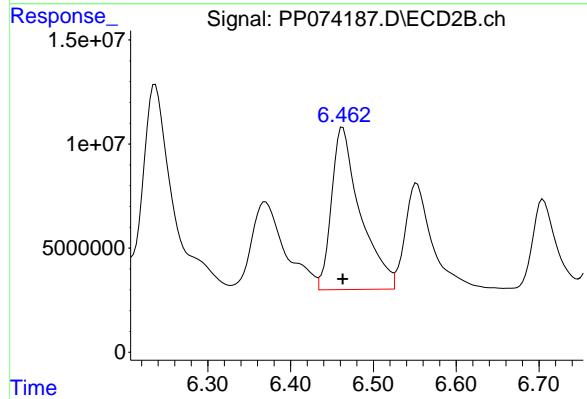

#29 AR-1254-4

R.T.: 6.463 min
 Delta R.T.: 0.000 min
 Response: 188549489
 Conc: 500.00 ng/ml

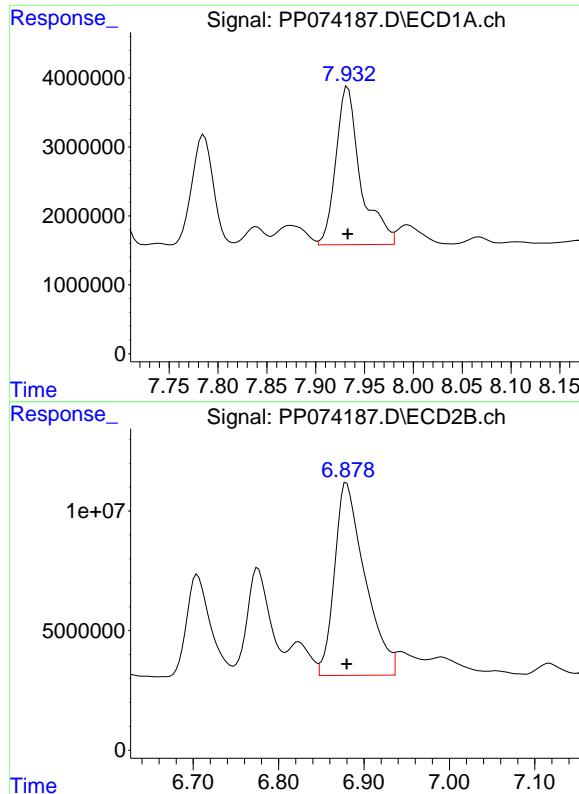

#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 40327283 ECD_P
 Conc: 500.00 ng/ml **ClientSampleId:**
 AR1254ICC500

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:50
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.658 | 3.803 | 29734018 | 92012238 | 26.684 | 22.775 |
| 2) SA Decachlor... | 10.431 | 8.821 | 26431747 | 157.0E6 | 26.995 | 25.657 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|---------|-----------|
| 26) L6 AR-1254-1 | 6.657 | 5.687 | 21966850 | 94373679 | 405.118 | 245.075 # |
| 27) L6 AR-1254-2 | 6.873 | 5.834 | 21644264 | 72682229 | 276.899 | 255.801 |
| 28) L6 AR-1254-3 | 7.235 | 6.236 | 23355124 | 131.7E6 | 276.458 | 258.769 |
| 29) L6 AR-1254-4 | 7.516 | 6.462 | 17399794 | 98587777 | 274.320 | 261.437 |
| 30) L6 AR-1254-5 | 7.932 | 6.879 | 22010158 | 98393861 | 272.894 | 247.080 |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 18:50
 Operator : YP\AJ
 Sample : AR1254ICC250
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 AR1254ICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 00:47:59 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 00:46:23 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

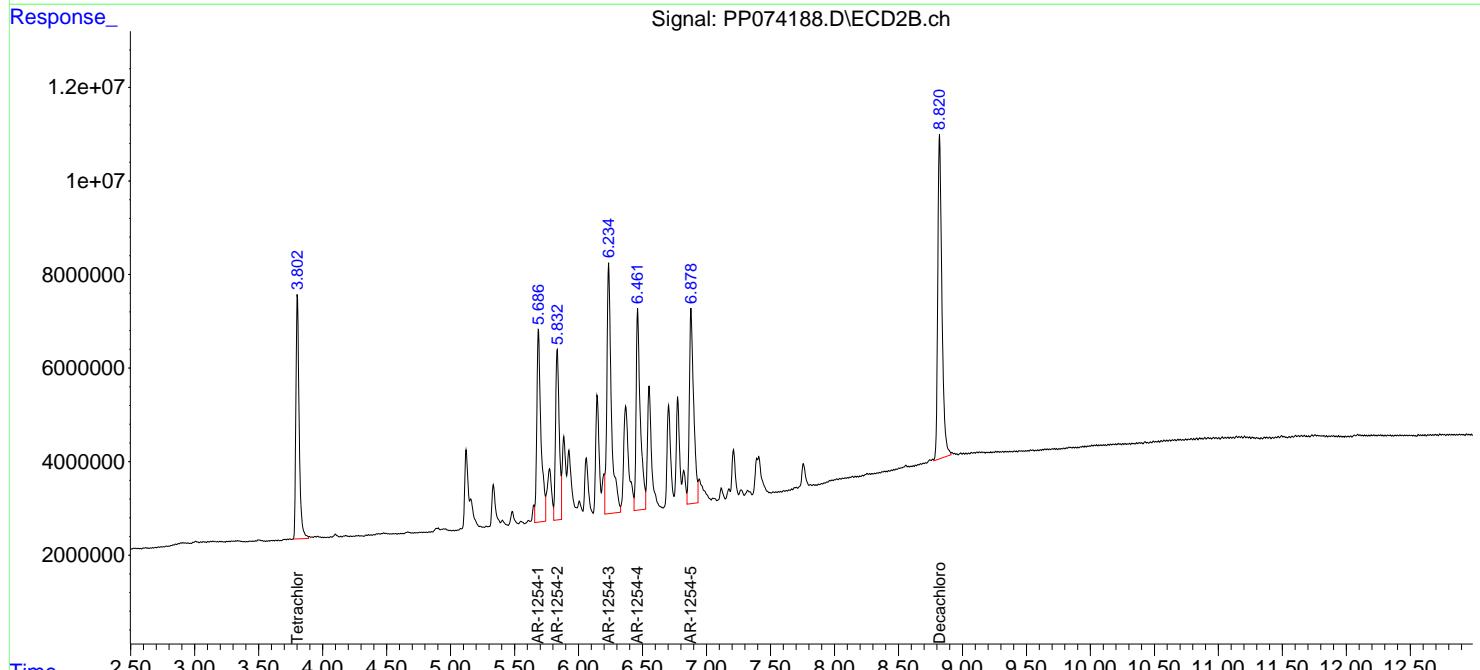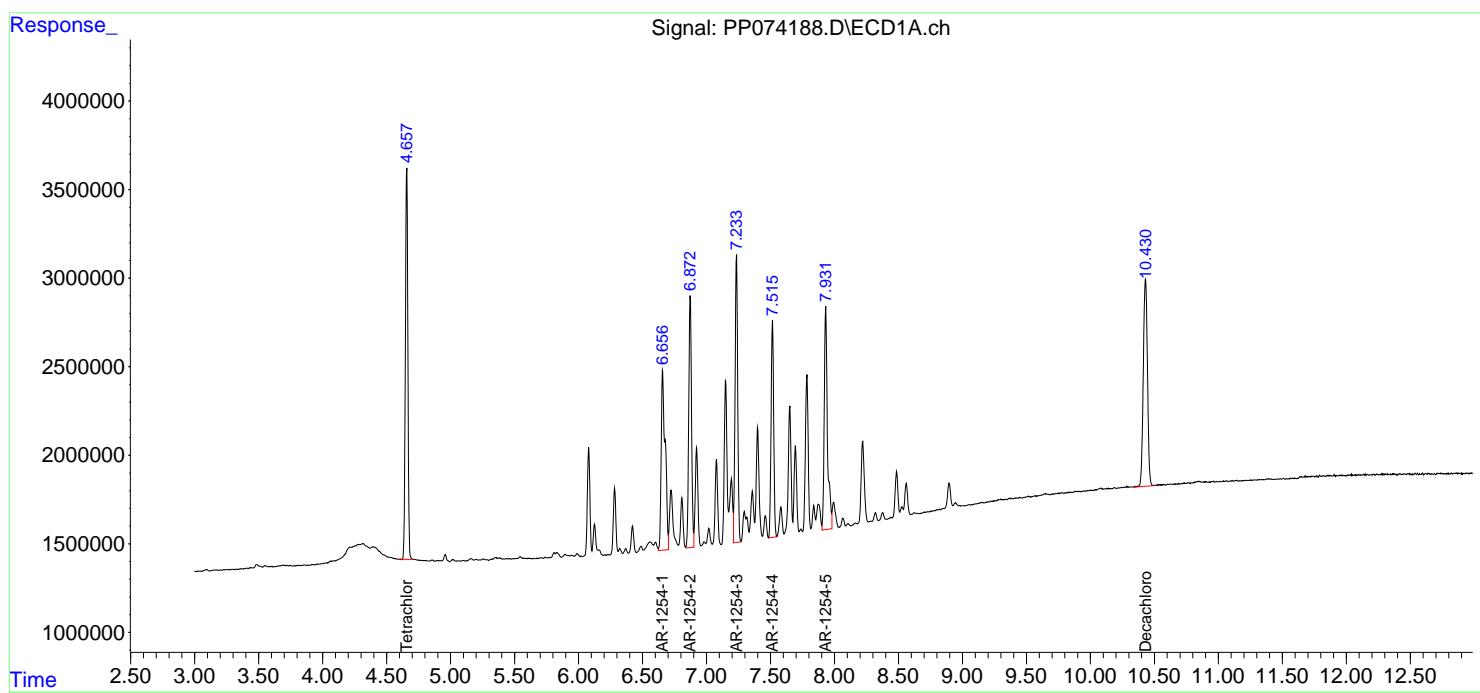

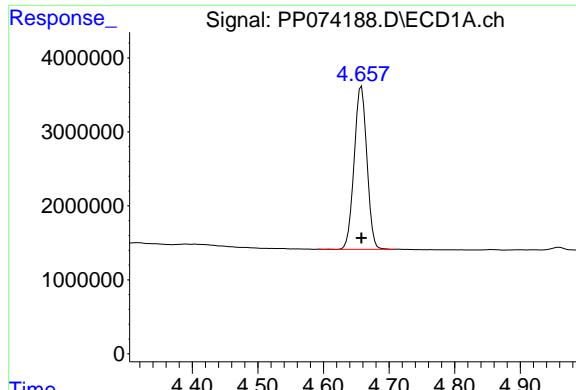

#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: 0.000 min
Response: 29734018
Conc: 26.68 ng/ml

Instrument:

ECD_P


ClientSampleId :

AR1254ICC250

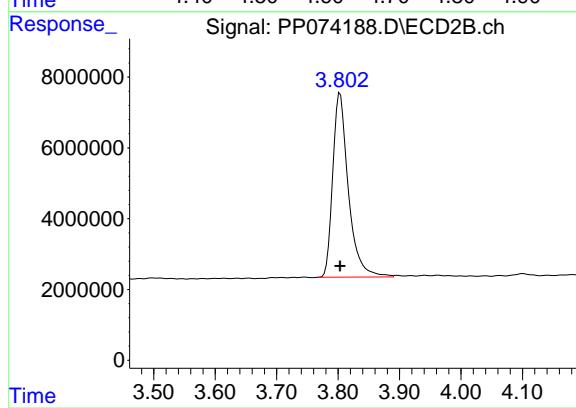


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.000 min
Response: 92012238
Conc: 22.78 ng/ml

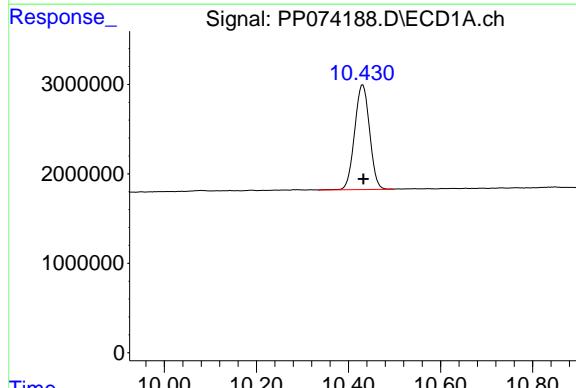


#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: -0.001 min
Response: 26431747
Conc: 27.00 ng/ml

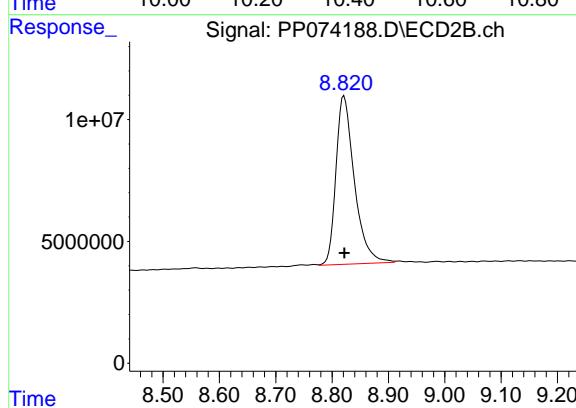

#2 Decachlorobiphenyl


R.T.: 8.821 min
Delta R.T.: 0.000 min
Response: 156986884
Conc: 25.66 ng/ml

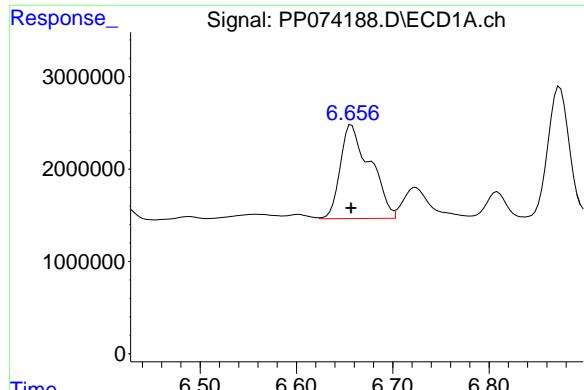

#26 AR-1254-1


R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 21966850
Conc: 405.12 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

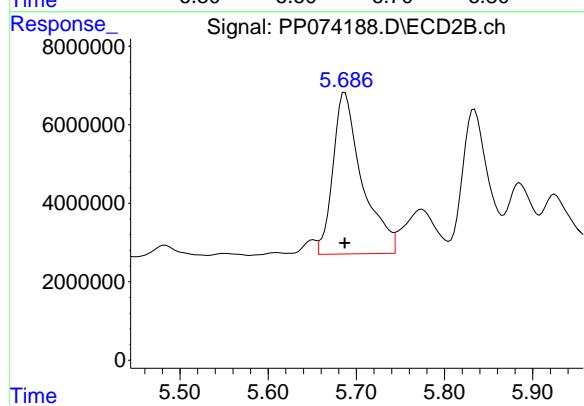


#26 AR-1254-1

R.T.: 5.687 min
Delta R.T.: 0.000 min
Response: 94373679
Conc: 245.07 ng/ml

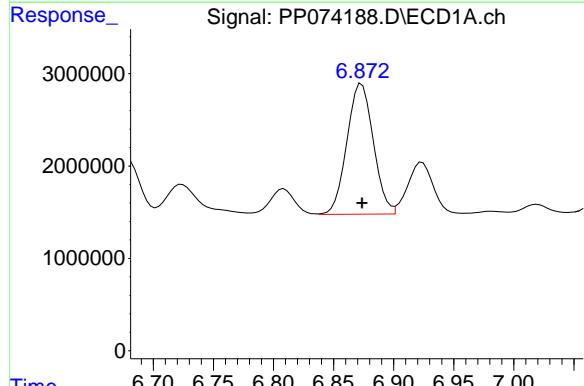


#27 AR-1254-2

R.T.: 6.873 min
Delta R.T.: 0.000 min
Response: 21644264
Conc: 276.90 ng/ml

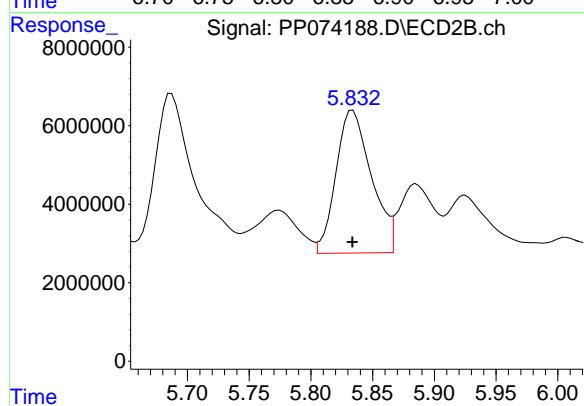


#27 AR-1254-2

R.T.: 5.834 min
Delta R.T.: 0.000 min
Response: 72682229
Conc: 255.80 ng/ml




#28 AR-1254-3

R.T.: 7.235 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 23355124 ECD_P
 Conc: 276.46 ng/ml **ClientSampleId:**
 AR1254ICC250

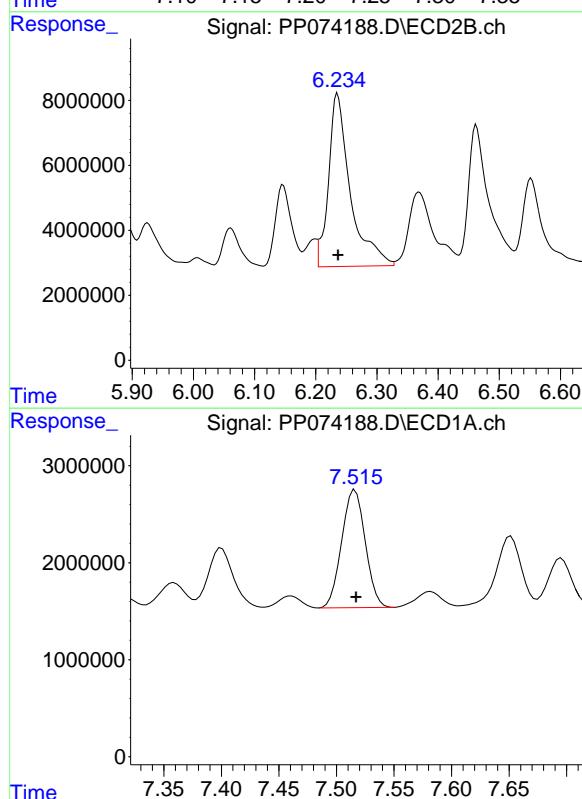


#29 AR-1254-4

R.T.: 7.516 min
 Delta R.T.: 0.000 min
 Response: 17399794
 Conc: 274.32 ng/ml

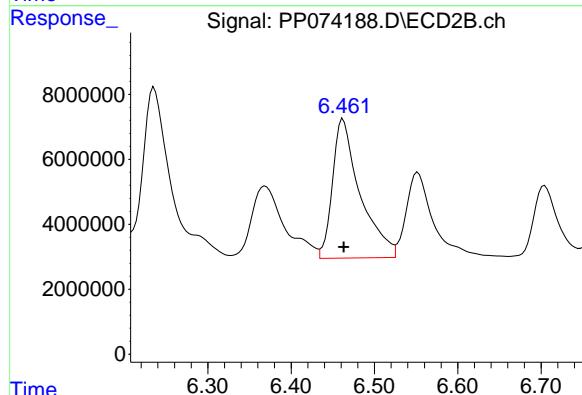

#29 AR-1254-4


R.T.: 6.462 min
 Delta R.T.: 0.000 min
 Response: 98587777
 Conc: 261.44 ng/ml



#30 AR-1254-5

R.T.: 7.932 min
Delta R.T.: 0.000 min
Response: 22010158
Conc: 272.89 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC250

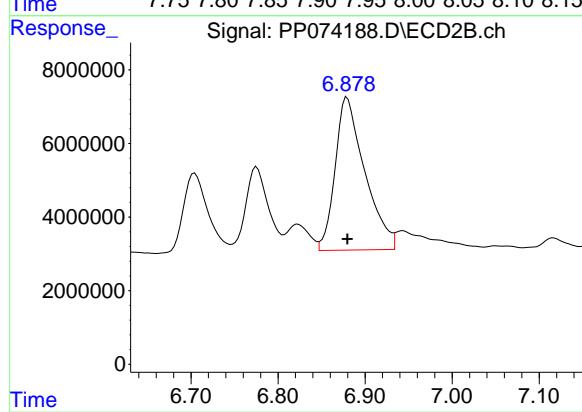

#30 AR-1254-5

R.T.: 6.879 min
Delta R.T.: 0.000 min
Response: 98393861
Conc: 247.08 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 19:23
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:03:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:03:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|---------|----------|-------|---------|
| 1) SA Tetrachlor... | 4.657 | 3.804 | 5935360 | 12647504 | 5.284 | 3.358 # |
| 2) SA Decachlor... | 10.430 | 8.823 | 5026515 | 24210870 | 5.158 | 4.086 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|---------|----------|--------|----------|
| 26) L6 AR-1254-1 | 6.656 | 5.689 | 4505164 | 16116298 | 83.459 | 44.012 # |
| 27) L6 AR-1254-2 | 6.872 | 5.836 | 4500635 | 12761430 | 56.609 | 45.869 |
| 28) L6 AR-1254-3 | 7.234 | 6.237 | 5142235 | 18482386 | 58.892 | 37.780 # |
| 29) L6 AR-1254-4 | 7.515 | 6.464 | 3412924 | 14935198 | 53.486 | 40.633 |
| 30) L6 AR-1254-5 | 7.931 | 6.881 | 4380720 | 14900727 | 53.986 | 37.906 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074189.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 19:23
 Operator : YP\AJ
 Sample : AR1254ICC050
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1254ICC050

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:03:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:03:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

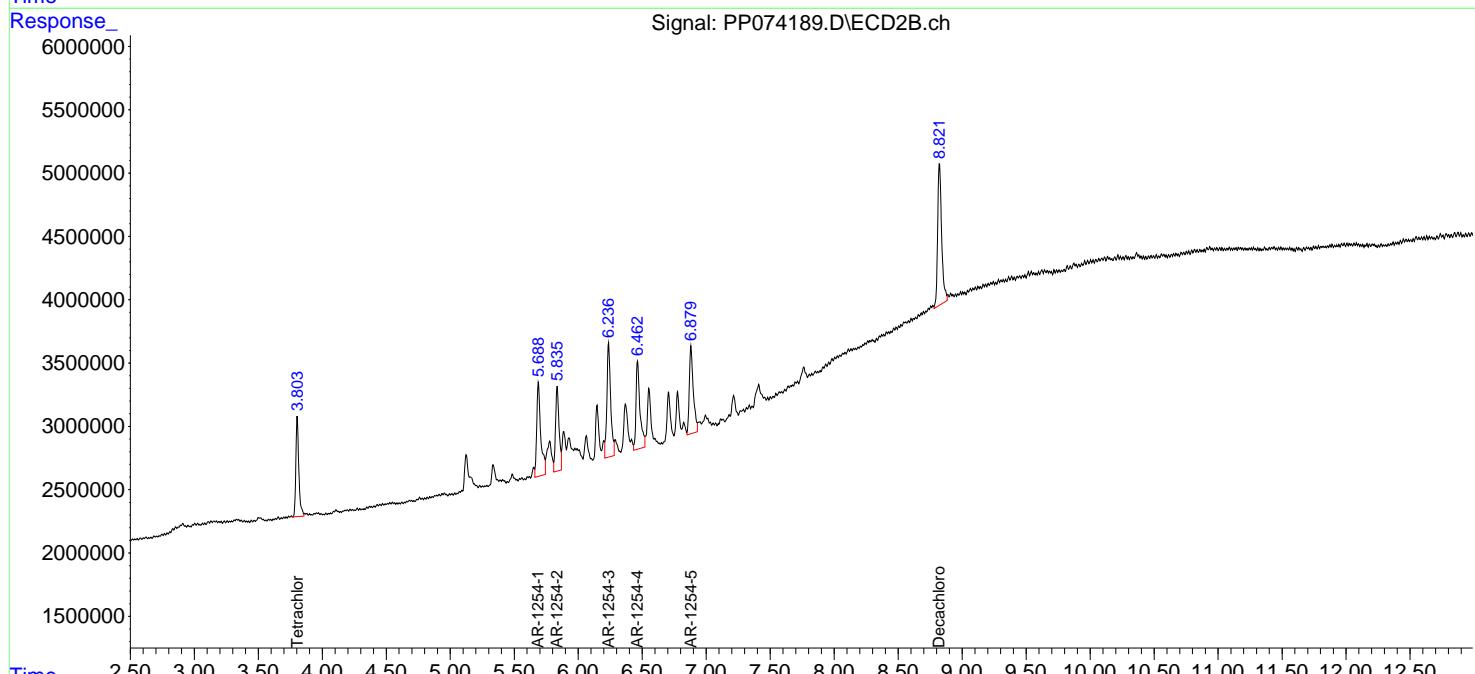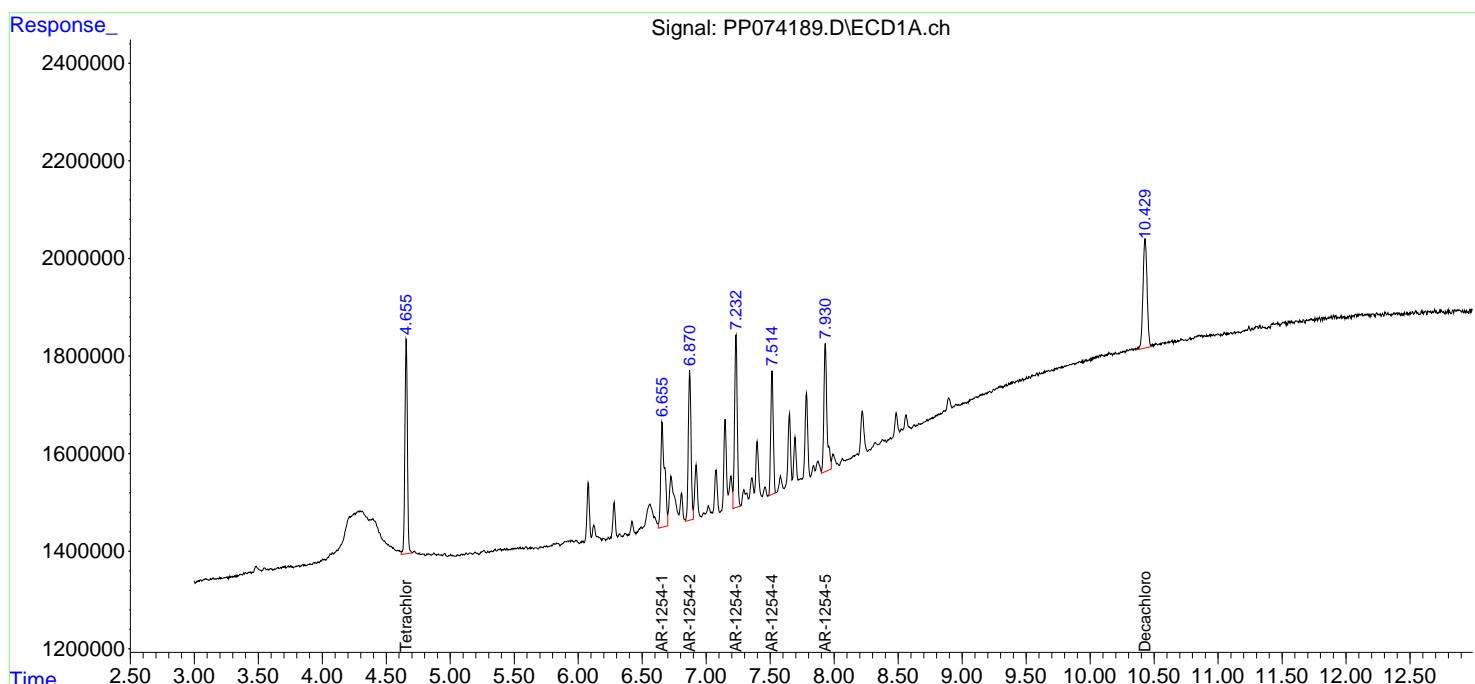

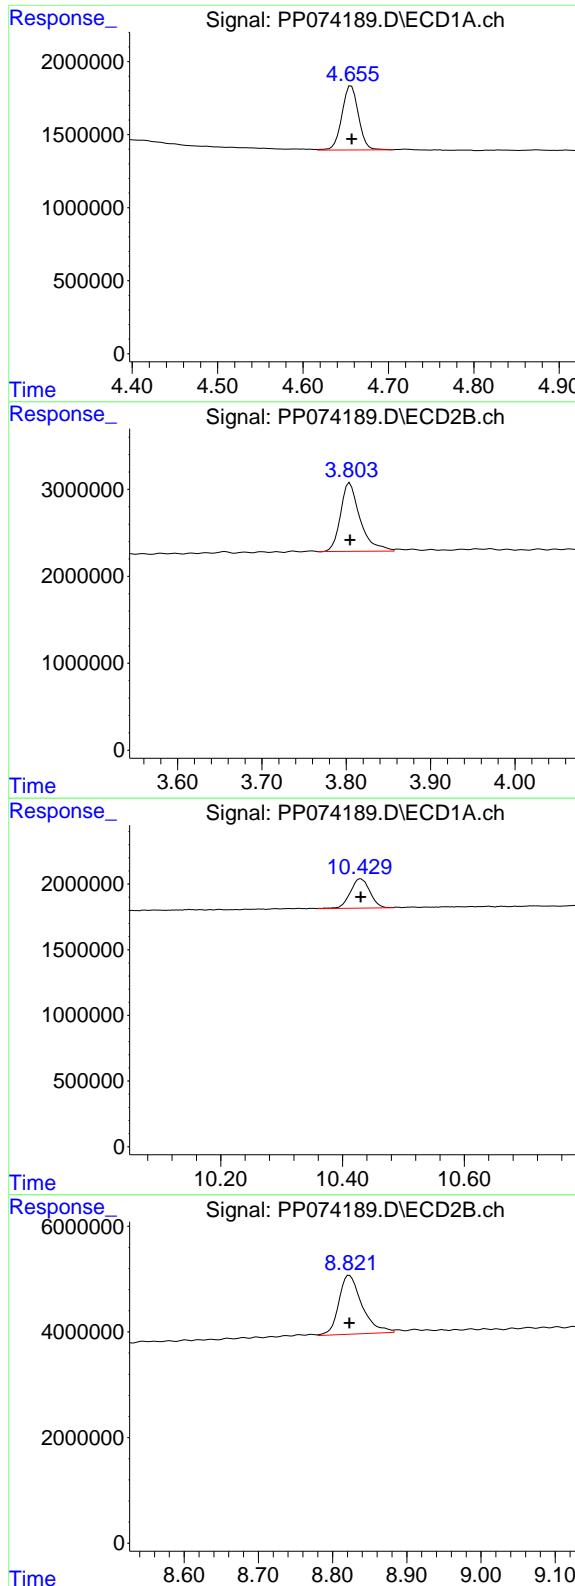

#1 Tetrachloro-m-xylene

R.T.: 4.657 min
 Delta R.T.: 0.000 min
 Response: 5935360
 Conc: 5.28 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1254ICC050

#1 Tetrachloro-m-xylene


R.T.: 3.804 min
 Delta R.T.: 0.000 min
 Response: 12647504
 Conc: 3.36 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.430 min
 Delta R.T.: 0.000 min
 Response: 5026515
 Conc: 5.16 ng/ml

#2 Decachlorobiphenyl


R.T.: 8.823 min
 Delta R.T.: 0.000 min
 Response: 24210870
 Conc: 4.09 ng/ml

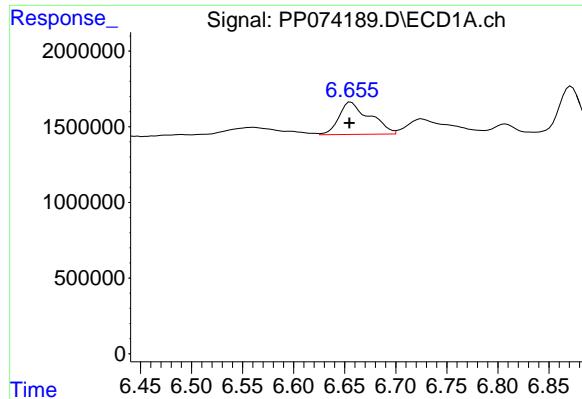

#26 AR-1254-1


R.T.: 6.656 min
Delta R.T.: 0.001 min
Response: 4505164
Conc: 83.46 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

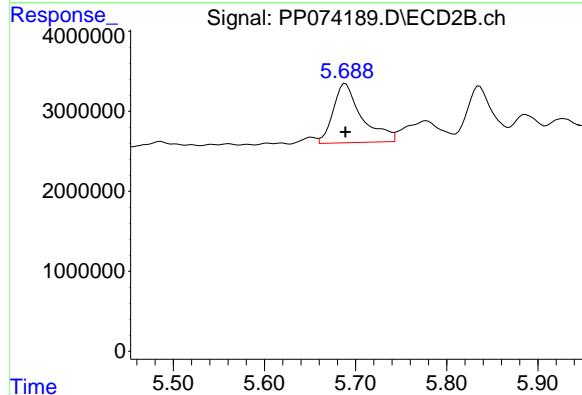


#26 AR-1254-1

R.T.: 5.689 min
Delta R.T.: 0.000 min
Response: 16116298
Conc: 44.01 ng/ml

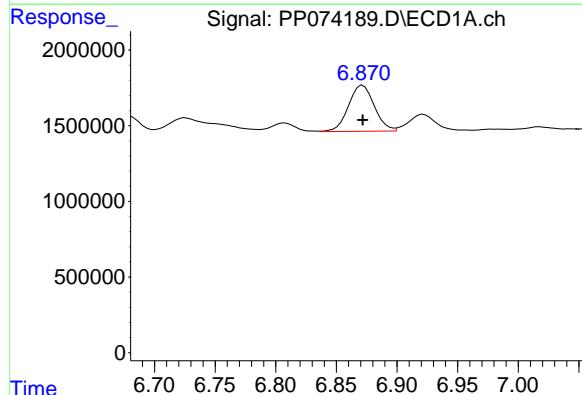


#27 AR-1254-2

R.T.: 6.872 min
Delta R.T.: 0.000 min
Response: 4500635
Conc: 56.61 ng/ml

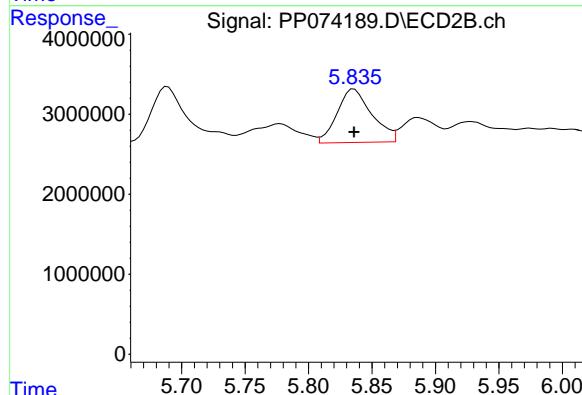

#27 AR-1254-2

R.T.: 5.836 min
Delta R.T.: 0.000 min
Response: 12761430
Conc: 45.87 ng/ml

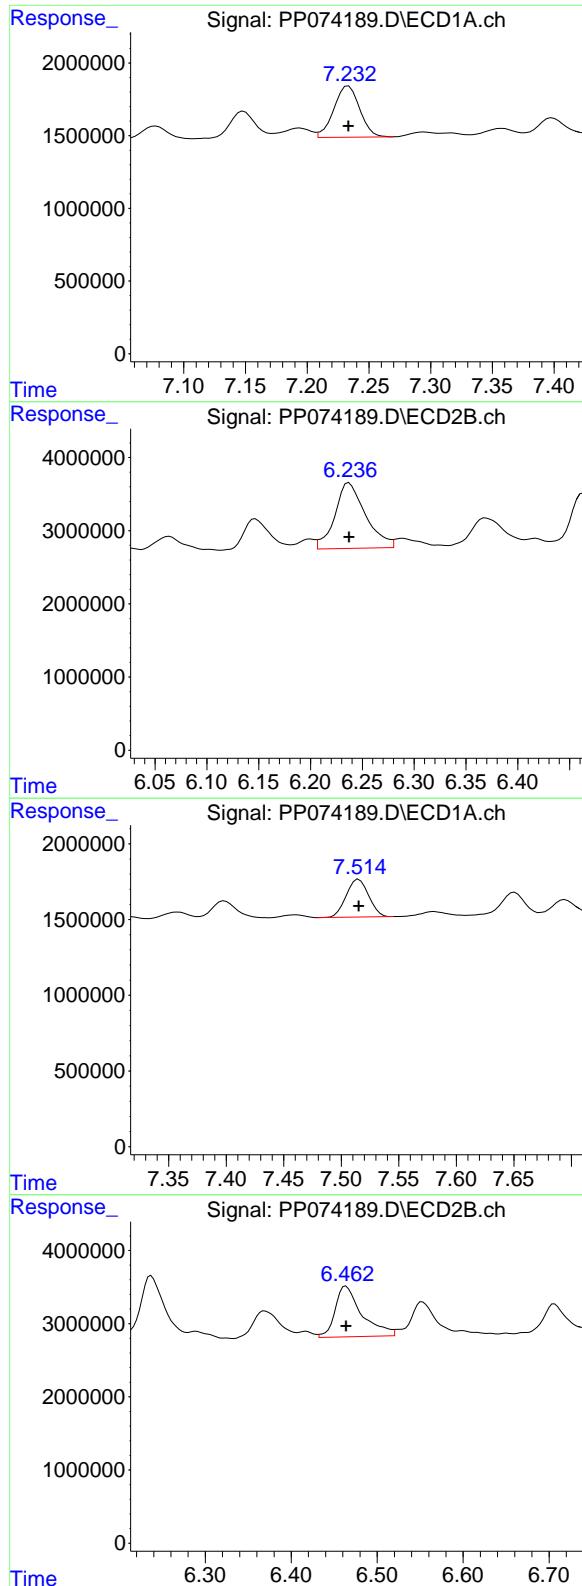

#28 AR-1254-3

R.T.: 7.234 min
 Delta R.T.: 0.000 min
 Response: 5142235
 Conc: 58.89 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1254ICC050

#28 AR-1254-3



R.T.: 6.237 min
 Delta R.T.: 0.000 min
 Response: 18482386
 Conc: 37.78 ng/ml

#29 AR-1254-4

R.T.: 7.515 min
 Delta R.T.: 0.000 min
 Response: 3412924
 Conc: 53.49 ng/ml

#29 AR-1254-4

R.T.: 6.464 min
 Delta R.T.: 0.000 min
 Response: 14935198
 Conc: 40.63 ng/ml

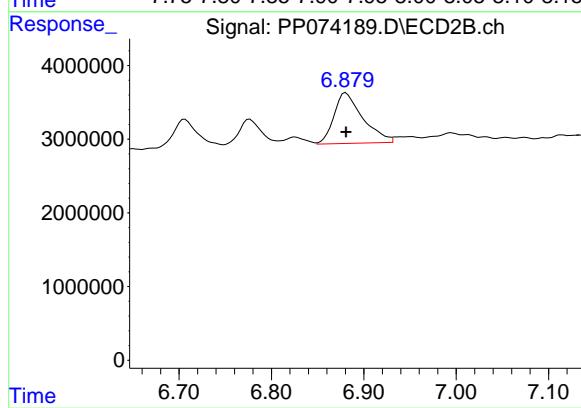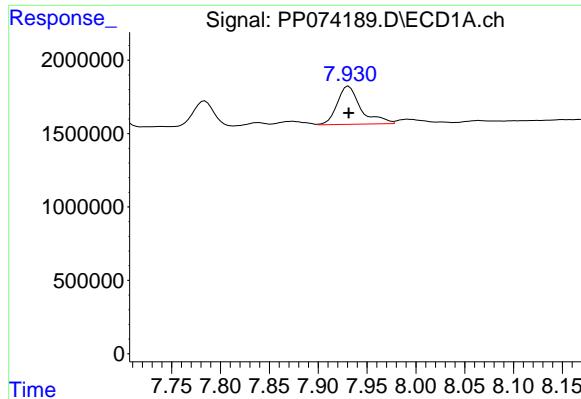

#30 AR-1254-5

R.T.: 7.931 min
Delta R.T.: 0.000 min
Response: 4380720
Conc: 53.99 ng/ml

Instrument: ECD_P
ClientSampleId: AR1254ICC050

#30 AR-1254-5

R.T.: 6.881 min
Delta R.T.: 0.000 min
Response: 14900727
Conc: 37.91 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 22:05
 Operator : YP\AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:36:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.655 | 3.804 | 55143327 | 198.9E6 | 49.310 | 51.866 |
| 2) SA Decachlor... | 10.427 | 8.822 | 47800939 | 295.6E6 | 49.220 | 49.156 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|------------|
| 3) L1 AR-1016-1 | 5.806 | 4.904 | 17499270 | 167.4E6 | 424.155 | 419.611 |
| 4) L1 AR-1016-2 | 5.827 | 4.962 | 25894594 | 77861664 | 426.307 | 414.579 |
| 5) L1 AR-1016-3 | 5.890 | 5.082 | 17050061 | 43676713 | 429.900 | 411.774 |
| 6) L1 AR-1016-4 | 5.987 | 5.123 | 14124012 | 42005219 | 433.991 | 384.593 |
| 7) L1 AR-1016-5 | 6.280 | 5.337 | 14033364 | 49362976 | 432.221 | 422.038 |
| 8) L2 AR-1221-1 | 4.850 | 4.014 | 2188169 | 5427967 | 130.531 | 110.583 |
| 9) L2 AR-1221-2 | 4.940 | 4.101 | 3152368 | 7977800 | 250.167 | 222.289 |
| 10) L2 AR-1221-3 | 5.015 | 4.177 | 10712240 | 35262086 | 292.403 | 260.767 |
| 11) L3 AR-1232-1 | 5.015 | 4.177 | 10712240 | 35262086 | 368.913 | 347.881 |
| 12) L3 AR-1232-2 | 5.541 | 4.904 | 13527303 | 167.4E6 | 899.259 | 960.470 |
| 13) L3 AR-1232-3 | 5.827 | 5.082 | 25894594 | 43676713 | 892.864 | 953.294 |
| 14) L3 AR-1232-4 | 5.987 | 5.165 | 14124012 | 78538633 | 913.063 | 1353.864 # |
| 15) L3 AR-1232-5 | 6.076 | 5.337 | 11989403 | 49362976 | 1023.335 | 1050.735 |
| 16) L4 AR-1242-1 | 5.806 | 4.904 | 17499270 | 167.4E6 | 469.580 | 484.954 |
| 17) L4 AR-1242-2 | 5.827 | 4.962 | 25894594 | 77861664 | 475.925 | 476.575 |
| 18) L4 AR-1242-3 | 5.890 | 5.082 | 17050061 | 43676713 | 477.113 | 473.468 |
| 19) L4 AR-1242-4 | 5.987 | 5.165 | 14124012 | 78538633 | 483.390 | 657.658 # |
| 20) L4 AR-1242-5 | 6.716 | 5.686 | 16823190 | 70286035 | 473.119 | 469.952 |
| 21) L5 AR-1248-1 | 5.806 | 4.904 | 17499270 | 167.4E6 | 624.650 | 782.387 # |
| 22) L5 AR-1248-2 | 6.076 | 5.123 | 11989403 | 42005219 | 297.791 | 287.092 |
| 23) L5 AR-1248-3 | 6.280 | 5.165 | 14033364 | 78538633 | 314.836 | 458.058 # |
| 24) L5 AR-1248-4 | 6.677 | 5.337 | 14725685 | 49362976 | 282.984 | 296.700 |
| 25) L5 AR-1248-5 | 6.716 | 5.726 | 16823190 | 76598345 | 295.438 | 263.255 |
| 26) L6 AR-1254-1 | 6.651 | 5.686 | 10912353 | 70286035 | 207.297 | 191.943 |
| 27) L6 AR-1254-2 | 6.872 | 5.834 | 13215605 | 16964136 | 166.224 | 60.974 # |
| 28) L6 AR-1254-3 | 7.231 | 6.236 | 5959793 | 21465299 | 68.255 | 43.877 # |
| 29) L6 AR-1254-4 | 7.512 | 6.461 | 4317662 | 17873856 | 67.665 | 48.628 # |
| 30) L6 AR-1254-5 | 7.928 | 6.879 | 1449445 | 4651318 | 17.862 | 11.833 # |
| 31) L7 AR-1260-1 | 7.400 | 6.552 | 593868 | 2870221 | 10.538 | 7.105 # |
| 32) L7 AR-1260-2 | 7.647 | 6.705 | 839562 | 1902548 | 12.319 | 6.084 # |
| 33) L7 AR-1260-3 | 8.025 | 6.943 | 47683 | 370567 | 0.895 | 0.940 |
| 34) L7 AR-1260-4 | 8.217 | 7.184 | 560766 | 72352 | 8.956 | 0.249 # |
| 35) L7 AR-1260-5 | 8.559 | 7.415 | 212917 | 384725 | 1.879 | 0.508 # |
| 36) L8 AR-1262-1 | 8.217 | 6.943 | 560766 | 370567 | 7.399 | 0.658 # |
| 37) L8 AR-1262-2 | 8.559 | 7.170 | 212917 | 147921 | 1.632 | 0.369 # |
| 38) L8 AR-1262-3 | 8.894 | 7.699 | 131960 | 339738 | 1.403 | 0.945 # |
| 39) L8 AR-1262-4 | 8.981 | 7.758 | 35860 | 593683 | 0.492 | 0.890 # |
| 40) L8 AR-1262-5 | 9.662 | 8.258 | 83218 | 116580 | 1.634 | 0.412 # |
| 41) L9 AR-1268-1 | 8.894 | 7.699 | 131960 | 339738 | 0.848 | 0.312 # |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074197.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 22:05
 Operator : YP\AJ
 Sample : AR1242ICV500
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1242

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:36:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|--------|-------|--------|---------|-------|---------|
| 42) L9 AR-1268-2 | 8.981 | 7.758 | 35860 | 593683 | 0.250 | 0.559 # |
| 43) L9 AR-1268-3 | 9.214 | 7.972 | 255483 | 1184209 | 2.138 | 1.423 # |
| 44) L9 AR-1268-4 | 9.662 | 8.258 | 83218 | 116580 | 1.415 | 0.378 # |
| 45) L9 AR-1268-5 | 10.072 | 8.563 | 363528 | 1086905 | 1.034 | 0.426 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125
Data File : PP074197.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Aug 2025 22:05
Operator : YP\AJ
Sample : AR1242ICV500
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1242

```
Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 02 01:36:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title  : GC EXTRACTABLES
QLast Update : Sat Aug 02 01:33:31 2025
Response via : Initial Calibration
Integrator: ChemStation
```

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

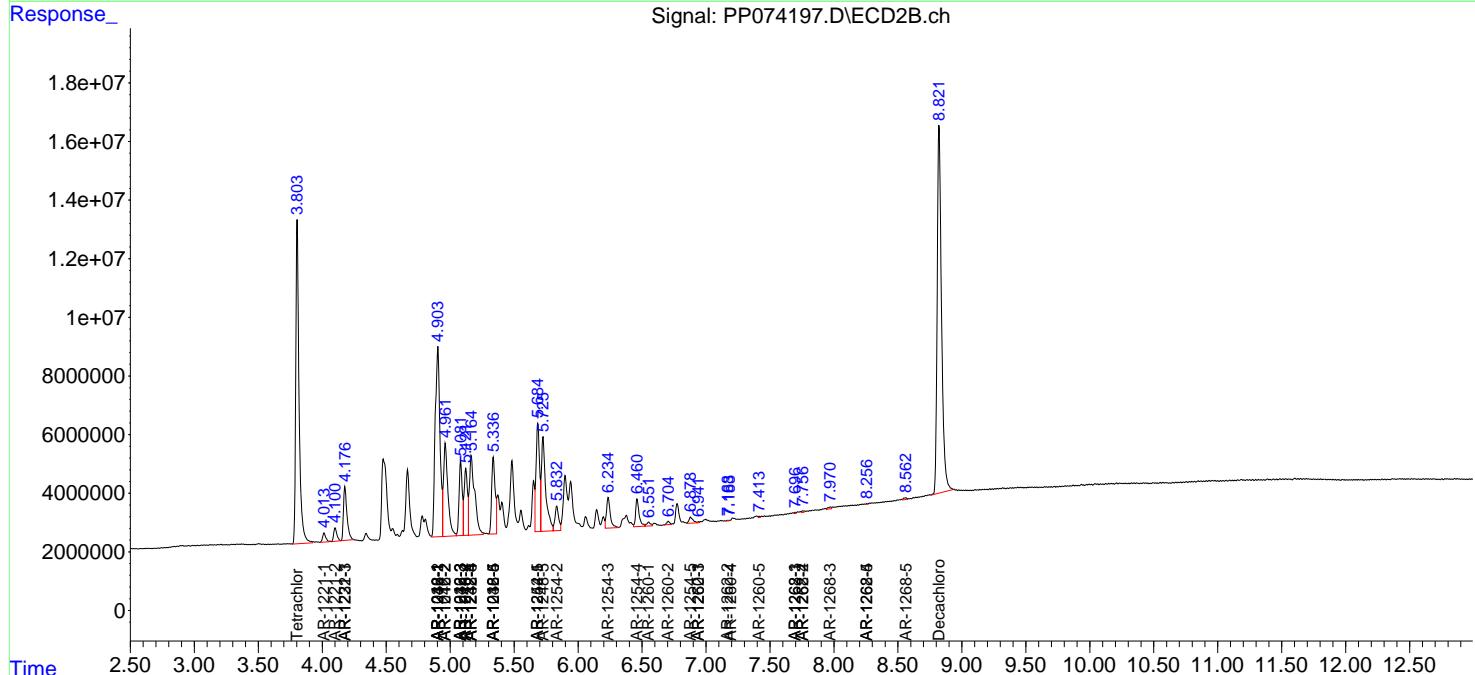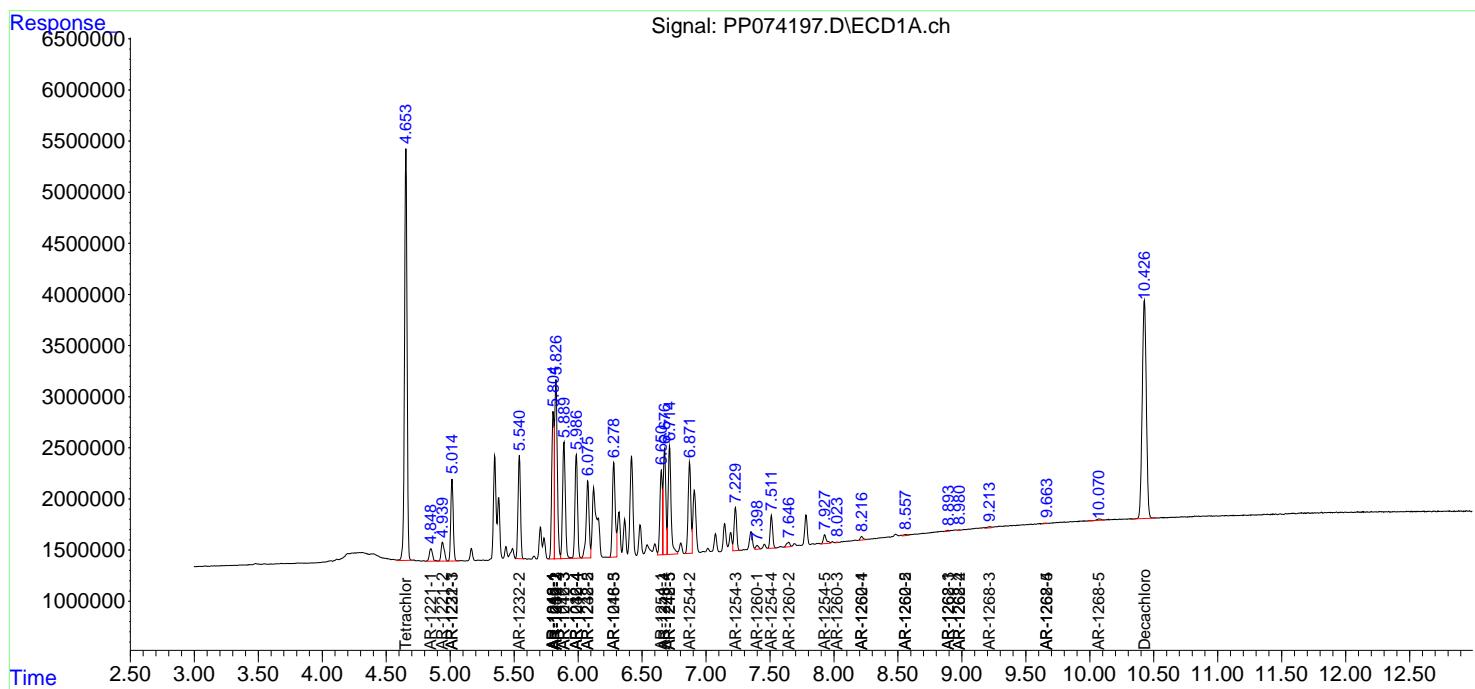


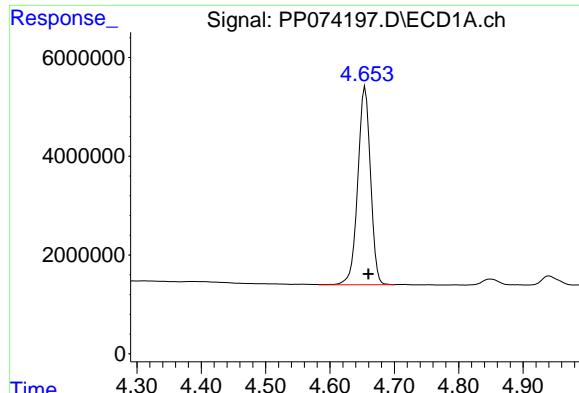

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: -0.005 min
Response: 55143327
Conc: 49.31 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

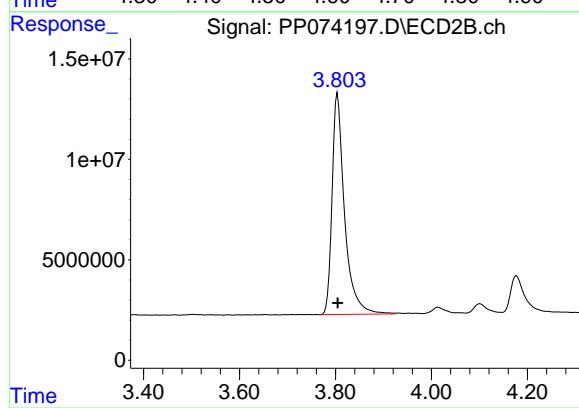


#1 Tetrachloro-m-xylene

R.T.: 3.804 min
Delta R.T.: 0.000 min
Response: 198876613
Conc: 51.87 ng/ml

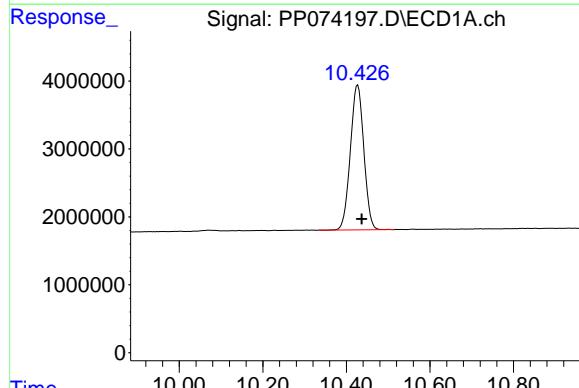


#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: -0.010 min
Response: 47800939
Conc: 49.22 ng/ml

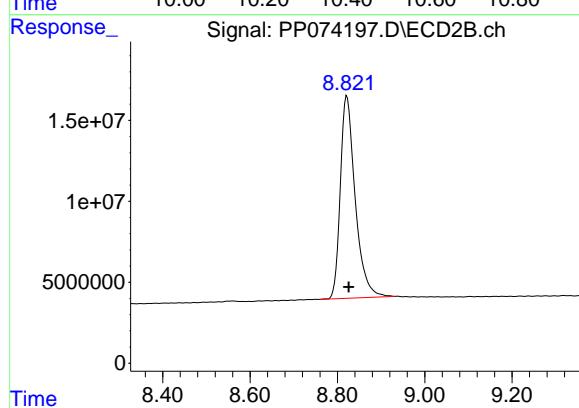

#2 Decachlorobiphenyl


R.T.: 8.822 min
Delta R.T.: -0.004 min
Response: 295607088
Conc: 49.16 ng/ml

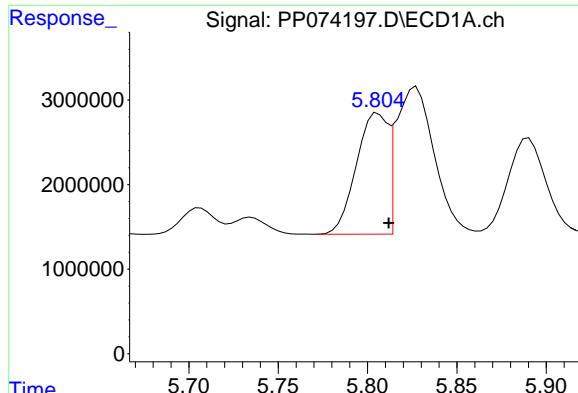

#3 AR-1016-1


R.T.: 5.806 min
 Delta R.T.: -0.006 min
 Response: 17499270
 Conc: 424.15 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

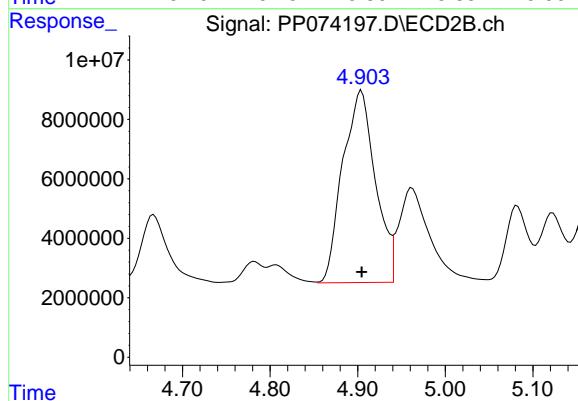


#3 AR-1016-1

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 167377399
 Conc: 419.61 ng/ml

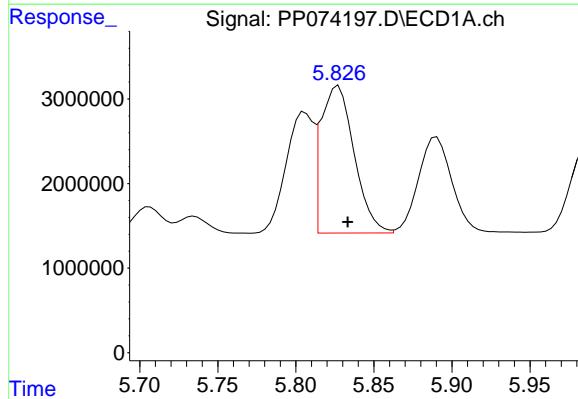


#4 AR-1016-2

R.T.: 5.827 min
 Delta R.T.: -0.006 min
 Response: 25894594
 Conc: 426.31 ng/ml

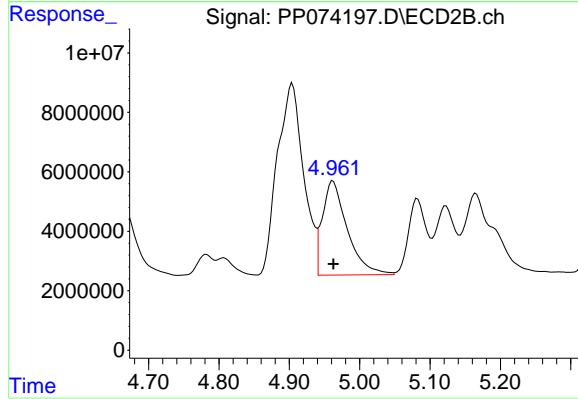

#4 AR-1016-2


R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 77861664
 Conc: 414.58 ng/ml

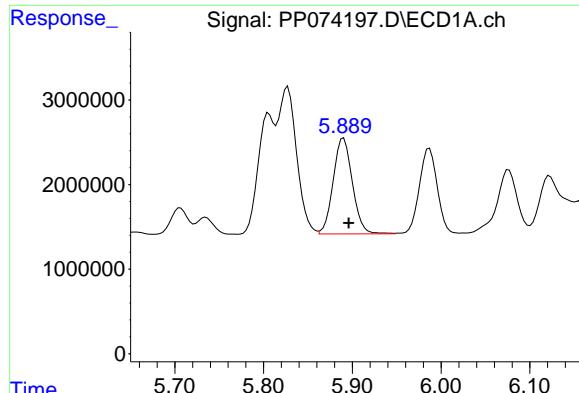

#5 AR-1016-3


R.T.: 5.890 min
 Delta R.T.: -0.006 min
 Response: 17050061
 Conc: 429.90 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

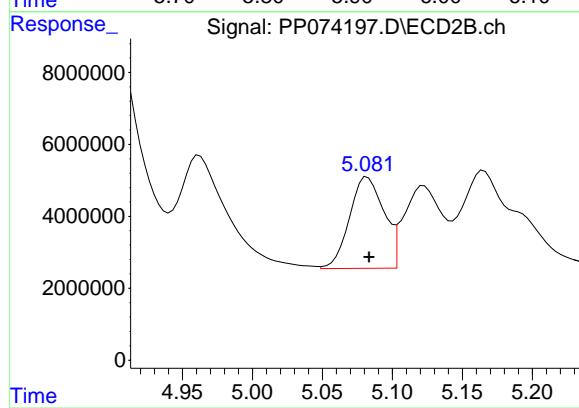


#5 AR-1016-3

R.T.: 5.082 min
 Delta R.T.: -0.001 min
 Response: 43676713
 Conc: 411.77 ng/ml

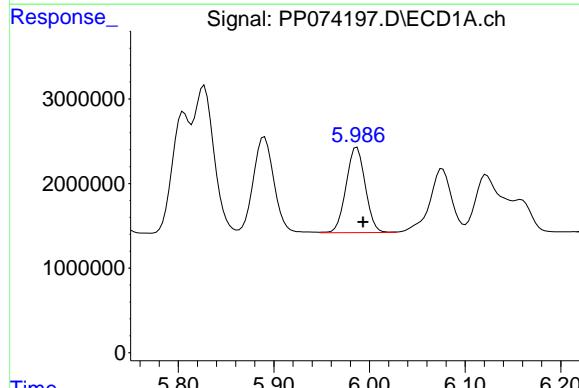


#6 AR-1016-4

R.T.: 5.987 min
 Delta R.T.: -0.006 min
 Response: 14124012
 Conc: 433.99 ng/ml

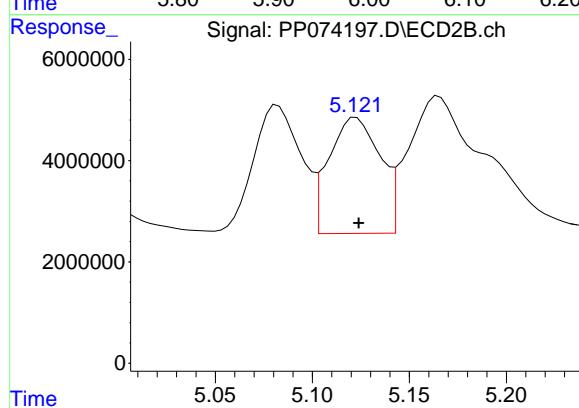

#6 AR-1016-4

R.T.: 5.123 min
 Delta R.T.: -0.001 min
 Response: 42005219
 Conc: 384.59 ng/ml

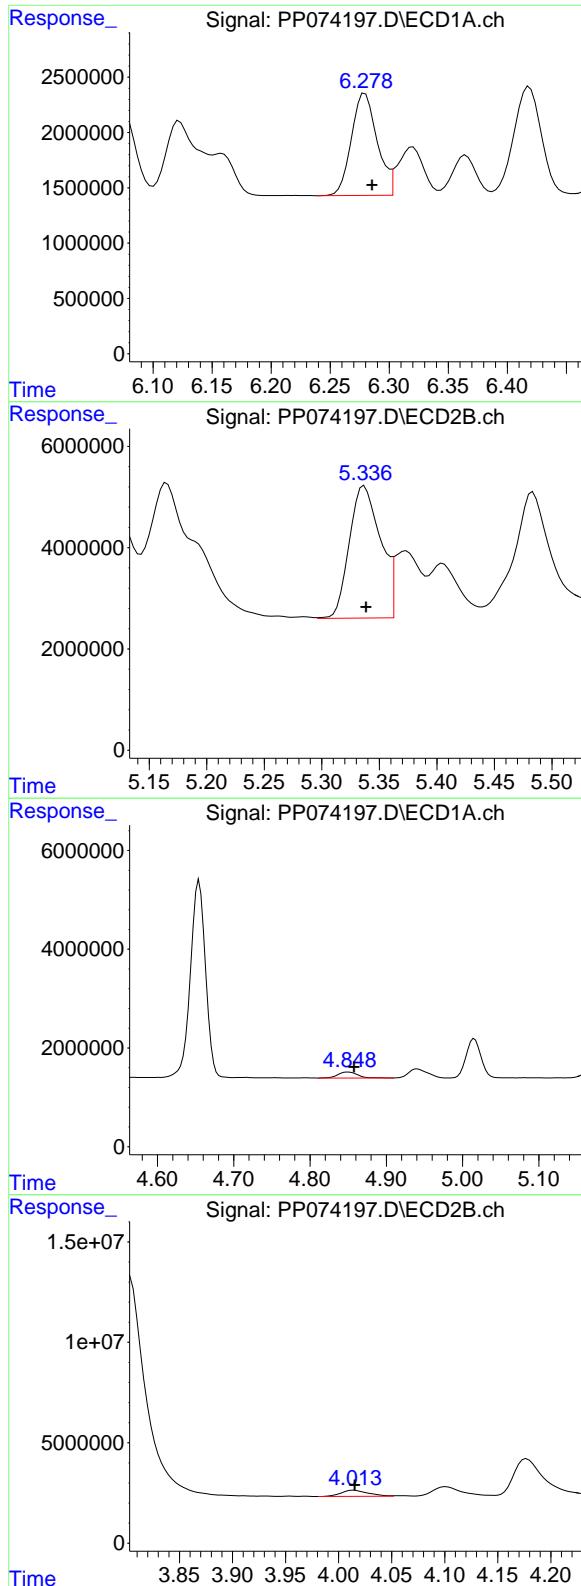

#7 AR-1016-5

R.T.: 6.280 min
 Delta R.T.: -0.006 min
 Response: 14033364
 Conc: 432.22 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#7 AR-1016-5


R.T.: 5.337 min
 Delta R.T.: -0.001 min
 Response: 49362976
 Conc: 422.04 ng/ml

#8 AR-1221-1

R.T.: 4.850 min
 Delta R.T.: -0.008 min
 Response: 2188169
 Conc: 130.53 ng/ml

#8 AR-1221-1


R.T.: 4.014 min
 Delta R.T.: 0.000 min
 Response: 5427967
 Conc: 110.58 ng/ml

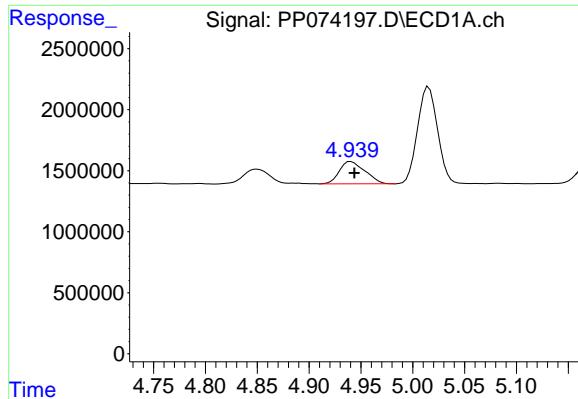

#9 AR-1221-2


R.T.: 4.940 min
Delta R.T.: -0.003 min
Response: 3152368
Conc: 250.17 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

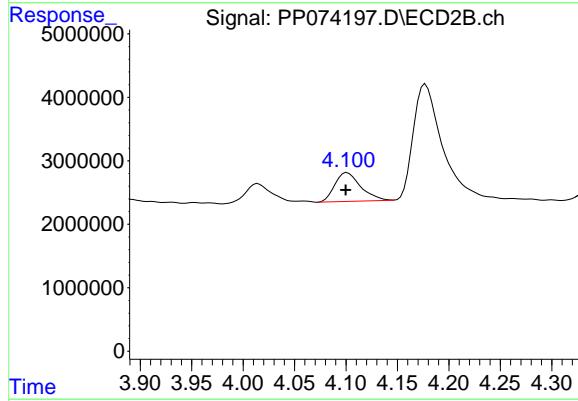


#9 AR-1221-2

R.T.: 4.101 min
Delta R.T.: 0.001 min
Response: 7977800
Conc: 222.29 ng/ml

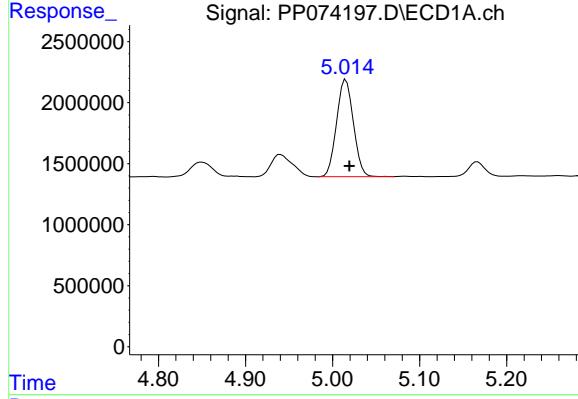


#10 AR-1221-3

R.T.: 5.015 min
Delta R.T.: -0.004 min
Response: 10712240
Conc: 292.40 ng/ml

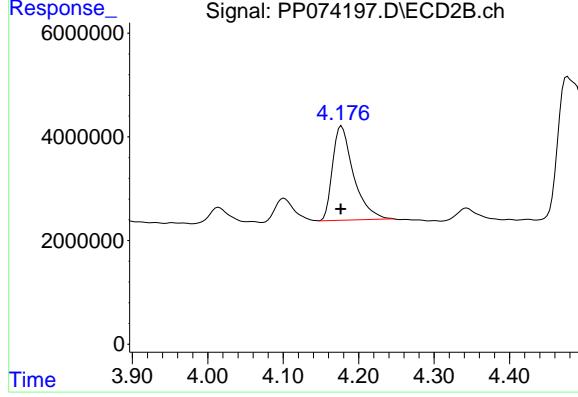

#10 AR-1221-3

R.T.: 4.177 min
Delta R.T.: 0.001 min
Response: 35262086
Conc: 260.77 ng/ml

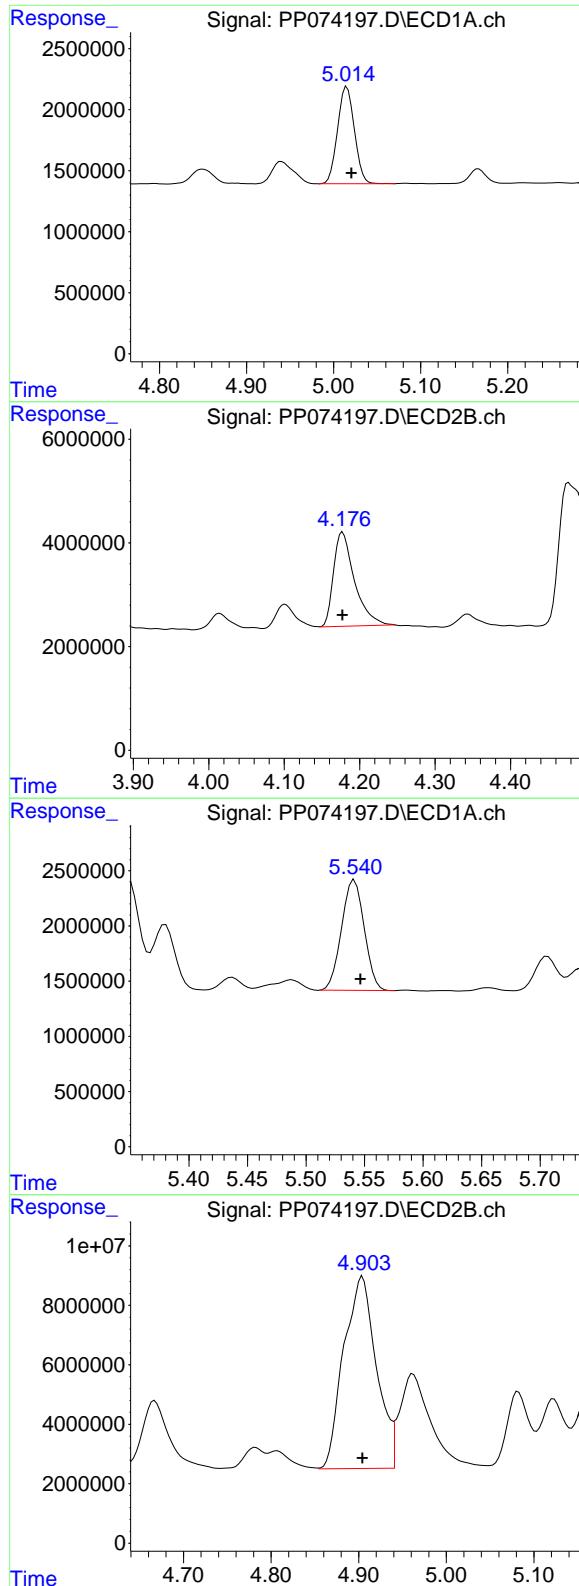

#11 AR-1232-1

R.T.: 5.015 min
 Delta R.T.: -0.005 min
 Response: 10712240
 Conc: 368.91 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#11 AR-1232-1


R.T.: 4.177 min
 Delta R.T.: 0.000 min
 Response: 35262086
 Conc: 347.88 ng/ml

#12 AR-1232-2

R.T.: 5.541 min
 Delta R.T.: -0.005 min
 Response: 13527303
 Conc: 899.26 ng/ml

#12 AR-1232-2

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 167377399
 Conc: 960.47 ng/ml

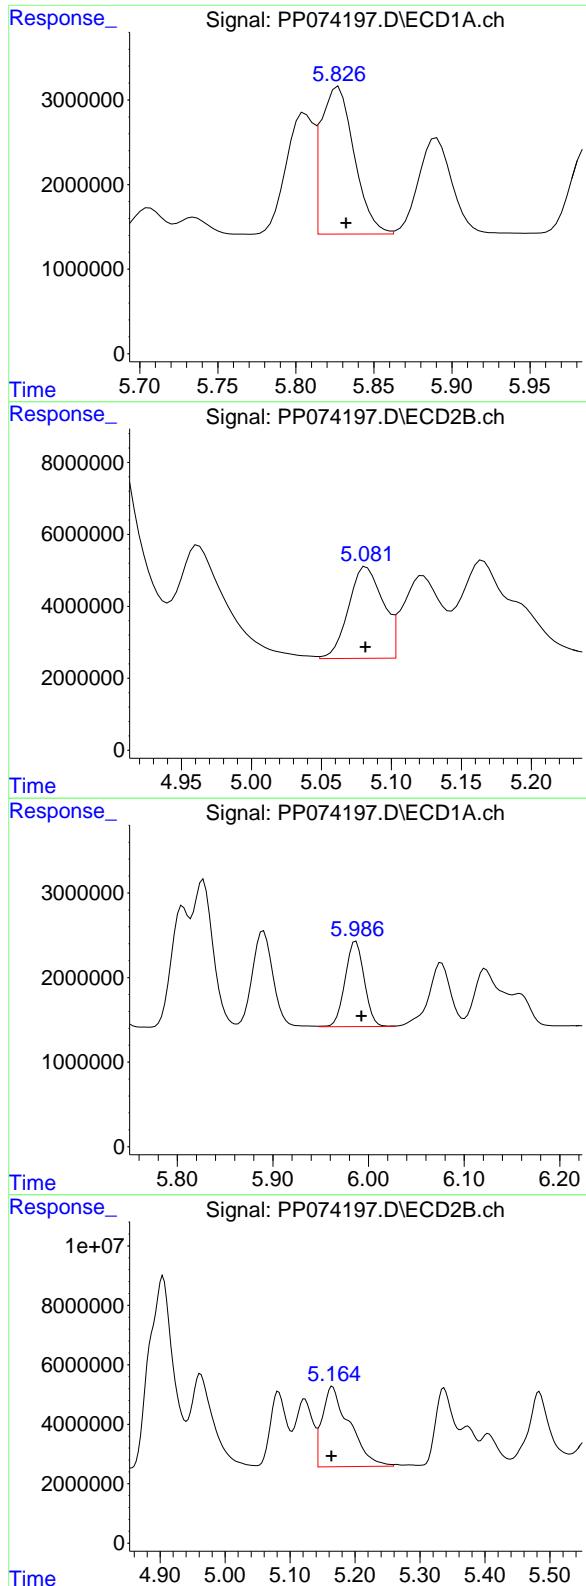

#13 AR-1232-3

R.T.: 5.827 min
 Delta R.T.: -0.005 min
 Response: 25894594
 Conc: 892.86 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#13 AR-1232-3


R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 43676713
 Conc: 953.29 ng/ml

#14 AR-1232-4

R.T.: 5.987 min
 Delta R.T.: -0.006 min
 Response: 14124012
 Conc: 913.06 ng/ml

#14 AR-1232-4


R.T.: 5.165 min
 Delta R.T.: 0.002 min
 Response: 78538633
 Conc: 1353.86 ng/ml



#15 AR-1232-5


R.T.: 6.076 min
 Delta R.T.: -0.006 min
 Response: 11989403
 Conc: 1023.33 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

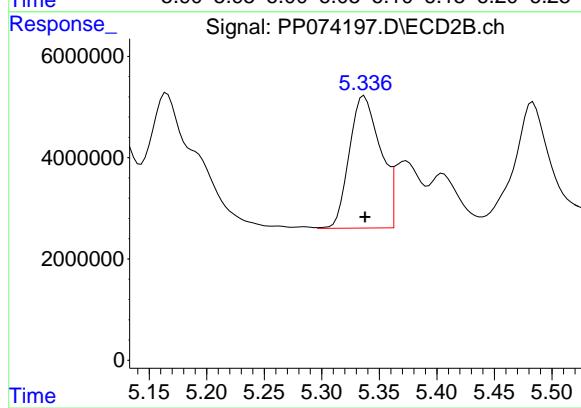


#15 AR-1232-5

R.T.: 5.337 min
 Delta R.T.: 0.000 min
 Response: 49362976
 Conc: 1050.74 ng/ml




#16 AR-1242-1

R.T.: 5.806 min
 Delta R.T.: -0.005 min
 Response: 17499270
 Conc: 469.58 ng/ml

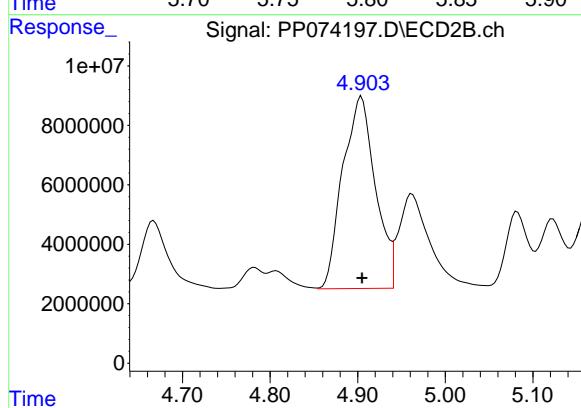

#16 AR-1242-1

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 167377399
 Conc: 484.95 ng/ml

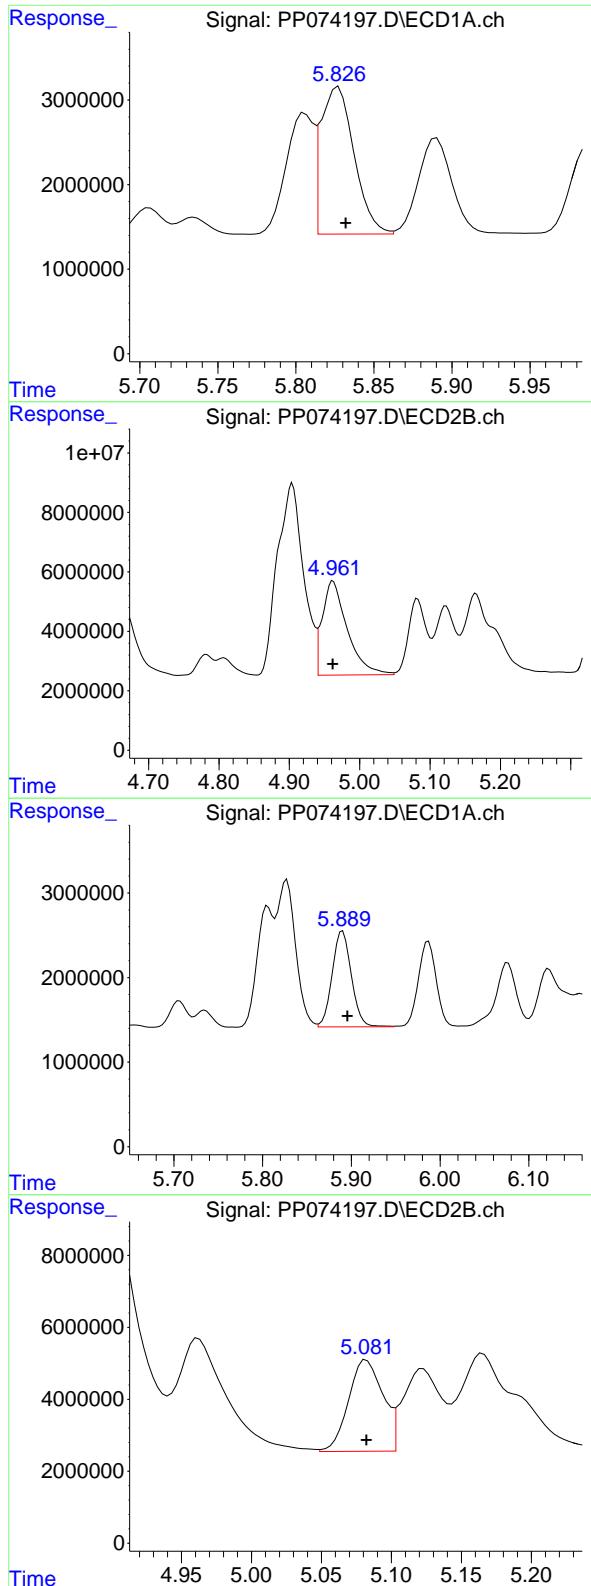

#17 AR-1242-2

R.T.: 5.827 min
 Delta R.T.: -0.005 min
 Response: 25894594
 Conc: 475.93 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#17 AR-1242-2


R.T.: 4.962 min
 Delta R.T.: 0.000 min
 Response: 77861664
 Conc: 476.57 ng/ml

#18 AR-1242-3

R.T.: 5.890 min
 Delta R.T.: -0.005 min
 Response: 17050061
 Conc: 477.11 ng/ml

#18 AR-1242-3


R.T.: 5.082 min
 Delta R.T.: 0.000 min
 Response: 43676713
 Conc: 473.47 ng/ml

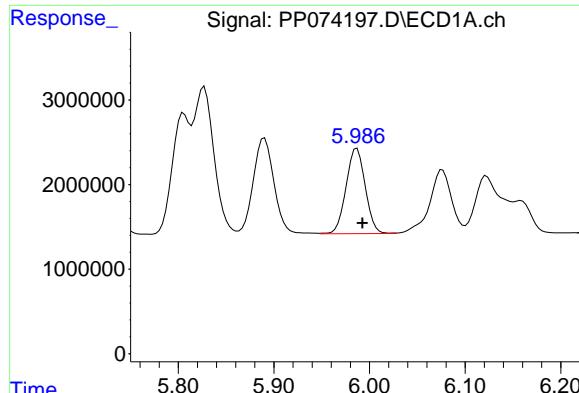

#19 AR-1242-4


R.T.: 5.987 min
 Delta R.T.: -0.006 min
 Response: 14124012
 Conc: 483.39 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

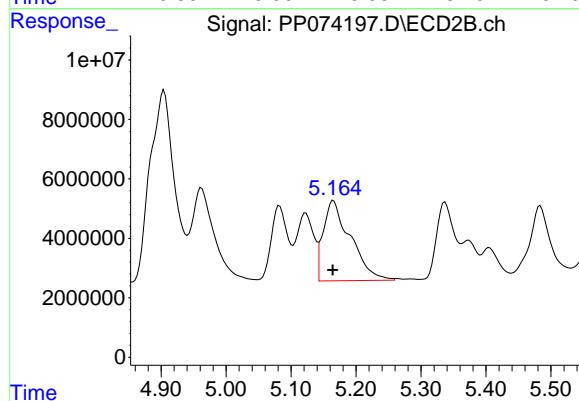


#19 AR-1242-4

R.T.: 5.165 min
 Delta R.T.: 0.001 min
 Response: 78538633
 Conc: 657.66 ng/ml

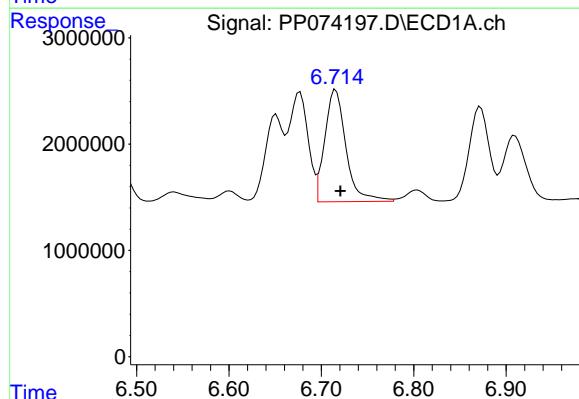


#20 AR-1242-5

R.T.: 6.716 min
 Delta R.T.: -0.005 min
 Response: 16823190
 Conc: 473.12 ng/ml

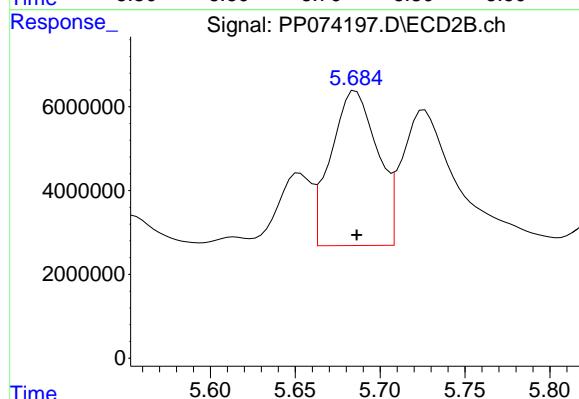

#20 AR-1242-5


R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 70286035
 Conc: 469.95 ng/ml

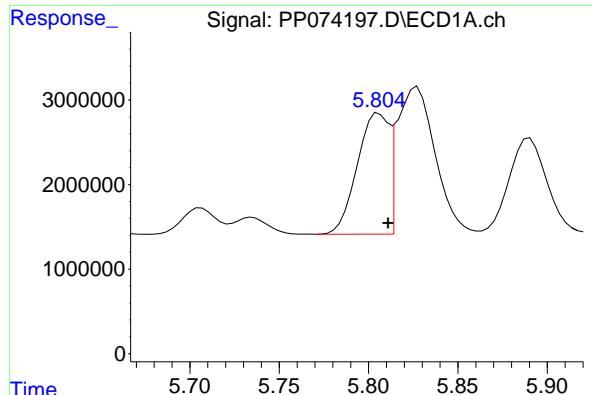

#21 AR-1248-1


R.T.: 5.806 min
 Delta R.T.: -0.005 min
 Response: 17499270
 Conc: 624.65 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

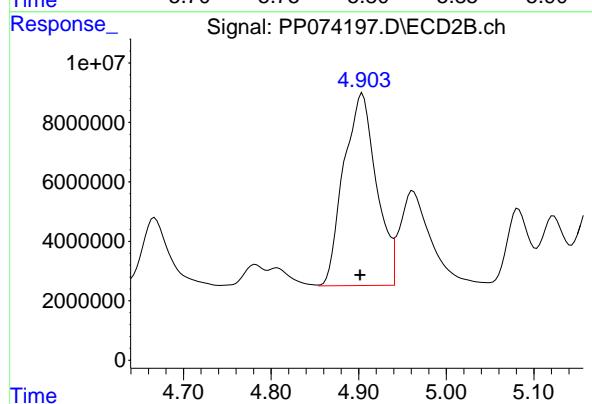


#21 AR-1248-1

R.T.: 4.904 min
 Delta R.T.: 0.003 min
 Response: 167377399
 Conc: 782.39 ng/ml

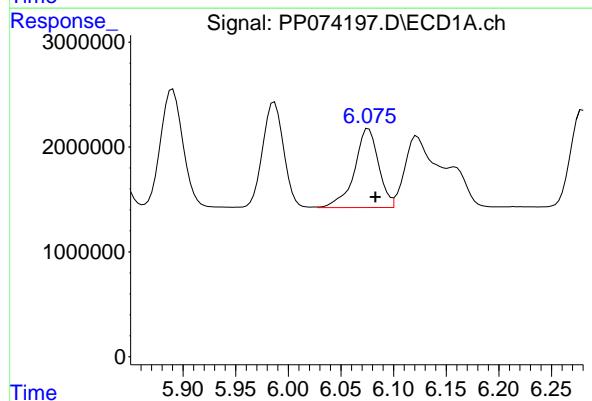


#22 AR-1248-2

R.T.: 6.076 min
 Delta R.T.: -0.006 min
 Response: 11989403
 Conc: 297.79 ng/ml

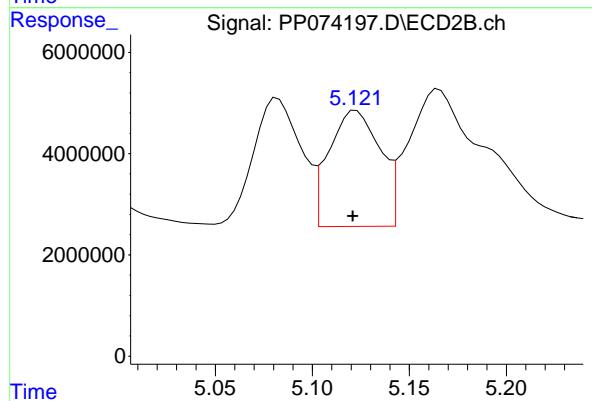

#22 AR-1248-2


R.T.: 5.123 min
 Delta R.T.: 0.002 min
 Response: 42005219
 Conc: 287.09 ng/ml

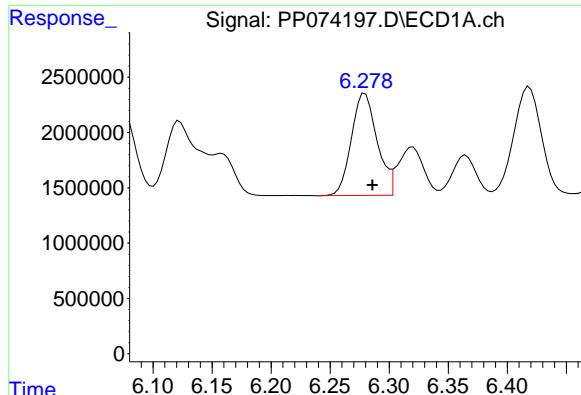

#23 AR-1248-3


R.T.: 6.280 min
 Delta R.T.: -0.006 min
 Response: 14033364
 Conc: 314.84 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

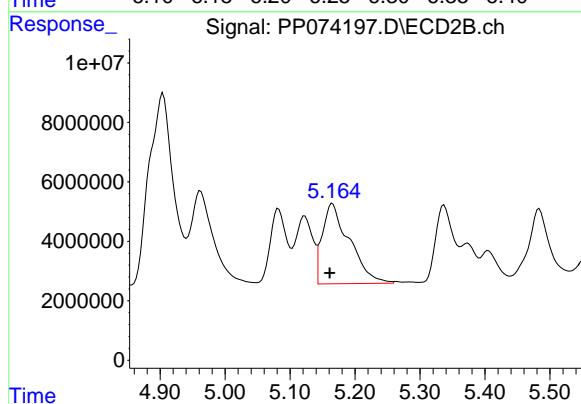


#23 AR-1248-3

R.T.: 5.165 min
 Delta R.T.: 0.004 min
 Response: 78538633
 Conc: 458.06 ng/ml

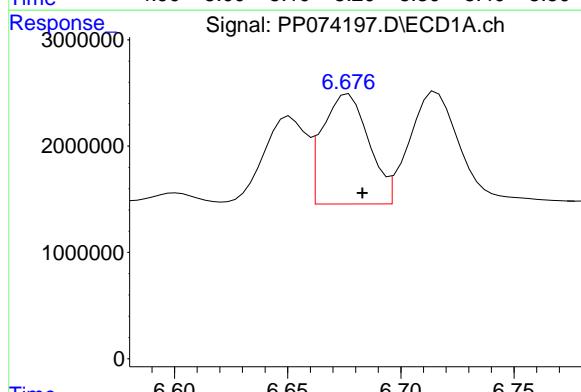


#24 AR-1248-4

R.T.: 6.677 min
 Delta R.T.: -0.006 min
 Response: 14725685
 Conc: 282.98 ng/ml

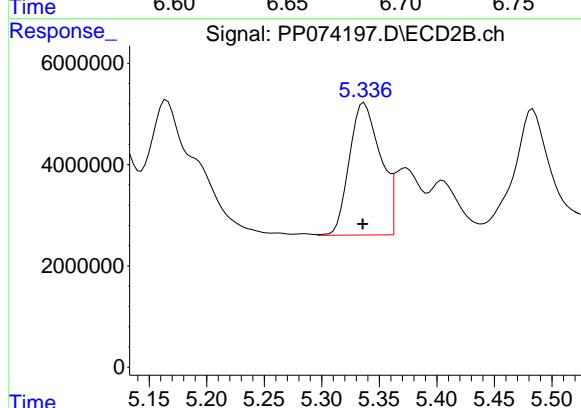

#24 AR-1248-4

R.T.: 5.337 min
 Delta R.T.: 0.002 min
 Response: 49362976
 Conc: 296.70 ng/ml

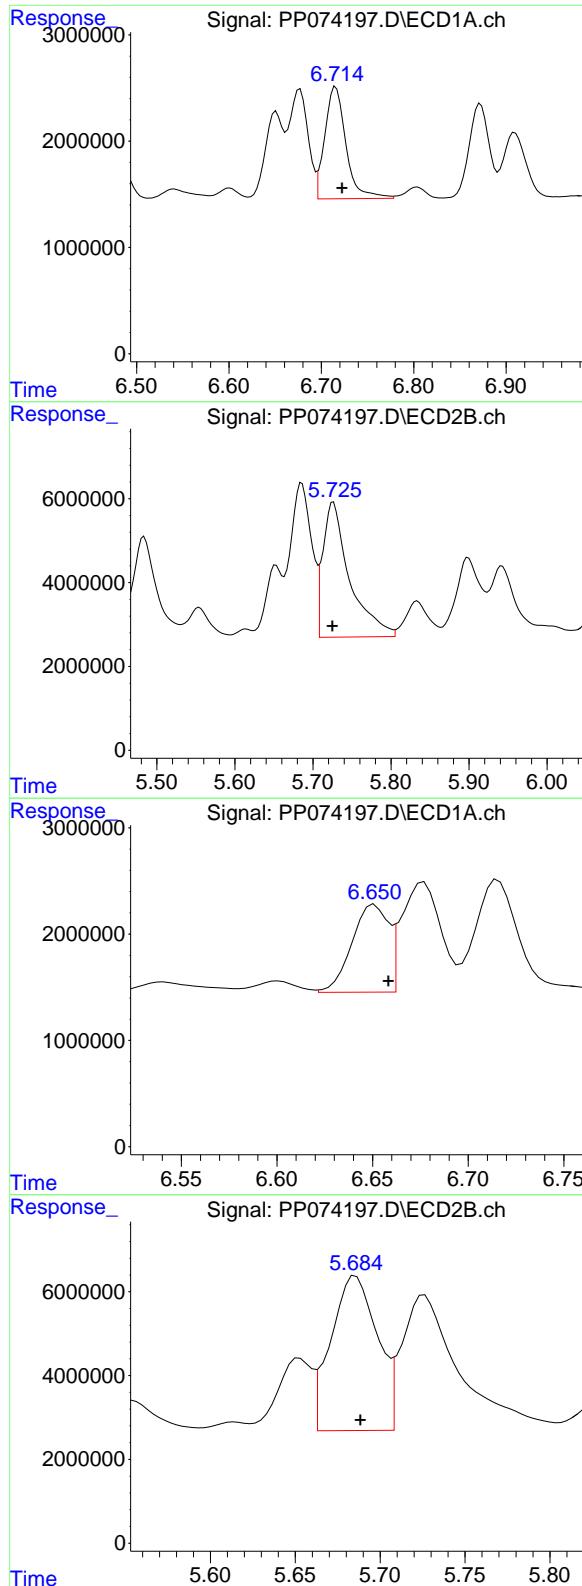

#25 AR-1248-5

R.T.: 6.716 min
 Delta R.T.: -0.007 min
 Response: 16823190
 Conc: 295.44 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#25 AR-1248-5


R.T.: 5.726 min
 Delta R.T.: 0.001 min
 Response: 76598345
 Conc: 263.26 ng/ml

#26 AR-1254-1

R.T.: 6.651 min
 Delta R.T.: -0.007 min
 Response: 10912353
 Conc: 207.30 ng/ml

#26 AR-1254-1

R.T.: 5.686 min
 Delta R.T.: -0.003 min
 Response: 70286035
 Conc: 191.94 ng/ml

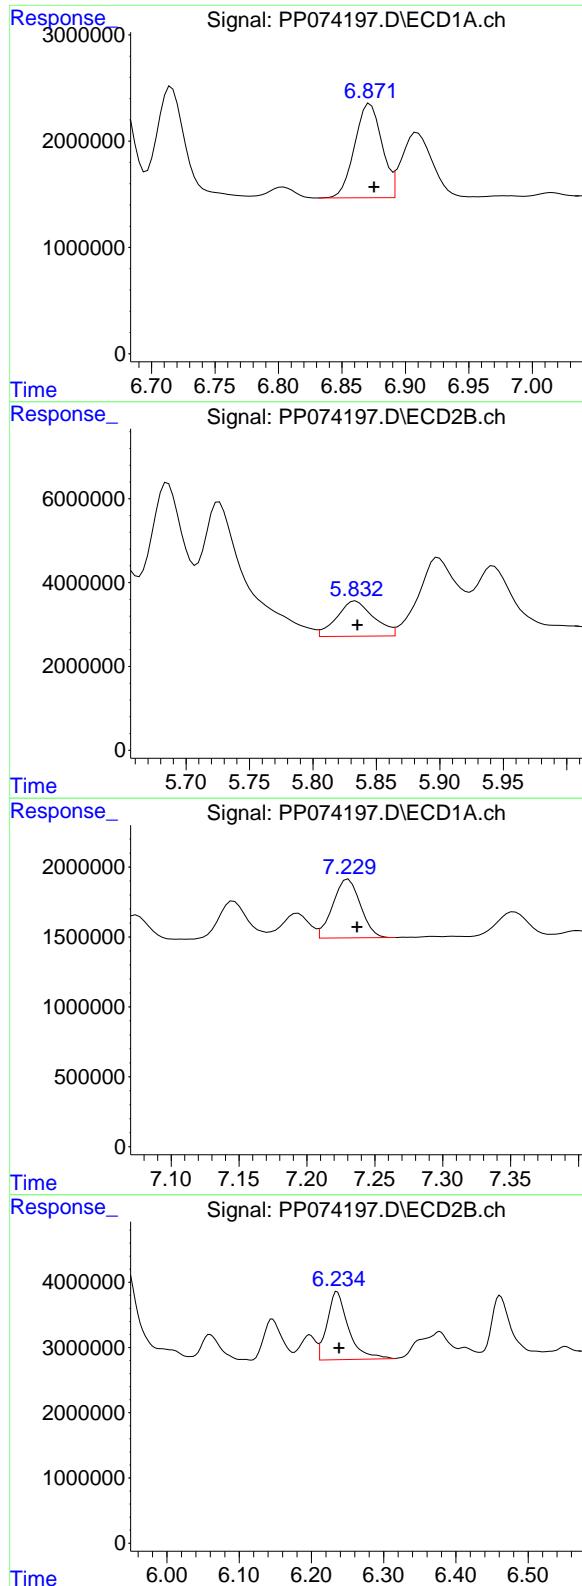

#27 AR-1254-2

R.T.: 6.872 min
 Delta R.T.: -0.003 min
 Response: 13215605
 Conc: 166.22 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#27 AR-1254-2


R.T.: 5.834 min
 Delta R.T.: -0.001 min
 Response: 16964136
 Conc: 60.97 ng/ml

#28 AR-1254-3

R.T.: 7.231 min
 Delta R.T.: -0.006 min
 Response: 5959793
 Conc: 68.26 ng/ml

#28 AR-1254-3


R.T.: 6.236 min
 Delta R.T.: -0.002 min
 Response: 21465299
 Conc: 43.88 ng/ml

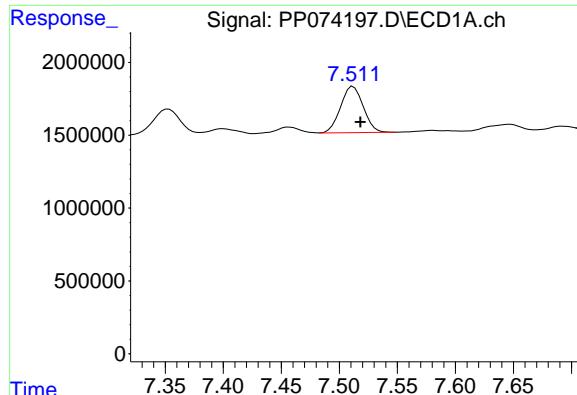

#29 AR-1254-4


R.T.: 7.512 min
Delta R.T.: -0.006 min
Response: 4317662
Conc: 67.66 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

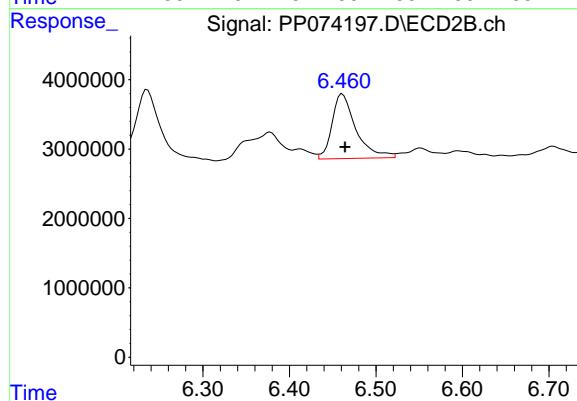


#29 AR-1254-4

R.T.: 6.461 min
Delta R.T.: -0.003 min
Response: 17873856
Conc: 48.63 ng/ml

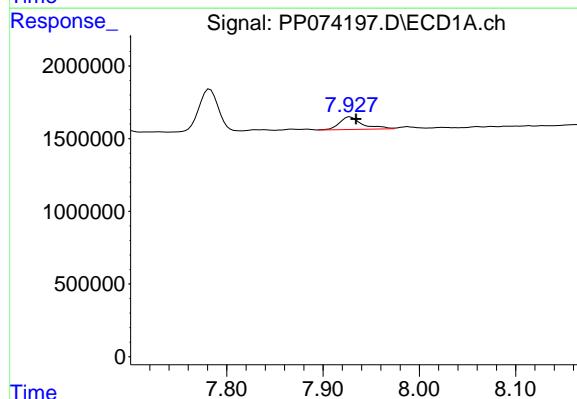


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.006 min
Response: 1449445
Conc: 17.86 ng/ml

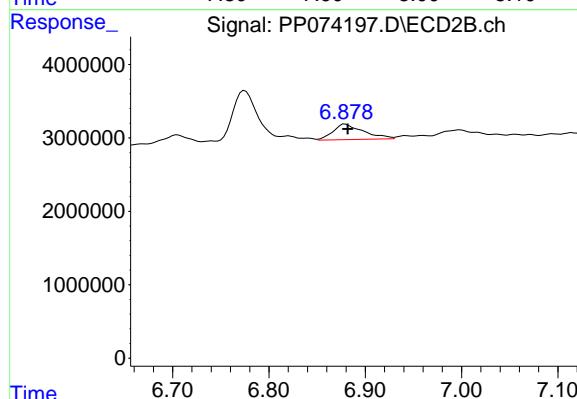

#30 AR-1254-5


R.T.: 6.879 min
Delta R.T.: -0.003 min
Response: 4651318
Conc: 11.83 ng/ml

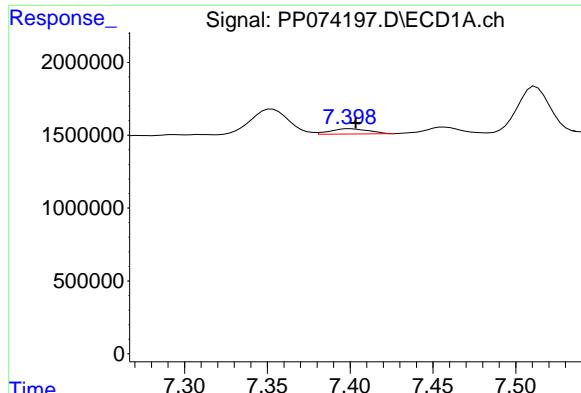

#31 AR-1260-1


R.T.: 7.400 min
Delta R.T.: -0.004 min
Response: 593868
Conc: 10.54 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

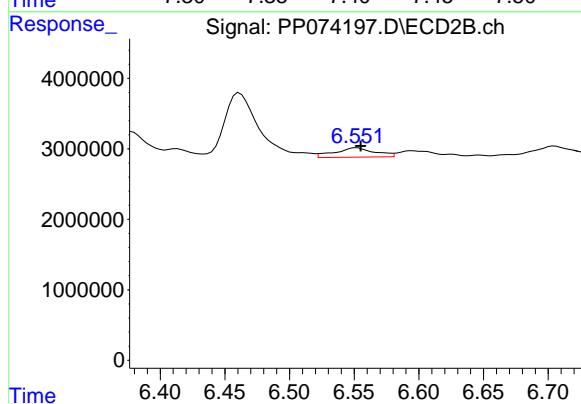


#31 AR-1260-1

R.T.: 6.552 min
Delta R.T.: -0.003 min
Response: 2870221
Conc: 7.11 ng/ml

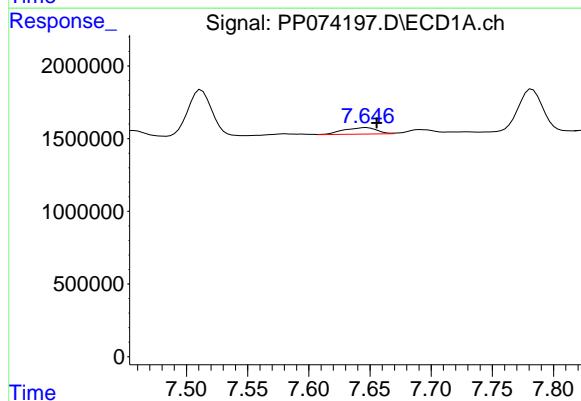


#32 AR-1260-2

R.T.: 7.647 min
Delta R.T.: -0.008 min
Response: 839562
Conc: 12.32 ng/ml

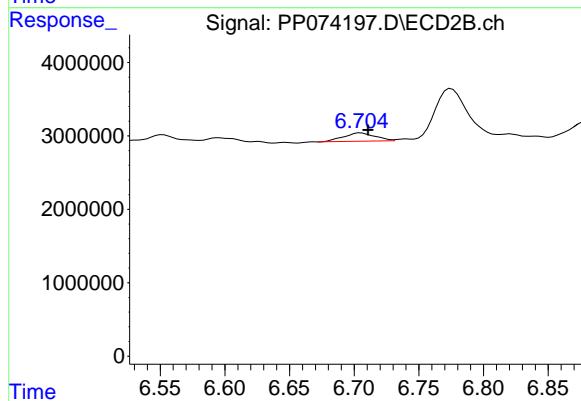

#32 AR-1260-2

R.T.: 6.705 min
Delta R.T.: -0.006 min
Response: 1902548
Conc: 6.08 ng/ml

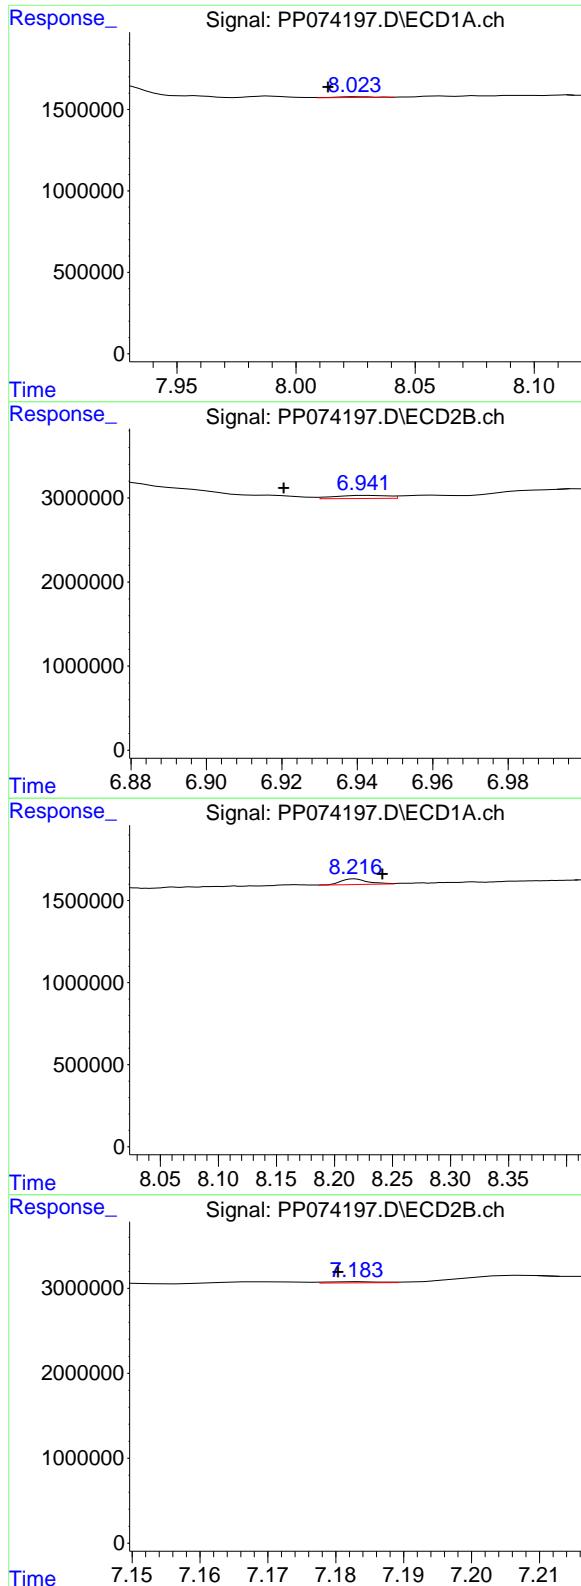

#33 AR-1260-3

R.T.: 8.025 min
 Delta R.T.: 0.011 min
 Response: 47683
 Conc: 0.89 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

#33 AR-1260-3


R.T.: 6.943 min
 Delta R.T.: 0.022 min
 Response: 370567
 Conc: 0.94 ng/ml

#34 AR-1260-4

R.T.: 8.217 min
 Delta R.T.: -0.024 min
 Response: 560766
 Conc: 8.96 ng/ml

#34 AR-1260-4

R.T.: 7.184 min
 Delta R.T.: 0.004 min
 Response: 72352
 Conc: 0.25 ng/ml

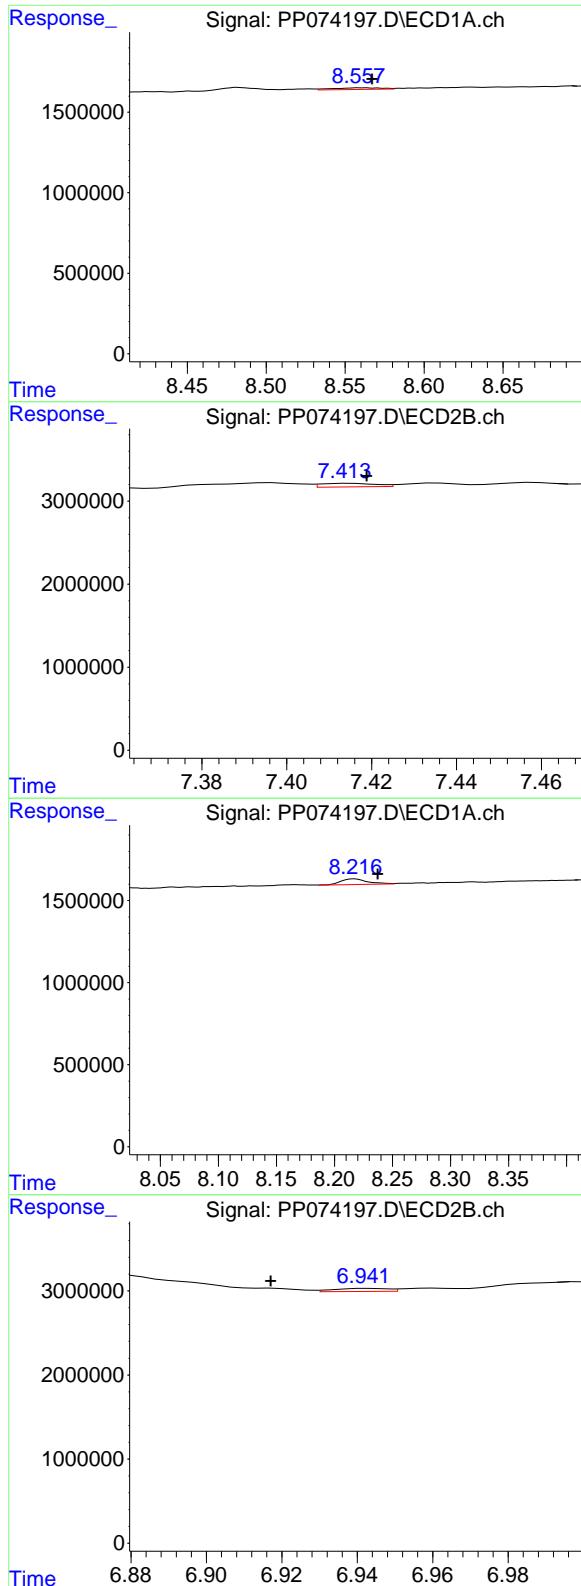

#35 AR-1260-5

R.T.: 8.559 min
 Delta R.T.: -0.008 min
 Response: 212917
 Conc: 1.88 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#35 AR-1260-5


R.T.: 7.415 min
 Delta R.T.: -0.004 min
 Response: 384725
 Conc: 0.51 ng/ml

#36 AR-1262-1

R.T.: 8.217 min
 Delta R.T.: -0.020 min
 Response: 560766
 Conc: 7.40 ng/ml

#36 AR-1262-1


R.T.: 6.943 min
 Delta R.T.: 0.026 min
 Response: 370567
 Conc: 0.66 ng/ml

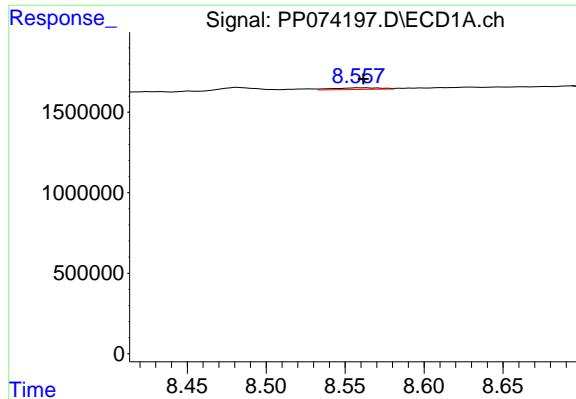

#37 AR-1262-2


R.T.: 8.559 min
Delta R.T.: -0.003 min
Response: 212917
Conc: 1.63 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

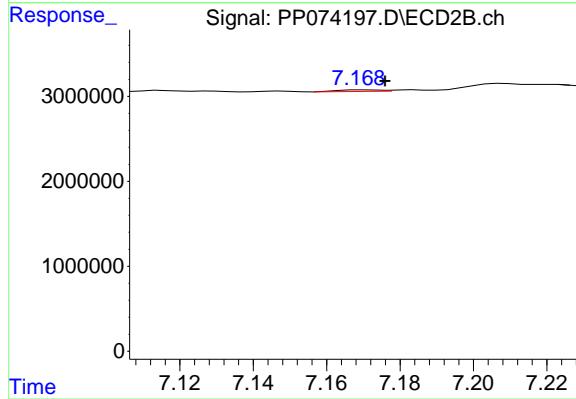


#37 AR-1262-2

R.T.: 7.170 min
Delta R.T.: -0.006 min
Response: 147921
Conc: 0.37 ng/ml

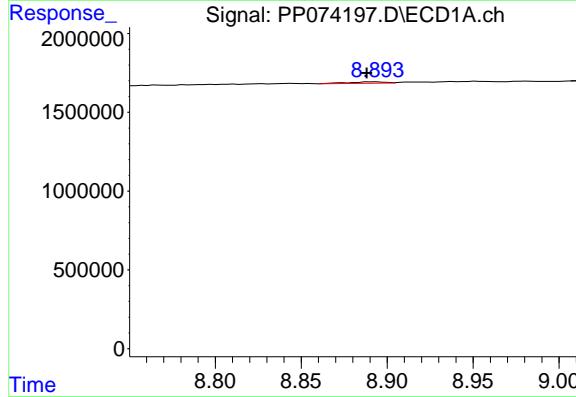


#38 AR-1262-3

R.T.: 8.894 min
Delta R.T.: 0.006 min
Response: 131960
Conc: 1.40 ng/ml

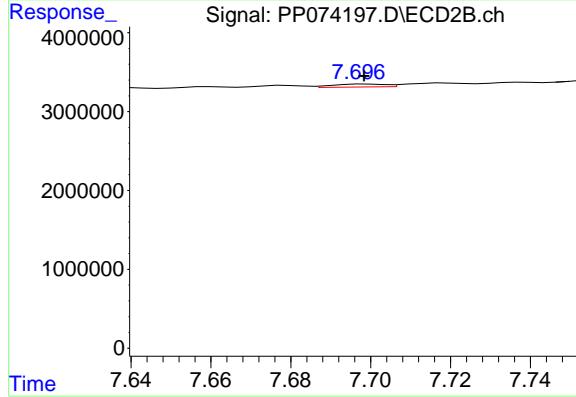

#38 AR-1262-3

R.T.: 7.699 min
Delta R.T.: 0.000 min
Response: 339738
Conc: 0.95 ng/ml

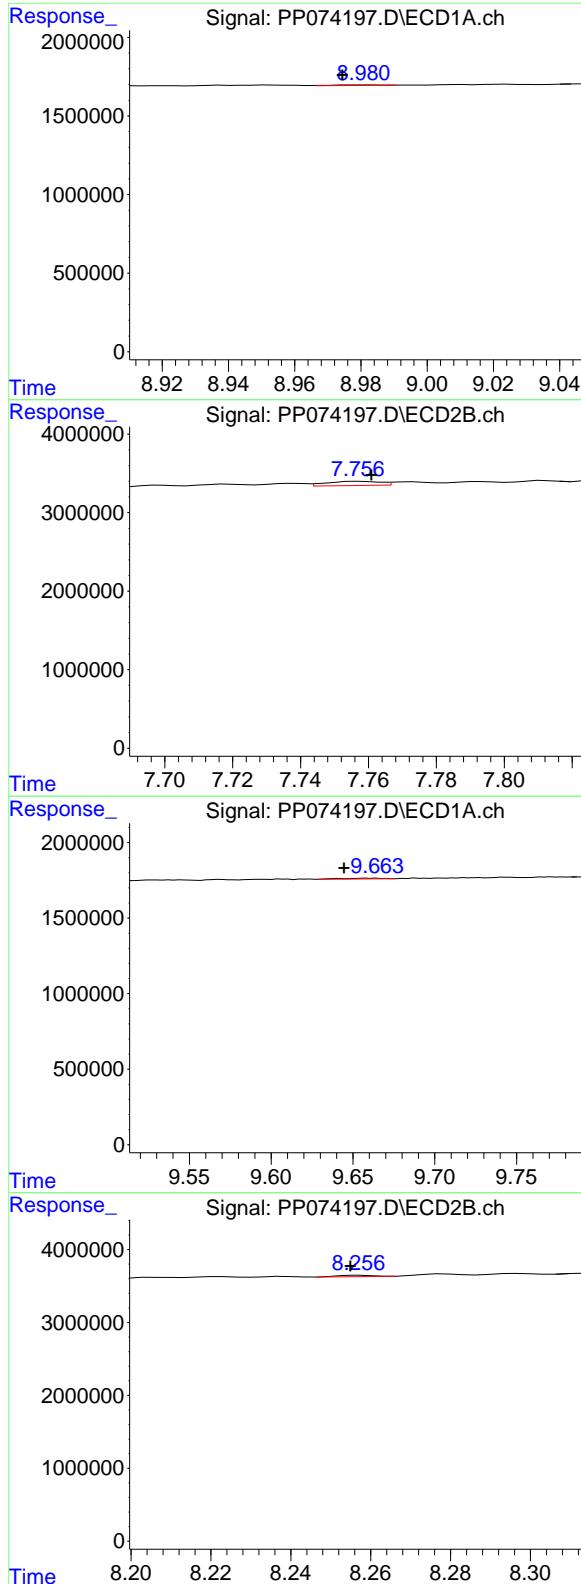

#39 AR-1262-4

R.T.: 8.981 min
 Delta R.T.: 0.007 min
 Response: 35860
 Conc: 0.49 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#39 AR-1262-4


R.T.: 7.758 min
 Delta R.T.: -0.003 min
 Response: 593683
 Conc: 0.89 ng/ml

#40 AR-1262-5

R.T.: 9.662 min
 Delta R.T.: 0.018 min
 Response: 83218
 Conc: 1.63 ng/ml

#40 AR-1262-5

R.T.: 8.258 min
 Delta R.T.: 0.003 min
 Response: 116580
 Conc: 0.41 ng/ml

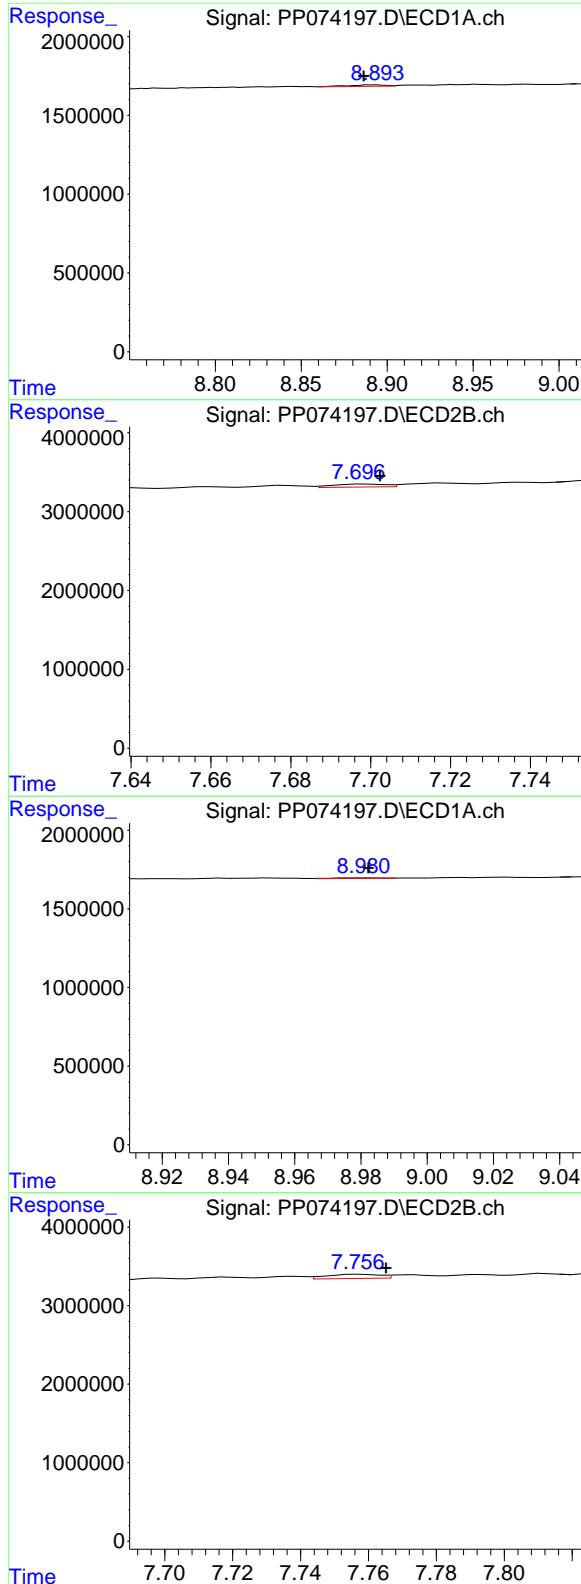

#41 AR-1268-1

R.T.: 8.894 min
 Delta R.T.: 0.008 min
 Response: 131960
 Conc: 0.85 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#41 AR-1268-1


R.T.: 7.699 min
 Delta R.T.: -0.004 min
 Response: 339738
 Conc: 0.31 ng/ml

#42 AR-1268-2

R.T.: 8.981 min
 Delta R.T.: -0.001 min
 Response: 35860
 Conc: 0.25 ng/ml

#42 AR-1268-2

R.T.: 7.758 min
 Delta R.T.: -0.008 min
 Response: 593683
 Conc: 0.56 ng/ml

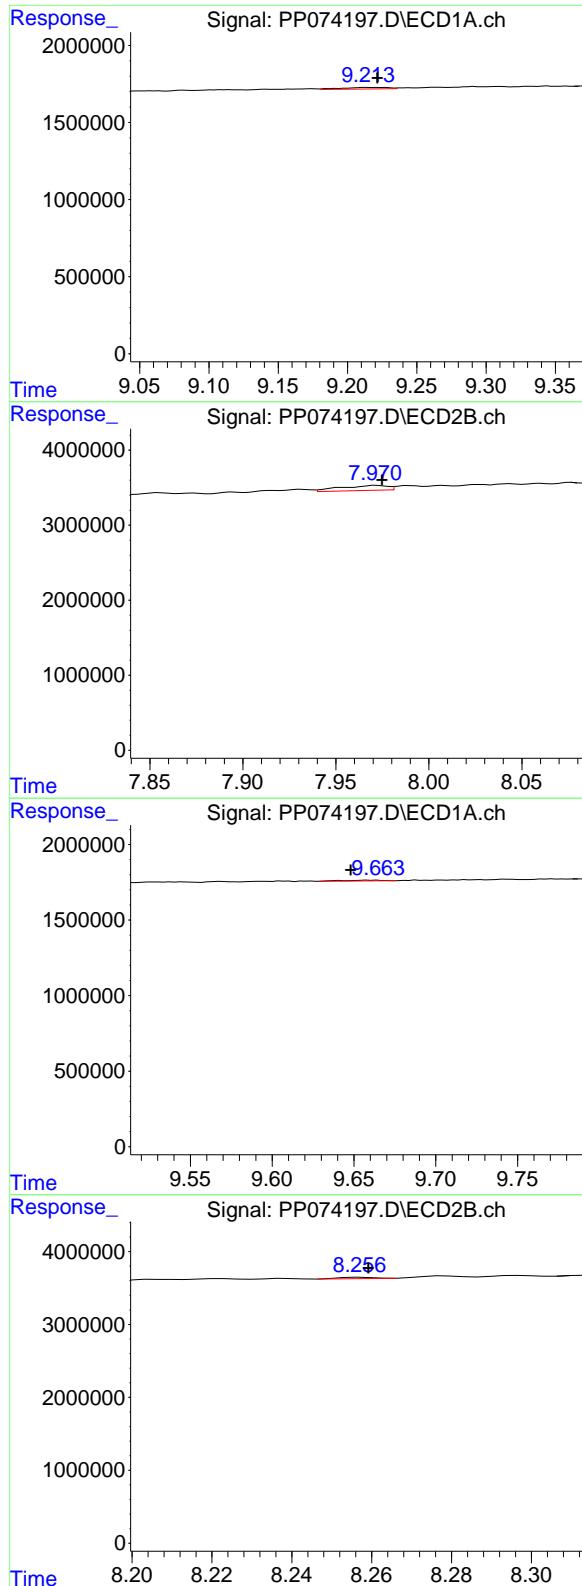

#43 AR-1268-3

R.T.: 9.214 min
 Delta R.T.: -0.007 min
 Response: 255483
 Conc: 2.14 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1242

#43 AR-1268-3


R.T.: 7.972 min
 Delta R.T.: -0.003 min
 Response: 1184209
 Conc: 1.42 ng/ml

#44 AR-1268-4

R.T.: 9.662 min
 Delta R.T.: 0.014 min
 Response: 83218
 Conc: 1.41 ng/ml

#44 AR-1268-4


R.T.: 8.258 min
 Delta R.T.: -0.001 min
 Response: 116580
 Conc: 0.38 ng/ml

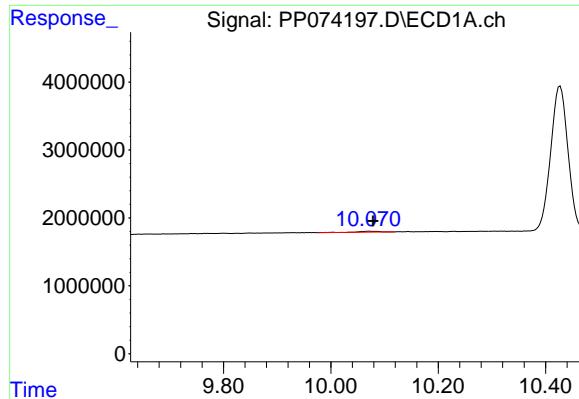

#45 AR-1268-5

R.T.: 10.072 min
Delta R.T.: -0.007 min
Response: 363528
Conc: 1.03 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1242

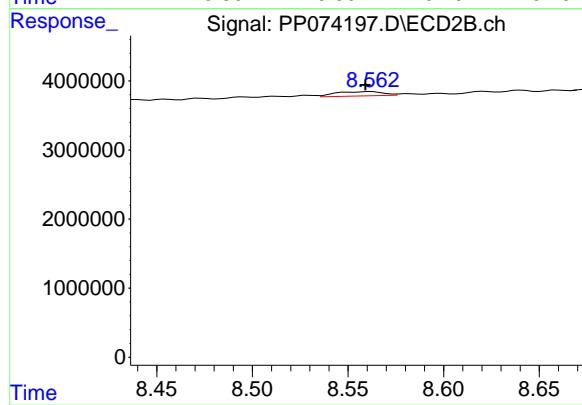

#45 AR-1268-5

R.T.: 8.563 min
Delta R.T.: 0.003 min
Response: 1086905
Conc: 0.43 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 23:10
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:37:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.656 | 3.803 | 53831323 | 191.6E6 | 48.137 | 49.971 |
| 2) SA Decachlor... | 10.430 | 8.820 | 47450930 | 299.2E6 | 48.860 | 49.761 |

Target Compounds

| | | | | | | |
|------------------|-------|--------|----------|----------|----------|------------|
| 3) L1 AR-1016-1 | 5.805 | 4.893 | 745970 | 3731555 | 18.081 | 9.355 # |
| 4) L1 AR-1016-2 | 5.830 | 4.957 | 872142 | 1734023 | 14.358 | 9.233 # |
| 5) L1 AR-1016-3 | 5.893 | 5.078 | 556819 | 966758 | 14.040 | 9.114 # |
| 6) L1 AR-1016-4 | 5.988 | 5.121 | 527061 | 57719879 | 16.195 | 528.473 # |
| 7) L1 AR-1016-5 | 6.280 | 5.333 | 9175288 | 35534075 | 282.594 | 303.805 |
| 8) L2 AR-1221-1 | 4.848 | 4.021 | 78676 | 154196 | 4.693 | 3.141 # |
| 9) L2 AR-1221-2 | 4.957 | 4.100 | 993840 | 2037869 | 78.870 | 56.782 # |
| 10) L2 AR-1221-3 | 5.016 | 4.173 | 244539 | 504753 | 6.675 | 3.733 # |
| 11) L3 AR-1232-1 | 5.016 | 4.173 | 244539 | 504753 | 8.422 | 4.980 # |
| 12) L3 AR-1232-2 | 5.542 | 4.893 | 289072 | 3731555 | 19.217 | 21.413 |
| 13) L3 AR-1232-3 | 5.830 | 5.078 | 872142 | 966758 | 30.072 | 21.101 # |
| 14) L3 AR-1232-4 | 5.988 | 5.157 | 527061 | 26883268 | 34.072 | 463.419 # |
| 15) L3 AR-1232-5 | 6.077 | 5.333 | 14812614 | 35534075 | 1264.305 | 756.375 # |
| 16) L4 AR-1242-1 | 5.805 | 4.893 | 745970 | 3731555 | 20.018 | 10.812 # |
| 17) L4 AR-1242-2 | 5.830 | 4.957 | 872142 | 1734023 | 16.029 | 10.614 # |
| 18) L4 AR-1242-3 | 5.893 | 5.078 | 556819 | 966758 | 15.582 | 10.480 # |
| 19) L4 AR-1242-4 | 5.988 | 5.157 | 527061 | 26883268 | 18.039 | 225.112 # |
| 20) L4 AR-1242-5 | 6.721 | 5.686 | 10174999 | 178.5E6 | 286.152 | 1193.575 # |
| 21) L5 AR-1248-1 | 5.805 | 4.893 | 745970 | 3731555 | 26.628 | 17.443 # |
| 22) L5 AR-1248-2 | 6.077 | 5.121 | 14812614 | 57719879 | 367.914 | 394.497 |
| 23) L5 AR-1248-3 | 6.280 | 5.157 | 9175288 | 26883268 | 205.846 | 156.790 |
| 24) L5 AR-1248-4 | 6.655 | 5.333 | 37990866 | 35534075 | 730.072 | 213.580 # |
| 25) L5 AR-1248-5 | 6.721 | 5.686f | 10174999 | 178.5E6 | 178.687 | 613.512 # |
| 26) L6 AR-1254-1 | 6.655 | 5.686 | 37990866 | 178.5E6 | 721.697 | 487.493 # |
| 27) L6 AR-1254-2 | 6.871 | 5.833 | 37599140 | 134.8E6 | 472.918 | 484.650 |
| 28) L6 AR-1254-3 | 7.233 | 6.235 | 40597005 | 245.2E6 | 464.942 | 501.115 |
| 29) L6 AR-1254-4 | 7.514 | 6.462 | 30708926 | 181.0E6 | 481.260 | 492.525 |
| 30) L6 AR-1254-5 | 7.930 | 6.878 | 38809795 | 188.2E6 | 478.279 | 478.748 |
| 31) L7 AR-1260-1 | 7.398 | 6.552 | 17543251 | 109.0E6 | 311.293 | 269.954 |
| 32) L7 AR-1260-2 | 7.650 | 6.704 | 19124212 | 77042973 | 280.610 | 246.381 |
| 33) L7 AR-1260-3 | 7.991 | 6.944 | 4844847 | 25122989 | 90.905 | 63.745 # |
| 34) L7 AR-1260-4 | 8.219 | 7.175 | 14487782 | 5653722 | 231.379 | 19.430 # |
| 35) L7 AR-1260-5 | 8.560 | 7.407 | 5145410 | 51502946 | 45.412 | 67.999 # |
| 36) L8 AR-1262-1 | 8.219 | 6.944 | 14487782 | 25122989 | 191.158 | 44.612 # |
| 37) L8 AR-1262-2 | 8.560 | 7.175 | 5145410 | 5653722 | 39.450 | 14.098 # |
| 38) L8 AR-1262-3 | 8.895 | 7.694 | 4365480 | 772104 | 46.406 | 2.148 # |
| 39) L8 AR-1262-4 | 8.979 | 7.757 | 118980 | 19007753 | 1.633 | 28.501 # |
| 40) L8 AR-1262-5 | 9.647 | 8.249 | 418724 | 666817 | 8.223 | 2.354 # |
| 41) L9 AR-1268-1 | 8.895 | 7.709 | 4365480 | 477278 | 28.050 | 0.438 # |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 23:10
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
ICVPP080125AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:37:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|--------|-------|--------|----------|-------|----------|
| 42) L9 AR-1268-2 | 8.979 | 7.757 | 118980 | 19007753 | 0.830 | 17.909 # |
| 43) L9 AR-1268-3 | 9.221 | 7.968 | 168840 | 472836 | 1.413 | 0.568 # |
| 44) L9 AR-1268-4 | 9.647 | 8.263 | 418724 | 437922 | 7.120 | 1.422 # |
| 45) L9 AR-1268-5 | 10.069 | 8.559 | 442219 | 1401468 | 1.257 | 0.550 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP080125\
 Data File : PP074199.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Aug 2025 23:10
 Operator : YP\AJ
 Sample : AR1254ICV500
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 ICVPP080125AR1254

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 02 01:37:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Sat Aug 02 01:33:31 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

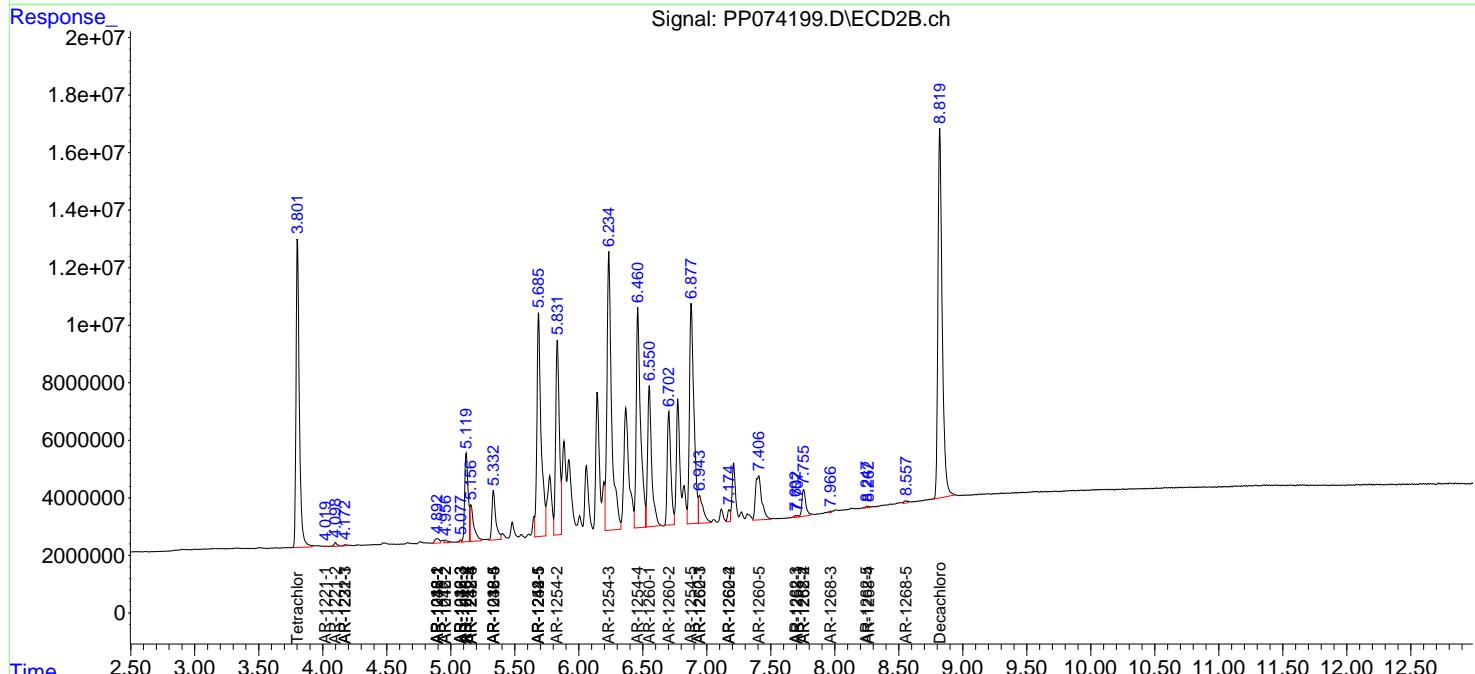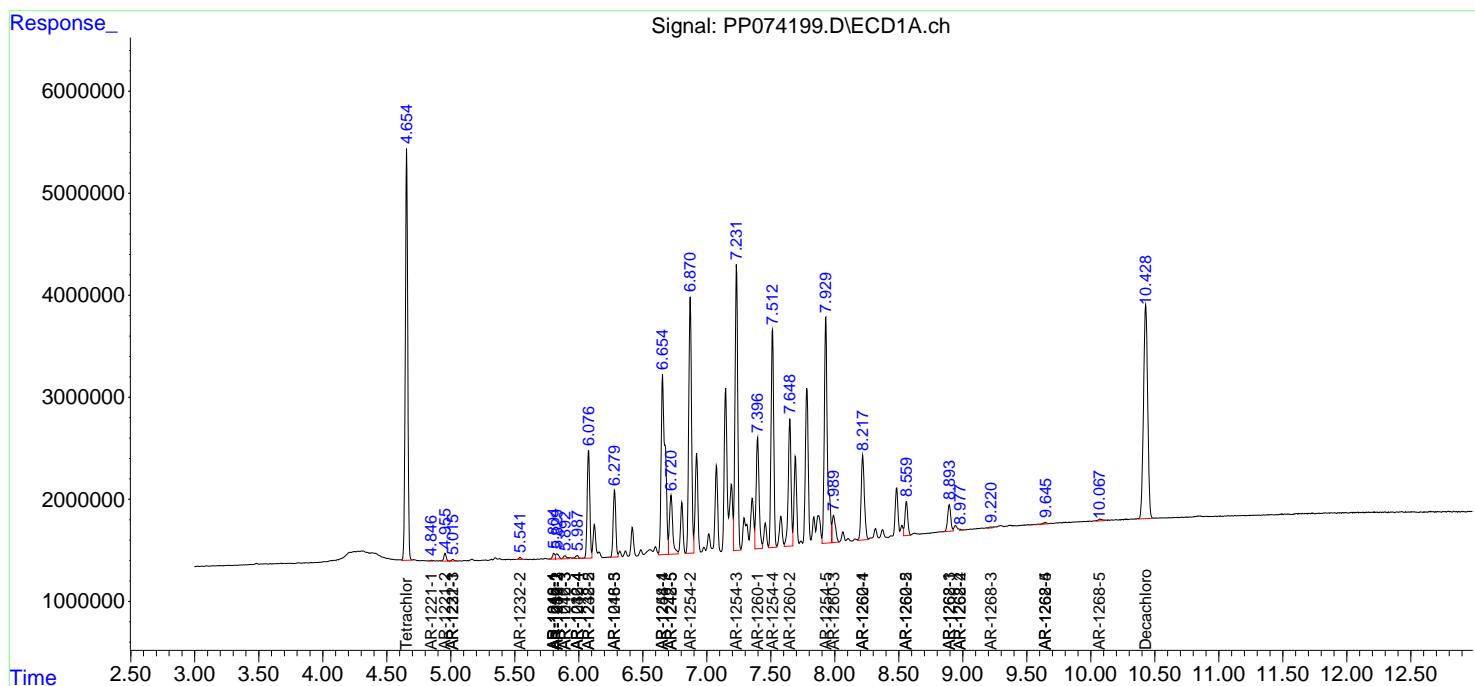




#1 Tetrachloro-m-xylene


R.T.: 4.656 min
Delta R.T.: -0.004 min
Response: 53831323
Conc: 48.14 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

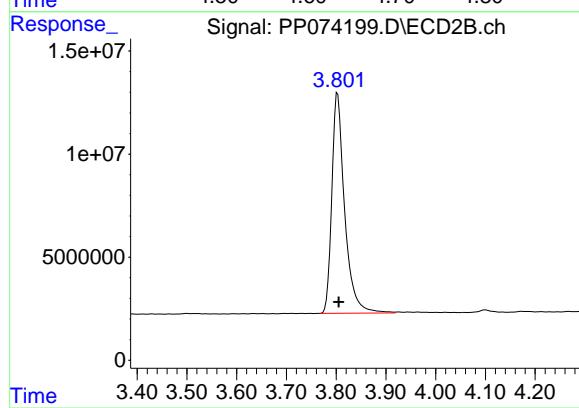


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: -0.002 min
Response: 191609515
Conc: 49.97 ng/ml

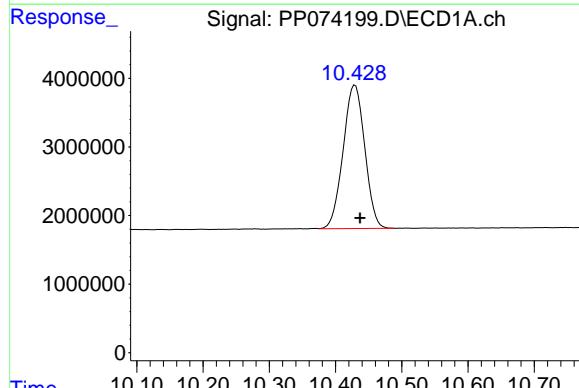


#2 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: -0.008 min
Response: 47450930
Conc: 48.86 ng/ml

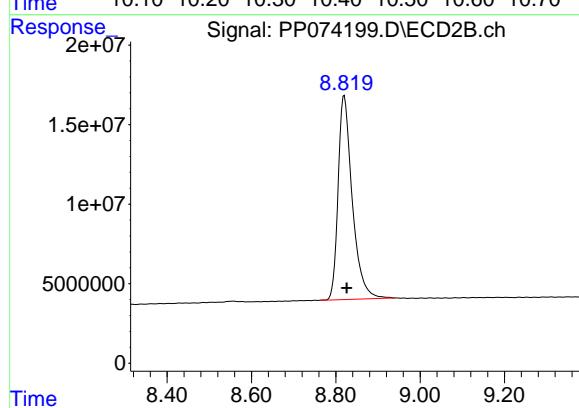

#2 Decachlorobiphenyl


R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 299243051
Conc: 49.76 ng/ml

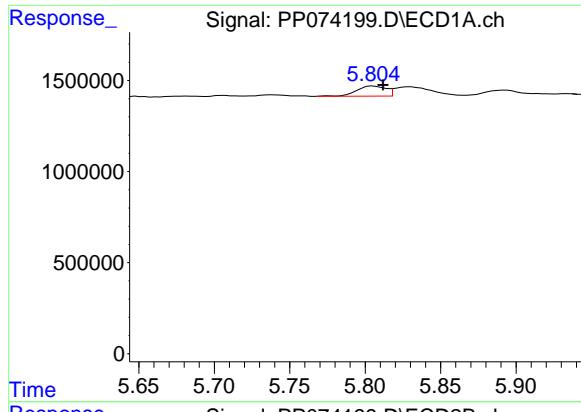

#3 AR-1016-1


R.T.: 5.805 min
Delta R.T.: -0.007 min
Response: 745970
Conc: 18.08 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

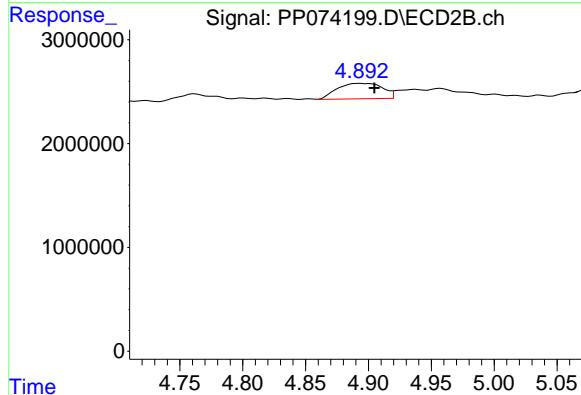


#3 AR-1016-1

R.T.: 4.893 min
Delta R.T.: -0.011 min
Response: 3731555
Conc: 9.35 ng/ml

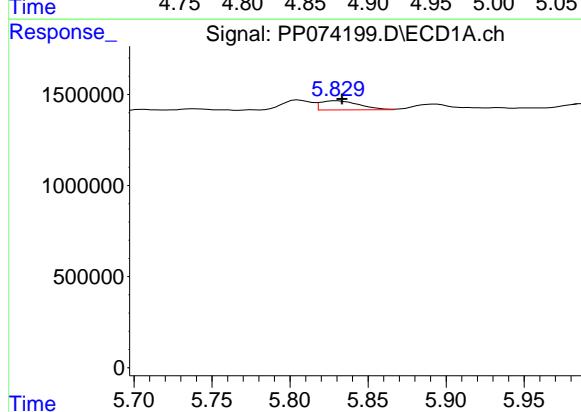


#4 AR-1016-2

R.T.: 5.830 min
Delta R.T.: -0.003 min
Response: 872142
Conc: 14.36 ng/ml

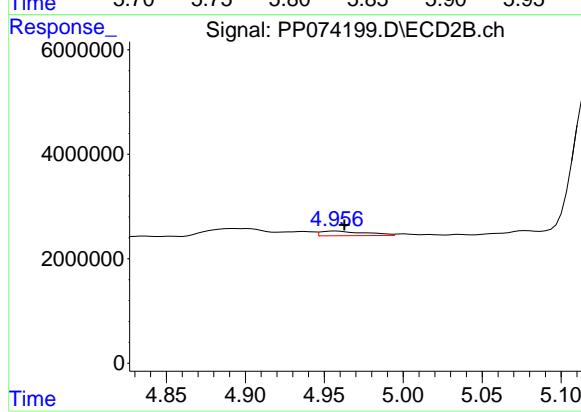

#4 AR-1016-2

R.T.: 4.957 min
Delta R.T.: -0.005 min
Response: 1734023
Conc: 9.23 ng/ml

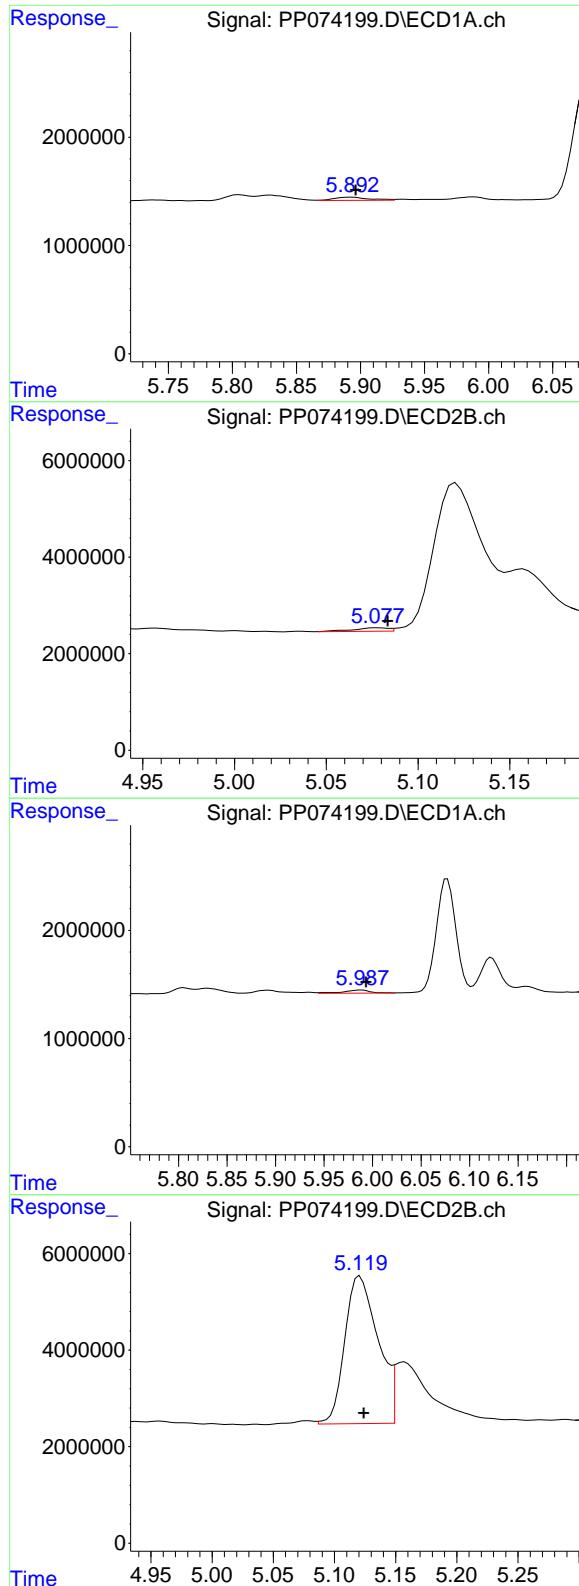

#5 AR-1016-3

R.T.: 5.893 min
 Delta R.T.: -0.003 min
 Response: 556819
 Conc: 14.04 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#5 AR-1016-3


R.T.: 5.078 min
 Delta R.T.: -0.006 min
 Response: 966758
 Conc: 9.11 ng/ml

#6 AR-1016-4

R.T.: 5.988 min
 Delta R.T.: -0.005 min
 Response: 527061
 Conc: 16.20 ng/ml

#6 AR-1016-4


R.T.: 5.121 min
 Delta R.T.: -0.003 min
 Response: 57719879
 Conc: 528.47 ng/ml

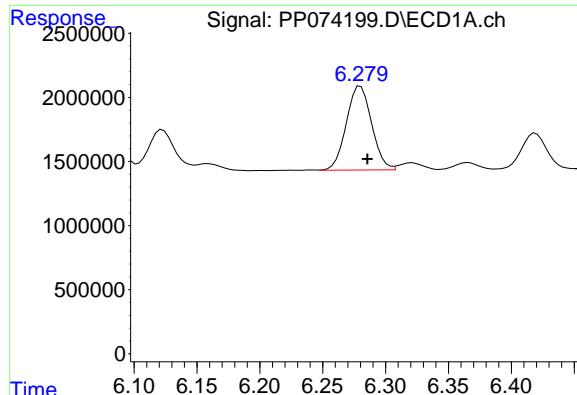

#7 AR-1016-5


R.T.: 6.280 min
 Delta R.T.: -0.005 min
 Response: 9175288
 Conc: 282.59 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

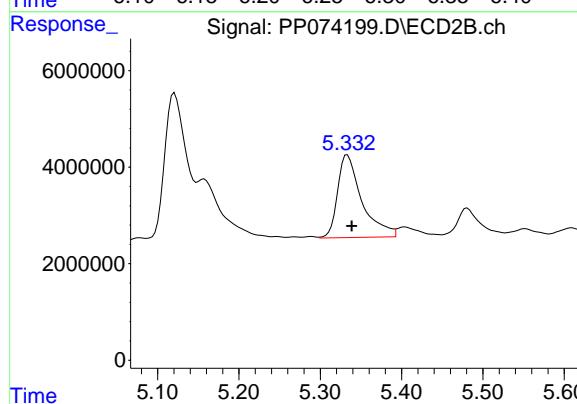


#7 AR-1016-5

R.T.: 5.333 min
 Delta R.T.: -0.005 min
 Response: 35534075
 Conc: 303.81 ng/ml

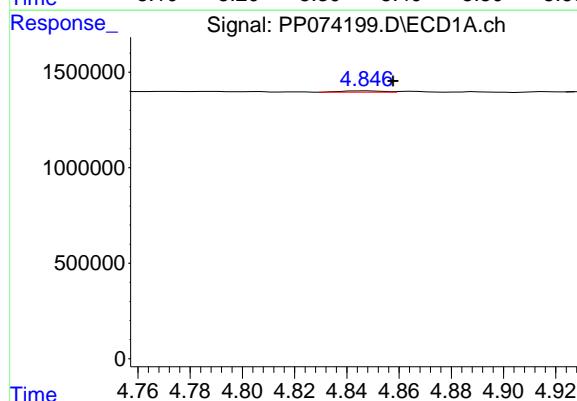


#8 AR-1221-1

R.T.: 4.848 min
 Delta R.T.: -0.010 min
 Response: 78676
 Conc: 4.69 ng/ml

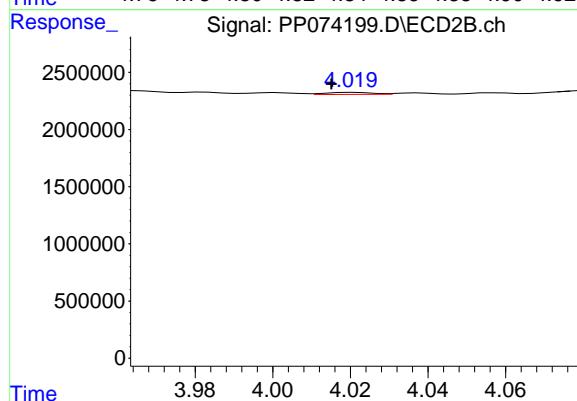

#8 AR-1221-1


R.T.: 4.021 min
 Delta R.T.: 0.006 min
 Response: 154196
 Conc: 3.14 ng/ml

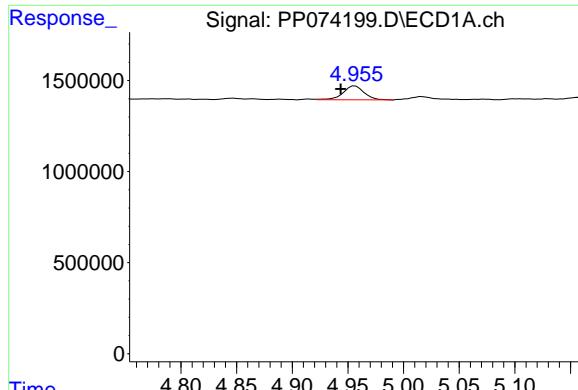

#9 AR-1221-2


R.T.: 4.957 min
Delta R.T.: 0.013 min
Response: 993840
Conc: 78.87 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

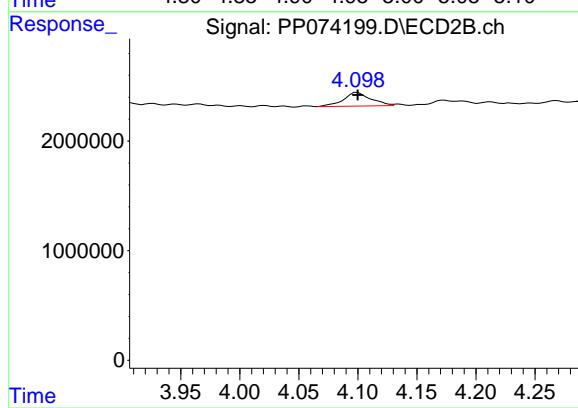


#9 AR-1221-2

R.T.: 4.100 min
Delta R.T.: 0.000 min
Response: 2037869
Conc: 56.78 ng/ml

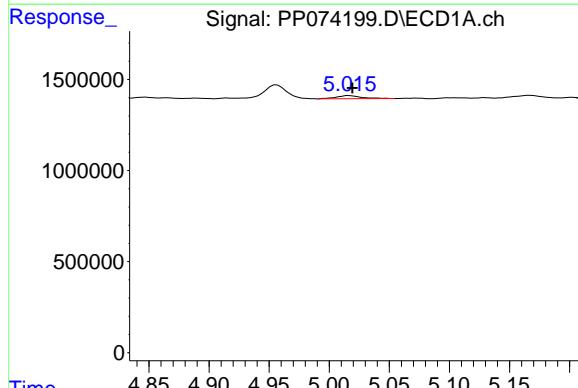


#10 AR-1221-3

R.T.: 5.016 min
Delta R.T.: -0.003 min
Response: 244539
Conc: 6.67 ng/ml

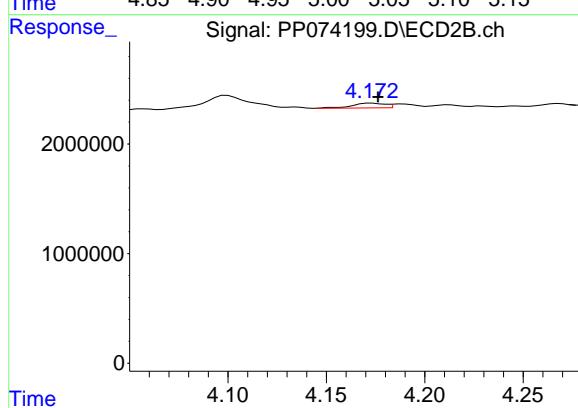

#10 AR-1221-3

R.T.: 4.173 min
Delta R.T.: -0.003 min
Response: 504753
Conc: 3.73 ng/ml

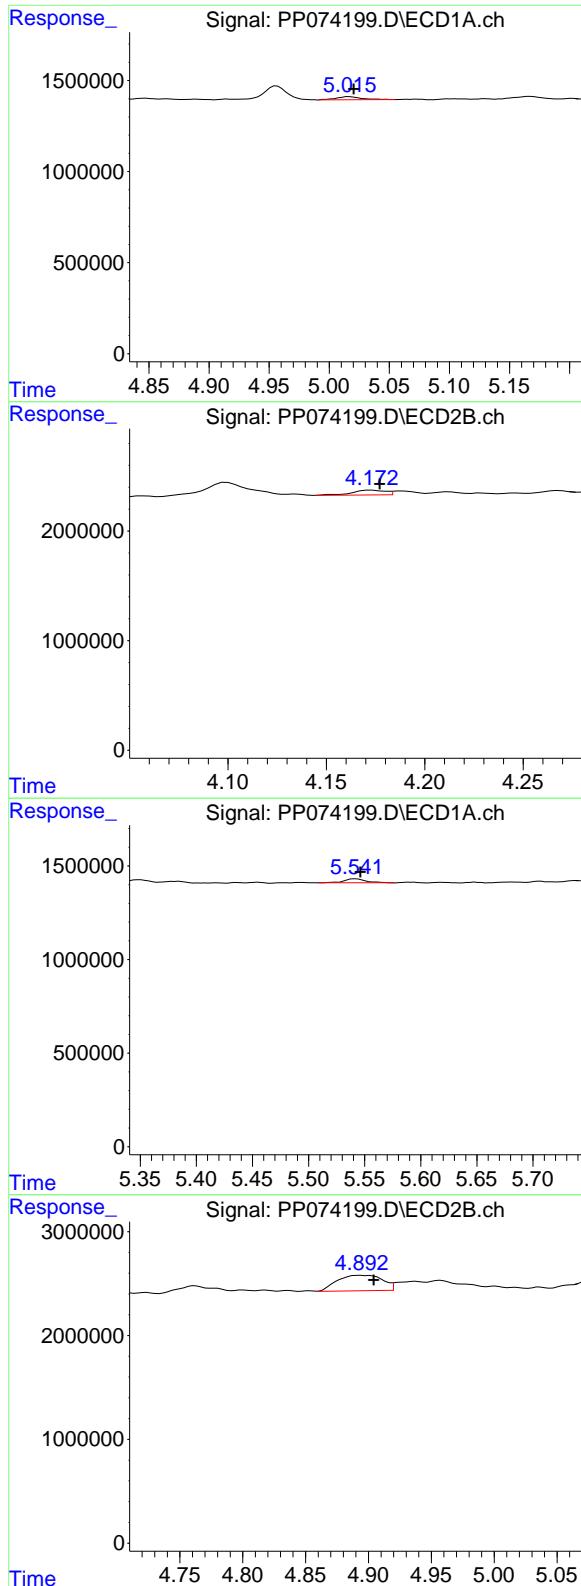

#11 AR-1232-1

R.T.: 5.016 min
 Delta R.T.: -0.004 min
 Response: 244539
 Conc: 8.42 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#11 AR-1232-1


R.T.: 4.173 min
 Delta R.T.: -0.004 min
 Response: 504753
 Conc: 4.98 ng/ml

#12 AR-1232-2

R.T.: 5.542 min
 Delta R.T.: -0.004 min
 Response: 289072
 Conc: 19.22 ng/ml

#12 AR-1232-2

R.T.: 4.893 min
 Delta R.T.: -0.011 min
 Response: 3731555
 Conc: 21.41 ng/ml

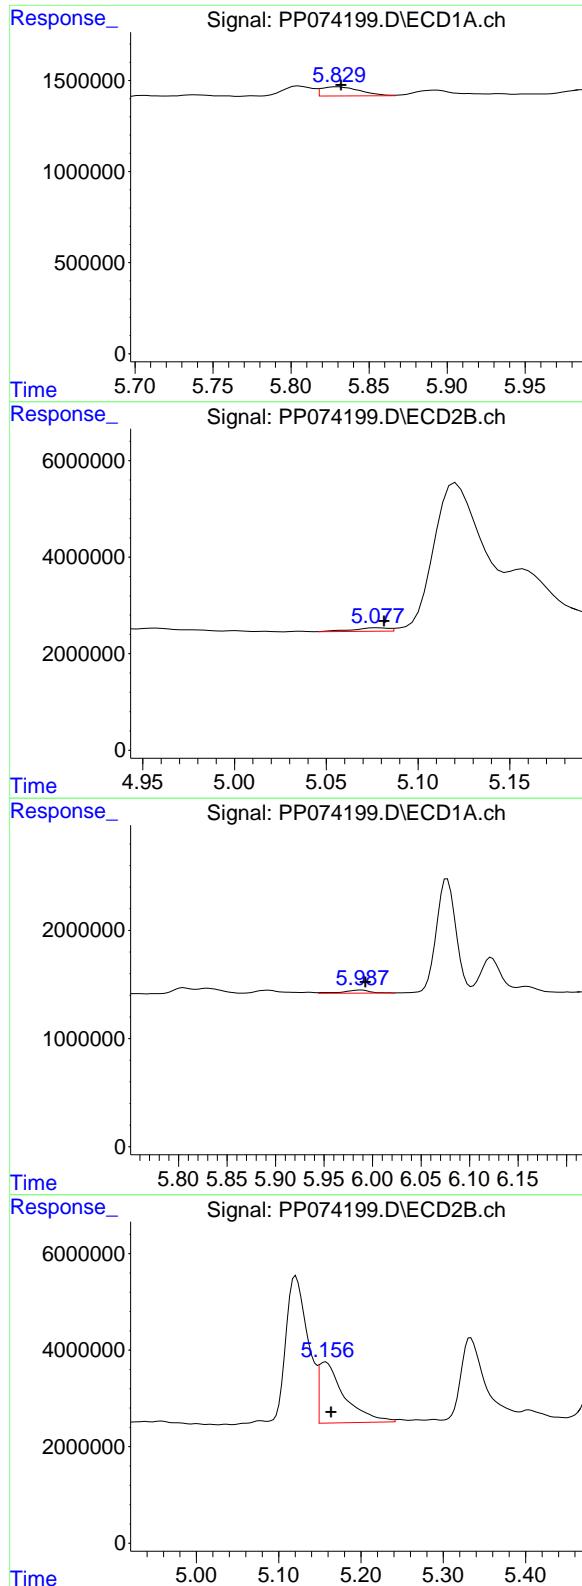

#13 AR-1232-3

R.T.: 5.830 min
 Delta R.T.: -0.002 min
 Response: 872142
 Conc: 30.07 ng/ml

Instrument: ECD_P
 ClientSampleId: ICPP080125AR1254

#13 AR-1232-3


R.T.: 5.078 min
 Delta R.T.: -0.003 min
 Response: 966758
 Conc: 21.10 ng/ml

#14 AR-1232-4

R.T.: 5.988 min
 Delta R.T.: -0.004 min
 Response: 527061
 Conc: 34.07 ng/ml

#14 AR-1232-4


R.T.: 5.157 min
 Delta R.T.: -0.006 min
 Response: 26883268
 Conc: 463.42 ng/ml



#15 AR-1232-5


R.T.: 6.077 min
 Delta R.T.: -0.005 min
 Response: 14812614
 Conc: 1264.31 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

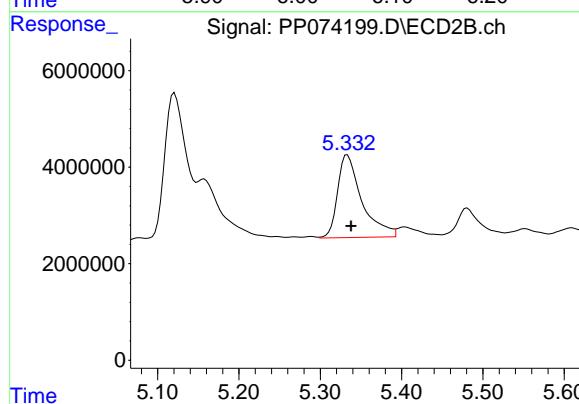


#15 AR-1232-5

R.T.: 5.333 min
 Delta R.T.: -0.004 min
 Response: 35534075
 Conc: 756.37 ng/ml

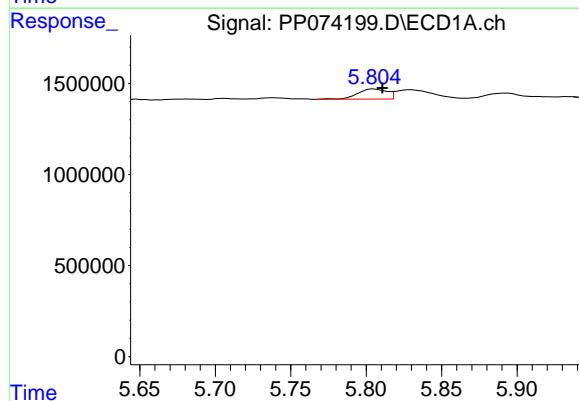


#16 AR-1242-1

R.T.: 5.805 min
 Delta R.T.: -0.006 min
 Response: 745970
 Conc: 20.02 ng/ml

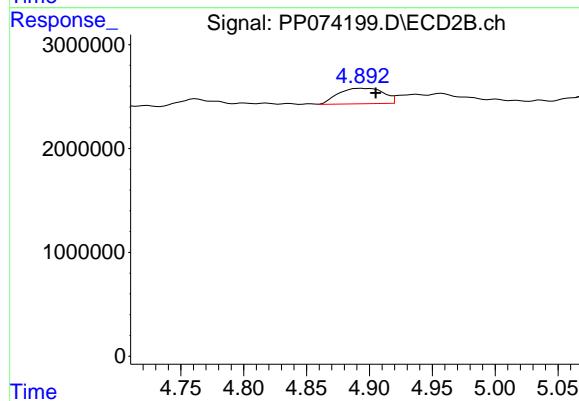

#16 AR-1242-1

R.T.: 4.893 min
 Delta R.T.: -0.012 min
 Response: 3731555
 Conc: 10.81 ng/ml

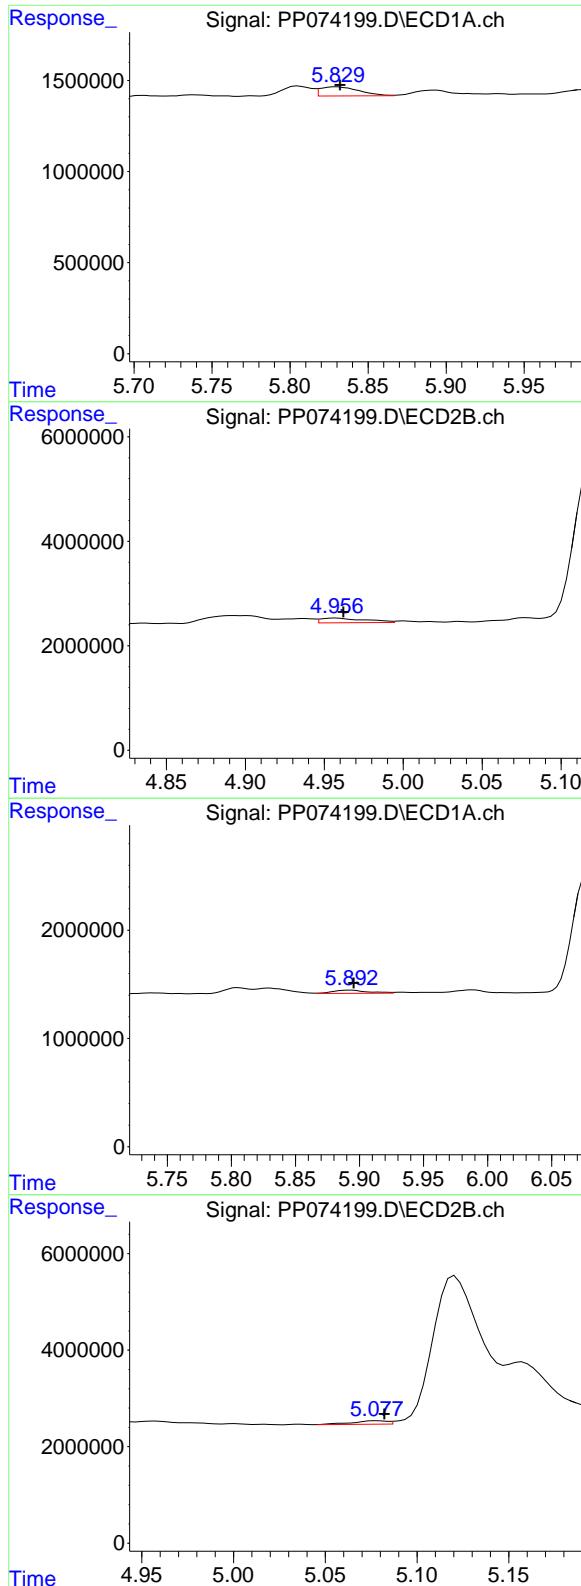

#17 AR-1242-2

R.T.: 5.830 min
 Delta R.T.: -0.002 min
 Response: 872142
 Conc: 16.03 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#17 AR-1242-2


R.T.: 4.957 min
 Delta R.T.: -0.005 min
 Response: 1734023
 Conc: 10.61 ng/ml

#18 AR-1242-3

R.T.: 5.893 min
 Delta R.T.: -0.002 min
 Response: 556819
 Conc: 15.58 ng/ml

#18 AR-1242-3


R.T.: 5.078 min
 Delta R.T.: -0.004 min
 Response: 966758
 Conc: 10.48 ng/ml



#19 AR-1242-4


R.T.: 5.988 min
 Delta R.T.: -0.004 min
 Response: 527061
 Conc: 18.04 ng/ml

Instrument: ECD_P
 ClientSampleId: ICP080125AR1254

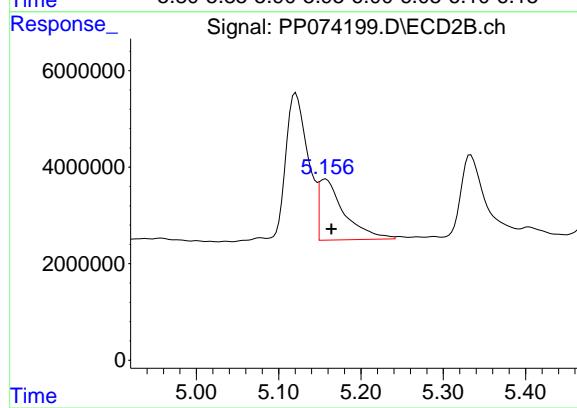


#19 AR-1242-4

R.T.: 5.157 min
 Delta R.T.: -0.007 min
 Response: 26883268
 Conc: 225.11 ng/ml

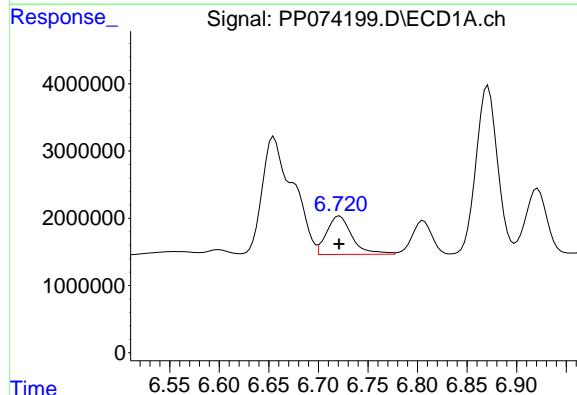


#20 AR-1242-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 10174999
 Conc: 286.15 ng/ml

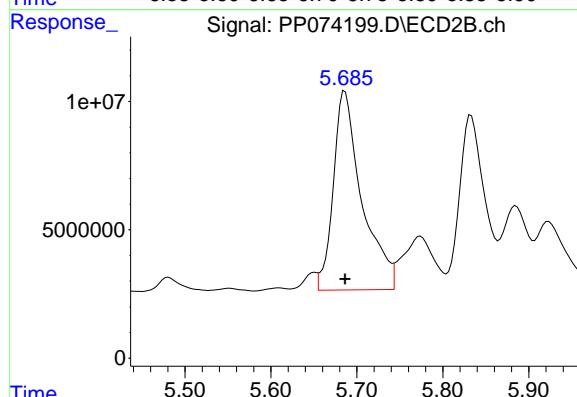

#20 AR-1242-5


R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 178511104
 Conc: 1193.58 ng/ml

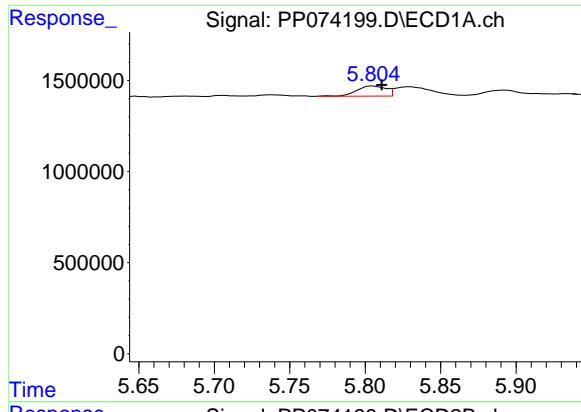

#21 AR-1248-1


R.T.: 5.805 min
Delta R.T.: -0.006 min
Response: 745970
Conc: 26.63 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

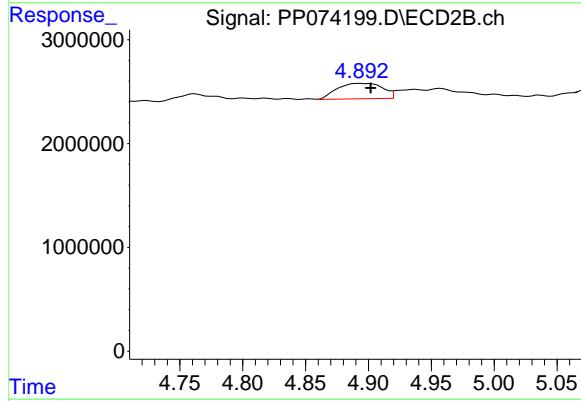


#21 AR-1248-1

R.T.: 4.893 min
Delta R.T.: -0.008 min
Response: 3731555
Conc: 17.44 ng/ml

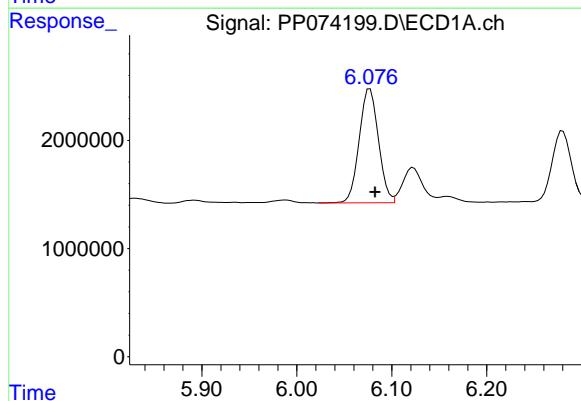


#22 AR-1248-2

R.T.: 6.077 min
Delta R.T.: -0.006 min
Response: 14812614
Conc: 367.91 ng/ml

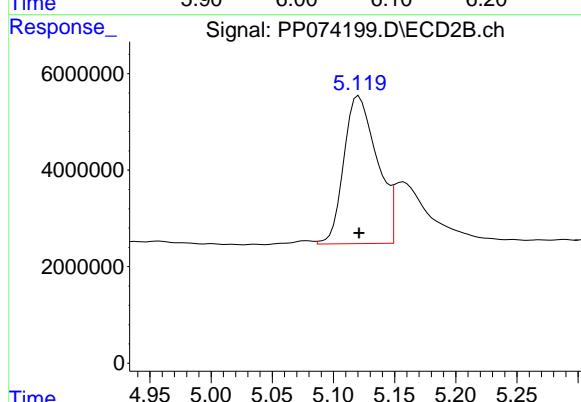

#22 AR-1248-2


R.T.: 5.121 min
Delta R.T.: 0.000 min
Response: 57719879
Conc: 394.50 ng/ml

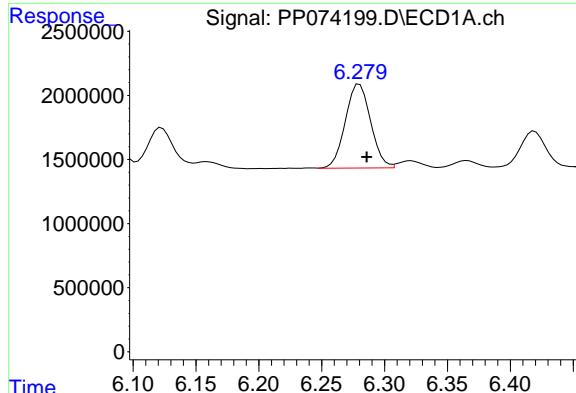

#23 AR-1248-3


R.T.: 6.280 min
 Delta R.T.: -0.006 min
 Response: 9175288
 Conc: 205.85 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

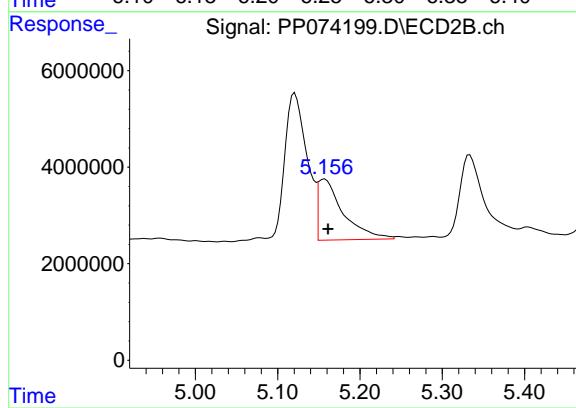


#23 AR-1248-3

R.T.: 5.157 min
 Delta R.T.: -0.004 min
 Response: 26883268
 Conc: 156.79 ng/ml

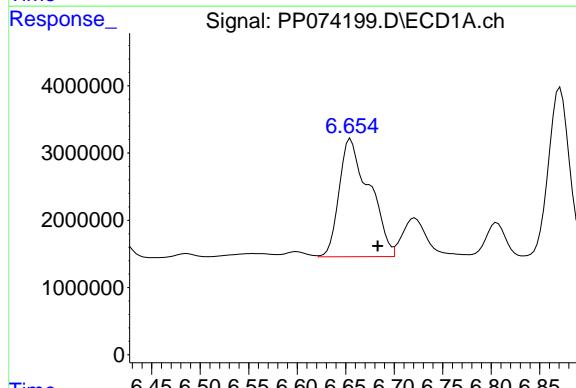


#24 AR-1248-4

R.T.: 6.655 min
 Delta R.T.: -0.028 min
 Response: 37990866
 Conc: 730.07 ng/ml

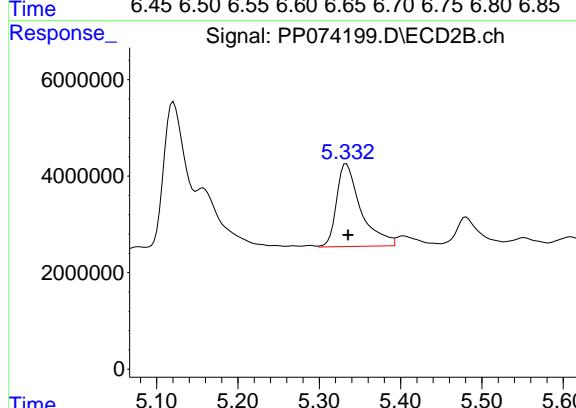

#24 AR-1248-4

R.T.: 5.333 min
 Delta R.T.: -0.002 min
 Response: 35534075
 Conc: 213.58 ng/ml

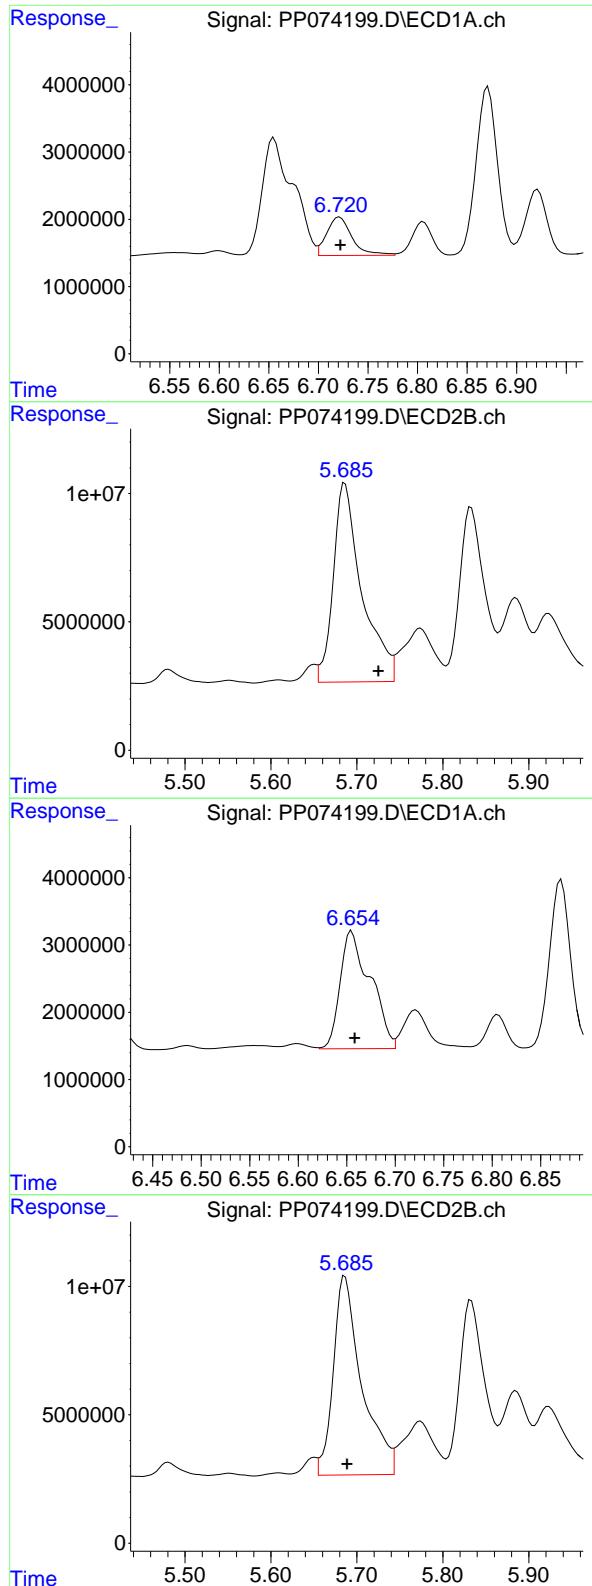

#25 AR-1248-5

R.T.: 6.721 min
 Delta R.T.: -0.001 min
 Response: 10174999
 Conc: 178.69 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#25 AR-1248-5


R.T.: 5.686 min
 Delta R.T.: -0.039 min
 Response: 178511104
 Conc: 613.51 ng/ml

#26 AR-1254-1

R.T.: 6.655 min
 Delta R.T.: -0.003 min
 Response: 37990866
 Conc: 721.70 ng/ml

#26 AR-1254-1


R.T.: 5.686 min
 Delta R.T.: -0.002 min
 Response: 178511104
 Conc: 487.49 ng/ml

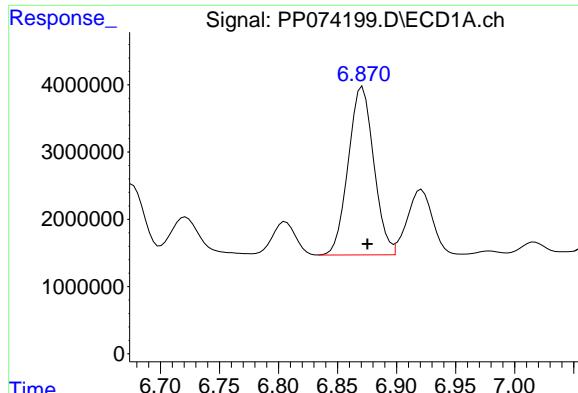

#27 AR-1254-2


R.T.: 6.871 min
 Delta R.T.: -0.004 min
 Response: 37599140
 Conc: 472.92 ng/ml

Instrument : ECD_P
 ClientSampleId : ICVPP080125AR1254

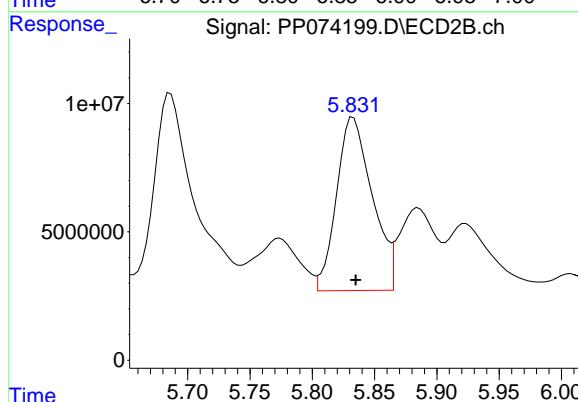


#27 AR-1254-2

R.T.: 5.833 min
 Delta R.T.: -0.002 min
 Response: 134837969
 Conc: 484.65 ng/ml

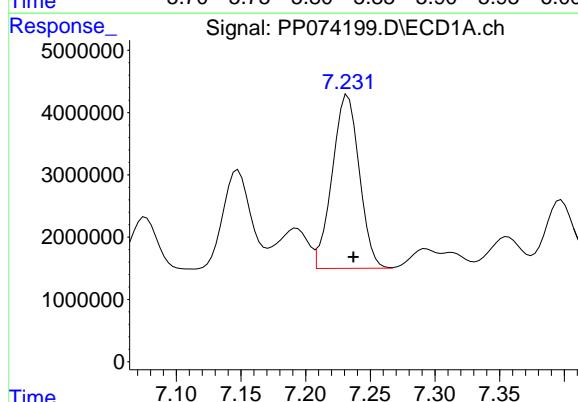


#28 AR-1254-3

R.T.: 7.233 min
 Delta R.T.: -0.004 min
 Response: 40597005
 Conc: 464.94 ng/ml

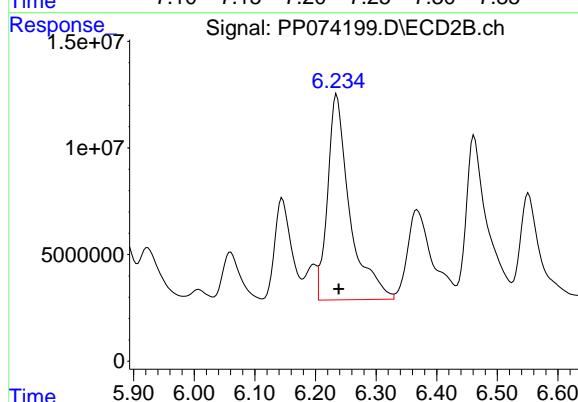

#28 AR-1254-3

R.T.: 6.235 min
 Delta R.T.: -0.003 min
 Response: 245151099
 Conc: 501.11 ng/ml

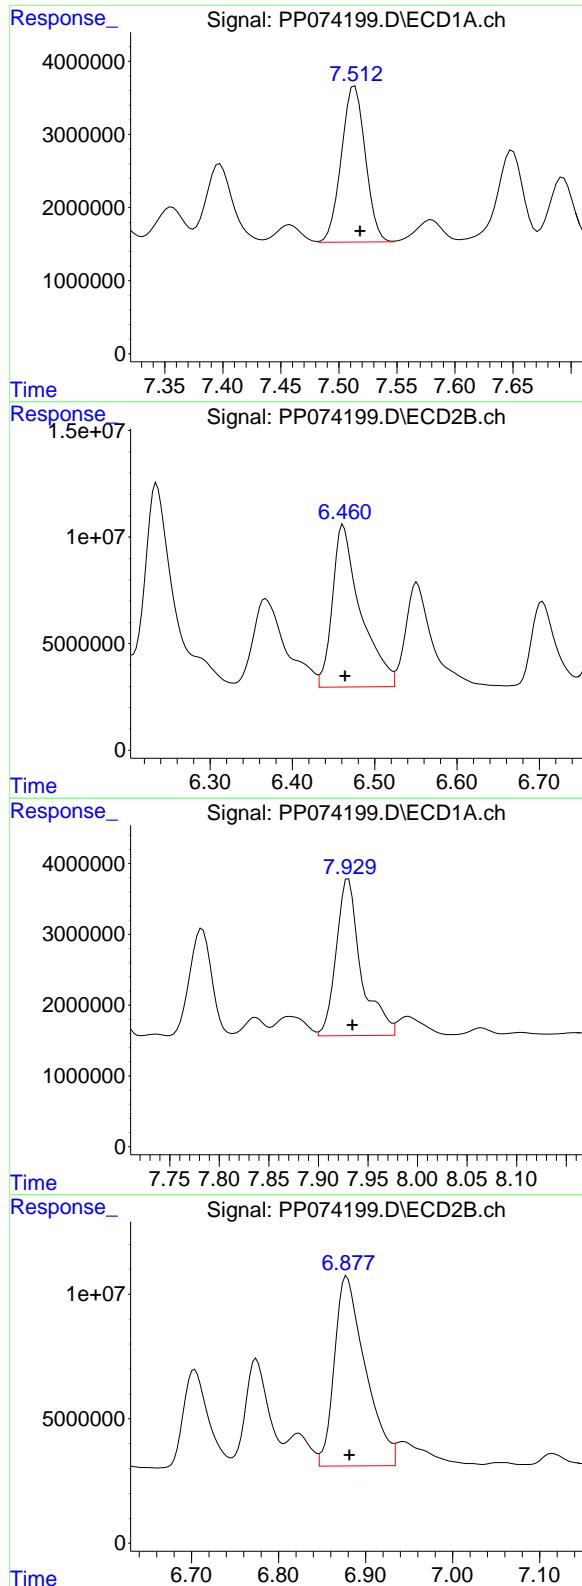

#29 AR-1254-4

R.T.: 7.514 min
 Delta R.T.: -0.005 min
 Response: 30708926
 Conc: 481.26 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#29 AR-1254-4


R.T.: 6.462 min
 Delta R.T.: -0.002 min
 Response: 181035006
 Conc: 492.52 ng/ml

#30 AR-1254-5

R.T.: 7.930 min
 Delta R.T.: -0.004 min
 Response: 38809795
 Conc: 478.28 ng/ml

#30 AR-1254-5

R.T.: 6.878 min
 Delta R.T.: -0.003 min
 Response: 188193102
 Conc: 478.75 ng/ml

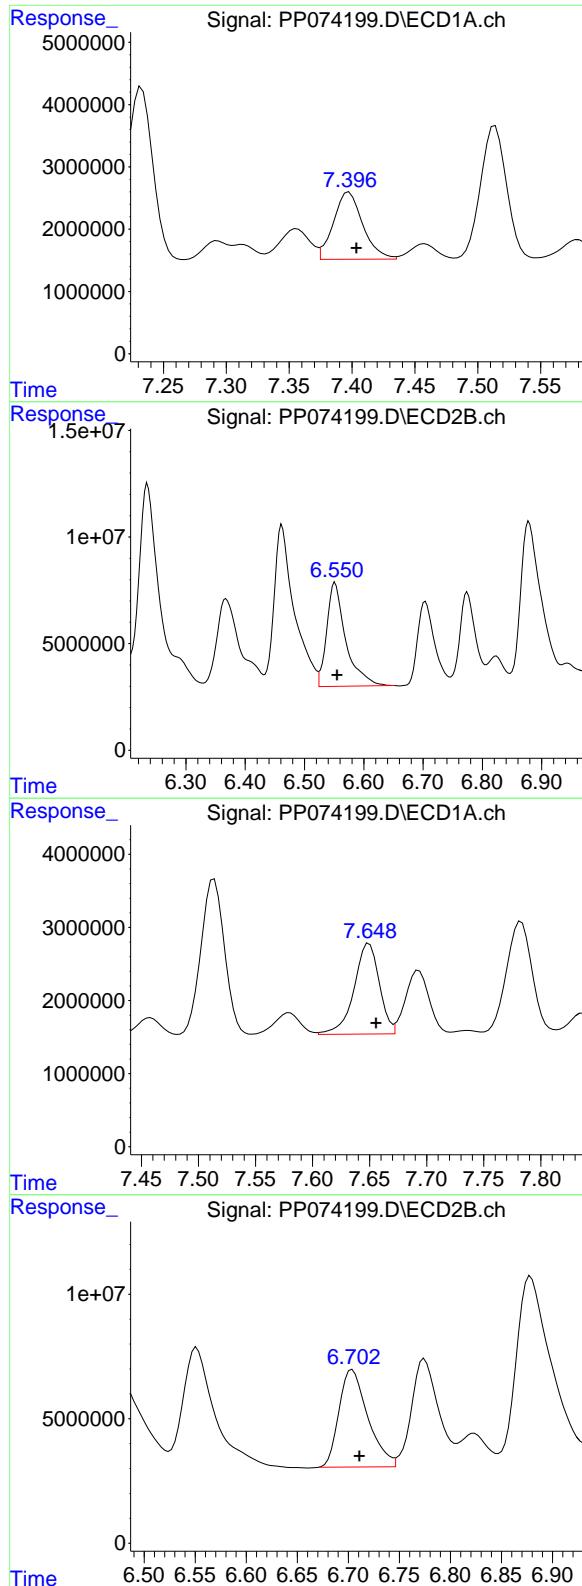

#31 AR-1260-1

R.T.: 7.398 min
 Delta R.T.: -0.006 min
 Response: 17543251
 Conc: 311.29 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#31 AR-1260-1


R.T.: 6.552 min
 Delta R.T.: -0.003 min
 Response: 109049999
 Conc: 269.95 ng/ml

#32 AR-1260-2

R.T.: 7.650 min
 Delta R.T.: -0.006 min
 Response: 19124212
 Conc: 280.61 ng/ml

#32 AR-1260-2

R.T.: 6.704 min
 Delta R.T.: -0.007 min
 Response: 77042973
 Conc: 246.38 ng/ml

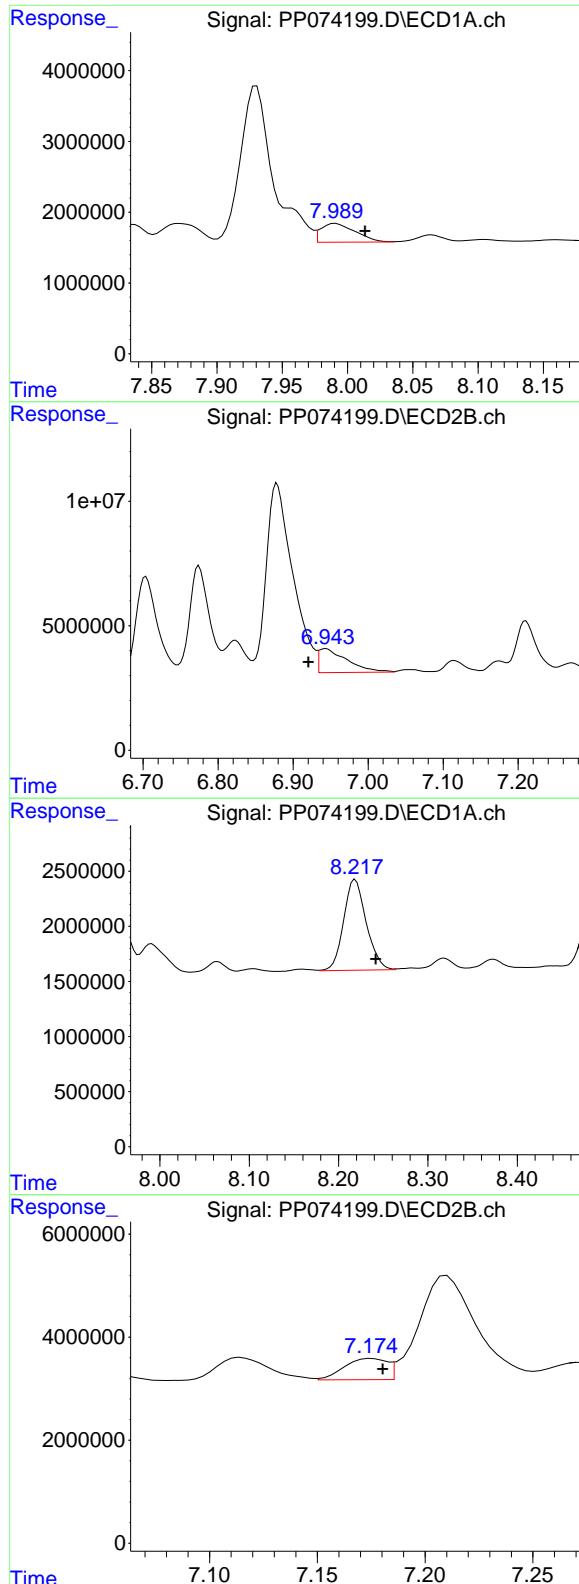

#33 AR-1260-3

R.T.: 7.991 min
 Delta R.T.: -0.023 min
 Response: 4844847
 Conc: 90.90 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

#33 AR-1260-3


R.T.: 6.944 min
 Delta R.T.: 0.023 min
 Response: 25122989
 Conc: 63.74 ng/ml

#34 AR-1260-4

R.T.: 8.219 min
 Delta R.T.: -0.023 min
 Response: 14487782
 Conc: 231.38 ng/ml

#34 AR-1260-4

R.T.: 7.175 min
 Delta R.T.: -0.005 min
 Response: 5653722
 Conc: 19.43 ng/ml

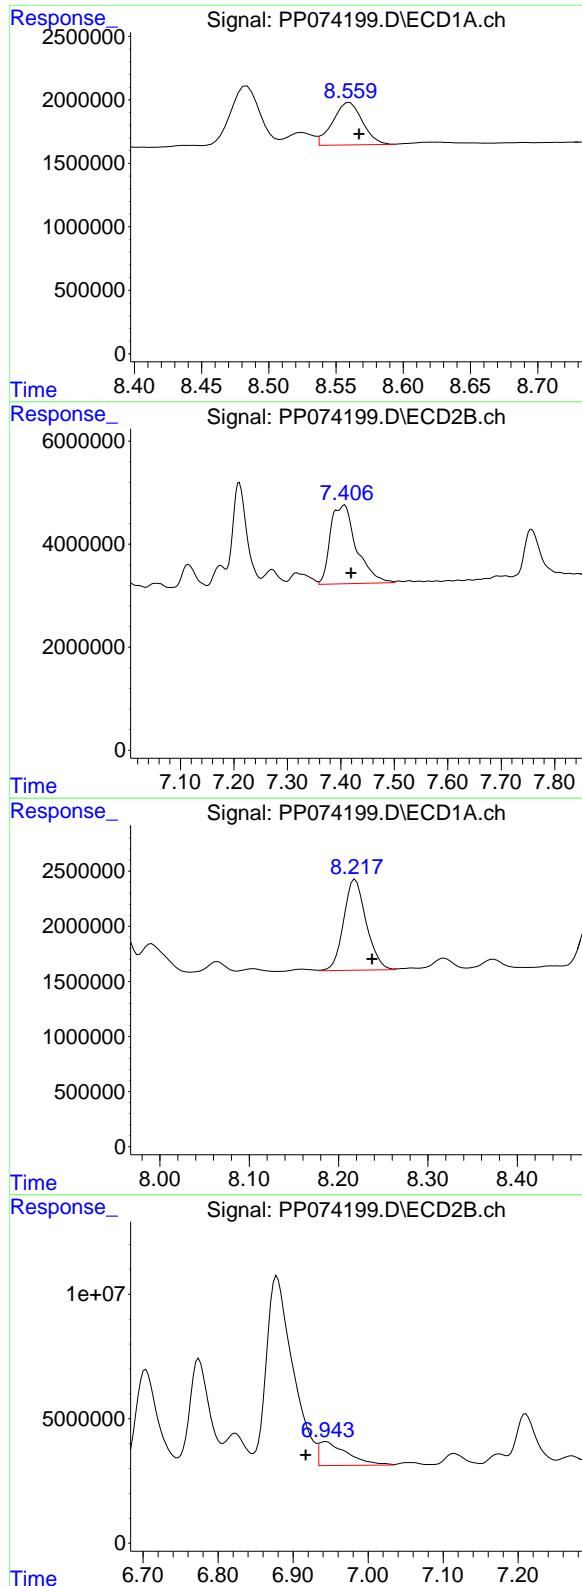

#35 AR-1260-5

R.T.: 8.560 min
 Delta R.T.: -0.007 min
 Response: 5145410
 Conc: 45.41 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#35 AR-1260-5


R.T.: 7.407 min
 Delta R.T.: -0.012 min
 Response: 51502946
 Conc: 68.00 ng/ml

#36 AR-1262-1

R.T.: 8.219 min
 Delta R.T.: -0.019 min
 Response: 14487782
 Conc: 191.16 ng/ml

#36 AR-1262-1


R.T.: 6.944 min
 Delta R.T.: 0.027 min
 Response: 25122989
 Conc: 44.61 ng/ml

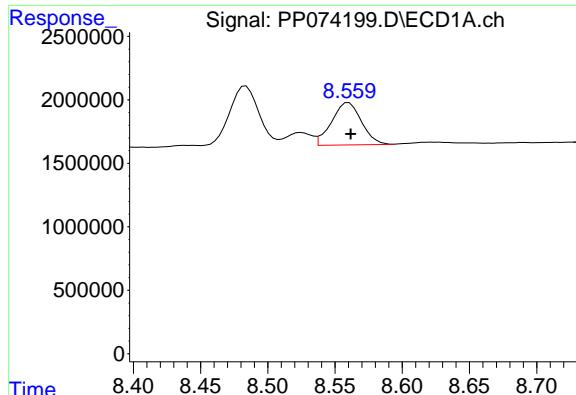

#37 AR-1262-2


R.T.: 8.560 min
Delta R.T.: -0.002 min
Response: 5145410
Conc: 39.45 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

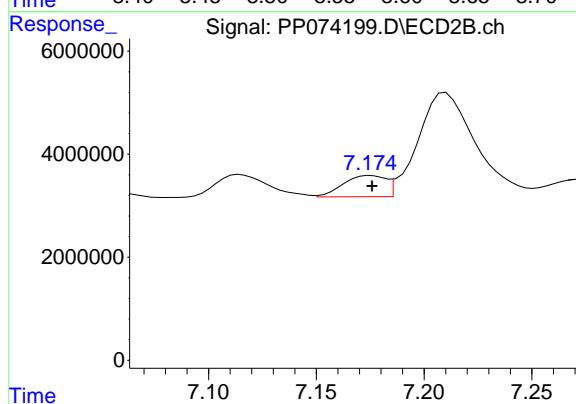


#37 AR-1262-2

R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 5653722
Conc: 14.10 ng/ml

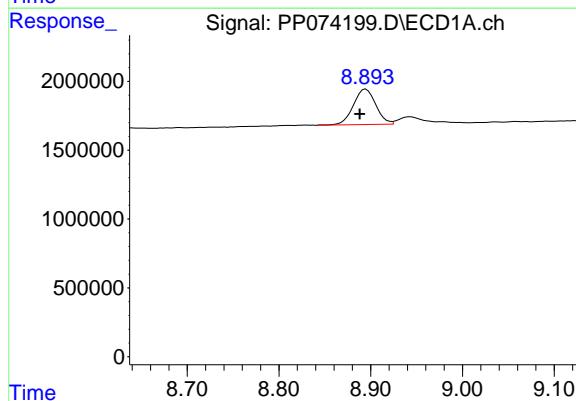


#38 AR-1262-3

R.T.: 8.895 min
Delta R.T.: 0.007 min
Response: 4365480
Conc: 46.41 ng/ml

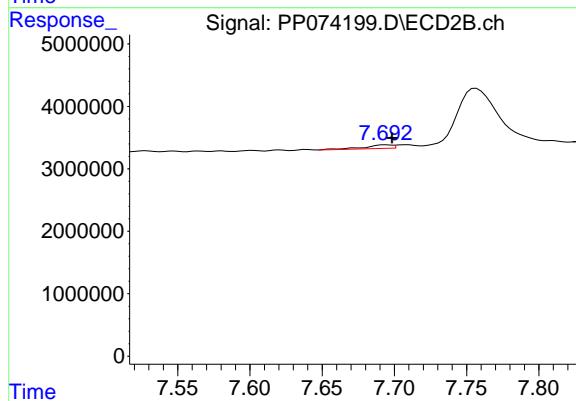

#38 AR-1262-3

R.T.: 7.694 min
Delta R.T.: -0.005 min
Response: 772104
Conc: 2.15 ng/ml

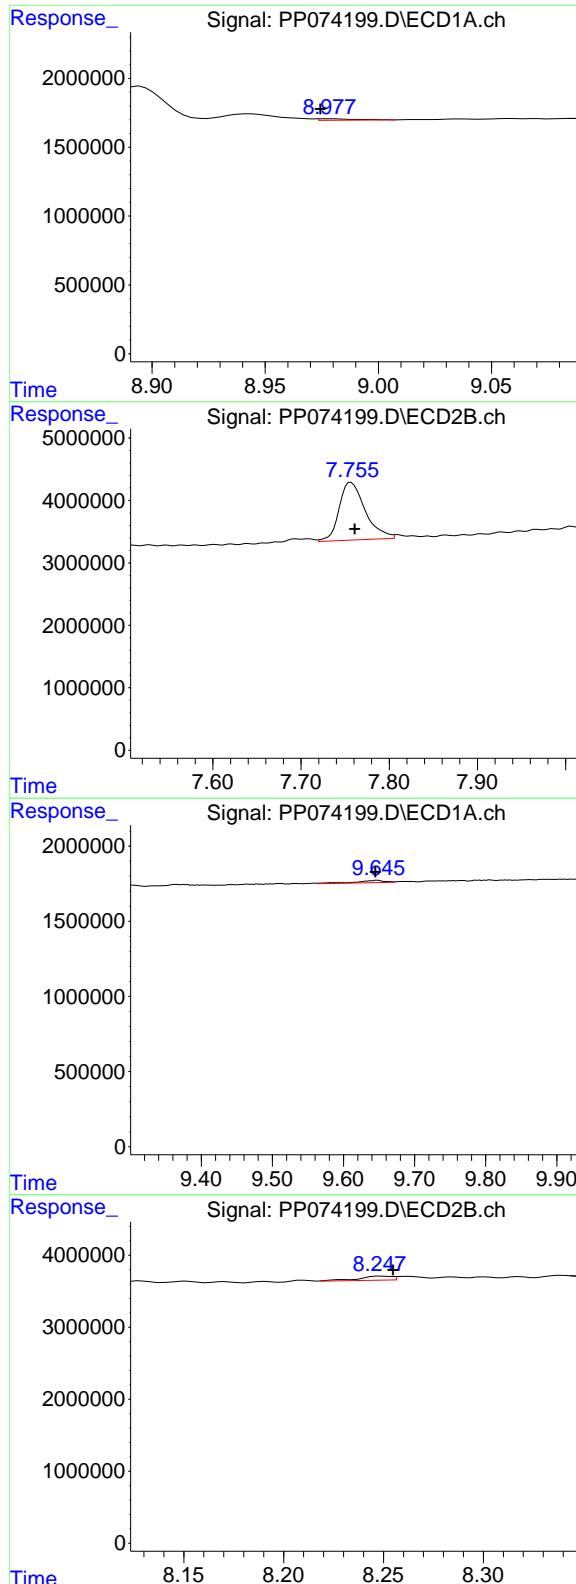

#39 AR-1262-4

R.T.: 8.979 min
 Delta R.T.: 0.004 min
 Response: 118980
 Conc: 1.63 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#39 AR-1262-4


R.T.: 7.757 min
 Delta R.T.: -0.004 min
 Response: 19007753
 Conc: 28.50 ng/ml

#40 AR-1262-5

R.T.: 9.647 min
 Delta R.T.: 0.003 min
 Response: 418724
 Conc: 8.22 ng/ml

#40 AR-1262-5

R.T.: 8.249 min
 Delta R.T.: -0.006 min
 Response: 666817
 Conc: 2.35 ng/ml

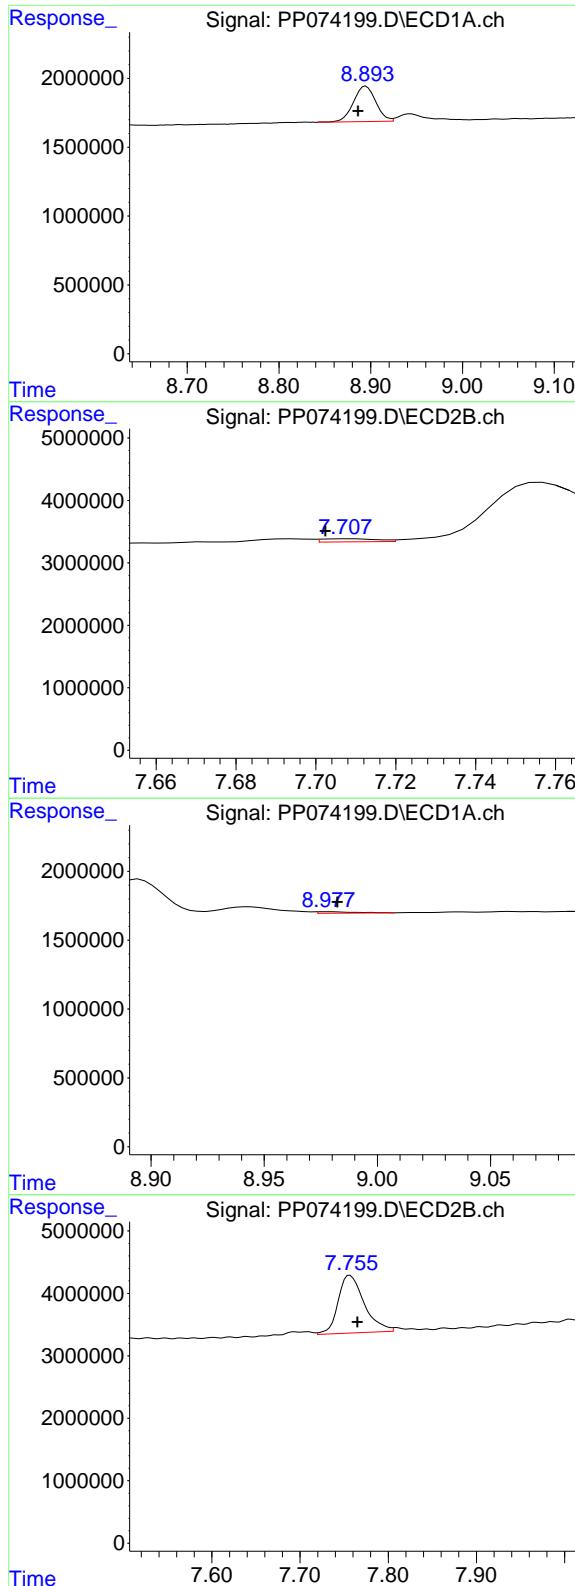

#41 AR-1268-1

R.T.: 8.895 min
 Delta R.T.: 0.008 min
 Response: 4365480
 Conc: 28.05 ng/ml

Instrument: ECD_P
 ClientSampleId: ICVPP080125AR1254

#41 AR-1268-1


R.T.: 7.709 min
 Delta R.T.: 0.007 min
 Response: 477278
 Conc: 0.44 ng/ml

#42 AR-1268-2

R.T.: 8.979 min
 Delta R.T.: -0.003 min
 Response: 118980
 Conc: 0.83 ng/ml

#42 AR-1268-2


R.T.: 7.757 min
 Delta R.T.: -0.009 min
 Response: 19007753
 Conc: 17.91 ng/ml

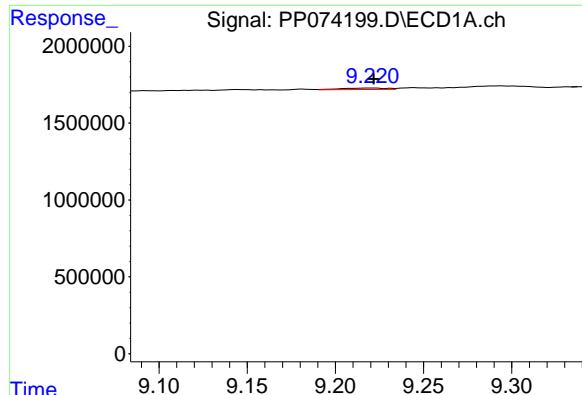

#43 AR-1268-3


R.T.: 9.221 min
Delta R.T.: 0.000 min
Response: 168840
Conc: 1.41 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

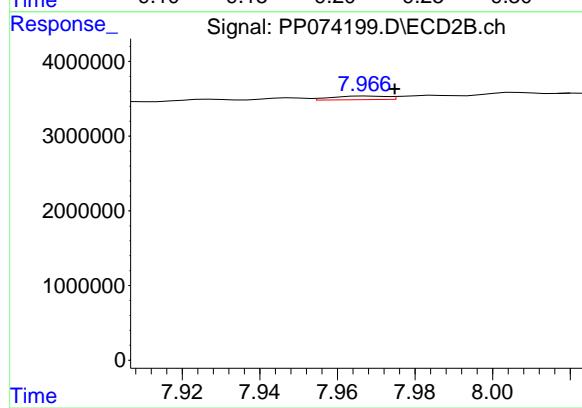


#43 AR-1268-3

R.T.: 7.968 min
Delta R.T.: -0.007 min
Response: 472836
Conc: 0.57 ng/ml

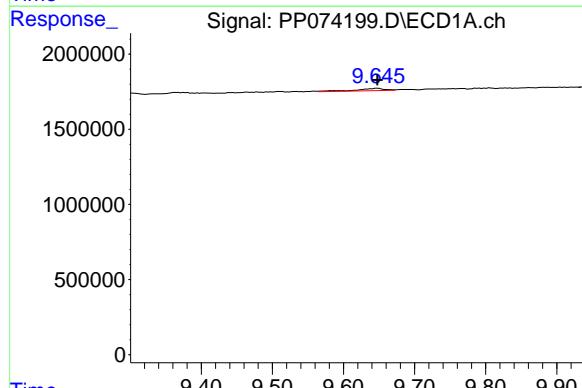


#44 AR-1268-4

R.T.: 9.647 min
Delta R.T.: 0.000 min
Response: 418724
Conc: 7.12 ng/ml

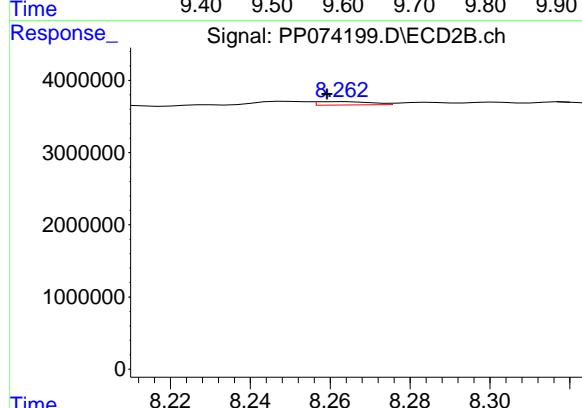

#44 AR-1268-4


R.T.: 8.263 min
Delta R.T.: 0.004 min
Response: 437922
Conc: 1.42 ng/ml

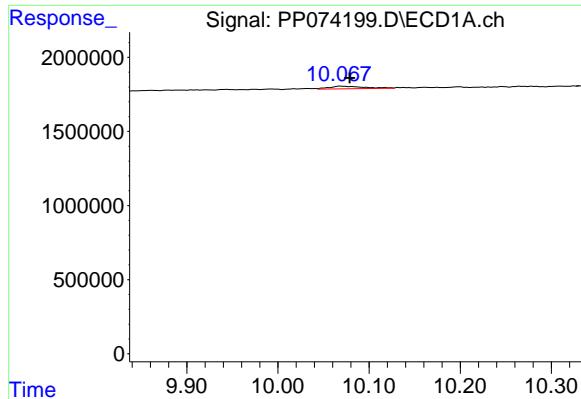

#45 AR-1268-5

R.T.: 10.069 min
Delta R.T.: -0.009 min
Response: 442219
Conc: 1.26 ng/ml

Instrument: ECD_P
ClientSampleId: ICVPP080125AR1254

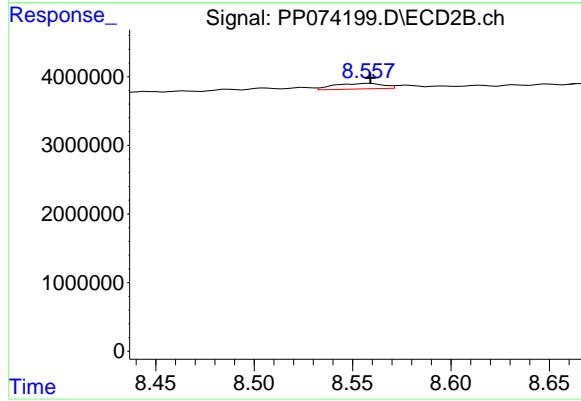

#45 AR-1268-5

R.T.: 8.559 min
Delta R.T.: 0.000 min
Response: 1401468
Conc: 0.55 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:05
 Operator : YP\AJ
 Sample : PB169205BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB169205BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 13:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.801 | 27178701 | 79780335 | 24.303 | 20.806 |
| 2) SA Decachlor... | 10.438 | 8.821 | 21836747 | 120.3E6 | 22.485 | 20.000 |

Target Compounds

| | | | | | | |
|------------------|-------|--------|----------|----------|----------|------------|
| 3) L1 AR-1016-1 | 5.809 | 4.902 | 22669527 | 228.6E6 | 549.474 | 573.187 |
| 4) L1 AR-1016-2 | 5.830 | 4.959 | 34110297 | 104.5E6 | 561.563 | 556.666 |
| 5) L1 AR-1016-3 | 5.893 | 5.080 | 22276842 | 56001049 | 561.688 | 527.965 |
| 6) L1 AR-1016-4 | 5.990 | 5.121 | 18317589 | 56446484 | 562.848 | 516.814 |
| 7) L1 AR-1016-5 | 6.283 | 5.334 | 17574695 | 66942868 | 541.292 | 572.341 |
| 8) L2 AR-1221-1 | 4.853 | 4.013 | 2634639 | 6691268 | 157.164 | 136.320 |
| 9) L2 AR-1221-2 | 4.942 | 4.098 | 3253773 | 8154385 | 258.214 | 227.209 |
| 10) L2 AR-1221-3 | 5.018 | 4.175 | 13169343 | 42774973 | 359.472 | 316.325 |
| 11) L3 AR-1232-1 | 5.018 | 4.175 | 13169343 | 42774973 | 453.532 | 422.000 |
| 12) L3 AR-1232-2 | 5.544 | 4.902 | 17607365 | 228.6E6 | 1170.491 | 1311.998 |
| 13) L3 AR-1232-3 | 5.830 | 5.080 | 34110297 | 56001049 | 1176.148 | 1222.287 |
| 14) L3 AR-1232-4 | 5.990 | 5.163 | 18317589 | 109.7E6 | 1184.161 | 1890.439 # |
| 15) L3 AR-1232-5 | 6.080 | 5.334 | 15956878 | 66942868 | 1361.972 | 1424.939 |
| 16) L4 AR-1242-1 | 5.809 | 4.902 | 22669527 | 228.6E6 | 608.320 | 662.445 |
| 17) L4 AR-1242-2 | 5.830 | 4.959 | 34110297 | 104.5E6 | 626.925 | 639.909 |
| 18) L4 AR-1242-3 | 5.893 | 5.080 | 22276842 | 56001049 | 623.375 | 607.067 |
| 19) L4 AR-1242-4 | 5.990 | 5.163 | 18317589 | 109.7E6 | 626.914 | 918.307 # |
| 20) L4 AR-1242-5 | 6.720 | 5.686 | 3662834 | 76796260 | 103.010 | 513.481 # |
| 21) L5 AR-1248-1 | 5.809 | 4.902 | 22669527 | 228.6E6 | 809.206 | 1068.737 # |
| 22) L5 AR-1248-2 | 6.080 | 5.121 | 15956878 | 56446484 | 396.335 | 385.794 |
| 23) L5 AR-1248-3 | 6.283 | 5.163 | 17574695 | 109.7E6 | 394.285 | 639.599 # |
| 24) L5 AR-1248-4 | 6.658 | 5.334 | 17077329 | 66942868 | 328.176 | 402.365 |
| 25) L5 AR-1248-5 | 6.720 | 5.686f | 3662834 | 76796260 | 64.324 | 263.936 # |
| 26) L6 AR-1254-1 | 6.658 | 5.686 | 17077329 | 76796260 | 324.411 | 209.722 # |
| 27) L6 AR-1254-2 | 6.873 | 5.832 | 14942029 | 64358610 | 187.939 | 231.325 |
| 28) L6 AR-1254-3 | 7.236 | 6.250 | 8784278 | 129.8E6 | 100.603 | 265.237 # |
| 29) L6 AR-1254-4 | 7.519 | 6.462 | 5607113 | 9342145 | 87.873 | 25.416 # |
| 30) L6 AR-1254-5 | 7.933 | 6.878 | 49832102 | 203.5E6 | 614.114 | 528.324 |
| 31) L7 AR-1260-1 | 7.401 | 6.551 | 31033148 | 236.1E6 | 550.662 | 584.486 |
| 32) L7 AR-1260-2 | 7.653 | 6.706 | 36070118 | 182.5E6 | 529.257 | 583.716 |
| 33) L7 AR-1260-3 | 8.012 | 6.915 | 24314378 | 204.9E6 | 456.215 | 519.977 |
| 34) L7 AR-1260-4 | 8.240 | 7.175 | 34948406 | 149.4E6 | 558.148 | 513.385 |
| 35) L7 AR-1260-5 | 8.566 | 7.415 | 51128845 | 382.8E6 | 451.250 | 505.423 |
| 36) L8 AR-1262-1 | 8.240 | 6.915 | 34948406 | 204.9E6 | 461.123 | 363.909 |
| 37) L8 AR-1262-2 | 8.566 | 7.175 | 51128845 | 149.4E6 | 392.002 | 372.508 |
| 38) L8 AR-1262-3 | 8.899 | 7.698 | 35659813 | 68577315 | 379.074 | 190.773 # |
| 39) L8 AR-1262-4 | 8.976 | 7.761 | 8821459 | 247.5E6 | 121.088 | 371.067 # |
| 40) L8 AR-1262-5 | 9.651 | 8.257 | 14529552 | 71597111 | 285.326 | 252.754 |
| 41) L9 AR-1268-1 | 8.899 | 7.698 | 35659813 | 68577315 | 229.128 | 62.900 # |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:05
 Operator : YP\AJ
 Sample : PB169205BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB169205BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 13:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|--------|-------|----------|----------|---------|-----------|
| 42) L9 AR-1268-2 | 8.976 | 7.761 | 8821459 | 247.5E6 | 61.505 | 233.173 # |
| 43) L9 AR-1268-3 | 9.224 | 7.969 | 1133561 | 5277612 | 9.488 | 6.344 # |
| 44) L9 AR-1268-4 | 9.651 | 8.257 | 14529552 | 71597111 | 247.048 | 232.413 |
| 45) L9 AR-1268-5 | 10.082 | 8.556 | 4915065 | 21332104 | 13.975 | 8.365 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:05
 Operator : YP\AJ
 Sample : PB169205BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB169205BS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 13:31:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation


Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

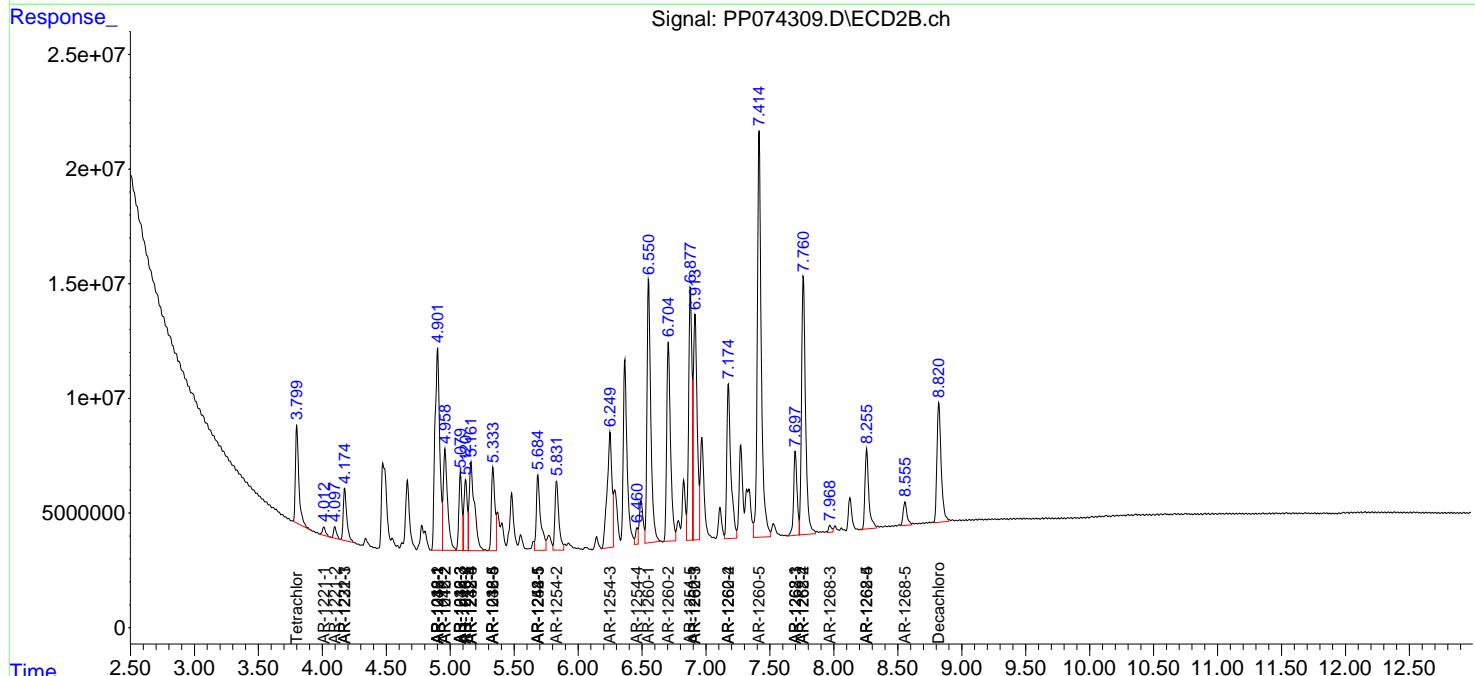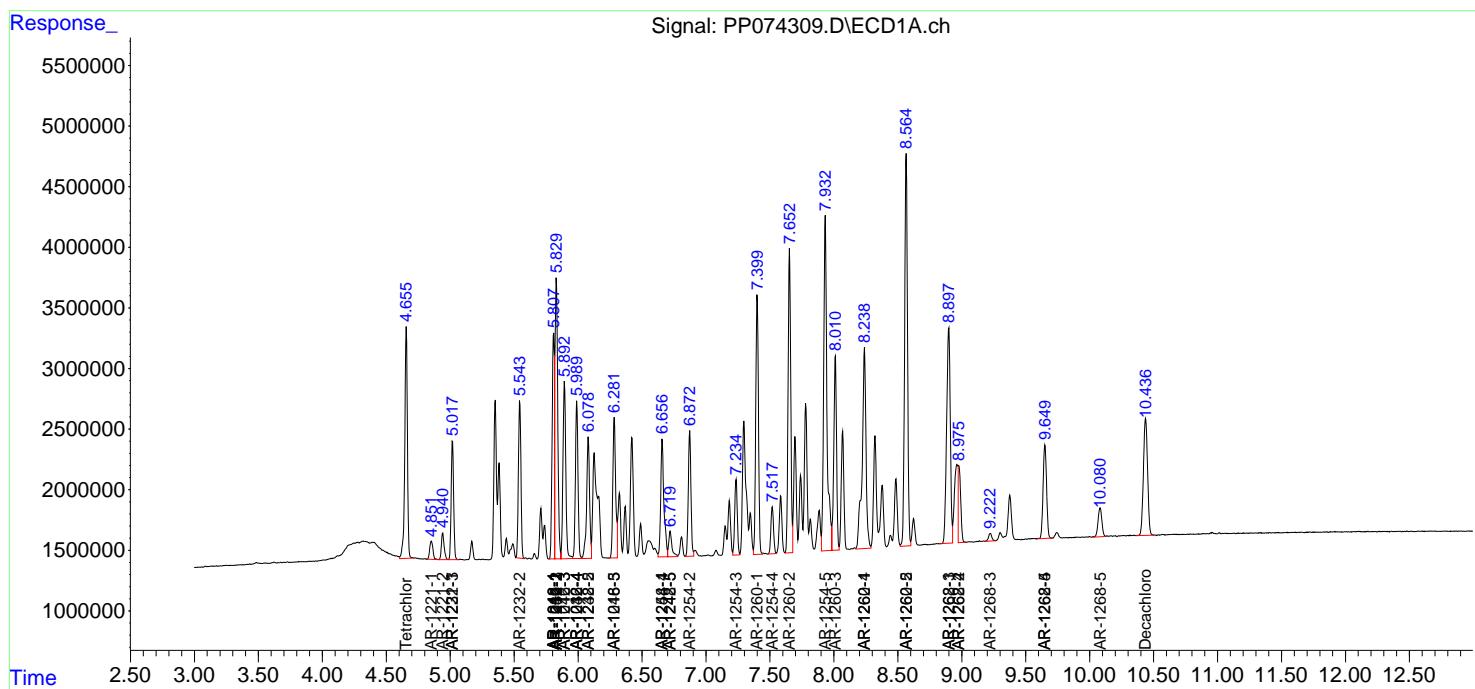

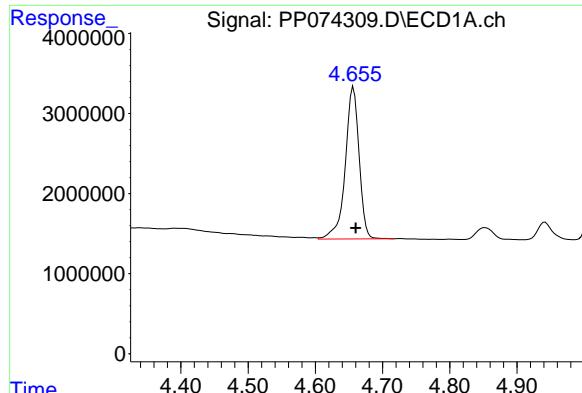


#1 Tetrachloro-m-xylene
R.T.: 4.657 min
Delta R.T.: -0.003 min
Response: 27178701
Conc: 24.30 ng/ml


Instrument: ECD_P
ClientSampleId: PB169205BS

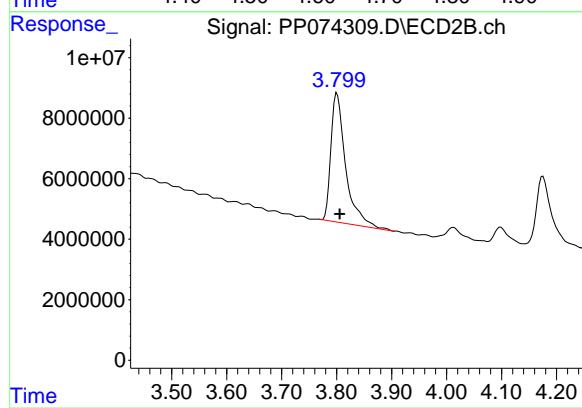


#1 Tetrachloro-m-xylene
R.T.: 3.801 min
Delta R.T.: -0.005 min
Response: 79780335
Conc: 20.81 ng/ml

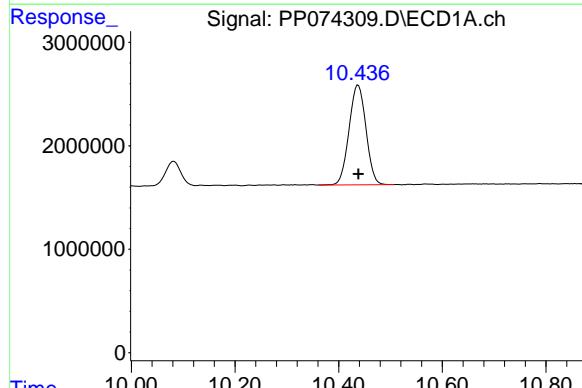

#2 Decachlorobiphenyl
R.T.: 10.438 min
Delta R.T.: 0.000 min
Response: 21836747
Conc: 22.49 ng/ml

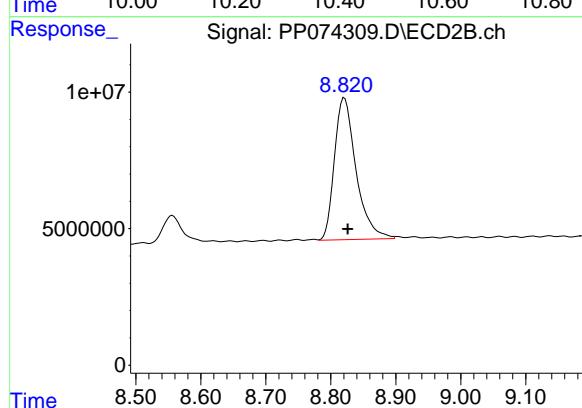

#2 Decachlorobiphenyl
R.T.: 8.821 min
Delta R.T.: -0.005 min
Response: 120271397
Conc: 20.00 ng/ml

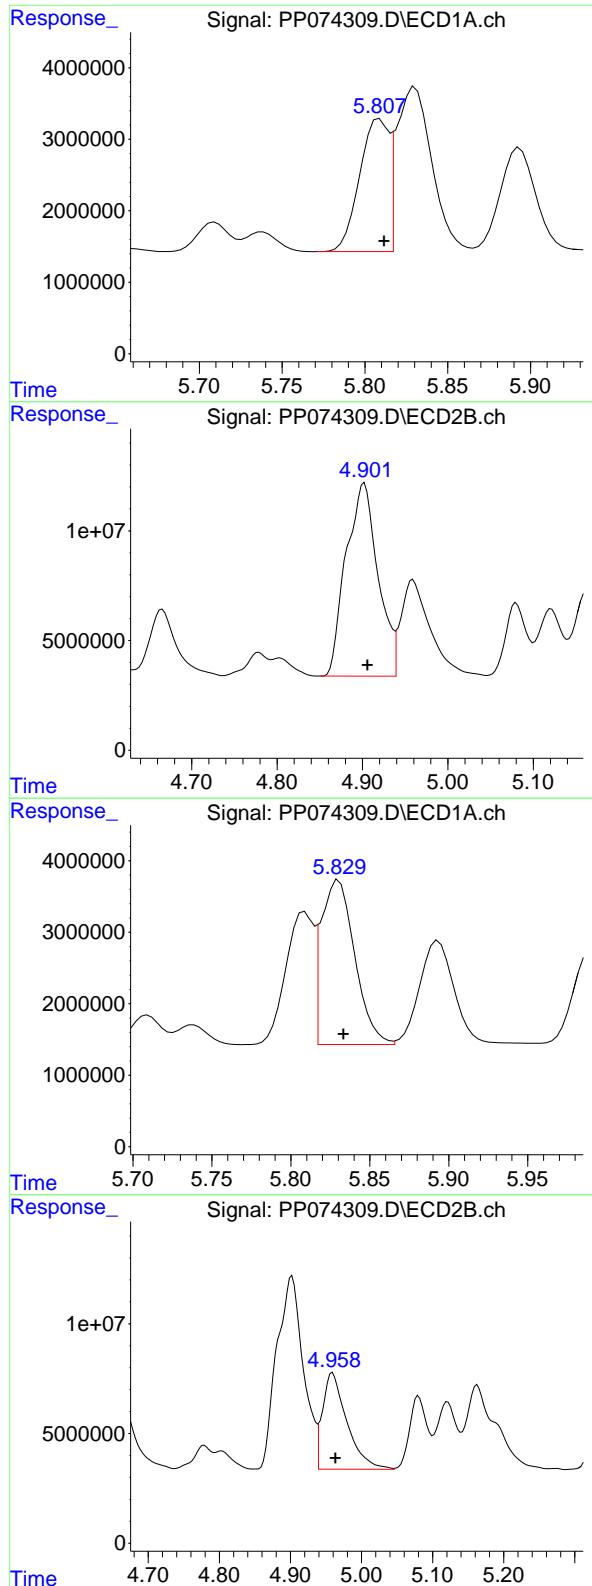

#3 AR-1016-1

R.T.: 5.809 min
 Delta R.T.: -0.003 min
 Response: 22669527
 Conc: 549.47 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#3 AR-1016-1


R.T.: 4.902 min
 Delta R.T.: -0.003 min
 Response: 228636880
 Conc: 573.19 ng/ml

#4 AR-1016-2

R.T.: 5.830 min
 Delta R.T.: -0.003 min
 Response: 34110297
 Conc: 561.56 ng/ml

#4 AR-1016-2


R.T.: 4.959 min
 Delta R.T.: -0.004 min
 Response: 104546878
 Conc: 556.67 ng/ml

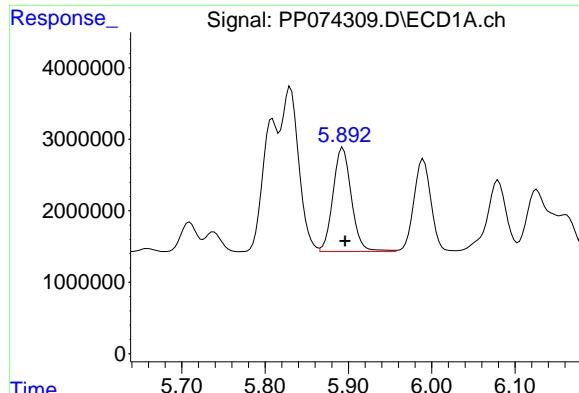

#5 AR-1016-3


R.T.: 5.893 min
 Delta R.T.: -0.003 min
 Response: 22276842
 Conc: 561.69 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

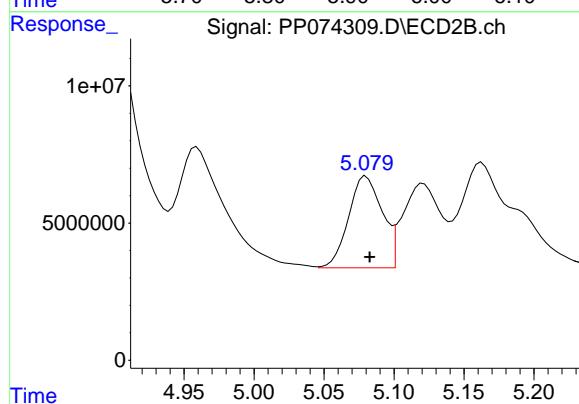


#5 AR-1016-3

R.T.: 5.080 min
 Delta R.T.: -0.003 min
 Response: 56001049
 Conc: 527.96 ng/ml

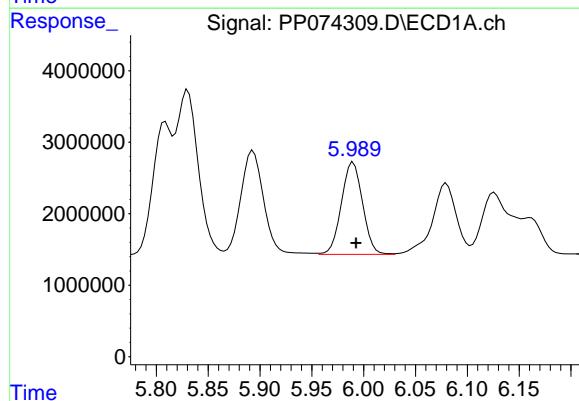


#6 AR-1016-4

R.T.: 5.990 min
 Delta R.T.: -0.003 min
 Response: 18317589
 Conc: 562.85 ng/ml

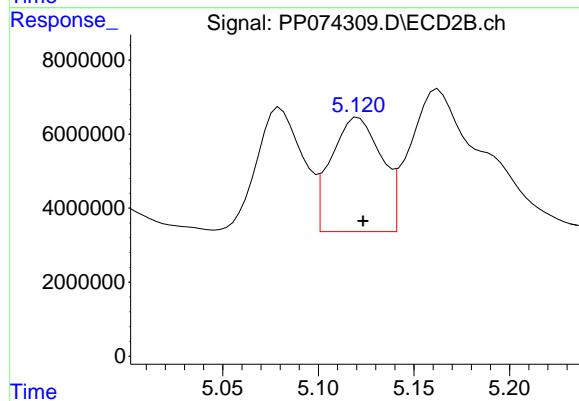

#6 AR-1016-4


R.T.: 5.121 min
 Delta R.T.: -0.002 min
 Response: 56446484
 Conc: 516.81 ng/ml

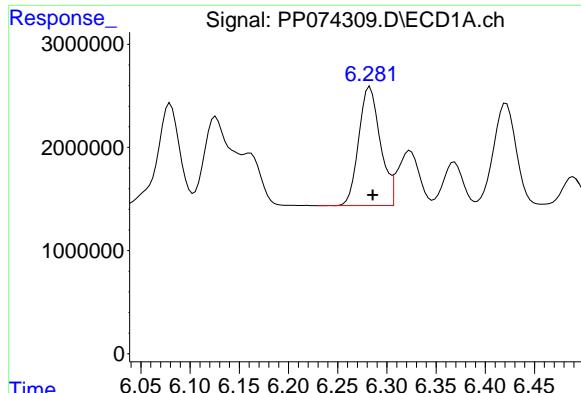

#7 AR-1016-5


R.T.: 6.283 min
 Delta R.T.: -0.003 min
 Response: 17574695
 Conc: 541.29 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

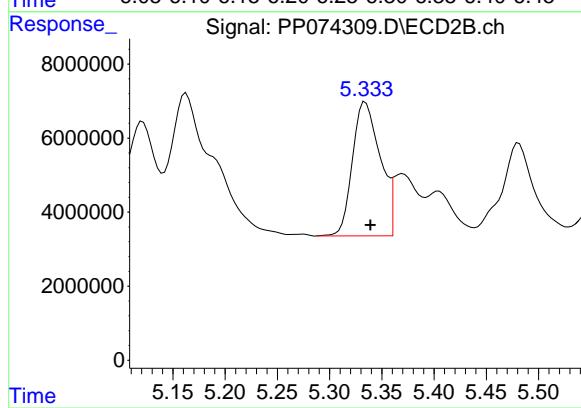


#7 AR-1016-5

R.T.: 5.334 min
 Delta R.T.: -0.005 min
 Response: 66942868
 Conc: 572.34 ng/ml

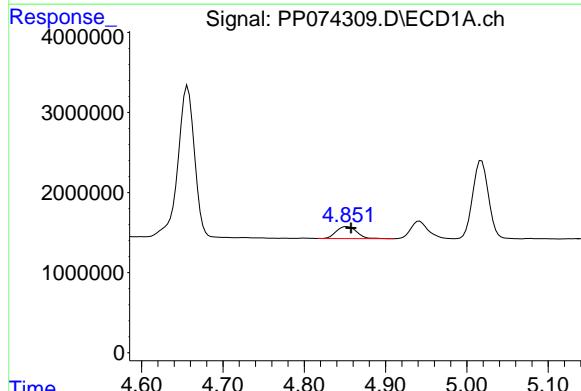


#8 AR-1221-1

R.T.: 4.853 min
 Delta R.T.: -0.005 min
 Response: 2634639
 Conc: 157.16 ng/ml

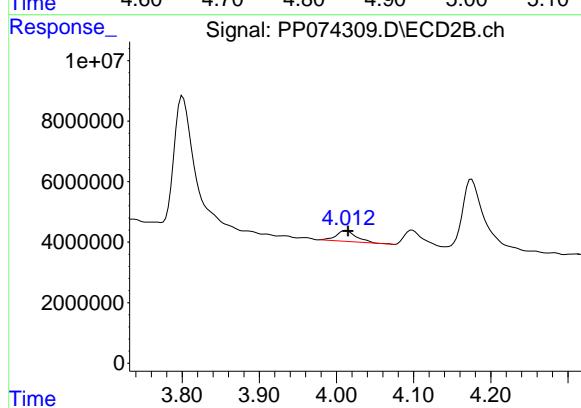

#8 AR-1221-1

R.T.: 4.013 min
 Delta R.T.: -0.003 min
 Response: 6691268
 Conc: 136.32 ng/ml

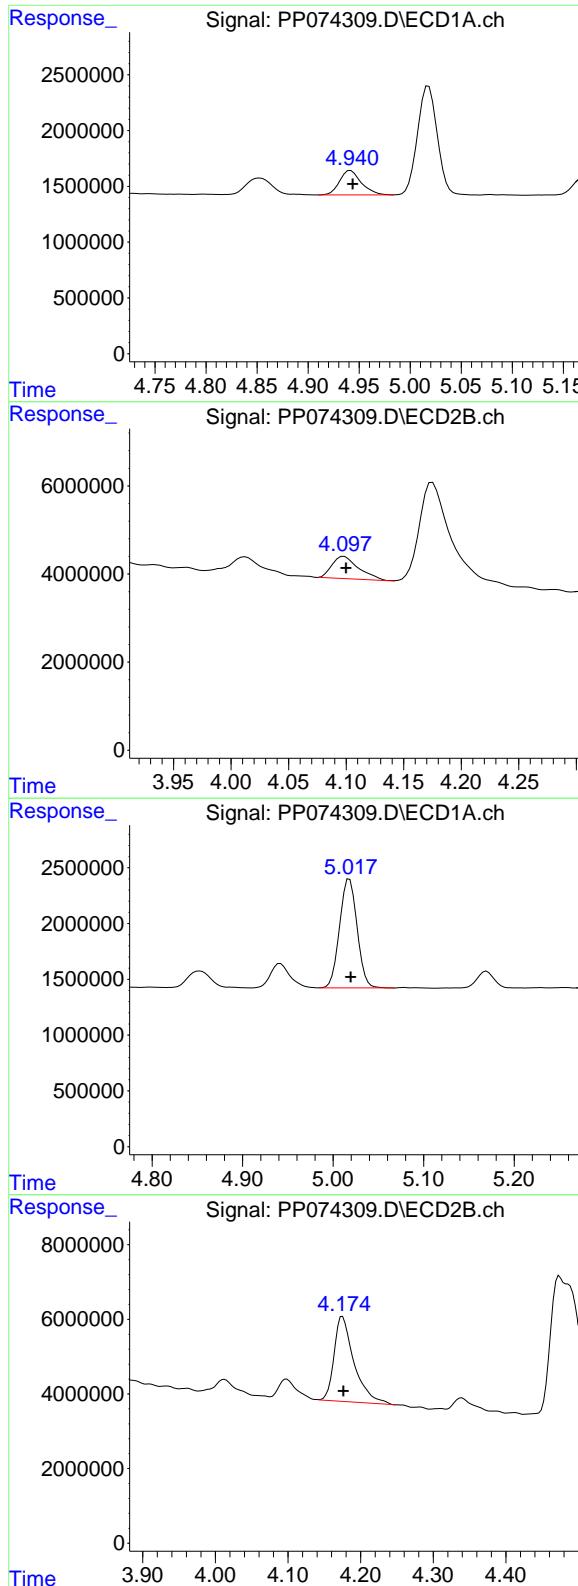

#9 AR-1221-2

R.T.: 4.942 min
 Delta R.T.: -0.002 min
 Response: 3253773
 Conc: 258.21 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#9 AR-1221-2


R.T.: 4.098 min
 Delta R.T.: -0.002 min
 Response: 8154385
 Conc: 227.21 ng/ml

#10 AR-1221-3

R.T.: 5.018 min
 Delta R.T.: -0.001 min
 Response: 13169343
 Conc: 359.47 ng/ml

#10 AR-1221-3


R.T.: 4.175 min
 Delta R.T.: -0.001 min
 Response: 42774973
 Conc: 316.33 ng/ml

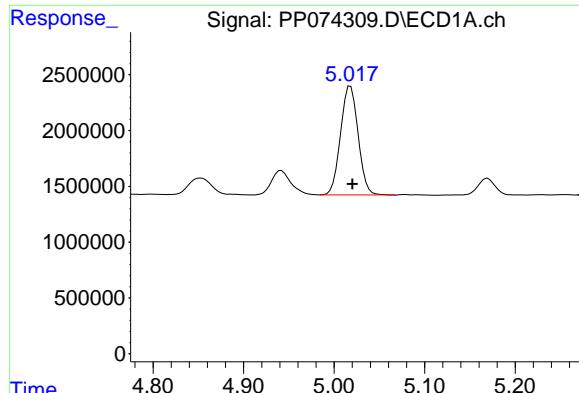

#11 AR-1232-1


R.T.: 5.018 min
 Delta R.T.: -0.002 min
 Response: 13169343
 Conc: 453.53 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

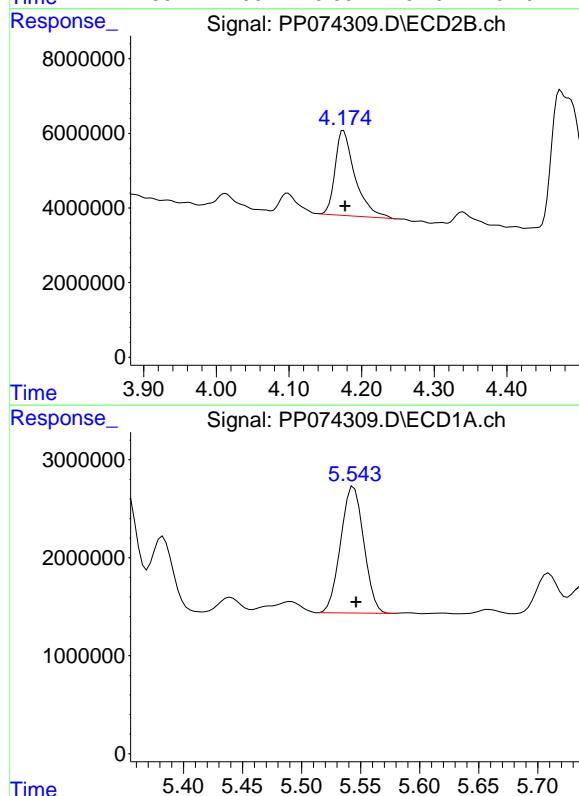


#12 AR-1232-2

R.T.: 5.544 min
 Delta R.T.: -0.002 min
 Response: 17607365
 Conc: 1170.49 ng/ml

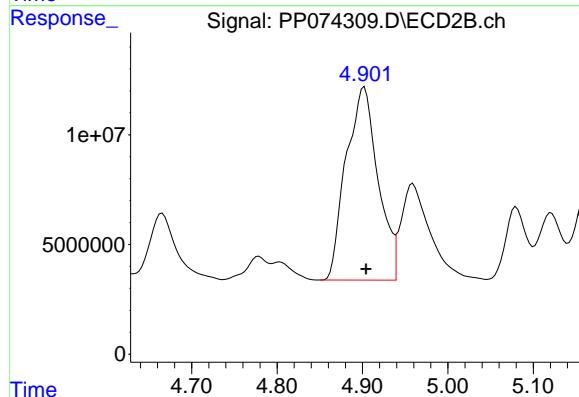

#12 AR-1232-2

R.T.: 4.902 min
 Delta R.T.: -0.002 min
 Response: 228636880
 Conc: 1312.00 ng/ml

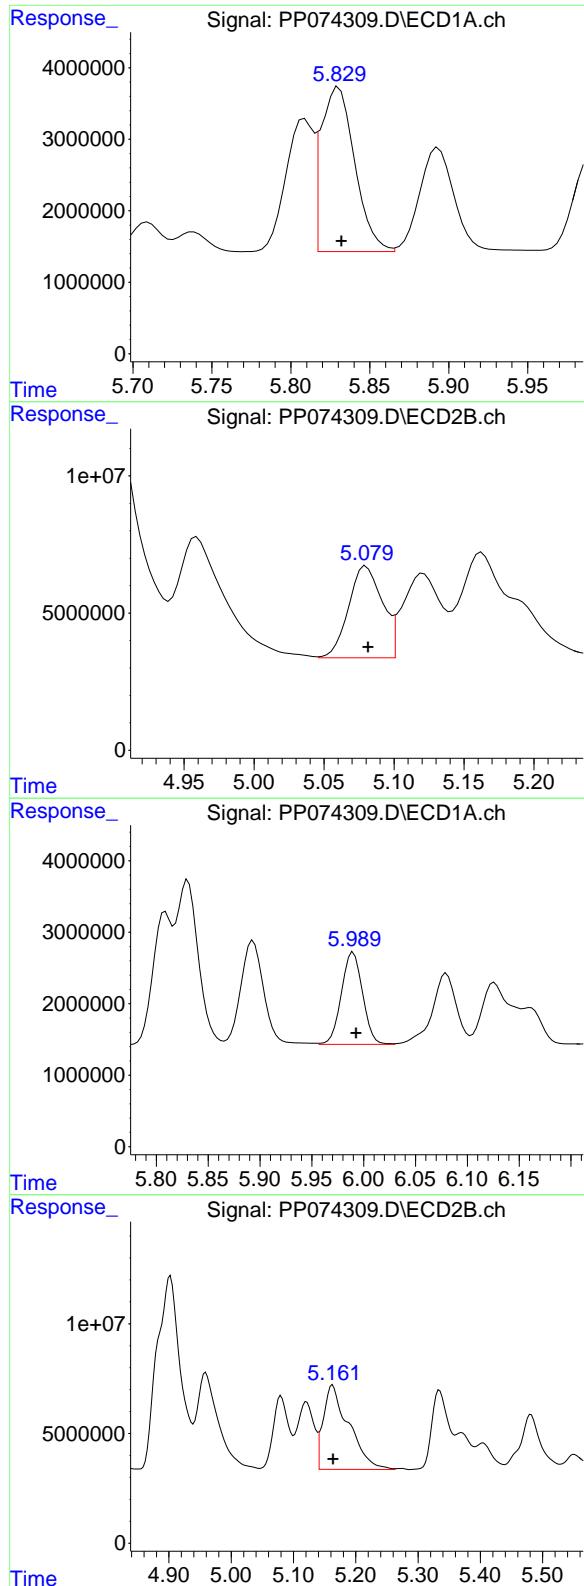

#13 AR-1232-3

R.T.: 5.830 min
 Delta R.T.: -0.002 min
 Response: 34110297
 Conc: 1176.15 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#13 AR-1232-3


R.T.: 5.080 min
 Delta R.T.: -0.001 min
 Response: 56001049
 Conc: 1222.29 ng/ml

#14 AR-1232-4

R.T.: 5.990 min
 Delta R.T.: -0.002 min
 Response: 18317589
 Conc: 1184.16 ng/ml


#14 AR-1232-4

R.T.: 5.163 min
 Delta R.T.: 0.000 min
 Response: 109665710
 Conc: 1890.44 ng/ml

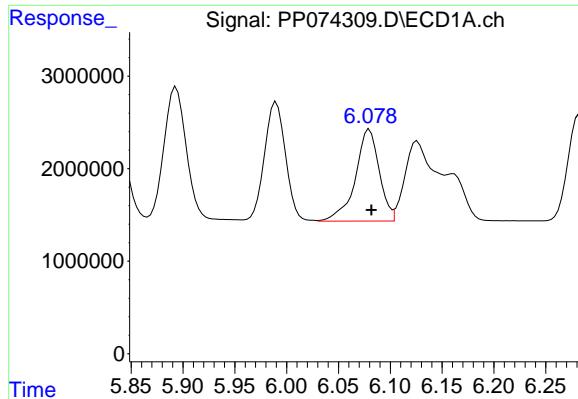


#15 AR-1232-5

R.T.: 6.080 min
 Delta R.T.: -0.002 min
 Response: 15956878
 Conc: 1361.97 ng/ml
Instrument: ECD_P
ClientSampleId: PB169205BS

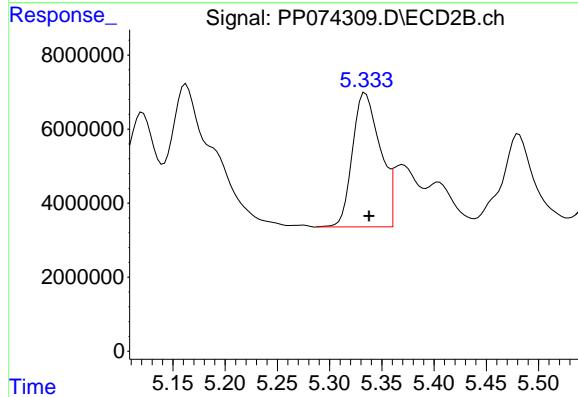


#15 AR-1232-5

R.T.: 5.334 min
 Delta R.T.: -0.003 min
 Response: 66942868
 Conc: 1424.94 ng/ml

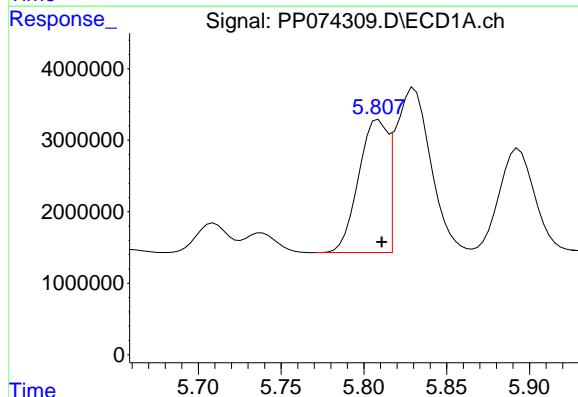


#16 AR-1242-1

R.T.: 5.809 min
 Delta R.T.: -0.002 min
 Response: 22669527
 Conc: 608.32 ng/ml

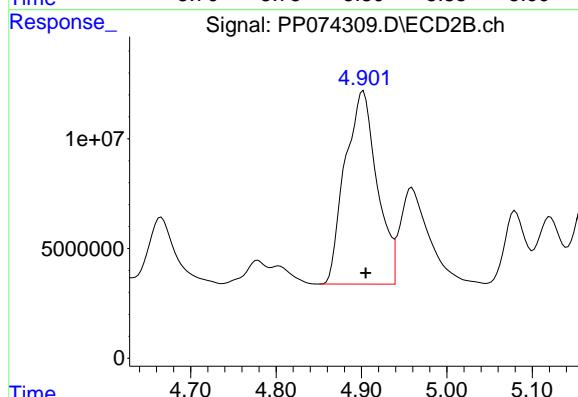

#16 AR-1242-1

R.T.: 4.902 min
 Delta R.T.: -0.003 min
 Response: 228636880
 Conc: 662.45 ng/ml

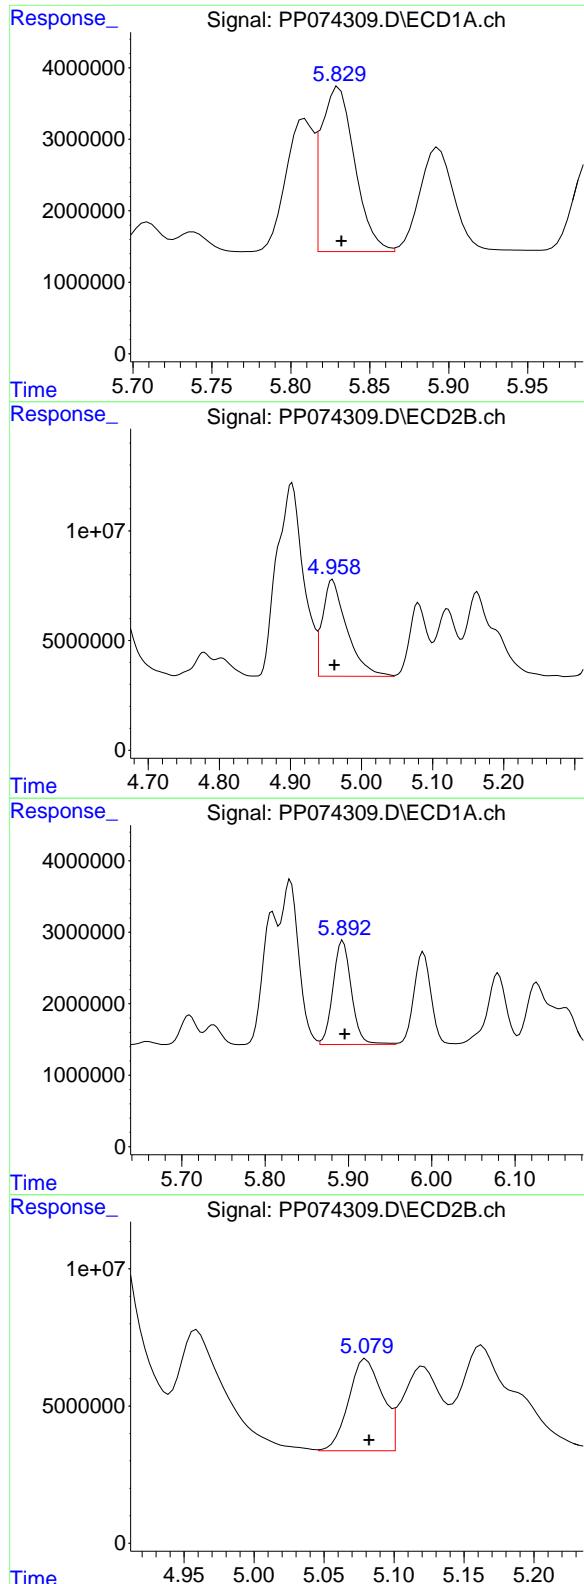

#17 AR-1242-2

R.T.: 5.830 min
 Delta R.T.: -0.002 min
 Response: 34110297
 Conc: 626.92 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#17 AR-1242-2


R.T.: 4.959 min
 Delta R.T.: -0.003 min
 Response: 104546878
 Conc: 639.91 ng/ml

#18 AR-1242-3

R.T.: 5.893 min
 Delta R.T.: -0.002 min
 Response: 22276842
 Conc: 623.38 ng/ml

#18 AR-1242-3


R.T.: 5.080 min
 Delta R.T.: -0.002 min
 Response: 56001049
 Conc: 607.07 ng/ml

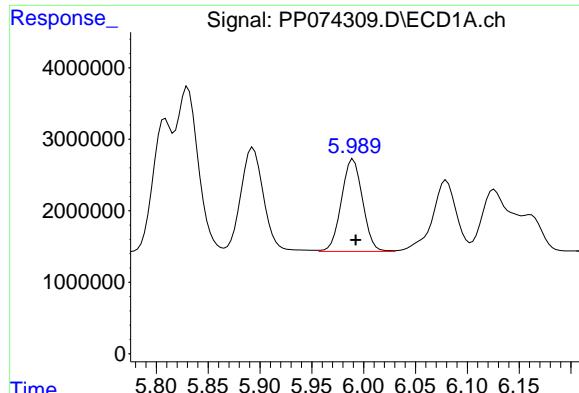

#19 AR-1242-4


R.T.: 5.990 min
 Delta R.T.: -0.002 min
 Response: 18317589
 Conc: 626.91 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

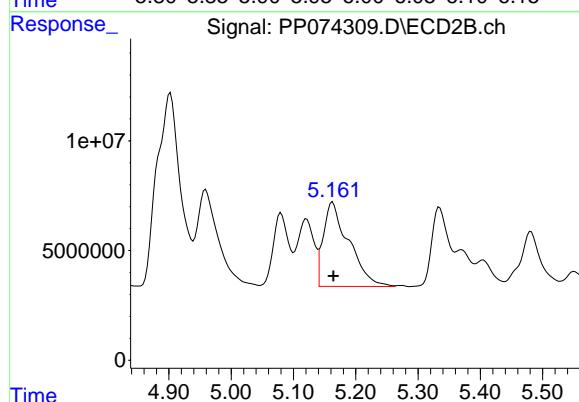


#19 AR-1242-4

R.T.: 5.163 min
 Delta R.T.: -0.001 min
 Response: 109665710
 Conc: 918.31 ng/ml

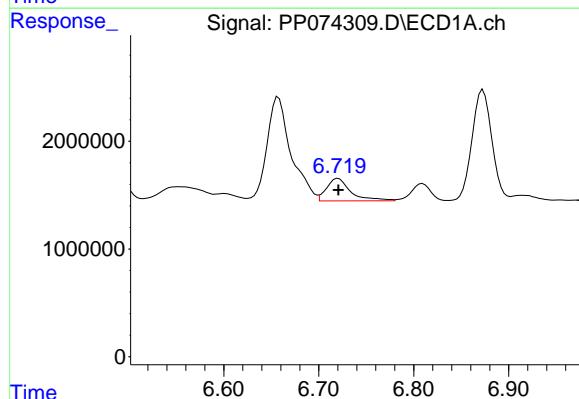


#20 AR-1242-5

R.T.: 6.720 min
 Delta R.T.: 0.000 min
 Response: 3662834
 Conc: 103.01 ng/ml

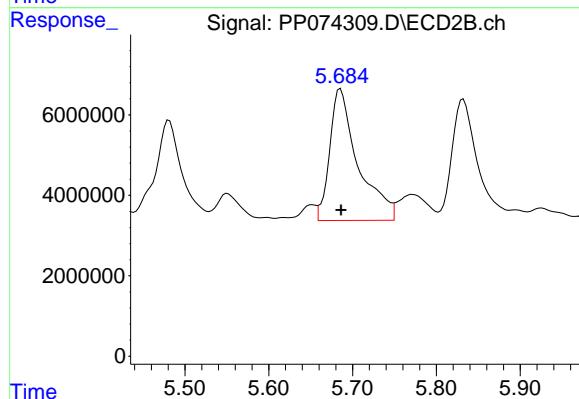

#20 AR-1242-5


R.T.: 5.686 min
 Delta R.T.: 0.000 min
 Response: 76796260
 Conc: 513.48 ng/ml

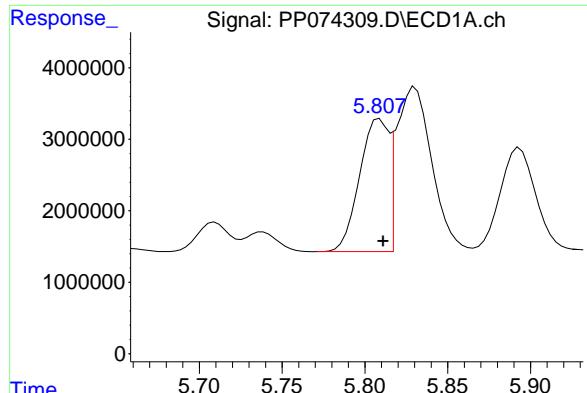

#21 AR-1248-1


R.T.: 5.809 min
 Delta R.T.: -0.002 min
 Response: 22669527
 Conc: 809.21 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

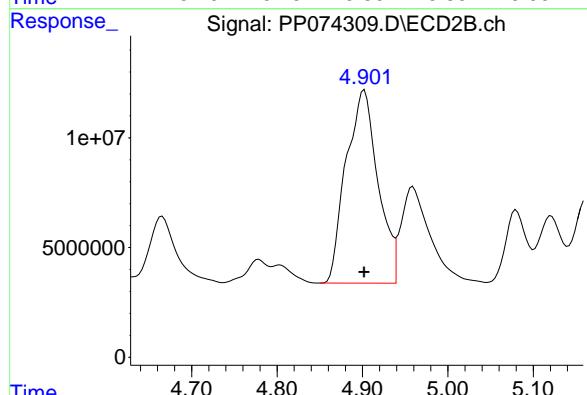


#21 AR-1248-1

R.T.: 4.902 min
 Delta R.T.: 0.000 min
 Response: 228636880
 Conc: 1068.74 ng/ml

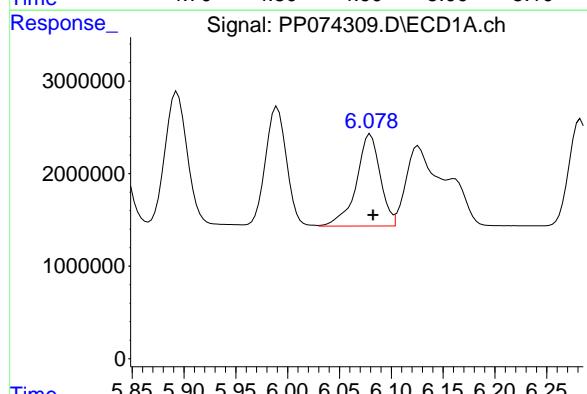


#22 AR-1248-2

R.T.: 6.080 min
 Delta R.T.: -0.003 min
 Response: 15956878
 Conc: 396.34 ng/ml

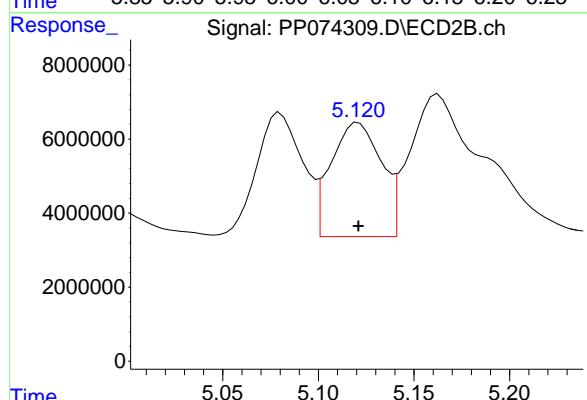

#22 AR-1248-2


R.T.: 5.121 min
 Delta R.T.: 0.000 min
 Response: 56446484
 Conc: 385.79 ng/ml

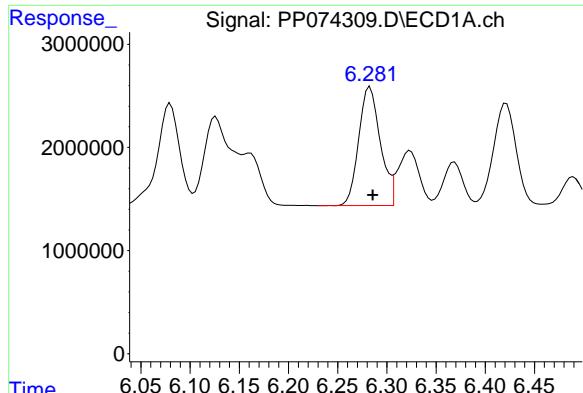

#23 AR-1248-3


R.T.: 6.283 min
 Delta R.T.: -0.003 min
 Response: 17574695
 Conc: 394.29 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

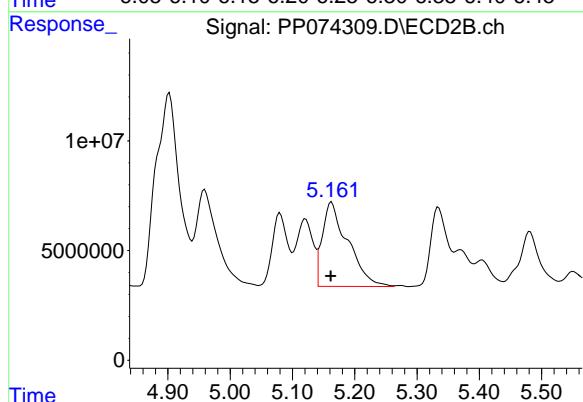


#23 AR-1248-3

R.T.: 5.163 min
 Delta R.T.: 0.001 min
 Response: 109665710
 Conc: 639.60 ng/ml

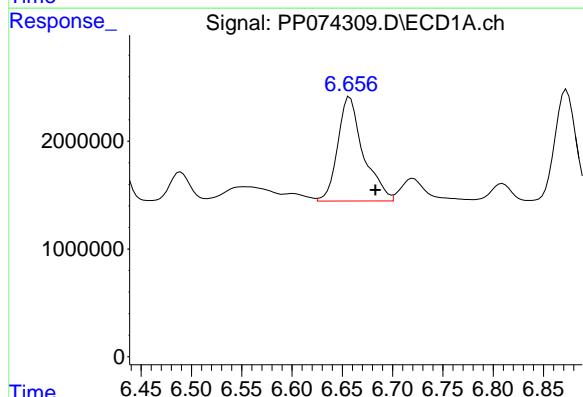


#24 AR-1248-4

R.T.: 6.658 min
 Delta R.T.: -0.025 min
 Response: 17077329
 Conc: 328.18 ng/ml

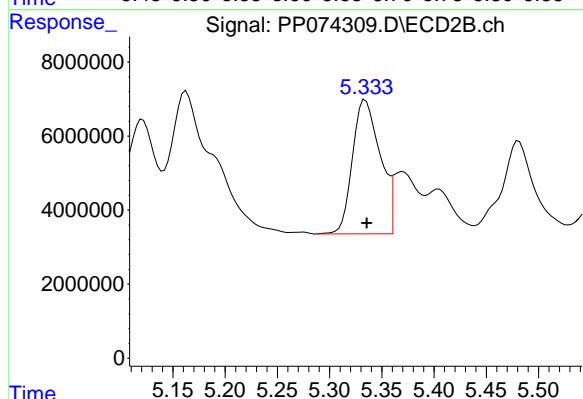

#24 AR-1248-4


R.T.: 5.334 min
 Delta R.T.: -0.001 min
 Response: 66942868
 Conc: 402.36 ng/ml



#25 AR-1248-5


R.T.: 6.720 min
 Delta R.T.: -0.002 min
 Response: 3662834
 Conc: 64.32 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

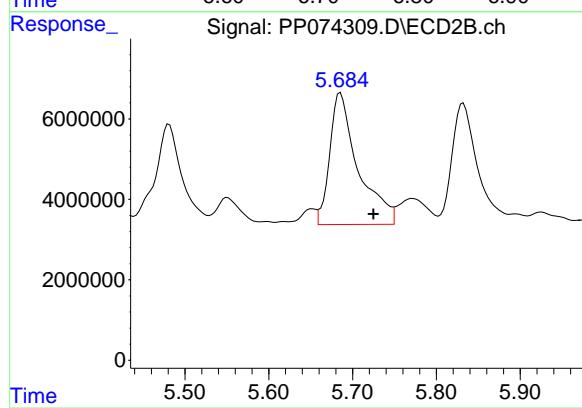


#25 AR-1248-5

R.T.: 5.686 min
 Delta R.T.: -0.040 min
 Response: 76796260
 Conc: 263.94 ng/ml




#26 AR-1254-1

R.T.: 6.658 min
 Delta R.T.: 0.000 min
 Response: 17077329
 Conc: 324.41 ng/ml

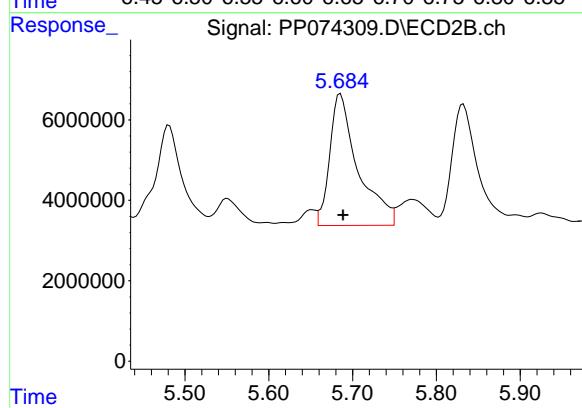

#26 AR-1254-1


R.T.: 5.686 min
 Delta R.T.: -0.003 min
 Response: 76796260
 Conc: 209.72 ng/ml



#27 AR-1254-2


R.T.: 6.873 min
 Delta R.T.: -0.002 min
 Response: 14942029
 Conc: 187.94 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

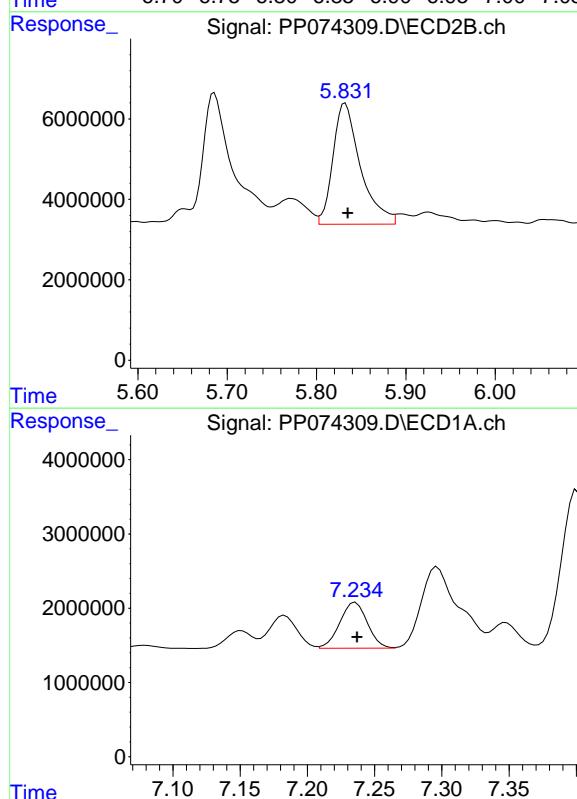


#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: -0.001 min
 Response: 8784278
 Conc: 100.60 ng/ml

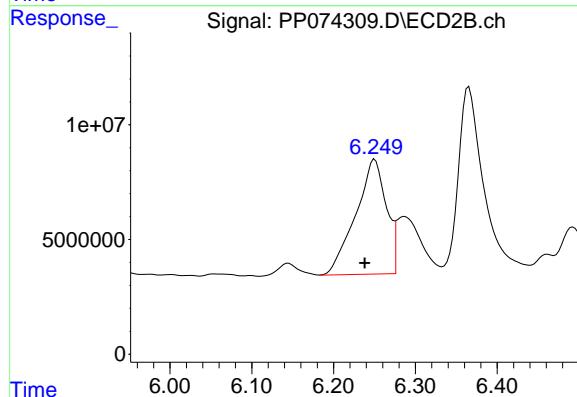

#28 AR-1254-3

R.T.: 6.250 min
 Delta R.T.: 0.012 min
 Response: 129756889
 Conc: 265.24 ng/ml

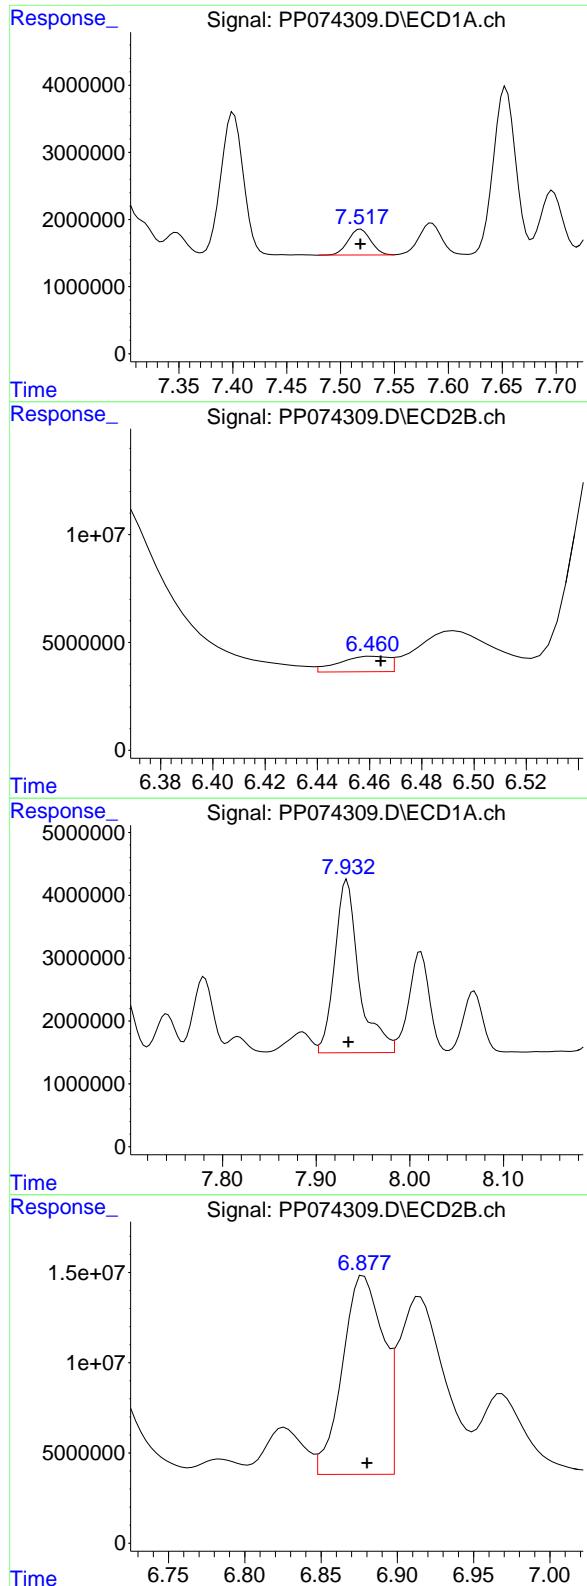

#29 AR-1254-4

R.T.: 7.519 min
 Delta R.T.: 0.000 min
 Response: 5607113
 Conc: 87.87 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#29 AR-1254-4


R.T.: 6.462 min
 Delta R.T.: -0.003 min
 Response: 9342145
 Conc: 25.42 ng/ml

#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: -0.001 min
 Response: 49832102
 Conc: 614.11 ng/ml

#30 AR-1254-5


R.T.: 6.878 min
 Delta R.T.: -0.002 min
 Response: 203492933
 Conc: 528.32 ng/ml

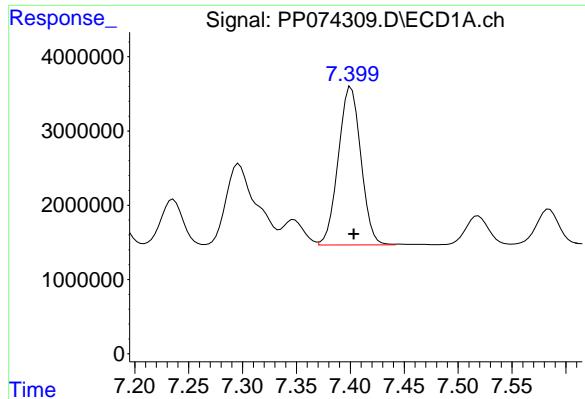

#31 AR-1260-1


R.T.: 7.401 min
 Delta R.T.: -0.002 min
 Response: 31033148
 Conc: 550.66 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

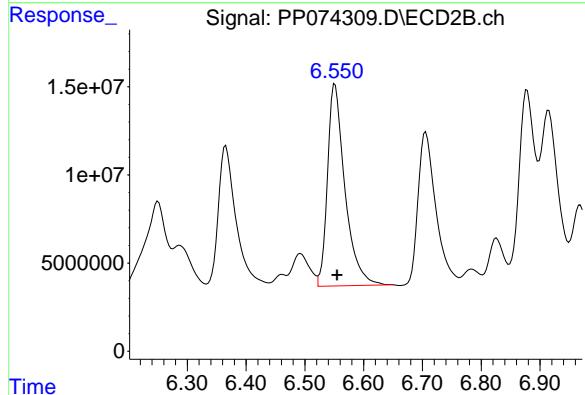


#31 AR-1260-1

R.T.: 6.551 min
 Delta R.T.: -0.004 min
 Response: 236107273
 Conc: 584.49 ng/ml

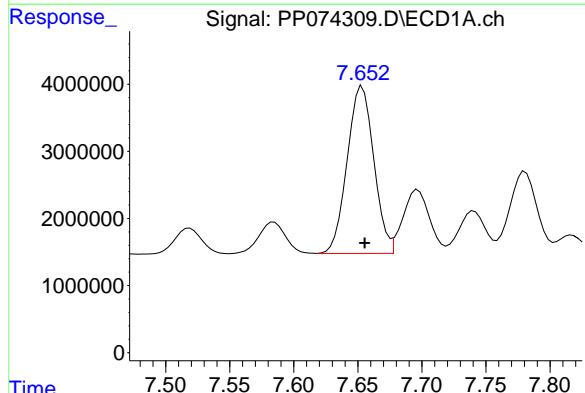


#32 AR-1260-2

R.T.: 7.653 min
 Delta R.T.: -0.002 min
 Response: 36070118
 Conc: 529.26 ng/ml

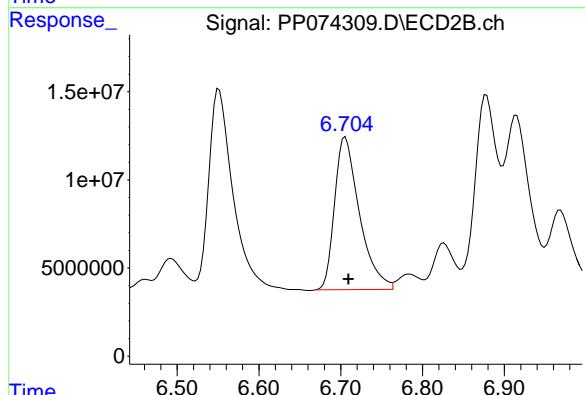

#32 AR-1260-2


R.T.: 6.706 min
 Delta R.T.: -0.004 min
 Response: 182527346
 Conc: 583.72 ng/ml

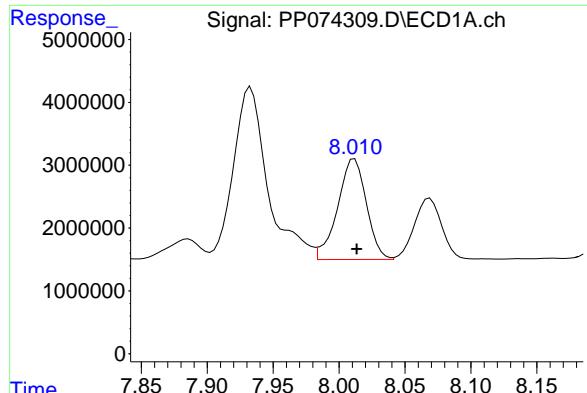

#33 AR-1260-3


R.T.: 8.012 min
 Delta R.T.: -0.002 min
 Response: 24314378
 Conc: 456.21 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

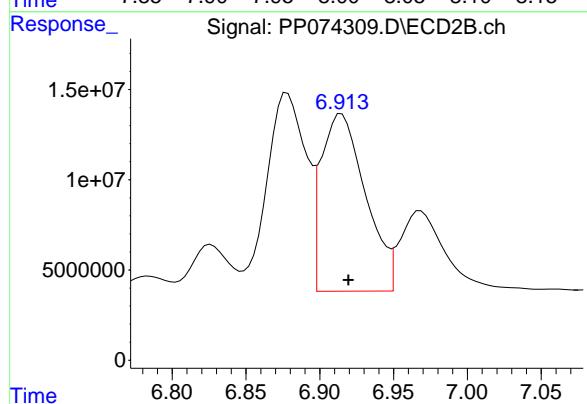


#33 AR-1260-3

R.T.: 6.915 min
 Delta R.T.: -0.005 min
 Response: 204932581
 Conc: 519.98 ng/ml

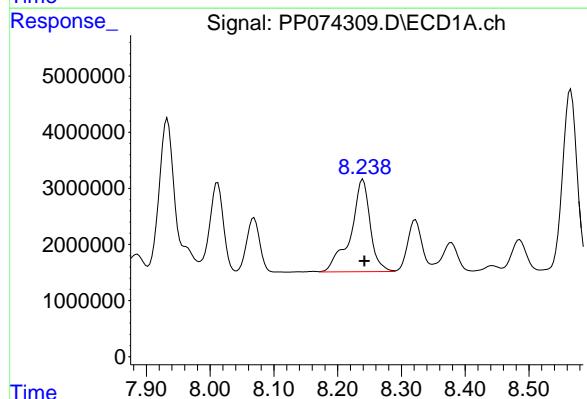


#34 AR-1260-4

R.T.: 8.240 min
 Delta R.T.: -0.002 min
 Response: 34948406
 Conc: 558.15 ng/ml

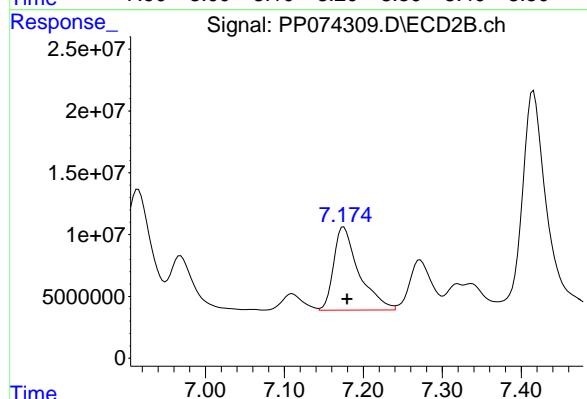

#34 AR-1260-4


R.T.: 7.175 min
 Delta R.T.: -0.004 min
 Response: 149384307
 Conc: 513.38 ng/ml

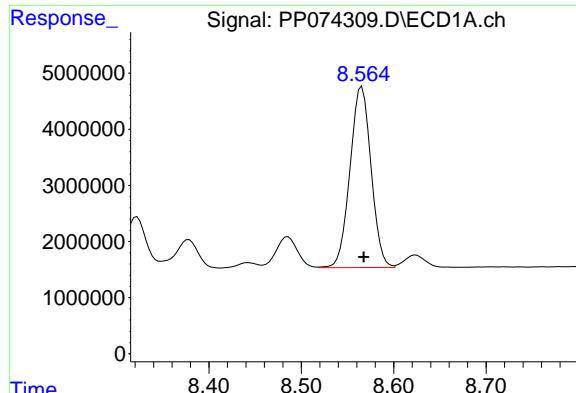

#35 AR-1260-5


R.T.: 8.566 min
 Delta R.T.: -0.002 min
 Response: 51128845
 Conc: 451.25 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

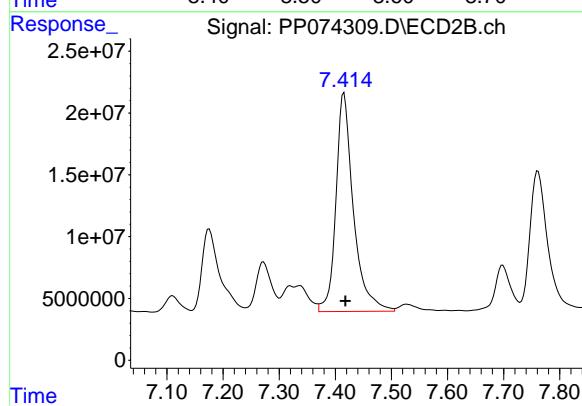


#35 AR-1260-5

R.T.: 7.415 min
 Delta R.T.: -0.003 min
 Response: 382812137
 Conc: 505.42 ng/ml

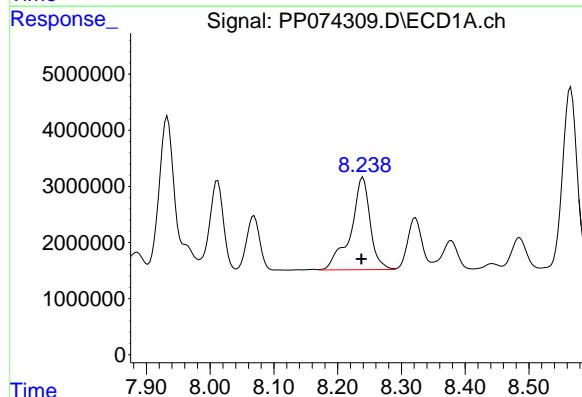


#36 AR-1262-1

R.T.: 8.240 min
 Delta R.T.: 0.002 min
 Response: 34948406
 Conc: 461.12 ng/ml

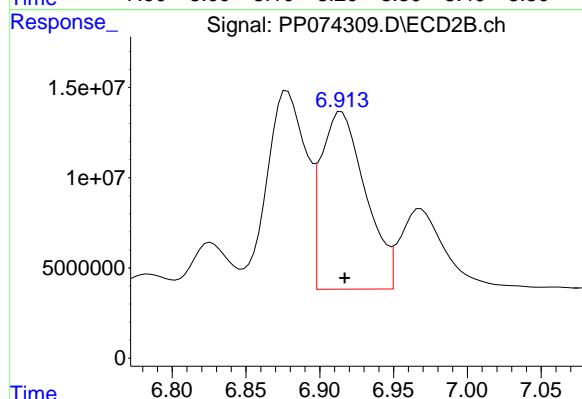

#36 AR-1262-1

R.T.: 6.915 min
 Delta R.T.: -0.002 min
 Response: 204932581
 Conc: 363.91 ng/ml

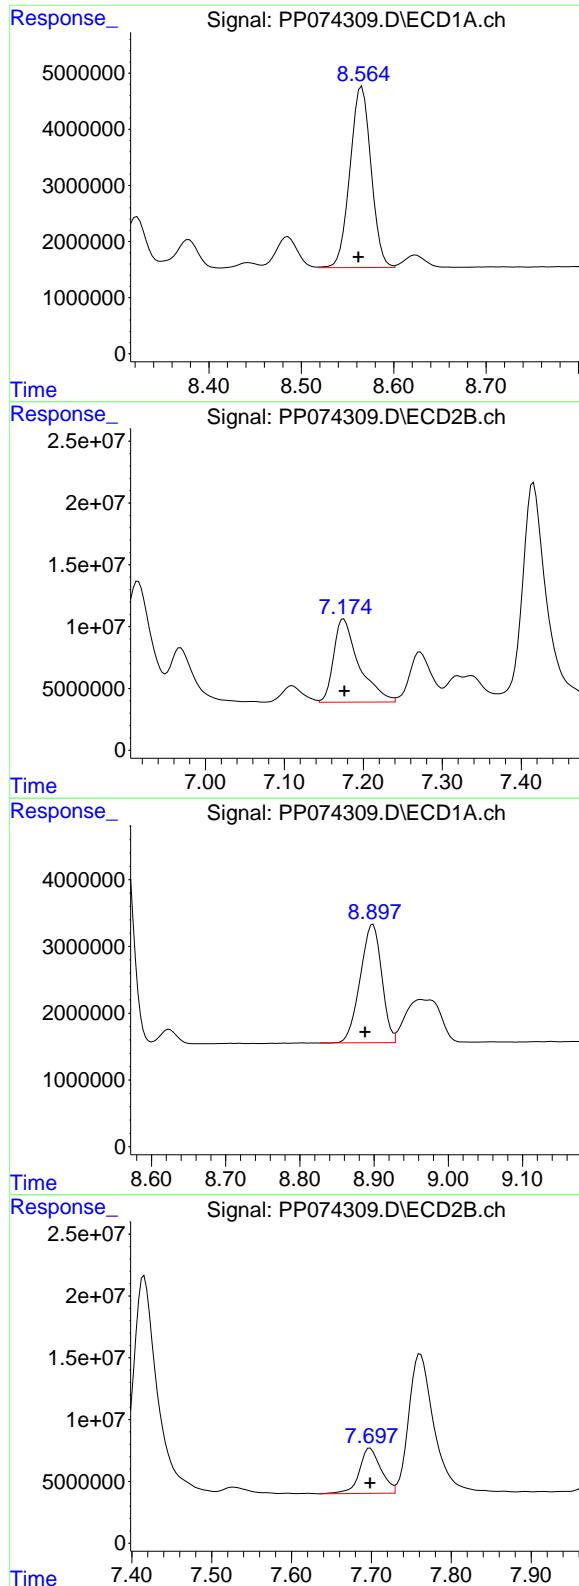

#37 AR-1262-2

R.T.: 8.566 min
 Delta R.T.: 0.004 min
 Response: 51128845
 Conc: 392.00 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#37 AR-1262-2


R.T.: 7.175 min
 Delta R.T.: 0.000 min
 Response: 149384307
 Conc: 372.51 ng/ml

#38 AR-1262-3

R.T.: 8.899 min
 Delta R.T.: 0.010 min
 Response: 35659813
 Conc: 379.07 ng/ml

#38 AR-1262-3

R.T.: 7.698 min
 Delta R.T.: 0.000 min
 Response: 68577315
 Conc: 190.77 ng/ml

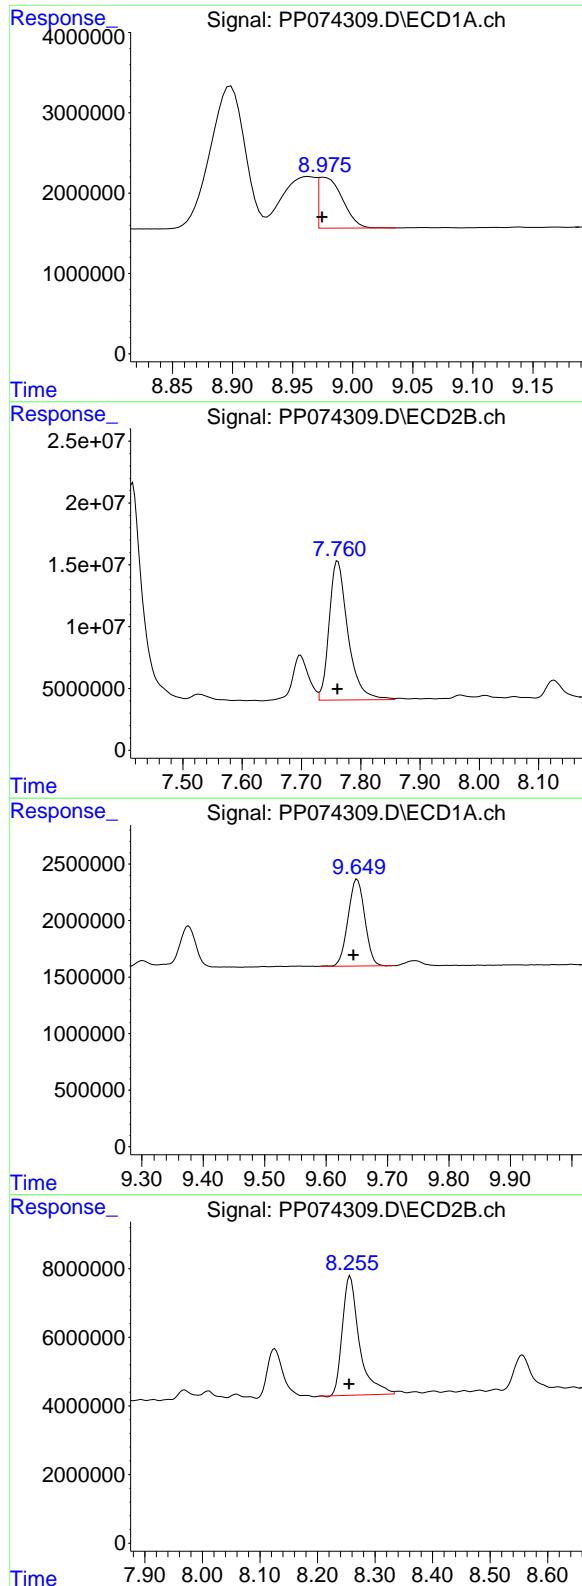

#39 AR-1262-4

R.T.: 8.976 min
 Delta R.T.: 0.002 min
 Response: 8821459
 Conc: 121.09 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#39 AR-1262-4


R.T.: 7.761 min
 Delta R.T.: 0.000 min
 Response: 247472529
 Conc: 371.07 ng/ml

#40 AR-1262-5

R.T.: 9.651 min
 Delta R.T.: 0.006 min
 Response: 14529552
 Conc: 285.33 ng/ml

#40 AR-1262-5

R.T.: 8.257 min
 Delta R.T.: 0.002 min
 Response: 71597111
 Conc: 252.75 ng/ml

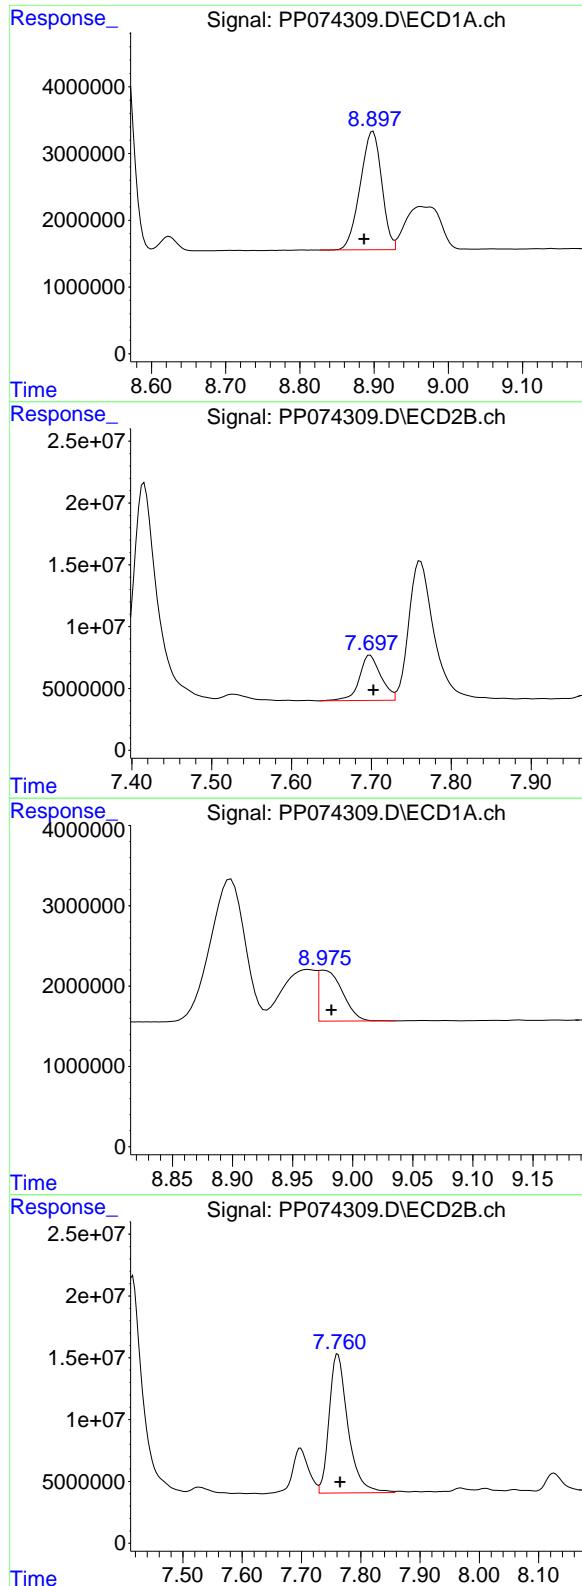

#41 AR-1268-1

R.T.: 8.899 min
 Delta R.T.: 0.012 min
 Response: 35659813
 Conc: 229.13 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#41 AR-1268-1


R.T.: 7.698 min
 Delta R.T.: -0.004 min
 Response: 68577315
 Conc: 62.90 ng/ml

#42 AR-1268-2

R.T.: 8.976 min
 Delta R.T.: -0.006 min
 Response: 8821459
 Conc: 61.51 ng/ml

#42 AR-1268-2

R.T.: 7.761 min
 Delta R.T.: -0.004 min
 Response: 247472529
 Conc: 233.17 ng/ml

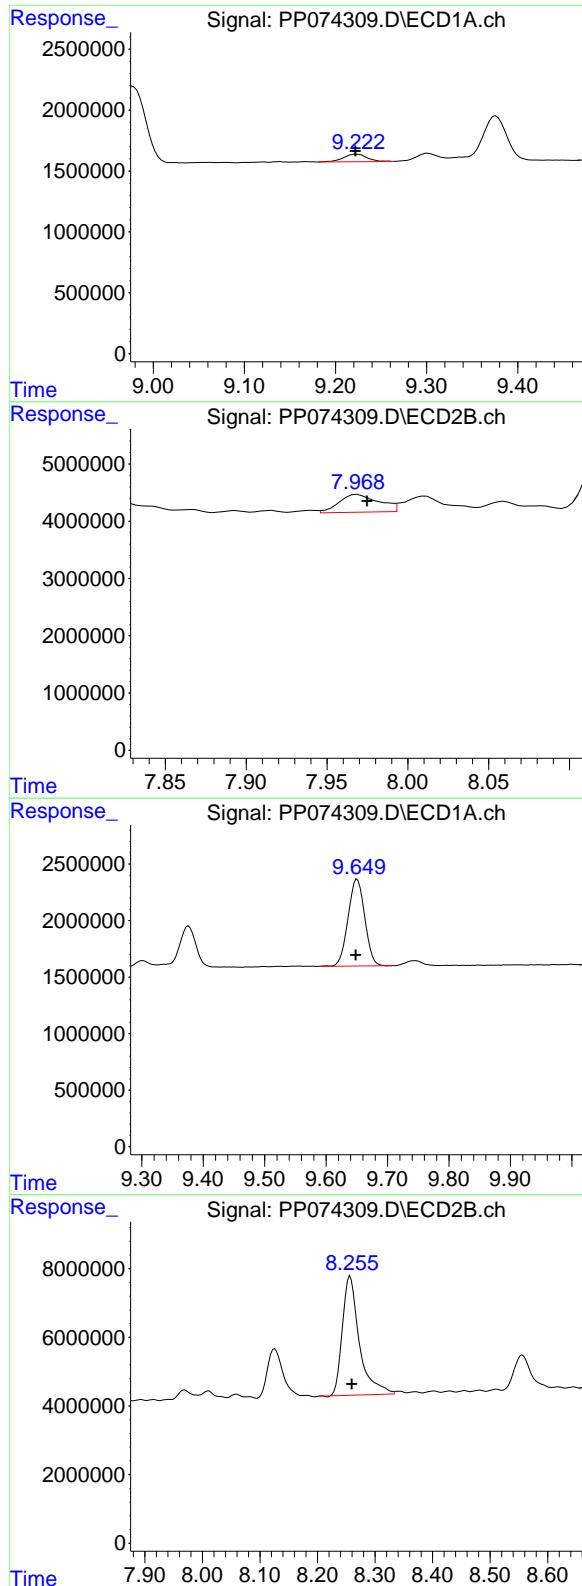

#43 AR-1268-3

R.T.: 9.224 min
 Delta R.T.: 0.002 min
 Response: 1133561
 Conc: 9.49 ng/ml

Instrument: ECD_P
 ClientSampleId: PB169205BS

#43 AR-1268-3


R.T.: 7.969 min
 Delta R.T.: -0.006 min
 Response: 5277612
 Conc: 6.34 ng/ml

#44 AR-1268-4

R.T.: 9.651 min
 Delta R.T.: 0.003 min
 Response: 14529552
 Conc: 247.05 ng/ml

#44 AR-1268-4

R.T.: 8.257 min
 Delta R.T.: -0.002 min
 Response: 71597111
 Conc: 232.41 ng/ml

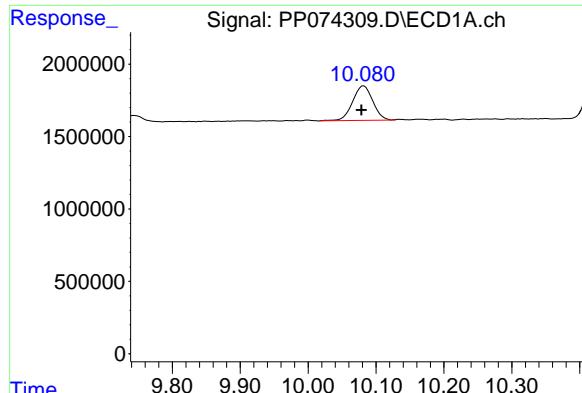

#45 AR-1268-5


R.T.: 10.082 min
Delta R.T.: 0.003 min
Response: 4915065
Conc: 13.98 ng/ml

Instrument:

ECD_P

ClientSampleId :

PB169205BS

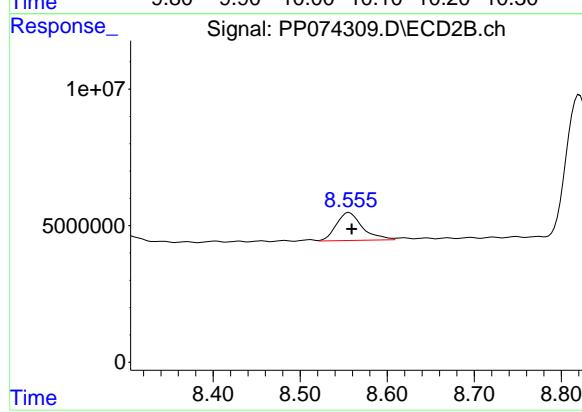

#45 AR-1268-5

R.T.: 8.556 min
Delta R.T.: -0.003 min
Response: 21332104
Conc: 8.37 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:37
 Operator : YP\AJ
 Sample : Q2830-01MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.657 | 3.800 | 29282786 | 84433109 | 26.185 | 22.020 |
| 2) SA Decachlor... | 10.437 | 8.820 | 19335273 | 105.2E6 | 19.909 | 17.488 |

Target Compounds

| | | | | | | |
|------------------|-------|--------|----------|----------|----------|------------|
| 3) L1 AR-1016-1 | 5.809 | 4.901 | 21480557 | 221.4E6 | 520.655 | 555.093 |
| 4) L1 AR-1016-2 | 5.831 | 4.958 | 31794685 | 105.4E6 | 523.441 | 561.178 |
| 5) L1 AR-1016-3 | 5.894 | 5.079 | 20638950 | 60560553 | 520.390 | 570.951 |
| 6) L1 AR-1016-4 | 5.991 | 5.119 | 17736155 | 58694992 | 544.982 | 537.401 |
| 7) L1 AR-1016-5 | 6.283 | 5.334 | 16474757 | 64653966 | 507.414 | 552.772 |
| 8) L2 AR-1221-1 | 4.853 | 4.014 | 2579183 | 7629131 | 153.856 | 155.426 |
| 9) L2 AR-1221-2 | 4.942 | 4.093 | 3210890 | 10889786 | 254.811 | 303.427 |
| 10) L2 AR-1221-3 | 5.018 | 4.174 | 12557806 | 45555195 | 342.780 | 336.886 |
| 11) L3 AR-1232-1 | 5.018 | 4.174 | 12557806 | 45555195 | 432.471 | 449.429 |
| 12) L3 AR-1232-2 | 5.545 | 4.901 | 16277760 | 221.4E6 | 1082.103 | 1270.582 |
| 13) L3 AR-1232-3 | 5.831 | 5.079 | 31794685 | 60560553 | 1096.304 | 1321.803 |
| 14) L3 AR-1232-4 | 5.991 | 5.161 | 17736155 | 109.7E6 | 1146.574 | 1891.791 # |
| 15) L3 AR-1232-5 | 6.080 | 5.334 | 15686090 | 64653966 | 1338.859 | 1376.218 |
| 16) L4 AR-1242-1 | 5.809 | 4.901 | 21480557 | 221.4E6 | 576.415 | 641.534 |
| 17) L4 AR-1242-2 | 5.831 | 4.958 | 31794685 | 105.4E6 | 584.365 | 645.096 |
| 18) L4 AR-1242-3 | 5.894 | 5.079 | 20638950 | 60560553 | 577.542 | 656.494 |
| 19) L4 AR-1242-4 | 5.991 | 5.161 | 17736155 | 109.7E6 | 607.015 | 918.964 # |
| 20) L4 AR-1242-5 | 6.720 | 5.684 | 3440400 | 76642613 | 96.755 | 512.454 # |
| 21) L5 AR-1248-1 | 5.809 | 4.901 | 21480557 | 221.4E6 | 766.765 | 1035.001 # |
| 22) L5 AR-1248-2 | 6.080 | 5.119 | 15686090 | 58694992 | 389.609 | 401.162 |
| 23) L5 AR-1248-3 | 6.283 | 5.161 | 16474757 | 109.7E6 | 369.608 | 640.057 # |
| 24) L5 AR-1248-4 | 6.657 | 5.334 | 15791645 | 64653966 | 303.469 | 388.607 # |
| 25) L5 AR-1248-5 | 6.720 | 5.684f | 3440400 | 76642613 | 60.418 | 263.407 # |
| 26) L6 AR-1254-1 | 6.657 | 5.684 | 15791645 | 76642613 | 299.987 | 209.302 # |
| 27) L6 AR-1254-2 | 6.873 | 5.831 | 13769891 | 62702065 | 173.196 | 225.371 # |
| 28) L6 AR-1254-3 | 7.236 | 6.249 | 7976373 | 123.3E6 | 91.350 | 252.126 # |
| 29) L6 AR-1254-4 | 7.518 | 6.459 | 5089508 | 8449703 | 79.761 | 22.988 # |
| 30) L6 AR-1254-5 | 7.933 | 6.877 | 44898403 | 177.0E6 | 553.312 | 459.617 |
| 31) L7 AR-1260-1 | 7.400 | 6.550 | 28140334 | 207.0E6 | 499.331 | 512.404 |
| 32) L7 AR-1260-2 | 7.653 | 6.704 | 32575808 | 157.6E6 | 477.985 | 503.902 |
| 33) L7 AR-1260-3 | 8.012 | 6.914 | 21771827 | 176.5E6 | 408.508 | 447.876 |
| 34) L7 AR-1260-4 | 8.240 | 7.175 | 32485197 | 132.7E6 | 518.809 | 455.876 |
| 35) L7 AR-1260-5 | 8.566 | 7.413 | 45863963 | 335.1E6 | 404.784 | 442.376 |
| 36) L8 AR-1262-1 | 8.240 | 6.914 | 32485197 | 176.5E6 | 428.623 | 313.448 # |
| 37) L8 AR-1262-2 | 8.566 | 7.175 | 45863963 | 132.7E6 | 351.637 | 330.780 |
| 38) L8 AR-1262-3 | 8.898 | 7.697 | 31725032 | 60525419 | 337.246 | 168.374 # |
| 39) L8 AR-1262-4 | 8.974 | 7.759 | 18734714 | 215.3E6 | 257.162 | 322.852 # |
| 40) L8 AR-1262-5 | 9.651 | 8.255 | 13091860 | 62242150 | 257.093 | 219.729 |
| 41) L9 AR-1268-1 | 8.898 | 7.697 | 31725032 | 60525419 | 203.845 | 55.514 # |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074311.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:37
 Operator : YP\AJ
 Sample : Q2830-01MS
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:12 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|--------|-------|----------|----------|---------|-----------|
| 42) L9 AR-1268-2 | 8.974 | 7.759 | 18734714 | 215.3E6 | 130.623 | 202.875 # |
| 43) L9 AR-1268-3 | 9.223 | 7.969 | 1275907 | 4368524 | 10.679 | 5.251 # |
| 44) L9 AR-1268-4 | 9.651 | 8.255 | 13091860 | 62242150 | 222.603 | 202.046 |
| 45) L9 AR-1268-5 | 10.081 | 8.554 | 4477807 | 18194131 | 12.732 | 7.135 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074311.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 13:37
Operator : YP\AJ
Sample : Q2830-01MS
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

```
Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 12 14:50:12 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title  : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation
```

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

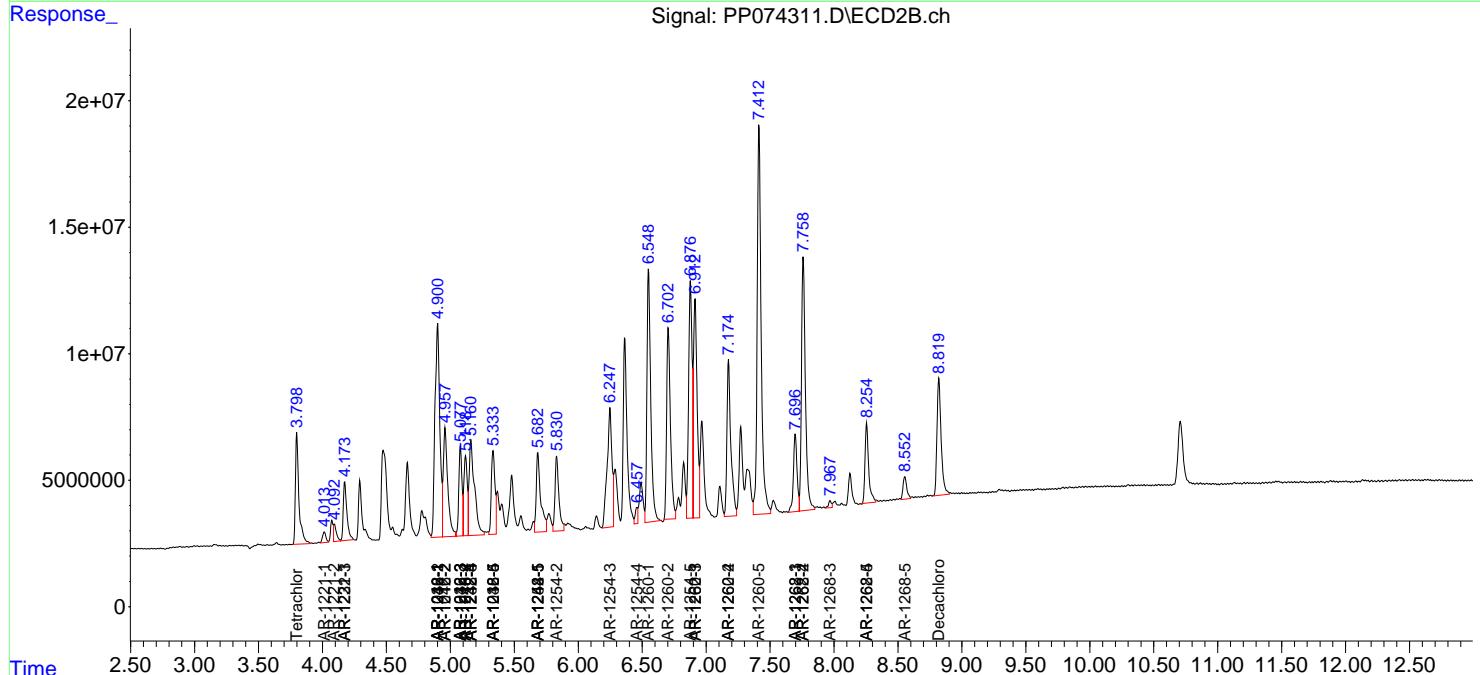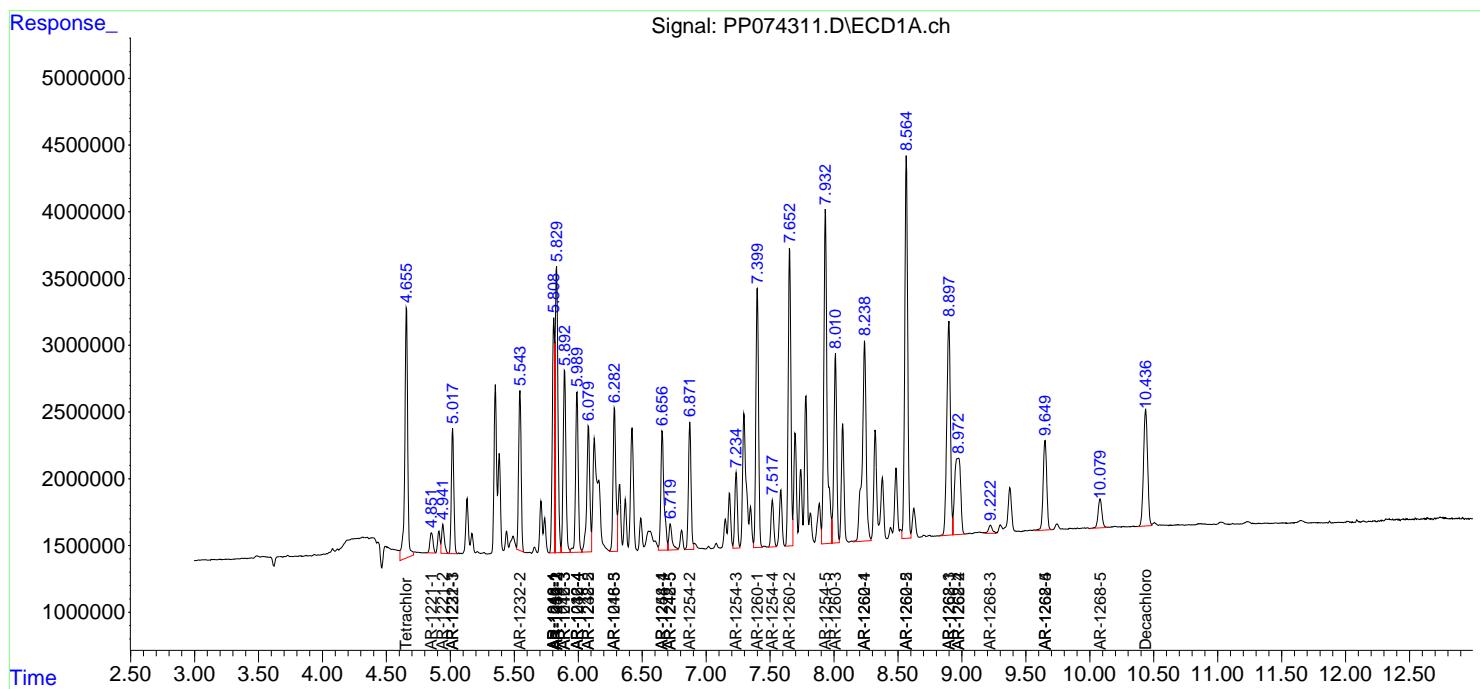




#1 Tetrachloro-m-xylene


R.T.: 4.657 min
Delta R.T.: -0.003 min
Response: 29282786
Conc: 26.18 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

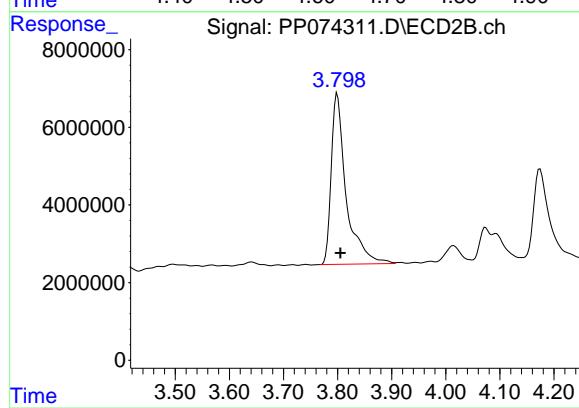


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: -0.006 min
Response: 84433109
Conc: 22.02 ng/ml

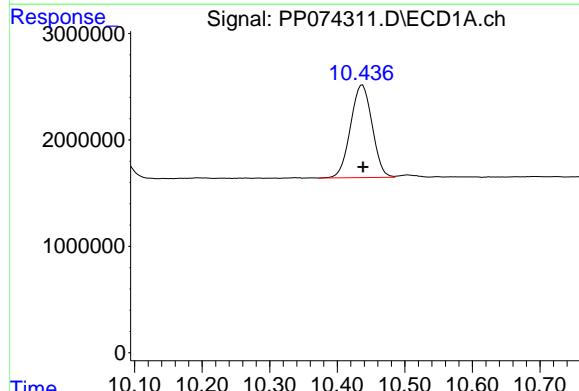


#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.000 min
Response: 19335273
Conc: 19.91 ng/ml

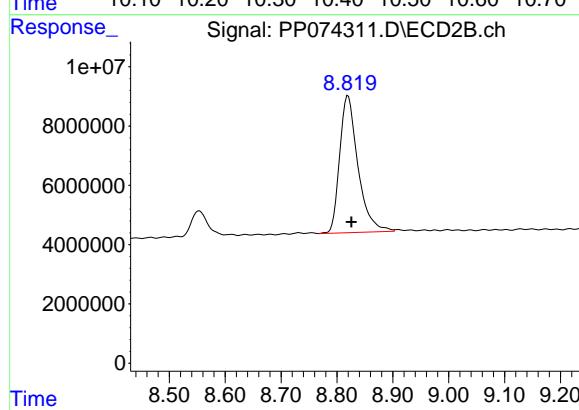

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 105164574
Conc: 17.49 ng/ml

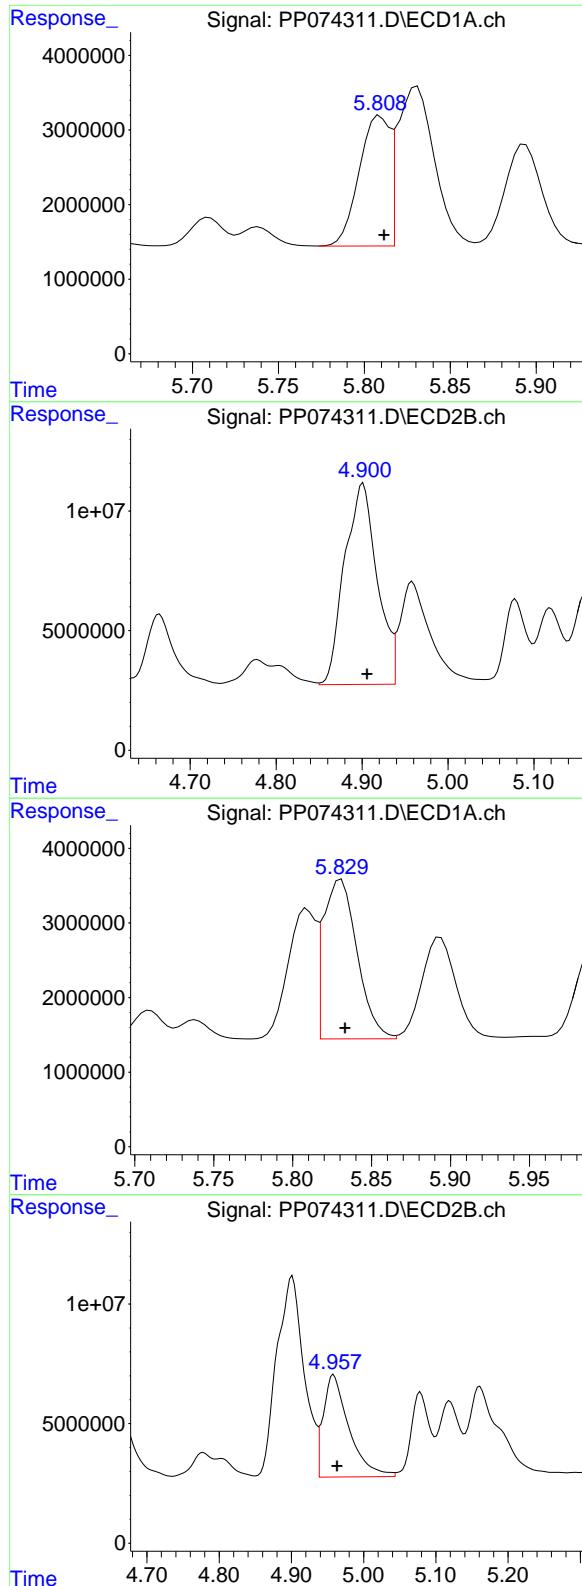

#3 AR-1016-1

R.T.: 5.809 min
 Delta R.T.: -0.002 min
 Response: 21480557
 Conc: 520.65 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#3 AR-1016-1


R.T.: 4.901 min
 Delta R.T.: -0.004 min
 Response: 221419556
 Conc: 555.09 ng/ml

#4 AR-1016-2

R.T.: 5.831 min
 Delta R.T.: -0.003 min
 Response: 31794685
 Conc: 523.44 ng/ml

#4 AR-1016-2


R.T.: 4.958 min
 Delta R.T.: -0.005 min
 Response: 105394294
 Conc: 561.18 ng/ml

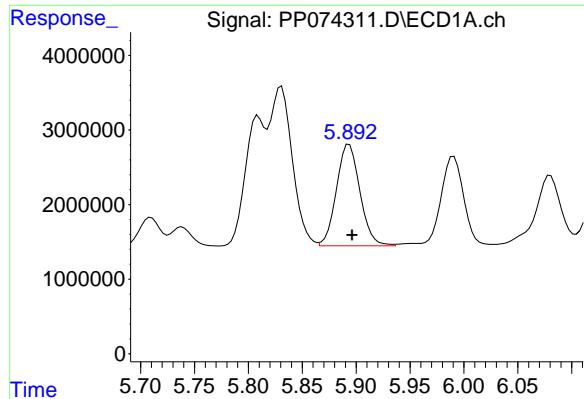

#5 AR-1016-3


R.T.: 5.894 min
 Delta R.T.: -0.003 min
 Response: 20638950
 Conc: 520.39 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

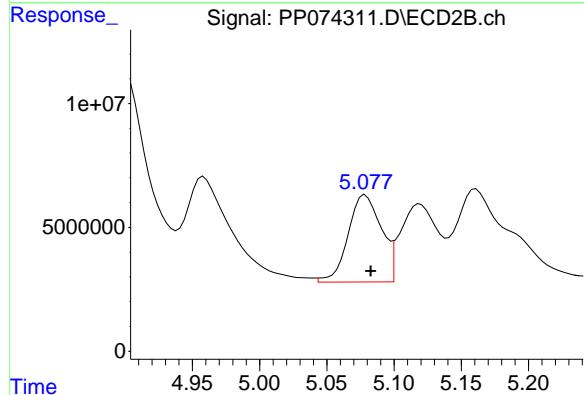


#5 AR-1016-3

R.T.: 5.079 min
 Delta R.T.: -0.004 min
 Response: 60560553
 Conc: 570.95 ng/ml

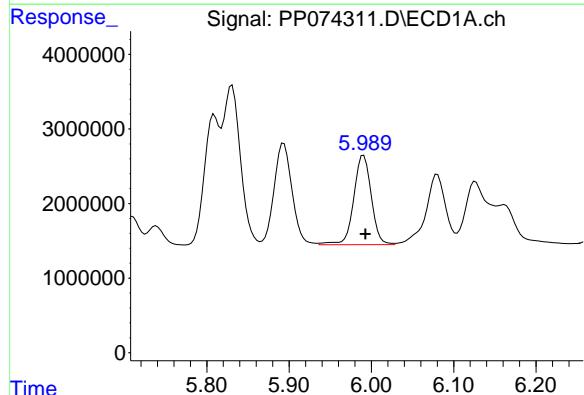


#6 AR-1016-4

R.T.: 5.991 min
 Delta R.T.: -0.002 min
 Response: 17736155
 Conc: 544.98 ng/ml

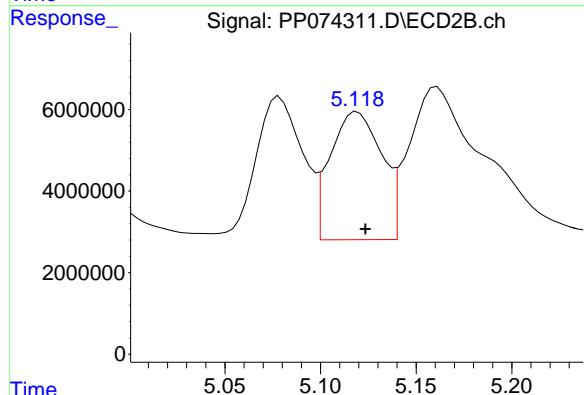

#6 AR-1016-4

R.T.: 5.119 min
 Delta R.T.: -0.004 min
 Response: 58694992
 Conc: 537.40 ng/ml

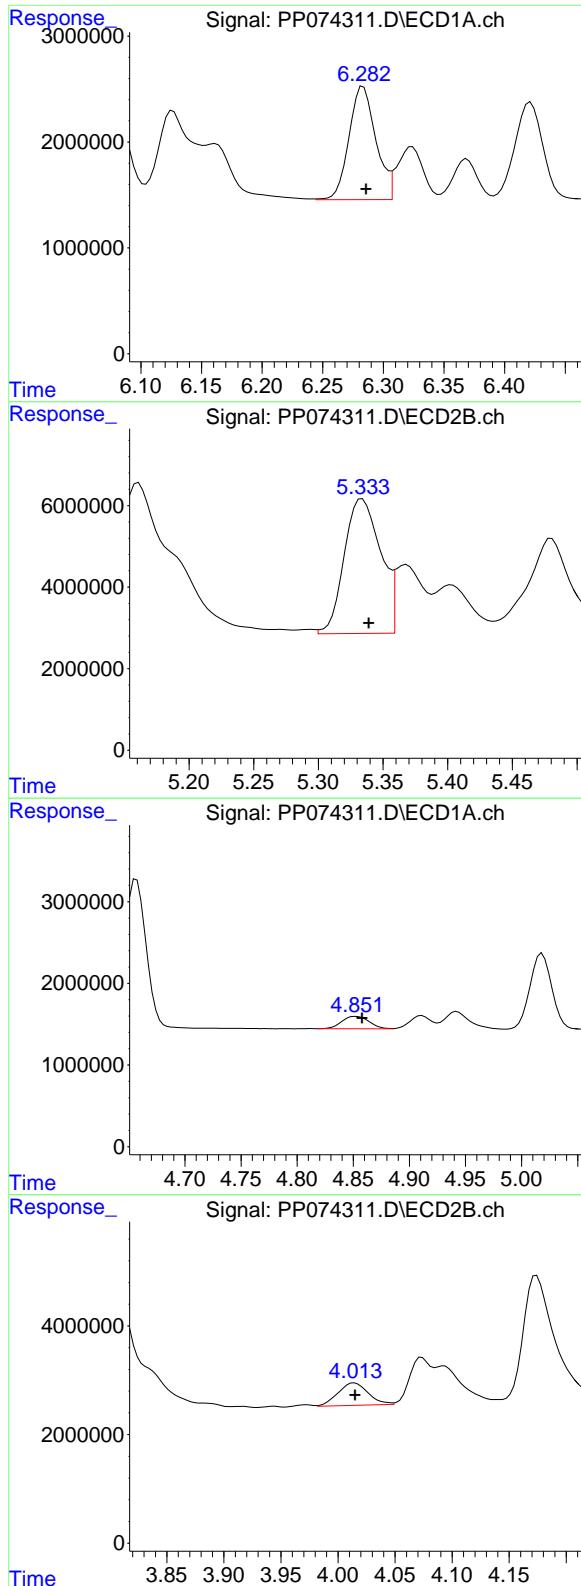

#7 AR-1016-5

R.T.: 6.283 min
 Delta R.T.: -0.002 min
 Response: 16474757
 Conc: 507.41 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#7 AR-1016-5


R.T.: 5.334 min
 Delta R.T.: -0.005 min
 Response: 64653966
 Conc: 552.77 ng/ml

#8 AR-1221-1

R.T.: 4.853 min
 Delta R.T.: -0.005 min
 Response: 2579183
 Conc: 153.86 ng/ml

#8 AR-1221-1


R.T.: 4.014 min
 Delta R.T.: 0.000 min
 Response: 7629131
 Conc: 155.43 ng/ml

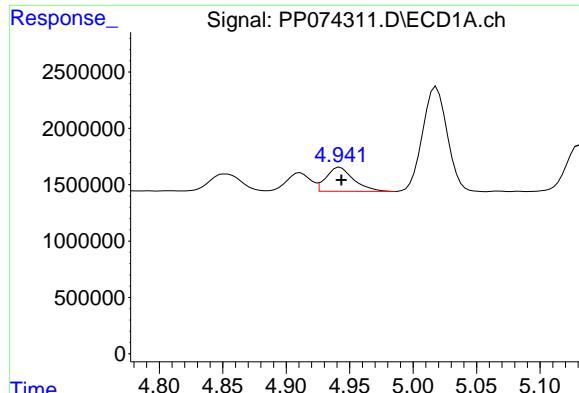

#9 AR-1221-2


R.T.: 4.942 min
 Delta R.T.: -0.001 min
 Response: 3210890
 Conc: 254.81 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

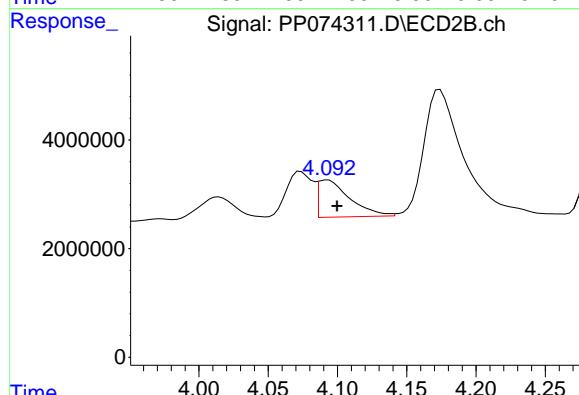


#9 AR-1221-2

R.T.: 4.093 min
 Delta R.T.: -0.007 min
 Response: 10889786
 Conc: 303.43 ng/ml

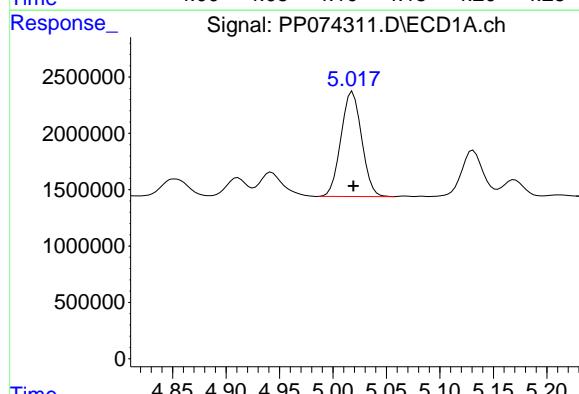


#10 AR-1221-3

R.T.: 5.018 min
 Delta R.T.: 0.000 min
 Response: 12557806
 Conc: 342.78 ng/ml

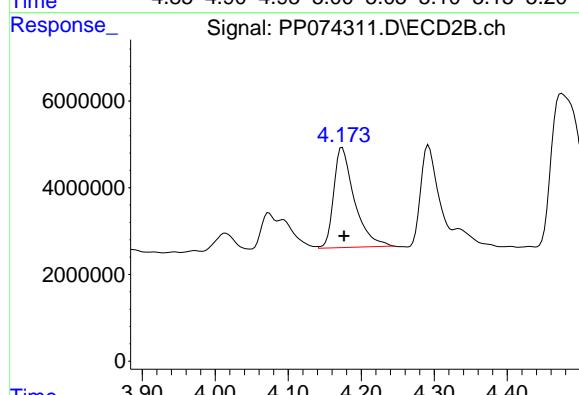

#10 AR-1221-3


R.T.: 4.174 min
 Delta R.T.: -0.002 min
 Response: 45555195
 Conc: 336.89 ng/ml

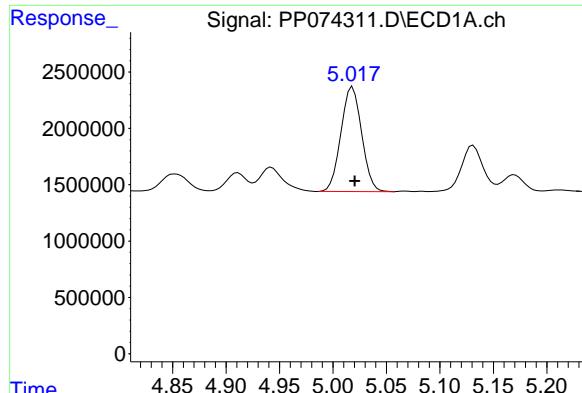

#11 AR-1232-1


R.T.: 5.018 min
 Delta R.T.: -0.002 min
 Response: 12557806
 Conc: 432.47 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVeway-TP-SOUTH-EASTMS

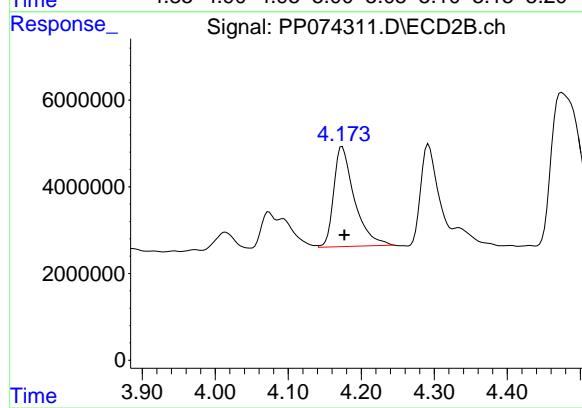


#11 AR-1232-1

R.T.: 4.174 min
 Delta R.T.: -0.003 min
 Response: 45555195
 Conc: 449.43 ng/ml

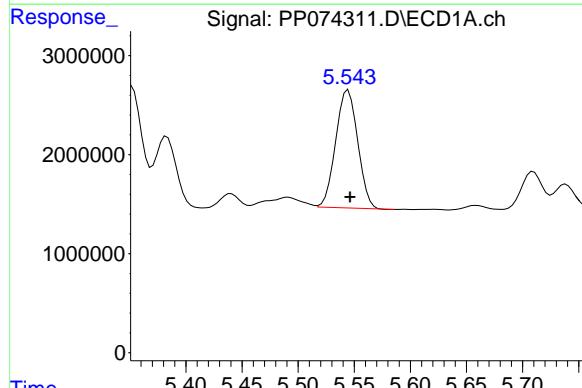


#12 AR-1232-2

R.T.: 5.545 min
 Delta R.T.: -0.002 min
 Response: 16277760
 Conc: 1082.10 ng/ml

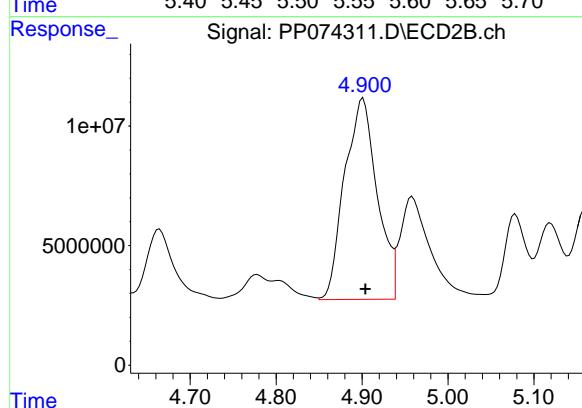

#12 AR-1232-2

R.T.: 4.901 min
 Delta R.T.: -0.003 min
 Response: 221419556
 Conc: 1270.58 ng/ml

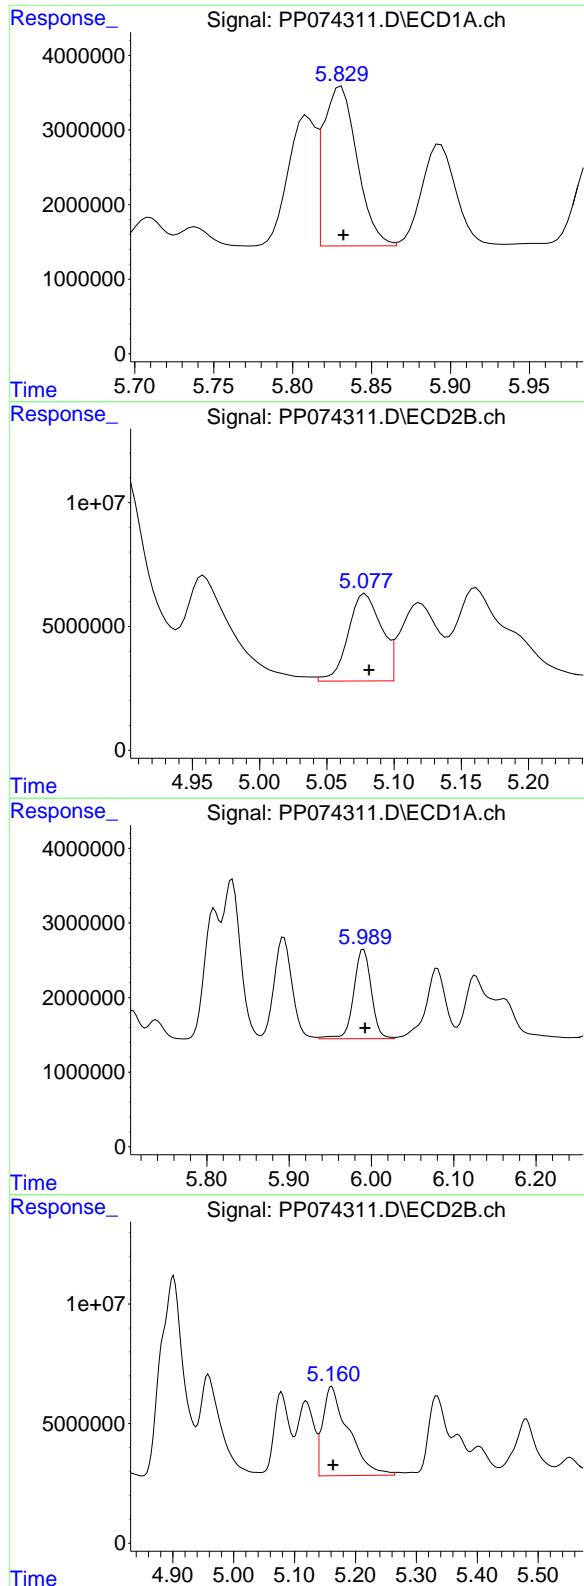

#13 AR-1232-3

R.T.: 5.831 min
 Delta R.T.: -0.001 min
 Response: 31794685
 Conc: 1096.30 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#13 AR-1232-3


R.T.: 5.079 min
 Delta R.T.: -0.003 min
 Response: 60560553
 Conc: 1321.80 ng/ml

#14 AR-1232-4

R.T.: 5.991 min
 Delta R.T.: -0.002 min
 Response: 17736155
 Conc: 1146.57 ng/ml

#14 AR-1232-4


R.T.: 5.161 min
 Delta R.T.: -0.003 min
 Response: 109744140
 Conc: 1891.79 ng/ml

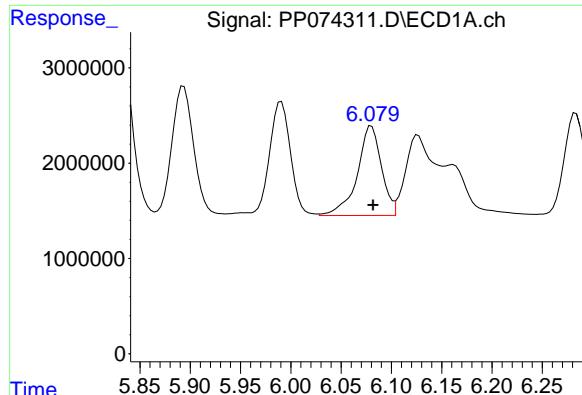

#15 AR-1232-5


R.T.: 6.080 min
 Delta R.T.: -0.002 min
 Response: 15686090
 Conc: 1338.86 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

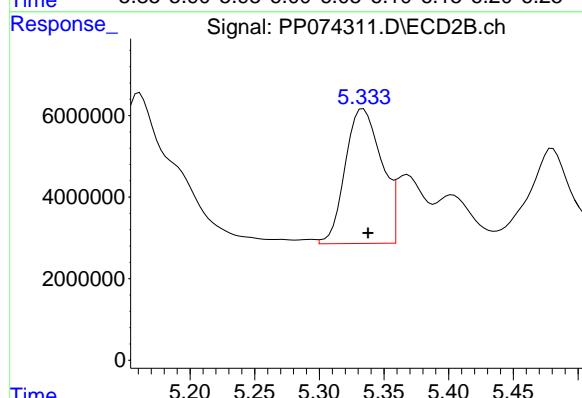


#15 AR-1232-5

R.T.: 5.334 min
 Delta R.T.: -0.004 min
 Response: 64653966
 Conc: 1376.22 ng/ml

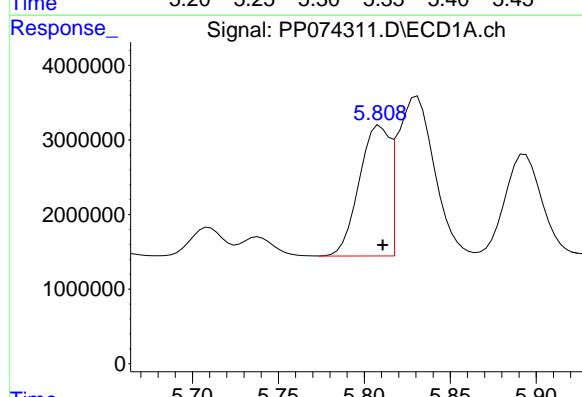


#16 AR-1242-1

R.T.: 5.809 min
 Delta R.T.: -0.002 min
 Response: 21480557
 Conc: 576.41 ng/ml

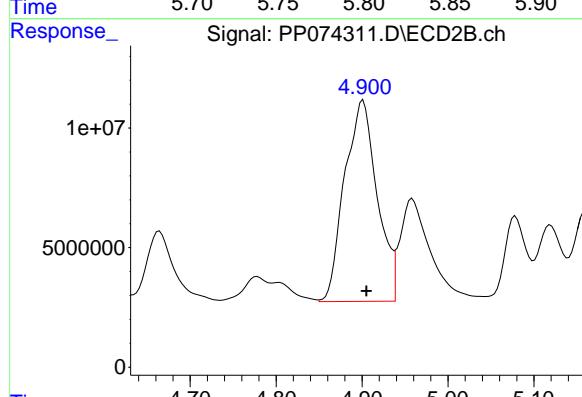

#16 AR-1242-1

R.T.: 4.901 min
 Delta R.T.: -0.004 min
 Response: 221419556
 Conc: 641.53 ng/ml

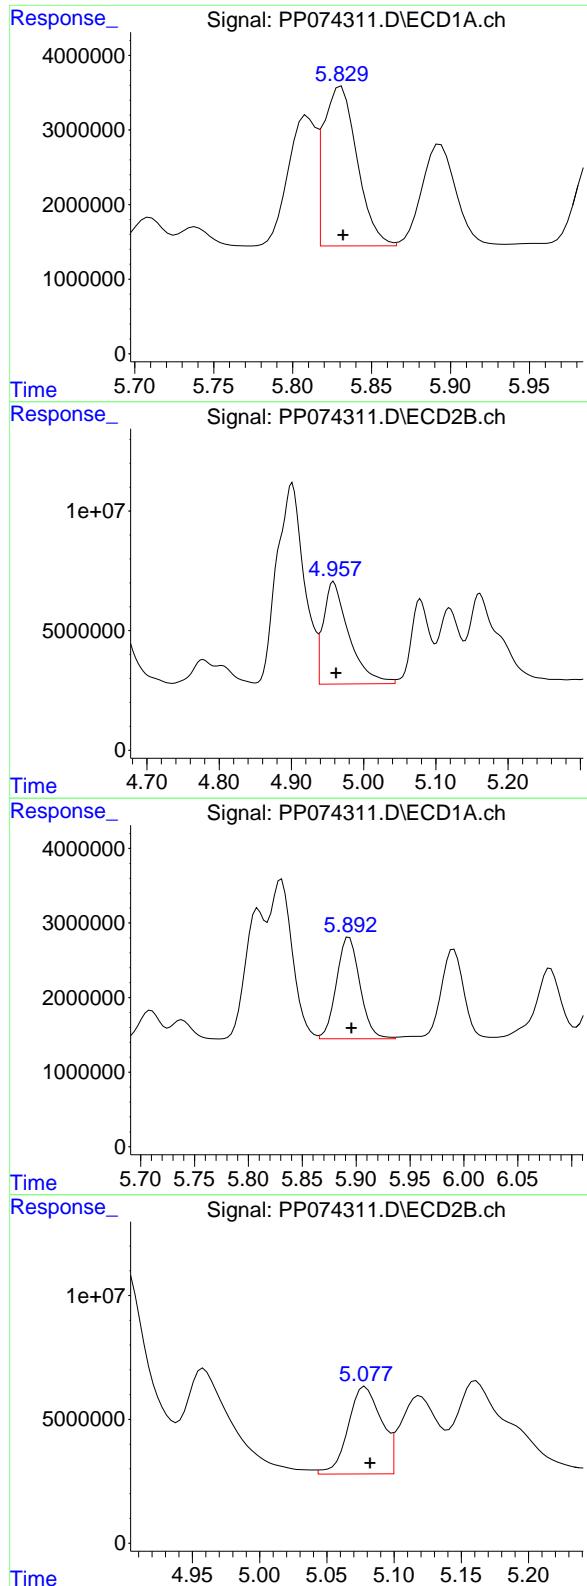

#17 AR-1242-2

R.T.: 5.831 min
 Delta R.T.: -0.001 min
 Response: 31794685
 Conc: 584.37 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#17 AR-1242-2


R.T.: 4.958 min
 Delta R.T.: -0.004 min
 Response: 105394294
 Conc: 645.10 ng/ml

#18 AR-1242-3

R.T.: 5.894 min
 Delta R.T.: -0.002 min
 Response: 20638950
 Conc: 577.54 ng/ml

#18 AR-1242-3


R.T.: 5.079 min
 Delta R.T.: -0.004 min
 Response: 60560553
 Conc: 656.49 ng/ml



#19 AR-1242-4


R.T.: 5.991 min
 Delta R.T.: -0.002 min
 Response: 17736155
 Conc: 607.01 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVeway-TP-SOUTH-EASTMS

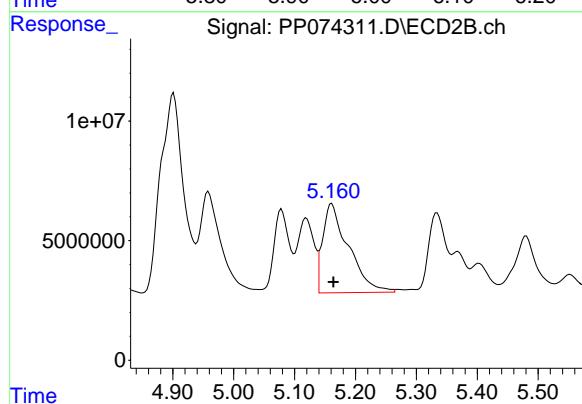


#19 AR-1242-4

R.T.: 5.161 min
 Delta R.T.: -0.003 min
 Response: 109744140
 Conc: 918.96 ng/ml

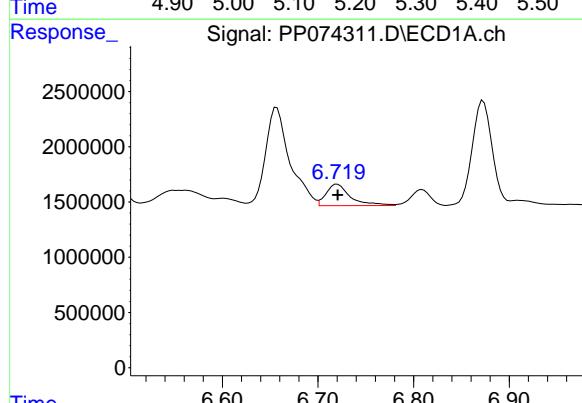


#20 AR-1242-5

R.T.: 6.720 min
 Delta R.T.: 0.000 min
 Response: 3440400
 Conc: 96.75 ng/ml

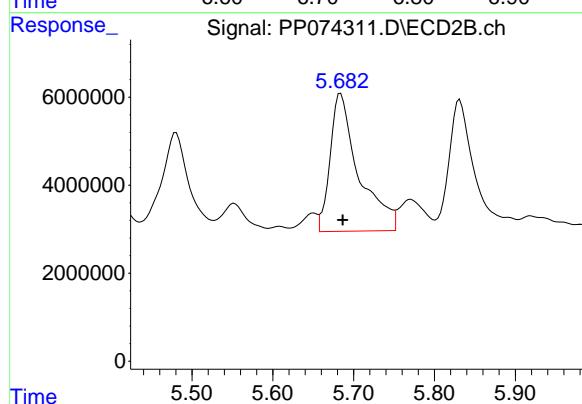

#20 AR-1242-5


R.T.: 5.684 min
 Delta R.T.: -0.002 min
 Response: 76642613
 Conc: 512.45 ng/ml

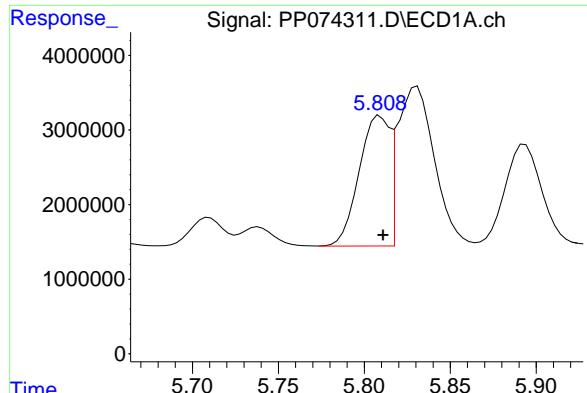

#21 AR-1248-1


R.T.: 5.809 min
 Delta R.T.: -0.002 min
 Response: 21480557
 Conc: 766.76 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

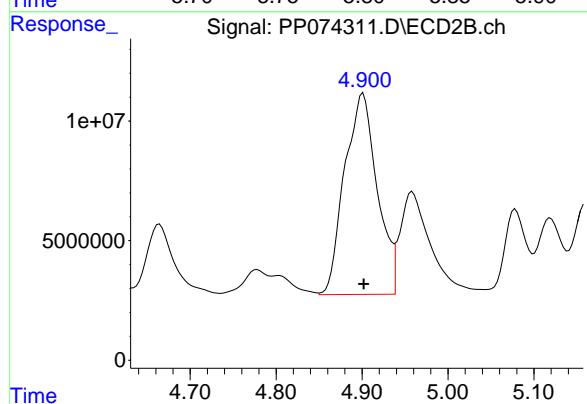


#21 AR-1248-1

R.T.: 4.901 min
 Delta R.T.: 0.000 min
 Response: 221419556
 Conc: 1035.00 ng/ml

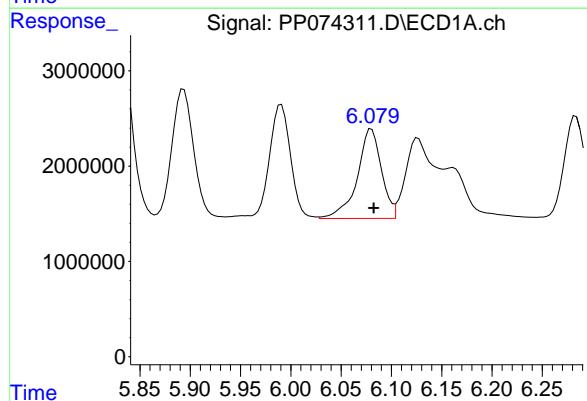


#22 AR-1248-2

R.T.: 6.080 min
 Delta R.T.: -0.002 min
 Response: 15686090
 Conc: 389.61 ng/ml

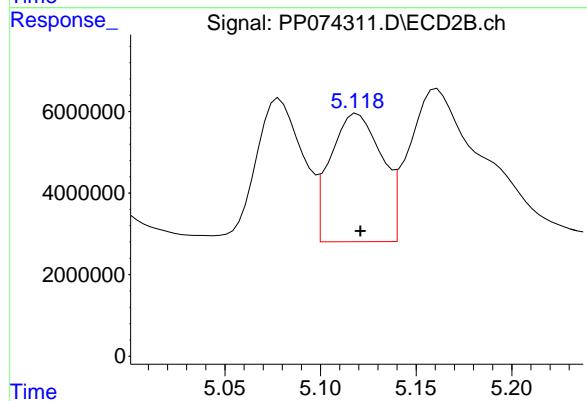

#22 AR-1248-2

R.T.: 5.119 min
 Delta R.T.: -0.002 min
 Response: 58694992
 Conc: 401.16 ng/ml

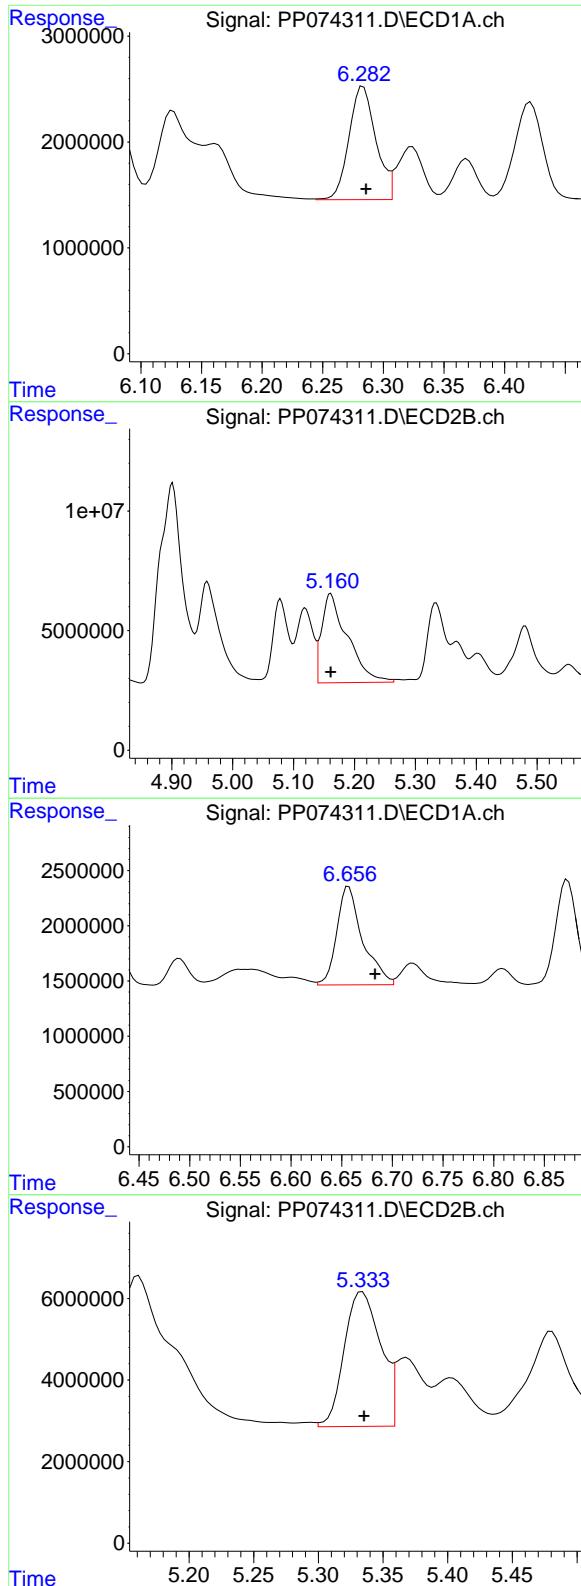

#23 AR-1248-3

R.T.: 6.283 min
 Delta R.T.: -0.002 min
 Response: 16474757
 Conc: 369.61 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVeway-TP-SOUTH-EASTMS

#23 AR-1248-3


R.T.: 5.161 min
 Delta R.T.: 0.000 min
 Response: 109744140
 Conc: 640.06 ng/ml

#24 AR-1248-4

R.T.: 6.657 min
 Delta R.T.: -0.026 min
 Response: 15791645
 Conc: 303.47 ng/ml

#24 AR-1248-4


R.T.: 5.334 min
 Delta R.T.: -0.001 min
 Response: 64653966
 Conc: 388.61 ng/ml



#25 AR-1248-5


R.T.: 6.720 min
 Delta R.T.: -0.002 min
 Response: 3440400
 Conc: 60.42 ng/ml

Instrument: ECD_P
 ClientSampleId : BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

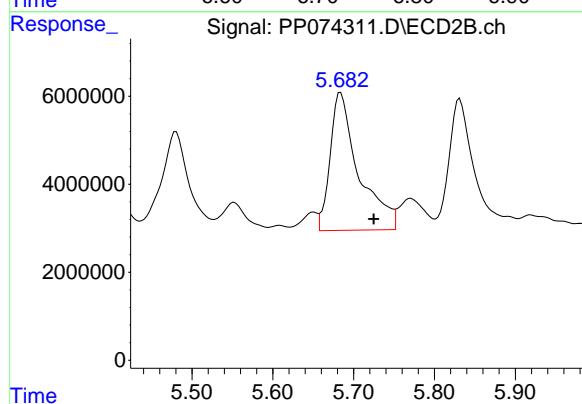


#25 AR-1248-5

R.T.: 5.684 min
 Delta R.T.: -0.041 min
 Response: 76642613
 Conc: 263.41 ng/ml

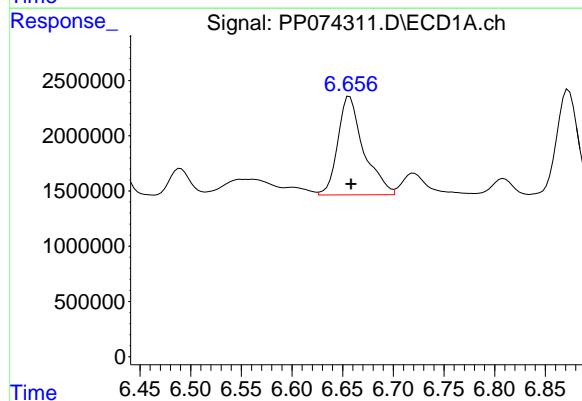


#26 AR-1254-1

R.T.: 6.657 min
 Delta R.T.: -0.001 min
 Response: 15791645
 Conc: 299.99 ng/ml

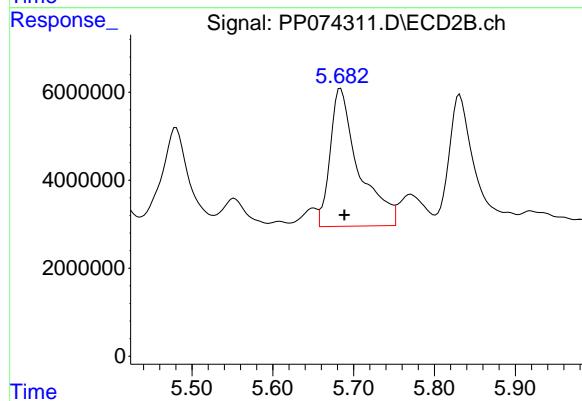

#26 AR-1254-1

R.T.: 5.684 min
 Delta R.T.: -0.004 min
 Response: 76642613
 Conc: 209.30 ng/ml

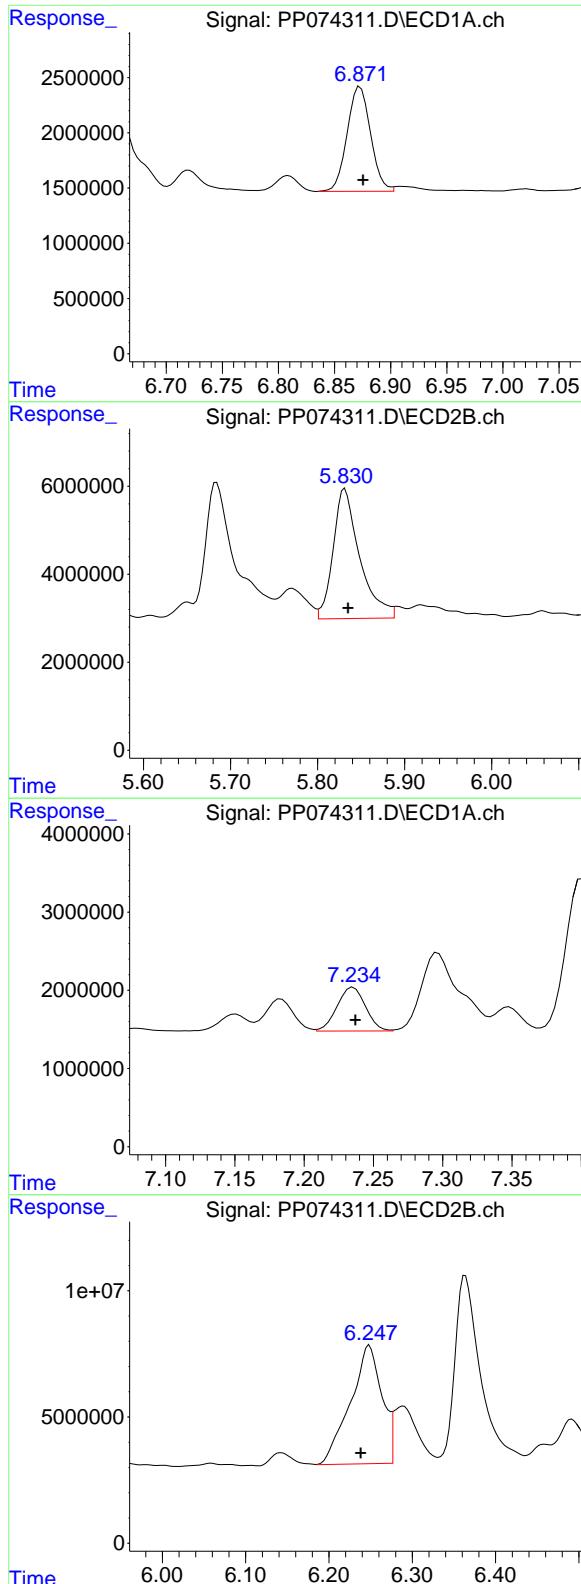

#27 AR-1254-2

R.T.: 6.873 min
 Delta R.T.: -0.003 min
 Response: 13769891
 Conc: 173.20 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#27 AR-1254-2


R.T.: 5.831 min
 Delta R.T.: -0.004 min
 Response: 62702065
 Conc: 225.37 ng/ml

#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: -0.001 min
 Response: 7976373
 Conc: 91.35 ng/ml

#28 AR-1254-3

R.T.: 6.249 min
 Delta R.T.: 0.010 min
 Response: 123342780
 Conc: 252.13 ng/ml

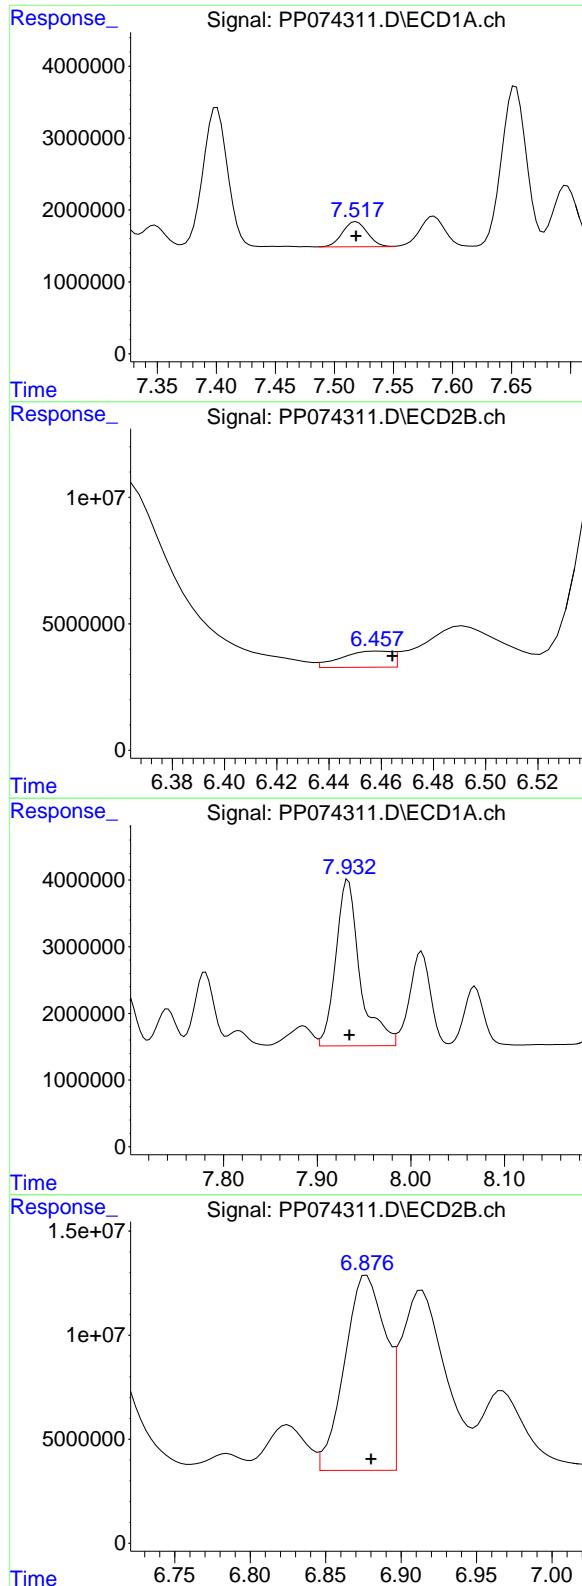

#29 AR-1254-4

R.T.: 7.518 min
 Delta R.T.: 0.000 min
 Response: 5089508
 Conc: 79.76 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#29 AR-1254-4


R.T.: 6.459 min
 Delta R.T.: -0.005 min
 Response: 8449703
 Conc: 22.99 ng/ml

#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: -0.001 min
 Response: 44898403
 Conc: 553.31 ng/ml

#30 AR-1254-5


R.T.: 6.877 min
 Delta R.T.: -0.003 min
 Response: 177029272
 Conc: 459.62 ng/ml

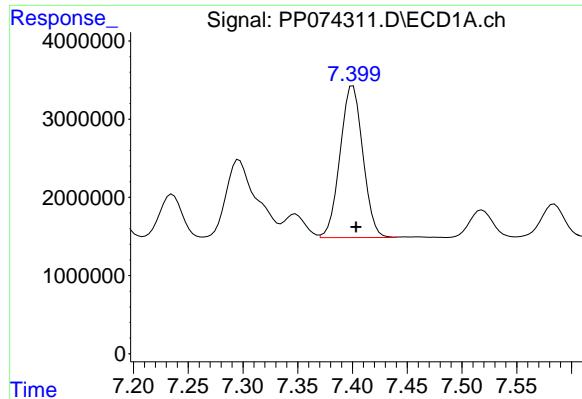

#31 AR-1260-1


R.T.: 7.400 min
 Delta R.T.: -0.003 min
 Response: 28140334
 Conc: 499.33 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

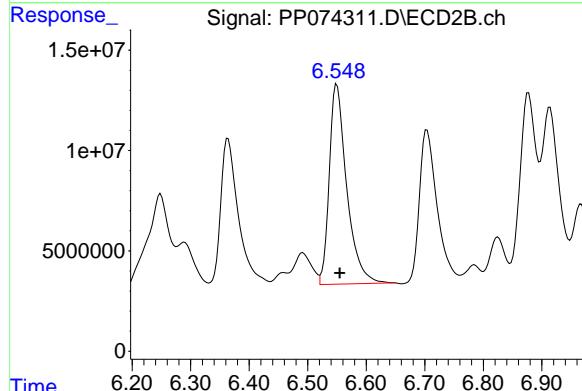


#31 AR-1260-1

R.T.: 6.550 min
 Delta R.T.: -0.005 min
 Response: 206989419
 Conc: 512.40 ng/ml




#32 AR-1260-2

R.T.: 7.653 min
 Delta R.T.: -0.002 min
 Response: 32575808
 Conc: 477.98 ng/ml

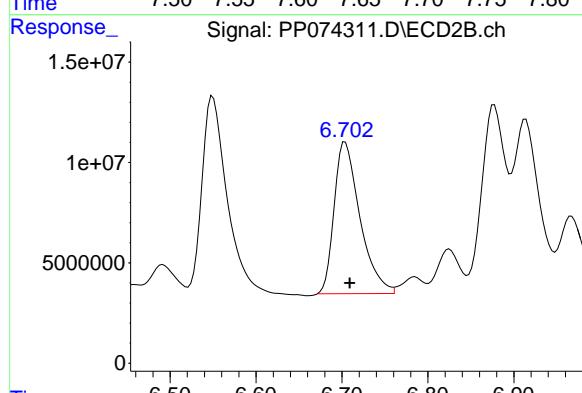

#32 AR-1260-2


R.T.: 6.704 min
 Delta R.T.: -0.005 min
 Response: 157569693
 Conc: 503.90 ng/ml

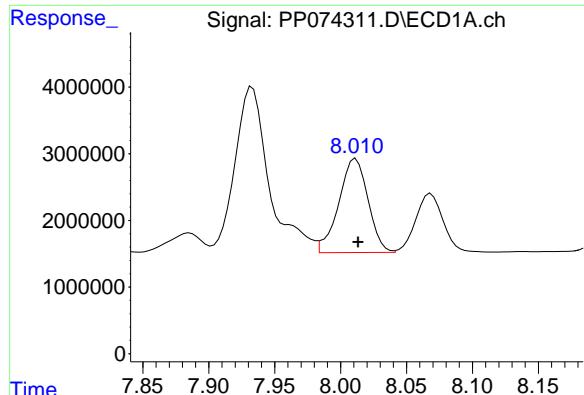

#33 AR-1260-3


R.T.: 8.012 min
 Delta R.T.: -0.002 min
 Response: 21771827
 Conc: 408.51 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

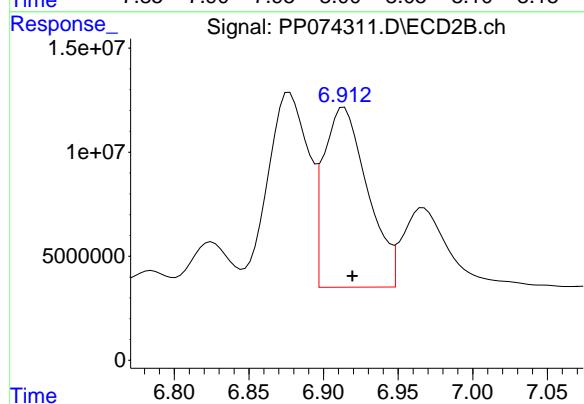


#33 AR-1260-3

R.T.: 6.914 min
 Delta R.T.: -0.006 min
 Response: 176516117
 Conc: 447.88 ng/ml

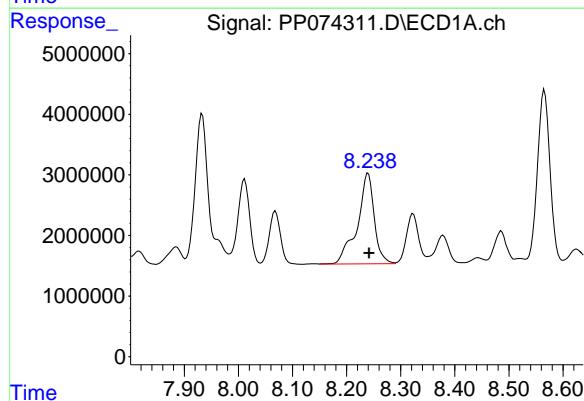


#34 AR-1260-4

R.T.: 8.240 min
 Delta R.T.: -0.002 min
 Response: 32485197
 Conc: 518.81 ng/ml

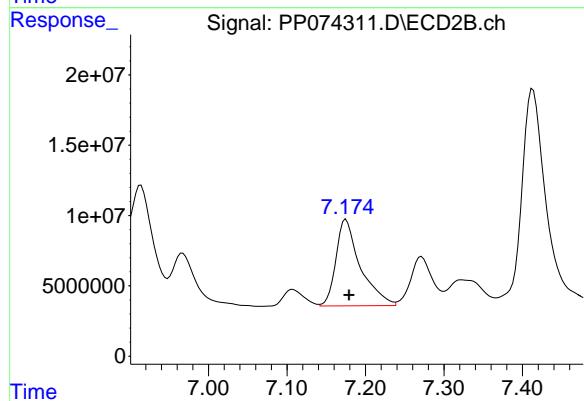

#34 AR-1260-4

R.T.: 7.175 min
 Delta R.T.: -0.004 min
 Response: 132650496
 Conc: 455.88 ng/ml

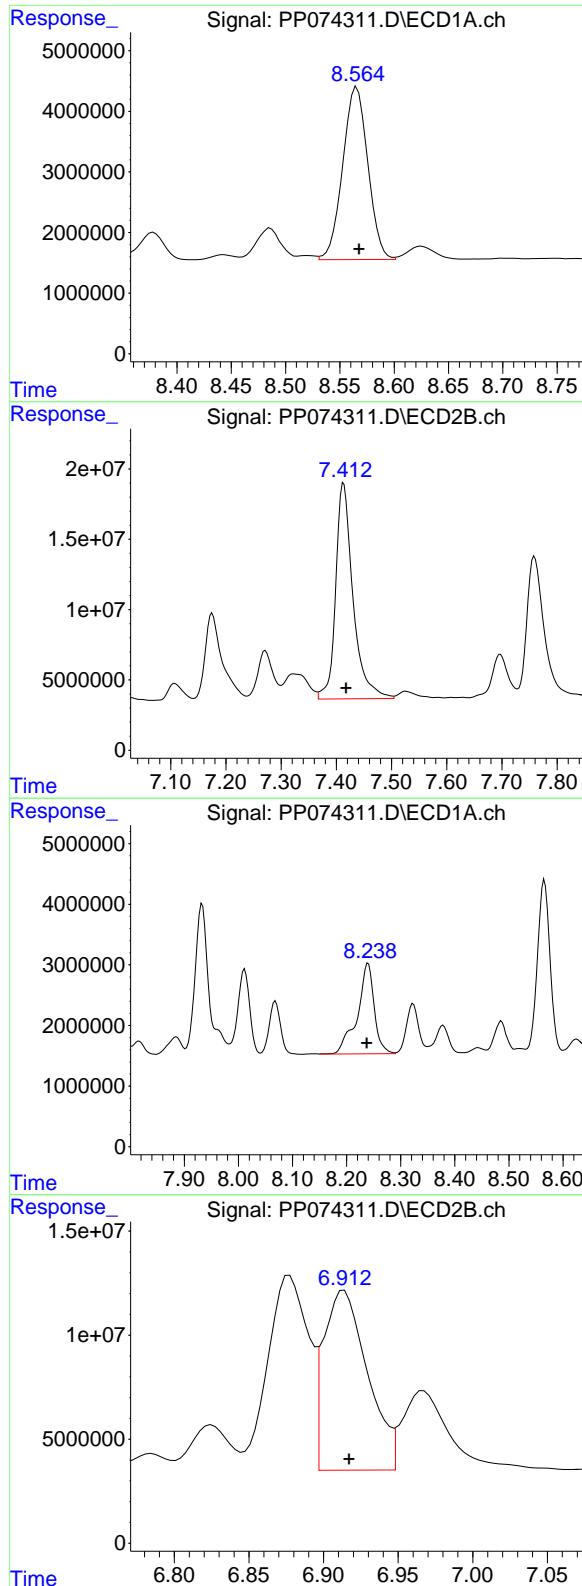

#35 AR-1260-5

R.T.: 8.566 min
 Delta R.T.: -0.002 min
 Response: 45863963
 Conc: 404.78 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#35 AR-1260-5


R.T.: 7.413 min
 Delta R.T.: -0.005 min
 Response: 335060197
 Conc: 442.38 ng/ml

#36 AR-1262-1

R.T.: 8.240 min
 Delta R.T.: 0.002 min
 Response: 32485197
 Conc: 428.62 ng/ml

#36 AR-1262-1

R.T.: 6.914 min
 Delta R.T.: -0.003 min
 Response: 176516117
 Conc: 313.45 ng/ml

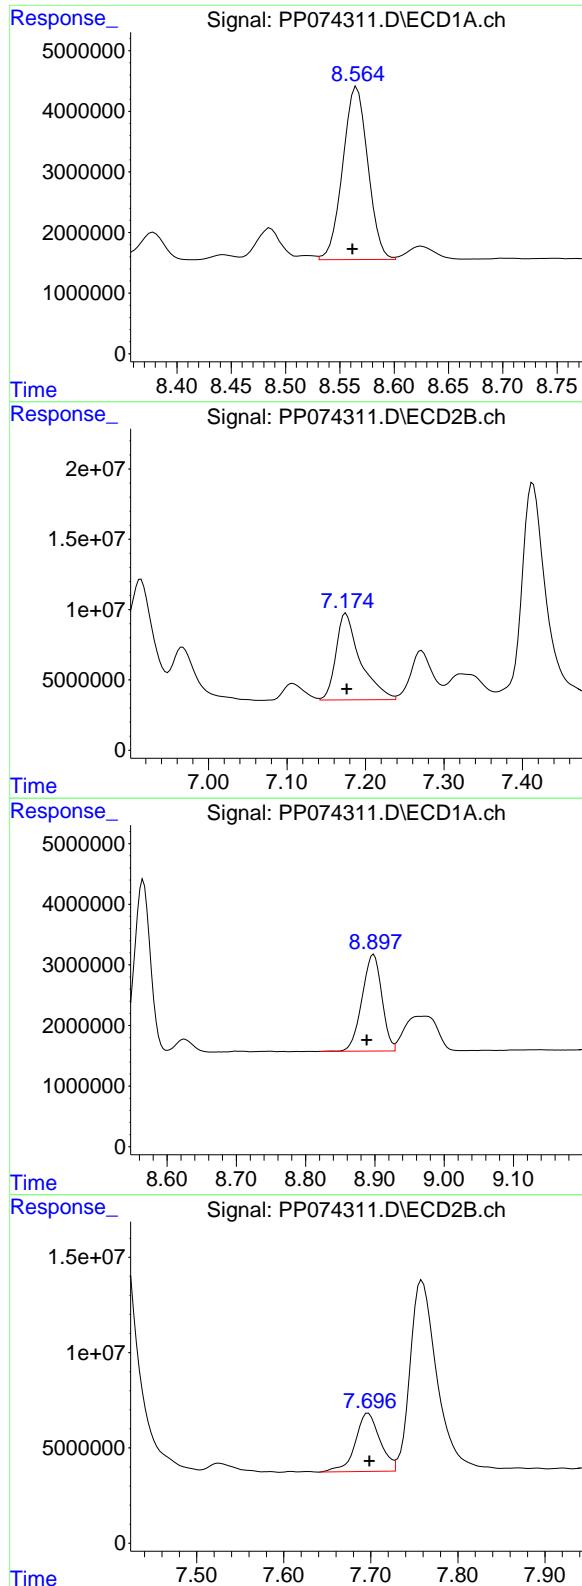

#37 AR-1262-2

R.T.: 8.566 min
 Delta R.T.: 0.004 min
 Response: 45863963
 Conc: 351.64 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#37 AR-1262-2


R.T.: 7.175 min
 Delta R.T.: 0.000 min
 Response: 132650496
 Conc: 330.78 ng/ml

#38 AR-1262-3

R.T.: 8.898 min
 Delta R.T.: 0.010 min
 Response: 31725032
 Conc: 337.25 ng/ml

#38 AR-1262-3

R.T.: 7.697 min
 Delta R.T.: -0.001 min
 Response: 60525419
 Conc: 168.37 ng/ml

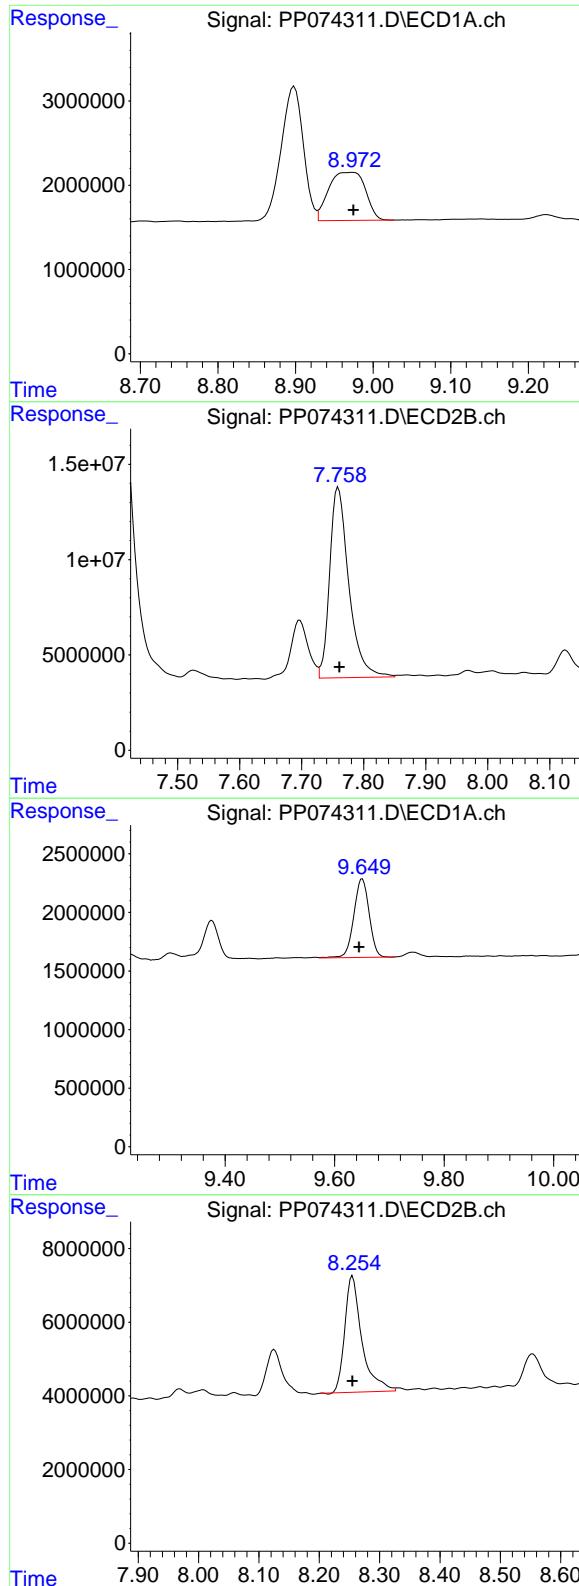

#39 AR-1262-4

R.T.: 8.974 min
 Delta R.T.: 0.000 min
 Response: 18734714
 Conc: 257.16 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#39 AR-1262-4


R.T.: 7.759 min
 Delta R.T.: -0.002 min
 Response: 215316810
 Conc: 322.85 ng/ml

#40 AR-1262-5

R.T.: 9.651 min
 Delta R.T.: 0.006 min
 Response: 13091860
 Conc: 257.09 ng/ml

#40 AR-1262-5


R.T.: 8.255 min
 Delta R.T.: 0.000 min
 Response: 62242150
 Conc: 219.73 ng/ml



#41 AR-1268-1


R.T.: 8.898 min
 Delta R.T.: 0.012 min
 Response: 31725032
 Conc: 203.85 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

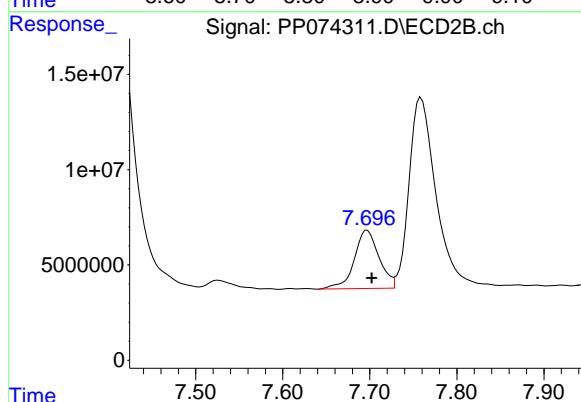


#41 AR-1268-1

R.T.: 7.697 min
 Delta R.T.: -0.005 min
 Response: 60525419
 Conc: 55.51 ng/ml

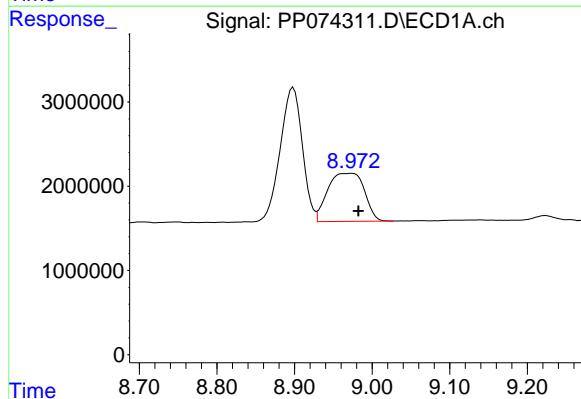


#42 AR-1268-2

R.T.: 8.974 min
 Delta R.T.: -0.009 min
 Response: 18734714
 Conc: 130.62 ng/ml

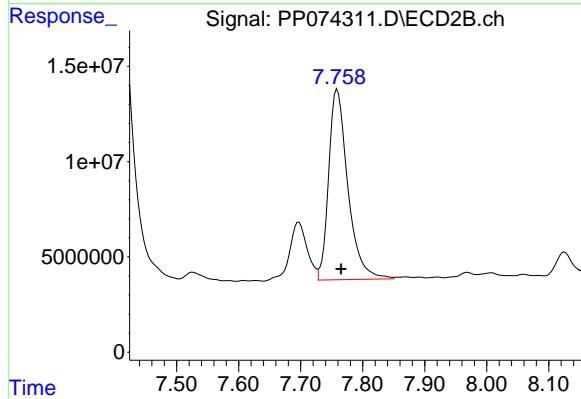

#42 AR-1268-2

R.T.: 7.759 min
 Delta R.T.: -0.006 min
 Response: 215316810
 Conc: 202.88 ng/ml

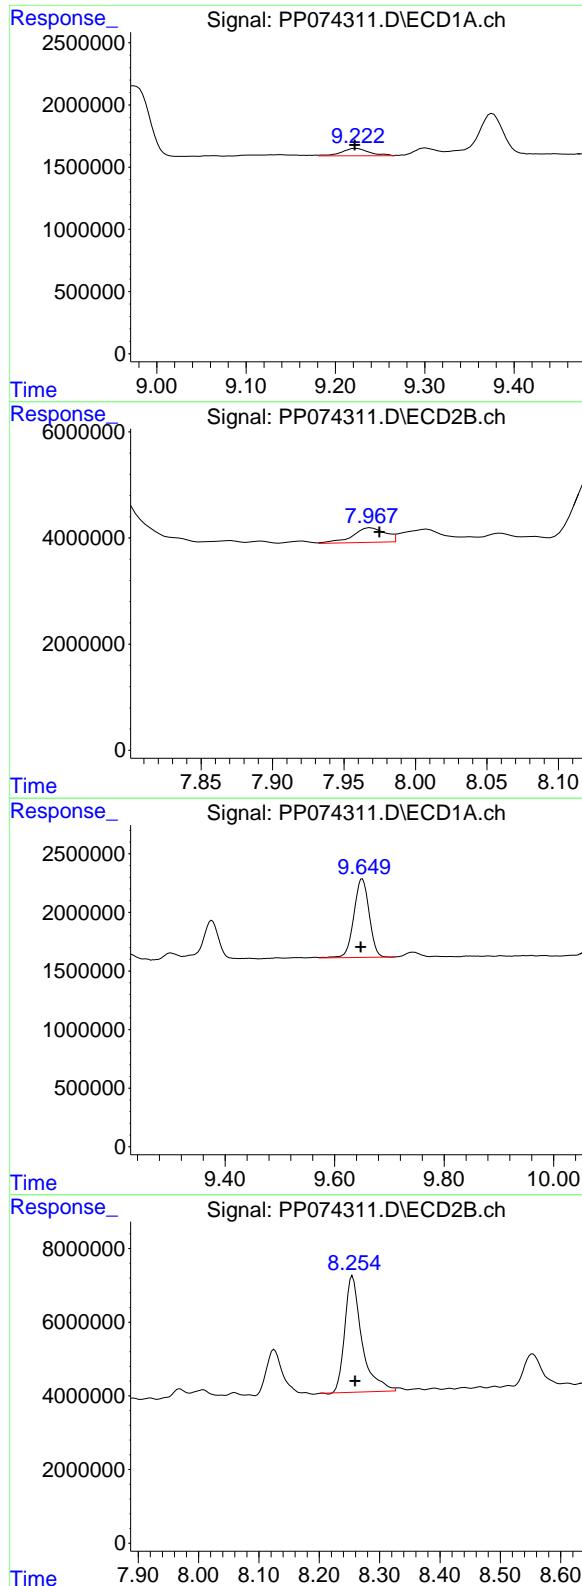

#43 AR-1268-3

R.T.: 9.223 min
 Delta R.T.: 0.002 min
 Response: 1275907
 Conc: 10.68 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#43 AR-1268-3


R.T.: 7.969 min
 Delta R.T.: -0.006 min
 Response: 4368524
 Conc: 5.25 ng/ml

#44 AR-1268-4

R.T.: 9.651 min
 Delta R.T.: 0.003 min
 Response: 13091860
 Conc: 222.60 ng/ml

#44 AR-1268-4

R.T.: 8.255 min
 Delta R.T.: -0.004 min
 Response: 62242150
 Conc: 202.05 ng/ml

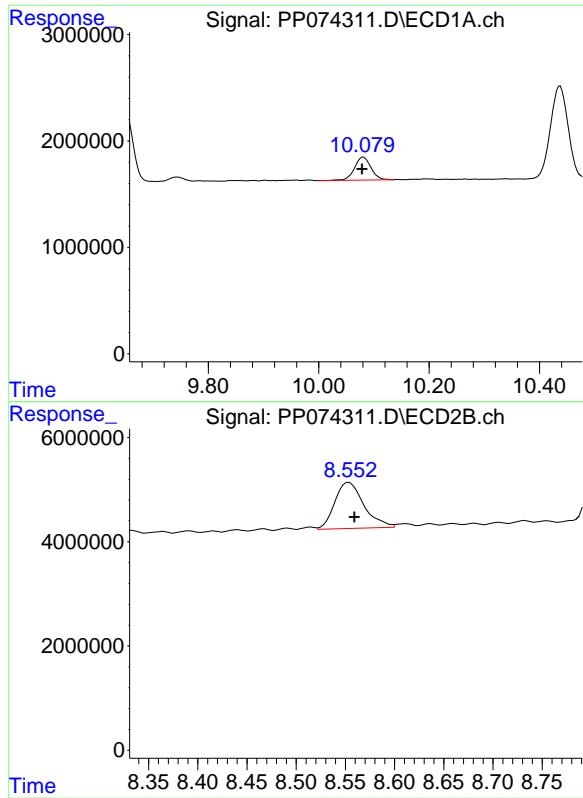

#45 AR-1268-5

R.T.: 10.081 min
 Delta R.T.: 0.002 min
 Response: 4477807
 Conc: 12.73 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMS

#45 AR-1268-5

R.T.: 8.554 min
 Delta R.T.: -0.005 min
 Response: 18194131
 Conc: 7.13 ng/ml

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:53
 Operator : YP\AJ
 Sample : Q2830-01MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ m Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|----------|--------|--------|
| 1) SA Tetrachlor... | 4.659 | 3.803 | 28248603 | 84782674 | 25.260 | 22.111 |
| 2) SA Decachlor... | 10.436 | 8.820 | 19391247 | 107.3E6 | 19.967 | 17.849 |

Target Compounds

| | | | | | | |
|------------------|-------|--------|----------|----------|----------|------------|
| 3) L1 AR-1016-1 | 5.811 | 4.904 | 22025300 | 229.5E6 | 533.859 | 575.363 |
| 4) L1 AR-1016-2 | 5.832 | 4.961 | 31957321 | 109.0E6 | 526.118 | 580.403 |
| 5) L1 AR-1016-3 | 5.895 | 5.081 | 21162376 | 59483478 | 533.588 | 560.796 |
| 6) L1 AR-1016-4 | 5.992 | 5.122 | 21722805 | 62077143 | 667.481 | 568.368 |
| 7) L1 AR-1016-5 | 6.284 | 5.337 | 16835913 | 66799585 | 518.538 | 571.116 |
| 8) L2 AR-1221-1 | 4.855 | 4.015 | 2799503 | 7506274 | 166.999 | 152.923 |
| 9) L2 AR-1221-2 | 4.944 | 4.096 | 3234077 | 11463855 | 256.651 | 319.422 |
| 10) L2 AR-1221-3 | 5.020 | 4.177 | 12623046 | 44378559 | 344.560 | 328.184 |
| 11) L3 AR-1232-1 | 5.020 | 4.177 | 12623046 | 44378559 | 434.718 | 437.821 |
| 12) L3 AR-1232-2 | 5.546 | 4.904 | 16536497 | 229.5E6 | 1099.303 | 1316.979 |
| 13) L3 AR-1232-3 | 5.832 | 5.081 | 31957321 | 59483478 | 1101.912 | 1298.295 |
| 14) L3 AR-1232-4 | 5.992 | 5.165 | 21722805 | 110.3E6 | 1404.296 | 1900.645 # |
| 15) L3 AR-1232-5 | 6.082 | 5.337 | 21659891 | 66799585 | 1848.743 | 1421.889 |
| 16) L4 AR-1242-1 | 5.811 | 4.904 | 22025300 | 229.5E6 | 591.032 | 664.961 |
| 17) L4 AR-1242-2 | 5.832 | 4.961 | 31957321 | 109.0E6 | 587.354 | 667.196 |
| 18) L4 AR-1242-3 | 5.895 | 5.081 | 21162376 | 59483478 | 592.189 | 644.818 |
| 19) L4 AR-1242-4 | 5.992 | 5.165 | 21722805 | 110.3E6 | 743.457 | 923.265 |
| 20) L4 AR-1242-5 | 6.721 | 5.687 | 3619251 | 78352361 | 101.784 | 523.886 # |
| 21) L5 AR-1248-1 | 5.811 | 4.904 | 22025300 | 229.5E6 | 786.210 | 1072.795 # |
| 22) L5 AR-1248-2 | 6.082 | 5.122 | 21659891 | 62077143 | 537.986 | 424.278 |
| 23) L5 AR-1248-3 | 6.284 | 5.165 | 16835913 | 110.3E6 | 377.711 | 643.052 # |
| 24) L5 AR-1248-4 | 6.659 | 5.337 | 16084366 | 66799585 | 309.094 | 401.504 # |
| 25) L5 AR-1248-5 | 6.721 | 5.687f | 3619251 | 78352361 | 63.559 | 269.284 # |
| 26) L6 AR-1254-1 | 6.659 | 5.687 | 16084366 | 78352361 | 305.548 | 213.971 # |
| 27) L6 AR-1254-2 | 6.874 | 5.833 | 14315175 | 64254931 | 180.055 | 230.953 # |
| 28) L6 AR-1254-3 | 7.236 | 6.251 | 7875880 | 128.3E6 | 90.200 | 262.171 # |
| 29) L6 AR-1254-4 | 7.519 | 6.461 | 5330889 | 8960018 | 83.544 | 24.377 # |
| 30) L6 AR-1254-5 | 7.933 | 6.879 | 45905141 | 181.8E6 | 565.719 | 472.046 |
| 31) L7 AR-1260-1 | 7.402 | 6.552 | 28910383 | 216.7E6 | 512.995 | 536.408 |
| 32) L7 AR-1260-2 | 7.654 | 6.707 | 33152517 | 164.0E6 | 486.447 | 524.348 |
| 33) L7 AR-1260-3 | 8.012 | 6.916 | 22216794 | 183.6E6 | 416.857 | 465.809 |
| 34) L7 AR-1260-4 | 8.240 | 7.176 | 33304829 | 137.0E6 | 531.899 | 470.828 |
| 35) L7 AR-1260-5 | 8.565 | 7.415 | 47018435 | 347.3E6 | 414.973 | 458.490 |
| 36) L8 AR-1262-1 | 8.240 | 6.916 | 33304829 | 183.6E6 | 439.437 | 325.999 # |
| 37) L8 AR-1262-2 | 8.565 | 7.176 | 47018435 | 137.0E6 | 360.488 | 341.629 |
| 38) L8 AR-1262-3 | 8.898 | 7.699 | 32396274 | 62513496 | 344.382 | 173.905 # |
| 39) L8 AR-1262-4 | 8.965 | 7.761 | 19192646 | 222.6E6 | 263.448 | 333.746 # |
| 40) L8 AR-1262-5 | 9.650 | 8.257 | 13192444 | 65413925 | 259.068 | 230.926 |
| 41) L9 AR-1268-1 | 8.898 | 7.699 | 32396274 | 62513496 | 208.158 | 57.338 # |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:53
 Operator : YP\AJ
 Sample : Q2830-01MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|--------|-------|----------|----------|---------|-----------|
| 42) L9 AR-1268-2 | 8.965 | 7.761 | 19192646 | 222.6E6 | 133.816 | 209.721 # |
| 43) L9 AR-1268-3 | 9.223 | 7.970 | 1061987 | 4622455 | 8.889 | 5.556 # |
| 44) L9 AR-1268-4 | 9.650 | 8.257 | 13192444 | 65413925 | 224.313 | 212.342 |
| 45) L9 AR-1268-5 | 10.081 | 8.555 | 4521037 | 19485839 | 12.855 | 7.641 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074312.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 13:53
 Operator : YP\AJ
 Sample : Q2830-01MSD
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BIN009-DRIVEWAY-TP-SOUTH-EASTMSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 12 14:50:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

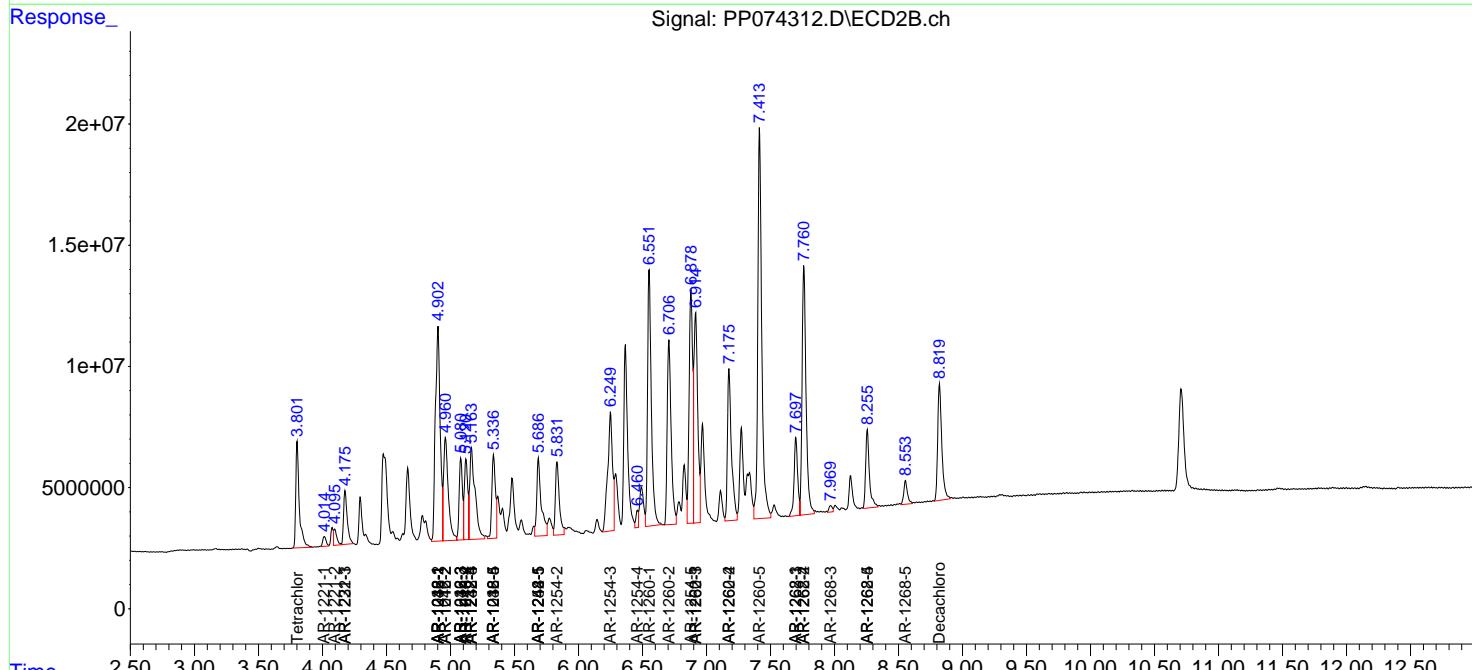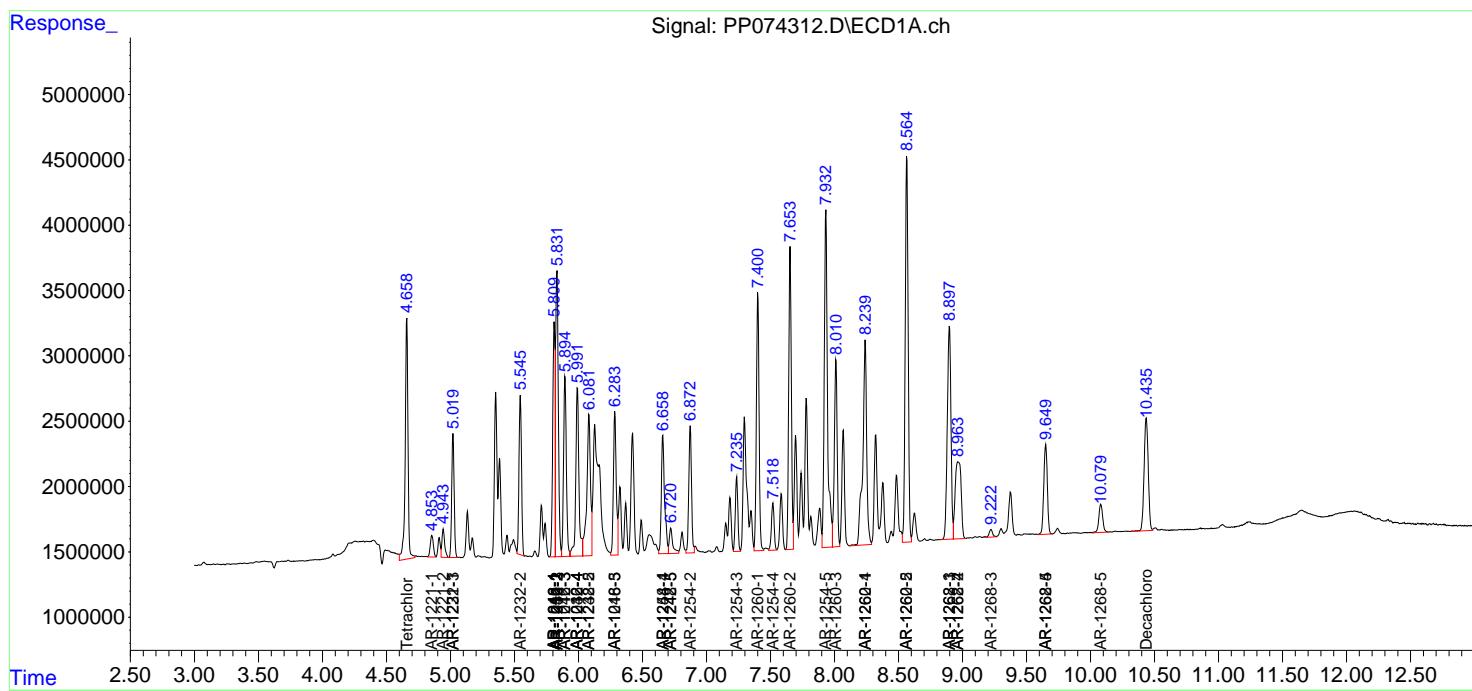

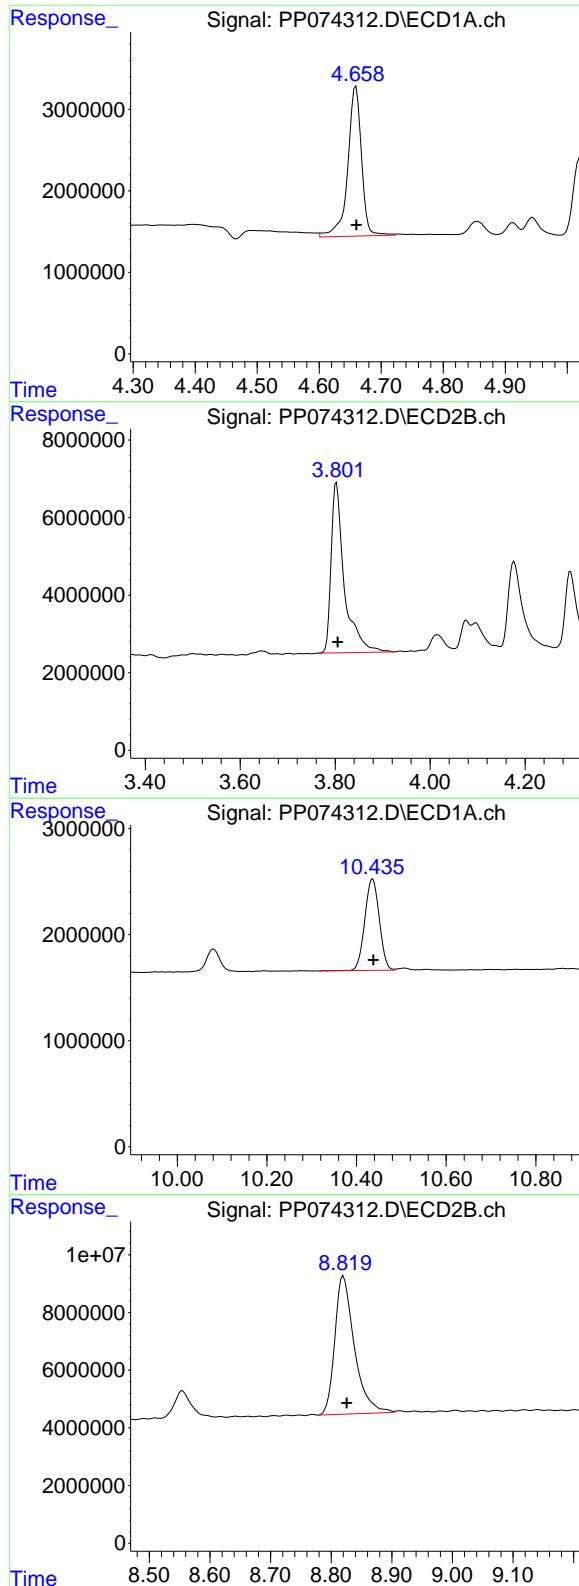

#1 Tetrachloro-m-xylene

R.T.: 4.659 min
 Delta R.T.: 0.000 min
 Response: 28248603
 Conc: 25.26 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

#1 Tetrachloro-m-xylene


R.T.: 3.803 min
 Delta R.T.: -0.003 min
 Response: 84782674
 Conc: 22.11 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.436 min
 Delta R.T.: -0.002 min
 Response: 19391247
 Conc: 19.97 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.820 min
 Delta R.T.: -0.006 min
 Response: 107334950
 Conc: 17.85 ng/ml

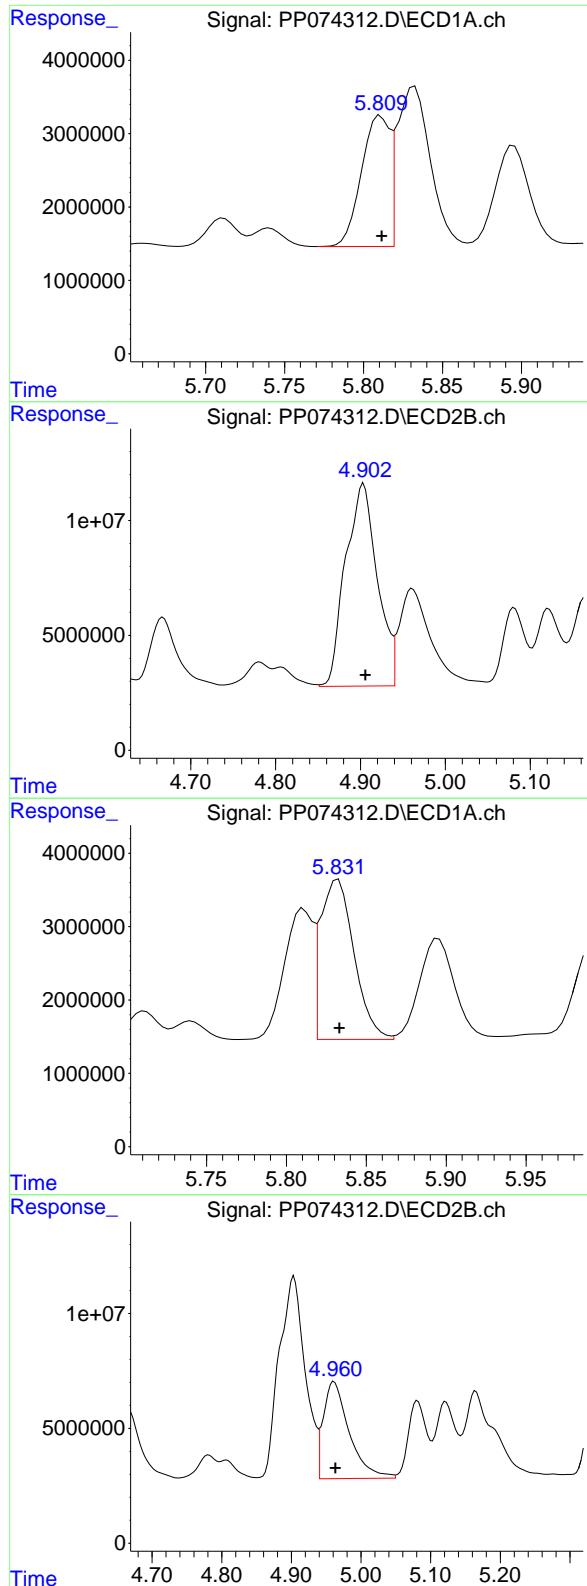

#3 AR-1016-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 22025300
 Conc: 533.86 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

#3 AR-1016-1


R.T.: 4.904 min
 Delta R.T.: -0.002 min
 Response: 229504954
 Conc: 575.36 ng/ml

#4 AR-1016-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 31957321
 Conc: 526.12 ng/ml

#4 AR-1016-2


R.T.: 4.961 min
 Delta R.T.: -0.002 min
 Response: 109004993
 Conc: 580.40 ng/ml



#5 AR-1016-3


R.T.: 5.895 min
 Delta R.T.: 0.000 min
 Response: 21162376
 Conc: 533.59 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

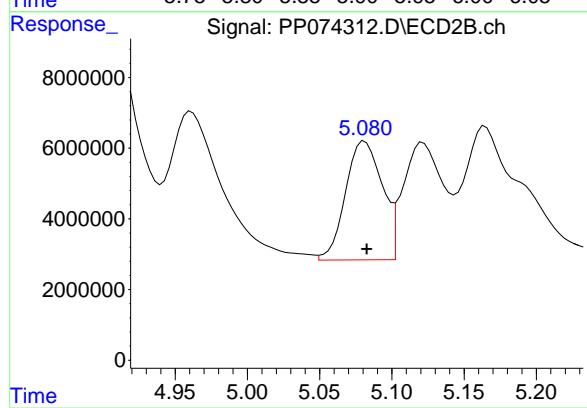


#5 AR-1016-3

R.T.: 5.081 min
 Delta R.T.: -0.001 min
 Response: 59483478
 Conc: 560.80 ng/ml

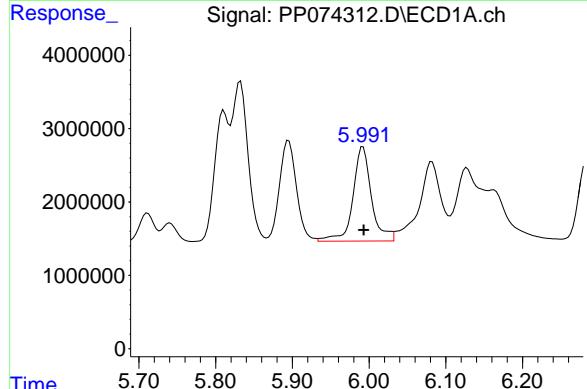


#6 AR-1016-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 21722805
 Conc: 667.48 ng/ml

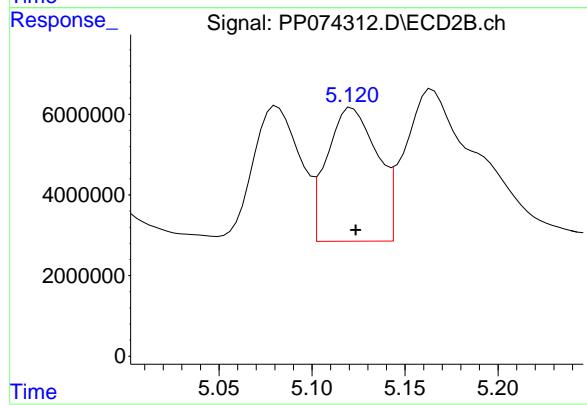

#6 AR-1016-4


R.T.: 5.122 min
 Delta R.T.: -0.002 min
 Response: 62077143
 Conc: 568.37 ng/ml

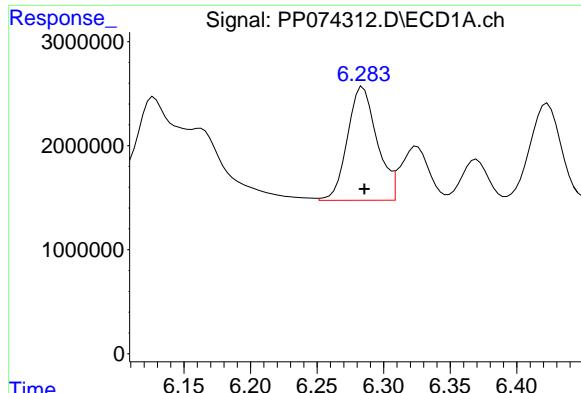

#7 AR-1016-5


R.T.: 6.284 min
 Delta R.T.: -0.001 min
 Response: 16835913
 Conc: 518.54 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

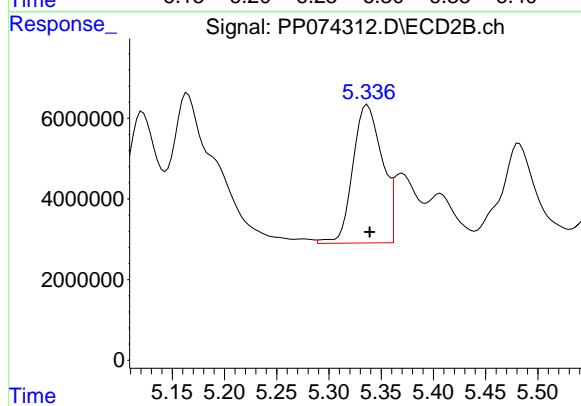


#7 AR-1016-5

R.T.: 5.337 min
 Delta R.T.: -0.002 min
 Response: 66799585
 Conc: 571.12 ng/ml




#8 AR-1221-1

R.T.: 4.855 min
 Delta R.T.: -0.003 min
 Response: 2799503
 Conc: 167.00 ng/ml

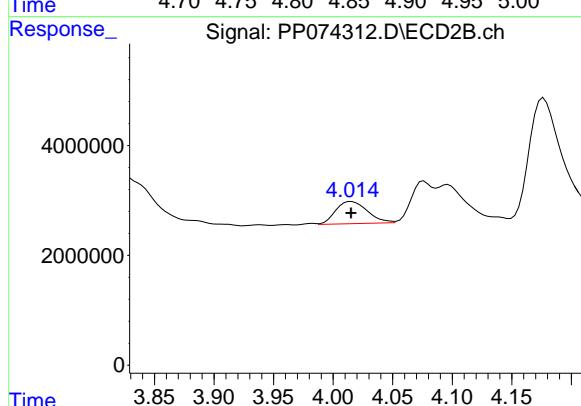

#8 AR-1221-1


R.T.: 4.015 min
 Delta R.T.: 0.000 min
 Response: 7506274
 Conc: 152.92 ng/ml

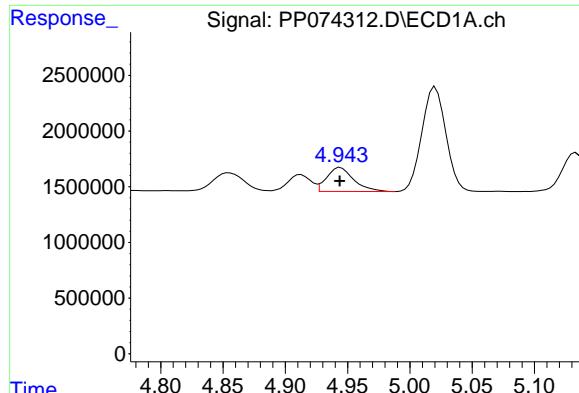

#9 AR-1221-2


R.T.: 4.944 min
Delta R.T.: 0.000 min
Response: 3234077
Conc: 256.65 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

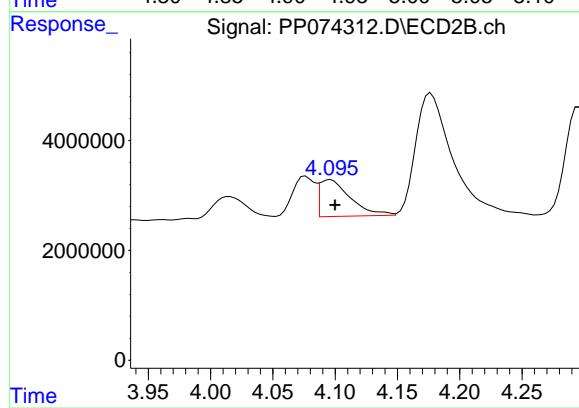


#9 AR-1221-2

R.T.: 4.096 min
Delta R.T.: -0.003 min
Response: 11463855
Conc: 319.42 ng/ml

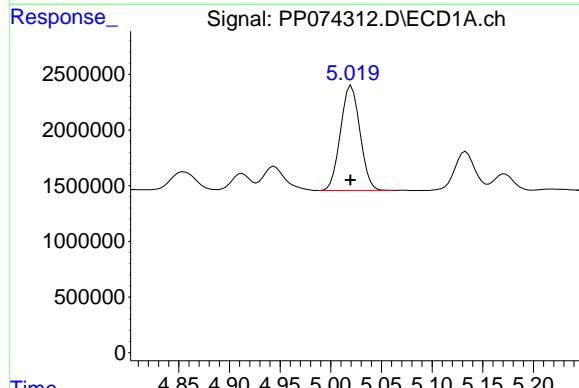


#10 AR-1221-3

R.T.: 5.020 min
Delta R.T.: 0.001 min
Response: 12623046
Conc: 344.56 ng/ml

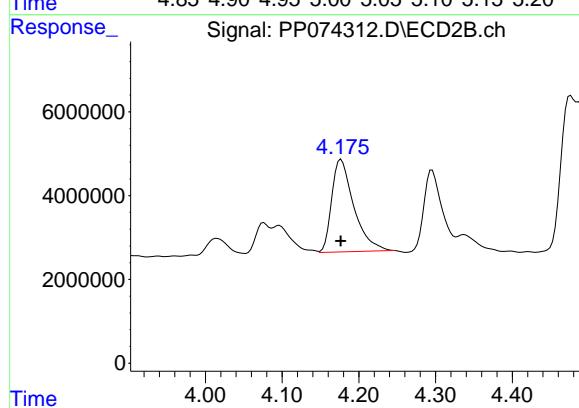

#10 AR-1221-3


R.T.: 4.177 min
Delta R.T.: 0.000 min
Response: 44378559
Conc: 328.18 ng/ml



#11 AR-1232-1


R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 12623046
 Conc: 434.72 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVeway-TP-SOUTH-EASTMSD

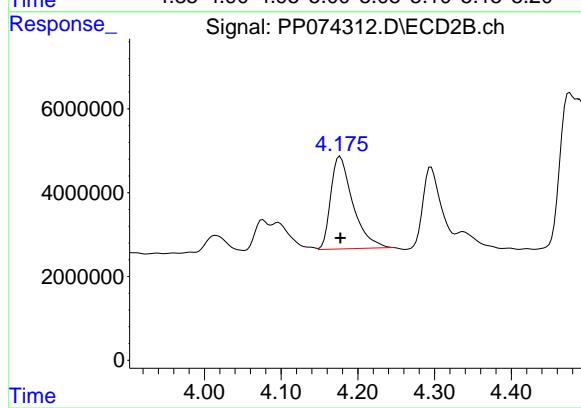


#11 AR-1232-1

R.T.: 4.177 min
 Delta R.T.: 0.000 min
 Response: 44378559
 Conc: 437.82 ng/ml




#12 AR-1232-2

R.T.: 5.546 min
 Delta R.T.: 0.000 min
 Response: 16536497
 Conc: 1099.30 ng/ml

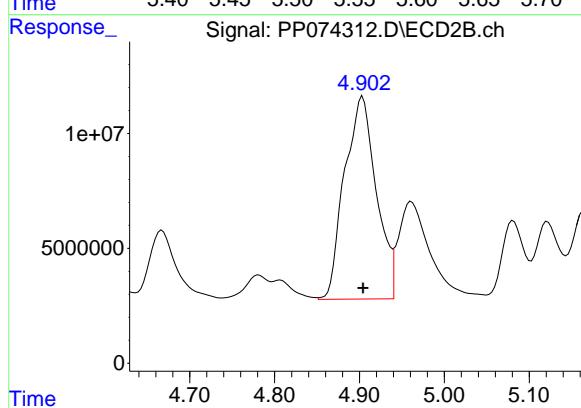


#12 AR-1232-2

R.T.: 4.904 min
 Delta R.T.: 0.000 min
 Response: 229504954
 Conc: 1316.98 ng/ml




#13 AR-1232-3

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 31957321
 Conc: 1101.91 ng/ml
Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

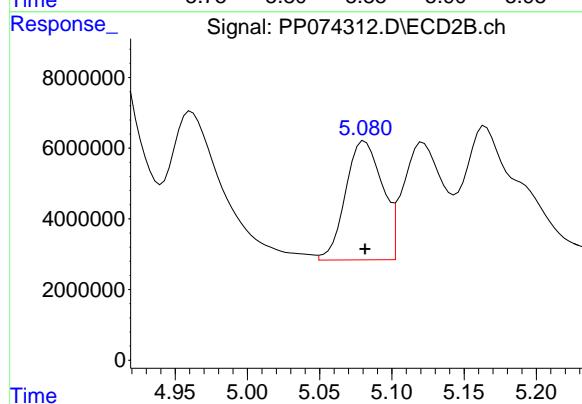


#13 AR-1232-3

R.T.: 5.081 min
 Delta R.T.: 0.000 min
 Response: 59483478
 Conc: 1298.29 ng/ml

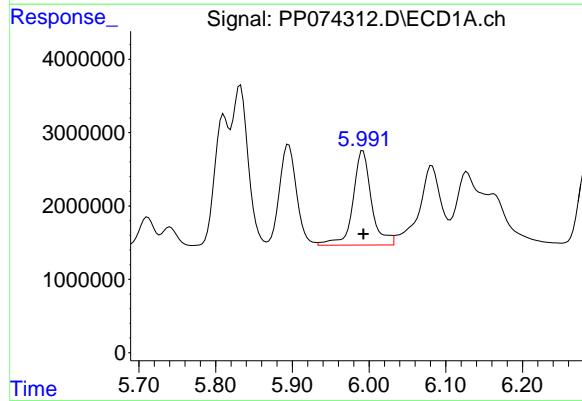


#14 AR-1232-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 21722805
 Conc: 1404.30 ng/ml

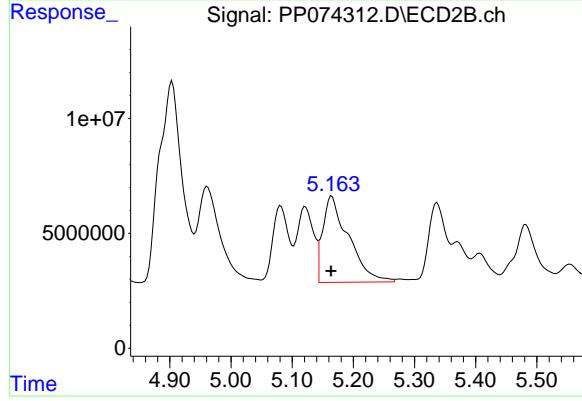

#14 AR-1232-4

R.T.: 5.165 min
 Delta R.T.: 0.001 min
 Response: 110257786
 Conc: 1900.65 ng/ml

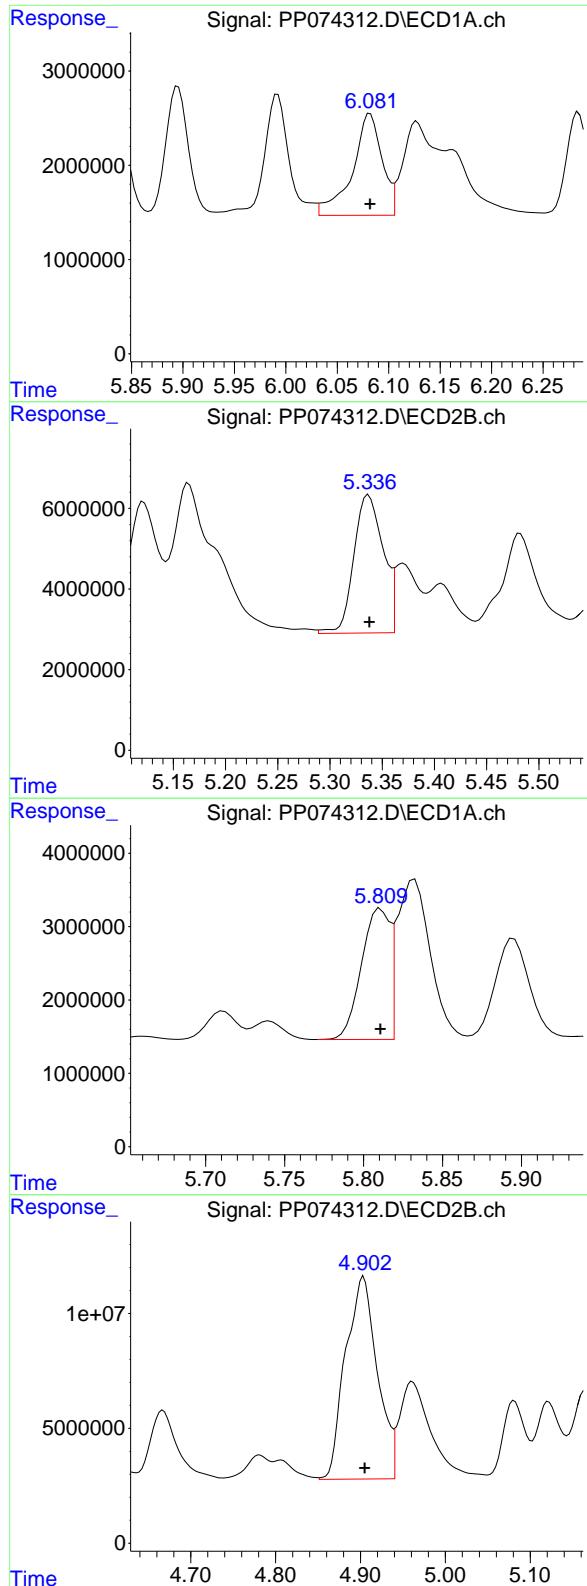

#15 AR-1232-5

R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 21659891
 Conc: 1848.74 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

#15 AR-1232-5


R.T.: 5.337 min
 Delta R.T.: 0.000 min
 Response: 66799585
 Conc: 1421.89 ng/ml

#16 AR-1242-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 22025300
 Conc: 591.03 ng/ml

#16 AR-1242-1


R.T.: 4.904 min
 Delta R.T.: -0.001 min
 Response: 229504954
 Conc: 664.96 ng/ml



#17 AR-1242-2


R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 31957321
 Conc: 587.35 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

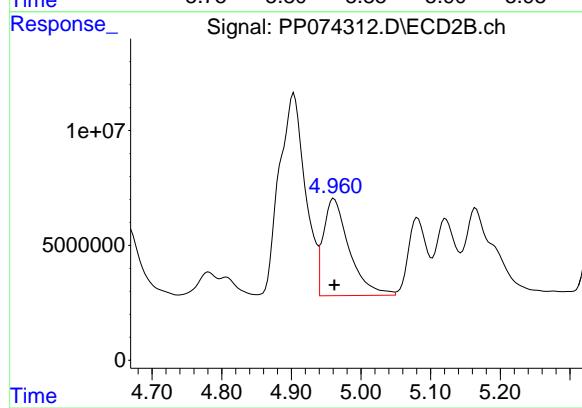


#17 AR-1242-2

R.T.: 4.961 min
 Delta R.T.: 0.000 min
 Response: 109004993
 Conc: 667.20 ng/ml

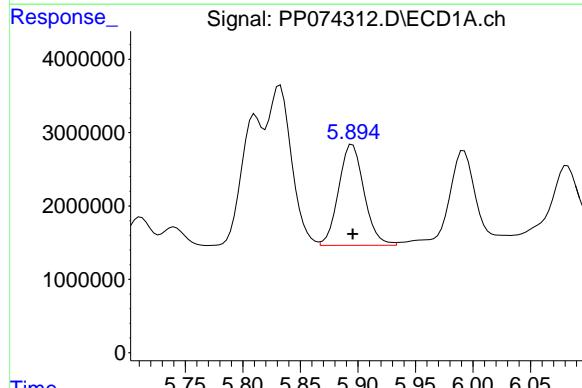


#18 AR-1242-3

R.T.: 5.895 min
 Delta R.T.: 0.000 min
 Response: 21162376
 Conc: 592.19 ng/ml

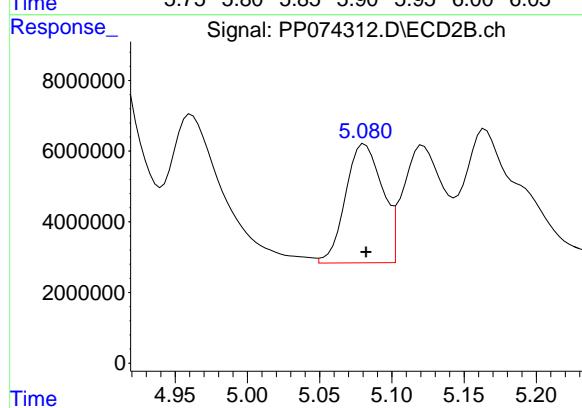

#18 AR-1242-3


R.T.: 5.081 min
 Delta R.T.: 0.000 min
 Response: 59483478
 Conc: 644.82 ng/ml

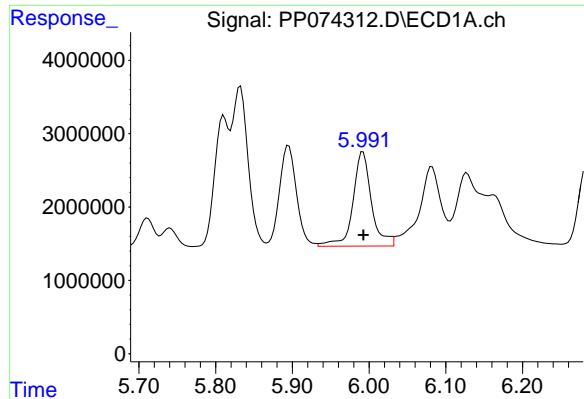

#19 AR-1242-4


R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 21722805
 Conc: 743.46 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

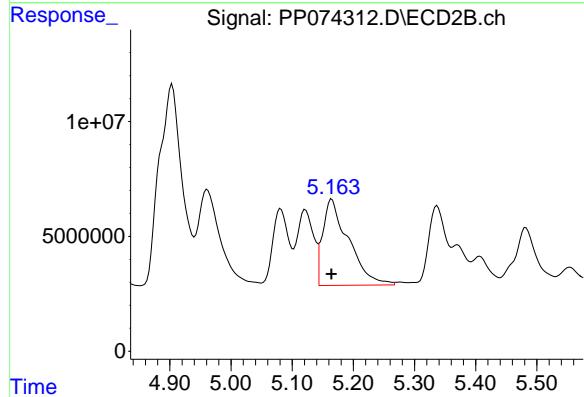


#19 AR-1242-4

R.T.: 5.165 min
 Delta R.T.: 0.000 min
 Response: 110257786
 Conc: 923.26 ng/ml

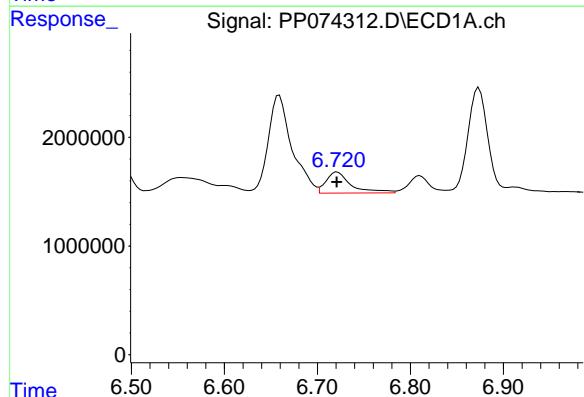


#20 AR-1242-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 3619251
 Conc: 101.78 ng/ml

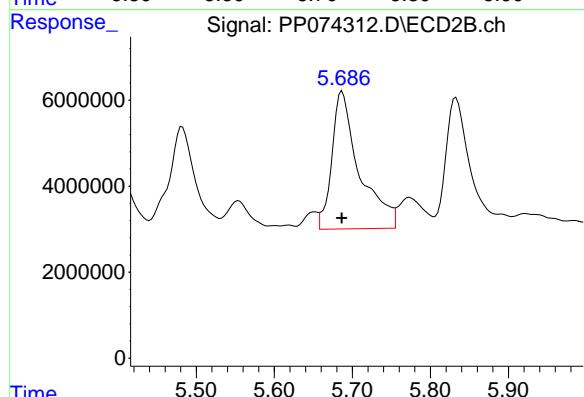

#20 AR-1242-5


R.T.: 5.687 min
 Delta R.T.: 0.000 min
 Response: 78352361
 Conc: 523.89 ng/ml



#21 AR-1248-1


R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 22025300
 Conc: 786.21 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

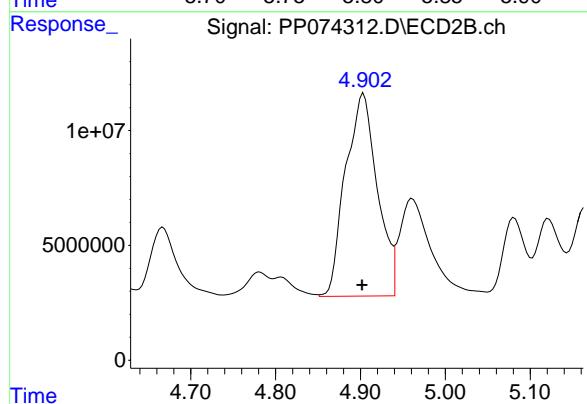


#21 AR-1248-1

R.T.: 4.904 min
 Delta R.T.: 0.002 min
 Response: 229504954
 Conc: 1072.80 ng/ml

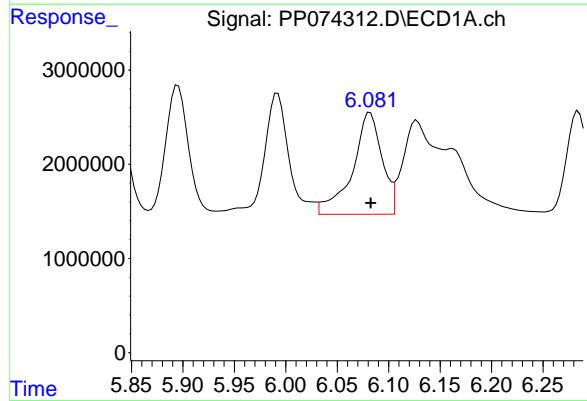


#22 AR-1248-2

R.T.: 6.082 min
 Delta R.T.: 0.000 min
 Response: 21659891
 Conc: 537.99 ng/ml

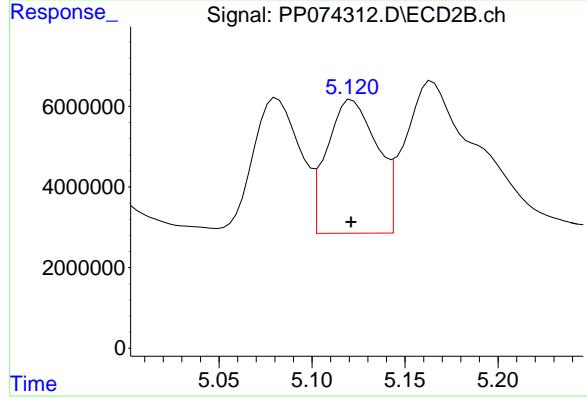

#22 AR-1248-2


R.T.: 5.122 min
 Delta R.T.: 0.000 min
 Response: 62077143
 Conc: 424.28 ng/ml



#23 AR-1248-3


R.T.: 6.284 min
 Delta R.T.: -0.001 min
 Response: 16835913
 Conc: 377.71 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVeway-TP-SOUTH-EASTMSD

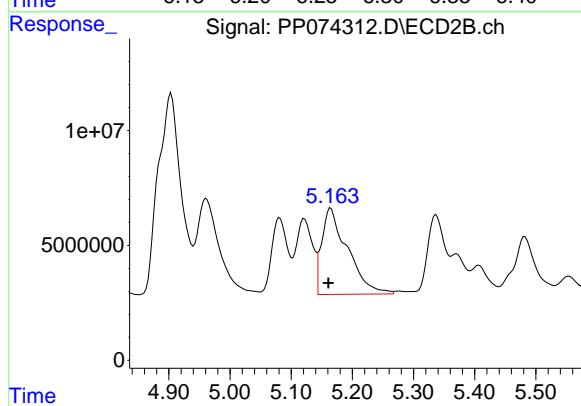


#23 AR-1248-3

R.T.: 5.165 min
 Delta R.T.: 0.004 min
 Response: 110257786
 Conc: 643.05 ng/ml




#24 AR-1248-4

R.T.: 6.659 min
 Delta R.T.: -0.024 min
 Response: 16084366
 Conc: 309.09 ng/ml

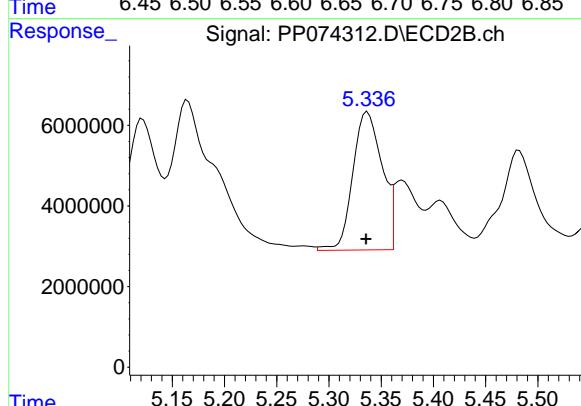

#24 AR-1248-4

R.T.: 5.337 min
 Delta R.T.: 0.002 min
 Response: 66799585
 Conc: 401.50 ng/ml

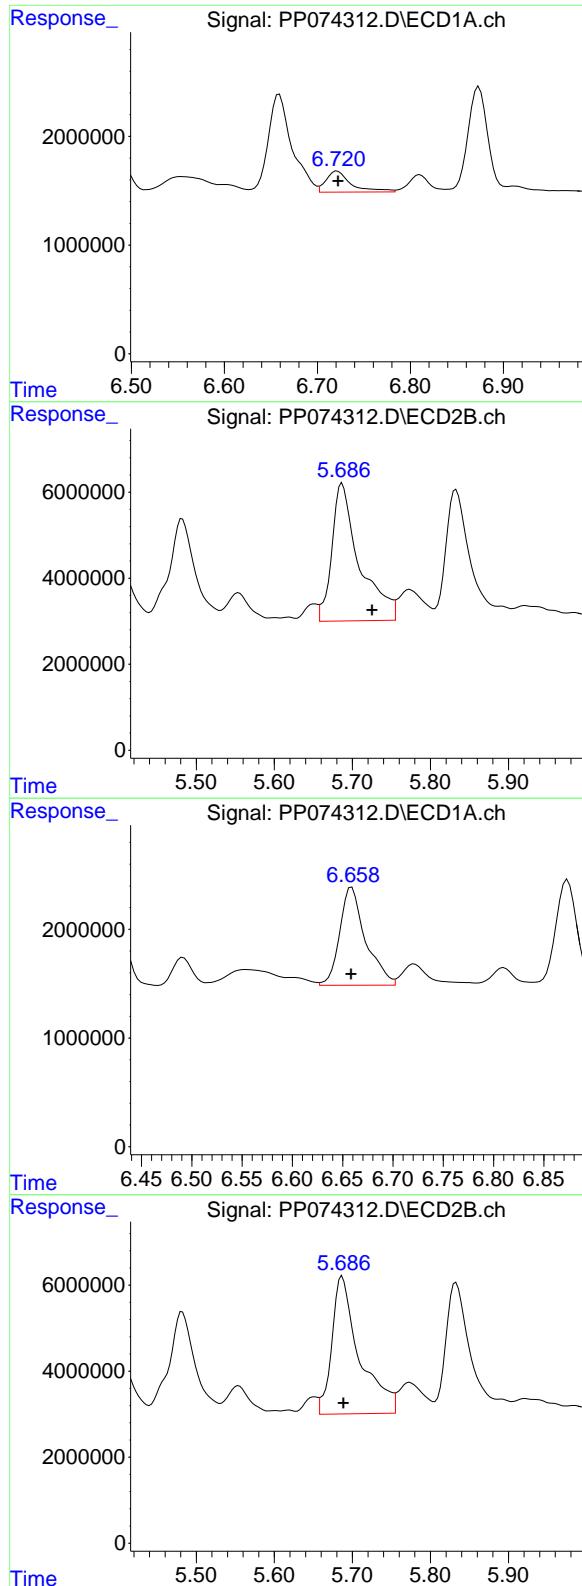

#25 AR-1248-5

R.T.: 6.721 min
 Delta R.T.: 0.000 min
 Response: 3619251
 Conc: 63.56 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVeway-TP-SOUTH-EASTMSD

#25 AR-1248-5


R.T.: 5.687 min
 Delta R.T.: -0.038 min
 Response: 78352361
 Conc: 269.28 ng/ml

#26 AR-1254-1

R.T.: 6.659 min
 Delta R.T.: 0.000 min
 Response: 16084366
 Conc: 305.55 ng/ml

#26 AR-1254-1


R.T.: 5.687 min
 Delta R.T.: -0.002 min
 Response: 78352361
 Conc: 213.97 ng/ml

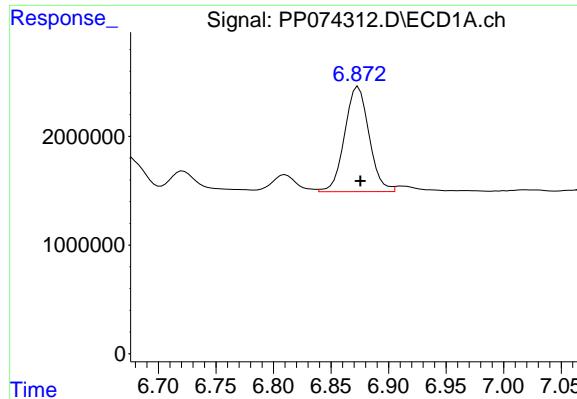

#27 AR-1254-2


R.T.: 6.874 min
 Delta R.T.: -0.002 min
 Response: 14315175
 Conc: 180.05 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

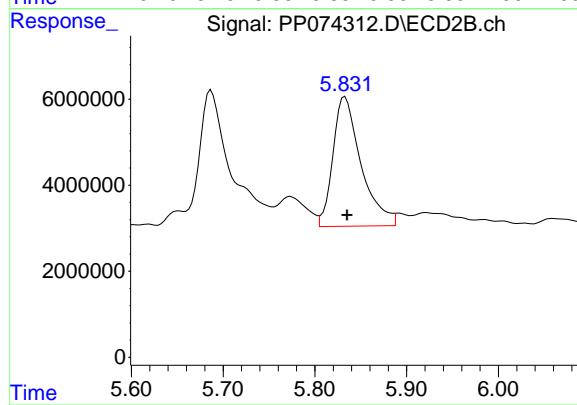


#27 AR-1254-2

R.T.: 5.833 min
 Delta R.T.: -0.002 min
 Response: 64254931
 Conc: 230.95 ng/ml

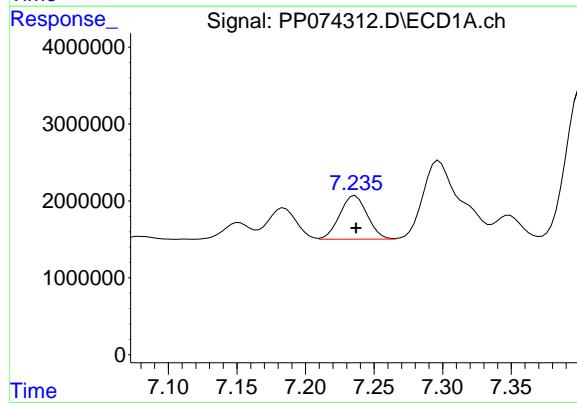


#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: 0.000 min
 Response: 7875880
 Conc: 90.20 ng/ml

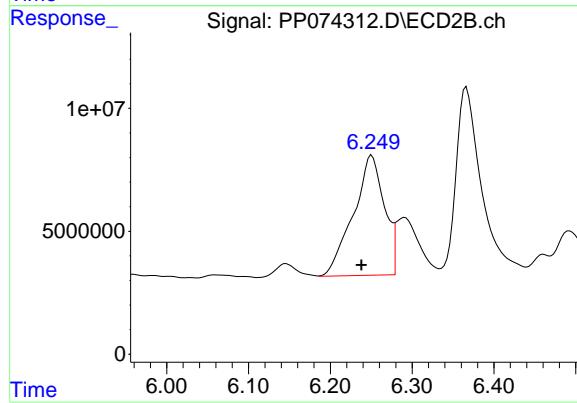

#28 AR-1254-3

R.T.: 6.251 min
 Delta R.T.: 0.013 min
 Response: 128256966
 Conc: 262.17 ng/ml

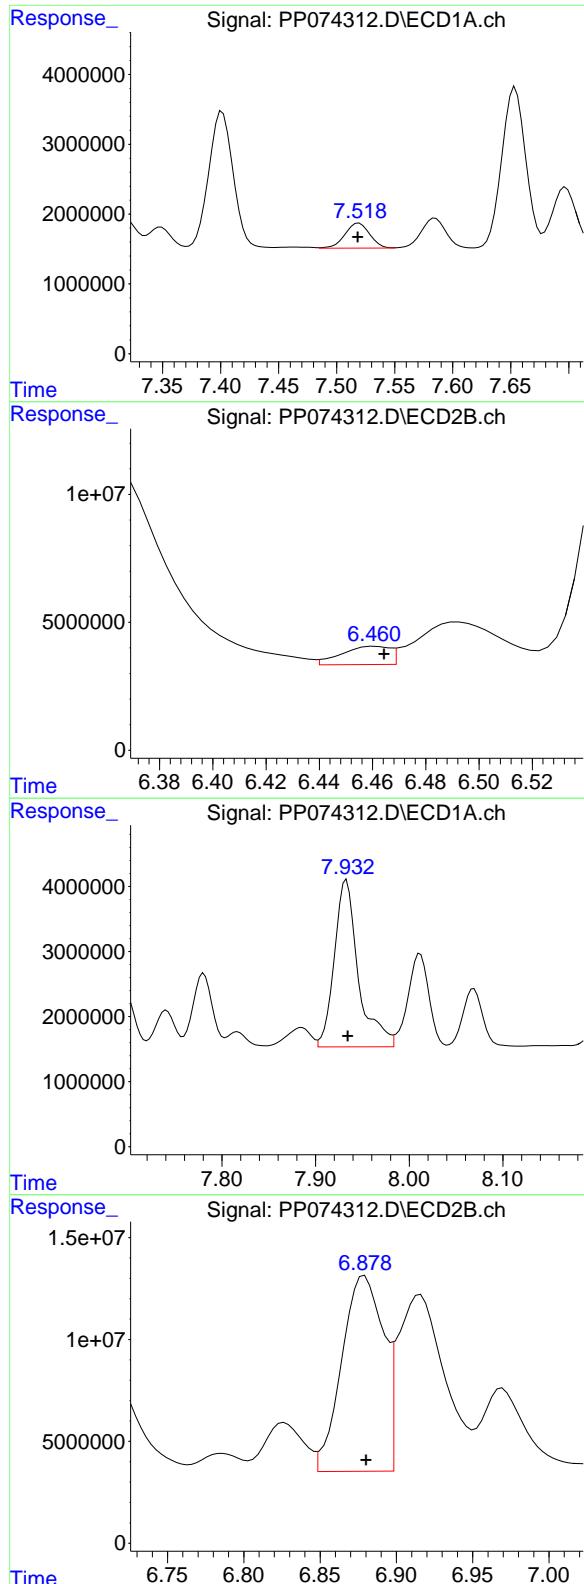

#29 AR-1254-4

R.T.: 7.519 min
 Delta R.T.: 0.000 min
 Response: 5330889
 Conc: 83.54 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

#29 AR-1254-4


R.T.: 6.461 min
 Delta R.T.: -0.003 min
 Response: 8960018
 Conc: 24.38 ng/ml

#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: -0.001 min
 Response: 45905141
 Conc: 565.72 ng/ml

#30 AR-1254-5


R.T.: 6.879 min
 Delta R.T.: 0.000 min
 Response: 181816593
 Conc: 472.05 ng/ml

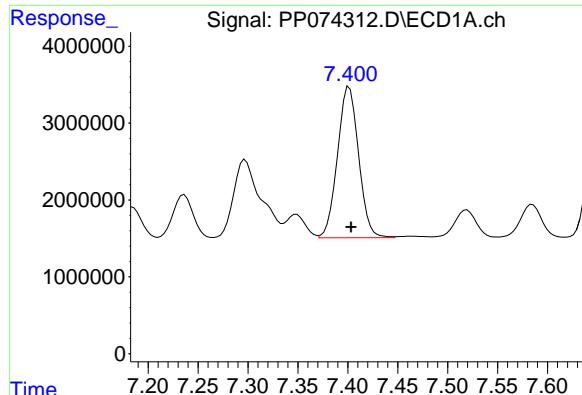

#31 AR-1260-1


R.T.: 7.402 min
 Delta R.T.: -0.002 min
 Response: 28910383
 Conc: 513.00 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

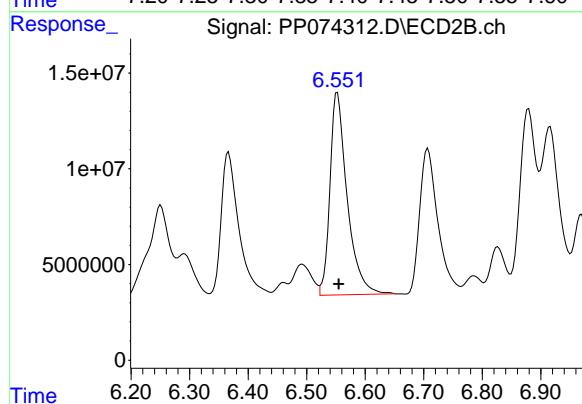


#31 AR-1260-1

R.T.: 6.552 min
 Delta R.T.: -0.002 min
 Response: 216685736
 Conc: 536.41 ng/ml

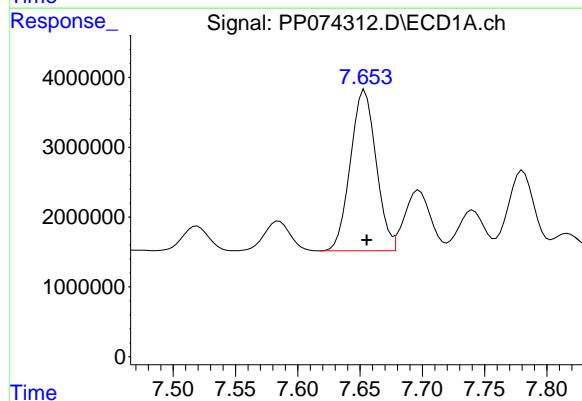


#32 AR-1260-2

R.T.: 7.654 min
 Delta R.T.: -0.002 min
 Response: 33152517
 Conc: 486.45 ng/ml

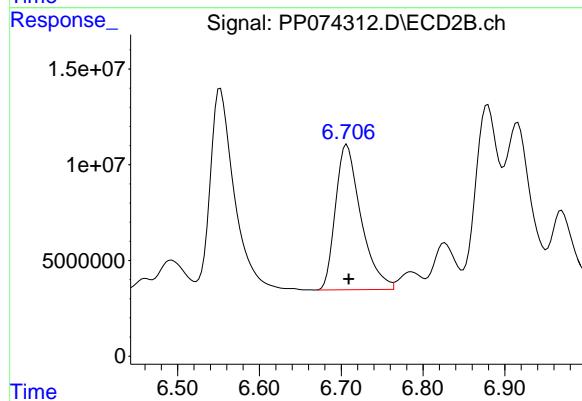

#32 AR-1260-2


R.T.: 6.707 min
 Delta R.T.: -0.002 min
 Response: 163962965
 Conc: 524.35 ng/ml

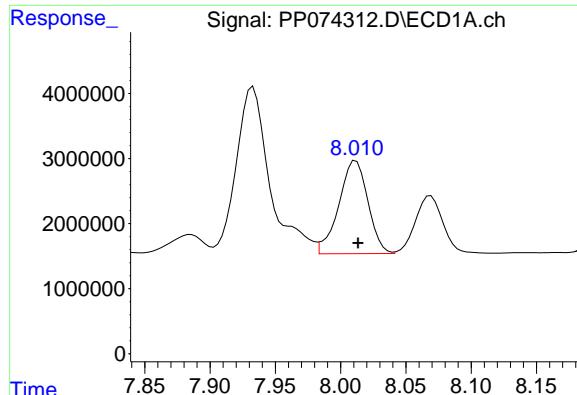

#33 AR-1260-3


R.T.: 8.012 min
 Delta R.T.: -0.002 min
 Response: 22216794
 Conc: 416.86 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

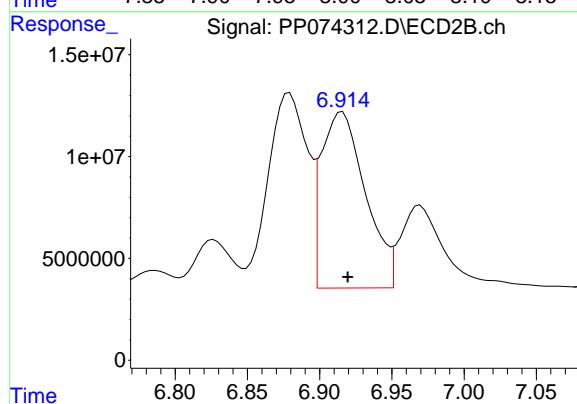


#33 AR-1260-3

R.T.: 6.916 min
 Delta R.T.: -0.004 min
 Response: 183583696
 Conc: 465.81 ng/ml

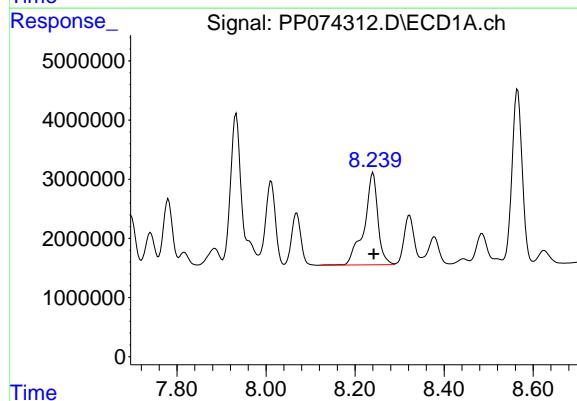


#34 AR-1260-4

R.T.: 8.240 min
 Delta R.T.: -0.001 min
 Response: 33304829
 Conc: 531.90 ng/ml

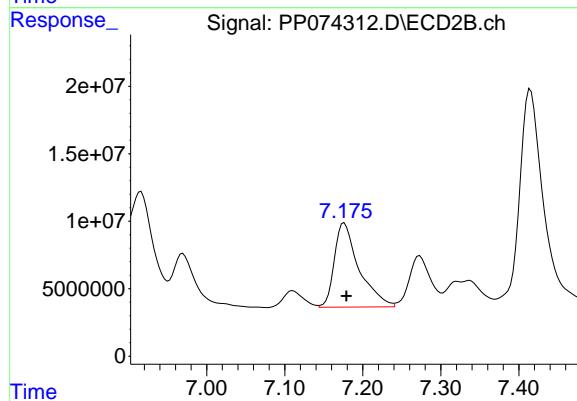

#34 AR-1260-4

R.T.: 7.176 min
 Delta R.T.: -0.003 min
 Response: 137001180
 Conc: 470.83 ng/ml

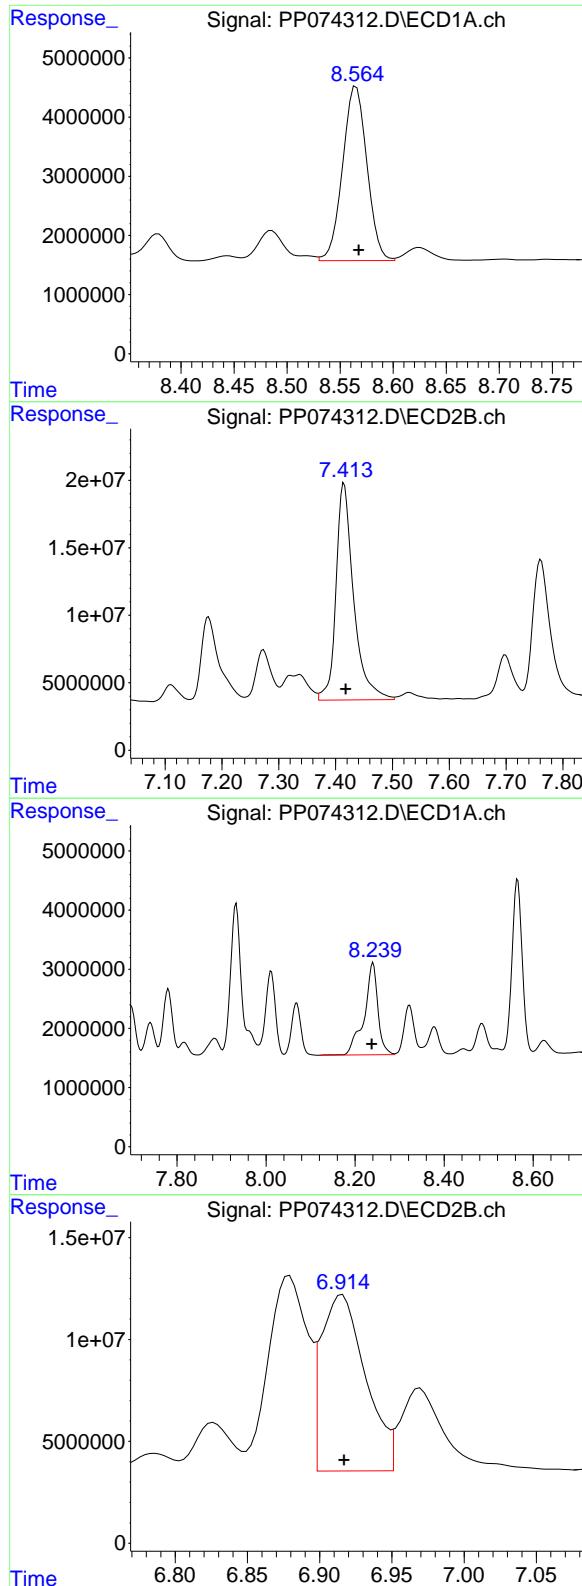

#35 AR-1260-5

R.T.: 8.565 min
 Delta R.T.: -0.002 min
 Response: 47018435
 Conc: 414.97 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

#35 AR-1260-5


R.T.: 7.415 min
 Delta R.T.: -0.003 min
 Response: 347264975
 Conc: 458.49 ng/ml

#36 AR-1262-1

R.T.: 8.240 min
 Delta R.T.: 0.003 min
 Response: 33304829
 Conc: 439.44 ng/ml

#36 AR-1262-1


R.T.: 6.916 min
 Delta R.T.: -0.001 min
 Response: 183583696
 Conc: 326.00 ng/ml



#37 AR-1262-2


R.T.: 8.565 min
 Delta R.T.: 0.003 min
 Response: 47018435
 Conc: 360.49 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

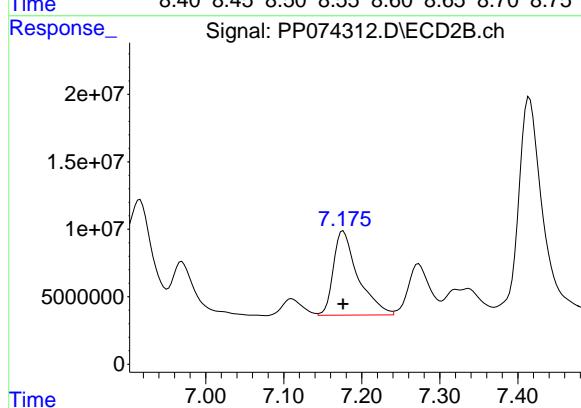


#37 AR-1262-2

R.T.: 7.176 min
 Delta R.T.: 0.000 min
 Response: 137001180
 Conc: 341.63 ng/ml




#38 AR-1262-3

R.T.: 8.898 min
 Delta R.T.: 0.010 min
 Response: 32396274
 Conc: 344.38 ng/ml

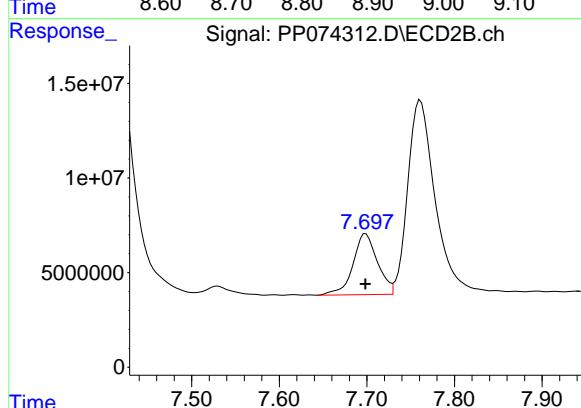

#38 AR-1262-3


R.T.: 7.699 min
 Delta R.T.: 0.000 min
 Response: 62513496
 Conc: 173.90 ng/ml

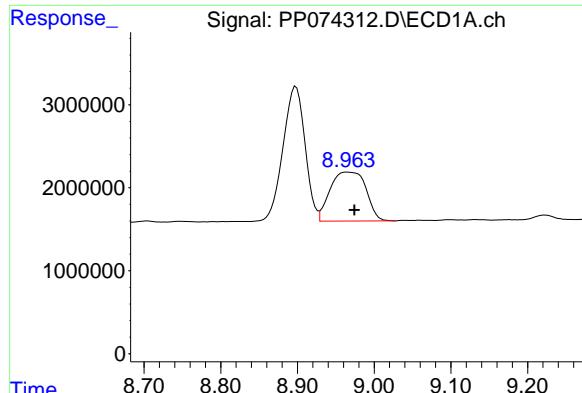

#39 AR-1262-4


R.T.: 8.965 min
 Delta R.T.: -0.009 min
 Response: 19192646
 Conc: 263.45 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

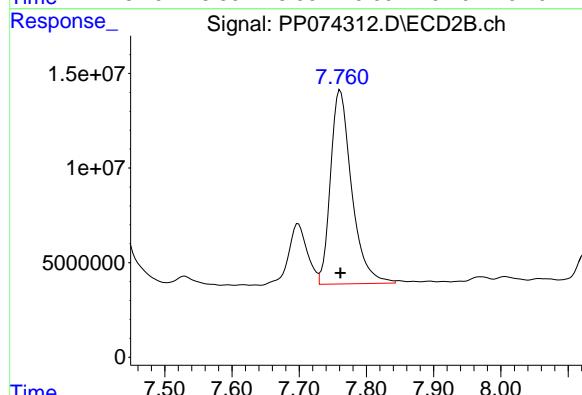


#39 AR-1262-4

R.T.: 7.761 min
 Delta R.T.: 0.000 min
 Response: 222582802
 Conc: 333.75 ng/ml

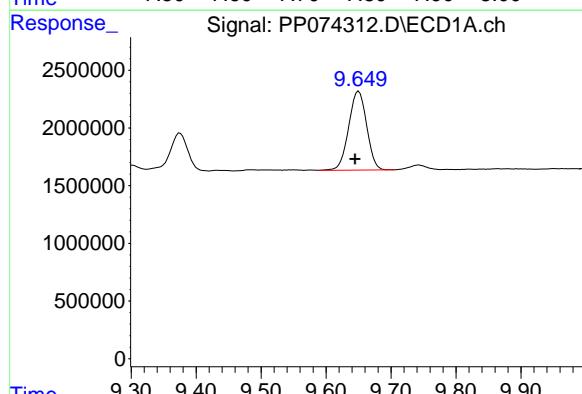


#40 AR-1262-5

R.T.: 9.650 min
 Delta R.T.: 0.006 min
 Response: 13192444
 Conc: 259.07 ng/ml

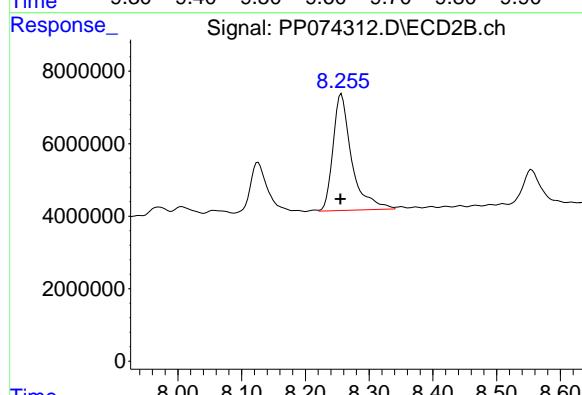

#40 AR-1262-5


R.T.: 8.257 min
 Delta R.T.: 0.002 min
 Response: 65413925
 Conc: 230.93 ng/ml

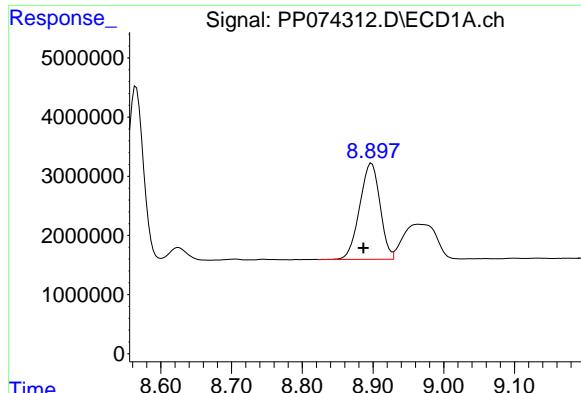

#41 AR-1268-1


R.T.: 8.898 min
 Delta R.T.: 0.012 min
 Response: 32396274
 Conc: 208.16 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

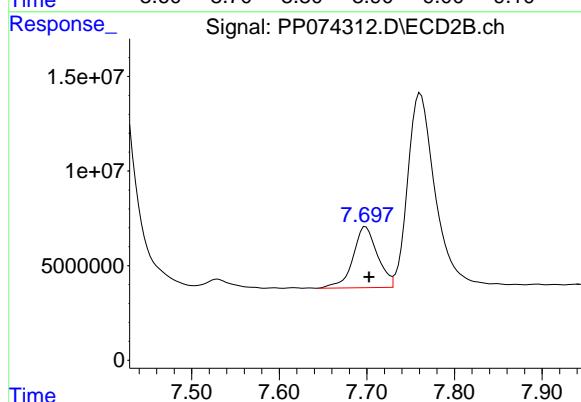


#41 AR-1268-1

R.T.: 7.699 min
 Delta R.T.: -0.004 min
 Response: 62513496
 Conc: 57.34 ng/ml

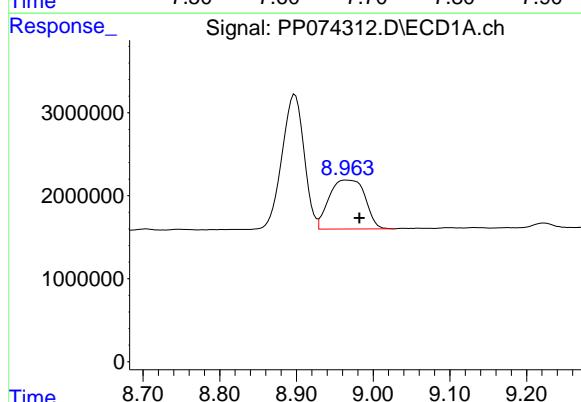


#42 AR-1268-2

R.T.: 8.965 min
 Delta R.T.: -0.017 min
 Response: 19192646
 Conc: 133.82 ng/ml

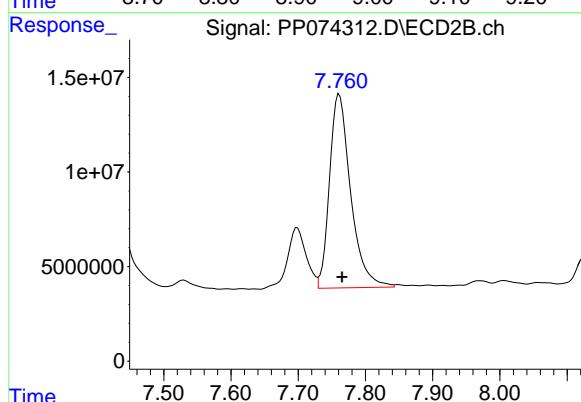

#42 AR-1268-2

R.T.: 7.761 min
 Delta R.T.: -0.004 min
 Response: 222582802
 Conc: 209.72 ng/ml

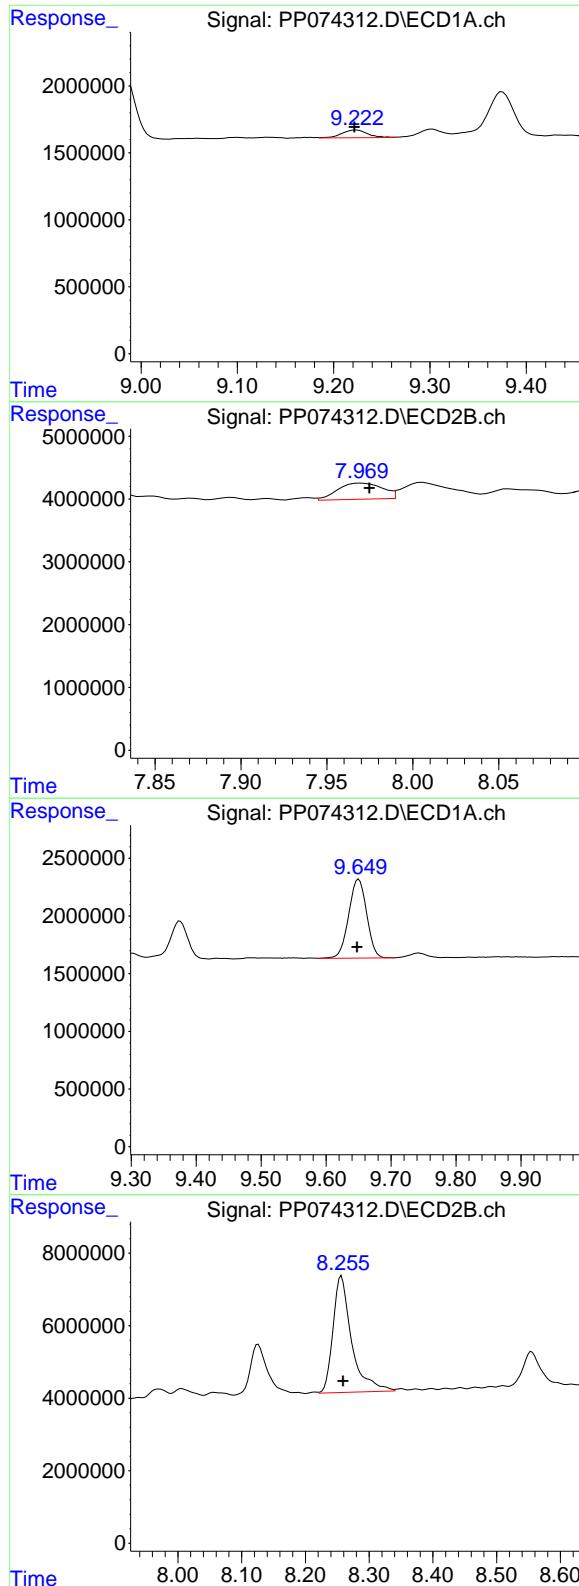

#43 AR-1268-3

R.T.: 9.223 min
 Delta R.T.: 0.001 min
 Response: 1061987
 Conc: 8.89 ng/ml

Instrument: ECD_P
ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

#43 AR-1268-3


R.T.: 7.970 min
 Delta R.T.: -0.005 min
 Response: 4622455
 Conc: 5.56 ng/ml

#44 AR-1268-4

R.T.: 9.650 min
 Delta R.T.: 0.002 min
 Response: 13192444
 Conc: 224.31 ng/ml

#44 AR-1268-4

R.T.: 8.257 min
 Delta R.T.: -0.003 min
 Response: 65413925
 Conc: 212.34 ng/ml

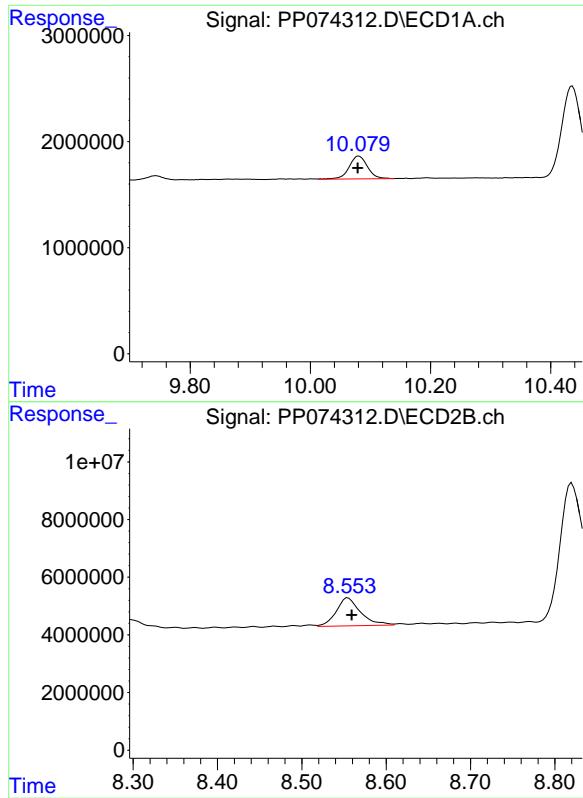

#45 AR-1268-5

R.T.: 10.081 min
 Delta R.T.: 0.002 min
 Response: 4521037
 Conc: 12.85 ng/ml

Instrument: ECD_P
 ClientSampleId: BIN0009-DRIVEWAY-TP-SOUTH-EASTMSD

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:48
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:54:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|----------|------|------|--------|--------|-------|-------|
|----------|------|------|--------|--------|-------|-------|

System Monitoring Compounds

| | | | | | | |
|---------------------|--------|-------|----------|---------|--------|--------|
| 1) SA Tetrachlor... | 4.659 | 3.803 | 64369772 | 233.9E6 | 57.560 | 60.987 |
| 2) SA Decachlor... | 10.436 | 8.820 | 50800485 | 333.5E6 | 52.309 | 55.456 |

Target Compounds

| | | | | | | |
|------------------|-------|-------|----------|----------|----------|------------|
| 3) L1 AR-1016-1 | 5.811 | 4.903 | 22974987 | 233.6E6 | 556.877 | 585.544 |
| 4) L1 AR-1016-2 | 5.832 | 4.960 | 33441672 | 115.6E6 | 550.555 | 615.345 |
| 5) L1 AR-1016-3 | 5.895 | 5.081 | 22187737 | 62696370 | 559.442 | 591.087 |
| 6) L1 AR-1016-4 | 5.992 | 5.122 | 18339102 | 65081402 | 563.509 | 595.874 |
| 7) L1 AR-1016-5 | 6.284 | 5.336 | 18014922 | 71852479 | 554.851 | 614.317 |
| 8) L2 AR-1221-1 | 4.854 | 4.013 | 2740944 | 7669936 | 163.506 | 156.258 |
| 9) L2 AR-1221-2 | 4.945 | 4.100 | 4124108 | 10102852 | 327.283 | 281.500 |
| 10) L2 AR-1221-3 | 5.020 | 4.176 | 13646312 | 48584576 | 372.492 | 359.288 |
| 11) L3 AR-1232-1 | 5.020 | 4.176 | 13646312 | 48584576 | 469.958 | 479.315 |
| 12) L3 AR-1232-2 | 5.546 | 4.903 | 17384703 | 233.6E6 | 1155.689 | 1340.284 |
| 13) L3 AR-1232-3 | 5.832 | 5.081 | 33441672 | 62696370 | 1153.093 | 1368.420 |
| 14) L3 AR-1232-4 | 5.992 | 5.164 | 18339102 | 115.7E6 | 1185.552 | 1995.265 # |
| 15) L3 AR-1232-5 | 6.081 | 5.336 | 16176910 | 71852479 | 1380.752 | 1529.445 |
| 16) L4 AR-1242-1 | 5.811 | 4.903 | 22974987 | 233.6E6 | 616.516 | 676.728 |
| 17) L4 AR-1242-2 | 5.832 | 4.960 | 33441672 | 115.6E6 | 614.636 | 707.363 |
| 18) L4 AR-1242-3 | 5.895 | 5.081 | 22187737 | 62696370 | 620.882 | 679.646 |
| 19) L4 AR-1242-4 | 5.992 | 5.164 | 18339102 | 115.7E6 | 627.651 | 969.228 # |
| 20) L4 AR-1242-5 | 6.722 | 5.686 | 6821787 | 88184525 | 191.849 | 589.626 # |
| 21) L5 AR-1248-1 | 5.811 | 4.903 | 22974987 | 233.6E6 | 820.109 | 1091.779 # |
| 22) L5 AR-1248-2 | 6.081 | 5.122 | 16176910 | 65081402 | 401.800 | 444.811 |
| 23) L5 AR-1248-3 | 6.284 | 5.164 | 18014922 | 115.7E6 | 404.162 | 675.065 # |
| 24) L5 AR-1248-4 | 6.658 | 5.336 | 23375703 | 71852479 | 449.212 | 431.874 |
| 25) L5 AR-1248-5 | 6.722 | 5.720 | 6821787 | 27151877 | 119.800 | 93.316 |
| 26) L6 AR-1254-1 | 6.658 | 5.686 | 23375703 | 88184525 | 444.059 | 240.822 # |
| 27) L6 AR-1254-2 | 6.874 | 5.833 | 14826525 | 70991951 | 186.486 | 255.168 # |
| 28) L6 AR-1254-3 | 7.236 | 6.250 | 9520749 | 139.6E6 | 109.038 | 285.322 # |
| 29) L6 AR-1254-4 | 7.519 | 6.461 | 6193777 | 13361436 | 97.067 | 36.351 # |
| 30) L6 AR-1254-5 | 7.933 | 6.879 | 47015566 | 180.5E6 | 579.404 | 468.662 |
| 31) L7 AR-1260-1 | 7.401 | 6.552 | 30236790 | 234.5E6 | 536.531 | 580.596 |
| 32) L7 AR-1260-2 | 7.654 | 6.706 | 35268906 | 177.9E6 | 517.501 | 568.793 |
| 33) L7 AR-1260-3 | 8.012 | 6.917 | 27864737 | 234.2E6 | 522.830 | 594.283 |
| 34) L7 AR-1260-4 | 8.240 | 7.175 | 33370027 | 169.9E6 | 532.940 | 583.961 |
| 35) L7 AR-1260-5 | 8.565 | 7.414 | 57421797 | 443.7E6 | 506.790 | 585.848 |
| 36) L8 AR-1262-1 | 8.240 | 6.917 | 33370027 | 234.2E6 | 440.298 | 415.912 |
| 37) L8 AR-1262-2 | 8.565 | 7.175 | 57421797 | 169.9E6 | 440.250 | 423.717 |
| 38) L8 AR-1262-3 | 8.897 | 7.698 | 39535257 | 94054093 | 420.271 | 261.647 # |
| 39) L8 AR-1262-4 | 8.976 | 7.761 | 26551541 | 296.1E6 | 364.460 | 444.010 |
| 40) L8 AR-1262-5 | 9.650 | 8.256 | 19147418 | 103.2E6 | 376.010 | 364.293 |
| 41) L9 AR-1268-1 | 8.897 | 7.698 | 39535257 | 94054093 | 254.029 | 86.267 # |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
 Data File : PP074316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Aug 2025 15:48
 Operator : YP\AJ
 Sample : AR1660CCC500
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 13 01:54:08 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Aug 04 11:01:49 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 μ l
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

| Compound | RT#1 | RT#2 | Resp#1 | Resp#2 | ng/ml | ng/ml |
|------------------|--------|-------|----------|----------|---------|-----------|
| 42) L9 AR-1268-2 | 8.976 | 7.761 | 26551541 | 296.1E6 | 185.124 | 279.009 # |
| 43) L9 AR-1268-3 | 9.223 | 7.968 | 1042857 | 4047686 | 8.729 | 4.865 # |
| 44) L9 AR-1268-4 | 9.650 | 8.256 | 19147418 | 103.2E6 | 325.567 | 334.977 |
| 45) L9 AR-1268-5 | 10.080 | 8.554 | 5562779 | 23797855 | 15.817 | 9.332 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP081225\
Data File : PP074316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Aug 2025 15:48
Operator : YP\AJ
Sample : AR1660CCC500
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
AR1660CCC500

```
Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 13 01:54:08 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP080125.M
Quant Title  : GC EXTRACTABLES
QLast Update : Mon Aug 04 11:01:49 2025
Response via : Initial Calibration
Integrator: ChemStation
```

Volume Inj. : 2 μ l
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50 μ Signal #2 Info : 30M x 0.32mm x 0.25 μ m

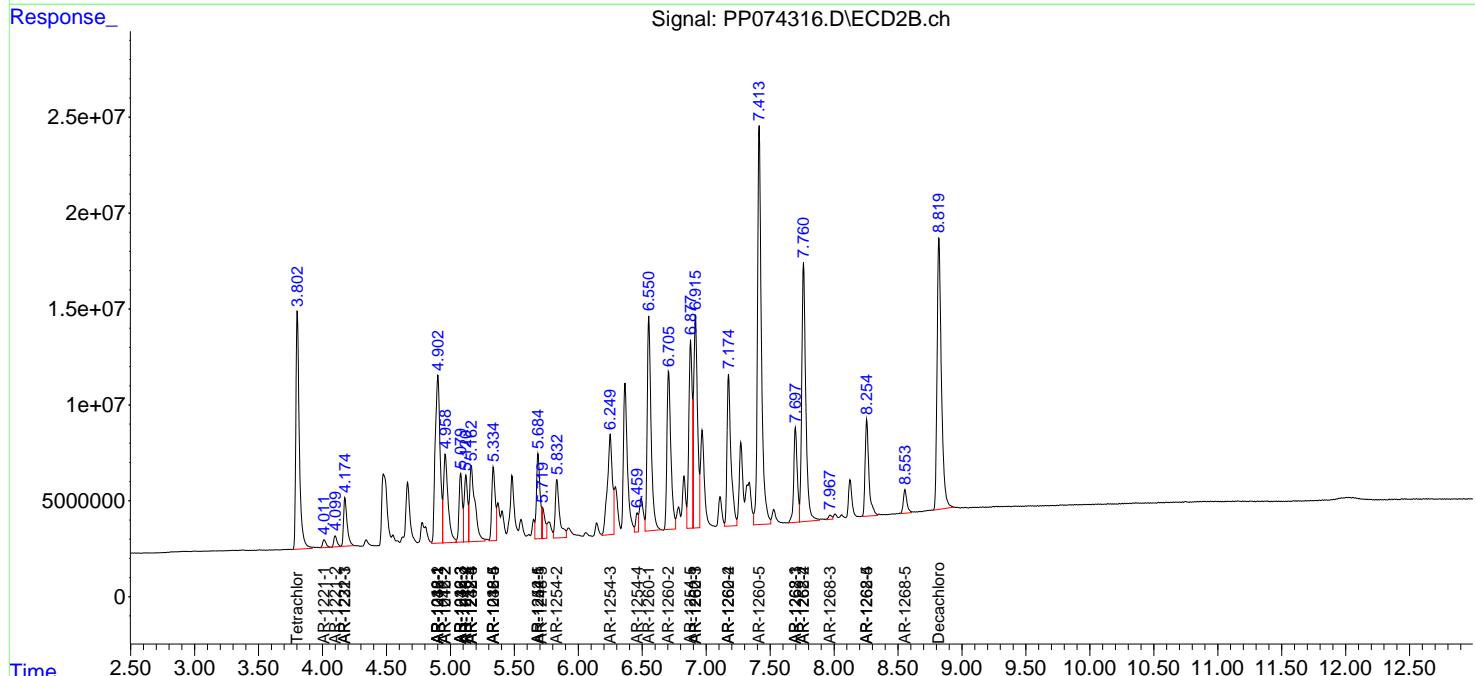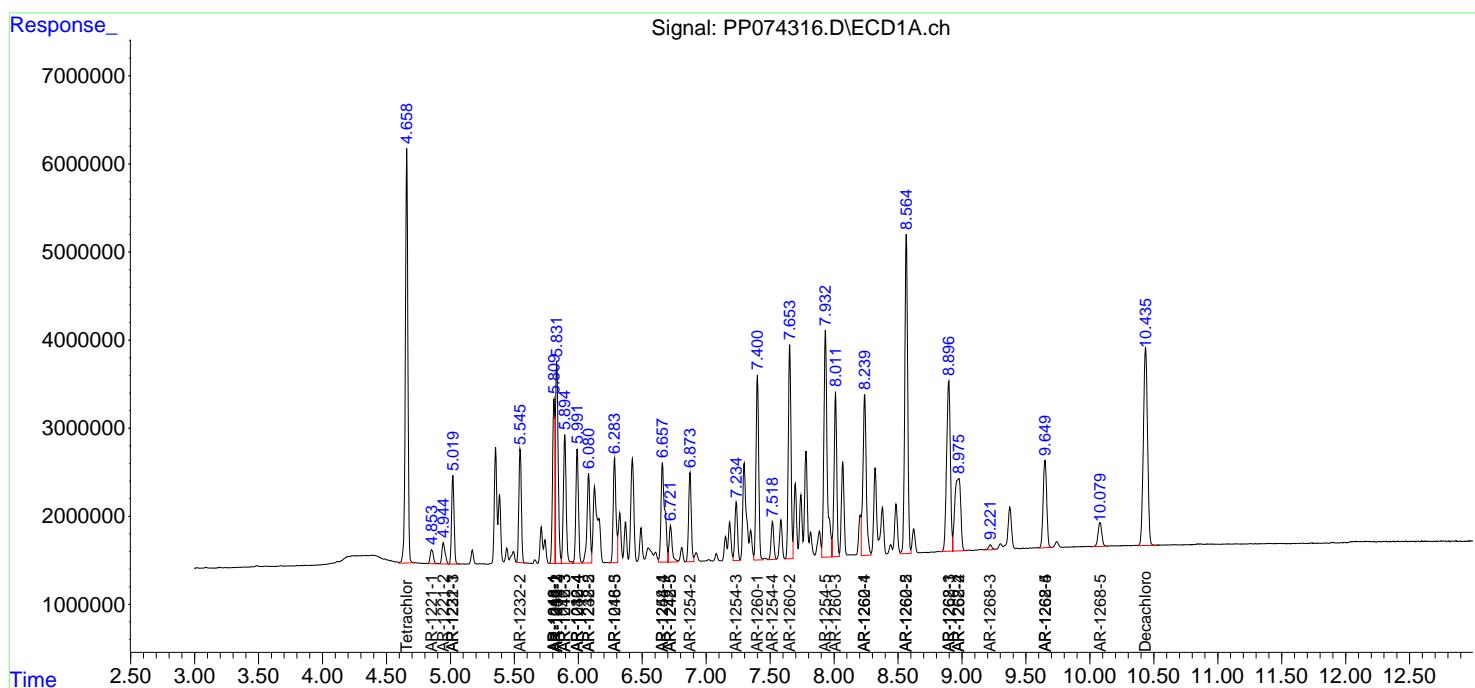

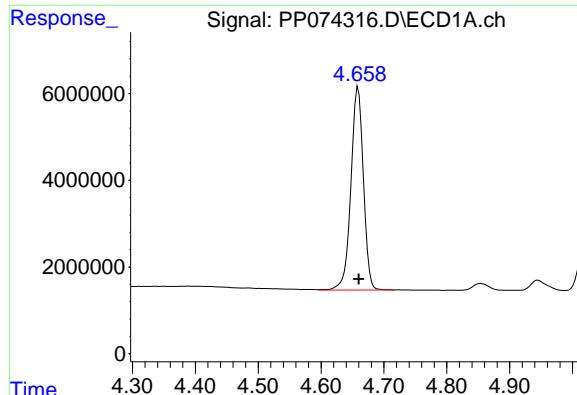


#1 Tetrachloro-m-xylene

R.T.: 4.659 min
Delta R.T.: 0.000 min
Response: 64369772
Conc: 57.56 ng/ml

Instrument:

ECD_P

ClientSampleId :
AR1660CCC500

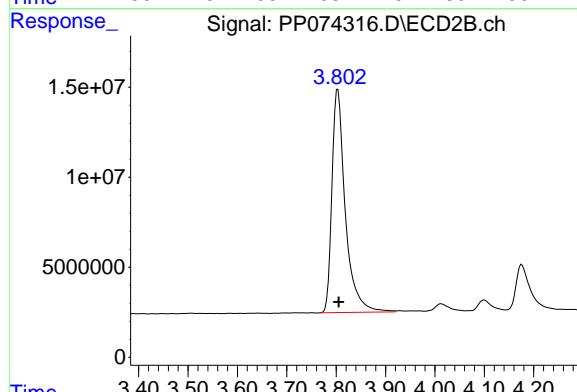

#1 Tetrachloro-m-xylene


R.T.: 3.803 min
Delta R.T.: -0.002 min
Response: 233851585
Conc: 60.99 ng/ml

#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: -0.002 min
Response: 50800485
Conc: 52.31 ng/ml

#2 Decachlorobiphenyl

R.T.: 8.820 min
Delta R.T.: -0.006 min
Response: 333491572
Conc: 55.46 ng/ml

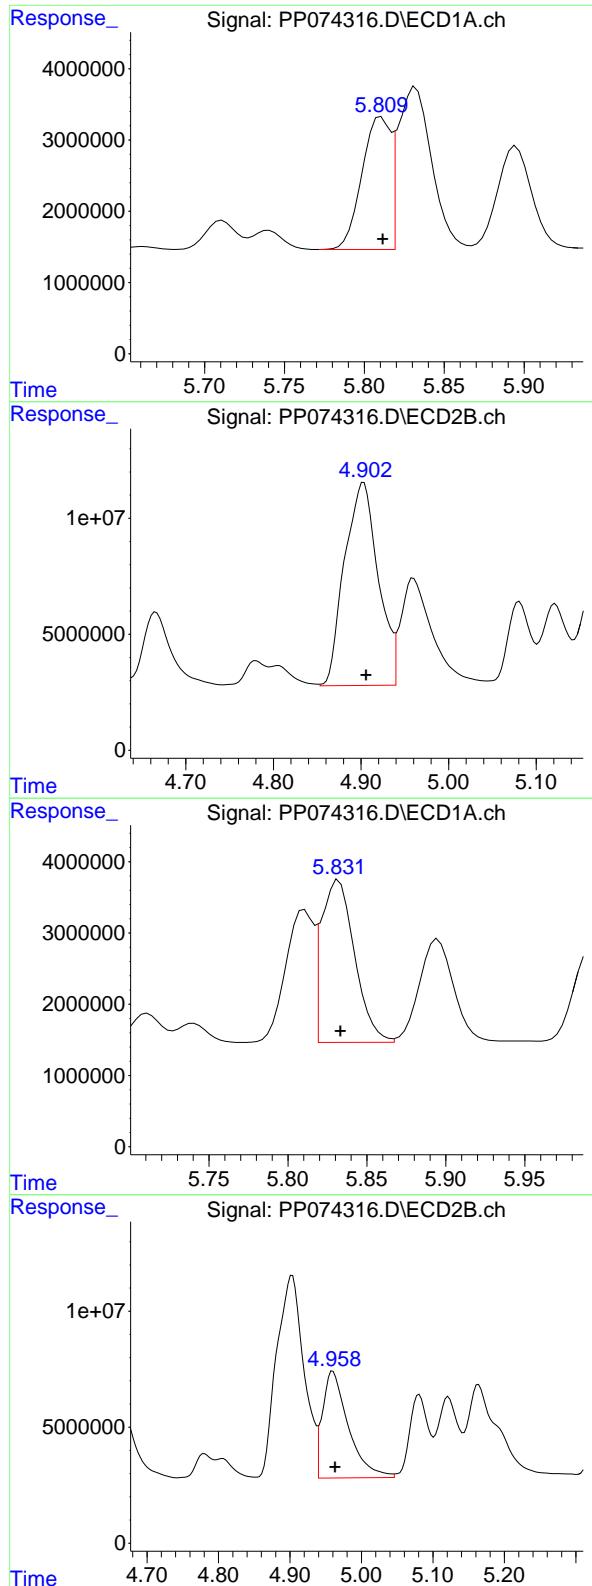

#3 AR-1016-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 22974987 ECD_P
 Conc: 556.88 ng/ml **ClientSampleId:**
 AR1660CCC500

#3 AR-1016-1


R.T.: 4.903 min
 Delta R.T.: -0.003 min
 Response: 233566270
 Conc: 585.54 ng/ml

#4 AR-1016-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 33441672
 Conc: 550.56 ng/ml

#4 AR-1016-2


R.T.: 4.960 min
 Delta R.T.: -0.003 min
 Response: 115567383
 Conc: 615.35 ng/ml

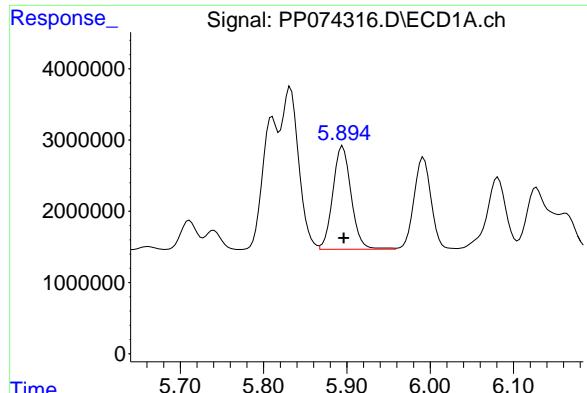

#5 AR-1016-3

R.T.: 5.895 min
 Delta R.T.: -0.001 min
 Response: 22187737
 Conc: 559.44 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

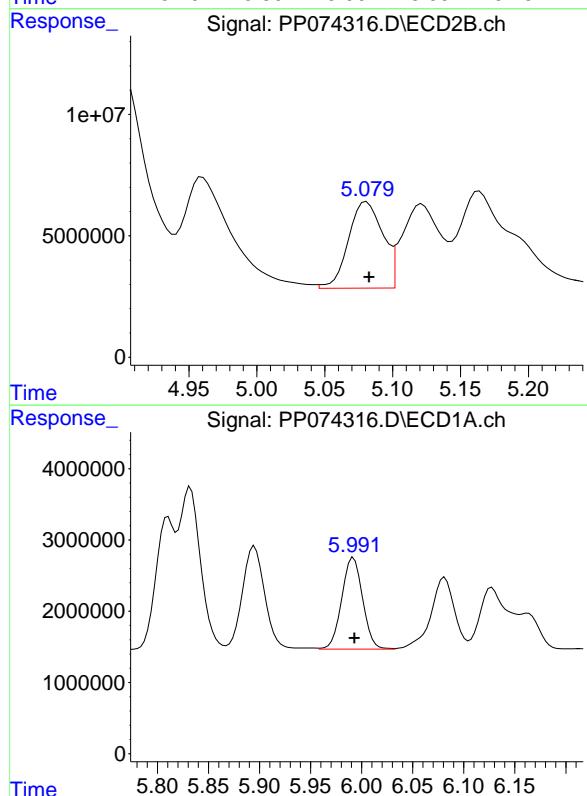


#6 AR-1016-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 18339102
 Conc: 563.51 ng/ml

#6 AR-1016-4


R.T.: 5.122 min
 Delta R.T.: -0.002 min
 Response: 65081402
 Conc: 595.87 ng/ml



#7 AR-1016-5


R.T.: 6.284 min
 Delta R.T.: -0.002 min
 Response: 18014922
 Conc: 554.85 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

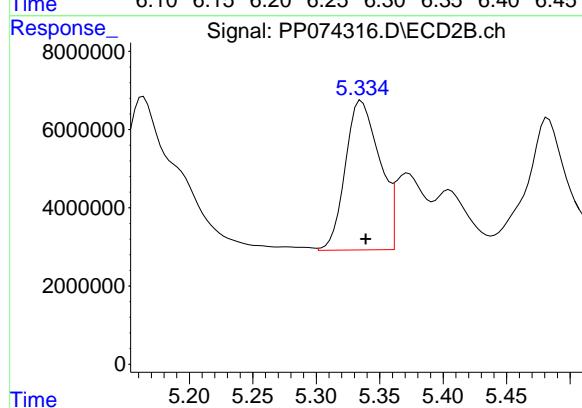


#7 AR-1016-5

R.T.: 5.336 min
 Delta R.T.: -0.003 min
 Response: 71852479
 Conc: 614.32 ng/ml

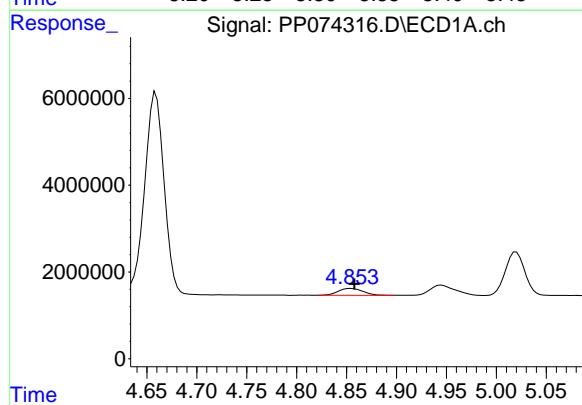


#8 AR-1221-1

R.T.: 4.854 min
 Delta R.T.: -0.003 min
 Response: 2740944
 Conc: 163.51 ng/ml

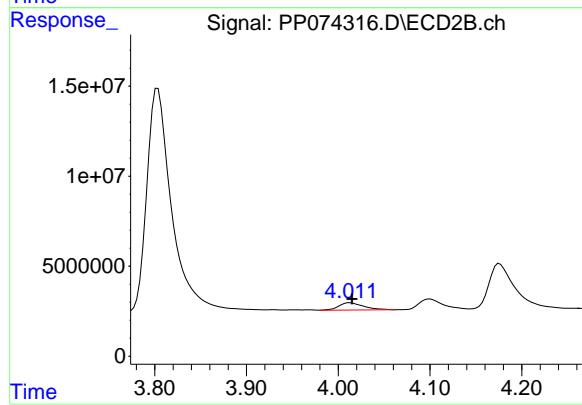

#8 AR-1221-1

R.T.: 4.013 min
 Delta R.T.: -0.002 min
 Response: 7669936
 Conc: 156.26 ng/ml

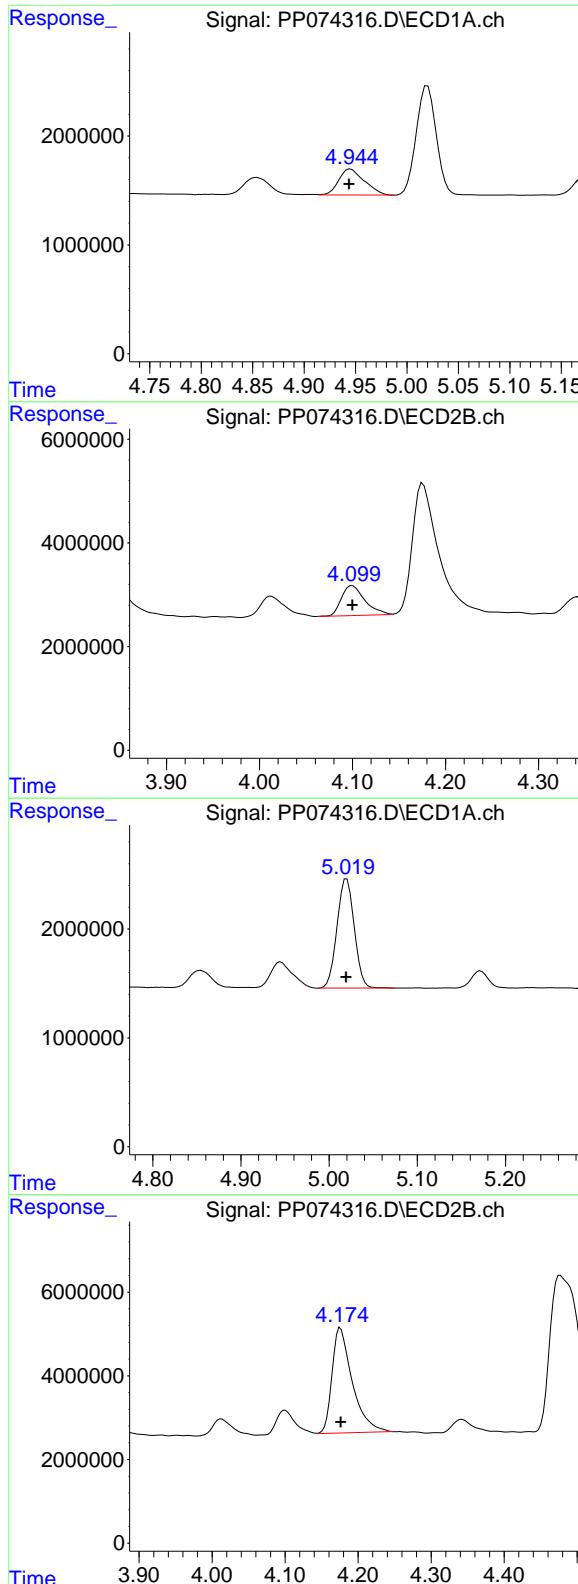

#9 AR-1221-2

R.T.: 4.945 min
 Delta R.T.: 0.002 min
 Response: 4124108
 Conc: 327.28 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#9 AR-1221-2


R.T.: 4.100 min
 Delta R.T.: 0.000 min
 Response: 10102852
 Conc: 281.50 ng/ml

#10 AR-1221-3

R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 13646312
 Conc: 372.49 ng/ml

#10 AR-1221-3

R.T.: 4.176 min
 Delta R.T.: 0.000 min
 Response: 48584576
 Conc: 359.29 ng/ml

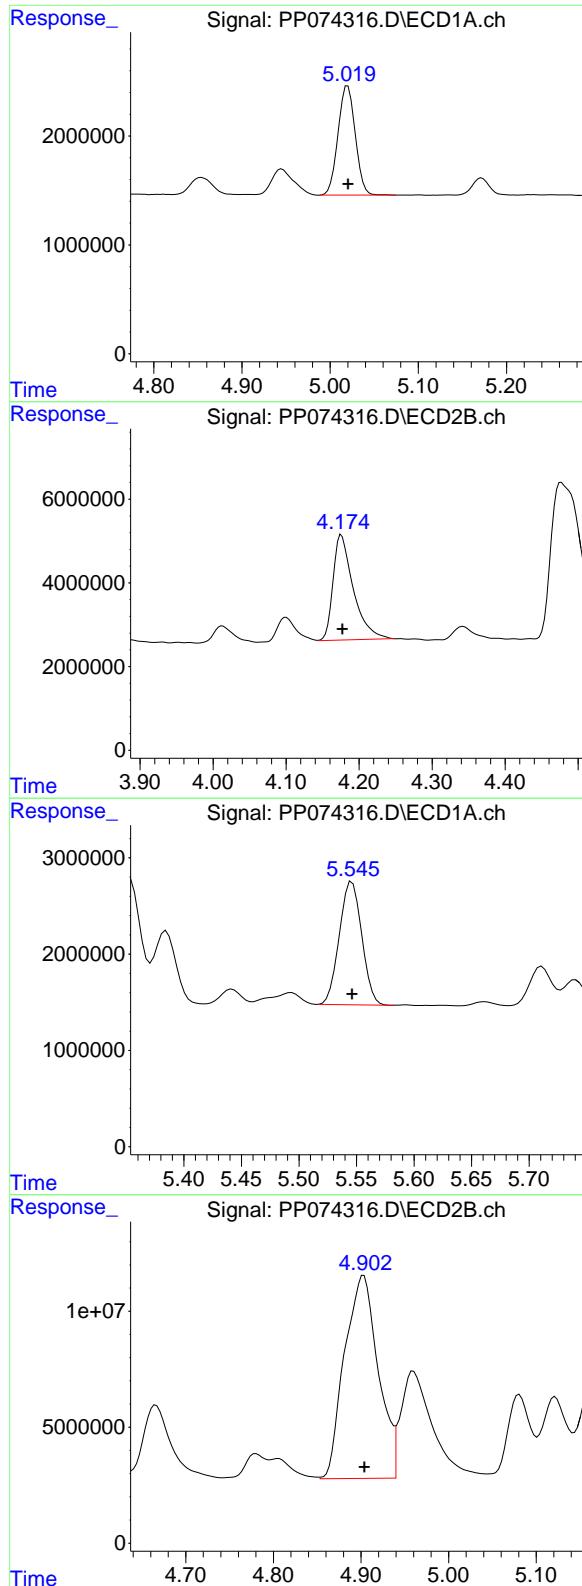

#11 AR-1232-1

R.T.: 5.020 min
 Delta R.T.: 0.000 min
 Response: 13646312
 Conc: 469.96 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#11 AR-1232-1


R.T.: 4.176 min
 Delta R.T.: -0.001 min
 Response: 48584576
 Conc: 479.32 ng/ml

#12 AR-1232-2

R.T.: 5.546 min
 Delta R.T.: 0.000 min
 Response: 17384703
 Conc: 1155.69 ng/ml

#12 AR-1232-2

R.T.: 4.903 min
 Delta R.T.: 0.000 min
 Response: 233566270
 Conc: 1340.28 ng/ml

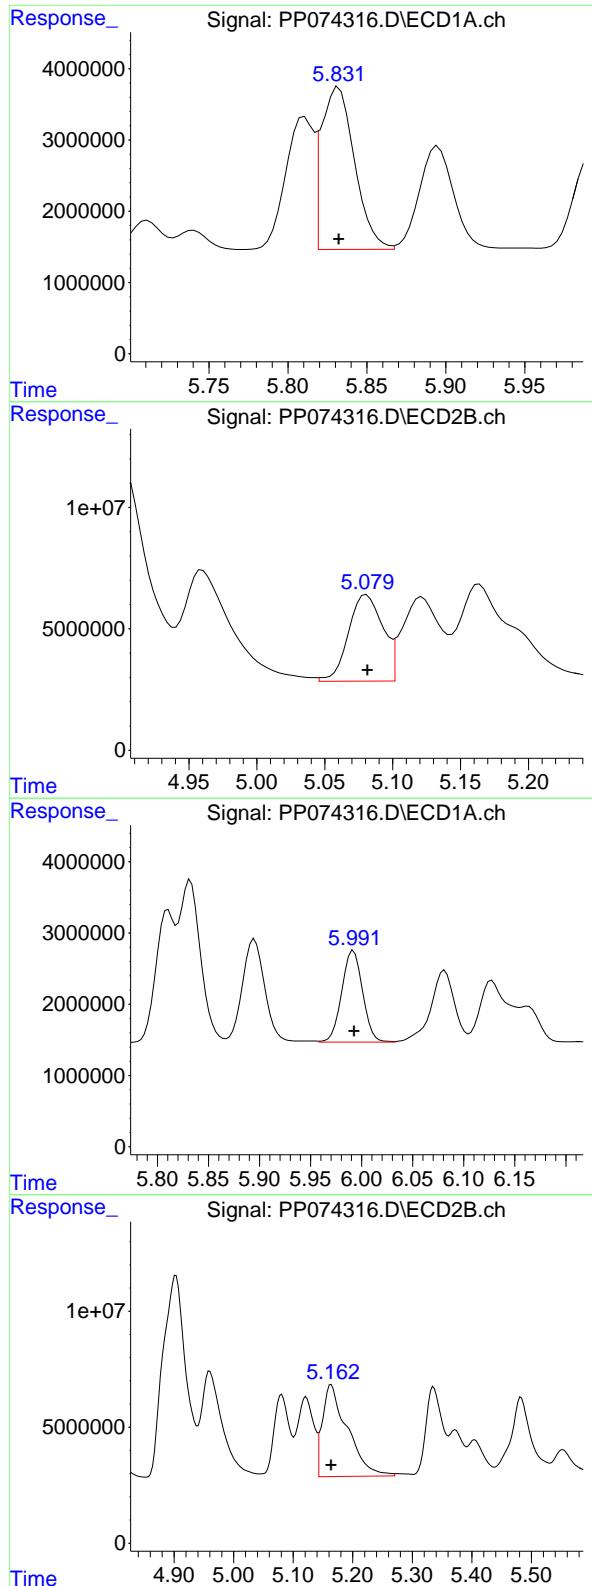

#13 AR-1232-3

R.T.: 5.832 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 33441672 ECD_P
 Conc: 1153.09 ng/ml **ClientSampleId:**
 AR1660CCC500

#13 AR-1232-3


R.T.: 5.081 min
 Delta R.T.: 0.000 min
 Response: 62696370
 Conc: 1368.42 ng/ml

#14 AR-1232-4

R.T.: 5.992 min
 Delta R.T.: 0.000 min
 Response: 18339102
 Conc: 1185.55 ng/ml


#14 AR-1232-4

R.T.: 5.164 min
 Delta R.T.: 0.000 min
 Response: 115746746
 Conc: 1995.27 ng/ml




#15 AR-1232-5

R.T.: 6.081 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 16176910 ECD_P
 Conc: 1380.75 ng/ml **ClientSampleId :**
 AR1660CCC500

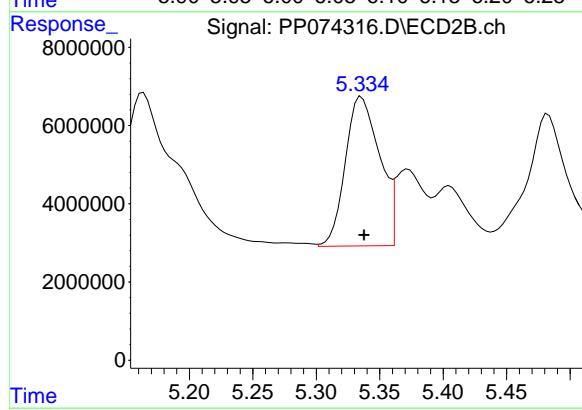


#15 AR-1232-5

R.T.: 5.336 min
 Delta R.T.: -0.002 min
 Response: 71852479
 Conc: 1529.44 ng/ml

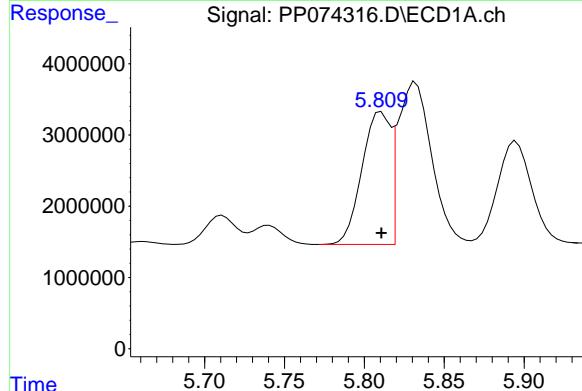


#16 AR-1242-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 22974987
 Conc: 616.52 ng/ml

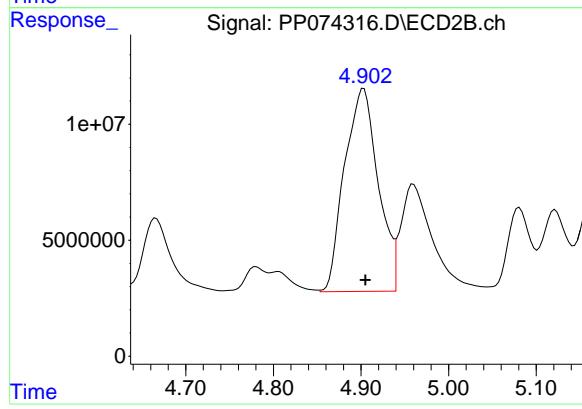

#16 AR-1242-1

R.T.: 4.903 min
 Delta R.T.: -0.002 min
 Response: 233566270
 Conc: 676.73 ng/ml

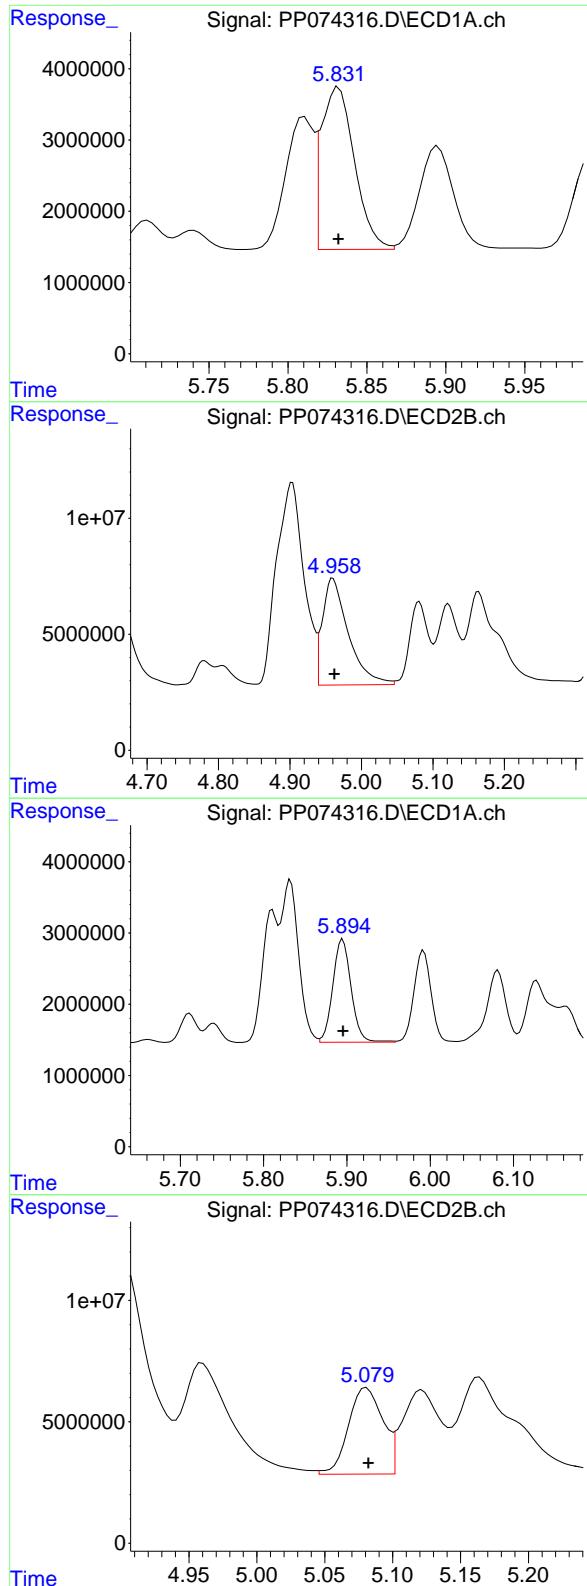

#17 AR-1242-2

R.T.: 5.832 min
 Delta R.T.: 0.000 min
 Response: 33441672
 Conc: 614.64 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#17 AR-1242-2


R.T.: 4.960 min
 Delta R.T.: -0.002 min
 Response: 115567383
 Conc: 707.36 ng/ml

#18 AR-1242-3

R.T.: 5.895 min
 Delta R.T.: 0.000 min
 Response: 22187737
 Conc: 620.88 ng/ml


#18 AR-1242-3

R.T.: 5.081 min
 Delta R.T.: -0.001 min
 Response: 62696370
 Conc: 679.65 ng/ml




#19 AR-1242-4

R.T.: 5.992 min
Delta R.T.: 0.000 min **Instrument:**
Response: 18339102 ECD_P
Conc: 627.65 ng/ml **ClientSampleId:**
AR1660CCC500

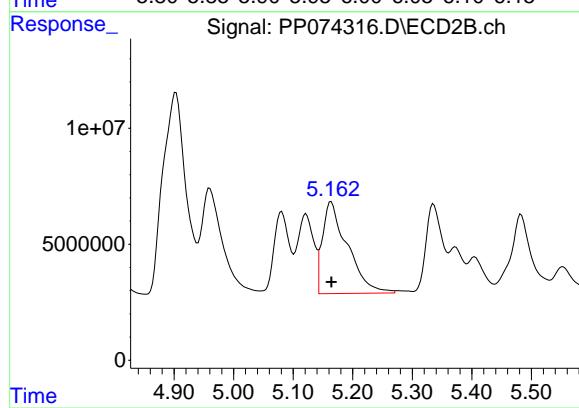


#19 AR-1242-4

R.T.: 5.164 min
Delta R.T.: 0.000 min
Response: 115746746
Conc: 969.23 ng/ml

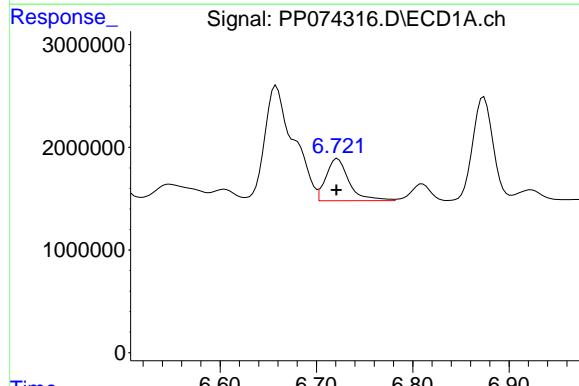


#20 AR-1242-5

R.T.: 6.722 min
Delta R.T.: 0.001 min
Response: 6821787
Conc: 191.85 ng/ml

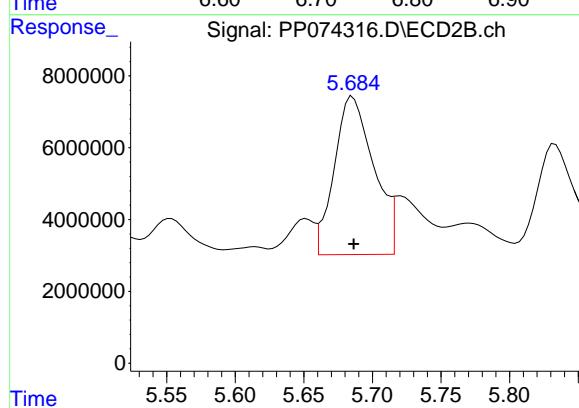

#20 AR-1242-5

R.T.: 5.686 min
Delta R.T.: 0.000 min
Response: 88184525
Conc: 589.63 ng/ml

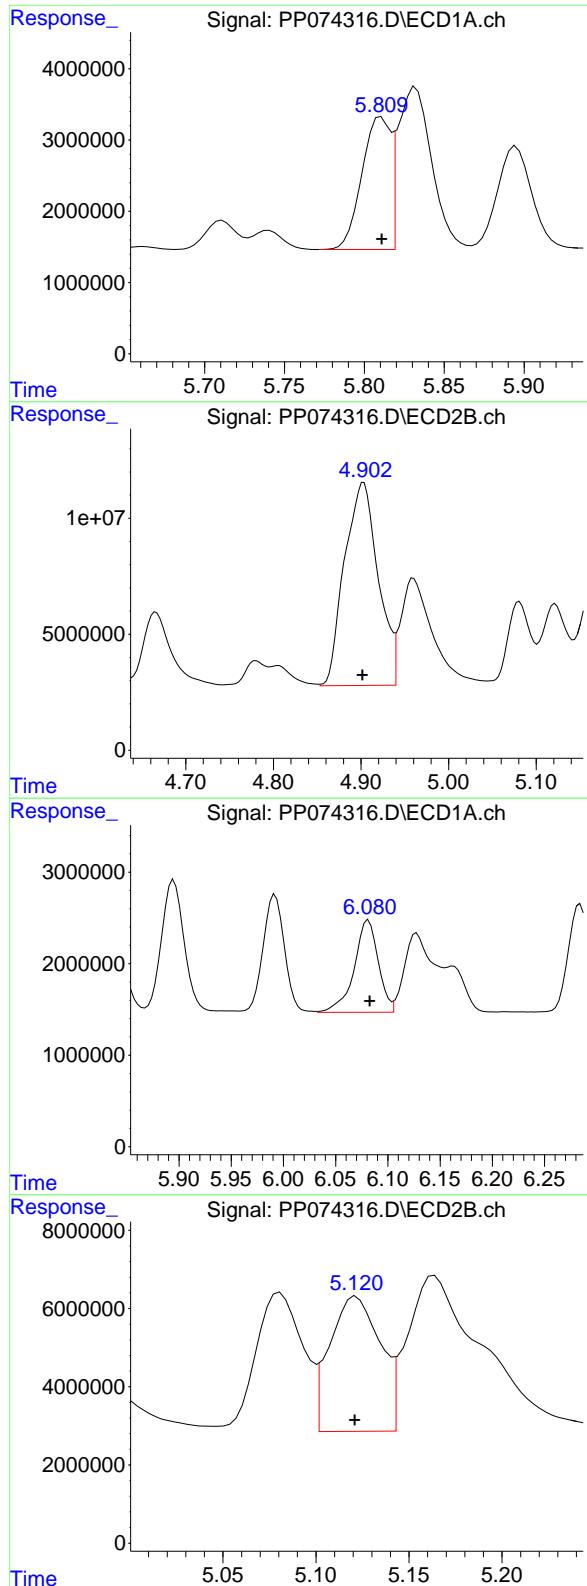

#21 AR-1248-1

R.T.: 5.811 min
 Delta R.T.: 0.000 min
 Response: 22974987
 Conc: 820.11 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#21 AR-1248-1


R.T.: 4.903 min
 Delta R.T.: 0.001 min
 Response: 233566270
 Conc: 1091.78 ng/ml

#22 AR-1248-2

R.T.: 6.081 min
 Delta R.T.: -0.001 min
 Response: 16176910
 Conc: 401.80 ng/ml

#22 AR-1248-2


R.T.: 5.122 min
 Delta R.T.: 0.000 min
 Response: 65081402
 Conc: 444.81 ng/ml

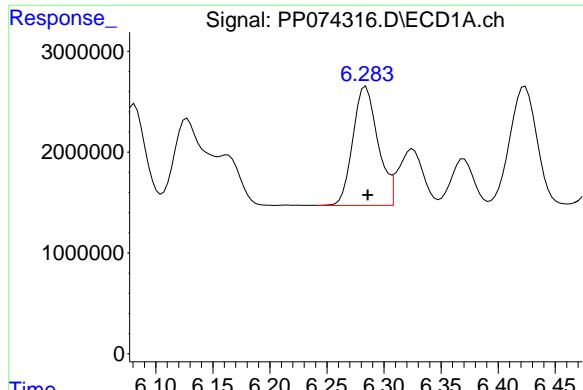

#23 AR-1248-3


R.T.: 6.284 min
Delta R.T.: -0.002 min
Response: 18014922
Conc: 404.16 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500

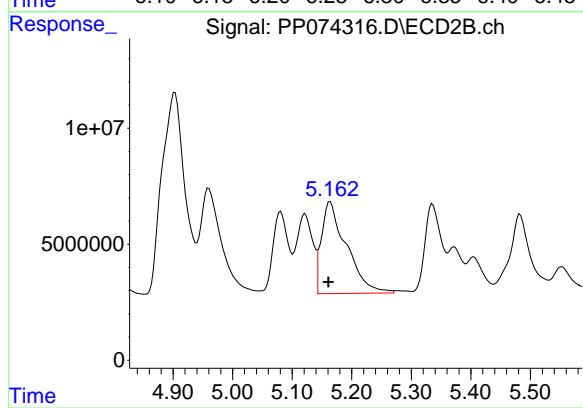


#23 AR-1248-3

R.T.: 5.164 min
Delta R.T.: 0.003 min
Response: 115746746
Conc: 675.07 ng/ml

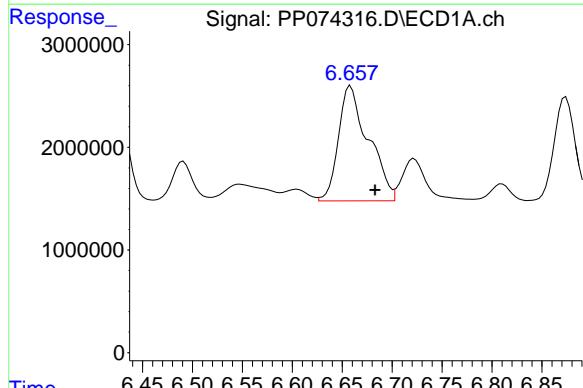


#24 AR-1248-4

R.T.: 6.658 min
Delta R.T.: -0.025 min
Response: 23375703
Conc: 449.21 ng/ml

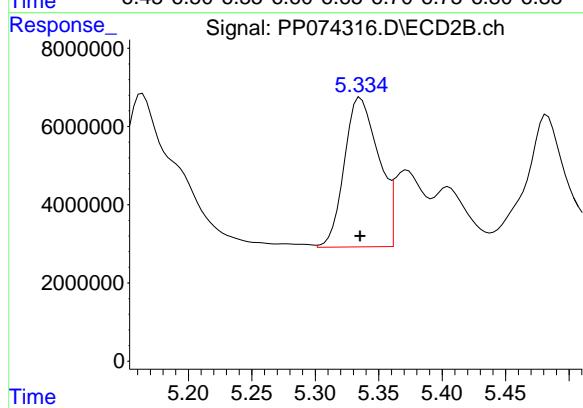

#24 AR-1248-4


R.T.: 5.336 min
Delta R.T.: 0.000 min
Response: 71852479
Conc: 431.87 ng/ml



#25 AR-1248-5


R.T.: 6.722 min
Delta R.T.: 0.000 min
Response: 6821787
Conc: 119.80 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500

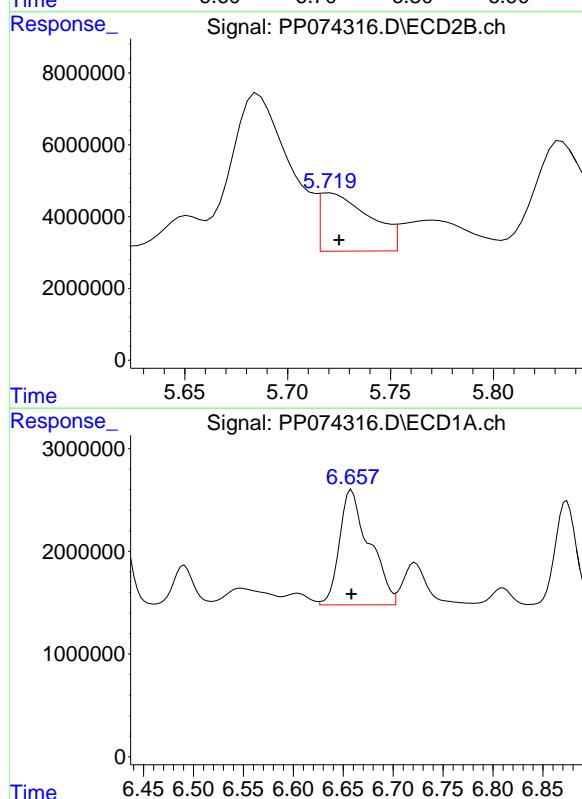


#26 AR-1254-1

R.T.: 6.658 min
Delta R.T.: 0.000 min
Response: 23375703
Conc: 444.06 ng/ml

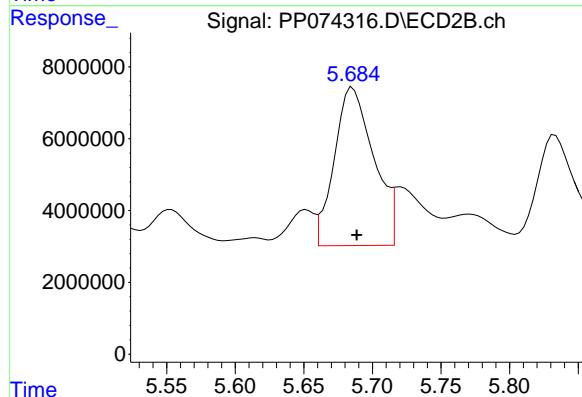

#26 AR-1254-1

R.T.: 5.686 min
Delta R.T.: -0.003 min
Response: 88184525
Conc: 240.82 ng/ml

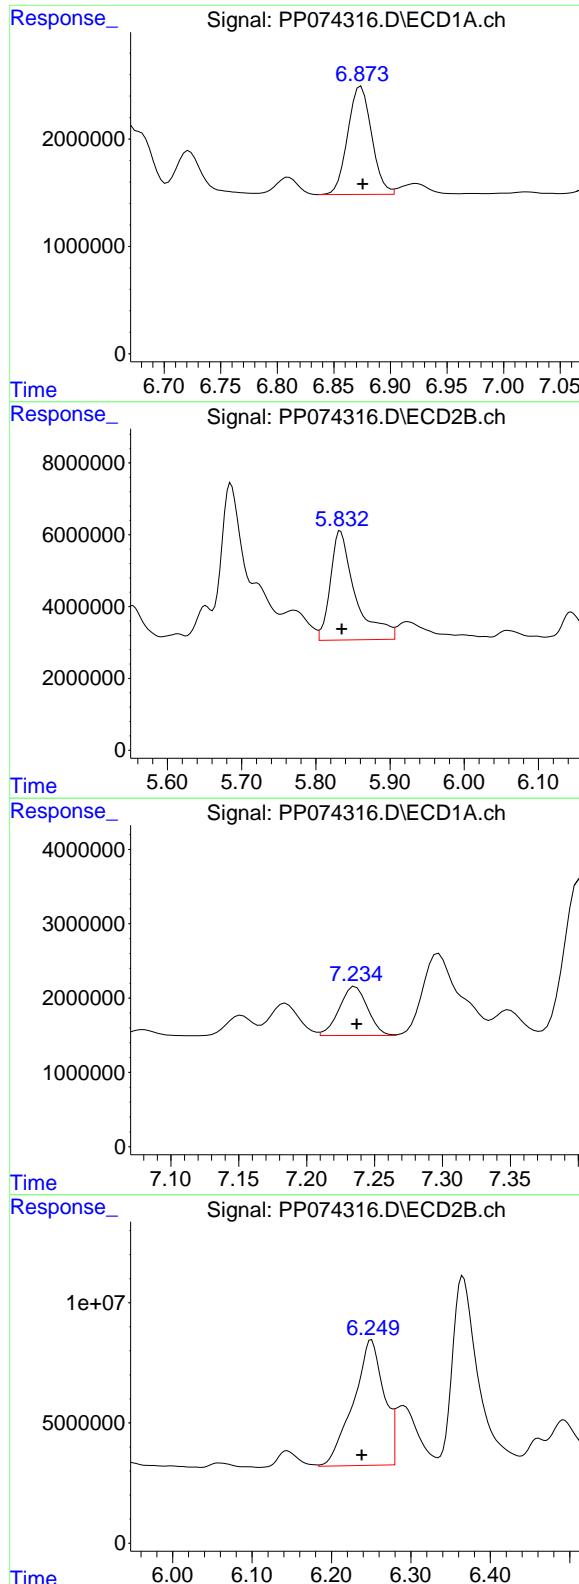

#27 AR-1254-2

R.T.: 6.874 min
 Delta R.T.: -0.001 min
 Response: 14826525
 Conc: 186.49 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

#27 AR-1254-2


R.T.: 5.833 min
 Delta R.T.: -0.002 min
 Response: 70991951
 Conc: 255.17 ng/ml

#28 AR-1254-3

R.T.: 7.236 min
 Delta R.T.: -0.001 min
 Response: 9520749
 Conc: 109.04 ng/ml


#28 AR-1254-3

R.T.: 6.250 min
 Delta R.T.: 0.012 min
 Response: 139582747
 Conc: 285.32 ng/ml

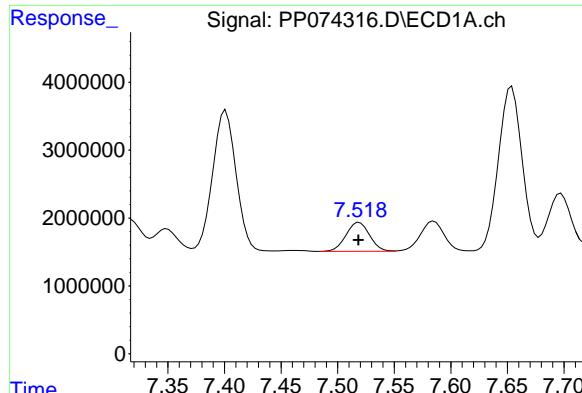


#29 AR-1254-4

R.T.: 7.519 min
 Delta R.T.: 0.000 min **Instrument:**
 Response: 6193777 ECD_P
 Conc: 97.07 ng/ml **ClientSampleId :**
 AR1660CCC500

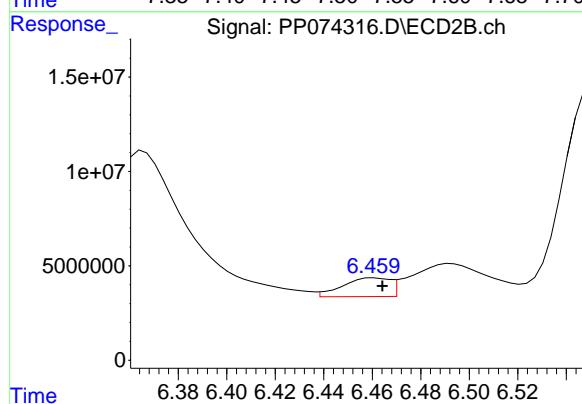


#29 AR-1254-4

R.T.: 6.461 min
 Delta R.T.: -0.003 min
 Response: 13361436
 Conc: 36.35 ng/ml

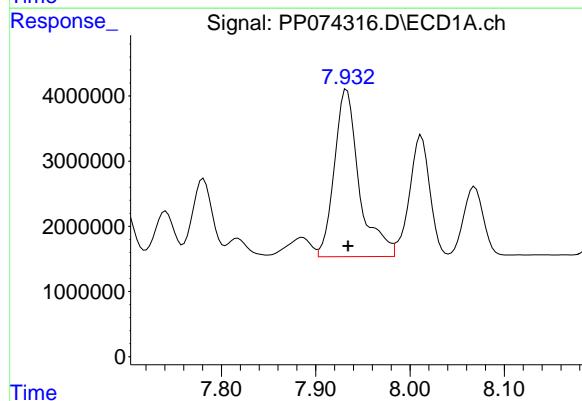


#30 AR-1254-5

R.T.: 7.933 min
 Delta R.T.: -0.002 min
 Response: 47015566
 Conc: 579.40 ng/ml

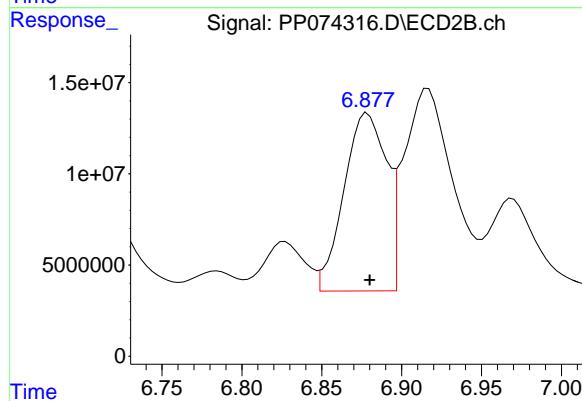

#30 AR-1254-5

R.T.: 6.879 min
 Delta R.T.: -0.001 min
 Response: 180513241
 Conc: 468.66 ng/ml

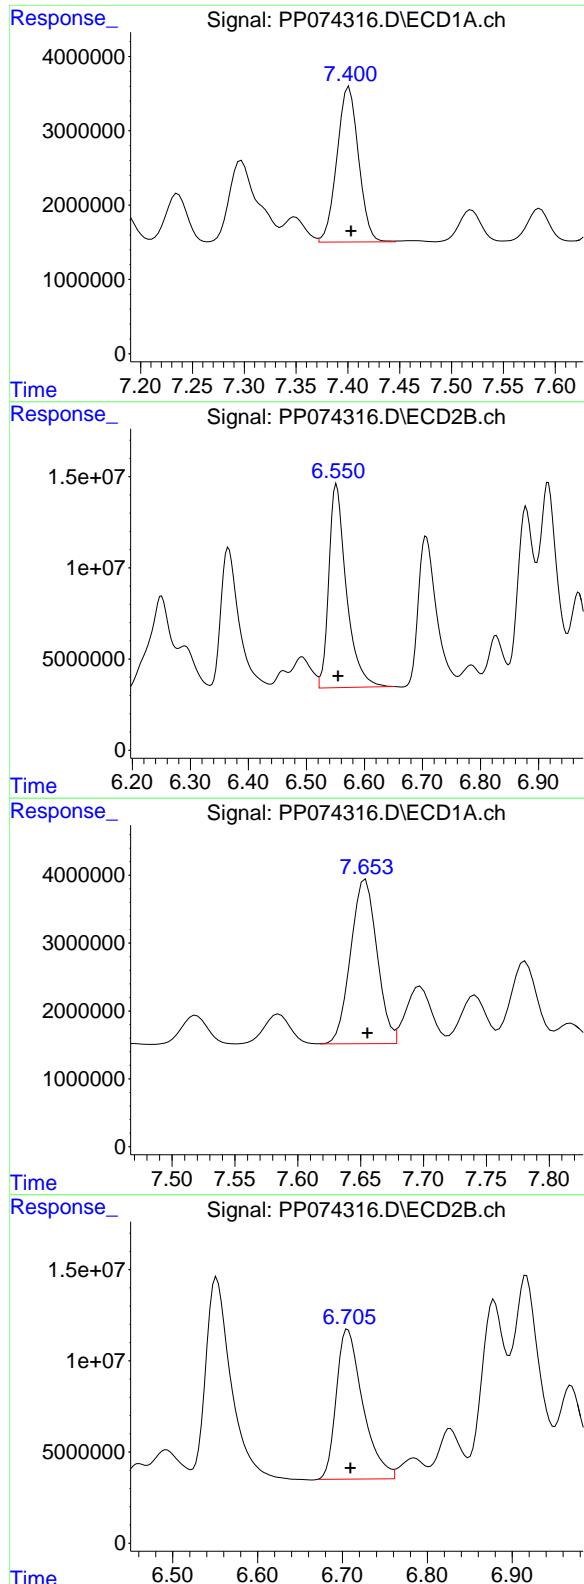

#31 AR-1260-1

R.T.: 7.401 min
 Delta R.T.: -0.002 min
 Response: 30236790
 Conc: 536.53 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500

#31 AR-1260-1


R.T.: 6.552 min
 Delta R.T.: -0.003 min
 Response: 234535731
 Conc: 580.60 ng/ml

#32 AR-1260-2

R.T.: 7.654 min
 Delta R.T.: -0.001 min
 Response: 35268906
 Conc: 517.50 ng/ml

#32 AR-1260-2


R.T.: 6.706 min
 Delta R.T.: -0.003 min
 Response: 177860970
 Conc: 568.79 ng/ml

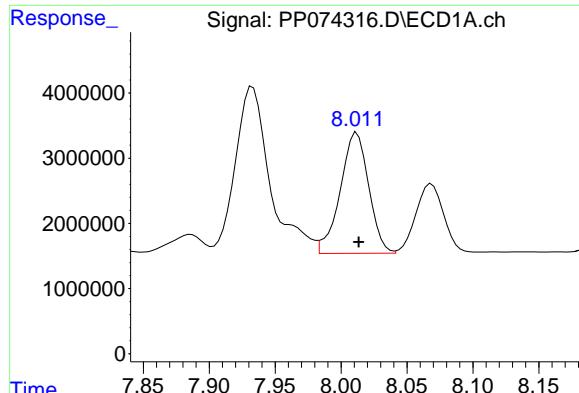

#33 AR-1260-3


R.T.: 8.012 min
 Delta R.T.: -0.001 min
 Response: 27864737
 Conc: 522.83 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

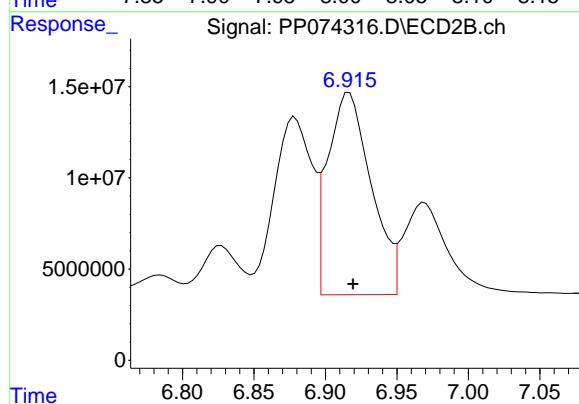


#33 AR-1260-3

R.T.: 6.917 min
 Delta R.T.: -0.003 min
 Response: 234217922
 Conc: 594.28 ng/ml

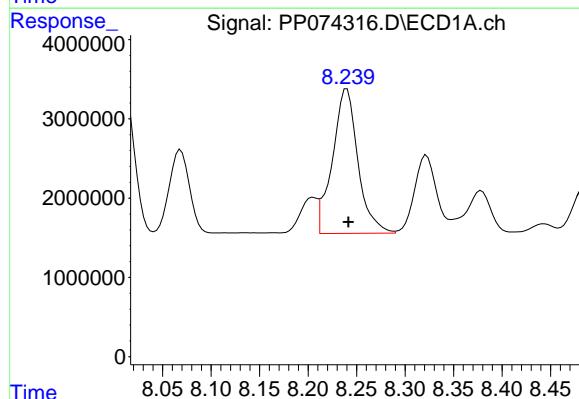


#34 AR-1260-4

R.T.: 8.240 min
 Delta R.T.: -0.002 min
 Response: 33370027
 Conc: 532.94 ng/ml

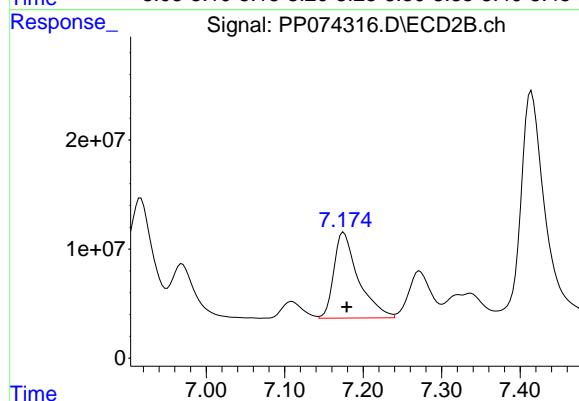

#34 AR-1260-4


R.T.: 7.175 min
 Delta R.T.: -0.004 min
 Response: 169920550
 Conc: 583.96 ng/ml

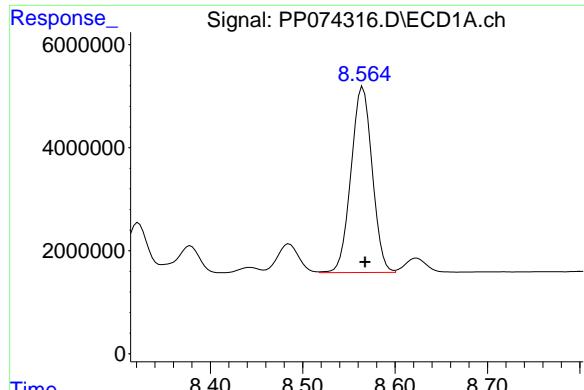

#35 AR-1260-5


R.T.: 8.565 min
 Delta R.T.: -0.002 min
 Response: 57421797
 Conc: 506.79 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

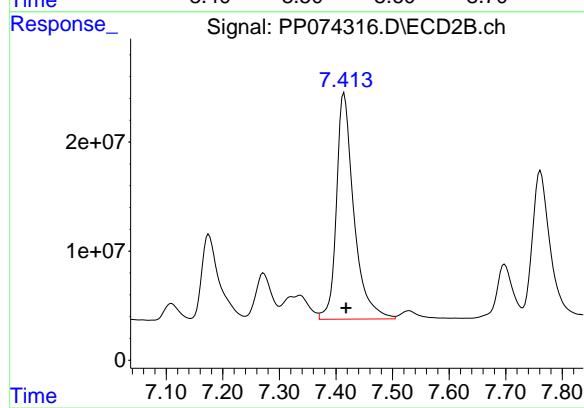


#35 AR-1260-5

R.T.: 7.414 min
 Delta R.T.: -0.004 min
 Response: 443727135
 Conc: 585.85 ng/ml

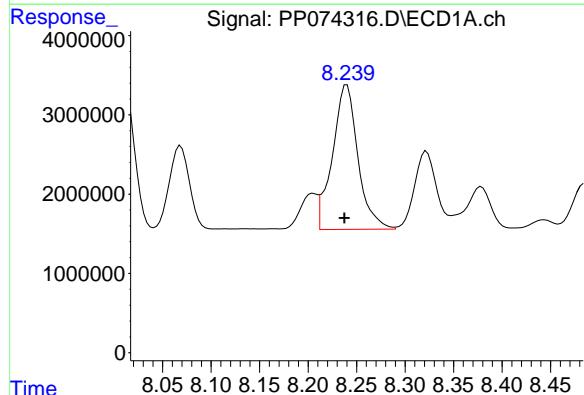


#36 AR-1262-1

R.T.: 8.240 min
 Delta R.T.: 0.003 min
 Response: 33370027
 Conc: 440.30 ng/ml

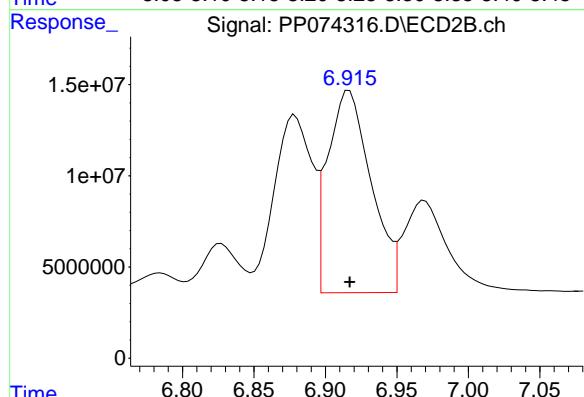

#36 AR-1262-1


R.T.: 6.917 min
 Delta R.T.: 0.000 min
 Response: 234217922
 Conc: 415.91 ng/ml



#37 AR-1262-2


R.T.: 8.565 min
Delta R.T.: 0.004 min
Response: 57421797
Conc: 440.25 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500

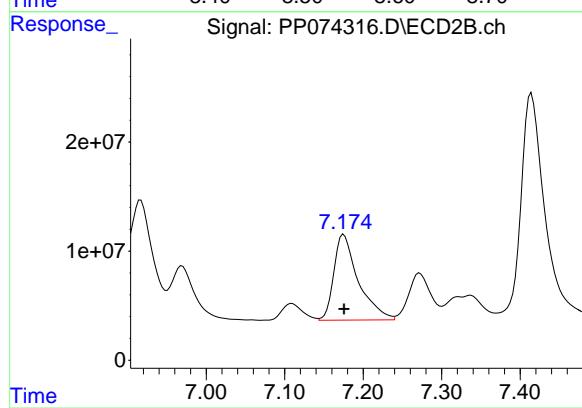


#37 AR-1262-2

R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 169920550
Conc: 423.72 ng/ml

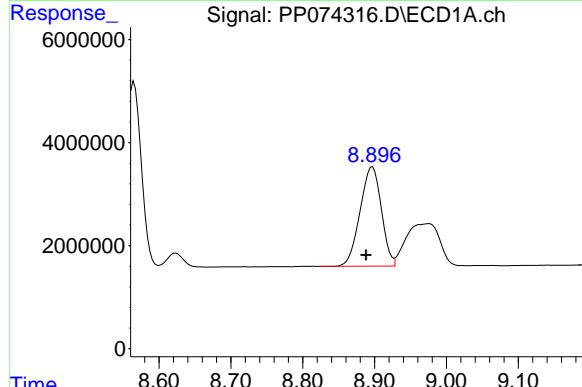


#38 AR-1262-3

R.T.: 8.897 min
Delta R.T.: 0.009 min
Response: 39535257
Conc: 420.27 ng/ml

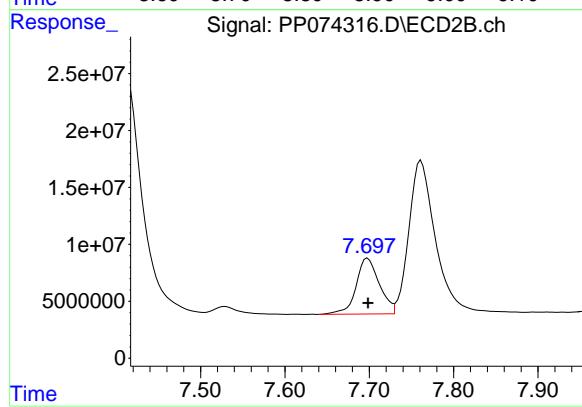

#38 AR-1262-3


R.T.: 7.698 min
Delta R.T.: 0.000 min
Response: 94054093
Conc: 261.65 ng/ml

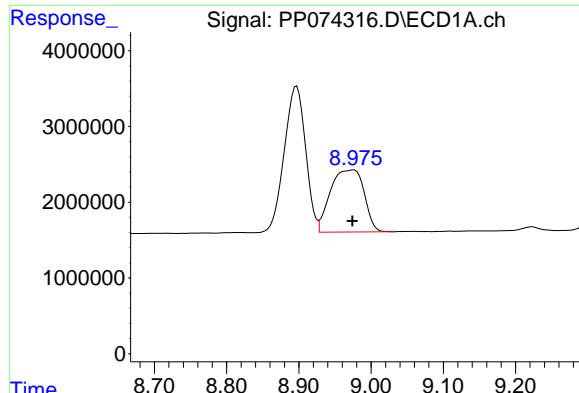

#39 AR-1262-4


R.T.: 8.976 min
 Delta R.T.: 0.002 min
 Response: 26551541
 Conc: 364.46 ng/ml

Instrument: ECD_P
 ClientSampleId: AR1660CCC500

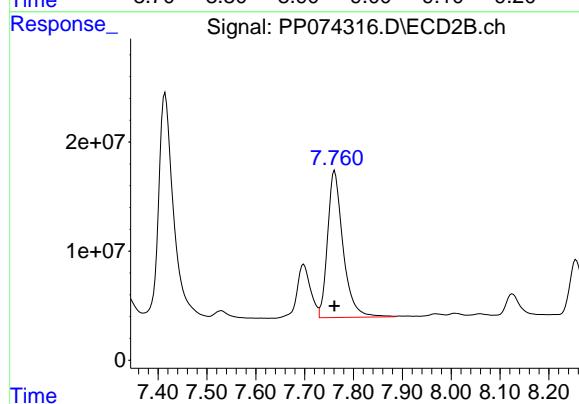


#39 AR-1262-4

R.T.: 7.761 min
 Delta R.T.: 0.000 min
 Response: 296119665
 Conc: 444.01 ng/ml

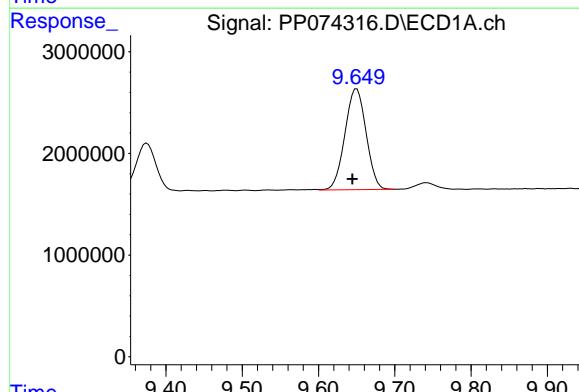


#40 AR-1262-5

R.T.: 9.650 min
 Delta R.T.: 0.005 min
 Response: 19147418
 Conc: 376.01 ng/ml

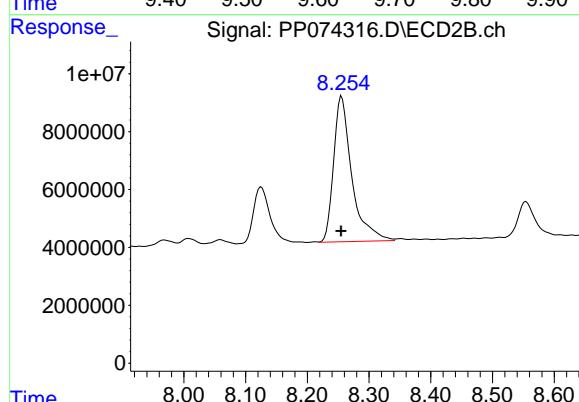

#40 AR-1262-5


R.T.: 8.256 min
 Delta R.T.: 0.000 min
 Response: 103192666
 Conc: 364.29 ng/ml



#41 AR-1268-1


R.T.: 8.897 min
Delta R.T.: 0.011 min
Response: 39535257
Conc: 254.03 ng/ml

Instrument: ECD_P
ClientSampleId: AR1660CCC500

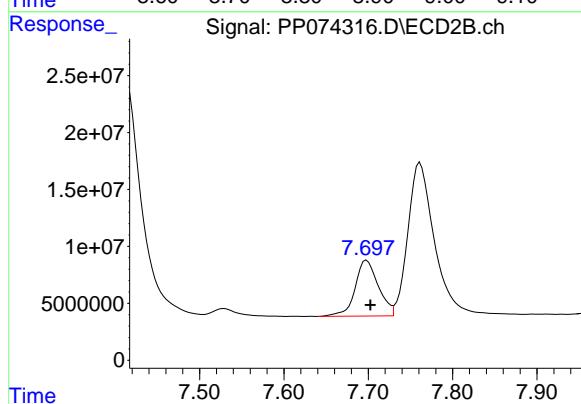


#41 AR-1268-1

R.T.: 7.698 min
Delta R.T.: -0.004 min
Response: 94054093
Conc: 86.27 ng/ml

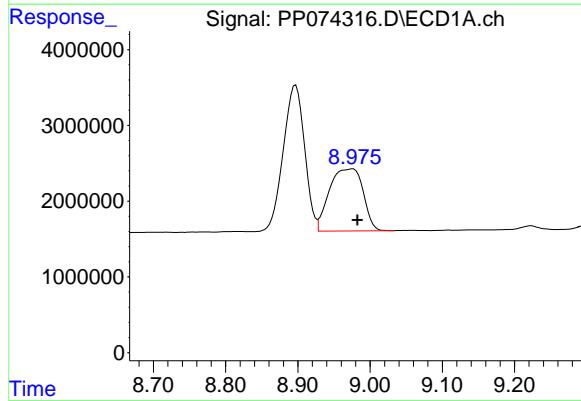


#42 AR-1268-2

R.T.: 8.976 min
Delta R.T.: -0.006 min
Response: 26551541
Conc: 185.12 ng/ml

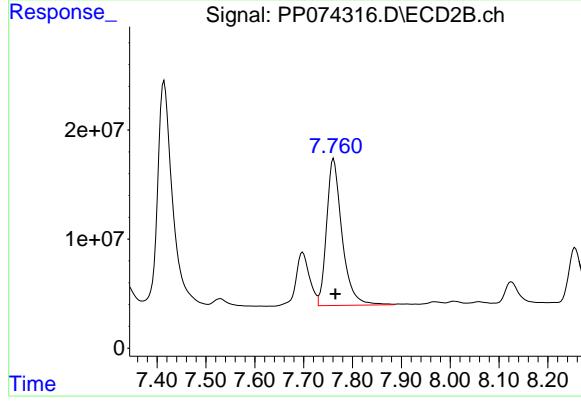


#42 AR-1268-2

R.T.: 7.761 min
Delta R.T.: -0.004 min
Response: 296119665
Conc: 279.01 ng/ml

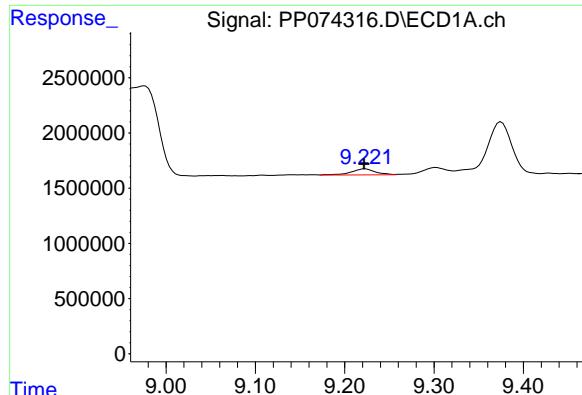


#43 AR-1268-3

R.T.: 9.223 min
 Delta R.T.: 0.001 min **Instrument:**
 Response: 1042857 ECD_P
 Conc: 8.73 ng/ml **ClientSampleId:**
 AR1660CCC500

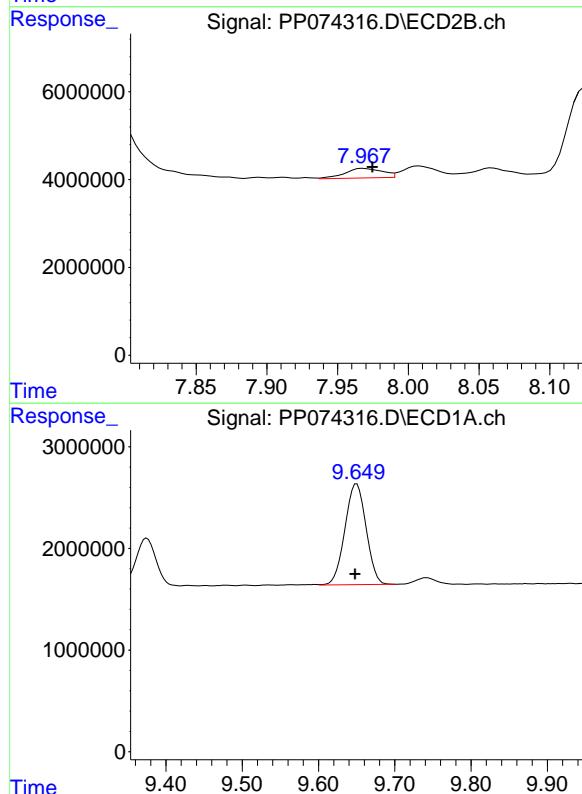


#44 AR-1268-4

R.T.: 9.650 min
 Delta R.T.: 0.002 min
 Response: 19147418
 Conc: 325.57 ng/ml

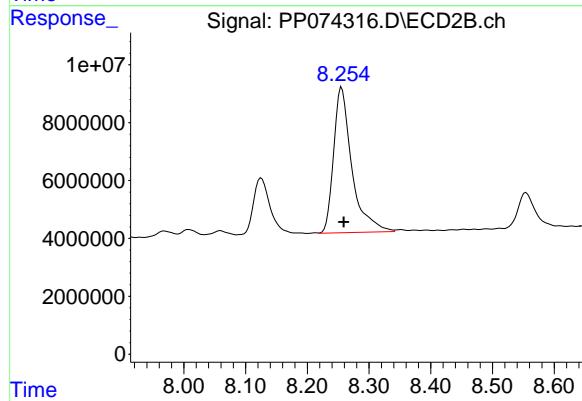

#44 AR-1268-4

R.T.: 8.256 min
 Delta R.T.: -0.003 min
 Response: 103192666
 Conc: 334.98 ng/ml

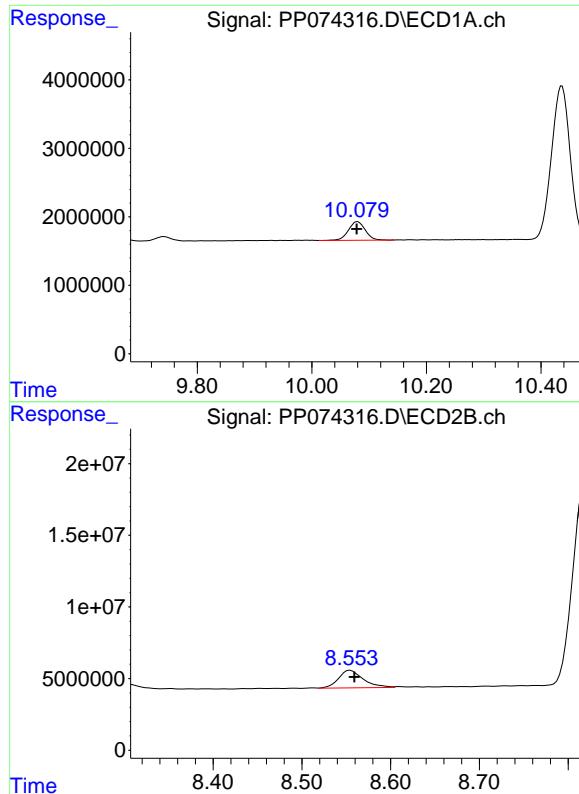

#45 AR-1268-5


R.T.: 10.080 min
Delta R.T.: 0.001 min
Response: 5562779
Conc: 15.82 ng/ml

Instrument:

ECD_P

ClientSampleId :

AR1660CCC500

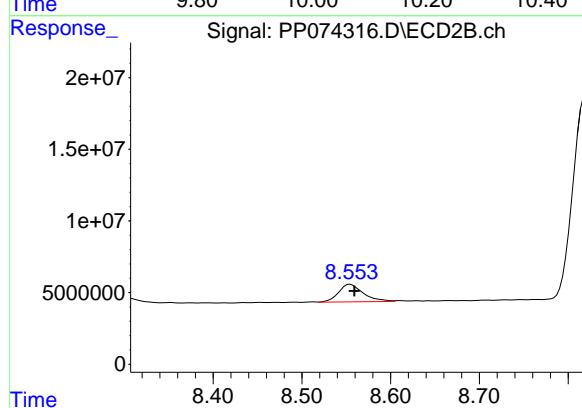

#45 AR-1268-5

R.T.: 8.554 min
Delta R.T.: -0.005 min
Response: 23797855
Conc: 9.33 ng/ml

1
2
3
4
5
6
7
8
9
10
11
12
13
14
15
16
17
18
19
20